



US 20080221412A1

(19) **United States**

(12) **Patent Application Publication**
Baker, et al.

(10) **Pub. No.: US 2008/0221412 A1**
(43) **Pub. Date: Sep. 11, 2008**

(54) **METHOD AND APPARATUS FOR SPECTROSCOPIC TISSUE ANALYTE MEASUREMENT**

Publication Classification

(51) **Int. Cl.**
A61B 5/00 (2006.01)
(52) **U.S. Cl.** **600/310**

(75) **Inventors:** **Clark R. Baker**, Newman, CA (US); **Nicholas J. Durr**, Austin, TX (US); **Murtaza Mogri**, Stanford, CA (US); **Carine Hoarau**, Lafayette, CA (US); **Rafael Ostrowski**, Pittsburg, CA (US); **Martin P. Debreczeny**, Danville, CA (US)

(57) **ABSTRACT**


Methods and systems for calculating body fluid metrics are provided. In accordance with an exemplary embodiment of the present technique, there is provided a method for calculating body fluid metrics by acquiring an absorbance spectrum of a subject's tissue over a range of near-infrared light, performing a multi-linear regression of the absorbance spectrum of the subject's tissue in relation to absorbance spectra of tissue constituents, and calculating body fluid metrics based on the results of the multi-linear regression. A system is provided having a sensor for emitting the light into the subject's tissue and detecting reflected, scattered, or transmitted light, a spectrometer for processing the detected light and generating the absorbance spectrum of the subject's tissue, memory for storing absorbance spectra of the tissue constituents and a multi-linear regression model, and a processor for performing the multi-linear regression and calculating the body fluid metrics.

Correspondence Address:
NELLCOR PURITAN BENNETT LLC
ATTN: IP LEGAL
60 Middletown Avenue
North Haven, CT 06473 (US)

(73) **Assignee:** **Nelcor Puritan Bennett LLC**

(21) **Appl. No.:** **11/716,482**

(22) **Filed:** **Mar. 9, 2007**

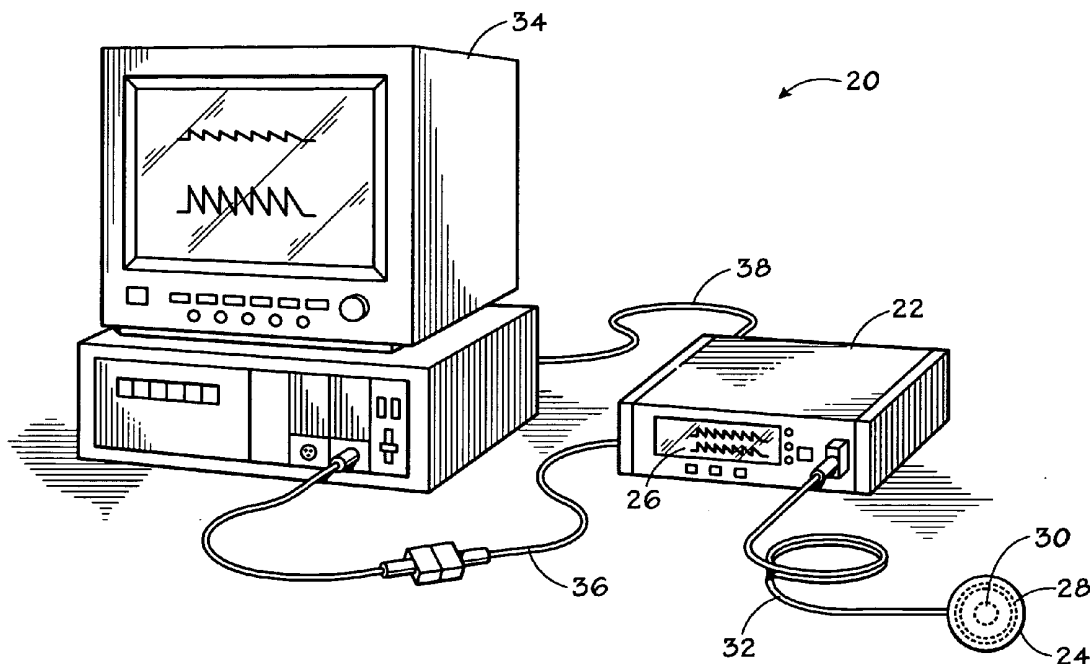

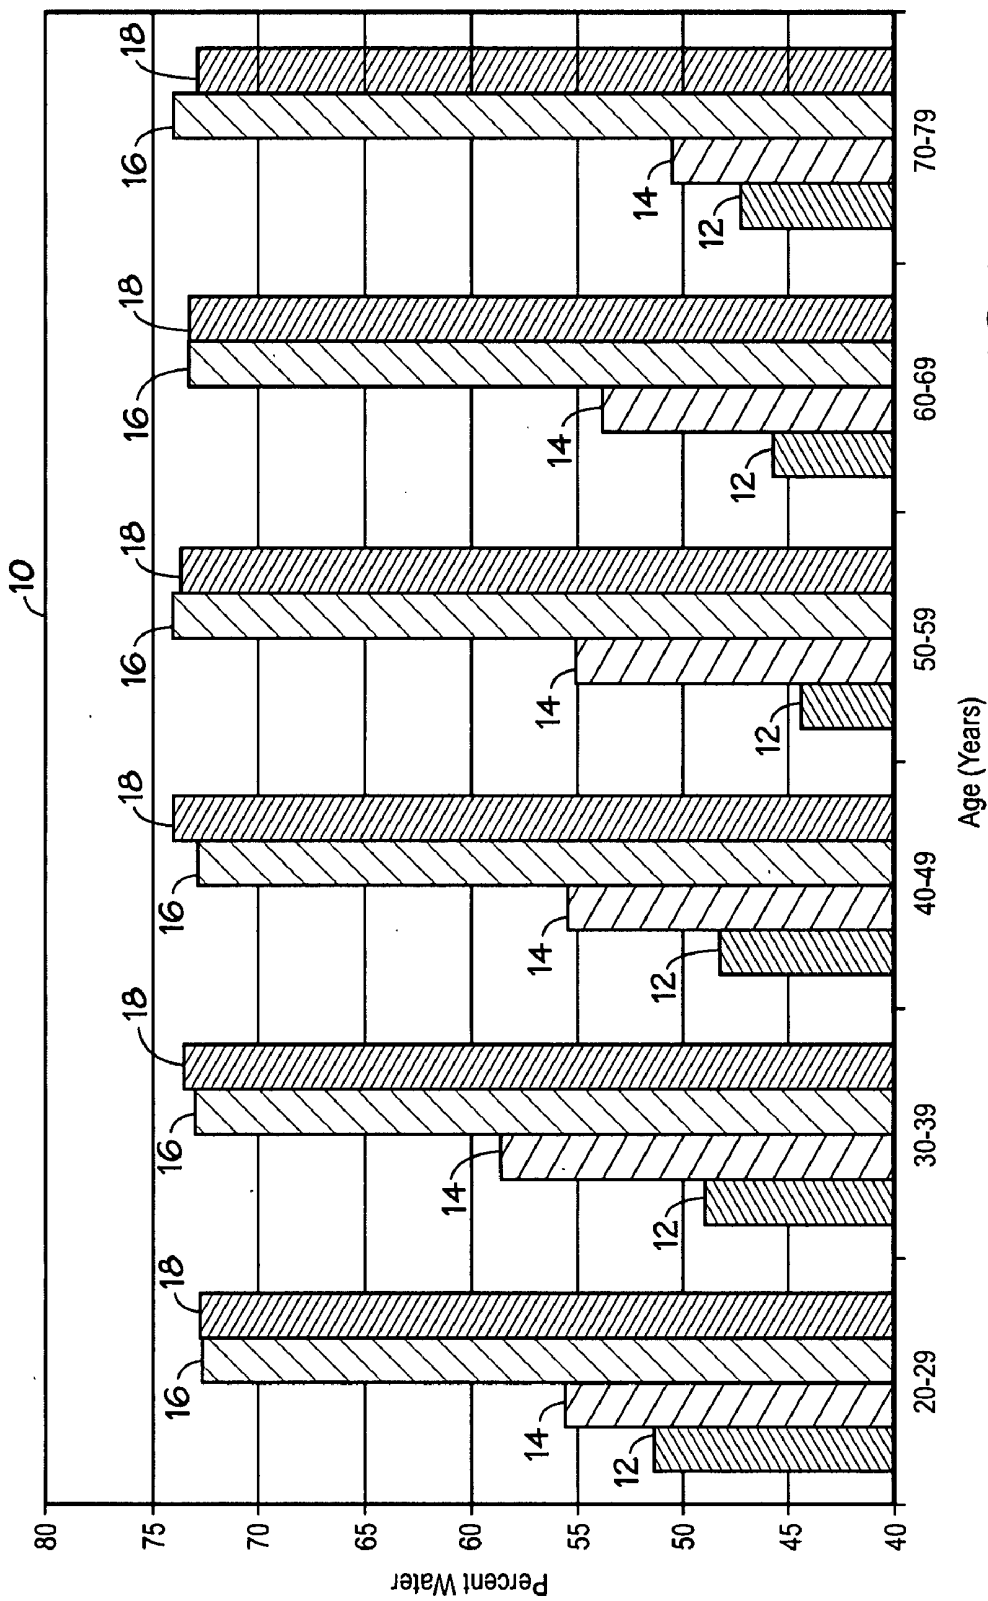


FIG. 1

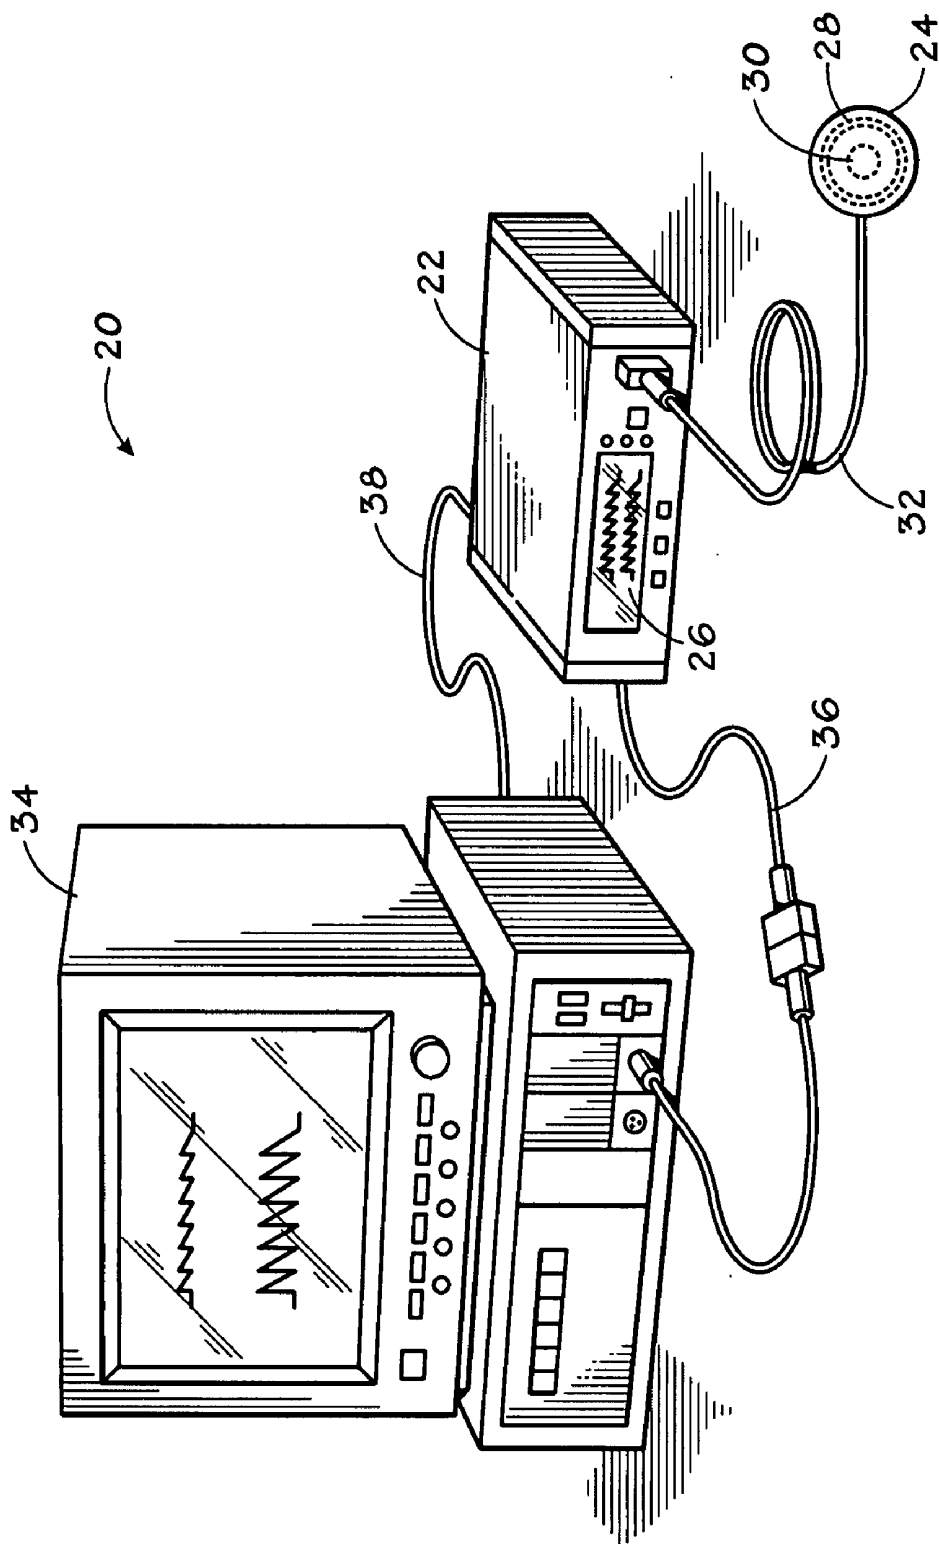


FIG. 2

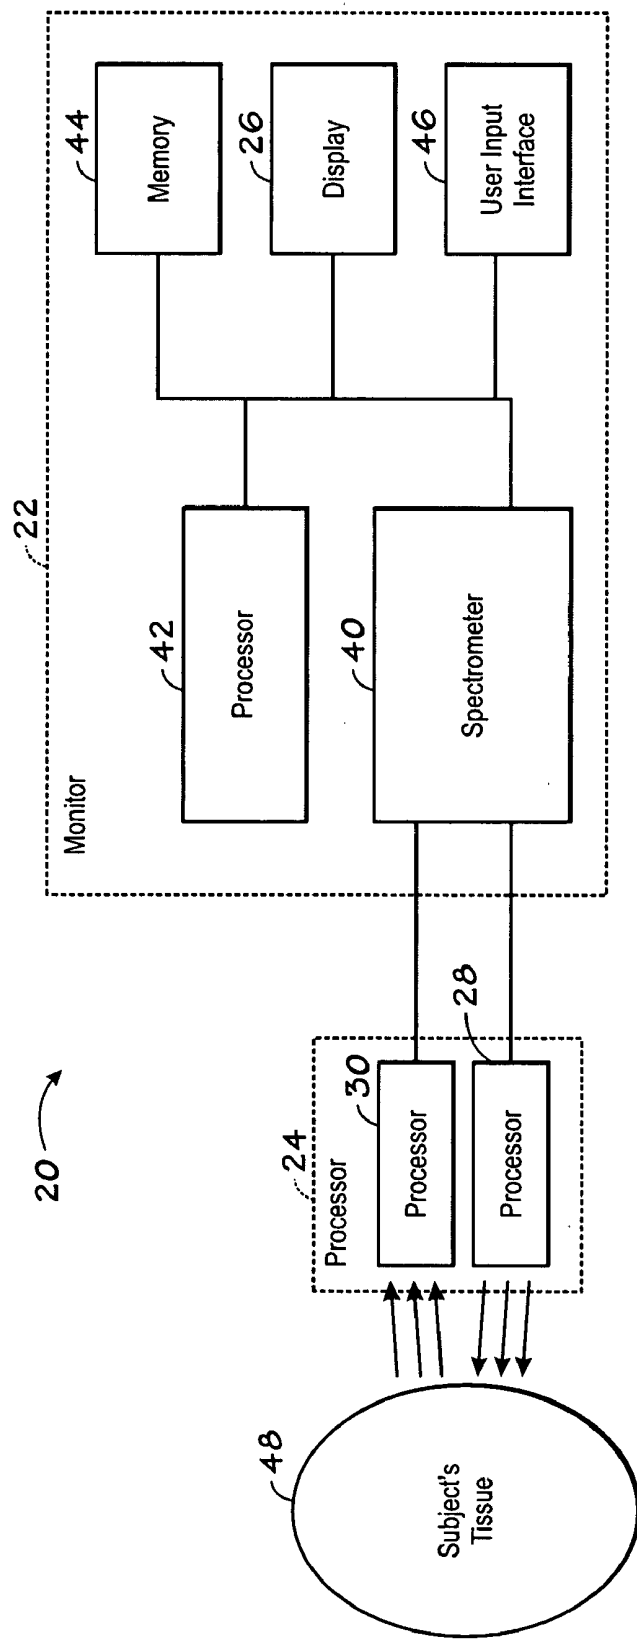


FIG. 3

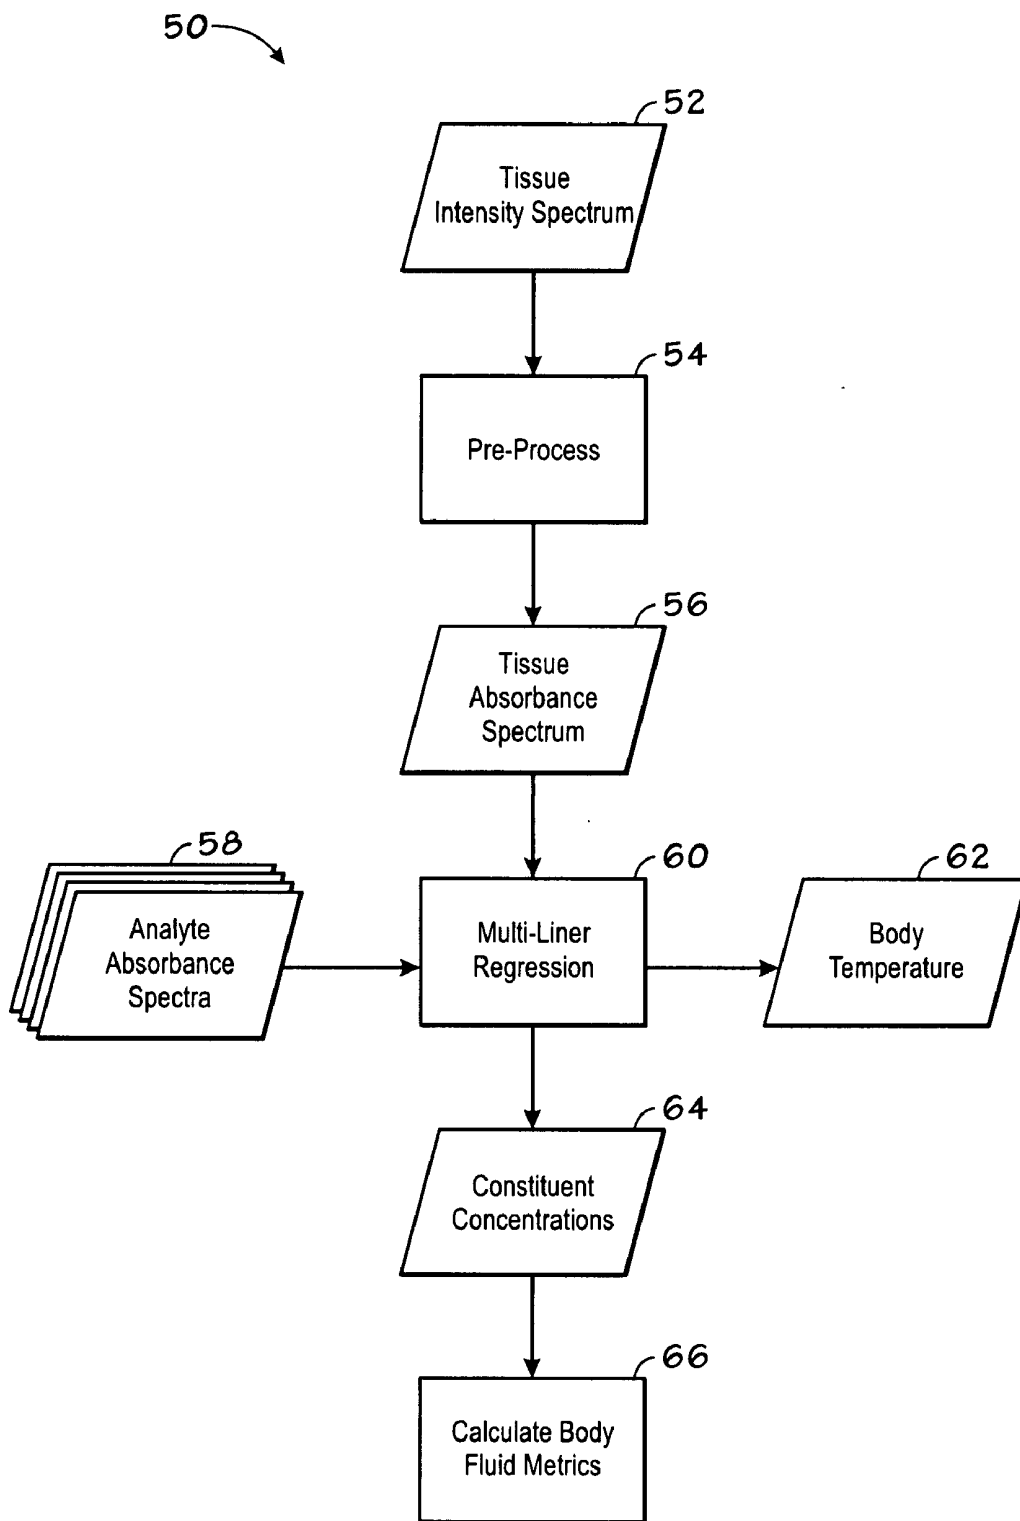


FIG. 4

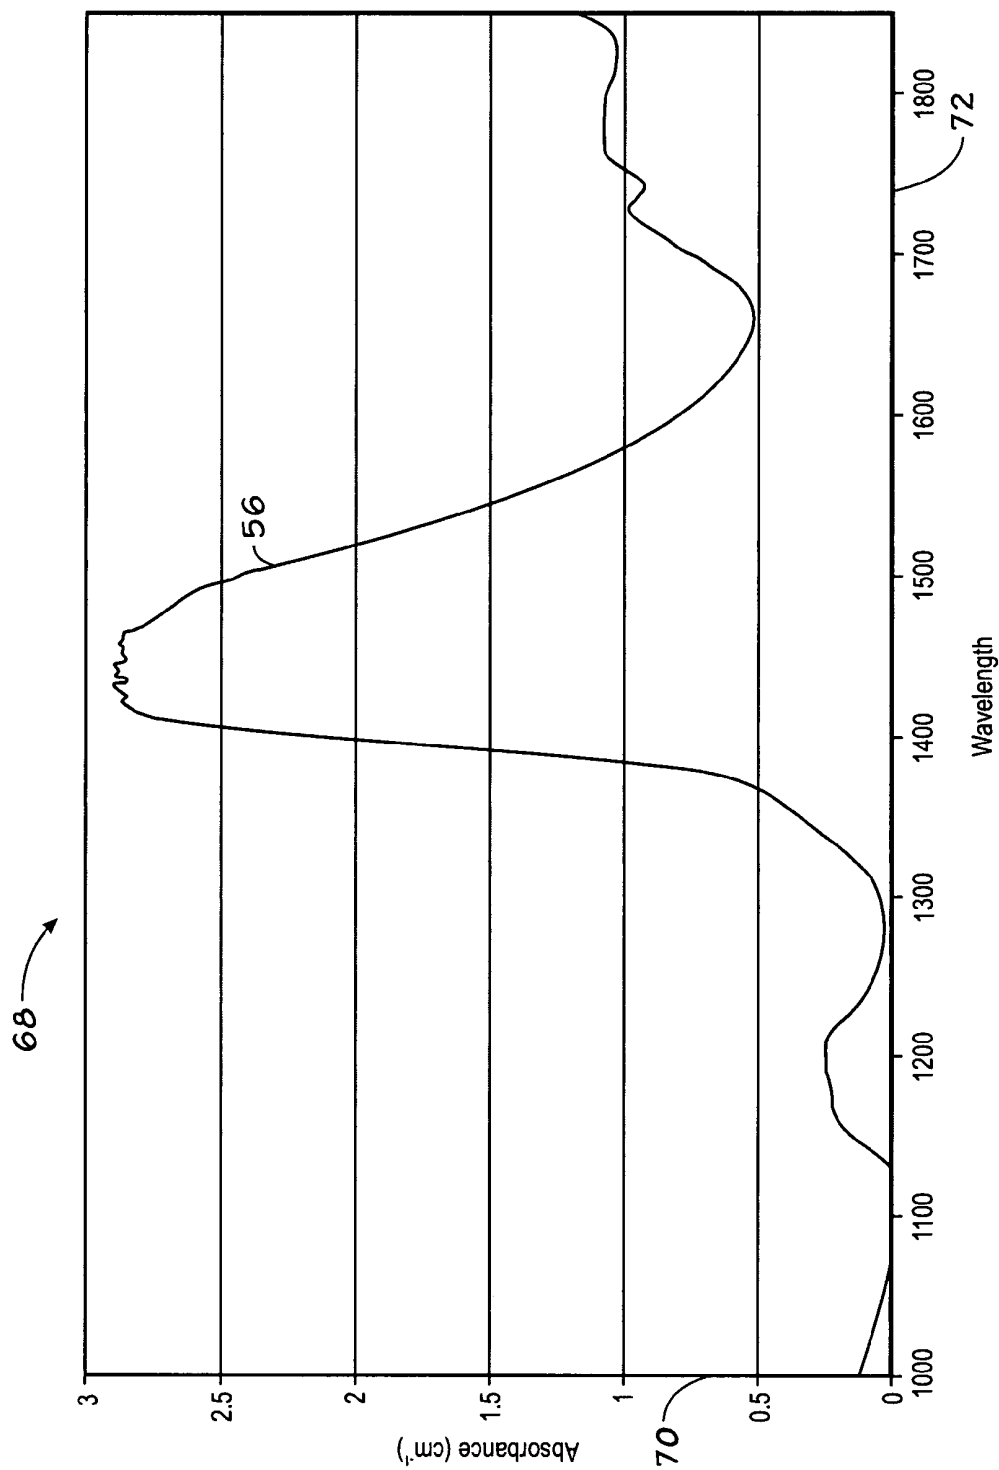


FIG. 5

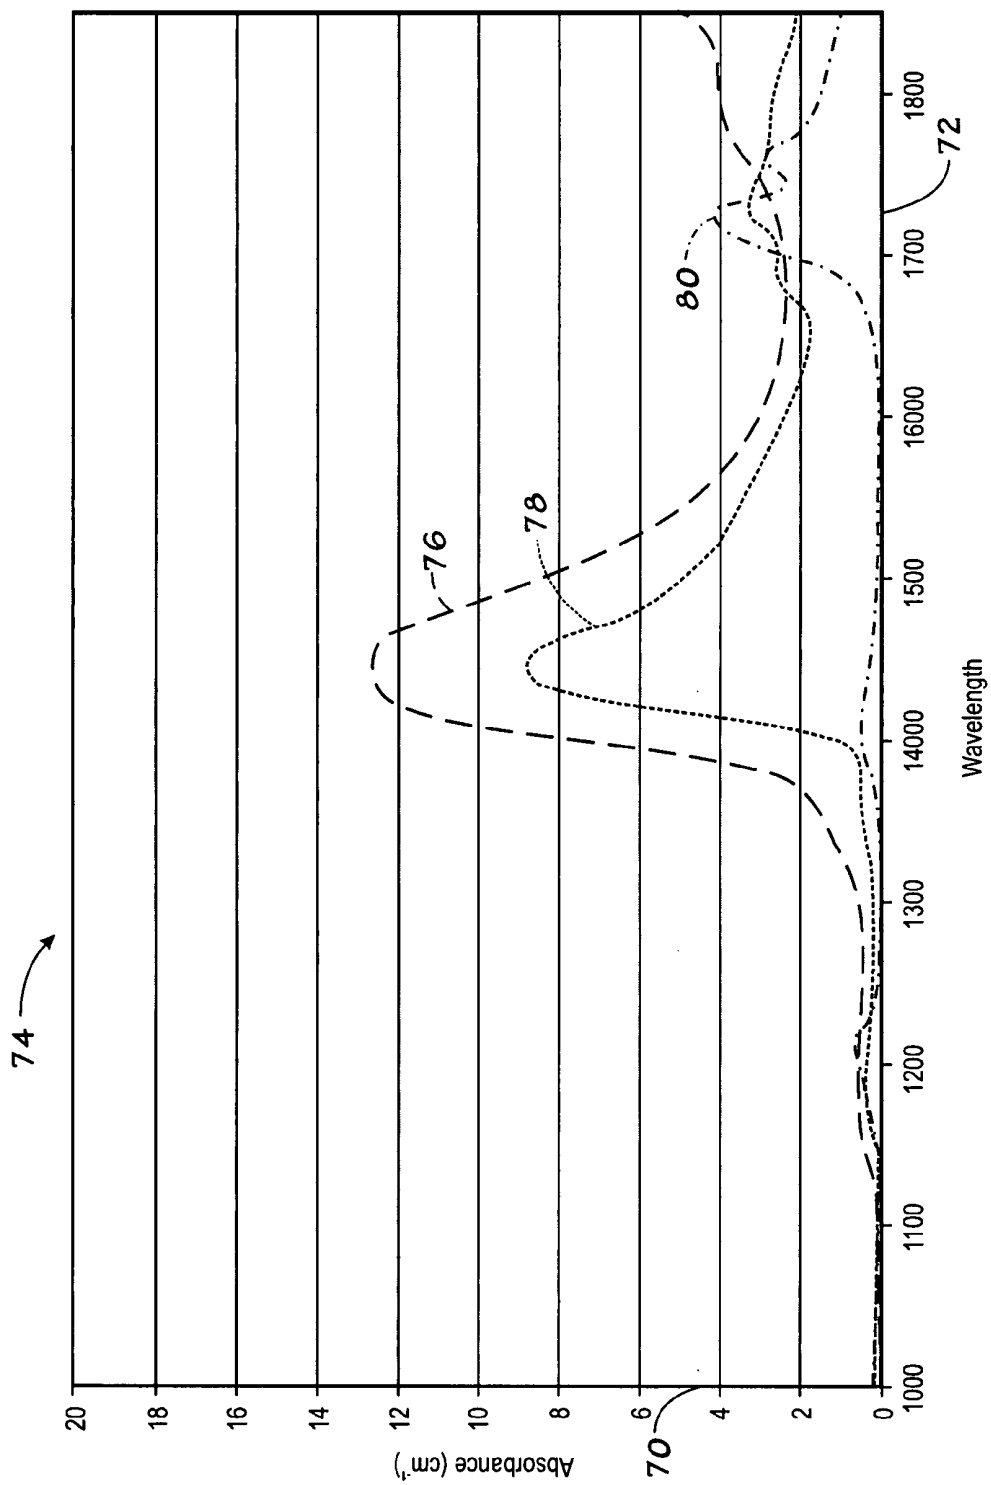


FIG. 6

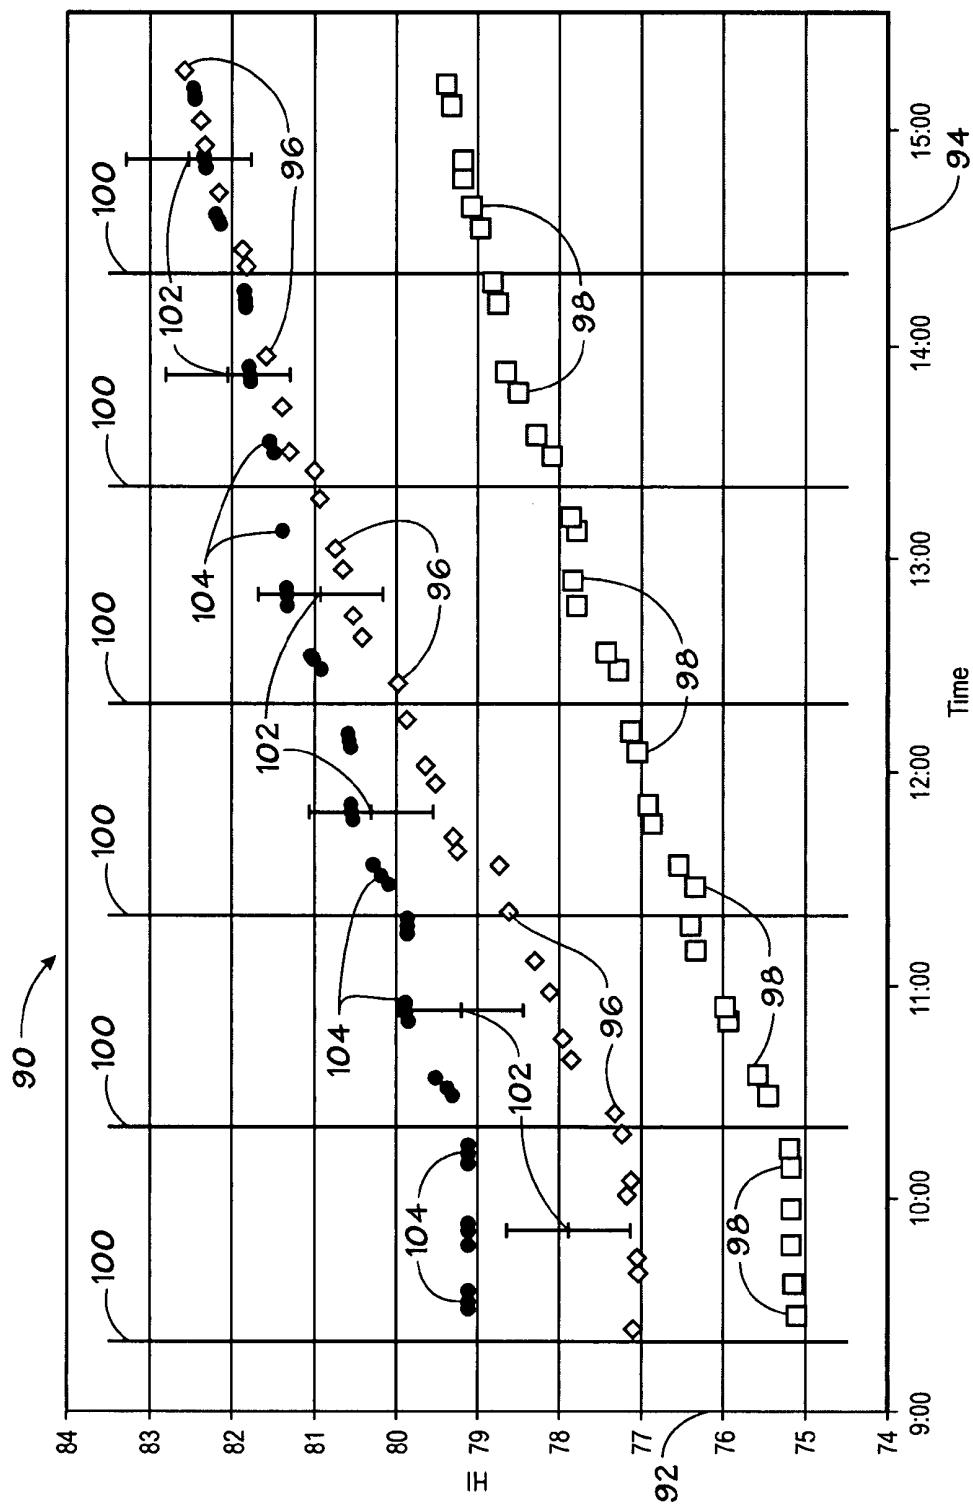


FIG. 7

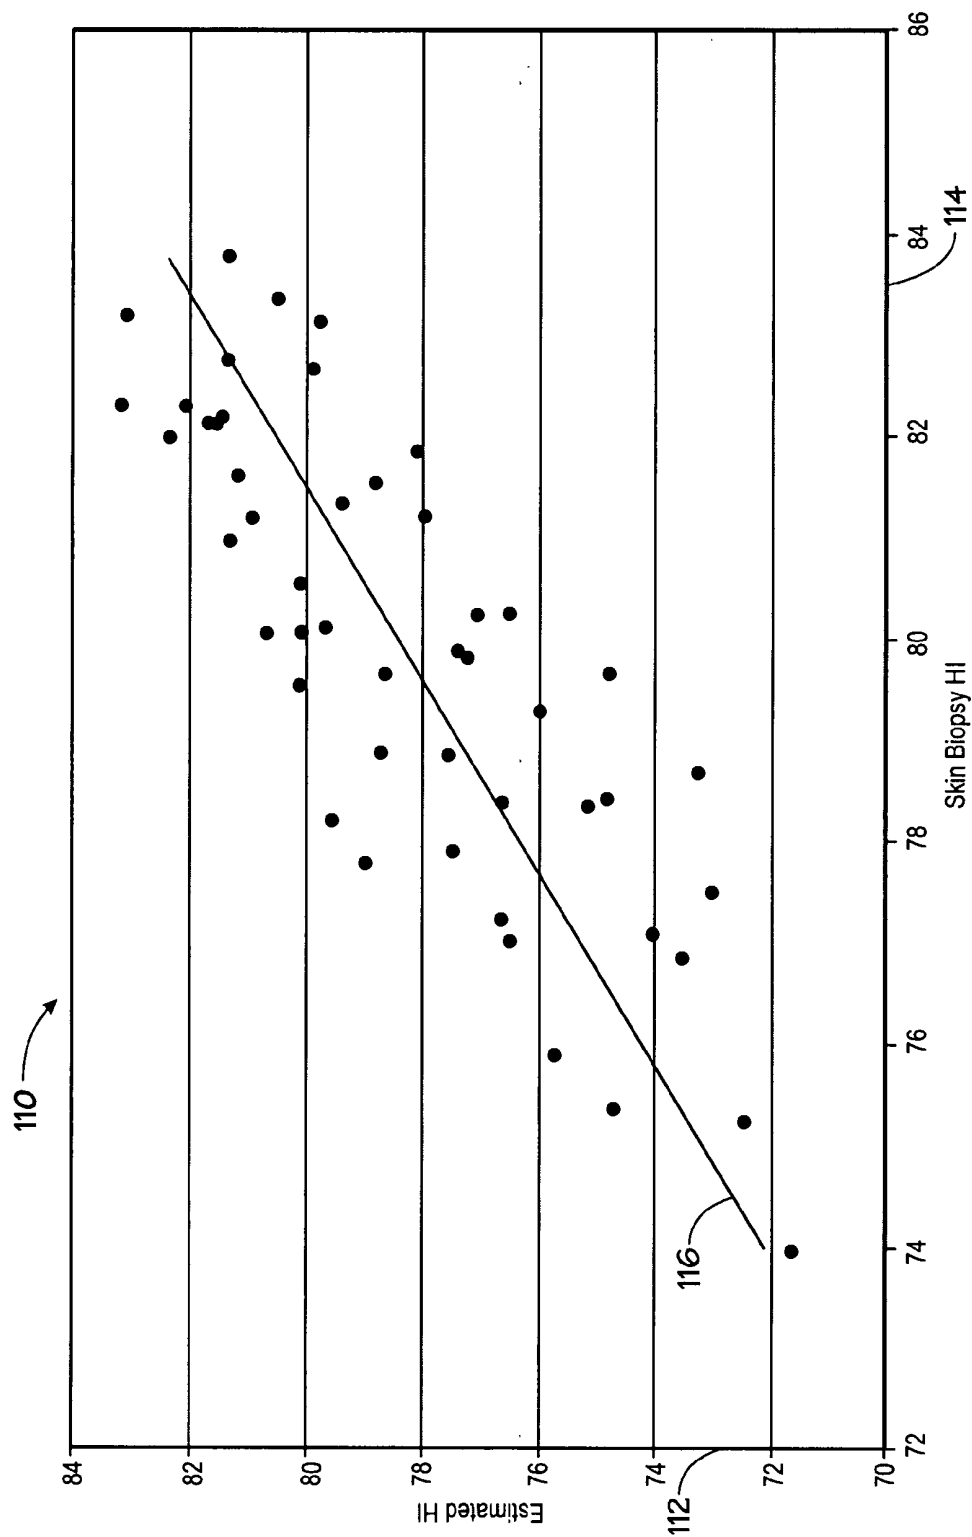


FIG. 8

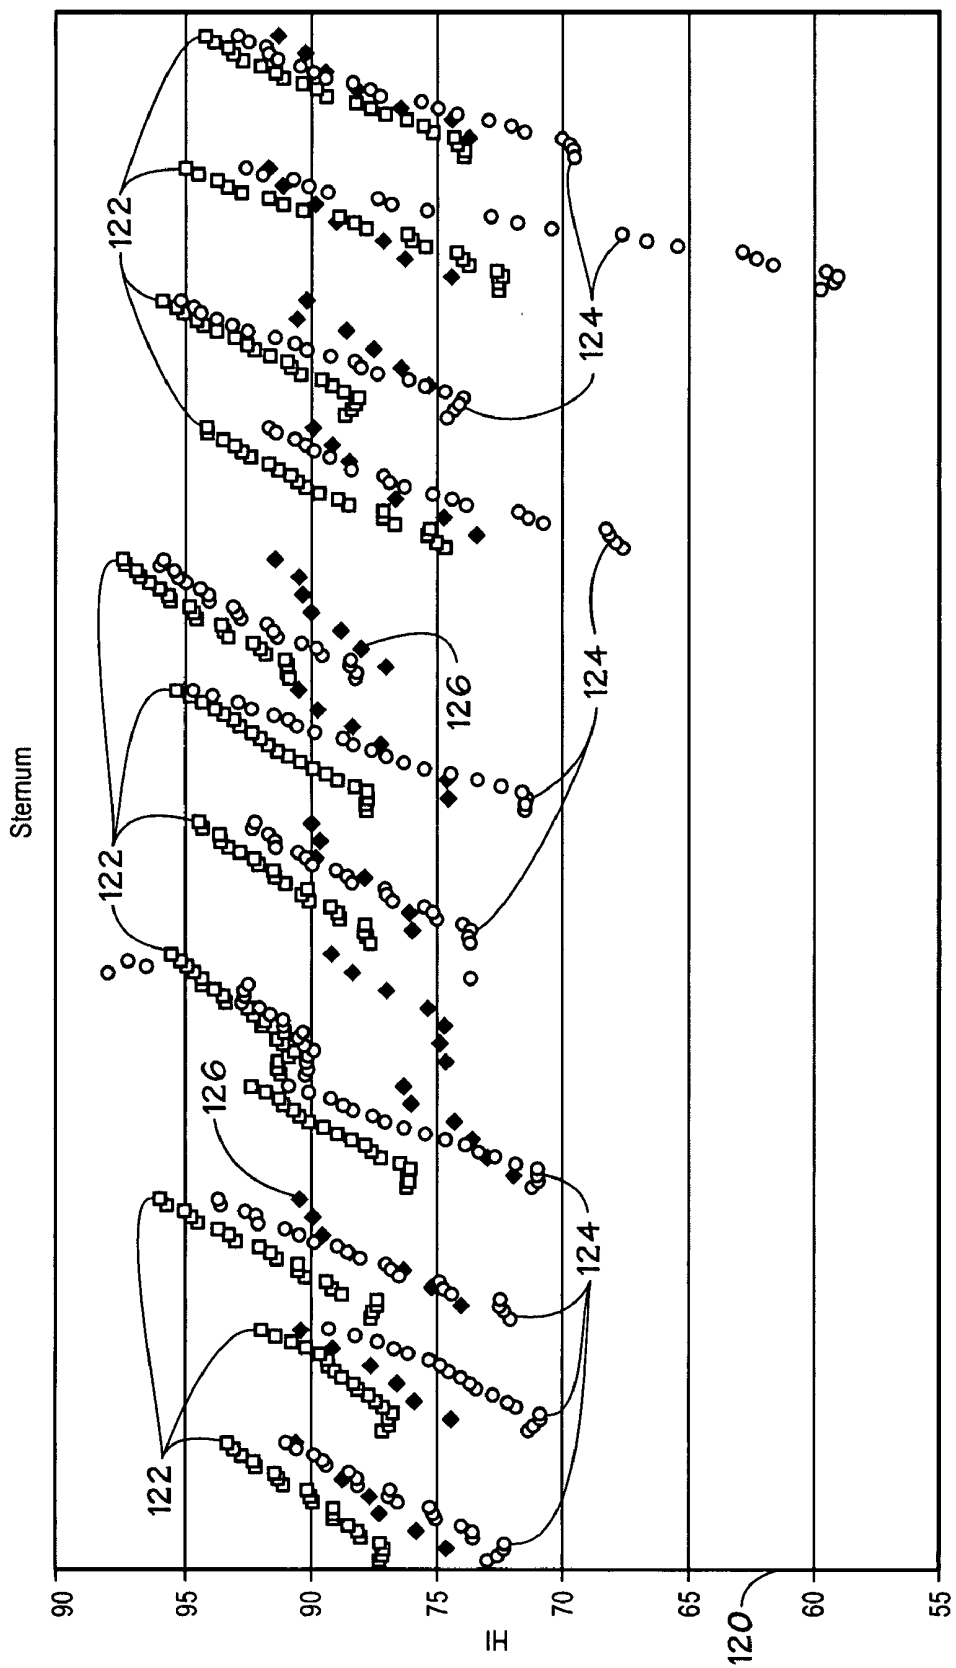


FIG. 9

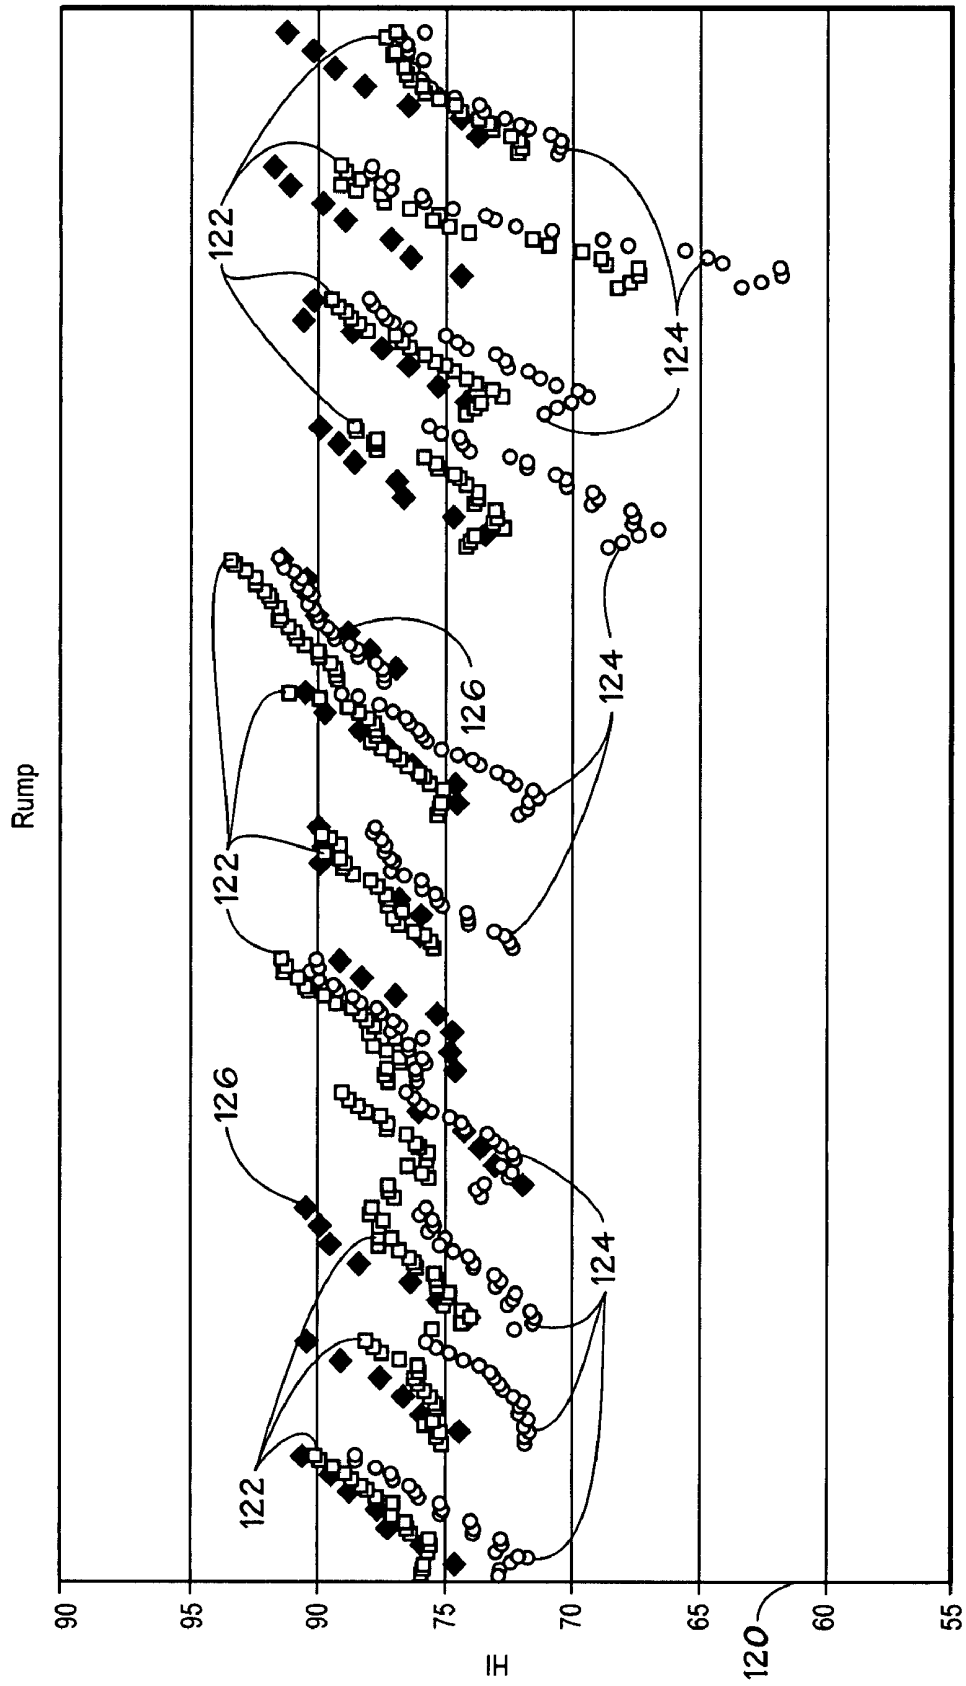


FIG. 10

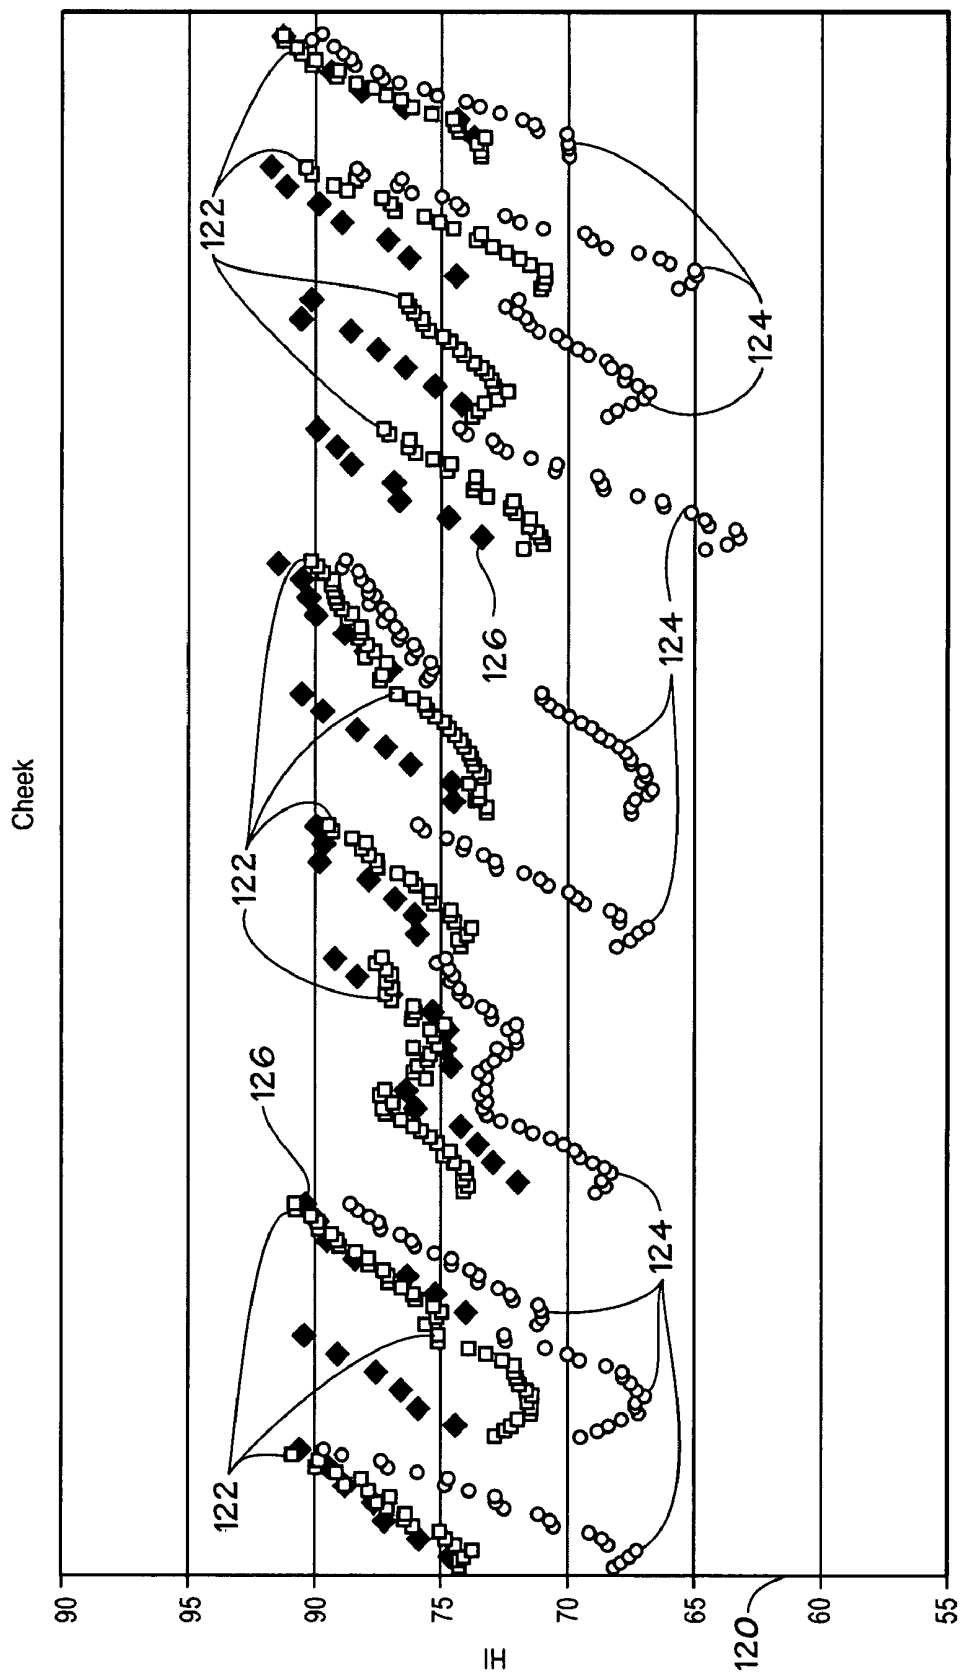


FIG. 11

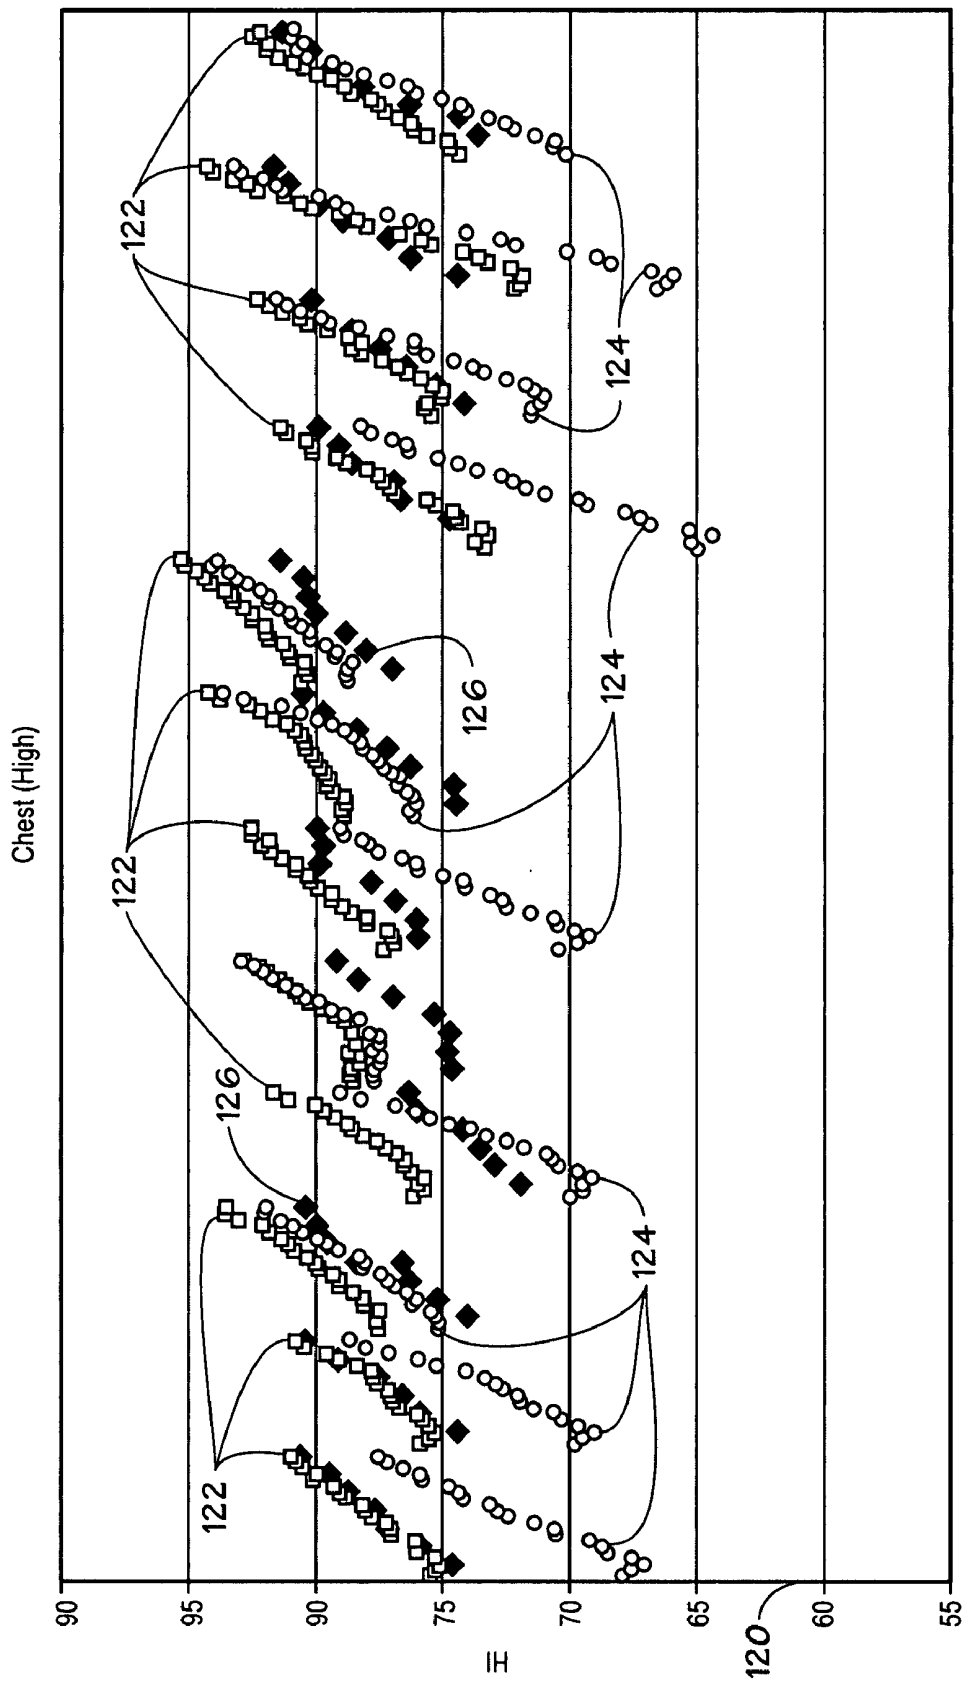


FIG. 12

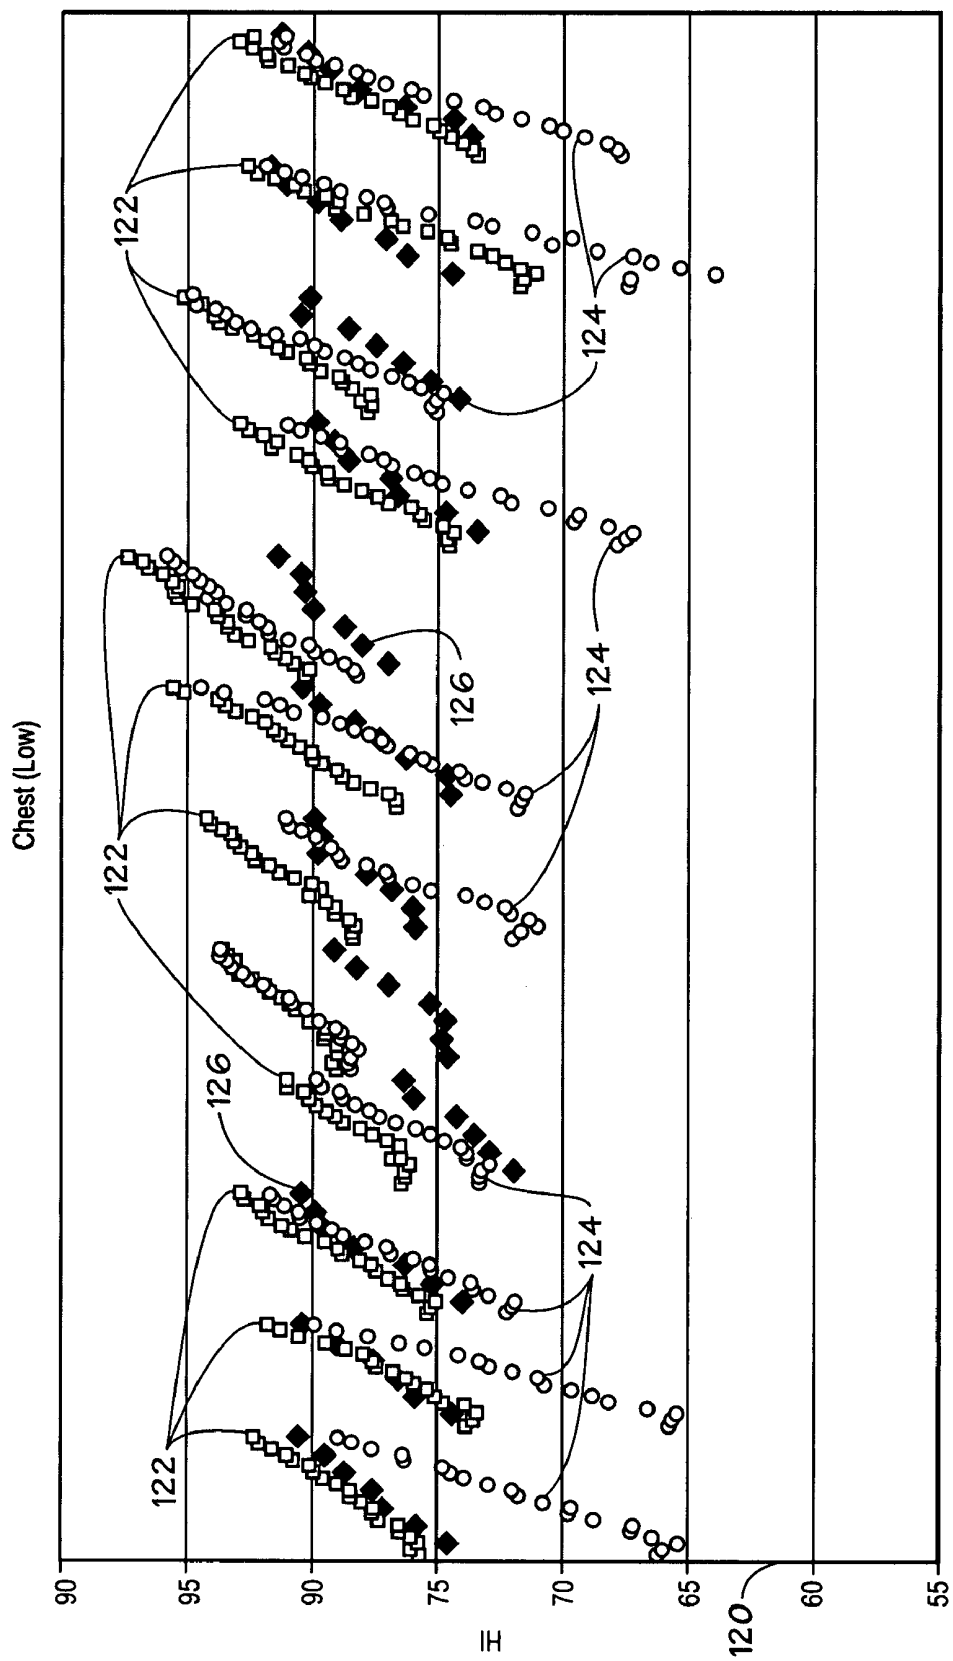


FIG. 13

METHOD AND APPARATUS FOR SPECTROSCOPIC TISSUE ANALYTE MEASUREMENT

SUMMARY

BACKGROUND OF THE INVENTION

[0001] 1. Field of the Invention

[0002] The present invention relates to medical methods and systems, and more particularly to methods and systems for estimating body fluid metrics.

[0003] 2. Description of the Related Art

[0004] This section is intended to introduce the reader to various aspects of art that may be related to various aspects of the present invention, which are described and/or claimed below. This discussion is believed to be helpful in providing the reader with background information to facilitate a better understanding of the various aspects of the present invention. Accordingly, it should be understood that these statements are to be read in this light, and not as admissions of prior art.

[0005] The maintenance of body fluid balance is of foremost concern in the care and treatment of critically ill patients, yet physicians have access to few diagnostic tools to assist them in this vital task. Patients with congestive heart failure, for example, frequently suffer from chronic systemic edema which must be controlled within tight limits to ensure adequate tissue perfusion and prevent dangerous electrolyte disturbances. Conversely, dehydration from diarrhea is one of the most common causes of hospitalization of infants and children and can be life-threatening if not recognized and treated promptly. Additionally, hospital admission of long-term care patients due to dehydration occurs with alarming frequency, high costs to the health care system, and frequently with poor outcomes for patients.

[0006] The most common method for judging the severity of edema or dehydration is based on the interpretation of subjective clinical signs (e.g., swelling of limbs, dry mucous membranes), with additional information provided by measurements of the frequency of urination, heart rate, serum urea nitrogen (SUN) to creatinine ratios, and blood electrolyte levels. However, none of these variables alone is a direct and quantitative measure of water retention or loss.

[0007] An indicator dilution technique, which provides the most accurate direct measure of water in body tissues, is the present de facto standard for assessment of body fluid distribution. However, indicators can take up to four hours to equilibrate in an adult, and require careful collection of fluid samples and extensive equipment for precise analysis, making the technique inconvenient for a clinical setting.

[0008] Alternatively, a great deal of research has been conducted regarding an electrical impedance technique, which involves the use of electrical impedance monitors for measurement of total body water. This electrical-impedance technique is based on measuring changes in the high-frequency (typically 10 KHz-1 MHz) electrical impedance of a portion of the body. However, while results of using the electrical-impedance technique for a single tissue have proven to be clinically useful, mixed results have been obtained with the electrical-impedance technique in clinical studies of whole body fluid disturbances, as reported by various investigators. The results generally indicate that the electrical-impedance technique can be inaccurate when measuring total body water. The rather poor accuracy of the technique seen in many studies points to unresolved deficiencies when applied in a clinical setting.

[0009] Certain aspects commensurate in scope with the originally claimed invention are set forth below. It should be understood that these aspects are presented merely to provide the reader with a brief summary of certain forms the invention might take and that these aspects are not intended to limit the scope of the invention. Indeed, the invention may encompass a variety of aspects that may not be set forth below.

[0010] There is provided a method for calculating one or more body fluid metrics, including acquiring an absorbance spectrum of a subject's tissue at a range of wavelengths of light, determining concentrations of a plurality of constituents of the subject's tissue by performing a multi-linear regression of the absorbance spectrum in relation to a plurality of absorbance spectra of the constituents, and calculating one or more body fluid metrics based on the concentrations.

[0011] There is further provided a method for calculating one or more body fluid metrics, including measuring an intensity spectrum of a subject's tissue, processing the intensity spectrum to determine an absorbance spectrum of the tissue, performing a multi-linear regression of the absorbance spectrum in relation to a plurality of analyte absorbance spectra, wherein the analytes are representative of tissue constituents, and determining concentrations of the tissue constituents based on the multi-linear regression.

[0012] There is further provided a system for calculating one or more body fluid metrics, including a sensor configured to emit a range of wavelengths of light into a subject's tissue and to detect reflected, scattered, or transmitted light, a spectrometer configured to process the reflected, scattered, or transmitted light and to generate an absorbance spectrum of the subject's tissue across the range of wavelengths of light, a memory configured to store a plurality of absorbance spectra of tissue constituents across the range of wavelengths of light and to store a multi-linear regression model, and a processor configured to perform a multi-linear regression of the absorbance spectrum of the subject's tissue with respect to the plurality of absorbance spectra of tissue constituents based on the multi-linear regression model and to calculate one or more body fluid metrics based on the multi-linear regression.

[0013] There is further provided one or more tangible, machine-readable media, having code executable to perform the acts of performing a multi-linear regression of an absorbance spectrum of a subject's tissue in relation to a plurality of absorbance spectra of skin constituents and calculating one or more body fluid metrics based on the multi-linear regression.

BRIEF DESCRIPTION OF THE DRAWINGS

[0014] Advantages of the invention may become apparent upon reading the following detailed description and upon reference to the drawings in which:

[0015] FIG. 1 is a bar graph of body water percentage in men and women across varying age groups as observed in accordance with an exemplary embodiment of the present invention;

[0016] FIG. 2 is a perspective view of a monitor coupled to a multi-parameter patient monitor and a sensor in accordance with an exemplary embodiment of the present invention;

[0017] FIG. 3 is a block diagram of the monitor coupled to a patient in accordance with an exemplary embodiment of the present invention;

[0018] FIG. 4 is a flow chart of a process related to calculating body fluid metrics in accordance with an exemplary embodiment of the present invention;

[0019] FIG. 5 is a graph of a skin absorbance spectrum as observed in accordance with an exemplary embodiment of the present invention;

[0020] FIG. 6 is a graph of analyte absorbance spectra as observed in accordance with an exemplary embodiment of the present invention;

[0021] FIG. 7 is a graph of a pig's hydration index as measured while the pig underwent overhydration in accordance with an exemplary embodiment of the present invention;

[0022] FIG. 8 is a graph of hydration index as determined by a monitor versus hydration index as determined by local skin biopsy for a study of eight pigs undergoing overhydration as observed in accordance with an exemplary embodiment of the present invention; and

[0023] FIGS. 9-13 are graphs illustrating a correlation between hydration index as determined by local skin biopsy and estimated hydration index calculated at various sensor sites using each of two wavelength bands for a study of twelve pigs undergoing non-isotonic overhydration as observed in accordance with an exemplary embodiment of the present invention.

DETAILED DESCRIPTION OF SPECIFIC EMBODIMENTS

[0024] One or more specific embodiments of the present invention will be described below. In an effort to provide a concise description of these embodiments, not all features of an actual implementation are described in the specification. It should be appreciated that in the development of any such actual implementation, as in any engineering or design project, numerous implementation-specific decisions must be made to achieve the developers' specific goals, such as compliance with system-related and business-related constraints, which may vary from one implementation to another. Moreover, it should be appreciated that such a development effort might be complex and time consuming, but would nevertheless be a routine undertaking of design, fabrication, and manufacture for those of ordinary skill having the benefit of this disclosure.

[0025] In accordance with present embodiments, a monitor may be used to non-invasively measure a relative quantity of a specific constituent in a subject's skin. For example, the monitor may be used to measure the percentage of water in the subject's tissue. To obtain such measurements, the monitor may be configured to use near-infrared (NIR) diffuse reflectance spectroscopy to measure the absorbance of water relative to other major tissue constituents. Specifically, the monitor may shine light into the subject's tissue and then measure an intensity of the light after it has been reflected, scattered, and/or transmitted by the tissue. By shining a wide-band light into a patient's tissue, a spectrum of the tissue absorbance over a range of light wavelengths may be measured or observed. In accordance with embodiments of the present invention, once the wide-band absorbance spectrum is measured, it may be utilized as essentially a weighted combination of the absorbance spectra of the tissue's constituents (e.g., water, fat, and proteins). Accordingly, the concentration of each of the constituents in the tissue may be determined by performing a multi-linear regression of the tissue absorbance spectrum using individual absorbance spectra of the tissue constituents. Further, based on the rela-

tive concentrations of the tissue constituents, one or more body fluid metrics may be calculated.

[0026] One body fluid metric which may be desirable to determine in a clinical setting is a patient's body water percentage. However, studies have shown that the fraction of total water in a human body varies significantly (e.g., varying from 44-58%) with age and gender. Such variations can create issues with the proper interpretation of total body water percentage measurements.

[0027] FIG. 1 includes a bar graph 10 that summarizes an exemplary study of the total water in a human body. According to the study results illustrated by bar graph 10, the percentage of water per total body weight in human females 12 is lower on average than the percentage of water per total body weight for human males 14 in the same age groups. The observed difference between genders is because lean tissue, such as muscle, is composed mostly of water, while fatty tissue contains relatively little water. Women have a higher proportion of body fat, therefore female bodies on average have a lower percentage of water per total body weight. However, when fat is excluded from the percent water calculation, a measurement of percentage water in lean tissue can be obtained. The fraction of water in lean tissue in healthy subjects is consistent across both gender and age (e.g., varying from 73-74%). In other words, the percentage water per lean body mass 16 in females is not significantly different from the percentage water per lean body mass 18 in males. This lean tissue water content may be referred to as the "hydration index" (HI). It is now recognized that the HI of skin is a good predictor for total body HI. This relationship between skin and total body HI is described in U.S. Pat. App. No. 60/857,045, entitled "METHOD AND APPARATUS FOR ACCESSING LOCAL AND WHOLE BODY HYDRATION," filed Nov. 6, 2006, which is herein incorporated by reference in its entirety for all purposes.

[0028] An exemplary system 20 which may be used to determine body fluid metrics, such as HI, in accordance with embodiments of the present invention is shown in FIG. 2. The system 20 may include a monitor 22 and a sensor 24. The monitor 22 may be configured to calculate body fluid metrics and display them on a display 26. The sensor 24 may include an emitter 28 for emitting light into a patient's tissue and a detector 30 for detecting the light after it passes through or is reflected by the patient's tissue. The sensor 24 may be communicatively coupled to the monitor 22 via a cable 32 or other suitable device, such as, for example, a wireless transmission device (not shown).

[0029] The system 20 may also include a multi-parameter patient monitor 34. The multi-parameter patient monitor 34 may be included in the system 20 to provide a central display for information from the monitor 22 and from other medical monitoring devices or systems (not shown). For example, the multi-parameter patient monitor 34 may display a patient's body fluid metrics from the monitor 22 along with a blood pressure measurement received from a blood pressure monitor (not shown). In addition to the monitor 22, or alternatively, the multi-parameter patient monitor 34 may be configured to calculate body fluid metrics. The monitor 22 may be communicatively coupled to the multi-parameter patient monitor 34 via a cable 36 or 38 coupled to a sensor input port or a digital communications port, respectively.

[0030] FIG. 3 is a block diagram of the exemplary system 20 of FIG. 2. Specifically, certain components of the monitor 22 and the sensor 24 are illustrated in FIG. 3. The monitor 22

generally includes a spectrometer 40, a processor 42, a memory 44, the display 26, and an input interface 46. More specifically, the monitor 22 may include components found in oximeters and tissue hydration monitors under development by Nellcor Puritan Bennett LLC of Pleasanton, Calif., such as those disclosed in the references mentioned above.

[0031] The sensor 24 includes the emitter 28 and the detector 30. Light emission and detection through the sensor 24 may be controlled by the spectrometer 40. It should be noted that the emitter 28 is configured to emit a range of wavelengths of light into a patient's tissue 48. Hence, the emitter 28 may include a plurality of illumination fibers for emitting light into the patient's tissue 48. The detector 30 may also consist of a plurality of detection fibers and may be configured to transmit light to the spectrometer 40 via the fibers. Light enters the detector 30 after passing through the patient's tissue 48. The spectrometer 40 may convert the intensity of the received light as a function of wavelength into an electrical signal for processing. The light intensity is directly related to the absorbance, scattering, and/or reflectance of light in the tissue 48. That is, when more light at a certain wavelength is absorbed, scattered, or reflected, less light of that wavelength is received from the tissue 48 by the detector 30. In the illustrated embodiment of the sensor 24 in FIG. 2, the illumination fibers making up emitter 28 are arranged in a circle around the detector 30. Other embodiments of the sensor 24 may include, for example, a circular detector surrounding an emitter or a parallel emitter and detector.

[0032] The detected light from the detector 30 may be transmitted to the spectrometer 40 in the monitor 22. The spectrometer 40 separates the detected light according to wavelength and converts the intensity to a measure of absorbance to determine an absorbance spectrum. The processor 42 may then perform a multi-linear regression on the measured absorbance spectrum, as described below, using estimated or standardized absorbance spectra of the individual tissue constituents. An algorithm for performing the multi-linear regression, as described below, along with the absorbance spectra information for each of the individual tissue constituents, may be stored in the memory 44. Additional information for use in the multi-linear regression algorithm, such as, for example, the subject's body or skin temperature, may be entered into the monitor 22 via the input interface 46 or via other sensor input ports (not shown).

[0033] The monitor 22 may be configured to calculate the hydration index, or other tissue hydration parameters, of a patient's tissue 38 by performing a multi-linear regression of a measured tissue absorbance spectrum in relation to absorbance spectra of known tissue constituents. FIG. 4 is a flow chart illustrating a process 50 by which body fluid metrics may be estimated. The intensity of light detected by detector 30 may be represented as a tissue intensity spectrum 52. The tissue intensity spectrum 52 may be pre-processed (Block 54), as described below, to produce a tissue absorbance spectrum 56. This tissue absorbance spectrum 56 may be compared to a plurality of analyte absorbance spectra 58 in a multi-linear regression (Block 60). In addition, other factors may be considered in the multi-linear regression (Block 60). For example, a patient's body temperature 62 may be input into the multi-linear regression (Block 60) as described below. The result of the multi-linear regression (Block 60) is the constituent concentrations 64. These constituent concentrations 64 may then be used to calculate body fluid metrics (Block 66) as described below.

[0034] The data pre-processing step (Block 54) may include correcting the spectrum of detected light 52 for instrument and sensor factors and converting the intensity spectrum 52 into the absorbance spectrum 56. An instrument factor may include, for example, a residual signal detected by the spectrometer 40 with the light source off, due to either ambient light or an offset voltage in the spectrometer's electronic circuitry. This residual signal may be subtracted from the tissue intensity spectrum 52 to correct associated inaccuracies. Another instrument factor may include differences in spectral resolutions between spectrometers, which may cause measurement inaccuracies. For example, the spectrometer 40 may have a different spectral resolution than the spectrometer on which the analyte absorbance spectra 58 were collected. This factor may be corrected by adjusting the known analyte absorbance spectra 58 for the spectral resolution of the spectrometer. That is, the resolution of the analyte absorbance spectra 58 may be scaled up or down depending on the resolutions of the spectrometer on which they were collected and the spectrometer 40 on which the patient's tissue 48 is measured.

[0035] Additional instrument and sensor factors may affect the detected intensity spectrum 52. These factors may be corrected in the conversion of the intensity spectrum 52 to the absorbance spectrum 56. Generally, intensity may be converted to absorbance according to the following equation:

$$A = -\log [I_{\text{detected}}/I_{\text{emitted}}] \quad (1)$$

where I is the intensity of light and A is absorbance. In accordance with present embodiments, I_{emitted} may be adjusted to account for sensor factors which affect the accuracy of Equation (1). For example, the spacing between the emitter 28 and the detector 30 on the sensor 24 may affect the slope and curvature of the detected intensity spectrum 52. Therefore, the detected intensity spectrum 52 may be divided by a reference intensity spectrum of a substance having minimal absorption and scattering similar to tissue. For example, a Teflon block has been found to approximate the bulk scattering of tissue. This Teflon block reference intensity spectrum may further be divided by the ratio of a previously-collected Teflon intensity spectrum to a previously-collected intensity spectrum of a total reflecting substance, such as a gold mirror. While a total reflecting surface may be used directly to establish the reference intensity spectrum, it may be desirable to use the Teflon block with a correction factor to establish the reference intensity spectrum because the Teflon block may be more portable and convenient than, for instance, a gold mirror.

[0036] The slope and curvature of the detected tissue intensity spectrum 52 may change with emitter-detector spacing as the scattering coefficients, and therefore the mean photon pathlengths, vary with wavelength. Therefore, the gold-to-Teflon ratio may be calculated and applied for the emitter-detector spacing used to collect the tissue intensity spectrum 52. The corrected reference spectrum compensates for wavelength-dependent emitter and detector characteristics according to the following equations:

$$A = -\log [I_{\text{detected}} / I_{\text{standard}}] \quad (2)$$

where -continued

$$I_{\text{standard}} = I_{\text{reflon,detected}} \times \frac{I_{\text{gold,standard}}}{I_{\text{reflon,standard}}}$$

Those skilled in the art will recognize that, depending on the design of the monitor **22**, I_{standard} may be acquired for each use, may be stored in the memory **44** or in a memory within the sensor **24**, or may be computed based on one or more measured or stored instrument or sensor characteristics. The resulting absorbance spectrum **56** represents the absorbance of the patient's tissue **48** across a range of wavelengths, as illustrated by an exemplary graph **68** in FIG. **5**. Specifically, the graph **68** includes absorbance values **70** plotted against wavelengths of emitted light **72**.

[0037] Returning to FIG. **4**, in order to perform the multi-linear regression (Block **60**) of the skin tissue absorbance spectrum **56**, the absorbance spectra **58** of the main constituents found in skin may be measured or approximated over the entire near-infrared region (i.e., approximately 1000-2500 nm). For example, FIG. **6** includes a graph **74** of the absorbance spectra **58** of known analytes representing some skin constituents. The illustrated absorbance spectra **58** include a water absorbance spectrum **76**, a protein absorbance spectrum **78**, and a lipid (fat) absorbance spectrum **80**. Other analytes for which known absorbance spectra may be collected and which may be used in embodiments of the present invention include oxygenated hemoglobin (HbO₂); deoxygenated hemoglobin (Hb); water at different temperatures; known mixtures of water, protein, and lipid; different varieties of proteins (e.g., elastin, albumin, keratin, and collagens); different varieties of lipids (e.g., oleic acid, cholesterol, palmitic acid, corn oil and canola oil); saturated and unsaturated fats; proteins dissolved in deuterium oxide ("heavy water"); and any other analyte representative of known skin constituents. The absorbance spectra **58** may be acquired by measuring light transmitted through a cuvette containing the representative, and desirably non-scattering, analyte.

[0038] Referring again to FIG. **4**, based on the measured analyte absorbance spectra **58**, the concentration of skin constituents **64** may be determined from the tissue absorbance spectrum **56** in the multi-linear regression (Block **60**). Multi-linear regression may be employed to determine a linear combination of the known analyte absorbance spectra **58**, such as absorbance spectra **76**, **78**, and **80**, that best matches the measured tissue absorbance spectrum **56**. In other words, the multi-linear regression determines to what extent each tissue constituent contributes to the values of the measured tissue absorbance spectrum **56**. The multi-linear regression (Block **60**) may be characterized by the following set of equations:

$$\begin{aligned} A_{\lambda_1}^M &= C_W A_{\lambda_1}^W + C_P A_{\lambda_1}^P + C_L A_{\lambda_1}^L + C_H A_{\lambda_1}^H + b \\ A_{\lambda_2}^M &= C_W A_{\lambda_2}^W + C_P A_{\lambda_2}^P + C_L A_{\lambda_2}^L + C_H A_{\lambda_2}^H + b \\ A_{\lambda_n}^M &= C_W A_{\lambda_n}^W + C_P A_{\lambda_n}^P + C_L A_{\lambda_n}^L + C_H A_{\lambda_n}^H + b \end{aligned} \quad (3)$$

where A is the absorbance, λ_n is the wavelength, C is the concentration **64** of the constituent, b is a wavelength-independent offset, M denotes the measured tissue **48**, W denotes water, P denotes proteins, L denotes lipids, and H denotes

oxygenated hemoglobin. Additional terms may be added for other analytes. This system may also be expressed using the following equation:

$$A^M = A^S C, \quad (4)$$

$$\text{where } A^M = \begin{pmatrix} A_{\lambda_1}^T \\ A_{\lambda_2}^T \\ \vdots \\ A_{\lambda_N}^T \end{pmatrix}, C = \begin{pmatrix} C_W \\ C_P \\ C_L \\ C_H \\ b \end{pmatrix}, \text{ and}$$

$$A^S = \begin{pmatrix} A_{\lambda_1}^W & A_{\lambda_1}^P & A_{\lambda_1}^L & A_{\lambda_1}^H & 1 \\ A_{\lambda_2}^W & A_{\lambda_2}^P & A_{\lambda_2}^L & A_{\lambda_2}^H & 1 \\ \vdots & \vdots & \vdots & \vdots & \vdots \\ A_{\lambda_N}^W & A_{\lambda_N}^P & A_{\lambda_N}^L & A_{\lambda_N}^H & 1 \end{pmatrix}$$

[0039] Given the measured tissue absorbance spectrum **56** (A^M) and the known analyte absorbance spectra **58** (A^S), the concentration **64** (C) of each constituent may be calculated. Because the measured tissue absorbance spectrum **56** and the known analyte absorbance spectra **58** may be represented as matrices, as illustrated in Equation (4), solving for the constituent concentrations **64** may be performed using a suitable matrix manipulation environment, such as, for example, MATLAB®, available commercially from The MathWorks, Natick, Mass. The matrix manipulation environment may, for example, be utilized to find the constituent concentrations **64** (C) in Equation (4) by multiplying each side of the equation by the inverse of the matrix representing the analyte absorbance spectra **58** (A^S). The matrix manipulation environment may, for example, be stored in the memory **44** of the monitor **22** for use by the processor **42**.

[0040] Equations (3) and (4) illustrate a simple multi-linear regression model which considers only four skin constituents and a wavelength-independent offset which accounts for variations in light input. Additional factors may be added to the equations to account for observed differences in estimated and actual body fluid metrics. For example, the multi-linear regression model may include a temperature component to account for temperature-dependent changes in hydrogen bonding which affect the width and center frequency of the water absorbance spectrum **76**. That is, the patient's body or skin temperature **62** may be measured and used as an input to the model. The effect of temperature on the water absorbance spectrum **76** is due to hydrogen bonds between molecules which decrease as temperature increases. In addition, it is believed that the degree of hydrogen bonding could be affected in vivo by the proximity of water molecules to either fat or protein and/or by the structural properties of the tissue rather than the bulk composition. The temperature component of the multi-linear regression model may include adjustment of the known water absorbance spectrum **76** for the measured body temperature **62** and/or use of a specific known water absorbance spectrum **76** corresponding to the measured temperature **62**. Thus, equation (3) may be rewritten as follows:

$$A_{\lambda_n}^M = C_W A_{\lambda_n}^W(T) + C_P A_{\lambda_n}^P + C_L A_{\lambda_n}^L + C_H A_{\lambda_n}^H + b, \quad (5)$$

where T is the patient's body temperature **62**, and the known absorbance spectrum of water **76** (A^W) is dependent on temperature **62**.

[0041] Further adjustments to the multi-linear regression model may consist of, for example, adding a slope factor in addition to the known analyte absorbance spectra (A^S) and the wavelength-independent offset (b). This slope factor may account for variation between tissues in the derivative of the tissue scattering coefficient with respect to wavelength which are independent of variation in the composition of the tissue. The slope factor may consist of, for example, another degree of freedom in the multi-linear regression and/or a known offset. Equation (5) may therefore be rewritten as follows:

$$A_{\lambda_n}^M = C_W A_{\lambda_n}^W(T) + C_P A_{\lambda_n}^P + C_L A_{\lambda_n}^L + C_H A_{\lambda_n}^H + b + s_{\lambda_n} \quad (6)$$

where s represents the slope factor. The slope factor may, for example, be a linear function, a quadratic or higher order polynomial function, or an exponential function of wavelength.

[0042] An additional factor may be added to the multi-linear regression model to account for the reduction in mean photon pathlength that occurs with increasing absorption coefficients. That is, tissue that is more absorbent at a given wavelength will preferentially absorb light deeper in the tissue, so that the photons reaching the detector will preferentially be those that traversed a shallower and shorter path through the tissue. This pathlength factor may be represented as a weighted function of the measured tissue absorbance spectrum. For example, the function may be a multiple of the square of the tissue absorbance spectrum **56** ($(A^M)^2$). In addition, if a spectrometer is used in which the wavelength calibration drifts, a weighted derivative of the tissue absorbance spectrum with respect to wavelength ($dA^M/d\lambda$) may be added as a calibration factor to the multi-linear regression model to account for shifts in the wavelength calibration. Including these pathlength and calibration factors, Equation (6) may be rewritten as follows:

$$A_{\lambda_n}^M = C_W A_{\lambda_n}^W(T) + C_P A_{\lambda_n}^P + C_L A_{\lambda_n}^L + C_H A_{\lambda_n}^H + b + s_{\lambda_n} + \alpha (A_{\lambda_n}^M)^2 + \beta \frac{dA_{\lambda_n}^M}{d\lambda} \quad (7)$$

where α and β are weighting coefficients.

[0043] A correction may also be made to account for the water content of fat (approximately 10-20%) and to exclude this fat-associated water from the lean-water estimate. Finally, hydration index, approximated as the ratio of water to non-fat analytes, may be computed (Block **66**) based on the concentrations of each tissue constituent obtained from the multi-linear regression according to the following equation:

$$HI = \frac{C_W}{C_W + C_P + C_H} \quad (8)$$

[0044] In an experimental test of the described multi-linear regression model, the algorithm was applied to data collected from both euhydrated humans and overhydrated pigs. These tissue absorbance spectra were gathered from a near-infrared array spectrometer with spectral resolution of about 18 nm. FIG. 7 includes a graph **90** that illustrates the results of an exemplary test of a pig undergoing overhydration. The graph **90** shows HI **92** over time **94** according to embodiments of the present invention. The measured tissue absorbance spectra used in calculating HI were obtained using a torso sensor

(data points **96**) and a forehead sensor (data points **98**). The emitter-detector spacing for the torso sensor was 5 mm and for the forehead sensor was 9 mm, and the wavelength range analyzed was 1000-1350 nm. Each vertical line **100** marks the time at which half a liter of fluid was administered to the subject.

[0045] In addition to estimating the HI, data collected by local biopsy (data points **102**) was analyzed by chemical methods, such as those described in S. E. Campbell et al., "A novel method to determine lean body water using localized skin biopsies: correlation between lean skin water and lean body water in an overhydration model," *American Journal of Physiology—Regulatory, Integrative and Comparative Physiology* 291 (2006), R1539-R1544, which is herein incorporated by reference in its entirety for all purposes. Whole body water fraction was calculated using the same chemical analysis method on the homogenized carcass after the end of the experiment. Weights measured during the course of each measurement were then used to back-calculate body water fractions (data points **104**). It is apparent from the graph **90** that the multi-linear regression method for estimating HI shows high correlation to chemical analyses of local skin biopsies and back-calculation of body water fractions from the homogenized carcass. Indeed, the data points obtained from each method clearly include similar trends.

[0046] Results of further experimentation on eight overhydrated pigs, illustrated in a graph **110** included in FIG. 8, show a good correlation between estimated HI **112** from the multi-linear regression model and HI **114** determined by skin biopsy. A torso sensor with an emitter-detector spacing of 2.5 mm and a wavelength range of 1000-1350 nm was used to collect data for the multi-linear regression. A linear trendline **116** describing the relationship between the estimated HI **112** and the skin biopsy HI **114** has an R-squared value of 0.68. An R-squared value of one would represent a perfect correlation between the estimated HI **112** and the skin biopsy HI **114**.

[0047] In addition, FIGS. 9-13 illustrate the results of a non-isotonic overhydration study performed on twelve pigs in which a hydration index **120** was calculated from sensors placed at five different locations on the pigs' bodies. In FIG. 9, the sensors were placed on the pigs' sterna; in FIG. 10, the sensors were placed on the rumps; in FIG. 11, the sensors were placed on the cheeks; in FIG. 12, the sensors were placed high on the pigs' chests; and in FIG. 13, the sensors were placed low on the pigs' chests. Data points **122** were calculated from light emitted in the range of 1000-1350 nm, while data points **124** were calculated using light in the range of 1530-1850 nm. One skilled in the art will understand that estimated HI calculated from the 1530-1850 nm range may be lower than the 1000-1350 nm range because the longer wavelengths do not penetrate as deeply into the skin, and shallower skin layers may have lower water content. Data points **126** represent the pigs' hydration indices as determined by skin biopsy. It can be seen from the graphs in FIGS. 9-13 that, for both the 1000-1350 nm range and the 1530-1850 nm range, the estimated HI (data points **122** and **124**) has a high correlation to the chemical analyses from local skin biopsies (data points **126**) for the sensor sites tested.

[0048] Results from studies such as those illustrated in FIGS. 7-13 show that estimation of HI according to embodiments of the present technique may be useful to apply in a clinical setting. The multi-linear regression method may allow for quick, accurate, and non-invasive determination of HI.

[0049] While the invention may be susceptible to various modifications and alternative forms, specific embodiments have been shown by way of example in the drawings and have been described in detail herein. However, it should be understood that the invention is not intended to be limited to the particular forms disclosed. Indeed, the present techniques may not only be applied to measurements of blood oxygen saturation, but these techniques may also be utilized for the measurement and/or analysis of other blood constituents. For example, using the same, different, or additional wavelengths, the present techniques may be utilized in conjunction with the measurement and/or analysis of carboxyhemoglobin, met-hemoglobin, total hemoglobin, intravascular dyes, and/or water content. The invention is to cover all modifications, equivalents, and alternatives falling within the spirit and scope of the invention as defined by the following appended claims.

What is claimed is:

1. A method for calculating one or more body fluid metrics, comprising:

acquiring an absorbance spectrum of a subject's tissue at a range of wavelengths of light;
determining concentrations of a plurality of constituents of the subject's tissue by performing a multi-linear regression of the absorbance spectrum in relation to a plurality of absorbance spectra of the constituents; and
calculating one or more body fluid metrics based on the concentrations.

2. The method of claim 1, wherein the one or more body fluid metrics comprises a hydration index.

3. The method of claim 1, wherein the one or more body fluid metrics comprises a percentage of a constituent of the subject's tissue relative to one or more other constituents.

4. The method of claim 1, wherein the range of wavelengths of light comprises a range of wavelengths of near-infrared light.

5. The method of claim 1, wherein the range of wavelengths of light comprises about 1000 nm to about 1350 nm.

6. The method of claim 1, wherein the range of wavelengths of light comprises about 1530 nm to about 1850 nm.

7. The method of claim 1, wherein the plurality of constituents of the subject's tissue comprise water, proteins, lipids, oxygenated hemoglobin, deoxygenated hemoglobin, or a combination thereof.

8. The method of claim 1, comprising acquiring the plurality of absorbance spectra of the constituents.

9. The method of claim 8, wherein acquiring the absorbance spectrum of the constituent comprises:

transmitting the range of wavelengths of light through an analyte representing the constituent;
measuring intensities of the transmitted light for the range of wavelengths; and
converting the intensities to absorbance measurements for the range of wavelengths.

10. The method of claim 1, comprising processing the absorbance spectrum of the subject's tissue, the absorbance spectra of the constituents, or a combination thereof to correct for instrument errors, sensor errors, or a combination thereof.

11. The method of claim 1, wherein performing the multi-linear regression comprises adjusting a constituent absorbance spectrum based on a subject's body temperature.

12. The method of claim 1, wherein performing the multi-linear regression comprises adding a slope factor to account for a tissue scattering coefficient.

13. The method of claim 1, wherein performing the multi-linear regression comprises adding a pathlength factor to account for a change in mean photon pathlength that occurs with a change in absorption coefficients.

14. The method of claim 1, wherein performing the multi-linear regression comprises adding a calibration factor to account for a shift in an instrument calibration.

15. The method of claim 1, wherein acquiring the absorbance spectrum of the subject's tissue comprises:
acquiring an intensity spectrum of the subject's tissue;
adjusting the intensity spectrum of the subject's tissue by comparison to a reference intensity spectrum; and
converting the adjusted intensity spectrum to the absorbance spectrum.

16. The method of claim 15, wherein the reference intensity spectrum comprises an intensity spectrum of a substance having minimal absorption and scattering similar to tissue, a total reflecting substance, or a combination thereof.

17. A method for calculating one or more body fluid metrics, comprising:

measuring an intensity spectrum of a subject's tissue;
processing the intensity spectrum to determine an absorbance spectrum of the tissue;
performing a multi-linear regression of the absorbance spectrum in relation to a plurality of analyte absorbance spectra, wherein the analytes are representative of tissue constituents; and
determining concentrations of the tissue constituents based on the multi-linear regression.

18. The method of claim 17, comprising determining a relative percentage of at least one tissue constituent to the other tissue constituents.

19. The method of claim 17, wherein the tissue constituents comprise water, proteins, lipids, oxygenated hemoglobin, deoxygenated hemoglobin, or a combination thereof.

20. The method of claim 17, wherein the intensity spectrum of the subject's tissue is measured over a range of near-infrared wavelengths of light.

21. The method of claim 17, wherein the intensity spectrum of the subject's tissue is measured over a range of light from approximately 1000-1350 nm.

22. The method of claim 17, wherein the intensity spectrum of the subject's tissue is measured over a range of light from approximately 1530-1850 nm.

23. The method of claim 17, wherein processing the intensity spectrum comprises adjusting the intensity spectrum to account for a residual instrument signal, a difference in scattering between the intensity spectrum of the subject's tissue and a reference intensity spectrum, or a combination thereof.

24. The method of claim 23, wherein the reference intensity spectrum comprises an intensity spectrum of a substance having minimal absorption and scattering similar to tissue, a total reflecting substance, or a combination thereof.

25. The method of claim 17, wherein performing a multi-linear regression comprises adjusting a constituent absorbance spectrum based on a subject's body temperature, adding a slope factor to account for a tissue scattering coefficient, adding a pathlength factor to account for a change in mean photon pathlength that occurs with a change in absorption coefficients, adding a calibration factor to account for a shift in an instrument calibration, or a combination thereof.

26. A system for calculating one or more body fluid metrics, comprising:

- a sensor configured to emit a range of wavelengths of light into a subject's tissue and to detect reflected, scattered, or transmitted light;
 - a spectrometer configured to process the reflected, scattered, or transmitted light and to generate an absorbance spectrum of the subject's tissue across the range of wavelengths of light;
 - a memory configured to store a plurality of absorbance spectra of tissue constituents across the range of wavelengths of light and to store a multi-linear regression model; and
 - a processor configured to perform a multi-linear regression of the absorbance spectrum of the subject's tissue with respect to the plurality of absorbance spectra of tissue constituents based on the multi-linear regression model and to calculate one or more body fluid metrics based on the multi-linear regression.
- 27.** The system of claim **26**, wherein the one or more body fluid metrics comprise a hydration index.
- 28.** The system of claim **26**, wherein the one or more body fluid metrics comprise a relative percentage of at least one tissue constituent to one or more other tissue constituents.
- 29.** The system of claim **26**, comprising a display configured to display the one or more body fluid metrics.
- 30.** The system of claim **26**, wherein the multi-linear regression comprises a constituent absorbance spectrum based on a subject's body temperature, a slope factor to account for a tissue scattering coefficient, a pathlength factor to account for a change in mean photon pathlength that occurs with a change in absorption coefficients, a calibration factor to account for a shift in an instrument calibration, or a combination thereof.
- 31.** One or more tangible, machine-readable media, comprising code executable to perform the acts of:
- performing a multi-linear regression of an absorbance spectrum of a subject's tissue in relation to a plurality of absorbance spectra of skin constituents; and
 - calculating one or more body fluid metrics based on the multi-linear regression.
- 32.** The tangible, machine-readable media of claim **31**, wherein calculating one or more body fluid metrics comprises calculating a hydration index.
- 33.** The tangible, machine-readable media of claim **31**, wherein calculating one or more body fluid metrics comprises

calculating a percentage of at least one skin constituent relative to one or more other skin constituents.

34. The tangible, machine-readable media of claim **31**, wherein performing a multi-linear regression comprises adjusting a constituent absorbance spectrum based on a subject's body temperature, adding a slope factor to account for a tissue scattering coefficient, adding a pathlength factor to account for a change in mean photon pathlength that occurs with a change in absorption coefficients, adding a calibration factor to account for a shift in an instrument calibration, or a combination thereof.

35. A monitor for calculating one or more body fluid metrics, comprising:

- a spectrometer configured to process light acquired from detection of reflected, scattered, or transmitted light emitted at a range of wavelengths into a subject's tissue and to generate an absorbance spectrum of the subject's tissue across the range of wavelengths of light;
- a memory configured to store a plurality of absorbance spectra of tissue constituents across the range of wavelengths of light and to store a multi-linear regression model; and
- a processor configured to perform a multi-linear regression of the absorbance spectrum of the subject's tissue with respect to the plurality of absorbance spectra of tissue constituents based on the multi-linear regression model and to calculate one or more body fluid metrics based on the multi-linear regression.

36. The monitor of claim **35**, wherein the one or more body fluid metrics comprise a hydration index.

37. The monitor of claim **35**, wherein the one or more body fluid metrics comprise a relative percentage of at least one tissue constituent to one or more other tissue constituents.

38. The monitor of claim **35**, comprising a display configured to display the one or more body fluid metrics.

39. The monitor of claim **35**, wherein the multi-linear regression comprises a constituent absorbance spectrum based on a subject's body temperature, a slope factor to account for a tissue scattering coefficient, a pathlength factor to account for a change in mean photon pathlength that occurs with a change in absorption coefficients, a calibration factor to account for a shift in an instrument calibration, or a combination thereof.

* * * * *

专利名称(译)	用于光谱组织分析物测量的方法和设备		
公开(公告)号	US20080221412A1	公开(公告)日	2008-09-11
申请号	US11/716482	申请日	2007-03-09
[标]申请(专利权)人(译)	内尔科尔普里坦贝内特公司		
申请(专利权)人(译)	NELLCOR PURITAN BENNETT LLC		
当前申请(专利权)人(译)	NELLCOR PURITAN BENNETT LLC		
[标]发明人	BAKER CLARK R DURR NICHOLAS J MOGRI MURTAZA HOARAU CARINE OSTROWSKI RAFAEL DEBRECZENY MARTIN P		
发明人	BAKER,, CLARK R. DURR, NICHOLAS J. MOGRI, MURTAZA HOARAU, CARINE OSTROWSKI, RAFAEL DEBRECZENY, MARTIN P.		
IPC分类号	A61B5/00		
CPC分类号	A61B5/0059 A61B5/4878 A61B5/4869		
其他公开文献	US8175665		
外部链接	Espacenet USPTO		

摘要(译)

提供了一种用于计算体液指标的方法和系统。根据本技术的示例性实施例，提供了一种用于通过近红外光范围内获取对象组织的吸收光谱来计算体液度量的方法，执行吸收光谱的多线性回归。受试者的组织与组织成分的吸收光谱有关，并基于多元线性回归的结果计算体液指标。提供一种系统，其具有用于将光发射到受试者组织中并检测反射，散射或透射光的传感器，用于处理检测到的光并产生受试者组织的吸收光谱的光谱仪，用于存储组织的吸收光谱的存储器成分和多元线性回归模型，以及用于执行多元线性回归和计算体液指标的处理器。

