



US008622903B2

(12) **United States Patent**
Jin et al.

(10) **Patent No.:** **US 8,622,903 B2**
(45) **Date of Patent:** ***Jan. 7, 2014**

(54) **CONTINUOUS GLUCOSE MONITORING
SYSTEM AND METHODS OF USE**

(75) Inventors: **Robert Y. Jin**, Irvine, CA (US); **Mark
K. Sloan**, Redwood City, CA (US)

(73) Assignee: **Abbott Diabetes Care Inc.**, Alameda,
CA (US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 0 days.

This patent is subject to a terminal dis-
claimer.

(21) Appl. No.: **13/481,256**

(22) Filed: **May 25, 2012**

(65) **Prior Publication Data**

US 2012/0232368 A1 Sep. 13, 2012

Related U.S. Application Data

(63) Continuation of application No. 12/902,138, filed on
Oct. 11, 2010, now Pat. No. 8,187,183, which is a
continuation of application No. 10/745,878, filed on
Dec. 26, 2003, now Pat. No. 7,811,231.

(60) Provisional application No. 60/437,374, filed on Dec.
31, 2002.

(51) **Int. Cl.**
A61B 5/00 (2006.01)

(52) **U.S. Cl.**
USPC **600/301; 600/365**

(58) **Field of Classification Search**
USPC 709/203, 204, 218
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,260,656 A	7/1966	Ross, Jr.
3,304,413 A	2/1967	Lehmann et al.
3,651,318 A	3/1972	Czekajewski

(Continued)

FOREIGN PATENT DOCUMENTS

DE	2903216	8/1979
DE	227029	9/1985

(Continued)

OTHER PUBLICATIONS

Abruna, H. D., et al., "Rectifying Interfaces Using Two-Layer Films
of Electrochemically Polymerized Vinylpyridine and
Vinylbipyridine Complexes of Ruthenium and Iron on Electrodes",
Journal of the American Chemical Society, vol. 103, No. 1, 1981, pp.
1-5.

(Continued)

Primary Examiner — Bill Thomson


Assistant Examiner — Shirley Jian

(74) *Attorney, Agent, or Firm* — Jackson & Co., LLP

(57) **ABSTRACT**

A continuous glucose monitoring system including a sensor
configured to detect one or more glucose levels, a transmitter
operatively coupled to the sensor, the transmitter configured
to receive the detected one or more glucose levels, the trans-
mitter further configured to transmit signals corresponding to
the detected one or more glucose levels, and a receiver opera-
tively coupled to the transmitter configured to receive trans-
mitted signals corresponding to the detected one or more
glucose levels, and methods thereof, are disclosed. In one
aspect, the transmitter may be configured to transmit a current
data point and at least one previous data point, the current data
point and the at least one previous data point corresponding to
the detected one or more glucose levels.

20 Claims, 6 Drawing Sheets

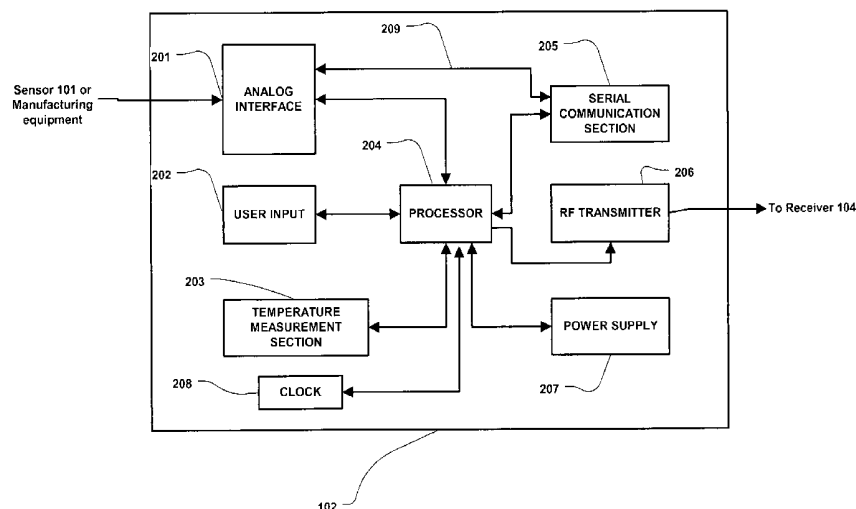

(56)

References Cited

U.S. PATENT DOCUMENTS

3,653,841	A	4/1972	Klein	4,543,955	A	10/1985	Schroeppel
3,698,386	A	10/1972	Fried	4,545,382	A	10/1985	Higgins et al.
3,719,564	A	3/1973	Lilly, Jr. et al.	4,552,840	A	11/1985	Riffer
3,768,014	A	10/1973	Smith et al.	4,560,534	A	12/1985	Kung et al.
3,776,832	A	12/1973	Oswin et al.	4,569,589	A	2/1986	Neufeld
3,785,939	A	1/1974	Hsu	4,571,292	A	2/1986	Liu et al.
3,919,051	A	11/1975	Koch et al.	4,573,994	A	3/1986	Fischell et al.
3,926,760	A	12/1975	Allen et al.	4,581,336	A	4/1986	Malloy et al.
3,972,320	A	8/1976	Kalman	4,595,011	A	6/1986	Phillips
3,979,274	A	9/1976	Newman	4,595,479	A	6/1986	Kimura et al.
4,008,717	A	2/1977	Kowarski	4,619,754	A	10/1986	Niki et al.
4,016,866	A	4/1977	Lawton	4,619,793	A	10/1986	Lee
4,036,749	A	7/1977	Anderson	4,627,445	A	12/1986	Garcia et al.
4,055,175	A	10/1977	Clemens et al.	4,627,908	A	12/1986	Miller
4,059,406	A	11/1977	Fleet	4,633,878	A	1/1987	Bombardien
4,076,596	A	2/1978	Connery et al.	4,633,881	A	1/1987	Moore et al.
4,098,574	A	7/1978	Dappen	4,637,403	A	1/1987	Garcia et al.
4,100,048	A	7/1978	Pompei et al.	RE32,361	E	2/1987	Duggan
4,129,128	A	12/1978	McFarlane	4,648,408	A	3/1987	Hutcheson et al.
4,151,845	A	5/1979	Clemens	4,650,547	A	3/1987	Gough
4,154,231	A	5/1979	Russell	4,653,513	A	3/1987	Dombrowski
4,168,205	A	9/1979	Danniger et al.	4,654,197	A	3/1987	Lilja et al.
4,172,770	A	10/1979	Semersky et al.	4,655,880	A	4/1987	Liu
4,178,916	A	12/1979	McNamara	4,655,885	A	4/1987	Hill et al.
4,206,755	A	6/1980	Klein	4,658,463	A	4/1987	Sugita et al.
4,224,125	A	9/1980	Nakamura et al.	4,671,288	A	6/1987	Gough
4,240,438	A	12/1980	Updike et al.	4,674,652	A	6/1987	Aten et al.
4,240,889	A	12/1980	Yoda et al.	4,679,562	A	7/1987	Luksha
4,245,634	A	1/1981	Albisser et al.	4,680,268	A	7/1987	Clark, Jr.
4,247,297	A	1/1981	Berti et al.	4,682,602	A	7/1987	Prohaska
4,271,449	A	6/1981	Grogan	4,684,537	A	8/1987	Graetzel et al.
4,318,784	A	3/1982	Higgins et al.	4,685,463	A	8/1987	Williams
4,327,725	A	5/1982	Cortese et al.	4,686,624	A	8/1987	Blum et al.
4,331,869	A	5/1982	Rollo	4,703,756	A	11/1987	Gough et al.
4,340,458	A	7/1982	Lerner et al.	4,714,462	A	12/1987	DiDomenico
4,344,438	A	8/1982	Schultz	4,718,893	A	1/1988	Dorman
4,352,960	A	10/1982	Dormer et al.	4,721,601	A	1/1988	Wrighton et al.
4,356,074	A	10/1982	Johnson	4,721,677	A	1/1988	Clark, Jr.
4,365,637	A	12/1982	Johnson	4,726,378	A	2/1988	Kaplan
4,366,033	A	12/1982	Richter et al.	4,726,716	A	2/1988	McGuire
4,375,399	A	3/1983	Havas et al.	4,731,726	A	3/1988	Allen, III
4,384,586	A	5/1983	Christiansen	4,749,985	A	6/1988	Corsberg
4,390,621	A	6/1983	Bauer	4,750,496	A	6/1988	Reinhart
4,392,933	A	7/1983	Nakamura et al.	4,757,022	A	7/1988	Shults et al.
4,401,122	A	8/1983	Clark, Jr.	4,758,323	A	7/1988	Davis et al.
4,404,066	A	9/1983	Johnson	4,759,371	A	7/1988	Franetzki
4,407,959	A	10/1983	Tsuji et al.	4,759,828	A	7/1988	Young et al.
4,417,588	A	11/1983	Houghton et al.	4,764,416	A	8/1988	Ueyama et al.
4,418,148	A	11/1983	Oberhardt	4,776,944	A	10/1988	Janata et al.
4,420,564	A	12/1983	Tsuji et al.	4,777,953	A	10/1988	Ash et al.
4,425,920	A	1/1984	Bourland et al.	4,779,618	A	10/1988	Mund et al.
4,427,004	A	1/1984	Miller et al.	4,781,798	A	11/1988	Gough
4,427,770	A	1/1984	Chen et al.	4,784,736	A	11/1988	Lonsdale et al.
4,431,004	A	2/1984	Bessman et al.	4,795,707	A	1/1989	Niiyama et al.
4,436,094	A	3/1984	Cerami	4,796,634	A	1/1989	Huntsman et al.
4,440,175	A	4/1984	Wilkins	4,803,625	A	2/1989	Fu et al.
4,444,892	A	4/1984	Malmros	4,805,624	A	2/1989	Yao et al.
4,450,842	A	5/1984	Zick et al.	4,813,424	A	3/1989	Wilkins
4,458,686	A	7/1984	Clark, Jr.	4,815,469	A	3/1989	Cohen et al.
4,461,691	A	7/1984	Frank	4,820,399	A	4/1989	Senda et al.
4,467,811	A	8/1984	Clark, Jr.	4,822,337	A	4/1989	Newhouse et al.
4,469,110	A	9/1984	Slama	4,830,959	A	5/1989	McNeil et al.
4,477,314	A	10/1984	Richter et al.	4,832,797	A	5/1989	Vadgama et al.
4,478,976	A	10/1984	Goertz et al.	4,835,372	A	5/1989	Gombrich et al.
4,483,924	A	11/1984	Tsuji et al.	RE32,947	E	6/1989	Dormer et al.
4,484,987	A	11/1984	Gough	4,837,049	A	6/1989	Byers et al.
4,494,950	A	1/1985	Fischell	4,840,893	A	6/1989	Hill et al.
4,512,348	A	4/1985	Uchigaki et al.	RE32,974	E	7/1989	Porat et al.
RE31,916	E	6/1985	Oswin et al.	4,844,076	A	7/1989	Lesho et al.
4,522,690	A	6/1985	Venkatsetty	4,845,035	A	7/1989	Fanta et al.
4,524,114	A	6/1985	Samuels et al.	4,848,351	A	7/1989	Finch
4,526,661	A	7/1985	Steckhan et al.	4,854,322	A	8/1989	Ash et al.
4,527,240	A	7/1985	Kvitash	4,856,340	A	8/1989	Garrison
4,534,356	A	8/1985	Papadakis	4,857,713	A	8/1989	Brown
4,538,616	A	9/1985	Rogoff	4,858,617	A	8/1989	Sanders
				4,870,561	A	9/1989	Love et al.
				4,871,351	A	10/1989	Feingold
				4,871,440	A	10/1989	Nagata et al.
				4,874,499	A	10/1989	Smith et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

4,874,500 A	10/1989	Madou et al.	5,111,539 A	5/1992	Hiruta et al.
4,890,620 A	1/1990	Gough	5,111,818 A	5/1992	Suzuji et al.
4,890,621 A	1/1990	Hakky	5,114,678 A	5/1992	Crawford et al.
4,894,137 A	1/1990	Takizawa et al.	5,120,420 A	6/1992	Nankai et al.
4,897,162 A	1/1990	Lewandowski et al.	5,120,421 A	6/1992	Glass et al.
4,897,173 A	1/1990	Nankai et al.	5,126,034 A	6/1992	Carter et al.
4,899,839 A	2/1990	Dessertine et al.	5,126,247 A	6/1992	Palmer et al.
4,909,908 A	3/1990	Ross et al.	5,130,009 A	7/1992	Marsoner et al.
4,911,794 A	3/1990	Parce et al.	5,133,856 A	7/1992	Yamaguchi et al.
4,917,800 A	4/1990	Lonsdale et al.	5,134,391 A	7/1992	Okada
4,919,141 A	4/1990	Zier et al.	5,135,003 A	8/1992	Souma
4,919,767 A	4/1990	Vadgama et al.	5,139,023 A	8/1992	Stanley et al.
4,920,969 A	5/1990	Suzuki	5,140,393 A	8/1992	Hijikihigawa et al.
4,920,977 A	5/1990	Haynes	5,141,868 A	8/1992	Shanks et al.
4,923,586 A	5/1990	Katayama et al.	5,161,532 A	11/1992	Joseph
4,925,268 A	5/1990	Iyer et al.	5,165,407 A	11/1992	Wilson et al.
4,927,516 A	5/1990	Yamaguchi et al.	5,168,046 A	12/1992	Hamamoto et al.
4,931,795 A	6/1990	Gord	5,174,291 A	12/1992	Schoonen et al.
4,934,369 A	6/1990	Maxwell	5,176,644 A	1/1993	Srisathapat et al.
4,935,105 A	6/1990	Churchouse	5,176,662 A	1/1993	Bartholomew et al.
4,935,345 A	6/1990	Guibeau et al.	5,182,707 A	1/1993	Cooper et al.
4,936,956 A	6/1990	Wrighton	5,184,359 A	2/1993	Tsukamura et al.
4,938,860 A	7/1990	Wogoman	5,185,256 A	2/1993	Nankai et al.
4,942,127 A	7/1990	Wada et al.	5,190,041 A	3/1993	Palti
4,944,299 A	7/1990	Silvian	5,192,415 A	3/1993	Yoshioka et al.
4,945,045 A	7/1990	Forrest et al.	5,192,416 A	3/1993	Wang et al.
4,950,378 A	8/1990	Nagara	5,193,539 A	3/1993	Schulman et al.
4,953,552 A	9/1990	DeMarzo	5,193,540 A	3/1993	Schulman et al.
4,954,129 A	9/1990	Giuliani et al.	5,197,322 A	3/1993	Indravudh
4,957,115 A	9/1990	Selker	5,198,367 A	3/1993	Aizawa et al.
4,958,632 A	9/1990	Duggan	5,200,051 A	4/1993	Cozzette et al.
4,968,400 A	11/1990	Shimomura et al.	5,202,261 A	4/1993	Musho et al.
4,969,468 A	11/1990	Byers et al.	5,205,920 A	4/1993	Oyama et al.
4,970,145 A	11/1990	Bennetto et al.	5,206,145 A	4/1993	Cattell
4,974,929 A	12/1990	Curry	5,208,154 A	5/1993	Weaver et al.
4,979,509 A	12/1990	Hakky	5,209,229 A	5/1993	Gilli
4,986,271 A	1/1991	Wilkins	5,215,887 A	6/1993	Saito
4,990,845 A	2/1991	Gord	5,216,597 A	6/1993	Beckers
4,991,582 A	2/1991	Byers et al.	5,217,442 A	6/1993	Davis
4,994,068 A	2/1991	Hufnagie	5,217,595 A	6/1993	Smith et al.
4,994,167 A	2/1991	Shults et al.	5,227,042 A	7/1993	Zawodzinski et al.
4,995,402 A	2/1991	Smith et al.	5,229,282 A	7/1993	Yoshioka et al.
5,001,054 A	3/1991	Wagner	5,246,867 A	9/1993	Lakowicz et al.
5,002,054 A	3/1991	Ash et al.	5,250,439 A	10/1993	Musho et al.
5,007,427 A	4/1991	Suzuki et al.	5,251,126 A	10/1993	Kahn et al.
5,016,172 A	5/1991	Dessertine	5,257,971 A	11/1993	Lord et al.
5,016,201 A	5/1991	Bryan et al.	5,257,980 A	11/1993	Van Antwerp et al.
5,019,974 A	5/1991	Beckers	5,261,401 A	11/1993	Baker et al.
5,034,192 A	7/1991	Wrighton et al.	5,262,035 A	11/1993	Gregg et al.
5,035,860 A	7/1991	Kleingeld et al.	5,262,305 A	11/1993	Heller et al.
5,036,860 A	8/1991	Leigh et al.	5,264,103 A	11/1993	Yoshioka et al.
5,036,861 A	8/1991	Sembrowich et al.	5,264,104 A	11/1993	Gregg et al.
5,037,527 A	8/1991	Hayashi et al.	5,264,105 A	11/1993	Gregg et al.
5,049,487 A	9/1991	Phillips et al.	5,264,106 A	11/1993	McAleer et al.
5,050,612 A	9/1991	Matsumura	5,265,888 A	11/1993	Yamamoto et al.
5,055,171 A	10/1991	Peck	5,266,179 A	11/1993	Nankai et al.
5,058,592 A	10/1991	Whisler	5,269,212 A	12/1993	Peters et al.
5,063,081 A	11/1991	Cozzette et al.	5,271,815 A	12/1993	Wong
5,068,536 A	11/1991	Rosenthal	5,272,060 A	12/1993	Hamamoto et al.
5,070,535 A	12/1991	Hochmair et al.	5,275,159 A	1/1994	Griebel
5,073,500 A	12/1991	Saito et al.	5,278,079 A	1/1994	Gubinski et al.
5,077,476 A	12/1991	Rosenthal	5,279,294 A	1/1994	Anderson
5,078,854 A	1/1992	Burgess et al.	5,282,950 A	2/1994	Dietze et al.
5,082,550 A	1/1992	Rishpon et al.	5,284,156 A	2/1994	Schramm et al.
5,082,786 A	1/1992	Nakamoto	5,285,792 A	2/1994	Sjoquist et al.
5,084,828 A	1/1992	Kaufman et al.	5,286,362 A	2/1994	Hoenes et al.
5,089,112 A	2/1992	Skotheim et al.	5,286,364 A	2/1994	Yacynych et al.
5,094,951 A	3/1992	Rosenberg	5,288,636 A	2/1994	Pollmann et al.
5,095,904 A	3/1992	Seligman et al.	5,291,887 A	3/1994	Stanley et al.
5,096,560 A	3/1992	Takai et al.	5,293,546 A	3/1994	Tadros et al.
5,096,836 A	3/1992	Macho et al.	5,299,571 A	4/1994	Mastrototaro
5,101,814 A	4/1992	Palti	5,304,468 A	4/1994	Phillips et al.
5,106,365 A	4/1992	Hernandez	5,307,263 A	4/1994	Brown
5,108,564 A	4/1992	Szuminsky et al.	5,309,919 A	5/1994	Snell et al.
5,109,850 A	5/1992	Blanco et al.	5,310,885 A	5/1994	Maier et al.
			5,320,098 A	6/1994	Davidson
			5,320,725 A	6/1994	Gregg et al.
			5,322,063 A	6/1994	Allen et al.
			5,324,303 A	6/1994	Strong et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

5,324,316 A	6/1994	Schulman et al.	5,525,511 A	6/1996	D'Costa
5,326,449 A	7/1994	Cunningham	5,526,120 A	6/1996	Jina et al.
5,337,258 A	8/1994	Dennis	5,527,307 A	6/1996	Srisathapat et al.
5,337,747 A	8/1994	Neftei	5,529,676 A	6/1996	Maley et al.
5,340,722 A	8/1994	Wolfbeis et al.	5,531,878 A	7/1996	Vadgama et al.
5,342,789 A	8/1994	Chick et al.	5,538,511 A	7/1996	Van Antwerp et al.
5,352,348 A	10/1994	Young et al.	5,545,152 A	8/1996	Funderburk et al.
5,356,348 A	10/1994	Bellio et al.	5,545,191 A	8/1996	Mann et al.
5,356,786 A	10/1994	Heller et al.	5,549,113 A	8/1996	Halleck et al.
5,358,514 A	10/1994	Schulman et al.	5,549,115 A	8/1996	Morgan et al.
5,364,797 A	11/1994	Olson et al.	5,552,027 A	9/1996	Birkle et al.
5,366,609 A	11/1994	White et al.	5,554,166 A	9/1996	Lange et al.
5,368,028 A	11/1994	Palti	5,556,524 A	9/1996	Albers
5,370,622 A	12/1994	Livingston et al.	5,560,357 A	10/1996	Faupei et al.
5,371,687 A	12/1994	Holmes, II et al.	5,562,713 A	10/1996	Silvian
5,371,734 A	12/1994	Fischer	5,565,085 A	10/1996	Ikeda et al.
5,372,133 A	12/1994	Hogen Esch	5,567,302 A	10/1996	Song et al.
5,376,070 A	12/1994	Purvis et al.	5,568,806 A	10/1996	Cheney, II et al.
5,376,251 A	12/1994	Kaneko et al.	5,569,186 A	10/1996	Lord et al.
5,377,258 A	12/1994	Bro	5,569,212 A	10/1996	Brown
5,378,628 A	1/1995	Gratzel et al.	5,573,647 A	11/1996	Maley et al.
5,379,238 A	1/1995	Stark	5,575,895 A	11/1996	Ikeda et al.
5,380,422 A	1/1995	Negishis et al.	5,580,527 A	12/1996	Bell et al.
5,382,346 A	1/1995	Uenoyama et al.	5,580,794 A	12/1996	Allen
5,387,327 A	2/1995	Khan	5,582,184 A	12/1996	Erickson et al.
5,390,671 A	2/1995	Lord et al.	5,582,697 A	12/1996	Ikeda et al.
5,391,250 A	2/1995	Cheney, II et al.	5,582,698 A	12/1996	Flaherty et al.
5,393,903 A	2/1995	Gratzel et al.	5,584,813 A	12/1996	Livingston et al.
5,395,504 A	3/1995	Saurer et al.	5,586,553 A	12/1996	Halli et al.
5,399,823 A	3/1995	McCusker	5,589,326 A	12/1996	Deng et al.
5,400,782 A	3/1995	Beaubiah	5,593,852 A	1/1997	Heller et al.
5,408,999 A	4/1995	Singh et al.	5,594,906 A	1/1997	Holmes, II et al.
5,410,471 A	4/1995	Alyfuku et al.	5,596,150 A	1/1997	Arndt et al.
5,410,474 A	4/1995	Fox	5,596,994 A	1/1997	Bro
5,411,647 A	5/1995	Johnson et al.	5,601,435 A	2/1997	Quy
5,413,690 A	5/1995	Kost et al.	5,601,694 A	2/1997	Maley et al.
5,422,246 A	6/1995	Koopal et al.	5,605,152 A	2/1997	Slate et al.
5,431,160 A	7/1995	Wilkins	5,611,900 A	3/1997	Worden et al.
5,431,691 A	7/1995	Snell et al.	5,615,671 A	4/1997	Schoonen et al.
5,431,921 A	7/1995	Thombre	5,616,222 A	4/1997	Maley et al.
5,433,710 A	7/1995	Van Antwerp et al.	5,617,851 A	4/1997	Lipkovker
5,437,973 A	8/1995	Vadgama et al.	5,623,925 A	4/1997	Swenson et al.
5,437,999 A	8/1995	Dieboid et al.	5,628,309 A	5/1997	Brown
5,445,611 A	8/1995	Eppstein et al.	5,628,310 A	5/1997	Rao et al.
5,445,920 A	8/1995	Saito	5,628,890 A	5/1997	Carter et al.
5,456,692 A	10/1995	Smith, Jr. et al.	5,629,981 A	5/1997	Nerlikar
5,456,940 A	10/1995	Funderburk	5,637,095 A	6/1997	Nason et al.
5,458,140 A	10/1995	Eppstein et al.	5,640,764 A	6/1997	Strojniak
5,460,618 A	10/1995	Harreld	5,640,954 A	6/1997	Pfeiffer et al.
5,462,064 A	10/1995	D'Angelo et al.	5,643,212 A	7/1997	Coutre et al.
5,462,525 A	10/1995	Srisathapat et al.	5,647,853 A	7/1997	Feldmann et al.
5,462,645 A	10/1995	Albery et al.	5,650,062 A	7/1997	Ikeda et al.
5,466,218 A	11/1995	Srisathapat et al.	5,651,767 A	7/1997	Schulman et al.
5,469,846 A	11/1995	Khan	5,651,869 A	7/1997	Yoshioka et al.
5,472,317 A	12/1995	Field et al.	5,660,163 A	8/1997	Schulman et al.
5,476,460 A	12/1995	Montalvo	5,665,065 A	9/1997	Colman et al.
5,477,855 A	12/1995	Schindler et al.	5,667,983 A	9/1997	Abel et al.
5,482,473 A	1/1996	Lord et al.	5,670,031 A	9/1997	Hintsche et al.
5,484,404 A	1/1996	Schulman et al.	5,678,571 A	10/1997	Brown
5,487,751 A	1/1996	Radons et al.	5,679,690 A	10/1997	Andre et al.
5,491,474 A	2/1996	Suni et al.	5,680,858 A	10/1997	Hansen et al.
5,494,562 A	2/1996	Maley et al.	5,682,233 A	10/1997	Brinda
5,496,453 A	3/1996	Uenoyama et al.	5,686,717 A	11/1997	Knowles et al.
5,497,772 A	3/1996	Schulman et al.	5,695,623 A	12/1997	Michel et al.
5,501,956 A	3/1996	Wada et al.	5,695,949 A	12/1997	Galen et al.
5,505,709 A	4/1996	Funderburk	5,701,894 A	12/1997	Cherry et al.
5,505,713 A	4/1996	Van Antwerp et al.	5,704,922 A	1/1998	Brown
5,507,288 A	4/1996	Bocker et al.	5,707,502 A	1/1998	McCaffrey et al.
5,508,171 A	4/1996	Walling et al.	5,708,247 A	1/1998	McAleer et al.
5,509,410 A	4/1996	Hill et al.	5,710,630 A	1/1998	Essenpreis et al.
5,514,103 A	5/1996	Srisathapat et al.	5,711,001 A	1/1998	Bussan et al.
5,514,253 A	5/1996	Davis et al.	5,711,297 A	1/1998	Iliff et al.
5,518,006 A	5/1996	Mawhirt et al.	5,711,861 A	1/1998	Ward et al.
5,520,787 A	5/1996	Hanagan et al.	5,711,862 A	1/1998	Sakoda et al.
5,522,865 A	6/1996	Schulman et al.	5,711,868 A	1/1998	Maley et al.
			5,718,234 A	2/1998	Warden et al.
			5,720,733 A	2/1998	Brown
			5,720,862 A	2/1998	Hamamoto et al.
			5,721,783 A	2/1998	Anderson

(56)

References Cited

U.S. PATENT DOCUMENTS

5,722,397 A	3/1998	Eppstein	5,945,345 A	8/1999	Blatt et al.
5,727,548 A	3/1998	Hill et al.	5,947,921 A	9/1999	Johnson et al.
5,730,124 A	3/1998	Yamauchi	5,948,512 A	9/1999	Kubota et al.
5,730,654 A	3/1998	Brown	5,950,632 A	9/1999	Reber et al.
5,735,273 A	4/1998	Kurnik et al.	5,951,300 A	9/1999	Brown
5,735,285 A	4/1998	Albert et al.	5,951,492 A	9/1999	Douglas et al.
5,741,211 A	4/1998	Renirie et al.	5,951,521 A	9/1999	Mastrototaro et al.
5,741,688 A	4/1998	Oxenboll et al.	5,951,836 A	9/1999	McAleer et al.
5,746,217 A	5/1998	Erickson et al.	5,954,643 A	9/1999	Van Antwerp
5,750,926 A	5/1998	Schulman et al.	5,954,685 A	9/1999	Tierney
5,770,028 A	6/1998	Maley et al.	5,954,700 A	9/1999	Kovelman
5,771,001 A	6/1998	Cobb	5,956,501 A	9/1999	Brown
5,771,890 A	6/1998	Tamada	5,957,854 A	9/1999	Besson et al.
5,772,586 A	6/1998	Heinonen et al.	5,957,890 A	9/1999	Mann et al.
5,777,060 A	7/1998	Van Antwerp	5,957,958 A	9/1999	Schulman et al.
5,779,665 A	7/1998	Mastrototaro et al.	5,960,403 A	9/1999	Brown
5,782,814 A	7/1998	Brown et al.	5,961,451 A	10/1999	Reber et al.
5,785,681 A	7/1998	Indravudh	5,964,993 A	10/1999	Blubaugh, Jr. et al.
5,786,439 A	7/1998	Van Antwerp et al.	5,965,380 A	10/1999	Heller et al.
5,786,584 A	7/1998	Button et al.	5,968,839 A	10/1999	Blatt et al.
5,788,678 A	8/1998	Van Antwerp	5,971,922 A	10/1999	Arita et al.
5,791,344 A	8/1998	Schulman et al.	5,971,941 A	10/1999	Simons et al.
5,792,117 A	8/1998	Brown	5,974,124 A	10/1999	Schlueter, Jr. et al.
5,800,420 A	9/1998	Gross et al.	5,977,476 A	11/1999	Guha et al.
5,804,048 A	9/1998	Wong et al.	5,981,294 A	11/1999	Blatt et al.
5,806,517 A	9/1998	Gerhardt et al.	5,989,409 A	11/1999	Kurnik et al.
5,807,315 A	9/1998	Van Antwerp et al.	5,994,476 A	11/1999	Shin et al.
5,807,375 A	9/1998	Gross et al.	5,995,860 A	11/1999	Sun et al.
5,814,599 A	9/1998	Mitragotri et al.	5,997,476 A	12/1999	Brown
5,820,551 A	10/1998	Hill et al.	5,999,848 A	12/1999	Gord et al.
5,820,570 A	10/1998	Erickson et al.	5,999,849 A	12/1999	Gord et al.
5,820,622 A	10/1998	Gross et al.	6,001,067 A	12/1999	Shults et al.
5,822,715 A	10/1998	Worthington et al.	6,002,954 A	12/1999	Van Antwerp et al.
5,825,488 A	10/1998	Kohl et al.	6,002,961 A	12/1999	Mitragotri et al.
5,827,179 A	10/1998	Lichter et al.	6,004,441 A	12/1999	Fujiwara et al.
5,827,183 A	10/1998	Kurnik et al.	6,011,984 A	1/2000	Van Antwerp et al.
5,827,184 A	10/1998	Netherly et al.	6,014,577 A	1/2000	Henning et al.
5,828,943 A	10/1998	Brown	6,018,678 A	1/2000	Mitragotri et al.
5,830,132 A	11/1998	Robinson	6,023,629 A	2/2000	Tamada
5,830,341 A	11/1998	Gilmartin	6,024,699 A	2/2000	Surwit et al.
5,832,448 A	11/1998	Brown	6,026,320 A	2/2000	Carlson et al.
5,834,224 A	11/1998	Ruger et al.	6,027,459 A	2/2000	Shain et al.
5,837,454 A	11/1998	Cozzette et al.	6,027,692 A	2/2000	Galen et al.
5,837,546 A	11/1998	Allen et al.	6,032,059 A	2/2000	Henning et al.
5,840,020 A	11/1998	Heinonen et al.	6,032,199 A	2/2000	Lim et al.
5,842,983 A	12/1998	Abel et al.	6,033,866 A	3/2000	Guo et al.
5,843,140 A	12/1998	Strojniak	6,035,237 A	3/2000	Schulman et al.
5,846,702 A	12/1998	Deng et al.	6,040,194 A	3/2000	Chick et al.
5,846,744 A	12/1998	Athey et al.	6,041,253 A	3/2000	Kost et al.
5,851,197 A	12/1998	Marano et al.	6,043,437 A	3/2000	Schulman et al.
5,854,078 A	12/1998	Asher et al.	6,049,727 A	4/2000	Crothall
5,854,189 A	12/1998	Kruse et al.	6,056,718 A	5/2000	Funderburk et al.
5,857,967 A	1/1999	Frid et al.	6,063,459 A	5/2000	Velte
5,857,983 A	1/1999	Douglas et al.	6,066,243 A	5/2000	Anderson et al.
5,860,917 A	1/1999	Comanor et al.	6,067,474 A	5/2000	Schulman et al.
5,862,803 A *	1/1999	Besson et al. 600/508	6,068,615 A	5/2000	Brown et al.
5,872,713 A	2/1999	Douglas et al.	6,071,249 A	6/2000	Cunningham et al.
5,876,484 A	3/1999	Raskin et al.	6,071,251 A	6/2000	Cunningham et al.
5,879,163 A	3/1999	Brown et al.	6,071,294 A	6/2000	Simons et al.
5,879,311 A	3/1999	Duchon et al.	6,071,391 A	6/2000	Gotoh et al.
5,880,829 A	3/1999	Kauhaniemi et al.	6,081,736 A	6/2000	Colvin et al.
5,882,494 A	3/1999	Van Antwerp	6,083,710 A	7/2000	Heller et al.
5,885,211 A	3/1999	Eppstein et al.	6,088,608 A	7/2000	Schulman et al.
5,887,133 A	3/1999	Brown et al.	6,091,975 A	7/2000	Daddona et al.
5,897,493 A	4/1999	Brown	6,091,976 A	7/2000	Pfeiffer et al.
5,898,025 A	4/1999	Burg et al.	6,093,156 A	7/2000	Cunningham et al.
5,899,855 A	5/1999	Brown	6,093,167 A	7/2000	Houben et al.
5,913,310 A	6/1999	Brown	6,093,172 A	7/2000	Funderburk et al.
5,917,346 A	6/1999	Gord	6,097,831 A	8/2000	Wieck et al.
5,918,603 A	7/1999	Brown	6,099,484 A	8/2000	Douglas et al.
5,925,021 A	7/1999	Castellano et al.	6,101,478 A	8/2000	Brown
5,931,791 A	8/1999	Saltzstein et al.	6,103,033 A	8/2000	Say et al.
5,933,136 A	8/1999	Brown	6,106,780 A	8/2000	Douglas et al.
5,940,801 A	8/1999	Brown	6,110,148 A	8/2000	Brown et al.
5,942,979 A	8/1999	Luppino	6,110,152 A	8/2000	Kovelman
			6,113,578 A	9/2000	Brown
			6,119,028 A	9/2000	Schulman et al.
			6,120,676 A	9/2000	Heller et al.
			6,121,009 A	9/2000	Heller et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,122,351	A	9/2000	Schlueter, Jr. et al.	6,295,506	B1	9/2001	Heinonen et al.
6,125,978	A	10/2000	Ando et al.	6,298,254	B2	10/2001	Tamada
6,134,461	A	10/2000	Say et al.	6,299,578	B1	10/2001	Kurnik et al.
6,134,504	A	10/2000	Douglas et al.	6,299,757	B1	10/2001	Feldman et al.
6,139,718	A	10/2000	Kurnik et al.	6,301,499	B1	10/2001	Carlson et al.
6,141,573	A	10/2000	Kurnik et al.	6,304,766	B1	10/2001	Colvin, Jr. et al.
6,142,939	A	11/2000	Eppstein et al.	6,309,351	B1	10/2001	Kurnik et al.
6,143,164	A	11/2000	Heller et al.	6,309,884	B1	10/2001	Cooper et al.
6,144,837	A	11/2000	Quy	6,315,721	B2	11/2001	Schulman et al.
6,144,869	A	11/2000	Berner et al.	6,319,540	B1	11/2001	Van Antwerp et al.
6,144,922	A	11/2000	Douglas et al.	6,326,160	B1	12/2001	Dunn et al.
6,148,094	A	11/2000	Kinsella	6,329,161	B1	12/2001	Heller et al.
6,150,128	A	11/2000	Uretsky	6,329,929	B1	12/2001	Weijand et al.
6,151,586	A	11/2000	Brown	6,330,426	B2	12/2001	Brown et al.
6,153,062	A	11/2000	Saito et al.	6,330,464	B1	12/2001	Colvin, Jr. et al.
6,153,069	A	11/2000	Pottgen et al.	6,331,518	B2	12/2001	Hemm et al.
6,159,147	A	12/2000	Lichter et al.	6,334,778	B1	1/2002	Brown
6,161,095	A	12/2000	Brown	6,336,900	B1	1/2002	Alleckson et al.
6,162,611	A	12/2000	Heller et al.	6,338,790	B1	1/2002	Feldman et al.
6,162,639	A	12/2000	Douglas	6,340,421	B1	1/2002	Vachon et al.
6,167,362	A	12/2000	Brown et al.	6,341,232	B1	1/2002	Conn et al.
6,168,563	B1	1/2001	Brown	6,356,776	B1	3/2002	Berner et al.
6,170,318	B1	1/2001	Lewis	6,360,888	B1	3/2002	McIvor et al.
6,175,752	B1	1/2001	Say et al.	6,366,793	B1	4/2002	Bell et al.
6,180,416	B1	1/2001	Kurnik et al.	6,366,794	B1	4/2002	Moussy et al.
6,186,145	B1	2/2001	Brown	6,368,141	B1	4/2002	Van Antwerp et al.
6,192,891	B1	2/2001	Gravel et al.	6,368,274	B1	4/2002	Van Antwerp et al.
6,193,873	B1	2/2001	Ohara et al.	6,370,410	B2	4/2002	Kurnik et al.
6,196,970	B1	3/2001	Brown	6,379,301	B1	4/2002	Worthington et al.
6,198,957	B1	3/2001	Green	6,383,767	B1	5/2002	Polak
6,201,979	B1	3/2001	Kurnik et al.	6,387,048	B1	5/2002	Schulman et al.
6,201,980	B1	3/2001	Darrow et al.	6,391,643	B1	5/2002	Chen et al.
6,206,841	B1	3/2001	Cunningham et al.	6,393,318	B1	5/2002	Conn et al.
6,206,856	B1	3/2001	Mahurkar	6,398,562	B1	6/2002	Butler et al.
6,208,894	B1	3/2001	Schulman et al.	6,405,066	B1	6/2002	Essenpreis et al.
6,210,272	B1	4/2001	Brown	6,413,393	B1	7/2002	Van Antwerp et al.
6,210,976	B1	4/2001	Sabbadini	6,418,332	B1	7/2002	Mastrototaro et al.
6,212,416	B1	4/2001	Ward et al.	6,424,847	B1	7/2002	Mastrototaro et al.
6,219,565	B1	4/2001	Cupp et al.	6,427,088	B1	7/2002	Bowman, IV et al.
6,219,574	B1	4/2001	Cormier et al.	6,434,409	B1	8/2002	Pfeiffer et al.
6,224,745	B1	5/2001	Baltruschat	6,438,414	B1	8/2002	Conn et al.
6,232,130	B1	5/2001	Wolf	6,440,068	B1	8/2002	Brown et al.
6,232,370	B1	5/2001	Kubota et al.	6,441,747	B1	8/2002	Khair et al.
6,233,471	B1	5/2001	Berner et al.	6,442,637	B1	8/2002	Hawkins et al.
6,233,539	B1	5/2001	Brown	6,443,942	B2	9/2002	Van Antwerp et al.
6,239,925	B1	5/2001	Ardrey et al.	6,454,710	B1	9/2002	Ballerstadt et al.
6,241,862	B1	6/2001	McAleer et al.	6,462,162	B2	10/2002	Van Antwerp et al.
6,246,330	B1	6/2001	Nielsen	6,464,848	B1	10/2002	Matsumoto
6,246,992	B1	6/2001	Brown	6,466,810	B1	10/2002	Ward et al.
6,248,065	B1	6/2001	Brown	6,468,222	B1	10/2002	Mault et al.
6,248,067	B1	6/2001	Causey, III et al.	6,472,122	B1	10/2002	Schulman et al.
6,248,093	B1	6/2001	Moberg	6,475,750	B1	11/2002	Han et al.
6,251,260	B1	6/2001	Heller et al.	6,477,395	B2	11/2002	Schulman et al.
6,252,032	B1	6/2001	Van Antwerp et al.	6,478,736	B1	11/2002	Mault
6,253,804	B1	7/2001	Safabash	6,480,730	B2	11/2002	Darrow et al.
6,254,586	B1	7/2001	Mann et al.	6,482,158	B2	11/2002	Mault
6,256,643	B1	7/2001	Cork et al.	6,482,604	B2	11/2002	Kwon
6,259,587	B1	7/2001	Sheldon et al.	6,484,045	B1	11/2002	Holker et al.
6,259,937	B1	7/2001	Schulman et al.	6,484,046	B1	11/2002	Say et al.
6,260,022	B1	7/2001	Brown	6,485,138	B1	11/2002	Kubota et al.
6,266,645	B1	7/2001	Simpson	6,494,830	B1	12/2002	Wessel
6,267,724	B1	7/2001	Taylor	6,496,728	B2	12/2002	Li et al.
6,268,161	B1	7/2001	Han et al.	6,505,059	B1	1/2003	Kollias et al.
6,270,455	B1	8/2001	Brown	6,512,939	B1	1/2003	Colvin et al.
6,272,364	B1	8/2001	Kurnik	6,513,532	B2	2/2003	Mault et al.
6,275,717	B1	8/2001	Gross et al.	6,514,718	B2	2/2003	Heller et al.
6,280,416	B1	8/2001	Van Antwerp et al.	6,515,593	B1	2/2003	Stark et al.
6,280,587	B1	8/2001	Matsumoto	6,520,326	B2	2/2003	McIvor et al.
6,281,006	B1	8/2001	Heller et al.	6,529,755	B2	3/2003	Kurnik et al.
6,283,943	B1	9/2001	Dy et al.	6,529,772	B2	3/2003	Carlson et al.
6,284,126	B1	9/2001	Kurnik et al.	6,530,915	B1	3/2003	Eppstein et al.
6,284,478	B1	9/2001	Heller et al.	6,534,322	B1	3/2003	Sabbadini
6,293,925	B1	9/2001	Safabash et al.	6,534,323	B1	3/2003	Sabbadini
6,294,281	B1	9/2001	Heller	6,535,753	B1	3/2003	Raskas
6,295,463	B1	9/2001	Stenzler	6,537,243	B1	3/2003	Henning et al.
				6,540,675	B2	4/2003	Aceti et al.
				6,544,212	B2	4/2003	Galley et al.
				6,546,269	B1	4/2003	Kurnik
				6,549,796	B2	4/2003	Sohrab

(56)

References Cited

U.S. PATENT DOCUMENTS

6,551,276 B1	4/2003	Mann et al.	6,743,635 B2	6/2004	Neel et al.
6,551,494 B1	4/2003	Heller et al.	6,749,587 B2	6/2004	Flaherty
6,553,244 B2	4/2003	Lesho et al.	6,750,311 B1	6/2004	Van Antwerp et al.
6,554,798 B1	4/2003	Mann et al.	6,758,810 B2	7/2004	Lebel et al.
6,558,320 B1	5/2003	Causey, III et al.	6,766,183 B2	7/2004	Walsh et al.
6,558,321 B1	5/2003	Burd et al.	6,766,201 B2	7/2004	Von Arx et al.
6,558,351 B1	5/2003	Steil et al.	6,768,425 B2	7/2004	Flaherty et al.
6,560,471 B1	5/2003	Heller et al.	6,770,030 B1	8/2004	Schaupp et al.
6,561,978 B1	5/2003	Conn et al.	6,770,729 B2	8/2004	Van Antwerp et al.
6,562,001 B2	5/2003	Lebel et al.	6,771,995 B2	8/2004	Kurnik et al.
6,564,105 B2	5/2003	Starkweather et al.	6,773,563 B2	8/2004	Matsumoto
6,565,509 B1	5/2003	Say et al.	6,780,297 B2	8/2004	Matsumoto et al.
6,571,128 B2	5/2003	Lebel et al.	6,780,871 B2	8/2004	Glick et al.
6,571,200 B1	5/2003	Mault	6,784,274 B2	8/2004	Van Antwerp et al.
6,576,101 B1	6/2003	Heller et al.	6,790,178 B1	9/2004	Mault et al.
6,576,117 B1	6/2003	Iketaki et al.	6,794,195 B2	9/2004	Colvin, Jr.
6,577,899 B2	6/2003	Lebel et al.	6,800,451 B2	10/2004	Daniloff et al.
6,579,498 B1	6/2003	Eglise	6,804,544 B2	10/2004	Van Antwerp et al.
6,579,690 B1	6/2003	Bonnecaze et al.	6,809,507 B2	10/2004	Morgan et al.
6,584,335 B1	6/2003	Haar et al.	6,809,653 B1	10/2004	Mann et al.
6,585,644 B2	7/2003	Lebel et al.	6,810,290 B2	10/2004	Lebel et al.
6,587,705 B1	7/2003	Kim et al.	6,811,533 B2	11/2004	Lebel et al.
6,591,125 B1	7/2003	Buse et al.	6,811,534 B2	11/2004	Bowman, IV et al.
6,591,126 B2	7/2003	Roeper et al.	6,811,659 B2	11/2004	Vachon
6,594,514 B2	7/2003	Berner et al.	6,812,031 B1	11/2004	Carlsson
6,595,919 B2	7/2003	Berner et al.	6,813,519 B2	11/2004	Lebel et al.
6,595,929 B2	7/2003	Stivorac et al.	6,816,742 B2	11/2004	Kim et al.
6,602,678 B2	8/2003	Kwon et al.	6,835,553 B2	12/2004	Han et al.
6,602,909 B1	8/2003	Jarowski	RE38,681 E	1/2005	Kurnik et al.
6,605,200 B1	8/2003	Mao et al.	6,840,912 B2	1/2005	Kloepfer et al.
6,605,201 B1	8/2003	Mao et al.	6,844,023 B2	1/2005	Schulman et al.
6,607,509 B2	8/2003	Bobroff et al.	6,849,237 B2	2/2005	Housefield et al.
6,610,012 B2	8/2003	Mault	6,850,790 B2	2/2005	Berner et al.
6,612,306 B1	9/2003	Mault	6,852,500 B1	2/2005	Hoss et al.
6,615,078 B1	9/2003	Burson et al.	6,852,694 B2	2/2005	Van Antwerp et al.
6,618,603 B2	9/2003	Varalli et al.	6,853,854 B1	2/2005	Proniewicz et al.
6,620,106 B2	9/2003	Mault	6,856,928 B2	2/2005	Harmon
6,627,058 B1	9/2003	Chan	6,858,403 B2	2/2005	Han et al.
6,629,934 B2	10/2003	Mault et al.	6,862,465 B2	3/2005	Shults et al.
6,633,772 B2	10/2003	Ford et al.	6,862,466 B2	3/2005	Ackerman
6,635,014 B2	10/2003	Starkweather et al.	6,872,200 B2	3/2005	Mann et al.
6,641,533 B2	11/2003	Causey, III et al.	6,873,268 B2	3/2005	Lebel et al.
6,642,015 B2	11/2003	Vachon et al.	6,881,551 B2	4/2005	Heller et al.
6,645,142 B2	11/2003	Braig et al.	6,882,940 B2	4/2005	Potts et al.
6,648,821 B2	11/2003	Lebel et al.	6,885,883 B2	4/2005	Parris et al.
6,653,091 B1	11/2003	Dunn et al.	6,892,085 B2	5/2005	McIvor et al.
6,654,625 B1	11/2003	Say et al.	6,895,263 B2	5/2005	Shin et al.
6,659,948 B2	12/2003	Lebel et al.	6,899,683 B2	5/2005	Mault et al.
6,668,196 B1	12/2003	Villegas et al.	6,899,684 B2	5/2005	Mault et al.
6,671,554 B2	12/2003	Gibson et al.	6,902,905 B2	6/2005	Burson et al.
6,673,625 B2	1/2004	Satcher, Jr. et al.	6,904,301 B2	6/2005	Raskas
6,682,938 B1	1/2004	Satcher, Jr. et al.	6,907,127 B1	6/2005	Kravitz et al.
6,683,040 B2	1/2004	Bragulla et al.	6,915,147 B2	7/2005	Lebel et al.
6,687,522 B2	2/2004	Tamada	6,918,874 B1 *	7/2005	Hatch et al. 600/365
6,687,546 B2	2/2004	Lebel et al.	6,922,578 B2	7/2005	Eppstein et al.
6,689,056 B1	2/2004	Kilcoyne et al.	RE38,775 E	8/2005	Kurnik et al.
6,693,069 B2	2/2004	Korber et al.	6,923,764 B2	8/2005	Aceti et al.
6,694,158 B2	2/2004	Polak	6,923,936 B2	8/2005	Swanson et al.
6,694,191 B2	2/2004	Starkweather et al.	6,927,246 B2	8/2005	Noronha et al.
6,695,860 B1	2/2004	Ward et al.	6,931,327 B2	8/2005	Goode, Jr. et al.
6,702,857 B2	3/2004	Brauker et al.	6,936,006 B2	8/2005	Sabra
6,704,587 B1	3/2004	Kumar et al.	6,936,029 B2	8/2005	Mann et al.
6,711,423 B2	3/2004	Colvin, Jr.	6,940,590 B2	9/2005	Colvin, Jr. et al.
6,723,046 B2	4/2004	Lichtenstein et al.	6,941,163 B2	9/2005	Ford et al.
6,728,560 B2	4/2004	Kollias et al.	6,950,708 B2	9/2005	Bowman, IV et al.
6,731,976 B2	5/2004	Penn et al.	6,952,603 B2	10/2005	Gerber et al.
6,733,446 B2	5/2004	Lebel et al.	6,954,673 B2	10/2005	Von Arx et al.
6,734,162 B2	5/2004	Van Antwerp et al.	6,955,650 B2	10/2005	Mault et al.
6,736,777 B2	5/2004	Kim et al.	6,957,102 B2	10/2005	Silver et al.
6,737,401 B2	5/2004	Kim et al.	6,957,107 B2	10/2005	Rogers et al.
6,738,654 B2	5/2004	Sohrab	6,958,705 B2	10/2005	Lebel et al.
6,740,075 B2	5/2004	Lebel et al.	6,968,294 B2	11/2005	Gutta et al.
6,741,163 B1	5/2004	Roberts	6,968,375 B1	11/2005	Brown
6,741,876 B1	5/2004	Seccina et al.	6,974,437 B2	12/2005	Lebel et al.
6,741,877 B1	5/2004	Shults et al.	6,978,182 B2	12/2005	Mazar et al.
			6,979,326 B2	12/2005	Mann et al.
			6,990,366 B2	1/2006	Say et al.
			6,991,096 B2	1/2006	Gottlieb et al.
			6,997,907 B2	2/2006	Safabash et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,997,920	B2	2/2006	Mann et al.	7,711,402	B2	5/2010	Shults et al.
6,998,247	B2	2/2006	Monfre et al.	7,713,574	B2	5/2010	Brister et al.
6,999,810	B2	2/2006	Berner et al.	7,715,893	B2	5/2010	Kamath et al.
7,003,336	B2	2/2006	Holker et al.	2001/0011224	A1	8/2001	Brown
7,003,341	B2	2/2006	Say et al.	2001/0016310	A1	8/2001	Brown et al.
7,004,901	B2	2/2006	Fish	2001/0016682	A1	8/2001	Berner et al.
7,005,857	B2	2/2006	Stiene et al.	2001/0016683	A1	8/2001	Darrow et al.
7,011,630	B2	3/2006	Desai et al.	2001/0020124	A1	9/2001	Tamada
7,018,366	B2	3/2006	Easter	2001/0029340	A1	10/2001	Mault et al.
7,018,568	B2	3/2006	Tierney	2001/0032278	A1	10/2001	Brown et al.
7,022,072	B2	4/2006	Fox et al.	2001/0037060	A1	11/2001	Thompson et al.
7,024,236	B2	4/2006	Ford et al.	2001/0037069	A1	11/2001	Carlson et al.
7,024,245	B2	4/2006	Lebel et al.	2001/0039504	A1	11/2001	Linberg et al.
7,025,743	B2	4/2006	Mann et al.	2001/0041830	A1	11/2001	Varalli et al.
7,029,444	B2	4/2006	Shin et al.	2001/0044581	A1	11/2001	Mault
7,039,810	B1	5/2006	Nichols	2001/0044588	A1	11/2001	Mault
7,041,468	B2	5/2006	Drucker et al.	2001/0047125	A1	11/2001	Quy
7,049,277	B2	5/2006	Bagulla et al.	2001/0049096	A1	12/2001	Brown
7,052,472	B1	5/2006	Miller et al.	2001/0049470	A1	12/2001	Mault et al.
7,052,483	B2	5/2006	Wojcik	2001/0051768	A1	12/2001	Schulman et al.
7,056,302	B2	6/2006	Douglas	2002/0002326	A1	1/2002	Causey, III et al.
7,074,307	B2	7/2006	Simpson et al.	2002/0002328	A1	1/2002	Tamada
7,081,195	B2	7/2006	Simpson et al.	2002/0004640	A1	1/2002	Conn et al.
7,098,803	B2	8/2006	Mann et al.	2002/0010414	A1	1/2002	Coston et al.
7,108,778	B2	9/2006	Simpson et al.	2002/0016530	A1	2/2002	Brown
7,109,878	B2	9/2006	Mann et al.	2002/0019022	A1	2/2002	Dunn et al.
7,110,803	B2	9/2006	Shults et al.	2002/0019586	A1	2/2002	Teller et al.
7,113,821	B1	9/2006	Sun et al.	2002/0019748	A1	2/2002	Brown
7,133,710	B2	11/2006	Acosta et al.	2002/0026937	A1	3/2002	Mault
7,134,999	B2	11/2006	Brauker et al.	2002/0027164	A1	3/2002	Mault et al.
7,136,689	B2	11/2006	Shults et al.	2002/0028995	A1	3/2002	Mault
7,137,964	B2	11/2006	Flaherty	2002/0040208	A1	4/2002	Flaherty et al.
7,150,975	B2	12/2006	Tamada et al.	2002/0042090	A1	4/2002	Heller et al.
7,163,511	B2	1/2007	Conn et al.	2002/0042561	A1	4/2002	Schulman et al.
7,171,274	B2	1/2007	Starkweather et al.	2002/0047867	A1	4/2002	Mault et al.
7,183,068	B2	2/2007	Burson et al.	2002/0049482	A1	4/2002	Fabian et al.
7,183,102	B2	2/2007	Monfre et al.	2002/0053637	A1	5/2002	Conn et al.
7,187,528	B2	3/2007	Talbot et al.	2002/0062069	A1	5/2002	Mault
7,189,341	B2	3/2007	Li et al.	2002/0063060	A1	5/2002	Gascoyne et al.
7,190,988	B2	3/2007	Say et al.	2002/0068858	A1	6/2002	Braig et al.
7,192,450	B2	3/2007	Brauker et al.	2002/0072858	A1	6/2002	Cheng
7,198,606	B2	4/2007	Boecker et al.	2002/0077765	A1	6/2002	Mault
7,226,978	B2	6/2007	Tapsak et al.	2002/0077766	A1	6/2002	Mault
7,228,163	B2	6/2007	Ackerman	2002/0081559	A1	6/2002	Brown et al.
7,233,817	B2	6/2007	Yen	2002/0083461	A1	6/2002	Hutcheson et al.
7,261,691	B1	8/2007	Asomani	2002/0087056	A1	7/2002	Aceti et al.
7,267,665	B2	9/2007	Steil et al.	2002/0091312	A1	7/2002	Berner et al.
7,276,029	B2	10/2007	Goode, Jr. et al.	2002/0103425	A1	8/2002	Mault
7,295,867	B2	11/2007	Berner et al.	2002/0107433	A1	8/2002	Mault
7,310,544	B2	12/2007	Brister et al.	2002/0107476	A1	8/2002	Mann et al.
7,318,816	B2	1/2008	Bobroff et al.	2002/0109600	A1	8/2002	Mault et al.
7,354,420	B2	4/2008	Steil et al.	2002/0109621	A1	8/2002	Khair et al.
7,364,592	B2	4/2008	Carr-Brendel et al.	2002/0119711	A1	8/2002	Van Antwerp et al.
7,366,556	B2	4/2008	Brister et al.	2002/0124017	A1	9/2002	Mault
7,379,765	B2	5/2008	Petisce et al.	2002/0128594	A1	9/2002	Das et al.
7,402,153	B2	7/2008	Steil et al.	2002/0130042	A1	9/2002	Moerman et al.
7,424,318	B2	9/2008	Brister et al.	2002/0133378	A1	9/2002	Mault et al.
7,460,898	B2	12/2008	Brister et al.	2002/0161286	A1	10/2002	Gerber et al.
7,467,003	B2	12/2008	Brister et al.	2002/0161288	A1	10/2002	Shin et al.
7,471,972	B2	12/2008	Rhodes et al.	2002/0177764	A1	11/2002	Sohrab
7,494,465	B2	2/2009	Brister et al.	2002/0198513	A1	12/2002	Lebel et al.
7,497,827	B2	3/2009	Brister et al.	2003/0023182	A1	1/2003	Mault et al.
7,519,408	B2	4/2009	Rasdal et al.	2003/0023317	A1	1/2003	Brauker et al.
7,583,990	B2	9/2009	Goode, Jr. et al.	2003/0028089	A1	2/2003	Galley et al.
7,591,801	B2	9/2009	Brauker et al.	2003/0028120	A1	2/2003	Mault et al.
7,599,726	B2	10/2009	Goode, Jr. et al.	2003/0032077	A1	2/2003	Itoh et al.
7,613,491	B2	11/2009	Boock et al.	2003/0032867	A1	2/2003	Crothall et al.
7,615,007	B2	11/2009	Shults et al.	2003/0032868	A1	2/2003	Graskov et al.
7,618,369	B2	11/2009	Hayter et al.	2003/0032874	A1	2/2003	Rhodes et al.
7,632,228	B2	12/2009	Brauker et al.	2003/0040683	A1	2/2003	Rule et al.
7,637,868	B2	12/2009	Saint et al.	2003/0042137	A1	3/2003	Mao et al.
7,640,048	B2	12/2009	Dobbles et al.	2003/0050537	A1	3/2003	Wessel
7,651,596	B2	1/2010	Petisce et al.	2003/0050546	A1	3/2003	Desai et al.
7,654,956	B2	2/2010	Brister et al.	2003/0065257	A1	4/2003	Mault et al.
7,657,297	B2	2/2010	Simpson et al.	2003/0065273	A1	4/2003	Mault et al.
				2003/0065274	A1	4/2003	Mault et al.
				2003/0065275	A1	4/2003	Mault et al.
				2003/0065308	A1	4/2003	Lebel et al.
				2003/0100040	A1	5/2003	Bonnecaze et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2003/0100821	A1	5/2003	Heller et al.	2004/0249253	A1	12/2004	Racchini et al.
2003/0105407	A1	6/2003	Pearce et al.	2004/0249254	A1	12/2004	Racchini et al.
2003/0108976	A1	6/2003	Braig et al.	2004/0249999	A1	12/2004	Connolly et al.
2003/0130616	A1	7/2003	Steil et al.	2004/0253736	A1	12/2004	Stout et al.
2003/0134347	A1	7/2003	Heller et al.	2004/0254429	A1	12/2004	Yang
2003/0135100	A1	7/2003	Kim et al.	2004/0254433	A1	12/2004	Bandis et al.
2003/0135333	A1	7/2003	Aceti et al.	2004/0254434	A1	12/2004	Goodnow et al.
2003/0153820	A1	8/2003	Berner et al.	2004/0260363	A1	12/2004	Von Arx et al.
2003/0153821	A1	8/2003	Berner et al.	2004/0263354	A1	12/2004	Mann et al.
2003/0158472	A1	8/2003	Sohrab	2005/0003470	A1	1/2005	Nelson et al.
2003/0158707	A1	8/2003	Doi	2005/0010087	A1	1/2005	Banet et al.
2003/0168338	A1	9/2003	Gao et al.	2005/0010269	A1	1/2005	Lebel et al.
2003/0175806	A1	9/2003	Rule et al.	2005/0027177	A1	2/2005	Shin et al.
2003/0176183	A1	9/2003	Drucker et al.	2005/0027179	A1	2/2005	Berner et al.
2003/0176933	A1	9/2003	Lebel et al.	2005/0027180	A1	2/2005	Goode, Jr. et al.
2003/0181851	A1	9/2003	Mann et al.	2005/0027181	A1	2/2005	Goode, Jr. et al.
2003/0181852	A1	9/2003	Mann et al.	2005/0027462	A1	2/2005	Goode, Jr. et al.
2003/0187338	A1	10/2003	Say et al.	2005/0027463	A1	2/2005	Goode, Jr. et al.
2003/0187525	A1	10/2003	Mann et al.	2005/0031689	A1	2/2005	Shults et al.
2003/0191376	A1	10/2003	Samuels et al.	2005/0033132	A1	2/2005	Shults et al.
2003/0191431	A1	10/2003	Mann et al.	2005/0038680	A1	2/2005	McMahon
2003/0195403	A1	10/2003	Berner et al.	2005/0043598	A1	2/2005	Goode, Jr. et al.
2003/0195462	A1	10/2003	Mann et al.	2005/0043894	A1	2/2005	Fernandez
2003/0199791	A1	10/2003	Boecker et al.	2005/0049473	A1	3/2005	Desai et al.
2003/0199903	A1	10/2003	Boecker et al.	2005/0051427	A1	3/2005	Brauker et al.
2003/0208110	A1	11/2003	Mault et al.	2005/0051440	A1	3/2005	Simpson et al.
2003/0208113	A1	11/2003	Mault et al.	2005/0054909	A1	3/2005	Petisce et al.
2003/0208133	A1	11/2003	Mault	2005/0056552	A1	3/2005	Simpson et al.
2003/0208409	A1	11/2003	Mault	2005/0090607	A1	4/2005	Tapsak et al.
2003/0212346	A1	11/2003	Yuzhakov et al.	2005/0112169	A1	5/2005	Brauker et al.
2003/0212379	A1	11/2003	Bylund et al.	2005/0113657	A1	5/2005	Alarcon et al.
2003/0217966	A1	11/2003	Tapsak et al.	2005/0113658	A1	5/2005	Jacobson et al.
2003/0224729	A1 *	12/2003	Arnold 455/59	2005/0118726	A1	6/2005	Schultz et al.
2003/0226695	A1	12/2003	Mault	2005/0121322	A1	6/2005	Say et al.
2003/0229514	A2	12/2003	Brown	2005/0124873	A1	6/2005	Shults et al.
2003/0232370	A1	12/2003	Trifiro	2005/0131346	A1	6/2005	Douglas
2003/0235817	A1	12/2003	Bartkowiak et al.	2005/0137471	A1	6/2005	Haar et al.
2004/0010207	A1	1/2004	Flaherty et al.	2005/0143635	A1	6/2005	Kamath et al.
2004/0011671	A1	1/2004	Shults et al.	2005/0143636	A1	6/2005	Zhang et al.
2004/0018486	A1	1/2004	Dunn et al.	2005/0143675	A1	6/2005	Neel et al.
2004/0039256	A1	2/2004	Kawatahara et al.	2005/0148003	A1	7/2005	Kieth et al.
2004/0040840	A1	3/2004	Mao et al.	2005/0154271	A1	7/2005	Rasdal et al.
2004/0045879	A1	3/2004	Shults et al.	2005/0161346	A1	7/2005	Simpson et al.
2004/0054263	A1	3/2004	Moerman et al.	2005/0171503	A1	8/2005	Van Den Berghe et al.
2004/0059201	A1	3/2004	Ginsberg	2005/0171513	A1	8/2005	Mann et al.
2004/0069164	A1	4/2004	Nakamura et al.	2005/0173245	A1	8/2005	Feldman et al.
2004/0072357	A1	4/2004	Stiene et al.	2005/0176136	A1	8/2005	Burd et al.
2004/0073095	A1	4/2004	Causey, III et al.	2005/0177036	A1	8/2005	Shults et al.
2004/0096959	A1	5/2004	Stiene et al.	2005/0181012	A1	8/2005	Saint et al.
2004/0106858	A1	6/2004	Say et al.	2005/0182306	A1	8/2005	Sloan et al.
2004/0106859	A1	6/2004	Say et al.	2005/0182451	A1	8/2005	Griffin et al.
2004/0108226	A1	6/2004	Polychronakos et al.	2005/0187720	A1	8/2005	Goode, Jr. et al.
2004/0122353	A1	6/2004	Shahmirian et al.	2005/0192557	A1	9/2005	Brauker et al.
2004/0122489	A1	6/2004	Mazar et al.	2005/0195930	A1	9/2005	Spital et al.
2004/0133164	A1	7/2004	Funderburk et al.	2005/0199494	A1	9/2005	Say et al.
2004/0138588	A1	7/2004	Saikley et al.	2005/0203360	A1	9/2005	Brauker et al.
2004/0153585	A1	8/2004	Kawatahara et al.	2005/0203707	A1	9/2005	Tsutsui et al.
2004/0162473	A1	8/2004	Sohrab	2005/0214892	A1	9/2005	Kovatchev et al.
2004/0164961	A1	8/2004	Bal et al.	2005/0215871	A1	9/2005	Feldman et al.
2004/0167383	A1	8/2004	Kim et al.	2005/0215872	A1	9/2005	Berner et al.
2004/0167801	A1	8/2004	Say et al.	2005/0239154	A1	10/2005	Feldman et al.
2004/0171921	A1	9/2004	Say et al.	2005/0239156	A1	10/2005	Drucker et al.
2004/0172284	A1	9/2004	Sullivan et al.	2005/0245795	A1	11/2005	Goode, Jr. et al.
2004/0176913	A1	9/2004	Kawatahara et al.	2005/0245799	A1	11/2005	Brauker et al.
2004/0186362	A1	9/2004	Brauker et al.	2005/0251083	A1	11/2005	Carr-Brendel et al.
2004/0186365	A1	9/2004	Jin et al.	2005/0261660	A1	11/2005	Choi
2004/0193025	A1	9/2004	Steil et al.	2005/0267780	A1	12/2005	Ray et al.
2004/0193090	A1	9/2004	Lebel et al.	2005/0271546	A1	12/2005	Gerber et al.
2004/0199059	A1	10/2004	Brauker et al.	2005/0271547	A1	12/2005	Gerber et al.
2004/0202576	A1	10/2004	Aceti et al.	2005/0272640	A1	12/2005	Doyle, III et al.
2004/0219664	A1	11/2004	Heller et al.	2005/0272985	A1	12/2005	Kotulla et al.
2004/0225338	A1	11/2004	Lebel et al.	2005/0277164	A1	12/2005	Drucker et al.
2004/0236200	A1	11/2004	Say et al.	2005/0287620	A1	12/2005	Heller et al.
2004/0248204	A1	12/2004	Moerman	2006/0001538	A1	1/2006	Kraft et al.
2004/0249250	A1	12/2004	McGee et al.	2006/0001550	A1	1/2006	Mann et al.
				2006/0001551	A1	1/2006	Kraft et al.
				2006/0003398	A1	1/2006	Heller et al.
				2006/0004271	A1	1/2006	Peyser et al.
				2006/0007017	A1	1/2006	Mann et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2006/0015020	A1	1/2006	Neale et al.	2007/0203966	A1	8/2007	Brauker et al.
2006/0015024	A1	1/2006	Brister et al.	2007/0208244	A1	9/2007	Brauker et al.
2006/0016700	A1	1/2006	Brister et al.	2007/0208245	A1	9/2007	Brauker et al.
2006/0019327	A1	1/2006	Brister et al.	2007/0208246	A1	9/2007	Brauker et al.
2006/0020186	A1	1/2006	Brister et al.	2007/0208247	A1	9/2007	Say et al.
2006/0020187	A1	1/2006	Brister et al.	2007/0213610	A1	9/2007	Say et al.
2006/0020188	A1	1/2006	Kamath et al.	2007/0213611	A1	9/2007	Simpson et al.
2006/0020189	A1	1/2006	Brister et al.	2007/0215491	A1	9/2007	Heller et al.
2006/0020190	A1	1/2006	Kamath et al.	2007/0218097	A1	9/2007	Heller et al.
2006/0020191	A1	1/2006	Brister et al.	2007/0235331	A1	10/2007	Simpson et al.
2006/0020192	A1	1/2006	Brister et al.	2007/0244380	A1	10/2007	Say et al.
2006/0025663	A1	2/2006	Talbot et al.	2007/0249919	A1	10/2007	Say et al.
2006/0031094	A1	2/2006	Cohen et al.	2007/0249920	A1	10/2007	Say et al.
2006/0036139	A1	2/2006	Brister et al.	2007/0249922	A1	10/2007	Peyser et al.
2006/0036140	A1	2/2006	Brister et al.	2008/0021436	A1	1/2008	Wolpert et al.
2006/0036141	A1	2/2006	Kamath et al.	2008/0021666	A1	1/2008	Goode, Jr. et al.
2006/0036142	A1	2/2006	Brister et al.	2008/0033254	A1	2/2008	Kamath et al.
2006/0036143	A1	2/2006	Brister et al.	2008/0033271	A1	2/2008	Say et al.
2006/0036144	A1	2/2006	Brister et al.	2008/0045824	A1	2/2008	Tapsak et al.
2006/0036145	A1	2/2006	Brister et al.	2008/0071156	A1	3/2008	Brister et al.
2006/0036187	A1	2/2006	Vos et al.	2008/0076997	A1	3/2008	Peyser et al.
2006/0040402	A1	2/2006	Brauker et al.	2008/0083617	A1	4/2008	Simpson et al.
2006/0052679	A1	3/2006	Kotulla et al.	2008/0086039	A1	4/2008	Heller et al.
2006/0058602	A1	3/2006	Kwiatkowski et al.	2008/0086040	A1	4/2008	Heller et al.
2006/0063218	A1	3/2006	Bartkowiak et al.	2008/0086041	A1	4/2008	Heller et al.
2006/0068208	A1	3/2006	Tapsak et al.	2008/0086042	A1	4/2008	Brister et al.
2006/0074564	A1	4/2006	Bartkowiak et al.	2008/0086043	A1	4/2008	Heller et al.
2006/0086624	A1	4/2006	Tapsak et al.	2008/0086044	A1	4/2008	Brister et al.
2006/0155180	A1	7/2006	Brister et al.	2008/0086273	A1	4/2008	Shults et al.
2006/0173444	A1	8/2006	Choy et al.	2008/0091094	A1	4/2008	Heller et al.
2006/0183984	A1	8/2006	Dobbles et al.	2008/0091095	A1	4/2008	Heller et al.
2006/0183985	A1	8/2006	Brister et al.	2008/0091096	A1	4/2008	Say et al.
2006/0189856	A1	8/2006	Petisce et al.	2008/0108942	A1	5/2008	Brister et al.
2006/0189863	A1	8/2006	Peyser et al.	2008/0167543	A1	7/2008	Say et al.
2006/0195029	A1	8/2006	Shults et al.	2008/0183061	A1	7/2008	Goode, Jr. et al.
2006/0198864	A1	9/2006	Shults et al.	2008/0183399	A1	7/2008	Goode, Jr. et al.
2006/0200019	A1	9/2006	Petisce et al.	2008/0188731	A1	8/2008	Brister et al.
2006/0200020	A1	9/2006	Brister et al.	2008/0189051	A1	8/2008	Goode, Jr. et al.
2006/0200022	A1	9/2006	Brauker et al.	2008/0194935	A1	8/2008	Brister et al.
2006/0211921	A1	9/2006	Brauker et al.	2008/0194936	A1	8/2008	Goode, Jr. et al.
2006/0222566	A1	10/2006	Brauker et al.	2008/0194937	A1	8/2008	Goode, Jr. et al.
2006/0224108	A1	10/2006	Brauker et al.	2008/0194938	A1	8/2008	Brister et al.
2006/0235285	A1	10/2006	Brister et al.	2008/0195232	A1	8/2008	Carr-Brendel et al.
2006/0247985	A1	11/2006	Liamos et al.	2008/0195967	A1	8/2008	Goode, Jr. et al.
2006/0258929	A1	11/2006	Goode, Jr. et al.	2008/0197024	A1	8/2008	Simpson et al.
2006/0270922	A1	11/2006	Brauker et al.	2008/0200788	A1	8/2008	Brister et al.
2006/0270923	A1	11/2006	Brauker et al.	2008/0200789	A1	8/2008	Brister et al.
2007/0016381	A1	1/2007	Kamath et al.	2008/0200791	A1	8/2008	Simpson et al.
2007/0027381	A1	2/2007	Stafford	2008/0208025	A1	8/2008	Shults et al.
2007/0027384	A1	2/2007	Brister et al.	2008/0214914	A1	9/2008	Say et al.
2007/0027385	A1	2/2007	Brister et al.	2008/0214915	A1	9/2008	Brister et al.
2007/0032706	A1	2/2007	Kamath et al.	2008/0214918	A1	9/2008	Brister et al.
2007/0032717	A1	2/2007	Brister et al.	2008/0228051	A1	9/2008	Shults et al.
2007/0032718	A1	2/2007	Shults et al.	2008/0228054	A1	9/2008	Shults et al.
2007/0045902	A1	3/2007	Brauker et al.	2008/0242961	A1	10/2008	Brister et al.
2007/0060814	A1	3/2007	Stafford	2008/0262329	A1	10/2008	Say et al.
2007/0066873	A1	3/2007	Kamath et al.	2008/0262469	A1	10/2008	Brister et al.
2007/0078320	A1	4/2007	Stafford	2008/0269672	A1	10/2008	Say et al.
2007/0078321	A1	4/2007	Mazza et al.	2008/0275313	A1	11/2008	Brister et al.
2007/0093704	A1	4/2007	Brister et al.	2008/0287764	A1	11/2008	Rasdal et al.
2007/0106135	A1	5/2007	Sloan et al.	2008/0287765	A1	11/2008	Rasdal et al.
2007/0149873	A1	6/2007	Say et al.	2008/0287766	A1	11/2008	Rasdal et al.
2007/0149874	A1	6/2007	Say et al.	2008/0296155	A1	12/2008	Shults et al.
2007/0151869	A1	7/2007	Heller et al.	2008/0306368	A1	12/2008	Goode, Jr. et al.
2007/0161879	A1	7/2007	Say et al.	2008/0306434	A1	12/2008	Dobbles et al.
2007/0161880	A1	7/2007	Say et al.	2008/0306435	A1	12/2008	Kamath et al.
2007/0163880	A1	7/2007	Woo et al.	2008/0306444	A1	12/2008	Brister et al.
2007/0179370	A1	8/2007	Say et al.	2008/0319292	A1	12/2008	Say et al.
2007/0179372	A1	8/2007	Say et al.	2009/0012379	A1	1/2009	Goode, Jr. et al.
2007/0191699	A1	8/2007	Say et al.	2009/0018424	A1	1/2009	Kamath et al.
2007/0191700	A1	8/2007	Say et al.	2009/0030294	A1	1/2009	Petisce et al.
2007/0197889	A1	8/2007	Brister et al.	2009/0036758	A1	2/2009	Brauker et al.
2007/0203408	A1	8/2007	Say et al.	2009/0036763	A1	2/2009	Brauker et al.
2007/0203410	A1	8/2007	Say et al.	2009/0043181	A1	2/2009	Brauker et al.
2007/0203411	A1	8/2007	Say et al.	2009/0043182	A1	2/2009	Brauker et al.
				2009/0043525	A1	2/2009	Brauker et al.
				2009/0043541	A1	2/2009	Brauker et al.
				2009/0043542	A1	2/2009	Brauker et al.
				2009/0045055	A1	2/2009	Rhodes et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2009/0062633 A1 3/2009 Brauker et al.
 2009/0062634 A1 3/2009 Say et al.
 2009/0062635 A1 3/2009 Brauker et al.
 2009/0069655 A1 3/2009 Say et al.
 2009/0069656 A1 3/2009 Say et al.
 2009/0069657 A1 3/2009 Say et al.
 2009/0069658 A1 3/2009 Say et al.
 2009/0076356 A1 3/2009 Simpson et al.
 2009/0076360 A1 3/2009 Brister et al.
 2009/0076361 A1 3/2009 Kamath et al.
 2009/0089999 A1 4/2009 Say et al.
 2009/0093696 A1 4/2009 Say et al.
 2009/0099432 A1 4/2009 Say et al.
 2009/0099435 A1 4/2009 Say et al.
 2009/0099436 A1 4/2009 Brister et al.
 2009/0124877 A1 5/2009 Goode, Jr. et al.
 2009/0124878 A1 5/2009 Goode, Jr. et al.
 2009/0124879 A1 5/2009 Brister et al.
 2009/0124964 A1 5/2009 Leach et al.
 2009/0131768 A1 5/2009 Simpson et al.
 2009/0131769 A1 5/2009 Leach et al.
 2009/0131776 A1 5/2009 Simpson et al.
 2009/0131777 A1 5/2009 Simpson et al.
 2009/0137886 A1 5/2009 Shariati et al.
 2009/0137887 A1 5/2009 Shariati et al.
 2009/0143659 A1 6/2009 Li et al.
 2009/0143660 A1 6/2009 Brister et al.
 2009/0156919 A1 6/2009 Brister et al.
 2009/0156924 A1 6/2009 Shariati et al.
 2009/0163781 A1 6/2009 Say et al.
 2009/0163788 A1 6/2009 Say et al.
 2009/0163789 A1 6/2009 Say et al.
 2009/0163790 A1 6/2009 Brister et al.
 2009/0163791 A1 6/2009 Brister et al.
 2009/0171179 A1 7/2009 Say et al.
 2009/0173628 A1 7/2009 Say et al.
 2009/0177054 A1 7/2009 Say et al.
 2009/0177055 A1 7/2009 Say et al.
 2009/0177056 A1 7/2009 Say et al.
 2009/0177057 A1 7/2009 Say et al.
 2009/0177058 A1 7/2009 Say et al.
 2009/0177059 A1 7/2009 Say et al.
 2009/0177060 A1 7/2009 Say et al.
 2009/0177061 A1 7/2009 Say et al.
 2009/0177062 A1 7/2009 Say et al.
 2009/0177063 A1 7/2009 Say et al.
 2009/0177064 A1 7/2009 Say et al.
 2009/0177065 A1 7/2009 Say et al.
 2009/0177066 A1 7/2009 Say et al.
 2009/0178459 A1 7/2009 Li et al.
 2009/0182212 A1 7/2009 Say et al.
 2009/0182213 A1 7/2009 Say et al.
 2009/0182214 A1 7/2009 Say et al.
 2009/0182215 A1 7/2009 Say et al.
 2009/0182217 A1 7/2009 Li et al.
 2009/0187088 A1 7/2009 Say et al.
 2009/0187089 A1 7/2009 Say et al.
 2009/0187090 A1 7/2009 Say et al.
 2009/0187091 A1 7/2009 Say et al.
 2009/0187092 A1 7/2009 Say et al.
 2009/0187093 A1 7/2009 Say et al.
 2009/0187094 A1 7/2009 Say et al.
 2009/0187095 A1 7/2009 Say et al.
 2009/0192366 A1 7/2009 Mensinger et al.
 2009/0192368 A1 7/2009 Say et al.
 2009/0192369 A1 7/2009 Say et al.
 2009/0192370 A1 7/2009 Say et al.
 2009/0192371 A1 7/2009 Say et al.
 2009/0192372 A1 7/2009 Say et al.
 2009/0192373 A1 7/2009 Say et al.
 2009/0192374 A1 7/2009 Say et al.
 2009/0192375 A1 7/2009 Say et al.
 2009/0192376 A1 7/2009 Say et al.
 2009/0192377 A1 7/2009 Say et al.
 2009/0192378 A1 7/2009 Say et al.

2009/0192379 A1 7/2009 Say et al.
 2009/0192380 A1 7/2009 Shariati et al.
 2009/0192722 A1 7/2009 Shariati et al.
 2009/0192724 A1 7/2009 Brauker et al.
 2009/0192745 A1 7/2009 Kamath et al.
 2009/0192751 A1 7/2009 Kamath et al.
 2009/0198115 A1 8/2009 Say et al.
 2009/0198116 A1 8/2009 Say et al.
 2009/0198175 A1 8/2009 Say et al.
 2009/0203978 A1 8/2009 Say et al.
 2009/0203981 A1 8/2009 Brauker et al.
 2009/0204341 A1 8/2009 Brauker et al.
 2009/0209838 A1 8/2009 Say et al.
 2009/0216101 A1 8/2009 Say et al.
 2009/0216103 A1 8/2009 Brister et al.
 2009/0227940 A1 9/2009 Say et al.
 2009/0227941 A1 9/2009 Say et al.
 2009/0228214 A1 9/2009 Say et al.
 2009/0240120 A1 9/2009 Mensinger et al.
 2009/0240128 A1 9/2009 Mensinger et al.
 2009/0240193 A1 9/2009 Mensinger et al.
 2009/0242399 A1 10/2009 Kamath et al.
 2009/0242425 A1 10/2009 Kamath et al.
 2009/0247855 A1 10/2009 Boock et al.
 2009/0247856 A1 10/2009 Boock et al.
 2009/0287073 A1 11/2009 Boock et al.
 2009/0287074 A1 11/2009 Shults et al.
 2009/0299155 A1 12/2009 Yang et al.
 2009/0299156 A1 12/2009 Simpson et al.
 2009/0299162 A1 12/2009 Brauker et al.
 2009/0299276 A1 12/2009 Brauker et al.
 2010/0010324 A1 1/2010 Brauker et al.
 2010/0010331 A1 1/2010 Brauker et al.
 2010/0010332 A1 1/2010 Brauker et al.
 2010/0016687 A1 1/2010 Brauker et al.
 2010/0016698 A1 1/2010 Rasdal et al.
 2010/0022855 A1 1/2010 Brauker et al.
 2010/0030038 A1 2/2010 Brauker et al.
 2010/0030053 A1 2/2010 Goode, Jr. et al.
 2010/0030484 A1 2/2010 Brauker et al.
 2010/0030485 A1 2/2010 Brauker et al.
 2010/0036215 A1 2/2010 Goode, Jr. et al.
 2010/0036216 A1 2/2010 Goode, Jr. et al.
 2010/0036222 A1 2/2010 Goode, Jr. et al.
 2010/0036223 A1 2/2010 Goode, Jr. et al.
 2010/0036225 A1 2/2010 Goode, Jr. et al.
 2010/0041971 A1 2/2010 Goode, Jr. et al.
 2010/0045465 A1 2/2010 Brauker et al.
 2010/0049024 A1 2/2010 Saint et al.
 2010/0063373 A1 3/2010 Kamath et al.
 2010/0076283 A1 3/2010 Simpson et al.
 2010/0081908 A1 4/2010 Dobbles et al.
 2010/0081910 A1 4/2010 Brister et al.
 2010/0087724 A1 4/2010 Brauker et al.
 2010/0096259 A1 4/2010 Zhang et al.
 2010/0099970 A1 4/2010 Shults et al.
 2010/0099971 A1 4/2010 Shults et al.
 2010/0119693 A1 5/2010 Tapsak et al.
 2010/0121169 A1 5/2010 Petisce et al.

FOREIGN PATENT DOCUMENTS

DE 3934299 10/1990
 DE 4234553 1/1995
 DE 4401400 7/1995
 EP 0010375 4/1980
 EP 0026995 4/1981
 EP 0048090 3/1982
 EP 0078636 5/1983
 EP 0080304 6/1983
 EP 0096228 12/1983
 EP 0096288 12/1983
 EP 0098592 1/1984
 EP 0125139 11/1984
 EP 0127958 12/1984
 EP 0136362 4/1985
 EP 0170375 2/1986
 EP 0177743 4/1986
 EP 0184909 6/1986

(56)

References Cited

FOREIGN PATENT DOCUMENTS

EP	0206218	12/1986	JP	9-285459	11/1997
EP	0230472	8/1987	JP	10-170471	6/1998
EP	0241309	10/1987	JP	2000-000231	1/2000
EP	0245073	11/1987	JP	2000-116628	4/2000
EP	0255291	2/1988	SU	1281988	1/1987
EP	0278647	8/1988	WO	WO-85/05119	11/1985
EP	0320109	6/1989	WO	WO-86/00513	1/1986
EP	0353328	2/1990	WO	WO-87/00513	1/1987
EP	0359831	3/1990	WO	WO-87/06040	10/1987
EP	0368209	5/1990	WO	WO-89/02246	3/1989
EP	0368290	5/1990	WO	WO-89/05119	6/1989
EP	0390390	10/1990	WO	WO-89/08713	9/1989
EP	0396788	11/1990	WO	WO-90/00367	1/1990
EP	0400918	12/1990	WO	WO-90/05300	5/1990
EP	0453283	10/1991	WO	WO-90/05910	5/1990
EP	0470290	2/1992	WO	WO-91/01680	2/1991
EP	0504835	9/1992	WO	WO-91/04704	4/1991
EP	0286118	1/1995	WO	WO-91/15993	10/1991
EP	0653718	5/1995	WO	WO-92/13271	8/1992
EP	0800082	10/1997	WO	WO-94/20602	9/1994
EP	0880936	12/1998	WO	WO-94/27140	11/1994
EP	0970655	1/2000	WO	WO-95/06240	3/1995
EP	1034734	9/2000	WO	WO-96/07908	3/1996
EP	1048264	11/2000	WO	WO-96/14026	5/1996
GB	1394171	5/1975	WO	WO-96/25089	8/1996
GB	1579690	11/1980	WO	WO-96/30431	10/1996
GB	1599241	9/1981	WO	WO-96/35370	11/1996
GB	2073891	10/1981	WO	WO-97/19344	5/1997
GB	2154003	8/1985	WO	WO-97/20207	6/1997
GB	2194892	3/1988	WO	WO-97/41421	11/1997
GB	2204408	11/1988	WO	WO-97/42882	11/1997
GB	2225637	6/1990	WO	WO-97/42883	11/1997
GB	2254436	10/1992	WO	WO-97/42886	11/1997
JP	54-041191	4/1979	WO	WO-97/42888	11/1997
JP	55-010581	1/1980	WO	WO-97/43962	11/1997
JP	55-010583	1/1980	WO	WO-97/46868	12/1997
JP	55-010584	1/1980	WO	WO-98/09167	3/1998
JP	55-012406	1/1980	WO	WO-98/24358	6/1998
JP	56-163447	12/1981	WO	WO-98/52045	11/1998
JP	57-070448	4/1982	WO	WO-98/52293	11/1998
JP	60-173457	9/1985	WO	WO-98/56293	12/1998
JP	60-173458	9/1985	WO	WO-99/05966	2/1999
JP	60-173459	9/1985	WO	WO-99/13574	3/1999
JP	60-210243	10/1985	WO	WO-99/32883	7/1999
JP	61-090050	5/1986	WO	WO-99/48419	9/1999
JP	62-085855	4/1987	WO	WO-99/58051	11/1999
JP	62-114747	5/1987	WO	WO-99/58973	11/1999
JP	63-058149	3/1988	WO	WO-00/18294	4/2000
JP	63-128252	5/1988	WO	WO-00/19887	4/2000
JP	63-139246	6/1988	WO	WO-00/20626	4/2000
JP	63-294799	12/1988	WO	WO-00/32098	6/2000
JP	63-317757	12/1988	WO	WO-00/49940	8/2000
JP	63-317758	12/1988	WO	WO-00/59370	10/2000
JP	1-114746	5/1989	WO	WO-00/59373	10/2000
JP	1-114747	5/1989	WO	WO-00/62665	10/2000
JP	1-124060	5/1989	WO	WO-00/74753	12/2000
JP	1-134244	5/1989	WO	WO-00/78210	12/2000
JP	1-156658	6/1989	WO	WO-00/78992	12/2000
JP	2-062958	3/1990	WO	WO-01/12158	2/2001
JP	2-120655	5/1990	WO	WO-01/33216	5/2001
JP	2-287145	11/1990	WO	WO-01/52727	7/2001
JP	2-310457	12/1990	WO	WO-01/52935	7/2001
JP	3-026956	2/1991	WO	WO-01/54753	8/2001
JP	3-028752	2/1991	WO	WO-01/57238	8/2001
JP	3-202764	9/1991	WO	WO-01/57239	8/2001
JP	5-072171	3/1993	WO	WO-01/58348	8/2001
JP	5-196595	8/1993	WO	WO-01/67009	9/2001
JP	6-190050	7/1994	WO	WO-01/68901	9/2001
JP	7-055757	3/1995	WO	WO-01/69222	9/2001
JP	7-072585	3/1995	WO	WO-01/88524	11/2001
JP	8-154903	6/1996	WO	WO-01/88534	11/2001
JP	8-285814	11/1996	WO	WO-02/16905	2/2002
JP	8-285815	11/1996	WO	WO-02/17210	2/2002
JP	9-021778	1/1997	WO	WO-02/058537	8/2002
JP	9-101280	4/1997	WO	WO-02/078512	10/2002
			WO	WO-03/072269	9/2003
			WO	WO-03/076893	9/2003
			WO	WO-03/082091	10/2003
			WO	WO-2004/061420	7/2004

(56)

References Cited

FOREIGN PATENT DOCUMENTS

WO	WO-2005/089103	9/2005
WO	WO-2006/119084	11/2006
WO	WO-2007/002189	1/2007
WO	WO-2007/016399	2/2007
WO	WO-2007/027381	3/2007
WO	WO-2007/027788	3/2007
WO	WO-2007/051139	5/2007
WO	WO-2007/053832	5/2007
WO	WO-2007/056638	5/2007

OTHER PUBLICATIONS

Albery, W. J., et al., "Amperometric Enzyme Electrodes Part II: Conducting Salts as Electrode Materials for the Oxidation of Glucose Oxidase", *Journal of Electro Analytical Chemistry*, vol. 194, 1985, pp. 223-235.

Albery, W. J., et al., "Amperometric Enzyme Electrodes", *Philosophical Transactions of the Royal Society of London*, vol. 316, 1987, pp. 107-119.

Alcock, S. J., et al., "Continuous Analyte Monitoring to Aid Clinical Practice", *IEEE Engineering in Medicine and Biology Magazine*, 1994, pp. 319-325.

Anderson, L. B., et al., "Thin-Layer Electrochemistry: Steady-State Methods of Studying Rate Processes", *Journal of Electroanalytical Chemistry*, vol. 10, 1965, pp. 295-305.

Armour, J. C., et al., "Application of Chronic Intravascular Blood Glucose Sensor in Dogs", *Diabetes*, vol. 39, 1990, pp. 1519-1526.

Bartlett, P. N., et al., "Covalent Binding of Electron Relays to Glucose Oxidase", *Journal of the Chemical Society, Chemical Communications*, 1987, pp. 1603-1604.

Bartlett, P. N., et al., "Modification of Glucose Oxidase by Tetrathiafulvalene", *Journal of the Chemical Society, Chemical Communications*, 1990, pp. 1135-1136.

Bartlett, P. N., et al., "Strategies for the Development of Amperometric Enzyme Electrodes", *Biosensors*, vol. 3, 1987/88, pp. 359-379.

Bennion, N., et al., "Alternate Site Glucose Testing: A Crossover Design", *Diabetes Technology & Therapeutics*, vol. 4, No. 1, 2002, pp. 25-33.

Bindra, D. S., et al., "Design and in Vitro Studies of a Needle-Type Glucose Sensor for Subcutaneous Monitoring", *Analytical Chemistry*, vol. 63, No. 17, 1991, pp. 1692-1696.

Blank, T. B., et al., "Clinical Results From a Non-Invasive Blood Glucose Monitor", *Optical Diagnostics and Sensing of Biological Fluids and Glucose and Cholesterol Monitoring II, Proceedings of SPIE*, vol. 4624, 2002, pp. 1-10.

Bobbioni-Harsch, E., et al., "Lifespan of Subcutaneous Glucose Sensors and Their Performances During Dynamic Glycaemia Changes in Rats", *Journal of Biomedical Engineering*, vol. 15, 1993, pp. 457-463.

Boedeker Plastics, Inc., "Polyethylene Specifications", *Web Page of Boedeker.com*, 2007, pp. 1-3.

Brandt, J., et al., "Covalent Attachment of Proteins to Polysaccharide Carriers by Means of Benzoquinone", *Biochimica et Biophysica Acta*, vol. 386, 1975, pp. 196-202.

Brooks, S. L., et al., "Development of an On-Line Glucose Sensor for Fermentation Monitoring", *Biosensors*, vol. 3, 1987/88, pp. 45-56.

Brownlee, M., et al., "A Glucose-Controlled Insulin-Delivery System: Semisynthetic Insulin Bound to Lectin", *Science*, vol. 206, 1979, 1190-1191.

Cass, A. E., et al., "Ferricinium Ion As an Electron Acceptor for Oxido-Reductases", *Journal of Electroanalytical Chemistry*, vol. 190, 1985, pp. 117-127.

Cass, A. E., et al., "Ferrocene-Medicated Enzyme Electrode for Amperometric Determination of Glucose", *Analytical Chemistry*, vol. 56, No. 4, 1984, 667-671.

Castner, J. F., et al., "Mass Transport and Reaction Kinetic Parameters Determined Electrochemically for Immobilized Glucose Oxidase", *Biochemistry*, vol. 23 No. 10, 1984, 2203-2210.

Claremont, D. J., et al., "Biosensors for Continuous in Vivo Glucose Monitoring", *Proceedings of the Annual International Conference of the IEEE Engineering in Medicine and Biology Society*, vol. 10, 1988.

Clark Jr., L. C., et al., "Differential Anodic Enzyme Polarography for the Measurement of Glucose", *Oxygen Transport to Tissue: Instrumentation, Methods, and Physiology*, 1973, pp. 127-133.

Clark Jr., L. C., et al., "Electrode Systems for Continuous Monitoring in Cardiovascular Surgery", *Annals New York Academy of Sciences*, 1962, pp. 29-45.

Clark Jr., L. C., et al., "Long-term Stability of Electroenzymatic Glucose Sensors Implanted in Mice", *American Society of Artificial Internal Organs Transactions*, vol. XXXIV, 1988, pp. 259-265.

Clarke, W. L., et al., "Evaluating Clinical Accuracy of Systems for Self-Monitoring of Blood Glucose", *Diabetes Care*, vol. 10, No. 5, 1987, pp. 622-628.

Complaint, "Abbott Diabetes Care, Inc. v. Dexcom, Inc.", filed Aug. 11, 2005.

Complaint, Amended, "Abbott Diabetes Care, Inc. v. Dexcom, Inc.", filed Jun. 27, 2006.

Csoregi, E., et al., "Design and Optimization of a Selective Subcutaneously Implantable Glucose Electrode Based on 'Wired' Glucose Oxidase", *Analytical Chemistry*, vol. 67, No. 7, 1995, pp. 1240-1244.

Csoregi, E., et al., "Design, Characterization, and One-Point in Vivo Calibration of a Subcutaneously Implanted Glucose Electrode", *Analytical Chemistry*, vol. 66 No. 19, 1994, pp. 3131-3138.

Csoregi, E., et al., "On-Line Glucose Monitoring by Using Microdialysis Sampling and Amperometric Detection Based on 'Wired' Glucose Oxidase in Carbon Paste", *Mikrochimica Acta*, vol. 121, 1995, pp. 31-40.

Dai, W. S., et al., "Hydrogel Membranes with Mesh Size Asymmetry Based on the Gradient Crosslinking of Poly(vinyl alcohol)", *Journal of Membrane Science*, vol. 156, 1999, pp. 67-79.

Davis, G., "Electrochemical Techniques for the Development of Amperometric Biosensors", *Biosensors*, vol. 1, 1985, pp. 161-178.

Degani, Y., et al., "Direct Electrical Communication Between Chemically Modified Enzymes and Metal Electrodes. 1. Electron Transfer from Glucose Oxidase to Metal Electrodes via Electron Relays, Bound Covalently to the Enzyme", *The Journal of Physical Chemistry*, vol. 91, No. 6, 1987, pp. 1285-1289.

Degani, Y., et al., "Direct Electrical Communication Between Chemically Modified Enzymes and Metal Electrodes. 2. Methods for Bonding Electron-Transfer Relays to Glucose Oxidase and D-Amino-Acid Oxidase", *Journal of the American Chemical Society*, vol. 110, No. 8, 1988, pp. 2615-2620.

Degani, Y., et al., "Electrical Communication Between Redox Centers of Glucose Oxidase and Electrodes via Electrostatically and Covalently Bound Redox Polymers", *Journal of the American Chemical Society*, vol. 111, 1989, pp. 2357-2358.

Denisevich, P., et al., "Unidirectional Current Flow and Charge State Trapping at Redox Polymer Interfaces on Bilayer Electrodes: Principles, Experimental Demonstration, and Theory", *Journal of the American Chemical Society*, vol. 103, 1981, pp. 4727-4737.

Dicks, J. M., et al., "Ferrocene Modified Polypyrrole with Immobilized Glucose Oxidase and its Application in Amperometric Glucose Microbiosensors", *Annales de Biologie Clinique*, vol. 47, 1989, pp. 607-619.

Ellis, C. D., et al., "Selectivity and Directed Charge Transfer through an Electroactive Metallopolymer Film", *Journal of the American Chemical Society*, vol. 103, No. 25, 1981, pp. 7480-7483.

Engstrom, R. C., "Electrochemical Pretreatment of Glassy Carbon Electrodes", *Analytical Chemistry*, vol. 54, No. 13, 1982, pp. 2310-2314.

Engstrom, R. C., et al., "Characterization of Electrochemically Pretreated Glassy Carbon Electrodes", *Analytical Chemistry*, vol. 56 No. 2, 1984, pp. 136-141.

Feldman, B., et al., "A Continuous Glucose Sensor Based on Wire Enzyme™ Technology—Results from a 3-Day Trial in Patients with Type 1 Diabetes", *Diabetes Technology & Therapeutics*, vol. 5, No. 5, 2003, pp. 769-779.

(56)

References Cited

OTHER PUBLICATIONS

- Feldman, B., et al., "Correlation of Glucose Concentrations in Interstitial Fluid and Venous Blood During Periods of Rapid Glucose Change", *Abbott Diabetes Care, Inc. Freestyle Navigator Continuous Glucose Monitor Pamphlet*, 2004.
- Feldman, B., et al., "Electron Transfer Kinetics at Redox Polymer/Solution Interfaces Using Microelectrodes and Twin Electrode Thin Layer Cells", *Journal of Electroanalytical Chemistry*, vol. 194, 1985, pp. 63-81.
- Fischer, H., et al., "Intramolecular Electron Transfer Medicated by 4,4'-Bipyridine and Related Bridging Groups", *Journal of the American Chemical Society*, vol. 98, No. 18, 1976, pp. 5512-5517.
- Flentge, F., et al., "An Enzyme-Reactor for Electrochemical Monitoring of Choline and Acetylcholine: Applications in High-Performance Liquid Chromatography, Brain Tissue, Microdialysis and Cerebrospinal Fluid", *Analytical Biochemistry*, vol. 204, 1992, pp. 305-310.
- Foulds, N. C., et al., "Enzyme Entrapment in Electrically Conducting Polymers: Immobilisation of Glucose Oxidase in Polypyrrole and its Application in Amperometric Glucose Sensors", *Journal of the Chemical Society, Faraday Transactions 1*, vol. 82, 1986, pp. 1259-1264.
- Foulds, N. C., et al., "Immobilization of Glucose Oxidase in Ferrocene-Modified Pyrrole Polymers", *Analytical Chemistry*, vol. 60, No. 22, 1988, pp. 2473-2478.
- Frew, J. E., et al., "Electron-Transfer Biosensors", *Philosophical Transactions of The Royal Society of London*, vol. 316, 1987, pp. 95-106.
- Godsland, I. F., et al., "Maximizing the Success Rate of Minimal Model Insulin Sensitivity Measurements in Humans: The Importance of Basal Glucose Levels", *Clinical Science*, vol. 101, 2001, pp. 1-9.
- Gorton, L., et al., "Selective Detection in Flow Analysis Based on the Combination of Immobilized Enzymes and Chemically Modified Electrodes", *Analytica Chimica Acta*, vol. 250, 1991, pp. 203-248.
- Graham, N. B., "Poly(ethylene oxide) and Related Hydrogels," *Hydrogels in Medicine and Pharmacy*, vol. II: Polymers, Chapter 4, 1987, pp. 95-113.
- Gregg, B. A., et al., "Cross-Linked Redox Gels Containing Glucose Oxidase for Amperometric Biosensor Applications", *Analytical Chemistry*, vol. 62, No. 3, 1990, pp. 258-263.
- Gregg, B. A., et al., "Redox Polymer Films Containing Enzymes. I. A Redox-Conducting Epoxy Cement: Synthesis, Characterization, and Electrocatalytic Oxidation of Hydroquinone", *Journal of Physical Chemistry*, vol. 95, No. 15, 1991, 5970-5975.
- Hale, P. D., et al., "A New Class of Amperometric Biosensor Incorporating a Polymeric Electron-Transfer Mediator", *Journal of the American Chemical Society*, vol. 111, No. 9, 1989, pp. 3482-3484.
- Hamilton, "Hamilton Needle Gauge Index", www.hamiltoncompany.com.
- Harrison, D. J., et al., "Characterization of Perfluorosulfonic Acid Polymer Coated Enzyme Electrodes and a Miniatureized Integrated Potentiostat for Glucose Analysis in Whole Blood", *Analytical Chemistry*, vol. 60, No. 19, 1988, pp. 2002-2007.
- Hawkrige, F. M., et al., "Indirect Coulometric Titration of Biological Electron Transport Components", *Analytical Chemistry*, vol. 45, No. 7, 1973, pp. 1021-1027.
- Heller, A., "Electrical Connection Enzyme Redox Centers to Electrodes", *Journal of Physical Chemistry*, vol. 96, No. 9, 1990, pp. 3579-3587.
- Heller, A., "Electrical Wiring of Redox Enzymes", *Accounts of Chemical Research* vol. 23, No. 5, 1990, 128-134.
- Heller, A., et al., "Amperometric Biosensors Based on Three-Dimensional Hydrogel-Forming Epoxy Networks", *Sensors and Actuators B*, vol. 13-14, 1993, pp. 180-183.
- Ianniello, R. M., et al., "Differential Pulse Voltammetric Study of Direct Electron Transfer in Glucose Oxidase Chemically Modified Graphite Electrodes", *Analytical Chemistry*, vol. 54, No. 7, 1982, pp. 1098-1101.
- Ianniello, R. M., et al., "Immobilized Enzyme Chemically Modified Electrode as an Amperometric Sensor", *Analytical Chemistry*, vol. 53, No. 13, 1981, pp. 2090-2095.
- Ikeda, T., et al., "Glucose Oxidase-Immobilized Benzoquinone-Carbon Paste Electrode as a Glucose Sensor", *Agricultural and Biological Chemistry*, vol. 49, No. 2, 1985, pp. 541-543.
- Ikeda, T., et al., "Kinetics of Outer-Sphere Electron Transfers Between Metal Complexes in Solutions and Polymeric Films on Modified Electrodes", *Journal of the American Chemical Society*, vol. 103, No. 25, 1981, pp. 7422-7425.
- Johnson, J. M., et al., "Potential-Dependent Enzymatic Activity in an Enzyme Thin-Layer Cell", *Analytical Chemistry*, vol. 54, No. 8, 1982, pp. 1377-1383.
- Johnson, K. W., "Reproducible Electrodeposition of Biomolecules for the Fabrication of Miniature Electroenzymatic Biosensors", *Sensors and Actuators B*, vol. 5, 1991, pp. 85-89.
- Johnson, K. W., et al., "In vivo Evaluation of an Electroenzymatic Glucose Sensor Implanted in Subcutaneous Tissue", *Biosensors & Bioelectronics*, vol. 7, 1992, pp. 709-714.
- Johnson, P. C., "Peripheral Circulation", John Wiley & Sons, 1978, pp. 198.
- Jonsson, G., et al., "An Amperometric Glucose Sensor Made by Modification of a Graphite Electrode Surface with Immobilized Glucose Oxidase and Adsorbed Mediator" *Biosensors*, vol. 1, 1985, pp. 355-368.
- Josowicz, M., et al., "Electrochemical Pretreatment of Thin Film Platinum Electrodes", *Journal of the Electrochemical Society*, vol. 135 No. 1, 1988, pp. 112-115.
- Jungheim, K., et al., "How Rapid Does Glucose Concentration Change in Daily Life of Patients with Type 1 Diabetes?", *Second Annual Diabetes Technology Meeting*, 2002, pp. A61-A62.
- Jungheim, K., et al., "Risky Delay of Hypoglycemia Detection by Glucose Monitoring at the Arm", *Diabetes Care*, vol. 24, No. 7, 2001, pp. 1303-1304.
- Kaplan, S. M., "Wiley Electrical and Electronics Engineering Dictionary", *IEEE Press*, 2004, pp. 141, 142, 548, 549.
- Katakis, I., et al., "Electrostatic Control of the Electron Transfer Enabling Binding of Recombinant Glucose Oxidase and Redox Polyelectrolytes", *Journal of the American Chemical Society*, vol. 116, No. 8, 1994, pp. 3617-3618.
- Katakis, I., et al., "L- α -Glycerophosphate and L-Lactate Electrodes Based on the Electrochemical 'Wiring' of Oxidases", *Analytical Chemistry*, vol. 64, No. 9, 1992, pp. 1008-1013.
- Kemp, G. J., "Theoretical Aspects of One-Point Calibration: Causes and Effects of Some Potential Errors, and Their Dependence on Concentration," *Clinical Chemistry*, vol. 30, NO. 7, 1984, pp. 1163-1167.
- Kenausis, G., et al., "'Wiring' of Glucose Oxidase and Lactate Oxidase Within a Hydrogel Made with Poly(vinyl pyridine) complexed with [Os(4,4'-dimethoxy-2,2'-bipyridine)₂C1⁺]/⁺2⁺", *Journal of the Chemical Society, Faraday Transactions*, vol. 92, No. 20, 1996, pp. 4131-4136.
- Kerner, W., et al., "The Function of a Hydrogen Peroxide-Detecting Electroenzymatic Glucose Electrode is Markedly Impaired in Human Subcutaneous Tissue and Plasma," *Biosensors & Bioelectronics*, vol. 8, 1993, pp. 473-482.
- Korf, J., et al., "Monitoring of Glucose and Lactate Using Microdialysis: Applications in Neonates and Rat Brain," *Developmental Neuroscience*, vol. 15, 1993, pp. 240-246.
- Koudelka, M., et al., "In-Vivo Behaviour of Hypodermically Implanted Microfabricated Glucose Sensors", *Biosensors & Bioelectronics*, vol. 6, 1991, pp. 31-36.
- Kruger, D., et al., "Psychological Motivation and Patient Education: A Role for Continuous Glucose Monitoring", *Diabetes Technology & Therapeutics*, vol. 2, Sup. 1, 2000, pp. S93-S97.
- Kulys, J., et al., "Mediatorless Peroxidase Electrode and Preparation of Bienzyme Sensors", *Bioelectrochemistry and Bioenergetics*, vol. 24, 1990, pp. 305-311.
- Lager, W., et al., "Implantable Electrocatalytic Glucose Sensor", *Hormone Metabolic Research*, vol. 26 1994, pp. 526-530.
- Laurell, T., "A Continuous Glucose Monitoring System Based on Microdialysis", *Journal of Medical Engineering & Technology*, vol. 16, No. 5, 1992, pp. 187-193.

(56)

References Cited

OTHER PUBLICATIONS

- Lindner, E., et al., "Flexible C(Kapton-Based) Microsensor Arrays of High Stability for Cardiovascular Applications", *Journal of the Chemical Society, Faraday Transactions*, vol. 89, No. 2, 1993, pp. 361-367.
- Lortz, J., et al., "What is Bluetooth? We Explain the Newest Short-Range Connectivity Technology", *Smart Computing Learning Series, Wireless Computing*, vol. 8, Issue 5, 2002, pp. 72-74.
- Maidan, R., et al., "Elimination of Electrooxidizable Interferant-Produced Currents in Amperometric Biosensors", *Analytical Chemistry*, vol. 64, No. 23, 1992, pp. 2889-2896.
- Malin, S. F., et al., "Noninvasive Prediction of Glucose by Near-Infrared Diffuse Reflectance Spectroscopy", *Clinical Chemistry*, vol. 45, No. 9, 1999, pp. 1651-1658.
- Marko-Varga, G., et al., "Enzyme-Based Biosensor as a Selective Detection Unit in Column Liquid Chromatography", *Journal of Chromatography A*, vol. 660, 1994, pp. 153-167.
- Mastrototaro, J. J., et al., "An Electroenzymatic Glucose Sensor Fabricated on a Flexible Substrate", *Sensors and Actuators B*, vol. 5, 1991, pp. 139-144.
- Mauras, N., et al., "Lack of Accuracy of Continuous Glucose Sensors in Healthy, Nondiabetic Children: Results of the Diabetes Research in Children Network (DirecNet) Accuracy Study", *Journal of Pediatrics*, 2004, pp. 770-775.
- McGarraugh, G., et al., "Glucose Measurements Using Blood Extracted from the Forearm and the Finger", *TheraSense, Inc.*, 2000, 16 pp. 1-16.
- McGarraugh, G., et al., "Physiological Influences on Off-Finger Glucose Testing", *Diabetes Technology & Therapeutics*, vol. 3, No. 3, 2001, pp. 367-376.
- McKean, B. D., et al., "A Telemetry-Instrumentation System for Chronically Implanted Glucose and Oxygen Sensors", *IEEE Transactions on Biomedical Engineering*, vol. 35, No. 7, 1988, pp. 526-532.
- McNeil, C. J., et al., "Thermostable Reduced Nicotinamide Adenine Dinucleotide Oxidase: Application to Amperometric Enzyme Assay", *Analytical Chemistry*, vol. 61, No. 1, 1989, pp. 25-29.
- Miyawaki, O., et al., "Electrochemical and Glucose Oxidase Coenzyme Activity of Flavin Adenine Dinucleotide Covalently Attached to Glassy Carbon at the Adenine Amino Group", *Biochimica et Biophysica Acta*, vol. 838, 1985, pp. 60-68.
- Moatti-Sirat, D., et al., "Evaluating in Vitro and in Vivo the Interference of Ascorbate and Acetaminophen on Glucose Detection by a Needle-Type Glucose Sensor", *Biosensors & Bioelectronics*, vol. 7, 1992, pp. 345-352.
- Moatti-Sirat, D., et al., "Reduction of Acetaminophen Interference in Glucose Sensors by a Composite Nafion Membrane: Demonstration in Rats and Man", *Diabetologia*, vol. 37, 1994, pp. 610-616.
- Moatti-Sirat, D., et al., "Towards Continuous Glucose Monitoring: In Vivo Evaluation of a Miniaturized Glucose Sensor Implanted for Several Days in Rat Subcutaneous Tissue", *Diabetologia*, vol. 35, 1992, pp. 224-330.
- Nagy, G., et al., "A New Type of Enzyme Electrode: The Ascorbic Acid Eliminator Electrode", *Life Sciences*, vol. 31, No. 23, 1982, pp. 2611-2616.
- Nakamura, S., et al., "Effect of Periodate Oxidation on the Structure and Properties of Glucose Oxidase", *Biochimica et Biophysica Acta*, vol. 445, 1976, pp. 294-308.
- Narasimham, K., et al., "p-Benzoquinone Activation of Metal Oxide Electrodes for Attachment of Enzymes", *Enzyme and Microbial Technology*, vol. 7, 1985, pp. 283-286.
- Ohara, T. J., "Osmium Bipyridyl Redox Polymers Used in Enzyme Electrodes", *Platinum Metals Review*, vol. 39, No. 2, 1995, pp. 54-62.
- Ohara, T. J., et al., "'Wired' Enzyme Electrodes for Amperometric Determination of Glucose or Lactate in the Presence of Interfering Substances", *Analytical Chemistry*, vol. 66, No. 15, 1994, pp. 2415-2457.
- Ohara, T. J., et al., "Glucose Electrodes Based on Cross-Linked [Os(bpy)₂Cl]^{+/2+} Complexed Poly(1-Vinylimidazole) Films", *Analytical Chemistry*, vol. 65, No. 23, 1993, pp. 3512-3517.
- Olivier, C. N., et al., "In Vivo Measurement of Carbon Dioxide Tension with a Miniature Electrodes", *Pflugers Archiv: European Journal of Physiology*, vol. 373, 1978, pp. 269-272.
- Paddock, R. M., et al., "Electrocatalytic Reduction of Hydrogen Peroxide via Direct Electron Transfer From Pyrolytic Graphite Electrodes to Irreversibly Adsorbed Cytochrome C Peroxidase", *Journal of Electroanalytical Chemistry*, vol. 260, 1989, pp. 487-494.
- Palleschi, G., et al., "A Study of Interferences in Glucose Measurements in Blood by Hydrogen Peroxide Based Glucose Probes", *Analytical Biochemistry*, vol. 159, 1986, pp. 114-121.
- Pankratov, I., et al., "Sol-Gel Derived Renewable-Surface Biosensors", *Journal of Electroanalytical Chemistry*, vol. 393, 1995, pp. 35-41.
- Pathak, C., et al., "Rapid Photopolymerization of Immunoprotective Gels in Contact with Cells and Tissue", *Journal of the American Chemical Society*, vol. 114, No. 21, 1992, pp. 8311-8312.
- Pickup, J., "Developing Glucose Sensors for in Vivo Use", *Tibtech*, vol. 11, 1993, pp. 285-291.
- Pickup, J., et al., "Implantable Glucose Sensors: Choosing the Appropriate Sensing Strategy", *Biosensors*, vol. 3, 1987/88, pp. 335-346.
- Pickup, J., et al., "In Vivo Molecular Sensing in Diabetes Mellitus: An Implantable Glucose Sensor with Direct Electron Transfer", *Diabetologia*, vol. 32, 1989, pp. 213-217.
- Pickup, J., et al., "Potentially-Implantable, Amperometric Glucose Sensors with Mediated Electron Transfer: Improving the Operating Stability", *Biosensors*, vol. 4, 1989, pp. 109-119.
- Pishko, M. V., et al., "Amperometric Glucose Microelectrodes Prepared Through Immobilization of Glucose Oxidase in Redox Hydrogels", *Analytical Chemistry*, vol. 63, No. 20, 1991, pp. 2268-2272.
- Poitout, V., et al., "A Glucose Monitoring System for on Line Estimation in Man of Blood Glucose Concentration Using a Miniaturized Glucose Sensor Implanted in the Subcutaneous Tissue and a Wearable Control Unit", *Diabetologia*, vol. 36, 1993, pp. 658-663.
- Poitout, V., et al., "Calibration in Dogs of a Subcutaneous Miniaturized Glucose Sensor Using a Glucose Meter for Blood Glucose Determination", *Biosensors & Bioelectronics*, vol. 7, 1992, pp. 587-592.
- Poitout, V., et al., "In Vitro and in Vivo Evaluation in Dogs of a Miniaturized Glucose Sensor", *ASAIO Transactions*, vol. 37, No. 3, 1991, pp. M298-M300.
- Pollak, A., et al., "Enzyme Immobilization by Condensation Copolymerization into Cross-Linked Polyacrylamide Gels", *Journal of the American Chemical Society*, vol. 102, No. 20, 1980, pp. 6324-6336.
- Quinn, C. P., et al., "Kinetics of Glucose Delivery to Subcutaneous Tissue in Rats Measured with 0.3-mm Amperometric Microsensors", *The American Physiological Society*, 1995, E155-E161.
- Reach, G., et al., "Can Continuous Glucose Monitoring Be Used for the Treatment of Diabetes?", *Analytical Chemistry*, vol. 64, No. 6, 1992, pp. 381-386.
- Rebrin, K., et al., "Automated Feedback Control of Subcutaneous Glucose Concentration in Diabetic Dogs", *Diabetologia*, vol. 32, 1989, pp. 573-576.
- Reusch, W., "Other Topics: Organometallic Chemistry: Organometallic Compounds: Main Group Organometallic Compounds," *Virtual Textbook of Organic Chemistry*, 1999, Rev. 2007, 25 pages.
- Roe, J. N., et al., "Bloodless Glucose Measurements", *Critical Review in Therapeutic Drug Carrier Systems*, vol. 15, Issue 3, 1998, pp. 199-241.
- Sacks (Ed), "Guidelines and Recommendations for Laboratory Analysis in the Diagnosis and Management of Diabetes Mellitus," *The National Academy of Clinical Biochemistry Presents Laboratory Medicine Practice Guidelines*, vol. 13, 2002, pp. 8-11, 21-23, 52-56, 63.
- Sakakida, M., et al., "Development of Ferrocene-Mediated Needle-Type Glucose Sensor as a Measure of Time Subcutaneous Tissue Glucose Concentrations", *Artificial Organs Today*, vol. 2, No. 2, 1992, pp. 145-158.
- Sakakida, M., et al., "Ferrocene-Mediated Needle-Type Glucose Sensor Covered with Newly Designed Biocompatible Membrane", *Sensors and Actuators B*, vol. 13-14, 1993, pp. 319-322.

(56)

References Cited

OTHER PUBLICATIONS

- Salehi, C., et al., "A Telemetry-Instrumentation System for Long-Term Implantable Glucose and Oxygen Sensors", *Analytical Letters*, vol. 29, No. 13, 1996, pp. 2289-2308.
- Samuels, G. J., et al., "An Electrode-Supported Oxidation Catalyst Based on Ruthenium (IV). pH 'Encapsulation' in a Polymer Film", *Journal of the American Chemical Society*, vol. 103, No. 2, 1981, pp. 307-312.
- Sasso, S. V., et al., "Electropolymerized 1,2-Diaminobenzene as a Means to Prevent Interferences and Fouling and to Stabilize Immobilized Enzyme in Electrochemical Biosensors", *Analytical Chemistry*, vol. 62, No. 11, 1990, pp. 1111-1117.
- Scheller, F. W., et al., "Second Generation Biosensors," *Biosensors & Bioelectronics*, vol. 6, 1991, pp. 245-253.
- Scheller, F., et al., "Enzyme Electrodes and Their Application", *Philosophical Transactions of The Royal Society of London B*, vol. 316, 1987, pp. 85-94.
- Schmehl, R. H., et al., "The Effect of Redox Site Concentration on the Rate of Mediated Oxidation of Solution Substrates by a Redox Copolymer Film", *Journal of Electroanalytical Chemistry*, vol. 152, 1983, pp. 97-109.
- Schmidt, F. J., et al., "Calibration of a Wearable Glucose Sensor", *The International Journal of Artificial Organs*, vol. 15, No. 1, 1992, pp. 55-61.
- Schmidtke, D. W., et al., "Measurement and Modeling of the Transient Difference Between Blood and Subcutaneous Glucose Concentrations in the Rat After Injection of Insulin", *Proceedings of the National Academy of Sciences*, vol. 95, 1998, pp. 294-299.
- Shaw, G. W., et al., "In Vitro Testing of a Simply Constructed, Highly Stable Glucose Sensor Suitable for Implantation in Diabetic Patients", *Biosensors & Bioelectronics*, vol. 6, 1991, pp. 401-406.
- Shichiri, M., et al., "Glycaemic Control in Pancreatectomized Dogs with a Wearable Artificial Endocrine Pancreas", *Diabetologia*, vol. 24, 1983, pp. 179-184.
- Shichiri, M., et al., "In Vivo Characteristics of Needle-Type of Subcutaneous Glucose—Measurements of Subcutaneous Glucose Concentrations in Human Volunteers", *Hormone and Metabolic Research Supplement Series*, vol. 20, 1988, pp. 17-20.
- Shichiri, M., et al., "Membrane Design for Extending the Long-Life of an Implantable Glucose Sensor", *Diabetes Nutrition and Metabolism*, vol. 2, 1989, pp. 309-313.
- Shichiri, M., et al., "Needle-type Glucose Sensor for Wearable Artificial Endocrine Pancreas", *Implantable Sensors for Closed-Loop Prosthetic Systems*, Chapter 15, 1985, pp. 197-210.
- Shichiri, M., et al., "Telemetry Glucose Monitoring Device with Needle-Type Glucose Sensor: A Useful Tool for Blood Glucose Monitoring in Diabetic Individuals", *Diabetes Care*, vol. 9, No. 3, 1986, pp. 298-301.
- Shichiri, M., et al., "Wearable Artificial Endocrine Pancreas With Needle-Type Glucose Sensor", *The Lancet*, 1982, pp. 1129-1131.
- Shults, M. C., et al., "A Telemetry-Instrumentation System for Monitoring Multiple Subcutaneously Implanted Glucose Sensors", *IEEE Transactions on Biomedical Engineering*, vol. 41, No. 10, 1994, pp. 937-942.
- Sittampalam, G., et al., "Surface-Modified Electrochemical Detector for Liquid Chromatography", *Analytical Chemistry*, vol. 55, No. 9, 1983, pp. 1608-1610.
- Skoog, D. A., et al., "Evaluation of Analytical Data," *Fundamentals of Analytical Chemistry*, 1966, pp. 55.
- Soegijoko, S., et al., "External Artificial Pancreas: A New Control Unit Using Microprocessor", *Hormone and Metabolic Research Supplement Series*, vol. 12, 1982, pp. 165-169.
- Sprules, S. D., et al., "Evaluation of a New Disposable Screen-Printed Sensor Strip for the Measurement of NADH and Its Modification to Produce a Lactate Biosensor Employing Microliter Volumes", *Electroanalysis*, vol. 8, No. 6, 1996, pp. 539-543.
- Sternberg, F., et al., "Calibration Problems of Subcutaneous Glucosensors when Applied 'In-Situ' in Man", *Hormone and Metabolic Research*, vol. 26, 1994, pp. 523-526.
- Sternberg, R., et al., "Covalent Enzyme Coupling on Cellulose Acetate Membranes for Glucose Sensor Development", *Analytical Chemistry*, vol. 60, No. 24, 1988, pp. 2781-2786.
- Sternberg, R., et al., "Study and Development of Multilayer Needle-Type Enzyme-Based Glucose Microsensors", *Biosensors*, vol. 4, 1988, pp. 27-40.
- Suekane, M., "Immobilization of Glucose Isomerase", *Zeitschrift für Allgemeine Mikrobiologie*, vol. 22, No. 8, 1982, pp. 565-576.
- Tajima, S., et al., "Simultaneous Determination of Glucose and 1,5-Anhydroglucitol", *Chemical Abstracts*, vol. 111, No. 25, 1989, pp. 394.
- Takamura, A., et al., Drug release from Poly(vinyl alcohol) Gel Prepared by Freeze-Thaw Procedure, *Journal of Controlled Release*, vol. 20, 1992, pp. 21-27.
- Tarasevich, M. R., "Bioelectrocatalysis", *Comprehensive Treatise of Electrochemistry*, vol. 10, 1985, pp. 231-295.
- Tatsuma, T., et al., "Enzyme Monolayer—and Bilayer—Modified Tin Oxide Electrodes for the Determination of Hydrogen Peroxide and Glucose", *Analytical Chemistry*, vol. 61, No. 21, 1989, pp. 2352-2355.
- Taylor, C., et al., "'Wiring' of Glucose Oxidase Within a Hydrogel Made with Polyvinyl Imidazole Complexed with [(Os-4,4'-dimethoxy-2,2'-bipyridine)C1]⁺²⁺", *Journal of Electroanalytical Chemistry*, vol. 396, 1995, pp. 511-515.
- Thompson, M., et al., "In Vivo Probes: Problems and Perspectives", *Clinical Biochemistry*, vol. 19, 1986, pp. 255-261.
- Trojanowicz, M., et al., "Enzyme Entrapped Polypyrrole Modified Electrode for Flow-Injection Determination of Glucose", *Biosensors & Bioelectronics*, vol. 5, 1990, pp. 149-156.
- Tsalikian, E., et al., "Accuracy of the GlucoWatch G2® Biographer and the Continuous Glucose Monitoring System During Hypoglycemia: Experience of the Diabetes Research in Children Network", *Diabetes Care*, vol. 27, No. 3, 2004, pp. 722-726.
- Turner, A., et al., "Diabetes Mellitus: Biosensors for Research and Management", *zBiosensors*, vol. 1, 1985, pp. 85-115.
- Turner, R. F., et al., "A Biocompatible Enzyme Electrode for Continuous in vivo Glucose Monitoring in Whole Blood", *Sensors and Actuators B*, vol. 1, 1990, pp. 561-564.
- Tuzhi, P., et al., "Constant Potential Pretreatment of Carbon Fiber Electrodes for in Vivo Electrochemistry", *Analytical Letters*, vol. 24, No. 6, 1991, pp. 935-945.
- Umana, M., "Protein-Modified Electrochemically Active Biomaterial Surface", *U.S. Army Research Office, Analytical and Chemical Sciences Research Triangle Institute*, 1988, pp. 1-9.
- Updike, S. J., et al., "Principles of Long-Term Implanted Sensors with Emphasis on Radiotelemetric Monitoring of Blood Glucose from Inside a Subcutaneous Foreign Body Capsule (FBC)", *Biosensors in the Body: Continuous in vivo Monitoring*, Chapter 4, 1997, pp. 117-137.
- Urban, G., et al., "Miniaturized Thin-Film Biosensors Using Covalently Immobilized Glucose Oxidase", *Biosensors & Bioelectronics*, vol. 6, 1991, pp. 555-562.
- Velho, G., et al., "In Vitro and in Vivo Stability of Electrode Potentials in Needle-Type Glucose Sensors", *Diabetes*, vol. 38, No. 2, 1989, pp. 164-171.
- Velho, G., et al., "Strategies for Calibrating a Subcutaneous Glucose Sensor", *Biomedica Biochimica Acta*, vol. 48, 1989, pp. 957-964.
- Von Woedtke, T., et al., "In Situ Calibration of Implanted Electrochemical Glucose Sensors", *Biomedica Biochimica Acta*, vol. 48, 1989, pp. 943-952.
- Vreeke, M. S., et al., "Hydrogen Peroxide Electrodes Based on Electrical Connection of Redox Centers of Various Peroxidases to Electrodes through a Three-Dimensional Electron-Relaying Polymer Network", *Diagnostic Biosensors Polymers*, Chapter 15, 1993, pp. 180-193.
- Vreeke, M., et al., "Hydrogen Peroxide and β -Nicotinamide Adenine Dinucleotide Sensing Amperometric Electrodes Based on Electrical Connection of Horseradish Peroxidase Redox Centers to Electrodes through a Three-Dimensional Electron Relaying Polymer Network", *Analytical Chemistry*, vol. 64 No. 24, 1992, pp. 3084-3090.


(56)

References Cited

OTHER PUBLICATIONS

- Wagner, J. G., et al., "Continuous Amperometric Monitoring of Glucose in a Brittle Diabetic Chimpanzee with a Miniature Subcutaneous Electrode", *Proceeding of the National Academy of Sciences USA*, 1998, pp. 6379-6382.
- Wang, D. L., et al., "Miniaturized Flexible Amperometric Lactate Probe", *Analytical Chemistry*, vol. 65, No. 8, 1993, pp. 1069-1073.
- Wang, J., et al., "Activation of Glassy Carbon Electrodes by Alternating Current Electrochemical Treatment", *Analytica Chimica Acta*, vol. 167, 1985, pp. 325-334.
- Wang, J., et al., "Amperometric Biosensing of Organic Peroxides with Peroxidase-Modified Electrodes", *Analytica Chimica Acta*, vol. 254, 1991, pp. 81-88.
- Wang, J., et al., "Highly Selective Membrane-Free, Mediator-Free Glucose Biosensor", *Analytical Chemistry*, vol. 66, No. 21, 1994, pp. 3600-3606.
- Wang, J., et al., "Screen-Printable Sol-Gel Enzyme-Containing Carbon Inks", *Analytical Chemistry*, vol. 68, No. 15, 1996, pp. 2705-2708.
- Wang, J., et al., "Sol-Gel-Derived Metal-Dispersed Carbon Composite Amperometric Biosensors", *Electroanalysis*, vol. 9, No. 1, 1997, pp. 52-55.
- Williams, D. L., et al., "Electrochemical-Enzymatic Analysis of Blood Glucose and Lactate", *Analytical Chemistry*, vol. 42 No. 1, 1970, pp. 118-121.
- Wilson, G. S., et al., "Progress Toward the Development of an Implantable Sensor for Glucose", *Clinical Chemistry*, vol. 38, No. 9, 1992, pp. 1613-1617.
- Wood, W. D., et al., "Hermetic Sealing with Epoxy", *Mechanical Engineering*, 1990, pp. 46-48.
- Yabuki, S., et al., "Electro-Conductive Enzyme Membrane", *Journal of the Chemical Society, Chemical Communications*, 1989, pp. 945-946.
- Yang, C., et al., "A Comparison of Physical Properties and Fuel Cell Performance of Nafion and Zirconium Phosphate/Nafion Composite Membranes", *Journal of Membrane Science*, vol. 237, 2004, pp. 145-161.
- Yang, L., et al., "Determination of Oxidase Enzyme Substrates Using Cross-Flow Thin-Layer Amperometry", *Electroanalysis*, vol. 8, No. 8-9, 1996, pp. 716-721.
- Yao, T., "A Chemically-Modified Enzyme Membrane Electrode as an Amperometric Glucose Sensor", *Analytica Chimica Acta*, vol. 148, 1983, pp. 27-33.
- Ye, L., et al., "High Current Density 'Wired' Quinoprotein Glucose Dehydrogenase Electrode", *Analytical Chemistry*, vol. 65, No. 3, 1993, pp. 238-241.
- Yildiz, A., et al., "Evaluation of an Improved Thin-Layer Electrode", *Analytical Chemistry*, vol. 40, No. 7, 1968, pp. 1018-1024.
- Zamzow, K., et al., "New Wearable Continuous Blood Glucose Monitor (BGM) and Artificial Pancreas (AP)", *Diabetes*, vol. 39, 1990, pp. 5A-20.
- Zhang, Y., et al., "Application of Cell Culture Toxicity Tests to the Development of Implantable Biosensors", *Biosensors & Bioelectronics*, vol. 6, 1991, pp. 653-661.
- Zhang, Y., et al., "Elimination of the Acetaminophen Interference in an Implantable Glucose Sensor", *Analytical Chemistry*, vol. 66, No. 7, 1994, pp. 1183-1188.
- European Patent Application No. 03808614.6, Examination Report mailed Dec. 30, 2011.
- European Patent Application No. 03808614.6, Supplementary European Search Report with International Filing Date of Dec. 26, 2003.
- PCT Application No. PCT/US2003/041640, International Preliminary Examination Report mailed Jul. 11, 2005.
- PCT Application No. PCT/US2003/041640, International Search Report mailed Dec. 28, 2004.
- U.S. Appl. No. 10/745,878, Notice of Allowance mailed Jul. 26, 2010.
- U.S. Appl. No. 10/745,878, Office Action mailed Feb. 10, 2006.
- U.S. Appl. No. 10/745,878, Office Action mailed Feb. 24, 2005.
- U.S. Appl. No. 10/745,878, Office Action mailed Feb. 5, 2010.
- U.S. Appl. No. 10/745,878, Office Action mailed May 30, 2008.
- U.S. Appl. No. 10/745,878, Office Action mailed Sep. 15, 2009.
- U.S. Appl. No. 10/745,878, Office Action mailed Sep. 21, 2007.
- U.S. Appl. No. 12/902,138, Notice of Allowance, mailed Feb. 23, 2012.
- U.S. Appl. No. 12/902,138, Office Action mailed Jan. 27, 2012.
- U.S. Appl. No. 12/902,138, Office Action mailed Jun. 7, 2011.

* cited by examiner

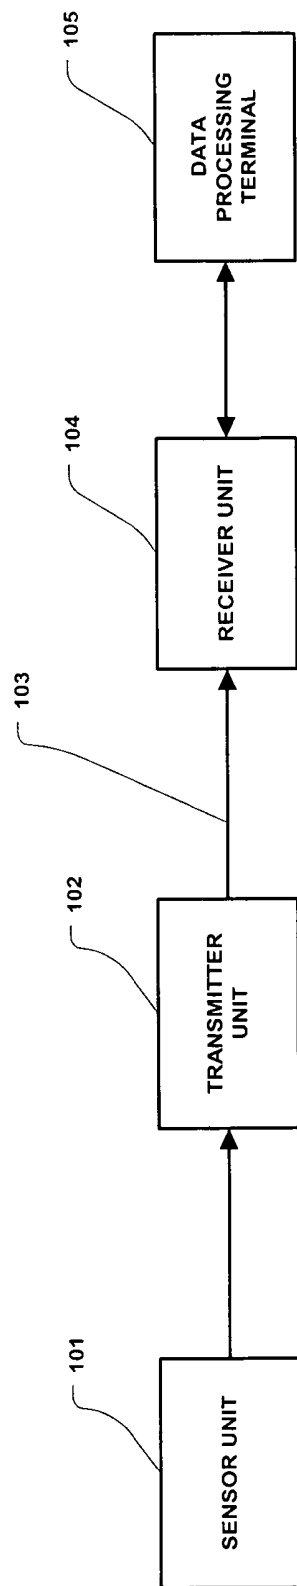

100

FIGURE 1

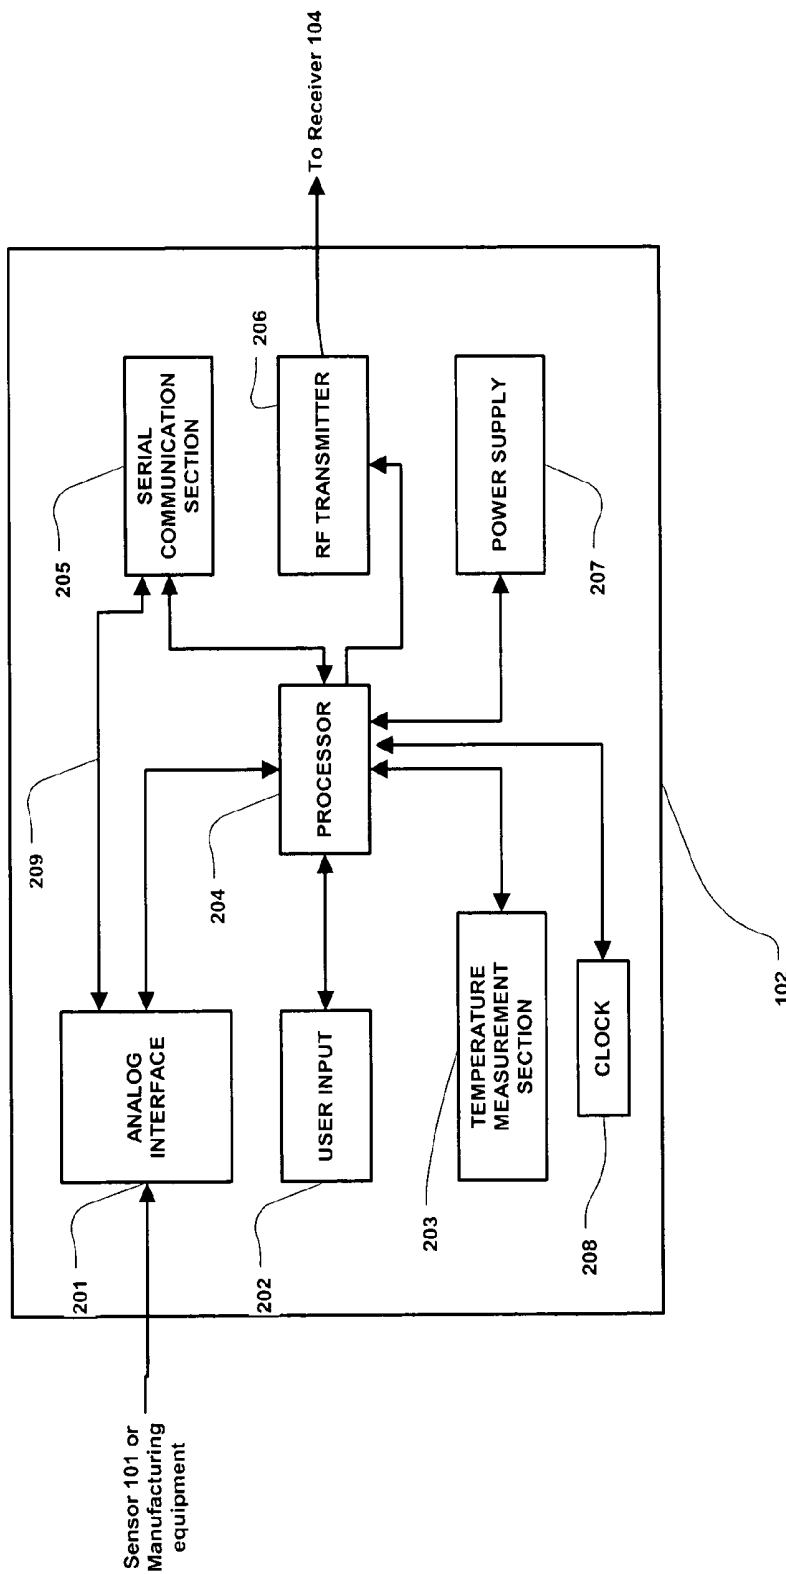


FIGURE 2

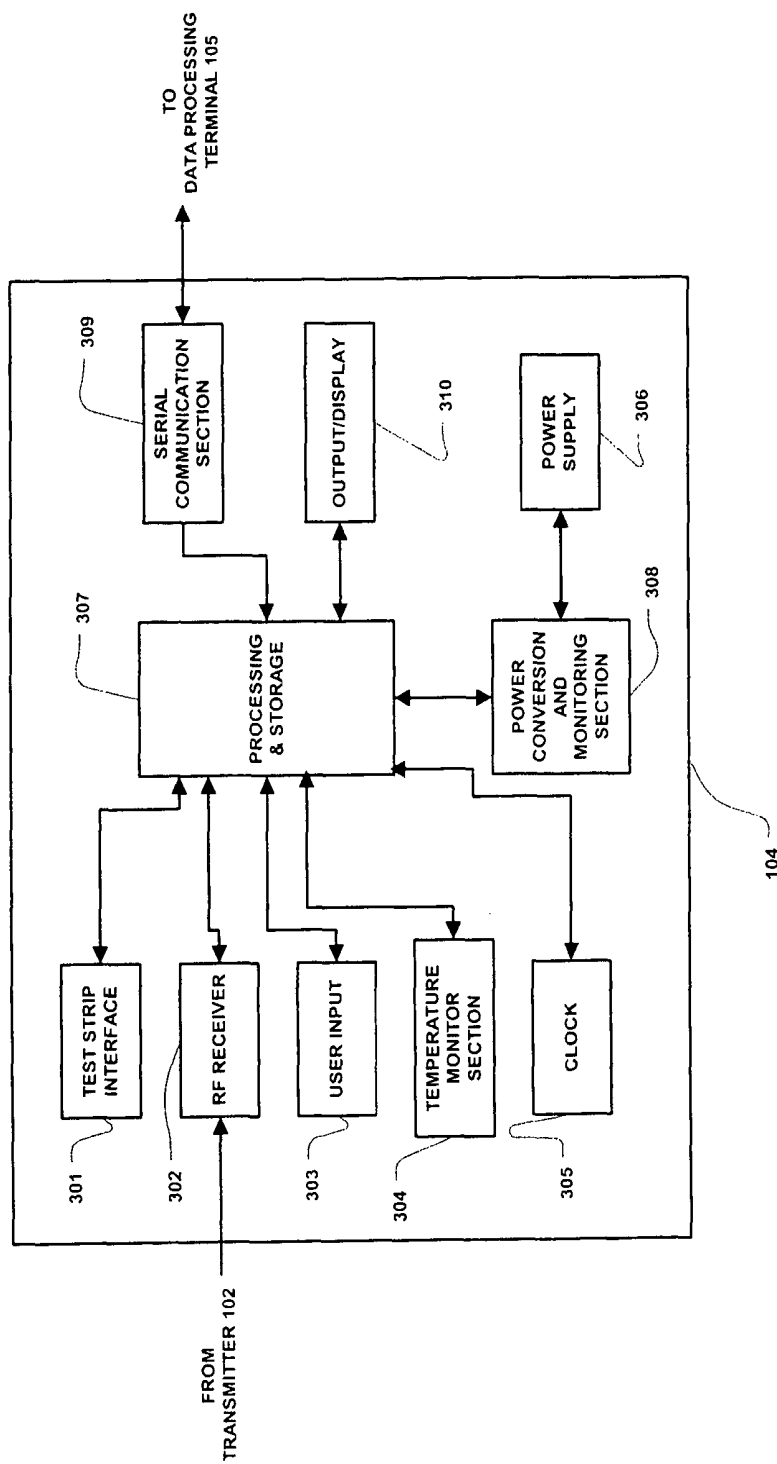


FIGURE 3

Byte		High Nibble	Low Nibble
0	TX ID (1sbyte)		
1	Tx Time		
2	Tx Status	Tx Status n1	Tx Status n0
3		Sensor n0	Tx Status n2
4		Sensor n2	Sensor n1
5		Tx Status-1 n1	Tx Status-1 n0
6		Sensor-1 n0	Tx Status-1 n2
7		Sensor-1 n2	Sensor-1 n1
8		Tx Status-2 n1	Tx Status-2 n0
9		Sensor-2 n0	Tx Status-2 n2
10		Sensor-2 n2	Sensor-2 n1
11		CV-1, Tx Status-1	CV, Tx Status
12		Tx Pending, Tx Batt	CV-2, Tx Status-2

FIGURE 4

1	Packed Data	13 bytes
2	Tx ID, middle sb	1 byte
3	Tx ID, msb	1 byte
4	Zero Pad	232 bytes
5	Parity Symbols	8 bytes
	Total	255 bytes

FIGURE 5A

1	Packed data	13 bytes
2	Parity Symbols	8 bytes
	Total	21 bytes

FIGURE 5B

1	0x00 0x00 0x12 0x34	4 bytes
1	Depadded Data Block Contents	21 bytes

FIGURE 5C

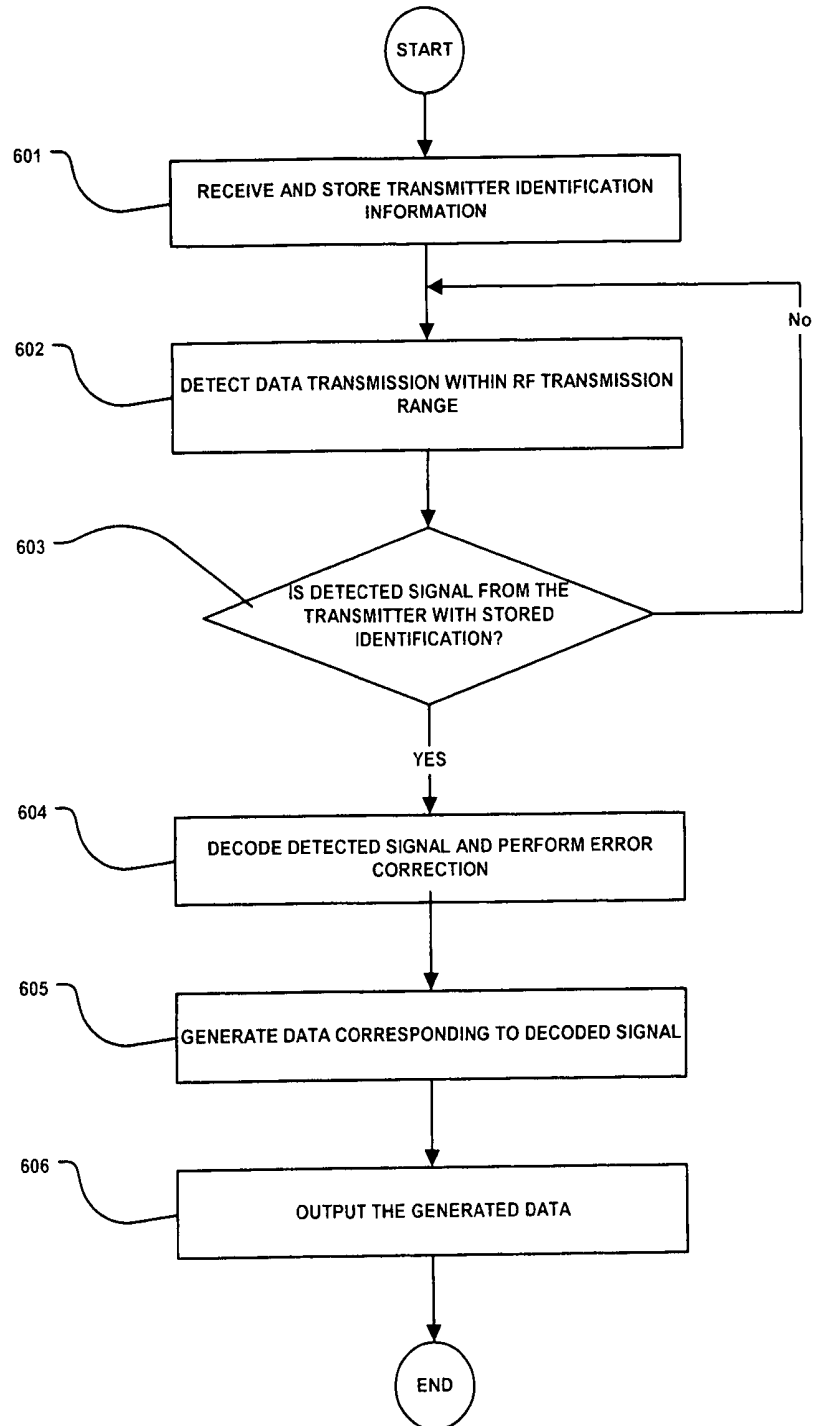


FIGURE 6

CONTINUOUS GLUCOSE MONITORING SYSTEM AND METHODS OF USE

RELATED APPLICATIONS

The present application is a continuation of U.S. patent application Ser. No. 12/902,138 filed Oct. 11, 2010, now U.S. Pat. No. 8,187,183, which is a continuation of U.S. patent application Ser. No. 10/745,878 filed Dec. 26, 2003, now U.S. Pat. No. 7,811,231, which claims the benefit of U.S. Provisional Application No. 60/437,374 filed Dec. 31, 2002, entitled "Continuous Glucose Monitoring System and Methods of Use", the disclosures of each of which are incorporated herein by reference for all purposes.

BACKGROUND

The present invention relates to continuous glucose monitoring systems. More specifically, the present invention relates to an in-vivo continuous glucose monitoring system which detects glucose levels continuously and transfers the detected glucose level information at predetermined time intervals to data processing devices for monitoring, diagnosis and analysis.

SUMMARY

A continuous glucose monitoring system in accordance with one embodiment of the present invention includes a sensor configured to detect one or more glucose levels, a transmitter operatively coupled to the sensor, the transmitter configured to receive the detected one or more glucose levels, the transmitter further configured to transmit signals corresponding to the detected one or more glucose levels, a receiver operatively coupled to the transmitter configured to receive transmitted signals corresponding to the detected one or more glucose levels, where the transmitter is configured to transmit a current data point and at least one previous data point, the current data point and the at least one previous data point corresponding to the detected one or more glucose levels.

The receiver may be operatively coupled to the transmitter via an RF communication link, and further, configured to decode the encoded signals received from the transmitter.

In one embodiment, the transmitter may be configured to periodically transmit a detected and processed glucose level from the sensor to the receiver via the RF data communication link. In one embodiment, the transmitter may be configured to sample four times every second to obtain 240 data points for each minute, and to transmit at a rate of one data point (e.g., an average value of the 240 sampled data points for the minute) per minute to the receiver.

The transmitter may be alternately configured to transmit three data points per minute to the receiver, the first data point representing the current sampled data, and the remaining two transmitted data points representing the immediately past two data points previously sent to the receiver. In this manner, in the case where the receiver does not successfully receive the sampled data from the transmitter, at the subsequent data transmission, the immediately prior transmitted data is received by the receiver. Thus, even with a faulty connection between the transmitter and the receiver, or a failed RF data link, the present approach ensures that missed data points may be ascertained from the subsequent data point transmissions without retransmission of the missed data points to the receiver.

The transmitter may be configured to encode the detected one or more glucose levels received from the sensor to generate encoded signals, and to transmit the encoded signals to the receiver. In one embodiment, the transmitter may be configured to transmit the encoded signals to the receiver at a transmission rate of one data point per minute. Further, the transmitter may be configured to transmit the current data point and the at least one previous data points in a single transmission per minute to the receiver. In one aspect, the current data point may correspond to a current glucose level, and where the at least one previous data point may include at least two previous data points corresponding respectively to at least two consecutive glucose levels, the one of the at least two consecutive glucose levels immediately preceding the current glucose level.

In a further embodiment, the receiver may include an output unit for outputting the received transmitted signals corresponding to one or more glucose levels. The output unit may include a display unit for displaying data corresponding to the one or more glucose levels, where the display unit may include one of a LCD display, a cathode ray tube display, and a plasma display.

The displayed data may include one or more of an alphanumeric representation corresponding to the one or more glucose levels, a graphical representation of the one or more glucose levels, and a three-dimensional representation of the one or more glucose levels. Moreover, the display unit may be configured to display the data corresponding to the one or more glucose levels substantially in real time.

Further, the output unit may include a speaker for outputting an audio signal corresponding to the one or more glucose levels.

In yet a further embodiment, the receiver may be configured to store an identification information corresponding to the transmitter.

The receiver may be further configured to perform a time hopping procedure for synchronizing with the transmitter. Alternatively, the receiver may be configured to synchronize with the transmitter based on the signal strength detected from the transmitter, where the detected signal strength exceeds a preset threshold level.

The transmitter in one embodiment may be encased in a substantially water-tight housing to ensure continuous operation even in the situation where the transmitter is in contact with water.

Furthermore, the transmitter may be configured with a disable switch which allows the user to temporarily disable the transmission of data to the receiver when the user is required to disable electronic devices, for example, when aboard an airplane. In another embodiment, the transmitter may be configured to operate in an additional third state (such as under Class B radiated emissions standard) in addition to the operational state and the disable state discussed above, so as to allow limited operation while aboard an airplane yet still complying with the Federal Aviation Administration (FAA) regulations. Additionally, the disable switch may also be configured to switch the transmitter between various operating modes such as fully functional transmission mode, post-manufacture sleep mode, and so on. In this manner, the power supply for the transmitter is optimized for prolonged usage by effectively managing the power usage.

Furthermore, the transmitter may be configured to transmit the data to the receiver in predetermined data packets, encoded, in one embodiment, using Reed Solomon encoding, and transmitted via the RF communication link. Additionally, in a further aspect of the present invention, the RF communication link between the transmitter and the receiver of the

continuous glucose monitoring system may be implemented using a low cost, off the shelf remote keyless entry (RKE) chip set.

The receiver in an additional embodiment may be configured to perform, among others, data decoding, error detection and correction (using, for example, forward error correction) on the encoded data packets received from the transmitter to minimize transmission errors such as transmitter stabilization errors and preamble bit errors resulting from noise. The receiver is further configured to perform a synchronized time hopping procedure with the transmitter to identify and synchronize with the corresponding transmitter for data transmission.

Additionally, the receiver may include a graphical user interface (GUI) for displaying the data received from the transmitter for the user. The GUI may include a liquid crystal display (LCD) with backlighting feature to enable visual display in dark surroundings. The receiver may also include an output unit for generating and outputting audible signal alerts for the user, or placing the receiver in a vibration mode for alerting the user by vibrating the receiver.

More specifically, in a further aspect, the receiver may be configured to, among others, display the received glucose levels on a display section of the receiver either real time or in response to user request, and provide visual (and/or auditory) notification to the user of the detected glucose levels being monitored. To this end, the receiver is configured to identify the corresponding transmitter from which it is to receive data via the RF data link, by initially storing the identification information of the transmitter, and performing a time hopping procedure to isolate the data transmission from the transmitter corresponding to the stored identification information and thus to synchronize with the transmitter. Alternatively, the receiver may be configured to identify the corresponding transmitter based on the signal strength detected from the transmitter, determined to exceed a preset threshold level.

A method in accordance with one embodiment of the present invention includes the steps of receiving an identification information corresponding to a transmitter, detecting data within a predetermined RF transmission range, determining whether the detected data is transmitted from the transmitter, decoding the detected data, and generating an output signal corresponding to the decoded data.

In one embodiment, the step of determining whether the detected data transmission is transmitted from the transmitter may be based on the received identification information. In another embodiment, the step of determining whether the detected data transmission is transmitted from the transmitter may be based on the signal strength and duration of the detected data within the predetermined RF transmission range.

In a further embodiment, the step of decoding may also include the step of performing error correction on the decoded data. Moreover, the step of decoding may include the step of performing Reed-Solomon decoding on the detected data.

In the manner described, the present invention provides a continuous glucose monitoring system that is simple to use and substantially compact so as to minimize any interference with the user's daily activities. Furthermore, the continuous glucose monitoring system may be configured to be substantially water-resistant so that the user may freely bathe, swim, or enjoy other water related activities while using the monitoring system. Moreover, the components comprising the monitoring system including the transmitter and the receiver are configured to operate in various modes to enable power savings, and thus enhancing post-manufacture shelf life.

INCORPORATION BY REFERENCE

Applicants herein incorporate by reference application Ser. No. 09/753,746 filed on Jan. 2, 2001, and issued on May 6, 2003 as U.S. Pat. No. 6,560,471, entitled "Analyte Monitoring Device and Methods of Use" assigned to the Assignee of the present application for all purposes.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 illustrates a continuous glucose monitoring system in accordance with one embodiment of the present invention;

FIG. 2 is a block diagram of the transmitter of the continuous glucose monitoring system shown in FIG. 1 in accordance with one embodiment of the present invention;

FIG. 3 is a block diagram of the receiver of the continuous glucose monitoring system shown in FIG. 1 in accordance with one embodiment of the present invention;

FIG. 4 illustrates a data packet of the transmitter of the continuous glucose monitoring system shown in FIG. 1 in accordance with one embodiment of the present invention;

FIGS. 5A, 5B and 5C illustrate a data packet table for Reed-Solomon encoding in the transmitter, a depadded data table, and a link prefix table, respectively, in accordance with one embodiment of the continuous glucose monitoring system of FIG. 1; and

FIG. 6 is a flowchart illustrating the time hopping procedure for the receiver of the continuous glucose monitoring system shown in FIG. 1 in accordance with one embodiment of the present invention.

DETAILED DESCRIPTION

FIG. 1 illustrates a continuous glucose monitoring system 100 in accordance with one embodiment of the present invention. In such embodiment, the continuous glucose monitoring system 100 includes a sensor 101, a transmitter 102 coupled to the sensor 101, and a receiver 104 which is configured to communicate with the transmitter 102 via a communication link 103. The receiver 104 may be further configured to transmit data to a data processing terminal 105 for evaluating the data received by the receiver 104. Only one sensor 101, transmitter 102, communication link 103, receiver 104, and data processing terminal 105 are shown in the embodiment of the continuous glucose monitoring system 100 illustrated in FIG. 1. However, it will be appreciated by one of ordinary skill in the art that the continuous glucose monitoring system 100 may include one or more sensor 101, transmitter 102, communication link 103, receiver 104, and data processing terminal 105, where each receiver 104 is uniquely synchronized with a respective transmitter 102.

In one embodiment of the present invention, the sensor 101 is physically positioned on the body of a user whose glucose is being monitored. The term user as used herein is intended to include humans, animals, as well as any other who might benefit from the use of the glucose monitoring system 100. The sensor 101 is configured to continuously sample the glucose level of the user and convert the sampled glucose level into a corresponding data signal for transmission by the transmitter 102. In one embodiment, the transmitter 102 is mounted on the sensor 101 so that both devices are positioned on the user's body. The transmitter 102 performs data processing such as filtering and encoding on data signals, each of which corresponds to a sampled glucose level of the user, for transmission to the receiver 104 via the communication link 103.

In one embodiment, the continuous glucose monitoring system **100** is configured as a one-way RF communication path from the transmitter **102** to the receiver **104**. In such embodiment, the transmitter **102** transmits the sampled data signals received from the sensor **101** without acknowledgement from the receiver **104** that the transmitted sampled data signals have been received. For example, the transmitter **102** may be configured to transmit the encoded sampled data signals at a fixed rate (e.g., at one minute intervals) after the completion of the initial power on procedure. Likewise, the receiver **104** may be configured to detect such transmitted encoded sampled data signals at predetermined time intervals.

As discussed in further detail below, in one embodiment of the present invention the receiver **104** includes two sections. The first section is an analog interface section that is configured to communicate with the transmitter **102** via the communication link **103**. In one embodiment, the analog interface section may include an RF receiver and an antenna for receiving and amplifying the data signals from the transmitter **102**, which are thereafter, demodulated with a local oscillator and filtered through a band-pass filter. The second section of the receiver **104** is a data processing section which is configured to process the data signals received from the transmitter **102** such as by performing data decoding, error detection and correction, data clock generation, and data bit recovery.

In operation, upon completing the power-on procedure, the receiver **104** is configured to detect the presence of the transmitter **102** within its range based on the strength of the detected data signals received from the transmitter **102**. For example, in one embodiment, the receiver **104** is configured to detect signals whose strength exceeds a predetermined level to identify the transmitter **102** from which the receiver **104** is to receive data. Alternatively, the receiver **104** in a further embodiment may be configured to respond to signal transmission for a predetermined transmitter identification information of a particular transmitter **102** such that, rather than detecting the signal strength of a transmitter **102** to identify the transmitter, the receiver **104** may be configured to detect transmitted signal of a predetermined transmitter **102** based on the transmitted transmitter identification information corresponding to the pre-assigned transmitter identification information for the particular receiver **104**.

In one embodiment, the identification information of the transmitters **102** includes a 16-bit ID number. In an alternate embodiment, the ID number may be a predetermined length including a 24-bit ID number or a 32-bit ID number. Further, any other length ID number may also be used. Thus, in the presence of multiple transmitters **102**, the receiver **104** will only recognize the transmitter **102** which corresponds to the stored identification information. Data signals transmitted from the other transmitters within the range of the receiver **104** are considered invalid signals.

Referring again to FIG. 1, where the receiver **104** determines the corresponding transmitter **102** based on the signal strength of the transmitter **102**, when the receiver **104** is initially powered-on, the receiver **104** is configured to continuously sample the signal strength of the data signals received from the transmitters within its range. If the signal strength of the data signals meets or exceeds the signal strength threshold level and the transmission duration threshold level, the receiver **104** returns a positive indication for the transmitter **102** transmitting the data signals. That is, in one embodiment, the receiver **104** is configured to positively identify the transmitter **102** after one data signal transmission. Thereafter, the receiver **104** is configured to detect positive indications for three consecutive data signal transmissions for

a predetermined time period. At such point, after three consecutive transmissions, the transmitter **102** is fully synchronized with the receiver **104**.

Upon identifying the appropriate transmitter **102**, the receiver **104** begins a decoding procedure to decode the received data signals. In one embodiment, a sampling clock signal may be obtained from the preamble portion of the received data signals. The decoded data signals, which include fixed length data fields, are then sampled with the sampling clock signal. In one embodiment of the present invention, based on the received data signals and the time interval between each of the three data signal transmissions, the receiver **104** determines the wait time period for receiving the next transmission from the identified and synchronized transmitter **102**. Upon successful synchronization, the receiver **104** begins receiving from the transmitter **102** data signals corresponding to the user's detected glucose level. As described in further detail below, the receiver **104** in one embodiment is configured to perform synchronized time hopping with the corresponding synchronized transmitter **102** via the communication link **103** to obtain the user's detected glucose level.

Referring yet again to FIG. 1, the data processing terminal **105** may include a personal computer, a portable computer such as a laptop or a handheld device (e.g., personal digital assistants (PDAs)), and the like, each of which is configured for data communication with the receiver via a wired or a wireless connection. Additionally, the data processing terminal **105** may further be connected to a data network (not shown) for storing, retrieving and updating data corresponding to the detected glucose level of the user.

FIG. 2 is a block diagram of the transmitter **102** of the continuous glucose monitoring system **100** in accordance with one embodiment of the present invention. The transmitter **102** includes an analog interface **201** configured to communicate with the sensor **101** (FIG. 1), a user input **202**, and a temperature detection section **203**, each of which is operatively coupled to a transmitter processor **204** such as a central processing unit (CPU). Further shown in FIG. 2 are a transmitter serial communication section **205** and an RF transmitter **206**, each of which is also operatively coupled to the transmitter processor **204**. Moreover, a power supply **207** is also provided in the transmitter **102** to provide the necessary power for the transmitter **102**. Additionally, as can be seen from the Figure, clock **208** is provided to, among others, supply real time information to the transmitter processor **204**.

In one embodiment, a unidirectional input path is established from the sensor **101** (FIG. 1) and/or manufacturing and testing equipment to the analog interface **201**, while a unidirectional output is established from the output of the RF transmitter **206**. In this manner, a data path is shown in FIG. 2 between the aforementioned unidirectional input and output via a dedicated link **209** from the analog interface **201** to serial communication section **205**, thereafter to the processor **204**, and then to the RF transmitter **206**. As such, in one embodiment, through the data path described above, the transmitter **102** is configured to transmit to the receiver **104** (FIG. 1), via the communication link **103** (FIG. 1), processed and encoded data signals received from the sensor **101** (FIG. 1). Additionally, the unidirectional communication data path between the analog interface **201** and the RF transmitter **206** discussed above allows for the configuration of the transmitter **102** for operation upon completion of the manufacturing process as well as for direct communication for diagnostic and testing purposes.

Referring back to FIG. 2, the user input **202** includes a disable device that allows the operation of the transmitter **102**

to be temporarily disabled, such as, by the user wearing the transmitter 102. In an alternate embodiment, the disable device of the user input 202 may be configured to initiate the power-up procedure of the transmitter 102.

As discussed above, the transmitter processor 204 is configured to transmit control signals to the various sections of the transmitter 102 during the operation of the transmitter 102. In one embodiment, the transmitter processor 204 also includes a memory (not shown) for storing data such as the identification information for the transmitter 102, as well as the data signals received from the sensor 101. The stored information may be retrieved and processed for transmission to the receiver 104 under the control of the transmitter processor 204. Furthermore, the power supply 207 may include a commercially available battery pack.

The physical configuration of the transmitter 102 is designed to be substantially water resistant, so that it may be immersed in non-saline water for a brief period of time without degradation in performance. Furthermore, in one embodiment, the transmitter 102 is designed so that it is substantially compact and light-weight, not weighing more than a predetermined weight such as, for example, approximately 18 grams. Furthermore, the dimensions of the transmitter 102 in one embodiment includes 52 mm in length, 30 mm in width and 12 mm in thickness. Such small size and weight enable the user to easily carry the transmitter 102.

The transmitter 102 is also configured such that the power supply section 207 is capable of providing power to the transmitter for a minimum of three months of continuous operation after having been stored for 18 months in a low-power (non-operating) mode. In one embodiment, this may be achieved by the transmitter processor 204 operating in low power modes in the non-operating state, for example, drawing no more than approximately 1 μ A. Indeed, in one embodiment, the final step during the manufacturing process of the transmitter 102 places the transmitter 102 in the lower power, non-operating state (i.e., post-manufacture sleep mode). In this manner, the shelf life of the transmitter 102 may be significantly improved.

Referring again to FIG. 2, the analog interface 201 of the transmitter 102 in one embodiment includes a sensor interface (not shown) configured to physically couple to the various sensor electrodes (such as, for example, working electrode, reference electrode, counter electrode, (not shown)) of the sensor 101 (FIG. 1) of the monitoring system 100. The analog interface section 201 further includes a potentiostat circuit (not shown) which is configured to generate the Poise voltage determined from the current signals received from the sensor electrodes. In particular, the Poise voltage is determined by setting the voltage difference between the working electrode and the reference electrode (i.e., the offset voltage between the working electrode and the reference electrode of the sensor 101). Further, the potentiostat circuit also includes a transimpedance amplifier for converting the current signal on the working electrode into a corresponding voltage signal proportional to the current. The signal from the potentiostat circuit is then low pass filtered with a predetermined cut-off frequency to provide anti-aliasing, and thereafter, passed through a gain stage to provide sufficient gain to allow accurate signal resolution detected from the sensor 101 for analog-to-digital conversion and encoding for transmission to the receiver 104.

Referring yet again to FIG. 2, the temperature detection section 203 of the transmitter 102 is configured to monitor the temperature of the skin near the sensor insertion site. The temperature reading is used to adjust the glucose readings obtained from the analog interface 201. As discussed above,

the input section 202 of the transmitter 102 includes the disable device which allows the user to temporarily disable the transmitter 102 such as for, example, to comply with the FAA regulations when aboard an aircraft. Moreover, in a further embodiment, the disable device may be further configured to interrupt the transmitter processor 204 of the transmitter 102 while in the low power, non-operating mode to initiate operation thereof.

The RF transmitter 206 of the transmitter 102 may be configured for operation in the frequency band of 315 MHz to 322 MHz, for example, in the United States. Further, in one embodiment, the RF transmitter 206 is configured to modulate the carrier frequency by performing Frequency Shift Keying and Manchester encoding. In one embodiment, the data transmission rate is 19,200 symbols per second, with a minimum transmission range for communication with the receiver 104.

FIG. 3 is a block diagram of the receiver 104 of the continuous glucose monitoring system 100 in accordance with one embodiment of the present invention. Referring to FIG. 3, the receiver 104 includes a blood glucose test strip interface 301, an RF receiver 302, an input 303, a temperature detection section 304, and a clock 305, each of which is operatively coupled to a receiver processor 307. As can be further seen from the Figure, the receiver 104 also includes a power supply 306 operatively coupled to a power conversion and monitoring section 308. Further, the power conversion and monitoring section 308 is also coupled to the receiver processor 307. Moreover, also shown are a receiver serial communication section 309, and an output 310, each operatively coupled to the receiver processor 307.

In one embodiment, the test strip interface 301 includes a glucose level testing portion to receive a manual insertion of a glucose testing strip, and thereby determine and display the glucose level of the testing strip on the output 310 of the receiver 104. This manual testing of glucose can be used to calibrate sensor 101. The RF receiver 302 is configured to communicate, via the communication link 103 (FIG. 1) with the RF transmitter 206 of the transmitter 102, to receive encoded data signals from the transmitter 102 for, among others, signal mixing, demodulation, and other data processing. The input 303 of the receiver 104 is configured to allow the user to enter information into the receiver 104 as needed. In one aspect, the input 303 may include one or more keys of a keypad, a touch-sensitive screen, or a voice-activated input command unit. The temperature detection section 304 is configured to provide temperature information of the receiver 104 to the receiver processor 307, while the clock 305 provides, among others, real time information to the receiver processor 307.

Each of the various components of the receiver 104 shown in FIG. 3 are powered by the power supply 306 which, in one embodiment, includes a battery. Furthermore, the power conversion and monitoring section 308 is configured to monitor the power usage by the various components in the receiver 104 for effective power management and to alert the user, for example, in the event of power usage which renders the receiver 104 in sub-optimal operating conditions. An example of such sub-optimal operating condition may include, for example, operating the vibration output mode (as discussed below) for a period of time thus substantially draining the power supply 306 while the processor 307 (thus, the receiver 104) is turned on. Moreover, the power conversion and monitoring section 308 may additionally be configured to include a reverse polarity protection circuit such as a field effect transistor (FET) configured as a battery activated switch.

The serial communication section 309 in the receiver 104 is configured to provide a bi-directional communication path from the testing and/or manufacturing equipment for, among others, initialization, testing, and configuration of the receiver 104. Serial communication section 309 can also be used to upload data to a computer, such as time-stamped blood glucose data. The communication link with an external device (not shown) can be made, for example, by cable, infrared (IR) or RF link. The output 310 of the receiver 104 is configured to provide, among others, a graphical user interface (GUI) such as a liquid crystal display (LCD) for displaying information. Additionally, the output 310 may also include an integrated speaker for outputting audible signals as well as to provide vibration output as commonly found in handheld electronic devices, such as mobile telephones presently available. In a further embodiment, the receiver 104 also includes an electro-luminescent lamp configured to provide backlighting to the output 310 for output visual display in dark ambient surroundings.

Referring back to FIG. 3, the receiver 104 in one embodiment may also include a storage section such as a programmable, non-volatile memory device as part of the processor 307, or provided separately in the receiver 104, operatively coupled to the processor 307. The processor 307 is further configured to perform Manchester decoding as well as error detection and correction upon the encoded data signals received from the transmitter 102 via the communication link 103.

In conjunction with FIGS. 4, 5A, 5B and 5C, a description is provided of a data packet from the transmitter 102 to the receiver 104 via the communication link 103.

FIG. 4 illustrates a data pack from the transmitter 102 (FIG. 1) in accordance with one embodiment of the present invention. Referring to FIG. 4, each data packet from the transmitter 102 includes 13 bytes as shown in the Figure. For example, the first byte (zero byte) includes the transmitter 102 identification information ("Tx ID"), while the third byte (byte two) provides transmitter status information, where a high nibble (byte) indicates an operating mode status, while a low nibble indicates a non-operating mode. In this manner, the signals received from the sensor 101 are packed into 13-byte data packs, for transmission to the receiver 104.

FIGS. 5A, 5B and 5C illustrate a data packet table for Reed-Solomon encoding in the transmitter, a depadded data table, and a link prefix table, respectively, in accordance with one embodiment of the continuous glucose monitoring system of FIG. 1. Referring to FIG. 5A, it can be seen that the Reed Solomon encoded data block contents include 13 bytes of packed data (FIG. 4), one byte of the middle significant bit of the transmitter identification information (Tx ID), one byte of the most significant bit of the transmitter identification information, 232 bytes of zero pads, 8 bytes of parity symbols, to comprise a total of 255 bytes. In one embodiment, the Reed Solomon encode procedure at the transmitter 102 uses 8 bit symbols for a 255 symbol block to generate 8 parity symbols. Thereafter, the transmitter 102 is configured to remove the 232 bytes of zero pads, resulting in the 21 bytes of depadded data block including the 13 bytes of packed data as well as the 8 bytes of the parity symbols as shown in FIG. 5B.

Thereafter, a link prefix is added to the depadded data block to complete the data packet for transmission to the receiver 104. The link prefix allows the receiver 104 to synchronize with the transmitter 102 as described in further detail below. More specifically, as shown in FIG. 5C, the transmitter 102 is configured to add 4 bytes of link prefix (0x00, 0x00, 0x12, and 0x34) to the 21 bytes of depadded data block to result in 25 bytes of data packet. Once powered up and enabled in

operational mode, the transmitter 102 is configured to transmit the 25 byte data packet once every minute. More specifically, the transmitter 102 is configured to Manchester encode the data at 2 bits per data bit (0=10; 1=01), and transmit the Manchester bits at 19,200 symbols per second. The transmitter 102 is configured to transmit the data packets with the most significant bit of byte zero first.

FIG. 6 is a flowchart illustrating the time hopping procedure for the receiver of the continuous glucose monitoring system shown in FIG. 1 in accordance with one embodiment of the present invention.

Referring to FIG. 6, upon completing the power up procedure as discussed above, the receiver 104 listens for the presence of a transmitter within the RF communication link range. At step 601, when the transmitter 102 is detected within the RF communication link range, the receiver 104 is configured to receive and store the identification information corresponding to the detected transmitter 102. Thereafter, at step 602, the receiver 104 is configured to detect (or sample) data transmission within its RF communication range. In one aspect, the receiver 104 is configured to identify a positive data transmission upon ascertaining that the data transmission is above a predetermined strength level for a given period of time (for example, receiving three separate data signals above the predetermined strength level from the transmitter 102 at one minute intervals over a period of five minutes).

At step 603, the receiver 104 is configured to determine whether the detected signals within the RF communication range is transmitted from the transmitter 102 having the transmitter identification information stored in the receiver 104. If it is determined at step 603 that the detected data transmission at step 602 does not originate from the transmitter with the stored transmitter identification information, then the procedure returns to step 602 and waits for the detection of the next data transmission.

On the other hand, if at step 603 it is determined that the detected data transmission is from the transmitter 102 corresponding to the stored transmitter identification information, then at step 604, the receiver proceeds with decoding the received data and performing error correction thereon. In one embodiment, the receiver is configured to perform Reed-Solomon decoding, where the transmitted data received by the receiver is encoded with Reed-Solomon encoding. Furthermore, the receiver is configured to perform forward error correction to minimize data error due to, for example, external noise, transmission noise and so on.

Referring back to FIG. 6, after decoding and error correcting the received data, the receiver 104 at step 605 generates output data corresponding to the decoded error corrected data received from the transmitter 102, and thereafter, at step 606, the receiver 104 outputs the generated output data for the user as a real time display of the output data, or alternatively, in response to the user operation requesting the display of the output data. Additionally, before displaying the output data for the user, other pre-processing procedures may be performed on the output data to for example, smooth out the output signals. In one aspect, the generated output data may include a visual graphical output displayed on the graphical user interface of the receiver. Alternatively, the output data may be numerically displayed representing the corresponding glucose level.

Referring now to FIGS. 4 and 6, the time hopping procedure of one embodiment is described. More specifically, since more than one transmitter 102 may be within the receiving range of a particular receiver 104, and each transmitting data every minute on the same frequency, transmitter units 102 are configured to transmit data packets at different times to avoid

co-location collisions (that is, where one or more receivers **104** cannot discern the data signals transmitted by their respective associated transmitter units **102** because they are transmitting at the same time).

In one aspect, transmitter **102** is configured to transmit once every minute randomly in a window of time of plus or minus 5 seconds (i.e., it time hops.) To conserve power, receiver **104** does not listen for its associated transmitter **102** during the entire 10 second receive window, but only at the predetermined time it knows the data packet will be coming from the corresponding transmitter **102**. In one embodiment, the 10 second window is divided into 400 different time segments of 25 milliseconds each. Before each RF transmission from the transmitter **102** takes place, both the transmitter **102** and the receiver **104** is configured to recognize in which one of the 400 time segments the data transmission will occur (or in which to start, if the transmission time exceeds 25 milliseconds). Accordingly, receiver **104** only listens for a RF transmission in a single 25 millisecond time segment each minute, which varies from minute to minute within the 10 second time window.

Moreover, each transmitter **102** is configured to maintain a "master time" clock that the associated receiver unit **104** may reference to each minute (based on the time of transmission and known offset for that minute). A counter also on the transmitter **102** may be configured to keep track of a value "Tx Time" that increments by 1 each minute, from 0 to 255 and then repeats. This Tx Time value is transmitted in the data packet each minute, shown as Byte **1** in FIG. **4**. Using the Tx Time value and the transmitter's unique identification information (TX ID, shown as Byte **0** in FIG. **4**), both the transmitter **102** and the receiver **104** can calculate which of the 400 time segments will be used for the subsequent transmission. In one embodiment, the function that is used to calculate the offset from the master clock 1-minute tick is a pseudo-random number generator that uses both the Tx Time and the TX ID as seed numbers. Accordingly, the transmission time varies pseudo-randomly within the 10 second window for 256 minutes, and then repeats the same time hopping sequence again for that particular transmitter **102**.

In the manner described above, in accordance with one embodiment of the present invention, co-location collisions may be avoided with the above-described time hopping procedure. That is, in the event that two transmitters interfere with one another during a particular transmission, they are not likely to fall within the same time segment in the following minute. As previously described, three glucose data points are transmitted each minute (one current and two redundant/historical), so collisions or other interference must occur for 3 consecutive data transmissions for data to be lost. In one aspect, when a transmission is missed, the receiver **104** may be configured to successively widen its listening window until normal transmissions from the respective transmitter **102** resume. Under this approach, the transmitter listens for up to 70 seconds when first synchronizing with a transmitter **102** so it is assured of receiving a transmission from transmitter **102** under normal conditions.

Various other modifications and alterations in the structure and method of operation of this invention will be apparent to those skilled in the art without departing from the scope and spirit of the invention. Although the invention has been described in connection with specific preferred embodiments, it should be understood that the invention as claimed should not be unduly limited to such specific embodiments. It is intended that the following claims define the scope of the

present invention and that structures and methods within the scope of these claims and their equivalents be covered thereby.

What is claimed is:

1. An analyte monitoring system, comprising:

a sensor configured to sample one or more analyte levels of interstitial fluid; and

a sensor electronics unit operatively coupled to the sensor, the sensor electronics unit comprising sensor electronics operatively coupled to the sensor and configured to receive the sampled one or more analyte levels, a memory for storing a plurality of data points corresponding to the sampled one or more analyte levels, a processor configured to generate one or more data packets for data communication to a receiver unit via the sensor electronics unit, and a temperature detection unit configured to monitor a temperature of an insertion site of the sensor to obtain a temperature reading, wherein the temperature reading is used to adjust the sampled one or more analyte levels;

wherein the sensor electronics unit includes programming to communicate the generated one or more data packets with each data communication, the one or more data packets including a current data point that corresponds to an analyte level of a current time period and at least one previous data point that corresponds to at least one analyte level of at least one previous time period, such that if the receiver unit does not successfully receive the current data point from the sensor electronics, at a subsequent data communication, the current data point and the at least one previous data point are re-communicated to the receiver unit with a new current data point, and the current data point is received at the receiver unit and ascertained from the subsequent data communication, and to transition from a sleep mode to a communication mode upon activation.

2. The system of claim 1, wherein the sensor electronics unit is operatively coupled to the receiver unit via a communication link prior to communication of the one or more data packets.

3. The system of claim 1, wherein the sensor electronics unit is configured to encode the sampled one or more analyte levels received from the sensor to generate encoded data packets, the sensor electronics unit further configured to communicate the encoded data packets to the receiver unit.

4. The system of claim 3, wherein the receiver unit is configured to decode encoded signals received from the sensor electronics unit.

5. The system of claim 1, wherein the one or more data packets includes data points sampled over a predetermined time period.

6. The system of claim 1, wherein the current data point corresponds to a current analyte level of the interstitial fluid, and wherein the at least one previous data point includes two consecutive analyte levels of the interstitial fluid, said one of the two consecutive analyte levels immediately preceding the current analyte level.

7. The system of claim 1, wherein the receiver unit is configured to receive the one or more data packets, and includes an output unit for outputting data related to the received one or more data packets, wherein the data is related to one or more glucose levels.

8. The system of claim 7, wherein the output unit includes a display unit for displaying data corresponding to the one or more glucose levels.

13

9. The system of claim 8, wherein the display unit includes one of a LCD display, a cathode ray tube display, and a plasma display.

10. The system of claim 8, wherein the displayed data includes one or more of an alphanumeric representation corresponding to the one or more glucose levels, a graphical representation of the one or more glucose levels, and a three-dimensional representation of the one or more glucose levels.

11. The system of claim 8, wherein the display unit is configured to display the data corresponding to the one or more glucose levels in real time.

12. The system of claim 7, wherein the output unit includes a speaker for outputting an audio signal corresponding to the one or more glucose levels.

13. The system of claim 1, wherein the receiver unit is configured to store an identification information corresponding to the sensor electronics unit.

14. The device of claim 1, wherein the sensor electronics unit is encased in a water tight housing.

15. The device of claim 1, wherein the sensor electronics unit includes a disable switch for temporarily disabling the communication of the data packets.

16. An apparatus, comprising:

a sensor electronics unit;

one or more processors operatively coupled to the sensor electronics unit; and

a memory for storing instructions which, when executed by the one or more processors, causes the one or more processors to receive one or more analyte levels sampled by a sensor, to storing a plurality of data points corresponding to the sampled one or more analyte levels in a memory, to generate one or more data packets for data communication to a receiver unit, to monitor a temperature of an insertion site of the sensor to obtain a temperature reading, wherein the temperature reading is

14

used to adjust the sampled one or more analyte levels, to communicate the generated one or more data packets to the receiver unit with each communication, the one or more data packets including a current data point that corresponds to an analyte level of a current time period and at least one previous data point that corresponds to at least one analyte level of at least one previous time period, such that if the receiver unit does not successfully receive the current data point from the sensor electronics, at a subsequent data communication, the current data point and the at least one previous data point are re-communicated to the receiver unit with a new current data point, and the current data point is received at the receiver unit and ascertained from the subsequent data communication, and to transition from a sleep mode to a communication mode upon activation.

17. The apparatus of claim 16, wherein the sensor electronics unit is operatively coupled to the receiver unit via a communication link prior to communication of the one or more data packets.

18. The apparatus of claim 16, wherein the memory for storing instructions which, when executed by the one or more processors, causes the one or more processors configured to encode the sampled one or more analyte levels received from the sensor to generate encoded data packets and to communicate the encoded data packets to the receiver unit.

19. The apparatus of claim 16, wherein the one or more data packets includes data points sampled over a predetermined time period.

20. The apparatus of claim 16, wherein the current data point corresponds to a current analyte level, and wherein the at least one previous data point includes two consecutive analyte levels, said one of the two consecutive analyte levels immediately preceding the current analyte level.

* * * * *

专利名称(译)	连续血糖监测系统和使用方法		
公开(公告)号	US8622903	公开(公告)日	2014-01-07
申请号	US13/481256	申请日	2012-05-25
[标]申请(专利权)人(译)	雅培糖尿病护理公司		
申请(专利权)人(译)	雅培糖尿病INC.		
当前申请(专利权)人(译)	雅培糖尿病INC.		
[标]发明人	JIN ROBERT Y SLOAN MARK K		
发明人	JIN, ROBERT Y. SLOAN, MARK K.		
IPC分类号	A61B5/00		
CPC分类号	A61B2562/08 A61B5/14532 A61B5/0002 A61B5/01		
优先权	60/437374 2002-12-31 US		
其他公开文献	US20120232368A1		
外部链接	Espacenet USPTO		

摘要(译)

一种连续血糖监测系统，包括配置成检测一个或多个葡萄糖水平的传感器，可操作地耦合到传感器的发射器，发射器配置成接收检测到的一个或多个葡萄糖水平，发射器还配置成发送与检测到的一个相对应的信号。本发明公开了一种或多种葡萄糖水平，以及可操作地耦合到发射器的接收器，其配置成接收对应于检测到的一种或多种葡萄糖水平的发射信号，及其方法。在一个方面，发射器可以被配置为发送当前数据点和至少一个先前数据点，当前数据点和至少一个先前数据点对应于检测到的一个或多个葡萄糖水平。

