



US008287531B2

(12) **United States Patent**  
**Mest**

(10) **Patent No.:** **US 8,287,531 B2**  
(45) **Date of Patent:** **\*Oct. 16, 2012**

(54) **CATHETER WITH ABLATION NEEDLE AND MAPPING ASSEMBLY**

(75) Inventor: **Robert A. Mest**, Long Beach, CA (US)

(73) Assignee: **Biosense Webster, Inc.**, Diamond Bar, CA (US)

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 1112 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **12/140,996**

(22) Filed: **Jun. 17, 2008**

(65) **Prior Publication Data**

US 2008/0249392 A1 Oct. 9, 2008

**Related U.S. Application Data**

(63) Continuation of application No. 11/322,603, filed on Dec. 30, 2005, now Pat. No. 7,387,630, which is a continuation of application No. 10/693,553, filed on Oct. 24, 2003, now Pat. No. 7,179,256.

(51) **Int. Cl.**

**A61B 18/14** (2006.01)

**A61F 2/00** (2006.01)

(52) **U.S. Cl.** ..... 606/41; 607/101

(58) **Field of Classification Search** ..... 606/42, 606/41; 607/101

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

5,551,426 A 9/1996 Hummel et al.  
5,702,438 A 12/1997 Avitall  
5,782,239 A 7/1998 Webster, Jr.

5,782,889 A 7/1998 Hognelid et al.  
5,800,484 A 9/1998 Gough et al.  
5,938,694 A 8/1999 Jaraczewski et al.  
6,014,579 A 1/2000 Pomeranz et al.

(Continued)

**FOREIGN PATENT DOCUMENTS**

EP 1 205 156 A2 5/2002

(Continued)

**OTHER PUBLICATIONS**

EPO Search Report dated Jan. 31, 2005 for European Patent Application No. 04256538.1.

*Primary Examiner* — Roy Gibson


*Assistant Examiner* — Jared W Pike

(74) *Attorney, Agent, or Firm* — Christie, Parker & Hale, LLP

(57) **ABSTRACT**

The invention is directed to a catheter that creates enhanced lesions using a needle electrode and can simultaneously map electrical activity at a plurality of points using an enhanced mapping assembly. The catheter comprises an elongated catheter body having at least one lumen extending longitudinally therethrough. A needle control handle is provided at the proximal end of the catheter body. A needle electrode assembly extends through the catheter body and needle control handle and has a proximal end attached to the needle control handle and a distal end within the distal end of the catheter body. A mapping assembly is mounted at the distal end of the catheter body and comprises at least two flexible spines. Each spine has a proximal end attached at the distal end of the catheter body and a free distal end. Each spine carries at least one electrode. The distal end of the needle electrode assembly is extendable past the proximal end of the mapping assembly upon manipulation of the needle control handle.

**20 Claims, 11 Drawing Sheets**

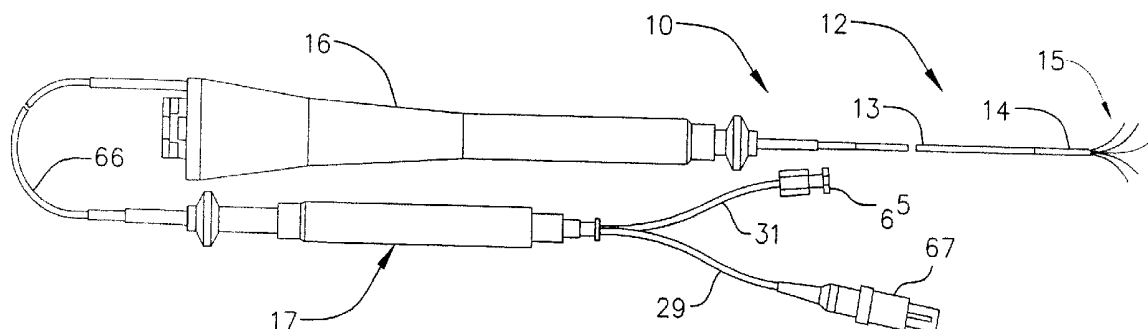

# US 8,287,531 B2

Page 2

## U.S. PATENT DOCUMENTS

6,053,937 A 4/2000 Edwards et al.  
6,286,512 B1 9/2001 Loeb et al.  
6,330,478 B1 12/2001 Lee et al.  
6,574,492 B1 \* 6/2003 Ben-Haim et al. .... 600/374  
6,748,255 B2 6/2004 Fuimaono et al.  
6,961,602 B2 11/2005 Fuimaono et al.  
7,179,256 B2 \* 2/2007 Mest ..... 606/41  
7,387,630 B2 \* 6/2008 Mest ..... 606/41  
2003/0010987 A1 1/2003 Banin et al.  
2003/0109871 A1 6/2003 Johnson et al.


2003/0125614 A1 \* 7/2003 Fuimaono et al. .... 600/374  
2004/0044277 A1 3/2004 Fuimaono et al.  
2004/0087848 A1 5/2004 Mejia  
2005/0090729 A1 4/2005 Solis et al.  
2006/0106377 A1 5/2006 Mest

## FOREIGN PATENT DOCUMENTS

EP 1297796 4/2003  
WO WO 02/054941 7/2002


\* cited by examiner

FIG. 1

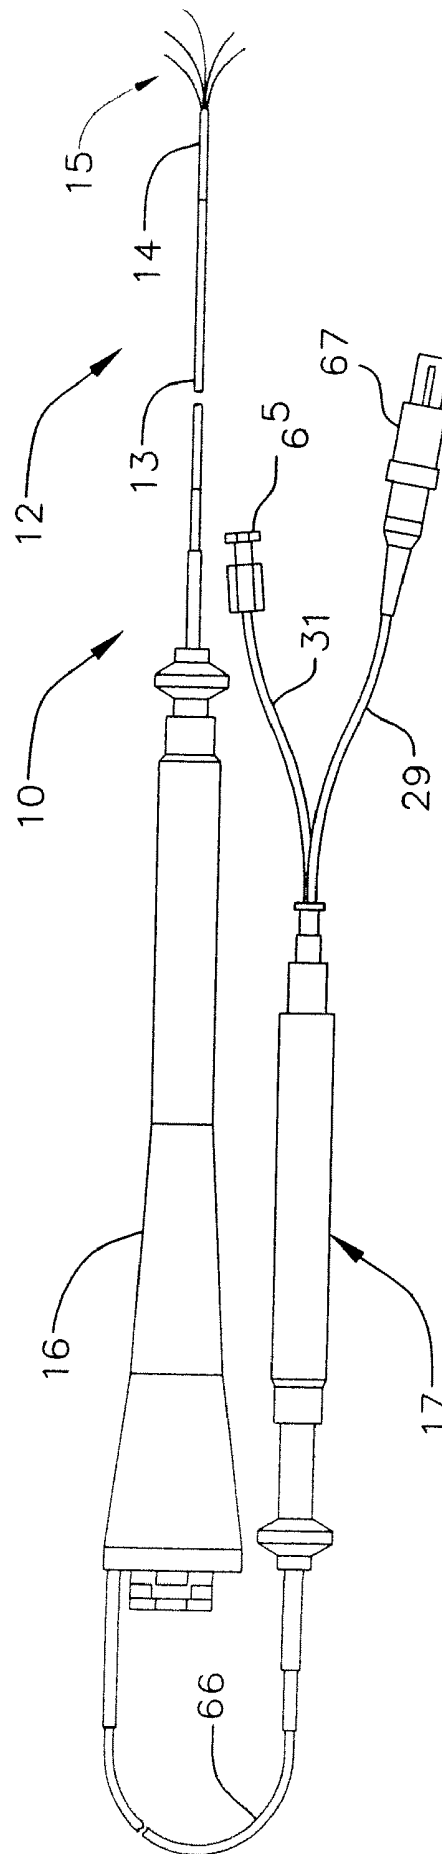




**FIG. 2B**  
(AREA B)

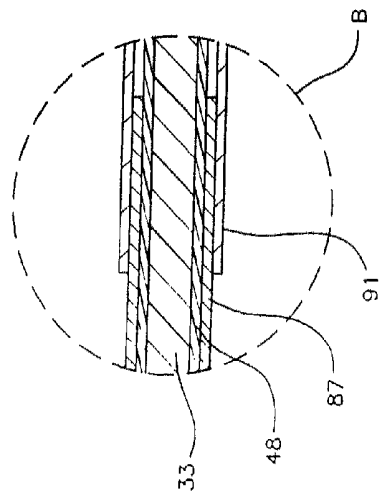

**FIG. 2A**  
(AREA A)

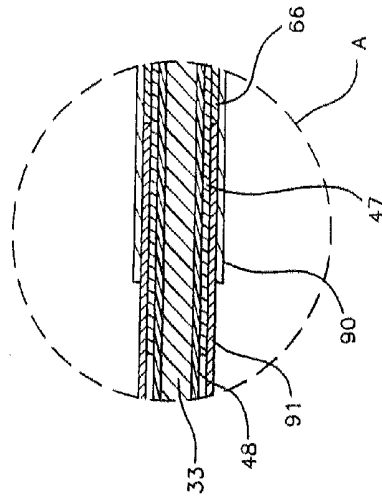

**FIG. 2C**  
(AREA C)


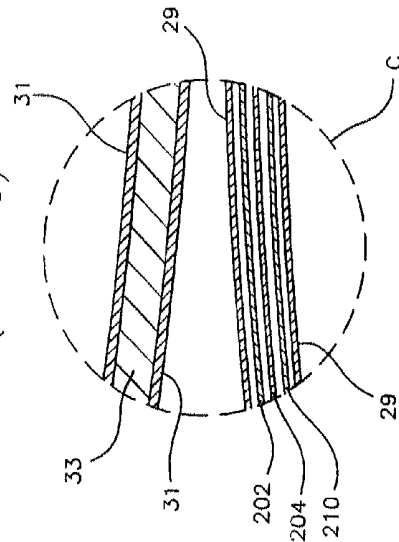


FIG. 3







*FIG. 4*

FIG. 5

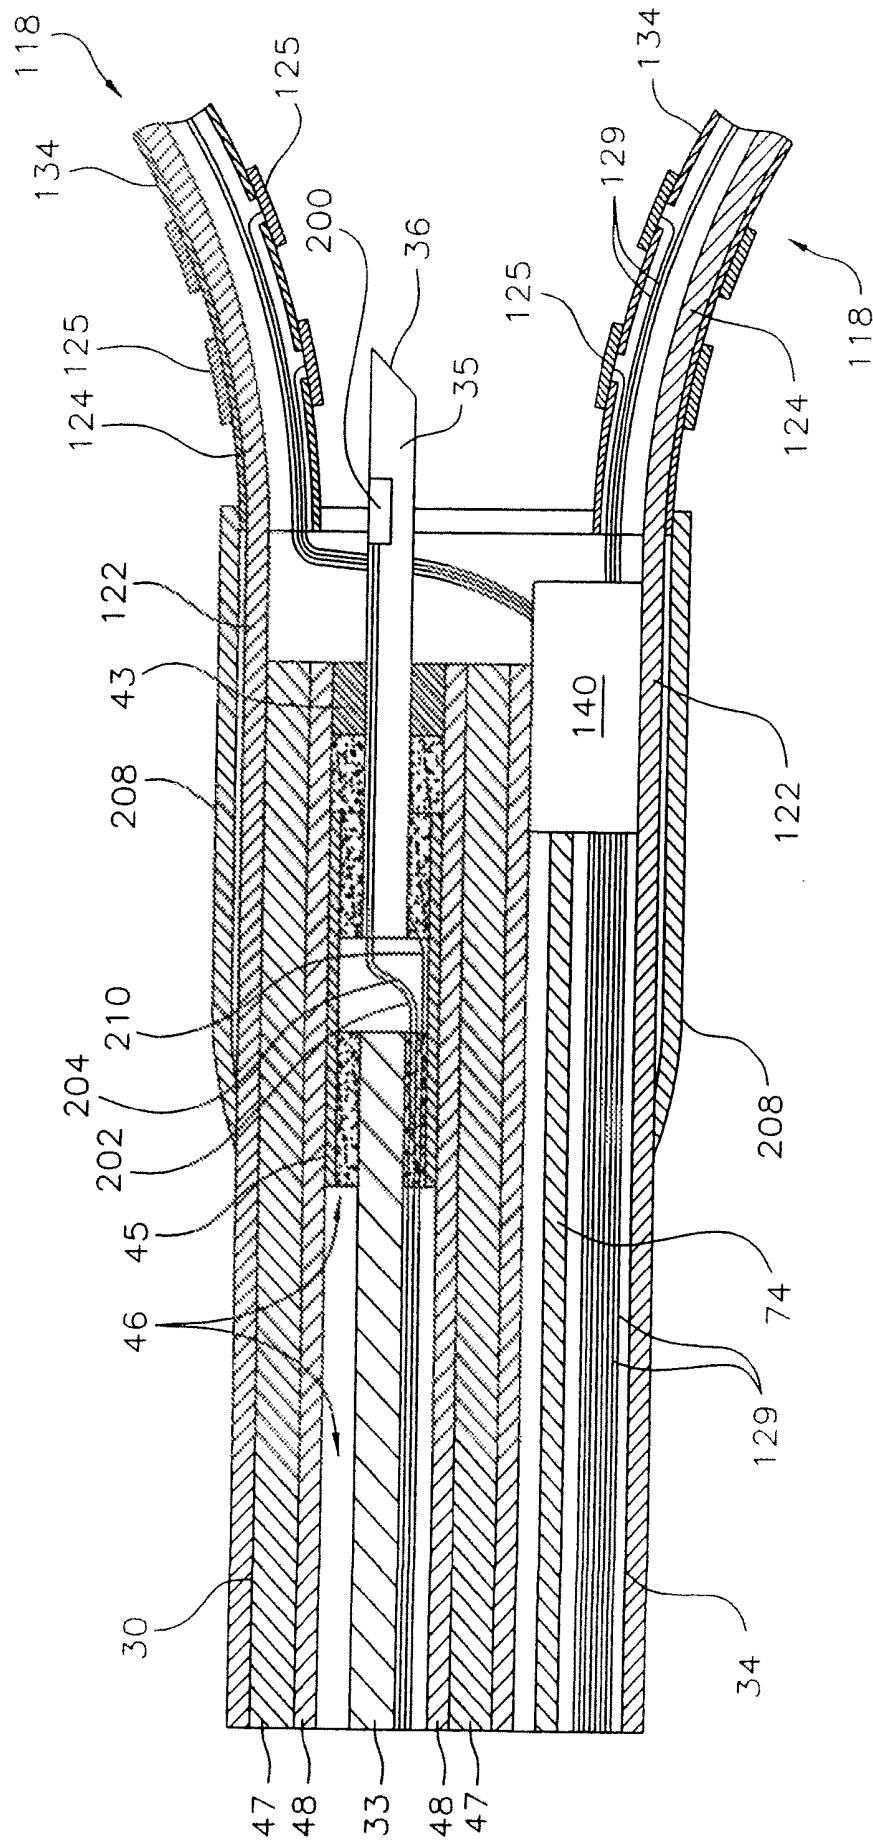



*FIG. 6*

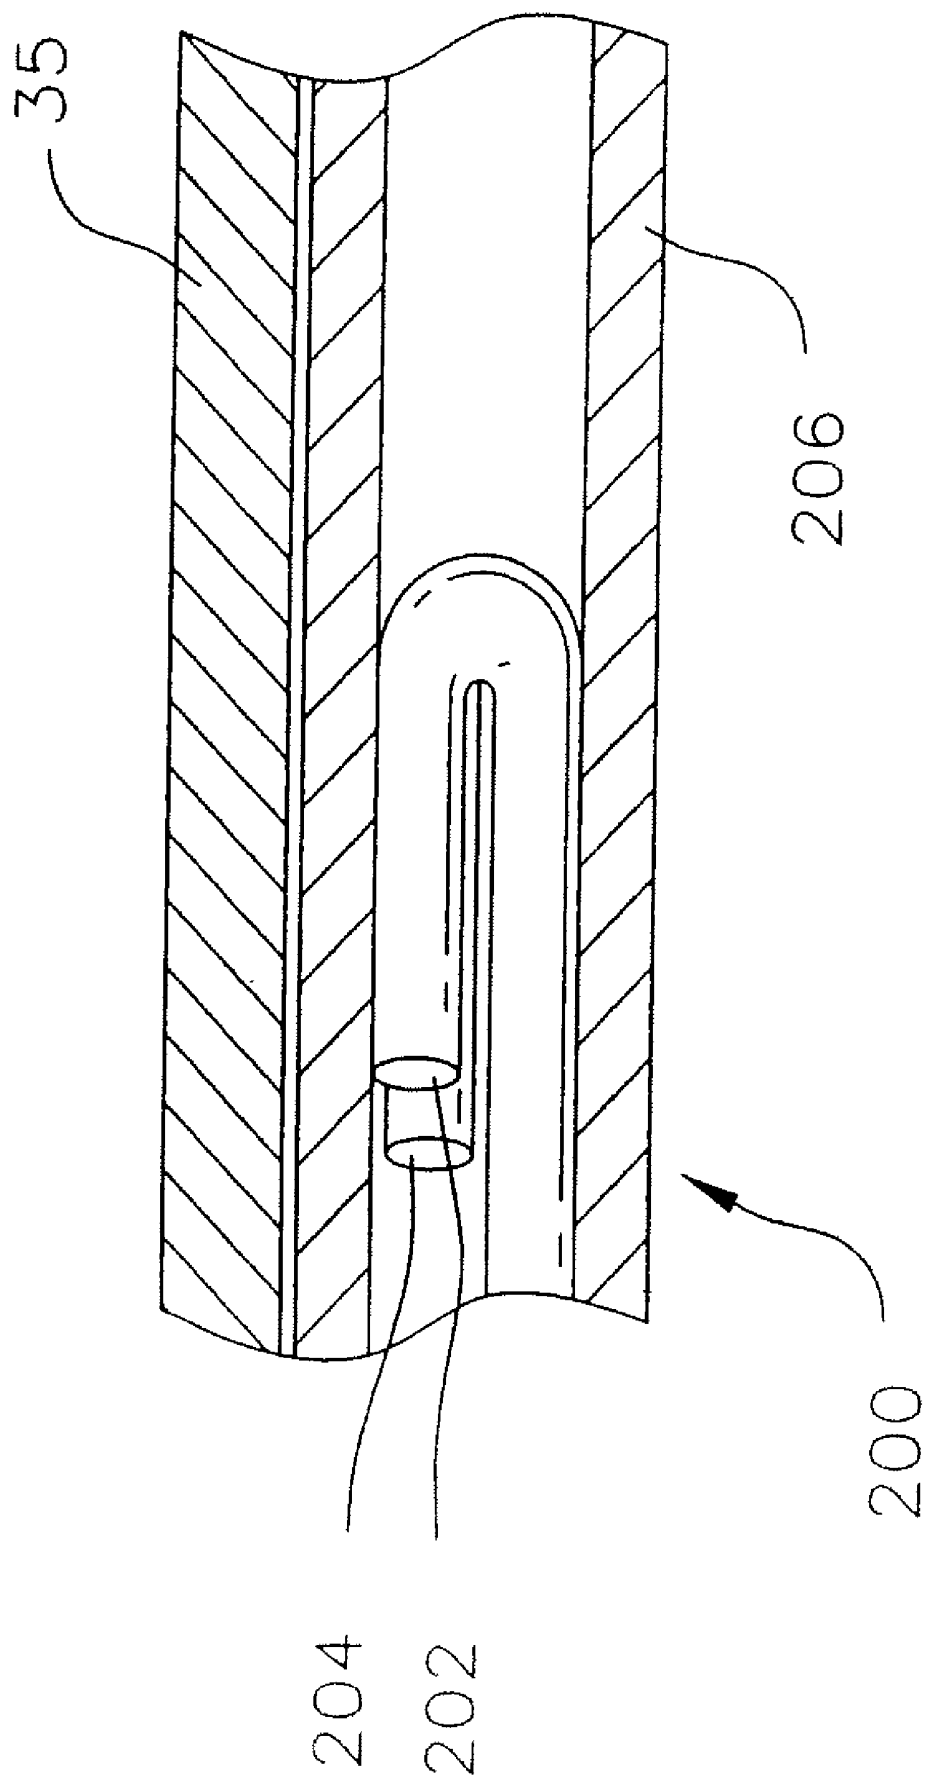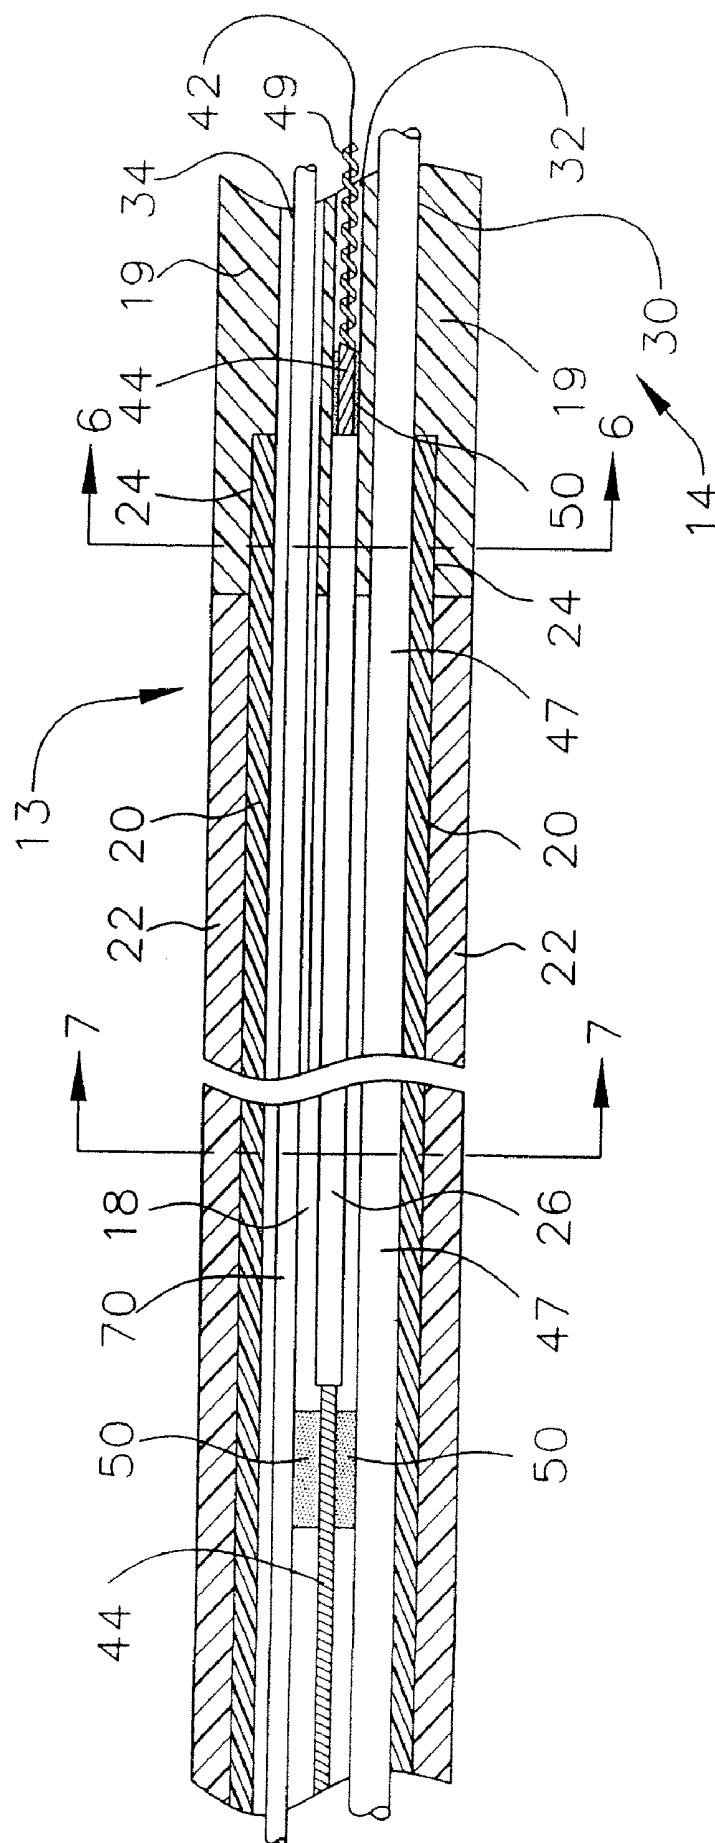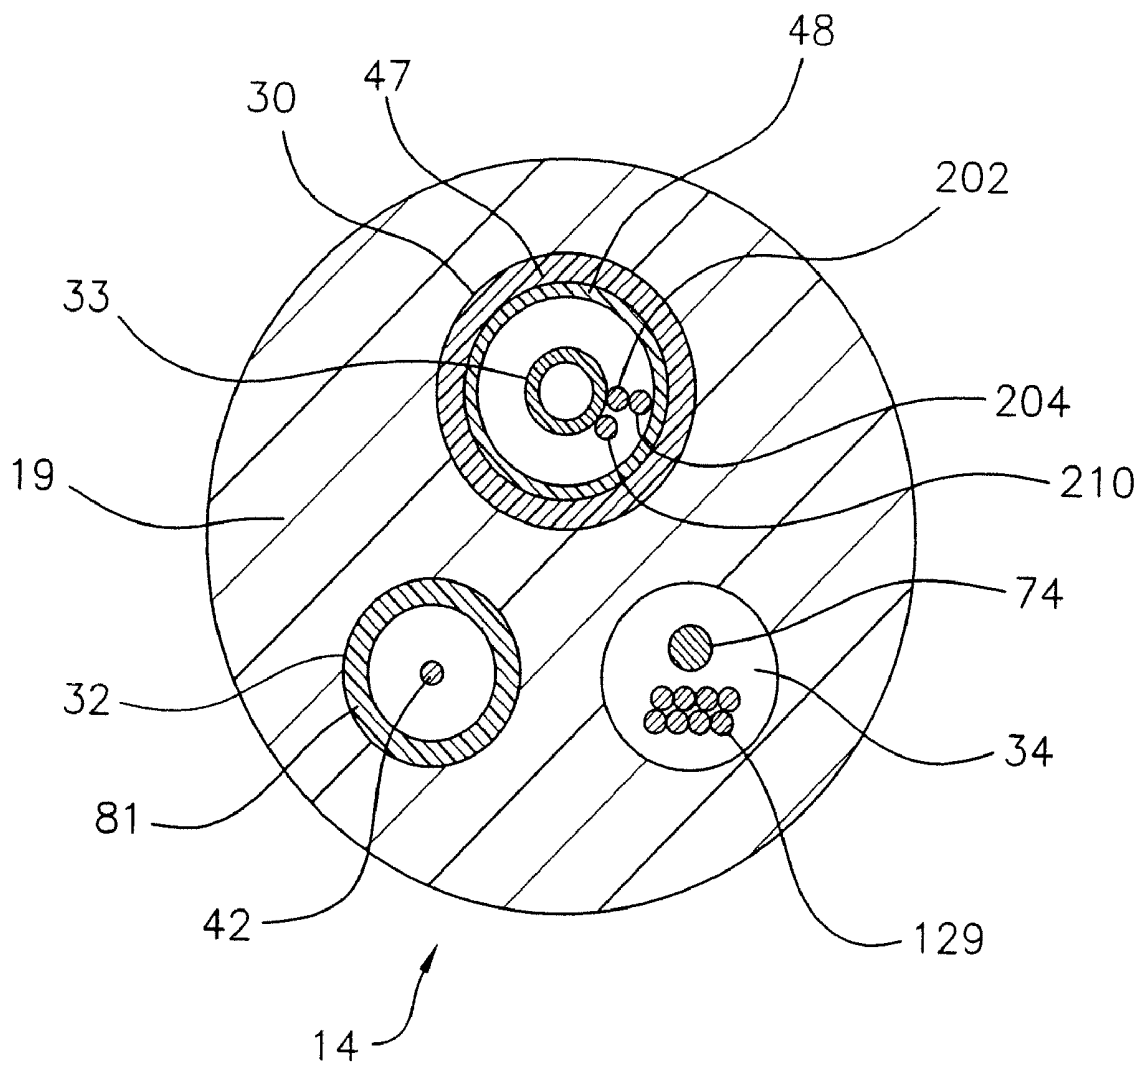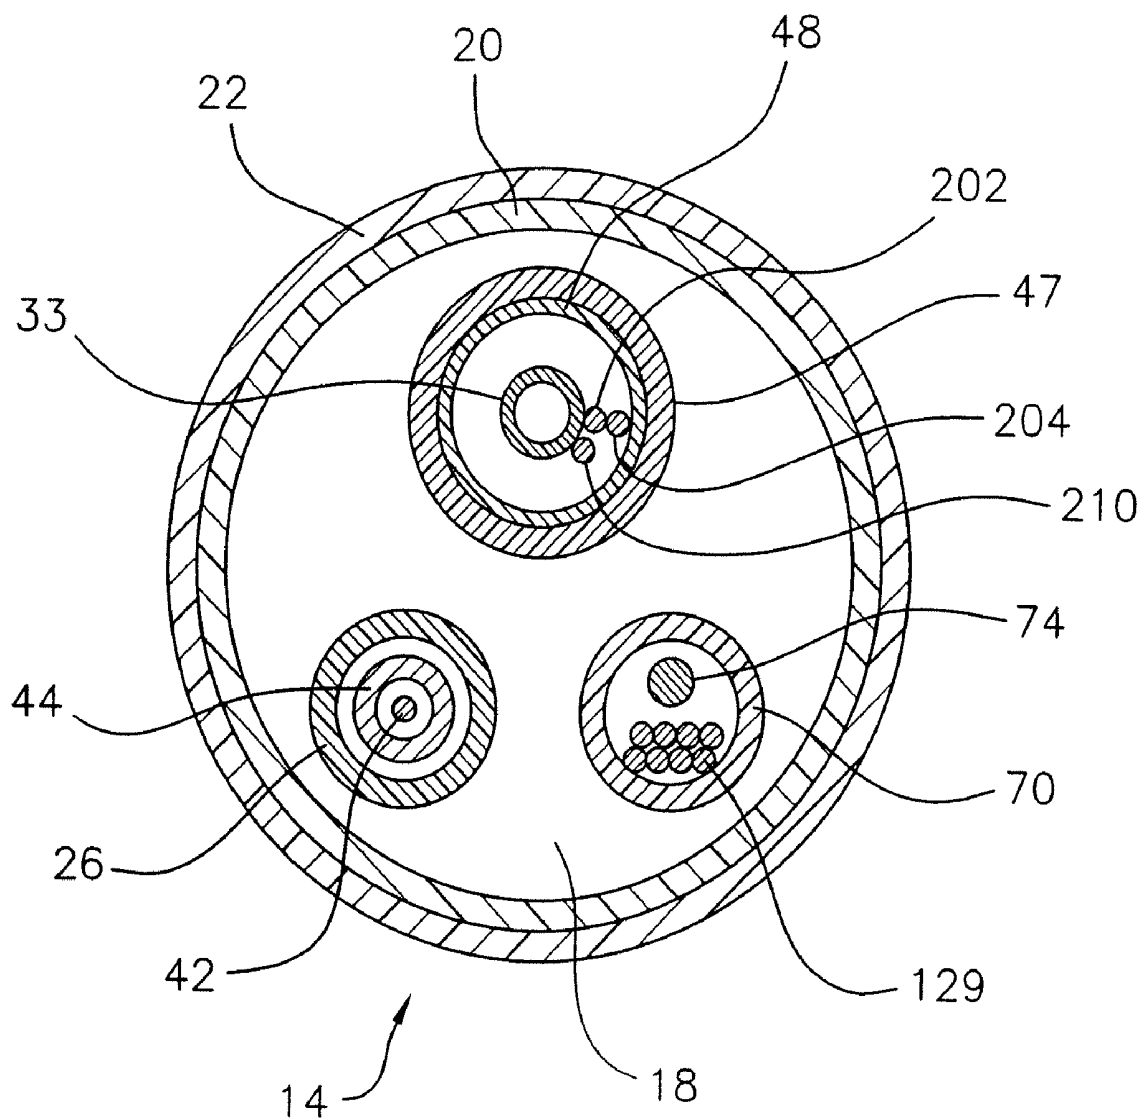*FIG. 7*

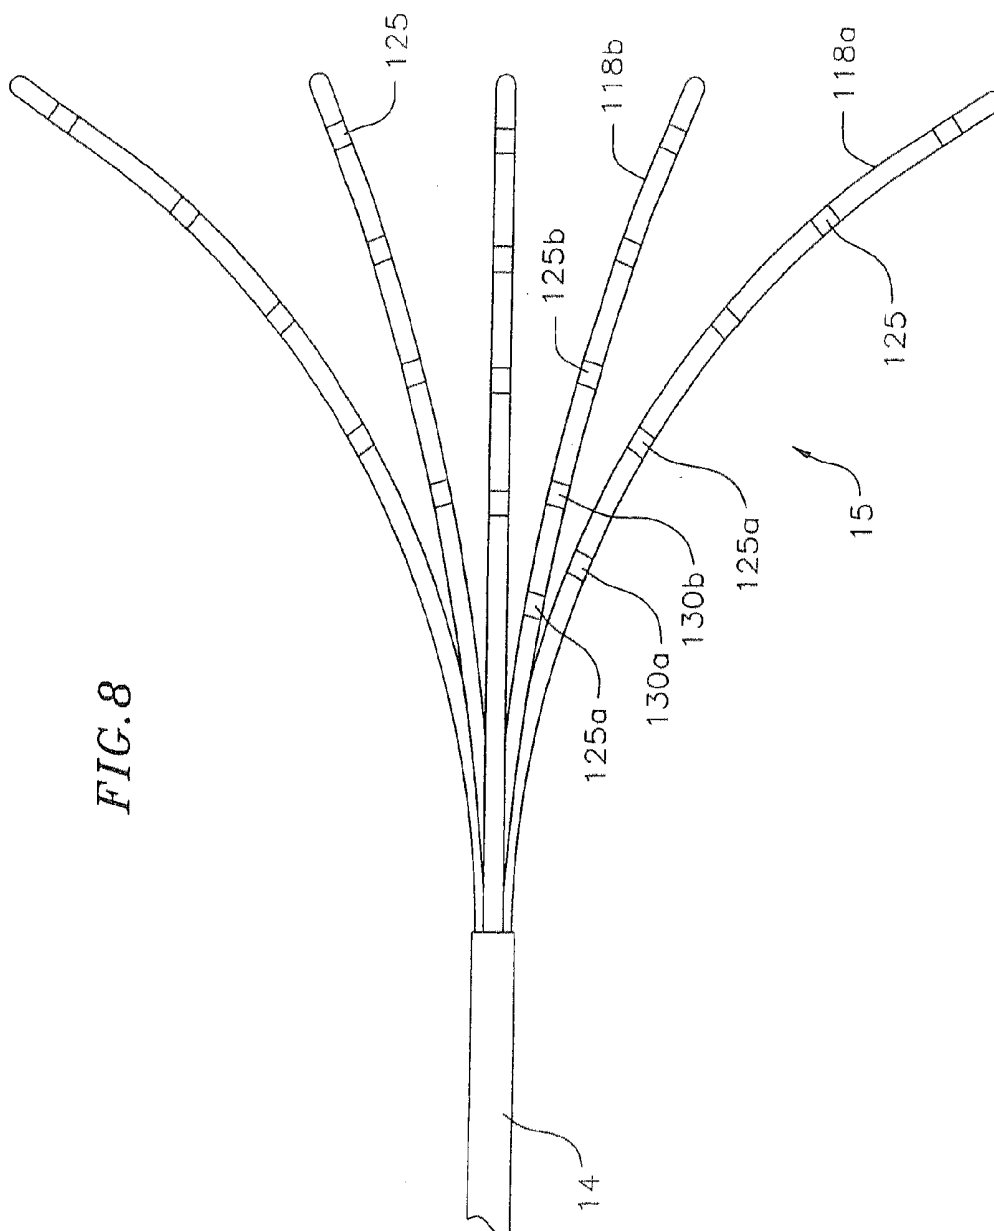


FIG. 9

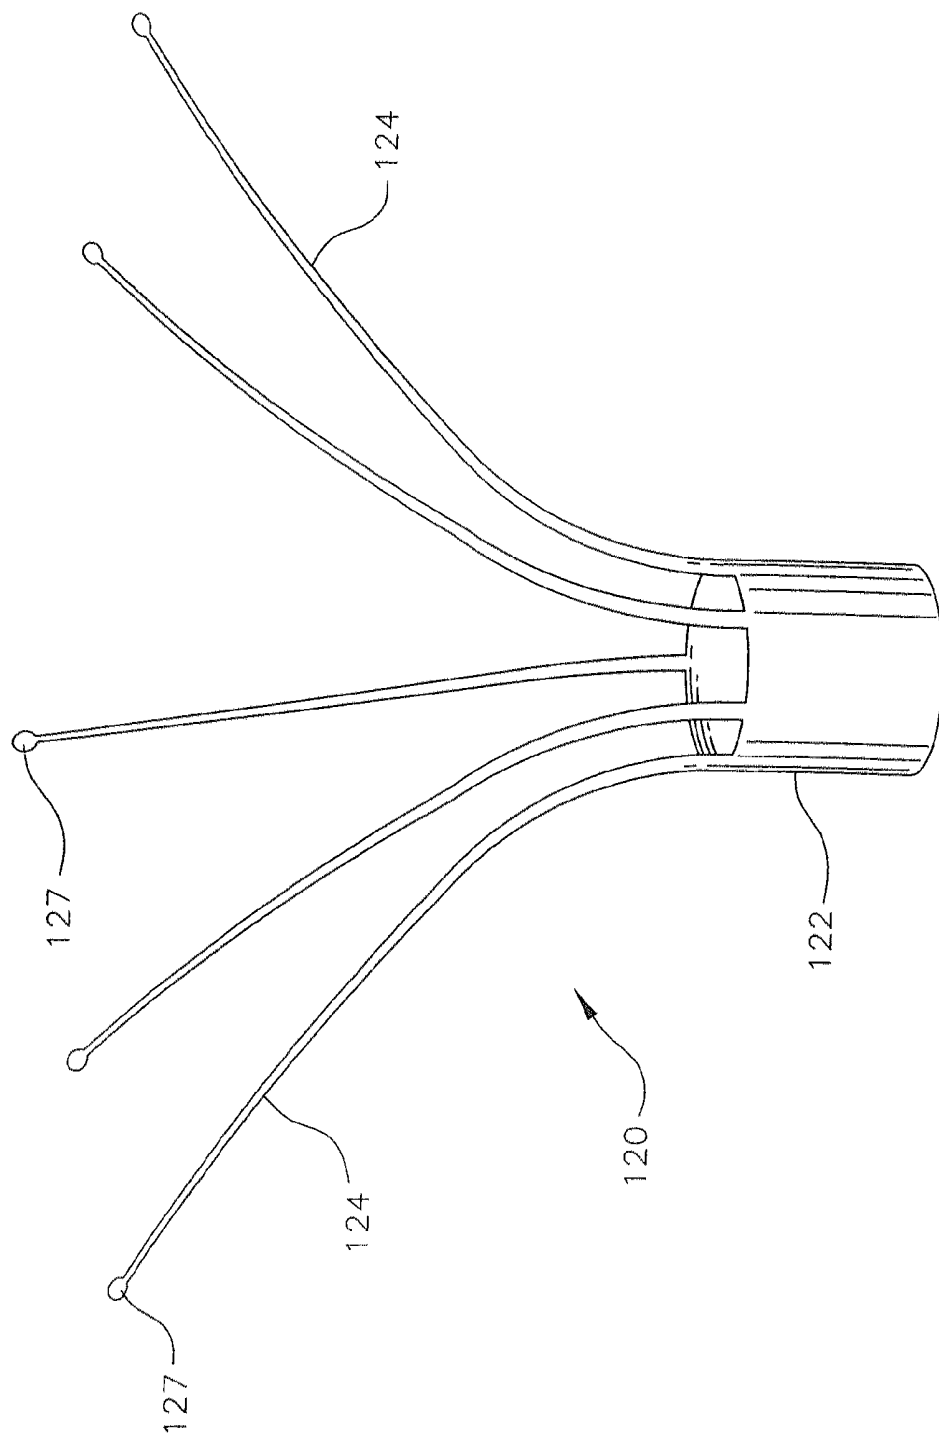


FIG. 10

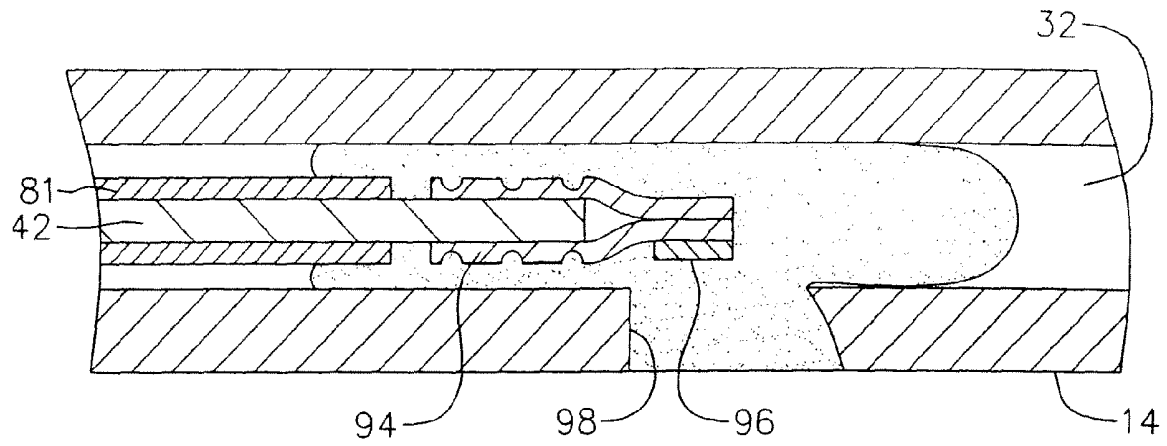


FIG. 11


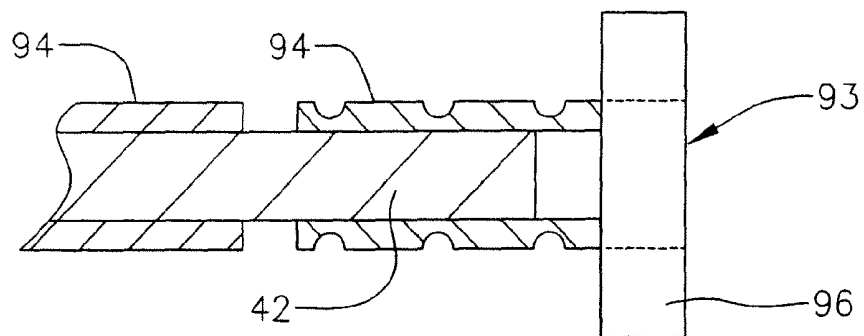


FIG. 12

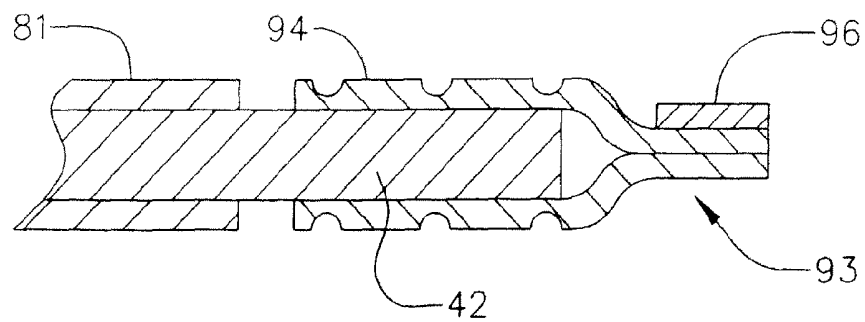

# CATHETER WITH ABLATION NEEDLE AND MAPPING ASSEMBLY

## CROSS-REFERENCE TO RELATED APPLICATION(S)

This application is a continuation of U.S. patent application Ser. No. 11/322,603, entitled CATHETER WITH ABLATION NEEDLE AND MAPPING ASSEMBLY, filed on Dec. 30, 2005, now U.S. Pat. No. 7,387,630 which is a continuation of U.S. patent application Ser. No. 10/693,553, entitled CATHETER WITH ABLATION NEEDLE AND MAPPING ASSEMBLY, filed Oct. 24, 2003, now U.S. Pat. No. 7,179,256 the entire contents of which is incorporated herein by reference.

## BACKGROUND OF THE INVENTION

Radiofrequency (RF) ablation of cardiac and other tissue is a well known method for creating thermal injury lesions at the tip of an electrode. Radiofrequency current is delivered between a skin (ground) patch and the electrode. Electrical resistance at the electrode-tissue interface results in direct resistive heating of a small area, the size of which depends upon the size of the electrode, electrode tissue contact, and current (density). See Avitall B, Helms R. Determinants of Radiofrequency-Induced Lesion Size in Huang S K S, Wilber D J (eds.): Radiofrequency Catheter Ablation of Cardiac Arrhythmias: Basic Concepts and Clinical Applications, 2<sup>nd</sup> ed. Armonk, N.Y., Futura Publishing Company, Inc., 2000: 47-80. Further tissue heating results from conduction of heat within the tissue to a larger zone. Tissue heated beyond a threshold of approximately 50-55° C. is irreversibly injured (ablated). See Nath S, and Haines D E. Pathophysiology of Lesion Formation by Radiofrequency Catheter Ablation, in Huang S K S, Wilber D J (eds.): Radiofrequency Catheter Ablation of Cardiac Arrhythmias: Basic Concepts and Clinical Applications, 2<sup>nd</sup> ed. Armonk, N.Y., Futura Publishing Company, Inc., 2000:26-28.

Resistive heating is caused by energy absorption due to electrical resistance. Energy absorption is related to the square of current density and inversely with tissue conductivity. Current density varies with conductivity and voltage and inversely with the square of radius from the ablating electrode. Therefore, energy absorption varies with conductivity, the square of applied voltage, and inversely with the fourth power of radius from the electrode. Resistive heating, therefore, is most heavily influenced by radius, and penetrates a very small distance from the ablating electrode. The rest of the lesion is created by thermal conduction from the area of resistive heating. See Lin J, Physical Aspects of Radiofrequency Ablation, in Huang S K S, Wilber D J (eds.): Radiofrequency Catheter Ablation of Cardiac Arrhythmias: Basic Concepts and Clinical Applications, 2<sup>nd</sup> ed. Armonk, N.Y., Futura Publishing Company, Inc., 2000:14-17. This imposes a limit on the size of ablation lesions that can be delivered from a surface electrode.

Theoretical methods to increase lesion size would include increasing electrode diameter, increasing the area of electrode contact with tissue, increasing tissue conductivity and penetrating the tissue to achieve greater depth and increase the area of contact, and delivering RF until maximal lesion size has been achieved (60-90 seconds for full maturation).

The electrode can be introduced to the tissue of interest directly (for superficial/skin structures), surgically, endoscopically, laparoscopically or using percutaneous transvascular (catheter-based) access. Catheter ablation is a well-

described and commonly performed method by which many cardiac arrhythmias are treated. See Miller J M, Zipes D P. Management of the Patient with Cardiac Arrhythmias. In Braunwald E, Zipes D, Libby P (eds): Heart Disease: A Textbook of Cardiovascular Medicine, 6<sup>th</sup> Ed. Philadelphia, Pa., W.B. Saunders Company, 2001: p742-752. Needle electrodes have been described for percutaneous or endoscopic ablation of solid-organ tumours, lung tumours, and abnormal neurologic structures. See, for example, McGahan J P, Schneider P, Brock J M, Tesluk H. Treatment of Liver Tumors by Percutaneous Radiofrequency Electrocautery. Seminars in Interventional Radiology 1993; 10:143-149; Rossi S, Fomari F, Buscarini L. Percutaneous Ultrasound-Guided Radiofrequency Electrocautery for the Treatment of Small Hepatocellular Carcinoma. J Intervent Radiol 1993; 8:97-103; and Livraghi T, Goldberg S N, Lazzaroni S, Meloni F, Monti F, Solbiati L. Saline-enhanced RF tissue ablation in the treatment of liver Metastases. Radiology 1995; 197(P):140 (abstr)].

Catheter ablation is sometimes limited by insufficient lesion size. See de Bakker J M T, van Capelle F J L, Janse M J et al. Macroreentry in the infarcted human heart: mechanism of ventricular tachycardias with a "focal" activation pattern. J Am Coll Cardiol 1991; 18:1005-1014; Kaltenbrunner W, Cardinal R, Dubuc M et al. Epicardial and endocardial mapping of ventricular tachycardia in patients with myocardial infarction. Is the origin of the tachycardia always subendocardially localized? Circulation 1991; 84:1058-1071. Stevenson W G, Friedman P L, Sager P T et al. Exploring postinfarction reentrant ventricular tachycardia with entrainment mapping. J Am coll Cardiol 1997; 29:1180-1189. Ablation of tissue from an endovascular approach results not only in heating of tissue, but of heating of the electrode. When the electrode reaches critical temperatures, denaturation of blood proteins causes coagulum formation. Impedance can then rise and limit current delivery. Within tissue, overheating can cause evaporation of tissue or blood water and steam bubble formation (steam "pops") with risk of uncontrolled tissue destruction or undesirable perforation of bodily structures. In cardiac ablation, clinical success is sometimes hampered by inadequate lesion depth and transverse diameter even when using catheters with active cooling of the tip. See Soejima K, Delacretaz E, Suzuki M et al. Saline-cooled versus standard radiofrequency catheter ablation for infarct-related ventricular tachycardias. Circulation 2001; 103:1858-1862. Theoretical solutions have included increasing the electrode size (increasing contact surface and increasing convective cooling by blood flow), improving electrode-tissue contact, actively cooling the electrode with fluid infusion, changing the material composition of the electrode to improve current delivery to tissue, and pulsing current delivery to allow intermittent cooling.

Needle electrodes improve contact with tissue and allow deep penetration of current delivery to areas of interest. Ablation may still be hampered by the small surface area of the needle electrode such that heating occurs at low power, and small lesions are created.

Additionally, it is desirable to map the electrical activity in the heart before, during or after ablation. If the mapping can be performed with the same catheter used for ablation, the user avoids the need for catheter exchange. Moreover, it is desirable to include a mapping assembly on the catheter comprising a plurality of electrodes that can be used to simultaneously map electrical activity at different positions within the heart to provide more efficient mapping.

## SUMMARY OF THE INVENTION

The present invention addresses the above concerns by providing a catheter that creates enhanced lesions using a

needle electrode and can simultaneously map electrical activity at a plurality of points using an enhanced mapping assembly. The catheter comprises an elongated catheter body having at least one lumen extending longitudinally therethrough. A needle control handle is provided at the proximal end of the catheter body. A needle electrode assembly extends through the catheter body and needle control handle and has a proximal end attached to the needle control handle and a distal end within the distal end of the catheter body. A mapping assembly is mounted at the distal end of the catheter body and comprises at least two flexible spines. Each spine has a proximal end attached at the distal end of the catheter body and a free distal end. Each spine carries at least one electrode. The distal end of the needle electrode assembly is extendable past the proximal end of the mapping assembly upon manipulation of the needle control handle.

#### BRIEF DESCRIPTION OF THE DRAWINGS

These and other features and advantages of the present invention will be better understood by reference to the following detailed description when considered in conjunction with the accompanying drawings wherein:

FIG. 1 is a side plan view of an embodiment of a catheter of the present invention.

FIG. 2 is a side cross-sectional view of the needle control handle where the needle electrode assembly is in a retracted position.

FIG. 2A is an enlarged close-up view of Area A in FIG. 2.

FIG. 2B is an enlarged close-up view of Area B in FIG. 2.

FIG. 2C is an enlarged close-up view of Area C in FIG. 2.

FIG. 3 is a schematic side cross-sectional view of the distal end of the distal shaft, including the proximal end of the mapping assembly.

FIG. 4 is a side cross-sectional view of the thermocouple mounted in the needle electrode assembly.

FIG. 5 is a side cross-sectional view of the catheter body, including the junction between the proximal shaft and the distal shaft.

FIG. 6 is an end cross-sectional view of the distal shaft of the catheter body shown in FIG. 5 along line 6-6.

FIG. 7 is an end cross-sectional view of the proximal shaft of the catheter body shown in FIG. 5 along line 7-7.

FIG. 8 is a side view of a mapping assembly according to the invention.

FIG. 9 is a perspective view of a support structure according to the present invention.

FIG. 10 is a side cross sectional view of a portion of the catheter tip section showing one means for attaching the puller wire.

FIG. 11 is a top cross sectional views of a preferred puller wire anchor.

FIG. 12 is a side cross sectional views of the puller wire anchor of FIG. 11.

#### DETAILED DESCRIPTION OF THE INVENTION

As shown in FIG. 1, the catheter 10 comprises an elongated catheter body 12 having a proximal shaft 13 and a distal shaft 14, a mapping assembly 15 mounted at the distal end of the distal shaft, a deflection control handle 16 attached to the proximal end of the proximal shaft, and a needle control handle 17 attached indirectly to the catheter body proximal to the deflection control handle.

With reference to FIGS. 5 and 7, the proximal shaft 13 comprises a single, central or axial lumen 18. The proximal shaft 13 is flexible, i.e., bendable, but substantially non-com-

pressible along its length. The proximal shaft 13 may be of any suitable construction and made of any suitable material. A presently preferred construction comprises an outer wall 22 made of polyurethane or nylon. The outer wall 22 comprises an imbedded braided mesh of stainless steel or the like to increase torsional stiffness of the proximal shaft 13 so that, when the deflection control handle 16 is rotated, the distal shaft 14 of the catheter 10 will rotate in a corresponding manner.

The outer diameter of the proximal shaft 13 is not critical, but is preferably no more than about 8 French. Likewise the thickness of the outer wall 22 is not critical. In the depicted embodiment, the inner surface of the outer wall 22 is lined with a stiffening tube 20, which can be made of any suitable material, preferably polyimide. The stiffening tube 20, along with the braided outer wall 22, provides improved torsional stability while at the same time minimizing the wall thickness of the catheter, thus maximizing the diameter of the single lumen. The outer diameter of the stiffening tube 20 is about the same as or slightly smaller than the inner diameter of the outer wall 22.

As shown in FIGS. 5 and 6, the distal shaft 14 comprises a short section of tubing 19 having three lumens, namely an infusion lumen 30, a puller wire lumen 32 and a lead wire lumen 34. The tubing 19 is made of a suitable non-toxic material that is preferably more flexible than the proximal shaft 13. A presently preferred material for the tubing 19 is braided polyurethane, i.e., polyurethane with an embedded mesh of braided stainless steel or the like. The outer diameter of the distal shaft 14, like that of the proximal shaft 13, is preferably no greater than about 8 French.

A preferred means for attaching the proximal shaft 13 to the distal shaft 14 is illustrated in FIG. 5. The proximal end of the distal shaft 14 comprises an inner counter bore 24 that receives the outer surface of the stiffener 20. The distal shaft 14 and proximal shaft 13 are attached by glue or the like. Other methods for attaching the proximal shaft 13 to the distal shaft 14 can be used in accordance with the invention.

The stiffening tube 20 is held in place relative to the outer wall 22 at the proximal shaft 13. In a preferred construction of the proximal shaft 13, a force is applied to the proximal end of the stiffening tube 20, which causes the distal end of the stiffening tube 20 to firmly push against the counter bore 24. While under compression, a first glue joint is made between the stiffening tube 20 and the outer wall 22 by a fast drying glue, e.g. Super Glue®. Thereafter a second glue joint is formed between the proximal ends of the stiffening tube 20 and outer wall 22 using a slower drying but stronger glue, e.g., polyurethane.

The depicted catheter includes a mechanism for deflecting the distal shaft 14 of the catheter body 12. In the depicted embodiment, a puller wire 42 extends into the puller wire lumen 32 of the distal shaft 14. The puller wire 42 is anchored at its proximal end to the deflection control handle 16 and anchored at its distal end to the distal shaft 14. The puller wire 42 is made of any suitable metal, such as stainless steel or Nitinol, and is preferably coated with Teflon® or the like. The coating imparts lubricity to the puller wire 42. The puller wire 42 preferably has a diameter ranging from about 0.006 to about 0.010 inches.

Referring to FIG. 5, the compression coil 44 extends from the proximal end of the proximal shaft 13 to the proximal end of the distal shaft 14. The compression coil 44 is made of any suitable metal, preferably stainless steel. The compression coil 44 is tightly wound on itself to provide flexibility, i.e., bending, but to resist compression. The inner diameter of the compression coil 44 is preferably slightly larger than the

diameter of the puller wire **42**. For example, when the puller wire **42** has a diameter of about 0.007 inches, the compression coil **44** preferably has an inner diameter of about 0.008 inches. The Teflon® coating on the puller wire **42** allows it to slide freely within the compression coil **44**. Along its length, the outer surface of the compression coil **44** is covered by a flexible, non-conductive sheath **26** to prevent contact between the compression coil **44** and any of the lead wires **129** or needle electrode assembly **46**. A non-conductive sheath **26** made of polyimide tubing is presently preferred. As shown in FIG. 5, the compression coil **44** is anchored at its proximal end to the proximal end of the stiffening tube **20** in the proximal shaft **13** by glue to form a glue joint **50** and at its distal end to the distal shaft **14** in the puller wire lumen **32**.

The puller wire **42** extends into the puller wire lumen **32** of the distal shaft **14**. Preferably the puller wire **42** is anchored at its distal end to the side of the distal shaft **14**, as shown in FIGS. 10 to 12. In this embodiment, a T-shaped anchor **93** is formed which comprises a short piece of tubular stainless steel **94**, e.g., hypodermic stock, which is fitted over the distal end of the puller wire **42** and crimped to fixedly secure it to the puller wire. The distal end of the tubular stainless steel **94** is fixedly attached, e.g., by welding, to a stainless steel cross-piece **96**, such as stainless steel ribbon or the like. The cross-piece **96** sits in a notch **98** in a wall of the distal shaft **14** that extends into the second lumen **32**. The stainless steel cross-piece **96** is larger than the notch **98** and, therefore, cannot be pulled through the notch. The portion of the notch **98** not filled by the cross-piece **96** is filled with glue or the like, preferably a polyurethane glue, which is harder than the material of the distal shaft **14**. Rough edges, if any, of the cross-piece **96** are polished to provide a smooth, continuous surface with the outer surface of the distal shaft **14**.

With further reference to FIG. 5, within the distal shaft **14**, and distal to the glue joint **50**, the turns of the compression coil are expanded longitudinally. Such expanded turns **49** are both bendable and compressible and preferably extend for a length of about 0.5 inch. The puller wire **42** extends through the expanded turns **49** then into a plastic, preferably Teflon®, sheath **81**, which prevents the puller wire from cutting into the wall of the distal shaft **14** when the distal shaft is deflected.

Any other suitable technique for anchoring the puller wire **42** in the distal shaft **14** can also be used. Alternatively, other means for deflecting the distal region can be provided, such as the deflection mechanism described in U.S. Pat. No. 5,537,686, the disclosure of which is incorporated herein by reference.

Longitudinal movement of the puller wire **42** relative to the catheter body **12**, which results in deflection of the distal shaft **14**, is accomplished by suitable manipulation of the control handle **16**. Examples of suitable control handles for use in the present invention are disclosed, for example, in U.S. Pat. Nos. Re 34,502, 5,897,529 and 6,575,931, the entire disclosures of which are incorporated herein by reference.

If desired, the catheter can include two or more puller wires (not shown) to enhance the ability to manipulate the distal shaft **14**. In such an embodiment, a second puller wire and a surrounding second compression coil extend through the proximal shaft **13** and into separate off-axis lumens (not shown) in the distal shaft. Suitable deflection control handles for use with a catheter having more than one puller wire are described in U.S. Pat. Nos. 6,123,699, 6,171,277, and 6,183,463, the disclosures of which are incorporated herein by reference.

As shown in FIG. 3, a needle electrode assembly **46** is provided. The needle electrode assembly **46** is used to ablate tissue while simultaneously injecting saline or other fluid to

conduct the ablation energy, thereby creating a theoretic increase in the effective size of the electrode. The needle electrode assembly **46** is extendable and retractable, and may be moved by manipulation of the needle control handle **17**, as described further below. FIG. 3 depicts the needle electrode assembly **46** in an extended position as it would be to ablate tissue. The distal end of the needle electrode assembly **46** may be withdrawn into the infusion lumen **30** to avoid injury, particularly during the time that the catheter is inserted through the vasculature of the body and during the time in which the catheter is removed from the body.

The needle electrode assembly **46** comprises a proximal tubing **33** joined, directly or indirectly, to a generally rigid, electrically-conductive distal tubing **35**, as shown in FIG. 3. The generally rigid nature of the distal tubing **35** allows it to pierce tissue in order to increase its effectiveness during ablation. In an exemplary embodiment, the distal tubing **35** is formed of Nitinol or stainless steel, and, as illustrated in FIG. 3, is preferably formed with a beveled edge **36** at the distal tip of the needle electrode assembly **46** to enhance its ability to pierce tissue. The proximal tubing **33** is preferably more flexible than the distal tubing **35** to allow the proximal tubing to bend as necessary with the flexible proximal shaft **13** of the catheter body **12**, for instance when the catheter is inserted into the vasculature of the body. The proximal tubing **33** of the needle electrode assembly **46** is preferably made of polyimide or polyether etherketone (PEEK), but can be made of any other suitable biocompatible material, such as plastic or metal.

A needle electrode lead wire **210** is electrically connected at its distal end to the electrically-conductive distal tubing **35** for supplying radio frequency energy or other suitable ablation energy to the distal tubing. The needle electrode lead wire **210** is soldered, welded or otherwise attached to the outside of the distal tubing **35**, but could be attached elsewhere to the distal tubing. The proximal end of the needle electrode lead wire **210** is attached to a suitable connector **67**, which in turn is connected to a suitable source of ablation energy (not shown).

Additionally, a temperature sensor is provided for measuring the temperature of the tissue being ablated by the needle electrode assembly **46** before, during or after ablation. Any conventional temperature sensor, e.g., a thermocouple or thermistor, may be used. In the depicted embodiment, the temperature sensor comprises a thermocouple **200** formed by an enameled wire pair, as best shown in FIG. 4. One wire of the wire pair is a copper wire **202**, e.g., a number 40 copper wire. The other wire of the wire pair is a constantan wire **204**. The wires **202** and **204** of the wire pair are electrically isolated from each other except at their distal ends, where they are twisted together, covered with a short piece of plastic tubing **206**, e.g., polyimide, and covered with epoxy. The plastic tubing **206** is then glued or otherwise attached to the inside wall of the distal tubing **35** of the needle electrode assembly **46**, as best shown in FIG. 3. The proximal ends of the wires **202** and **204** extend out the proximal end of the distal tubing **35** and are attached to an appropriate connector (not shown) connectable to a suitable temperature monitor (not shown). In an alternative embodiment, the copper wire **202** of the thermocouple can also be used as the lead wire for the needle electrode assembly **46**.

The proximal tubing **33** of the needle electrode assembly **46** extends from the needle control handle **17**, through the deflection control handle **16**, through the proximal shaft **13**, and into the infusion lumen **30** of the distal shaft **14**. The proximal end of the distal tubing **35** is spaced slightly from the distal end of the proximal tubing **33** and extends through



the infusion lumen 30 of the distal shaft 14. The proximal and distal tubings 33 and 35 are mounted, preferably coaxially, within an outer plastic tube 48. The outer plastic tube 48 can be glued or otherwise attached to the proximal and distal tubings to form a single structure that, as described below, is longitudinally moveable relative to the catheter body 12. The outer plastic tube 48 extends through the catheter body 12 with the proximal tubing and protects the needle electrode lead wire 210 and thermocouple wires 202 and 204, which extend between the proximal tubing 33 and outer plastic tube 48, when the needle electrode assembly 46 is moved relative to the catheter body. The needle electrode lead wire 210 and thermocouple wires 202 and 204 extend out through a hole (not shown) in the outer plastic tube 48 within the deflection control handle 16 and are attached to appropriate connectors, as noted above.

FIG. 3 shows one arrangement for joining the outer plastic tube 48 to the proximal and distal tubings 33 and 35. Specifically, a small piece of plastic tubing 45, for example, polyimide tubing, is placed over the discontinuity between the proximal and distal tubings 33 and 35 and attached to the proximal and distal tubings by polyurethane glue or the like to form a single infusion passage through which saline or other fluid can pass from the proximal tubing to the distal tubing. The small piece of plastic tubing 45 helps to protect the thermocouple wires 202 and 204 and the needle electrode lead wire 210. A small, preferably non-conductive, spacer 43 is mounted between the distal tubing 35 and the distal end of the outer plastic tube 48, and optionally glued in place. The spacer 43 prevents bodily fluid from entering into the distal end of the needle electrode assembly 46.

In an exemplary embodiment, the proximal tubing 33 of the needle electrode assembly 46 has an inner diameter of 0.014 inch and an outer diameter of 0.016 inch. The distal tubing 35 has an inner diameter of 0.014 inch and an outer diameter of 0.018 inch and a length of about 1.0 inch. Further, the distal tubing 35 extends past the distal end of the distal shaft 14 about 14 mm. The small plastic tubing 45 has an inner diameter of 0.022 inch and an outer diameter of 0.024, the outer plastic tube 48 has an inner diameter of 0.025 inch and an outer diameter of 0.035 inch, and the plastic spacer 43 has an inner diameter of 0.017 inch and an outer diameter of 0.024 inch.

Within the catheter body 12, the needle electrode assembly 46, comprising the proximal tubing 33, distal tubing 35, spacer 43, plastic tubing 45 and outer plastic tube 48, is slidably mounted, preferably coaxially, within a protective tube 47 that is stationary relative to the catheter body. The protective tube 47, which is preferably made of polyimide, serves to prevent the needle electrode assembly 46 from buckling during extension and retraction of the needle electrode assembly relative to the catheter body 12. The protective tube 47 additionally serves to provide a fluid-tight seal surrounding the needle electrode assembly 46. Within the deflection control handle 16, the protective tube 47 and needle electrode assembly 46 extend into a protective shaft 66, which is preferably made of polyurethane.

Other needle electrode assembly designs are contemplated within the scope of the invention. For example, the needle electrode assembly can comprise a single electrically-conductive tube, such as a Nitinol tube, that extends from the needle control handle 17 to the distal end of the catheter. Such a design is described in U.S. patent application Ser. No. 09/711,648, entitled "Injection Catheter with Needle Electrode," the disclosure of which is incorporated herein by reference.

Longitudinal movement of the needle electrode assembly 46 is achieved using the needle control handle 17. The needle electrode assembly 46 and protective tube 47 extend from the deflection control handle 16 to the needle control handle 17 within the protective shaft 66.

As illustrated in FIG. 2, in one embodiment the needle control handle 17 comprises a generally cylindrical outer body 80 having proximal and distal ends, a piston chamber 82 extending a part of the way therethrough, and a needle passage 83 extending a part of the way therethrough. The piston chamber 82 extends from the proximal end of the handle part way into the body 80, but does not extend out the distal end of the body. The needle passage 83, which has a diameter less than that of the piston chamber 82, extends from the distal end of the piston chamber to the distal end of the outer body 80.

A piston 84, having proximal and distal ends, is slidably mounted within the piston chamber 82. A proximal fitting 86 is mounted in and fixedly attached to the proximal end of the piston 84. The proximal fitting 86 includes a tubular distal region 87 that extends distally from the main body of the proximal fitting. The piston 84 has an axial passage 85 through which the proximal tubing 33 of the needle electrode assembly 46 extends, as described in more detail below. A compression spring 88 is mounted within the piston chamber 82 between the distal end of the piston 84 and the outer body 80. The compression spring 88 can either be arranged between the piston 84 and outer body 80, or can have one end in contact with or fixed to the piston, while the other end is in contact with or fixed to the outer body.

The proximal tubing 33, outer plastic tube 48, protective tube 47 and protective shaft 66 extend from the deflection control handle 16 into the distal end of the needle passage 83, as best shown in AREA A of FIG. 2. Within the needle passage 83, the proximal tubing 33, outer plastic tube 48, protective tube 47 and protective shaft 66 extend into a first metal tube 90, which is preferably made of stainless steel. If desired, the first metal tube 90 could instead be made of a rigid plastic material. The first metal tube 90 is secured to the outer body 80 of the needle control handle 17 by a set screw 101 or any other suitable means. The protective shaft 66 terminates at its proximal end within the first metal tube 90.

A second metal tube 91 is provided with its distal end mounted, preferably coaxially, inside the proximal end of the first metal tube 90 and with its distal end abutting the proximal end of the protective shaft 66. The second metal tube 91 is fixed in place relative to the first metal tube 90 by the set screw 101. The second metal tube 91, like the first metal tube 90, could alternatively be made of a rigid plastic material.

The proximal end of the second metal tube 91 is mounted, preferably coaxially, around the distal end of the tubular distal region 87 of the proximal fitting 86, with the second metal tube being longitudinally movable relative to the tubular distal region 87. Accordingly, when the piston 84 is moved distally relative to the outer body 80, the tubular distal region 87 moves distally into the second metal tube 91. As shown in AREA B of FIG. 2, the proximal tubing 33 and outer plastic tube 48 extend through the second metal tube 91 and into the tubular distal region 87 of the proximal fitting 86. The outer plastic tube 48 terminates in and is fixedly attached to the proximal fitting 86 to thereby attach the outer plastic tube, and thus the needle electrode assembly 46, to the piston 84. Within the proximal fitting 86, the proximal tubing 33 extends out of the outer plastic tube 48 and into a first protective sheath 31, as shown in AREA C of FIG. 2, and is connected to a luer connector 65, which is connected to an irrigation pump or other suitable fluid infusion source (not shown), as is known in the art. Similarly, the needle electrode lead wire 210

and the thermocouple wires **202** and **204** extend out of the outer plastic tube **48** and into a second protective sheath **29**, as also shown in AREA C of FIG. 2, which is connected to a suitable connector **67**, such as a 10-pin electrical connector, for connecting the needle electrode lead wire to a source of ablation energy and the thermocouple wires to a suitable monitoring system.

In use, force is applied to the piston **84** to cause distal movement of the piston relative to the outer body **80**, which compresses the compression spring **88**. This movement causes the needle electrode assembly **46** to correspondingly move distally relative to the outer body **80**, protective shaft **66**, protective tube **47**, proximal shaft **13**, and distal shaft **14** so that the distal tubing **35** of the needle electrode assembly extends outside the distal end of the distal shaft. When the force is removed from the piston **84**, the compression spring **88** pushes the piston proximally to its original position, thus causing the distal tubing **35** of the needle electrode assembly **46** to retract back into the distal end of the distal shaft **14**. Upon distal movement of the piston **84**, the tubular distal region **87** of the proximal fitting **86** moves distally into the second metal tube **91** to prevent the proximal tubing **33** and the outer plastic tube **48** of the needle electrode assembly **46** from buckling within the axial passage **85**.

The piston **84** further comprises a longitudinal slot **100** extending along a portion of its outer edge. A securing means **102**, such as a set screw, pin, or other locking mechanism, extends through the outer body **80** and into the longitudinal slot **100**. This design limits the distance that the piston **84** can be slid proximally out of the piston chamber **82**. When the needle electrode assembly **46** is in the retracted position, preferably the securing means **102** is at or near the distal end of the longitudinal slot **100**.

The proximal end of the piston **84** has a threaded outer surface **104**. A circular thumb control **106** is rotatably mounted on the proximal end of the piston **84**. The thumb control **106** has a threaded inner surface **108** that interacts with the threaded outer surface **104** of the piston. The thumb control **106** acts as a stop, limiting the distance that the piston **84** can be pushed into the piston chamber **82**, and thus the distance that the needle electrode assembly **46** can be extended out of the distal end of the catheter. The threaded surfaces of the thumb control **106** and piston **84** allow the thumb control to be moved closer or farther from the proximal end of the outer body **80** so that the extension distance of the needle electrode assembly **46** can be controlled by the physician. A securing means, such as a tension screw **110** is provided in the thumb control **106** to control the tension between the thumb control and piston **84**. As would be recognized by one skilled in the art, the thumb control **106** can be replaced by any other mechanism that can act as a stop for limiting the distance that the piston **84** extends into the piston chamber **82**, and it is not necessary, although it is preferred, that the stop be adjustable relative to the piston.

As noted above, the mapping assembly **15** is mounted on the distal end of the distal shaft **14**. With reference to FIGS. 3 and 8, the mapping assembly **15** comprises two or more flexible spines **118**. Each spine **118** has a proximal end attached to the distal end of the catheter body **12** and a free distal end, i.e., the distal end is not attached to any of the other spines, to the catheter body, or to any other structure that confines movement of the distal end of that spine. As will be recognized by one skilled in the art, the number of spines **118** can vary as desired depending on the particular application, so that the mapping assembly **15** has at least two spines, preferably at least three spines, more preferably at least five spines and as many as eight or more spines. The spines **118**

are moveable between an expanded arrangement, wherein, for example, each spine arcs outward from the distal end of the catheter body **12**, as shown in FIG. 8, and a collapsed arrangement (not shown), wherein, for example, each spine is disposed generally along a longitudinal axis of the catheter body so that the spines are capable of fitting within a lumen of a guiding sheath. As described in more detail below, each spine **118** carries at least one electrode, preferably a ring electrode, such that when the spines are positioned in contact with heart tissue, each spine is capable of obtaining electrical and mechanical data.

In the embodiment shown in FIG. 8, the mapping assembly **15** includes five spines **118**, and each spine has a pre-formed configuration in which the spine arcs outwardly from the catheter body **12**. However, other spine shapes and configurations are contemplated within the invention. With reference to FIG. 3, each spine **118** comprises a support arm **124** and a non-conductive covering **134** in surrounding relation to the support arm **124**. The support arm **124** comprises a metal or plastic material that has shape memory, such that the support arm forms an initial shape (i.e., part of the expanded configuration) when no external forces are applied, forms a deflected shape (e.g., part of the collapsed configuration) when external force is applied, and returns to its initial shape when the external force is released. In one embodiment, each support arm **124** comprises a superelastic material, for example, a nickel-titanium alloy such as nitinol. In a preferred embodiment, the non-conductive covering **134** comprises a biocompatible plastic tubing, such as polyurethane or polyimide tubing. The non-conductive covering **134** may be glued to the support arm **124** or attached indirectly by being glued to the distal end of the distal tubing **35**. The non-conductive covering **134** may be attached to the support arm **124** by any other suitable method.

As noted above, each spine **118** carries at least one electrode mounted along its length. In the depicted embodiment, four ring electrodes **125** are mounted on the non-conductive covering **134** of each spine **118**, but fewer or additional ring electrodes may be used as desired. Each ring electrode **125** has a length preferably up to about 2 mm, more preferably from about 0.5 mm to about 1 mm. Preferably the ring electrodes **125** are generally evenly-spaced along the length of each spine **118**.

Each ring electrode **125** is electrically connected to an electrode lead wire **129**, which in turn is electrically connected to a connector (not shown), which can be incorporated into the deflection control handle **16** or provided outside of the catheter. The connector is connected to an appropriate mapping or monitoring system (not shown). Each electrode lead wire **129** extends from the connector, through the deflection control handle **16**, through the central lumen **18** in the proximal shaft **13** of the catheter body **12**, through the lead wire lumen **34** of the distal shaft **14**, and into the non-conductive covering **134** of one of the spines **118**, where it is attached to its corresponding ring electrode **125**. Within the proximal shaft **13** and deflection control handle **16**, the lead wires **129** extend through a protective tube **70**, which can be eliminated if desired.

Each lead wire **129**, which includes a non-conductive coating over almost all of its length, is attached to its corresponding ring electrode **125** by any suitable method. An exemplary method for attaching a lead wire **129** to a ring electrode **125** involves first making a small hole through an outer wall of the non-conductive covering **134**. Such a hole can be created, for example, by inserting a needle through the non-conductive covering **134** and heating the needle sufficiently to form a permanent hole. The lead wire **129** is then drawn through the

hole by using a microhook or the like. The end of the lead wire **129** is then stripped of any coating and welded to the underside of the ring electrode **125**, which is then slid into position over the hole and fixed in place with polyurethane glue or the like. Alternatively, each ring electrode **125** may be formed by wrapping the lead wire **129** around the non-conductive covering **134** a number of times and stripping the lead wire of its own non-conductive coating on its outwardly facing surfaces. In such an instance, the lead wire **129** functions as a ring electrode.

In the depicted embodiment, two of the spines **118** each carry a marker band **130a**, **130b** to help the user identify the orientation of the mapping assembly **15** under fluoroscopy. Each marker band **130a**, **130b** comprises a metal ring (e.g., a ring electrode not attached to a lead wire) of sufficient radioactivity. The marker bands **130** and **130b** may be placed along any part of the spine **118**, as long as they are not in contact with any of the ring electrodes **125**. Preferably, a first marker band **130a** is placed on a first spine **118a** between the most proximal ring electrode **125a** and the distal shaft **14**, and a second marker band **130b** is placed on a second spine **118b** between the most proximal ring electrode **125a** and the second most proximal ring electrode **125b**.

In the depicted embodiment, the spines **118** of the mapping assembly **15** are supported and given their desired shape by a support structure **120** comprising a base **122** and plurality of support arms **124** extending from the base, as best shown in FIG. 9. The base **122** of the support structure **120** is generally cylindrically shaped for mounting over the distal end of the tubing **19** of the distal shaft **14**. The support arms **124** each have a proximal end attached to the base **122** and a free distal end, as described above. The number of support arms **124** on the support structure corresponds to the desired number of spines **118** on the mapping assembly, and in the depicted embodiment is five.

In a preferred embodiment, the support structure **120** is manufactured from a single metal tube, and thus has a unitary structure. In a particularly preferred embodiment, the support structure **120** is manufactured from a nickel-titanium alloy, for instance, Nitinol. Preferably, the base is a right circular cylinder and has a diameter slightly larger than the distal end of the distal shaft **14**.

In the depicted embodiment, each support arm **124** is tapered slightly from its proximal end to its distal end, which allows for greater distal flexibility while maintaining the desired curvature at the proximal end. Each support arm **124** also includes a disc-shaped tip **127**, which provides more surface area for the distal end of the support arm **124** to be glued to its corresponding non-conductive covering **134**.

During assembly, the base **122** of the support structure **120** is mounted over the distal end of the tubing **19** of the distal shaft **14**. Non-conductive coverings **134** are introduced over the support arms **124** to form the spines **118** of the mapping assembly **15**. After the ring electrodes **125** are mounted on the spines **118** as described above and the other desired components are assembled within the catheter, a piece of tubular plastic **208** is mounted over the base **122** of the support structure **120** and optionally glued in place. The piece of tubular plastic **208** also covers the proximal ends of the non-conductive coverings **134**.

Other methods and structures for forming and supporting the mapping assembly are within the scope of the invention. An example of an alternative design for the mapping assembly according to the invention is described in U.S. patent application Ser. No. 10/040,932, entitled "Catheter Having

Multiple Spines Each Having Electrical, Mapping and Location Sensing Capabilities," the disclosure of which is incorporated herein by reference.

In the depicted embodiment, as shown in FIG. 3, the catheter further includes at least one location sensor **140**. The location sensor **140** is used to determine the coordinates of the mapping assembly **15** at each instant when the mapping assembly **15** is being used to collect one or more electrical mapping data points. As a result, both electrical and locational data can be obtained for each data point that is mapped. In the depicted embodiment, a single location sensor **140** is mounted in the distal end of the distal shaft **14** within the cylindrical base **122** of the support structure **120**. Alternatively, the catheter can include multiple location sensors **140**, one mounted within each spine **118** of the mapping assembly **15**, as described in U.S. patent application Ser. No. 10/040,932, entitled "Catheter Having Multiple Spines Each Having Electrical, Mapping and Location Sensing Capabilities," the entire disclosure of which is incorporated herein by reference.

The location sensor **140** is connected to a corresponding sensor cable **74**. The sensor cable **74** extends, along with the lead wires **129**, through the lead wire lumen **34** of the distal shaft **14**, and through the proximal shaft **13** within the protective tube **70** and then into the deflection control handle **16** and out of the proximal end of the deflection control handle within an umbilical cord (not shown) to a sensor control module (not shown) that houses a circuit board (not shown). Alternatively, the circuit board can be housed within the control handle **16**, for example, as described in U.S. Pat. No. 6,024,739, the disclosure of which is incorporated herein by reference. The sensor cable **74** comprises multiple wires encased within a plastic covered sheath. In the sensor control module, the wires of the sensor cable **74** are connected to the circuit board. The circuit board amplifies the signal received from the location sensor **140** and transmits it to a computer in a form understandable by the computer by means of a sensor connector at the proximal end of the sensor control module. Also, because the catheter is designed for single use only, the circuit board preferably contains an EPROM chip that shuts down the circuit board approximately twenty-four hours after the catheter has been used. This prevents the catheter, or at least the location sensor **140**, from being used twice.

Preferably the location sensor **140** is an electromagnetic location sensor. For example, the location sensor **140** may comprise a magnetic-field-responsive coil, as described in U.S. Pat. No. 5,391,199, or a plurality of such coils, as described in International Publication WO 96/05758. The plurality of coils enables the six-dimensional coordinates (i.e. the three positional and the three orientational coordinates) of the location sensor **140** to be determined. Alternatively, any suitable location sensor known in the art may be used, such as electrical, magnetic or acoustic sensors. Suitable location sensors for use with the present invention are also described, for example, in U.S. Pat. Nos. 5,558,091, 5,443,489, 5,480,422, 5,546,951, and 5,568,809, International Publication Nos. WO 95/02995, WO 97/24983, and WO 98/29033, and U.S. patent application Ser. No. 09/882,125 filed Jun. 15, 2001, entitled "Position Sensor Having Core with High Permeability Material," the disclosures of which are incorporated herein by reference.

Using this technology, the physician can visually map a heart chamber. This mapping is done by advancing the distal shaft **14** into a heart chamber until contact is made with the heart wall. This position is recorded and saved. The distal shaft **14** is then moved to another position in contact with the heart wall and again the position is recorded and saved.

The location sensor **140** can be used alone or more preferably in combination with the ring electrodes **125**. By combining the location sensor **140** and electrodes **125**, a physician can simultaneously map the contours or shape of the heart chamber, the electrical activity of the heart, and the extent of displacement of the catheter and hence identify the presence and location of the ischemic tissue. Specifically, the location sensor **125** is used to monitor the precise location of the distal end of the catheter in the heart and the extent of catheter displacement. The ring electrodes **125** are used to monitor the strength of the electrical signals at that location.

The preceding description has been presented with reference to presently preferred embodiments of the invention. Workers skilled in the art and technology to which this invention pertains will appreciate that alterations and changes in the described structure may be practiced without meaningful departing from the principal, spirit and scope of this invention.

Accordingly, the foregoing description should not be read as pertaining only to the precise structures described and illustrated in the accompanying drawings, but rather should be read consistent with and as support to the following claims which are to have their fullest and fair scope.

What is claimed is:

1. An injection catheter comprising:
  - an elongated catheter body having at least one lumen extending longitudinally therethrough;
  - a needle control handle at a proximal end of the catheter body;
  - a needle electrode assembly extending through the catheter body and needle control handle and having a proximal end attached to the needle control handle and a distal end within a distal end of the catheter body;
  - a mapping assembly, having proximal and distal ends, mounted at the distal end of the catheter body and comprising at least two flexible spines, each spine having a proximal end attached at the distal end of the catheter body and a free distal end, wherein each spine carries at least one electrode; and
  - at least one location sensor;
  - wherein the distal end of the needle electrode assembly is extendable past the proximal end of the mapping assembly upon manipulation of the needle control handle.
2. The catheter of claim 1, wherein each spine comprises a non-conductive covering having a support arm that has shape memory disposed therein.
3. The catheter of claim 2, wherein each support arm comprises Nitinol.
4. The catheter of claim 1, wherein the mapping assembly is moveable between an expanded arrangement, in which each spine extends radially outward from the catheter body, and a collapsed arrangement, in which each spine is disposed generally along a longitudinal axis of the catheter body.
5. The catheter of claim 4, wherein, when the mapping assembly is in its expanded arrangement, each spine extends radially outwardly from the catheter body and forms an arced shape.
6. The catheter of claim 1, wherein the mapping assembly comprises at least five spines.
7. The catheter of claim 1, further comprising an electrode lead wire having a first end electrically connected to the

needle electrode assembly and a second end electrically connected to a source of ablation energy.

8. The catheter of claim 1, wherein the needle electrode assembly comprises a distal tubing having proximal and distal ends and comprising an electrically conductive material and a proximal tubing comprising a material more flexible than the distal tubing and having a distal end attached, directly or indirectly, to the proximal end of the distal tubing.

9. The catheter of claim 8, wherein the distal tubing comprises metal and the proximal tubing comprises plastic.

10. The catheter of claim 8, wherein the distal tubing comprises Nitinol or stainless steel.

11. The catheter of claim 8, wherein the proximal tubing comprises polyimide or PEEK.

12. The catheter of claim 8, wherein the distal end of the distal tubing forms a beveled edge.

13. The catheter of claim 8, wherein the needle electrode assembly further comprises an intermediate tubing joining the proximal and distal tubings.

14. The catheter of claim 8, wherein the needle electrode assembly further comprises an outer plastic tubing fixedly attached, directly or indirectly, to the proximal and distal tubings so that the outer plastic tubing is moveable with the proximal and distal tubings relative to the catheter body.

15. The catheter of claim 14, wherein the electrode lead wire is fixedly attached to the distal tubing and extends within the outer plastic tubing and outside the proximal tubing.

16. The catheter of claim 8, further comprising a temperature sensor mounted within the distal tubing.

17. The catheter of claim 1, further comprising a temperature sensor mounted in or around the needle electrode assembly.

18. An injection catheter comprising:
 

- an elongated catheter body having at least one lumen extending longitudinally therethrough;
- a needle control handle at a proximal end of the catheter body;
- a needle electrode assembly extending through the catheter body and needle control handle and having a proximal end attached to the needle control handle and a distal end within a distal end of the catheter body; and
- a mapping assembly, having proximal and distal ends, mounted at the distal end of the catheter body and comprising at least two flexible spines, each spine having a proximal end attached at the distal end of the catheter body and a free distal end, wherein each spine carries at least one electrode and at least one location sensor;
- wherein the distal end of the needle electrode assembly is extendable past the proximal end of the mapping assembly upon manipulation of the needle control handle.

19. The catheter of claim 18, wherein each spine comprises a non-conductive covering having a support arm that has shape memory disposed therein.

20. The catheter of claim 18, wherein the mapping assembly is moveable between an expanded arrangement, in which each spine extends radially outward from the catheter body, and a collapsed arrangement, in which each spine is disposed generally along a longitudinal axis of the catheter body.

专利名称(译)	带消融针和标测组件的导管		
公开(公告)号	<a href="#">US8287531</a>	公开(公告)日	2012-10-16
申请号	US12/140996	申请日	2008-06-17
[标]申请(专利权)人(译)	韦伯斯特生物官能公司		
申请(专利权)人(译)	生物传感韦伯斯特, INC.		
当前申请(专利权)人(译)	生物传感韦伯斯特, INC.		
[标]发明人	MEST ROBERT A		
发明人	MEST, ROBERT A.		
IPC分类号	A61B18/14 A61F2/00 A61B5/0408 A61B5/00 A61B5/042 A61B5/0478 A61B5/0492 A61M25/00		
CPC分类号	A61B5/0422 A61B5/6859 A61B18/1477 A61B5/01 A61B18/1492 A61B2018/00214 A61B2018/00577 A61B2018/00839 A61B2018/00898 A61B2018/1475		
审查员(译)	GIBSON, ROY		
其他公开文献	US20080249392A1		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

#### 摘要(译)

本发明涉及一种导管，该导管使用针电极产生增强的损伤，并且可以使用增强的标测组件同时在多个点处绘制电活动。导管包括细长的导管主体，该导管主体具有至少一个纵向延伸穿过其中的内腔。针控制手柄设置在导管主体的近端。针电极组件延伸穿过导管主体和针控制手柄，并且具有连接到针控制手柄的近端和位于导管主体的远端内的远端。标测组件安装在导管主体的远端，并包括至少两个柔性脊。每个脊柱具有附接在导管主体的远端处的近端和自由远端。每个脊柱携带至少一个电极。在操纵针控制手柄时，针电极组件的远端可延伸超过标测组件的近端。

