



(19) **United States**

(12) **Patent Application Publication** (10) **Pub. No.: US 2003/0100846 A1**

Custer et al. (43) **Pub. Date: May 29, 2003**

(54) **SYSTEM, METHOD, AND DEVICE FOR NON-INVASIVE BODY FLUID SAMPLING AND ANALYSIS**

(52) **U.S. Cl. 600/573**

(76) **Inventors: Linda Custer, Marlborough, MA (US); Tuan A. Elstrom, Lake Bluff, IL (US); Scott C. Kellogg, Boston, MA (US); Joseph Kost, Cambridge, MA (US); Nicholas F. Warner, Belmont, MA (US)**

(57) **ABSTRACT**

A system, method, and device for non-invasive body fluid sampling is provided. According to one embodiment of the present invention, the system includes a controller that controls the generation of ultrasound; an ultrasonic applicator that applies the ultrasound to an area of biological membrane; a receiver that contacts the area of biological membrane and receives body fluid through and out of the area of biological membrane; and a meter that interacts with the receiver and detects the presence of at least one analyte in the body fluid in the receiver. The receiver may include a membrane and a medium, such as a hydrogel, a fluid, or a liquid, that is contained in the membrane. According to one embodiment of the present invention, the method includes the steps of (1) identifying an area of biological membrane having a permeability level; (2) increasing the permeability level of the area of biological membrane; (3) contacting the area of biological membrane with a receiver; (4) extracting body fluid through and out of the area of biological membrane; (5) providing an external force to enhance the body fluid extraction; (6) collecting the body fluid in the receiver; (7) analyzing the collected body fluid for the presence of at least one analyte; and (8) providing the results of the step of analyzing the body fluid.

Correspondence Address:
Brobeck Phleger & Harrison
Intellectual Property Department
Suite 800
1333 H Street NW
Washington, DC 20005 (US)

(21) **Appl. No.: 09/979,096**

(22) **PCT Filed: Mar. 16, 2001**


(86) **PCT No.: PCT/US01/08489**

Related U.S. Application Data

(60) **Provisional application No. 60/189,971, filed on Mar. 17, 2000.**

Publication Classification

(51) **Int. Cl.⁷ A61B 5/00**

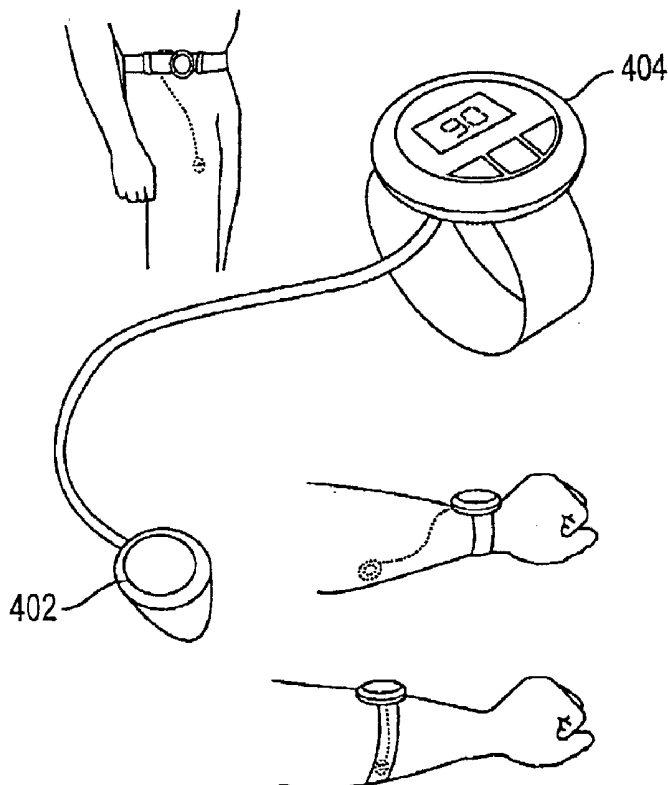

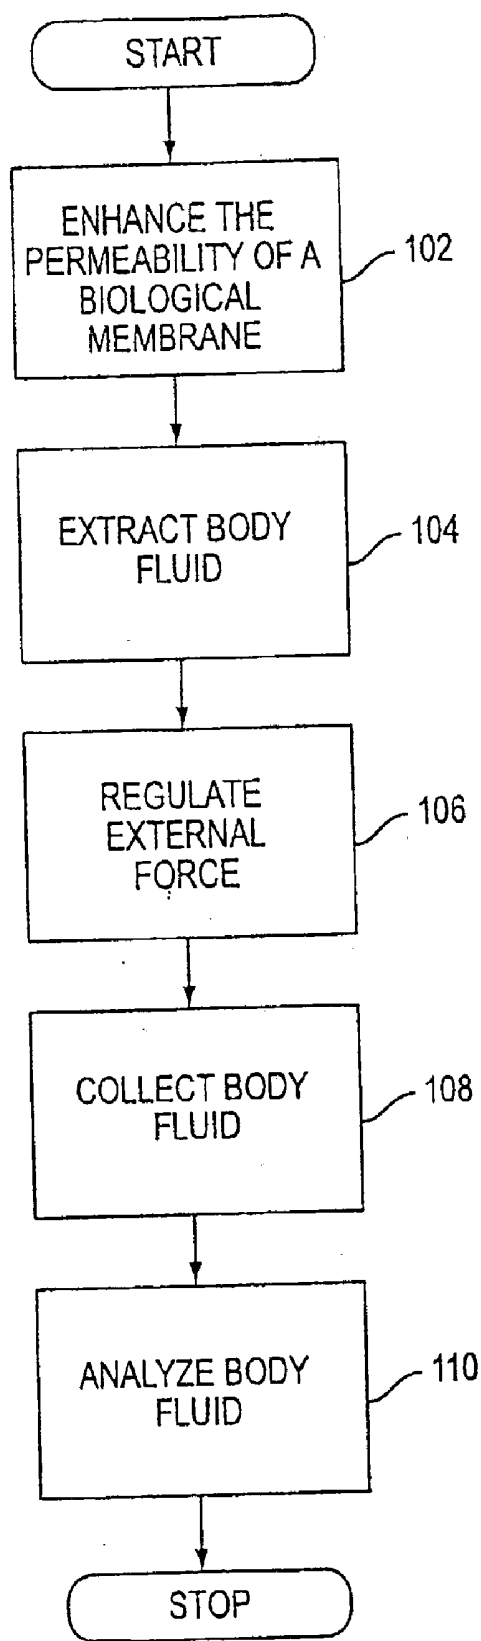


FIG. 1

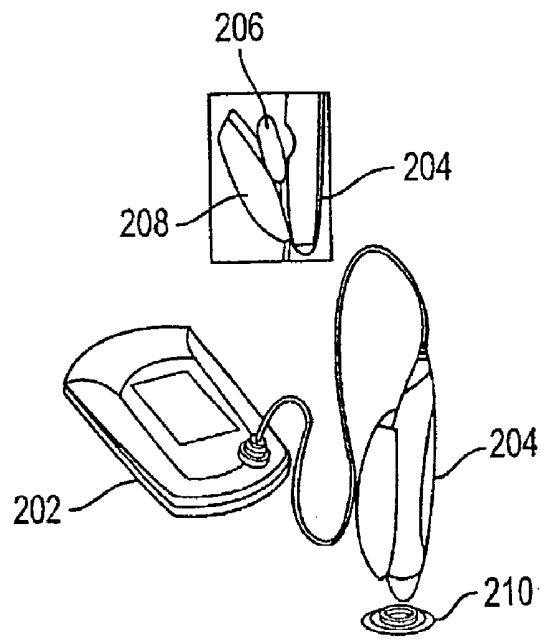


FIG. 2

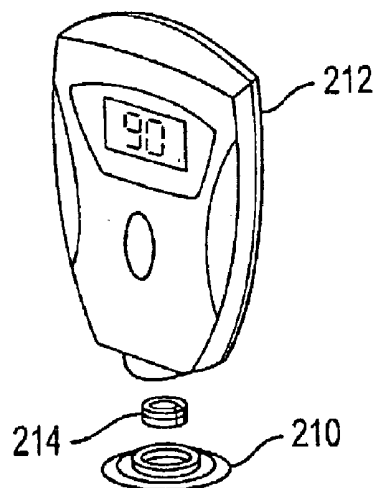


FIG. 3

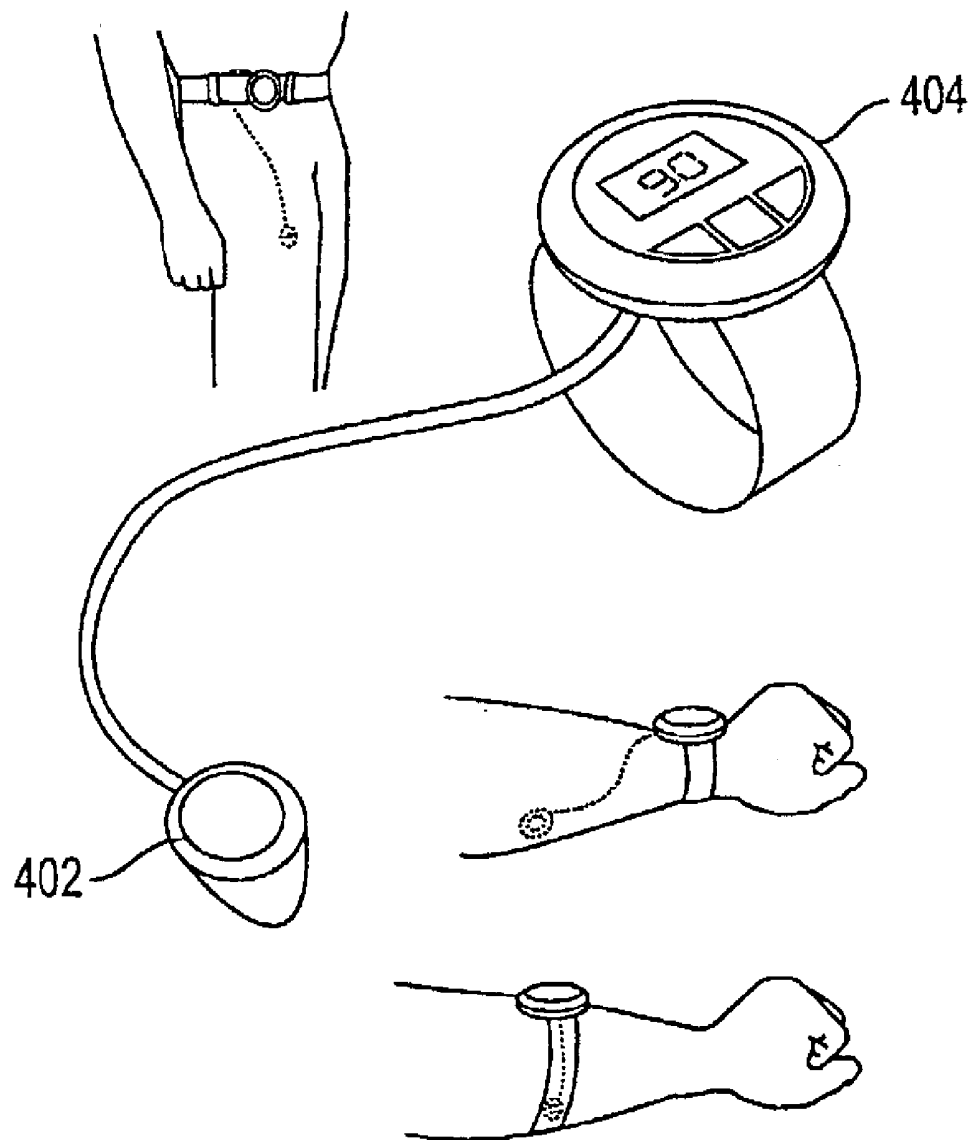


FIG. 4

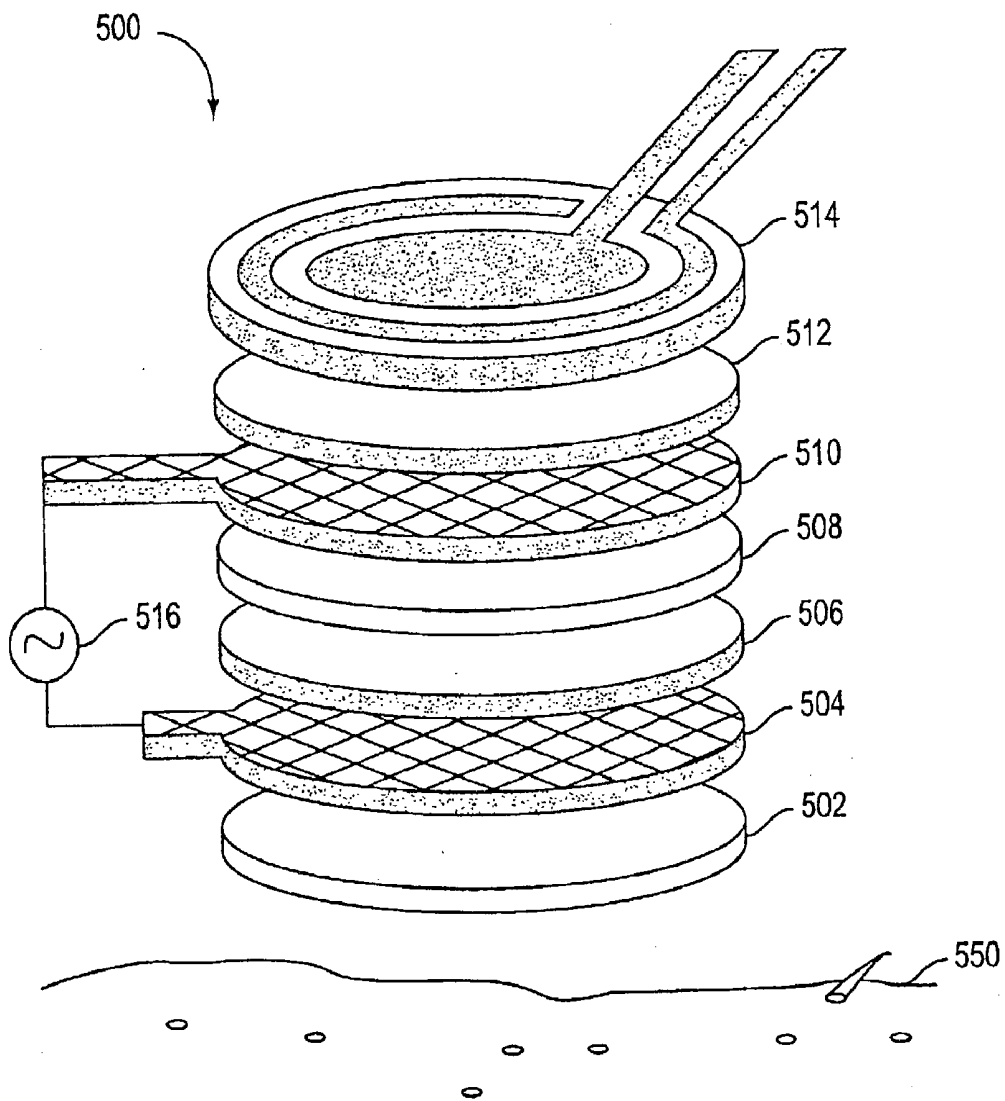


FIG. 5

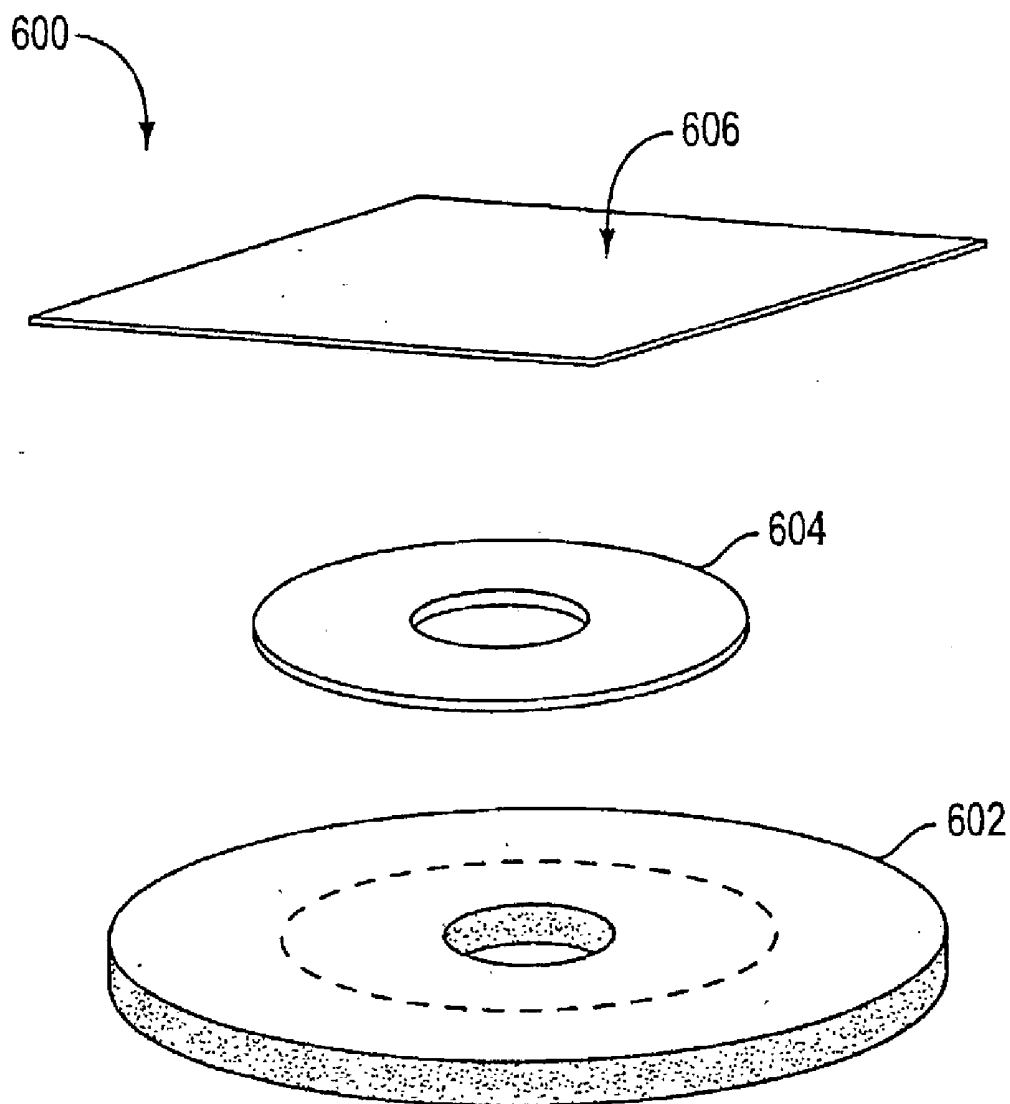


FIG. 6

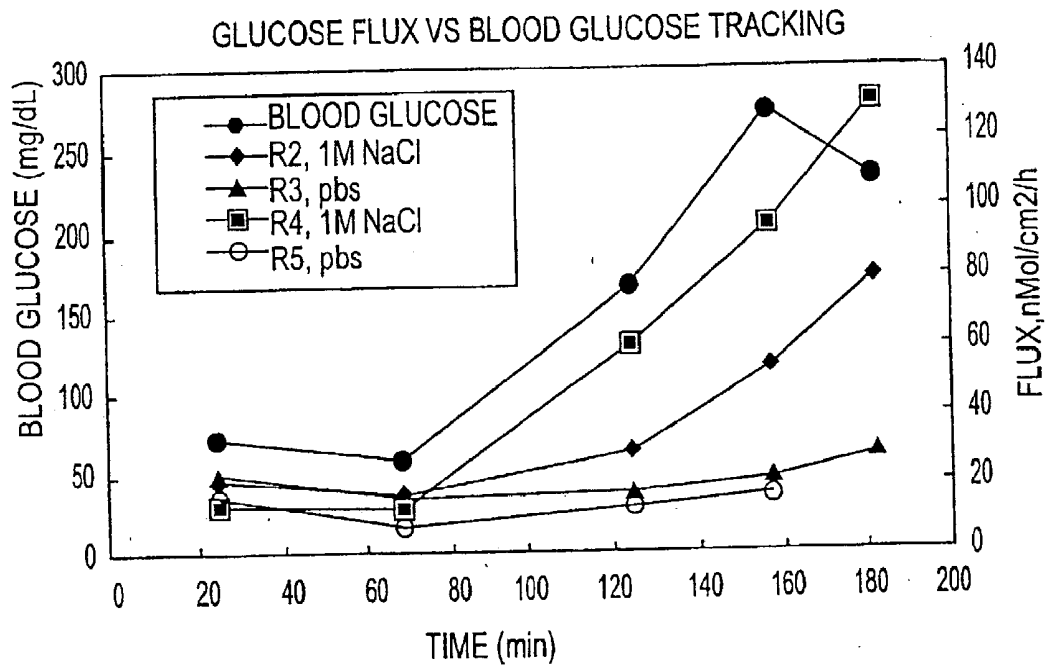


FIG. 7

SYSTEM, METHOD, AND DEVICE FOR NON-INVASIVE BODY FLUID SAMPLING AND ANALYSIS

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] The present invention claims the benefit of U.S. Provisional Patent Application No. 60/189,971, filed Mar. 17, 2000, the disclosure of which is hereby incorporated by reference in its entirety.

[0002] In addition, the invention is related to U.S. patent application Ser. No. 08/885,931, entitled "Ultrasound Enhancement of Transdermal Transport"; U.S. patent application Ser. No. 09/260,265, entitled "Chemical and Physical Enhancers and Ultrasound for Transdermal Drug Delivery"; and PCT International Patent Appl'n Ser. No. PCT/US99/30067, entitled "Method and Apparatus for Enhancement of Transdermal Transport", the disclosures of which are hereby incorporated, by reference, in their entirety.

BACKGROUND OF THE INVENTION

[0003] 1. Field of the Invention

[0004] The present invention relates to non-invasive sampling of body fluids, and, more particularly, to a system, method, and device for non-invasive body fluid sampling and analysis.

[0005] 2. Description of the Related Art

[0006] Diabetics frequently prick their fingers and forearms to obtain blood in order to monitor their blood glucose concentration. This practice of using blood to perform frequent monitoring can be painful and inconvenient. New, less painful methods of sampling body fluids have been contemplated and disclosed. For example, these painless methods include the use of tiny needles, the use of iontophoresis, and the use of ultrasound to sample body fluid, such as blood and interstitial fluid.

[0007] It has been shown that the application of ultrasound can enhance skin permeability. Examples of such are disclosed in U.S. Pat. No. 4,767,402, U.S. Pat. No. 5,947,921, and U.S. Pat. No. 6,002,961, the disclosures of which are incorporated, by reference, in their entirety. Ultrasound may be applied to the stratum corneum via a coupling medium in order to disrupt the lipid bilayers through the action of cavitation and its bioacoustic effects. The disruption of stratum corneum, a barrier to transport, allows the enhanced diffusion of analyte, such as glucose or drugs, through, into, and out of the skin.

[0008] Transport of analytes and body fluids can be enhanced further by the action of a motive force. These motive forces include, inter alia, sonophoretic, iontophoretic, electromotive, pressure force, vacuum, electromagnetic motive, thermal force, magnetic force, chemomotive, capillary action, and osmotic. The use of active forces provide a means for obtaining fluid for subsequent analysis.

[0009] The application of a motive force before, during, and after making the skin permeable has been disclosed in U.S. Pat. No. 5,279,543, U.S. Pat. No. 5,722,397, U.S. Pat. No. 5,947,921, U.S. Pat. No. 6,002,961, and U.S. Pat. No. 6,009,343, the disclosures of which are incorporated by reference in their entirety. The purpose of using a motive

force is to actively extract body fluid and its content out of the skin for the purpose of analysis. As mentioned, active forces, such as vacuum, sonophoresis, and electrosmotic forces, can create convective flow through the stratum corneum. Although these forces can be used for extraction of body fluids, there are certain limitations that may apply when the forces are applied to human skin. For example, a major limitation is the flow and volume of body fluid that can be transported across the stratum corneum. In general, high-pressure force is necessary in order to transport fluid across an enhanced permeable area of stratum corneum. The application of vacuum on skin for an extended period may cause physical separation of the epidermis from the dermis, resulting in bruises and blisters.

[0010] Another example of a limitation is the amount of energy that can be applied to the skin in order to create convective flow. Extraction of usable volume of body fluid has the potential to cause pain and skin damage with prolonged exposure to ultrasound. In a similar manner, electro-osmotic extraction of body fluid through stratum corneum has the potential to cause skin damage due the need to use high current density. It is evident that there are limitations to the use of the mentioned extraction methods when applied to human skin.

SUMMARY OF THE INVENTION

[0011] Therefore, a need has arisen for a system, method, and device for noninvasive body fluid sampling and analysis that overcomes these and other drawbacks of the related art.

[0012] Therefore, a need has arisen for a method of enhancing the permeability of a biological membrane, such as skin, buccal, and nails, for an extended period of time, and a method for extracting body fluid to perform blood, interstitial fluid, lymph, or other body fluid analyte monitoring in a discrete or continuous manner that is noninvasive and practical.

[0013] A method for non-invasive body fluid sampling and analysis is disclosed. According to one, embodiment of the present invention, the method includes the steps of (1) identifying an area of biological membrane having a permeability level; (2) increasing the permeability level of the area of biological membrane; (3) contacting the area of biological membrane with a receiver; (4) extracting body fluid through and out of the area of biological membrane; (5) providing an external force to enhance the body fluid extraction; (6) collecting the body fluid in the receiver; (7) analyzing the collected body fluid for the presence of at least one analyte; and (8) providing the results of the step of analyzing the body fluid.

[0014] The area of biological membrane may be made permeable using ultrasound with controlled dosimetry. Extraction of body fluid may be performed on the area exposed to ultrasound using osmotic transport. The body fluid may be collected using a receiver. The receiver may be attached to the biological membrane in a form of a patch, a wearable reservoir, a membrane, an absorbent strip, a hydrogel, or an equivalent. The receiver may be analyzed for the presence of various analytes indicative of blood analytes. The analysis may comprise the use of electrochemical, biochemical, optical, fluorescence, absorbance, reflectance, Raman, magnetic, mass spectrometry, infra-red (IR) spectroscopy measurement methods and combinations thereof.

The receiver may also be attached to a secondary receiver where the concentration of analyte in the secondary receiver is continuously maintained substantially lower than that in the body fluid so the chemical concentration driving force between body fluid and secondary receiver is maximized. This may be achieved by chemical reaction or volume for dilution or similar means. In one embodiment, the receiver and the secondary receiver may operate on different principles (e.g., osmosis, dilution, etc.). In another embodiment, the receivers may operate on the same principle.

[0015] A system for non-invasive body fluid sampling and analysis is disclosed. According to one embodiment of the present invention, the system includes a controller that controls the generation of ultrasound; an ultrasonic applicator that applies the ultrasound to an area of biological membrane; a receiver that contacts the area of biological membrane and receives body fluid through and out of the area of biological membrane; and a meter that interacts with the receiver and detects the presence of at least one analyte in the body fluid in the receiver. The receiver may include a membrane and a medium, such as a hydrogel, a fluid, or a liquid, that is contained within the membrane.

[0016] A method for noninvasive body fluid sampling and analysis is disclosed. According to one embodiment of the present invention, the method includes the steps of (1) enhancing a permeability level of an area of biological membrane; (2) attaching a receiver to the area of biological membrane; (3) extracting an analyte through and out of the area of biological membrane; (4) collecting the body fluid in the receiver; and (5) determining a concentration of at least one analyte in the body fluid.

[0017] A device for noninvasive body fluid sampling and analysis is disclosed. According to one embodiment of the present invention, the device includes a receiver that is attached to an area of biological membrane with an enhanced permeability and receives body fluid through and out of the area of biological membrane, and a wearable meter that detects the presence of at least one analyte in the received body fluid and indicates a concentration of that analyte. The receiver may include a membrane and a medium, such as a hydrogel, a fluid, or a liquid, that is contained in the membrane. The meter may include a processor and a device that detects the presence of the analyte. The detecting device may include an electrochemical detector; a biochemical detector; a fluorescence detector; an absorbance detector; a reflectance detector; a Raman detector; a magnetic detector; a mass spectrometry detector; an IR spectroscopy detector; and combinations thereof.

[0018] According to one embodiment of the present invention, osmotic forces may be used to sample body fluid from and through a biological membrane in an on-demand manner. The osmotic agent in solution, gel, hydrogel, or other form may be applied to the ultrasound-treated biological membrane using a receiver, such as a thin liquid reservoir, whenever the concentration of an analyte needs to be determined for diagnosis and monitoring. The receiver may be attached to the biological membrane using an adhesive. The receiver may be attached to the biological membrane for a brief duration. The solution in the receiver may be subsequently removed and analyzed for the presence of analytes. In one embodiment, the receiver may be constructed in the form of a patch. The receiver may contain a hydrogel

and osmotic agent. The receiver may combine the osmotic agent and the chemical reagents to detect the presence of the analyte. The reagents may allow the use of electrochemical, biochemical, optical, fluorescence, absorbance, reflectance, Raman, magnetic, mass spectrometry, infrared (IR) spectroscopy measurement methods and combinations thereof to be performed on the receiver.

[0019] In another embodiment, osmotic forces may be used to sample body fluid from or through a biological membrane in a periodic or a continuous manner. The osmotic agent in solution form may be applied to the ultrasound-treated biological membrane using a thin receiver, such as a thin liquid reservoir, whenever the concentration of analyte needs to be determined for diagnosis and monitoring. The receiver may be attached to biological membrane using an adhesive. In one embodiment, the receiver may be constructed in the form of a patch. The receiver may contain a hydrogel that contains the osmotic agent. The receiver may contain means for manipulating the intensity and duration of the osmotic force. The intensity of the osmotic force may be manipulated using electric field forces, magnetic field forces, electromagnetic field forces, biochemical reactions, chemicals, molarity adjustment, adjusting solvents, adjusting pH, ultrasonic field forces, electro-osmotic field forces, iontophoretic field forces, electroporatic field forces and combinations thereof. The duration of the osmotic force may be manipulated using electric field forces, magnetic field forces, electromagnetic field forces, biochemical reactions, chemicals, molarity adjustment, adjusting solvents, adjusting pH, ultrasonic field forces, electroosmotic field forces, iontophoretic field forces, electroporatic field forces and combinations thereof. The receiver may combine the osmotic agent and the biochemical reagents to detect the presence of the analyte. The reagents may allow the use of electrochemical, biochemical, optical, fluorescence, absorbance, reflectance, Raman, magnetic, mass spectrometry, IR spectroscopy measurement methods and combinations thereof to be performed on the receiver. The receiver may also be removed periodically for detection.

[0020] In one embodiment, the intensity, duration, and frequency of exposure of biological membrane to osmotic forces may be manipulated by using an electric current to cause a change in the concentration of the osmotic agent that is in contact with the ultrasound-exposed biological membrane. The osmotic agent may be a multi-charged agent that can dissociate into several charged species. These charged species may be transported using electric field forces. A membrane may be used to isolate the charged species. The charged species freely diffuse and combine upon removal of the electric field force.

[0021] In one embodiment, the intensity, duration, and frequency of exposure of biological membrane to osmotic forces may be manipulated by using active forces to cause a change in the concentration of the osmotic agent that is in contact with the ultrasound-exposed biological membrane. The osmotic agent may be a neutral charge agent. The agent may be transported using a variety of field forces. The field force depends on the constitutive and colligative properties of the chosen agent. The field force generates a force necessary to move the osmotic agent toward and away from the biological membrane surface. The movement of the

osmotic agent modulates the periodic and continuous extraction of body fluid through the stratum corneum.

[0022] In one embodiment, the intensity, duration, and frequency of exposure of biological membrane to osmotic forces may be manipulated by changing the concentration of the osmotic agent that is in contact with the ultrasound-exposed biological membrane. Manipulating the volume of the solvent and the volume of the hydrogel containing the osmotic agent may cause a change in the concentration of the osmotic agent. The volume of the hydrogel can be changed by constructing a hydrogel wherein its volume is sensitive to the concentrations of molecules that can diffuse into the gel. One example is a hydrogel constructed to be sensitive to the molecule glucose. The hydrogel volume can also be changed by manipulating its temperature and by changing the pH of the gel.

[0023] A receiver that is attached to an area of biological membrane with an enhanced permeability and receives body fluid through and out of the area of biological membrane is disclosed. According to one embodiment of the present invention, the receiver includes a first grid; a medium layer comprising at least one agent; a membrane that induces a concentration gradient barrier for the at least one agent; a counter grid; an oxidase layer; a detection layer; and a voltage source that provides a potential difference between the first grid and the counter grid. The body fluid, which may include blood, interstitial fluid, analyte, and lymph, may flow out of, or through, the biological membrane, to the detector layer via the first grid, the counter grid, and the oxidase layer.

[0024] It is a technical advantage of the present invention that a system, method, and device for non-invasive sampling and analysis of body fluids is disclosed. It is another technical advantage of the present invention that a concentration of an analyte may be measured continuously or periodically.

BRIEF DESCRIPTION OF THE DRAWINGS

[0025] For a more complete understanding of the present invention, the objects and advantages thereof, reference is now made to the following descriptions taken in connection with the accompanying drawings in which:

[0026] **FIG. 1** is a flowchart depicting a method for non-invasive body fluid sampling according to one embodiment of the present invention;

[0027] **FIG. 2** depicts a device for controlled application of ultrasound to a biological membrane to enhance the permeability of the biological membrane according to one embodiment of the present invention;

[0028] **FIG. 3** depicts the components to perform discrete extraction and measurement of body fluid to infer analyte concentrations according to one embodiment of the present invention;

[0029] **FIG. 4** depicts the components to perform continuous extraction and measurement of body fluid to infer analyte concentrations according to one embodiment of the present invention;

[0030] **FIG. 5** depicts an approach to periodic monitoring of an analyte by performing periodic osmotic extractions of body fluid according to one embodiment of the present invention;

[0031] **FIG. 6** depicts the components of a wearable extraction chamber according to one embodiment of the present invention; and

[0032] **FIG. 7** depicts a graph of glucose flux versus blood glucose concentration according to one embodiment of the present invention.

DETAILED DESCRIPTION OF THE INVENTION

[0033] The preferred embodiment of the present invention and its advantages are best understood by referring to **FIGS. 1 through 7** of the drawings, like numerals being used for like and corresponding parts of the various drawings.

[0034] As used herein, the term "body fluid" may include blood, interstitial fluid, lymph, and/or analyte. In addition, as used herein, the term "biological membrane" may include tissue, mucous membranes and comified tissues, including skin, buccal, and nails. Further, as used herein, the term "force" may also include force gradients.

[0035] Although the present invention may be described in conjunction with human applications, veterinary applications are within the contemplation and the scope of the present invention.

[0036] Referring to **FIG. 1**, a flowchart depicting a method for non-invasive body fluid sampling and analysis according to one embodiment of the present invention is provided. In step **102**, the permeability of an area of biological membrane is enhanced. In one embodiment, the area of biological membrane may be located on the volar forearm of a mammalian subject. In another embodiment, the area of biological membrane may be located on a thigh of a mammalian subject. In yet another embodiment, the area of biological membrane may be located on the abdomen. In still another embodiment, the area of biological membrane may be located on the back. Other body locations may also be used.

[0037] In general, several techniques may be used to enhance the permeability of the biological membrane, such as creating physical micropores, physically disrupting the lipid bilayers, chemically modifying the lipid bilayers, physically disrupting the stratum corneum, and chemically modifying the stratum corneum. The creation of micropores, or the disruption thereof, may be achieved by physical penetration using a needle, a microneedle, a silicon microneedle, a laser, a laser in combination with an absorbing dye, a heat source, an ultrasonic needle, an ultrasonic transducer, cryogenic ablation, RF ablation, photo-acoustic ablation, and combinations thereof.

[0038] In a preferred embodiment, ultrasound may be applied to the area of biological membrane to enhance its permeability. Ultrasound is generally defined as sound at a frequency of greater than about 20 kHz. Therapeutic ultrasound is typically between 20 kHz and 5 MHz. Near ultrasound is typically about 10 kHz to about 20 kHz. It should be understood that in addition to ultrasound, near ultrasound may be used in embodiments of the present invention.

[0039] In general, ultrasound, or near ultrasound, is preferably applied to the area of biological membrane at a frequency sufficient to cause cavitation and increase the

permeability of the biological membrane. In one embodiment, ultrasound may be applied at a frequency of from about 10 kHz to about 500 kHz. In another embodiment, ultrasound may be applied at a frequency of from about 20 kHz to about 150 kHz. In yet another embodiment, the ultrasound may be applied at 50 kHz. Other frequencies of ultrasound may be applied to enhance the permeability level of the biological membrane.

[0040] In one embodiment, the ultrasound may have an intensity in the range of about 0 to about 100 watt/cm², and preferably in the range of 0 to about 20 watt/cm². Other appropriate intensities may be used as desired.

[0041] Techniques for increasing the permeability of a biological membrane are disclosed in U.S. Pat. No. 6,190,315 to Kost et al., the disclosure of which is hereby incorporated by reference in its entirety.

[0042] In step 104, body fluid is extracted through or out of the area of biological membrane. In one embodiment, an external force, such as an osmotic force, may assist in the extraction. In one embodiment, the osmotic force may be controlled before, during, and after the permeability of the biological membrane is enhanced.

[0043] In one embodiment, the osmotic force may be generated by the application of an osmotic agent to the area of biological membrane. The osmotic agent may be in the form of an element, a molecule, a macromolecule, a chemical compound, or combinations thereof. The osmotic agent may also be combined with a liquid solution, a hydrogel, a gel, or an agent having a similar function.

[0044] In step 106, the magnitude, intensity, and duration of the external force may be regulated by at least one additional first energy and/or force. In one embodiment, the first additional energy and/or force may be applied to control and regulate the movement and function of the osmotic agent for extraction of body fluid through and out of the biological membrane. The first additional energy and/or force may be provided in the form of heat, a temperature force, a pressure force, an electromotive force, a mechanical agitation, ultrasound, iontophoresis, an electromagnetic force, a magnetic force, a photothermal force, a photoacoustic force, and combinations thereof. The effect of an electric field and ultrasound on transdermal drug delivery is disclosed in U.S. Pat. No. 6,041,253, the disclosure of which is incorporated, by reference, in its entirety.

[0045] In one embodiment, if the first additional energy and/or force is provided by ultrasound, the frequency of the ultrasound may be provided at a different frequency than the frequency used to enhance the permeability of the biological membrane. In one embodiment, the frequency of the first additional energy/force ultrasound may be higher than the frequency of the permeability enhancing ultrasound.

[0046] In step 108, the body fluid may be collected in a receiver. In one embodiment, the receiver may be contacted with the biological membrane in a form of a patch, a wearable reservoir, a membrane, an absorbent strip, a hydrogel, or a structure that performs an equivalent function. Other types and configurations of receivers may be used.

[0047] In one embodiment, the receiver may be provided with a secondary receiver having an analyte concentration that is continuously maintained to be substantially lower

than the analyte concentration in the body fluid, so the chemical concentration driving force between body fluid and secondary receiver is maximized. This may be achieved by chemical reaction or volume for dilution or similar means.

[0048] In one embodiment, a second external energy/force may be applied between the first receiver and the secondary receiver. In one embodiment, the second external energy/force may be different (e.g., a different type of external force) from the first external energy/force. In another embodiment, the second external energy/force may be the same (e.g., the same type of external force) as the first external energy/force. The first and second external energy/force may vary in type, duration, and intensity, and may be controlled through different additional energy and/or forces.

[0049] In step 110, the collected body fluid may be analyzed. In one embodiment, the analysis may include the use of appropriate methods, such as electrochemical, biochemical, optical, fluorescence, absorbance, reflectance, Raman, magnetic, mass spectrometry, infra-red (IR) spectroscopy measurement, and combinations thereof.

[0050] In one embodiment, multiple analytes may be analyzed simultaneously, in parallel, or in series. The results from these multiple analyses may be used in combination with algorithms, for example, to increase the accuracy, or precision, or both, of the analysis and measurements.

[0051] In one embodiment, the receiver may be removed from contact with the biological membrane in order to analyze the collected body fluid. In another embodiment, the receiver may remain in contact with the biological membrane as the collected body fluid is analyzed.

[0052] Referring to FIG. 2, a device for the controlled application of ultrasound to biological membrane to enhance the permeability of a biological membrane according to one embodiment of the present invention is shown. Device 200 includes controller 202, which interfaces with ultrasound applicator 204 by any suitable means, such as a cable. Controller 202 controls the application of ultrasound to the area of biological membrane. In one embodiment, ultrasound or near ultrasound having an intensity in the range of about 0 to about 20 watt/cm² may be generated by controller 202 and ultrasound applicator 204. In one embodiment, the ultrasound may have a frequency of about 20 kHz to about 150 kHz. In another embodiment, the ultrasound may have a frequency of 50 kHz. Other ultrasound frequencies may also be used.

[0053] In addition, controller 202 may include a display, such as a LCD or a LED display, in order to convey information to the user as required. Controller 202 may also include a user interface as is known in the art.

[0054] Ultrasound applicator 204 may be provided with cartridge 206, which contains ultrasound coupling solution 208. Cartridge 206 may be made of any material, such as plastic, that may encapsulate ultrasound coupling solution 208. Suitable ultrasound coupling solutions 208 include, but is not limited to, water, saline, alcohols including ethanol and isopropanol (in a concentration range of 10 to 100% in aqueous solution), surfactants such as Triton X-100, SLS, or SDS (preferably in a concentration range of between 0.001 and 10% in aqueous solution), DMSO (preferably in a concentration range of between 10 and 100% in aqueous solution), fatty acids such as linoleic acid (preferably in a

concentration range of between 0.1 and 2% in ethanol-water (50:50) mixture), azone (preferably in a concentration range of between 0.1 and 10% in ethanol-water (50:50) mixture), polyethylene glycol in a concentration range of preferably between 0.1 and 50% in aqueous solution, histamine in a concentration range of preferably between 0.1 and 100 mg/ml in aqueous solution, EDTA in a concentration range of preferably between one and 100 mM, sodium hydroxide in a concentration range of preferably between one and 100 mM, sodium octyl sulfate, N-tauroylsarcosine, octyltrimethyl ammoniumbromide, dodecyltrimethyl ammoniumbromide, tetradecyltrimethyl ammoniumbromide, hexadecyltrimethyl ammoniumbromide, dodecylpyridinium chloride hydrate, SPAN 20, BRIJ 30, glycolic acid ethoxylate 4-terbutyl phenyl ether, IGEPAL CO-210, and combinations thereof.

[0055] In one embodiment, the coupling medium may also include a chemical enhancer. Transport enhancement may be obtained by adding capillary permeability enhancers, for example, histamine, to the coupling medium. The concentration of histamine in the coupling medium may be in the range of between 0.1 and 100 mg/ml. These agents may be delivered across the biological membrane during application of ultrasound and may cause local edema that increases local fluid pressure and may enhance transport of analytes across the biological membrane. In addition, the occurrence of free fluid due to edema may induce cavitation locally so as to enhance transport of analytes across the biological membrane.

[0056] In one embodiment, cartridge 206 may be pierced when inserted into ultrasound applicator 204, and ultrasound coupling solution 208 may be transferred to a chamber (not shown).

[0057] A target identifying device, such as target ring 210, may be attached to the area of biological membrane that will have its permeability increased. Target ring 210 may be attached to the area of biological membrane by a transdermal adhesive (not shown). In one embodiment, target ring 210 may have the transdermal adhesive pre-applied, and may be disposed after each use. In another embodiment, target ring 210 may be reusable.

[0058] Target ring 210 may be made of any suitable material, including plastic, ceramic, rubber, foam, etc. In general, target ring 210 identifies the area of biological membrane for permeability enhancement and body fluid extraction. In one embodiment, target ring 210 may be used to hold receiver 214 in contact with the biological membrane after the permeability of the biological membrane has been increased.

[0059] In one embodiment, target ring 210 may be used to monitor the permeability level of the biological membrane, as disclosed in PCT International Patent Appl'n Ser. No. PCT/US99/30067, entitled "Method and Apparatus for Enhancement of Transdermal Transport," the disclosure of which is incorporated by reference in its entirety. In such an embodiment, target ring 210 may interface with ultrasound applicator 204.

[0060] Ultrasound applicator 204 may be applied to target ring 210 and activated to expose ultrasound coupling solution 208 to the biological membrane. Controller 202 controls ultrasound applicator 204 to transmit ultrasound through

ultrasound coupling solution 208. During ultrasound exposure, controller 202 may monitor changes in biological membrane permeability, and may display this information to the user.

[0061] Controller 202 may cease, or discontinue, the application of ultrasound once a predetermined level of biological membrane permeability is reached. This level of permeability may be preprogrammed, or it may be determined in real-time as the ultrasound is applied. The predetermined level of permeability may be programmed for each individual due to biological membrane differences among individuals.

[0062] After the predetermined level of permeability is reached, ultrasound coupling solution 208 may be vacuated from chamber (not shown) into cartridge 206, which may then be discarded. In another embodiment, ultrasound coupling solution 208 may be vacuated into a holding area (not shown) in ultrasound applicator 204, and later discharged. Ultrasound applicator 204 may then be removed from target ring 210.

[0063] Referring to FIG. 3, an device for the analysis of body fluid according to one embodiment of the present invention is provided. Receiver 214 may be placed into target ring 210 to perform a discrete, or on-demand, extraction of body fluid through and/or out of the biological membrane. Receiver 214 may contain a medium, such as a hydrogel layer, that incorporates an osmotic agent. In one embodiment, the hydrogel may be formulated to contain phosphate buffered saline (PBS), with the saline being sodium chloride having a concentration range of about 0.01 M to about 10 M. The hydrogel may be buffered at pH 7. Other osmotic agents may also be used in place of, or in addition to, sodium chloride. Preferably, these osmotic agents are non-irritating, non-staining, and non-immunogenic. Examples of such osmotic agents include, inter alia, lactate and magnesium sulfate.

[0064] In another embodiment, receiver 214 may include a fluid or liquid medium, such as water or a buffer, that is contained within a semi-permeable membrane. Receiver 214 may also include a spongy material, such as foam.

[0065] Receiver 214 may be applied to the biological membrane to contact the ultrasound exposed biological membrane. In one embodiment, receiver 214 may be applied to the biological membrane for a time period sufficient to collect an amount of body fluid sufficient for detection. In another embodiment, receiver 214 may be applied to the biological membrane for a sufficient time period to collect a predetermined amount of body fluid. In yet another embodiment, receiver 214 may be applied to the biological membrane for a predetermined time. In one embodiment, the contact between receiver 214 and the biological membrane may last for 15 minutes or less. In another embodiment, the contact between receiver 214 and the biological membrane may last for 5 minutes or less. In still another embodiment, the contact between receiver 214 and the biological membrane may last for 2 minutes or less. The actual duration of contact may depend on the sensitivity of the detection method used for analysis.

[0066] In one embodiment, the medium of receiver 214 may contain at least one reagent (not shown) in order to detect the presence of certain analytes in the body fluid that

has been extracted from or through the biological membrane. In one embodiment, the hydrogel layer of receiver **214** may contain the reagents, and the reagents may be attached to the hydrogel by ionic and/or covalent means, or may be immobilized by gel entrapment. The reagents may also be arranged as an adjacent layer to the hydrogel wherein the analyte from the body fluid that has been extracted into the hydrogel can diffuse into and react to generate by-products. The by-products may then be detected using electrochemical, biochemical, optical, fluorescence, absorbance, reflectance, Raman, magnetic, mass spectrometry, IR spectroscopy measurement methods and combinations thereof.

[0067] The detection methods may be performed by meter **212**. Meter **212** may include a processor (not shown) and a display, such as an LCD display. Other suitable displays may be provided.

[0068] In one embodiment, meter **212** may provide an interface that allows information be downloaded to an external device, such as a computer. Such an interface may allow the connection of interface cables, or it may be a wireless interface.

[0069] Meter **212** may be configured to determine body fluid glucose concentration by incorporating glucose oxidase in the medium of receiver **214**. In one embodiment, glucose from extracted body fluid may react with glucose oxidase to generate hydrogen peroxide. Hydrogen peroxide may be detected by the oxidation of hydrogen peroxide at the surface of electrodes incorporated into receiver **214**. The oxidation of hydrogen peroxide transfers electrons onto the electrode surface which generates a current flow that can be quantified using a potentiostat, which may be incorporated into meter **212**. A glucose concentration proportional to the concentration of hydrogen peroxide may be calculated, and the result may be reported to the user via a display. Various configurations of electrodes and reagents, known to those of ordinary skill in the art, may be incorporated to perform detection and analysis of glucose and other analytes.

[0070] Meter **212** may also be configured to simultaneously measure the concentration of an analyte, such as glucose, where the body fluid concentration is expected to fluctuate, and an analyte, like creatinine or calcium, where the body fluid concentration is expected to remain relatively stable over minutes, hours, or days. An analyte concentration, which may be determined by an algorithm that takes into account the relative concentrations of the fluctuating and the more stable analyte, may be reported to the user via a display.

[0071] In another embodiment, meter **212** may analyze multiple analytes simultaneously, in parallel, or in series. The results from these multiple analyses may be used in combination with algorithms, for example, to increase the accuracy, or precision, or both, of the analysis and measurements.

[0072] Receiver **214** may be discarded after the extraction and measurement steps. In another embodiment, receiver **214** may be reused. In one embodiment, receiver **214** may be cleaned, sanitized, etc. before it may be reused. Various configurations of electrodes and reagents, known to those of ordinary skill in the art, may be incorporated to perform detection and analysis of glucose and other analytes.

[0073] Referring to **FIG. 4**, an device for the continuous extraction and analysis of body fluid to infer analyte concentrations according to another embodiment of the present invention is provided. As shown in the figure, a biological membrane site on the forearm, the abdomen, or thigh may be exposed to ultrasound; other biological membrane sites, such as those on the back, may also be used. Receiver **402**, which may be similar to receiver **214**, may contact the ultrasound exposed biological membrane site to perform continuous extraction of body fluid. In one embodiment, receiver **402** may contain a medium, such as a hydrogel layer, that may incorporate an osmotic agent, such as sodium chloride. The hydrogel is formulated to contain phosphate buffered saline (PBS), with the saline being sodium chloride in the concentration range of 0.01 M to 10 M. The hydrogel may be buffered at pH 7.

[0074] Other osmotic agents may also be used in place of, or in addition to, sodium chloride. These osmotic agents are preferably non-irritating, non-staining, and non-immunogenic. Examples of these other osmotic agents may include, inter alia, lactate and magnesium sulfate. Receiver **402** may be applied to contact the ultrasound exposed biological membrane. In one embodiment, the duration of this contact may be 12-24 hours, or more. In another embodiment, other durations of contact, including substantially shorter durations, and substantially longer durations, may be used as desired.

[0075] In another embodiment, receiver **402** may include a fluid or liquid medium, such as water or a buffer, that is contained within a semi-permeable membrane. Receiver **402** may also include a spongy material, such as foam.

[0076] In one embodiment, the medium of receiver **402** may contain at least one reagent (not shown) that detects the presence of analytes in the body fluid that has been extracted thorough and out of the biological membrane. In one embodiment, the hydrogel layer of receiver **402** may contain reagents that may be attached by ionic and covalent means to the hydrogel, or may be immobilized by gel entrapment. The reagents may also be arranged as an adjacent layer to the hydrogel wherein the analyte from the body fluid that has been extracted into the hydrogel may diffuse into and react to generate by-products. The by-products may be detected using electrochemical, biochemical, optical, fluorescence, absorbance, reflectance, Raman, magnetic, mass spectrometry, IR spectroscopy measurement methods and combinations thereof.

[0077] The detection methods and results may be performed and presented to the user by meter **404**, which may be similar in function to meter **212**, discussed above. In one embodiment, meter **404** may be wearable. For example, as depicted in the figure, meter **404** may be worn a manner similar to the way a wristwatch is worn. Meter **404** may also be worn on a belt, in a pocket, etc.

[0078] Meter **404** may incorporate power and electronics to control the periodic extraction of body fluid, to detect analyte, and to present the analyte concentration in a continuous manner. Meter **404** may contain electronics and software for the acquisition of sensor signals, and may perform signal processing, and may store analysis and trending information.

[0079] In one embodiment, meter **404** may provide an interface that allows information be downloaded to an

external device, such as a computer. Such an interface may allow the connection of interface cables, or it may be a wireless interface.

[0080] Meter **404** may be configured to determine body fluid glucose concentration by incorporating glucose oxidase in the medium. In one embodiment, glucose from extracted body fluid may react with glucose oxidase to generate hydrogen peroxide. Hydrogen peroxide may be detected by the oxidation of hydrogen peroxide at the surface of electrodes incorporated into receiver **402**. The oxidation of hydrogen peroxide transfers electrons onto the electrode surface which generates a current flow that can be quantified using a potentiostat, which may be incorporated into meter **404**. A glucose concentration proportional to the concentration of hydrogen peroxide may be calculated and the result may be reported to the user via a display. Various configurations of electrodes and reagents, known to those of ordinary skill in the art, may be incorporated to perform detection and analysis of glucose and other analytes.

[0081] In one embodiment, meter **404** may also be configured to simultaneously measure concentration of an analyte, such as glucose, where the body fluid concentration is expected to fluctuate, and an analyte, like creatinine or calcium, where the body fluid concentration is expected to remain relatively stable over minutes, hours, or days. An analyte concentration, which may be determined by an algorithm that takes into account the relative concentrations of the fluctuating and the more stable analyte, may be reported to the user via a display.

[0082] In another embodiment, meter **404** may analyze multiple analytes simultaneously, in parallel, or in series. The results from these multiple analyses may be used in combination with algorithms, for example, to increase the accuracy, or precision, or both, of the analysis and measurements.

[0083] In another embodiment, receiver **402** may be removed from contact with the biological membrane for analysis by meter **404**. Receiver **402** may be put in contact with the biological membrane after such analysis.

[0084] Meter **404** may provide analyte readings to the user in a periodic or a continuous manner. For example, in one embodiment, in continuous monitoring of the analyte glucose, glucose concentration may be displayed to the user every 30 minutes, more preferably every 15 minutes, most preferable every 5 minutes, or even more frequently. In another embodiment, the glucose concentration may be displayed continuously. The period may depend on the sensitivity and method of analyte detection. In continuous glucose monitoring, in one embodiment, glucose detection may be performed by an electrochemical method using electrodes and reagents incorporated into receiver **402** and detection and analysis performed by meter **404**. During the measurement period, osmotic extraction of body fluid may be performed continuously by the hydrogel layer of receiver **402**. Body fluid may accumulate in the hydrogel of receiver **402**. Glucose in body fluid diffuses to react with glucose oxidase and is converted into hydrogen peroxide. The hydrogen peroxide is consumed by poisoning the working electrode with respect to a reference electrode. During the resting period, hydrogen peroxide accumulates and is consumed or destroyed before the measuring period. The magnitude of the working potential can be applied to rapidly consume the build up of hydrogen peroxide.

[0085] Referring to **FIG. 5**, an approach to periodic monitoring of an analyte by performing periodic osmotic extractions of body fluid according to another embodiment of the present invention is shown. The osmotic extraction intensity and frequency may be manipulated by using an osmotic agent that dissociates into multiple charged species, and an electrical potential may be used to move the concentration of charges toward and away from biological membrane surface **550**. Receiver **500** may include grid, mesh, or screen **504**; medium **506**, which may be a hydrogel layer; membrane **508**; counter grid, mesh, or screen **510**; oxidase layer **512**; and detection layer **514**. Grid **504** and counter grid **510** may be connected to voltage source **516**. Membrane **508** may be a semi-permeable membrane that is used to induce a concentration gradient barrier for the osmotic agent contained in medium **506**. The preferable osmotic agent may contain negative and positive species or counter ions. Manipulating the concentration of charged species at the boundary adjacent to the stratum corneum of the ultrasound-exposed biological membrane may provide periodic extraction of body fluid.

[0086] In one embodiment, receiver **500** may make contact with the skin through contact medium **502**, which may be a hydrogel, or other suitable medium.

[0087] The concentration of the charged species may be manipulated by applying a potential difference between grid **504** and counter grid **510** using voltage source **516**. In one embodiment, the potential difference may be of a magnitude that is sufficient to manipulate the osmotic agent. The polarity of the grid may also be changed to transport charges toward and away from biological membrane surface **550**. Grid **504** and counter grid **510** may be configured with optimum porosity as to allow body fluid and/or analyte to travel out of stratum corneum, through grid **504**, through grid **510**, and into oxidase layer **512**, and ultimately to detection layer **514**. Oxidase layer **512** may be used with an appropriate catalyst, or enzyme, to confer specificity of analyte detection. Detection layer **514** may include working and reference electrodes (not shown) that allow for the detection of the by-products of oxidase layer **512** to quantify the concentration of the desired analyte of detection.

EXAMPLE

[0088] In order to better understand the present invention, an example is provided. The example does not limit the present invention in any way, and is intended to illustrate an embodiment of the present invention.

[0089] The following is a description of experiments which implemented painless extraction, collection, and analysis of body fluid to determine body fluid glucose concentration in a human using a hyperosmotic extraction fluid and comparing this condition with iso-osmotic extraction fluid, in accordance with one embodiment of the present invention. Although body fluid glucose concentration serves as an example to demonstrate feasibility, other analytes are within the contemplation of the present invention. In addition, multiple analytes may be measured and/or analyzed simultaneously, in parallel, or in series, and results from these multiple measurements may be used in combination with algorithms, for example, to increase the accuracy or precision or both of measurements. As may be recognized by one of ordinary skill in the art, these steps may be automated and implemented with the device described above.

[0090] Four sites on the volar forearm of a human volunteer were treated with ultrasound using the device described in FIG. 2. The ultrasound transducer and its housing were placed on the volar forearm of the volunteer with enough pressure to produce a good contact between the skin and the outer transducer housing, and to prevent leaking. The area surrounding the transducer was then filled with a coupling medium of sodium dodecyl sulfate and silica particles in phosphate-buffered saline (PBS). Ultrasound was briefly applied (5-30 s), the transducer apparatus was removed from the biological membrane, and the skin was rinsed with tap water and dried.

[0091] FIG. 6 describes the components of wearable extraction chamber 600. Four extraction chambers were placed on each sonicated site of the human volunteer. Thin circular foam chamber 602 was constructed using foam MED 5636 Avery Dennison ($\frac{7}{16}$ " ID \times $1\frac{1}{8}$ " OD). Foam chambers 602 were attached concentrically to the sonicated biological membrane sites using double-sided adhesive (Adhesive Arcade 8570, $\frac{7}{16}$ " ID \times $\frac{7}{8}$ " OD) attached to one side of element 602. The other side of foam chamber 602 was attached concentrically to double-sided adhesive 604 (Adhesive Arcade 8570, $\frac{7}{16}$ " ID \times $\frac{7}{8}$ " OD). Thin transparent lid 606 was made of 3M Polyester 1012 ($1\frac{1}{8}$ " \times $1\frac{1}{8}$ "). Double-sided adhesive 604 permitted thin transparent lid 606 to be attached to foam chamber 602 after placement of liquid into the inner diameter of foam chamber 602 when attached to biological membrane. Thin transparent lid 606 acted as a lid to prevent liquid from leaking out of the extraction chamber, and to allow the extraction chambers to be wearable for an extended period of time.

[0092] Each extraction chamber was alternately filled with 100 μ l of extraction solution for 15 min and 100 μ l hydration solution for 10-40 min. Extraction solution was PBS; on two sites the PBS contained additional NaCl to bring the total concentration of NaCl to 1 M. Hydration solution was PBS for all sites.

[0093] Solutions were collected and analyzed for glucose concentration using high-pressure liquid chromatography. The results of the HPLC concentration were normalized for the injection amount and the total solution volume, and were reported as glucose flux (Q_g), the mass of glucose that crossed the sonicated site per unit time per unit area. Body fluid glucose concentrations (C_{bg}) were obtained by testing capillary blood obtained from a lanced finger in a Bayer Glucometer Elite meter. It was hypothesized that Q_g would be linearly proportional to C_{bg} . FIG. 7 shows a graph of Q_g versus C_{bg} . Unexpectedly, Q_g from the sonicated sites exposed to 1 M NaCl correlated to C_{bg} much more strongly than Q_g from the sonicated sites exposed to 0.15 M NaCl.

[0094] Other embodiments and uses of the invention will be apparent to those skilled in the art from consideration of the specification and practice of the invention disclosed herein. All references cited herein, including all U.S. and foreign patents and patent applications, are specifically and entirely hereby incorporated herein by reference. It is intended that the specification and examples be considered exemplary only, with the true scope and spirit of the invention indicated by the following claims.

1. A method for non-invasive body fluid sampling and analysis, comprising:

identifying an area of biological membrane having a permeability level;

increasing the permeability level of the area of biological membrane;

contacting the area of biological membrane with a receiver;

extracting body fluid through and out of the area of biological membrane;

providing an external force to enhance the body fluid extraction;

collecting the body fluid in the receiver;

analyzing the collected body fluid for the presence of at least one analyte; and

providing the results of the step of analyzing the body fluid.

2. The method of claim 1, wherein the step of identifying an area of biological membrane having a permeability level comprises:

providing a target identifying device to the area of biological membrane.

3. The method of claim 1, wherein the step of increasing the permeability level of the area of biological membrane comprises:

applying ultrasound having a frequency range of from about 10 kHz to about 500 kHz to the area of biological membrane.

4. The method of claim 1, wherein the step of increasing the permeability level of the area of biological membrane comprises:

applying ultrasound having a frequency range of from about 20 kHz to about 150 kHz to the area of biological membrane.

5. The method of claim 1, wherein the step of increasing the permeability level of the area of biological membrane comprises:

applying ultrasound having a frequency of about 50 kHz to the area of biological membrane.

6. The method of claim 1, wherein the step of increasing the permeability level of the area of biological membrane comprises:

increasing the permeability level of the area of biological membrane to a predetermined level.

7. The method of claim 1, wherein the step of increasing the permeability level of the area of biological membrane comprises:

increasing the permeability level of the biological membrane with a method selected from the group consisting of: creating physical micropores in the area of biological membrane; physically disrupting lipid bilayers in the area of biological membrane; chemically modifying lipid bilayers in the area of biological membrane; physically disrupting the stratum corneum in the area of biological membrane; and chemically modifying the stratum corneum in the area of biological membrane.

8. The method of claim 1, further comprising the steps of: providing the receiver with a second receiver, the second receiver having a concentration of the at least one analyte; and maintaining the concentration of the at least one analyte in the second receiver at a level that is lower than a concentration of the at least one analyte in the body fluid.
9. The method of claim 8, further comprising the step of: providing a second external force to the second receiver.
10. The method of claim 9, wherein the first external force and the second external force differ in at least one of a type, duration, and an intensity.
11. The method of claim 1, wherein the step of providing an external force to enhance the body fluid extraction comprises: generating at least one osmotic force to enhance the body fluid extraction.
12. The method of claim 11, wherein the step of generating at least one osmotic force to enhance the body fluid extraction comprises: generating the at least one osmotic force by applying at least one osmotic agent to the area of biological membrane.
13. The method of claim 11, wherein the step of generating at least one osmotic force to enhance the body fluid extraction comprises: regulating the at least one osmotic force with an external force selected from the group consisting of heat, a temperature force, a pressure force, an electromotive force, mechanical agitation, ultrasound, iontophoresis, an electromagnetic force, a magnetic force, a photo-thermal force, a photoacoustic force, and combinations thereof.
14. The method of claim 11, wherein the step of generating at least one osmotic force to enhance the body fluid extraction comprises: manipulating at least one of an intensity of the at least one osmotic force, a duration of the at least one osmotic force, and a frequency of the at least one osmotic force with an external force.
15. The method of claim 14, wherein the external force is generated by a method selected from the group consisting of: applying an electric field force, applying a magnetic field force; applying an electromagnetic field force; applying a chemical; adjusting a molarity of the at least one osmotic agent; adjusting a pH level of the at least one osmotic agent; applying an ultrasonic field force; applying an electroosmotic field force; applying an iontophoretic field force; applying an electroporatic field force; and combinations thereof.
16. The method of claim 1, wherein the step of analyzing the body fluid for the presence of at least one analyte comprises: providing the receiver with at least one reagent to detect the at least one analyte.
17. The method of claim 1, wherein the step of analyzing the body fluid for the presence of at least one analyte comprises: using a method selected from the group consisting of electrochemical, biochemical, optical, fluorescence, absorbance, reflectance, Raman, magnetic, mass spectrometry, IR spectroscopy measurement methods, and combinations thereof to detect the presence of the at least one analyte.
18. The method of claim 1, wherein the step of analyzing the body fluid for the presence of at least one analyte comprises: providing a meter to analyze the body fluid using a method selected from the group consisting of electrochemical, biochemical, optical, fluorescence, absorbance, reflectance, Raman, magnetic, mass spectrometry, IR spectroscopy measurement methods, and combinations thereof to detect the presence of the at least one analyte.
19. The method of claim 1, wherein the step of analyzing the collected body fluid for the presence of at least one analyte comprises: periodically analyzing the collected body fluid for the presence of at least one analyte.
20. The method of claim 1, wherein the step of analyzing the collected body fluid for the presence of at least one analyte comprises: continuously analyzing the collected body fluid for the presence of at least one analyte.
21. The method of claim 1, wherein the step of analyzing the collected body fluid for the presence of at least one analyte comprises: determining a concentration of the at least one analyte in the body fluid.
22. The method of claim 1, wherein the step of analyzing the collected body fluid for the presence of at least one analyte comprises: determining a concentration of the at least one analyte in the body fluid based on a concentration of a plurality of analytes in the body fluid.
23. The method of claim 1, further comprising the step of removing the receiver from the area of biological membrane after a predetermined condition.
24. The method of claim 23, wherein the step of removing the receiver from the area of biological membrane after a predetermined condition comprises: removing the receiver from the area of biological membrane after an amount of body fluid sufficient for analysis is collected in the receiver.
25. The method of claim 23, wherein the step of removing the receiver from the area of biological membrane after a predetermined condition comprises: removing the receiver from the area of biological membrane within 15 minutes after the receiver contacts the area of biological membrane.
26. The method of claim 23, wherein the step of removing the receiver from the area of biological membrane after a predetermined condition comprises: removing the receiver from the area of biological membrane within 10 minutes after the receiver contacts the area of biological membrane.
27. The method of claim 23, wherein the step of removing the receiver from the area of biological membrane after a predetermined condition comprises:

- removing the receiver from the area of biological membrane within 5 minutes after the receiver contacts the area of biological membrane.
- 28.** The method of claim 1, wherein the step of providing the results of the step of analyzing the body fluid comprises:
- displaying the results of the step of analyzing the body fluid.
- 29.** A system for non-invasive body fluid sampling and analysis comprising:
- a controller that controls the generation of ultrasound;
 - an ultrasonic applicator that applies the ultrasound to an area of biological membrane;
 - a receiver that contacts the area of biological membrane and receives body fluid through and out of the area of biological membrane, the receiver comprising:
 - a membrane; and
 - a medium contained in the membrane; and
 - a meter that interacts with the receiver and detects the presence of at least one analyte in the body fluid in the receiver.
- 30.** The system of claim 29, wherein the controller comprises:
- a device that measures the permeability level of the area of biological membrane.
- 31.** The system of claim 29, further comprising:
- a cartridge containing an ultrasonic coupling solution that is inserted into the ultrasound applicator.
- 32.** The system of claim 31, wherein the ultrasonic applicator comprises:
- a cartridge chamber that receives the cartridge; and
 - a solution chamber that receives the ultrasonic coupling solution from the cartridge.
- 33.** The system of claim 29, wherein the medium comprises at least one osmotic agent and at least one of a hydrogel layer, a fluid, and a liquid.
- 34.** The system of claim 33, wherein the osmotic agent comprises:
- at least one of sodium chloride, lactate, and magnesium sulfate.
- 35.** The system of claim 33, wherein the medium further comprises:
- at least one reagent.
- 36.** The system of claim 29, wherein the meter comprises:
- a processor; and
 - a device that detects the presence of the analyte selected from the group consisting of: an electrochemical detector; a biochemical detector; a fluorescence detector; an absorbance detector; a reflectance detector; a Raman detector; a magnetic detector; a mass spectrometry detector; an IR spectroscopy detector; and combinations thereof.
- 37.** The system of claim 29, wherein the meter comprises a display that displays an analyte concentration.
- 38.** The system of claim 29, further comprising:
- a device that provides a first additional energy/force to the area of biological membrane.
- 39.** The system of claim 29, further comprising:
- a target ring that is attached to the area of biological membrane.
- 40.** The system of claim 29, wherein the target ring is preapplied with an adhesive.
- 41.** The system of claim 38, further comprising:
- a second receiver in communication with the receiver and having a concentration of the at least one analyte;
- wherein the concentration of the at least one analyte in the second receiver is maintained at a level that is lower than a concentration of the at least one analyte in the body fluid.
- 42.** The system of claim 41, further comprising:
- a device that provides a second additional energy/force to the receiver.
- 43.** The system of claim 42, wherein the first additional energy/force and the second additional energy/force differ in at least one of a type, a duration, and an intensity.
- 44.** The system of claim 29, wherein the meter is wearable.
- 45.** A method for noninvasive body fluid sampling and analysis, comprising:
- enhancing a permeability level of an area of biological membrane;
 - attaching a receiver to the area of biological membrane;
 - extracting a body fluid through and out of the area of biological membrane;
 - collecting the body fluid in the receiver; and
 - determining a concentration of at least one analyte in the body fluid.
- 46.** The method of claim 45, wherein the step of attaching a receiver to the area of biological membrane comprises:
- using an adhesive to contact the receiver to the area of biological membrane.
- 47.** The method of claim 45, wherein the step of determining a concentration of at least one analyte in the body fluid comprises:
- using a method selected from the group consisting of electrochemical, biochemical, optical, fluorescence, absorbance, reflectance, Raman, magnetic, mass spectrometry, IR spectroscopy measurement methods, and combinations thereof to detect the presence of the at least one analyte.
- 48.** The method of claim 45, wherein the step of determining a concentration of at least one analyte in the body fluid comprises:
- providing a meter to analyze the body fluid using a method selected from the group consisting of electrochemical, biochemical, optical, fluorescence, absorbance, reflectance, Raman, magnetic, mass spectrometry, IR spectroscopy measurement methods, and combinations thereof to detect the presence of the at least one analyte.
- 49.** The method of claim 48, further comprising the step of:
- wearing the meter.

50. The method of claim 45, wherein the step of determining a concentration of at least one analyte in the body fluid comprises:

continuously determining the concentration of at least one analyte in the body fluid.

51. The method of claim 45, wherein the step of determining a concentration of at least one analyte in the body fluid comprises:

periodically determining the concentration of at least one analyte in the body fluid.

52. The method of claim 45, wherein the step of determining a concentration of at least one analyte in the body fluid comprises:

determining the concentration of the at least one analyte in the body fluid based on a concentration of a plurality of analytes in the body fluid.

53. The method of claim 45, further comprising:

displaying the concentration of the at least one analyte.

54. The method of claim 45, wherein the step of attaching a receiver to the area of biological membrane comprises:

attaching the receiver to the area of biological membrane for at least 24 hours.

55. The method of claim 45, wherein the step of attaching a receiver to the area of biological membrane comprises:

attaching the receiver to the area of biological membrane for at least 12 hours.

56. The method of claim 45, wherein the step of attaching a receiver to the area of biological membrane comprises:

attaching the receiver to the area of biological membrane for at least 6 hours.

57. The method of claim 45, wherein the step of attaching a receiver to the area of biological membrane comprises:

attaching the receiver to the area of biological membrane for at least 2 hours.

58. A device for noninvasive body fluid sampling and analysis, comprising:

a receiver that is attached to an area of biological membrane with an enhanced permeability and receives body fluid through and out of the area of biological membrane, the receiver comprising:

a membrane; and

a medium contained in the membrane; and

wearable meter that detects the presence of at least one analyte in the received body fluid and indicates a concentration of that analyte, the wearable meter comprising:

a processor; and

a device that detects the presence of the analyte selected from the group consisting of: an electrochemical detector; a biochemical detector; a fluorescence detector; an absorbance detector; a reflectance detector; a Raman detector; a magnetic detector; a mass spectrometry detector; an IR spectroscopy detector; and combinations thereof.

59. The device of claim 58, wherein the medium comprises:

at least one osmotic agent and at least one of a hydrogel layer, a fluid, and a liquid.

60. The device of claim 59, wherein the osmotic agent comprises:

at least one of sodium chloride, lactate, and magnesium sulfate.

61. The device of claim 59, wherein the medium further comprises:

at least one reagent.

62. The device of claim 58, wherein the wearable meter further comprises:

a display that displays an analyte concentration.

63. The device of claim 58, wherein the receiver further comprises:

a transdermal adhesive.

64. A receiver that is attached to an area of biological membrane with an enhanced permeability and receives body fluid through and out of the area of biological membrane, the receiver comprising:

a first grid;

a medium layer comprising at least one agent;

a membrane that induces a concentration gradient barrier for the at least one agent;

a counter grid;

an oxidase layer;

a detection layer; and

a voltage source that provides a potential difference between the first grid and the counter grid;

wherein the body fluid flows out of or through the biological membrane to the detector layer via the first grid, the counter grid, and the oxidase layer.

65. The receiver of claim 64, wherein the body fluid comprises at least one of blood, interstitial fluid, analyte, and lymph.

66. The receiver of claim 64, wherein the medium layer comprises at least one of a hydrogel and a liquid.

67. The receiver of claim 64, wherein the at least one agent comprises an osmotic agent.

68. The receiver of claim 67, wherein the osmotic agent comprises negative and positive charged species.

69. The receiver of claim 68, wherein a concentration of the charged species can be changed with the voltage source.

70. The receiver of claim 64, wherein the oxidase layer comprises:

at least one catalyst or enzyme that to detect at least one analyte.

71. The receiver of claim 64, wherein the detection layer further comprises:

at least one working electrode; and

at least one reference electrode;

wherein the at least one working electrode and the at least one reference electrode allow for the detection of the by-products of the oxidase layer to quantify a concentration of the desired analyte of detection.

专利名称(译)	用于非侵入性体液采样和分析的系统，方法和装置		
公开(公告)号	US20030100846A1	公开(公告)日	2003-05-29
申请号	US09/979096	申请日	2001-03-16
[标]申请(专利权)人(译)	CUSTER LINDA ELSTROM TUAN 一个 KELLOGG SCOTT C KOST JOSEPH WARNER NICHOLAS F		
申请(专利权)人(译)	CUSTER LINDA ELSTROM TUAN A. KELLOGG SCOTT C. KOST JOSEPH WARNER NICHOLAS F.		
当前申请(专利权)人(译)	CUSTER LINDA ELSTROM TUAN A. KELLOGG SCOTT C. KOST JOSEPH WARNER NICHOLAS F.		
[标]发明人	CUSTER LINDA ELSTROM TUAN A KELLOGG SCOTT C KOST JOSEPH WARNER NICHOLAS F		
发明人	CUSTER, LINDA ELSTROM, TUAN A. KELLOGG, SCOTT C. KOST, JOSEPH WARNER, NICHOLAS F.		
IPC分类号	A61B5/00 A61B5/15 A61B8/00 A61B10/00 A61M25/02 A61M37/00		
CPC分类号	A61B5/1405 A61B5/14514 A61B5/14532 A61B8/00 A61M2025/0206 A61B2010/008 A61M25/02 A61M37/0092 A61B10/0045 A61B5/150022 A61B5/150083 A61B5/150358 A61B5/150755 A61B5 /15087 A61B5/150969 A61B5/15134 A61B5/157		
优先权	60/142951 1999-07-12 US 60/142941 1999-07-12 US 60/142975 1999-07-12 US 60/070813 1998-01-08 US 60/189971 2000-03-17 US 60/142950 1999-07-12 US 60/112953 1998-12-18 US PCT/US1999/030065 1999-12-17 WO		
其他公开文献	US7066884		
外部链接	Espacenet USPTO		
摘要(译)			

提供了一种用于非侵入性体液采样的系统，方法和设备。根据本发明的一个实施例，该系统包括控制超声波产生的控制器；超声波施加器，将超声波应用于生物膜区域；接收器，其接触生物膜区域并接收通过和离开生物膜区域的体液；和一个与接收器相互作用并检测接收器体液中至少有一种分析物存在的仪表。接收器可包括膜和包含在膜中的介质，例如水凝胶，流体或液体。根据本发明的一个实施方案，该方法包括以下步骤：
(1) 鉴定具有渗透性水平的生物膜的区域；(2) 提高生物膜面积的渗透性水平；(3) 将生物膜区域与接收器接触；(4) 通过生物膜区域提取体液；(5) 提供外力以增强体液提取；(6) 收集接收器中的体液；(7) 分析收集的体液中是否存在至少一种分析物；(8) 提供分析体液的结果。

