



US 20130338456A1

(19) **United States**(12) **Patent Application Publication**
Ellingsen et al.(10) **Pub. No.: US 2013/0338456 A1**(43) **Pub. Date: Dec. 19, 2013**(54) **SENSOR DEVICE FOR SENSING BODY
FLUID DENSITY AND/OR MEMBRANE
RESISTANCE****Publication Classification**(51) **Int. Cl.***A61B 5/00* (2006.01)*A61B 5/01* (2006.01)*A61B 7/00* (2006.01)*A61B 5/11* (2006.01)*A61B 5/145* (2006.01)*A61B 5/1455* (2006.01)(52) **U.S. Cl.**CPC *A61B 5/7278* (2013.01); *A61B 5/14532*
(2013.01); *A61B 5/7225* (2013.01); *A61B*
5/442 (2013.01); *A61B 5/443* (2013.01); *A61B*
5/1455 (2013.01); *A61B 7/00* (2013.01); *A61B*
5/11 (2013.01); *A61B 5/01* (2013.01)

USPC 600/316; 600/365

(75) Inventors: **Olav Ellingsen**, Oslo (NO); **Bjarte**
Sorebo Ellingsen, Oslo (NO)(73) Assignee: **MECSENSE AS**, OSLO (NO)(21) Appl. No.: **13/979,348**(22) PCT Filed: **Jan. 12, 2012**(86) PCT No.: **PCT/NO12/00003**

§ 371 (c)(1),


(2), (4) Date: **Sep. 4, 2013**(30) **Foreign Application Priority Data**

Jan. 12, 2011 (NO) 20110070

(57)

ABSTRACT

The present invention relates to a sensor device for measuring tensile variation against a membrane separating a liquid such as the skin on humans and animals and any other membrane separating a liquid on one of its sides.

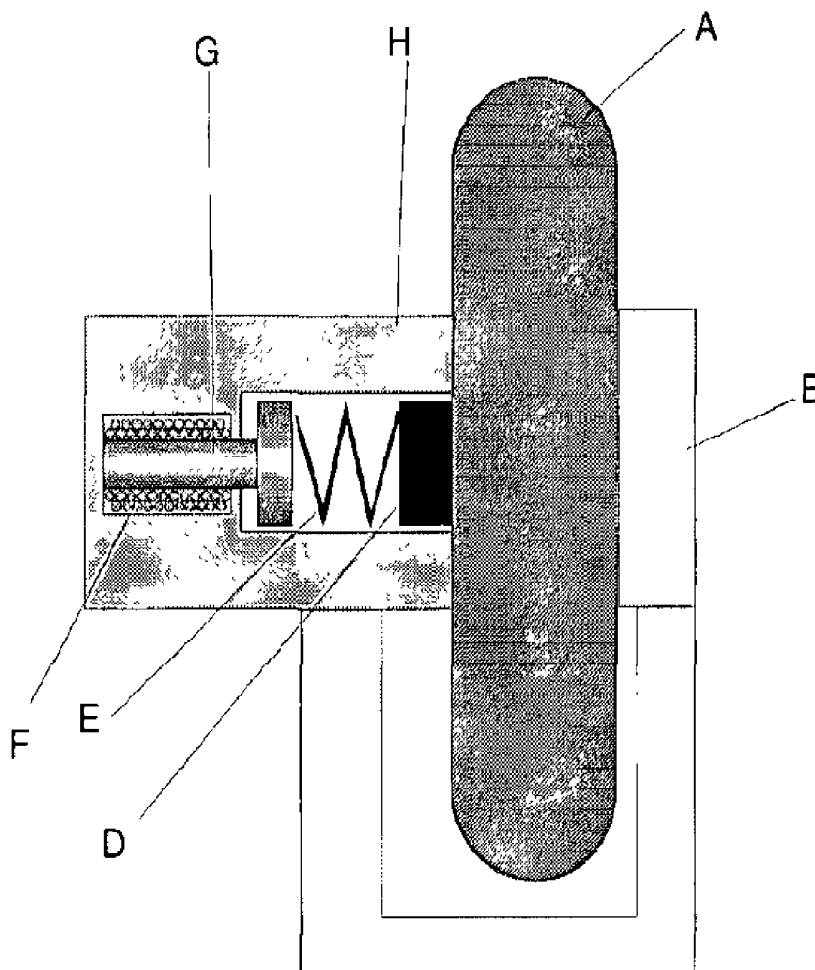

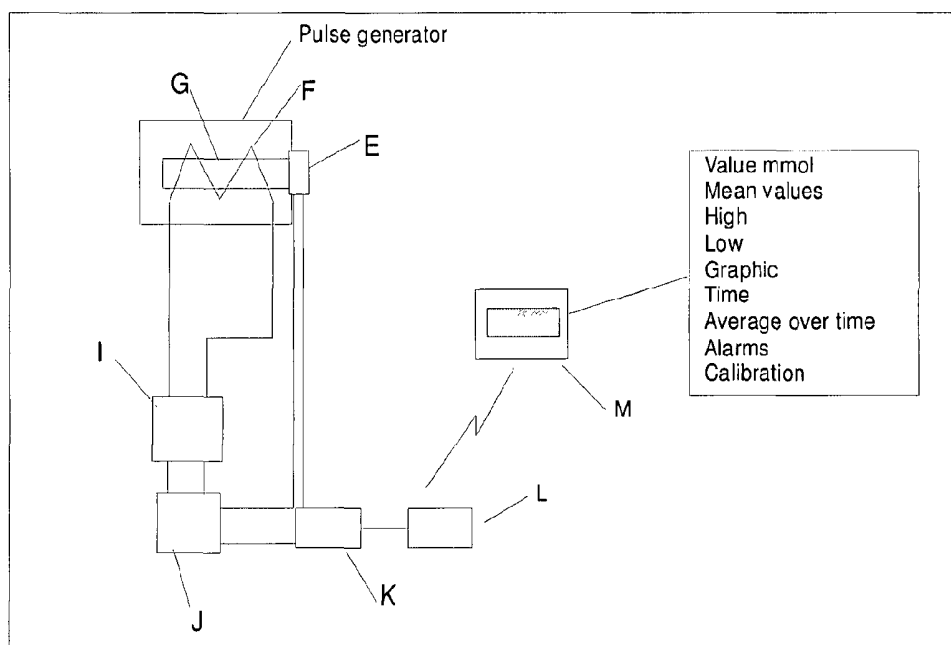
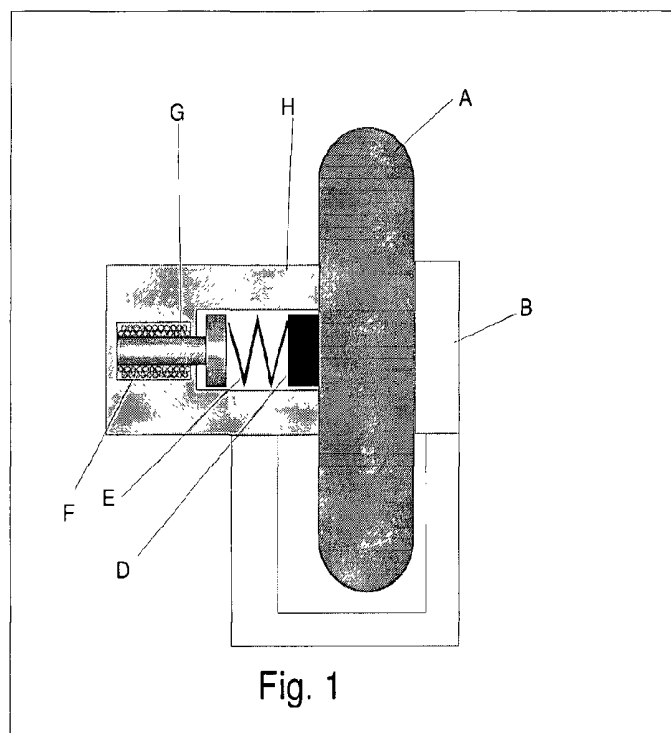
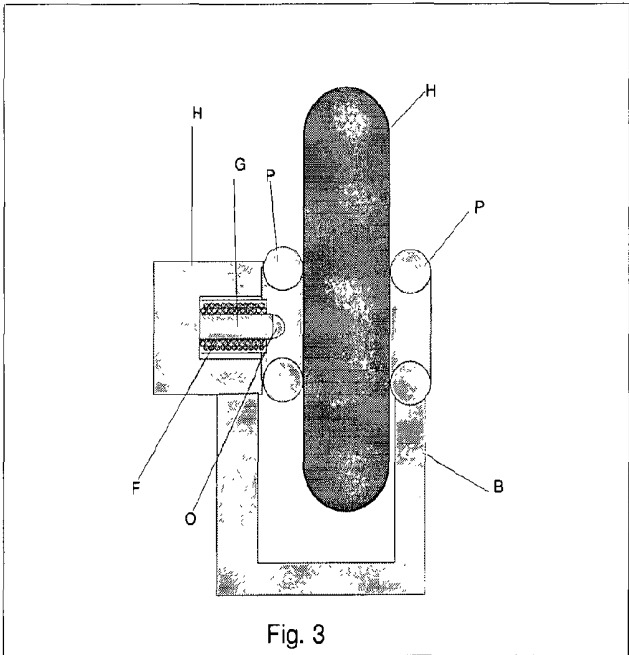
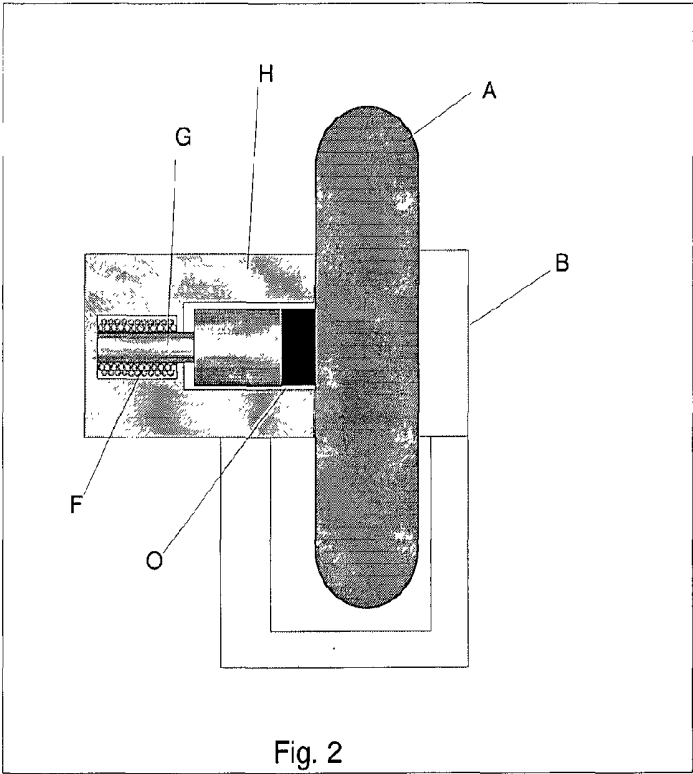


Fig. 1A



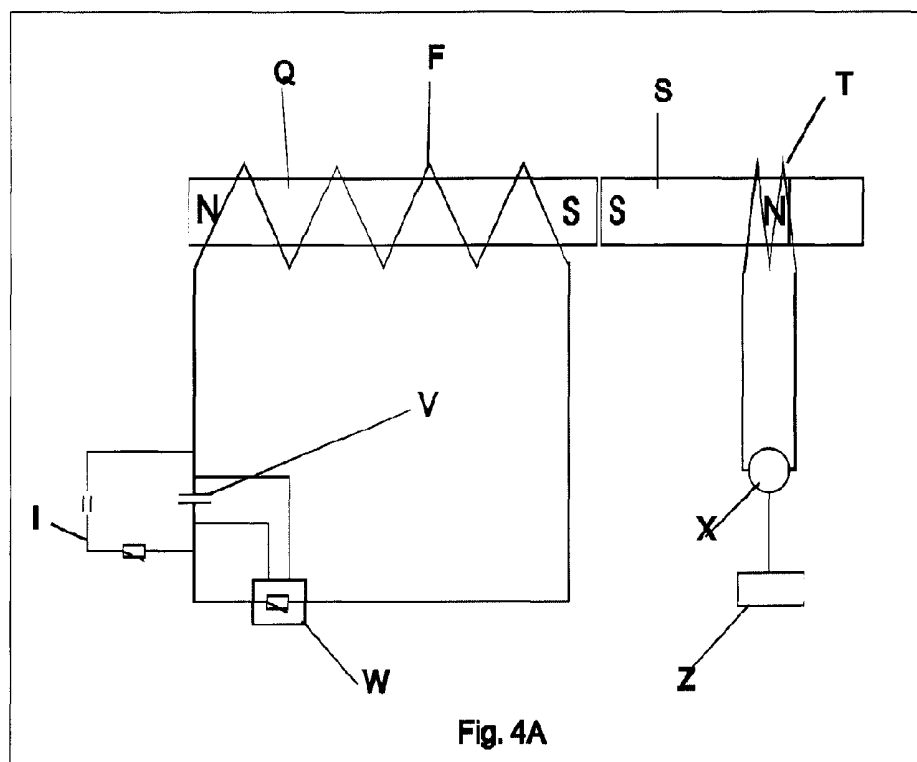
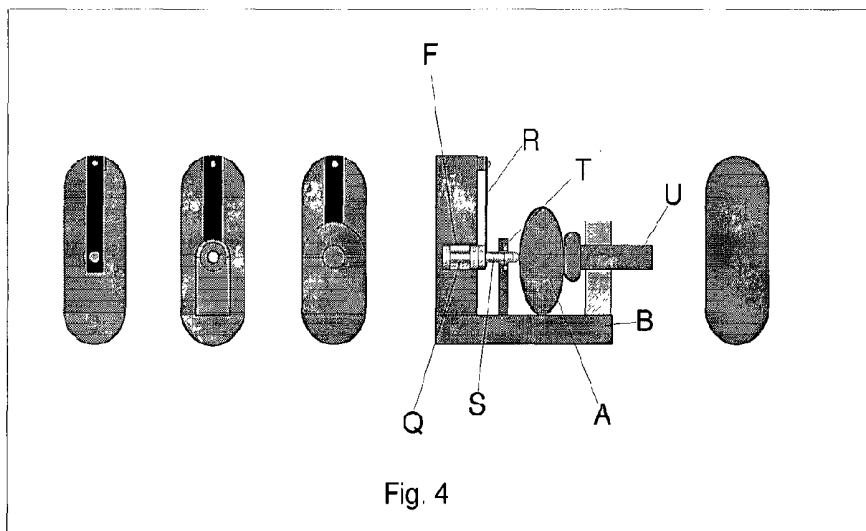


Fig. 5

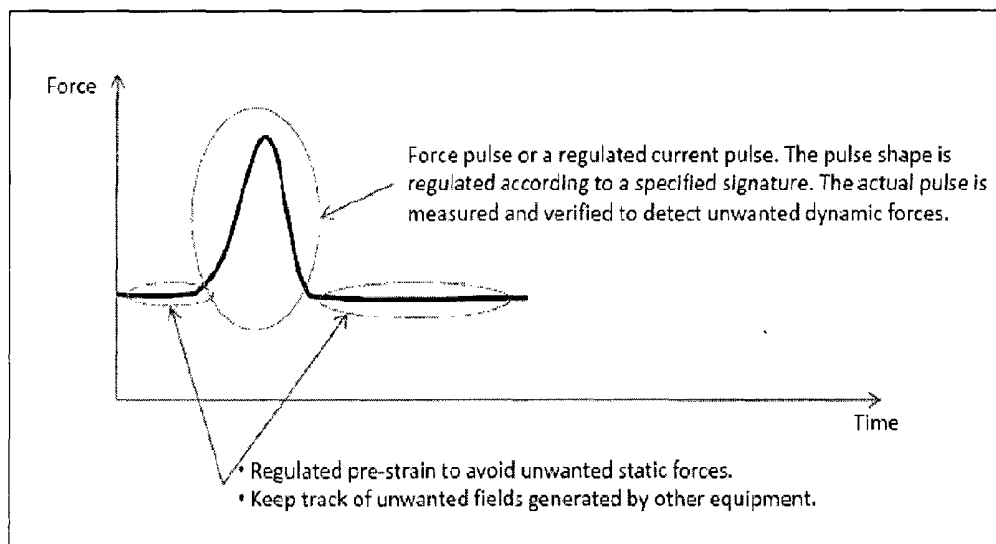
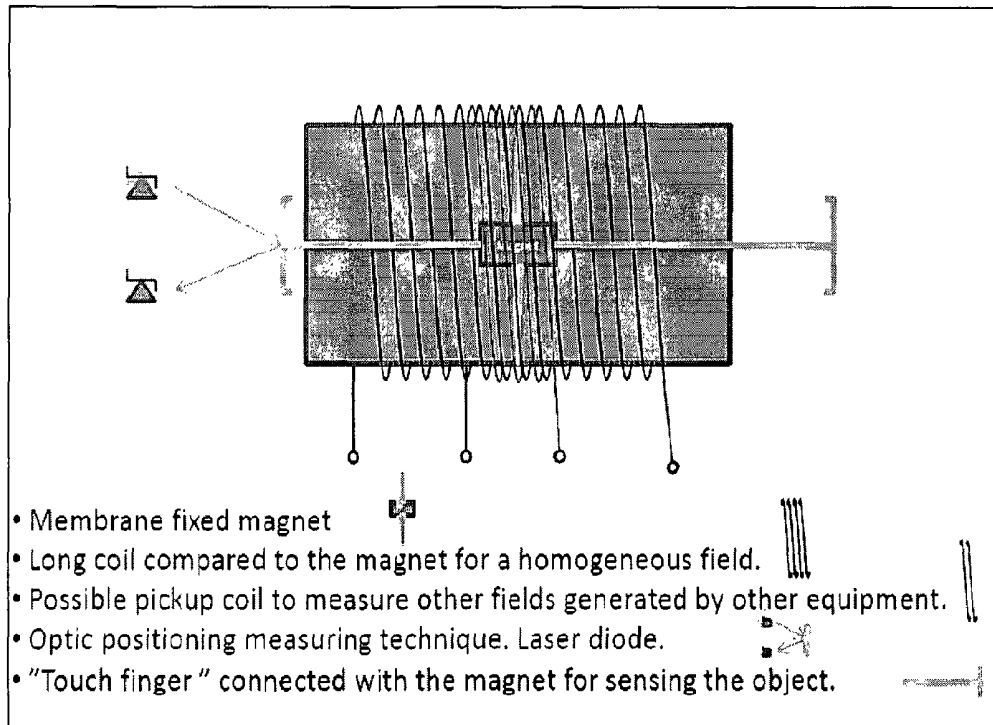
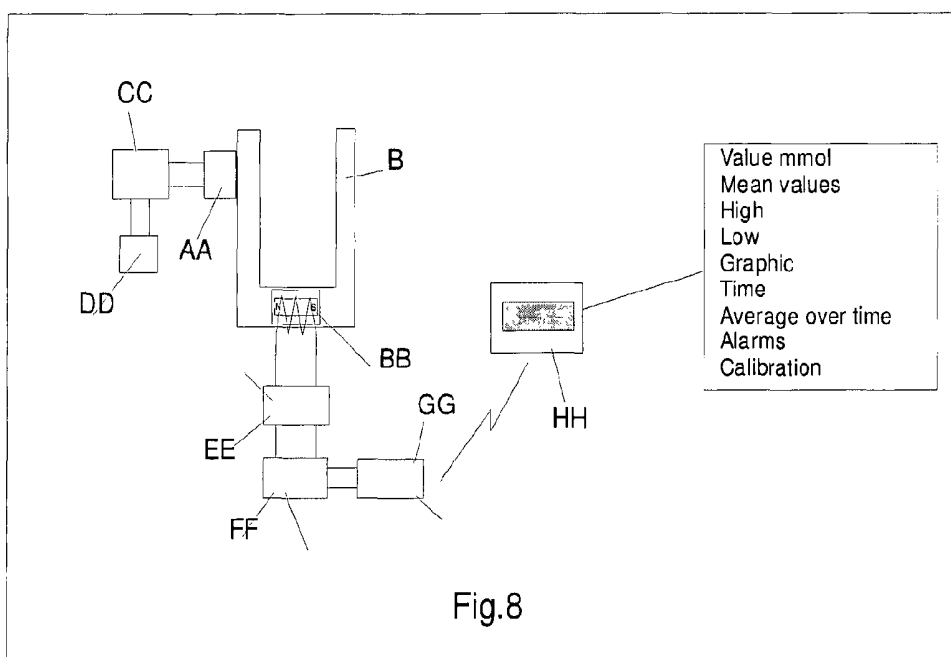
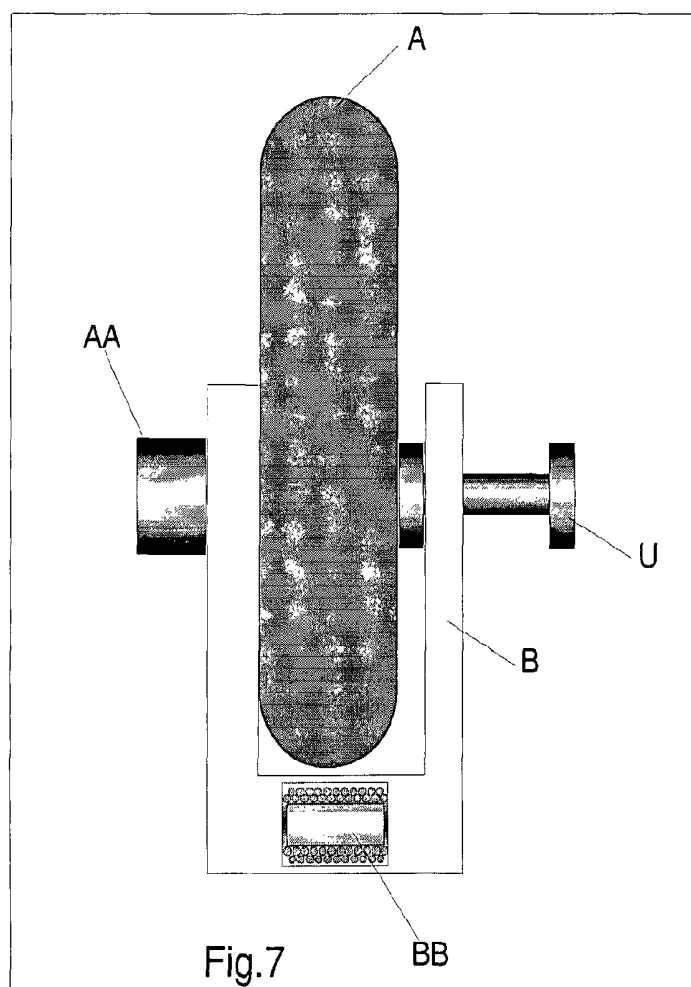
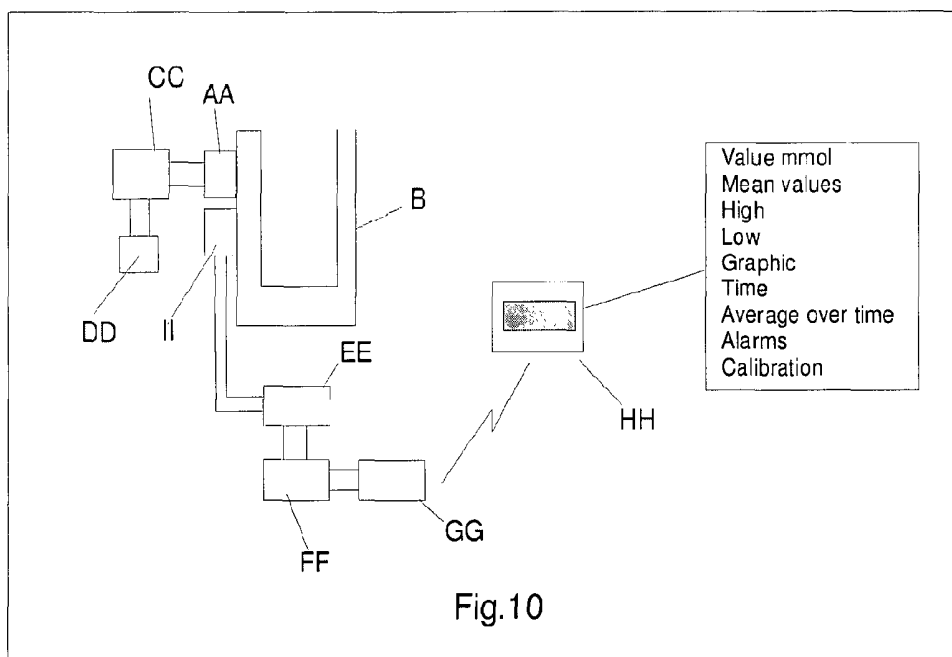
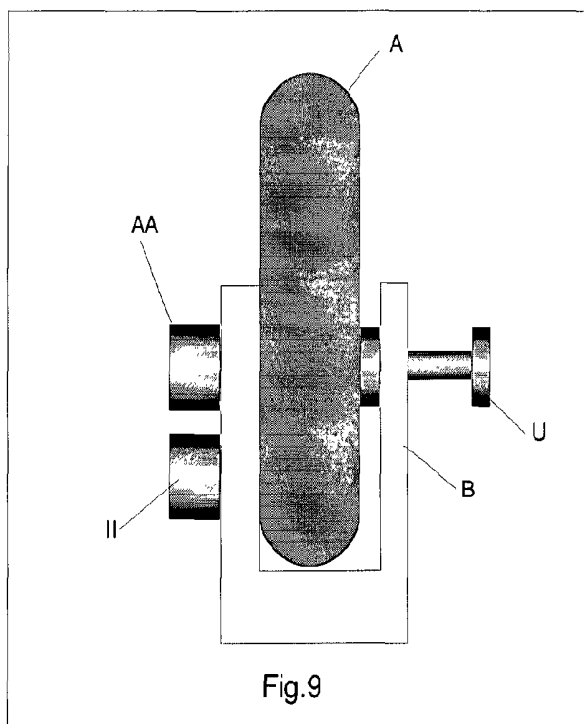
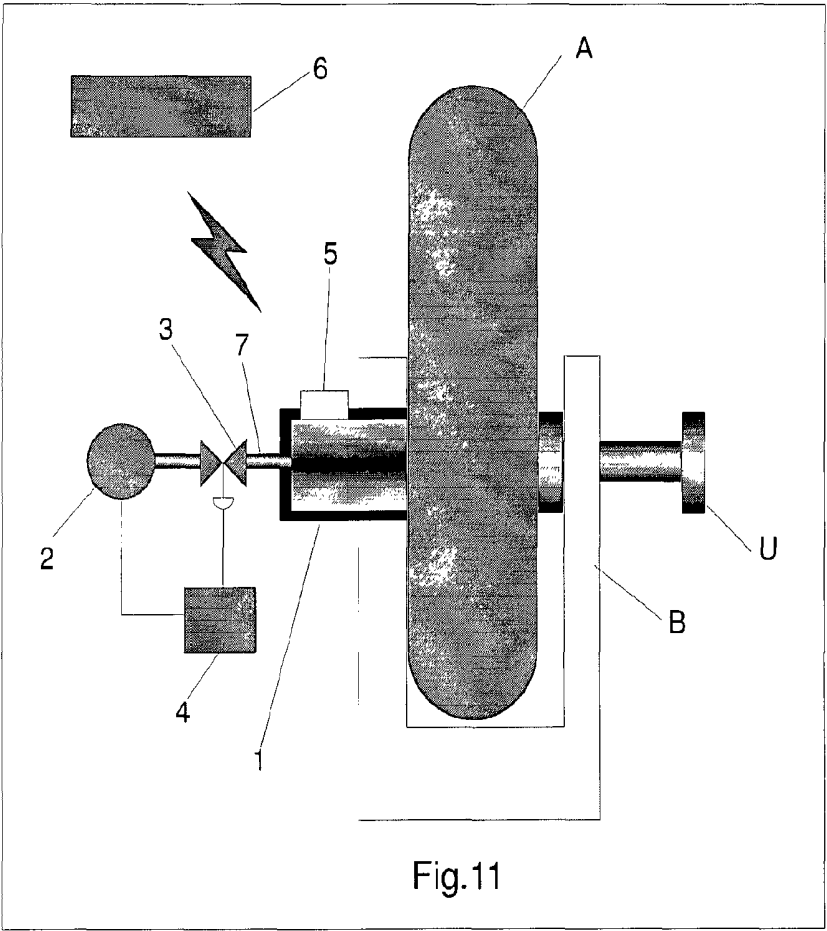
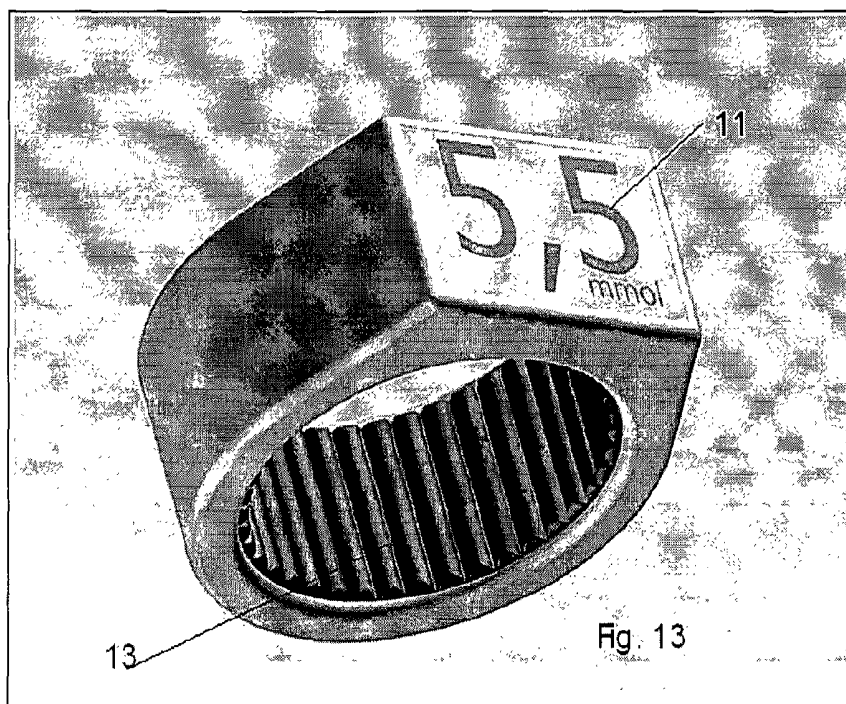
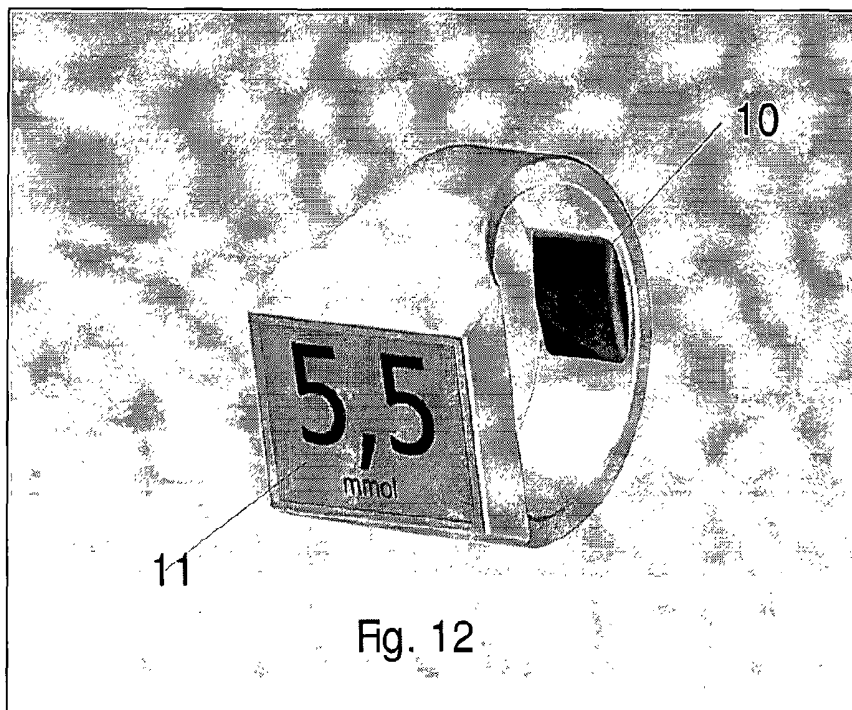


Fig. 6









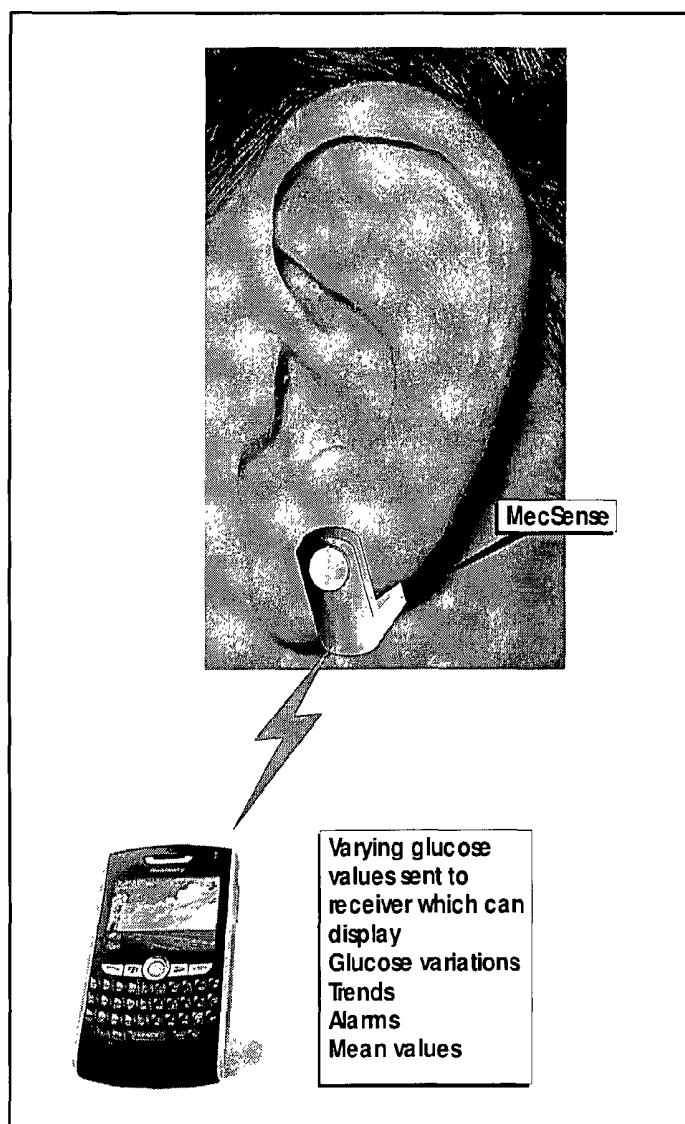


Fig. 14

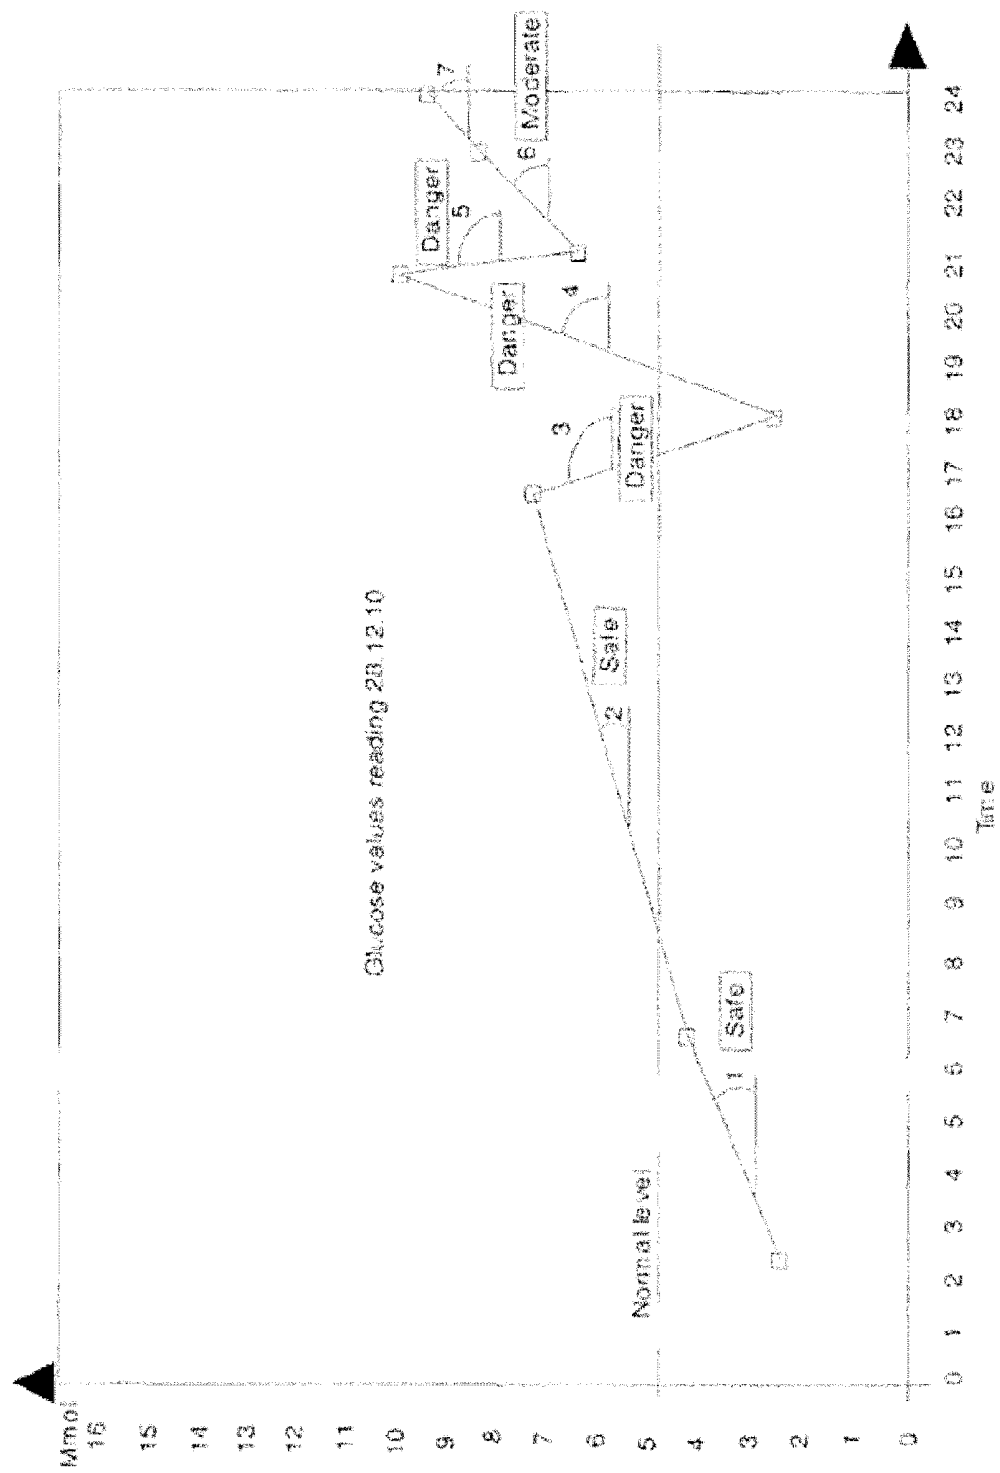


Figure 15

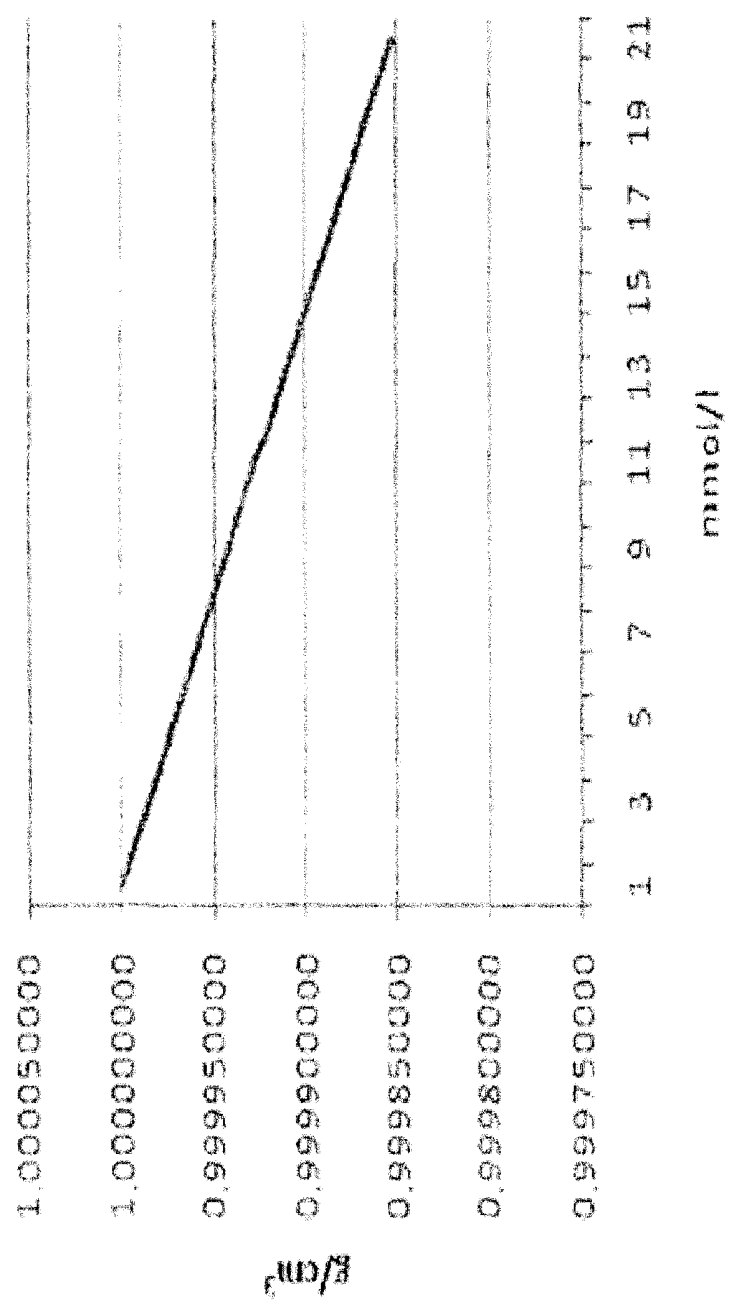


Figure 16

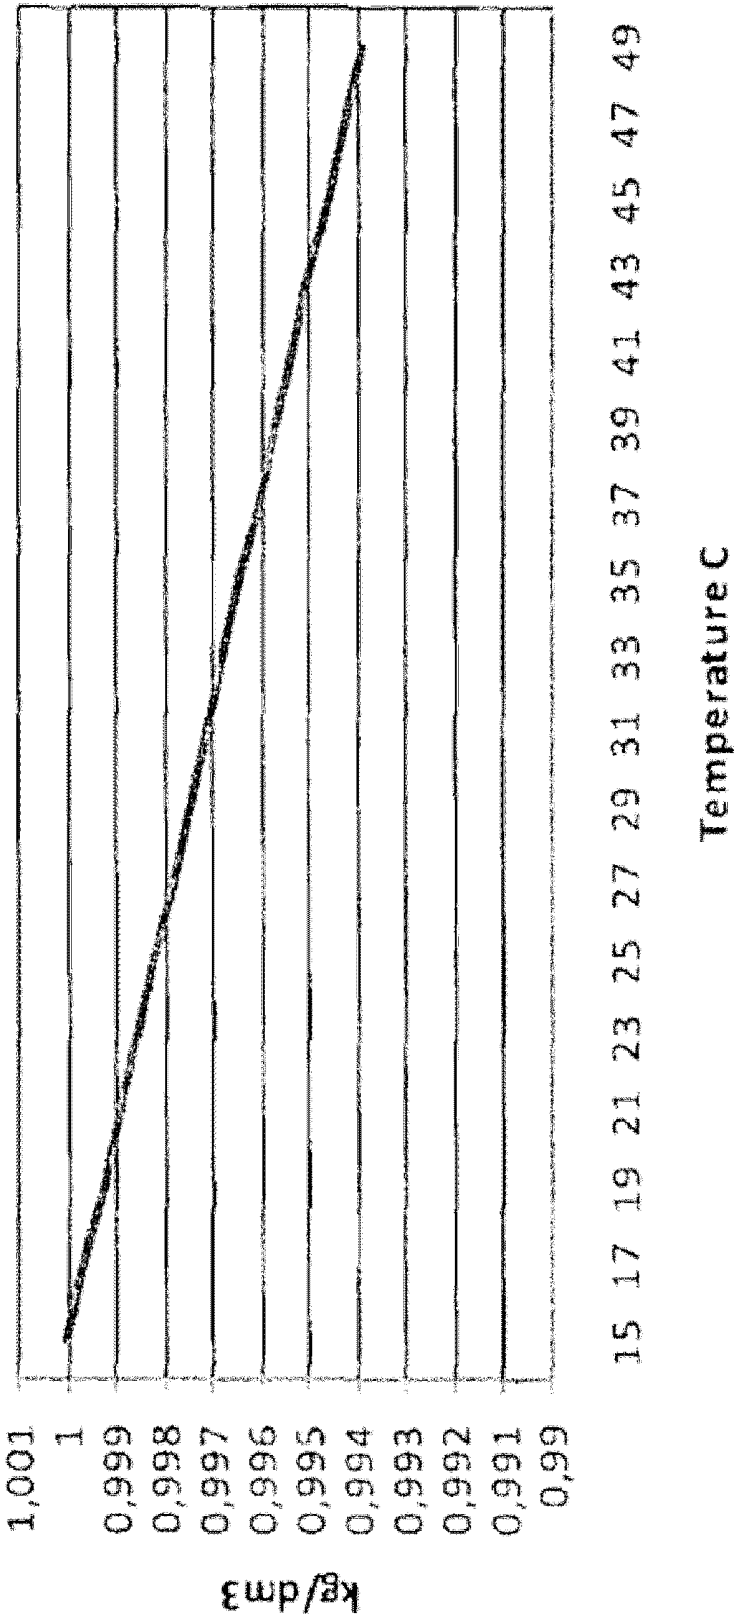


Figure 17

SENSOR DEVICE FOR SENSING BODY FLUID DENSITY AND/OR MEMBRANE RESISTANCE

FIELD OF THE INVENTION

[0001] The present invention is related to a sensor for measuring tensile variation against a membrane separating a liquid such as the skin on humans and animals and any other membrane separating a liquid on one of its sides.

BACKGROUND OF THE INVENTION

[0002] The tensile stress or resistance of a membrane is dependent upon a number of factors, such as the elasticity of the membrane and the density of the liquid separated by the membrane.

[0003] A special case of interest is the tensile variation of the skin which can be interpreted as caused by the variation of the density of the body fluid. One such substance which causes rapid variation of the composition of the body fluids is its content of glucose. As the variations of glucose in diabetics are of paramount importance for the patients, measuring the glucose level in diabetics has been recognized for decades. Some 30 years ago, the only way to measure the glucose level was to apply a drop of blood on a strip where the color on the strip changed by the glucose level. The color was compared on a bar showing the corresponding glucose level for each color. As this principle was inaccurate, the industry started to develop electronic devices which electrically could detect the glucose level on a strip with a blood sample. Over the years this technology has resulted in a number of different devices varying in size, design and features.

[0004] Even though these meters represent a vast benefit to diabetics, they are not continuous, and all need a blood sample. Thus extensive research has been carried out in order to develop a continuous glucose sensor without the need of a blood sample.

[0005] Today there exist invasive glucose sensors that are continuous. A needle has to be inserted through the skin whereby interstitial liquid can be drawn to the sensor which by the aid of glucose oxidase shows varying glucose levels on a handheld receiver. The drawback is that the technology is invasive, and that the needle from time to time has to be changed. Unfortunately the injection site may also become inflamed whereby the users have to stop using the device because of discomfort.

[0006] The dream has been and is to develop a sensor which is non-invasive or implanted. One such approach has been to use the absorption of a beam of infrared light through the skin. However, as the absorption of the spectra in water is far greater than that of glucose this approach is very difficult in order to get reliable glucose data.

SUMMARY OF THE INVENTION

[0007] The present invention provides a sensor for measuring the density of a body, or the resistance of a membrane such as human skin, in a non-invasive manner, comprising a pulse generator, a temperature sensor and a transducer for registration of the speed of the pulse as a function of the body fluid and the elasticity of the skin, wherein said transducer is connected to a microprocessor in which the signal from the transducer is transformed into values for the relative density of said body fluid.

[0008] In a preferred embodiment of the present invention the pulse generating device generates a pulse in the form of a mechanical pulse, a vibrating force, a compressed air/liquid pulse or a sound wave.

[0009] In one embodiment of the invention the pulse generated is a mechanical pulse, which may be generated by an electromagnet or a magneto-strictive material and where the detection of the pulse is recorded by a detection coil or by a variable capacitor, light diode, accelerometer, microphone or any other sensitive pick up device capable of monitoring the impact of the mechanical pulse.

[0010] In another embodiment of the invention the mechanical pulse can be a single pulse, a pulse train or in the form of vibrations.

[0011] In another embodiment of the invention the mechanical pulse can be generated by a pneumatic or hydraulic impulse.

[0012] In another embodiment of the invention the recorded values are computed to give the rate of the changes of the glucose values and where the rate is shown on a display either in digits and/or graphs with associated warnings and recommendations to the user.

BRIEF DESCRIPTION OF THE DRAWINGS

[0013] The following drawings show examples of the principle of the invention, but it is to be understood that any design can be applied to exploit the principle in detecting the variations of the density in body fluid as a measure for detecting variation of the concentration of a solute in the liquid, without deviating from the present invention, which is limited solely by the claims of this invention.

[0014] Below the invention will be described in more detail by reference to the enclosed drawing, wherein:

[0015] FIG. 1 illustrates an embodiment of the invention wherein a constant pulse is used.

[0016] FIG. 2 shows the wiring diagram for the embodiment of FIG. 1.

[0017] FIG. 3 illustrates another embodiment of the invention.

[0018] FIG. 4 shows a further variation of the embodiment of FIG. 1.

[0019] FIG. 5 shows the layout of the pulse generator in the embodiment illustrated in FIG. 4.

[0020] FIG. 6 shows the pulse shape generated by the pulse generator of FIG. 5.

[0021] FIG. 7 illustrates another embodiment of the present invention.

[0022] FIG. 8 shows the principle layout of the wiring diagram of FIG. 7.

[0023] FIG. 9 illustrates a variation of the principle shown in FIG. 7.

[0024] FIG. 10 shows the wiring diagram for the embodiment of FIG. 9.

[0025] FIG. 11 shows still another embodiment of the present invention.

[0026] FIG. 12 illustrates an embodiment of an instrument incorporating the present sensor.

[0027] FIG. 13 illustrates another embodiment of an instrument incorporating the sensor according to the invention.

[0028] FIG. 14 Wireless transmission of data.

[0029] FIG. 15. Continuous monitoring of the development of glucose values.

[0030] FIG. 16. Density of water with varying sugar content.

[0031] FIG. 17. Density of water versus temperature.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

[0032] The objective of this invention is not to measure the actual density of the body fluid. This could be done by extracting body fluid with a syringe for measurement in a laboratory with i.e. a density meter made by Mettler Toledo. We are measuring the relative and varying density of the body fluid through the skin. The density is dependent on the composition of the fluid in its bodily environment. Due to cell membranes in tissues and muscles the density or viscosity of the body fluid will be higher inside the body than outside when applying a mechanical pulse impact on the skin. All physical objects in the body like bones will as well impact the relative density we measure. Dependent on the location of the sensor it will need to be calibrated using a standard glucose sensor. The density measurement value is dependent on the location of the sensor due to bodily structures. Once it is calibrated it will detect variations from that set point.

[0033] In addition to show the glucose values, a continuous reading of the values would give an even more important value for the diabetics. By continuous monitoring of the development of the glucose values, it is possible to compute the rate by which the values fall and rise. By present readings which give an exact number, it is not possible to see how fast the values are changing. This is shown in FIG. 15 for readings over 24 hours.

[0034] In FIG. 15, the angles 1 and 2 show a moderate increase of the glucose values. At 17:00 o'clock the reading shows 7.2 mmol/l, but it was not possible to predict the value at 18:00 o'clock and not how fast it would drop to 2.4 mmol/l. With continuous monitoring, it would be possible to show the drop rate expressed by the angle 3 and thereby take action to prevent the fall towards hypoglycemia.

[0035] To accomplish this, we searched for other physical changes of the blood caused by the variations of the glucose level which could be detected without penetrating the skin.

[0036] The body fluid, in living humans and animals, contains thousands of different molecules and organisms, and where the concentration of some of these varies slowly whereas others can vary rapidly. The latter is the case for glucose in diabetics, lactic acid in human and animal athletes, cholesterol, virus, bacteria, loss of water etc. It is the concentration of all the molecules together with the property of the body liquid which gives the density of the said liquid with its solutes.

[0037] The object of the present invention is to make an instrument/sensor, which can be applied non-invasively for example on the ear lobe, and where a transducer transmits a pulse, or a pulse train such as vibrations into the body fluid.

[0038] The acceleration of a body is following Newton's second law $F=m*a$ (N) where m is the mass of the body in kg and a is the acceleration in m/s^2 .

[0039] When applying a constant mechanical pulse into the fluid, one will have varying accelerations according to:

$$a_x = F/m_x (m/s^2)$$

[0040] Where F is the constant pulse in N and m_x is the varying mass,

[0041] If applying a constant acceleration, one will experience a varying force according to:

$$F_x = m_x * a (N)$$

[0042] Where m_x is the varying mass and a is the constant acceleration.

[0043] These variations can be picked up by different existing elements such as piezo electrical crystals, detection coils, silicon pressure transducers or accelerator meters, light diodes or other sensitive pick up instruments.

[0044] For normal diabetics, the density of the body fluid will be a measure of the changed level of glucose in the fluid and for athletes; a changed density can be a measure of an increased level of lactic acid. The same will apply for dehydration, as loss of water will concentrate the normal molecules and substances present in the body fluid.

[0045] The following table shows values of the glucose molecule.

Avogadro's number $N_A =$	6.02E+23 GLUCOSE a
Molecular weight $M = g$ (Dalton)	180
Specific weight $sg = g/cm^3$	1.544
Volume of one mol $V = M/sg = cm^3$	116.58
Volume each molecule $dV = V/N_A = cm^3$	1.93655E-22
Packing factor $x = \%$	47.6
Diameter molecule $D = (6 * V/3.14)^{1/2} = cm$	1.50826E-07
Diameter molecule $D = A =$	1.51
Peritoneal concentration:	
mmol/l	5.00
Mass mg/l	900.00
Mass g/l	0.90
Mass in an average body of 80 kg (l) = g	72.00
Osmotic pressure $x = 2.58 Mo = (kPa)$	12.90
Osmotic pressure $p = 2.58 Mo = mbar$	129.00
Molecular concentration mmol/l	1
Osmotic pressure $p = mbar$	25.4

② indicates text missing or illegible when filed

[0046] FIG. 16 shows the density variation in water caused by variations of glucose from 1 to 20 mmol/liter.

[0047] As can be seen, the variations are, as expected, linear. As the variations take place beginning after the fifth digit after comma, the sensor must have a high enough sensitivity to register these variations.

[0048] The density is, however, also dependent upon the temperature because of the expansion coefficient of the liquids which has to be taken into consideration and compensated for. The volume of a liquid expands by the following equation:

$$V_x = V_1 * (1 + \mu(t_2 - t_1)) (dm^3)$$

[0049] Where is the reference volume in question, μ =expansion coefficient which for water is $0.18*10^{-3}$, t_2 is the increase of the temperature and t_1 is the reference temperature. The general equation of the density is $p=m/V$ where m is the mass for the given volume V . Thus for a mass m (kg) at the volume V_1 (the density will change by the equation:

$$P_x = m/V_x = m/(V_1 * (\mu(t_2 - t_1)) (kg/dm^3))$$

[0050] The variation of the density of water between 15 and 49 C is shown in the FIG. 17.

[0051] The variation of the density caused by the temperature is compensated by a mathematical algorithm in the processor which processes the recorded data from the pulse thereby giving the density at the temperature by the calibration of the sensor. The calibration of the sensor takes place by adjusting the set point at a glucose level given by a standard

glucose meter whereby the set point of the temperature is automatically set by the thermometer incorporated in the sensor. From this set point, the sensor detects the variations caused both by the variation of the tension in the skin and the solutes in the body liquid and the temperature.

[0052] The present invention thus provides a sensor for measuring the density of a body liquid by generating a pulse or pulses that hits the skin and where a transducer will pick up the speed of the pulse which is dependent on the composition of the body fluid and the elasticity of the skin. The pulse may be a mechanical pulse, vibration or a compressed air/liquid pulse or any other means of a pulse like a sound wave that will be recorded by a pickup device that may be a pickup coil, microphone, silicone pressure transducer, stretch pad, accelerometer meters, light diodes or other sensitive instruments. A temperature sensor touching the skin will continuously record the temperature close to the area where the pulse hits the skin, the transducer delivers the results to a microprocessor or an ASIC that has an algorithm that calculates the relative density which is dependent on the composition of the fluid. One such substance which causes rapid variation of the body fluids composition is its content of glucose. The results of the readings caused by the variation of the glucose content are therefore an estimate of the glucose level. The glucose data can be transmitted wirelessly or by wire to an external receiver where the readings are shown on a display as glucose values expressed in mmol per liter or any other unit, such as mg per liter (see FIG. 14). The sensor may have alarms for high and low glucose levels. Since the sensor device has to be calibrated by the user by using a standard glucose sensor, the sensor may receive this calibration with Bluetooth making the user able to send the calibration data by cell phone. The cell phone may also be the device used for displaying the glucose data. The microcontroller or the ASIC in the glucose sensor is programmed to interpret input data like calibration data or other data that makes it respond to glucose values with an underlying text. The receiving device will have a keyboard making the user able to send information to the glucose sensor and the software needed to do so.

[0053] The software that handles the data sent from the above mentioned glucose sensor includes alternative display of the signals (digits or graphs), warning signals and different computing of historical data such as mean values of the glucose level, the rate of which the values raise and falls. In the case of hypo/hyperglycemia, an alarm will go off at preset points. The same is the case if the rise and fall rate is faster or slower than preset values. If the temperature is too high, a warning text preferably informs the user that the displayed value may be wrong if the user is suffering from dehydration and or low salt level. The user can also add information about exercise and what kind of food he or she will eat in addition to the amount of insulin and type of insulin injected or tablets, so that the glucose values becomes understandable. Preferably the software may deliver comments and suggestions of what to do.

[0054] The present invention also provides a sensor for measuring the resistance of a membrane, such as skin, having a complex or single fluid on one of its sides, caused by the change of the membrane and the fluid characteristics caused by variation of the membrane elasticity and the fluid composition. Such as that observed by varying glucose level in diabetics and lactic acids in humans and animals, by measuring the acceleration or pressure variations of the membrane and the body fluids in accordance with Newton's second law

with a mechanical pulse and/or vibrations applied to the tissue which can be the ear lobe. Variations of the body fluids density and the membranes elasticity gives a measure of the variations of the membranes elasticity and the concentration of solutes in the fluids to be recorded from a set value.

[0055] According to the present invention the mechanical pulse can be generated by an electromagnet with an iron core which is made magnetic when energizing the electro magnet and where the pulse body can be a permanent magnet having the same pole as the pole in the iron rod, which causes the permanent magnet to be repelled from the iron core. The pulse can also be generated by a magnetostrictive material which expands under the influence of a magnetic field. The detection of the pulse can be recorded by a detection coil or by a variable capacitor.

[0056] Another way to implement the present invention would be to apply a vibrating force to the membrane where the damping of the vibrations and its amplitudes is dependent upon the attenuation of the fluid which is caused by the variations of the density of the body fluids and the membrane's elasticity. The amplitudes will give a measure of the variations of the membrane's elasticity and the concentration of solutes in the fluids to be recorded from a set value and which is shown as variation of the glucose level either in mmol/liter or mg/dl or any other unit.

[0057] The vibration force may be generated by a magnetic or piezo electric vibrator and the amplitudes of which can be detected either with a small self inducing linear or circular generator or any other receiver, such as a microphone which can detect variations of the changed amplitudes caused by the changed elasticity of the membrane caused by variations of the composition of the liquid on one of its sides.

[0058] The present invention also provides a structure for a sensor for measuring at least one property of a tissue object, the structure comprising first and second elongate carriers being connected at respective base sections thereof and extending there from in substantially same directions, and having means for clamping respective first sections of the first and second elongate carrier sections located distally from the base sections, to respective opposite sides of the tissue object, wherein the first carrier carrying in the first section thereof a first transducer having an excitation input and comprising an actuator having a movable element being arranged to be accelerated in a direction of the first section of the second carrier in response to excitation energy provided to the excitation input, so as to be capable of delivering at least part of the excitation energy to the tissue object, and the second carrier carrying in the first section thereof a second transducer having a signal output and comprising a pick-up being arranged to be accelerated in a direction of the first section of the first carrier for providing energy at the signal output in response to acceleration of the movable element, so as to be capable of delivering on the signal output a receive signal including at least part of excitation energy picked up from the tissue object.

[0059] In a preferred embodiment of the present invention the sensor comprises the above structure, and transceiver and signal processing circuitry are coupled to the excitation input and the signal output, and are arranged a) to provide the excitation energy in form of a single pulse, a pulse train or variation, according to a predetermined temporal pattern, b) to prepare and store receive signal data, and c) to process stored receive signal data with respect to the temporal pattern to determine the variation.

[0060] FIG. 1 illustrates an instrument with a constant pulse F. The instrument consists of a housing H which is built up with a second body B having a clamping device, body H which houses the coil F with its iron rod G and a variable resistor or capacitor E attached to an impact body D. When applying a current pulse from a power source to the coil, it will accelerate the iron rod against the resistor or capacitor connected to the impact body against the ear lobe A. The different densities will give different readings of the variable resistor or condenser and where the readings can be given in values for the glucose level. The instrument must be calibrated before use, which is done by measuring the glucose level with a standard glucose meter. By the shown value of the glucose level, the instrument will show varying readings from the set point.

[0061] FIG. 1A shows the wiring diagram for this solution where I is a timer which reads the impulse time, J is a power source which rapidly discharges a current to the coil. The discharged power is the same for each pulse and this can be accomplished by discharging the current from a loaded capacitor. E is the variable resistor or capacitor which detects the force from the activated rod. The force is transmitted to a microprocessor K which computes the signal and transmits it to a sender L which transmits the signal either wirelessly or by wire to a receiver M which shows the detected signal as variations from the set point. If a premeasured glucose level was say 5 mmol/liter, the shown impulse value at that glucose level is shown as the same value for whatever value the impulse gave, for example x. By a value of x+z, this shows a figure value higher than 5.

[0062] FIG. 2 shows an instrument as in FIG. 1, but where the variable resistor or capacitor is replaced with a silicon pressure transducer or a silicon accelerometer O which picks up the pressure or acceleration generated by the constant pulse.

[0063] The pulse will be accelerating the transducers against the skin and the pressure recorded is dependent upon the density of the displaced tissue. When using an accelerometer, the acceleration is dependent upon the mass of the displaced tissue—in both cases; the density is a function of the glucose content.

[0064] The wiring diagram will be similar to the wiring diagram FIG. 1A.

[0065] FIG. 3 shows still another layout where the ear lobe support on both sides are ring shaped P and where the impact part (pressure transducer) on the iron rod in resting position does not touch the skin before the pulse generator is activated. It is to be understood that the impulse generator can be any kind of a rapid accelerator such as a piezo electrical pulse generator where it is the expansion of the piezo electrical crystal which gives the mechanical movement. The piezo electrical crystal can also be replaced with another material which expands under the influence of a magnetic field, such as Terfonol which is an alloy of Terbium, Dysprosium and Ferrum. The wiring diagram will more or less be as for FIG. 1.

[0066] It is to be understood that the principle can be applied to any configuration which can be given by Newton's laws.

[0067] The recorded data can be sent to a hand held instrument, such as a cell phone by BLUETOOTH®.

[0068] FIG. 4 shows an example of the lay-out in accordance with FIG. 1 and FIG. 4A shows the associated wiring diagram of FIG. 4.

[0069] A movable permanent magnet S is given a magnetic impulse generated by activation coil F having a fixed and not movable iron core Q. As the moveable magnet is moving, its one pole will, in a detection coil T, create a current in the coil where the values voltage and current (V and I) are dependent upon the velocity of the magnet which in turn is dependent upon the resistance in the end of the magnet caused by variation of the density of the displaced fluid in the ear lobe. In order to have the same mechanical resistance of the moveable magnet, it is shown attached to a flexible spring R, which maintains its elastic properties over time. The tension of the sensor against the ear lobe is adjusted by the screw device U.

[0070] FIG. 4A shows the wiring diagram of FIG. 4 with the power source I and the capacitor V which is opened for charge drainage by the resistor W. The detection coil is shown as T, where the generated current is detected by the current detector X and which values are shown in the reader Z.

[0071] FIG. 5 shows the practical lay-out of the pulse generator, and FIG. 6 shows the pulse shape generated from the pulse generator.

[0072] The following calculations can be shown as an illustration of the principle:

Basic equation $F = m \cdot a$				N
$m =$ mass to be accelerated				kg
$a =$ acceleration				m/s^2
A constant pulse with a constant force, gives a variable acceleration which varies with m				
ASSUMPTIONS				
Diameter of fluid droplet $d =$	3	m.m. =	0.03	dm
Volume of fluid droplet	0.00001413			dm ³
$V = d^3 \cdot 3.14/6 =$				
Mass of droplet $dm_x = V \cdot sg_x =$				
Impact length $s =$	0.25	m.m. =	0.00025	m
Variable acceleration				m/s^2
$a_x = F/m_x =$				
Force $F =$	0.00001			N
Travel time $t_x = 2 \cdot s \cdot m_x/F =$				s
Acceleration $a_x = 2 \cdot s/t_x^2 =$				m/s^3
Impulse time $dT =$	1	ms =	0.001	s
Velocity at end of pulse $v = a_x \cdot t_x/2 =$			0.5000	m/s

[0073] The result of the calculations are shown below.

Glucose conc.		Density of glucose				Volum water cm ³	Weight of Water Gw (gt)	Total Weight Gx = Gg + GW gr
		0.961 kg/dm ³ =	0.961 g/cm ³ Weight of glucose Gg (gr)					
0	mmol/l =	0	mg/l =	0	g/l =	0	cm ³	1000
1	mmol/l =	180	mg/l =	0.18	g/l =	0.18770489	cm ³	999.8126951
2	mmol/l =	360	mg/l =	0.36	g/l =	0.3740978	cm ³	999.8253902
3	mmol/l =	540	mg/l =	0.54	g/l =	0.56191407	cm ³	999.4380857
4	mmol/l =	720	mg/l =	0.72	g/l =	0.74921956	cm ³	999.2507804
5	mmol/l =	900	mg/l =	0.9	g/l =	0.93652445	cm ³	999.0634255
6	mmol/l =	1080	mg/l =	1.08	g/l =	1.12382934	cm ³	908.8761707
7	mmol/l =	1260	mg/l =	1.26	g/l =	1.31113424	cm ³	998.6838458
8	mmol/l =	1440	mg/l =	1.41	g/l =	1.49843913	cm ³	998.5015609
9	mmol/l =	1620	mg/l =	1.52	g/l =	1.68974402	cm ³	998.314258
10	mmol/l =	1800	mg/l =	1.8	g/l =	1.87304891	cm ³	988.1269911
11	mmol/l =	1980	mg/l =	1.98	g/l =	2.0608538	cm ³	937.9336462
12	mmol/l =	2160	mg/l =	2.16	g/l =	2.24763869	cm ³	997.7523413
13	mmol/l =	2340	mg/l =	2.34	g/l =	2.43496358	cm ³	997.5630164
14	mmol/l =	2520	mg/l =	2.52	g/l =	2.62228847	cm ³	997.3777315
15	mmol/l =	2700	mg/l =	2.7	g/l =	2.80957116	cm ³	997.1904266
16	mmol/l =	2680	mg/l =	2.89	g/l =	2.99687825	cm ³	897.0011217
17	mmol/l =	3060	mg/l =	1.06	g/l =	3.78418114	cm ³	998.8158169
18	mmol/l =	3240	mg/l =	3.24	g/l =	3.37148803	cm ³	996.628112
19	mmol/l =	3420	mg/l =	3.42	g/l =	3.55879292	cm ³	996.4412073
20	mmol/l =	3600	mg/l =	3.6	g/l =	3.74609781	cm ⁴	996.2539022

Glucose conc.	Density sg.	Weight		By constand a		By contant F	
		droplper gr	Fx (N)	tx (s)	② = 2 * ②②		
0	1.000000000 g/cm ³	0.014130000	0.007065000	0.00070650000	1001.71845		
1	0.999992695 g/cm ³	0.014129897	0.007064948	0.00070649484	1001.71308		
2	0.999985390 g/cm ³	0.014129794	0.007054397	0.00070648968	1001.74722		
3	0.999973085 g/cm ³	0.014129690	0.007064845	0.00070648452	1001.76255		
4	0.999970780 g/cm ³	0.014129587	0.007064794	0.00070642938	1001.77699		
5	0.999983476 g/cm ³	0.014129484	0.007064742	0.00070647420	1001.79163		
6	0.999956171 g/cm ³	0.014129181	0.007064590	0.00070616903	1001.88626		
7	0.999948866 g/cm ³	0.014129277	0.007064539	0.00070646387	1001.8209		
8	0.999541561 g/cm ³	0.014125174	0.007064587	0.00070645871	1001.83554		
9	0.999834256 g/cm ³	0.014179071	0.007064536	0.00070645355	1001.85017		
10	0.999928951 g/cm ³	0.014128968	0.007064484	0.00070644839	1001.56481		
11	0.999919648 g/cm ³	0.014128895	0.007064432	0.00070644232	1001.87945		
12	0.999912341 g/cm ³	0.014128751	0.007064381	0.00070643805	1001.89409		
13	0.999905085 g/cm ³	0.014128658	0.007064329	0.00070643291	1001.90874		
14	0.999837732 g/cm ³	0.014128533	0.007064277	0.00070642775	1001.92387		
15	0.999800427 g/cm ³	0.014128452	0.007064226	0.00070642255	1001.93801		
16	0.999681122 g/cm ³	0.014128349	0.007064174	0.00070641745	1001.53265		
17	0.999875817 g/cm ³	0.014128745	0.007864123	0.00070641236	1001.96725		
18	0.999868512 g/cm ³	0.014128142	0.007064071	0.00070640718	1001.98192		
19	0.999861207 g/cm ³	0.014128039	0.007064019	0.00070640154	1001.99657		
20	0.999853902 g/cm ⁴	0.014127936	0.007061968	0.00070639678	1002.01121		

② indicates text missing or illegible when filed

[0074] Yet another principle to detect the variation of the combined resistance from a membrane and its associated liquid is to apply a vibrating force on a body connected to the ear lobe. By applying vibration force to the body, its damping will depend on flexibility of the membrane, here the skin, and the physical properties of the body liquid. As the density of the liquid changes, the amplitude of the vibrations will increase by increasing density and vice versa and is thus a value of the varying resistance of the ear lobe.

[0075] FIG. 7 shows an example of this principle where an U-shaped body B is connected to an ear lobe A, having a frequency controllable vibrator AA and a generator BB which consists of a magnet core surrounded by a coil. When the vibrator is activated, the body, such as the ear lobe, comes into vibrations and accelerates the magnetic core. The accelera-

tions of the core is dependent upon the amplitude of the vibrations which again is dependent upon the damping of the vibrations caused by the variations in the body fluid.

[0076] FIG. 8 shows the principle layout of the wiring diagram of FIG. 7.

[0077] CC is a power source which activates the vibrator AA, and its frequency is controlled by a frequency controller DD. The generator BB is connected to an ampere meter EE which passes the recorded current values to a microprocessor FF which computes the values and by wire or wirelessly by GG sends the values to the receiver HH which presents the values of the variations of the vibrations in numbers from a preset point, as explained above.

[0078] FIG. 9 shows the same principle as shown in FIG. 7, but where the generator is replaced by a microphone II attached to the body detecting the variations of the amplitude.

[0079] FIG. 10 shows the principle layout of the wiring diagram for FIG. 9.

[0080] There exist a number of patents which utilize acceleration versus density to record a property of a solid, gas or liquid. U.S. Pat. No. 2,358,374 shows an instrument for measuring the density of a liquid and/or gas by means of a vibrating body (vane) immersed in a liquid. We are not immersing any body in the fluid itself, but applying a pulse or vibration on a membrane separating the fluid, i.e. the skin on living humans or animals.

[0081] The objective of the present invention is not to give a figure of the actual density of the fluid, but to show the variation of the fluids density, the membranes elasticity and viscosity caused by the change of composition of the fluid either it being the density or viscosity which both contribute to give a distinct signal of the resistance the sensor senses as described above. As stated above, the sensor needs to be calibrated by measuring the glucose content by a standard glucose sensor whereby the sensor will detect the variation from the set point. For example, if the measured glucose level is 5.5 mmol, whatever signal the sensor is given, this signal is set to be 5.5 mmol and any changes from this value will vary from this set point.

[0082] Still another means to generate a pulse which can be used according to the principle of the invention as described herein, is to use an air pulse as illustrated in FIG. 11.

[0083] Shown is a body B) attached to the ear lobe A) having a hollow body 1) connected to a pipe 7) and a rapid releasing valve 3) connected to an air source 2) which can be a micro compressor or another suitable means to compress air. On the hollow body 1) is attached a pressure sensor 5) having incorporated a temperature sensor and electronics for transferring values to an external reader 6). When the pressure in the air source 2) has reached a preset pressure, the pressure is detected by a pressure detector 4) which transmits a signal to the valve 3) to open, thus letting an air pulse to escape into the hollow body 1) and towards the air lobe. The compression of the air pulse will be dependent upon the elasticity of the skin and the underlying tissue with its fluid content which density is dependent upon the concentration of the fluid solutes.

[0084] The pressure is detected by the pressure transducer 5). As the pressure pulse can be affected by the surrounding temperature, a microprocessor attached to the transducer 5) or on the body B), compensates the signal by the recorded temperature to a preset mean temperature for the system.

[0085] A further application of the principles can be obtained by using vibration force where the amplitude of the vibrations also follows Newton's first law and where the damping of the vibrations is dependent upon the attenuation of the fluid which again is dependent upon its dissolved solutes and thereby its density.

[0086] This vibration principle can also be incorporated in other housings such as a ring on a finger.

[0087] FIG. 12 shows a layout of the principle when using a pulse impact body shown as a pillow 10) inside the ring and where 11) is a display showing the read out value from the processor and power source located under the display.

[0088] FIG. 13, shows a layout with a vibration source 13) arranged as a number of vibrating elements inside a ring and with the display and the associated electronics arranged as in FIG. 12.

[0089] The use of vibration force can be applied by any design of the sensors and for any location of the same, for example on the ear lobe.

[0090] Having described preferred embodiments of the invention it will be apparent to those skilled in the art that other embodiments incorporating the concepts may be used. These and other examples of the invention illustrated above are intended by way of examples only and the actual scope of the invention is to be determined from the following claims.

1. A sensor for measuring the density of a body fluid, or the resistance of a membrane such as human skin, in a non-invasive manner comprising a pulse generator, a temperature sensor and a transducer configured to register the speed of the pulse as a function of the body fluid and the elasticity of the skin following Newton's first law:

$$F=m*a,$$

where m is the mass of the displayed fluid and a is its acceleration in m/s^2 when applying a constant force F in Newton (N), wherein said transducer is connected to a microprocessor in which a signal from the transducer is transformed into values for the relative density of said body fluid.

2. The sensor of claim 1, wherein the pulse generating device generates a pulse in a form of a mechanical pulse, a vibrating force, a compressed air/liquid pulse or a sound wave.

3. The sensor of claim 2, wherein the pulse generating device generates a mechanical pulse.

4. The sensor of claim 3, wherein the mechanical pulse is generated by a pneumatic or hydraulic impulse.

5. The sensor of claim 3, wherein the mechanical pulse is generated by an electromagnet or a magneto-strictive material and wherein the detection of the pulse is recorded by a detection coil or by a variable capacitor, light diode, accelerometer, microphone or any other sensitive pick up devices capable of monitoring the impact of the mechanical pulse.

6. The sensor of claim 5, wherein the mechanical pulse is a single pulse, a pulse train or in the form of vibration

7. A sensor in accordance with claim 1, wherein a rate of the change of glucose values is computed and wherein the rate is shown on a display either in digits and/or graphs with associated warnings and recommendations to the user.

* * * * *

专利名称(译)	用于感测体液密度和/或膜电阻的传感器装置		
公开(公告)号	US20130338456A1	公开(公告)日	2013-12-19
申请号	US13/979348	申请日	2012-01-12
[标]申请(专利权)人(译)	ELLINGSEN OLAV ELLINGSEN比阿特SØREBØ		
申请(专利权)人(译)	ELLINGSEN奥拉夫 ELLINGSEN, 比阿特SOREBO		
当前申请(专利权)人(译)	MECSENSE AS		
[标]发明人	ELLINGSEN OLAV ELLINGSEN BJARTE SOREBO		
发明人	ELLINGSEN, OLAV ELLINGSEN, BJARTE SOREBO		
IPC分类号	A61B5/00 A61B5/01 A61B7/00 A61B5/11 A61B5/145 A61B5/1455		
CPC分类号	A61B5/0051 A61B5/14532 A61B5/6816 G01N9/24 G01N9/26 A61B5/7278 A61B7/00 A61B5/443 A61B5/442 A61B5/1455 A61B5/11 A61B5/01 A61B5/7225		
优先权	20110070 2011-01-12 NO		
其他公开文献	US9888883		
外部链接	Espacenet USPTO		

摘要(译)

传感器装置技术领域本发明涉及一种用于测量相对于膜的拉伸变化的传感器装置, 所述膜分离诸如人和动物的皮肤之类的液体以及在其一侧上分离液体的任何其他膜。

