



US009603652B2

(12) **United States Patent**
Carlton et al.

(10) **Patent No.:** **US 9,603,652 B2**
(45) **Date of Patent:** **Mar. 28, 2017**

(54) **ELECTROSURGICAL INSTRUMENT INCLUDING A SENSOR**

USPC ... 606/38, 42, 52, 41; 607/98-100, 102, 115
See application file for complete search history.

(75) Inventors: **John D. Carlton**, Las Vegas, NV (US);
Darren Odom, Longmont, CO (US)

(56) **References Cited**

(73) Assignee: **COVIDIEN LP**, Mansfield, MA (US)

U.S. PATENT DOCUMENTS

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 1638 days.

371,664 A 10/1887 Brannan et al.
702,472 A 6/1902 Pignolet
728,883 A 5/1903 Downes
1,586,645 A 6/1926 Bierman
(Continued)

(21) Appl. No.: **12/195,624**

FOREIGN PATENT DOCUMENTS

(22) Filed: **Aug. 21, 2008**

CA 2104423 2/1994
DE 2415263 10/1975

(65) **Prior Publication Data**

(Continued)

US 2010/0049187 A1 Feb. 25, 2010

OTHER PUBLICATIONS

(51) **Int. Cl.**

A61B 18/14 (2006.01)
A61B 18/12 (2006.01)
A61B 5/00 (2006.01)
A61B 17/00 (2006.01)
A61B 18/00 (2006.01)

Michael Choti, "Abdominoperineal Resection with the LigaSure Vessel Sealing System and LigaSure Atlas 20 cm Open Instrument"; Innovations That Work, Jun. 2003.

(Continued)

(52) **U.S. Cl.**

CPC **A61B 18/1206** (2013.01); **A61B 5/0059** (2013.01); **A61B 18/1442** (2013.01); **A61B 5/0008** (2013.01); **A61B 18/1445** (2013.01); **A61B 2017/00057** (2013.01); **A61B 2018/00702** (2013.01); **A61B 2018/00791** (2013.01)

Primary Examiner — Thomas Giuliani


(57) **ABSTRACT**

(58) **Field of Classification Search**

CPC A61B 18/1233; A61B 18/1442; A61B 18/1445; A61B 18/1447; A61B 2018/00577; A61B 2018/00589; A61B 2018/00595; A61B 2018/00601; A61B 2018/00607; A61B 2018/0063; A61B 2018/00642; A61B 2018/00666; A61B 2018/00702; A61B 2018/00791; A61B 2018/126; A61B 2018/146; A61B 2017/00057; A61B 5/0059

An electrosurgical system includes an electrosurgical generator, an electrosurgical instrument, an optical clarity sensor and a control component. The electrosurgical generator generates electrosurgical energy for use during electrosurgery. The electrosurgical instrument is coupled to the electrosurgical generator and treats tissue. The optical clarity sensor is coupled to the electrosurgical generator and is adapted to measure tissue with at least two optical frequencies. The control component is operatively coupled to the optical clarity sensor and receives sensor data therefrom. The control component communicates control instructions to the electrosurgical generator to control the generation of the electrosurgical energy.

12 Claims, 2 Drawing Sheets

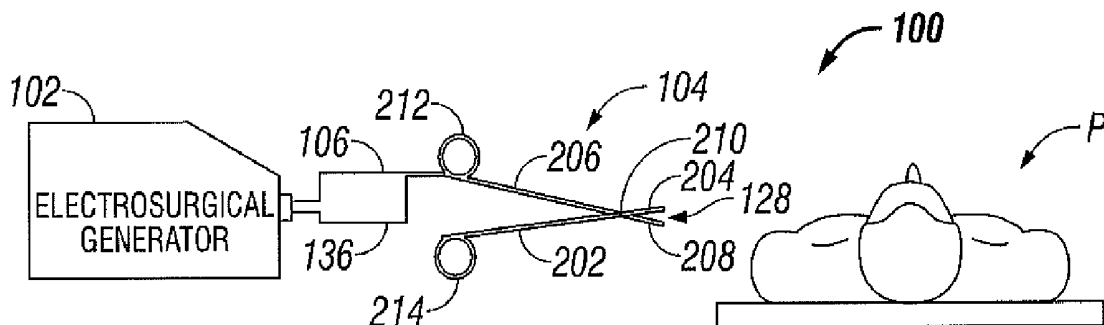

(56)

References Cited

U.S. PATENT DOCUMENTS

1,813,902 A	7/1931	Bovie	4,685,459 A	8/1987	Koch et al.
1,822,330 A	9/1931	Ainslie	4,733,662 A	3/1988	DeSatnick et al.
1,852,542 A	4/1932	Sovatkin	D295,893 S	5/1988	Sharkany et al.
2,002,594 A	5/1935	Wappler et al.	D295,894 S	5/1988	Sharkany et al.
2,011,169 A	8/1935	Wappler	4,754,892 A	7/1988	Retief
2,031,682 A	2/1936	Wappler et al.	4,763,669 A	8/1988	Jaeger
2,054,149 A	9/1936	Wappler	4,805,623 A *	2/1989	Jobsis A61B 5/14551 250/339.12
2,176,479 A	10/1939	Willis	4,827,929 A	5/1989	Hodge
2,305,156 A	4/1941	Grubel	4,829,313 A	5/1989	Taggart
2,279,753 A	4/1942	Knopp	4,846,171 A	7/1989	Kauphusman et al.
2,327,353 A	8/1943	Karle	4,887,612 A	12/1989	Esser et al.
2,632,661 A	8/1948	Cristofv	4,938,761 A	7/1990	Ensslin
2,668,538 A	2/1954	Baker	4,947,009 A	8/1990	Osika et al.
2,796,065 A	6/1957	Kapp	4,985,030 A	1/1991	Melzer et al.
3,073,311 A	1/1963	Tibbs et al.	5,007,908 A	4/1991	Rydell
3,372,288 A	3/1968	Wigington	5,026,370 A	6/1991	Lottick
3,459,187 A	8/1969	Pallotta	5,026,371 A	6/1991	Rydell et al.
3,643,663 A	2/1972	Sutter	5,035,695 A	7/1991	Weber, Jr. et al.
3,648,001 A	3/1972	Anderson et al.	5,037,433 A	8/1991	Wilk et al.
3,651,811 A	3/1972	Hildebrandt et al.	5,042,707 A	8/1991	Taheri
3,678,229 A	7/1972	Osika	5,047,046 A	9/1991	Bodoia
3,720,896 A	3/1973	Beierlein	5,078,716 A	1/1992	Doll
3,763,726 A	10/1973	Hildebrand	5,084,057 A	1/1992	Green et al.
3,779,918 A	12/1973	Ikeda et al.	5,085,659 A	2/1992	Rydell
3,801,766 A	4/1974	Morrison, Jr.	5,099,840 A	3/1992	Goble et al.
3,862,630 A	1/1975	Balamuth	5,100,430 A	3/1992	Avellanet et al.
3,863,339 A	2/1975	Reaney et al.	5,108,392 A	4/1992	Spingler
3,866,610 A	2/1975	Kletschka	5,112,343 A	5/1992	Thornton
3,911,766 A	10/1975	Fridolph et al.	5,116,332 A	5/1992	Lottick
3,920,021 A	11/1975	Hiltebrandt	5,147,357 A	9/1992	Rose et al.
3,921,641 A	11/1975	Hulka	5,151,102 A	9/1992	Kamiyama et al.
3,938,527 A	2/1976	Rioux et al.	5,151,978 A	9/1992	Bronikowski et al.
3,952,749 A	4/1976	Fridolph et al.	5,176,695 A	1/1993	Dulebohn
3,970,088 A	7/1976	Morrison	5,190,541 A	3/1993	Abele et al.
3,987,795 A	10/1976	Morrison	5,196,009 A	3/1993	Kirwan, Jr.
4,005,714 A	2/1977	Hiltebrandt	5,197,964 A	3/1993	Parins
4,016,881 A	4/1977	Rioux et al.	5,209,747 A	5/1993	Knoepfler
4,041,952 A	8/1977	Morrison, Jr. et al.	5,211,655 A	5/1993	Hasson
4,043,342 A	8/1977	Morrison, Jr.	5,215,101 A	6/1993	Jacobs et al.
4,074,718 A	2/1978	Morrison, Jr.	5,217,457 A	6/1993	Delahuerga et al.
4,076,028 A	2/1978	Simmons	5,217,458 A	6/1993	Parins
4,080,820 A	3/1978	Allen	5,217,460 A	6/1993	Knoepfler
4,088,134 A	5/1978	Mazzariello	5,219,354 A	6/1993	Choudhury et al.
4,112,950 A	9/1978	Pike	5,244,462 A	9/1993	Delahuerga et al.
4,127,222 A	11/1978	Adams	5,250,047 A	10/1993	Rydell
4,128,099 A	12/1978	Bauer	5,250,063 A	10/1993	Abidin et al.
4,165,746 A	8/1979	Burgin	5,258,001 A	11/1993	Corman
4,187,420 A	2/1980	Piber	5,258,006 A	11/1993	Rydell et al.
4,233,734 A	11/1980	Bies	5,261,918 A	11/1993	Phillips et al.
4,236,470 A	12/1980	Stenson	5,275,615 A	1/1994	Rose
4,300,564 A	11/1981	Furihata	5,277,201 A	1/1994	Stern
4,311,145 A	1/1982	Esty et al.	5,282,799 A	2/1994	Rydell
D263,020 S	2/1982	Rau, III	5,282,800 A	2/1994	Foshee et al.
4,370,980 A	2/1983	Lottick	5,282,826 A	2/1994	Quadri
4,375,218 A	3/1983	DiGeronimo	5,290,286 A	3/1994	Parins
4,416,276 A	11/1983	Newton et al.	5,300,082 A	4/1994	Sharpe et al.
4,418,692 A	12/1983	Guay	5,304,203 A	4/1994	El-Mallawany et al.
4,443,935 A	4/1984	Zamba et al.	5,308,353 A	5/1994	Beurrier
4,452,246 A	6/1984	Bader et al.	5,308,357 A	5/1994	Lichtman
4,470,786 A	9/1984	Sano et al.	5,313,027 A	5/1994	Inoue et al.
4,492,231 A	1/1985	Auth	5,314,445 A	5/1994	Degwitz et al.
4,493,320 A	1/1985	Treat	5,318,589 A	6/1994	Lichtman
4,503,855 A	3/1985	Maslanka	5,324,289 A	6/1994	Eggers
4,506,669 A	3/1985	Blake, III	D348,930 S	7/1994	Olson
4,509,518 A	4/1985	McGarry et al.	5,326,806 A	7/1994	Yokoshima et al.
4,552,143 A	11/1985	Lottick	5,330,471 A	7/1994	Eggers
4,574,804 A	3/1986	Kurwa	5,330,502 A	7/1994	Hassler et al.
4,597,379 A	7/1986	Kihn et al.	5,334,183 A	8/1994	Wuchinich
4,600,007 A	7/1986	Lahodny et al.	5,334,215 A	8/1994	Chen
4,624,254 A	11/1986	McGarry et al.	5,336,220 A	8/1994	Ryan et al.
4,655,215 A	4/1987	Pike	5,336,221 A	8/1994	Anderson
4,655,216 A	4/1987	Tischer	5,342,359 A	8/1994	Rydell
4,657,016 A	4/1987	Garito et al.	5,342,381 A	8/1994	Tidemand
4,662,372 A	5/1987	Sharkany et al.	5,342,393 A	8/1994	Stack
4,671,274 A	6/1987	Sorochenko	5,344,424 A	9/1994	Roberts et al.
			5,350,391 A	9/1994	Iacovelli
			5,352,222 A	10/1994	Rydell
			5,354,271 A	10/1994	Voda

(56)

References Cited

U.S. PATENT DOCUMENTS

5,356,408 A	10/1994	Rydell	5,564,615 A	10/1996	Bishop et al.
5,366,477 A	11/1994	LeMarie, III et al.	5,569,241 A	10/1996	Edwardds
5,368,600 A	11/1994	Failla et al.	5,569,243 A	10/1996	Kortenbach et al.
5,374,277 A	12/1994	Hassler	5,571,100 A	11/1996	Goble et al.
5,376,089 A	12/1994	Smith	5,573,424 A	11/1996	Poppe
5,383,875 A	1/1995	Bays et al.	5,573,534 A	11/1996	Stone
5,383,897 A	1/1995	Wholey	5,573,535 A	11/1996	Viklund
5,389,098 A	2/1995	Tsuruta et al.	5,575,799 A	11/1996	Bolanos et al.
5,389,103 A	2/1995	Melzer et al.	5,575,805 A	11/1996	Li
5,389,104 A	2/1995	Hahnen et al.	5,578,052 A	11/1996	Koros et al.
5,391,166 A	2/1995	Eggers	5,579,781 A	12/1996	Cooke
5,391,183 A	2/1995	Janzen et al.	5,582,611 A	12/1996	Tsukagoshi et al.
5,396,900 A	3/1995	Slater et al.	5,582,617 A	12/1996	Klieman et al.
5,403,312 A	4/1995	Yates et al.	5,585,896 A	12/1996	Yamazaki et al.
5,403,342 A	4/1995	Tovey et al.	5,590,570 A	1/1997	LeMaire, III et al.
5,405,344 A	4/1995	Williamson et al.	5,591,181 A	1/1997	Stone et al.
5,409,763 A	4/1995	Serizawa et al.	5,597,107 A	1/1997	Knodel et al.
5,411,519 A	5/1995	Tovey et al.	5,601,224 A	2/1997	Bishop et al.
5,411,520 A	5/1995	Nash et al.	5,601,601 A	2/1997	Tal et al.
5,413,571 A	5/1995	Katsaros et al.	5,601,641 A	2/1997	Stephens
5,415,656 A	5/1995	Tihon et al.	5,603,711 A	2/1997	Parins et al.
5,415,657 A	5/1995	Taymor-Luria	5,603,723 A	2/1997	Aranyi et al.
5,422,567 A	6/1995	Matsunaga	5,611,798 A	3/1997	Eggers
5,423,810 A	6/1995	Goble et al.	5,611,808 A	3/1997	Hossain et al.
5,425,690 A	6/1995	Chang	5,611,813 A	3/1997	Lichtman
5,425,739 A	6/1995	Jessen	5,620,415 A	4/1997	Lucey et al.
5,429,616 A	7/1995	Schaffer	5,620,453 A	4/1997	Nallakrishnan
5,431,672 A	7/1995	Cote et al.	5,620,459 A	4/1997	Lichtman
5,431,674 A	7/1995	Basile et al.	5,624,452 A	4/1997	Yates
5,437,292 A	8/1995	Kipshidze et al.	5,626,578 A	5/1997	Tihon
5,438,302 A	8/1995	Goble	5,626,609 A	5/1997	Zvenyatsky et al.
5,439,478 A	8/1995	Palmer	5,630,833 A	5/1997	Katsaros et al.
5,441,517 A	8/1995	Kensley et al.	5,637,110 A	6/1997	Pennybacker et al.
5,443,463 A	8/1995	Stern et al.	5,638,003 A	6/1997	Hall
5,443,464 A	8/1995	Russell et al.	5,643,294 A	7/1997	Tovey et al.
5,443,480 A	8/1995	Jacobs et al.	5,647,869 A	7/1997	Goble et al.
5,445,638 A	8/1995	Rydell et al.	5,647,871 A	7/1997	Levine et al.
5,445,658 A	8/1995	Durrfeld et al.	5,649,959 A	7/1997	Hannam et al.
5,449,480 A	9/1995	Kuriya et al.	5,655,650 A	8/1997	Naitou
5,451,224 A	9/1995	Goble et al.	5,658,281 A	8/1997	Heard
5,454,823 A	10/1995	Richardson et al.	D384,413 S	9/1997	Zlock et al.
5,454,827 A	10/1995	Aust et al.	5,662,667 A	9/1997	Knodel
5,456,684 A	10/1995	Schmidt et al.	5,665,100 A	9/1997	Yoon
5,458,598 A	10/1995	Feinberg et al.	5,667,526 A	9/1997	Levin
5,460,629 A	10/1995	Shlain et al.	5,674,220 A	10/1997	Fox et al.
5,461,765 A	10/1995	Linden et al.	5,674,229 A	10/1997	Tovey et al.
5,462,546 A	10/1995	Rydell	5,681,282 A	10/1997	Eggers et al.
5,472,442 A	12/1995	Klicek	5,688,270 A	11/1997	Yates et al.
5,472,443 A	12/1995	Cordis et al.	5,690,652 A	11/1997	Wurster et al.
5,478,351 A	12/1995	Meade et al.	5,690,653 A	11/1997	Richardson et al.
5,480,406 A	1/1996	Nolan et al.	5,693,051 A	12/1997	Schulze et al.
5,480,409 A	1/1996	Riza	5,693,920 A	12/1997	Maeda
5,484,436 A	1/1996	Eggers et al.	5,695,522 A	12/1997	LeMaire, III et al.
5,496,312 A	3/1996	Klicek	5,700,261 A	12/1997	Brinkerhoff
5,496,317 A	3/1996	Goble et al.	5,700,270 A	12/1997	Peyser et al.
5,496,347 A	3/1996	Hashiguchi et al.	5,702,390 A	12/1997	Austin et al.
5,499,997 A	3/1996	Sharpe et al.	5,707,369 A	1/1998	Vaitekunas et al.
5,509,922 A	4/1996	Aranyi et al.	5,709,680 A	1/1998	Yates et al.
5,512,721 A	4/1996	Young et al.	5,716,366 A	2/1998	Yates
5,514,134 A	5/1996	Rydell et al.	5,720,744 A	2/1998	Eggleston et al.
5,527,313 A	6/1996	Scott et al.	5,722,421 A	3/1998	Francese et al.
5,528,833 A	6/1996	Sakuma	5,725,536 A	3/1998	Oberlin et al.
5,529,067 A	6/1996	Larsen et al.	5,727,428 A	3/1998	LeMaire, III et al.
5,531,744 A	7/1996	Nardella et al.	5,735,848 A	4/1998	Yates et al.
5,536,251 A	7/1996	Evard et al.	5,743,906 A	4/1998	Parins et al.
5,540,684 A	7/1996	Hassler, Jr.	5,752,973 A	5/1998	Kieturakis
5,540,685 A	7/1996	Parins et al.	5,755,717 A	5/1998	Yates et al.
5,540,706 A	7/1996	Aust et al.	5,759,188 A	6/1998	Yoon
5,540,715 A	7/1996	Katsaros et al.	5,762,609 A *	6/1998	Benaron G01N 21/4795 600/473
5,542,945 A	8/1996	Fritzsch	5,766,130 A	6/1998	Selmonosky
5,558,671 A	9/1996	Yates	5,766,166 A	6/1998	Hooven
5,558,672 A	9/1996	Edwards et al.	5,766,170 A	6/1998	Eggers
5,562,619 A	10/1996	Mirarchi et al.	5,766,196 A	6/1998	Griffiths
5,562,699 A	10/1996	Heimberger et al.	5,769,849 A	6/1998	Eggers
5,562,720 A	10/1996	Stern et al.	5,772,655 A	6/1998	Bauer et al.
			5,772,670 A	6/1998	Brosa
			5,776,128 A	7/1998	Eggers
			5,776,130 A	7/1998	Buyse et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

5,779,646 A	7/1998	Koblish et al.	6,004,332 A	12/1999	Yoon et al.
5,779,701 A	7/1998	McBrayer et al.	6,004,335 A	12/1999	Vaitekunas et al.
H1745 H	8/1998	Paraschac	6,010,516 A	1/2000	Hulka et al.
5,792,137 A	8/1998	Carr et al.	6,017,358 A	1/2000	Yoon et al.
5,792,165 A	8/1998	Klieman et al.	6,021,693 A	2/2000	Feng-Sing
5,792,177 A	8/1998	Kaseda	6,024,741 A	2/2000	Williamson et al.
5,797,537 A	8/1998	Oberlin et al.	6,024,743 A	2/2000	Edwards
5,797,927 A	8/1998	Yoon	6,024,744 A	2/2000	Kese et al.
5,797,938 A	8/1998	Paraschac et al.	6,027,522 A	2/2000	Palmer
5,797,941 A	8/1998	Schulze et al.	6,030,384 A	2/2000	Nezhat
5,797,958 A	8/1998	Yoon	6,033,399 A	3/2000	Gines
5,800,449 A	9/1998	Wales	6,039,733 A	3/2000	Buyse et al.
5,807,393 A	9/1998	Williamson, IV et al.	6,041,679 A	3/2000	Slater et al.
5,810,764 A	9/1998	Eggers et al.	6,050,996 A	4/2000	Schmaltz et al.
5,810,805 A	9/1998	Sutcu et al.	6,053,914 A	4/2000	Eggers et al.
5,810,808 A	9/1998	Eggers	6,053,933 A	4/2000	Balazs et al.
5,810,811 A	9/1998	Yates et al.	D424,694 S	5/2000	Tetzlaff et al.
5,810,877 A	9/1998	Roth et al.	D425,201 S	5/2000	Tetzlaff et al.
5,814,043 A	9/1998	Shapeton	6,059,782 A	5/2000	Novak et al.
5,814,054 A	9/1998	Kortenbach et al.	6,066,139 A	5/2000	Ryan et al.
5,817,093 A	10/1998	Williamson, IV et al.	6,074,386 A	6/2000	Goble et al.
5,817,119 A	10/1998	Klieman et al.	6,077,287 A	6/2000	Taylor et al.
5,820,630 A	10/1998	Lind	6,080,180 A	6/2000	Yoon et al.
5,824,978 A	10/1998	Karasik et al.	RE36,795 E	7/2000	Rydell
5,827,271 A	10/1998	Buyse et al.	6,083,223 A	7/2000	Baker
5,827,279 A	10/1998	Hughett et al.	6,086,586 A	7/2000	Hooven
5,827,281 A	10/1998	Levin	6,086,601 A	7/2000	Yoon
5,827,323 A	10/1998	Klieman et al.	6,090,107 A	7/2000	Borgmeier et al.
5,827,548 A	10/1998	Lavallee et al.	6,096,037 A	8/2000	Mulier et al.
5,833,690 A	11/1998	Yates et al.	6,099,550 A	8/2000	Yoon
5,843,080 A	12/1998	Fleenor et al.	6,102,909 A	8/2000	Chen et al.
5,849,022 A	12/1998	Sakashita et al.	6,106,542 A	8/2000	Toybin et al.
5,853,412 A	12/1998	Mayenberger	6,110,171 A	8/2000	Rydell
5,859,527 A	1/1999	Cook	6,113,596 A	9/2000	Hooven et al.
5,860,976 A	1/1999	Billings et al.	6,113,598 A	9/2000	Baker
5,876,401 A	3/1999	Schulze et al.	6,117,158 A	9/2000	Measamer et al.
5,876,412 A	3/1999	Piraka	6,122,549 A	9/2000	Sharkey et al.
5,882,567 A	3/1999	Cavallaro et al.	6,123,701 A	9/2000	Nezhat
5,891,141 A	4/1999	Rydell	H1904 H	10/2000	Yates et al.
5,891,142 A	4/1999	Eggers et al.	6,126,658 A	10/2000	Baker
5,893,863 A	4/1999	Yoon	6,126,665 A	10/2000	Yoon
5,893,875 A	4/1999	O'Connor et al.	6,139,563 A	10/2000	Cosgrove, III et al.
5,893,877 A	4/1999	Gampp, Jr. et al.	6,143,005 A	11/2000	Yoon et al.
5,897,563 A	4/1999	Yoon et al.	6,152,923 A	11/2000	Ryan
5,902,301 A	5/1999	Olig	6,162,220 A	12/2000	Nezhat
5,906,630 A	5/1999	Anderhub et al.	6,171,316 B1	1/2001	Kovac et al.
5,908,420 A	6/1999	Parins et al.	6,174,309 B1	1/2001	Wrublewski et al.
5,908,432 A	6/1999	Pan	6,178,628 B1	1/2001	Clemens et al.
5,911,719 A	6/1999	Eggers	6,179,834 B1	1/2001	Buyse et al.
5,913,874 A	6/1999	Berns et al.	6,179,837 B1	1/2001	Hooven
5,921,916 A	7/1999	Aeikens et al.	6,183,467 B1	2/2001	Shapeton et al.
5,921,984 A	7/1999	Sutcu et al.	6,187,003 B1	2/2001	Buyse et al.
5,925,043 A	7/1999	Kumar et al.	6,190,386 B1	2/2001	Rydell
5,928,136 A	7/1999	Barry	6,190,400 B1	2/2001	VanDeMoer et al.
5,935,126 A	8/1999	Riza	6,193,718 B1	2/2001	Kortenbach et al.
5,941,869 A	8/1999	Patterson et al.	6,206,876 B1	3/2001	Levine et al.
5,944,718 A	8/1999	Dafforn et al.	6,206,877 B1	3/2001	Kese et al.
5,951,546 A	9/1999	Lorentzen	6,206,893 B1	3/2001	Klein et al.
5,951,549 A	9/1999	Richardson et al.	6,214,028 B1	4/2001	Yoon et al.
5,954,720 A	9/1999	Wilson et al.	6,214,034 B1 *	4/2001	Azar 607/89
5,954,731 A	9/1999	Yoon	6,217,602 B1	4/2001	Redmon
5,954,733 A	9/1999	Yoon	6,217,615 B1	4/2001	Sioshansi et al.
5,957,923 A	9/1999	Hahnen et al.	6,221,039 B1	4/2001	Durgin et al.
5,957,937 A	9/1999	Yoon	6,223,100 B1	4/2001	Green
5,960,544 A	10/1999	Beyers	6,224,593 B1	5/2001	Ryan et al.
5,961,514 A	10/1999	Long et al.	6,224,614 B1	5/2001	Yoon
5,964,758 A	10/1999	Dresden	6,228,080 B1	5/2001	Gines
5,976,132 A	11/1999	Morris	6,228,083 B1	5/2001	Lands et al.
5,984,932 A	11/1999	Yoon	6,248,124 B1	6/2001	Pedros et al.
5,984,938 A	11/1999	Yoon	6,248,944 B1	6/2001	Ito
5,984,939 A	11/1999	Yoon	6,261,307 B1	7/2001	Yoon et al.
5,989,277 A	11/1999	LeMaire, III et al.	6,267,761 B1	7/2001	Ryan
5,993,466 A	11/1999	Yoon	6,270,497 B1	8/2001	Sekino et al.
5,993,467 A	11/1999	Yoon	6,270,508 B1	8/2001	Klieman et al.
5,997,565 A	12/1999	Inoue	6,273,887 B1	8/2001	Yamauchi et al.
			6,277,117 B1	8/2001	Tetzlaff et al.
			6,280,458 B1	8/2001	Boche et al.
			6,283,961 B1	9/2001	Underwood et al.
			D449,886 S	10/2001	Tetzlaff et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,298,550	B1	10/2001	Kirwan	6,676,660	B2	1/2004	Wampler et al.
6,302,424	B1	10/2001	Gisinger et al.	6,676,676	B2	1/2004	Danitz et al.
6,319,262	B1	11/2001	Bates et al.	6,679,882	B1	1/2004	Kornerup
6,319,451	B1	11/2001	Brune	6,682,527	B2	1/2004	Strul
6,322,561	B1	11/2001	Eggers et al.	6,682,528	B2	1/2004	Frazier et al.
6,322,580	B1	11/2001	Kanner	6,685,724	B1	2/2004	Haluck
6,325,795	B1	12/2001	Lindemann et al.	6,689,131	B2	2/2004	McClurken
6,334,860	B1	1/2002	Dorn	6,692,445	B2	2/2004	Roberts et al.
6,334,861	B1	1/2002	Chandler et al.	6,693,246	B1	2/2004	Rudolph et al.
6,345,532	B1	2/2002	Coudray et al.	6,695,840	B2	2/2004	Schulze
6,350,264	B1	2/2002	Hooven	6,702,810	B2	3/2004	McClurken et al.
6,352,536	B1	3/2002	Buyse et al.	6,723,092	B2	4/2004	Brown et al.
6,358,249	B1	3/2002	Chen et al.	6,726,068	B2	4/2004	Miller
6,358,259	B1	3/2002	Swain et al.	6,726,686	B2	4/2004	Buyse et al.
6,358,268	B1	3/2002	Hunt et al.	6,726,694	B2	4/2004	Blatter et al.
6,364,879	B1	4/2002	Chen et al.	6,733,498	B2	5/2004	Paton et al.
D457,958	S	5/2002	Dycus et al.	6,736,813	B2	5/2004	Yamauchi et al.
D457,959	S	5/2002	Tetzlaff et al.	6,743,229	B2	6/2004	Buyse et al.
6,387,094	B1	5/2002	Eitenmuller	6,743,230	B2	6/2004	Lutze et al.
6,391,035	B1	5/2002	Appleby et al.	6,743,239	B1	6/2004	Kuehn et al.
6,398,779	B1	6/2002	Buyse et al.	6,743,240	B2	6/2004	Smith et al.
6,402,747	B1	6/2002	Lindemann et al.	6,755,843	B2	6/2004	Chung et al.
6,409,728	B1	6/2002	Ehr et al.	6,756,553	B1	6/2004	Yamaguchi et al.
H2037	H	7/2002	Yates et al.	6,757,977	B2	7/2004	Dambal et al.
6,419,675	B1	7/2002	Gallo, Sr.	D493,888	S	8/2004	Reschke
6,425,896	B1	7/2002	Baltschun et al.	6,770,072	B1	8/2004	Truckai et al.
6,432,112	B2	8/2002	Brock et al.	6,773,409	B2	8/2004	Truckai et al.
6,440,144	B1	8/2002	Bacher	6,773,432	B1	8/2004	Clayman et al.
6,443,952	B1	9/2002	Mulier et al.	6,773,434	B2	8/2004	Ciarrocca
6,443,970	B1	9/2002	Schulze et al.	6,773,441	B1	8/2004	Laufer et al.
6,451,018	B1	9/2002	Lands et al.	6,775,575	B2	8/2004	Bommannan et al.
6,458,125	B1	10/2002	Cosmescu	6,776,780	B2	8/2004	Mulier et al.
6,458,128	B1	10/2002	Schulze	6,786,905	B2	9/2004	Swanson et al.
6,458,130	B1	10/2002	Frazier et al.	6,790,217	B2	9/2004	Schulze et al.
6,461,352	B2	10/2002	Morgan et al.	6,796,981	B2	9/2004	Wham et al.
6,461,368	B2	10/2002	Fogarty et al.	D496,997	S	10/2004	Dycus et al.
6,464,701	B1	10/2002	Hooven et al.	6,800,825	B1	10/2004	Sasaki et al.
6,464,702	B2	10/2002	Schulze et al.	6,802,843	B2	10/2004	Truckai et al.
6,464,704	B2	10/2002	Schmaltz et al.	6,808,525	B2	10/2004	Latterell et al.
6,485,489	B2	11/2002	Teirstein et al.	D499,181	S	11/2004	Dycus et al.
6,494,888	B1	12/2002	Laufer et al.	6,818,000	B2	11/2004	Muller et al.
6,500,176	B1	12/2002	Truckai et al.	6,821,285	B2	11/2004	Laufer et al.
6,506,196	B1	1/2003	Laufer	6,835,200	B2	12/2004	Laufer et al.
6,508,815	B1	1/2003	Strul et al.	6,857,357	B2	2/2005	Fujii
6,511,480	B1	1/2003	Tetzlaff et al.	6,860,880	B2	3/2005	Treat et al.
6,514,215	B1	2/2003	Ouchi	6,887,240	B1	5/2005	Lands et al.
6,514,252	B2	2/2003	Nezhat et al.	6,889,116	B2	5/2005	Jinno
6,517,539	B1	2/2003	Smith et al.	6,914,201	B2	7/2005	Van Vooren et al.
6,527,771	B1	3/2003	Weadock et al.	6,926,716	B2	8/2005	Baker et al.
6,533,784	B2	3/2003	Truckai et al.	6,929,644	B2	8/2005	Truckai et al.
6,545,239	B2	4/2003	Spedale et al.	6,932,810	B2	8/2005	Ryan
6,558,385	B1	5/2003	McClurken et al.	6,932,816	B2	8/2005	Phan
6,562,037	B2	5/2003	Paton et al.	6,934,134	B2	8/2005	Mori et al.
6,569,105	B1	5/2003	Kortenbach et al.	6,936,061	B2	8/2005	Sasaki
6,582,450	B2	6/2003	Ouchi	D509,297	S	9/2005	Wells
6,585,735	B1	7/2003	Frazier et al.	6,942,662	B2	9/2005	Goble et al.
6,602,252	B2	8/2003	Mollenauer	6,943,311	B2	9/2005	Miyako
6,605,790	B2	8/2003	Yoshida	6,953,430	B2	10/2005	Kodooka
6,616,658	B2	9/2003	Ineson	6,953,461	B2	10/2005	McClurken et al.
6,616,661	B2	9/2003	Wellman et al.	6,958,070	B2	10/2005	Witt et al.
6,620,161	B2	9/2003	Schulze et al.	6,960,210	B2	11/2005	Lands et al.
6,620,184	B2	9/2003	De Laforcade et al.	6,964,662	B2	11/2005	Kidooka
6,626,901	B1	9/2003	Treat et al.	6,966,907	B2	11/2005	Goble
6,638,287	B2	10/2003	Danitz et al.	6,972,017	B2	12/2005	Smith et al.
6,641,595	B1	11/2003	Moran et al.	6,977,495	B2	12/2005	Donofrio
6,652,514	B2	11/2003	Ellman et al.	6,979,786	B2	12/2005	Aukland et al.
6,652,521	B2	11/2003	Schulze	6,981,628	B2	1/2006	Wales
6,656,175	B2	12/2003	Francischelli et al.	6,987,244	B2	1/2006	Bauer
6,656,177	B2	12/2003	Truckai et al.	6,994,707	B2	2/2006	Ellman et al.
6,660,072	B2	12/2003	Chatterjee	6,994,709	B2	2/2006	Iida
6,663,639	B1	12/2003	Laufer et al.	6,997,931	B2	2/2006	Sauer et al.
6,663,641	B1	12/2003	Kovac et al.	7,001,381	B2	2/2006	Harano et al.
6,666,854	B1	12/2003	Lange	7,011,657	B2	3/2006	Truckai et al.
6,669,696	B2	12/2003	Bacher et al.	7,033,354	B2	4/2006	Keppel
6,673,092	B1	1/2004	Bacher	7,033,356	B2	4/2006	Latterell et al.
				7,041,102	B2	5/2006	Truckai et al.
				7,044,948	B2	5/2006	Keppel
				7,052,489	B2	5/2006	Griego et al.
				7,052,496	B2	5/2006	Yamauchi

(56)

References Cited

U.S. PATENT DOCUMENTS

7,063,715 B2	6/2006	Onuki et al.	D575,401 S	8/2008	Hixson et al.
D525,361 S	7/2006	Hushka	7,435,249 B2	10/2008	Buyse et al.
7,070,597 B2	7/2006	Truckai et al.	7,442,193 B2	10/2008	Shields et al.
7,083,618 B2	8/2006	Couture et al.	7,442,194 B2	10/2008	Dumbauld et al.
7,083,619 B2	8/2006	Truckai et al.	7,445,621 B2	11/2008	Dumbauld et al.
7,083,620 B2	8/2006	Jahns et al.	7,458,972 B2	12/2008	Keppel
7,087,051 B2	8/2006	Bourne et al.	7,473,253 B2	1/2009	Dycus et al.
7,087,054 B2	8/2006	Truckai et al.	7,481,810 B2	1/2009	Dumbauld et al.
7,090,673 B2	8/2006	Dycus et al.	7,487,780 B2	2/2009	Hooven
7,090,689 B2	8/2006	Nagase et al.	7,491,201 B2	2/2009	Shields et al.
7,101,371 B2	9/2006	Dycus et al.	7,491,202 B2	2/2009	Odom et al.
7,101,372 B2	9/2006	Dycus et al.	7,500,975 B2	3/2009	Cunningham et al.
7,101,373 B2	9/2006	Dycus et al.	7,510,556 B2	3/2009	Nguyen et al.
7,103,947 B2	9/2006	Sartor et al.	7,513,898 B2	4/2009	Johnson et al.
7,107,124 B2	9/2006	Green	7,540,872 B2	6/2009	Schechter et al.
7,112,199 B2	9/2006	Cosmescu	7,549,995 B2	6/2009	Schultz
D531,311 S	10/2006	Guerra et al.	7,553,312 B2	6/2009	Tetzlaff et al.
7,115,123 B2	10/2006	Knowlton et al.	2002/0013583 A1	1/2002	Camran et al.
7,118,570 B2	10/2006	Tetzlaff et al.	2002/0049442 A1	4/2002	Roberts et al.
7,118,587 B2	10/2006	Dycus et al.	2002/0099372 A1	7/2002	Schulze et al.
7,131,860 B2	11/2006	Sartor et al.	2002/0107517 A1	8/2002	Witt et al.
7,131,970 B2	11/2006	Moses et al.	2002/0111624 A1	8/2002	Witt et al.
7,131,971 B2	11/2006	Dycus et al.	2002/0188294 A1	12/2002	Couture et al.
7,135,020 B2	11/2006	Lawes et al.	2003/0014052 A1	1/2003	Buyse et al.
7,137,980 B2	11/2006	Buyse et al.	2003/0014053 A1	1/2003	Nguyen et al.
D533,942 S	12/2006	Kerr et al.	2003/0018331 A1	1/2003	Dycus et al.
7,145,757 B2	12/2006	Shea et al.	2003/0018332 A1	1/2003	Schmaltz et al.
7,147,638 B2	12/2006	Chapman et al.	2003/0032956 A1	2/2003	Lands et al.
7,150,097 B2	12/2006	Sremcich et al.	2003/0069570 A1	4/2003	Witzel et al.
7,150,749 B2	12/2006	Dycus et al.	2003/0069571 A1	4/2003	Treat et al.
7,153,314 B2	12/2006	Laufer et al.	2003/0078578 A1	4/2003	Truckai et al.
D535,027 S	1/2007	James et al.	2003/0109875 A1	6/2003	Tetzlaff et al.
7,156,842 B2	1/2007	Sartor et al.	2003/0114851 A1	6/2003	Truckai et al.
7,156,846 B2	1/2007	Dycus et al.	2003/0139741 A1	7/2003	Goble et al.
7,160,298 B2	1/2007	Lawes et al.	2003/0139742 A1	7/2003	Wampler et al.
7,160,299 B2	1/2007	Baily	2003/0158548 A1	8/2003	Phan et al.
7,169,146 B2	1/2007	Truckai et al.	2003/0158549 A1	8/2003	Swanson
7,179,255 B2	2/2007	Lettice et al.	2003/0171747 A1	9/2003	Kanehira et al.
7,179,258 B2	2/2007	Buyse et al.	2003/0181910 A1	9/2003	Dycus et al.
7,195,631 B2	3/2007	Dumbauld	2003/0216732 A1	11/2003	Truckai et al.
D541,418 S	4/2007	Schechter et al.	2003/0220637 A1	11/2003	Truckai et al.
7,207,990 B2	4/2007	Lands et al.	2003/0229344 A1	12/2003	Dycus et al.
D541,938 S	5/2007	Kerr et al.	2003/0236325 A1	12/2003	Bonora
7,223,264 B2	5/2007	Daniel et al.	2003/0236518 A1	12/2003	Marchitto et al.
7,223,265 B2	5/2007	Keppel	2004/0015163 A1*	1/2004	Buyse et al. 606/34
7,232,440 B2	6/2007	Dumbauld et al.	2004/0030330 A1	2/2004	Brassell et al.
7,241,288 B2	7/2007	Braun	2004/0030332 A1	2/2004	Knowlton et al.
7,241,296 B2	7/2007	Buyse et al.	2004/0049185 A1	3/2004	Latterell et al.
7,244,257 B2	7/2007	Podjahnsky et al.	2004/0064151 A1	4/2004	Mollenauer
7,246,734 B2	7/2007	Shelto, IV	2004/0073238 A1	4/2004	Makower
7,248,944 B2	7/2007	Green	2004/0073256 A1	4/2004	Marchitto et al.
7,252,667 B2	8/2007	Moses et al.	2004/0078035 A1	4/2004	Kanehira et al.
7,255,697 B2	8/2007	Dycus et al.	2004/0082952 A1	4/2004	Dycus et al.
7,267,677 B2	9/2007	Johnson et al.	2004/0087943 A1	5/2004	Dycus et al.
7,270,660 B2	9/2007	Ryan	2004/0115296 A1	6/2004	Duffin
7,270,664 B2	9/2007	Johnson et al.	2004/0116924 A1	6/2004	Dycus et al.
7,276,068 B2	10/2007	Johnson et al.	2004/0116979 A1	6/2004	Truckai et al.
7,300,435 B2	11/2007	Wham et al.	2004/0143263 A1	7/2004	Schechter et al.
7,303,557 B2	12/2007	Wham et al.	2004/0148035 A1	7/2004	Barrett et al.
7,311,709 B2	12/2007	Truckai et al.	2004/0162557 A1	8/2004	Tetzlaff et al.
7,314,471 B2	1/2008	Holman	2004/0193153 A1	9/2004	Sarter et al.
7,318,823 B2	1/2008	Sharps et al.	2004/0199181 A1	10/2004	Knodel et al.
7,329,256 B2	2/2008	Johnson et al.	2004/0210282 A1	10/2004	Flock et al.
7,329,257 B2	2/2008	Kanehira et al.	2004/0224590 A1	11/2004	Rawa et al.
D564,662 S	3/2008	Moses et al.	2004/0230189 A1	11/2004	Keppel
7,338,526 B2	3/2008	Steinberg	2004/0236326 A1	11/2004	Schulze et al.
7,342,754 B2	3/2008	Fitzgerald et al.	2004/0243125 A1	12/2004	Dycus et al.
7,344,268 B2	3/2008	Jhigamian	2004/0249374 A1	12/2004	Tetzlaff et al.
D567,943 S	4/2008	Moses et al.	2004/0260281 A1	12/2004	Baxter, III et al.
7,367,976 B2	5/2008	Lawes et al.	2005/0004564 A1	1/2005	Wham et al.
7,377,920 B2	5/2008	Buyse et al.	2005/0004569 A1	1/2005	Witt et al.
7,384,420 B2	6/2008	Dycus et al.	2005/0033278 A1	2/2005	McClurken et al.
7,384,421 B2	6/2008	Hushka	2005/0059934 A1	3/2005	Wenchell et al.
7,396,336 B2	7/2008	Orszulak et al.	2005/0096645 A1	5/2005	Wellman et al.
D575,395 S	8/2008	Hushka	2005/0101951 A1	5/2005	Wham et al.
			2005/0101952 A1	5/2005	Lands et al.
			2005/0113818 A1	5/2005	Sartor et al.
			2005/0113819 A1	5/2005	Wham et al.
			2005/0113826 A1	5/2005	Johnson et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2005/0149017 A1 7/2005 Dycus
 2005/0149151 A1 7/2005 Orszulak et al.
 2005/0154387 A1 7/2005 Moses et al.
 2005/0187547 A1 8/2005 Sugi
 2005/0197659 A1 9/2005 Bahney
 2005/0203504 A1 9/2005 Wham et al.
 2006/0025760 A1* 2/2006 Podhajsky 606/38
 2006/0052778 A1 3/2006 Chapman et al.
 2006/0052779 A1 3/2006 Hammill
 2006/0064085 A1 3/2006 Schechter et al.
 2006/0064086 A1 3/2006 Odom
 2006/0074417 A1 4/2006 Cunningham et al.
 2006/0079888 A1 4/2006 Mulier et al.
 2006/0079890 A1 4/2006 Guerra
 2006/0079891 A1 4/2006 Arts et al.
 2006/0079933 A1 4/2006 Hushka et al.
 2006/0084973 A1 4/2006 Hushka
 2006/0089670 A1 4/2006 Hushka
 2006/0116675 A1 6/2006 McClurken et al.
 2006/0129146 A1 6/2006 Dycus et al.
 2006/0167450 A1 7/2006 Johnson et al.
 2006/0167452 A1 7/2006 Moses et al.
 2006/0173452 A1 8/2006 Buysse et al.
 2006/0189981 A1 8/2006 Dycus et al.
 2006/0190035 A1 8/2006 Hushka et al.
 2006/0217709 A1 9/2006 Couture et al.
 2006/0229666 A1 10/2006 Suzuki et al.
 2006/0253126 A1 11/2006 Bjerken et al.
 2006/0259036 A1 11/2006 Tetzlaff et al.
 2006/0264922 A1 11/2006 Sartor et al.
 2006/0264931 A1 11/2006 Chapman et al.
 2006/0283093 A1 12/2006 Petrovic et al.
 2006/0287641 A1 12/2006 Perlín
 2007/0016182 A1 1/2007 Lipson et al.
 2007/0016187 A1 1/2007 Weinberg et al.
 2007/0043352 A1 2/2007 Garrison et al.
 2007/0043353 A1 2/2007 Dycus et al.
 2007/0060919 A1 3/2007 Isaacson et al.
 2007/0062017 A1 3/2007 Dycus et al.
 2007/0074807 A1 4/2007 Guerra
 2007/0078456 A1 4/2007 Dumbauld et al.
 2007/0078458 A1 4/2007 Dumbauld et al.
 2007/0078459 A1 4/2007 Johnson et al.
 2007/0088356 A1 4/2007 Moses et al.
 2007/0106295 A1 5/2007 Garrison et al.
 2007/0106297 A1 5/2007 Dumbauld et al.
 2007/0118111 A1 5/2007 Weinberg
 2007/0118115 A1 5/2007 Artale et al.
 2007/0142833 A1 6/2007 Dycus et al.
 2007/0142834 A1 6/2007 Dumbauld
 2007/0156139 A1 7/2007 Schechter et al.
 2007/0156140 A1 7/2007 Baily
 2007/0173811 A1* 7/2007 Couture et al. 606/39
 2007/0173814 A1 7/2007 Hixson et al.
 2007/0179499 A1 8/2007 Garrison
 2007/0179571 A1* 8/2007 De Taboada A61N 5/0613
 607/88
 2007/0198011 A1 8/2007 Sugita
 2007/0213712 A1 9/2007 Buysse et al.
 2007/0255279 A1 11/2007 Buysse et al.
 2007/0260235 A1 11/2007 Podhajsky
 2007/0260238 A1 11/2007 Guerra
 2007/0260241 A1 11/2007 Dalla Betta et al.
 2007/0260242 A1 11/2007 Dycus et al.
 2007/0265616 A1 11/2007 Couture et al.
 2008/0004616 A1 1/2008 Patrick
 2008/0009860 A1* 1/2008 Odom 606/51
 2008/0015575 A1 1/2008 Odom et al.
 2008/0021450 A1 1/2008 Couture
 2008/0033428 A1 2/2008 Artale et al.
 2008/0039835 A1 2/2008 Johnson et al.
 2008/0039836 A1 2/2008 Odom et al.
 2008/0045947 A1 2/2008 Johnson et al.
 2008/0058802 A1 3/2008 Couture et al.
 2008/0082100 A1 4/2008 Orton et al.

2008/0091189 A1 4/2008 Carlton
 2008/0114356 A1 5/2008 Johnson et al.
 2008/0167651 A1 7/2008 Tetzlaff et al.
 2008/0195093 A1 8/2008 Couture et al.
 2008/0215051 A1 9/2008 Buysse et al.
 2008/0221409 A1* 9/2008 Hoarau A61B 5/0075
 600/310
 2008/0243120 A1 10/2008 Lawes et al.
 2008/0249527 A1 10/2008 Couture
 2008/0312653 A1 12/2008 Arts et al.
 2008/0319442 A1 12/2008 Unger et al.
 2009/0012520 A1 1/2009 Hixson et al.
 2009/0018535 A1 1/2009 Schechter et al.
 2009/0024126 A1 1/2009 Artale et al.
 2009/0043304 A1 2/2009 Tetzlaff et al.
 2009/0048596 A1 2/2009 Shields et al.
 2009/0062794 A1 3/2009 Buysse et al.
 2009/0082766 A1 3/2009 Unger et al.
 2009/0082767 A1 3/2009 Unger et al.
 2009/0082769 A1 3/2009 Unger et al.
 2009/0088738 A1 4/2009 Guerra et al.
 2009/0088739 A1 4/2009 Hushka et al.
 2009/0088740 A1 4/2009 Guerra et al.
 2009/0088741 A1 4/2009 Hushka et al.
 2009/0088744 A1 4/2009 Townsend
 2009/0088745 A1 4/2009 Hushka et al.
 2009/0088746 A1 4/2009 Hushka et al.
 2009/0088747 A1 4/2009 Hushka et al.
 2009/0088748 A1 4/2009 Guerra et al.
 2009/0088749 A1 4/2009 Hushka et al.
 2009/0088750 A1 4/2009 Hushka et al.
 2009/0112206 A1 4/2009 Dumbauld et al.
 2009/0131934 A1 5/2009 Odom et al.
 2009/0149853 A1 6/2009 Shields et al.
 2009/0149854 A1 6/2009 Cunningham et al.
 2009/0171350 A1 7/2009 Dycus et al.
 2009/0171353 A1 7/2009 Johnson et al.
 2009/0182327 A1 7/2009 Unger
 2009/0187188 A1 7/2009 Guerra et al.
 2012/0165818 A1* 6/2012 Odom 606/51

FOREIGN PATENT DOCUMENTS

DE 2514501 10/1976
 DE 2627679 1/1977
 DE 3612646 4/1987
 DE 8712328 3/1988
 DE 4303882 8/1994
 DE 4403252 8/1995
 DE 19515914 7/1996
 DE 29616210 1/1997
 DE 19608716 4/1997
 DE 19751106 5/1998
 DE 19751108 5/1999
 DE 19738457 1/2009
 EP 0364216 4/1990
 EP 0467501 1/1992
 EP 0518230 12/1992
 EP 0541930 5/1993
 EP 0572131 12/1993
 EP 0584787 3/1994
 EP 0589453 3/1994
 EP 0589555 3/1994
 EP 0623316 11/1994
 EP 0624348 11/1994
 EP 0650701 5/1995
 EP 0694290 3/1996
 EP 0717966 6/1996
 EP 0754437 3/1997
 EP 0517243 9/1997
 EP 0853922 7/1998
 EP 0875209 11/1998
 EP 0878169 11/1998
 EP 0887046 1/1999
 EP 0923907 6/1999
 EP 0986990 3/2000
 EP 1034747 9/2000
 EP 1034748 9/2000
 EP 1025807 10/2000

(56)

References Cited

FOREIGN PATENT DOCUMENTS

EP	1034746	10/2000
EP	1050278	11/2000
EP	1053719	11/2000
EP	1053720	11/2000
EP	1055399	11/2000
EP	1055400	11/2000
EP	1080694	3/2001
EP	1082944	3/2001
EP	1159926	12/2001
EP	1177771	2/2002
EP	1301135	4/2003
EP	1330991	7/2003
EP	1486177	6/2004
EP	1472984	11/2004
EP	0774232	1/2005
EP	1527747	5/2005
EP	1530952	5/2005
EP	1532932	5/2005
EP	1535581	6/2005
EP	1609430	12/2005
EP	1632192	3/2006
EP	1642543	4/2006
EP	1645238	4/2006
EP	1645240	4/2006
EP	1649821	4/2006
EP	1707143	10/2006
EP	1769765	4/2007
EP	1769766	4/2007
EP	1929970	6/2008
EP	1683496	12/2008
GB	623316	5/1949
GB	1490585	11/1977
GB	2214430 A	6/1989
GB	2213416 A	8/1989
JP	61-501068	9/1984
JP	65-502328	3/1992
JP	5-5106	1/1993
JP	5-40112	2/1993
JP	06343644 A2	12/1994
JP	07265328 A2	10/1995
JP	08056955 A2	3/1996
JP	08252263 A2	10/1996
JP	09010223 A2	1/1997
JP	11244298 A2	9/1999
JP	2000-342599 A2	12/2000
JP	2000-350732 A2	12/2000
JP	2001-008944 A2	1/2001
JP	2001-029356 A2	2/2001
JP	2001-128990 A2	5/2001
SU	401367	11/1974
WO	WO 89/00757	1/1989
WO	WO 92/04873	4/1992
WO	WO 92/06642	4/1992
WO	WO 93/21845	11/1993
WO	WO 94/08524	4/1994
WO	WO 94/20025	9/1994
WO	WO 95/02369	1/1995
WO	WO 95/07662	3/1995
WO	WO 95/15124	6/1995
WO	WO 96/05776	2/1996
WO	WO 96/22056	7/1996
WO	WO 96/13218	9/1996
WO	WO 97/00646	1/1997
WO	WO 97/00647	1/1997
WO	WO 97/10764	3/1997
WO	WO 97/24073	7/1997
WO	WO 97/24993	7/1997
WO	WO 98/27880	7/1998
WO	WO 99/03407	1/1999
WO	WO 99/03408	1/1999
WO	WO 99/03409	1/1999
WO	WO 99/12488	3/1999
WO	WO 99/23933	5/1999
WO	WO 99/40857	8/1999
WO	WO 99/40861	8/1999

WO	WO 99/51158	10/1999
WO	WO 99/66850	12/1999
WO	WO 00/24330	5/2000
WO	WO 00/24331	5/2000
WO	WO 00/36986	6/2000
WO	WO 00/41638	7/2000
WO	WO 00/47124	8/2000
WO	WO 00/53112	9/2000
WO	WO 01/17448	3/2001
WO	WO 01/54604	8/2001
WO	WO 02/07627	1/2002
WO	WO 02/067798	9/2002
WO	WO 02/080783	10/2002
WO	WO 02/080784	10/2002
WO	WO 02/080785	10/2002
WO	WO 02/080786	10/2002
WO	WO 02/080793	10/2002
WO	WO 02/080794	10/2002
WO	WO 02/080795	10/2002
WO	WO 02/080796	10/2002
WO	WO 02/080797	10/2002
WO	WO 02/080798	10/2002
WO	WO 02/080799	10/2002
WO	WO 02/081170	10/2002
WO	WO 03/061500	7/2003
WO	WO 03/090630	11/2003
WO	WO 03/101311	12/2003
WO	WO 2004/032776	4/2004
WO	WO 2004/032777	4/2004
WO	WO 2004/052221	6/2004
WO	WO 2004/073488	9/2004
WO	WO 2004/073490	9/2004
WO	WO 2004/073753	9/2004
WO	WO 2004/082495	9/2004
WO	WO 2004/098383	11/2004
WO	WO 2004/103156	12/2004
WO	WO 2005/004734	1/2005
WO	WO 2005/004735	1/2005
WO	WO 2005/110264	11/2005
WO	WO 2008/045348	4/2008
WO	WO 2008/045350	4/2008
WO	WO 2008/112147	9/2008
WO	WO 2009/005850	1/2009

OTHER PUBLICATIONS

Chung et al., "Clinical Experience of Sutureless Closed Hemorrhoidectomy with LigaSure" Diseases of the Colon & Rectum vol. 46, No. 1 Jan. 2003.

Carbonell et al., "Comparison of theGyrus PlasmaKinetic Sealer and the Valleylab LigaSure Device in the Hemostasis of Small, Medium, and Large-Sized Arteries" Carolinas Laparoscopic and Advanced Surgery Program, Carolinas Medical Center, Charlotte, NC; Date: Aug. 2003.

Peterson et al. "Comparison of Healing Process Following Ligation with Sutures and Bipolar Vessel Sealing" Surgical Technology International (2001).

"Electrosurgery: A Historical Overview" Innovations in Electrosurgery; Sales/Product Literature; Dec. 31, 2000.

Johnson et al. "Evaluation of a Bipolar Electrothermal Vessel Sealing Device in Hemorrhoidectomy" Sales/Product Literature; Jan. 2004.

E. David Crawford "Evaluation of a New Vessel Sealing Device in Urologic Cancer Surgery" Sales/Product Literature 2000.

Johnson et al. "Evaluation of the LigaSure Vessel Sealing System in Hemorrhoidectomy" American College of Surgeons (ACS) Clinica Congress Poster (2000).

Muller et al., "Extended Left Hemicolectomy Using the LigaSure Vessel Sealing System" Innovations That Work, Sep. 1999.

Kennedy et al. "High-burst-strength, feedback-controlled bipolar vessel sealing" Surgical Endoscopy (1998) 12: 876-878.

Carus et al., "Initial Experience With the LigaSure Vessel Sealing System in Abdominal Surgery" Innovations That Work, Jun. 2002.

Heniford et al. "Initial Research and Clinical Results with an Electrothermal Bipolar Vessel Sealer" Oct. 1999.

(56)

References Cited

OTHER PUBLICATIONS

- Heniford et al. "Initial Results with an Electrothermal Bipolar Vessel Sealer" *Surgical Endoscopy* (2000) 15:799-801.
- Herman et al., "Laparoscopic Intestinal Resection With the LigaSure Vessel Sealing System: A Case Report"; *Innovations That Work*, Feb. 2002.
- Koyle et al., "Laparoscopic Palomo Varicocele Ligation in Children and Adolescents" *Pediatric Endosurgery & Innovative Techniques*, vol. 6, No. 1, 2002.
- W. Scott Helton, "LigaSure Vessel Sealing System: Revolutionary Hemostasis Product for General Surgery"; *Sales/Product Literature* 1999.
- LigaSure Vessel Sealing System, the Seal of Confidence in General, Gynecologic, Urologic, and Laparoscopic Surgery; *Sales/Product Literature*; Apr. 2002.
- Joseph Ortenberg "LigaSure System Used in Laparoscopic 1st and 2nd Stage Orchiopexy" *Innovations That Work*, Nov. 2002.
- Sigel et al. "The Mechanism of Blood Vessel Closure by High Frequency Electrocoagulation" *Surgery Gynecology & Obstetrics*, Oct. 1965 pp. 823-831.
- Sampayan et al., "Multilayer Ultra-High Gradient Insulator Technology" *Discharges and Electrical Insulation in Vacuum*, 1998. Netherlands Aug. 17-21, 1998; vol. 2, pp. 740-743.
- Paul G. Horgan, "A Novel Technique for Parenchymal Division During Hepatectomy" *The American Journal of Surgery*, vol. 181, No. 3, Apr. 2001 pp. 236-237.
- Olsson et al. "Radical Cystectomy in Females" *Current Surgical Techniques in Urology*, vol. 14, Issue 3, 2001.
- Palazzo et al. "Randomized clinical trial of Ligasure versus open haemorrhoidectomy" *British Journal of Surgery* 2002, 89, 154-157.
- Levy et al. "Randomized Trial of Suture Versus Electrosurgical Bipolar Vessel Sealing in Vaginal Hysterectomy" *Obstetrics & Gynecology*, vol. 102, No. 1, Jul. 2003.
- "Reducing Needlestick Injuries in the Operating Room" *Sales/Product Literature* 2001.
- Bergdahl et al. "Studies on Coagulation and the Development of an Automatic Computerized Bipolar Coagulator" *J.Neurosurg*, vol. 75, Jul. 1991, pp. 148-151.
- Strasberg et al. "A Phase I Study of the LigaSure Vessel Sealing System in Hepatic Surgery" *Section of HPB Surger*, Washington University School of Medicine, St. Louis MO, Presented at AHPBA, Feb. 2001.
- Sayfan et al. "Sutureless Closed Hemorrhoidectomy: A New Technique" *Annals of Surgery* vol. 234 No. 1 Jul. 2001; pp. 21-24.
- Levy et al., "Update on Hysterectomy—New Technologies and Techniques" *OBG Management*, Feb. 2003.
- Dulemba et al. "Use of a Bipolar Electrothermal Vessel Sealer in Laparoscopically Assisted Vaginal Hysterectomy" *Sales/Product Literature*; Jan. 2004.
- Strasberg et al., "Use of a Bipolar Vessel-Sealing Device for Parenchymal Transection During Liver Surgery" *Journal of Gastrointestinal Surgery*, vol. 6, No. 4, Jul./Aug. 2002 pp. 569-574.
- Sengupta et al., "Use of a Computer-Controlled Bipolar Diathermy System in Radical Prostatectomies and Other Open Urological Surgery" *ANZ Journal of Surgery* (2001) 71.9 pp. 538-540.
- Rothenberg et al. "Use of the LigaSure Vessel Sealing System in Minimally Invasive Surgery in Children" *Int'l Pediatric Endosurgery Group (IPEG)* 2000.
- Crawford et al. "Use of the LigaSure Vessel Sealing System in Urologic Cancer Surgery" *Grand Rounds in Urology* 1999 vol. 1 Issue 4 pp. 10-17.
- Craig Johnson, "Use of the LigaSure Vessel Sealing System in Bloodless Hemorrhoidectomy" *Innovations That Work*, Mar. 2000.
- Levy et al. "Use of a New Energy-based Vessel Ligation Device During Vaginal Hysterectomy" *Int'l Federation of Gynecology and Obstetrics (FIGO) World Congress* 1999.
- Barbara Levy, "Use of a New Vessel Ligation Device During Vaginal Hysterectomy" *FIGO* 2000, Washington, D.C.
- E. David Crawford "Use of a Novel Vessel Sealing Technology in Management of the Dorsal Venous Complex" *Sales/Product Literature* 2000.
- Jarrett et al., "Use of the LigaSure Vessel Sealing System for Peri-Hilar Vessels in Laparoscopic Nephrectomy" *Sales/Product Literature* 2000.
- Crouch et al. "A Velocity-Dependent Model for Needle Insertion in Soft Tissue" *MICCAI* 2005; LNCS 3750 pp. 624-632, Dated: 2005.
- McLellan et al. "Vessel Sealing for Hemostasis During Pelvic Surgery" *Int'l Federation of Gynecology and Obstetrics FIGO World Congress* 2000, Washington, D.C.
- McLellan et al. "Vessel Sealing for Hemostasis During Gynecologic Surgery" *Sales/Product Literature* 1999.
- Int'l Search Report EP 98944778 dated Oct. 31, 2000.
- Int'l Search Report EP 98957771 dated Aug. 9, 2001.
- Int'l Search Report EP 98958575.7 dated Sep. 20, 2002.
- Int'l Search Report EP 04013772 dated Apr. 1, 2005.
- Int'l Search Report EP 04027314 dated Mar. 10, 2005.
- Int'l Search Report EP 04027479 dated Mar. 8, 2005.
- Int'l Search Report EP 04027705 dated Feb. 3, 2005.
- Int'l Search Report EP 04752343.6 dated Jul. 20, 2007.
- Int'l Search Report EP 05002671.5 dated Dec. 22, 2008.
- Int'l Search Report EP 05002674.9 dated Jan. 16, 2009.
- Int'l Search Report EP 05013463.4 dated Sep. 28, 2005.
- Int'l Search Report EP 05013895 dated Oct. 14, 2005.
- Int'l Search Report EP 05016399 dated Jan. 5, 2006.
- Int'l Search Report EP 05017281 dated Nov. 16, 2005.
- Int'l Search Report EP 05019130.3 dated Oct. 18, 2005.
- Int'l Search Report EP 05019429.9 dated May 6, 2008.
- Int'l Search Report EP 05020665.5 dated Feb. 16, 2006.
- Int'l Search Report EP 05020666.3 dated Feb. 17, 2006.
- Int'l Search Report EP 05021197.8 dated Jan. 31, 2006.
- Int'l Search Report EP 05021779.3 dated Jan. 18, 2006.
- Int'l Search Report EP 05021780.1 dated Feb. 9, 2006.
- Int'l Search Report EP 05021937.7 dated Jan. 13, 2006.
- Int'l Search Report—extended—EP 05021937.7 dated Mar. 6, 2006.
- Int'l Search Report EP 05023017.6 dated Feb. 16, 2006.
- Int'l Search Report EP 06002279.5 dated Mar. 22, 2006.
- Int'l Search Report EP 06005185.1 dated Apr. 18, 2006.
- Int'l Search Report EP 06006716 dated Aug. 4, 2006.
- Int'l Search Report EP 06008515.6 dated Jan. 8, 2009.
- Int'l Search Report EP 06008779.8 dated Jun. 13, 2006.
- Int'l Search Report EP 06014461.5 dated Oct. 20, 2006.
- Int'l Search Report EP 06020574.7 dated Sep. 21, 2007.
- Int'l Search Report EP 06020583.8 dated Jan. 30, 2007.
- Int'l Search Report EP 06020584.6 dated Jan. 12, 2007.
- Int'l Search Report EP 06020756.0 dated Feb. 5, 2007.
- Int'l Search Report EP 06 024122.1 dated Mar. 19, 2007.
- Int'l Search Report EP 06024123.9 dated Feb. 26, 2007.
- Int'l Search Report EP 07 001480.8 dated Apr. 12, 2007.
- Int'l Search Report EP 07 001488.1 dated May 29, 2007.
- Int'l Search Report EP 07 009026.1 dated Sep. 12, 2007.
- Int'l Search Report Extended—EP 07 009029.5 dated Jul. 12, 2007.
- Int'l Search Report EP 07 009321.6 dated Aug. 17, 2007.
- Int'l Search Report EP 07 010672.9 dated Oct. 1, 2007.
- Int'l Search Report EP 07 013779.9 dated Oct. 18, 2007.
- Int'l Search Report EP 07 014016 dated Jan. 28, 2008.
- Int'l Search Report EP 07 015191.5 dated Dec. 19, 2007.
- Int'l Search Report EP 07 015601.3 dated Dec. 6, 2007.
- Int'l Search Report EP 07 020283.3 dated Jan. 16, 2008.
- Int'l Search Report EP 07 021646.0 dated Jul. 9, 2008.
- Int'l Search Report EP 07 021647.8 dated May 2, 2008.
- Int'l Search Report EP 08 02692.5 dated Dec. 12, 2008.
- Int'l Search Report EP 08 004655.0 dated Jun. 24, 2008.
- Int'l Search Report EP 08 006732.5 dated Jul. 29, 2008.
- Int'l Search Report EP 08 006917.2 dated Jul. 3, 2008.
- Int'l Search Report EP 08 016539.2 dated Jan. 8, 2009.
- Int'l Search Report PCT/US98/18640 dated Dec. 17, 1998.
- Int'l Search Report PCT/US98/23950 dated Dec. 29, 1998.
- Int'l Search Report PCT/US98/24281 dated Feb. 22, 1999.
- Int'l Search Report PCT/US99/24869 dated Feb. 3, 2000.
- Int'l Search Report PCT/US01/11218 dated Aug. 3, 2001.

(56)

References Cited

OTHER PUBLICATIONS

International Search Report PCT/US01/11224 dated Nov. 13, 2001.
Int'l Search Report PCT/US01/11340 dated Aug. 7, 2001.
Int'l Search Report PCT/US01/11420 dated Oct. 8, 2001.
Int'l Search Report PCT/US02/01890 dated Jul. 17, 2002.
Int'l Search Report PCT/US02/11100 dated Jul. 9, 2002.
Int'l Search Report PCT/US03/28534 dated Dec. 19, 2003.
Int'l Search Report PCT/US04/03436 dated Oct. 5, 2004.
Int'l Search Report PCT/US04/13273 dated Nov. 22, 2004.
Int'l Search Report PCT/US04/15311 dated Nov. 18, 2004.
Int'l Search Report PCT/US07/021438 dated Apr. 1, 2008.
Int'l Search Report PCT/US07/021440 dated Apr. 8, 2008.
Int'l Search Report PCT/US08/61498 dated Sep. 22, 2008.
European Search Report for EP 09 16 8153 dated Dec. 18, 2009.
Int'l Search Report EP 09 152267.2 Dated Jun. 15, 2009.
Int'l Search Report EP 09 152898.4 Dated Jun. 10, 2009.
Int'l Search Report PCT/US09/032690 dated Jun. 16, 2009.
Examination Report for application No. 09 168 153.6 dated Jul. 29, 2016.

* cited by examiner

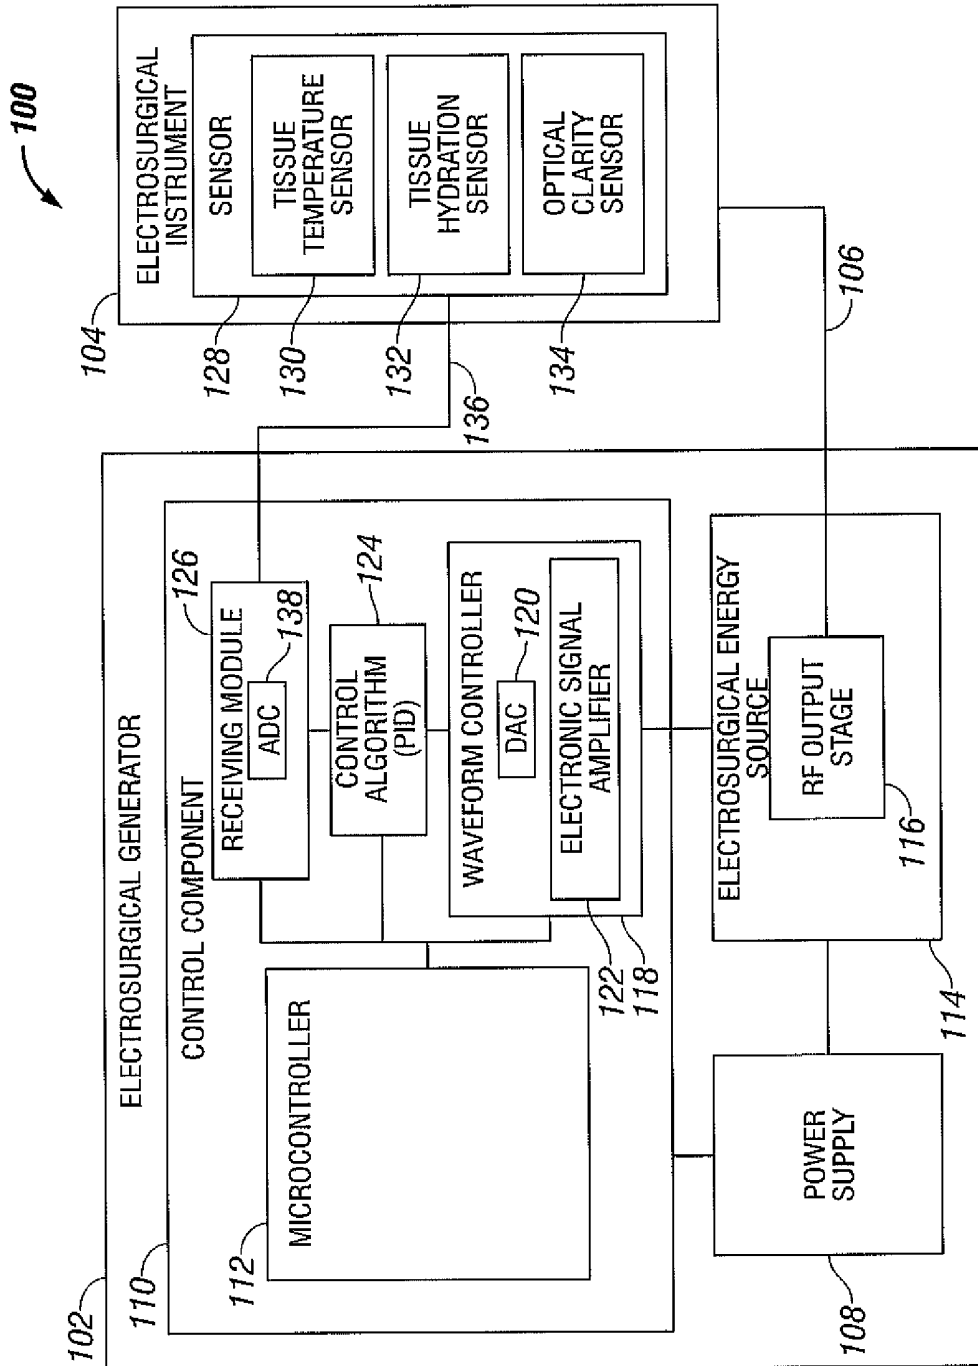


FIG. 1

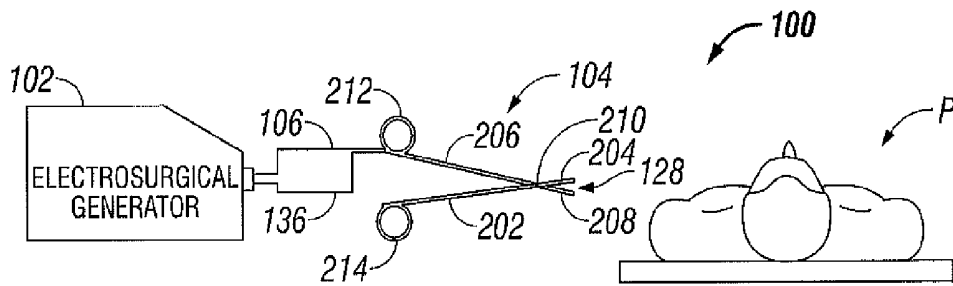


FIG. 2A

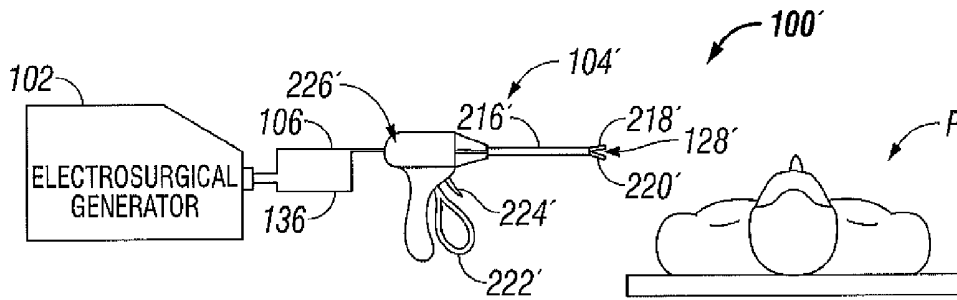


FIG. 2B

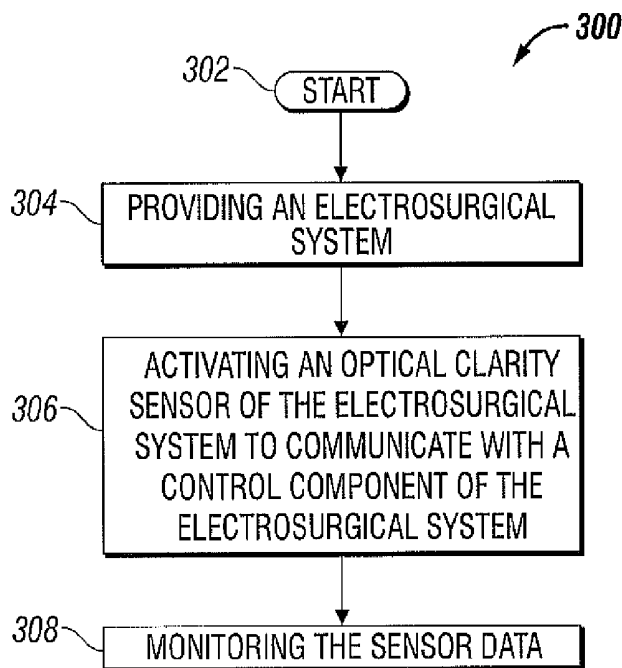


FIG. 3

ELECTROSURGICAL INSTRUMENT INCLUDING A SENSOR

CROSS REFERENCE TO RELATED APPLICATION

This application is related to U.S. application Ser. No. 10/427,832, filed on May 1, 2003 by Buysse et al., now U.S. Pat. No. 7,137,980 entitled "Method and system for controlling output of RF medical generator", the entire contents thereof are hereby incorporated by reference in its entirety herein.

BACKGROUND

Technical Field

The present disclosure relates to an electrosurgical system and method and more particularly, the present disclosure relates to an electrosurgical system and method that includes an electrosurgical instrument with a sensor, such as a temperature sensor, a tissue hydration sensor, and an optical clarity sensor.

Description of Related Art

Electrosurgery is the application of electricity and/or electromagnetic energy to cut or modify biological tissue during a surgical procedure. Generally, electrosurgery utilizes an electrosurgical generator, a return electrode, and a source electrode. The electrosurgical generator produces an electromagnetic wave (referred to herein as "electrosurgery energy"), typically above 100 kilohertz, between the return and source electrodes when applied to tissue. The electromagnetic wave created therebetween dissipates energy as heat as it travels from one electrode to the other. Electromagnetic frequencies above 100 kilohertz are employed to avoid muscle and/or nerve stimulation.

During electrosurgery, current generated by the electrosurgical generator is conducted through the patient's tissue disposed between the two electrodes. The current causes the tissue to heat up as the electromagnetic waves overcome the tissue impedance. Although many other variables affect the total heating of the tissue, usually more current density directly correlates to increased heating. Electrosurgical energy is typically used for cutting, dissecting, ablating, coagulating, and/or sealing tissue.

The two basic types of electrosurgery employed are monopolar and bipolar electrosurgery; however, both types use an "active" and a "return" electrode. In bipolar electrosurgery, the surgical instrument has an active electrode and a return electrode on the same instrument or in very close proximity, usually causing current to flow through a smaller amount of tissue. In monopolar electrosurgery, the return electrode is located elsewhere on the patient's body and is usually not part of the electrosurgical instrument itself. In monopolar electrosurgery, the return electrode is part of a device usually referred to as a return pad.

The effectiveness of the application of electrosurgical energy is affected by a variety of factors, including the patient's age, weight, the type of tissue being modified, and the desired tissue effect. Different voltages, currents, duty cycles and frequencies are used to cause a variety of tissue effects. For example, coagulation requires the application of different electrosurgical energy compared to cutting.

Many electrosurgical procedures require cutting or ligating blood vessels or vascular tissue. A surgeon can cauterize, coagulate, desiccate, and/or reduce bleeding by controlling

the intensity, frequency and duration of the electrosurgical energy applied to the tissue between the electrodes of the electrosurgical instrument.

The process of coagulating vessels is different from electrosurgical vessel sealing. For the purposes herein, "coagulation" is defined as a process of desiccating tissue wherein the tissue cells are ruptured and dried. "Vessel sealing" or "tissue sealing" is defined as the process of liquefying the collagen in the tissue so that it reforms into a fused mass. Coagulation of small vessels is sufficient to permanently close them, while larger vessels need to be sealed to assure permanent closure.

A way to achieve effective operation of the electrosurgical instrument is to monitor the electrosurgical energy directly. Additionally or alternatively, the tissue being acted upon can be monitored. This monitoring can be used in a feedback loop of a control component that controls the generation of the electrosurgical energy.

SUMMARY

The present disclosure relates to an electrosurgical system and method and more particularly, the present disclosure relates to an electrosurgical system and method that includes an electrosurgical instrument with a sensor, such as a temperature sensor, a tissue hydration sensor, and an optical clarity sensor.

In one embodiment of the present disclosure, an electrosurgical system includes an electrosurgical generator, an electrosurgical instrument, an optical clarity sensor and a control component. The electrosurgical generator generates electrosurgical energy for use during electrosurgery. The electrosurgical instrument is coupled to the electrosurgical generator and treats tissue. The optical clarity sensor is coupled to the electrosurgical generator and is adapted to measure tissue with at least two optical frequencies. The control component is operatively coupled to the optical clarity sensor and receives sensor data therefrom. The control component communicates control instructions to the electrosurgical generator to control the generation of the electrosurgical energy.

In another embodiment of the present disclosure, the sensor data includes optical clarity measurements of tissue. The control component instructs the electrosurgical generator to generate the electrosurgical energy corresponding to the optical clarity measurements which corresponds to tissue being less than about 60 degrees Celsius or less than about 100 degrees Celsius.

In another embodiment of the present disclosure, the control component instructs the electrosurgical generator to generate the electrosurgical energy corresponding to at least one optical clarity measurement being in a predetermined range and/or tissue hydration being within a predetermined range. Additionally or alternatively, the control component instructs the electrosurgical generator to generate the electrosurgical energy when the at least one optical clarity measurement falls within a predetermined range.

In another embodiment of the present disclosure, the electrosurgical instrument includes a shaft, a drive assembly, and a movable handle. The shaft has first and second jaw members at a distal end thereof. One or both of the jaw members include an electrode disposed thereon which applies the electrosurgical energy to tissue. One (or both) of the jaw members includes the optical clarity sensor disposed thereon. The drive assembly is operatively coupled to the shaft and moves one of the jaw members relative to the other from a first position to a second position. In the first position,

the first jaw member is disposed in spaced relation relative to the second jaw member and in the second position, the first jaw member grasps tissue. The movable handle actuates the drive assembly.

In another embodiment of the present disclosure, the electrosurgical instrument includes first and second shafts having first and second jaw members, respectively. The second shaft is pivotally connected to the first shaft. One (or both) of the jaw members includes an electrode disposed thereon configured to apply the electrosurgical energy to tissue. One of the jaw members includes the optical clarity sensor disposed thereon.

In another embodiment of the present disclosure, one or more of the optical frequencies of the at least two optical frequencies is adapted to be a reference, is adapted to be substantially absorbed by water and/or is adapted such that water is substantially translucent to the optical frequency. The at least two optical frequencies may include first and second optical frequencies such that the first optical frequency is adapted to be substantially absorbed by water and the second optical frequency is adapted such that water is substantially translucent to the second optical frequency. The sensor data may include a first measurement of the first optical frequency and second measurement of the second optical frequency. The electrosurgical generator can compare the first measurement to the second measurement, e.g., such that at least one of tissue hydration, tissue temperature, optical clarity and tissue thickness is determined.

In yet another embodiment of the present disclosure, an electrosurgical generator includes a control component. The control component includes a receiving module, a waveform controller and a control algorithm. The control component is at least partially implemented by an operative set of processor executable instructions configured for execution by at least one processor. The receiving module is operatively connected to an optical clarity sensor and receives sensor data therefrom. The optical clarity sensor is adapted to measure tissue with at least two optical frequencies and the sensor data includes a tissue temperature sensor measurement, a tissue hydration sensor measurement, and/or an optical clarity sensor measurement utilizing the at least two optical frequencies. The waveform controller communicates control instructions to the electrosurgical generator to control the generation of electrosurgical energy. The control algorithm is in operative communication with the receiving module and the waveform controller. The control algorithm processes the data to calculate the control instructions and communicates the control instructions to the waveform controller.

The control algorithm may be a proportional-integral-derivative control algorithm. The control module may include one or more microcontrollers to execute the operative set of processor executable instructions. The receiving module may include an analog to digital conversion circuit configured to convert the data from an analog signal to a digital signal and/or the waveform controller includes a digital-to-analog conversion circuit configured to convert the control instructions from a digital signal to an analog signal. The waveform controller may include an electronic signal amplifier configured to amplify the analog signal of the control instructions such that the amplified analog signal instructs the electrosurgical generator.

In another embodiment of the present disclosure, a method for controlling generation of electrosurgical energy includes: providing an electrosurgical system; activating an optical clarity sensor of the electrosurgical system to com-

municate with the control component; and monitoring sensor data from the optical clarity sensor.

BRIEF DESCRIPTION OF THE DRAWINGS

These and other advantages will become more apparent from the following detailed description of the various embodiments of the present disclosure with reference to the drawings wherein:

FIG. 1 is a schematic block diagram of an electrosurgical system that includes an electrosurgical instrument with a sensor according to the present disclosure;

FIGS. 2A-2B are schematic block diagrams of an electrosurgical system according to the present disclosure; and

FIG. 3 is a flow chart diagram illustrating a method for using an electrosurgical system that includes an electrosurgical instrument with a sensor according to the present disclosure.

DETAILED DESCRIPTION

Referring to the drawings, FIG. 1 is a block diagram depicting an electrosurgical system 100. Electrosurgical system 100 includes electrosurgical generator 102 that generates electrosurgical energy. The electrosurgical energy is used to perform electrosurgery on a patient using electrosurgical instrument 104.

Electrosurgical generator 102 may have several user interface devices (e.g., touch screens, switches, dials, and the like) to assist a surgeon to achieve the desired results. The surgeon can use the user interface devices to input various data parameters into electrosurgical generator 102. However, not all factors can be known and/or are readily known to the surgeon. For example, the specific physiology of patient P (e.g., age, weight, electrolyte density, PH, osmolarity, fluid volume and pressure, diseases and the like), temperature, humidity, and other factors that may influence electrosurgery, may not be readily known to the surgeon.

Thus, to better assist in ensuring an effective electrosurgical procedure, electrosurgical generator 102 may use several techniques to adjust the applied electrosurgical energy. Some such techniques include calculating or monitoring the tissue impedance, current, voltage, duty cycle, tissue resistance and the like. Electrosurgical generator 102 can use these calculated or monitored properties to make adjustments to the electrosurgical energy applied to tissue by electrosurgical instrument 104. Additionally or alternatively, as is discussed in more detail below, feedback data may be provided to electrosurgical generator 102 by electrosurgical instrument 104.

Electrosurgical instrument 104 can be a monopolar electrosurgical instrument or a bipolar electrosurgical instrument. For example, electrosurgical instrument 104 may be forceps, a vessel sealing electrosurgical instrument, a cutting electrosurgical instrument, or the like. The electrosurgical energy generated by electrosurgical generator 102 is transferred to electrosurgical instrument 104 via cable 106. Cable 106 includes an active path and a return path. The active and/or return paths may be made out of a sufficiently conductive material having an appropriate geometry. For example, cable 106 may be a coaxial cable having a geometry that mitigates attenuation losses within the frequency range of the electrosurgical energy.

Electrosurgical generator 102 may be powered by Alternating Current or Direct Current (referred to herein as "AC" and "DC", respectively); however, it is preferable that electrosurgical generator 102 is powered by a power source

via a standardized receptacle outlet, e.g., a 110 volt outlet as typically found within the United States. Although electro-surgical generator **102** is connected to an external power source, power supply **108** conditions and converts the external power source (e.g., AC power from a outlet) to sufficiently power various parts of electro-surgical generator **102**.

For example, consider that control component **110** includes microcontroller **112**; microcontrollers typically need a DC power source, such as a 5-Volt DC power source. Thus, power supply **108** can also include circuitry to ensure that microcontroller **112** is sufficiently powered, e.g., circuitry that includes transformers, rectifiers, capacitors, voltage regulators, or the like. Additionally, power supply **104** supplies power to control component **110** and electro-surgical energy source **114**.

Electro-surgical energy source **114** includes circuitry sufficient to translate instructions from waveform controller **118** from one form to another form more conducive for interpretation by RF output stage **116**. RF output stage **116** includes circuitry to safely and efficiently transfer the electro-surgical energy to electro-surgical instrument **104**. For example, RF output stage **116** may include an output transformer providing an isolated ground, an output amplifier, impedance matching circuitry to facilitate efficient power transfer, or the like, while electro-surgical energy source **114** may include a variable output power supply connection, voltage scaling circuitry, a buffer such as a voltage follower, or the like.

RF output stage **116** may be connected to cable **106** using an RF connector, such as an coaxial cable female connector, facilitating low attenuation injection of the electro-surgical energy into cable **106**. Also, electro-surgical energy source **114** implements the instructions received from waveform controller **118** while ensuring that RF output stage **116** properly complies with the instructions. For example, waveform controller **118** may send multiple signals regarding the desired characteristics of the electro-surgical energy to be injected into cable **106**, and electro-surgical energy source **114** translates those signals to ensure that RF output stage **116** complies with the instructions by comparing a voltage sense to an RF drive (not depicted in FIG. 1). Additionally or alternatively, electro-surgical energy source **114** may include safety and/or isolation circuitry.

Electro-surgical component **102** also includes control component **110**. Control component **110** may be implemented in hardware, software, firmware, or some combination thereof, and includes waveform controller **118**, control algorithm **124**, and receiving module **126**. For example, control algorithm **124** may be implemented in software processed by microcontroller **112**.

Waveform controller **118** instructs electro-surgical energy source **114** to maintain a particular amplitude, voltage, current, frequency, duty cycle, and/or other properties of the electro-surgical energy for application to tissue. Waveform controller **118** includes a digital to analog converter (referred to herein as a “DAC”) **120** and electronic signal amplifier **122**. Additionally or alternatively, waveform controller **118** may include output relays, scaling relays, and/or an output waveform microcontroller (not depicted). Waveform controller **118** can also instruct the electro-surgical energy source **114** using an analog or a digital signal. For example, waveform controller **118** may have a digital waveform stored therein for converting the waveform to analog form via DAC **120**. Electro-surgical signal amplifier **112** may amplify the analog waveform by a scalar value, e.g., 10, before sending the waveform to electro-surgical energy source **114**.

However, control component **110** determines what properties the electro-surgical energy should have based upon sensor data, specifically, control component **110** can form a feed-back loop with sensor **128**. Sensor **128** may include tissue temperature sensor **130**, tissue hydration sensor **132**, and/or optical clarity sensor **134**. The sensor data is received by receiving module **126** via cable **136**. The sensor data may be in analog or digital form. Additionally or alternatively, the sensor data may be converted from analog to digital form via analog to digital converter (referred to herein as “ADC”) **138**.

The sensor data is processed by control algorithm **124** to calculate the control instructions. The calculated control instructions are communicated to waveform controller **118**. Control algorithm **124** may be a proportional-integral-derivative control algorithm and/or some other control algorithm to facilitate application of the electro-surgical energy to achieve the desired tissue effect.

Referring simultaneously to FIGS. 1, 2A, and 2B, sensor **128** may be located on electro-surgical instrument **104** and is shown in two embodiments by FIGS. 2A and 2B. Electro-surgical instrument **104** may include an active and/or a return electrode, and sensor **128** may be disposed on or near at least one of the electrodes, or otherwise positioned to take at least one tissue measurement of Patient P of FIGS. 2A and 2B. Cable **106** may include an active path and a return path for apply electro-surgical energy to patient P while electro-surgical generator **102** receives sensor data through cable **136**.

Referring to the drawings, FIG. 2A shows an open electro-surgical instrument **104** that includes shaft **202** with jaw member **204** on the end. Electro-surgical instrument **104** also includes shaft **206** with jaw member **208** on the end as well. Shaft **206** is attached to shaft **202** via pivot **210** making them pivotally connected. Pivot **210** may be formed from pins, bearings, axels, or the like to assist in the movement of jaws **204** and **208** relative to each other. Grips **212** and **214** move shafts **206** and **202**, respectively, allowing a surgeon to grip and/or compress tissue of patient P between jaw members **204** and **208**. For example, a surgeon may apply pressure to force grips **212** and **214** together when a vessel is positioned between jaw members **204** and **208**, gripping the vessel. Electro-surgical energy may then be applied between jaw members **204** and **208** by electrodes, sealing the vessel. Sensor **128** may be used by electro-surgical generator **102** to assist in the vessel sealing (discussed in more detail below). Further details relating to open instrument vessel sealing are discussed in commonly-owned U.S. application Ser. No. 10/962,116.

Referring now to FIG. 2B, another embodiment is shown of electro-surgical system **100** for use with an electro-surgical instrument **104'**. Electro-surgical instrument **104'** includes a shaft **216'** that has a distal end that includes jaw members **218'** and **220'**. Within electro-surgical instrument **104'**, a drive assembly (not shown) actuates jaw members **219'** and **220'** so that initially they are spaced by a distance, and, when actuated, move relative to each other. Actuation assembly includes handle **220'** that when “squeezed” causes jaw members **218'** and **220'** to move closer together pivotally, approximately pivoting along their attachment point to the distal end of shaft **216'**. Trigger **226'** causes the electro-surgical generator **102** to apply the electro-surgical energy. Jaw members **220'** and **218'** may each have an active and/or a return electrode. Sensor **128** may be disposed on or near one of the electrodes. Additionally or alternatively, sensor **128**

can be positioned to take at least one measurement of tissue of patient P and send the measurement to electrosurgical generator via cable 136.

Referring again to FIG. 1, as mentioned previously, sensor 128 may include tissue temperature sensor 130, tissue hydration sensor 132, and optical clarity sensor 134, and can communicate data through cable 136 to electrosurgical generator 102; the data may include a tissue temperature measurement, a tissue hydration measurement, and an optical clarity measurement of tissue.

Tissue temperature sensor 130 can measure tissue temperature and communicate one or more tissue temperature measurements to electrosurgical generator 102. The biology of tissue is highly sensitive to temperature. For example, above 60 degrees Celsius, collagen protein denatures causing the tissue bond strength to be reduced. Above 100 degrees Celsius, the water within the cell vaporizes leading to cell destruction. Electrosurgical generator 102 can monitor the tissue temperature via temperature measurements received by receiving module 126 through cable 136, and adjust the electrosurgical energy based upon the received measurements to achieve a desired result, e.g., by keeping the tissue temperature measurements below a value, above a value, and/or within a predetermined range.

For example, for tissue cutting, it may be desirable to generate electrosurgical energy to ensure that the tissue is above about 100 degrees Celsius. In other applications, such as vessel sealing, it is more desirable to maintain a tissue temperature of less than about 60 degrees Celsius. Also, a predetermined range may be used to ensure that the temperature is high enough to cause tissue fusion but low enough to prevent loss of tissue strength. Programming of the tissue temperature desired (or range desired) may be preprogrammed within electrosurgical generator 102, or may manually be set by the operator.

Tissue temperature sensor 130 may include a contact or a non-contact temperature sensor. Tissue temperature sensor 130 also include a ratio or optical pyrometer, a thermal imager temperature sensor, fiber optic based temperature sensor, thermocouples, thermistors, resistance temperature detector ("RTD"), semiconductor, or the like to measure temperature. Note that cable 136 may include one or more conductive cable paths (i.e., wires) and/or may include a fiber optic cable path (also referred to herein as a "fiber optic cable"). Additionally or alternatively, sensor 128 may include additional components or circuitry to aide in the communication of measurements to electrosurgical generator 102. For example, electrosurgical generator 102 may provide power to circuitry within sensor 128 via cable 136 to enable the circuitry to communicate measurements to electrosurgical generator 102 using a pulsed width modulation based communication technique. Also, cable 106 may be bundled with cable 136 (not depicted).

Tissue hydration sensor 132 can communicate to electrosurgical generator 102 a tissue hydration measurement of some tissue of patient P (see FIGS. 2A and 2B). For example, tissue hydration sensor 132 can approximate tissue hydration of the tissue between jaw members 204 and 208 of FIG. 2A, and/or between jaw members 218' and 220' of FIG. 2B. The measurement of the tissue hydration may be accomplished using an optical based sensor, electrical based sensor, or other sufficient tissue hydration sensor. As tissue is heated the water therein may evaporate slowly. The tissue hydration sensor 132 may measure this decreasing tissue hydration and communicate a series of tissue hydration measurements to receiving module 126 via cable 136. Control Algorithm 126 may instruct waveform controller 118 to

continue to apply the electrosurgical energy until the tissue hydration sensor 132 falls within a predetermined threshold.

For example, during electrosurgery a surgeon may use surgical instrument 216 of FIG. 2A to clamp onto a vessel between jaw members 204 and 208. The surgeon may then activate the electrosurgical energy (e.g., by a foot pedal) to start the vessel sealing. The initial tissue hydration measurement of tissue hydration sensor 132 may be, for exemplary purposes only, about 60% water content, and control algorithm 124 may have a predetermined threshold of 30% water content. As the electrosurgical energy is applied, consecutive tissue hydration measurements measured by tissue hydration sensor 132 measures the reducing water content and instructs waveform controller 118 to continue to apply the electrosurgical energy until control algorithm 124 detects an approximate 30% water content tissue hydration measurement. When the 30% water content tissue hydration measurement is detected, control algorithm 124 may instruct waveform controller 118 to stop applying electrosurgical energy to electrosurgical instrument 104. An alarm and/or an indicator may indicate to the surgeon that the vessel is sealed.

Referring simultaneously to FIGS. 1, 2A, and 2B, sensor 128 includes optical clarity sensor 134. Optical clarity sensor 134 may use optical frequencies which may be visible or outside of visual perception to make an optical clarity measurement.

Referring to FIG. 2A, an optical source may inject photons from jaw member 204 through tissue and to jaw member 208 where an absorption and/or transparency measurement can be made. Jaw member 204 may include an LED, a laser, a fiber optical coupling lens, or the like. Additionally or alternatively, cable 136 may include a fiber optic cable that carries light from electrosurgical generator 102 that is focused to travel from jaw member 204 through tissue and to jaw member 208. Jaw member 208 may include a fiber optic coupling lens to gather the photons and carry them back to electrosurgical generator 102 through a fiber optic cable located within cable 136.

For example, electrosurgical generator 102 may include a semiconductor based laser that injects photons into a fiber optic cable within cable 136. The photons travel down the core of the fiber optic cable to jaw member 204, where a lens injects the photons into tissue contained within jaw members 204 and 208. Jaw member 208, in this example, contains a lens that couples the photons back into a fiber optic cable that carries the photons to electrosurgical generator 102. Receiving module 126 may include photodetector that measures the amount of photons that are received, and converts received photons into an electronic signal. Referring to FIG. 2B, jaw members 218' and 220' may behave similarly to the jaw members 204 and 208 of FIG. 2A, with regards to optical clarity sensor 134.

Optical clarity sensor 134 may utilize a broadband optical wavelength that has a relatively large bandwidth, e.g., a wavelength produced by a LED source. Additionally or alternatively, optical clarity sensor 134 may utilize several optical wavelengths to measure wavelength-dependent optical clarity of the tissue.

For example, optical clarity sensor 134 may use a first wavelength that is more readily absorbed by water than by other molecules found within the tissue, and a second wavelength that is more readily absorbed by a particular protein found throughout human tissue. When the electrosurgical energy is applied to the tissue, the absorption characteristics of the two wavelengths may be compared. If a surgeon is applying too much pressure to the tissue causing

the tissue to be “squeezed out” of the jaw members, both wavelengths should have an increase in optical transmissibility because the tissue is “thinning” between the jaw members. However, if only the first wavelength (the one that is more readily absorbed by the water) has an increase of optical transmissibility while the second wavelength maintains its optical transmissibility measurement, the reasons for the changes to the optical transmissibility of the first wavelength is more likely to be due to the evaporation of water. Therefore, optical clarity sensor **134** may use multiple optical wavelengths to communicate an optical clarity sensor measurement to electrosurgical generator **102** to measure wavelength-dependent optical clarity, e.g., by using wave division multiplexing.

Referring to the drawings, FIG. **3** is a flow chart diagram illustrating a method **300** for using an electrosurgical system that includes an electrosurgical instrument with a sensor. Method **300** starts at step **302** and includes providing an electrosurgical system **304**. The electrosurgical system of step **302** may be electrosurgical system **100** as shown in FIGS. **1**, **2A**, **2B**, a monopolar electrosurgical system, or a bipolar electrosurgical system. The electrosurgical system of step **304** includes an optical clarity sensor and a control component. Method **300** further includes step **306** which is activating the optical clarity sensor of the electrosurgical system (of step **304**) to communicate with a control component of the electrosurgical system (of step **304**). The sensor of step **306** may be sensor **128** of FIG. **1** and includes optical clarity sensor **134**. Also, the control component may be control component **110** of FIG. **1**. Additionally, method **300** includes monitoring the sensor data **308**. The sensor data of step **308** may be communicated via cable **136** to control component **110**, that is received by receiving module **126** of FIG. **1**.

While several embodiments of the disclosure have been shown in the drawings, it is not intended that the disclosure be limited thereto, as it is intended that the disclosure be as broad in scope as the art will allow and that the specification be read likewise. Therefore, the above description should not be construed as limiting, but merely as exemplifications of particular embodiments. Those skilled in the art will envision other modifications within the scope and spirit of the claims appended hereto.

What is claimed is:

1. An electrosurgical system, comprising:
 - an electrosurgical generator configured to generate electrosurgical energy for use during electrosurgery;
 - an electrosurgical instrument operatively coupled to the electrosurgical generator and configured to treat tissue;
 - a light source operatively coupled to the electrosurgical generator, the light source configured to transmit light through a first side of the tissue;
 - an optical clarity sensor operatively coupled to the electrosurgical generator and configured to detect light from the light source transmitted through the tissue at a second, opposing side of the tissue, wherein the optical clarity sensor is adapted to measure the light transmitted through the tissue at at least two optical frequencies, wherein the light at a first optical frequency of the at least two optical frequencies is readily absorbed by water and the light at a second optical frequency of the at least two optical frequencies is readily absorbed by protein found in tissue; and
 - a control component operatively coupled to the optical clarity sensor configured to receive sensor data therefrom, wherein the control component is configured to compare absorption characteristics of the tissue at the at

least two optical frequencies and communicate control instructions to the electrosurgical generator to control the generation of the electrosurgical energy.

2. An electrosurgical system according to claim **1**, wherein the sensor data includes at least one optical clarity measurement of tissue, wherein the control component is configured to instruct the electrosurgical generator to generate the electrosurgical energy corresponding to the at least one optical clarity measurement corresponding to tissue being less than about 60 degrees Celsius.

3. An electrosurgical system according to claim **1**, wherein the sensor data includes at least one optical clarity measurement of tissue, wherein the control component is configured to instruct the electrosurgical generator to generate the electrosurgical energy corresponding to the at least one optical clarity measurement being less than about 100 degrees Celsius.

4. An electrosurgical system according to claim **1**, wherein the sensor data includes at least one optical clarity measurement of tissue, wherein the control component is configured to instruct the electrosurgical generator to generate the electrosurgical energy corresponding to the at least one optical clarity measurement being in a predetermined range.

5. An electrosurgical system according to claim **1**, wherein the sensor data includes at least one optical clarity measurement of tissue, wherein the control component is configured to instruct the electrosurgical generator to generate the electrosurgical energy when the at least one optical clarity measurement corresponds to tissue hydration being within a predetermined range.

6. An electrosurgical system according to claim **1**, wherein the electrosurgical instrument includes:

- a shaft having a first jaw member and a second jaw member at a distal end thereof, at least one of said jaw members including an electrode disposed thereon configured to apply the electrosurgical energy to tissue, wherein at least one of the jaw members includes the optical clarity sensor disposed thereon and the other jaw member includes the light source disposed thereon;
- a drive assembly operatively coupled to the shaft which is positionable to move at least one of the first jaw member or second jaw member relative to the other from a first position wherein the first jaw member is disposed in spaced relation relative to the second jaw member to a second position wherein the first and second jaw members are configured to grasp tissue; and
- a movable handle which actuates the drive assembly.

7. An electrosurgical system according to claim **1**, wherein the electrosurgical instrument includes:

- a first shaft having a first jaw member; and
- a second shaft having a second jaw member, wherein the second shaft is pivotally connected to the first shaft, at least one of said jaw members includes an electrode disposed thereon configured to apply the electrosurgical energy to tissue, at least one of the jaw members includes the optical clarity sensor disposed thereon.

8. The electrosurgical system according to claim **1**, wherein an optical frequency of the at least two optical frequencies is a reference frequency.

9. The electrosurgical system according to claim **1**, wherein an optical frequency of the at least two optical frequencies is adapted such that water is substantially translucent to the optical frequency.

10. The electrosurgical system according to claim **1**, wherein the light at the first optical frequency of the at least two optical frequencies is adapted to be substantially

absorbed by water and the light at the second optical frequency of the at least two optical frequencies is adapted such that water is substantially translucent to the second optical frequency.

11. The electrosurgical system according to claim 10, 5 wherein the sensor data includes a first measurement of the first optical frequency and a second measurement of the second optical frequency, wherein the electrosurgical generator is configured to compare the first measurement to the second measurement. 10

12. The electrosurgical system according to claim 10, wherein the sensor data includes a first measurement of the first optical frequency and a second measurement of the second optical frequency, wherein the electrosurgical generator is configured to compare the first measurement to the second measurement such that at least one of tissue hydration, tissue temperature, optical clarity and tissue thickness is determined. 15

* * * * *

专利名称(译)	电外科器械包括传感器		
公开(公告)号	US9603652	公开(公告)日	2017-03-28
申请号	US12/195624	申请日	2008-08-21
[标]申请(专利权)人(译)	CARLTON约翰·D· ODOM DARREN		
申请(专利权)人(译)	CARLTON约翰·D· ODOM DARREN		
当前申请(专利权)人(译)	COVIDIEN LP		
[标]发明人	CARLTON JOHN D ODOM DARREN		
发明人	CARLTON, JOHN D. ODOM, DARREN		
IPC分类号	A61B18/14 A61B18/12 A61B18/00 A61B5/00 A61B17/00		
CPC分类号	A61B18/1206 A61B5/0059 A61B18/1442 A61B5/0008 A61B18/1445 A61B2017/00057 A61B2018/00702 A61B2018/00791		
其他公开文献	US20100049187A1		
外部链接	Espacenet USPTO		

摘要(译)

电外科系统包括电外科发生器，电外科器械，光学透明度传感器和控制部件。电外科发生器产生电外科能量以在电外科手术期间使用。电外科器械耦合到电外科发生器并治疗组织。光学透明度传感器耦合到电外科发生器并适于测量具有至少两个光学频率的组织。控制部件可操作地耦合到光学透明度传感器并接收传感器数据。控制部件将控制指令传送到电外科发生器以控制电外科能量的产生。

