



US 20020115914A1

(19) **United States**(12) **Patent Application Publication****Russ**(10) **Pub. No.: US 2002/0115914 A1**(43) **Pub. Date: Aug. 22, 2002**(54) **PATIENT MONITORING AREA NETWORK****Publication Classification**(76) Inventor: **Tomas Russ**, Carlisle, MA (US)(51) **Int. Cl.<sup>7</sup>** ..... **A61B 5/00**(52) **U.S. Cl.** ..... **600/300; 128/903**


Correspondence Address:

**Siemens Corporation  
Intellectual Property Department  
186 Wood Avenue South  
Iselin, NJ 08830 (US)**(21) Appl. No.: **10/075,674**(22) Filed: **Feb. 13, 2002****Related U.S. Application Data**

(60) Provisional application No. 60/268,770, filed on Feb. 14, 2001.

(57) **ABSTRACT**

A system that allows patient monitoring data obtained by patient connected devices to be transferred by wireless signals to another device such as a patient monitoring processor. The same patient connected devices are used to transfer data to the patient monitor processor or a central station depending on the location of the patient. A single device is used for both a personal area network and a telemetry/transport application. The same wireless technology is used in both situations and eliminates the need to deploy more than one antenna/receiver system. Existing wireless transfer protocols such as Bluetooth are used, thereby reducing transmission power when the two communicating devices are in close proximity.

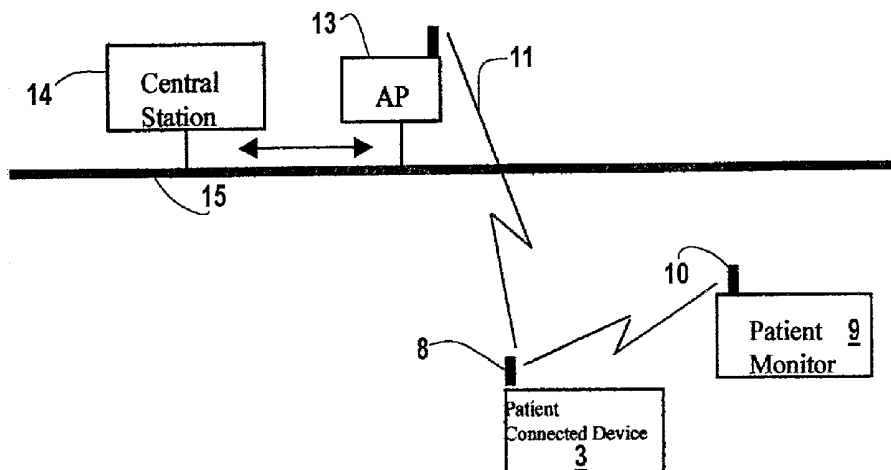

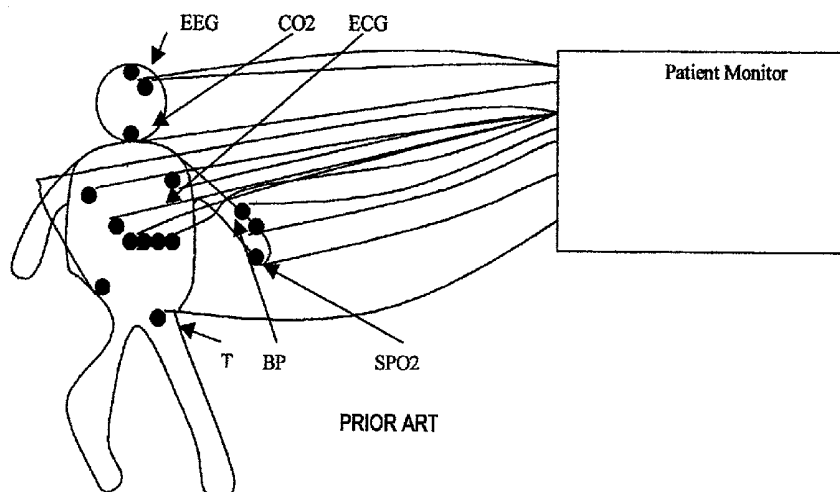


Figure 1

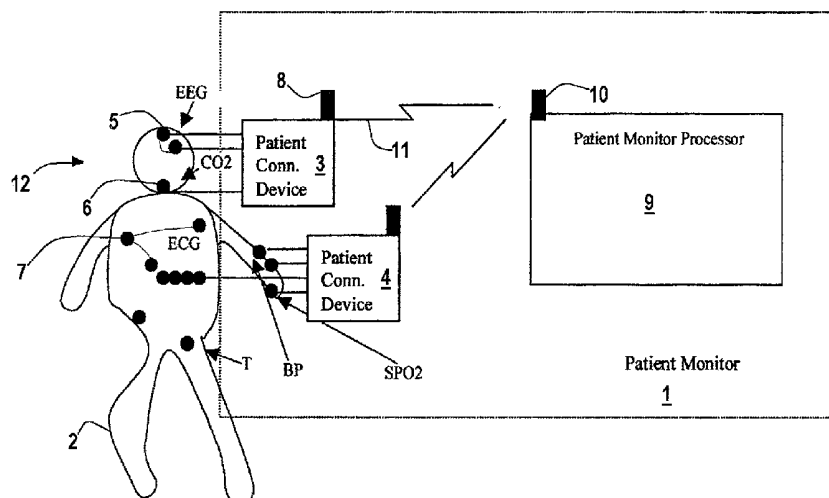


Figure 2

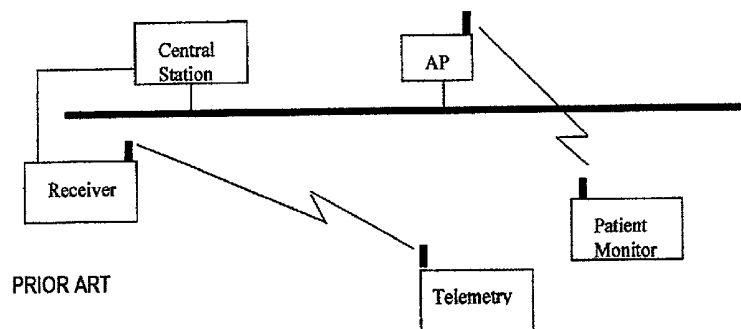
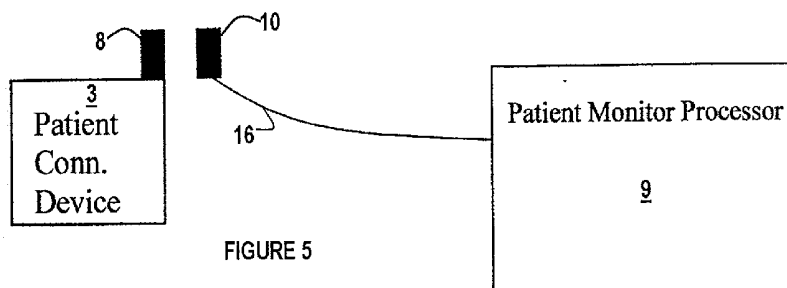
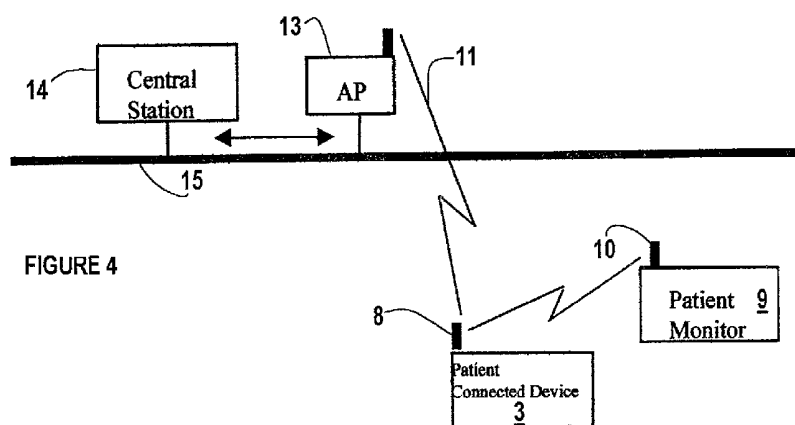


Figure 3



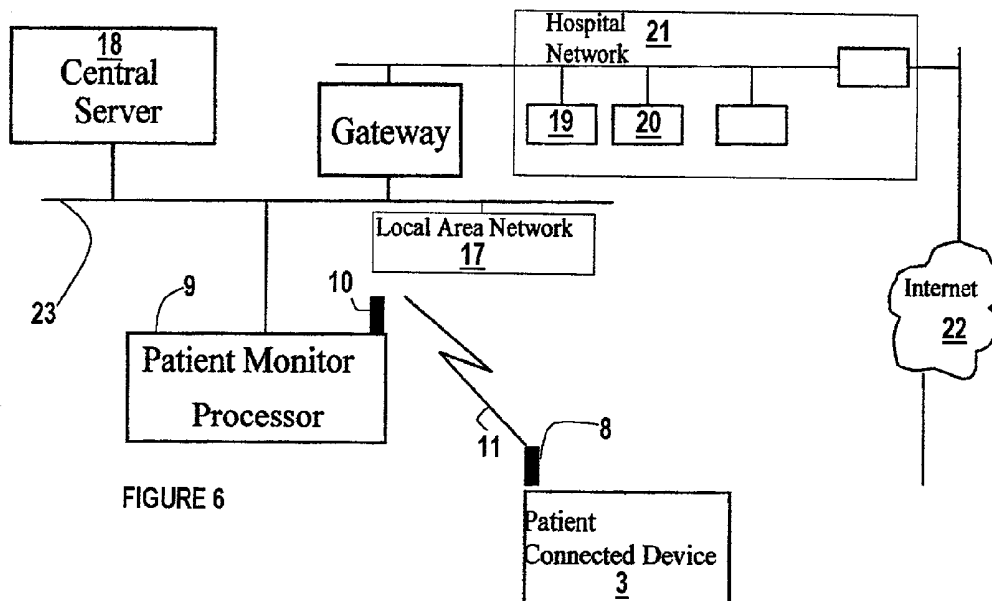


FIGURE 6

## PATIENT MONITORING AREA NETWORK

[0001] This application is based on provisional patent application No. 60/268,770 filed on Feb. 14, 2001.

## FIELD OF THE INVENTION

[0002] This invention relates generally to the field of medical devices and more particularly to a wireless data gathering and transmission system to be used with patients receiving treatment in a hospital.

## BACKGROUND OF THE INVENTION

[0003] In a typical patient monitoring environment several electrodes or sensors are attached to a patient and then connected through wires to a Patient Monitor Processor as depicted in **FIG. 1**. In an operating room, for example, wires from five, six or ten electrocardiogram (EKG) electrodes, an SpO<sub>2</sub> sensor, a CO<sub>2</sub> sensor, one, two or four pressure transducers, a pressure cuff, one or more temperature transducers and EEG electrodes may have to be connected between the patient and the Patient Monitoring Processor. This presents a particularly complex cable management problem for the attending physician or nurse. Considerable time can be consumed in disentangling the patient when they must be disconnected or transferred to another area of the hospital. Ideally, a reduction or elimination of all of the cable connections between the patient and the Patient Monitor Processor could be achieved. This could be effectively accomplished by the use of two way wireless transmission and reception between one or more Patient Connected Devices and the Patient Monitor Processor while using the same underlying wireless technology.

[0004] Wireless data acquisition systems are well known in the biomedical area. For example, U.S. Pat. No. 5,704,351 issued to Mortara discloses a multiple channel biomedical digital telemetry transmitter. Mortara teaches an eight channel biomedical transmitter specifically directed to an electrocardiogram (EKG) signal transmission in the 902 to 928 MHz band. The Mortara device includes input circuitry and an analog to digital converter which receives the input signal from an EKG electrode and converts it to a digital signal which is inputted to a microprocessor. The microprocessor then converts the digital signal to a serial digital output signal which is used to frequency modulate the radio frequency carrier signal for telemetry transmission. The carrier frequency is adjustable within the 902 to 928 MHz band by two manual frequency setting switches. The use of these manual switches is the only adjustment available on the Mortara device and is capable only of manually setting the specific frequency within the 902 to 928 MHz band. The input circuitry and analog to digital converter are not adjustable or adaptable to accept different input signal characteristics. Further, the Mortara device cannot be adjusted by programming or otherwise to operate in any other frequency band. Finally, the Mortara device is only a transmitter and is unable to receive RF or other signals to control its operation.

[0005] Similarly, U.S. Pat. No. 5,755,230, issued to Schmidt et al. discloses a device for monitoring a physiological signal, in particular an EEG, and transmitting the signal by RF to a receiver. Like Mortara, the Schmidt et al. device cannot be modified or adjusted to receive inputs from different physiological sensors.

[0006] U.S. Pat. No. 5,579,775, entitled DYNAMIC CONTROL OF A PATIENT MONITORING SYSTEM, issued to Dempsey discloses a patient monitoring system with a telemetry subsystem which monitors and transmits an RF signal representing the signals it receives from one or more physiological monitoring instruments. Unlike Mortara and Schmidt et al., Dempsey teaches a receiving subsystem which can receive RF signals in a backchannel arrangement in order to control the operation of the system. However, Dempsey does not include the capability to adjust or modify the input by programming or otherwise in response to different physiological signals. The device relies on separate monitoring sections in order to accommodate different physiological signals such as EEG, EKG and SpO<sub>2</sub>.

[0007] U.S. Pat. No. 5,417,222, also issued to Dempsey, discloses a portable processor which may be interconnected to a telemetry monitor at the I/O port. The Dempsey '222 device includes a telemetry monitor comprising a physiological monitor which receives selected physiological signals indicating a specific physiological condition of the patient. The physiological monitor is a specific type of monitor that reads signals of a specific physiological function such as EKG, for example. In the event that a different physiological function is to be monitored such as EEG a different physiological monitor must be employed. In particular, Dempsey '222 discloses the interface of a programmable processor (the Hewlett Packard 100LX palmtop processor) with a physiological monitor. The device is not able to adapt or change the physiological monitor, by software or otherwise, to accept different physiological signals.

[0008] The Fluke corporation manufactures a wireless data acquisition system under the trade name of "Wireless Logger". The "Wireless Logger" is an integration of Fluke's Hydra Data Logger, a portable instrument monitor/analyzer, which accepts wired external inputs, with an RF modem. The Hydra Data Logger includes a universal input module which accepts and conditions external inputs. The resulting signals are transmitted by the modem to another modem interconnected to a personal computer. The separate modem and universal input module are relatively large and consume up to ten watts of power. The operation of the system is not software programmable. RF Neulink markets a similar system utilizing the VHF (136-280 MHz) and UHF (403-512 MHz) bands.

[0009] U.S. Pat. No. 6,167,258, entitled PROGRAMMABLE WIRELESS DATA ACQUISITION SYSTEM, issued to Schmidt et al, discloses the use of a signal processing module which is capable of accepting multiple external inputs having different characteristics and ranges. The '258 Schmidt et al. device, through programming, converts and conditions the external inputs, generates an RF signal encoded with data corresponding to the external inputs and transmits the signal to a base station.

[0010] U.S. Pat. No. 6,230,049, entitled INTEGRATED SYSTEM FOR EEG MONITORING AND ELECTRICAL STIMULATION WITH A MULTIPLICITY OF ELECTRODES, issued to Fischell et al., discloses an integrated EEG monitoring and electrical stimulation system that has a wireless link between a patient electronics module and an EEG analysis workstation.

[0011] In general, the prior art attempts at monitoring and transferring patient data are illustrated in **FIGS. 1 and 3**. In

none of these cases is the same patient connected device used to transfer data to either a patient monitor processor or a central station with the same underlying wireless technology. Accordingly, a need remains for a system based on the same underlying technology that allows patient monitoring data collected by multiple monitors connected to a patient to be wirelessly transferred to another device such as a Patient Monitoring Processor for the purpose of displaying, synchronizing and processing the data.

#### SUMMARY OF THE INVENTION

[0012] The present invention is a system that allows patient monitoring data collected by one or more sensors or devices connected to a patient to be wirelessly transferred to another device, such as a patient monitoring processor. The transferred data may be displayed, synchronized and otherwise processed. The patient monitoring processor may be located in close proximity to the patient or at some distance depending on the mode of operation of the patient monitoring system. The wireless data transfer operates in both directions, that is, data can also be transferred from the patient monitor processor to the patient connected devices. The same patient connected device is used to transfer and receive data to or from either a patient monitor processor, a central station or both depending on the state of the patient without any alteration of the patient connected device hardware.

#### BRIEF DESCRIPTION OF THE DRAWINGS

[0013] FIG. 1 is a schematic diagram of a prior art system for monitoring a patient;

[0014] FIG. 2 is a schematic diagram of a patient monitoring system constructed according to the principles of the present invention;

[0015] FIG. 3 is a schematic diagram of a prior art patient monitoring telemetry system;

[0016] FIG. 4 is a schematic diagram of wireless patient monitoring system constructed according to the principles of the present invention;

[0017] FIG. 5 is a schematic diagram of an antenna arrangement used in the system depicted in FIG. 2; and

[0018] FIG. 6 a schematic diagram of a patient monitoring processor subsystem as utilized in the system depicted in FIG. 2.

#### DETAILED DESCRIPTION OF THE INVENTION

[0019] Referring to FIG. 2, a two way wireless patient monitoring system is shown generally at 1. The patient 2 is attached to a plurality of patient connected devices 3 and 4. Patient connected device 3, for example, contains an EEG sensor 5, carbon dioxide monitor 6 and an ECG sensor 7. Each sensor 5, 6 and 7 is interconnected to a common device 3 which contains suitable data gathering electronics as well as an RF transceiver interconnected to antenna 8. Also contained within the common device 3 is microprocessor which enables the device 3 to function as a slave station in a piconet. Patient connected device 4 operates in a manner similar to patient connected device 3.

[0020] A patient monitoring processor 9 includes a microprocessor and RF transceiver which is interconnected to antenna 10. Signals 11 are transferred between the patient connected device 3 and the patient monitoring processor 9 which can act as either a master or slave station within a wireless cell without any change of the patient monitoring processor hardware. The wireless data is transferred using any suitable protocol of which the Bluetooth standard is an example. Bluetooth technology provides a universal radio interface in the 2.45 GHz frequency band that enables portable electronic devices to connect and communicate wirelessly via short range ad hoc networks.

[0021] Bluetooth technology is described for example in Haartsen, "Bluetooth, The Universal Radio Interface for Ad Hoc, Wireless Connectivity", Ericsson Review No. 3, 1998, pp. 110-117. A wireless cell or "piconet" composed of the patient monitoring processor 9 acting in this case as the master station and the patient connected devices 3 and 4 acting as slave stations permits the transfer of physiological data from any of the patient connected devices 3 and 4 to the patient monitoring processor 9 for the purpose of displaying data, interpreting data and synchronizing the operation of the several patient connected devices. This architecture creates a personal area network 12.

[0022] Referring also to FIG. 4, the same patient connected devices 3 and 4 (device 4 not shown) are also able to transfer data to a device other than the patient monitor processor 9. In particular, there will be instances where the patient 2 is being transferred from one area to another or perhaps is well enough to be able to walk around the area on her own. In those instances there would still be a desire to monitor the patient from a distance. The patient connected device 3 can transmit the data signal 11 to the patient monitor 9, but can also simultaneously or serially (consecutively) transmit the data signal 11 to an auxiliary processor 13, depending on the location of the patient 2. The auxiliary processor 13 is interconnected to a central station 14 by a conventional network 15.

[0023] Referring also to FIG. 5, the power of the wireless transceiver housed within the patient connected device 3 can be adjusted to minimize interference with other piconets in the area, and to minimize the number of receiving stations when transferring telemetry. Existing Bluetooth specifications are designed to reduce transmission power when the two communicating devices are in close proximity. The benefit of reduced power consumption is to extend battery life of the patient connected device 3 and to reduce the likelihood of interference with other nearby wireless devices. Ideally the antennae of both communicating devices should be as close together as possible. The Bluetooth master antenna 10 which is connected to the patient monitor processor 9 is located at the end of an extension cable 16 in order to reduce the distance to the antenna 8 of patient connected device 3.

[0024] The present system 12 separates the physiological signal acquisition (obtained via patient connected devices 3 and 4) from the backend processing and display of the signals accomplished by the patient monitor processor 9. Referring also to FIG. 6, the E patient monitor processor is a standard workstation or web browser device. The patient monitor processor 9 is connected to a local area network 17 and performs functions not only as the local display for

patient monitoring but also retrieves other useful information for the physician who may reside elsewhere. Such information for example is contained in a central database server **18** on the local area network **17**, or the information may be contained in other places **19**, **20** in the overall hospital network **21**. Information may also be obtained from the internet **22**. The patient monitor processor **9** may be used as a local display and also as a window into other medical and nonmedical information accessible through the network connection **23**.

I claim:

1. A patient area network, comprising:

(a) at least one patient connected device, comprising

a sensor adapted to detect and store at least one physiological parameter from a patient; and

a radio frequency transceiver adapted to communicate with a patient monitor processor

(b) a patient monitor processor adapted to receive wireless physiological data from the patient connected device and to transmit wireless instructions to the patient connected device, the patient monitor processor being configured to act as one of (i) a master station within a cell and (ii) a slave station within a cell.

2. The patient area network of claim 1 wherein the patient monitor processor is configured to:

display physiological data received from each patient connected device;

interpret physiological data received from each patient connected device; and

synchronize operation of each patient connected device with every other patient connected device;

3. The patient area network of claim 2 further comprising a central station adapted to send and receive data from each patient connected device.

4. The patient area network of claim 3 wherein the central station further comprises:

a radio frequency transceiver configured to communicate with each patient connected device.

5. The patient area network of claim 4 further comprising a wireless data transfer protocol adapted to reduce transmission power in response to close proximity of a patient connected device to any data receiving device within the cell.

6. The patient area network of claim 5 further comprising:

a master antenna; and

an extension cable interconnecting the master antenna and the patient monitor processor configured to decrease separation between the patient connected device and the patient monitor processor.

7. The patient area network of claim 6 wherein the patient monitor processor comprises a web browser.

8. The patient area network of claim 7 wherein the patient monitor processor is interconnected to a local area network.

9. The patient area network of claim 8 wherein the local area network comprises an internet connection.

10. A method of monitoring physiological signals from a patient, comprising the steps of:

attaching at least one physiological parameter sensor to a patient;

interconnecting the physiological parameter sensor to a first wireless transceiver;

transmitting a physiological data signal from the first wireless transceiver to a patient monitor processor;

interconnecting the patient monitor processor to a second wireless transceiver transmitting informational data from the second wireless transceiver to the first wireless transceiver; and

designating the patient monitor processor as one of (a) a master station in a wireless cell and (b) a slave station in a wireless cell.

11. The method of claim 10, further comprising the steps of:

interconnecting an auxiliary processor to a central station;

transmitting data from the first wireless transceiver to the auxiliary processor; and

transmitting data from the auxiliary processor to the first wireless transceiver.

12. The method of claim 11 further comprising the step of communicating between the first wireless transceiver and the auxiliary processor by means of a wireless protocol that reduces transmission power as path length between the first wireless transceiver and the auxiliary processor decreases.

13. The method of claim 12, further comprising the step of interconnecting an antenna to the second wireless transceiver by means of an extension cable so as to decrease the path length between the antenna and the first wireless transceiver.

14. The method of claim 13, further comprising the step of configuring the patient monitor processor as a web browser.

15. The method of claim 14 further comprising the step of interconnecting the patient monitor processor to a local area network.

16. The method of claim 15 further comprising the step of linking the local area network to an internet connection.

17. A method of monitoring physiological signals from a patient, comprising the steps of:

attaching at least one physiological parameter sensor to a patient;

interconnecting the physiological parameter sensor to a first wireless transceiver;

conditioning a physiological data signal for at least one of, (a) an ambulatory patient mode and (b) a non-ambulatory patient mode; and

transmitting said physiological data signal from the first wireless transceiver to a patient monitor processor.

18. The method of claim 17 further comprising the step of adaptively selecting between said ambulatory patient mode and said non-ambulatory patient mode in response to user command.

19. The method of claim 17 wherein

said transmitting step uses a single transmitter for both said ambulatory patient mode and said non-ambulatory patient mode.

20. The method of claim 17 further comprising the steps of

attaching a plurality of physiological parameter sensors of different type to a patient;

interconnecting said physiological parameter sensors-to at least one wireless transceiver;

conditioning physiological data signals containing different types of physiological data for at least one of, (a) an ambulatory patient mode and (b) a non-ambulatory patient mode; and

transmitting said physiological data signals from said at least one wireless transceiver to a patient monitor processor.

21. The method of claim 20 including the step of

using a map for dynamically allocating said physiological data signals to corresponding ports on said at least one transceiver.

22. The method of claim 20 wherein

said different types of physiological data include at least two of, (a) EKG data, (b) ECG data, (c) EEG data, (d) blood pressure data, (e) respiratory data, (f) blood parameter data, (g) pulse rate data and (h) muscle activity associated data.

\* \* \* \* \*



专利名称(译)	患者监测区域网络		
公开(公告)号	<a href="#">US20020115914A1</a>	公开(公告)日	2002-08-22
申请号	US10/075674	申请日	2002-02-13
[标]申请(专利权)人(译)	RUSS TOMAS		
申请(专利权)人(译)	RUSS TOMAS		
当前申请(专利权)人(译)	德尔格医疗系统公司.		
[标]发明人	RUSS TOMAS		
发明人	RUSS, TOMAS		
IPC分类号	A61B5/00 A61B5/0476		
CPC分类号	A61B5/0006 A61B5/0024 A61B5/145 Y10S128/903 Y10S128/904		
优先权	60/268770 2001-02-14 US		
其他公开文献	US6749566		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

#### 摘要(译)

允许患者监测由患者连接的设备获得的数据的系统通过无线信号传输到诸如患者监测处理器的另一设备。根据患者的位置，使用相同的患者连接设备将数据传输到患者监视器处理器或中心站。单个设备用于个人区域网络和遥测/传输应用。在这两种情况下都使用相同的无线技术，无需部署多个天线/接收器系统。使用诸如蓝牙的现有无线传输协议，从而当两个通信设备非常接近时降低传输功率。

