



(19) **United States**

(12) **Patent Application Publication**  
**Hanoun**

(10) **Pub. No.: US 2012/0029936 A1**

(43) **Pub. Date: Feb. 2, 2012**

(54) **ERGONOMIC/PHYSIOTHERAPY PROGRAMME MONITORING SYSTEM AND METHOD OF USING SAME**

(76) Inventor: **Reed Hanoun, Mississauga (CA)**

(21) Appl. No.: **13/255,800**

(22) PCT Filed: **Mar. 11, 2009**

(86) PCT No.: **PCT/CA09/00303**

§ 371 (c)(1),  
(2), (4) Date: **Oct. 14, 2011**

**Publication Classification**

(51) **Int. Cl.**  
**G06Q 50/00** (2012.01)  
**A61B 5/00** (2006.01)

(52) **U.S. Cl.** ..... **705/2; 600/300**

(57) **ABSTRACT**

A user's personal biometric information such as age, sex, weight, height as well as the use's lifestyle information, such as job description, smoker status and physical fitness, and any injury or malady type is uploaded onto a host computer.

Target heart rate, energy and/or caloric consumption levels related to wellness or rehabilitation goals for a particular job type and injury are then selected having regard to fitness levels for an individual of comparable age, performing a similar job function are then downloaded to a wearable monitoring unit. The wearable monitoring unit (WMU) is provided for measuring the user's heart rate and dynamic energy and/or caloric expenditure over one to four weeks. The wearable monitoring unit includes a heart rate monitor, a unit accelerometer, a global positioning system (GPS), one or more force-micro-sensors, and an audio and/or video output. The audio/video output is operable to provide information and/or motivational prompts to the user in the event the heart rate, energy expenditure and/or caloric expenditure falls below or exceeds preselected target expenditures over a particular time segment of the selected time period. A display provides a continuously updated visual indication of whether or not the use has achieved the preselected optimum caloric burn or energy expenditure for that particular time segment. The WMU is provided with an internal calendar/clock, a processor and/or memory. The processor compares wellness or measured heart rate and energy expenditure for multiple time segments against target levels stored as the user-specific wellness or rehabilitative physiotherapy programme tailored to provide the maximum therapeutic benefit to the user. The comparison is then used to generate compliance output data to either the user and/or the employer.

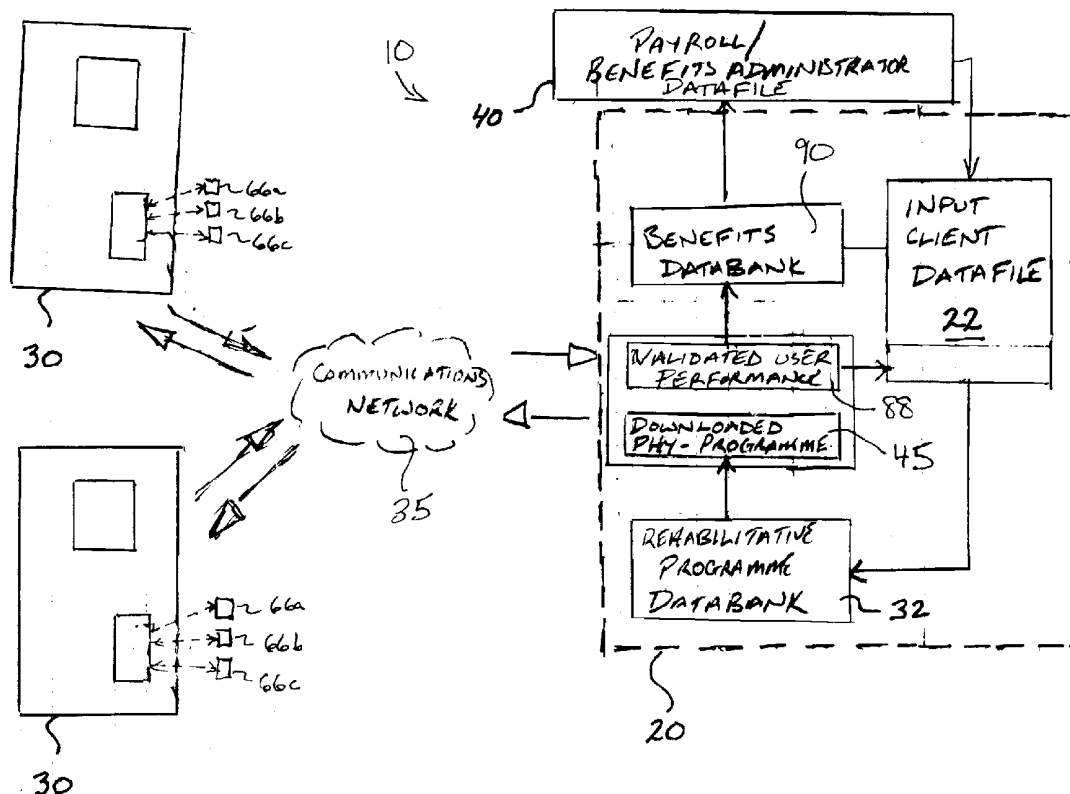


Fig. 1

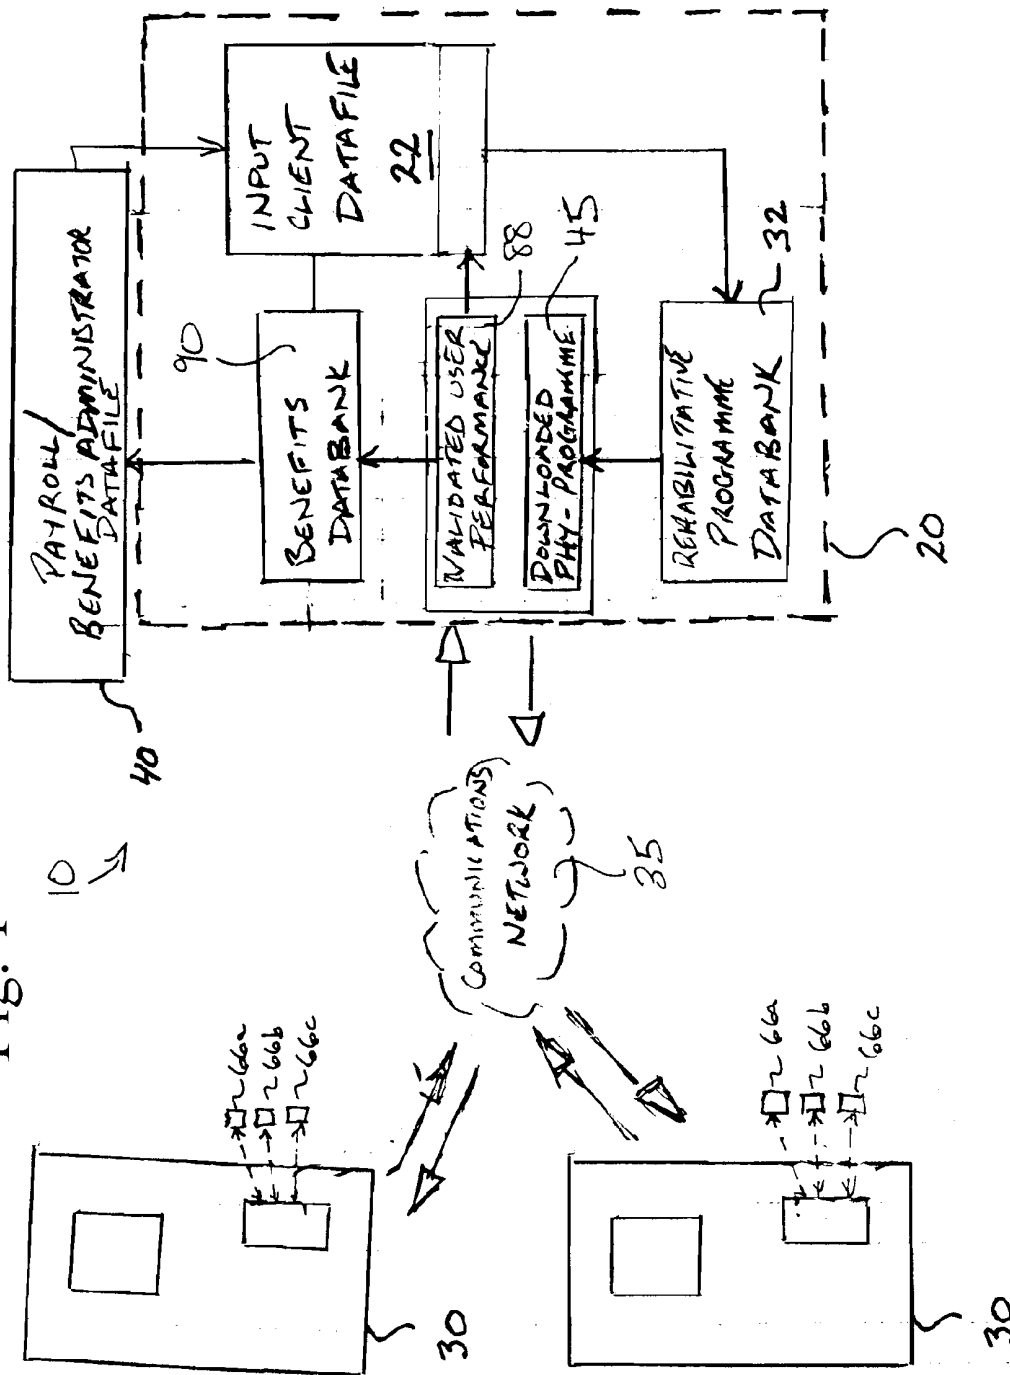


Fig. 2


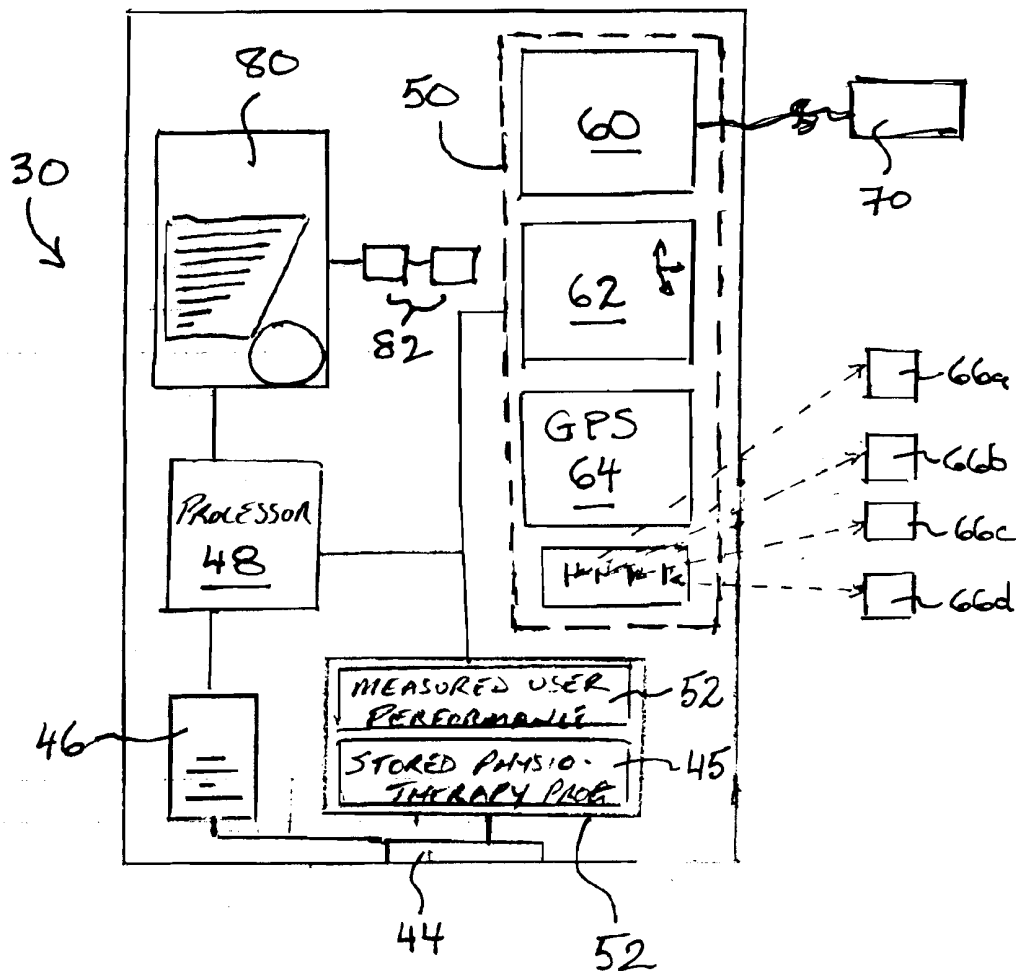


Fig. 3

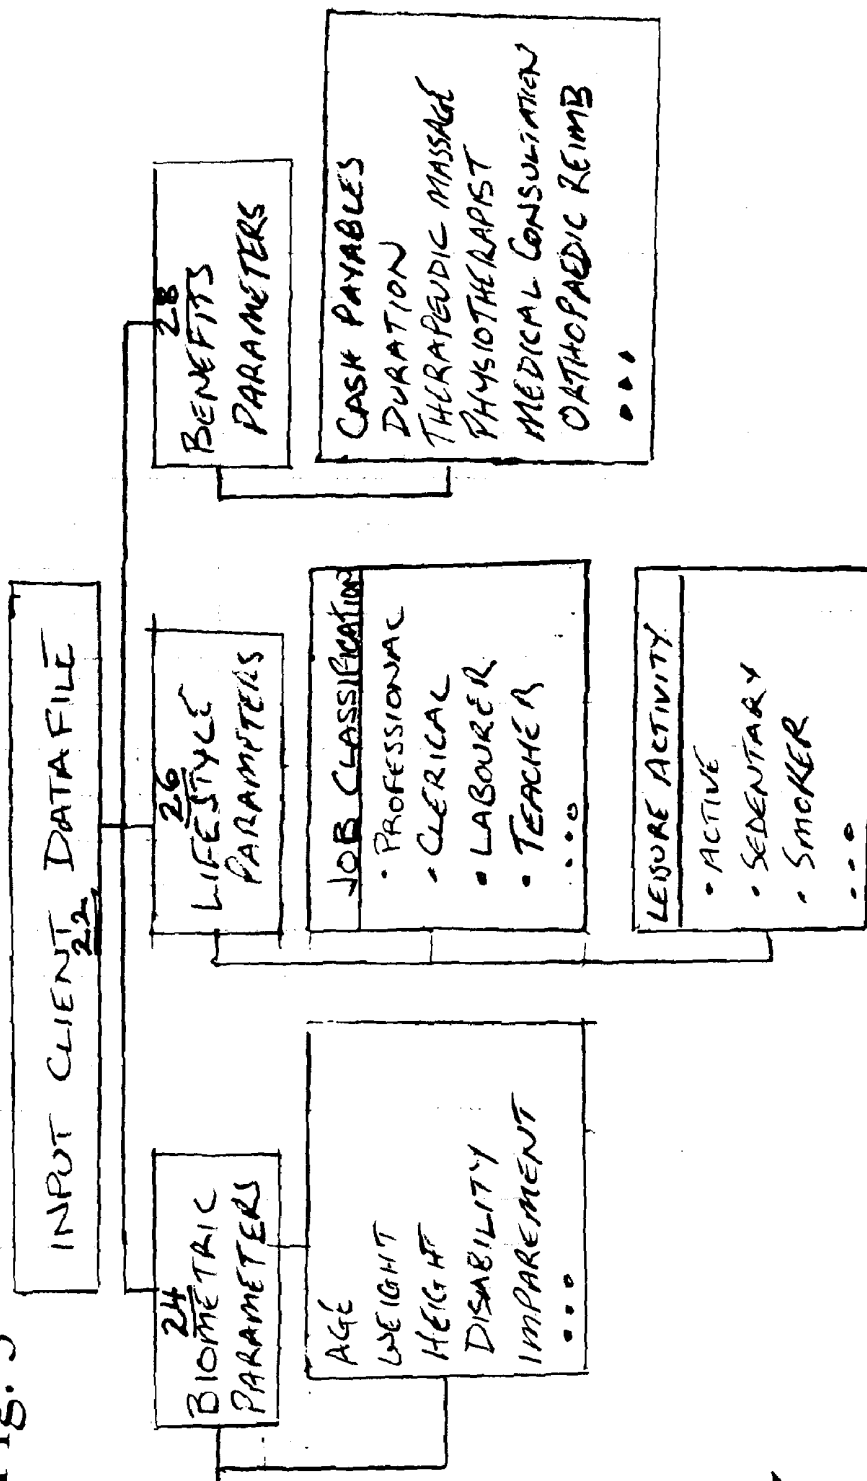

22 →

Fig. 4

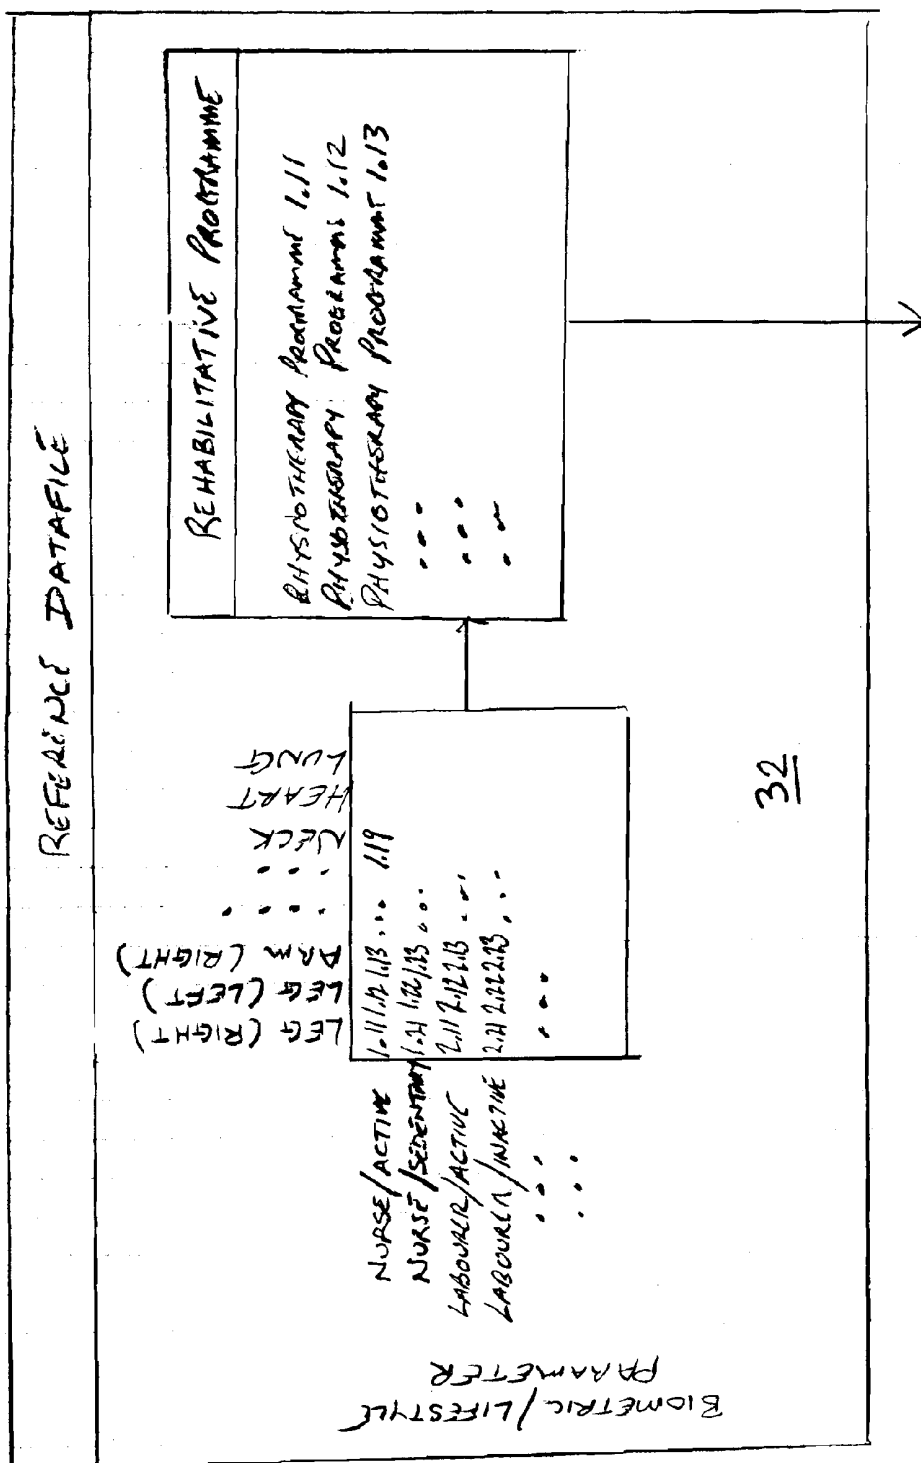


Fig. 5


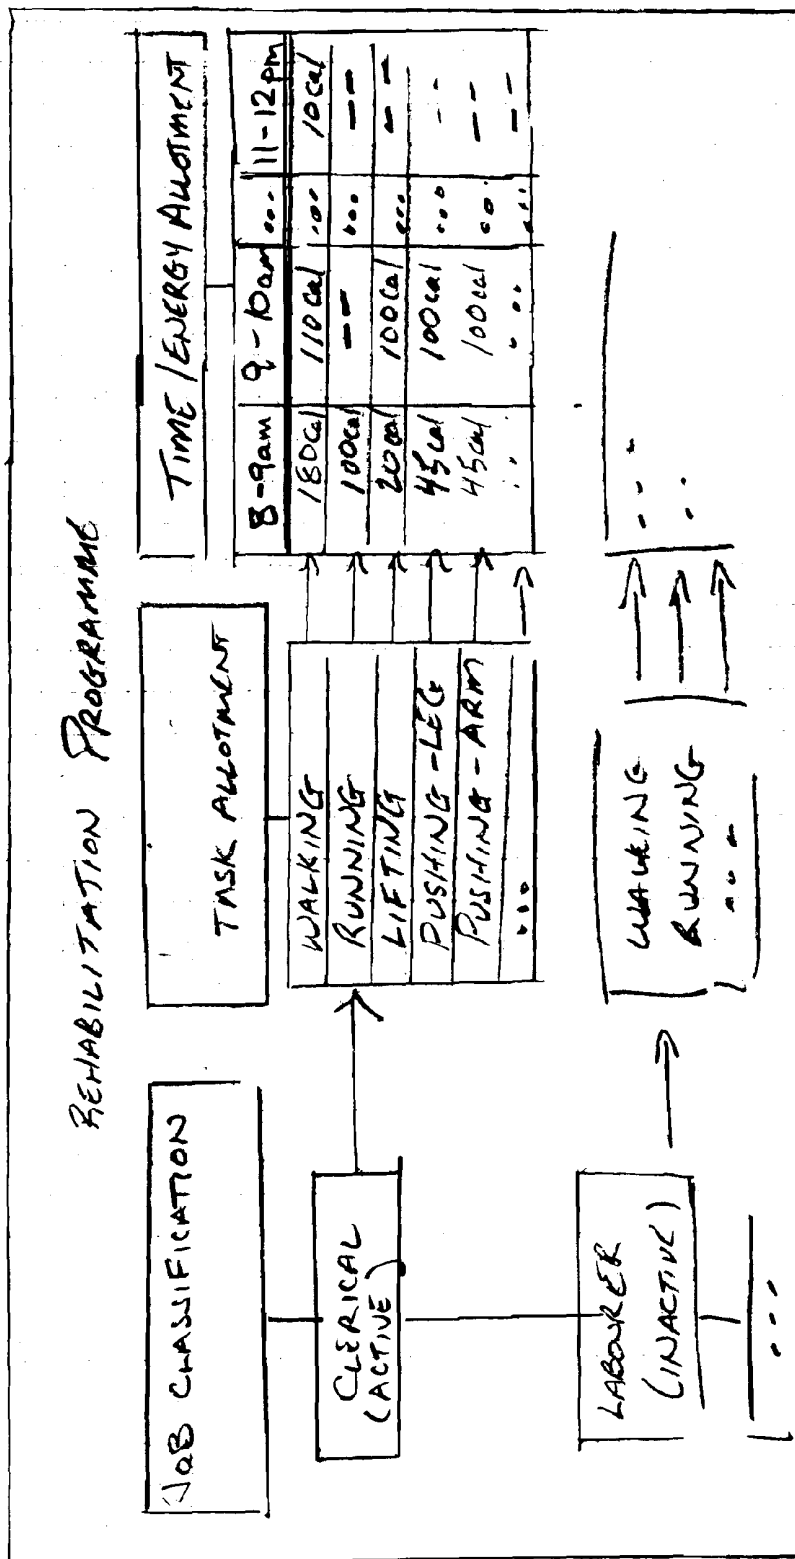


Fig. 6

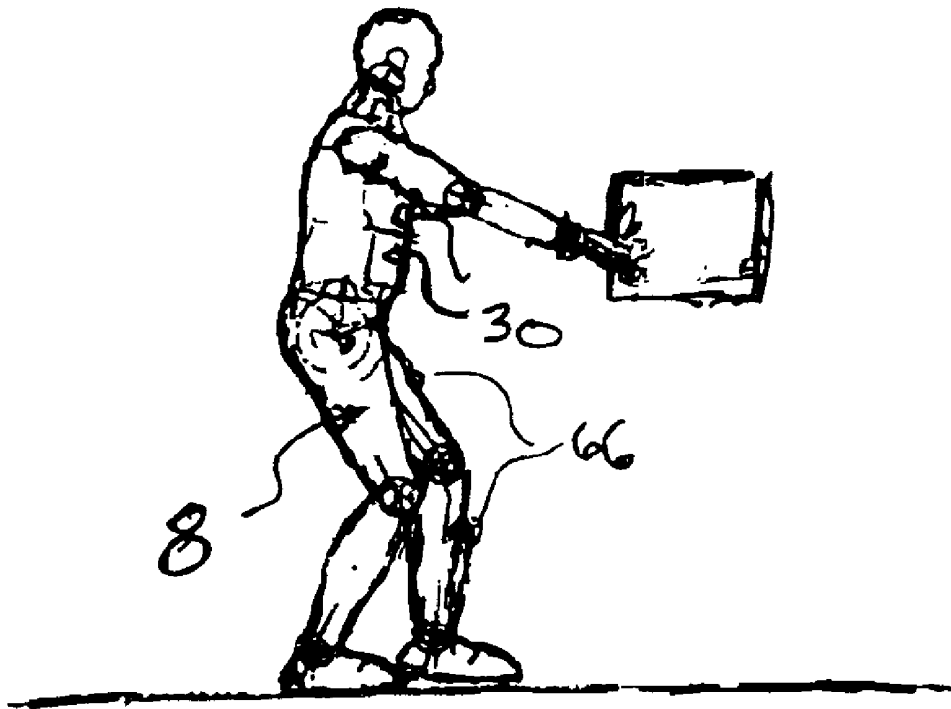

**ERGONOMIC/PHYSIOTHERAPY  
PROGRAMME MONITORING SYSTEM AND  
METHOD OF USING SAME**

SCOPE OF THE INVENTION

**[0001]** The present invention relates to an ergonomic based preventative and functional rehabilitative system which allows for the daily monitoring and coaching of a user's physical and functional activities, and more preferably a system which is operable to monitor and coach one or more individuals' dynamic performance and compliance with a preselected ergonomic preventative and therapeutic or rehabilitative physiotherapy regime which, for example, is implemented to provide a rehabilitative or wellness benefit to the particular user.

BACKGROUND OF THE INVENTION

**[0002]** Where an individual at risk of injury, or one that has sustained an injury and is receiving disability or sickness benefits from his or her employer or an insurance company, there is an incentive to not only an employee or injured party, but also the employer or benefit provider in ensuring compliance with general wellness or rehabilitative physiotherapy regimes. In particular, the adoption of not only healthy workplace activities, but daily activities which promote cardiovascular exercise and whole body wellness, will advantageously reduce employee risk of physical injury, absenteeism and increase overall productivity. In the case of injured or ill workers, the failure to comply with a prescribed rehabilitative physiotherapy schedule lengthens the recovery times, increasing both job-loss time and benefit costs to the employer and the insurer. Furthermore, employees that fail to participate in ergonomics and functional preventative programs prescribed, increase the risk of injury.

**[0003]** Most strokes and serious automobile or industrial accidents which result in severe injury to an individual typically necessitate that the individual undertake a lengthy and comprehensive rehabilitative exercise regime in order to regain pre-accident wellness and/or mobility. Such regimes often require the user to undertake lengthy, and frequently physically demanding rehabilitative exercises or physiotherapy delivered at a health clinic supplemented with physical activities delivered at a health club and or at home to rebuild damaged muscle and bone tissues. There is furthermore often a direct correlation to the individual's commitment and adherence to the physiotherapy regime and the speed and effectiveness of the recovery which can hinder best clinical practices. In a worst-case scenario, the failure to adhere to a necessary physiotherapy routine may result in muscle tissues atrophying, leading to irrevocable permanent disabilities in the patient.

**[0004]** In addition, as a result of limited resources, scheduled physiotherapy sessions typically involve the patient spending as little as between 30 and 60 minutes with a trained physiotherapist each day. The applicant has appreciated that if a physiotherapy regime can be established over an extended time and/or over an entire waking day, week or month, health delivery programming can be administered at a lower cost at a health and fitness facility and/or supplemented with home

based physical activity, and the patient's compliance thereto monitored and validated, enhanced patient recovery rates may be obtained.

SUMMARY OF THE INVENTION

**[0005]** The present invention provides for a system which includes a personal mobile health and fitness monitoring and coaching device or unit which stores target heart rate and/or caloric consumption data including other daily functional programming as prescribed by a healthcare provider, which correlates to a selected wellness or rehabilitative physiotherapy programme. More preferably, the monitoring and coaching unit is adapted to be worn by the user. The unit is operable to allow the user to periodically or continuously monitor and manage his or her physical state, based on physical state of activity based on knowledge and real-time analysis of heart rate, caloric expenditure, energy burn, functional and/or dynamic body movements, over a selected period, as well as compliance with a selected wellness or physiotherapeutic programme. The wearable monitoring unit is preferably operable to record and/or download data which is indicative of the user's physical activities, energy expenditure and/or physical performance over the selected period of time, as well as providing analysis and feedback based thereon. The collected data is most preferably compared or validated against preselected standards for the selected wellness or physiotherapy programme. Most preferably, the selected programme is chosen specifically having regard to a desired health or therapeutic benefit to the user.

**[0006]** Although not essential, in a preferred embodiment, the compared data may then be used to provide the user and/or the user's employer or other benefit provider with an indication as to whether or not compliance with the wellness or physiotherapy regime is being achieved; and whether best practices are applied.

**[0007]** Accordingly, one object of the invention is to provide a coaching, programming and monitoring system for ensuring compliance with a preselected wellness or physiotherapy programme which is selected to either maintain or improve the user's overall health.

**[0008]** Another object of the invention is to provide an outpatient physiotherapy coaching, programming and compliance monitoring system for a patient having an injury or malady in need of rehabilitative physiotherapy, and which allows for the remote monitoring an outpatient's compliance with a rehabilitative physiotherapy programme which is selected specifically to provide a therapeutic benefit to the patient, having regard to his or her injury or malady.

**[0009]** Another object of the invention is to provide an employer and/or patient benefit management system which is operable to maximize an individual's compliance with a selected ergonomic, wellness and/or physiotherapy programme selected to achieve a more healthy lifestyle, or to minimize ergonomic injury and the time for patient recovery, so as to reduce lost employee productivity and/or benefit costs.

**[0010]** In a preferred construction, a wearable monitoring unit (WMU) is provided for measuring the user's heart rate and dynamic energy and/or caloric expenditure over an extended period of time. Preferably the time period extends over the bulk of at least one waking day, and most preferably over at least one to four weeks. The wearable monitoring unit includes one or more of a heart rate monitor, a unit accelerometer, a global positioning system (GPS), and one or more

force micro-sensors. Optionally the WMU may also be provided with a digital audio and/or video Mp3 player and an audio and/or video output. The audio/video output is preferably operable to provide information and/or motivational prompts to the user in the event the heart rate, energy expenditure and/or caloric expenditure falls below or exceeds preselected target expenditures over a particular time segment of the selected time period. In a preferred construction, the WMU includes a display on a front panel which is used to provide a continuously updated visual indication of whether or not the user has achieved the preselected optimum caloric burn or energy expenditure for that particular time segment. In an alternate constructions, the WMU may be provided with wireless communication capability, allowing for its interface with other exercise devices, and/or used to upload and download heart rate, dynamic energy and/or caloric expenditure data and/or programming for group activities, such as staffed or unstaffed aerobic classes and the like.

**[0011]** In another possible construction, the WMU is provided with an internal calendar/clock, a processor and/or memory. The processor is operable to compare wellness or measured heart rate and energy expenditures for multiple time segments against target levels stored as the user-specific wellness or rehabilitative physiotherapy programme and which are tailored to provide the maximum therapeutic benefit to the user. Preferably the comparison of the target heart rate and energy expenditures against the user's actual measured heart rate, energy and/or caloric expenditure for the actual measured time is used to generate compliance output data to either the user and/or the employer.

**[0012]** In one embodiment, the user's personal biometric information such as age, sex, weight, height as well as the user's lifestyle information, such as job description, smoker status and physical fitness, and any injury or malady type is input directly or uploaded via the internet onto a host computer/portal or central processing unit (CPU). Target heart rate, energy and/or caloric consumption levels related to wellness or rehabilitation goals for a particular job type and injury are then selected having regard to fitness levels for an individual of comparable age, performing a similar job function. Alternately, employers or medical professionals may select unique and/or enhanced target fitness levels having regard to a desired wellness or rehabilitative programme chosen to maximize health benefits to the employee.

**[0013]** Accordingly, in one aspect the present invention resides in a physiotherapy compliance monitoring system for ensuring a user's compliance with a preselected physiotherapy programme over a selected time period, the system including, a data management system including, a reference database for storing datafiles providing preferred target heart rate and joule expenditure standards for a plurality of rehabilitation programmes, said rehabilitation programmes correlated to a biometric parameter, a lifestyle profile parameter and an injury or malady type to be rehabilitated, said biometric parameters comprising at least one of said user's age and weight, a client database for storing input client data indicative of each of said user's injury or malady, said user's biometric parameters, lifestyle profile information for said user, and benefit data correlated to a user's health benefit, a processing unit operable to output as said preselected physiotherapy programme a selected one of said rehabilitation programmes correlated to said input client data, a wearable monitoring device for communicating with said data management system and being operable to measure said user's

caloric and/or joule expenditure over the selected time period, the monitoring device including, an internal clock, memory for storing said preselected physiotherapy programme as downloaded user specific heart rate and joule expenditure standards over the selected time period, a heart rate monitoring sensor for monitoring and outputting heart rate data signals indicative of said user's heart rate over the selected time, at least one accelerometer for monitoring and outputting joule data signals indicative of at least one of movement by said user and physical force on at least part of said user's body over the selected time period, an internal processor for comparing said heart rate data signals and said joule data signals to said user specific heart rate and joule expenditure standards over said selected time period, and outputting a compliance output value which is dependent on the comparison, and wherein the data management system is operable to modify the user's health benefit data in response to the output value.

**[0014]** In another aspect, the present invention resides in an ergonomic monitoring system for monitoring and validating compliance with a preselected wellness or physiotherapy programme by a user, the system including, a data management system including, a reference database for storing a plurality of datafiles providing preferred target heart rate and caloric and/or joule expenditure standards for a plurality of wellness and rehabilitation programmes correlated to an injury, disability and a lifestyle profile, and a preselected biometric parameter, said biometric parameters comprising at least one of user age, and weight, a client database for storing client data indicative of biometric parameters of said user and at least one of a disability, injury and lifestyle profile of said user, a processing unit operable to output as said preselected wellness or physiotherapy programme a selected one of said wellness and rehabilitation programmes which correlates at least in part to at least one of said user's injury, disability and lifestyle profile, and said preselected biometric parameters, a wearable monitoring device for communicating with said data management system and being operable to measure said user's total daily caloric expenditure, the monitoring device including, an internal clock, memory for storing said selected wellness and rehabilitation physiotherapy programme as time dependent user specific heart rate and caloric and/or joule expenditure standards for a preselected time period, a heart rate monitoring sensor for monitoring and outputting heart rate data signals indicative of said user's heart rate, and an accelerometer for monitoring and outputting caloric and/or joule data signals indicative of at least one of movement by said user and physical force on at least part of said user's body, a processor for receiving said heart rate data signals and said caloric and/or joule data signals as input values and validating said input values to said user specific heart rate and caloric and/or joule expenditure standards over said preselected time period, and outputting a compliance output data indicative of any difference between said input values and said user specific heart rate and caloric and/or joule expenditure standards, a display for providing said user with a visual representation of said compliance output data.

**[0015]** In a further aspect, the present invention resides in a method of using a wearable monitoring device for validating a user's compliance with a physiotherapy programme selected to provide a therapeutic advantage to the user, the wearable monitoring device including a heart rate monitoring sensor for monitoring and outputting heart rate data signals indicative of said user's heart rate, and an accelerometer for monitoring and outputting caloric and/or joule data signals

indicative of at least one of movement by said user and physical force on at least part of said user's body, the method comprising, providing a reference database storing a plurality of datafiles for preferred target heart rate and caloric and/or joule expenditure standards for a plurality of rehabilitation programmes, said rehabilitation programmes correlated to a preselected biometric parameters and injury type, said biometric parameters comprising at least said user's age and weight, providing a client database storing input client data indicative of a user's injury, age, weight, and benefit data, downloading to the wearable monitoring device as said physiotherapy programme a selected one of said rehabilitation programme correlated to the user's input client data, validating as input values said heart rate data signals and said caloric and/or joule data signals to said user specific heart rate and caloric and/or joule expenditure over a preselected time period, and outputting a compliance output data indicative of any difference between said input values and said user specific heart rate and caloric and/or joule expenditure, and recording a change in said benefit data in response to the compliance output data.

#### BRIEF DESCRIPTION OF THE DRAWINGS

**[0016]** Reference may now be had to the following detailed description, taken together with the accompanying drawings in which:

**[0017]** FIG. 1 shows schematically a physiotherapy compliance monitoring system in accordance with a preferred embodiment of the invention;

**[0018]** FIG. 2 illustrates schematically the wearable monitoring unit (WMU) used in the monitoring system of FIG. 1;

**[0019]** FIG. 3 illustrates schematically the input client datafiles used in the data management system used in the monitoring system of FIG. 1;

**[0020]** FIG. 4 illustrates schematically the reference datafile architecture used in the data management system used in the monitoring system of FIG. 1;

**[0021]** FIG. 5 illustrates schematically a preferred rehabilitation programme architecture used in the reference datafiles of FIG. 4; and

**[0022]** FIG. 6 illustrates schematically the wearable monitoring unit (WMU) of FIG. 2 in use in the monitoring and validation of a preselected whole-day physiotherapy programme in accordance with a preferred embodiment.

#### DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

**[0023]** Reference is made to FIG. 1 which schematically illustrates an ergonomic monitoring system 10 which, as will be described, is most preferably used in the monitoring and validation of a user's compliance with a preselected rehabilitative physiotherapy programme. The system 10 provides an advantage over conventional fitness monitoring systems in that unlike existing systems which focus primarily on the user's health club activity over a 45 minute to 1 hour workout, the monitoring system 10 permits the monitoring and validation of compliance with a preselected physiotherapy regime over an entire waking day for periods of upto weeks or even months. The present system 10 may furthermore be used to provide not only periodic or real-time visual and aural behavioural modification guides and/or prompts to the user 8 (FIG. 6) throughout the entire day, but also allows for the adjustment of user rewards and/or benefits as added incentives to

adhere to the physiotherapy programme. In a preferred method of use, the selected physiotherapy programme is chosen having regard to the individual specific need of physical rehabilitation by the user 8. By way of non-limiting examples, these could include user injury or malady, such a stroke, back injury, heart attack, or to therapeutic exercise to the user's arms or legs after an automobile or industrial accident.

**[0024]** The system 10 includes a central processing unit 20, and at least one, and preferably a number of portable wearable monitoring units (WMU) 30 operable to be concurrently worn by different multiple users as part of the system operation. Each WMU 30 has a size and configuration selected to be easily carried and worn by the user 8 during his or her daily waking routine, without significantly encumbering daily activities.

**[0025]** The central processing unit 20 is most preferably housed as part of a mainframe computer by the user's employer, insurance company, HMO, or other benefit provider or administrator, and is electronically connected to an administrator payroll or benefit datafile 40. The benefit datafile 40 may be housed on the CPU 20 itself, or alternately stored at a remote location, and electronically linked to the CPU 20 electronically via a local or global computer network connection. Housed on the central processing unit 20 is an input client datafile 22, as well as a reference datafile 32 of stored rehabilitative programmes.

**[0026]** The input client datafile 22, shown best in FIG. 3, includes memory for storing input client data. The input client data contains information specific to the individual user 8. As shown best in FIG. 3, the client datafile 22 preferably includes user specific biometric parameters 24, user specific lifestyle parameters 26, as well as user specific benefit parameters 28. Biometric parameters 24 most preferably relate to the individual's physical status including the user's age, weight, height, as well as indications respecting any disability to be treated as part of the rehabilitative programme, or other impairments which for example, may result from pre-existing injuries. Disabilities to be treated may, by way of non-limiting example, include the partial paralysis of the user's legs or arms resulting from stroke or physical trauma, mobility loss resulting from spinal injuries, or muscular or skeletal damage caused by load straining or repetitive stress movements.

**[0027]** Lifestyle parameters 26 most preferably include particulars as to the user's profession, as well as indications of the user's leisure activities. Leisure activity particulars may include whether the individual is highly active and exercises regularly, smokes, any drug or prescription usage or whether the user has a sedentary lifestyle. Although not essential, most preferably, the lifestyle parameters are used to provide a weighting (i.e. active, inactive) of any pre-injury/trauma personal health or performance index (PI).

**[0028]** The individual benefit parameters 28 included in the input client datafile 22 may include without restriction, a dollar amount that the user 8 is entitled to receive in either disability or workers compensation payments under either an at-fault or no-fault insurance regime; particulars as to benefit duration where payments are time defined; as well as collateral non-monetary benefits, such as access credits for counselling, message therapy, hydrotherapy, prosthetic entitlement and the like.

**[0029]** As shown best in FIG. 4, the reference datafile 32 includes a series of individual downloadable rehabilitative physiotherapy programmes. Each downloadable rehabilitative programme is chosen to correlate to a preselected exer-

cise for a given injury type. The stored programmes furthermore stipulate preferred user specific target heart rates, and preferred caloric and energy or joule expenditure standards for the particular type of exercise, and are furthermore linked to the biometric and lifestyle parameters for the user **8** over a preselected period of time. Each of the physiotherapy programmes typically also include downloadable aural and/or video instructions as well as music, which provide to the user **8** with instructions to undertake physical activities ranging from stair climbing, to walking or lifting, or more intense cardiovascular workouts which are of a chosen duration and/or intensity. The physical activities are selected having regard to a particular time of day, and are chosen to achieve a pre-determined heart rate and caloric and/or energy burn. It is envisioned that the physiotherapy programmes stored in the datafile **32** each provide preferred heart rate and caloric and joule expenditure standards to be achieved throughout individual time segments, such as each half-hour, hour or two-hour period of an average waking day. The expenditure standards account for the user **8** not only undertaking a robust rehabilitative therapeutic exercise for a selected time segment (i.e. a particular hour), but also in undertaking day-to-day activities for a given time

[0030] As shown best in FIGS. **4** and **5**, in one possible architecture, the physiotherapy programmes are individually correlated to specific biometric and lifestyle parameters. Preferably, each programme is furthermore correlated to a specific muscle, limb or malady in need of rehabilitation. In this regard, each general class of job category is pre-allocated with an average daily caloric/joule expenditure for selected time segments (i.e. each hour/pre-breakfast etc.) throughout the day, and which are in turn correlated to the specific user disability/impairment in need of rehabilitation.

[0031] The physiotherapy programme provided by the CPU **20** is most preferably calibrated to increase or decrease desired heart rate and/or physical activity target expenditures in accordance with projected expenditures having regard to healthy individuals with equivalent lifestyle parameters, the specific time of day and anticipated activity. For example, during weekday business hours, the downloaded physiotherapy programme adjusts to reflect that the user's ability to provide elevated heart rates and physical activities may be limited by his/her employment duties. During these time segments, the target data operates to provide only moderate visual cues to the user **8** to adjust heart rate or activities tailored to both desired rehabilitative exercises and real world expectations.

[0032] FIG. **2** shows schematically the wearable monitoring unit **30**. The WMU **30** is operable to communicate with the central processing unit **20** to both download and store a user specific rehabilitative physiotherapy programme **45** thereto, as well as to upload the user's validated performance or compliance data. In a simplified mode of operation, data transfer between the CPU **20** and the WMU **30** is achieved by the uploading and downloading of datafiles via a PC (not shown) through a communicating network **35** such as a conventional home internet connection. Data downloading between the WMU **30** and the network **35** is achieved through a hardwired connection to the PC. FIG. **2** shows best each WMU **30** as having an internal USB connector port **44**. The connection port **44** is used for electronically coupling the WMU **30** with the PC docking station (not shown) so as to facilitate the electronic downloading and uploading of programmes and data. Alternatively, the WMU **30** may also

incorporate a wireless radio module operable to communicate to a base housed station, such as a wireless router on a PC network. Wireless module communications may be activated through a hall-effect sensor which is operable to detect a magnet housed in the docking station at a physiotherapist or home PC. Alternatively, the PC could be omitted entirely, with either wireless or direct wired communication occurring between the CPU **20** and WMU **30**, or by hardwiring, or direct plug-in.

[0033] As indicated, each WMU **30** has an overall size and weight selected so as to be comfortably worn by the user **8** as a fully portable device. The WMU **30** is therefore preferably provided as a small multi-function mobile fitness monitoring and tracking device. The WMU **30** is adapted to be worn comfortably by the user **8** throughout the entire waking day, as he or she performs not only a specific physiotherapy or rehabilitative workout, but also most daily tasks. The WMU **30** is operated by way of a rechargeable battery **46** and preferably is approximately the size of a small cell phone or pager. The rechargeable battery **46** is chargeable through the USB connection port **44** in a conventional manner, as for example during data downloading and uploading from the PC, or a wall charging device. A sleep mode and wake-up function are preferably used to conserve power and provide an expected battery life in excess of seven days.

[0034] In addition to the battery **44**, the WMU **30** is provided internally with an internal calendar/clock processor **48**, a performance sensor array **50** and internal portable data storage/memory **52**. The sensor array **50** includes a number of different types of sensors used to measure different physical attributes of the user **8** over the course of the preselected time segments, such as each hour, throughout the waking day. As will be described, the sensor array **50** is electronically linked to both the clock/processor **48** and the data storage/memory **52** to allow for the comparison and validation of measured user data, such as heart rate, caloric burn and/or energy burn, against the preselected target values provided by the selected physiotherapy programme **45** download from the CPU **20**.

[0035] Preferably the sensor array **50** includes a heart rate sensor **60**, an internal unit accelerometer **62**, a global positioning sensor (GPS **64**), and where the WMU **30** is used in the validation of a physiotherapy programme **45** for providing rehabilitative therapy for one or more of the user's **8** limbs, a number of force micro-sensors **66a**, **66b**, **66c**, **66d**. The heart rate sensor **60** includes a remote contact sensor pad **70** which is adapted for placement against a pulse point on the user's **8** skin in the monitoring and recording of heart rate data signals which reflect the user's heart rate during WMU **30** operation. Most preferably the WMU **30** incorporates as sensor **60**, a means of wirelessly receiving heart rate pulse data from a wireless chest strap heart rate sensor device. Heart rate data is monitored and stored periodically (i.e. every 5 minutes) in the memory **52**. More preferably heart rate variability is also calculated and stored as a value. As will be described, the heart rate sensor **60** is used to monitor whether or not a prescribed target heart rate has been achieved for a given time segment through the entire day. This measured heart rate is then compared against the target heart rate for the corresponding time segment in the preselected physiotherapy programme **45**.

[0036] The internal accelerometer **64** is preferably of a 3-axis operational design which is used to measure whole body motion when the WMU **30** is worn on the user **8**. By providing a belt mount **47**, the orientation of the accelerom-

eter **62** with relation to the user's **8** body is advantageously fixed so that the output from each axis is directionally known. In one preferred operational mode, the x-axis is down (giving a +1 g signal when stationary). The y-axis is selected forward and the z-axis is inwardly towards the body (i.e. twisting). In general, the accelerometer **62** signals are continuously analysed together with signals from the GPS sensor **64** and the type of activity determined, with both the activity type and activity dynamic energy stored in memory **52**. The data can then be analyzed in real time, and in this manner, the types and extent of activity detected are:

- [0037] Walking and distance; (Note: Position the device)
- [0038] Running and distance; (as a body motion and analysis)
- [0039] Jumping and distance; (device that can be used to determine steps as one of its functions)
- [0040] Sitting/Standing
- [0041] Lying Down
- [0042] Rolling
- [0043] Passive transportation distance (i.e. car or other transportation journey).
- [0044] Dynamic energy and activity

The accelerometer **62** is thus operable to monitor and output joule data signals which provide an indication of the movement of the user **8**. Additionally, the microprocessor **48** provides an analysis algorithm used to filter the accelerometer **62** data and determine the validity of a step. Step count and time is then recorded and saved as time-stamped measured user performance data in the memory **52** periodically (i.e. every 5 minutes). In addition the bounce height of the x-axis will be analysed to gain a measure of distance travelled during each step.

[0045] The force micro-sensors **66a**, **66b**, **66c**, **66d** are provided in a preferred embodiment in the form of miniature remote accelerometer sensors such as micro-miniature piezoelectric accelerometers. In the case of leg or arm injuries, the sensors **66** adapted for direct securement to the limbs of the user **8** in the manner shown in FIG. 6. The micro-sensors **66** preferably provide joule data signals to the processor **48** which are indicative of the movement of the specific limb in need of physiotherapy, and/or the physical force or exertion performed thereon throughout the day. Sensors **66** are most preferably wirelessly linked to the WMU **30**, although hard-wired sensors may also be used.

[0046] The clock/micro-processor **48** allows the data collected by the heart rate sensor **60**, accelerometer **62**, GPS **64** and force micro-sensors **66** to be time-stamped. The micro-processor **48** preferably also controls all WMU **30** operational features, and includes self-testing and diagnostics functions. This information is uploadable to the CPU **20** so that functional errors with the WMU **30** can be indicated to the user **8**. The microprocessor **48** manages the WMU **30** data storage/memory **52**.

[0047] In a simplified construction a master output display **80** and operational mode control buttons **82**, allow the user to select a specific operating mode for the WMU **30**, and either upload to the CPU **20** data relating to the validation of the user's heart rate, caloric and/or energy expenditures and/or download physiotherapy programmes for playback. The device memory **52** is used to receive and store the preselected physiotherapy programme **45** which is downloaded by the CPU **20** and which is tailored specifically having regard to the input client data, having regard to the specific user injury or malady which is in need of rehabilitation. Optionally, the

WMU **30** may operate a number of operational modes including: as an interactive device for a specified limited timed physiotherapy regime; as a daily monitor used to record the user's activity heart rate and caloric expenditure; and as a rehabilitation coach as part of an outpatient whole-day physiotherapy regime.

[0048] In the embodiment shown in FIG. 2, the WMU display **80** consists of an LED array which is divided into multiple sections. Although not essential, each section is preferably operable to provide feedback to the user **8** through a colour indication display. In a simplified design, the sections of the display **80** incorporate LEDs which are operable to emit the colours red, yellow or green as visual prompts to the user **8**, to provide a visual indication of whether or not the user's **8** heart rate, caloric and/or joule expenditure and overall physical activity or total energy (joule) expenditure meets or exceeds the preselected target standards for the preselected physiotherapy programme **45** at each particular time segment or time of day. The display **80** provides a visual colour indicator of the comparison of the measured state of the user's heart rate, caloric and energy consumption, activity rate, and health as against pre-defined programme goals for both the particular day, and particular time segment as determined by the clock/microprocessor **48**. The colour indicator feedback is activated by the output switch **82**, with the goal for the user to achieve green for each section.

[0049] The internal processor **48** is operable to compare both the heart data signals, as well as the caloric and joule expenditure data signals which are received from the accelerometer sensor **62**, GPS **64** and the force micro-sensors **66**. The processor **48** then compares the measured user heart rate and joule data with the heart rate and joule expenditure standards which are contained in the preselected physiotherapy programme **45** stored in the memory **52** and provide validated compliance output data **88**. Although not essential, most preferably the comparison between the measured data and the stored standards is performed on a real-time basis by the processor **48** throughout the entire day, as the user **8** wears the device. Concurrently, the display **80** provides the user **8** with a visual indication of his/her compliance with the heart rate and expenditure standards. This advantageously allows the user **8** to implement minor, or of necessary major adjustment to his/her physical activities either in real-time or following each time segment, to ensure continued compliance with the preselected rehabilitation programme **45**. In one possible mode, WMU **30** may produce a data table used to control the feedback light. This data is uploadable from the WMU **30** to the CPU **20** during the time it is connected to a PC. For the user **8**, the data table is based on their information in a unique user account at the portal. Data may, for example, include the following Table 1.

TABLE 1

Date and Time
Degree of Movement
Movement Type
Heart Rate
HRV
Dynamic Energy
Activity Type

[0050] The total PI expected could be calculated using Basal Metabolic Rate and Activity level (or similar), with or without other values based on the specific physiotherapy

goals of the user **8** depending on his or her specific disability and/or malady. This value is then allocated to a specific pre-selected daily periods, as for example, is shown in Table 2.

TABLE 2

Time Segment	Time	General PI to be Achieved	Physiotherapy Targets	Special or Additional Activity Targets
1	12 am-6 am	200	100	0
2	6 am-8 am	400	0	0
3	1 pm-3 pm	300	100	200
4	5 pm-9 am	600	0	0

The present system preferably also allows the user **8** at the end of each segment to "top up" by performing additional therapeutic exercises so as to reach the total target caloric and/or joule burn and/or heart rate levels for a particular day. With the indication that the target heart and/or overall caloric and/or energy expenditure levels for a time segment has not yet been achieved, the user **8** may download from the CPU **30** a supplemental physiotherapy routine consisting of music, video and/or instructions. This downloaded routine is selected to enable the user **8** to complete the required level of necessary physiotherapy workout used to achieve the target fitness level and target heart level, and having regard to the actual measured values for the particular day. Following at the end of each day, the user may then upload from the WMU **30** data representative of actual physiotherapy activities and heart rate data.

[0051] In a preferred mode, the user's physical activity is measured throughout the day and tracked by the WMU **30** using the sensor array **50**. The collected data is converted to the universal Performance Index (PI) scale based on the user's **8** pre-input physical characteristics. Feedback is customized to activity and energy expenditures throughout a day based on the user's **8** type of injury or malady and correlated physiotherapy programme which has been pre-selected. The portability and light weight of the WMU **30** allows it to be worn by the user **8** throughout his/her waking day to collect data relating to the user's overall heart rate, and energy and/or caloric expenditure. The data collected is uploaded (via PC) to the CPU **20** as a compliance output data **88** to provide feedback to the user's employer and/or physiotherapist. The uploaded compliance output data **88** provides an indication of whether the user's **8** caloric and/or joules expended as a result of the user's physical activity equals or exceeds the target level.

[0052] Although not essential, most preferably the compliance output value **88** is used to reset the categories and/or frequency or available user benefits stored within a benefits databank **90**. The benefits databank **90** is then immediately or periodically downloaded from the central processing unit **20** to the benefit administrator datafile **40**. The compliance output data **88** thus not only provides the employer or benefits administrator with an indication as to whether or not the user **8** is meeting target heart rate, caloric and/joule data expenditures in compliance with the selected physiotherapy programme, but also may be used to automatically adjust use, benefits and incentives. To provide an added incentive to the user **8** to maintain compliance with the physiotherapy programme, depending on the compliance output data **88**, the benefits administrator datafile **40** may be adjusted to alter the user's benefits. In one scenario where the user **8** complies with the physiotherapy programme **45**, the benefits databank

**90** is operated to increase benefit payments over the early part of the rehabilitation schedule. This may advantageously provide positive reinforcement resulting in the user's earlier recovery, and an earlier return to work. Conversely, a user **8** could be penalized, receiving reduced benefits if the compliance output data **88** indicates the user **8** is not maintaining an acceptable level of conformity to the rehabilitative physiotherapy programme **45**. Such reduced benefits could include, by way of non-limiting example, either a restriction in non-monetary benefits, or a reduction in the value and/or frequency of momentary benefits paid to the user **8**.

[0053] Although the detailed description describes the system **10** as being used in the monitoring of the user's **8** compliance with a rehabilitative physiotherapy regime, the invention is not so limited. In an alternate application, the system could be used as a general ergonomic monitoring system by employers. It is envisioned that the present system **10** may advantageously be used to allow the monitoring of employee compliance with one or more preselected wellness and/or lifestyle programmes. Such wellness programmes may be selected, again having regard to essentially the same biometric and lifestyle parameters of the employee.

[0054] It is to be appreciated that employee wellness and ergonomic programmes are selected to provide an overall health benefit to the employee, with a view to reducing employee absenteeism and increasing overall health. In such an application, the employer may also provide incentives for employee participants, such as increased pay, time off or access to health facilities or other non-monetary benefits. The system **10** of such an application would operate in substantially the same manner as that previously described with a view to providing reduced health benefit costs to the employer.

[0055] Although the preferred embodiment describes the WMU **30** as having a clock/processor **48** and memory **52** operably to store and validate measured user performance data **52** with the downloaded standards, the invention is not so limited. In a more economical construction, data storage and validation processing may be achieved by way of a user's home personal computer or PC. A user's PC may also be provided to facilitate date and firmware downloads between the CPU **20** and WMU **30**. User performance information from the WMU **30** may also be stored directly on a PC, allowing the user to monitor any changes in performance data and obtain feedback therefrom. In a more preferred construction, a firmware version is saved which is unique to the device ID for the WMU **30** at the CPU **20**. Any firmware updates will be posted on the CPU **20** and downloaded as appropriate.

[0056] Optionally, the physiotherapy database may be connected to the central CPU **20** to automatically upload information with respect to the user's in hospital physiotherapy regime.

[0057] Although not essential, in a preferred construction a digital audio video player **80** is preferably also provided within the WMU **30** which allows music, video and/or audio instructions to be downloaded from the CPU **20** for playback to the user **8**.

[0058] Although the detailed descriptions and illustrates various preferred embodiments, the invention is not so limited. Many modifications and variations will occur to persons skilled in the art. For a definition of the invention, reference may now be had to the appended claims.

1. A physiotherapy compliance monitoring system for ensuring a user's compliance with a preselected physiotherapy program over a selected time period, the system including,

- a data management system including,
- a reference database for storing datafiles providing preferred target heart rate and joule expenditure standards for a plurality of rehabilitation programs, said rehabilitation programs correlated to a biometric parameter, a lifestyle profile parameter and an injury or malady type to be rehabilitated, said biometric parameters comprising at least one of said user's age and weight,
- a client database for storing input client data indicative of each of said user's injury or malady, said user's biometric parameters, lifestyle profile information for said user, and benefit data correlated to a user's health benefit,
- a processing unit operable to output as said preselected physiotherapy program a selected one of said rehabilitation programs correlated to said input client data,
- a wearable monitoring device for communicating with said data management system and being operable to measure at least one of said user's caloric and joule expenditure over the selected time period, the monitoring device including,
- an internal clock,
- memory for storing said preselected physiotherapy program as downloaded user specific heart rate and joule expenditure standards over the selected time period,
- a heart rate monitoring sensor for monitoring and outputting heart rate data signals indicative of said user's heart rate over the selected time,
- at least one accelerometer for monitoring and outputting joule data signals indicative of at least one of movement by said user and physical force on at least part of said user's body over the selected time period,
- an internal processor for comparing said heart rate data signals and said joule data signals to said user specific heart rate and joule expenditure standards over said selected time period, and outputting a compliance output value which is dependent on the comparison, and
- wherein the data management system is operable to modify the user's health benefit data in response to the output value.

2. The monitoring system of claim 1 further wherein the wearable monitoring device includes a display for providing a visual representation of said compliance output value and any modification or potential modification to the user's health benefit data to the user.

3. The monitoring system of claim 2, wherein said biometric parameters comprise each of said user's age and weight, and said lifestyle profile information comprises at least one of a categorization of said user's job, weighting factors respecting the user's pre-injury health and indication of any pre-existing user disabilities.

4. The monitoring system of claim 2, wherein said lifestyle profile parameters include data selected from preselected classes of job categories, and preselected classes of leisure activity categories.

5. The monitoring system of claim 2, wherein said wearable monitoring device is a portable monitoring device operable to provide said visual representation of said output value data substantially in real time.

6. The monitoring system as claimed in claim 2, wherein the selected time period comprises at least eight hours.

7. The monitoring system as claimed in claim 2, wherein the selected time period comprises the average waking times over at least a one week interval.

8. Use of the monitoring system as claimed in claim 1, comprising, inputting said client data into said client database, downloading said preselected physiotherapy program to said wearable device in response to said input client data, and with said user wearing said wearable device during said selected time period, actuating said internal processor to compare said heart rate signals and said joule data signals to said user specific heart rate and joule expenditure standards to generate said compliance output value, and modifying the user's health benefit data in response to the compliance output value.

9. Use of the monitoring system as claimed in claim 8, wherein said wearable monitoring device is operated to provide a visual indication to said user in response to the compliance output value which is indicative of any modification to the user's health benefit data.

10. An ergonomic monitoring system for monitoring and validating compliance with a preselected wellness or physiotherapy program by a user, the system including,

- a data management system including,
- a reference database for storing a plurality of datafiles providing preferred target heart rate and at least one of caloric and joule expenditure standards for a plurality of wellness and rehabilitation programs correlated to an injury, disability and a lifestyle profile, and a preselected biometric parameter, said biometric parameters comprising at least one of user age, and weight,
- a client database for storing client data indicative of biometric parameters of said user and at least one of a disability, injury and lifestyle profile of said user,
- a processing unit operable to output as said preselected wellness or physiotherapy program a selected one of said wellness and rehabilitation programs which correlates at least in part to at least one of said user's injury, disability and lifestyle profile, and said preselected biometric parameters,
- a wearable monitoring device for communicating with said data management system and being operable to measure said user's total daily caloric expenditure, the monitoring device including,
- an internal clock,
- memory for storing said selected wellness and rehabilitation physiotherapy program as time dependent user specific heart rate and caloric and/or joule expenditure standards for a preselected time period,
- a heart rate monitoring sensor for monitoring and outputting heart rate data signals indicative of said user's heart rate, and
- an accelerometer for monitoring and outputting at least one of caloric and joule data signals indicative of at least one of movement by said user and physical force on at least part of said user's body,
- a processor for receiving said heart rate data signals and said caloric and/or joule data signals as input values and validating said input values to said user specific heart rate and at least one of caloric and joule expenditure standards over said preselected time period, and outputting a compliance output data indicative of any difference between said input values and said user specific heart rate and at least one of caloric and joule expenditure standards,

a display for providing said user with a visual representation of said compliance output data.

**11.** The monitoring system of claim **10**, wherein said lifestyle profile includes data selected from preselected job categories, and preselected leisure activity categories.

**12.** The monitoring system of claim **10**, wherein said wearable monitoring device is a portable monitoring device operable to provide said visual representation of said output value data substantially in real time.

**13.** The monitoring system of claim **10**, wherein the preselected time period comprises an average waking day.

**14.** The monitoring system of claim **10**, wherein said selected wellness and physiotherapy program comprises a rehabilitative therapy program, said at least one of caloric and joule expenditure standards comprise joule expenditure standards for a selected injured body part, and wherein said at least part of said user's body is a part in need of rehabilitative physiotherapy.

**15.** The monitoring system of claim **14**, wherein said client data further includes benefit data correlated to a health or monetary benefit to said user, the data management system operable to receive the compliance output data and modify the benefit data for the user in response to compliance output data.

**16.** Use of the system as claimed in claim **15**, comprising, inputting said client data into said client database, downloading said selected program to said wearable device in response to said input data, and with said user wearing said wearable device during said selected time period, actuating said internal processor to compare said heart rate signals and said joule data signals to said user specific heart rate and joule expenditure standard to output said compliance output data, and modifying the user's health benefit data in response to the compliance output data.

**17.** Use of the system as claimed in claim **15**, wherein said wearable monitoring device is operated to provide a visual indication to said user in response to an actual or potential change to the user's benefit data.

**18.** A method of using a wearable monitoring device for validating a user's compliance with a physiotherapy program selected to provide a therapeutic advantage to the user,

the wearable monitoring device including a heart rate monitoring sensor for monitoring and outputting heart rate data signals indicative of said user's heart rate, and an accelerometer for monitoring and outputting at least one of caloric and joule data signals indicative of at least one of movement by said user and physical force on at least part of said user's body,

the method comprising,

providing a reference database storing a plurality of data-files for preferred target heart rate and caloric and/or joule expenditure standards for a plurality of rehabilitation programs, said rehabilitation programs correlated to

a preselected biometric parameters and injury type, said biometric parameters comprising at least said user's age and weight,

providing a client database storing input client data indicative of a user's injury, age, weight, and benefit data, downloading to the wearable monitoring device as said physiotherapy program a selected one of said rehabilitation program correlated to the user's input client data, validating as input values said heart rate data signals and said at least one of caloric and joule data signals to said user specific heart rate and at least one of caloric and joule expenditure over a preselected time period, and outputting a compliance output data indicative of any difference between said input values and said user specific heart rate and said at least one of caloric and joule expenditure, and

recording a change in said benefit data in response to the compliance output data.

**19.** The method of claim **18** further comprising displaying to said user a visual representation of said compliance output data which is indicative of any change or potential change in said benefit data.

**20.** The method of claim **19**, wherein the visual representation is displayed to said user substantially in at least a bi-hourly frequency substantially throughout the user's waking day.

**21.** The monitoring system of claims **1**, wherein said rehabilitation program is correlated to an injury to at least one of said user's arm and leg, said wearable device further including a plurality of force micro-sensors which are attachable to an arm and/or leg in need of rehabilitation, said micro-sensor operable to provide data signals to said internal processor representative of energy expenditure by said at least one of arm and leg.

**22.** The monitoring system as claimed in claim **10**, wherein said wellness and rehabilitative physiotherapy programs include a plurality of rehabilitative physiotherapy programs each for providing a therapeutic benefit in remediation to an injury to said user's limbs, said wearable device comprises at least one force micro-processor which are attachable to an injured limb for providing data signals to said processor representative of said user's energy expended by movement of said injured limb.

**23.** The method of claim **18**, wherein the wearable monitoring device further includes at least one force micro-sensor which is attachable to a limb of said user, and processor circuitry for receiving force signals from said micro-sensor which are representative of measured movements and/or forces applied to said limb, said method further comprising, attaching said at least one force micro-sensor to a limb of said user in need of wellness or physiotherapeutic exercise, and validating said force signals by said processor as part of said input values.

\* \* \* \* \*

专利名称(译)	人体工程学/物理治疗程序监控系统及其使用方法		
公开(公告)号	<a href="#">US20120029936A1</a>	公开(公告)日	2012-02-02
申请号	US13/255800	申请日	2009-03-11
[标]申请(专利权)人(译)	农REED		
申请(专利权)人(译)	农REED		
当前申请(专利权)人(译)	农REED		
[标]发明人	HANOUN REED		
发明人	HANOUN, REED		
IPC分类号	G06Q50/00 A61B5/00 G06Q50/22		
CPC分类号	A61B5/0205 A61B5/103 G06Q50/22 G06F19/3418 G06F19/3481 A61B5/4866 A61B5/7405 G16H20/30 G16H40/67		
其他公开文献	US9468382		
外部链接	<a href="#">Espacenet</a>	<a href="#">USPTO</a>	

摘要(译)

用户的个人生物信息，例如年龄，性别，体重，身高以及使用者的生活方式信息，例如工作描述，吸烟者状态和身体健康，以及任何伤害或疾病类型被上传到主计算机上。然后根据可比年龄的个体的健康水平选择与特定工作类型和伤害的健康或康复目标相关的目标心率，能量和/或热量消耗水平，然后将执行类似的工作功能下载到可穿戴设备监测单位。可穿戴监测单元 (WMU) 用于在一到四周内测量用户的心率和动态能量和/或热量消耗。可穿戴监测单元包括心率监测器，单元加速计，全球定位系统 (GPS)，一个或多个力 - 微传感器，以及音频和/或视频输出。音频/视频输出可操作以在事件中向用户提供信息和/或激励提示在所选时间段的特定时间段内，心率，能量消耗和/或热量消耗低于或超过预选的目标支出。显示器提供持续更新的视觉指示，表明该使用是否已达到该特定时间段的预选最佳卡路里燃烧或能量消耗。WMU具有内部日历/时钟，处理器和/或存储器处理器将多个时间段的健康或测量的心率和能量消耗与作为用户特定的健康或康复程序存储的目标水平进行比较，以提供对用户的最大治疗益处。然后，该比较用于向用户和/或雇主生成合规性输出数据。

