



(19) **United States**

(12) **Patent Application Publication**
Elghazzawi

(10) **Pub. No.: US 2002/0007114 A1**

(43) **Pub. Date: Jan. 17, 2002**

(54) **METHOD AND APPARATUS FOR
DETECTING A PHYSIOLOGICAL
PARAMETER**

Publication Classification

(51) **Int. Cl.⁷** A61B 5/00
(52) **U.S. Cl.** 600/323

(76) **Inventor: Ziad Elghazzawi, Newton, MA (US)**

(57) **ABSTRACT**

Correspondence Address:
Siemens Corporation
Intellectual Property Department
186 Wood Avenue South
Iselin, NJ 08830 (US)


A system for detecting a physiological parameter from a physiological signal, includes a source of the physiological signal. Circuitry, coupled to the signal source, detects spectral peaks in the physiological signal. Calculating circuitry, coupled to the spectral peak detecting circuitry, calculates a parameter value corresponding to each detected spectral peak. Weighting circuitry, coupled to the calculating circuitry and the spectral peak detecting circuit, assigns a weight to each peak according to a feature of a signal and the parameter value corresponding to that peak. Circuitry, coupled to the weighting circuitry, selects the peak according to a predetermined criterion. Output circuitry, coupled to the selecting circuitry and the calculating circuitry, then generates the parameter value corresponding to the selected peak.

(21) **Appl. No.: 09/777,546**

(22) **Filed: Feb. 6, 2001**

Related U.S. Application Data

(63) **Non-provisional of provisional application No. 60/181,482, filed on Feb. 10, 2000.**

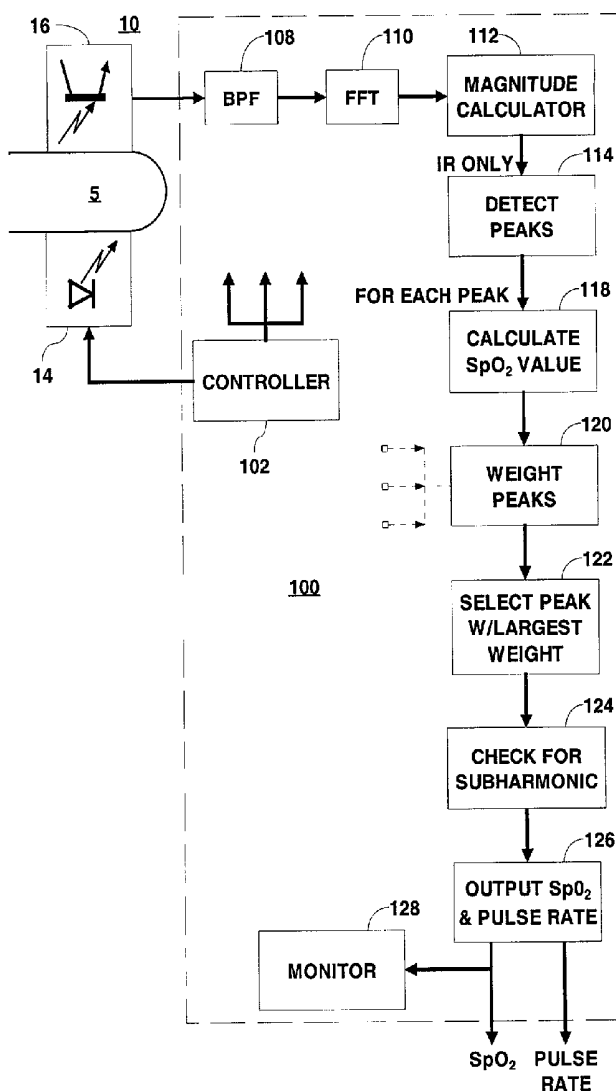

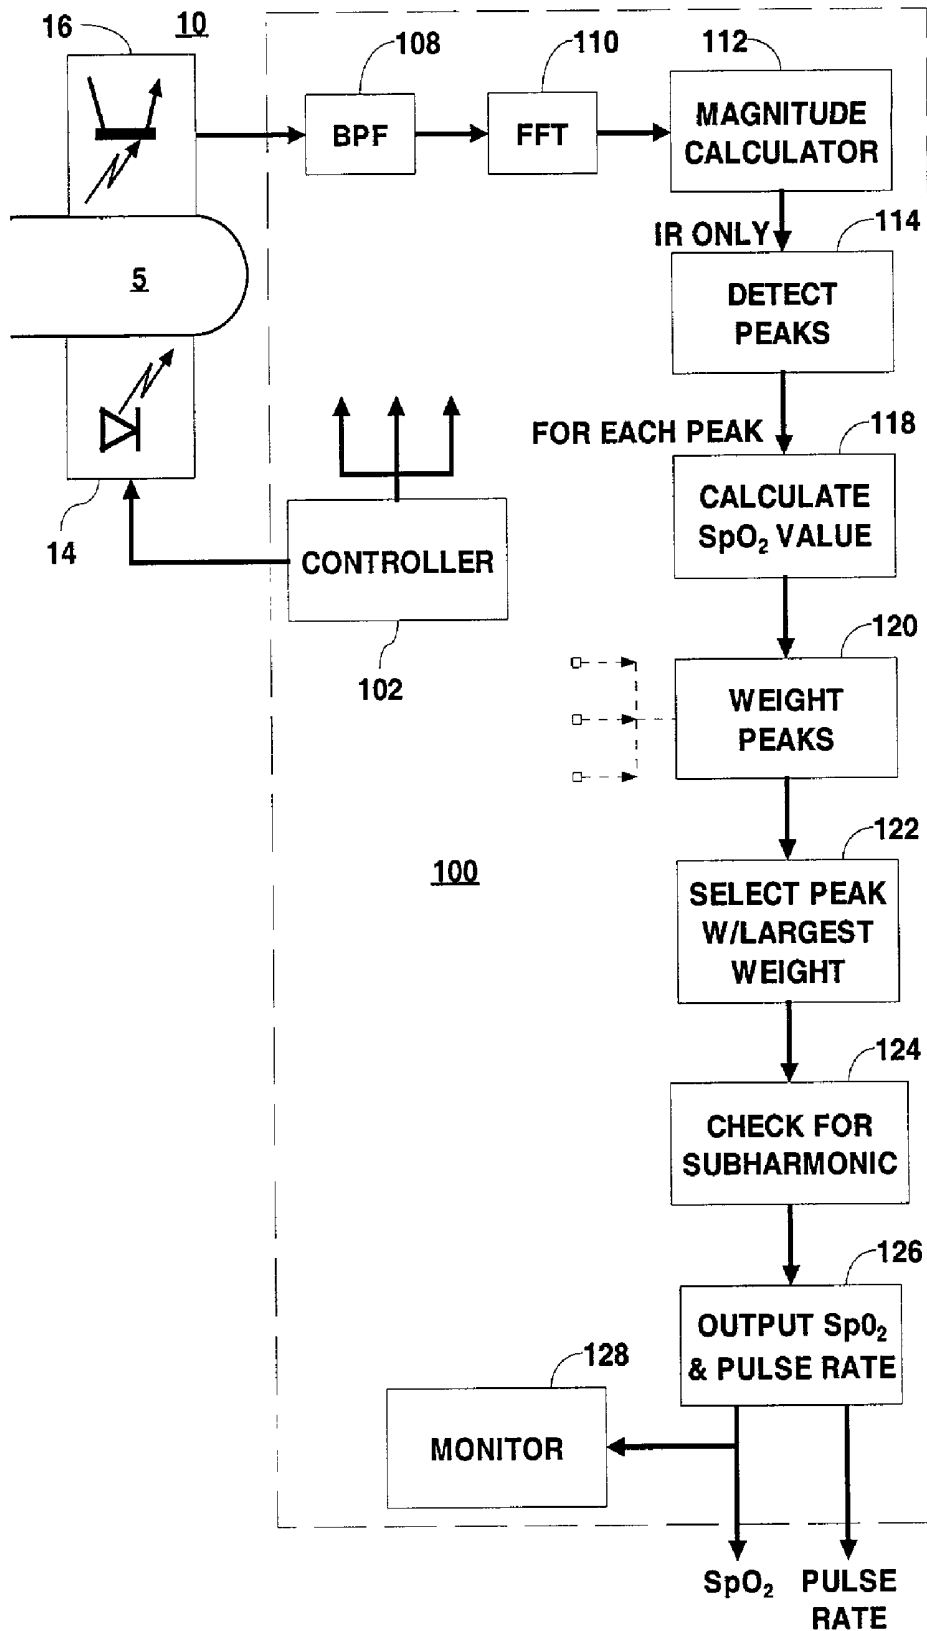


Fig. 1

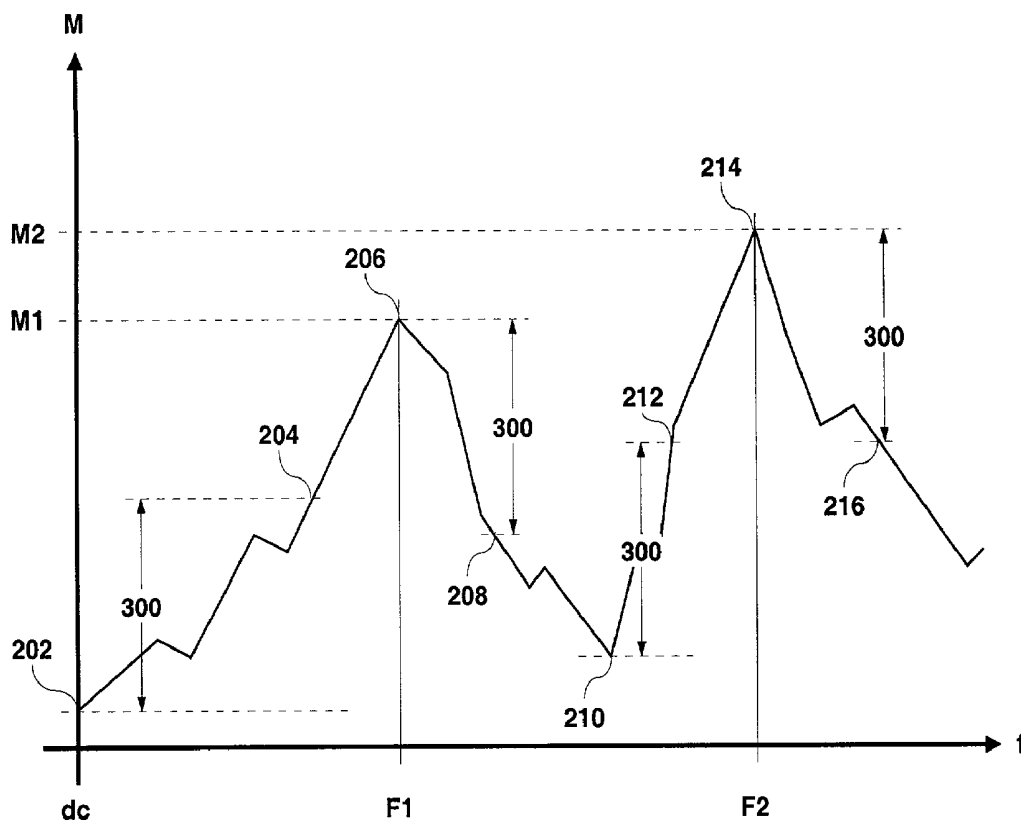


Fig. 2

METHOD AND APPARATUS FOR DETECTING A PHYSIOLOGICAL PARAMETER

CROSS REFERENCE TO RELATED APPLICATIONS

[0001] This application expressly claims the benefit of earlier filing date and right of priority from the following co-pending patent application, which is assigned to the assignee of the present invention and have the same inventor: U.S. Provisional Application Serial No. 60/181,482 (Attorney Docket No. 00 P 7459 US), filed on Feb. 10, 2000, entitled "METHOD AND APPARATUS FOR DETECTING A PHYSIOLOGICAL PARAMETER." The above cited patent application is expressly incorporated in its entirety by reference.

FIELD OF THE INVENTION

[0002] The present invention relates to detecting a desired physiological parameter from physiological electrical signals, and more particularly to removing artifacts from the physiological signal in order to more accurately detect the desired parameter.

BACKGROUND OF THE INVENTION

[0003] It is often required to detect a physiological parameter from electrical physiological signals. For example, parameters related to the functioning of the heart are detected using known electrocardiogram systems; parameters related to the functioning of the brain are detected using known electroencephalogram systems, and the parameters of blood oxygen concentration and pulse rate are detected using known oximeter systems. In the remainder of this application, pulse oximeter systems will be described in more detail, though one skilled in the art will understand that the systems, circuits, and methods in the description may be modified to apply to other systems which detect physiological parameters from electrical physiological signals.

[0004] Known oximeter systems use light signals to detect the blood oxygen concentration. Light of two different wavelengths is made incident on blood perfused flesh, and either transmitted or reflected light is detected, converted to an electrical physiological signal, and that electrical signal processed to detect the physiological parameter of blood oxygen concentration, all in a known manner. It is well known that many factors introduce noise into the electrical signal: for example patient movement, changes in ambient light level, and, to a lesser extent, EMI from power wiring and/or other operating electrical equipment in the vicinity of the oximeter system.

[0005] In order to enhance accuracy, much work has been done to detect accurately the electrical oximetry signals in the noise inherent in such systems. Some prior art systems transform the time domain electrical physiological signal (including noise) into the frequency domain, and perform further processing in the frequency domain. Such systems use a Fourier transform to transform the electrical physiological signal into the frequency domain. More specifically, a discrete Fourier transform of some form, preferably a fast Fourier transform (FFT) is used. The frequency domain signals are then analyzed to separate the physiological signal from the noise and detect the desired parameter.

[0006] U.S. Pat. No. 6,122,535, issued Sep. 19, 2000 to Kaestle et al., illustrates a system in which FFTs are calculated of both the IR and red light representative signals generated by the oxymetric sensor. From the FFTs, a magnitude transform is calculated for both the red and IR signals. The magnitude transform for one of the signals is plotted on the x axis against the magnitude transform for the other of the two signals on the y axis. The resulting x-y plot includes what are termed needles extending radially away from the origin. The magnitude and angle of these needles, and other parameters related to them, are compiled in a table. Each entry in the table is scored according to various criteria. The entry with the highest score is selected as representing the actual pulse rate of the patient. Data from the FFT related to this entry is then processed to generate pulse rate and blood oxygen concentration (SpO₂) parameters.

[0007] U.S. Pat. No. 6,094,592, issued Jul. 25, 2000 to Yorkey et al. illustrates another system in which FFTs are calculated on both the IR and red light representative signals generated by the oxymetric sensor. An SpO₂ parameter is calculated for each and every point in the FFT. A histogram is then constructed of all the SpO₂ parameters previously calculated. One of the SpO₂ parameters is selected from the histogram information according to a set of rules. This SpO₂ value is displayed as the blood oxygen concentration parameter.

[0008] U.S. Pat. No. 5,924,980, issued Jul. 20, 1999 to Coetzee, illustrates yet another system in which FFTs are calculated on both the IR and red light representative signals generated by the oxymetric sensor. In this patent, "good" and "bad" portions of the light representative signals generated by the oxymetric sensor are identified by comparing the light representative signals to an "ideal" waveform. Outliers are identified and deleted by correlating the red and IR light representative signals. As a result of the correlation the adverse effect of the noise signals is minimized, and the SpO₂ value is calculated in a more accurate manner.

[0009] All of these prior art systems require a substantial amount of processing, and consequently a substantial amount of power. A system which requires less processing and consumes less power is desirable.

BRIEF SUMMARY OF THE INVENTION

[0010] In accordance with principles of the present invention, a system for detecting a physiological parameter from a physiological signal, includes a source of the physiological signal. Circuitry, coupled to the signal source, detects spectral peaks in the physiological signal. Calculating circuitry, coupled to the spectral peak detecting circuitry, calculates a parameter value corresponding to each detected spectral peak. Weighting circuitry, coupled to the calculating circuitry and the spectral peak detecting circuit, assigns a weight to each peak according to a feature of a signal and the parameter value corresponding to that peak. Circuitry, coupled to the weighting circuitry, selects the peak according to a predetermined criterion. Output circuitry, coupled to the selecting circuitry and the calculating circuitry, then generates the parameter value corresponding to the selected peak.

BRIEF DESCRIPTION OF THE DRAWING

[0011] In the drawing::

[0012] **FIG. 1** is a block diagram illustrating a blood oxygen concentration (SpO₂) detection system according to principles of the present invention;

[0013] **FIG. 2** is a diagram illustrating the method of detecting a spectral peak useful in the system illustrated in **FIG. 1**.

DETAILED DESCRIPTION OF THE INVENTION

[0014] **FIG. 1** is a block diagram representing the blood oxygen concentration (SpO₂) detection system according to principles of the present invention. In **FIG. 1** an oxymetric sensor **10**, represented by the combination of a light source **14** and a light sensor **16**, is connected to a control circuit **100**. In **FIG. 1** an output terminal of a controller **102** is coupled to an input terminal of a light source **14**. Additional output terminals of controller **102** are coupled to respective control input terminals (not shown) of other circuitry within the control circuit **100**. One skilled in the art will understand what control signals are required, how to generate them, and how to interconnect them with the circuitry within the control circuit **100** requiring them.

[0015] The light source **14** is configured to emit light incident on blood perfused flesh **5**, such as a finger or ear lobe, as is known. The light transmitted through, or reflected from, the flesh **5** is received by a light sensor **16**. An output terminal of light sensor **16** is coupled to a serial connection of a band pass filter (BPF) **108**, an FFT calculating circuit **110**, a magnitude calculator **112**, a peak detector **114**, an SpO₂ value calculator **118**, a peak weighting circuit **120**, peak selection circuitry **122**, subharmonic checking circuitry **124**, and circuitry **126** which produces output signals representing the SpO₂ and pulse rate parameters. A first output terminal of the output circuit **126**, generates the SpO₂ parameter value and is further coupled with input terminal of a monitor **128**. A second output terminal of the output circuit **126** produces a pulse rate representative signal.

[0016] In operation, the light source **14** includes at least two light emitting diodes: one emitting light at the red wavelength, the other emitting light at the IR wavelength, in response to the control signal from the controller **102**. The controller **102** supplies signals to the light source **14** conditioning the light source **14** to produce alternating light signals at the respective wavelengths. Alternately, the controller **102** may condition the LEDs to emit light during mutually exclusive time periods including a time period when no light is emitted by either LED, all in a known manner. The light sensor **16** receives light signals either transmitted through or reflected from the flesh **5**. The signals are processed in the appropriate way to produce separate red and IR electrical signals representing the received signals from the corresponding LED in the light source **14**, in a known manner. This processing can include noise filtering, dark (no LED light) period processing, gain control, and possibly conversion to digital samples, all in a known manner. In the remainder the diagram, the red and IR electrical signals are represented by single signal lines, unless specifically described otherwise. One skilled in the art will also understand that some of this processing may be

performed within the control circuit **100**, though such circuitry is not shown in order to simplify the figure.

[0017] Because the electrical physiological signals of interest are known to exist only in the frequency band from 0.5 Hz to 5 Hz, the band pass filter **108** filters the received light representative signals and passes only those frequencies within this pass band. The FFT calculating circuit **110** performs a transform of the filtered red and IR signals into the frequency domain. The red and IR FFTs are converted to magnitude transforms by the magnitude calculator **112** in the standard manner. Circuit **114** detects peaks in the magnitude FFT of the IR signal only. Any of the plurality of known methods for detecting peaks may be used on the IR magnitude FFT to detect the peaks.

[0018] **FIG. 2** is a diagram illustrating the method of detecting a spectral peak useful in the system illustrated in **FIG. 1**. In **FIG. 2**, the IR magnitude FFT is traversed from the dc point upward in frequency. A peak is detected whenever the magnitude of the IR FFT rises from a magnitude of the starting point by at least a predetermined amount (e.g. 300) before the magnitude of the IR FFT drops by the predetermined amount below the peak. The detected peak has associated with it a frequency and a magnitude. The frequency of the detected peak is the frequency location in the FFT at which the maximum magnitude is detected, and the maximum magnitude at that frequency location is the peak magnitude.

[0019] Referring more specifically to **FIG. 2**, an exemplary IR magnitude FFT is illustrated. One skilled in the art will understand that such an FFT consists of an ordered set of magnitude values, each value representing the magnitude of the IR signal at a corresponding frequency. However, in order to more clearly describe the method for detecting peak values, this set of values is represented by a line graph representing the magnitude spectrum. Starting at the dc point **202**, the magnitude of the IR FFT is monitored to detect when it exceeds the dc value by a predetermined value, which is the illustrated embodiment is 300. In **FIG. 2** this occurs at point **204**. From point **204**, the maximum value of the magnitude of the IR FFT is continually updated, and the magnitude of the IR FFT is monitored to detect when it decreases from the maximum value by the predetermined amount (e.g. 300). More specifically, a maximum is detected at point **206**. This maximum has a value of M1 and a frequency of F1. This peak is selected when the magnitude of the IR FFT drops below the maximum magnitude M1 by the predetermined amount (300), which occurs at point **208**. From point **208**, the minimum value of the magnitude of the IR FFT is continually updated, and the magnitude of the IR FFT is monitored to detect when it increases from the minimum value by the predetermined amount (300). More specifically, a minimum is detected at point **210**. This minimum is selected when the magnitude of the IR FFT exceeds the minimum magnitude at point **210** by the predetermined amount (300), which occurs at point **212**. The magnitude and frequency of the minimum point are not relevant.

[0020] From point **210** the process described above repeats to detect further peaks. Consequently, as described above, from point **212** the maximum value of the magnitude of the IR FFT is continually updated, and the magnitude of the IR FFT is monitored to detect when it decreases from the

maximum value by the predetermined amount (300). A second maximum is detected at point **214**. This maximum has a value of **M2** and a frequency of **F2**. This peak is selected when the magnitude of the IR FFT drops below the maximum magnitude **M2** by the predetermined amount (300), which occurs at point **216**. All such peaks are detected in this manner. These peaks are further processed as described below. Alternatively, a predetermined maximum number of peaks may be further processed (e.g. 10 to 30). In this case, the 10 to 30 peaks with the largest magnitudes are further processed, as described below, while the remainder are discarded.

[**0021**] The calculating circuitry **118** calculates in SpO₂ value for the frequency of each peak identified by the peak detecting circuitry **114**. For each such peak, the calculation is based on the ratio R, given in equation (1) below, in which ACred represents the magnitude of the red FFT at the location of the peak detected in the IR FFT; DCred represents the magnitude of the red FFT at the zero frequency (DC) location; ACir represents the magnitude of the IR FFT at the location of the peak, and DCir represents the magnitude of the IR FFT at the zero frequency (DC) location. The ratio R is then used as an input parameter to an experimentally determined look up table to determine the SpO₂ value corresponding to that ratio.

$$R = \frac{\log \frac{ACred + DCred}{DCred}}{\log \frac{ACir + DCir}{DCir}} \quad (1)$$

[**0022**] Each peak detected by the peak detector **114** is then weighted by weighting circuit **120**. The weighting in general is based on the SpO₂ value calculated in the calculating circuitry **118**, and other signal features. These signal features may be related to the physiological signals themselves, or to some other signal as illustrated in phantom **FIG. 1** by signal lines coupled to a second input terminal of the weighting circuit **120**. These signal features could, for example, be a value, slope or integral or some other function of one or more signals, including the physiological signals, in either the time or frequency domain.

[**0023**] In the illustrated embodiment, the weight W is calculated, as illustrated in equation (2) below, by taking the SpO₂ value calculated by the calculating circuit **118**, squaring it, and multiplying by the magnitude of the corresponding IR FFT peak (ACir) to produce the weight W corresponding to that peak.

$$W = (\text{SpO}_2)^2 \cdot \text{ACir} \quad (2)$$

[**0024**] The selection circuitry **122** selects a peak according to a predetermined criterion. In the illustrated embodiment, the peak having the largest weight W is selected as the peak representing the actual pulse rate.

[**0025**] However, if the peak selected the selecting circuitry **122** is between her 0.75 Hz and 1.4 Hz, then it is possible that the frequency of this peak represents not the pulse rate, but instead the first harmonic of the pulse rate and that the spectral peak representing the frequency of the fundamental is masked by noise. Thus, one further check may optionally be performed before the final selection of a peak representing the pulse rate.

[**0026**] Checking circuitry **124** checks the frequency of the peak selected by the selecting circuit **122** to determine if it is between 0.75 Hz and 1.4 Hz. If it is, then the location in the magnitude IR FFT at ½ of the frequency represented by the selected peak is checked to determine if it has been identified as a peak. If that location is not a peak, then the peak initially selected by the selection circuitry **122** is selected as the peak, and the pulse rate and SpO₂ values corresponding to that peak are produced at the output terminals of the output circuit **126** and displayed on the monitor **128**.

[**0027**] On the other hand, if the location of the IR magnitude FFT at ½ of the frequency of the peak initially selected by selecting circuit **122** is determined to also be a peak, then the magnitude of that peak (lower peak) is compared to the magnitude of the peak initially selected by the selecting circuit **122** (upper peak). If the magnitude of the lower peak is greater than twice the magnitude of the upper peak, then the SpO₂ values calculated for the lower and upper peaks are compared. If the SpO₂ value (expressed as a percentage) for the lower peak is more than two percent greater than the SpO₂ value for the upper peak, then the lower peak is assumed to be the fundamental, and the frequency of the lower peak is assumed to represent the pulse rate. In this case the pulse rate and the SpO₂ values corresponding to the lower peak are produced at the output terminals of the output circuit **126** and displayed on the monitor **128**. Otherwise, the upper peak is assumed to be the fundamental, and the pulse rate and the SpO₂ values corresponding to the upper peak are produced at the output terminals of the output circuit **126** and displayed on the monitor **128**.

[**0028**] The system illustrated in **FIG. 1** is described above as consisting of separate interconnected hardware elements, and such a system could be implemented in that manner. However, one skilled in the art will understand that the control circuit **100** could also be implemented as a computer system, operating under control of a control program, in which signals received from the light sensor **16** are converted into samples in digital form by an analog to digital converter in a known manner. The digital samples are received by the computer **100**, and all filtering, transforms, and other calculations and comparisons are carried out by the computer under control of a program stored in a memory (not shown) all in a known manner.

[**0029**] By detecting spectral peaks in the electrical red and IR light signals, the amount of calculations which must be performed, relative to the prior art methods, described above, is decreased, and consequently the power required to detect the pulse rate and SpO₂ level is decreased as well.

What is claimed is:

1. A system for detecting a physiological parameter from a physiological signal, comprising:

a source of the physiological signal;

circuitry, coupled to the signal source, for detecting spectral peaks in the physiological signal;

calculating circuitry, coupled to the spectral peak detecting circuitry, for calculating a parameter value corresponding to each detected spectral peak;

weighting circuitry, coupled to the calculating circuitry, for weighting each peak according to a signal feature and the parameter value corresponding to that peak;

circuitry, coupled to the weighting circuitry, for selecting a peak according to a predetermined criterion; and

output circuitry, coupled to the selecting circuitry and the calculating circuitry, for generating the parameter value corresponding to the selected peak.

2. The system of claim 1 further comprising a bandpass filter coupled between the signal source and the spectral peak detecting circuit.

3. The system of claim 1 wherein the spectral peak detecting circuitry comprises:

a transform circuit, coupled to the signal source, for transforming the physiological signal to the frequency domain; and

circuitry for detecting spectral peaks in the frequency domain transform of the physiological signal.

4. The system of claim 3 wherein the transform circuit comprises a Fourier transform circuit.

5. The system of claim 4 wherein:

the Fourier transform circuit comprises an FFT circuit; and

the spectral peak detecting circuitry comprises circuitry for calculating the magnitude of the FFT transform of the physiological signal, and a circuit for detecting peaks in the magnitude FFT transform.

6. The system of claim 1 wherein the weighting circuitry weights each peak according to respective signal features of one or more signals and the parameter value corresponding to that peak.

7. The system of claim 1 wherein the weighting circuitry weights each peak according to the magnitude of the detected spectral peak and the parameter value corresponding to that peak.

8. The system of claim 1 wherein the selecting circuitry selects the peak having the largest weight.

9. A system for detecting blood oxygen concentration (SpO₂) from a physiological signal, comprising:

a source of the physiological signal;

circuitry, coupled to the signal source, for detecting spectral peaks in the physiological signal;

calculating circuitry, coupled to the spectral peak detecting circuitry, for calculating the SpO₂ value corresponding to each detected spectral peak;

weighting circuitry, coupled to the calculating circuitry and the spectral peak detecting circuit, for weighting each peak according to the magnitude of the detected spectral peak and the SpO₂ value corresponding to that peak;

circuitry, coupled to the weighting circuitry, for selecting the peak having the largest weight; and

output circuitry, coupled to the selecting circuitry and the calculating circuitry, for generating the parameter value corresponding to the selected peak.

10. The system of claim 9 further comprising a bandpass filter coupled between the signal source and the detecting circuitry.

11. The system of claim 10 wherein the passband of the bandpass filter is between around 0.5 Hz and around 5 Hz.

12. The system of claim 9 wherein the signal source comprises a source of a red signal representing received red light and a source of an IR signal representing received IR light.

13. The system of claim 12 wherein:

the spectral peak detecting circuitry comprises a Fourier transform circuit which generates transformed red and IR signals corresponding to the red and IR signals, respectively; and

the detecting circuitry detects peaks in the transformed IR signal.

14. The system of claim 13 wherein:

the Fourier transform circuit comprises an FFT circuit; and

the peak detecting circuit further comprises a circuit for generating the magnitude transform of the IR signal, and detecting peaks in the magnitude transform of the IR signal.

15. The system of claim 13 wherein the calculating circuitry comprises:

circuitry for calculating a ratio R value according to the equation:

$$R = \frac{\log \frac{ACred + DCred}{DCred}}{\log \frac{ACir + DCir}{DCir}} \quad (1)$$

wherein ACred represents the magnitude of the transformed red signal at each peak, DCred represents the DC magnitude of transformed red signal, ACir represents the magnitude of the transformed IR signal at each peak, and DCir represents the DC magnitude of the IR signal.; and

a lookup table for looking up the SpO₂ value according to the ratio R.

16. The system of claim 13 wherein the weighting circuitry comprises circuitry for calculating the weight W according to the equation:

$$W = (\text{SpO}_2)^2 \cdot ACir$$

wherein ACir represents the magnitude of the transformed IR signal at each peak.

17. The system of claim 9 wherein each detected peak is further associated with a frequency, and the system further comprises:

circuitry for determining if the frequency associated with the selected peak is within a predetermined frequency range and if the frequency associated with the selected peak is within the predetermined frequency range, then:

checking if the transformed signal at one-half the frequency associated with the selected peak is also a peak, and if the signal at one-half the frequency associated with the selected peak is also a peak, then:

comparing the respective magnitudes associated with the selected peak and the peak at one-half the frequency associated with the selected peak, and

if the magnitude of the peak at one-half the frequency associated with the selected peak is greater than the magnitude of the selected peak by a predetermined factor, and the SpO₂ value associated with the peak at one-half the frequency associated with the selected peak is greater than the SpO₂ value associated with the selected peak by a predetermined amount, then selecting the peak at one-half the frequency of the selected peak.

18. The system of claim 17 wherein the predetermined factor is substantially two.

19. The system of claim 17 wherein the SpO₂ value is expressed at a percentage; and the predetermined amount is substantially 2%.

20. The system of claim 17 wherein the predetermined frequency range is from around 0.5 Hz to around 1.4 Hz.

21. The system of claim 9 comprised in a computer system, operating under control of a control program.

22. A method for detecting a physiological parameter from a physiological signal, comprising the steps of:

receiving the physiological signal representing the parameter;

detecting spectral peaks in the physiological signal;

calculating the physiological parameter corresponding to each peak;

weighting each peak according to a signal feature and the physiological parameter corresponding to that peak;

selecting a peak according to a predetermined criterion; and

generating the physiological parameter corresponding to the selected peak.

23. The method of claim 22 further comprising, before peak detecting step, the step of limiting the bandwidth of the physiological signal.

24. The method of claim 22 wherein the peak detecting step comprises the steps of:

calculating the Fourier transform of the physiological signal; and

detecting peaks in the transform of the physiological signal.

25. The method of claim 24 wherein the peak detecting step further comprises the step of calculating the magnitude Fourier transform of the physiological signal.

26. The method of claim 22 wherein the weighting step comprises the step of weighting each peak according to respective features of one or more signals and the physiological parameter corresponding to the peak.

27. The method of claim 26 wherein the weighting step comprises the step of weighting each peak according to the magnitude of the peak and the physiological parameter corresponding to the peak.

28. The method of claim 22 wherein the selecting step comprises the step of selecting the peak having the largest weight.

29. A method for detecting blood oxygen concentration (SpO₂) from a physiological signal, comprising the steps of:

receiving the physiological signal representing the SpO₂ value;

detecting spectral peaks in the physiological signal;

calculating the SpO₂ value corresponding to each peak;

weighting each peak according to magnitude of the peak and the SpO₂ value corresponding to that peak;

selecting the peak with the highest weight; and

generating the SpO₂ value corresponding to the selected peak.

30. The method of claim 29 further comprising, before the detecting step, the step of limiting the bandwidth of the physiological signal.

31. The method of claim 30 wherein the limiting step comprises the step of limiting the bandwidth to from around 0.5 Hz to around 5 Hz.

32. The method of claim 29 wherein:

the receiving step comprises the step of receiving a red signal representing received red light and an IR signal representing received IR light;

the transforming step comprises the step of transforming the red and IR signals to transformed red and IR signals, respectively; and

the detecting step comprises the step of detecting peaks in the transformed IR signal.

33. The method of claim 32 wherein the transforming step further comprises the step of transforming the red and IR signals to magnitude transformed red and IR signals, respectively.

34. The method of claim 32 wherein the transformed physiological signal has a DC magnitude, and the calculating step comprises the steps of:

calculating a ratio R value according to the equation:

$$R = \frac{\log \frac{ACred + DCred}{DCred}}{\log \frac{ACir + DCir}{DCir}} \quad (1)$$

wherein ACred represents the magnitude of the transformed red signal at each peak, DCred represents the DC magnitude of transformed red signal, ACir represents the magnitude of the transformed IR signal at each peak, and DCir represents the DC magnitude of the IR signal; and

looking up the SpO₂ value from a lookup table according to the ratio R.

35. The method of claim 32 wherein the weighting step comprises the step of calculating the weight W according to the equation:

$$W = (\text{SpO}_2)^2 \cdot ACir$$

wherein ACir represents the magnitude of the transformed IR signal at each peak.

36. The method of claim 29 wherein each detected peak is further associated with a frequency, and the method further comprises, after the selecting step, the steps of:

determining if the frequency associated with the selected peak is within a predetermined frequency range and if the frequency associated with the selected peak is within the predetermined frequency range, then performing the steps of:

checking if the transformed signal at one-half the frequency associated with the selected peak is also a peak and if the signal at one-half the frequency associated with the selected peak is also a peak, then performing the steps of:

comparing the respective magnitudes associated with the selected peak and the peak at one-half the frequency associated with the selected peak; and

if the magnitude of the peak at one-half the frequency associated with the selected peak is greater than a predetermined factor times the magnitude

of the selected peak, and the SpO₂ value associated with the peak at one-half the frequency associated with the selected peak is greater than the SpO₂ value associated with the selected peak by a predetermined amount, then selecting the peak at one-half the frequency of the selected peak.

37. The method of claim 36 wherein the predetermined factor is substantially two.

38. The method of claim 36 wherein the SpO₂ value is expressed at a percentage; and the predetermined amount is substantially 2%.

39. The method of claim 36 wherein the predetermined frequency range is from about 0.5 Hz to about 1.4 Hz.

* * * * *

专利名称(译)	用于检测生理参数的方法和设备		
公开(公告)号	US20020007114A1	公开(公告)日	2002-01-17
申请号	US09/777546	申请日	2001-02-06
[标]申请(专利权)人(译)	ELGHAZZAWI ZIAD		
申请(专利权)人(译)	ELGHAZZAWI ZIAD		
当前申请(专利权)人(译)	ELGHAZZAWI ZIAD		
[标]发明人	ELGHAZZAWI ZIAD		
发明人	ELGHAZZAWI, ZIAD		
IPC分类号	A61B5/0452 A61B5/00 A61B5/0476 A61B5/145 A61B5/1455		
CPC分类号	A61B5/1455 A61B5/14551 A61B5/7203 A61B5/7257		
优先权	60/181482 2000-02-10 US		
其他公开文献	US6574491		
外部链接	Espacenet USPTO		

摘要(译)

一种用于从生理信号中检测生理参数的系统，包括生理信号的来源。耦合到信号源的电路检测生理信号中的光谱峰值。耦合到光谱峰值检测电路的计算电路计算对应于每个检测到的光谱峰值的参数值。加权电路耦合到计算电路和频谱峰值检测电路，根据信号的特征和对应于该峰值的参数值为每个峰值分配权重。耦合到加权电路的电路根据预定标准选择峰值。然后，耦合到选择电路和计算电路的输出电路产生对应于所选峰值的参数值。

