



US 20080200783A9

(19) **United States**
(12) **Patent Application Publication**
Blank et al.

(10) **Pub. No.: US 2008/0200783 A9**
(48) **Pub. Date: Aug. 21, 2008**
CORRECTED PUBLICATION

(54) **METHOD AND APPARATUS FOR CONTROL OF SKIN PERFUSION FOR INDIRECT GLUCOSE MEASUREMENT**

Continuation-in-part of application No. 10/349,573, filed on Jan. 22, 2003, now Pat. No. 7,039,446.

(76) Inventors: **Thomas B. Blank**, Chandler, AZ (US); **Timothy L. Ruchti**, Gilbert, AZ (US); **Mutua Mattu**, Gilbert, AZ (US); **Marcy Makarewicz**, Chandler, AZ (US); **Stephen L. Monfre**, Gilbert, AZ (US); **Alexander D. Lorenz**, Chandler, AZ (US)

(60) Provisional application No. 60/363,345, filed on Mar. 8, 2002. Provisional application No. 60/235,369, filed on Sep. 26, 2000.

Publication Classification

(51) **Int. Cl.**
A61B 5/00 (2006.01)
(52) **U.S. Cl.** **600/322; 600/306**

Correspondence Address:
GLENN PATENT GROUP
3475 EDISON WAY, SUITE L
MENLO PARK, CA 94025 (US)

(57) **ABSTRACT**

A method and apparatus for noninvasive glucose measurement measures glucose indirectly from the natural response of tissue to variations in analyte concentration. The indirect measurement method utilizes factors affected by or correlated with the concentration of glucose, such as refractive index, electrolyte distribution or tissue scattering. Measurement reliability is greatly improved by stabilizing optical properties of the tissue at the measurement site, thus blood perfusion rates at the sample site are regulated. Perfusion is monitored and stabilized by spectroscopically measuring a control parameter, such as skin temperature, that directly affects perfusion. The control parameter is maintained in a range about a set point, thus stabilizing perfusion. Skin temperature is controlled using a variety of means, including the use of active heating and cooling elements, passive devices, such as thermal wraps, and through the use of a heated coupling medium having favorable heat transfer properties.

(21) Appl. No.: **10/384,049**

(22) Filed: **Mar. 7, 2003**

Prior Publication Data


(15) Correction of US 2004/0039271 A1 Feb. 26, 2004

See (60) Related U.S. Application Data.

(65) US 2004/0039271 A1 Feb. 26, 2004

Related U.S. Application Data

(63) Continuation-in-part of application No. 09/955,531, filed on Sep. 17, 2001, now Pat. No. 6,640,117.

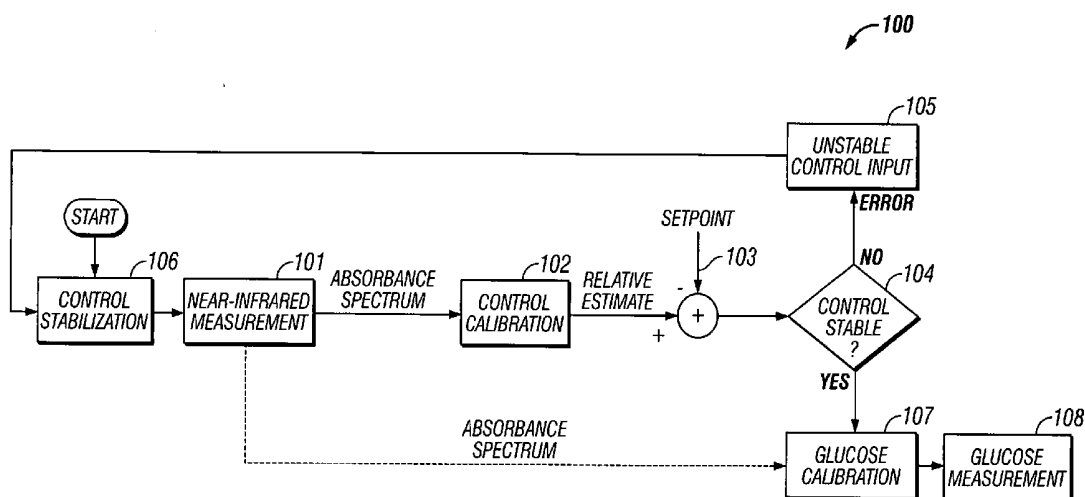

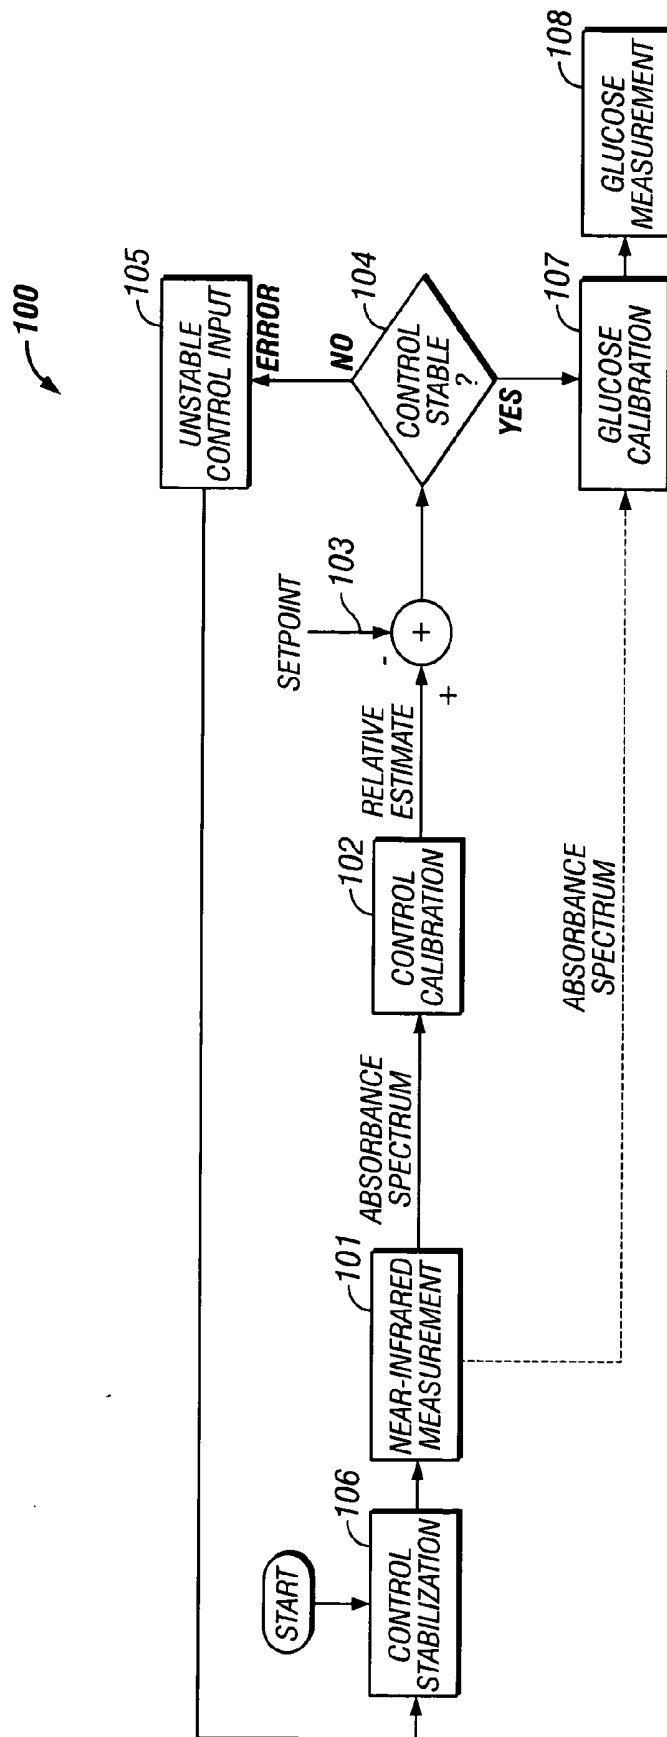


FIG. 1

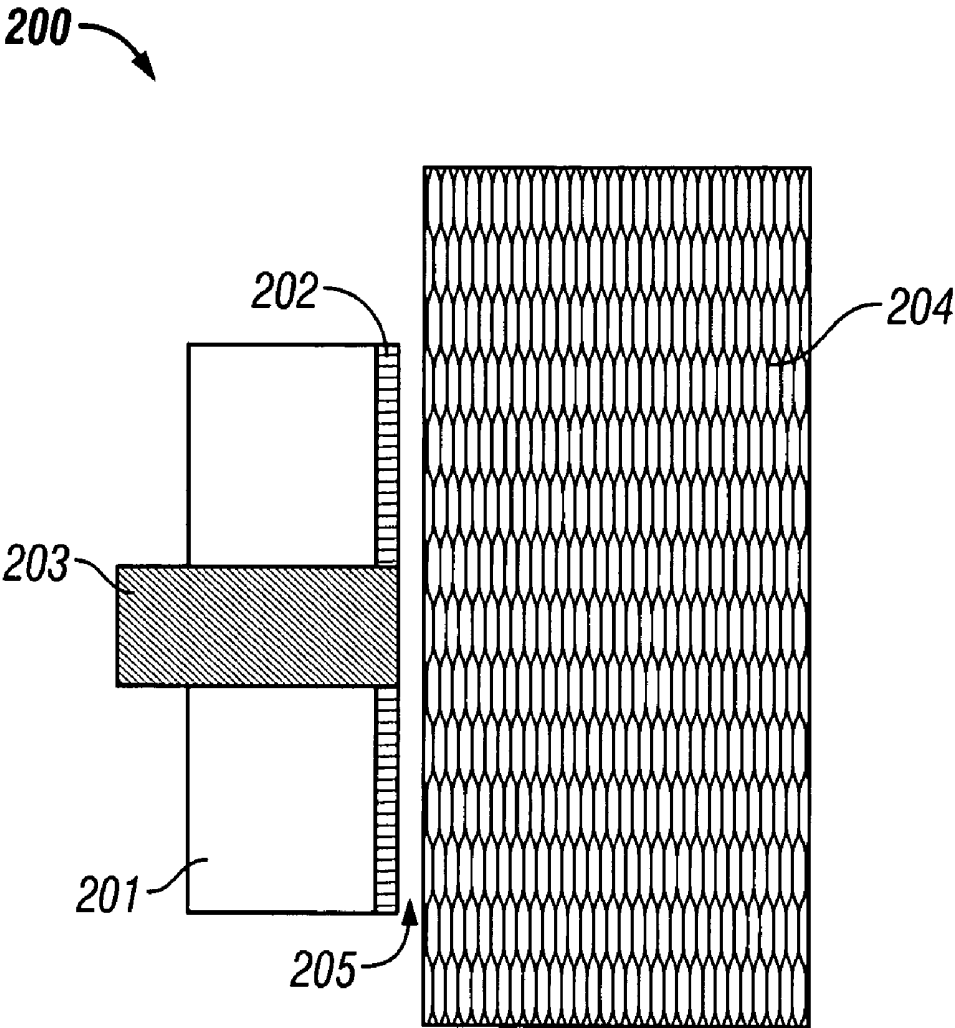


FIG. 2

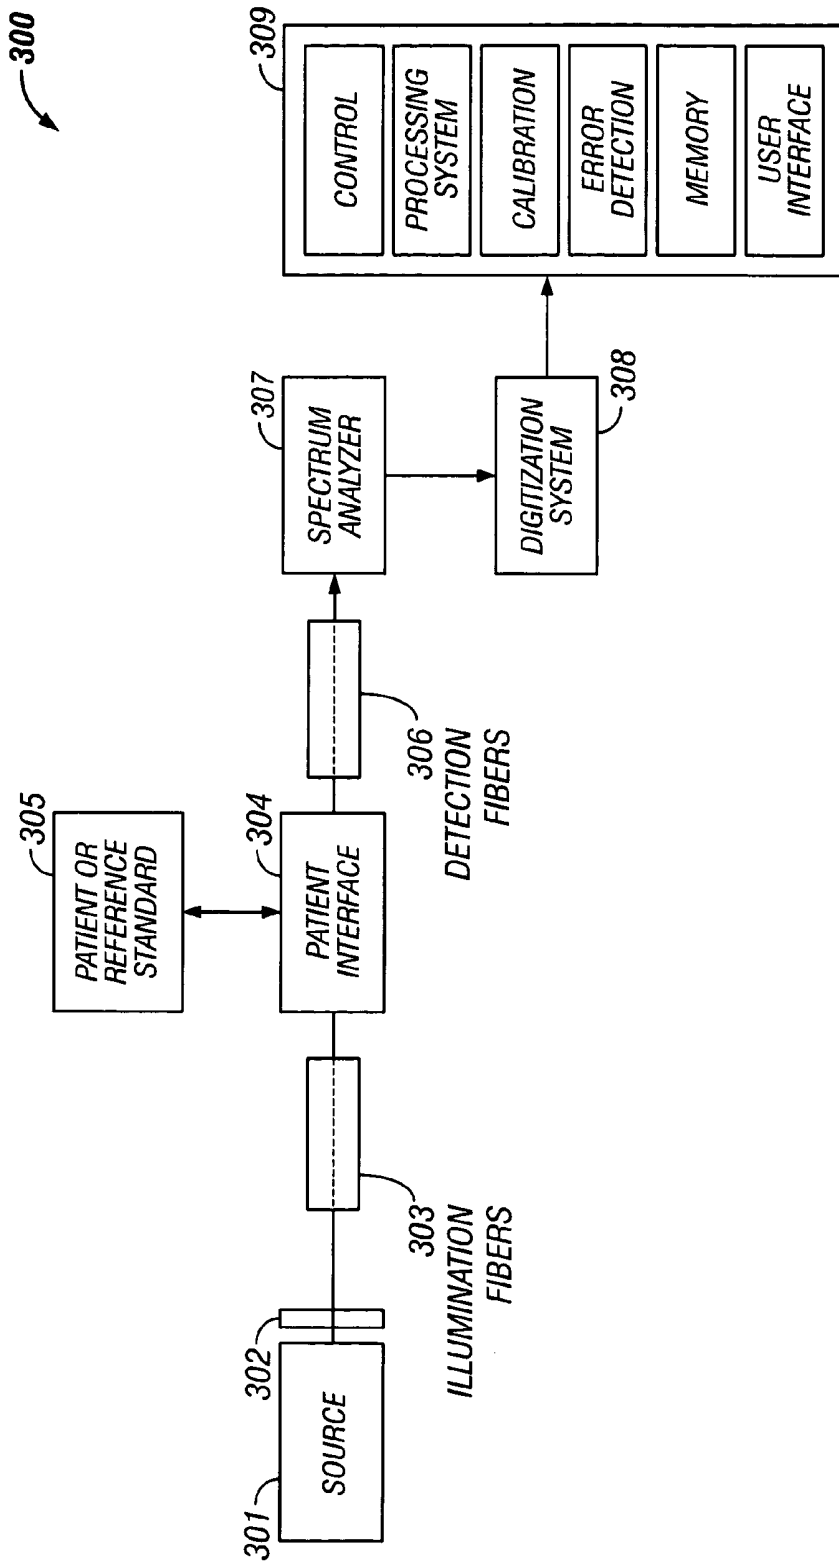


FIG. 3

METHOD AND APPARATUS FOR CONTROL OF SKIN PERFUSION FOR INDIRECT GLUCOSE MEASUREMENT

CROSS REFERENCE TO RELATED APPLICATIONS

[0001] This application claims benefit of U.S. Provisional Patent Application Ser. No. 60/363,345, filed Mar. 8, 2002; and is a Continuation-in-part of U.S. patent application Ser. No. 09/955,531, filed Sep. 17, 2001, which claims benefit of U.S. Provisional Patent Application Ser. No. 60/235,369, filed Sep. 26, 2000.

BACKGROUND OF THE INVENTION

[0002] 1. Field of the Invention

[0003] This invention relates generally to the field of non-invasive glucose measurement. More particularly, the invention relates to control of optical properties of the sampling site to improve reliability of a noninvasive glucose measurement.

[0004] 2. Background Information

[0005] Diabetes is a chronic disease involving the improper production and utilization of insulin, a hormone that facilitates glucose uptake into cells. While a precise cause of diabetes is unknown, both genetic and environmental factors such as obesity and lack of exercise appear to play roles. Persons with diabetes have increased health risk in three broad categories: cardiovascular heart disease, retinopathy, and neuropathy. Potential disease complications include heart disease and stroke, high blood pressure, kidney disease, neuropathy, retinopathy, diabetic ketoacidosis, skin conditions, gum disease, impotence, and fetal complications.

Diabetes Prevalence and Trends

[0006] The incidence of diabetes is both common and on the increase, making the disease a leading cause of death and disability worldwide. The World Health Organization (WHO) estimates that diabetes currently afflicts one hundred fifty-four million people worldwide. Fifty-four million people with diabetes live in developed countries. The WHO estimates that the incidence of diabetes will grow to three hundred million by the year 2025. In the United States, 15.7 million people or 5.9% of the population are estimated to have diabetes. Within the United States, the prevalence of adults diagnosed with diabetes increased by six percent in 1999 and rose by thirty-three percent between 1990 and 1998. This corresponds to approximately eight hundred thousand new cases every year in America. The estimated total cost to the United States economy exceeds \$90 billion per year. National Institutes of Health, *Diabetes Statistics*, Publication No. 98-3926, Bethesda Md. (1997).

[0007] Long-term clinical studies show that the onset of diabetes related complications can be significantly reduced through proper control of blood glucose levels. The Diabetes Control and Complications Trial Research Group, *The effect of intensive treatment of diabetes on the development and progression of long-term complications in insulin-dependent diabetes mellitus*, N Eng J of Med, 329:977-86 (1993); and 1 U.K. Prospective Diabetes Study (UKPDS) Group, *Intensive blood-glucose control with sulphonylureas or insulin compared with conventional treatment and risk of complications in patients with type 2 diabetes*, Lancet, 352:837-853 (1998);

and 1Y. Ohkubo, H. Kishikawa, E. Araki, T. Miyata, S. Isami, S. Motoyoshi, Y. Kojima, N. Furuyoshi, M. Shichizi, *Intensive insulin therapy prevents the progression of diabetic microvascular complications in Japanese patients with non-insulin-dependent diabetes mellitus: a randomized prospective 6-year study*, Diabetes Res Clin Pract, 28:103-117 (1995).

[0008] A vital element of diabetes management is the self-monitoring of blood glucose levels in the home environment. However, current monitoring techniques discourage regular use due to the inconvenient and painful nature of drawing blood through the skin prior to analysis. See The Diabetes Control and Complication Trial Research Group, *supra*. As a result, noninvasive measurement of glucose has been identified as a beneficial development for the management of diabetes. Implantable glucose analyzers eventually coupled to an insulin delivery system providing an artificial pancreas are also being pursued.

Glucose Measurement: History, Approaches, and Technologies

[0009] The treatment of diabetes has progressed through several stages. The combined development of insulin therapy and the development of devices for the self-monitoring of blood glucose in the home led to a radical improvement in the lives of individuals afflicted with diabetes. Self-monitoring of blood glucose has progressed through multiple stages from early testing that used urine samples to the current standard of invasive finger stick samples that are more accurate but somewhat painful. The development of alternative site glucose measurement technology has somewhat mitigated the pain aspects, but poses a biohazard. Alternate site blood glucose concentration levels are also known to differ from those taken at the fingertip during periods when glucose concentrations are rapidly changing. The difference is related to circulatory transport of glucose to peripheral tissues: Alternate site tissue sites with lower blood perfusion than the finger will exhibit a delay in the rise and fall of glucose levels when compared with finger blood glucose.

[0010] Current research is focused on the development of noninvasive technologies that will totally eliminate the pain associated with glucose determination and fluid biohazard issues. Another important area of research involves the combination of automated glucose measurement and insulin therapy. Progress has been reported in the research on implantable or full-loop systems that have been proposed to incorporate both glucose measurement and control through automated insulin delivery. In the interim, a device that provides noninvasive, automatic, or (nearly) continuous measurement of glucose levels would clearly be useful to those afflicted with diabetes. Various systems have been developed with this goal in mind. J. Tamada, S. Garg, L. Jovanovic, K. Pitzer, S. Fermi, R. Potts, *Noninvasive glucose monitoring comprehensive clinical results*, JAMA, 282:1839-1844 (1999) describe a minimally-invasive monitoring system reported that provides three readings of interstitial fluid glucose per hour, each delayed by up to fifteen minutes due to the sample acquisition process. The measurement is made through an electrochemical-enzymatic sensor on a sample of interstitial fluid that is drawn through the skin using an iontophoresis technique. Other approaches, such as the continuous monitoring system reported by T. Gross, B. Bode, D. Einhorn, D. Kayne, J. Reed, N. White and J. Mastrototaro,

Performance evaluation of the Minimed® continuous glucose monitoring system during patient home use, Diabetes Technology & Therapeutics, Vol. 2, Num. 1, (2000) involve the surgical implantation of a sensor in tissue. Health risks due to sensor implantation or measurement delay remain as obstacles to efficacious use of these devices in directing insulin therapy. To date, a fully noninvasive alternative has not been approved by the FDA.

Noninvasive Glucose Measurement

[0011] There exist a number of noninvasive approaches for glucose determination. These approaches vary widely, but have at least two common steps. First, an apparatus is utilized to acquire a reading from the body without obtaining a biological sample. Second, an algorithm is utilized to convert this reading into a glucose determination.

[0012] A generalized approach to noninvasive glucose measurement utilizes some form of spectroscopy to acquire the signal or spectrum from a measurement site on the subject's body. Techniques include but are not limited to: impedance, Raman, and fluorescence; as well as techniques using light, from the ultraviolet through the infrared [ultraviolet (200 to 400 nm), visible (400 to 700 nm), near-IR (700 to 2500 nm or 14,286 to 4000 cm^{-1}), infrared (2500 to 14,285 nm or 4000-700 cm^{-1})]. A specific near infrared range for noninvasive glucose determination in diffuse reflectance mode is about 1100 to 2500 nm or ranges or sets of ranges therein. K. Hazen, *Glucose Determination in Biological Matrices Using Near-infrared Spectroscopy*, doctoral dissertation, University of Iowa (1995). It is important to note, that these techniques are distinct from the minimally invasive techniques listed above in that the sample analyzed is a portion of the human body in situ, not a biological sample extracted from the human body.

[0013] Potential sites for the noninvasive measurement have been identified from the ear lobe, oral mucosa, arm, and eye to the fingertip. It is important to note that noninvasive techniques do not have to be based upon spectroscopy. Within the context of the invention, any device that reads glucose from the body without penetrating the skin and collecting a biological sample is classified as a noninvasive glucose analyzer.

[0014] To date, noninvasive glucose measurement has conventionally employed a direct measurement approach, in which the net analyte signal due to the absorption of light by glucose in the tissue is used to calculate the glucose concentration. There exist formidable challenges to the development of reliable methods of glucose measurement using a direct approach. Among these challenges are the size of the glucose signal relative to the spectral background, the heterogeneity of the sample, the multi-layered structure of the skin, the rapid variation related to hydration levels, changes in the volume fraction of blood in the tissue, hormonal stimulation, temperature fluctuations, and blood analyte levels. Control of the optical properties of the sample site is essential to the success of any method of noninvasive glucose measurement using a direct measurement approach.

Calibration And Utilization Of Noninvasive Glucose Meters

[0015] One noninvasive technology, near-infrared spectroscopy, provides the opportunity for both frequent and painless noninvasive measurement of glucose. This approach involves the illumination of a spot on the body with near-

infrared (NIR) electromagnetic radiation, light in the wavelength range 700 to 2500 nm. The light is partially absorbed and scattered, according to its interaction with the constituents of the tissue. The actual tissue volume that is sampled is the portion of irradiated tissue from which light is collected and transported to the spectrometer detection system. Generation of a suitable calibration involves development of a mathematical relationship between an in vivo near-infrared spectral measurement and a corresponding reference blood glucose concentration. The model generation process includes the collection of a multiplicity of matched spectrum/reference glucose pairs followed by the calculation of a regression model between the multiple independent variables contained in each spectral vector and the associated single dependent reference glucose value. Reference blood glucose values are typically obtained directly through the use of measurement tools like the HEMOCUE (YSI, Inc., Yellow Springs Ohio) or any other reliable invasive glucose analyzer.

[0016] The Beer-Lambert Law, equation 1 infra, defines a proportionality constant between glucose concentration and spectral light absorbed at a single spectral wavelength in the special case where no interfering spectral signatures are present. In equation 1, A is the scalar absorbance measurement at a given wavelength of light, ϵ is the molar absorptivity associated with the molecule of interest at the same given wavelength, b is the distance (or pathlength) that the light travels through the sample, and C is the concentration of the molecule of interest (glucose).

$$A = \epsilon b C$$

[0017] A number of interferences do exist for the near-infrared measurement making the correction for these interferences necessary. Correction is achieved by using multiple wavelengths in each spectrum in a multivariate regression model. Such a model is proven means for compensation of spectral interferences, requiring some measure of uniqueness in the spectral signature of the glucose.

$$= C$$

[0018] In equation 2, boldface type denotes vector variables. The expression is interpreted as the outer product of the regression vector k and the absorbance spectrum vector A , consisting of the absorbance at a multiplicity of selected wavelengths, is equal to the glucose concentration C of the sample.

[0019] Common multivariate approaches that can be used to solve the equation 2 for the regression vector k can include partial least squares (PLS) and principal component regression (PCR). Nonparametric methods of calibration such as neural networks and multiple adaptive regression splines (MARS) can also be used to model an expression analogous to equation 2 in the case where Beer's law deviations are present and the relation becomes nonlinear.

[0020] Because every method of glucose measurement has error, it is beneficial that the primary reference device, which is used to develop and evaluate noninvasive calibrations for blood glucose, be as accurate as possible to minimize the uncertainty in the model. An instrument with a percentage error of five or less is most desirable. An instrument having a percentage error of up to ten would be suitable, though the error of the device being calibrated may increase.

Instrumentation

[0021] Non invasive

[0022] A number of technologies have been proposed for measuring glucose non-invasively, all of which involve some type of tissue measurement. Spectroscopy-based noninvasive glucose analyzers utilize the measured interaction of the tissue sample with electromagnetic radiation (EMR) or another type of energy input that leads to an emission of EMR to acquire the signal or spectrum. Examples include but are not limited to Nuclear Magnetic Resonance (NMR) spectroscopy, UV, visible near-infrared, mid-infrared, and far-infrared spectroscopy, tissue impedance spectroscopy, Raman spectroscopy, and fluorescence spectroscopy. The near infrared range for noninvasive glucose determination in diffuse reflectance mode is about 1100 to 2500 nm or ranges therein. Hazen (1995), supra. It is important to define noninvasive techniques as being distinct from invasive techniques in that the noninvasive sample is analyzed in-situ, as opposed to invasively extracting a biological sample through the skin for analysis. The actual tissue volume that is sampled is the portion of irradiated tissue from which light is reflected or transmitted to the spectrometer detection system. All of these techniques share the common characteristic that, as secondary calibration methods, they require a calibration, model or other transformation to convert the measured signal to an estimate of the glucose concentration using reference measurements based on a primary method, such as invasive measurements from samples of venous or capillary blood.

[0023] A number of spectrometer configurations exist for collecting noninvasive spectra from regions of the body. Typically a spectrometer has one or more beam paths from a source to a detector. A light source may include a blackbody source, a tungsten-halogen source, one or more LED's, or one or more laser diodes. For multi-wavelength spectrometers a wavelength selection device may be utilized or a series of optical filters may be utilized for wavelength selection. Wavelength selection devices include dispersive elements such as prisms, and gratings of various types. Nondispersive wavelength selective devices include interferometers, successive illumination of the elements of an LED array, and wavelength selective filters. Detectors may be in the form of one or more single element detectors or one or more arrays or bundles of detectors. Detector materials are selected to obtain the desired signal measurement characteristics over the necessary wavelength ranges. Light collection optics such as fiber optics, lenses, and mirrors are commonly utilized in various configurations within a spectrometer to direct light from the source to the detector by way of a sample.

[0024] The interface of the glucose analyzer to the tissue includes a patient interface module for directing light into and collecting light from the tissue measurement site. Optical conduits for directing and collecting light may include a light pipe, fiber optics, a focusing lens system, or a light directing mirror system.

[0025] The scanning of the tissue can be done continuously when pulsation effects do not affect the tissue area being tested, or the scanning can be done intermittently between pulses. The collected signal (near-infrared radiation in this case) is converted to a voltage and sampled through an analog-to-digital converter for analysis on a microprocessor based system and the result displayed.

Related Skin Physiology

[0026] One of the primary functions of cutaneous skin is to provide a means for thermoregulatory control of body temperature. Blood at approximately 98° F. is pumped to the outer skin layers to provide nutrients, is a means for waste removal, and is a mechanism for thermoregulatory control. In the case of warm ambient temperatures, heat can be dissipated from the core of the body when increased blood flow is combined with the cooling effects of sweat evaporation on the skin surface. In the case of cool ambient temperatures, heat can also be used to warm a cool skin surface, but rapid heat loss associated with touching cold objects is limited by constrictively reducing blood flow to the superficial tissues. These thermoregulatory mechanisms typically use constriction or dilation of capillary vessels and the concomitant variation in blood flow to control the potential for heat transfer to and from the body. Capillary diameters can vary tenfold during these processes.

[0027] A tenfold variation in capillary vessel diameter can lead to substantial changes in the composition and optical properties of the tissue. Such variation in the measured tissue sample can lead to poor sampling precision over a sequential series of measurements. Sample normalization of a varying signal derived from the heterogeneous, layered structure of skin can be of limited effectiveness due to spectral nonlinearities imposed by the compositional variation of the layers and the sequential path of light through the various layers of skin. Specifically, the broadband source light is filtered uniquely in the wavelength domain by each skin layer according to the changing compositions and varying optical densities that result with a perfusion shift in the tissue. The result is that the optical sample is destabilized in a nonlinear manner that is difficult or impossible to normalize with a high degree of accuracy. It follows that the modeling of glucose concentration will be most efficacious under the conditions that variations in the optical properties of the sample are minimized excepting where changes in the optical properties are a direct result of glucose variation.

[0028] Accuracy and robustness are improved with thermal control in the case of either a conventional direct measurement or an indirect measurement, described below, of blood glucose. Thermally or mechanically stimulated changes in optical properties will complicate direct noninvasive glucose determinations. Thermal perturbations are addressed herein using the knowledge of human vascular response to heat and cold and by limiting temperature transients due to skin contact with objects that differ by more than 5 degrees F. from typical resting skin temperatures of 85-95° F.

DESCRIPTION OF RELATED TECHNOLOGY

[0029] There are a number of issues related to obtaining representative samples in analytical technologies. Factors affecting sample stability may be environmental or natural physiological variation that can arise from variations in sample site location or time dependent physiologies. Environmental factors, such as temperature, can affect instrumentation, electronics, and physiological components. For example, in near-IR spectroscopy, environmental temperature may affect either or both of the alignment of a spectrometer and the temperature of the probing device, which secondarily affects the tissue temperature upon contact. In the case of noninvasive glucose determination performed via

near-IR spectroscopy, the result of these changes is a change in the acquired spectra due to the effect of temperature and pressure on tissue optical properties.

[0030] Furthermore, temperature effects the localized perfusion of the tissue. The localized perfusion is important for several reasons. First, vasodilatation of the surface capillaries affects the amount of blood present near the skin surface. This change can effect the glucose concentration in the sampled tissue volume. Second, it has been reported that blood at alternative sites, such as the forearm, can contain glucose concentrations that are dampened and/or delayed versus blood in well perfused areas, such as an artery, vein, or fingertip capillary bed. K. Jungheim, T. Koschinsky, *Glucose Monitoring at the Arm*, *Diabetes Care*, 25:956-960 (2002); and K. Jungheim, T. Koschinsky, *Risky delay of hypoglycemia detection by glucose monitoring at the arm*, *Diabetes Care*, 24:1303-1304 (2001); and J. Fischer, K. Hazen, M. Welch, L. Hockersmith, J. Coates, *Comparisons of capillary blood glucose concentrations from the fingertips and the volar aspects of the left and right forearms*, American Diabetes Association, 62nd Annual Meeting (Jun. 14, 2002).

[0031] A number of approaches have been utilized to minimize this lag. For example, M. Rohrscheib, C. Gardner, M. Robinson, *Method and apparatus for noninvasive blood analyte measurement with fluid compartment equilibration*, U.S. Pat. No. 6,240,306 (May 29, 2001) suggests applying heat to the skin surface to increase perfusion. The Rohrscheib patent describes elevating localized skin temperature from 35° C. by at least 5° C. and preferably by about 7° C. in order to equilibrate the glucose concentration between the vascular system and skin tissue. The reported mechanism involves the local dilation of capillaries to increase blood flow, which results in a partial equalization of the venous and capillary glucose concentrations. Rohrscheib, et al. further teach use of vasodilating agents such as nicotinic acid, methyl nicotinamide, minoxidil, nitroglycerin, histamine, capsaicin, or menthol to increase local blood flow. While tissue perfusion can be increased to maximal levels though application of thermal energy, it has the additional undesirable effect of destabilizing optical properties of the tissue sample.

[0032] A method and apparatus for sample site temperature stabilization in conjunction with near-IR based noninvasive glucose determination has been reported. K. Hazen (1995), supra, pp. 193-249. This method utilizes a heater in thermal contact with the sampling site, but the methodology is for a direct reading of glucose and the temperatures are elevated to above forty degrees centigrade.

[0033] There exists therefore a need in the art for a noninvasive method of glucose measurement that overcomes the difficulties inherent in methods based on direct measurement of a net analyte signal. There further exists a need to maximize the reliability of such a method by providing a means for controlling and/or eliminating the fluctuation of optical properties of tissue sample by stabilizing perfusion of the sample site.

SUMMARY OF THE INVENTION

[0034] The invention provides methods and a system for non-invasively measuring key constituents and properties of tissue. A target analyte is measured indirectly based on the natural response of tissue to variations in analyte concentration. The indirect method of measuring utilizes factors that

are effected by or correlated with the concentration of glucose, such as the index of refraction, electrolyte distribution or reduced scattering coefficient of the bulk tissue. An indirect measurement means that an ancillary effect due to changes in glucose concentration is being measured.

[0035] The reliability of the measurement is greatly improved by stabilizing the optical properties of the tissue at the measurement site, thus means are provided for regulating blood perfusion rates at the sample site. In one embodiment, perfusion is monitored and stabilized by spectroscopically measuring a control parameter, such as skin temperature, that directly affects perfusion. The control parameter is maintained in a range about a set point, thus stabilizing perfusion. Skin temperature is controlled using a variety of means, including the use of active heating and cooling elements, passive devices, such as thermal wraps, and through the use of a heated coupling medium having favorable heat transfer properties.

BRIEF DESCRIPTION OF THE DRAWINGS

[0036] FIG. 1 provides a flow diagram of a method for regulating a control parameter at a tissue measurement site according to the invention;

[0037] FIG. 2 provides a schematic diagram of a subject interface module according to the invention; and

[0038] FIG. 3 shows a schematic diagram of an apparatus for noninvasive glucose determination according to the invention.

DETAILED DESCRIPTION

Indirect Measurement

[0039] A method for indirectly determining a concentration of a target analyte, such as glucose, non-invasively is described in the commonly-assigned U.S. patent application Ser. No. 10/xxx,xxx (SENS0006), the entirety of which is hereby incorporated by reference as if fully set forth herein. The method takes advantage of the fact that tissue properties are responsive to and reflect physiological variations in the tissue related to variations in the concentration of analyte. An analytical signal is collected at a sampling site on a subject's body. Features are extracted from the analytical signals that are indicative of the target analyte on the sampled tissue. Analyte concentration is calculated indirectly by applying a calibration model to the features. The extracted features are reflective of changes in tissue properties, which themselves are responsive to and reflect physiological variations in the tissue related to variations in the concentration of analyte. Thus, indirect measurement measures a target analyte by measuring an ancillary effect of the target analyte.

[0040] The invention provides a method and apparatus of noninvasive glucose measurement in which blood perfusion at the sample site is regulated through regulation of a control parameter that directly influences perfusion, such as skin temperature. FIG. 1 shows a flow diagram of a method for noninvasive glucose determination that includes perfusion control at the sample site. As shown in FIG. 1, perfusion is controlled through the provision of a feedback loop that maintains the control parameter within an acceptable range about a set point. For example, blood perfusion increases rapidly and is volatile above skin temperatures of 40° C., thus it is desirable to regulate skin temperature at the sampling site to

a range between approximately 30 and 40° C.; preferably the skin temperature is controlled between 30 and 35° C. More preferably, the skin is controlled to within one degree of a control set-point in a range of 30 to 35° C. The control set point is established by the environmental conditions and the patient physiology at the time of a periodic instrument bias correction. Notably, only the outermost 100 μm of skin temperature need be controlled, as below this depth the capillary bed controls the skin temperature. While the invention specifically provides a method of indirect measurement as described above, the principle of controlling blood perfusion is also readily applied to noninvasive measurement approaches in which analyte concentration is directly determined based on the net analyte signal.

[0041] In the preferred embodiment, local perfusion is monitored spectroscopically and controlled through regulation of the control parameter. The invented method generally includes steps of:

[0042] Measuring an analytical signal **101**. As shown in FIG. 1, the analytical signal is a near-infrared absorbance spectrum. However, the principles of the invention are applicable to other noninvasive measurement technologies as well. Measurement may be performed using instrumentation as shown in FIG. 3;

[0043] The control parameter is measured spectroscopically through application of a first calibration model to the spectral measurement **102**, and the value of the parameter relative to the set point **103** is determined;

[0044] The relative value of the control parameter is evaluated **104** to determine if it is within the acceptable range about the set point **103**;

[0045] If the control parameter measurement is acceptable, a glucose calibration **107** is applied to the spectral measurement to produce a glucose measurement;

[0046] If the control parameter measurement isn't within an acceptable, an error is generated, and the value is supplied as an input **105** to an element **106** for regulating the control parameter. The loop is repeated, with the control parameter being repeatedly evaluated until the measurement is within the acceptable range.

[0047] One embodiment of the above invention provides a method and apparatus for minimizing the confounding effects in a noninvasive spectral measurement attributable to shifts in skin temperature at the tissue measurement site. Near-infrared measurements of skin combined with associated skin temperature reference measurements are used to develop NIR temperature calibrations that require only NIR tissue scans to predict skin surface temperature. Methods of developing calibrations for spectral analysis may employ a variety of multivariate analytical techniques that are well known to those skilled in the art. NIR skin temperature calibration is made possible by the known shifting of the 1450 or 1900 nm water band with variations in skin temperature. The calibration model incorporates the shift information implicitly in the multivariate regression coefficients. Temperature measurement and control of human tissue is important in noninvasive NIR measurement because it provides a means of simplifying the complex overlapping spectral effects that inhibit extraction of the analyte signal. The extra temperature measurement hardware and the associated cost and complexity are avoided by using NIR temperature measurement.

[0048] Skin temperature at the measurement site is spectroscopically monitored by calculating temperature values through the application of a multivariate calibration model that correlates spectroscopic changes with shifts in skin temperature. Advantageously, thermal time constants imposed by conventional temperature sensing devices are eliminated, providing near-instantaneous temperature readings.

[0049] Temperature control may be either active or passive.

[0050] Passive control is achieved through the selective application and removal of an occlusive thermal wrap. Active control is provided by a thermistor applied to the skin in the vicinity of the measurement site. Active and passive control may be applied in complementary fashion or they may be used separately. In a particularly preferred embodiment of the invention, the control means is incorporated into the measurement instrument, wherein the calculated skin temperature values provide the feedback in a closed loop that drives the control device. In an alternate embodiment of the invention, the temperature values are supplied to an operator, who then applies active and/or passive control to achieve and maintain a skin temperature within the target range. By monitoring skin temperature spectroscopically and employing methods of passive and/or active control it is possible to reduce the effects of skin temperature variation on the spectral measurement. Active control may be by way of a conductive element, as described above, or it may also be provided by a radiative element.

Non-Spectroscopic Control

[0051] Alternately, perfusion can be controlled in an open-loop fashion by maintaining skin temperature at a specific set-point, as shown in FIG. 2. The control of skin temperature is performed conductively through heating and cooling element **201** included as part of a patient interface module **200**. In one embodiment, the heating and cooling element may be energy transfer pads. Alternately, skin temperature is controlled through radiative energy transfer from an energy source. The system may include means for monitoring the skin temperature at the measurement site either spectroscopically or through a temperature probe (not shown). During use, a noninvasive probe **203** is placed against the skin at the sample site **204**. A coupling medium **205** is employed between the patient interface **202** and the tissue **204**. The coupling medium serves to facilitate heat transfer between the patient interface **202** and the tissue **204**.

Skin Temperature Regulation Using Heated Coupling Medium.

[0052] As previously mentioned, the coupling medium itself may serve to control skin temperature at the sampling site. Thus, an embodiment of the invention is possible in which a heated coupling medium provides the thermal energy to maintain the skin of a sampling site at or near a set point. A number of compounds are suitable for use as a coupling medium; for example, silicone oil. Glycerol and mineral oil could also be used, but they are less desirable alternatives, in view of the fact that both materials contain carbon-hydrogen bonds that could interfere with spectroscopic analysis of an analyte such as glucose.

[0053] A particularly preferred embodiment of the coupling medium is the perfluorinated liquid FLUORINERT, either FC-40 or FC-70 (3M COMPANY, ST. PAUL Minn.). While the FLUORINERT functions to reduce surface reflec-

tion variations in the noninvasive **20** measurement, its heat transfer properties are well suited for use as a thermal regulator. Because the FLUORINERT comes into contact with skin at the measurement site, heat can be transferred across the skin if the temperature of the FLUORINERT differs from that of the skin.

[**0054**] Heated FLUORINERT can be used in place of a heated probe with the advantage of reduced power consumption when compared with a temperature controlled metal probe contact surface. The advantage is gained by the rapid heating of small amounts of FLUORINERT just prior to the measurement. Periodic rapid heating saves power over continuous heating of the metal heater contact surface thereby reducing power consumption and lengthening battery life. The use of heated FLUORINERT also allows for the relocation of the heating electronics away from the probe for increased safety. The use of heated FLUORINERT also allows for the heating of the tissue at the measurement site, which is not heated directly by the probe surface heater as it is not in contact with the tissue at the measurement site. During use, a portion of the heated FLUORINERT is disposed between the patient interface of the probe and the skin surface of the measurement site. Alternatively, the coupling fluid may be heated by the source element in embodiments where the source element is in close proximity to the sampling site.

Instrumentation

[**0055**] While a variety of sensors or instrument configurations are suitable for practice of the invention, FIG. 3 provides a schematic diagram of a preferred embodiment of the sensor. The sensor includes a radiation source such as a tungsten halogen near-infrared radiation source **301**, a wavelength selection filter **302** passing light in a range of approximately 1150 to 1850 nm; optional illumination fibers **303** for conveying the source photons to an in-vivo skin sample **204**; an interface **200** to the sample site, for example, a patient's forearm; detection fibers **306** for gathering diffusely reflected and transmitted radiation from the skin to a spectrum analyzer **307** that includes, for example a grating (not shown), and a detector array (not shown) to detect the radiation; an AD (analog-to-digital) converter **308** for converting the detected signal to a voltage; and processing means **309** for converting the voltage into a glucose concentration.

[**0056**] Although the invention has been described herein with reference to certain preferred embodiments, one skilled in the art will readily appreciate that other applications may be substituted for those set forth herein without departing from the spirit and scope of the present invention. Accordingly, the invention should only be limited by the claims included below.

1. A noninvasive method of measuring a tissue analyte, comprising steps of:

- stabilizing optical properties of said tissue at a measurement site;
- collecting an analytical signal from the tissue, said collected signal comprising a tissue measurement;
- extracting features from the analytical signal indicative of the affect of the target analyte on the probed tissue; and
- calculating concentration of said analyte indirectly by application of a calibration model to said features.

2. The method of claim 1, wherein said step of stabilizing optical properties comprises stabilizing perfusion at said measurement site.

3. The method of claim 2, wherein said step of stabilizing perfusion comprises:

- controlling skin temperature at said measurement site.

4. The method of claim 3, wherein step of controlling skin temperature at said measurement site comprises any of the steps of:

- applying a passive means of temperature control; and

- applying an active means of temperature control.

5. The method of claim 4, wherein said passive means of temperature control comprises a thermal wrap applied by an operator.

6. The method of claim 4, wherein said active means of temperature control comprises any of:

- at least one radiative heating element;

- at least one conductive heating/cooling element.

7. The method of claim 6, wherein said one or both of said at least one radiative element and said at least one conductive heating/cooling element are embodied within a subject interface of a measurement sensor.

8. The method of claim 3, wherein said step of controlling skin temperature at said measurement site comprises steps of:

- providing a coupling medium;

- heating a portion of said coupling medium; and

- disposing said heated portion of said coupling medium between a patient interface of patient interface module and said skin at said measurement site, wherein transfer of thermal energy from said heated portion of said coupling medium to said skin occurs.

9. The method of claim 8, wherein said coupling medium comprises any of:

- silicone oil;

- mineral oil; and

- glycerol.

10. The method of claim 8, wherein said coupling medium comprises a perfluorocarbon liquid.

11. The method of claim 10, wherein said perfluorocarbon liquid comprises FLUORINERT perfluorocarbon liquid.

12. The method of claim 11, wherein said FLUORINERT perfluorocarbon liquid comprises one of FC-40 and FC-70.

13. The method of claim 3, wherein skin temperature is controlled to between approximately 30 and 40 degrees centigrade;

14. The method of claim 13, wherein skin temperature is controlled to between approximately 30 and 35 degrees centigrade.

15. The method of claim 3, wherein skin temperature is maintained to within approximately 1 degree centigrade of a set point.

16. The method of claim 15, wherein outermost 100 μm of said skin is controlled to within approximately 1 degree centigrade of a set point.

17. The method of claim 1, wherein said analyte comprises glucose.

18. A noninvasive method of measuring a tissue analyte, comprising steps of:

providing a coupling medium;

heating a portion of said coupling medium;

disposing said heated portion of said coupling medium between a measurement probe and a skin surface at a sampling site;

collecting an analytical signal from the tissue, said collected signal comprising a tissue measurement; and

calculating concentration of said analyte from said tissue measurement.

19. The method of claim 18, wherein said coupling medium comprises a perfluorocarbon liquid.

20. The method of claim 19, wherein said perfluorocarbon liquid comprises FLUORINERT perfluorocarbon liquid.

21. The method of claim 20, wherein said FLUORINERT perfluorocarbon liquid comprises one of FC-40 and FC-70.

22. The method of claim 18, further comprising a step of: extracting features from the analytical signal indicative of the effect of the target analyte on the probed tissue.

23. The method of claim 19, wherein said step of calculating concentration of said analyte from said tissue measurement comprises calculating concentration of said analyte indirectly by application of a calibration model to said features.

24. The method of claim 18, wherein said analyte comprises glucose.

* * * * *

专利名称(译)	用于控制间接葡萄糖测量的皮肤灌注的方法和设备		
公开(公告)号	US20080200783A9	公开(公告)日	2008-08-21
申请号	US10/384049	申请日	2003-03-07
[标]申请(专利权)人(译)	BLANK THOMAS 乙 Ruchti酒店TIMOTHY大号 MATTU穆图阿 MAKAREWICZ MARCY MONFRE STEPHEN大号 LORENZ ALEXANDERÐ		
申请(专利权)人(译)	BLANK THOMAS B. Ruchti酒店TIMOTHY L. MATTU穆图阿 MAKAREWICZ MARCY MONFRE斯蒂芬L. LORENZ ALEXANDER D.		
当前申请(专利权)人(译)	GLT收购CORP.		
[标]发明人	BLANK THOMAS B RUCHTI TIMOTHY L MATTU MUTUA MAKAREWICZ MARCY MONFRE STEPHEN L LORENZ ALEXANDER D		
发明人	BLANK, THOMAS B. RUCHTI, TIMOTHY L. MATTU, MUTUA MAKAREWICZ, MARCY MONFRE, STEPHEN L. LORENZ, ALEXANDER D.		
IPC分类号	A61B5/00 G01N21/31 G01N21/33 G01N21/35 G01N21/65		
CPC分类号	A61B5/14532 A61B5/1455 A61B5/1491 A61B5/1495 G01N2021/3595 G01N21/31 G01N21/33 G01N21/359 G01N21/65 A61B2560/0223		
优先权	60/235369 2000-09-26 US 60/363345 2002-03-08 US		
其他公开文献	US20040039271A1 US7509153		
外部链接	Espacenet USPTO		

摘要(译)

用于非侵入性葡萄糖测量的方法和设备间接地从组织的自然响应测量葡萄糖到分析物浓度的变化。间接测量方法利用受葡萄糖浓度影响或与葡萄糖浓度相关的因素，例如折射率，电解质分布或组织散射。通过稳定测量部位处的组织的光学性质极大地改善了测量可靠性，因此调节了样品部位处的血液灌注速率。通过光谱测量直接影响灌注的控制参数（例如皮肤温度）来监测和稳定灌注。控制参数保持在约设定点的范围内，从而稳定灌注。使用各种手段控制皮肤温度，包括使用主动加热和冷却元件，无源装置，例如热包裹，以及通过使用具有有利传热性能的加热耦合介质。

