



(19) **United States**

(12) **Patent Application Publication**
Eberle et al.

(10) **Pub. No.: US 2013/0211855 A1**
(43) **Pub. Date: Aug. 15, 2013**

(54) **ALGORITHM FOR NARRATIVE GENERATION**

Publication Classification

(76) Inventors: **LeAnne M. Eberle**, Mahtomedi, MN (US); **David L. Perschbacher**, Coon Rapids, MN (US); **Chen Yee Wong**, Shoreview, MN (US); **Weiguang Shao**, Woodbury, MN (US)

(51) **Int. Cl.**
G06F 19/00 (2006.01)
A61B 5/00 (2006.01)
(52) **U.S. Cl.**
CPC **G06F 19/3487** (2013.01); **A61B 5/0022** (2013.01)
USPC **705/3**; 600/518; 600/515; 600/529

(21) Appl. No.: **13/589,513**

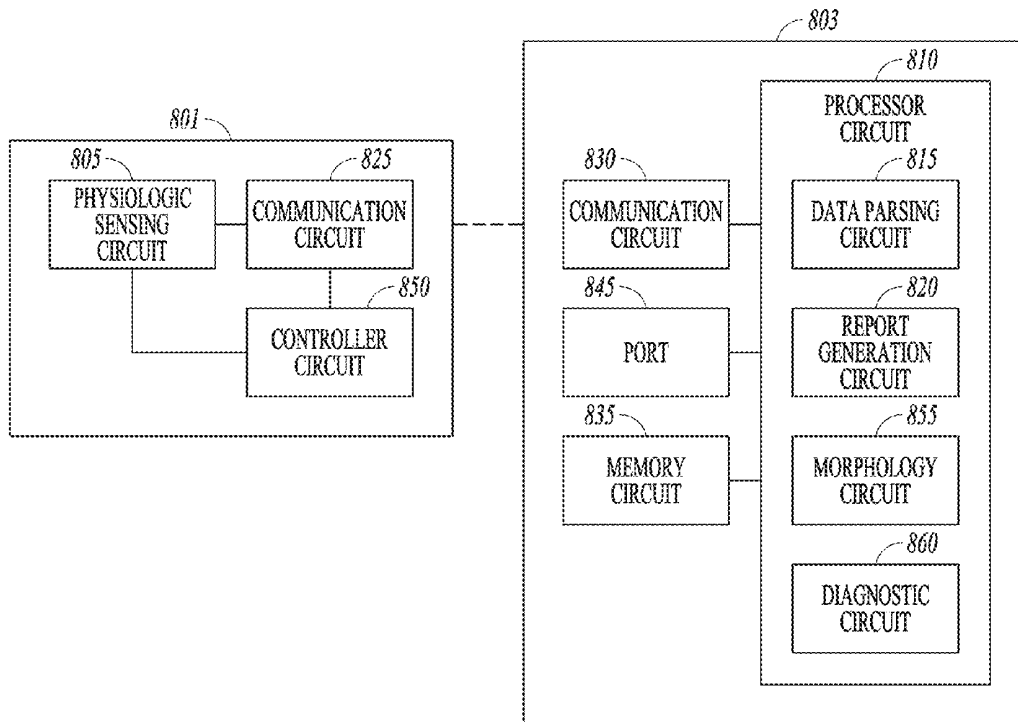
(57) **ABSTRACT**

(22) Filed: **Aug. 20, 2012**

A system comprises a physiologic sensing circuit configured to generate physiologic data for a subject and a processing circuit. The processing circuit includes a data parsing circuit configured to parse the physiologic data to identify one or more physiologic events and a report generation circuit. The report generation circuit is configured to associate narrative text with the identified physiologic events according to a text generating rule and generate a narrative report for the identified physiologic events using the narrative text.

Related U.S. Application Data

(60) Provisional application No. 61/528,372, filed on Aug. 29, 2011.



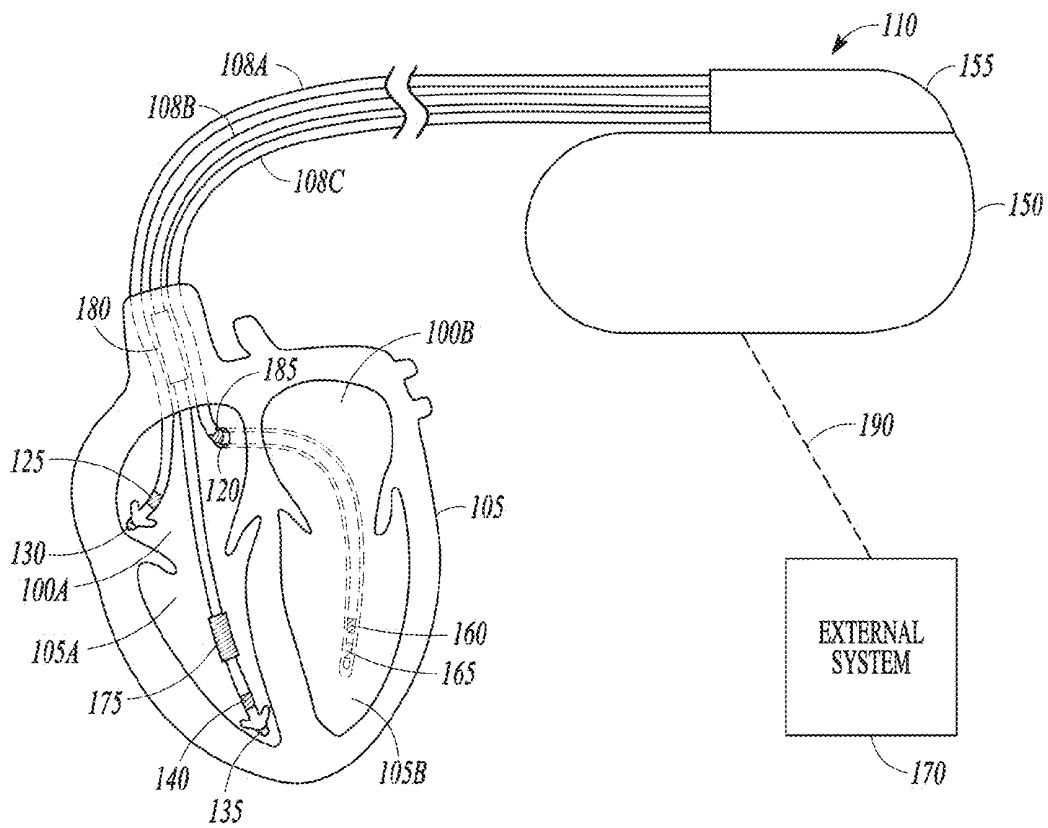


FIG. 1

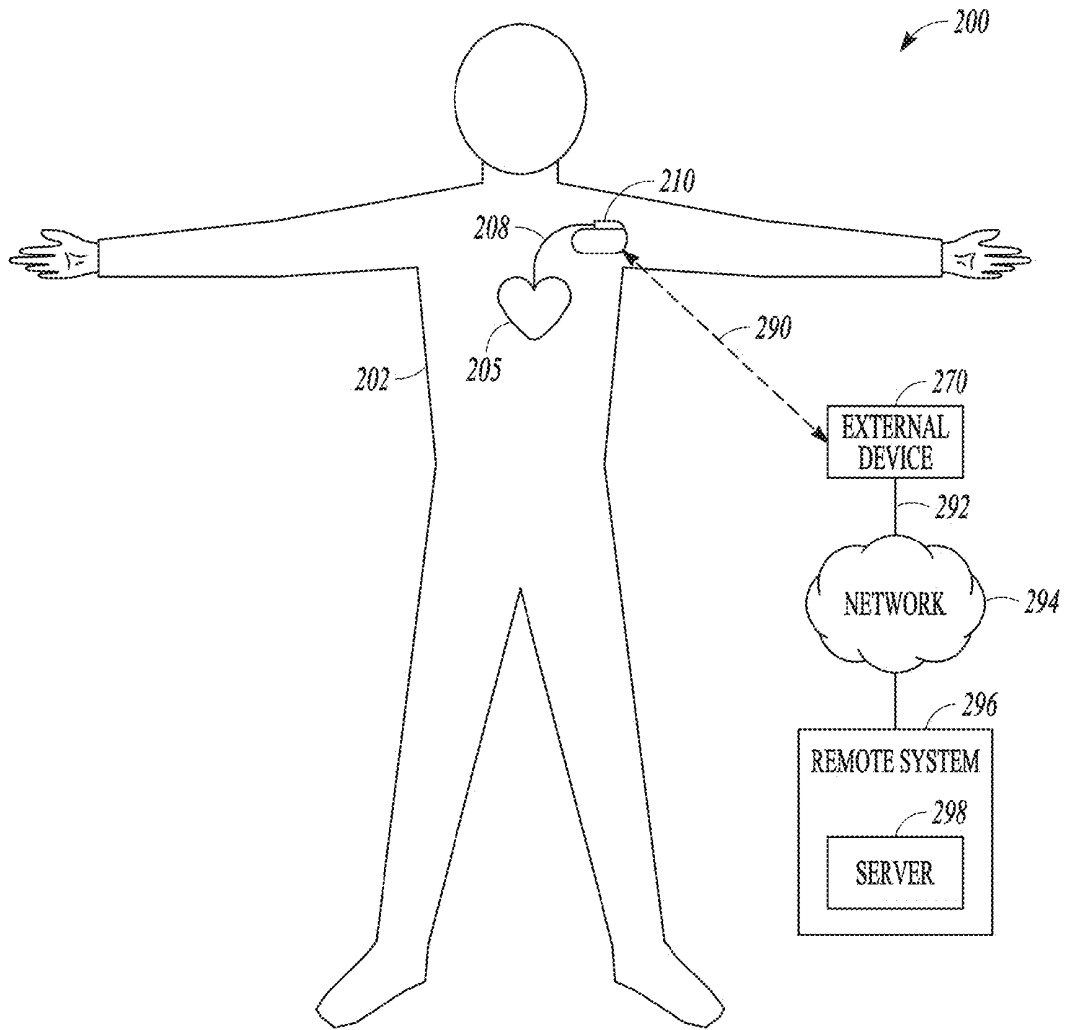


FIG. 2

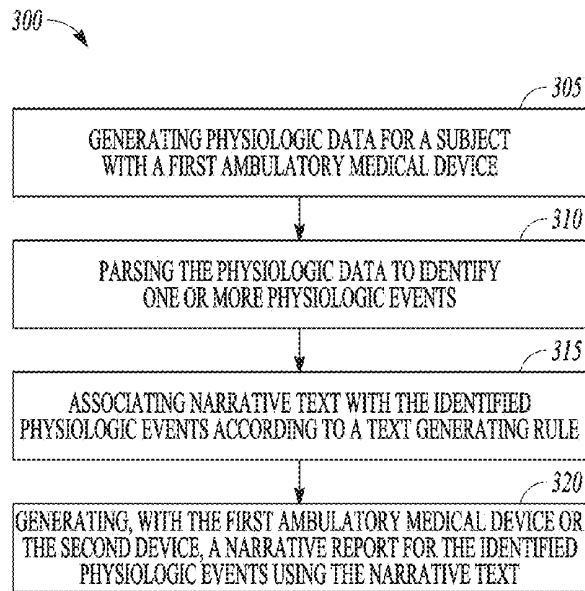


FIG. 3

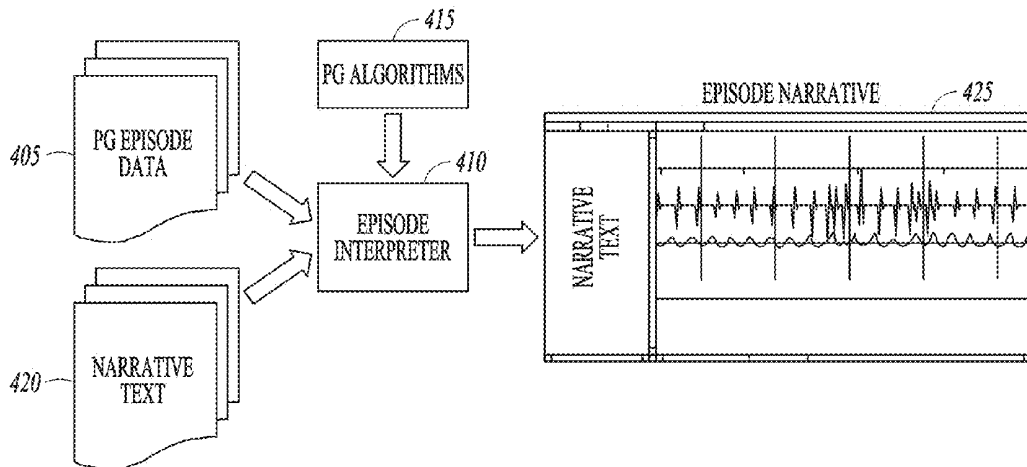


FIG. 4

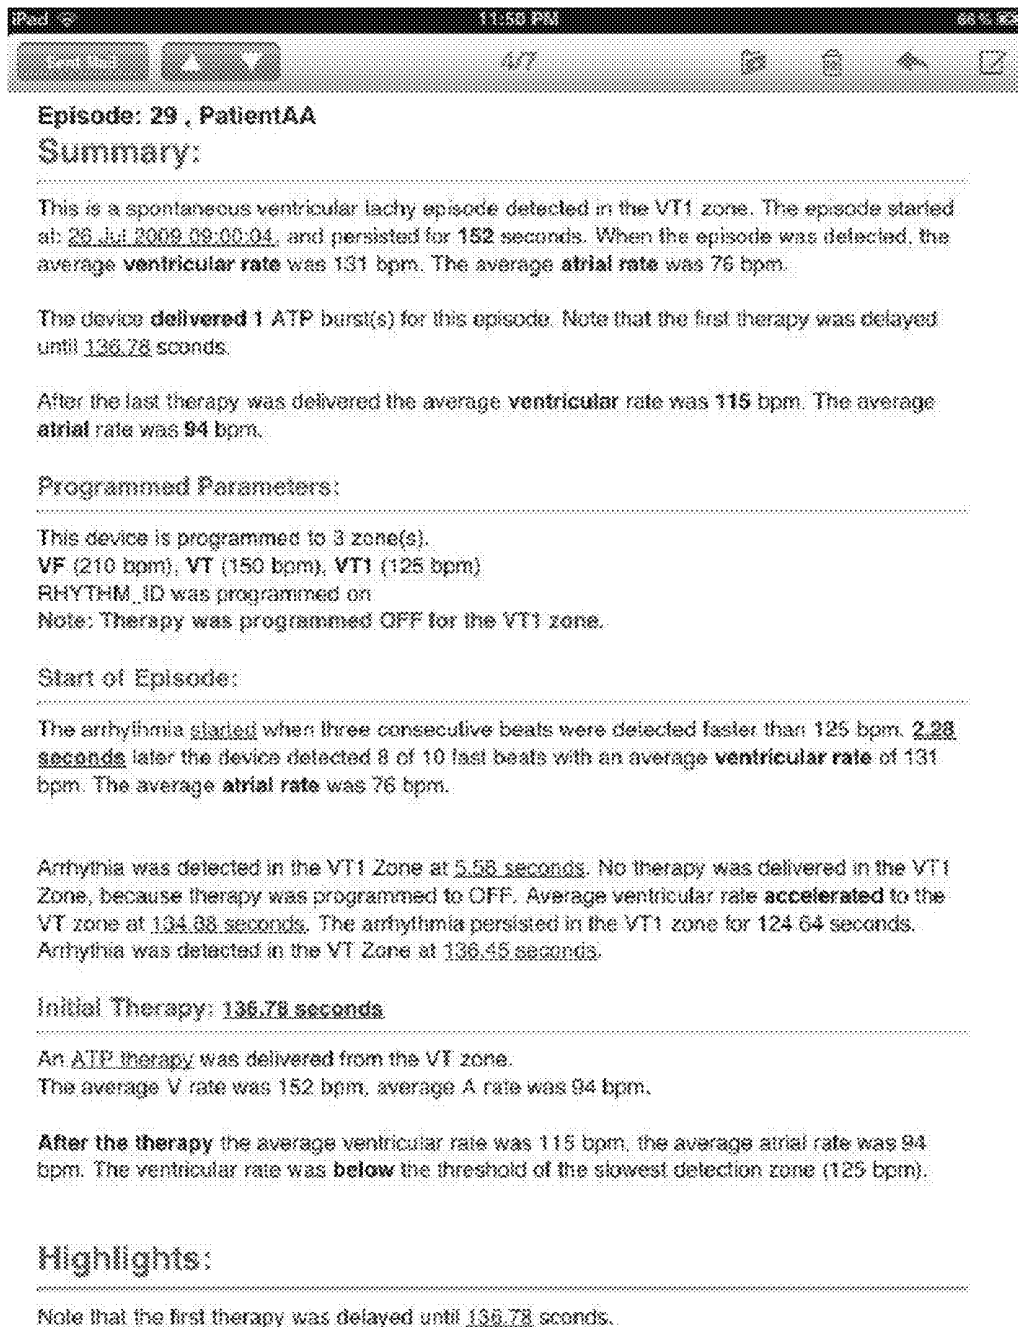
*FIG. 5*



FIG. 6

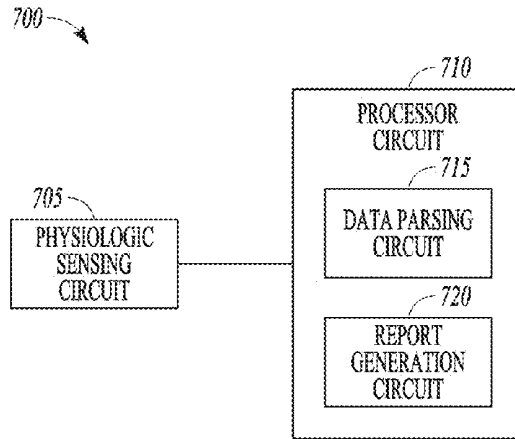


FIG. 7

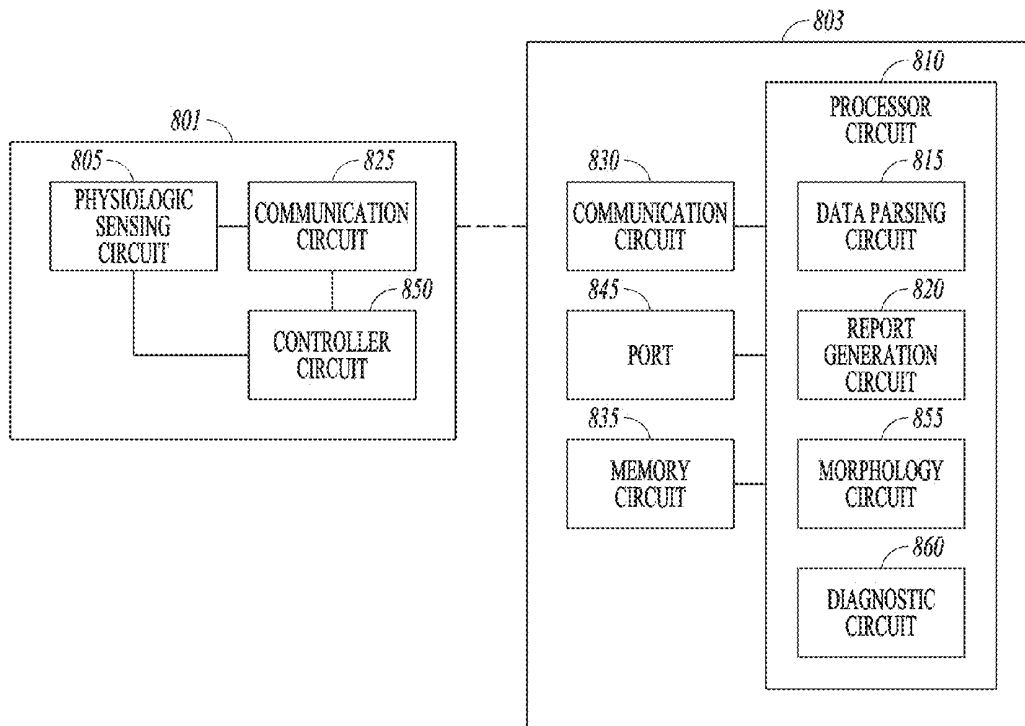


FIG. 8

		PROGRAMMED ENHANCEMENTS				
		1	2	3	4	5
		V>A = Off; Afb = Off; Slab = Off; CCT = Off	V>A = Off; Afb = Off; Slab = Off; CCT = On	V>A = Off; Afb = Off; Slab = On; CCT = Off	V>A = On; Afb = On; Slab = On; CCT = Off	V>A = On; Afb = On; Slab = On; CCT = On
CCT	Stability	A>Afb	V>A			
UnCrr	Unstable	T	F	TrAlways	TrUncorr	InUnstbl/Afb
UnCrr	Unstable	T	T	TrAlways	TrUncorr	TrV>A
UnCrr	Unstable	F	F	TrAlways	TrUncorr	TrNoMfb
UnCrr	Unstable	F	T	TrAlways	TrUncorr	TrV>A
UnCrr	Stable	T	F	TrAlways	TrSbl	TrIncorrSbl
UnCrr	Stable	T	T	TrAlways	TrUncorr	TrV>A
UnCrr	Stable	F	F	TrAlways	TrUncorr	TrSblOrNoMfb
UnCrr	Stable	F	T	TrAlways	TrUncorr	TrV>A
Corr	Unstable	T	F	TrAlways	InCrr	InUnstbl/Afb
Corr	Unstable	T	T	TrAlways	InCrr	TrV>A
Corr	Unstable	F	F	TrAlways	InCrr	InCrr
Corr	Unstable	F	T	TrAlways	InCrr	TrV>A
Corr	Stable	T	F	TrAlways	InCrr	InCrr
Corr	Stable	T	T	TrAlways	InCrr	TrV>A
Corr	Stable	F	F	TrAlways	InCrr	TrSblOrNoMfb
Corr	Stable	F	T	TrAlways	InCrr	TrV>A

FIG. 9A

THERAPY WAS INITIALLY INHIBITED WHEN <EnType> DECLARED THE DETECTED RHYTHM SVT BECAUSE...
 THERAPY WAS DELIVERED BECAUSE...

TAG	DESCRIPTION
InhAfib	AFIB WAS PRESENT.
InhCorr	IT MATCHED THE NORMAL SINUS TEMPLATE.
InhCorrOrUnstblAfib	IT MATCHED THE NORMAL SINUS TEMPLATE. THE PRESENCE OF AFIB COMBINED WITH THE UNSTABLE VENTRICULAR RHYTHM REINFORCED THE SVT RHYTHM DETERMINATION.
InhGrad	THE ARRHYTHMIA ONSET WAS GRADUAL.
InhGradNoAfib	THE ARRHYTHMIA ONSET WAS GRADUAL AND AFIB WAS NOT PRESENT.
InhGradOrUnstbl	THE ARRHYTHMIA ONSET WAS GRADUAL. THE UNSTABLE VENTRICULAR RHYTHM REINFORCED THE SVT RHYTHM DETERMINATION.
InhGradUnstbl	THE ARRHYTHMIA ONSET WAS GRADUAL AND THE VENTRICULAR RHYTHM WAS UNSTABLE.
InhUnstbl	THE VENTRICULAR RHYTHM WAS UNSTABLE.
InhUnstblAfib	THE VENTRICULAR RHYTHM WAS UNSTABLE AND AFIB WAS PRESENT.
InhUnstblOrGradNoAfib	THE VENTRICULAR RHYTHM WAS UNSTABLE. THE GRADUAL ARRHYTHMIA ONSET COMBINED WITH THE ABSENCE OF AFIB REINFORCED THE SVT RHYTHM DETERMINATION.
TrtAlways	THE VENTRICULAR RATE PERSISTED IN THE <ZONE> ZONE. THERAPY INHIBITORS WERE PROGRAMMED OFF.
TrtNoAfib	THE VENTRICULAR RATE PERSISTED IN THE <ZONE> ZONE AND AFIB WAS NOT PRESENT.
TrtStbl	THE VENTRICULAR RATE PERSISTED IN THE <ZONE> ZONE AND THE VENTRICULAR RHYTHM WAS STABLE.
TrtStblAfib	THE VENTRICULAR RATE PERSISTED IN THE <ZONE> ZONE, THE VENTRICULAR RHYTHM WAS STABLE, AND AFIB WAS PRESENT.
TrtOrNoAfib	THE VENTRICULAR RATE PERSISTED IN THE <ZONE> ZONE AND THE VENTRICULAR RHYTHM WAS STABLE. THE ABSENCE OF AFIB REINFORCED THE DECISION TO TREAT.
TrtSud	THE ARRHYTHMIA ONSET WAS SUDDEN AND THE VENTRICULAR RATE PERSISTED IN THE <ZONE> ZONE.
TrtSudNoAfib	THE ARRHYTHMIA ONSET WAS SUDDEN, THE VENTRICULAR RATE PERSISTED IN THE <ZONE> ZONE, AND AFIB WAS NOT PRESENT.
TrtSudNoStbl	THE VENTRICULAR RATE PERSISTED IN THE <ZONE> ZONE AND THE VENTRICULAR RHYTHM WAS STABLE. THE SUDDEN ARRHYTHMIA ONSET REINFORCED THE DECISION TO TREAT.
TrtSudStbl	THE ARRHYTHMIA ONSET WAS SUDDEN, THE VENTRICULAR RATE PERSISTED IN THE <ZONE> ZONE, AND THE VENTRICULAR RHYTHM WAS STABLE.
TrtSudStblOrStblAfib	THE ARRHYTHMIA ONSET WAS SUDDEN, THE VENTRICULAR RATE PERSISTED IN THE <ZONE> ZONE, AND THE VENTRICULAR RHYTHM WAS STABLE. THE PRESENCE OF AFIB WITH A STABLE VENTRICULAR RHYTHM REINFORCED THE DECISION TO TREAT.
TrtUncorr	THE VENTRICULAR RATE PERSISTED IN THE <ZONE> ZONE AND THE RHYTHM DID NOT MATCH THE NORMAL SINUS TEMPLATE.
TrtUncorrOrNoAfib	THE VENTRICULAR RATE PERSISTED IN THE <ZONE> ZONE AND THE RHYTHM DID NOT MATCH THE NORMAL SINUS TEMPLATE. THE ABSENCE OF AFIB REINFORCED THE DECISION TO TREAT.
TrtUncorrOrStbl	THE VENTRICULAR RATE PERSISTED IN THE <ZONE> ZONE AND THE RHYTHM DID NOT MATCH THE NORMAL SINUS TEMPLATE. THE STABLE VENTRICULAR RHYTHM REINFORCED THE DECISION TO TREAT.
TrtUncorrOrStblOrNoAfib	THE VENTRICULAR RATE PERSISTED IN THE <ZONE> ZONE AND THE RHYTHM DID NOT MATCH THE NORMAL SINUS TEMPLATE. THE STABLE VENTRICULAR RHYTHM AND THE ABSENCE OF AFIB REINFORCED THE DECISION TO TREAT.
TrtV>A	THE VENTRICULAR RATE PERSISTED IN THE <ZONE> ZONE AND THE VENTRICULAR RATE WAS FASTER THAN THE ATRIAL RATE.

FIG. 9B

DEFINING ACTION: APPLY ENHANCEMENTS IN CHART V EVENT HANDLER										DESCRIPTION
INPT										
ONSET ENABLED	ONSET GRADUAL	STABILITY INH ENABLED	AEB ENABLED	VGA ENABLED	CCT ENABLED	RYTHM UNSTABLE INH	STABILITY AND ONSET AEB IS PAST IV	GREATER AT CCT IS SIMILAR		
1	TRUE	FALSE				TRUE				THERAPY WAS INHIBITED BECAUSE...
2	FALSE									THE ARRHYTHMIA ONSET WAS GRADUAL.
3										THE VENTRICULAR RHYTHM WAS UNSTABLE.
4						TRUE				THE ARRHYTHMIA ONSET WAS GRADUAL.
5	TRUE		FALSE							THE VENTRICULAR RHYTHM WAS UNSTABLE.
6	FALSE						TRUE			THE ARRHYTHMIA ONSET WAS GRADUAL AND THE VENTRICULAR RHYTHM WAS UNSTABLE.
7						TRUE				THE ARRHYTHMIA ONSET WAS GRADUAL, THE VENTRICULAR RHYTHM WAS UNSTABLE, AND AEB WAS PRESENT.
8							FALSE			THE ARRHYTHMIA ONSET WAS GRADUAL, THE VENTRICULAR RHYTHM WAS UNSTABLE, AND AEB WAS NOT PRESENT.
9			TRUE	FALSE		TRUE				THE VENTRICULAR RHYTHM WAS UNSTABLE AND AEB WAS PRESENT.
10	TRUE									THE ARRHYTHMIA ONSET WAS GRADUAL.
11	FALSE					TRUE				THE VENTRICULAR RHYTHM WAS UNSTABLE.
12										THE ARRHYTHMIA ONSET WAS GRADUAL.
13										THE VENTRICULAR RHYTHM WAS UNSTABLE.
14	TRUE		FALSE							THE ARRHYTHMIA ONSET WAS GRADUAL AND THE VENTRICULAR RHYTHM WAS UNSTABLE.
15	FALSE						TRUE			THE VENTRICULAR RHYTHM WAS UNSTABLE AND AEB WAS PRESENT.
16						TRUE				THE VENTRICULAR RHYTHM WAS UNSTABLE.
17	TRUE				FALSE	FALSE				THE ARRHYTHMIA ONSET WAS GRADUAL, THE VENTRICULAR RHYTHM WAS UNSTABLE, AND AEB WAS NOT PRESENT.
18								TRUE		THE RHYTHM MATCHED THE NORMAL SINUS TEMPLATE.
19			TRUE	TRUE		TRUE		FALSE		THE VENTRICULAR RHYTHM WAS UNSTABLE AND AEB WAS PRESENT.
20	FALSE		FALSE		TRUE					THE RHYTHM MATCHED THE NORMAL SINUS TEMPLATE.

FIG. 10

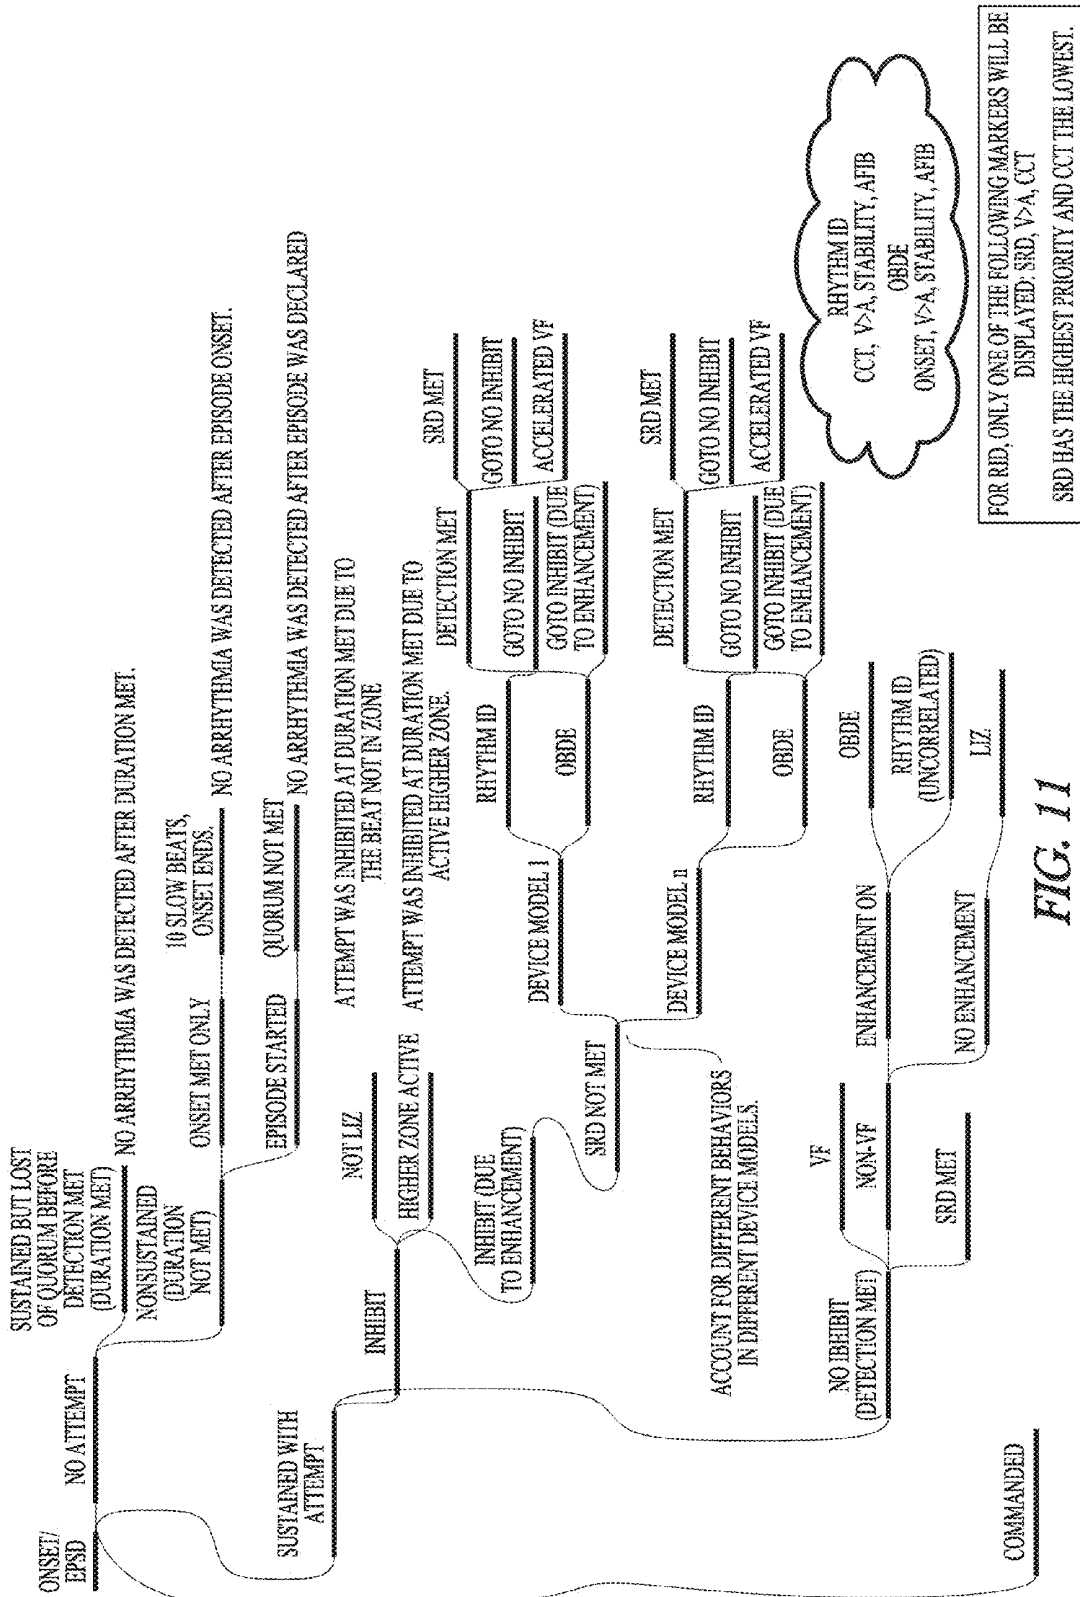


FIG. 11

ALGORITHM FOR NARRATIVE GENERATION

CLAIM OF PRIORITY

[0001] This application claims the benefit of priority under 35 U.S.C. §119(e) of Eberle et al., U.S. Provisional Patent Application Ser. No. 61/528,372, filed on Aug. 29, 2011, the benefit of priority of which is claimed hereby, and is incorporated by reference herein in its entirety.

BACKGROUND

[0002] Ambulatory medical devices include devices designed to be implanted into a patient. Some examples of these implantable medical devices (IMDs) include cardiac function management (CFM) devices such as implantable pacemakers, implantable cardioverter defibrillators (ICDs), cardiac resynchronization therapy devices (CRTs), and devices that include a combination of such capabilities. The devices can be used to treat patients or subjects using electrical or other therapy or to aid a physician or caregiver in patient diagnosis through internal monitoring of a patient's condition. The devices may include one or more electrodes in communication with one or more sense amplifiers to monitor electrical heart activity within a patient, and often include one or more sensors to monitor one or more other internal patient parameters. Other examples of IMDs include implantable diagnostic devices, implantable drug delivery systems, or implantable devices with neural stimulation capability.

[0003] Ambulatory medical devices also include wearable medical devices (WMDs) such as wearable cardioverter defibrillators (WCDs). WCDs are monitors that include surface electrodes. The surface electrodes are arranged to provide one or both of monitoring surface electrocardiograms (ECGs) and delivering cardioverter and defibrillator shock therapy.

[0004] Data collected by an ambulatory medical device can be used to generate a report on the health of the patient. Some ambulatory medical devices are designed to communicate information to a second separate device that generates the report. For example, an implantable device typically communicates information wirelessly to an external device. If the device is wearable, the report can be generated by the ambulatory device itself.

[0005] Because the amount of available storage in an ambulatory medical device may be limited, information collected by the ambulatory medical device may be limited to simple data entry form. Reports generated from the collected data may be difficult for the reader to comprehend.

Overview

[0006] This document relates generally to systems, devices, and methods that provide therapy to a patient or subject. In particular it relates to, systems, devices, and methods for automatic report generation by such devices.

[0007] A system example includes a physiologic sensing circuit configured to generate physiologic data for a subject and a processing circuit. The processing circuit includes a data parsing circuit configured to parse the physiologic data to identify one or more physiologic events and a report generation circuit. The report generation circuit is configured to associate narrative text with the identified physiologic events

according to a text generating rule and generate a narrative report for the identified physiologic events using the narrative text.

[0008] This section is intended to provide an overview of subject matter of the present patent application. It is not intended to provide an exclusive or exhaustive explanation of the invention. The detailed description is included to provide further information about the present patent application.

BRIEF DESCRIPTION OF THE DRAWINGS

[0009] In the drawings, which are not necessarily drawn to scale, like numerals may describe similar components in different views. Like numerals having different letter suffixes may represent different instances of similar components. The drawings illustrate generally, by way of example, but not by way of limitation, the various examples discussed in the present document.

[0010] FIG. 1 is an illustration of an example of portions of a system that uses an ambulatory medical device.

[0011] FIG. 2 is an illustration of portions of another system that uses an ambulatory medical device.

[0012] FIG. 3 is a flow diagram of an example of a method of automatically generating a narrative report using a medical device.

[0013] FIG. 4 shows an example of process flow to generate a narrative report.

[0014] FIG. 5 shows an example of narrative text for a narrative report.

[0015] FIG. 6 shows an example of narrative text for a narrative report in a language different from the example in FIG. 5.

[0016] FIG. 7 is a block diagram of an example of portions of an electronic system for generating a narrative report that explains physiologic events of a subject.

[0017] FIG. 8 is a block diagram of another example of portions of an electronic system for generating a narrative report.

[0018] FIGS. 9A-9B show portions of an example of a lookup table.

[0019] FIG. 10 shows a portion of an example of a set of logic rules.

[0020] FIG. 11 shows portions of an example of a decision tree.

DETAILED DESCRIPTION

[0021] An ambulatory medical device (e.g., an IMD or WMD) can include one or more of the features, structures, methods, or combinations thereof described herein. For example, a cardiac monitor or a cardiac stimulator may be implemented to include one or more of the advantageous features or processes described below. Such a device may be implemented to provide a variety of therapeutic or diagnostic functions.

[0022] FIG. 1 is an illustration of an example of portions of a system that uses an IMD 110 or other ambulatory medical device that can be capable of moving about with the subject, such as chronically during activities of daily living. Examples of IMD 110 include, without limitation, a pacemaker, a defibrillator, a cardiac resynchronization therapy (CRT) device, or a combination of such devices. The system 100 also typically includes an IMD programmer or other external

device **170** that communicates wireless signals **190** with the IMD **110**, such as by using radio frequency (RF) or other telemetry signals.

[0023] The IMD **110** can be coupled by one or more leads **108A-C** to heart **105**. Cardiac leads **108A-C** include a proximal end that is coupled to IMD **110** and a distal end, coupled by electrical contacts or “electrodes” to one or more portions of a heart **105**. The electrodes typically deliver cardioversion, defibrillation, pacing, or resynchronization therapy, or combinations thereof to at least one chamber of the heart **105**. The electrodes may be electrically coupled to sense amplifiers to sense electrical cardiac signals.

[0024] Sensed electrical cardiac signals can be sampled to create an electrogram. An electrogram can be analyzed by the IMD and/or can be stored in the IMD and later communicated to an external device where the sampled signals can be displayed for analysis.

[0025] Heart **105** includes a right atrium **100A**, a left atrium **100B**, a right ventricle **105A**, a left ventricle **105B**, and a coronary sinus **120** extending from right atrium **100A**. Right atrial (RA) lead **108A** includes electrodes (electrical contacts, such as ring electrode **125** and tip electrode **130**) disposed in an atrium **100A** of heart **105** for sensing signals, or delivering pacing therapy, or both, to the atrium **100A**.

[0026] Right ventricular (RV) lead **108B** includes one or more electrodes, such as tip electrode **135** and ring electrode **140**, for sensing signals, delivering pacing therapy, or both sensing signals and delivering pacing therapy. Lead **108B** optionally also includes additional electrodes, such as for delivering atrial cardioversion, atrial defibrillation, ventricular cardioversion, ventricular defibrillation, or combinations thereof to heart **105**. Such electrodes typically have larger surface areas than pacing electrodes in order to handle the larger energies involved in defibrillation. Lead **108B** optionally provides resynchronization therapy to the heart **105**. Resynchronization therapy is typically delivered to the ventricles in order to better synchronize the timing of depolarizations between ventricles.

[0027] The IMD **110** can include a third cardiac lead **108C** attached to the IMD **110** through the header **155**. The third cardiac lead **108C** includes electrodes **160** and **165** placed in a coronary vein lying epicardially on the left ventricle (LV) **105B** via the coronary vein. The third cardiac lead **108C** may include anywhere from two to eight electrodes, and may include a ring electrode **185** positioned near the coronary sinus (CS) **120**.

[0028] Lead **108B** can include a first defibrillation coil electrode **175** located proximal to tip and ring electrodes **135**, **140** for placement in a right ventricle, and a second defibrillation coil electrode **180** located proximal to the first defibrillation coil **175**, tip electrode **135**, and ring electrode **140** for placement in the superior vena cava (SVC). In some examples, high-energy shock therapy is delivered from the first or RV coil **175** to the second or SVC coil **180**. The combination of electrodes used in shock therapy is sometimes called a shock channel or shock vector because the combination of electrodes can result in delivery of therapy in a particular direction. In some examples, the SVC coil **180** is electrically tied to an electrode formed on the hermetically-sealed IMD housing or can **150**. This improves defibrillation by delivering current from the RV coil **175** more uniformly over the ventricular myocardium. In some examples, the therapy is delivered from the RV coil **175** only to the electrode formed on the

IMD can **150**. In some examples, the coil electrodes **175**, **180** are used in combination with other electrodes for sensing signals.

[0029] Note that although a specific arrangement of leads and electrodes are shown the illustration, an IMD can be configured with a variety of electrode arrangements, including transvenous, endocardial, and epicardial electrodes (i.e., intrathoracic electrodes), and/or subcutaneous, non-intrathoracic electrodes, including can, header, and indifferent electrodes, and subcutaneous array or lead electrodes (i.e., non-intrathoracic electrodes). The present methods and systems will work in a variety of configurations and with a variety of electrodes. Other forms of electrodes include meshes and patches which can be applied to portions of heart **105** or which can be implanted in other areas of the body to help “steer” electrical currents produced by IMD **110**.

[0030] FIG. 2 is an illustration of portions of another system **200** that uses an IMD **210** to provide a therapy to a patient **202**. The system **200** typically includes an external device **270** that communicates with a remote system **296** via a network **294**. The network **294** can be a communication network such as a phone network or a computer network (e.g., the internet). In some examples, the external device includes a repeater and communicated via the network using a link **292** that may be wired or wireless. In some examples, the remote system **296** provides patient management functions and may include one or more servers **298** to perform the functions.

[0031] As noted previously, episode history reports can be automatically generated using information collected by ambulatory medical devices. The reports can include a history of one or more health-related episodes of the patient. These episodes can involve physiologic events experienced by the patient during a time period of interest. Physiologic data can be collected during the episode by the ambulatory device using sensors incorporated into the device or using sensors in signal communication with the device.

[0032] However, a clinician may have difficulty in comprehending these episode history reports. For instance, the clinician may have difficulty relating the episode data to the algorithms performed by the device, or the clinician may have difficulty in determining the relationships of several physiologic events that occur during one or more of the episodes. This may result in the clinician having difficulty in tailoring parameters to the patient, in mistakes being made in programming the ambulatory medical device, and in inappropriate therapy being provided to the patient.

[0033] It would be desirable for the automatic report to include a narrative description or a natural language description of episode histories based on the data collected by the ambulatory medical device. This natural language can be language a clinician would use to express physiologic events of the patient, rather than a report with device-based terms and abbreviations. A report in narrative form can improve a clinician’s understanding of decisions made by the ambulatory medical device and interactions of the features of the device. This can improve the tailoring of the device to the patient and may reduce inappropriate therapy.

[0034] FIG. 3 is a flow diagram of an example of a method **300** of automatically generating a narrative report using a medical device. The narrative report can be a narrative language description of events related to the health of the patient or subject. At block **305**, physiologic data for the subject is generated with a first ambulatory medical device. At block

310, the physiologic data is parsed to identify one or more physiological events of the subject.

[0035] The ambulatory medical device can be a wearable device such as a WCD, or a wearable monitoring device. In this case, the data can be parsed by the ambulatory medical device. If the ambulatory medical device is an implantable medical device, such as an ICD or pacemaker, the physiological data can be collected by the ambulatory medical device and communicated to a separate device, such as a device programmer or a repeater. A repeater can then pass the data on to a network such as a computer network or a cellular phone network to be received by a server or cell phone. The data can then be parsed by the programmer, server, or an application on the cell phone.

[0036] In some examples, the ambulatory medical device includes a cardiac signal sensing circuit and the physiologic data to be parsed can include electrograms and markers associated with the electrograms. If the ambulatory medical device includes an accelerometer or other motion sensor, the physiologic data can include patient activity data. If the ambulatory medical device includes a respiration sensor, the physiologic data can include respiratory data. Other examples include heart sound data and intracardiac and transthoracic impedance data.

[0037] The physiologic event can be events related to the hemodynamic function of the subject. Examples of physiologic events include, among other things, a change in heart rate, an episode of an abnormally slow heart rate or bradycardia, and an episode of an abnormally fast heart rate or tachyarrhythmia. Tachyarrhythmia includes ventricular tachycardia (VT) which originates from the ventricles. Tachyarrhythmia also includes rapid and irregular heart rate, or fibrillation, including ventricular fibrillation (VF). Abnormally rapid heart rate can also be due to supraventricular tachycardia (SVT). SVT includes arrhythmias such as atrial tachycardia, atrial flutter, and atrial fibrillation. Other examples of physiologic events include an episode of ischemia, a change in status of heart failure (HF) of the patient, and sinus tachycardia. Sinus tachycardia or ST is a normal response to exercise or an elevated emotional state for example. If the ambulatory medical device provides therapy to the patient, the physiologic event can be therapy delivered to the patient in response to the detected bradycardia, tachyarrhythmia, ischemia, and change in HF.

[0038] At block **315**, narrative text is associated with the identified physiologic events according to a text generating rule. The text generating rule can include, among other things, a decision tree, a lookup table, or a specified set of logic rules. At block **320**, a narrative report for the identified physiologic events is generated using the narrative text. The narrative report can be generated with the ambulatory medical device or a second separate device.

[0039] FIG. 4 shows an example of process flow to generate a narrative report. In the example, physiologic episode data **405** is collected using a pulse generator (PG) such as a pacemaker, cardioverter/defibrillator, or combination pacemaker cardioverter/defibrillator. The episode data **405** is communicated (e.g., by wireless telemetry) to a separate device having an episode interpreter **410**. The episode interpreter **410** parses the episode data to identify physiologic events in the data. The episode interpreter **410** may also receive information as to the type of PG and may use information related to the type or types of algorithms **415** performable by the PG type in identifying the physiologic events. For example, the episode inter-

preter **410** may determine from the PG type that the PG uses a tachyarrhythmia detection enhancement to rate zone detection, such as ventricular rate being greater than the atrial rate ($V_{rate} > A_{rate}$) for example. The episode interpreter **410** may parse the episode data for V_{rate} being greater than A_{rate} before interpreting an event as tachyarrhythmia.

[0040] The episode interpreter **410** then pulls in narrative text **420** to form into a report that is a narrative of the episode **425**. The narrative text **420** may include text strings that correspond to events identified during the parsing of data. Some examples of text strings are shown below in Table 1. The text strings are accumulated and formatted to generate a narrative of the episode **425**.

[0041] As shown in the example, the narrative of the episode **425** can include graphical representations of the physiologic data. Narrative text for the episode or episodes is shown displayed to the left of the graphical representation. The narrative report can be displayed on the separate device, sent to a printer to generate a printout of the narrative, or saved to a file (e.g., a disk or a *.pdf) for later access and viewing or for including the narrative report in electronic mail (e-mail).

[0042] FIG. 5 shows an example of narrative text for a narrative report. Note that the first paragraph of the report explains in narrative language that the patient experienced an episode of ventricular tachycardia, instead of merely providing a marker in the graphical portion for VT. In some examples the text and graphical representations are interactive. For instance, the text can include a time or an event in the episode and clicking on the text for the time or event changes the graphical representation or an indication on the graphical representation to the specified time or event. As shown in the text example of FIG. 5, clicking on the text for "started" may change the graphical representation to show the arrhythmia start while clicking on the time text "136.78" seconds changes the graphical representation to 136.78 seconds after the episode start.

[0043] FIG. 6 shows an example of narrative text for a narrative report in a language different from the example in FIG. 5. The device generating the report may include selectable screen options for generating the narrative report in different languages.

[0044] FIG. 7 is a block diagram of an example of portions of an electronic system for generating a narrative report that explains physiologic events of a subject. The system **700** includes a physiologic sensing circuit **705** and a processor circuit **710**. The physiologic sensing circuit **705** generates physiologic data associated with the subject. The processor circuit **710** can include a microprocessor, a digital signal processor, application specific integrated circuit (ASIC), or other type of processor, interpreting or executing instructions in software modules or firmware modules. The processor circuit **710** includes other circuits or sub-circuits to perform the functions described. These circuits may include software, hardware, firmware or any combination thereof. Multiple functions can be performed in one or more of the circuits or sub-circuits as desired.

[0045] The processor circuit **710** includes a data parsing circuit **715** and a report generation circuit **720**. The data parsing circuit **715** parses the physiologic data to identify one or more physiologic events. The report generation circuit **720** associates narrative text with the identified physiologic events according to a text generating rule, and generates a narrative report for the identified physiologic events using the narrative text.

[0046] According to some examples, the physiologic sensing circuit 705 and the processor circuit 710 are included in the same medical device, such as a wearable medical device. The physiologic sensing circuit 705 can include skin surface electrodes to obtain ECG data. The data parsing circuit 715 can parse the ECG data to identify cardiac depolarizations. Using the identified depolarizations, the data parsing circuit 715 can identify heart rate and cardiac arrhythmias such as tachyarrhythmia and bradycardia. In some examples, the physiologic sensing circuit 705 can include a respiration sensor to detect motion (such as by an accelerometer for example) of the chest cavity of the subject to detect breathing of the subject and generate respiration data. The data parsing circuit 715 may parse the ECG data and respiration data to determine an HF status of the subject.

[0047] According to some examples, the physiologic sensing circuit and the processor circuit are included in separate medical devices. FIG. 8 is a block diagram of another example of portions of an electronic system for generating a narrative report. The system 800 includes a first ambulatory medical device 801 and a second device 803. The ambulatory medical device 801 includes a physiologic sensing circuit 805 that generates physiologic data for a subject, and a communication circuit 825 to communicate the physiologic data wirelessly to a separate device.

[0048] The second device 803 includes a communication circuit 830 to receive the physiologic data and a processor circuit 810. The processor circuit 810 includes a data parsing circuit 815 and a report generation circuit 820. In certain examples, the second device 803 can be a programmer for the ambulatory medical device 801. In certain examples, the second device 803 can be a laptop computer, tablet computer, or cell phone, and the report generation circuit 820 may execute an application to generate a narrative report.

[0049] In some examples, physiologic data is received by the second device 803 from a third device (e.g., another ambulatory medical device or a server). The data parsing circuit 815 is configured to associate physiologic data from the third device with the physiologic data communicated from the ambulatory medical device, and the report generation circuit 820 is configured to associate narrative text with the identified physiologic events and the associated physiologic data.

[0050] The report generation circuit 820 includes a text generating rule to associate narrative text to the physiologic data collected by the physiologic sensing circuit 805 of the ambulatory medical device 801. In some examples, the text generating rule includes a lookup table. Entries of the lookup table can be linked to narrative text. The lookup table may be stored in a memory circuit 835 that can be integral to the processor circuit 810 or can be communicatively coupled to the processor circuit 810. The communicative coupling allows the processor to communicate with the memory even though there may be intervening circuitry.

[0051] FIGS. 9A-9B show portions of an example of a lookup table used to associate narrative text to the physiologic data. The portion of the lookup table in FIG. 9A is used to determine a tag that is then used as an index or link to narrative text, such as the portion of narrative text shown in FIG. 9B. In the example, the ambulatory medical device 801 is an ICD and includes the physiologic sensing circuit 805 includes a cardiac signal sensing circuit. Rows of the table in FIG. 9A correspond to characteristics of a detected heart rhythm in the sensed physiologic data. The characteristics can be deter-

mined by the data parsing circuit 815. In some examples, the data parsing circuit 815 can be included in the ambulatory medical device 801 and the determined characteristics of the detected rhythm are communicated to the second device 803.

[0052] The columns for the detected rhythm correspond to detection enhancements to rate-based detection for an ICD. The columns indicate whether the rhythm during an episode correlated to a template rhythm, whether the rhythm was stable or unstable, whether the atrial rate (A) was greater than a threshold rate used to detect atrial fibrillation (Afib), and whether the ventricular rate (V) was greater than the atrial rate.

[0053] The table in FIG. 9A also includes columns that correspond to the detection enhancements being programmed "on" or "off." Thus, the narrative text can indicate a relationship between events detected in the heart rhythm and programmed parameters of the ambulatory medical device 801. For instance, if the rhythm is uncorrelated, is unstable, the atrial rate indicates atrial fibrillation, and the ventricular rate is not greater than the atrial rate, the first row of the table results in the "TrtAlways" (treat always, or initiate therapy) tag being selected if all of the detection enhancements are programmed off. If the stability enhancement is programmed "on" (the third programmed enhancements column), the first row of the table results in the "InhUnstbl" (inhibit unstable) tag being selected.

[0054] A selected tag is then indexed into the table of FIG. 9B. The tags in bold indicate a case where a decision by an ambulatory medical device (e.g., the ambulatory medical device 801 in FIG. 8) results in therapy (e.g., cardioversion or defibrillation) being delivered by the medical device, and tags in non-bold correspond to a decision that results in therapy being inhibited. The selected tags can then index text that can be linked with the narrative text at the top of the table in FIG. 9B. For the TrtAlways tag, the narrative text string "Therapy was delivered because the ventricular rate persisted in the <zone> zone. Therapy inhibitors were programmed Off;" is generated using the lookup table. The text field <zone> would include text to indicate a tachyarrhythmia zone that included the detected rate, such as ventricular tachycardia ("VT zone") or ventricular fibrillation ("VF zone") for example. For the InhUnstbl tag, the narrative text string "Therapy was initially inhibited when Stability declared the detected rhythm SVT because the ventricular rhythm was unstable;" is generated using the lookup table.

[0055] In some examples, the text generating rule includes a specified set of logic rules. Narrative text is linked to the results or outcome of the logic rules. FIG. 10 shows a portion of an example of a set of logic rules used to associate narrative text to the physiologic data. In the example shown, the logic rules are shown in the form of a table. In certain examples, the logic rules can be implanted as a series of IF-THEN statements. In the example in the Figure, the logic rules include an indication (e.g., true or false) of whether a certain condition is detected in the physiologic data. In some examples, the logic rules also include indications of whether certain parameters are programmed on or off in the ambulatory medical device. The logic rule in the first row of the Figure is valid when the onset detection enhancement is enabled, the detected onset of the rhythm was gradual, and the detection enhancements for stability, atrial fibrillation, V rate greater than A rate, and correlation were all disabled or programmed off. When the logic rule of the row is valid, the narrative text string "Therapy

was inhibited because the arrhythmia onset was gradual,” (as shown in the right column) is generated using the logic rules.

[0056] In some examples, the text generating rule can be a decision tree and the report generation circuit **820** associates narrative text with the identified physiologic events according to at least the decision tree. FIG. **11** shows portions of an example of a decision tree used to associate narrative text to the physiologic data. The example shown corresponds to a portion in which an onset of an episode of tachyarrhythmia is detected in the physiologic data. The three main branches of the decision tree shown correspond to the ambulatory medical device making no attempt to convert the rhythm of the detected episode, to the episode being sustained after an attempt to convert the episode, and an attempt to convert the episode as a result of a command received by the ambulatory medical device.

[0057] Nodes of the decision tree are linked to narrative text. For instance, for the second sub-branch from the top of the Figure, if no attempt was made by the ambulatory medical device to convert the rhythm because the duration was not sustained (SRD not met), the detection requirement for onset was the only requirement met, and onset was declared ended after ten slow beats, the narrative text “No arrhythmia was detected after the episode onset was detected” is associated to the identified physiologic event (of tachyarrhythmia onset) using the decision tree. In another example, if the onset episode was sustained after a conversion attempt, but a subsequent conversion attempt was inhibited due to the last heart beat not being in the detection for delivery of therapy (not LIZ), then the narrative text “Attempt was inhibited at duration met due to a beat not being in the detection zone” is associated to the identified physiologic event using the decision tree.

[0058] The narrative text may be included in the decision tree itself (e.g., at the end of the sub-branches) or the decision tree may include links to narrative text in a stored table, such as narrative text shown in Table 1. The portion of the decision tree in the example also shows how useful a narrative report can be to a clinician. The generated narrative report explains events in plain language rather than in terms of industry jargon such as LIZ (Last beat was In the detection Zone to deliver therapy), SRD (sustained rhythm duration) met, or OBDE (one button detection enhancement) enabled.

[0059] In some examples, at least a portion of the text generating rule is specific to a model type of the ambulatory medical device. For instance, the decision tree portion in FIG. **11** shows sub-branches specific to capabilities of Device Model **1** through Device Model **n**. In FIG. **9A**, portions of the lookup table can correspond to specific device model types, and in FIG. **10**, a logic rule can include an entry for a device model type (e.g., Device Model **1**=true or false).

[0060] Returning to FIG. **8**, in some examples the ambulatory medical device **801** includes a controller circuit **850**. The controller circuit **850** can be a processor circuit or the controller circuit **850** can be a sequencer. A sequencer refers to a state machine or other circuit that sequentially steps through a fixed series of steps to perform one or more functions. The steps are typically implemented in hardware or firmware. The controller circuit **840** initiates communication of one or more indications of a decision or adjudication, made by the ambulatory medical device **801**, in association with the physiologic data.

[0061] The report generation circuit **820** associates narrative text with the decision indications and generates a narra-

tive report for the identified one or more physiologic events and the indications of decisions made by the first medical device using the narrative text. For instance, the data parsing circuit **815** may identify an episode of ventricular tachyarrhythmia using (e.g., by parsing) the physiologic data. The report generation circuit **820** is configured to include, in the generated narrative report, an indication of a decision whether to treat the episode of ventricular tachyarrhythmia using device-based therapy. For example, the report generation circuit **820** may include the lookup table of table of FIG. **9B** and indicate in the narrative text a device-based decision as to whether therapy was delivered or inhibited and the reason or reasons why. In another example, the report generation circuit **820** may include an implementation of the decision tree of FIG. **11** and indicate in the narrative text whether therapy was attempted or inhibited according to the branches of the decision tree.

[0062] In some examples, the second device **803** receives a rationale for the adjudication or decision made by the first ambulatory medical device **801** in association with the communicated physiologic data. The report generation circuit **820** associates narrative text with the rationale for the adjudication or decision, and generates, using the narrative text, a narrative report according to the identified physiologic events, the indication of the adjudication, and the rationale for the adjudication or decision.

[0063] In some examples, the report generation circuit **820** relates a decision made by the first ambulatory medical device to a specified device parameter setting that influenced the decision. For instance, the communicated physiologic data may include the results of one or more tachyarrhythmia detection enhancements of the first ambulatory medical device. In certain examples, the data can include indications of whether the specific detection enhancements were enabled during a detected tachyarrhythmia episode. The report generation circuit **820** is configured to associate narrative text with the results and include the narrative text in the generated narrative report. Examples of detection enhancements for correlation, rhythm stability, atrial rate, and ventricular rate greater than atrial rate are shown in the examples, FIGS. **9A**, **9B**, **10**, and **11**.

[0064] In some examples, the data parsing circuit **815** may identify an episode of bradycardia using the physiologic data. The report generation circuit **820** includes, in the generated narrative report, an indication of a decision whether to treat the episode of bradycardia using device-based therapy.

[0065] As explained previously, the physiologic sensing circuit **805** can include a cardiac signal sensing circuit to generate the physiologic data. In some examples, the physiologic sensing circuit **805** includes a heart sound sensing circuit. Heart sounds are associated with mechanical vibrations from activity of a patient’s heart and the flow of blood through the heart. Heart sounds recur with each cardiac cycle and are separated and classified according to the activity associated with the vibration. The first heart sound (S1) is the vibrational sound made by the heart during tensing of the mitral valve. The second heart sound (S2) marks the beginning of diastole. The third heart sound (S3) and fourth heart sound (S4) are related to filling pressures of the left ventricle during diastole.

[0066] A heart sound sensing circuit produces an electrical signal which is representative of mechanical activity of a patient’s heart. Regional shortening causes changes in the heart sounds detectable with a heart sound sensor. A descrip-

tion of systems and methods for sensing wall motion is found in the commonly assigned, U.S. patent application Ser. No. 11/135,985, now U.S. Pat. No. 7,424,321, entitled "Systems and Methods for Multi-Axis Cardiac Vibration Measurements," filed May 24, 2005, which is incorporated herein by reference in its entirety. The physiologic data can include heart sound data. The data parsing circuit **815** may parse the heart sound data to detect an episode of myocardial ischemia. The report generation circuit **820** may associate narrative text with an indication of ischemia and may indicate a device-based decision based on the detection of ischemia, such as initiating a regimen of protection pacing for example.

[0067] In some examples, the physiologic sensing circuit **805** includes a cardiac impedance sensing circuit. Cardiac impedance changes measure changes in chamber volumes. Regional changes in cardiac relaxation may be measured using measurements of cardiac impedance using an impedance sensing circuit. Similarly, the strength of contraction may be inferred from changes in the rate of decrease of cardiac impedance during cardiac contraction. Systems and methods to measure intracardiac impedance are described in Citak et al., U.S. Pat. No. 4,773,401, entitled "Physiologic Control of Pacemaker Rate Using Pre-Ejection Interval as the Controlling Parameter," filed Aug. 21, 1987, which is incorporated herein by reference in its entirety. The data parsing circuit **815** may parse cardiac impedance data to detect an episode of ischemia and the report generation circuit **820** may associate narrative text with one or more an indication of the ischemia a device-based decision based on the detection of ischemia.

[0068] In some examples, the physiologic sensing circuit **805** includes a physical activity sensing circuit, such as an accelerometer for example, to provide a signal representative of activity of the subject. The report generation circuit **820** may associate narrative text with an indication of patient activity and may indicate a device-based decision based on determined activity of the patient, such as an increase in paced heart rate for example.

[0069] In some examples, the physiologic sensing circuit **805** includes a respiration sensing circuit to provide a signal representative of respiration of the subject. An example of an implantable respiration sensor is a transthoracic impedance sensor to measure minute respiration volume. An approach to measuring transthoracic impedance is described in Hartley et al., U.S. Pat. No. 6,076,015, "Rate Adaptive Cardiac Rhythm Management Device Using Transthoracic Impedance," filed Feb. 27, 1998, which is incorporated herein by reference in its entirety. The physiologic data can include respiration data such as breathing tidal volume for example. The data parsing circuit **815** may use one or more of respiration data, physical activity data, and cardiac depolarization data to determine a change in HF status of the subject. The report generation circuit **820** may associate narrative text with an indication of the change in HF status of the patient as well as any device-based decision based on the HF status, such as a change in resynchronization pacing therapy for example.

[0070] In some examples, the data parsing circuit **815** provides an adjudication of a physiologic event. For instance, the data parsing circuit **815** may identify cardiac arrhythmia (e.g., an episode of bradycardia or tachyarrhythmia) from the physiologic data and the report generation circuit **820** associates narrative text with the adjudicated event.

[0071] In some examples, the second device **803** includes a port **845**. In some examples, the port **845** includes a commu-

nication port or "comm" port to receive information from a third device. In certain examples the port is a wired interface (e.g., a Universal Serial Bus or USB), and in certain examples the port **845** is a wireless interface. In some examples, the port **845** includes a user interface to receive information entered by a user. The second device **803** may receive an indication of adjudication of an identified physiologic event via the port **845**. The report generation circuit **820** is configured to change the content of the generated narrative report, or the amount of detail in the generated narrative report, related to the identified physiologic event based on the received adjudication.

[0072] For instance, the data parsing circuit **815** may identify a physiologic event in the physiologic data as SVT. The second device **803** may receive an indication of adjudication related to the episode of SVT and the report generation circuit **820** changes an amount of detail in the generated narrative report related to SVT detection enhancements. The adjudication may be received from a separate device or via a user interface. In another example, the data parsing circuit **815** may identify a physiologic event in the physiologic data as VT and an indication of adjudication of the episode is received via the port **845** that the episode is SVT. The report generation circuit **820** changes the content of the narrative report accordingly.

[0073] In some examples, the physiologic sensing circuit **805** produces samples of a sensed physiologic signal as at least a portion of the physiologic data. The physiologic sensing circuit **805** may include a sampling circuit to generate digital valued samples of one or more of a sensed cardiac signal, a heart sound signal, a respiration signal, an impedance signal, or an activity signal. The port **845** may receive an indication (e.g., via a user interface) of a specified segment of the sensed and sampled physiologic signal for which to generate the narrative report.

[0074] In some examples, the second device **803** includes a display (not shown) to display a graphical representation of physiologic data such as is shown in FIG. 4. For instance, the physiologic sensing circuit **805** may include a cardiac signal sensing circuit. The ambulatory medical device **801** may include a controller circuit **850** that recurrently initiates sensing of electrograms using the cardiac signal sensing circuit. The report generation circuit **820** can incorporate a graphical representation of a comparison of two or more sensed electrograms in the generated narrative report. In certain examples, the report generation circuit **820** incorporates a graphical representation of one or more of one or more of a sensed cardiac signal, a heart sound signal, a respiration signal, an impedance signal, or an activity signal in the generated narrative report. The generated narrative report can be displayed, communicated to a printer to generate a printout of the narrative, or saved to a file for later access and viewing or for including the narrative report in e-mail.

[0075] According to some examples, the data parsing circuit **815** is able to determine a relationship between multiple identified physiologic events according to determined attributes of the physiologic events. In some examples, the data parsing circuit **815** is able to identify physiologic events of the same type. For example, the processor circuit **810** can include a morphology circuit **855** that identifies physiologic events for a subject using the communicated physiologic data, and compares morphology of the physiologic events. In certain examples, the morphology circuit **855** compares sensed cardiac signals to identify physiologic events of the same type. Descriptions of systems to identify physiologic

events using signal morphology can be found in Hsu et al., U.S. Pat. No. 6,438,410, "System and Method for Classifying Cardiac Complexes," filed May 3, 2001, which is incorporated herein by reference in its entirety.

[0076] The data parsing circuit **815** can identify the physiologic events having the same type and the report generation circuit **820** can include narrative text related to a result of the morphology comparison in the generated narrative report. In some examples, the data parsing circuit **815** is able to identify physiologic events of the same type as belonging to the same event. For instance, the data parsing circuit **815** may use proximity of the identified physiologic events to determine that they are actually included in the single event. For example, multiple episodes of tachyarrhythmia may actually belong to the same single episode of tachyarrhythmia.

[0077] In some examples, the data parsing circuit identifies physiologic events of different types by parsing the physiologic data. The processor circuit **810** may include a diagnostic circuit **860** configured to determine a link, if any, between the different physiologic events. In certain examples, the

diagnostic circuit **860** uses attributes such as proximity of the identified physiologic events to determine a link between the events. In certain examples, the diagnostic circuit **860** uses duration of identified physiologic events to determine that the physiologic events are related. The report generation circuit **820** includes narrative text in the generated narrative report to indicate any determined link between the different physiologic events.

[0078] Automatically generating a narrative description or a natural language description of episode histories using a medical device may reduce any difficulty a clinician may have in comprehending episode history reports, such as by indicating the relationships of several physiologic events that occur during one or more of the episodes for example. This may result in reduced difficulty for the clinician in tailoring parameters to the patient, which can reduce reliance by clinicians on technical services provided by the device manufacturer. This may also reduce mistakes being made in programming the ambulatory medical device and reduce inappropriate therapy being provided to the patient.

TABLE 1

Event Start
<ol style="list-style-type: none"> 1. This episode started spontaneously within 30 seconds of a commanded induction. 2. The episode started at <start> when three consecutive beats were detected faster than <intvl> bpm. 3. The episode started at <start> when <therapy> was commanded.
Episode Start
<ol style="list-style-type: none"> 1. The arrhythmia onset was declared <Sudden/Gradual>, because the calculated Onset of <meas> was greater than/less than/equal to the programmed Onset threshold of <thres> <units>.
Rates
<ol style="list-style-type: none"> 1. When the episode started, the ventricular rate was <vrate> bpm and the atrial rate was <arate> bpm. 2. When <therapy> was commanded, the ventricular rate was <vrate> bpm and the atrial rate was <arate> bpm. 3. When the device decided to attempt therapy, the ventricular rate <was/increased to/decreased to> <vrate> bpm and the atrial rate <was/increased to/decreased to> <arate> bpm. 4. <time> seconds after therapy delivery, the ventricular rate <was/increased to/decreased to> <vrate> bpm and the atrial rate <was/increased to/decreased to> <arate> bpm.
Non-Sustained
<ol style="list-style-type: none"> 1. The arrhythmia was non-sustained.
No Attempt
<ol style="list-style-type: none"> 1. The arrhythmia was sustained but the episode spontaneously ended before therapy was indicated.
Therapy Initially Inhibited
<ol style="list-style-type: none"> 1. Therapy was initially inhibited when Onset/Stability declared the detected rhythm SVT because the arrhythmia onset was gradual. <ol style="list-style-type: none"> a. The unstable ventricular rhythm reinforced the SVT rhythm determination. 2. Therapy was initially inhibited when Onset/Stability declared the detected rhythm SVT because the ventricular rhythm was unstable. <ol style="list-style-type: none"> a. The gradual arrhythmia onset combined with the absence of Afib reinforced the SVT rhythm determination. 3. Therapy was initially inhibited when Onset/Stability declared the detected rhythm SVT because the arrhythmia onset was gradual and the ventricular rhythm was unstable. 4. Therapy was initially inhibited when Onset/Stability declared the detected rhythm SVT because the ventricular rhythm was unstable and Afib was present. 5. Therapy was initially inhibited when Onset/Stability declared the detected rhythm SVT because the arrhythmia onset was gradual and Afib was not present. 6. Therapy was initially inhibited when Onset/Stability declared the detected rhythm SVT because Afib was present. 7. Therapy was initially inhibited when Rhythm ID declared the detected rhythm SVT because it matched the normal sinus template. <ol style="list-style-type: none"> a. The presence of Afib combined with the unstable ventricular rhythm reinforced the SVT rhythm determination.

TABLE 1-continued

<p>8. Therapy was initially inhibited when Rhythm ID declared the detected rhythm SVT because the ventricular rhythm was unstable and Afib was present.</p> <p>9. When therapy was initially inhibited, the rhythm was stable/unstable because the measured Stability Variance of <stb> ms was <greater than/less than/equal to> the Stability Threshold of <thresh> ms. the rhythm was determined (not) to be Afib, because at least/fewer than 6 of 10 beats were faster than the Afib Threshold of <thresh> bpm. the ventricular rate was not 10 bpm faster than the atrial rate. beats were (not) correlated with the normal sinus template. The measured RhythmMatch was <RhythmMatch>% Therapy Delivered</p>
<p>1. VF therapy was subsequently delivered after the rhythm accelerated to the VF zone.</p> <p>2. Therapy was attempted because the ventricular rate persisted in the <zone> zone. a. Therapy inhibitors were programmed Off.</p> <p>3. Therapy was attempted because the ventricular rate persisted in the <zone> zone and was at least 10 bpm faster than the atrial rate.</p> <p>4. Therapy was attempted because the ventricular rate persisted in the <zone> zone and the programmed Sustained Rate Duration expired after <mm:ss>, overriding therapy inhibition by <EnhType>.</p> <p>5. Therapy was attempted because the arrhythmia onset was sudden and the ventricular rate persisted in the <zone> zone.</p> <p>6. Therapy was attempted because the ventricular rate persisted in the <zone> zone and the ventricular rhythm was stable. a. The absence of Afib reinforced the decision to treat. b. The sudden arrhythmia onset reinforced the decision to treat.</p> <p>7. Therapy was attempted because the arrhythmia onset was sudden, the ventricular rate persisted in the <zone> zone, and the ventricular rhythm was stable. a. The presence of Afib with a stable ventricular rhythm reinforced the decision to treat.</p> <p>8. Therapy was attempted because the ventricular rate persisted in the <zone> zone and Afib was not present.</p> <p>9. Therapy was attempted because the ventricular rate persisted in the <zone> zone, the ventricular rhythm was stable, and Afib was present.</p> <p>10. Therapy was attempted because the arrhythmia onset was sudden, the ventricular rate persisted in the <zone> zone, and Afib was not present.</p> <p>11. Therapy was attempted because the ventricular rate persisted in the <zone> zone and the rhythm did not match the normal sinus template. a. The absence of Afib reinforced the decision to treat. b. The stable ventricular rhythm reinforced the decision to treat. c. The stable ventricular rhythm and the absence of Afib reinforced the decision to treat.</p> <p>12. When the device decided to attempt therapy, the rhythm was <stable/unstable> because the measured Stability Variance of <stb> ms was <greater than/less than/equal to> the Stability Threshold of <thresh> ms. the rhythm was determined (not) to be Afib, because at least/fewer than 6 of 10 beats were faster than the Afib Threshold of <thresh> bpm. the ventricular rate was (not) 10 bpm faster than the atrial rate. beats were (not) correlated with the normal sinus template. The measured RhythmMatch was <RhythmMatch>% Episode End</p>
<p>1. The episode ended at <end>.</p> <p>2. The episode ended at <end>, <time> seconds after therapy was delivered.</p> <p>3. The episode ended at <end> due to a command from the PRM.</p> <p>4. The episode ended at <end> due to programming of the V-tachy parameters.</p>

Additional Notes

[0079] Example 1 includes subject matter (such as a system) comprising a physiologic sensing circuit configured to generate physiologic data for a subject and a processor circuit. The processor circuit includes a data parsing circuit configured to parse the physiologic data to identify one or more physiologic events and a report generation circuit. The report generation circuit is configured to associate narrative text with the identified physiologic events according to a text generating rule and generate a narrative report for the identified physiologic events using the narrative report.

[0080] In Example 2, the subject matter of Example 1 optionally includes a report generation circuit configured to associate narrative text with the identified physiologic events according to at least one of: a decision tree where nodes of the decision tree are linked to narrative text, a lookup table where entries of the lookup table are linked to narrative text, and a specified set of logic rules.

[0081] In Example 3, the subject matter of one or any combination of Examples 1 and 2 includes a physiologic sensing circuit that is included in a first ambulatory medical device, and wherein at least a portion of the text generating rule is specific to a model type of the first medical device.

[0082] In Example 4, the subject matter of one or any combination of Examples 1-3 optionally includes a physiologic sensing circuit that is included in a first ambulatory medical device. The first ambulatory medical device optionally includes: a communication circuit configured to communicate the physiologic data to a separate device, and a controller circuit configured to communicate, in association with the physiologic data, one or more indications of a decision made by the first ambulatory medical device. The processor circuit is optionally included in a second device that includes a communication circuit configured to receive the physiologic data, and the report generation circuit is optionally configured to: associate narrative text with the decision indications, and generate a narrative report for the identified one or more physiologic events and the indications of decisions made by the first medical device using the narrative text.

[0083] In Example 5, the subject matter of Example 4 optionally includes a controller circuit configured to communicate a rationale for the decision made by the first ambulatory medical device in association with the physiologic data. The report generation circuit is optionally configured to: associate narrative text with the rationale for the decision, and generate, using the narrative text, a narrative report for the identified one or more physiologic events, the indication of the decision made by the first medical device, and the rationale for the decision.

[0084] In Example 6, the subject matter of one or any combination of Examples 4 and 5 optionally include a report generation circuit configured to relate a decision made by the first ambulatory medical device to a specified device parameter setting that influenced the decision.

[0085] In Example 7, the subject matter of Example 6 optionally includes a data parsing circuit configured to identify an episode of at least one of tachyarrhythmia or bradycardia using the physiologic data, and the report generation circuit is optionally configured to include, in the generated narrative report, an indication of a decision whether to treat the episode of tachyarrhythmia or bradycardia using device-based therapy.

[0086] In Example 8, the subject matter of one or any combination of Examples 4-7 optionally includes the second device having a port configured to receive an indication of adjudication of an identified physiologic event, and the report generation circuit is optionally configured to change content of the generated narrative report related to the identified physiologic event based on the received adjudication.

[0087] In Example 9, the subject matter of one or any combination of Examples 1-8 optionally includes a physiologic sensing circuit that includes at least one of: a cardiac signal sensing circuit, a heart sound sensing circuit, respiration sensing circuit, a cardiac impedance sensing circuit, and a physical activity sensing circuit.

[0088] In Example 10, the subject matter of one or any combination of Examples 1-9 optionally includes a physiologic sensing circuit configured to produce samples of a sensed physiologic signal as at least a portion of the physiologic data, and the subject matter optionally includes a user interface configured to receive an indication of a specified segment of the sensed physiologic signal for which to generate the narrative report.

[0089] Example 11 can include subject matter (such as a method, a means for performing acts, or a machine-readable medium including instructions that, when performed by the machine, cause the machine to perform acts), or can option-

ally be combined with the subject matter of one or any combination of Examples 1-10 to include such subject matter, comprising generating physiologic data for a subject with a first ambulatory medical device, parsing the physiologic data to identify one or more physiologic events (where the physiologic data is parsed using the first ambulatory medical device or a second separate device), associating narrative text with the identified physiologic events according to a text generating rule, and generating, with the first ambulatory medical device or the second device, a narrative report for the identified physiologic events using the narrative text.

[0090] In Example 12, the subject matter of Example 11 optionally includes associating narrative text with the identified physiologic events according to at least one of: a decision tree wherein nodes of the decision tree are linked to narrative text, a lookup table where entries of the lookup table are linked to narrative text, and a specified set of logic rules.

[0091] In Example 13, the subject matter of one or any combination of Examples 11 and 12 optionally includes at least a portion of a text generating rule that corresponds to a specified model of the first medical device.

[0092] In Example 14, the subject matter of one or any combination of Example 11-13 optionally includes communicating, between the first ambulatory medical device and the second device, one or more indications of a decision made by the first ambulatory medical device in association with the physiologic data, and associating, using the second device, narrative text with the indications. The generating a narrative report optionally includes generating a narrative report for the identified one or more physiologic events and the indications of decisions made by the first medical device using the narrative text.

[0093] In Example 15, the subject matter of Example 14 optionally includes communicating a rationale for the decision made by the first ambulatory medical device in association with the communicated physiologic data, and associating, using the second device, narrative text with the rationale for the decision. The generating a narrative report optionally includes generating, using the narrative text, a narrative report for the identified one or more physiologic events, the indication of the decision made by the first medical device, and the rationale for the decision.

[0094] In Example 16, the subject matter of one or any combination of Examples 11-15 optionally includes identifying a plurality of physiologic events of a same type for a subject using the communicated physiologic data, comparing one or more attributes of the physiologic data associated with the physiologic events using the second device, and including narrative text related to a result of the comparison in the generated narrative report.

[0095] In Example 17, the subject matter of Example 16 optionally includes recurrently obtaining electrograms of the patient, and incorporating a graphical representation of a comparison of two or more obtained electrograms in the generated narrative report.

[0096] In Example 18, the subject matter of one or any combination of Examples 11-17 optionally includes parsing the physiologic data to identify a plurality of physiologic events for the subject, determining a relationship, if any, between the physiologic events, determining a relationship, if any, between the physiologic events and at least one of a programmed parameter or a decision made by the first ambulatory medical device, and including narrative text in the generated narrative report to indicate the relationship

between the physiologic events, the programmed parameter and the device based decision.

[0097] In Example 19, the subject matter of one or any combination of Examples 11-18 optionally includes associating physiologic data from at least one of the second device or a third device with the communicated physiologic data, and associating narrative text with the identified physiologic events and the associated physiologic data.

[0098] In Example 20, the subject matter of one or any combination of Examples 11-19 optionally includes receiving, by the second device, an indication of adjudication of an identified physiologic event, and changing content of the generated narrative report related to the identified physiologic event based on the received adjudication.

[0099] Example 21 can include, or can optionally be combined with any portion or combination of any portions of any one or more of Examples 1-20 to include, subject matter that can include means for performing any one or more of the functions of Examples 1-20, or a machine-readable medium including instructions that, when performed by a machine, cause the machine to perform any one or more of the functions of Examples 1-20.

[0100] These non-limiting examples can be combined in any permutation or combination.

[0101] The above detailed description includes references to the accompanying drawings, which form a part of the detailed description. The drawings show, by way of illustration, specific embodiments in which the invention can be practiced. These embodiments are also referred to herein as "examples." In the event of inconsistent usages between this document and documents incorporated by reference, the usage in the incorporated reference(s) should be considered supplementary to that of this document; for irreconcilable inconsistencies, the usage in this document controls.

[0102] In this document, the terms "a" or "an" are used, as is common in patent documents, to include one or more than one, independent of any other instances or usages of "at least one" or "one or more." In this document, the term "or" is used to refer to a nonexclusive or, such that "A or B" includes "A but not B," "B but not A," and "A and B," unless otherwise indicated. In the appended claims, the terms "including" and "in which" are used as the plain-English equivalents of the respective terms "comprising" and "wherein." Also, in the following claims, the terms "including" and "comprising" are open-ended, that is, a system, device, article, or process that includes elements in addition to those listed after such a term in a claim are still deemed to fall within the scope of that claim. Moreover, in the following claims, the terms "first," "second," and "third," etc. are used merely as labels, and are not intended to impose numerical requirements on their objects.

[0103] Method examples described herein can be machine or computer-implemented at least in part. Some examples can include a computer-readable medium or machine-readable medium encoded with instructions operable to configure an electronic device to perform methods as described in the above examples. An implementation of such methods can include code, such as microcode, assembly language code, a higher-level language code, or the like. Such code can include computer readable instructions for performing various methods. The code can form portions of computer program products. Further, the code can be tangibly stored on one or more volatile or non-volatile computer-readable media during execution or at other times. These computer-readable media

can include, but are not limited to, hard disks, removable magnetic disks, removable optical disks (e.g., compact disks and digital video disks), magnetic cassettes, memory cards or sticks, random access memories (RAM's), read only memories (ROM's), and the like. In some examples, a carrier medium can carry code implementing the methods. The term "carrier medium" can be used to represent carrier waves on which code is transmitted.

[0104] The above description is intended to be illustrative, and not restrictive. For example, the above-described examples (or one or more aspects thereof) may be used in combination with each other. Other embodiments can be used, such as by one of ordinary skill in the art upon reviewing the above description. The Abstract is provided to comply with 37 C.F.R. §1.72(b), to allow the reader to quickly ascertain the nature of the technical disclosure. It is submitted with the understanding that it will not be used to interpret or limit the scope or meaning of the claims. Also, in the above Detailed Description, various features may be grouped together to streamline the disclosure. This should not be interpreted as intending that an unclaimed disclosed feature is essential to any claim. Rather, inventive subject matter may lie in less than all features of a particular disclosed embodiment. Thus, the following claims are hereby incorporated into the Detailed Description, with each claim standing on its own as a separate embodiment. The scope of the invention should be determined with reference to the appended claims, along with the full scope of equivalents to which such claims are entitled.

What is claimed is:

1. A system comprising:

a physiologic sensing circuit configured to generate physiologic data for a subject; and

a processor circuit including:

a data parsing circuit configured to parse the physiologic data to identify one or more physiologic events;

a report generation circuit configured to:

associate narrative text with the identified physiologic events according to a text generating rule; and

generate a narrative report for the identified physiologic events using the narrative text.

2. The system of claim 1, wherein the report generation circuit is configured to associate narrative text with the identified physiologic events according to at least one of:

a decision tree, wherein nodes of the decision tree are linked to narrative text;

a lookup table, wherein entries of the lookup table are linked to narrative text; and

a specified set of logic rules.

3. The system of claim 1, wherein the physiologic sensing circuit is included in a first ambulatory medical device, and wherein at least a portion of the text generating rule is specific to a model type of the first medical device.

4. The system of claim 1,

wherein the physiologic sensing circuit is included in a first ambulatory medical device that includes:

a communication circuit configured to communicate the physiologic data to a separate device; and

a controller circuit configured to communicate, in association with the physiologic data, one or more indications of a decision made by the first ambulatory medical device; and

- wherein the processor circuit is included in a second device that includes a communication circuit configured to receive the physiologic data, and
- wherein the report generation circuit is configured to:
- associate narrative text with the decision indications; and
 - generate a narrative report for the identified one or more physiologic events and the indications of decisions made by the first medical device using the narrative text.
- 5.** The system of claim **4**,
- wherein the controller circuit is configured to communicate a rationale for the decision made by the first ambulatory medical device in association with the physiologic data; and
- wherein the report generation circuit is configured to:
- associate narrative text with the rationale for the decision, and
 - generate, using the narrative text, a narrative report for the identified one or more physiologic events, the indication of the decision made by the first medical device, and the rationale for the decision.
- 6.** The system of claim **4**, wherein the report generation circuit is configured to relate a decision made by the first ambulatory medical device to a specified device parameter setting that influenced the decision.
- 7.** The system of claim **6**,
- wherein the data parsing circuit is configured to identify an episode of at least one of tachyarrhythmia or bradycardia using the physiologic data, and
- wherein the report generation circuit is configured to include, in the generated narrative report, an indication of a decision whether to treat the episode of tachyarrhythmia or bradycardia using device-based therapy.
- 8.** The system of claim **4**, wherein the second device includes a port configured to receive an indication of adjudication of an identified physiologic event, and
- wherein the report generation circuit is configured to change content of the generated narrative report related to the identified physiologic event based on the received adjudication.
- 9.** The system of claim **1**, wherein the physiologic sensing circuit includes at least one of:
- a cardiac signal sensing circuit;
 - a heart sound sensing circuit;
 - respiration sensing circuit;
 - a cardiac impedance sensing circuit; and
 - a physical activity sensing circuit.
- 10.** The system of claim **1**,
- wherein the physiologic sensing circuit is configured to produce samples of a sensed physiologic signal as at least a portion of the physiologic data,
- wherein the system includes a user interface configured to receive an indication of a specified segment of the sensed physiologic signal for which to generate the narrative report.
- 11.** A method comprising:
- generating physiologic data for a subject with a first ambulatory medical device;
 - parsing the physiologic data to identify one or more physiologic events, wherein the physiologic data is parsed using the first ambulatory medical device or a second separate device;
 - associating narrative text with the identified physiologic events according to a text generating rule; and
 - generating, with the first ambulatory medical device or the second device, a narrative report for the identified physiologic events using the narrative text.
- 12.** The method of claim **11**, wherein associating narrative text with the identified physiologic events according to a text generating rule includes associating narrative text with the identified physiologic events according to at least one of:
- a decision tree, wherein nodes of the decision tree are linked to narrative text;
 - a lookup table, wherein entries of the lookup table are linked to narrative text; and
 - a specified set of logic rules.
- 13.** The method of claim **11**, wherein at least a portion of the text generating rule corresponds to a specified model of the first medical device.
- 14.** The method of claim **11**, including:
- communicating, between the first ambulatory medical device and the second device, one or more indications of a decision made by the first ambulatory medical device in association with the physiologic data; and
 - associating, using the second device, narrative text with the indications, and
 - wherein generating a narrative report includes generating a narrative report for the identified one or more physiologic events and the indications of decisions made by the first medical device using the narrative text.
- 15.** The method of claim **14**, including:
- communicating a rationale for the decision made by the first ambulatory medical device in association with the communicated physiologic data; and
 - associating, using the second device, narrative text with the rationale for the decision, and
 - wherein generating a narrative report includes generating, using the narrative text, a narrative report for the identified one or more physiologic events, the indication of the decision made by the first medical device, and the rationale for the decision.
- 16.** The method of claim **11**, including:
- identifying a plurality of physiologic events of a same type for a subject using the communicated physiologic data; comparing one or more attributes of the physiologic data associated with the physiologic events using the second device; and
 - including narrative text related to a result of the comparison in the generated narrative report.
- 17.** The method of claim **16**,
- wherein identifying a plurality of physiologic events includes recurrently obtaining electrograms of the patient, and
 - wherein generating a narrative report includes incorporating a graphical representation of a comparison of two or more obtained electrograms in the generated narrative report.
- 18.** The method of claim **11**, including:
- parsing the physiologic data to identify a plurality of physiologic events for the subject;
 - determining a relationship, if any, between the physiologic events;
 - determining a relationship, if any, between the physiologic events and at least one of a programmed parameter or a decision made by the first ambulatory medical device; and

including narrative text in the generated narrative report to indicate the relationship between the physiologic events, the programmed parameter and the device based decision.

19. The method of claim **11**, including:

associating physiologic data from at least one of the second device or a third device with the communicated physiologic data, and

wherein associating narrative text includes associating narrative text with the identified physiologic events and the associated physiologic data.

20. The method of claim **11**, including:

receiving, by the second device, an indication of adjudication of an identified physiologic event; and

changing content of the generated narrative report related to the identified physiologic event based on the received adjudication.

* * * * *

专利名称(译)	叙事生成算法		
公开(公告)号	US20130211855A1	公开(公告)日	2013-08-15
申请号	US13/589513	申请日	2012-08-20
[标]申请(专利权)人(译)	EBERLE LEANNE中号 PERSCHBACHER DAVID大号 黄陈YEE 邵伟光		
申请(专利权)人(译)	EBERLE, LEANNE M. PERSCHBACHER, DAVID L. 黄, 陈YEE 邵, 伟光		
当前申请(专利权)人(译)	EBERLE, LEANNE M. PERSCHBACHER, DAVID L. 黄, 陈YEE 邵, 伟光		
[标]发明人	EBERLE LEANNE M PERSCHBACHER DAVID L WONG CHEN YEE SHAO WEIGUANG		
发明人	EBERLE, LEANNE M. PERSCHBACHER, DAVID L. WONG, CHEN YEE SHAO, WEIGUANG		
IPC分类号	G06F19/00 A61B5/00		
CPC分类号	A61N1/37282 A61N1/362 A61B5/0022 G06F19/3487 G06F19/3418 A61N1/37258 G16H15/00 G16H40/67		
优先权	61/528372 2011-08-29 US		
外部链接	Espacenet USPTO		

摘要(译)

一种系统包括被配置为生成对象的生理数据的生理感测电路和处理电路。处理电路包括配置成解析生理数据以识别一个或多个生理事件的数据解析电路和报告生成电路。报告生成电路被配置为根据文本生成规则将叙述文本与所识别的生理事件相关联，并使用所述叙述文本生成所识别的生理事件的叙述性报告。

