



US009002441B2

(12) **United States Patent**  
**Heil et al.**

(10) **Patent No.:** **US 9,002,441 B2**  
(45) **Date of Patent:** **Apr. 7, 2015**

(54) **ELECTRONIC FETAL MONITORING APPLICATIONS AND DISPLAY**

USPC ..... 600/511, 595, 509; 607/32  
See application file for complete search history.

(75) Inventors: **Christopher Heil**, Liberty, MO (US);  
**Jeremy Flores**, Overland Park, KS (US);  
**Carol George**, Spring Hill, KS (US)

(56) **References Cited**

(73) Assignee: **Cerner Innovation, Inc.**, Kansas City, KS (US)

U.S. PATENT DOCUMENTS

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 560 days.

5,442,940	A *	8/1995	Secker et al.	600/483
5,724,985	A *	3/1998	Snell et al.	600/510
5,785,660	A *	7/1998	van Lake et al.	600/523
7,412,283	B2 *	8/2008	Ginzburg et al.	600/517
2003/0208128	A1 *	11/2003	Hamilton et al.	600/509
2004/0054295	A1 *	3/2004	Ramseth	600/509
2004/0197727	A1 *	10/2004	Sachdeva et al.	433/24
2006/0265020	A1 *	11/2006	Fischell et al.	607/30
2008/0154155	A1 *	6/2008	Nishihara et al.	600/595
2009/0240158	A1 *	9/2009	Hamilton et al.	600/511
2011/0282225	A1 *	11/2011	Anderson et al.	600/510

(21) Appl. No.: **12/564,569**

\* cited by examiner

(22) Filed: **Sep. 22, 2009**

(65) **Prior Publication Data**

US 2011/0071414 A1 Mar. 24, 2011

*Primary Examiner* — Niketa Patel

*Assistant Examiner* — William Levicky

(51) **Int. Cl.**  
**A61B 5/04** (2006.01)  
**A61B 5/0444** (2006.01)  
**A61B 5/00** (2006.01)

(74) *Attorney, Agent, or Firm* — Shook, Hardy & Bacon L.L.P


(52) **U.S. Cl.**  
CPC ..... **A61B 5/0444** (2013.01); **A61B 5/0011** (2013.01); **A61B 5/411** (2013.01); **A61B 5/4362** (2013.01)

(57) **ABSTRACT**

Systems, methods, and computer-readable media for managing healthcare environments are provided. In embodiments, a first waveform tracing for data received from one or more medical devices for a first individual is displayed. A second waveform tracing for data received from one or more medical devices for a second individual is displayed. In response to the determination to hide the first waveform tracing, only displaying the second waveform tracing.

(58) **Field of Classification Search**  
CPC ..... A61B 5/0006; A61B 5/02405; A61B 5/02411; A61B 5/033; A61B 5/0444; A61B 5/4356; A61B 5/4343; A61B 5/435; A61B 5/0011; A61B 5/024

**6 Claims, 15 Drawing Sheets**

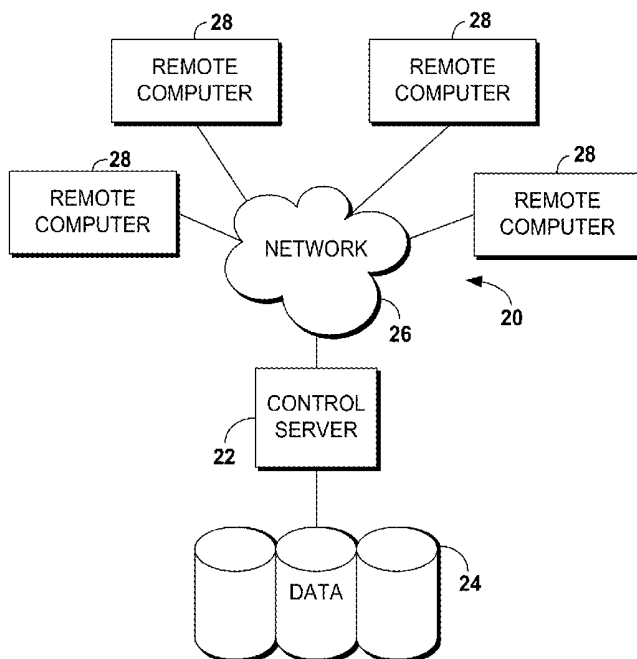

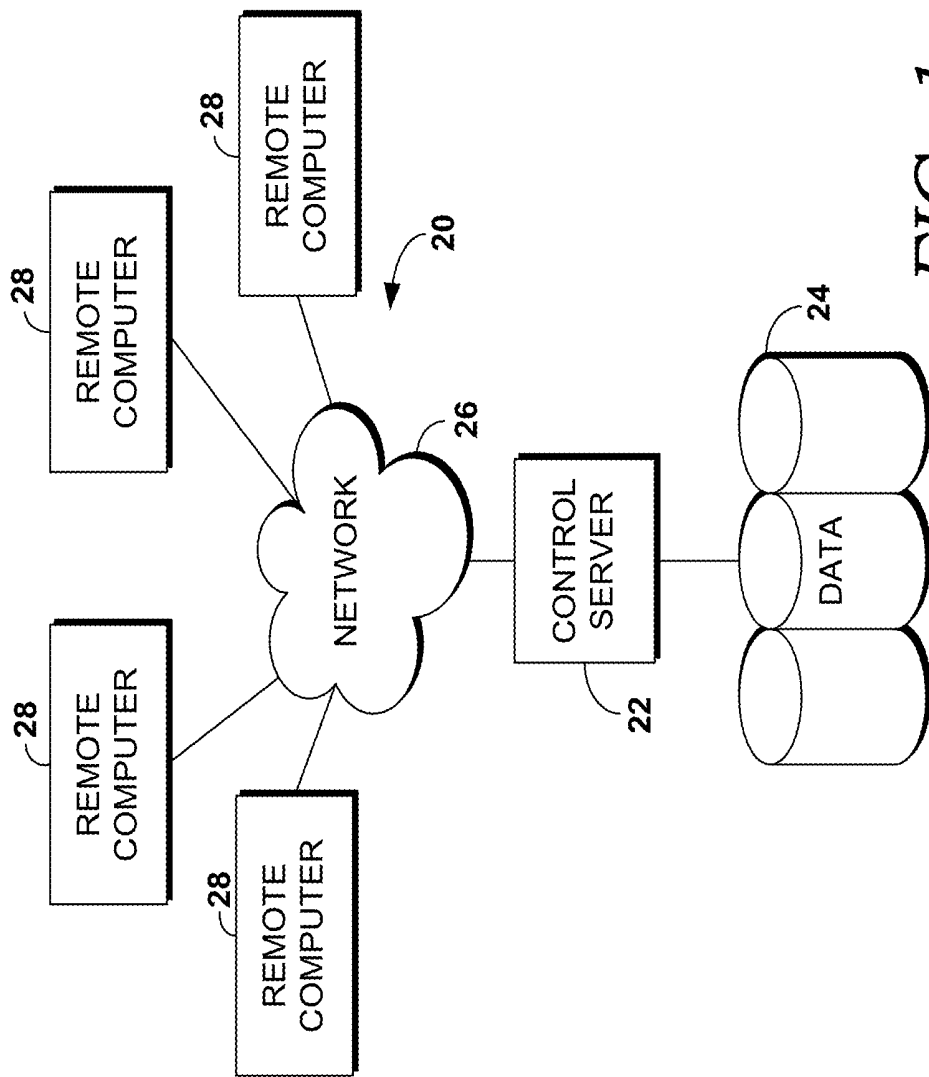


FIG. 1.

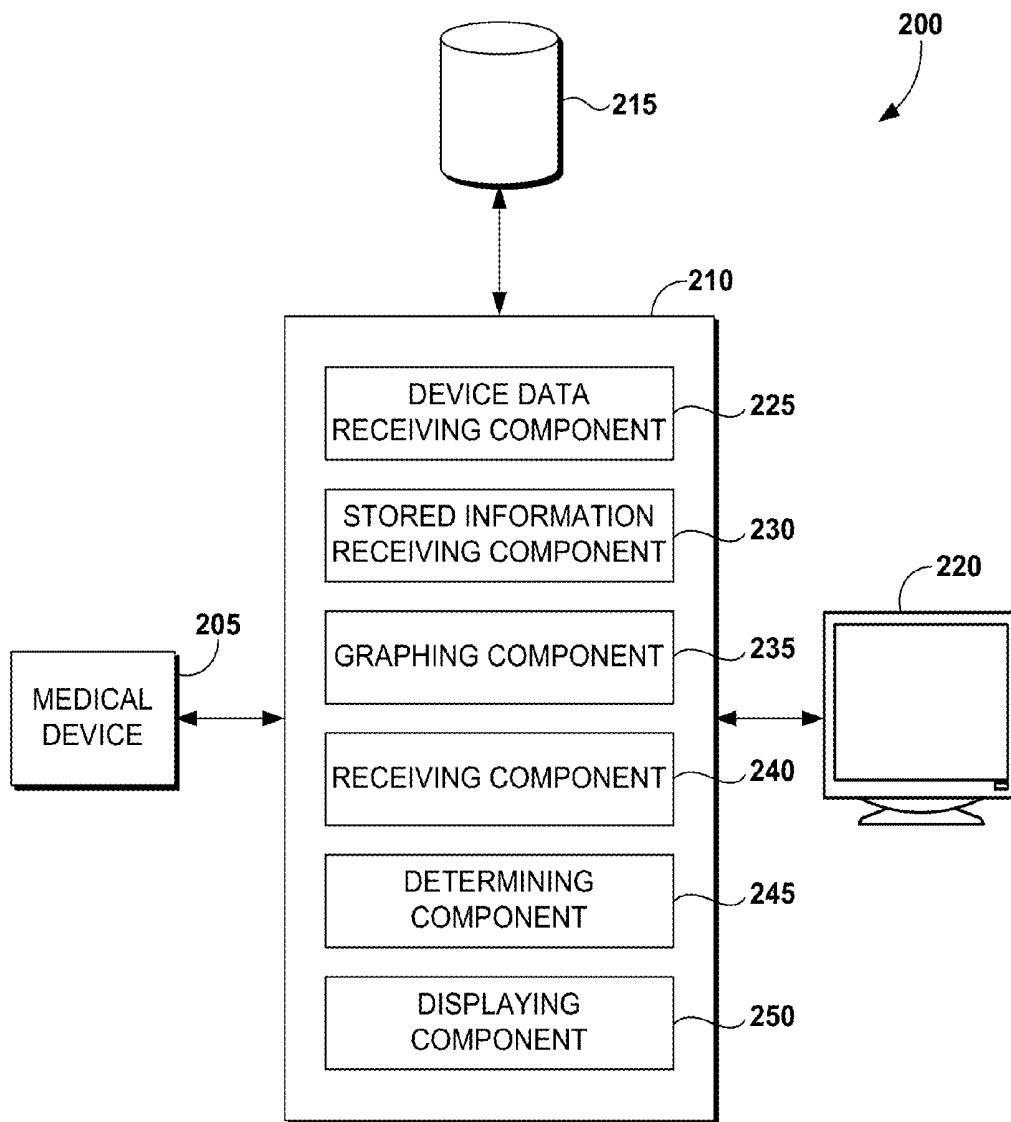


FIG. 2.

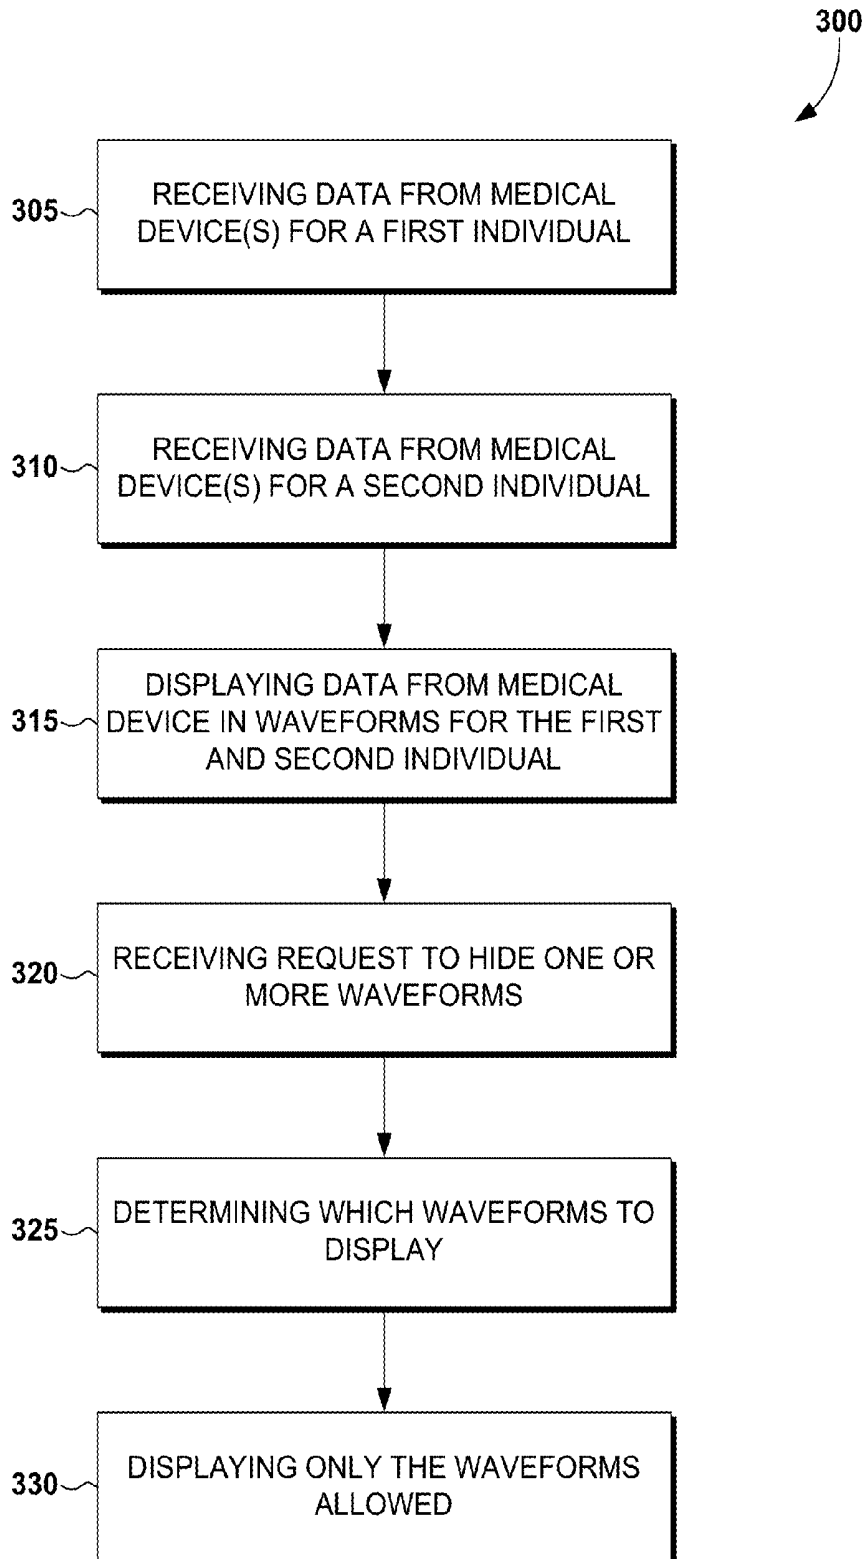


FIG. 3.


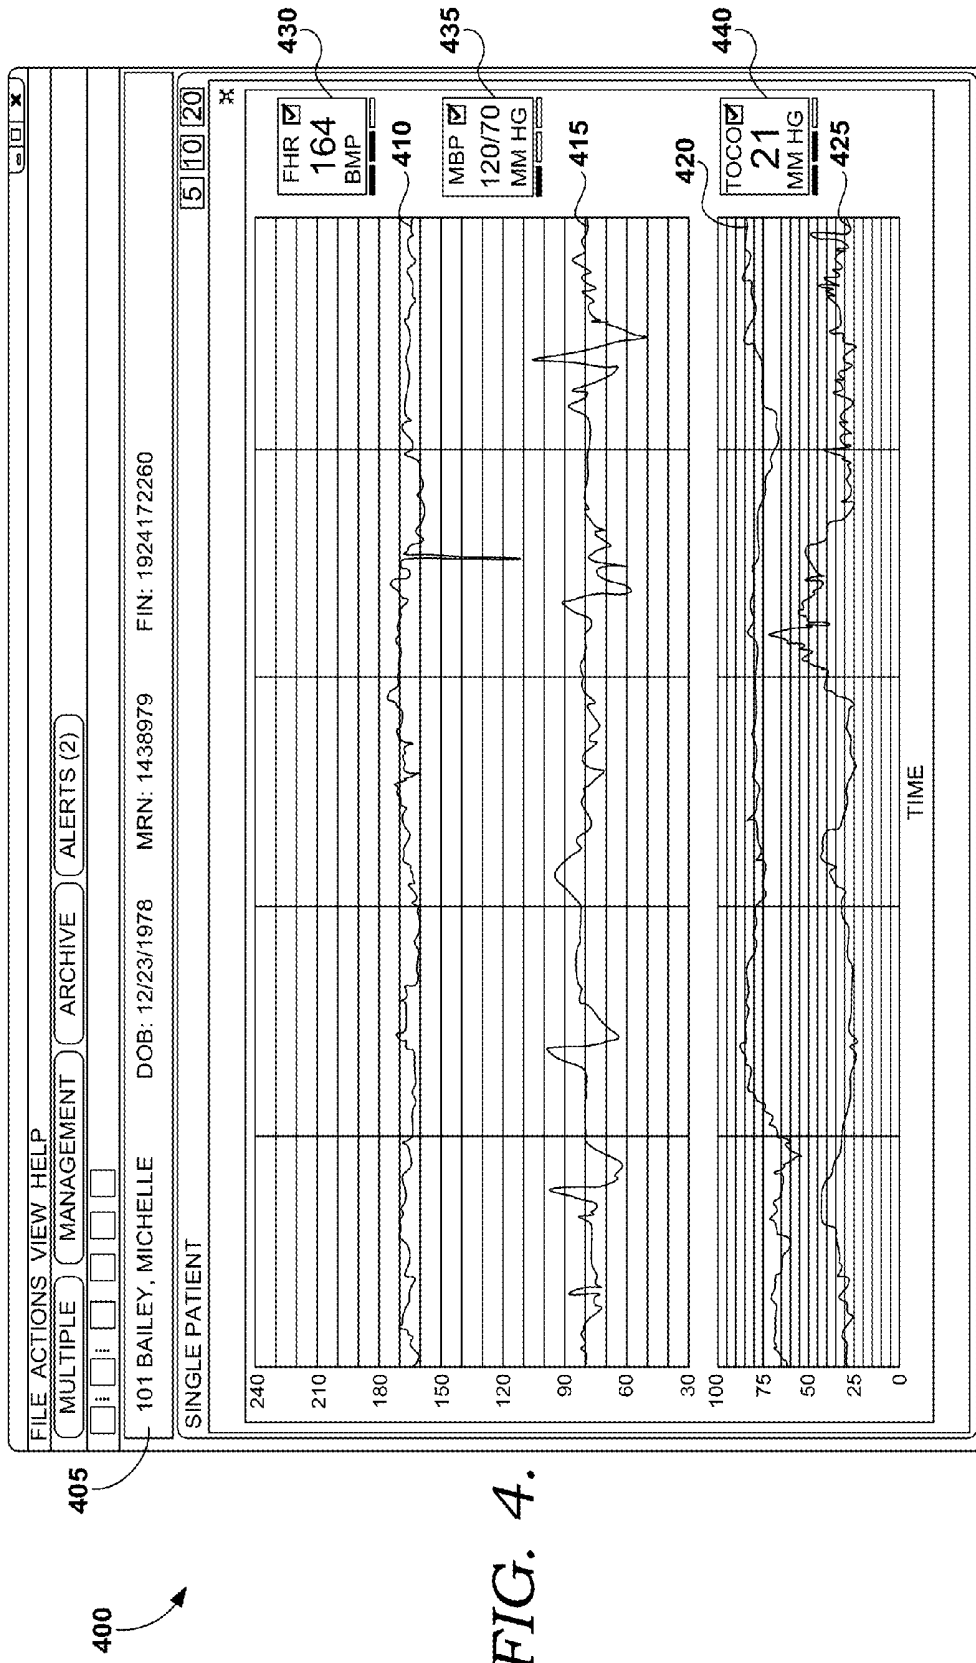


FIG. 4.

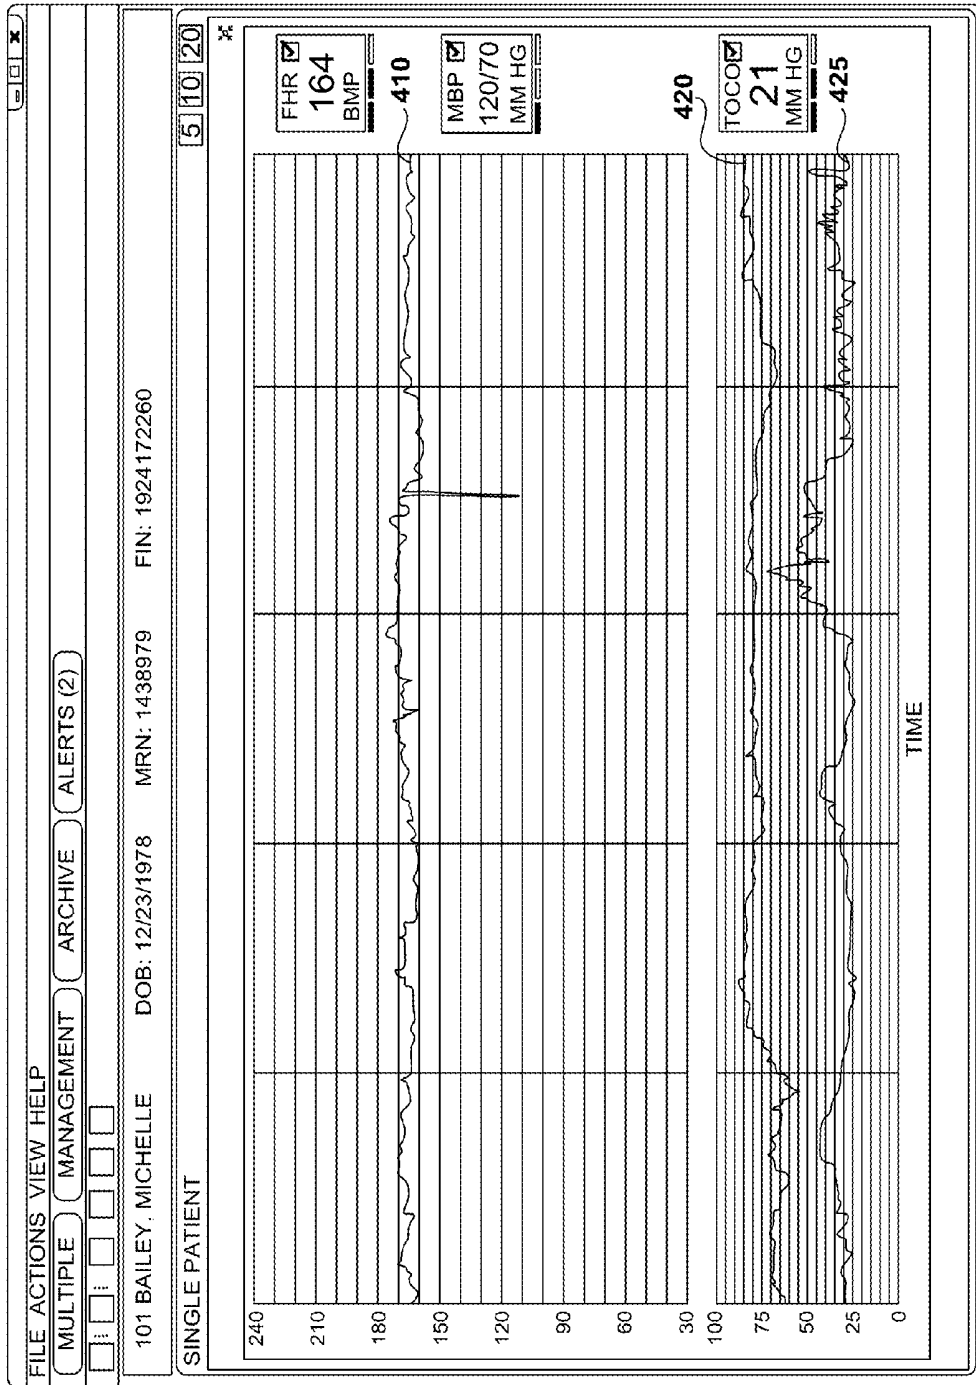

500






FIG. 5.

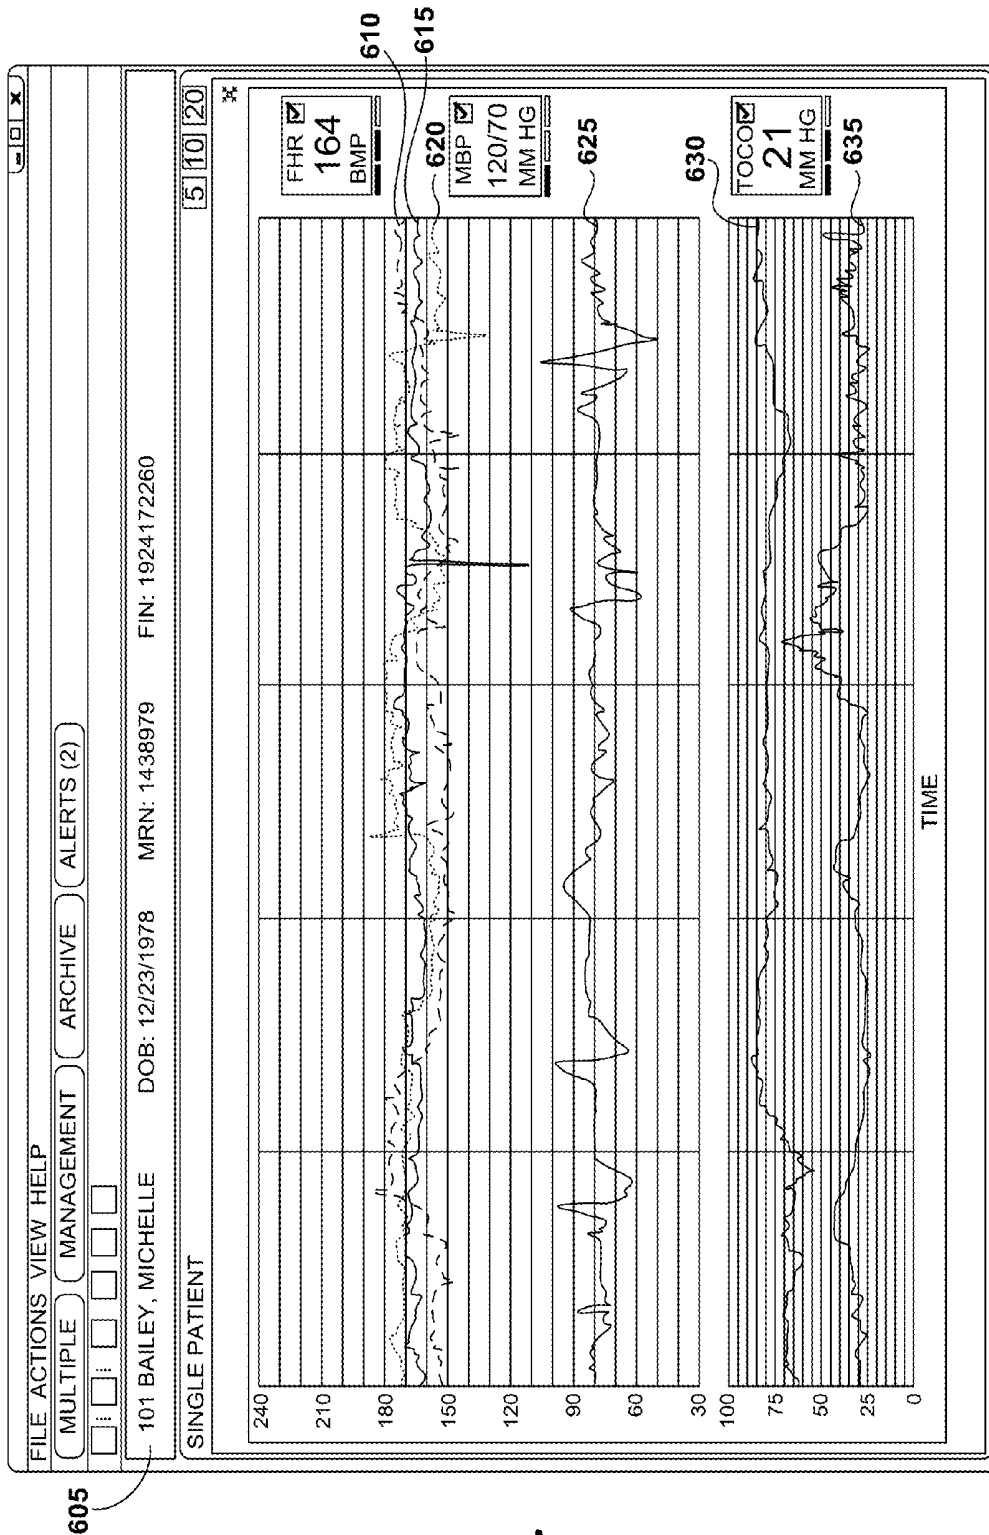

605

600

FIG. 6.

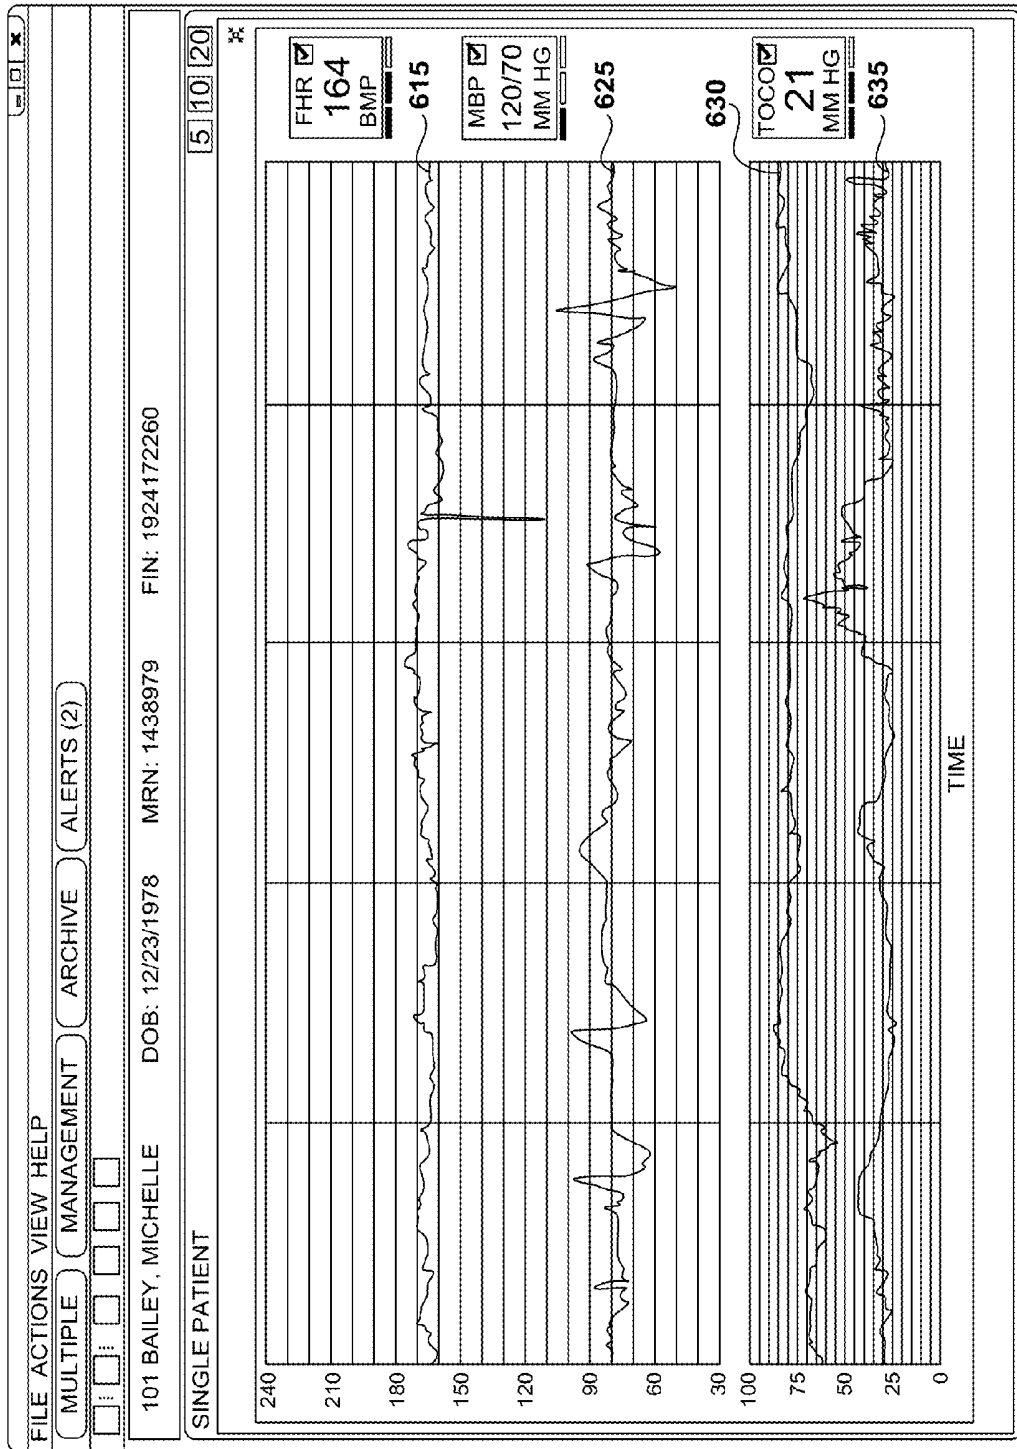

700

FIG. 7.


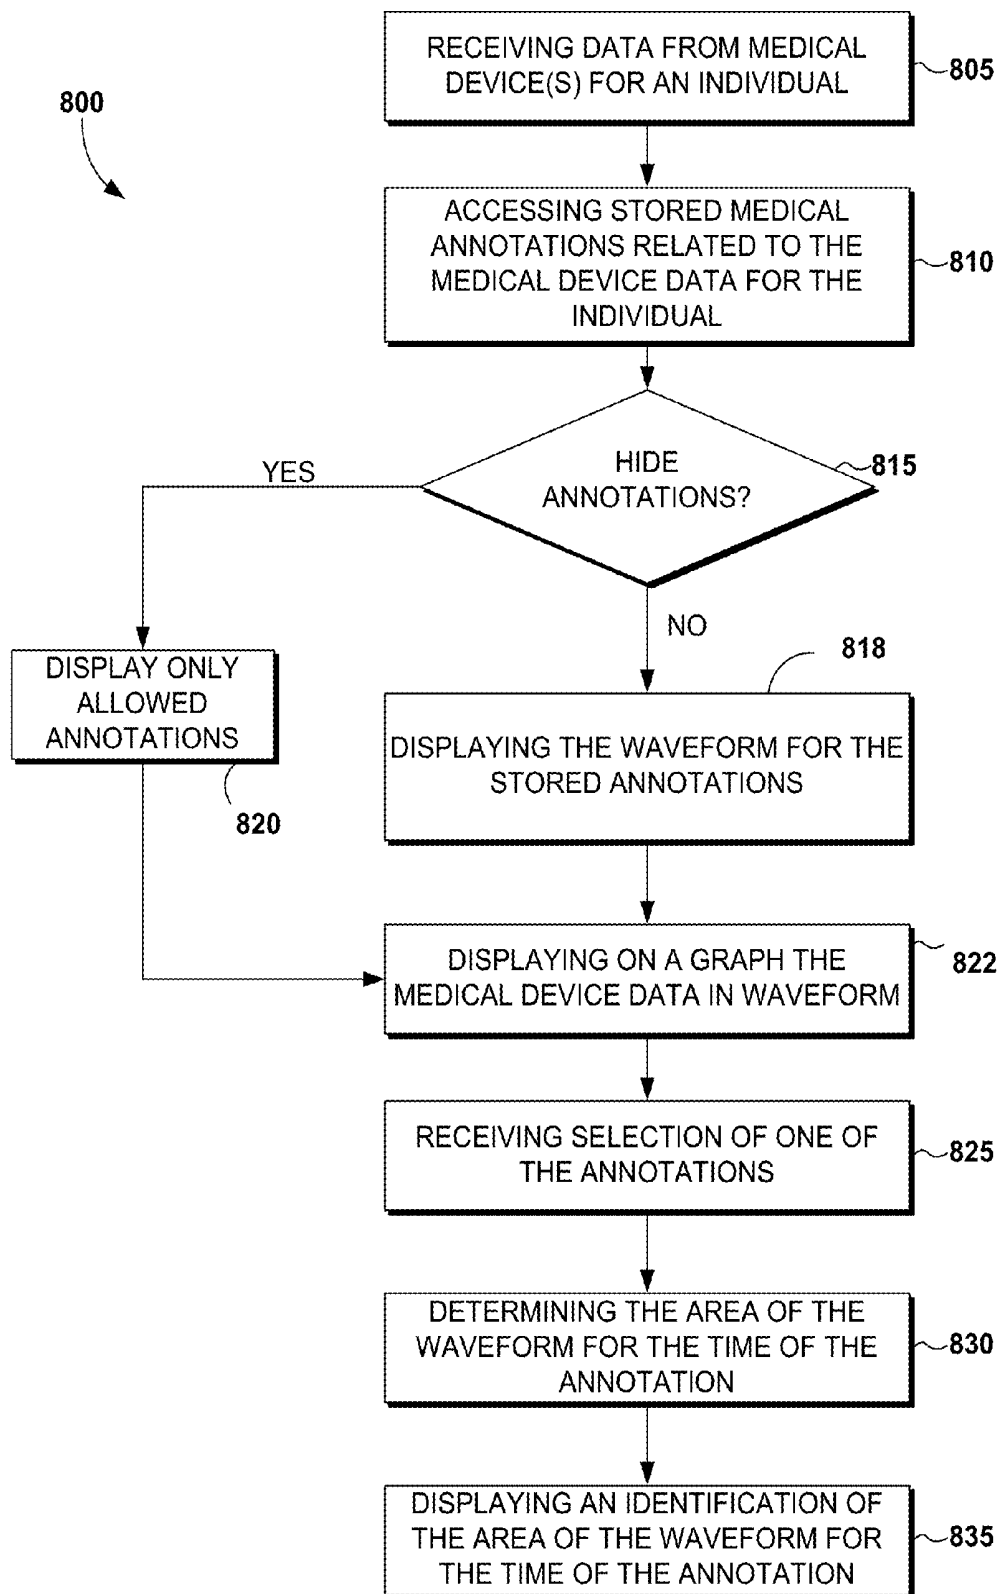


FIG. 8.

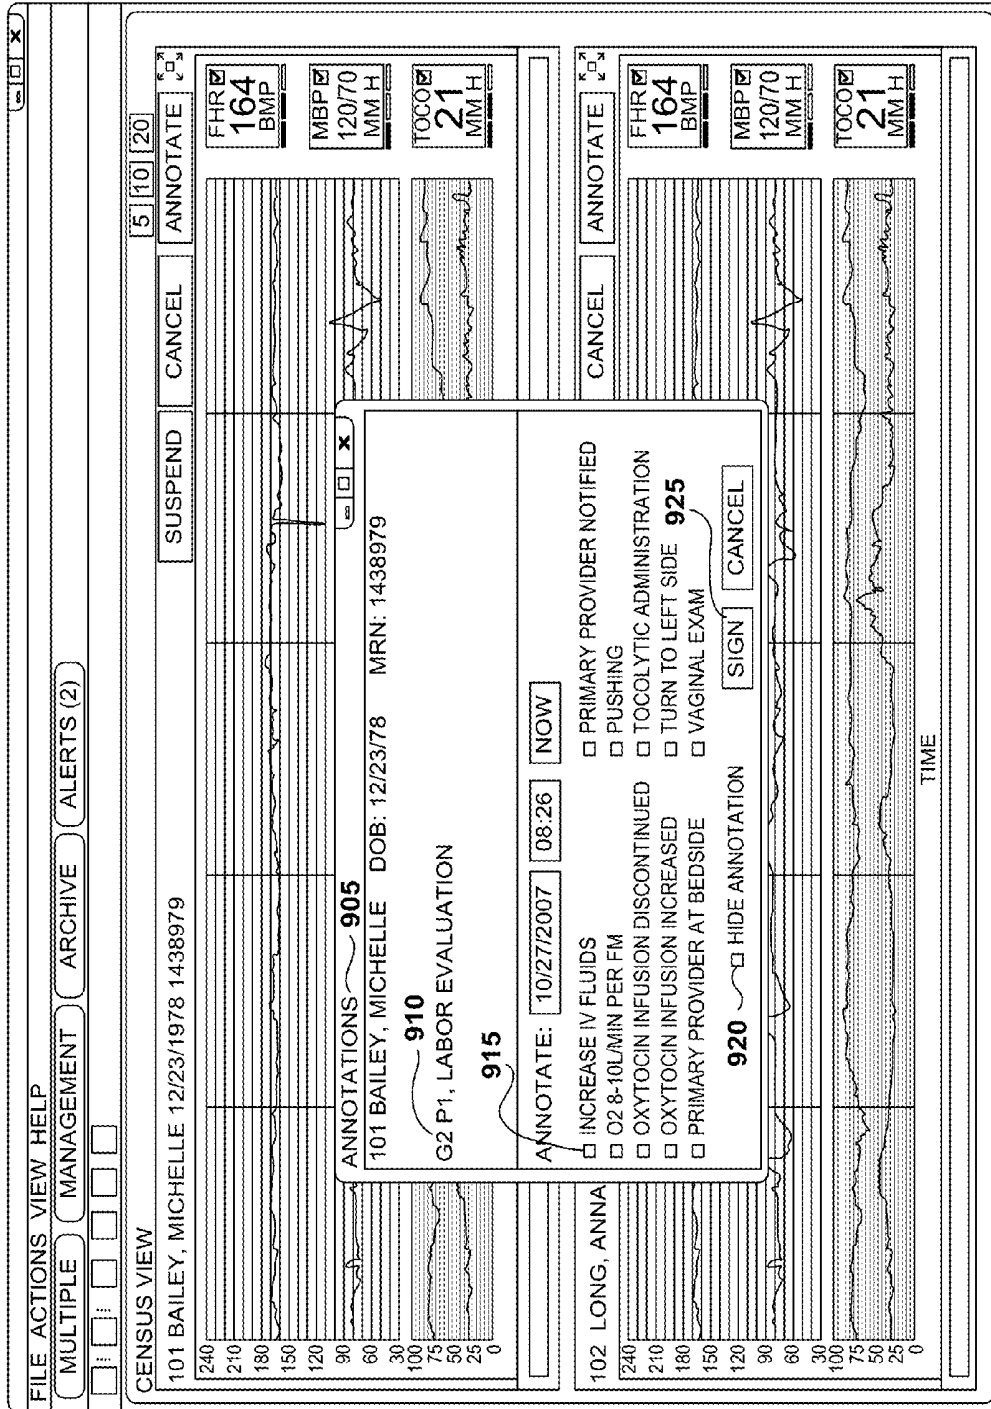

900

FIG. 9.

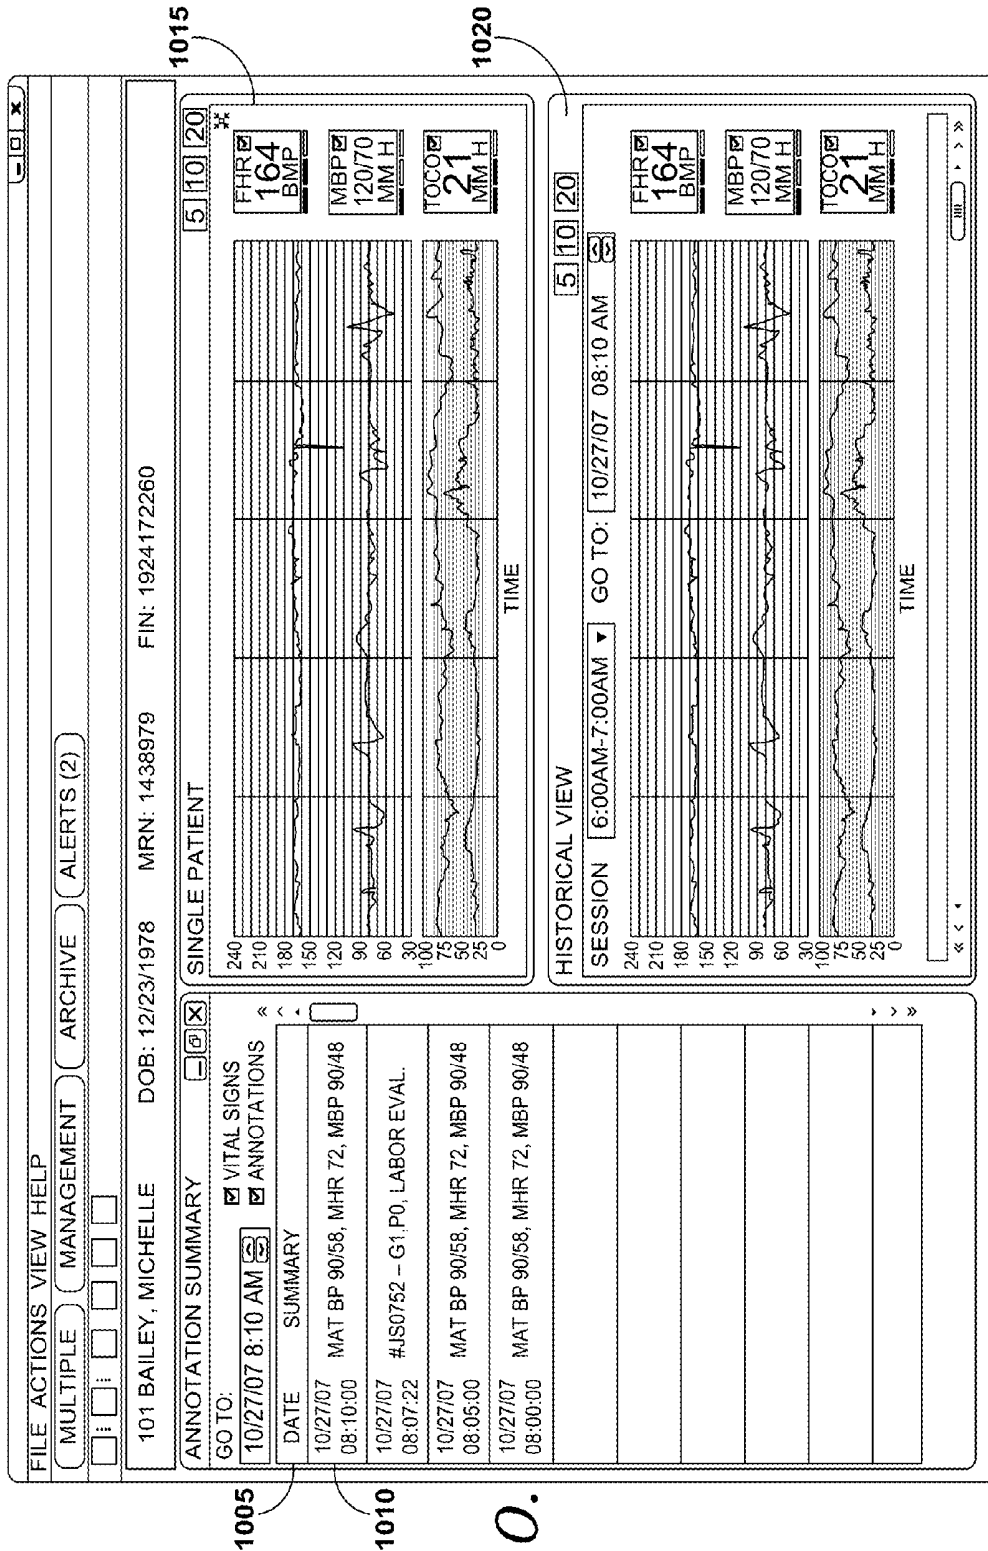


FIG. 10.

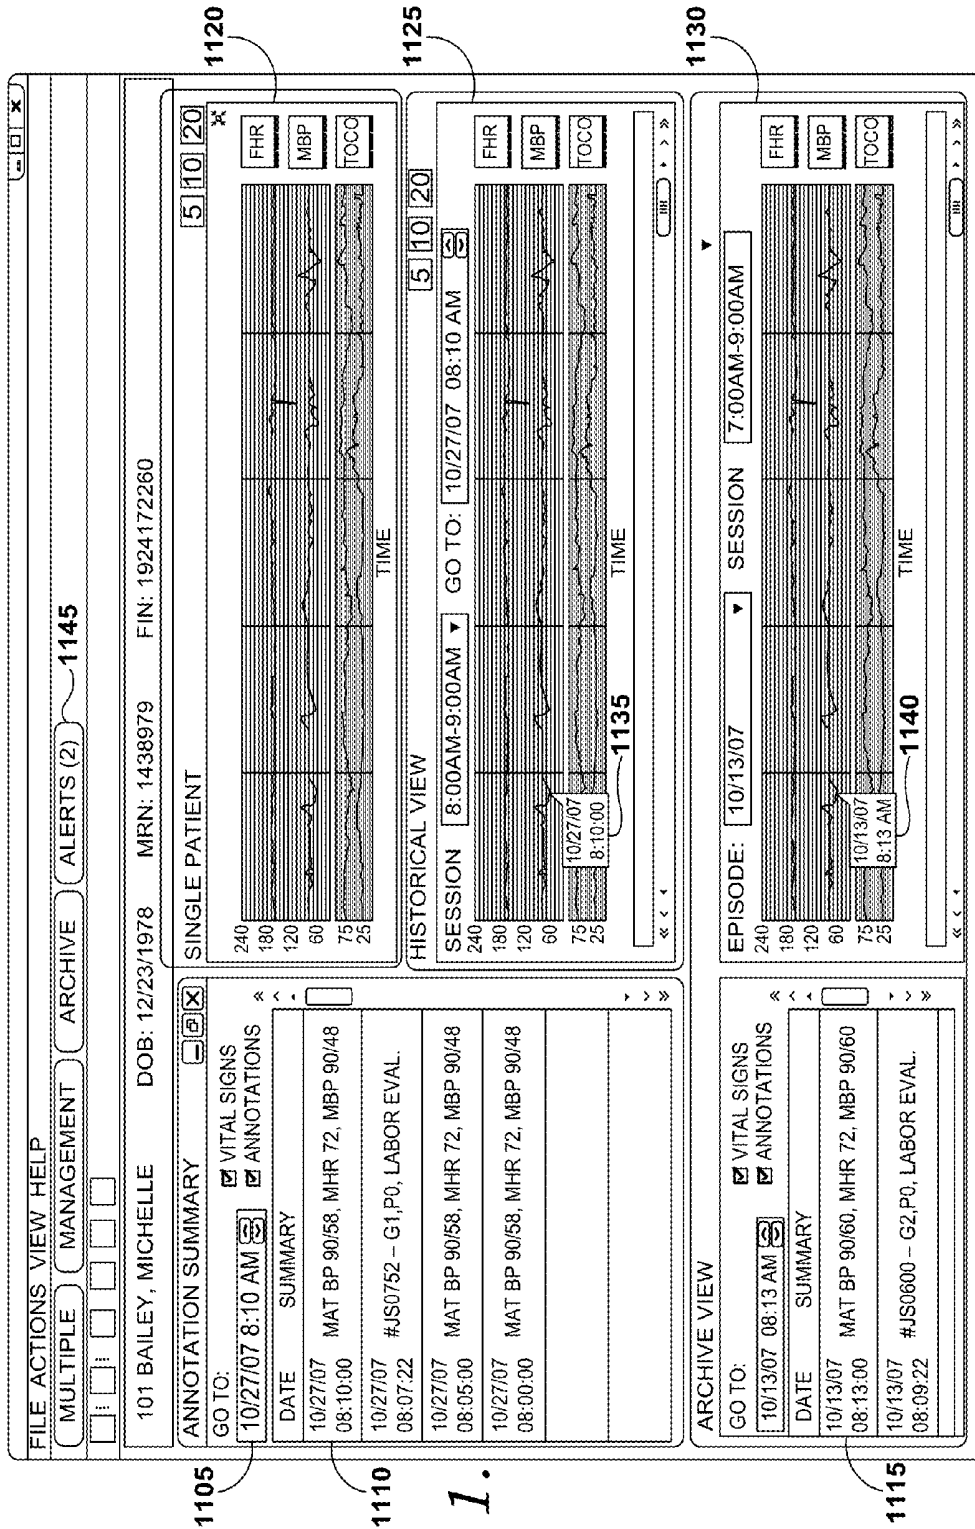


FIG. 11.

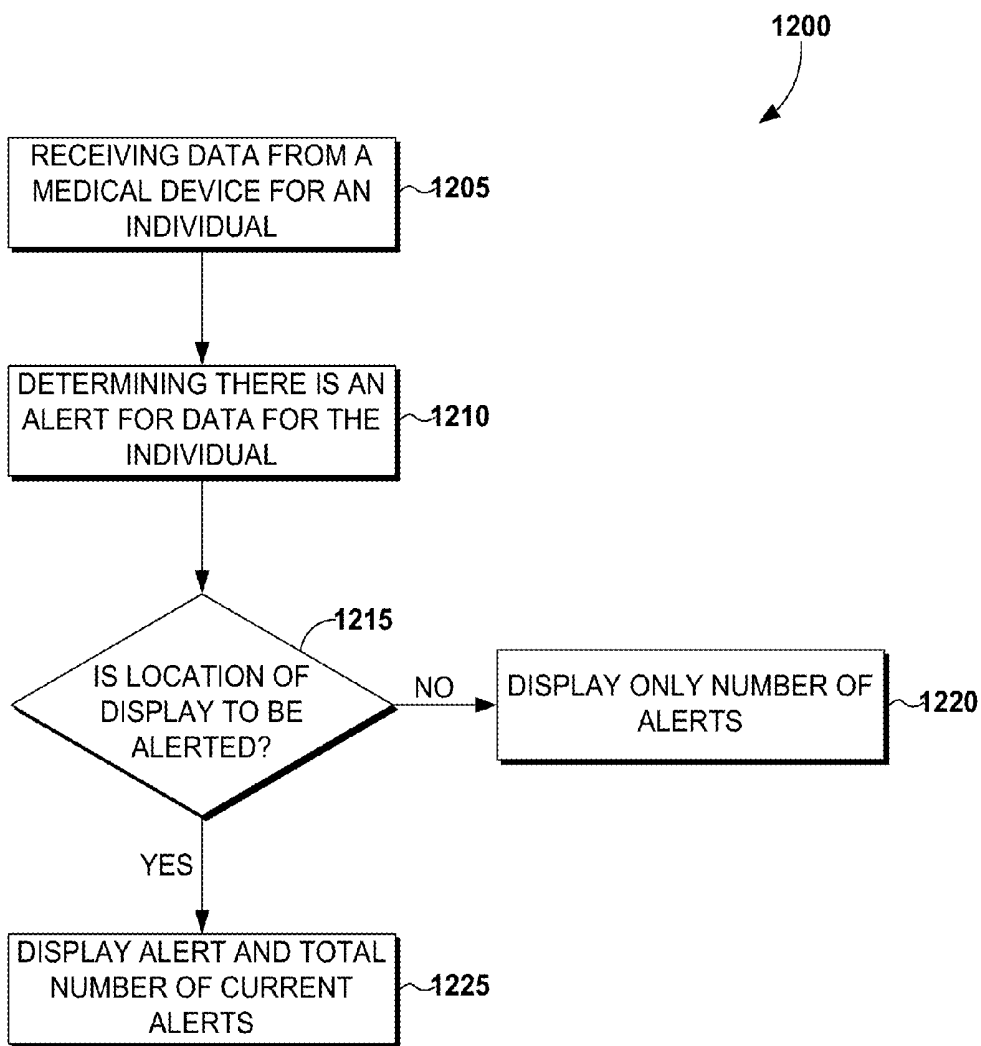


FIG. 12.

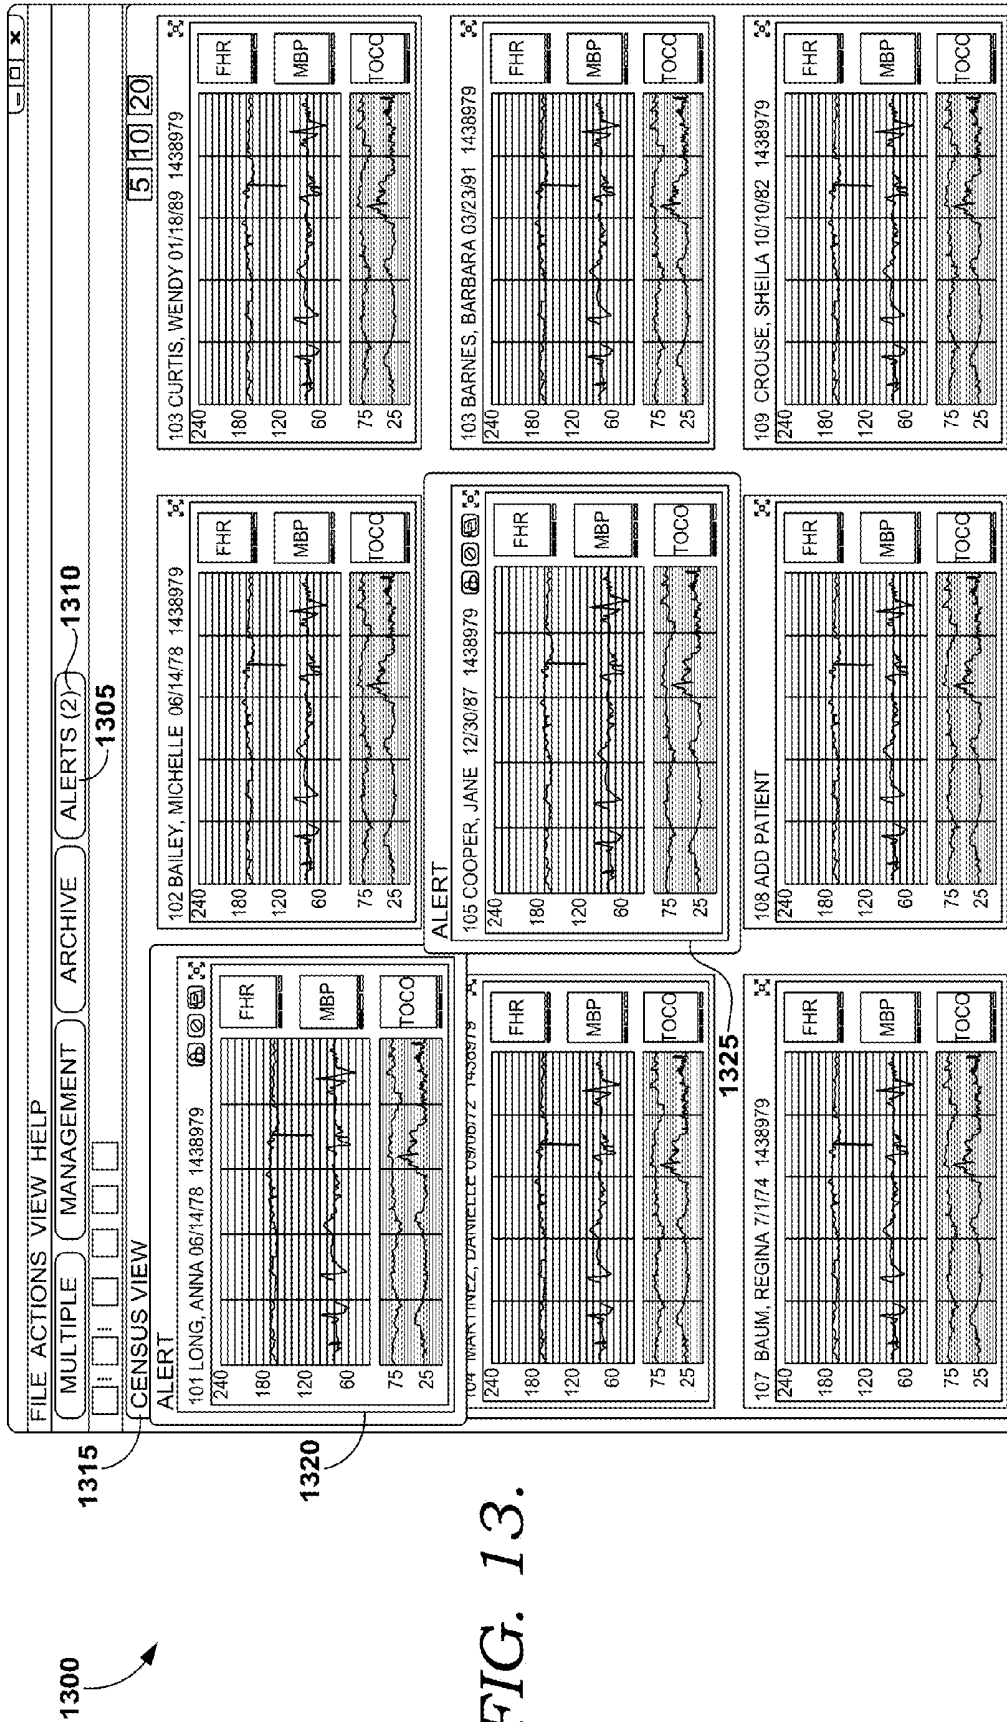


FIG. 13.


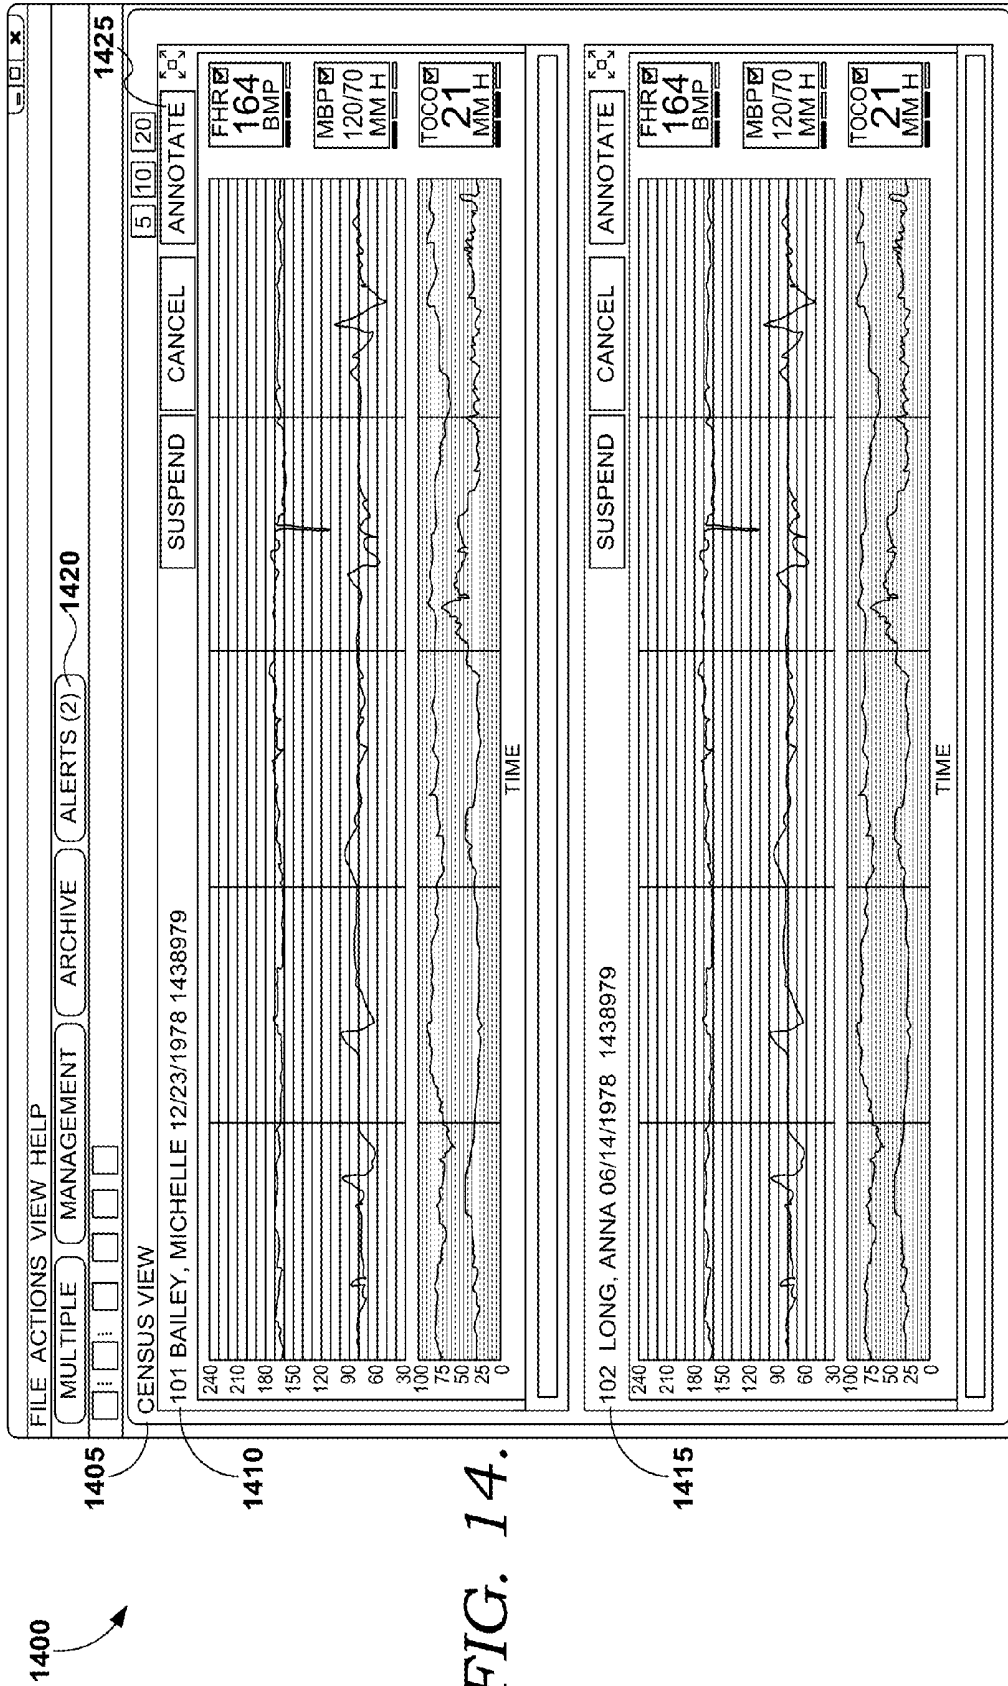


FIG. 14.

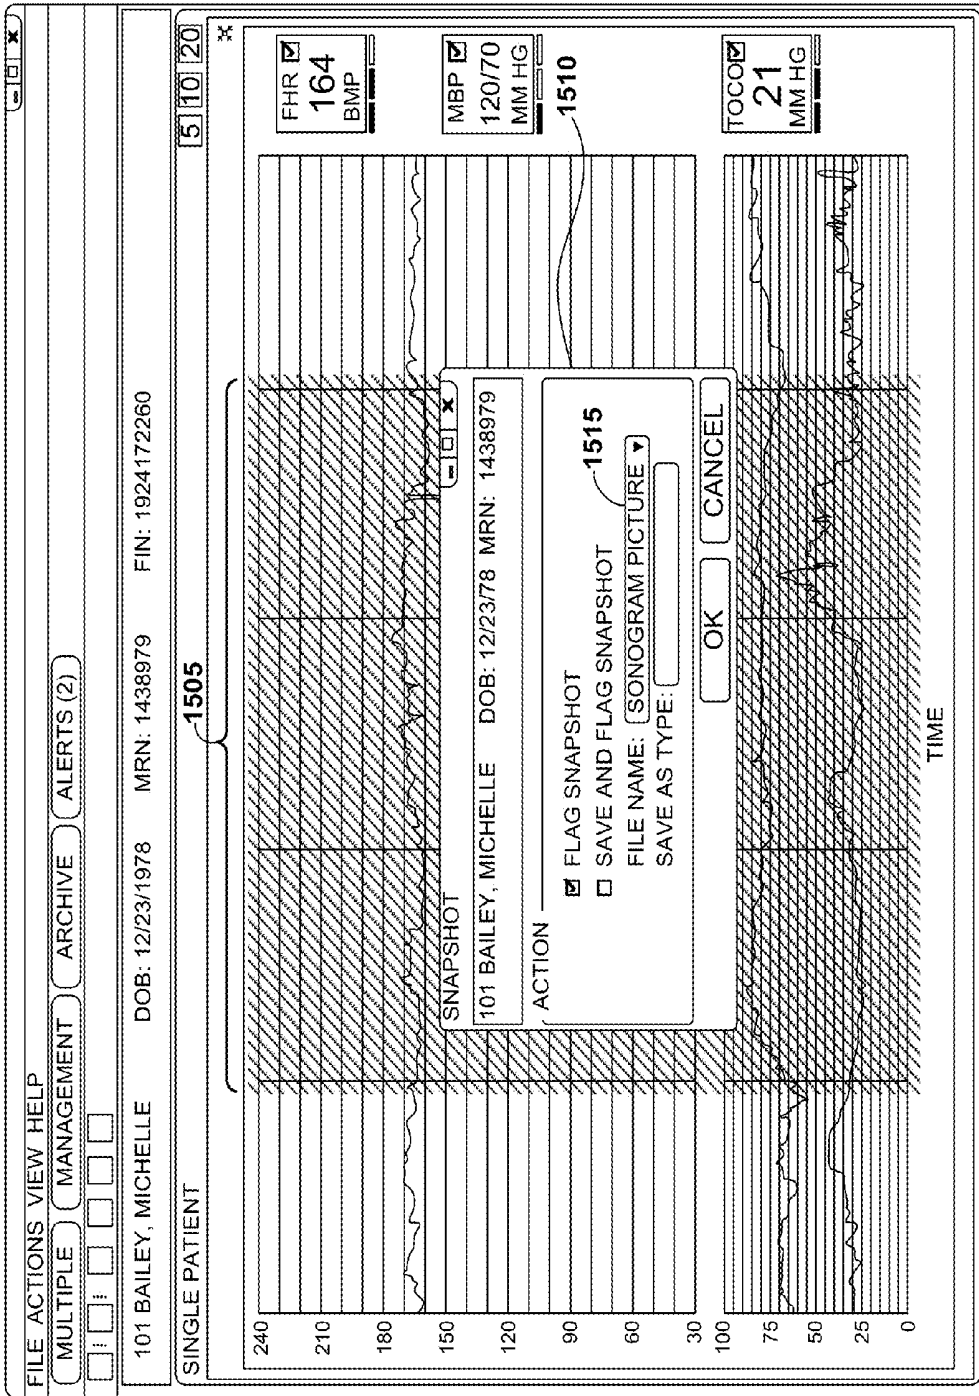

1500

FIG. 15.

1

## ELECTRONIC FETAL MONITORING APPLICATIONS AND DISPLAY

### BACKGROUND

Electronic fetal monitoring (EFM) is the use of electronic fetal heart-rate monitoring for the evaluation of fetal well-being. EFM devices are used during pregnancy, labor and birth in over 99% of patients. Clinicians base clinical decisions utilizing the waveform information produced by EFM devices. EFM devices may show fetal heart rate deceleration and acceleration patterns that are monitored by clinicians. Additional information such as heart rate, blood pressure and uterine pressure and contraction information may also be monitored. This information maybe used by clinicians to determine if a fetus is healthy or if medical intervention, such as delivery by surgical operation, is necessary.

### SUMMARY

This summary is provided to introduce a selection of concepts in a simplified form that are further described below in the Detailed Description. This summary is not intended to identify key features or essential features of the claimed subject matter, nor is it intended to be used as an aid in determining the scope of the claimed subject matter.

Embodiments of the present invention relate to methods, systems and computer storage media having computer-executable instructions embodied thereon that, when executed, cause a computing device to perform a method of displaying waveform tracings for data received from one or more medical devices. A first waveform tracing for data received from one or more medical devices for a first individual is displayed. A second waveform tracing for data received from one or more medical devices for a second individual is displayed. In response to the determination to hide the first waveform tracing, only displaying second waveform tracing.

Embodiments of the present invention relate to methods, systems and computer storage media having computer-executable instructions embodied thereon that, when executed, cause a computing device to perform a method of displaying on a user device alarm-triggering events detected by the medical device based on the location of the user device. Patient data which triggers an alarm is received from a medical device. The physical location of first and second user display devices is determined. The physical location of the first and second user display devices is independent from the users logged onto the first and second user display devices. It is determined that the physical location of the first user display device is designated to have the alarm displayed. It is determined that the physical location of the second user display device is not designated to have the alarm displayed. In response to the determinations, the content of the alarm is displayed on the first user display device and not the second user display device.

Embodiments of the present invention relate to methods, systems and computer storage media having computer-executable instructions embodied thereon that, when executed, cause a computing device to perform a method of displaying medical annotations for a patient. A first medical annotation for a patient relating to one or more of the patient's demographic information, medical condition, or status is received from a clinician. A request not to display the first annotation when annotations are displayed for the patient is received. The first annotation for the patient and the request to hide the first annotation are stored in the patient's electronic medical record. Additional medical annotations are received and

2

stored for the patient. A request from to view medical annotations for the patient is received. The stored first annotation and additional annotations are accessed for the patient. It is determined that the first annotation has been requested not to be displayed. In response to the determination, the additional patient annotations are displayed but the first annotation for the patient is not.

### BRIEF DESCRIPTION OF THE DRAWINGS

Embodiments are described in detail below with reference to the attached drawing figures, wherein:

FIG. 1 is a block diagram of an exemplary computing environment suitable for use in implementing embodiments of the present invention;

FIG. 2 is an exemplary system architecture suitable for use in implementing embodiments of the present invention;

FIG. 3 is an illustrative flow diagram of a method for displaying waveform tracings from a medical device for two individuals, in accordance with an embodiment of the present invention;

FIG. 4 is an illustrative screen display showing waveform tracings from one or more medical devices, in accordance with an embodiment of the present invention;

FIG. 5 is an illustrative screen display showing waveform tracings from one or more medical devices with at least one waveform disabled, in accordance with an embodiment of the present invention;

FIG. 6 is an illustrative screen display showing waveform tracings for multiple fetuses, in accordance with an embodiment of the present invention;

FIG. 7 is an illustrative screen display showing waveform tracings from one or more medical devices showing only one of multiple fetuses, in accordance with an embodiment of the present invention;

FIG. 8 is an illustrative flow diagram of a method for simultaneously displaying waveform tracings from one or more individuals and related medical annotations, in accordance with an embodiment of the present invention;

FIG. 9 is an illustrative screen display for allowing a user to input medical annotations for a labor and delivery patient, in accordance with an embodiment of the present invention;

FIG. 10 is an illustrative screen display showing current and historical waveform tracings and textual annotations for a patient, in accordance with an embodiment of the present invention;

FIG. 11 is an illustrative screen display showing a portion of a waveform tracing related to a medical annotation, in accordance with an embodiment of the present invention;

FIG. 12 is an illustrative flow diagram of a method for displaying alerts, in accordance with an embodiment of the present invention;

FIG. 13 is an illustrative screen display showing alerts and waveform tracings for multiple maternity patients, in accordance with an embodiment of the present invention;

FIG. 14 is an illustrative screen display showing waveform tracings for maternity patients satisfying alert conditions, in accordance with an embodiment of the present invention; and

FIG. 15 is an illustrative screen display showing the identification of a portion of the waveform tracing for a patient being monitored, in accordance with an embodiment of the present invention.

### DETAILED DESCRIPTION

The subject matter of the present invention is described with specificity herein to meet statutory requirements. How-

ever, the description itself is not intended to limit the scope of this patent. Rather, the inventors have contemplated that the claimed subject matter might also be embodied in other ways, to include different steps or combinations of steps similar to the ones described in this document, in conjunction with other present or future technologies.

Having briefly described embodiments of the present invention, an exemplary operating environment suitable for use in implementing embodiments of the present invention is described below.

Referring to the drawings in general, and initially to FIG. 1 in particular, an exemplary computing system environment, a medical information computing system environment, with which embodiments of the present invention may be implemented is illustrated and designated generally as reference numeral 20. It will be understood and appreciated by those of ordinary skill in the art that the illustrated medical information computing system environment 20 is merely an example of one suitable computing environment and is not intended to suggest any limitation as to the scope of use or functionality of the invention. Neither should the medical information computing system environment 20 be interpreted as having any dependency or requirement relating to any single component or combination of components illustrated therein.

The present invention may be operational with numerous other general purpose or special purpose computing system environments or configurations. Examples of well-known computing systems, environments, and/or configurations that may be suitable for use with the present invention include, by way of example only, personal computers, server computers, hand-held or laptop devices, multiprocessor systems, microprocessor-based systems, set top boxes, programmable consumer electronics, network PCs, minicomputers, mainframe computers, distributed computing environments that include any of the above-mentioned systems or devices, and the like.

The present invention may be described in the general context of computer-executable instructions, such as program modules, being executed by a computer. Generally, program modules include, but are not limited to, routines, programs, objects, components, and data structures that perform particular tasks or implement particular abstract data types. The present invention may also be practiced in distributed computing environments where tasks are performed by remote processing devices that are linked through a communications network. In a distributed computing environment, program modules may be located in association with local and/or remote computer storage media including, by way of example only, memory storage devices.

With continued reference to FIG. 1, the exemplary medical information computing system environment 20 includes a general purpose computing device in the form of a control server 22. Components of the control server 22 may include, without limitation, a processing unit, internal system memory, and a suitable system bus for coupling various system components, including database cluster 24, with the control server 22. The system bus may be any of several types of bus structures, including a memory bus or memory controller, a peripheral bus, and a local bus, using any of a variety of bus architectures. By way of example, and not limitation, such architectures include Industry Standard Architecture (ISA) bus, Micro Channel Architecture (MCA) bus, Enhanced ISA (EISA) bus, Video Electronic Standards Association (VESA) local bus, and Peripheral Component Interconnect (PCI) bus, also known as Mezzanine bus.

The control server 22 typically includes therein, or has access to, a variety of computer-readable media, for instance, database cluster 24. Computer-readable media can be any

available media that may be accessed by server 22, and includes volatile and nonvolatile media, as well as removable and non-removable media. By way of example, and not limitation, computer-readable media may include computer storage media. Computer storage media may include, without limitation, volatile and nonvolatile media, as well as removable and non-removable media implemented in any method or technology for storage of information, such as computer-readable instructions, data structures, program modules, or other data. In this regard, computer storage media may include, but is not limited to, RAM, ROM, EEPROM, flash memory or other memory technology, CD-ROM, digital versatile disks (DVDs) or other optical disk storage, magnetic cassettes, magnetic tape, magnetic disk storage, or other magnetic storage device, or any other medium which can be used to store the desired information and which may be accessed by the control server 22. By way of example, and not limitation, communication media includes wired media such as a wired network or direct-wired connection, and wireless media such as acoustic, RF, infrared, and other wireless media. Combinations of any of the above also may be included within the scope of computer-readable media.

The computer storage media discussed above and illustrated in FIG. 1, including database cluster 24, provide storage of computer-readable instructions, data structures, program modules, and other data for the control server 22. The control server 22 may operate in a computer network 26 using logical connections to one or more remote computers 28. Remote computers 28 may be located at a variety of locations in a medical or research environment, for example, but not limited to, clinical laboratories (e.g., molecular diagnostic laboratories), hospitals and other inpatient settings, veterinary environments, ambulatory settings, medical billing and financial offices, hospital administration settings, home health care environments, and clinicians' offices. Clinicians may include, but are not limited to, a treating physician or physicians, specialists such as surgeons, radiologists, cardiologists, and oncologists, emergency medical technicians, physicians' assistants, nurse practitioners, nurses, nurses' aides, pharmacists, dieticians, microbiologists, laboratory experts, laboratory technologists, genetic counselors, researchers, veterinarians, students, and the like. The remote computers 28 may also be physically located in non-traditional medical care environments so that the entire health care community may be capable of integration on the network. The remote computers 28 may be personal computers, servers, routers, network PCs, peer devices, other common network nodes, or the like, and may include some or all of the elements described above in relation to the control server 22. The devices can be personal digital assistants or other like devices.

Exemplary computer networks 26 may include, without limitation, local area networks (LANs) and/or wide area networks (WANs). Such networking environments are commonplace in offices, enterprise-wide computer networks, intranets, and the Internet. When utilized in a WAN networking environment, the control server 22 may include a modem or other means for establishing communications over the WAN, such as the Internet. In a networked environment, program modules or portions thereof may be stored in association with the control server 22, the database cluster 24, or any of the remote computers 28. For example, and not by way of limitation, various application programs may reside on the memory associated with any one or more of the remote computers 28. It will be appreciated by those of ordinary skill in the art that the network connections shown are exemplary and

other means of establishing a communications link between the computers (e.g., control server **22** and remote computers **28**) may be utilized.

In operation, a clinician may enter commands and information into the control server **22** or convey the commands and information to the control server **22** via one or more of the remote computers **28** through input devices, such as a keyboard, a pointing device (commonly referred to as a mouse), a trackball, or a touch pad. Other input devices may include, without limitation, microphones, satellite dishes, scanners, or the like. Commands and information may also be sent directly from a remote healthcare device to the control server **22**. In addition to a monitor, the control server **22** and/or remote computers **28** may include other peripheral output devices, such as speakers and a printer.

Although many other internal components of the control server **22** and the remote computers **28** are not shown, those of ordinary skill in the art will appreciate that such components and their interconnection are well known. Accordingly, additional details concerning the internal construction of the control server **22** and the remote computers **28** are not further disclosed herein.

Fetal monitoring module **210** may reside on one or more computing devices, such as, for example, computing device **22** described above with reference to FIG. **1**. By way of example only and not limitation, computing devices may be a server, personal computer, desktop computer, laptop computer, handheld device, mobile handset, consumer electronic device, or the like. It should be noted, however, that embodiments are not limited to implementation on such computing devices, but may be implemented on any a variety of different types of computing devices within the scope of embodiments thereof.

As previously set forth, embodiments of the present invention related to computing systems for monitoring and displaying information regarding the health of mother and baby during pregnancy, labor and delivery. With reference to FIG. **2**, a block diagram is illustrated that shows an exemplary computing system architecture for displaying and monitoring information during pregnancy, labor and delivery. It will be appreciated that the computing system architecture shown in FIG. **2** is merely an example of one suitable computing system and is not intended as having any dependency or requirement related to any single module/component or combination of modules/components.

The computing system includes one or more medical devices **205**, fetal monitoring module **210**, database **215** and graphical display **220**. Discrete data elements are received from device **205**. A medical device **205** may be any device, stationary or otherwise, that may be used to treat a patient in a hospital, doctor's office, etc. For exemplary purposes only and not limitation, medical devices include fetal heart rate monitors, blood pressure monitors, uterine pressure and contraction activity monitors, blood oxygen saturation monitors, maternal heart rate monitors, other monitors, ventilators, pumps (e.g., infusion pumps, balloon pumps), a patient's bed, sequential compression devices, electronic security devices, and the like.

Database **215** contains a variety of information data for the patient in a patient's electronic medical record (EMR). As utilized herein, the acronym "EMR" is not meant to be limiting, and may broadly refer to any or all aspects of the patient's medical record rendered in a digital format. Generally, the EMR is supported by systems configured to coordinate the storage and retrieval of individual records with the aid of computing devices. As such, a variety of types of healthcare-related information may be stored and accessed in

this way. By way of example, the EMR may store one or more of the following types of information: patient demographic; medical history (e.g., examination and progress reports of health and illnesses); medicine and allergy lists/immunization status; laboratory test results, radiology images (e.g., X-rays, CTs, MRIs, etc.); evidence-based recommendations for specific medical conditions; a record of appointments and physician's notes; billing records; and data received from an associated medical device. Accordingly, systems that employ EMRs reduce medical errors, increase physician efficiency, and reduce costs, as well as promote standardization of healthcare. Graphical display device **220** may be a monitor, computer screen, project device or other hardware device for displaying output capable of displaying graphical user interfaces.

Fetal monitoring module **210** receives and displays data from a medical device for mother and baby during pregnancy, labor and delivery. Fetal monitoring module **210** may reside on one or more computing devices, such as, for example, computing device **22** described above with reference to FIG. **1**. By way of example, computing device **22** includes a computer processor and may be a server, personal computer, desktop computer, laptop computer, handheld device, mobile handset, consumer electronic device, or the like.

Fetal monitoring module **210** comprises device data receiving component **215**, stored information receiving component **230**, graphing component **235**, receiving component **240**, determining component **245** and displaying component **250**. Device data receiving component **225**, receives discrete data from one or more medical devices **205**. It will be appreciated that while fetal monitoring module **210** is depicted as being connected to a single medical device **225**, fetal monitoring module **210** may receive discrete data from multiple medical devices including medical devices monitoring both a mother and her unborn baby.

The data received by data receiving component **225** includes device related output from the medical device. For example, data receiving component **225** may receive data from a fetal heart monitor, a maternal heart monitor, maternal blood pressure monitor, ultrasound, fetal scalp electrodes and a uterine pressure monitor. In one embodiment, the patient is continuously monitored and new data points are sent to the data receiving component **225** such that they may be plotted and displayed in a waveform quickly or in real-time.

Stored information receiving component **230** receives information from database **215** including a variety of information data for the patient in a patient's electronic medical record (EMR). By way of example, the EMR may store one or more of the following types of information: annotations regarding a patient's condition; patient demographic; medical history (e.g., examination and progress reports of health and illnesses); medicine and allergy lists/immunization status; laboratory test results, radiology images (e.g., sonogram, X-rays, CTs, MRIs, etc.); evidence-based recommendations for specific medical conditions; a record of appointments and physician's notes; billing records; and data received from an associated medical device.

Graphing component **235** converts the data received from medical device **205** into electronic waveforms that can be displayed as tracings or graphs. The term waveform refers to the shape of a graph of the varying quantity against time. Exemplary electronic waveforms for data from medical devices are shown in FIGS. **6-9**. For example, as data comes in indicating a patient's heart rate, it is graphed as function of time in a waveform. In the exemplary waveforms, the newest data is plotted on the right side of the waveform. The prior data points are to the left of the newest plotted point. Exem-

plary data that is received and may be displayed in waveform includes, but is not limited to, fetal blood oxygenation saturation level, uterine activity, maternal heart rate, maternal EKG data, maternal blood pressure, fetal heart rate (beats per minute) and maternal blood oxygen saturation level. Fetal blood oxygenation saturation level (FapO<sub>2</sub>%) may include discrete data elements such as oxygenation saturation level, CO<sub>2</sub> level, base excess and pH. Uterine activity may include discrete data elements such as uterine pressure and contraction activity of the uterine muscle (mmHG) and may be measured using tocodynamometry to determine progress of labor. Maternal heart rate is captured as beats per minute. Maternal blood pressure discrete data elements include systolic blood pressure (mmHG), diastolic blood pressure (mmHG) and mean arterial pressure (mmHG). Fetal heart rate includes beats per minute and may be captured by a monitor, ultrasound, and fetal scalp electrodes. Maternal blood oxygenation saturation level (SpO<sub>2</sub>%) may include discrete data elements such as oxygenation saturation level, CO<sub>2</sub> level, base excess and pH.

Receiving component **240** receives inputs from a user utilizing a computing device **220** with a processor such as computing device **22** of FIG. **1**. Receiving component **240** may receive a variety of inputs. For example, subcomponents of receiving component **240** receive inputs including requests to hide one or more of the waveforms, textual annotations, requests to hide one or more textual annotations, requests to save snapshots of a particular time period of the waveforms and associate the snapshots with other files, requests to view alerts, inputs of patient information and a variety of other inputs. These inputs will be discussed in more detail below. It will be appreciated that receiving component **240** comprises at least one subcomponent and may have any number of subcomponents. Alternatively, one or more subcomponents may be separate receiving components.

Determining component **245** makes a variety of determinations utilizing the input received by receiving component **210** and may have a number of subcomponents. For example, one subcomponent of determining component **245** determines to no longer display a waveform on the graphical user interface if a request to hide the waveform is received. One subcomponent of determining component **245** determines to hide annotations displayed if there has been a request to hide an annotation. Another subcomponent of determining component **245** determines an area of the one or more waveforms that is associated with the time of a selected annotation. It will be appreciated that determining component **245** comprises at least one subcomponent and may have a number of subcomponents. Alternatively, one or more subcomponents may be separate determining components.

Displaying component **250** utilizes a computer processor to display on display device **220** a variety of information. The information displayed regarding the patient's condition may come from medical device **205** and database **215**. For example, subcomponents of displaying component **250** display graphical user interfaces including information on patient alerts, number of alerts, waveforms for one or more individuals, patient information and annotations. It will be appreciated that displaying component **250** comprises at least one subcomponent and may have a number of subcomponents. Alternatively, one or more subcomponents may be separate determining components.

Referring next to FIG. **3**, a computer-implemented method **300** for determining and displaying only requested medical device waveforms for one or more individuals is shown. Computer-implemented method **300** is performed by one or more computer processors. At step **305**, monitoring data from

one or more medical devices for a first individual are received. In one embodiment, the first individual is a maternity patient. Exemplary monitoring data for the maternity patient includes heart rate data from a heart rate monitor, uterine pressure and contraction information from a uterine pressure and contraction activity monitor, blood oxygen saturation data from a blood oxygen saturation monitor(s) and blood pressure from a blood pressure monitor(s).

At step **310**, monitoring data from one or more medical devices for a second individual is received. In one embodiment, the second individual is the unborn baby of the maternity patient. Exemplary monitoring data for the unborn baby of the maternity patient includes fetal heart rate from a fetal heart rate monitor and fetal blood oxygen saturation data from a blood oxygen saturation monitor. In one embodiment, the first individual may be an unborn baby of a maternity patient and the second individual is a second unborn baby of the same maternity patient.

At step **315**, the data from the medical devices for the first and second individuals is displayed as waveform tracings. Graphing component **235** converts the data received from medical device **205** into electronic waveform tracings that can be displayed by displaying component **250** as tracings or graphs. The term waveform refers to the shape of a graph of the varying quantity against time. Exemplary electronic waveforms for data from medical devices are shown in FIGS. **6-9**.

At step **320** of FIG. **3**, a request to hide one or more of the waveforms displayed is received. In one embodiment, a user, such as a nurse or doctor, may request to hide one or more of the waveforms displayed for a first individual (e.g., patient, maternity patient or unborn baby of maternity patient) and/or second individual (e.g., patient, maternity patient or unborn baby of maternity patient). For example, and as discussed in more detail below, a user may choose to hide a waveform tracing for a maternity patient (e.g., waveform tracing not needed or is interfering with a waveform being displayed for the unborn baby). The request may be a request to hide or alternatively a request to view only certain waveforms.

At step **325**, it is determined which waveforms to display based on the request from the user. For example, if the user has requested to view only the waveform of one unborn baby from a group of multiple babies, the determining component **245** would determine to display only the waveform of the one unborn baby and not the waveforms of the other babies. In another example, only the waveform tracing(s) of the maternity patient and not the unborn baby may be selected to be displayed. At step **330**, only the waveforms as determined by determining component **245** to be displayed are displayed. Furthermore, it will be appreciated that waveform tracings for more than two babies may be displayed.

With reference to FIG. **4**, a graphical user interface embodied on a computer-storage media showing data waveforms from one or more medical devices is shown. Display **400** includes waveform tracings for a single maternity patient **405** and her unborn baby. Waveform tracings for fetal heart rate **410**, maternal blood pressure **415**, maternal heart rate **420** and tocodynamometry (TOCO) **425**. Maternal blood pressure waveform **435**, maternal heart rate waveform **420** and maternal uterine pressure and contraction waveform **425** are displayed for a first individual (maternity patient) along with fetal heart rate waveform **410** for a second individual (unborn baby of maternity patient). Display **400** also includes a display of the most recent numerical value of the data received from medical devices. Numerical measurements for patient **405** and her unborn baby for fetal heart rate **430** maternal

blood pressure **435** and TOCO **440** are displayed on the graphical user interface along with the waveform of the data.

For example, with reference to FIGS. **4** and **5**, a user has selected in FIG. **4** to hide the waveform **415** for maternal blood pressure as it interfering with fetal heart rate waveform **410** for which the clinician wants to see more clearly. The selection is received by receiving component **210** of FIG. **2**. It is determined by a subcomponent of determining component **245** that waveform **415** is no longer to be displayed. Thus, in graphical user interface **500** of FIG. **5**, waveform **415** is disabled and displaying component **250** displays the waveforms **410**, **420** and **425** and not waveform **415**.

With reference to FIGS. **6** and **7**, graphical user interfaces embodied on a computer-storage media displaying continuous data waveforms from one or more medical devices for two or more individuals is shown. Display **600** includes waveform tracings for a single maternity patient **605** and her unborn triplet babies **610**, **615**, and **620**. In one example, if one of the multiples appears to be in distress, the clinician may choose to view only the waveform of the unborn baby in distress and hide the waveforms for one or more of the other unborn babies. The selection to hide one of the waveforms is received by receiving component **240** of FIG. **2**. It is determined by determining component **245** that only waveform **615** is to be displayed. Thus, waveforms **610** and **620** are disabled and in graphical user interface display **700** of FIG. **7** displaying component **250** displays only waveform **615** and not waveforms **620** and **625**.

Referring next to FIG. **8**, a computer-implemented method **800** for determining and displaying the area of a medical device waveform for an individual corresponding to the time of a textual annotation is shown. Computer-implemented method **800** is performed by one or more computer processors. At step **805**, monitoring data from one or more medical devices for a first individual are received. In one embodiment, the first individual is a maternity patient. Exemplary monitoring data for the maternity patient includes heart rate data from a heart rate monitor, uterine pressure and contraction information from a uterine pressure and contraction activity monitor, blood oxygen saturation data from a blood oxygen saturation monitors and blood pressure from a blood pressure monitors.

At step **810**, medical annotations related to the data received from the one or more medical devices is accessed and received. Medical annotations are accessed from database **215**. The medical annotations may include textual notes, comments and observations by a clinician regarding are variety of things relating to the patient including the patient's condition, medical history, demographic information, test results and tasks and examinations performed for the patient. Common medical annotations utilized in labor and delivery may be displayed for selection by the clinician. In addition to accessing the medical annotations, any indication that one or more of the medical annotations should not be displayed is also accessed from database **215**. The input of medical annotations is described below in more detail with reference to FIG. **9**. At step **815**, it is determined whether any of the annotations accessed from database **215** should be hidden. For example, a clinician may select to have certain annotations hidden at the time of entry or thereafter.

If it is determined that no annotations have been requested to be hidden at step **815**, all related annotations are displayed at step **818**. If it is determined that one or more annotations for the patient are to be hidden, at step **820**, only annotations not identified to be hidden are displayed. At step **822**, data from the medical devices for the first and second individuals is displayed as waveforms. As discussed above, the data from

the medical devices is converted into electronic waveforms that can be displayed as tracings or graphs.

In one embodiment, at step **825**, a user may select one or more of the annotations displayed at steps **820** and **822**. The user may choose to view the related portion of a waveform tracing for the annotation by selecting or clicking on the annotation. At step **830**, the associated area of one or more displayed waveforms is determined. For example, if an annotation was documented as occurring at 8:00 p.m., the area of one or more of the associated waveform for 8:00 p.m. for the individual is displayed. This may be done on a waveform with the most current data or in a separate waveform with historical data. In one embodiment, the current data waveform is displayed simultaneously with a historical data waveform for the individual and the area. This is described below in more detail with reference to FIG. **10**.

As shown in FIG. **9**, an exemplary graphical user interface **900** for allowing a user to input medical annotations for a labor and delivery patient is shown. As depicted in FIG. **9**, the annotation box **905** is displayed along with waveform of medical device data for the maternity patient and unborn baby. Textual annotations may be input by a clinician into text box **910**. Common medical annotations **915** for labor and delivery that may be selected by a clinician include, but are not limited to, increase IV fluids, O<sub>2</sub> 8-10 L/Min per FM, oxytocin infusion discontinued, oxytocin infusion increased, primary provider at bedside, primary provider notified, pushing, tocolytic administration, patient turned to left side and vaginal examination. The clinician may select sign button **925** to send and store any annotations made. The annotations along with the associated time and date when the annotation was made are then stored in database **215**.

With regard to FIG. **9**, a user, such as a nurse or doctor, may enter or select an annotation and choose to have it hidden for privacy reasons by selecting check box **1520**. For example, sensitive information about the maternity patient, such as past pregnancies, terminated pregnancies, medical conditions (e.g., sexually transmitted diseases) and demographic information (e.g., weight) may be selected to be hidden by the clinicians so that non-medical personnel in the patient's room cannot see the annotations. Non-medical personnel may include persons in a non-medical care giving role such as family and friends of the patient and personnel of the health-care facility that have no need to know the medical information contained in the annotation. This annotation and the selection to "hide" the annotation are stored in a database, such as database **215**.

With reference to FIG. **10**, an exemplary graphical user interface **1000** for displaying waveform data and related medical annotations for a patient is shown. As depicted in FIG. **10**, medical annotations **1005** are in an area on the user interface **1000** separate from the display areas of current **1015** and historical **1020** waveform tracings for the patient. The current waveform tracing **1015** has the most recent data for the patient from one more medical devices. Historical waveform tracing **1020** has historical data for the patient from one or more medical devices for a specific time period. In this example, the exemplary specific historical time period for the patient is from 6 a.m. to 7 a.m. on Oct. 27, 2007. Medical annotations **1005** for the patient are listed from the most recent to the oldest. For example, medical annotation **1010** of maternal blood pressure and maternal heart rate is the most recent medical annotation for the patient.

Referring next to FIG. **11**, an exemplary graphical user interface **1100** for displaying current, historical and archived waveform tracings along with medical annotations for a patient is shown. As depicted in FIG. **11**, medical annotations

**1105** are in an area on the user interface **1100** separate from the display areas of current **1120**, historical **1125** and archived **1130** waveform tracings of data for the patient from one or more medical devices. The time frame on a waveform associated with a selected medical annotation is displayed. The current waveform tracing **1120** has the most recent data for the patient from one or more medical devices on Oct. 27, 2007. Historical waveform tracing **1125** has historical data for the patient from one or more medical devices for a specific time period. In this example, the exemplary specific historical time period for the patient is from 6 a.m. to 7 a.m. on Oct. 27, 2007 which is an earlier time period of the same visit of the patient as the current **1120** waveform tracing. For example, the same visit of the patient may be an admission to a hospital or a doctor's visit. Archived waveform tracing **1130** is for a different visit of the patient on Oct. 13, 2007. In this example, the archive view includes annotations **1115** and waveform tracing **1130** for a previous hospital admittance or doctor's visit for the patient.

As described with reference to FIG. 8, a user may select one of the annotations **1110** and **1115** to view the related portion of the corresponding current **1120**, historical **1125** or archived **1130** waveform tracing. For example, if annotation **1110** (made at 8:10 a.m. on Oct. 27, 2007) is selected by a user, the associated time period (8:00 to 9:00 a.m. on Oct. 27, 2007) on of the historical waveform tracing **1125** is displayed. An identification **1135** of the time corresponding to the time of the annotation (8:10 a.m. on Oct. 27, 2007) is displayed on waveform tracing **1125**. If the user selects annotation **1115**, the associated time period of the archived annotation is displayed on the archived waveform tracing **1130**. An identification **1140** of the time corresponding annotation time is displayed on archived waveform tracing **1130**.

Referring next to FIG. 12, a computer-implemented method **1200** for displaying patient alert information based on location is shown. Computer-implemented method **1200** is executed by one or more computer processors. At step **1205**, monitoring data from one or more medical devices for a patient is received. In one embodiment, the patient is a maternity patient or an unborn baby. Exemplary monitoring data is described above.

At step **1210**, it is determined that the monitoring data received satisfies a rule that would trigger an alert. Exemplary rules include determining data for a heart rate is outside of a specified range, a patient's blood pressure outside of a specified range, uterine pressure and contraction data outside of a specified range, blood oxygen levels outside of a specified range and other data outside of a specified range. At step **1215**, it is determined whether the location of the device displaying patient information is to be alerted. The determination is based on the physical location of the device and is not dependent on which user is logged on or signed into the device. In some instances, based on location of the device, all alerts for all patients are to be displayed. For example, a nurse manager may want to see all alerts for all patients. In some instances, based on the location of the display device, all alerts for only some patients are to be displayed. For example, if a floor is divided into multiple nursing units, each nursing unit including four patient rooms, only alerts for the patients in the patient rooms of the nursing unit will be displayed on devices located in the nursing unit. In some instances, based on the location of the display device, no alerts are to be displayed and only the number of alerts is to be displayed. For example, as the caregivers in the operating or c-section room cannot leave to respond to any alerts, an operating or c-section room may be designated as a location to display only the number of alerts and not the actual alert information.

At step **1220**, if it is determined the display device location is not to display the content of the alerts; only the number of alerts is displayed. Alternatively, no information is displayed. At step **1225**, if it is determined that the display device location is to display the alerts and alert content, the alert, alert content and total number of current alerts are displayed. In one embodiment, the alert and alert content are displayed at the display device location.

Referring next to FIG. 13, an exemplary graphical user interface **1300** displaying waveform tracings of monitored data for multiple maternity patients **1315**. Based on the location of the display device being utilized to display graphical user interface **1300**, all alerts for all patients are displayed. It can be seen in exemplary graphical user interface **1300** that exemplary patients Anna Long **1320** and Jane Cooper **1325** are highlighted and are in alert. In addition, the total number of alerts **1305** is displayed on the graphical user interface so that a user can see how many alerts there are and identify necessary personnel to address the alerts. In this example, there are a total of two (2) **1310** patients in alert. A user may choose to view only waveform tracings for those patients with alerts. In one embodiment, this is done by selecting alert button **1305**.

Referring next to FIG. 14, an exemplary graphical user interface **1400** displaying waveform tracings for patients with alerts **1425** is shown. Graphical user interface **1400** includes the waveform tracings for fictitious patient Michelle Bailey **1410** and Anna Long **1415**. A user may select to suspend, cancel and/or enter a textual annotation **1425** for the patient regarding the alert from graphical user interface **1400**. The total number patients with alerts **1420** is displayed on the graphical user interface.

FIG. 15 is an exemplary graphical user interface **1500** allowing a user to flag and store a portion of a waveform tracing **1505**. Graphical user interface **1500** includes multiple waveform tracings for fictitious patient Michelle Bailey. A user, such as a nurse or clinician, flags a portion of the waveform tracing **1505**. The user may then select to associate the portion of the waveform tracing **1505** with additional information for the patient such as textual entries, pictures, video, sonogram photographs, sonogram video, laboratory results and other stored files for the patient that relate to the time period of the waveform tracing **1505**. For example, the portion of the waveform tracing **1505** may be for the period while a sonogram was being performed for the patient.

Many different arrangements of the various components depicted, as well as components not shown, are possible without departing from the scope of the claims below. Embodiments of our technology have been described with the intent to be illustrative rather than restrictive. Alternative embodiments will become apparent to readers of this disclosure after and because of reading it. Alternative means of implementing the aforementioned can be completed without departing from the scope of the claims below. Certain features and subcombinations are of utility and may be employed without reference to other features and subcombinations and are contemplated within the scope of the claims.

The invention claimed is:

1. Non-transitory computer storage media having computer-executable instructions embodied thereon that, when executed, cause a computing device to perform a method of displaying waveform tracings for data received from one or more medical devices, the method comprising:

receiving a first set of medical annotations at a time, t, the first set of medical annotations comprising user-inputted textual notes, comments, and observations related to one or more of a first individual's demographic information,

13

medical condition, or status, wherein the time,  $t$ , corresponds to a first hospital admittance or doctor's visit for the first individual;

receiving an indication that a first medical annotation of the first set of medical annotations be hidden; 5

storing the first set of medical annotations in a database including storing the indication that the first medical annotation be hidden;

receiving a first set of data from a medical device for the first individual at the time,  $t$ , the medical device monitoring the first individual for one of maternal uterine activity or maternal heart rate activity at the time,  $t$ ; 10

storing the first set of data from the medical device in the database;

receiving a second set of data from the medical device for the first individual at a current time,  $t_1$ , the medical device monitoring the first individual for one of maternal uterine activity or maternal heart rate activity at the current time,  $t_1$ , wherein the current time,  $t_1$ , corresponds to a second hospital admittance or doctor's visit for the first individual, the second hospital admittance or doctor's visit occurring at a different date and time than the first hospital admittance or doctor's visit; 20

converting the second set of data into a first waveform tracing; 25

accessing from the database the first set of medical annotations database including the indication that the first medical annotation be hidden;

displaying, except for the first medical annotation, on a user interface the user-inputted textual notes, comments, and observations comprising the first set of medical annotations simultaneously with the first waveform tracing; 30

subsequent to displaying, except for the first medical annotation, on the user interface the user-inputted textual notes, comments and observations comprising the first set of medical annotations simultaneously with the first 35

14

waveform tracing, receiving a user selection of a second medical annotation of the first set of medical annotations;

accessing from the database the first set of data and converting the first set of data into a second waveform tracing; and

while continuing to display, except for the first medical annotation, the first set of medical annotations and the first waveform tracing, displaying on the user interface the second waveform tracing, wherein the second waveform tracing includes an indication of the time,  $t$ , at which the first set of data from the medical device was received.

2. The media of claim 1, further comprising: subsequently receiving a user input to hide at least the first waveform tracing or the second waveform tracing; and in response to receiving the subsequent user input, hiding the at least the first waveform tracing or the second waveform tracing.

3. The media of claim 1, further comprising: displaying additional waveform tracings for the first individual.

4. The media of claim 1, wherein the first individual is a maternity patient.

5. The media of claim 4, further comprising: while displaying the first and second waveform tracings on the user interface, displaying a third waveform tracing on the user interface, the third waveform tracing corresponding to a third set of data received from one or more medical devices for a second individual, wherein the second individual is an unborn baby of the maternity patient, and wherein the one or more medical devices monitor the second individual for one of fetal blood oxygenation saturation levels or fetal heart rate for the unborn baby.

6. The media of claim 5, further comprising: displaying additional waveform tracings for the second individual.

\* \* \* \* \*

专利名称(译)	电子胎儿监护应用和显示		
公开(公告)号	<a href="#">US9002441</a>	公开(公告)日	2015-04-07
申请号	US12/564569	申请日	2009-09-22
[标]申请(专利权)人(译)	CERNER创新		
申请(专利权)人(译)	CERNER创新, INC.		
当前申请(专利权)人(译)	CERNER创新, INC.		
[标]发明人	HEIL CHRISTOPHER FLORES JEREMY GEORGE CAROL		
发明人	HEIL, CHRISTOPHER FLORES, JEREMY GEORGE, CAROL		
IPC分类号	A61B5/04 A61B5/00 A61B5/0444		
CPC分类号	A61B5/0444 A61B5/0011 A61B5/411 A61B5/4362 A61B5/746 A61B5/7282 A61B5/742		
审查员(译)	帕特尔NIKETA		
其他公开文献	US20110071414A1		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

摘要(译)

提供了用于管理医疗保健环境的系统，方法和计算机可读介质。在实施例中，显示针对从第一个体的一个或多个医疗设备接收的数据的第一波形跟踪。显示针对第二个体从一个或多个医疗设备接收的数据的第二波形跟踪。响应于隐藏第一波形跟踪的确定，仅显示第二波形跟踪。

