



US 20170347894A1


(19) **United States**(12) **Patent Application Publication**
Bhushan et al.(10) **Pub. No.: US 2017/0347894 A1**(43) **Pub. Date: Dec. 7, 2017**(54) **SYSTEM AND METHOD FOR CONTINUOUS
MONITORING OF BLOOD PRESSURE***A61B 5/021* (2006.01)*A61B 5/024* (2006.01)(71) Applicant: **Fourth Frontier Technologies Pvt.
Ltd., Bangalore (IN)**(52) **U.S. Cl.**CPC *A61B 5/0205* (2013.01); *A61B 5/14546*
(2013.01); *A61B 5/0402* (2013.01); *A61B 5/11*
(2013.01); *A61B 5/14542* (2013.01); *A61B*
5/746 (2013.01); *A61B 5/681* (2013.01); *A61B*
5/02416 (2013.01); *A61B 5/6832* (2013.01);
A61B 5/021 (2013.01); *A61B 2562/0219*
(2013.01)(72) Inventors: **Manav Bhushan, Noida (IN); Sandeep
Sibal, Bangalore (IN)**(73) Assignee: **Fourth Frontier Technologies Pvt.
Ltd., Bangalore (IN)**(21) Appl. No.: **15/373,753**(22) Filed: **Dec. 9, 2016**(30) **Foreign Application Priority Data**

Jun. 3, 2016 (IN) 201641019151

Jun. 3, 2016 (IN) 201641019197

Publication Classification(51) **Int. Cl.***A61B 5/0205* (2006.01)*A61B 5/0402* (2006.01)*A61B 5/00* (2006.01)*A61B 5/145* (2006.01)*A61B 5/11* (2006.01)**ABSTRACT**

The present invention describes a system and method for continuous monitoring of central (aortic) and peripheral Blood Pressure. The system includes a fully mobile, non-invasive, continuous blood pressure monitoring system that includes one or more Biostrip devices affixed on a user, coupled with an application running on a computing device, which is further connected to a web server in the cloud. The system performs various computations on the Biostrip device, or on the gateway device (Smartphone or Smart-watch), or on the Cloud, and provides the user and authorized third parties with various insights about the blood pressure levels of the user. Further, the system enables the user to receive biofeedback training for controlling hypertension, and schedule online appointments, pay online for such appointments, share data the data securely to obtain insights.

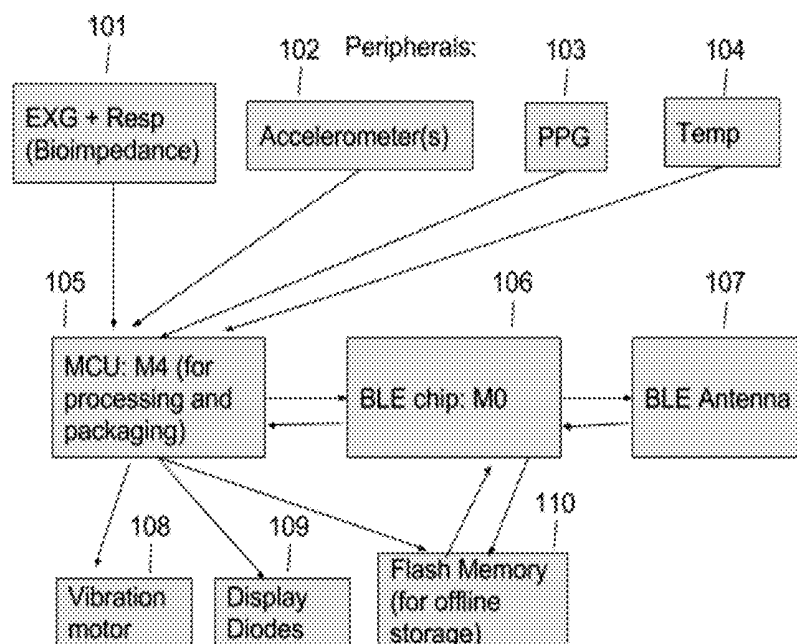Schematic Layout for Data Transfer**Schematic layout of the device and data transfer protocol in one particular****embodiment.**

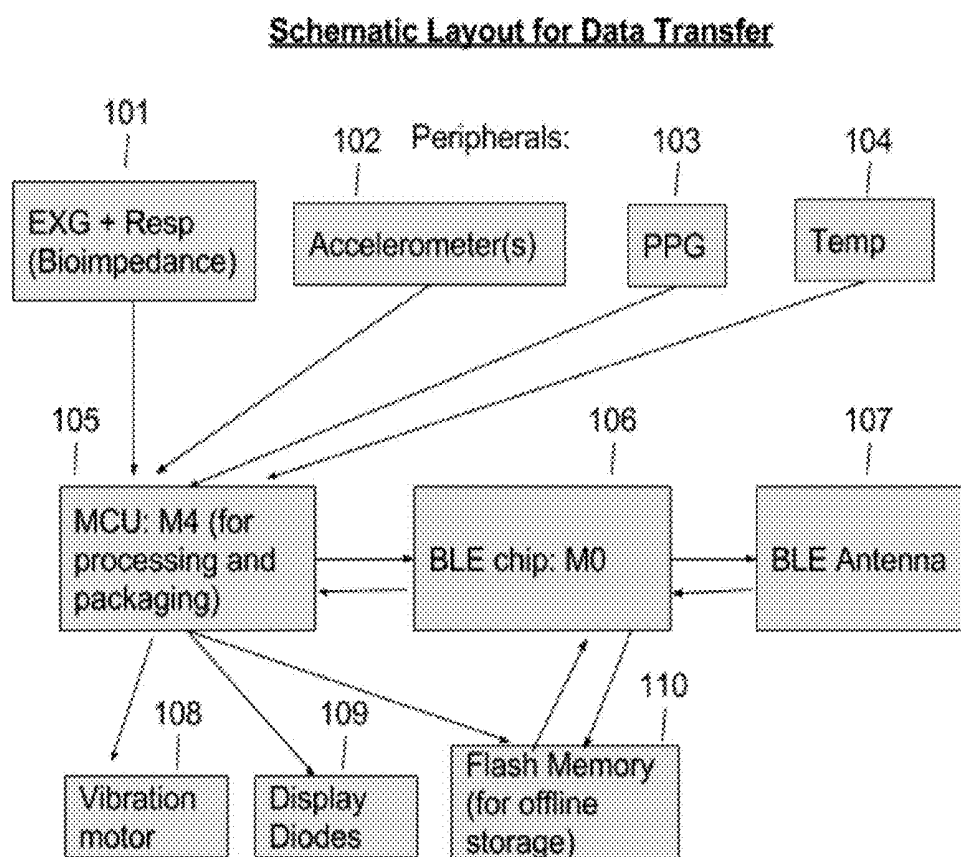


Fig 1: Schematic layout of the device and data transfer protocol in one particular embodiment.


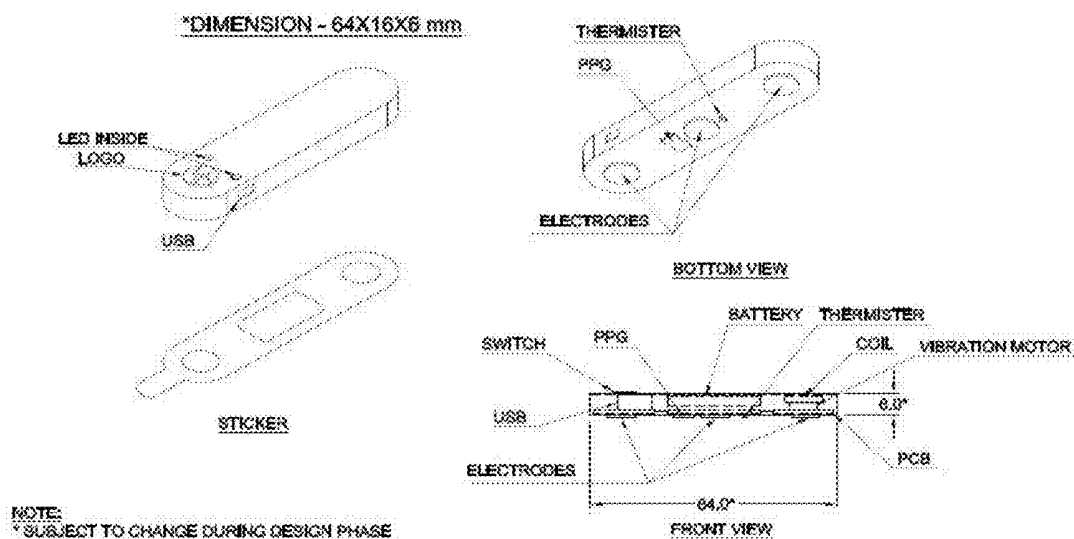


Fig. 2: Biostrip device and sticking mechanism in one embodiment.

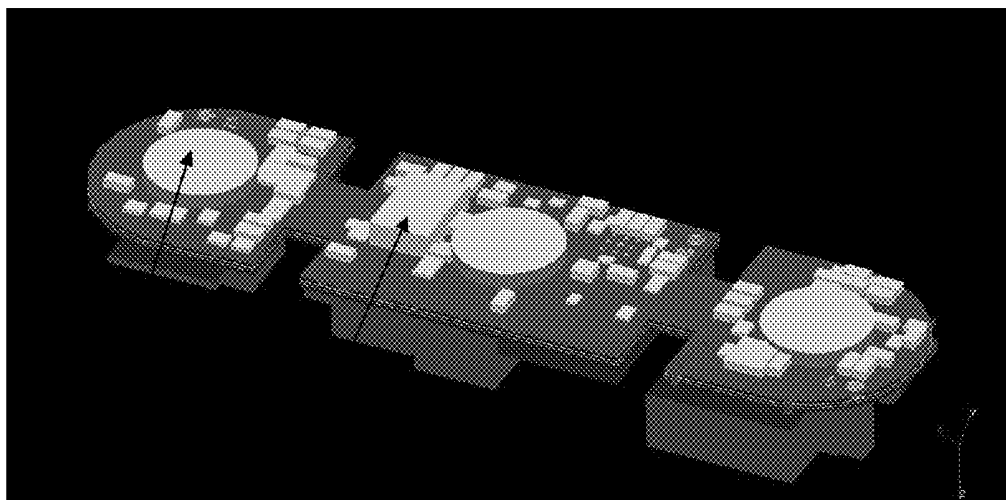

111

112

FIG. 3: 3D layout of the device in one embodiment.

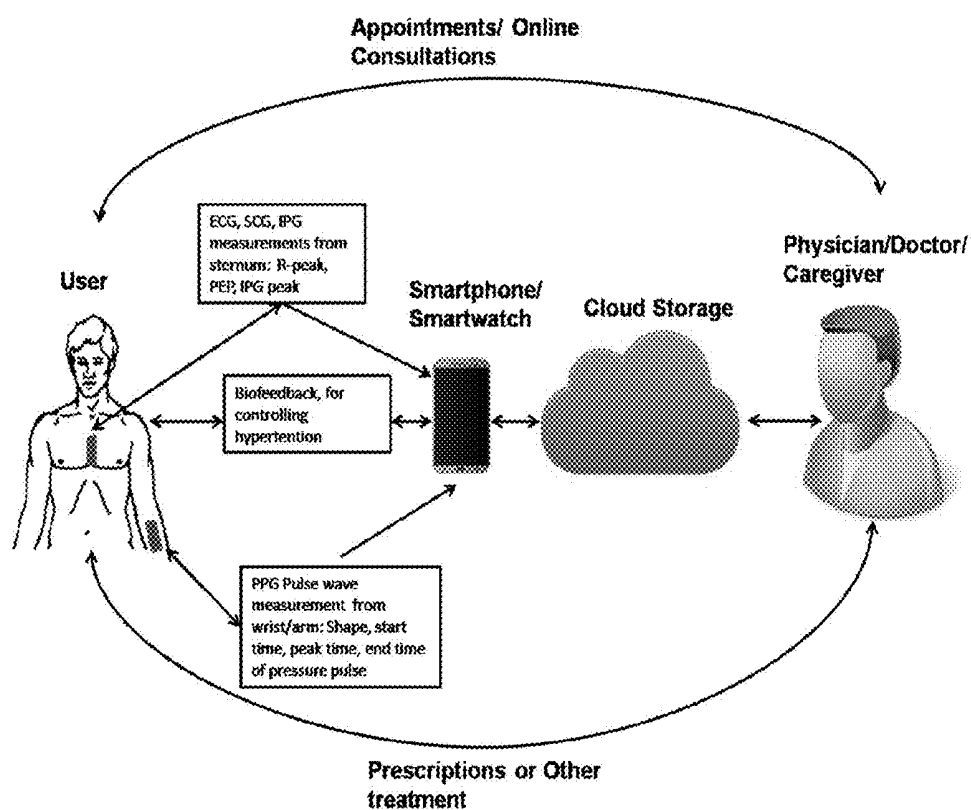


Fig 4: Schematic layout of the complete Blood Pressure monitoring system protocol in one particular embodiment.

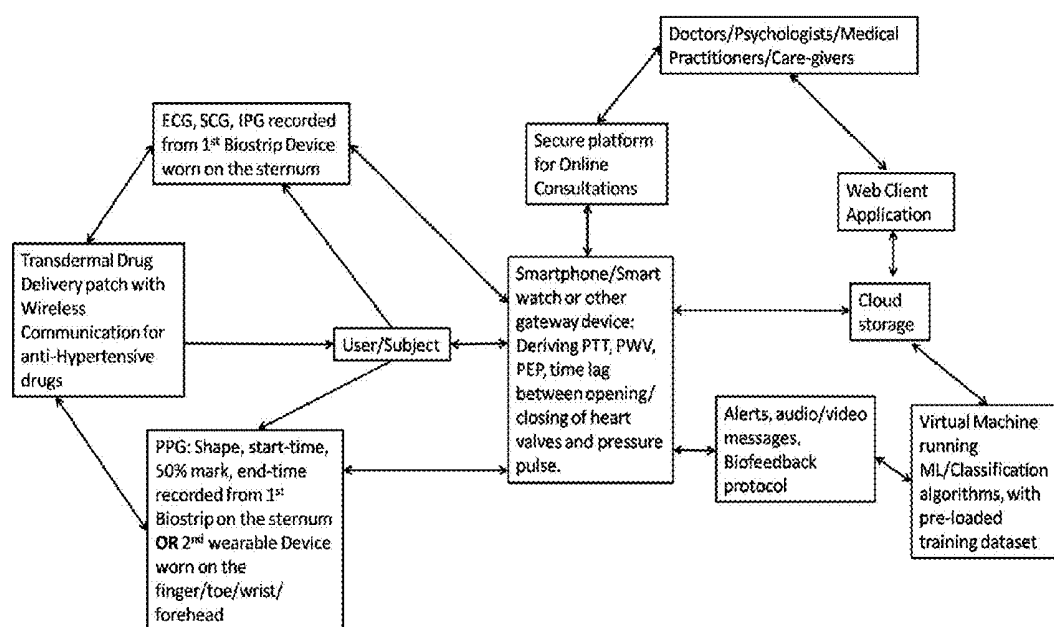


Fig. 5: Detailed mechanism for data transfer, storage and processing of the Blood

Pressure monitoring system in one particular embodiment.

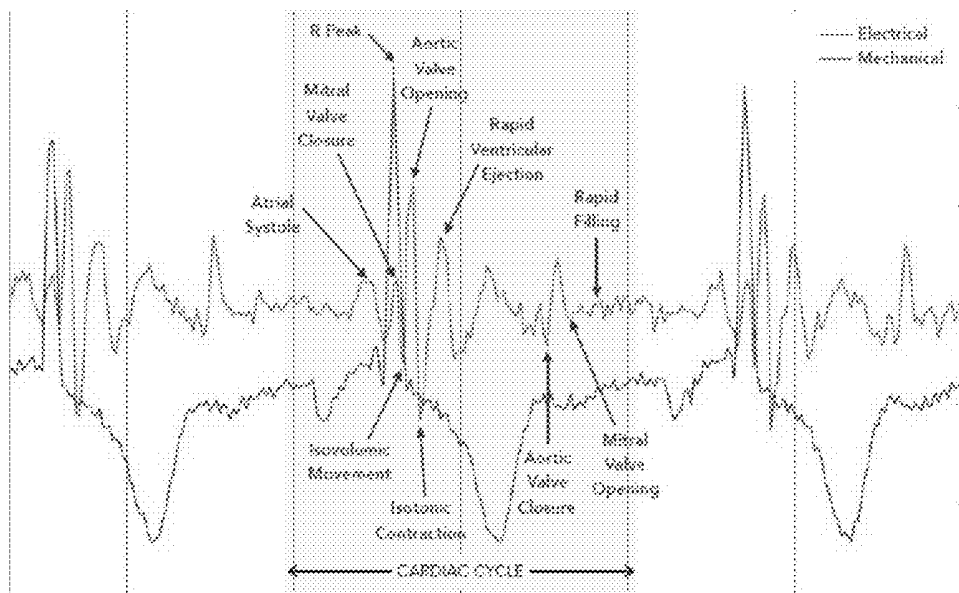


Fig. 6: Detailed cardiac cycle, as observed from the electrical and mechanical sensors present on the Biostrap device placed on the sternum.

SYSTEM AND METHOD FOR CONTINUOUS MONITORING OF BLOOD PRESSURE

TECHNICAL FIELD

[0001] The present invention relates generally to medical devices. More particularly, the invention relates to continuous medical monitoring and wearable devices used for monitoring blood pressure.

BACKGROUND OF THE INVENTION

[0002] The demand for wearable health monitoring devices and systems is increasing due to rapid development in technology, increasing health costs, aging population, and the like. To address this demand, a variety of prototypes and commercial products have been produced, aimed at providing real-time feedback about the patient's health condition, either to the user himself or to a medical professional, while also being capable of alerting an individual when possible life-threatening health conditions occur.

[0003] Conventional wearable systems usually collect medical data from only a single sensor, in periodic increments. Hence, there is a need for a system and method for a wearable device having an efficient and effective monitoring system that collects continuous data. Further, there is a need for a system and method for alerting the patient through a vibration or alerts on a phone or watch.

[0004] According to the Health Technology Assessment program, which is part of the NIH, Hypertension is defined as "persistently high blood pressure (BP), with currently accepted thresholds in the UK at 140/90 mmHg. It is one of the most prevalent and powerful risk factors contributing to the development of cardiovascular disease (CVD), and one of the most important preventable causes of premature morbidity and mortality in developed and developing countries. The estimated lifetime risk of middle-aged men and women developing hypertension is 80-90%. The most common type of hypertension is essential hypertension, which has no known cause, and has an estimated prevalence of 30.6%. Currently available treatment options typically include lifestyle changes, dietary restrictions and pharmacological agents.

[0005] The predominant measurement technique for measuring BP is through a cuff-based device placed on the upper arm, which occludes the blood flow to measure systolic BP, and then slowly deflates, either mechanically or manually, to measure diastolic BP. However, such a cuff-based device is quite cumbersome, and not conducive for continuous, 24/7 monitoring. Further, the cuff-based monitors measure only peripheral (not central) BP, when it is known that central (aortic) BP is a much better correlate of cardio-vascular disease and other abnormalities. Further, without continuous monitoring of BP, it is impossible to track the effect of different kinds of environmental factors, and therapeutic intervention upon the BP levels.

[0006] In order to overcome the challenge of continuous, non-invasive blood pressure measurement, a small self-contained, cuff-less device capable of monitoring central (aortic) and peripheral blood pressure is required.

[0007] The above-mentioned shortcomings, disadvantages and problems are addressed herein.

OBJECTS OF THE INVENTION

[0008] The various embodiments of the present invention provide a system and method for a continuous health monitoring of a user using a wearable device. An object of the present invention is to provide, and is also one or more of, a wireless, reusable, rechargeable, flexible, light-weight wearable device that monitors various physiological parameters (in particular, Blood Pressure) of the user continuously.

[0009] Another object of the present invention is to transmit the monitored data to a computing device such as a smartphone or a smartwatch or other gateway device through wireless communication such as Bluetooth (a trademark of Bluetooth SIG, Inc.), ZigBee (a trademark of the Zigbee Alliance) or other Near-Field Communication ("NFC") protocol.

[0010] Yet another object of the present invention is to collect medical quality data from a plurality of sensors including, but not limited to Electromyography ("EMG"), Electrocardiography ("ECG" or "EKG"), Electroencephalography ("EEG"), EXG, respiration, Photoplethysmograph ("PPG") temperature sensors, accelerometers and the like, and transmit the data to the required computing device after initial processing.

[0011] Various embodiments of the present invention provide a system and method for a continuous central (aortic) and peripheral blood pressure monitoring system using one or more wearable devices. The system includes one or more wearable devices (referred to herein alternatively as the "BioStrip" device), coupled with an application running on a computing device such as a smartphone, smartwatch, and the like, which is connected to a web server in the cloud, and performs various computations on the wearable device, or the computing device, or a cloud computing device where the data is stored, and more computationally intensive processes are performed.

[0012] Another object of the present invention is to combine information obtained by the sensors of the wearable device for analyzing and monitoring blood pressure. This includes processing and cleaning the signal, and quantifying the quality of each individual signal, in a manner described herein.

[0013] Yet another object of the present invention is to transmit alerts to the user and to one or more authorized contacts when there is a variation of the blood pressure beyond a pre-determined threshold.

[0014] Yet another object of the present invention is to automatically trigger a biofeedback protocol through a mobile application in an audio or a video format, to control the blood pressure of the user.

[0015] Yet another object of the present invention is to facilitate automatic storage of the blood pressure data in a secure location on the cloud and allow concerned personnel to view the data easily through a web client.

[0016] Yet another object of the present invention is to allow the users to schedule appointments online and pay consultation fees through a payment gateway.

[0017] The various embodiments of the present invention provide a system and method for continuous blood pressure monitoring using one or more wearable devices. The present system provides a complete blood pressure monitoring system that has the ability to perform non-invasive, fully mobile, and continuous (as opposed to episodic), cuff-less monitoring of central (aortic) and peripheral blood pressure levels.

[0018] The present invention provides a blood pressure monitoring system has the ability to combine information from multiple sensors—ECG, Respiration (from skin impedance), Implantable Pulse Generator (“IPG”), PPG, Galvanic Skin Response device (“GSR”), Electrodermal activity (“EDA”), movement (from accelerometers), seismocardiography (“SCG”), skin temperature, blood glucose, levels of oxygen and haemoglobin in the blood, and hence calculate a very accurate value of blood pressure for each user, and also show correlations with other parameters.

[0019] The present invention provides the blood pressure monitoring system described herein allowing the wearable device (biostrip) to send automatic alerts to user, and authorized third party contacts, when abnormal blood pressure levels are detected. Such alerts are delivered by way of messages on the smartphone/smartwatch, or using a display or vibration motor on the device itself.

[0020] The present invention includes the ability to automatically trigger a biofeedback protocol through the mobile application in audio/video format, to reduce the blood pressure levels of the user, and control situations of hypertension.

[0021] The present invention facilitates automatic storage of all the blood pressure data in a secure location on the cloud, and allows doctors and care-givers to view this data easily through a web client, at their own convenience.

[0022] Further, the system allows the user to consult doctors/psychologists or care-givers online, or book appointments with doctors through online, and pay consultation fee through payment gateway, thus completing the loop between diagnosis and treatment.

[0023] In one embodiment, the blood pressure monitoring system also couples with a transdermal drug delivery mechanism, and is used to automatically control the dosage of the drug being delivered to treat the user for hypertension or hypotension.

[0024] These and other objects and advantages of the present invention will become readily apparent from the following detailed description taken in conjunction with the accompanying drawings.

SUMMARY OF THE INVENTION

[0025] The various embodiments of the present invention provide a system and method for continuous health monitoring of the user. The system includes a wearable device that is reusable, rechargeable and coupled with a disposable two-sided sticker, which together form a patch called a ‘Biostrip device’. The wearable device includes a plurality of electrodes, an electronic circuitry to measure electric potentials for one or more channels, a circuitry for measuring electric impedance on the skin using electrodes, and one or more accelerometers along with a reflectance-based PPG module. The wearable device is designed to measure the EXG (which refers to a combination of ECG, EEG, and EMG), heart rate, respiration cycles, blood oxygenation, seismocardiography (SCG), subject movements, blood pressure, blood glucose and levels of Haemoglobin (Hb) and other blood gases (such as Carbon Dioxide) of the user.

[0026] In particular, the present invention describes a non-invasive, wireless, fully mobile and continuous blood pressure monitoring system that works in conjunction with a plurality of wearable devices, and allows the user to transmit the monitored data securely to a concerned person. The device further allows for scheduling appointments and

conducting online consultations with physicians and other medical experts when required. The system monitors health parameters including, but not limited to: ECG, Seismocardiograph (SCG), impedance plethysmography (IPG), electrodermal Activity (EDA), skin temperature, blood oxygenation, and perhaps including: CO₂ levels in the blood, haemoglobin levels in the blood and blood glucose levels: to give the user comprehensive information about the blood pressure levels, and variations of the pressure levels in accordance with the other parameters mentioned herein. The system described here has the ability to record medical data from multiple users, and to then use machine learning algorithms to derive insights and provide recommendations for each particular user, and to facilitate online consultations with data sharing.

[0027] These and other aspects of the embodiments herein will be better appreciated and understood when considered in conjunction with the following description and the accompanying drawings. It should be understood, however, that the following descriptions, while indicating the preferred embodiments and numerous specific details thereof, are given by way of an illustration and not of a limitation. Many changes and modifications may be made within the scope of the embodiments herein without departing from the spirit thereof, and the embodiments herein include all such modifications.

BRIEF DESCRIPTION OF THE DRAWINGS

[0028] The other objects, features and advantages will occur to those skilled in the art from the following description of the preferred embodiment and the accompanying drawings in which:

[0029] FIG. 1 is a system diagram illustrating the different component blocks of the Biostrip device, according to one particular embodiment of the present invention.

[0030] FIG. 2 illustrates the 3D design, and mechanism for wearing the device, according to one particular embodiment of the present invention. It is to be noted that instead of using a double-sided sticker to affix the device, the device may also be affixed with the help of a strap or other such accompaniment.

[0031] FIG. 3 illustrates the 3D layout of the device, according to one particular embodiment of the present invention. The two narrower parts in the middle of the three larger parts indicate the flexible portion of the Biostrip device, which allow it to adhere to irregular surfaces.

[0032] FIG. 4 illustrates a system diagram that shows the process of monitoring the blood pressure levels of the user, according to an embodiment of the present invention.

[0033] FIG. 5 illustrates a block diagram for the data analysis of the monitored data, according to an embodiment of the present invention.

[0034] FIG. 6 shows the ECG signal obtained from the electrical sensors, overlaid with the SCG signal obtained from the mechanical sensors on board the device.

[0035] Although the specific features of the present invention are shown in some drawings and not in others. This is done for convenience only as each feature may be combined with any or all of the other features in accordance with the present invention.

DETAILED DESCRIPTION OF THE INVENTION

[0036] In the following detailed description, reference is made to the accompanying drawings that form a part hereof, and in which the specific embodiments that may be practiced is shown by way of illustration. These embodiments are described in sufficient detail to enable those skilled in the art to practice the embodiments and it is to be understood that the logical, mechanical and other changes may be made without departing from the scope of the embodiments. The following detailed description is therefore not to be taken in a limiting sense.

[0037] The various embodiments of the present invention provide a system and method for continuous monitoring of a user's health. The system includes a wearable device and corresponding computing device. The wearable device (hereon referred to as the "Biostrap" device) includes an electronic module or a component that is reusable and rechargeable (via micro-USB or wirelessly or both) and is stuck on one side with a two-sided adhesive tape, which is meant for a single use only. For each use, the user peels off one side of the sticker, affixes it to the underside of the device, then peels of the other side, and affixes the wearable device (Biostrap) on himself/herself. The entire wearable device (Biostrap) is thus stuck on the user and is completely wireless and self-contained. Though it is to be noted that in another embodiment, the device may be affixed to different locations on the user's body with the help of flexible straps.

[0038] The system includes one or more small wearable, rechargeable Biostraps, along with a gateway device (such as a Smartphone or Smartwatch). One exemplary Biostrap is constructed on three hard printed circuit boards ("PCBs") connected by two flexible connecting PCBs that contain a number of physiological monitors (described below), a processor or microcontroller ("MCU"), a wireless communication hub, a vibration motor, a USB port for charging and data transfer, LEDs, switches, a wireless recharging coil, and several other accompanying components.

[0039] The wearable device may include two or more electrodes connected to a single analog front end system, which further transmits the signal to an analog-to-digital converter (ADC) and then on to an MCU, which together measure an electrical signal of the Electro Cardio Gram (ECG) when stuck on the chest, or EEG when stuck on the forehead, or EMG when stuck on a muscle, or a combination of all three. These parameters are collectively referred to herein as EXG.

[0040] The Biostrap device includes a reflective Photoplethysmograph ("PPG") module attached to the underside of the device, and in direct visual contact with the skin on the chest/wrist/forehead or other location where the device adheres. The PPG module includes two or more LEDs, and one or more photodiodes, which measure the changes in the intensity of reflected light of different wavelengths. The PPG module is capable of measuring blood oxygenation, as well as levels of Haemoglobin, and other blood gases, such as CO₂ and is also capable of measuring heart rate, and other measures derived from changes in blood flow.

[0041] The wearable (Biostrap) device includes one or more accelerometers capable of measuring acceleration below a predetermined resolution level. For example, the resolution is set to 0.5 milli-Gs (G-forces, also known as G's, are the units to measure acceleration) or less, and hence capable of measuring steps, breathing, heartbeats, opening

and closing of heart valves, and the like, when placed at the sternum. The accelerometer(s) records Seismocardiography (SCG) when affixed to particular parts of the chest. The wearable device (Biostrap) also includes a tap-detection functionality built in, which allow the user to activate different kinds of processes with a single/double tap.

[0042] In addition to the above, the Biostrap contains a vibration motor to alert the user under certain predefined circumstances. Alerts are sent when some abnormality is detected from the bio-signals being recorded—either on the device itself in real-time, or on the cloud, or on the findings of a doctor looking at the database on the web client.

[0043] The Biostrap contains one or more LEDs, visible through the casing, or placed on top of the casing, which communicates different information about the device status and functionality to the user.

[0044] The Biostrap contains a microprocessor or other processor to collect data from the multiple sensors, which implements a series of algorithms on the wearable device itself. The Biostrap also contains an integrated circuit for wireless data communication that enables it to connect and communicate, and send to and receive data from, a smart-phone/smartwatch or another gateway device such as a wifi router. The wearable device is charged through a micro-USB connection, or through a wireless charger, and hence can be reused many times. The Biostrap also contains a memory chip that allows it to store data for long periods of time, and then to communicate this saved data to other locations.

[0045] The Biostrap device, as part of the Blood Pressure monitoring system, monitors health parameters including, but not limited to: ECG, seismocardiograph (SCG), skin impedance, impedance plethysmography (IPG), pulse plethysmograph (PPG), galvanic skin response (GSR), electro dermal activity (EDA), subject orientation and subject motion, to calculate a value of blood pressure.

[0046] In addition to the above, the system records skin temperature, blood oxygenation, CO₂ levels in the blood, haemoglobin levels in the blood, blood glucose, in order to provide the user with more detailed information on the blood pressure levels are varying with detailed inputs on how the BP levels are varying with respect to the other physiological parameters mentioned above.

[0047] In one embodiment, the blood pressure is calculated from a combination of: (a) the pulse transit time (PTT), calculated as the delay between the R-peak of the ECG, and the beginning, or the half-way point, or the peak of the PPG pulse; (b) pulse wave velocity, calculated as the estimated distance travelled by the blood between the heart and the sternum, divided by the PTT calculated as stated above; (c) the Pre Ejection Period (PEP), measured from the difference between the R-peak measured from the ECG, and the mechanical heart beat measured from the accelerometer in the SCG; (d) the time delay between the R-peak as measured from the ECG, and the peak measured from the IPG; (e) time delays between the opening and closing of the valves, as measured from the SCG, and time-lag between the valve opening and the R-peak as measured from the ECG, and the peak of the Pulse wave, as measured from the PPG; all measured on a single device affixed on the sternum of the subject, and combined with individual factors such as age, sex, height, weight and medical conditions of the user.

[0048] In another embodiment, the blood pressure is calculated from a combination of measurements from two wearable (bio-strip) devices: one affixed on the sternum, and

measuring ECG, SCG, IPG, and another one affixed on the wrist or forehead or other part of the exposed skin, measuring PPG. According to an embodiment of the present invention, all values measured from the delay between the PPG pulse and the R-peak of the ECG or heartbeat from the SCG or valve openings from the SCG or peak of the IPG are adjusted for the increased distance between the two devices, and individual factors such as age, sex, height, weight and medical conditions of the user.

[0049] According to an embodiment of the present invention, the blood pressure is calculated by using a linear or quadratic or logarithmic equation that combines the values of PEP, PWV (or PTT), the heart rate at that instant, respiration rate, shape of the PPG pulse wave, as well as other quantities measured from one or more wearable devices.

[0050] In another embodiment, a dataset containing PTT/PWV and PEP values, along with actual systolic and diastolic BP measurements, is used as a training set, and instantaneous measurements of PEP, PWV (or PTT), the heart-rate, respiration rate, shape of the PPG pulse wave, as well as other quantities measured from one or more wearable devices, are combined with individual factors such as age, sex, height, weight, and the like, and then used as inputs for a regression model, to obtain a value for systolic and diastolic BP.

[0051] In one instance, where the User is wearing a single Biostrip on the sternum measuring ECG, PPG and SCG, the equation used to derive systolic and diastolic central (aortic) BP are of the form:

$$\begin{aligned} SBP &= x_1 * PWV_{peak} + x_2 * PEP + x_3 * IHR + x_4 * \text{amp}(AO) + \\ & x_5 * \text{amp}(PPG) + x_6 * LVET + x_7 * SCG_{_XZ} + \\ & x_8 * PPG_{foot-peak} + x_9 * \text{Height} + x_{10} * \text{Weight} + \\ & x_{11} * \text{Age} + x_{12} * PPG_{W50} + x_{13} * PPG_{W75} + MC \\ DBP &= y_1 * PWV_{foot} + y_2 * PEP + y_3 * IHR + y_4 * \text{amp}(AO) + \\ & y_5 * \text{amp}(PPG) + y_6 * LVET + y_7 * SCG_{_XZ} + \\ & y_8 * PPG_{foot-peak} + y_9 * \text{Height} + y_{10} * \text{Weight} + \\ & y_{11} * \text{Age} + y_{12} * PPG_{W50} + y_{13} * PPG_{W75} + MC \end{aligned}$$

[0052] The equation may adjusted as needed. Here, PWV_{peak} refers to the Pulse Wave Velocity, as measured between the R-peak of the ECG, and the peak of the Pulse Wave in the arterioles at the sternum (near the xiphoid process, or on the manubrium); PWV_{foot} refers to the Pulse Wave Velocity, as measured between the R-peak of the ECG, and the foot (or beginning) of the Pulse Wave in the arterioles at the sternum (near the xiphoid process, or on the manubrium); PEP refers to the Pre-Ejection Period, or the time interval between the R-peak of the ECG and the AO opening peak of the SCG; IHR is the Instantaneous Heart Rate; LVET is the Left Ventricular Ejection Time, measured as the time interval between the Aortic valve opening and closing; $SCG_{_XZ}$ is the time interval between the beginning of the peak on the X-axis of the SCG, and the mid-point of the Z-axis of the SCG; $PPG_{foot-peak}$ is the time delay between the foot and peak of the PPG curve; PPG_{W50} is the width of the PPG pulse (as a proportion of one hear-beat cycle) when it is at 50% of the peak value; PPG_{W75} is the width of the PPG pulse (as a proportion of one hear-beat cycle) when it is at 75% of the peak value; and MC is a constant that is dependent on the prior medical conditions of the patient.

[0053] The constants x_i and y_i in the above equations are derived from a training set containing data for over 100

patients with data recorded for ECG, PPG, SCG and SBP and DBP, over a 1-4 hour interval, using a Linear Regression Machine Learning algorithm.

[0054] In another instance, where the user is wearing a single Biostrip on the sternum measuring ECG, PPG and SCG, the equation used to derive systolic and diastolic central (aortic) BP are of the form:

$$\begin{aligned} SBP &= x_1 * \log_e(a_1(PWV)) + x_2 * PEP + x_3 * IHR + x_4 * \text{amp} \\ & (AO) + x_5 * \text{amp}(PPG) + x_6 * LVET + x_7 * SCG_{_XZ} + \\ & x_8 * \text{Height} + x_9 * \text{Weight} + x_{10} * \text{Age} + MC \\ DBP &= y_1 * \log_e(a_2(PWV)) + y_2 * PEP + y_3 * IHR + y_4 * \text{amp} \\ & (AO) + y_5 * \text{amp}(PPG) + y_6 * LVET + y_7 * SCG_{_XZ} + \\ & y_8 * \text{Height} + y_9 * \text{Weight} + y_{10} * \text{Age} + MC \end{aligned}$$

[0055] It should be noted that other forms or variations of the equation are also contemplated by the invention. Here, PWV refers to the Pulse Wave Velocity, as measured between the R-peak of the ECG, and the arrival of the Pulse Wave in the arterioles at the sternum (near the Xiphoid process, or on the manubrium); PEP refers to the Pre-Ejection Period, or the time interval between the R-peak of the ECG and the AO opening peak of the SCG; IHR is the Instantaneous Heart Rate; LVET is the Left Ventricular Ejection Time, measured as the time interval between the Aortic valve opening and closing; $SCG_{_XZ}$ is the time interval between the beginning of the peak on the X-axis of the SCG, and the mid-point of the Z-axis of the SCG; and MC is a constant that is dependent on the prior medical conditions of the patient.

[0056] The constants x_i and y_i in the above equations are derived from a Training set containing data for over 100 patients with data recorded for ECG, PPG, SCG and SBP and DBP, over a 1-4 hour interval, using a Linear Regression Machine Learning algorithm.

[0057] In another instance, where the user is wearing a single Biostrip on the sternum measuring ECG, PPG and SCG, the equation used to derive systolic and diastolic central (aortic) BP are Quadratic variations of the equation described above. This equation is of the form:

$$\begin{aligned} SBP &= x_1 * PWV_{peak} + x_2 * PEP + x_3 * IHR + x_4 * \text{amp}(AO) + \\ & x_5 * \text{amp}(PPG) + x_6 * LVET + x_7 * SCG_{_XZ} + \\ & x_8 * \text{Height} + x_9 * \text{Weight} + x_{10} * \text{Age} + x_{11} * (PWV)^2 + \\ & x_{12} * (PEP)^2 + x_{13} * (IHR)^2 + x_{14} * (\text{amp}(AO))^2 + \\ & x_{15} * \text{amp}((PPG)^2) + x_{16} * (LVET)^2 + x_{17} * (SCG_{_XZ})^2 + MC \\ DBP &= y_1 * PWV_{foot} + y_2 * PEP + y_3 * IHR + y_4 * \text{amp}(AO) + \\ & y_5 * \text{amp}(PPG) + y_6 * LVET + y_7 * SCG_{_XZ} + \\ & y_8 * \text{Height} + y_9 * \text{Weight} + y_{10} * \text{Age} + y_{11} * (PWV)^2 + \\ & y_{12} * (PEP)^2 + y_{13} * (IHR)^2 + y_{14} * (\text{amp}(AO))^2 + \\ & y_{15} * \text{amp}((PPG)^2) + y_{16} * (LVET)^2 + y_{17} * (SCG_{_XZ})^2 + MC \end{aligned}$$

[0058] Here, PWV refers to the Pulse Wave Velocity, as measured between the R-peak of the ECG, and the arrival of the Pulse Wave in the arterioles at the sternum (near the Xiphoid process, or on the manubrium); PEP refers to the Pre-Ejection Period, or the time interval between the R-peak of the ECG and the AO opening peak of the SCG; IHR is the Instantaneous Heart Rate; LVET is the Left Ventricular Ejection Time, measured as the time interval between the Aortic valve opening and closing; $SCG_{_XZ}$ is the time interval between the beginning of the peak on the X-axis of the SCG, and the mid-point of the Z-axis of the SCG; and MC is a constant that is dependent on the prior medical conditions of the patient.

[0059] The constants x_i and y_i in the above equations are derived from a training set containing data for over 50 patients with data recorded for ECG, PPG, SCG and SBP and DBP, over a 1-4 hour interval, using a Quadratic Regression Machine Learning algorithm.

[0060] In another instance, where the user is wearing a single Biostrip on the sternum measuring ECG, PPG and SCG, the equation used to derive systolic and diastolic central (aortic) BP are of the form:

$$SBP=f_1(IHR,PWV_{peak},PEP,LVET,amp(AO),amp(PPG),SCG_{XZ},Age,Height,Weight)$$

$$DBP=f_2(IHR,PWV_{foot},PEP,LVET,amp(AO),amp(PPG),SCG_{XZ},Age,Height,Weight)$$

[0061] Here f_1 and f_2 are derived from variants of: a) Support Vector Machine; b) Bayesian Ridge Regression Model; c) K-Nearest-Neighbours Regression Model; d) Random Forest Regression model.

[0062] In another instance, where the user is wearing a single Biostrip on the sternum measuring only ECG and SCG, the equation used to derive systolic and diastolic central (aortic) BP are of the form given in [43]-[46] with x_1 , x_5 and y_1 , y_5 are set to 0, or of the form:

$$SBP=f_1(IHR,PEP,LVET,amp(AO),SCG_{XZ},Age,Height,Weight)$$

$$DBP=f_2(IHR,PEP,LVET,amp(AO),SCG_{XZ},Age,Height,Weight)$$

[0063] Here f_1 and f_2 are derived from variants of: a) Support Vector Machine; b) Bayesian Ridge Regression Model; c) K-Nearest-Neighbours Regression Model; d) Random Forest Regression model.

[0064] In another instance, where the user is wearing a single Biostrip on the sternum measuring only SCG, the equation used to derive systolic and diastolic central (aortic) BP are of the form given in [43]-[46] with x_1 , x_2 , x_5 and y_1 , y_2 , y_5 are set to 0, or of the form:

$$SBP=f_1(IHR,LVET,amp(AO),SCG_{XZ},Age,Height,Weight)$$

$$DBP=f_2(IHR,LVET,amp(AO),SCG_{XZ},Age,Height,Weight)$$

[0065] Here f_1 and f_2 are derived from variants of: a) Support Vector Machine; b) Bayesian Ridge Regression Model; c) K-Nearest-Neighbours Regression Model; d) Random Forest Regression model.

[0066] In one particular embodiment, where the user is wearing only one Biostrip on the sternum, measuring only ECG and SCG, the Pulse Transit Time between the opening of the aortic valve, and the time-point at which the pressure pulse hits the aortic arch, is determined by the time-gap between the AO peak on the Z-axis plot of the SCG, and the sharp peak immediately after that, on the Y-axis of the SCG, which denotes the time of arrival of the pressure pulse, at the aortic arch. This interval, denoted by SCG_{YZ} , provides the PWV measured in the aorta itself, which can be used with calibration, or with a population-based model, to calculate central (aortic) blood pressure in the following manner:

$$SBP=f_1(IHR,LVET,amp(AO),SCG_{YZ},Age,Height,Weight)DBP=f_2(IHR,LVET,amp(AO),SCG_{YZ},Age,Height,Weight)$$

[0067] In another instance, the central (aortic) SBP and DBP values are calculated in exactly the same way described

above, except that: (1) PWV is replaced by PWV_{HW} , which is the value of PWV normalized for Height and Weight; (2) PEP is replaced by PEP_{HW} , which is the value of PEP normalized for Height and Weight; (3) IHR is replaced by IHR_{age} , which is the value of IHR normalized for age; and (4) the constants x_8 , x_9 , x_{10} and y_8 , y_9 , y_{10} are set to 0.

[0068] In another embodiment, SBP and DBP are calculated in the manner described above, except with the difference that the constants x_i and y_i from the above equations are determined by calibrating the system against a regular cuff-based BP monitor, or an invasive arterial BP monitor for each individual, instead of determining the values from a population-based regression model.

[0069] In the calibration based approach, values for the constants x_i and y_i from above may be determined by asking the User to measure their BP using a standard device (such as the Omron BP monitor), while wearing the Biostrip, in different orientations. For example, User may be asked to measure systolic and diastolic BP three times each while standing, sitting and lying down. Each calibration method will result in one individual regression model, with its own set of constants $\{x_i\}$ and $\{y_i\}$.

[0070] In another instance, where the user is wearing two Biostrips, one on the sternum, measuring ECG and SCG, and one on the wrist measuring PPG, the peripheral SBP and DBP values are calculated using the same mathematical models described above, but where PWV is measured between the R-peak of the ECG (measured anywhere on the chest) or the AO peak measured from the SCG on the sternum, and arrival of the Pulse Wave on the wrist.

[0071] In another instance, where the user is wearing two Biostrips, one on the sternum, measuring ECG and SCG, and one on the forehead measuring PPG, the peripheral SBP and DBP values are calculated using the same mathematical models described above, but where PWV is measured between the R-peak of the ECG (measured anywhere on the chest) or the AO peak measured from the SCG on the sternum, and the arrival of the pulse wave on the forehead.

[0072] In one particular embodiment, where the user is wearing two Biostrips or other wearable devices containing only an accelerometer and a wireless communication module, one on the sternum, measuring SCG, and one on the wrist measuring mechanical movements of the pulse, the peripheral (not central) SBP and DBP values are calculated using the same mathematical models described above, but where PWV is measured between the AO peak measured from the SCG on the sternum, and the mechanical pulse wave measured on the wrist with the accelerometer. In this case, the constants x_2 , x_5 and y_2 , y_5 are set to 0.

[0073] In one particular embodiment, the user is wearing two Biostrips, or other wearable devices containing only an accelerometer and a wireless communication module, one on either wrist, measuring mechanical movements of the pulse. In this case, the time delay between the arrival of the pulse wave on one wrist, in comparison with the other wrist, is used in place of PTT in the models described. In this case, the SBP and DBP values are calculated using the values of $PTT_{foot-foot}$, $PTT_{peak-foot}$, $PTT_{foot-peak}$, and $PTT_{peak-peak}$, and the difference between the them, where the foot and peak are always of different wrists. Abnormal values of the above mentioned factors may also be used to trigger an alert for the User, to indicate possible Ischemia or other cardio-vascular disease in one branch of blood vessels.

[0074] In one particular embodiment, the Blood Pressure is estimated while the User holds the Biostrip in his hands, with the left index finger covering one electrode on the left, and the right index finger covering the right-most electrode and the central electrode and the PPG sensor (which falls between the right-most electrode and the central electrode) at the same time. This is an episodic measurement of Blood Pressure, where the user holds the device in this manner for at least 30 seconds, and PTT is calculated by the delay between the R-peak on the ECG, and the foot/peak/50% mark of the PPG curve measured on the index finger. This is converted into PWV by dividing by the distance between the heart and the finger (which is estimated from the subject's height and weight). The PWV_{foot} and PWV_{peak} is then used to estimate systolic and diastolic BP based on: (a) calibration based method for each individual; (b) population-based regression model using factors such as height, weight, age, gender and prior medical history.

[0075] In one particular embodiment, the Biostrip attached to the sternum is used to measure ECG and SCG, to determine the values of PEP, LVET, Amp(AO), systolic time, diastolic time, etc, and the User puts his finger on the LED on a smartphone to measure PPG, and the 4F application running on the phone estimates the PTT from the R-peak and Aortic Valve opening measured on the Biostrip, and the foot and peak of the PPG curve as measured on the smartphone. The equation used to determine SBP and DBP are of the form described above, but the constants determined take into account the larger distance between the Heart and the wrist, and the measurement obtained is for peripheral blood pressure, as opposed to central (aortic) blood pressure.

[0076] In another embodiment, the blood pressure is calculated from a combination of measurements of the Biostrip device affixed on the sternum, and measuring ECG, SCG, IPG; and another ring-shaped device worn on one of the fingers or toes of the user, measuring PPG on the finger/toe. According to an embodiment of the present invention, the values measured from the delay between the PPG pulse and the R-peak of the ECG or heartbeat from the SCG or valve openings from the SCG or peak of the IPG are adjusted for the increased distance between the heart and the finger/toe of the user, and individual factors such as age, sex, height, weight and medical conditions of the user.

[0077] The ring-shaped device mentioned in the above embodiment contains at least two LEDs emitting light at different wavelengths, one photodiode making measurements at regular intervals, a Bluetooth or other NFC module communicating data to the computing device in a wireless manner, and a battery to run all of the above. This device includes a plurality of other sensors, and the operation is synchronised with the operation of the wearable (bio-strip) device affixed on the sternum.

[0078] In one embodiment of the system, the processor running on the device first collects data from all the sensors, and also performs signal processing and cleaning, using one of the following protocols:

[0079] a) Calculate the SSD (sum of squared differences) value of the Histogram of the measured signal and Histogram of the ideal ECG signal (ECG_i), after applying a Bandpass filter with a low cut-off of 2 Hz, and a high cut-off of 30 Hz, using 20 bins, two times the sampling frequency ("2xfs") samples for the Histogram, and 8xfs or 4xfs number of samples in each

window for the Bandpass filter (e.g. 1000 or 500 sample window for a sampling rate of 125 Hz). The Histogram of the ideal ECG signal is stored in the CPU memory before-hand, to perform this estimation. Signal quality of a 2xfs sample window is now calculated to be:

$$\text{Signal_Quality}(X) = \max\{0, [(20 - \text{SSD}(X, ECG_i)/X)/20 \times 100]\}$$

This assumes an threshold of 20, or in other words assumes that a Chi-squared value of more than 20 means that the signal is pure noise. However, this threshold may be automatically adjusted based on other measurements.

[0080] b) Calculate the FFT of the measured signal X, after applying a Bandpass filter of 2 to 30 Hz, and calculate the SSD value of the FFT of the measured signal, and FFT of the ideal signal (ECG_i). This values: $\text{SSD}(\text{FFT}(X), \text{FFT}(ECG_i))/\text{FFT}(X)$, can be used to quantify signal quality in a manner similar to (a) above.

[0081] c) In the third method, R-peaks are detected by applying a median filter with window size 2xfs, and then another median filter with window size 7, then subtract it from the original signal.

[0082] In one particular embodiment of the invention, the Biostrip device also contains a photoelectric and/or thermoelectric module for harvesting energy from the light or heat in the environment, or the heat emanating from the body, or energy generated from motion. This energy is used to charge the battery, or to run the components of the device itself.

[0083] In another embodiment, the device also contains an electronic display, which allows the User to observe different parameters in the device itself. The display may further have the capability to detect the touch of the User, and accept commands using a touchscreen.

[0084] In another embodiment, the device contains an acoustic sensor, which allows it to record and process sounds and also perform basic processing on it. This acoustic sensor may be used to record ambient sounds, as well as breathing/wheezing sounds when the device is placed on the chest.

[0085] In another embodiment, the device contains a microfluidic sensor that can detect the quantity of different chemicals in sweat, and correlate them with varying values of Blood Pressure to provide more detailed insights to the User. In this embodiment, the microfluidic sensor may detect parameters including, but not limited to: pH levels, chloride levels, lactate levels and glucose levels in the sweat.

[0086] In another particular embodiment, the device contains a particulate matter sensor, that can detect and measure the amount of PM2.5 and PM10 particles in the immediate environment of the device, including a specific detection of cigarette smoke in the environment.

[0087] According to an embodiment of the present invention, the blood pressure calculated as stated above may be combined with other parameters measured from the device or smartphone or both, and used to diagnose and inform the user if he is in a state of hypertension, and also describe the probable cause of the hypertension. This diagnosis may use a training and classification protocol where the training set is pre-loaded on the web server, and is used to classify the recording from the wearable (Biostrip) devices(s) in real-time, either on the device itself, or on the computing device operated by the user. The training and classification protocol uses algorithms such as Artificial Neural Networks algorithm, Support Vector Machine and a Naive Bayes Classifier.

[0088] The blood pressure monitoring system has the ability to combine all the parameters mentioned above, from multiple locations on the body, with each user wearing one or more wearable devices (bio-strip), and thus obtaining derived parameters that combine information from various locations.

[0089] The system further includes a system to automatically alert the user, or any authorised third party (friend, family, doctor or other care-giver) when the computed blood pressure levels cross a certain predefined or adaptive threshold, and further trigger a biofeedback protocol shown in the form of an application on the phone or other device to enable the user to regain a low level of blood pressure.

[0090] The biofeedback protocol referred to above uses audio or video inputs to the user, delivered through an application running on the computing device of the user, which synchronize with the device affixed on the user via wireless communication protocol.

[0091] According to an embodiment of the present invention, the application running on the computing device also trigger other kinds of responses/alerts for the user, upon detecting different levels of blood pressure that are indicative of hypertension, including but not limited to: (a) YouTube videos or other videos stored on the external SD card, or podcasts being played on a theme that is pre-selected by the user, or automatically estimated from the behaviour pattern of the User; (b) songs or other audio tracks played through the smartphone or other multimedia device; (c) jokes displayed on the smartphone.

[0092] The system also allows the user, or the caregiver to instantly transfer the stored medical data related to blood pressure, to a concerned physician or caregiver through the application running on the smartphone securely, so that the third party has an option to view the user data on the computing device.

[0093] In addition, the system allows the user or the caregiver to instantly book appointments with a concerned doctor at a given hospital or clinic, and also to conduct an 'Online Consultation', by way of an audio/video VOIP call, or a regular phone call, or some other kind of communication protocol over the web.

[0094] The blood pressure monitoring system includes the capability of initiating an appointment or online consultation as mentioned above, and also for facilitating the payment for such a service by way of an online payment gateway in a secure manner.

[0095] During an online consultation, the system also allows the concerned personnel to view certain parts of the user's data, and to make episodic measurements from the Biostrip device, through instructions delivered to the patient, and thereafter to view the data in real-time through a web application. In this manner, the system facilitates a "Virtual Examination."

[0096] The system used information collected from other sensors on the smartphone or tablet or other device, about the user's environment, in order to present the parent or care-giver with a periodic report of the blood pressure levels recorded during different activities, at different times of the day. The application on the phone further gives recommendations to the parent or care-giver for different ways of reducing pain levels at different times of the day.

[0097] Additionally, the application running on the phone may also have a mechanism for collecting data from any of the other sensors or applications running on the smartphone,

as well as subjective, user-inputted data from the care-giver, as and when the user undergoes different activities, and reaches different blood pressure levels, and other mental/physical states. This data can subsequently be used to improve the recommendations and tips/messages for the same user, as well as other users, while maintaining privacy of data for each user.

[0098] The system further uses the information collected from other sensors on computing device, about the environment of the user, in order to present the user and the authorized third-party with periodic report of the user blood pressure levels of the user recorded during different activities, at different times of the day. The application on the phone further gives recommendations to the user or care-giver or the concerned doctor for different ways of controlling blood pressure levels more effectively at different times of the day.

[0099] The system stores the individual parameters, such as age, sex, medical history for each user, and combines anonymised information of multiple users from different locations on the cloud, in order to present each individual user with data about the user's blood pressure levels and activities in comparison with a similar population, and in order to give the user information about where they stand with respect to other users, in terms of percentiles and other comparative measures.

[0100] The system combines subjective information and information from multiple sensors on multiple users, as described above, to run machine learning algorithms, Bayesian classifiers or other kinds of training and testing protocols, in order to provide alerts that are customized for each individual, based on the normal parameters for users in the same demographic section.

[0101] FIG. 1 illustrates a schematic diagram of the invention. A plurality of sensors **101,102,103,104** record data, and transmit the data to a microcontroller **105**. The microcontroller may instead be a microprocessor or any other suitable computing device for processing data. The data is processed by the microprocessor **105** and then sent for transmission to the Bluetooth low energy ("BLE")/Wireless transmission module **106**. Module **106** communicates the data to a smartphone or another gateway device. In certain embodiments, the microprocessor **105** simply stores the data on the device itself, on a memory chip **110**, for transmitting the data at a later time to another device. The wearable (Biostrip) device also contains status diodes **109** which indicate different states of the device, and a vibration motor **108**, which can alert the user when configured to do so, either by the MCU or upon receiving an instruction from the smartphone.

[0102] FIG. 2 illustrates an exemplary configuration of the device, including the form factor of the device. In one embodiment, the device includes a removable sticker part, which is disposable, and meant to be removed after certain periods of time. According to an embodiment of the present invention, the removable sticker is double sided, and one side affixes to the device, whereas the other side affixed to the skin of the patient.

[0103] The wearable device shown in FIG. 2 is flexible, and hence it is able to conform to the shape of the location of the body upon which it is affixed. Further, the sticker shown in FIG. 2 has cut-out holes so that the biomedical sensors affixed on the lower part of the device can be directly in contact with the skin.

[0104] FIG. 3 illustrates the 3D layout of the device in one embodiment, including the shape and heights of the different electrical and mechanical components. The lighter top surface denotes the components on the lower side of the device, facing the skin. The three circular objects show the electrodes 111, whereas the light rectangular part shows the optical sensor 112, all of which are directly in contact with the skin when the device is worn.

[0105] Further, FIG. 3 shows the electrical components on the upper side of the device, facing away from the subject when worn, on the bottom of the drawing. These components include a microprocessor 105, a Bluetooth module 106, an analog front end for processing the electrical signals, and several other components.

[0106] FIG. 4 illustrates one particular embodiment of the device, where the data for ECG, IPG, SCG, respiration, skin temperature and movement is first collected from a wearable device (bio-strip) affixed at the sternum, and data for PPG, hand motion recorded from a second wearable device (bio-strip) affixed on the arm/wrist.

[0107] As shown in FIG. 4, data is transferred to the smartphone (or other gateway device), using a wireless communication protocol. According to an embodiment of the present invention, from the computing device such as a smartphone, the data transferred to a secure location on the web (cloud) from where it can be accessed by the authorized third party such as a doctor or a concerned medical professional.

[0108] FIG. 4 also illustrates that within the system, the user may directly consult the doctor, or the doctor can send alerts or prescriptions to the user.

[0109] As shown in FIG. 5, the monitoring system described in the application combines data from multiple sensors on one or more devices, and transfers it to the smartphone, where values such as PTT, PWV, PEP, and the like are calculated, and subsequently used to calculate the values for systolic and diastolic blood pressure.

[0110] FIG. 5 illustrates that this above mentioned data is stored in a centralized, secure database that is HIPAA compliant. This data is then accessed by a virtual machine running various data processing, machine learning and classification algorithms to calculate a more accurate value of Blood Pressure, and also the correlation of Blood Pressure values with other individual or environmental factors.

[0111] This virtual machine, shown in FIG. 5, is able to store results in the database, and also send alerts and other messages directly to patients so that they can act appropriately.

[0112] As shown in FIG. 5, the virtual machine running classification algorithms triggers a biofeedback protocol, delivered to the patient through the smartphone application, to help in management of stress or chronic pain for the user. The biofeedback protocol mentioned above may also be triggered directly from the smartphone application, without requiring any communication with the cloud.

[0113] FIG. 5 also shows that the data used to calculate BP may also be communicated to a Transdermal Drug Delivery system (TDDS), which contains a module for Wireless Communication, so that the dosage of different blood pressure medications being delivered can be regulated automatically by the blood pressure measurements taken through the system.

[0114] Further, FIG. 5 shows that the data stored on the cloud database can be accessed by the concerned doctors via

a web client application, and the doctors can also send alerts or recommendations directly to the patients.

[0115] Additionally, illustrated in FIG. 5 is the concerned doctors and patients can directly interact with each other by way of online consultations or video/audio messages and chats, using a secure channel set up for them to interact and share data with each other.

[0116] FIG. 6 shows an example of the electrical and mechanical signals obtained from a functioning Biostrip device placed on the sternum. The red line shows the mechanical signals, which show the opening and closing of the aortic and mitral valves, along with other events from the cardiac cycle. The blue line shows the electrical signals (ECG) obtained on the sternum, which identifies the R-peak, and the PQRS complex. The cardiac time intervals (PEP, LVET, IVRT, IVCT) referred to earlier in the application are calculated as the time difference between these events.

[0117] One or more embodiments of the present invention have been described. Nevertheless, it will be understood that various modifications may be made without departing from the spirit and scope of the invention. Accordingly, other embodiments are within the scope of the following claims.

What is claimed is:

1. A wearable device having opposing first and second sides for monitoring of blood pressure comprising:

a biostrip, the biostrip including a first printed circuit board (PCB), a second PCB; and a flexible third PCB in electrical connection with the first PCB and second PCB, the biostrip comprising:

a plurality of physiological sensors;
a processor;
a wireless communication hub;
an accelerometer; and

a Photoplethysmograph (“PPG”) module containing 2 or more LEDs emitting light at different wavelengths, and one or more photodiodes, affixed to the first side of the device,

a two-sided adhesive, a first side of the adhesive affixed to the biostrip and an opposing second side of the adhesive configured to affix to a user at a second side; and
a gateway device.

2. The device of claim 1 further comprising a vibration motor.

3. The device of claim 1 wherein the device contains an analog front-end and at least two electrodes, and is configured to measure the EXG (ECG/EMG/EEG) from different locations on the body.

4. The device of claim 1 wherein the device is configured to measure a property selected from the group consisting of: respiration cycles, blood oxygenation, seismocardiography (SCG), subject movements, blood pressure, blood glucose, and blood carbon dioxide levels and combinations thereof.

5. The device of claim 1 wherein the adhesive includes a plurality of cut-out holes, the cut-out holes adapted to receive at least one sensor, the cut-out holes further adapted to allow the sensor to be affixed directly on the user's skin.

6. The device of claim 1 wherein the one of the PCBs further comprises one or more of the following:

a USB port for charging the device and transfer data from the device;
a plurality of LEDs;
a thermoelectric or photoelectric panel for harvesting energy from the body heat, or from light or heat in the environment;

an electronic display; and
a wireless charging coil.

7. The device of claim 1 wherein the PPG is configured to measure blood oxygenation, haemoglobin levels, heart rate, and carbon dioxide levels.

8. The device of claim 1, wherein the device is configured to receive information from the plurality of physiological sensors and further configured to perform local processing, the local processing including applying bandpass filters, median/mean filters, and peak detection, calculating time intervals between events on different physiological signals, the local processing configured to derive parameters related to the health of the individual.

9. The device of claim 1 wherein the parameters are selected from the group consisting of: Heart Rate, Respiration Rate, Pulse Wave Velocity, Blood Pressure, Respiratory Sinus Arrhythmia, and Cardiac Time Intervals.

10. The device of claim 9 wherein the plurality of physiological sensors includes an ECG sensor, the device further configured to combine information from the ECG sensor and the PPG sensor to calculate PAT_{foot} , PAT_{peak} , $PAT_{50\%}$, on the user's chest when the device is stuck on the sternum, and the device is further configured to use the calculations to determine central (aortic) Systolic and Diastolic Blood Pressure on board the device, using a calibration based approach, where Blood Pressure is measured for the first time using a standard BHS/AAHS certified BP monitor or a Sphygmomanometer.

11. The device of claim 9 wherein the plurality of physiological sensors includes an ECG sensor, the device further configured to combine information from the ECG sensor and the PPG sensor to calculate PAT_{foot} , PAT_{peak} , $PAT_{50\%}$, on the user's fingers when the device is held with the index finger of one hand covering one electrode, and the index finger of the other hand covering two electrodes and the PPG sensor, which are together used to estimate peripheral Systolic and Diastolic Blood Pressure.

12. A wearable device for continuous monitoring of blood pressure comprising:

a biostrip, the biostrip including a first printed circuit board (PCB), a second PCB; and a flexible third PCB connecting the first PCB and second PCB, the third PCB comprising:

a plurality of physiological sensors, the physiological sensors including an ECG sensor and an SCG sensor (accelerometer);

a processor;

a wireless communication hub; an accelerometer; and a vibration motor;

a single-use two-sided adhesive, the adhesive affixed to the biostrip at a first side and to a user at a second side; and

a gateway device.

13. The device of claim 12 wherein the gateway device is selected from a group consisting of a smartphone or smartwatch.

14. The device of claim 12 further comprising a reflective PPG (photoplethysmograph) sensor on the underside of the device, the reflective PPG sensor comprising of at least two or more LEDs, including one red and one infra-red LED, and one or more photodiodes, wherein the device is configured to measure the Pulse pressure wave, Heart Rate, blood oxygen levels and carbon dioxide levels in the Blood.

15. The device of claim 12 wherein information is combined from the ECG sensor and the accelerometer measuring SCG to calculate pre-ejection period (PEP), the IVRT, IVCT, Systolic time, diastolic time, Aortic Arch Interval (time period between the Aortic valve opening and the peak on the Y-axis of the SCG following 20-100 ms after AO), and other cardiac time intervals when placed on the sternum, to calculate a value of central systolic and diastolic Blood Pressure based on the calibration method.

16. A system, which uses a device according to claim 12, to estimate the systolic and diastolic Blood Pressure values, and a smartphone/smartwatch to display the said values, and to communicate the values to a third party or caregiver via a wireless communication protocol. The said system may also have the capability of sending automatic alerts to the User or caregiver or any third party that has been authorized to receive alerts by the User.

17. The device of claim 13 wherein the calculation of the central aortic Systolic and Diastolic Blood Pressure is performed using a population-based regression model that includes SBP, DBP and height, weight, gender and prior medical conditions of each subject.

18. The device of claim 12, that uses only the data obtained from the SCG or PCG sensor (high sensitivity accelerometer) alone, and the values of PEP, LVET, IVRT, IVCT, $Amp(AO_{peak})$, time interval between the opening of the Aortic valve and the pressure pulse reaching the aortic arch, as measured by the distance between the peak on the Z-axis (AO opening) and the subsequent peak on the Y-axis (pressure pulse reaching the aortic arch), when placed on the sternum, to estimate a value of central (aortic) Blood Pressure, using a calibration based approach, assuming that the person has already calibrated using a regular, certified BP monitor or using a population-based regression model that includes information on the one or more of the above mentioned parameters, SBP, DBP and height, weight, gender and prior medical conditions of each subject.

19. The device of claim 12, wherein the ECG and SCG signal are obtained from the device, and a PPG signal is acquired from a smartphone or smartwatch where the User places his/her finger on an in-built LED on the smartphone/smartwatch, and the time interval between the R-peak on the ECG, the AO-peak on the SCG and the PPG_{foot} , PPG_{peak} and $PPG_{50\%}$ from the finger is obtained after synchronizing all signals on the smartphone, to estimate a value of peripheral systolic and diastolic Blood Pressure using the calibration based approach or the population model based approach.

20. A system according to claim 15, in conjunction with a smartphone/smartwatch, to measure systolic and diastolic Blood Pressure from a combination of: ECG and/or SCG measured on one device stuck on the chest or held in the hands, or stuck on the forehead; and the PPG pulse as measured on a different device, when placed on the forehead or foot or wrist or sternum or held in the hand; together sending data to the smartphone/smartwatch or other gateway device (which could also be one of the two Biostrips themselves), which computes the PAT_{foot} , PAT_{peak} , $PAT_{50\%}$, PEP or other value to estimate systolic and diastolic Blood Pressure. A system according to claim 15, that uses two Biostrips, or other wearable devices containing only an accelerometer and a wireless communication module, one

on either wrist, measuring mechanical movements of the pulse. In this case, the time delay between the arrival of the pulse wave on one wrist, in comparison with the other wrist, is used in place of PTT between the chest and the finger. In this case, the SBP and DBP values are calculated using the values of $PTT_{foot-foot}$, $PTT_{peak-foot}$, $PTT_{foot-peak}$, and $PTT_{peak-peak}$, and the difference between the them (where the foot and peak are always of different wrists).

21. The device of claim **12** wherein the vibration is configured to be triggered by the processor pre-defined abnormal conditions such as high systolic blood pressure, low systolic blood pressure, high diastolic blood pressure, and low diastolic blood pressure are detected.

22. A system according to claim **15**, that uses two Bio-strips or other wearable devices containing only an accelerometer and a wireless communication module, one on the sternum, measuring SCG, and one on the wrist measuring mechanical movements of the pulse, the peripheral (not central) SBP and DBP values are calculated using PWV as

measured between the AO peak measured from the SCG on the sternum, and the mechanical pulse wave measured on the wrist with the accelerometer.


23. A system, according to claim **15**, that uses one Biostrip device affixed on the sternum, and measuring ECG and SCG; and another ring-shaped device worn on one of the fingers or toes of the user, measuring PPG on the finger/toe. The values of PAT_{foot} , PAT_{peak} , $PAT_{50\%}$ are calculated between the R-peak of the ECG or the AO-peak on the SCG, and the PPG curve measured on the ring sensor, and are used to calculate the peripheral Systolic and Diastolic Blood Pressure on board the device, using a calibration based approach, assuming that the person has already calibrated using a regular, certified BP monitor, or using a population-based regression model that includes information on the one or more of the above mentioned parameters, SBP, DBP and height, weight, gender and prior medical conditions of each subject.

* * * * *

专利名称(译)	用于连续监测血压的系统和方法		
公开(公告)号	US20170347894A1	公开(公告)日	2017-12-07
申请号	US15/373753	申请日	2016-12-09
[标]发明人	BHUSHAN MANAV SIBAL SANDEEP		
发明人	BHUSHAN, MANAV SIBAL, SANDEEP		
IPC分类号	A61B5/0205 A61B5/0402 A61B5/00 A61B5/145 A61B5/11 A61B5/021 A61B5/024		
CPC分类号	A61B5/0205 A61B5/0402 A61B5/14542 A61B5/14546 A61B5/11 A61B5/6832 A61B5/746 A61B5/02416 A61B5/021 A61B2562/0219 A61B5/681 A61B5/0022 A61B5/0452 G16H40/67		
外部链接	Espacenet USPTO		

摘要(译)

本发明描述了一种用于连续监测中枢（主动脉）和外周血压的系统和方法。该系统包括完全移动的，非侵入性的连续血压监测系统，其包括固定在用户上的一个或多个Biostrip设备，与运行在计算设备上的应用程序耦合，该计算设备还连接到云中的web服务器。系统在Biostrip设备上或在网关设备（智能手机或智能手表）上或在云上执行各种计算，并向用户和授权的第三方提供关于用户的血压水平的各种见解。此外，该系统使用户能够接收用于控制高血压的生物反馈训练，并安排在线预约，在线支付这些预约，安全地共享数据以获得见解。

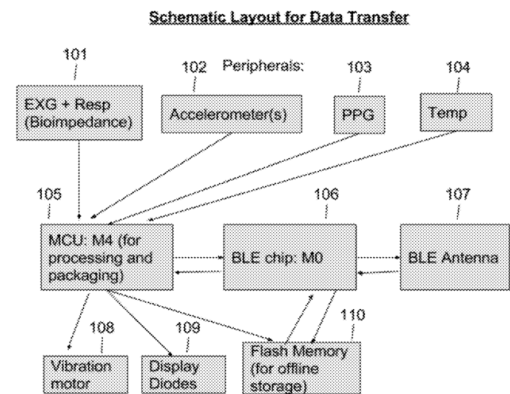

Schematic layout of the device and data transfer protocol in one particular embodiment