



US010052037B2

(12) **United States Patent**
Kinast et al.

(10) **Patent No.: US 10,052,037 B2**
(45) **Date of Patent: Aug. 21, 2018**

(54) **NON-INVASIVE BLOOD PRESSURE MEASUREMENT SYSTEM**

5/02028; A61B 8/02; A61B 5/02255;
A61B 7/045; A61B 5/0295; A61B
5/0402; A61B 5/0261; A61B 5/7203;
A61B 5/7271;

(71) Applicant: **Masimo Corporation**, Irvine, CA (US)

(Continued)

(72) Inventors: **Eric Karl Kinast**, Santa Ana, CA (US);
Valery G. Telfort, Irvine, CA (US)

(56) **References Cited**

(73) Assignee: **Masimo Corporation**, Irvine, CA (US)

U.S. PATENT DOCUMENTS

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

4,960,128 A 10/1990 Gordon et al.
4,964,408 A 10/1990 Hink et al.

(Continued)

FOREIGN PATENT DOCUMENTS

(21) Appl. No.: **15/229,840**

WO WO 2011039580 A2 * 4/2011 A61B 5/021

(22) Filed: **Aug. 5, 2016**

OTHER PUBLICATIONS

(65) **Prior Publication Data**

US 8,845,543, 09/2014, Diab et al. (withdrawn)
US 9,579,050, 02/2017, Al-Ali (withdrawn)

US 2017/0027456 A1 Feb. 2, 2017

Primary Examiner — Meredith Weare
(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson & Bear, LLP

Related U.S. Application Data

(63) Continuation of application No. 13/189,396, filed on Jul. 22, 2011, now Pat. No. 9,408,542.

(Continued)

(51) **Int. Cl.**
A61B 5/021 (2006.01)
A61B 7/00 (2006.01)

(Continued)


(52) **U.S. Cl.**
CPC **A61B 5/02125** (2013.01); **A61B 5/0205** (2013.01); **A61B 5/02028** (2013.01);
(Continued)

(58) **Field of Classification Search**
CPC ... A61B 5/02125; A61B 5/7246; A61B 5/725; A61B 7/02; A61B 5/0205; A61B

(57) **ABSTRACT**

A system for non-invasively determining an indication of an individual's blood pressure is described. In certain embodiments, the system calculates pulse wave transit time using two acoustic sensors. The system can include a first acoustic sensor configured to monitor heart sounds of the patient corresponding to ventricular systole and diastole and a second acoustic sensor configured to monitor arterial pulse sounds at an arterial location remote from the heart. The system can advantageously calculate a arterial pulse wave transit time (PWTT) that does not include the pre-ejection period time delay. In certain embodiments, the system further includes a processor that calculates the arterial PWTT obtained from the acoustic sensors. The system can use this arterial PWTT to determine whether to trigger an occlusive cuff measurement.

18 Claims, 25 Drawing Sheets

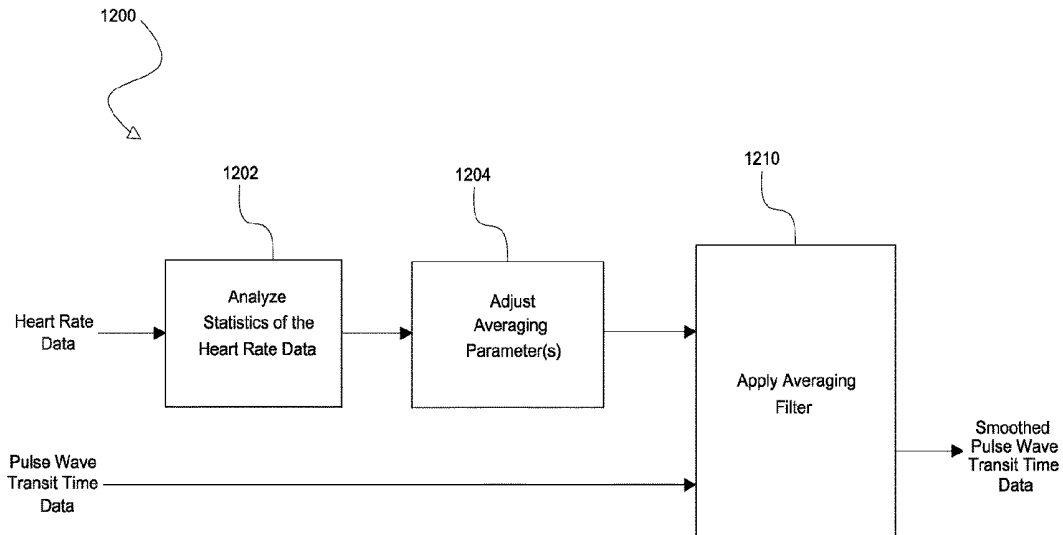

Related U.S. Application Data					
		5,533,511	A	7/1996	Kaspari et al.
		5,534,851	A	7/1996	Russek
(60)	Provisional application No. 61/366,862, filed on Jul. 22, 2010, provisional application No. 61/469,511, filed on Mar. 30, 2011.	5,561,275	A	10/1996	Savage et al.
		5,562,002	A	10/1996	Lalin
		5,590,649	A	1/1997	Caro et al.
		5,602,924	A	2/1997	Durand et al.
		5,632,272	A	5/1997	Diab et al.
(51)	Int. Cl.	5,638,816	A	6/1997	Kiani-Azarbayjany et al.
	<i>A61B 5/024</i> (2006.01)	5,638,818	A	6/1997	Diab et al.
	<i>A61B 5/00</i> (2006.01)	5,645,440	A	7/1997	Tobler et al.
	<i>A61B 5/026</i> (2006.01)	5,685,299	A	11/1997	Diab et al.
	<i>A61B 5/0285</i> (2006.01)	D393,830	S	4/1998	Tobler et al.
	<i>A61B 5/0295</i> (2006.01)	5,743,262	A	4/1998	Lepper, Jr. et al.
	<i>A61B 5/0402</i> (2006.01)	5,758,644	A	6/1998	Diab et al.
	<i>A61B 7/04</i> (2006.01)	5,760,910	A	6/1998	Lepper, Jr. et al.
	<i>A61B 5/02</i> (2006.01)	5,769,785	A	6/1998	Diab et al.
	<i>A61B 5/0205</i> (2006.01)	5,782,757	A	7/1998	Diab et al.
	<i>A61B 5/0225</i> (2006.01)	5,785,659	A	7/1998	Caro et al.
	<i>A61B 7/02</i> (2006.01)	5,791,347	A	8/1998	Flaherty et al.
	<i>A61B 8/02</i> (2006.01)	5,810,734	A	9/1998	Caro et al.
	<i>A61B 5/0452</i> (2006.01)	5,823,950	A	10/1998	Diab et al.
	<i>A61B 5/029</i> (2006.01)	5,830,131	A	11/1998	Caro et al.
	<i>A61B 5/053</i> (2006.01)	5,833,618	A	11/1998	Caro et al.
	<i>A61B 5/0245</i> (2006.01)	5,860,919	A	1/1999	Kiani-Azarbayjany et al.
	<i>A61B 5/08</i> (2006.01)	5,890,929	A	4/1999	Mills et al.
	<i>A61B 5/1455</i> (2006.01)	5,904,654	A	5/1999	Wohltmann et al.
(52)	U.S. Cl.	5,919,134	A	7/1999	Diab
	CPC <i>A61B 5/0261</i> (2013.01); <i>A61B 5/0285</i> (2013.01); <i>A61B 5/0295</i> (2013.01); <i>A61B 5/02255</i> (2013.01); <i>A61B 5/02416</i> (2013.01); <i>A61B 5/0402</i> (2013.01); <i>A61B 5/7203</i> (2013.01); <i>A61B 5/725</i> (2013.01); <i>A61B 5/7246</i> (2013.01); <i>A61B 5/7271</i> (2013.01); <i>A61B 7/00</i> (2013.01); <i>A61B 7/02</i> (2013.01); <i>A61B 7/045</i> (2013.01); <i>A61B 8/02</i> (2013.01); <i>A61B 5/024</i> (2013.01); <i>A61B 5/029</i> (2013.01); <i>A61B 5/0245</i> (2013.01); <i>A61B 5/0452</i> (2013.01); <i>A61B 5/053</i> (2013.01); <i>A61B 5/0816</i> (2013.01); <i>A61B 5/14551</i> (2013.01); <i>A61B 2560/0223</i> (2013.01); <i>A61B 2562/0204</i> (2013.01); <i>A61B 2562/04</i> (2013.01); <i>A61B 2562/06</i> (2013.01)	5,934,925	A	8/1999	Tobler et al.
		5,940,182	A	8/1999	Lepper, Jr. et al.
		5,995,855	A	11/1999	Kiani et al.
		5,997,343	A	12/1999	Mills et al.
		6,002,952	A	12/1999	Diab et al.
		6,011,986	A	1/2000	Diab et al.
		6,027,452	A	2/2000	Flaherty et al.
		6,036,642	A	3/2000	Diab et al.
		6,045,509	A	4/2000	Caro et al.
		6,067,462	A	5/2000	Diab et al.
		6,081,735	A	6/2000	Diab et al.
		6,088,607	A	7/2000	Diab et al.
		6,110,522	A	8/2000	Lepper, Jr. et al.
		6,124,597	A	9/2000	Shehada
		6,128,521	A	10/2000	Marro et al.
		6,129,675	A	10/2000	Jay
		6,144,868	A	11/2000	Parker
		6,151,516	A	11/2000	Kiani-Azarbayjany et al.
		6,152,754	A	11/2000	Gerhardt et al.
		6,157,850	A	12/2000	Diab et al.
		6,165,005	A	12/2000	Mills et al.
		6,184,521	B1	2/2001	Coffin, IV et al.
(58)	Field of Classification Search	6,206,830	B1	3/2001	Diab et al.
	CPC <i>A61B 5/0285</i> ; <i>A61B 5/02416</i> ; <i>A61B 7/00</i> ; <i>A61B 5/14551</i>	6,229,856	B1	5/2001	Diab et al.
	See application file for complete search history.	6,232,609	B1	5/2001	Snyder et al.
		6,236,872	B1	5/2001	Diab et al.
		6,241,683	B1	6/2001	Macklem et al.
		6,253,097	B1	6/2001	Aronow et al.
(56)	References Cited	6,256,523	B1	7/2001	Diab et al.
	U.S. PATENT DOCUMENTS	6,263,222	B1	7/2001	Diab et al.
		6,278,522	B1	8/2001	Lepper, Jr. et al.
		6,280,213	B1	8/2001	Tobler et al.
		6,285,896	B1	9/2001	Tobler et al.
		6,301,493	B1	10/2001	Marro et al.
		6,317,627	B1	11/2001	Ennen et al.
		6,321,100	B1	11/2001	Parker
		6,325,761	B1	12/2001	Jay
		6,334,065	B1	12/2001	Al-Ali et al.
		6,343,224	B1	1/2002	Parker
		6,349,228	B1	2/2002	Kiani et al.
		6,360,114	B1	3/2002	Diab et al.
		6,368,283	B1	4/2002	Xu et al.
		6,371,921	B1	4/2002	Caro et al.
		6,377,829	B1	4/2002	Al-Ali
		6,388,240	B2	5/2002	Schulz et al.
		6,397,091	B2	5/2002	Diab et al.
		6,430,437	B1	8/2002	Marro
		6,430,525	B1	8/2002	Weber et al.
		6,463,311	B1	10/2002	Diab
		6,470,199	B1	10/2002	Kopotic et al.
		6,501,975	B2	12/2002	Diab et al.
		6,505,059	B1	1/2003	Kollias et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,515,273	B2	2/2003	Al-Ali	7,096,054	B2	8/2006	Abdul-Hafiz et al.
6,519,487	B1	2/2003	Parker	7,132,641	B2	11/2006	Schulz et al.
6,525,386	B1	2/2003	Mills et al.	7,142,901	B2	11/2006	Kiani et al.
6,526,300	B1	2/2003	Kiani et al.	7,149,561	B2	12/2006	Diab
6,541,756	B2	4/2003	Schulz et al.	7,186,966	B2	3/2007	Al-Ali
6,542,764	B1	4/2003	Al-Ali et al.	7,190,261	B2	3/2007	Al-Ali
6,580,086	B1	6/2003	Schulz et al.	7,215,984	B2	5/2007	Diab
6,584,336	B1	6/2003	Ali et al.	7,215,986	B2	5/2007	Diab
6,595,316	B2	7/2003	Cybulski et al.	7,221,971	B2	5/2007	Diab
6,597,932	B2	7/2003	Tian et al.	7,225,006	B2	5/2007	Al-Ali et al.
6,597,933	B2	7/2003	Kiani et al.	7,225,007	B2	5/2007	Al-Ali
6,606,511	B1	8/2003	Ali et al.	RE39,672	E	6/2007	Shehada et al.
6,632,181	B2	10/2003	Flaherty et al.	7,239,905	B2	7/2007	Kiani-Azarbayjany et al.
6,639,668	B1	10/2003	Trepagnier	7,245,953	B1	7/2007	Parker
6,640,116	B2	10/2003	Diab	7,254,429	B2	8/2007	Schurman et al.
6,643,530	B2	11/2003	Diab et al.	7,254,431	B2	8/2007	Al-Ali
6,650,917	B2	11/2003	Diab et al.	7,254,433	B2	8/2007	Diab et al.
6,654,624	B2	11/2003	Diab et al.	7,254,434	B2	8/2007	Schulz et al.
6,658,276	B2	12/2003	Kiani et al.	7,272,425	B2	9/2007	Al-Ali
6,661,161	B1	12/2003	Lanzo et al.	7,274,955	B2	9/2007	Kiani et al.
6,671,531	B2	12/2003	Al-Ali et al.	D554,263	S	10/2007	Al-Ali
6,678,543	B2	1/2004	Diab et al.	7,280,858	B2	10/2007	Al-Ali et al.
6,684,090	B2	1/2004	Ali et al.	7,289,835	B2	10/2007	Mansfield et al.
6,684,091	B2	1/2004	Parker	7,292,883	B2	11/2007	De Felice et al.
6,697,656	B1	2/2004	Al-Ali	7,295,866	B2	11/2007	Al-Ali
6,697,657	B1	2/2004	Shehada et al.	7,328,053	B1	2/2008	Diab et al.
6,697,658	B2	2/2004	Al-Ali	7,332,784	B2	2/2008	Mills et al.
RE38,476	E	3/2004	Diab et al.	7,340,287	B2	3/2008	Mason et al.
6,699,194	B1	3/2004	Diab et al.	7,341,559	B2	3/2008	Schulz et al.
6,714,804	B2	3/2004	Al-Ali et al.	7,343,186	B2	3/2008	Lamego et al.
RE38,492	E	4/2004	Diab et al.	D566,282	S	4/2008	Al-Ali et al.
6,721,582	B2	4/2004	Trepagnier et al.	7,355,512	B1	4/2008	Al-Ali
6,721,585	B1	4/2004	Parker	7,356,365	B2	4/2008	Schurman
6,725,075	B2	4/2004	Al-Ali	7,371,981	B2	5/2008	Abdul-Hafiz
6,728,560	B2	4/2004	Kollias et al.	7,373,193	B2	5/2008	Al-Ali et al.
6,735,459	B2	5/2004	Parker	7,373,194	B2	5/2008	Weber et al.
6,745,060	B2	6/2004	Diab et al.	7,376,453	B1	5/2008	Diab et al.
6,760,607	B2	7/2004	Al-Ali	7,377,794	B2	5/2008	Al Ali et al.
6,770,028	B1	8/2004	Ali et al.	7,377,899	B2	5/2008	Weber et al.
6,771,994	B2	8/2004	Kiani et al.	7,383,070	B2	6/2008	Diab et al.
6,792,300	B1	9/2004	Diab et al.	7,415,297	B2	8/2008	Al-Ali et al.
6,813,511	B2	11/2004	Diab et al.	7,428,432	B2	9/2008	Ali et al.
6,816,741	B2	11/2004	Diab	7,438,683	B2	10/2008	Al-Ali et al.
6,822,564	B2	11/2004	Al-Ali	7,440,787	B2	10/2008	Diab
6,826,419	B2	11/2004	Diab et al.	7,454,240	B2	11/2008	Diab et al.
6,830,711	B2	12/2004	Mills et al.	7,467,002	B2	12/2008	Weber et al.
6,850,787	B2	2/2005	Weber et al.	7,469,157	B2	12/2008	Diab et al.
6,850,788	B2	2/2005	Al-Ali	7,471,969	B2	12/2008	Diab et al.
6,852,083	B2	2/2005	Caro et al.	7,471,971	B2	12/2008	Diab et al.
6,861,639	B2	3/2005	Al-Ali	7,483,729	B2	1/2009	Al-Ali et al.
6,898,452	B2	5/2005	Al-Ali et al.	7,483,730	B2	1/2009	Diab et al.
6,920,345	B2	7/2005	Al-Ali et al.	7,489,958	B2	2/2009	Diab et al.
6,931,268	B1	8/2005	Kiani-Azarbayjany et al.	7,496,391	B2	2/2009	Diab et al.
6,934,570	B2	8/2005	Kiani et al.	7,496,393	B2	2/2009	Diab et al.
6,939,305	B2	9/2005	Flaherty et al.	D587,657	S	3/2009	Al-Ali et al.
6,943,348	B1	9/2005	Coffin, IV	7,499,741	B2	3/2009	Diab et al.
6,950,687	B2	9/2005	Al-Ali	7,499,835	B2	3/2009	Weber et al.
6,961,598	B2	11/2005	Diab	7,500,950	B2	3/2009	Al-Ali et al.
6,970,792	B1	11/2005	Diab	7,509,154	B2	3/2009	Diab et al.
6,979,812	B2	12/2005	Al-Ali	7,509,494	B2	3/2009	Al-Ali
6,985,764	B2	1/2006	Mason et al.	7,510,849	B2	3/2009	Schurman et al.
6,993,371	B2	1/2006	Kiani et al.	7,526,328	B2	4/2009	Diab et al.
6,996,427	B2	2/2006	Ali et al.	7,530,942	B1	5/2009	Diab
6,999,904	B2	2/2006	Weber et al.	7,530,949	B2	5/2009	Al Ali et al.
7,003,338	B2	2/2006	Weber et al.	7,530,955	B2	5/2009	Diab et al.
7,003,339	B2	2/2006	Diab et al.	7,563,110	B2	7/2009	Al-Ali et al.
7,015,451	B2	3/2006	Dalke et al.	7,596,398	B2	9/2009	Al-Ali et al.
7,024,233	B2	4/2006	Ali et al.	7,618,375	B2	11/2009	Flaherty
7,027,849	B2	4/2006	Al-Ali	D606,659	S	12/2009	Kiani et al.
7,030,749	B2	4/2006	Al-Ali	7,647,083	B2	1/2010	Al-Ali et al.
7,039,449	B2	5/2006	Al-Ali	D609,193	S	2/2010	Al-Ali et al.
7,041,060	B2	5/2006	Flaherty et al.	D614,305	S	4/2010	Al-Ali et al.
7,044,918	B2	5/2006	Diab	RE41,317	E	5/2010	Parker
7,067,893	B2	6/2006	Mills et al.	7,729,733	B2	6/2010	Al-Ali et al.
7,096,052	B2	8/2006	Mason et al.	7,734,320	B2	6/2010	Al-Ali
				7,761,127	B2	7/2010	Al-Ali et al.
				7,761,128	B2	7/2010	Al-Ali et al.
				7,764,982	B2	7/2010	Dalke et al.
				D621,516	S	8/2010	Kiani et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

7,791,155 B2	9/2010	Diab	8,315,683 B2	11/2012	Al-Ali et al.
7,801,581 B2	9/2010	Diab	RE43,860 E	12/2012	Parker
7,822,452 B2	10/2010	Schurman et al.	8,337,403 B2	12/2012	Al-Ali et al.
RE41,912 E	11/2010	Parker	8,346,330 B2	1/2013	Lamego
7,844,313 B2	11/2010	Kiani et al.	8,353,842 B2	1/2013	Al-Ali et al.
7,844,314 B2	11/2010	Al-Ali	8,355,766 B2	1/2013	MacNeish, III et al.
7,844,315 B2	11/2010	Al-Ali	8,359,080 B2	1/2013	Diab et al.
7,865,222 B2	1/2011	Weber et al.	8,364,223 B2	1/2013	Al-Ali et al.
7,873,497 B2	1/2011	Weber et al.	8,364,226 B2	1/2013	Diab et al.
7,880,606 B2	2/2011	Al-Ali	8,374,665 B2	2/2013	Lamego
7,880,626 B2	2/2011	Al-Ali et al.	8,385,995 B2	2/2013	Al-Ali et al.
7,891,355 B2	2/2011	Al-Ali et al.	8,385,996 B2	2/2013	Smith et al.
7,894,868 B2	2/2011	Al-Ali et al.	8,388,353 B2	3/2013	Kiani
7,899,507 B2	3/2011	Al-Ali et al.	8,399,822 B2	3/2013	Al-Ali
7,899,518 B2	3/2011	Trepagnier et al.	8,401,602 B2	3/2013	Kiani
7,904,132 B2	3/2011	Weber et al.	8,405,608 B2	3/2013	Al-Ali et al.
7,909,772 B2	3/2011	Popov et al.	8,414,499 B2	4/2013	Al-Ali et al.
7,910,875 B2	3/2011	Al-Ali	8,418,524 B2	4/2013	Al-Ali
7,919,713 B2	4/2011	Al-Ali et al.	8,423,106 B2	4/2013	Lamego et al.
7,937,128 B2	5/2011	Al-Ali	8,428,967 B2	4/2013	Olsen et al.
7,937,129 B2	5/2011	Mason et al.	8,430,817 B1	4/2013	Al-Ali et al.
7,937,130 B2	5/2011	Diab et al.	8,437,825 B2	5/2013	Dalvi et al.
7,941,199 B2	5/2011	Kiani	8,455,290 B2	6/2013	Siskavich
7,951,086 B2	5/2011	Flaherty et al.	8,457,703 B2	6/2013	Al-Ali
7,957,780 B2	6/2011	Lamego et al.	8,457,707 B2	6/2013	Kiani
7,962,188 B2	6/2011	Kiani et al.	8,463,349 B2	6/2013	Diab et al.
7,962,190 B1	6/2011	Diab et al.	8,466,286 B2	6/2013	Bellot et al.
7,976,472 B2	7/2011	Kiani	8,471,713 B2	6/2013	Poeze et al.
7,988,637 B2	8/2011	Diab	8,473,020 B2	6/2013	Kiani et al.
7,990,382 B2	8/2011	Kiani	8,483,787 B2	7/2013	Al-Ali et al.
7,991,446 B2	8/2011	Ali et al.	8,489,364 B2	7/2013	Weber et al.
8,000,761 B2	8/2011	Al-Ali	8,498,684 B2	7/2013	Weber et al.
8,008,088 B2	8/2011	Bellott et al.	8,504,128 B2	8/2013	Blank et al.
RE42,753 E	9/2011	Kiani-Azarbayjany et al.	8,509,867 B2	8/2013	Workman et al.
8,019,400 B2	9/2011	Diab et al.	8,515,509 B2	8/2013	Bruinsma et al.
8,028,701 B2	10/2011	Al-Ali et al.	8,523,781 B2	9/2013	Al-Ali
8,029,765 B2	10/2011	Bellott et al.	8,529,301 B2	9/2013	Al-Ali et al.
8,036,727 B2	10/2011	Schurman et al.	8,532,727 B2	9/2013	Ali et al.
8,036,728 B2	10/2011	Diab et al.	8,532,728 B2	9/2013	Diab et al.
8,046,040 B2	10/2011	Ali et al.	D692,145 S	10/2013	Al-Ali et al.
8,046,041 B2	10/2011	Diab et al.	8,547,209 B2	10/2013	Kiani et al.
8,046,042 B2	10/2011	Diab et al.	8,548,548 B2	10/2013	Al-Ali
8,048,040 B2	11/2011	Kiani	8,548,549 B2	10/2013	Schurman et al.
8,050,728 B2	11/2011	Al-Ali et al.	8,548,550 B2	10/2013	Al-Ali et al.
RE43,169 E	2/2012	Parker	8,560,032 B2	10/2013	Al-Ali et al.
8,118,620 B2	2/2012	Al-Ali et al.	8,560,034 B1	10/2013	Diab et al.
8,126,528 B2	2/2012	Diab et al.	8,570,167 B2	10/2013	Al-Ali
8,128,572 B2	3/2012	Diab et al.	8,570,503 B2	10/2013	Vo et al.
8,130,105 B2	3/2012	Al-Ali et al.	8,571,617 B2	10/2013	Reichgott et al.
8,145,287 B2	3/2012	Diab et al.	8,571,618 B1	10/2013	Lamego et al.
8,150,487 B2	4/2012	Diab et al.	8,571,619 B2	10/2013	Al-Ali et al.
8,175,672 B2	5/2012	Parker	8,577,431 B2	11/2013	Lamego et al.
8,180,420 B2	5/2012	Diab et al.	8,581,732 B2	11/2013	Al-Ali et al.
8,182,443 B1	5/2012	Kiani	8,584,345 B2	11/2013	Al-Ali et al.
8,185,180 B2	5/2012	Diab et al.	8,588,880 B2	11/2013	Abdul-Hafiz et al.
8,190,223 B2	5/2012	Al-Ali et al.	8,600,467 B2	12/2013	Al-Ali et al.
8,190,227 B2	5/2012	Diab et al.	8,606,342 B2	12/2013	Diab
8,203,438 B2	6/2012	Kiani et al.	8,626,255 B2	1/2014	Al-Ali et al.
8,203,704 B2	6/2012	Merritt et al.	8,630,691 B2	1/2014	Lamego et al.
8,204,566 B2	6/2012	Schurman et al.	8,634,889 B2	1/2014	Al-Ali et al.
8,219,172 B2	7/2012	Schurman et al.	8,641,631 B2	2/2014	Sierra et al.
8,224,411 B2	7/2012	Al-Ali et al.	8,652,060 B2	2/2014	Al-Ali
8,228,181 B2	7/2012	Al-Ali	8,663,107 B2	3/2014	Kiani
8,229,533 B2	7/2012	Diab et al.	8,666,468 B1	3/2014	Al-Ali
8,233,955 B2	7/2012	Al-Ali et al.	8,667,967 B2	3/2014	Al-Ali et al.
8,244,325 B2	8/2012	Al-Ali et al.	8,670,811 B2	3/2014	O'Reilly
8,255,026 B1	8/2012	Al-Ali	8,670,814 B2	3/2014	Diab et al.
8,255,027 B2	8/2012	Al-Ali et al.	8,676,286 B2	3/2014	Weber et al.
8,255,028 B2	8/2012	Al-Ali et al.	8,682,407 B2	3/2014	Al-Ali
8,260,577 B2	9/2012	Weber et al.	RE44,823 E	4/2014	Parker
8,265,723 B1	9/2012	McHale et al.	RE44,875 E	4/2014	Kiani et al.
8,274,360 B2	9/2012	SamPATH et al.	8,690,799 B2	4/2014	Telfort et al.
8,301,217 B2	10/2012	Al-Ali et al.	8,700,112 B2	4/2014	Kiani
8,306,596 B2	11/2012	Schurman et al.	8,702,627 B2	4/2014	Telfort et al.
8,310,336 B2	11/2012	Muhsin et al.	8,706,179 B2	4/2014	Parker
			8,712,494 B1	4/2014	MacNeish, III et al.
			8,715,206 B2	5/2014	Telfort et al.
			8,718,735 B2	5/2014	Lamego et al.
			8,718,737 B2	5/2014	Diab et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

8,718,738 B2	5/2014	Blank et al.	9,142,117 B2	9/2015	Muhsin et al.
8,720,249 B2	5/2014	Al-Ali	9,153,112 B1	10/2015	Kiani et al.
8,721,541 B2	5/2014	Al-Ali et al.	9,153,121 B2	10/2015	Kiani et al.
8,721,542 B2	5/2014	Al-Ali et al.	9,161,696 B2	10/2015	Al-Ali et al.
8,723,677 B1	5/2014	Kiani	9,161,713 B2	10/2015	Al-Ali et al.
8,740,792 B1	6/2014	Kiani et al.	9,167,995 B2	10/2015	Lamego et al.
8,754,776 B2	6/2014	Poeze et al.	9,176,141 B2	11/2015	Al-Ali et al.
8,755,535 B2	6/2014	Telfort et al.	9,186,102 B2	11/2015	Bruinsma et al.
8,755,856 B2	6/2014	Diab et al.	9,192,312 B2	11/2015	Al-Ali
8,755,872 B1	6/2014	Marinow	9,192,329 B2	11/2015	Al-Ali
8,761,850 B2	6/2014	Lamego	9,192,351 B1	11/2015	Telfort et al.
8,764,671 B2	7/2014	Kiani	9,195,385 B2	11/2015	Al-Ali et al.
8,768,423 B2	7/2014	Shakespeare et al.	9,211,072 B2	12/2015	Kiani
8,771,204 B2	7/2014	Telfort et al.	9,211,095 B1	12/2015	Al-Ali
8,777,634 B2	7/2014	Kiani et al.	9,218,454 B2	12/2015	Kiani et al.
8,781,543 B2	7/2014	Diab et al.	9,226,696 B2	1/2016	Kiani
8,781,544 B2	7/2014	Al-Ali et al.	9,241,662 B2	1/2016	Al-Ali et al.
8,781,549 B2	7/2014	Al-Ali et al.	9,245,668 B1	1/2016	Vo et al.
8,788,003 B2	7/2014	Schurman et al.	9,259,185 B2	2/2016	Abdul-Hafiz et al.
8,790,268 B2	7/2014	Al-Ali	9,267,572 B2	2/2016	Barker et al.
8,801,613 B2	8/2014	Al-Ali et al.	9,277,880 B2	3/2016	Poeze et al.
8,821,397 B2	9/2014	Al-Ali et al.	9,289,167 B2	3/2016	Diab et al.
8,821,415 B2	9/2014	Al-Ali et al.	9,295,421 B2	3/2016	Kiani et al.
8,830,449 B1	9/2014	Lamego et al.	9,307,928 B1	4/2016	Al-Ali et al.
8,831,700 B2	9/2014	Schurman et al.	9,323,894 B2	4/2016	Kiani
8,840,549 B2	9/2014	Al-Ali et al.	D755,392 S	5/2016	Hwang et al.
8,847,740 B2	9/2014	Kiani et al.	9,326,712 B1	5/2016	Kiani
8,849,365 B2	9/2014	Smith et al.	9,333,316 B2	5/2016	Kiani
8,852,094 B2	10/2014	Al-Ali et al.	9,339,220 B2	5/2016	Lamego et al.
8,852,994 B2	10/2014	Wojtczuk et al.	9,341,565 B2	5/2016	Lamego et al.
8,868,147 B2	10/2014	Stippick et al.	9,351,673 B2	5/2016	Diab et al.
8,868,150 B2	10/2014	Al-Ali et al.	9,351,675 B2	5/2016	Al-Ali et al.
8,870,792 B2	10/2014	Al-Ali et al.	9,364,181 B2	6/2016	Kiani et al.
8,886,271 B2	11/2014	Kiani et al.	9,368,671 B2	6/2016	Wojtczuk et al.
8,888,539 B2	11/2014	Al-Ali et al.	9,370,325 B2	6/2016	Al-Ali et al.
8,888,708 B2	11/2014	Diab et al.	9,370,326 B2	6/2016	McHale et al.
8,892,180 B2	11/2014	Weber et al.	9,370,335 B2	6/2016	Al-Ali et al.
8,897,847 B2	11/2014	Al-Ali	9,375,185 B2	6/2016	Ali et al.
8,909,310 B2	12/2014	Lamego et al.	9,386,953 B2	7/2016	Al-Ali
8,911,377 B2	12/2014	Al-Ali	9,386,961 B2	7/2016	Al-Ali et al.
8,912,909 B2	12/2014	Al-Ali et al.	9,392,945 B2	7/2016	Al-Ali et al.
8,920,317 B2	12/2014	Al-Ali et al.	9,397,448 B2	7/2016	Al-Ali et al.
8,921,699 B2	12/2014	Al-Ali et al.	9,408,542 B1 *	8/2016	Kinast A61B 5/02125
8,922,382 B2	12/2014	Al-Ali et al.	9,436,645 B2	9/2016	Al-Ali et al.
8,929,964 B2	1/2015	Al-Ali et al.	9,445,759 B1	9/2016	Lamego et al.
8,942,777 B2	1/2015	Diab et al.	9,466,919 B2	10/2016	Kiani et al.
8,948,834 B2	2/2015	Diab et al.	9,474,474 B2	10/2016	Lamego et al.
8,948,835 B2	2/2015	Diab	9,480,422 B2	11/2016	Al-Ali
8,965,471 B2	2/2015	Lamego	9,480,435 B2	11/2016	Olsen
8,983,564 B2	3/2015	Al-Ali	9,492,110 B2	11/2016	Al-Ali et al.
8,989,831 B2	3/2015	Al-Ali et al.	9,510,779 B2	12/2016	Poeze et al.
8,996,085 B2	3/2015	Kiani et al.	9,517,024 B2	12/2016	Kiani et al.
8,998,809 B2	4/2015	Kiani	9,532,722 B2	1/2017	Lamego et al.
9,028,429 B2	5/2015	Telfort et al.	9,538,949 B2	1/2017	Al-Ali et al.
9,037,207 B2	5/2015	Al-Ali et al.	9,538,980 B2	1/2017	Telfort et al.
9,060,721 B2	6/2015	Reichgott et al.	9,549,696 B2	1/2017	Lamego et al.
9,066,666 B2	6/2015	Kiani	9,554,737 B2	1/2017	Schurman et al.
9,066,680 B1	6/2015	Al-Ali et al.	9,560,996 B2	2/2017	Kiani
9,072,474 B2	7/2015	Al-Ali et al.	9,560,998 B2	2/2017	Al-Ali et al.
9,078,560 B2	7/2015	Schurman et al.	9,566,019 B2	2/2017	Al-Ali et al.
9,084,569 B2	7/2015	Weber et al.	9,579,039 B2	2/2017	Jansen et al.
9,095,316 B2	8/2015	Welch et al.	9,591,975 B2	3/2017	Dalvi et al.
9,106,038 B2	8/2015	Telfort et al.	9,622,693 B2	4/2017	Diab
9,107,625 B2	8/2015	Telfort et al.	2003/0018248 A1 *	1/2003	Kreger A61B 5/0456 600/413
9,107,626 B2	8/2015	Al-Ali et al.	2003/0171661 A1 *	9/2003	Tong A61B 5/04004 600/300
9,113,831 B2	8/2015	Al-Ali	2007/0282478 A1	12/2007	Al-Ali et al.
9,113,832 B2	8/2015	Al-Ali	2009/0247984 A1	10/2009	Lamego et al.
9,119,595 B2	9/2015	Lamego	2009/0275813 A1	11/2009	Davis
9,131,881 B2	9/2015	Diab et al.	2009/0275844 A1	11/2009	Al-Ali
9,131,882 B2	9/2015	Al-Ali et al.	2010/0004518 A1	1/2010	Vo et al.
9,131,883 B2	9/2015	Al-Ali	2010/0030040 A1	2/2010	Poeze et al.
9,131,917 B2	9/2015	Telfort et al.	2010/0060350 A1 *	3/2010	Zhang H03H 11/1286 327/553
9,138,180 B1	9/2015	Coverston et al.	2011/0082711 A1	4/2011	Poeze et al.
9,138,182 B2	9/2015	Al-Ali et al.	2011/0087083 A1	4/2011	Poeze et al.
9,138,192 B2	9/2015	Weber et al.	2011/0105854 A1	5/2011	Kiani et al.
			2011/0125060 A1	5/2011	Telfort et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2011/0208015	A1	8/2011	Welch et al.	2014/0316218	A1	10/2014	Purdon et al.
2011/0213212	A1	9/2011	Al-Ali	2014/0316228	A1	10/2014	Blank et al.
2011/0230733	A1	9/2011	Al-Ali	2014/0323825	A1	10/2014	Al-Ali et al.
2011/0237969	A1	9/2011	Eckerbom et al.	2014/0323897	A1	10/2014	Brown et al.
2011/0288383	A1	11/2011	Diab	2014/0323898	A1	10/2014	Purdon et al.
2011/0301444	A1	12/2011	Al-Ali	2014/0330092	A1	11/2014	Al-Ali et al.
2012/0041316	A1	2/2012	Al-Ali et al.	2014/0330098	A1	11/2014	Merritt et al.
2012/0046557	A1	2/2012	Kiani	2014/0330099	A1	11/2014	Al-Ali et al.
2012/0059267	A1	3/2012	Lamego et al.	2014/0336481	A1	11/2014	Shakespeare et al.
2012/0088984	A1	4/2012	Al-Ali et al.	2014/0357966	A1	12/2014	Al-Ali et al.
2012/0165629	A1	6/2012	Merritt et al.	2014/0371548	A1	12/2014	Al-Ali et al.
2012/0179006	A1	7/2012	Jansen et al.	2014/0371632	A1	12/2014	Al-Ali et al.
2012/0209082	A1	8/2012	Al-Ali	2014/0378784	A1	12/2014	Kiani et al.
2012/0209084	A1	8/2012	Olsen et al.	2015/0005600	A1	1/2015	Blank et al.
2012/0283524	A1	11/2012	Kiani et al.	2015/0011907	A1	1/2015	Purdon et al.
2012/0296178	A1	11/2012	Lamego et al.	2015/0012231	A1	1/2015	Poeze et al.
2012/0319816	A1	12/2012	Al-Ali	2015/0018650	A1	1/2015	Al-Ali et al.
2012/0330112	A1	12/2012	Lamego et al.	2015/0025406	A1	1/2015	Al-Ali
2013/0023775	A1	1/2013	Lamego et al.	2015/0032029	A1	1/2015	Al-Ali et al.
2013/0041591	A1	2/2013	Lamego	2015/0038859	A1	2/2015	Dalvi et al.
2013/0046204	A1	2/2013	Lamego et al.	2015/0045637	A1	2/2015	Dalvi
2013/0060147	A1	3/2013	Welch et al.	2015/0051462	A1	2/2015	Olsen
2013/0096405	A1	4/2013	Garfio	2015/0080754	A1	3/2015	Purdon et al.
2013/0096936	A1	4/2013	SamPATH et al.	2015/0087936	A1	3/2015	Al-Ali et al.
2013/0190581	A1	7/2013	Al-Ali et al.	2015/0094546	A1	4/2015	Al-Ali
2013/0211214	A1	8/2013	Olsen	2015/0097701	A1	4/2015	Al-Ali et al.
2013/0243021	A1	9/2013	Siskavich	2015/0099950	A1	4/2015	Al-Ali et al.
2013/0253334	A1	9/2013	Al-Ali et al.	2015/0099951	A1	4/2015	Al-Ali et al.
2013/0262730	A1	10/2013	Al-Ali et al.	2015/0099955	A1	4/2015	Al-Ali et al.
2013/0267804	A1	10/2013	Al-Ali	2015/0101844	A1	4/2015	Al-Ali et al.
2013/0274572	A1	10/2013	Al-Ali et al.	2015/0106121	A1	4/2015	Muhsin et al.
2013/0296672	A1	11/2013	O'Neil et al.	2015/0112151	A1	4/2015	Muhsin et al.
2013/0296713	A1	11/2013	Al-Ali et al.	2015/0116076	A1	4/2015	Al-Ali et al.
2013/0317370	A1	11/2013	Dalvi et al.	2015/0126830	A1	5/2015	Schurman et al.
2013/0324808	A1	12/2013	Al-Ali et al.	2015/0133755	A1	5/2015	Smith et al.
2013/0331660	A1	12/2013	Al-Ali et al.	2015/0140863	A1	5/2015	Al-Ali et al.
2013/0331670	A1	12/2013	Kiani	2015/0141781	A1	5/2015	Weber et al.
2014/0012100	A1	1/2014	Al-Ali et al.	2015/0165312	A1	6/2015	Kiani
2014/0034353	A1	2/2014	Al-Ali et al.	2015/0196237	A1	7/2015	Lamego
2014/0051953	A1	2/2014	Lamego et al.	2015/0201874	A1	7/2015	Diab
2014/0066783	A1	3/2014	Kiani et al.	2015/0208966	A1	7/2015	Al-Ali
2014/0077956	A1	3/2014	SamPATH et al.	2015/0216459	A1	8/2015	Al-Ali et al.
2014/0081100	A1	3/2014	Muhsin et al.	2015/0230755	A1	8/2015	Al-Ali et al.
2014/0081175	A1	3/2014	Telfort	2015/0238722	A1	8/2015	Al-Ali
2014/0094667	A1	4/2014	Schurman et al.	2015/0245773	A1	9/2015	Lamego et al.
2014/0100434	A1	4/2014	Diab et al.	2015/0245794	A1	9/2015	Al-Ali
2014/0114199	A1	4/2014	Lamego et al.	2015/0257689	A1	9/2015	Al-Ali et al.
2014/0120564	A1	5/2014	Workman et al.	2015/0272514	A1	10/2015	Kiani et al.
2014/0121482	A1	5/2014	Merritt et al.	2015/0351697	A1	12/2015	Weber et al.
2014/0121483	A1	5/2014	Kiani	2015/0351704	A1	12/2015	Kiani et al.
2014/0127137	A1	5/2014	Bellott et al.	2015/0359429	A1	12/2015	Al-Ali et al.
2014/0129702	A1	5/2014	Lamego et al.	2015/0366472	A1	12/2015	Kiani
2014/0135588	A1	5/2014	Al-Ali et al.	2015/0366507	A1	12/2015	Blank
2014/0142401	A1	5/2014	Al-Ali et al.	2015/0374298	A1	12/2015	Al-Ali et al.
2014/0163344	A1	6/2014	Al-Ali	2015/0380875	A1	12/2015	Coverston et al.
2014/0163402	A1	6/2014	Lamego et al.	2016/0000362	A1	1/2016	Diab et al.
2014/0166076	A1	6/2014	Kiani et al.	2016/0007930	A1	1/2016	Weber et al.
2014/0171763	A1	6/2014	Diab	2016/0029932	A1	2/2016	Al-Ali
2014/0180038	A1	6/2014	Kiani	2016/0029933	A1	2/2016	Al-Ali et al.
2014/0180154	A1	6/2014	Sierra et al.	2016/0045118	A1	2/2016	Kiani
2014/0180160	A1	6/2014	Brown et al.	2016/0051205	A1	2/2016	Al-Ali et al.
2014/0187973	A1	7/2014	Brown et al.	2016/0058338	A1	3/2016	Schurman et al.
2014/0194766	A1	7/2014	Al-Ali et al.	2016/0058347	A1	3/2016	Reichgott et al.
2014/0206963	A1	7/2014	Al-Ali	2016/0066823	A1	3/2016	Kind et al.
2014/0213864	A1	7/2014	Abdul-Hafiz et al.	2016/0066824	A1	3/2016	Al-Ali et al.
2014/0266790	A1	9/2014	Al-Ali et al.	2016/0066879	A1	3/2016	Telfort et al.
2014/0275808	A1	9/2014	Poeze et al.	2016/0072429	A1	3/2016	Kiani et al.
2014/0275835	A1	9/2014	Lamego et al.	2016/0073967	A1	3/2016	Lamego et al.
2014/0275871	A1	9/2014	Lamego et al.	2016/0081552	A1	3/2016	Wojtczuk et al.
2014/0275872	A1	9/2014	Merritt et al.	2016/0095543	A1	4/2016	Telfort et al.
2014/0275881	A1	9/2014	Lamego et al.	2016/0095548	A1	4/2016	Al-Ali et al.
2014/0276115	A1	9/2014	Dalvi et al.	2016/0103598	A1	4/2016	Al-Ali et al.
2014/0288400	A1	9/2014	Diab et al.	2016/0113527	A1	4/2016	Al-Ali et al.
2014/0303520	A1	10/2014	Telfort et al.	2016/0143548	A1	5/2016	Al-Ali
2014/0316217	A1	10/2014	Purdon et al.	2016/0166183	A1	6/2016	Poeze et al.
				2016/0166188	A1	6/2016	Bruinsma et al.
				2016/0166210	A1	6/2016	Al-Ali
				2016/0192869	A1	7/2016	Kiani et al.
				2016/0196388	A1	7/2016	Lamego

(56)

References Cited

U.S. PATENT DOCUMENTS

2016/0197436 A1 7/2016 Barker et al.
2016/0213281 A1 7/2016 Eckerbom et al.
2016/0228043 A1 8/2016 O'Neil et al.
2016/0233632 A1 8/2016 Scruggs et al.
2016/0234944 A1 8/2016 Schmidt et al.
2016/0270735 A1 9/2016 Diab et al.
2016/0283665 A1 9/2016 Sampath et al.
2016/0287090 A1 10/2016 Al-Ali et al.
2016/0287786 A1 10/2016 Kiani
2016/0296169 A1 10/2016 McHale et al.
2016/0310052 A1 10/2016 Al-Ali et al.
2016/0314260 A1 10/2016 Kiani
2016/0324486 A1 11/2016 Al-Ali et al.
2016/0324488 A1 11/2016 Olsen
2016/0327984 A1 11/2016 Al-Ali et al.
2016/0328528 A1 11/2016 Al-Ali et al.
2016/0331332 A1 11/2016 Al-Ali
2016/0367173 A1 12/2016 Dalvi et al.
2017/0007134 A1 1/2017 Al-Ali et al.
2017/0007190 A1 1/2017 Al-Ali et al.
2017/0007198 A1 1/2017 Al-Ali et al.
2017/0014084 A1 1/2017 Al-Ali et al.
2017/0021099 A1 1/2017 Al-Ali et al.
2017/0027456 A1 2/2017 Kinast et al.
2017/0042488 A1 2/2017 Muhsin
2017/0055847 A1 3/2017 Kiani et al.
2017/0055851 A1 3/2017 Al-Ali
2017/0055882 A1 3/2017 Al-Ali et al.
2017/0055887 A1 3/2017 Al-Ali
2017/0055896 A1 3/2017 Al-Ali et al.
2017/0079594 A1 3/2017 Telfort et al.
2017/0086723 A1 3/2017 Al-Ali et al.

* cited by examiner

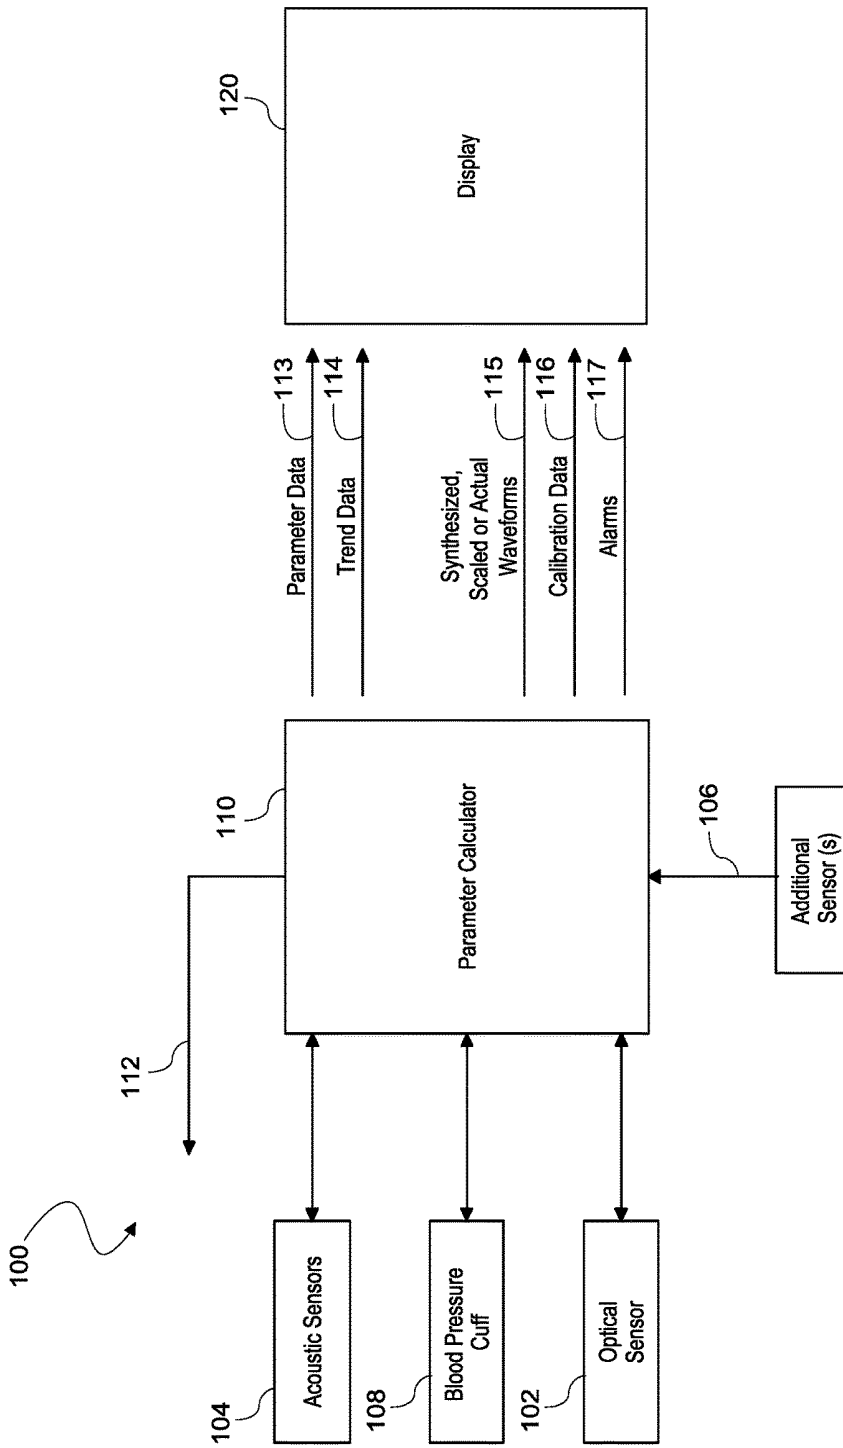


FIG. 1

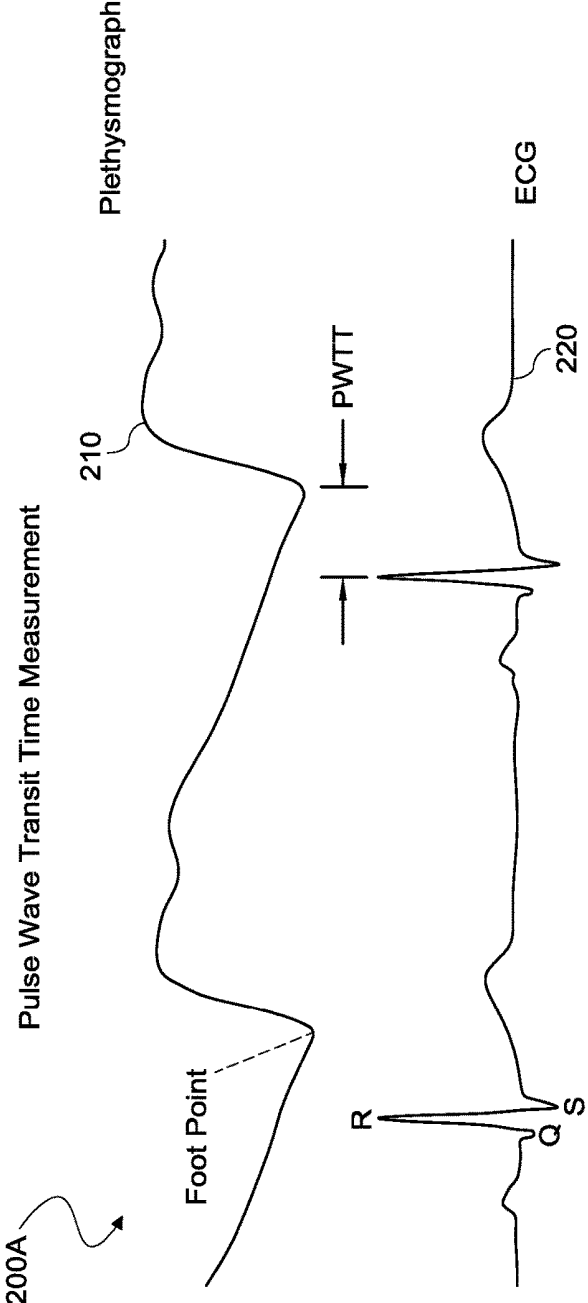


FIG. 2A

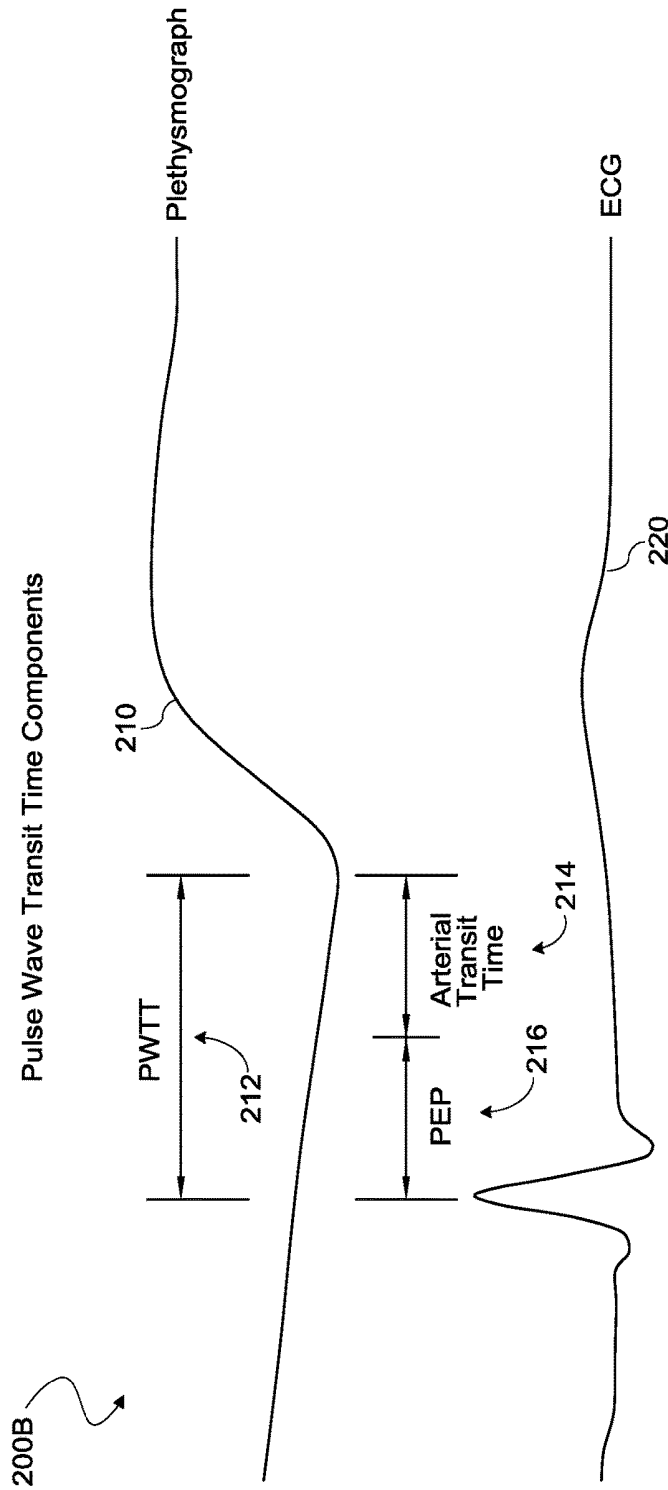


FIG. 2B

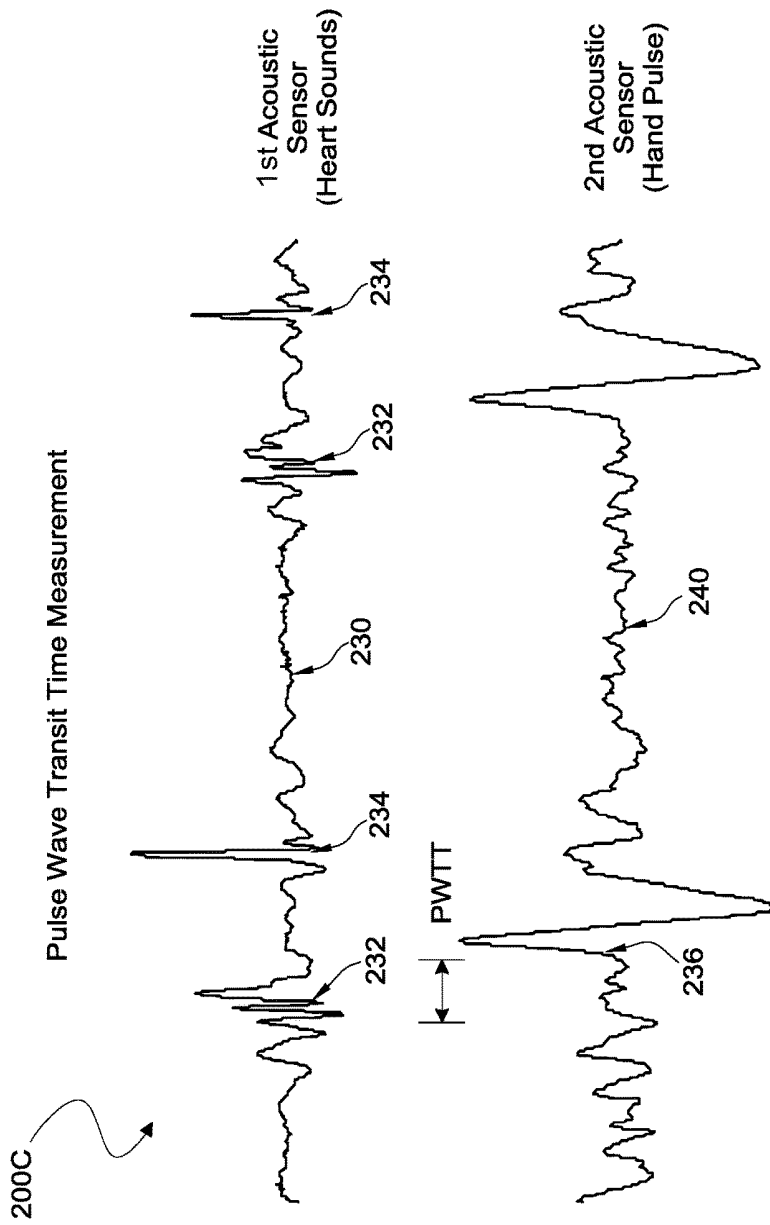


FIG. 2C

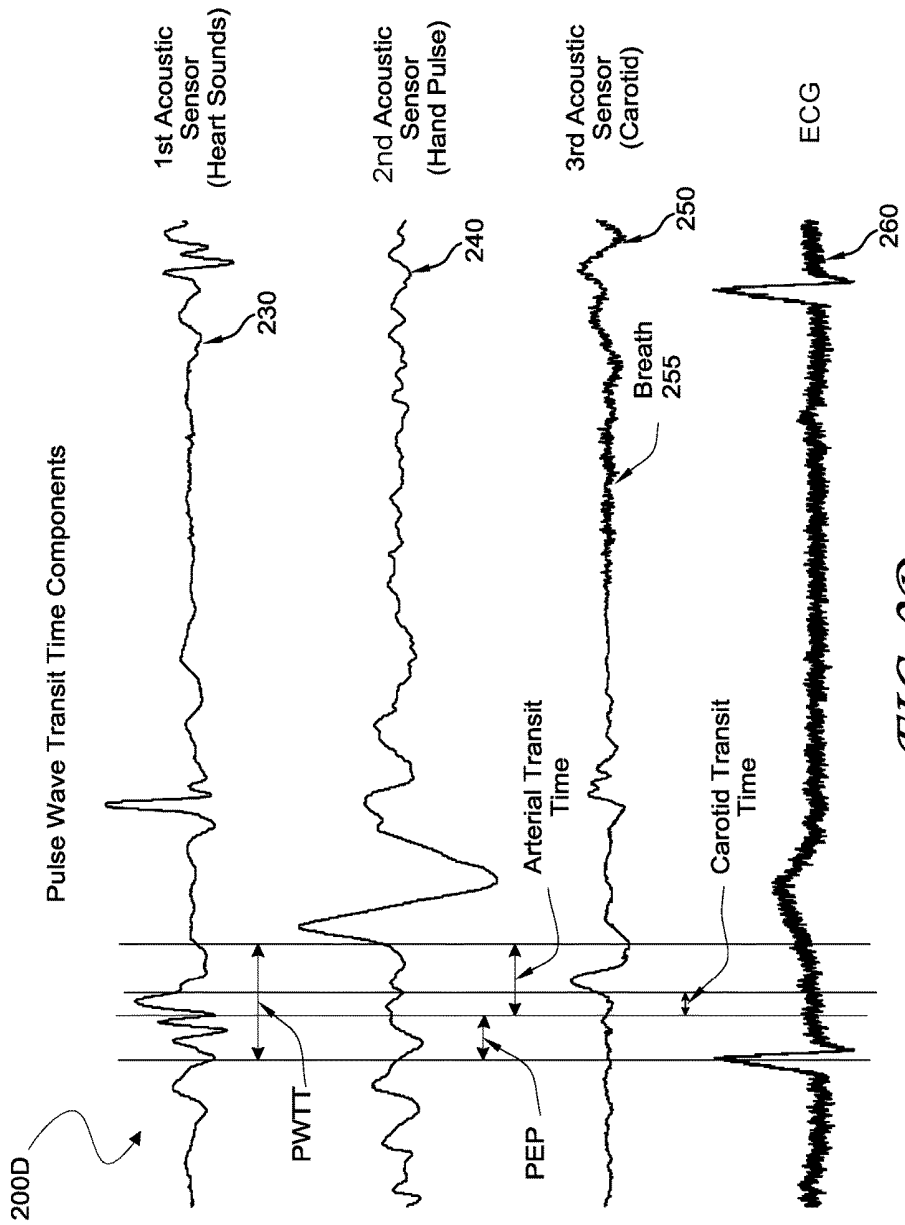


FIG. 2D

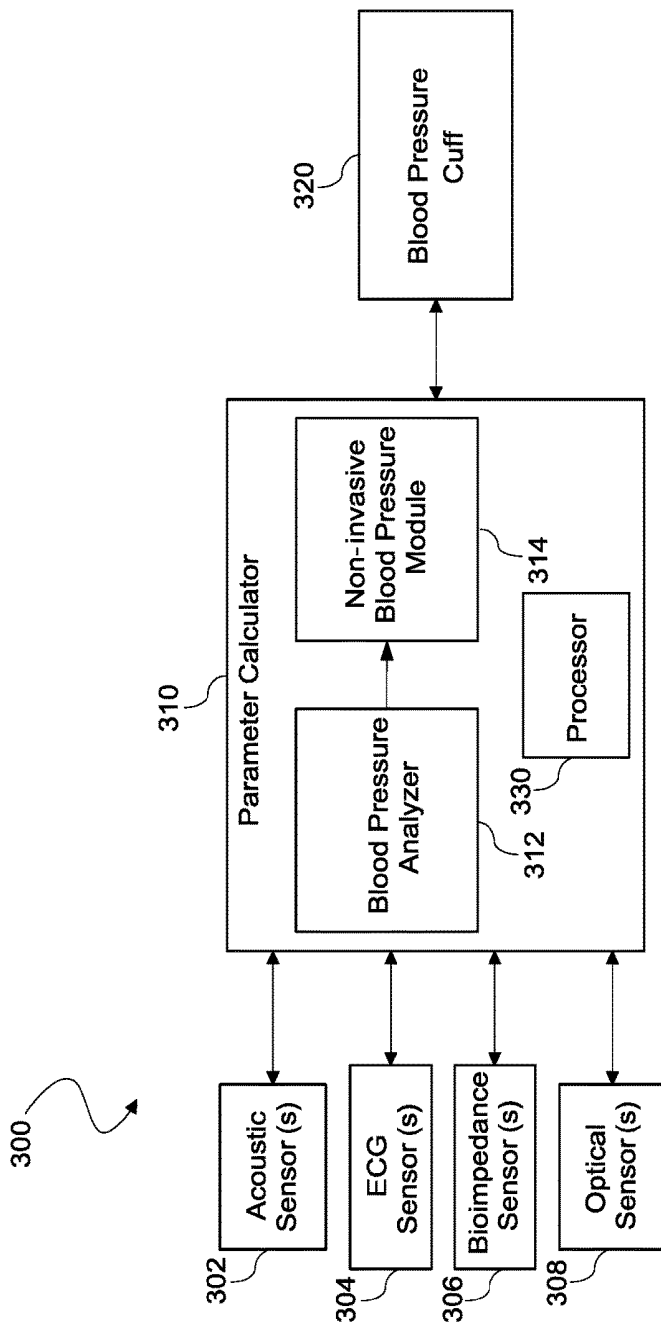


FIG. 3

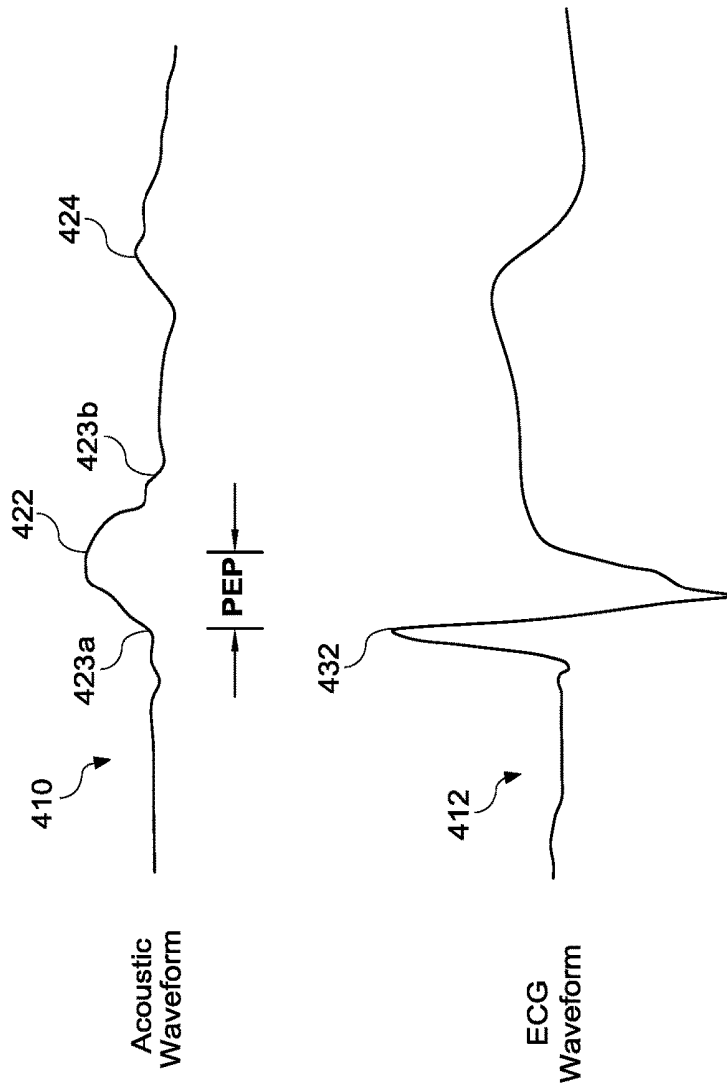


FIG. 4A

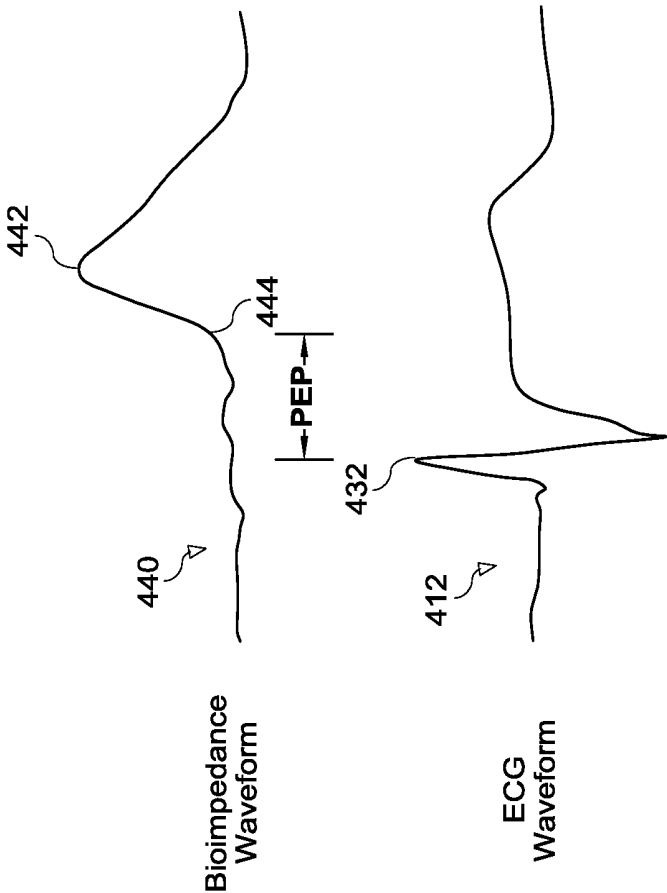


FIG. 4B

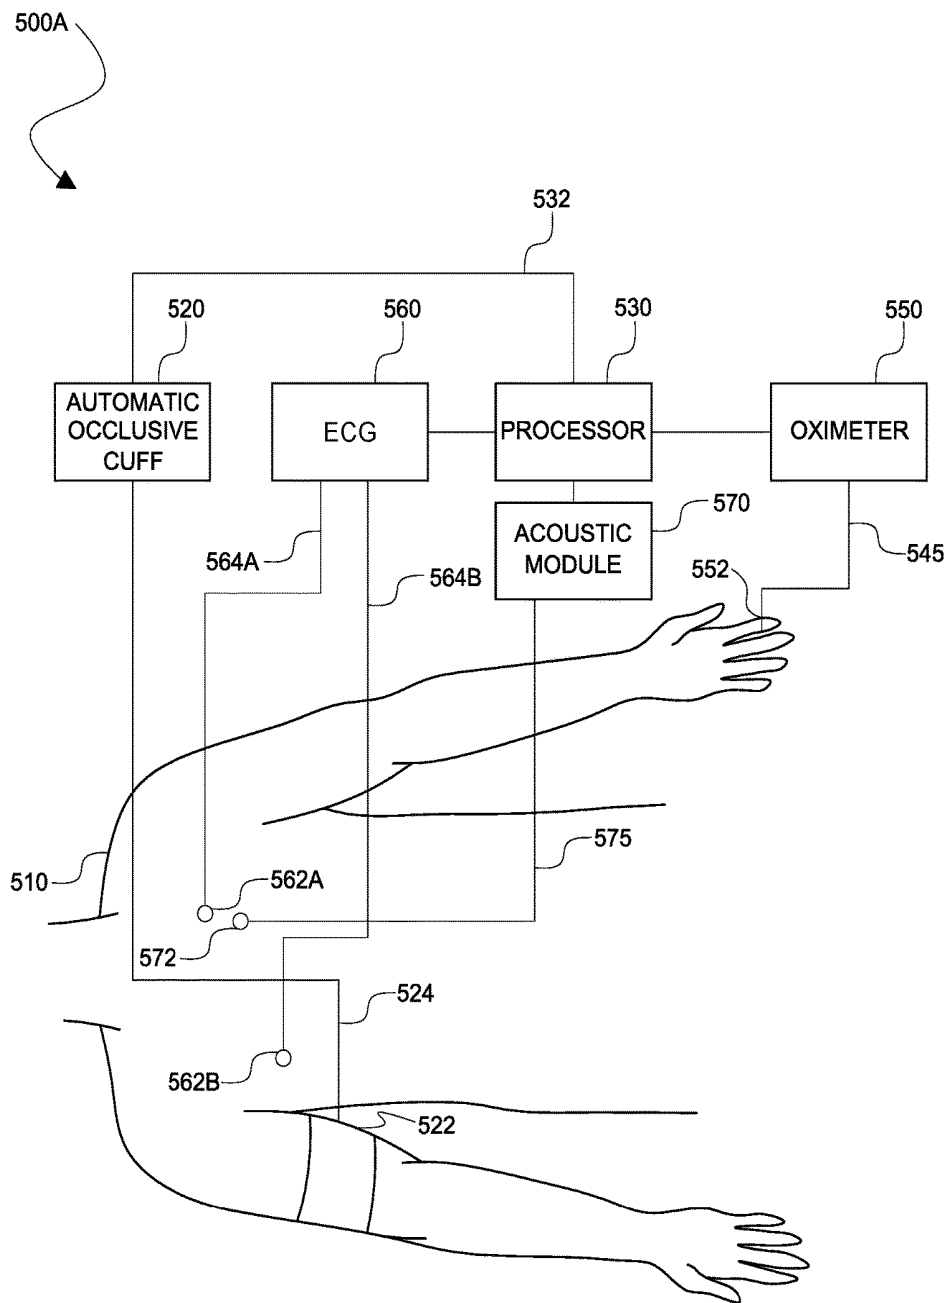


FIG. 5A

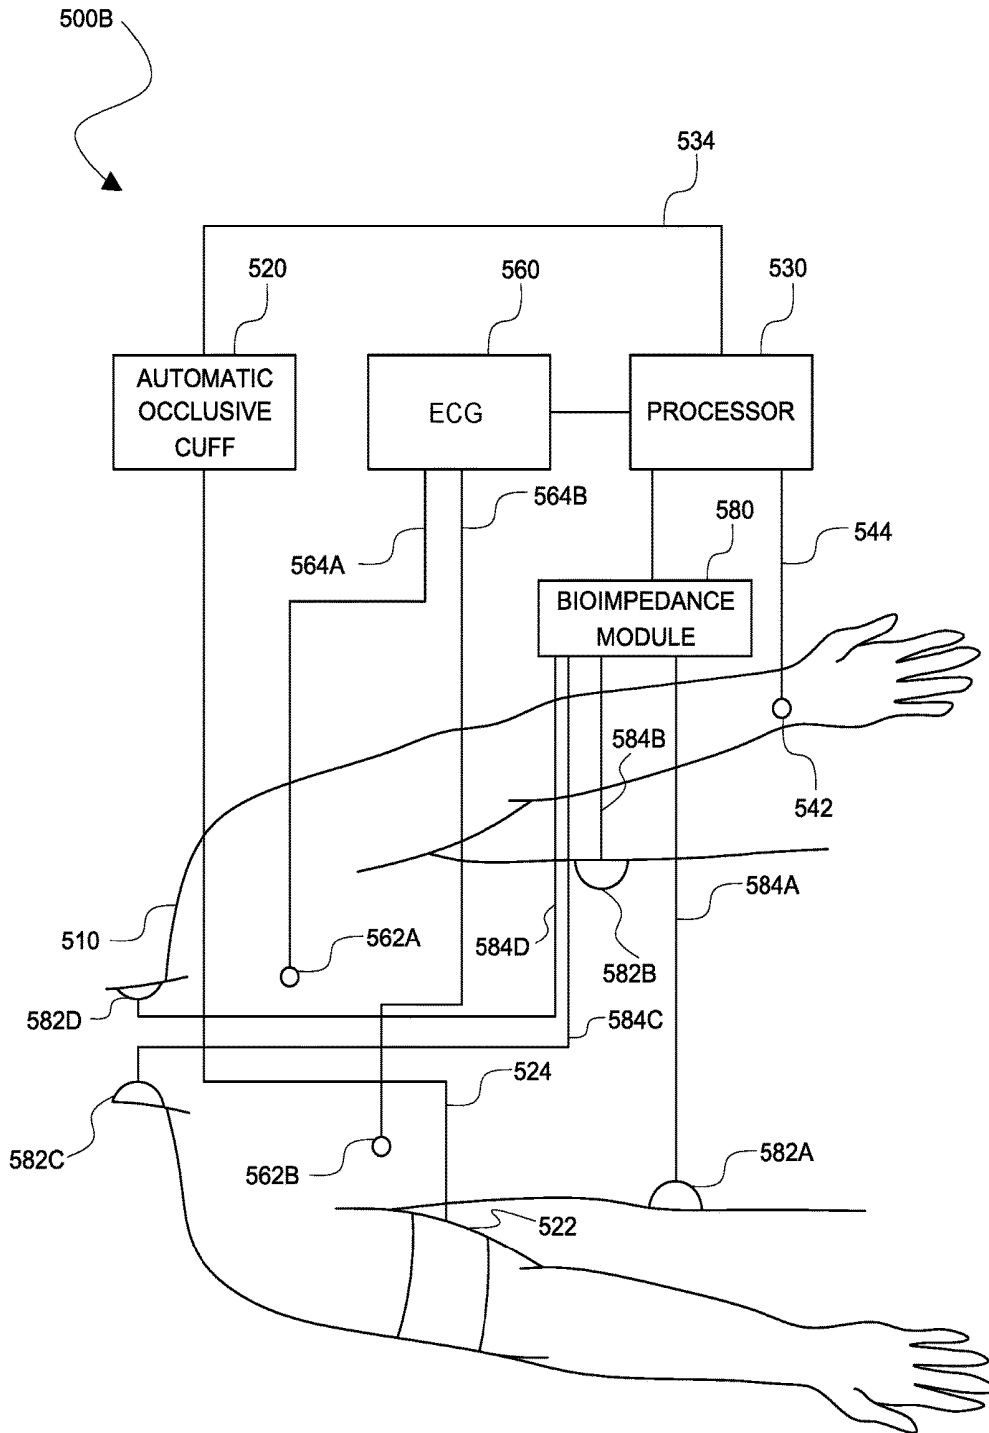
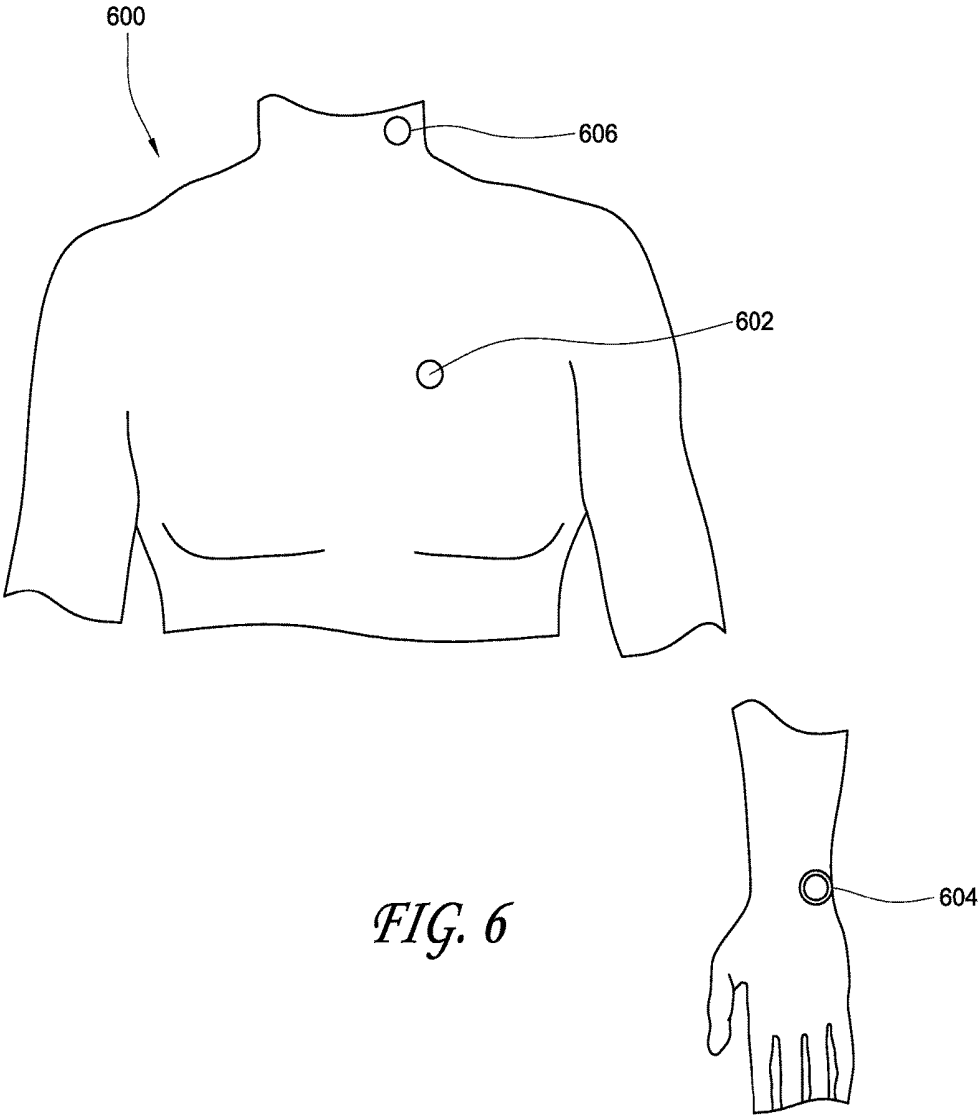


FIG. 5B



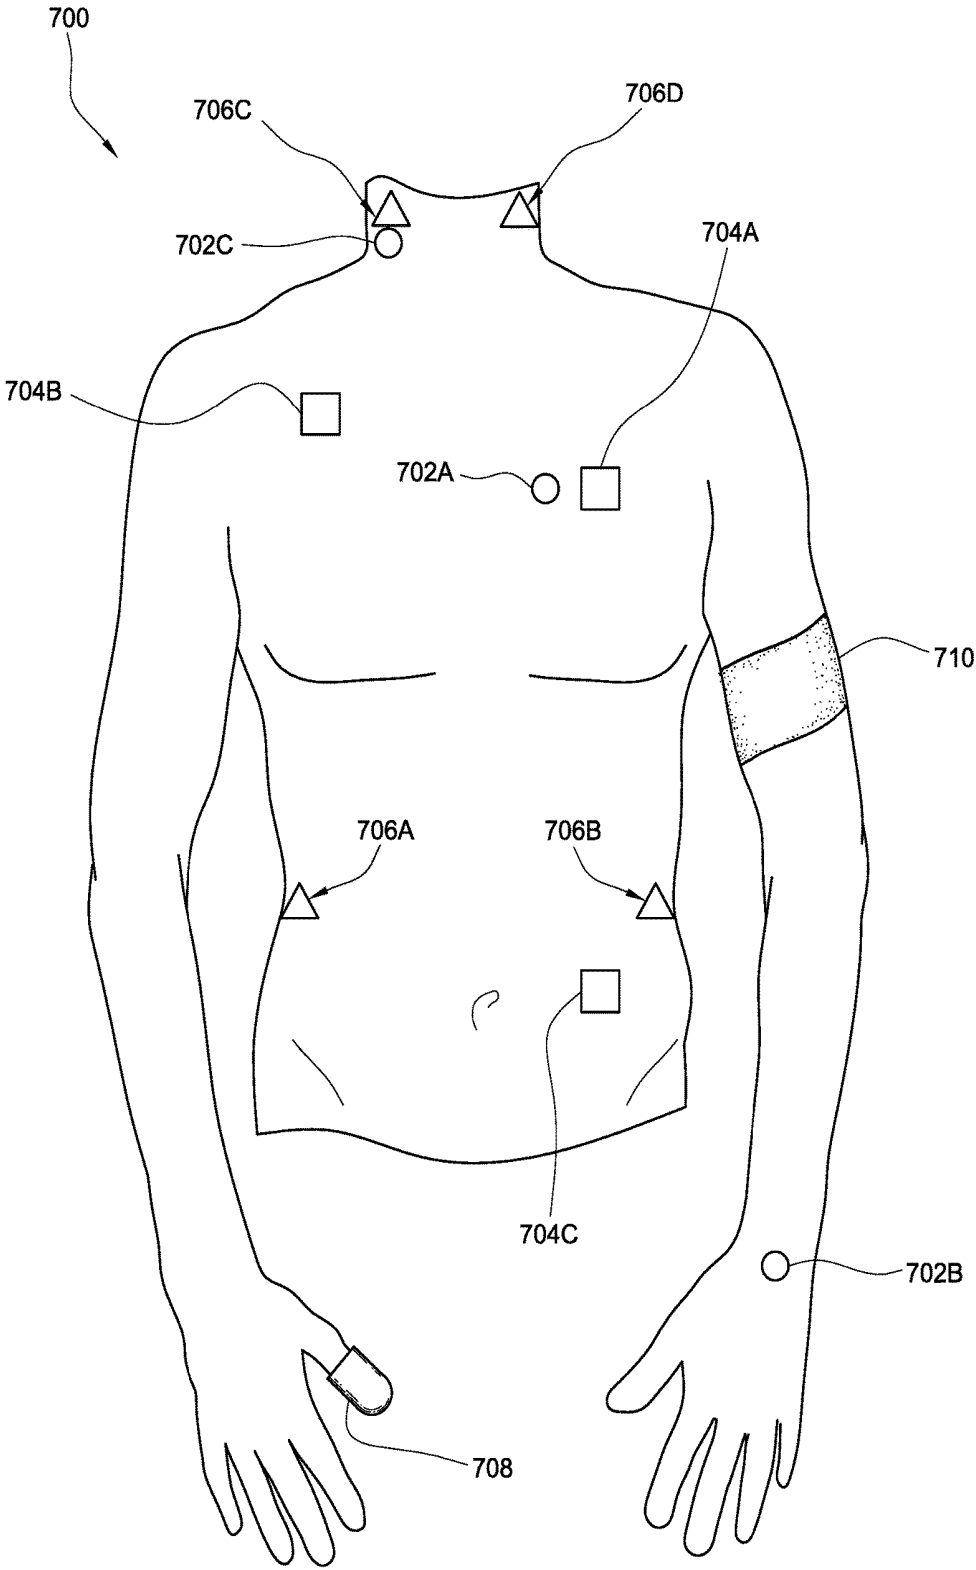
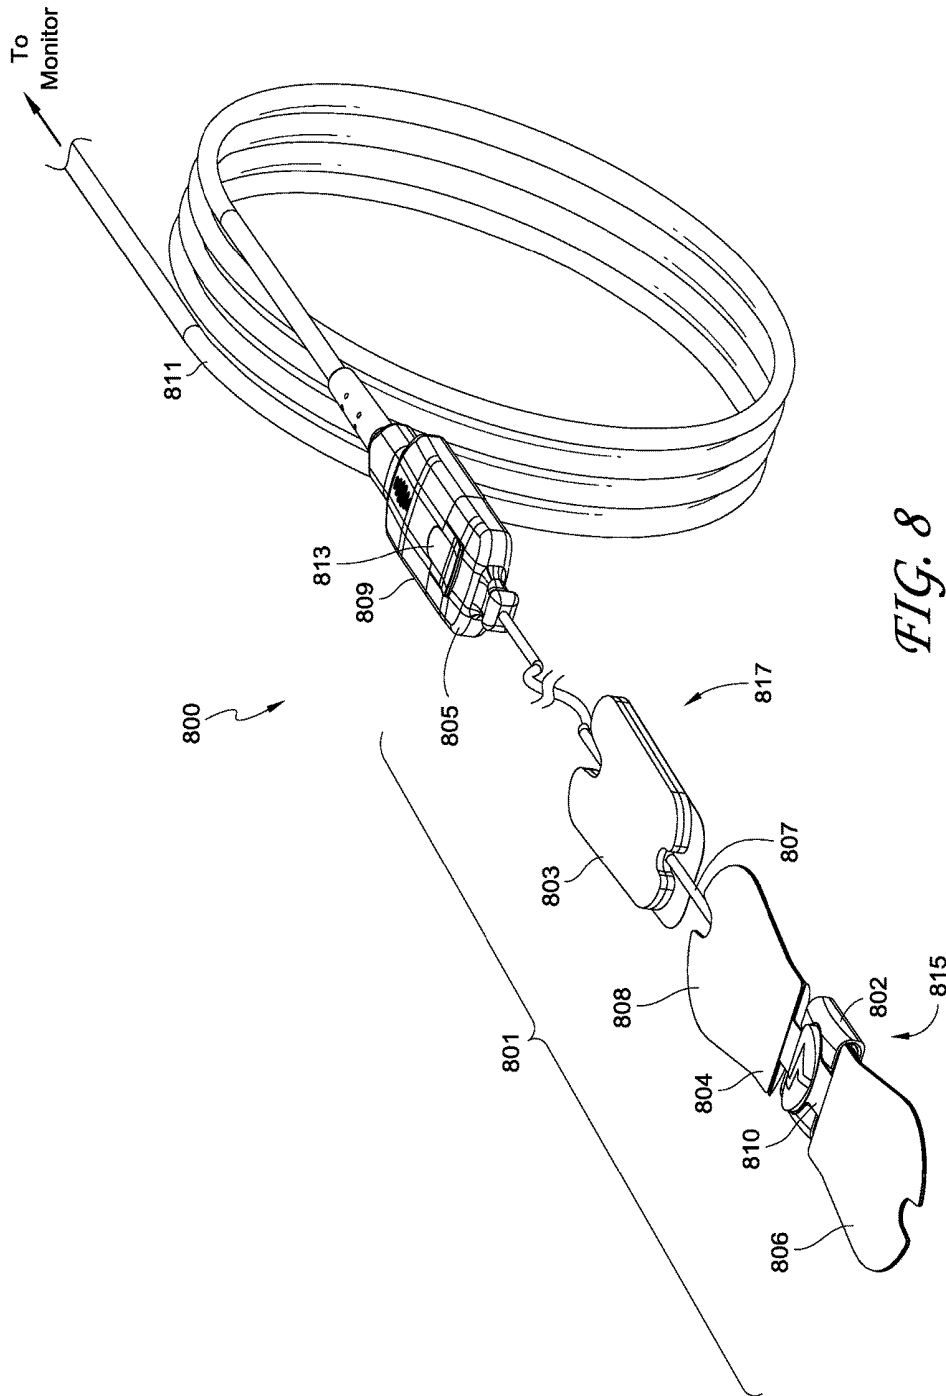


FIG. 7



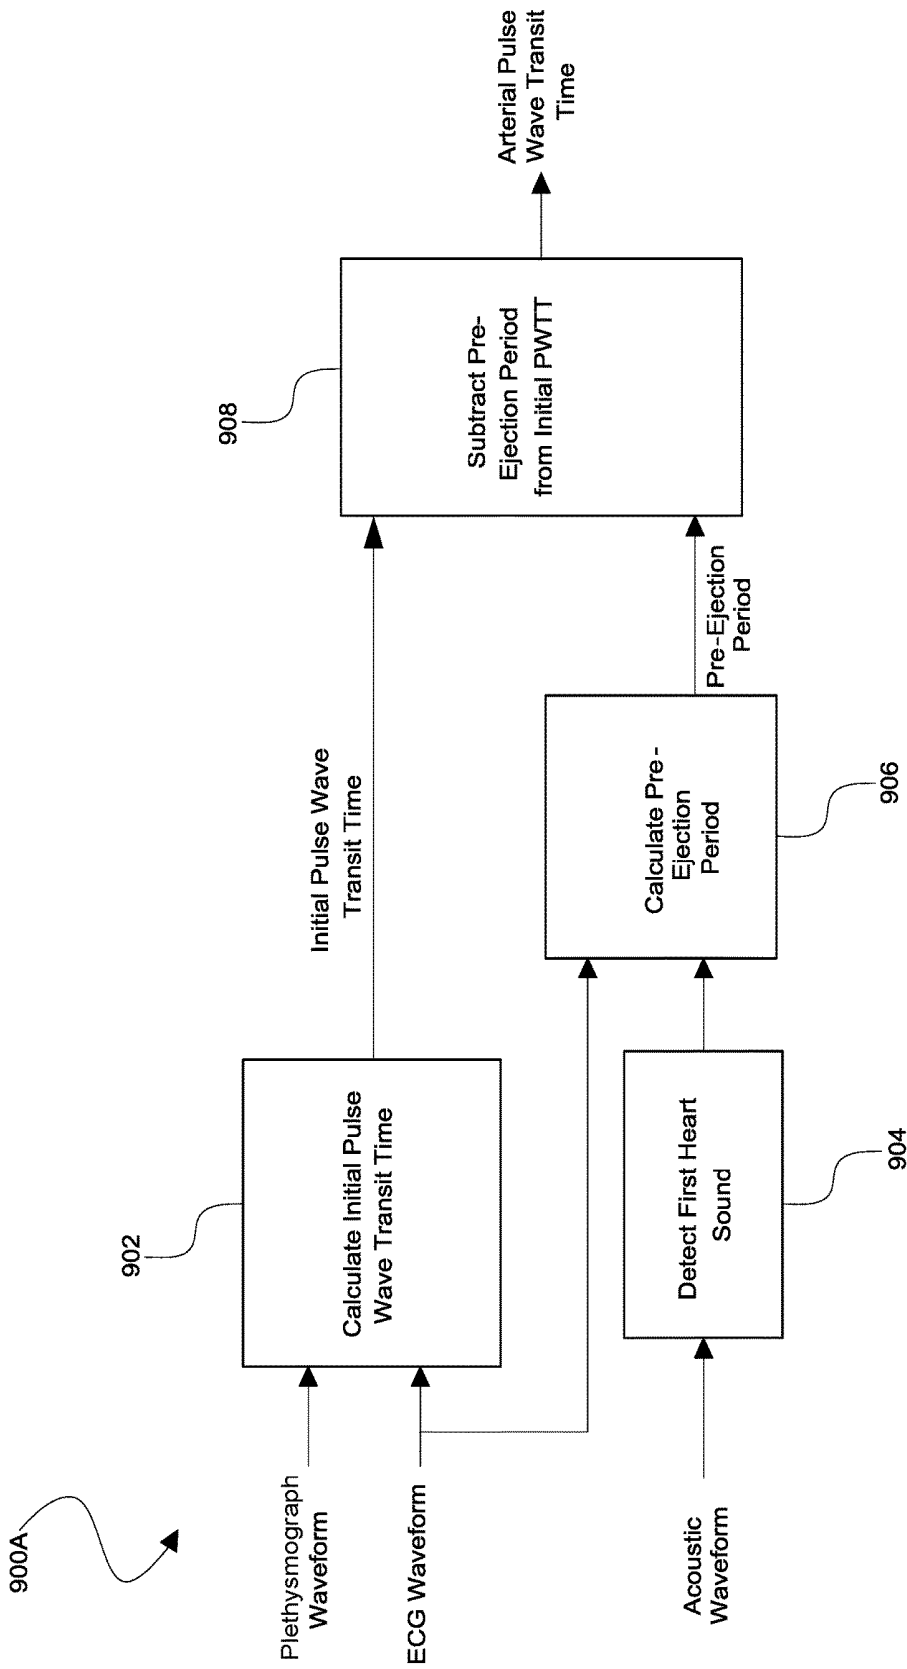


FIG. 9A

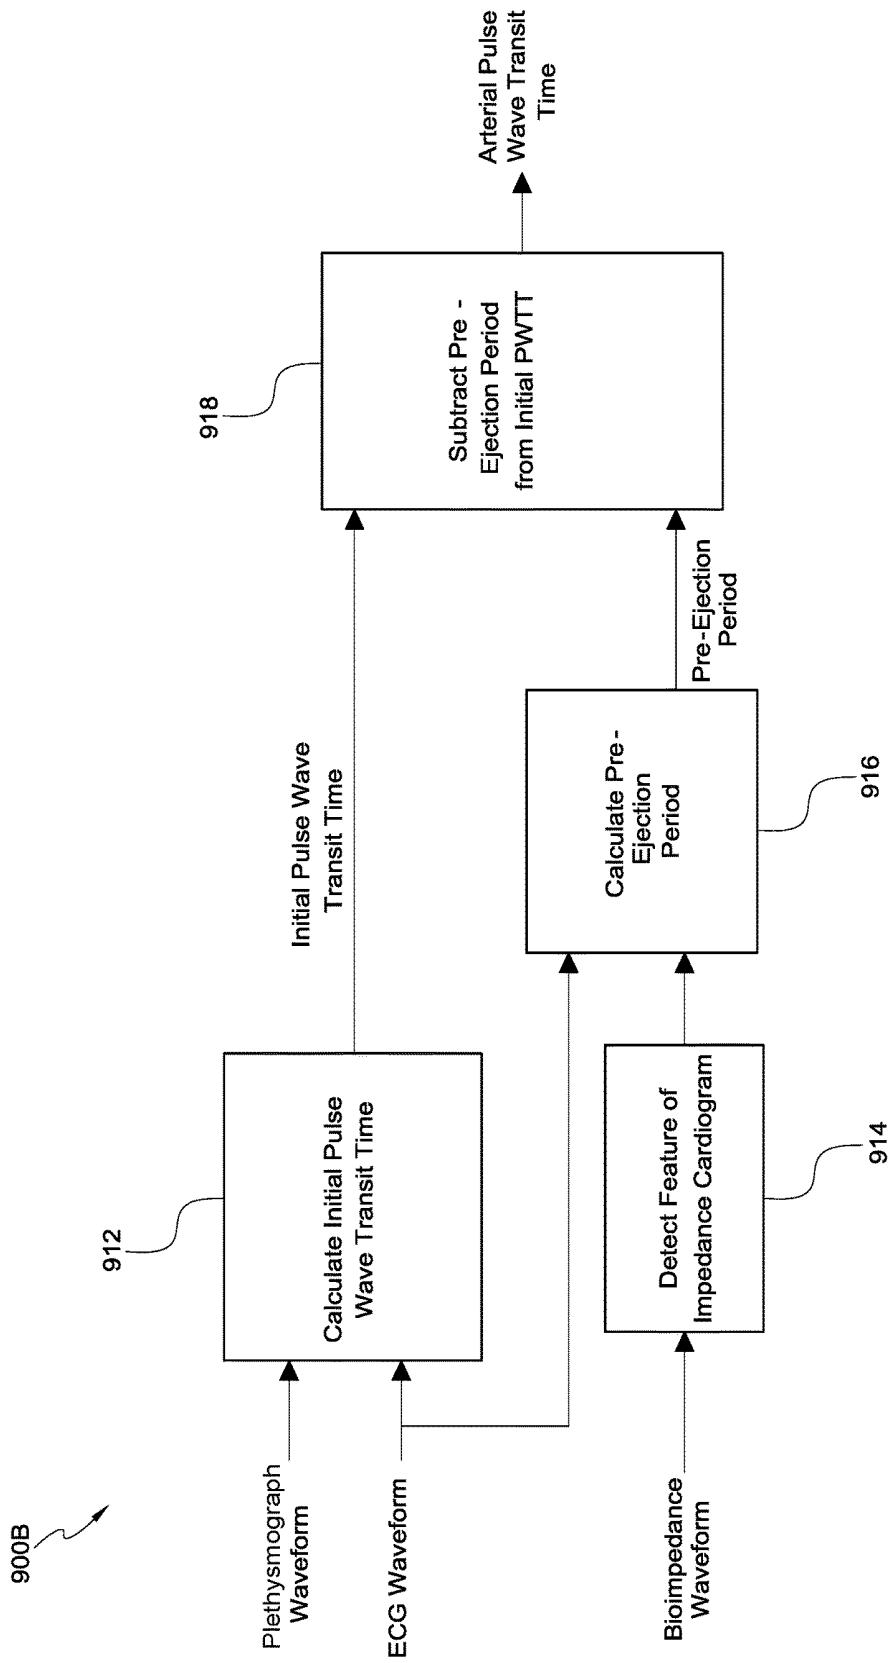


FIG. 9B

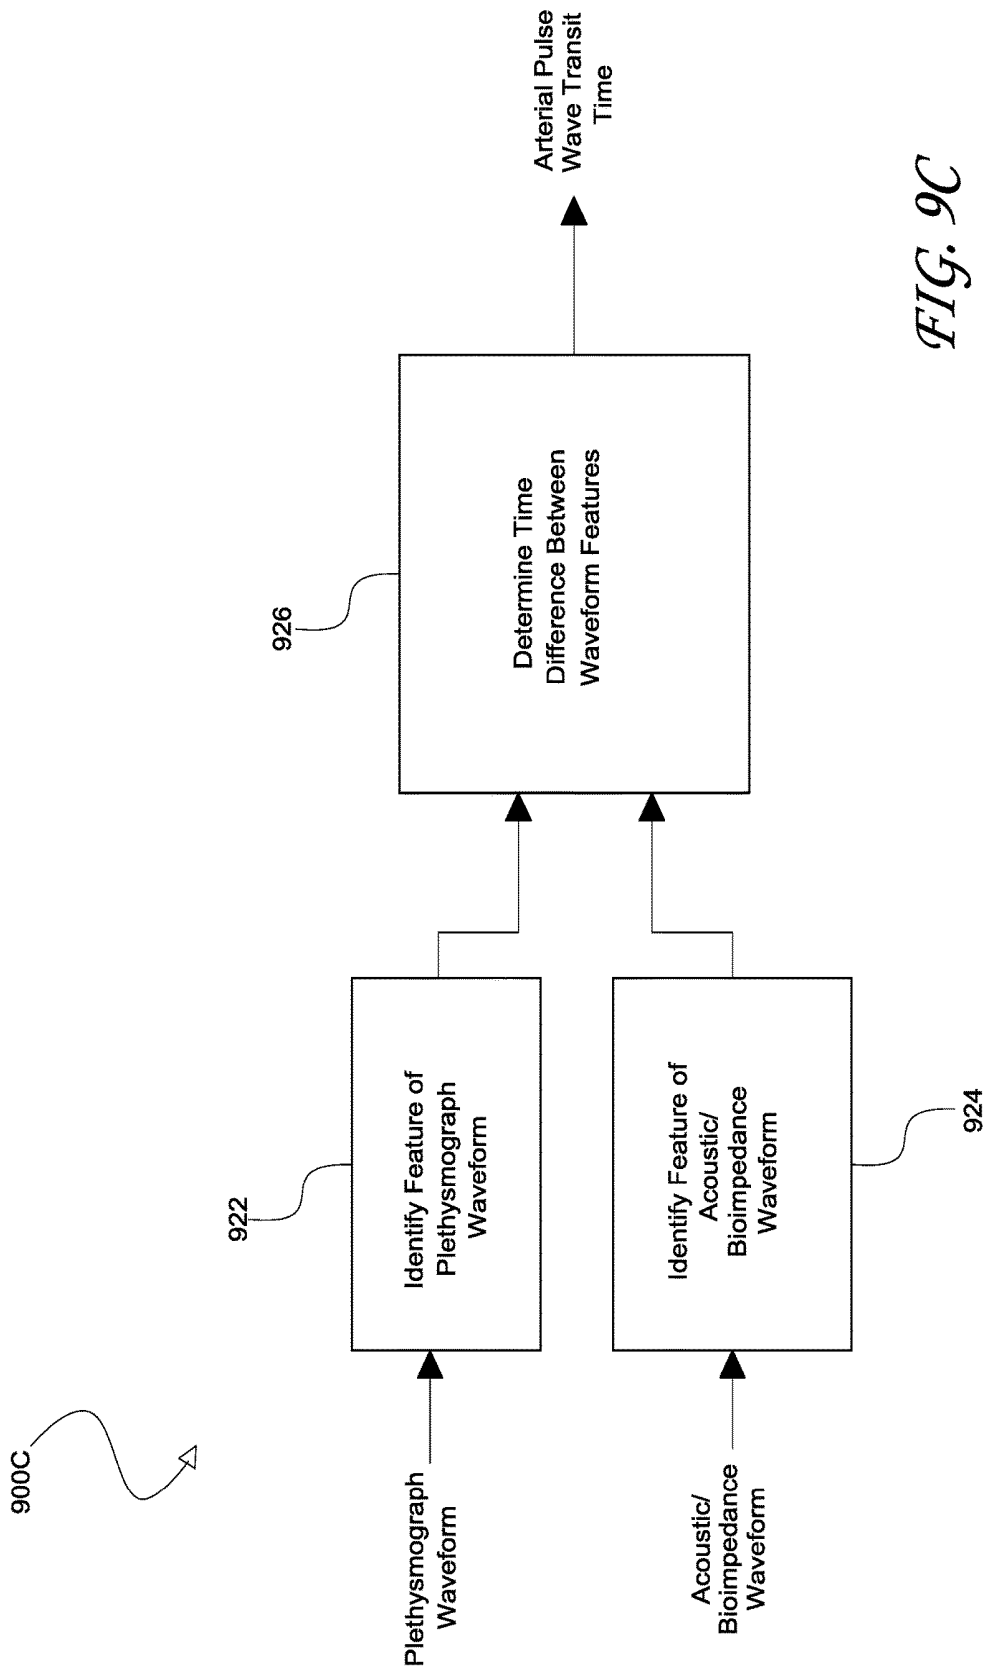


FIG. 9C

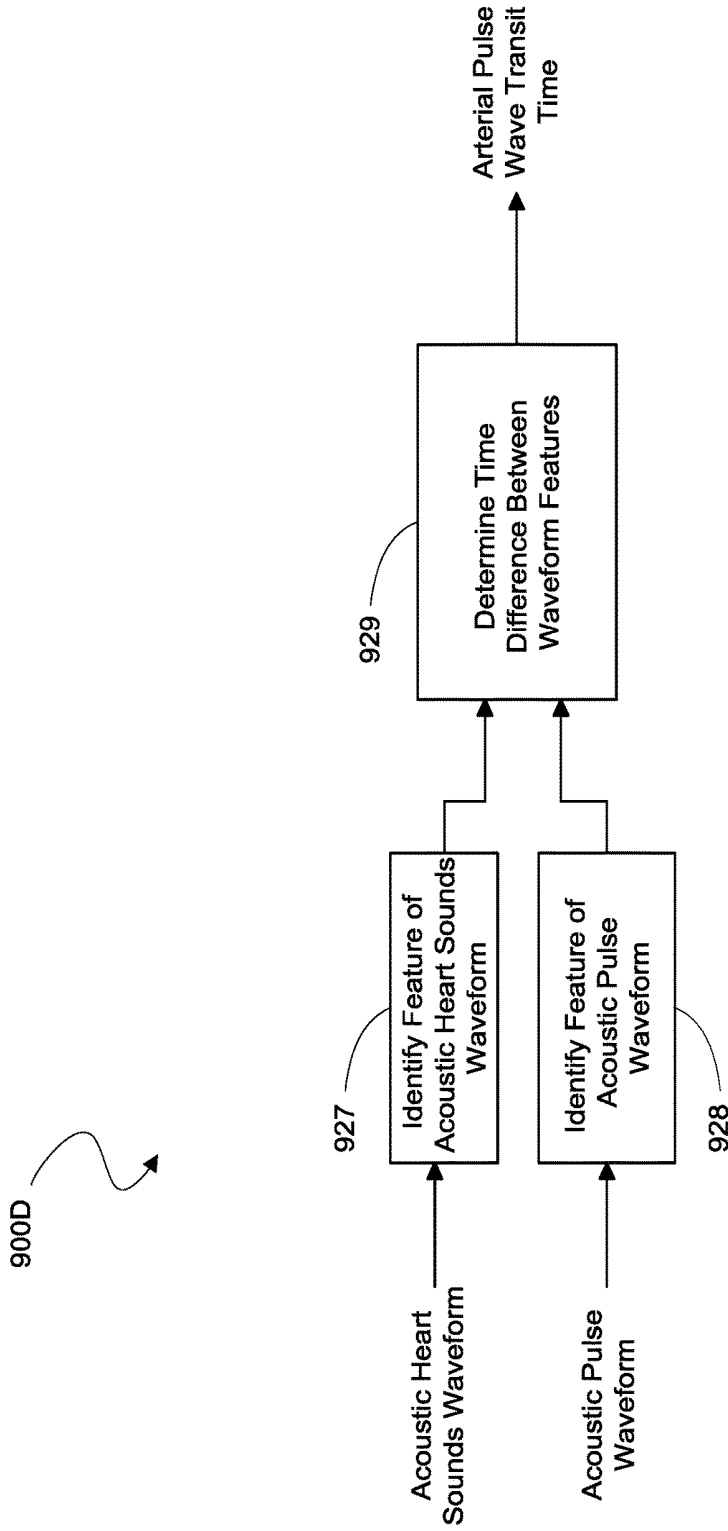


FIG. 9D

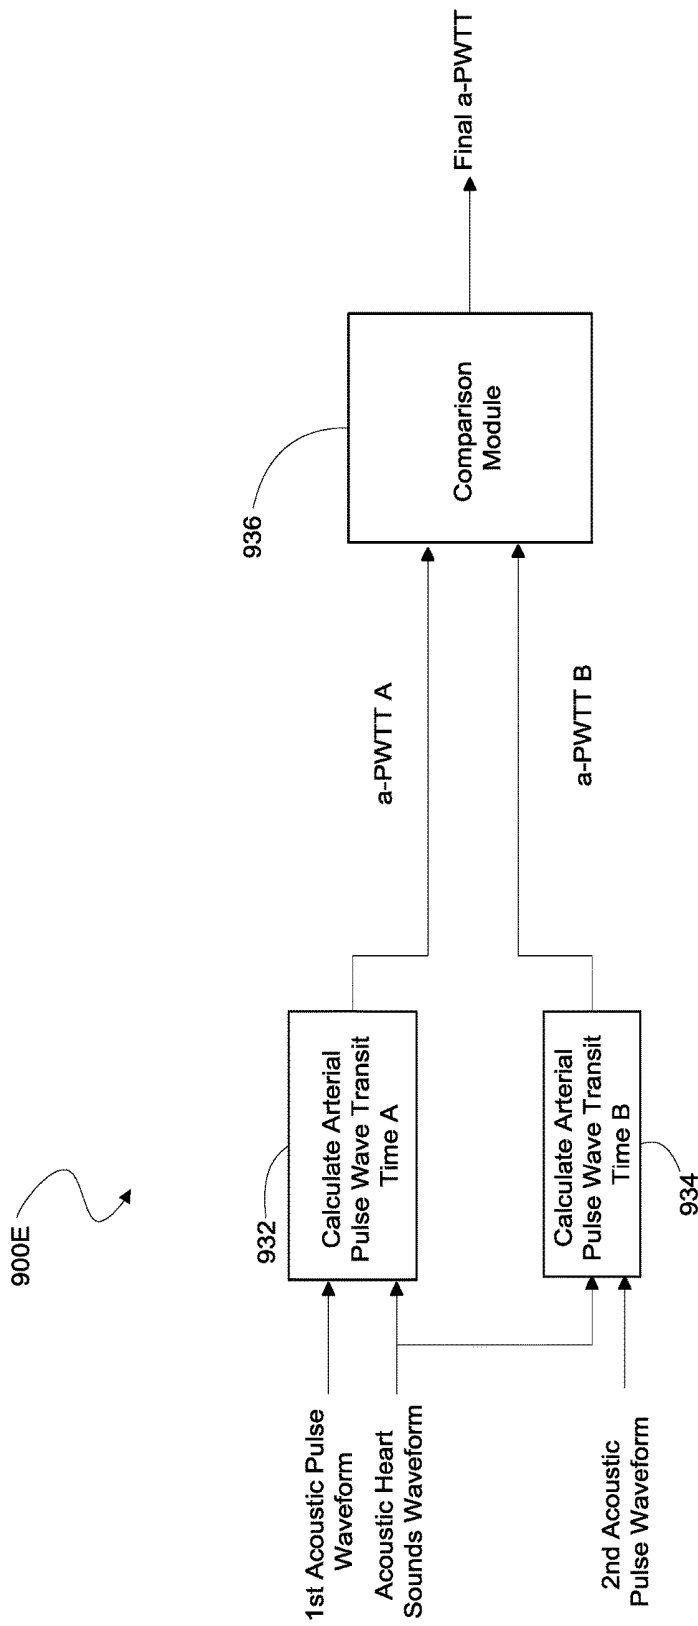


FIG. 9E

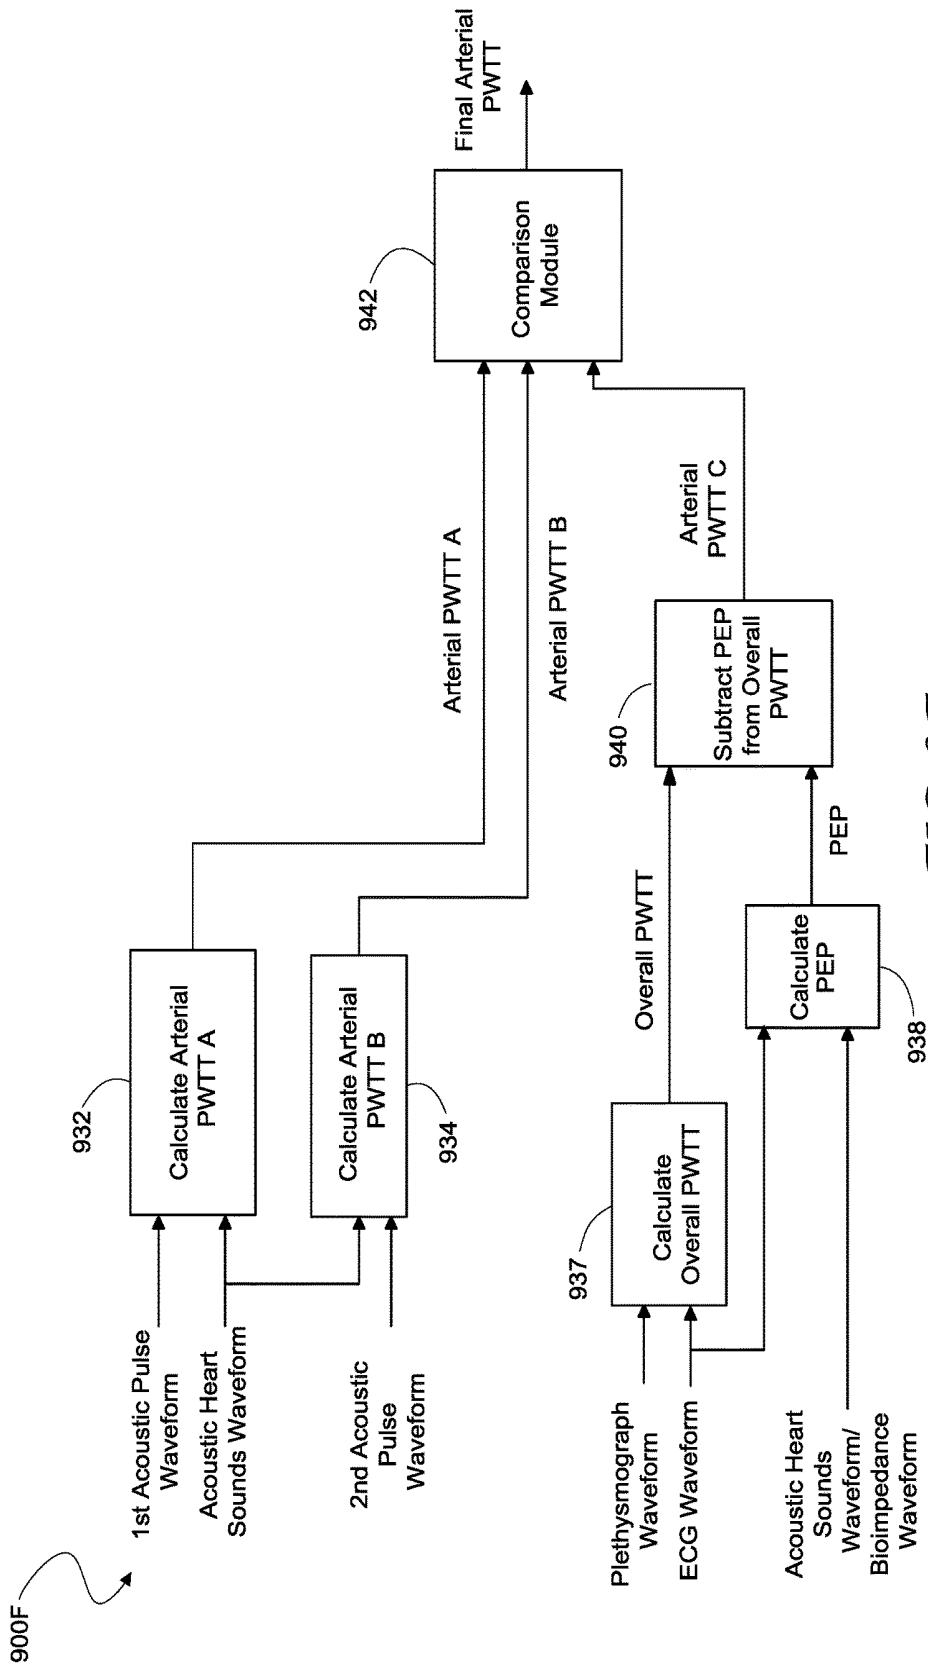


FIG. 9F

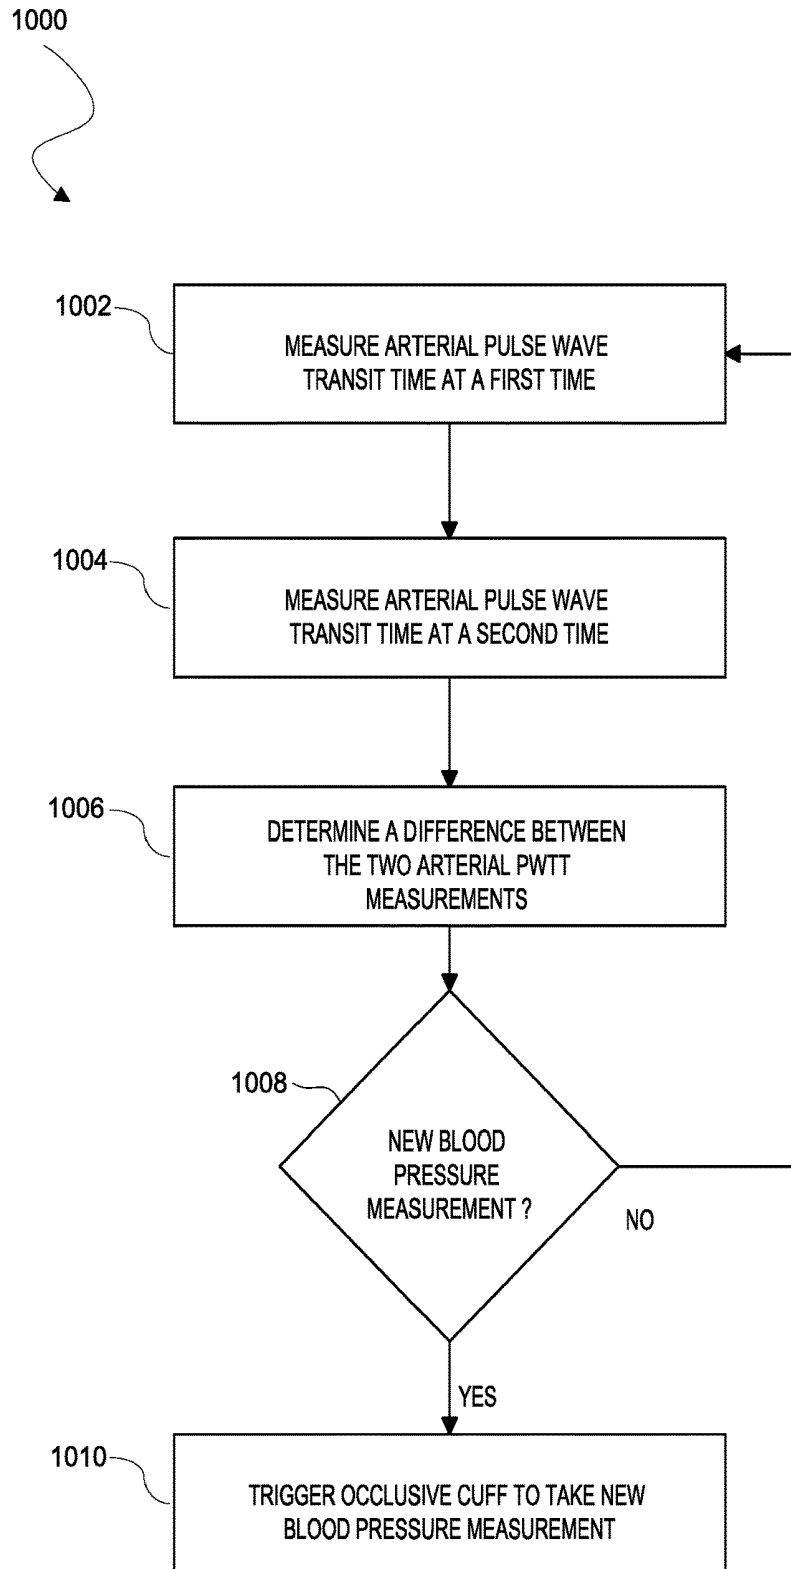


FIG. 10

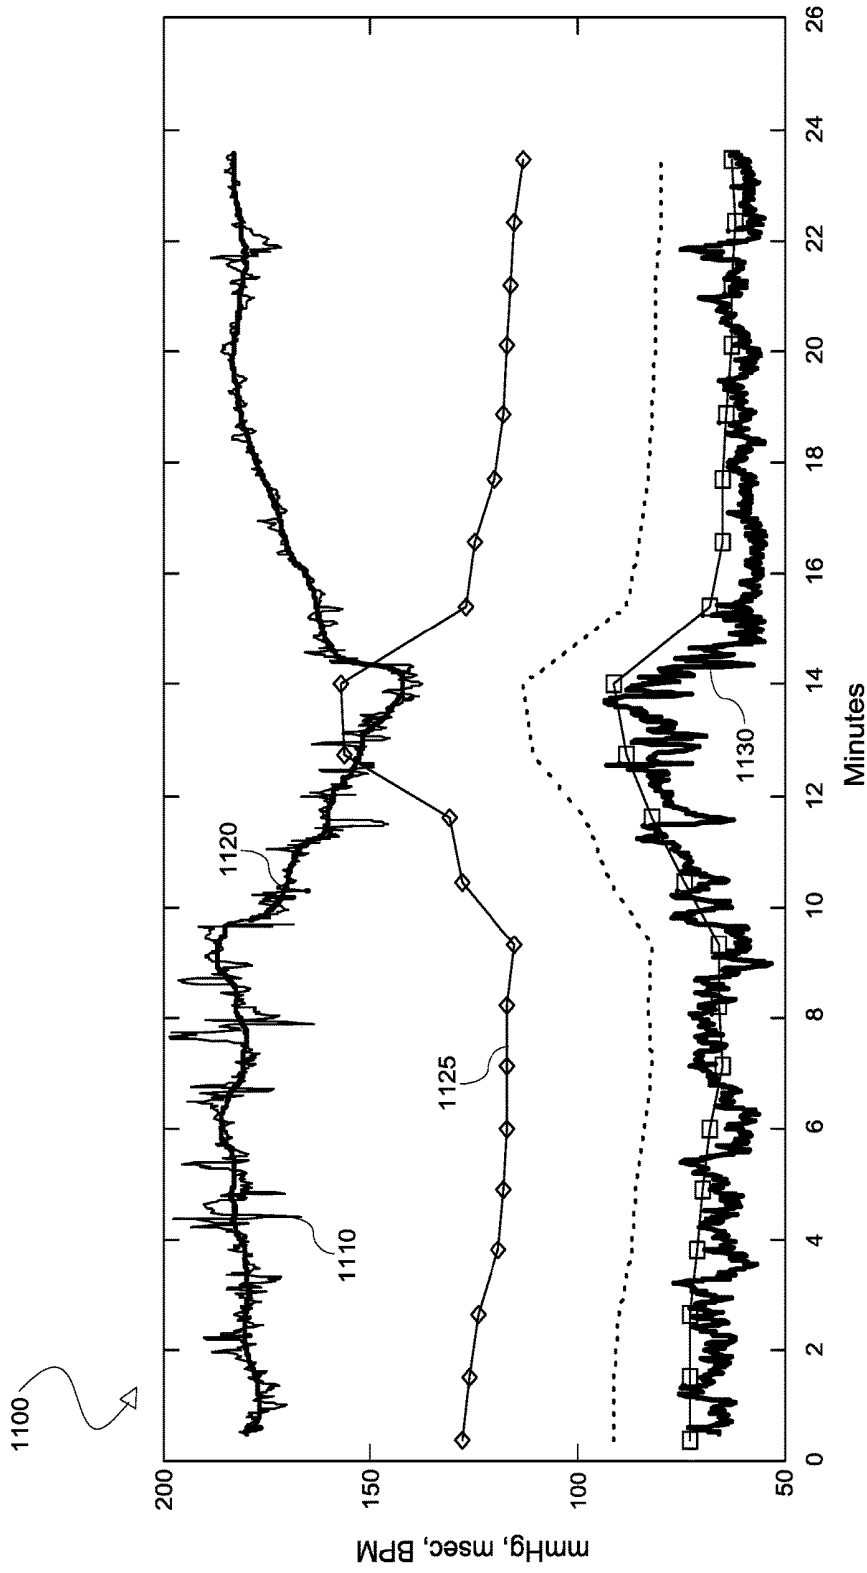


FIG. 11

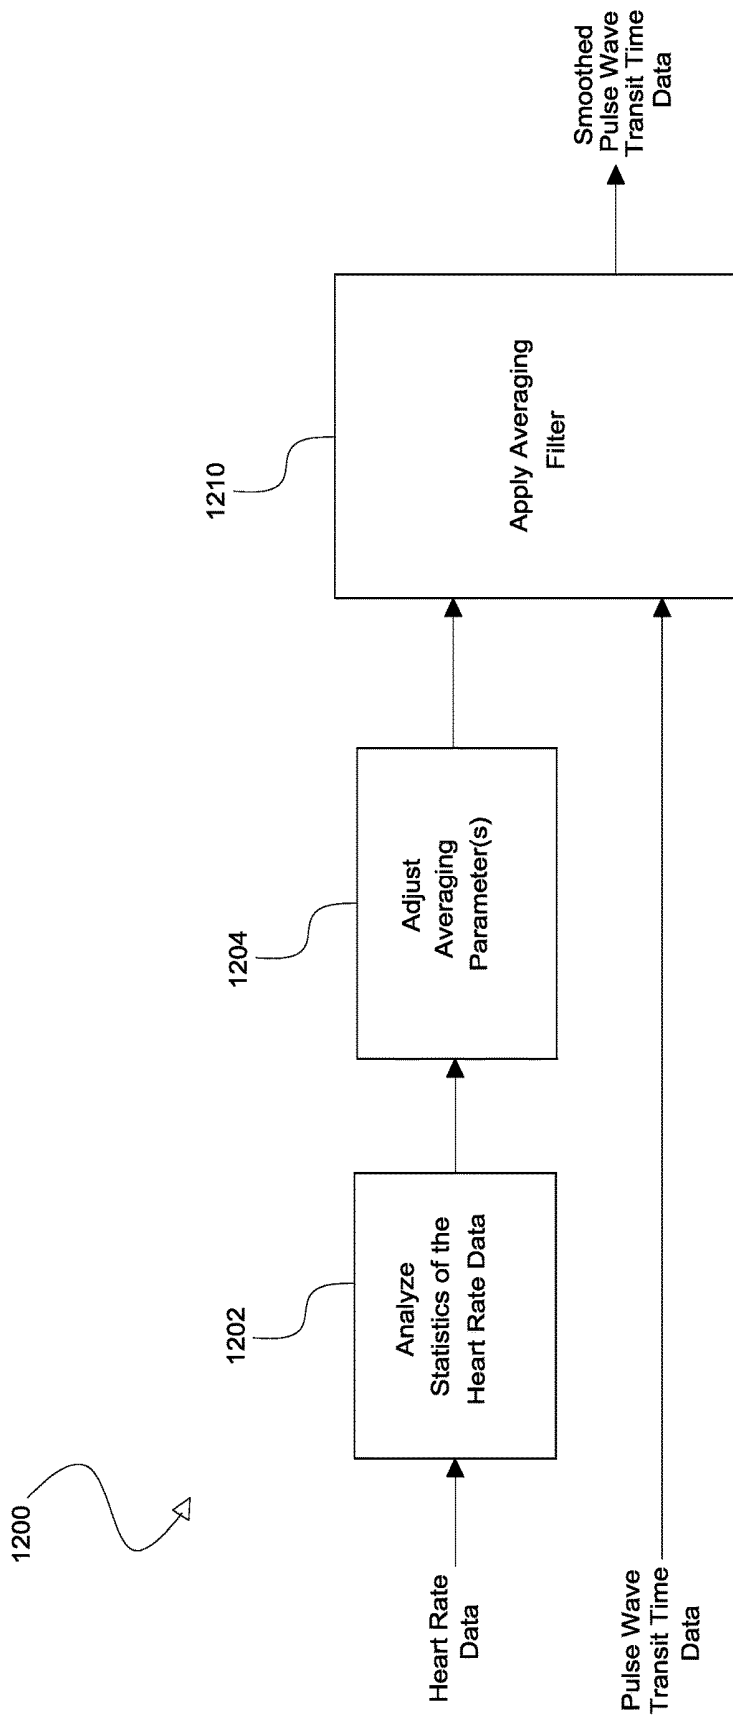


FIG. 12

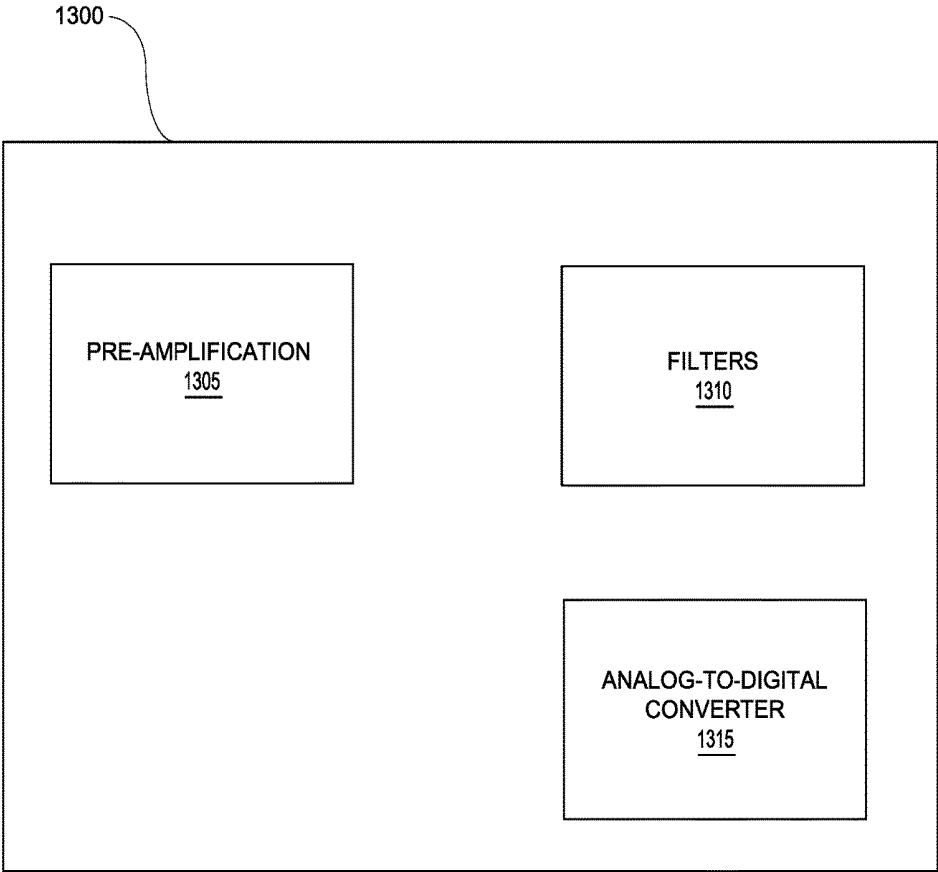


FIG. 13

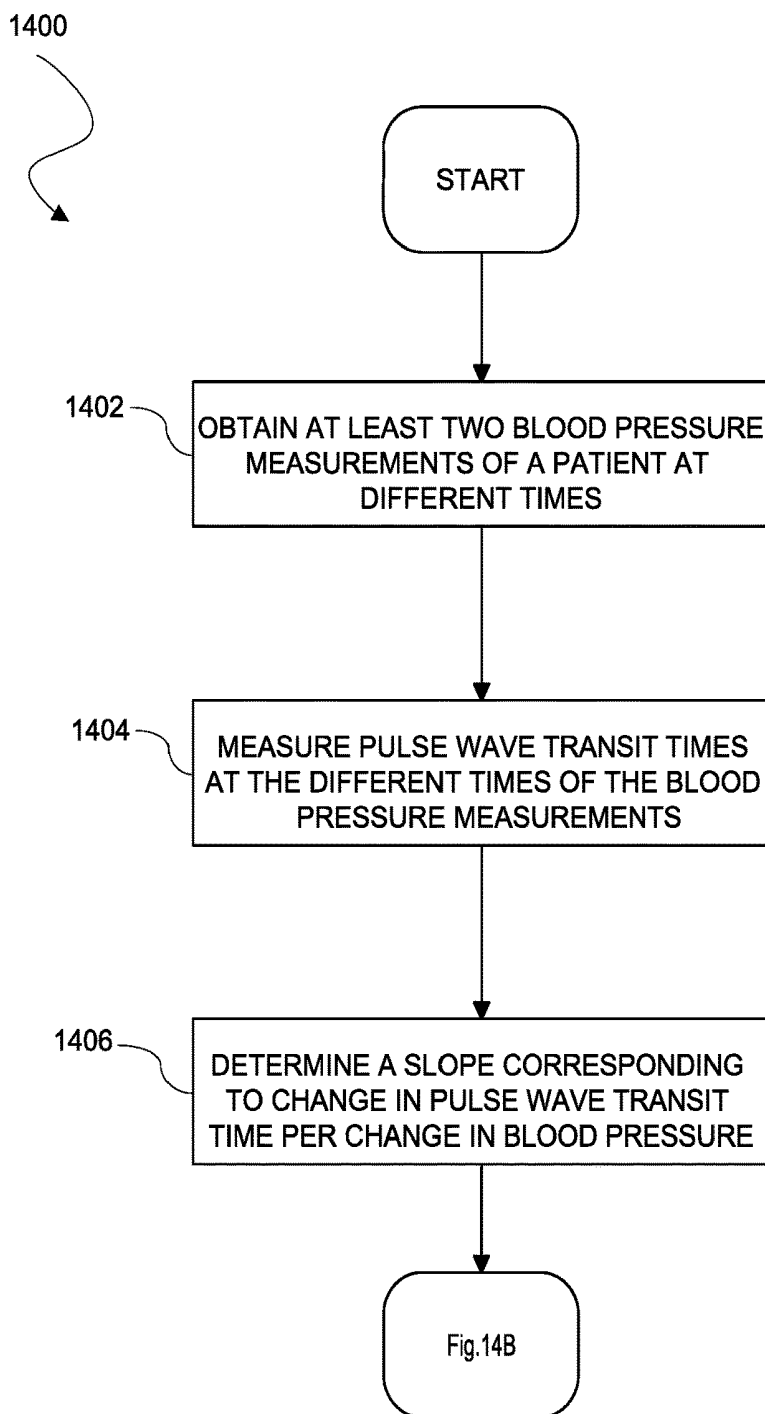


FIG. 14A

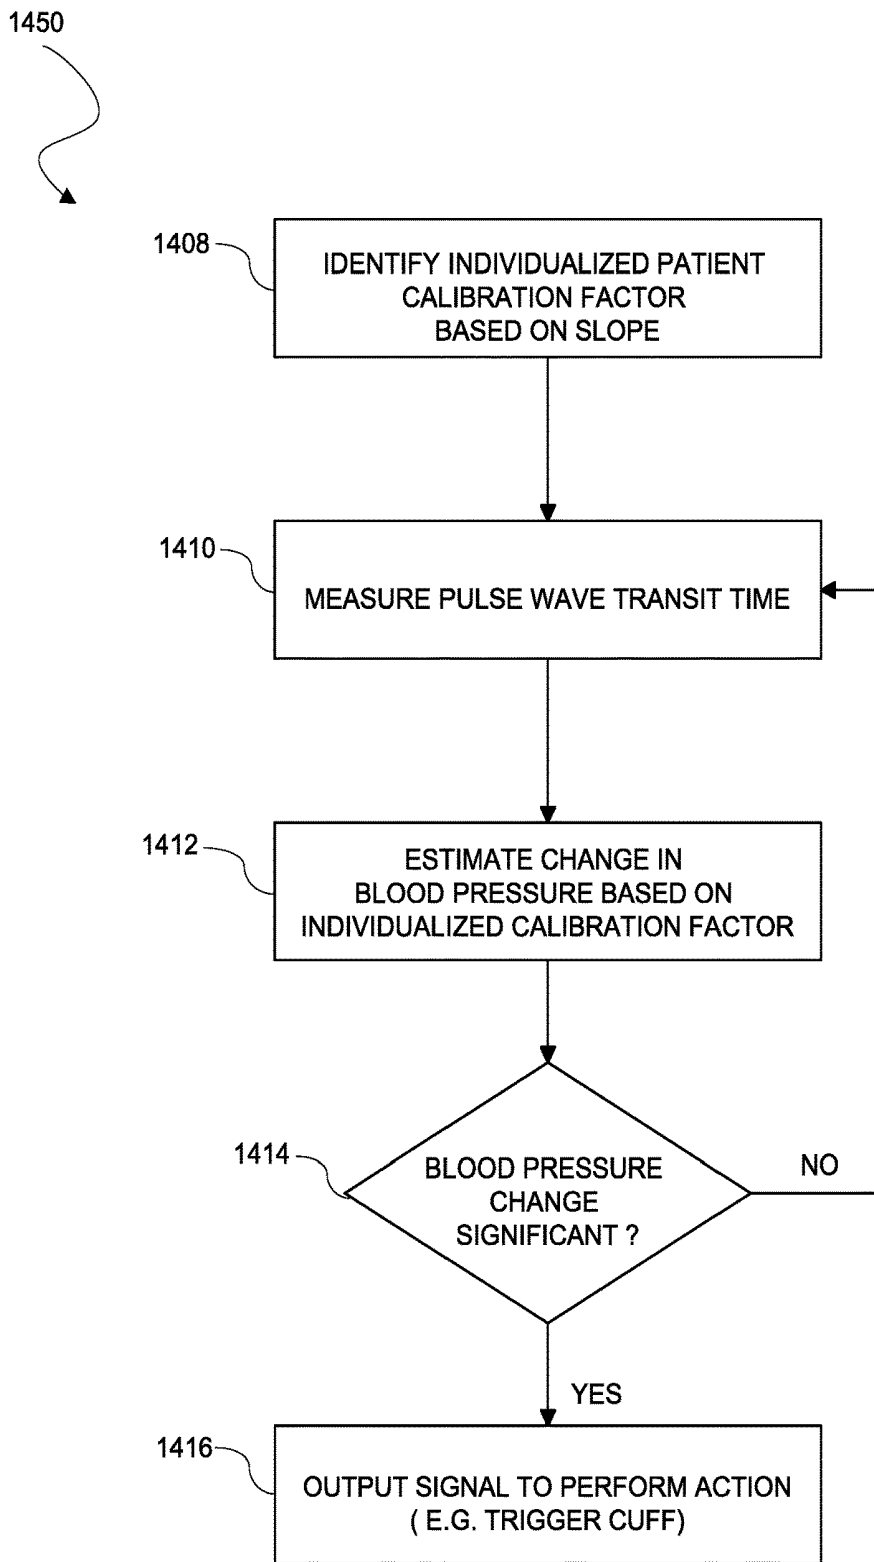


FIG. 14B

NON-INVASIVE BLOOD PRESSURE MEASUREMENT SYSTEM

RELATED APPLICATIONS

This application is a continuation of U.S. patent application Ser. No. 13/189,396, filed Jul. 22, 2011, entitled "Non-Invasive Blood Pressure Measurement System," which claims priority under 35 U.S.C. § 119(e) to U.S. Provisional Application No. 61/366,862, filed Jul. 22, 2010, entitled "System for Triggering a Non-Invasive Blood Pressure Device" and to U.S. Provisional Application No. 61/469,511, filed Mar. 30, 2011, entitled "Non-Invasive Blood Pressure Measurement System," the disclosures of which are hereby incorporated by reference in their entirety.

BACKGROUND

Prolonged reduction or loss of blood pressure in a patient severely limits the amount of tissue perfusion of the patient and therefore causes damage to or death of the tissue. Although some tissues can tolerate hypoperfusion for long periods of time, the brain, heart and kidneys are very sensitive to a reduction in blood flow. Thus, during and after medical procedures and at other times, blood pressure is a frequently monitored vital sign. Blood pressure can be affected by the type of medical procedure performed and by physiological factors such as the body's reaction to the medical procedure. Moreover, blood pressure is often manipulated and controlled using various medications. Medical procedures, physiological factors, and medications can cause the blood pressure of a patient to change rapidly.

The traditional method of measuring blood pressure is with a stethoscope, occlusive cuff, and pressure manometer. Blood pressure cuff instruments make only a spot-check measurement, so repetitive interval measurements are often used to trend patient status. More frequent intervals improve vigilance at the expense of patient discomfort, possible patient injury (e.g., due to occlusion of blood vessels), and excessive battery consumption.

SUMMARY

In certain embodiments, a method of monitoring blood pressure of a patient includes receiving a physiological electrical signal from an electrical sensor coupled with a patient. The physiological electrical signal can reflect electrical activity of the patient's heart. The method may also include receiving a cardiac ejection signal from a second sensor coupled with the patient. This cardiac ejection signal can reflect a cardiac ejection event associated with ejection of blood from the patient's heart. In addition, the method may include receiving an arterial pulse signal from a third sensor coupled with a limb of the patient. The method can also include determining an arterial pulse wave transit time (PWTT) that compensates for a pre-ejection period of a cardiac cycle associated with the patient's heart, based at least partly on the physiological electrical signal, the cardiac ejection signal, and the arterial pulse signal. Moreover, the method may include triggering an occlusive blood pressure cuff to obtain a blood pressure measurement from the patient responsive to a change in the arterial PWTT.

For purposes of summarizing the disclosure, certain aspects, advantages and novel features of the inventions have been described herein. It is to be understood that not necessarily all such advantages can be achieved in accordance with any particular embodiment of the inventions

disclosed herein. Thus, the inventions disclosed herein can be embodied or carried out in a manner that achieves or optimizes one advantage or group of advantages as taught herein without necessarily achieving other advantages as can be taught or suggested herein.

BRIEF DESCRIPTION OF THE DRAWINGS

Throughout the drawings, reference numbers can be re-used to indicate correspondence between referenced elements. The drawings are provided to illustrate embodiments of the inventions described herein and not to limit the scope thereof.

FIG. 1 illustrates an embodiment of a parameter calculation system;

FIGS. 2A and 2B illustrate plots of plethysmograph and electrocardiograph (ECG) waveforms that can be used to calculate pulse wave transit time (PWTT);

FIGS. 2C and 2D illustrate plots of acoustic waveforms that can be used to calculate PWTT;

FIG. 3 illustrates another embodiment of a blood pressure monitoring system;

FIG. 4A illustrates a plot of acoustic and ECG waveforms;

FIG. 4B illustrates a plot of bioimpedance and ECG waveforms;

FIGS. 5A and 5B illustrate embodiments of blood pressure monitoring systems coupled to a patient;

FIG. 6 illustrates example positioning locations for the acoustic sensors that can be used in the various systems and methods described herein;

FIG. 7 illustrates example positioning locations for acoustic, electrocardiograph (ECG), optical and bioimpedance sensors that can be used in the various systems and methods described herein;

FIG. 8 illustrates an example acoustic sensor that can be used in the various systems described herein;

FIGS. 9A through 9F illustrate embodiments of calculating arterial PWTT;

FIG. 10 illustrates an embodiment of a process for triggering an occlusive blood pressure measurement;

FIG. 11 illustrates plots of PWTT and heart rate waveforms;

FIG. 12 illustrates an embodiment of a dynamic PWTT averaging system;

FIG. 13 illustrates an embodiment of front end circuitry that can be used in the parameter calculation systems described herein to reduce phase impact on the calculations of PWTT;

FIGS. 14A and 14B illustrate an embodiment of a process for calibrating PWTT measurements based on an individualized patient calibration factor.

DETAILED DESCRIPTION

The propagation time of an arterial pulse wave from the heart to an extremity is related to blood pressure. Currently available blood pressure monitoring systems estimate this propagation time by detecting a time difference between points on an electrocardiograph (ECG) waveform and a photoplethysmograph waveform. This estimated propagation time is sometimes referred to as pulse wave transit time (PWTT) or time difference of arrival (TDOA). Currently available blood pressure monitoring systems trigger an automatic occlusive cuff to take a blood pressure measurement based on detected changes in PWTT. When the PWTT has not changed substantially, the blood pressure monitoring system usually does not trigger an occlusive blood pressure

measurement. As a result, such a system automatically adjusts the frequency of occlusive blood pressure measurements to obtain better data while potentially reducing discomfort for the patient.

A drawback with existing blood pressure systems is that PWTT as calculated by these systems is not always an accurate indicator of blood pressure or changes in blood pressure. One reason for this inaccuracy is that currently-available systems do not account for a patient's pre-ejection period (PEP) when computing PWTT. The PEP can include the difference in time between an electrical trigger that initiates ventricular contraction (e.g., as detected by an ECG sensor) and the actual ejection of blood from the ventricles into the aorta. Accordingly, the calculated PWTT does not accurately represent the actual propagation time of the arterial pulse from the heart to an extremity, which can result in inaccuracy in the blood pressure variability measurements.

Another reason for the inaccuracy of existing blood pressure systems is that the photoplethysmograph waveform is typically obtained from an optical sensor coupled to a finger of the patient. Studies have shown that pulse wave velocity slows greatly at the transition from the arteries to the smaller vessels and capillaries, adding considerable delay to the arterial PWTT. This time delay can account for up to 50% of the arterial PWTT. The use of an acoustic sensor positioned over an artery to monitor arterial pulse instead of capillary flow can advantageously remove the effect of the artery-to-capillary transition delay component of the arterial pulse wave transit time measurements.

This disclosure describes, among other features, a system for non-invasively determining an indication of an individual's blood pressure. In certain embodiments, the system dynamically accounts for a patient's PEP when calculating PWTT. The system can include an optical sensor that obtains plethysmograph information from a patient. The system can further include an electrical sensor, which can be any sensor that obtains information relating to the electrical activity of the patient's heart (such as an ECG sensor). In addition, the system can include another sensor, such as an acoustic sensor or a bioimpedance sensor, which can obtain information about cardiac ejections from the patient's heart. In certain embodiments, the system further includes a processor that calculates PWTT compensated for PEP using the information obtained from the optical, electrical, acoustic, and/or bioimpedance sensors. The system can use this compensated PWTT to determine whether to trigger an occlusive cuff measurement.

In some embodiments, the system determines an arterial pulse wave transit time measurement from features of two acoustic waveforms. The system can include an acoustic heart sounds sensor that obtains heart sound information from a patient. The system can further include an acoustic pulse sensor, which can be placed at a location remote from the patient's heart at which peripheral arterial pulse pressure wave vibrations can be monitored (such as at a patient's wrist or neck). In addition, the system can include one or more other sensors, such as a second acoustic pulse sensor, ECG sensors, optical sensors, and/or bioimpedance sensors. In certain embodiments, the system further includes a processor that calculates arterial PWTT using the information obtained from the acoustic and/or other sensors. The system can use the arterial PWTT measurements to estimate changes in blood pressure and to aid in determining whether to trigger an occlusive cuff measurement.

In some embodiments, the system also compensates PWTT data for noise. For example, the system can use a

noise reference signal to reduce noise in the PWTT data. The noise reference signal can be derived from the patient's heart rate. The system can reduce noise in the PWTT, for example, by adaptively reducing the noise based on the noise reference signal or by dynamically adjusting an averaging time used to average the PWTT data, among other possible techniques.

Moreover, in certain embodiments, the non-invasive blood pressure measurement system also calibrates PWTT data based on an individualized patient calibration factor. A calibration function or curve can be determined that maps PWTT measurements to blood pressure values. The slope of the calibration curve can be determined experimentally and can vary greatly from patient to patient. In some embodiments, the system determines an individualized, or personalized, patient calibration factor based on the determined slope. The patient calibration factor can then be used to interpret subsequent PWTT measurements to estimate changes in blood pressure. The individualized patient calibration can advantageously reduce the occurrence of unnecessary blood pressure cuff measurements and/or false alarms.

System Overview

FIG. 1 illustrates an embodiment of a parameter calculation system **100**. In certain embodiments, the parameter calculation system **100** non-invasively obtains an indication of changes in a patient's blood pressure. The parameter calculation system **100** can use the measured blood pressure changes to trigger a blood pressure cuff **108** to obtain an occlusive blood pressure measurement. Advantageously, in certain embodiments, the parameter calculation system **100** uses the arterial pulse wave transit time, which accounts for a patient's pre-ejection period (PEP) when calculating changes in blood pressure. The parameter calculation system **100** can therefore more accurately determine when an occlusive blood pressure measurement is appropriate.

In the depicted embodiment, the parameter calculation system **100** includes a parameter calculator **110** and a display **120**. The parameter calculator **110** can include hardware (such as one or more processors), software, and/or firmware for measuring a physiological parameter such as blood pressure. Inputs to the parameter calculator **110** can include, among others, optical sensor data provided by an optical sensor **102**, acoustic sensor data provided by one or more acoustic sensors **104**, and/or additional sensor data provided by one or more additional sensors **106**. The optical sensor **102** can be a pulse oximetry sensor, a co-oximetry sensor, or the like. The acoustic sensors **104** can be biological sound sensors. The biological sounds may include heart, breathing, and/or digestive system sounds, in addition to many other physiological phenomena. The additional sensors **106** can include any sensing device that provides physiological data to the parameter calculator **110**. For example, the additional sensors **106** can include an electrical sensor configured to provide an ECG signal, an acoustic sensor, and/or a bioimpedance sensor, or any other sensing device.

The optical sensor **102** can use spectrophotometry techniques to measure a variety of blood constituents, including for example, oxygen saturation, hemoglobin, methemoglobin, carboxyhemoglobin, other hemoglobin species, concentrations of the same, and the like. In addition, the optical sensor **102** can also be used to measure a variety of other physiological parameters, including pulse rate, perfusion, and the like. The optical sensor **102** can include one or more emitters that shine one or more wavelengths of light through tissue of a living person, such as through a finger, toe, or

foot. One or more detectors can receive the transmitted light after attenuation by the tissue and can generate one or more signals responsive to the attenuated light.

In certain embodiments, the parameter calculator **110** derives a photoplethysmograph from the optical sensor data. The photoplethysmograph (sometimes referred to herein as a “plethysmograph,” “photopleth” or “pleth”) can be a waveform that can represent changes in blood volume as measured by one or more wavelengths of light irradiated at a tissue site of a patient. The photoplethysmograph can be caused by arterial pulsation, and as such, can be related to arterial blood pressure. Thus, in some embodiments, the parameter calculator **110** uses the optical sensor data to derive an indication of blood pressure for a patient.

In one embodiment, the parameter calculator **110** can use the optical sensor data and the additional sensor data **106** to derive one or more indications of blood pressure. For example, a combination of the optical sensor data and data from electrical sensor(s), acoustic sensor(s) **104**, and/or bioimpedance sensors(s) can be used to determine an amount of time that it takes for a pulse to travel through an artery from a patient’s heart to a measurement site. This time can be referred to as an arterial pulse-wave transit time (a-PWTT). Advantageously, in certain embodiments, the parameter calculator **110** can more accurately determine the a-PWTT based at least in part on the additional sensor data **106** obtained from an acoustic (**104**) and/or bioimpedance sensor. In particular, using the additional sensor data **106**, the parameter calculator **110** can account for a patient’s cardiac pre-ejection period (PEP) when calculating a-PWTT. In other embodiments, the parameter calculator **110** uses the acoustic sensor data derived from acoustic sensors **104** alone to derive one or more indications of blood pressure. Using the estimated changes in blood pressure, the parameter calculator **110** can trigger a blood pressure cuff **108** to obtain an occlusive blood pressure measurement.

The parameter calculator **110** can output parameter data **113** indicative of the calculated parameters, including blood pressure, for presentation to a user. The parameter data **113** can be displayed on a display device **120**. In another embodiment, the parameter calculator **110** provides parameter values as an output **112** to another device, for example, a device providing an audible response, or over a network to a remote device. For example, a remote device might be a computer located at a nurses’ station or a clinician’s handheld device.

The parameter calculator **110** can also calculate trend data reflecting trend information for the parameter data **113**. The parameter calculator **110** can also synthesize or scale waveform data. In addition to outputting the parameter data **113**, the parameter calculator **110** can output trend data **114**, synthesized, scaled, or actual waveforms **115**, calibration data **116**, and alarms **117**. The parameter calculator **110** can provide the outputs **113**, **114**, **115**, **116** to the display **120**, to a separate patient monitoring device, or to another device configured to receive physiological parameter information.

In an embodiment, the parameter calculator **110** is implemented in a single monitoring device. In an embodiment, the features of the parameter calculator **110** are distributed among separate devices. In an embodiment, the parameter calculator **110** includes a processor, processor board, or an Original Equipment Manufacture (OEM) board. In an embodiment, the parameter calculator **110** is portable. Data communicated between the various components of the parameter calculation system **100** can be communicated through cables or wirelessly. Other inputs and/or outputs can be included with the system **100**.

The display **120** of the parameter calculation system **100** can be part of a patient monitor (not shown), which can also include other components, such as a speaker, power button, removable storage or memory (e.g., a flash card slot), an AC power port, and one or more network interfaces, such as a universal serial bus interface or an Ethernet port. The display **120** can indicate a measurement for blood pressure, for example, a measurement of the systolic and diastolic blood pressure in mmHg. Other physiological parameter values, waveforms, trend data, calibration data, alarms, and the like can also be output on the display **120**.

Although the parameter calculator **110** is described as calculating changes in blood pressure, in some embodiments, the parameter calculator **110** calculates actual blood pressure values from the acoustic and/or additional sensor data. In addition, the parameter calculation system **100** can also measure other physiological parameters besides blood pressure, such as pulse rate, oxygen saturation (SpO₂), hemoglobin, total hemoglobin, hemoglobin species (e.g., methemoglobin, carboxyhemoglobin, or the like), carbon monoxide or dioxide, perfusion, and glucose, among a variety of other parameters.

Further, in some embodiments, the parameter calculator **110** uses acoustic sensor data (from the acoustic sensor(s) **104**) to determine any of a variety of respiratory parameters of a patient, including respiratory rate, inspiratory time, expiratory time, inspiratory to expiratory (I:E) ratio, inspiratory flow, expiratory flow, tidal volume, minute volume, apnea duration, hypopnea duration, breath sounds (e.g., rales, rhonchi, and stridor), and changes in breath sounds such as decreased volume or change in airflow (either increase or decrease). In addition, in some cases the parameter calculator **110** monitors other physiological sounds from the acoustic sensor **104** data, such as heart rate (e.g., to help with probe off detection), heart sounds (S1, S2, S3, S4, and murmurs), and change in heart sounds such as normal to murmur or split heart sounds indicating fluid overload. Moreover, a second acoustic sensor **104** may be placed over the chest for better heart sound detection. The parameter calculator **110** may keep user inputs to a minimum (example, height) and use a Health Level 7 (HL7) interface to automatically input patient demography.

Example PWTT Calculations

FIG. 2A depicts an embodiment of a plot **200A** that illustrates an example PWTT calculation. In the plot **200A**, a plethysmograph waveform **210** and an ECG waveform **220** are shown. The plethysmograph waveform **210** can be obtained from an optical sensor **102** as described above. The ECG waveform **220** can be obtained from an electrical sensor.

The plethysmograph waveform **210** can reflect changes in pulsatile flow of blood in body tissue of a patient. The ECG waveform **220** can reflect electrical activity of a patient’s heart. The ECG waveform **220** can have features including, for example, a Q-wave, an R-wave peak, and an S-wave, among others. A segment of the ECG waveform **220** from the Q point to the S point can be referred to as a QRS complex, which can represent ventricular activation.

Velocity of a blood pressure wave in the arteries has a correlation with blood pressure. As the length of an artery is typically constant or approximately constant, the time that it takes for the blood pressure wave to travel from the heart to an extremity can be used to derive an indication of blood pressure. In currently available monitoring systems, a measure of such time, referred to as PWTT, has been used to infer changes in blood pressure. In some embodiments, the PWTT can represent a difference in time between a feature

of the plethysmograph waveform **210** and a feature of the ECG waveform **220**. For example, in one embodiment, the PWTT can be obtained from the difference in time between the R-wave peak on the ECG waveform **220** and a foot point on the plethysmograph waveform **210**. The foot point of the plethysmograph waveform **210** can correspond to the time of earliest onset of arrival of the pulse at a location away from the heart (e.g., at a patient's finger). In other embodiments, the PWTT can be obtained from the difference in time between either the Q-wave or the S-wave on the ECG waveform **220** and a feature on the plethysmograph waveform **210** (e.g., a foot point, peak, or some other feature).

Calculated in this manner from the plethysmograph and ECG waveforms **210**, **220**, PWTT can be fairly accurate for some patients. However, in some cases, using PWTT to measure changes in blood pressure provides inaccurate or unexpected results. At least a partial explanation of these unexpected results can be seen in FIG. **2B**.

In FIG. **2B**, an example plot **200** is shown that includes a plethysmograph waveform **210** and an ECG waveform **220**. An overall PWTT **212** can be calculated from a point on the ECG waveform **220** to a point of the plethysmograph waveform **210**, as described above. However, the overall PWTT **212** can actually include at least two components— an arterial pulse wave transit time (sometimes referred to as “a-PWTT”) **214** and a pre-ejection period (PEP) **216**.

The PEP **216** can be defined in different ways. For instance, in certain embodiments, the PEP **216** includes the difference in time between ventricular contraction and cardiac ejection of blood into the aorta. The PEP **216** can also be considered as a measured interval from the onset of ventricular depolarization, such as a Q-wave (or other feature) of an ECG, to the beginning of mechanical contraction of the heart muscle. For example, the PEP **216** can represent the difference in time from the onset of the QRS complex of the ECG signal **220** to when cardiac ejection actually occurs. Further, the PEP **216** can also be considered as the time interval from the beginning of the electrical activation of the ventricles to the opening of the aortic valve.

The value of the PEP **216** can fluctuate based on patient condition, age, sex, and medications taken by the patient, among possibly other factors. In some patients, the PEP **216** can account for a significant portion of the PWTT **212**, including even as much as about 50% of the PWTT **212**. Because PEP **216** can account for a significant portion of overall PWTT **212**, including the PEP **216** in a PWTT measurement can result in inaccurate determinations of changes in a patient's blood pressure. In certain circumstances, this can even lead to not detecting a clinically significant change in blood pressure and not initiating an occlusive cuff measurement for confirmation. FIG. **2B** also illustrates that it can prove difficult to derive the PEP **216** from a feature of a plethysmograph signal and a feature of an ECG signal.

Thus, in certain embodiments, the arterial PWTT **214**, which accounts for the PEP **216**, can more accurately correlate with changes in a patient's blood pressure than the overall PWTT **212**. Thus, it can be advantageous to detect changes in the arterial PWTT **214** and to use these changes to trigger occlusive cuff measurements. The arterial PWTT **214** can be determined in some embodiments by calculating the PEP **216** and subtracting the PEP **216** value from the overall PWTT **212**.

The PEP **216** can be derived, at least in part, from another physiological signal. Such a physiological signal can be indicative of cardiac ejection. Example physiological signals can include, but are not limited to, bioimpedance signals and

acoustic signals. For example, in one embodiment, the PEP **216** can be derived from a feature of the ECG waveform **220** and a feature of another physiological signal. As another example, in another embodiment, the PEP **216** can be derived from a feature of the plethysmograph waveform **210** and a feature of another physiological signal. As yet another example, the PEP **216** can be accounted for by deriving arterial PWTT directly from a feature of an acoustic heart sound waveform and an acoustic waveform on an extremity, such as the hand, wrist, or limb.

FIG. **2C** depicts an embodiment of a plot **200C** that illustrates an example PWTT calculation that compensates for PEP using multiple acoustic sensors. In the plot **200C**, a first acoustic waveform **230** and a second acoustic waveform **240** are shown. The first acoustic waveform **230** can be obtained from a first acoustic sensor positioned proximate a heart of a patient to monitor heart sounds of the patient. The heart sounds can be indicative of the closing of heart valves: the atrioventricular valves (mitral valve and tricuspid valve) and the semilunar valves (aortic valve and pulmonary valve). The closing of the heart valves corresponds to ventricular systole and diastole. The second acoustic waveform **240** can be obtained from a second acoustic sensor positioned at an arterial location away from the heart and configured to monitor peripheral pulse pressure wave vibrations or sounds at the arterial location. For example, the second acoustic sensor can be positioned proximate a wrist artery (e.g., radial artery, ulnar artery), proximate a carotid artery on the neck of the patient, or proximate an artery of the leg.

The first acoustic waveform **230** can include heart sounds of the patient corresponding to the closing of heart valves at the transition between ventricular systole and diastole. For example, the heart sounds can include first heart sounds (e.g., S1 heart sounds) **232** corresponding to the closure of the atrioventricular valves at the time ventricular systole begins and ventricular diastole ends and second heart sounds (e.g., S2 heart sounds) **234** corresponding to the closure of the aortic valve and the pulmonary valve at the time ventricular systole ends and ventricular diastole begins. The occurrence of the S1 heart sound can identify the start time of ejection of blood from the heart and the occurrence of the S2 heart sound can mark the end time or approximate end time of ejection of blood from the heart. Accordingly, the actual ejection of blood from the ventricles may occur for patients at the first heart sound (e.g., at the start, peak, or end of the first heart sound), between the start of the first heart sound (the S1 sound) and the start of the second heart sound (the S2 sound), or at the second heart sound (e.g., start, peak, or end of the second heart sound).

The second acoustic waveform **240** can include an arterial pulse at a second location remote from the heart (e.g., at a patient's wrist or neck). The second acoustic waveform **240** shown in FIG. **2C** includes audio information of the peripheral arterial pulse at a patient's wrist, hand, or arm (or foot, ankle, or leg). For convenience, although the peripheral arterial pulse can be detected at a variety of locations on the body, the wrist will be used as an illustrative example for the remainder of this specification. The second acoustic waveform **240** may display a pressure wave received at the patient's wrist some time prior to actual arrival of the blood at the periphery.

In some embodiments, the arterial PWTT can represent a difference in time between a feature of the first acoustic waveform (e.g., heart sounds waveform) and a feature of the second acoustic waveform (e.g., wrist pulse waveform). For example, in one embodiment, the arterial PWTT can be

obtained from the difference in time between a feature of the first heart sound (the S1 sound) **232** on the acoustic heart sounds waveform **230** (e.g., start, maximum peak, end, some other feature of the S1 sound **242**) and a feature of the acoustic wrist pulse waveform **240** (e.g., bottom onset or upstroke point **236** of the waveform **240** or start, maximum peak, end, some other feature of the waveform **240**). In other embodiments, the arterial PWTT can be obtained from the difference in time between a determined centroid location of the S1 sound **232** or a location of the centroid of the energy from the start of the S1 sound **232** until the start of the S2 sound **234** and a feature on the acoustic wrist pulse waveform (e.g., a bottom onset, a foot point, a peak, or some other feature). In some embodiments, the envelope of the waveform **230** or **240** is obtained and used in the analysis described herein, e.g., by finding a feature of the envelope rather than the waveform **230** or **240** itself.

In one embodiment, the arterial PWTT can be obtained from the difference in time from a location between the S1 and S2 heart sounds **232**, **234** and/or between a centroid of the energy of the S1 and S2 sounds **232**, **234** and the bottom onset of a corresponding pulse of an acoustic arterial pulse waveform (e.g., an acoustic wrist pulse waveform or an acoustic carotid pulse waveform). In some embodiments, an arterial PWTT determination based on identified features of two mechanical acoustic waveforms advantageously provides a more stable result than a PWTT determination based on an identified feature of an electrical waveform (e.g., ECG waveform) and an identified feature of a mechanical waveform (e.g., photoplethysmograph waveform).

Turning to FIG. 20, a plot **200D** is shown that includes a set of four example waveforms. The acoustic heart sounds waveform **230** and the acoustic wrist pulse waveform **240** are illustrated again, along with a third acoustic waveform (an acoustic carotid pulse waveform) **250** and an ECG waveform **260**. The plot **200D** helps to illustrate the two components that make up an overall PWTT measurement in certain embodiments: a pre-ejection period (PEP) component and an arterial transit time component. The use of two acoustic sensors results in PWTT or time-difference-of-arrival calculations that, in certain embodiments, more accurately reflect arterial pulse wave transit time, thereby allowing blood pressure measurements to be taken more efficiently.

The acoustic carotid pulse waveform **250** can help to provide another measurement indicator (e.g., a control or reference or another input component) that can be used to determine the arterial pulse wave transit time or other arterial properties because the distance is known between the two sensors. The acoustic carotid pulse waveform **250** or any of the other waveforms can provide an indication of patient breathing, as shown by the presence of noise **255** on the acoustic carotid pulse waveform **250**. In some implementations, the acoustic carotid pulse waveform **230** can be used in place of the wrist pulse waveform **240** to determine the arterial PWTT.

In some embodiments, the PEP is derived from one or more features of one or more acoustic signals. In one embodiment, the PEP is determined from the time of the start of the S1 heart sound **232** to the time of the end of the S1 heart sound **232**. In other embodiments, the PEP can be derived from a feature of an ECG waveform **260** and a feature of another physiological signal (e.g., a pleth signal or an acoustic signal). One way to measure PEP is to determine the difference between an R wave peak of the ECG waveform **260** and a feature of the S1 sound **212** on the acoustic heart sounds waveform **230** (e.g., a foot point, peak, cen-

triod, or other feature or derived location). More generally, PEP can be determined as a difference in time between any feature of the ECG waveform **260** and any feature of the acoustic heart sounds waveform **230**, including in some embodiments, a feature of the S2 heart sound **234**. The PEP can vary depending on patient pathology, and a determination of PEP can provide information regarding heart conditions to a clinician. In some embodiments, PEP is not calculated or used at all by the parameter calculation system **100** because the arterial PWTT is determined by the acoustic sensors.

FIG. 3 illustrates an embodiment of a blood pressure monitoring system **300** that can determine PWTT measurements (including a-PWTT measurements) from signals received from various sensors. The blood pressure monitoring system **300** can implement certain features of the parameter calculation system **100** described above. In particular, the system **300** can periodically measure blood pressure using a blood pressure cuff **320**, which can be an automatic occlusive cuff or the like. In addition, the system **300** can perform PWTT calculations to noninvasively detect changes in a patient's blood pressure. The illustrated blood pressure monitoring system **300** includes sensors and associated modules that can advantageously be used to monitor blood pressure. The depicted modules can be implemented in hardware and/or in software (e.g., as executed by one or more processors **330** or computing devices).

In the depicted embodiment, the system **300** includes a parameter calculator **310**, which can be implemented in hardware and/or software. The parameter calculator **310** is a more detailed implementation of the parameter calculator **110** of FIG. 1 and can include all the features thereof. Various sensors communicate with the parameter calculator **310**. These sensors include two or more acoustic sensors **302**, one or more ECG sensors **304**, one or more bioimpedance sensors **306**, and one or more optical sensors **308**. The acoustic sensors **302** can include piezoelectric transducers or other acoustic transducers for measuring a patient's body sounds, such as breathing and heart sounds. The ECG sensor(s) **304** can include ECG leads or the like for measuring the electrical activity of the heart. The bioimpedance sensor(s) **306** can include electrodes placed on the neck and/or thorax for measuring the impedance of electrical signals in the body. More detailed embodiments of these sensors are described below with respect to FIGS. 5-8.

The example parameter calculator **310** shown includes a blood pressure analyzer **312** and a noninvasive blood pressure module **314**. The blood pressure analyzer **312** can calculate arterial PWTT using the outputs of some or all of the various sensors **302**, **304**, **306**, and **308**. Based at least in part on this calculated PWTT, the blood pressure analyzer **312** can send a trigger signal to the noninvasive blood pressure module **314**. In response to receiving this trigger signal, the non-invasive blood pressure module **314** can cause the blood pressure cuff **320** to take a blood pressure measurement. In some embodiments, the non-invasive blood pressure module **314** is a separate component from the parameter calculator **310**, for example, on an Original Equipment Manufacture (OEM) board or the like.

In one embodiment, the acoustic sensor **302** is placed over the heart or near the heart of a patient so as to detect heart sounds of the patient. The acoustic sensor **302** can be positioned on the chest, back, neck, side, abdomen, or other area of the body so as to detect the heart sounds. Heart sounds can include, among others, first and second heart sounds. The first heart sound can correspond to systole, or the contraction of the ventricles and corresponding ejection

of blood from the heart. PEP can therefore be measured as a time difference between a feature of the ECG waveform derived from the electrical sensor(s) 304 and a first heart sound feature of an acoustic waveform derived from the acoustic sensor 302. The second heart sound can correspond to the beginning of diastole.

For example, referring to FIG. 4A, an example acoustic waveform 410 and ECG waveform 412 are shown that illustrate one possible PEP calculation. The acoustic waveform 410 includes peaks 422, 424 that correspond to example first and second heart sounds, respectively. The ECG waveform 412 includes a peak 432 corresponding to the R wave of the QRS complex. One way to measure PEP is to determine the difference between the R wave peak 432 and the first heart sound peak 422. In another embodiment, the PEP is measured as a difference between the R wave peak 432 and a foot 423a or 423b of the acoustic waveform 410. More generally, PEP can be determined as a difference in time between any feature of the ECG waveform 412 and any feature of the acoustic waveform 410, including in some embodiments, a feature of the second heart sound peak 424.

Referring again to FIG. 3, PWTT measurements (e.g., PEP or a-PWTT measurements) can also be calculated using the one or more bioimpedance sensors 306. The bioimpedance sensors 306 can implement principles of impedance cardiography, which can also be referred to as thoracic electrical bioimpedance. The bioimpedance sensors 306 can measure the impedance of a patient's chest cavity by injecting alternating (or direct) current through the patient's chest. The current tends to seek the path of least resistance, which is the patient's blood-filled aorta. The blood volume and velocity in the aorta can change with each heartbeat, resulting in corresponding changes in impedance measured by the bioimpedance electrodes. These changes in impedance can be used to derive PEP.

For instance, referring to FIG. 4B, an example bioimpedance waveform 440 is shown together with the ECG waveform 412 of FIG. 4A. The bioimpedance waveform includes a peak 442 that corresponds to a peak change in impedance with respect to time. This peak 442 can correspond to ejection of blood from the heart, corresponding to a current change in the aorta resulting from a heartbeat. Thus, PEP can be measured between a feature of the ECG waveform 412 and a feature of the bioimpedance waveform 440. For instance, PEP can be measured between the R wave peak 432 and a foot point 444 of the bioimpedance waveform 440. This foot point 444 is sometimes referred to as the "B" point of the bioimpedance waveform 440 and corresponds to the maximum rate of change of the waveform 440. The PEP can also be measured from the R wave peak 432 (or another feature of the ECG waveform 412) and the peak 442 of the bioimpedance waveform.

Thus, in certain embodiments, the acoustic and/or bioimpedance sensors 302, 306 of FIG. 3 can be used in conjunction with the ECG sensor(s) 304 to calculate PEP. In some implementations, only an acoustic sensor 302 and ECG sensor(s) 304 are used to calculate PEP. Other implementations employ only bioimpedance sensor(s) 306 and ECG sensor(s) 304 to calculate PEP. Still other embodiments of the system 300 can calculate PEP using acoustic sensor(s) 302 and separately calculate PEP using bioimpedance sensor(s) 306. The blood pressure analyzer 312 can average or otherwise combine the PEP calculations from these different sensors 302, 306 in some embodiments.

In other implementations, two acoustic sensors 302 of FIG. 3 are used to calculate PWTT measurements (e.g., a-PWTT or PEP measurements). In some implementations,

multiple techniques can be used to calculate PEP or a-PWTT. In some embodiments, the blood pressure analyzer 312 can average or otherwise combine the PWTT calculations from these different sensors. In other embodiments, PWTT measurements obtained from the one or more of the sensors can be used to assess confidence in the PWTT measurements obtained from other of the sensors. Additional details will be further described below in connection with FIGS. 9A-9C.

FIG. 5A illustrates a more detailed embodiment of a blood pressure monitoring system 500A including an acoustic sensor coupled to a patient. The blood pressure monitoring system 500A can implement certain features of the blood pressure monitoring system 300 and parameter calculation system 100 described above. The illustrated blood pressure monitoring system 500A includes sensors, associated modules, and a processor 530 that can advantageously be used to monitor blood pressure. The depicted modules can be implemented in hardware and/or in software (e.g., as executed by the processor 530).

The illustrated blood pressure monitoring system 500A is coupled to a patient 510. The patient 510 is shown with a cuff 522 attached to an upper arm. The cuff 522 can be implemented in combination with an automatic occlusive cuff control unit 520. The cuff 522 can be in communication with the automatic occlusive cuff control unit 520 via a cable 524. The control unit 520 can control the inflation of the cuff 522 and receive signals from the cuff 522 regarding systolic and diastolic blood pressure.

In addition to the automatic occlusive cuff, ECG sensors 562A and 562B can be coupled to the patient 510. The ECG sensors 562A, 562B can provide any of the ECG signals described above. The ECG sensors 562A and 562B can be implemented as dual electrodes or split electrodes. While the illustrated blood pressure monitoring system includes two ECG sensors 562A and 562B, in other embodiments, only one ECG sensor can be coupled to patient 510. In yet other embodiments, more than two ECG sensors can be coupled to the patient 510, such as three or more sensors. In addition, ECG sensors can be placed at different measurement site(s) than illustrated in FIG. 5A. For example, one or more ECG sensors could be coupled to the back of the patient 510.

The illustrated ECG sensors 562A, 562B can be coupled to an ECG unit 560 via cables 564A and 564B, respectively. The ECG unit 560 can interface with the ECG sensors 562A, 562B and provide an ECG signal to the processor 530. In some embodiments, the ECG unit can convert and output of ECG sensors 562A, 562B from an analog signal to a digital signal and/or perform other pre-processing. The ECG unit 560 can be implemented separate from the processor 530 or alternatively as part of the processor 530.

An optical sensor 552 can also be coupled to the patient 510. The optical sensor 552 can provide any of the plethysmograph waveforms illustrated in FIGS. 2A and 2B and/or the optical sensor data 104 described above in connection with FIG. 1. The illustrated optical sensor 552 can be coupled to oximeter unit 550 via cable 554. The oximeter unit 560 can interface with the optical sensor 552 and provide an optical signal to the processor 530. In some embodiments, the oximeter unit 550 can convert and output of optical sensor 552 from an analog signal to a digital signal and/or perform other pre-processing. The oximeter unit 550 can be implemented separate from the processor 530 or alternatively as part of the processor 530. It should be noted that in certain embodiments, the optical sensor 552 can provide data to a monitor other than a pulse oximeter.

An acoustic sensor **572** can also be coupled to the patient **510**. The acoustic sensor **552** can provide any of the acoustic signals and waveforms described above. The illustrated acoustic sensor **572** is coupled to the patient **510** at a measurement site near the patient's heart. In other embodiments, the acoustic sensor can be coupled to the patient **510** at different measurement sites, so long as the acoustic sensor can provide useful information indicative of cardiac ejection. In other embodiments, more than one acoustic sensor **572** can be used. More detail regarding the acoustic sensor **572** will be provided below in connection with FIG. 6.

The acoustic module **570** can be coupled to the acoustic sensor **572** via cable **574**. The acoustic module **570** can interface with the acoustic sensor **572** and provide an acoustic signal to the processor **530**. In some embodiments, the acoustic module can convert and output of the acoustic sensor **572** from an analog signal to a digital signal and/or perform other pre-processing. The acoustic module **570** can be implemented separate from the processor **530** or alternatively as part of the processor **530**.

The processor **530** can advantageously be used to measure indicators of blood pressure, such as PWTT, PEP, and/or arterial PWTT, using information provided by the ECG unit **560**, the oximeter unit **550**, and the acoustic module **570**. The processor **530** can include, for example, one or more microprocessors, microcontrollers, cores, digital signal processors (DSPs), or the like. The processor **530** can store instructions in a computer-readable medium. The processor **530** can also perform other operations for the blood pressure monitoring system **500A** that are not explicitly described herein.

The processor **530** can also be coupled to the automatic occlusive cuff control unit **520** via line **532**. The processor **530** can receive information regarding a blood pressure measurement of the patient **510** from the automatic occlusive cuff control unit **520**, and can activate the automatic occlusive cuff control unit **520** via the line **532**.

In certain embodiments, the processor **530** determines the arterial PWTT, compensated for PEP, using the acoustic sensor **572**, the ECG sensors **562A**, and the optical sensor **552**. The processor **530** can track changes in this arterial PWTT and trigger the automatic occlusive cuff control unit **520** to take a blood pressure measurement with the cuff **522**. The PEP-compensated arterial PWTT calculations can be more accurate than currently-available PWTT calculations that do not take PEP into account. Thus, in certain embodiments, the blood pressure monitoring system **500A** can more effectively monitor the patient's **510** blood pressure with potentially greater comfort for the patient **510**.

FIG. 5B illustrates another embodiment of a blood pressure monitoring system **500B** including bioimpedance sensors **582** coupled to the patient **510**. The blood pressure monitoring system **500B** can implement certain features of the blood pressure monitoring system **300** and parameter calculation system **100** described above. The illustrated blood pressure monitoring system **500B** can be substantially similar to the blood pressure monitoring system **500A** of FIG. 5A. However, bioimpedance sensors **582A**, **582B**, **582C**, **582D** and a bioimpedance module **580** are included in place of the acoustic sensor **572** and the acoustic module **570**.

The bioimpedance sensors **582A**, **582B**, **582C**, **582D** can be coupled to the patient **510** at various measurement sites. For example, as illustrated, two bioimpedance sensors **582A** and **582B** can be coupled to the sides of the patient **510** and two bioimpedance sensors **582C** and **582D** can be coupled to the neck of the patient **510**. Other suitable measurement

sites can be used in other embodiments. The bioimpedance sensors **582A**, **582B**, **582C**, **582D** can be used to provide the bioimpedance waveforms described above with respect to FIG. 4B and/or any of the additional sensor data **106** described above in connection with FIG. 1. Suitable bioimpedance sensors **582** can include electrodes or the like.

The bioimpedance unit **580** can be coupled to one or more of the bioimpedance sensors **582A**, **582B**, **582C**, **582D** via one or more cables **584A**, **584B**, **584C**, **584D**, respectively. The bioimpedance unit **580** can interface with one or more of the bioimpedance sensors **582A**, **582B**, **582C**, **582D** and provide one or more bioimpedance signals to the processor **530**. In some embodiments, the bioimpedance unit **580** can convert an output of one or more of the bioimpedance sensors **582A**, **582B**, **582C**, **582D** from an analog signal to a digital signal and/or perform other pre-processing. The bioimpedance unit **580** can be implemented separate from the processor **530** or alternatively as part of the processor **530**.

In certain embodiments, the processor **530** determines the arterial PWTT, compensated for PEP, using the bioimpedance sensors **582**, the ECG sensors **562A**, **562B** and the optical sensor **552**. The processor **530** can track changes in this arterial PWTT and trigger the automatic occlusive cuff control unit **520** to take a blood pressure measurement with the cuff **522**. The PEP-compensated arterial PWTT calculations can be more accurate than currently-available PWTT calculations that do not take PEP into account. Thus, in certain embodiments, the blood pressure monitoring system **500B** can more effectively monitor the patient's **510** blood pressure with potentially greater comfort for the patient **510**.

Although shown separately for ease of illustration, in certain embodiments the ECG sensors **562A**, **562B** and the bioimpedance sensors **582** can be combined. For instance, the bioimpedance sensors **582** can obtain ECG data in some implementations, and vice versa.

FIG. 6 illustrates example positioning locations for the acoustic sensors that can be used in the various systems and methods described herein (such as the parameter calculation system **100** and the blood pressure monitoring system **300**). As described above, a first acoustic sensor **602** can be placed over the heart or near the heart of a patient so as to detect heart sounds of the patient. In some embodiments, the acoustic heart sounds sensor **602** can be positioned over the heart in or near the second intercostal space; however, the acoustic heart sounds sensor **602** can be positioned at other locations (such as the chest, back, neck, side, abdomen, or other area of the body) so as to more accurately detect particular heart sounds (e.g., the S1 and S2 sounds). In some implementations, the acoustic heart sounds sensor **602** can be positioned at a location at which both the S1 and S2 heart sounds can be effectively measured. In other implementations, the acoustic heart sounds sensor **602** can be positioned at a location configured to obtain increased signal strength for a particular heart sound without regard to other heart sounds.

With continued reference to FIG. 6, a second acoustic sensor **604** can be placed at or near an artery on or near the wrist of a patient to measure an arterial pulse at a distance from the heart. For example, the second acoustic sensor **604** can be placed over the ulnar artery or the radial artery to obtain information indicative of a wrist pulse. A third acoustic sensor **606** can be placed on a neck of a patient at a location over or near a carotid artery to obtain information indicative of a carotid pulse. In some implementations, all three acoustic sensors are used. In other implementations, only the acoustic heart sounds sensor **602** and one of the

other two sensors are used. The sensors of FIG. 6 can be coupled to a parameter calculation system (e.g., the parameter calculation system 100 or the blood pressure monitoring system 300). FIG. 6 merely illustrates example locations for the types of sensors that can be used in various implementations; other suitable locations may also be used.

FIG. 7 illustrates example positioning locations for acoustic, electrocardiograph (ECG), bioimpedance and optical sensors that can be used in the various systems and methods described herein (such as the blood pressure monitoring system 300). The acoustic sensors 702A-702C are illustrated as circles, the ECG sensors 704A-704C are illustrated as squares, and the bioimpedance sensors 706A-706D are illustrated as triangles. FIG. 7 also illustrates an optical sensor 708 and an occlusive blood pressure cuff 710. The sensors of FIG. 7 can be coupled to a blood pressure monitoring system (e.g., the blood pressure monitoring system 300). Although FIG. 7 illustrates multiple sensors and multiple positioning locations, all of the sensors and/or positioning locations need not be used; FIG. 7 merely illustrates example locations for the types of sensors that can be used in various implementations. The number, locations, and type of sensors used can vary.

The blood pressure cuff 710 can be attached to an upper arm. The cuff 710 can be implemented in combination with an automatic occlusive cuff control unit (not shown). The cuff 710 can be in communication with the automatic occlusive cuff control unit via a cable and/or hose. The control unit can control the inflation of the cuff 710 and receive signals from the cuff 710 regarding systolic and diastolic blood pressure.

The acoustic sensors 702A-702C can be coupled to an acoustic module (not shown) via one or more cables or wirelessly. The acoustic module can interface with the acoustic sensors 702A-702C and provide acoustic signals to the processor 330. In some embodiments, the acoustic module can convert an output of the acoustic sensors 702A-702C from an analog signal to a digital signal and/or perform other pre-processing. The acoustic module can be implemented separate from the processor 330 or alternatively as part of the processor 330 or even as part of one or more of the sensors 702A-702C.

The ECG sensors 704A-704C can provide any of the ECG signals described herein. The ECG sensors 704A-704C can be implemented as dual electrodes or split electrodes. While the patient 700 in FIG. 7 has three ECG sensors 704A-704C, in other embodiments, only one ECG sensor or two ECG sensors can be coupled to the patient 700. In yet other embodiments, more than three ECG sensors can be coupled to the patient 700, such as four or more sensors. In addition, ECG sensors can be placed at different measurement site(s) than illustrated in FIG. 7. For example, one or more ECG sensors could be coupled to the back of the patient 700.

The illustrated ECG sensors 704A-704C can be coupled to an ECG unit (not shown) via cables or wirelessly. The ECG unit can interface with the ECG sensors 704A-704C and provide an ECG signal to a processor 330. In some embodiments, the ECG unit can convert an output of ECG sensors 704A-704C from an analog signal to a digital signal and/or perform other pre-processing. The ECG unit can be implemented separate from the processor 330 or alternatively as part of the processor 330.

The bioimpedance sensors 706A-706D can be coupled to the patient 700 at various measurement sites. For example, as illustrated, two bioimpedance sensors 706A and 706B can be coupled to the sides of the patient 700 and two bioimpedance sensors 706C and 706D can be coupled to the neck of

the patient 700. Other suitable measurement sites can be used in other embodiments. The bioimpedance sensors 706A-706D can be used to provide bioimpedance waveforms that can be used in determining measurements indicative of blood pressure (e.g., overall PWTT, PEP, arterial PWTT). Suitable bioimpedance sensors 706A-706D can include electrodes or the like.

The bioimpedance sensors 706A-706D can be coupled to a bioimpedance unit (not shown). The bioimpedance unit can interface with one or more of the bioimpedance sensors 706A-706D and provide one or more bioimpedance signals to the processor 330. In some embodiments, the bioimpedance unit can convert an output of one or more of the bioimpedance sensors 706A-706D from an analog signal to a digital signal and/or perform other pre-processing. The bioimpedance unit can be implemented separate from the processor 330 or alternatively as part of the processor 330.

Although shown separately for ease of illustration, in certain embodiments the ECG sensors 704A-704C and the bioimpedance sensors 706A-706D can be combined. For instance, the bioimpedance sensors 706A-706D can obtain ECG data in some implementations, and vice versa.

An optical sensor 708 can also be coupled to the patient 700 (e.g., to a patient's finger). The illustrated optical sensor 708 can be coupled to an oximeter unit (not shown) via a cable or wirelessly. The oximeter unit can interface with the optical sensor 708 and provide an optical signal to a processor 330. In some embodiments, the oximeter unit can convert an output of optical sensor 708 from an analog signal to a digital signal and/or perform other pre-processing. The oximeter unit can be implemented separate from the processor 330 or alternatively as part of the processor 330. It should be noted that in certain embodiments, the optical sensor 708 can provide data to a monitor other than a pulse oximeter.

The processor 330 of FIG. 3 can advantageously be used to measure indicators of blood pressure, such as PWTT, PEP, and/or arterial PWTT, using information provided by the acoustic module, the ECG unit, the oximeter unit, and/or the bioimpedance unit. The processor 330 can include, for example, a microprocessor, microcontroller, a core, a digital signal processor (DSP), or the like. The processor 330 can store instructions in a computer-readable medium. The processor 330 can also perform other operations for the blood pressure monitoring system 300 that are not explicitly described herein.

The processor 330 can also be coupled to the automatic occlusive cuff control unit. The processor 330 can receive information regarding a blood pressure measurement of the patient 700 from the automatic occlusive cuff control unit, and can activate the automatic occlusive cuff control unit.

In certain embodiments, the processor 330 determines the arterial PWTT, using two of the acoustic sensors 702A-702C, independently or in conjunction with an additional acoustic sensor, one or more of the ECG sensors 704A-704C, one or more bioimpedance sensors 706A-706D, and the optical sensor 708. In some embodiments, the processor 330 determines the arterial PWTT using a combination of one or more acoustic sensors and one or more non-acoustic sensors (for example, using two bioimpedance sensors and one acoustic sensor). The processor 330 can track changes in this arterial PWTT and trigger the automatic occlusive cuff control unit to take a blood pressure measurement with the cuff 710. The arterial PWTT calculations obtained can be more accurate than currently-available PWTT calculations that do not take PEP into account or require subtraction of the PEP to determine the arterial PWTT.

FIG. 8 illustrates an example acoustic sensor system 800 that can be used in any of the blood pressure monitoring systems described herein, such as the systems 100 and 300. FIG. 8 is a top perspective of a sensor system 800 including an acoustic sensor assembly 801 suitable for use as any acoustic sensor described herein and a monitor cable 811. The sensor assembly 801 can include an acoustic sensor 815, a cable assembly 817, and a connector 805. The sensor 815, in one embodiment, can include a sensor subassembly 802 and an attachment subassembly 804. The cable assembly 817 of one embodiment can include a cable 807 and a patient anchor 803. The various components can be connected to one another via the sensor cable 807. The sensor connector subassembly 805 can be removably attached to a monitor connector 809, which can be connected to parameter calculator or other physiological monitor (not shown) via the monitor cable 811. In one embodiment, the sensor assembly 801 can communicate with the physiological monitor wirelessly.

In an embodiment, the sensor assembly 801 can include a sensing element, such as, for example, a piezoelectric device or other acoustic sensing device. The sensing element can generate a voltage that is responsive to vibrations generated by the patient, and the sensor can include circuitry to transmit the voltage generated by the sensing element to a processor for processing. In an embodiment, the acoustic sensor assembly 801 can include circuitry for detecting and transmitting information related to biological sounds to a physiological monitor. These biological sounds may include heart, breathing, and/or digestive system sounds, in addition to many other physiological phenomena. The acoustic sensor 815 in certain embodiments can be a biological sound sensor, such as the sensors described herein. In some embodiments, the biological sound sensor is one of the sensors such as those described in the U.S. patent application Ser. No. 12/044,883, filed Mar. 7, 2008, entitled "Systems and Methods for Determining a Physiological Condition Using an Acoustic Monitor," which is incorporated in its entirety by reference herein. In other embodiments, the acoustic sensor 815 can include a biological sound sensor such as those described in U.S. Pat. No. 8,661,161, which is incorporated by reference herein. Other embodiments include other suitable acoustic sensors.

The attachment sub-assembly 804 can include a first elongate portion 806 and a second elongate portion 808. The first elongate portion 806 and the second elongate portion 808 can include patient adhesive (e.g., in some embodiments, tape, glue, a suction device, etc.) attached to an elongate member 810. The adhesive on the elongate portions 806, 808 can be used to secure the sensor subassembly 802 to a patient's skin. The elongate member 810 can beneficially bias the sensor subassembly 802 in tension against the patient's skin and reduce stress on the connection between the patient adhesive and the skin. A removable backing can be provided with the patient adhesive to protect the adhesive surface prior to affixing to a patient's skin.

The sensor cable 807 can be electrically coupled to the sensor subassembly 802 via a printed circuit board ("PCB") (not shown) in the sensor subassembly 802. Through this contact, signals can be communicated from the sensor subassembly to the physiological monitor via the sensor cable 807 and the cable 811.

In various embodiments, not all of the components illustrated in FIG. 8 are included in the sensor system 800. For example, in various embodiments, one or more of the patient anchor 803 and the attachment subassembly 804 are not included. In one embodiment, for example, a bandage or

tape is used instead of the attachment subassembly 804 to attach the sensor subassembly 602 to a measurement site. Moreover, such bandages or tapes may be a variety of different shapes including generally elongate, circular and oval, for example.

FIGS. 9A, 9B, and 9C illustrate embodiments of processes 900A, 900B, and 900C for calculating PWTT values compensated for PEP. The processes 900A, 900B, 900C can be implemented as part of any of the blood pressure monitoring systems described herein, such as the blood pressure monitoring systems 100, 300, 500A, and 500B. More particularly, the process 900A illustrates an embodiment of obtaining compensated PWTT using information obtained from an acoustic sensor. The process 900B illustrates an embodiment of PWTT calculation using bioimpedance sensors. The process 900C illustrates an embodiment of calculating PWTT without using an ECG sensor.

Referring specifically to FIG. 9A, plethysmograph, ECG, and acoustic waveforms are received by the process 900A. At block 902, an initial PWTT is calculated from the plethysmograph and ECG waveforms. This initial PWTT is determined in one embodiment by determining a time difference between features of the ECG and plethysmograph waveforms. Features on these waveforms can be determined using signal processing techniques including, but not limited to, taking derivatives of the waveforms, detecting peaks and troughs of the waveform, comparing the waveforms to models and/or thresholds, and the like. For example, an R-wave peak on an ECG waveform can be determined by detecting a point at which the ECG signal is above a (potentially adaptive) threshold and the derivative of the ECG signal is zero. As another example, a foot point on a plethysmograph waveform can be identified by the point at which the derivative of the plethysmograph waveform is zero in a time window defined after an R-wave peak. Such signal processing can be performed dynamically in real time. Alternatively or additionally, such signal processing can be performed during post processing of data.

As described above, this initial PWTT can include the arterial PWTT as well as the PEP. Thus, to obtain the arterial PWTT, further blocks of the process 900A can determine PEP so as to compensate the initial PWTT for the PEP. At block 904, a first heart sound is detected from the acoustic waveform. The PEP is then calculated at block 906 by determining a time difference between a feature of the ECG waveform and a feature of the first heart sound. The feature used on the ECG waveform to calculate the PEP 906 can be the same feature used to calculate the initial PWTT at block 902. Alternatively, different ECG features can be used to calculate PEP and the initial PWTT. At block 908, the PEP is subtracted from the initial PWTT to produce an arterial PWTT value. This arterial PWTT value can be used in determining if an automatic occlusive cuff should take a blood pressure measurement from a patient (see FIG. 10).

Advantageously, in certain embodiments, the process 900A can be performed continuously or substantially continuously so as to monitor a patient's arterial PWTT over time. The process 900A can therefore dynamically determine a patient's changing PEP over time and can compensate initial PWTT values according to this changing PEP. The process 900A can therefore, in certain embodiments, calculate more accurate PWTT than currently-available devices.

It should further be noted that the process 900A shown can also be more accurate than processes that calculate the arterial PWTT without using an ECG waveform. Because of its prominent R-wave peak, the ECG waveform can be a

more reliable triggering point than cardiac ejection signals such as heart sounds or bioimpedance signals. Accordingly, the ECG signal can be used to identify relevant cardiac ejection signal. For example, the subsequent cardiac ejection signal after an ECG signal may be the next cardiac ejection signal of interest.

Another advantage of using the ECG as a triggering signal for calculating PWTT is related to the occasional ambiguity of the cardiac ejection signal. In some cases, it may be difficult or impossible to distinguish a cardiac ejection signal from noise. In such cases, the parameter calculator 110 or 310 can use the previous PEP value as the current PEP value and calculate arterial PWTT as the difference between the ECG-to-arterial pulse signal and the previous PEP value. As PEP values may change infrequently, this substitution may be accurate.

Further, because the occurrence and/or location of the cardiac ejection signal can be ambiguous, it can be beneficial to more aggressively average the PEP measurements over time to compensate for this ambiguity. For example, a relatively slower averaging filter, which may include a longer time window of data points, may be applied to the PEP values. In contrast, the overall PWTT values may change more rapidly (see, e.g., FIG. 11), and it may be beneficial to apply a relatively faster averaging filter having a relatively shorter time window to these values.

FIG. 9B illustrates another embodiment of a process 900B that uses bioimpedance information to calculate arterial PWTT. The process 900B is substantially similar to the process 900A, except that the process 900B analyzes a bioimpedance waveform instead of an acoustic waveform.

Like the process 900A, the process 900B receives a plethysmograph waveform and an ECG waveform. At block 912, an initial PWTT is calculated from these waveforms in the manner described above with respect to FIG. 9A. At block 914, the bioimpedance waveform (or impedance cardiogram) is analyzed to detect a feature, such as a foot point, a peak change in impedance, an inflection point, or the like. At block 916, the PEP is calculated as a time difference between a feature of the ECG waveform and the feature on the bioimpedance waveform. For example, the point of maximum impedance change can be compared with a feature of the ECG waveform to determine the PEP. At block 918, the calculated PEP value is subtracted from the initial PWTT to determine the arterial PWTT. This arterial PWTT value can be used in determining if an automatic occlusive cuff should take a blood pressure measurement from a patient (see FIG. 10).

Like the process 900A, the process 900B can be performed continuously or substantially continuously so as to monitor a patient's arterial PWTT over time. The process 900B can therefore dynamically determine a patient's changing PEP over time and can compensate initial PWTT values according to this changing PEP. The process 900B can therefore, in certain embodiments, calculate more accurate PWTT than currently-available devices.

FIG. 9C illustrates another embodiment of a process 900C for calculating PWTT. However, the process 900C can advantageously calculate PWTT using an optical and acoustic signal or an optical and bioimpedance signal, without using an ECG signal. Thus, the process 900C uses fewer sensors to calculate arterial PWTT.

The process 900C receives a plethysmograph and acoustic waveform, or a plethysmograph and bioimpedance waveform. At block 922, a feature of the plethysmograph waveform is identified. At block 924, a feature of the acoustic or bioimpedance waveform is identified. Cardiac ejection can

precede the arrival of the resulting pulse at an extremity. Thus, a feature from the plethysmograph waveform obtained at the extremity can be identified when it occurs at a later time than the identified feature from the acoustic or bioimpedance waveform.

At block 926, a time difference between the identified waveform features is determined. This time is the arterial PWTT. This arterial PWTT value can be used in determining if an automatic occlusive cuff should take a blood pressure measurement from a patient (see FIG. 10).

Like the processes 900A and 900B, the process 900C can be performed continuously or substantially continuously so as to monitor a patient's arterial PWTT over time. The process 900C can therefore dynamically determine a patient's changing PEP over time and can compensate initial PWTT values according to this changing PEP. The process 900C can therefore, in certain embodiments, calculate more accurate PWTT than currently-available devices.

The process 900C can be modified in one embodiment to receive an ECG signal input to assist with identifying the feature of the plethysmograph waveform at block 922. It can be difficult to properly identify features from the plethysmograph waveform due to the double-peak nature of the waveform, as well as due to noise. An ECG signal, on the other hand, can have clearly-identifiable landmarks, including the R wave peak, among others. An ECG signal can therefore be used as a gating function to determine which feature of the plethysmograph waveform should be considered and/or which feature of the acoustic or bioimpedance waveform should be considered. In one embodiment, the first peak, foot point, or other feature in the plethysmograph occurring after a feature identified from the ECG signal can be identified as the relevant plethysmograph feature. Similarly, the first foot peak, or other feature of the acoustic or bioimpedance waveform occurring after a feature identified from the ECG signal can be identified as the relevant cardiac ejection signal feature. The ECG signal can therefore resolve ambiguities in the plethysmograph waveform, thereby improving noise immunity and/or noise reduction. Similarly, the ECG signal can also be used as a reliable identifier of a cardiac ejection signal, thereby improving the accuracy of the arterial PWTT calculation.

FIGS. 9D-9F illustrate additional embodiments of processes 900D, 900E, 900F for calculating arterial PWTT values, refining calculated arterial PWTT values, and/or determining confidence of arterial PWTT values. In some implementations, arterial PWTT values are determined from acoustic waveforms of signals from only two acoustic sensors, as described in connection with FIG. 9D. In other implementations, arterial PWTT values are determined using waveforms of signals from three or more acoustic sensors (as described in connection with FIG. 9E) or from one or more non-acoustic sensors, in addition to the two acoustic sensors (as described in connection with FIG. 9F). Each of the depicted blocks or modules of the processes 900 can be implemented by hardware and/or software modules.

With reference to FIG. 9D, the process 900D can advantageously calculate arterial PWTT using two acoustic signals, without using an ECG signal. Thus, the process 900D uses two mechanical signals rather than one electrical signal and one mechanical signal, thereby improving stability and accuracy of the arterial PWTT calculations. The use of the two acoustic signals also removes the necessity to subtract out the PEP component of the overall PWTT and instead reflects the arterial PWTT alone.

The process 900D receives an acoustic heart sounds waveform and an acoustic pulse waveform. The acoustic

pulse waveform can be, for example, an acoustic wrist pulse waveform or an acoustic carotid pulse waveform, as described above; however, the acoustic pulse waveform can be received from an acoustic sensor positioned at other locations as well. At block 927, a feature of the acoustic heart sounds waveform is identified. At block 928, a feature of the acoustic pulse waveform is identified. The feature of the acoustic heart sounds waveform can correspond to the time of cardiac ejection, which precedes the time of arrival of the resulting pulse at a location of the acoustic sensor from which the acoustic pulse waveform is generated.

Features on these waveforms can be determined using signal processing techniques including, but not limited to, taking derivatives of the waveforms, detecting peaks and troughs of the waveform, comparing the waveforms to models and/or thresholds, determining the centroid of a feature of the waveform, taking an envelope of a portion of the waveform and identifying a feature of the envelope, combinations of the same, and the like. For example, a foot point on an acoustic waveform can be identified by the point at which the derivative of the acoustic waveform is zero in a time window defined after an electrical trigger (e.g., as identified by an ECG sensor). As another example, a centroid or "middle" of a pulse, burst or wave of an acoustic waveform can be determined. In some embodiments, the centroid can be determined by constructing an amplitude envelope of the pulse, sound burst, or pressure wave and then performing a normalized weighting of each time point according to the envelope amplitude, with the highest energy point of the envelope being the centroid time of the pulse or sound (e.g., heart sound). The centroid determination can be performed in the time domain or frequency domain. In some embodiments, the centroid determination includes sampling and/or filtering of the pulse, sound burst, or pressure wave. Such signal processing can be performed dynamically, in real time. Alternatively or additionally, such signal processing can be performed during post processing of data.

At block 929, a time difference between the identified waveform features is determined. This time can be considered to be the arterial PWTT in one embodiment. This arterial PWTT value can be used in determining if an automatic occlusive cuff should take a blood pressure measurement from a patient (see FIG. 8). The process 900D can be performed continuously or substantially continuously so as to monitor a patient's arterial PWTT over time. Alternatively, the process 900D can be performed as a spot-check upon occurrence of predetermined conditions or at predetermined time intervals.

The process 900D can be modified in one embodiment to receive an ECG signal input to assist with identifying the feature of the acoustic heart sounds waveform at block 927. It can be difficult to properly identify features from acoustic waveforms due to noise or other characteristics. An ECG signal, on the other hand, can have clearly-identifiable landmarks, including the R wave peak, among others. An ECG signal can therefore be used as a gating function to determine which heart sound should be considered. In one embodiment, the first heart sound of the acoustic heart sounds waveform occurring after a feature identified from the ECG signal can be identified as the relevant acoustic heart sounds feature. The ECG signal can therefore resolve ambiguities in the acoustic waveforms, thereby improving noise immunity and/or noise reduction. In some embodiments, the ECG signal can be used to identify the transition from electrical to mechanical behavior. The time delay between the ECG signal and the first heart sound (e.g., S1 sound) detected by the acoustic heart sounds sensor can

provide an indication of the health of the heart or other potential pathological conditions that may warrant medical attention. However, the ECG signal input is not used or needed in other embodiments.

FIGS. 9E and 9F illustrate embodiments of processes 900E, 900C for determining PWTT values, refining calculated PWTT values, and/or determining confidence of PWTT values. More particularly, the process 900E illustrates an embodiment of a process for calculating, refining, or assessing PWTT values using information obtained from multiple acoustic sensors, one of which is an acoustic heart sounds sensor. The process 900C illustrates an embodiment of a system for arterial PWTT calculation, refinement, or assessment using acoustic sensors in conjunction with additional sensors, such as ECG sensors, optical sensors, and/or bioimpedance sensors. The processes 900E, 900C can be implemented as part of the parameter calculation system 100 or the blood pressure monitoring system 300. Each of the depicted blocks or modules of the processes 900 can be implemented by hardware and/or software modules.

Referring specifically to FIG. 9E, the process 900E receives three acoustic waveforms. These three acoustic waveforms can include an acoustic heart sounds waveform and two acoustic pulse waveforms (a first pulse waveform and a second pulse waveform). For example, the acoustic pulse waveforms can include a wrist pulse waveform and a carotid pulse waveform. The acoustic heart sounds waveform and a first pulse waveform (e.g., wrist pulse waveform) can be received by PWTT determination block 932 and the acoustic heart sounds waveform and a second pulse waveform can be received by PWTT determination block 934. The PWTT determination block 932 can calculate a first arterial PWTT (a-PWTT A) value from the acoustic heart sounds waveform and the first acoustic pulse waveform. The PWTT determination block 934 can calculate a second arterial PWTT (a-PWTT B) value from the acoustic heart sounds waveform and the second acoustic pulse waveform. These initial arterial PWTT measurements are determined in one embodiment by determining a time difference between features of the acoustic heart sounds waveform and the acoustic pulse waveform (as described in connection with FIG. 9A).

In some implementations, the initial arterial PWTT values (a-PWTT A and a-PWTT B) can be provided to a comparison module 936. The comparison module 906 can analyze the two initial arterial PWTT values to generate a final arterial PWTT output value. In some implementations, the comparison module 936 can compare the two initial arterial PWTT values to determine a difference between the two values. The comparison module 936 can derive a confidence value from the calculated difference. In other implementations, the comparison module 936 can average or otherwise combine the two initial arterial PWTT values to output a refined final arterial PWTT output value. In some embodiments, the two initial arterial PWTT values are weighted. In yet other implementations, the comparison module 936 can select one of the two initial arterial PWTT values to output as the final arterial PWTT output value. The comparison module 936 can make this selection based on confidence values, based on comparison to historical data or thresholds, based on patient-specific factors, and/or the like.

In some embodiments, the second pulse acoustic waveform can simply be used to provide another reference or gating point in identifying a feature of the first pulse acoustic waveform. In other embodiments, the second pulse acoustic waveform can be used to identify other patient characteris-

tics (e.g., patient breaths, respiratory rate, respiratory pause, or other respiratory conditions, as discussed above).

FIG. 9F illustrates an embodiment of a process 900C that uses information obtained from one or more non-acoustic sensors in addition to one or more acoustic sensors to calculate, refine, or assess arterial PWTT measurements.

Like the process 900E, the process 900E can calculate two arterial PWTT values (a-PWTT A and a-PWTT B) at PWTT determination blocks 932 and 934, respectively. The process 900C can also receive an ECG signal input, a plethysmograph signal input, and/or a bioimpedance signal input in addition to the acoustic signal inputs. An overall PWTT value (including arterial PWTT and PEP components) can be calculated at PWTT determination block 937 by determining a time difference between a feature of a plethysmograph waveform and a feature of an ECG waveform. Further blocks of the process 900C can determine PEP so as to compensate the overall PWTT for the PEP. The PEP is calculated at block 938 by determining a time difference between a feature of the ECG waveform and a feature of the acoustic heart sounds waveform or a bioimpedance waveform in the manner described above. The feature used on the ECG waveform to calculate the PEP 938 can be the same feature used to calculate the overall PWTT at block 936. Alternatively, different ECG features can be used to calculate PEP and the overall PWTT. At block 940, the PEP is subtracted from the initial PWTT to produce a third arterial PWTT value (a-PWTT C).

In other embodiments, the third arterial PWTT value can be derived from a time difference between a feature of an acoustic waveform or a bioimpedance waveform and a pleth waveform such that PEP need not be calculated, as described above.

Similar to the process 900E, the three arterial PWTT values can be received by the comparison module 936 and analyzed to output a final arterial PWTT value. In some implementations, the comparison module 936 can compare the three initial arterial PWTT values to determine differences between any two of the three values. The comparison module 936 can derive a confidence value from the calculated differences. In other implementations, the comparison module 936 can average or otherwise combine the three initial arterial PWTT values to output a refined final arterial PWTT output value. In some embodiments, the three initial arterial PWTT values are weighted. In yet other implementations, the comparison module 936 can select one of the three initial arterial PWTT values to output as the final arterial PWTT output value. The comparison module 936 can make this selection based on confidence values, based on comparison to historical data or thresholds, based on patient-specific factors, and/or the like.

In other embodiments, arterial PWTT values can be calculated using one or more non-acoustic sensors in combination with one or more acoustic sensors. For example, arterial PWTT values can be calculated from time differences between a feature of a bioimpedance waveform (e.g., generated from signals received from two bioimpedance sensors) and a feature of an acoustic waveform (e.g., received from an acoustic pulse sensor positioned over or proximate a wrist, leg or carotid artery).

FIG. 10 illustrates an embodiment of a process 1000 for determining whether to trigger an alternative blood pressure measurement. This process 1000 can be implemented by any of the systems 100, 300, described above. Advantageously, in certain embodiments, the process 1000 can determine, based at least partly on non-invasive PWTT measurements, whether to trigger an automatic occlusive cuff. As a result,

continuous or substantially continuous monitoring of a user's blood pressure can occur, allowing the frequency of occlusive cuff measurements to potentially be reduced.

At block 1002, a first arterial PWTT measurement is determined at a first point in time. The arterial PWTT can be determined using any of the techniques above, such as by calculating PEP and by compensating an overall PWTT value with the PEP. Similarly, a second arterial PWTT measurement is taken at a second point in time at block 1004. These arterial PWTT measurements can be taken from successive heart beats in one embodiment. In another embodiment, the first and second arterial PWTT values each represent arterial PWTT values averaged over multiple heartbeats.

At block 1006, a difference between the two arterial PWTT measurements is determined. It is then determined at decision block 1008 whether a new blood pressure measurement is required. In certain embodiments, this decision can be made by determining whether the difference between the two measurements is greater than a threshold. A difference greater than a threshold can be indicative of a change in a patient's blood pressure. Therefore, if the difference is greater than the threshold, an occlusive cuff is triggered to take a new blood pressure measurement at block 1010. If the difference is not greater than the threshold, then the process 1000 loops back to block 1002. Effectively, the process 1000 therefore can trigger occlusive cuff measurements when the threshold is exceeded and can continue monitoring arterial PWTT measurements otherwise.

In certain embodiments, the process 1000 analyzes changes in arterial PWTT measurements using an absolute difference technique or a moving difference technique. With the absolute difference technique, the process 1000 measures the PWTT at a first fixed time. Subsequent arterial PWTT measurements (e.g., the second measurement at block 1004) are compared to the initial arterial PWTT at the first fixed time to determine whether the difference between these measurements exceeds a threshold. With the moving difference technique, the first and second arterial PWTT measurements are compared for successive points in time. The first arterial PWTT measurement is therefore not taken at a fixed time but instead changes over time. Thus, the moving difference technique can approximate a derivative of the arterial PWTT measurements. The moving difference can be compared to a threshold at block 1008. An advantage of using the moving difference technique is that it can potentially ignore drifts in arterial PWTT measurements due to calibration changes or other errors.

Thus, in certain embodiments, the process 1000 can refrain from triggering an occlusive cuff until the non-invasive measurement differs enough to trigger such a measurement. Advantageously, in certain embodiments, the process 1000 can therefore allow a user to postpone the discomfort and potential physiological damage associated with occlusive blood pressure measurements, while the non-invasive measurement (e.g., arterial PWTT) is within a certain tolerance.

Although the PWTT measurements have been described herein as being used to trigger an occlusive cuff, in certain embodiments the PWTT measurements can also or instead be used to derive an estimate of blood pressure. A calibration function or curve can be determined that maps PWTT measurements to blood pressure values. The slope and intercept of the calibration curve can be determined experimentally.

PWTT Noise Compensation

As described above, in addition to compensating PWTT for PEP, the parameter calculation system **100** can also compensate PWTT data for noise. FIGS. **11** and **12** illustrate embodiments for compensating PWTT data for noise. By compensating PWTT data for noise, more accurate PWTT measurements can be obtained. The features described with respect to FIGS. **11** and **12** can be used in combination with any of the features described herein.

FIG. **11** depicts an example plot **1100** that illustrates noise in a set of arterial PWTT data. In the example plot **1100**, PWTT values taken over time are represented as a PWTT waveform **1110**. Variability in the PWTT waveform **1110** reflects noise in the PWTT waveform **1110**. Noisy PWTT data can lead to lower quality PWTT measurements, resulting in too frequent or too infrequent triggering of a blood pressure cuff. In certain circumstances, noisy PWTT can even lead to missing a clinically significant change in blood pressure.

One technique to reduce the effects of noise in the PWTT data is to average the PWTT data overtime. A time-averaged PWTT waveform **1120** is shown in FIG. **11**. The average can be calculated from PWTT data points taken over a certain time period. PWTT data points can be averaged by applying a smoothing filter, such as a low pass filter. Determining a number of PWTT data points and/or an averaging time to include in an average can involve tradeoffs. A longer averaging time can reduce the presence of noise in the PWTT data. However, a longer averaging time can also reduce the benefits of using PWTT as an indicator of blood pressure to trigger an occlusive cuff. For example, a long averaging time can cause rapidly-changing features on a waveform to be missed. In contrast, a shorter averaging time using fewer data PWTT data points may not sufficiently filter out noise.

In certain embodiments, averaging can be improved by dynamically adjusting the averaging time according to the amount of noise present in the PWTT data. If a higher level of noise is present, a longer averaging time can be selected. Conversely, if less noise is present, a shorter averaging time can be used. However, it can be difficult to differentiate noise from signal in the PWTT data. Thus, determining the level of the noise in the PWTT data and therefore the amount of averaging to perform can be nontrivial.

To select an appropriate averaging time, in one embodiment a signal correlated with the PWTT data can be analyzed. Heart rate is such a correlated signal, and respiratory rate is another. An example heart rate signal is shown plotted over time as a waveform **1130** in FIG. **11**. The variability of the heart rate waveform **1130** corresponds to the variability of the PWTT data **1110**, indicating that the heart rate and PWTT can be correlated. The heart rate waveform **1130** (or respiratory rate) can therefore be analyzed to determine the amount of noise present in the PWTT data to thereby select an averaging time for the PWTT data. Likewise, in some applications, such as where accurate heart rate measurements are desired, it can be useful to analyze the PWTT data to determine an averaging time for the heart rate data. Dynamic signal averaging is described in greater detail below with respect to FIG. **10**.

Another possible use of the heart rate (or respiratory rate) data is to use the heart rate (or respiratory rate) as a noise reference in an adaptive filter. For example, the system **100** (or any other system described herein) can adaptively filter or adaptively cancel noise in the PWTT data using the heart rate as a noise reference. Any of a variety of adaptive algorithms can be used by the parameter calculation system **100**. For instance, the adaptive algorithm can implement one

or more of the following: a least mean squares algorithm (LMS), a least squares algorithm, a recursive least squares (RLS) algorithm, a Kalman filter, a joint process estimator, an adaptive joint process estimator, a least-squares lattice joint process estimator, a least-squares lattice predictor, a correlation canceller, optimized or frequency domain implementations of any of the above, any other linear predictor, combinations of the same, and the like. In still other embodiments, the PWTT data can be both adaptively filtered and averaged using a dynamically-adjusted averaging filter.

Further, as can be seen in FIG. **11**, the PWTT data in the waveforms **1110** or **1120** can be correlated with a systolic blood pressure data **1125** over time. As shown, the relationship between the PWTT data and the systolic blood pressure data **1125** can be inverse or approximately inverse.

FIG. **12** illustrates an embodiment of a signal averaging process **1200**. The signal averaging process **1200** can be implemented by any of the systems **120**, **300**, **500A**, or **500B** described above. Advantageously, in certain embodiments, the process **1200** uses heart rate data to dynamically adjust the averaging time of an averaging filter applied to the PWTT data.

At block **1202**, statistics of the heart rate data are analyzed to determine a measure of the noise in the heart rate data. A variety of statistics of the heart rate data can be calculated at block **1202**, including variance, standard deviation, and entropy, combinations of the same, and the like. For example, the standard deviation can be calculated from the heart rate data to measure the degree of dispersion or variability in the heart rate data. A higher standard deviation can reflect greater variability in the heart rate data, which can in turn reflect more noise in the heart rate data. Conversely, a lower standard deviation can reflect lower noise in the heart rate data. More generally, any measure of variation or change in the heart rate data can be calculated at block **1202**.

At block **1204**, one or more averaging parameters of an averaging filter can be adjusted based on the statistical calculation. In one embodiment, an averaging parameter such as averaging time is adjusted. For example, if the standard deviation of the heart rate data is relatively high, reflecting more noise, a relatively long averaging time can be selected. On the other hand, if the standard deviation is relatively lower, reflecting less noise, a relatively shorter averaging time can be selected. More generally, the one or more averaging parameters can include any parameter of the averaging filter that can be tuned. The averaging parameters can therefore include the order of the averaging filter, the number of points averaged (e.g., for a simple moving average filter), the time constant of the filter (e.g., for a low pass averaging filter), and an array of coefficients for more complex averaging filters (such as any of the adaptive filters described above with respect to FIG. **9**).

At block **1210**, the averaging filter with the selected averaging time is applied to the PWTT data. Averaging can include computing a mean, median, and/or mode. In some embodiments, a weighted average of PWTT measurements can be applied. For example, the averaging filter can place a greater weight on more recent PWTT data and/or data with a corresponding statistic that indicates lower variability. For signals with relatively lower variability in the heart rate data, the averaging filter may not be applied to the PWTT input at all. Further, in other embodiments, the statistics of the PWTT signal can be evaluated to determine the amount of noise and therefore averaging time, rather than evaluating the statistics of the heart rate signal.

Phase Impact Reduction

In some embodiments, the PWTT measurements and calculations described herein are determined in terms of time. Accordingly, phase delay or phase noise can be introduced between successive filters of the parameter calculation system or blood pressure monitoring system. FIG. 13 illustrates an embodiment of front end circuitry 1300 that can be configured to condition analog electrical signals output by the acoustic sensors for processing. In some embodiments, the front end circuitry 1300 can reduce the phase impact introduced into the system. The front end circuitry 1300 can include a pre-amplification module 1305, one or more filters 1310, and an analog-to-digital converter (ADC) 1315.

The pre-amplification module 1305 can receive and amplify the voltage signal from the acoustic sensors, such as by a predetermined gain. In some implementations, the pre-amplification module 1305 introduces a high input impedance to drop the high pass filtering effect of the piezoelectric acoustic sensors. In some implementations, the pre-amplification module 1305 includes circuitry to convert an AC signal output from the acoustic sensor to a DC signal. In some implementations, the one or more filters 1310 include one or more low pass filters to allow the low frequency heart and pulse acoustic signals detected by the acoustic sensors while attenuating high frequency signals, such as high frequency noise. The one or more filters 1310 may include other types of filters, such as high pass or bandpass filters, instead of or in addition to, the one or more low pass filters. In some implementations, the one or more filters 1310 can be adjusted to reduce the phase distortion by changing the location of the zeros and/or poles of the one or more filters 1310.

In some implementations, the cutoff frequency of the acoustic sensors (which can be represented as capacitors in terms of frequency response analysis) can effectively be changed to a much lower frequency than an acoustic sensor used for respiration detection (e.g., to 0.01 Hz or 0.1 Hz). According to some embodiments, the acoustic sensors can have a cutoff frequency that is inversely dependent on the capacitance of the sensor and the input resistance of the amplifier or other circuit that receives the signal. The acoustic sensors may be modified to achieve a much lower cutoff frequency. For example, the low frequency response can be extended by changing the piezoelectric characteristics of the acoustic sensor (e.g., making the capacitance of the piezoelectric material itself larger, such as by the composition, size, thickness, etc. of the piezoelectric material), by making the input resistance higher, and/or by placing a large (as compared to the piezoelectric capacitance) capacitor in shunt with the acoustic sensor. In some embodiments, rather than lowering the cutoff frequency of the acoustic sensor itself, a compensatory filter can be inserted in the signal path. In one embodiment, the cutoff frequency is allowed to be significantly higher than the frequency band of interest, such that the acoustic sensor is effectively responsive to the derivative of the signal. Thus, the compensatory filter can be an integrator, which recreates the original acoustic signal. In some embodiments, it may be neither necessary nor desirable to extend the low frequency response of the acoustic sensors. The output from the filters 1310 can be amplified into a higher voltage signal and then converted to a digital signal by the ADC converter 1315. In some embodiments, using a single ADC converter 1315 to convert each signal, or multiple of the signals, including acoustic, electrical, and/or optical, can also reduce phase distortion between the signals. Further, oversampling in the

ADC 1315 can also reduce phase distortion between the signals. The digital signal can then pass to a digital signal processor for processing in preparation for display on a monitor or screen.

5 Patient Calibration

FIGS. 14A and 14B illustrate an embodiment of a process 1400 for calibrating pulse wave transit time measurements based on a personalized patient calibration factor. Pulse wave transit time measurements can vary depending on changes in blood pressure. The variance can be defined by a slope measurement, which can be the change in pulse wave transit time per the change in pressure (e.g., change in number of milliseconds per change in number of millimeters of mercury (mmHg)). The variance, or slope, of the calibration curve can differ greatly from patient to patient. For example, the slope can vary by a factor of between 2:1 to 4:1 or greater between patients. This variance can be due to a variety of physiological factors, such as hemodynamic factors of capillary flow or perfusion. The slope may also vary based on the introduction of drugs (including even blood pressure regulation drugs), patient comorbidity, gender, age, or other factors. Accordingly, it can be advantageous to determine the slope of the PWTT/blood pressure calibration curve for the individual patient and use the determined slope to interpret subsequent PWTT measurements.

The individualized patient calibration process 1400 can reduce the effect of slope variability between patients by uniquely and individually calibrating the PWTT measurements for the individual patient, thereby reducing the inaccuracy of blood pressure measurement frequency or false alarms based on PWTT measurements. The individualized patient calibration process 1400 therefore advantageously provides a mechanism for more efficient interpretation of PWTT measurements for individual patients by compensating for the variability of slope. Alternatively, in one embodiment, a patient monitor (such as any of those described herein) can calculate a baseline PWTT variability offset that is applied to the calculation of PWTT for multiple patients. This baseline adjustment may, but need not, be calibrated to individual patients or segments of patients (e.g., segments for drug users, segments based on gender, age, or comorbidity).

The term PWTT measurements as used herein with respect to FIGS. 14A and 14B can refer to overall PWTT (including PEP and a-PWTT components) or arterial PWTT. The individualized patient calibration process 1400 can be implemented by the blood pressure monitoring systems and/or parameter calculation systems described herein (e.g., systems 140 and 300).

The calibration process 1400 begins at block 1402, wherein at least two blood pressure measurements of a patient are obtained at different times. The blood pressure measurements can include just systolic blood pressure measurements, just diastolic blood pressure measurements, and/or combinations of the systolic and diastolic blood pressure measurements (for example, mean or median blood pressure measurements).

In some implementations, blood pressure measurements can be taken at two different elevations of known hydrostatic pressure at two different times. For example, a first blood pressure measurement can be taken when the patient is lying down on a bed or table with the arm at the patient's side and a second blood pressure measurement can be taken with the arm raised up at least approximately perpendicularly to the patient's body. The blood pressure measurements can be normalized to account for changes in pressure due to the change in elevation. The changes in pressure due to the

change in elevation can be determined based on a measured or known distance between the locations of the measurements and calculated or known hydrostatic pressure and/or based on actual hydrostatic pressure measurements. The distance and/or pressure measurements can be obtained by any of a variety of sensors or transducers. In some embodiments, a wrist cuff is used to obtain the blood pressure measurements (which, in some embodiments, reduces the effects of the arterial-to-capillary time delays addressed above). Other methods can be used to obtain blood pressure measurements over time in accordance with yet other implementations.

At block **1404**, pulse wave transit times are measured to correspond with the blood pressure measurements. Although block **1404** is illustrated as occurring after block **1402**, the pulse wave transit times can be measured simultaneously or substantially simultaneously (e.g., within a few seconds or within a few milliseconds) with the blood pressure measurements. Accordingly, the pulse wave transit times can be mapped to their corresponding blood pressure measurements. The blood pressure measurements and pulse wave transit time measurements can be stored in memory (at least temporarily). In some embodiments, the memory can include a predetermined capacity of measurements and the oldest measurements can be replaced by new measurements when capacity has been reached. The stored measurements can be used to generate a calibration curve defined by a plot of the pulse wave transit times on one axis (e.g., vertical axis) and the corresponding blood pressure measurements on the other axis (e.g., horizontal axis).

At block **1406**, an individual patient's slope corresponding to the change in pulse wave transit time per change in blood pressure (e.g., slope of the calibration curve) is determined from the blood pressure and PWTT measurements obtained at block **1402** and block **1404**. A patient's PWTT ms/mmHg slope can be determined from two or more blood pressure measurements and two or more corresponding PWTT measurements. In accordance with some embodiments, the slope is inferred over time from a plurality of frequent blood pressure and corresponding PWTT measurements. The slope determination can then be refined over time through less frequent natural blood pressure and corresponding PWTT measurements.

Based on the determined slope of the patient, a personalized, or individualized, patient calibration factor can be identified at block **1408** and used to interpret subsequent pulse wave transit time measurements of the patient with reduced concern for patient variability.

At block **1410**, a pulse wave transit time is measured (for example, an arterial pulse wave transit time can be measured as described herein). At block **1412**, the process **1400** estimates a change in the patient's blood pressure based on the measured pulse wave transit time. The measured pulse wave transit time has been calibrated using the individualized patient calibration factor, thereby reducing patient variability.

At decision block **1414**, the process **1400** determines whether the estimated blood pressure change satisfies a condition that warrants performance of an action (e.g., whether the estimated blood pressure change is significant enough to perform an action). The condition can be, for example, a blood pressure change that exceeds a threshold blood pressure change value, cuff triggering value, a patient alarm triggering value, and/or the like. The condition can be patient-specific based on patient-specific factors or generic to all patients. If the condition is satisfied, the process **1400** proceeds to block **1416**, wherein an appropriate action is

performed based on the satisfied condition. For example, if an estimated blood pressure change exceeds a threshold change, a blood pressure cuff measurement can be triggered to determine and/or confirm the accuracy of the estimated blood pressure change. In some embodiments, the new blood pressure measurement can be added to a running tally to refine the individualized patient calibration factor.

As another example, if an estimated blood pressure change exceeds an alarm condition, a patient alarm can be triggered so that the patient can receive immediate medical attention. In some embodiments, the alarm is triggered only if confidence in the estimated blood pressure change is above a predetermined level. In some embodiments, a blood pressure measurement is obtained to confirm the accuracy of the estimated blood pressure change prior to triggering an alarm.

In some implementations, the determination of whether the blood pressure change is significant enough to warrant an action at block **1408** includes a multivariate determination based on other factors in addition to pulse wave transit time (e.g., heart rate). For example, if heart rate and pulse wave transit time are changing, it is more likely that the blood pressure is changing in a manner such that an action is recommended to be performed.

In some situations, the patient's calibration curve slope can change due to changes in patient conditions (e.g., changes in hemodynamic state, introduction of drugs, etc.). Accordingly, in some implementations, the slope is tracked over time to determine whether a recalibration process may be recommended. Other inputs or physiological parameters, such as heart rate, can be analyzed in determining whether recalibration of the personalized patient calibration factor should be performed as well.

In other implementations, a slope of a patient's blood pressure over time can be determined instead of, or in addition to, the PWTT/blood pressure calibration curve slope and used to identify a personalized patient calibration factor, which can in turn be used to interpret pulse wave transit time measurements.

Terminology

Many other variations than those described herein will be apparent from this disclosure. For example, depending on the embodiment, certain acts, events, or functions of any of the algorithms described herein can be performed in a different sequence, can be added, merged, or left out all together (e.g., not all described acts or events are necessary for the practice of the algorithms). Moreover, in certain embodiments, acts or events can be performed concurrently, e.g., through multi-threaded processing, interrupt processing, or multiple processors or processor cores or on other parallel architectures, rather than sequentially. In addition, different tasks or processes can be performed by different machines and/or computing systems that can function together.

The various illustrative logical blocks, modules, and algorithm steps described in connection with the embodiments disclosed herein can be implemented as electronic hardware, computer software, or combinations of both. To clearly illustrate this interchangeability of hardware and software, various illustrative components, blocks, modules, and steps have been described above generally in terms of their functionality. Whether such functionality is implemented as hardware or software depends upon the particular application and design constraints imposed on the overall system. For example, the parameter calculation system **100** can be implemented by one or more computer systems or by a computer system including one or more processors. The

described functionality can be implemented in varying ways for each particular application, but such implementation decisions should not be interpreted as causing a departure from the scope of the disclosure.

The various illustrative logical blocks and modules described in connection with the embodiments disclosed herein can be implemented or performed by a machine, such as a general purpose processor, a digital signal processor (DSP), an application specific integrated circuit (ASIC), a field programmable gate array (FPGA) or other programmable logic device, discrete gate or transistor logic, discrete hardware components, or any combination thereof designed to perform the functions described herein. A general purpose processor can be a microprocessor, but in the alternative, the processor can be a controller, microcontroller, or state machine, combinations of the same, or the like. A processor can also be implemented as a combination of computing devices, e.g., a combination of a DSP and a microprocessor, a plurality of microprocessors, one or more microprocessors in conjunction with a DSP core, or any other such configuration. A computing environment can include any type of computer system, including, but not limited to, a computer system based on a microprocessor, a mainframe computer, a digital signal processor, a portable computing device, a personal organizer, a device controller, and a computational engine within an appliance, to name a few.

The steps of a method, process, or algorithm described in connection with the embodiments disclosed herein can be embodied directly in hardware, in a software module executed by a processor, or in a combination of the two. A software module can reside in RAM memory, flash memory, ROM memory, EPROM memory, EEPROM memory, registers, hard disk, a removable disk, a CD-ROM, or any other form of non-transitory computer-readable storage medium, media, or physical computer storage known in the art. An exemplary storage medium can be coupled to the processor such that the processor can read information from, and/or write information to, the storage medium. The storage medium can be external to or remote from the processor. For example, the storage medium may be a storage device accessible by the processor over a network. In the alternative, the storage medium can be integral to the processor. The processor and the storage medium can reside in an ASIC. The ASIC can reside in a user terminal. In the alternative, the processor and the storage medium can reside as discrete components in a user terminal.

Conditional language used herein, such as, among others, "can," "might," "may," "e.g.," and the like, unless specifically stated otherwise, or otherwise understood within the context as used, is generally intended to convey that certain embodiments include, while other embodiments do not include, certain features, elements and/or states. Thus, such conditional language is not generally intended to imply that features, elements and/or states are in any way required for one or more embodiments or that one or more embodiments necessarily include logic for deciding, with or without author input or prompting, whether these features, elements and/or states are included or are to be performed in any particular embodiment. The terms "comprising," "including," "having," and the like are synonymous and are used inclusively, in an open-ended fashion, and do not exclude additional elements, features, acts, operations, and so forth. Also, the term "or" is used in its inclusive sense (and not in its exclusive sense) so that when used, for example, to connect a list of elements, the term "or" means one, some, or all of the elements in the list.

While the above detailed description has shown, described, and pointed out novel features as applied to various embodiments, it will be understood that various omissions, substitutions, and changes in the form and details of the devices or algorithms illustrated can be made without departing from the spirit of the disclosure. As will be recognized, certain embodiments of the inventions described herein can be embodied within a form that does not provide all of the features and benefits set forth herein, as some features can be used or practiced separately from others.

What is claimed is:

1. An electronic method for monitoring blood pressure of a patient, the method comprising:

receiving physiological electrical information associated with a patient, the physiological electrical information configured to reflect electrical activity of the patient's heart;

receiving a cardiac ejection information associated with the patient, the cardiac ejection information reflecting ejection of blood from the patient's heart;

receiving arterial pulse information associated with a limb of the patient from an acoustic sensor;

determining an arterial pulse wave transit time (PWTT) measurement that compensates for a pre-ejection period of a cardiac cycle associated with the patient's heart, based at least partly on the physiological electrical information, the cardiac ejection information, and the arterial pulse information;

receiving a heart rate signal that is correlated with a set of arterial PWTT measurements, including the arterial PWTT measurement;

determining a variability in the received heart rate signal; adjusting an averaging parameter for an averaging filter configured to be applied to the set of arterial PWTT measurements based on the variability;

applying the averaging filter to the set of arterial PWTT measurements to thereby selectively reduce noise in the set of arterial PWTT measurements; and

monitoring blood pressure of the patient based on the application of the averaging filter to the set of arterial PWTT measurements.

2. The electronic method of claim 1, wherein the averaging parameter comprises one or more of the following: an averaging time, a filter order, a number of averaging points, and a value of one or more coefficients.

3. The electronic method of claim 1, wherein the variability comprises a statistic.

4. The electronic method of claim 3, wherein the statistic comprises a standard deviation of the heart rate signal.

5. The electronic method of claim 4, wherein said adjusting comprises selecting a longer averaging time responsive to the standard deviation having a higher value compared with a shorter averaging time responsive to the standard deviation having a lower value.

6. The electronic method of claim 5, wherein the averaging filter is configured to have a longer averaging time for a first portion of the set of arterial PWTT measurements and a shorter averaging time for a second portion of the set of arterial PWTT measurements.

7. The electronic method of claim 1, further comprising: adaptively compensating a noise component of the set of arterial PWTT measurements using the determined variability.

8. The electronic method of claim 7, wherein said adaptively compensating comprises applying an adaptive filter to the set of arterial PWTT measurements.

9. The electronic method of claim 8, wherein said applying the adaptive filter comprises using the heart rate signal as a noise reference for the adaptive filter.

10. An electronic method for monitoring blood pressure of a patient, the method comprising:

receiving physiological electrical information associated with a patient, the physiological electrical information configured to reflect electrical activity of the patient's heart;

receiving a cardiac ejection information associated with the patient, the cardiac ejection information reflecting ejection of blood from the patient's heart;

receiving arterial pulse information associated with a limb of the patient from an acoustic sensor;

determining an arterial pulse wave transit time (PWTT) measurement that compensates for a pre-ejection period of a cardiac cycle associated with the patient's heart, based at least partly on the physiological electrical information, the cardiac ejection information, and the arterial pulse information;

receiving a respiratory rate signal that is correlated with a set of arterial PWTT measurements, including the arterial PWTT measurement;

determining a variability in the received respiratory rate signal;

adjusting an averaging parameter for an averaging filter configured to be applied to the set of arterial PWTT measurements based on the variability;

applying the averaging filter to the set of arterial PWTT measurements to thereby selectively reduce noise in the set of arterial PWTT measurements; and

monitoring blood pressure of the patient based on the application of the averaging filter to the set of arterial PWTT measurements.

11. The electronic method of claim 10, wherein the averaging parameter comprises one or more of the following: an averaging time, a filter order, a number of averaging points, and a value of one or more coefficients.

12. The electronic method of claim 10, wherein the variability comprises a statistic.

13. The electronic method of claim 12, wherein the statistic comprises a standard deviation of the respiratory rate signal.

14. The electronic method of claim 13, wherein said adjusting comprises selecting a longer averaging time responsive to the standard deviation having a higher value compared with a shorter averaging time responsive to the standard deviation having a lower value.

15. The electronic method of claim 14, wherein the averaging filter is configured to have a longer averaging time for a first portion of the set of arterial PWTT measurements and a shorter averaging time for a second portion of the set of arterial PWTT measurements.

16. The electronic method of claim 10, further comprising:

adaptively compensating a noise component of the set of arterial PWTT measurements using the determined variability.

17. The electronic method of claim 16, wherein said adaptively compensating comprises applying an adaptive filter to the set of arterial PWTT measurements.

18. The electronic method of claim 17, wherein said applying the adaptive filter comprises using the respiratory rate signal as a noise reference for the adaptive filter.

* * * * *

专利名称(译)	无创血压测量系统		
公开(公告)号	US10052037	公开(公告)日	2018-08-21
申请号	US15/229840	申请日	2016-08-05
[标]申请(专利权)人(译)	KINAST ERIC KARL TELFORT VALERY 摹		
申请(专利权)人(译)	KINAST , ERIC KARL TELFORT 瓦列里G.		
当前申请(专利权)人(译)	Masimo公司		
[标]发明人	KINAST ERIC KARL TELFORT VALERY G		
发明人	KINAST, ERIC KARL TELFORT, VALERY G.		
IPC分类号	A61B5/021 A61B5/026 A61B5/00 A61B5/024 A61B7/00 A61B5/0285 A61B8/02 A61B7/02 A61B5/0225 A61B5/0205 A61B5/02 A61B5/0295 A61B5/0402 A61B7/04 A61B5/029 A61B5/0452 A61B5/0245 A61B5/08 A61B5/053 A61B5/1455		
CPC分类号	A61B5/02125 A61B5/02028 A61B5/0261 A61B5/0285 A61B5/0295 A61B5/02255 A61B5/02416 A61B5 /0402 A61B5/7203 A61B5/725 A61B5/7246 A61B5/7271 A61B7/00 A61B7/02 A61B7/045 A61B8/02 A61B5/0205 A61B2562/06 A61B5/024 A61B5/029 A61B5/0245 A61B5/0452 A61B5/053 A61B5/0816 A61B5/14551 A61B2560/0223 A61B2562/0204 A61B2562/04 A61B5/02405		
优先权	61/366862 2010-07-22 US 61/469511 2011-03-30 US		
其他公开文献	US20170027456A1		
外部链接	Espacenet		

摘要(译)

描述了一种用于非侵入性地确定个体血压的指示的系统。在某些实施例中，系统使用两个声学传感器计算脉搏波传播时间。该系统可包括：第一声传感器，被配置为监测对应于心室收缩和心脏舒张的患者的心音；以及第二声传感器，被配置为监测远离心脏的动脉位置处的动脉脉搏声。该系统可以有利地计算不包括射血前期间延迟的动脉脉搏波传播时间（PWTT）。在某些实施例中，该系统还包括处理器，其计算从声学传感器获得的动脉PWTT。系统可以使用该动脉PWTT来确定是否触发闭塞性袖带测量。

