



US 20190082972A1

(19) **United States**(12) **Patent Application Publication**
Tao et al.(10) **Pub. No.: US 2019/0082972 A1**(43) **Pub. Date: Mar. 21, 2019**(54) **SYSTEMS AND METHODS FOR
NON-CONTACT MONITORING OF
BALLISTOCARDIOGRAM,
PHOTOPLETHYSMOGRAM, BLOOD
PRESSURE AND ABNORMAL HEART
RHYTHM****Publication Classification**(51) **Int. Cl.***A61B 5/0205* (2006.01)*A61B 5/00* (2006.01)*A61B 5/11* (2006.01)*A61B 5/021* (2006.01)*G06T 7/20* (2006.01)(71) Applicant: **ARIZONA BOARD OF REGENTS
ON BEHALF OF ARIZONA STATE
UNIVERSITY**, Tempe, AZ (US)(72) Inventors: **Nongjian Tao**, Tempe, AZ (US);
Dangdang Shao, Tempe, AZ (US)(73) Assignee: **Arizona Board of Regents on Behalf
of Arizona State University**, Tempe,
AZ (US)(52) **U.S. Cl.**CPC *A61B 5/0205* (2013.01); *A61B 5/0077*
(2013.01); *A61B 5/02416* (2013.01); *A61B*
5/02125 (2013.01); *G06T 7/20* (2013.01);
A61B 5/1102 (2013.01)


(57)

ABSTRACT(21) Appl. No.: **16/083,052**(22) PCT Filed: **Mar. 8, 2017**(86) PCT No.: **PCT/US17/21302**

§ 371 (c)(1),

(2) Date: **Sep. 7, 2018****Related U.S. Application Data**(60) Provisional application No. 62/307,064, filed on Mar.
11, 2016.

Various embodiments of systems and methods for tracking ballistocardiogram, photoplethysmogram, blood pressure and abnormal heart rhythm based on optical imaging of a human body are disclosed. Ballistocardiogram and photoplethysmogram signals from a similar region of the human body are simultaneously obtained, and the time delay between the two signals is used to determine the blood pressure of the subject, together with other physiological parameters of the subject, including gender, age, weight, height, heart rate, stroke volume, blood pressure and abnormal heart rhythm obtained using other methods.

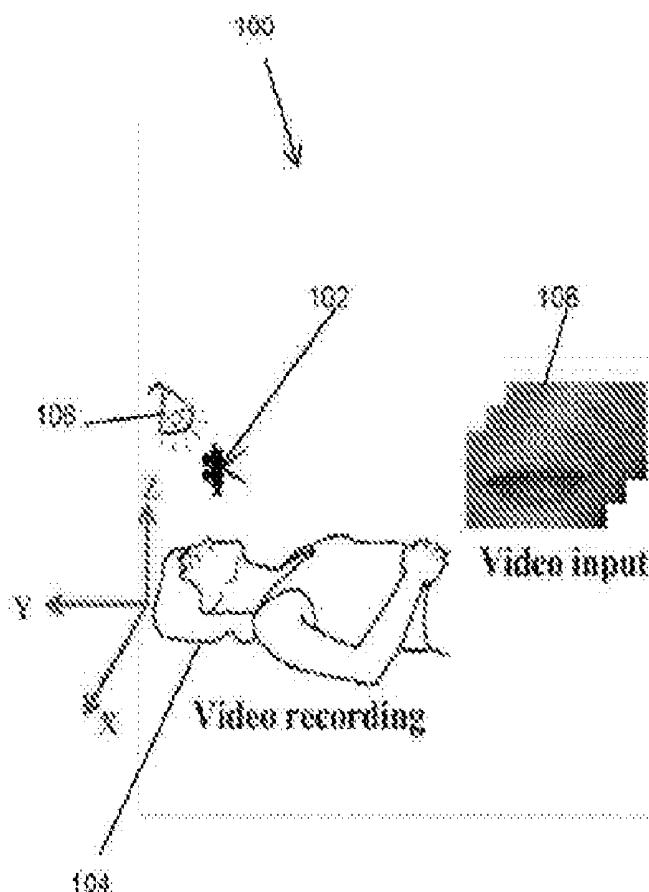

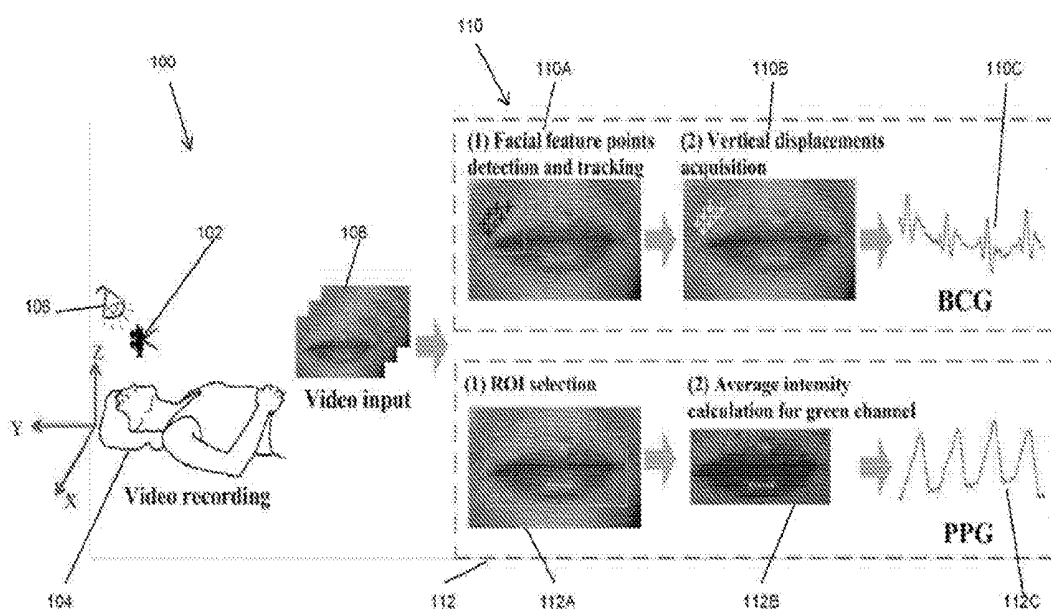


FIG. 1A

FIG. 1B

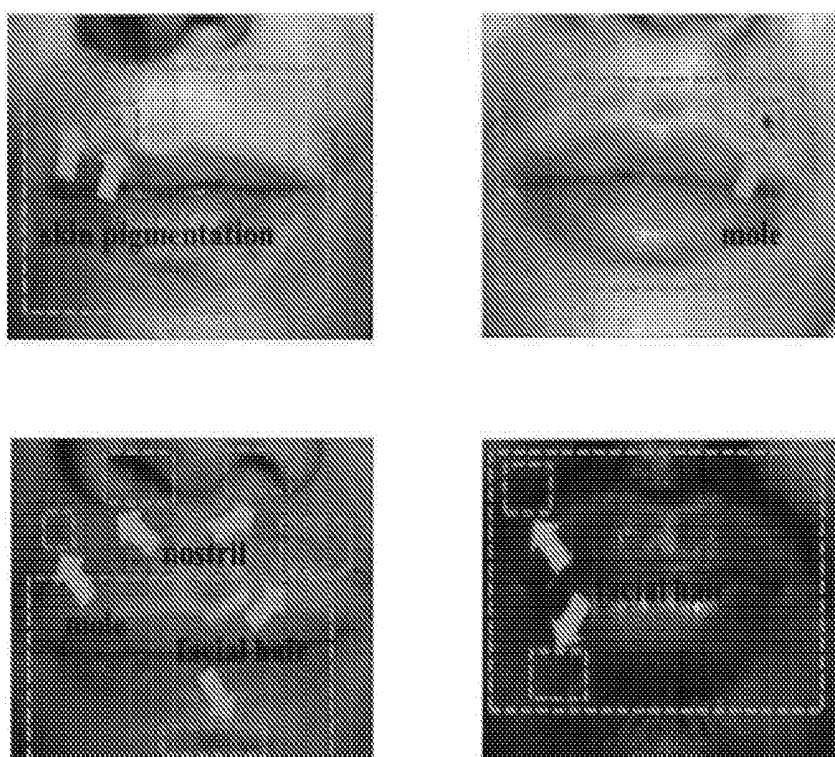


FIG. 1C

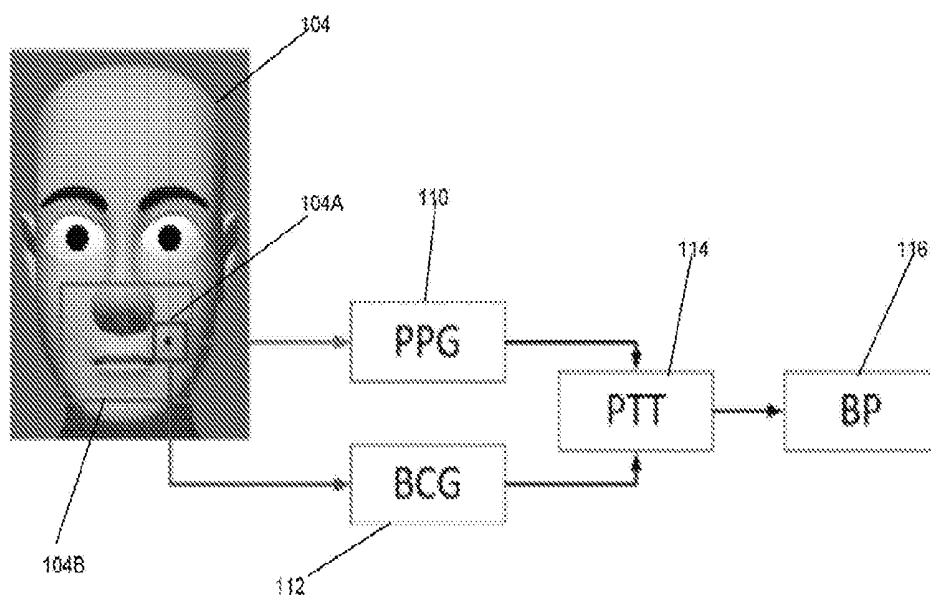


FIG. 2

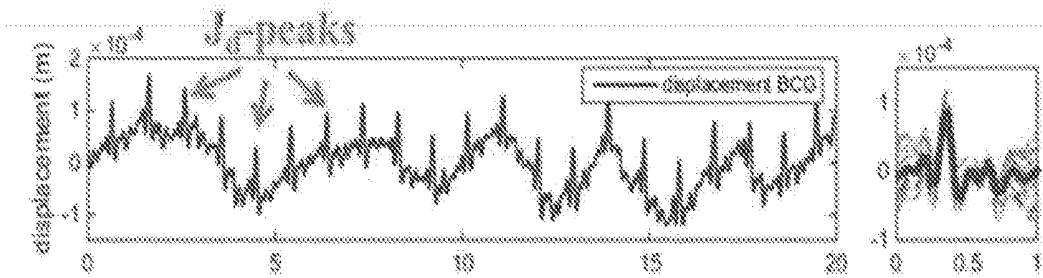


FIG. 3A

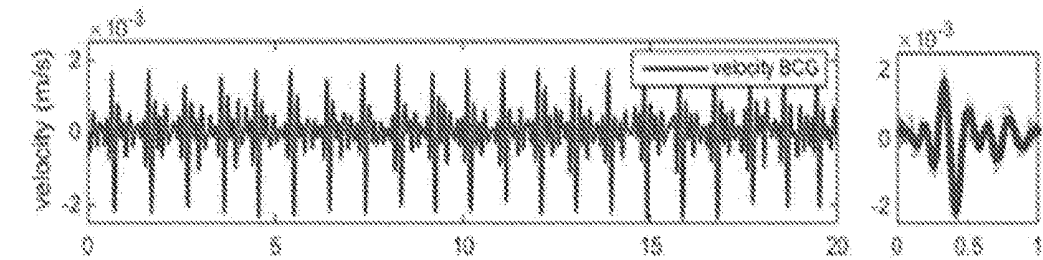


FIG. 3B

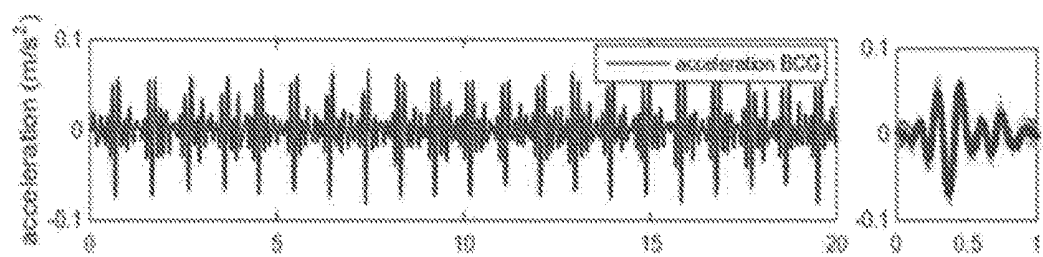


FIG. 3C

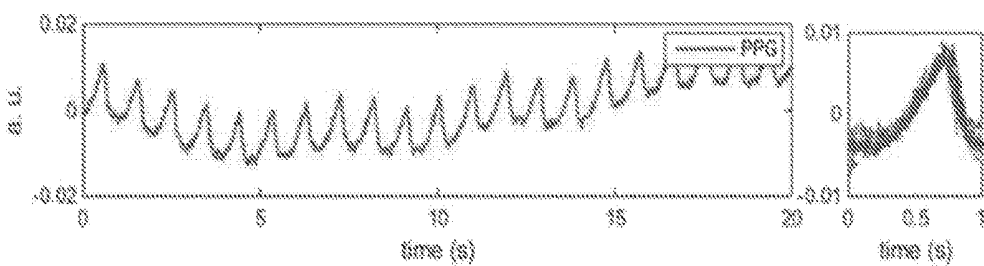


FIG. 3D

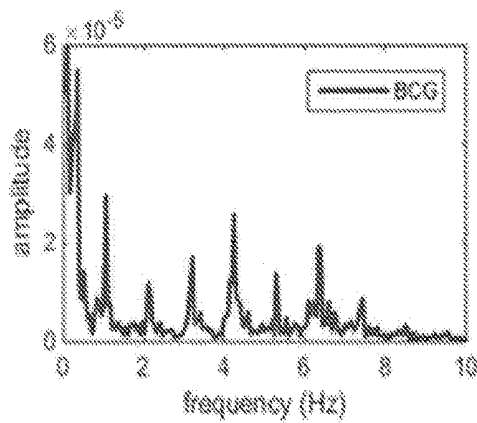


FIG. 3E

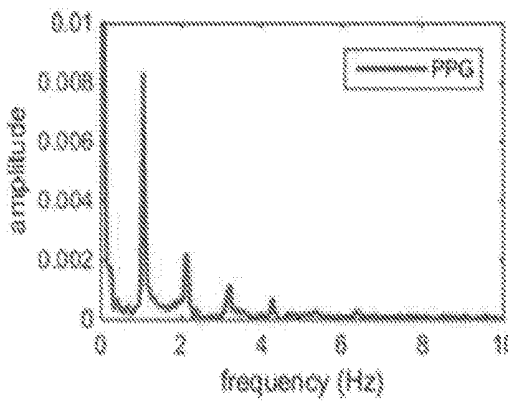


FIG. 3F

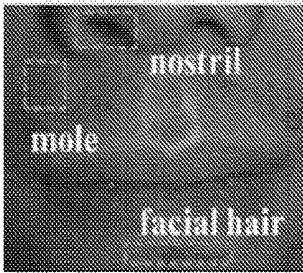


FIG. 4A

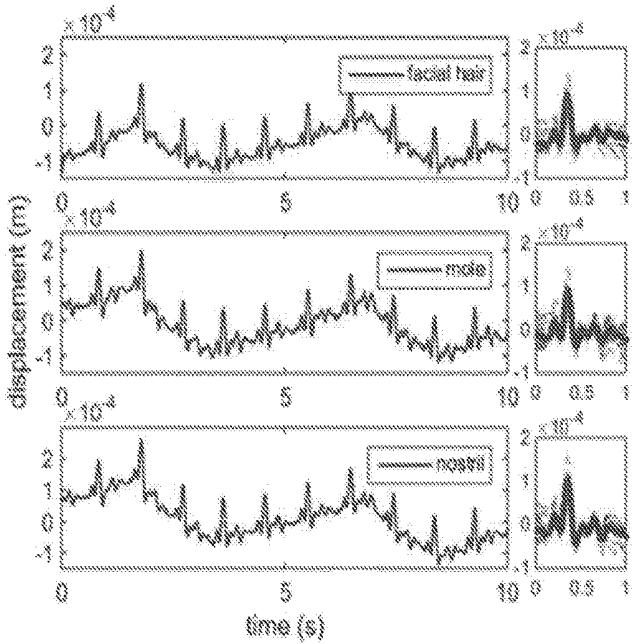


FIG. 4B

FIG. 4C

FIG. 4D

FIG. 5A

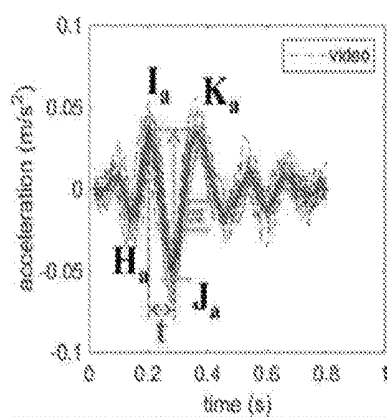


FIG. 5B

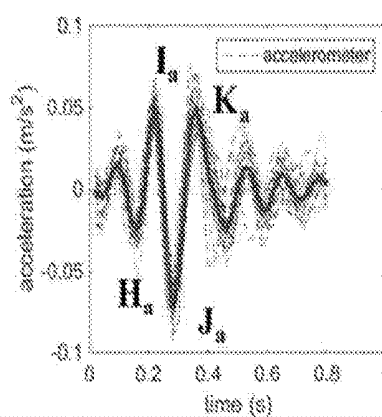


FIG. 5C

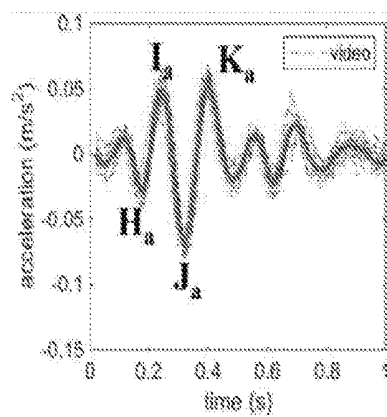
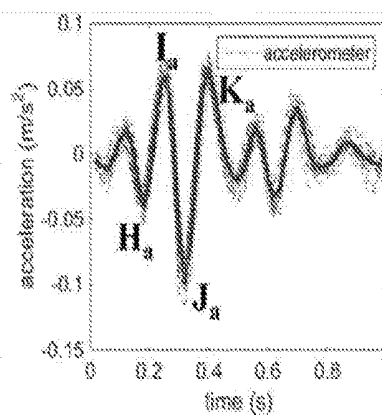


FIG. 5D



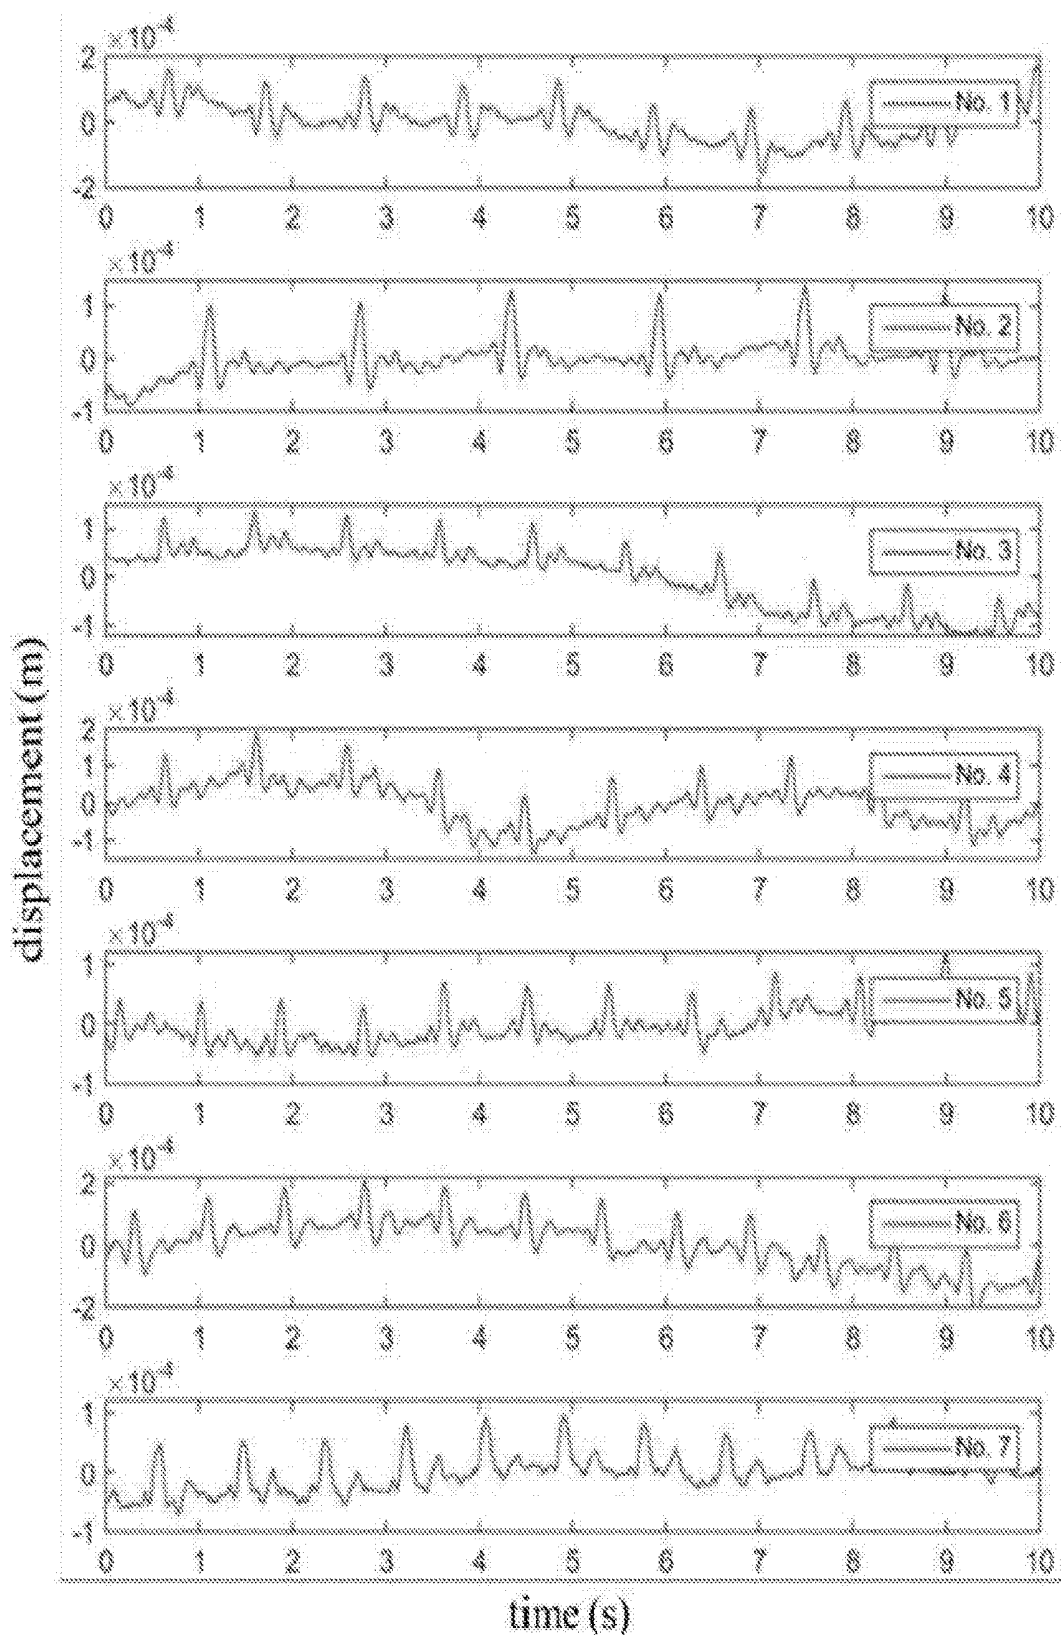


FIG. 6

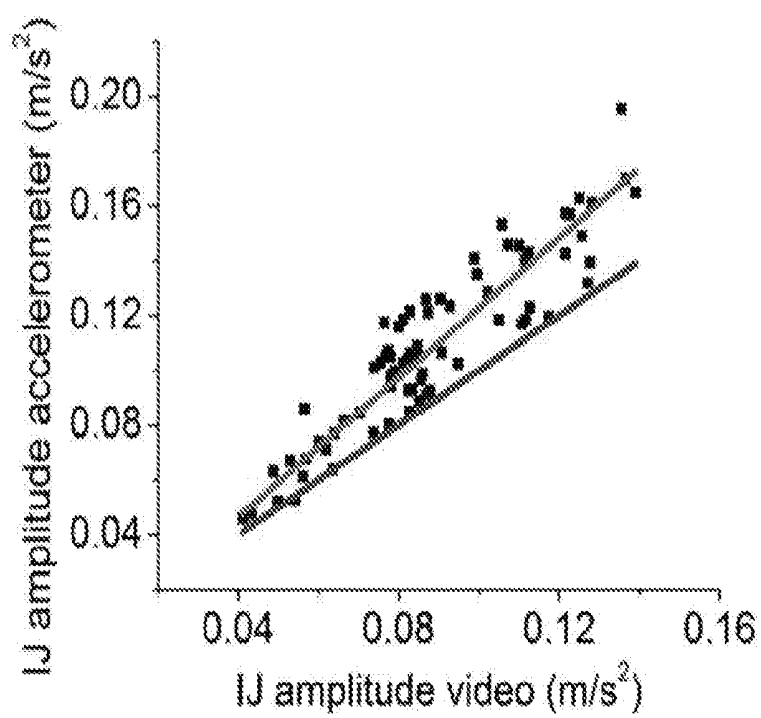


FIG. 7

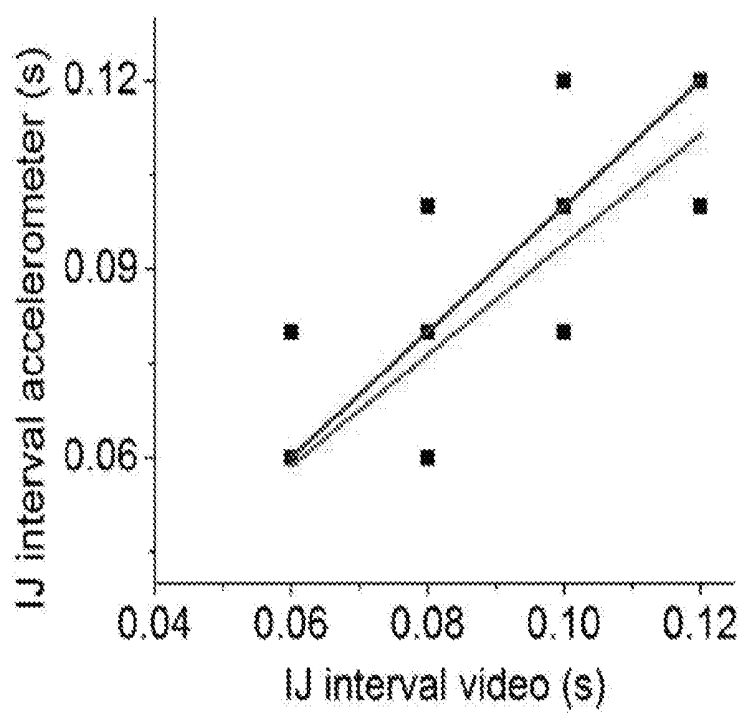


FIG. 8

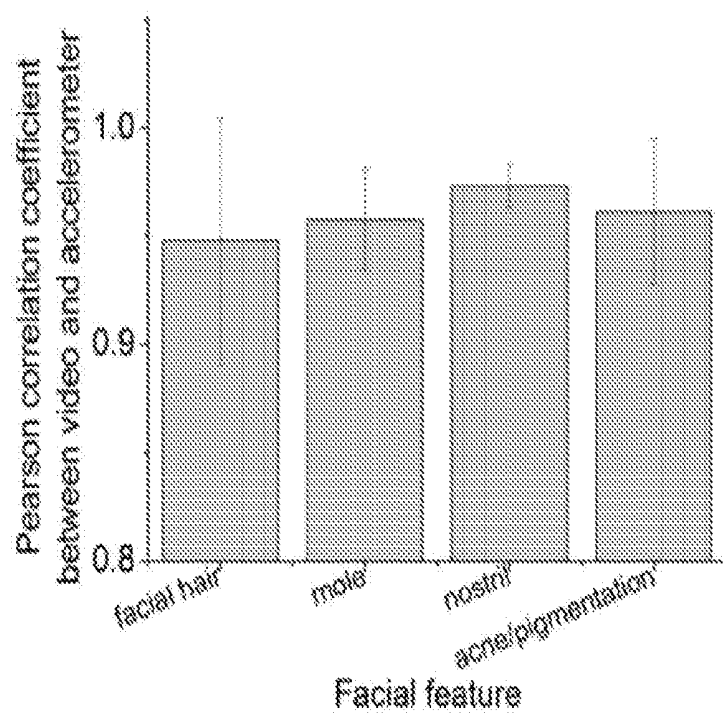


FIG. 9

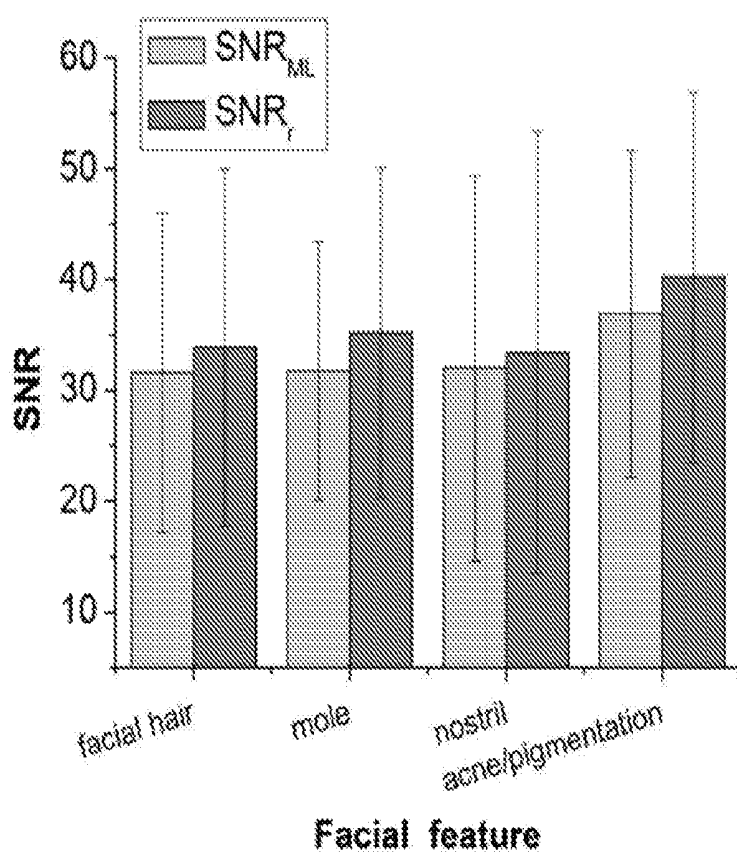


FIG. 10

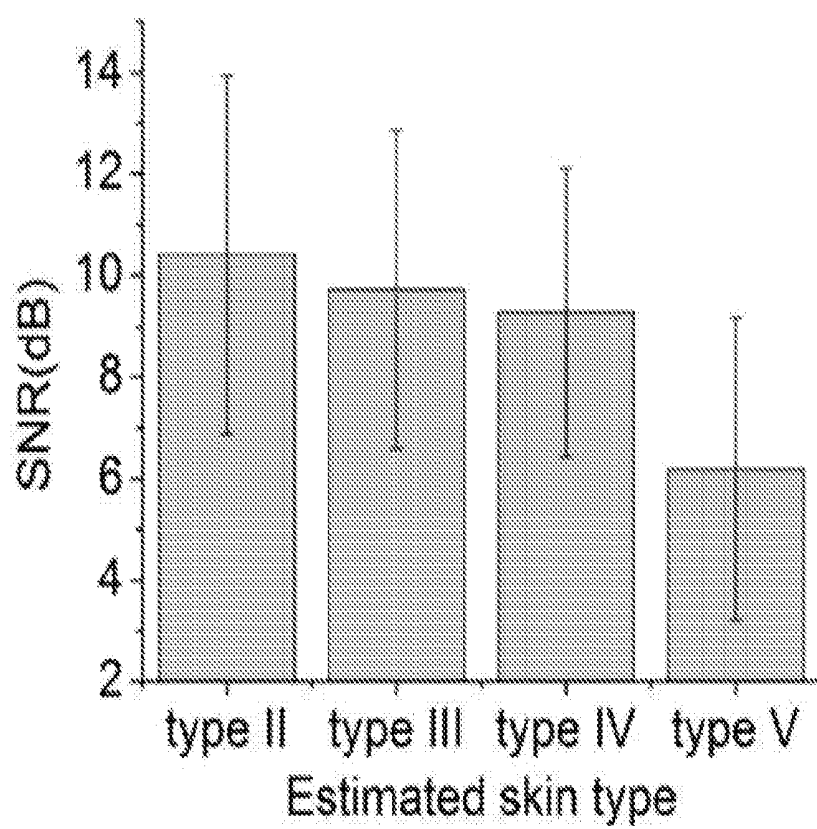


FIG. 11

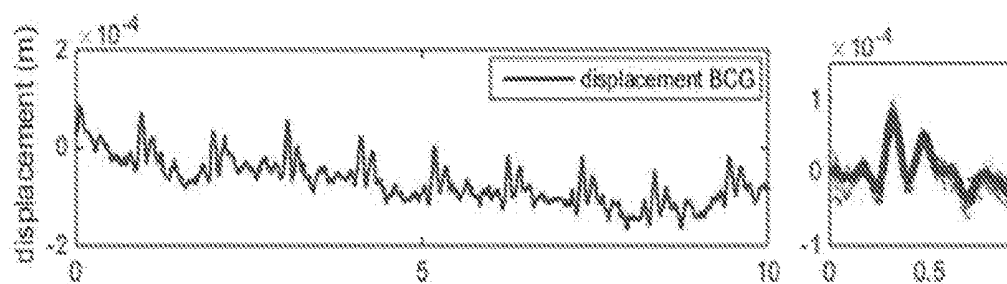


FIG. 12A

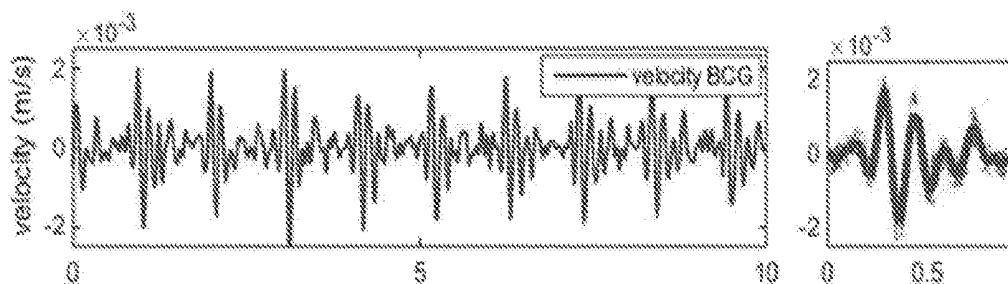


FIG. 12B

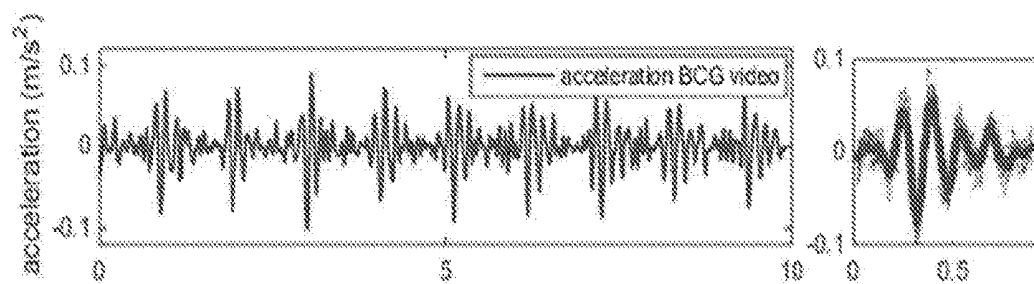


FIG. 12C

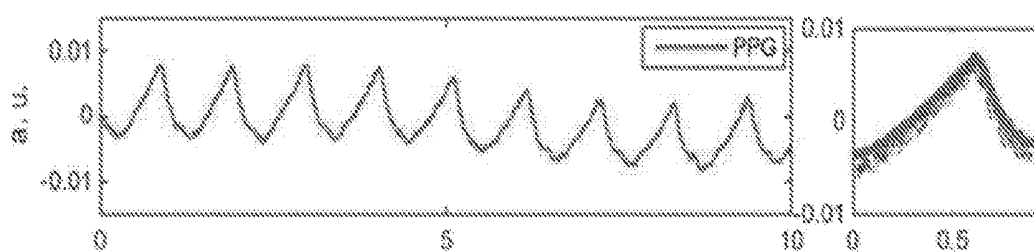


FIG. 12D

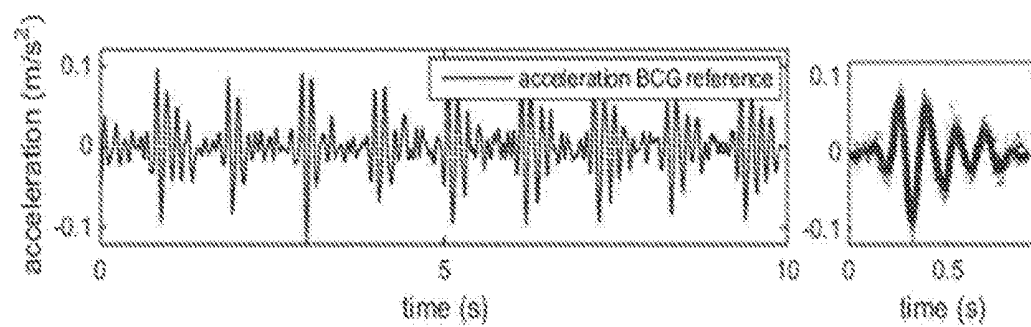


FIG. 12E

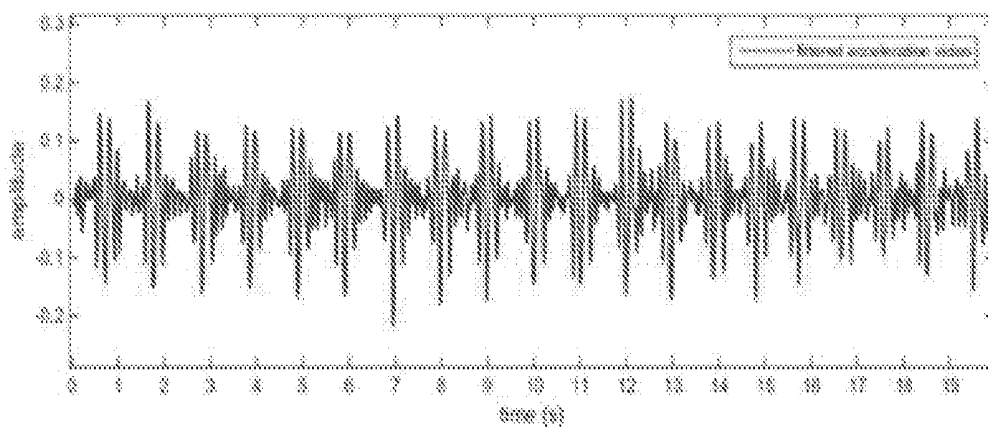


FIG. 13A

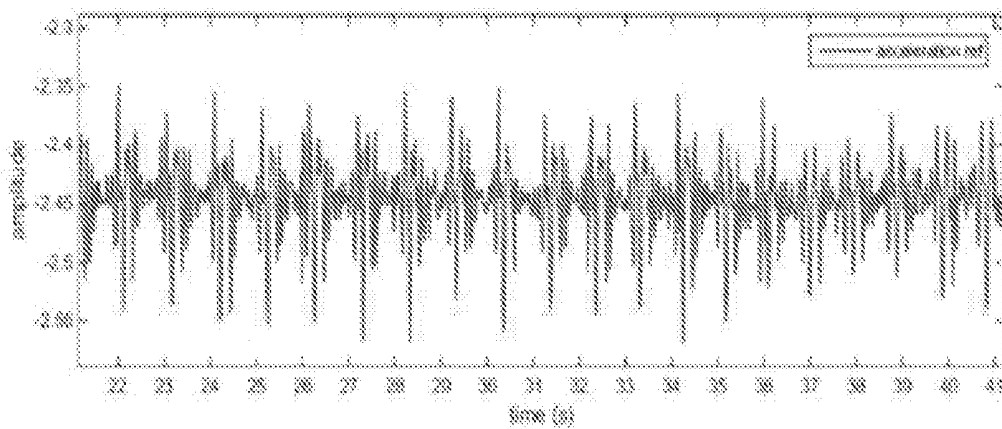


FIG. 13B

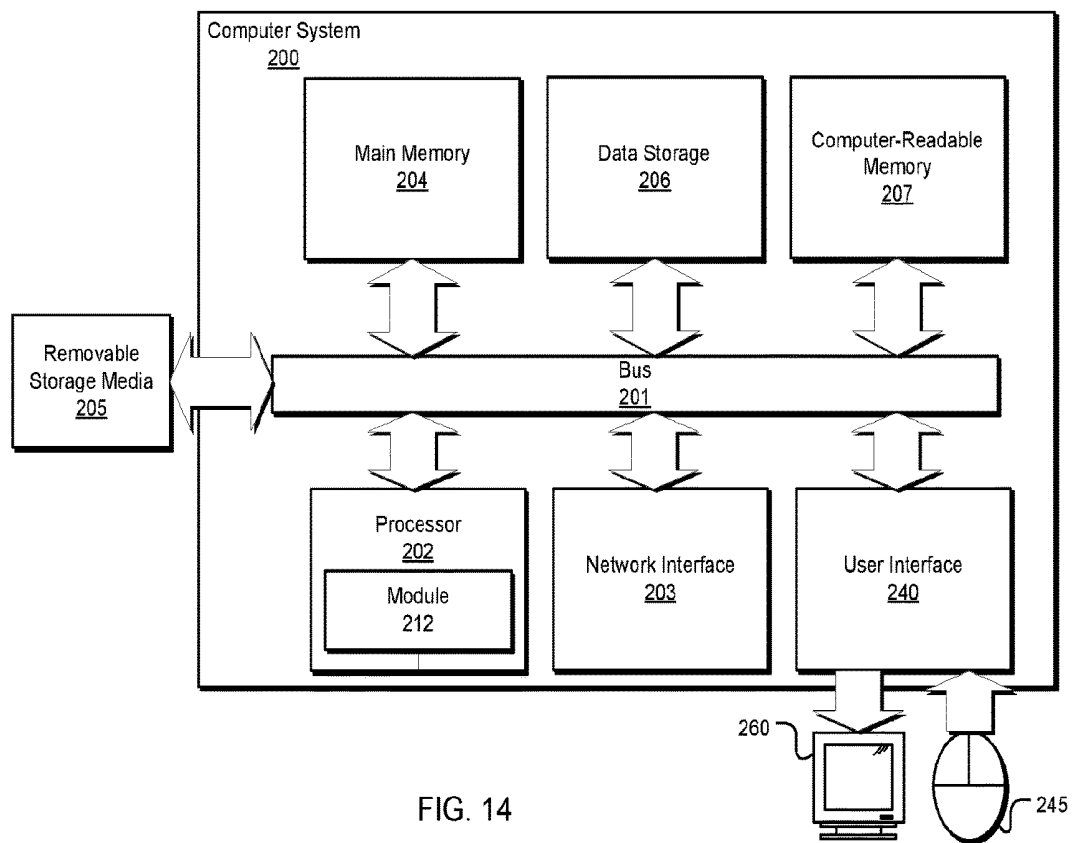


FIG. 14

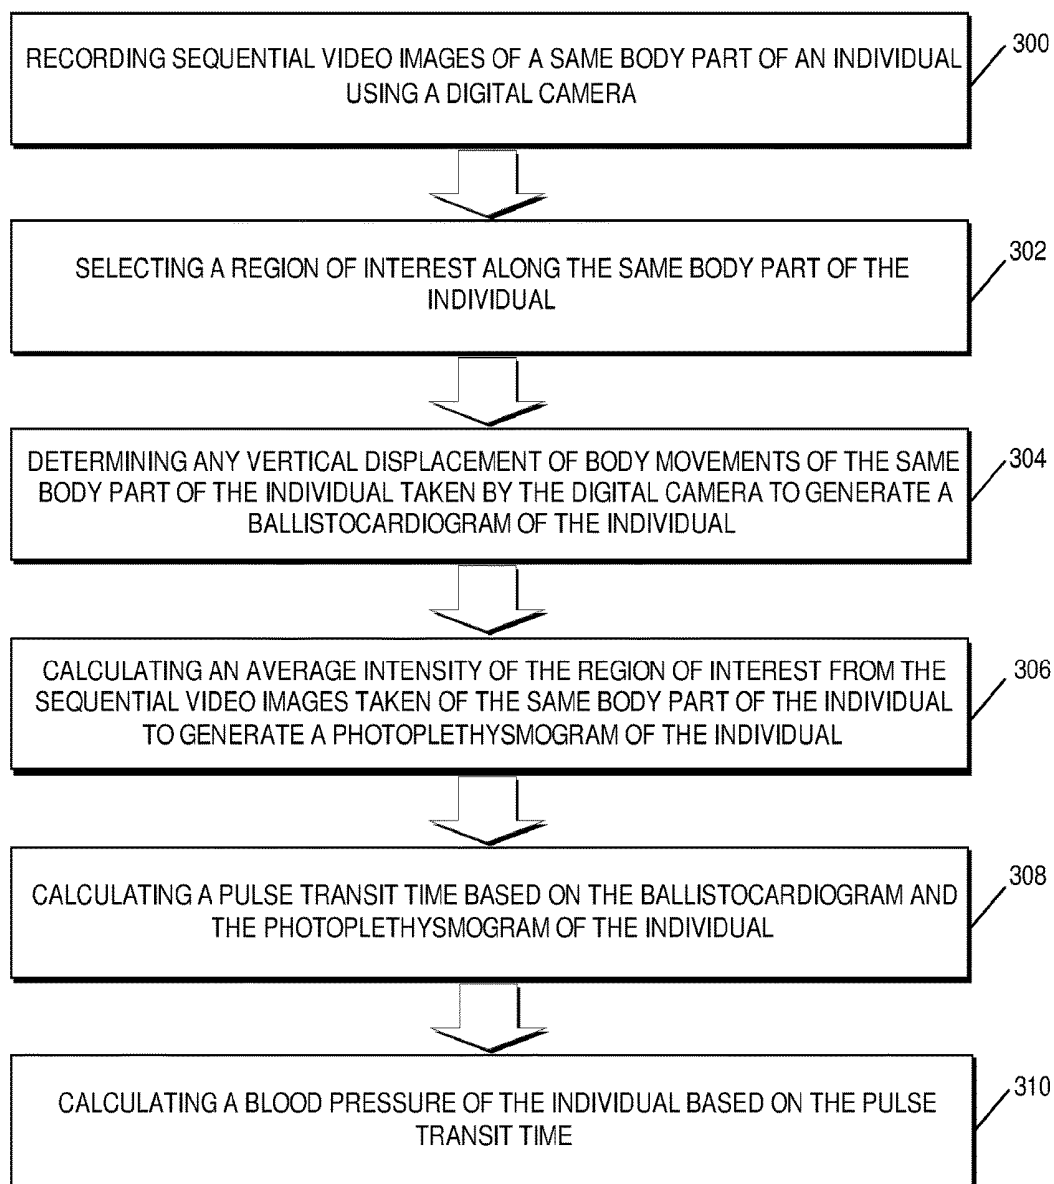


FIG. 15

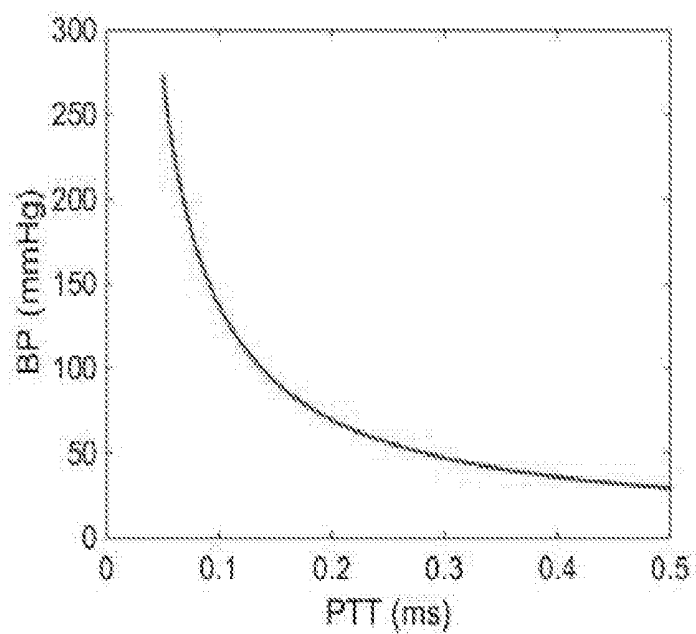


FIG. 16

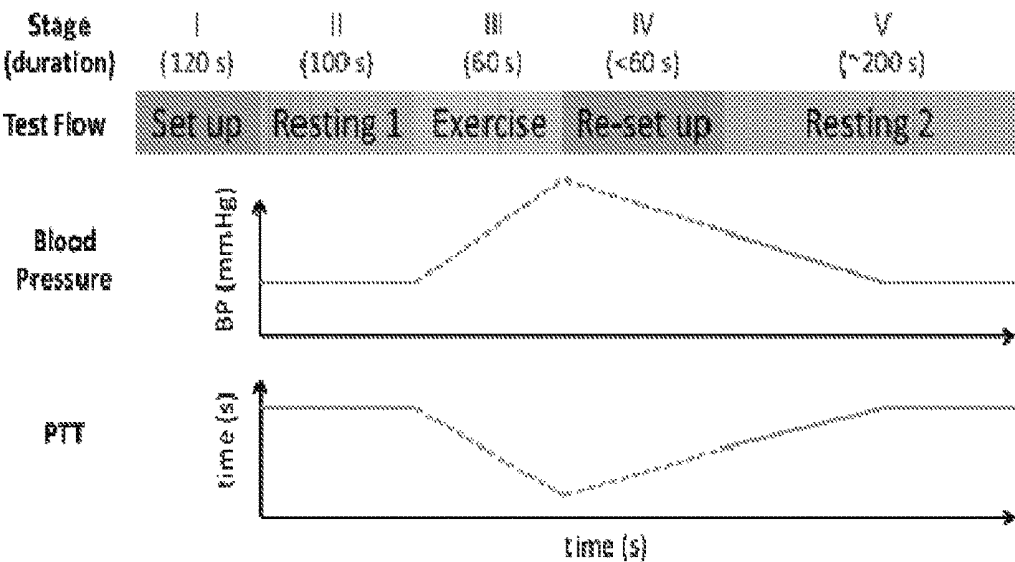
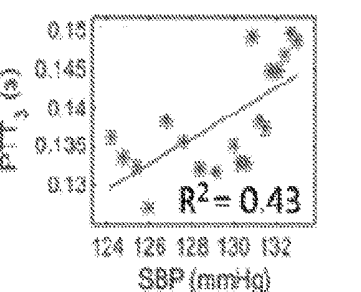
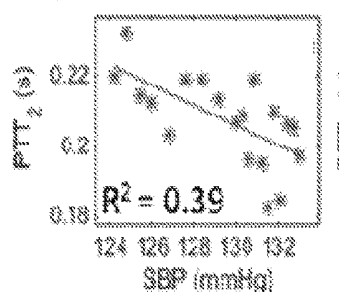
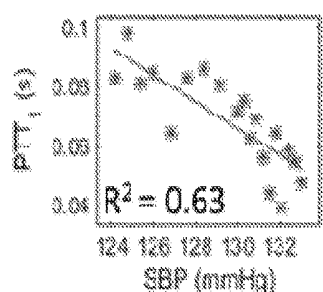
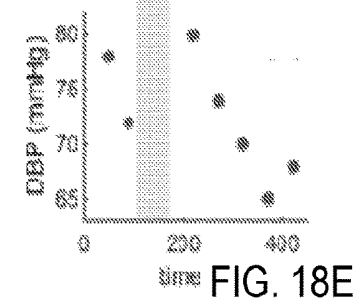
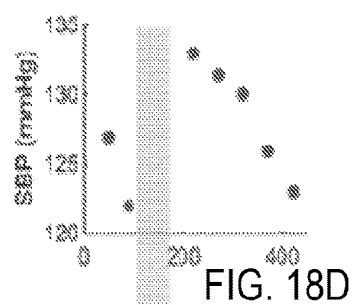
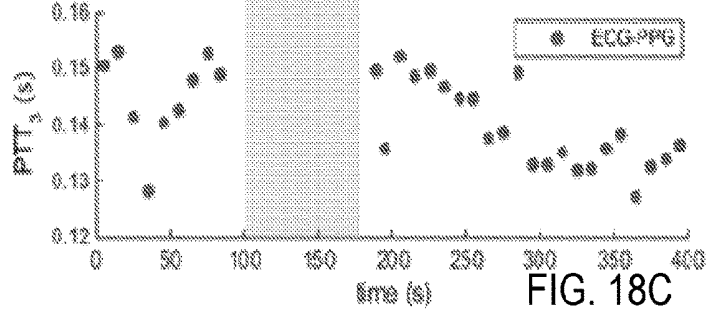
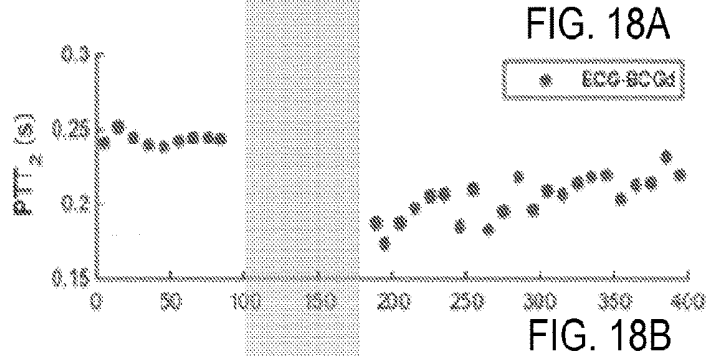
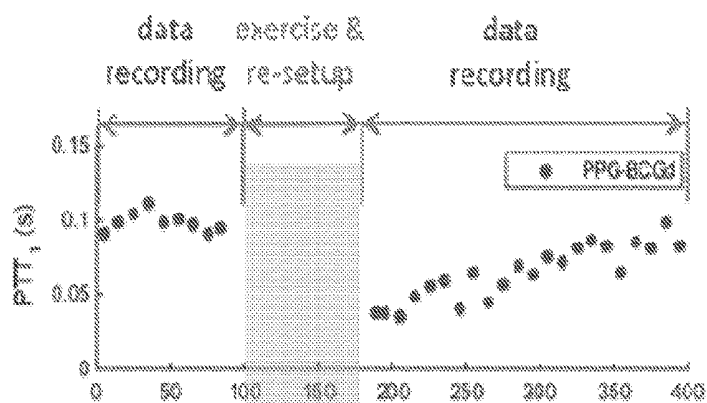
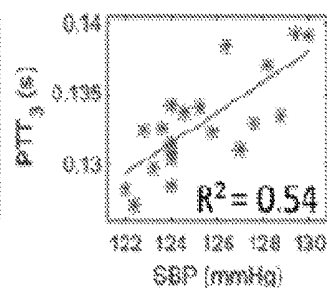
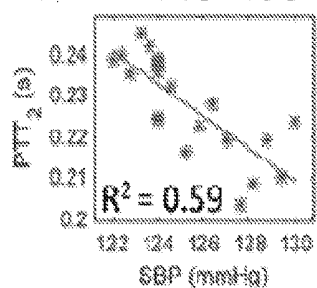
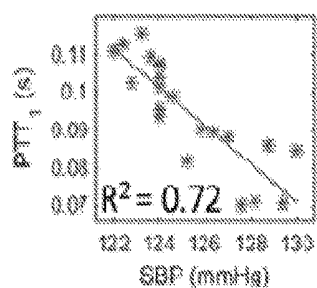
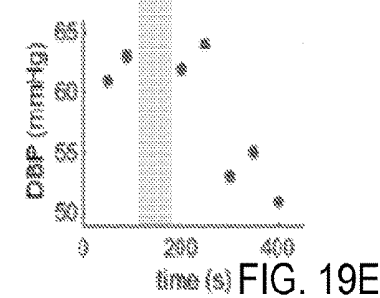
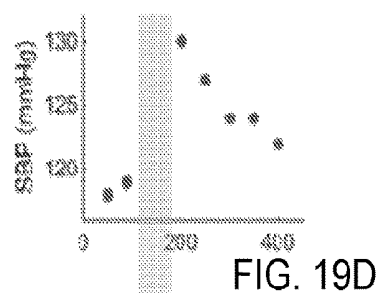
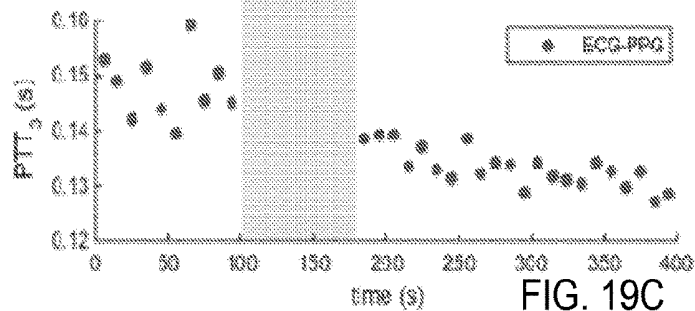
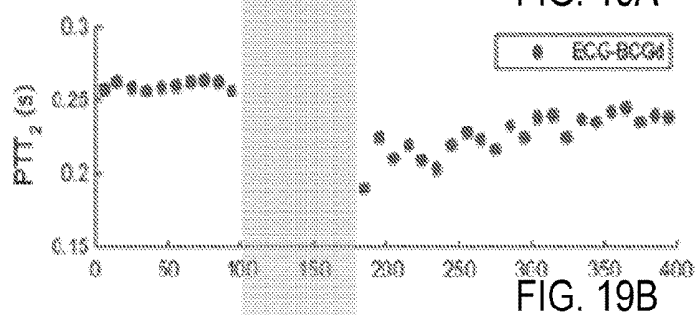
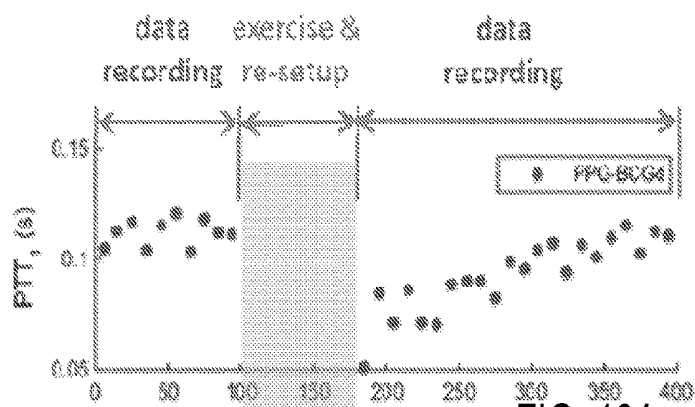
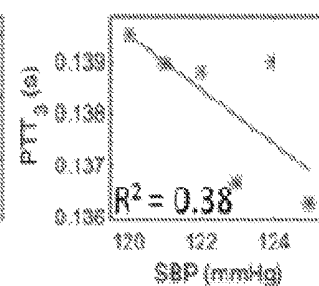
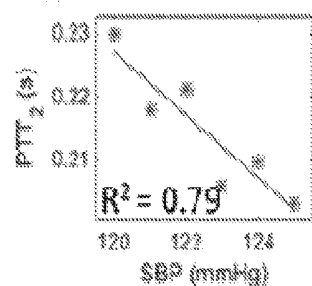
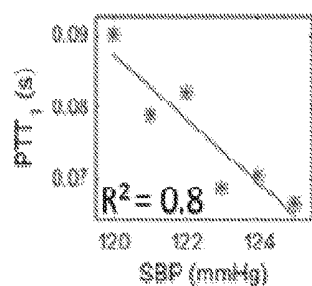
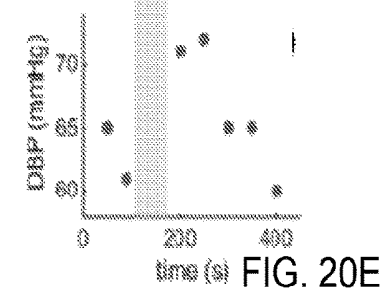
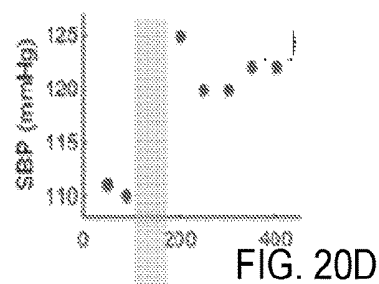
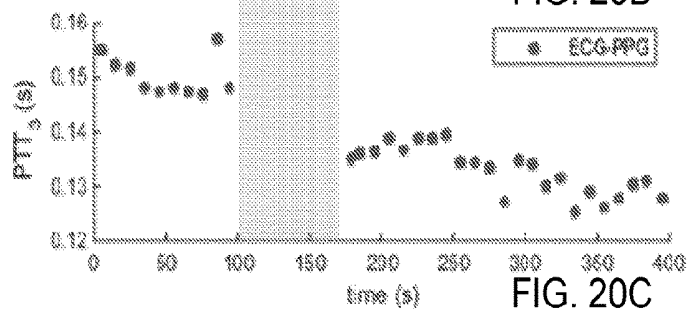
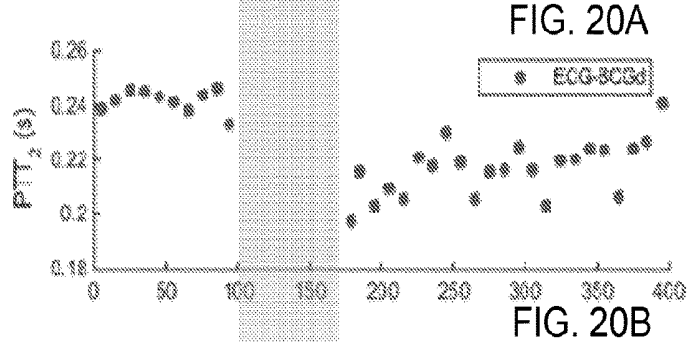
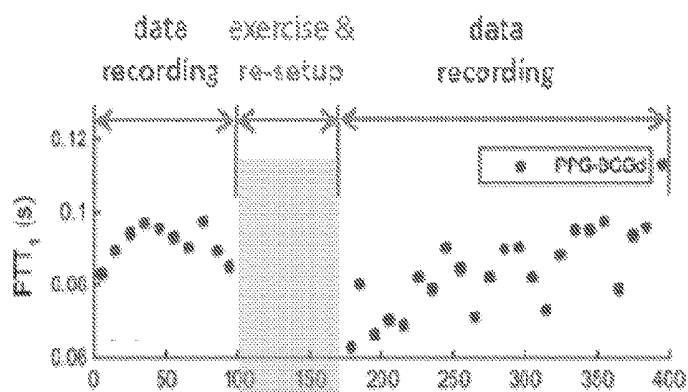


FIG. 17







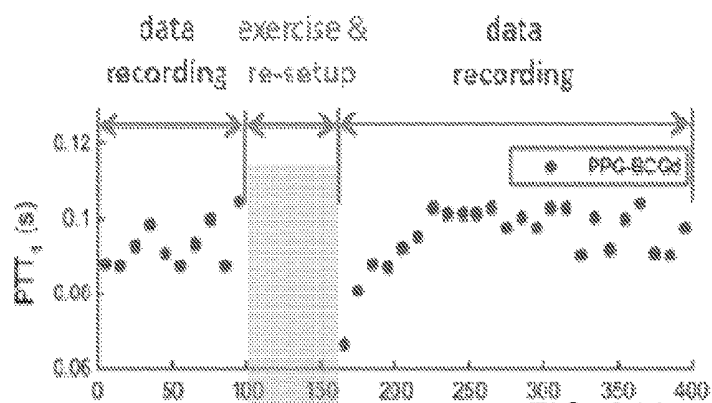


FIG. 21A

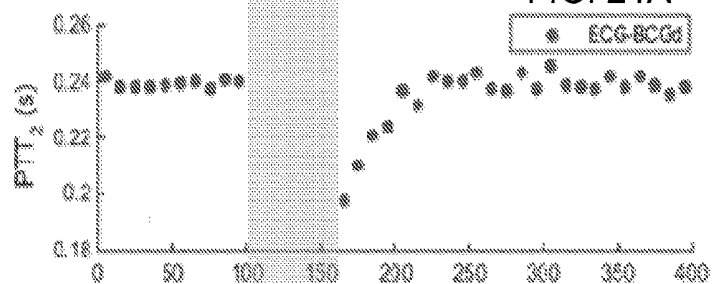


FIG. 21B

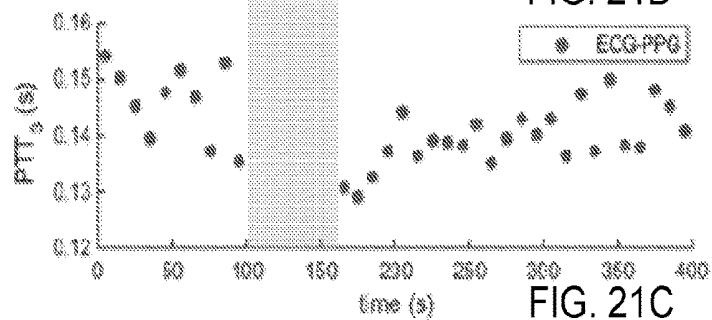


FIG. 21C

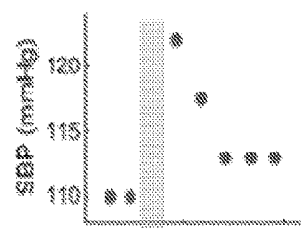


FIG. 21D

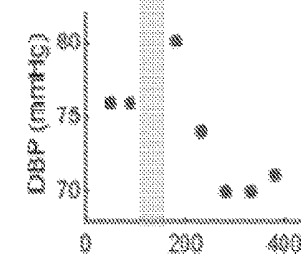


FIG. 21E

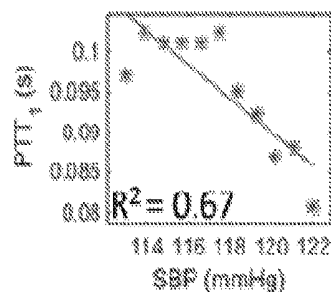


FIG. 21F

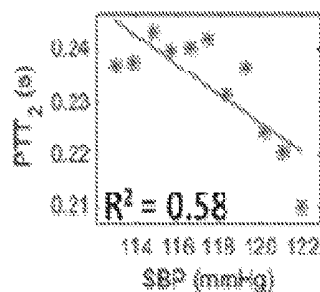


FIG. 21G

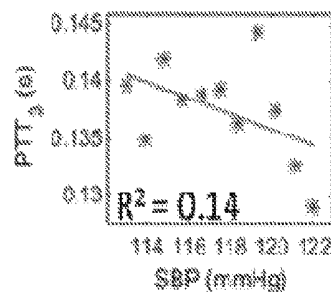


FIG. 21H

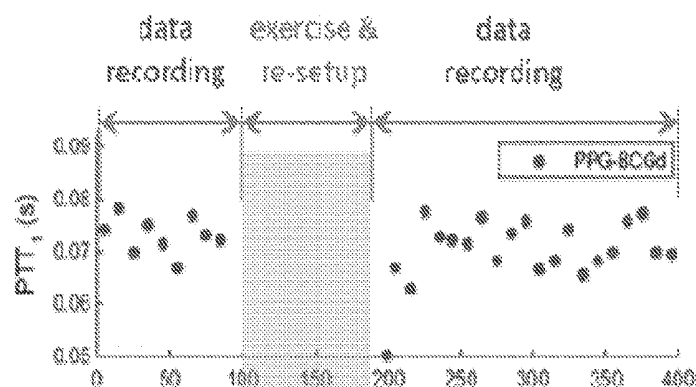


FIG. 22A

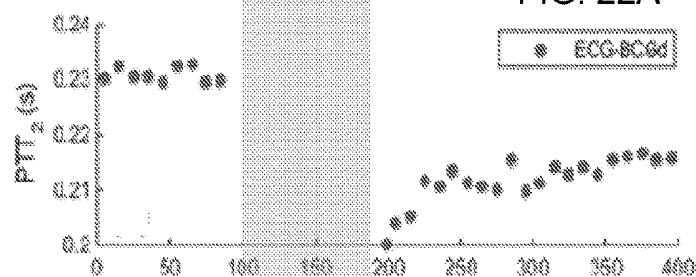


FIG. 22B

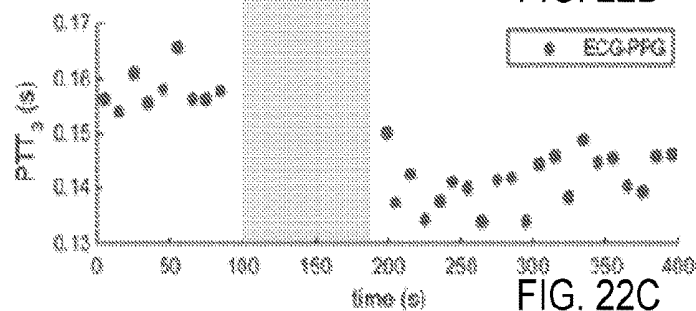


FIG. 22C




FIG. 22D

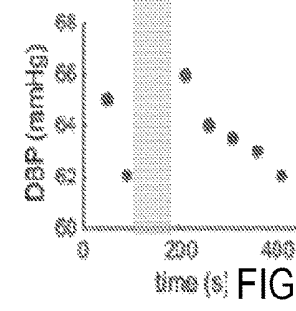


FIG. 22E

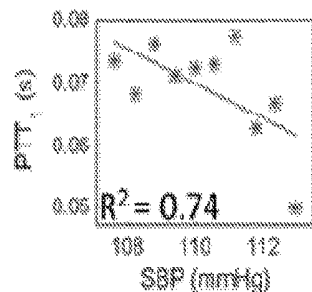


FIG. 22F

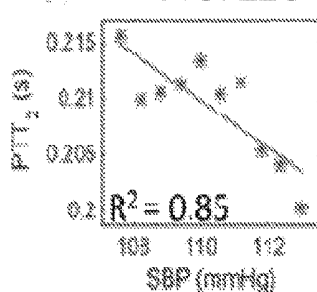


FIG. 22G

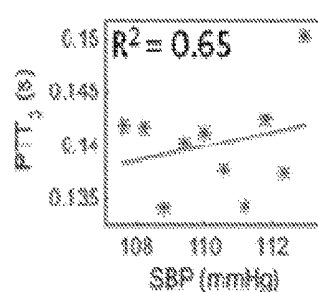


FIG. 22H

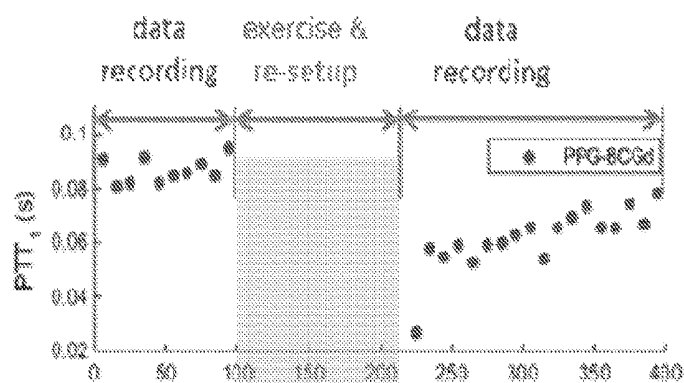


FIG. 23A

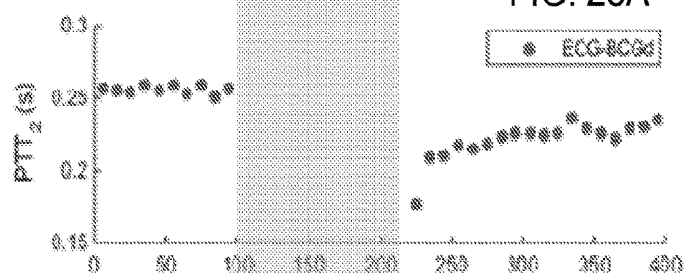


FIG. 23B

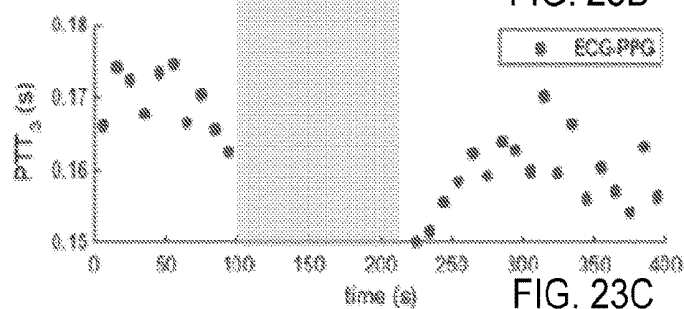


FIG. 23C

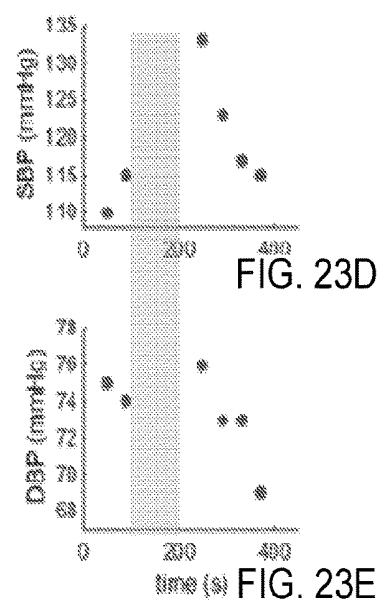


FIG. 23D

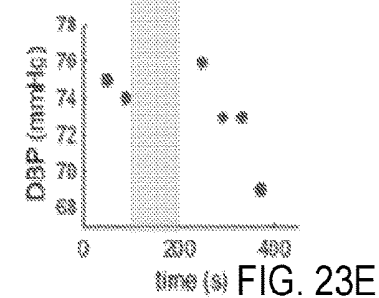


FIG. 23E

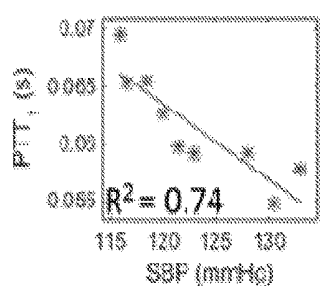


FIG. 23F

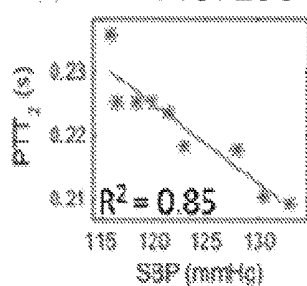


FIG. 23G









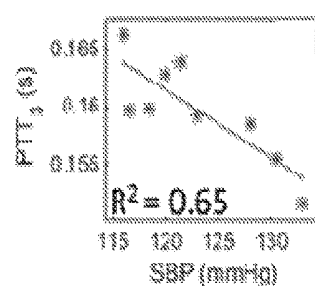


FIG. 23H

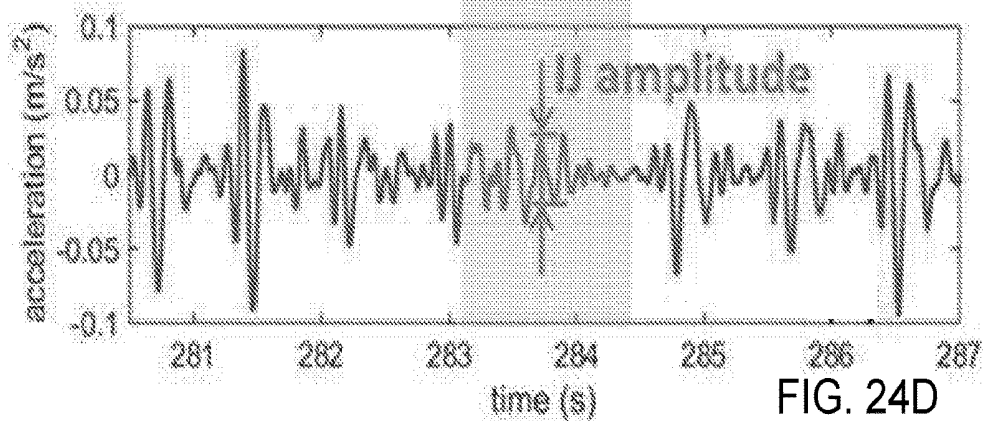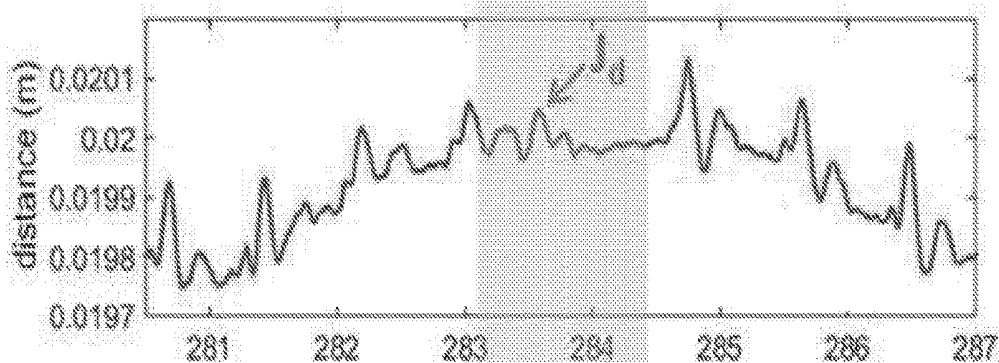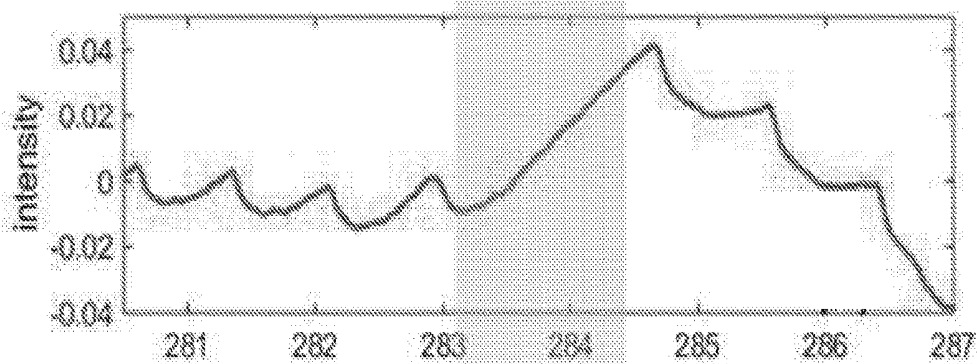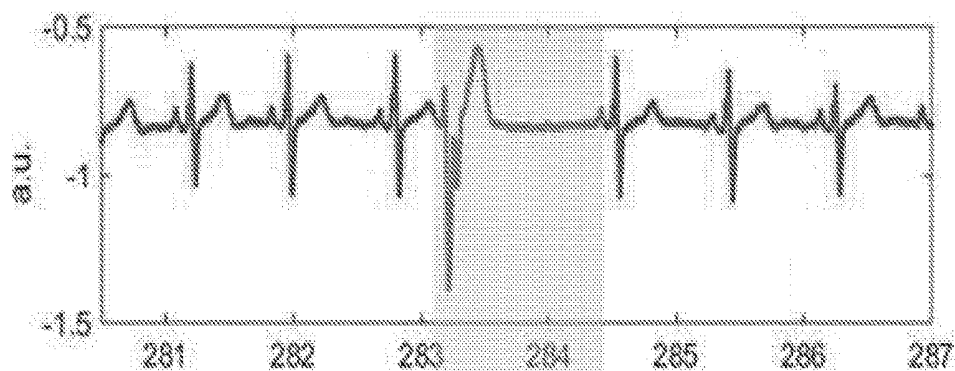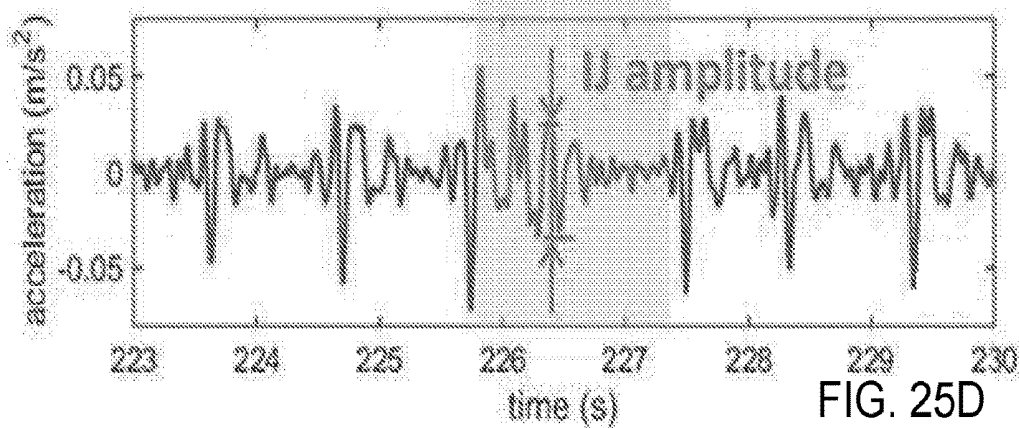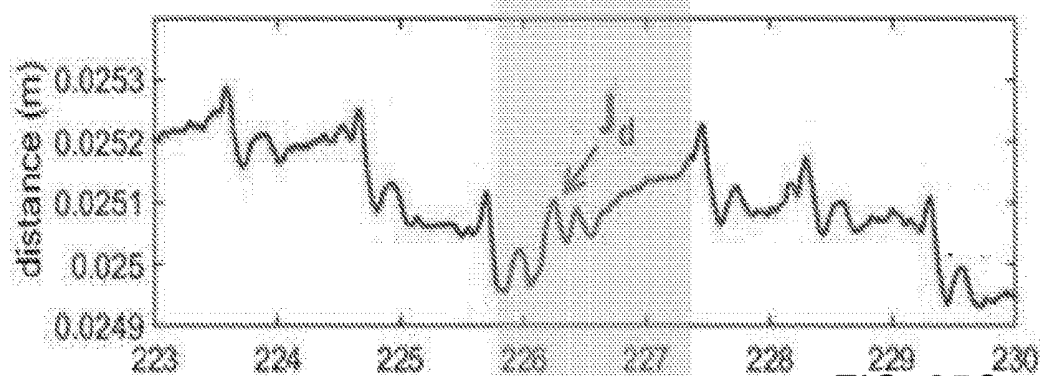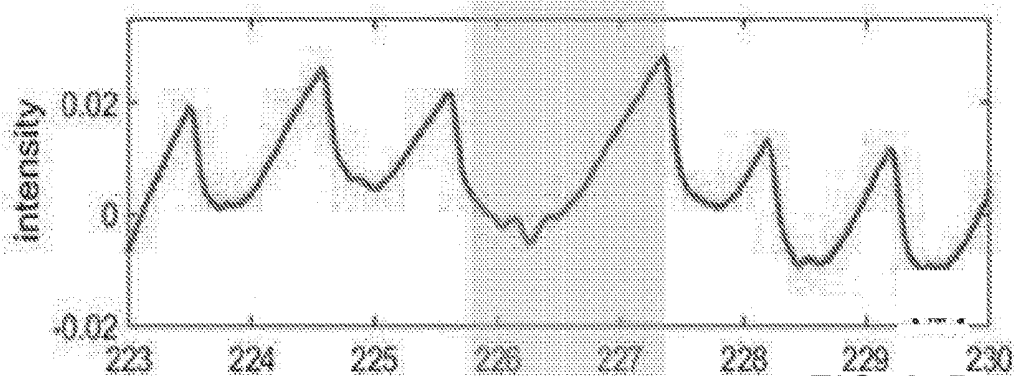

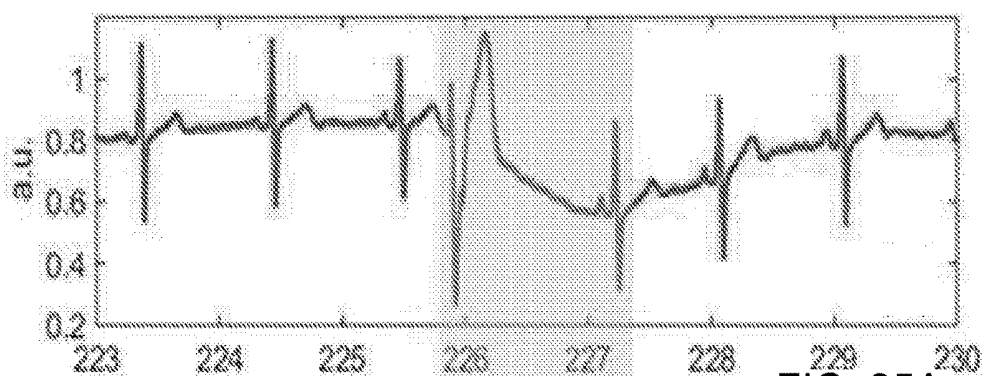

SYSTEMS AND METHODS FOR NON-CONTACT MONITORING OF BALLISTOCARDIOGRAM, PHOTOPLETHYSMOGRAM, BLOOD PRESSURE AND ABNORMAL HEART RHYTHM

FIELD

[0001] The present disclosure generally relates generally to non-contact and non-invasive monitoring of a subject individual, and in particular to non-contact and non-invasive monitoring of physiological parameters of the subject individual such as ballistocardiogram, photoplethysmogram, pulse transit time, and blood pressure.

BACKGROUND

[0002] Ballistocardiogram (BCG) refers to the repetitive body motion generated by cardiac contraction and ejection of blood during cardiac cycles. BCG can be determined from the displacement, velocity or acceleration of body parts, such as head and legs of an individual.

[0003] BCG includes important features with physiological relevance, and can be used for idiopathic hypertrophic subaortic stenosis diagnose and early detection of coronary heart disease. For example, the “IJ wave” is a well-accepted method to measure atrial ejection force associated with BCG.

[0004] The traditional method to measure BCG is based on a mechanical system, such as a suspended bed, or a suspended rigid platform. Electro kinetic devices based on electrochemical principle to measure BCG are known, but such traditional equipment used in these BCG measurement methods are bulky and complicated, compared with other medical procedures, such as electrocardiography (ECG). As a result, the development and utilization of BCG in health and medical applications has been slow.

[0005] Since 2000, with the development of the new sensor technology, BCG has attracted interest again. A research team has developed an ear-worm device that can monitor ECG, BCG and PPG signals together. The BCG signal is obtained from an accelerometer integrated in the device. Other researchers have used a weighing scale installed with a force or pressure sensor to monitor BCG signals, while other researchers have used a polypropylene film coated with electrically conductive layers to measure BCG. However, these aforementioned methods require direct contact of the BCG device with the subject body.

[0006] Using a non-contact method to monitor BCG signal has not been well established. Other researchers have reported a method to detect heart rate by tracking the vertical movement of head, but this method does not provide a BCG waveform. In addition, other researchers have used a camera with an MPT marker attached to a user's nasal bridge to track the head movement induced by BCG. Unfortunately, attaching a marker to a person's nose is not practical or at least not desirable. Furthermore, this method also requires that subject to wear a head coil fixated with a cushion to avoid motion artifacts.

[0007] Blood pressure is a critical vital sign, which is measured currently with an inflatable cuff; however, the use of an inflatable cuff is inconvenient and also makes it hard to continuously monitor a subject's blood pressure. Different approaches have been attempted to develop cuffless blood

pressure measurement. MEMS devices, such as an accelerometer and a conducting polymer actuator, have been used for this purpose. Optical methods based on pulse transit time (PTT) have also been used to infer blood pressure values. PTT is the time required for a pulse signal to travel from one part of the body to another. Most published PTT-based blood pressure monitoring research has focused on the time difference between ECG and photoplethysmogram (PPG) signals. Other researchers have presented a method to monitor blood pressure based on BCG obtained from a microbending fiber sensor, and PPG obtained from a contact-based finger probe. One study used a weighting scale to measure BCG and ECG, and showed that the time interval between these two signals was strongly correlated to cardiac pre-ejection period. These studies suggest that BCG is potentially an alternative to ECG for measuring PTT, and blood pressure, but they all require wearing or using one or more multiple devices in contact with the subject body.

[0008] There are also reports on non-contact or imaging-based measurement of PTT based on PPG signals at two different body parts. One study used one camera to record PPT between a subject's face and hand. Another study used one camera to capture blood volume pulses from a subject's face, hand or foot, to extract the corresponding PTT, while another study disclosed the use of the front and back cameras of a smartphone to determine PTT. These conventional systems all require measuring PPG signals from two different body parts. To achieve good accuracy, the two body parts are preferably well separated by a distance, which requires clear imaging of the two body parts; however, this requirement makes it hard to accomplish such clear imaging with a single camera. For example, in one study, the subject must place his/her hand close to the face so that both the hand and face can be clearly imaged. Traditional methods detect premature ventricular contraction (PVC) through ECG measurement to find abnormal heartbeat based on contract-based approach. The electrodes used in ECG are attached to patents' chest directly, which may cause discomfort and skin rashes. Based on the foregoing, there is a need for systems and methods for better non-contact monitoring to determine BCG, PPG, PTT blood pressure and abnormal heart rhythm of a subject individual.

BRIEF DESCRIPTION OF THE DRAWINGS

[0009] FIG. 1A is a schematic illustration showing one setup of a non-contact monitoring system for determining BCG and PPG; FIG. 1B is a simplified illustration showing the video input analysis used by the non-contact monitoring system to determine BCG and PPG according to one embodiment; and FIG. 1C are images showing regions of interest for BCG (green rectangles) and PPG (blue rectangles) acquisitions, according to one aspect of the present disclosure;

[0010] FIG. 2 is a simplified illustration showing one method for non-contact monitoring of blood pressure based on the simultaneous monitoring of BCG and PPG taken from one region of an individual according to one embodiment, according to one aspect of the present disclosure;

[0011] FIG. 3A-3F are graphical representations of detected signals with corresponding ensemble averages for displacement BCG, velocity BCG, acceleration BCG, PPG, displacement BCG frequency spectrum, and PPG frequency spectrum, according to one aspect of the present disclosure;

[0012] FIGS. 4A-4D are graphical representations of BCG waveforms detected from different facial features with corresponding ensemble averages, according to one aspect of the present disclosure;

[0013] FIGS. 5A-5D are graphical representations showing the comparison of acceleration BCG waveforms obtained with the non-contact monitoring system, according to one aspect of the present disclosure;

[0014] FIG. 6 is a graphical representation of displacement BCGs obtained from different subjects, according to one aspect of the present disclosure;

[0015] FIG. 7 is a graphical representation of the correlation between the IJ amplitudes of BCGs obtained using the non-contact monitoring system, according to one aspect of the present disclosure;

[0016] FIG. 8 is a graphical representation of the correlation between the IJ intervals of acceleration BCGs obtained using the non-contact monitoring system, according to one aspect of the present disclosure;

[0017] FIG. 9 is a graphical representation of the Pearson correlation coefficients between the non-contact monitoring system and the reference device with different facial features, according to one aspect of the present disclosure;

[0018] FIG. 10 is a graphical representation of the SNR estimation of BCG using the non-contact monitoring system, with standard deviation, based on the maximum likelihood (SNR_{ML}) and sample correlation coefficient (SNR_r), according to one aspect of the present disclosure;

[0019] FIG. 11 is a graphical representation of SNR of PPG from different skin categories with standard deviation, according to one aspect of the present disclosure;

[0020] FIGS. 12A-12E are graphical representations of detected signals with corresponding ensemble averages for displacement BCG, velocity BCG, acceleration BCG, PPG from video-based method, PPG, and acceleration BCG from a reference device when the subject is at a sitting position, according to one aspect of the present disclosure;

[0021] FIGS. 13A and 13B are graphs showing a comparison of BCG detection from a video-based method and an accelerometer-based method according to one embodiment;

[0022] FIG. 14 is a simplified block diagram that illustrates the hardware and software components of the non-contact monitoring system according to one embodiment; and

[0023] FIG. 15 is a flow chart illustrating a method for determining BCG and PPG using the non-contact monitoring system according to one embodiment.

[0024] FIG. 16 shows the relationship between PTT and blood pressure, according to one aspect of the present disclosure;

[0025] FIG. 17 is a graphical representation showing the experiment workflow and estimated changes in blood pressure and PTT, according to one aspect of the present disclosure;

[0026] FIGS. 18A-18H are graphical representations showing PTTs and blood pressure results and correlations from subject number one, according to one aspect of the present disclosure;

[0027] FIGS. 19A-19H are graphical representations showing PTTs and blood pressure results and correlations from subject number two, according to one aspect of the present disclosure;

[0028] FIGS. 20A-20H are graphical representations showing PTTs and blood pressure results and correlations from subject number three, according to one aspect of the present disclosure;

[0029] FIGS. 21A-21H are graphical representations showing PTTs and blood pressure results and correlations from subject number four, according to one aspect of the present disclosure;

[0030] FIGS. 22A-22H are graphical representations showing PTTs and blood pressure results and correlations from subject number five, according to one aspect of the present disclosure;

[0031] FIGS. 23A-23H are graphical representations showing PTTs and blood pressure results and correlations from subject number six, according to one aspect of the present disclosure;

[0032] FIGS. 24A-24D are graphical representations showing PVC occurrence in different cardiac signals, according to one aspect of the present disclosure; and

[0033] FIGS. 25A-25D are graphical representations showing PVC occurrence in the same subject on another day, according to one aspect of the present disclosure.

[0034] Corresponding reference characters indicate corresponding elements among the view of the drawings. The headings used in the figures do not limit the scope of the claims.

DETAILED DESCRIPTION

[0035] The present disclosure relates to a system and method to simultaneously measure BCG and PPG from the same body part of an individual, such as a face of a subject individual, with optical imaging. In some embodiments, the face or hand of the individual is a preferred body part because the skin of the individual is usually uncovered, allowing for clear imaging of that body part. The regions for the BCG and PPG measurements are preferably the same or close to each region of the individual, which makes it easy to obtain high-resolution optical images with a single camera, and assist to reduce common noise that occurs when measuring several physiological signals from a single region of the individual. The present disclosure further relates to the detection of PPT from the BCG and PPG pulses, and the determination of blood pressure of the subject based on the calculated PTT, together with other physiological parameters, including gender, age, weight and BMI. Referring to the drawings, embodiments of a non-contact monitoring system for determining BCG, PPG, PTT and/or blood pressure and PVC are illustrated and generally indicated as 100 in FIGS. 1-25.

Tracking of PPG and BCG

[0036] In some embodiments, the PPG and BCG are determined simultaneously from a similar region of the same body part of an individual, e.g., face, using a single digital camera that records the sequential video images of the particular body part of the individual and communicates those images to a controller. Different imaging and data processing algorithms executed by the controller can be used to determine PPG and BCG, respectively. To determine PPG, the image intensity change of the skin region of the individual's body part is analyzed based on the video images taken by the single digital camera, while to determine BCG, subtle body movements of the individual associated with

cardiac activity in the video images are tracked and analyzed. Various algorithms and methods for determining PPG and BCG using the controller are described in greater detail below.

[0037] For BCG detection, a region of interest (ROI) is detected, including at least one body feature, such as a facial feature. For each subject, based on his or her personal characteristics, it was found that multiple options of the body feature that could be used to track BCG. Examples of the features that we have successfully used include but not limited to mole, facial hair, nostril, acne, and skin pigmentation. The BCGs from different facial features on the same subject were similar (FIGS. 4A-4D).

[0038] Mouth, and its surrounding area, was selected as the ROI due to the availability of abundant distinct facial features for BCG tracking (FIG. 1C). The PPG signal obtained from this ROI was also satisfactory.

[0039] Feature points in the defined ROI were detected from the first frame of the video using various methods. The motion of each detected feature point was tracked over video frames with the Kanade-Lucas-Tomasi algorithm (KLT). For an affine motion field

$$\delta = Dx + d \quad (1)$$

[0040] where d is the translation of the feature window's center and D is the deformation matrix, which is given by

$$D = \begin{bmatrix} d_{xx} & d_{xy} \\ d_{yx} & d_{yy} \end{bmatrix}. \quad (2)$$

[0041] KLT determines the motion parameters D and d that minimize the dissimilarity e between two adjacent frames, viz. I and J, in a given feature window around position x. e is expressed as

$$e = \int_w \{J[(1 + D)x + d] - I(x)\}^2 w(x) dx. \quad (3)$$

[0042] The vertical displacement (in the direction along feet to head) contains BCG, which was analyzed in detail. To convert the feature dimensions represented in terms of the number of pixels into meters, a conversion factor was defined as

$$\alpha = \frac{\text{feature_dimension}(m)}{\text{feature_pixel_number(pixel)}}. \quad (4)$$

[0043] This conversion factor was determined by measuring facial feature dimension (e.g., mouth) using a ruler and counting the pixel numbers of the corresponding feature in the image.

[0044] For each frame, n, the vertical components of point locations, y_b , were averaged over all the detected feature points, and plotted against time to provide displacement BCG_d, which can be written as

$$BCG_d(n) = \frac{\sum_{i=1}^k y_i(n)}{k} \times \alpha, \quad (5)$$

[0045] where k is the number of detected feature points and may vary depending on the type of facial feature.

[0046] The first and second temporal derivatives of the displacement BCG were then calculated, leading to velocity BCG, and acceleration BCG_a, respectively.

[0047] A method is used to calculate PPG, whereby the image intensity of green and red channels, I_g and I_r , were averaged over all the ROI pixels in every frame, and then normalized by the corresponding averages, $\mu(I_g)$, and $\mu(I_r)$, over a time interval,

$$PPG(n) = \frac{I_g(n)/\mu(I_g)}{I_r(n)/\mu(I_r)} - 1. \quad (6)$$

[0048] This method is less affected by motion compared to the method when a single color channel (e.g., green) is used.

PPG Evaluation

[0049] Signal-to-noise ratio (SNR) was analyzed for the measured PPG. A 1200-point FFT was computed and detected the heart rate using peak detection in the frequency domain. The majority of PPG power is found around heart rate (~1 Hz) and its corresponding harmonics. The signal power was then defined as the sum of the squared magnitudes of 5 bins around the heart rate, and 5 bins each around the second and third harmonics. The noise power was the sum of the squared magnitudes of all the other bins in the pulse frequency range (0.5-4 Hz). The ratio of signal power to noise power provided SNR according to

$$SNR = 10 \log_{10} \left(\frac{\sum_{f=0.5}^4 (U_t(f)S(f))^2}{\sum_{f=0.5}^4 (1 - U_t(f))S(f)^2} \right) \quad (7)$$

[0050] where S(f) is the spectrum of the signal, f is the frequency (Hz), and $U_t(f)$ is a binary window to pass the pulse frequency and isolate the noise frequency.

BCG Feature Extraction and Evaluation

[0051] Several features were extracted from measured BCG waveforms, including ensemble averages, IJ intervals and amplitudes. Ensemble averaging was performed over the obtained waveforms to look into the morphology of these signals. In order to obtain the ensemble average, the 20 seconds duration signal was plotted as an eye diagram over one cardiac cycle. Multiple individual cycles (~20 beats) were aligned and then averaged to obtain an ensemble waveform. This is similar to the methods reported in literature to analyze BCG. A time duration of 20 seconds results in adequately stable ensemble waveform. IJ interval was calculated as the time difference between acceleration BCG

I_a peak and J_a peak in the same beat, while IJ amplitude was the absolute value of the amplitude from I_a peak to J_a peak.

[0052] Compared to PPG, BCG frequency components are more complex and have a wider distribution in the spectrum (FIGS. 3E and 3F). The majority of BCG power stays in the range of 1-10 Hz. Therefore, the SNR of BCG was evaluated based on two methods: one of them employing maximum likelihood and the other using sample correlation coefficient.

[0053] SNR estimation based on maximum likelihood can be obtained by:

$$SNR_{ML} = \frac{2 \sum_{i=1}^N EA_{sub,1}(i) EA_{sub,2}(i)}{\sum_{i=1}^N (EA_{sub,1}(i) - EA_{sub,2}(i))^2} \quad (8)$$

[0054] where $EA_{sub,1}$ is the sub-ensemble average for the first 10 seconds of the measured displacement BCG, and $EA_{sub,2}$ is that for the remaining 10 seconds. N is the number of samples in the sub-ensemble averages, and i is the sample time index.

[0055] Another SNR estimation method is based on sample correlation coefficient r :

$$r = \frac{\sum_{i=1}^N EA_{sub,1}(i) EA_{sub,2}(i)}{\sqrt{\sum_{i=1}^N EA_{sub,1}(i)^2 \sum_{i=1}^N EA_{sub,2}(i)^2}} \quad (9)$$

[0056] The SNR can be then calculated as:

$$SNR_r = A \frac{r}{1-r} + B, \quad (10)$$

[0057] where A and B are given by:

$$A = \exp\left(\frac{-2}{N-3}\right), \quad (11)$$

$$B = -\frac{1}{2} \left(1 - \exp\left(\frac{-2}{N-3}\right) \right). \quad (12)$$

[0058] To validate the presented BCG detection method for the non-contact monitoring system 100, the measured BCG waveforms were compared against those in literature, and also carried out BCG measurement simultaneously with the accelerometer, which is a well-accepted method for acceleration BCG monitoring. The accelerometer (LSM330) used for the purpose of this study is that found in a commercial off-the-shelf Samsung S4 smartphone. The sample rate of the accelerometer was set at 50 Hz, and based on the datasheet, the linear acceleration sensitivity was typically around 0.007 m/s². The noise level was about 0.005 m/s², which was estimated from the standard deviation by keeping the smartphone stationary on a flat surface for 30 seconds. For measurements with test subjects, the

smartphone was placed on the subject's forehead and held in place with a rubber band (FIG. 1A). The y-axis (feet-head direction) acceleration measured by the accelerometer was compared to the vertical acceleration BCG obtained using the presented method. The Pearson's linear correlation coefficients between ensemble averages, IJ amplitudes and intervals obtained using the two methods were calculated.

Pilot Study Participant Information

[0059] A small-scale pilot study was carried out to demonstrate the presented video-based method for monitoring BCG and PPG simultaneously. The study included 23 subjects (approved by Institutional Review Board at Arizona State University, No. STUDY00003483). The subjects included 15 males and 8 females of different ages (29±5 years old, mean±SD) and ethnic profiles, and from different regions (North America, South America, East Asia and South India). The skin colors of the subjects ranged from type II (white) to type V (brown) based on the Fitzpatrick scale. Informed consents were obtained from all the subjects following an approved protocol. None of the subjects had any known cardiovascular disease.

[0060] A schematic illustration of an experimental setup of one embodiment of the non-contact monitoring system 100 having a controller for determining BCG and PPG shown in FIG. 1A. In some embodiments, a digital camera 102, such as Pike, F-032C digital camera noted above, is used to capture the videos of individual's face 104. In some embodiments, the frame rate can be set at 60 frames per second, although other frame rates may also be used. The video images can be taken by the camera 102 under ambient light condition (e.g., an ordinary 60 W fluorescent lamp). There is no specific requirement on the light source 106 as far as it can provide sufficient illumination of the individual 104 to ensure clear images of the individual's body part 104 (e.g., face) taken by the camera 102. In some embodiments, the individual 104 can stand, sit or lie down on a yoga mat at a distance of approximately 0.5 meters from the lens of the camera 102. Other postures of the individual 104, and distance between the camera 102 and the individual 104 can also be used. The video frames and any associated data are received at the controller, which may implemented by a computer system 200. For example, all the videos and data may be processed and analyzed with software executed by a processor 202 of the computer system 200 shown in FIG. 17 as shall be described in greater detail below.

[0061] As shown in FIGS. 1B and 2, PPG signals 110 and BCG signals 112 are obtained from the same video of the individual's face 104 taken by the camera 102. The video is recorded for typically about ~30 seconds in each test. After the video is captured, a region of interest (ROI) 104A and 104B on the individual's face 104 is selected to extract PPG signals 110 and BCG signals 112 using the following algorithms discussed below that are executed on the processor 202 (FIG. 14).

PPG Algorithm

[0062] Many different algorithms published in literature can be used to determine PPG from the time sequential images (video) of an individual 104. The most straightforward algorithm is used to determine the image intensity

averaged over the selection ROI for each frame, and then plot the average intensity vs. time to obtain the PPG signal of the individual.

BCG Algorithm

[0063] For BCG detection, a particular feature within the ROI of the face of the individual **104** is selected. Examples of the feature include a mole, nostril, hair and skin texture. After the selection of a face feature, the geometric position of the feature is determined and tracked over time. The geometric position can be described in x, y and z dimensions (FIG. 1A illustrates the definition of the x, y and z directions). In some embodiments, angles may also be included to describe orientation of the feature. The x, y, and z displacements are plotted against time to obtain BCG displacement signals shown in FIG. 14A. The signal in one direction, such as y direction, may be substantially larger than those in other directions. The 1st-derivative and 2nd-derivative of the acquired BCG displacement signal are calculated as BCG velocity and BCG acceleration signals, respectively.

[0064] BCG contains important physiological information. For example, the H peak is related to the motion of the heart early in systole, and the main IJK indicates the ventricular ejection and aortic flow. Specifically, the IJ amplitude reflects ventricular ejection and is highly correlated with stroke volume.

[0065] To validate the BCG measurement results, the accelerometer in a Samsung S4 smartphone may be used as a reference. For example, in some embodiments the smartphone may be positioned on the individual's forehead and fixed by an elastic band. The acceleration in x, y and z directions may then be obtained with the y-axis acceleration of the accelerometer representing the vertical movement of the individual **104**, which is plotted in FIGS. 14A and 14B for comparison.

Determination of PTT

[0066] Once PPG **110** and BCG **112** are determined, PTT **114**, the relative time shift between the PPG **110** and BCG **112** pulses is obtained. In some embodiments, one method to determine the PTT **114** (FIG. 2) is determine the position of the most pronounced peak in the BCG signal **112** and the position of the most defined valley in PPG signal **110**.

Determination of Blood Pressure

[0067] PTT **114** is related to blood pressure, which is one of the most important physiological parameters. However the relation between blood pressure **116** (FIG. 2) and PTT **114** (FIG. 2) may vary with each individual **104**. Several factors affect blood pressure **116**, including peripheral resistance, vessel elasticity, blood volume and cardiac output. The cardiac output can be calculated from heart rate and stroke volume, where the heart rate can be calculated from either PPG signal **110** or BCG signal **112**, and the stroke volume can be found from the BCG signal **112**.

[0068] In some embodiments, to determine the blood pressure **116** of an individual **104** from PTT **114**, it is preferable to include heart rate stroke volume, and other physiological parameters from BCG **112** and PPG **110** in the formulism. In some embodiments, accurate measurement of blood pressure **116** from PTT **114** may include calibration with a reference technology, such as traditional blood pres-

sure equipment. In some embodiments, another calibration method may use the blood pressure **116** change when the individual **104** changes his/her position from lying flat to sitting up.

[0069] In other embodiments, a different approach to determine blood pressure **116** from PTT **114** is to create a model that relates blood pressure to PTT **114**, age, gender, weight and height of the individual **104**, as well as heart rate stroke volume, and other physiological parameters determined from BCG signals **112** and PPG signals **110**. This approach does not require calibration, but it will be based on a large cohort study to establish the model.

Initial Test Results

BCG and PPG

[0070] The displacement BCG and PPG simultaneously was obtained from a video of each subject. FIGS. 3A-3F show the results for a male subject. The J_d -peak, one of the most prominent features of BCG, is clearly resolved in the displacement BCG obtained with the presented video method (FIG. 3A). The corresponding velocity and acceleration BCGs were obtained by taking first and second temporal derivatives, and then filtering them with a 2nd order Butterworth filter with a passband of [0.5, 10] Hz (FIG. 3A and FIG. 3C). The obtained PPG is shown in FIG. 3D). DC bias is removed from these signals. Ensemble averages of these waveforms are provided on the right of the figures. The power spectra of the displacement BCG and PPG are shown in FIGS. 3E and 3F).

[0071] FIGS. 4A-4D show the BCGs detected from three different facial features (facial hair, mole and nostril) using the same video of a male subject. BCGs obtained from different features look very similar. The Pearson's linear correlation coefficients between every two signals are larger than 0.95, implying that the displacement BCGs obtained from the three features are strongly correlated.

Validation of BCG Detection

[0072] To validate the video-based noncontact method for BCG detection, simultaneous measurement of BCG with a reference device (accelerometer) were carried out. The acceleration BCGs along feet-head direction obtained using the present method, and the reference methods are plotted in FIGS. 5A-5D. Both waveforms are filtered with a 2nd order Butterworth filter with a passband of [0.5, 10] Hz. The obtained BCG waveform from the video is resampled from 60 Hz to 50 Hz to match the sampling rate of the accelerometer for comparison purpose. The overall patterns and the obtained cardiac cycles from the two methods are consistent with each other, which validates the presented noncontact method for BCG monitoring.

[0073] To further examine the detailed features of the BCGs obtained with the two methods, ensemble averaging was performed for two subjects over a duration of 20 seconds, and the resulting waveforms, including individual cycles (dash lines) and ensemble averages (solid lines), are shown in FIGS. 5A-5D. (solid line). The major waves (H, I, J, and K), IJ amplitude (|a|), and IJ interval (t) are denoted with letters, FIG. 5B illustrates BCG for the female subject shown in FIG. 5A, measured simultaneously using an accelerometer. FIG. 5C illustrates BCG waveforms, for a male subject (heart rate=1.1 Hz), measured from 19 individual

cardiac cycles (dash lines) and ensemble average for the 19 cycles (solid line). FIG. 5D illustrates the BCG for the male subject shown in FIG. 5C, measured simultaneously using an accelerometer.

[0074] For both subjects, the major peaks in BCG waveforms from the presented and reference methods are similar, and the Pearson's linear correlation coefficients are larger than 0.95, implying that the test results obtained from the two methods are strongly related. Furthermore, the obtained BCGs from both methods are also consistent with the typical direct body measurement BCG waveforms reported in literature.

Small Scale Pilot Study

[0075] In the small-scale pilot study, a test was performed as described in above on each subject. FIG. 6 shows the displacement BCGs obtained from seven different subjects for the purpose of demonstration. The overall BCG waveforms are similar for all subjects, but the detailed features show substantial variations due to different physiological attributes, which have also been reported by other literatures. The largest amplitudes of the measured displacement BCG J-peaks ranged from 1×10^{-4} to 2×10^{-4} m. The velocity and acceleration peaks varied from 2×10^{-3} to 6×10^{-3} m/s, and 0.05 to 0.15 m/s², respectively. These values are comparable to those reported by other researchers using different methods (Table 1). For the same subject, the measurement error for these values was about 10% in consecutive tests.

TABLE 1

BCG VALUES COMPARISON		
BCG Type	References	Presented Method
displacement (m)	6×10^{-5} [28], 1.5×10^{-4} [50], 10^{-4} [45],	1.5×10^{-4}
velocity (m/s)	2.5×10^{-3} [28],	4×10^{-4}
acceleration (m/s ²)	0.1 [9, 17], 0.08 [45]	0.09

The reference values are estimated from the report test results (plots). The values from the presented method are averaged over 23 healthy subjects.

[0076] The IJ amplitudes (I) and intervals (t) of acceleration BCGs determined using the non-contact monitoring system were compared with those using the reference accelerometer. FIGS. 7 and 8 show the plots of these two values from 73 tests with linear least square regression. Good linear correlation is found between the presented and reference methods for both plots ($R^2=0.82$ and $R^2=0.7$). The difference between the two methods may be attributed to different body locations (mouth region for presented method and forehead for accelerometer). The accuracy may also be affected by the calibration error.

[0077] FIG. 9 summarizes the Pearson's linear correlation coefficients between the BCGs measured using the presented method and reference accelerometer. FIG. 10 shows the BCG SNR values based on maximum likelihood (8) and sample correlation coefficient (10) using the presented method. All the test results are divided into four groups based on the types of facial features used for motion tracking. The SNR values and the standard deviations are comparable using weighing scale. FIGS. 9 and 10 suggest that the selection of facial features is not a key factor for video-based BCG monitoring since the values are comparable among different features.

[0078] To evaluate PPG quality, we plotted the PPG SNR, as shown in FIG. 11. All the test results are divided into four different skin types. The overall SNR values are comparable to other studies. The SNR values from lighter skin tone subjects are better than darker skin tone subjects, which have also been reported by other researchers.

Signals from Other Posture

[0079] The non-contact monitoring system was validated against a sitting position of the subject. For example, FIGS. 12A-12E. illustrate the signals obtained when the subject was sitting on a chair. BCG was obtained by tracking facial feature (mole) and PPG was obtained from the mouth region, using the same methods as described above. The subject was the same as the one in FIGS. 3A-3D. An accelerometer was also used as a reference device for comparison. The Pearson's linear correlation coefficient between the presented method (FIG. 12C) and reference device (FIG. 12E) was shown to be 0.97. BCG waveforms show the difference between sitting and supine positions, which has also been reported in other literature.

[0080] FIG. 14 illustrates an example of a suitable computing and networking environment used to implement various aspects of the present disclosure. Example embodiments described herein may be implemented at least in part in electronic circuitry; in computer hardware executing firmware and/or software instructions; and/or in combinations thereof. Example embodiments also may be implemented using a computer program product (e.g., a computer program tangibly or non-transitorily embodied in a machine-readable medium and including instructions for execution by, or to control the operation of, a data processing apparatus, such as, for example, one or more programmable processors or computers). A computer program may be written in any form of programming language, including compiled or interpreted languages, and may be deployed in any form, including as a stand-alone program or as a subroutine or other unit suitable for use in a computing environment. Also, a computer program can be deployed to be executed on one computer, or to be executed on multiple computers at one site or distributed across multiple sites and interconnected by a communication network.

[0081] Certain embodiments are described herein as including one or more modules. Such modules are hardware-implemented, and thus include at least one tangible unit capable of performing certain operations and may be configured or arranged in a certain manner. For example, a hardware-implemented module may comprise dedicated circuitry that is permanently configured (e.g., as a special-purpose processor, such as a field-programmable gate array (FPGA) or an application-specific integrated circuit (ASIC)) to perform certain operations. A hardware-implemented module may also comprise programmable circuitry (e.g., as encompassed within a general-purpose processor or other programmable processor) that is temporarily configured by software or firmware to perform certain operations. In some example embodiments, one or more computer systems (e.g., a standalone system, a client and/or server computer system, or a peer-to-peer computer system) or one or more processors may be configured by software (e.g., an application or application portion) as a hardware-implemented module that operates to perform certain operations as described herein.

[0082] Accordingly, the term "hardware-implemented module" encompasses a tangible entity, be that an entity that is physically constructed, permanently configured (e.g.,

hardwired), or temporarily configured (e.g., programmed) to operate in a certain manner and/or to perform certain operations described herein. Considering embodiments in which hardware-implemented modules are temporarily configured (e.g., programmed), each of the hardware-implemented modules need not be configured or instantiated at any one instance in time. For example, where the hardware-implemented modules comprise a general-purpose processor configured using software, the general-purpose processor may be configured as respective different hardware-implemented modules **212** at different times. Software may accordingly configure a processor **202**, for example, to constitute a particular hardware-implemented module at one instance of time and to constitute a different hardware-implemented module at a different instance of time.

[0083] Hardware-implemented modules **212** may provide information to, and/or receive information from, other hardware-implemented modules **212**. Accordingly, the described hardware-implemented modules **212** may be regarded as being communicatively coupled. Where multiple of such hardware-implemented modules **212** exist contemporaneously, communications may be achieved through signal transmission (e.g., over appropriate circuits and buses) that connect the hardware-implemented modules. In embodiments in which multiple hardware-implemented modules **212** are configured or instantiated at different times, communications between such hardware-implemented modules may be achieved, for example, through the storage and retrieval of information in memory structures to which the multiple hardware-implemented modules **212** have access. For example, one hardware-implemented module **212** may perform an operation, and may store the output of that operation in a memory device to which it is communicatively coupled. A further hardware-implemented module **212** may then, at a later time, access the memory device to retrieve and process the stored output. Hardware-implemented modules **212** may also initiate communications with input or output devices.

[0084] As illustrated, the computing and networking environment **200** may a general purpose computing device **200**, although it is contemplated that the networking environment **200** may include other computing systems, such as personal computers, server computers, hand-held or laptop devices, tablet devices, multiprocessor systems, microprocessor-based systems, set top boxes, programmable consumer electronic devices, network PCs, minicomputers, mainframe computers, digital signal processors, state machines, logic circuitries, distributed computing environments that include any of the above computing systems or devices, and the like.

[0085] Components of the general purpose computing device **200** may include various hardware components, such as a processing unit **202**, a main memory **204** (e.g., a system memory), and a system bus **201** that couples various system components of the general purpose computing device **200** to the processing unit **202**. The system bus **201** may be any of several types of bus structures including a memory bus or memory controller, a peripheral bus, and a local bus using any of a variety of bus architectures. For example, such architectures may include Industry Standard Architecture (ISA) bus, Micro Channel Architecture (MCA) bus, Enhanced ISA (EISA) bus, Video Electronics Standards Association (VESA) local bus, and Peripheral Component Interconnect (PCI) bus also known as Mezzanine bus.

[0086] The general purpose computing device **200** may further include a variety of computer-readable media **207** that includes removable/non-removable media and volatile/nonvolatile media, but excludes transitory propagated signals. Computer-readable media **207** may also include computer storage media and communication media. Computer storage media includes removable/non-removable media and volatile/nonvolatile media implemented in any method or technology for storage of information, such as computer-readable instructions, data structures, program modules or other data, such as RAM, ROM, EEPROM, flash memory or other memory technology, CD-ROM, digital versatile disks (DVD) or other optical disk storage, magnetic cassettes, magnetic tape, magnetic disk storage or other magnetic storage devices, or any other medium that may be used to store the desired information/data and which may be accessed by the general purpose computing device **200**. Communication media includes computer-readable instructions, data structures, program modules or other data in a modulated data signal such as a carrier wave or other transport mechanism and includes any information delivery media. The term “modulated data signal” means a signal that has one or more of its characteristics set or changed in such a manner as to encode information in the signal. For example, communication media may include wired media such as a wired network or direct-wired connection and wireless media such as acoustic, RF, infrared, and/or other wireless media, or some combination thereof. Computer-readable media may be embodied as a computer program product, such as software stored on computer storage media.

[0087] The main memory **204** includes computer storage media in the form of volatile/nonvolatile memory such as read only memory (ROM) and random access memory (RAM). A basic input/output system (BIOS), containing the basic routines that help to transfer information between elements within the general purpose computing device **200** (e.g., during start-up) is typically stored in ROM. RAM typically contains data and/or program modules that are immediately accessible to and/or presently being operated on by processing unit **202**. For example, in one embodiment, data storage **206** holds an operating system, application programs, and other program modules and program data.

[0088] Data storage **206** may also include other removable/non-removable, volatile/nonvolatile computer storage media. For example, data storage **206** may be: a hard disk drive that reads from or writes to non-removable, nonvolatile magnetic media; a magnetic disk drive that reads from or writes to a removable, nonvolatile magnetic disk; and/or an optical disk drive that reads from or writes to a removable, nonvolatile optical disk such as a CD-ROM or other optical media. Other removable/non-removable, volatile/nonvolatile computer storage media may include magnetic tape cassettes, flash memory cards, digital versatile disks, digital video tape, solid state RAM, solid state ROM, and the like. The drives and their associated computer storage media provide storage of computer-readable instructions, data structures, program modules and other data for the general purpose computing device **200**.

[0089] A user may enter commands and information through a user interface **240** or other input devices **245** such as a tablet, electronic digitizer, a microphone, keyboard, and/or pointing device, commonly referred to as mouse, trackball or touch pad. Other input devices **245** may include a joystick, game pad, satellite dish, scanner, or the like.

Additionally, voice inputs, gesture inputs (e.g., via hands or fingers), or other natural user interfaces may also be used with the appropriate input devices, such as a microphone, camera, tablet, touch pad, glove, or other sensor. These and other input devices **245** are often connected to the processing unit **202** through a user interface **240** that is coupled to the system bus **201**, but may be connected by other interface and bus structures, such as a parallel port, game port or a universal serial bus (USB). A monitor **260** or other type of display device is also connected to the system bus **201** via user interface **240**, such as a video interface. The monitor **260** may also be integrated with a touch-screen panel or the like.

[0090] The general purpose computing device **200** may operate in a networked or cloud-computing environment using logical connections of a network Interface **203** to one or more remote devices, such as a remote computer. The remote computer may be a personal computer, a server, a router, a network PC, a peer device or other common network node, and typically includes many or all of the elements described above relative to the general purpose computing device **200**. The logical connection may include one or more local area networks (LAN) and one or more wide area networks (WAN), but may also include other networks. Such networking environments are commonplace in offices, enterprise-wide computer networks, intranets and the Internet.

[0091] When used in a networked or cloud-computing environment, the general purpose computing device **200** may be connected to a public and/or private network through the network interface **203**. In such embodiments, a modem or other means for establishing communications over the network is connected to the system bus **201** via the network interface **203** or other appropriate mechanism. A wireless networking component including an interface and antenna may be coupled through a suitable device such as an access point or peer computer to a network. In a networked environment, program modules depicted relative to the general purpose computing device **200**, or portions thereof, may be stored in the remote memory storage device.

[0092] Referring to FIG. 15, a flow chart illustrates the operation of one method performed by the controller, including the hardware-implemented module **212** executed by the processor **202** of the computing device **200** to simultaneously measure BCG and PPG from the same body part of an individual as illustrated in FIG. 1B. At block **300**, recording sequential video images **108** of a same body part of an individual using digital camera **102**. At block **302**, selecting a region of interest **112A** along the same body part of the individual. At block **304**, tracking body movements **110A** of the same body part of the individual in the sequential video images **108** taken by the digital camera **102**. At block **304**, determining any vertical displacements **110B** of body movements of the same body part of the individual in the sequential video images **108** taken by the digital camera **102** to generate a BCG **110C** of the individual. At block **306**, calculating an average intensity **112B** of the region of interest from the sequential video images **108** taken of the same body part of the individual to generate a PPG **112C** of the individual. At block **308**, calculating a pulse transit time based on the BCG **110C** and PPG **112C**. At block **310**, calculating a blood pressure of the individual based on the pulse transit time.

Relationship Between Pulse Transit Time and Blood Pressure

[0093] The relationship between PTT and BP has been analyzed with the arterial wall model and the arterial wave propagation model. If the arterial vessel is modeled as an elastic cylindrical tube, then PTT can be regarded as the time for a pressure wave to travel along the tube over a distance of l . This leads to,

$$PTT = \sqrt{C/A} \quad (13)$$

[0094] where ρ is blood density, A is the vessel cross-sectional area, and C is compliance that measures the blood vessel's ability to resist pressure. Pressure (P) can be expressed in terms of PTT as,

$$P = P_1 \sqrt{\frac{A_m \cdot \rho \cdot l^2}{\pi A \cdot P_1 \cdot PTT^2} - 1} + P_0 \quad (14)$$

[0095] where A_m , P_0 and P_1 are subject-specific parameters and where A_m , P_0 and P_1 are subject-specific parameters. If we assume the values of the parameters based on reference, an inverse correlation can be found between PTT and BP in FIG. 16.

[0096] Other researchers have also reported BP can be empirically correlated with PTT with different equations such as

$$BP = K_1 \ln(PTT) + K_2, \quad (15)$$

$$BP = \frac{K_1}{PTT} + K_2, \quad (16)$$

$$BP = \frac{K_1}{(PTT - K_2)^2} + K_3, \quad (17)$$

where K are subject-specific parameters [100]. Therefore, it is expected to see some dependence between BP and PTT.

Method of Measurement

[0097] A Pike camera (F-032C) was used to monitor PPG and BCG, meanwhile EPIC Sensors (PS25451) were used to monitor ECG as a reference cardiac signal. Prominent features of these signals were identified by the time they occurred in each cardiac cycle. The features included: ECG "R" peak, PPG peak and displacement BCG "J_d" peak. The time difference was estimated between every two signals in each cardiac cycle, which included: (1) PTT₁: time delay from displacement BCG "J_d" peak to PPG peak; (2) PTT₂: time delay from ECG "R" peak to displacement BCG "J_d" peak; and (3) PTT₃: time delay from ECG "R" peak to PPG peak. The obtained time delays were plotted against time. Within these values, PTT₁ can be obtained by using camera. Obtained PTT values were averaged every 10 seconds to reduce the influence of artifacts (e.g. respiration). A commercial cuff-based blood pressure monitor (Omron BP786) was used as reference to record BP values about every 40-50 seconds. The measurement error of the reference BP monitor is about ± 5 mmHg.

Design of Experiment

[0098] To validate the presented method for blood pressure tracking, the subjects were asked to do exercises to alter their blood pressure. Researchers have reported that systolic blood pressure (SBP) is inversely correlated with PTT after exercise. Depending on the effort level and body condition of the subjects, SBP was changed from 5 to 30 mmHg, and diastolic blood pressure (DBP) was changed from 1 to 10 mmHg. Based on literature, SBP correlates better with PTT compared with DBP.

[0099] Each experiment had five stages including a 400-second video recording. The five stages (FIG. 20) are as follows:

[0100] Stage I: System setup (120 seconds). The subject is asked to lie down and maintain a relaxed state. Camera was adjusted to a proper view with good focus for video recording. Two ECG electrodes were connected to the skin. Reference BP monitor is attached to subject's upper arm through a cuff.

[0101] Stage II: Resting 1 (100 seconds). Video and ECG data are recorded simultaneously. Reference BP monitors measures the BP values every 40-50 seconds.

[0102] Stage III: Exercise (60 seconds). The subject was asked to take moderate exercise (sit up or push up) for about 1 minute.

[0103] Stage IV: Re-setup (20-60 seconds). The subject was asked to lie down and relax. Camera, ECG sensors and reference BP monitor were set up again to measure corresponding values from subject after taking exercise. The re-setup is tried to be done as soon as possible, normally it takes about 20-60 seconds.

[0104] Stage V: Resting 2 (~200 seconds). The non-contact monitoring system 100 resumed collecting data till the end of the experiment.

[0105] Due to the intense body motions in Stage III and IV, data recording (including video, ECG and reference BP) is not able to be performed during these two time periods. The estimated changes in BP and PTT in different stages are illustrated in FIG. 17.

[0106] FIGS. 18A-18H show the blood pressure tracking results and correlations with SBP measured by reference technology with a male subject (#1). Obtained PTT values were averaged every 10 seconds to reduce the influence of artifacts (FIGS. 18A-18C). SBP and DBP values were obtained from reference BP monitor every 50 seconds. The timing of the BP values was obtained when the BP readings were available on the display of the device. The shadow areas indicate the time periods during which measurements were not able to be obtained due to the subject having recently exercised or waiting for system setup (FIGS. 18A-18E). Correlations are calculated between PTT values and SBP during BP recovery period after exercise (FIGS. 18F-18H). The SBP values were interpolated to reach a time resolution as 10 seconds. In regular cuff-based BP device, SBP value was obtained earlier than DBP, therefore, SBP was shifted in time by 20 seconds to compensate for this delay. Outliners were removed which may have been caused by different sources of artifacts, for instance, unwanted body motions or slow response of reference method. The increase of SBP due to the subject taking exercise in the experiment was about 10 mmHg.

[0107] Correlation between blood pressure (especially SBP) and PTT values can be seen from all the plots in FIGS. 18A-18C. The trends are clearer with FIG. 18A and FIG.

18B. After taking exercise, the PTT values were lower than those before taking exercise. A quick recovery can be noticed right after the exercise and then followed by a slow climbing up. Among the three calculation methods, using PTT from PPG to BCG to track blood pressure is the main interest of my work since both PPG and BCG waveforms can be obtained by a single camera simultaneously.

[0108] FIGS. 19-23 illustrate the experimental results following the same protocols obtained from male subjects #2, #3, and female subjects #4, #5, #6.

[0109] Within all the subjects, PTT_1 and PTT_2 show overall better correlations with BP compared with PTT_3 . Relying completely on ECG may introduce variability in the pre-ejection period, and PPG at current state has insignificant noise level. Combining these two factors together probably makes PTT_3 have the worst correlation with BP.

Detection of Premature Ventricular Contraction

[0110] During the experiment for BP monitoring, Premature Ventricular Contraction (PVC) was also detected with both presented video-based method and reference ECG.

[0111] PVC is the extra, abnormal heartbeat that begins in one of the heart's two lower chambers. It is a sign of decreased oxygenation to the heart muscle. It occurs in most people at some point with the feeling as "skipped beats". Causes of PVC may include medications, alcohol, anxiety and so on. For most people with isolated PVCs, treatment is not needed. However, if PVCs occur continuously for longer than 30 seconds, it may indicate serious cardiac condition.

[0112] Traditional method to diagnose PVC is based on ECG. PVC pattern can be easily distinguished from a normal heart beat. Normally, to detect PVC, the patients are required to wear a conventional Holter monitor to record ECG continuously for about 48 hours, and the data will be saved and analyzed by doctors later. The electrodes of Holter monitor are attached to the patients' chest, resulting in discomfort and limitation of freedom. Other than ECG-based methods, researchers have also reported PVC detection based on PPG and BCG waveforms with contact-based methods. In PPG recorded by sensor attached to finger, PVC can be recognized by an abnormal longer peak-peak interval. Some methods detect PVC based on acceleration BCG using weighing scale by finding the significantly lower BCG "I_J" amplitudes.

[0113] During experimentation, the occurrences of PVC were found with one subject. The frequency of PVC appearance was about twice in 5 minutes. The PVC patterns can be recognized from both PPG and BCG waveforms and the happenings of PVC were also confirmed by the synchronized ECG recordings.

[0114] FIGS. 24A-D and 25A-D show the occurrences of PVC with the same subject in different days. The shadow areas indicate the occurrences of PVC. ECG, PPG and BCG waveforms were recording simultaneously. In ECG (FIG. 24A and FIG. 25A), the abnormal forms of PVC were found in QRS-complex. In PPG (FIG. 24B and FIG. 25B), longer peak-peak intervals were found. In displacement BCG (FIG. 24C and FIG. 25C), J_d peaks show lower amplitudes and the whole cycles looked uncomplete compared with regular heartbeat cycles. In acceleration BCG (FIG. 24D and FIG. 25D), the "I_J" amplitudes of PVC were lower than those in neighboring normal heartbeat cycles.

[0115] In the blood pressure experiment, the subjects were asked to take exercise to change their blood pressure. Taking

exercise makes muscles need more oxygen. As a result, the heart pumps more blood around the body together with more powerful contractions which will make blood pressure increase. However, exercise may introduce extra body motions which will influence the PPG and BCG qualities, especially for BCG, which is a recording of small body movement. New test protocols may be needed to validate presented method without introduction of extra motion artifacts. One of the potential solutions is using medicine (e.g. Nitroglycerin), which will change blood pressure without extra body movements. However, the implementation of this protocol may need collaboration with professional medical staff.

[0116] Individual calibration is a limitation of blood pressure monitoring using PTT method, which is due to the individual mechanical properties of the vascular wall and other factors. Currently, PTT-based methods have been proved to track the trend of blood pressure change especially for SBP, however, getting absolute blood pressure values without calibration is difficult to achieve.

[0117] Using video-based technique potentially can provide a non-contact solution for PVC long term monitoring. A better understanding of PVC patterns in PPG and BCG may help to automatic recognition of such events.

[0118] It should be understood from the foregoing that, while particular embodiments have been illustrated and described, various modifications can be made thereto without departing from the spirit and scope of the invention as will be apparent to those skilled in the art. Such changes and modifications are within the scope and teachings of this invention as defined in the claims appended hereto.

What is claimed is:

1. A method for monitoring an individual having a body part, the method comprising:

receiving a set of sequential video frames of the body part of the individual at a controller, the set of sequential video frames captured using a camera;

defining a region of interest of the body part in a first video frame of the set of sequential video frames, the region of interest including a body feature;

tracking motion of the body feature over the set of sequential video frames using the controller;

generating an acceleration ballistocardiogram from a first derivative of the displacement ballistocardiogram using the controller;

averaging a first image intensity of a first color channel over pixels corresponding to the region of interest in the set of sequential video frames using the controller; and

averaging a second image intensity of a second color channel over the pixels corresponding to the region of interest in the set of sequential video frames using the controller.

2. The method of claim 1, further comprising:

generating a displacement ballistocardiogram based on the motion of the body feature using the controller;

generating a velocity ballistocardiogram from a first derivative of the displacement ballistocardiogram using the controller; and

generating a photoplethysmogram by normalizing the first image intensity and the second image intensity over a time interval.

3. The method of claim 1, wherein the motion of the body feature is tracked by:

determining a translation of a center of the body feature; and

minimizing a dissimilarity between adjacent frames in the set of sequential video frames.

4. The method of claim 1, wherein the displacement ballistocardiogram is determined by plotting averaged vertical components of point locations for the body feature for each frame of the set of sequential video frames against time.

5. The method of claim 1, wherein the body feature is a facial feature and the body part is a face of the individual.

6. The method of claim 1, wherein the first color channel is green and the second color channel is red.

7. The method of claim 1, wherein the camera is a single optical camera.

8. The method of claim 1, further comprising:

generating a pulse transit time from at least one of the photoplethysmogram and the ballistocardiogram using the controller.

9. The method of claim 8, further comprising:

determining blood pressure of the individual from the pulse transit time using the controller.

10. A method for monitoring an individual having a body part, the method comprising:

receiving a set of sequential video frames of the body part of the individual at a controller, the set of sequential video frames captured using a single camera;

defining a region of interest of the body part in a first video frame of the set of sequential video frames, the region of interest including a body feature;

tracking motion of the body feature over the set of sequential video frames using the controller;

generating a ballistocardiogram pulse based on the motion of the body feature using the controller; and

generating a photoplethysmogram pulse based on an image intensity averaged over the region of interest for each frame in the set of sequential video frames and plotted against time using the controller.

11. The method of claim 10, wherein the ballistocardiogram pulse include a velocity ballistocardiogram pulse and an acceleration ballistocardiogram pulse.

12. The method of claim 10, further comprising:

generating a pulse transit time based on a relative time shift between the ballistocardiogram pulse and the photoplethysmogram pulse.

13. The method of claim 12, further comprising:

determining a blood pressure for the individual from at least one of the pulse transit time, cardiac output, peripheral resistance, vessel elasticity, or blood volume.

14. The method of claim 13, further comprising:

determining a heart rate for the individual from the ballistocardiogram pulse or the photoplethysmogram pulse;

determining a stroke volume for the individual from the ballistocardiogram pulse; and

determining the cardiac output from the heart rate and the stroke volume.

15. A system for monitoring an individual having a body part, the system comprising:

a camera disposed relative to the body part of the individual, the camera capturing a set of sequential video frames of the body part of the individual;

a controller in communication with the camera, the controller generating a ballistocardiogram pulse and a photoplethysmogram pulse from the set of sequential video frames, the ballistocardiogram pulse generated from a vertical displacement of a body feature within a defined region of interest of the body part and tracked over the set of sequential video frames, the photoplethysmogram pulse generated based on an image intensity averaged over the region of interest for each frame in the set of sequential video frames and plotted against time.

16. The system of claim **15**, wherein the controller generates a pulse transit time based on a relative time shift between the ballistocardiogram pulse and the photoplethysmogram pulse.

17. The system of claim **16**, wherein the controller determines a blood pressure for the individual from the pulse transit time.

18. The system of claim **15**, wherein the controller determines a Premature Ventricular Contraction (PVC) based on the ballistocardiogram pulse and the photoplethysmogram pulse from the set of sequential video frames.

19. The system of claim **15**, wherein the ballistocardiogram pulse includes a velocity ballistocardiogram pulse and an acceleration ballistocardiogram pulse.

20. The system of claim **15**, wherein the image intensity is averaged for a first color channel and a second color channel.

* * * * *

专利名称(译)	用于非接触式监测心冲击描记图，光电容积描记图，血压和异常心律的系统和方法		
公开(公告)号	US20190082972A1	公开(公告)日	2019-03-21
申请号	US16/083052	申请日	2017-03-08
申请(专利权)人(译)	加州大学董事会代表亚利桑那州立大学亚利桑那板		
当前申请(专利权)人(译)	加州大学董事会代表亚利桑那州立大学亚利桑那板		
[标]发明人	TAO NONGJIAN SHAO DANGDANG		
发明人	TAO, NONGJIAN SHAO, DANGDANG		
IPC分类号	A61B5/0205 A61B5/00 A61B5/11 A61B5/021 G06T7/20		
CPC分类号	A61B5/0205 A61B5/0077 A61B5/1102 A61B5/02125 G06T7/20 A61B5/02416 G06T2207/30076		
优先权	62/307064 2016-03-11 US		
外部链接	Espacenet USPTO		

摘要(译)

公开了用于基于人体的光学成像跟踪心冲击描记图，光电容积描记图，血压和异常心律的系统和方法的各种实施例。同时获得来自人体相似区域的心冲击描记图和光电容积描记图信号，并使用两个信号之间的时间延迟来确定受试者的血压以及受试者的其他生理参数，包括性别，年龄，体重，高度，心率，每搏输出量，血压和使用其他方法获得的心律异常。

