




US 20190150718A1

(19) **United States**(12) **Patent Application Publication**
Melsky(10) **Pub. No.: US 2019/0150718 A1**(43) **Pub. Date: May 23, 2019**(54) **METHOD FOR VISUALIZING TISSUE WITH
AN ICG DYE COMPOSITION DURING
ABLATION PROCEDURES***A61B 18/20* (2006.01)*A61B 1/06* (2006.01)(52) **U.S. Cl.**CPC *A61B 1/043* (2013.01); *A61B 5/0071*
(2013.01); *A61B 5/0084* (2013.01); *A61B*
2090/373 (2016.02); *A61B 18/20* (2013.01);
A61B 1/0638 (2013.01); *A61B 5/4836*
(2013.01)(71) Applicant: **CardioFocus, Inc.**, Marlborough, MA
(US)(72) Inventor: **Gerald Melsky**, Lexington, MA (US)(21) Appl. No.: **16/259,483**(22) Filed: **Jan. 28, 2019**

(57)

ABSTRACT**Related U.S. Application Data**(62) Division of application No. 14/697,065, filed on Apr.
27, 2015.(60) Provisional application No. 61/985,142, filed on Apr.
28, 2014.**Publication Classification**(51) **Int. Cl.***A61B 1/04* (2006.01)*A61B 5/00* (2006.01)

A system is provided for identifying the sufficiency of lesions formed during a tissue ablation procedure. The system and method include administering an ICG composition to the patient and forming one or more lesions at a surgical site. The method further includes applying energy of a type and in an amount sufficient to cause ICG in the patient to fluoresce. An image of the tissue and lesion at the surgical site is obtained while the ICG fluoresces. The lesion is distinguished from surrounding de novo tissue based on areas of fluorescence to allow a user to evaluate the quality of the lesion.

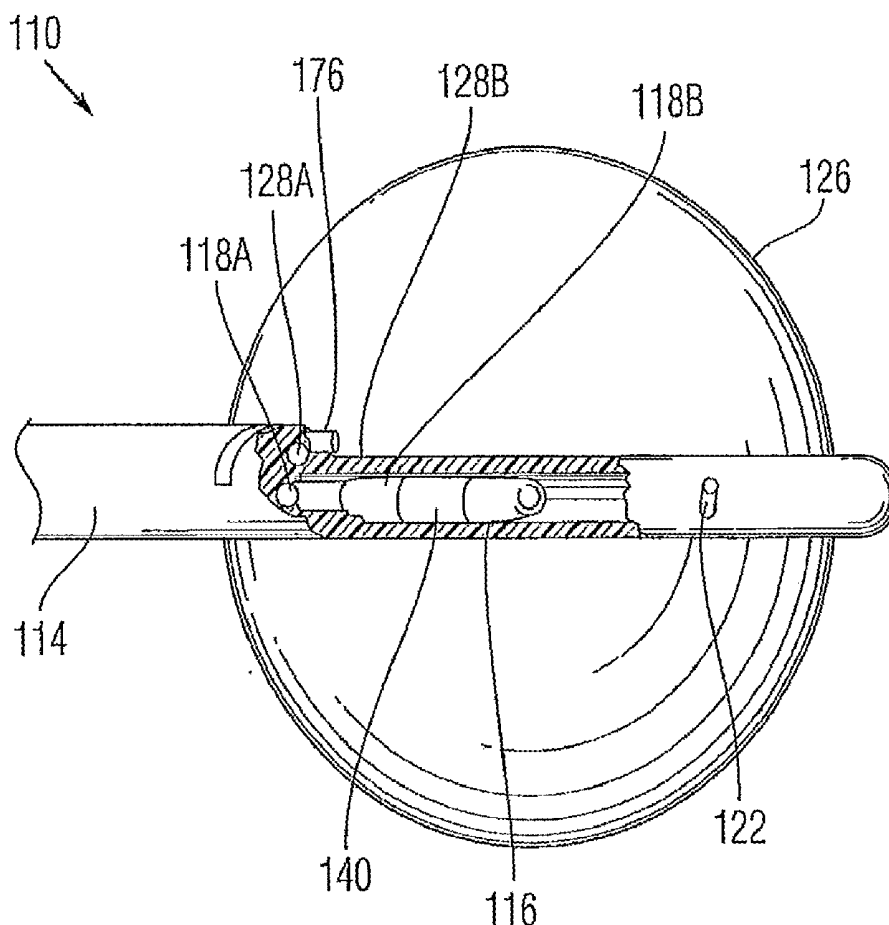

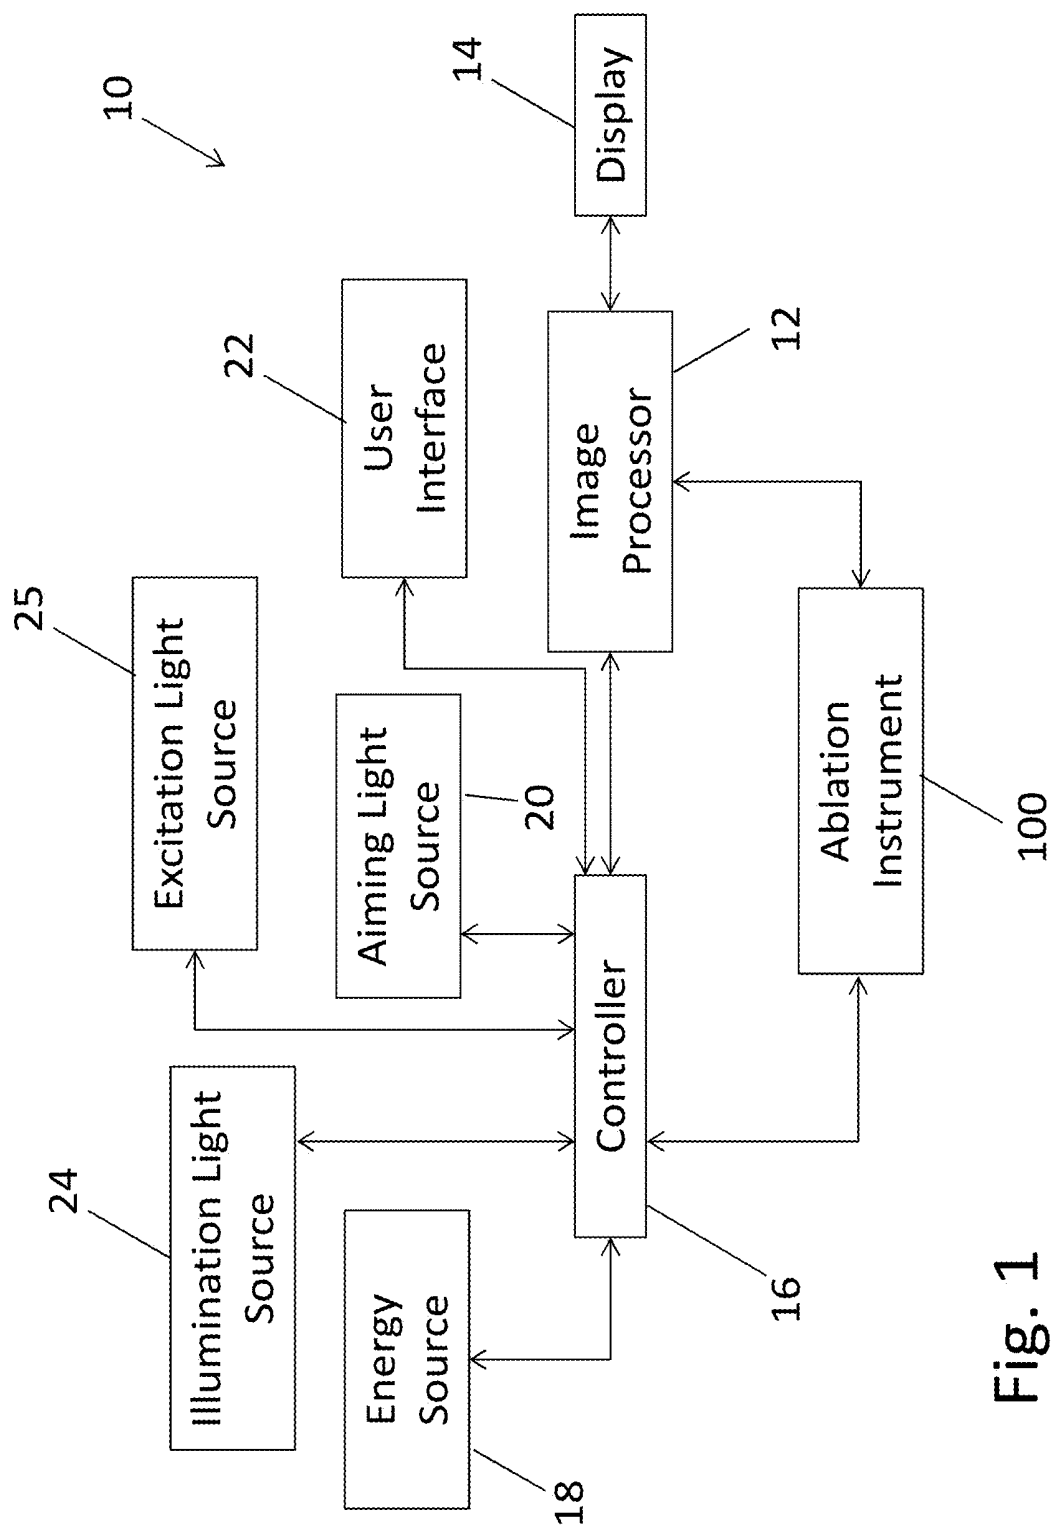


Fig. 1

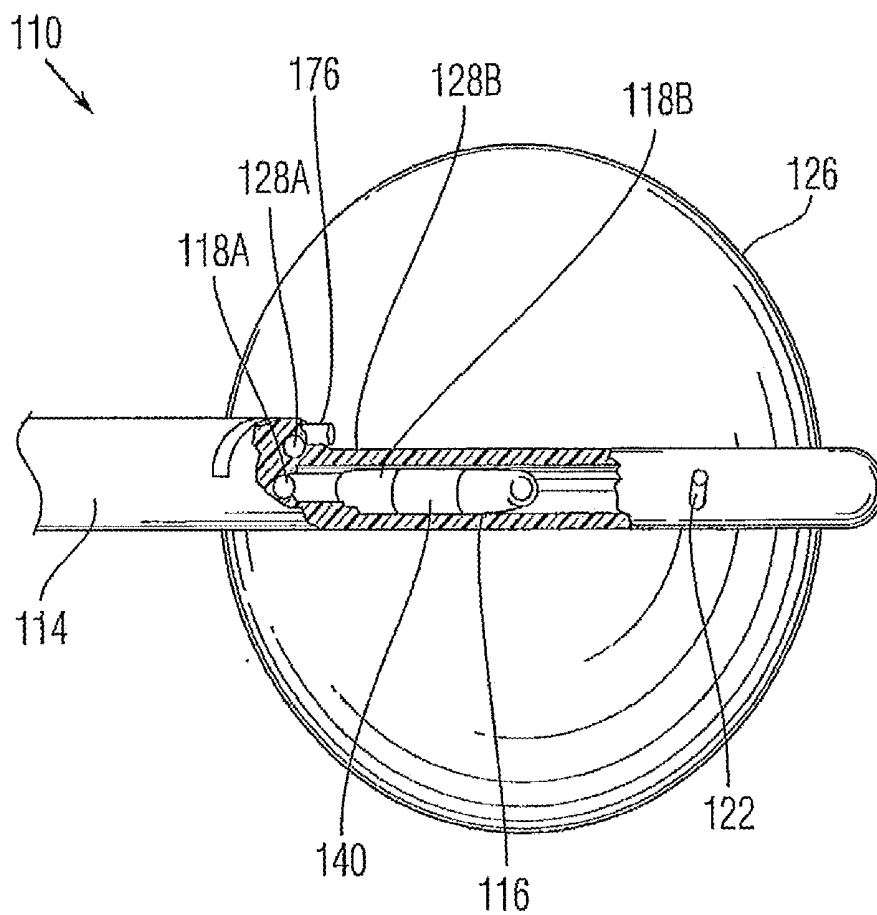


Fig. 2

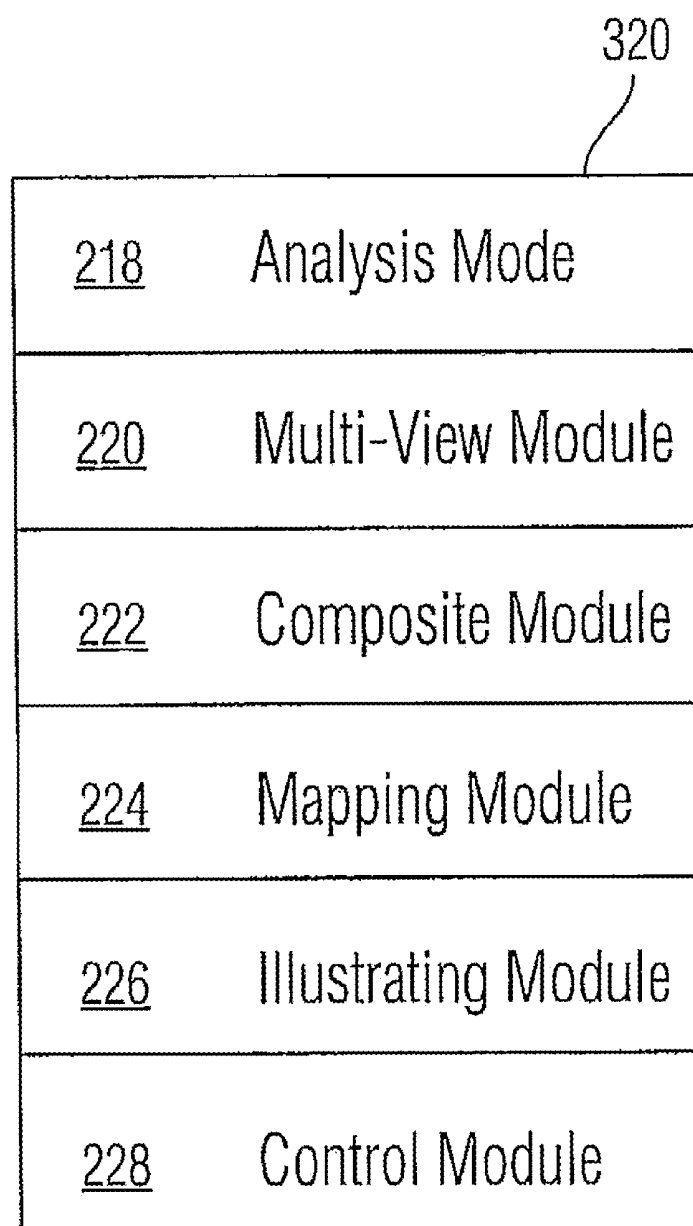


Fig. 3

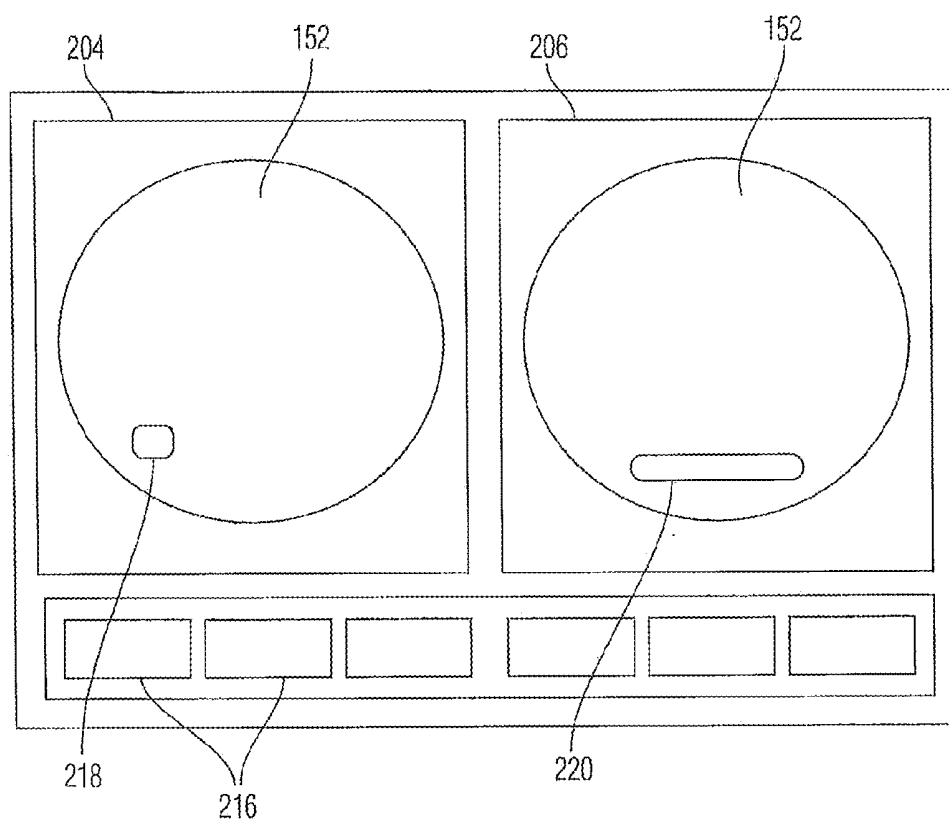


Fig. 4

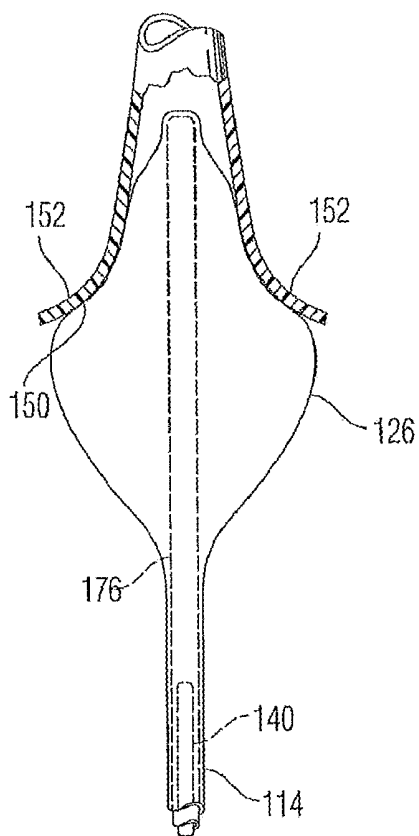


Fig. 5

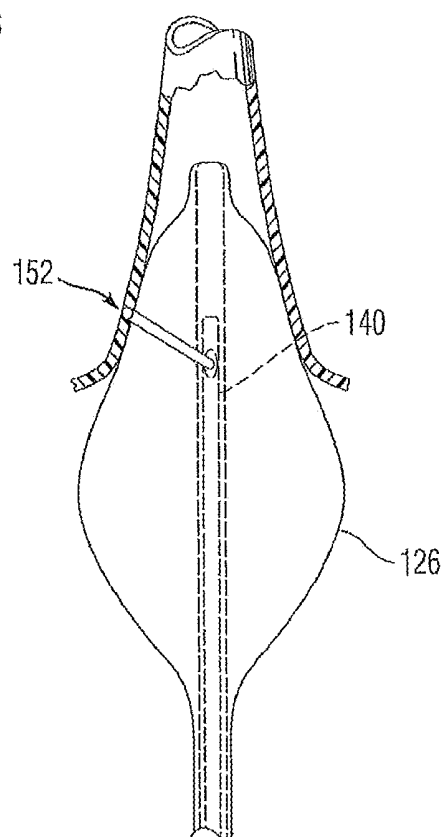


Fig. 6

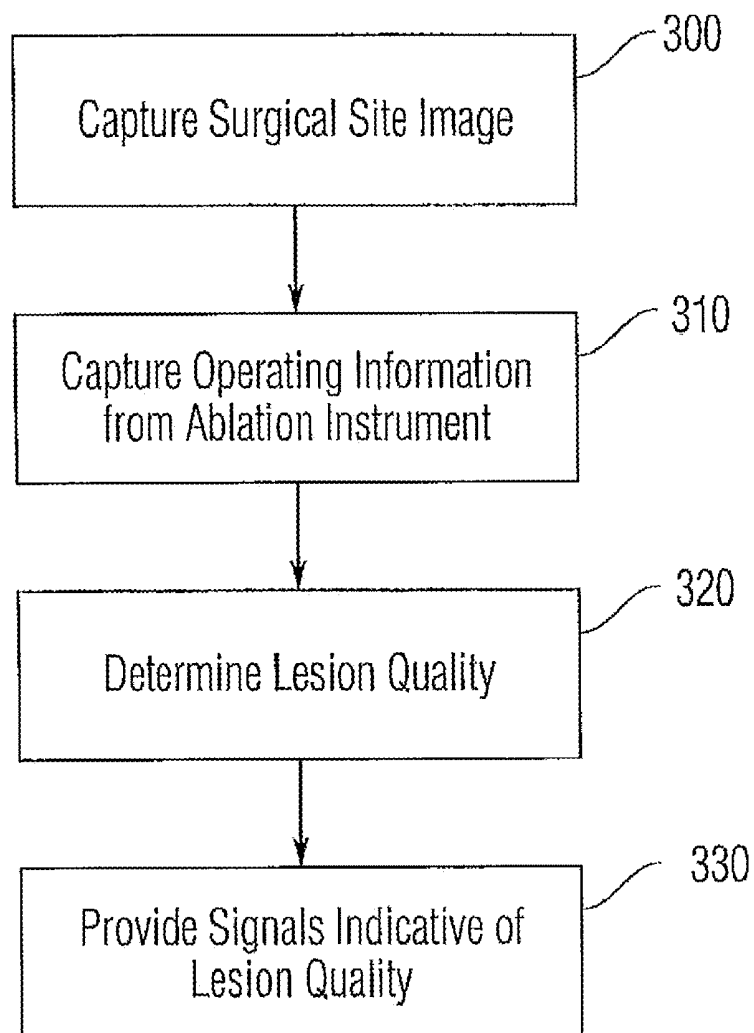


Fig. 7

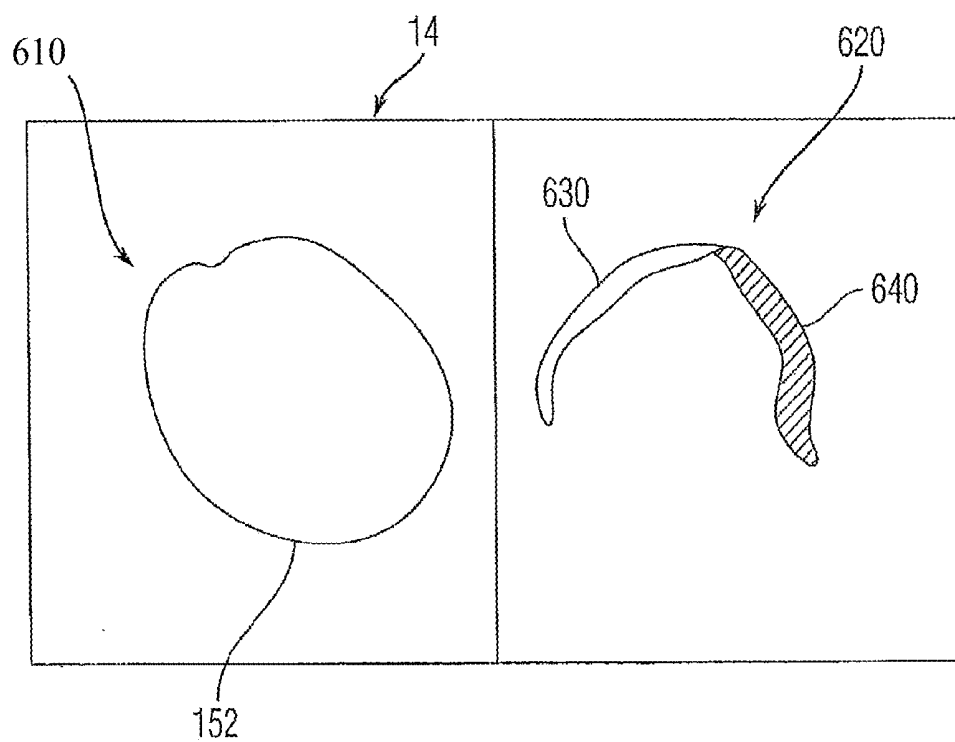


Fig. 8

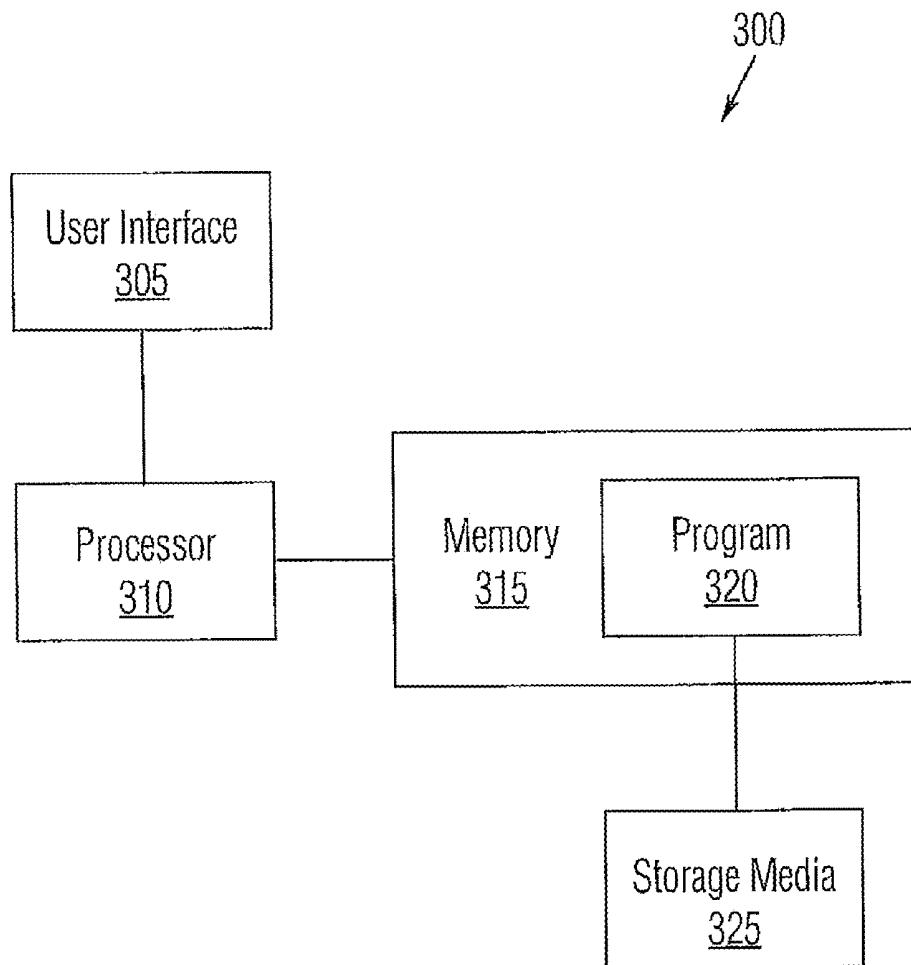


Fig. 9

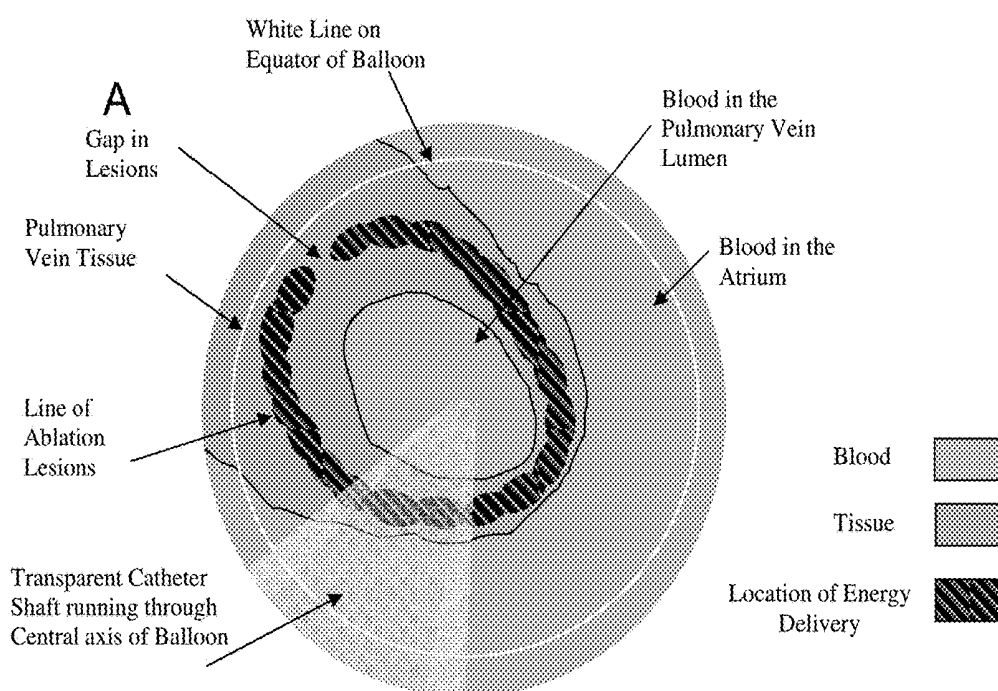


Fig. 10

METHOD FOR VISUALIZING TISSUE WITH AN ICG DYE COMPOSITION DURING ABLATION PROCEDURES

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application is a divisional of U.S. Non-Provisional patent application Ser. No. 14/697,065, filed on Apr. 27, 2015, which is based on and claims priority to U.S. Provisional Patent Application Ser. No. 61/985,142, filed on Apr. 28, 2014, all of which are incorporated by reference, as if expressly set forth in their respective entireties herein.

TECHNICAL FIELD

[0002] The present disclosure relates to ablation instruments and methods of use thereof, in particular to ablation catheters and methods for visualizing tissue using an ICG dye composition to identify and distinguish ablative tissue from de novo tissue.

BACKGROUND

[0003] Cardiac arrhythmias (e.g., fibrillation) are irregularities in the normal beating pattern of the heart and can manifest themselves in either the atria or the ventricles of the heart. For example, atrial fibrillation is a form of arrhythmia characterized by rapid randomized contractions of atrial myocardium, causing an irregular, often rapid ventricular rate. The regular pumping function of the atria is replaced by a disorganized, ineffective quivering as a result of chaotic conduction of electrical signals through the upper chambers of the heart. Atrial fibrillation is often associated with other forms of cardiovascular disease, including congestive heart failure, rheumatic heart disease, coronary artery disease, left ventricular hypertrophy, cardiomyopathy, or hypertension.

[0004] It is now understood that recurrent atrial fibrillation (paroxysmal and persistent) is triggered by rapidly firing tissue, (called "ectopic foci"), that are located in one or more of the four pulmonary veins, which attach to the rear of the left atrium. It has been found that atrial fibrillation may be cured by electrically isolating the pulmonary veins from the rest of the atrium.

[0005] Various techniques have been employed for pulmonary vein isolation. A common purpose of each of these techniques is to replace cardiac muscle cells with scar tissue, which scar tissue cannot conduct normal electrical activity within the heart.

[0006] In one known approach, circumferential ablation of tissue at the junction of the pulmonary veins and the left atrium has been practiced to treat atrial fibrillation. By ablating the heart tissue at selected locations, electrical conductivity from one segment to another can be blocked and the resulting segments become too small to sustain the fibrillatory process on their own.

[0007] Several types of ablation devices have recently been proposed for creating lesions to treat cardiac arrhythmias. Many of the recently proposed ablation instruments are percutaneous devices that are designed to create such lesions from within the heart. Such devices are positioned in the heart by catheterization of the patient, e.g., by passing the ablation instrument into the heart via a blood vessel, such as the femoral vein.

[0008] Typically, percutaneous devices are positioned with the assistance of a guide catheter and guide wire, which

are first advanced into heart. In one common approach, a guide catheter or similar guide device is advanced through the vasculature and into the left atrium of the heart. A guide wire is then advanced toward a pulmonary vein. A catheter instrument with an expandable element is then advanced through the guide catheter and over the guide wire and into the pulmonary vein where the expandable element (e.g., a balloon) is inflated. The balloon includes a circumferential ablation element, e.g., an energy emitting device, such as a laser, disposed in the inner surface of the balloon, which performs the ablation procedure.

[0009] It is noted that ablation near or within the pulmonary vein can result in complications. Overtreatment deep within a vein can result in stenosis (closure of the vein itself), necrosis or other structural damage, any of which can necessitate immediate open chest surgery. Conversely, undertreatment in which scar tissue formed is not continuous and/or insufficient to replace the cardiac muscles sought to be electrically isolated from the atrium will cause the surgical ablation procedure to be unsuccessful. Thus, repeating of the surgical ablation procedure is then required which is almost always undesirable.

[0010] Currently, when laser energy has been applied to a region of tissue at an ostium of the PV there is little to no visible change to that region of tissue when viewed through an endoscope thereby presenting the problem of distinguishing treated tissue (e.g., lesion) from de novo tissue.

[0011] The lesions are not visible for various reasons. For example, the ablation energy in these procedures typically penetrates deeply into the atrial tissue to create the lesion while leaving the endocardial surface relatively undamaged. Additionally, color video cameras are often not sensitive enough to discriminate the subtle color changes that distinguish treated and untreated tissue. Also, the light levels delivered to the site are limited since they typically travel to the treatment site via a small optical fiber thereby further hindering the ability of video cameras to visualize these distinctions.

[0012] Thus, there remains a need in the art for systems and methods configured to accurately and immediately discriminate lesions from de novo tissue, thereby allowing the user (surgeon or more specifically and electrophysiologist or interventional radiologist) to take corrective action in real time to ensure a complete lesion is formed.

SUMMARY

[0013] The present invention is directed to the use of an indocyanine green (ICG dye) composition as part of an imaging system for distinguishing lesions from de novo tissue. A tissue ablation system for identification of a lesion formed by directed energy emission at a surgical site of a patient includes a source of an indocyanine green (ICG dye) composition for delivery into a body of the patient including to the surgical site. The system further includes a tissue ablation instrument for use at the surgical site. The instrument includes a movable directed first energy emitter configured to emit a variable amount of directed energy for ablating tissue and forming a lesion at the surgical site. A second energy emitter is provided for applying energy of a type and in an amount sufficient to cause the ICG composition to fluoresce. The system further includes an imaging device that is configured to obtain an image of the surgical site while the ICG fluoresces with the lesion being visually identifiable relative to de-novo tissue based on a lack of

observable fluorescence at locations of the lesion, while the de-novo tissue is characterized by areas of fluorescence. A display, such as a computer monitor, displays the image in real time.

[0014] Since the formed lesion is immediately and readily visually distinguishable from the de novo tissue and blood due to the bright fluorescence of the de novo tissue and blood versus the formed lesion being characterized by a lack of fluorescence, the user (surgeon) can detect deficiencies in the lesion, such as gaps or breaks in the lesion, and take immediate corrective measures.

[0015] These and other aspects, features and benefits of the invention can be further appreciated from the accompanying drawings, which illustrate certain embodiments of the invention together with the detailed description thereof.

BRIEF DESCRIPTION OF THE DRAWINGS

[0016] The objects and features of the invention may be understood with reference to the following detailed description of an illustrative embodiment of the present invention taken together in conjunction with the accompanying drawings in which:

[0017] FIG. 1 is a block diagram depicting the components of an endoscope-guided cardiac ablation system according to the invention;

[0018] FIG. 2 is a schematic view of the of the cardiac ablation instrument of the cardiac ablation system of FIG. 1;

[0019] FIG. 3 is a block diagram of the processor modules used in the cardiac ablation instrument.

[0020] FIG. 4 illustrates a user interface in the form of a splint-screen arrangement for displaying information;

[0021] FIG. 5 is a schematic view of the cardiac ablation instrument of FIG. 2 shown in a treatment position at a surgical site in the pulmonary vein;

[0022] FIG. 6 is a schematic view of the cardiac ablation instrument of FIG. 2 with its compliant balloon inflated and its ablation element deployed at one of a plurality of locations;

[0023] FIG. 7 is a flow diagram illustrating the steps performed by the ablator system of FIG. 1 for determining the quality of lesions formed during a surgical ablation procedure;

[0024] FIG. 8 is a screen shot of the display of FIG. 1 depicting visual warning signals indicative of insufficient lesions;

[0025] FIG. 9 is a block diagram of a computer system configured to employ one ablation method of the present invention; and


[0026] FIG. 10 is a representative view of a treatment site from along a longitudinal axis of a catheter.

DETAILED DESCRIPTION OF CERTAIN EMBODIMENTS OF THE INVENTION

[0027] The present invention will now be described more fully with reference to the accompanying drawings, in which illustrated embodiments of the present invention are shown. The present invention is not limited in any way to any of the illustrated embodiments.

[0028] In accordance with the present invention and as described in detail below, a visualization system/method that uses ICG dye for distinguishing ablated tissue from de novo tissue.

[0029] Indocyanine green (ICG) is a cyanine dye used in medical diagnostics. ICG dye has the following formula:

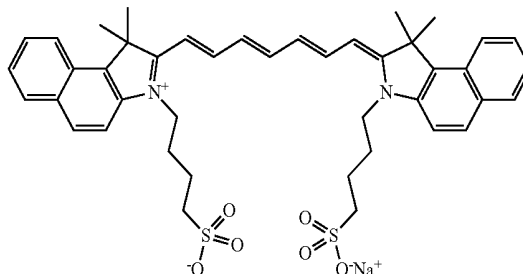

[0030] ICG dye is traditionally used for determining cardiac output, hepatic function, and liver blood flow, and for ophthalmic angiography. It has a peak spectral absorption at about 800 nm. These infrared frequencies penetrate retinal layers and other tissue allowing ICG angiography to image deeper patterns of circulation than fluorescein angiography. ICG binds tightly to plasma proteins and becomes confined to the vascular system. ICG has a half-life of 150 to 180 seconds and is removed from circulation exclusively by the liver to bile juice.

[0031] ICG is a fluorescent dye which is used in medicine as an indicator substance (e.g. for photometric hepatic function diagnostics and fluorescence angiography) in cardiac, circulatory, hepatic and ophthalmic conditions. ICG is typically administered intravenously and, depending on liver performance, is eliminated from the body with a half-life of approximately 3-4 minutes. ICG sodium salt is normally available in powder form and can be dissolved in various solvents; 5% (<5% depending on batch) sodium iodide is usually added to ensure better solubility. The sterile lyophilisate of a water-ICG solution is approved in many European countries and the United States under the names ICG-Pulsion and IC-Green as a diagnostic for intravenous use.

[0032] The absorption and fluorescence spectrum of ICG is in the near infrared region. Both depend to some degree on the solvent used and the concentration. ICG absorbs mainly between 600 nm and 900 nm and emits fluorescence between 750 nm and 950 nm. The large overlapping of the absorption and fluorescence spectra leads to a marked reabsorption of the fluorescence by ICG itself. The fluorescence spectrum is very wide. Its maximum values are approximately 810 nm in water and approximately 830 nm in blood. For medical applications based on absorption, the maximum absorption at approximately 800 nm (in blood plasma at low concentrations) is important. In combination with fluorescence detection, lasers with a wavelength of around 780 to 815 nm are used. At this wavelength, ICG still absorbs very well and yet it is still technically possible to suppress the excitation light in order to detect the fluorescence.

[0033] FIG. 1 is a schematic block diagram illustrating an ablator/endoscopic system in accordance with the invention, designated generally by reference numeral 10. Ablator system 10 preferably includes a surgical ablation instrument 100 preferably including an endoscope and ablation instrument as discussed below. The surgical ablation instrument 100 can be any number of different ablation instruments that are commercially available including those disclosed by Applicant in previous U.S. patents and patent applications (e.g., U.S. patent application publication Nos. 2009/

0326320 and 2011/0082451, each of which is hereby incorporated by reference in its entirety). In general, the ablation instrument **100** is of a type that emits ablation energy sufficient to cause formation of an ablation at a tissue target site.

[0034] The ablator system **10** further preferably includes an aiming light source **20** and an illumination light source **24**. A processor **12** designed to accept input and output data from the connected instruments, display and controller and process that data into visual information. Also included is an excitation light source **YY** that emits light in the wavelength range adequate to excite the ICG dye fluorescence. In some embodiments the illumination light source **24** may be identical to the excitation source **YY**. Alternatively the illumination light source **24** may provide a broadband white light illumination for normal endoscopic imaging and then be converted to an excitation light source by using an optical filter to remove wavelengths away from the absorption peak of ICG.

[0035] As will also be appreciated from the below discussion, an endoscope is preferably provided in ablation instrument **100** and has the capability of capturing both live images and recording still images. An illumination light is used to provide operating light to the surgical site. The illumination light is of a frequency that allows the user to differentiate between different tissues present at the operating site. An aiming light source **20** is used to visualize the location where energy will be delivered by the ablation instrument **100** to tissue. It is envisioned that the aiming light will be of a wavelength that can be recorded by an image capture device and visible on a display.

[0036] Composite Imaging System

[0037] The processor **12** is designed to process live visual data as well as data from the ablation instrument controllers and display. The processor is configured execute a series of software and/or hardware modules configured to interpret, manipulate and record visual information received from the surgical site. The processor **12** is further configured to manipulate and provide illustrative and graphical overlays and composite or hybrid visual data to the display device.

[0038] As seen in FIG. 1, the system **10** further includes a controller **16**, an energy source **18**, aiming light source **20** and a user interface **22**. Controller **16** is preferably configured to control the output of the energy source **18** and the illumination and excitation sources **24** and **25** of an energy transmitter as well as determine the distance and movement of an energy transmitter relative to tissue at an ablation surgical site (as discussed further below). As will also be appreciated from the below discussion, an endoscope is preferably supported by the ablation instrument **100** and captures images that can be processed by the processor **12** to determine whether sufficient ablative energy deliveries have been directed to a specific area of a surgical site. Data obtained from the endoscope includes real-time video or still images of the surgical site as seen from the ablation instrument.

[0039] The aiming light source **20** is used to visualize the surgical site location **120** where energy will be delivered by the ablation instrument **100** to tissue **130**. Preferably, the aiming light source **20** outputs light in a visible region of the electromagnetic spectrum. If a suitable ablation path is seen by the user, the controller **16** transmits radiant energy, via energy source **18**, from the ablation instrument **100** to a target tissue site **120** to effect ablation by lesions. It is to be

appreciated that the term “radiant energy” as used herein is intended to encompass energy sources that do not rely primarily on conductive or convective heat transfer. Such sources include, but are not limited to, acoustic, laser and electromagnetic radiation sources and, more specifically, include microwave, x-ray, gamma-ray, ultrasonic and radiant light sources. Additionally, the term “light” as used herein is intended to encompass electromagnetic radiation including, but not limited to, visible light, infrared and ultraviolet radiation.

[0040] The illumination light source **24** is a light source used to provide proper illumination to the surgical site. The illuminate is configured so that natural biological tones and hues can be easily identifiable by an operator.

[0041] The controller **16** can provide the user with the ability to control the function of the aiming light source, the user input devices, and the ablation instrument. The controller serves as the primary control interface for the ablation system. Through the controller, the user can turn on and off both the aiming and illumination lights. Furthermore the controller possesses the ability to change the illumination and aiming light intensity. The ability to switch user interfaces or display devices is also envisioned. Additionally, the controller gives access to the ablation instrument, including control over the intensity of the discharge, duration and location of ablative energy discharges. The controller **16** can further provide a safety shutoff to the system in the event that a clear transmission pathway between the radiant energy source and the target tissue is lost during energy delivery (e.g., see commonly owned U.S. patent application Ser. No. 12/896,010, filed Oct. 1, 2010, which is hereby incorporated by reference in its entirety).

[0042] The controller can be separate microprocessor based control interface hardware or it can be a portion of a configured as a module operating through a processor based computer system configured to accept and control inputs from various physical devices.

[0043] As shown in FIG. 3, a set of modules cooperate with one another to provide the information presented through the interface of the system of FIG. 1. Thus, for example, there is an analysis module **218**, a multiple view module **220**, a composite module **222**, a mapping module **224**, an illustrating module **226**, and a control interface module **228**. Each of these modules can comprise hardware, code executing in a processor, or both, that configures a machines such as a workstation to implement the functionality described herein.

[0044] With further reference to FIG. 3, the analysis module **218** includes instructions for analyzing a lesion and determining if it is sufficient for the desired treatment. The analysis module is configured to inspect the image data captured by the image capture device and a lesion of sufficient dimensions and quality has been formed. The analysis module **218** can be implemented as discrete sub-modules to provide functions such as receiving data on the duration and intensity of an ablative emission. An additional sub module is capable of evaluating the duration of the energy emission and comparing it to a look up table of sufficient duration and intensity values suitable to form a proper lesion.

[0045] The multiple view module **220** includes instructions for configuring the processor **12** to provide multiple images to the display. The multiple view module configures the display to depict at least two image depiction areas. In

a first image depiction area, the live video stream of the surgical site is displayed to the user. In a second image depiction area, a still image, highlighting the last target of ablative energy is depicted.

[0046] The composite module **222** includes instructions for combining a series of still images and producing a composite image that depicts the target location of the ablative emission in each still image. The compositing module **222** can be implemented as discrete sub-modules to provide functions such as altering the transparency of each still image layer of the composite image so that a time based map of ablation locations can be produced. Another function implemented by the submodules is construction of a video or slideshow from a sequence of still images.

[0047] The mapping module **224** includes instructions for overlaying proposed treatment paths on the live image. The mapping module is configured to show showing colored markers indicating acceptable levels of ablative energy depositing. For example the mapping module is capable of generating a green colored visual marker and superposing it over the live image to indicate areas that have yet to receive levels of ablative energy necessary for treatment. Conversely, the mapping module **224** is also capable of simultaneously generating a red colored (or other color) visual marker and superimposing it over the live image to indicate areas that have received sufficient quantities of ablative energy suitable lesions. The mapping module **224** can be implemented as discrete sub-modules to provide functions such as receiving data on the duration and intensity of an ablative emission and correlating that specific instance to a specific stored image.

[0048] The illustrating module **226** includes instructions for providing an image to the display, wherein the image is an illustration or graphical representation of the surgical site. The illustrating module **226** is configured to allow annotation of the illustrated image as well as comparison between the live image and the illustrated image. For example, and as shown in FIG. 8, display **14** provides a first screen portion **610** depicting the actual surgical site **152** as viewed from endoscope **176**. Display **14** also illustrates a second screen portion **620** illustrating a graphical depiction of the surgical site **152** indicating the actual path of the energy transmitter **140** on the tissue at the surgical site wherein the path consists of a trace indicating the sufficiency of the formed lesions in which a solid trace **630** indicates sufficient lesions and a hashed trace **640** indicates insufficient lesions.

[0049] The control module **220** includes instruction for orientating and accessing the functions of each of the other modules, as well as communicating with the controller and inputting information or manipulating the parameters of the data being displayed during operation. The manipulation and controlling functions can be implemented as discrete sub-modules with instructions for selecting operation modes, control interfaces, display orientation, recording modes, storage device location and data entry.

[0050] The user refers to the live video feed from the image capture device to determine where to direct a radiant energy transmission. Upon first use of the device, a live video image and a still image of the surgical site are depicted on the display. As seen in FIG. 4, the processor **12** outputs to the display **14** at least two separately defined image depiction areas **204**, **206**. One image depiction area **204** is reserved for displaying live video transmitted from the surgical site **152**. At least one other image depiction area **206**

is used to depict an image or a composite image comprised of several still images representing specific moments in time during the surgical procedure.

[0051] The live video shown to the user will allow the user to see the reflection of the aiming light **218** and hence direct ablative energy. It is envisioned that the first still image **210** depicted will be a still image captured at a point in time prior to the initiation of the first radiant energy emission. For instance, at a point in time prior to the emission of radiant energy, the image capture device records an image **210** of the surgical site **152** that depicts the surgical site **152** without the aiming light. By taking a still image **210** of the site, the user can record a baseline image of the surgical site before any treatment has been commenced. Furthermore, through the functions of the illustrative module, an illustration of the untouched **152** can be generated. During emission of radiant energy a still image **210** is taken of the surgical site **152**. The characteristics of the ablative event (e.g. information regarding the duration and intensity of the radiant of the energy emission) are stored and associated with the image depicting that specific emission. In addition, the reflection the aiming light will be visible in the still image, providing a location indicator as to where the energy was directed. A series of these still images can be combined by using the composite module. By modifying the opacity of each image, the reflected light of the aiming light for each ablative event will be visible in the composite image. In this way, a complete record **220** of where energy was directed will become available. Furthermore, because the composite image is composed a series of individual images representing a specific period of time during the procedure, a time based map of the entire operation can also be produced in real time or for subsequent review.

[0052] Also visible in FIG. 4 are control interfaces **216** for accessing the control module. The control interfaces allow the user to select image style and opacity as well and initiating the functions of the other modules. Furthermore the functions of the controller **16** are also controllable from the control interface.

[0053] It is to be appreciated the invention is not to be understood to be limited to the two image depiction areas discussed above with reference to FIG. 3 or 4, but rather may encompass any number of image depiction areas in which the images and representations of the surgical site **152** can be reviewed. With reference to FIG. 8 the images shown by the display **14** can be manipulated by the modules to illustrate the presence of sufficient or insufficient lesion formation. For instance, the display **14** may illustrate the image of the surgical site **152** viewed from the endoscope **176** wherein varying shades of grey and white depict tissue and lesions and in the event insufficient lesions are determined to be formed, or a red marker can be superimposed on the image of the surgical site **152** at the location where the insufficient lesion was determined. Coincidentally, an audio signal may also be emitted from ablator system **10** causing further warning to the user.

[0054] Therefore, if the user is not satisfied with the quality of the lesion produced, or the modules indicate that a sufficient lesion was not produced, the user can promptly redo the treatment of a specific tissue location (spot treatment). Conversely, if the modules indicate that a sufficient lesion was formed, the user can confidently move on to a new tissue location to continue the treatment thus saving time and effort by avoiding the need to more closely

examine the tissue location that was just treated. Hence, once the entire treatment is performed, the modules of the system permit the surgeon to view all treatment segments forming the entire ablation arc to see if a continuous, uninterrupted ablation has been formed (or see if the ablation has the intended, desired shape). If there are visible gaps or other imperfections with the formed ablation, the surgeon can move the energy transmitter **140** to the proper location for retreatment of these areas until the desired ablation is formed. The process can then be repeated to determine and confirm that the gap was eliminated.

[0055] As a result, the mapping, analyzing and illustrating functions performed by the ablation system of the present invention overcome the disadvantages associated with prior ablation surgical procedures and results in increased ablation success rates due to a more optimal and more accurate viewing and quality determination of the spot lesions created to form the continuous ablation at the tissue location for the surgical site **152**.

[0056] With reference now to FIG. 5, a description of ablation instrument **100** is provided. FIG. 5 provides a schematic, cross-sectional view of an ablation instrument **100**, including an elongate body **114**, a central lumen tubing **116** and a compliant balloon **126** inflatable via one or more ports **122** in the central tubing **116**. The central tubing **116** can also house an energy emitter that is capable of both axial movement and rotation within a lumen formed in the elongate body **114**. The energy emitter is also described herein as being an energy transmitter, an energy emitter (or lesion generator), a radiant energy emitter and a radiant energy transmitter (ablation element). Additionally formed in the elongated body **114** (also referred to herein as the catheter body) there can be a plurality of additional lumens, through which certain devices or instruments can be passed. For example, the catheter body **114** also provides lumens **118A** and **118B** for extraction (or circulation) of an inflation fluid, an endoscope **176** and illumination and excitation fibers **128A** and **128B**.

[0057] It should be understood that the embodiments illustrated in the drawings are only a few of the cardiac ablation instruments that can be utilized in accordance with the present invention. Further descriptions of other embodiments can be found, for example, in commonly owned, co-pending U.S. patent application Ser. No. 10/357,156, filed Feb. 3, 2003, U.S. patent application Ser. No. 09/924,393, filed Aug. 7, 2001, each of which is expressly incorporated by reference.

[0058] With reference now to FIGS. 5-6, the ablation instrument **100** is preferably designed such that upon disposition within the heart (e.g., proximal to a pulmonary vein), the balloon **126** can be inflated such that a shoulder portion **150** of the balloon **126** will be urged into close proximity with a target region **152** of cardiac tissue. As shown in FIG. 4, the energy emitter (or "lesion generator") **140** can be positioned to deliver ablative energy to the target region **152** to form a continuous lesion. The term "continuous" in the context of a lesion is intended to mean a lesion that substantially blocks electrical conduction between tissue segments on opposite sides of the lesion.

[0059] The radiant energy emitter **140** is shown in FIG. 2 disposed within the balloon **126** remotely from the target tissue (e.g., within a central lumen **116** of the catheter body **114** or otherwise disposed within the balloon). In one illustrated embodiment, the radiant energy transmitter (abla-

tion element) **140** includes at least one optical fiber coupled to a distal light projecting, optical element, which cooperate to project a spot of ablative light energy through the instrument **100** to the target site **152** (in FIG. 6). The catheter body **114**, projection balloon **126** and inflation/ablation fluids are all preferably substantially transparent to the radiant energy at the selected wavelength of the energy source as well as to the absorption and emission wavelengths of ICG dye to provide a low-loss transmission pathway from the radiant energy transmitter **140** to the target site **152**. It should be understood that the term "balloon" encompasses deformable hollow shapes which can be inflated into various configurations including spherical, obloid, tear drop, etc., shapes dependent upon the requirements of the body cavity. Such balloon elements can be elastic or simply capable of unfolding or unwrapping into an expanded state. The balloon can further encompass multiple chamber configurations.

[0060] Also disposed within the instrument **100** is a reflectance sensor, preferably an endoscope **176** capable of capturing an image of the target site **152** and/or the instrument position. The endoscope **176** is typically an optical fiber bundle with a lens or other optical coupler at its distal end to receive light. The reflectance sensor/endoscope can also include an illumination source, such one or more optical fibers coupled to a light source or sources. Alternatively illumination and excitation light may be delivered through separate optical fibers as indicated by **128A** in FIG. 2. Endoscopes are available commercially from various sources. The endoscope can further include an optical head assembly, as detailed in more detail below, to increase the field of view. In one illustrated embodiment, ablation element **140** and endoscope **176** are adapted for independent axial movement within the catheter body **14**.

[0061] The term "endoscope" as used herein is intended to encompass optical imaging devices, generally, including but not limited to endoscopes, fiberscopes, cardioscopes, angioscopes and other optical fiber-based imaging devices. More generally, "endoscope" encompasses any light-guiding (or waveguide) structure capable of transmitting an "image" of an object to a location for viewing, such as display **14**.

[0062] Preferably, spot lesions are formed at the target site **152** by applying radiant energy from the energy transmitter **140** to target tissue. The applied radiant energy may be applied in an energy range from about 50 Joules/cm² to about 1000 Joules/cm², or preferably from about 75 Joules/cm² to about 750 Joules/cm². The power levels applied by the energy emitter can range from about 10 Watts/cm² to about 150 Watts/cm² and the duration of energy delivery can range from about 1 second to about 1 minute, preferably from about 5 seconds to about 45 seconds, or more preferably from about 10 to about 30 seconds. For example, for power levels between 10 and 75 Watts/cm² it can be advantageous to apply the radiant energy for about 30 seconds. Lesser durations, e.g., of 10 to 20 seconds, can be used for power levels of 75 to 150 Watts/cm². It is to be understood the above figures are provided as examples and the energy, power and time duration figures set forth above are provided merely as examples and are not to be understood to be limited thereto.

[0063] In the illustrated embodiment of the ablation instrument **100** shown in FIGS. 5-6, the energy emitter **140** is a radiant energy emitter including at least one optical fiber coupled to a distal light projecting optical element, which cooperate to project a spot of ablative light energy through

the instrument **100** to the target site **152**. The optical element can further comprise one or more lens elements and/or refractive elements capable of projecting a spot or arc-shaped beam of radiation. Alternatively, the lesion generator may generate an annulus or partial ring of ablative radiation, as described in more detail in commonly owned U.S. Pat. No. 6,423,055 issued Jul. 22, 2002, herein incorporated by reference for its disclosure related thereto.

[0064] Since the radiant energy (e.g., a laser) emitted from the energy emitter **140** is typically outside the visual light spectrum that can be detected by the human eye, the ablation instrument **100** includes an aiming light preferably having a pulsed operating mode in which visible light from the aiming light unit is delivered in pulses to cause intermittent illumination of the tissue at the target site **152**. This gives the aiming light an appearance of being a blinking light. By delivering the visible aiming light in pulses, the surgeon is able to directly observe the tissue that is being treated at the target site **152**, using an endoscope, between the aiming light pulses.

[0065] During a surgical ablation procedure, the endoscope **176** is used to determine the extent of tissue ablation by sensing the change in color of the tissue as it is ablated and at a time when the aiming beam is in an off cycle via the display **14**. In other words, between the blinking (pulses) of the aiming light, the surgeon can observe the treated tissue to determine how the treatment is progressing since the endoscope **176** is used to determine the extent of tissue ablation by sensing the change in color of the tissue as it is ablated and at a time when the aiming beam is in an off cycle. However, many conditions may cause the actual detection of change in color of tissue being ablated to be difficult and/or unreliable in regards to whether proper spot lesions are formed by the energy transmitter **140** on the tissue at the ablation surgical site **152**. For instance, insufficient illumination at the surgical site **152** can make it difficult, if not impossible, to ascertain whether proper spot lesions were formed at the surgical site as viewed on display **14**.

[0066] The processor **12** of ablator system **10** obviates this problem by determining the quality of the lesion formed on the tissue at the target site **152** which may be viewed on monitor **14** and/or indicated to a surgeon visual overlay or audio cues. With reference now to the flow diagram of FIG. 7, the method of operation for determining the quality of spot lesions at an ablation surgical site **152** will now be discussed.

[0067] Starting at step **300**, the processor **12** captures the image from endoscope **176** of the tissue being ablated at the surgical site. At step **310**, the processor **12** also captures information relating to the energy transmitter **140** from controller **16**. The captured energy transmitter **140** information includes: the amount of radiant energy (power) applied by energy transmitter **140** on the tissue at the surgical site **152** to form spot lesions; the distance the energy transmitter **140** is from tissue to be ablated via spot lesions; and the rate of movement of energy transmitter **140** relative to the tissue at the surgical site **152**. It is to be appreciated that aforesaid information captured regarding energy transmitter **140** is not to be understood to be limited thereto as more or less information may be captured that is necessary to determine the quality of the spot lesions formed on the tissue at the surgical site.

[0068] The processor **12** then preferably uses algorithmic techniques to determine whether a sufficient spot lesion has just recently been formed on the tissue at the surgical site (step **320**). In other words, given the distance the energy transmitter **140** is located from the tissue at the surgical site **152**, the rate of movement of the energy transmitter **140** relative to the tissue at the surgical site **152** (e.g., the amount of time that energy is applied to the tissue at a given location), and the amount of energy being applied, a determination is made as to whether a sufficient spot lesion has been formed on the tissue at a location which the energy transmitter is applying ablation energy thereto. A lookup table or other similar means may also be used by processor **12** for determining the aforesaid lesion quality. A spot lesion is to be understood as being sufficient when it comprises enough scar tissue effective to block the transmission of electrical signals therethrough.

[0069] The processor **12** is preferably further operative and configured to provide a signal to the surgeon indicative of whether a sufficient spot lesion has been formed (step **330**). This indicative signal may be provided in the event an insufficient or no spot lesion was formed on the tissue at the surgical site **152** that was subject to the energy transmitter **140** dispersing energy thereto. This indicative signal may be an audio and/or visual signal. The audio signal may consist of a warning tone and the visual signal may consist of a marker (e.g., color red) superimposed on the display **14** illustrating the surgical site **152** (provided via endoscope **176**) at the location at which the insufficient spot lesion was determined. Thus, when image processor **12** determines an insufficient spot lesion has been formed, the aforesaid warning signal is promptly provided to the surgeon enabling the surgeon to revisit the tissue having the insufficient lesion and make proper adjustments with the energy transmitter **140** (e.g., apply more energy, close the distance between energy transmitter **140** and the surgical site and/or slow the movement of energy transmitter **140** relative to the surgical site) so as to now form sufficient lesions.

[0070] FIG. 9 is a block diagram of one computer system **300** configured for employment of method **100**. System **300** includes a user interface **305**, a processor **310**, and a memory **315**. System **300** may be implemented on a general purpose microcomputer, such as one of the members of the Sun® Microsystems family of computer systems, one of the members of the IBM® Personal Computer family, one of the members of the Apple® Computer family, or a myriad of other conventional workstations. Although system **300** is represented herein as a standalone system, it is not limited to such, but instead can be coupled to other computer systems via a network (not shown).

[0071] Memory **315** is a memory for storing data and instructions suitable for controlling the operation of processor **310**. An implementation of memory **315** would include a random access memory (RAM), a hard drive and a read only memory (ROM). One of the components stored in memory **315** is a program **320**.

[0072] Program **320** includes instructions for controlling processor **310** to execute method **100**. Program **320** may be implemented as a single module or as a plurality of modules that operate in cooperation with one another. Program **320** is contemplated as representing a software embodiment of the method described hereinabove.

[0073] User interface **305** includes an input device, such as a keyboard, touch screen, tablet, or speech recognition

subsystem, for enabling a user to communicate information and command selections to processor 310. User interface 305 also includes an output device such as a display or a printer. In the case of a touch screen, the input and output functions are provided by the same structure. A cursor control such as a mouse, track-ball, or joy stick, allows the user to manipulate a cursor on the display for communicating additional information and command selections to processor 310.

[0074] While program 320 is indicated as already loaded into memory 315, it may be configured on a storage media 325 for subsequent loading into memory 315. Storage media 325 can be any conventional storage media such as a magnetic tape, an optical storage media, a compact disc, or a floppy disc. Alternatively, storage media 325 can be a random access memory, or other type of electronic storage, located on a remote storage system.

[0075] The methods described herein have been indicated in connection with flow diagrams that facilitate a description of the principal processes; however, certain blocks can be invoked in an arbitrary order, such as when the events drive the program flow such as in an object-oriented program. Accordingly, the flow diagram is to be understood as an example flow and that the blocks can be invoked in a different order than as illustrated.

[0076] It should be understood that various combination, alternatives and modifications of the present invention could be devised by those skilled in the art. The present invention is intended to embrace all such alternatives, modifications and variances that fall within the scope of the appended claims.

[0077] Although described in connection with cardiac ablation procedures, it should be clear that the instruments and systems of the present invention can be used for a variety of other procedures where treatment with radiant energy is desirable, including laparoscopic, endoluminal, perivisceral, endoscopic, thoracoscopic, intra-articular and hybrid approaches.

[0078] Use of ICG Dye for Visualization of Treated Tissue

[0079] In accordance with the present invention, an ICG dye composition is used for visualizing ablated tissue and allowing the ablated tissue to be visually distinguished from de-novo tissue.

[0080] A suitable and biologically sufficient amount of ICG dye is delivered to the patient either immediately prior to performing the ablation procedure; during the ablative procedure or immediately after the ablation procedure. The timing and time period for delivering the ICG dye is sufficient to allow the ICG dye to travel through the bloodstream to the ablation tissue site where the ICG dye binds to plasma proteins and permit visualization of the ablated tissue since the ablated tissue (a lesion) is visually distinguishable from de novo tissue (non-ablated tissue) as a result of the binding properties of the ICG dye.

[0081] Accordingly, after the ICG dye is injected into the patient's arm (e.g., through an IV) or is otherwise delivered into the patient, it travels through the bloodstream to the target tissue in less than 1 minute (e.g., in about 15 to 20 seconds). As discussed herein, one of the properties of the ICG dye is that it binds to blood plasma protein and therefore, any tissue that absorbs the ICG dye (e.g., ICG binds with blood plasma protein) is readily distinguishable from tissue that does not absorb the ICG dye due to the difference in observable fluorescence.

[0082] As is understood, ablated tissue is tissue which has undergone coagulative necrosis due to energy being applied to the tissue. Unlike, the surrounding de-novo tissue, the ablated tissue does not have blood flowing therein and therefore, the ICG dye bound to blood plasma protein is carried into the ablated tissue to a far lesser extent than it is carried into de novo tissue. The result is that the ablated tissue does not absorb the ICG dye and is thus marked by a lack of fluorescence.

[0083] FIG. 10 is a representative endoscopic view of a treatment site from along a longitudinal axis of the catheter. This view is preferably displayed on a display, such as a monitor and the ablated tissue is displayed in a visually distinguished manner relative to the de-novo (untreated) tissue. In particular and as a result of the use of the ICG dye, areas that contain blood (such as blood in the pulmonary vein lumen and blood in the atrium, etc.) are represented by high levels of fluorescence (which is graphically represented in the figure), while the area of the ablated tissue has a darker appearance due to a lack of ICG dye. In other words, the ablated tissue is easily distinguishable from the surrounding blood rich areas since the areas of ablated tissue lack the fluorescence that is exhibited in the blood rich areas.

[0084] In FIG. 10, the areas of blood/tissue are visually differentiated from the locations of the energy delivery (the formation of the lesions) by the use of cross-hatching. The catheter shaft and are also visually distinguished from the blood/tissue and the lesions (by cross-hatching). As discussed herein, in FIG. 10, the cross-hatched areas that denote blood/tissue are the areas of fluorescence when the appropriate energy is applied to the surgical site to cause the area to fluoresce

[0085] The ablation system 10 described herein is modified by the inclusion of an excitation light that emits light at the proper excitation wavelength (e.g., about 805 nm) instead of the use of a white light that is used in other ablation procedures. The device also includes an imaging device, such as a camera or the like, which includes appropriate filters and is constructed to be able to detect and record near IR light near the peak of the ICG emission spectra (i.e., about 835 nm) on out to the limit of the ICG dye fluorescence spectrum (i.e. 880 nm) while filtering out all of the excitation light to allow the emitted fluorescence to be visible as shown in FIG. 10).

[0086] The principle of fluorescence imaging using ICG dye involves the following steps. The tissue of interest is illuminated at a selected excitation wavelength (about 750 nm to about 805 nm) while observing it at longer emission wavelengths (e.g., over 815 nm in the case of 805 nm excitation). Filters are preferably used as part of the imaging device to prevent mixing of the excitation (strong) and fluorescing (weak) rays to sum at a sensor or the like that is part of the overall imaging system. Even if the fluorescence is only a small fraction of the excitation intensity, a surprisingly good signal to noise ratio (SNR) is attached. A brightly fluorescing object (mostly blood and well perfused tissue) can be seen on a display. Without the use of filters, a weak fluorescence image cannot be seen among the strong reflection of the excitation light.

[0087] ICG fluoresces at about 800 nm and longer wavelengths. The exact shape of the observed spectra can depend somewhat on the chemical environment and physical conditions of the ICG molecules like temperature and ICG

concentration as well as the absorption spectra of the tissue through which some of the emitted light must pass.

[0088] One of the advantageous properties of ICG is the fast binding to plasma proteins, especially lipoproteins, makes repeated intraoperational applications of ICG possible. The binding to plasma proteins does not alter the protein structures, which is one sign of nontoxicity. It is believed that ICG binds to the lipids of lipoprotein complexes (β -lipoprotein), and that the bind results in more intense fluorescence than ICG bound to for example, free cholesterol. Binding to protein proteins also shifts, slowly, taking several minutes, the absorption peak, at 780 nm, toward longer wavelengths, to 805 nm. It has been reported that absorption peak maximum was observed at 810 nm in the epidermal cell cultures, and at 805-810 nm in the human skin in vivo. The emission peak is also shifted similarly.

[0089] The Imaging System

[0090] The imaging system in accordance with the present invention includes an appropriate imaging device that is configured to monitor, in real time, the condition of the tissue at the surgical site and in particular, allow the physician to readily distinguish between ablated tissue and de novo tissue that has not been ablated. The imaging system allows the observed image to be displayed in real-time on a display and/or recorded and stored in memory.

[0091] An endoscope can be used to obtain an image of the ablated tissue as described herein. The endoscope is inserted into the body and positioned adjacent the area of interest. An instrument is then used in combination with the endoscope to provide energy at an appropriate wavelength to cause the ICG dye within the subject tissue to fluoresce so that the image can be obtained. Similarly, a second instrument can be used with the endoscope that permits the image of the fluorescing ICG dye within the tissue to be obtained. For example, an optical device is connected to a CCD camera can be used in conjunction with the endoscopic procedures of the present invention. The optical device and the CCD camera permits the physician to view the target tissue in the heart. When the imaging device is in the form of a CCD camera, the device includes software and equipment that effectively filters light (reflected light) of certain wavelength (s) and in particular, the imaging device can include one or more video chips and corresponding bandpass filters and/or other filter arrangements that allow the fluorescence emission of the ICG dye to be filtered out and then further processed. As is known, a traditional filter (e.g., a bandpass filter) can be tailored to a specific waveband of a certain width and is centered at a specific wavelength (i.e., the fluorescence emission).

[0092] Combined Visible and Fluorescence Images

[0093] According to one embodiment, fluorescence imaging can be done so that both visible or excitation and fluorescence images are displayed together as one image. The fluorescence image along may contain only a few details so that the visible image greatly helps to locate the fluorescing parts with the help of landmarks seen in the visible image. Typically, the fluorescence channel is shown, rendered, in colors like vivid green, having a striking color contrast to the visible image of tissues. The type of visualization is especially important in intraoperational use, where the fluorescing parts, like blood veins and healthy de novo tissue, should be recognized easily and immediately. Image registration software can then be used to combine the two images in proper alignment.

[0094] Review of Ablation Quality

[0095] The present invention thus allows the surgeon to view the formed ablation(s) (lesion) in real-time and to evaluate the quality of the formed ablation(s) to allow the surgeon to decide whether additional ablation treatment is needed. For example, if the surgeon views the display and notices that the formed ablation(s) includes a defect, such as a void (gap or break) along its length, or is otherwise not acceptable, then the **[text missing or illegible when filed]**

[0096] A gap formed along the length of the lesion is readily recognizable since the area of the gap will exhibit fluorescence, while the other sections of the lesion lack fluorescence and appear dark. In FIG. 10, a gap (break) A is present in the lesion and is readily and immediately discoverable by the surgeon when viewing the display due to the fact that the area A (the gap area) fluoresces, while the lesion has a dark color on the display. Thus, holes/gaps located along the lesion are easily seen due to these areas appearing as fluorescent "hot spots" relative to the adjacent dark areas which represent the formed lesion(s).

[0097] After viewing the display, the surgeon can then further ablate the tissue to close off the gap or otherwise correct the formed ablation such that a complete ablation is formed as desired. The surgeon can then check the video display after performing such additional ablation to make sure that the lesion is complete as represented by a continuous dark segment (lack of fluorescence) on the video display. In other words, once corrective action is taken and these fluorescent "hot spots" are eliminated by ablating the tissue at such location, the "hot spots" will disappear. The vivid fluorescent colors that indicate the lack of ablated tissue and instead show areas of blood flow and de-novo tissue allow the surgeon in real-time to see deficiencies in the formed lesion (ablation) and take immediate corrective action, thereby ensuring that the lesion (ablation) is fully formed and will act to block electrical signals as desired.

[0098] U.S. patent application publication No. 2009/0326320 discloses other details of exemplary imaging systems and is hereby incorporated by reference in its entirety. It will be understood that one or more of the features disclosed in that document can be implemented in the imaging system of the present invention in that the imaging system can include more than one means for visualizing the surgical site and providing the user (surgeon) with helpful feedback and information concerning the quality of the lesion (i.e., whether the lesion is a continuous, uninterrupted structure, etc.).

[0099] One skilled in the art will appreciate further features and advantages of the invention based on the above-described embodiments. Accordingly, the invention is not to be limited by what has been particularly shown and described, except as indicated by the appended claims. All publications and references cited herein are expressly incorporated herein by reference in their entirety.

What is claimed:

1. A method for distinguishing lesions from de novo tissue comprising the steps of:

- administering an ICG composition to the patient;
- forming one or more lesions at a surgical site;
- applying energy of a type and in an amount sufficient to cause ICG in the patient to fluoresce;
- obtaining an image of the tissue and lesion at the surgical site while the ICG fluoresces; and

distinguishing the lesion from surrounding de novo tissue based on areas of fluorescence to allow a user to evaluate the quality of the lesion.

2. The method of claim 1, wherein areas of the lesion are characterized by a lack of fluorescence.

3. The method of claim 1, wherein blood and the de novo tissue are characterized by areas of fluorescence.

4. The method of claim 1, wherein the step of applying energy comprises applying light that has a wavelength that is sufficient to cause the ICG to fluoresce.

5. The method of claim 1, wherein the image is in real-time.

6. The method of claim 1, further including the step of ablating tissue to complete the lesion in one or more areas of fluorescence along the lesion which represent breaks or gaps in the lesion.

7. The method of claim 1, further including the step of filtering light that is captured by an imaging device to limit the light to a wavelength at which ICG fluoresces.

8. The method of claim 1, further including the step of processing the filtered light to produce the image.

9. The method of claim 7, wherein the wavelength is about 805 nm.

10. The method of claim 1, wherein a common ablation instrument includes both an energy emitter for forming the lesion and a light beam for applying energy of the type and in the amount sufficient to cause the ICG composition to fluoresce.

11. The method of claim 1, wherein the quality of the lesion is evaluating by evaluating whether a continuous ablation ring is formed in the tissue as depicted by a lack of fluorescence along the continuous ablation ring; wherein an image processor receives the images from endoscope of the surgical site and is configured to combine both visible light images of the surgical site which show anatomical landmarks with fluorescence images obtained with excitation light used to cause ICG in the patient to fluoresce and display the combined images as a single combined image.

* * * * *

专利名称(译)	在消融手术期间用ICG染料组合物使组织可视化的方法		
公开(公告)号	US20190150718A1	公开(公告)日	2019-05-23
申请号	US16/259483	申请日	2019-01-28
[标]申请(专利权)人(译)	卡迪奥福克斯有限公司		
申请(专利权)人(译)	CARDIOFOCUS INC.		
当前申请(专利权)人(译)	CARDIOFOCUS INC.		
[标]发明人	MELSKY GERALD		
发明人	MELSKY, GERALD		
IPC分类号	A61B1/04 A61B5/00 A61B18/20 A61B1/06		
CPC分类号	A61B1/043 A61B5/0071 A61B5/0084 A61B5/4836 A61B18/20 A61B1/0638 A61B2090/373 A61B2018/00577 A61B2017/00061 A61B90/361 A61B2090/376 A61B2090/3941 A61B1/0005 A61B2018/00982 A61B90/30 A61B5/0036		
优先权	61/985142 2014-04-28 US		
外部链接	Espacenet USPTO		

摘要(译)

提供了一种用于识别组织消融手术期间形成的损伤的充分性的系统。该系统和方法包括向患者施用ICG组合物并在手术部位形成一个或多个损伤。该方法还包括施加足以使患者中的ICG发荧光的类型和量的能量。在ICG发荧光的同时获得手术部位处的组织和病变的图像。基于荧光区域将病变与周围的从头组织区分开以允许用户评估病变的质量。

