



US009788735B2

(12) **United States Patent**  
**Al-Ali**

(10) **Patent No.:** **US 9,788,735 B2**  
(45) **Date of Patent:** **\*Oct. 17, 2017**

(54) **BODY WORN MOBILE MEDICAL PATIENT MONITOR**

(71) Applicant: **MASIMO CORPORATION**, Irvine,  
CA (US)

(72) Inventor: **Ammar Al-Ali**, San Juan Capistrano,  
CA (US)

(73) Assignee: **MASIMO CORPORATION**, Irvine,  
CA (US)

(\*) Notice: Subject to any disclaimer, the term of this  
patent is extended or adjusted under 35  
U.S.C. 154(b) by 0 days.

This patent is subject to a terminal dis-  
claimer.

(21) Appl. No.: **15/499,619**

(22) Filed: **Apr. 27, 2017**

(65) **Prior Publication Data**

US 2017/0224233 A1 Aug. 10, 2017

**Related U.S. Application Data**

(63) Continuation of application No. 15/448,989, filed on  
Mar. 3, 2017, which is a continuation of application  
(Continued)

(51) **Int. Cl.**  
**A61B 5/1455** (2006.01)  
**A61B 5/0205** (2006.01)  
(Continued)

(52) **U.S. Cl.**  
CPC ..... **A61B 5/0205** (2013.01); **A61B 5/0024**  
(2013.01); **A61B 5/021** (2013.01);  
(Continued)

(58) **Field of Classification Search**  
CPC ... A61B 5/0002; A61B 5/0004; A61B 5/0024;  
A61B 5/02; A61B 5/0205; A61B 5/0402;  
(Continued)

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

3,646,606 A 2/1972 Buxton et al.  
3,690,313 A 9/1972 Weppner et al.  
(Continued)

**FOREIGN PATENT DOCUMENTS**

EP 0602459 6/1994  
EP 0 735 499 10/1996  
(Continued)

**OTHER PUBLICATIONS**

US 8,845,543, 09/2014, Diab et al. (withdrawn)  
(Continued)


*Primary Examiner* — Eric Winakur

(74) *Attorney, Agent, or Firm* — Knobbe Martens Olson  
& Bear LLP

(57) **ABSTRACT**

A body worn mobile medical monitoring device configured to minimize cable wiring from a sensor by placement of one or more sensor communication ports. The body worn mobile medical monitoring device includes a housing securable on a lower arm of a patient, a display, and a sensor communication port positioned on a side of the housing and configured to face a hand of the lower arm of the patient when the mobile medical monitoring device is mounted to the lower arm of the patient. The sensor communication port provides wired communication with a pulse oximetry sensor attached to a digit of the hand of the patient, and is positioned on the side of the housing such that a path from the port on the side of the housing to the digit of the patient is shorter than any other path from any other side of the housing to the digit.

**20 Claims, 17 Drawing Sheets**

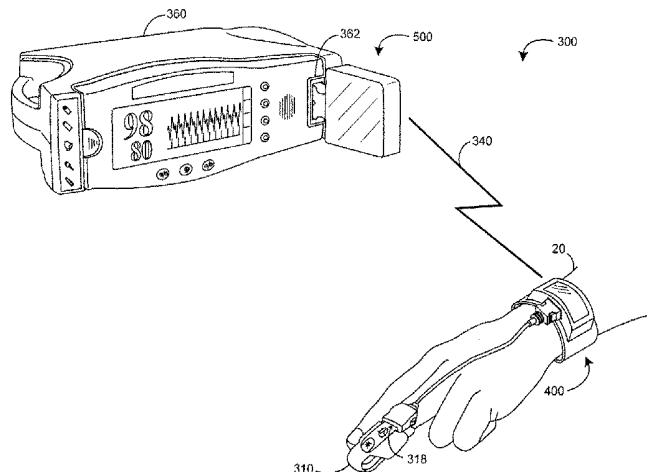

**Related U.S. Application Data**

- No. 14/815,232, filed on Jul. 31, 2015, now abandoned, which is a continuation of application No. 14/217,788, filed on Mar. 18, 2014, now Pat. No. 9,113,832, which is a continuation of application No. 14/037,137, filed on Sep. 25, 2013, now Pat. No. 9,113,831, which is a continuation of application No. 12/955,826, filed on Nov. 29, 2010, now Pat. No. 8,548,548, which is a continuation of application No. 11/417,006, filed on May 3, 2006, now Pat. No. 7,844,315, which is a continuation of application No. 11/048,330, filed on Feb. 1, 2005, now Pat. No. 7,844,314, which is a continuation of application No. 10/377,933, filed on Feb. 28, 2003, now Pat. No. 6,850,788.
- (60) Provisional application No. 60/367,428, filed on Mar. 25, 2002.
- (51) **Int. Cl.**  
*A61B 5/00* (2006.01)  
*A61B 5/021* (2006.01)  
*A61B 5/0404* (2006.01)
- (52) **U.S. Cl.**  
 CPC ..... *A61B 5/0404* (2013.01); *A61B 5/14552* (2013.01); *A61B 5/6824* (2013.01); *A61B 5/6826* (2013.01); *A61B 5/6831* (2013.01); *A61B 2562/222* (2013.01); *A61B 2562/227* (2013.01)
- (58) **Field of Classification Search**  
 CPC . A61B 5/1455; A61B 5/14551; A61B 5/6825; A61B 5/6826; A61B 5/6831; A61B 5/72; A61B 2560/0443; A61B 2562/06  
 See application file for complete search history.

**(56) References Cited**

## U.S. PATENT DOCUMENTS

|             |         |                    |             |         |                          |
|-------------|---------|--------------------|-------------|---------|--------------------------|
| 3,810,102 A | 5/1974  | Parks, III et al.  | 5,333,106 A | 7/1994  | Lanpher et al.           |
| 3,815,583 A | 6/1974  | Scheidt            | 5,337,744 A | 8/1994  | Branigan                 |
| 3,972,320 A | 8/1976  | Kalman             | 5,341,805 A | 8/1994  | Stavridi et al.          |
| 3,978,849 A | 9/1976  | Geneen             | 5,348,008 A | 9/1994  | Bornn et al.             |
| 4,013,067 A | 3/1977  | Kresse et al.      | 5,358,519 A | 10/1994 | Grandjean                |
| 4,108,166 A | 8/1978  | Schmid             | D353,195 S  | 12/1994 | Savage et al.            |
| 4,231,354 A | 11/1980 | Kurtz et al.       | D353,196 S  | 12/1994 | Savage et al.            |
| 4,589,415 A | 5/1986  | Haaga              | 5,375,599 A | 12/1994 | Shimizu                  |
| 4,662,378 A | 5/1987  | Thomis             | 5,375,604 A | 12/1994 | Kelly et al.             |
| 4,773,422 A | 9/1988  | Isaacson et al.    | 5,377,676 A | 1/1995  | Vari et al.              |
| 4,838,275 A | 6/1989  | Lee                | 5,392,777 A | 2/1995  | Swedlow et al.           |
| 4,852,570 A | 8/1989  | Levine             | 5,400,794 A | 3/1995  | Gorman                   |
| 4,960,128 A | 10/1990 | Gordon et al.      | D357,982 S  | 5/1995  | Dahl et al.              |
| 4,964,408 A | 10/1990 | Hink et al.        | 5,416,695 A | 5/1995  | Stutman et al.           |
| RE33,643 E  | 7/1991  | Isaacson et al.    | 5,417,222 A | 5/1995  | Dempsey et al.           |
| 5,041,187 A | 8/1991  | Hink et al.        | D359,546 S  | 6/1995  | Savage et al.            |
| 5,069,213 A | 12/1991 | Polczynski         | 5,431,170 A | 7/1995  | Mathews                  |
| 5,090,410 A | 2/1992  | Saper et al.       | 5,434,611 A | 7/1995  | Tamura                   |
| 5,092,340 A | 3/1992  | Yamaguchi et al.   | D361,840 S  | 8/1995  | Savage et al.            |
| 5,140,519 A | 8/1992  | Friesdorf et al.   | D362,063 S  | 9/1995  | Savage et al.            |
| 5,159,932 A | 11/1992 | Zanetti et al.     | 5,452,717 A | 9/1995  | Branigan et al.          |
| 5,161,539 A | 11/1992 | Evans et al.       | D363,120 S  | 10/1995 | Savage et al.            |
| 5,163,438 A | 11/1992 | Gordon et al.      | 5,456,252 A | 10/1995 | Vari et al.              |
| 5,203,342 A | 4/1993  | Sakai              | 5,479,934 A | 1/1996  | Imran                    |
| 5,262,944 A | 11/1993 | Weisner et al.     | 5,482,036 A | 1/1996  | Diab et al.              |
| 5,277,189 A | 1/1994  | Jacobs             | 5,483,968 A | 1/1996  | Adam et al.              |
| 5,278,627 A | 1/1994  | Aoyagi et al.      | 5,490,505 A | 2/1996  | Diab et al.              |
| 5,282,474 A | 2/1994  | Valdes Sosa et al. | 5,490,523 A | 2/1996  | Isaacson et al.          |
| 5,296,688 A | 3/1994  | Hamilton et al.    | 5,494,041 A | 2/1996  | Wilk                     |
| 5,318,037 A | 6/1994  | Evans et al.       | 5,494,043 A | 2/1996  | O'Sullivan et al.        |
| 5,319,355 A | 6/1994  | Russek             | 5,503,149 A | 4/1996  | Beavin                   |
| 5,331,549 A | 7/1994  | Crawford, Jr.      | 5,505,202 A | 4/1996  | Mogi et al.              |
|             |         |                    | 5,511,553 A | 4/1996  | Segalowitz               |
|             |         |                    | 5,533,511 A | 7/1996  | Kaspari et al.           |
|             |         |                    | 5,534,851 A | 7/1996  | Russek                   |
|             |         |                    | 5,537,289 A | 7/1996  | Dahl                     |
|             |         |                    | 5,544,649 A | 8/1996  | David et al.             |
|             |         |                    | 5,553,609 A | 9/1996  | Chen et al.              |
|             |         |                    | 5,558,638 A | 9/1996  | Evers et al.             |
|             |         |                    | 5,561,275 A | 10/1996 | Savage et al.            |
|             |         |                    | 5,562,002 A | 10/1996 | Lalin                    |
|             |         |                    | 5,566,676 A | 10/1996 | Rosenfeldt et al.        |
|             |         |                    | 5,576,952 A | 11/1996 | Stutman et al.           |
|             |         |                    | 5,579,001 A | 11/1996 | Dempsey et al.           |
|             |         |                    | 5,584,296 A | 12/1996 | Cui et al.               |
|             |         |                    | 5,590,649 A | 1/1997  | Caro et al.              |
|             |         |                    | 5,602,924 A | 2/1997  | Durand et al.            |
|             |         |                    | 5,619,991 A | 4/1997  | Sloane                   |
|             |         |                    | 5,632,272 A | 5/1997  | Diab et al.              |
|             |         |                    | 5,638,816 A | 6/1997  | Kiani-Azarbayjany et al. |
|             |         |                    | 5,638,818 A | 6/1997  | Diab et al.              |
|             |         |                    | 5,640,967 A | 6/1997  | Fine et al.              |
|             |         |                    | 5,645,440 A | 7/1997  | Tobler et al.            |
|             |         |                    | 5,658,316 A | 8/1997  | Lamond et al.            |
|             |         |                    | 5,673,692 A | 10/1997 | Schulze et al.           |
|             |         |                    | 5,685,299 A | 11/1997 | Diab et al.              |
|             |         |                    | 5,685,314 A | 11/1997 | Geheb et al.             |
|             |         |                    | 5,687,717 A | 11/1997 | Halpern et al.           |
|             |         |                    | 5,694,020 A | 12/1997 | Lang et al.              |
|             |         |                    | 5,724,580 A | 3/1998  | Levin et al.             |
|             |         |                    | 5,724,983 A | 3/1998  | Selker et al.            |
|             |         |                    | 5,725,308 A | 3/1998  | Smith et al.             |
|             |         |                    | 5,734,739 A | 3/1998  | Sheehan et al.           |
|             |         |                    | D393,830 S  | 4/1998  | Tobler et al.            |
|             |         |                    | 5,743,262 A | 4/1998  | Lepper, Jr. et al.       |
|             |         |                    | 5,746,697 A | 5/1998  | Swedlow et al.           |
|             |         |                    | 5,758,079 A | 5/1998  | Ludwig et al.            |
|             |         |                    | 5,758,644 A | 6/1998  | Diab et al.              |
|             |         |                    | 5,760,910 A | 6/1998  | Lepper, Jr. et al.       |
|             |         |                    | 5,769,785 A | 6/1998  | Diab et al.              |
|             |         |                    | 5,772,585 A | 6/1998  | Lavin et al.             |
|             |         |                    | 5,779,631 A | 7/1998  | Chance                   |
|             |         |                    | 5,782,757 A | 7/1998  | Diab et al.              |
|             |         |                    | 5,782,805 A | 7/1998  | Meinzer                  |
|             |         |                    | 5,785,659 A | 7/1998  | Caro et al.              |
|             |         |                    | 5,791,347 A | 8/1998  | Flaherty et al.          |
|             |         |                    | 5,792,052 A | 8/1998  | Isaacson et al.          |
|             |         |                    | 5,800,349 A | 9/1998  | Isaacson et al.          |
|             |         |                    | 5,801,637 A | 9/1998  | Lomholt Ole              |

(56)

## References Cited

## U.S. PATENT DOCUMENTS

|              |         |                          |                |         |                                     |
|--------------|---------|--------------------------|----------------|---------|-------------------------------------|
| 5,810,734 A  | 9/1998  | Caro et al.              | 6,206,830 B1   | 3/2001  | Diab et al.                         |
| 5,813,403 A  | 9/1998  | Soller et al.            | 6,215,403 B1   | 4/2001  | Chan et al.                         |
| 5,822,544 A  | 10/1998 | Chaco et al.             | 6,221,012 B1   | 4/2001  | Maschke et al.                      |
| 5,822,546 A  | 10/1998 | George                   | 6,224,553 B1   | 5/2001  | Nevo                                |
| 5,823,950 A  | 10/1998 | Diab et al.              | 6,229,856 B1   | 5/2001  | Diab et al.                         |
| 5,829,723 A  | 11/1998 | Brunner                  | 6,230,142 B1   | 5/2001  | Benigno et al.                      |
| 5,830,131 A  | 11/1998 | Caro et al.              | 6,232,609 B1   | 5/2001  | Snyder et al.                       |
| 5,830,137 A  | 11/1998 | Scharf                   | 6,236,872 B1   | 5/2001  | Diab et al.                         |
| 5,833,618 A  | 11/1998 | Caro et al.              | 6,241,683 B1   | 6/2001  | Macklem et al.                      |
| RE36,000 E   | 12/1998 | Swedlow et al.           | 6,241,684 B1 * | 6/2001  | Amano ..... A61B 5/02438<br>600/503 |
| 5,855,550 A  | 1/1999  | Lai et al.               | 6,251,113 B1   | 6/2001  | Appelbaum                           |
| 5,860,919 A  | 1/1999  | Kiani-Azarbayjany et al. | 6,253,097 B1   | 6/2001  | Aronow et al.                       |
| 5,865,736 A  | 2/1999  | Baker et al.             | 6,256,523 B1   | 7/2001  | Diab et al.                         |
| 5,876,351 A  | 3/1999  | Rohde                    | 6,263,222 B1   | 7/2001  | Diab et al.                         |
| 5,879,292 A  | 3/1999  | Sternberg et al.         | 6,267,723 B1   | 7/2001  | Matsumura et al.                    |
| 5,890,929 A  | 4/1999  | Mills et al.             | 6,269,262 B1   | 7/2001  | Kandori et al.                      |
| 5,904,654 A  | 5/1999  | Wohltmann et al.         | 6,278,522 B1   | 8/2001  | Lepper, Jr. et al.                  |
| 5,910,139 A  | 6/1999  | Cochran et al.           | 6,280,213 B1   | 8/2001  | Tobler et al.                       |
| 5,919,134 A  | 7/1999  | Diab                     | 6,285,896 B1   | 9/2001  | Tobler et al.                       |
| 5,921,920 A  | 7/1999  | Marshall et al.          | 6,289,238 B1   | 9/2001  | Besson et al.                       |
| 5,924,074 A  | 7/1999  | Evans                    | 6,301,493 B1   | 10/2001 | Marro et al.                        |
| 5,931,160 A  | 8/1999  | Gilmore et al.           | 6,304,767 B1   | 10/2001 | Soller et al.                       |
| 5,931,791 A  | 8/1999  | Saltzstein et al.        | 6,312,378 B1   | 11/2001 | Bardy                               |
| 5,934,925 A  | 8/1999  | Tobler et al.            | 6,317,627 B1   | 11/2001 | Ennen et al.                        |
| 5,940,182 A  | 8/1999  | Lepper, Jr. et al.       | 6,321,100 B1   | 11/2001 | Parker                              |
| 5,942,986 A  | 8/1999  | Shabot et al.            | 6,322,502 B1   | 11/2001 | Schoenberg et al.                   |
| 5,957,854 A  | 9/1999  | Besson et al.            | 6,325,761 B1   | 12/2001 | Jay                                 |
| 5,987,519 A  | 11/1999 | Peifer et al.            | 6,329,139 B1   | 12/2001 | Nova et al.                         |
| 5,995,855 A  | 11/1999 | Kiani et al.             | 6,334,065 B1   | 12/2001 | Al-Ali et al.                       |
| 5,997,343 A  | 12/1999 | Mills et al.             | 6,338,039 B1   | 1/2002  | Lonski et al.                       |
| 6,002,952 A  | 12/1999 | Diab et al.              | 6,343,224 B1   | 1/2002  | Parker                              |
| 6,006,119 A  | 12/1999 | Soller et al.            | 6,349,228 B1   | 2/2002  | Kiani et al.                        |
| 6,011,985 A  | 1/2000  | Athan et al.             | 6,352,504 B1   | 3/2002  | Ise                                 |
| 6,011,986 A  | 1/2000  | Diab et al.              | 6,354,235 B1   | 3/2002  | Davies                              |
| 6,014,346 A  | 1/2000  | Malone                   | 6,360,114 B1   | 3/2002  | Diab et al.                         |
| 6,018,673 A  | 1/2000  | Chin et al.              | 6,364,834 B1   | 4/2002  | Reuss et al.                        |
| 6,024,699 A  | 2/2000  | Surwit et al.            | 6,364,839 B1   | 4/2002  | Little et al.                       |
| 6,027,452 A  | 2/2000  | Flaherty et al.          | 6,368,283 B1   | 4/2002  | Xu et al.                           |
| 6,032,678 A  | 3/2000  | Rottem                   | 6,371,921 B1   | 4/2002  | Caro et al.                         |
| 6,035,230 A  | 3/2000  | Kang et al.              | 6,374,129 B1   | 4/2002  | Chin et al.                         |
| 6,036,642 A  | 3/2000  | Diab et al.              | 6,377,829 B1   | 4/2002  | Al-Ali                              |
| 6,036,718 A  | 3/2000  | Ledford et al.           | 6,385,476 B1   | 5/2002  | Osadchy et al.                      |
| 6,045,509 A  | 4/2000  | Caro et al.              | 6,385,589 B1   | 5/2002  | Trusheim et al.                     |
| 6,045,527 A  | 4/2000  | Appelbaum et al.         | 6,387,039 B1   | 5/2002  | Moses                               |
| 6,057,758 A  | 5/2000  | Dempsey et al.           | 6,388,240 B2   | 5/2002  | Schulz et al.                       |
| 6,067,462 A  | 5/2000  | Diab et al.              | 6,397,091 B2   | 5/2002  | Diab et al.                         |
| 6,081,735 A  | 6/2000  | Diab et al.              | 6,405,083 B1   | 6/2002  | Rockwell et al.                     |
| 6,088,607 A  | 7/2000  | Diab et al.              | 6,407,335 B1   | 6/2002  | Franklin-Lees                       |
| 6,090,056 A  | 7/2000  | Bystrom et al.           | 6,430,437 B1   | 8/2002  | Marro                               |
| 6,093,146 A  | 7/2000  | Filangeri                | 6,430,525 B1   | 8/2002  | Weber et al.                        |
| 6,101,478 A  | 8/2000  | Brown                    | 6,440,067 B1   | 8/2002  | Deluca et al.                       |
| 6,106,463 A  | 8/2000  | Wilk                     | 6,454,708 B1   | 9/2002  | Ferguson et al.                     |
| 6,110,522 A  | 8/2000  | Lepper, Jr. et al.       | 6,463,311 B1   | 10/2002 | Diab                                |
| 6,124,597 A  | 9/2000  | Shehada                  | 6,470,199 B1   | 10/2002 | Kopotic et al.                      |
| 6,128,521 A  | 10/2000 | Marro et al.             | 6,470,893 B1   | 10/2002 | Boesen                              |
| 6,129,675 A  | 10/2000 | Jay                      | 6,491,647 B1   | 12/2002 | Bridger et al.                      |
| 6,132,218 A  | 10/2000 | Benja-Athon              | 6,501,975 B2   | 12/2002 | Diab et al.                         |
| 6,139,494 A  | 10/2000 | Cairnes                  | 6,505,059 B1   | 1/2003  | Kollias et al.                      |
| 6,144,868 A  | 11/2000 | Parker                   | 6,515,273 B2   | 2/2003  | Al-Ali                              |
| 6,151,516 A  | 11/2000 | Kiani-Azarbayjany et al. | 6,516,289 B2 * | 2/2003  | David ..... A61B 5/04085<br>600/503 |
| 6,152,754 A  | 11/2000 | Gerhardt et al.          | 6,519,487 B1   | 2/2003  | Parker                              |
| 6,154,667 A  | 11/2000 | Miura et al.             | 6,524,240 B1   | 2/2003  | Thede                               |
| 6,157,850 A  | 12/2000 | Diab et al.              | 6,525,386 B1   | 2/2003  | Mills et al.                        |
| 6,165,005 A  | 12/2000 | Mills et al.             | 6,526,300 B1   | 2/2003  | Kiani et al.                        |
| 6,167,258 A  | 12/2000 | Schmidt et al.           | 6,541,756 B2   | 4/2003  | Schulz et al.                       |
| D437,058 S   | 1/2001  | Gozani                   | 6,542,764 B1   | 4/2003  | Al-Ali et al.                       |
| 6,168,563 B1 | 1/2001  | Brown                    | 6,544,173 B2   | 4/2003  | West et al.                         |
| 6,171,237 B1 | 1/2001  | Avitall et al.           | 6,544,174 B2   | 4/2003  | West et al.                         |
| 6,175,752 B1 | 1/2001  | Say et al.               | 6,551,243 B2   | 4/2003  | Bocionek et al.                     |
| 6,178,343 B1 | 1/2001  | Bindzus et al.           | 6,553,242 B1   | 4/2003  | Sarussi                             |
| 6,183,417 B1 | 2/2001  | Gehab et al.             | 6,577,893 B1   | 6/2003  | Besson et al.                       |
| 6,184,521 B1 | 2/2001  | Coffin, IV et al.        | 6,578,428 B1   | 6/2003  | Dromms et al.                       |
| 6,185,448 B1 | 2/2001  | Borovsky                 | 6,580,086 B1   | 6/2003  | Schulz et al.                       |
| 6,190,327 B1 | 2/2001  | Isaacson et al.          | 6,584,336 B1   | 6/2003  | Ali et al.                          |
| 6,195,576 B1 | 2/2001  | John                     | 6,595,316 B2   | 7/2003  | Cybulski et al.                     |
|              |         |                          | 6,597,932 B2   | 7/2003  | Tian et al.                         |
|              |         |                          | 6,597,933 B2   | 7/2003  | Kiani et al.                        |

(56)

## References Cited

## U.S. PATENT DOCUMENTS

|              |         |                          |              |         |                          |
|--------------|---------|--------------------------|--------------|---------|--------------------------|
| 6,606,511 B1 | 8/2003  | Ali et al.               | 6,939,305 B2 | 9/2005  | Flaherty et al.          |
| 6,612,984 B1 | 9/2003  | Kerr, II                 | 6,942,616 B2 | 9/2005  | Kerr, II                 |
| 6,616,606 B1 | 9/2003  | Petersen et al.          | 6,943,348 B1 | 9/2005  | Coffin, IV               |
| 6,632,181 B2 | 10/2003 | Flaherty et al.          | 6,950,687 B2 | 9/2005  | Al-Ali                   |
| 6,639,668 B1 | 10/2003 | Trepagnier               | 6,952,340 B2 | 10/2005 | Son                      |
| 6,640,116 B2 | 10/2003 | Diab                     | 6,961,598 B2 | 11/2005 | Diab                     |
| 6,641,533 B2 | 11/2003 | Causey et al.            | 6,970,792 B1 | 11/2005 | Diab                     |
| 6,643,530 B2 | 11/2003 | Diab et al.              | 6,979,812 B2 | 12/2005 | Al-Ali                   |
| 6,646,556 B1 | 11/2003 | Smith et al.             | 6,980,419 B2 | 12/2005 | Smith et al.             |
| 6,650,917 B2 | 11/2003 | Diab et al.              | 6,983,179 B2 | 1/2006  | Ben-haim                 |
| 6,650,939 B2 | 11/2003 | Takpke, II et al.        | 6,985,764 B2 | 1/2006  | Mason et al.             |
| 6,654,624 B2 | 11/2003 | Diab et al.              | 6,988,989 B2 | 1/2006  | Weiner et al.            |
| D483,872 S   | 12/2003 | Cruz et al.              | 6,990,087 B2 | 1/2006  | Rao et al.               |
| 6,658,276 B2 | 12/2003 | Kianl et al.             | 6,993,371 B2 | 1/2006  | Kiani et al.             |
| 6,661,161 B1 | 12/2003 | Lanzo et al.             | 6,996,427 B2 | 2/2006  | Ali et al.               |
| 6,663,570 B2 | 12/2003 | Mott et al.              | 6,997,884 B2 | 2/2006  | Ulmsten                  |
| 6,671,531 B2 | 12/2003 | Al-Ali et al.            | 6,999,904 B2 | 2/2006  | Weber et al.             |
| 6,678,543 B2 | 1/2004  | Diab et al.              | 7,003,338 B2 | 2/2006  | Weber et al.             |
| 6,684,090 B2 | 1/2004  | Ali et al.               | 7,003,339 B2 | 2/2006  | Diab et al.              |
| 6,684,091 B2 | 1/2004  | Parker                   | 7,015,451 B2 | 3/2006  | Dalke et al.             |
| 6,694,160 B2 | 2/2004  | Chin                     | 7,024,233 B2 | 4/2006  | Ali et al.               |
| 6,694,180 B1 | 2/2004  | Boesen                   | 7,025,729 B2 | 4/2006  | De Chazal et al.         |
| 6,697,656 B1 | 2/2004  | Al-Ali                   | 7,027,849 B2 | 4/2006  | Al-Ali                   |
| 6,697,657 B1 | 2/2004  | Shehada et al.           | 7,030,749 B2 | 4/2006  | Al-Ali                   |
| 6,697,658 B2 | 2/2004  | Al-Ali                   | 7,033,761 B2 | 4/2006  | Shafer                   |
| RE38,476 E   | 3/2004  | Diab et al.              | 7,035,686 B2 | 4/2006  | Hogan                    |
| 6,699,194 B1 | 3/2004  | Diab et al.              | 7,039,449 B2 | 5/2006  | Al-Ali                   |
| 6,714,804 B2 | 3/2004  | Al-Ali et al.            | 7,041,060 B2 | 5/2006  | Flaherty et al.          |
| RE38,492 E   | 4/2004  | Diab et al.              | 7,044,918 B2 | 5/2006  | Diab                     |
| 6,719,694 B2 | 4/2004  | Weng et al.              | 7,044,930 B2 | 5/2006  | Stromberg                |
| 6,720,734 B2 | 4/2004  | Norris                   | 7,063,666 B2 | 6/2006  | Weng et al.              |
| 6,721,582 B2 | 4/2004  | Trepagnier et al.        | 7,067,893 B2 | 6/2006  | Mills et al.             |
| 6,721,585 B1 | 4/2004  | Parker                   | 7,079,035 B2 | 7/2006  | Bock et al.              |
| 6,725,075 B2 | 4/2004  | Al-Ali                   | 7,096,052 B2 | 8/2006  | Mason et al.             |
| 6,725,086 B2 | 4/2004  | Marinello                | 7,096,054 B2 | 8/2006  | Abdul-Hafiz et al.       |
| 6,728,560 B2 | 4/2004  | Kollias et al.           | 7,125,382 B2 | 10/2006 | Zhou et al.              |
| 6,731,962 B1 | 5/2004  | Katarow et al.           | 7,132,641 B2 | 11/2006 | Schulz et al.            |
| 6,735,459 B2 | 5/2004  | Parker                   | 7,142,901 B2 | 11/2006 | Kiani et al.             |
| 6,745,060 B2 | 6/2004  | Diab et al.              | 7,149,561 B2 | 12/2006 | Diab                     |
| 6,746,406 B2 | 6/2004  | Lia et al.               | 7,186,966 B2 | 3/2007  | Al-Ali                   |
| 6,750,463 B1 | 6/2004  | Riley                    | 7,188,621 B2 | 3/2007  | DeVries et al.           |
| 6,751,492 B2 | 6/2004  | Ben-haim                 | 7,190,261 B2 | 3/2007  | Al-Ali                   |
| 6,760,607 B2 | 7/2004  | Al-Ali                   | 7,208,119 B1 | 4/2007  | Kurtock et al.           |
| 6,766,188 B2 | 7/2004  | Soller                   | 7,215,984 B2 | 5/2007  | Diab                     |
| 6,770,028 B1 | 8/2004  | Ali et al.               | 7,215,986 B2 | 5/2007  | Diab                     |
| 6,771,994 B2 | 8/2004  | Kiani et al.             | 7,221,971 B2 | 5/2007  | Diab                     |
| 6,783,492 B2 | 8/2004  | Dominguez                | 7,225,006 B2 | 5/2007  | Al-Ali et al.            |
| 6,790,178 B1 | 9/2004  | Mault et al.             | 7,225,007 B2 | 5/2007  | Al-Ali                   |
| 6,792,300 B1 | 9/2004  | Diab et al.              | RE39,672 E   | 6/2007  | Shehada et al.           |
| 6,795,724 B2 | 9/2004  | Hogan                    | 7,229,415 B2 | 6/2007  | Schwartz                 |
| 6,796,186 B2 | 9/2004  | Lia et al.               | 7,239,905 B2 | 7/2007  | Kiani-Azarbayjany et al. |
| 6,804,656 B1 | 10/2004 | Rosenfeld                | 7,241,287 B2 | 7/2007  | Shehada et al.           |
| 6,807,050 B1 | 10/2004 | Whitehorn et al.         | 7,244,251 B2 | 7/2007  | Shehada et al.           |
| 6,813,511 B2 | 11/2004 | Diab et al.              | 7,245,373 B2 | 7/2007  | Soller et al.            |
| 6,816,741 B2 | 11/2004 | Diab                     | 7,245,953 B1 | 7/2007  | Parker                   |
| 6,817,979 B2 | 11/2004 | Nihtila et al.           | 7,252,659 B2 | 8/2007  | Shehada et al.           |
| 6,822,564 B2 | 11/2004 | Al-Ali                   | 7,254,429 B2 | 8/2007  | Schurman et al.          |
| 6,826,419 B2 | 11/2004 | Diab et al.              | 7,254,431 B2 | 8/2007  | Al-Ali                   |
| 6,830,711 B2 | 12/2004 | Mills et al.             | 7,254,433 B2 | 8/2007  | Diab et al.              |
| 6,837,848 B2 | 1/2005  | Bonner et al.            | 7,254,434 B2 | 8/2007  | Schulz et al.            |
| 6,841,535 B2 | 1/2005  | Divita et al.            | 7,256,708 B2 | 8/2007  | Rosenfeld                |
| 6,845,256 B2 | 1/2005  | Chin et al.              | 7,257,438 B2 | 8/2007  | Kinast                   |
| 6,850,787 B2 | 2/2005  | Weber et al.             | 7,261,697 B2 | 8/2007  | Berstein                 |
| 6,850,788 B2 | 2/2005  | Al-Ali                   | 7,264,616 B2 | 9/2007  | Shehada et al.           |
| 6,852,083 B2 | 2/2005  | Caro et al.              | 7,267,671 B2 | 9/2007  | Shehada et al.           |
| 6,855,112 B2 | 2/2005  | Kao et al.               | 7,272,425 B2 | 9/2007  | Al-Ali                   |
| 6,860,266 B2 | 3/2005  | Blike                    | 7,274,955 B2 | 9/2007  | Kiani et al.             |
| 6,861,639 B2 | 3/2005  | Al-Ali                   | D554,263 S   | 10/2007 | Al-Ali                   |
| 6,897,788 B2 | 5/2005  | Khair et al.             | 7,280,858 B2 | 10/2007 | Al-Ali et al.            |
| 6,898,452 B2 | 5/2005  | Al-Ali et al.            | 7,285,090 B2 | 10/2007 | Stivorice                |
| 6,907,237 B1 | 6/2005  | Dorenbosch et al.        | 7,289,835 B2 | 10/2007 | Mansfield et al.         |
| 6,915,149 B2 | 7/2005  | Ben-haim                 | 7,292,883 B2 | 11/2007 | De Felice et al.         |
| 6,920,345 B2 | 7/2005  | Al-Ali et al.            | 7,295,866 B2 | 11/2007 | Al-Ali                   |
| 6,931,268 B1 | 8/2005  | Kiani-Azarbayjany et al. | 7,307,543 B2 | 12/2007 | Rosenfeld                |
| 6,934,570 B2 | 8/2005  | Kiani et al.             | 7,313,423 B2 | 12/2007 | Griffin et al.           |
|              |         |                          | 7,314,446 B2 | 1/2008  | Byrd et al.              |
|              |         |                          | 7,315,825 B2 | 1/2008  | Rosenfeld                |
|              |         |                          | 7,321,862 B2 | 1/2008  | Rosenfeld                |
|              |         |                          | 7,322,971 B2 | 1/2008  | Shehada et al.           |

(56)

## References Cited

## U.S. PATENT DOCUMENTS

|           |    |         |                  |           |    |         |                     |
|-----------|----|---------|------------------|-----------|----|---------|---------------------|
| 7,328,053 | B1 | 2/2008  | Diab et al.      | D606,659  | S  | 12/2009 | Kiani et al.        |
| 7,332,784 | B2 | 2/2008  | Mills et al.     | 7,639,145 | B2 | 12/2009 | Lawson et al.       |
| 7,340,287 | B2 | 3/2008  | Mason et al.     | 7,647,083 | B2 | 1/2010  | Al-Ali et al.       |
| 7,341,559 | B2 | 3/2008  | Schulz et al.    | 7,650,291 | B2 | 1/2010  | Rosenfeld           |
| 7,343,186 | B2 | 3/2008  | Lamego et al.    | D609,193  | S  | 2/2010  | Al-Ali et al.       |
| D566,282  | S  | 4/2008  | Al-Ali et al.    | 7,654,966 | B2 | 2/2010  | Westinskow et al.   |
| 7,355,512 | B1 | 4/2008  | Al-Ali           | 7,684,845 | B2 | 3/2010  | Juan                |
| 7,356,178 | B2 | 4/2008  | Ziel et al.      | 7,689,437 | B1 | 3/2010  | Teller et al.       |
| 7,356,365 | B2 | 4/2008  | Schurman         | RE41,236  | E  | 4/2010  | Seely               |
| 7,359,742 | B2 | 4/2008  | Maser et al.     | D614,305  | S  | 4/2010  | Al-Ali et al.       |
| 7,371,981 | B2 | 5/2008  | Abdul-Hafiz      | 7,693,697 | B2 | 4/2010  | Westinskow et al.   |
| 7,373,193 | B2 | 5/2008  | Al-Ali et al.    | RE41,317  | E  | 5/2010  | Parker              |
| 7,373,194 | B2 | 5/2008  | Weber et al.     | D615,655  | S  | 5/2010  | Maser et al.        |
| 7,376,453 | B1 | 5/2008  | Diab et al.      | 7,722,542 | B2 | 5/2010  | Lia et al.          |
| 7,377,794 | B2 | 5/2008  | Al-Ali et al.    | 7,729,733 | B2 | 6/2010  | Al-Ali et al.       |
| 7,377,899 | B2 | 5/2008  | Weber et al.     | 7,734,320 | B2 | 6/2010  | Al-Ali              |
| 7,378,975 | B1 | 5/2008  | Smith et al.     | 7,736,318 | B2 | 6/2010  | Consentino et al.   |
| 7,382,247 | B2 | 6/2008  | Welch et al.     | 7,740,590 | B2 | 6/2010  | Bernstein           |
| 7,383,070 | B2 | 6/2008  | Diab et al.      | 7,761,127 | B2 | 7/2010  | Al-Ali et al.       |
| 7,390,299 | B2 | 6/2008  | Weiner et al.    | 7,761,128 | B2 | 7/2010  | Al-Ali et al.       |
| 7,392,074 | B2 | 6/2008  | Isaacson et al.  | 7,763,420 | B2 | 7/2010  | Strizker et al.     |
| 7,395,216 | B2 | 7/2008  | Rosenfeld        | 7,764,982 | B2 | 7/2010  | Dalke et al.        |
| 7,411,509 | B2 | 8/2008  | Rosenfeld        | D621,515  | S  | 8/2010  | Chua et al.         |
| 7,413,546 | B2 | 8/2008  | Agutter et al.   | D621,516  | S  | 8/2010  | Kiani et al.        |
| 7,415,297 | B2 | 8/2008  | Al-Ali et al.    | 7,766,818 | B2 | 8/2010  | Iketani et al.      |
| 7,419,483 | B2 | 9/2008  | Shehada          | 7,774,060 | B2 | 8/2010  | Westenskow et al.   |
| 7,428,432 | B2 | 9/2008  | Ali et al.       | 7,778,851 | B2 | 8/2010  | Schoenberg et al.   |
| 7,433,827 | B2 | 10/2008 | Rosenfeld        | 7,791,155 | B2 | 9/2010  | Diab                |
| 7,438,683 | B2 | 10/2008 | Al-Ali et al.    | 7,794,407 | B2 | 9/2010  | Rothenberg          |
| 7,439,856 | B2 | 10/2008 | Weiner et al.    | 7,801,581 | B2 | 9/2010  | Diab                |
| 7,440,787 | B2 | 10/2008 | Diab             | 7,801,605 | B2 | 9/2010  | Smirles et al.      |
| 7,454,240 | B2 | 11/2008 | Diab et al.      | 7,806,830 | B2 | 10/2010 | Bernstein           |
| 7,454,359 | B2 | 11/2008 | Rosenfeld        | 7,820,184 | B2 | 10/2010 | Strizker et al.     |
| 7,454,360 | B2 | 11/2008 | Rosenfeld        | 7,822,452 | B2 | 10/2010 | Schurman et al.     |
| 7,462,151 | B2 | 12/2008 | Childre et al.   | RE41,912  | E  | 11/2010 | Parker              |
| 7,467,002 | B2 | 12/2008 | Weber et al.     | 7,831,450 | B2 | 11/2010 | Schoenberg          |
| 7,467,094 | B2 | 12/2008 | Rosenfeld        | 7,841,986 | B2 | 11/2010 | He et al.           |
| 7,469,157 | B2 | 12/2008 | Diab et al.      | 7,844,313 | B2 | 11/2010 | Kiani et al.        |
| 7,471,969 | B2 | 12/2008 | Diab et al.      | 7,844,314 | B2 | 11/2010 | Al-Ali              |
| 7,471,971 | B2 | 12/2008 | Diab et al.      | 7,844,315 | B2 | 11/2010 | Al-Ali              |
| 7,475,019 | B2 | 1/2009  | Rosenfeld        | 7,848,935 | B2 | 12/2010 | Gotlib              |
| 7,483,729 | B2 | 1/2009  | Al-Ali et al.    | 7,858,322 | B2 | 12/2010 | Tymianski et al.    |
| 7,483,730 | B2 | 1/2009  | Diab et al.      | 7,865,222 | B2 | 1/2011  | Weber et al.        |
| 7,486,977 | B2 | 2/2009  | Sweitzer et al.  | 7,865,232 | B1 | 1/2011  | Krishnaswamy et al. |
| 7,489,250 | B2 | 2/2009  | Bock et al.      | 7,873,497 | B2 | 1/2011  | Weber et al.        |
| 7,489,958 | B2 | 2/2009  | Diab et al.      | 7,880,606 | B2 | 2/2011  | Al-Ali              |
| 7,496,391 | B2 | 2/2009  | Diab et al.      | 7,880,626 | B2 | 2/2011  | Al-Ali et al.       |
| 7,496,393 | B2 | 2/2009  | Diab et al.      | 7,881,892 | B2 | 2/2011  | Soyemi et al.       |
| D587,657  | S  | 3/2009  | Al-Ali et al.    | 7,884,314 | B2 | 2/2011  | Hamada              |
| 7,497,828 | B1 | 3/2009  | Wilk et al.      | 7,890,156 | B2 | 2/2011  | Ooi et al.          |
| 7,499,739 | B2 | 3/2009  | Sweitzer et al.  | 7,891,355 | B2 | 2/2011  | Al-Ali et al.       |
| 7,499,741 | B2 | 3/2009  | Diab et al.      | 7,894,868 | B2 | 2/2011  | Al-Ali et al.       |
| 7,499,835 | B2 | 3/2009  | Weber et al.     | 7,899,507 | B2 | 3/2011  | Al-Ali et al.       |
| 7,500,950 | B2 | 3/2009  | Al-Ali et al.    | 7,899,518 | B2 | 3/2011  | Trepagnier et al.   |
| 7,509,154 | B2 | 3/2009  | Diab et al.      | 7,904,132 | B2 | 3/2011  | Weber et al.        |
| 7,509,494 | B2 | 3/2009  | Al-Ali           | 7,909,772 | B2 | 3/2011  | Popov et al.        |
| 7,510,849 | B2 | 3/2009  | Schurman et al.  | 7,910,875 | B2 | 3/2011  | Al-Ali              |
| 7,515,043 | B2 | 4/2009  | Welch et al.     | 7,914,514 | B2 | 3/2011  | Calderon            |
| 7,515,044 | B2 | 4/2009  | Welch et al.     | 7,919,713 | B2 | 4/2011  | Al-Ali et al.       |
| 7,526,328 | B2 | 4/2009  | Diab et al.      | 7,937,128 | B2 | 5/2011  | Al-Ali              |
| 7,530,942 | B1 | 5/2009  | Diab             | 7,937,129 | B2 | 5/2011  | Mason et al.        |
| 7,530,949 | B2 | 5/2009  | Al Ali et al.    | 7,937,130 | B2 | 5/2011  | Diab et al.         |
| 7,530,955 | B2 | 5/2009  | Diab et al.      | 7,941,199 | B2 | 5/2011  | Kiani               |
| 7,532,919 | B2 | 5/2009  | Soyemi et al.    | 7,951,086 | B2 | 5/2011  | Flaherty et al.     |
| 7,549,961 | B1 | 6/2009  | Hwang            | 7,957,780 | B2 | 6/2011  | Lamego et al.       |
| 7,551,717 | B2 | 6/2009  | Tome et al.      | 7,962,188 | B2 | 6/2011  | Kiani et al.        |
| 7,559,520 | B2 | 7/2009  | Quijano et al.   | 7,962,190 | B1 | 6/2011  | Diab et al.         |
| 7,563,110 | B2 | 7/2009  | Al-Ali et al.    | 7,963,927 | B2 | 6/2011  | Kelleher et al.     |
| 7,577,475 | B2 | 8/2009  | Cosentino et al. | 7,967,749 | B2 | 6/2011  | Hutchinson et al.   |
| 7,590,950 | B2 | 9/2009  | Collins et al.   | 7,970,450 | B2 | 6/2011  | Kroecker            |
| 7,596,398 | B2 | 9/2009  | Al-Ali et al.    | 7,976,472 | B2 | 7/2011  | Kiani               |
| 7,597,665 | B2 | 10/2009 | Wilk et al.      | 7,988,637 | B2 | 8/2011  | Diab                |
| 7,612,999 | B2 | 11/2009 | Clark et al.     | 7,988,639 | B2 | 8/2011  | Starks              |
| 7,616,303 | B2 | 11/2009 | Yang et al.      | 7,990,382 | B2 | 8/2011  | Kiani               |
| 7,618,375 | B2 | 11/2009 | Flaherty         | 7,991,446 | B2 | 8/2011  | Al-Ali et al.       |
|           |    |         |                  | 7,991,463 | B2 | 8/2011  | Kelleher et al.     |
|           |    |         |                  | 7,991,625 | B2 | 8/2011  | Rosenfeld           |
|           |    |         |                  | 8,000,761 | B2 | 8/2011  | Al-Ali              |
|           |    |         |                  | 8,008,088 | B2 | 8/2011  | Bellott et al.      |

(56)

## References Cited

## U.S. PATENT DOCUMENTS

|              |         |                          |              |         |                      |
|--------------|---------|--------------------------|--------------|---------|----------------------|
| RE42,753 E   | 9/2011  | Kiani-Azarbayjany et al. | 8,355,766 B2 | 1/2013  | MacNeish, III et al. |
| 8,019,400 B2 | 9/2011  | Diab et al.              | 8,359,080 B2 | 1/2013  | Diab et al.          |
| 8,027,846 B2 | 9/2011  | Schoenberg               | 8,360,936 B2 | 1/2013  | Dibenedetto et al.   |
| 8,028,701 B2 | 10/2011 | Al-Ali et al.            | 8,364,223 B2 | 1/2013  | Al-Ali et al.        |
| 8,029,765 B2 | 10/2011 | Bellott et al.           | 8,364,226 B2 | 1/2013  | Diab et al.          |
| 8,033,996 B2 | 10/2011 | Behar                    | 8,374,665 B2 | 2/2013  | Lamego               |
| 8,036,727 B2 | 10/2011 | Schurman et al.          | 8,385,972 B2 | 2/2013  | Bochenko et al.      |
| 8,036,728 B2 | 10/2011 | Diab et al.              | 8,385,995 B2 | 2/2013  | Al-ali et al.        |
| 8,036,736 B2 | 10/2011 | Snyder et al.            | 8,385,996 B2 | 2/2013  | Smith et al.         |
| 8,038,625 B2 | 10/2011 | Afonso et al.            | D679,018 S   | 3/2013  | Fullerton et al.     |
| 8,046,040 B2 | 10/2011 | Ali et al.               | 8,388,353 B2 | 3/2013  | Kiani et al.         |
| 8,046,041 B2 | 10/2011 | Diab et al.              | 8,399,822 B2 | 3/2013  | Al-Ali               |
| 8,046,042 B2 | 10/2011 | Diab et al.              | 8,401,602 B2 | 3/2013  | Kiani                |
| 8,048,040 B2 | 11/2011 | Kiani                    | 8,401,874 B2 | 3/2013  | Rosenfeld            |
| 8,050,728 B2 | 11/2011 | Al-Ali et al.            | 8,405,608 B2 | 3/2013  | Al-Ali et al.        |
| 8,068,104 B2 | 11/2011 | Rampersad                | 8,414,499 B2 | 4/2013  | Al-Ali et al.        |
| 8,073,707 B2 | 12/2011 | Teller et al.            | 8,418,524 B2 | 4/2013  | Al-Ali               |
| 8,094,013 B1 | 1/2012  | Lee et al.               | 8,423,106 B2 | 4/2013  | Lamego et al.        |
| RE43,169 E   | 2/2012  | Parker                   | 8,428,967 B2 | 4/2013  | Olsen et al.         |
| 8,118,620 B2 | 2/2012  | Al-Ali et al.            | 8,430,817 B1 | 4/2013  | Al-Ali et al.        |
| 8,126,528 B2 | 2/2012  | Diab et al.              | 8,437,825 B2 | 5/2013  | Dalvi et al.         |
| 8,128,572 B2 | 3/2012  | Diab et al.              | 8,455,290 B2 | 6/2013  | Siskavich            |
| 8,130,105 B2 | 3/2012  | Al-Ali et al.            | 8,457,703 B2 | 6/2013  | Al-Ali               |
| 8,145,287 B2 | 3/2012  | Diab et al.              | 8,457,704 B2 | 6/2013  | Sweitzer et al.      |
| 8,150,487 B2 | 4/2012  | Diab et al.              | 8,457,707 B2 | 6/2013  | Kiani                |
| D659,836 S   | 5/2012  | Bensch et al.            | 8,463,349 B2 | 6/2013  | Diab et al.          |
| 8,170,887 B2 | 5/2012  | Rosenfeld                | 8,466,286 B2 | 6/2013  | Bellot et al.        |
| 8,175,672 B2 | 5/2012  | Parker                   | 8,467,556 B2 | 6/2013  | Shennib et al.       |
| 8,175,895 B2 | 5/2012  | Rosenfeld                | 8,471,713 B2 | 6/2013  | Poeze et al.         |
| 8,180,420 B2 | 5/2012  | Diab et al.              | 8,473,020 B2 | 6/2013  | Kiani et al.         |
| 8,182,443 B1 | 5/2012  | Kiani                    | 8,483,787 B2 | 7/2013  | Al-Ali et al.        |
| 8,185,180 B2 | 5/2012  | Diab et al.              | 8,489,167 B2 | 7/2013  | Buxton et al.        |
| 8,190,223 B2 | 5/2012  | Al-Ali et al.            | 8,489,364 B2 | 7/2013  | Weber et al.         |
| 8,190,227 B2 | 5/2012  | Diab et al.              | 8,498,684 B2 | 7/2013  | Weber et al.         |
| 8,200,308 B2 | 6/2012  | Zhang et al.             | 8,500,692 B2 | 8/2013  | Yodfat et al.        |
| 8,203,438 B2 | 6/2012  | Kiani et al.             | 8,504,128 B2 | 8/2013  | Blank et al.         |
| 8,203,704 B2 | 6/2012  | Merritt et al.           | 8,509,867 B2 | 8/2013  | Workman et al.       |
| 8,204,566 B2 | 6/2012  | Schurman et al.          | 8,515,509 B2 | 8/2013  | Bruinsma et al.      |
| 8,206,312 B2 | 6/2012  | Farquhar                 | 8,523,781 B2 | 9/2013  | Al-Ali               |
| 8,214,007 B2 | 7/2012  | Baker et al.             | 8,529,301 B2 | 9/2013  | Al-Ali et al.        |
| 8,219,172 B2 | 7/2012  | Schurman et al.          | 8,532,727 B2 | 9/2013  | Ali et al.           |
| 8,224,411 B2 | 7/2012  | Al-Ali et al.            | 8,532,728 B2 | 9/2013  | Diab et al.          |
| 8,228,181 B2 | 7/2012  | Al-Ali                   | D692,145 S   | 10/2013 | Al-Ali et al.        |
| 8,229,533 B2 | 7/2012  | Diab et al.              | 8,545,445 B2 | 10/2013 | Kamen et al.         |
| 8,233,955 B2 | 7/2012  | Al-Ali et al.            | 8,547,209 B2 | 10/2013 | Kiani et al.         |
| 8,235,907 B2 | 8/2012  | Wilk et al.              | 8,548,548 B2 | 10/2013 | Al-Ali               |
| 8,239,780 B2 | 8/2012  | Manetta et al.           | 8,548,549 B2 | 10/2013 | Schurman et al.      |
| 8,241,213 B2 | 8/2012  | Lynn et al.              | 8,548,550 B2 | 10/2013 | Al-Ali et al.        |
| 8,244,325 B2 | 8/2012  | Al-Ali et al.            | 8,560,032 B2 | 10/2013 | Al-Ali et al.        |
| 8,249,815 B2 | 8/2012  | Taylor                   | 8,560,034 B1 | 10/2013 | Diab et al.          |
| 8,255,026 B1 | 8/2012  | Al-Ali                   | 8,564,613 B2 | 10/2013 | Prior et al.         |
| 8,255,027 B2 | 8/2012  | Al-Ali et al.            | 8,565,847 B2 | 10/2013 | Buxton et al.        |
| 8,255,028 B2 | 8/2012  | Al-Ali et al.            | 8,568,361 B2 | 10/2013 | Yodfat et al.        |
| 8,260,577 B2 | 9/2012  | Weber et al.             | 8,570,167 B2 | 10/2013 | Al-Ali               |
| 8,265,723 B1 | 9/2012  | McHale et al.            | 8,570,503 B2 | 10/2013 | Vo et al.            |
| 8,274,360 B2 | 9/2012  | Sampath et al.           | 8,571,617 B2 | 10/2013 | Reichgott et al.     |
| 8,294,588 B2 | 10/2012 | Fisher et al.            | 8,571,618 B1 | 10/2013 | Lamego et al.        |
| 8,294,716 B2 | 10/2012 | Lord et al.              | 8,571,619 B2 | 10/2013 | Al-Ali et al.        |
| 8,301,217 B2 | 10/2012 | Al-Ali et al.            | 8,577,431 B2 | 11/2013 | Lamego et al.        |
| 8,306,596 B2 | 11/2012 | Schurman et al.          | 8,578,082 B2 | 11/2013 | Medina et al.        |
| 8,310,336 B2 | 11/2012 | Muhsin et al.            | 8,579,813 B2 | 11/2013 | Causey, III et al.   |
| 8,311,747 B2 | 11/2012 | Taylor                   | 8,581,732 B2 | 11/2013 | Al-Ali et al.        |
| 8,311,748 B2 | 11/2012 | Taylor et al.            | 8,584,345 B2 | 11/2013 | Al-Ali et al.        |
| 8,315,683 B2 | 11/2012 | Al-Ali et al.            | 8,588,880 B2 | 11/2013 | Abdul-Hafiz et al.   |
| 8,315,812 B2 | 11/2012 | Taylor                   | 8,588,924 B2 | 11/2013 | Dion                 |
| 8,315,813 B2 | 11/2012 | Taylor et al.            | 8,597,287 B2 | 12/2013 | Benamou et al.       |
| 8,315,814 B2 | 11/2012 | Taylor et al.            | 8,600,467 B2 | 12/2013 | Al-Ali et al.        |
| 8,321,150 B2 | 11/2012 | Taylor                   | 8,600,777 B2 | 12/2013 | Schoenberg           |
| RE43,860 E   | 12/2012 | Parker                   | 8,606,342 B2 | 12/2013 | Diab                 |
| 8,326,392 B2 | 12/2012 | Grubac et al.            | 8,615,281 B2 | 12/2013 | Yodfat et al.        |
| 8,326,649 B2 | 12/2012 | Rosenfeld                | 8,620,678 B2 | 12/2013 | Gotlib               |
| 8,328,793 B2 | 12/2012 | Birkenbach et al.        | 8,626,255 B2 | 1/2014  | Al-Ali et al.        |
| 8,337,403 B2 | 12/2012 | Al-Ali et al.            | 8,630,691 B2 | 1/2014  | Lamego et al.        |
| 8,346,330 B2 | 1/2013  | Lamego                   | 8,634,889 B2 | 1/2014  | Al-Ali et al.        |
| 8,353,842 B2 | 1/2013  | Al-Ali et al.            | 8,641,631 B2 | 2/2014  | Sierra et al.        |
|              |         |                          | 8,641,670 B2 | 2/2014  | Yodfat et al.        |
|              |         |                          | 8,652,060 B2 | 2/2014  | Al-Ali               |
|              |         |                          | 8,663,107 B2 | 3/2014  | Kiani                |
|              |         |                          | 8,666,468 B1 | 3/2014  | Al-Ali               |

(56)

## References Cited

## U.S. PATENT DOCUMENTS

|           |    |         |                      |           |    |         |                    |
|-----------|----|---------|----------------------|-----------|----|---------|--------------------|
| 8,667,967 | B2 | 3/2014  | Al-Ali et al.        | 8,929,964 | B2 | 1/2015  | Al-Ali et al.      |
| 8,670,810 | B2 | 3/2014  | Isaacson             | 8,939,914 | B2 | 1/2015  | Turnquist et al.   |
| 8,670,811 | B2 | 3/2014  | O'Reilly             | 8,942,777 | B2 | 1/2015  | Diab et al.        |
| 8,670,814 | B2 | 3/2014  | Diab et al.          | 8,948,834 | B2 | 2/2015  | Diab et al.        |
| 8,676,286 | B2 | 3/2014  | Weber et al.         | 8,948,835 | B2 | 2/2015  | Diab               |
| 8,682,407 | B2 | 3/2014  | Al-Ali               | 8,951,248 | B2 | 2/2015  | Messerly et al.    |
| RE44,823  | E  | 4/2014  | Parker               | 8,956,292 | B2 | 2/2015  | Wekell et al.      |
| RE44,875  | E  | 4/2014  | Kiani et al.         | 8,962,170 | B2 | 2/2015  | Frey et al.        |
| 8,690,771 | B2 | 4/2014  | Wekell et al.        | 8,965,471 | B2 | 2/2015  | Lamego             |
| 8,690,799 | B2 | 4/2014  | Telfort et al.       | 8,977,351 | B2 | 3/2015  | Kivisto            |
| 8,695,206 | B2 | 4/2014  | Isaacson et al.      | 8,983,564 | B2 | 3/2015  | Al-Ali             |
| 8,700,112 | B2 | 4/2014  | Kiani                | 8,989,831 | B2 | 3/2015  | Al-Ali et al.      |
| 8,702,627 | B2 | 4/2014  | Telfort et al.       | 8,996,085 | B2 | 3/2015  | Kiani et al.       |
| 8,706,179 | B2 | 4/2014  | Parker               | 8,998,809 | B2 | 4/2015  | Kiani              |
| 8,712,494 | B1 | 4/2014  | MacNeish, III et al. | 9,014,778 | B2 | 4/2015  | Datta et al.       |
| 8,715,206 | B2 | 5/2014  | Telfort et al.       | 9,017,355 | B2 | 4/2015  | Smith et al.       |
| 8,718,735 | B2 | 5/2014  | Lamego et al.        | 9,028,407 | B1 | 5/2015  | Bennett-Guerrero   |
| 8,718,737 | B2 | 5/2014  | Diab et al.          | 9,028,429 | B2 | 5/2015  | Telfort et al.     |
| 8,718,738 | B2 | 5/2014  | Blank et al.         | 9,037,207 | B2 | 5/2015  | Al-Ali et al.      |
| 8,720,249 | B2 | 5/2014  | Al-Ali               | 9,041,529 | B2 | 5/2015  | Booij et al.       |
| 8,721,541 | B2 | 5/2014  | Al-Ali et al.        | 9,057,689 | B2 | 6/2015  | Soller             |
| 8,721,542 | B2 | 5/2014  | Al-Ali et al.        | 9,060,721 | B2 | 6/2015  | Reichgott et al.   |
| 8,723,677 | B1 | 5/2014  | Kiani                | 9,066,666 | B2 | 6/2015  | Kiani              |
| 8,725,226 | B2 | 5/2014  | Isaacson et al.      | 9,066,680 | B1 | 6/2015  | Al-Ali et al.      |
| 8,740,792 | B1 | 6/2014  | Kiani et al.         | 9,072,474 | B2 | 7/2015  | Al-Ali et al.      |
| 8,754,776 | B2 | 6/2014  | Poeze et al.         | 9,078,560 | B2 | 7/2015  | Schurman et al.    |
| 8,755,535 | B2 | 6/2014  | Telfort et al.       | 9,084,569 | B2 | 7/2015  | Weber et al.       |
| 8,755,856 | B2 | 6/2014  | Diab et al.          | 9,095,291 | B2 | 8/2015  | Soller             |
| 8,755,872 | B1 | 6/2014  | Marinow              | 9,095,316 | B2 | 8/2015  | Welch et al.       |
| 8,761,850 | B2 | 6/2014  | Lamego               | 9,106,038 | B2 | 8/2015  | Telfort et al.     |
| 8,761,852 | B2 | 6/2014  | Parthasarathy        | 9,107,625 | B2 | 8/2015  | Telfort et al.     |
| D709,846  | S  | 7/2014  | Oswaks               | 9,107,626 | B2 | 8/2015  | Al-Ali et al.      |
| 8,764,671 | B2 | 7/2014  | Kiani                | 9,113,831 | B2 | 8/2015  | Al-Ali             |
| 8,768,423 | B2 | 7/2014  | Shakespeare et al.   | 9,113,832 | B2 | 8/2015  | Al-Ali             |
| 8,771,204 | B2 | 7/2014  | Telfort et al.       | 9,119,595 | B2 | 9/2015  | Lamego             |
| 8,777,634 | B2 | 7/2014  | Kiani et al.         | 9,131,881 | B2 | 9/2015  | Diab et al.        |
| 8,781,543 | B2 | 7/2014  | Diab et al.          | 9,131,882 | B2 | 9/2015  | Al-Ali et al.      |
| 8,781,544 | B2 | 7/2014  | Al-Ali et al.        | 9,131,883 | B2 | 9/2015  | Al-Ali             |
| 8,781,549 | B2 | 7/2014  | Al-Ali et al.        | 9,131,917 | B2 | 9/2015  | Telfort et al.     |
| 8,788,003 | B2 | 7/2014  | Schurman et al.      | 9,138,180 | B1 | 9/2015  | Coverston et al.   |
| 8,790,268 | B2 | 7/2014  | Al-Ali               | 9,138,182 | B2 | 9/2015  | Al-Ali et al.      |
| 8,792,950 | B2 | 7/2014  | Larsen et al.        | 9,138,192 | B2 | 9/2015  | Weber et al.       |
| 8,801,613 | B2 | 8/2014  | Al-Ali et al.        | 9,142,117 | B2 | 9/2015  | Muhsin et al.      |
| 8,814,822 | B2 | 8/2014  | Yodfat et al.        | 9,149,228 | B2 | 10/2015 | Kinast             |
| 8,818,477 | B2 | 8/2014  | Soller               | 9,153,112 | B1 | 10/2015 | Kiani et al.       |
| 8,821,397 | B2 | 9/2014  | Al-Ali et al.        | 9,153,121 | B2 | 10/2015 | Kiani et al.       |
| 8,821,415 | B2 | 9/2014  | Al-Ali et al.        | 9,161,696 | B2 | 10/2015 | Al-Ali et al.      |
| 8,830,449 | B1 | 9/2014  | Lamego et al.        | 9,161,713 | B2 | 10/2015 | Al-Ali et al.      |
| 8,831,700 | B2 | 9/2014  | Schurman et al.      | 9,167,995 | B2 | 10/2015 | Lamego et al.      |
| 8,840,549 | B2 | 9/2014  | Al-Ali et al.        | 9,173,993 | B2 | 11/2015 | Yodfat et al.      |
| 8,845,530 | B2 | 9/2014  | Bruce et al.         | 9,176,141 | B2 | 11/2015 | Al-Ali et al.      |
| 8,847,740 | B2 | 9/2014  | Kiani et al.         | 9,183,738 | B1 | 11/2015 | Allen, Sr. et al.  |
| 8,849,365 | B2 | 9/2014  | Smith et al.         | 9,186,102 | B2 | 11/2015 | Bruinsma et al.    |
| 8,852,094 | B2 | 10/2014 | Al-Ali et al.        | 9,192,312 | B2 | 11/2015 | Al-Ali             |
| 8,852,994 | B2 | 10/2014 | Wojtczuk et al.      | 9,192,329 | B2 | 11/2015 | Al-Ali             |
| 8,866,620 | B2 | 10/2014 | Amir                 | 9,192,351 | B1 | 11/2015 | Telfort et al.     |
| 8,868,147 | B2 | 10/2014 | Stippick et al.      | 9,195,385 | B2 | 11/2015 | Al-Ali et al.      |
| 8,868,150 | B2 | 10/2014 | Al-Ali et al.        | D745,167  | S  | 12/2015 | Canas et al.       |
| 8,870,792 | B2 | 10/2014 | Al-Ali et al.        | 9,211,072 | B2 | 12/2015 | Kiani              |
| 8,873,035 | B2 | 10/2014 | Yang et al.          | 9,211,095 | B1 | 12/2015 | Al-Ali             |
| D718,455  | S  | 11/2014 | Maser et al.         | 9,218,454 | B2 | 12/2015 | Kiani et al.       |
| 8,878,888 | B2 | 11/2014 | Rosenfeld            | 9,226,696 | B2 | 1/2016  | Kiani              |
| 8,886,271 | B2 | 11/2014 | Kiani et al.         | 9,241,662 | B2 | 1/2016  | Al-Ali et al.      |
| 8,888,539 | B2 | 11/2014 | Al-Ali et al.        | 9,245,668 | B1 | 1/2016  | Vo et al.          |
| 8,888,708 | B2 | 11/2014 | Diab et al.          | 9,254,087 | B2 | 2/2016  | Isaacson et al.    |
| 8,892,180 | B2 | 11/2014 | Weber et al.         | 9,259,185 | B2 | 2/2016  | Abdul-Hafiz et al. |
| 8,897,847 | B2 | 11/2014 | Al-Ali               | 9,262,586 | B2 | 2/2016  | Steiger et al.     |
| 8,903,467 | B2 | 12/2014 | Sweitzer et al.      | 9,267,572 | B2 | 2/2016  | Barker et al.      |
| 8,907,287 | B2 | 12/2014 | Vanderpohl           | 9,277,864 | B2 | 3/2016  | Yang et al.        |
| 8,909,310 | B2 | 12/2014 | Lamego et al.        | 9,277,880 | B2 | 3/2016  | Poeze et al.       |
| 8,911,377 | B2 | 12/2014 | Al-Ali               | 9,289,167 | B2 | 3/2016  | Diab et al.        |
| 8,912,909 | B2 | 12/2014 | Al-Ali et al.        | 9,295,421 | B2 | 3/2016  | Kiani et al.       |
| 8,920,317 | B2 | 12/2014 | Al-Ali et al.        | 9,307,928 | B1 | 4/2016  | Al-Ali et al.      |
| 8,921,699 | B2 | 12/2014 | Al-Ali et al.        | 9,323,894 | B2 | 4/2016  | Kiani              |
| 8,922,382 | B2 | 12/2014 | Al-Ali et al.        | D755,392  | S  | 5/2016  | Hwang et al.       |
|           |    |         |                      | 9,326,712 | B1 | 5/2016  | Kiani              |
|           |    |         |                      | 9,333,316 | B2 | 5/2016  | Kiani              |
|           |    |         |                      | 9,339,220 | B2 | 5/2016  | Lamego et al.      |
|           |    |         |                      | 9,341,565 | B2 | 5/2016  | Lamego et al.      |

(56)

## References Cited

## U.S. PATENT DOCUMENTS

|                 |         |                  |                 |         |                     |
|-----------------|---------|------------------|-----------------|---------|---------------------|
| 9,351,673 B2    | 5/2016  | Diab et al.      | 2005/0119580 A1 | 6/2005  | Eveland             |
| 9,351,675 B2    | 5/2016  | Al-Ali et al.    | 2005/0124864 A1 | 6/2005  | Mack et al.         |
| 9,364,155 B2    | 6/2016  | Bardy et al.     | 2005/0125256 A1 | 6/2005  | Schoenberg          |
| 9,364,181 B2    | 6/2016  | Kiani et al.     | 2005/0131288 A1 | 6/2005  | Turner et al.       |
| 9,368,671 B2    | 6/2016  | Wojtczuk et al.  | 2005/0164933 A1 | 7/2005  | Tymianski et al.    |
| 9,370,325 B2    | 6/2016  | Al-Ali et al.    | 2005/0191294 A1 | 9/2005  | Arap et al.         |
| 9,370,326 B2    | 6/2016  | McHale et al.    | 2005/0197550 A1 | 9/2005  | Al-Ali et al.       |
| 9,370,335 B2    | 6/2016  | Al-ali et al.    | 2005/0228298 A1 | 10/2005 | Banet et al.        |
| 9,375,179 B2    | 6/2016  | Schultz et al.   | 2005/0228299 A1 | 10/2005 | Banet               |
| 9,375,185 B2    | 6/2016  | Ali et al.       | 2005/0234317 A1 | 10/2005 | Kiani               |
| 9,386,953 B2    | 7/2016  | Al-Ali           | 2005/0245839 A1 | 11/2005 | Stivoric et al.     |
| 9,386,961 B2    | 7/2016  | Al-Ali et al.    | 2005/0268401 A1 | 12/2005 | Dixon et al.        |
| 9,392,945 B2    | 7/2016  | Al-Ali et al.    | 2005/0277872 A1 | 12/2005 | Colby, Jr. et al.   |
| 9,397,448 B2    | 7/2016  | Al-Ali et al.    | 2006/0049936 A1 | 3/2006  | Collins, Jr. et al. |
| 9,402,544 B2    | 8/2016  | Yee et al.       | 2006/0058647 A1 | 3/2006  | Strommer et al.     |
| 9,436,645 B2    | 9/2016  | Al-Ali et al.    | 2006/0089543 A1 | 4/2006  | Kim et al.          |
| 9,439,566 B2    | 9/2016  | Arne et al.      | 2006/0089546 A1 | 4/2006  | Mahony et al.       |
| 9,480,408 B2    | 11/2016 | Isaacson et al.  | 2006/0094936 A1 | 5/2006  | Russ                |
| 9,498,158 B2    | 11/2016 | Isaacson         | 2006/0106294 A1 | 5/2006  | Maser et al.        |
| 9,529,762 B2    | 12/2016 | Gisler et al.    | 2006/0149393 A1 | 7/2006  | Calderon            |
| 2001/0011355 A1 | 8/2001  | Kawai            | 2006/0155175 A1 | 7/2006  | Ogino et al.        |
| 2001/0031922 A1 | 10/2001 | Weng et al.      | 2006/0167351 A1 | 7/2006  | Isaacson et al.     |
| 2001/0046366 A1 | 11/2001 | Susskind         | 2006/0217684 A1 | 9/2006  | Shehada et al.      |
| 2002/0045836 A1 | 4/2002  | Alkawwas         | 2006/0217685 A1 | 9/2006  | Shehada et al.      |
| 2002/0052311 A1 | 5/2002  | Solomon et al.   | 2006/0224413 A1 | 10/2006 | Kim et al.          |
| 2002/0063690 A1 | 5/2002  | Chung et al.     | 2006/0235300 A1 | 10/2006 | Weng et al.         |
| 2002/0099277 A1 | 7/2002  | Harry et al.     | 2006/0253042 A1 | 11/2006 | Stahmann et al.     |
| 2002/0107436 A1 | 8/2002  | Barton           | 2006/0276714 A1 | 12/2006 | Holt et al.         |
| 2002/0140675 A1 | 10/2002 | Ali et al.       | 2007/0000490 A1 | 1/2007  | DeVries et al.      |
| 2002/0165462 A1 | 11/2002 | Westbrook et al. | 2007/0002533 A1 | 1/2007  | Kogan et al.        |
| 2002/0177758 A1 | 11/2002 | Schoenberg       | 2007/0021675 A1 | 1/2007  | Childre et al.      |
| 2002/0198445 A1 | 12/2002 | Dominguez et al. | 2007/0027368 A1 | 2/2007  | Collins et al.      |
| 2003/0027326 A1 | 2/2003  | Ulmsten et al.   | 2007/0032733 A1 | 2/2007  | Burton et al.       |
| 2003/0033102 A1 | 2/2003  | Dietiker         | 2007/0055116 A1 | 3/2007  | Clark et al.        |
| 2003/0052787 A1 | 3/2003  | Zerhusen et al.  | 2007/0055544 A1 | 3/2007  | Jung et al.         |
| 2003/0058838 A1 | 3/2003  | Wengrovitz       | 2007/0060798 A1 | 3/2007  | Krupnik et al.      |
| 2003/0149349 A1 | 8/2003  | Jensen           | 2007/0088406 A1 | 4/2007  | Bennett et al.      |
| 2003/0158466 A1 | 8/2003  | Lynn et al.      | 2007/0096897 A1 | 5/2007  | Weiner              |
| 2003/0181798 A1 | 9/2003  | Al-Ali           | 2007/0100222 A1 | 5/2007  | Mastrototaro et al. |
| 2003/0181817 A1 | 9/2003  | Mori             | 2007/0118399 A1 | 5/2007  | Avinash et al.      |
| 2003/0214408 A1 | 11/2003 | Grajales et al.  | 2007/0140475 A1 | 6/2007  | Kurtock et al.      |
| 2003/0216670 A1 | 11/2003 | Beggs            | 2007/0156033 A1 | 7/2007  | Causey et al.       |
| 2003/0229276 A1 | 12/2003 | Sarussi et al.   | 2007/0157285 A1 | 7/2007  | Frank et al.        |
| 2004/0000713 A1 | 1/2004  | Yamashita et al. | 2007/0159332 A1 | 7/2007  | Koblasz             |
| 2004/0013647 A1 | 1/2004  | Solomon et al.   | 2007/0163589 A1 | 7/2007  | DeVries et al.      |
| 2004/0097797 A1 | 5/2004  | Porges et al.    | 2007/0185390 A1 | 8/2007  | Perkins et al.      |
| 2004/0102687 A1 | 5/2004  | Brashears et al. | 2007/0232941 A1 | 10/2007 | Rabinovich          |
| 2004/0122787 A1 | 6/2004  | Avinash et al.   | 2007/0244724 A1 | 10/2007 | Pendergast et al.   |
| 2004/0126007 A1 | 7/2004  | Ziel et al.      | 2007/0254593 A1 | 11/2007 | Jollota et al.      |
| 2004/0127775 A1 | 7/2004  | Miyazaki et al.  | 2007/0255114 A1 | 11/2007 | Ackermann et al.    |
| 2004/0139571 A1 | 7/2004  | Chang et al.     | 2007/0255116 A1 | 11/2007 | Mehta et al.        |
| 2004/0147818 A1 | 7/2004  | Levy et al.      | 2007/0255250 A1 | 11/2007 | Moberg              |
| 2004/0186357 A1 | 9/2004  | Soderberg et al. | 2007/0282478 A1 | 12/2007 | Al-Ali et al.       |
| 2004/0230118 A1 | 11/2004 | Shehada et al.   | 2008/0000479 A1 | 1/2008  | Elaz et al.         |
| 2004/0230132 A1 | 11/2004 | Shehada et al.   | 2008/0003200 A1 | 1/2008  | Arap et al.         |
| 2004/0230179 A1 | 11/2004 | Shehada et al.   | 2008/0021854 A1 | 1/2008  | Jung et al.         |
| 2004/0242976 A1 | 12/2004 | Abreu            | 2008/0033661 A1 | 2/2008  | Syroid et al.       |
| 2004/0243017 A1 | 12/2004 | Causevic         | 2008/0039701 A1 | 2/2008  | Ali et al.          |
| 2004/0249670 A1 | 12/2004 | Noguchi et al.   | 2008/0053438 A1 | 3/2008  | DeVries et al.      |
| 2004/0254431 A1 | 12/2004 | Shehada et al.   | 2008/0058657 A1 | 3/2008  | Schwartz et al.     |
| 2004/0254432 A1 | 12/2004 | Shehada et al.   | 2008/0090626 A1 | 4/2008  | Griffin et al.      |
| 2004/0260161 A1 | 12/2004 | Melker et al.    | 2008/0091089 A1 | 4/2008  | Guillory et al.     |
| 2004/0267103 A1 | 12/2004 | Li et al.        | 2008/0091090 A1 | 4/2008  | Guillory et al.     |
| 2005/0010087 A1 | 1/2005  | Banet et al.     | 2008/0091471 A1 | 4/2008  | Michon et al.       |
| 2005/0020918 A1 | 1/2005  | Wilk et al.      | 2008/0097167 A1 | 4/2008  | Yudkovitch et al.   |
| 2005/0038326 A1 | 2/2005  | Mathur           | 2008/0099366 A1 | 5/2008  | Niemiec et al.      |
| 2005/0038332 A1 | 2/2005  | Saidara et al.   | 2008/0113621 A1 | 5/2008  | Parthasarathy       |
| 2005/0038680 A1 | 2/2005  | McMahon          | 2008/0119412 A1 | 5/2008  | Tymianski et al.    |
| 2005/0070773 A1 | 3/2005  | Chin et al.      | 2008/0138278 A1 | 6/2008  | Scherz et al.       |
| 2005/0070775 A1 | 3/2005  | Chin et al.      | 2008/0169922 A1 | 7/2008  | Issokson            |
| 2005/0080336 A1 | 4/2005  | Byrd et al.      | 2008/0171919 A1 | 7/2008  | Stivoric et al.     |
| 2005/0096542 A1 | 5/2005  | Weng et al.      | 2008/0188795 A1 | 8/2008  | Katz et al.         |
| 2005/0106713 A1 | 5/2005  | Phan et al.      | 2008/0194918 A1 | 8/2008  | Kulik et al.        |
| 2005/0113653 A1 | 5/2005  | Fox et al.       | 2008/0208009 A1 | 8/2008  | Shklarski           |
| 2005/0113655 A1 | 5/2005  | Hull             | 2008/0208023 A1 | 8/2008  | Grubac et al.       |
|                 |         |                  | 2008/0208912 A1 | 8/2008  | Garibaldi           |
|                 |         |                  | 2008/0221396 A1 | 9/2008  | Garces et al.       |
|                 |         |                  | 2008/0221420 A1 | 9/2008  | Grubac et al.       |
|                 |         |                  | 2008/0222251 A1 | 9/2008  | Parthasarathy       |

(56)

## References Cited

## U.S. PATENT DOCUMENTS

|                 |         |                     |                 |         |                     |
|-----------------|---------|---------------------|-----------------|---------|---------------------|
| 2008/0228077 A1 | 9/2008  | Wilk et al.         | 2011/0087083 A1 | 4/2011  | Poeze et al.        |
| 2008/0275309 A1 | 11/2008 | Stivoric et al.     | 2011/0087084 A1 | 4/2011  | Jeong et al.        |
| 2008/0281167 A1 | 11/2008 | Soderberg et al.    | 2011/0087117 A1 | 4/2011  | Tremper et al.      |
| 2008/0281168 A1 | 11/2008 | Gibson et al.       | 2011/0087756 A1 | 4/2011  | Biondi              |
| 2008/0281181 A1 | 11/2008 | Manziona et al.     | 2011/0098583 A1 | 4/2011  | Pandia et al.       |
| 2008/0287751 A1 | 11/2008 | Stivoric et al.     | 2011/0105854 A1 | 5/2011  | Kiani et al.        |
| 2008/0292172 A1 | 11/2008 | Assmann et al.      | 2011/0105956 A1 | 5/2011  | Hirth               |
| 2008/0300020 A1 | 12/2008 | Nishizawa et al.    | 2011/0118573 A1 | 5/2011  | Mckenna             |
| 2008/0319275 A1 | 12/2008 | Chiu et al.         | 2011/0125060 A1 | 5/2011  | Telfort et al.      |
| 2008/0319354 A1 | 12/2008 | Bell et al.         | 2011/0152629 A1 | 6/2011  | Eaton et al.        |
| 2009/0005651 A1 | 1/2009  | Ward et al.         | 2011/0172967 A1 | 7/2011  | Al-Ali et al.       |
| 2009/0018808 A1 | 1/2009  | Bronstein et al.    | 2011/0184252 A1 | 7/2011  | Archer et al.       |
| 2009/0024008 A1 | 1/2009  | Brunner et al.      | 2011/0184253 A1 | 7/2011  | Archer et al.       |
| 2009/0043172 A1 | 2/2009  | Zagorchev et al.    | 2011/0208015 A1 | 8/2011  | Welch et al.        |
| 2009/0043180 A1 | 2/2009  | Tschautscher et al. | 2011/0208018 A1 | 8/2011  | Kiani               |
| 2009/0052623 A1 | 2/2009  | Tome et al.         | 2011/0208073 A1 | 8/2011  | Matsukawa et al.    |
| 2009/0054735 A1 | 2/2009  | Higgins et al.      | 2011/0209915 A1 | 9/2011  | Telfort et al.      |
| 2009/0062682 A1 | 3/2009  | Bland et al.        | 2011/0212090 A1 | 9/2011  | Pedersen et al.     |
| 2009/0069642 A1 | 3/2009  | Gao et al.          | 2011/0213212 A1 | 9/2011  | Al-Ali              |
| 2009/0099480 A1 | 4/2009  | Salgo et al.        | 2011/0227739 A1 | 9/2011  | Gilham et al.       |
| 2009/0119330 A1 | 5/2009  | Sampath et al.      | 2011/0230733 A1 | 9/2011  | Al-Ali              |
| 2009/0119843 A1 | 5/2009  | Rodgers et al.      | 2011/0237911 A1 | 9/2011  | Lamego et al.       |
| 2009/0124867 A1 | 5/2009  | Hirsh et al.        | 2011/0237969 A1 | 9/2011  | Eckerbom et al.     |
| 2009/0131759 A1 | 5/2009  | Sims et al.         | 2011/0257544 A1 | 10/2011 | Kaasinen et al.     |
| 2009/0143832 A1 | 6/2009  | Saba                | 2011/0263203 A1 | 10/2011 | Parthasarathy       |
| 2009/0157058 A1 | 6/2009  | Ferren et al.       | 2011/0288383 A1 | 11/2011 | Diab                |
| 2009/0171170 A1 | 7/2009  | Li et al.           | 2011/0295094 A1 | 12/2011 | Doyle et al.        |
| 2009/0171225 A1 | 7/2009  | Gadodia et al.      | 2011/0301444 A1 | 12/2011 | Al-Ali              |
| 2009/0177090 A1 | 7/2009  | Grunwald et al.     | 2012/0004579 A1 | 1/2012  | Luo et al.          |
| 2009/0182287 A1 | 7/2009  | Kassab              | 2012/0029300 A1 | 2/2012  | Paquet              |
| 2009/0226372 A1 | 9/2009  | Ruuslahti et al.    | 2012/0029879 A1 | 2/2012  | Sing et al.         |
| 2009/0247984 A1 | 10/2009 | Lamego et al.       | 2012/0041316 A1 | 2/2012  | Al-Ali et al.       |
| 2009/0259114 A1 | 10/2009 | Johnson et al.      | 2012/0046557 A1 | 2/2012  | Kiani               |
| 2009/0264778 A1 | 10/2009 | Markowitz et al.    | 2012/0059230 A1 | 3/2012  | Teller et al.       |
| 2009/0275813 A1 | 11/2009 | Davis               | 2012/0059267 A1 | 3/2012  | Lamego et al.       |
| 2009/0275844 A1 | 11/2009 | Al-Ali              | 2012/0071771 A1 | 3/2012  | Behar               |
| 2009/0281462 A1 | 11/2009 | Heliot et al.       | 2012/0075464 A1 | 3/2012  | Derenne et al.      |
| 2009/0299157 A1 | 12/2009 | Telfort et al.      | 2012/0088984 A1 | 4/2012  | Al-Ali et al.       |
| 2009/0299675 A1 | 12/2009 | Isaacson et al.     | 2012/0095778 A1 | 4/2012  | Gross et al.        |
| 2009/0309645 A1 | 12/2009 | Isaacson et al.     | 2012/0101353 A1 | 4/2012  | Reggiardo et al.    |
| 2009/0309755 A1 | 12/2009 | Williamson et al.   | 2012/0116175 A1 | 5/2012  | Al-Ali et al.       |
| 2009/0322540 A1 | 12/2009 | Richardson et al.   | 2012/0123799 A1 | 5/2012  | Nolen et al.        |
| 2010/0004518 A1 | 1/2010  | Vo et al.           | 2012/0136221 A1 | 5/2012  | Killen et al.       |
| 2010/0030040 A1 | 2/2010  | Poeze et al.        | 2012/0165629 A1 | 6/2012  | Merritt et al.      |
| 2010/0030094 A1 | 2/2010  | Lundback            | 2012/0179006 A1 | 7/2012  | Jansen et al.       |
| 2010/0036209 A1 | 2/2010  | Ferren et al.       | 2012/0184120 A1 | 7/2012  | Basta et al.        |
| 2010/0069725 A1 | 3/2010  | Al-Ali              | 2012/0197619 A1 | 8/2012  | Namer Yelin et al.  |
| 2010/0125188 A1 | 5/2010  | Schilling et al.    | 2012/0203078 A1 | 8/2012  | Sze et al.          |
| 2010/0125217 A1 | 5/2010  | Kuo et al.          | 2012/0209082 A1 | 8/2012  | Al-Ali              |
| 2010/0130840 A1 | 5/2010  | Isaacson et al.     | 2012/0209084 A1 | 8/2012  | Olsen et al.        |
| 2010/0144627 A1 | 6/2010  | Vitek et al.        | 2012/0226160 A1 | 9/2012  | Kudoh               |
| 2010/0185101 A1 | 7/2010  | Sakai et al.        | 2012/0227739 A1 | 9/2012  | Kiani               |
| 2010/0198622 A1 | 8/2010  | Gajic et al.        | 2012/0239434 A1 | 9/2012  | Breslow et al.      |
| 2010/0210924 A1 | 8/2010  | Parthasarathy       | 2012/0242501 A1 | 9/2012  | Tran et al.         |
| 2010/0210958 A1 | 8/2010  | Manwaring et al.    | 2012/0265039 A1 | 10/2012 | Kiani               |
| 2010/0298659 A1 | 11/2010 | McCombie et al.     | 2012/0277597 A1 | 11/2012 | Eshbaugh et al.     |
| 2010/0298660 A1 | 11/2010 | McCombie et al.     | 2012/0282583 A1 | 11/2012 | Thaler et al.       |
| 2010/0298661 A1 | 11/2010 | McCombie et al.     | 2012/0283524 A1 | 11/2012 | Kiani et al.        |
| 2010/0298742 A1 | 11/2010 | Perlman et al.      | 2012/0284053 A1 | 11/2012 | Rosenfeld           |
| 2010/0305412 A1 | 12/2010 | Darrach et al.      | 2012/0286955 A1 | 11/2012 | Welch et al.        |
| 2010/0309207 A1 | 12/2010 | Prior et al.        | 2012/0289800 A1 | 11/2012 | Isaacson et al.     |
| 2010/0312079 A1 | 12/2010 | Larsen et al.       | 2012/0294801 A1 | 11/2012 | Scherz et al.       |
| 2010/0312080 A1 | 12/2010 | Isaacson            | 2012/0296178 A1 | 11/2012 | Lamego et al.       |
| 2010/0312103 A1 | 12/2010 | Gorek et al.        | 2012/0302894 A1 | 11/2012 | Diab et al.         |
| 2010/0317936 A1 | 12/2010 | Al-Ali et al.       | 2012/0303476 A1 | 11/2012 | Krzyzanowski et al. |
| 2010/0317951 A1 | 12/2010 | Rutkowski et al.    | 2012/0304784 A1 | 12/2012 | Isaacson et al.     |
| 2011/0021930 A1 | 1/2011  | Mazzeo et al.       | 2012/0319816 A1 | 12/2012 | Al-Ali              |
| 2011/0023130 A1 | 1/2011  | Gudgel et al.       | 2012/0330112 A1 | 12/2012 | Lamego et al.       |
| 2011/0028809 A1 | 2/2011  | Goodman             | 2013/0006131 A1 | 1/2013  | Narayan et al.      |
| 2011/0046495 A1 | 2/2011  | Osypka              | 2013/0006151 A1 | 1/2013  | Main et al.         |
| 2011/0066051 A1 | 3/2011  | Moon et al.         | 2013/0023775 A1 | 1/2013  | Lamego et al.       |
| 2011/0077473 A1 | 3/2011  | Lisogurski          | 2013/0035603 A1 | 2/2013  | Jarausich et al.    |
| 2011/0078596 A1 | 3/2011  | Rawlins et al.      | 2013/0041591 A1 | 2/2013  | Lamego              |
| 2011/0080294 A1 | 4/2011  | Tanishima et al.    | 2013/0046197 A1 | 2/2013  | Dlugos, Jr. et al.  |
| 2011/0082711 A1 | 4/2011  | Poeze et al.        | 2013/0046204 A1 | 2/2013  | Lamego et al.       |
|                 |         |                     | 2013/0060108 A1 | 3/2013  | Schurman et al.     |
|                 |         |                     | 2013/0060147 A1 | 3/2013  | Welch et al.        |
|                 |         |                     | 2013/0079610 A1 | 3/2013  | Al-Ali              |
|                 |         |                     | 2013/0092805 A1 | 4/2013  | Funk et al.         |

(56)

## References Cited

## U.S. PATENT DOCUMENTS

|              |    |         |                    |              |    |         |                      |
|--------------|----|---------|--------------------|--------------|----|---------|----------------------|
| 2013/0096405 | A1 | 4/2013  | Garfio             | 2014/0194711 | A1 | 7/2014  | Al-Ali               |
| 2013/0096936 | A1 | 4/2013  | Sampath et al.     | 2014/0194766 | A1 | 7/2014  | Al-Ali et al.        |
| 2013/0109929 | A1 | 5/2013  | Menzel             | 2014/0200422 | A1 | 7/2014  | Weber et al.         |
| 2013/0109935 | A1 | 5/2013  | Al-Ali et al.      | 2014/0206963 | A1 | 7/2014  | Al-Ali               |
| 2013/0123616 | A1 | 5/2013  | Merritt et al.     | 2014/0213864 | A1 | 7/2014  | Abdul-Hafiz et al.   |
| 2013/0162433 | A1 | 6/2013  | Muhsin et al.      | 2014/0221798 | A1 | 8/2014  | Isaacson             |
| 2013/0178749 | A1 | 7/2013  | Lamego             | 2014/0243627 | A1 | 8/2014  | Diab et al.          |
| 2013/0190581 | A1 | 7/2013  | Al-Ali et al.      | 2014/0243632 | A1 | 8/2014  | Ulrich et al.        |
| 2013/0197328 | A1 | 8/2013  | Diab et al.        | 2014/0257057 | A1 | 9/2014  | Reis Cunha et al.    |
| 2013/0197364 | A1 | 8/2013  | Han                | 2014/0266787 | A1 | 9/2014  | Tran                 |
| 2013/0211214 | A1 | 8/2013  | Olsen              | 2014/0266790 | A1 | 9/2014  | Al-Ali et al.        |
| 2013/0243021 | A1 | 9/2013  | Siskavich          | 2014/0275808 | A1 | 9/2014  | Poeze et al.         |
| 2013/0253334 | A1 | 9/2013  | Al-Ali et al.      | 2014/0275816 | A1 | 9/2014  | Sandmore             |
| 2013/0261494 | A1 | 10/2013 | Bloom et al.       | 2014/0275835 | A1 | 9/2014  | Lamego et al.        |
| 2013/0267804 | A1 | 10/2013 | Al-Ali             | 2014/0275871 | A1 | 9/2014  | Lamego et al.        |
| 2013/0274571 | A1 | 10/2013 | Diab et al.        | 2014/0275872 | A1 | 9/2014  | Merritt et al.       |
| 2013/0274572 | A1 | 10/2013 | Al-Ali et al.      | 2014/0275881 | A1 | 9/2014  | Lamego et al.        |
| 2013/0279109 | A1 | 10/2013 | Lindblad et al.    | 2014/0275883 | A1 | 9/2014  | Haisley et al.       |
| 2013/0296672 | A1 | 11/2013 | O'Neil et al.      | 2014/0275885 | A1 | 9/2014  | Isaacson et al.      |
| 2013/0296713 | A1 | 11/2013 | Al-Ali et al.      | 2014/0275932 | A1 | 9/2014  | Zadig                |
| 2013/0310667 | A1 | 11/2013 | Grubac et al.      | 2014/0276115 | A1 | 9/2014  | Dalvi et al.         |
| 2013/0317327 | A1 | 11/2013 | Al-Ali et al.      | 2014/0288388 | A1 | 9/2014  | Isaacson et al.      |
| 2013/0317370 | A1 | 11/2013 | Dalvi et al.       | 2014/0288400 | A1 | 9/2014  | Diab et al.          |
| 2013/0317393 | A1 | 11/2013 | Weiss et al.       | 2014/0296664 | A1 | 10/2014 | Bruinsma et al.      |
| 2013/0324804 | A1 | 12/2013 | McKeown et al.     | 2014/0303520 | A1 | 10/2014 | Telfort et al.       |
| 2013/0324808 | A1 | 12/2013 | Al-Ali et al.      | 2014/0309506 | A1 | 10/2014 | Lamego et al.        |
| 2013/0324817 | A1 | 12/2013 | Diab               | 2014/0309559 | A1 | 10/2014 | Telfort et al.       |
| 2013/0331660 | A1 | 12/2013 | Al-Ali et al.      | 2014/0316217 | A1 | 10/2014 | Purdon et al.        |
| 2013/0331670 | A1 | 12/2013 | Kiani              | 2014/0316218 | A1 | 10/2014 | Purdon et al.        |
| 2013/0338461 | A1 | 12/2013 | Lamego et al.      | 2014/0316228 | A1 | 10/2014 | Blank et al.         |
| 2013/0340176 | A1 | 12/2013 | Stevens et al.     | 2014/0323825 | A1 | 10/2014 | Al-Ali et al.        |
| 2014/0012100 | A1 | 1/2014  | Al-Ali et al.      | 2014/0323897 | A1 | 10/2014 | Brown et al.         |
| 2014/0022081 | A1 | 1/2014  | Ribble et al.      | 2014/0323898 | A1 | 10/2014 | Purdon et al.        |
| 2014/0025306 | A1 | 1/2014  | Weber et al.       | 2014/0330092 | A1 | 11/2014 | Al-Ali et al.        |
| 2014/0031650 | A1 | 1/2014  | Weber et al.       | 2014/0330098 | A1 | 11/2014 | Merritt et al.       |
| 2014/0034353 | A1 | 2/2014  | Al-Ali et al.      | 2014/0330099 | A1 | 11/2014 | Al-Ali et al.        |
| 2014/0046674 | A1 | 2/2014  | Rosenfeld et al.   | 2014/0333440 | A1 | 11/2014 | Kiani                |
| 2014/0051952 | A1 | 2/2014  | Reichgott et al.   | 2014/0336481 | A1 | 11/2014 | Shakespeare et al.   |
| 2014/0051953 | A1 | 2/2014  | Lamego et al.      | 2014/0343389 | A1 | 11/2014 | Goldstein et al.     |
| 2014/0051954 | A1 | 2/2014  | Al-Ali et al.      | 2014/0343436 | A1 | 11/2014 | Kiani                |
| 2014/0058230 | A1 | 2/2014  | Abdul-Hafiz et al. | 2014/0343889 | A1 | 11/2014 | Ben Shalom et al.    |
| 2014/0066783 | A1 | 3/2014  | Kiani et al.       | 2014/0357966 | A1 | 12/2014 | Al-Ali et al.        |
| 2014/0066880 | A1 | 3/2014  | Prince et al.      | 2014/0357970 | A1 | 12/2014 | Larsen et al.        |
| 2014/0073167 | A1 | 3/2014  | Al-Ali et al.      | 2014/0364705 | A1 | 12/2014 | Parthasarathy et al. |
| 2014/0077956 | A1 | 3/2014  | Sampath et al.     | 2014/0371548 | A1 | 12/2014 | Al-Ali et al.        |
| 2014/0081097 | A1 | 3/2014  | Al-Ali et al.      | 2014/0371632 | A1 | 12/2014 | Al-Ali et al.        |
| 2014/0081100 | A1 | 3/2014  | Muhsin et al.      | 2014/0378784 | A1 | 12/2014 | Kiani et al.         |
| 2014/0081175 | A1 | 3/2014  | Telfort            | 2015/0005600 | A1 | 1/2015  | Blank et al.         |
| 2014/0094667 | A1 | 4/2014  | Schurman et al.    | 2015/0011907 | A1 | 1/2015  | Purdon et al.        |
| 2014/0100434 | A1 | 4/2014  | Diab et al.        | 2015/0012231 | A1 | 1/2015  | Poeze et al.         |
| 2014/0114199 | A1 | 4/2014  | Lamego et al.      | 2015/0018650 | A1 | 1/2015  | Al-Ali et al.        |
| 2014/0120564 | A1 | 5/2014  | Workman et al.     | 2015/0025406 | A1 | 1/2015  | Al-Ali               |
| 2014/0121482 | A1 | 5/2014  | Merritt et al.     | 2015/0031970 | A1 | 1/2015  | Lain                 |
| 2014/0121483 | A1 | 5/2014  | Kiani              | 2015/0032029 | A1 | 1/2015  | Al-Ali et al.        |
| 2014/0127137 | A1 | 5/2014  | Bellott et al.     | 2015/0038859 | A1 | 2/2015  | Dalvi et al.         |
| 2014/0128696 | A1 | 5/2014  | Al-Ali             | 2015/0045637 | A1 | 2/2015  | Dalvi                |
| 2014/0128699 | A1 | 5/2014  | Al-Ali et al.      | 2015/0051462 | A1 | 2/2015  | Olsen                |
| 2014/0129702 | A1 | 5/2014  | Lamego et al.      | 2015/0080754 | A1 | 3/2015  | Purdon et al.        |
| 2014/0135588 | A1 | 5/2014  | Al-Ali et al.      | 2015/0087936 | A1 | 3/2015  | Al-Ali et al.        |
| 2014/0135602 | A1 | 5/2014  | Lemke et al.       | 2015/0094546 | A1 | 4/2015  | Al-Ali               |
| 2014/0142399 | A1 | 5/2014  | Al-Ali et al.      | 2015/0094618 | A1 | 4/2015  | Russell et al.       |
| 2014/0142401 | A1 | 5/2014  | Al-Ali et al.      | 2015/0097701 | A1 | 4/2015  | Al-Ali et al.        |
| 2014/0142402 | A1 | 5/2014  | Al-Ali et al.      | 2015/0099950 | A1 | 4/2015  | Al-Ali et al.        |
| 2014/0152673 | A1 | 6/2014  | Lynn et al.        | 2015/0099951 | A1 | 4/2015  | Al-Ali et al.        |
| 2014/0155712 | A1 | 6/2014  | Lamego et al.      | 2015/0099955 | A1 | 4/2015  | Al-Ali et al.        |
| 2014/0163344 | A1 | 6/2014  | Al-Ali             | 2015/0101844 | A1 | 4/2015  | Al-Ali et al.        |
| 2014/0163402 | A1 | 6/2014  | Lamego et al.      | 2015/0106121 | A1 | 4/2015  | Muhsin et al.        |
| 2014/0166076 | A1 | 6/2014  | Kiani et al.       | 2015/0112151 | A1 | 4/2015  | Muhsin et al.        |
| 2014/0171763 | A1 | 6/2014  | Diab               | 2015/0116076 | A1 | 4/2015  | Al-Ali et al.        |
| 2014/0180038 | A1 | 6/2014  | Kiani              | 2015/0126830 | A1 | 5/2015  | Schurman et al.      |
| 2014/0180154 | A1 | 6/2014  | Sierra et al.      | 2015/0133755 | A1 | 5/2015  | Smith et al.         |
| 2014/0180160 | A1 | 6/2014  | Brown et al.       | 2015/0140863 | A1 | 5/2015  | Al-Ali et al.        |
| 2014/0187973 | A1 | 7/2014  | Brown et al.       | 2015/0141779 | A1 | 5/2015  | Johnson et al.       |
| 2014/0188516 | A1 | 7/2014  | Kamen et al.       | 2015/0141780 | A1 | 5/2015  | Meyer et al.         |
| 2014/0194709 | A1 | 7/2014  | Al-Ali et al.      | 2015/0141781 | A1 | 5/2015  | Weber et al.         |
|              |    |         |                    | 2015/0165312 | A1 | 6/2015  | Kiani                |
|              |    |         |                    | 2015/0196237 | A1 | 7/2015  | Lamego               |
|              |    |         |                    | 2015/0201874 | A1 | 7/2015  | Diab                 |
|              |    |         |                    | 2015/0208966 | A1 | 7/2015  | Al-Ali               |

(56)

## References Cited

## U.S. PATENT DOCUMENTS

|              |    |         |                  |
|--------------|----|---------|------------------|
| 2015/0216459 | A1 | 8/2015  | Al-Ali et al.    |
| 2015/0230755 | A1 | 8/2015  | Al-Ali et al.    |
| 2015/0238094 | A1 | 8/2015  | Lai et al.       |
| 2015/0238722 | A1 | 8/2015  | Al-Ali           |
| 2015/0245773 | A1 | 9/2015  | Lamego et al.    |
| 2015/0245794 | A1 | 9/2015  | Al-Ali           |
| 2015/0257689 | A1 | 9/2015  | Al-Ali et al.    |
| 2015/0272514 | A1 | 10/2015 | Kiani et al.     |
| 2015/0289814 | A1 | 10/2015 | Magar et al.     |
| 2015/0351697 | A1 | 12/2015 | Weber et al.     |
| 2015/0351704 | A1 | 12/2015 | Kiani et al.     |
| 2015/0359429 | A1 | 12/2015 | Al-Ali et al.    |
| 2015/0366472 | A1 | 12/2015 | Kiani            |
| 2015/0366507 | A1 | 12/2015 | Blank            |
| 2015/0374298 | A1 | 12/2015 | Al-Ali et al.    |
| 2015/0374905 | A1 | 12/2015 | Yodfat et al.    |
| 2015/0380875 | A1 | 12/2015 | Coverston et al. |
| 2016/0000362 | A1 | 1/2016  | Diab et al.      |
| 2016/0007930 | A1 | 1/2016  | Weber et al.     |
| 2016/0029932 | A1 | 2/2016  | Al-Ali           |
| 2016/0029933 | A1 | 2/2016  | Al-Ali et al.    |
| 2016/0045118 | A1 | 2/2016  | Kiani            |
| 2016/0051205 | A1 | 2/2016  | Al-Ali et al.    |
| 2016/0058338 | A1 | 3/2016  | Schurman et al.  |
| 2016/0058347 | A1 | 3/2016  | Reichgott et al. |
| 2016/0066823 | A1 | 3/2016  | Al-Ali et al.    |
| 2016/0066824 | A1 | 3/2016  | Al-Ali et al.    |
| 2016/0066879 | A1 | 3/2016  | Telfort et al.   |
| 2016/0072429 | A1 | 3/2016  | Kiani et al.     |
| 2016/0073967 | A1 | 3/2016  | Lamego et al.    |
| 2016/0081552 | A1 | 3/2016  | Wojtczuk et al.  |
| 2016/0095543 | A1 | 4/2016  | Telfort et al.   |
| 2016/0095548 | A1 | 4/2016  | Al-Ali et al.    |
| 2016/0103598 | A1 | 4/2016  | Al-Ali et al.    |
| 2016/0106914 | A1 | 4/2016  | Yodfat et al.    |
| 2016/0113527 | A1 | 4/2016  | Al-Ali           |
| 2016/0143548 | A1 | 5/2016  | Al-Ali           |
| 2016/0166183 | A1 | 6/2016  | Poeze et al.     |
| 2016/0166188 | A1 | 6/2016  | Bruinsma et al.  |
| 2016/0166210 | A1 | 6/2016  | Al-Ali           |
| 2016/0166213 | A1 | 6/2016  | Isaacson         |
| 2016/0192869 | A1 | 7/2016  | Kiani et al.     |
| 2016/0196388 | A1 | 7/2016  | Lamego           |
| 2016/0197436 | A1 | 7/2016  | Barker et al.    |
| 2016/0213281 | A1 | 7/2016  | Eckerbom et al.  |
| 2016/0235344 | A1 | 8/2016  | Auerbach         |
| 2016/0262673 | A1 | 9/2016  | Skorich et al.   |
| 2016/0324486 | A1 | 11/2016 | Al-Ali et al.    |
| 2016/0327984 | A1 | 11/2016 | Al-Ali et al.    |
| 2016/0328528 | A1 | 11/2016 | Al-Ali et al.    |
| 2016/0359150 | A1 | 12/2016 | Martin et al.    |
| 2016/0367164 | A1 | 12/2016 | Felix            |

## FOREIGN PATENT DOCUMENTS

|    |             |         |
|----|-------------|---------|
| EP | 1408823     | 5/2010  |
| EP | 2 335 569   | 6/2011  |
| EP | 2 766 834   | 8/2014  |
| EP | 2 811 894   | 12/2014 |
| JP | 10-336064   | 12/1998 |
| JP | 2001-501847 | 2/2001  |
| JP | 2002-165764 | 6/2002  |
| JP | 2002-172096 | 6/2002  |
| JP | 2003-275183 | 9/2003  |
| JP | 2004-024551 | 1/2004  |
| JP | 2005-218036 | 8/2005  |
| JP | 2005-295375 | 10/2005 |
| JP | 2007-021213 | 2/2007  |
| JP | 2007-095365 | 4/2007  |
| JP | 2007-174051 | 7/2007  |
| JP | 2008-541045 | 11/2008 |
| JP | 2009-017959 | 1/2009  |
| JP | 2009-207836 | 9/2009  |
| JP | 2010-503134 | 1/2010  |
| JP | 2010-524510 | 7/2010  |

|    |                |         |
|----|----------------|---------|
| JP | 2011-519607    | 7/2011  |
| JP | 2011-152261    | 8/2011  |
| JP | 2014-533997    | 12/2014 |
| RU | 2199723        | 2/2003  |
| WO | WO 96/16591    | 6/1996  |
| WO | WO 97/00708    | 1/1997  |
| WO | WO 98/15224    | 4/1998  |
| WO | WO 98/29790    | 7/1998  |
| WO | WO 98/39749    | 9/1998  |
| WO | WO 99/13766    | 3/1999  |
| WO | WO 99/56613    | 11/1999 |
| WO | WO 00/62665    | 10/2000 |
| WO | WO 00/63713    | 10/2000 |
| WO | WO 00/69328    | 11/2000 |
| WO | WO 01/41634    | 6/2001  |
| WO | WO 03/065926   | 8/2003  |
| WO | WO 2004/056266 | 7/2004  |
| WO | WO 2004/059551 | 7/2004  |
| WO | WO 2005/048830 | 6/2005  |
| WO | WO 2005/092177 | 10/2005 |
| WO | WO 2006/051461 | 5/2006  |
| WO | WO 2011/001302 | 1/2011  |
| WO | WO 2011/002904 | 1/2011  |
| WO | WO 2011/025549 | 3/2011  |
| WO | WO 2013/056160 | 4/2013  |
| WO | WO 2013/119982 | 8/2013  |
| WO | WO 2015/054665 | 4/2015  |

## OTHER PUBLICATIONS

Capuano et al., "Remote Telemetry—New Twists for Old Technology", *Nursing Management*, Jul. 1995, vol. 26, No. 7, pp. 26-32.

Elmer-Dewitt, Philip, "Apple's iWatch: The killer apps may be in hospitals, not health clubs", *Fortune.com*, Feb. 3, 2014, <http://fortune.com/2012/02/03/apples-iwatch-the-killer-apps-may-me-in-hospitals-not-health-clubs/>, 4 pages.

Grundy et al., "Telemedicine in Critical Care: An Experiment in Health Care Delivery", *JACEP*, Oct. 1977, vol. 6, No. 10, pp. 439-444.

Grundy et al., "Telemedicine in Critical Care: Problems in Design, Implementation and Assessment", *Jul. 1982*, vol. 10, No. 7, pp. 471-475.

Rysavy, Peter, "Making the Call with Two-Way Paging", *Network Computing*, Published Jan. 15, 1997, [www.rysavy.com/Articles/twoway.htm](http://www.rysavy.com/Articles/twoway.htm), pp. 5.

Wachter et al., "The Employment of an Iterative Design Process to Develop a Pulmonary Graphical Display", *Journal of the American Medical Informatics Association*, vol. 10, No. 4, Jul./Aug. 2003, pp. 363-372.

Official Communication in European Application No. 10195398.2 dated Jul. 5, 2012.

Official Communication in European Application No. 10195398.2 dated Jun. 15, 2015.

International Search Report & Written Opinion in PCT Application No. PCT/US2013/025384, dated Aug. 6, 2013.

International Search Report & Written Opinion in PCT Application No. PCT/US2012/060109, dated Jun. 5, 2013.

International Preliminary Report on Patentability in PCT Application No. PCT/US2012/060109, dated Apr. 24, 2014.

International Search Report & Written Opinion in PCT Application No. PCT/US2014/060177, dated Dec. 19, 2014.

International Preliminary Report on Patentability & Written Opinion in PCT Application No. PCT/US2013/025384, dated Aug. 21, 2014.

International Preliminary Report on Patentability & Written Opinion in PCT Application No. PCT/US2014/060177, dated Apr. 21, 2016.

Crilly et al., "An Integrated Pulse Oximeter System for Telemedicine Applications", *IEEE Instrumentation and Measurement Technology Conference*, Ottawa, Canada, May 19-21, 1997, in 3 pages.

"Medicine" *Textbook of Anaesthesiology*/Ed. By Aitkonhead A.R. et al., vol. 1, 1999, pp. 437-440.

(56)

**References Cited**

OTHER PUBLICATIONS

Dissertation thesis for an MBA class given by the inventor on Dec. 18, 2004. "Reducing Health Care Costs and improving Patient Care with the Uni-Ox Pulse Oximeter from Snap Medical Technologies", Robert Sweitzer and Samantha Goetz, in 7 pages.

European Search Report in EP Application No. 02 748 235.5, dated Oct. 4, 2006.

Official Communication in EP Application No. 02 748 235.5, dated Jul. 25, 2008.

International Search Report in PCT Application No. PCT/US02/03434, dated Dec. 19, 2002.

\* cited by examiner

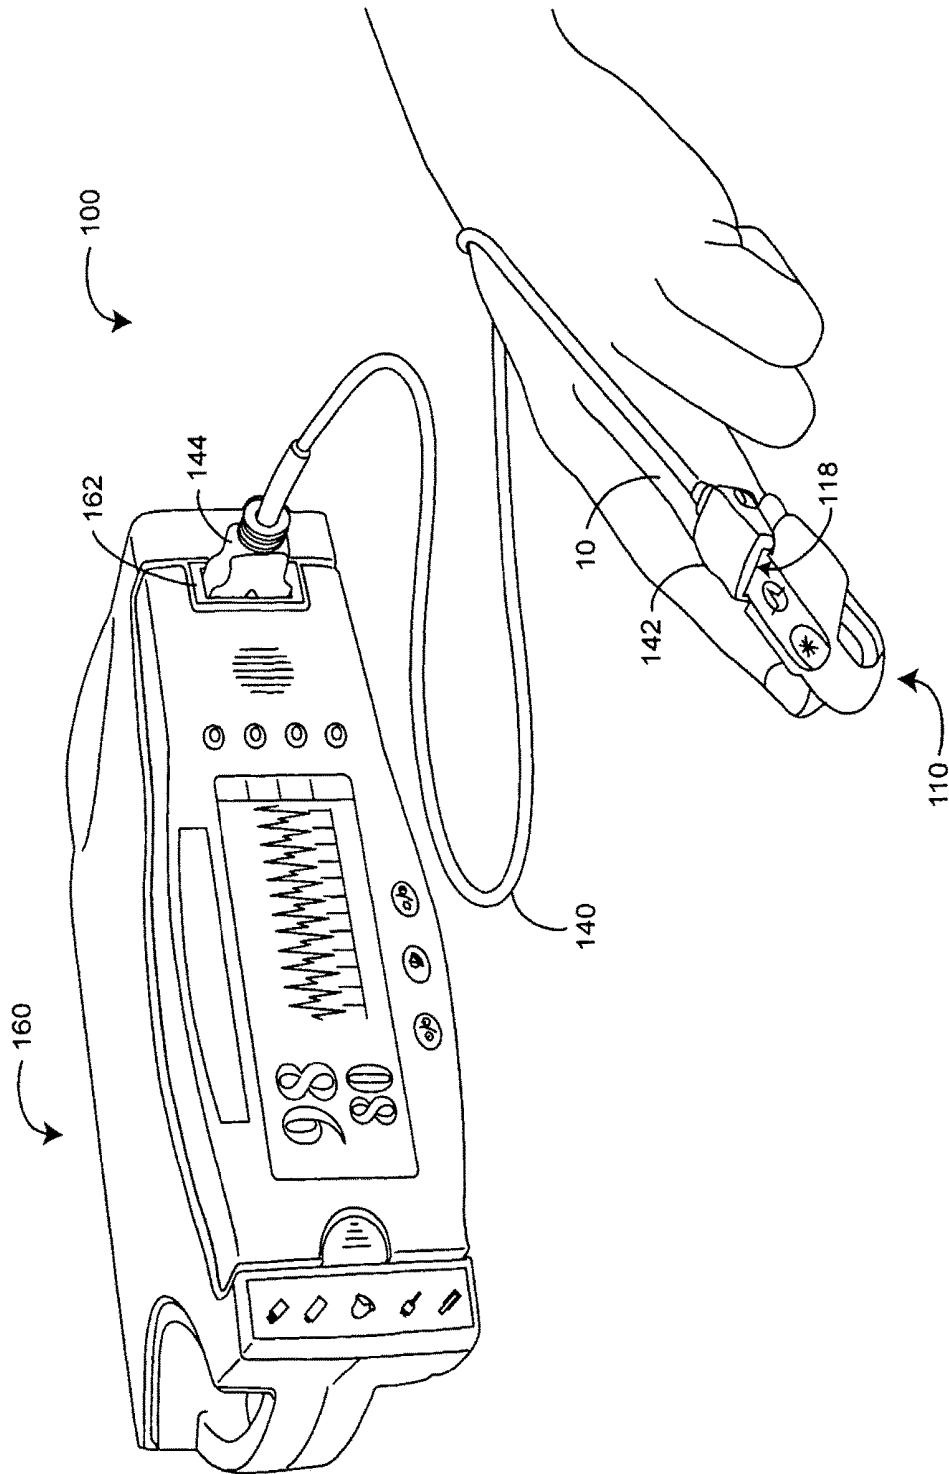


FIG. 1 (Prior Art)

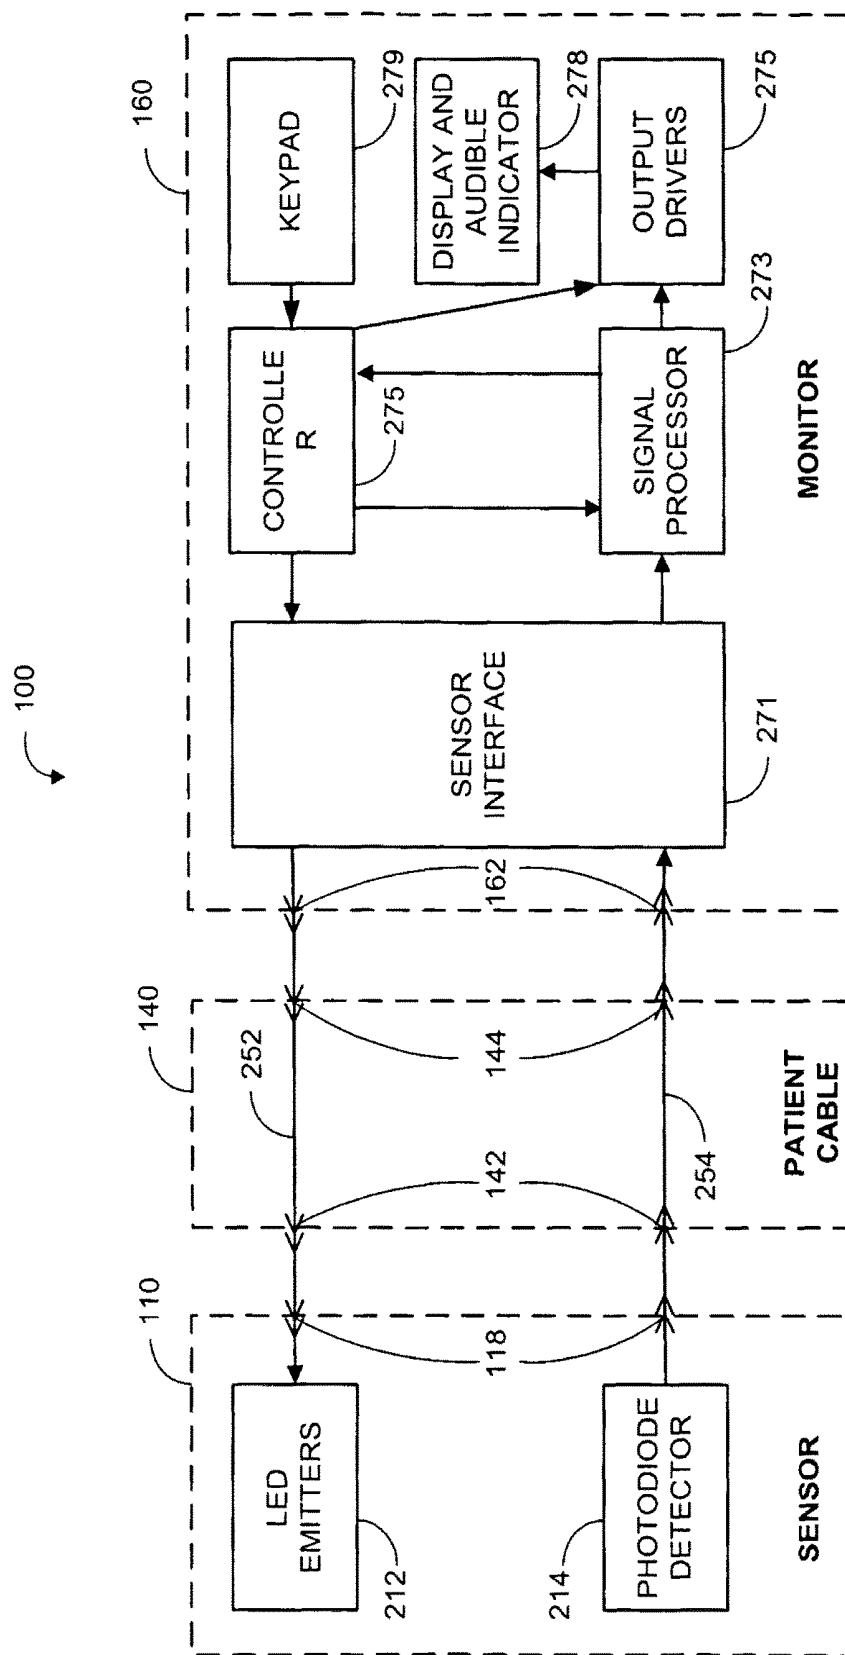


FIG. 2 (Prior Art)

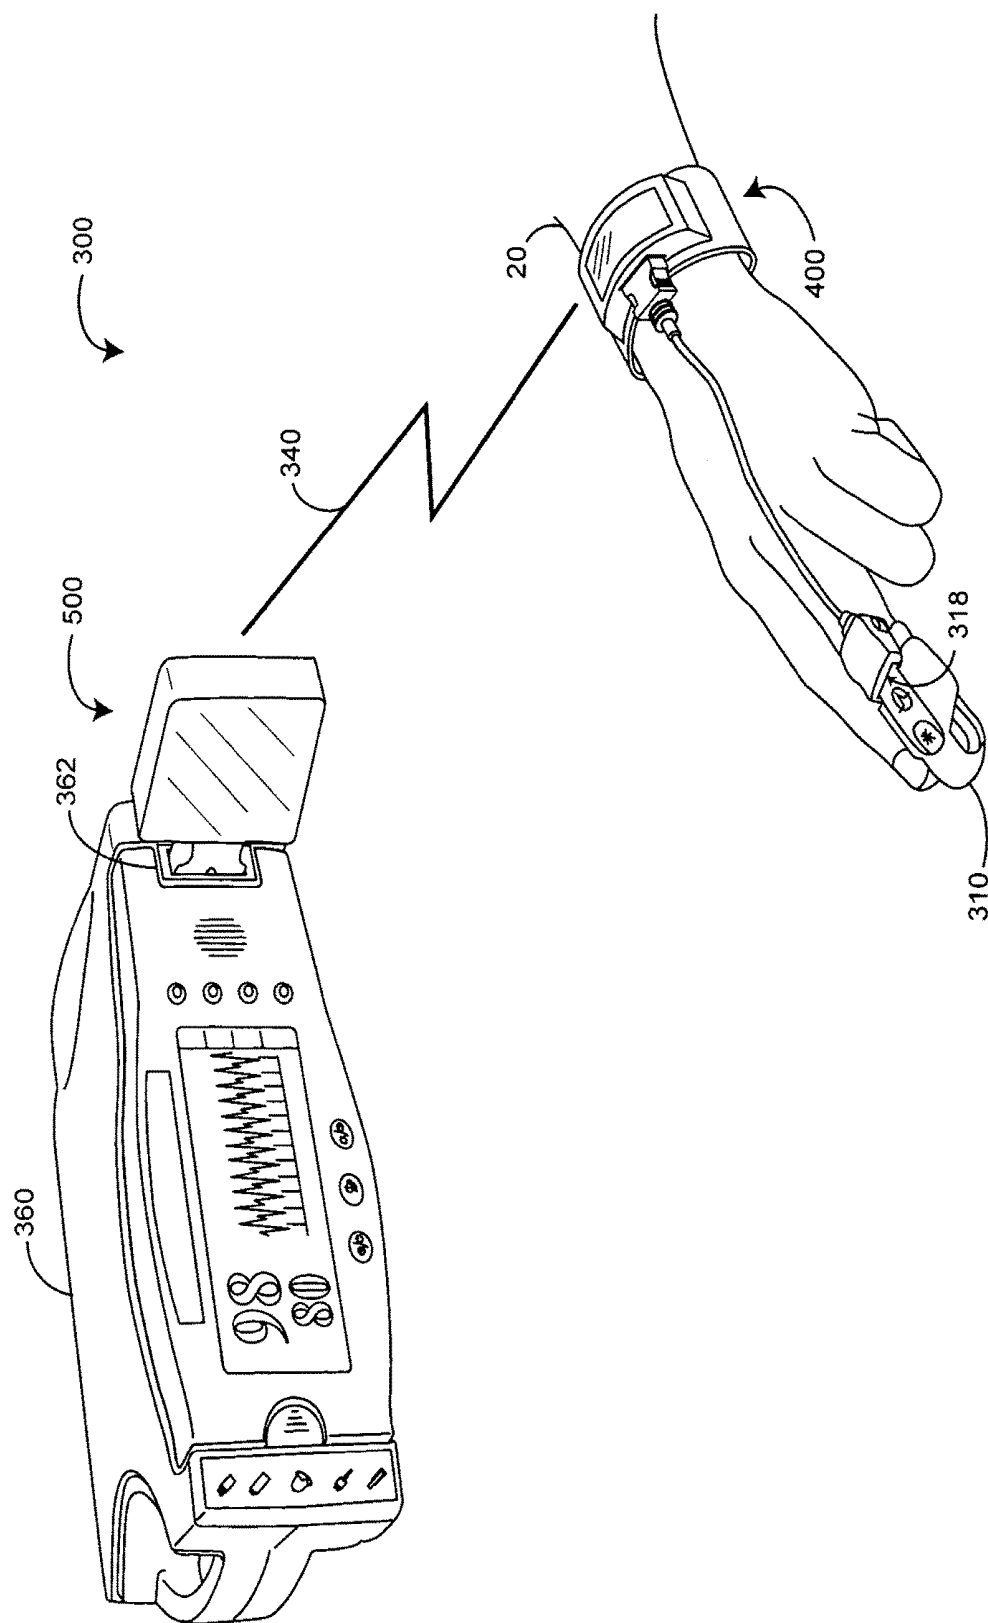


FIG. 3

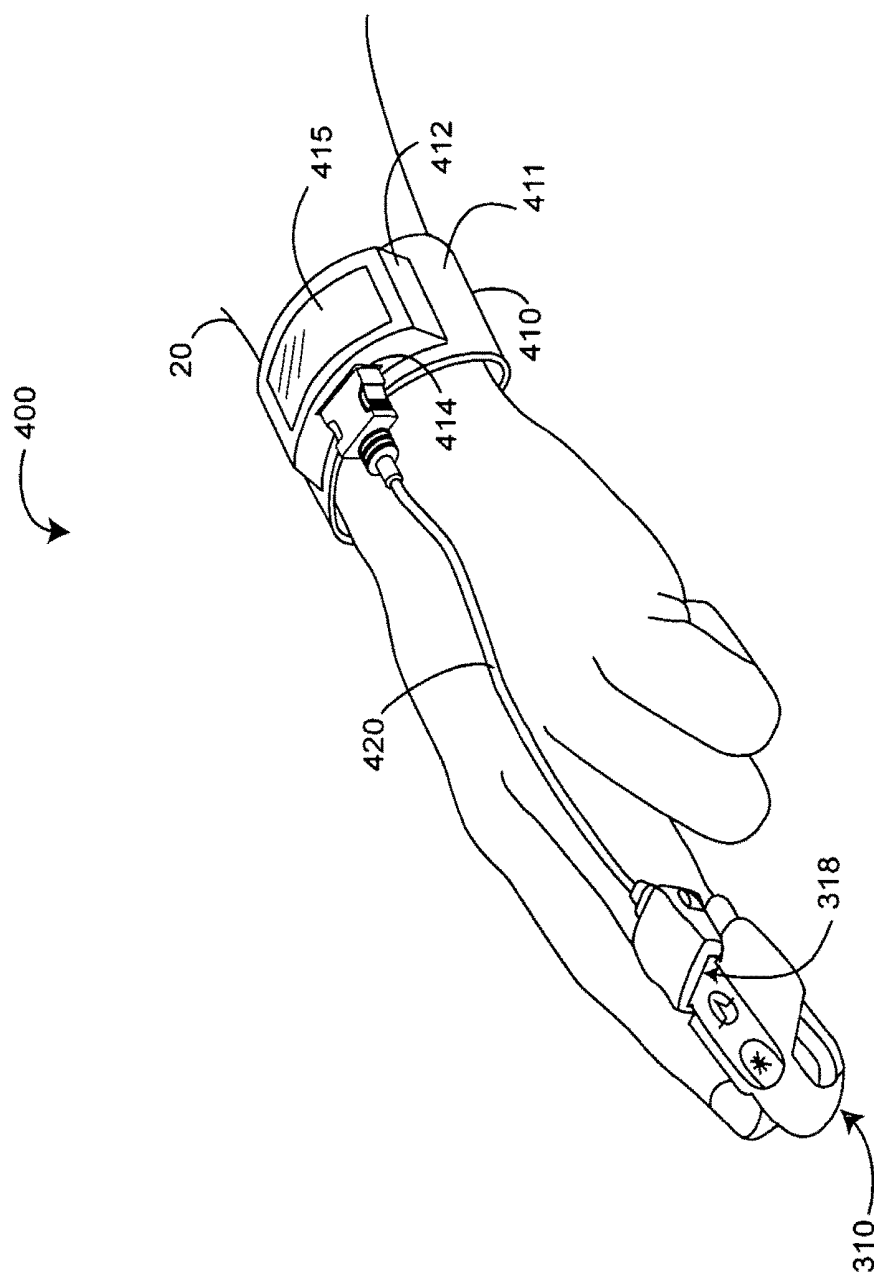


FIG. 4A

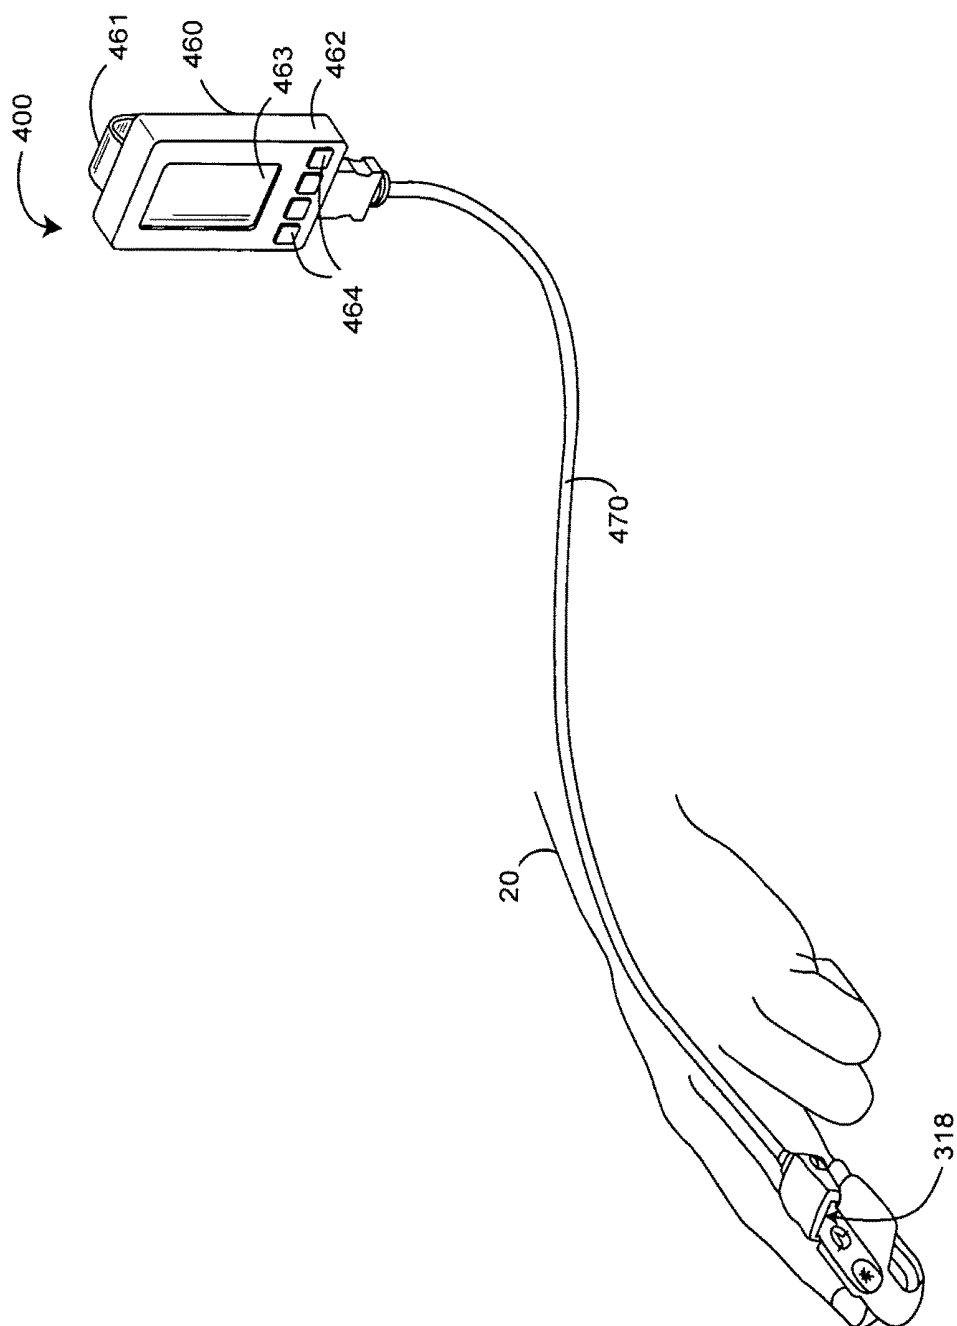


FIG. 4B

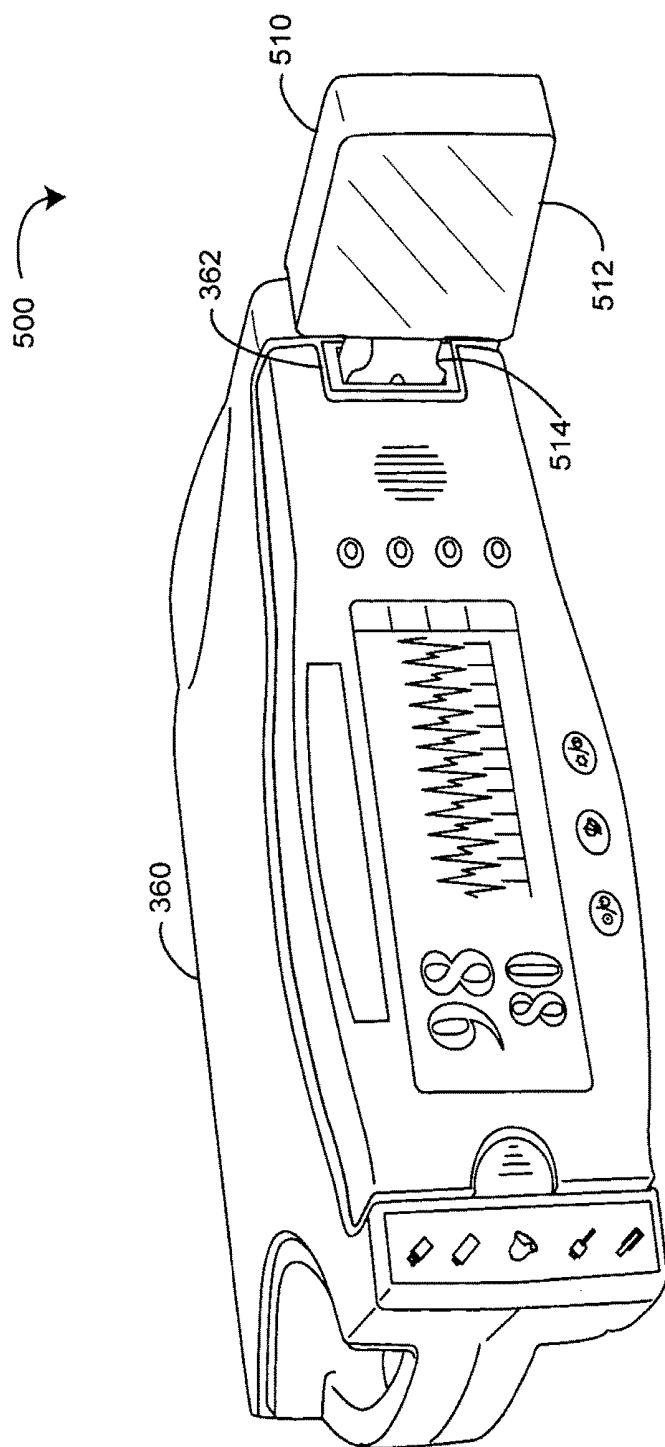


FIG. 5A

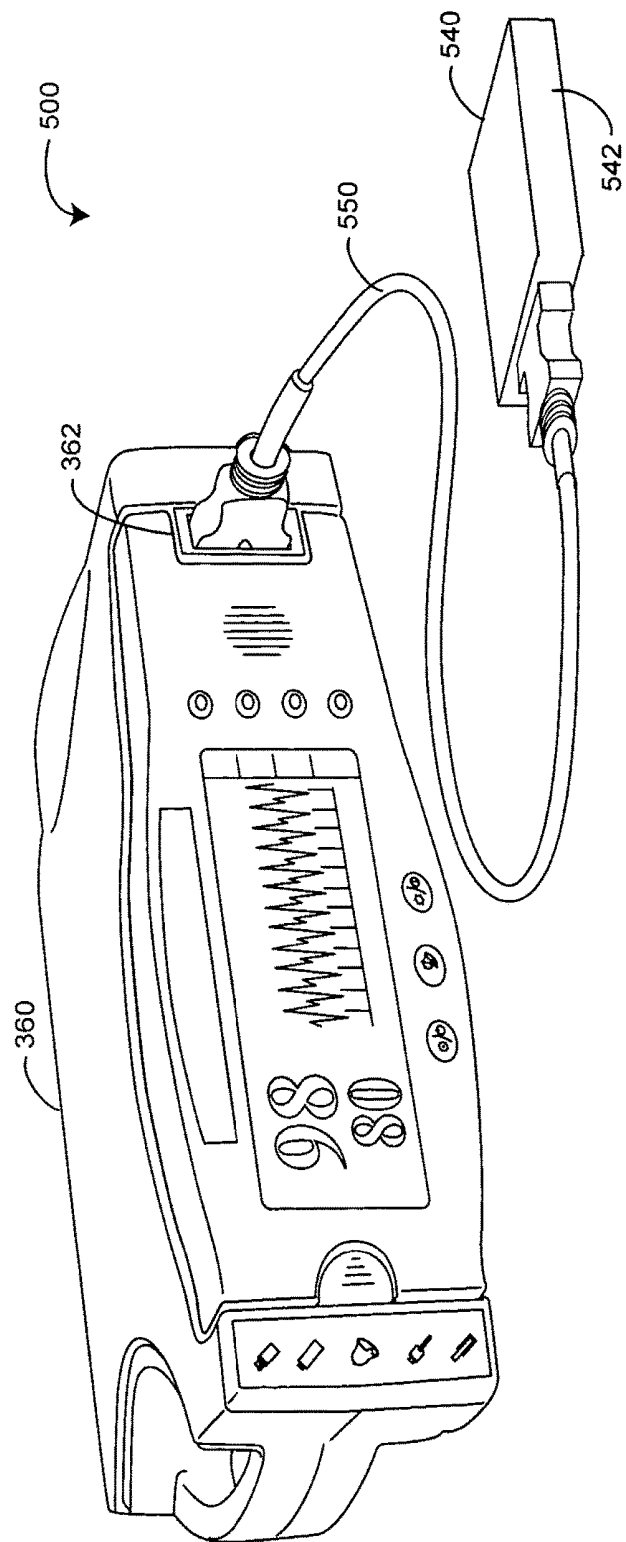


FIG. 5B

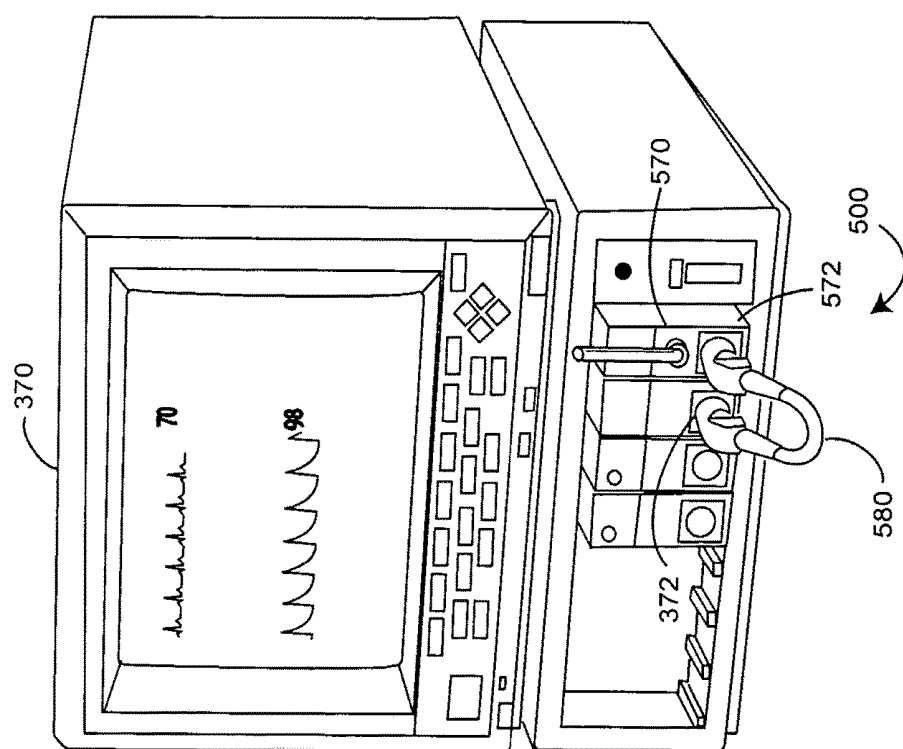


FIG. 5C

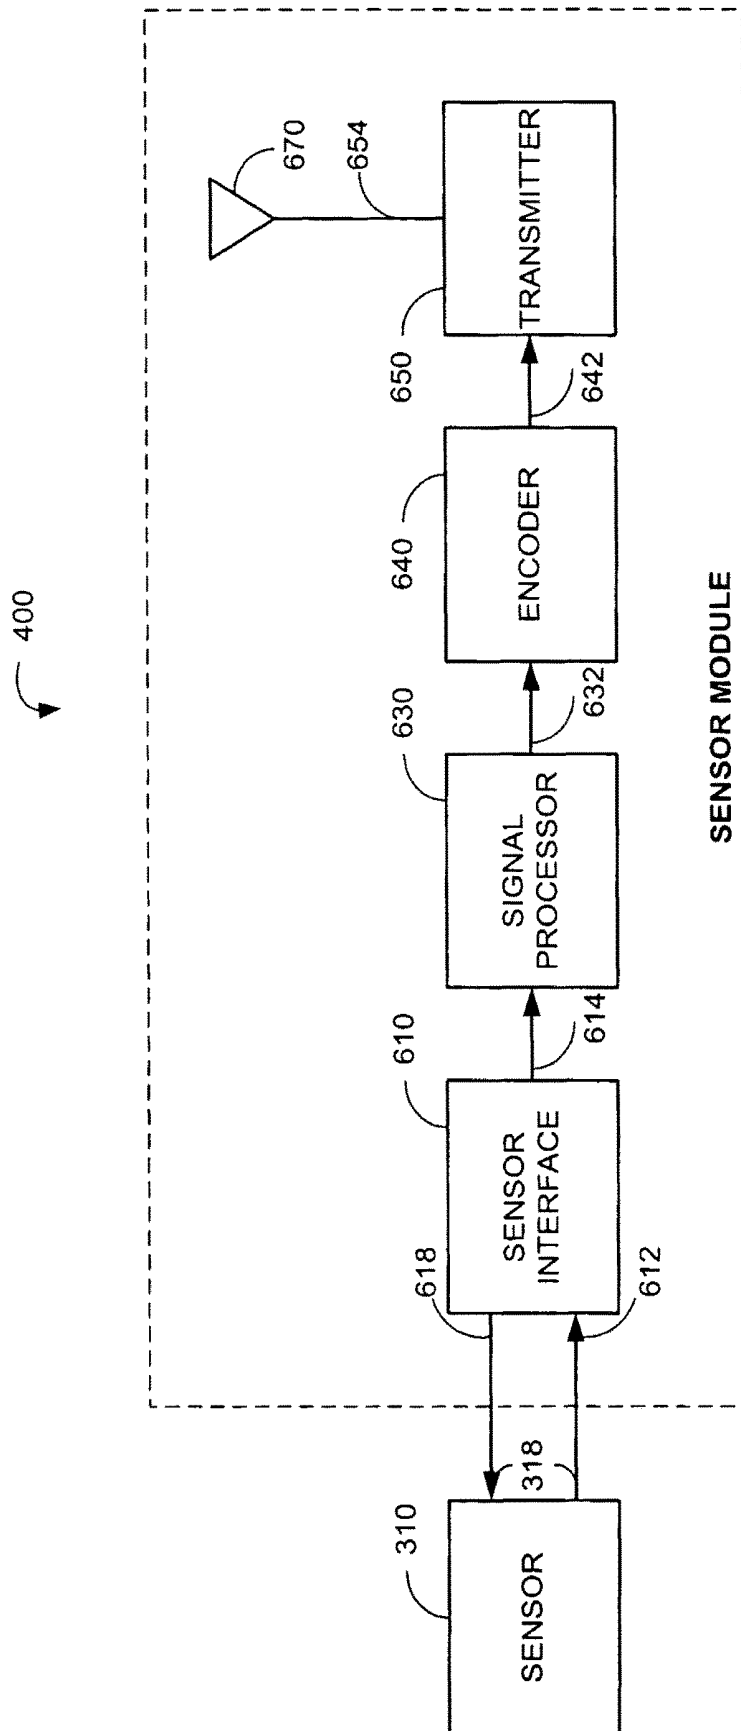


FIG. 6

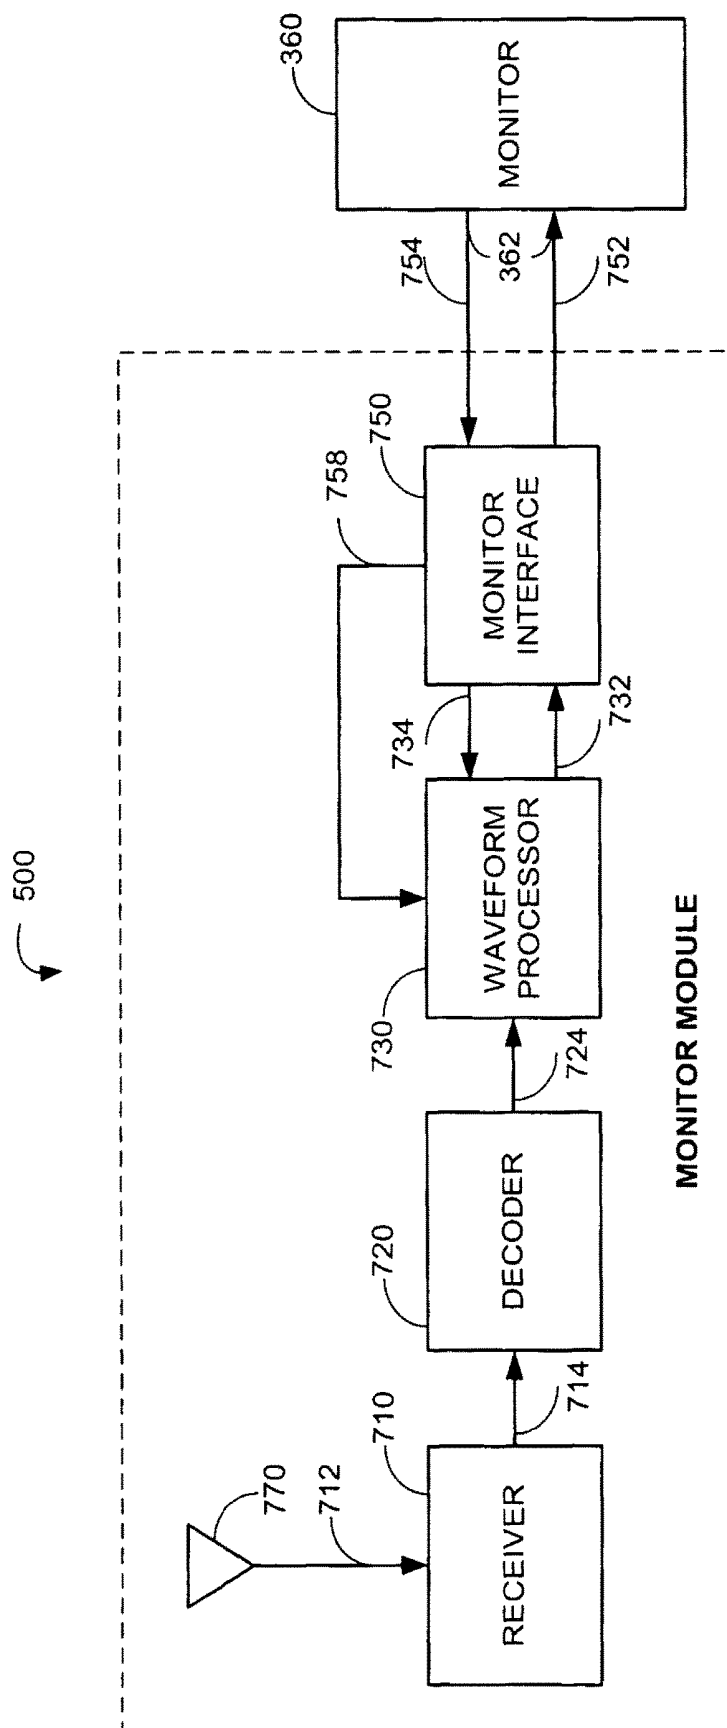


FIG. 7

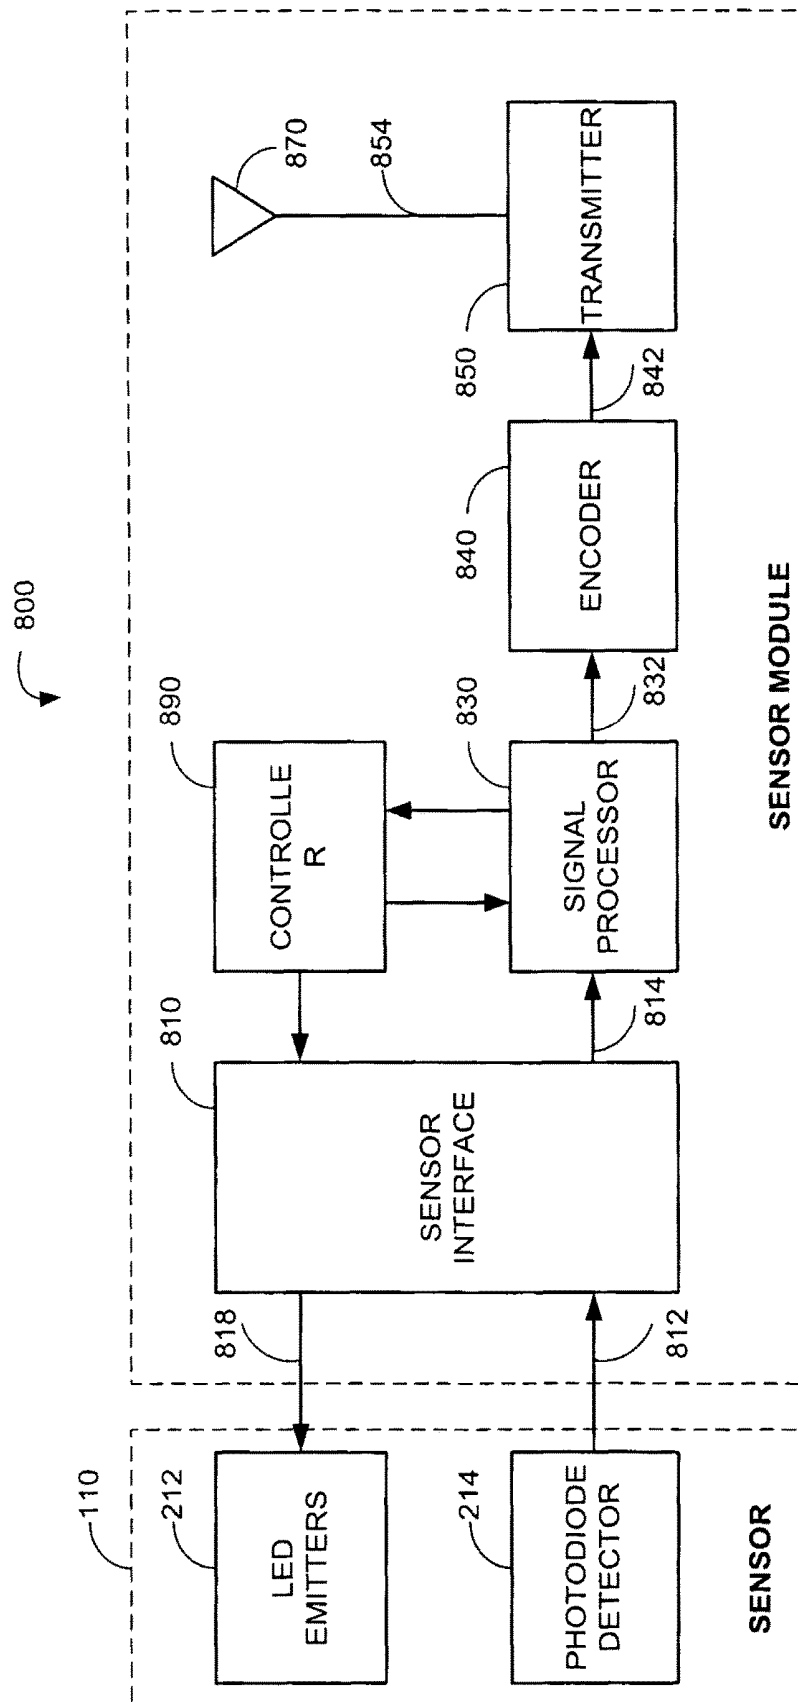


FIG. 8

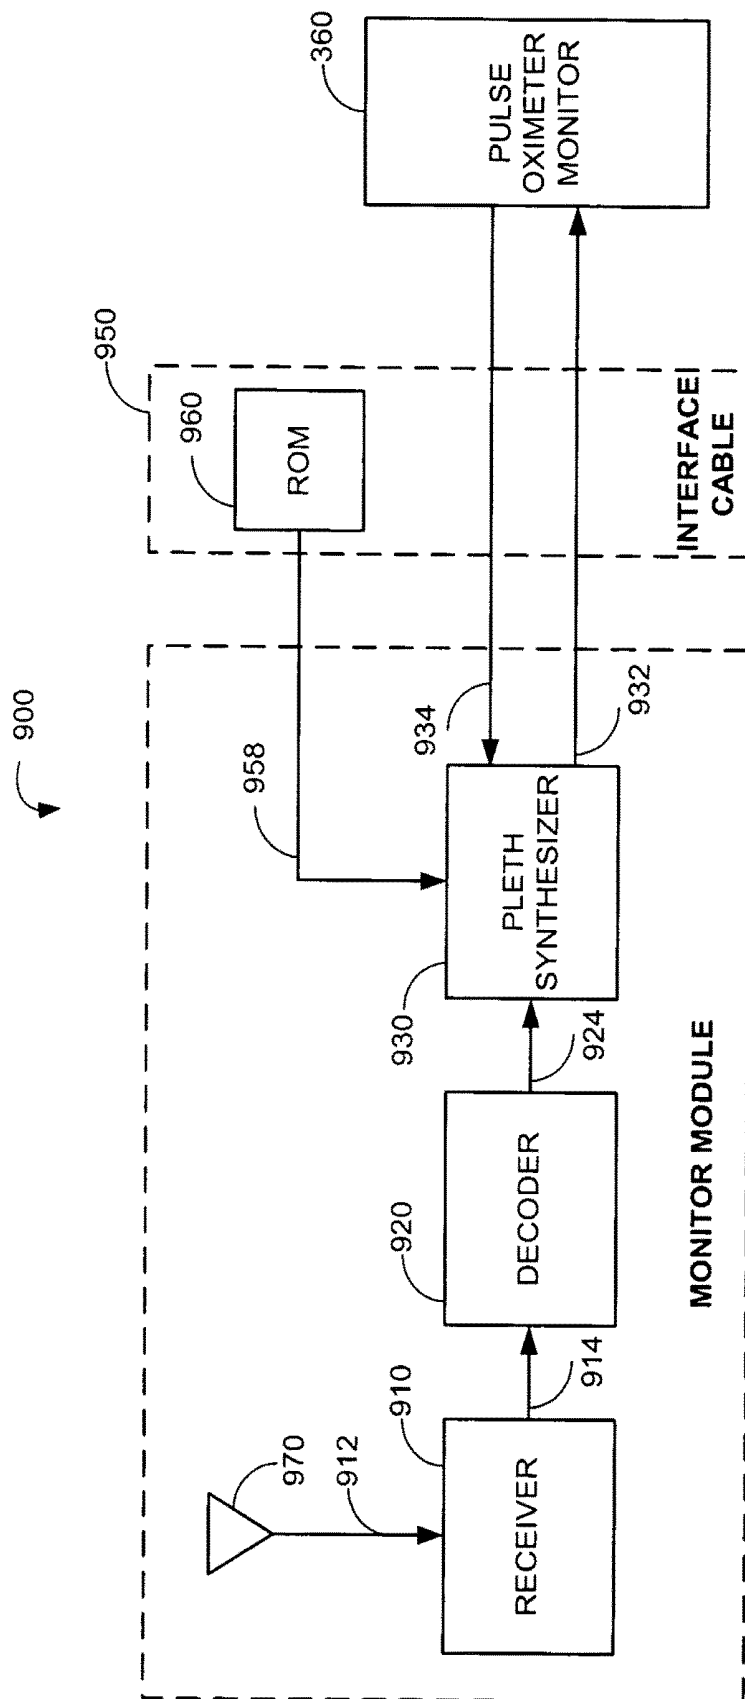


FIG. 9

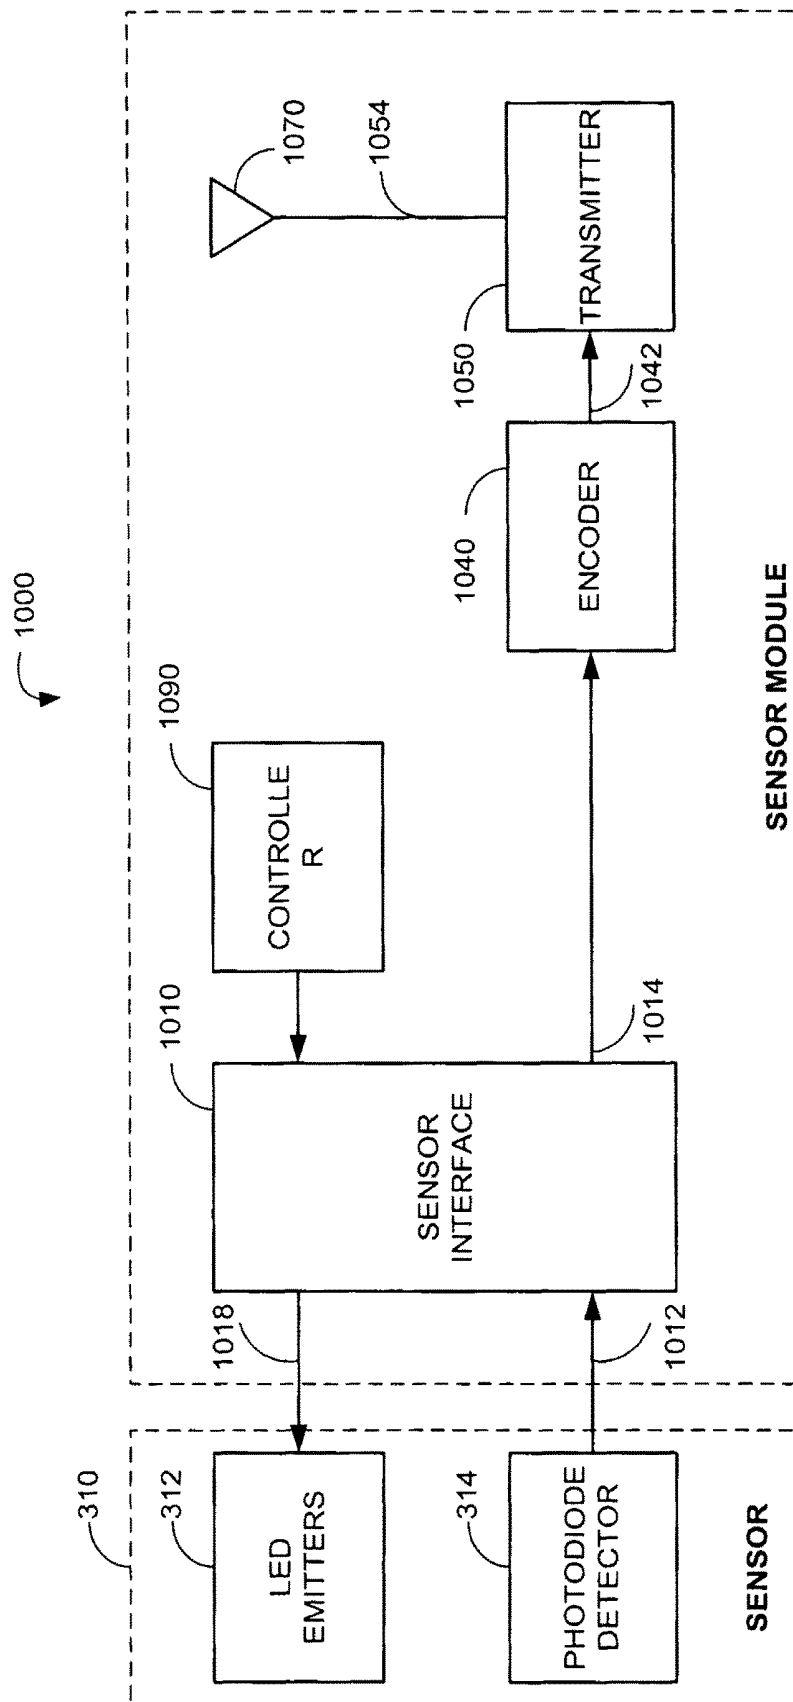


FIG. 10

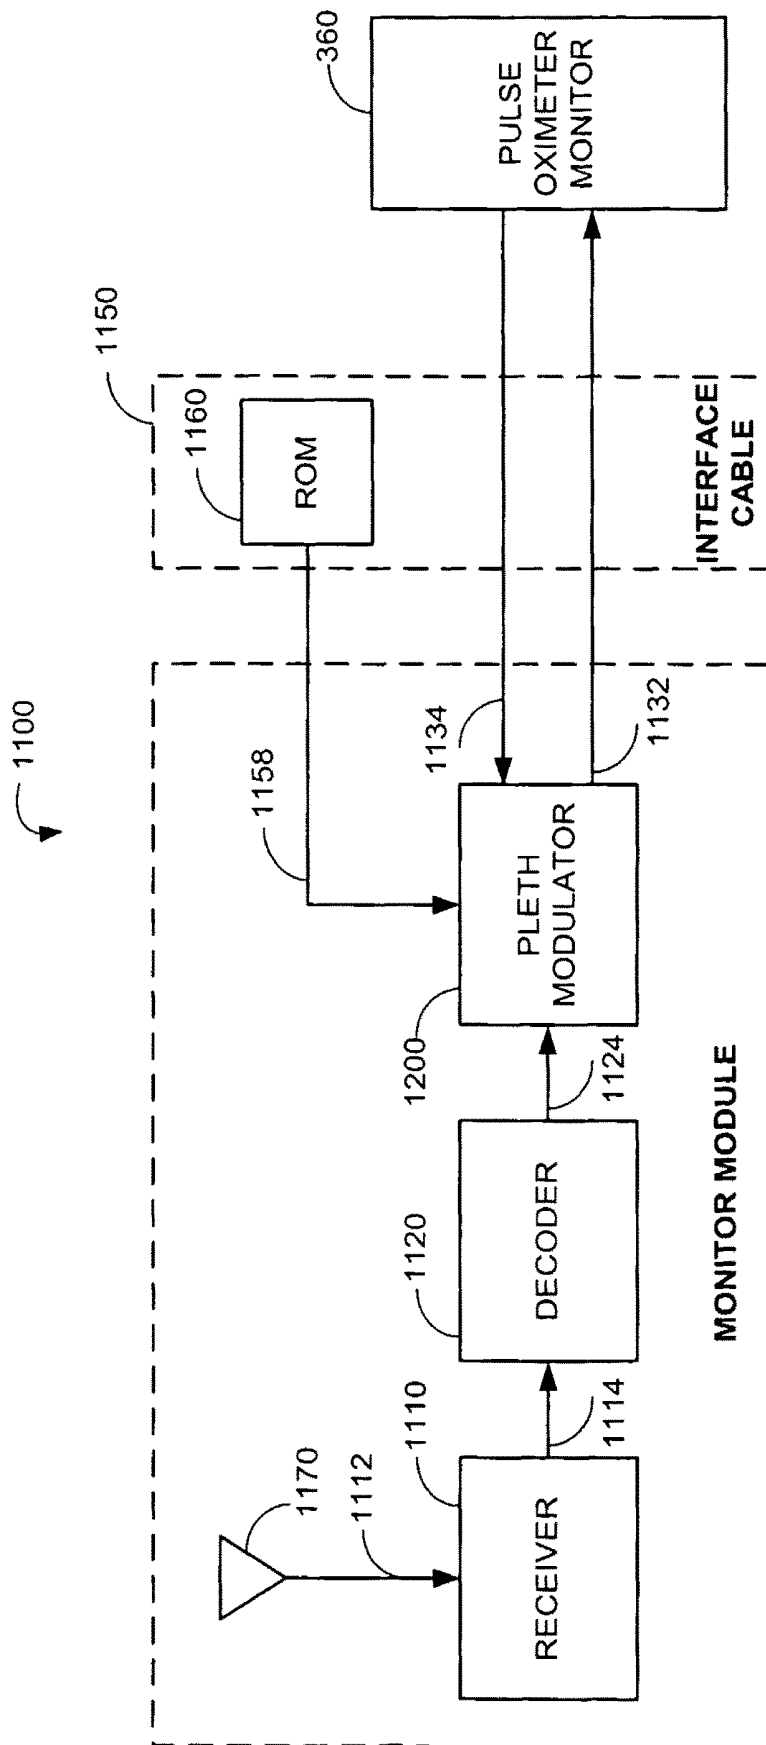


FIG. 11

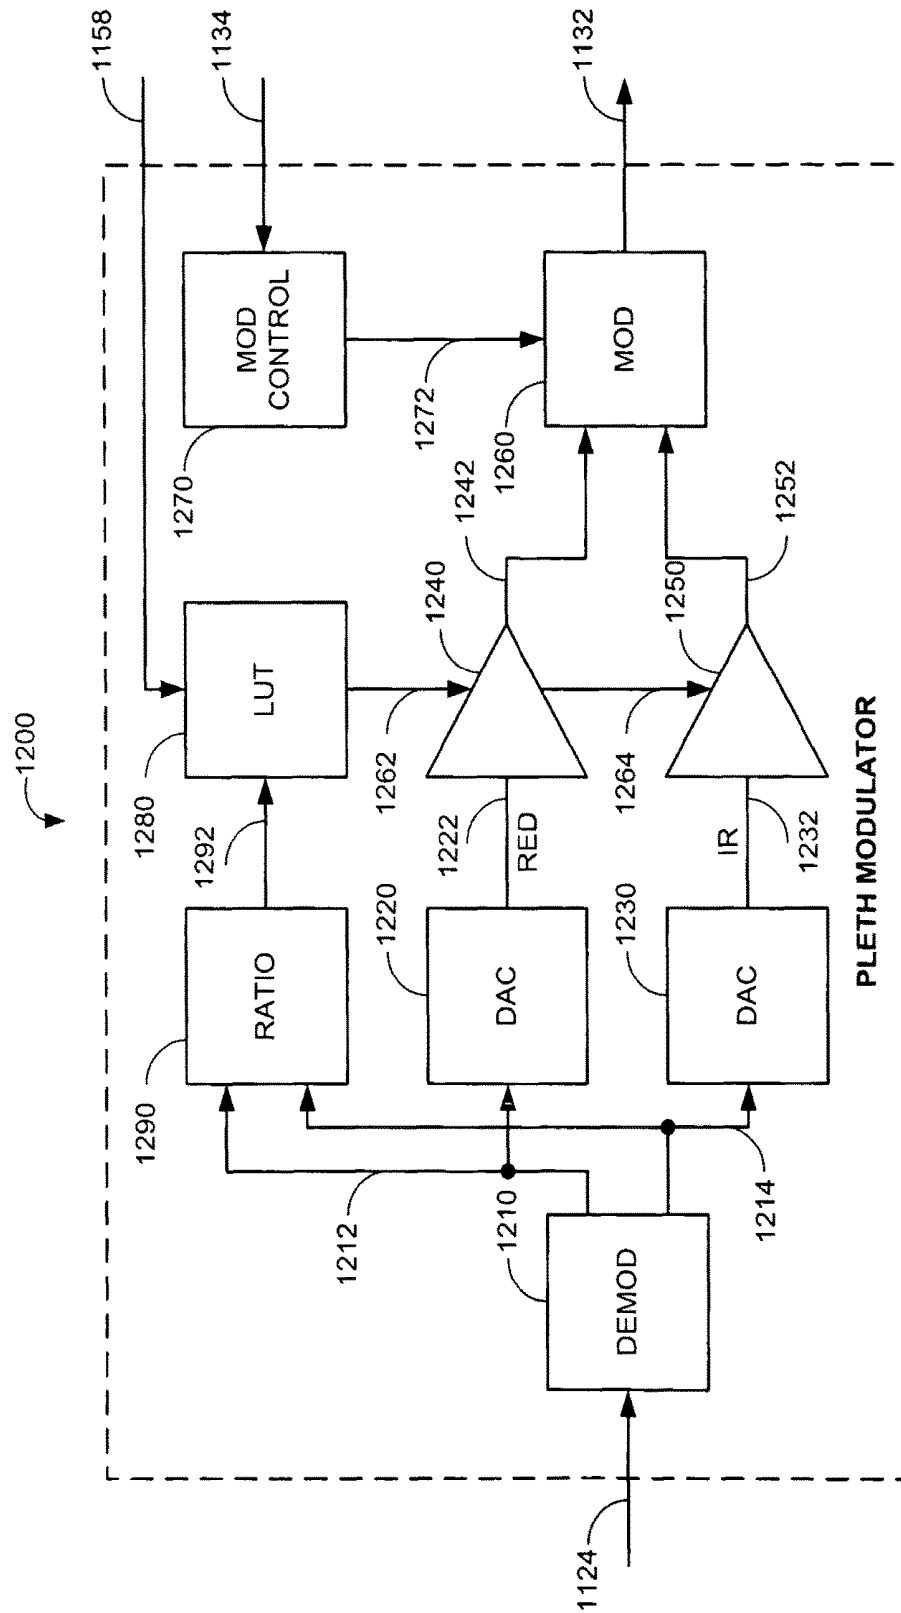


FIG. 12

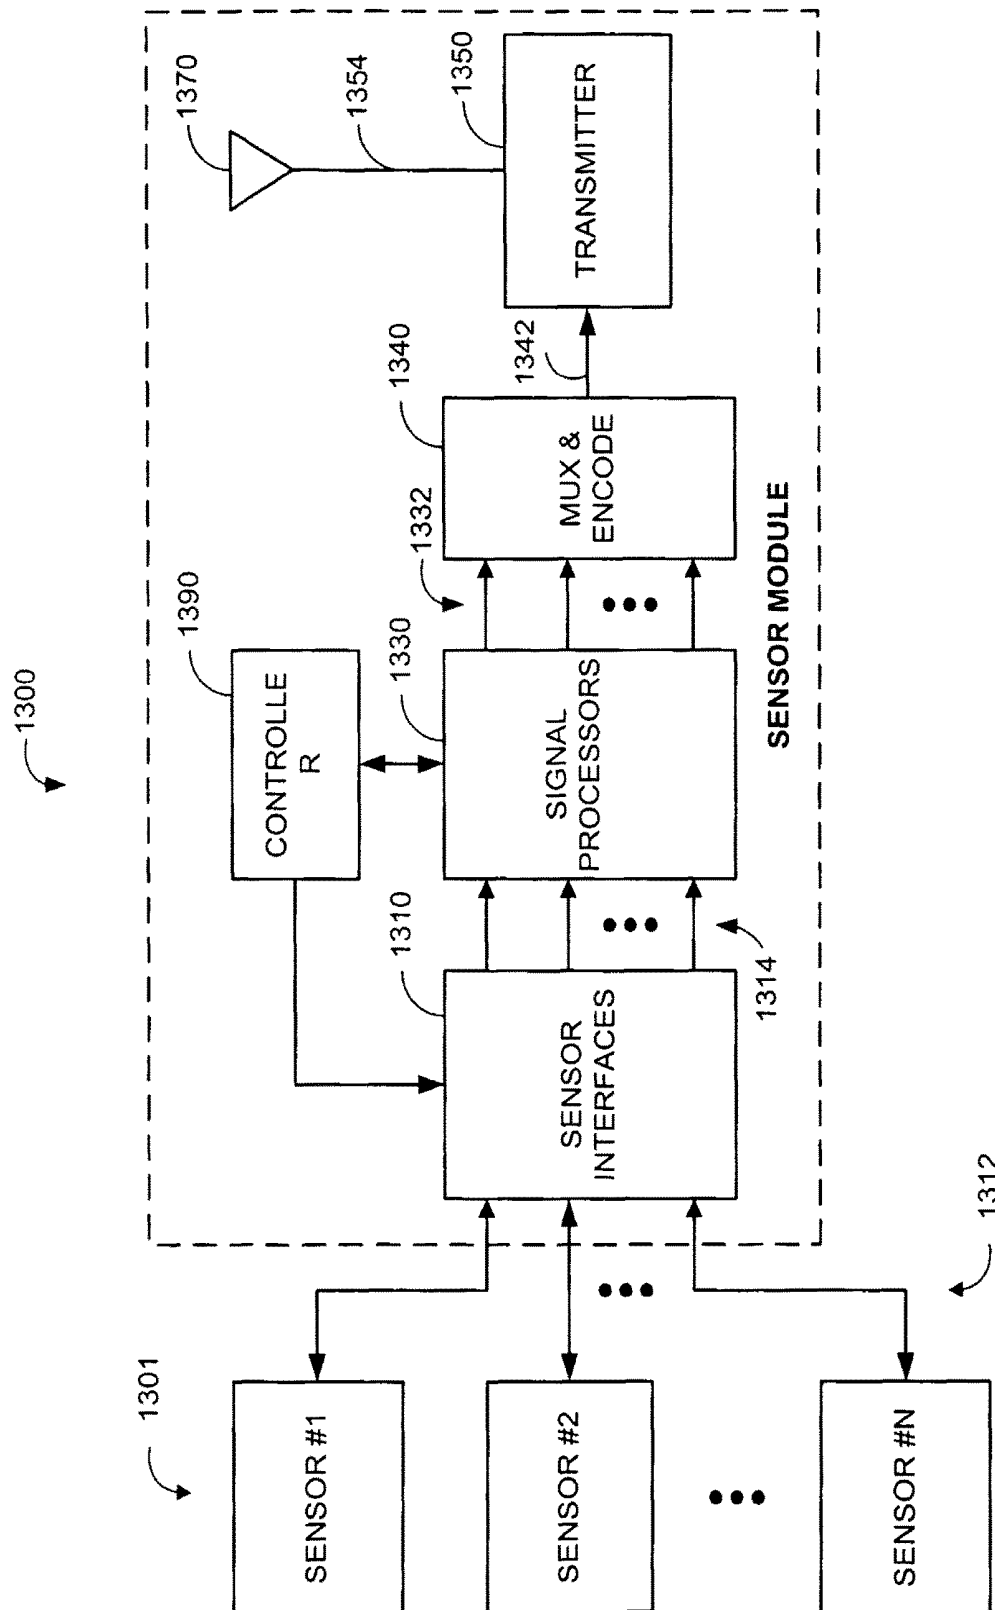


FIG. 13

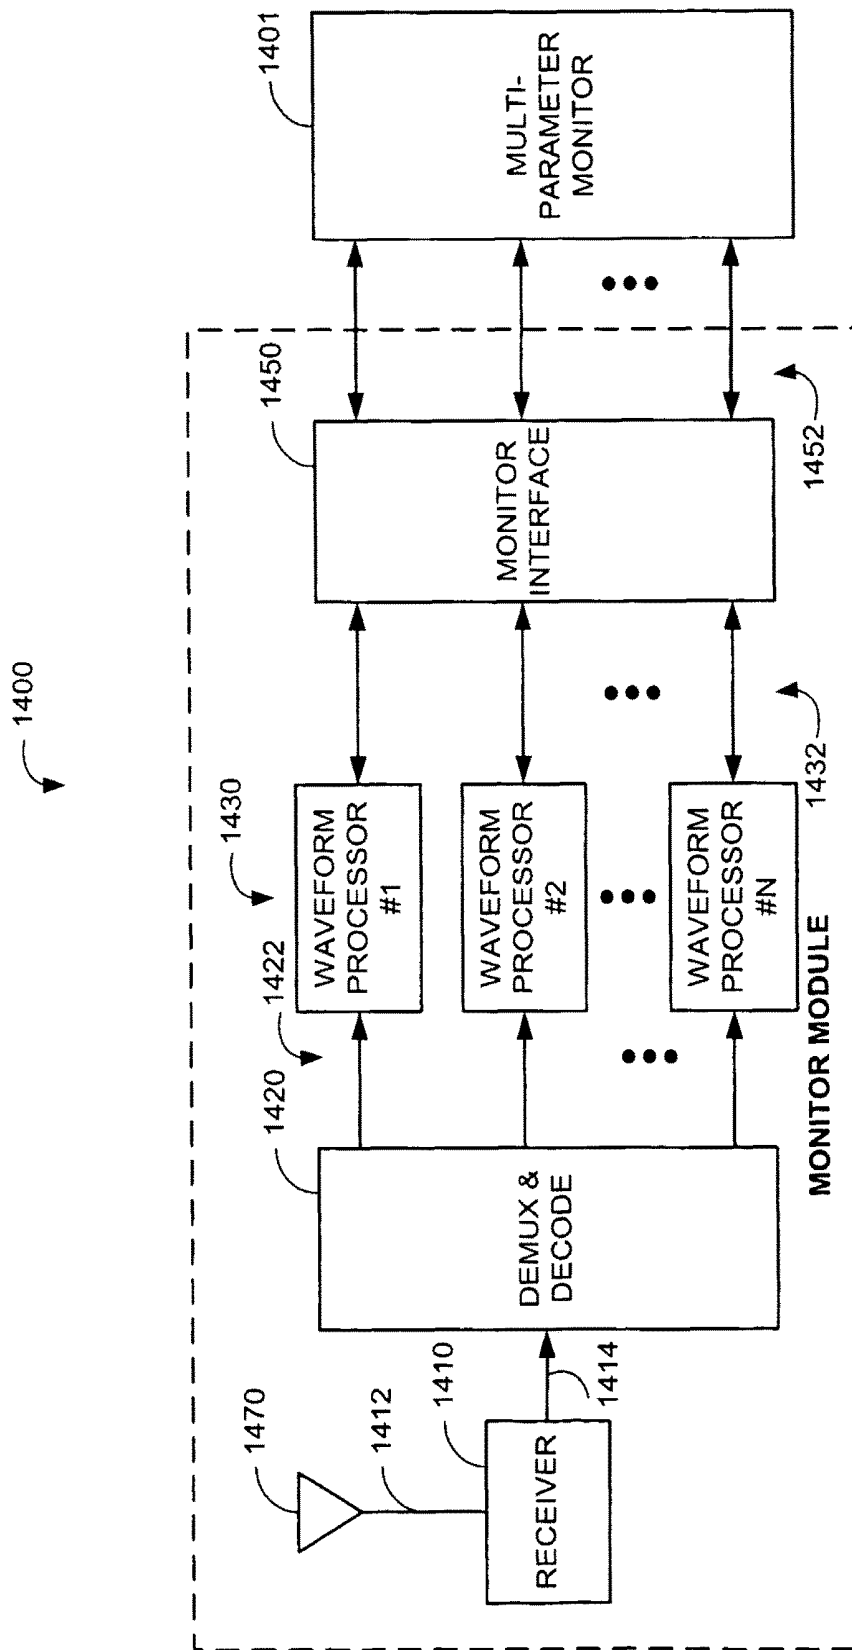


FIG. 14

# BODY WORN MOBILE MEDICAL PATIENT MONITOR

## REFERENCE TO RELATED APPLICATION

The present application is a continuation of U.S. patent application Ser. No. 15/448,989, filed on Mar. 3, 2017, entitled "Physiological Measurement Communications Adapter," which is a continuation of U.S. patent application Ser. No. 14/815,232, filed on Jul. 31, 2015, entitled "Physiological Measurement Communications Adapter," which is a continuation of U.S. patent application Ser. No. 14/217,788, filed on Mar. 18, 2014, entitled "Wrist-Mounted Physiological Measurement Device," now U.S. Pat. No. 9,113,832, which is a continuation of U.S. patent application Ser. No. 14/037,137, filed on Sep. 25, 2013, entitled "Physiological Measurement Communications Adapter," now U.S. Pat. No. 9,113,831, which is a continuation of U.S. patent application Ser. No. 12/955,826, filed on Nov. 29, 2010, entitled "Physiological Measurement Communications Adapter," now U.S. Pat. No. 8,548,548, which is a continuation of U.S. patent application Ser. No. 11/417,006, filed on May 3, 2006, entitled "Physiological Measurement Communications Adapter," now U.S. Pat. No. 7,844,315, which claims priority benefit under 35 U.S.C. §120 to, and is a continuation of, U.S. patent application Ser. No. 11/048,330, filed Feb. 1, 2005, entitled "Physiological Measurement Communications Adapter," now U.S. Pat. No. 7,844,314, which is a continuation of U.S. patent application Ser. No. 10/377,933, entitled "Physiological Measurement Communications Adapter," now U.S. Pat. No. 6,850,788, which claims priority benefit under 35 U.S.C. §119(e) from U.S. Provisional Application No. 60/367,428, filed Mar. 25, 2002, entitled "Physiological Measurement Communications Adapter." The present application also incorporates the foregoing utility disclosures herein by reference.

## BACKGROUND OF THE INVENTION

Patient vital sign monitoring may include measurements of blood oxygen, blood pressure, respiratory gas, and EKG among other parameters. Each of these physiological parameters typically requires a sensor in contact with a patient and a cable connecting the sensor to a monitoring device. For example, FIGS. 1-2 illustrate a conventional pulse oximetry system 100 used for the measurement of blood oxygen. As shown in FIG. 1, a pulse oximetry system has a sensor 110, a patient cable 140 and a monitor 160. The sensor 110 is typically attached to a finger 10 as shown. The sensor 110 has a plug 118 that inserts into a patient cable socket 142. The monitor 160 has a socket 162 that accepts a patient cable plug 144. The patient cable 140 transmits an LED drive signal 252 (FIG. 2) from the monitor 160 to the sensor 110 and a resulting detector signal 254 (FIG. 2) from the sensor 110 to the monitor 160. The monitor 160 processes the detector signal 254 (FIG. 2) to provide, typically, a numerical readout of the patient's oxygen saturation, a numerical readout of pulse rate, and an audible indicator or "beep" that occurs in response to each arterial pulse.

As shown in FIG. 2, the sensor 110 has both red and infrared LED emitters 212 and a photodiode detector 214. The monitor 160 has a sensor interface 271, a signal processor 273, a controller 275, output drivers 276, a display and audible indicator 278, and a keypad 279. The monitor 160 determines oxygen saturation by computing the differential absorption by arterial blood of the two wavelengths emitted by the sensor emitters 212, as is well-known in the

art. The sensor interface 271 provides LED drive current 252 which alternately activates the red and IR LED emitters 212. The photodiode detector 214 generates a signal 254 corresponding to the red and infrared light energy attenuated from transmission through the patient finger 10 (FIG. 1). The sensor interface 271 also has input circuitry for amplification, filtering and digitization of the detector signal 254. The signal processor 273 calculates a ratio of detected red and infrared intensities, and an arterial oxygen saturation value is empirically determined based on that ratio. The controller 275 provides hardware and software interfaces for managing the display and audible indicator 278 and keypad 279. The display and audible indicator 278 shows the computed oxygen status, as described above, and provides the pulse beep as well as alarms indicating oxygen desaturation events. The keypad 279 provides a user interface for setting alarm thresholds, alarm enablement, and display options, to name a few.

## SUMMARY OF THE INVENTION

Conventional physiological measurement systems are limited by the patient cable connection between sensor and monitor. A patient must be located in the immediate vicinity of the monitor. Also, patient relocation requires either disconnection of monitoring equipment and a corresponding loss of measurements or an awkward simultaneous movement of patient equipment and cables. Various devices have been proposed or implemented to provide wireless communication links between sensors and monitors, freeing patients from the patient cable tether. These devices, however, are incapable of working with the large installed base of existing monitors and sensors, requiring caregivers and medical institutions to suffer expensive wireless upgrades. It is desirable, therefore, to provide a communications adapter that is plug-compatible both with existing sensors and monitors and that implements a wireless link replacement for the patient cable.

An aspect of a physiological measurement communications adapter comprises a sensor interface configured to receive a sensor signal. A transmitter modulates a first baseband signal responsive to the sensor signal so as to generate a transmit signal. A receiver demodulates a receive signal corresponding to the transmit signal so as to generate a second baseband signal corresponding to the first baseband signal. Further, a monitor interface is configured to communicate a waveform responsive to the second baseband signal to a sensor port of a monitor. The waveform is adapted to the monitor so that measurements derived by the monitor from the waveform are generally equivalent to measurements derivable from the sensor signal. The communications adapter may further comprise a signal processor having an input in communications with the sensor interface, where the signal processor is operable to derive a parameter responsive to the sensor signal and where the first baseband signal is responsive to the parameter. The parameter may correspond to at least one of a measured oxygen saturation and a pulse rate.

One embodiment may further comprise a waveform generator that synthesizes the waveform from a predetermined shape. The waveform generator synthesizes the waveform at a frequency adjusted to be generally equivalent to the pulse rate. The waveform may have a first amplitude and a second amplitude, and the waveform generator may be configured to adjusted the amplitudes so that measurements derived by the monitor are generally equivalent to a measured oxygen saturation.

In another embodiment, the sensor interface is operable on the sensor signal to provide a plethysmograph signal output, where the first baseband signal is responsive to the plethysmograph signal. This embodiment may further comprise a waveform modulator that modifies a decoded signal responsive to the second baseband signal to provide the waveform. The waveform modulator may comprise a demodulator that separates a first signal and a second signal from the decoded signal, an amplifier that adjusts amplitudes of the first and second signals to generate a first adjusted signal and a second adjusted signal, and a modulator that combines the first and second adjusted signals into the waveform. The amplitudes of the first and second signals may be responsive to predetermined calibration data for the sensor and the monitor.

An aspect of a physiological measurement communications adapter method comprises the steps of inputting a sensor signal at a patient location, communicating patient data derived from the sensor signal between the patient location and a monitor location, constructing a waveform at the monitor location responsive to the sensor signal, and providing the waveform to a monitor via a sensor port. The waveform is constructed so that the monitor calculates a parameter generally equivalent to a measurement derivable from the sensor signal.

In one embodiment, the communicating step may comprise the substeps of deriving a conditioned signal from the sensor signal, calculating a parameter signal from the conditioned signal, and transmitting the parameter signal from the patient location to the monitor location. The constructing step may comprise the substep of synthesizing the waveform from the parameter signal. In an alternative embodiment, the communicating step may comprise the substeps of deriving a conditioned signal from said sensor signal and transmitting the conditioned signal from the patient location to the monitor location. The constructing step may comprise the substeps of demodulating the conditioned signal and re-modulating the conditioned signal to generate the waveform. The providing step may comprise the substeps of inputting a monitor signal from an LED drive output of the sensor port, modulating the waveform in response to the monitor signal, and outputting the waveform on a detector input of the sensor port.

Another aspect of a physiological measurement communications adapter comprises a sensor interface means for inputting a sensor signal and outputting a conditioned signal, a transmitter means for sending data responsive to the sensor signal, and a receiver means for receiving the data. The communications adapter further comprises a waveform processor means for constructing a waveform from the data so that measurements derived by a monitor from the waveform are generally equivalent to measurements derivable from the sensor signal, and a monitor interface means for communicating the waveform to a sensor port of the monitor. The communications adapter may further comprise a signal processor means for deriving a parameter signal from the conditioned signal, where the data comprises the parameter signal. The waveform processor means may comprise a means for synthesizing the waveform from the parameter signal. The data may comprise the conditioned signal, and the waveform processor means may comprise a means for modulating the conditioned signal in response to the monitor.

#### BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is an illustration of a prior art pulse oximetry system;

FIG. 2 is a functional block diagram of a prior art pulse oximetry system;

FIG. 3 is an illustration of a physiological measurement communications adapter;

FIGS. 4A-B are illustrations of communications adapter sensor modules;

FIGS. 5A-C are illustrations of communications adapter monitor modules;

FIG. 6 is a functional block diagram of a communications adapter sensor module;

FIG. 7 is a functional block diagram of a communications adapter monitor module;

FIG. 8 is a functional block diagram of a sensor module configured to transmit measured pulse oximeter parameters;

FIG. 9 is a functional block diagram of a monitor module configured to receive measured pulse oximeter parameters;

FIG. 10 is a functional block diagram of a sensor module configured to transmit a plethysmograph;

FIG. 11 is a functional block diagram of a monitor module configured to receive a plethysmograph;

FIG. 12 is a functional block diagram of a waveform modulator;

FIG. 13 is a functional block diagram of a sensor module configured for multiple sensors; and

FIG. 14 is a functional block diagram of a monitor module configured for multiple sensors.

#### DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

##### Overview

FIG. 3 illustrates one embodiment of a communications adapter. FIGS. 4-5 illustrate physical configurations for a communications adapter. In particular, FIGS. 4A-B illustrate sensor module configurations and FIGS. 5A-C illustrate monitor module configurations. FIGS. 6-14 illustrate communications adapter functions. In particular, FIGS. 6-7 illustrate general functions for a sensor module and a monitor module, respectively. FIGS. 8-9 functionally illustrate a communications adapter where derived pulse oximetry parameters, such as saturation and pulse rate are transmitted between a sensor module and a monitor module. Also, FIGS. 10-12 functionally illustrate a communications adapter where a plethysmograph is transmitted between a sensor module and a monitor module. FIGS. 13-14 functionally illustrate a multiple-parameter communications adapter.

FIG. 3 illustrates a communications adapter 300 having a sensor module 400 and a monitor module 500. The communications adapter 300 communicates patient data derived from a sensor 310 between the sensor module 400, which is located proximate a patient 20 and the monitor module 500, which is located proximate a monitor 360. A wireless link 340 is provided between the sensor module 400 and the monitor module 500, replacing the conventional patient cable, such as a pulse oximetry patient cable 140 (FIG. 1). Advantageously, the sensor module 400 is plug-compatible with a conventional sensor 310. In particular, the sensor connector 318 connects to the sensor module 400 in a similar manner as to a patient cable. Further, the sensor module 400 outputs a drive signal to the sensor 310 and inputs a sensor signal from the sensor 310 in an equivalent manner as a conventional monitor 360. The sensor module 400 may be battery powered or externally powered. External power may be for recharging internal batteries or for powering the sensor module during operation or both.

As shown in FIG. 3, the monitor module 500 is advantageously plug-compatible with a conventional monitor 360. In particular, the monitor's sensor port 362 connects to the monitor module 500 in a similar manner as to a patient cable, such as a pulse oximetry patient cable 140 (FIG. 1). Further, the monitor module 500 inputs a drive signal from the monitor 360 and outputs a corresponding sensor signal to the monitor 360 in an equivalent manner as a conventional sensor 310. As such, the combination sensor module 400 and monitor module 500 provide a plug-compatible wireless replacement for a patient cable, adapting an existing wired physiological measurement system into a wireless physiological measurement system. The monitor module 500 may be battery powered, powered from the monitor, such as by tapping current from a monitor's LED drive, or externally powered from an independent AC or DC power source.

Although a communications adapter 300 is described herein with respect to a pulse oximetry sensor and monitor, one of ordinary skill in the art will recognize that a communications adapter may provide a plug-compatible wireless replace for a patient cable that connects any physiological sensor and corresponding monitor. For example, a communications adapter 300 may be applied to a biopotential sensor, a non-invasive blood pressure (NIBP) sensor, a respiratory rate sensor, a glucose sensor and the corresponding monitors, to name a few.

#### Sensor Module Physical Configurations

FIGS. 4A-B illustrate physical embodiments of a sensor module 400. FIG. 4A illustrates a wrist-mounted module 410 having a wrist strap 411, a case 412 and an auxiliary cable 420. The case 412 contains the sensor module electronics, which are functionally described with respect to FIG. 6, below. The case 412 is mounted to the wrist strap 411, which attaches the wrist-mounted module 410 to a patient 20. The auxiliary cable 420 mates to a sensor connector 318 and a module connector 414, providing a wired link between a conventional sensor 310 and the wrist-mounted module 410. Alternatively, the auxiliary cable 420 is directly wired to the sensor module 400. The wrist-mounted module 410 may have a display 415 that shows sensor measurements, module status and other visual indicators, such as monitor status. The wrist-mounted module 410 may also have keys (not shown) or other input mechanisms to control its operational mode and characteristics. In an alternative embodiment, the sensor 310 may have a tail (not shown) that connects directly to the wrist-mounted module 410, eliminating the auxiliary cable 420.

FIG. 4B illustrates a clip-on module 460 having a clip 461, a case 462 and an auxiliary cable 470. The clip 461 attaches the clip-on module 460 to patient clothing or objects near a patient 20, such as a bed frame. The auxiliary cable 470 mates to the sensor connector 318 and functions as for the auxiliary cable 420 (FIG. 4A) of the wrist-mounted module 410 (FIG. 4A), described above. The clip-on module 460 may have a display 463 and keys 464 as for the wrist-mounted module 410 (FIG. 4A). Either the wrist-mounted module 410 or the clip-on module 460 may have other input or output ports (not shown) that download software, configure the module, or provide a wired connection to other measurement instruments or computing devices, to name a few examples.

#### Monitor Module Physical Configurations

FIGS. 5A-C illustrate physical embodiments of a monitor module 500. FIG. 5A illustrates a direct-connect module 510 having a case 512 and an integrated monitor connector 514. The case 512 contains the monitor module electronics, which are functionally described with respect to FIG. 7,

below. The monitor connector 514 mimics that of the monitor end of a patient cable, such as a pulse oximetry patient cable 140 (FIG. 1), and electrically and mechanically connects the monitor module 510 to the monitor 360 via the monitor's sensor port 362.

FIG. 5B illustrates a cable-connect module 540 having a case 542 and an auxiliary cable 550. The case 542 functions as for the direct-connect module 510 (FIG. 5A), described above. Instead of directly plugging into the monitor 360, the cable-connect module 540 utilizes the auxiliary cable 550, which mimics the monitor end of a patient cable, such as a pulse oximetry patient cable 140 (FIG. 1), and electrically connects the cable-connect module 540 to the monitor sensor port 362.

FIG. 5C illustrates a plug-in module 570 having a plug-in case 572 and an auxiliary cable 580. The plug-in case 572 is mechanically compatible with the plug-in chassis of a multiparameter monitor 370 and may or may not electrically connect to the chassis backplane. The auxiliary cable 580 mimics a patient cable and electrically connects the plug-in module 570 to the sensor port 372 of another plug-in device. A direct-connect module 510 (FIG. 5A) or a cable-connect module 540 (FIG. 5B) may also be used with a multiparameter monitor 370.

In a multiparameter embodiment, such as described with respect to FIGS. 13-14, below, a monitor module 500 may connect to multiple plug-in devices of a multiparameter monitor 370. For example, a cable-connect module 540 (FIG. 5B) may have multiple auxiliary cables 550 (FIG. 5B) that connect to multiple plug-in devices installed within a multiparameter monitor chassis. Similarly, a plug-in module 570 may have one or more auxiliary cables 580 with multiple connectors for attaching to the sensor ports 372 of multiple plug-in devices.

#### Communications Adapter Functions

FIGS. 6-7 illustrate functional embodiments of a communications adapter. FIG. 6 illustrates a sensor module 400 having a sensor interface 610, a signal processor 630, an encoder 640, a transmitter 650 and a transmitting antenna 670. A physiological sensor 310 provides an input sensor signal 612 at the sensor connector 318. Depending on the sensor 310, the sensor module 400 may provide one or more drive signals 618 to the sensor 310. The sensor interface 610 inputs the sensor signal 612 and outputs a conditioned signal 614. The conditioned signal 614 may be coupled to the transmitter 650 or further processed by a signal processor 630. If the sensor module configuration utilizes a signal processor 630, it derives a parameter signal 632 responsive to the sensor signal 612, which is then coupled to the transmitter 650. Regardless, the transmitter 650 inputs a baseband signal 642 that is responsive to the sensor signal 612. The transmitter 650 modulates the baseband signal 642 with a carrier to generate a transmit signal 654. The transmit signal 654 may be derived by various amplitude, frequency or phase modulation schemes, as is well known in the art. The transmit signal 654 is coupled to the transmit antenna 670, which provides wireless communications to a corresponding receive antenna 770 (FIG. 7), as described below.

As shown in FIG. 6, the sensor interface 610 conditions and digitizes the sensor signal 612 to generate the conditioned signal 614. Sensor signal conditioning may be performed in the analog domain or digital domain or both and may include amplification and filtering in the analog domain and filtering, buffering and data rate modification in the digital domain, to name a few. The resulting conditioned signal 614 is responsive to the sensor signal 612 and may be used to calculate or derive a parameter signal 632.

Further shown in FIG. 6, the signal processor 630 performs signal processing on the conditioned signal 614 to generate the parameter signal 632. The signal processing may include buffering, digital filtering, smoothing, averaging, adaptive filtering and frequency transforms to name a few. The resulting parameter signal 632 may be a measurement calculated or derived from the conditioned signal, such as oxygen saturation, pulse rate, blood glucose, blood pressure and EKG to name a few. Also, the parameter signal 632 may be an intermediate result from which the above-stated measurements may be calculated or derived.

As described above, the sensor interface 610 performs mixed analog and digital pre-processing of an analog sensor signal and provides a digital output signal to the signal processor 630. The signal processor 630 then performs digital post-processing of the front-end processor output. In alternative embodiments, the input sensor signal 612 and the output conditioned signal 614 may be either analog or digital, the front-end processing may be purely analog or purely digital, and the back-end processing may be purely analog or mixed analog or digital.

In addition, FIG. 6 shows an encoder 640, which translates a digital word or serial bit stream, for example, into the baseband signal 642, as is well-known in the art. The baseband signal 642 comprises the symbol stream that drives the transmit signal 654 modulation, and may be a single signal or multiple related signal components, such as in-phase and quadrature signals. The encoder 640 may include data compression and redundancy, also well-known in the art.

FIG. 7 illustrates a monitor module 500 having a receive antenna 770, a receiver 710, a decoder 720, a waveform processor 730 and a monitor interface 750. A receive signal 712 is coupled from the receive antenna 770, which provides wireless communications to a corresponding transmit antenna 670 (FIG. 6), as described above. The receiver 710 inputs the receive signal 712, which corresponds to the transmit signal 654 (FIG. 6). The receiver 710 demodulates the receive signal to generate a baseband signal 714. The decoder 720 translates the symbols of the demodulated baseband signal 714 into a decoded signal 724, such as a digital word stream or bit stream. The waveform processor 730 inputs the decoded signal 724 and generates a constructed signal 732. The monitor interface 750 is configured to communicate the constructed signal 732 to a sensor port 362 of a monitor 360. The monitor 360 may output a sensor drive signal 754, which the monitor interface 750 inputs to the waveform processor 730 as a monitor drive signal 734. The waveform processor 730 may utilize the monitor drive signal 734 to generate the constructed signal 732. The monitor interface 750 may also provide characterization information 758 to the waveform processor 730, relating to the monitor 360, the sensor 310 or both, that the waveform processor 730 utilizes to generate the constructed signal 732.

The constructed signal 732 is adapted to the monitor 360 so that measurements derived by the monitor 360 from the constructed signal 732 are generally equivalent to measurements derivable from the sensor signal 612 (FIG. 6). Note that the sensor 310 (FIG. 6) may or may not be directly compatible with the monitor 360. If the sensor 310 (FIG. 6) is compatible with the monitor 360, the constructed signal 732 is generated so that measurements derived by the monitor 360 from the constructed signal 732 are generally equivalent (within clinical significance) with those derivable directly from the sensor signal 612 (FIG. 6). If the sensor 310 (FIG. 6) is not compatible with the monitor 360, the constructed signal 732 is generated so that measurements

derived by the monitor 360 from the constructed signal 732 are generally equivalent to those derivable directly from the sensor signal 612 (FIG. 6) using a compatible monitor.

#### Wireless Pulse Oximetry

FIGS. 8-11 illustrate pulse oximeter embodiments of a communications adapter. FIGS. 8-9 illustrate a sensor module and a monitor module, respectively, configured to communicate measured pulse oximeter parameters. FIG. 10-11 illustrate a sensor module and a monitor module, respectively, configured to communicate a plethysmograph signal. Parameter Transmission

FIG. 8 illustrates a pulse oximetry sensor module 800 having a sensor interface 810, signal processor 830, encoder 840, transmitter 850, transmitting antenna 870 and controller 890. The sensor interface 810, signal processor 830 and controller 890 function as described with respect to FIG. 2, above. The sensor interface 810 communicates with a standard pulse oximetry sensor 310, providing an LED drive signal 818 to the LED emitters 312 and receiving a sensor signal 812 from the detector 314 in response. The sensor interface 810 provides front-end processing of the sensor signal 812, also described above, providing a plethysmograph signal 814 to the signal processor 830. The signal processor 830 then derives a parameter signal 832 that comprises a real time measurement of oxygen saturation and pulse rate. The parameter signal 832 may include other parameters, such as measurements of perfusion index and signal quality. In one embodiment, the signal processor is an MS-5 or MS-7 board available from Masimo Corporation, Irvine, Calif.

As shown in FIG. 8, the encoder 840, the transmitter 850 and the transmitting antenna 870 function as described with respect to FIG. 6, above. For example, the parameter signal 832 may be a digital word stream that is serialized into a bit stream and encoded into a baseband signal 842. The baseband signal 842 may be, for example, two bit symbols that drive a quadrature phase shift keyed (QPSK) modulator in the transmitter 850. Other encodings and modulations are also applicable, as described above. The transmitter 850 inputs the baseband signal 842 and generates a transmit signal 854 that is a modulated carrier having a frequency suitable for short-range transmission, such as within a hospital room, doctor's office, emergency vehicle or critical care ward, to name a few. The transmit signal 854 is coupled to the transmit antenna 870, which provides wireless communications to a corresponding receive antenna 970 (FIG. 9), as described below.

FIG. 9 illustrates a monitor module 900 having a receive antenna 970, a receiver 910, a decoder 920, a waveform generator 930 and an interface cable 950. The receive antenna 970, receiver 910 and decoder 920 function as described with respect to FIG. 7, above. In particular, the receive signal 912 is coupled from the receive antenna 970, which provides wireless communications to a corresponding transmit antenna 870 (FIG. 8). The receiver 910 inputs the receive signal 912, which corresponds to the transmit signal 854 (FIG. 8). The receiver 910 demodulates the receive signal 912 to generate a baseband signal 914. Not accounting for transmission errors, the baseband signal 914 corresponds to the sensor module baseband signal 842 (FIG. 8), for example a symbol stream of two bits each. The decoder 920 assembles the baseband signal 914 into a parameter signal 924, which, for example, may be a sequence of digital words corresponding to oxygen saturation and pulse rate.

Again, not accounting for transmission errors, the monitor module parameter signal 924 corresponds to the sensor module parameter signal 832 (FIG. 8), derived by the signal processor 830 (FIG. 8).

Also shown in FIG. 9, the waveform generator 930 is a particular embodiment of the waveform processor 730 (FIG. 7) described above. The waveform generator 930 generates a synthesized waveform 932 that the pulse oximeter monitor 360 can process to calculate SpO<sub>2</sub> and pulse rate values or exception messages. In the present embodiment, the waveform generator output does not reflect a physiological waveform. In particular, the synthesized waveform is not physiological data from the sensor module 800, but is a waveform synthesized from predetermined stored waveform data to cause the monitor 360 to calculate oxygen saturation and pulse rate equivalent to or generally equivalent (within clinical significance) to that calculated by the signal processor 830 (FIG. 8). The actual intensity signal from the patient received by the detector 314 (FIG. 8) is not provided to the monitor 360 in the present embodiment. Indeed, the waveform provided to the monitor 360 will usually not resemble a plethysmographic waveform or other physiological data from the patient to whom the sensor module 800 (FIG. 8) is attached.

The synthesized waveform 932 is modulated according to the drive signal input 934. That is, the pulse oximeter monitor 360 expects to receive a red and IR modulated intensity signal originating from a detector, as described with respect to FIGS. 1-2, above. The waveform generator 930 generates the synthesized waveform 932 with a predetermined shape, such as a triangular or sawtooth waveform stored in waveform generator memory or derived by a waveform generator algorithm. The waveform is modulated synchronously with the drive input 934 with first and second amplitudes that are processed in the monitor 360 as red and IR portions of a sensor signal. The frequency and the first and second amplitudes are adjusted so that pulse rate and oxygen saturation measurements derived by the pulse oximeter monitor 360 are generally equivalent to the parameter measurements derived by the signal processor 830 (FIG. 8), as described above. One embodiment of a waveform generator 930 is described in U.S. Patent Application No. 60/117,097 entitled "Universal/Upgrading Pulse Oximeter," assigned to Masimo Corporation, Irvine, Calif. and incorporated by reference herein. Although the waveform generator 930 is described above as synthesizing a waveform that does not resemble a physiological signal, one of ordinary skill will recognize that another embodiment of the waveform generator 930 could incorporate, for example, a plethysmograph simulator or other physiological signal simulator.

Further shown in FIG. 9, the interface cable 950 functions in a manner similar to the monitor interface 750 (FIG. 7) described above. The interface cable 950 is configured to communicate the synthesized waveform 932 to the monitor 360 sensor port and to communicate the sensor drive signal 934 to the waveform generator 930. The interface cable 950 may include a ROM 960 that contains monitor and sensor characterization data. The ROM 960 is read by the waveform generator 930 so that the synthesized waveform 932 is adapted to a particular monitor 360. For example, the ROM 960 may contain calibration data of red/IR versus oxygen saturation, waveform amplitude and waveform shape information. An interface cable is described in U.S. Patent Application No. 60/117,092, referenced above. Monitor-specific SatShare™ brand interface cables are available from Masimo Corporation, Irvine, Calif. In an alternative

embodiment, such as a direct connect monitor module as illustrated in FIG. 5A, an interface cable 950 is not used and the ROM 960 may be incorporated within the monitor module 900 itself.

#### 5 Plethysmograph Transmission

FIG. 10 illustrates another pulse oximetry sensor module 1000 having a sensor interface 1010, encoder 1040, transmitter 1050, transmitting antenna 1070 and controller 1090, which have the corresponding functions as those described with respect to FIG. 8, above. The encoder 1040, however, inputs a plethysmograph signal 1014 rather than oxygen saturation and pulse rate measurements 832 (FIG. 8). Thus, the sensor module 1000 according to this embodiment encodes and transmits a plethysmograph signal 1014 to a corresponding monitor module 1100 (FIG. 11) in contrast to derived physiological parameters, such as oxygen saturation and pulse rate. The plethysmograph signal 1014 is illustrated in FIG. 10 as being a direct output from the sensor interface 1010. In another embodiment, the sensor module 1000 incorporates a decimation processor, not shown, after the sensor interface 1010 so as to provide a plethysmograph signal 1014 having a reduced sample rate.

FIG. 11 illustrates another pulse oximetry monitor module 1100 having a receive antenna 1170, a receiver 1110, a decoder 1120 and an interface cable 1150, which have the corresponding functions as those described with respect to FIG. 9, above. This monitor module embodiment 1100, however, has a waveform modulator 1200 rather than a waveform generator 930 (FIG. 9), as described above. The waveform modulator 1200 inputs a plethysmograph signal from the decoder 1120 rather than oxygen saturation and pulse rate measurements, as described with respect to FIG. 9, above. Further, the waveform modulator 1200 provides an modulated waveform 1132 to the pulse oximeter monitor 360 rather than a synthesized waveform, as described with respect to FIG. 9. The modulated waveform 1132 is a plethysmographic waveform modulated according to the monitor drive signal input 1134. That is, the waveform modulator 1200 does not synthesize a waveform, but rather modifies the received plethysmograph signal 1124 to cause the monitor 360 to calculate oxygen saturation and pulse rate generally equivalent (within clinical significance) to that derivable by a compatible, calibrated pulse oximeter directly from the sensor signal 1012 (FIG. 10). The waveform modulator 1200 is described in further detail with respect to FIG. 12, below.

FIG. 12 shows a waveform modulator 1200 having a demodulator 1210, a red digital-to-analog converter (DAC) 1220, an IR DAC 1230, a red amplifier 1240, an IR amplifier 1250, a modulator 1260, a modulator control 1270, a look-up table (LUT) 1280 and a ratio calculator 1290. The waveform modulator 1200 demodulates red and IR plethysmographs ("pleths") from the decoder output 1124 into a separate red pleth 1222 and IR pleth 1232. The waveform modulator 1200 also adjusts the amplitudes of the pleths 1222, 1232 according to stored calibration curves for the sensor 310 (FIG. 10) and the monitor 360 (FIG. 11). Further, the waveform modulator 1200 re-modulates the adjusted red pleth 1242 and adjusted IR pleth 1252, generating a modulated waveform 1132 to the monitor 360 (FIG. 11).

As shown in FIG. 12, the demodulator 1210 performs the demodulation function described above, generating digital red and IR pleth signals 1212, 1214. The DACs 1220, 1230 convert the digital pleth signals 1212, 1214 to corresponding analog pleth signals 1222, 1232. The amplifiers 1240, 1250 have variable gain control inputs 1262, 1264 and perform the amplitude adjustment function described above, gener-

11

ating adjusted red and IR pleth signals **1242**, **1252**. The modulator **1260** performs the re-modulation function described above, combining the adjusted red and IR pleth signals **1242**, **1252** according to a control signal **1272**. The modulator control **1270** generates the control signal **1272** synchronously with the LED drive signal(s) **1134** from the monitor **360**.

Also shown in FIG. **12**, the ratio calculator **1290** derives a red/IR ratio from the demodulator outputs **1212**, **1214**. The LUT **1280** stores empirical calibration data for the sensor **310** (FIG. **10**). The LUT **1280** also downloads monitor-specific calibration data from the ROM **1160** (FIG. **11**) via the ROM output **1158**. From this calibration data, the LUT **1280** determines a desired red/IR ratio for the modulated waveform **1132** and generates red and IR gain outputs **1262**, **1264** to the corresponding amplifiers **1240**, **1250**, accordingly. A desired red/IR ratio is one that allows the monitor **360** (FIG. **11**) to derive oxygen saturation measurements from the modulated waveform **1132** that are generally equivalent to that derivable directly from the sensor signal **1012** (FIG. **10**).

One of ordinary skill in the art will recognize that some of the signal processing functions described with respect to FIGS. **8-11** may be performed either within a sensor module or within a monitor module. Signal processing functions performed within a sensor module may advantageously reduce the transmission bandwidth to a monitor module at a cost of increased sensor module size and power consumption. Likewise, signal processing functions performed within a monitor module may reduce sensor module size and power consumption at a cost of increase transmission bandwidth.

For example, a monitor module embodiment **900** (FIG. **9**) described above receives measured pulse oximeter parameters, such as oxygen saturation and pulse rate, and generates a corresponding synthesized waveform. In that embodiment, the oxygen saturation and pulse rate computations are performed within a sensor module **800** (FIG. **8**). Another monitor module embodiment **1100** (FIG. **11**), also described above, receives a plethysmograph waveform and generates a remodulated waveform. In that embodiment, minimal signal processing is performed within a sensor module **1000** (FIG. **10**). In yet another embodiment, not shown, a sensor module transmits a plethysmograph waveform or a decimated plethysmograph waveform having a reduced sample rate. A corresponding monitor module has a signal processor, such as described with respect to FIG. **8**, in addition to a waveform generator, as described with respect to FIG. **9**. The signal processor computes pulse oximeter parameters and the waveform generator generates a corresponding synthesized waveform, as described above. In this embodiment, minimal signal processing is performed within the sensor module, and the monitor module functions are performed on the pulse oximeter parameters computed within the monitor module.

#### Wireless Multiple Parameter Measurements

FIGS. **13-14** illustrate a multiple parameter communications adapter. FIG. **13** illustrates a multiple parameter sensor module **1300** having sensor interfaces **1310**, one or more signal processors **1330**, a multiplexer and encoder **1340**, a transmitter **1350**, a transmitting antenna **1370** and a controller **1390**. One or more physiological sensors **1301** provide input sensor signals **1312** to the sensor module **1300**. Depending on the particular sensors **1301**, the sensor module **1300** may provide one or more drive signals **1312** to the sensors **1301** as determined by the controller **1390**. The sensor interfaces **1310** input the sensor signals **1312** and

12

output one or more conditioned signals **1314**. The conditioned signals **1314** may be coupled to the transmitter **1350** or further processed by the signal processors **1330**. If the sensor module configuration utilizes signal processors **1330**, it derives multiple parameter signals **1332** responsive to the sensor signals **1312**, which are then coupled to the transmitter **1350**. Regardless, the transmitter **1350** inputs a baseband signal **1342** that is responsive to the sensor signals **1312**. The transmitter **1350** modulates the baseband signal **1342** with a carrier to generate a transmit signal **1354**, which is coupled to the transmit antenna **1370** and communicated to a corresponding receive antenna **1470** (FIG. **14**), as described with respect to FIG. **6**, above. Alternatively, there may be multiple baseband signals **1342**, and the transmitter **1350** may transmit on multiple frequency channels, where each channel conveys data responsive to one or more of the sensor signals **1314**.

As shown in FIG. **13**, the sensor interface **1310** conditions and digitizes the sensor signals **1312** as described for a single sensor with respect to FIG. **6**, above. The resulting conditioned signals **1314** are responsive to the sensor signals **1312**. The signal processors **1330** perform signal processing on the conditioned signals **1314** to derive parameter signals **1332**, as described for a single conditioned signal with respect to FIG. **6**, above. The parameter signals **1332** may be physiological measurements such as oxygen saturation, pulse rate, blood glucose, blood pressure, EKG, respiration rate and body temperature to name a few, or may be intermediate results from which the above-stated measurements may be calculated or derived. The multiplexer and encoder **1340** combines multiple digital word or serial bit streams into a single digital word or bit stream. The multiplexer and encoder also encodes the digital word or bit stream to generate the baseband signal **1342**, as described with respect to FIG. **6**, above.

FIG. **14** illustrates a multiple parameter monitor module **1400** having a receive antenna **1470**, a receiver **1410**, a demultiplexer and decoder **1420**, one or more waveform processors **1430** and a monitor interface **1450**. The receiver **1410** inputs and demodulates the receive signal **1412** corresponding to the transmit signal **1354** (FIG. **13**) to generate a baseband signal **1414** as described with respect to FIG. **7**, above. The demultiplexer and decoder **1420** separates the symbol streams corresponding to the multiple conditioned signals **1314** (FIG. **13**) and/or parameter signals **1332** (FIG. **13**) and translates these symbol streams into multiple decoded signals **1422**, as described for a single symbol stream with respect to FIG. **7**, above. Alternatively, multiple frequency channels are received to generate multiple baseband signals, each of which are decoded to yield multiple decoded signals **1422**. The waveform processors **1430** input the decoded signals **1422** and generate multiple constructed signals **1432**, as described for a single decoded signal with respect to FIGS. **7-12**, above. The monitor interface **1450** is configured to communicate the constructed signals **1432** to the sensor ports of a multiple parameter monitor **1401** or multiple single parameter monitors, in a manner similar to that for a single constructed signal, as described with respect to FIGS. **7-12**, above. In particular, the constructed signals **1432** are adapted to the monitor **1401** so that measurements derived by the monitor **1401** from the constructed signals **1432** are generally equivalent to measurements derivable directly from the sensor signals **1312** (FIG. **13**).

A physiological measurement communications adapter is described above with respect to wireless communications and, in particular, radio frequency communications. A sensor module and monitor module, however, may also communi-

13

cate via wired communications, such as telephone, Internet or fiberoptic cable to name a few. Further, wireless communications can also utilize light frequencies, such as IR or laser to name a few.

A physiological measurement communications adapter has been disclosed in detail in connection with various embodiments. These embodiments are disclosed by way of examples only. One of ordinary skill in the art will appreciate many variations and modifications of a physiological measurement communications adapter within the scope of the claims that follow.

What is claimed is:

1. A body worn mobile medical monitoring device configured to minimize cable wiring from a sensor by placement of one or more sensor communication ports, the mobile medical monitoring device comprising:

a housing configured to be secured on a lower arm of a patient being monitored via a strap extending around the lower arm of the patient;

a display positioned on a face of the housing, opposite the strap, so as to be visible to a user;

a first sensor communication port positioned on a side of the housing and configured to face a hand of the lower arm of the patient when the mobile medical monitoring device is mounted to the lower arm of the patient, wherein:

the side of the housing faces the hand of the lower arm of the patient of the patient when the mobile medical monitoring device is mounted to the lower arm of the patient,

the first sensor communication port is configured to provide wired communication with a pulse oximetry sensor attached to a digit of the hand of the patient, the wired communication with the pulse oximetry sensor provided at least partly in the analog domain, and

the first sensor communication port is positioned on the side of the housing such that a path from the first sensor communication port on the side of the housing to the digit of the patient is substantially perpendicular to the side of the housing and shorter than any other path from any other side of the housing to the digit of the patient;

a plurality of additional sensor communications ports positioned on the housing and configured to provide wired communication with a plurality of additional physiological sensors at least partly in the digital domain; and

one or more processors and a transmitter configured to: display, on the display, physiological measurements derived from the pulse oximetry sensor and the plurality of additional physiological sensors; and wirelessly transmit information indicative of the physiological measurements to a remote computing device.

2. The mobile medical monitoring device of claim 1, wherein the wired communication with the pulse oximetry sensor is provided via a tail extending from the pulse oximetry sensor.

3. The mobile medical monitoring device of claim 2, wherein the tail comprises a cable that is configured to be removably attachable to the first sensor communication port.

4. The mobile medical monitoring device of claim 3, wherein a length of the cable corresponds to the path from the sensor communication port on the side of the housing to the digit of the patient.

14

5. The mobile medical monitoring device of claim 3, wherein the cable is appropriately sized based on the path from the sensor communication port on the side of the housing to the digit of the patient.

6. The mobile medical monitoring device of claim 3, wherein the path from the sensor communication port on the side of the housing to the digit of the patient runs at least partly along a backside of the hand of the patient.

7. The mobile medical monitoring device of claim 1, wherein the face of the housing comprises a single user interface.

8. The mobile medical monitoring device of claim 7, wherein the single user interface comprises the display.

9. The mobile medical monitoring device of claim 8, wherein:

the housing comprises a back side that is opposite the face of the housing,

the strap is mountable to the back side of the housing, and

the face of the housing is raised from the strap and the lower arm of the patient to enable positioning of the first sensor communication port on the side of the housing between the lower arm of the patient and the face of the housing.

10. The mobile medical monitoring device of claim 9, wherein:

the front side of the housing comprises a bezel and the display, and

a top of the first sensor communication port is located below the face of the housing.

11. The mobile medical monitoring device of claim 10, wherein the display is positioned centrally on the face of the housing.

12. The mobile medical monitoring device of claim 11, wherein the display positioned on the face of the housing is sized such that the display covers most of a length of a shortest dimension of the face of the housing.

13. A body worn, battery-powered medical monitoring device configured to provide on-patient and remote monitoring of patient physiological parameters, the medical monitoring device comprising:

a battery configured to provide power to the medical monitoring device such that the medical monitoring device may operate without a wired power connection;

a case configured to house the battery;

a strap configured to attach the case to an arm of a patient and be mountable to the case;

a first communications port positioned on a face of a side of the case configured to be nearest to a hand of the arm of the patient when the case is mounted to the arm of the patient, the first communications port configured to removably couple with a cable of a finger- or thumb-type pulse oximetry sensor and positioned on the face of the side of the case to provide a path from the first communications port to a digit of the hand of the patient that avoids tangling of the cable, the first communications port configured such that the cable perpendicularly extends from the face of the side of the case when the cable is coupled to the first communications port;

a second communications port configured to provide wired communications with a second physiological sensor arrangement at least partly via digital communications;

a third communications port configured to provide wired communications with a third physiological sensor arrangement;

## 15

a display configured to provide real time measurements of patient physiological parameters based at least in part on data obtained from at least the pulse oximetry sensor via the first communications port; and  
 a transmitter configured to wirelessly transmit information indicative of real time measurements of patient physiological parameters based at least in part on data obtained from the pulse oximetry sensor via the first communications port.

14. The medical monitoring device of claim 13, wherein the path from the first communications port to a digit of the hand is shorter than any path from any communications port located on any other side of the case to the digit of the hand.

15. The medical monitoring device of claim 13 further comprising:

one or more hardware processors configured to:

process the data obtained from the pulse oximetry sensor; and

determine, based at least in part on the data, the real time measurements of patient physiological parameters.

16. The medical monitoring device of claim 15, wherein: the one or more hardware processors are further configured to:

receive additional data from at least the second physiological sensor arrangement and the third physiological sensor arrangement;

determine, based at least in part on the additional data, real time measurements of additional patient physiological parameters; and

cause to be displayed, on the display, the real time measurements of additional patient physiological parameters; and

the transmitter is further configured to:

wirelessly transmit information indicative of real time measurements of additional patient physiological parameters based at least in part on the additional data.

17. The medical monitoring device of claim 16, wherein the display is positioned on a front, user-facing side of the case to enable a user to view the real time measurements of patient physiological parameters and the real time measurements of additional patient physiological parameters.

18. The medical monitoring device of claim 17, wherein the second physiological sensor arrangement comprises an EKG sensor arrangement and the third physiological sensor arrangement comprises a blood pressure sensor arrangement.

19. The medical monitoring device of claim 18, wherein: the first, second, and third communication ports are communicatively coupled to respective first, second, and third sensor interfaces; and

the first, second, and third sensor interfaces are uniquely configured to receive signals from the respective pulse oximetry sensor, EKG sensor arrangement, and blood pressure sensor arrangement.

20. A body worn portable patient monitoring device configured to provide on-patient and remote monitoring of patient physiological parameters, the portable patient monitoring device comprising:

a pulse oximetry sensor configured to be wrapped around a digit of a patient, the pulse oximetry sensor including at least:

a light emitter configured to emit light into a tissue site of the digit of the patient;

## 16

a light detector configured output a first signal responsive to at least a portion of the emitted light after attenuation by tissue of the tissue site; and

a cable extending from the pulse oximetry sensor and configured to electrically convey the first signal;

a blood pressure sensor configured to output a second signal responsive to at least a blood pressure parameter of the patient;

an additional sensor arrangement configured to output a third signal responsive to at least one additional physiological parameter of the patient other than blood pressure or oxygen saturation, the at least one additional physiological parameter including at least one of: temperature or respiration rate;

a housing configured to be secured to a lower arm of the patient, the housing having a size and shape configured to be secured to the lower arm of the patient;

a strap mountable to the back side of the housing, the strap configured to secure the housing to the lower arm of the patient;

a display positioned on a front side of the housing that is opposite a back side of the housing, the display configured to show a status of the portable patient monitoring device and one or more parameter measurements so as to be viewable by a user, wherein the display is positioned centrally on the front side of the display and is sized such that the display spans most of a length of a shortest dimension of the front side of the housing, and wherein the front side of the housing comprises a single user interface and a bezel;

one or more user input mechanisms configured to control an operational mode of the portable patient monitoring device in response to inputs from a user;

a first sensor port positioned on a face of a first side of the housing, wherein:

the face of the first side of the housing is configured to face toward a hand having the digit of the patient under measurement when the housing is secured to the lower arm of the patient,

the first sensor port is configured to removably physically couple with the pulse oximetry sensor via the cable and to electrically receive the first signal from the pulse oximetry sensor,

the cable is configured to run from the first sensor port, at least part way along a path substantially perpendicular to the face of the first side of the housing, down the arm of the patient, and to the digit of the patient to which the pulse oximetry sensor is configured to be wrapped around,

the front side of the housing is raised from the strap and the lower arm of the patient to enable positioning of the first sensor port on the first side of the housing between the lower arm of the patient and the front side of the housing, and

a top of the first sensor port is located below the front of the housing;

a second sensor port positioned on the housing and configured to provide wired electrical communication with the blood pressure sensor arrangement and to electrically receive second signal from the blood pressure sensor arrangement;

a third sensor port positioned on the housing and configured to provide electrical wired communication with the additional sensor arrangement and to electrically receive the third signal from the additional sensor arrangement;

17

a rechargeable battery positioned within the housing and configured to power the portable patient monitoring device such that the portable patient monitoring device is portable and wearable by the patient;

one or more signal processing arrangements positioned 5 within the housing and configured to:

receive the first signal from the pulse oximetry sensor via one or more sensor interfaces, wherein the first signal is provided at least partly as an analog signal;

process the first signal from the pulse oximetry sensor 10 to determine measurements of oxygen saturation and pulse rate;

receive the second signal from the blood pressure sensor arrangement via the one or more sensor interfaces, the second signal responsive to at least a 15 blood pressure parameter of the patient;

receive the third signal from the additional sensor arrangement via the one or more sensor interfaces, the third signal responsive to the at least one additional physiological parameter of the patient includ-

18

ing at least one of: temperature or respiration rate, wherein the third signal is provided at least partly as a digital signal; and

cause the measurements of oxygen saturation, pulse rate, blood pressure, and the at least one additional physiological parameter to all be displayed on the display of the portable patient monitoring device; and

a transmitter positioned within the housing and configured to:

wirelessly transmit a transmit signal including the information indicating the measurements of oxygen saturation, pulse rate, blood pressure, and the at least one additional physiological parameter to a separate computing device configured to display, on a remote display, the measurements of oxygen saturation, pulse rate, blood pressure, and the at least one additional physiological parameter.

\* \* \* \* \*

|                |                                                                                                                                                                                                                                                                                                                                                           |         |            |
|----------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|---------|------------|
| 专利名称(译)        | 身体佩带的流动医疗患者显示器                                                                                                                                                                                                                                                                                                                                            |         |            |
| 公开(公告)号        | <a href="#">US9788735</a>                                                                                                                                                                                                                                                                                                                                 | 公开(公告)日 | 2017-10-17 |
| 申请号            | US15/499619                                                                                                                                                                                                                                                                                                                                               | 申请日     | 2017-04-27 |
| [标]申请(专利权)人(译) | 梅西莫股份有限公司                                                                                                                                                                                                                                                                                                                                                 |         |            |
| 申请(专利权)人(译)    | Masimo公司                                                                                                                                                                                                                                                                                                                                                  |         |            |
| 当前申请(专利权)人(译)  | Masimo公司                                                                                                                                                                                                                                                                                                                                                  |         |            |
| [标]发明人         | AL ALI AMMAR                                                                                                                                                                                                                                                                                                                                              |         |            |
| 发明人            | AL-ALI, AMMAR                                                                                                                                                                                                                                                                                                                                             |         |            |
| IPC分类号         | A61B5/1455 A61B5/0205 A61B5/00 A61B5/021 A61B5/0404 A61B5/024                                                                                                                                                                                                                                                                                             |         |            |
| CPC分类号         | A61B5/0205 A61B5/0024 A61B5/021 A61B5/0404 A61B5/14552 A61B5/6824 A61B5/6826 A61B5/6831 A61B2562/222 A61B2562/227 A61B5/002 A61B5/02438 A61B5/1455 A61B5/6838 H04W4/70 Y10S128/903 A61B5/0004 A61B5/0015 A61B5/0026 A61B5/02427 A61B5/0402 A61B5/0428 A61B5/72 A61B5/7228 A61B5/7271 A61B5/742 A61B5/7425 A61B5/7445 A61B5/7475 A61B2560/0214 G08B21/0453 |         |            |
| 优先权            | 14/217788 2015-08-25 US<br>14/037137 2015-08-25 US<br>12/955826 2013-10-01 US<br>11/417006 2010-11-30 US<br>11/048330 2010-11-30 US<br>10/377933 2005-02-01 US<br>60/367428 2002-03-25 US                                                                                                                                                                 |         |            |
| 其他公开文献         | US20170224233A1                                                                                                                                                                                                                                                                                                                                           |         |            |
| 外部链接           | <a href="#">Espacenet</a> <a href="#">USPTO</a>                                                                                                                                                                                                                                                                                                           |         |            |

#### 摘要(译)

身体佩戴的移动医疗监测设备，其被配置为通过放置一个或多个传感器通信端口来最小化来自传感器的电缆布线。身体佩戴的移动医疗监测装置包括可固定在患者下臂上的壳体，显示器和位于壳体一侧的传感器通信端口，并配置成当移动时面向患者下臂的手医疗监测装置安装在患者的下臂上。传感器通信端口提供与脉搏血氧饱和度传感器的有线通信，脉搏血氧饱和度传感器连接到患者手的手指，并且位于壳体的侧面，使得从壳体侧面上的端口到数字的数字。患者比从房屋的任何其他侧面到数字的任何其他路径短。

