



US 20190231197A1

(19) **United States**

(12) **Patent Application Publication**

**Kirszenblat et al.**

(10) **Pub. No.: US 2019/0231197 A1**

(43) **Pub. Date: Aug. 1, 2019**

(54) **MEASURING RESPIRATION WITH AN IN-EAR ACCELEROMETER**

(71) Applicant: **Bose Corporation**, Framingham, MA (US)

(72) Inventors: **Romain Kirszenblat**, Allston, MA (US); **Mikhail Ioffe**, Newton, MA (US)

(73) Assignee: **Bose Corporation**, Framingham, MA (US)

(21) Appl. No.: **15/881,034**

(22) Filed: **Jan. 26, 2018**


**Publication Classification**

(51) **Int. Cl.**  
*A61B 5/0205* (2006.01)  
*A61B 5/00* (2006.01)  
*H04R 1/10* (2006.01)

(52) **U.S. Cl.**  
CPC ..... *A61B 5/0205* (2013.01); *A61B 5/7278* (2013.01); *A61B 5/7257* (2013.01); *A61B 5/02438* (2013.01); *H04R 1/1016* (2013.01); *H04R 1/1075* (2013.01); *H04R 1/1041* (2013.01); *A61B 5/6803* (2013.01)

(57) **ABSTRACT**

An earphone includes a loudspeaker, a microphone, a housing supporting the loudspeaker and microphone, and an ear tip surrounding the housing and configured to acoustically couple both the loudspeaker and the microphone to an ear canal of a user, and to acoustically close the entrance to the user's ear canal. A processor receives input audio signals from the microphone, detects peaks having a frequency of around 1 Hz in the input audio signals, based on the detected peaks, computes an instantaneous heart rate, measures a frequency of an oscillation within the instantaneous heart rate, and based on the frequency of the oscillation, computes a rate of respiration.

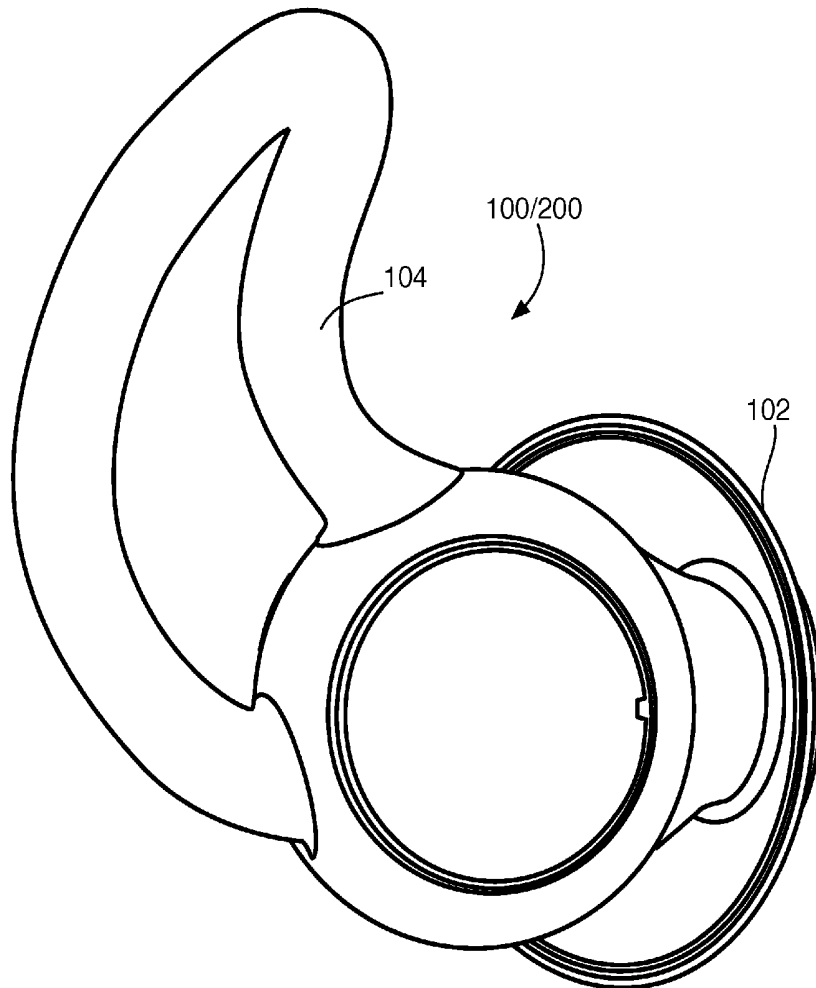

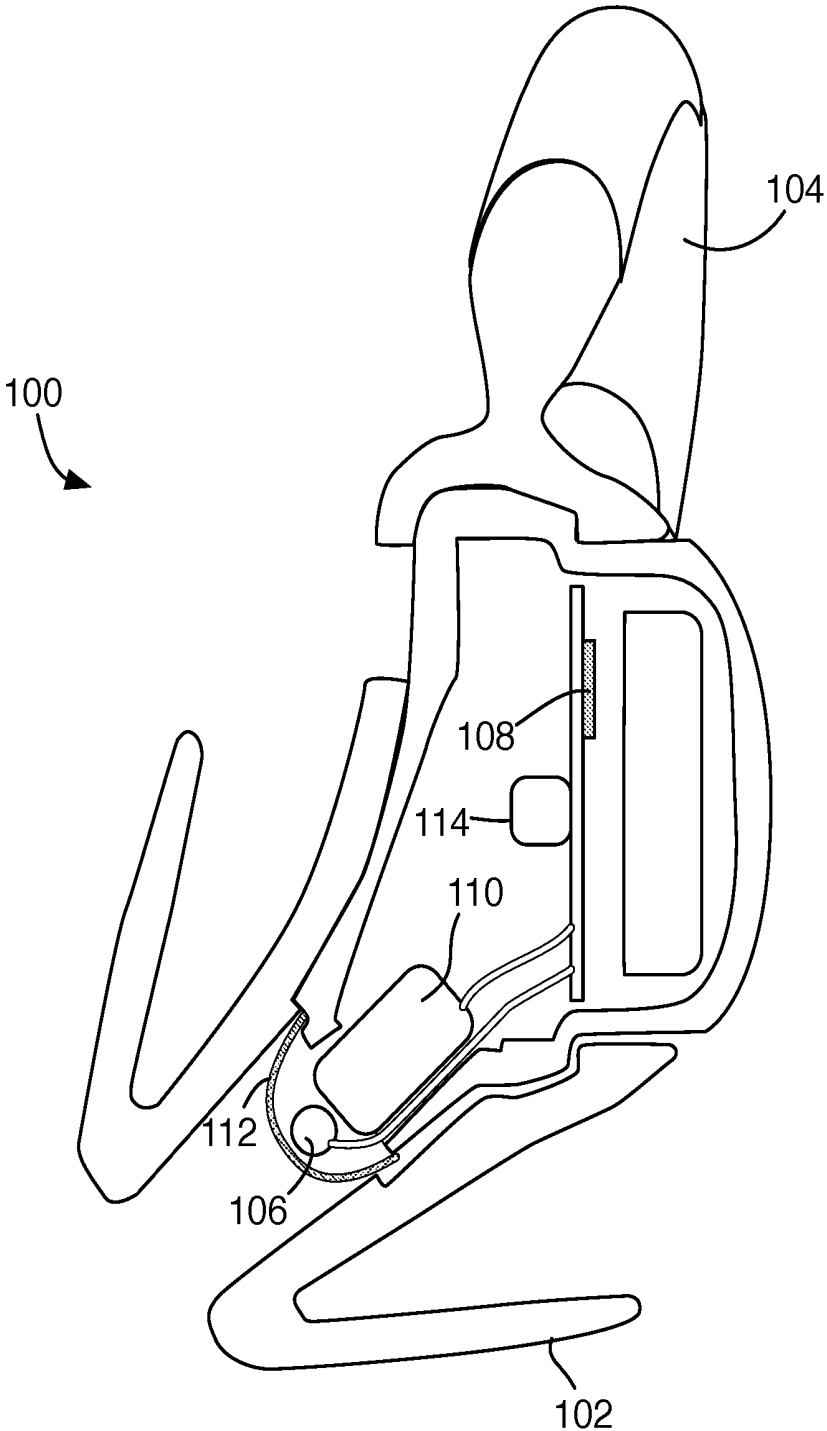


Fig. 1

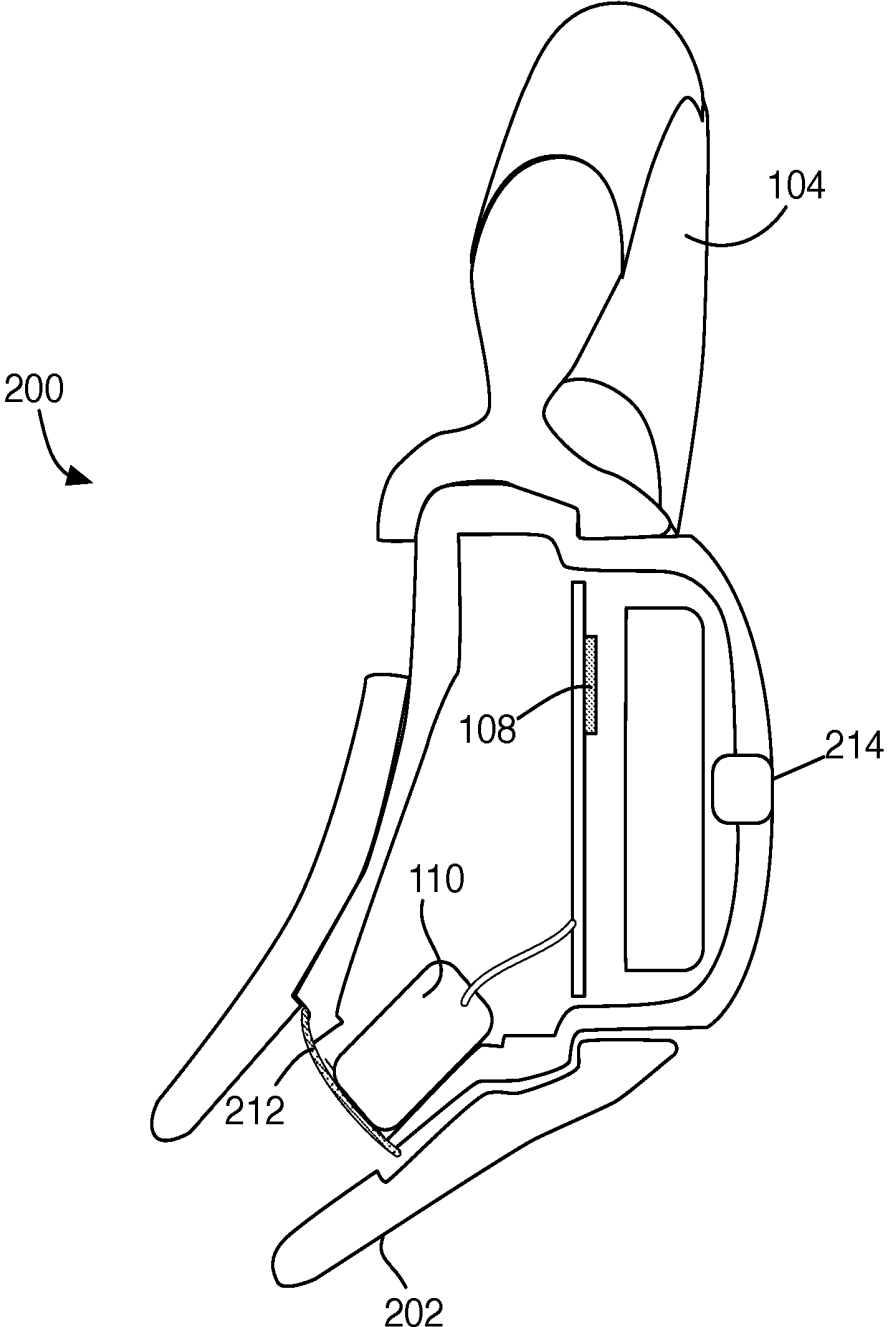


Fig. 2

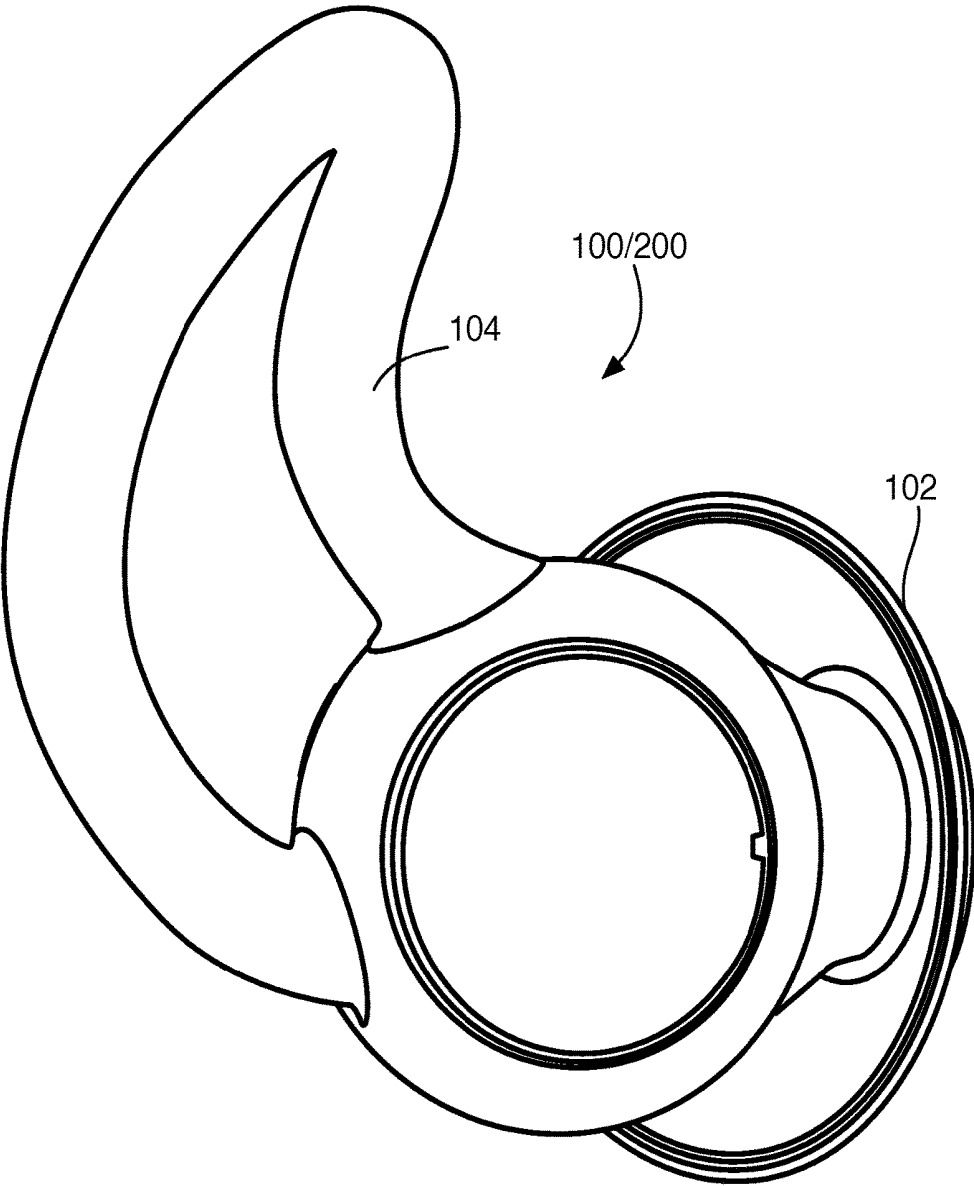


Fig. 3

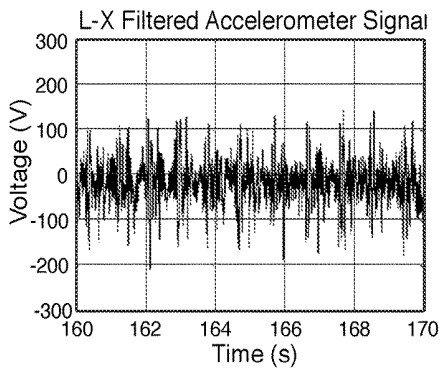


Fig. 4A

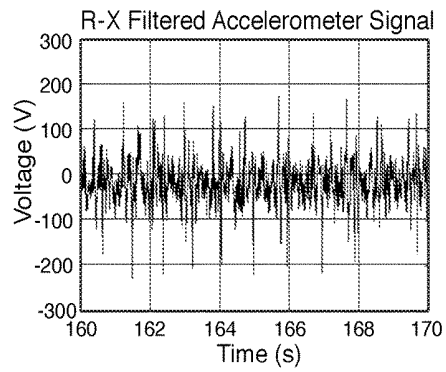


Fig. 4B

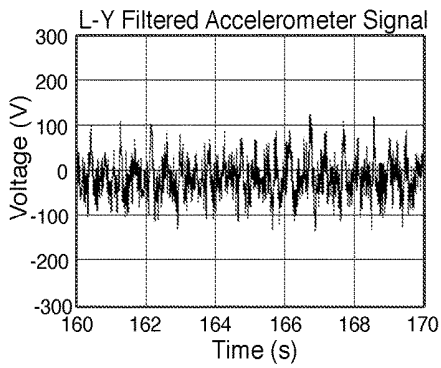


Fig. 4C

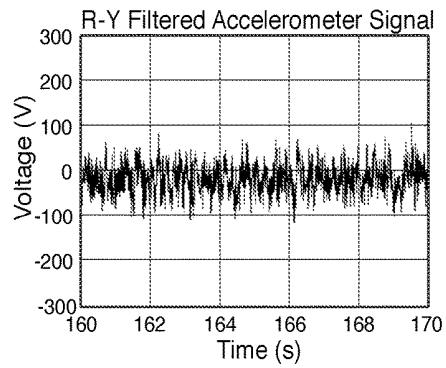


Fig. 4D

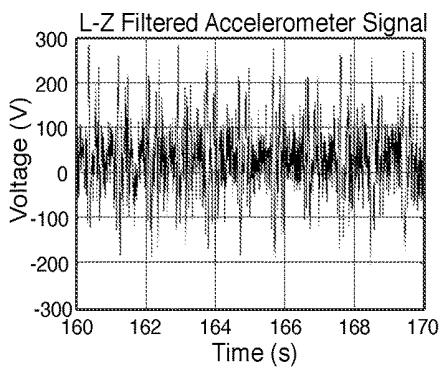


Fig. 4E

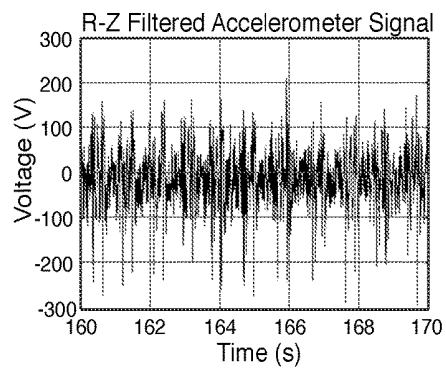


Fig. 4F

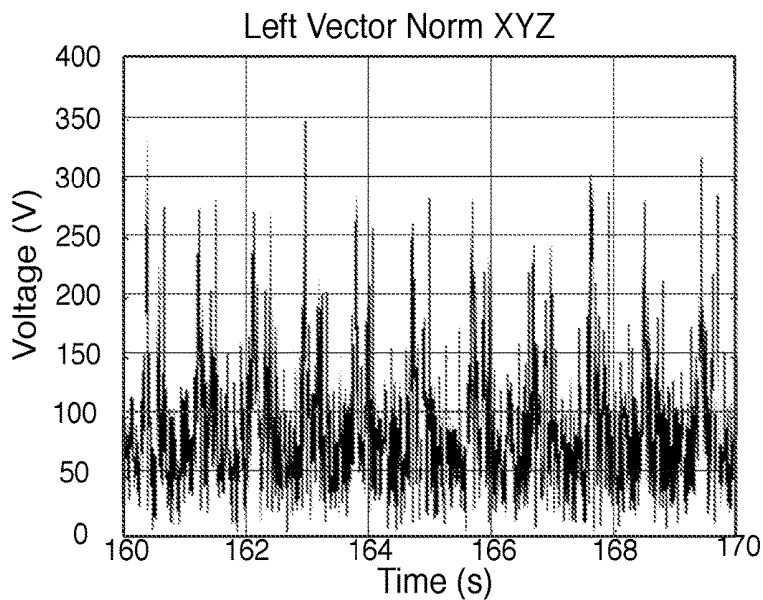


Fig. 5A

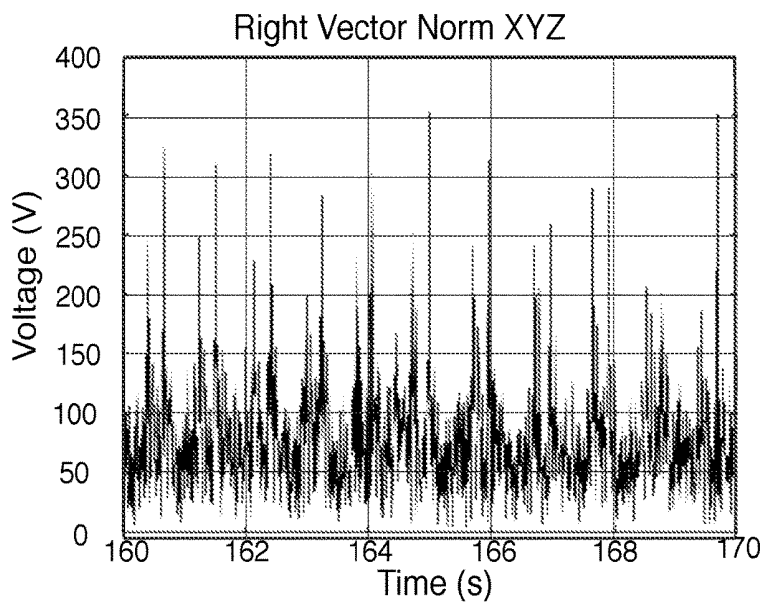


Fig. 5B

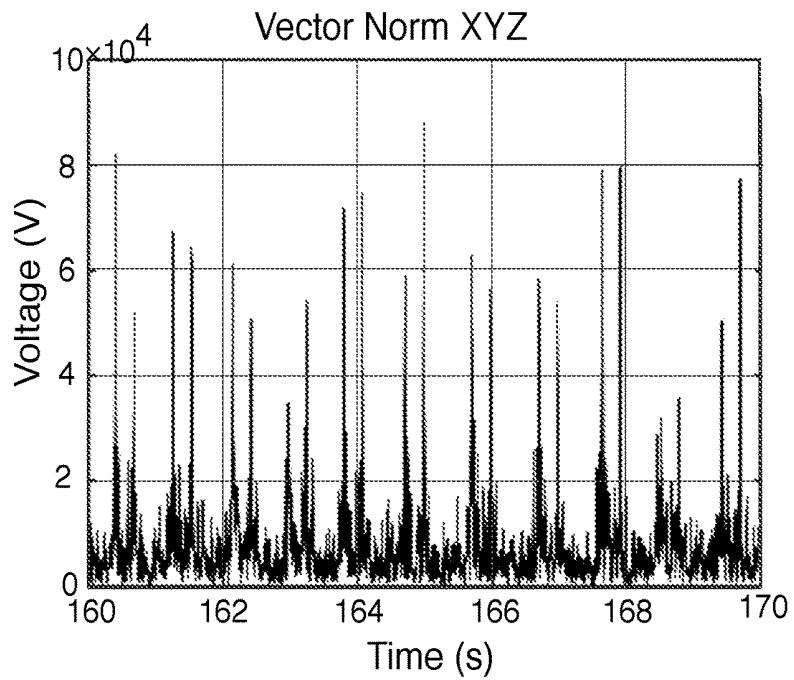


Fig. 6

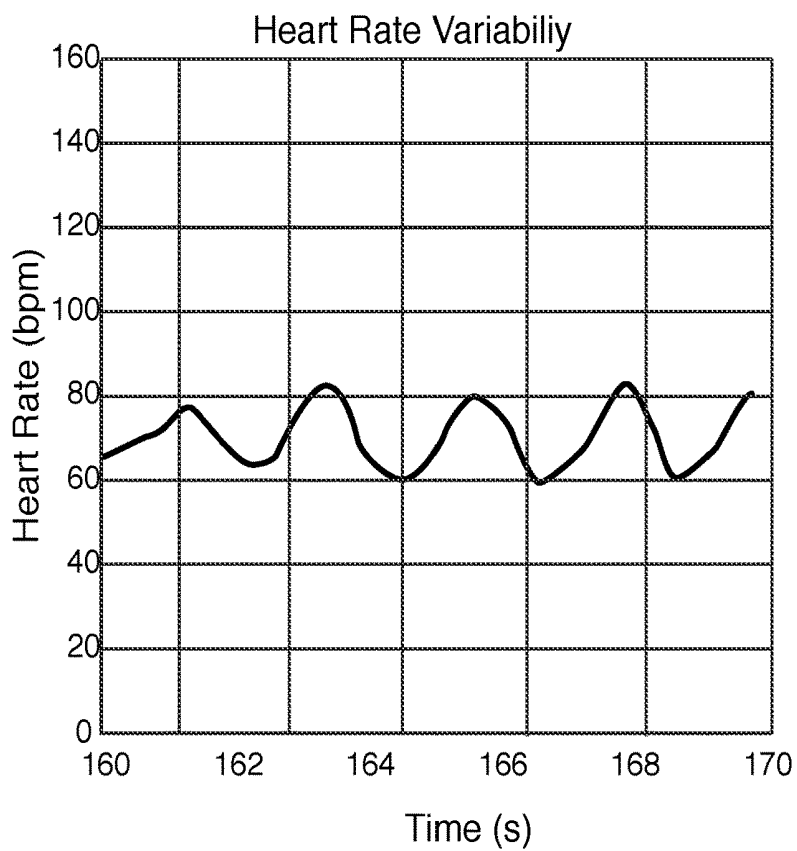


Fig. 7

## MEASURING RESPIRATION WITH AN IN-EAR ACCELEROMETER

### RELATED APPLICATIONS

**[0001]** This application is related to, and incorporates by reference, U.S. patent application Ser. No. 15/106,989, filed Jun. 21, 2016; application Ser. No. 15/348,400, filed Nov. 10, 2016; and application Ser. No. 15/352,034, filed Nov. 17, 2016, all titled Intelligent Earplug System. It is also related to U.S. patent application Ser. No. 15/267,567, entitled Sleep Assistance Device; application Ser. No. 15/267,464, entitled Sleep Quality Scoring and Improvement; application Ser. No. 15/267,552, entitled Intelligent Wake-Up System; application Ser. No. 15/267,848, entitled Sleep System; application Ser. No. 15/267,858, entitled User Interface for a Sleep System; and application Ser. No. 15/267,886, entitled Sleep Assessment Using a Home Sleep System, all of which were filed on Sep. 16, 2016. It is also related to U.S. patent application Ser. No. 15/655,836, titled Sleep Assistance Device For Multiple Users, and Ser. Nos. 15/655,845, 15/655,853, and 15/655,857, all titled Earphones for Measuring and Entraining Respiration, filed Jul. 20, 2017, and incorporated here by reference.

### BACKGROUND

**[0002]** This disclosure relates to earphones for measuring and entraining respiration.

**[0003]** Sleeplessness and poor or interrupted sleep may significantly affect a person's health. Poor sleep may be caused by such factors as ambient noise, stress, medical conditions, or discomfort. Thus, there exists a need for a sleep aid that can help address the underlying causes of poor sleep without adversely affecting the user's health in other, unintended ways.

### SUMMARY

**[0004]** In general, in one aspect, a system includes an earphone with a loudspeaker, an accelerometer, a housing supporting the loudspeaker and accelerometer, and an ear tip surrounding the housing and configured to acoustically couple the loudspeaker to an ear canal of a user, and a processor. The processor receives input signals from the accelerometer in response to motion of the earphone, and detects peaks in the input signals. Based on the detected peaks, the processor computes an instantaneous heart rate, measures a frequency of an oscillation within the instantaneous heart rate, and based on the frequency of the oscillation, computes a rate of respiration.

**[0005]** Implementations may include one or more of the following, in any combination. The accelerometer may be located on a circuit board within the earphone. The housing may include an outer shell of the earphone, and the accelerometer may be located in the outer shell. The input signals may include acceleration measurements for each of three axes, and the processor may detect the peaks by combining the three acceleration measurements into the norm of the three measurements. The processor may receive second input signals from a second accelerometer in a second earphone, including second acceleration measurements for each of three axes of the second accelerometer, combine the second three acceleration measurements into the norm of the second three measurements, detect the peaks by combining the norm of the three measurements from the first accel-

ometer with the norm of the three measurements from the second accelerometer, and detect peaks within the result of the combination. Combining the norms may include multiplying the amplitude of the norm of the first three acceleration measurements by the amplitude of the norm of the second three acceleration measurements, at each time that the two accelerometers' measurements are sampled. The processor may adjust output audio signals based on the rate of respiration, and provide the output audio signals to the loudspeaker.

**[0006]** Adjusting the output audio signals may include adjusting a rhythm of the output audio signals to be about one cycle per minute less than the detected respiration rate. Adjusting the output audio signals may include transitioning the output audio signals from respiration entrainment sounds to masking sounds. Adjusting the output audio signals may include transitioning the output audio signals from masking sounds to awakening sounds. The earphone may include a memory storing sound files, and providing the output audio signals may include retrieving a first sound file from the memory. Adjusting the output audio signals may include retrieving a second sound file from the memory and using the second sound file to generate the output audio signal.

**[0007]** The processor may be integrated within the earphone. The processor may be integrated within a portable computing device. The processor may measure the frequency of the oscillation within the instantaneous heart rate by computing a fast Fourier transform (FFT) of the instantaneous heart rate. The processor may measure the frequency of the oscillation within the instantaneous heart rate by computing a gradient of the instantaneous heart rate, and computing a fast Fourier transform (FFT) of the gradient of the instantaneous heart rate. The processor may measure the frequency of the oscillation within the instantaneous heart rate by detecting peaks of the instantaneous heart rate. The processor may measure the frequency of the oscillation within the instantaneous heart rate by fitting a sine function to the instantaneous heart rate, the frequency of the sine being the frequency of the oscillation. The ear tip may be configured to acoustically close the entrance to the user's ear canal.

**[0008]** In general, in one aspect, measuring the respiration rate of a user of an earphone includes receiving input signals from an accelerometer supported within the earphone, the input signals including acceleration measurements for each of three axes, and, in a processor, combining the three acceleration measurements into the norm of the three measurements, detecting peaks in the norm of the accelerometer measurements, based on the detected peaks, computing an instantaneous heart rate, measuring a frequency of an oscillation within the instantaneous heart rate, and based on the frequency of the oscillation, computing a rate of respiration.

**[0009]** Implementations may include one or more of the following, in any combination. Measuring the frequency of the oscillation within the instantaneous heart rate may include computing a fast Fourier transform (FFT) of the instantaneous heart rate. Measuring the frequency of the oscillation within the instantaneous heart rate may include computing a gradient of the instantaneous heart rate, and computing a fast Fourier transform (FFT) of the gradient of the instantaneous heart rate. Measuring the frequency of the oscillation within the instantaneous heart rate may include detecting peaks of the instantaneous heart rate. Measuring the frequency of the oscillation within the instantaneous

heart rate may include fitting a sine function to the instantaneous heart rate, the frequency of the sine being the frequency of the oscillation. Second input acceleration signals may be received from a second accelerometer supported within a second earphone, the second input signals including acceleration measurements for each of three axes of the second accelerometer; the processor may detect the peaks by combining the second three acceleration measurements into the norm of the second three measurements, combining the norm of the first three acceleration measurements with the norm of the second three acceleration measurements, and detecting peaks within the result of the combination.

[0010] Advantages include sensing the respiration rate at the ear without interference from audio signals being generated by the earphone, and without a need to seal the ear interface.

[0011] All examples and features mentioned above can be combined in any technically possible way. Other features and advantages will be apparent from the description and the claims.

#### BRIEF DESCRIPTION OF THE DRAWINGS

[0012] FIGS. 1 and 2 show cross-sectional views of earphones with an integrated accelerometer.

[0013] FIG. 3 shows an external view of the system of FIG. 1 or 2.

[0014] FIGS. 4A, 4B, 4C, 4D, 4E, 4F, 5A, 5B, 6, and 7 show graphs of sensor readings

#### DESCRIPTION

[0015] Several of the above-referenced applications describe a bedside system that detects a user's respiration rate and uses that to infer and manage their sleep state. In particular, to assist the user with falling to sleep, the system plays sounds that have a rhythm slightly slower than the user's own respiration rate. This naturally leads the user to slow their breathing to match the rhythm of the sounds, in a process referred to as entrainment. As the user slows their rate of respiration, the rate of the sounds is further reduced, in a feedback loop that leads the user gradually to sleep. Once the user falls asleep (as indicated by artifacts in their respiration rate), the system switches to playing masking sounds, which diminish the user's ability to detect, and be disturbed by, external sounds. If the user is detected to be waking up too early, entrainment may be reactivated. When it is time for the user to wake up, the system may coordinate wake-up sounds with the user's sleep state and other information to wake the user in the least-disruptive way possible.

[0016] Others of the above-referenced applications describe intelligent earplugs which the user can wear while sleeping, and which provide masking sounds through the night, and alarm or alert sounds when needed. These earplugs are controlled by a smartphone, but principally operate autonomously, playing stored masking sounds until instructed otherwise by the controlling phone, or based on an internal clock. It would be advantageous if the intelligent earplugs could play the respiration-entraining sounds of the bedside systems, to help the user fall asleep without disturbing others who may be sharing the bed or room. One solution to that, described in co-pending application Ser. No. 15/655,836, is for the sleep system to inform the earplugs of the user's respiration rate and sleep state, and for the

earplugs to adjust the rate of a rhythmic component in stored entrainment sounds as in the out-loud system.

[0017] The Ser. Nos. 15/655,853 and 15/655,857 applications describe how to add respiration sensing to the earplugs themselves, using microphones, so that the external system is not required, and the earplugs can operate fully autonomously, or with only a smart phone to control them.

[0018] The technique described in the '853 application, of using a microphone to measure heart rate variability, and from that deriving respiration rate, can also be performed using an accelerometer, as described below.

[0019] As shown in FIGS. 1 and 3, sleep-sensing earphones 100 include an ear tip sealing structure 102 that blocks, or occludes, the entrance to the ear canal. The earphones 200 in FIG. 2 omit the sealing structure 102, having instead an ear tip structure 202 that merely seats the earphone in the ear, without sealing the canal entrance. Aside from the different sealing structures, FIGS. 1 and 2 show cross-sections of two different earphone examples, while FIG. 3 shows an exterior view, for reference. The example of FIG. 3 uses the sealing structure 102 from FIG. 1, but the earbud of FIG. 2 would have similar appearance. A retaining structure 104 helps retain the earphone in the ear, and puts pressure on the sealing structure 102, if present, to maintain the seal by pushing on the concha, opposite to where the sealing structure meets the ear canal. The sealing structure 102 helps to passively block outside sounds from entering the ear, increasing the effectiveness of the masking sounds played by the earphones.

[0020] In the example of FIG. 1, an accelerometer 114 is located on the circuit board of earphone 100. In the example of FIG. 2, an accelerometer 214 is located in the outer shell of the earphone 200. In both examples, the accelerometer is able to detect motion of the earphone caused by the user's heartbeat, using the principles of ballistocardiography. Unlike techniques using a microphone, the accelerometer 114/214 can produce a usable signal without having to seal the ear canal, and can be located anywhere on the earphone, as demonstrated by these two examples. The processor 108 on-board each earphone (or in one, if they coordinate their action) can then extract the respiration rate from the accelerometer output, and adjust the timing of entrainment sounds being played to the user through a speaker 110. In the example of FIG. 1, the microphone is still present, for use in other functions, such as providing active noise cancellation or voice interface input.

[0021] The heartbeat is derived from the accelerometer signals, and the respiration rate is derived from the heart rate variability (HRV). FIGS. 4A-4F show the output accelerometer signals for three axes, as reported by accelerometers in both the left and right ears, filtered using a third-order Butterworth low-pass filter with a cutoff frequency of 50 Hz. The user's pulse is present in all six signals, but the signal to noise ratio (SNR) is not very high. In particular, in this example, the X and Z axes (4A, 4B, 4E, 4F) have much better SNR than the Y axis (4C and 4D, where the pulse is barely visible), but neither of them would easily yield the heart rate. In other examples, depending on the precise orientation of the earphones in the ears of the user, different axes could have a better or worse SNR on another user. Because the goal is to obtain the beat-to-beat heart rate, time average methods cannot be used to filter out the noise.

[0022] Instead of separately using the axes, we can combine the three axes of each ear into their norm:

$$N = \sqrt{x^2 + y^2 + z^2} \quad (1)$$

Graphs of the two norms, one for each ear, are shown in FIGS. 5A and 5B. Using the norm of the three axes not only improves the SNR, but also immunizes the reading to the exact orientation of the earphone in the user's ear. Other methods of combining the signals from the three axes may also be used.

**[0023]** Combining the amplitudes of the two signals at each time sample, such as by multiplication, can greatly increase the signal to noise ratio, as shown in FIG. 6. Note that each beat is represented by two peaks close to each other. Various standard de-duplicating procedures, such as envelope fitting, can be used to combine the peaks or otherwise manage the duplication.

**[0024]** Applying a peak-finding algorithm to the combined accelerometer signals and observing the distance between consecutive peaks yields the beat-to-beat, or instantaneous, heart rate value, shown in FIG. 7. Note that the peaks in the curve in FIG. 7 do not map to the pairs of peaks in FIG. 6—the shape of the curve in FIG. 7 shows the variability in the distance between the pairs of peaks in FIG. 6.

**[0025]** FIG. 7 shows that there is a cyclic variability to the instantaneous heart rate. The period of this variability happens to be the respiration rate—as the user inhales, their heart rate increases, and as they exhale, their heart rate decreases. Applying another peak detection step, or other frequency analysis such as a fast Fourier transform (FFT) or fitting a sine to the curve, to the instantaneous heart rate or to its gradient, reveals the respiration rate.

**[0026]** Embodiments of the systems and methods described above comprise computer components and computer-implemented steps that will be apparent to those skilled in the art. For example, it should be understood by one of skill in the art that the computer-implemented steps may be stored as computer-executable instructions on a computer-readable medium such as, for example, hard disks, optical disks, solid-state disks, flash ROMS, nonvolatile ROM, and RAM. Furthermore, it should be understood by one of skill in the art that the computer-executable instructions may be executed on a variety of processors such as, for example, microprocessors, digital signal processors, and gate arrays. For ease of exposition, not every step or element of the systems and methods described above is described herein as part of a computer system, but those skilled in the art will recognize that each step or element may have a corresponding computer system or software component. Such computer system and software components are therefore enabled by describing their corresponding steps or elements (that is, their functionality), and are within the scope of the disclosure.

**[0027]** A number of implementations have been described. Nevertheless, it will be understood that additional modifications may be made without departing from the scope of the inventive concepts described herein, and, accordingly, other embodiments are within the scope of the following claims.

What is claimed is:

1. A system comprising:

an earphone comprising:

a loudspeaker;

an accelerometer;

a housing supporting the loudspeaker and accelerometer; and

an ear tip surrounding the housing and configured to acoustically couple the loudspeaker to an ear canal of a user;

and

a processor configured to:

receive input signals from the accelerometer in response to motion of the earphone;

detect peaks in the input signals;

based on the detected peaks, compute an instantaneous heart rate;

measure a frequency of an oscillation within the instantaneous heart rate; and

based on the frequency of the oscillation, compute a rate of respiration.

2. The system of claim 1, wherein the accelerometer is located on a circuit board within the earphone.

3. The system of claim 1, wherein the housing comprises an outer shell of the earphone, and the accelerometer is located in the outer shell.

4. The system of claim 1, wherein:

the input signals comprise acceleration measurements for each of three axes, and

the processor is configured to detect the peaks by combining the three acceleration measurements into the norm of the three measurements.

5. The system of claim 4, further comprising:

a second earphone comprising:

a second loudspeaker;

a second accelerometer;

a second housing supporting the second loudspeaker and second accelerometer; and

a second ear tip surrounding the second housing and configured to acoustically couple the second loudspeaker to a second ear canal of the user;

wherein the processor is further configured to:

receive second input signals from the second accelerometer comprising second acceleration measurements for each of three axes of the second accelerometer;

combine the second three acceleration measurements into the norm of the second three measurements

and

detect the peaks by combining the norm of the three measurements from the first accelerometer with the norm of the three measurements from the second accelerometer, and detecting peaks within the result of the combination.

6. The system of claim 5, wherein combining the norms comprises multiplying the amplitude of the norm of the first three acceleration measurements by the amplitude of the norm of the second three acceleration measurements, at each time that the two accelerometers' measurements are sampled.

7. The system of claim 1, wherein the processor is further configured to adjust output audio signals based on the rate of respiration, and provide the output audio signals to the loudspeaker.

8. The system of claim 7, wherein adjusting the output audio signals comprises adjusting a rhythm of the output audio signals to be about one cycle per minute less than the detected respiration rate.

9. The system of claim 7, wherein adjusting the output audio signals comprises transitioning the output audio signals from respiration entrainment sounds to masking sounds.

10. The system of claim 7, wherein adjusting the output audio signals comprises transitioning the output audio signals from masking sounds to awakening sounds.

11. The system of claim 7, wherein the earphone further includes a memory storing sound files; and providing the output audio signals comprises retrieving a first sound file from the memory.

12. The system of claim 11, wherein adjusting the output audio signals comprises retrieving a second sound file from the memory and using the second sound file to generate the output audio signal.

13. The system of claim 1, wherein the processor is integrated within the earphone.

14. The system of claim 1, wherein the processor is integrated within a portable computing device.

15. The system of claim 1, wherein the processor is configured to measure the frequency of the oscillation within the instantaneous heart rate by computing a fast Fourier transform (FFT) of the instantaneous heart rate.

16. The system of claim 1, wherein the processor is configured to measure the frequency of the oscillation within the instantaneous heart rate by computing a gradient of the instantaneous heart rate; and

computing a fast Fourier transform (FFT) of the gradient of the instantaneous heart rate.

17. The system of claim 1, wherein the processor is configured to measure the frequency of the oscillation within the instantaneous heart rate by detecting peaks of the instantaneous heart rate.

18. The system of claim 1, wherein the processor is configured to measure the frequency of the oscillation within the instantaneous heart rate by fitting a sine function to the instantaneous heart rate, the frequency of the sine being the frequency of the oscillation.

19. The system of claim 1, wherein the ear tip is configured to acoustically close the entrance to the user's ear canal.

20. A method of measuring the respiration rate of a user of an earphone, the method comprising:

receiving input signals from an accelerometer supported within the earphone, the input signals including acceleration measurements for each of three axes; and

in a processor,

combining the three acceleration measurements into the norm of the three measurements, detecting peaks in the norm of the accelerometer measurements, based on the detected peaks, computing an instantaneous heart rate, measuring a frequency of an oscillation within the instantaneous heart rate, and based on the frequency of the oscillation, computing a rate of respiration.

21. The method of claim 20, wherein measuring the frequency of the oscillation within the instantaneous heart rate comprises computing a fast Fourier transform (FFT) of the instantaneous heart rate.

22. The method of claim 20, wherein measuring the frequency of the oscillation within the instantaneous heart rate comprises:

computing a gradient of the instantaneous heart rate; and computing a fast Fourier transform (FFT) of the gradient of the instantaneous heart rate.

23. The method of claim 20, wherein measuring the frequency of the oscillation within the instantaneous heart rate comprises detecting peaks of the instantaneous heart rate.

24. The method of claim 20, wherein measuring the frequency of the oscillation within the instantaneous heart rate comprises fitting a sine function to the instantaneous heart rate, the frequency of the sine being the frequency of the oscillation.

25. The method of claim 20, further comprising:

receiving second input acceleration signals from a second accelerometer supported within a second earphone, the second input signals including acceleration measurements for each of three axes of the second accelerometer;

in the processor, detecting the peaks by:

combining the second three acceleration measurements into the norm of the second three measurements

combining the norm of the first three acceleration measurements with the norm of the second three acceleration measurements, and detecting peaks within the result of the combination.

\* \* \* \* \*

专利名称(译)	使用入耳式加速度计测量呼吸		
公开(公告)号	<a href="#">US20190231197A1</a>	公开(公告)日	2019-08-01
申请号	US15/881034	申请日	2018-01-26
[标]申请(专利权)人(译)	伯斯有限公司		
申请(专利权)人(译)	Bose公司		
当前申请(专利权)人(译)	Bose公司		
[标]发明人	KIRSZENBLAT ROMAIN IOFFE MIKHAIL		
发明人	KIRSZENBLAT, ROMAIN IOFFE, MIKHAIL		
IPC分类号	A61B5/0205 A61B5/00 H04R1/10		
CPC分类号	A61B5/0205 A61B5/7278 A61B5/7257 A61B5/6803 H04R1/1016 H04R1/1075 H04R1/1041 A61B5/02438 A61B5/0816 A61B2562/0219 A61B5/02444 A61B5/1102 A61B5/6815 A61B2560/0462 A61B2562/166 H04R1/1083		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

摘要(译)

耳机包括扬声器，麦克风，支撑扬声器和麦克风的外壳，以及围绕外壳并配置为将扬声器和麦克风声学地耦合到用户的耳道并且声学地关闭入口的耳塞。用户的耳道。处理器从麦克风接收输入音频信号，基于检测到的峰值检测输入音频信号中具有大约1Hz的频率的峰值，计算瞬时心率，测量瞬时心率内的振荡频率，以及根据振荡频率，计算呼吸率。

