



US 20170360314A1

(19) **United States**

(12) **Patent Application Publication**
Proença et al.

(10) **Pub. No.: US 2017/0360314 A1**

(43) **Pub. Date: Dec. 21, 2017**

(54) **METHOD, APPARATUS AND COMPUTER PROGRAM FOR DETERMINING A BLOOD PRESSURE VALUE**

Publication Classification

(51) **Int. Cl.**

A61B 5/021 (2006.01)

A61B 5/0215 (2006.01)

A61B 5/00 (2006.01)

(52) **U.S. Cl.**

CPC *A61B 5/02116* (2013.01); *A61B 5/7221* (2013.01); *A61B 5/7278* (2013.01); *A61B 5/02125* (2013.01); *A61B 5/02156* (2013.01); *A61B 5/02154* (2013.01); *A61B 2562/0219* (2013.01)

(71) Applicant: **CSEM Centre Suisse d'Electronique et de Microtechnique SA - Recherche et Développement, Neuchâtel (CH)**

(72) Inventors: **Martin Proença, Marly (CH); Josep Sola i Caros, Corcelles (CH); Matthieu Lemay, St-Sulpice (CH); Christophe Verjus, Neuchâtel (CH)**

(21) Appl. No.: **15/543,299**

(22) PCT Filed: **Jun. 18, 2015**


(86) PCT No.: **PCT/EP2015/063765**

§ 371 (c)(1),

(2) Date: **Jul. 13, 2017**

ABSTRACT

(57) Method for determining a blood pressure value including the steps of: providing a pulsatility signal, determining a time-related feature and a normalized amplitude-related feature on the basis of the pulsatility signal; and calculating a blood pressure value on the basis of a blood pressure function depending on the time-related feature, the normalized amplitude-related feature and function parameters.

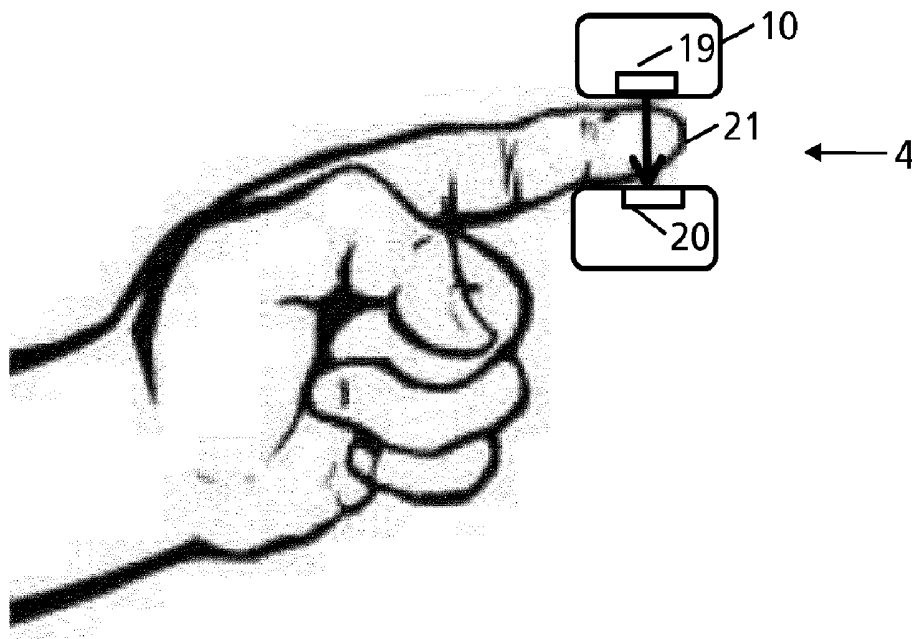

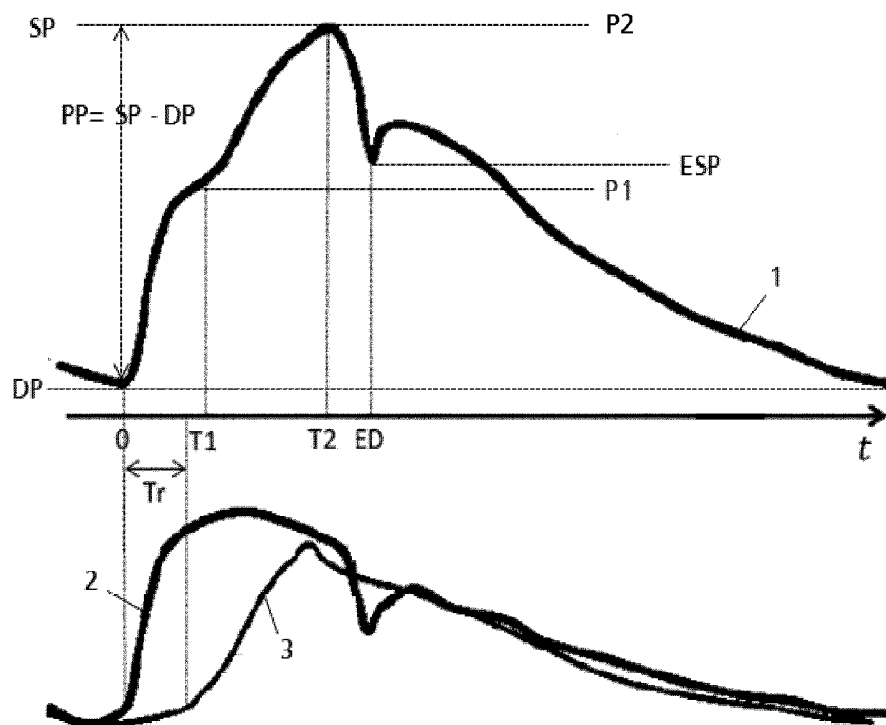


Fig. 1 PRIOR ART

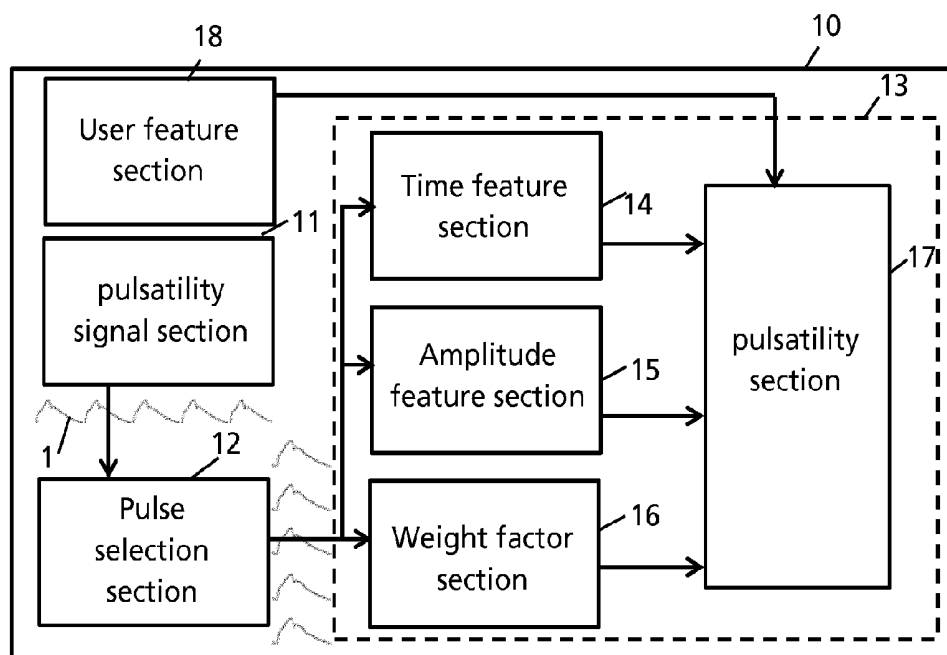


Fig. 2

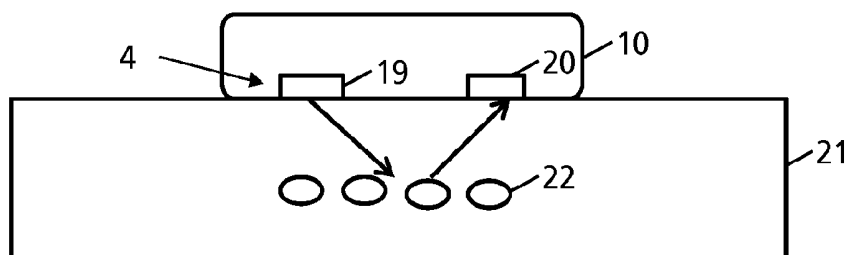


Fig. 3

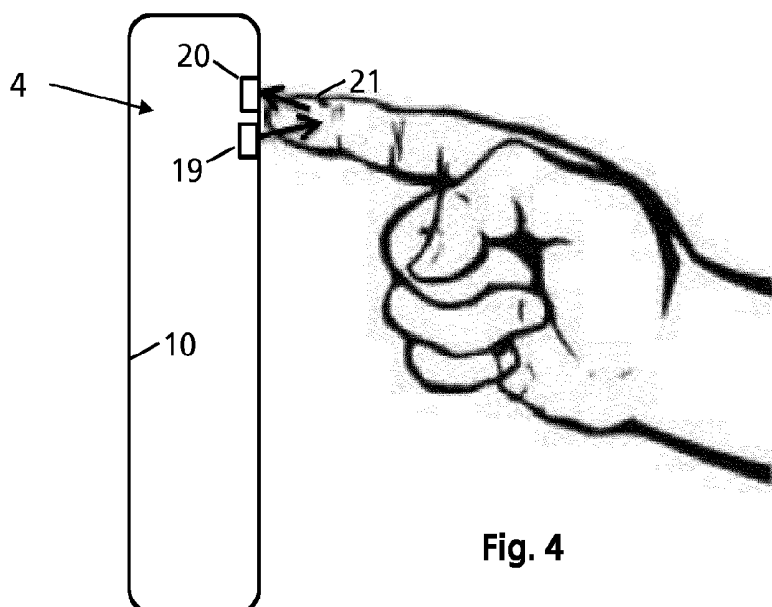


Fig. 4

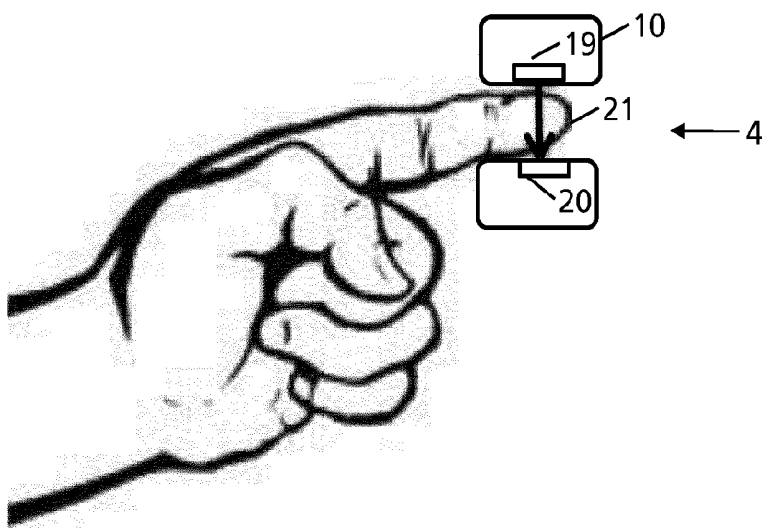


Fig. 5

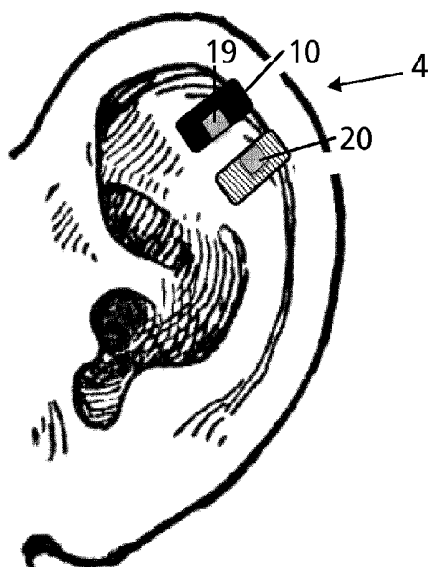


Fig. 6

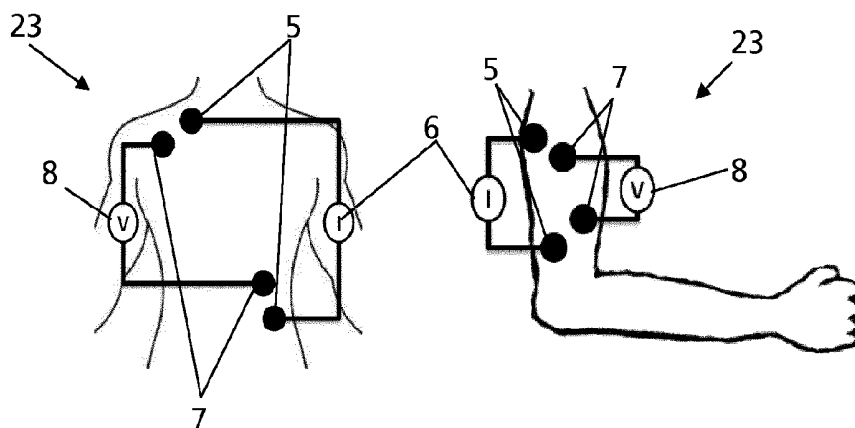


Fig. 7

Fig. 8

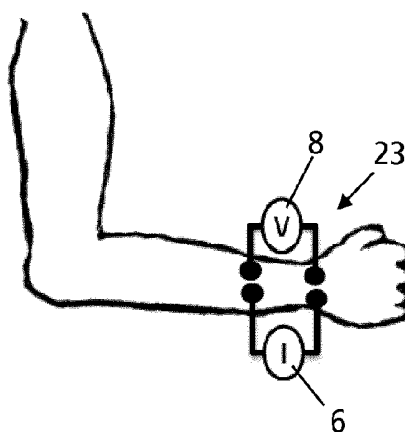


Fig. 9

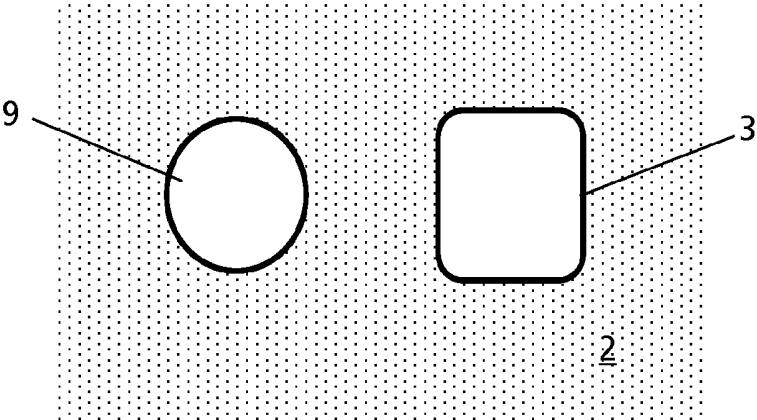


Fig. 10

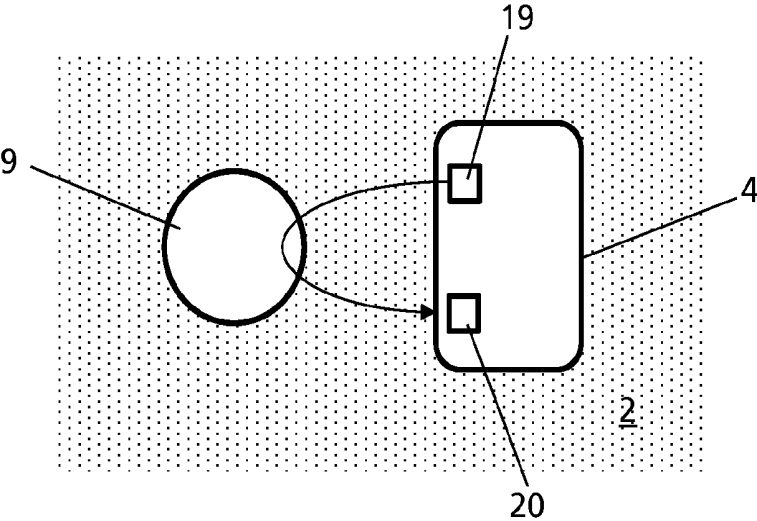


Fig. 11

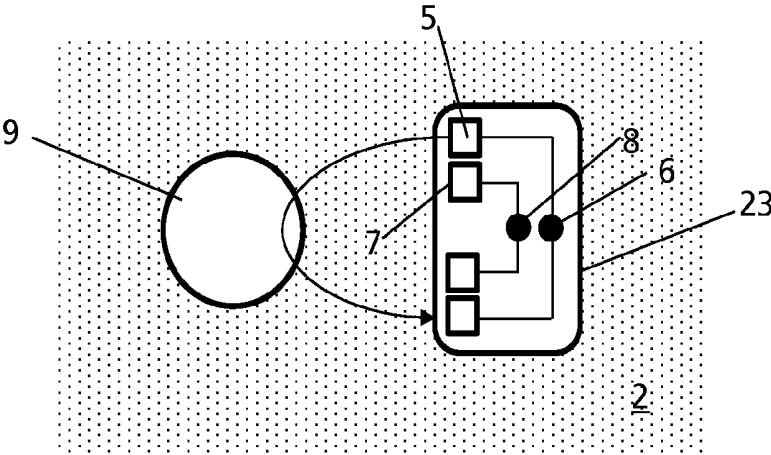


Fig. 12

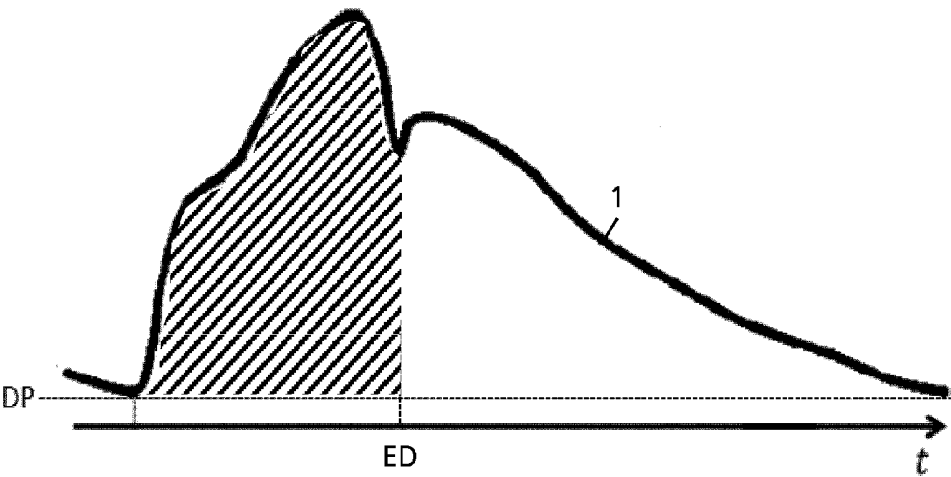


Fig. 13

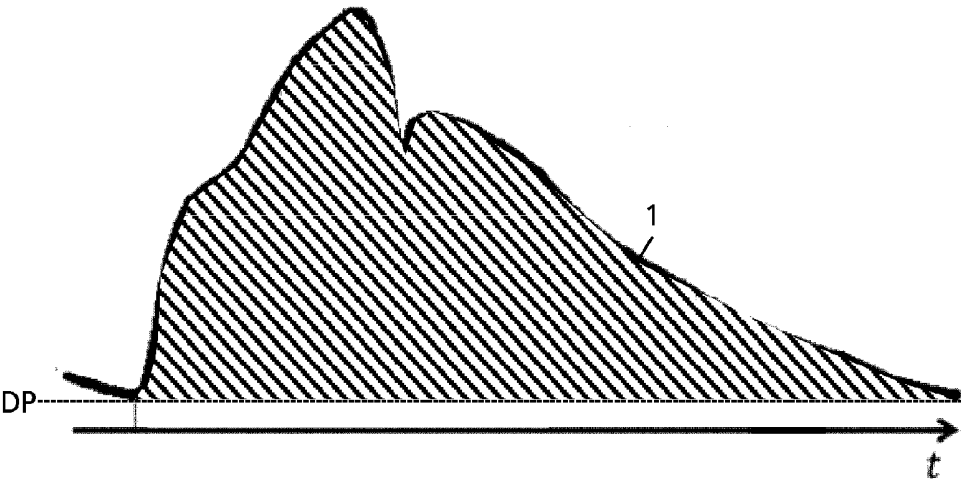


Fig. 14

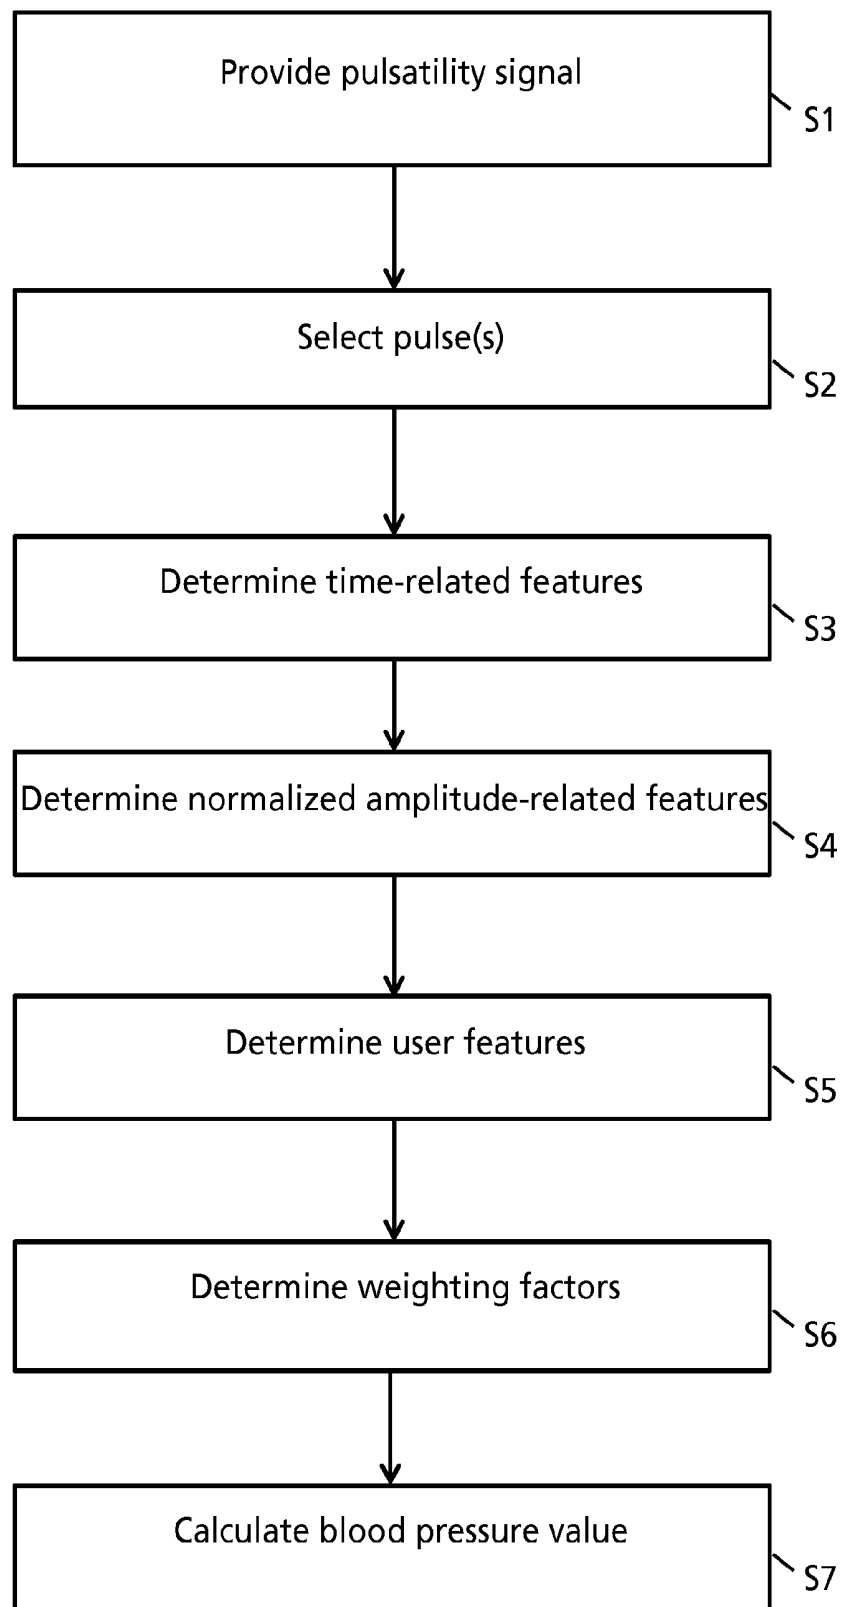


Fig. 15

METHOD, APPARATUS AND COMPUTER PROGRAM FOR DETERMINING A BLOOD PRESSURE VALUE

FIELD OF THE INVENTION

[0001] The present invention concerns a method, apparatus and computer program for determining a blood pressure value.

DESCRIPTION OF RELATED ART

[0002] Blood pressure is the pressure exerted by circulating blood upon the walls of blood vessels. A person's blood pressure is usually expressed in terms of the systolic pressure (maximum pressure within an artery during the cardiac cycle), diastolic pressure (minimum pressure within an artery during the cardiac cycle) or pulse pressure (the difference between the systolic and the diastolic pressure values).

[0003] Systolic, diastolic and pulse pressure values are used to detect certain health or fitness states of a body and/or to detect diseases.

[0004] However, to measure systolic, diastolic or pulse pressure values requires measuring a blood pressure signal via an invasive sensor (sensors placed within an artery).

[0005] In the recent time, there were many attempts to provide estimates of blood pressure values on the basis of pulsatility signals, instead of invasive blood pressure signals. Pulsatility signals have the advantage that are easy to be measured non-invasively. These attempts have even increased because of the commercialization of low quality sensors that can be used in wearable devices, e.g. like a photoplethysmogram (PPG) implemented in consumer electronics.

[0006] FIG. 1 shows an example of a pulsatility signal 1 for one heart beat. A pulsatility signal 1 is the superposition of the forward pulsatility signal 2 generated by a forward pressure wave propagating within the artery, and the backward pulsatility signal 3 generated by a pressure wave reflecting back within the artery.

[0007] Conventionally, blood pressure values are obtained by analyzing the shape and waveforms of such pulsatility signals. Unfortunately, pulsatility signals are signals related to the blood pressure signals, but are not real blood pressure signals. The amplitude and shape distortions of pulsatility signals have been shown to lead to large errors on the estimation of blood pressure values. In particular, the values of DP (diastolic pressure), SP (systolic pressure), P1 (central initial systolic peak) and ESP (pressure at the end of systole) of a pulsatility signal do correspond neither in amplitude nor in timing with the DP, SP, P1 and ESP values of the underlying blood pressure signal.

[0008] However, because of the major advantage of using pulsatility signals instead of invasive blood pressure signals, several attempts to derive BP values from pulsatility signals are disclosed in the state of the art:

[0009] U.S. Pat. No. 5,140,990 discloses a mapping of PPG signal amplitudes into BP values according to a physiological model.

[0010] JP2000217796 discloses the mapping of several features extracted from the second derivative of a PPG signal into a BP value.

[0011] U.S. Pat. No. 7,238,159 discloses calculating a BP-related value from the parameters of a mathematical model fitted to a PPG waveform.

[0012] U.S. Pat. No. 7,326,180 discloses the comparison of a BP value against features calculated from a pulse wave monitor: comparison is done in order to evaluate the cardiovascular status of a patient.

[0013] US2011/0196244 discloses an apparatus to measure BP by means of processing a PPG signal. The PPG signal is processed by an ARMA filter and a random forest operator.

[0014] U.S. Pat. No. 8,398,556 discloses the calculation of a BP value from a feature based on the area under a portion of a PPG waveform.

[0015] However, all those features for the blood pressure value are not sufficiently robust against gain changes due to electronic drifts, skin colors, sensor-skin interface and/or do not provide blood pressure measurements sufficiently accurate.

BRIEF SUMMARY OF THE INVENTION

[0016] The object is to provide a method, an apparatus and a computer program for determining a blood pressure value which yields a robust and accurate value for the blood pressure from the pulsatility signal.

[0017] The object is solved by the independent claims.

[0018] The combination of a time-related and an amplitude-related feature to calculate the blood pressure value gives an accurate and robust estimate for the blood pressure value.

[0019] The combination of a time-related feature and an amplitude-related feature in a single blood pressure function has been found to provide highly reliable blood pressure values. Because of the fact that the information contained in both features is independent and complementary, this combination overcomes the performances of known methods for determining blood pressure values using a pulsatility signal. In addition, the use of a normalized amplitude-related feature (instead of an amplitude-related feature) makes the value even more independent from electronic drifts, skin colors and sensor-skin interface, facilitating the implementation of the method of the invention in low-cost consumer electronic devices. Another advantage is that the method disclosed herein can be applied on very simple pulsatility signals such as photoplethysmogram signals.

[0020] The dependent claims refer to advantageous embodiments of the invention.

BRIEF DESCRIPTION OF THE DRAWINGS

[0021] The invention will be better understood with the aid of the description of an embodiment given by way of example and illustrated by the figures, in which:

[0022] FIG. 1 shows an example of a typical pulsatility signal.

[0023] FIG. 2 shows an embodiment of the apparatus for determining a blood pressure value.

[0024] FIG. 3 shows a wrist device with a reflective PPG pulsatility sensor, according to an embodiment.

[0025] FIG. 4 shows a smartphone with a reflective PPG pulsatility sensor, according to an embodiment.

[0026] FIG. 5 shows a fingertip device with a transmission PPG pulsatility sensor, according to an embodiment.

[0027] FIG. 6 shows an ear device with a transmission PPG pulsatility sensor, according to an embodiment.

[0028] FIG. 7 shows a chest device with an impedance pulsatility sensor, according to an embodiment.

[0029] FIG. 8 shows an arm device with an impedance pulsatility sensor, according to an embodiment.

[0030] FIG. 9 shows a wrist device with an impedance pulsatility sensor, according to an embodiment.

[0031] FIG. 10 shows an implanted accelerometer pulsatility sensor, according to an embodiment.

[0032] FIG. 11 shows an implanted PPG pulsatility sensor, according to an embodiment.

[0033] FIG. 12 shows an implanted impedance pulsatility sensor, according to an embodiment.

[0034] FIG. 13 shows the ejection area under the pulsatility signal.

[0035] FIG. 14 shows the total area under the pulsatility signal.

[0036] FIG. 15 shows an embodiment of the method for determining a blood pressure value.

DETAILED DESCRIPTION OF POSSIBLE EMBODIMENTS OF THE INVENTION

[0037] FIG. 2 shows an embodiment of the apparatus 10 for determining a blood pressure value. The apparatus 10 comprises a pulsatility signal section 11, a pulse selection section 12, a calculation section 13 and a user feature section 18.

[0038] The pulsatility signal section 11 is configured to provide a pulsatility signal. In one embodiment, the pulsatility signal section 11 could be simply an interface configured to receive data representing a pulsatility signal. In another embodiment, the pulsatility signal section 11 could be or comprise a pulsatility sensor for measuring the pulsatility signal of a user. A pulsatility signal can be defined as a signal containing information on the periodic variation of blood flow and arterial diameter of a given segment of the arterial tree. The periodic variations are typically generated by the arrival of a pressure pulse at the given segment of the arterial tree.

[0039] In one embodiment, the pulsatility sensor is a PPG sensor. The PPG sensor can be transmission-based or reflective. FIG. 3 shows an example apparatus 10 with a reflective PPG sensor 4. The apparatus 10 is realized in a wrist device with a light source 19 and a light detector 20 on the side of the wrist device being in contact with the arm skin 21 of a user. Due to the pulsatility of blood flow through the tissue in the subcutaneous vasculature 22, the reflective index of the skin 21 changes. The pulsatility signal of the user can be measured on the basis of the reflective index of the skin 21. The wrist device can comprise also the sections 12 and/or 13 and/or 18 forming the complete apparatus 10. Alternatively, the sections 12 and/or 13 and/or 18 can be arranged in another device of the apparatus 10 connected with the wrist device (e.g. by a cable or a wireless connection). The wrist device 10 can be for example a wrist device like a watch connected to a smart phone. FIG. 4 shows another embodiment of the apparatus 10 realized in a smartphone with the light source 19 and the light detector 20. The light source 19 can for example be realized by a flash of the smart phone 10. The light detector 20 can for example be realized by a camera (e.g. CCD) of the smartphone 10. FIG. 5 shows another embodiment of the apparatus 10 comprising a fingertip device with a transmission PPG sensor 4 with the

light source 19 and the light detector 20. The fingertip device can comprise also the sections 12 and/or 13 and/or 18 forming the complete apparatus 10. Alternatively, the sections 12 and/or 13 and/or 18 can be arranged in another device of the apparatus 10 connected with the fingertip device. An alternative transmission PPG sensor 4 can be arranged at the ear. Such a transmission PPG sensor 4 can for example be included in a hearing aid device.

[0040] However, a pulsatility sensor is not restricted to PPG sensors. Also bioimpedance pulsatility sensors are possible as shown in FIGS. 7 to 9. Such a bioimpedance sensor 23 comprises two electrodes 5 for injecting a current 6 and two further electrodes 7 for measuring a voltage 8. This allows also to measure the pulsatility signal. FIG. 7 shows a chest device with an impedance pulsatility sensor. FIG. 8 shows an arm device with an impedance pulsatility sensor 23. FIG. 9 shows a wrist device with an impedance pulsatility sensor 23. The pulsatility sensors where non-invasive sensors. Also implantable pulsatility sensors are possible. The pulsatility signal can for example be measured by an implanted accelerometer sensor 3 implanted in the body tissue 2 in the vicinity of an artery 9 (see FIG. 10). The pulsatility signal can for example be measured by an implanted PPG sensor 4 implanted in vicinity of an artery (see FIG. 11). The pulsatility signal can for example be measured by an implanted impedance sensor 23 implanted in vicinity of an artery 9 (see FIG. 12). The pulsatility signal can for example be measured by an invasive arterial sensor implanted within an artery (not shown).

[0041] The pulsatility signal 1 of a user is a signal representing the pulsatility amplitude of blood flow through the tissue over the time of the user as shown in FIG. 1. The pulsatility signal is a periodic signal with the period given by the heartbeat of the user. The pulsatility signal consists therefore of a sequence of pulses. FIG. 1 shows one exemplary pulse of the pulsatility signal 1.

[0042] The pulse selection section 12 determines at least one pulse in the pulsatility signal 1 of the user. In a preferred embodiment, the pulse selection section 12 selects a plurality of pulses which are given to the calculation section 13. The plurality of pulses can be a fix number of consecutive pulses. Preferably, N consecutive pulses of the pulsatility signal are identified and $M < N$ pulses of the N pulses are selected to be given to the calculation section 13. The M pulses can be selected on the basis of a quality criterion. The quality criterion can be defined to identify the presence of a measurement artifact. For example, because measurement artifacts tend to be associated to very large amplitude signals, the (M-N) pulses with the largest amplitudes (e.g. largest SP or largest total surface under the pulse) can be removed. In another embodiment, only one pulse can be selected and given to the calculation section 13. This is in particular advantageous for high quality pulsatility sensor and/or for high time resolution applications. In one embodiment, the start and end time of each pulse can be detected on the basis of signal analysis. Alternatively, the start and/or end point of each pulse can be detected on the basis of a second measurement. The second measurement should depend also on the heartbeat. This second measurement can be for example an electrocardiogram (ECG) signal from which the start time of each pulse (corresponding to the end time of the previous pulse) can be retrieved. The ECG signal can therefore be used as trigger signal for finding the start of each pulse of the pulsatility signal 1 of the user. The second

measurement can for example also be a PPG signal, a bioimpedance signal or any suitable pulsatility signal.

[0043] The user feature section **18** is configured to provide user feature UF about the user related to the pulsatility signal **1**. The user feature UF can be used in the calculation section **13**. The user feature section **18** can comprise a storage section for storing the user feature(s). The user feature section **18** can alternatively or additionally comprise a user interface for entering the user feature(s). Examples for user features UF are one or any combination of gender, age, height, body mass index, Gender can be mathematically expressed by a binary value, e.g. by 1 for female and 0 for male or vice versa. However, the user feature section **18** is optional and is not necessary, if the blood pressure value calculated in the calculation section **13** is independent of a user feature.

[0044] The calculation section **13** comprises a time feature section **14**, an amplitude feature section **15**, a weight factor section **16** and a blood pressure section **17**. The calculation section **13** is configured to calculate a blood pressure value on the basis of the pulse(s) received from the pulse selection section **12**. In one embodiment, the calculation section **13** calculates one blood pressure value on request. In another embodiment, the calculation section **13** calculates continuously new blood pressure values, wherein for each calculation period one blood pressure value is calculated. In the latter case, the pulse selection section **12** gives within each calculation period one pulse or M pulses of the pulsatility signal **1** used for the calculation of a blood pressure value for this calculation period. In the following, the functioning of the calculation section **13** and its components is described for the calculation of one blood pressure value. For the calculation of a plurality of blood pressure values, this functioning is simply repeated.

[0045] The time feature section **14** is configured to determine at least one time-related feature TRF on the basis of the pulse(s) received from the pulse selection section **12**. Preferably, the at least one time-related feature TRF_i feature is computed from each pulse i of the M pulses of the pulsatility signal **1** received from the pulse selection section **12** so that for each time-related feature M values will be calculated. However, it is also possible to compute a time related feature TRF on the basis of M pulses, e.g. the heart rate. If only one pulse is received from the pulse selection section **12** for one blood pressure calculation period, the at least one time related feature TRF is computed only for this pulse. A time-related feature is preferably any time duration within a pulse, the inverse of such a time duration, or any other value computed from such a time duration, e.g. the average of a time duration or its inverse of a plurality of peaks. Examples for such a time-related feature are the time to first peak T1 (duration between the start time of the pulse and its first peak or shoulder of pulse), time to second peak T2 (duration between start time of pulse and second peak or shoulder of pulse), inverse time to first peak $1/T1$, inverse of time to second peak $1/T2$, time between first and second peak $T2-T1$, time to reflection Tr (duration between start time of pulse and arrival time of the reflected (backward) wave), ejection duration ED (duration between start time of pulse and time of closure of the aortic valve), heart rate. The detection and/or calculation of these time-related features TRF is well-known in the state of the art and is not described here in more detail. The at least one time-related feature TRF comprises L equal one, two, or more distinct time-related

features TRF_j . In the case that for each pulse i of the M pulses, L distinct time-related features $TRF_{i,j}$ are calculated, for each calculation period, M*L time-related features $TRF_{i,j}$ are calculated.

[0046] The amplitude feature section **15** is configured to determine at least one normalized amplitude-related feature NAF on the basis of the pulse(s) received from the pulse selection section **12**. Preferably, at least one normalized amplitude-related NAF_i feature is computed from each pulse i of the M pulses of the pulse pressure signal **1** received from the pulse selection section **12**. However, it is also possible to compute a normalized amplitude-related feature NAF on the basis of the average of the M pulses. If only one pulse is received from the pulse selection section **12** (e.g. for one/each calculation period), the at least one normalized amplitude-related feature NAF is computed only for this pulse. An amplitude-related feature AF is preferably any value based on an amplitude value of the pulsatility signal **1**. A normalized amplitude-related feature NAF is an amplitude-related feature normalized by another amplitude-related feature. Normalization is preferably performed by a ratio of two amplitude-related features $NAF=AF1/AF2$. In one embodiment, such a normalized amplitude-related feature NAF is a normalized end-systolic pressure $nESP=(ESP-DP)/PP$ calculated by the difference of the absolute end-systolic pressure ESP and the diastolic pressure DP divided or normalized by the pulse pressure PP. In one embodiment, such a normalized amplitude-related feature NAF is a first augmentation index $Alx=(P2-P1)/PP$ calculated by the difference of the pressure amplitude of the second peak P2 and the pressure amplitude of the first peak P1 divided or normalized by the pulse pressure PP. In one embodiment, such a normalized amplitude-related feature NAF is a second augmentation index $Alp=(P2-DP)/(P1-DP)$ calculated by the difference of the pressure amplitude of the second peak P2 and the diastolic pressure amplitude DP divided or normalized by the difference of the pressure amplitude of the first peak P1 and the diastolic pressure amplitude DP. In one embodiment, such a normalized amplitude-related feature NAF is a normalized ejection area $nEjecA$ (see FIG. 13). The normalized ejection area is calculated as the surface under the pulsatility signal **1** for the ejection duration ED divided or normalized by the area under the pulsatility signal **1** for the duration of this pulse (see FIG. 14). The surface under the pulsatility signal **1** for the ejection duration ED does preferably not include the surface $DP*ED$ below the diastolic pressure DP as shown in FIG. 13, but it is also possible to use the surface under the pulsatility signal **1** for the ejection duration ED with the surface $DP*ED$ below the diastolic pressure DP. The surface under the pulsatility signal **1** for the duration T of the pulse does preferably not include the surface $DP*T$ below the diastolic pressure DP as shown in FIG. 14, but it is also possible to use the surface under the pulsatility signal **1** for the pulse duration T with the surface $DP*T$ below the diastolic pressure DP, if the surface $DP*ED$ below the diastolic pressure is also considered for the ejection duration. The detection and/or calculation of the mentioned normalized amplitude-related features NAF are well-known and are therefore not described in more detail here. The at least one normalized amplitude-related features NAF comprises K equal one, two, or more distinct normalized amplitude-related features NAF_j . In the case that for each pulse i of the M pulses, K distinct normalized ampli-

tude-related features $NAF_{i,j}$ are calculated so that, for each calculation period, $M \times K$ normalized amplitude-related features $NAF_{i,j}$ are calculated.

[0047] The weight factor section 16 is optional and only necessary, if the calculation section 13 calculates a weighted average of the time-related feature(s) TRF and/or the normalized amplitude-related feature(s) NAF over a plurality of pulses with weights depending on the plurality of pulses. The weight factor section 16 is configured to calculate a weighting factor WF_i for each pulse i of the plurality M of pulses received from the pulse selection section. The weighting factor WF_i is preferably calculated on the basis of a quality criterion of the pulse. This could be for example the error of the pulse i relative to the average of the M pulses. Such an error can be calculated by a normalized accumulation of the errors between the points of the average pulse and the corresponding points of the respective pulse i . The errors can be the absolute errors, the quadratic errors, or any other measure for the error.

[0048] In one embodiment, the weighting factor WF_i is based on a morphological error. A morphological error can be defined as a value describing the morphology of a particular pulse. Typical morphologies have been defined in the literature (Nichols et al, "McDonald's blood flow in arteries", Oxford University Press 2005, ISBN 0 340 80941 8) and describe the timing and amplitude relationships between P1, P2, T1 and T2 (see FIG. 1). These morphologies may change among subjects depending on their age and cardiovascular status. Typical morphologies are Type C (associated to young subjects), Type B (associated to mid-age subjects), and Type A and D (associated to elderly and ill subjects). Other sub-morphologies can be defined as well. In a preferred embodiment, the weighting factor WF_i of the pulse i depends on how much the pulsatility signal i matches to a typical morphology. This could be for example the error of the pulse i relative to the most likely subject pulse morphology according to his age and health status.

[0049] In a yet preferred embodiment, the weighting factor WF_i of the pulse i depends on the morphological error of the pulse i and the error of the pulse i relative to the average of the M pulses. In one embodiment, the calculated quality criterion of each pulse i , e.g. the mentioned error and/or the morphological error, is compared to a quality threshold. Based on the comparison (above or below) the weight factor WF_i is set to zero (0) for bad quality and one (1) for a good quality. According to this binary weighting procedure only the pulses with a certain quality are used.

[0050] The pulsatility signal (1) can comprise a further plurality of pulses being larger than the plurality of pulses, wherein the plurality of pulses is selected among the further plurality of pulses by removing the pulses with the largest amplitude.

[0051] The blood pressure section 17 is configured to calculate a blood pressure value on the basis of the at least one time-related feature TRF and the at least one amplitude-related feature NAF. In one (optional) embodiment, a blood pressure function for calculating the blood pressure value depends additionally on the at least one user feature. In one embodiment, a blood pressure function for calculating the blood pressure value depends linearly on the at least one time-related feature TRF and the at least one normalized amplitude-related feature NAF. In one embodiment, a blood pressure function for calculating the blood pressure value depends linearly on the used feature(s) (TRF, NAF and/or

UF). Preferably, each feature is weighted relative to the other features by linear feature coefficients, like the linear time coefficient(s) kt , the linear amplitude coefficient(s) ka and the linear user coefficient ku . The linear time coefficient(s) kt and the linear amplitude coefficient(s) ka and, if user feature(s) UF is/are considered, a linear user coefficient ku fix the relative influence of the time-related feature(s) TRF and the normalized amplitude-related feature(s) and, if user features UF are considered, the user feature UF on the blood pressure value. If one or more of the features are calculated for a plurality of pulses, the feature coefficient k remains the same for the same feature for all pulses. In one embodiment, the blood pressure function depends on the at least one time-related feature TRF_i and the at least one amplitude-related feature NAF_i of a plurality of pulses i . In this case, the function for the blood pressure value BP is direct proportional to

$$\sum_{i=1}^M WF_i \cdot \left[\left(\sum_{j=1}^L kt_j \cdot TRF_{i,j} \right) + \left(\sum_{j=1}^K ka_j \cdot NAF_{i,j} \right) \right]$$

with M pulses, L time-related features TRF and K normalized amplitude-related features NAF with L being one, two or more and with K being one, two or more. If $M=1$ only one pulse is considered. If $L=1$, only one time-related feature TRF is considered. If $K=1$, only one normalized amplitude-related feature is considered. Therefore, the linear feature coefficient might be different for each feature, but is the same for the same feature of different pulses. Considering also user features UF, the function for the blood pressure value BP is direct proportional to

$$\sum_{i=1}^M WF_i \cdot \left[\left(\sum_{j=1}^L kt_j \cdot TRF_{i,j} \right) + \left(\sum_{j=1}^K ka_j \cdot NAF_{i,j} \right) + \left(\sum_{j=1}^U ku_j \cdot UF_j \right) \right]$$

with M pulses, L time-related features TRF, K normalized amplitude-related features NAF and U user features with L being one, two or more, with K being one, two or more and U being one, two or more. If $U=1$, only one user feature is considered. Obviously, the term of the user features could be taken out of the sum over the pulses, if the weight factors WF sum up to one or if the user coefficients are adapted accordingly.

[0052] In one embodiment, the feature coefficients kt , ka , ku are predetermined and stored in a storage section of the blood pressure section 17. In one embodiment, the feature coefficients kt , ka , ku are configurable. The feature coefficients kt , ka , ku can be set by a user or an administrator. The features coefficients kt , ka , ku can also be determined by an automatic process, e.g. a calibration process. The calibration process comprises the step of measuring the blood pressure of the user with an independent sensor and minimizing the error of the blood pressure value calculated by the blood pressure section on the basis of the feature coefficients kt , ka , ku . In medical applications, the apparatus can include a user interface for entering once or periodically blood pressure values measured independently. This allows an online monitoring of the blood pressure of the user which reaches almost

the preciseness of traditional cuff measurements, if the independent measurements are measured by cuff measurements of the blood pressure.

[0053] The calibration process can further include also the selection of the best time-related features and/or normalized amplitude-related features and/or user-related features among O potential features. This can be performed by performing the above described calibration process for all O! (factorial of O) potential combination of features and select the best combination of feature including at least one time-related feature and at least one normalized amplitude-related feature.

[0054] Even if the blood pressure value is calculated without having any absolute pressure amplitude value, the inventive method yields a robust blood pressure value. If the method is used without a calibration on the particular user, the results are still good enough to robustly detect hypotension (low blood pressure), normal blood pressure and hypertension (high blood pressure). If the method is used with a calibration on the particular user, the results yield a good estimate of the blood pressure value which is even good enough for medical applications. Such an algorithm could be used with pulse oximetry fingertip sensors including a PPG transmission sensor as shown in FIG. 5 or for other medical sensors shown for example in FIGS. 6 to 9 and described above. This would allow an online monitoring of the blood pressure with high preciseness instead of the state of the art cuff measurements which can only be repeated in fixed time intervals.

[0055] FIG. 15 shows an embodiment of the method for determining a blood pressure value.

[0056] In step S1, a pulsatility signal of the user is provided as described in more detail with respect to the pulsatility signal section 11. In step S2, a pulse or a number of pulses are selected from the provided blood pressure signal of Si. In step S3, at least one time-related feature is determined for the one pulse or for each of the number of pulses as described in more detail with respect to the time feature section 14. In step S4, at least one normalized amplitude-related feature is determined for the one pulse or for each of the number of pulses as described in more detail with respect to the amplitude feature section 15. In optional step S5, at least one user feature is determined as described in more detail with respect to the user feature section 18. In optional step S6, a weighting factor WF_i is determined for each of the number of pulses as described in more detail with respect to the weight factor section 16. In step S7, the blood pressure value is calculated on the basis of the at least one time-related feature TRF and the at least one normalized amplitude-related feature NAF and optionally on the weighting factors WF and the at least one user feature(s) as described in more detail with respect to the blood pressure section 17.

What is claimed is:

1. Method for determining a blood pressure value comprising the steps of:

- providing a pulsatility signal of a user;
- determining a first feature and a second feature on the basis of the pulsatility signal;
- calculating a blood pressure value on the basis of a blood pressure function depending on the first feature, the second feature and function parameters;
- the first feature being a time-related feature comprising a time duration within a pulse, and the second feature

being a normalized amplitude-related feature, wherein the calculating does not use a non-normalized amplitude-related feature.

2. Method according to claim 1,

wherein a time-related feature and a normalized amplitude-related feature are calculated on the basis of the pulsatility signal from each respective pulse of a plurality of pulses of the pulsatility signal,

wherein for each of the plurality of pulses a weighting factor is calculated on the basis of the pulsatility signal of the respective pulse, and

wherein the blood pressure function calculates the blood pressure value on the basis of a weighted combination, wherein the time-related feature and the normalized amplitude-related feature of each respective pulse is weighted with the weighting factor of the respective pulse.

3. Method according to claim 2, wherein the weighting factors are calculated on the basis of the error of the plurality of pulses from an average of the plurality of pulses and/or on the basis of morphology errors of the pulses.

4. Method according to claim 1, wherein the blood pressure function depends further on a user feature.

5. Method according to claim 1, wherein the blood pressure function is linear with respect to the time-related feature and the normalized amplitude-related feature.

6. Method according to claim 5, wherein the function parameters comprise a time-related coefficient and an amplitude-related coefficient, wherein the time-related feature is multiplied with the time-related coefficient and the normalized amplitude-related feature is multiplied with the amplitude-related coefficient before summing up the time-related feature with the normalized amplitude-related feature.

7. Method according to claim 4,

wherein the blood pressure function is linear with respect to the user feature,

wherein the function parameters comprise a user coefficient which is multiplied with the user feature before adding the user feature to the time-related feature and the normalized amplitude-related feature.

8. Method according to claim 4, wherein the user feature is based on one or a combination of:

- gender;
- age;
- body mass index;
- height.

9. Method according to claim 1, wherein function parameters are predetermined.

10. Method according to claim 1, wherein function parameters are calibrated on the basis of an independent measurement of the blood pressure of the user.

11. Method according to claim 1, wherein the features used for calculating the blood pressure value are automatically determined out of a plurality of features.

12. Method according to claim 1, wherein the time related feature is based on one or a combination of:

- time to first peak;
- time to second peak;
- inverse time to first peak;
- inverse of time to second peak,
- time between first and second peak,
- time to reflection,
- ejection duration,
- heart rate.

13. Method according to claim 1, wherein the normalized amplitude-related feature is based on one or a combination of:

- a normalized end-systolic pressure;
- an augmentation index;
- a normalized ejection area.

14. Method according to claim 1, wherein the step of providing the pulsatility signal comprises the step of measuring the pulsatility signal.

15. Method according to claim 14, wherein the pulsatility signal is measured on the basis of one of a photoplethysmogram, an impedance sensor, an implantable accelerometer sensor, an implantable optical sensor, an implantable impedance sensor or an invasive arterial sensor.

16. Computer program configured to perform a method when carried out on a processor, the method comprising providing a pulsatility signal of a user;

- determining a time-related feature comprising a time duration within a pulse and a normalized amplitude-related feature, on the basis of the pulsatility signal;
- calculating a blood pressure value on the basis of a blood pressure function depending on the time-related feature, the normalized amplitude-related feature and function parameters;

wherein the calculating does not use a non-normalized amplitude-related feature.

17. Apparatus for determining a blood pressure value comprising:

- a pulsatility signal section for providing a pulsatility signal of a user;
- a first feature calculation section for calculating a first feature on the basis of the pulsatility signal;
- a second feature calculation section for calculating a second feature on the basis of the pulsatility signal;
- a blood pressure section for calculating a blood pressure value on the basis of a function depending on the first feature, the second feature and function parameters;

the first feature being a time-related feature comprising a time duration within a pulse, and the second feature is a normalized amplitude-related feature, wherein the blood pressure section does not use a non-normalized amplitude-related feature for calculating the blood pressure value.

18. Apparatus according to claim 17 further comprising a pulse selection section for selecting a plurality of pulses of the pulsatility signal, wherein the first feature calculation section is configured to calculate the time-related feature for each of the plurality of pulses, wherein the second feature calculation section is configured to calculate the normalized amplitude-related feature for each pulse of the plurality of pulses, wherein the blood pressure section is configured for calculating the blood pressure value on the basis of a combination of the time-related features and the normalized amplitude-related features of the plurality of pulses.

19. Apparatus according to claim 18 further comprising a weighting factor section for calculating for each of the plurality of pulses a weighting factor on the basis of the respective pulse, wherein the blood pressure section is configured for calculating the blood pressure value on the basis of the weighted average, wherein the time-related feature and the normalized amplitude-related feature of each respective pulse is weighted with the weighting factor of the respective pulse.

20. Apparatus according to claim 18, wherein the pulsatility signal section comprises further a sensor for measuring a pulsatility signal.

21. Apparatus according to claim 20, wherein the sensor is:

- a PPG sensor;
- an impedance sensor;
- an implantable accelerometer sensor;
- an implantable optical sensor;
- an implantable impedance sensor; or
- an invasive arterial sensor.

* * * * *

专利名称(译)	用于确定血压值的方法，设备和计算机程序		
公开(公告)号	US20170360314A1	公开(公告)日	2017-12-21
申请号	US15/543299	申请日	2015-06-18
申请(专利权)人(译)	CSEM中心SUISSE D'电子与DE显微技术SA - RECHERCHE ET DEVELOPPEMENT		
当前申请(专利权)人(译)	CSEM中心SUISSE D'电子与DE显微技术SA - RECHERCHE ET DEVELOPPEMENT		
[标]发明人	PROENCA MARTIN SOLA I CAROS JOSEP LEMAY MATTHIEU VERJUS CHRISTOPHE		
发明人	PROENCA, MARTIN SOLA I CAROS, JOSEP LEMAY, MATTHIEU VERJUS, CHRISTOPHE		
IPC分类号	A61B5/021 A61B5/0215 A61B5/00		
CPC分类号	A61B5/02116 A61B5/02125 A61B5/02154 A61B2562/0219 A61B5/7278 A61B5/02156 A61B5/7221 A61B5/02108 A61B5/02416 A61B5/02438 A61B5/0535 A61B5/7235		
外部链接	Espacenet USPTO		

摘要(译)

用于确定血压值的方法包括以下步骤：提供脉动信号，基于脉动信号确定时间相关特征和归一化幅度相关特征；根据时间相关特征，归一化幅度相关特征和函数参数，根据血压函数计算血压值。

