



US 20180235504A1

(19) **United States**

(12) **Patent Application Publication**

Shin et al.

(10) **Pub. No.: US 2018/0235504 A1**

(43) **Pub. Date: Aug. 23, 2018**

(54) **ELECTROCARDIOGRAM (ECG) SENSOR CHIP, SYSTEM ON CHIP (SOC), AND WEARABLE APPLIANCE**

Publication Classification

(51) **Int. Cl.**

A61B 5/0428 (2006.01)
A61B 5/00 (2006.01)
A61B 5/0432 (2006.01)
A61B 5/0404 (2006.01)
A61B 5/0456 (2006.01)

(52) **U.S. Cl.**

CPC *A61B 5/04288* (2013.01); *A61B 5/681* (2013.01); *A61B 5/04325* (2013.01); *A61B 5/0404* (2013.01); *A61B 5/6803* (2013.01); *A61B 5/7225* (2013.01); *A61B 5/6833* (2013.01); *A61B 5/6824* (2013.01); *A61B 5/746* (2013.01); *A61B 5/0456* (2013.01)

(71) Applicant: **SAMSUNG ELECTRONICS CO., LTD.**, Suwon-si (KR)

(72) Inventors: **Seung Chul Shin**, Seoul (KR); **Hyung Jong Ko**, Seongnam-Si (KR); **Jung Su Kim**, Yongin-Si (KR); **Yong In Park**, Seoul (KR); **Won Hyuk Jung**, Yongin-Si (KR); **Yun Cheol Han**, Yongin-Si (KR)

(21) Appl. No.: **15/958,908**

(22) Filed: **Apr. 20, 2018**

Related U.S. Application Data

(62) Division of application No. 14/840,154, filed on Aug. 31, 2015, now Pat. No. 9,974,461.

Foreign Application Priority Data

Nov. 17, 2014 (KR) 10-2014-0160011

(57)

ABSTRACT

An ECG sensor chip used in a wearable appliance includes; a switch controlled by a switching signal, an amplifier that amplifies a difference between first and second ECG signals, and a location indicator that generates the switching signal. The switch passes either a first ECG signal or second ECG signal in response to the switching signal.

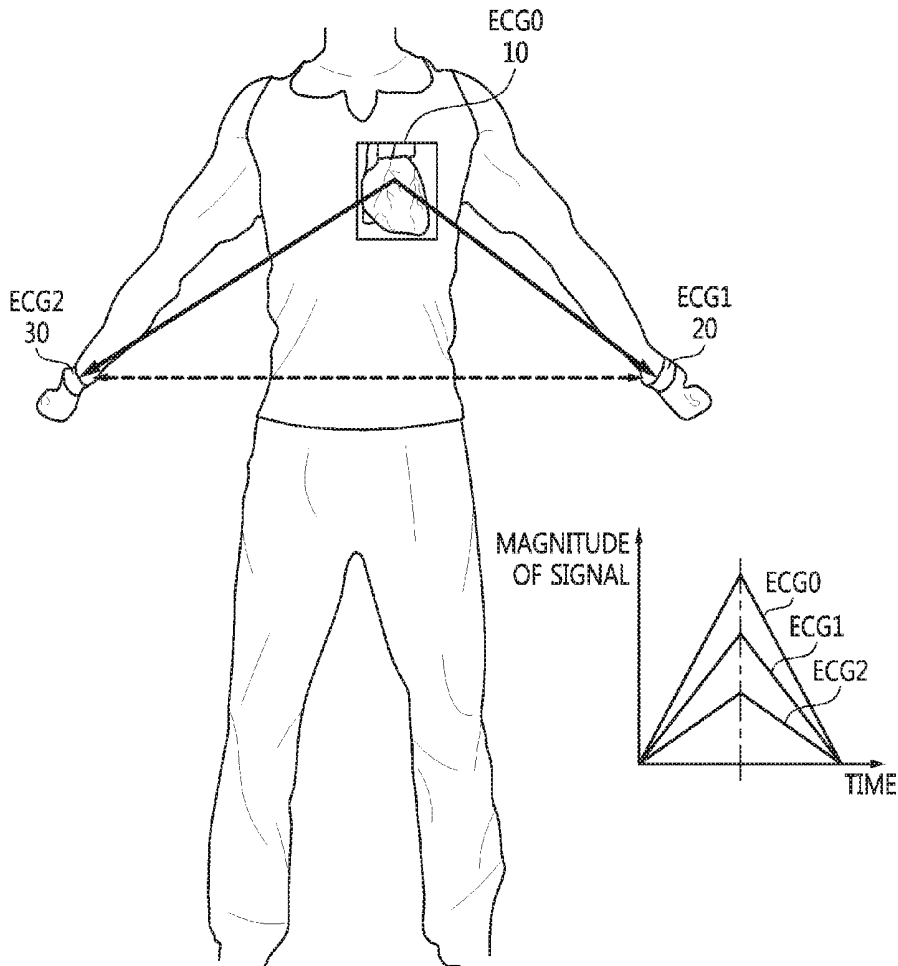


FIG. 1

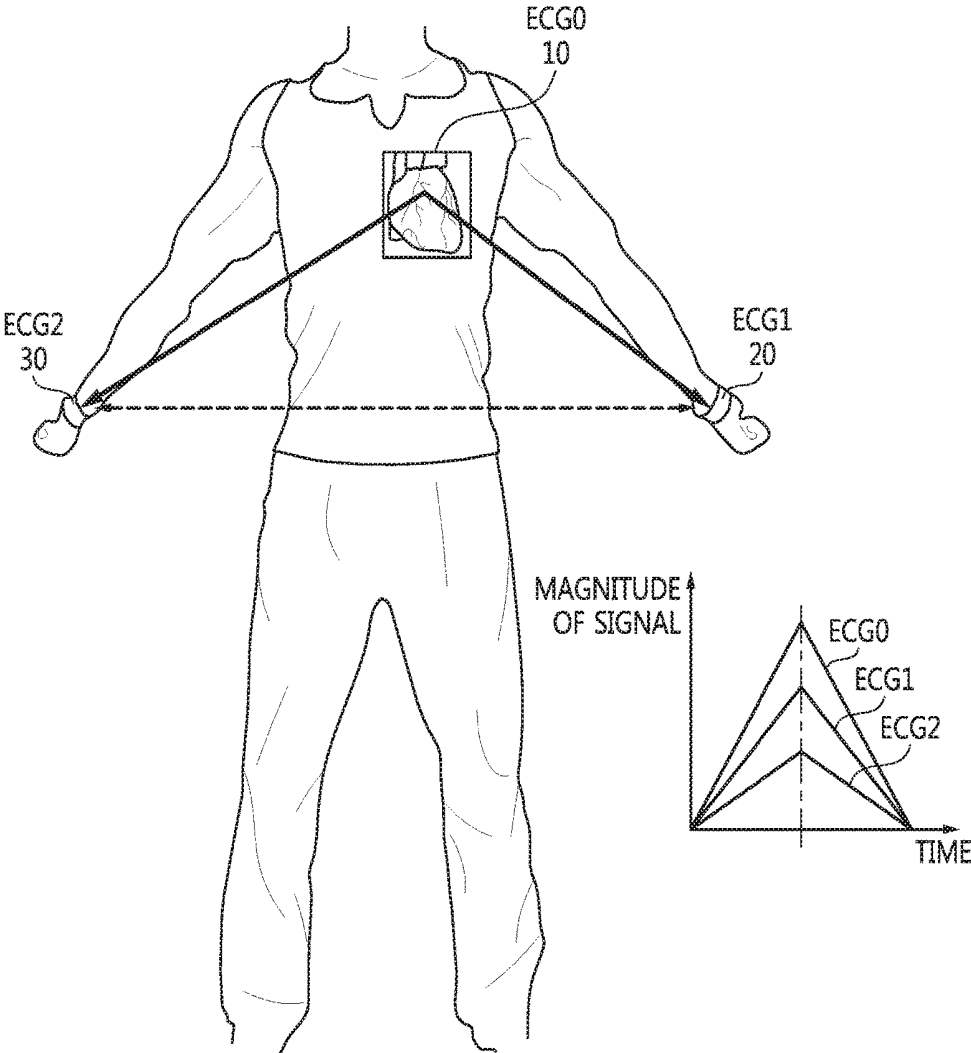


FIG. 2C

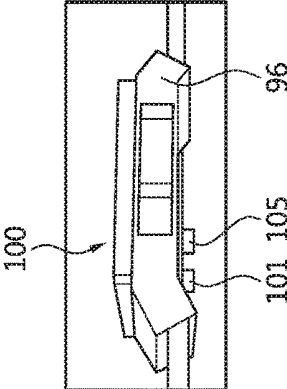


FIG. 2B

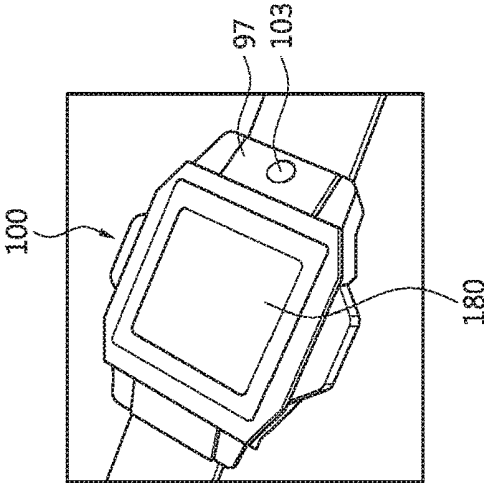


FIG. 2A

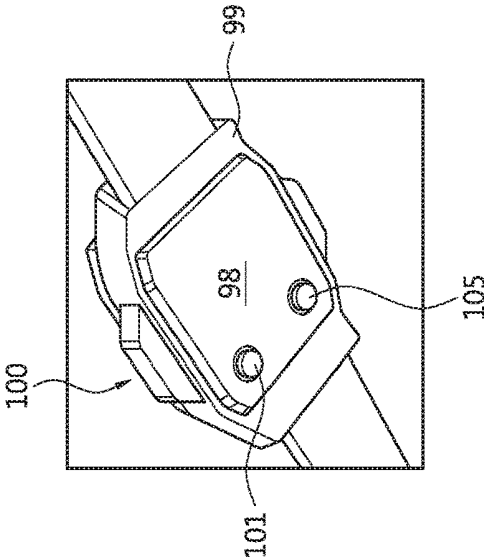


FIG. 3A

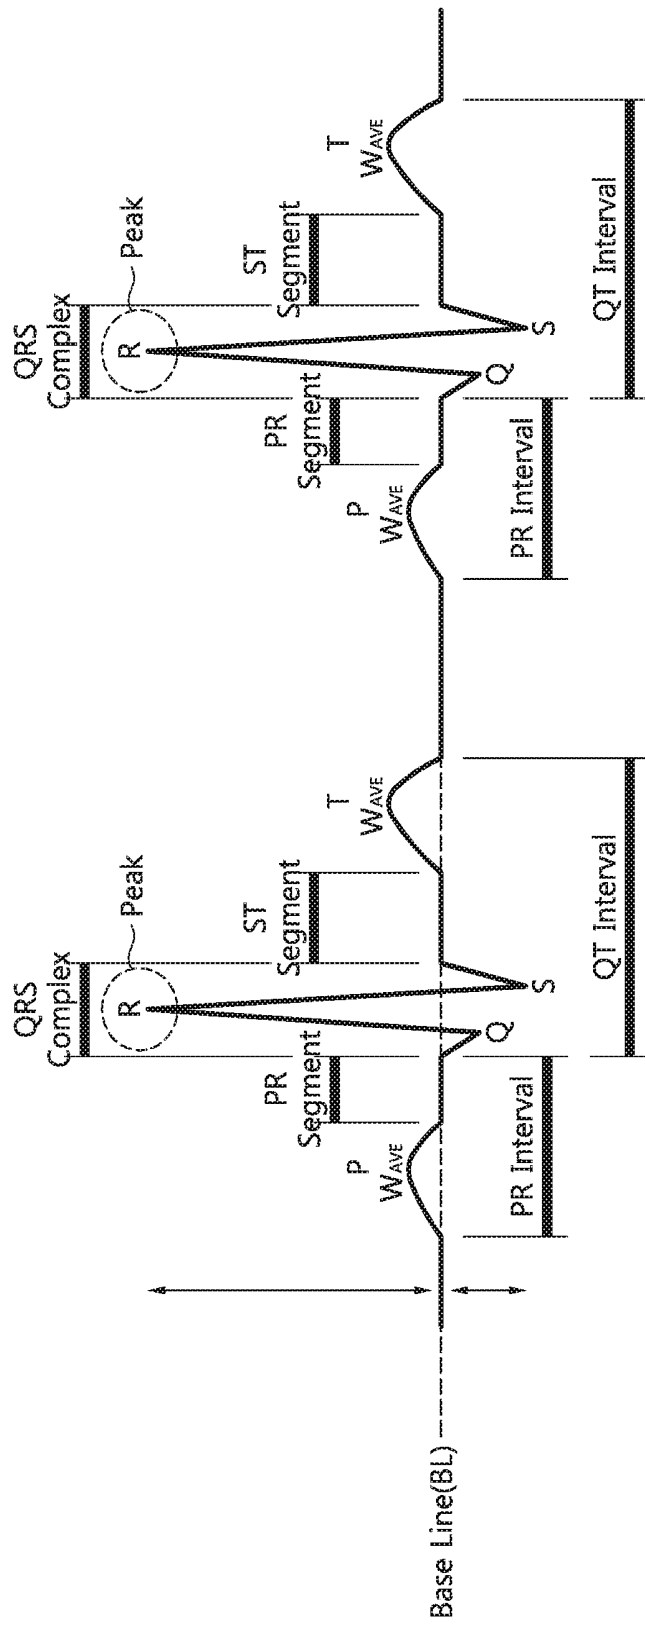


FIG. 3B

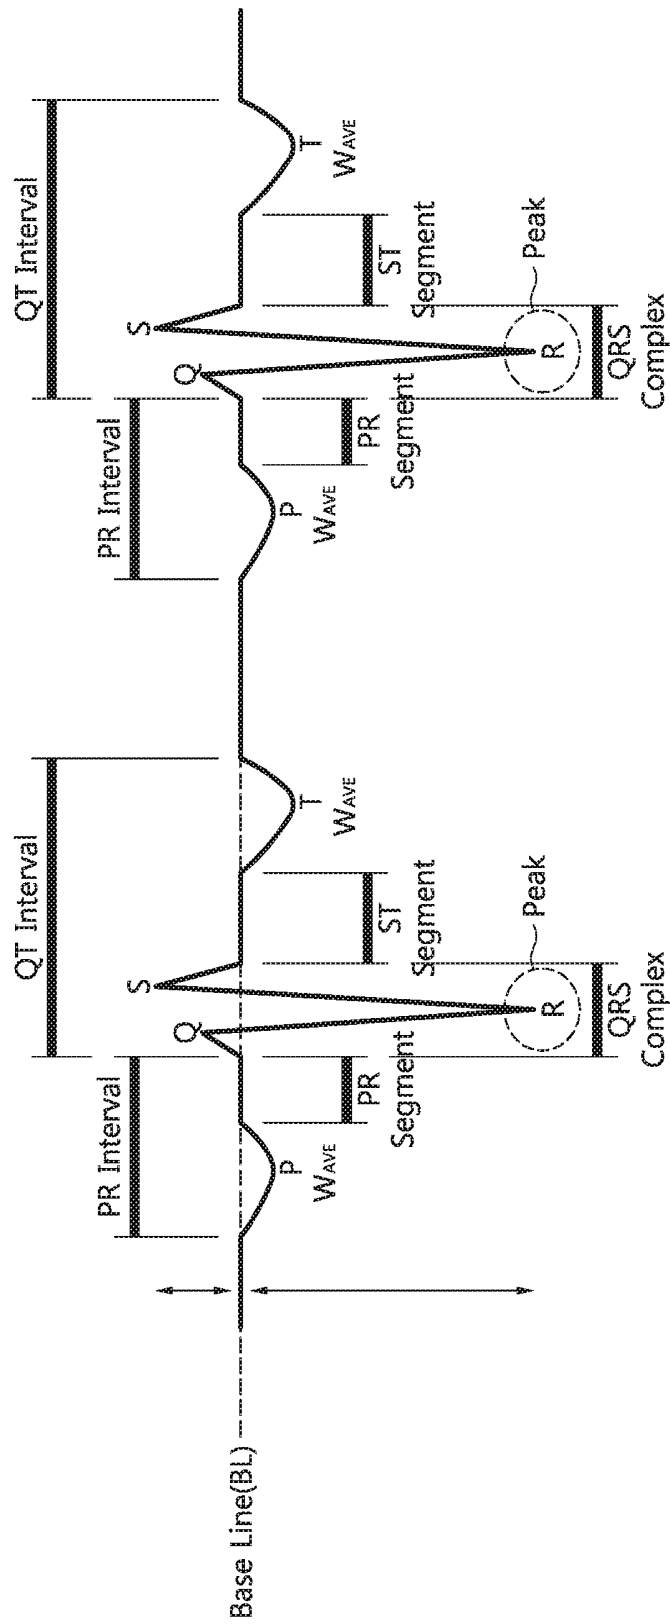


FIG. 4

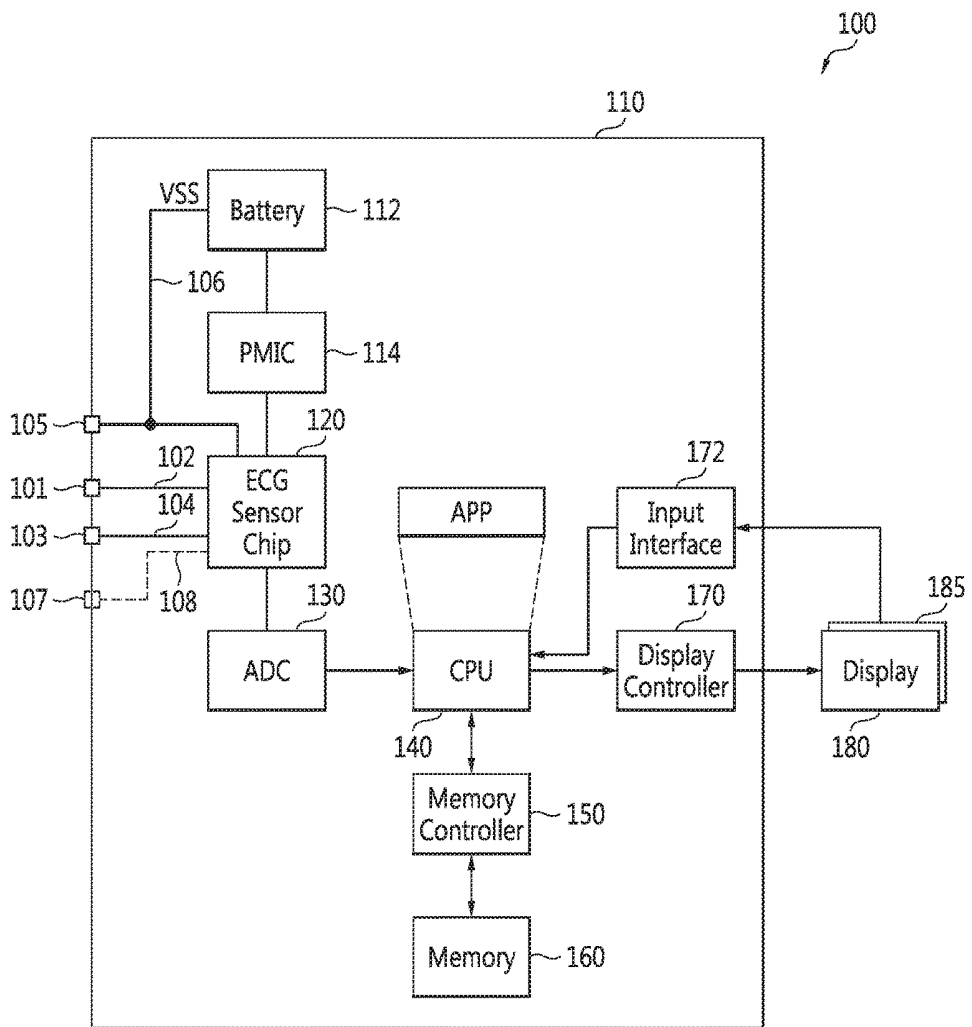


FIG. 5

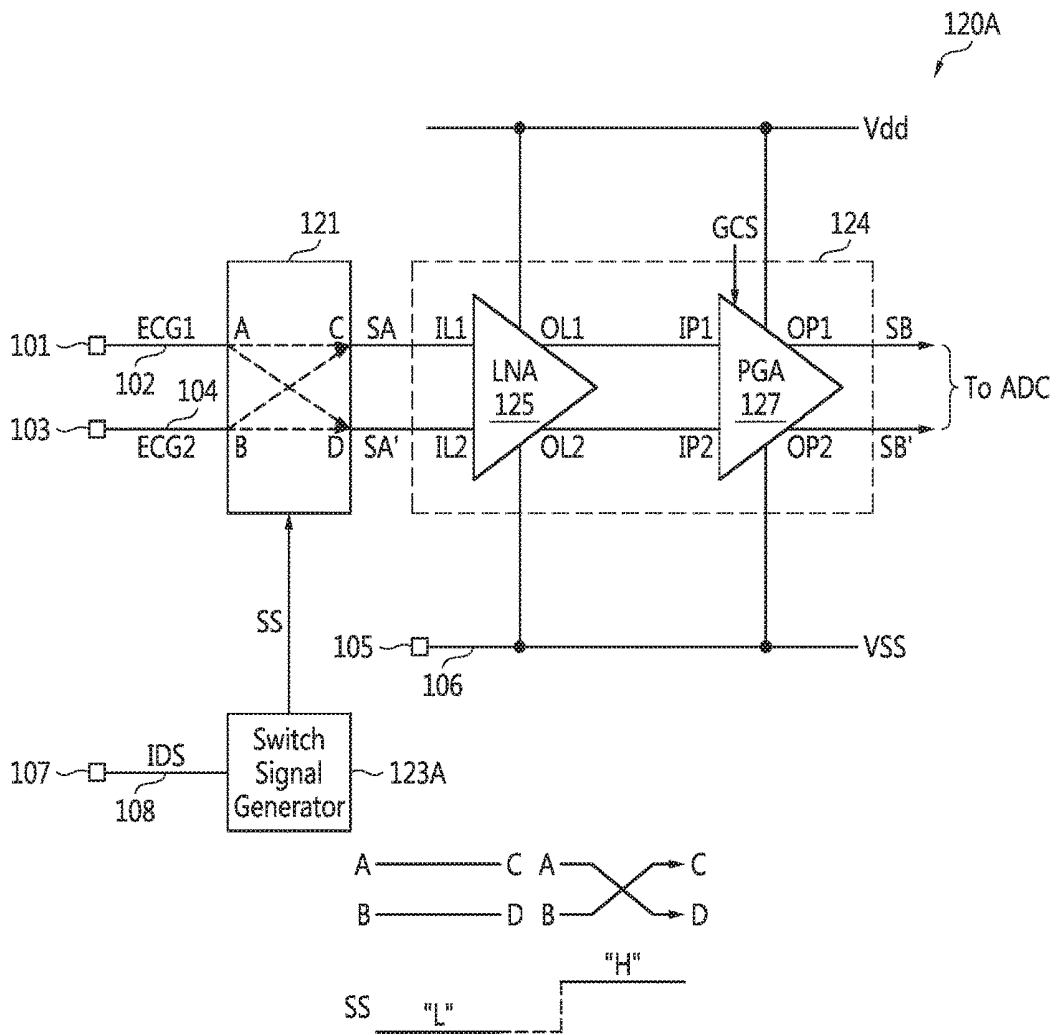


FIG. 6A

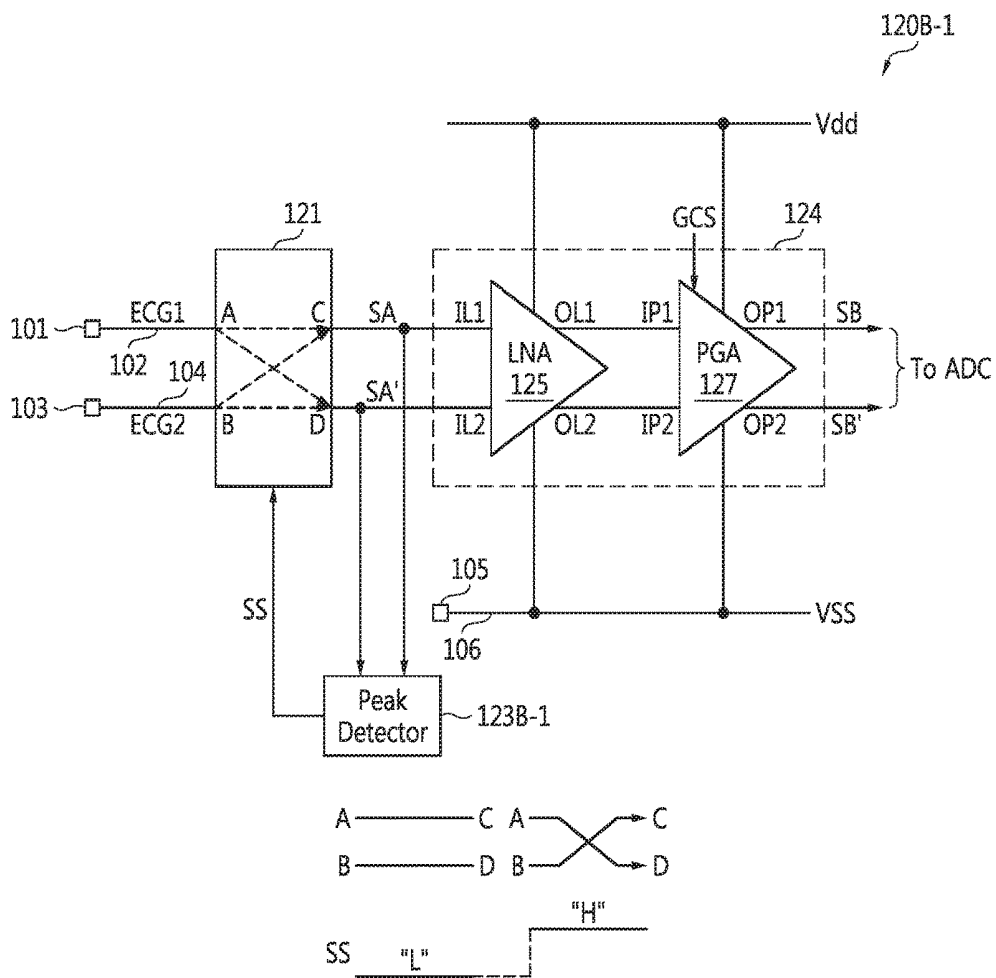


FIG. 6B

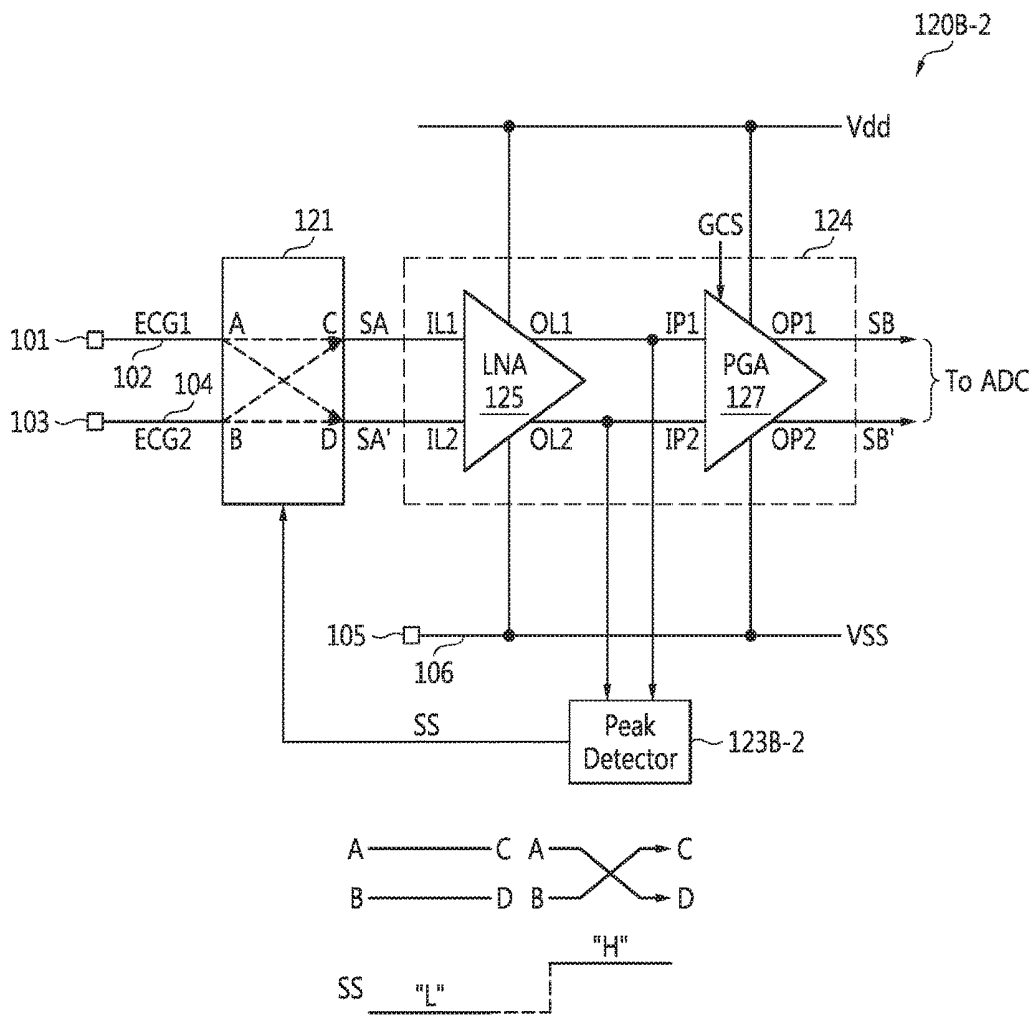


FIG. 6C

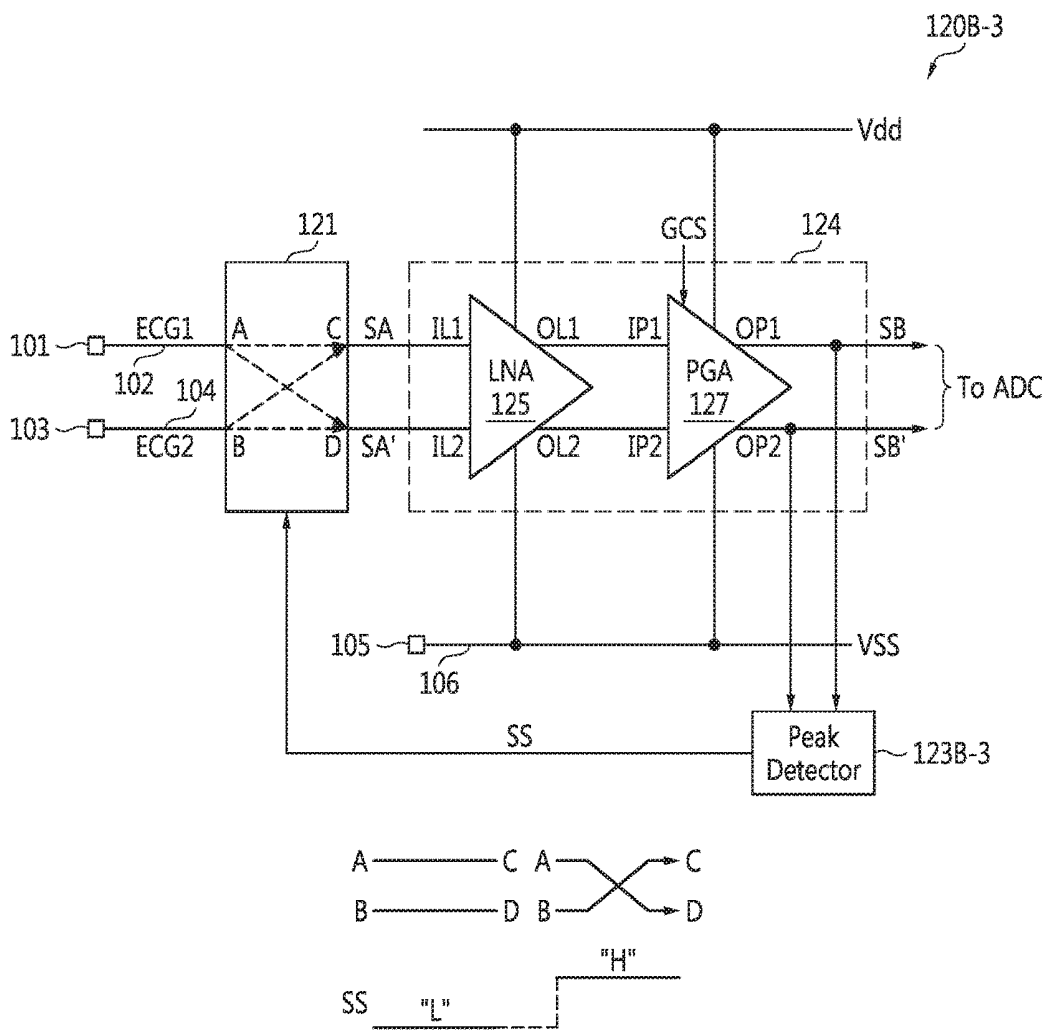


FIG. 7

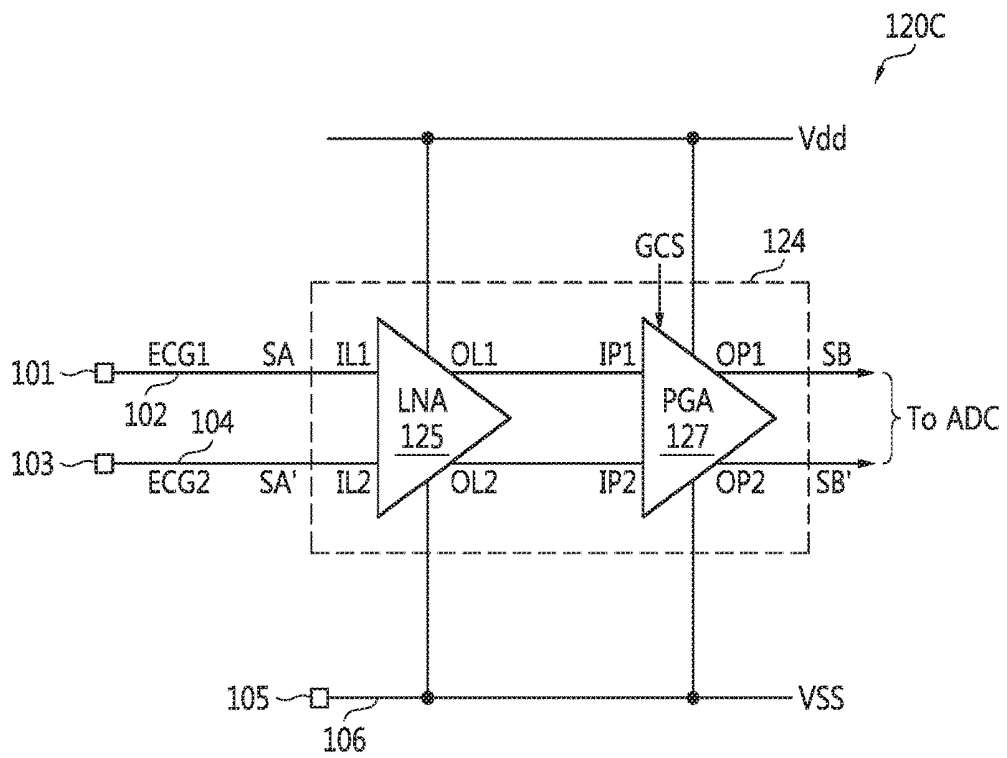


FIG. 8

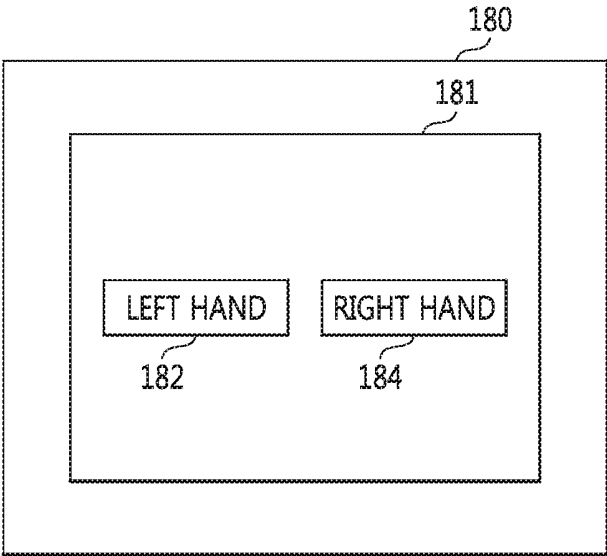


FIG. 9

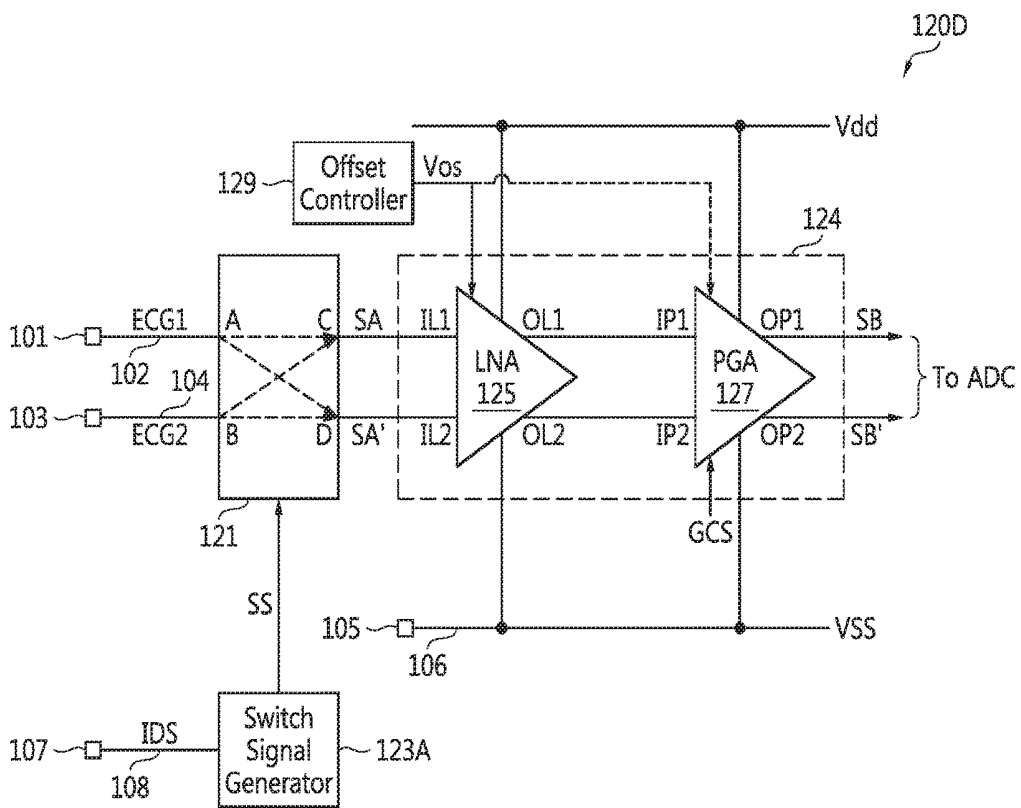


FIG. 10A

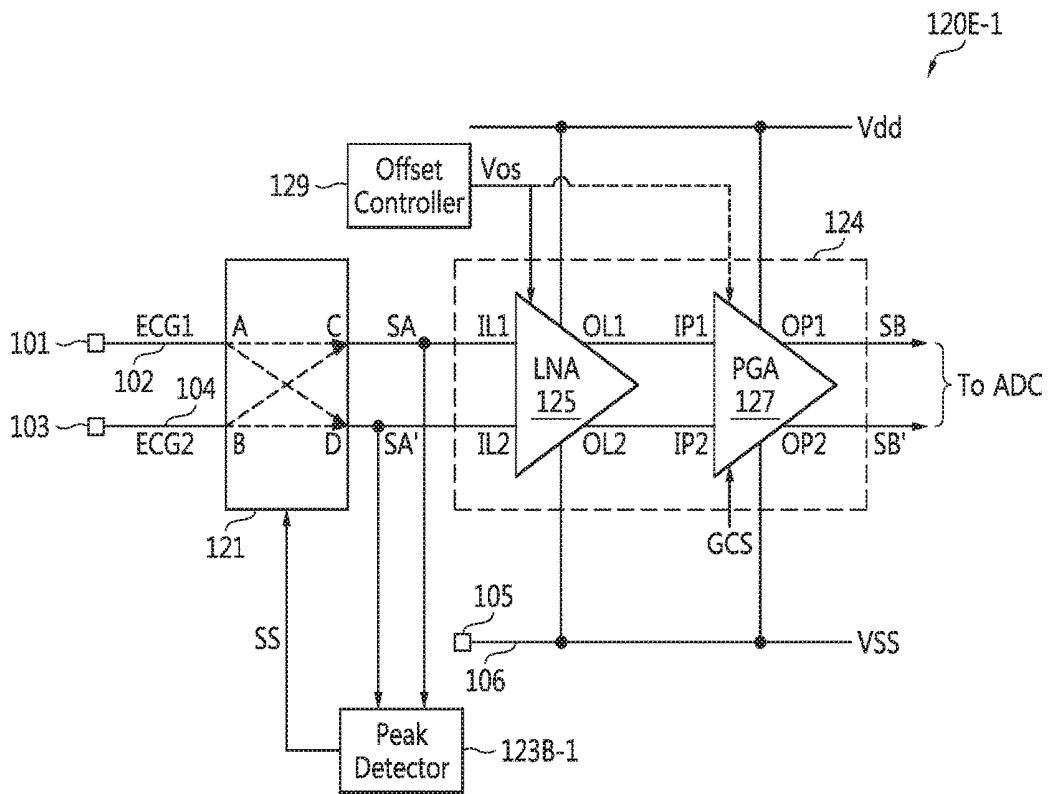


FIG. 10B

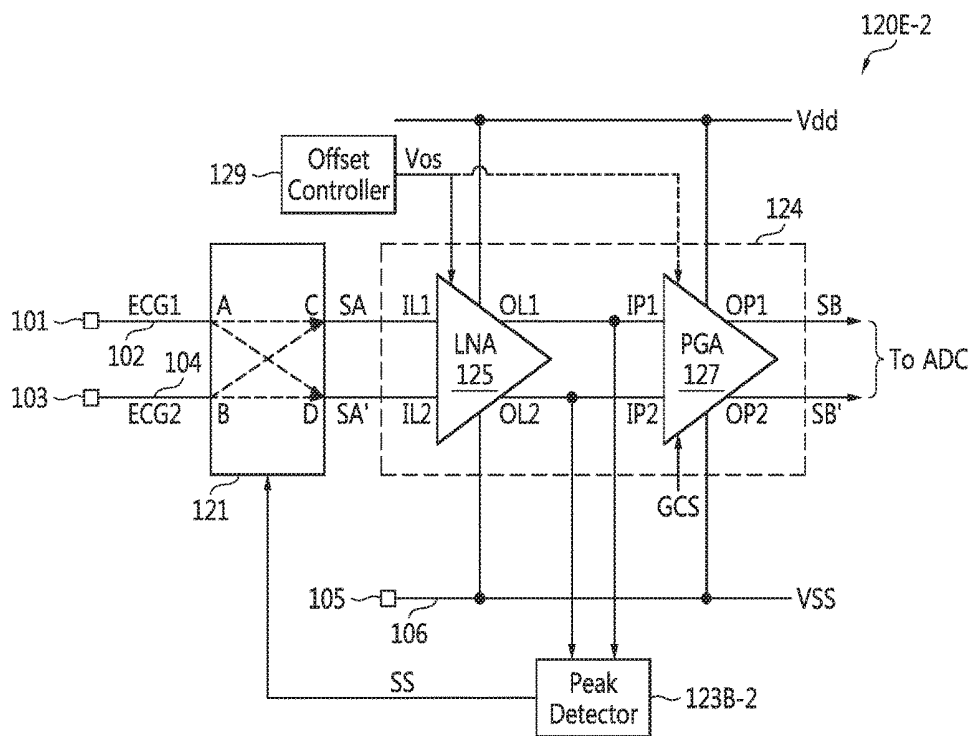


FIG. 10C

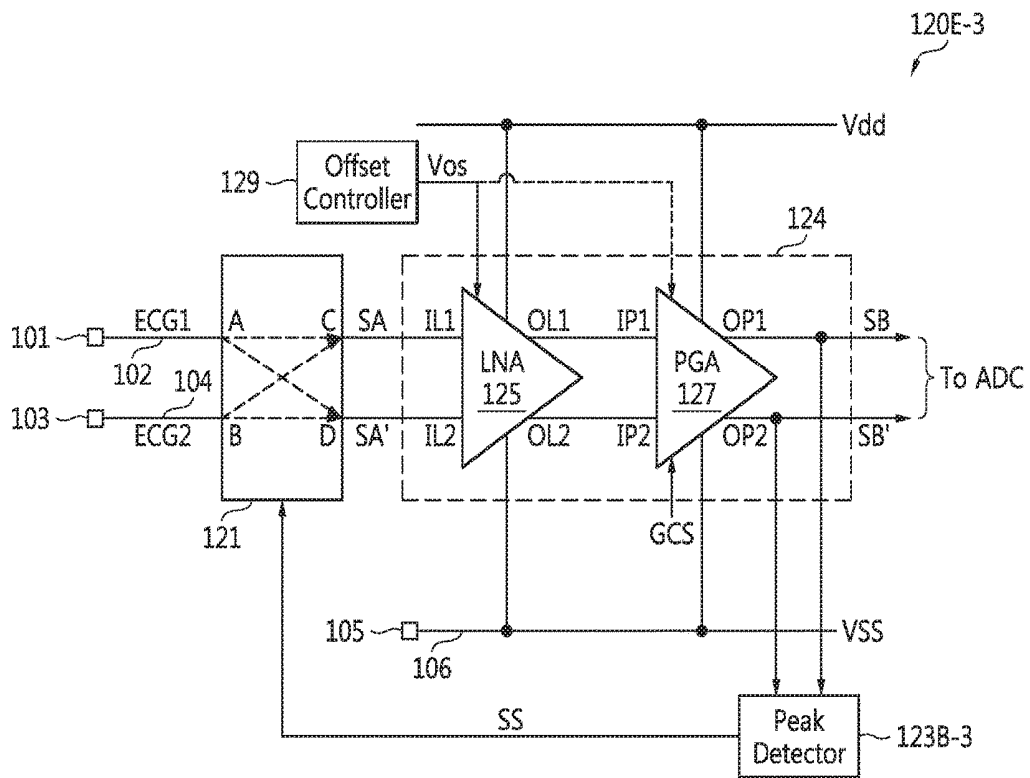


FIG. 11

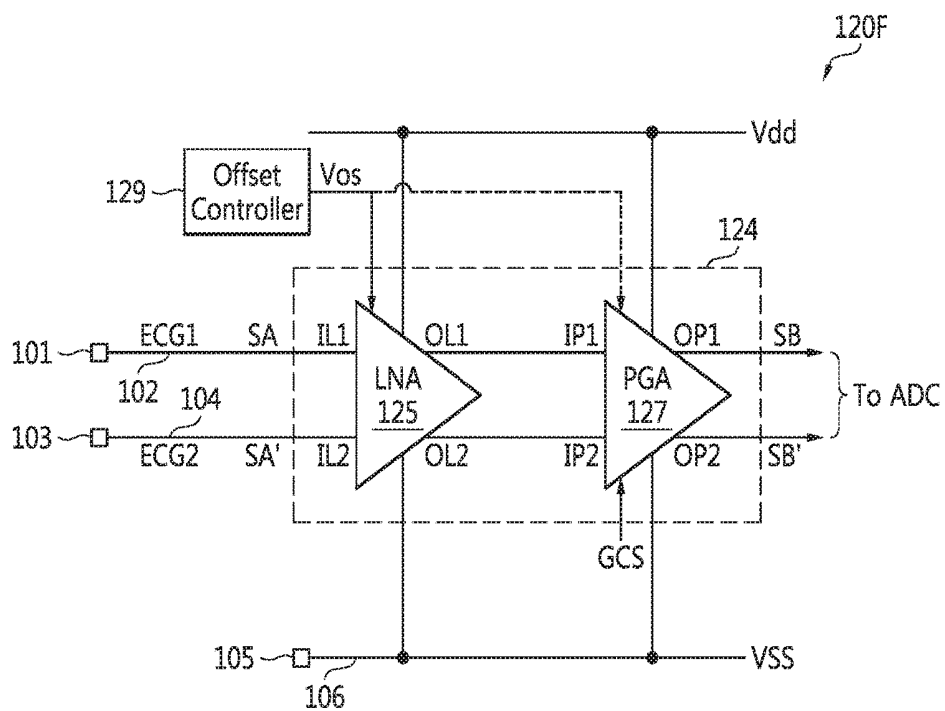


FIG. 12B

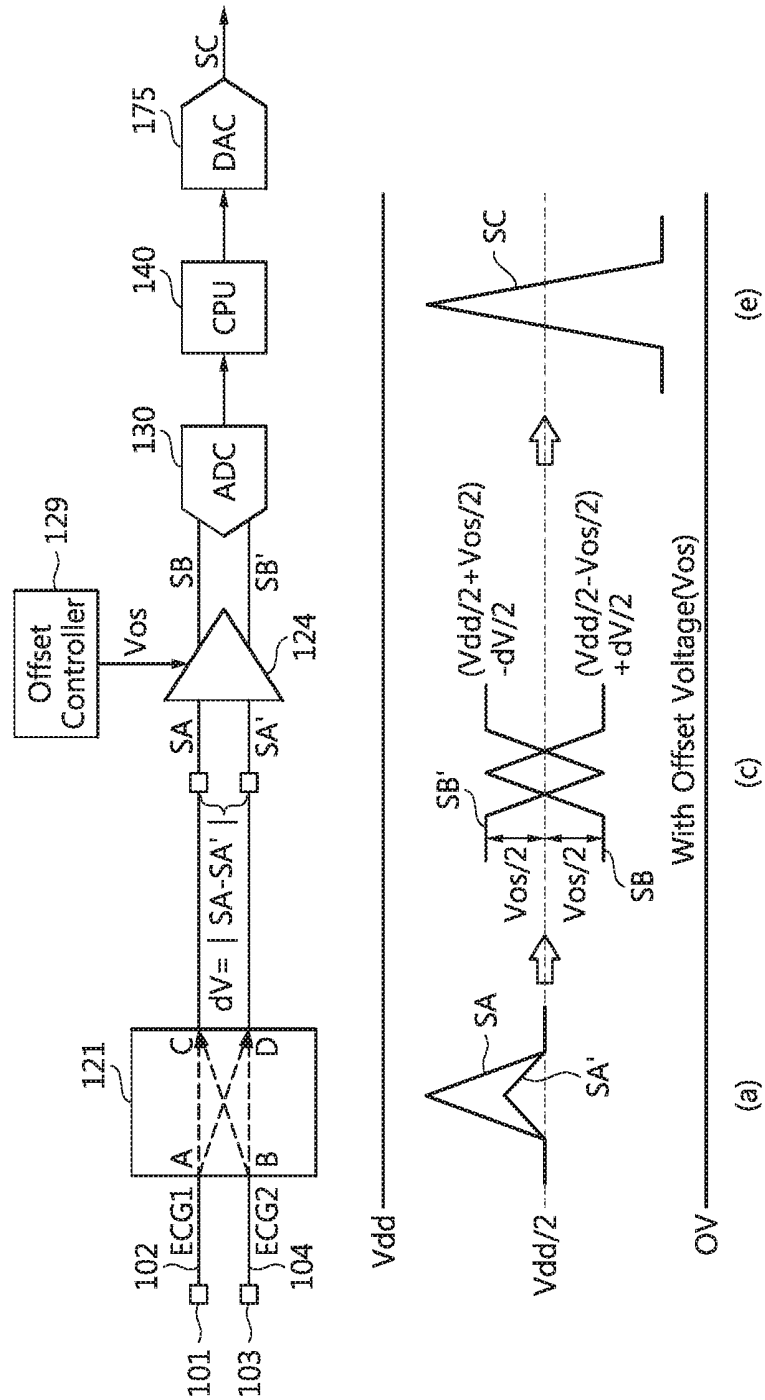


FIG. 13

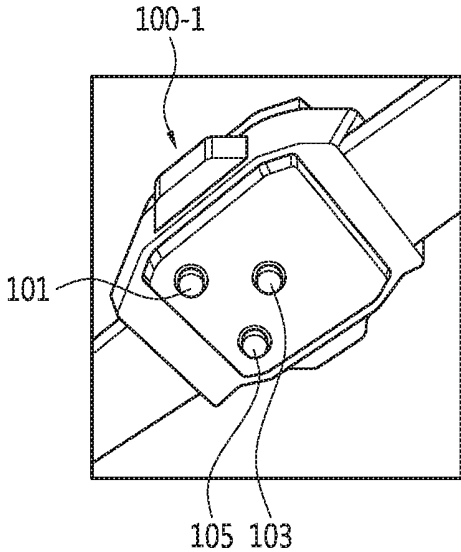


FIG. 14

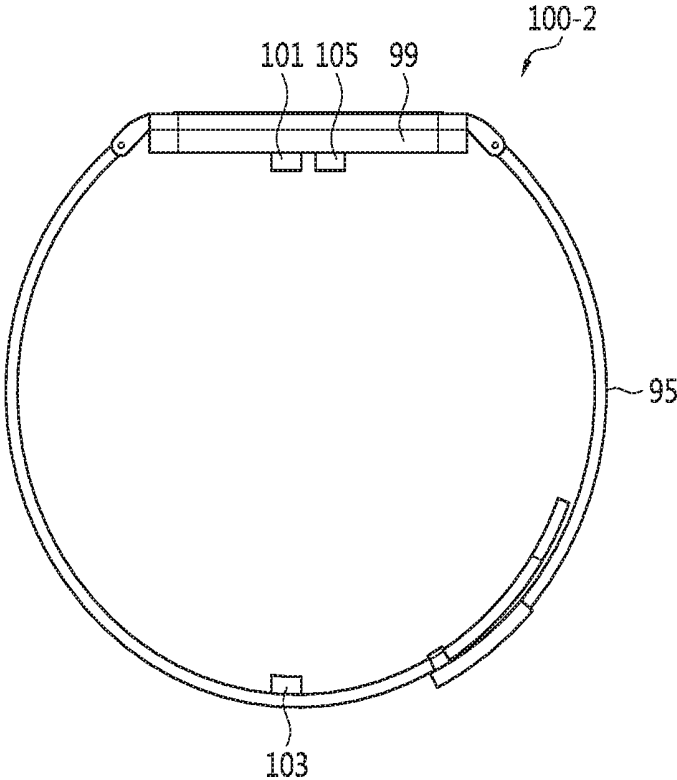


FIG. 15

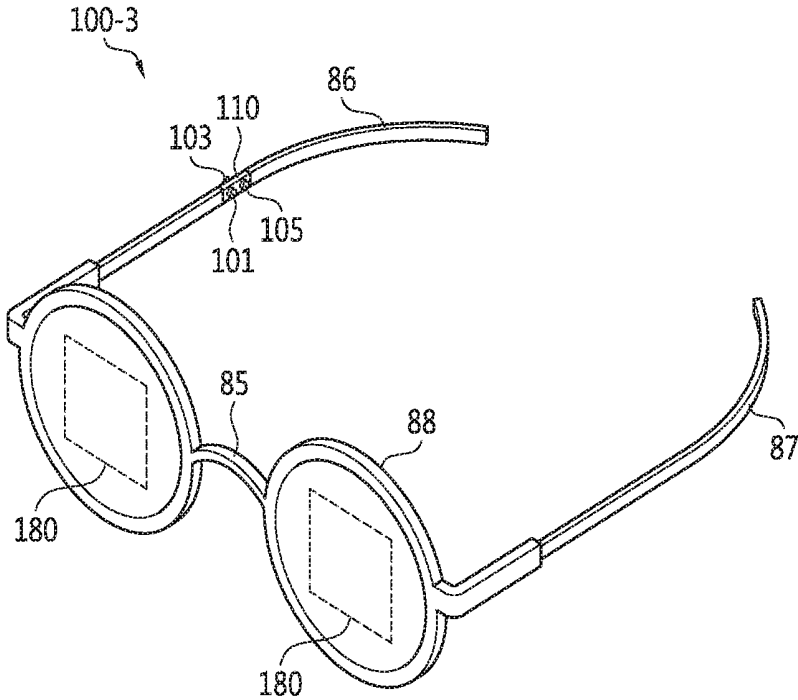


FIG. 16A

100-4

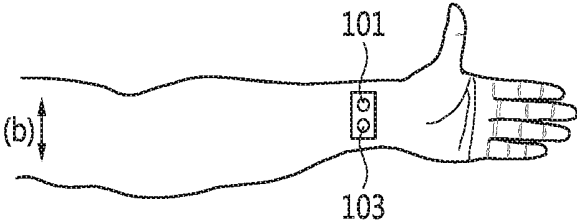


FIG. 16B

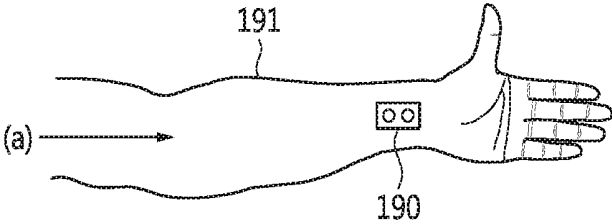


FIG. 17

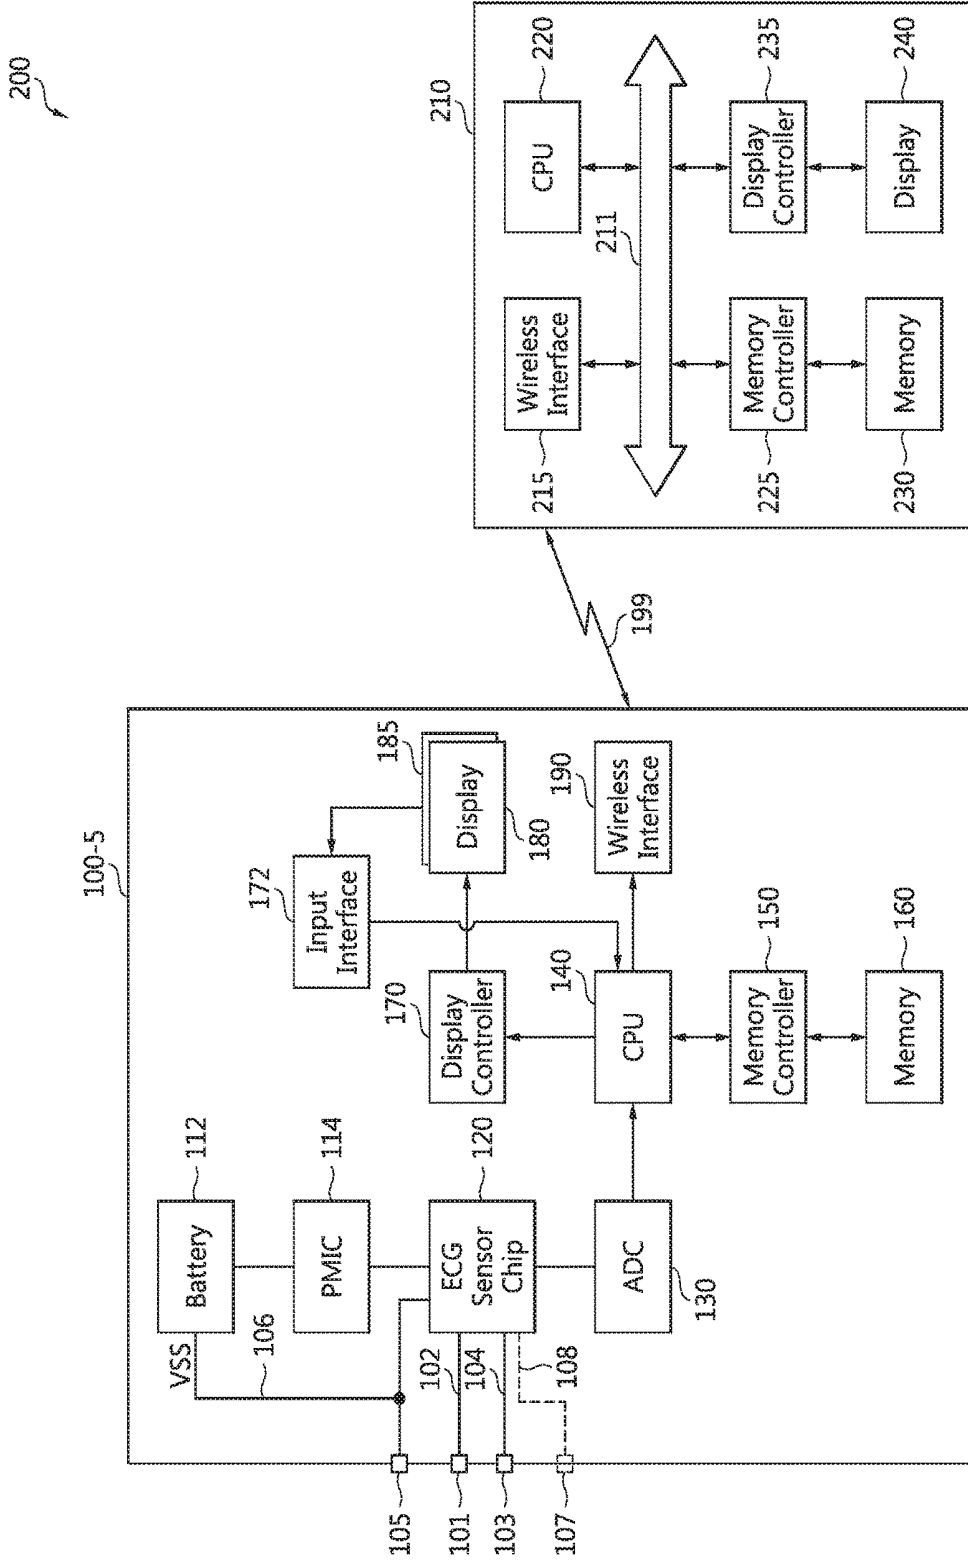


FIG. 18

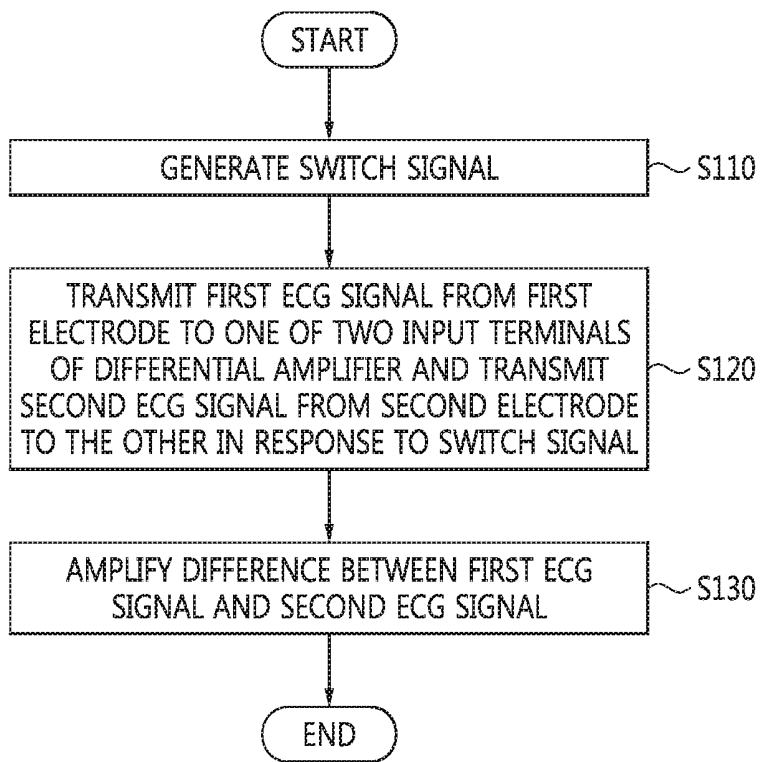


FIG. 19

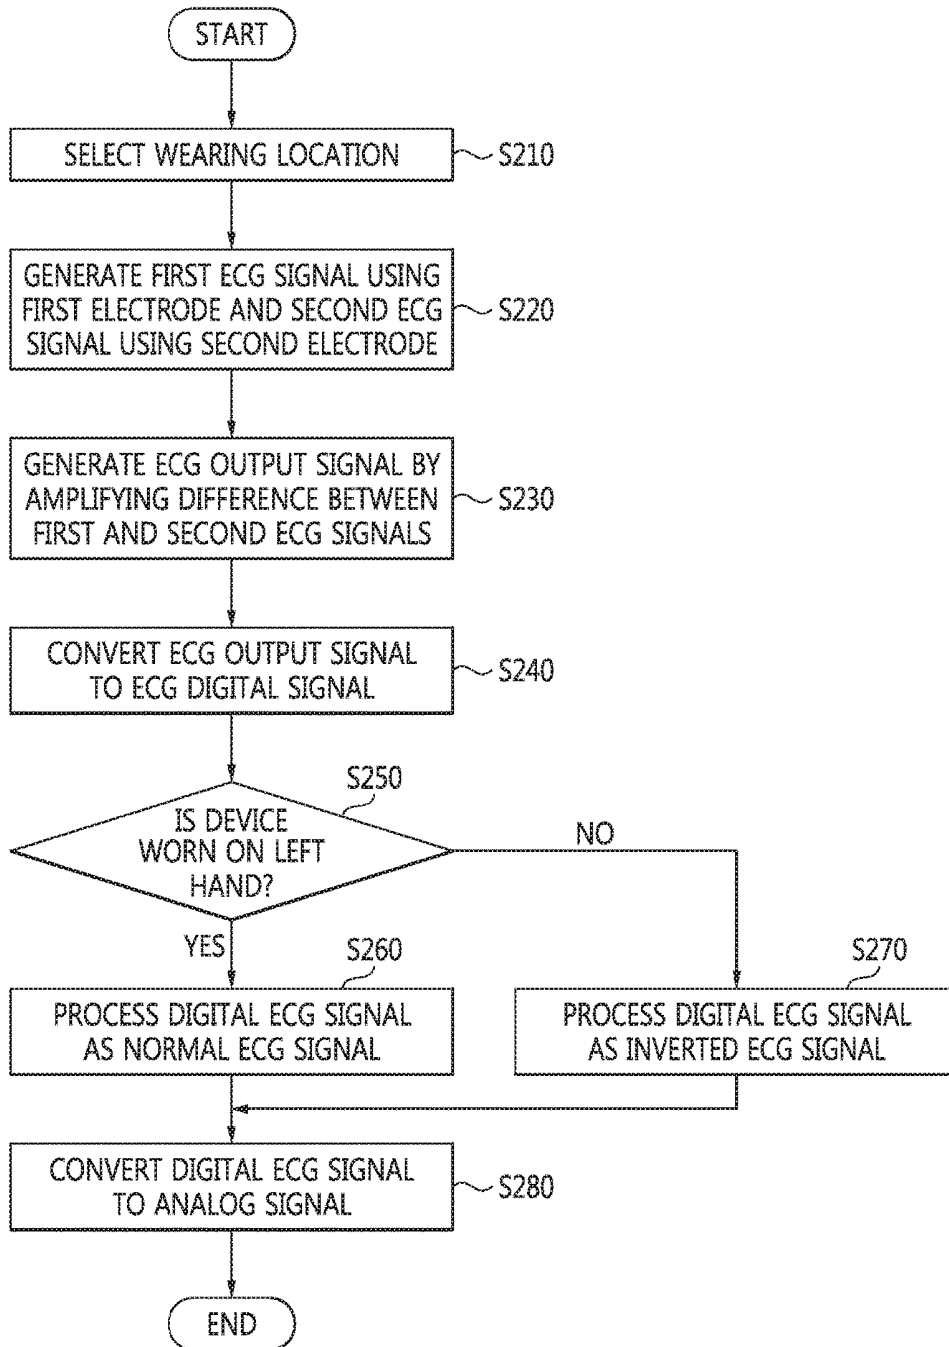


FIG. 20


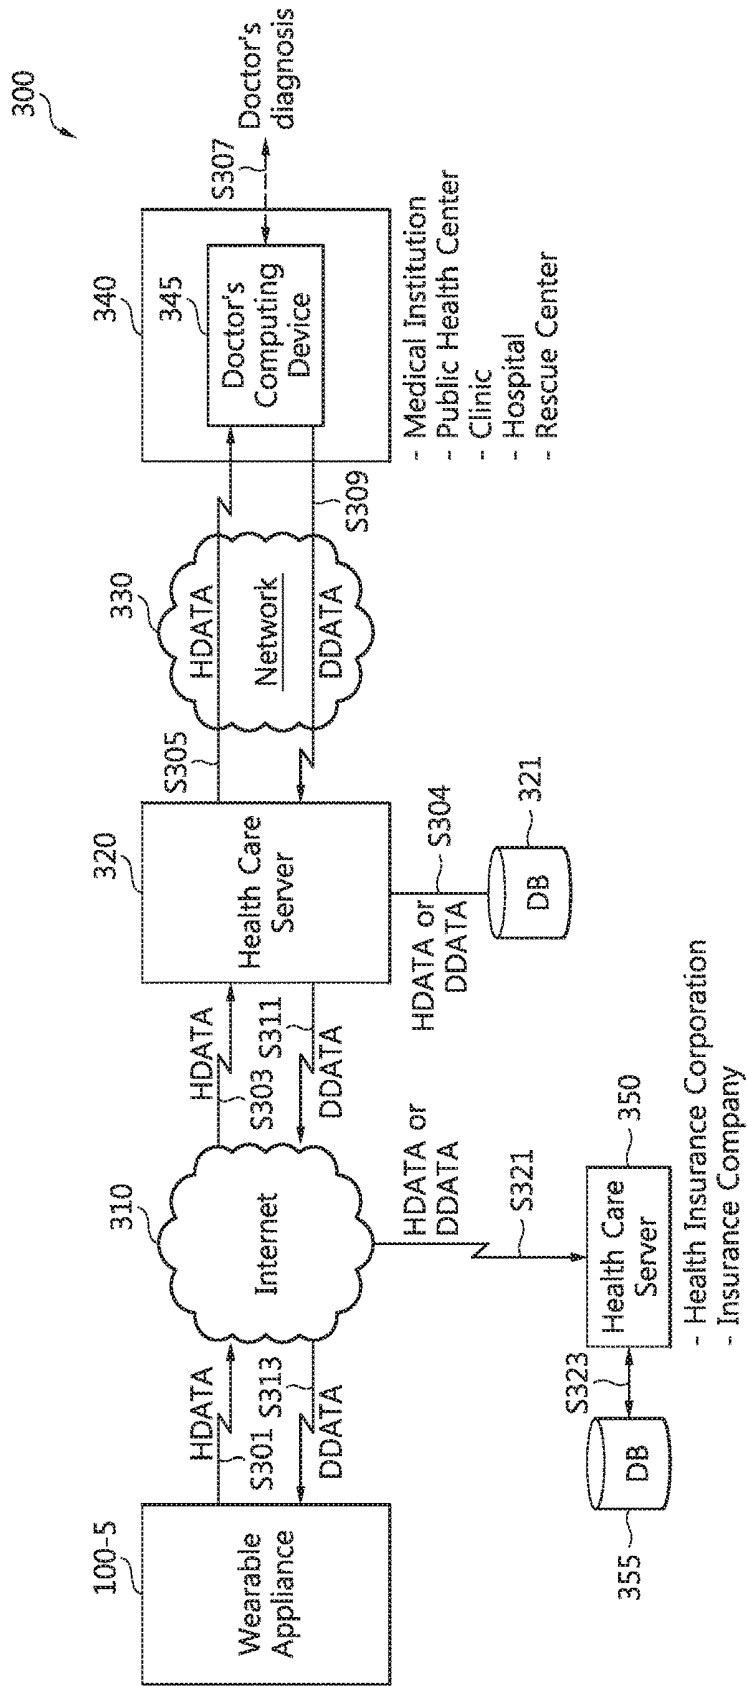


FIG. 21

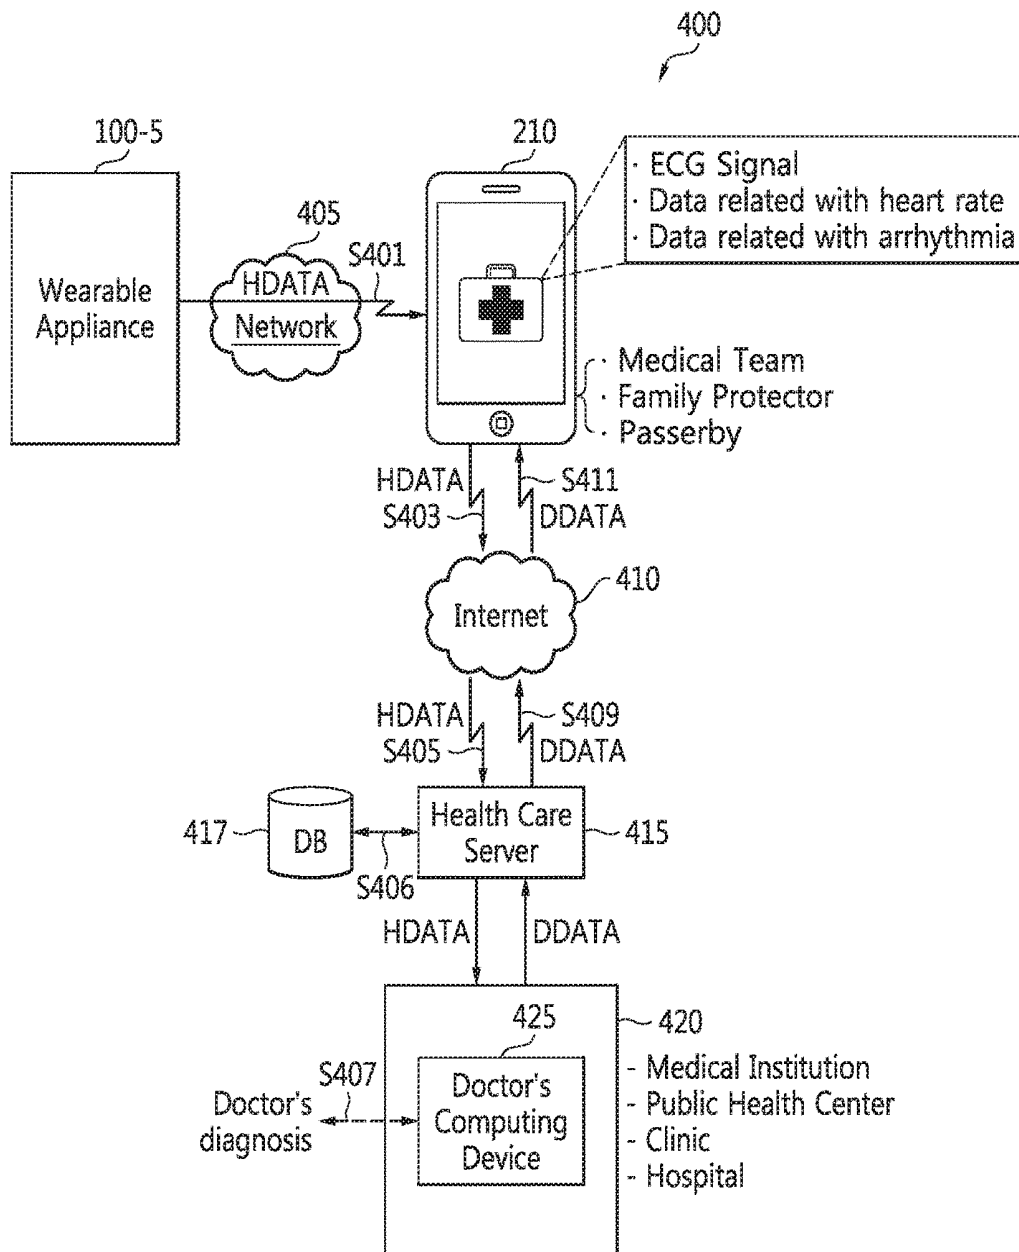

**ELECTROCARDIOGRAM (ECG) SENSOR
CHIP, SYSTEM ON CHIP (SOC), AND
WEARABLE APPLIANCE**

**CROSS REFERENCE TO RELATED
APPLICATION(S)**

[0001] This is a Divisional of U.S. application Ser. No. 14/840,154, filed Aug. 31, 2015, which claims priority under 35 U.S.C. 119 from Korean Patent Application No. 10-2014-0160011 filed on Nov. 17, 2014, the subject matter of which is hereby incorporated by reference.

BACKGROUND

[0002] Embodiments of the inventive concept relate generally to wearable electronic healthcare appliances and more particularly to electrocardiogram (ECG) sensor chips configured for use in wearable healthcare appliances, systems-on-chip incorporating such ECG sensor chips and related healthcare appliances.

[0003] Strong consumer demand for wearable healthcare appliances (hereafter, simply “appliances”) capable of monitoring and recording health conditions has followed a growing social emphasis on personal responsibility in health matters. With continued improvements in the miniaturization of electronics, consumers are now able to obtain small, portable devices capable of providing monitoring, recording, and/or displaying a number of health-related conditions. Many of these devices are “wearable” in the sense that they are conveniently configured for use in a manner that allows a user to comfortably wear the device for periods of time.

[0004] There are many different characteristics of a person’s body that—when properly monitored and interpreted—provide meaningful information regarding the overall health of the person. One important characteristic is the electrical signal(s) associated with operation of the heart. It is well recognized that the heart’s electrical activity may be monitored by a set of routine medical tests commonly referred to as an electrocardiogram (ECG).

[0005] An ECG may be administered for a variety of reasons including; checking on the overall activity of a heart, identifying the cause of unexplained chest pain like the pain commonly associated with heart attack, pericarditis and angina, identifying the cause certain symptoms commonly associated with heart disease such as shortness of breath, dizziness, fainting and heart palpitations, monitoring the effect of certain medicines on the heart, checking on the operation of mechanical devices implanted in the heart, and defining a health baseline to better monitor chronic health conditions such as high blood pressure, high cholesterol, cigarette smoking and diabetes.

[0006] The typical ECG is administered in a doctor’s office to a reclining patient by carefully attaching ten (10) electrical leads to designated locations on the patient’s body and thereafter recording a set of electrical signals over a period of time. While indisputably useful to medical professionals and harmless to the patient, the typical ECG is far from convenient.

[0007] More recently, improved techniques have allowed an ECG-like monitoring of heart-related bioelectrical signals using a wearable device instead of a clumsy set of electrical leads. In this manner, certain aspects of a person’s physical condition may be conveniently monitored over longer periods of time outside of a doctor’s office. However,

such portable devices have heretofore suffered from signal detection problems and significant constraints on acceptable wearable locations of such devices on a person’s body. That is, when conventional wearable devices capable of detecting an ECG-like signal are randomly positioned on a person’s body the diagnostic results are often disappointing.

SUMMARY

[0008] In one aspect, certain embodiments of the inventive concept provide an electrocardiogram (ECG) sensor chip configured for use in a wearable appliance and including; a switch controlled by a switching signal and including a first switch input that receives a first ECG signal, a second switch input that receives a second ECG signal, a first switch output, and a second switch output, an amplifier including a first amplifier input that receives one of the first ECG signal and the second ECG signal from the first switch output and a second amplifier input that receives the other one of the first ECG signal and the second ECG signal from the second switch output, and amplifies a difference between the first ECG signal and second ECG signal, and a location indicator that generates the switching signal in one of a first state and a second state, wherein in response to the first state of the switching signal, the switch passes the first ECG signal from the first switch input to the first switch output and passes the second ECG signal from the second switch input to the second switch output, and in response to the second state of the switching signal, the switch passes the first ECG signal from the first switch input to the second switch output and passes the second ECG signal from the second switch input to the first switch output.

[0009] In another aspect, certain embodiments of the inventive concept provide a system configured for use in a wearable appliance, the system including; an electrocardiogram (ECG) sensor chip that receives a first ECG signal from a first ECG sensor and a second ECG signal from a second ECG sensor, and includes an amplifier that amplifies a difference between the first ECG signal and second ECG signal to generate a first ECG output signal and a second ECG output signal, an analog-to-digital converter (ADC) that receives the first and second ECG output signals and generates corresponding ECG digital signals, and a processor that receives the ECG digital signals and processes the ECG digital signals in response to received location information indicating a location of the wearable appliance as worn by a user.

[0010] In another aspect, certain embodiments of the inventive concept provide a wearable appliance worn at a location on a user and including; a first electrocardiogram (ECG) electrode, a second ECG electrode, an ECG sensor chip that receives a first ECG signal from the first ECG electrode and a second ECG signal from the second ECG electrode, the ECG sensor chip comprising, a switch controlled by a switching signal and including a first switch input that receives the first ECG signal, a second switch input that receives the second ECG signal, a first switch output, and a second switch output, an amplifier including a first amplifier input that receives one of the first ECG signal and the second ECG signal from the first switch output and a second amplifier input that receives the other one of the first ECG signal and the second ECG signal from the second switch output, and generates an amplified difference signal between the first ECG signal and the second ECG signal, and a location indicator that generates the switching signal

in one of a first state and a second state, wherein in response to the first state of the switching signal, the switch passes the first ECG signal from the first switch input to the first switch output and passes the second ECG signal from the second switch input to the second switch output, and in response to the second state of the switching signal, the switch passes the first ECG signal from the first switch input to the second switch output and passes the second ECG signal from the second switch input to the first switch out.

[0011] In another aspect, certain embodiments of the inventive concept provide a system on a chip (SoC) including an electrocardiogram (ECG) sensor chip that includes; a switch controlled by a switching signal and including a first switch input that receives a first ECG signal from a first ECG sensor, a second switch input that receives a second ECG signal from a second ECG sensor, a first switch output, and a second switch output, an amplifier including a first amplifier input that receives one of the first ECG signal and the second ECG signal from the first switch output, and a second amplifier input that receives the other one of the first ECG signal and the second ECG signal from the second switch output and generates an amplified difference signal between the first ECG signal and the second ECG signal, and a location indicator that generates the switching signal having one of a first state and a second state, wherein in response to the switching signal having the first state, the switch passes the first ECG signal from the first switch input to the first switch output and passes the second ECG signal from the second switch input to the second switch output, and in response to the switching signal having the second state, the switch passes the first ECG signal from the first switch input to the second switch output and passes the second ECG signal from the second switch input to the first switch out, and an analog-to-digital converter (ADC) that receives the amplified difference signal and generates corresponding ECG digital signals, and a Central Processing Unit (CPU) that receives the ECG digital signals and generates display information that controls generation of a visual image on a display.

[0012] In another aspect, certain embodiments of the inventive concept provide a data processing system including; a wearable appliance including the ECG sensor chip, and a computing device configured to communicate information with the wearable appliance via at least one of a wireless connection and a hardwired connection. The wearable appliance includes; a first electrocardiogram (ECG) electrode, a second ECG electrode, and an ECG sensor chip that receives a first ECG signal from the first ECG electrode and a second ECG signal from the second ECG electrode, wherein the ECG sensor chip includes a switch controlled by a switching signal and including a first switch input that receives the first ECG signal, a second switch input that receives the second ECG signal, a first switch output, and a second switch output, an amplifier including a first amplifier input that receives one of the first ECG signal and the second ECG signal from the first switch output and a second amplifier input that receives the other one of the first ECG signal and the second ECG signal from the second switch output, and generates an amplified difference signal between the first ECG signal and the second ECG signal, and a location indicator that generates the switching signal in one of a first state and a second state, wherein in response to the first state of the switching signal, the switch passes the first ECG signal from the first switch input to the first switch

output and passes the second ECG signal from the second switch input to the second switch output, and in response to the second state of the switching signal, the switch passes the first ECG signal from the first switch input to the second switch output and passes the second ECG signal from the second switch input to the first switch out.

[0013] In another aspect, certain embodiments of the inventive concept provide a method of operating an electrocardiogram (ECG) sensor chip receiving a first ECG signal and a second ECG signal and being incorporated in a wearable appliance worn by a user, the method including; generating a switching signal, using the switching signal to control operation of a switch, wherein in response to the switching signal having a first state, the first ECG signal passes from a first switch input to a first switch output and the second ECG signal passes from a second switch input to a second switch output, else in response to the switching signal having a second state, the first ECG signal passes from the first switch input to the second switch output and the second ECG signal passes from the second switch input to the first switch output, and amplifying a difference between the first ECG signal and the second ECG signal using an amplifier connected to the first switch output and the second switch output.

BRIEF DESCRIPTION OF THE DRAWINGS

[0014] The above and other features and advantages of the inventive concept will become more apparent to those skilled in the art upon consideration of certain exemplary embodiments illustrated in the attached drawings, in which:

[0015] FIG. 1 is a conceptual diagram illustrating the capture of an electrocardiogram (ECG) signal according to embodiments of the inventive concept;

[0016] FIG. 2, inclusive of FIGS. 2A, 2B and 2C, is a perspective diagram illustrating in one example a wearable appliance capable of capturing an ECG signal according to embodiments of the inventive concept;

[0017] FIG. 3, inclusive of FIGS. 3A and 3B, is a set of comparative waveform diagrams further illustrating the capture of an ECG signal using a wearable appliance like the one shown in FIG. 2;

[0018] FIG. 4 is a block diagram illustrating a wearable appliance according to certain embodiments of the inventive concept;

[0019] FIGS. 5, 6A, 6B, 6C and 7 are respective circuit diagrams further illustrating in different examples the ECG sensor chip 120 of FIG. 4;

[0020] FIG. 8 is a diagram illustrating a graphical user interface (GUI) that may be displayed by a display incorporated in a wearable appliance according to certain embodiments of the inventive concept;

[0021] FIGS. 9, 10A, 10B, 10C and 11 are respective circuit diagrams further illustrating in different examples the ECG sensor chip 120 of FIG. 4.

[0022] FIGS. 12A and 12B are conceptual diagrams illustrating the use of voltage offsets in the capture and amplification of an ECG signal according to certain embodiments of the inventive concept;

[0023] FIGS. 13, 14, 15, 16A and 16B are respective, perspective diagrams variously illustrating in different examples certain wearable appliances capable of capturing an ECG signal according to embodiments of the inventive concept;

[0024] FIG. 17 is a block diagram of a data processing system including a wearable appliance including an ECG sensor chip according to embodiments of the inventive concept;

[0025] FIG. 18 is a flowchart generally summarizing a method of operating an ECG sensor chip according to embodiments of the inventive concept;

[0026] FIG. 19 is a flowchart summarizing a method of selectively operating a wearable appliance according to embodiments of the inventive concept; and

[0027] FIGS. 20 and 21 are respective block diagrams of data processing systems including a wearable appliance including the ECG sensor chip according to certain embodiments of the inventive concept.

DETAILED DESCRIPTION

[0028] Certain embodiments of the inventive concept will now be described in some additional detail with reference to the accompanying drawings. This inventive concept may, however, be embodied in many different forms and should not be construed as being limited only the illustrated embodiments. Rather, these embodiments are provided so that this disclosure will be thorough and complete, and will fully convey the scope of the invention to those skilled in the art. Throughout the written description and drawings, like reference numbers and labels are used to denote like or similar elements.

[0029] It will be understood that when an element is referred to as being “connected” or “coupled” to another element, it can be directly connected or coupled to the other element or intervening elements may be present. In contrast, when an element is referred to as being “directly connected” or “directly coupled” to another element, there are no intervening elements present. As used herein, the term “and/or” includes any and all combinations of one or more of the associated listed items and may be abbreviated as “/”.

[0030] It will be understood that, although the terms first, second, etc. may be used herein to describe various elements, these elements should not be limited by these terms. These terms are only used to distinguish one element from another. For example, a first signal could be termed a second signal, and, similarly, a second signal could be termed a first signal without departing from the teachings of the disclosure.

[0031] The terminology used herein is for the purpose of describing particular embodiments only and is not intended to be limiting of the invention. As used herein, the singular forms “a”, “an” and “the” are intended to include the plural forms as well, unless the context clearly indicates otherwise. It will be further understood that the terms “comprises” and/or “comprising,” or “includes” and/or “including” when used in this specification, specify the presence of stated features, regions, integers, steps, operations, elements, and/or components, but do not preclude the presence or addition of one or more other features, regions, integers, steps, operations, elements, components, and/or groups thereof.

[0032] Unless otherwise defined, all terms (including technical and scientific terms) used herein have the same meaning as commonly understood by one of ordinary skill in the art to which this invention belongs. It will be further understood that terms, such as those defined in commonly used dictionaries, should be interpreted as having a meaning that is consistent with their meaning in the context of the

relevant art and/or the present application, and will not be interpreted in an idealized or overly formal sense unless expressly so defined herein.

[0033] The term “wearable appliance” is used hereafter to denote a broad class of user-wearable electronic devices that may be used to detect, capture, monitor and/or record one or more bioelectrical signal(s) associated with the user’s body. Wearable appliances will have variety of configurations variously appropriate to different applications and dispositions on the user’s body. Certain wearable appliances consistent with the inventive concept will be publicly apparent when worn by a user and will be readily recognizable as common fashion accessories such as a watches, rings, bracelets, anklets, necklaces, headphones, hats, eye glasses, etc. In this regard, certain embodiments of the inventive concept may be physically incorporated within common electrical devices capable of performing their normal function(s), like watches that tell time and headphones that provide audio signals, for example. Other wearable appliances consistent with the inventive concept will be incorporated within articles of clothing such as neckties, wristbands, headbands, shirts, undershirts, bras, etc. Still other wearable appliances consistent with the inventive concept will be more appropriately worn underneath clothing and may take the form of skin-adhering patches of various sizes, shapes and compositions.

[0034] (FIG.) 1 is a conceptual diagram illustrating the capture of a bioelectrical signal associated with the operation of a user’s heart. As noted above, this type of signal is routinely captured by an electrocardiogram (ECG) test. Thus, for purposes of the description that follows, this type of signal—in all of its variations and manifestations within the human body and in all of its electrically captureable forms, whether singularly or as a combination—will hereafter be generally referred to as an “ECG signal”. Accordingly, in

[0035] FIG. 1 the capture of an ECG signal is illustrated. In this context, the term “capture” refers to any process that identifies, detects, acquires and/or measures an ECG signal sufficient to generate at least one analog signal, or corresponding digital data, that accurately represents the electrical activity of the user’s heart as manifested by an ECG signal.

[0036] Under the foregoing definition, a user will only produce a single ECG signal associated with the activity of his/her heart. However, the ECG signal will be differently manifested and differently captured at different locations on the user’s body. Ideally, an ECG signal would be captured by one or more ECG sensors placed on appropriate locations directly proximate the user’s heart (e.g., a first location 10 in FIG. 1 capturing a first ECG signal ECG0). Unfortunately, while the first location 10 centered over the user’s heart provides the strongest (i.e., highest differential amplitude) ECG signal, it is not necessarily convenient and the disposition of sensors at this location may be uncomfortable to the user during physical exercise. Accordingly, it is often highly desirable for the user of a wearable appliance to be able to place the constituent ECG sensors on a more convenient location of his/her body, such as a wrist.

[0037] This dispositional flexibility is one feature sadly lacking in many conventional devices. Such conventional devices routinely mandate an exact disposition location and any departure from this location greatly impairs an accurate ECG signal capture. In contrast, wearable appliances

according to the inventive concept recognize that an ECG signal will be differently manifested when captured at different locations on a user's body. However, wearable appliances according to the inventive concept nonetheless provide a user with the flexibility of wear the wearable appliance at a location deemed most comfortable or most convenient to the user.

[0038] For example with reference to FIG. 1, certain aspects of the inventive concept recognize that a second ECG signal (ECG1) apparent at a second location 20 (i.e., the user's left wrist) will be less strong than the first ECG signal (ECG0) at the first location 10, and that a third ECG signal (ECG2) apparent at a third location 30 (i.e., the user's right wrist) will be less strong than the second ECG signal (ECG1). That is, the inventive concept recognizes that increasing the distance between an ECG signal capture location on a user's body and the user's heart tends to decrease the input signal-to-noise ratio (SNR) of the captured ECG signal. Nonetheless, embodiments of the inventive concept are configured in such a manner that allow a user to reasonably wear a wearable appliance at multiple desirable locations on his/her body.

[0039] FIG. 2, inclusive of FIGS. 2A, 2B and 2C, is a set of perspective diagrams illustrating a wearable appliance 100 capable of capturing and processing an ECG signal according to certain embodiments of the inventive concept. Although the wearable appliance 100 shown in FIG. 2 is a watch, those of ordinary skill in the art will recognize that this is merely one convenient example, and wearable appliances consistent with the inventive concept may take many different forms.

[0040] The wearable appliance 100 of FIG. 2 comprises a watch body 99 housing circuitry and/or software used to implement the functionality of the wearable appliance 100, as well as circuitry and/or software used to provide typical watch functionality. A first ECG electrode 101 and a ground electrode 105 protrude from a bottom surface 98 of the watch body 99. When normally worn by a user at a desired location, such as a left or right wrist, the bottom surface 98 of the watch body 99. Hence, the protruding first ECG electrode 101 and ground electrode 105 are placed in direct contact with the user's skin when the wearable appliance 100 is worn by the user. This direct skin contact is highly beneficial to the capture of an ECG signal by the watch 100. In contrast, a second ECG electrode 103 may be disposed on a top surface 97 of the watch body 99 opposing the bottom surface 98. Alternately, the second ECG electrode 103 may be disposed on a side surface 96 of the watch body 99. When normally worn by a user, the top surface 97 and side surfaces 96 of the watch body 99, along with the second ECG electrode 103 are readily accessible to the user. In the embodiment illustrated in FIG. 2, the first ECG electrode 101 may be designated a positive electrode, and the second ECG electrode 103 may be designated a negative electrode.

[0041] In this context, the term "ECG sensor" refers to any one of a number of different bioelectrical, electro-mechanical, and/or electrical components capable of capturing an ECG signal when placed proximate to or directly in contact with the user's body.

[0042] Although in FIG. 2, the ground electrode 105 is disposed on the bottom surface 98 of the body 99 proximate the first ECG electrode 101, other embodiments of the inventive concept may differently place the ground electrode 105, or completely omit it. However, the use of the ground

electrode 105 may significantly aid in ECG signal synchronization between the wearable appliance 100 and the user. That is, use of the ground electrode 105 prevents floating of the ECG signal during capture of the ECG signal by an ECG sensor chip included in the wearable appliance 100. As a result, the combination of various ECG sensors and the ECG sensor chip in the wearable appliance 100 may be more reliably operated.

[0043] FIG. 3, inclusive of FIGS. 3A and 3B, further illustrates the typical nature of an ECG signal being variously captured by the wearable appliance 100 of FIG. 2. Referring to FIGS. 1, 2, and 3A, an ECG signal having the waveform shown in FIG. 3A may be captured by an ECG sensor chip of the watch-type wearable appliance 100 when worn on the left wrist of the user (location 20 in FIG. 1), and when the second ECG electrode 103 is depressed by the user using a finger of his/her right hand (location 30 in FIG. 1). In other words, when the second ECG electrode 103 contacts the finger of the right hand, the first electrode 101 and ground electrode 105 are placed in contact with the skin of the user's left wrist.

[0044] Of particular note with respect to the ECG signal waveform shown in FIG. 3A, a positive ECG signal peak ("R") is periodically manifest above the ECG signal baseline. Of course, the polarity (positive or negative) of ECG signal peak above or below the ECG signal baseline is a matter of definition for the ECG sensor chip of the wearable appliance 100.

[0045] Referring now to FIGS. 1, 2, and 3B, the ECG signal having the waveform shown in FIG. 3B may be captured by an ECG sensor chip of the watch-type wearable appliance 100 when worn on the right wrist of the user (location 30 in FIG. 1), and when the second ECG electrode 103 is depressed by the user using a finger of his/her left hand (location 20 in FIG. 1). In other words, when the second ECG electrode 103 contacts the finger of the left hand, the first electrode 101 and ground electrode 105 are placed in contact with the skin of the user's right wrist.

[0046] Of particular note with respect to the ECG signal waveform shown in FIG. 3B, a negative ECG signal peak ("R") is periodically manifest below the ECG signal baseline. More importantly, the absolute value of the difference between the ECG baseline and the ECG signal peak captured at the right wrist may be less than the absolute value of the difference between the ECG baseline and the ECG signal peak captured at the left wrist. Therefore, all other things remaining equal, the ECG signal apparent at the right wrist may be more difficult to accurately capture than the ECG signal apparent at the left wrist. As a result, more signal processing time and resources may be required from the ECG sensor chip when the wearable appliance 100 of FIG. 2 is worn on a user's right wrist, or some other location manifesting a relatively weaker version of the ECG signal.

[0047] FIG. 4 is a block diagram further illustrating in one example the wearable appliance 100 of FIG. 2. Here, the wearable appliance 100 generally comprises a processing unit 110 and a display 180. The display 180 is an optional component, but may prove very useful in certain embodiments of the inventive concept, such as the watch-wearable appliance 100 of FIG. 2.

[0048] The processing unit 110 may be used to receive, capture and process an ECG signal and to control the operation of the display 180 some other external circuitry responsive to the ECG signal. The processing unit 110 may

alternately or additionally be used to derive a control signal from the captured ECG signal, where this control signal may be provided to one or more external circuits.

[0049] The processing unit 110 of FIG. 4 includes a first signal port (e.g., a pad, terminal or similar electrical element) receiving a first ECG signal from the first ECG electrode 101, a second signal port receiving a second ECG signal from the second ECG electrode 103, a third signal port receiving a ground signal from the ground electrode 105. In addition, the processing unit 110 of FIG. 4 includes a battery 112, a power management integrated circuit (PMIC) 114, an ECG sensor chip 120, an analog-to-digital converter (ADC) 130, a central processing unit (CPU) 140, a memory controller 150, a memory 160, a display controller 170, and an input interface 172.

[0050] Optionally, the processing unit 110 may also include a fourth signal port configured to receive a location signal provided by (e.g.,) a user-activated, location input element 107 discussed in further detail hereafter.

[0051] Assuming for purposes of this description that the wearable appliance 100 of FIG. 4 is similar to the wearable appliance of FIG. 2, it is further assumed that the first ECG electrode 101 and the ground electrode 105 may commonly be placed in contact with either the left wrist or the right wrist of the user, and that the second ECG electrode 103 is placed in contact with the right hand or the left hand of the user, respectively. Under these assumed conditions, the first ECG signal is provided to the processing unit 110 via the first signal port, the second ECG signal is provided to the processing unit 110 via the second signal port, and the ground signal is provided to the processing unit 110 via the third signal port.

[0052] The first signal port is connected to the ECG sensor chip 120 via a first signal line 102, the second signal port is connected to the ECG sensor chip 120 via a second signal line 104, and the third signal port is connected to the battery 112 via a third signal line 106. In this regard, a ground voltage (VSS) may be communicated to one or more of the processing unit 110 components, such as the PMIC 114, ECG sensor chip 120, ADC 130, CPU 140, memory controller 150, memory 160, display controller 170, and/or input interface 172.

[0053] In combination, the battery 112 and PMIC 114 may be used to provide one or more power voltages (not shown) to the processing unit 110 components, display 180, and/or input device 185.

[0054] The ECG sensor chip 120 may be used to receive and process the first ECG signal and the second ECG signal in order to generate one or more ECG output signal(s). For example, the ECG sensor chip 120 may be used to amplify a voltage difference between the first and second ECG signals in order to generate a corresponding, amplified ECG output signal(s).

[0055] Assuming that the ECG output signal(s) are analog in nature, the ADC 130 may be used to receive the ECG output signal(s) and convert the ECG output signal(s) into one or more corresponding ECG digital signal(s). In this regard, certain embodiments of the inventive concept use differential, first and second ECG output signals provided from the ECG sensor chip 120, received by the ADC 130, and then respectively used by the ADC 130 to generate respective first and second ECG digital signals. Thereafter, the first and second ECG digital signals may be provided to the CPU 140.

[0056] The CPU 140 may be used to control the overall operation of all processing unit 110 components, as well as the display 180 and user input device 185. In response to one or more ECG digital signals provided by the ADC 130, the CPU 140 may perform one or more data processing routines adapted to calculate, for example, the user's heart rate. Alternately or additionally, the CPU 140 may be used to identify an arrhythmia or irregular heartbeat for the user. Such data processing routines may be controlled by one or more applications (APP) running on the CPU 140. The programming code used to implement such applications, wholly or in part, may be stored in the memory 160. Regardless of the particular data processing routines run in relation to the ECG digital signal(s) received from the ADC 130 by the CPU 140, the CPU 140 may provide corresponding control signal(s) and/or data (hereafter, control signal/data) to the display controller 170.

[0057] In one exemplary data processing routine, an application running on the CPU 140 may be used to count over a defined period of time a number of ECG peaks identified in one or more ECG signal(s). (See, e.g., FIG. 3). The counted number of ECG peaks may be used to calculate the user's heart rate, and corresponding control signal/data may be communicated from the CPU 140 to the display controller 170 in response to this calculation.

[0058] In another exemplary data processing routine, an application running on the CPU 140 may be used to calculate a time interval between sequential ECG peaks identified in one or more ECG signal(s). The calculated interval may be used to identify an arrhythmia, and corresponding control signal/data may be communicated to the display controller 170 in response to this calculation.

[0059] The memory 160 may be used to store ECG digital signals received from the ADC 130, intermediate computational data generated by an application running on the CPU 140, and/or control signal/data provided by the CPU 140 to the display controller 170.

[0060] Thus, the ECG digital signals, which may be respectively or collectively derived from one or more analog ECG signal(s) received by the ECG sensor chip 120, may be variously processed by the CPU 140 under the control of one or more application(s). For example, assuming the provision of multiple ECG digital signals, the CPU 140 may invert one or more of the ECG digital signal(s) for use during a subsequent data processing routine.

[0061] Exemplary configurations for the ECG sensor chip 120 of FIG. 4 are illustrated in FIGS. 5, 6, 7, 9, 10, and 11.

[0062] The memory controller 150 may be used to write data received from the CPU 140 to the memory 160 and/or read data from the memory 160. The memory 160 may be configured from volatile and/or non-volatile memory. Volatile memory may be random access memory (RAM), dynamic RAM (DRAM), or static RAM (SRAM). Non-volatile memory may be electrically erasable programmable read-only memory (EEPROM), flash memory, magnetic RAM (MRAM), spin-transfer torque MRAM, ferroelectric RAM (FeRAM), phase-change RAM (PRAM), or resistive RAM (RRAM). The memory 160 may be implemented as a smart card, a secure digital (SD) card, a multimedia card (MMC), an embedded MMC (eMMC), an embedded multi-chip package (eMCP), a perfect page NAND (PPN), a universal flash storage (UFS), a solid state drive (SSD), or an embedded SSD (eSSD). The memory 160 may also be implemented as fixed memory or removable memory.

[0063] Although a single memory controller 150 and memory 160 are shown in FIG. 4 for clarity of the description, the memory 160 may include a number of separately or collectively implemented memory device controlled by one or more the memory controller(s) 150, where such memory devices may be similar or different in their operational nature and/or configuration.

[0064] As noted above, the display controller 170 receives certain control signal/data from the CPU 140 and controls the operation of the display 180 according to one or more conventionally understood interfaces. Thus, display controller 170 may be used to control the generation and display of visual images related to the control signals and/or data provided by the CPU 140 under the control of (e.g.,) firmware executed by the CPU 140.

[0065] The input interface 172 may be used to communicate data input via the user input device 185 and/or display 180 to the CPU 140. The user input device 185 may be a device, such as a touch screen controller, a touch sensor, or touch pad capable of generating various input signals (or data) controlling the operation of the wearable appliance 100. In certain embodiments of the inventive concept, the user input device 185 will be a graphical user interface (GUI) displayed on the display 180. FIG. 8 shows one example of a user-interactive GUI that may be displayed on a display 180. The CPU 140 may be used to receive user input signals and/or data provided by the user input device 185 via input interface 172. One or more applications (APP) may be programmed or controlled to in response to such user input signals and/or data.

[0066] In certain embodiments of the inventive concept, it may prove advantageous to implement the processing unit 110 of FIG. 4, or some sub-set of the processing unit 110 components, as a single integrated circuit (IC) chip of the form commonly referred to as a System on Chip (SoC). In one example, the ECG sensor chip 120, PMIC 114, ADC 130 and CPU 140 may be implemented as a SoC. Alternately, the memory controller 150 and memory 160 may be added to the ECG sensor chip 120, PMIC 114, ADC 130 and CPU 140 when implemented as a SoC. In this regard, the memory 160 may be implemented as a SRAM, a DRAM, a small-capacity flash memory, or a large-capacity flash memory in the SoC.

[0067] When the memory controller 150 and memory 160 are integrated into a single semiconductor package, the SoC need not include these commonly provided components. Rather, a first semiconductor package including the SoC, and a second semiconductor package including the memory controller 150 and memory 160 may be variously stacked one on top of the other using (e.g.,) stack balls attached or bonded to a printed circuit board (PCB). The first package and second package may be configured using a package on package (PoP) technique in this regard.

[0068] FIG. 5 is a block diagram further illustrating in one example (120A) the ECG sensor chip 120 of FIG. 4. Referring collectively to FIGS. 1, 2, 3, 4 and 5, the ECG sensor chip 120A includes a switch circuit 121, a switch signal generator 123A, and a differential amplifier 124.

[0069] The location input element 107 of FIG. 5 is assumed to be a mechanical button according to certain embodiments of the inventive concept. When appropriately activated by the user, the button 107 provides an "location indication signal" (IDS) to the switch signal generator 123A. For example, again assuming the watch-wearable appliance

100 of FIG. 2, the button 107 may be provided on the watch body 99 in a manner that allows the left hand or right hand of the user to operate it when the watch 100 is worn on the opposing right wrist or left wrist. Further, with this assumption, the switch circuit 121 will receive the first ECG signal (ECG1) from the first ECG electrode 101 via the first signal line 102, and will also receive the second ECG signal (ECG2) from the second electrode 103 via the second signal line 104.

[0070] In the ECG sensor chip 120A of FIG. 5, the switch signal generator 123A is assumed to generate a switch signal (SS) having at a first (e.g., a logical "low") level (or "first state") in response to a positive indication signal. In response to the switch signal having the first level, the switch circuit 121 operates to apply the first ECG signal received at a first switch input A to a first switch output C, and to apply the second ECG signal received at a second switch input B to a second switch output D. The switch signal generator 123A is further assumed to generate the switch signal having at a second (e.g., a logical "high") level (or "second state") in response to a negative indication signal. In response to the switch signal having the second level, the switch circuit 121 operates to apply the first ECG signal received at the first switch input A to the second switch output D, and to apply the second ECG signal received at the second switch input B to the first switch output C.

[0071] The definition of positive/negative indication signals with respect to the user operation of the location input element (e.g., button) 107 is a matter of design choice. Various types and forms of buttons may be used, and may be variously activated/deactivated (e.g., pressed down, pulled up, toggled, turned or touched) by a user.

[0072] For example, assuming the use of the watch-wearable appliance 100 described in relation to FIG. 2, when the user chooses to wear the watch 100 on his/her left wrist and therefore leaves the button 107 deactivated per the instructions provided with the watch 100, the deactivated state of the button 107 generates the positive indication signal that is applied to the switch signal generator 123A via the signal line 108. In contrast, when the user chooses to wear the watch 100 on his/her right wrist and therefore activates the button 107, the activated state of the button 107 generates the negative indication signal that is applied to the switch signal generator 123A via the signal line 108. Then, the switch signal generator 123A may respond as described above to switch or not-switch the first and second ECG signals.

[0073] The differential amplifier 124 receives and amplifies the first and second ECG signals (SA and SA') respectively provided at the first and second switch outputs C and D of the switch circuit 121, and communicates amplified differential signals SB and SB' to the ADC 130. The differential amplifier 124 will preferably have a low noise characteristic and a high amplification factor. Accordingly, in the example of FIG. 5, the differential amplifier 124 is assumed to include a (front-end) low noise amplifier (LNA) 125 and a (back-end) programmable gain amplifier (PGA) 127. In this regard, an operating voltage V_{dd} and ground voltage V_{SS} are applied to the LNA 125 and PGA 127 as operating voltages.

[0074] The LNA 125 may be used to initially (or intermediately) amplify a difference between the first and second ECG signals received via respective LNA inputs IL1 and IL2 and to respectively provide amplified first and second

ECG signals (e.g., first and second differential signals) at LNA outputs OL1 and OL2. The PGA 127 may then be used to further amplify the difference between the first and second ECG signals received via respective PGA inputs IP1 and IP2 in response to an input gain control signal (GCS), and to respectively provide further amplified first and second ECG signals at PGA outputs OP1 and OP2.

[0075] In this manner, the ECG sensor chip 120A of FIG. 5 is able to process ECG signal(s) no matter the location (e.g., left wrist/right wrist of a user) from which the ECG signal(s) are acquired by the wearable appliance 100 in response to the user's operation of a location input element. Of course, the watch-wearable appliance 100 example drawn in relation to left/right wrists of a user is only one example. Differently configured wearable appliances according to embodiments of the inventive concept may be differently located and will incorporate an appropriate location input element.

[0076] FIG. 6 is a block diagram further illustrating in another example (120B) the ECG sensor chip 120 of FIG. 4. Referring to FIGS. 1, 2, 3, 4, 5 and 6, the ECG sensor chip 120B again includes the switch circuit 121 and differential amplifier 124 previously described in relation to the embodiment illustrated in FIG. 5. Accordingly, these elements and their related signals will not be described in relation to FIG. 6.

[0077] However, the ECG sensor chip 120B of FIG. 6 includes a different type of "location indicator" as compared with the ECG sensor chip 120A described in relation to FIG. 5. Namely, instead of using a switch signal generator 123A responsive to an indication signal (IDS) generated by a location input element (e.g., button 107) activated/deactivated by the user, the switch signal (SS) applied in the ECG sensor chip 102B of FIG. 6 is generated by a peak detector 123B.

[0078] Notably, the peak detector 123B used in the ECG sensor chip 120B of FIG. 6 is an example of a switch signal generating unit that "automatically" provides the switching signal based on the nature of the received ECG signal(s). By way of comparison, the combination of switch signal generator 123A and button 107 are used in the ECG sensor chip 120A of FIG. 5 is an example of a switch signal generating unit that "manually" provides the switching signal.

[0079] It is assumed for purposes of this description that the peak detector 123B generates the switch signal having the first level by operational default. Thus, again assuming the watch-wearable appliance 100 example of FIG. 2, when a user wears the watch 100 on his/her left wrist and touches the second electrode 103 with his/her right hand, the resulting first and second ECG signals (see FIG. 3) will be automatically detected at the LNA outputs OL1 and OL2, or alternately at the PGA outputs OP1 and OP2. Upon detection of the first and second ECG signals by the peak detector 123B, the respective waveforms (or aspects of the waveforms, like the ECG peak) will be interrupted to indirectly determine the location of the watch-wearable appliance as worn by the user.

[0080] Thus, when a relatively stronger first ECG signal apparent at the first LNA output OL1 is detected in relation to a relatively weaker second ECG signal apparent at the second LNA output OL2, the peak detector interrupts this result as the watch 100 being worn on the left wrist and generates the switching signal having the first level (i.e., the default option). In contrast, when a relatively weaker first

ECG signal apparent at the first LNA output OL1 is detected in relation to a relatively stronger second ECG signal apparent at the second LNA output OL2, the peak detector interrupts this result as the watch 100 being worn on the right wrist and generates the switching signal having the second level.

[0081] Here, the switch 121 operates as previously described in relation to the switching signal (SS).

[0082] Thus, in certain embodiments of the inventive concept, the peak detector 123B may be used to determine whether at least one ECG peak in amplified, first and second ECG signals respectively apparent at outputs of the LNA 125 or PGA 127 is above or below the ECG signal baseline. In response to this determination, the peak detector 123B may be used to generate the switch signal having an appropriate level. That is, when at least one of the ECG peaks of the amplified, first and second ECG signals is detected above the baseline as shown in FIG. 3A, the peak detector 123B will generate the switch signal with the first level. However, when at least one of the ECG peaks of the amplified, first and second ECG signals is detected below the baseline as shown in FIG. 3B, the peak detector 123B will generate the switch signal with the second level.

[0083] Here again, an ECG sensor chip 120B according to certain embodiments of the inventive concept correctly processes received ECG signal(s) regardless of the location (e.g., left/right wrist) that the user decides to wear the wearable appliance acquiring the ECG signal(s).

[0084] Although the peak detector 123B of FIG. 6 is illustrated as detecting amplified first and second ECG signals apparent at the respective outputs of the LNA 125 (or the PGA 127), the first and second ECG signals apparent at the switch circuit 121 may be detected in other embodiment of the inventive concept.

[0085] FIG. 7 is a block diagram further illustrating in still another example (120C) the ECG sensor chip 120 of FIG. 4. Referring to FIGS. 1, 2, 3, 4 and 7, the ECG sensor chip 120C substantially includes only the differential amplifier 124, as compared with the previous two exemplary embodiments.

[0086] In the absence of a switch 121, the LNA 125 of FIG. 7 may directly receive the first ECG signal via the first signal line 102 and the second ECG signal via the second signal line 104. Following amplification of a voltage difference between these two ECG signals as previously described, the first and second ECG output signals respectively apparent at the first and second PGA outputs OP1 and OP2, are communicated to the ADC 130, and the processing and interruption of these ECG output signals is left to the CPU 140 based on location information identifying a location at which the user wears the wearable appliance. For example, CPU processing and interpretation of ECG digital signals derived from the first and second ECG signals may be performed without user-provided input (automatically) or with user-provided input, such as location information input via the user input device 185 or a GUI displayed on the display 180.

[0087] Referring again to FIGS. 4, 7 and 8, the GUI 181 displayed on display 180 may be created by an application (APP) running on the CPU 140. Again assuming the watch-wearable appliance 100 of FIG. 2, the user may be asked to indicate as part of an application execution via the GUI 181 the location of the watch 100 (e.g., on the left or right wrist) as worn by the user.

[0088] Such an indication may be easily made by selecting and touching one of the GUI icons 182 or 184 displayed on the display 180. Thereafter, the input device 185 may be used to communicate location indication data (e.g., a sensed touch signal) to the CPU 140 via the input interface 172. The CPU 140 may then be used to appropriately process (e.g.,) the ECG output signals provided to the CPU 140 by the ADC 130 and associated with the first and second ECG signals, whether the first and second ECG signals are presented to the amplifier 124 as shown in FIG. 3B or as shown in FIG. 3A.

[0089] Of further note, the foregoing selection by the user between the GUI icons 182 and 184 may occur either before, or after the first and second ECG signals are received by the amplifier 124.

[0090] Thus, it has been shown with reference to the embodiments respectively illustrated in FIGS. 5, 6 and 7 that an ECG sensor chip of various designs may be used to determine (or respond to) the location of a wearable appliance, and process ECG signal(s) captured by the wearable appliance regardless of the location. This wearable appliance location determination and subsequent ECG signal processing capabilities may be implemented using manual or automatic detection approaches, and may be implemented using hardware-based and/or software-based solutions.

[0091] The embodiments of the inventive concept illustrated in FIGS. 9, 10 and 11 (120D, 120E and 120F) are respectively analogous to the embodiments previously described in relation to FIGS. 5, 6 and 7 (120A, 120B and 120C). However, in each one of the embodiments illustrated in FIGS. 9, 10 and 11 (120D, 120E and 120F), the amplifier 124 has been modified to include an offset controller 129 that provides voltage control offsets to one or both of the LNA 125 and PGA 127. Thus, the differential amplifier 124 included in each of these additional embodiments functions as a differential amplifier with an offset characteristics.

[0092] FIG. 12 is a conceptual diagram illustrating a general approach whereby offset voltages are used in conjunction with the amplifier 124 to generate an amplified ECG signal (SC) that is more easily discriminated. Referring to FIG. 12 and holding in mind the previous descriptions of the embodiments illustrated in FIGS. 4, 5, 6 and 7, a digital-to-analog converter (DAC) 175 is added behind the ADC 130. Here, the DAC 175 may be provided as part of the display controller 170 or display 180. That is, the display 180 may include a display driver IC having the DAC 175.

[0093] A voltage difference “dV” is equal to the absolute value of a difference between the first ECG signal (SA) and the second ECG signal (SA'), where operating voltages of Vdd and 0V are assumed for the LNA 125 and PGA 127. During the differential amplification with voltage offset of the first and second ECG signals, as shown in FIG. 12, the first ECG signal SA applied to a first input of the LNA 125 and the second ECG signal SA' applied to a second input of the LNA 125 have the relationship shown at (a) of FIG. 12.

[0094] Before an offset voltage (Vos) is applied to the differential amplifier 124, and particularly to the LNA 125, the ECG output signals SB and SB' provided by the differential amplifier 124 will be symmetrical around Vdd/2 as shown in (b) of FIG. 12. Thus, when the offset voltage is not applied to the differential amplifier 124, an amplified differential output signal SC' provided to the DAC 175 will be as shown in (d) of FIG. 12. This generated version of the

amplified differential ECG signal SC' extends over only about half of the voltage range between Vdd and 0V.

[0095] However, when the offset voltage is applied to the differential amplifier 124, and particularly to the LNA 125, the output ECG signals SB and SB' of the differential amplifier 124 will again be symmetrical around Vdd/2, but will be modified by the offset voltage value Vos as shown in (c) of FIG. 12. As a result of this offset voltage modification, the amplified differential ECG signal SC illustrated in (e) of FIG. 12 occupies the full operating voltage range.

[0096] Of note, the signal-to-noise ratio for the amplified differential ECG signal is much better when an offset voltage is applied. That is, when an offset voltage is applied to the differential amplifier 124, and particularly to the LNA 125, the difference between the first and second ECG signals is more pronouncedly amplified.

[0097] As shown in FIGS. 9, 10 and 11, one or more offset voltages (singularly or collectively, Vos) provided by the offset controller 129 may be applied one or both of the LNA 125 and PGA 127. A first offset voltage applied to the LNA 125 may be the same or different from a second offset voltage applied to the PGA 127.

[0098] FIG. 13 is a perspective diagram illustrating a wearable appliance 100-1 capable of capturing and processing one or more ECG signal(s) according to certain embodiments of the inventive concept. Referring to FIG. 13, the wearable appliance 100-1 again takes the form of a wrist watch, but now includes the first electrode 101, second electrode 103, and ground electrode 105 commonly arranged proximate one another on a bottom surface of the watch 100-1. A processing unit 110 and display 180 similar to those previously described may be included in the wearable appliance 100-1. Optionally, the wearable appliance 100-1 may also include the input device 185 and/or the user-activated location input device (e.g., button) 107 previously described.

[0099] FIG. 14 is a perspective diagram illustrating a wearable appliance 100-2 capable of capturing and processing one or more ECG signal(s) according to certain embodiments of the inventive concept. Referring to FIG. 14, the wearable appliance 100-2 again takes the form of a wrist watch and includes first electrode 101 and ground electrode 105 protruding from a bottom surface of watch body 99 supported on the user's wrist by a watch strap 95. The second electrode 103 is arranged on a portion of the watch strap 95 directly opposite the watch body 99. Here again, the processing unit 110, display 180, user input 185 and/or user-activated location input device 107 previously described may be included in the wearable appliance 100-2.

[0100] FIG. 15 is a perspective diagram illustrating a wearable appliance 100-3 capable of capturing and processing one or more ECG signal(s) according to certain embodiments of the inventive concept. The eye glasses-wearable appliance 100-3 includes one or more of first, second and ground electrodes 101, 103, and 105, as previously described, processing unit 110, and optionally, one or more displays 180, where the eye glasses 100-3 include left and right lens parts 88 connected by a bridge part 85, a left arm member 87 supporting the eye glasses on a left side of a user's head, and a right arm member 86 supporting the eye glasses on a right side of the user's head.

[0101] Although the eye glasses of FIG. 15 are illustrated as having the first electrode 101, second electrode 103 and ground electrode 105 disposed closely proximate one to

another on a single arm member, this need not always be the case. For example, the second electrode **103** may be disposed on the opposing left arm member **87** instead of the right arm member **86** having the first electrode **101** and ground electrode **105**. Further, one or more displays **180** may be incorporated within one or both of the lens parts **88**.

[0102] In certain embodiments of the inventive concept, the processing unit **110** and a power source may be provided on a SoC disposed on one or both arm member(s) **87/86** of the eye glasses **100-3** along with one or more ECG sensors **101, 103** and **105**. However, one or more of the ECG sensors **101, 130** and **105** may be separately disposed on the eye glasses **100-3** external to the SoC.

[0103] FIG. **16**, inclusive of FIGS. **16A** and **16B**, is a perspective diagram illustrating a wearable appliance **100-4** capable of capturing and processing one or more ECG signal(s) according to certain embodiments of the inventive concept. Here, the wearable appliance **100-4** takes the form of a skin-adhering patch **190** that may be directly applied to a desired location by a user. One or more ECG-sensing electrodes (e.g., first ECG electrode **101** and second ECG electrode **1030**) may be incorporated within the patch **190**, along with a processing unit **110** consistent with the previously described embodiments.

[0104] Of particular note, the arrangement of the sensors in patch **190** of FIG. **16B** “along” the direction of the primary veins running through the user’s arm **191** (i.e., direction “a”) has been found to be more effective in facilitating the capture of an ECG signal than the arrangement of the sensors in patch **190** of FIG. **16A** “across” the direction of the primary veins running through the user’s arm **191** (i.e., direction “b”).

[0105] The embodiment of FIG. **16** is drawn to a user’s lower arm, but those skilled in the art will understand from the foregoing description that other patch-embodiments consistent with the inventive concept may be configured for use in relation to other user locations such as the upper arm, upper or lower leg, neck, etc.

[0106] FIG. **17** is a block diagram of a data processing system **200** including a wearable appliance **100-5** including the ECG sensor chip **120** FIG. **4** according to embodiments of the inventive concept. Referring to FIG. **17**, the data processing system **200** includes the wearable appliance **100-5** and a computing device **210** configured to communicate with the wearable appliance via a wireless and/or a hardwired connection **199**.

[0107] The wearable appliance **100-5** may be configured like the wearable appliance previously described in relation to FIG. **4**, except for the additional provision of a wireless interface **190**. The wireless interface **190** may be used to communicate data processed by the CPU **140** to the computing device **210** using the wireless connection **199**. The data may include data related with an ECG signal (or ECG waveform), data related with a heart rate, and/or data related with arrhythmia. The wireless interface **190** may support Bluetooth, Bluetooth low energy (BLE), near field communication (NFC), radio-frequency identification (RFID), or WiFi.

[0108] The computing device **210** illustrated in FIG. **17** comprises; a wireless interface **215**, a CPU **220**, a memory controller **225**, a memory **230**, a display controller **235**, and a display **240**. The computing device **210** may be implemented as a mobile computing device or a server. The server may be used to provide a telemedicine service, for example.

[0109] The wireless interface **215**, the CPU **220**, the memory controller **225**, the memory **230**, the display controller **235**, and the display **240** may communicate with one another through a bus structure **211**. The wireless interface **215** may communicate with the wireless interface **190**. The wireless interface **215** may support Bluetooth, BLE, NFC, RFID, or WiFi.

[0110] The CPU **220** may control the memory controller **225** and the display controller **235** through the bus structure **211**.

[0111] The memory controller **225** may write data (e.g., data about an ECG) to the memory **230** or may read data (e.g., data about an ECG) from the memory **230** according to the control of the CPU **220**. The memory **230** may be implemented using volatile and/or non-volatile memory.

[0112] The display controller **235** may transmit data from the CPU **220** or the memory controller **225** to the display **240** through interface according to the control of the CPU **220**. The data may include data related with an ECG signal (or ECG waveform), data related with a heart rate, and/or data related with arrhythmia

[0113] FIG. **18** is a flowchart summarizing a method of using an ECG sensor chip in a wearable appliance according to certain embodiments of the inventive concept. Referring to FIGS. **4, 5** and **6**, as well as FIGS. **13, 14, 15, 16** and **17**, the switch signal generator **123A** or the peak detector **123B** may be used to generate the switch signal (SS) and then communicate the switch signal to the switch circuit **121** (**S110**). As described above, in response to the switch signal having the first level, the switch circuit **121** will pass the first ECG signal **ECG1** received via the first input terminal A to the first output terminal C and the second ECG signal **ECG2** received via the second input terminal B to the second output terminal D. Alternately, in response to the switch signal having the second level, the switch circuit **121** will pass the first ECG signal **ECG1** received via the first input terminal A to the second output terminal D and the second ECG signal **ECG2** received via the second input terminal B to the first output terminal C (**S120**).

[0114] The differential amplifier **124** then amplifies the difference between the first ECG signal (SA) apparent at the first input terminal IL1 and the second ECG signal (SA') apparent at the second input terminal IL2, and output the amplified ECG output signals (SB and SB') to the ADC **130** (**S130**).

[0115] As described above with reference to FIGS. **9** and **10**, when the offset controller **129** applies the offset voltage V_{os} to the differential amplifier **124**, the differential amplifier **124** may output the amplified signals SB and SB' reflecting the offset voltage V_{os} to the ADC **130**, as described with reference to FIG. **12** and with respect to operation **S130**.

[0116] FIG. **19** is a flowchart summarizing a method of using a wearable appliance according to certain embodiments of the inventive concept. Referring to FIGS. **4, 7, 11, 13, 14, 15, 16** and **18**, a user of the wearable appliance (e.g., **100, 100-1, 100-2, 100-3, 100-4** or **100-5**) may select an icon (**182** or **184**) from the GUI **181** displayed on the display **180** using the input device **185** (**S210**) before beginning the process of ECG signal capture.

[0117] Here, it is assumed that the first electrode **101** and ground electrode **105** are placed in contact with one of the left hand or right hand, while the second electrode **103** is contacted by the other one of the left hand or right hand. As

a result, the first electrode **101** generates the first ECG signal and the second electrode **103** generates the second ECG signal ECG2 (**S220**).

[**0118**] The differential amplifier **124** is then used to amplify a difference between the first ECG signal and second ECG signal, generate amplified ECG output signals (SB and SB'), and communicate the amplified ECG output signals to the ADC **130** (**S230**). The ADC **130** then converts the amplified ECG output signals SB and SB' into corresponding digital ECG signals (**S240**).

[**0119**] When the user selected an icon (e.g. **182**) during operation **S210**, corresponding location information was communicated to the CPU **140** via input device **185** and user interface **172**. Thus, under the foregoing assumptions, when the wearable appliance is worn on the left wrist and a finger of the right hand makes contact with the second electrode **103**, an ECG signal having the waveform of FIG. 3A is generated. Accordingly, the CPU **140** processes the resulting digital ECG signals provided by the ADC **130** based on the location information by processing the digital ECG signal as a normal (or non-inverted) ECG signal (**S260**).

[**0120**] However, assuming that the user selected the icon **184** in operation **S210**, different location information is communicated to the CPU **140** via the input device **185** and user interface **172**. Thus, when the wearable appliance is worn on the right wrist and a finger of the left hand makes contact with the second electrode **103**, the resulting ECG signal will have the waveform of FIG. 3B. Accordingly, the CPU **140** will process the corresponding digital ECG signal provided by from the ADC **130** based on the location information and process the digital ECG signal as an inverted ECG signal (**S270**).

[**0121**] Thereafter, the display controller **170** or the DAC **175** of the display **180** may be used to convert certain digital control signal/data provided by the CPU **140** into one or more analog signal(s) (**S280**).

[**0122**] FIG. 20 is a block diagram of a data processing system **300** including a wearable appliance **100-5** including an ECG sensor chip like the one described in relation to FIG. 4 according to certain embodiments of the inventive concept. The data processing system **300** may be used to provide one or more tele-medicine service(s) adapted to monitor, record, characterize and/or protect the health of a user wearing the wearable appliance **100-5**.

[**0123**] Thus, referring to FIG. 20, the data processing system **300** includes the wearable appliance **100-5** and a first health care server **320** configured to communicate data derived or monitored by the wearable appliance via a wireless network (e.g., the internet **310**, or similar distributed, wireless communication system). In certain embodiments of the inventive concept, the data processing system **300** may further include a second health care server **350** similarly configured to communicate with the wearable appliance **100-5** and/or the first health care server **320**. Here, for example, it is assumed that an insurance entity manages the second health care server **350** and its constituent database **355**.

[**0124**] When the user of the wearable appliance **100-5** causes the execute of an application installed in the wearable appliance **100-5**, a wireless interface of the wearable appliance **100-5** will communicate health-related data (HDATA) to the health care server **320** via the internet **310** (**S301**). It is assumed that the application is capable of storing a uniform resource locator (URL) associated with the first

health care server **320** and/or the second health care server **350**. Thus, the application may be used to communicate health data (HDATA) to the first health care server **320** and/or the second health care server **350** using the URL.

[**0125**] The wireless network **310** may be used to communicate the health data (HDATA) to the first health care server **320** (**S303**) and/or the second health care server **320** (**S321**). In this regard, the health data may include data associated with or derived from one or more ECG signal(s), including data related indicating the user's heart rate.

[**0126**] The first health care server **320** receives the health data (**S303**), may store it, as necessary, in a constituent database **321** (**S304**), and communicate the health data—or data derived from the health data—to a doctor's computing device **345** via the network **330** (**S305**). In this context, the doctor's computing device **345** may be a personal computer (PC) or a tablet PC. Assuming that the doctor works at a medical institution (e.g., a private medical practice, public health care center, clinic, hospital, or rescue center **340**), his/her computing device may be administered or integrated with a larger patient data system in order to monitor received health data, and diagnose the user's medical state. In response to the health data, the doctor and/or his/her representative(s) may then input diagnostic data (DDATA) (e.g., information related to a doctor's counsel or diagnosis) to the doctor's computing device **345** (**S307**). The doctor's computing device **345** may then communicate the diagnostic data to the first health care server **320** via the network **330** (**S309**). The first health care server **320** receives the diagnostic data, stores it in the database **321** (**S304**), and communicates it to the wearable appliance **100-5** and/or the second health care server **350** via the wireless network **310** (**S311**, **S313** and/or **S321**). In response to the diagnostic data, the wearable appliance **100-5** may display the certain data via its display **185** under the control of the application executed by the CPU **140**, and in certain embodiments of the inventive concept, the second health care server **350** may store the diagnostic data in the database **355** (**S323**).

[**0127**] In this manner, the user of the wearable appliance **100-5** may receive diagnostic data from a health care professional is something approximating real time communications, depending on the medical professional's ability to receive and respond to the health data communicated by the wearable appliance **100-5**.

[**0128**] FIG. 21 is a block diagram of a data processing system **400** including a wearable appliance **100-5** including the ECG sensor chip like the one described in relation to FIG. 4 according to certain embodiments of the inventive concept. Like the data processing system **300** of FIG. 20, the data processing system **400** of FIG. 21 may be used to provide one or more tele-medicine services.

[**0129**] Referring to FIG. 21, the data processing system **400** includes the wearable appliance **100-5** and a computing device **210** configured to communicate with the wearable appliance **100-5** via a wireless network (e.g., an internet **405**). According to some embodiments, the data processing system **400** may further include health care server **415** configured to communicate with the computing device **210** via a wireless network (e.g., an internet **410**).

[**0130**] When a user of the wearable appliance **100-5** causes execute of an application installed in the wearable appliance **100-5**, a wireless interface of the wearable appliance **100-5** will communicate health data (HDATA) to the computing device **210** via the wireless network **405** (**S401**).

The health data may include one or more ECG signal(s) indicating the user's heart rate.

[0131] In certain embodiments of the inventive concept, the computing device 210 may receive the health data from the wearable appliance 100-5 via a near field communication (NFC) scanning method or tagging method. Here, it is assumed that an application capable of receiving the health data from the wearable appliance 100-5 is installed on the computing device 210. For example, the wearable appliance 100-5 may operate as a NFC tag and the computing device 210 may operate as NFC reader. As described above, the application installed in the computing device 210 may store a URL associated with a health care server 415 configured to communicate with the computing device 210 and a doctor's computing device 425.

[0132] When the doctor's computing device 210 receives the health data from the wearable appliance 100-5, the computing device 210 may generate an indication and/or display the health data or data derived therefrom. If the doctor's intervention is warranted, the computing device 210 may be used to communicate diagnostic data (DDATA) and the health data to the health care server 415 via an internet 410 under the control of an application controlled by the doctor or his/her medical team. Thus, the application may communicate the health data to the health care server 415 using the URL of the health care server 415.

[0133] In this manner, the health care server 415 may receive the health data (S405), stores it in a constituent database 417 (S406), and communicate the health data to a doctor's computing device 425 via a network. Here again, the network may be a wired communication network and/or a wireless communication network, and doctor's computing device 425 may be a personal computer (PC) or a tablet PC.

[0134] Where the doctor works in a medical institution, public health care center, clinic, hospital, or rescue center 420, the computing device 425 may be functionally integrated with patient services systems used to monitor health data and diagnose a user's medical state. The doctor may input diagnostic data in response to the health data to the doctor's computing device 425 (S407). The doctor's computing device 425 may then communicate the diagnostic data to the health care server 415 via the network.

[0135] The health care server 415 then receives the diagnostic data, stores it in the database 417, and communicates it to the computing device 210 via the wireless internet 410 (S409 and S411). The computing device 210 may display the data DDATA via a display 185 under the control of the application program executed by the CPU 140.

[0136] In some certain embodiments, if the user has an emergency, the medical team, the family protector, or the passerby may perform emergency treatment for the user in response to the diagnostic data displayed by the computing device 210. For example, if necessary, the medical team, family protector, or passerby may engage in a video call with the doctor using the computing device 210. Accordingly, the medical team, family protector, or passerby may administer appropriate emergency treatment to the user under the guidance of the doctor. Further, the medical team, family protector, or passerby may provide real time feedback in response to the doctor's monitoring and/or diagnosis.

[0137] According to the foregoing embodiments of the inventive concept, an ECG sensor chip may or may not invert a captured ECG signal according to a switch signal. In addition, the ECG sensor chip using an amplifier config-

ured with an offset controller may be used to reduce noise and improve signal differentiation. According to embodiments of the inventive concept, a wearable appliance will appropriately process one or more ECG signals in response to the location at which the wearable appliance is worn by a user.

[0138] The foregoing embodiments are illustrative in nature. The scope of the inventive concept is defined by the following claims and their equivalents.

What is claimed is:

1. A system configured for use in a wearable appliance, the system comprising:

an electrocardiogram (ECG) sensor chip that receives a first ECG signal from a first ECG sensor and a second ECG signal from a second ECG sensor, and includes an amplifier that amplifies a difference between the first ECG signal and the second ECG signal to generate a first ECG output signal and a second ECG output signal;

an analog-to-digital converter (ADC) that receives the first ECG output signal and the second ECG output signal and generates corresponding ECG digital signals; and

a processor that receives the ECG digital signals and processes the ECG digital signals in response to received location information indicating a location of the wearable appliance as worn by a user.

2. The system of claim 1, wherein the location information is generated in response to user activation/deactivation of a user-activated location input element.

3. The system of claim 2, wherein the user-activated location input element is one of a mechanical button disposed on the wearable appliance, an icon presented on a graphical user interface provided by a display disposed on the wearable appliance, and a user input device disposed on a computing device wirelessly connected to the wearable appliance.

4. The system of claim 1, wherein the amplifier comprises a front-end low noise amplifier that receives the first ECG signal and the second ECG signal from a switch, and generates an intermediate amplified first ECG signal and an intermediate amplified second ECG signal, and a back-end programmable gain amplifier that receives the intermediate amplified first ECG signal and the intermediate amplified second ECG signal from the front-end low noise amplifier, and generates an amplified first ECG signal and an amplified second ECG signal.

5. The system of claim 4, further comprising:

an offset controller that provides a voltage control offset to at least one of the front-end low noise amplifier and the back-end programmable gain amplifier.

6. The system of claim 1,

wherein the electrocardiogram sensor chip further includes:

a switch controlled by a switching signal and including a first switch input that receives the first ECG signal, a second switch input that receives the second ECG signal, a first switch output, and a second switch output; and

a location indicator that generates the switching signal in one of a first state and a second state,

wherein the amplifier includes a first amplifier input that receives one of the first ECG signal and the second ECG signal from the first switch output and a second

amplifier input that receives the other one of the first ECG signal and the second ECG signal from the second switch output, and amplifies a difference between the first ECG signal and the second ECG signal;

wherein, in response to the first state of the switching signal, the switch passes the first ECG signal from the first switch input to the first switch output and passes the second ECG signal from the second switch input to the second switch output, and in response to the second state of the switching signal, the switch passes the first ECG signal from the first switch input to the second switch output and passes the second ECG signal from the second switch input to the first switch output,

wherein the location indicator comprises a switch signal generator that generates the switching signal in one of the first state and the second state in response to an indication signal that is generated in response to user activation/deactivation of a user-activated location input element, and the user-activated location input element is one of a mechanical button disposed on the wearable appliance, an icon of a graphical user interface presented on a display disposed on the wearable appliance, and a user input device disposed on a computing device wirelessly connected to the wearable appliance.

7. The system of claim 1,

wherein the electrocardiogram sensor chip further includes:

a switch controlled by a switching signal and including a first switch input that receives the first ECG signal, a second switch input that receives the second ECG signal, a first switch output, and a second switch output; and

a location indicator that generates the switching signal in one of a first state and a second state,

wherein the amplifier includes a first amplifier input that receives one of the first ECG signal and the second ECG signal from the first switch output and a second amplifier input that receives the other one of the first ECG signal and the second ECG signal from the second switch output, and amplifies a difference between the first ECG signal and the second ECG signal;

wherein, in response to the first state of the switching signal, the switch passes the first ECG signal from the first switch input to the first switch output and passes the second ECG signal from the second switch input to the second switch output, and in response to the second state of the switching signal, the switch passes the first ECG signal from the first switch input to the second switch output and passes the second ECG signal from the second switch input to the first switch output,

wherein the location indicator comprises a switch signal generator that generates the switching signal in one of the first state and the second state in response to an indication signal generated in response to user activation/deactivation of a user-activated location input element, and

wherein the amplifier comprises:

a front-end low noise amplifier that receives the first ECG signal and the second ECG signal from the switch, and generates an intermediate amplified first ECG signal and an intermediate amplified second ECG signal; and

a back-end programmable gain amplifier that receives the intermediate amplified first ECG signal and the intermediate amplified second ECG signal from the low noise amplifier, and generates an amplified first ECG signal and an amplified second ECG signal.

8. The system of claim 7, wherein the electrocardiogram sensor chip further includes:

an offset controller that provides a voltage control offset to at least one of the front-end low noise amplifier and the back-end programmable gain amplifier.

9. The system of claim 1, wherein the system is installed in a wearable appliance that comprises:

a first electrocardiogram (ECG) electrode disposed on a first surface of the wearable appliance;

a second ECG electrode disposed on a second surface of the wearable appliance different from the first surface; and

a ground electrode disposed on a third surface of the wearable appliance in contact with the user at the location when the wearable appliance is worn by the user;

wherein the ECG sensor chip receives the first ECG signal from the first ECG electrode and the second ECG signal from the second ECG electrode,

wherein the ECG sensor chip comprises:

a switch controlled by a switching signal and including a first switch input that receives the first ECG signal, a second switch input that receives the second ECG signal, a first switch output, and a second switch output; and

a location indicator that generates the switching signal in one of a first state and a second state, wherein, in response to the first state of the switching signal, the switch passes the first ECG signal from the first switch input to the first switch output and passes the second ECG signal from the second switch input to the second switch output, and in response to the second state of the switching signal, the switch passes the first ECG signal from the first switch input to the second switch output and passes the second ECG signal from the second switch input to the first switch output,

wherein the amplifier includes a first amplifier input that receives one of the first ECG signal and the second ECG signal from the first switch output and a second amplifier input that receives the other one of the first ECG signal and the second ECG signal from the second switch output, and generates an amplified difference signal between the first ECG signal and the second ECG signal;

wherein the first surface and third surface are a same surface of the wearable appliance, such that the ground electrode and first ECG electrode are proximately disposed on the same surface of the wearable appliance in contact with the user at the location when the wearable appliance is worn by the user, and wherein the wearable appliance is a watch, the location is a wrist of the user, the same surface is a bottom surface of the watch, and the second surface is one of a top surface and a side surface of the watch.

10. The system of claim 1, wherein the system is installed in the wearable appliance, and the wearable appliance is worn at a location on a user and comprises:

- a first electrocardiogram (ECG) electrode disposed on a first surface of the wearable appliance; and
a second ECG electrode disposed on a second surface of the wearable appliance different from the first surface; wherein the ECG sensor chip receives a first ECG signal from the first ECG electrode and a second ECG signal from the second ECG electrode, and
wherein the ECG sensor chip comprises;
a switch controlled by a switching signal and including a first switch input that receives the first ECG signal, a second switch input that receives the second ECG signal, a first switch output, and a second switch output; and
a location indicator that generates the switching signal in one of a first state and a second state, wherein, in response to the first state of the switching signal, the switch passes the first ECG signal from the first switch input to the first switch output and passes the second ECG signal from the second switch input to the second switch output, and in response to the second state of the switching signal, the switch passes the first ECG signal from the first switch input to the second switch output and passes the second ECG signal from the second switch input to the first switch output,
wherein the amplifier includes a first amplifier input that receives one of the first ECG signal and the second ECG signal from the first switch output and a second amplifier input that receives the other one of the first ECG signal and the second ECG signal from the second switch output, and generates an amplified difference signal between the first ECG signal and the second ECG signal;
wherein the wearable appliance is a watch comprising a watch body and a watch strap that attaches the watch body to a wrist of the user,
wherein the first surface and a third surface on which a ground electrode is disposed are a bottom surface of the watch body in contact with the wrist of the user when the watch is worn by the user, and
wherein a second surface is a portion of the watch strap, and
wherein the second surface is a portion of the watch strap directly opposite the watch body when the watch is worn by the user.
- 11.** The system of claim 1, wherein the system is installed in the wearable appliance, and the wearable appliance is worn at a location on a user and comprises:
a first electrocardiogram (ECG) electrode; and
a second ECG electrode;
wherein the ECG sensor chip receives a first ECG signal from the first ECG electrode and a second ECG signal from the second ECG electrode, and comprises;
a switch controlled by a switching signal and including a first switch input that receives the first ECG signal, a second switch input that receives the second ECG signal, a first switch output, and a second switch output; and
a location indicator that generates the switching signal in one of a first state and a second state, wherein, in response to the first state of the switching signal, the switch passes the first ECG signal from the first switch input to the first switch output and passes the second ECG signal from the second switch input to the second switch output, and in response to the second state of the switching signal, the switch passes the first ECG signal from the first switch input to the second switch output and passes the second ECG signal from the second switch input to the first switch output,
wherein the amplifier includes a first amplifier input that receives one of the first ECG signal and the second ECG signal from the first switch output and a second amplifier input that receives the other one of the first ECG signal and the second ECG signal from the second switch output, and generates an amplified difference signal between the first ECG signal and the second ECG signal;
wherein the wearable appliance is eye glasses, comprising:
left and right lens parts connected by a bridge part;
a left arm member that supports the eye glasses on a left side of a user's head; and
a right arm member that supports the eye glasses on a right side of the user's head,
wherein at least one of the first ECG electrode and the second ECG electrode is disposed on one of the left arm member and right arm member in contact with the user's head when the glasses are worn by the user, and
wherein one of the first ECG electrode and the second ECG electrode is disposed on the left arm member, and the other one of the first ECG electrode and the second ECG electrode is disposed on the right arm member.
- 12.** The system of claim 1, wherein the system is installed in the wearable appliance, and the wearable appliance is worn at a location on a user and comprises:
a first electrocardiogram (ECG) electrode;
a second ECG electrode;
an analog-to-digital converter (ADC);
a Central Processing Unit (CPU); and
a display,
wherein the ECG sensor chip receives a first ECG signal from the first ECG electrode and a second ECG signal from the second ECG electrode, and comprises;
a switch controlled by a switching signal and including a first switch input that receives the first ECG signal, a second switch input that receives the second ECG signal, a first switch output, and a second switch output; and
a location indicator that generates the switching signal in one of a first state and a second state, wherein, in response to the first state of the switching signal, the switch passes the first ECG signal from the first switch input to the first switch output and passes the second ECG signal from the second switch input to the second switch output, and in response to the second state of the switching signal, the switch passes the first ECG signal from the first switch input to the second switch output and passes the second ECG signal from the second switch input to the first switch output,
wherein the amplifier includes a first amplifier input that receives one of the first ECG signal and the second ECG signal from the first switch output and a second amplifier input that receives the other one of the first ECG signal and the second ECG signal from the second switch output, and generates an amplified difference signal between the first ECG signal and the second ECG signal;

switch output, and generates an amplified difference signal between the first ECG signal and the second ECG signal;

wherein the analog-to-digital converter (ADC) receives the amplified difference signal from the amplifier and generates a corresponding ECG digital signals;

wherein the Central Processing Unit (CPU) receives the ECG digital signals from the ADC and generates corresponding display data; and

wherein the display is configured to generate a visual image in response to the display data received from the CPU.

13. The system of claim 1, wherein the system is installed in the wearable appliance, and the wearable appliance is worn at a location on a user and comprises:

- a first electrocardiogram (ECG) electrode;
- a second ECG electrode;
- an analog-to-digital converter (ADC);
- a Central Processing Unit (CPU); and
- a display,

wherein the ECG sensor chip receives a first ECG signal from the first ECG electrode and a second ECG signal from the second ECG electrode, and comprises:

- a switch controlled by a switching signal and including
 - a first switch input that receives the first ECG signal,
 - a second switch input that receives the second ECG signal, a first switch output, and a second switch output; and
- a location indicator that generates the switching signal in one of a first state and a second state, wherein, in response to the first state of the switching signal, the switch passes the first ECG signal from the first switch input to the first switch output and passes the second ECG signal from the second switch input to the second switch output, and in response to the second state of the switching signal, the switch passes the first ECG signal from the first switch input to the second switch output and passes the second ECG signal from the second switch input to the first switch output,

wherein the amplifier includes a first amplifier input that receives one of the first ECG signal and the second ECG signal from the first switch output and a second amplifier input that receives the other one of the first ECG signal and the second ECG signal from the second switch output, and generates an amplified difference signal between the first ECG signal and the second ECG signal;

wherein the wearable appliance is eye glasses, comprising:

- left and right lens parts connected by a bridge part;
- a left arm member that supports the eye glasses on a left side of a user's head; and
- a right arm member that supports the eye glasses on a right side of the user's head,

wherein at least one of the first ECG electrode and the second ECG electrode is disposed on one of the left arm member and right arm member in contact with user's head when the glasses are worn by the user,

wherein the analog-to-digital converter (ADC) receives the amplified difference signal from the amplifier and generates a corresponding ECG digital signals;

wherein the Central Processing Unit (CPU) receives the ECG digital signals from the ADC and generates corresponding display data; and

wherein the display is configured to generate a visual image in response to the display data received from the CPU, wherein the display is operationally integrated with at least one of the left lens part and right lens parts such that the visual image is visible to the user when the eye glasses are worn by the user.

14. A data processing system, comprising:

- a wearable appliance including an electrocardiogram (ECG) sensor chip; and

- a computing device configured to communicate information with the wearable appliance via at least one of a wireless connection and a hardwired connection,

wherein the wearable appliance includes:

- a first electrocardiogram (ECG) electrode;

- a second ECG electrode; and

- an ECG sensor chip that receives a first ECG signal from the first ECG electrode and a second ECG signal from the second ECG electrode, wherein the ECG sensor chip includes a switch controlled by a switching signal and including a first switch input that receives the first ECG signal, a second switch input that receives the second ECG signal, a first switch output, and a second switch output, an amplifier including a first amplifier input that receives one of the first ECG signal and the second ECG signal from the first switch output and a second amplifier input that receives the other one of the first ECG signal and the second ECG signal from the second switch output, and generates an amplified difference signal between the first ECG signal and the second ECG signal, and a location indicator that generates the switching signal in one of a first state and a second state, wherein, in response to the first state of the switching signal, the switch passes the first ECG signal from the first switch input to the first switch output and passes the second ECG signal from the second switch input to the second switch output, and in response to the second state of the switching signal, the switch passes the first ECG signal from the first switch input to the second switch output and passes the second ECG signal from the second switch input to the first switch output.

15. The data processing system of claim 14, wherein the wireless connection supports communication of the information using at least one of Bluetooth, Bluetooth low energy (BLE), near field communication (NFC), radio-frequency identification (RFID), and WiFi.

16. A method of operating an electrocardiogram (ECG) sensor chip receiving a first ECG signal and a second ECG signal and being incorporated in a wearable appliance worn by a user, the method comprising:

- generating a switching signal;

- using the switching signal to control operation of a switch, wherein, in response to the switching signal having a first state, the first ECG signal passes from a first switch input to a first switch output and the second ECG signal passes from a second switch input to a second switch output, else in response to the switching signal having a second state, the first ECG signal passes from the first

switch input to the second switch output and the second ECG signal passes from the second switch input to the first switch output; and
amplifying a difference between the first ECG signal and the second ECG signal using an amplifier connected to the first switch output and the second switch output.

17. The method of claim **16**, wherein the generating of the switching signal comprises:
receiving a location indication signal from a user-activated location input element and generating the switching signal in response to the location indication signal, wherein the user-activated location input element is activated or deactivated in response to a location of the wearable appliance worn by the user.

18. The method of claim **17**, wherein the user-activated location input element is one of a mechanical button disposed on the wearable appliance, an icon of a graphical user interface presented on a display disposed on the wearable appliance, and a user input device disposed on a computing device wirelessly connected to the wearable appliance.

19. The method of claim **16**, wherein the generating of the switching signal comprises:
peak detecting the first ECG signal and peak detecting the second ECG signal to obtain a peak-detected first ECG signal and a peak-detected second ECG signal; and
generating the switching signal in response to a difference between the peak-detected first ECG signal and the peak-detected second ECG signal.

20. The method of claim **16**, further comprising:
generating ECG digital signals from the amplified difference between the first ECG signal and the second ECG signal;
generating control signal/data from the ECG digital signals; and
using the control signal/data to control a display displaying an image visible to the user that indicates a health condition related to at least one of the first ECG signal and the second ECG signal.

* * * * *

专利名称(译)	心电图 (ECG) 传感器芯片 , 芯片上系统 (SoC) 和可佩戴的器具		
公开(公告)号	US20180235504A1	公开(公告)日	2018-08-23
申请号	US15/958908	申请日	2018-04-20
[标]申请(专利权)人(译)	三星电子株式会社		
申请(专利权)人(译)	SAMSUNG ELECTRONICS CO. , LTD.		
当前申请(专利权)人(译)	SAMSUNG ELECTRONICS CO. , LTD.		
[标]发明人	SHIN SEUNG CHUL KO HYUNG JONG KIM JUNG SU PARK YONG IN JUNG WON HYUK HAN YUN CHEOL		
发明人	SHIN, SEUNG CHUL KO, HYUNG JONG KIM, JUNG SU PARK, YONG IN JUNG, WON HYUK HAN, YUN CHEOL		
IPC分类号	A61B5/0428 A61B5/00 A61B5/0432 A61B5/0404 A61B5/0456		
CPC分类号	A61B5/6824 A61B5/0456 A61B5/04325 A61B5/0404 A61B5/04288 A61B5/6833 A61B5/7225 A61B5/6803 A61B5/681 A61B5/746		
优先权	1020140160011 2014-11-17 KR		
外部链接	Espacenet USPTO		

摘要(译)

用于可穿戴设备的ECG传感器芯片包括：由开关信号控制的开关，放大第一和第二ECG信号之间的差的放大器，以及产生开关信号的位置指示器。响应于切换信号，开关传递第一ECG信号或第二ECG信号。

