

US010052042B2

(12) **United States Patent**  
**Jain et al.**

(10) **Patent No.:** **US 10,052,042 B2**  
(45) **Date of Patent:** **Aug. 21, 2018**

(54) **CONTACTLESS ELECTRIC CARDIOGRAM SYSTEM**

(58) **Field of Classification Search**  
CPC ..... A61B 5/04085; A61B 5/04284; A61B 2562/0214

(71) Applicant: **RR Sequences Inc.**, Montreal (CA)

See application file for complete search history.

(72) Inventors: **Deepak Bobby Jain**, Brossard (CA); **Joshua Weeks**, Montreal (CA); **David Nadezhdin**, Montreal (CA); **Jean-Francois Asselin**, Brossard (CA)

(56) **References Cited**

U.S. PATENT DOCUMENTS

(73) Assignee: **RR SEQUENCES INC.**, Montreal, Quebec (CA)

6,553,246 B1 4/2003 Wenger  
6,584,343 B1 6/2003 Ransbury et al.  
(Continued)

(\* ) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 272 days.

FOREIGN PATENT DOCUMENTS

(21) Appl. No.: **14/893,293**

DE 102010034192 A1 2/2012  
GB 2489704 A 10/2012  
(Continued)

(22) PCT Filed: **Sep. 23, 2015**

OTHER PUBLICATIONS

(86) PCT No.: **PCT/CA2015/050938**

European Application No. 15794450, Supplementary European Search Report, dated Apr. 5, 2017.

§ 371 (c)(1),

(2) Date: **Nov. 23, 2015**

(Continued)

(87) PCT Pub. No.: **WO2016/044933**

PCT Pub. Date: **Mar. 31, 2016**

*Primary Examiner* — Michael Kahelin  
(74) *Attorney, Agent, or Firm* — Michael G. Johnston; Moore & Van Allen PLLC

(65) **Prior Publication Data**

US 2016/0287128 A1 Oct. 6, 2016

**Related U.S. Application Data**

(60) Provisional application No. 62/206,542, filed on Aug. 18, 2015, provisional application No. 62/054,189, filed on Sep. 23, 2014.

(57) **ABSTRACT**

(51) **Int. Cl.**

**A61B 5/0408** (2006.01)

**A61B 5/0402** (2006.01)

(Continued)


A system for providing a standard electrocardiogram (ECG) signal for a human body using contactless ECG sensors for outputting to existing medical equipment or for storage or viewing on a remote device. The system comprises a digital processing module (DPM) adapted to connect to an array of contactless ECG sensors provided in a fabric or the like. A selection mechanism is embedded into the DPM which allows the DPM to identify body parts using the ECG signals of the different ECG sensors and select for each body part the best sensor lead. The DPM may then produce the standard ECG signal using the selected ECG signals for the different body parts detected. The system is adapted to continuously re-examine the selection to ensure that the best leads are selected for a given body part following a move-

(Continued)

(52) **U.S. Cl.**

CPC ..... **A61B 5/04085** (2013.01); **A61B 5/0402** (2013.01); **A61B 5/0424** (2013.01);

(Continued)

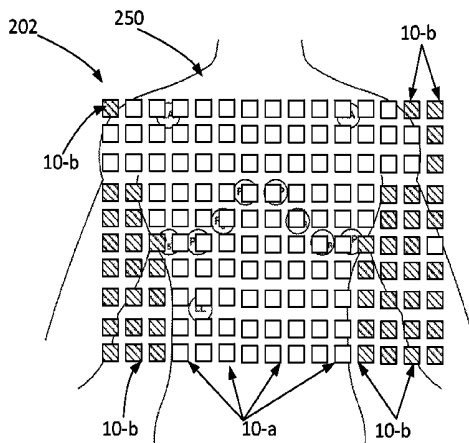

ment of the body part, thereby, allowing for continuous and un-interrupted ECG monitoring of the patient.

**20 Claims, 10 Drawing Sheets**

9,037,221	B2	5/2015	Bocko et al.	
2005/0113703	A1	5/2005	Farringdon et al.	
2009/0138059	A1	5/2009	Ouwerkerk	
2013/0204100	A1*	8/2013	Acquista .....	A61B 5/0006 600/301
2015/0054495	A1	2/2015	Lem et al.	
2015/0094603	A1	4/2015	Eilebrecht	

(51) **Int. Cl.**

- A61B 5/00* (2006.01)
- A61B 5/0424* (2006.01)
- A61B 5/0428* (2006.01)
- A61B 5/11* (2006.01)
- A61B 5/04* (2006.01)

(52) **U.S. Cl.**

- CPC ..... *A61B 5/04028* (2013.01); *A61B 5/04284* (2013.01); *A61B 5/1114* (2013.01); *A61B 5/6844* (2013.01); *A61B 5/7221* (2013.01); *A61B 5/0006* (2013.01); *A61B 5/04012* (2013.01); *A61B 2562/0214* (2013.01); *A61B 2562/046* (2013.01); *A61B 2562/164* (2013.01)

(56) **References Cited**

U.S. PATENT DOCUMENTS

8,792,957	B2	7/2014	Greene et al.
8,897,860	B2	11/2014	Volpe et al.

FOREIGN PATENT DOCUMENTS

KR	101227413	B1	2/2013
WO	2009074955	A1	6/2009

OTHER PUBLICATIONS

Serteyn A et al; "Motion Artifacts in Capacitive ECG Measurements: Reducing the Combined Effect of DC Voltages and Capacitance Changes Using an Injection Signal," IEEE Transactions on Biomedical Engineering, 2004, pp. 264-273, vol. 62.

Wartzek T et al; "ECG on the Road: Robust and Unobtrusive Estimation of Heart Rate," IEEE Transactions on Biomedical Engineering, 2011, pp. 3112-3120, vol. 58.

RR Sequences Inc., Canadian Patent Application No. 2,911,304, Office Action, dated Mar. 24, 2016.

RR Sequences Inc., International Application No. PCT/CA2015/050938, International Search Report, dated Dec. 2, 2015.

\* cited by examiner

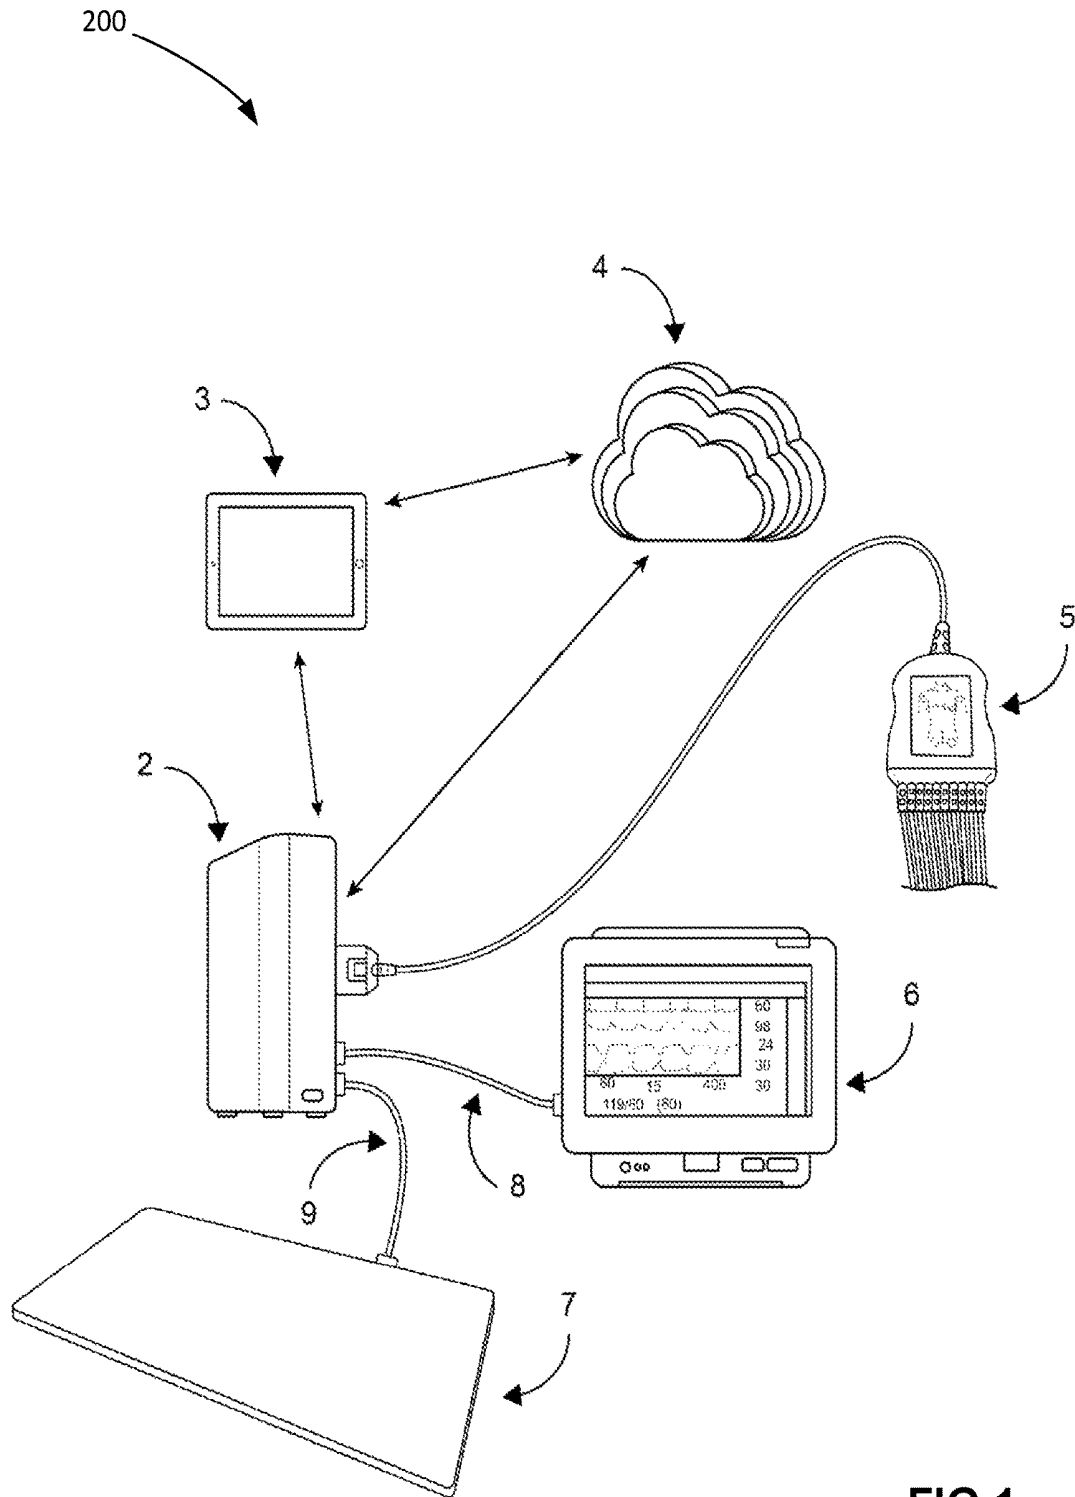


FIG.1

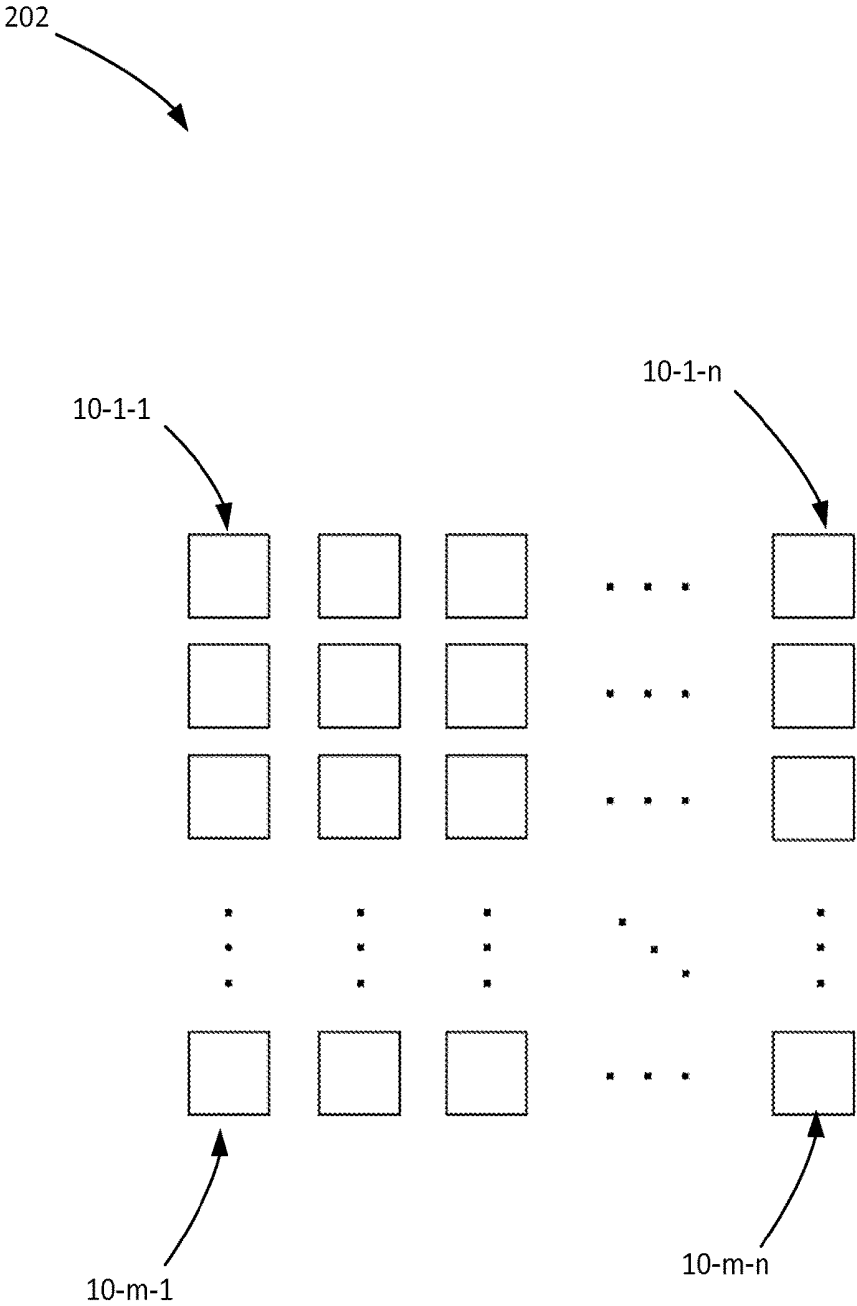


FIG.2

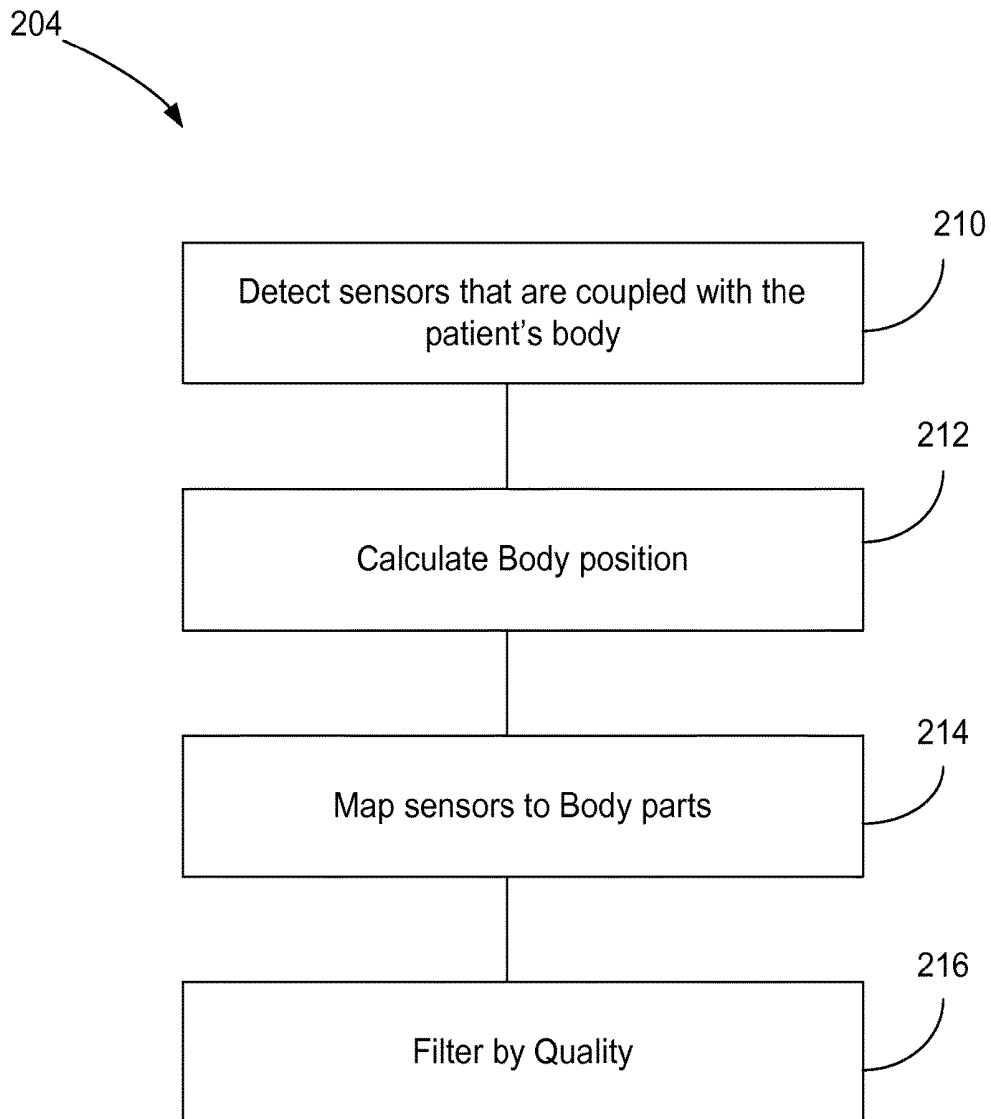


FIG.3

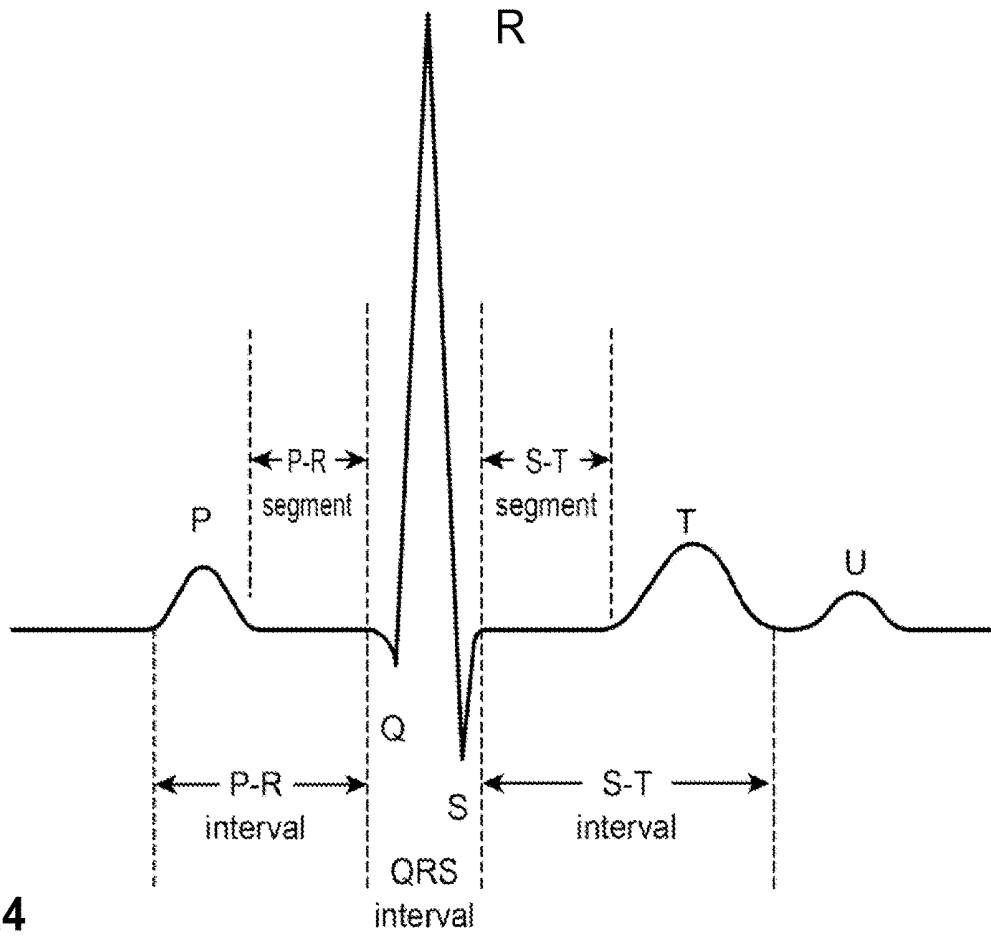


FIG.4

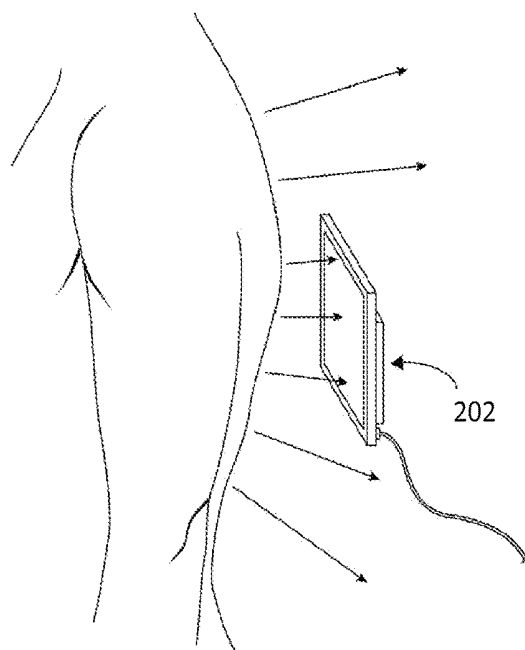


FIG.5

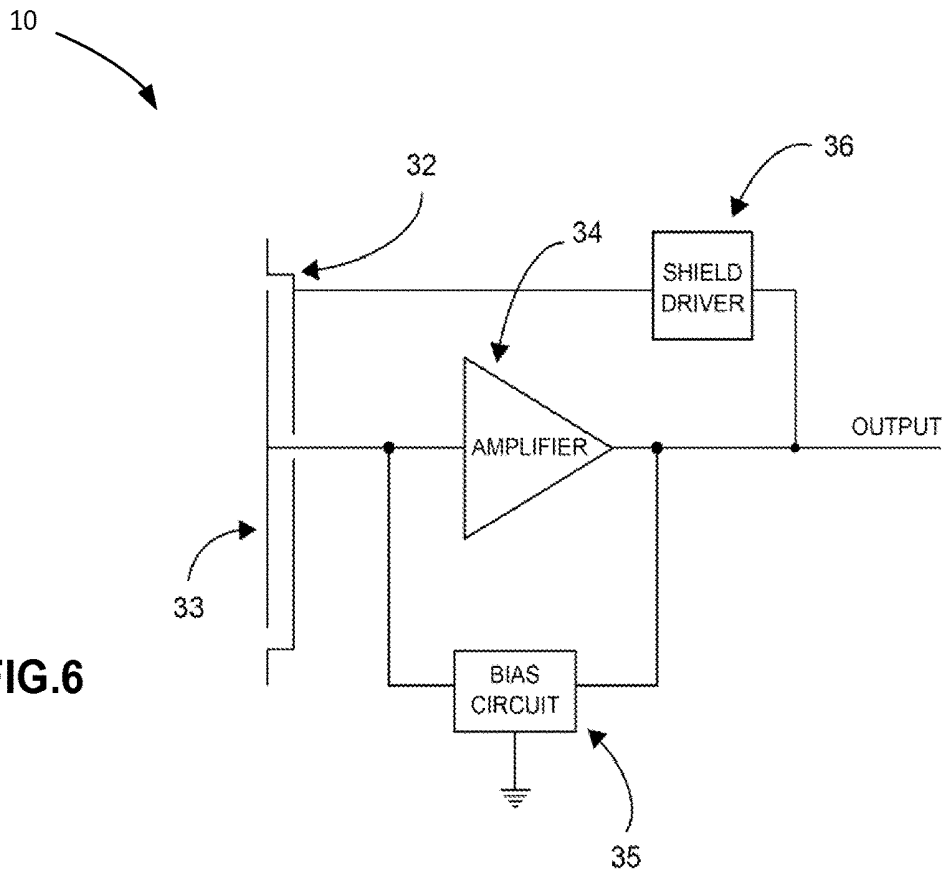


FIG. 6

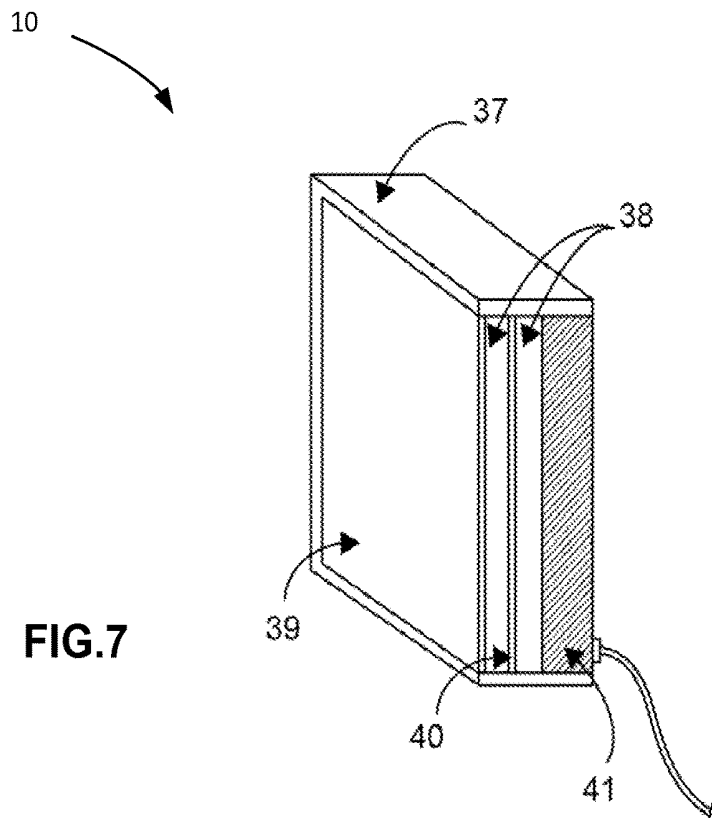


FIG. 7

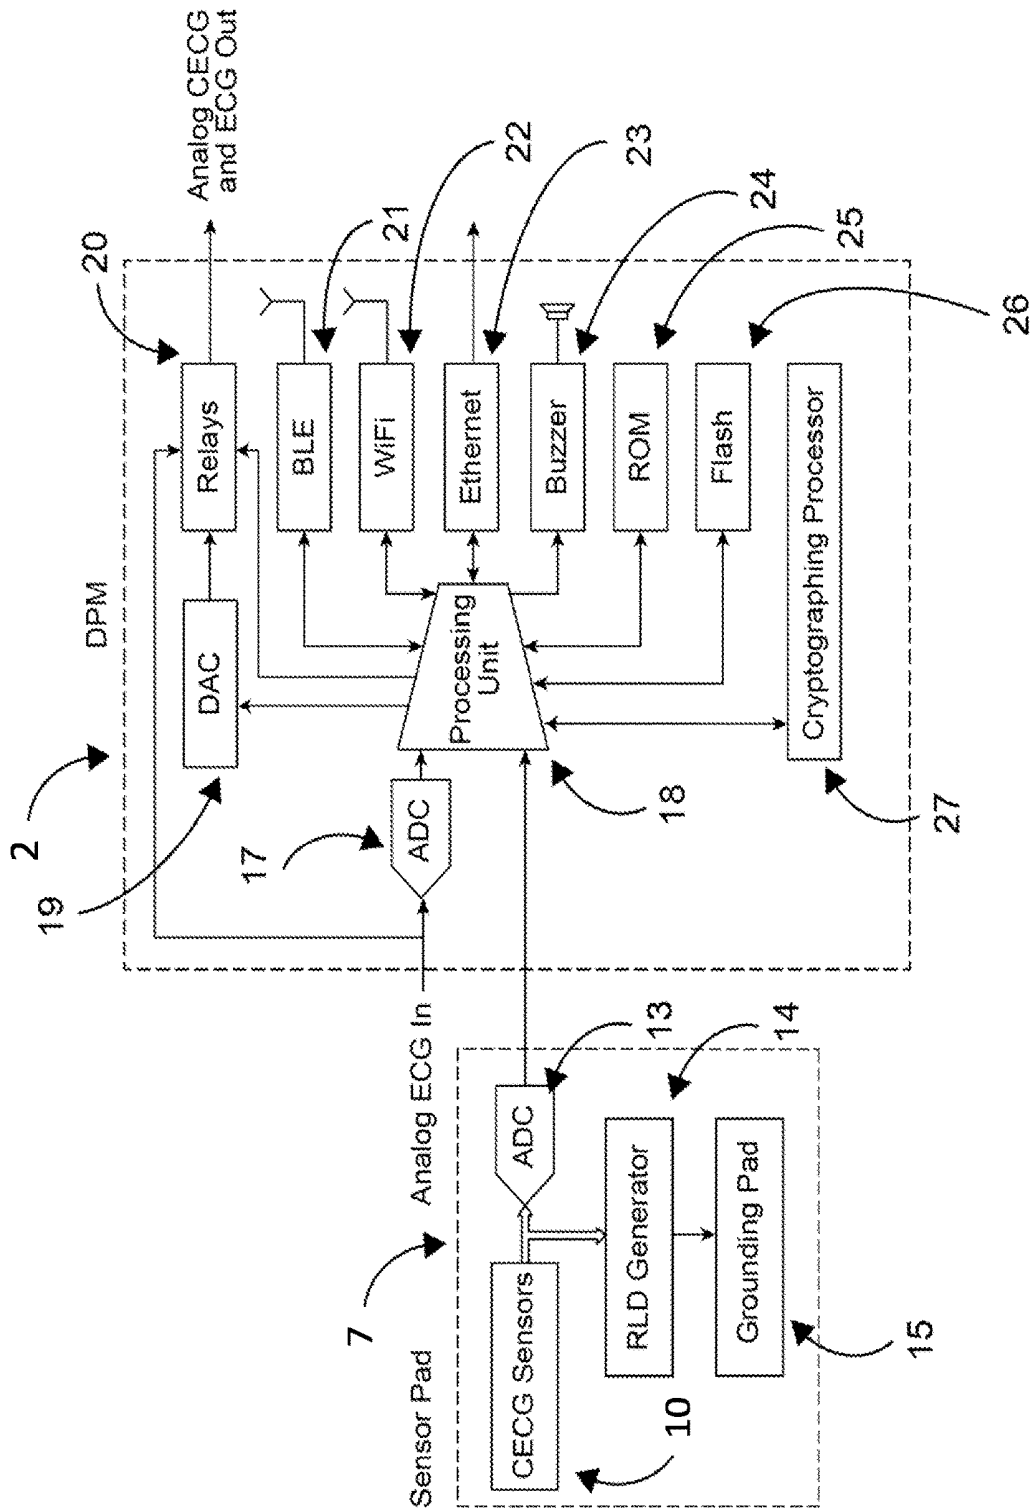


FIG. 8

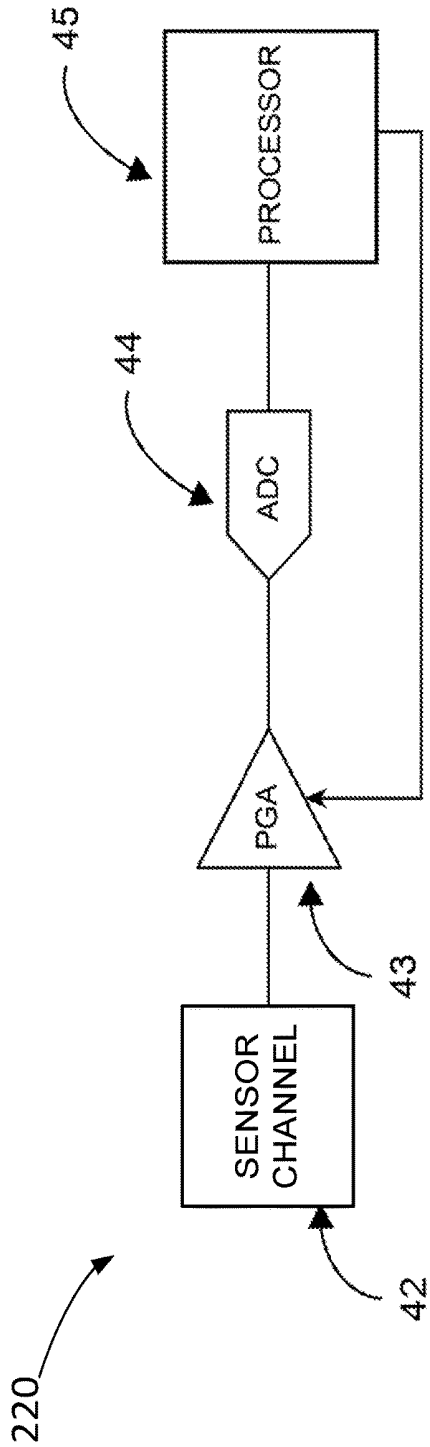


FIG.9

14

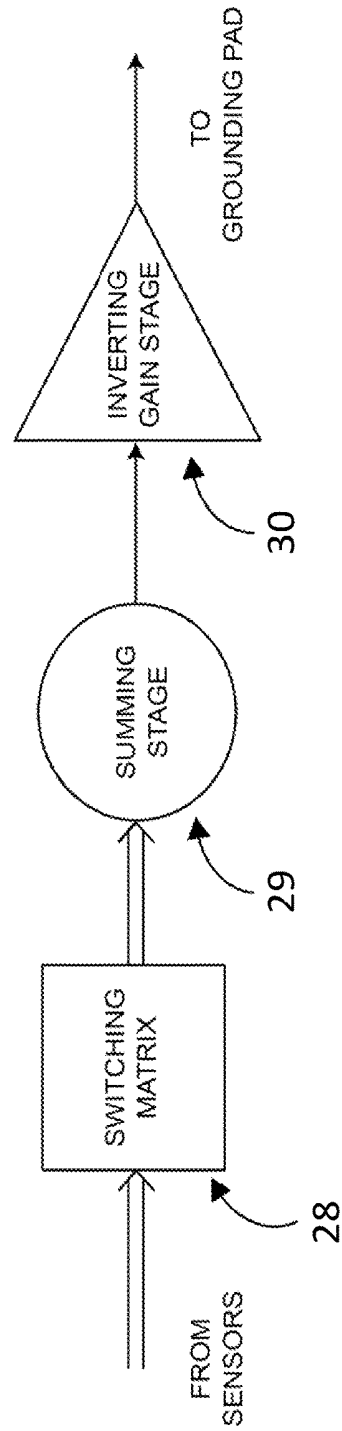


FIG.10

FIG.11

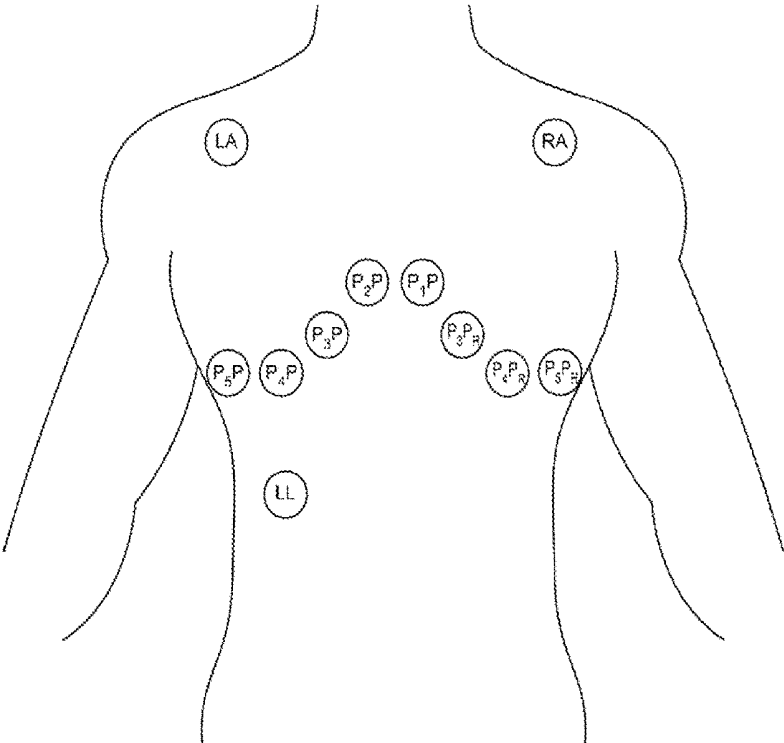
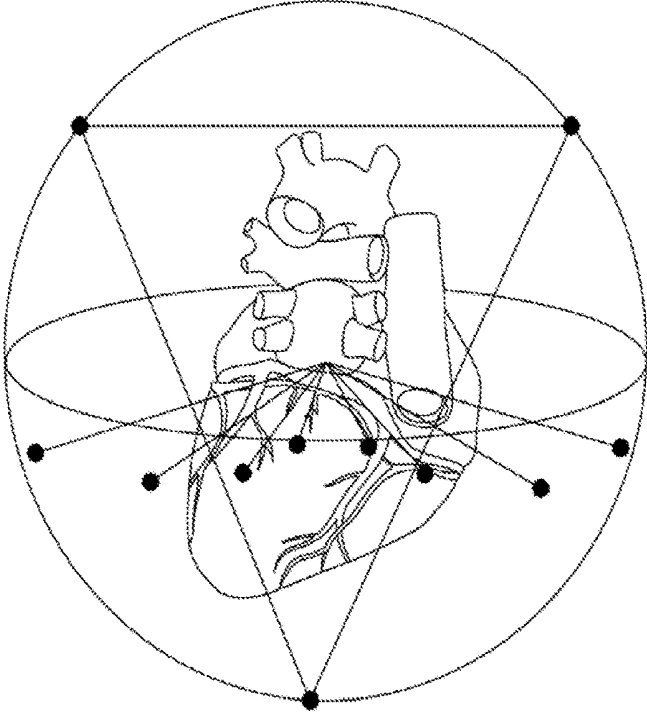


FIG.12



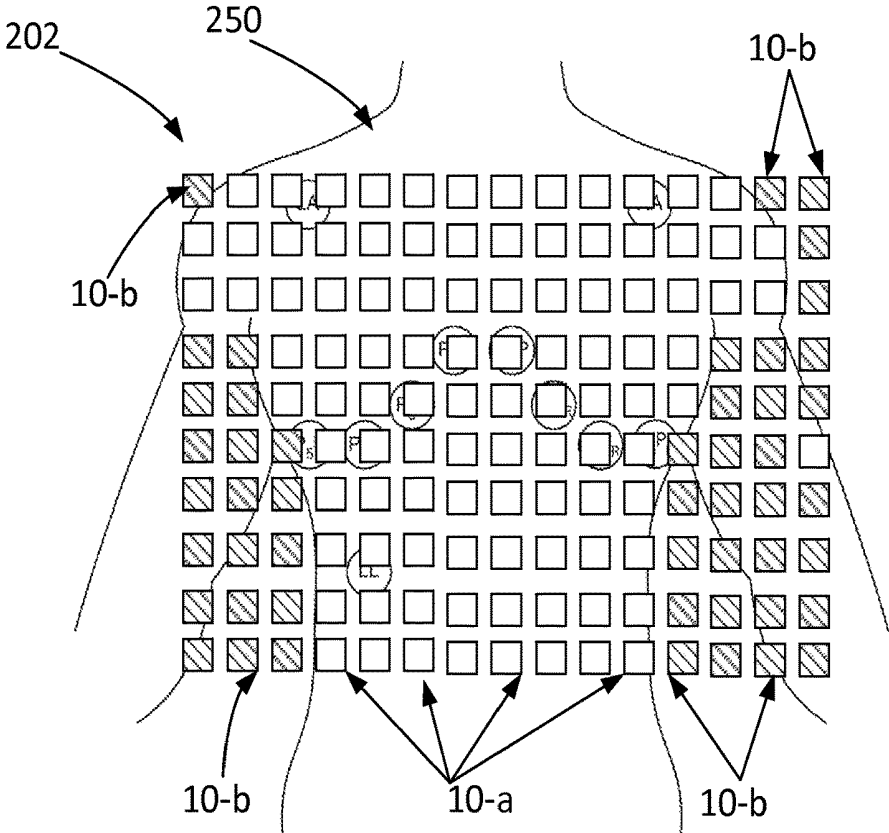


FIG.13a

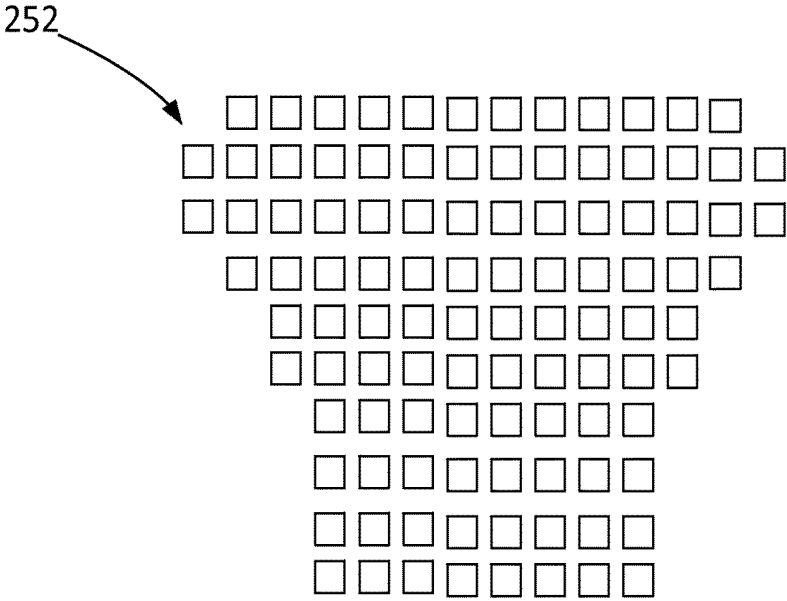


FIG.13b

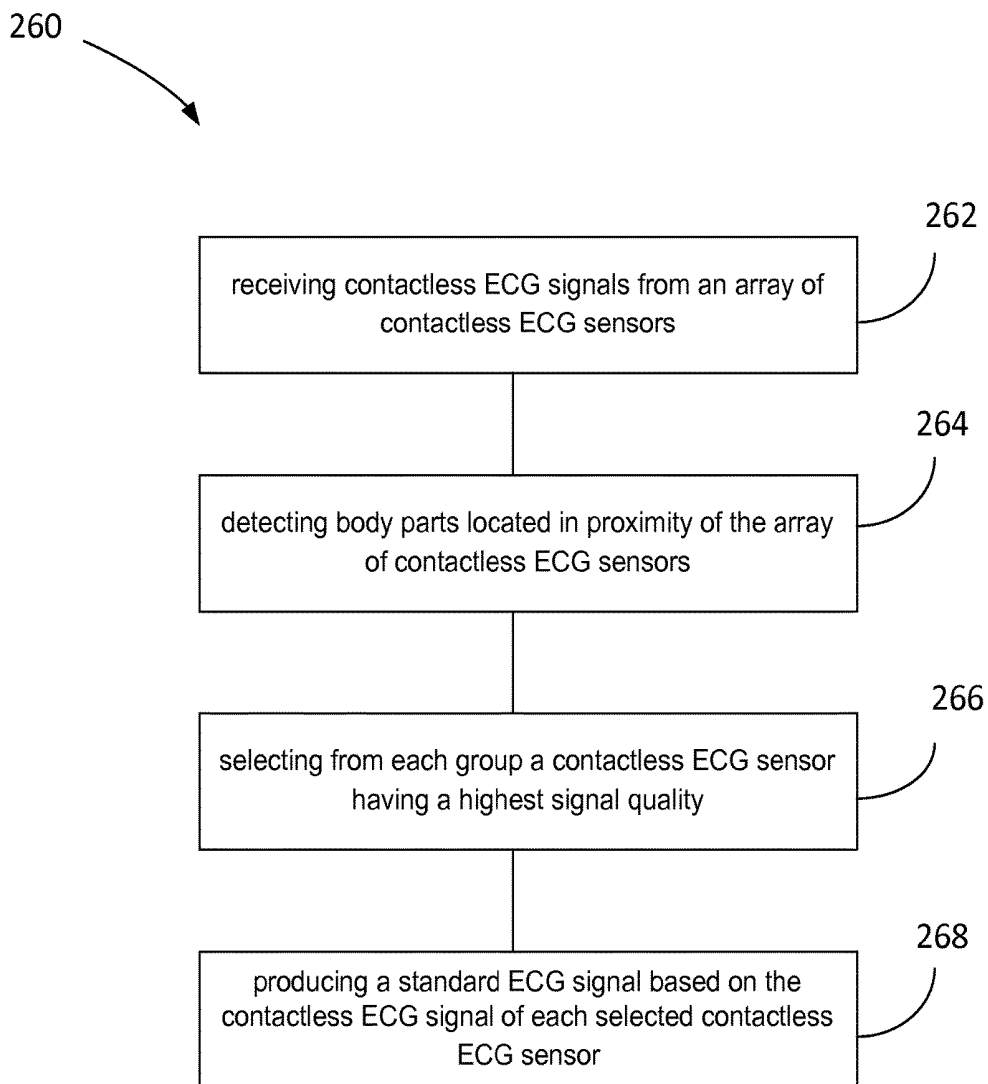


FIG.14

## CONTACTLESS ELECTRIC CARDIOGRAM SYSTEM

### CROSS-REFERENCE TO RELATED APPLICATIONS

This application claims priority under of U.S. provisional patent application 62/054,189 filed on Sep. 23, 2015 and U.S. provisional patent application 62/206,542 filed on Aug. 18, 2015, the specifications of which are hereby incorporated by reference.

### BACKGROUND

#### (a) Field

The subject matter generally relates to electro-cardiogram systems.

#### (b) Related Prior Art

Electrocardiograms (hereinafter ECG's) are the only reliable measurement of heart rate, arrhythmia detection, resting ECG abnormalities that necessitate mandatory further testing, changes from previous ECG's.

The ECG is one of the basic diagnostic and follow up screening tools used in medicine for a large number of cardiac and non-cardiac diseases. While the standard 12-lead electrocardiogram holds a wealth of information, it only captures data for 10 seconds. Long term monitoring with multiple leads provides even more information and leads to better access to changes in the electrocardiogram.

The lack of long term monitoring is an important medical problem for multiple reasons. The lack of a baseline electrocardiogram in a patient's file often results in confusion and needless additional exams in patients who have ECGs done for the first time which are normal for them, but abnormal according to established criteria. Often, if an old ECG, even one from 10 years prior, is available that is the same as the perceived abnormal ECG, no further exams are required. In other words, the ability to compare a current ECG to an old one is of immense medical value. An unchanged one results in fewer examinations.

Traditional electrocardiographic measurement systems that rely on contact electrodes (electrodes which form a galvanic connection with the patient's body) present challenges when ECG monitoring is required immediately, unobtrusively or frequently. Traditional contact electrodes require placement by a trained healthcare provider on a clean, prepared skin surface to ensure accurate location (and therefore morphology) and signal quality. Limitations of standard wet gel contact electrode placement include placing them on the body correctly and removing them within their time limit to avoid skin reactions.

Apart from their inability to provide long term monitoring, their availability is also limited as discussed below.

Ideally, ECGs should be performed on all patients as part of the routine medical visit, especially if the patient has symptoms that necessitate medical attention. However, the availability of the test is limited. Their availability is limited due to the cost of the ECG equipment and the un-availability of the technicians needed to perform the test on patients to put the leads on the patient correctly. With respect to ECG costs, most physicians do not invest in having the test on site. Even in hospitals, telemetry units are limited to about 6 to 10 units located outside of the intensive care units for the entire patients in a large hospital.

Another disadvantage is that standard electrodes have multiple problems that limit proper and widespread use of the ECG. These problems are:

1. The electrodes react with the skin due to the metal, gel, and adhesive reactions, which requires multiple changes during a hospital stay;
2. The lack of knowledge required to correctly place the electrodes;
3. The time for placing the electrodes;
4. The complications associated with extended monitoring such as when the electrodes fall off regularly due to sweat, patient's movement, improper placement, etc;
5. ECG's derived using standard electrodes are prone to muscular artifacts that result in false ECG's.

A further disadvantage is that the electrocardiogram obtained with standard electrodes is labor and material intensive. Even a telemetry unit can take, in certain cases, upwards of 2-3 hours per day per patient of nursing time to install and re-install standard electrodes.

Yet a further disadvantage is that ECGs are a source of nosocomial infection spread in hospitals because of wires and their contact with nursing and hospital staff, and frequent nursing attention to the electrodes.

Accordingly, there is a need in the market for a system and method which address the shortcomings addressed above.

### SUMMARY

The embodiments describe an ECG system which allows for frequent, inexpensive and accessible recording of ECG data from any patient or person easily, unobtrusively and quickly by eliminating the need to manually identify and prepare areas on the patient's body for contact sensors and to place sensors on those areas. The described system circumvents issues associated with contact electrodes by being contactless and by allowing multi-hour, multiple lead monitoring on a daily basis and for life.

In one aspect, there is provided a medical apparatus (aka DPM) for providing electrocardiogram (ECG) signals for a human body using contactless ECG sensors, the medical apparatus comprising: an input adapted to receive contactless ECG signals from an array of contactless ECG sensors; a processor adapted to perform a selection process including: detecting body parts located in proximity of the array of contactless ECG sensors; associating a group of contactless ECG sensors with each detected body part; selecting from each group a contactless ECG sensor having a highest signal quality; the processor being adapted to produce a standard ECG signal based on the received contactless ECG signal of each selected contactless ECG sensor; and an output for sending the standard ECG signal.

The Medical apparatus may be a lightweight portable device that weighs less than 2 lbs.

In an embodiment, the selection process further comprises the steps of: obtaining a body outline of the human body using the contactless ECG signals associated with the contactless ECG sensors located in proximity of the human body; determining a position of the human body on the array of contactless ECG sensors; dividing the contactless ECG sensors into groups and associating each group to a body part using the body outline and the position of the human body; and from each group, selecting the contactless ECG sensor providing the contactless ECG signal having the highest quality.

In an embodiment, the processor may identify the contactless ECG sensors that are located in close proximity to the human body by measuring an impedance between each contactless ECG sensor and the human body.

In another embodiment, the medical apparatus may be adapted to select another contactless ECG sensor for a given

body part following a movement of the human body with respect to the array of contactless ECG sensors. In a further embodiment, the processor may be adapted to re-run the selection process continuously to perform the selection of the other contactless ECG sensor. The processor may also be adapted to continuously monitor a signal quality of the selected contactless ECG sensor associated with each body part to re-run the selection process when the signal quality drops beyond a given threshold.

The medical apparatus may comprise different operation modes comprising: a contactless mode which outputs a first standard ECG signal resulting from the contactless ECG signals; a hybrid mode which outputs a second standard ECG signal resulting from the contactless ECG signals and conventional ECG signals received from conventional contact electrodes; and a bypass mode which outputs a third standard ECG signal resulting from conventional ECG signals received from conventional contact electrodes.

The medical apparatus may further comprise an automatic gain control mechanism adapted to control relative impedance differences between different contactless ECG sensors and absolute impedance of each contactless ECG sensor to the human body due to a difference in distance or clothing materials between each contactless ECG sensor and the human body.

A wired/wireless data port may be provided for transmitting the standard ECG signal to a remote device over a data network.

In another aspect, a system for providing electrocardiogram (ECG) signals for a human body using contactless ECG sensors, the system comprising: a sensor pad comprising an array of contactless ECG sensors; a processor operatively connected to the sensor pad and adapted to receive contactless ECG signals from the contactless ECG sensors and perform a selection process including: detecting body parts located in proximity of the array of contactless ECG sensors; associating a group of contactless ECG sensors with each detected body part; selecting from each group a contactless ECG sensor having a highest signal quality; the processor being adapted to produce a standard ECG signal based on the contactless ECG signal of each selected contactless ECG sensor; and an output for sending the standard ECG signal.

In an embodiment, the sensor pad comprises a grounding pad for placing in proximity of and at distance from the human body, the grounding pad being adapted to provide a capacitively coupled ground reference to the human body for reducing interference.

In another embodiment, the grounding pad may be driven with a feedback signal derived from the contactless ECG signals.

The system may further comprise a drive signal generator configured to feed the grounding pad with a high frequency signal that is outside of an ECG frequency band for determining the capacitively coupled ground reference for each contactless ECG sensor.

In an embodiment, the contactless ECG sensor may comprise: a capacitive electrode adapted to be capacitively coupled to the human body for outputting an electrical charge which is representative of an electrical cardiac activity; an electrodynamic sensor configured to detect and amplify the electrical charge produced by the capacitive electrode; and an electrode shield physically provided in proximity of the electrode for reducing a stray interference at an input of the electrodynamic sensor.

The contactless ECG sensor may be made of a flexible material.

In an embodiment, the sensor pad may be provided in a fabric with which the human body comes in contact.

In a further aspect, there is provided a method for providing electrocardiogram (ECG) signals for a human body using contactless ECG sensors, the method comprising: receiving contactless ECG signals from an array of contactless ECG sensors; detecting body parts located in proximity of the array of contactless ECG sensors; associating a group of contactless ECG sensors with each detected body part; selecting from each group a contactless ECG sensor having a highest signal quality; and producing a standard ECG signal based on the contactless ECG signal of each selected contactless ECG sensor.

The method may further comprise obtaining a body outline of the human body using the contactless ECG signals associated with the contactless ECG sensors located in proximity of the human body; determining a position of the human body on the array of contactless ECG sensor; dividing the contactless ECG sensors into groups and associate each group to a body part using the body outline and the position of the human body; and from each group, selecting the contactless ECG sensor providing the contactless ECG signal having the highest quality.

In an embodiment, the method further comprises identifying the contactless ECG sensors that are located in close proximity to the human body by measuring an impedance between each contactless ECG sensor and the human body.

The method may further repeat the steps of detecting to selecting continuously for selecting another contactless ECG sensor for a given body part following a movement of the human body with respect to the array of contactless ECG sensors. In one embodiment, it is possible to continuously monitor a signal quality of the selected contactless ECG sensor associated with each body part and repeat the steps of detecting to selecting for selecting another contactless ECG sensor for a given body part when the signal quality drops beyond a given threshold following a movement of the human body with respect to the array of contactless ECG sensors.

The following terms are defined below:

The term lead is intended to mean a difference in measured voltage between two locations on the human body that provide and show PQRSTU waveforms.

The term ECG lead is intended to mean a medically defined ECG signal based on a difference in measured voltage between two medically defined locations on the human body.

Standard ECG signal is an ECG signal that interfaces with existing medical equipment and conforms to ECG standards. A standard ECG signal may include a single rhythm strip or any number of standard medically defined ECG leads.

A rhythm strip is any lead that shows the rhythm between the PQRSTU waveforms. The rhythm strip does not require that the ECG signal be taken from the medically defined ECG locations.

Features and advantages of the subject matter hereof will become more apparent in light of the following detailed description of selected embodiments, as illustrated in the accompanying figures. As will be realized, the subject matter disclosed and claimed is capable of modifications in various respects, all without departing from the scope of the claims. Accordingly, the drawings and the description are to be regarded as illustrative in nature, and not as restrictive and the full scope of the subject matter is set forth in the claims.

## BRIEF DESCRIPTION OF THE DRAWINGS

Further features and advantages of the present disclosure will become apparent from the following detailed description, taken in combination with the appended drawings, in which:

FIG. 1 is a block diagram of an exemplary ECG system in accordance with an embodiment;

FIG. 2 illustrates a non-limiting example of a sensor matrix in accordance with an embodiment;

FIG. 3 is a flowchart illustrating the main steps performed by the selection algorithm, in accordance with an embodiment;

FIG. 4 illustrates an example of a full PQRSTU waveform obtained for a patient using a system in accordance with an embodiment;

FIG. 5 illustrates how the sensor array captures ECG signals without direct contact with the patient's skin;

FIG. 6 is a block diagram illustrating an exemplary sensor design of a contactless ECG sensor, in accordance with an embodiment;

FIG. 7 illustrates an example of a physical design of a contactless ECG sensor, in accordance with an embodiment;

FIG. 8 illustrates an exemplary block diagram of an overall design of a system in accordance with an embodiment;

FIG. 9 is a block diagram illustrating an exemplary gain control mechanism, in accordance with an embodiment

FIG. 10 is an exemplary block diagram illustrating the function of the RLD generator, in accordance with an embodiment

FIG. 11 shows medically recognized ECG locations for obtaining standard ECG leads;

FIG. 12 illustrates an example of standard ECG leads, each lead being shown as a vector between two locations on the human body;

FIGS. 13a&13b illustrate an example of how the system determines the body outline of the patient; and

FIG. 14 is flowchart of a method for providing electrocardiogram (ECG) signals for a human body using contactless ECG sensors.

It will be noted that throughout the appended drawings, like features are identified by like reference numerals.

## DETAILED DESCRIPTION

A system for providing a standard electrocardiogram (ECG) signal for a human body using contactless ECG sensors for outputting to exiting medical equipment (as well as to new/dedicated monitors, or for viewing on a display device associated with a computing device) or for storage or viewing on a remote/local device. The system comprises a digital processing module (DPM) adapted to connect to an array of contactless ECG sensors provided in a fabric or the like. A selection mechanism is embedded into the DPM which allows the DPM to identify body parts using the ECG signals of the different ECG sensors and select for each body part the best sensor lead. The DPM may then produce the standard ECG signal using the selected ECG signals for the different body parts detected. The system is adapted to continuously re-examine the selection to ensure that the best leads are selected for a given body part following a movement of the body part, thereby, allowing for continuous and un-interrupted ECG monitoring of the patient.

The present invention will be more readily understood by referring to the following examples which are given to illustrate the invention rather than to limit its scope.

Referring now to the drawings, FIG. 1 is a block diagram of an exemplary ECG system 200 in accordance with an embodiment. As shown in FIG. 1 the system 200 comprises an array of contactless sensors provided in a sensor pad 7 (in a non-limiting example of implementation), and a digital processing module (DPM) 2 which is operatively connected to the array of sensors using a cable 9 for obtaining sensor readings from the sensors provided in the pad 7. The DPM 2 may be configured to simultaneously record the electrophysiological activity of the heart (body surface potential map) as well as identify the best electrodes/sensors to output a standards ECG signal (+posterior precordials) into existing medical equipment (6). The DPM may be connected to a mobile device (3) or the cloud (4) via the internet or a data network to make the data readily available for doctors and in real-time so that doctors can quickly diagnose arrhythmic and ischemic changes detected by the DPM 2.

In a non-limiting example, the DPM 2 may be provided as a lightweight portable medical device which weighs about 2 lbs or less and may be carried around for performing the continuous ECG monitoring.

As stated above, the DPM 2 may be configured to produce an output signal which conforms to existing medical standards so that the output signal is identical to those that are acquired by a standard contact ECG system and may be viewed/read using existing medical equipment 6 in a plug and play manner (whereby no changes are to be made to the existing medical equipment to read and output the standard ECG signal received from the DPM). The DPM 2 may include a data output plug adapted to receive a standard cable (8) to output a signal that be simultaneously read using an existing medical equipment 6. The DPM 2 may also be able to simultaneously record contact ECG information if a standard trunk cable 5 is attached.

However, the DPM 2 may also have its own display device embedded in it or associated with it and may be adapted to send/stream the standard ECG signal via a communications/data network to make the standard ECG signal available on a local/remote personal computer or portable device.

It should be noted that FIG. 1 illustrates a non-limiting example of implementation. Changes to the system 200 are possible without departing from the scope of the invention as defined in the claims. For example, although FIG. 1 illustrates cables for communicating the data between different modules, it is also contemplated that wireless connections may be used including but not limited to: Wi-Fi, Bluetooth etc.

Furthermore, the sensor array may be in a variety of other objects including: clothing, beds, and vehicle devices/components. In another example, the sensor array may be provided in a plurality of devices including but not limited to: furniture (e.g. chair, bed/mattress/cover, sofa, seat, mattress), in-vehicle devices (e.g. seat, headrest, steering wheel etc.), or in a wearable device (e.g. jacket, shirt, t-shirt, sweater, bra etc.).

## Selection Algorithm

Traditional ECG dictates electrode locations that are based on physiology of the patient whereby traditional contact electrodes are adhered to these locations, maintaining relative body position regardless of the patient's movement. For example, the V1 electrode should be placed on the 4<sup>th</sup> intercostal space to the right of the sternum, the RA electrode should be placed on the right arm, the LA electrode on the same location as the RA electrode but on the left arm the RL electrode should be placed on the right leg, lateral calf muscle and so on . . . as exemplified in FIG. 11. The

importance of these electrodes and their locations lies in the fact that the difference in voltage between two specific locations represents a medically defined ECG lead (as discussed with respect to FIGS. 11 and 12), and the lead in electrocardiography represents a vector along which the heart's depolarization is measured and recorded to produce the electrocardiogram.

Therefore in order to produce an ECG signal that is compatible with traditional ECG standards it is necessary to follow the same principle although data is being collected in a contactless manner.

FIG. 2 illustrates a non-limiting example of a sensor matrix 202 in accordance with an embodiment. As shown in FIG. 2 the matrix 202 comprises n columns and m rows of sensors 10 arranged in a matrix configuration such that no matter how the patient is placed on the matrix 202, there would always be at least one sensor at a location on the patient's body that corresponds to the physical placement of a conventional ECG electrode. Using an adaptive algorithm embedded in the DPM 2, the matrix 202 may be used for obtaining a continuous ECG reading by selecting a given sensor 10 from the matrix 202 which corresponds to a defined ECG location on the patient's body.

FIG. 3 is a flowchart illustrating the main steps performed by a selection algorithm 204, in accordance with an embodiment. At step 210 the algorithm detects which sensors 10 are in close proximity to the patient's body, by measuring the impedance between each sensor 10 and the patient. This allows for detecting the sensors 10 that can be used to obtain data from. ECG signals output by these sensors 10 (the ones determined to be in close proximity of the body) are then analyzed to obtain a body outline of the patient.

In a non-limiting example of implementation, the embodiments may use different types of information to obtain the body outline. The first type is the coupling impedance which represents the distance between the body and the sensor. When the coupling impedance is too high, the sensor is too far from the body and cannot be used. The second type is the signal itself e.g. morphology of the signal and how the signal looks like to see whether the signal has the usual ECG pattern or not (PQRSTU waveforms). The third type of information relates to the geometrical locations of the ECG sensors providing good ECG signals. These sensors and their location provide an indication on the geometrical shape of the human body as exemplified in FIGS. 13a and 13b. In the example of FIG. 13a, assuming that a user 250 is laying down on a mattress having the sensor pad 202 embedded therein, the sensors 10a that are in proximity of the patient's body will obtain a good ECG signals while the sensors 10b outside of the patient's body will not obtain a good signal. Based on this information and the location of each sensor on the pad 202, the DPM 2 may obtain an outline 252 of the patient's body from which the DPM may determine the shape, width and other dimensions of the patient's body as exemplified in FIG. 13b. Using this information and a set of rules embedded in the DPM 2, the DPM 2 may then detect/determine locations of body parts and associate one or more sensors 10 with each body part/body location for ECG purposes as discussed below.

At step 212 the algorithm analyses the ECG signal received from the sensors and combines it with the body outline already detected to find the position of the patient's body on the pad. At step 214 the algorithms performs a mapping of where on the body each sensor 10 is located using the information obtained from steps 210 and 212. Once groups of sensors are found to be near each major body part for ECG purposes (Right Arm, Left Arm, etc.), the

signals from those adjacent sensors are compared and filtered at step 216 to select a single sensor with the best ECG signal to receive and record therefrom ECG data for that respective body part.

In an embodiment, the DPM 2 may be adapted to run the selection algorithm 204 continuously and dynamically in order to re-examine the readings obtained from the sensors 10 in real time to re-verify the selection of the sensor 10 having the best ECG reading to constantly take into consideration the patient's movement whereby a new sensor 10 may be selected which provides a better reading than the one previously selected before the movement.

In another embodiment, the system may detect when a patient moves and determines when it is necessary to run the algorithm again to recalculate whether or not a new selection needs to be made. For example, the system may monitor the signal's strength/quality and determine to re-run the selection algorithm 204 when the signal quality drops below a given threshold.

#### Detection of PQRSTU waveforms

As discussed above, the system may be configured to record cardiac electrophysiological activity and ECG. Specifically, the system may be designed to acquire the full PQRSTU spectrum constituent ECG waveforms as exemplified in FIG. 4 which illustrates an example of a full PQRSTU waveform obtained for a patient using a system in accordance with an embodiment. The PQRSTU waveforms illustrated in FIG. 4 are generated by the heart and captured by the system to be viewed by doctors for diagnosis. In an embodiment, the system captures the ECG readings and processes them to produce ECG signals that may be read and viewed using existing medical equipment and produces waveforms that are identical to those produced by standard contact ECG systems, and as such can be used in place of standard ECG systems for all applications.

Needless to say, the contactless sensors 10 do not produce an output that is compatible with existing medical equipment's (e.g. monitors and the like) and therefore cannot interface with these equipment, hence the need for further processing. In an embodiment, the DPM converts the acquired signal into a format that complies with the international standards for existing medical equipment. This allows for a seamless replacement of conventional contact ECG systems without the need to replace existing diagnostic medical devices or re-train doctors and medical professionals. Such conversion may be performed in the DPM 2 using a combination of digital signal processing and analog output circuitry in the Digital to Analog Converter stage (19).

#### Sensor Design

As discussed above, the embodiments obtain ECG readings of the patient using contactless ECG sensors 10. The sensors 10 are specifically designed to capture high quality ECG from a patient without requiring direct electrical contact with the patient's skin. This allows to place the sensors 10 at some distance from the patient and/or to be separated from the patient's skin by a fabric such as clothing, bedding, etc. as exemplified in FIG. 5 which illustrates an example of how the sensor array captures ECG signals without direct contact with the patient's skin.

FIG. 6 is a block diagram illustrating an exemplary sensor design in accordance with an embodiment. As shown in FIG. 6 the sensor 10 may include a conductive electrode 33, an electrode shield 32, and an electrodynamic sensor including an amplifier 34 and a bias circuit 35 voltage. In the exemplary design of FIG. 6, the gain/current buffering amplifier 34 may be used in a type of negative feedback topology, and the input bias network 35 is adapted to increase the effective

input impedance of the amplifier **34**, to preserve the signal quality of the acquired ECG. The input of the electrodynamic sensor is connected to the conductive electrode **33**. A shield driving circuitry (**36**) may be employed to generate a feedback signal to connect to the electrode shield (**32**) to further increase the signal to noise (SNR) ratio by reducing parasitic capacitance seen at the input of the electrodynamic sensor.

The electrode **33** may be capacitively coupled to the patient's body by being in proximity to, but not touching the skin/body. This can be accomplished by laying on a bed with an array of sensors **10** embedded in it (as non-limiting example of implementation), while clothed. The electric field near the surface of the patient's skin that is created from the electrical activity of the heart capacitively induces a charge on the conductive electrode **33** without direct electrical contact. This charge may then be collected and amplified by the electrodynamic sensor, which produces an electrical signal (voltage) that is representative of the electrical activity of the heart in that location (complete PQRSTU).

The electrode shield **32** is configured to reduce the amount of stray interference that the electrodynamic sensor receives and also decrease the effective capacitance of the input of the amplifier **34**, which helps to preserve signal quality of the acquired ECG.

In a non-limiting example of implementation, both the electrode **33** and the electrode shield **32** may be made of an elastic/flexible material which allows the sensor **10** to better adapt to the geometry of the human body and obtain better ECG readings. At the same time this configuration allows the sensors **10** to be seamlessly provided in the fabric (or any of the following: gel/silicone/rubber type pad/mat etc.) in which the sensor array is to be placed.

FIG. 7 illustrates an example of a physical design of the sensor **10**. As exemplified in FIG. 7, the physical design includes the conductive electrode **33** physically implemented as a layer **39**, the shield **32** physically implemented as the layer **40**, and the remaining of the circuitry embedded in the layer **41**. The entire structure may be produced on a substrate **37** which may also be a printed circuit board, for example. In the design illustrated in FIG. 7, the layers **39**, **40** and **41** may be insulated from each other by dielectric layers **38** to provide electrical insulation.

Right Leg Drive

FIG. 8 illustrates an exemplary block diagram of an overall design of a system in accordance with an embodiment.

Referring to FIG. 8, and as discussed above with respect to FIG. 1, the system may include a sensor pad **7** comprising contactless ECG sensors (hereinafter CECG sensors **10**) which may be provided in the form of an array **202** such as that shown in FIG. 2. The sensor pad **7** may also include a grounding pad **15**, a driving circuitry e.g. a right leg drive (RLD) generator **14** (discussed below), and an ND converter **13**. The sensor pad **7** outputs the digitized ECG readings of the sensors **10** to the DPM **2**. The RLD generator **14** is configured to feed the grounding pad **15** with a high frequency signal that is outside of the ECG frequency band. This high frequency signal is then coupled through the patient's body to the CECG sensors, where the amplitude is recorded and analyzed by the DPM **2**. This gives the system a metric of how well-coupled each sensor is to the patient, effectively an impedance measurement to determine what the signal quality is from each sensor.

In addition to the digitized CECG sensor data, the DPM **2** may also be configured to receive standard ECG data of conventional electrodes in an analog format. Such analog

ECG data is optionally acquired through the use of standard contact electrodes and a trunk cable (**5**). The analog signals may be converted using an ADC **17**. The signals may then be filtered using a digital signal processing unit **18**, and output over a variety of wired and wireless interfaces (Wi-Fi (**22**)/Ethernet (**23**) to a mobile app (**3**)/cloud server (**4**) and through the 'Analog CECG & ECG out' interface to existing medical equipment (**6**).

The DPM **2** may include some sort of non-volatile memory e.g. flash memory **26** for storage of ECG data (if necessary). The DPM **2** may also be configured to perform diagnosis for acute issues, and send a warning over any one of the communication interfaces or an integrated sound alarm (**24**). The DPM **2** may also include a Bluetooth Low Energy interface (**21**) to enable configuration by the user through a mobile device. A Read Only Memory (**25**) may also be included to store a unique identifier. A Cryptographic processing module (**27**) may also be used to encrypt and decrypt data transmitted/received through the communication interfaces, and securely stores keys for this data encryption.

All sensor data (contactless and contact) can be sent over the wired and wireless interfaces. The selection algorithm **204** (discussed above in FIG. 3) decides which sensor information should be output over the analog interface **19** to existing medical equipment. A relay **20** may be provided to switch between the analog data received from the conventional electrodes and the contactless sensors **10** and to allow the DPM **2** to compare between the two. In DPM **2** can be configured to be turned off to act like a pass-through cable, without affecting the contact ECG signal if desired (controlled by the Processing Unit and Relays (**20**)). It can also be used in 'hybrid mode', during which a combination of CECG and ECG sensors can be output over the analog interface, if it improves the quality of the ECG signal.

Automatic gain correction

Due to the large, yet finite, input impedance of the electrophysiological sensors **10**, variations in the capacitive coupling between each sensor **10** and the patient's body (e.g. changes in the distance between each sensor and the body) can cause variations in the gain of each sensor channel. This has the effect of affecting the amplitude of ECG leads, in the same way that a dried out contact adhesive electrode produces a lower quality signal than a new one. To address the problem, a gain control mechanism is provided which allows the system to control relative impedance differences between different contactless ECG sensors, and an absolute impedance between each contactless ECG sensor and the human body due to a difference in distance between each contactless ECG sensor and the human body. As shown in FIG. 9, a programmable gain amplifier **43** (either in the analog or digital domains) may be provided on each sensor channel **42** to offset the change in gain caused by differences in coupling between the sensors **10** and the patient. FIG. 9 is a block diagram illustrating an exemplary gain control mechanism in accordance with an embodiment. As shown in FIG. 9, the gain control mechanism **220** may include a feedback loop including an ADC **44** coupled between the PGA **43** and a processor **45** which itself is connected to the PGA **43** to control its gain in real-time as the change is occurring.

The processor **45** may be a dedicated processor and may also be a processor module embedded into the processing unit **18** of the DPM **2**.

Referring back to FIG. 8, a grounding pad **15** is shown which in operation should be placed near, but not in contact with (at a distance), the patient's body. This pad is driven

with a feedback signal derived from the ECG signals to provide a capacitively coupled ground reference to the patient's body. The feedback signal is derived in such a way to increase the common mode rejection ratio (CMRR) of the system (by over 10 dB, typically). This reduces interference from common mode signals and preserves the signal quality of the acquired ECG.

FIG. 10 is an exemplary block diagram illustrating the function of the RLD generator 14, in accordance with an embodiment. As shown in FIG. 10, data received from the sensors is selected (or discarded) using a switching matrix (29) which selects specific sensors 10 to obtain data from using an RLD algorithm implemented digitally in the processing unit (18). The signals are then summed (29), inverted and amplified (30). This constitutes the driving signal for the grounding pad 15.

The RLD algorithm is configured to monitor the common mode signal acquired from each sensor (and by extension, the ECG signals output from selection algorithm). The RLD algorithm may select the set of sensors that increases the common mode rejection ratio of the system after the RLD signal is applied to the patient in the feedback configuration. Acquired Leads

As discussed above, the ability to compare a current ECG to an old one is of an immense medical value and this is not possible with existing systems which do not allow for long term monitoring. For example, an abnormal ECG does not prove acute cardiac disease, and a normal ECG does not exclude cardiac disease. It is therefore necessary to compare new ECG with ECG's made in the past. Hallmarks may include

- Is there a change in rhythm?
- Is there a change in frequency?
- Is there a change in conduction time?
- Is there a change in heart axis?
- Are there new pathological Q's?
- Is there a change in R wave size?
- Is there a change in ST?
- Is there a change in T wave?

The above changes immediately result in further investigations. Changes in the electrocardiogram can be further classified as acute and chronic, however, both require comparison electrocardiograms.

In general, as the number of electrodes used increases, the monitoring time that is possible decreases. Currently, one major limitation of the current standards is the difficulty in obtaining long term monitoring with multiple electrodes due to the inherent limitation of placing multiple electrodes and maintaining them on the body.

The system described above allows for serial comparison of electrocardiograms for the first time. The system has proven to acquire posterior ECG leads. According to a modified Mason-Likar lead system, a 16 lead ECG can be acquired from the patient laying on the matrix of sensors, embedded in a mattress, chair, etc. The acquired leads include: Leads I, II, III, aVr, aVl, aVf, V1, V1R, V2, V2R, V3, V3R, V4, V4R, V5, V5R as exemplified in FIG. 11 and FIG. 12. FIG. 11 shows medically recognized ECG locations for obtaining standard ECG leads, and FIG. 12 illustrates an example of standard ECG leads, each lead being shown as a vector between two locations on the human body.

The pad including the sensors 10 can be placed, unperceivably under a mattress so that ECG data can be acquired from posterior leads; e.g. the prone position. The system may be based on the Mason-Likar sensor placement used for the acquisition of the ECG during stress testing. Standard 12 lead ECG placement is not used because of myopotentials,

motion, artifacts, etc. and is limited to the 10 second 12 lead ECG printout and is not practical for short to long term monitoring.

Posterior placed electrodes are an accepted method of ECG acquisition, and indeed are used as an adjunct in certain situations to the more commonly used method of anterior lead placements. Anterior lead placement is currently the only type of lead placement used because of convenience. However, prone position ECG leads are performed in certain situations with standard electrodes, but because of the inherent difficulties, is not a standard.

FIG. 14 is a flowchart of a method for providing electrocardiogram (ECG) signals for a human body using contactless ECG sensors. As shown in FIG. 14, the method 260 begins at step 262 by receiving contactless ECG signals from an array of contactless ECG sensors. Step 264 comprises detecting body parts located in proximity of the array of contactless ECG sensors. Step 266 comprises selecting from each group a contactless ECG sensor having a highest signal quality. Step 268 comprises producing a standard ECG signal based on the contactless ECG signal of each selected contactless ECG sensor.

While preferred embodiments have been described above and illustrated in the accompanying drawings, it will be evident to those skilled in the art that modifications may be made without departing from this disclosure. Such modifications are considered as possible variants comprised in the scope of the disclosure.

The invention claimed is:

1. A Digital Processing Module (DPM) for providing electrocardiogram (ECG) signals for a human body for storage and/or viewing on a remote/local device, the DPM comprising:

an input adapted to receive contactless ECG signals for the human body from an array of contactless ECG sensors;

a processor adapted to perform a selection process including:

obtaining a body outline of the human body using data received from contactless ECG sensors located in proximity of the human body;

detecting one or more body parts located in the body outline using a set of rules embedded in the DPM;

associating a group of contactless ECG sensors with each detected body part;

selecting from each group a contactless ECG sensor having a highest signal quality for the body part associated with that group of contactless ECG sensors;

the processor being adapted to produce a standard ECG signal based on the contactless ECG signals received from the selected contactless ECG sensors; and an output for sending the standard ECG signal to the remote/local device.

2. The DPM of claim 1, wherein the processor is further adapted to perform the steps of:

a. determining a position of the human body on the array of contactless ECG sensors;

b. dividing the contactless ECG sensors into groups and associating each group to a body part using the body outline and the position of the human body; and

c. from each group, selecting the contactless ECG sensor providing the highest signal quality.

3. The DPM of claim 2, wherein the processor identifies the contactless ECG sensors that are located in close proximity to the human body by measuring an impedance between each contactless ECG sensor and the human body.

13

4. The DPM of claim 1, wherein the processor is adapted to select another contactless ECG sensor for a given body part following a movement of the human body with respect to the array of contactless ECG sensors.

5. The DPM of claim 4, wherein the processor is adapted to re-run the selection process continuously to perform the selection of the other contactless ECG sensor.

6. The DPM of claim 4, wherein the processor is adapted to continuously monitor a current signal quality of the selected contactless ECG sensor associated with each body part to re-run the selection process when the current signal quality drops beyond a given threshold.

7. The DPM of claim 1, further comprising an automatic gain control mechanism adapted to control relative impedance differences between different contactless ECG sensors, and an absolute impedance between each contactless ECG sensor and the human body due to a difference in distance or type of clothing material between each contactless ECG sensor and the human body.

8. The DPM of claim 1, further comprising a wired/wireless data port for transmitting the standard ECG signal to a remote device over a data network.

9. A system for providing electrocardiogram (ECG) signals for a human body for storage and/or viewing on a remote/local device, the system comprising:

a fabric including a sensor pad comprising an array of contactless ECG sensors;

a processor operatively connected to the sensor pad and adapted to receive contactless ECG signals from the contactless ECG sensors and perform a selection process including:

obtaining a body outline of the human body using data received from contactless ECG sensors located in proximity of the human body;

detecting one or more body parts located in the body outline using a set of rules embedded in the DPM; associating a group of contactless ECG sensors with each detected body part;

selecting from each group a contactless ECG sensor having a highest signal quality for the body part associated with that group of contactless ECG sensors;

the processor being adapted to produce a standard ECG signal based on the contactless ECG signals received from the selected contactless ECG sensors; and an output for outputting the standard ECG signal to the remote/local device.

10. The system of claim 9, wherein the sensor pad comprises a grounding pad for placing in proximity of and at distance from the human body, the grounding pad being adapted to provide a capacitively coupled ground reference to the human body for reducing interference.

11. The system of claim 10, further comprising a drive signal generator configured to feed the grounding pad with a high frequency signal that is outside of an ECG frequency band for determining the capacitively coupled ground reference for each contactless ECG sensor.

12. The system of claim 9, wherein the contactless ECG sensor comprises:

a capacitive electrode adapted to be capacitively coupled to the human body for outputting an electrical charge which is representative of an electrical cardiac activity;

14

an electrodynamic sensor configured to detect and amplify the electrical charge produced by the capacitive electrode; and

an electrode shield physically provided in proximity of the electrode for reducing a stray interference at an input of the electrodynamic sensor.

13. The system of claim 12, wherein the contactless ECG sensor is made of a flexible material.

14. The system of claim 12, wherein the sensor pad is provided in a fabric with which the human body comes in contact or in one of: a gel, silicone, a rubber type pad, and a mat.

15. A method for providing electrocardiogram (ECG) signals for a human body using contactless ECG sensors, the method comprising:

receiving contactless ECG signals from an array of contactless ECG sensors;

obtaining a body outline of the human body; detecting body parts located in the body outline;

associating a group of contactless ECG sensors with each detected body part;

selecting from each group a contactless ECG sensor having a highest signal quality for the body part associated with that group of contactless ECG sensors;

producing and outputting a standard ECG signal based on the contactless ECG signals received from the selected contactless ECG sensor.

16. The method of claim 15, further comprising: determining a position of the human body on the array of contactless ECG sensors;

dividing the contactless ECG sensors into groups and associating each group to a body part using the body outline and the position of the human body;

for each group, selecting the contactless ECG sensor providing the contactless ECG signal having the highest signal quality.

17. The method of claim 16, further comprising identifying the contactless ECG sensors that are located in close proximity to the human body by measuring an impedance between each contactless ECG sensor and the human body.

18. The method of claim 15, further comprising: repeating the steps of detecting to selecting continuously for selecting another contactless ECG sensor for a given body part following a movement of the human body with respect to the array of contactless ECG sensors.

19. The method of claim 15, further comprising continuously monitoring a current signal quality of the selected contactless ECG sensor associated with each body part; and

when the current signal quality drops beyond a given threshold following a movement of the human body with respect to the array of contactless ECG sensors, repeating the steps of detecting, associating and selecting to select another contactless ECG sensor for at least one of the body parts.

20. The method of claim 15, further comprising controlling relative impedance differences between different contactless ECG sensors, and an absolute impedance between each contactless ECG sensor and the human body due to a difference in distance or a type of clothing material between each contactless ECG sensor and the human body.

\* \* \* \* \*

专利名称(译)	非接触式心电图系统		
公开(公告)号	<a href="#">US10052042</a>	公开(公告)日	2018-08-21
申请号	US14/893293	申请日	2015-09-23
[标]申请(专利权)人(译)	RR序列		
申请(专利权)人(译)	RR序列INC.		
当前申请(专利权)人(译)	RR序列INC.		
[标]发明人	JAIN DEEPAK BOBBY WEEKS JOSHUA NADEZHDIN DAVID ASSELIN JEAN FRANCOIS		
发明人	JAIN, DEEPAK BOBBY WEEKS, JOSHUA NADEZHDIN, DAVID ASSELIN, JEAN-FRANCOIS		
IPC分类号	A61B5/0408 A61B5/0424 A61B5/00 A61B5/0428 A61B5/11 A61B5/0402 A61B5/04		
CPC分类号	A61B5/04085 A61B5/0402 A61B5/0424 A61B5/04028 A61B5/04284 A61B5/1114 A61B5/7221 A61B5/6844 A61B2562/164 A61B5/0006 A61B5/04012 A61B2562/0214 A61B2562/046		
代理人(译)	JOHNSTON , MICHAEL G.		
优先权	62/206542 2015-08-18 US 62/054189 2014-09-23 US		
其他公开文献	US20160287128A1		
外部链接	<a href="#">Espacenet</a>		

摘要(译)

一种用于使用非接触式ECG传感器为人体提供标准心电图 ( ECG ) 信号的系 统，用于输出到现有的医疗设备或用于在远程设备上存储或查看。该系统包括数字处理模块 ( DPM ) ，其适于连接到织物等中提供的非接触式ECG传感器阵列。选择机制嵌入到DPM中，允许DPM使用不同ECG传感器的ECG信号识别身体部位，并为每个身体部位选择最佳传感器导联。然后，DPM可以使用所选择的ECG信号产生标准ECG信号，用于检测到的不同身体部位。该系统适于连续地重新检查选择，以确保在身体部位移动后为给定的身体部位选择最佳引线，从而允许对患者进行连续和不间断的ECG监测。

