


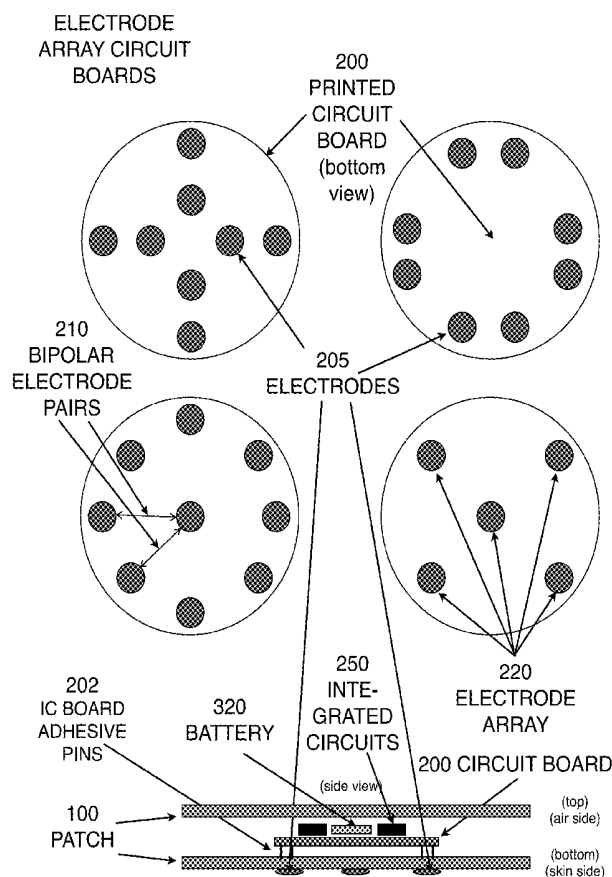



US 20160045137A1



(19) **United States**(12) **Patent Application Publication**
Axelrod(10) **Pub. No.: US 2016/0045137 A1**(43) **Pub. Date: Feb. 18, 2016**(54) **WEARABLE WIRELESS PATCHES
CONTAINING ELECTRODE PAIR ARRAYS
FOR GASTROINTESTINAL
ELECTRODIAGNOSTICS**(52) **U.S. CL.**
CPC *A61B 5/04882* (2013.01); *A61B 5/0492*
(2013.01); *A61B 5/04012* (2013.01); *A61B*
5/0004 (2013.01); *A61B 5/6823* (2013.01);
A61B 5/02055 (2013.01); *A61B 5/1116*
(2013.01)(71) Applicant: **GTech**, Freemont, CA (US)(72) Inventor: **Steve Axelrod**, Los Altos, CA (US)(73) Assignee: **GTech**, Freemont, CA (US)(21) Appl. No.: **14/051,440**(22) Filed: **Oct. 10, 2013****Related U.S. Application Data**(60) Provisional application No. 61/712,100, filed on Oct.
10, 2012.**Publication Classification**(51) **Int. Cl.**
A61B 5/0488 (2006.01)
A61B 5/0205 (2006.01)
A61B 5/00 (2006.01)
A61B 5/0492 (2006.01)
A61B 5/04 (2006.01)(57) **ABSTRACT**

A system and method for profiling electrical activity in smooth muscle of the gastrointestinal tract muscular of a patient are disclosed. The system includes electromyographic-sensing patches adapted for placement on the skin of the abdomen of the patient. Each patch has at least one bipolar electrode pair, or a multitude arranged in an array, and is enabled for communication of a signal indicative of a sensed electromyographic signal. The system further includes networked computing devices. The local patch device is configured for wireless communication between the EMG-sensing patches and a local computing device, to enable wireless transmission from the patch to the networked computing devices. The networked computing device is configured to process large aggregate collections of multi-hour or day signals received from the local computing device to yield diagnostically valuable physiological parameters of gastrointestinal smooth muscle electrical activity.



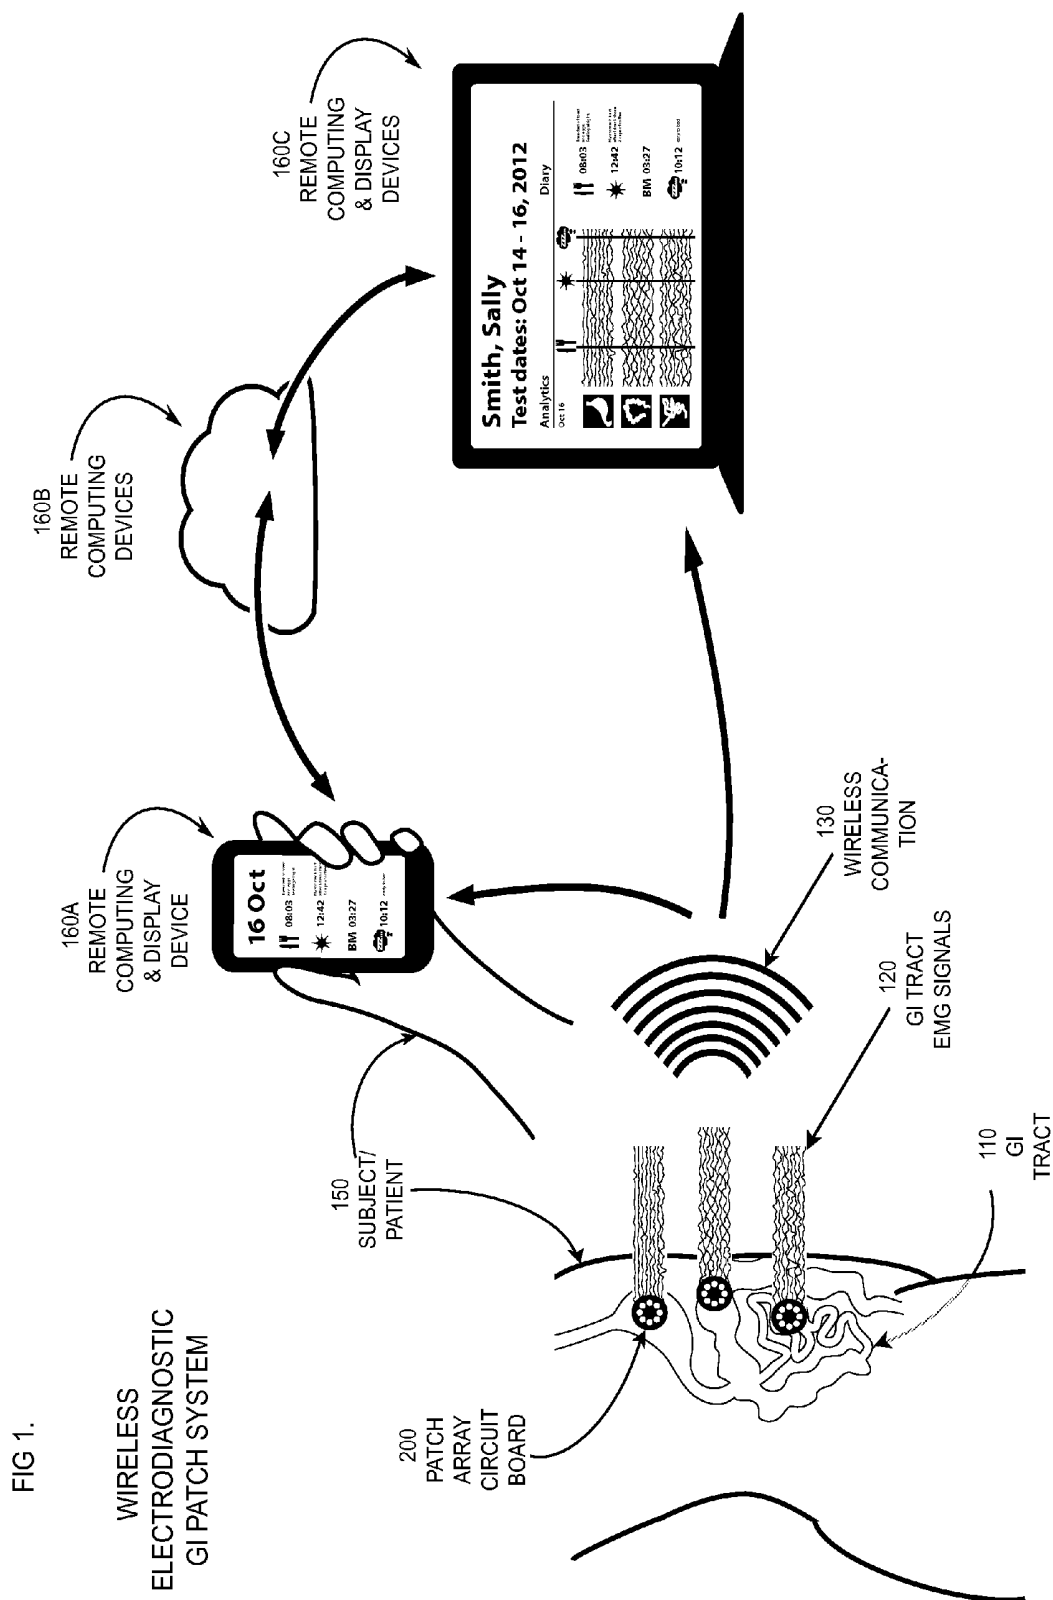

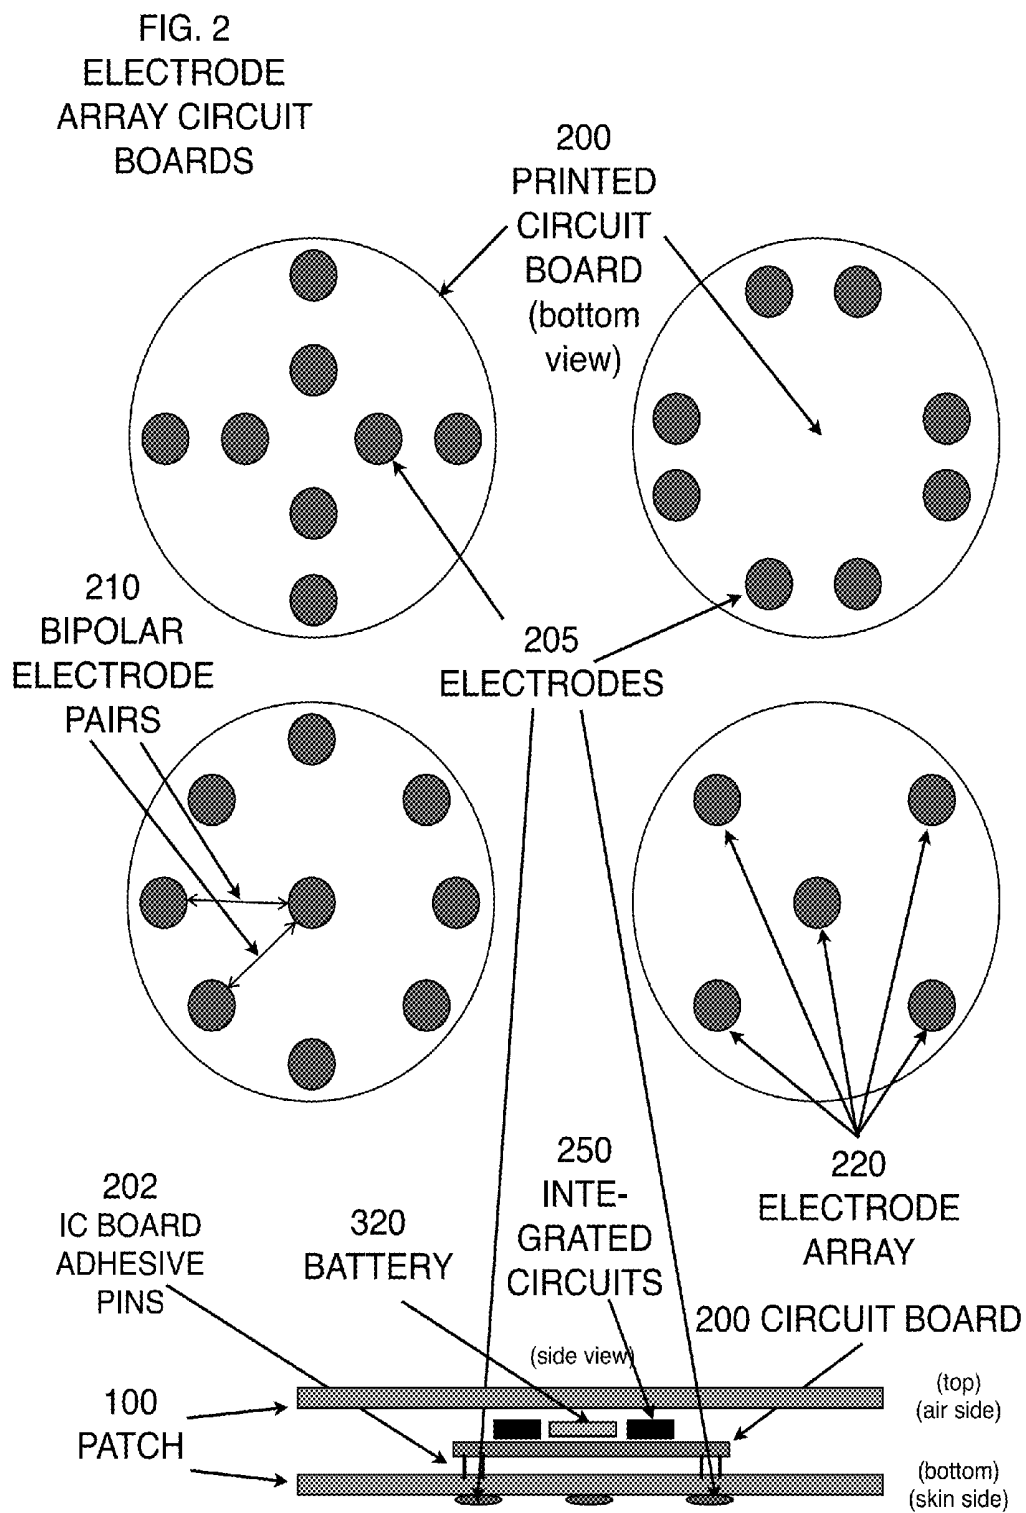

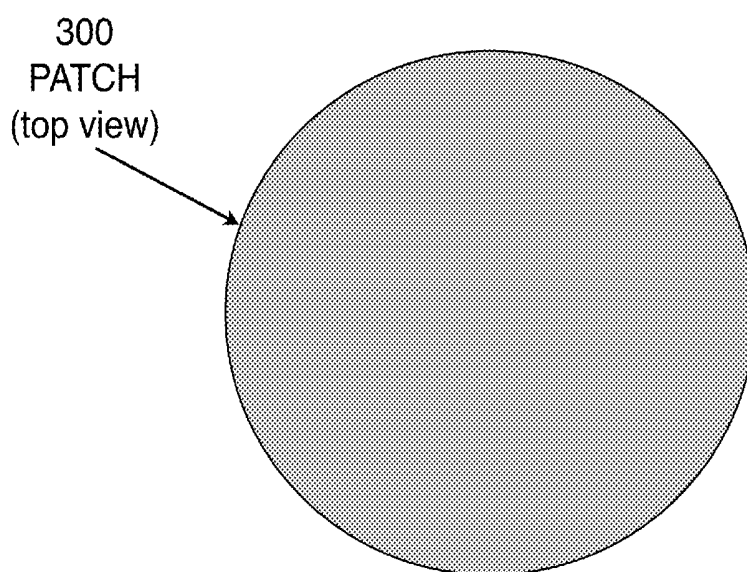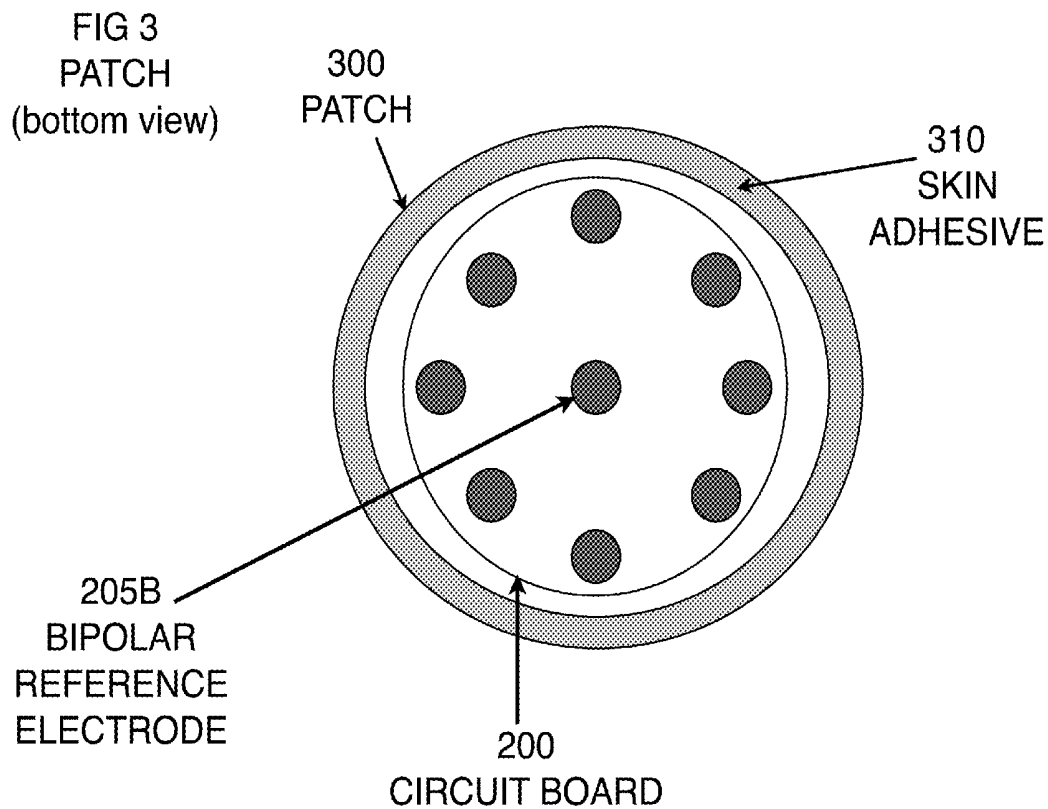

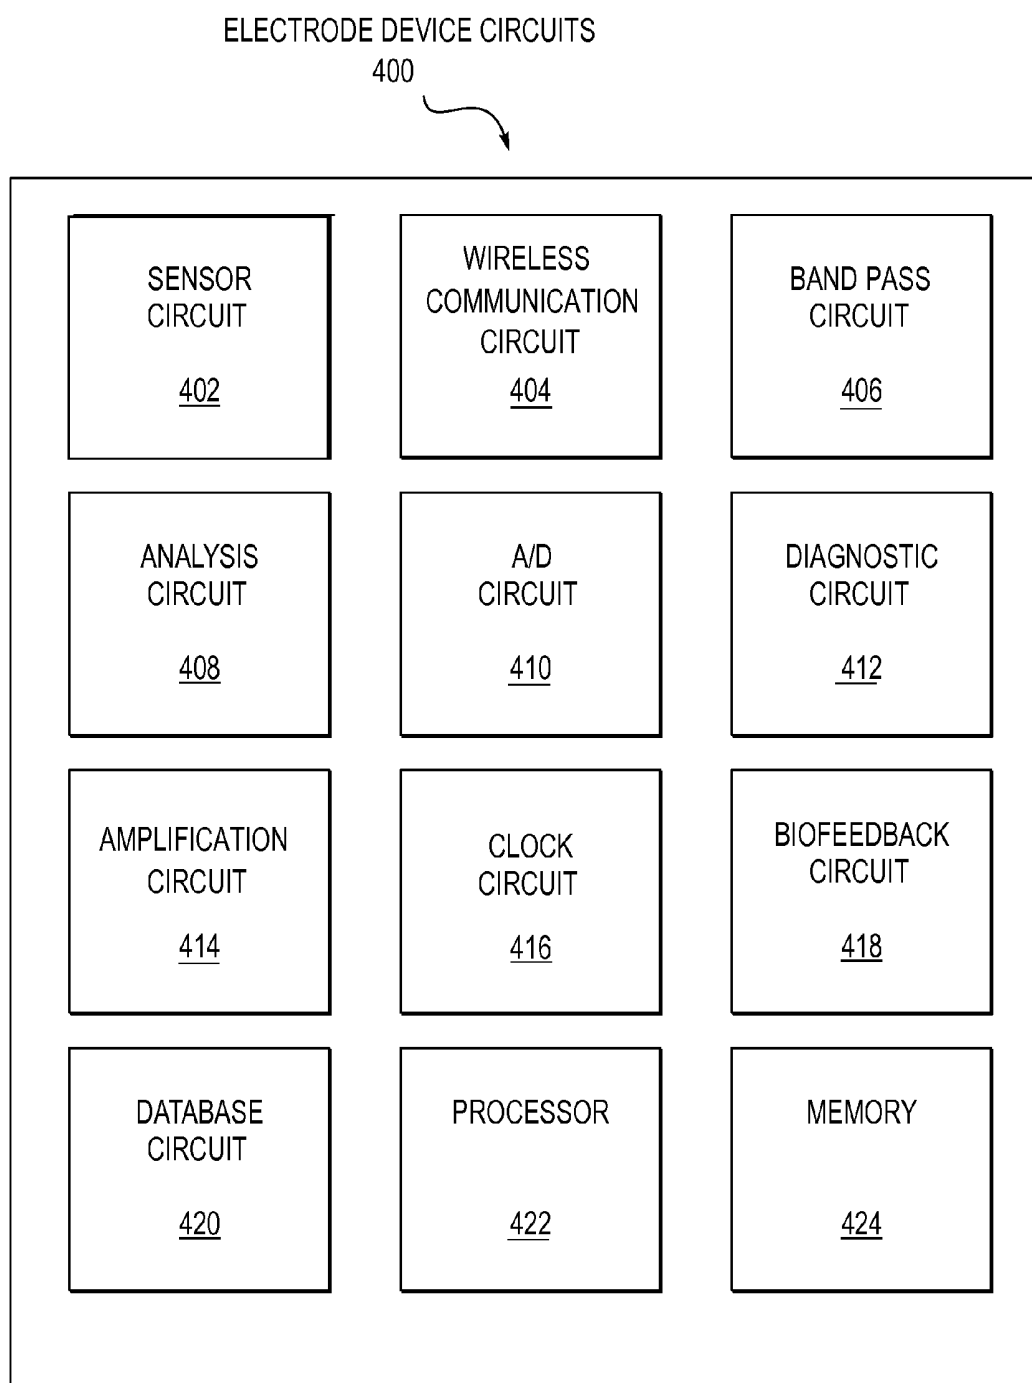


FIG. 4


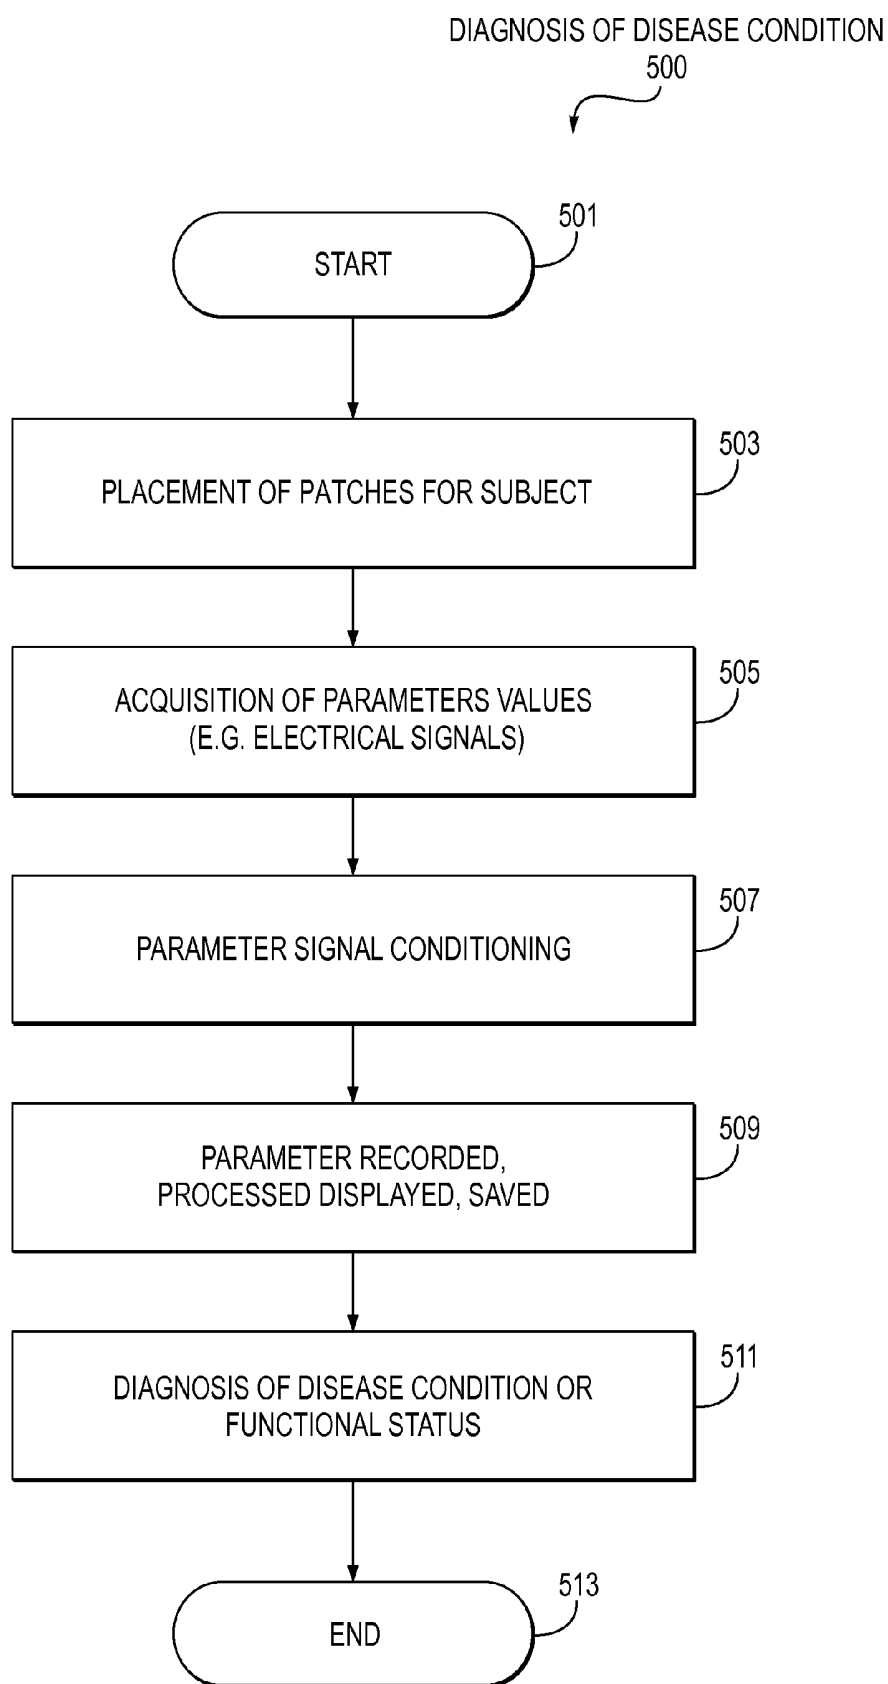


FIG. 5

FIG. 6

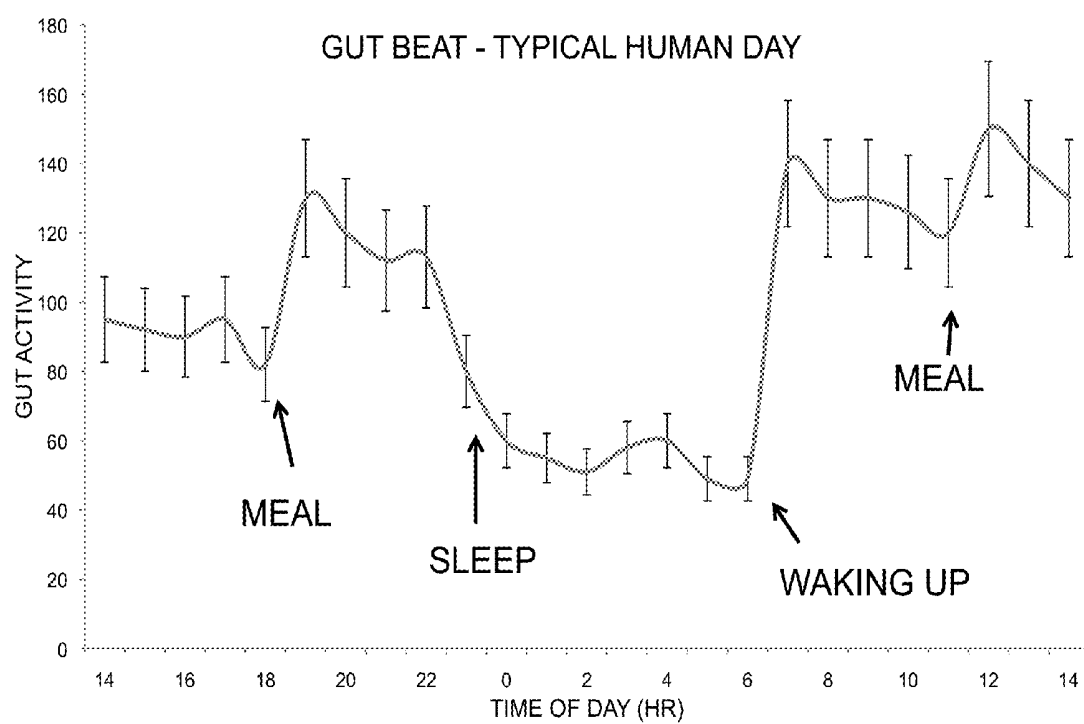

**WEARABLE WIRELESS PATCHES
CONTAINING ELECTRODE PAIR ARRAYS
FOR GASTROINTESTINAL
ELECTRODIAGNOSTICS**

TECHNICAL FIELD

[0001] This disclosure relates generally to electromyographic (EMG) and electrodiagnostic systems and methods for profiling electrical activity within the smooth muscle of the gastrointestinal tract, and more particularly to systems and methods for mathematically extracting salient patterns of diseased electromyographic activity of the gastrointestinal tract from gathering large data sets of multi-hour and multi-day recordings from ambulatory patients with wearable, disposable, wirelessly-enabled sensor patches, and for diagnosing various gastrointestinal disorders. The disclosed invention can further be used in gastrointestinal drug research and discovery, and for possible treatments of certain GI tract disorders.

BACKGROUND

[0002] The majority of gastrointestinal motility tests are invasive and a source of much discomfort and patient anxiety and expense. Therefore, advancing the state of the art in noninvasive technologies is highly desired. The present invention utilizes combinations of electrogastrography and electroenterography (EGG & EEnG), both of which allow for noninvasive and potentially long term ambulatory data collection of patients, which in turn provides for greater patient convenience and comfort, lower costs, and more powerful diagnostic potential. EGG captures the rhythmical electrical activity of the stomach through electrodes located on the abdomen in the vicinity of the stomach, while EEnG captures the intestinal slow muscle electrical activity which may present anywhere on the abdomen.

[0003] Methods and systems for obtaining EMG data from the gastrointestinal tract of patients, particularly patients who appear to suffer from disorders related to gastrointestinal motility, are known in the prior art and practiced by specialists in the art. Such systems and methods typically are used in a procedure that occurs in a clinical setting, within a time frame of several hours, and wherein the patient needs to be substantially in repose. Further, the testing procedure usually asks the patient to adhere to a preliminary schedule of eating, and of eating a standardized meal. Finally, the typical electrographic measuring system is only taking measurements from a very small set of EMG bipolar electrodes, typically two or three, and thus measuring just a small sample of the entire gastrointestinal system, while using a large, extremely expensive, typical medical office Electrodiagnostic signal amplification and data acquisition machine.

[0004] These constraints, however practical and appropriate, nevertheless likely limit the scope of data derived from such studies. The data are limited in GI tract coverage and time frame. A study is only feasible for several hours, during which a patient can tolerate or comply with the constraint on normal physical activity. This limitation should be understood against the perspective that, in reality, gastrointestinal activity occurs in the context of a daily cycle, and that daily cycle occurs in the context of activities of daily living. Gastrointestinal pain or discomfort also can be cyclical or chaotically intermittent throughout the day, or over the course of several days. Such intermittency may or may not be obviously

tied to activities associated with the gastrointestinal tract specifically, or the more general and varied activities of daily living. Accordingly, it is proposed and likely that the diagnostic value of gastrointestinal activity data derived from tests that include such constraints has always been limited in its potential, thus greatly limiting the adoption and use of this field of GI diagnostic technology.

[0005] Further, such a gastrointestinal EMG study, as currently practiced, is expensive in that it occupies space in the clinic, and it occupies the time of the healthcare provider who is administering the testing procedure. As a consequence of a cost that limits the prevalence of such testing, the testing is generally applied to severe cases of gastrointestinal distress or to cases that are otherwise difficult to diagnose. And further still, the limited use of such testing limits the accumulation of data as a whole, which would advance understanding of the relationship between dysfunctional gastrointestinal electrical activity and gastrointestinal disorders.

[0006] Thus, there is a strong need in the medical marketplace for systems and methods that are more affordable, and which provide a more comprehensive view of gastrointestinal activity throughout a day or for longer periods, and which can monitor such activity while the patient is free to conduct the normal activities of daily living.

[0007] There are many examples in the prior art of remote, ambulatory, monitoring, recording and alarm EMG (and other medical sensor) systems. Although the presently disclosed system can include those functions, it is not the ideal objective and embodiment of this invention.

[0008] Instead, it is further a novel objective of the ideal embodiment of the present invention to allow for the easy and inexpensive collection of large spatial (skin attachable patches with distributed arrays of inexpensive orthogonal bipolar electrodes allowing coverage over the entire, or large sections, of the midsection) and temporal (over time, ambulatory subjects going about their normal lives for hours to days) data sets.

[0009] All of the currently encountered prior art do not discuss concurrent multi-organ recordings, nor discuss whole digestive track, multi-day recordings for the purposes of GI tract disorder diagnosis. It is furthermore strongly suggested that the presently included invention is not wholly meant as a real-time monitor, since ideal embodiments will entail intermittent patch data storage and transmission in order to optimize battery life.

[0010] Additionally, the current state of the art generally allows for a few electrodes, without clear guidance on exact placement or spacing on the body, and recordings made in office for, at most, a few hours. The presently known art also teaches wearable EMG devices for continuous status monitoring, real-time disease event alarms, or personal health data recording. For example, in US patent application 20130046150, titled, Method for diagnosis and treatment of disorders of the gastrointestinal tract, and apparatus for use therewith, by inventor Uday Devanaboyina teaches a wearable, portable EMG system for long term home use, but does not teach a plurality of electrode array based wireless patches to cover the entire GI tract.

[0011] Additionally, wireless, wearable, home-use based ECG heart monitoring devices are well known in the art. For example, Biotronik US patent application 20130046150, teaches "Long-term cutaneous cardiac monitoring". The system disclosed is for long-term heart monitoring via a disposable adhesive surface patch for cutaneous mounting with

built-in electrodes and wireless communication with a remote service center. However, the nature of cardiac heart muscle tissue signals is very different than that of the Gastrointestinal system, and thus, the patent does not teach about grids of electrodes or complex aggregate spatiotemporal data analysis. Cardiac systems typically require only two or three electrode pairs, and individual heart beats are analyzed or monitored, rather than aggregate heart beat data.

[0012] Furthermore, numerous examples of small, disposable, wireless, adhesive wearable medical EMG data collection patches exist in the marketplace. For example, DELTA Danish Electronics, Light & Acoustics, Inc., Denmark, has developed an ePatch® system for home health monitoring. (<http://epatch.madebydelta.com>). While this system and others are examples of the growing trend of wearable medical devices, it does not teach beyond the well known EGG medical practices—few electrodes, primarily for monitoring purposes, and analyzed linearly rather than aggregately. No suggestion is made for full GI tract monitoring by arrays of electrodes over long time periods for advanced spatiotemporal data pattern analysis.

[0013] Additionally, there are numerous research papers exploring the use of wireless EMG and EGG systems for home health monitoring. For example, S. Haddab, et al, proposes a “Microcontroller-Based System for Electrogastrography Monitoring Through Wireless Transmission” system. However, like all other commercial and scientific EGG efforts, his efforts are short term (four hours maximum), and with a minimum of traditional electrodes. No suggestion of multi-day recording is made. The mathematical analysis was of the traditional type designed to remove noise and artifact from the linear signal, rather than achieve diagnostic successes through spatiotemporal pattern analysis of data aggregated from in-situ subjects over multi-day periods.

[0014] The same is true of Haahr, R. G., et al, who despite their promising work on “A wearable ‘electronic patch’ for wireless continuous monitoring of chronically diseased patients”, they specifically teach a “wearable health system . . . made as an electronic patch . . . (and) for the EMG application three standard dry silver electrodes are used separated by 10 mm.”

[0015] U.S. Pat. No. 7,593,768, “Detection of smooth muscle motor activity”, discloses EMG peak detection in the frequency spectrum and calculating the energy of the peaks for the stomach and small Intestine using internal and surface electrodes. It does not teach towards the presently disclosed invention. Specifically, only mention of the recording time involved a maximum time of two hours, and the maximum number of electrodes mentioned was eight. Furthermore, these eight electrodes were implanted, not external, and their data was summed up into one time series, not analyzed as a spatial temporal pattern. Nor is there any mention of wearable or wireless data collection for ambulatory, at home data collection.

[0016] While there is a long history of minor success with EGG approaches, and EGG/EEG possesses important information regarding the physiological and functional state of the GI tract, the cost and limited diagnostic benefit has so far prevented the mainstream and large scale medical mainstream use of EGG and EEG.

[0017] Furthermore, there is enormous variability in the anatomical nature and structure and organ placement and tissue densities among patients. There is also enormous variability in both the healthy and disordered GI tract slow muscle

rhythmic activity physical parameters and patterns. These two factors prevent any kind of EMG electrode placement standardization, and limit the effectiveness of EMG in diagnosing the large number of different GI tract disorders commonly encountered in the clinical setting.

[0018] Thus, it is an objective of the present invention to create a system that places enough of an array of particularly arranged electrodes over larger GI tract areas, or the entire GI tract, to obviate the issues caused by non-standard electrode placements or individual anatomical variability.

[0019] It is not suggested herein that any one particular electrode array placement patterns is the focus or limit of the presently disclosed invention. There exist an almost infinite variety of different electrode arrangements, some of which will possess differing pros and cons with regards to optimization of cost versus data collection versus additional engineering, diagnostic, and business consideration.

[0020] It is instead suggested that by having any plurality of variously spaced, orthogonally arranged bipolar electrode pairs on a patch, with one or more patches covering the entire, or large part, of one or more digestive organs, sufficiently ideal diagnostic data sets can be collected, throughout a single days normal digestive activities, (a single “gut beat”), for sufficient mathematical post-processing to yield great diagnostic value. Furthermore, by employing multiple electrodes and patches, it is also possible to dynamically alter which electrodes form bipolar pairs based on incoming data optimization algorithms. Importantly, a plurality of smaller patches, rather than one single giant patch, is an ideal embodiment because smaller patches help prevent significant lateral movement of electrodes on the skin.

[0021] In addition to the previously mentioned limitations of standard EGG, there are many sources of data variability, including patient height, weight, anatomy, skin condition, recent food consumption history, metabolic rest state, and the like. Furthermore, data variability is additionally introduced from highly variable placement of electrodes or patches, or in equipment manufacturing variations, and of course the variability caused by different disorders and the general chaotic and nonlinear dynamic nature of biological systems. These large variations negatively impact diagnostic effectiveness of all previous known systems. This variability problem is compounded further by the fact that EGG is a lower amplitude signal compared to other bodily electrophysiological signals, such as the heartbeat or breathing, and thus easily influenced by both random sources of variation and systematic influence factors.

[0022] It is thus an objective of the presently disclosed invention to effectively avoid these limitations by use of the presently disclosed patches, in combination with continual or intermittent data collection and transmission over periods of many hours, days, in combination with advanced mathematical techniques, in both the time and frequency domains.

[0023] The usual 24 hour circadian cycle of the body is well representative of the digestive cycle of the normal or healthy body. Research has shown that the digestive system follows a similar 24 hour pattern, with low GI activity during sleep, increased activity after waking and temporary increases following breakfast and other meals, with defecation often occurring at more or less the same time each day. This full cycle of GI activity might be called a “gut beat” in analogy to the heartbeat cycle of the heart. Inasmuch as there are events such as Giant Migrating Contractions (GMC’s) and Migrating Motor Complexes (MMC’s) associated with propulsion

of the contents of the intestines that occur on the order of a few to several times per gut beat, capturing data for at least one full day is essential to develop an understanding of the workings of an individual's digestive system with the intent to diagnose abnormality. In fact due to normal variability it is further advantageous to sample for several days to better quantify infrequent events, capture rare events, and reduce statistical noise in the measurement of common events.

[0024] An example of a common event is the increase in degree of muscular activity in any of the stomach, small intestine or colon after a meal. In general all these organs respond to meal ingestion either within minutes or tens of minutes, and quantifying that increase has diagnostic value. An example of an uncommon event is limited propulsion of the luminal contents of the small intestine, which typically happen several times per day in healthy subjects. An example of a rare event is defecation, which happens on average once per day for healthy subjects, but for patients with constipation it may only happen once every several days.

[0025] Thus, we would characterize this combination of multiple patches of multiple electrode pair arrays designed to sample, store, and wirelessly transmit data intermittently to remote computer servers over a larger segment of time, as the collection of spatiotemporal electromyographic data. And while there are an infinite number of ways for the remote servers to mathematically and algorithmically analyze and display said aggregates of such large data sets, the presently ideal embodied invention utilizes techniques such as time series analysis, time-dependent frequency analysis, and pattern matching analysis.

[0026] It will be appreciated by persons skilled in the art that the present invention is not limited to what has been particularly shown and described hereinabove. Rather, the scope of the present invention includes both combinations and subcombinations of the various features described hereinabove, as well as variations and modifications thereof that are not in the prior art, which would occur to persons skilled in the art upon reading the foregoing description.

BRIEF DESCRIPTION OF THE DRAWINGS

[0027] Various embodiments of the invention are disclosed in the following detailed description and accompanying drawings. Other features and advantages of the invention will become apparent from the following detailed description in conjunction with the drawings, wherein:

[0028] FIG. 1 schematically illustrates the preferred embodiment of the entire wearable, wireless, GI electrodiagnostic data aggregating and diagnostic system;

[0029] FIG. 2 shows a bottom view of a multi-electrode configuration of the disposable unit 100, shown with its corresponding electronic controller detached and spaced from the disposable unit 100;

[0030] FIG. 3 provides a simplified bottom view of a patch, and FIG. 1B provides a simplified bottom view, of a wearable, disposable/recyclable unit 100 and an electrode patch EMG circuit 200 and it's array of nine bipolar electrodes 205 as an exemplary example of the invention;

[0031] FIG. 4 illustrates a functional view of a system 200 with various circuit modules including a processor and memory to run the software.

[0032] FIG. 5 is a flow chart of the diagnosis process of typical GI disease condition 500.

[0033] FIG. 6 is a data chart of the typical human daily "Gut Beat", or GI tract activity of a normally behaving person,

which is the ideal minimum sample period for maximum GI disorder diagnostic functionality of the presently disclosed invention.

DETAILED DESCRIPTION OF THE DRAWINGS

[0034] The following description is of preferred versions of the invention, and the invention is not limited to these preferred versions. The scope of the invention should be determined with reference to the claims set forth at the end of this document.

[0035] FIG. 1 schematically illustrates the preferred embodiment of the entire wearable, wireless, GI electrodiagnostic data aggregating and diagnostic system, including hand held computing devices 160a for easy patient 150 supplemental data entry, and remote computer display devices 160c for patch 300 wireless transmission 130 in order for remote computer servers 160b to process for display the GI tract 110 physiological parameters 120 for doctor diagnostic assistance.

[0036] Figure presents a system wide view, with a set of multi-day-wearable patches 300/200 that sense, amplify and digitize myoelectric data 120 at the skin surface 150 originating in the smooth muscles of the stomach, small intestine and colon, 110 and transfer the data wirelessly 130 to a handheld computing device 160a, the patches having two or more bipolar pairs of electrodes 205 arranged substantially orthogonally, the patches further having onboard sensors that are capable of measuring any of acceleration, velocity or position 402; the computing device further capable of allowing the patient to enter 420 information 160a relevant to their gastrointestinal (GI) tract such as meal contents, bowel movements or abdominal pain, synchronizing and combining this information with the time-stamped 416 raw data 120 and uploading both to a cloud server 160b or other wireless host; the host serving as a repository for further processing or download to a processing device, the processing device using time and frequency based algorithms to extract events and patterns of events that relate to the activity of the aforementioned GI organs 120, specifically slow waves that are associated with mixing and propulsion of their contents as part of digestion and elimination, with the purpose of providing diagnostic information on the activity of the organs as they relate to functional GI disorders (FGIDs) such as irritable bowel disorder (IBS). The computing device further having the ability to coordinate data transfer schedules with the patches to accommodate either regularly scheduled transfers 404 or reconnecting when temporarily out of range, and the further ability to identify patches individually.

[0037] FIG. 2 schematically illustrates the electrode array circuit board 200. The disposable unit 200 has at least two, but preferably eight embedded bipolar pair electrodes 205 arranged in an array 220. Preferably, the inter-electrode distance is between 1 and 2 inches. The electrodes 205 are embedded inside the printed circuit board patch unit 200, with an ideally slight extension for greater skin contact. The circuit board 200 will likely be entombed in waterproof resin for greater water resistance, and the patch housing itself 300 will ideally have water resistant properties.

[0038] FIG. 3 shows a bottom and top view of an exemplary patch 300 and electrode array circuit board 200. Long-term non-invasive GI tract monitoring, an inexpensive, light, water resistant and disposable skin-adhesive unit 100 is provided. Because the unit is disposable, it can be easily replaced with another disposable unit after its usage for a few days. The

bottom of the disposable unit **100** has an adhesive surface **110** that can be affixed to the patient's skin for at least 7 days. One exemplary type of such adhesive material is the pressure-sensitive adhesive which forms a bond when pressure is applied to stick the adhesive to the adherent (e.g., the patient's skin).

[0039] FIGS. 4 and 5 illustrates flow charts and functional views of the system when in use.

[0040] FIG. 6 is a data chart of the typical human daily "Gut Beat", or GI tract activity of a normally behaving person, which is the ideal minimum sample period for maximum GI disorder diagnostic functionality of the presently disclosed invention.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

[0041] The following is a detailed description of exemplary embodiments to illustrate the principles of the invention. The embodiments are provided to illustrate aspects of the invention, but the invention is not limited to any embodiment. The scope of the invention encompasses numerous alternatives, modifications and equivalent; it is limited only by the claims.

[0042] Typical embodiments of a local computing device are sized to be handheld or generally portable. This physical aspect of the device is appropriate for the operation of the system simply because the patient needs to have this local device with himself or herself, or very close at hand, at least substantially throughout the duration of the monitoring period. Typical examples of a local computing device, per currently available technology, include mobile telephones, personal digital assistants, and tablet devices.

[0043] Embodiments of a local computing device can communicate through wireless networks by way of cell phone frequencies, satellite communication frequencies, wifi networks, or any network that can form a communication route to a networked computing device. Wireless transmission of data to a networked computing device may occur by way of an intervening remote data storage server, such server often referred to generically as "the cloud".

[0044] Electromyography is a general term for acquiring or monitoring signals as emanated from physiological sources. Electromyography as applied particularly to the smooth muscle of the gastrointestinal tract from the GI tract can also be termed electrogastrography or electroenterography.

[0045] Embodiments of the disclosed system and methods may be applied toward monitoring the electrical activity of the gastrointestinal tract of human subjects of any age, including infants, children, adolescents, and adults. Embodiments may also be applied to monitoring the electrical activity of the gastrointestinal tract of non-human animals, non-human mammals in particular.

[0046] Bluetooth LE is a current example of a low energy transmission capability appropriate for operation of the disclosed technology. Other low energy electronic communication protocols that may be developed in the future are included as embodiments. The low energy aspect of communication that the EMG-sensing patches makes use contributes to the ability of a battery to sustain operation of the patches for sustained periods of operation, such as 24 hours or more of continuous monitoring.

[0047] An intermittent schedule of signal transmission or transmitting in response to a query is a feature that conserves battery power, and contributes to the ability of a battery to

sustain operation of the patches for sustained periods of operation, such as 24 hours or more of continuous monitoring.

[0048] Additionally, each Bluetooth enabled patch will possess a unique identifier, so that the EMG sensing patches are able to transmit a unique identifier to the local computing device. This will allow identification of individual patches—both those located on one patient, or those located on different patients or subjects in the same general vicinity.

[0049] The unique identifier term, as used herein, generally refers to a serial number, an arbitrary number, or an accession number that is applied to it by the system or by a human operator. This identifier does not necessarily include any locational information per se, although locational information could be associated with the identifier by a human operator or by an aspect of the system.

[0050] It is also advantageous for the operation of the patch that the battery has a high charge capacity. Additionally, embodiments of the technology include any future technological advancements that may be made regarding recharging of batteries, particularly by way of induction or solar power

[0051] Numerous specific details are set forth in the following description in order to provide a thorough understanding of the invention. However, the invention may be practiced according to the claims without some or all of these specific details. For the purpose of clarity, technical material that is known in the technical fields related to the invention has not been described in detail so that the invention is not unnecessarily obscured.

1. A wearable non-invasive wireless electrodiagnostic patch system for profiling gastrointestinal tract muscular activity of a subject, comprising:

a set of electromyographic-sensing patches adapted for multi-day constant attachment to the skin surface of the midsection of a subject,

each patch of said set comprising a particularly arranged array of bipolar electrode pairs,

each patch enabled for collecting, storing, processing and communicating a range of full to partial time segments of sensed spatiotemporal electromyographic signals from the subject to remote computing and display devices,

wherein said computing devices are configured to mathematically and algorithmically process and analyze aggregated amounts of said spatiotemporal electromyographic signals to yield visually displayable, diagnostically-valuable physiological parameters of gastrointestinal smooth muscle electrical activity of said subject.

2. The particularly arranged array of bipolar electrode pairs of claim 1, where the distribution and orientation pattern allows for a maximum number of electrodes pairs to be arranged substantially orthogonally to each other in order to better sense signals originating from any orientation or location.

3. The system of claim 1, wherein said parameters comprise any of frequency, amplitude, power, or periodicity of electrical activity, as well as periodicity of larger time frame patterns of electrical activity, said parameters further assignable to a region of the gastrointestinal tract.

4. The communicating of said patches EMG data from claim 1 to said remote computing devices wirelessly, selected from the group consisting of Bluetooth, wifi, cellular, infrared, and the like.

5. The patches of claim 1, wherein said patches are selected from the group:

designed to be used as a larger number of smaller patches, to cover a large portion of the GI tract, so as to minimize lateral slippage and movement of electrodes,
designed so each electrode pair are aligned radially,
designed so each electrode pair are aligned along a circumferential line.

designed so one electrode is a ground electrode and is configured to pair with a plurality of active electrodes, each pairing representing a bipolar electrode pair, and
designed so the ground electrode is disposed centrally within a circumferential arrangement of the plurality of active electrodes.

6. The system of claim 1, wherein each of the EMG-sensing patches comprises a memory capacity sufficient to store accumulated signal for a period of up to at least one hour.

7. The system of claim 1, wherein the networked computing device comprises one or more data analysis applications, said applications configured to analyze data transmitted to it from the local electronic device, and said data analysis is selected from the group comprising,

individuation of processed data according to unique identifiers with which data coming from each patch is tagged,

desired signal isolation based on subtraction or relative weighting of patterns ascribable to sources other than gastrointestinal smooth muscle,

comprises inclusion of data directly entered into the local electronic device by the patient,

comprises inclusion of data entered directly into a computing device by a healthcare professional, and
comprises recognition of each EMG-sensing patch according to a coordinate-mapped location on the body of the patient.

8. The mathematical and algorithmic analysis of said aggregated large data sets of claim 1, wherein said analysis is selected from the group including time series analysis, time-dependent frequency analysis, and pattern matching analysis.

9. The subject of claim 1, wherein the subject includes both humans and animals, and said diagnostically-valuable physiological parameters are valuable for both diagnosing GI tract diseases, and diagnosing the effects of various foods, pharmaceutical drugs, and other substances on GI tract activity and health.

10. The subject of claim 1, wherein said subject is enabled in a manner selected from the group;

being able to go about their daily lives,

being able to manually enter consumed food descriptions into their medical records via portable, desktop, and handheld computing devices,

being able to manually enter qualitative or quantitative values of GI pain and its location, bloating, nausea and other disease symptoms experienced and their time experienced,

being able to take pictures of meals to be consumed as additional data to be included in the analysis,

being able to take pictures of meals to be consumed, with automated interpretation of nutritional content, as additional data to be included in the analysis,

being able to record still pictures, audio and video messages that are entered into their medical records.

11. The electrodiagnostic patch system of claim 1, further comprising additional sensors selected from the group comprising of accelerometers, motion sensors and position sen-

sors. heart rate sensor, blood pressure meter, respiration rate, blood oxygen levels, body temperature, galvanic skin response, skin-electrode impedance, electrode-electrode impedance, accelerometers, audio microphones, photography, videography, ECG and EEG.

12. A low-cost, non-invasive method of profiling gastrointestinal tract muscular activity of an ambulatory patient comprising:

placing at least one EMG-sensing patch on a skin surface of the patient proximate the gastrointestinal tract, said EMG-sensing patch comprising particularly selected arrays of bipolar electrode pairs;

acquiring electrical signals from one to all regions of the gastrointestinal tract with at least some subset of said plurality of electrode pairs arranged as arrays on each individual patch,

acquiring electrical signals from one or more regions of the gastrointestinal tract with at least some subset of said plurality of said EMG-sensing patches;

acquiring electrical signals at intervals ranging from intermittently to continuously from ambulatory patients living and behaving normally over at least a substantial portion of one day;

wirelessly transmitting said acquired electronic signal data to nearby networked computing devices; and

collecting, transmitting, and mathematically processing the acquired aggregated signals on any of the said computing devices to yield and display physiological parameters of gastrointestinal electrical activity collected from patients.

13. A non-invasive, wearable, low-cost full GI tract electrodiagnostic device and method, comprising:

a plurality of electromyographic-sensing wearable patches covering substantially all of the GI tract,

said patches adapted for placement on the skin surface of the midsection region of a subject,

said patches optionally available in a variety of sizes, shapes, and bipolar electrode densities and array distribution configurations, each said patch comprising at least one bipolar electrode pair,

said patch additionally enabled for intermittent to continuous, wireless communication of a signal indicative of a sensed, recorded, electromyographic signal;

said electrodes linked to an electronic devices, wherein said electronic devices include;

amplifier circuits, and

band pass filter circuits, and

analog to digital converter circuits, and

memory circuits, and

wireless data transmission circuits and associated antenna, and

a light, ultra-compact power source, and

a water-resistant housing,

said housing being made for multi-day adherence to said subjects body, and

said electronic device being in wireless communication with networked computing devices, and

wherein said networked computing device is configured to utilize advanced mathematical and algorithmic processes to analyze aggregate signals received from the local electronic device in order to yield remotely viewable physiological parameters of gastrointestinal smooth muscle electrical activity for the purposes of diagnosis and treatment of GI disorders.

* * * * *

专利名称(译)	可穿戴无线贴片，包含用于胃肠道电诊断的电极对阵列		
公开(公告)号	US20160045137A1	公开(公告)日	2016-02-18
申请号	US14/051440	申请日	2013-10-10
[标]申请(专利权)人(译)	中山市卓梅尼控制技术有限公司		
申请(专利权)人(译)	GTECH		
当前申请(专利权)人(译)	GTECH		
[标]发明人	AXELROD STEVE		
发明人	AXELROD, STEVE		
IPC分类号	A61B5/0488 A61B5/00 A61B5/0205 A61B5/04 A61B5/0492		
CPC分类号	A61B5/04882 A61B5/0492 A61B5/04012 A61B5/0004 A61B5/6823 A61B5/02055 A61B5/0476 A61B5/02438 A61B5/021 A61B5/0816 A61B5/14542 A61B5/0533 A61B5/0402 A61B5/1116 A61B5/04884		
优先权	61/712100 2012-10-10 US		
其他公开文献	US9943264		
外部链接	Espacenet USPTO		

摘要(译)

公开了一种用于描绘患者胃肠道肌肉的平滑肌中的电活动的系统和方法。该系统包括适于放置在患者腹部皮肤上的肌电图感应贴片。每个贴片具有至少一个双极电极对，或者以阵列排列的多个电极，并且能够传送指示所感测的肌电信号的信号。该系统还包括联网的计算设备。本地补丁设备被配置用于EMG感测补丁和本地计算设备之间的无线通信，以实现从补丁到联网计算设备的无线传输。联网计算设备被配置为处理从本地计算设备接收的多小时或天信号的大集合集合，以产生胃肠平滑肌电活动的诊断上有价值的生理参数。

