



US010448871B2

(12) **United States Patent**
Al-Ali

(10) **Patent No.:** **US 10,448,871 B2**
(45) **Date of Patent:** ***Oct. 22, 2019**

(54) **ADVANCED PULSE OXIMETRY SENSOR**

(71) Applicant: **MASIMO CORPORATION**, Irvine, CA (US)

(72) Inventor: **Ammar Al-Ali**, San Juan Capistrano, CA (US)

(73) Assignee: **Masimo Corporation**, Irvine, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 409 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **15/195,199**

(22) Filed: **Jun. 28, 2016**

(65) **Prior Publication Data**

US 2017/0000394 A1 Jan. 5, 2017

Related U.S. Application Data

(60) Provisional application No. 62/188,430, filed on Jul. 2, 2015.

(51) **Int. Cl.**
A61B 5/1455 (2006.01)
A61B 5/00 (2006.01)
(Continued)

(52) **U.S. Cl.**
CPC **A61B 5/1452** (2013.01); **A61B 5/0002** (2013.01); **A61B 5/02416** (2013.01);
(Continued)

(58) **Field of Classification Search**

None

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,960,128 A 10/1990 Gordon et al.
4,964,408 A 10/1990 Hink et al.
(Continued)

FOREIGN PATENT DOCUMENTS

EP 0781527 A1 7/1997
EP 2277440 A1 1/2011
WO WO 02/028274 4/2002

OTHER PUBLICATIONS

US 8,845,543 B2, 09/2014, Diab et al. (withdrawn)
(Continued)

Primary Examiner — Eric F Winakur


Assistant Examiner — Marjan Fardanesh

(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson & Bear, LLP

(57) **ABSTRACT**

A non-invasive, optical-based physiological monitoring system is disclosed. One embodiment includes an emitter configured to emit light. A diffuser is configured to receive and spread the emitted light, and to emit the spread light at a tissue measurement site. The system further includes a concentrator configured to receive the spread light after it has been attenuated by or reflected from the tissue measurement site. The concentrator is also configured to collect and concentrate the received light and to emit the concentrated light to a detector. The detector is configured to detect the concentrated light and to transmit a signal representative of the detected light. A processor is configured to receive the transmitted signal and to determine a physiological parameter, such as, for example, arterial oxygen saturation, in the tissue measurement site.

28 Claims, 7 Drawing Sheets

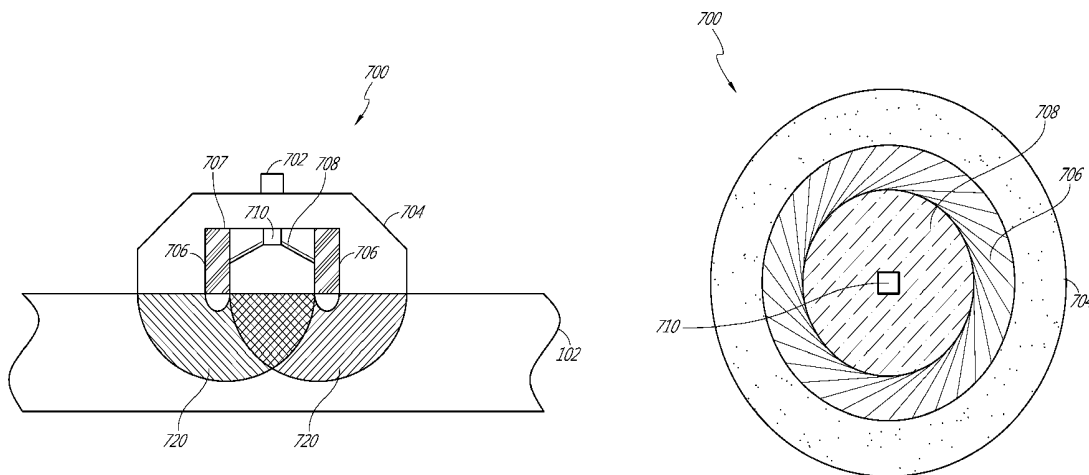

(51)	Int. Cl.		6,036,642 A	3/2000	Diab et al.
	A61B 5/024	(2006.01)	6,045,509 A	4/2000	Caro et al.
	A61B 5/145	(2006.01)	6,067,462 A	5/2000	Diab et al.
(52)	U.S. Cl.		6,081,735 A	6/2000	Diab et al.
	CPC	A61B 5/14532 (2013.01); A61B 5/14546 (2013.01); A61B 5/4875 (2013.01); A61B 5/6826 (2013.01); A61B 5/7278 (2013.01); A61B 5/742 (2013.01); A61B 2562/04 (2013.01)	6,088,607 A	7/2000	Diab et al.
			6,110,522 A	8/2000	Lepper, Jr. et al.
			6,124,597 A	9/2000	Shehada
			6,128,521 A	10/2000	Marro et al.
			6,129,675 A	10/2000	Jay
			6,144,868 A	11/2000	Parker
			6,151,516 A	11/2000	Kiani-Azarbayjany et al.
			6,152,754 A	11/2000	Gerhardt et al.
			6,157,850 A	12/2000	Diab et al.
			6,165,005 A	12/2000	Mills et al.
			6,184,521 B1	2/2001	Coffin, IV et al.
			6,206,830 B1	3/2001	Diab et al.
			6,223,063 B1	4/2001	Chaiken et al.
			6,229,856 B1	5/2001	Diab et al.
			6,232,609 B1	5/2001	Snyder et al.
			6,236,872 B1	5/2001	Diab et al.
			6,241,683 B1	6/2001	Macklem et al.
			6,253,097 B1	6/2001	Aronow et al.
		6,256,523 B1	7/2001	Diab et al.	
		6,263,222 B1	7/2001	Diab et al.	
		6,278,522 B1	8/2001	Lepper, Jr. et al.	
		6,280,213 B1	8/2001	Tobler et al.	
		6,285,896 B1	9/2001	Tobler et al.	
		6,301,493 B1	10/2001	Marro et al.	
		6,308,089 B1	10/2001	von der Ruhr et al.	
		6,317,627 B1	11/2001	Ennen et al.	
		6,321,100 B1	11/2001	Parker	
		6,325,761 B1	12/2001	Jay	
		6,334,065 B1	12/2001	Al-Ali et al.	
		6,343,223 B1 *	1/2002	Chin A61B 5/14552 600/323	
			6,343,224 B1	1/2002	Parker
			6,349,228 B1	2/2002	Kiani et al.
			6,360,114 B1	3/2002	Diab et al.
			6,368,283 B1	4/2002	Xu et al.
			6,371,921 B1	4/2002	Caro et al.
			6,377,829 B1	4/2002	Al-Ali
			6,388,240 B2	5/2002	Schulz et al.
			6,397,091 B2	5/2002	Diab et al.
			6,430,437 B1	8/2002	Marro
			6,430,525 B1	8/2002	Weber et al.
			6,463,311 B1	10/2002	Diab
			6,470,199 B1	10/2002	Kopotic et al.
			6,501,975 B2	12/2002	Diab et al.
			6,505,059 B1	1/2003	Kollias et al.
			6,515,273 B2	2/2003	Al-Ali
			6,519,487 B1	2/2003	Parker
			6,525,386 B1	2/2003	Mills et al.
			6,526,300 B1	2/2003	Kiani et al.
			6,541,756 B2	4/2003	Schulz et al.
			6,542,764 B1	4/2003	Al-Ali et al.
			6,580,086 B1	6/2003	Schulz et al.
			6,584,336 B1	6/2003	Ali et al.
			6,595,316 B2	7/2003	Cybulski et al.
			6,597,932 B2	7/2003	Tian et al.
			6,597,933 B2	7/2003	Kiani et al.
			6,606,511 B1	8/2003	Ali et al.
			6,632,181 B2	10/2003	Flaherty et al.
			6,639,668 B1	10/2003	Trepagnier
			6,640,116 B2	10/2003	Diab
			6,643,530 B2	11/2003	Diab et al.
			6,650,917 B2	11/2003	Diab et al.
			6,654,624 B2	11/2003	Diab et al.
			6,658,276 B2	12/2003	Kiani et al.
			6,661,161 B1	12/2003	Lanzo et al.
			6,671,526 B1	12/2003	Aoyagi et al.
			6,671,531 B2	12/2003	Al-Ali et al.
			6,678,543 B2	1/2004	Diab et al.
			6,684,090 B2	1/2004	Ali et al.
			6,684,091 B2	1/2004	Parker
			6,697,656 B1	2/2004	Al-Ali
			6,697,657 B1	2/2004	Shehada et al.
			6,697,658 B2	2/2004	Al-Ali
			RE38,476 E	3/2004	Diab et al.
			6,699,194 B1	3/2004	Diab et al.
(56)	References Cited				
	U.S. PATENT DOCUMENTS				
	5,041,187 A	8/1991	Hink et al.		
	5,069,213 A	12/1991	Polczynski		
	5,099,842 A	3/1992	Mannheimer et al.		
	5,163,438 A	11/1992	Gordon et al.		
	5,319,355 A	6/1994	Russek		
	5,337,744 A	8/1994	Branigan		
	5,341,805 A	8/1994	Stavridi et al.		
	D353,195 S	12/1994	Savage et al.		
	D353,196 S	12/1994	Savage et al.		
	5,377,676 A	1/1995	Vari et al.		
	D359,546 S	6/1995	Savage et al.		
	5,431,170 A	7/1995	Mathews		
	D361,840 S	8/1995	Savage et al.		
	D362,063 S	9/1995	Savage et al.		
	5,452,717 A	9/1995	Branigan et al.		
	D363,120 S	10/1995	Savage et al.		
	5,456,252 A	10/1995	Vari et al.		
	5,479,934 A	1/1996	Imran		
	5,482,036 A	1/1996	Diab et al.		
	5,490,505 A	2/1996	Diab et al.		
	5,494,043 A	2/1996	O'Sullivan et al.		
	5,497,771 A *	3/1996	Rosenheimer A61B 5/14542 600/323		
	5,533,511 A	7/1996	Kaspari et al.		
	5,534,851 A	7/1996	Russek		
	5,561,275 A	10/1996	Savage et al.		
	5,562,002 A	10/1996	Lalin		
	5,584,296 A *	12/1996	Cui A61B 5/14552 356/41		
	5,590,649 A	1/1997	Caro et al.		
	5,601,079 A	2/1997	Wong et al.		
	5,602,924 A	2/1997	Durand et al.		
	5,623,925 A	4/1997	Swenson et al.		
	5,632,272 A	5/1997	Diab et al.		
	5,638,816 A	6/1997	Kiani-Azarbayjany et al.		
	5,638,818 A	6/1997	Diab et al.		
	5,645,440 A	7/1997	Tobler et al.		
	5,685,299 A	11/1997	Diab et al.		
	D393,830 S	4/1998	Tobler et al.		
	5,743,262 A	4/1998	Lepper, Jr. et al.		
	5,758,644 A	6/1998	Diab et al.		
	5,760,910 A	6/1998	Lepper, Jr. et al.		
	5,769,785 A	6/1998	Diab et al.		
	5,782,757 A	7/1998	Diab et al.		
	5,785,659 A	7/1998	Caro et al.		
	5,791,347 A	8/1998	Flaherty et al.		
	5,810,734 A	9/1998	Caro et al.		
	5,823,950 A	10/1998	Diab et al.		
	5,830,131 A	11/1998	Caro et al.		
	5,830,137 A	11/1998	Scharf		
	5,833,618 A	11/1998	Caro et al.		
	5,860,919 A	1/1999	Kiani-Azarbayjany et al.		
	5,890,929 A	4/1999	Mills et al.		
	5,904,654 A	5/1999	Wohltmann et al.		
	5,919,134 A	7/1999	Diab		
	5,934,925 A	8/1999	Tobler et al.		
	5,940,182 A	8/1999	Lepper, Jr. et al.		
	5,987,343 A	11/1999	Kinast		
	5,995,855 A	11/1999	Kiani et al.		
	5,997,343 A	12/1999	Mills et al.		
	6,002,952 A	12/1999	Diab et al.		
	6,011,986 A	1/2000	Diab et al.		
	6,027,452 A	2/2000	Flaherty et al.		

(56)

References Cited

U.S. PATENT DOCUMENTS

6,714,804 B2	3/2004	Al-Ali et al.	7,341,559 B2	3/2008	Schulz et al.
RE38,492 E	4/2004	Diab et al.	7,343,186 B2	3/2008	Lamego et al.
6,721,582 B2	4/2004	Trepagnier et al.	D566,282 S	4/2008	Al-Ali et al.
6,721,585 B1	4/2004	Parker	7,355,512 B1	4/2008	Al-Ali
6,725,075 B2	4/2004	Al-Ali	7,356,365 B2	4/2008	Schurman
6,728,560 B2	4/2004	Kollias et al.	7,371,981 B2	5/2008	Abdul-Hafiz
6,735,459 B2	5/2004	Parker	7,373,193 B2	5/2008	Al-Ali et al.
6,745,060 B2	6/2004	Diab et al.	7,373,194 B2	5/2008	Weber et al.
6,760,607 B2	7/2004	Al-Ali	7,376,453 B1	5/2008	Diab et al.
6,770,028 B1	8/2004	Ali et al.	7,377,794 B2	5/2008	Al-Ali et al.
6,771,994 B2	8/2004	Kiani et al.	7,377,899 B2	5/2008	Weber et al.
6,792,300 B1	9/2004	Diab et al.	7,383,070 B2	6/2008	Diab et al.
6,813,511 B2	11/2004	Diab et al.	7,415,297 B2	8/2008	Al-Ali et al.
6,816,741 B2	11/2004	Diab	7,428,432 B2	9/2008	Ali et al.
6,822,564 B2	11/2004	Al-Ali	7,438,683 B2	10/2008	Al-Ali et al.
6,826,419 B2	11/2004	Diab et al.	7,440,787 B2	10/2008	Diab
6,830,711 B2	12/2004	Mills et al.	7,454,240 B2	11/2008	Diab et al.
6,850,787 B2	2/2005	Weber et al.	7,467,002 B2	12/2008	Weber et al.
6,850,788 B2	2/2005	Al-Ali	7,469,157 B2	12/2008	Diab et al.
6,852,083 B2	2/2005	Caro et al.	7,471,969 B2	12/2008	Diab et al.
6,861,639 B2	3/2005	Al-Ali	7,471,971 B2	12/2008	Diab et al.
6,898,452 B2	5/2005	Al-Ali et al.	7,483,729 B2	1/2009	Al-Ali et al.
6,920,345 B2	7/2005	Al-Ali et al.	7,483,730 B2	1/2009	Diab et al.
6,931,268 B1	8/2005	Kiani-Azarbayjany et al.	7,489,958 B2	2/2009	Diab et al.
6,934,570 B2	8/2005	Kiani et al.	7,496,391 B2	2/2009	Diab et al.
6,939,305 B2	9/2005	Flaherty et al.	7,496,393 B2	2/2009	Diab et al.
6,943,348 B1	9/2005	Coffin, IV	D587,657 S	3/2009	Al-Ali et al.
6,950,687 B2	9/2005	Al-Ali	7,499,741 B2	3/2009	Diab et al.
6,961,598 B2	11/2005	Diab	7,499,835 B2	3/2009	Weber et al.
6,970,792 B1	11/2005	Diab	7,500,950 B2	3/2009	Al-Ali et al.
6,979,812 B2	12/2005	Al-Ali	7,509,154 B2	3/2009	Diab et al.
6,985,764 B2	1/2006	Mason et al.	7,509,494 B2	3/2009	Al-Ali
6,993,371 B2	1/2006	Kiani et al.	7,510,849 B2	3/2009	Schurman et al.
6,996,427 B2	2/2006	Ali et al.	7,519,327 B2	4/2009	White
6,999,904 B2	2/2006	Weber et al.	7,526,328 B2	4/2009	Diab et al.
7,003,338 B2	2/2006	Weber et al.	7,530,942 B1	5/2009	Diab
7,003,339 B2	2/2006	Diab et al.	7,530,949 B2	5/2009	Al Ali et al.
7,015,451 B2	3/2006	Dalke et al.	7,530,955 B2	5/2009	Diab et al.
7,024,233 B2	4/2006	Ali et al.	7,563,110 B2	7/2009	Al-Ali et al.
7,027,849 B2	4/2006	Al-Ali	7,596,398 B2	9/2009	Al-Ali et al.
7,030,749 B2	4/2006	Al-Ali	7,601,123 B2	10/2009	Tweed et al.
7,039,449 B2	5/2006	Al-Ali	7,618,375 B2	11/2009	Flaherty
7,041,060 B2	5/2006	Flaherty et al.	D606,659 S	12/2009	Kiani et al.
7,044,918 B2	5/2006	Diab	7,647,083 B2	1/2010	Al-Ali et al.
7,048,687 B1	5/2006	Reuss et al.	D609,193 S	2/2010	Al-Ali et al.
7,067,893 B2	6/2006	Mills et al.	D614,305 S	4/2010	Al-Ali et al.
7,096,052 B2	8/2006	Mason et al.	RE41,317 E	5/2010	Parker
7,096,054 B2	8/2006	Abdul-Hafiz et al.	7,726,209 B2	6/2010	Ruotoistenmäki
7,132,641 B2	11/2006	Schulz et al.	7,729,733 B2	6/2010	Al-Ali et al.
7,142,901 B2	11/2006	Kiani et al.	7,734,320 B2	6/2010	Al-Ali
7,149,561 B2	12/2006	Diab	7,761,127 B2	7/2010	Al-Ali et al.
7,186,966 B2	3/2007	Al-Ali	7,761,128 B2	7/2010	Al-Ali et al.
7,190,261 B2	3/2007	Al-Ali	7,764,982 B2	7/2010	Dalke et al.
7,215,984 B2	5/2007	Diab	D621,516 S	8/2010	Kiani et al.
7,215,986 B2	5/2007	Diab	7,791,155 B2	9/2010	Diab
7,221,971 B2	5/2007	Diab	7,801,581 B2	9/2010	Diab
7,225,006 B2	5/2007	Al-Ali et al.	7,822,452 B2	10/2010	Schurman et al.
7,225,007 B2	5/2007	Al-Ali	RE41,912 E	11/2010	Parker
RE39,672 E	6/2007	Shehada et al.	7,844,313 B2	11/2010	Kiani et al.
7,239,905 B2	7/2007	Kiani-Azarbayjany et al.	7,844,314 B2	11/2010	Al-Ali
7,245,953 B1	7/2007	Parker	7,844,315 B2	11/2010	Al-Ali
7,254,429 B2	8/2007	Schurman et al.	7,862,523 B2	1/2011	Ruotoistenmaki
7,254,431 B2	8/2007	Al-Ali	7,865,222 B2	1/2011	Weber et al.
7,254,433 B2	8/2007	Diab et al.	7,873,497 B2	1/2011	Weber et al.
7,254,434 B2	8/2007	Schulz et al.	7,880,606 B2	2/2011	Al-Ali
7,272,425 B2	9/2007	Al-Ali	7,880,626 B2	2/2011	Al-Ali et al.
7,274,955 B2	9/2007	Kiani et al.	7,891,355 B2	2/2011	Al-Ali et al.
D554,263 S	10/2007	Al-Ali	7,894,868 B2	2/2011	Al-Ali et al.
7,280,858 B2	10/2007	Al-Ali et al.	7,899,507 B2	3/2011	Al-Ali et al.
7,289,835 B2	10/2007	Mansfield et al.	7,899,518 B2	3/2011	Trepagnier et al.
7,292,883 B2	11/2007	De Felice et al.	7,904,132 B2	3/2011	Weber et al.
7,295,866 B2	11/2007	Al-Ali	7,909,772 B2	3/2011	Popov et al.
7,328,053 B1	2/2008	Diab et al.	7,910,875 B2	3/2011	Al-Ali
7,332,784 B2	2/2008	Mills et al.	7,919,713 B2	4/2011	Al-Ali et al.
7,340,287 B2	3/2008	Mason et al.	7,937,128 B2	5/2011	Al-Ali
			7,937,129 B2	5/2011	Mason et al.
			7,937,130 B2	5/2011	Diab et al.
			7,941,199 B2	5/2011	Kiani
			7,951,086 B2	5/2011	Flaherty et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

7,957,780 B2	6/2011	Lamego et al.	8,437,825 B2	5/2013	Dalvi et al.
7,962,188 B2	6/2011	Kiani et al.	8,452,364 B2	5/2013	Hannula et al.
7,962,190 B1	6/2011	Diab et al.	8,455,290 B2	6/2013	Siskavich
7,976,472 B2	7/2011	Kiani	8,457,703 B2	6/2013	Al-Ali
7,988,637 B2	8/2011	Diab	8,457,707 B2	6/2013	Kiani
7,990,382 B2	8/2011	Kiani	8,463,349 B2	6/2013	Diab et al.
7,991,446 B2	8/2011	Al-Ali et al.	8,466,286 B2	6/2013	Bellot et al.
8,000,761 B2	8/2011	Al-Ali	8,471,713 B2	6/2013	Poeze et al.
8,008,088 B2	8/2011	Bellott et al.	8,473,020 B2	6/2013	Kiani et al.
RE42,753 E	9/2011	Kiani-Azarbayjany et al.	8,483,787 B2	7/2013	Al-Ali et al.
8,019,400 B2	9/2011	Diab et al.	8,489,364 B2	7/2013	Weber et al.
8,028,701 B2	10/2011	Al-Ali et al.	8,498,684 B2	7/2013	Weber et al.
8,029,765 B2	10/2011	Bellott et al.	8,504,128 B2	8/2013	Blank et al.
8,036,727 B2	10/2011	Schurman et al.	8,509,867 B2	8/2013	Workman et al.
8,036,728 B2	10/2011	Diab et al.	8,515,509 B2	8/2013	Bruinsma et al.
8,046,040 B2	10/2011	Ali et al.	8,523,781 B2	9/2013	Al-Ali
8,046,041 B2	10/2011	Diab et al.	8,529,301 B2	9/2013	Al-Ali et al.
8,046,042 B2	10/2011	Diab et al.	8,532,727 B2	9/2013	Ali et al.
8,048,040 B2	11/2011	Kiani	8,532,728 B2	9/2013	Diab et al.
8,050,728 B2	11/2011	Al-Ali et al.	D692,145 S	10/2013	Al-Ali et al.
RE43,169 E	2/2012	Parker	8,547,209 B2	10/2013	Kiani et al.
8,118,620 B2	2/2012	Al-Ali et al.	8,548,548 B2	10/2013	Al-Ali
8,126,528 B2	2/2012	Diab et al.	8,548,549 B2	10/2013	Schurman et al.
8,128,572 B2	3/2012	Diab et al.	8,548,550 B2	10/2013	Al-Ali et al.
8,130,105 B2	3/2012	Al-Ali et al.	8,560,032 B2	10/2013	Al-Ali et al.
8,145,287 B2	3/2012	Diab et al.	8,560,034 B1	10/2013	Diab et al.
8,150,487 B2	4/2012	Diab et al.	8,570,167 B2	10/2013	Al-Ali
8,175,672 B2	5/2012	Parker	8,570,503 B2	10/2013	Vo et al.
8,180,420 B2	5/2012	Diab et al.	8,571,617 B2	10/2013	Reichgott et al.
8,182,443 B1	5/2012	Kiani	8,571,618 B1	10/2013	Lamego et al.
8,185,180 B2	5/2012	Diab et al.	8,571,619 B2	10/2013	Al-Ali et al.
8,190,223 B2	5/2012	Al-Ali et al.	8,577,431 B2	11/2013	Lamego et al.
8,190,227 B2	5/2012	Diab et al.	8,581,732 B2	11/2013	Al-Ali et al.
8,203,438 B2	6/2012	Kiani et al.	8,584,345 B2	11/2013	Al-Ali et al.
8,203,704 B2	6/2012	Merritt et al.	8,588,880 B2	11/2013	Abdul-Hafiz et al.
8,204,566 B2	6/2012	Schurman et al.	8,600,467 B2	12/2013	Al-Ali et al.
8,219,172 B2	7/2012	Schurman et al.	8,606,342 B2	12/2013	Diab
8,224,411 B2	7/2012	Al-Ali et al.	8,615,290 B2	12/2013	Lin et al.
8,228,181 B2	7/2012	Al-Ali	8,626,255 B2	1/2014	Al-Ali et al.
8,229,533 B2	7/2012	Diab et al.	8,630,691 B2	1/2014	Lamego et al.
8,233,955 B2	7/2012	Al-Ali et al.	8,634,889 B2	1/2014	Al-Ali et al.
8,244,325 B2	8/2012	Al-Ali et al.	8,641,631 B2	2/2014	Sierra et al.
8,255,026 B1	8/2012	Al-Ali	8,652,060 B2	2/2014	Al-Ali
8,255,027 B2	8/2012	Al-Ali et al.	8,655,004 B2	2/2014	Prest et al.
8,255,028 B2	8/2012	Al-Ali et al.	8,663,107 B2	3/2014	Kiani
8,260,577 B2	9/2012	Weber et al.	8,666,468 B1	3/2014	Al-Ali
8,265,723 B1	9/2012	McHale et al.	8,667,967 B2	3/2014	Al-Ali et al.
8,274,360 B2	9/2012	Sampath et al.	8,670,811 B2	3/2014	O'Reilly
8,280,473 B2	10/2012	Al-Ali	8,670,814 B2	3/2014	Diab et al.
8,289,130 B2	10/2012	Nakajima et al.	8,676,286 B2	3/2014	Weber et al.
8,301,217 B2	10/2012	Al-Ali et al.	8,682,407 B2	3/2014	Al-Ali
8,306,596 B2	11/2012	Schurman et al.	RE44,823 E	4/2014	Parker
8,310,336 B2	11/2012	Muhsin et al.	RE44,875 E	4/2014	Kiani et al.
8,315,683 B2	11/2012	Al-Ali et al.	8,690,799 B2	4/2014	Telfort et al.
RE43,860 E	12/2012	Parker	8,700,112 B2	4/2014	Kiani
8,337,403 B2	12/2012	Al-Ali et al.	8,702,627 B2	4/2014	Telfort et al.
8,346,330 B2	1/2013	Lamego	8,706,179 B2	4/2014	Parker
8,353,842 B2	1/2013	Al-Ali et al.	8,712,494 B1	4/2014	MacNeish, III et al.
8,355,766 B2	1/2013	MacNeish, III et al.	8,715,206 B2	5/2014	Telfort et al.
8,359,080 B2	1/2013	Diab et al.	8,718,735 B2	5/2014	Lamego et al.
8,364,223 B2	1/2013	Al-Ali et al.	8,718,737 B2	5/2014	Diab et al.
8,364,226 B2	1/2013	Diab et al.	8,718,738 B2	5/2014	Blank et al.
8,364,389 B2	1/2013	Dorogusker et al.	8,720,249 B2	5/2014	Al-Ali
8,374,665 B2	2/2013	Lamego	8,721,541 B2	5/2014	Al-Ali et al.
8,385,995 B2	2/2013	Al-Ali et al.	8,721,542 B2	5/2014	Al-Ali et al.
8,385,996 B2	2/2013	Smith et al.	8,723,677 B1	5/2014	Kiani
8,388,353 B2	3/2013	Kiani et al.	8,740,792 B1	6/2014	Kiani et al.
8,399,822 B2	3/2013	Al-Ali	8,754,776 B2	6/2014	Poeze et al.
8,401,602 B2	3/2013	Kiani	8,755,535 B2	6/2014	Telfort et al.
8,405,608 B2	3/2013	Al-Ali et al.	8,755,856 B2	6/2014	Diab et al.
8,414,499 B2	4/2013	Al-Ali et al.	8,755,872 B1	6/2014	Marinow
8,418,524 B2	4/2013	Al-Ali	8,760,517 B2	6/2014	Sarwar et al.
8,423,106 B2	4/2013	Lamego et al.	8,761,850 B2	6/2014	Lamego
8,428,967 B2	4/2013	Olsen et al.	8,764,671 B2	7/2014	Kiani
8,430,817 B1	4/2013	Al-Ali et al.	8,768,423 B2	7/2014	Shakespeare et al.
			8,771,204 B2	7/2014	Telfort et al.
			8,777,634 B2	7/2014	Kiani et al.
			8,781,543 B2	7/2014	Diab et al.
			8,781,544 B2	7/2014	Al-Ali et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

8,781,549	B2	7/2014	Al-Ali et al.	9,218,454	B2	12/2015	Kiani et al.
8,788,003	B2	7/2014	Schurman et al.	9,226,696	B2	1/2016	Kiani
8,790,268	B2	7/2014	Al-Ali	9,241,662	B2	1/2016	Al-Ali et al.
8,801,613	B2	8/2014	Al-Ali et al.	9,245,668	B1	1/2016	Vo et al.
8,821,397	B2	9/2014	Al-Ali et al.	9,259,185	B2	2/2016	Abdul-Hafiz et al.
8,821,415	B2	9/2014	Al-Ali et al.	9,267,572	B2	2/2016	Barker et al.
8,830,449	B1	9/2014	Lamego et al.	9,277,880	B2	3/2016	Poeze et al.
8,831,700	B2	9/2014	Schurman et al.	9,289,167	B2	3/2016	Diab et al.
8,840,549	B2	9/2014	Al-Ali et al.	9,295,421	B2	3/2016	Kiani et al.
8,847,740	B2	9/2014	Kiani et al.	9,307,928	B1	4/2016	Al-Ali et al.
8,849,365	B2	9/2014	Smith et al.	9,311,382	B2	4/2016	Varoglu et al.
8,852,094	B2	10/2014	Al-Ali et al.	9,323,894	B2	4/2016	Kiani
8,852,994	B2	10/2014	Wojtczuk et al.	D755,392	S	5/2016	Hwang et al.
8,868,147	B2	10/2014	Stippick et al.	9,326,712	B1	5/2016	Kiani
8,868,150	B2	10/2014	Al-Ali et al.	9,333,316	B2	5/2016	Kiani
8,870,792	B2	10/2014	Al-Ali et al.	9,339,220	B2	5/2016	Lamego et al.
8,886,271	B2	11/2014	Kiani et al.	9,341,565	B2	5/2016	Lamego et al.
8,888,539	B2	11/2014	Al-Ali et al.	9,351,673	B2	5/2016	Diab et al.
8,888,708	B2	11/2014	Diab et al.	9,351,675	B2	5/2016	Al-Ali et al.
8,892,180	B2	11/2014	Weber et al.	9,357,665	B2	5/2016	Myers et al.
8,897,847	B2	11/2014	Al-Ali	9,364,181	B2	6/2016	Kiani et al.
8,909,310	B2	12/2014	Lamego et al.	9,368,671	B2	6/2016	Wojtczuk et al.
8,911,377	B2	12/2014	Al-Ali	9,370,325	B2	6/2016	Al-Ali et al.
8,912,909	B2	12/2014	Al-Ali et al.	9,370,326	B2	6/2016	McHale et al.
8,920,317	B2	12/2014	Al-Ali et al.	9,370,335	B2	6/2016	Al-Ali et al.
8,921,699	B2	12/2014	Al-Ali et al.	9,375,185	B2	6/2016	Ali et al.
8,922,382	B2	12/2014	Al-Ali et al.	9,386,953	B2	7/2016	Al-Ali
8,929,964	B2	1/2015	Al-Ali et al.	9,386,961	B2	7/2016	Al-Ali et al.
8,942,777	B2	1/2015	Diab et al.	9,392,945	B2	7/2016	Al-Ali et al.
8,948,834	B2	2/2015	Diab et al.	9,397,448	B2	7/2016	Al-Ali et al.
8,948,835	B2	2/2015	Diab	9,408,542	B1	8/2016	Kinast et al.
8,965,471	B2	2/2015	Lamego	9,436,645	B2	9/2016	Al-Ali et al.
8,983,564	B2	3/2015	Al-Ali	9,445,759	B1	9/2016	Lamego et al.
8,989,831	B2	3/2015	Al-Ali et al.	9,466,919	B2	10/2016	Kiani et al.
8,996,085	B2	3/2015	Kiani et al.	9,474,474	B2	10/2016	Lamego et al.
8,998,809	B2	4/2015	Kiani	9,480,422	B2	11/2016	Al-Ali
9,028,429	B2	5/2015	Telfort et al.	9,480,435	B2	11/2016	Olsen
9,037,207	B2	5/2015	Al-Ali et al.	9,489,081	B2	11/2016	Anzures et al.
9,060,721	B2	6/2015	Reichgott et al.	9,492,110	B2	11/2016	Al-Ali et al.
9,066,666	B2	6/2015	Kiani	9,497,534	B2	11/2016	Prest et al.
9,066,680	B1	6/2015	Al-Ali et al.	9,510,779	B2	12/2016	Poeze et al.
9,072,437	B2	7/2015	Paalasmaa	9,517,024	B2	12/2016	Kiani et al.
9,072,474	B2	7/2015	Al-Ali et al.	9,526,430	B2	12/2016	Srinivas et al.
9,078,560	B2	7/2015	Schurman et al.	9,532,722	B2	1/2017	Lamego et al.
9,081,889	B2	7/2015	Ingrassia, Jr. et al.	9,538,949	B2	1/2017	Al-Ali et al.
9,084,569	B2	7/2015	Weber et al.	9,538,980	B2	1/2017	Telfort et al.
9,095,316	B2	8/2015	Welch et al.	9,549,696	B2	1/2017	Lamego et al.
9,106,038	B2	8/2015	Telfort et al.	9,553,625	B2	1/2017	Hatanaka et al.
9,107,625	B2	8/2015	Telfort et al.	9,554,737	B2	1/2017	Schurman et al.
9,107,626	B2	8/2015	Al-Ali et al.	9,560,996	B2	2/2017	Kiani
9,113,831	B2	8/2015	Al-Ali	9,560,998	B2	2/2017	Al-Ali et al.
9,113,832	B2	8/2015	Al-Ali	9,566,019	B2	2/2017	Al-Ali et al.
9,119,595	B2	9/2015	Lamego	9,579,039	B2	2/2017	Jansen et al.
9,131,881	B2	9/2015	Diab et al.	9,591,975	B2	3/2017	Dalvi et al.
9,131,882	B2	9/2015	Al-Ali et al.	9,593,969	B2	3/2017	King
9,131,883	B2	9/2015	Al-Ali	9,622,692	B2	4/2017	Lamego et al.
9,131,917	B2	9/2015	Telfort et al.	9,622,693	B2	4/2017	Diab
9,138,180	B1	9/2015	Coverston et al.	D788,312	S	5/2017	Al-Ali et al.
9,138,182	B2	9/2015	Al-Ali et al.	9,636,055	B2	5/2017	Al-Ali et al.
9,138,192	B2	9/2015	Weber et al.	9,636,056	B2	5/2017	Al-Ali
9,142,117	B2	9/2015	Muhsin et al.	9,649,054	B2	5/2017	Lamego et al.
9,153,112	B1	10/2015	Kiani et al.	9,651,405	B1	5/2017	Gowreesunker et al.
9,153,121	B2	10/2015	Kiani et al.	9,662,052	B2	5/2017	Al-Ali et al.
9,161,696	B2	10/2015	Al-Ali et al.	9,668,676	B2	6/2017	Culbert
9,161,713	B2	10/2015	Al-Ali et al.	9,668,679	B2	6/2017	Schurman et al.
9,167,995	B2	10/2015	Lamego et al.	9,668,680	B2	6/2017	Bruinsma et al.
9,176,141	B2	11/2015	Al-Ali et al.	9,668,703	B2	6/2017	Al-Ali
9,186,102	B2	11/2015	Bruinsma et al.	9,675,286	B2	6/2017	Diab
9,192,312	B2	11/2015	Al-Ali	9,687,160	B2	6/2017	Kiani
9,192,329	B2	11/2015	Al-Ali	9,693,719	B2	7/2017	Al-Ali et al.
9,192,351	B1	11/2015	Telfort et al.	9,693,737	B2	7/2017	Al-Ali
9,195,385	B2	11/2015	Al-Ali et al.	9,697,928	B2	7/2017	Al-Ali et al.
9,210,566	B2	12/2015	Ziemianska et al.	9,699,546	B2	7/2017	Qian et al.
9,211,072	B2	12/2015	Kiani	9,716,937	B2	7/2017	Qian et al.
9,211,095	B1	12/2015	Al-Ali	9,717,425	B2	8/2017	Kiani et al.
				9,717,458	B2	8/2017	Lamego et al.
				9,723,997	B1	8/2017	Lamego
				9,724,016	B1	8/2017	Al-Ali et al.
				9,724,024	B2	8/2017	Al-Ali

(56)

References Cited

U.S. PATENT DOCUMENTS

9,724,025 B1	8/2017	Kiani et al.	10,058,275 B2	8/2018	Al-Ali et al.
9,730,640 B2	8/2017	Diab et al.	10,064,562 B2	9/2018	Al-Ali
9,743,887 B2	8/2017	Al-Ali et al.	10,066,970 B2	9/2018	Gowreesunker et al.
9,749,232 B2	8/2017	Sampath et al.	10,076,257 B2	9/2018	Lin et al.
9,750,442 B2	9/2017	Olsen	10,078,052 B2	9/2018	Ness et al.
9,750,443 B2	9/2017	Smith et al.	10,086,138 B1	10/2018	Novak, Jr.
9,750,461 B1	9/2017	Telfort	10,092,200 B2	10/2018	Al-Ali et al.
9,775,545 B2	10/2017	Al-Ali et al.	10,092,249 B2	10/2018	Kiani et al.
9,775,546 B2	10/2017	Diab et al.	10,098,550 B2	10/2018	Al-Ali et al.
9,775,570 B2	10/2017	Al-Ali	10,098,591 B2	10/2018	Al-Ali et al.
9,778,079 B1	10/2017	Al-Ali et al.	10,098,610 B2	10/2018	Al-Ali et al.
9,781,984 B2	10/2017	Baranski et al.	D833,624 S	11/2018	DeJong et al.
9,782,077 B2	10/2017	Lamego et al.	10,123,726 B2	11/2018	Al-Ali et al.
9,782,110 B2	10/2017	Kiani	10,130,289 B2	11/2018	Al-Ali et al.
9,787,568 B2	10/2017	Lamego et al.	10,130,291 B2	11/2018	Schurman et al.
9,788,735 B2	10/2017	Al-Ali	D835,282 S	12/2018	Barker et al.
9,788,768 B2	10/2017	Al-Ali et al.	D835,283 S	12/2018	Barker et al.
9,795,300 B2	10/2017	Al-Ali	D835,284 S	12/2018	Barker et al.
9,795,310 B2	10/2017	Al-Ali	D835,285 S	12/2018	Barker et al.
9,795,358 B2	10/2017	Telfort et al.	10,149,616 B2	12/2018	Al-Ali et al.
9,795,739 B2	10/2017	Al-Ali et al.	10,154,815 B2	12/2018	Al-Ali et al.
9,801,556 B2	10/2017	Kiani	10,159,412 B2	12/2018	Lamego et al.
9,801,588 B2	10/2017	Weber et al.	10,188,296 B2	1/2019	Al-Ali et al.
9,808,188 B1	11/2017	Perea et al.	10,188,331 B1	1/2019	Al-Ali et al.
9,814,418 B2	11/2017	Weber et al.	10,188,348 B2	1/2019	Kiani et al.
9,820,691 B2	11/2017	Kiani	RE47,218 E	2/2019	Al-Ali
9,833,152 B2	12/2017	Kiani et al.	RE47,244 E	2/2019	Kiani et al.
9,833,180 B2	12/2017	Shakespeare et al.	RE47,249 E	2/2019	Kiani et al.
9,838,775 B2	12/2017	Qian et al.	10,194,847 B2	2/2019	Al-Ali
9,839,379 B2	12/2017	Al-Ali et al.	10,194,848 B1	2/2019	Kiani et al.
9,839,381 B1	12/2017	Weber et al.	10,201,298 B2	2/2019	Al-Ali et al.
9,847,002 B2	12/2017	Kiani et al.	10,205,272 B2	2/2019	Kiani et al.
9,847,749 B2	12/2017	Kiani et al.	10,205,291 B2	2/2019	Scruggs et al.
9,848,800 B1	12/2017	Lee et al.	10,213,108 B2	2/2019	Al-Ali
9,848,806 B2	12/2017	Al-Ali et al.	10,219,706 B2	3/2019	Al-Ali
9,848,807 B2	12/2017	Lamego	10,219,746 B2	3/2019	McHale et al.
9,848,823 B2	12/2017	Raghuram et al.	10,226,187 B2	3/2019	Al-Ali et al.
9,861,298 B2	1/2018	Eckerbom et al.	10,226,576 B2	3/2019	Kiani
9,861,304 B2	1/2018	Al-Ali et al.	10,231,657 B2	3/2019	Al-Ali et al.
9,861,305 B1	1/2018	Weber et al.	10,231,670 B2	3/2019	Blank et al.
9,866,671 B1	1/2018	Thompson et al.	10,231,676 B2	3/2019	Al-Ali et al.
9,867,575 B2	1/2018	Maani et al.	RE47,353 E	4/2019	Kiani et al.
9,867,578 B2	1/2018	Al-Ali et al.	10,251,585 B2	4/2019	Al-Ali et al.
9,872,623 B2	1/2018	Al-Ali	10,251,586 B2	4/2019	Lamego
9,876,320 B2	1/2018	Coverston et al.	10,255,994 B2	4/2019	Sampath et al.
9,877,650 B2	1/2018	Muhsin et al.	10,258,265 B1	4/2019	Poeze et al.
9,877,686 B2	1/2018	Al-Ali et al.	10,258,266 B1	4/2019	Poeze et al.
9,891,079 B2	2/2018	Dalvi	10,271,748 B2	4/2019	Al-Ali
9,895,107 B2	2/2018	Al-Ali et al.	10,278,626 B2	5/2019	Schurman et al.
9,898,049 B2	2/2018	Myers et al.	10,278,648 B2	5/2019	Al-Ali et al.
9,913,617 B2	3/2018	Al-Ali et al.	10,279,247 B2	5/2019	Kiani
9,918,646 B2	3/2018	Singh Alvarado et al.	10,292,628 B1	5/2019	Poeze et al.
9,924,893 B2	3/2018	Schurman et al.	10,292,657 B2	5/2019	Abdul-Hafiz et al.
9,924,897 B1	3/2018	Abdul-Hafiz	10,292,664 B2	5/2019	Al-Ali
9,936,917 B2	4/2018	Poeze et al.	10,299,708 B1	5/2019	Poeze et al.
9,943,269 B2	4/2018	Muhsin et al.	10,299,709 B2	5/2019	Perea et al.
9,949,676 B2	4/2018	Al-Ali	10,305,775 B2	5/2019	Lamego et al.
9,952,095 B1	4/2018	Hotelling et al.	10,307,111 B2	6/2019	Muhsin et al.
9,955,937 B2	5/2018	Telfort	10,325,681 B2	6/2019	Sampath et al.
9,965,946 B2	5/2018	Al-Ali	10,327,337 B2	6/2019	Triman et al.
9,980,667 B2	5/2018	Kiani et al.	2002/0042558 A1	4/2002	Mendelson
D820,865 S	6/2018	Muhsin et al.	2003/0036690 A1	2/2003	Geddes et al.
9,986,919 B2	6/2018	Lamego et al.	2004/0054290 A1	3/2004	Chance
9,986,952 B2	6/2018	Dalvi et al.	2004/0114783 A1 *	6/2004	Spycher G06K 9/00046
9,989,560 B2	6/2018	Poeze et al.			382/124
9,993,207 B2	6/2018	Al-Ali et al.	2005/0277819 A1	12/2005	Kiani et al.
10,007,758 B2	6/2018	Al-Ali et al.	2006/0161054 A1	7/2006	Reuss et al.
D822,215 S	7/2018	Al-Ali et al.	2007/0282478 A1	12/2007	Al-Ali et al.
D822,216 S	7/2018	Barker et al.	2008/0030468 A1	2/2008	Al-Ali et al.
10,010,276 B2	7/2018	Al-Ali et al.	2009/0247984 A1	10/2009	Lamego et al.
10,032,002 B2	7/2018	Kiani et al.	2009/0275813 A1	11/2009	Davis
10,039,080 B2	7/2018	Miller et al.	2009/0275844 A1	11/2009	Al-Ali
10,039,482 B2	8/2018	Al-Ali et al.	2010/0004518 A1	1/2010	Vo et al.
10,052,037 B2	8/2018	Kinast et al.	2010/0030040 A1	2/2010	Poeze et al.
10,055,121 B2	8/2018	Chaudhri et al.	2011/0004106 A1	1/2011	Iwamiya et al.
			2011/0082711 A1	4/2011	Poeze et al.
			2011/0085721 A1	4/2011	Guyon et al.
			2011/0105854 A1	5/2011	Kiani et al.
			2011/0125060 A1	5/2011	Telfort et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2011/0208015	A1	8/2011	Welch et al.	2014/0303520	A1	10/2014	Telfort et al.
2011/0213212	A1	9/2011	Al-Ali	2014/0316217	A1	10/2014	Purdon et al.
2011/0230733	A1	9/2011	Al-Ali	2014/0316218	A1	10/2014	Purdon et al.
2011/0237969	A1	9/2011	Eckerbom et al.	2014/0316228	A1	10/2014	Blank et al.
2011/0288383	A1	11/2011	Diab	2014/0323825	A1	10/2014	Al-Ali et al.
2011/0301444	A1	12/2011	Al-Ali	2014/0323897	A1	10/2014	Brown et al.
2012/0041316	A1	2/2012	Al-Ali et al.	2014/0323898	A1	10/2014	Purdon et al.
2012/0046557	A1	2/2012	Kiani	2014/0330092	A1	11/2014	Al-Ali et al.
2012/0059267	A1	3/2012	Lamego et al.	2014/0330098	A1	11/2014	Merritt et al.
2012/0088984	A1	4/2012	Al-Ali et al.	2014/0330099	A1	11/2014	Al-Ali et al.
2012/0165629	A1	6/2012	Merritt et al.	2014/0336481	A1	11/2014	Shakespeare et al.
2012/0179006	A1	7/2012	Jansen et al.	2014/0357966	A1	12/2014	Al-Ali et al.
2012/0209082	A1	8/2012	Al-Ali	2014/0371548	A1	12/2014	Al-Ali et al.
2012/0209084	A1	8/2012	Olsen et al.	2014/0371632	A1	12/2014	Al-Ali et al.
2012/0283524	A1	11/2012	Kiani et al.	2014/0378784	A1	12/2014	Kiani et al.
2012/0296178	A1	11/2012	Lamego et al.	2015/0005600	A1	1/2015	Blank et al.
2012/0319816	A1	12/2012	Al-Ali	2015/0011907	A1	1/2015	Purdon et al.
2012/0330112	A1	12/2012	Lamego et al.	2015/0012231	A1	1/2015	Poeze et al.
2013/0006076	A1	1/2013	McHale	2015/0018650	A1	1/2015	Al-Ali et al.
2013/0023775	A1	1/2013	Lamego et al.	2015/0025406	A1	1/2015	Al-Ali
2013/0041591	A1	2/2013	Lamego	2015/0032029	A1	1/2015	Al-Ali et al.
2013/0046204	A1	2/2013	Lamego et al.	2015/0038859	A1	2/2015	Dalvi et al.
2013/0060147	A1	3/2013	Welch et al.	2015/0045637	A1	2/2015	Dalvi
2013/0096405	A1	4/2013	Garfio	2015/0045685	A1	2/2015	Al-Ali et al.
2013/0096936	A1	4/2013	Sampath et al.	2015/0051462	A1	2/2015	Olsen
2013/0190581	A1	7/2013	Al-Ali et al.	2015/0080754	A1	3/2015	Purdon et al.
2013/0211214	A1	8/2013	Olsen	2015/0087936	A1	3/2015	Al-Ali et al.
2013/0243021	A1	9/2013	Siskavich	2015/0094546	A1	4/2015	Al-Ali
2013/0253334	A1	9/2013	Al-Ali et al.	2015/0097701	A1	4/2015	Al-Ali et al.
2013/0262730	A1	10/2013	Al-Ali et al.	2015/0099324	A1	4/2015	Wojtczuk et al.
2013/0267804	A1	10/2013	Al-Ali	2015/0099950	A1	4/2015	Al-Ali et al.
2013/0274572	A1	10/2013	Al-Ali et al.	2015/0099951	A1	4/2015	Al-Ali et al.
2013/0296672	A1	11/2013	O'Neil et al.	2015/0099955	A1	4/2015	Al-Ali et al.
2013/0296713	A1	11/2013	Al-Ali et al.	2015/0101844	A1	4/2015	Al-Ali et al.
2013/0317370	A1	11/2013	Dalvi et al.	2015/0106121	A1	4/2015	Muhsin et al.
2013/0324808	A1	12/2013	Al-Ali et al.	2015/0112151	A1	4/2015	Muhsin et al.
2013/0331660	A1	12/2013	Al-Ali et al.	2015/0116076	A1	4/2015	Al-Ali et al.
2013/0331670	A1	12/2013	Kiani	2015/0126830	A1	5/2015	Schurman et al.
2014/0012100	A1	1/2014	Al-Ali et al.	2015/0133755	A1	5/2015	Smith et al.
2014/0034353	A1	2/2014	Al-Ali et al.	2015/0140863	A1	5/2015	Al-Ali et al.
2014/0051953	A1	2/2014	Lamego et al.	2015/0141781	A1	5/2015	Weber et al.
2014/0066783	A1	3/2014	Kiani et al.	2015/0165312	A1	6/2015	Kiani
2014/0077956	A1	3/2014	Sampath et al.	2015/0173671	A1	6/2015	Paalasmaa et al.
2014/0081100	A1	3/2014	Muhsin et al.	2015/0196237	A1	7/2015	Lamego
2014/0081175	A1	3/2014	Telfort	2015/0201874	A1	7/2015	Diab
2014/0094667	A1	4/2014	Schurman et al.	2015/0208966	A1	7/2015	Al-Ali
2014/0100434	A1	4/2014	Diab et al.	2015/0216459	A1	8/2015	Al-Ali et al.
2014/0114199	A1	4/2014	Lamego et al.	2015/0230755	A1	8/2015	Al-Ali et al.
2014/0120564	A1	5/2014	Workman et al.	2015/0238722	A1	8/2015	Al-Ali
2014/0121482	A1	5/2014	Merritt et al.	2015/0245773	A1	9/2015	Lamego et al.
2014/0121483	A1	5/2014	Kiani	2015/0245793	A1	9/2015	Al-Ali et al.
2014/0127137	A1	5/2014	Bellott et al.	2015/0245794	A1	9/2015	Al-Ali
2014/0129702	A1	5/2014	Lamego et al.	2015/0255001	A1	9/2015	Haughav et al.
2014/0135588	A1	5/2014	Al-Ali et al.	2015/0257689	A1	9/2015	Al-Ali et al.
2014/0142401	A1	5/2014	Al-Ali et al.	2015/0272514	A1	10/2015	Kiani et al.
2014/0163344	A1	6/2014	Al-Ali	2015/0281424	A1	10/2015	Vock et al.
2014/0163402	A1	6/2014	Lamego et al.	2015/0318100	A1	11/2015	Rothkopf et al.
2014/0166076	A1	6/2014	Kiani et al.	2015/0351697	A1	12/2015	Weber et al.
2014/0171146	A1	6/2014	Ma et al.	2015/0351704	A1	12/2015	Kiani et al.
2014/0171763	A1	6/2014	Diab	2015/0359429	A1	12/2015	Al-Ali et al.
2014/0180038	A1	6/2014	Kiani	2015/0366472	A1	12/2015	Kiani
2014/0180154	A1	6/2014	Sierra et al.	2015/0366507	A1	12/2015	Blank
2014/0180160	A1	6/2014	Brown et al.	2015/0374298	A1	12/2015	Al-Ali et al.
2014/0187973	A1	7/2014	Brown et al.	2015/0380875	A1	12/2015	Coverston et al.
2014/0194766	A1	7/2014	Al-Ali et al.	2016/0000362	A1	1/2016	Diab et al.
2014/0206963	A1	7/2014	Al-Ali	2016/0007930	A1	1/2016	Weber et al.
2014/0213864	A1	7/2014	Abdul-Hafiz et al.	2016/0019360	A1	1/2016	Pahwa et al.
2014/0266790	A1	9/2014	Al-Ali et al.	2016/0023245	A1	1/2016	Zadesky et al.
2014/0275808	A1	9/2014	Poeze et al.	2016/0029932	A1	2/2016	Al-Ali
2014/0275835	A1	9/2014	Lamego et al.	2016/0029933	A1	2/2016	Al-Ali et al.
2014/0275871	A1	9/2014	Lamego et al.	2016/0038045	A1	2/2016	Shapiro
2014/0275872	A1	9/2014	Merritt et al.	2016/0045118	A1	2/2016	Kiani
2014/0275881	A1	9/2014	Lamego et al.	2016/0051157	A1	2/2016	Waydo
2014/0276115	A1	9/2014	Dalvi et al.	2016/0051158	A1	2/2016	Silva
2014/0288400	A1	9/2014	Diab et al.	2016/0051205	A1	2/2016	Al-Ali et al.
				2016/0058302	A1	3/2016	Raghuram et al.
				2016/0058309	A1	3/2016	Han
				2016/0058312	A1	3/2016	Han et al.
				2016/0058338	A1	3/2016	Schurman et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2016/0058347 A1	3/2016	Reichgott et al.	2017/0196470 A1	7/2017	Lamego et al.
2016/0058356 A1	3/2016	Raghuram et al.	2017/0224262 A1	8/2017	Al-Ali
2016/0058370 A1	3/2016	Raghuram et al.	2017/0228516 A1	8/2017	Sampath et al.
2016/0066823 A1	3/2016	Kind et al.	2017/0245790 A1	8/2017	Al-Ali et al.
2016/0066824 A1	3/2016	Al-Ali et al.	2017/0248446 A1	8/2017	Gowreesunker et al.
2016/0066879 A1	3/2016	Telfort et al.	2017/0251974 A1	9/2017	Shreim et al.
2016/0071392 A1	3/2016	Hankey et al.	2017/0251975 A1	9/2017	Shreim et al.
2016/0072429 A1	3/2016	Kiani et al.	2017/0258403 A1	9/2017	Abdul-Hafiz et al.
2016/0073967 A1	3/2016	Lamego et al.	2017/0273619 A1	9/2017	Alvarado et al.
2016/0081552 A1	3/2016	Wojtczuk et al.	2017/0281024 A1	10/2017	Narasimhan et al.
2016/0095543 A1	4/2016	Telfort et al.	2017/0293727 A1	10/2017	Klaassen et al.
2016/0095548 A1	4/2016	Al-Ali et al.	2017/0311851 A1	11/2017	Schurman et al.
2016/0103598 A1	4/2016	Al-Ali et al.	2017/0311891 A1	11/2017	Kiani et al.
2016/0113527 A1	4/2016	Al-Ali et al.	2017/0325698 A1	11/2017	Allec et al.
2016/0143548 A1	5/2016	Al-Ali	2017/0325728 A1	11/2017	Al-Ali et al.
2016/0154950 A1	6/2016	Nakajima et al.	2017/0325744 A1	11/2017	Allec et al.
2016/0157780 A1	6/2016	Rimminen et al.	2017/0332976 A1	11/2017	Al-Ali et al.
2016/0166182 A1	6/2016	Al-Ali et al.	2017/0340209 A1	11/2017	Klaassen et al.
2016/0166183 A1	6/2016	Poeze et al.	2017/0340219 A1	11/2017	Sullivan et al.
2016/0196388 A1	7/2016	Lamego	2017/0340293 A1	11/2017	Al-Ali et al.
2016/0197436 A1	7/2016	Barker et al.	2017/0347885 A1	12/2017	Tan et al.
2016/0213281 A1	7/2016	Eckerbom et al.	2017/0354332 A1	12/2017	Lamego
2016/0213309 A1	7/2016	Sannholm et al.	2017/0354795 A1	12/2017	Blahnik et al.
2016/0228043 A1	8/2016	O'Neil et al.	2017/0358239 A1	12/2017	Arney et al.
2016/0233632 A1	8/2016	Scruggs et al.	2017/0358240 A1	12/2017	Blahnik et al.
2016/0234944 A1	8/2016	Schmidt et al.	2017/0358242 A1	12/2017	Thompson et al.
2016/0256058 A1	9/2016	Pham et al.	2017/0360306 A1	12/2017	Narasimhan et al.
2016/0256082 A1	9/2016	Ely et al.	2017/0360310 A1	12/2017	Kiani et al.
2016/0267238 A1	9/2016	Nag	2017/0366657 A1	12/2017	Thompson et al.
2016/0270735 A1	9/2016	Diab et al.	2017/0367632 A1	12/2017	Al-Ali et al.
2016/0283665 A1	9/2016	Sampath et al.	2018/0008146 A1	1/2018	Al-Ali et al.
2016/0287090 A1	10/2016	Al-Ali et al.	2018/0013562 A1	1/2018	Haider et al.
2016/0287181 A1	10/2016	Han et al.	2018/0014752 A1	1/2018	Al-Ali et al.
2016/0287786 A1	10/2016	Kiani	2018/0014781 A1	1/2018	Clavelle et al.
2016/0296169 A1	10/2016	McHale et al.	2018/0025287 A1	1/2018	Mathew et al.
2016/0296173 A1	10/2016	Culbert	2018/0056129 A1	1/2018	Narasimha Rao et al.
2016/0296174 A1	10/2016	Isikman et al.	2018/0028124 A1	2/2018	Al-Ali et al.
2016/0310027 A1	10/2016	Han	2018/0042556 A1	2/2018	Shahparnia et al.
2016/0310052 A1	10/2016	Al-Ali et al.	2018/0049694 A1	2/2018	Singh Alvarado et al.
2016/0314260 A1	10/2016	Kiani	2018/0050235 A1	2/2018	Tan et al.
2016/0324488 A1	11/2016	Olsen	2018/0055375 A1	3/2018	Martinez et al.
2016/0327984 A1	11/2016	Al-Ali et al.	2018/0055385 A1	3/2018	Al-Ali
2016/0331332 A1	11/2016	Al-Ali	2018/0055390 A1	3/2018	Kiani et al.
2016/0367173 A1	12/2016	Dalvi et al.	2018/0055430 A1	3/2018	Diab et al.
2016/0378069 A1	12/2016	Rothkopf	2018/0055439 A1	3/2018	Pham et al.
2016/0378071 A1	12/2016	Rothkopf	2018/0064381 A1	3/2018	Shakespeare et al.
2017/0000394 A1	1/2017	Al-Ali et al.	2018/0069776 A1	3/2018	Lamego et al.
2017/0007134 A1	1/2017	Al-Ali et al.	2018/0070867 A1	3/2018	Smith et al.
2017/0007183 A1	1/2017	Dusan et al.	2018/0078151 A1	3/2018	Allec et al.
2017/0007198 A1	1/2017	Al-Ali et al.	2018/0078182 A1	3/2018	Chen et al.
2017/0010858 A1	1/2017	Prest et al.	2018/0082767 A1	3/2018	Al-Ali et al.
2017/0014083 A1	1/2017	Diab et al.	2018/0085068 A1	3/2018	Telfort
2017/0014084 A1	1/2017	Al-Ali et al.	2018/0087937 A1	3/2018	Al-Ali et al.
2017/0024748 A1	1/2017	Haider	2018/0103874 A1	4/2018	Lee et al.
2017/0042488 A1	2/2017	Muhsin	2018/0103905 A1	4/2018	Kiani
2017/0055851 A1	3/2017	Al-Ali	2018/0110469 A1	4/2018	Maani et al.
2017/0055882 A1	3/2017	Al-Ali et al.	2018/0110478 A1	4/2018	Al-Ali
2017/0055887 A1	3/2017	Al-Ali	2018/0116575 A1	5/2018	Perea et al.
2017/0055896 A1	3/2017	Al-Ali et al.	2018/0125368 A1	5/2018	Lamego et al.
2017/0074897 A1	3/2017	Mermel et al.	2018/0125430 A1	5/2018	Al-Ali et al.
2017/0079594 A1	3/2017	Telfort et al.	2018/0125445 A1	5/2018	Telfort et al.
2017/0084133 A1	3/2017	Cardinali et al.	2018/0130325 A1	5/2018	Kiani et al.
2017/0086689 A1	3/2017	Shui et al.	2018/0132769 A1	5/2018	Weber et al.
2017/0086723 A1	3/2017	Al-Ali et al.	2018/0132770 A1	5/2018	Lamego
2017/0086742 A1	3/2017	Harrison-Noonan et al.	2018/0146901 A1	5/2018	Al-Ali et al.
2017/0086743 A1	3/2017	Bushnell et al.	2018/0146902 A1	5/2018	Kiani et al.
2017/0094450 A1	3/2017	Tu et al.	2018/0153418 A1	6/2018	Sullivan et al.
2017/0143281 A1	5/2017	Olsen	2018/0153442 A1	6/2018	Eckerbom et al.
2017/0147774 A1	5/2017	Kiani	2018/0153446 A1	6/2018	Kiani
2017/0156620 A1	6/2017	Al-Ali et al.	2018/0153447 A1	6/2018	Al-Ali et al.
2017/0164884 A1	6/2017	Culbert et al.	2018/0153448 A1	6/2018	Weber et al.
2017/0173632 A1	6/2017	Al-Ali	2018/0161499 A1	6/2018	Al-Ali et al.
2017/0187146 A1	6/2017	Kiani et al.	2018/0164853 A1	6/2018	Myers et al.
2017/0188919 A1	7/2017	Al-Ali et al.	2018/0168491 A1	6/2018	Al-Ali et al.
2017/0196464 A1	7/2017	Jansen et al.	2018/0174679 A1	6/2018	Sampath et al.
			2018/0174680 A1	6/2018	Sampath et al.
			2018/0182484 A1	6/2018	Sampath et al.
			2018/0184917 A1	7/2018	Kiani
			2018/0192924 A1	7/2018	Al-Ali

(56)

References Cited

U.S. PATENT DOCUMENTS

2018/0192953 A1 7/2018 Shreim et al.
 2018/0192955 A1 7/2018 Al-Ali et al.
 2018/0196514 A1 7/2018 Allec et al.
 2018/0199871 A1 7/2018 Pauley et al.
 2018/0206795 A1 7/2018 Al-Ali
 2018/0206815 A1 7/2018 Telfort
 2018/0213583 A1 7/2018 Al-Ali
 2018/0214031 A1 8/2018 Kiani et al.
 2018/0214090 A1 8/2018 Al-Ali et al.
 2018/0218792 A1 8/2018 Muhsin et al.
 2018/0225960 A1 8/2018 Al-Ali et al.
 2018/0228414 A1 8/2018 Shao et al.
 2018/0238718 A1 8/2018 Dalvi
 2018/0238734 A1 8/2018 Hotelling et al.
 2018/0242853 A1 8/2018 Al-Ali
 2018/0242921 A1 8/2018 Muhsin et al.
 2018/0242923 A1 8/2018 Al-Ali et al.
 2018/0242924 A1 8/2018 Barker et al.
 2018/0242926 A1 8/2018 Muhsin et al.
 2018/0247353 A1 8/2018 Al-Ali et al.
 2018/0247712 A1 8/2018 Muhsin et al.
 2018/0249933 A1 9/2018 Schurman et al.
 2018/0253947 A1 9/2018 Muhsin et al.
 2018/0256087 A1 9/2018 Al-Ali et al.
 2018/0256113 A1 9/2018 Weber et al.
 2018/0279956 A1 10/2018 Waydo et al.
 2018/0285094 A1 10/2018 Housel et al.
 2018/0289325 A1 10/2018 Poeze et al.
 2018/0289337 A1 10/2018 Al-Ali et al.
 2018/0296161 A1 10/2018 Shreim et al.
 2018/0300919 A1 10/2018 Muhsin et al.
 2018/0310822 A1 11/2018 Indorf et al.
 2018/0310823 A1 11/2018 Al-Ali et al.
 2018/0317826 A1 11/2018 Muhsin
 2018/0317841 A1 11/2018 Novak, Jr.
 2018/0333055 A1 11/2018 Lamago et al.
 2018/0333087 A1 11/2018 Al-Ali
 2019/0000317 A1 1/2019 Muhsin et al.

2019/0000362 A1 1/2019 Kiani et al.
 2019/0015023 A1 1/2019 Monfre
 2019/0021638 A1 1/2019 Al-Ali et al.
 2019/0029574 A1 1/2019 Schurman et al.
 2019/0029578 A1 1/2019 Al-Ali et al.
 2019/0038143 A1 2/2019 Al-Ali
 2019/0058280 A1 2/2019 Al-Ali et al.
 2019/0058281 A1 2/2019 Al-Ali et al.
 2019/0069813 A1 3/2019 Al-Ali
 2019/0069814 A1 3/2019 Al-Ali
 2019/0076028 A1 3/2019 Al-Ali et al.
 2019/0082979 A1 3/2019 Al-Ali et al.
 2019/0090748 A1 3/2019 Al-Ali
 2019/0090760 A1 3/2019 Kinast et al.
 2019/0090764 A1 3/2019 Al-Ali
 2019/0104973 A1 4/2019 Poeze et al.
 2019/0110719 A1 4/2019 Poeze et al.
 2019/0117070 A1 4/2019 Muhsin et al.
 2019/0117139 A1 4/2019 Al-Ali et al.
 2019/0117140 A1 4/2019 Al-Ali et al.
 2019/0117141 A1 4/2019 Al-Ali
 2019/0117930 A1 4/2019 Al-Ali
 2019/0122763 A1 4/2019 Sampath et al.
 2019/0133525 A1 5/2019 Al-Ali et al.
 2019/0142283 A1 5/2019 Lamago et al.
 2019/0142344 A1 5/2019 Telfort et al.
 2019/0150800 A1 5/2019 Poeze et al.
 2019/0150856 A1 5/2019 Kiani et al.
 2019/0167161 A1 6/2019 Al-Ali et al.
 2019/0175019 A1 6/2019 Al-Ali et al.
 2019/0192076 A1 6/2019 McHale et al.

OTHER PUBLICATIONS

Written Opinion received in International Application No. PCT/US2016/040190, dated Jan. 2, 2018.

Konig, V. et al., "Reflectance Pulse Oximetry—Principles and Obstetric Application in the Zurich System," J Clin Monit 1998; 14: 403-412.

* cited by examiner

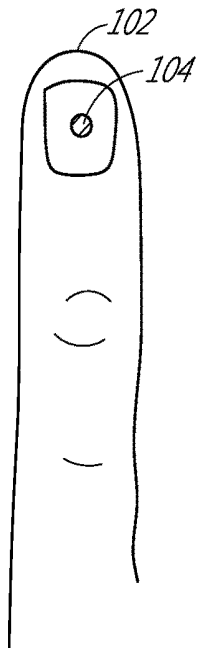


FIG. 1
(PRIOR ART)

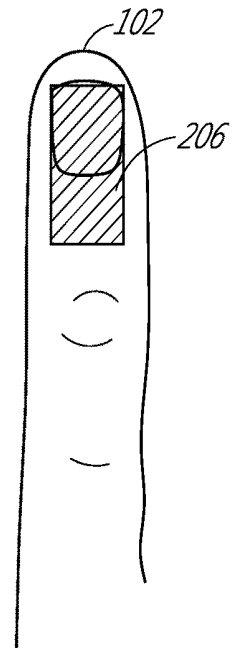


FIG. 2

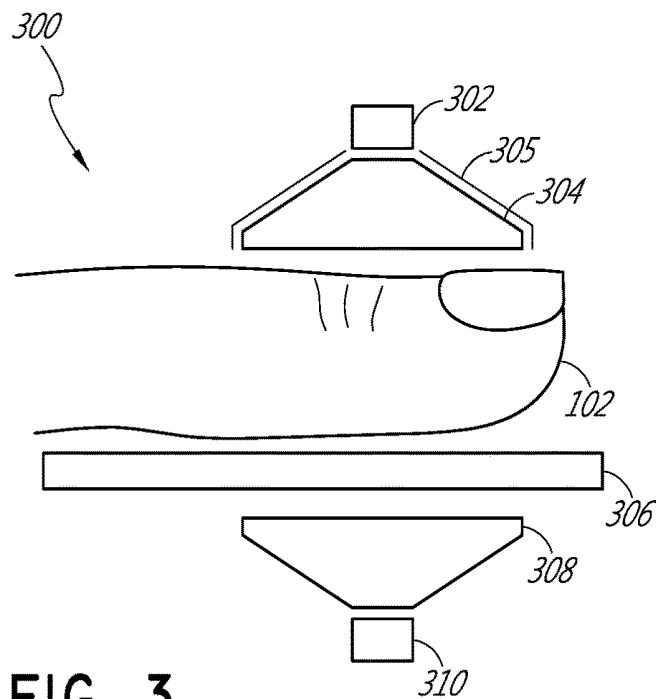


FIG. 3

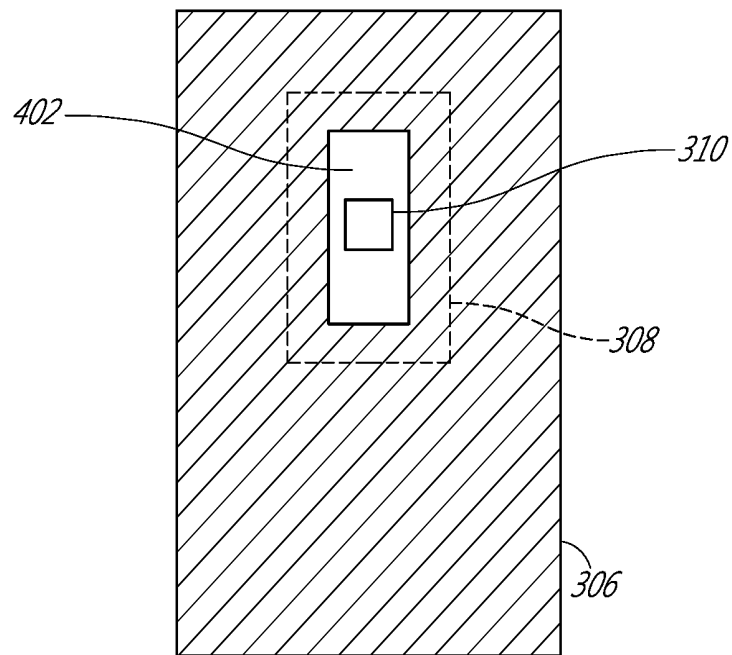


FIG. 4A

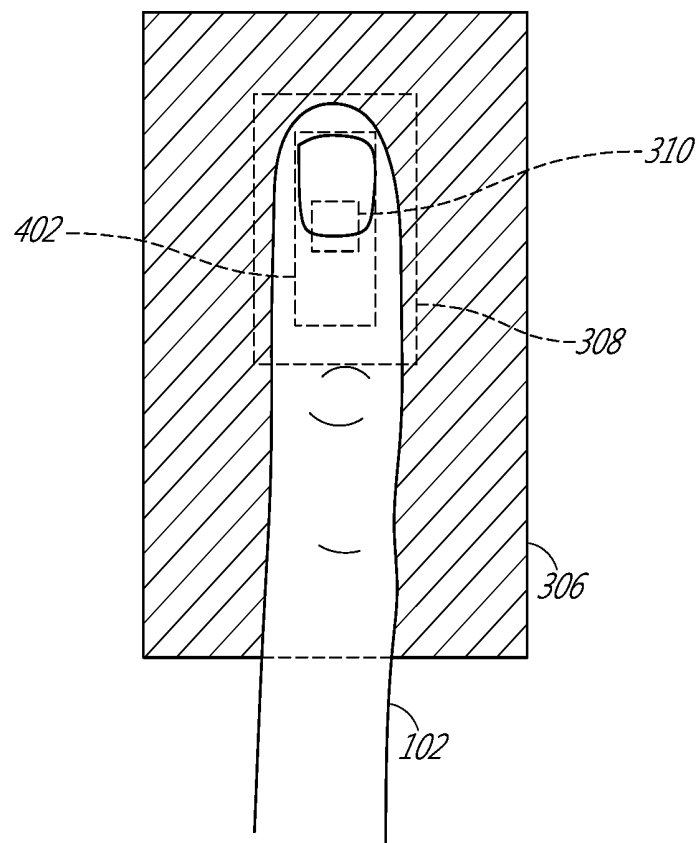


FIG. 4B

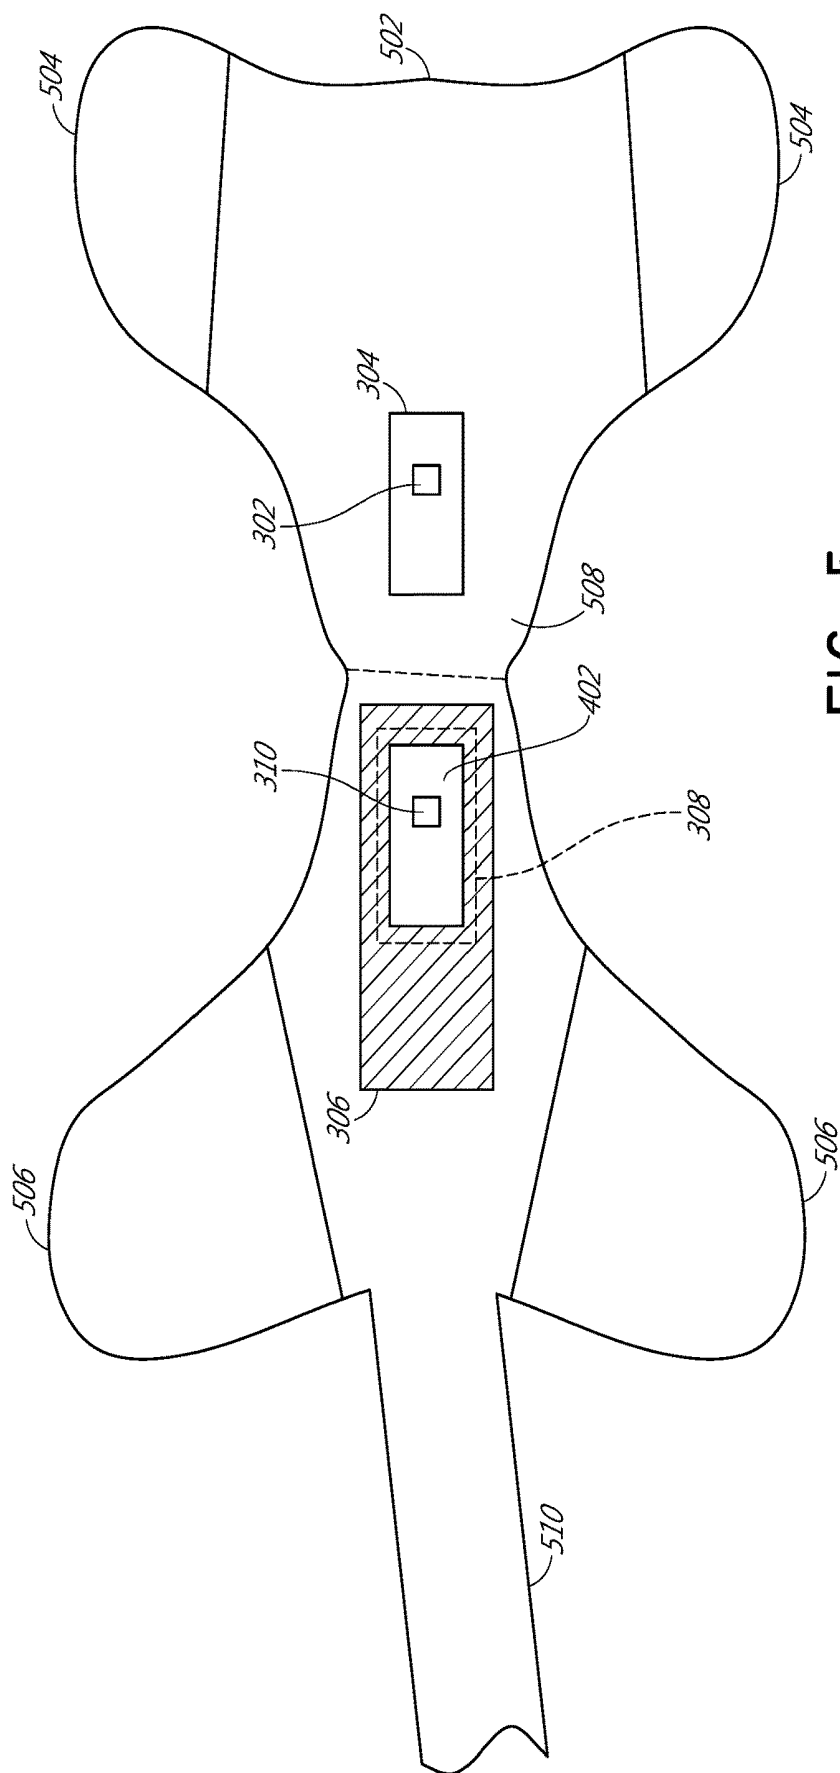


FIG. 5

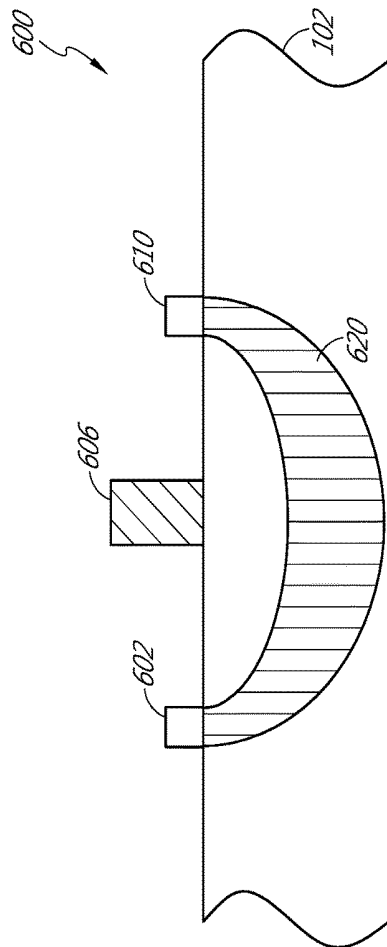


FIG. 6
(PRIOR ART)

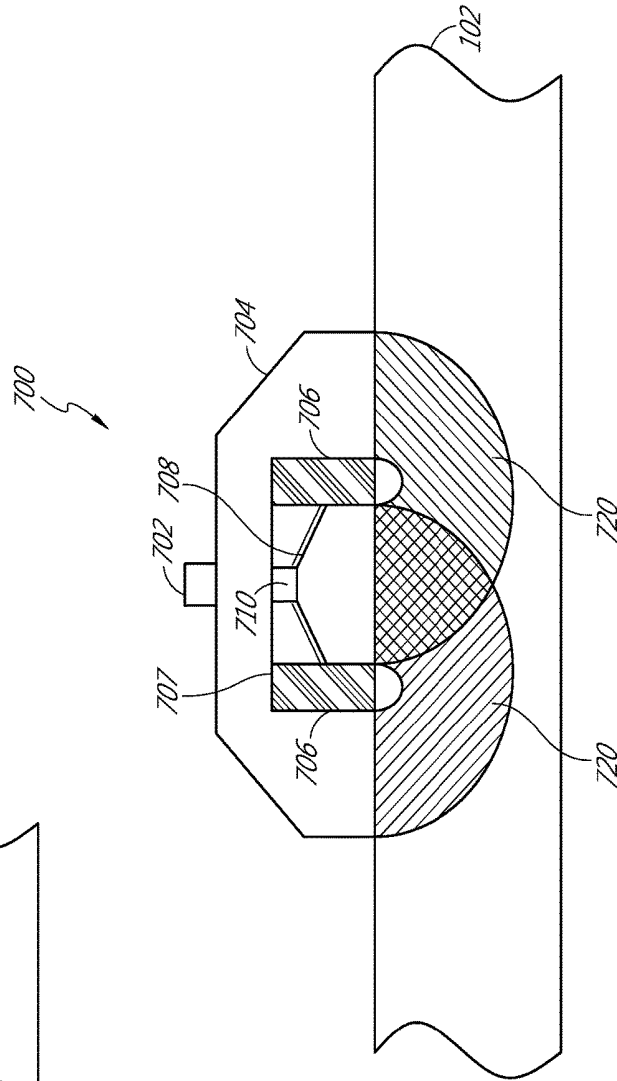


FIG. 7A

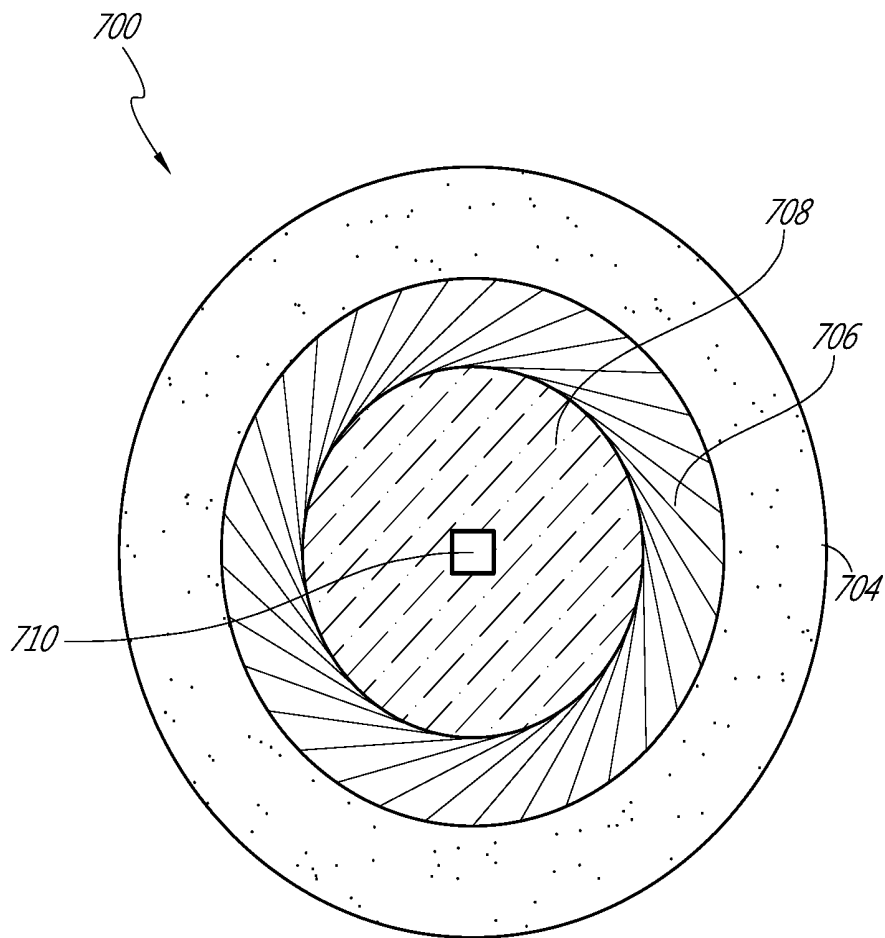


FIG. 7B

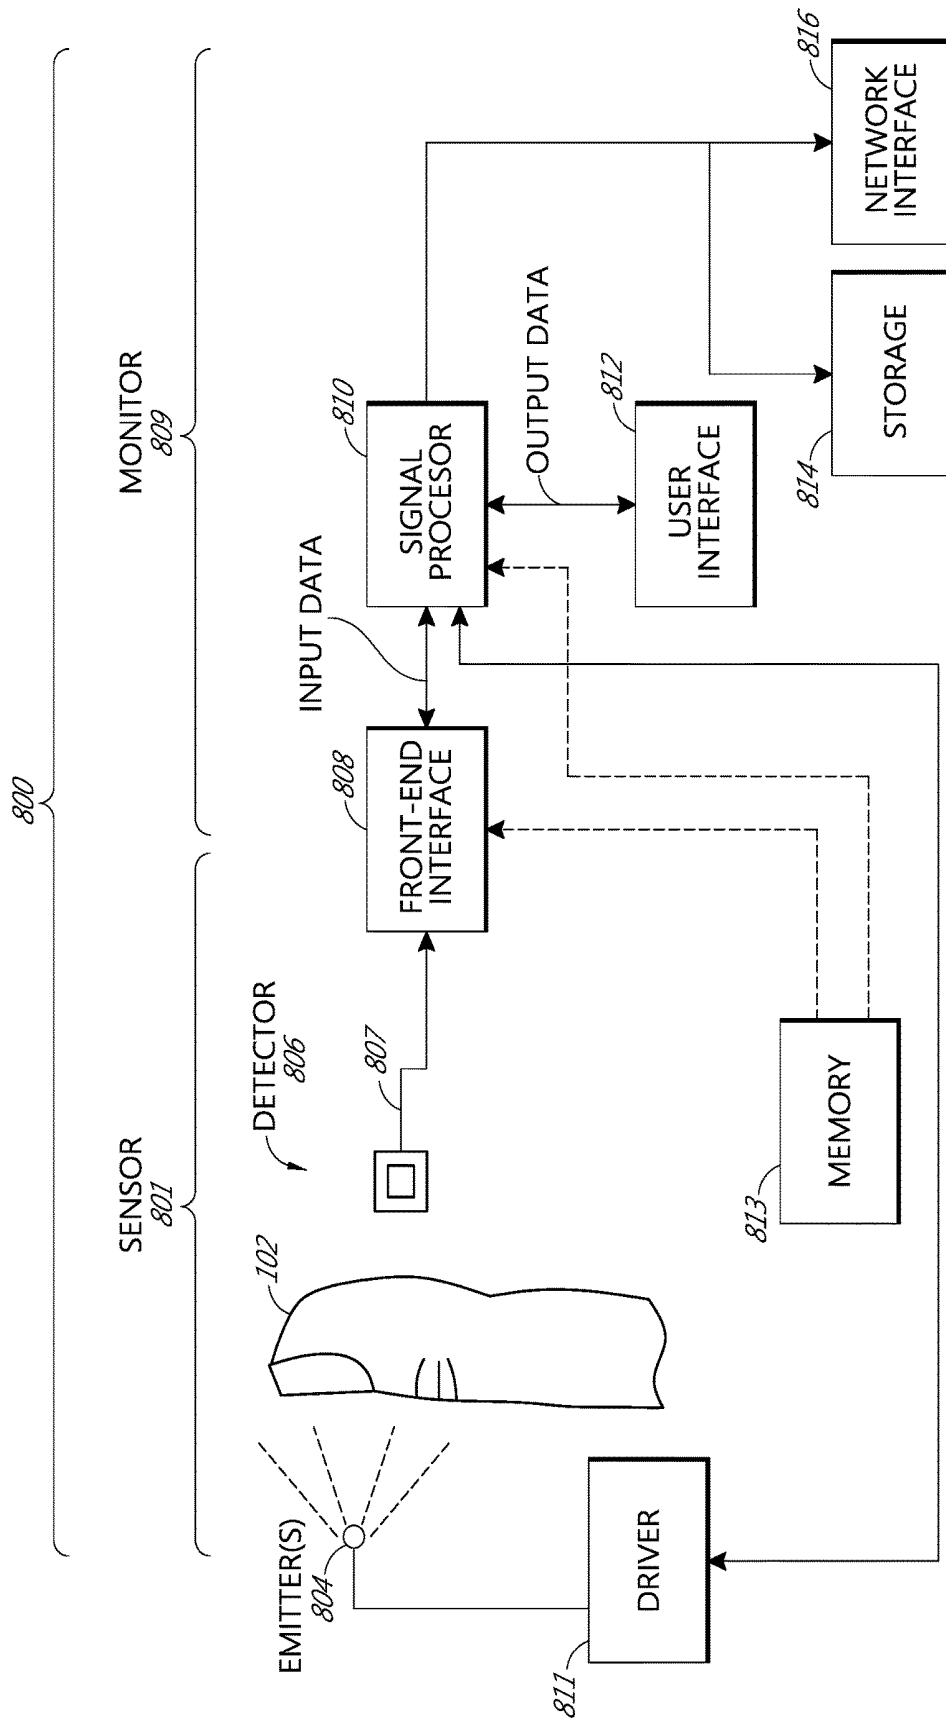


FIG. 8

1

ADVANCED PULSE OXIMETRY SENSOR**INCORPORATION BY REFERENCE TO ANY
PRIORITY APPLICATIONS**

This present application claims priority benefit under 35 U.S.C. § 119(e) from U.S. Provisional Application No. 62/188,430, filed Jul. 2, 2015, entitled “Advanced Pulse Oximetry Sensor,” which is incorporated by reference herein. Any and all applications for which a foreign or domestic priority claim is identified in the Application Data Sheet as filed with the present application are hereby incorporated by reference under 37 CFR 1.57.

FIELD OF THE DISCLOSURE

The present disclosure relates to the field of non-invasive optical-based physiological monitoring sensors, and more particularly to systems, devices and methods for improving the non-invasive measurement accuracy of oxygen saturation, among other physiological parameters.

BACKGROUND

Spectroscopy is a common technique for measuring the concentration of organic and some inorganic constituents of a solution. The theoretical basis of this technique is the Beer-Lambert law, which states that the concentration c_i of an absorbent in solution can be determined by the intensity of light transmitted through the solution, knowing the path-length d_{80} , the intensity of the incident light $I_{0,\lambda}$, and the extinction coefficient $\epsilon_{i,\lambda}$ at a particular wavelength λ .

In generalized form, the Beer-Lambert law is expressed as:

$$I_{\lambda} = I_{0,\lambda} e^{-d_{\lambda} \cdot \mu_{a,\lambda}} \quad (1)$$

$$\mu_{a,\lambda} = \sum_{i=1}^n \epsilon_{i,\lambda} \cdot c_i \quad (2)$$

where $\Xi_{a,\lambda}$ is the bulk absorption coefficient and represents the probability of absorption per unit length. The minimum number of discrete wavelengths that are required to solve equations 1 and 2 is the number of significant absorbers that are present in the solution.

A practical application of this technique is pulse oximetry, which utilizes a noninvasive sensor to measure oxygen saturation and pulse rate, among other physiological parameters. Pulse oximetry relies on a sensor attached externally to the patient to output signals indicative of various physiological parameters, such as a patient's blood constituents and/or analytes, including for example a percent value for arterial oxygen saturation, among other physiological parameters. The sensor has an emitter that transmits optical radiation of one or more wavelengths into a tissue site and a detector that responds to the intensity of the optical radiation after absorption by pulsatile arterial blood flowing within the tissue site. Based upon this response, a processor determines the relative concentrations of oxygenated hemoglobin (HbO₂) and deoxygenated hemoglobin (Hb) in the blood so as to derive oxygen saturation, which can provide early detection of potentially hazardous decreases in a patient's oxygen supply.

A pulse oximetry system generally includes a patient monitor, a communications medium such as a cable, and/or

2

a physiological sensor having one or more light emitters and a detector, such as one or more light-emitting diodes (LEDs) and a photodetector. The sensor is attached to a tissue site, such as a finger, toe, earlobe, nose, hand, foot, or other site having pulsatile blood flow which can be penetrated by light from the one or more emitters. The detector is responsive to the emitted light after attenuation or reflection by pulsatile blood flowing in the tissue site. The detector outputs a detector signal to the monitor over the communication medium. The monitor processes the signal to provide a numerical readout of physiological parameters such as oxygen saturation (SpO₂) and/or pulse rate. A pulse oximetry sensor is described in U.S. Pat. No. 6,088,607 entitled Low Noise Optical Probe; pulse oximetry signal processing is described in U.S. Pat. Nos. 6,650,917 and 6,699,194 entitled Signal Processing Apparatus and Signal Processing Apparatus and Method, respectively; a pulse oximeter monitor is described in U.S. Pat. No. 6,584,336 entitled Universal/Upgrading Pulse Oximeter; all of which are assigned to Masimo Corporation, Irvine, Calif., and each is incorporated by reference herein in its entirety.

There are many sources of measurement error introduced to pulse oximetry systems. Some such sources of error include the pulse oximetry system's electronic components, including emitters and detectors, as well as chemical and structural physiological differences between patients. Another source of measurement error is the effect of multiple scattering of photons as the photons pass through the patient's tissue (arterial blood) and arrive at the sensor's light detector.

SUMMARY

This disclosure describes embodiments of non-invasive methods, devices, and systems for measuring blood constituents, analytes, and/or substances such as, by way of non-limiting example, oxygen, carboxyhemoglobin, methemoglobin, total hemoglobin, glucose, proteins, lipids, a percentage thereof (e.g., saturation), pulse rate, perfusion index, oxygen content, total hemoglobin, Oxygen Reserve Index™ (ORI™) or for measuring many other physiologically relevant patient characteristics. These characteristics can relate to, for example, pulse rate, hydration, trending information and analysis, and the like.

In an embodiment, an optical physiological measurement system includes an emitter configured to emit light of one or more wavelengths. The system also includes a diffuser configured to receive the emitted light, to spread the received light, and to emit the spread light over a larger tissue area than would otherwise be penetrated by the emitter directly emitting light at a tissue measurement site. The tissue measurement site can include, such as, for example, a finger, a wrist, or the like. The system further includes a concentrator configured to receive the spread light after it has been attenuated by or reflected from the tissue measurement site. The concentrator is also configured to collect and concentrate the received light and to emit the concentrated light to a detector. The detector is configured to detect the concentrated light and to transmit a signal indicative of the detected light. The system also includes a processor configured to receive the transmitted signal indicative of the detected light and to determine, based on an amount of absorption, an analyte of interest, such as, for example, arterial oxygen saturation or other parameter, in the tissue measurement site.

In certain embodiments of the present disclosure, the diffuser comprises glass, ground glass, glass beads, opal

glass, or a microlens-based, band-limited, engineered diffuser that can deliver efficient and uniform illumination. In some embodiments the diffuser is further configured to define a surface area shape by which the emitted spread light is distributed onto a surface of the tissue measurement site. The defined surface area shape can include, by way of non-limiting example, a shape that is substantially rectangular, square, circular, oval, or annular, among others.

According to some embodiments, the optical physiological measurement system includes an optical filter having a light-absorbing surface that faces the tissue measurement site. The optical filter also has an opening that is configured to allow the spread light, after being attenuated by the tissue measurement site, to be received by the concentrator. In an embodiment, the opening has dimensions, wherein the dimensions of the opening are similar to the defined surface area shape by which the emitted spread light is distributed onto the surface of the tissue measurement site. In an embodiment, the opening has dimensions that are larger than the defined surface area shape by which the emitted spread light is distributed onto the surface of the tissue measurement site. In other embodiments, the dimensions of the opening in the optical filter are not the same as the diffuser opening, but the dimensions are larger than the detector package.

In other embodiments of the present disclosure, the concentrator comprises glass, ground glass, glass beads, opal glass, or a compound parabolic concentrator. In some embodiments the concentrator comprises a cylindrical structure having a truncated circular conical structure on top. The truncated section is adjacent the detector. The light concentrator is structured to receive the emitted optical radiation, after reflection by the tissue measurement site, and to direct the reflected light to the detector.

In accordance with certain embodiments of the present disclosure, the processor is configured to determine an average level of the light detected by the detector. The average level of light is used to determine a physiological parameter in the tissue measurement site.

According to another embodiment, a method to determine a constituent or analyte in a patient's blood is disclosed. The method includes emitting, from an emitter, light of at least one wavelength; spreading, with a diffuser, the emitted light and emitting the spread light from the diffuser to a tissue measurement site; receiving, by a concentrator, the spread light after the spread light has been attenuated by the tissue measurement site; concentrating, by the concentrator, the received light and emitting the concentrated light from the concentrator to a detector; detecting, with the detector, the emitted concentrated light; transmitting, from the detector, a signal responsive to the detected light; receiving, by a processor, the transmitted signal responsive to the detected light; and processing, by the processor, the received signal responsive to the detected light to determine a physiological parameter.

In some embodiments, the method to determine a constituent or analyte in a patient's blood includes filtering, with a light-absorbing detector filter, scattered portions of the emitted spread light. According to an embodiment, the light-absorbing detector filter is substantially rectangular in shape and has outer dimensions in the range of approximately 1-5 cm in width and approximately 2-8 cm in length, and has an opening through which emitted light may pass, the opening having dimensions in the range of approximately 0.25-3 cm in width and approximately 1-7 cm in length. In another embodiment, the light-absorbing detector filter is substantially square in shape and has outer dimen-

sions in the range of approximately 0.25-10 cm², and has an opening through which emitted light may pass, the opening having dimensions in the range of approximately 0.1-8 cm². In yet another embodiment, the light-absorbing detector filter is substantially rectangular in shape and has outer dimensions of approximately 3 cm in width and approximately 6 cm in length, and has an opening through which emitted light may pass, the opening having dimensions of approximately 1.5 cm in width and approximately 4 cm in length.

In still other embodiments of the method to determine a constituent or analyte in a patient's blood, spreading, with a diffuser, the emitted light and emitting the spread light from the diffuser to a tissue measurement site is performed by at least one of a glass diffuser, a ground glass diffuser, a glass bead diffuser, an opal glass diffuser, and an engineered diffuser. In some embodiments the emitted spread light is emitted with a substantially uniform intensity profile. And in some embodiments, emitting the spread light from the diffuser to the tissue measurement site includes spreading the emitted light so as to define a surface area shape by which the emitted spread light is distributed onto a surface of the tissue measurement site.

According to yet another embodiment, a pulse oximeter is disclosed. The pulse oximeter includes an emitter configured to emit light at one or more wavelengths. The pulse oximeter also includes a diffuser configured to receive the emitted light, to spread the received light, and to emit the spread light directed at a tissue measurement sight. The pulse oximeter also includes a detector configured to detect the emitted spread light after being attenuated by or reflected from the tissue measurement site and to transmit a signal indicative of the detected light. The pulse oximeter also includes a processor configured to receive the transmitted signal and to process the received signal to determine an average absorbance of a blood constituent or analyte in the tissue measurement site over a larger measurement site area than can be performed with a point light source or point detector. In some embodiments, the diffuser is further configured to define a surface area shape by which the emitted spread light is distributed onto a surface of the tissue measurement site, and the detector is further configured to have a detection area corresponding to the defined surface area shape by which the emitted spread light is distributed onto the surface of the tissue measurement site. According to some embodiments, the detector comprises an array of detectors configured to cover the detection area. In still other embodiments, the processor is further configured to determine an average of the detected light.

For purposes of summarizing, certain aspects, advantages and novel features of the disclosure have been described herein. It is to be understood that not necessarily all such advantages can be achieved in accordance with any particular embodiment of the systems, devices and/or methods disclosed herein. Thus, the subject matter of the disclosure herein can be embodied or carried out in a manner that achieves or optimizes one advantage or group of advantages as taught herein without necessarily achieving other advantages as can be taught or suggested herein.

BRIEF DESCRIPTION OF THE DRAWINGS

Throughout the drawings, reference numbers can be used to indicate correspondence between referenced elements. The drawings are provided to illustrate embodiments of the disclosure described herein and not to limit the scope thereof.

FIG. 1 illustrates a conventional approach to two-dimensional pulse oximetry in which the emitter is configured to emit optical radiation as a point optical source.

FIG. 2 illustrates the disclosed three-dimensional approach to pulse oximetry in which the emitted light irradiates a substantially larger volume of tissue as compared to the point source approach described with respect to FIG. 1.

FIG. 3 illustrates schematically a side view of a three-dimensional pulse oximetry sensor according to an embodiment of the present disclosure.

FIG. 4A is a top view of a portion of a three-dimensional pulse oximetry sensor according to an embodiment of the present disclosure.

FIG. 4B illustrates the top view of a portion of the three-dimensional pulse oximetry sensor shown in FIG. 4A, with the addition of a tissue measurement site in operational position.

FIG. 5 illustrates a top view of a three-dimensional pulse oximetry sensor according to an embodiment of the present disclosure.

FIG. 6 illustrates a conventional two-dimensional approach to reflective pulse oximetry in which the emitter is configured to emit optical radiation as a point optical source.

FIG. 7A is a simplified schematic side view illustration of a reflective three-dimensional pulse oximetry sensor according to an embodiment of the present disclosure.

FIG. 7B is a simplified schematic top view illustration of the three-dimensional reflective pulse oximetry sensor of FIG. 7A.

FIG. 8 illustrates a block diagram of an example pulse oximetry system capable of noninvasively measuring one or more blood analytes in a monitored patient, according to an embodiment of the disclosure.

DETAILED DESCRIPTION

FIG. 1 illustrates schematically a conventional pulse oximetry sensor having a two-dimensional (2D) approach to pulse oximetry. As illustrated, the emitter 104 is configured to emit optical radiation as a point optical source, i.e., an optical radiation source that has negligible dimensions such that it may be considered as a point. This approach is referred to herein as “two-dimensional” pulse oximetry because it applies a two-dimensional analytical model to the three-dimensional space of the tissue measurement site 102 of the patient. Point optical sources feature a defined, freely selectable, and homogeneous light beam area. Light beams emitted from LED point sources often exhibit a strong focus which can produce a usually sharply-defined and evenly-lit illuminated spot often with high intensity dynamics. Illustratively, when looking at the surface of the tissue measurement site 102 (or “sample tissue”), which in this example is a finger, a small point-like surface area of tissue 204 is irradiated by a point optical source. In some embodiments, the irradiated circular area of the point optical source is in the range between 8 and 150 microns. Illustratively, the emitted point optical source of light enters the tissue measurement site 102 as a point of light. As the light penetrates the depth of the tissue 102, it does so as a line or vector, representing a two-dimensional construct within a three-dimensional structure, namely the patient's tissue 102.

Use of a point optical source is believed to reduce variability in light pathlength which would lead to more accurate oximetry measurements. However, in practice, photons do not travel in straight paths. Instead, the light particles scatter, bouncing around between various irregular

objects (such as, for example, red blood cells) in the patient's blood. Accordingly, photon pathlengths vary depending on, among other things, their particular journeys through and around the tissue at the measurement site 102. This phenomenon is referred to as “multiple scattering.” In a study, the effects of multiple scattering were examined by comparing the results of photon diffusion analysis with those obtained using an analysis based on the Beer-Lambert law, which neglects multiple scattering in the determination of light pathlength. The study found that the difference between the average lengths of the paths traveled by red and infrared photons makes the oximeter's calibration curve (based on measurements obtained from normal subjects) sensitive to the total attenuation coefficients of the tissue in the two wavelength bands used for pulse oximetry, as well as to absorption by the pulsating arterial blood.

FIG. 2 illustrates schematically the disclosed systems, devices, and methods to implement three-dimensional (3D) pulse oximetry in which the emitted light irradiates a larger volume of tissue at the measurement site 102 as compared to the 2D point optical source approach described with respect to FIG. 1. In an embodiment, again looking at the surface of the tissue measurement site 102, the irradiated surface area 206 of the measurement site 102 is substantially rectangular in shape with dimensions in the range of approximately 0.25-3 cm in width and approximately 1-6 cm in length. In another embodiment, the irradiated surface area 206 of the measurement site 102 is substantially rectangular in shape and has dimensions of approximately 1.5 cm in width and approximately 2 cm in length. In another embodiment, the irradiated surface area 206 of the measurement site 102 is substantially rectangular in shape and has dimensions of approximately 0.5 cm in width and approximately 1 cm in length. In another embodiment, the irradiated surface area 206 of the measurement site 102 is substantially rectangular in shape has dimensions of approximately 1 cm in width and approximately 1.5 cm in length. In yet another embodiment, the irradiated surface area 206 of the measurement site 102 is substantially square in shape and has dimensions in a range of approximately 0.25-9 cm². In certain embodiments, the irradiated surface area 206 of the measurement site 102 is within a range of approximately 0.5-2 cm in width, and approximately 1-4 cm in length. Of course a skilled artisan will appreciate that many other shapes and dimensions of irradiated surface area 206 can be used. Advantageously, by irradiating the tissue measurement site 102 with a surface area 206, the presently disclosed systems, devices, and methods apply a three-dimensional analytical model to the three-dimensional structure being measured, namely, the patient's sample tissue 102.

According to the Beer-Lambert law, the amount of light absorbed by a substance is proportional to the concentration of the light-absorbing substance in the irradiated solution (i.e., arterial blood). Advantageously, by irradiating a larger volume of tissue 102, a larger sample size of light attenuated (or reflected) by the tissue 102 is measured. The larger, 3D sample provides a data set that is more representative of the complete interaction of the emitted light as it passes through the patient's blood as compared to the 2D point source approach described above with respect to FIG. 1. By taking an average of the detected light, as detected over a surface area substantially larger than a single point, the disclosed pulse oximetry systems, devices, and methods will yield a more accurate measurement of the emitted light absorbed by the tissue, which will lead to a more accurate oxygen saturation measurement.

FIG. 3 illustrates schematically a side view of a pulse oximetry 3D sensor 300 according to an embodiment of the present disclosure. In the illustrated embodiment, the 3D sensor 300 irradiates the tissue measurement site 102 and detects the emitted light, after being attenuated by the tissue measurement site 102. In other embodiments, for example, as describe below with respect to FIGS. 7A and 7B, the 3D sensor 300 can be arranged to detect light that is reflected by the tissue measurement site 102. The 3D sensor 300 includes an emitter 302, a light diffuser 304, a light-absorbing detector filter 306, a light concentrator 308, and a detector 310. In some optional embodiments, the 3D sensor 300 further includes a reflector 305. The reflector 305 can be a metallic reflector or other type of reflector. Reflector 305 can be a coating, film, layer or other type of reflector. The reflector 305 can serve as a reflector to prevent emitted light from emitting out of a top portion of the light diffuser 304 such that light from the emitter 302 is directed in the tissue rather than escaping out of a side or top of the light diffuser 304. Additionally, the reflector 305 can prevent ambient light from entering the diffuser 304 which might ultimately cause errors within the detected light. The reflector 305 also prevent light piping that might occur if light from the detector 302 is able to escape from the light diffuser 304 and be piped around a sensor securement mechanism to detector 310 without passing through the patient's tissue 102.

The emitter 302 can serve as the source of optical radiation transmitted towards the tissue measurement site 102. The emitter 302 can include one or more sources of optical radiation, such as LEDs, laser diodes, incandescent bulbs with appropriate frequency-selective filters, combinations of the same, or the like. In an embodiment, the emitter 302 includes sets of optical sources that are capable of emitting visible and near-infrared optical radiation. In some embodiments, the emitter 302 transmits optical radiation of red and infrared wavelengths, at approximately 650 nm and approximately 940 nm, respectively. In some embodiments, the emitter 302 includes a single source optical radiation.

The light diffuser 304 receives the optical radiation emitted from the emitter 302 and spreads the optical radiation over an area, such as the area 206 depicted in FIG. 2. In some embodiments, the light diffuser 304 is a beam shaper that can homogenize the input light beam from the emitter 302, shape the output intensity profile of the received light, and define the way (e.g., the shape or pattern) the emitted light is distributed to the tissue measurement site 102. Examples of materials that can be used to realize the light diffuser 304 include, without limitation, a white surface, glass, ground glass, glass beads, polytetrafluoroethylene (also known as Teflon®), opal glass, and greyed glass, to name a few. Additionally, engineered diffusers can be used to realize the diffuser 304 by providing customized light shaping with respect to intensity and distribution. Such diffusers can, for example, deliver substantially uniform illumination over a specified target area (such as, for example, irradiated surface area 206) in an energy-efficient manner. Examples of engineered diffusers can include molded plastics with specific shapes, patterns or textures designed to diffuse the emitter light across the entirety of the patient's tissue surface.

Advantageously, the diffuser 304 can receive emitted light in the form of a point optical source and spread the light to fit a desired surface area on a plane defined by the surface of the tissue measurement site 102. In an embodiment, the diffuser 304 is made of ground glass which spreads the emitted light with a Gaussian intensity profile. In another embodiment the diffuser 304 includes glass beads. In some embodiments, the diffuser 304 is constructed so as to diffuse

the emitted light in a Lambertian pattern. A Lambertian pattern is one in which the radiation intensity is substantially constant throughout the area of dispersion. One such diffuser 304 is made from opal glass. Opal glass is similar to ground glass, but has one surface coated with a milky white coating to diffuse light evenly. In an embodiment, the diffuser 304 is capable of distributing the emitted light on the surface of a plane (e.g., the surface of the tissue measurement site 102) in a predefined geometry (e.g., a rectangle, square, or circle), and with a substantially uniform intensity profile and energy distribution. In some embodiments, the efficiency, or the amount of light transmitted by the diffuser 304, is greater than 70% of the light emitted by the emitter 302. In some embodiments, the efficiency is greater than 90% of the emitted light. Other optical elements known in the art may be used for the diffuser 304.

In an embodiment, the diffuser 304 has a substantially rectangular shape having dimensions within a range of approximately 0.5-2 cm in width and approximately 1-4 centimeters in length. In another embodiment, the substantially rectangular shape of the diffuser 304 has dimensions of approximately 0.5 cm in width and approximately 1 cm in length. In another embodiment, the diffuser's 304 substantially rectangular shape has dimensions of approximately 1 cm in width and approximately 1.5 cm in length. In yet another embodiment, the diffuser 304 has a substantially square shape with dimensions in the range of approximately 0.25-10 cm².

The light-absorbing detector filter 306, which is also depicted in FIG. 4A in a top view, is a planar surface having an opening 402 through which the emitted light may pass after being attenuated by the tissue measurement site 102. In the depicted embodiment, the opening 402 is rectangular-shaped, with dimensions substantially similar to the irradiated surface area 206. According to an embodiment, the light-absorbing detector filter is substantially rectangular in shape and has outer dimensions of 4 cm in width and 8 cm in length, and has an opening through which emitted light may pass, the opening having dimensions of 2 cm in width and 5 cm in length. In another embodiment, the light-absorbing detector filter is substantially rectangular in shape and has outer dimensions in the range of 1-3 cm in width and 2-8 cm in length, and has an opening through which emitted light may pass, the opening having dimensions in the range of 0.25-2 cm in width and 1-4 cm in length. In yet another embodiment, the light-absorbing detector filter is substantially rectangular in shape and has outer dimensions of 3 cm in width and 6 cm in length, and has an opening through which emitted light may pass, the opening having dimensions of 1.5 cm in width and 4 cm in length.

The top surface of the light-absorbing filter 306 (facing the tissue measurement site 102 and the emitter 302) is coated with a material that absorbs light, such as, for example, black pigment. Many other types of light-absorbing materials are well known in the art and can be used with the detector filter 306. During operation, light emitted from the emitter 302 can reflect off of the tissue measurement site 102 (or other structures within the 3D sensor 300) to neighboring portions of the 3D sensor 300. If those neighboring portions of the 3D sensor 300 possess reflective surfaces, then the light can reflect back to the tissue measurement site 102, progress through the tissue and arrive at the detector 310. Such multiple scattering can result in detecting photons whose pathlengths are considerably longer than most of the light that is detected, thereby introducing variations in pathlength which will affect the accuracy of the measurements of the pulse oximetry 3D sensor 300.

Advantageously, the light-absorbing filter **306** reduces or eliminates the amount of emitted light that is reflected in this manner because it absorbs such reflected light, thereby stopping the chain of scattering events. In certain embodiments, the sensor-facing surfaces of other portions of the 3D sensor **300** are covered in light-absorbing material to further decrease the effect of reflective multiple scattering.

The light concentrator **308** is a structure to receive the emitted optical radiation, after attenuation by the tissue measurement site **102**, to collect and concentrate the dispersed optical radiation, and to direct the collected and concentrated optical radiation to the detector **310**. In an embodiment, the light concentrator **308** is made of ground glass or glass beads. In some embodiments, the light concentrator **308** includes a compound parabolic concentrator.

As described above with respect to FIG. 1, the detector **310** captures and measures light from the tissue measurement site **102**. For example, the detector **310** can capture and measure light transmitted from the emitter **302** that has been attenuated by the tissue in the measurement site **102**. The detector **310** can output a detector signal responsive to the light captured or measured. The detector **310** can be implemented using one or more photodiodes, phototransistors, or the like. In addition, a plurality of detectors **310** can be arranged in an array with a spatial configuration corresponding to the irradiated surface area **206** to capture the attenuated or reflected light from the tissue measurement site.

Referring to FIG. 4A, a top view of a portion of the 3D sensor **300** is provided. The light-absorbing detector filter **306** is illustrated having a top surface coated with a light-absorbing material. The light-absorbing material can be a black opaque material or coating or any other dark color or coating configured to absorb light. Additionally, a rectangular opening **402** is positioned relative to the light concentrator **308** (shown in phantom) and the detector **310** such that light may pass through the rectangular opening **402**, into the light concentrator **308**, and to the detector **310**. FIG. 4B illustrates the top view of a portion of the 3D sensor **300** as in FIG. 4A, with the addition of the tissue measurement site **102** in operational position. Accordingly, the rectangular opening **402**, the light concentrator **308** and the detector **310** are shown in phantom as being under the tissue measurement site **102**. In FIGS. 4A and 4B, the light concentrator **308** is shown to have dimensions significantly larger than the dimensions of the rectangular opening **402**. In other embodiments, the dimensions of the light concentrator **308**, the rectangular opening **402**, and the irradiated surface area **206** are substantially similar.

FIG. 5 illustrates a top view of a 3D pulse oximetry sensor **500** according to an embodiment of the present disclosure. The 3D sensor **500** is configured to be worn on a patient's finger **102**. The 3D sensor **500** includes an adhesive substrate **502** having front flaps **504** and rear flaps **506** extending outward from a center portion **508** of the 3D sensor **500**. The center portion **508** includes components of the 3D pulse oximetry sensor **300** described with respect to FIGS. 3, 4A and 4B. On the front side of the adhesive substrate **502** the emitter **302** and the light diffuser **304** are positioned. On the rear side of the adhesive substrate **502** the light-absorbent detector filter **306**, the light concentrator **308** and the detector **310** are positioned. In use, the patient's finger serving as the tissue measurement site **102** is positioned over the rectangular opening **402** such that when the front portion of the adhesive substrate is folded over on top of the patient's finger **102**, the emitter **302** and the light diffuser **304** are aligned with the measurement site **102**, the filter **306**, the light concentrator **308** and the detector **310**. Once alignment

is established, the front and rear flaps **504**, **506** can be wrapped around the finger measurement site **102** such that the adhesive substrate **502** provides a secure contact between the patient's skin and the 3D sensor **500**. FIG. 5 also illustrates an example of a sensor connector cable **510** which is used to connect the 3D sensor **500** to a monitor **809**, as described with respect to FIG. 8.

FIG. 6 is a simplified schematic illustration of a conventional, 2D approach to reflective pulse oximetry in which the emitter is configured to emit optical radiation as a point optical source. Reflective pulse oximetry is a method by which the emitter and detector are located on the same side of the tissue measurement site **102**. Light is emitted into a tissue measurement site **102** and attenuated. The emitted light passes into the tissue **102** and is then reflected back to the same side of the tissue measurement site **102** as the emitter. As illustrated in FIG. 6, a depicted reflective 2D pulse oximetry sensor **600** includes an emitter **602**, a light block **606**, and a detector **610**. The light block **606** is necessary because the emitter **602** and the detector **610** are located on the same side of the tissue measurement site **102**. Accordingly, the light block **606** prevents incident emitter light, which did not enter the tissue measurement site **102**, from arriving at the detector **610**. The depicted 2D pulse oximetry sensor **600** is configured to emit light as a point source. As depicted in FIG. 6, a simplified illustration of the light path **620** of the emitted light from the emitter **602**, through the tissue measurement site **102**, and to the detector **610** is provided. Notably, a point source of light is emitted, and a point source of light is detected. As discussed above with respect to FIG. 1, use of a point optical source can result in substantial measurement error due to pathlength variability resulting from the multiple scatter phenomenon. The sample space provided by a 2D point optical emitter source is not large enough to account for pathlength variability, which will skew measurement results.

FIGS. 7A and 7B are simplified schematic side and top views, respectively, of a 3D reflective pulse oximetry sensor **700** according to an embodiment of the present disclosure. In the illustrated embodiment, the 3D sensor **700** irradiates the tissue measurement site **102** and detects the emitted light that is reflected by the tissue measurement site **102**. The 3D sensor **700** can be placed on a portion of the patient's body that has relatively flat surface, such as, for example a wrist, because the emitter **702** and detector **710** are on located the same side of the tissue measurement site **102**. The 3D sensor **700** includes an emitter **702**, a light diffuser **704**, a light block **706**, a light concentrator **708**, and a detector **710**.

As previously described, the emitter **702** can serve as the source of optical radiation transmitted towards the tissue measurement site **102**. The emitter **702** can include one or more sources of optical radiation. Such sources of optical radiation can include LEDs, laser diodes, incandescent bulbs with appropriate frequency-selective filters, combinations of the same, or the like. In an embodiment, the emitter **702** includes sets of optical sources that are capable of emitting visible and near-infrared optical radiation. In some embodiments, the emitter **702** transmits optical radiation of red and infrared wavelengths, at approximately 650 nm and approximately 940 nm, respectively. In some embodiments, the emitter **702** includes a single source of optical radiation.

The light diffuser **704** receives the optical radiation emitted from the emitter **302** and homogeneously spreads the optical radiation over a wide, donut-shaped area, such as the area outlined by the light diffuser **704** as depicted in FIG. 7B. Advantageously, the diffuser **704** can receive emitted light in the form of a 2D point optical source (or any other

form) and spread the light to fit the desired surface area on a plane defined by the surface of the tissue measurement site **102**. In an embodiment, the diffuser **704** is made of ground glass or glass beads. A skilled artisan will understand that may other materials can be used to make the light diffuser **704**.

The light blocker **706** includes an annular ring having a cover portion **707** sized and shaped to form a light isolation chamber for the light concentrator **708** and the detector **710**. (For purposes of illustration, the light block cover **707** is not illustrated in FIG. 7B.) The light blocker **706** and the cover **707** can be made of any material that optically isolates the light concentrator **708** and the detector **710**. The light isolation chamber formed by the light blocker **706** and cover **708** ensures that the only light detected by the detector **710** is light that is reflected from the tissue measurement site.

The light concentrator **708** is a cylindrical structure with a truncated circular conical structure on top, the truncated section of which is adjacent the detector **710**. The light concentrator **708** is structured to receive the emitted optical radiation, after reflection by the tissue measurement site **102**, and to direct the reflected light to the detector **710**. In an embodiment, the light concentrator **708** is made of ground glass or glass beads. In some embodiments, the light concentrator **708** includes a compound parabolic concentrator.

As previously described, the detector **710** captures and measures light from the tissue measurement site **102**. For example, the detector **710** can capture and measure light transmitted from the emitter **702** that has been reflected from the tissue in the measurement site **102**. The detector **710** can output a detector signal responsive to the light captured or measured. The detector **710** can be implemented using one or more photodiodes, phototransistors, or the like. In addition, a plurality of detectors **710** can be arranged in an array with a spatial configuration corresponding to the irradiated surface area depicted in FIG. 7B by the light concentrator **708** to capture the reflected light from the tissue measurement site.

Advantageously, the light path **720** illustrated in FIG. 7A depicts a substantial sample of reflected light that enter the light isolation chamber formed by the light blocker **706** and cover **707**. As previously discussed, the large sample of reflected light (as compared to the reflected light collected using the 2D point optical source approach) provides the opportunity to take an average of the detected light, to derive a more accurate measurement of the emitted light absorbed by the tissue, which will lead to a more accurate oxygen saturation measurement.

Referring now to FIG. 7B, a top view of the 3D sensor **700** is illustrated with both the emitter **702** and the light blocker cover **707** removed for ease of illustration. The outer ring illustrates the footprint of the light diffuser **704**. As light is emitted from the emitter **702** (not shown in FIG. 7B), it is diffused homogenously and directed to the tissue measurement site **102**. The light blocker **706** forms the circular wall of a light isolation chamber to keep incident light from being sensed by the detector **710**. The light blocker cover **707** blocks incidental light from entering the light isolation chamber from above. The light concentrator **708** collects the reflected light from the tissue measurement site **102** and funnels it upward toward the detector **710** at the center of the 3D sensor **700**.

FIG. 8 illustrates an example of an optical physiological measurement system **800**, which may also be referred to herein as a pulse oximetry system **800**. In certain embodiments, the pulse oximetry system **800** noninvasively mea-

sures a blood analyte, such as oxygen, carboxyhemoglobin, methemoglobin, total hemoglobin, glucose, proteins, lipids, a percentage thereof (e.g., saturation), pulse rate, perfusion index, oxygen content, total hemoglobin, Oxygen Reserve Index™ (ORI™) or many other physiologically relevant patient characteristics. These characteristics can relate to, for example, pulse rate, hydration, trending information and analysis, and the like. The system **800** can also measure additional blood analytes and/or other physiological parameters useful in determining a state or trend of wellness of a patient.

The pulse oximetry system **800** can measure analyte concentrations at least in part by detecting optical radiation attenuated by tissue at a measurement site **102**. The measurement site **102** can be any location on a patient's body, such as a finger, foot, earlobe, wrist, forehead, or the like.

The pulse oximetry system **800** can include a sensor **801** (or multiple sensors) that is coupled to a processing device or physiological monitor **809**. In an embodiment, the sensor **801** and the monitor **809** are integrated together into a single unit. In another embodiment, the sensor **801** and the monitor **809** are separate from each other and communicate with one another in any suitable manner, such as via a wired or wireless connection. The sensor **801** and monitor **809** can be attachable and detachable from each other for the convenience of the user or caregiver, for ease of storage, sterility issues, or the like.

In the depicted embodiment shown in FIG. 8, the sensor **801** includes an emitter **804**, a detector **806**, and a front-end interface **808**. The emitter **804** can serve as the source of optical radiation transmitted towards measurement site **102**. The emitter **804** can include one or more sources of optical radiation, such as light emitting diodes (LEDs), laser diodes, incandescent bulbs with appropriate frequency-selective filters, combinations of the same, or the like. In an embodiment, the emitter **804** includes sets of optical sources that are capable of emitting visible and near-infrared optical radiation.

The pulse oximetry system **800** also includes a driver **811** that drives the emitter **804**. The driver **811** can be a circuit or the like that is controlled by the monitor **809**. For example, the driver **811** can provide pulses of current to the emitter **804**. In an embodiment, the driver **811** drives the emitter **804** in a progressive fashion, such as in an alternating manner. The driver **811** can drive the emitter **804** with a series of pulses for some wavelengths that can penetrate tissue relatively well and for other wavelengths that tend to be significantly absorbed in tissue. A wide variety of other driving powers and driving methodologies can be used in various embodiments. The driver **811** can be synchronized with other parts of the sensor **801** to minimize or reduce jitter in the timing of pulses of optical radiation emitted from the emitter **804**. In some embodiments, the driver **811** is capable of driving the emitter **804** to emit optical radiation in a pattern that varies by less than about 10 parts-per-million.

The detector **806** captures and measures light from the tissue measurement site **102**. For example, the detector **806** can capture and measure light transmitted from the emitter **804** that has been attenuated or reflected from the tissue at the measurement site **102**. The detector **806** can output a detector signal **107** responsive to the light captured and measured. The detector **806** can be implemented using one or more photodiodes, phototransistors, or the like. In some embodiments, a detector **806** is implemented in detector package to capture and measure light from the tissue measurement site **102** of the patient. The detector package can

include a photodiode chip mounted to leads and enclosed in an encapsulant. In some embodiments, the dimensions of the detector package are approximately 2 square centimeters. In other embodiments, the dimensions of the detector package are approximately 1.5 centimeters in width and approximately 2 centimeters in length.

The front-end interface **808** provides an interface that adapts the output of the detectors **806**, which is responsive to desired physiological parameters. For example, the front-end interface **808** can adapt the signal **807** received from the detector **806** into a form that can be processed by the monitor **809**, for example, by a signal processor **810** in the monitor **809**. The front-end interface **808** can have its components assembled in the sensor **801**, in the monitor **809**, in a connecting cabling (if used), in combinations of the same, or the like. The location of the front-end interface **808** can be chosen based on various factors including space desired for components, desired noise reductions or limits, desired heat reductions or limits, and the like.

The front-end interface **808** can be coupled to the detector **806** and to the signal processor **810** using a bus, wire, electrical or optical cable, flex circuit, or some other form of signal connection. The front-end interface **808** can also be at least partially integrated with various components, such as the detectors **806**. For example, the front-end interface **808** can include one or more integrated circuits that are on the same circuit board as the detector **806**. Other configurations can also be used.

As shown in FIG. 8, the monitor **909** can include the signal processor **810** and a user interface, such as a display **812**. The monitor **809** can also include optional outputs alone or in combination with the display **812**, such as a storage device **814** and a network interface **816**. In an embodiment, the signal processor **810** includes processing logic that determines measurements for desired analytes based on the signals received from the detector **806**. The signal processor **810** can be implemented using one or more microprocessors or sub-processors (e.g., cores), digital signal processors, application specific integrated circuits (ASICs), field programmable gate arrays (FPGAs), combinations of the same, and the like.

The signal processor **810** can provide various signals that control the operation of the sensor **801**. For example, the signal processor **810** can provide an emitter control signal to the driver **811**. This control signal can be useful in order to synchronize, minimize, or reduce jitter in the timing of pulses emitted from the emitter **804**. Accordingly, this control signal can be useful in order to cause optical radiation pulses emitted from the emitter **804** to follow a precise timing and consistent pattern. For example, when a transimpedance-based front-end interface **808** is used, the control signal from the signal processor **810** can provide synchronization with an analog-to-digital converter (ADC) in order to avoid aliasing, cross-talk, and the like. As also shown, an optional memory **813** can be included in the front-end interface **808** and/or in the signal processor **810**. This memory **813** can serve as a buffer or storage location for the front-end interface **808** and/or the signal processor **810**, among other uses.

The user interface **812** can provide an output, e.g., on a display, for presentation to a user of the pulse oximetry system **800**. The user interface **812** can be implemented as a touch-screen display, a liquid crystal display (LCD), an organic LED display, or the like. In alternative embodiments, the pulse oximetry system **800** can be provided without a user interface **812** and can simply provide an output signal to a separate display or system.

The storage device **814** and a network interface **816** represent other optional output connections that can be included in the monitor **809**. The storage device **814** can include any computer-readable medium, such as a memory device, hard disk storage, EEPROM, flash drive, or the like. The various software and/or firmware applications can be stored in the storage device **814**, which can be executed by the signal processor **810** or another processor of the monitor **809**. The network interface **816** can be a serial bus port (RS-232/RS-485), a Universal Serial Bus (USB) port, an Ethernet port, a wireless interface (e.g., WiFi such as any 802.1x interface, including an internal wireless card), or other suitable communication device(s) that allows the monitor **809** to communicate and share data with other devices. The monitor **809** can also include various other components not shown, such as a microprocessor, graphics processor, or controller to output the user interface **812**, to control data communications, to compute data trending, or to perform other operations.

Although not shown in the depicted embodiment, the pulse oximetry system **800** can include various other components or can be configured in different ways. For example, the sensor **801** can have both the emitter **804** and detector **806** on the same side of the tissue measurement site **102** and use reflectance to measure analytes.

Although the foregoing disclosure has been described in terms of certain preferred embodiments, many other variations than those described herein will be apparent to those of ordinary skill in the art.

Conditional language used herein, such as, among others, “can,” “might,” “may,” “e.g.,” and the like, unless specifically stated otherwise, or otherwise understood within the context as used, is generally intended to convey that certain embodiments include, while other embodiments do not include, certain features, elements and/or states. Thus, such conditional language is not generally intended to imply that features, elements and/or states are in any way required for one or more embodiments or that one or more embodiments necessarily include logic for deciding, with or without author input or prompting, whether these features, elements and/or states are included or are to be performed in any particular embodiment. The terms “comprising,” “including,” “having,” and the like are synonymous and are used inclusively, in an open-ended fashion, and do not exclude additional elements, features, acts, operations, and so forth. Also, the term “or” is used in its inclusive sense (and not in its exclusive sense) so that when used, for example, to connect a list of elements, the term “or” means one, some, or all of the elements in the list. Further, the term “each,” as used herein, in addition to having its ordinary meaning, can mean any subset of a set of elements to which the term “each” is applied.

While the above detailed description has shown, described, and pointed out novel features as applied to various embodiments, it will be understood that various omissions, substitutions, and changes in the form and details of the systems, devices or algorithms illustrated can be made without departing from the spirit of the disclosure. As will be recognized, certain embodiments of the disclosure described herein can be embodied within a form that does not provide all of the features and benefits set forth herein, as some features can be used or practiced separately from others.

The term “and/or” herein has its broadest, least limiting meaning which is the disclosure includes A alone, B alone, both A and B together, or A or B alternatively, but does not require both A and B or require one of A or one of B. As used

15

herein, the phrase “at least one of” A, B, “and” C should be construed to mean a logical A or B or C, using a non-exclusive logical or.

The apparatuses and methods described herein may be implemented by one or more computer programs executed by one or more processors. The computer programs include processor-executable instructions that are stored on a non-transitory tangible computer readable medium. The computer programs may also include stored data. Non-limiting examples of the non-transitory tangible computer readable medium are nonvolatile memory, magnetic storage, and optical storage. Although the foregoing disclosure has been described in terms of certain preferred embodiments, other embodiments will be apparent to those of ordinary skill in the art from the disclosure herein. Additionally, other combinations, omissions, substitutions and modifications will be apparent to the skilled artisan in view of the disclosure herein. Accordingly, the present invention is not intended to be limited by the description of the preferred embodiments, but is to be defined by reference to claims.

Additionally, all publications, patents, and patent applications mentioned in this specification are herein incorporated by reference to the same extent as if each individual publication, patent, or patent application were specifically and individually indicated to be incorporated by reference.

What is claimed is:

1. An optical physiological measurement device configured for placement on a patient at a tissue measurement site, the device comprising:

one or more emitters configured to emit light so as to irradiate the tissue measurement site; and

a plurality of detectors configured to detect the emitted light after attenuation by and reflection from a portion of the tissue measurement site, the portion of the tissue measurement site having an at least partially circular shape bounded by a light block, the tissue measurement site located on a wrist of the patient, the plurality of detectors further configured to transmit a signal responsive to the detected light;

wherein the light block comprises an annular ring having a circular shape located between the emitted light at the tissue measurement site and the plurality of detectors, the light block reducing an amount of incident light emitted from the one or more emitters from being detected by the plurality of detectors, wherein the plurality of detectors are arranged in an array having a spatial configuration corresponding to the shape of the portion of the tissue measurement site.

2. The optical physiological measurement device of claim 1, further comprising a processor configured to receive the transmitted signal responsive to the detected light and to determine a physiological parameter.

3. The optical physiological measurement device of claim 2, wherein the parameter is arterial oxygen saturation.

4. The optical physiological measurement device of claim 1, further comprising a diffuser which receives, spreads and emits the spread light, wherein the emitted spread light is directed at the tissue measurement site.

5. The optical physiological measurement device of claim 4, further comprising a concentrator which receives the light after attenuation by tissue of the patient, concentrates the received light and emits the concentrated light in the direction of the plurality of detectors.

6. The optical physiological measurement device of claim 5, wherein the concentrator comprises at least one of glass, ground glass, glass beads, opal glass, and a compound parabolic concentrator.

16

7. The optical physiological measurement device of claim 4, wherein the diffuser comprises at least one of a glass diffuser, ground glass diffuser, a glass bead diffuser, an opal glass diffuser, and an engineered diffuser.

8. The optical physiological measurement device of claim 4, wherein the diffuser emits the spread light with a substantially uniform intensity profile.

9. The optical physiological measurement system of claim 4, wherein the diffuser defines a surface area shape by which the emitted spread light is distributed onto a surface of the tissue measurement site.

10. The optical physiological measurement device of claim 1, wherein the one or more emitters are positioned outside the annular ring when the optical physiological measurement device is placed on the patient at the tissue measurement site, and wherein the plurality of detectors are positioned inside the annular ring when the optical physiological measurement device is placed on the patient at the tissue measurement site.

11. A method to determine a constituent or analyte in a patient's blood, the method comprising:

emitting, from at least one emitter of an optical sensor, light of one or more wavelengths so as to irradiate a tissue measurement site, wherein the tissue measurement site is located on a wrist of a patient;

detecting, with a plurality of detectors, the emitted light after attenuation by and reflection from a portion of the tissue measurement site, the portion having an at least partially circular shape; and providing an annular ring located between the emitted light at the tissue measurement site and the plurality of detectors, wherein the annular ring reduces an amount of incident light emitted from the at least one emitter from arriving at the plurality of detectors, and wherein the plurality of detectors are arranged in an array having a spatial configuration corresponding to the shape of the portion of the tissue measurement site.

12. The method of claim 11, further comprising:

transmitting, from the a plurality of detectors, a signal responsive to the detected light;

receiving, by a processor, the transmitted signal responsive to the detected light; and

processing, by the processor, the received signal responsive to the detected light to determine a physiological parameter.

13. The method of claim 11, further comprising spreading, with a diffuser, the emitted light and emitting the spread light from the diffuser to the tissue measurement site, wherein the diffuser spreads the light over a greater area of the tissue measurement site than would otherwise be illuminated by the emitter directly emitting light at the tissue measurement site.

14. The method of claim 13, further comprising receiving, by a concentrator, the emitted spread light after the spread light has been attenuated by and reflected from the tissue measurement site and concentrating, by the concentrator, the received light and emitting the concentrated light from the concentrator to the a plurality of detectors.

15. The method of claim 14, wherein concentrating, by the concentrator, the received light and emitting the concentrated light from the concentrator to the plurality of detectors is performed by at least one of a glass concentrator, a glass bead concentrator, an opal glass concentrator, and a compound parabolic concentrator.

16. The method of claim 13, wherein spreading, with a diffuser, the emitted light and emitting the spread light from the diffuser to the tissue measurement site is performed by

17

at least one of a glass diffuser, a glass bead diffuser, an opal glass diffuser, and an engineered diffuser.

17. The method of claim 13, wherein spreading, with a diffuser, the emitted light and emitting the spread light from the diffuser to the tissue measurement site further comprises spreading the emitted light with a substantially uniform intensity profile.

18. The method of claim 13, wherein spreading, with a diffuser, the emitted light and emitting the spread light from the diffuser to the tissue measurement site further comprises spreading the emitted light so as to define a surface area shape by which the emitted spread light is distributed onto a surface of the tissue measurement site.

19. The method of claim 11, wherein the at least one emitter is positioned outside the annular ring when the optical sensor is placed on the patient at the tissue measurement site, and wherein the plurality of detectors are positioned inside the annular ring when the optical sensor is placed on the patient at the tissue measurement site.

20. A pulse oximeter sensor comprising:

one or more optical sources configured to emit light at one or more wavelengths, wherein, when the pulse oximeter sensor is placed on a patient at a tissue measurement site, the one or more optical sources are positioned in a reflectance measurement configuration on a first side of the tissue measurement site, and wherein the one or more optical sources are configured to irradiate the tissue measurement site; a plurality of detectors configured to detect light emitted from the one or more optical sources after attenuation by a portion of the tissue measurement site, the portion of the tissue measurement site having an at least partially circular shape, the plurality of detectors arranged in an array having a spatial configuration corresponding to the shape of the portion of the tissue measurement site so as to capture the emitted light reflected from the tissue measurement site, wherein the plurality of detectors are positioned in a reflectance measurement configuration on the first side of the tissue measurement site when the pulse oximeter sensor is placed on the patient, the plurality of detectors further configured to output a signal responsive to the detected light; and a light block comprising an annular ring located between the emitted light at the tissue measurement site and the plurality of detectors, the light block reducing an amount of incident light emitted from the one or more optical sources from arriving at the plurality of detectors.

21. The pulse oximeter sensor of claim 20, further comprising a concentrator which concentrates the emitted light after it has been attenuated by the tissue measurement site and directs the concentrated light toward the plurality of detectors.

22. The pulse oximeter sensor of claim 20, wherein the plurality of detectors are further configured to output the signals response to the detected light to a processor configured to receive the signals responsive to the detected light and to determine a physiological parameter.

23. The pulse oximeter sensor of claim 20, further comprising a diffuser configured to receive the emitted light, to

18

spread the received light, and to emit the spread light, wherein the emitted spread light is directed at the tissue measurement site.

24. The pulse oximeter sensor of claim 23, wherein the diffuser is further configured to define a surface area shape by which the emitted spread light is distributed onto a surface of the tissue measurement site.

25. The pulse oximeter sensor of claim 20, wherein the one or more optical sources are positioned outside the annular ring when the pulse oximeter sensor is placed on the patient at the tissue measurement site, and wherein the plurality of detectors are positioned inside the annular ring when the pulse oximeter sensor is placed on the patient at the tissue measurement site.

26. A pulse oximeter sensor comprising:

one or more optical sources configured to emit light at one or more wavelengths, wherein, when the pulse oximeter sensor is placed on a patient at a tissue measurement site, the one or more optical sources are positioned in a reflectance measurement configuration on a first side of the tissue measurement site, and wherein the one or more optical sources are configured to irradiate the tissue measurement site, and wherein the tissue measurement site is located on a wrist of the patient; a plurality of detectors configured to detect light emitted from the one or more optical sources after attenuation by and reflection from a portion of the tissue measurement site, the portion of the tissue measurement site having an annular shape, wherein the plurality of detectors are positioned in a reflectance measurement configuration on the first side of the tissue measurement site when the pulse oximeter sensor is placed on the patient, the plurality of detectors further configured to output signals responsive to the detected light; and a light block comprising an annular ring located between the emitted light at the tissue measurement site and the plurality of detectors, the light block reducing an amount of incident light emitted from the one or more optical sources that does not enter the tissue measurement site arriving at the plurality of detectors, wherein the plurality of detectors are positioned in an array having a spatial configuration corresponding to the annular shape of the portion of the tissue measurement site.

27. The pulse oximeter sensor of claim 26, wherein the plurality of detectors are further configured to transmit the output signals responsive to the detected light to a processor configured to receive the signals responsive to the detected light and to determine a physiological parameter.

28. The pulse oximeter sensor of claim 26, wherein the one or more optical sources are positioned outside the annular ring when the pulse oximeter sensor is placed on the patient at the tissue measurement site, and wherein the plurality of detectors are positioned inside the annular ring when the pulse oximeter sensor is placed on the patient at the tissue measurement site.

* * * * *

专利名称(译)	先进的脉搏血氧饱和度传感器		
公开(公告)号	US10448871	公开(公告)日	2019-10-22
申请号	US15/195199	申请日	2016-06-28
[标]申请(专利权)人(译)	梅西莫股份有限公司		
申请(专利权)人(译)	Masimo公司		
当前申请(专利权)人(译)	Masimo公司		
[标]发明人	AL ALI AMMAR		
发明人	AL-ALI, AMMAR		
IPC分类号	A61B5/1455 A61B5/024 A61B5/00 A61B5/145		
CPC分类号	A61B5/14532 A61B5/4875 A61B5/742 A61B5/14546 A61B5/02416 A61B5/6826 A61B5/7278 A61B5/0002 A61B5/14552 A61B2562/04		
优先权	62/188430 2015-07-02 US		
其他公开文献	US20170000394A1		
外部链接	Espacenet		

摘要(译)

公开了基于光学的非侵入性生理监测系统。一个实施例包括配置为发射光的发射器。漫射器被配置为接收和扩散所发射的光，并在组织测量部位处发射所扩散的光。该系统还包括集中器，该集中器被配置为在已被组织测量部位衰减或反射后接收扩展光。聚光器还被配置为收集并聚光接收到的光，并将聚光发射到检测器。检测器被配置为检测会聚的光并传输代表检测到的光的信号。处理器被配置为接收所传输的信号并确定组织测量部位中的生理参数，例如动脉血氧饱和度。

