



US 20170035313A1

(19) **United States**

(12) **Patent Application Publication**
HONG et al.

(10) **Pub. No.: US 2017/0035313 A1**
(43) **Pub. Date: Feb. 9, 2017**

(54) **MOVEMENT PATTERN MEASURING
APPARATUS USING EEG AND EMG AND
METHOD THEREOF**

A61B 5/11 (2006.01)

A61B 5/0476 (2006.01)

A61B 5/0488 (2006.01)

(71) Applicant: **SOONGSIL UNIVERSITY
RESEARCH CONSORTIUM
TECHNO- PAR, Seoul (KR)**

(52) **U.S. Cl.**

CPC *A61B 5/04012* (2013.01); *A61B 5/0476*
(2013.01); *A61B 5/0488* (2013.01); *A61B*
5/1126 (2013.01); *A61B 5/7264* (2013.01);
A61B 5/7207 (2013.01)

(72) Inventors: **Jiman HONG, Seoul (KR); Giwook
KANG, Seoul (KR)**

(73) Assignee: **SOONGSIL UNIVERSITY
RESEARCH CONSORTIUM
TECHNO- PARK, Seoul (KR)**

(21) Appl. No.: **15/219,294**

(22) Filed: **Jul. 26, 2016**

(30) **Foreign Application Priority Data**

Aug. 3, 2015 (KR) 10-2015-0109470

Publication Classification

(51) **Int. Cl.**


A61B 5/04 (2006.01)

A61B 5/00 (2006.01)


(57)

ABSTRACT


Disclosed is an apparatus for measuring movements of a user, which may include: a sample pattern storing unit for storing one or more sample patterns which are obtained by patterning EEG waveforms and EMG values; a communication unit for receiving an EEG waveform and an EMG value of the user measured by the EEG and EMG sensors; a pattern normalizing unit for selecting sample patterns with the highest similarity to the received user's patterns among the stored sample patterns, and for normalizing the received user's patterns so that their amplitudes and periods coincide with those of the selected sample patterns; a movement estimating unit for estimating movement of the user by inputting the normalized EEG waveform and EMG value in an artificial neural network algorithm; and a movement determining unit for calculating the user's movement by applying each weight value of the EEG and EMG to each movement estimation value.

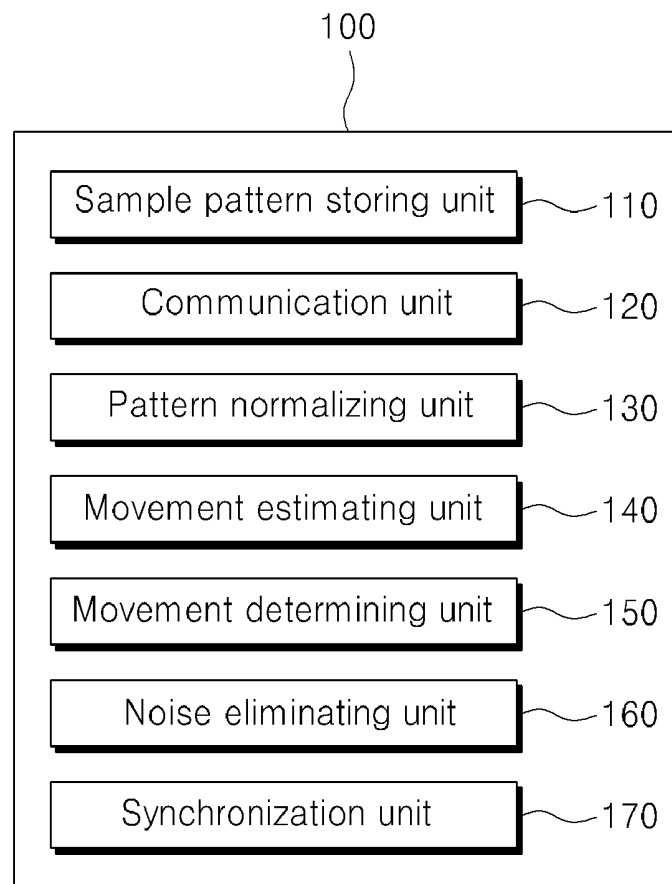


【FIG. 1】

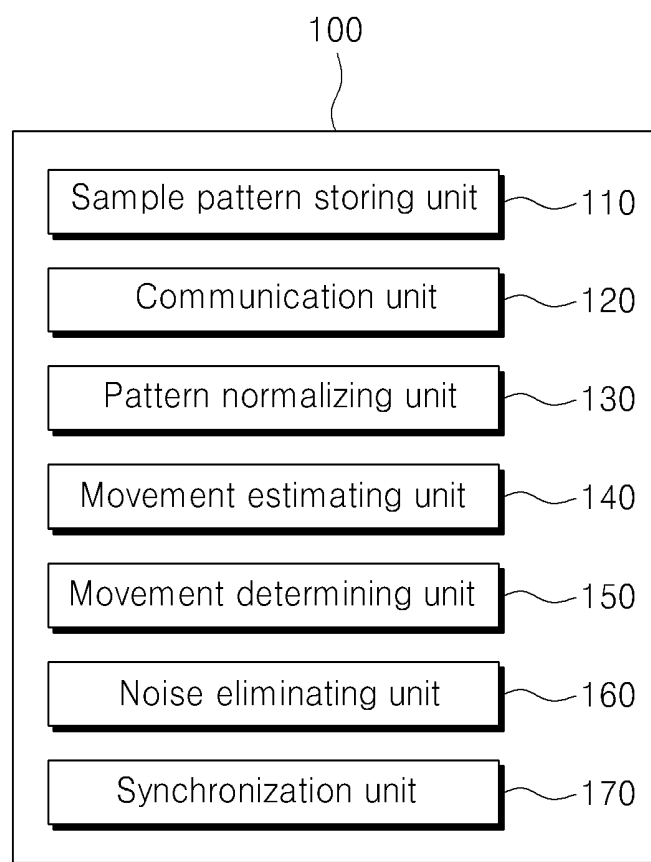

【FIG. 2】

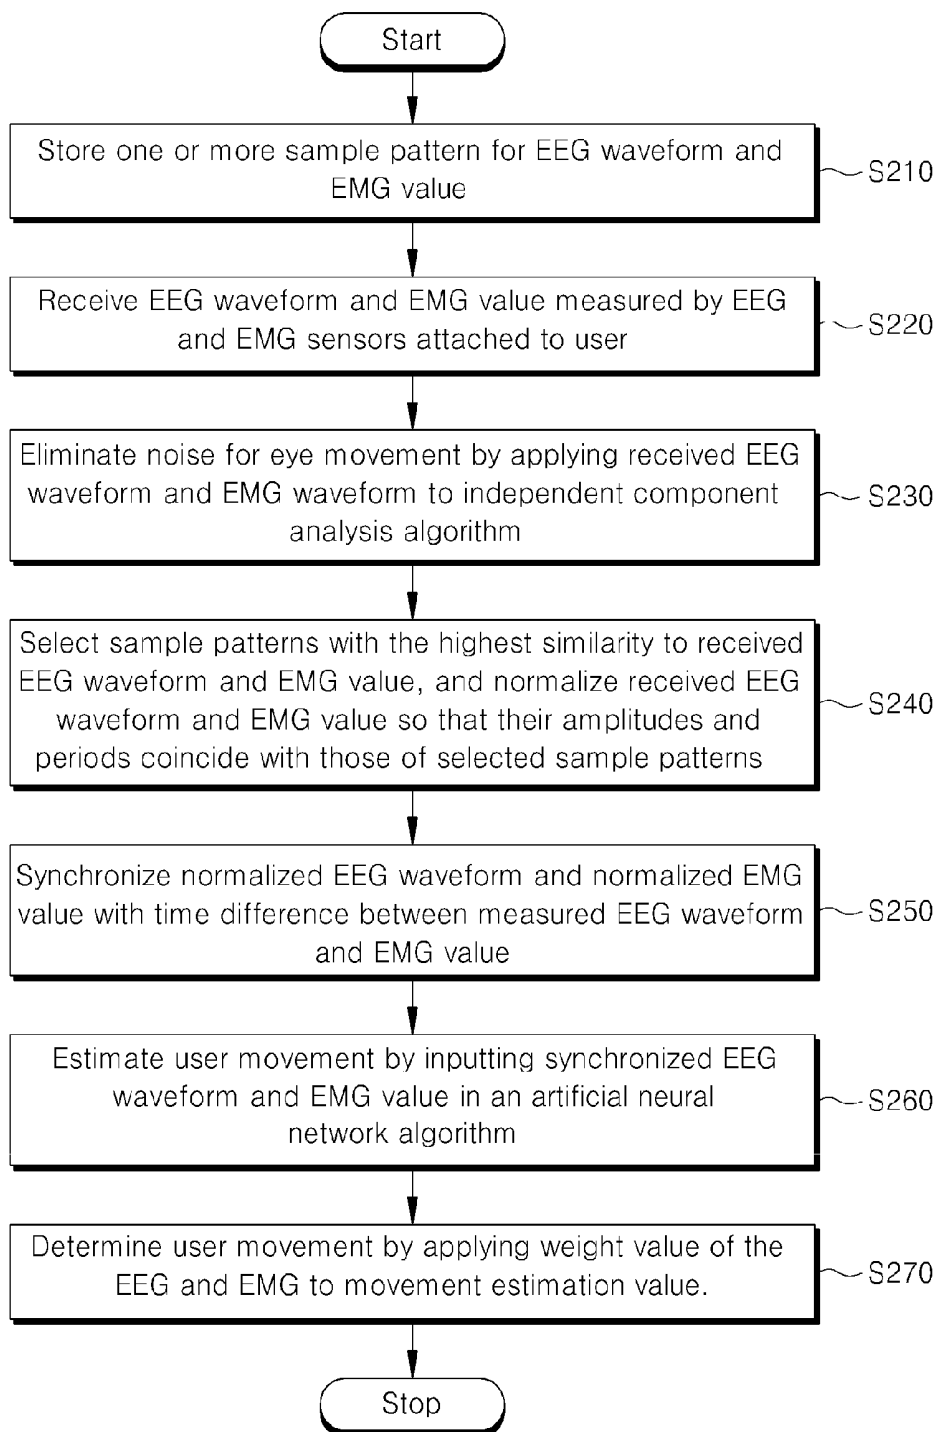

【FIG. 3】

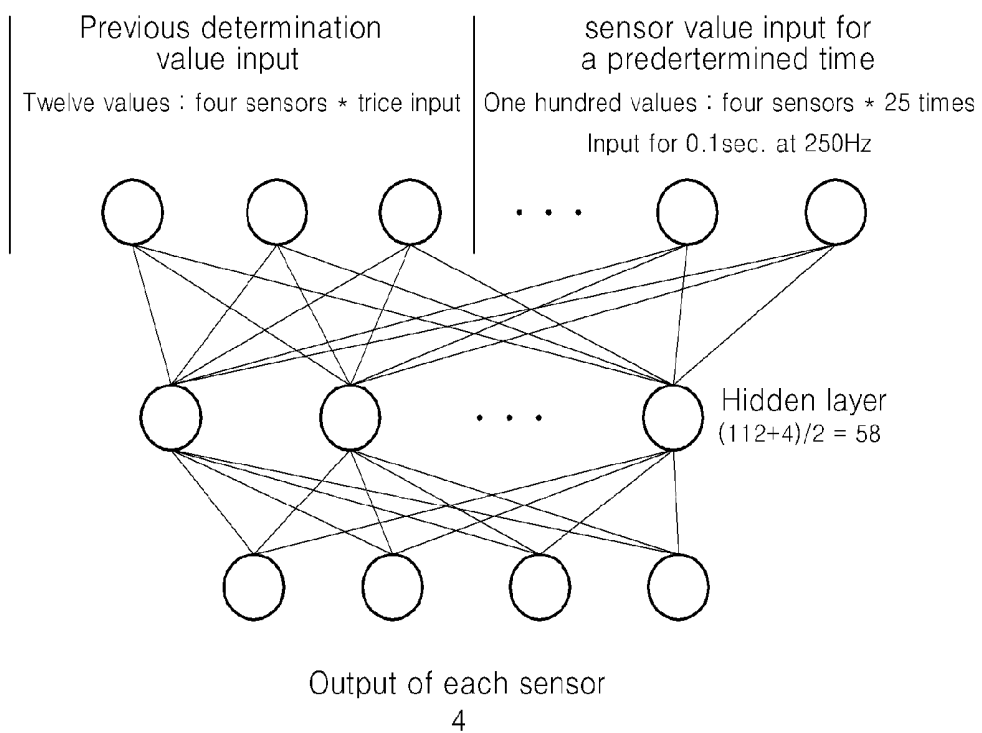

**MOVEMENT PATTERN MEASURING
APPARATUS USING EEG AND EMG AND
METHOD THEREOF**

**CROSS-REFERENCE TO RELATED
APPLICATION**

[0001] This application claims priority to and the benefit of Korean Patent Application No. 10-2015-0109470 filed in the Korean Intellectual Property Office on Aug. 3, 2015, the entire contents of which are incorporated herein by reference.

BACKGROUND OF THE INVENTION

[0002] (a) Field of the Invention

[0003] The present disclosure relates to a movement pattern measuring apparatus using electroencephalogram (EEG) and electromyogram (EMG) data and a method thereof. More particularly, the present disclosure relates to an apparatus and a method for analyzing user movement patterns by using EEG waveforms and EMG values measured from a user.

[0004] (b) Description of the Related Art

[0005] Human-Computer Interface (HCI) based bio-signal is a technology which enables the interfaces between human and computers by using bio-signals which can be artificially created, particularly when the elderly and infirm, and the disabled use the computers. Further, this is a technology which creates commands for controlling operation of rehabilitation tools such as a wheelchair, an artificial limb, etc., and can be utilized as the interface for a wearable computer or crippled people.

[0006] In HCI, since the bio-signals based on EEG and EMG can be used as input signals without using a keyboard or a touchpad, direct activities for input are not required. Accordingly, in the field of HCI, for disabled people with uncomfortable legs and arms, technologies related with the computer input and the artificial limb have been studied.

[0007] Brainwave signals or EEG signals refer to electrical fluctuation created by interactions between neurons in the nervous system, and are measured by electrodes placed on the scalp. These EEG signals may be used for sleep state analysis, concentration or tension degree measurement, schematic feeling recognition, etc.

[0008] HCI using the EEG signals is also applied to games. In this case, without any controller or keyboard, only brainwaves are used as inputs of the computer. Currently, researches on a game input technology capable of being most widely used and allowing various inputs have been actively attempted. By using that the concentration degree can be measured via the brainwaves, another research, which utilizes a result obtained from a waveform of a psychiatric patient in the meditation state for a diagnosis, is also being done.

[0009] As such, various technologies using the brainwaves serving as a means for HCI have been studied, but there are some problems. Noise and artifacts are inevitably mixed in the measured brainwave, so information loss by the noise and artifacts may occur. These bring a difficulty in analyzing the information.

[0010] Since a waveform measured by an EEG sensor when a user performs a specific activity has a simple wavelength, the brainwave corresponding to the specific activity may have one kind of wavelength, but the activity

corresponding to one kind of wavelength may be plural. In order to accurately match the measured brainwave with the specific activity, therefore, a technology of measuring EEG and EMG using EEG and EMG sensors together is required.

[0011] Further, in known technologies, to pattern the measured brainwave, the most similar pattern of a series of patterns stored in a database was selected. However, because each person's brainwave has different amplitude, such a patterning has a limitation in searching an accurate pattern. Accordingly, after several measurements, a normalization process for the individual brainwaves should be performed.

[0012] Korean Patent Publication No. 10-1293446 (published on Aug. 5, 2013) discloses a background technique of the present disclosure.

SUMMARY OF THE INVENTION

[0013] The present invention has been made in an effort to provide an apparatus and a method for analyzing user movement patterns by using EEG waveforms and EMG values measured from a user.

[0014] To accomplish the objects of the present disclosure, an exemplary embodiment of the present disclosure provides an apparatus for measuring movements of a user by using an electroencephalogram (EEG) sensor and an electromyogram (EMG) sensor, which may include: a sample pattern storing unit for storing one or more sample patterns which are obtained by patterning EEG waveforms and EMG values; a communication unit for receiving an EEG waveform and an EMG value of the user measured by the EEG and EMG sensors; a pattern normalizing unit for selecting sample patterns with the highest similarity to the received user's EEG waveform and EMG value among the stored sample patterns, and for normalizing the received EEG waveform and EMG value so that their amplitudes and periods coincide with those of the selected sample patterns; a movement estimating unit for estimating movement of the user by inputting the normalized EEG waveform and EMG value in an artificial neural network algorithm; and a movement determining unit for calculating the user's movement by applying each weight value of the EEG and EMG to each movement estimation value.

[0015] The apparatus may further include: a noise eliminating unit for eliminating noise for eye movement by applying the EEG waveform and EMG value, received from the EEG sensor and EMG sensor, to an independent component analysis algorithm; and a synchronization unit for synchronizing the normalized EEG waveform and the normalized EMG value by using a time difference between the EEG waveform and EMG value measured by the EEG sensor and EMG sensor.

[0016] The pattern normalizing unit may normalize the noise-eliminated EEG waveform and EMG value by using normalization ratios which are set with control ratios used for controlling the amplitudes and periods of the noise-eliminated EEG waveform and EMG value to coincide with those of the selected sample patterns or which are set by being externally inputted.

[0017] The movement estimating unit may estimate the user's movement by using the synchronized EEG waveform and EMG value at the current time, the synchronized EEG waveform and EMG value at time prior to the current time, and a movement estimation value outputted through the artificial neural network at time prior to the current time, as input values of the artificial neural network algorithm.

[0018] The sample pattern storing unit may pattern the normalized EEG waveform and EEG value, and a movement estimation value outputted from the artificial neural network algorithm, and may store them as one sample pattern.

[0019] The movement determining unit may set a movement estimation value depending on the EMG values to have the weight value larger than that of a movement estimation value depending on the EEG waveforms.

[0020] Another exemplary embodiment of the present disclosure provides a movement pattern measuring method using a movement pattern measuring apparatus, which may include: storing one or more sample patterns which are obtained by patterning EEG waveforms and EMG values; receiving an EEG waveform and an EMG value measured by an EEG sensor and an EMG sensor attached to a user; selecting sample patterns with the highest similarity to the received user's EEG waveform and EMG value among the stored sample patterns, and normalizing the received EEG waveform and EMG value so that their amplitudes and periods coincide with those of the selected sample patterns; estimating movement of the user by inputting the normalized EEG waveform and EMG value in an artificial neural network algorithm; and determining the user's movement by applying each weight value of the EEG and EMG to each movement estimation value.

[0021] According to the present disclosure, since the movement of the current user is estimated and determined with the measured EEG waveform and EMG value at the current time, the EEG waveform and EMG value measured at time prior to at the current time, and the movement estimation value at time prior to at the current time, more accurate movement determination becomes possible.

[0022] Further, the normalization for each person can be adequately performed by utilizing data measured from each person. Furthermore, by utilizing the EEG and EMG sensors together, the present disclosure can more accurately determine the user's movement even with a small number of sensors compared with conventional technologies. Accordingly, the cost of normalization for each person, and the cost of sensors can be reduced.

BRIEF DESCRIPTION OF THE DRAWINGS

[0023] FIG. 1 is a schematic view of a movement pattern measuring apparatus according to an exemplary embodiment of the present disclosure.

[0024] FIG. 2 is a flow chart illustrating a movement pattern measuring method according to the exemplary embodiment of the present disclosure.

[0025] FIG. 3 exemplarily illustrates scheme of an artificial neural network algorithm of the movement pattern measuring apparatus according to the exemplary embodiment of the present disclosure.

DETAILED DESCRIPTION OF THE INVENTION

[0026] The present invention will be described more fully hereinafter with reference to the accompanying drawings, in which exemplary embodiments of the invention are shown. As those skilled in the art would realize, the described embodiments may be modified in various different ways, all without departing from the spirit or scope of the present invention. The drawings and description are to be regarded

as illustrative in nature and not restrictive, and like reference numerals designate like elements throughout the specification.

[0027] In addition, unless explicitly described to the contrary, the word "comprise" and variations such as "comprises" or "comprising" will be understood to imply the inclusion of stated elements, but not the exclusion of any other elements.

[0028] The present disclosure relates to a movement pattern measuring apparatus using electroencephalogram (EEG) and electromyogram (EMG) data, and provides a method allowing a user's movement to be more accurately determined with EEG waveforms and EMG values measured by EEG and EMG sensors.

[0029] In an exemplary embodiment of the present disclosure, two EEG sensors and two EMG sensors are used. The two EEG sensors are placed on the frontal lobe, and the two EMG sensors are placed on specific body parts desired to be measured. The movement pattern measuring apparatus receives EEG and EMG data measured by the sensors attached to the user's body, eliminates noise from the received data by using an independent component analysis algorithm, normalizes the data, and then determines the user's movement through an artificial neural network algorithm. Since the determined movement value and measured data are stored and utilized again, normalization for each person is possible and the user's movement can be more accurately determined.

[0030] Hereinafter, the movement pattern measuring apparatus according to the exemplary embodiment of the present disclosure will be described in detail with reference to the accompanying drawings.

[0031] FIG. 1 is a schematic view of a movement pattern measuring apparatus according to an exemplary embodiment of the present disclosure.

[0032] The movement pattern measuring apparatus 100 includes a sample pattern storing unit 110, a communication unit 120, a pattern normalizing unit 130, and a movement estimating unit 140, and a movement determining unit 150. The movement pattern measuring apparatus 100 may further include a noise eliminating unit 160 and a synchronization unit 170.

[0033] The sample pattern storing unit 110 stores one or more sample patterns for electroencephalogram (EEG) waveforms and electromyogram (EMG) values. The sample pattern storing unit 110 has already stored a sample pattern which is obtained by patterning the amplitude of an EEG waveform, or an EMG value for a specific movement, but may further store another sample pattern which is obtained by patterning a newly measured EEG waveform or EMG value.

[0034] The communication unit 120 receives an EEG waveform and EMG value of a user, measured by an EEG sensor and an EMG sensor.

[0035] The communication unit 120 may receive the EEG waveform and the EMG value measured by the EEG sensor and the EMG sensor through a wired network or a wireless network. Examples of the wireless network are short-range communications including Zigbee, Bluetooth, NFC (near field communication), etc., and long-range communications including 3G, 4G, LTE, and LTE-A, but the present disclosure is not necessarily limited thereto.

[0036] The pattern normalizing unit 130 receives the EEG waveform and EMG value from the communication unit 120

or the noise eliminating unit **160**, selects sample patterns with the highest similarity to the received user's EEG waveform and EMG value among the stored sample patterns, and normalizes the received EEG waveform and EMG value so that their amplitudes and periods coincide with those of the selected sample patterns.

[0037] The movement estimating unit **140** estimates movement of the user by inputting the normalized EEG waveform and EMG value in an artificial neural network algorithm.

[0038] Here, the artificial neural network refers to the entire models of networks, in which artificial neurons or nodes, which form a network through connections between synapses, have problem-solving ability by varying the strength of connection between the synapses through learning. The process of estimating the user's movement using this artificial neural network will be described later in further detail.

[0039] The movement determining unit **150** calculates the user's movement by applying each weight value of the EEG and EMG to each movement estimation value.

[0040] The noise eliminating unit **160** eliminates noise for eye movement by applying the EEG waveform and EMG value, received from the EEG sensor and EMG sensor, to an independent component analysis algorithm. Here, the independent component analysis algorithm is a computational method for separating a multivariate signal into additive subcomponents. Particularly, the independent component analysis is a special case of blind signal separation.

[0041] The synchronization unit **170** synchronizes the normalized EEG waveform and the normalized EMG value by using a time difference between the received EEG waveform and EMG value.

[0042] When the user attempts a specific movement, a brain signal is first created, and the movement is performed in response to the created brain signal. That is, the EEG waveform is measured in advance of the EMG value. For this reason, the synchronization unit **170** first calculates the time difference between the received EEG waveform and EMG value, and synchronizes the time of the normalized EEG waveform and the normalized EMG value by using the calculated time difference so that both can represent the same movement.

[0043] Hereinafter, a method for measuring the user's movement using the movement pattern measuring apparatus according to the exemplary embodiment of the present disclosure is described in detail with reference to FIG. 2 and FIG. 3.

[0044] FIG. 2 is a flow chart illustrating a movement pattern measuring method according to the exemplary embodiment of the present disclosure, and FIG. 3 exemplarily illustrates scheme of an artificial neural network algorithm of the movement pattern measuring apparatus according to the exemplary embodiment of the present disclosure.

[0045] First, at step S210, the movement pattern measuring apparatus **100** stores one or more sample patterns which are obtained by patterning EEG waveforms and EMG values. The sample patterns refer to standard EEG waveforms and EMG values of the ordinary persons, and movements corresponding to those EEG waveforms and EMG values, all of which are previously recorded and stored.

[0046] In addition, in the case in which the user's movement has been determined with the EEG waveform and EMG value measured from the user, the movement pattern

measuring apparatus **100** may store another sample pattern obtained by patterning the EEG waveform and EMG value used for determining the user's movement, and the determined movement value.

[0047] Next, at step S220, the movement pattern measuring apparatus **100** receives an EEG waveform and an EMG value, each measured by the EEG sensor and EMG sensor which are attached to the user.

[0048] The movement pattern measuring apparatus **100** may receive EEG waveforms and EMG values in real time or at certain time intervals, communicating with the EEG sensor and EMG sensor.

[0049] The EEG sensor and EMG sensor are connected to the movement pattern measuring apparatus **100** by wires so that the measured EEG waveform and EMG value can be communicated thereto. However, they may be wirelessly connected to the movement pattern measuring apparatus **100**.

[0050] Examples of wireless network are short-range communications including Zigbee, Bluetooth, NFC (near field communication), etc., and long-range communications including 3G, 4G, LTE, and LTE-A, but the present disclosure is not necessarily limited thereto.

[0051] Next, at step S230, the movement pattern measuring apparatus **100** eliminates noise for eye movement by applying the EEG waveform and EMG value, received from the EEG sensor and EMG sensor, to an independent component analysis algorithm.

[0052] There is a higher possibility of generating noise and artifact in the EEG waveform and the EMG value measured by the EEG sensor and EMG sensor. In this case, to obtain an accurate measurement value, the noise and artifact should be removed. The movement pattern measuring apparatus **100** can eliminate EEG signals for the eye movement from the measured EEG waveforms by applying them to the independent component analysis algorithm. That is, the noise can be efficiently eliminated because the EEG signals are separated to be source signals which are maximally independent and minimally dependent by the independent component analysis algorithm.

[0053] In addition, the movement pattern measuring apparatus **100** may also eliminate any noise and artifact with no causal relationship to the user's movement as well as the noise for the eye movement. For example, in the case in which the user has tic disorder which may have an influence on the EEG waveform and the EMG value, the movement pattern measuring apparatus **100** can eliminate the corresponding noise and artifact from the measured EEG waveform and the EMG value.

[0054] Next, at step S240, the movement pattern measuring apparatus **100** selects sample patterns with the highest similarity to the EEG waveform and EMG value which the noise and artifact have been removed from, and normalizes the EEG waveform and EMG value so that their amplitudes and periods coincide with those of the selected sample patterns.

[0055] In detail, the movement pattern measuring apparatus **100** analyzes features of the received EEG waveform and EMG value, and selects two sample patterns which are determined to be most similar to the features of the received EEG waveform and EMG value. Since each person has a different EEG waveform and EMG value, to accurately determine the user's movement, the movement pattern measuring apparatus **100** normalizes the received EEG wave-

form and EMG value so that their amplitudes and periods coincide with those of the selected sample patterns.

[0056] In such a normalization process, the movement pattern measuring apparatus 100 stores control ratios in an additional storage device, and may use the stored control ratios when the EEG waveform and EMG value, which are measured after storing the normalization ratios, are normalized.

[0057] That is, the movement pattern measuring apparatus 100 may normalize the noise-eliminated EEG waveform and EMG value by using normalization ratios which are set with control ratios used for controlling the amplitudes and periods of the noise-eliminated EEG waveform and EMG value to coincide with those of the selected sample patterns or which are set by being externally inputted.

[0058] Here, the most frequently stored ratio of the stored ratios during N (N is a natural number) normalization processes are performed may be set as the normalization ratio by the movement pattern measuring apparatus 100. In the normalization process performed after the normalization ratio has been set, the set normalization ratio is first applied to this process, and if the ratio is inadequate, the amplitudes and periods of the EEG waveform and EMG value may be controlled again for the normalization.

[0059] Then, at step S250, the movement pattern measuring apparatus 100 synchronizes the normalized EEG waveform and the normalized EMG value by using the time difference between the measured EEG waveform and the EMG value.

[0060] Even if the movement pattern measuring apparatus 100 receives the EEG waveforms and EMG values from the EEG sensor and EMG sensor in real time or at certain time intervals, the EEG waveform and EMG value, both representing the same movement, are measured at different time points. Accordingly, the movement pattern measuring apparatus 100 synchronizes the EEG waveform and EMG value for the same movement by controlling the time difference therebetween based on either of them.

[0061] For example, in the case when the user to which the EEG and EMG sensors are attached attempts a specific movement, the movement pattern measuring apparatus 100 may calculate the time difference between a time point of creating an EEG waveform in response to a brain signal for the specific movement and a time point of creating an EMG value of moving muscles by the brain signal, or may receive the time difference from the user, and then synchronizes the two time points by using the calculated or received time difference.

[0062] Next, at step S260, the movement pattern measuring apparatus 100 estimates the user's movement by inputting the normalized EEG waveform and EMG value in the artificial neural network.

[0063] In addition, the movement pattern measuring apparatus 100 may estimate the user's movement by using the synchronized EEG waveform and EMG value at the current time, the synchronized EEG waveform and EMG value at time prior to the current time, and a movement estimation value outputted through the artificial neural network at time prior to the current time, as input values of the artificial neural network algorithm.

[0064] In FIG. 3, the artificial neural network algorithm is configured by an input layer, at least one intermediate hidden layer, and an output layer.

[0065] On the assumption that the user's movement is in a flow having the context, the movement pattern measuring apparatus 100 may use all of the sensor values synchronized at the current time and at time prior to the current time, and the movement estimation value outputted at time prior to the current time, as input values of the artificial neural network algorithm.

[0066] As described above, two EEG sensors and two EMG sensors are used in the present disclosure. Accordingly, values recorded by four sensors may be used as inputs of the artificial neural network algorithm.

[0067] As shown in FIG. 3, the movement pattern measuring apparatus 100 according to the exemplary embodiment of the present disclosure uses a three-layered model as a scheme of the artificial neural network algorithm. However, the present disclosure is not necessarily limited thereto. Each circular node represents an artificial neuron with problem-solving ability by varying the strength of connection between the synapses through learning.

[0068] In an example shown in FIG. 3, the input layer of the artificial neural network inputs twelve normalized sensor values, which are resulted from three normalization processes for the two EEG sensors and two EMG sensors at time prior to the current time, as previous determination values, measures the sensor values for a predetermined time (for example, 0.1 sec. based on 250 Hz), and inputs the synchronized sensor values. In the exemplary embodiment of the present disclosure, an intermediate value of the input nodes and output nodes is 58, but it is not necessarily limited thereto. The movement pattern measuring apparatus 100 forms enough nodes at the intermediate hidden layer, and outputs each movement estimation value for the respective four sensors.

[0069] When a new user to which the sensors are attached uses the movement pattern measuring apparatus 100 for the first time, the movement pattern measuring apparatus 100 may estimate the user's movement by using the nodes previously trained with the sample values. When the normalization of EEG waveform and EMG value has been completed and a predetermined amount of information about the corresponding user has been accumulated, the movement pattern measuring apparatus 100 trains the nodes with the previous determination values, and includes a recent determination value in the input in order to estimate the user's movement more accurately.

[0070] Next, at step S270, the movement pattern measuring apparatus 100 determines the user's movement by applying the weight values of EEG waveform and the EMG value to the estimated user's movement.

[0071] In detail, the movement pattern measuring apparatus 100 finally determines the user's movement by respectively applying the weight value of EEG waveform and the weight value of the EMG value to the movement estimation value depending on the EEG waveforms measured by two EEG sensors, and to the movement estimation value depending on the EMG values measured by two EMG sensors.

[0072] In this case, the movement estimation value depending on the EMG values may have the weight value larger than that of the movement estimation value depending on the EEG waveforms. This is why the EMG value measured from actually moving muscles has higher accuracy and comparatively less noise and artifact than the EEG signal for commanding the movement. For this reason, the

movement pattern measuring apparatus **100** may set the weight value of the EMG value to be larger than that of the EEG waveform.

[0073] As such, when the user's movement has been determined with the measured EEG waveforms and EMG values, the normalized EEG waveform or EEG value for the determined movement, and the movement estimation value outputted from the artificial neural network algorithm are patterned and stored as one sample pattern.

[0074] That is, the movement pattern measuring apparatus **100** stores the measured input value, estimated input value, and resultant value again as one sample pattern, and may utilize this sample pattern at the steps **S240** and **S260**.

[0075] According to the exemplary embodiment of the present disclosure, since the movement of the current user is estimated and determined with the measured EEG waveform and EMG value at the current time, the EEG waveform and EMG value measured at time prior to at the current time, and the movement estimation value at time prior to at the current time, more accurate movement determination becomes possible.

[0076] Further, the normalization for each person can be adequately performed by utilizing data measured from each person. Furthermore, by utilizing the EEG and EMG sensors together, the present disclosure can more accurately determine the user's movement even with a small number of sensors compared with conventional technologies. Accordingly, the cost of normalization for each person, and the cost of sensors can be reduced.

[0077] Example embodiments have been disclosed herein and although specific terms are employed, they are used and are to be interpreted in a generic and descriptive sense only and not for purpose of limitation. In some examples, as would be apparent to one of ordinary skill in the art as of the filing of the present application, features, characteristics and/or elements described in connection with a particular embodiment may be used singly or in combination with features, characteristics and/or elements described in connection with other embodiments unless otherwise specifically indicated. Accordingly, it will be understood by those of skill in the art that various changes in form and details may be made without departing from the spirit and scope of the present invention as set forth in the following claims.

What is claimed is:

1. An apparatus for measuring movements of a user by using an electroencephalogram (EEG) sensor and an electromyogram (EMG) sensor, which comprising:

a sample pattern storing unit for storing one or more sample patterns which are obtained by patterning EEG waveforms and EMG values;

a communication unit for receiving an EEG waveform and an EMG value of the user measured by the EEG and EMG sensors;

a pattern normalizing unit for selecting sample patterns with the highest similarity to the received user's EEG waveform and EMG value among the stored sample patterns, and for normalizing the received EEG waveform and EMG value so that their amplitudes and periods coincide with those of the selected sample patterns;

a movement estimating unit for estimating movement of the user by inputting the normalized EEG waveform and EMG value in an artificial neural network algorithm; and

a movement determining unit for determining the user's movement by applying each weight value of the EEG and EMG to each movement estimation value.

2. The apparatus of claim **1**, further comprising:

a noise eliminating unit for eliminating noise for eye movement by applying the EEG waveform and EMG value, received from the EEG sensor and EMG sensor, to an independent component analysis algorithm; and

a synchronization unit for synchronizing the normalized EEG waveform and the normalized EMG value with a time difference between the EEG waveform and EMG value measured by the EEG sensor and EMG sensor.

3. The apparatus of claim **2**, wherein the pattern normalizing unit normalizes the noise-eliminated EEG waveform and EMG value by using normalization ratios which are set with control ratios used for controlling the amplitudes and periods of the noise-eliminated EEG waveform and EMG value to coincide with those of the selected sample patterns or which are set by being externally inputted.

4. The apparatus of claim **3**, wherein the movement estimating unit estimates the user's movement by using the synchronized EEG waveform and EMG value at the current time, the synchronized EEG waveform and EMG value at time prior to the current time, and a movement estimation value outputted through the artificial neural network at time prior to the current time, as input values of the artificial neural network algorithm.

5. The apparatus of claim **4**, wherein the sample pattern storing unit patterns the normalized EEG waveform and EEG value, and a movement estimation value outputted from the artificial neural network algorithm, and then stores them as one sample pattern.

6. The apparatus of claim **1**, wherein the movement determining unit sets a movement estimation value depending on the EMG values to have the weight value larger than that of a movement estimation value depending on the EEG waveforms.

7. A movement pattern measuring method using a movement pattern measuring apparatus, comprising:

storing one or more sample patterns which are obtained by patterning EEG waveforms and EMG values;

receiving an EEG waveform and an EMG value measured by an EEG sensor and an EMG sensor attached to a user;

selecting sample patterns with the highest similarity to the received user's EEG waveform and EMG value among the stored sample patterns, and normalizing the received EEG waveform and EMG value so that their amplitudes and periods coincide with those of the selected sample patterns;

estimating movement of the user by inputting the normalized EEG waveform and EMG value in an artificial neural network algorithm; and

determining the user's movement by applying each weight value of the EEG and EMG to each movement estimation value.

8. The method of claim **7**, further comprising:

eliminating noise for eye movement by applying the EEG waveform and EMG value, received from the EEG sensor and EMG sensor, to an independent component analysis algorithm; and

synchronizing the normalized EEG waveform and the normalized EMG value by using a time difference

between the EEG waveform and EMG value measured by the EEG sensor and EMG sensor.

9. The method of claim 8, wherein the normalizing of the received EEG waveform and EMG value includes normalizing the noise-eliminated EEG waveform and EMG value by using normalization ratios which are set with control ratios used for controlling the amplitudes and periods of the noise-eliminated EEG waveform and EMG value to coincide with those of the selected sample patterns or which are set by being externally inputted.

10. The method of claim 9, wherein the estimating of the user's movement includes estimating the user's movement by using the synchronized EEG waveform and EMG value at the current time, the synchronized EEG waveform and EMG value at time prior to the current time, and a movement estimation value outputted through the artificial neural network at time prior to the current time, as input values of the artificial neural network algorithm.

11. The method of claim 10, wherein the storing of one or more sample patterns includes patterning the normalized EEG waveform and EEG value, and a movement estimation value outputted from the artificial neural network algorithm, and storing them as one sample pattern.

12. The method of claim 7, wherein the determining of the user's movement includes setting a movement estimation value depending on the EMG values to have the weight value larger than that of a movement estimation value depending on the EEG waveforms.

* * * * *

专利名称(译)	使用脑电图和心电图的运动模式测量设备及其方法		
公开(公告)号	US20170035313A1	公开(公告)日	2017-02-09
申请号	US15/219294	申请日	2016-07-26
当前申请(专利权)人(译)	崇实大学研究协会TECHNO- PARK		
[标]发明人	HONG JIMAN KANG GIWOOK		
发明人	HONG, JIMAN KANG, GIWOOK		
IPC分类号	A61B5/04 A61B5/00 A61B5/11 A61B5/0476 A61B5/0488		
CPC分类号	A61B5/04012 A61B5/0476 A61B5/7207 A61B5/1126 A61B5/7264 A61B5/0488 G16H50/20		
优先权	1020150109470 2015-08-03 KR		
其他公开文献	US10105105		
外部链接	Espacenet USPTO		

摘要(译)

公开了一种用于测量用户的运动的装置，其可以包括：采样模式存储单元，用于存储通过对EEG波形和EMG值进行图案化而获得的一个或多个采样模式；通信单元，用于接收由所述EEG和EMG传感器测量的所述用户的EEG波形和EMG值；模式正规化单元，用于从所存储的采样模式中选择与接收的用户模式具有最高相似性的采样模式，并且用于将接收的用户模式归一化，使得它们的振幅和周期与所选择的采样模式的振幅和周期一致；运动估计单元，用于通过在人工神经网络算法中输入归一化的EEG波形和EMG值来估计用户的运动；以及运动确定单元，用于通过将EEG和EMG的每个加权值应用于每个运动估计值来计算用户的运动。

