



US 20190021597A1

(19) **United States**

(12) **Patent Application Publication**

**Nagy et al.**

(10) **Pub. No.: US 2019/0021597 A1**

(43) **Pub. Date: Jan. 24, 2019**

(54) **PHYSIOLOGICAL MONITORING SYSTEM**

(71) Applicant: **Endotronix, Inc.**, Lisle, IL (US)

(72) Inventors: **Michael Nagy**, Lombard, IL (US);  
**Harry Rowland**, Plainfield, IL (US);  
**Ariel Johnson**, Chicago, IL (US); **Brett Quas**, Pewaukee, WI (US)

(21) Appl. No.: **16/040,034**

(22) Filed: **Jul. 19, 2018**

**Related U.S. Application Data**

(60) Provisional application No. 62/534,261, filed on Jul. 19, 2017.

**Publication Classification**


(51) **Int. Cl.**  
*A61B 5/00* (2006.01)  
*A61B 5/1455* (2006.01)  
*G16H 10/60* (2006.01)


(52) **U.S. Cl.**

CPC ..... *A61B 5/0022* (2013.01); *A61B 5/0006* (2013.01); *A61B 5/021* (2013.01); *G16H 10/60* (2018.01); *A61B 5/0031* (2013.01); *A61B 5/1455* (2013.01)

(57) **ABSTRACT**

Disclosed is a physiologic monitoring system comprising a central hub in communication with a management portal for communicating physiologic measurements taken from a plurality of peripheral devices on a patient. At least one non-invasive peripheral device may measure physiologic data from a patient and be in communication with said central hub. A system including an invasive peripheral device may be associated with said patient and be in communication with said central hub. The central hub may be scalable to collect and communicate measurements from the non-invasive peripheral device and the invasive peripheral device. The at least one non-invasive peripheral device may include a blood pressure cuff, an oxygen sensor, a weight scale, and an ECG monitor. The invasive peripheral device may include a wireless sensor reader that may be adapted to measure physiologic data from a sensor implant placed within the cardiovascular system of said patient.

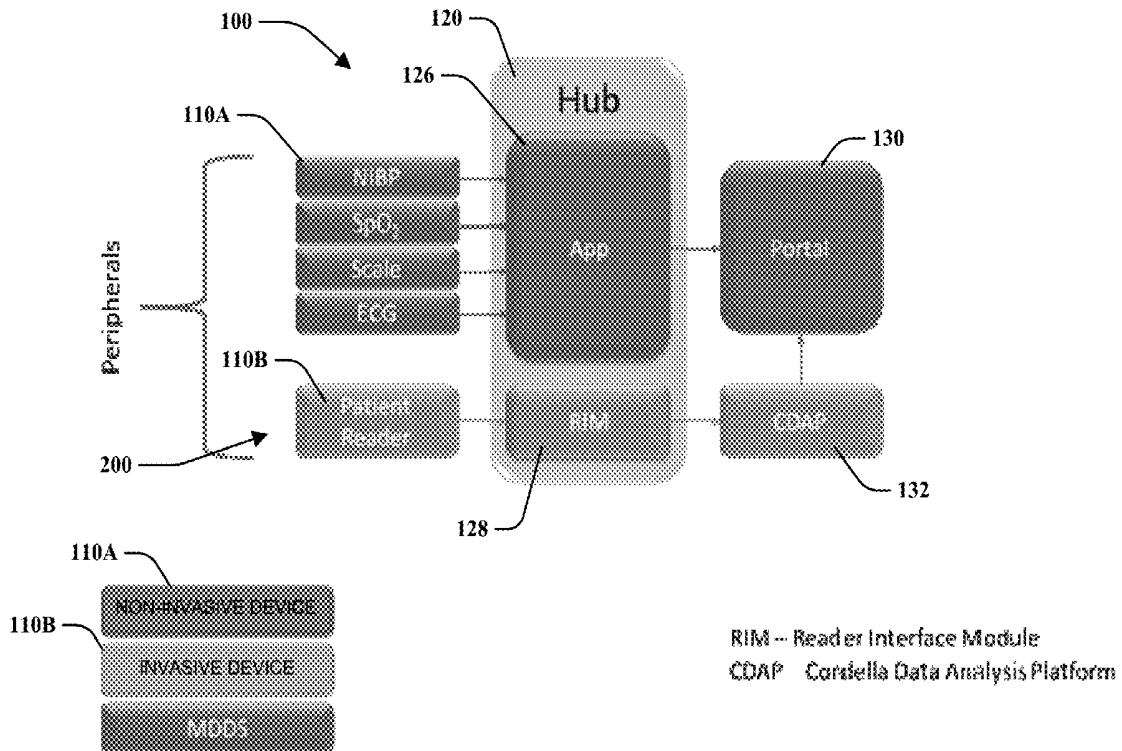

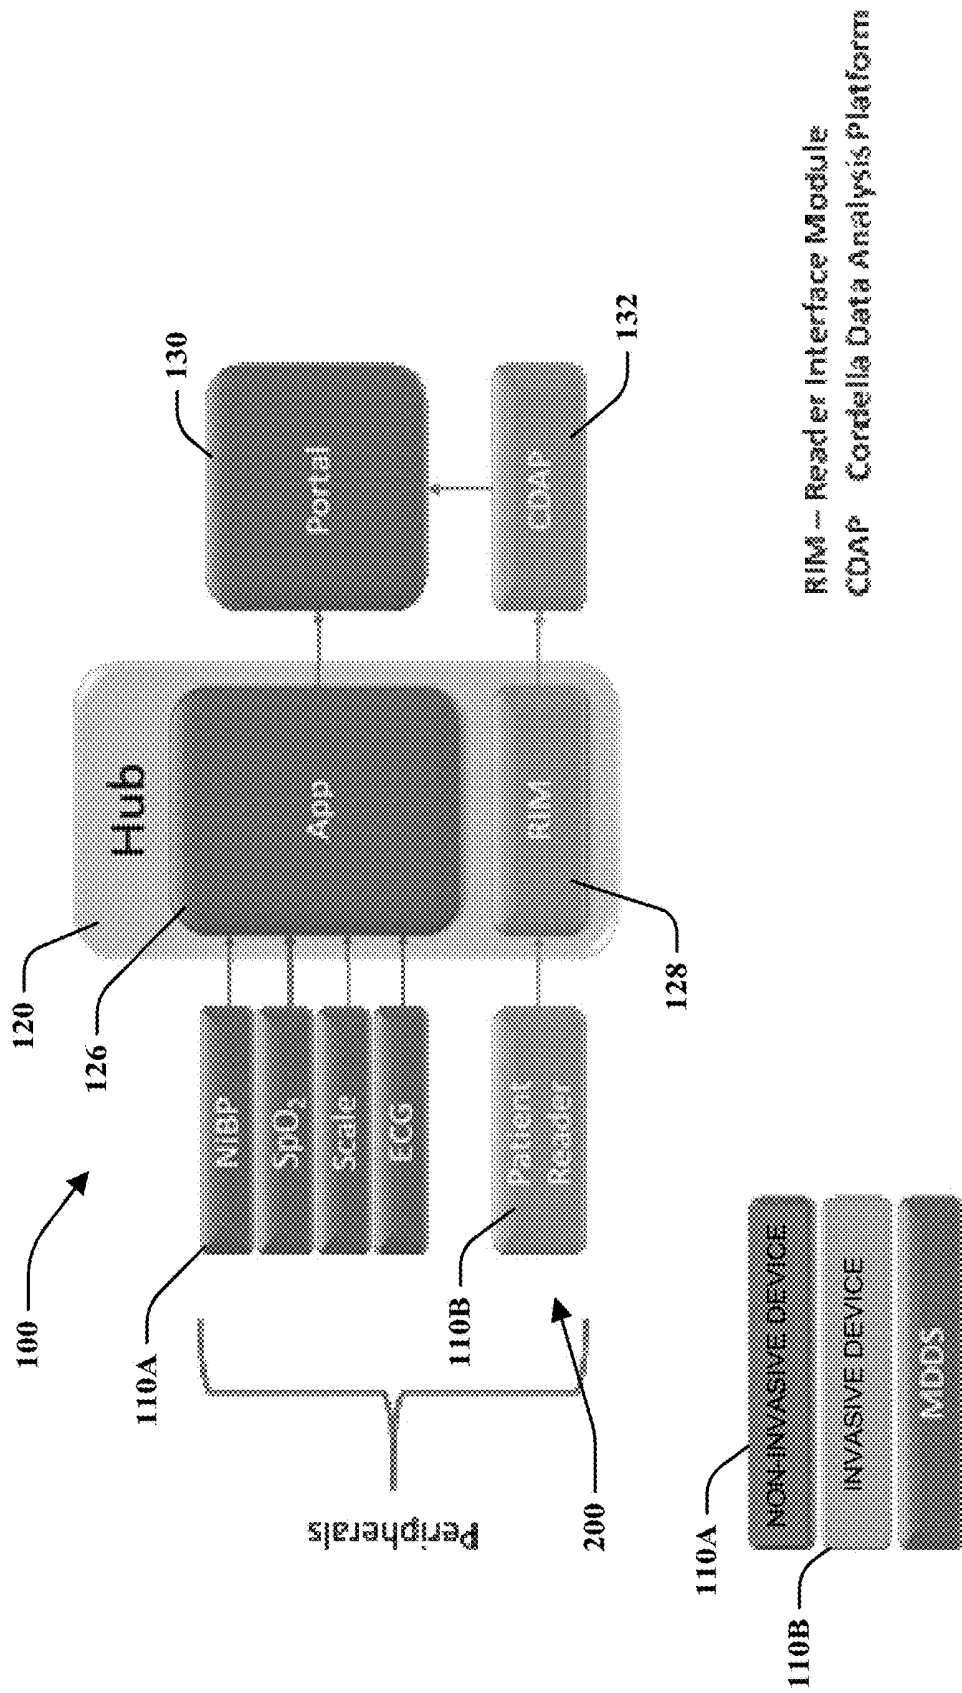

RIM --- Reader Interface Module  
 CDAP --- Cordella Data Analysis Platform

**FIG. 1**

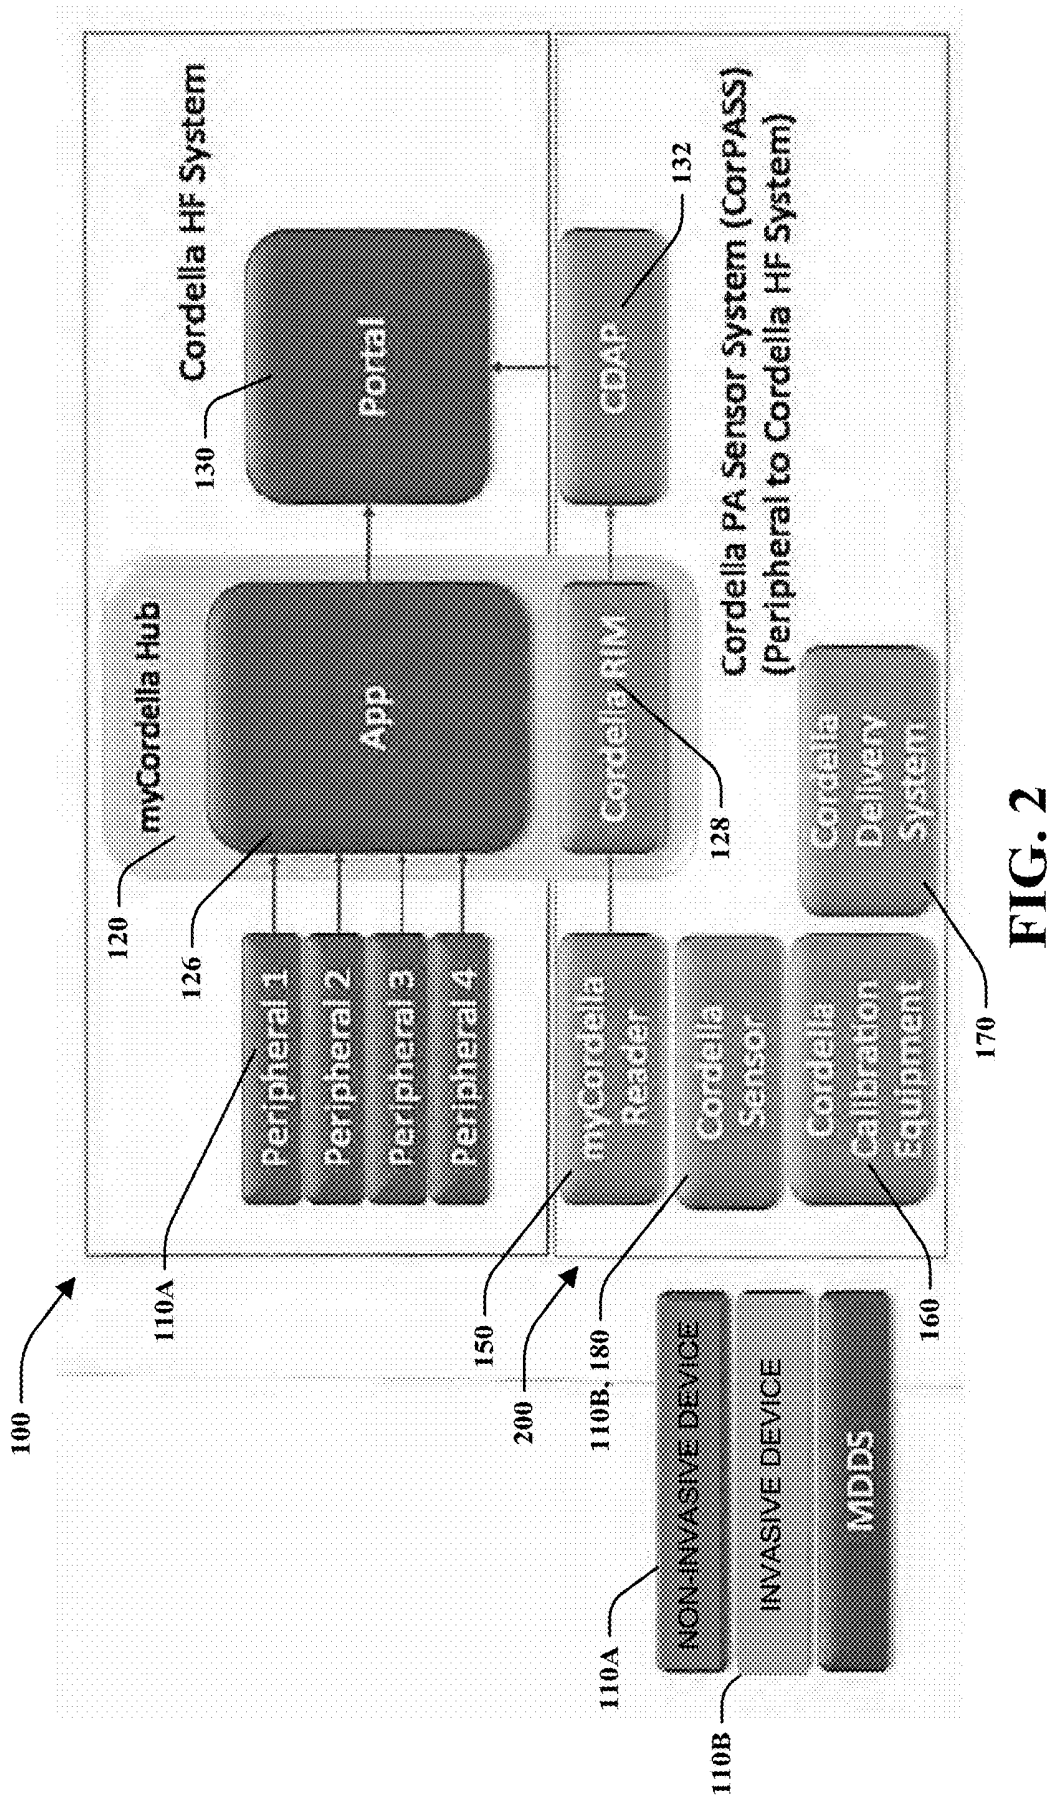


FIG. 2



FIG. 4

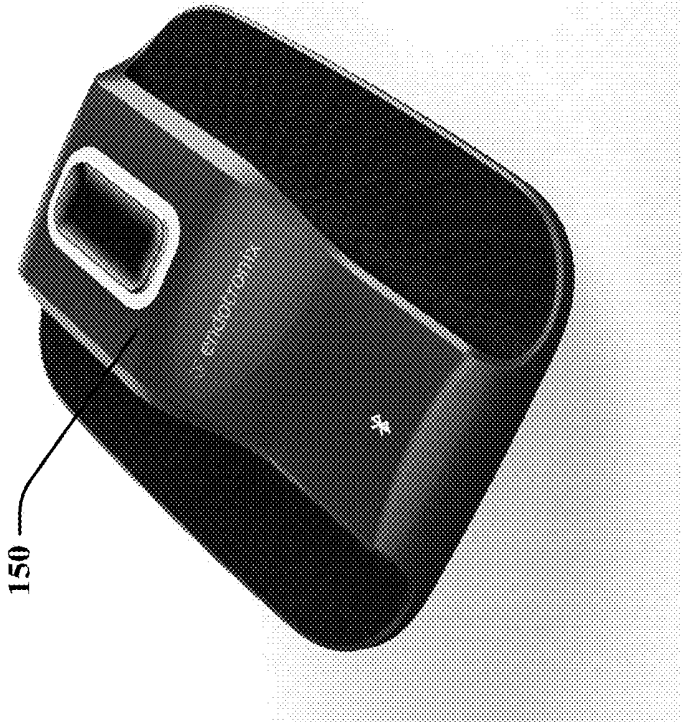
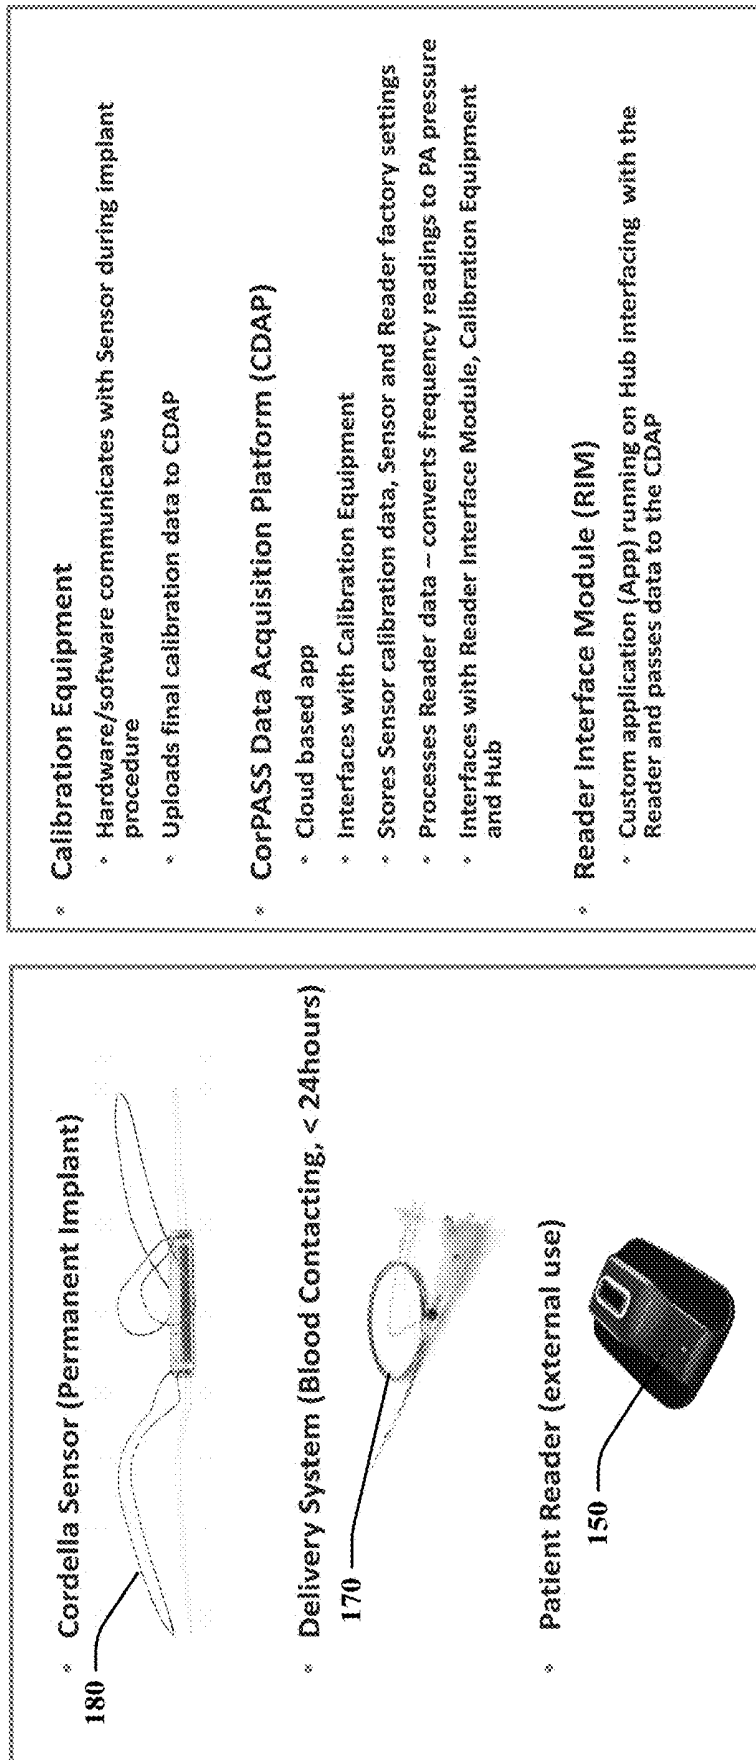


FIG. 3



**FIG. 5**

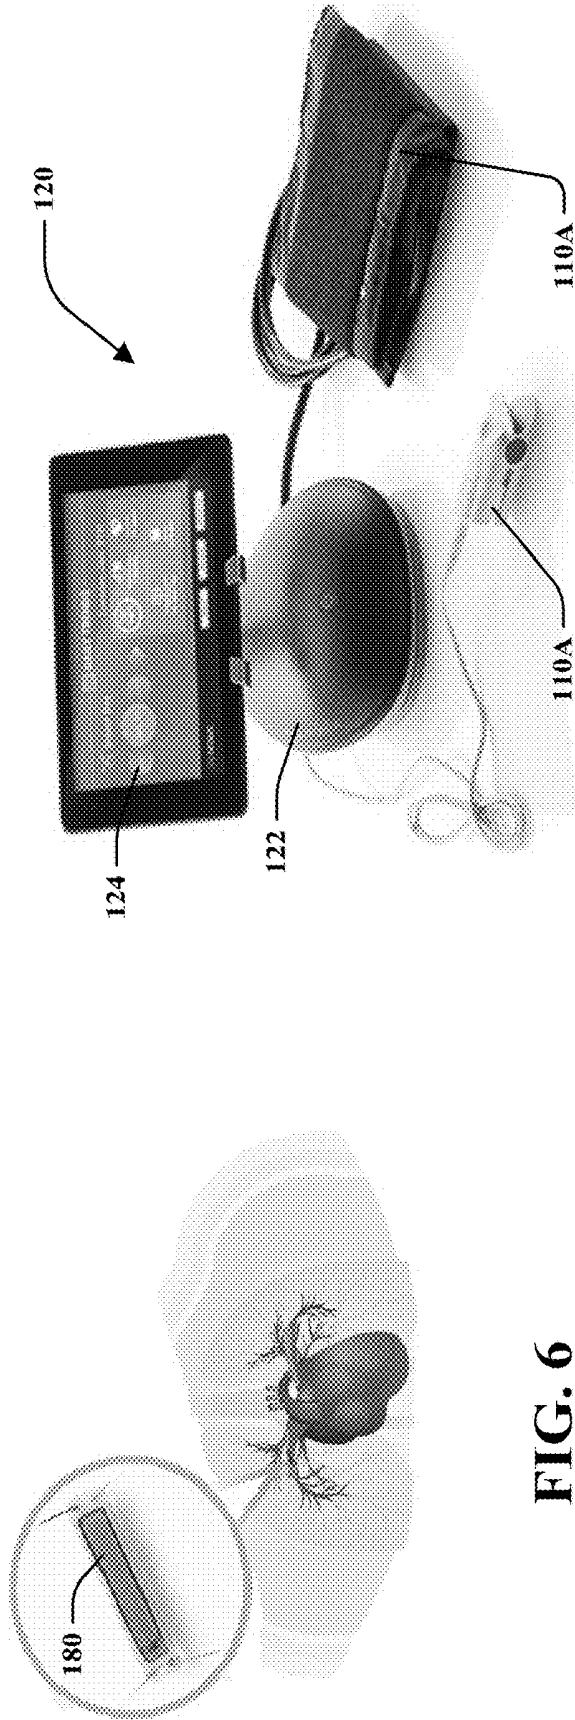


FIG. 6

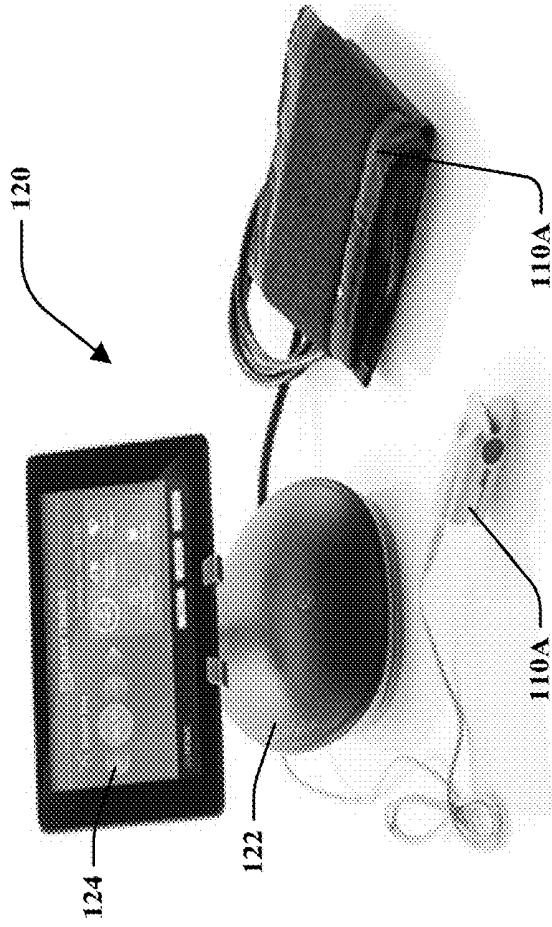


FIG. 7

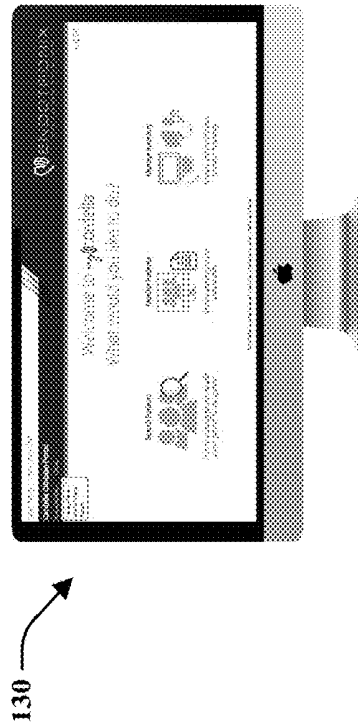


FIG. 8

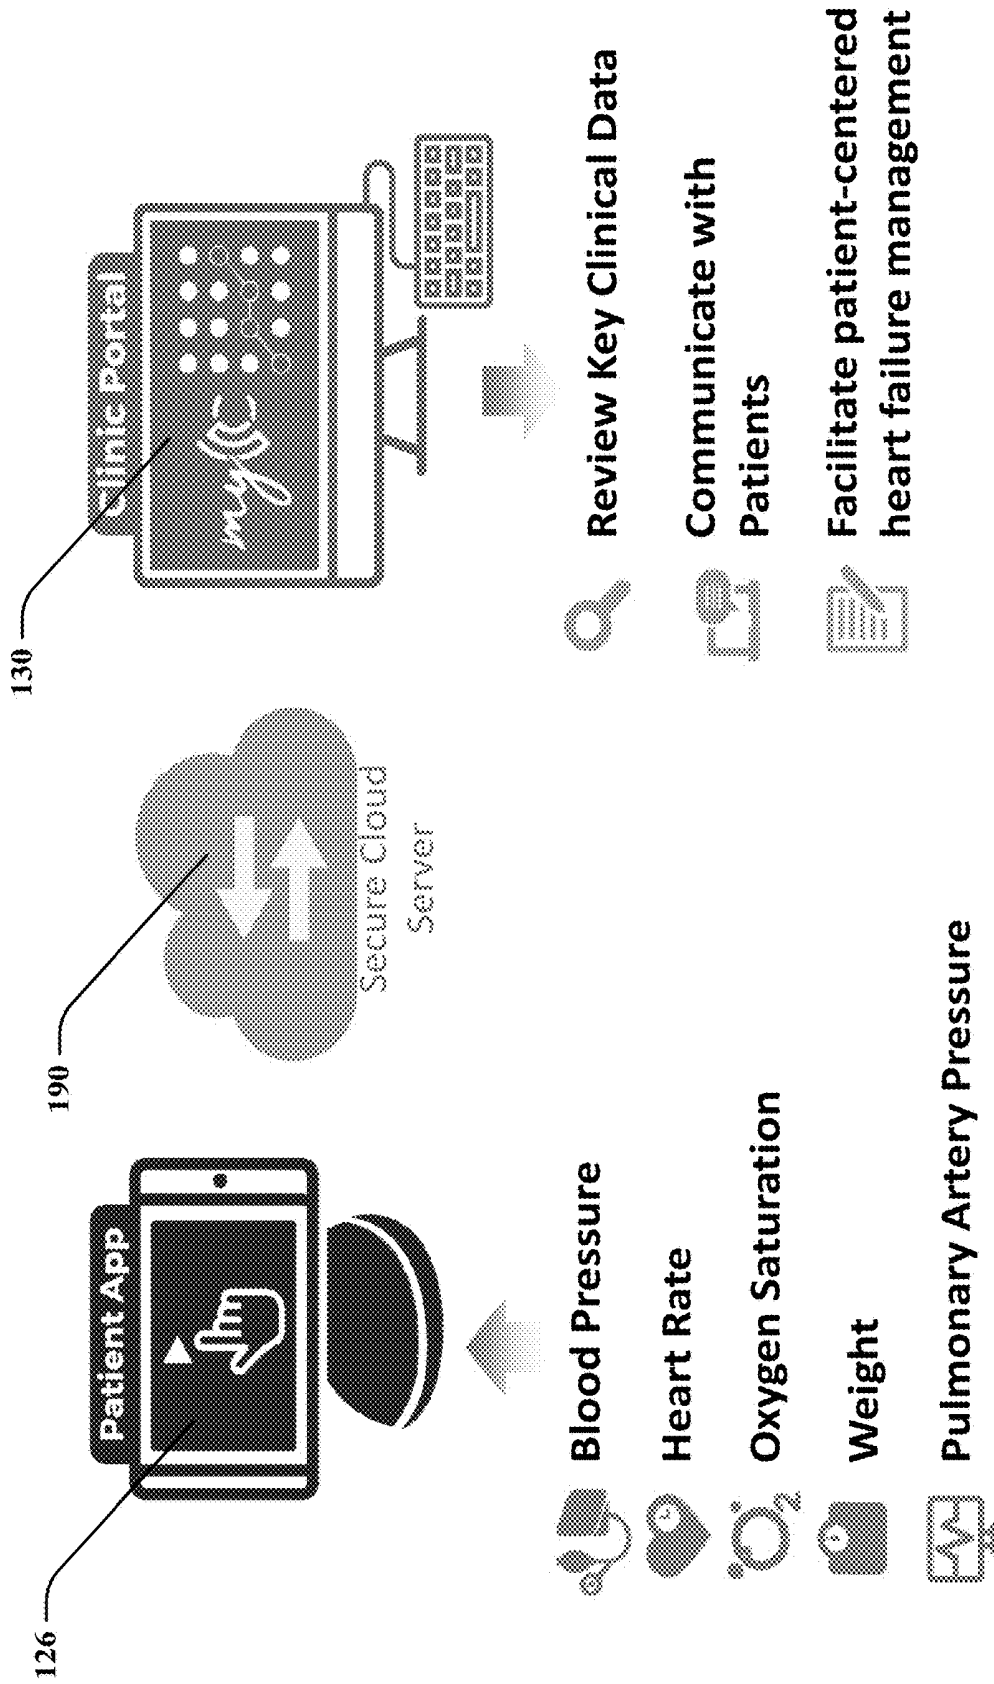


FIG. 9

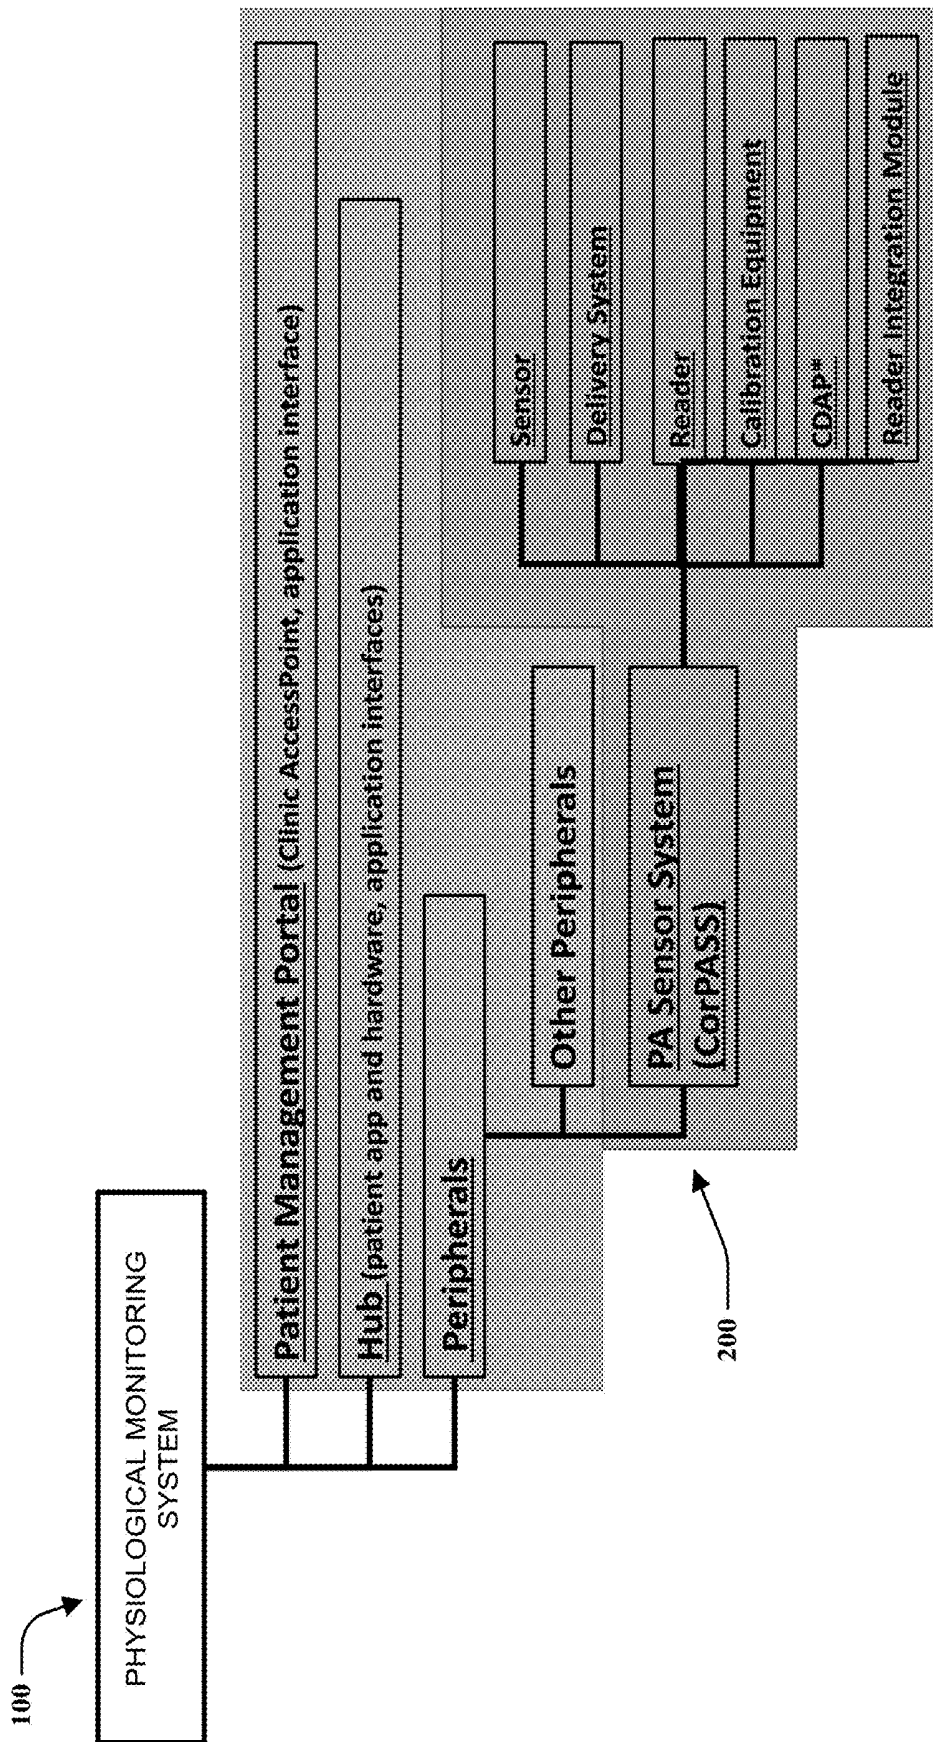


FIG. 10

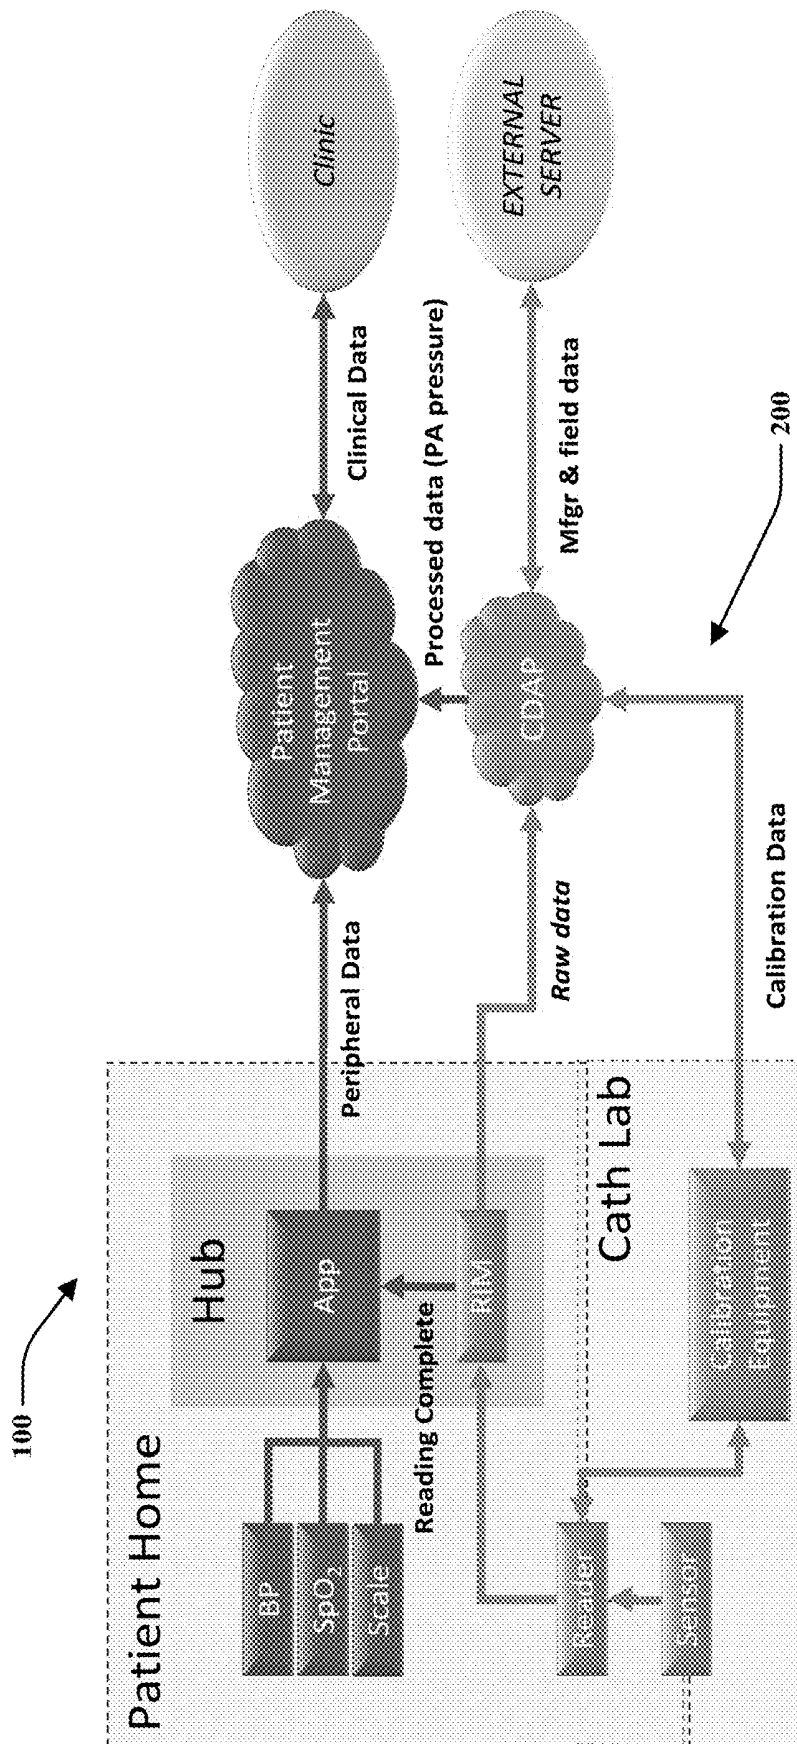


FIG. 11

## PHYSIOLOGICAL MONITORING SYSTEM

### CROSS REFERENCE TO RELATED APPLICATIONS

[0001] This application claims priority to U.S. Provisional Patent Application Ser No. 62/534,261 filed on Jul. 19, 2017, which is incorporated by reference herein.

### TECHNICAL FIELD

[0002] This invention relates generally to a physiological monitoring system for measuring, communicating, tracking, and recording various physiologic data from a patient.

### BACKGROUND

[0003] A conventional healthcare delivery system may include a clinician or care management team such as doctors, nurses, physician assistants, etc. that interacts with an integrated information system such as a computer system running various data management programs. The information system may be populated with patient data in an electronic medical record database. Within this healthcare delivery context, a significant problem exists in that while the patient may be fully monitored while being treated by the care management team, once the patient progresses from in-patient to out-patient, healthcare delivery is often reduced in quality because of lack of adequate monitoring of the patient. Furthermore, the clinician may comprise a number of unrelated healthcare professionals that may not communicate with each other or the hospital. This disconnected nature of the system may result in patients receiving improper care.

[0004] Various systems have been created in an attempt to solve these issues. In particular, various computer implemented methods have been adapted to improve communication to bridge the gap between clinicians and monitoring of patient physiologic data. Commonly, bedside physiological monitoring systems are implemented at hospitals to constantly monitor patients during their stay. Many of these methods incorporate computer systems to monitor physiologic data taken from peripheral devices that may be categorized as non-invasive such as blood pressure cuffs, oxygen sensors or weight scales. Some of these devices are even available in the home of the patient. However, these methods and systems are not capable of interacting with peripheral devices that include more invasive monitoring techniques, such as implants.

[0005] In the United States, the U.S. Food and Drug Administration (FDA) regulates the commercialization of medical devices and systems. The FDA classifies medical devices based on the risks associated with the device. As such, devices and systems are classified into one of three categories—Class I, Class II, and Class III. Class I devices are deemed to be low risk and are therefore subject to the least regulatory controls. For example, a weight scale is classified as Class I device. Class II devices are higher risk devices than Class I and require greater regulatory controls to provide reasonable assurance of the device's safety and effectiveness. For example, noninvasive blood pressure measurement systems are Class II devices. A noninvasive blood pressure measurement system is identified by the FDA as a device that provides a signal from which systolic, diastolic, mean, or any combination of the three pressures can be derived through the use of transducers placed on the

surface of the body. Class III devices are generally the highest risk devices and are therefore subject to the highest level of regulatory control. Class III devices must typically be approved by FDA before they are free to be commercialized. For example, replacement heart valves and implantable pacemaker pulse generators are classified as Class III devices.

[0006] Thus, there is a need to provide an improved system for managing and monitoring physiological measurements from both non-invasive peripheral devices as well as invasive types of peripheral devices. Additionally, there is also a need to be able to provide this system at the residence of the patient or a more mobile system for use by patients outside of a hospital or clinic. Further, there is a need to provide a method of care for chronic end stage diseases that incorporates a system of various components to streamline communication and ease of implementation.

### BRIEF DESCRIPTION OF THE DRAWINGS

[0007] Objects and advantages together with the operation of the invention may be better understood by reference to the following detailed description taken in connection with the following illustrations, wherein:

[0008] FIG. 1 illustrates a block diagram of an embodiment of a physiological monitoring system in accordance with the instant disclosure;

[0009] FIG. 2 illustrates a block diagram of another embodiment of a physiological monitoring system in accordance with the instant disclosure;

[0010] FIG. 3 illustrates an embodiment of a reader device that may be a peripheral device to the physiological monitoring system of the instant disclosure;

[0011] FIG. 4 illustrates an embodiment of a docking station for the reader device that may be a peripheral device to the physiological monitoring system of the instant disclosure;

[0012] FIG. 5 illustrates an implant that may be implanted in a cardiovascular system of a patient which may be a peripheral device to the physiological monitoring system of the instant disclosure;

[0013] FIG. 6 illustrates a hub, a graphical user interface, a cuff, and an oxygen sensor of the physiological monitoring system;

[0014] FIG. 7 illustrates a portal of the physiological monitoring system;

[0015] FIG. 8 illustrates a diagram including peripheral devices of the physiological monitoring system;

[0016] FIG. 9 illustrates a diagram of the function of the physiological monitoring system;

[0017] FIG. 10 illustrates a diagram of the physiologic monitoring system of the instant application; and

[0018] FIG. 11 illustrates a schematic flow chart illustrating features of the physiologic monitoring system of the instant application.

### SUMMARY

[0019] Disclosed is a physiologic monitoring system comprising a central hub in communication with a management portal. At least one non-invasive peripheral device may measure physiologic data from a patient in communication with said central hub and an invasive peripheral system associated with said patient may be in communication with said central hub. The central hub may be scalable to collect

data and communicate with the non-invasive peripheral device and the invasive peripheral system such that data from the non-invasive peripheral device and the invasive peripheral system are selectively communicated to the management portal. The at least one non-invasive peripheral device may include a blood pressure cuff, an oxygen sensor, a weight scale, and an ECG monitor. The invasive peripheral system may include an invasive peripheral device, wherein said invasive peripheral device includes at least one of an implantable sensor an actuator, a dialysis assembly, a drug delivery device, an infusion pump, a neuro-stimulation assembly, an oxygen delivery system, or a ventricular assistance device. A wireless sensor reader and a docking station may be part of the invasive peripheral system wherein the wireless sensor reader may be adapted to measure physiologic data from an implantable sensor placed within a cardiovascular system of said patient. The central hub may include a graphical user interface for displaying a patient application. The central hub may include a reader interface module in communication with the invasive peripheral system. The management portal may be in communication with a data analysis platform that is configured to receive data from the reader interface module, analyze the received data to generate processed data and communicate the processed data to the management portal.

**[0020]** In another embodiment, provided is a method of monitoring physiologic data comprising the step of measuring physiologic data from a patient with at least one non-invasive peripheral device. The step of measuring physiologic data from said patient with a system that includes an invasive peripheral device. The step of communicating said physiologic data to a central hub; and the step of communicating said physiologic data to a management portal to display to a clinical specialist. A plurality of health-related questions may be generated by the central hub to be answered by the patient and communicated to the management hub for display to the clinical specialist. The physiologic data may be aggregated and displayed by the central hub. The physiologic data may be aggregated and displayed at the management portal. The non-invasive peripheral device may include at least one of a blood pressure cuff, an oxygen sensor, a weight scale, and an ECG monitor. The invasive peripheral device may include at least one of an implantable sensor, an actuator, a dialysis assembly, a drug delivery device, an infusion pump, a neuro-stimulation assembly, an oxygen delivery system, or a ventricular assistance device. The implantable sensor and a wireless sensor reader may communicate to measure physiologic data from said implantable sensor placed within a cardiovascular system of said patient. Physiologic data measured from a patient with at least one non invasive peripheral device may be communicated to the management portal to display to said clinical specialist, wherein said clinical specialist analyzes said communicated physiologic data to prescribe an invasive peripheral device for use by said patient. The measured physiologic data may be communicated to a reader interface module of the central hub from the invasive peripheral device. The measured physiologic data from said invasive peripheral device may be communicated to a data analysis platform from the reader interface module wherein said data analysis platform analyzes said measured physiologic data and generates processed data wherein said processed data is communicated to the management portal.

**[0021]** In another embodiment, provided is a physiologic monitoring system comprising a central hub in communication with a management portal, said central hub includes a reader interface module and a graphical user interface for displaying a patient application. At least one non-invasive peripheral device to measure physiologic data from a patient in communication with said central hub. A peripheral system that includes an invasive peripheral device to measure physiologic data from said patient in communication with said central hub, the peripheral system is in communication with said reader interface module. The central hub is scalable to collect and communicate measurements from the non-invasive peripheral device and the invasive peripheral device. The management portal may be in communication with a data analysis platform configured to receive data from said reader interface module and display said data at the management portal. The at least one non-invasive peripheral device includes a blood pressure cuff, an oxygen sensor, a weight scale, and an ECG monitor. The invasive peripheral device includes an implantable sensor. The data analysis platform may be configured to interface with the peripheral system and the invasive peripheral device to calibrate said invasive peripheral device.

**[0022]** In another embodiment, provided is a method of monitoring physiologic data comprising measuring physiologic data from a patient with at least one non invasive peripheral device. Physiologic data is communicated to a central hub, said central hub includes a reader interface module. Physiologic data is communicated to a management portal to display to a specialist clinician. The communicated physiologic data is analyzed to prescribe a system that includes an invasive peripheral device for use by the patient. Physiologic data may be measured from said patient with said system that includes said invasive peripheral device. Physiologic data may be communicated to said reader interface module of said central hub. Physiologic data may be communicated to said management portal to display to a clinician specialist. The physiologic data may be aggregated and displayed at the management portal. The non-invasive peripheral device includes at least one of a blood pressure cuff, an oxygen sensor, a weight scale, and an ECG monitor. The invasive peripheral device includes at least one of an implantable sensor, an actuator, a dialysis assembly, a drug delivery device, an infusion pump, a neuro-stimulation assembly, an oxygen delivery system, or a ventricular assistance device.

#### DETAILED DESCRIPTION

**[0023]** Reference will now be made in detail to exemplary embodiments of the present invention, examples of which are illustrated in the accompanying drawings. It is to be understood that other embodiments may be utilized and structural and functional changes may be made without departing from the respective scope of the present invention.

**[0024]** The disclosed physiological monitoring system **100** collects, records, and transmits physiologic data from the patient to clinician(s) for assessment, patient communication, and patient-centered heart health management. The physiologic monitoring system includes the ability to monitor blood pressure, heart rate, blood oxygen, weight and responses to heart failure guideline-directed health assessment questions while the patient may be located remotely from the clinician. The monitoring system may be adapted for use with various peripheral devices for physiological

measurements such as a blood pressure cuff, a pulse oximetry sensor, and a weight scale while also being adapted for use with a system that incorporates an invasive peripheral device. In one embodiment, an invasive system may be referred to herein as the Cordella™ Pulmonary Artery Sensing System (CorPASS) **200**. The CorPASS **200** is a system that is designed to measure pulmonary artery blood pressure from an implant sensor placed within the cardiovascular system of a patient. In other embodiments, an invasive system may include an invasive peripheral device such as an implantable sensor, an actuator, a dialysis assembly, a drug delivery device, an infusion pump, a neurostimulation assembly, an oxygen delivery system, or a ventricular assistance device.

[0025] It is a focus of the instant disclosure to provide monitoring of end stage diseases and allow a clinical specialist in the related field of such end stage disease to oversee that monitoring. End stage diseases may include diseases that have no known cure such as heart failure and kidney failure as well as certain types of cancers. The system and method of the instant disclosure focuses to provide permanent chronic care for end stage diseases wherein such care is provided by clinical specialists in the field such as a cardiologist, nephrologist, or even an oncologist and related staff members with authorization. Further, it is also a focus of the instant disclosure to provide such care in a way that optimizes the interaction between the clinical specialists (or staff member overseen by the clinical specialist in the field) by specifically tailoring a management portal to the clinical workflow of the clinical specialists.

[0026] As illustrated by FIGS. **1** and **2**, the monitoring system **100** includes a plurality of peripheral devices **110A**, **110B**, a central hub **120**, and a management portal **130**. The peripheral devices may include non-invasive devices **110A** and invasive devices **110B** as will be discussed more fully herein. The monitoring system **100** allows a user to collect data from a patient via the peripherals **110A**, **110B** and then transmit the data from the central hub **120** to the management portal **130** through a communication network. The system **100** may include a central database may record the data and allow for retrospective review of patient physiological functions.

[0027] It is noted that user equipment devices including the central hub **120**, management portal **130** and the peripheral devices **110A**, **110B** can communicate with each other and with other elements via a network, for instance, a wireless network, or a wireline network. A “network” can include broadband wide-area networks such as cellular networks, local-area networks, wireless local-area networks (e.g., Wi-Fi), and personal area networks, such as near-field communication networks including BLUETOOTH®. Communication across a network may include packet-based communications, radio and frequency/amplitude modulations networks, and the like. In those embodiments in which it is hardwired, any appropriate kind or type of networking cables may be utilized. For example, USB cables, dedicated wires, coaxial cables, optical fiber cables, twisted pair cables, Ethernet, HDMI and the like.

[0028] The peripheral devices **110A**, **110B** may be adapted to collect various vital signals from a patient and communicate these signals to the central hub **120**. The peripheral devices may include non-invasive peripheral devices **110A**. These non-invasive peripheral devices **110A** may include a non-invasive blood pressure monitor (NiBP), a blood oxy-

gen saturation level monitor (SpO<sub>2</sub>), a weight scale (Scale), an electrocardiogram monitor (ECG) or other patient device for measuring vital signs such as, for example, glucose levels. Additionally, an invasive peripheral device **110B** may also be adapted to communicate with the central hub **120** in a particular manner. An example of an invasive peripheral device **110B** includes an implantable sensor surgically positioned within the body of a patient and its associated components to take readings from the implantable sensor, however this application is not limited to just one type of invasive peripheral system and device and the system may be scalable to include various types of invasive devices.

[0029] The CorPASS system **200** is an example of an invasive peripheral system that incorporates an invasive peripheral device **110B**. As illustrated by FIGS. **3-6**, the CorPASS system **200** may include an implant sensor **180**, a delivery system **170**, a reader **150**, and a docking station (calibration equipment) **160**. The wireless sensor reader **150** includes various features and may take readings of the implant sensor **180** within the cardiovascular system of a patient.

[0030] Current designs for wireless sensor readers that communicate with invasive sensors, are disclosed in U.S. Provisional Patent Application No. 62/463,203 filed on Feb. 24, 2017, U.S. Pat. No. 8,154,389 filed on Apr. 7, 2008, U.S. Pat. No. 8,432,265 filed on Mar. 19, 2012, U.S. Pat. No. 8,493,187 filed on Mar. 19, 2010, and U.S. Pat. No. 8,570,186 filed on Apr. 25, 2012, U.S. patent application Ser. No. 14/842,973 filed on Sep. 2, 2015, and U.S. patent application Ser. No. 15/213,712 filed on Jul. 19, 2016, each of which are incorporated by reference in their entireties herein. These patents disclose systems configured to communicate wirelessly with an implant and obtain a reading.

[0031] The implant sensor **180** may take pulmonary artery pressure measurements and communicate them to the wireless sensor reader **150**. Examples of an implant sensor **180** are disclosed in U.S. patent application Ser. No. 15/213,712 filed Jul. 19, 2016 and its related family of patents, each of which are incorporated by reference in their entireties. Delivery systems **170** for implanting the sensor into a patient are disclosed in PCT Patent Application No. PCT/US2011/45583 titled PRESSURE SENSOR, CENTERING ANCHOR, DELIVERY SYSTEM AND METHOD, which is also incorporated by reference in its entirety herein. A docking station **160** may receive and communicate with the reader **150** as well as charge and calibrate the reader **150**. The docking station **160** may be an example of calibration equipment comprising hardware and software that communicates with the sensor during an implant procedure. An example of a docking station **160** is disclosed in U.S. patent application Ser. No. 14/842,973, which is incorporated by reference in its entirety herein. The CorPASS system **200** may be useful in assisting diagnosis and treatment of many diseases. For the purposes of clarity, the peripheral device **110B** of the CorPASS system may be either the reader **150** or the docking station **160** as either device may be configured to communicate with the central hub **120**.

[0032] End stage diseases may have various categories or stages based on the severity of the disease. For example, the New York Heart Association (NYHA) classifies heart failure between class I through class IV depending upon severity. Further, kidney failure is also classified to be between stage 1 and stage 5 depending upon severity. Thus, it may be particularly relevant for early class or early stage patients

that utilize the monitoring system 100 with only having non-invasive peripheral devices 110A during such early class or early stages of end stage diseases to assist the clinical specialists to identify if the patient is a candidate for receiving care that utilizes a system that incorporates an invasive peripheral system and device 110B for monitoring or otherwise actuating or dispensing medical care. In such a scenario, it is contemplated that the monitoring system 100 may provide physiological data from non-invasive peripheral devices 110A such that the clinician may analyze the data to diagnose the existence that late stage, late class, or chronic end stage disease may be occurring in a patient wherein invasive steps are necessary for providing appropriate further care. Notification of such a progression from early stage/early class to late stage/late class may occur over time while a patient has been utilizing the monitoring system 100 without use of an invasive peripheral device 110B wherein as the patient has been prescribed use of such an invasive peripheral device 110B, the monitoring system 100 provides for seamless integration with both the non-invasive and invasive peripheral devices 110A, 110B such that an improvement in appropriate care may be provided. This seamless integration of the monitoring system 100 allows for monitoring of physiologic data as well as efficiently accepting, processing, and transferring data from all devices 110A, 110B.

[0033] FIG. 7 illustrates an embodiment of the central hub 120 and various non-invasive peripheral devices 110A including a non-invasive blood pressure monitor (NIBP) and a blood oxygen saturation level monitor (SpO<sub>2</sub>). The central hub 120 may include a base 122 and a graphical user interface 124. The base 122 may include various ports for selective attachment to the peripherals and the graphical user interface 124. The base 122 may include at least one input or switch to toggle power to or various modes of the system 100. The graphical user interface 124 may be on a patient facing monitor that displays a program identified herein as a patient application 126 (FIGS. 1 and 2). Alternatively, the central hub 120 may be a tablet, cell phone, laptop, or other computing device. The patient application 126 may be stored in a computer readable medium or database or be a web based application accessible through the central hub 120. The patient application 126 may be an interactive program that prompts a patient to provide answers to various questions that may be material to a clinical diagnosis. The patient application 126 may be a standalone program that is adapted to remind the patient to obtain physiologic measurements and respond to health-related questions. Further, the patient application 126 may include instructions to the patient to identify how to properly use the peripheral devices and how to collect measurements representative of biometric or physiologic data. Once measurements have been taken, the patient application 126 may aggregate the collected data and may analyze that data to determine a status of the patient's health. Alternatively, the patient application 126 may aggregate the collected data and send it to the clinical portal 130 or another database where analysis of the data may take place to determine a status of the patient's health, such as a database designed for artificial intelligence or machine learning. Alternatively, the patient application 126 may aggregate the collected data and send it to the clinical portal 130 or another database where analysis of the data may take place by a clinician or other medical care provider to determine a status of the patient's health. The patient

application 126 may receive various types of data from an external database to display to the patient. The patient application 126 may generate or display a summary or snapshot of the patient's health status and related data or messages that may be displayed on the graphical user interface 124. The collected physiologic data and patient's health status information may be communicated to the management portal 130. The central hub 120 may be particularly located at a patient's residence or be remotely located from a clinician's office or hospital.

[0034] The central hub 120 may also include a reader interface module (RIM) 128 that is a subsystem to the patient application 126. The RIM 128 may be a program stored on a computer readable medium that is configured to communicate with the CorPASS system 200 or with other invasive peripheral systems and in particular the invasive peripheral device 110B. The RIM 128 may function separately from the patient application 126 but may communicate information to the patient application 126 to allow information to be displayed on the graphical user interface 124. The interaction between the patient application 126 and the RIM 128 includes separate functionality as the patient application 126 is designed to communicate with non-invasive peripheral devices 110A while the RIM 128 is designed to communicate with invasive peripheral devices 110B. The separate functionality may exist within the central hub 120 such that the hub 120 may be scalable to function with only non-invasive peripheral devices 110A, with only the invasive peripheral devices 110B, or with both non-invasive and invasive devices 110A, 110B. The RIM 128 may be a custom application running on the hub 120 that interfaces with the reader 150 and/or docking station 160 and passes collected physiologic data to a data analysis platform 132.

[0035] As illustrated by FIG. 8, the management portal 130 may be a clinic facing application that is intended to be accessible by a clinician. The management portal 130, as shown by FIG. 8, may be an interactive program that is stored in a computer readable medium or database. Alternatively, the portal 130 may be a web-based application that is displayed on a clinic facing display such as a computer, tablet, smartphone or other device. The management portal 130 may aggregate and display the collected physiologic data or patient's health status information and other related data or messages from the hub 120. This information may include physiologic data measured from the peripheral devices 110A, 110B as well as patient responses to various questions including health related questions that have been transported by the central hub 120.

[0036] The management portal 130 is specifically tailored to be optimized for a clinical workflow of clinical specialists and associated medical care providers. The particular clinical specialists contemplated by this disclosure includes cardiologists, nephrologists, orthopedist, gastroenterologist, hepatologist, neurologist, psychiatrist, critical care specialists, endocrinologist, oncologist, and ophthalmologists. The clinical workflow of clinical specialists include clinician facing dashboards set up to minimize time spent reviewing the monitored physiologic data and messages and also to track the clinician's time and billing data for interfacing with billing related programs and systems. For example, in a typical cardiologist clinic, a single nurse may manage a high number of patients wherein that nurse or clinician is allotted a minimal amount of time, such as only 15 minutes per

patient per week. The management portal **130** is optimized to minimize interruption of workflow tendencies, is subject to minimal training, and provides effective communication of relevant data while also communicating billing and timing information to associated billing programs and systems.

[0037] FIGS. **1**, **2**, and **11** illustrate that the management portal **130** may also include or communicate with the data analysis platform **132**, referred to herein as the Cordella™ Data Analysis Platform (CDAP) **132**. The CDAP may be a subsystem to the management portal **130**. The CDAP **132** may be a program stored on a computer readable medium that is configured to communicate with the CorPASS system **200** or other invasive peripheral system or device **110B** and in particular the RIM **128** of the CorPASS system **200**. Alternatively, the CDAP **132** may be a web based application or a database designed for artificial intelligence or machine learning. In one embodiment, the CDAP **132** may function separately from the management portal **130** and the patient application **126** of the central hub **120** but may communicate information to the management portal **130** and may be stored on an external server. The interaction between the management portal **130** and the CDAP **132** includes separate functionality as the management portal **130** is designed to communicate with and display information monitored from non-invasive peripheral devices **110A** while the CDAP **132** is designed to communicate with and display information from invasive peripheral devices **110B**. The separate functionality may exist within the management portal **130** such that the portal **130** may be scalable to function with only non-invasive peripheral devices **110A**, with only the invasive peripheral devices **110B**, or with both devices **110A**, **110B**. The CDAP **132** may interface with calibration equipment such as the docking station **160**, may store sensor calibration data, as well as sensor and reader factory settings. The CDAP **132** may process physiologic data monitored by the reader **150** and convert raw data such as frequency readings to processed data such as pulmonary artery pressure measurements. The CDAP **132** may communicate the processed data such as pulmonary artery pressure measurements to the management portal **130**. The CDAP **132** may interface with the RIM **128**, calibration equipment **160**, and central hub **120** and may also be in communication with an external server to communicate manufacture and field related data. The CDAP **132** may also allow for machine learning of physiologic and/or other data. Additionally, the RIM **128** and the CDAP **132** may interface with at least one of the following invasive peripheral devices **110B** including an implantable sensor, an actuator, a dialysis assembly, a drug delivery device, an infusion pump, a neuro-stimulation assembly, an oxygen delivery system, and a ventricular assistance device.

[0038] Turning to FIG. **2**, the RIM **128** and CDAP **132** may be subsystems to or communicate with the central hub **120** and management portal **130** respectively. It is illustrated that the physiological monitoring system **100** and the CorPASS **200** may operate separately or may be integrated to allow collected physiologic data from each peripheral devices **110A** and **110B** to be analyzed and displayed by respective graphic user displays of the central hub **120** and management portal **130**.

[0039] As illustrated by FIG. **9**, the patient app **126** may display various types of physiologic or biometric data including data representative of blood pressure, heart rate,

oxygen saturation, weight, and pulmonary artery pressure. This information may be displayed on the graphical user display **124**. Additionally, the management portal **130** may be configured to allow a clinician to review key clinical data (representative of the measured physiologic data), communicate with patients through the patient application **126**, and facilitate patient centered heart failure management. In this embodiment, the patient application **126** communicates with the management portal **130** through a secure cloud server **190**.

[0040] FIG. **10** illustrates a hierarchical flow chart of the physiological monitoring system **100**. This chart illustrates that the CorPASS system **200**, which may include a sensor, delivery system, reader, calibration equipment, CDAP, and reader integration module (RIM), interfaces with the other peripheral devices **110A** while being configured to communicate with the central hub **120** and management portal **130**. The system is designed to be in compliance with US federal regulations including 21 CFR 820.30—Medical Device Design Controls and ISO 13485:2007/EN-ISO 13485:2016.

[0041] Stated another way, the system **100** may be described as the Cordella Heart Failure System which collects, records, and transmits physiologic data and communications from the patient at home to clinician(s) for assessment, patient communication, and patient-centered heart failure management. The system **100** includes at least the following components:

[0042] 1. myCordella Patient Management Portal: **130** a clinic facing, web-based application which aggregates and displays the health status of patients, including biometric data and responses to health-related questions transmitted from the myCordella Hub **120** in the patient's home. The streamlined workflow defined by the Portal **130** enables clinicians to efficiently and effectively review patients; record notes and actions taken based on data trends; communicate with the patient and other clinicians regarding the patient's health status, and; provide supporting documentation for the clinician's continued, proactive management of the patient.

[0043] 2. myCordella Hub: **120** an intuitive, patient-facing, device with a standalone application that reminds the patient daily to obtain physiologic measurements and respond to health-related questions; instructs the patient on proper collection of biometric data; aggregates collected data to provide a snapshot of the patient's health status, and; securely transmits the patient's current health status to the myCordella Patient Management Portal **130**.

[0044] 3. myCordella Peripherals: **110A** medical or consumer health devices that collect biometric data (e.g. blood pressure, heart rate, blood oxygen and weight) and communicate with the myCordella Hub **120** to transmit data unaltered for display in the myCordella Patient Management Portal **130**.

[0045] 4. Cordella Pulmonary Artery Sensor System (CorPASS): **110B**, **200** an innovative myCordella Peripheral designed for on-demand measurement of pulmonary artery pressure from the patient's home or elsewhere (to identify pulmonary congestion suggestive of worsening heart failure through trends in pulmonary artery pressures). The Cordella PA Sensor System includes: a catheter-based Delivery System **170** with a pre-loaded Sensor **180** for implant; Calibration

Equipment **160** for collecting relevant calibration information during implantation; a myCordella Patient Reader **150** which enables patients to measure PA pressure at home from the sensor **180** implanted within the patient; and a cloud-based data analysis platform to store and analyze home PA pressure readings. Pulmonary artery pressure data is collected from the Cordella Sensor with the myCordella Patient Reader by the patient at home. The Reader uploads its data through the Reader Interface Module on the myCordella Hub to the data analysis platform where the analyzed data is shared with the myCordella Patient Management Portal **130**, enabling a more complete picture of the health status of the patient(s).

**[0046]** When used together the components of the Cordella Heart Failure System **100** enable proactive, patient-centered heart failure management. FIG. **11** schematizes the Cordella subsystems and the data flow between them.

**[0047]** The embodiments of this disclosure have been described above and, obviously, modifications and alternations will occur to others upon reading and understanding this specification. The claims as follows are intended to include all modifications and alterations insofar as they are within the scope of the claims or the equivalent thereof.

1. A physiologic monitoring system comprising:
  - a central hub in communication with a management portal;
  - at least one non-invasive peripheral device to measure physiologic data from a patient in communication with said central hub; and
  - an invasive peripheral system associated with said patient and in communication with said central hub;
  - wherein the central hub is scalable to collect data and communicate with the non-invasive peripheral device and the invasive peripheral system such that data from the non-invasive peripheral device and the invasive peripheral system are selectively communicated to the management portal.
2. The physiologic monitoring system of claim **1** wherein said at least one non-invasive peripheral device includes a blood pressure cuff, an oxygen sensor, a weight scale, and an ECG monitor.
3. The physiologic monitoring system of claim **1** wherein said invasive peripheral system includes an invasive peripheral device, wherein said invasive peripheral device includes at least one of an implantable sensor, an actuator, a dialysis assembly, a drug delivery device, an infusion pump, a neuro-stimulation assembly, an oxygen delivery system, or a ventricular assistance device.
4. The physiologic monitoring system of claim **3** further comprising a wireless sensor reader and a docking station, the wireless sensor reader adapted to measure physiologic data from said implantable sensor placed within a cardiovascular system of said patient.
5. The physiologic monitoring system of claim **1** wherein said central hub includes a graphical user interface for displaying a patient application.
6. The physiologic monitoring system of claim **3** wherein said central hub includes a reader interface module in communication with the invasive peripheral system.
7. The physiologic monitoring system of claim **6** wherein said management portal is in communication with a data analysis platform that is configured to receive data from the

reader interface module, analyze the received data to generate processed data, and communicate the processed data to the management portal.

8. A method of monitoring physiologic data comprising:
  - measuring physiologic data from a patient with at least one non invasive peripheral device;
  - measuring physiologic data from said patient with a system that includes an invasive peripheral device;
  - communicating said physiologic data to a central hub; and
  - communicating said physiologic data to a management portal to display to a clinical specialists.
9. The method of monitoring physiologic data of claim **8** further comprising generating a plurality of health-related questions by the central hub to be answered by the patient.
10. The method of monitoring physiologic data of claim **8** further comprising aggregating the physiologic data and displaying the physiologic data at the central hub.
11. The method of monitoring physiologic data of claim **8** further comprising aggregating the physiologic data and displaying the physiologic data at the management portal.
12. The method of monitoring physiologic data of claim **8** wherein said non-invasive peripheral device includes at least one of a blood pressure cuff, an oxygen sensor, a weight scale, and an ECG monitor.
13. The method of monitoring physiologic data of claim **8** wherein said invasive peripheral device includes at least one of an implantable sensor, an actuator, a dialysis assembly, a drug delivery device, an infusion pump, a neuro-stimulation assembly, an oxygen delivery system, or a ventricular assistance device.
14. The method of monitoring physiologic data of claim **13** further comprising communicating between said implantable sensor and a wireless sensor reader to measure physiologic data from said implantable sensor placed within a cardiovascular system of said patient.
15. The method of monitoring physiologic data of claim **8** wherein physiologic data measured from a patient with at least one non invasive peripheral device is communicated to the management portal to display to said clinical specialist, wherein said clinical specialist analyzes said communicated physiologic data to prescribe an invasive peripheral device for use by said patient.
16. The method of monitoring physiologic data of claim **8** further comprising communicating measured physiologic data to a reader interface module of the central hub from the invasive peripheral device.
17. The method of monitoring physiologic data of claim **8** further comprising communicating measured physiologic data from said invasive peripheral device to a data analysis platform from the reader interface module wherein said data analysis platform analyzes said measured physiologic data and generates processed data wherein said processed data is communicated to the management portal.
18. A physiologic monitoring system comprising:
  - a central hub in communication with a management portal, said central hub includes a reader interface module and a graphical user interface for displaying a patient application;
  - at least one non-invasive peripheral device to measure physiologic data from a patient in communication with said central hub;
  - a peripheral system that includes an invasive peripheral device to measure physiologic data from said patient in

communication with said central hub, the peripheral system in communication with said reader interface module;

wherein the central hub is scalable to collect and communicate measurements from the non-invasive peripheral device and the invasive peripheral device; and

wherein said management portal is in communication with a data analysis platform configured to receive data from said reader interface module and display said data at the management portal.

**19.** The physiologic monitoring system of claim **18** wherein said at least one non-invasive peripheral device includes a blood pressure cuff, an oxygen sensor, a weight scale, and an ECG monitor.

**20.** The physiologic monitoring system of claim **18** wherein said invasive peripheral device includes an implantable sensor.

**21.** The physiologic monitoring system of claim **18** wherein said data analysis platform is configured to interface with the peripheral system and the invasive peripheral device to calibrate said invasive peripheral device.

**22.** A method of monitoring physiologic data comprising: measuring physiologic data from a patient with at least one non invasive peripheral device;

communicating said physiologic data to a central hub, said central hub includes a reader interface module;

communicating said physiologic data to a management portal to display to a specialist clinician;

analyzing said communicated physiologic data to prescribe a system that includes an invasive peripheral device for use by the patient;

measuring physiologic data from said patient with said system that includes said invasive peripheral device;

communicating said physiologic data to said reader interface module of said central hub;

communicating said physiologic data to said management portal to display to a clinician.

**23.** The method of monitoring physiologic data of claim **22** further comprising aggregating the physiologic data and displaying the physiologic data at the management portal.

**24.** The method of monitoring physiologic data of claim **22** wherein said non-invasive peripheral device includes at least one of a blood pressure cuff, an oxygen sensor, a weight scale, and an ECG monitor.

**25.** The method of monitoring physiologic data of claim **22** wherein said invasive peripheral device includes at least one of an implantable sensor, an actuator, a dialysis assembly, a drug delivery device, an infusion pump, a neurostimulation assembly, an oxygen delivery system, or a ventricular assistance device.

\* \* \* \* \*

专利名称(译)	生理监测系统		
公开(公告)号	<a href="#">US20190021597A1</a>	公开(公告)日	2019-01-24
申请号	US16/040034	申请日	2018-07-19
[标]申请(专利权)人(译)	因多卓尼克斯公司		
申请(专利权)人(译)	ENDOTRONIX INC.		
当前申请(专利权)人(译)	ENDOTRONIX INC.		
[标]发明人	NAGY MICHAEL ROWLAND HARRY JOHNSON ARIEL QUAS BRETT		
发明人	NAGY, MICHAEL ROWLAND, HARRY JOHNSON, ARIEL QUAS, BRETT		
IPC分类号	A61B5/00 A61B5/1455 G16H10/60		
CPC分类号	A61B5/0022 A61B5/0006 A61B5/1455 G16H10/60 A61B5/0031 A61B5/021 A61B5/7465 A61B5/0402 A61B5/0205 G16H10/20 A61B5/14551 A61M1/101 A61M1/1086 A61M1/122 A61M5/142 A61M5/1723 A61M2205/3507 A61M2205/505 A61M2230/04 A61M2230/20 A61N1/3605 G16H40/67		
优先权	62/534261 2017-07-19 US		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

摘要(译)

公开了一种生理监测系统，其包括与管理门户通信的中心枢纽，用于传送从患者身上的多个外围设备获取的生理测量值。至少一个非侵入性外围设备可以测量来自患者的生理数据并且与所述中央集线器通信。包括侵入性外围设备的系统可以与所述患者相关联并且与所述中央集线器通信。中央集线器可以是可缩放的，以收集和传送来自非侵入性外围设备和侵入式外围设备的测量结果。至少一个非侵入性外围设备可包括血压袖带，氧传感器，体重计和ECG监视器。侵入式外围设备可以包括无线传感器读取器，其可以适于测量来自放置在所述患者的心血管系统内的传感器植入物的生理数据。

