



US010143425B1

(12) **United States Patent**
Zhao et al.

(10) **Patent No.:** **US 10,143,425 B1**
(45) **Date of Patent:** **Dec. 4, 2018**

(54) **METHODS OF DATA ACQUISITION
QUALITY AND DATA FUSION FOR
PERSONAL PORTABLE WIRELESS VITAL
SIGNS SCANNER**

(71) Applicant: **SCANADU INCORPORATED**,
Moffett Field, CA (US)

(72) Inventors: **Wenyi Zhao**, Mountain View, CA (US);
Brandon Dennis Woolsey, San Jose,
CA (US); **Walter De Brouwer**, Los
Altos, CA (US); **Eron Anthony**
Villarreal, San Jose, CA (US);
Whitney Morgan McGowan, San Jose,
CA (US); **Martin Zizi**, Enines (BE)

(73) Assignee: **Scanadu Incorporated**, Sunnyvale, CA
(US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 239 days.

(21) Appl. No.: **14/292,820**

(22) Filed: **May 30, 2014**

Related U.S. Application Data

(60) Provisional application No. 61/875,681, filed on Sep.
9, 2013, provisional application No. 61/924,230, filed
on Jan. 6, 2014.

(51) **Int. Cl.**
A61B 5/00 (2006.01)
A61B 5/0205 (2006.01)
A61B 5/0402 (2006.01)
A61B 5/1455 (2006.01)
A61B 5/11 (2006.01)

(52) **U.S. Cl.**
CPC **A61B 5/7221** (2013.01); **A61B 5/02055**
(2013.01); **A61B 5/0402** (2013.01); **A61B 5/11**
(2013.01); **A61B 5/14551** (2013.01); **A61B**
5/742 (2013.01)

(58) **Field of Classification Search**
CPC A61B 1/00172; A61B 5/0002
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

6,261,238 B1 * 7/2001 Gavriely A61B 5/087
600/532
2005/0137653 A1 * 6/2005 Friedman A61B 5/0002
607/60

(Continued)

Primary Examiner — Amanda Hulbert


Assistant Examiner — Natasha Patel

(74) *Attorney, Agent, or Firm* — Alford Law Group, Inc.;
Tobi Clinton

(57) **ABSTRACT**

In one embodiment of the invention, an interactive vital signs scanning method is disclosed including concurrently scanning for a plurality of vital signs with a portable vital signs scanner; detecting movement of the portable vital signs scanner during the scanning for the plurality of vital signs; and determining a measure of quality of the scanning for the plurality of vital signs with the portable vital signs scanner. In another embodiment, a method of improving the quality of vital signs data is disclosed including concurrently sensing data from a plurality of vital signs sensors over a period of time with a portable vital signs scanner; determining a plurality of vital sign values for a respective plurality of vital signs in response to the sensed data from the plurality of vital signs sensors over the period of time; and fusing at least two vital sign values of the plurality of vital sign values for the respective plurality of vital signs.

34 Claims, 27 Drawing Sheets

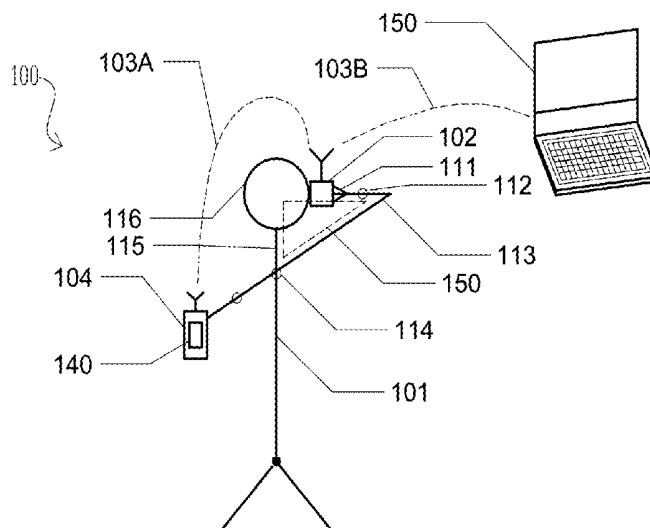

(56)

References Cited

U.S. PATENT DOCUMENTS

2007/0142715	A1 *	6/2007	Banet	A61B 5/0006 600/301
2007/0219059	A1 *	9/2007	Schwartz	A61B 5/0205 482/8
2008/0300504	A1 *	12/2008	Lefkov	A61B 5/053 600/547
2009/0275805	A1 *	11/2009	Lane	A61B 5/01 600/300
2011/0066051	A1 *	3/2011	Moon	A61B 5/0002 600/509
2012/0029310	A1 *	2/2012	Paquet	A61B 5/0008 600/301
2013/0217979	A1 *	8/2013	Blackadar	A61B 5/0205 600/301

* cited by examiner

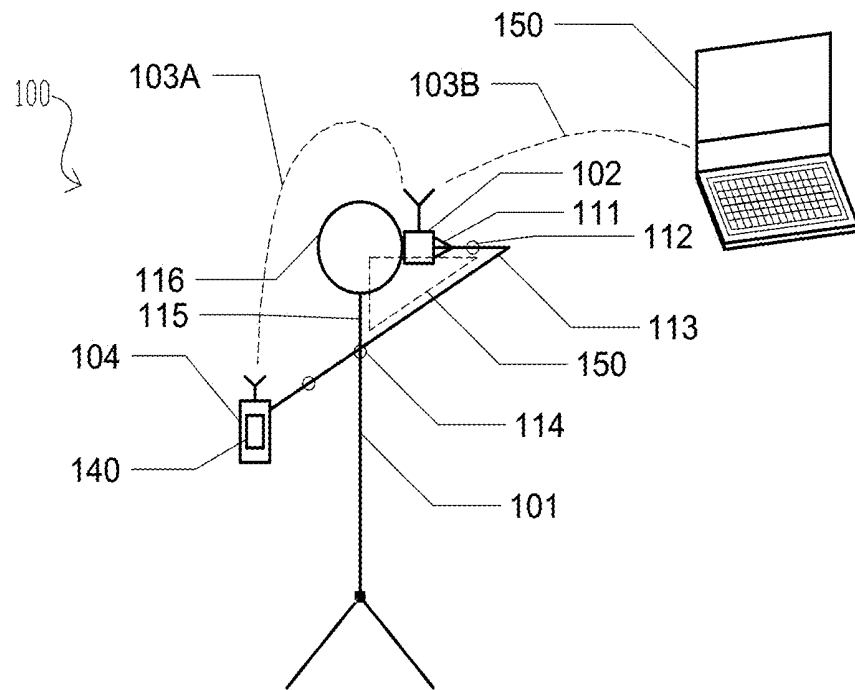


FIG. 1A

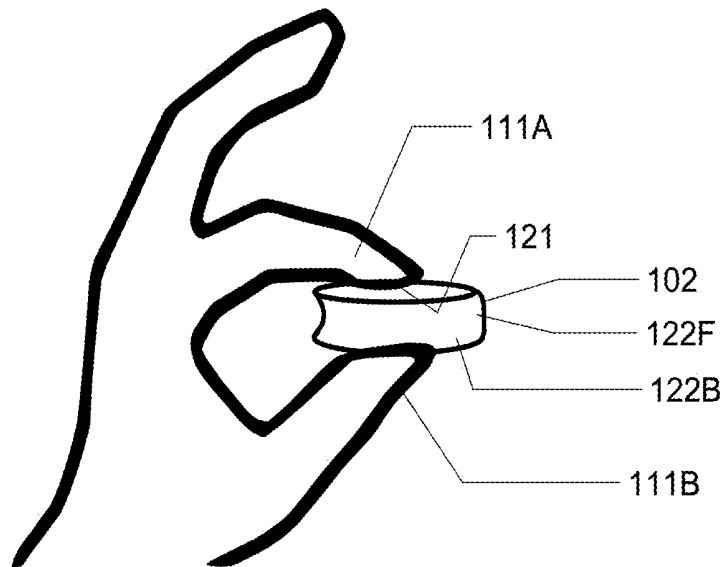


FIG. 1B

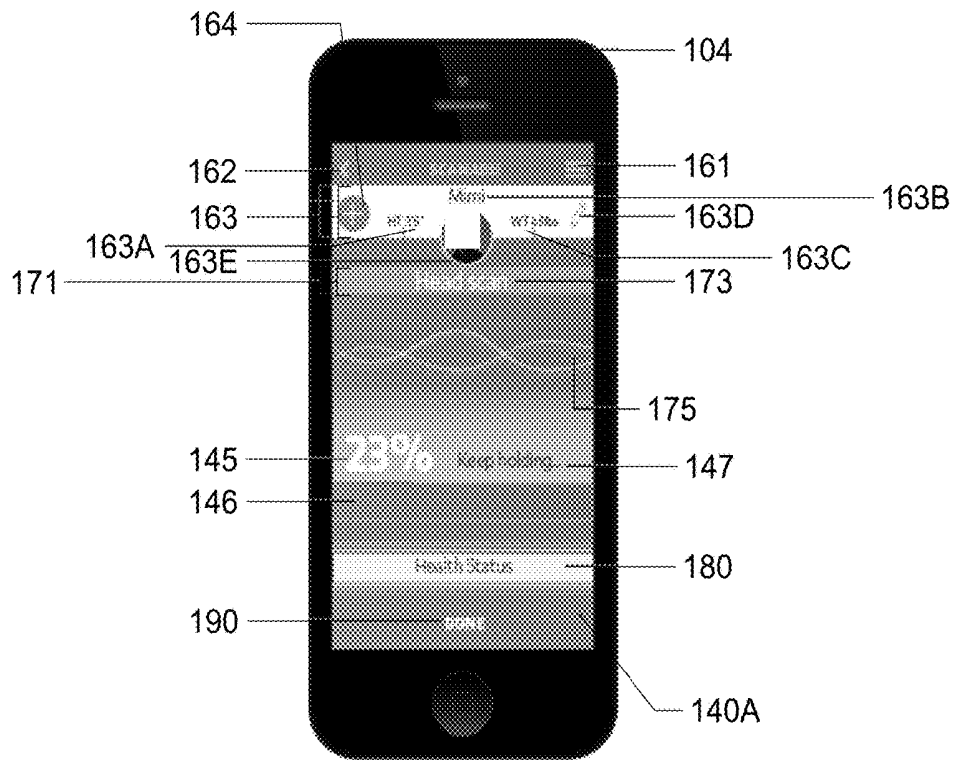


FIG. 1C

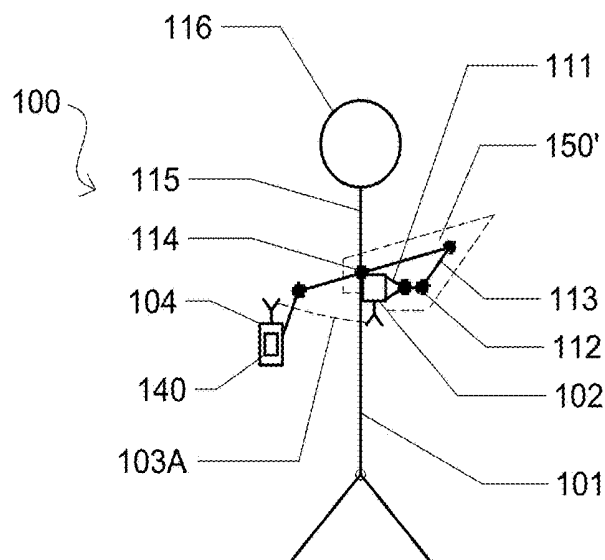


FIG. 1D

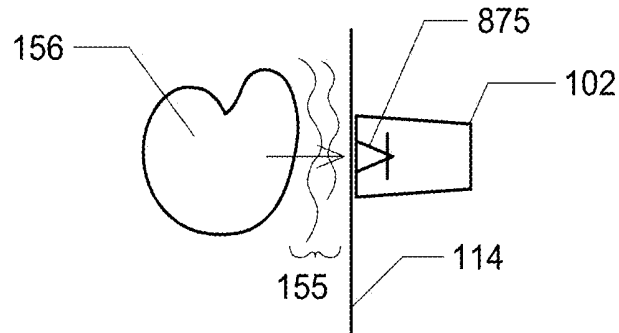


FIG. 1E

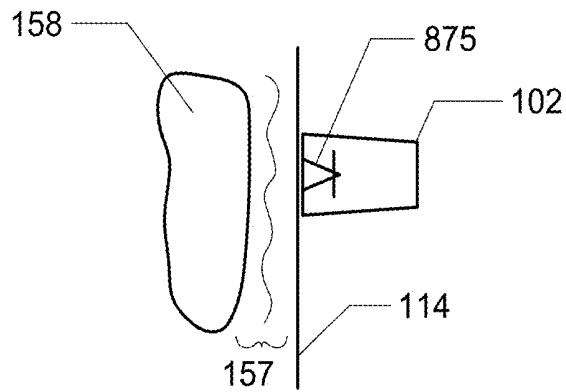


FIG. 1F

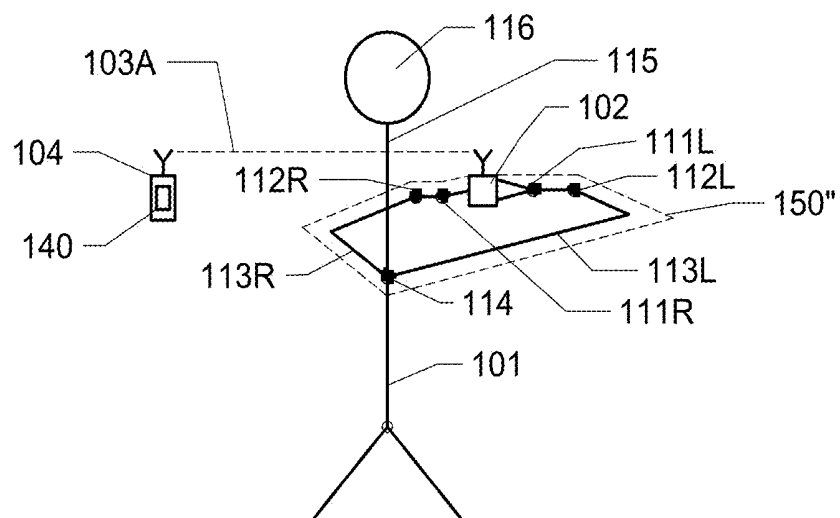


FIG. 1G

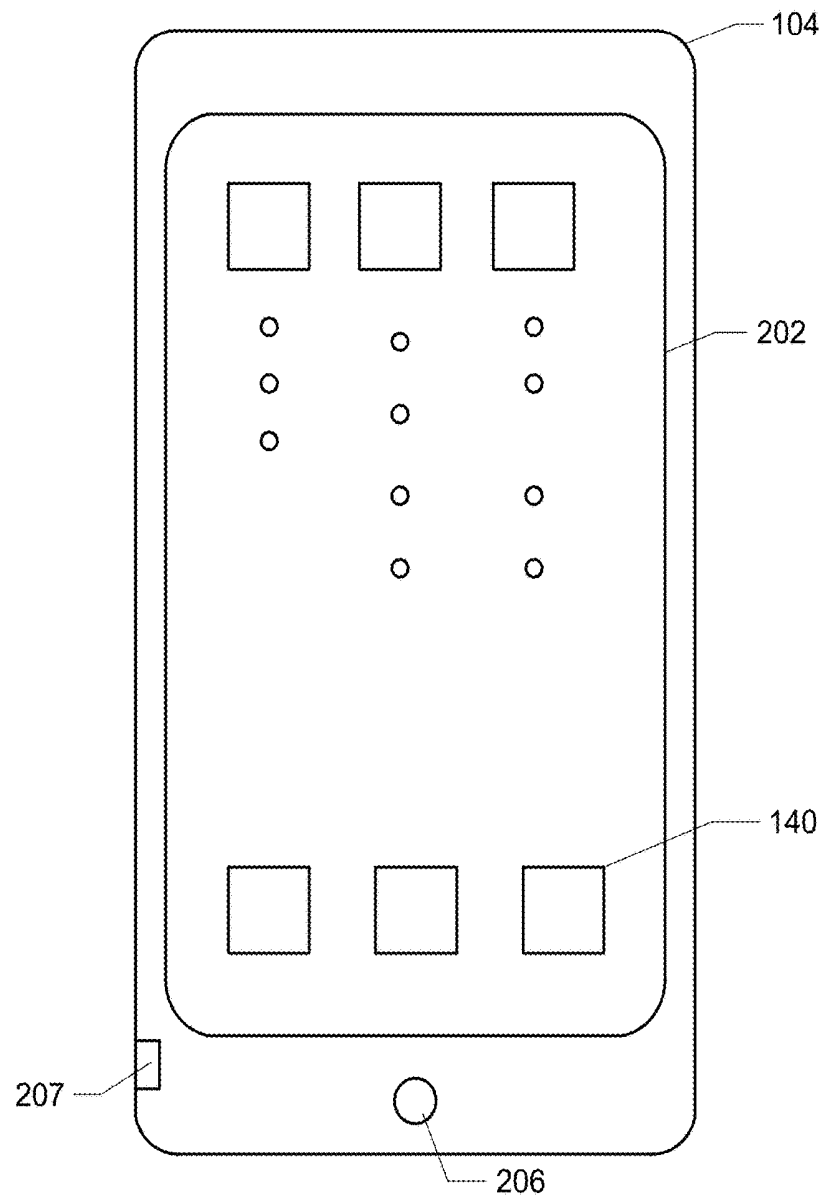


FIG. 2A

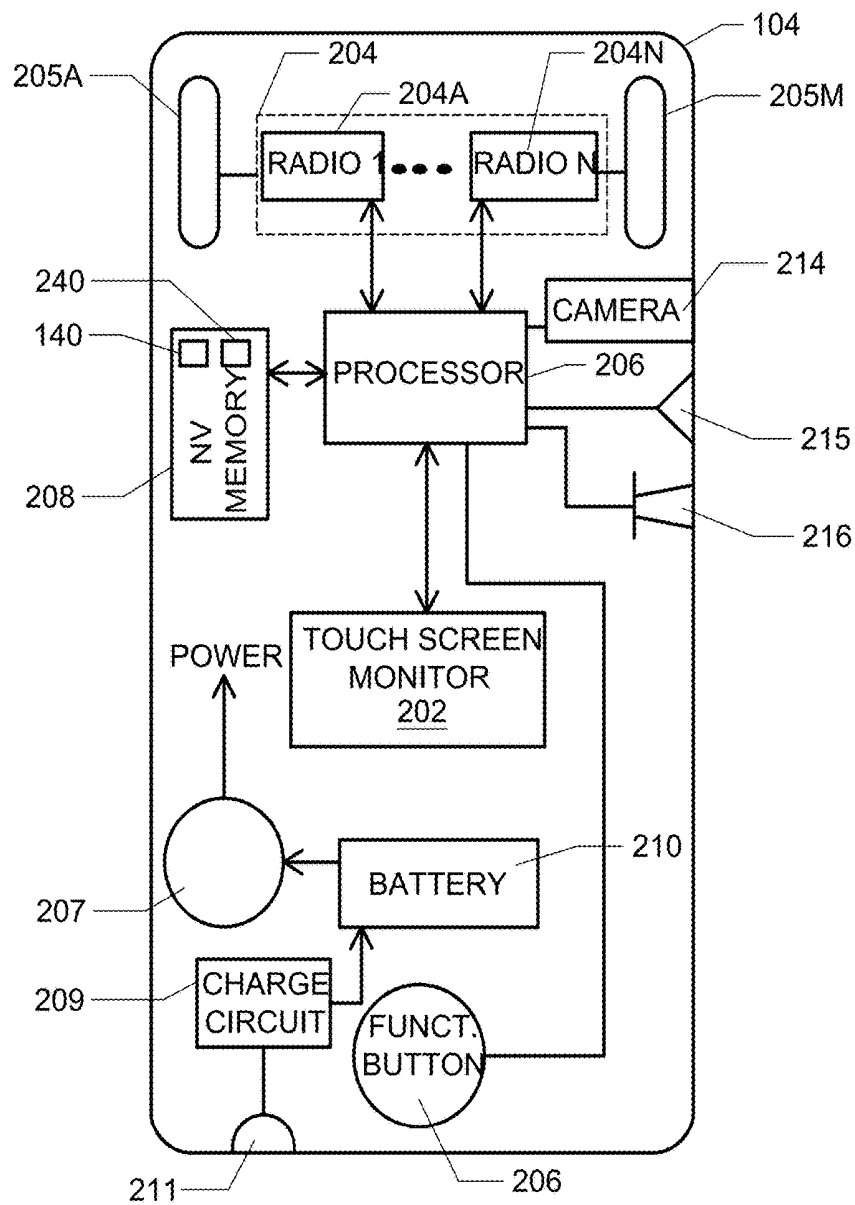


FIG. 2B

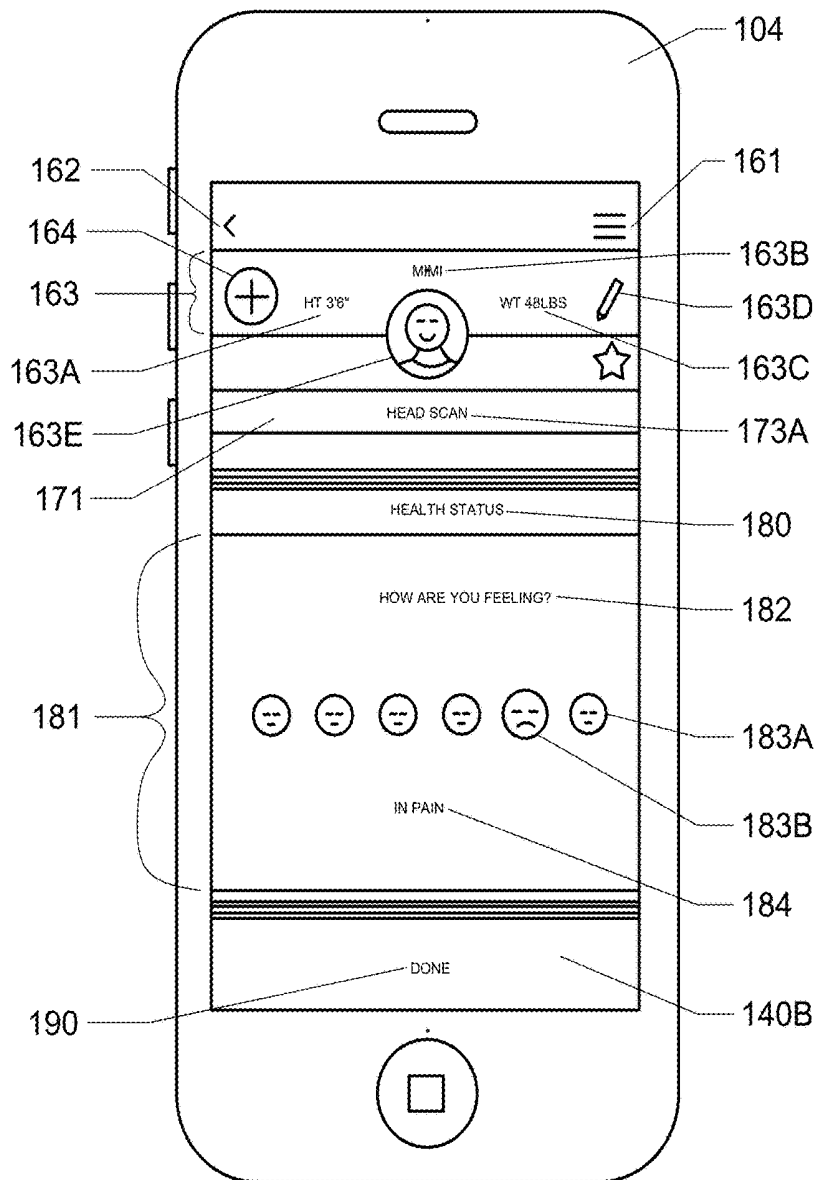


FIG. 3A

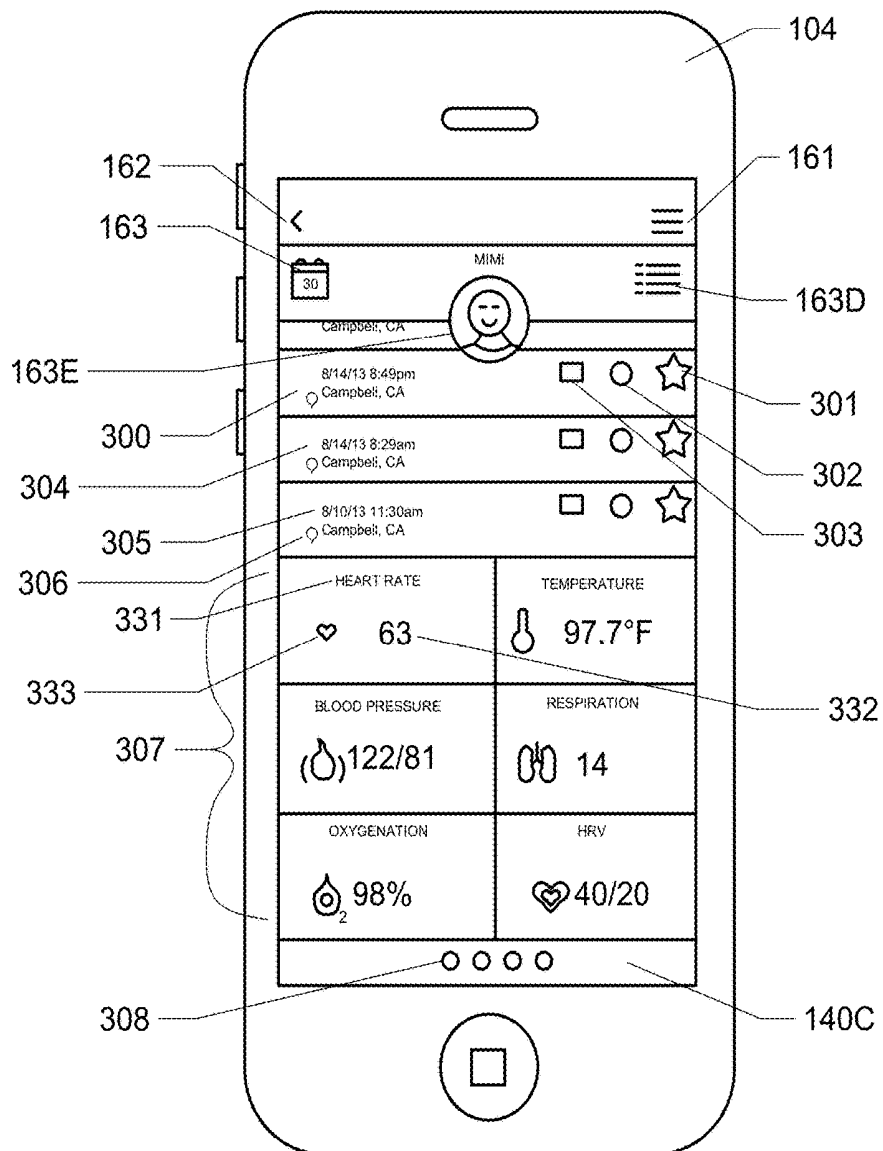


FIG. 3B

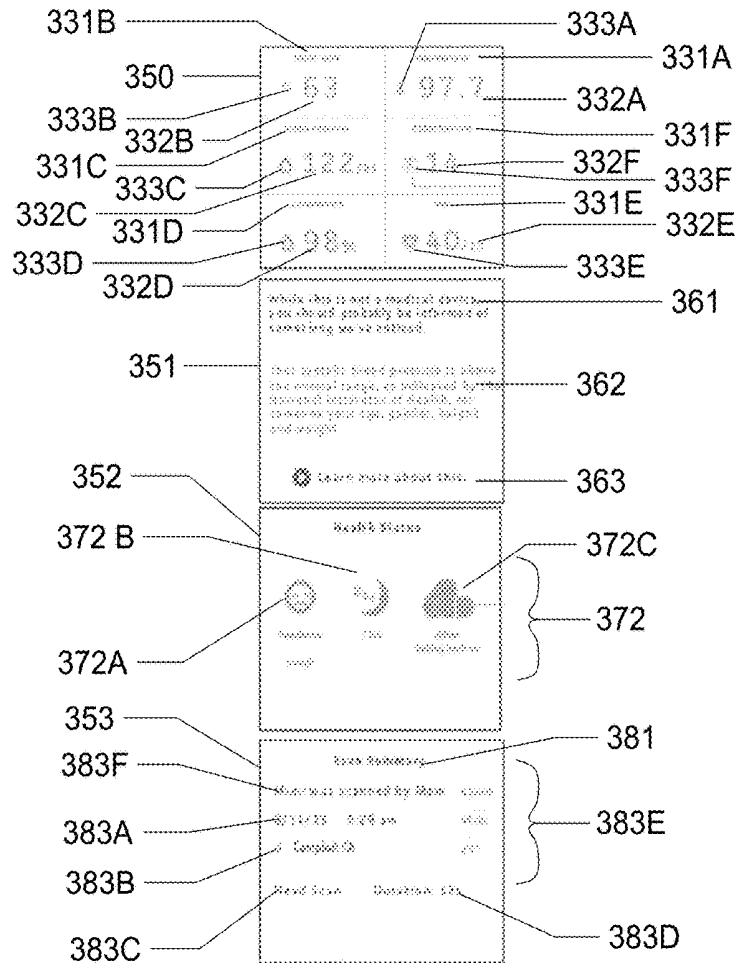


FIG. 3C

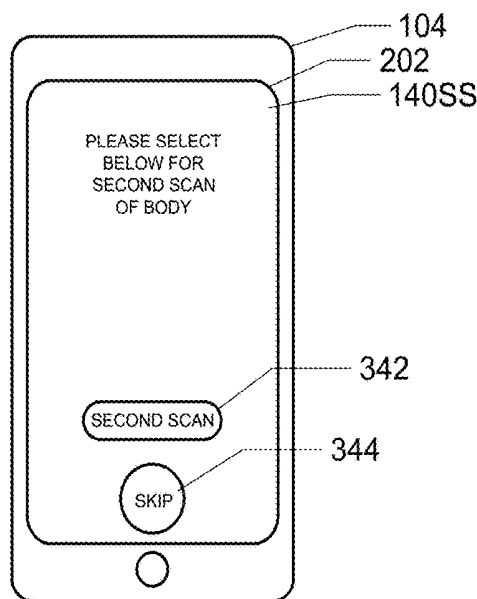


FIG. 3D

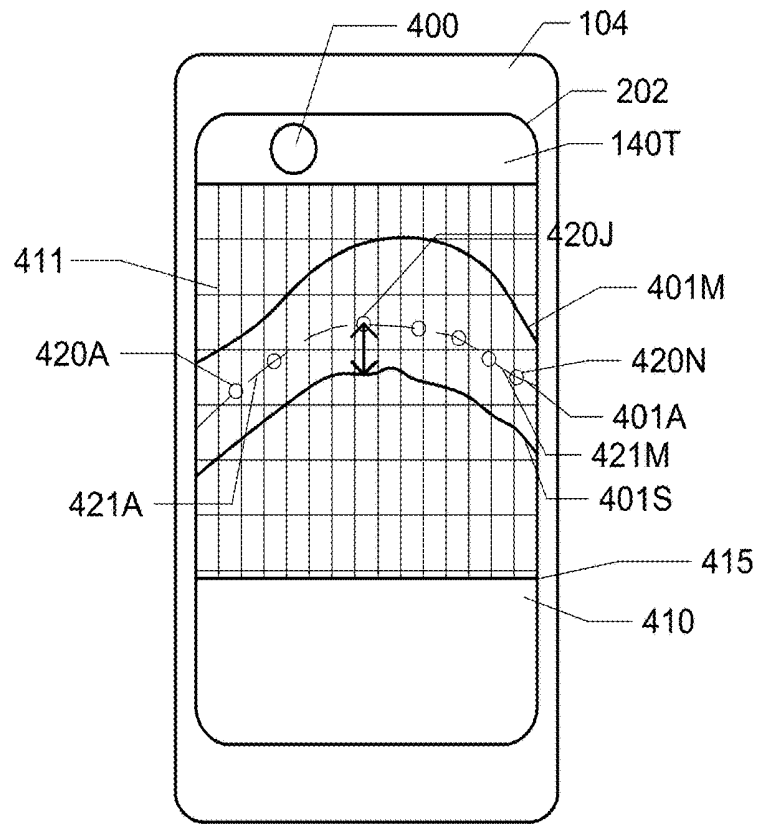


FIG. 4A

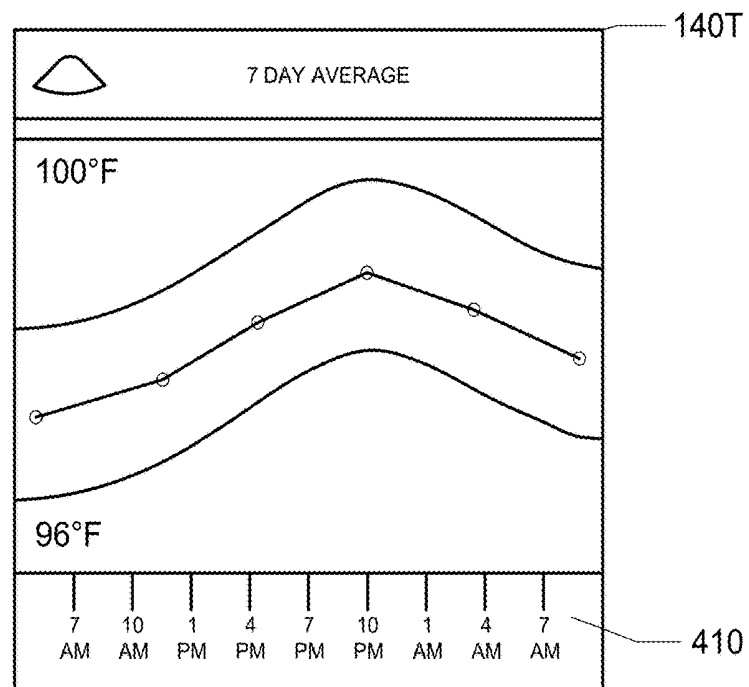


FIG. 4B

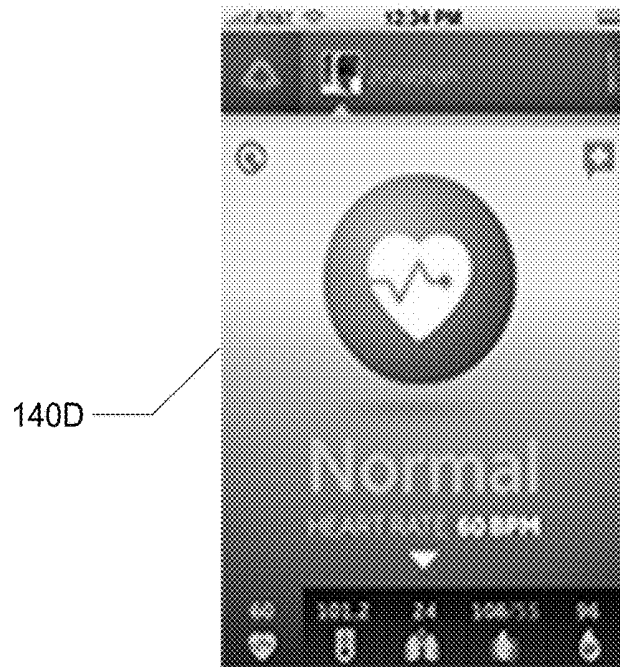


FIG. 5A

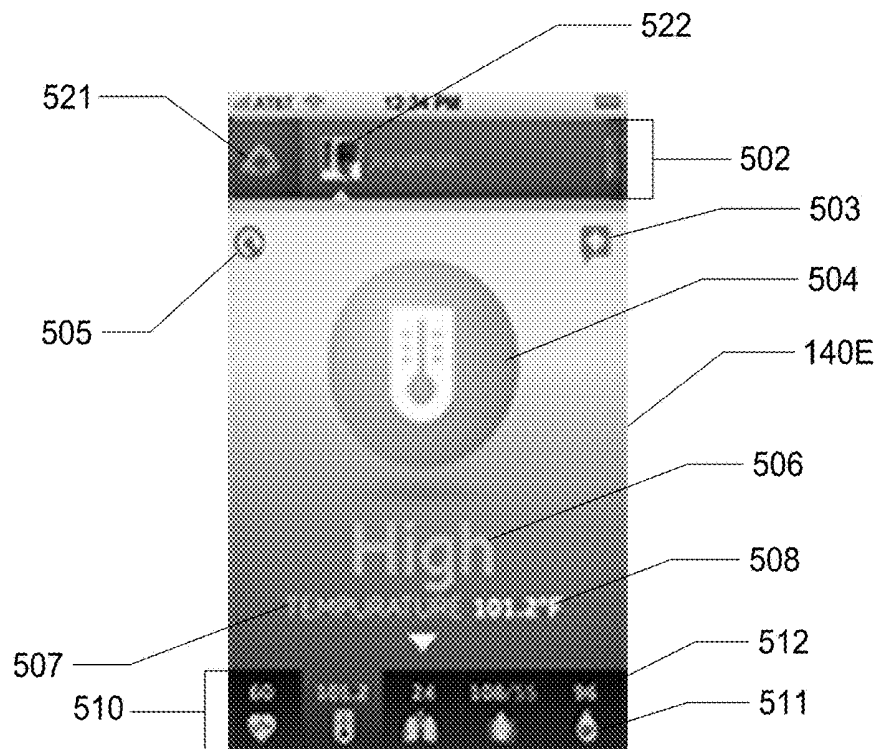


FIG. 5B

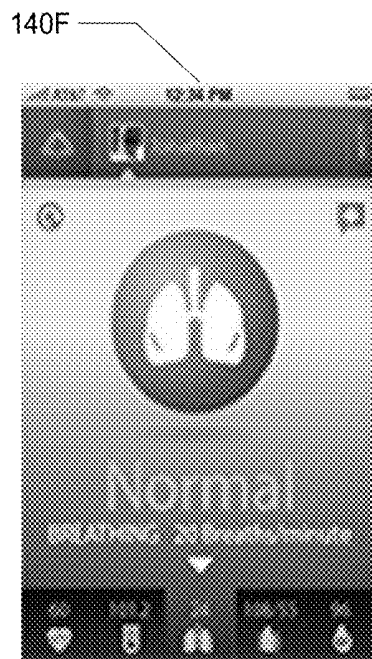


FIG. 5C

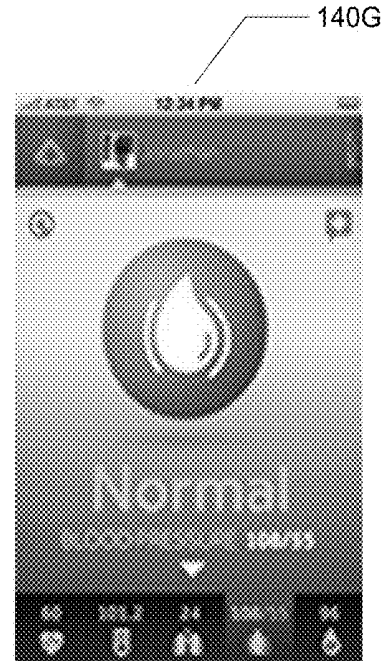


FIG. 5D

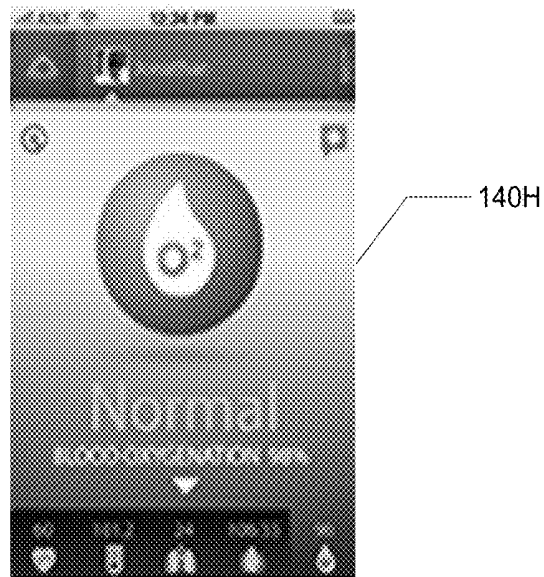


FIG. 5E

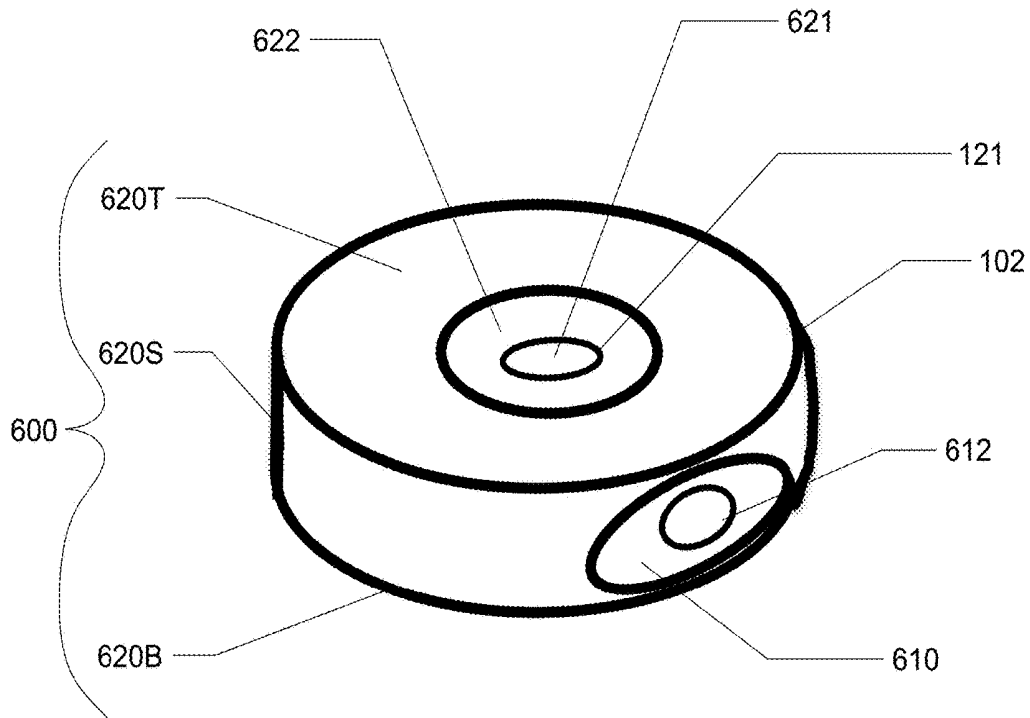


FIG. 6A

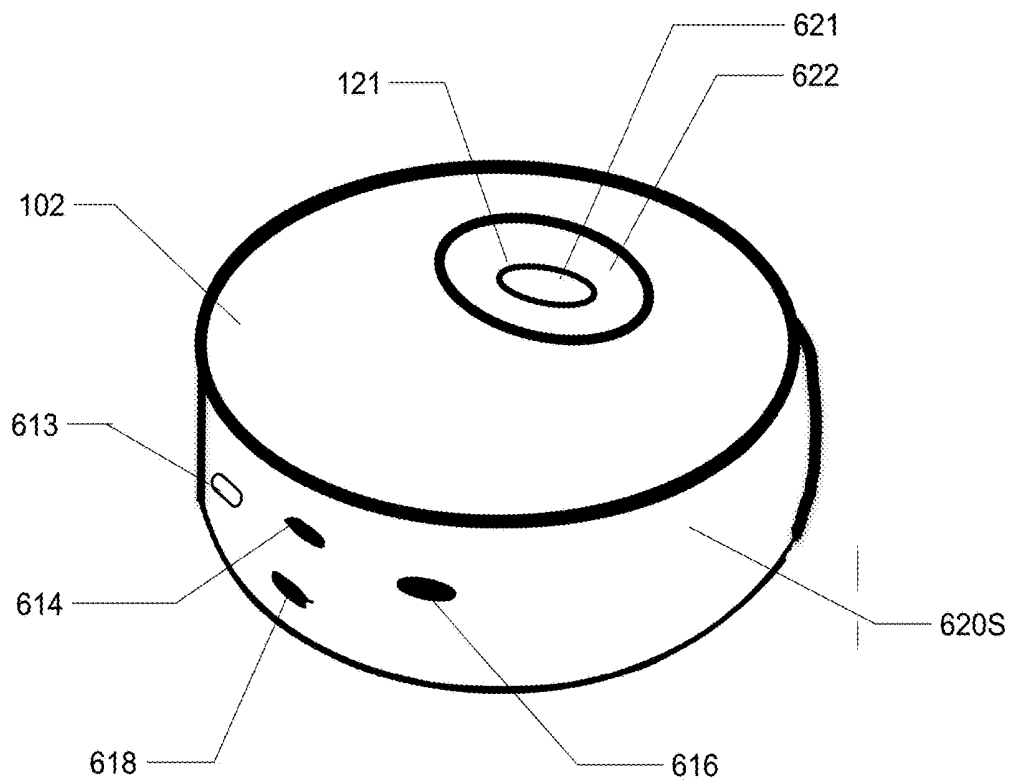


FIG. 6B

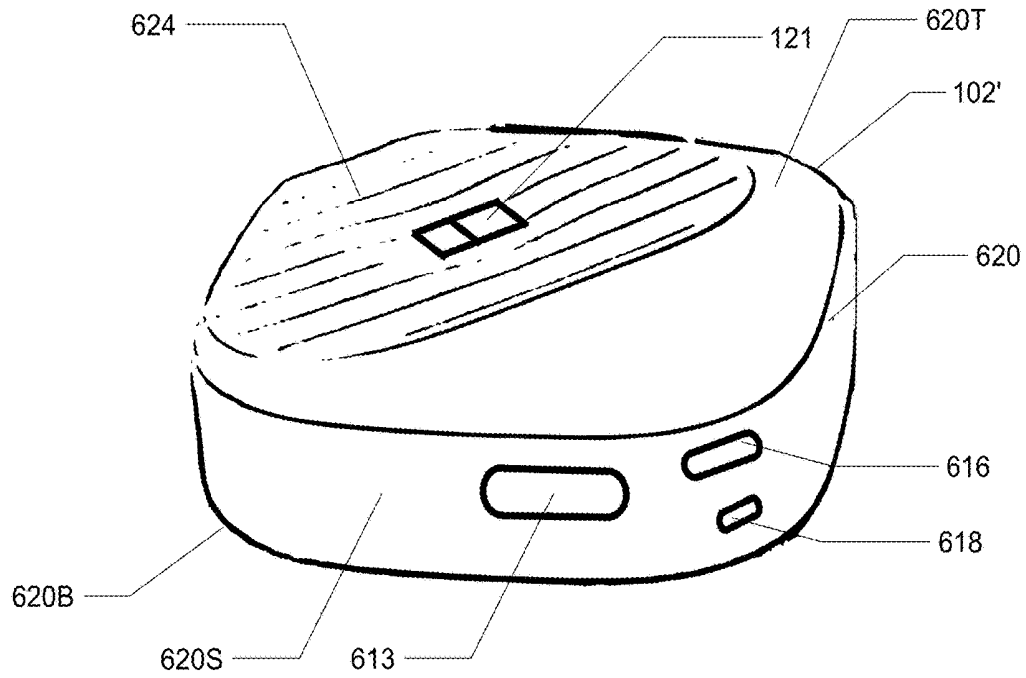


FIG. 6C

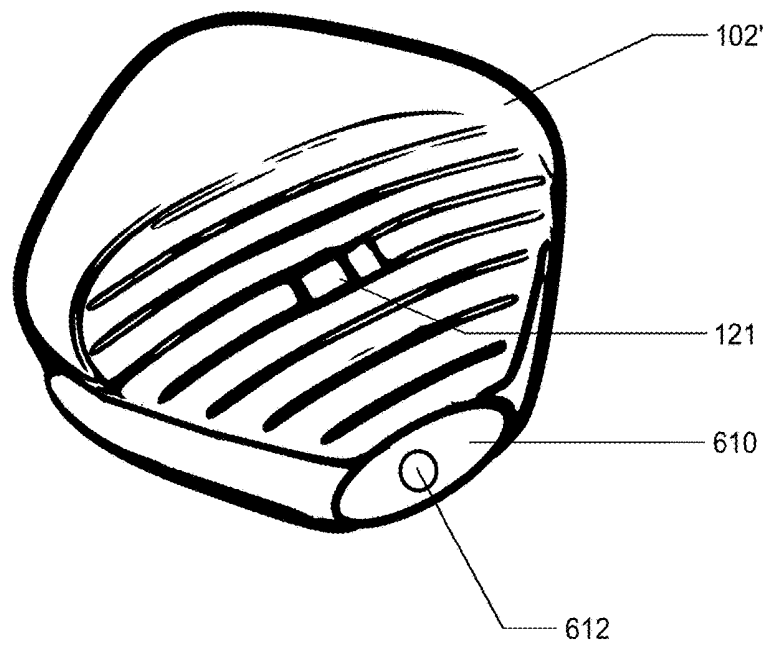


FIG. 6D

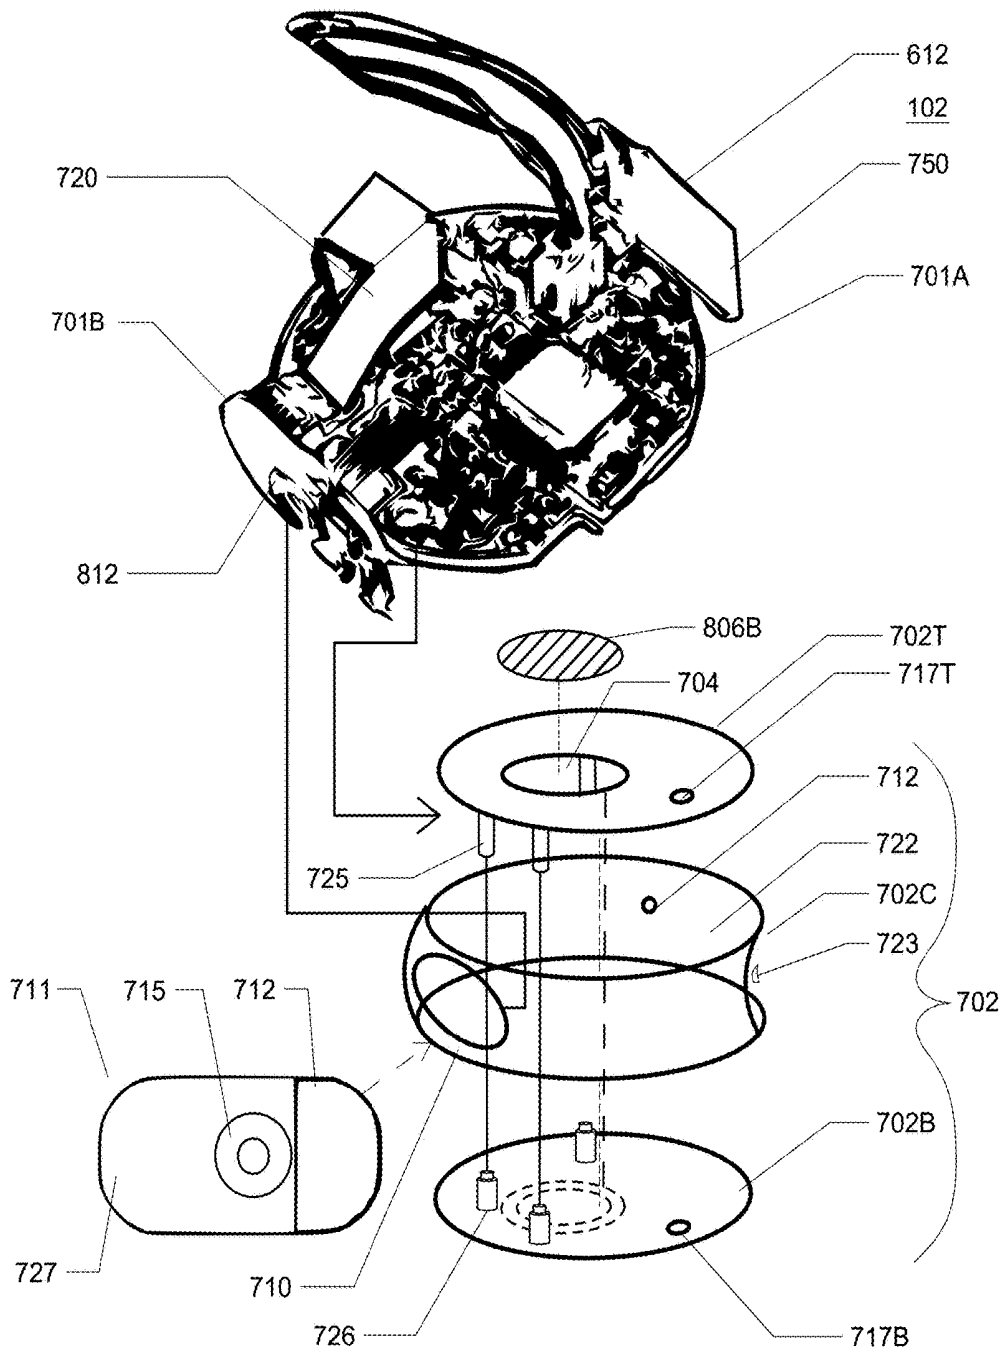


FIG. 7A

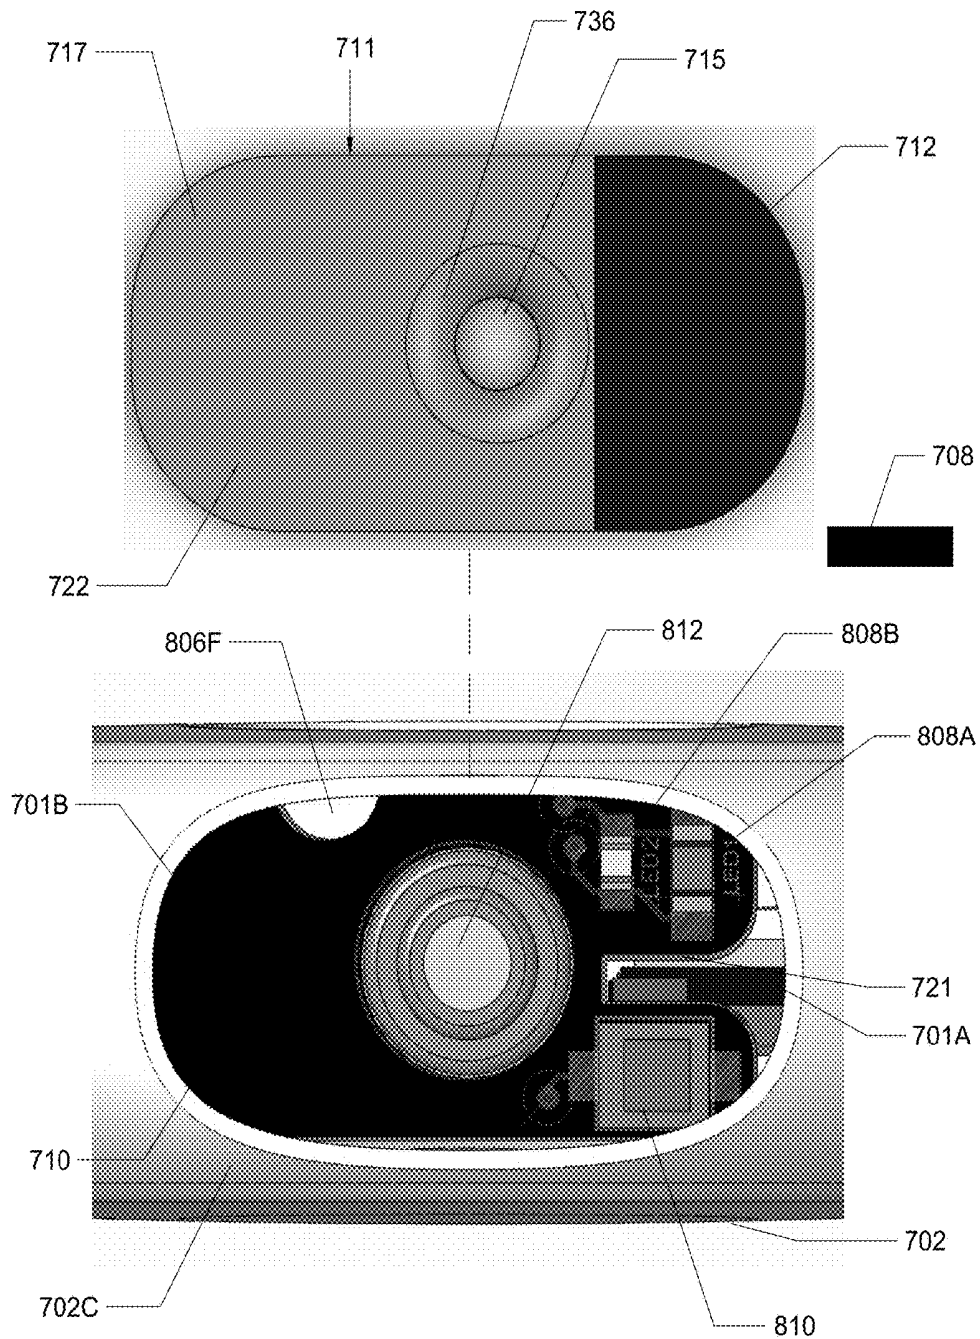


FIG. 7B

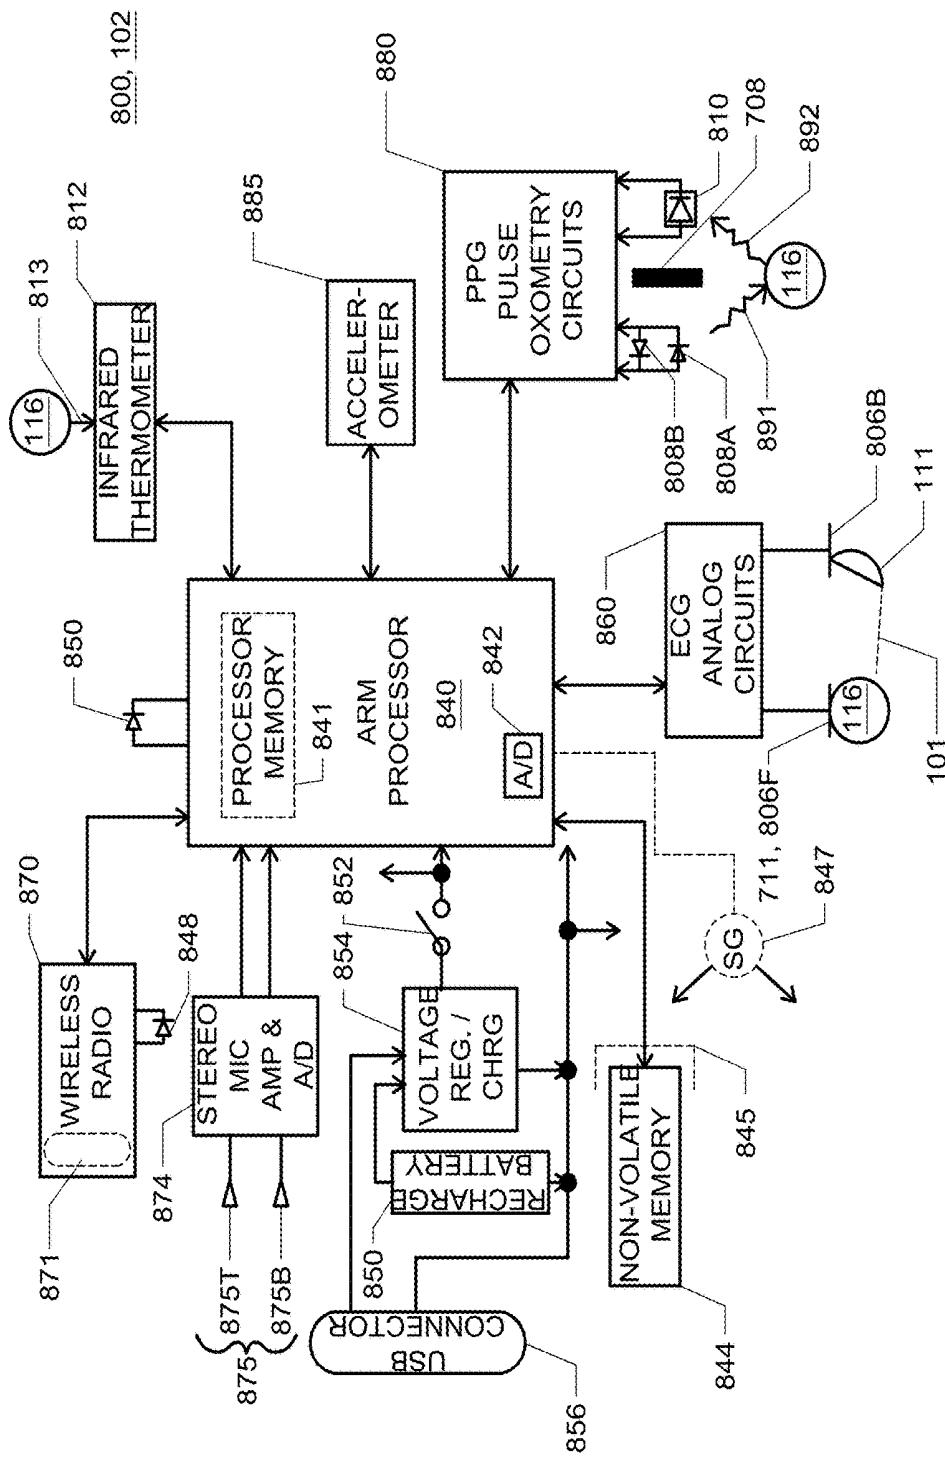


FIG. 8A

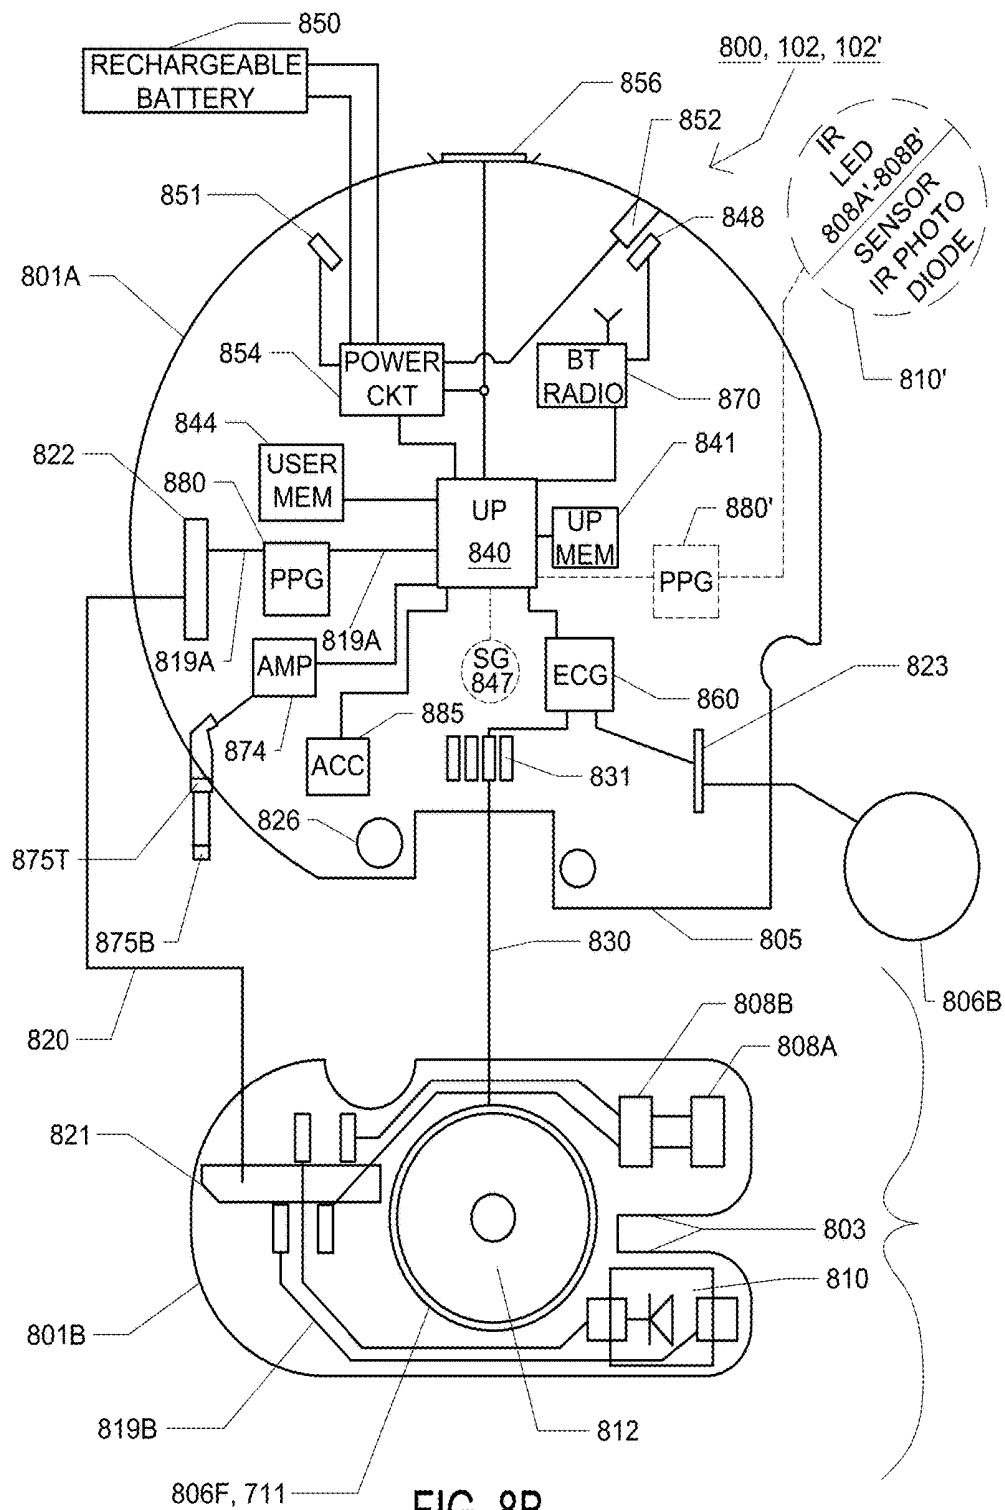


FIG. 8B

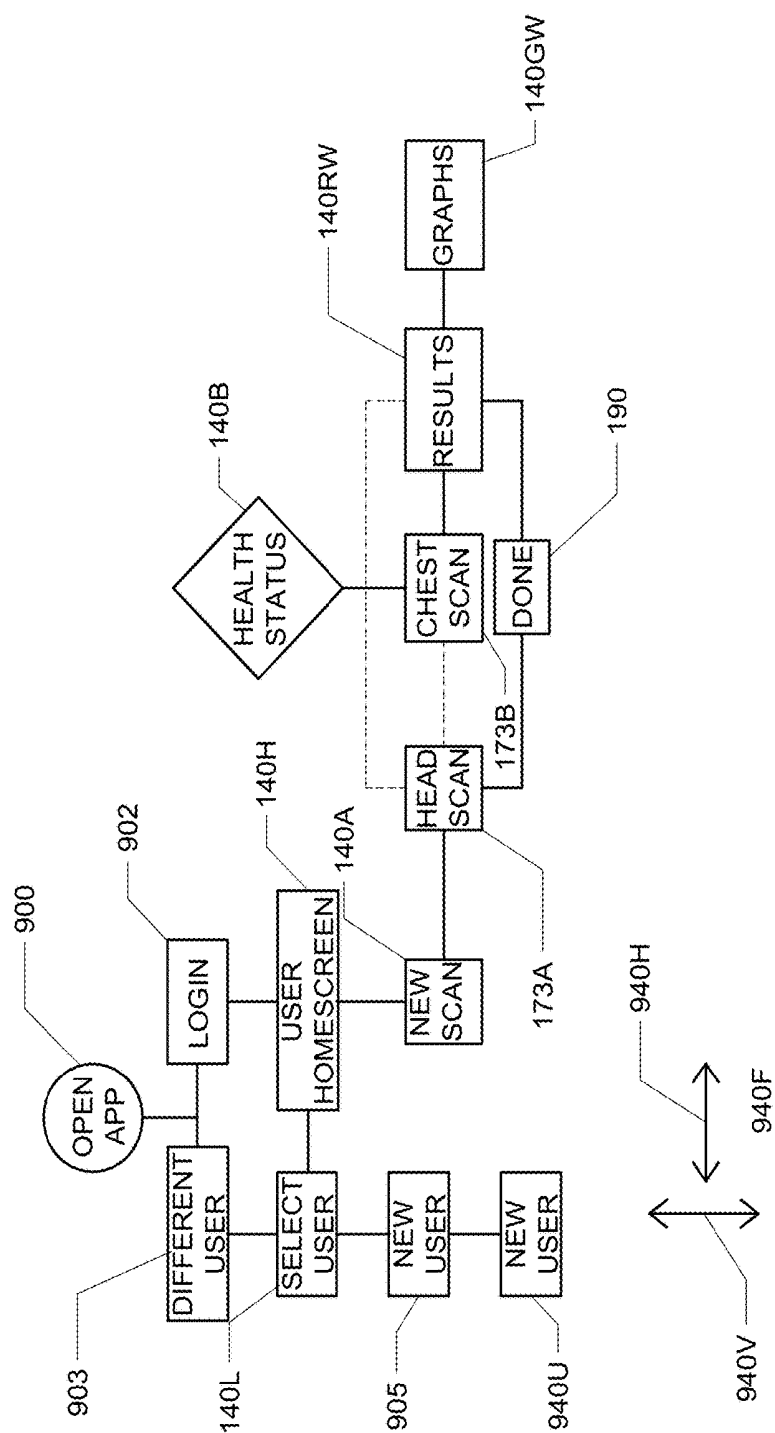


FIG. 9

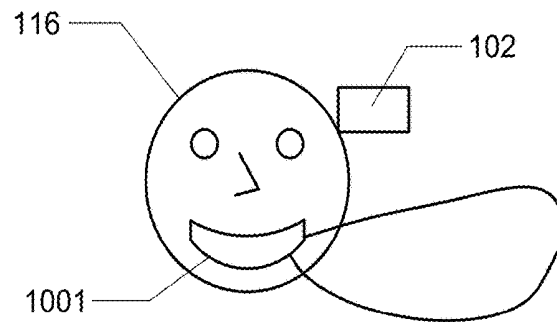


FIG. 10A

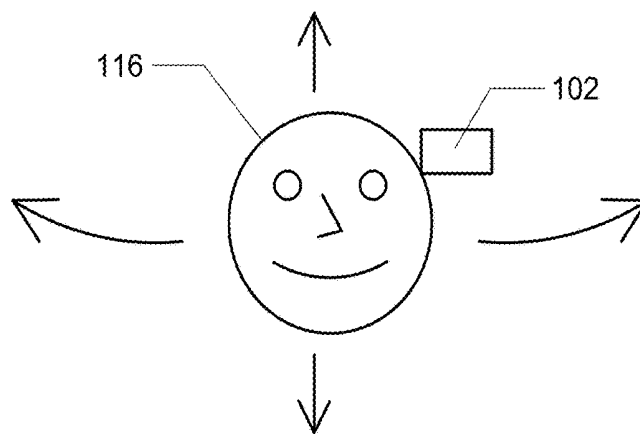


FIG. 10B

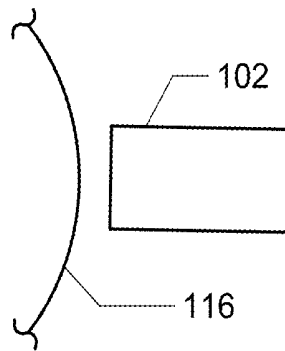


FIG. 11A

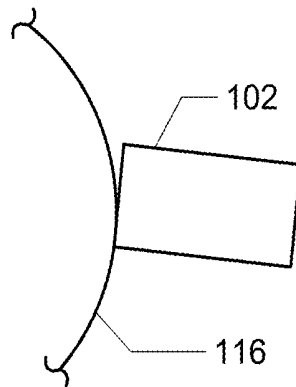


FIG. 11B

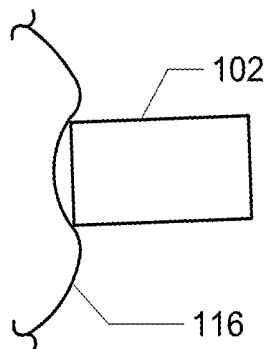


FIG. 11C

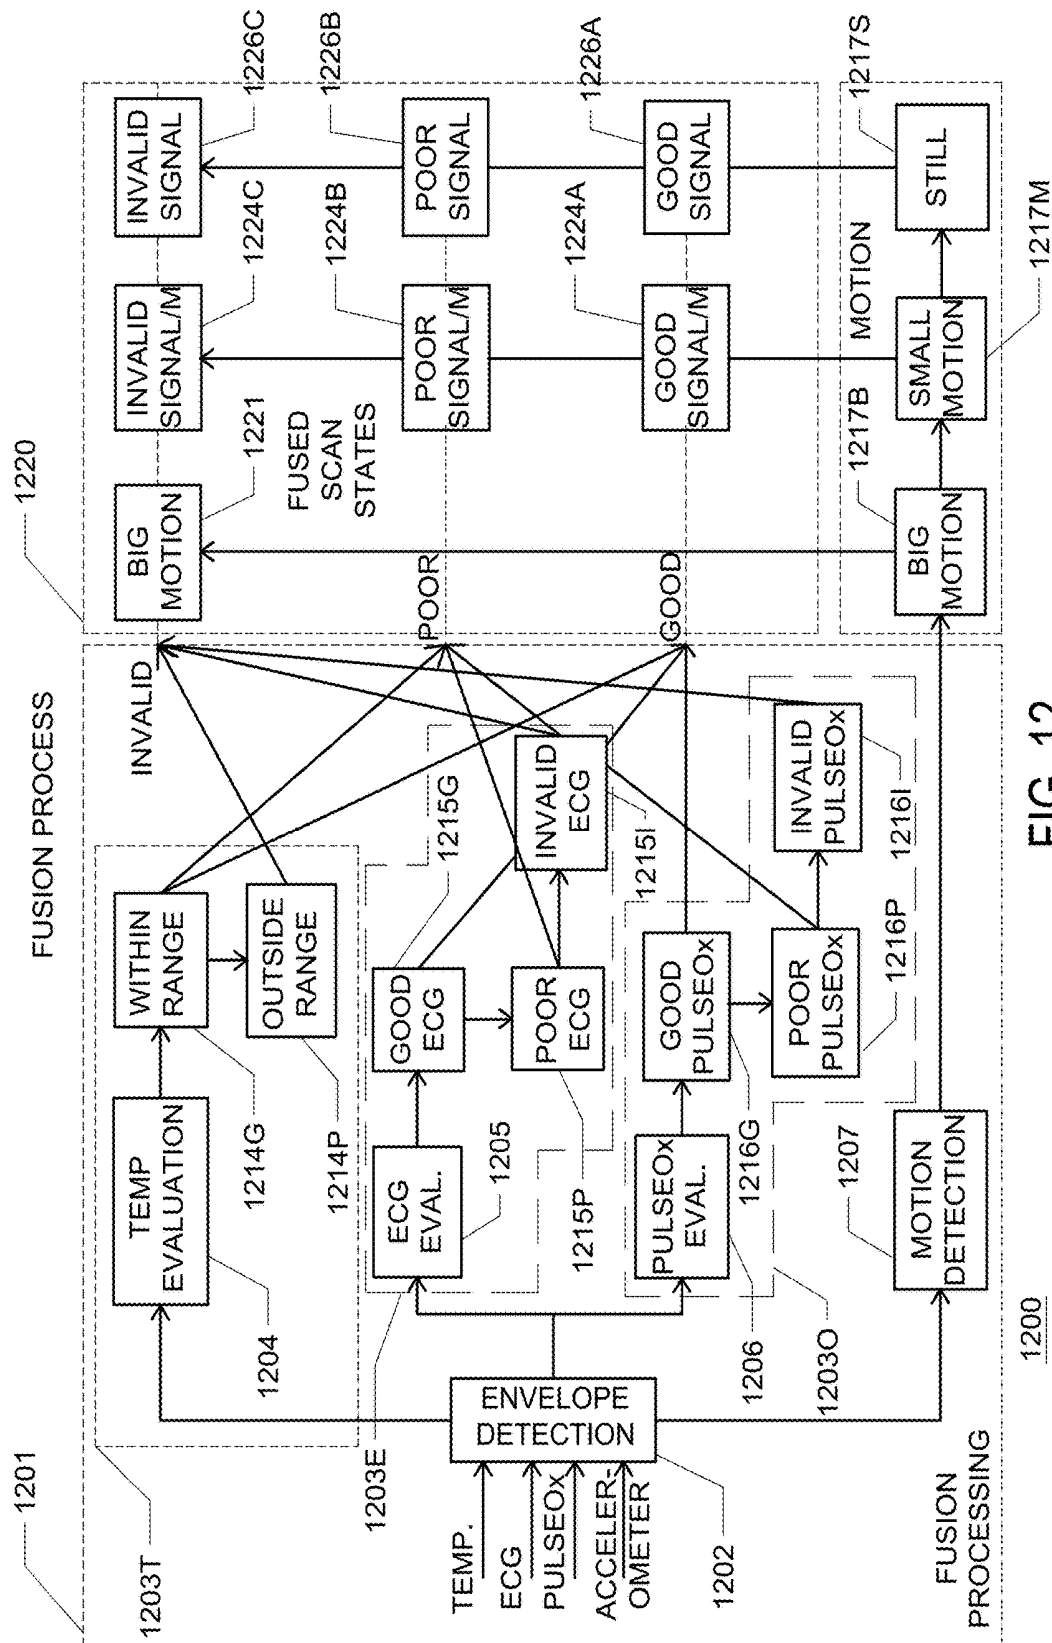


FIG. 12

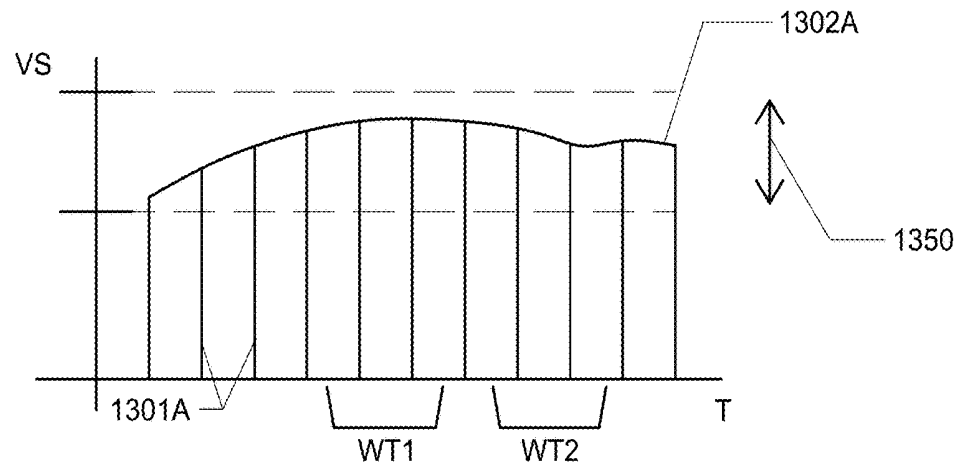


FIG. 13A

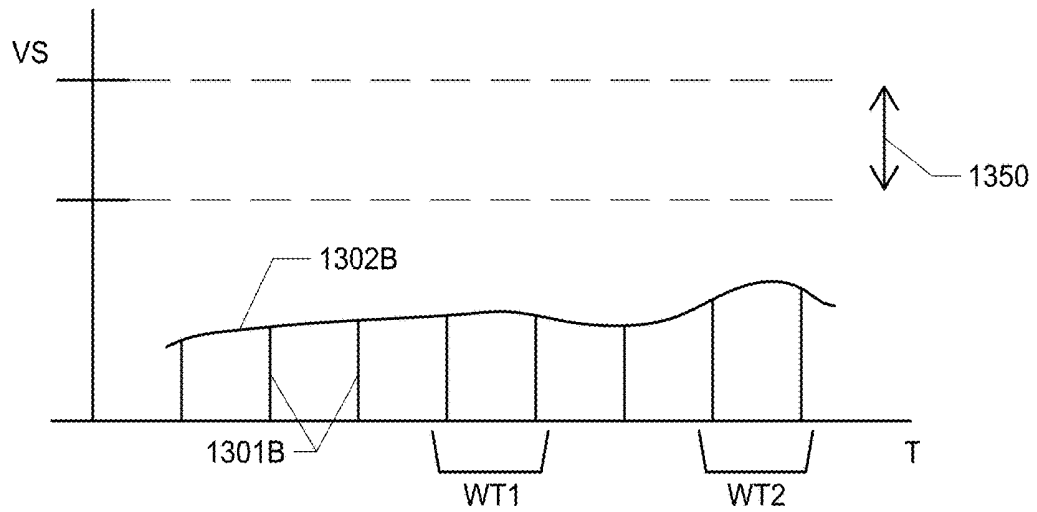
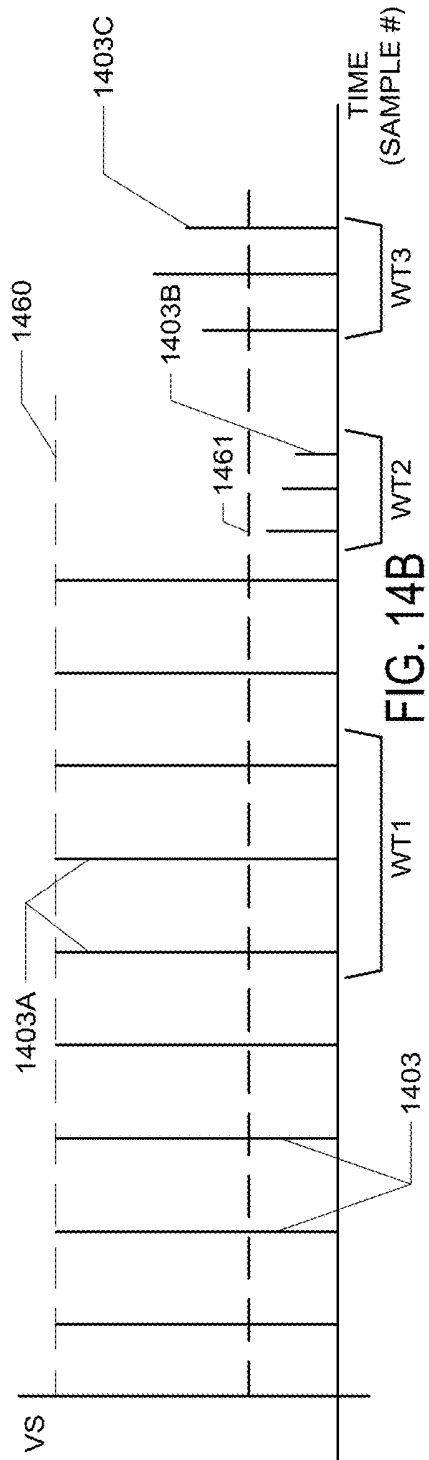
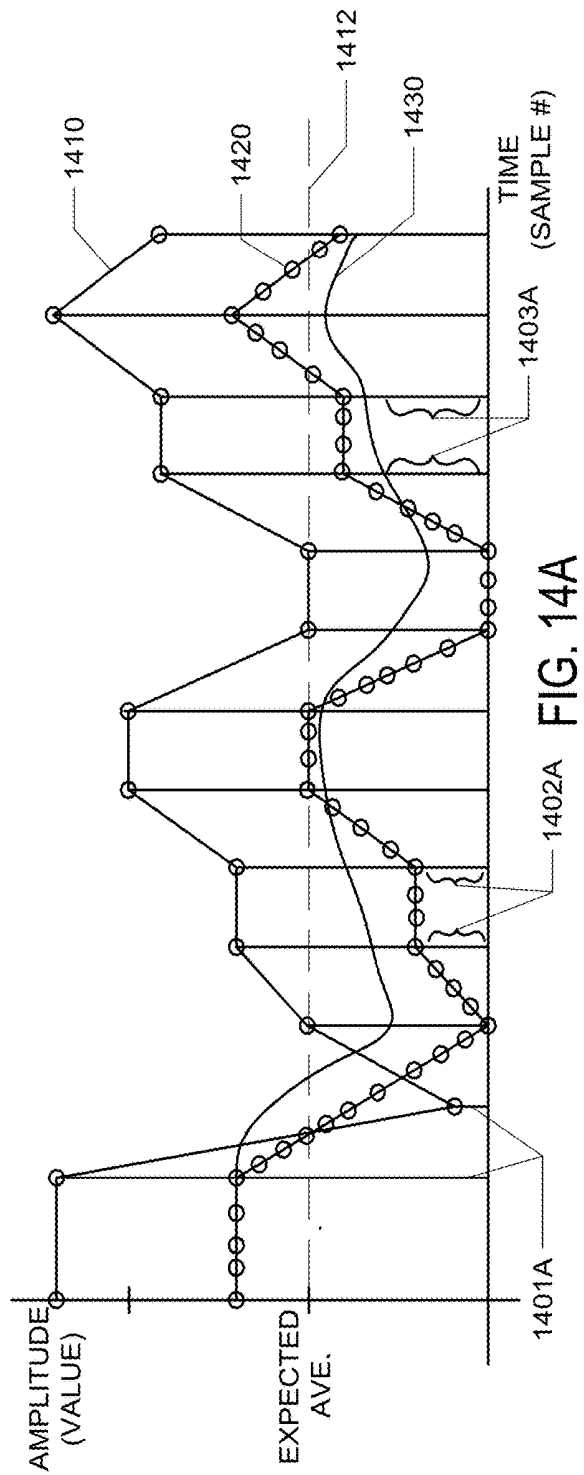


FIG. 13B



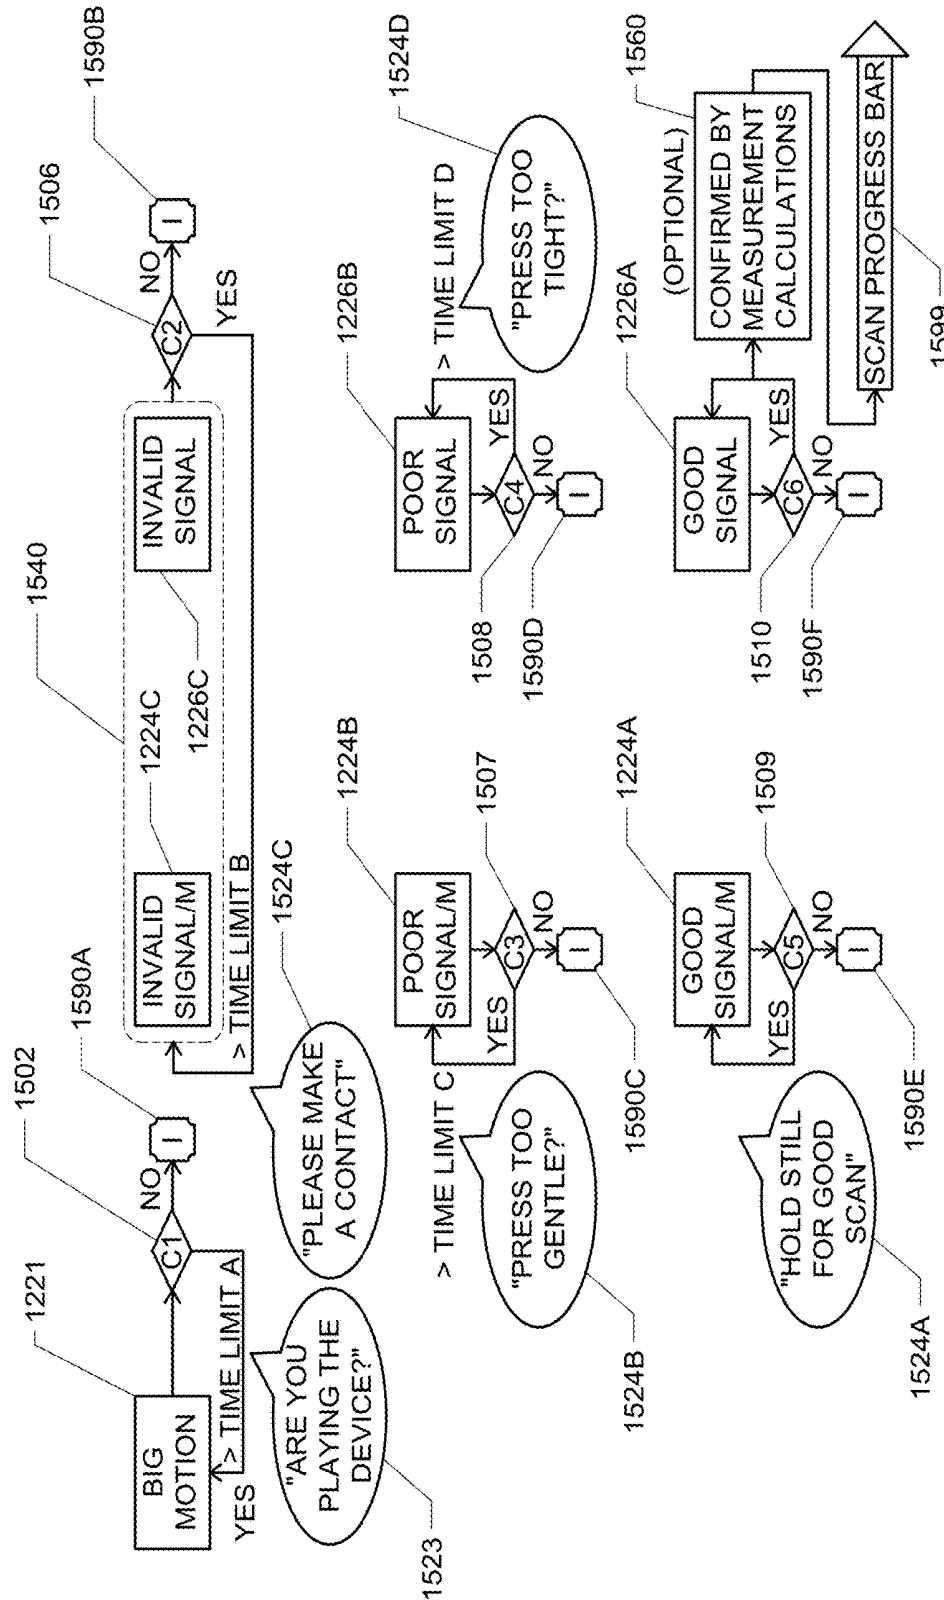


FIG. 15A

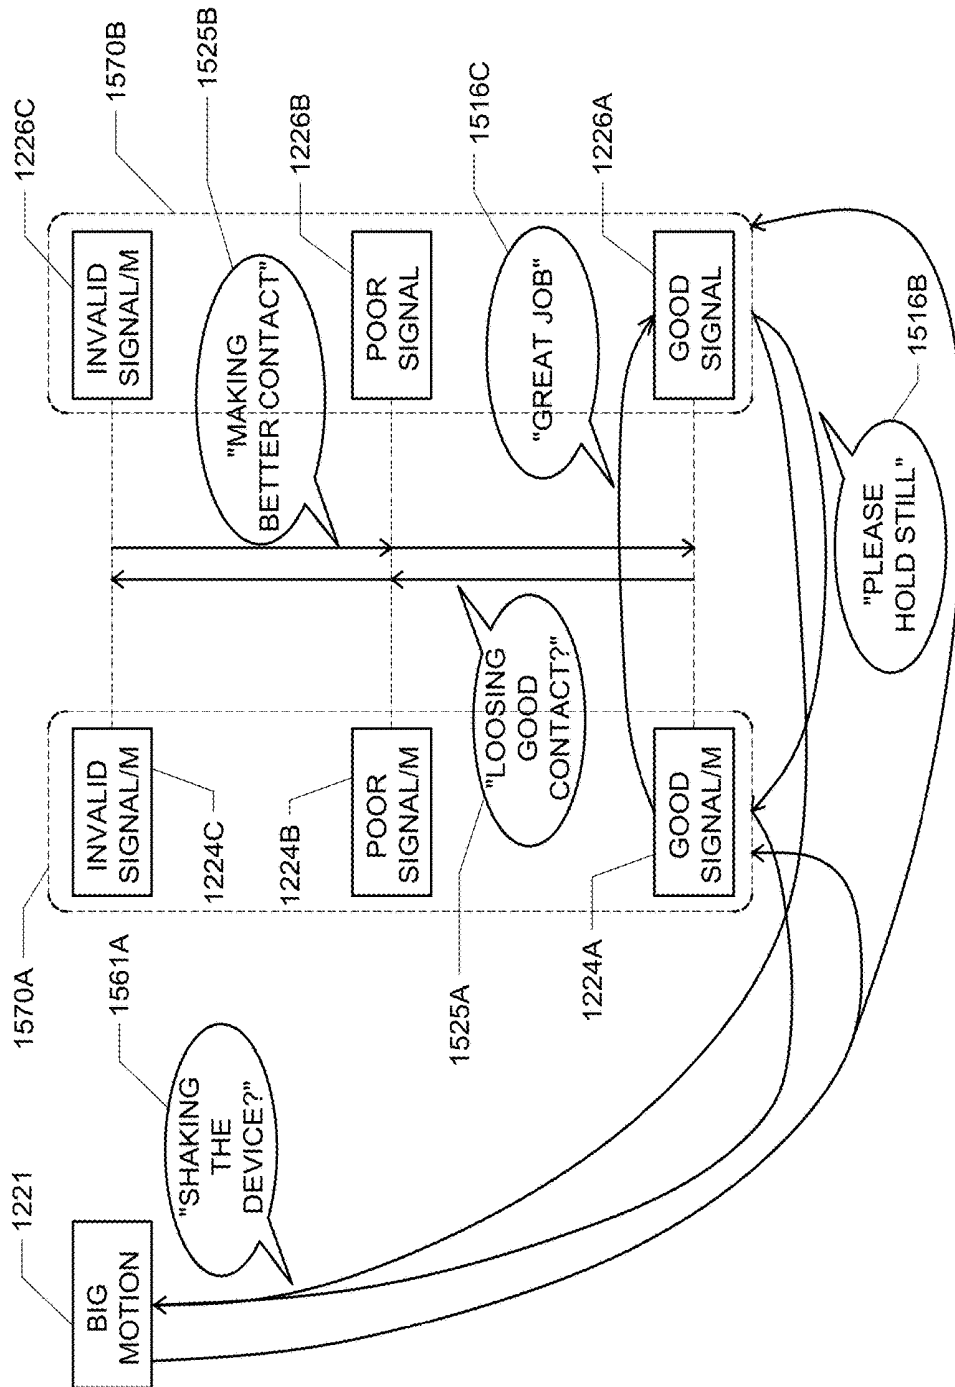


FIG. 15B

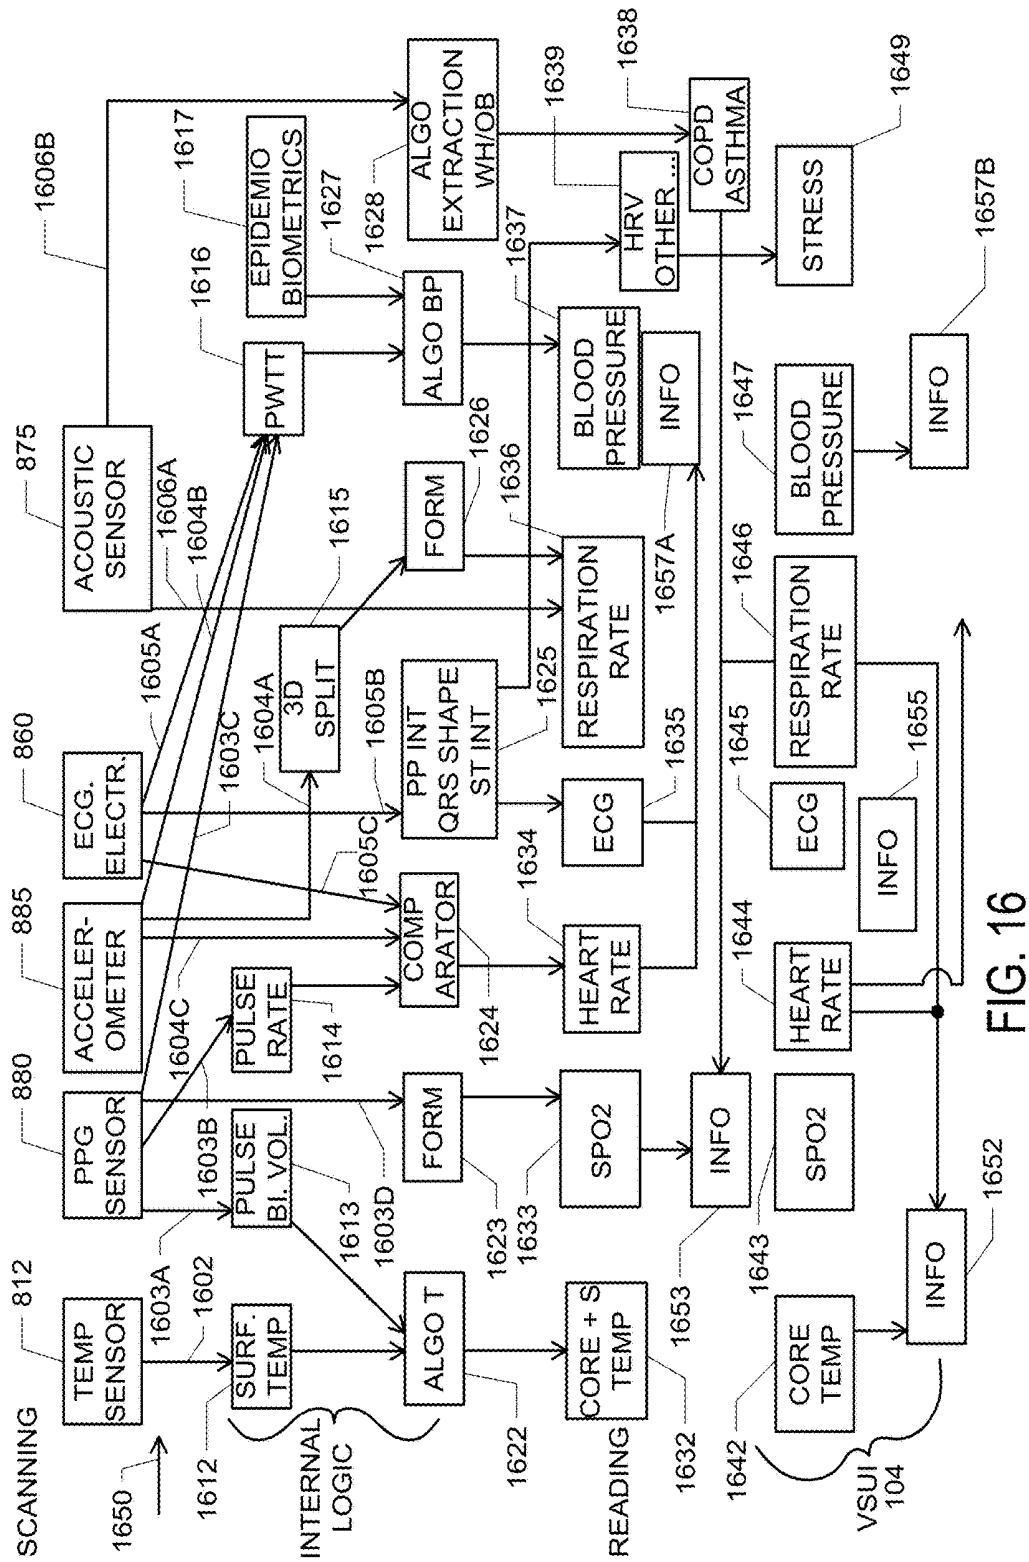


FIG. 16

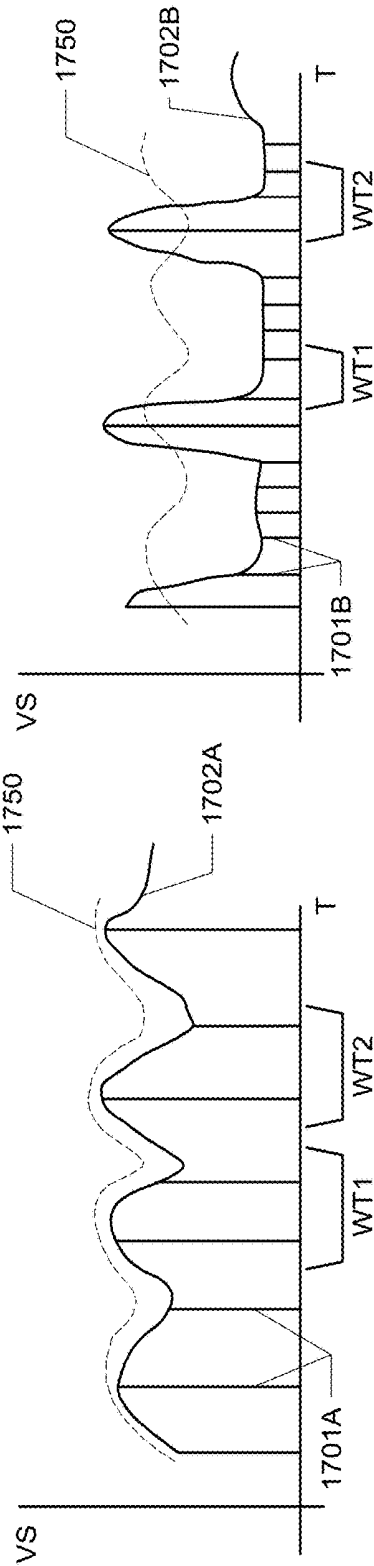


FIG. 17A

FIG. 17B

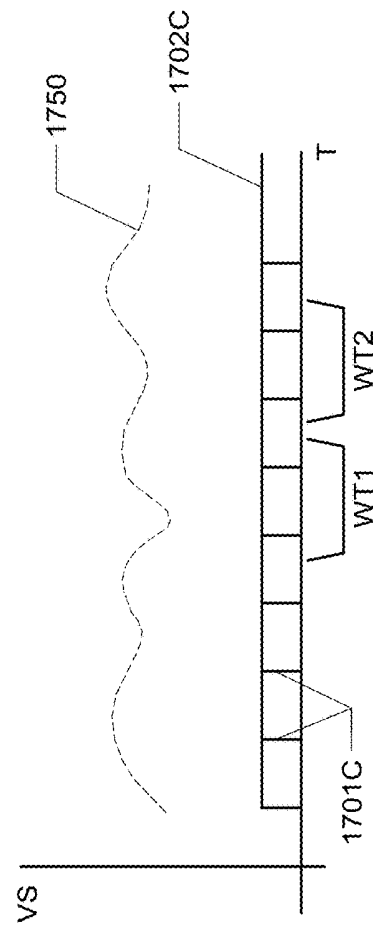


FIG. 17C

1

METHODS OF DATA ACQUISITION QUALITY AND DATA FUSION FOR PERSONAL PORTABLE WIRELESS VITAL SIGNS SCANNER

CROSS REFERENCE TO RELATED APPLICATIONS

This non-provisional patent application claims priority to U.S. provisional patent application No. 61/875,681; entitled SYSTEMS, METHODS, AND APPARATUS FOR PERSONAL PORTABLE WIRELESS VITAL SIGNS SCANNER filed by inventors Wenyi Zhao et al., on Sep. 9, 2013; and U.S. provisional patent application No. 61/924,230; entitled DATA ACQUISITION QUALITY AND DATA FUSION FOR PERSONAL PORTABLE WIRELESS VITAL SIGNS SCANNER filed by inventors Wenyi Zhao et al., on Jan. 6, 2014; both of which are incorporated herein by reference.

FIELD OF THE INVENTION

This invention generally relates to vital signs scanning with a portable device having multiple integrated vital sign sensors.

BACKGROUND OF THE INVENTION

Healthcare is a key element of any modern society. Over the years, it has brought people the benefit of the latest technological breakthroughs that are safeguarded by well-established regulatory process. The practice of medical practitioners has also evolved into highly specialized fields and subfields. One of the most important aspects of medicine is preventive care. A significant portion of healthcare costs could be reduced if ailments are diagnosed early. Yet many of the tools to diagnose early symptoms are unavailable to the average consumer.

Vital signs of one's body, such as temperature for example, form the base map of one's health. Fluctuations in our vital signs may be predictive of undiagnosed ailments. It's important to have easy access to their vital signs as frequently as needed. Yet the average consumer has no easy method of obtaining many of their vital signs without visiting a hospital or clinic. One of the easiest-to-measure vital signs is body temperature. Consumers are able to measure body temperature at home with an inexpensive home thermometer. However the average consumer still does not have easy access to devices for measuring the other important vital signs of one's body, such as blood oxygenation or blood pressure for example. The technology is available to measure the important vital signs, but typically limited to clinics and hospitals.

Consumers do not have a way to measure all of their important vital signs at home. Consumers cannot visit their physician five or more times a day to constantly monitor their vital signs. This has put the average consumer with a medical condition into a difficult situation, where they do not know what to do with their condition when they need vital signs information while at home or traveling. The few options the average consumer has with an unknown medical condition include staying calm and doing nothing, calling their primary care providers (PCP) to get an appointment, or visiting an emergency room (ER) and waiting for hours.

Even if the consumer opted to do one of the latter options, the PCP or ER may not be able to provide personalized advice without knowing the specifics about their patients.

2

The physician may have some idea about one's health condition based on an annual exam but the data may be outdated and useless with a current medical condition.

As a result, the average consumer may not receive the best medical care due to the lack of information. And together, with PCPs, we also manage to add more cost to the health-care system that is already very expensive as people live longer.

The problem, simply put, is that consumer access to basic health care is rather limited. It is desirable to improve the quality and access to basic health care for average consumers.

SUMMARY OF THE INVENTION

The embodiments of the invention are best summarized by the claims below. Insofar as a summary is required, one embodiment of the invention can be described as a portable vital signs scanner with an interactive user interface to improve scan data quality.

This summary is provided to efficiently present the general concept of one or more embodiments of the invention and should not be interpreted as limiting the scope of the claims.

BRIEF DESCRIPTION OF THE DRAWINGS

These and other features, aspects, and advantages of the present disclosure will now be described with reference to the drawings of embodiments, which embodiments are intended to illustrate and not to limit the disclosure, as are described in varying degrees of detail below.

FIG. 1A is a diagram illustrating an exemplary vital signs scanning system with the scanner held at the forehead/temple.

FIG. 1B is a perspective view of a user squeezing the exemplary vital signs scanner.

FIG. 1C is a diagram illustrating a portable wireless multifunctional device with a scan screen of a vital signs scanning user interface.

FIG. 1D is another diagram illustrating an exemplary vital signs scanning system with the scanner held at a chest position.

FIGS. 1E-1F are diagrams illustrating how microphones of the exemplary vital signs scanner can capture body sounds, such as from a user's heart or lung.

FIG. 1G is another diagram illustrating an exemplary vital signs scanning system with the scanner held in fingers of each hand.

FIG. 2A illustrates an exemplary portable wireless multifunction device to execute the vital signs scanning application.

FIG. 2B illustrates a schematic representation of the components of the portable wireless multifunctional device.

FIG. 3A is an exemplary health status window displayed on the portable wireless multifunctional device by the vital signs scanning user interface (VSUI).

FIG. 3B is an exemplary scan results window displayed on the portable wireless multifunctional device by the vital signs scanning user interface.

FIG. 3C illustrates exemplary slide windows generated on the portable wireless multifunctional device by the vital signs scanning user interface.

FIG. 3D illustrates an exemplary second scan selection window of the vital signs scanning application on the portable wireless device.

FIGS. 4A-4B illustrate a temperature averaging window generated in a touch screen of the portable wireless multifunction device by the vital signs scanning software application.

FIGS. 5A-5E illustrate prognosis windows for vital signs in a touch screen of the portable wireless multifunction device.

FIGS. 6A-6B are perspective views of an embodiment of the invention.

FIGS. 6C-6D are perspective views of another embodiment of the invention.

FIG. 7A is an exploded view of the exemplary portable wireless vital signs scanner.

FIG. 7B illustrates a partially assembled exemplary portable wireless vital signs scanner

FIG. 8A illustrates a functional block diagram of electronic circuitry within the exemplary portable wireless vital signs scanner.

FIG. 8B illustrates a main printed circuit board coupled to a daughter printed circuit board with various electronic circuitry within the exemplary portable wireless vital signs scanner mounted to each.

FIG. 9 illustrates an exemplary hierarchy of the vital signs graphical user interface provided by the vital signs scanning software application executed by the personal wireless multifunction device.

FIGS. 10A-10B illustrate diagrams of sources of movement of the vital signs scanner that can degrade data capture.

FIGS. 11A-11C illustrate diagrams of sources of various degraded quality in the capture of vital signs data by the vital signs scanner.

FIG. 12 illustrates a functional block diagram of the interactive scanning system.

FIGS. 13A-13B illustrates exemplary graphs of determining quality of vital signs data within an expected range.

FIG. 14A illustrates exemplary graphs of forming an envelope curve of vital signs data.

FIG. 14B illustrates an exemplary graph of determining quality of vital signs data with a pair of threshold levels.

FIG. 15A illustrates a functional block diagram of the interactive scanning process and user feedback (feedback to the user from the scanner and/or portable wireless device) when remaining in the same scan state.

FIG. 15B illustrates a functional block diagram of the interactive scanning process and user feedback (feedback to the user from the scanner and/or portable wireless device) when transitioning to a different scan state.

FIG. 16 illustrates a functional block diagram of the methods of data fusion for improving vital sign measurement quality.

FIGS. 17A-17C illustrates exemplary graphs to confirm the quality of vital signs data with an expected curve.

DETAILED DESCRIPTION

Many alternative embodiments of the present aspects may be appropriate and are contemplated, including as described in these detailed embodiments, though also including alternatives that may not be expressly shown or described herein but as obvious variants or obviously contemplated according to one of ordinary skill based on reviewing the totality of this disclosure in combination with other available information. For example, it is contemplated that features shown and described with respect to one or more particular embodiments may also be included in combination with another embodiment even though not expressly shown and described in that specific combination.

For purpose of efficiency, reference numbers may be repeated between the figures where they are intended to represent similar features between otherwise varied embodiments, though those features may also incorporate certain differences between embodiments if and to the extent specified as such or otherwise apparent to one of ordinary skill (such as differences clearly shown between them in the respective figures).

It is desirable for consumers to take greater control of their own basic health and work with their primary care providers (PCPs) to provide personalized healthcare. Some embodiments of the invention provide a consumer device that is small enough to be carried in a pocket or purse with which effortless vital signs scans can be performed, anytime, anywhere. The consumer device, referred to as a vital signs scanner, can transfer the vital signs results to a portable wireless multifunction device, such as a smartphone, for storage and display to a user over time to illustrate health trends. The vital signs scanner allows consumers to take greater control of their own basic health and work with PCPs to provide personalized healthcare.

The vital signs scanner allows users to efficiently measure multiple vital signs simultaneously. Vital signs scanning with the vital signs scanner is quick and easy and very convenient in that it can simultaneously capture a plurality of vital signs data with one scanning session (one or two vital signs scans) at a given time and date. The vital signs data is transferred to a user's own portable multifunction touch screen device, e.g. a smart phone. The portable multifunction device, with the assistance of vital signs scanning software, displays the scanning results in an intuitive user interface that is simple to understand.

The vital signs scanning device provides a method of vital signs scanning to help solve the missing information link so a user can take control of managing his/her own health. In addition to providing vital signs scanning, the vital signs scanner and system also stores the users vital signs measurements and trends over time of a day and date. The vital signs scanner and system provides easy access (almost anywhere at anytime) to important vital signs measurements such as blood oxygenation, blood pressure, heart rate, etc. The vital signs scanner and system can help share up-to-date vital signs data with a user's PCP for better diagnosis of medical conditions. Perhaps even more importantly, sharing of history and trends of vital signs data before and after an ailment with the user's PCP can provide clues to its cause and not just indicate the symptoms.

The personal wireless vital signs scanner combines aesthetic design with functionality. The personal wireless vital signs scanner is light weight and easily fits into one hand (e.g., handheld). The personal wireless vital signs scanner can be held and operated with just two fingers of one hand. The user's other hand is free to hold a smartphone with a vital signs scanning application running to control the vital signs scanning process and view the scanning results. Vital signs data of a users body can change at different times of each day. The personal wireless vital signs scanner is so small, light, and esthetically pleasing that a user may desire to take it with them to perform a plurality of vital signs scans at different times throughout his/her day over a plurality of days.

The vital signs scanner may fuse data together from various data sources, referred to as a fusion process, in different ways in order to increase measurement accuracy, increase quality control of data acquisition, and/or provide additional information to a user. The data that may be fused together includes concurrent information or data streams

originating from different sensors in the vital signs scanner; different information in a data stream originating from the same sensor; information in an internal data stream from a sensor in the vital signs scanner and external generated data, such as data originating from a user's input, biometrics or one or more databases; or any combination thereof. To facilitate the fusion process, the data streams may be split, independently processed in parallel, and recombined or compared against each other depending on the needs for the information. For example, a fusion process may involve comparing scan data in independent data streams from a plurality of sensors to cross-validate the quality of their scan data.

A portable vital signs scanner and system may prove to be useful for healthcare professionals as well. For example, patients could scan for their own vital signs themselves in a busy hospital, clinic or doctors office, rather than wait in long lines just to get a simple checkup before seeing the doctor. The patients scans are then uploaded to a server at the hospital, clinic, or office. With these self-obtained vital signs scans of patients being uploaded to a server, medical assistants and nurses, ordinarily checking for vital signs, can better spend their time curing the ailments of the patients.

The self-obtained vital signs scans of patients may also serve to triage the patients that are waiting for medical care. For example, a self-obtained vital signs scan of a patient indicating an elevated or irregular heart rate may signal hospital staff to attend to this patient immediately or at least a higher priority in a queue of patients. In this manner, the self-obtained vital signs scans of patients provide a clinic staff with a sense of the severity of the condition of patients waiting and can make appropriate schedule priority adjustments, if needed.

Referring now to FIG. 1A, a diagram illustrating a vital signs scanning system **100** is shown. The scanning system **100** includes a portable wireless vital signs scanner **102** and a portable wireless multifunction device **104** in wireless communication with each other over a wireless communication channel **103A**. The vital signs scanner **102** includes a plurality of sensors designed to read vital signs from a user's body **101**. An instance or snap shot of vital signs, such as temperature, heart rate, blood oxygenation (SpO₂), electrocardiogram (ECG), and possibly stress levels, all synchronously measured, can be reported to the device **104** by the scanner **102** in less than a minute. Exemplary methods and algorithms for determining one or more of these vital signs from the sensor data are described in International Application No. PCT/US2013/061046, filed by Scanadu Corporation on 19 Oct. 2012, having international publication no. WO 2013/066642, entitled AUTOMATED PERSONAL MEDICAL DIAGNOSTIC SYSTEM, METHOD, AND ARRANGEMENT, claiming priority to U.S. Patent No. 61/549,134 filed on 19 Oct. 2011, and is hereby incorporated by reference.

The algorithms and processes disclosed in International Application No. PCT/US2013/061046 are based upon one or more of the following references (all of which are incorporated herein in their entirety): *Pulse transit time: an appraisal of potential clinical applications*, Thorax 1999; 54:452-457 [doi:10.1136/thx.54.5.452] [http://thorax.bmj.com/content/54/5/452.full]; U.S. Pat. No. 6,723,054; U.S. Pat. No. 6,527,728; U.S. Publication No. 2007/0276632; and U.S. Publication No. 2003/0199771; Severinghaus, John W., Honda Yoshiyuki (April 1987), "History of Blood Gas Analysis. VII. Pulse Oximetry", Journal of Clinical Monitoring # (2): 135-138; Millikan G. A. (1942). "The oximeter: an instrument for measuring continuously oxygen-saturation

of arterial blood in man", Rev. Sci. Instrum 13 (10): 434-44 [doi:10.1063/1.1769941]; U.S. Pat. No. 6,385,471; U.S. Pat. No. 5,934,277; U.S. Pat. No. 5,503,148; U.S. Pat. No. 5,351,685; U.S. Pat. No. 5,259,381; U.S. Pat. No. 4,883,353; U.S. Pat. No. 4,824,242; U.S. Pat. No. 4,807,631; U.S. Pat. No. 4,796,636; U.S. Pat. No. 4,714,080; U.S. Pat. No. 4,623,248; and U.S. Pat. No. 4,266,554.

Integration of multiple sensors and scan quality algorithms make it possible to monitor the quality of the scanning process and then provide feedback to the user to control the interactive scanning process and provide a good user experience in the vital signs scanning process. As used herein, user feedback means feedback provided by the scanner and/or portable wireless device through the user interface or otherwise to the user, including any scan quality feedback that is provided to the user. User input means any input that a user provides to the scanner and/or portable wireless device.

The wireless vital signs scanner **102** may perform vital signs scans and display the results in under a minute. Generally scans may be completed in approximately ten seconds. The length of a scanning session may depend on the user's ability to correctly utilize the scanner **102**. For example, if the user moves too much during the scanning session, the session will last longer as the device **104** prompts the user to remain still.

Different types of scans may also take different lengths of time. For example, in a standard ten second head scan where the scanner is held against a user's forehead or temple (forehead/temple), temperature, SpO₂, ECG, heart rate, and blood pressure may be measured. For a thirty (30) second extended head scan, vital signs such as blood pressure and heart rate variability (related to emotional stress) may be captured. For a thirty second chest scan from a user's chest, respiration rate and body sounds may be measured or collected. In any case, the scanning sessions are still short and convenient.

Short scanning sessions have several advantages. A short scanning session allows a user to take a quick break from their daily activities to perform a scan anywhere and at any time. The ease and rapidness of performing a vital signs scan will encourage users to perform the scan multiple times a day, providing more complete and accurate trending data. The invention provides a consumer oriented scanner that a user can use anytime anywhere to obtain multiple vital sign measurements in seconds.

Short scanning sessions also conserve power. With ten second scans, the scanner may last approximately one week under normal usage with one full battery charge. If the power is on for a total of about 30 seconds for each scan, then total power-on time for each day is less than one hour with 100 scans per day. In this case, the scanner **102** may operate for a week at a time between battery recharging sessions.

Scanner **102** is an elegant consumer device that is portable. Unlike other vital sign monitors, scanner **102** does not need to be worn. Scanner **102** is perhaps the smallest consumer device that can measure multiple vital signs simultaneously. Measuring approximately 60 mm in diameter and 18 mm high, the scanner **102** can be easily places in a pocket or purse for use at any time convenient to the user. At any time the user has a moment to spare, the scanner **102** may be used to obtain multiple vital sign measurements by simply finger-holding it against the user's forehead/temple, and/or chest.

Using a multifunction device **104** to display the vital signs scanning results allows the scanner **102** to maintain a

compact size and minimalist form. Multifunction device **104** may be any portable wireless multifunction device such as a smartphone, tablet PC, or the so called smart watches. Generally these devices are pre-owned and already available to the average consumer, so utilizing the display capabilities of multifunction device **104** does not detract from the portability of the invention. The ubiquity of smartphones also means that the average consumer does not need to pay more for a dedicated display device. Combining the vital signs scanner **102** with, a smartphone that a user already has, allows one to take control and greater responsibility for his/her health without sacrificing valuable time and money.

To display the vital signs scanning results, the portable wireless digital device **104** executes a vital signs scanning software application **140**. The instructions of the vital signs scanning software application **140** are executable with the operating system, (e.g., Android and iOS), of the multifunction device **104**. Once the software application is active, the user may power up the vital signs scanner **102**. Upon power up, the vital signs scanner **102** is paired with the portable wireless digital device **104** to form the communication channel **103A** between them. Accordingly, each of the scanner **102** and multifunction device **104** has a compatible wireless radio to form a compatible wireless communication channel. In one embodiment, the communication channel **103A** is a Bluetooth version 4, a smart low energy (LE) supported channel that each wireless radio supports. The vital signs scanner **102** sends the vital sign information wirelessly to the portable wireless multifunction scanner **102** over the wireless communication channel **103A** for storage and further analysis.

With the communication channel **103A** available, the vital signs scanner **102** is pressed against a user's forehead/temple. The forehead/temple is identified as the single place with enough blood vessels and thin skin so that temperature, pulse oximetry and ECG can be obtained in sync and time-stamped. A scanning button is pressed on the user interface of the application **140** of the portable wireless multifunction device **104** to start the scanner **102** scanning for vital signs information of the user. After scanning for approximately 10 seconds or less, the vital signs scanner **102** sends the vital sign information wirelessly to the portable wireless multifunction device **102**. The multifunction device **104** may display the results of the scan on a touchscreen display.

The vital signs scanner **102** is used periodically to scan for vital signs each day. Statistical information regarding a plurality of scans each day over a plurality of days can be generated and displayed on the touchscreen display device of the device **140**. The vital signs scanning software application **140** informs a user of how those vital sign measurements may change during times of a day and over a plurality of days.

An important aspect of the invention is the quality of the scanning results. To optimize the scanning session results, the scanner **102** is designed to be easy to use to minimize user error. Similarly, the scanning software application is intuitive and easy to use. With minimal instruction, an average user can generate medical grade vital signs scans within minutes of using the invention for the first time.

To further optimize scanning results, scan quality algorithm monitor the vital signs scanning process and provides feedback (visual and/or audible) to the user through the multifunction device **104**, and/or alternatively an optional sound generator (see audible sound generator **847** in FIGS. **8A-8B**) in the scanner **102**. The user feedback may help the

user to perform a better vital signs scan with the wireless vital signs scanner and acquire good quality vital signs measurements.

Integration of multiple sensors allows for synergistic accuracy of vital signs scans. For example, integration of an accelerometer enables motion detection that is often associated with poor signals of pulse oximetry and ECG. In another example, abnormal signals of both pulse oximetry and ECG suggest the device is not held against the body properly. This can be further confirmed by comparing the surface temperature and ambient temperature of the sensor when not in touch with the user.

Quality checking of individual vital sign measurements is based on fusion of data from multiple differing sensors, including a motion sensor, such as an accelerometer. Signal quality may be checked based on dynamic range detection and thresholding, for example. To make the process more robust, known signal processing techniques, such as envelope detection, can be applied to the raw signals from the sensors as a preprocessing or screening step. Quality checking of raw sensor signals from the sensors makes sensor data fusion more robust by rejecting bad signals. Thus, fusing results of multiple sensors can provide better individual measurements of each vital sign.

The intuitive scanning user interface (UI) is designed, in combination with scan quality algorithms and the device's self-diagnostic capability, to help users to finish a vital signs scan successfully. There is the quality indicator from the quality algorithm, the progress bar, and texts that provides feedback to the user to ensure a successful scanning session. For example, suggestions to "hold still" or "hold device to your forehead/temple" may prompt the user to correct his/her poor scanning behavior.

The scanning system **100** is user friendly so that it can be used multiple times during the day to obtain data about a user's body **101**. One person or one family can exclusively use the scanning system **100** and scanner **102** at home as a personal vital signs scanner. In this manner, a measure of one's personal health and medical data can be obtained right at home with the scanning system **100** without seeing a doctor or being admitted to a hospital. Each scan only lasts approximately ten to thirty seconds and obtains multiple vital signs measurements so users can take the scan repeatedly throughout the day without being inconvenienced.

The scanning system **100** can be used to personally analyze and track one's own vital signs to see various trends over time. Accordingly, the vital signs data can be accumulated over a plurality of days and a plurality of scans at various times each day, then stored in non-volatile manner with the device **104** so the data does not get lost. The vital signs data can also be backed up to a computer, a storage device, or storage server so it is not lost if the device **104** is lost or stolen. The storage server having greater storage may also be used to accumulate one's user data over a plurality of years when the device **104** is limited by its built-in storage capacity.

In operation, the vital signs scanning system **100** forms an electrical circuit **150** with the user's body **101**. The circuit **150** is formed between first and second electrodes of the portable wireless vital signs scanner **102**. From a first electrode of the scanner **102**, the circuit **150** is made with the fingers **111**, the hand **112**, the arm **113**, the chest **114**, the neck **115**, and the head **116** of the user's body **101** to a front electrode. Preferably, the portable wireless vital signs scanner **102** forms an electrical connection to the forehead/temple portion of the head **116** of a user's body **101**. Fingers **111** not only serve to hold the scanner **102**, but also as one

contact point for one-lead ECG (the other one-lead ECG contact point is forehead/temple). Preferably the thumb finger **111** in one embodiment and the index finger in another embodiment forms an electrical connection with the portable wireless vital signs scanner **102**.

The vital signs scanning system **100** may optionally include a personal computer **150** in wireless communication with the portable wireless vital signs scanner **102** over an alternate or additional wireless communication channel **103B**.

Referring now to FIG. 1B, a perspective view of a user's fingers **111A-111B** squeezing the vital signs scanner **102** is shown. The vital signs scanner **102** is squeezed between the user's fingers to form at least one electrical connection. The front side sensors and a front electrode in the vital signs scanner **102** are then pressed against the user's forehead/temple to form an additional electrical connection. The small size 60 mm×60 mm×18 mm allows the scanner **102** to be held by just two fingers of one hand. At a weight of approximately 60 g (e.g., less than one pound), the scanner **102** may be used by just about any person, from a child to the very elderly. Finger-held form-factor, ten to thirty seconds per scan, scan quality algorithm with feedback and an intuitive scanning user interface on a personal portable multifunction device, all help make vital signs scanning fast and easy while producing quality results.

Preferably, the scanner **102** is held between the thumb **111B** and forefinger **111A** of the user's left hand. The forefinger **111A** may also rest over a sensor **121** and forms an electrical connection to an electrode around the sensor in one embodiment. In another embodiment, the thumb finger **111B** makes contact with a bottom electrode **122B**. The thumb of the left hand couples to the bottom electrical contact (electrode) on the bottom-housing portion of the scanner.

The forefinger makes contact with a rectangular glass plate over an oximeter sensor **121** in one embodiment. In another embodiment, the oximeter sensor **121** is moved to the front side of the vital signs scanner **102** so that extraneous light is less likely to interfere with the its readings.

A front side electrode **122F** makes contact with the user's forehead or temple (forehead/temple), when it is pressed up against his/her head. An infrared (IR) thermometer sensor is combined with the front side electrode **122F**. The IR thermometer sensor makes temperature readings at the user's forehead/temple. An oximeter sensor may also be located near the front side electrode **122F**.

With the thumb finger **111B** in contact with the bottom electrode **122B**, a circuit may be formed through the finger and the hand of the user and a portion of his body back to the front side electrode **122F** in the vital signs scanner **102**. Once proper placement of scanner **102** is made, a scan button is selected in the software application **140** of the device **104** to command the scanner to scan the vital signs from the user's body and forward them to multifunction device **104**.

Referring now to FIG. 1C, an exemplary initial scan screen window **140A** of the vital signs scanning application **140** is illustrated. The initial window **140A** includes an instruction scan messaging **147** with instruction scan message text and optionally an instruction figure to show the user how the vital signs scanner **102** is utilized. As indicated by the instruction scan message, the user is to keep holding the scanner to the user's left temple for the best scan.

The initial window **140A** further includes a menu button **161**, a back button **162**, an edit button **163D**, a tag information button **164**, a health status button **180**, and a done

button **190**. The tag information button **164** is used to add user information as well as tag scans with the circumstances under which a scan was undertaken, such as after eating or after exercise. The initial window **140A** includes a user information bar **163** including information regarding a user's height, user's name **163B**, user's weight **163C**, and a user's profile picture **163E**. In this manner, the user is clear as to whom is logged into the vital signs scanner user interface and for who's body is to be scanned. The initial window **140A** further includes a scan type indicator **173**, indicating a head scan type during a first scanning or a chest scan type during a second scanning period. The initial window **140A** further includes a scan quality indicator **175**, a scan progress bar **146**, and a scan progress percentage indicator **146**. The scan quality indicator is one form of quality feedback that may be employed by the scanning system to inform and train the user to acquire better scan data. The initial window **140A** further includes a scan type slider **171** to select the type of scan that is to be performed. The menu button **161** can take the user to the next screen or a different screen within the vital signs scanning user interface. The edit button **163D** can edit information and select options that are available in the vital signs scanning application **140**.

The vital signs scanning application **140** may include an option to enter the user's symptoms by selecting the health status button **180**. A photo may also be taken of the medical condition of a user by use of a camera in the device **104** and a photo button. Additionally, a user may add a note to his health status using the device **104** and an add note button.

The status of the scanner **102**, such as powered on/off, Bluetooth connection, battery charge status, and/or ready to scan, may also be displayed in one or more of the user interface windows of the vital signs scanning application **140**.

The scanner **102** can collect a diverse set of physiological information (e.g., vital signs) during one or two acquisition periods totaling approximately sixty seconds (head scan, extended head scan, and/or chest scan).

Referring now to FIG. 1D, a diagram of an exemplary vital signs scanning system with the scanner held at the chest position is illustrated. In this embodiment, vital signs are first acquired from a first scanning period (e.g., approximately 10-second scan) at the forehead/temple as shown in FIG. 1A. Vital signs may further be acquired by secondary scans. A longer or extended scan at the forehead/temple with the scanner **102** may be used to capture sensor data as shown in FIG. 1A during a second scanning period. Alternatively or additionally, a subsequent scan conducted near the chest of the user may be performed during another scanning period, such as shown in FIG. 1D.

A secondary extended scan at the forehead/temple may be over a range of time from about thirty seconds up to a minute so that measures of heart rate variability and respiration rate may be obtained. The secondary extended scan at the forehead/temple can also provide for a more robust and accurate measurement of blood pressure. In terms of using the scanner, the primary and secondary scans at the forehead/temple may occur in one single scan (e.g., 10-second or 30-second) or two separate scans (e.g., a first at 10 seconds and then a second at 30 seconds).

The secondary extended scan near the chest, a chest scan, is mainly to capture vital signs of respiration rate and additional physiological information from the captured body sounds. The vital signs scanned at the chest area may also include heart rate variability. Noise may also be captured in the signals captured by the sensors of the scanner that can be

used to better extract the desired signal data. The secondary extended scan near the chest may last for a period from thirty seconds to a minute. The vital signs scanning application executed on the multifunction device **104** may prompt the user for one or both scan locations.

The secondary chest scan can be selected by the scan type slider **171** shown in FIG. 1C. A second or third scan may be selected with a finger swipe to perform the second scan or the third scan at the chest of the user. If only the first head scan was desired, a done button **190** may be selected to avoid the secondary scans. This may be because its inconvenient due to timing or to perform against ones chest with the vital signs scanner, such as when it is inconvenient to do so in public.

As mentioned herein, a chest scan may be performed with the scanner **102** as shown by FIGS. 1D, 1E, and 1F, for example. In FIG. 1D, a second circuit **150'** may be formed with the users body **101** between the electrodes of the scanner **102**. The second circuit **150'** in this case includes the chest **114**, the arm **113**, the hand **112**, and the finger **111** of the user.

In an alternate embodiment, another circuit **150''** may be formed with the users body between the electrodes of the scanner **102** while the device **104** is nearby. This alternate circuit **150''** is formed by fingers on different hands coupling to the electrodes of the scanner **102**. A left finger **111L** may couple to a bottom or top electrode in the scanner **102**. A right finger **111R** may be coupled to the front electrode of the scanner **102**. From a left finger **111L** in a left hand **112L** of the user, the circuit in the body includes, the left finger **111L**, the left hand **112L**, the left arm **113L**, the chest **114**, the right arm **113R**, the right hand **112R**, and a right finger **111R**, such as shown in FIG. 1G, to complete a circuit with the scanner **102**.

In either case, the ECG circuitry in the scanner **102** may then obtain further data regarding heart activity of the user that can be combined/fused with the heart activity data of a first scan, to improve the measure of vital signs of heart activity. The vital sign measures of heart activity may then be sent to the device **104** for display to the user on its built-in touchscreen display.

Temperature of the body adjacent the user's chest **114**, if reliable, may also be used by the scanner to improve scanning results of temperature. Temperature at the user's finger **111R**, if reliable, may also be used by the scanner to improve scanning results of temperature.

With the scanner adjacent the users chest, near or over the heart during the chest scan, clothed or unclothed, an accelerometer (see accelerometer **885** in FIGS. 8A-8B) in the scanner **102** may be used to capture movement of the chest as a measure of respiration rate. The vital signs data from these measures are computed by the processor **840** and then sent to the device **140**. With the accelerometer within the scanner **102**, data for measuring heartbeat and respiration rhythm can be acquired over clothing, without the user needing to undress. Heartbeat and respiration rhythm based on scan data from the accelerometer has the added advantage of allowing cross-correlation with other data streams from other sensors.

FIGS. 1E and 1F illustrate the use of the microphones **875** in the scanner **102** to capture body sounds around the chest **114**, such as heart sounds **155** and lung or breathing sounds **157**. These body sounds may be recorded to capture another symptom of a user's medical condition. Body sounds that are captured may also be used to judge the quality of the vital signs scanning process. The recorded body sounds may be

stored locally in the memory of the scanner and/or sent to the device **140** for storage with the vital signs data of the same time and date.

Scan data captured by the scanner may provide person-specific biometrics information. Phase spaces (poincare plots) of accelerometric data can provide an element of person-specific biometric data, an identification linked to person specific noise in the acquired signals. Using chaos mathematics and various analytic tools on cross-correlated or uncorrelated data streams from the human body, it is possible to obtain positive identification of any user linked to each person specific noise in the acquired data signals. This noise originates in the numerous minor and major anatomical and functional differences between the various users. The noise being person-specific acts like electronic fingerprints of a user.

Referring now to FIG. 2A, a portable wireless multifunction device **104** is illustrated that can execute the vital signs scanning application **140**. The portable wireless multifunction device **104** includes a text screen **202**, at least one function button **206**, and a power button or switch **207**. The multifunction device **104** may display a plurality of application icons on the touch screen **202**. One of these icons may be the vital signs scanning application software icon **140**.

Referring now to FIG. 2B, a block diagram of the personal wireless digital device **104** is illustrated. The portable wireless multifunction device **104** may be a smart phone, a tablet computer, a portable music player, or a wireless portable storage device, for example, that include a processor, a touch screen, and a memory from which application software instructions may be executed.

As shown in FIG. 2B, the portable wireless multifunction device **104** includes a touch screen monitor **202**, one or more wireless radio transmitters-receivers (wireless radios) **204A-204M** coupled to their respective antenna **205A-205M**, a processor **206**, non-volatile memory **208**, at least one function button **206**, and a cover button **207** that can switch power on to each electronic circuit within the portable wireless multifunction device **104**. At least one of the wireless radios **204A-204M** are compatible with the wireless radio in the wireless vital signs scanner **102**.

The portable wireless multifunction device **104** may further include a camera **214**, a microphone **215**, and a speaker **216** coupled to the processor **206** as shown. Furthermore the portable wireless digital device includes a battery **210** coupled to the power button **207**. Typically the battery **210** is a rechargeable battery such that an external power source may be coupled thereto via an external power connector **211** and a charge circuit **209**.

Non-volatile memory **208** of the personal wireless digital device may store the vital signs scanning application software **140** and data **220** related to the vital signs scan application software. The processor **206** can read and write to the non-volatile memory such that the vital signs scanning application software can provide a user interface to a user via the touch screen display device **202**. As discussed previously, the initial vital sign scanning window **140I** may be provided as shown in FIG. 1C.

The camera **214** of the portable wireless digital device **104** may take photographs of a user's conditions or symptoms via the photograph entry button **175** of the user interface. The photographs may be stored as part of the data **240** in the non-volatile memory. The microphone **215** in the portable wireless multifunction device **104** may optionally be used to capture body sounds similar to the microphones in the scanner **102**, as is shown in FIGS. 1E-1F.

The speaker **216** of the portable wireless digital device **104** may optionally be used to provide audible user feedback to the user of the vital signs scanner **102** to improve the vital signs scan quality as is discussed herein.

Referring now to FIG. 3A, an exemplary scanning window **140A** is shown being displayed by the touch screen display device **202** of the portable wireless multi-function device **104**. The scanning application software **140** generates the various images consisting of a scanning progress bar **310**, a scanning icon **312**, a first vital signs graph **314A**, a second vital signs graph **314B**, one or more result buttons **320**, and one or more status icons **324**.

The status icon **324** may be a wireless connection status icon indicating that the portable wireless digital device **104** is connected to the vital signs scanner **102**. The button **320** may be a results button to which to switch to another scanning window/screen of a user interface provided by the scanning application software **140**. The scanning icon **312** may include the plurality of color bars **312A-312E** that randomly vary in color and length to indicate that scanning is occurring. The scanning progress bar **310** illustrates the progress of the scanning session being performed by the portable wireless vital signs scanner **102**. In this case data is being sent from the scanner **102** to the portable wireless multifunction device **104**.

Briefly referring back to FIG. 1C, the initial window **140A** includes a user menu button **161** that may be used to display a users menu on how to operate the vital signs scanner. The initial window **140A** may further be changed to a graph window to show plots of prior scan data stored in the device **104**. A graph button may be provided to do so or a finger swipe may be used.

The first vital signs can be displayed in graph form over different day granularity such as 1 day, 1 week, 1 month, 3 months, 9 months and 1 year. Graphs may be electrocardiogram (ECG) graphs to illustrate the electrical activity to show the user's heart rate or heart rate variability. The waveforms displayed in the graphs are captured by the scanning process of the portable wireless vital signs scanner **102**. A second vital signs graph may be oxygenation graph related to photoelectric plethysmogram (PPG) from the data obtained by the pulse oximeter. The scanner captures a user's blood volume pulse of both oxygenated and deoxygenated blood. From the photoplethysmography waveforms (oxygenated and deoxygenated) a user's oxygen saturation can be obtained and displayed in the oxygenation graph.

Referring now to FIG. 3A, a health status window/screen **140B** of the user interface software **140** is shown being displayed by the touch screen display device **202** of the device **104**. The screen **140B** includes a number of similar items illustrated in screen **140A** of FIG. 1B and are not repeated here. The health status slider window/screen **140B** (it can be slid sideways) includes a health status button **180**, a health status window **181**. The health status slider window **181** includes a display of a health status question **182** to obtain further information from a user. To respond, the health status slider window **181** includes a plurality of selectable health status response indicators **183A**. The user selects one which becomes highlighted over the others, such as health status response selected icon **183B**. The health status slider window **181** further includes a health status selected response information **184**, such as "In Pain", that is displayed to the user to confirm the selected health status response.

Referring now to FIG. 3B, a scanning results window/screen **140C** is shown being displayed by the touch screen display device **202** of the device **104**. The screen **140C**

includes a number of similar items illustrated in screen **140A** of FIG. 1C and are not repeated here. The exemplary scanning results window **140C** may be generated by the user after selecting a results button under the menu button or by one or more sliding finger gestures (e.g., down and/or to the right).

The scanning results window **140C** includes a results filter button **163D**, and a calendar button **163**. The scanning results window **140C** displays one or more scanning sessions **300** each including a completed scan type indicator **301**, an interpretive message indicator **302**, a picture tag indicator **303**, a date/time stamp **305**, and a location time stamp **306**. The scanning session that is selected for display on the device **104** is highlighted by a selected scan indicator **304**. The scanning results window **140C** further displays a results information slider window **307** and slider number indicators **308**.

Referring now to FIGS. 3B-3C, the results information slider window **307** of the scanning results window **140C** can be slid sideways by a user's finger to display different slides. As shown in FIG. 3C, the different slides or windows displayed in the slider window **307** include a vital sign measurements results slide **350**, an interpretive message slide **351**, a health status report slide **352**, and a scan summary information slide **353**.

The vital sign measurements results slide **350** includes a plurality of vital signs icons **333A-333F** (collectively **333**), a plurality of associated vital signs measurements **332A-332F** (collectively **332**), and a plurality of associated vital measured labels **331A-331F** (collectively **331**). The vital measured labels **331** and vital signs measurements **332** indicated in the slide may include heart rate **331B,332B**; breathing (respiration) rate **331F,332F**; temperature **331A,332A**; blood pressure **331C,332C**; heart rate variability (HRV) **331E,332E**; and blood oxygenation **331D,332D**. The associated vital signs icons **333** may include a heart icon **333B**, a breathing (lung) icon **333F**, a thermometer icon **333A**, a blood pressure icon **333C**, a variable heart icon **333E**, and an oxygenation icon **333D**.

The actual measurements captured during the scanning process are illustrated by the numeric number values of the vital sign measurements **332**. For example, the heart rate measurement **332B** of sixty-three (63) is shown near the heart icon **333B** and the heart rate text label **331B**. The numeric values of the vital measurements **332** may be the average measurements captured during the scan that was immediately performed recently or that scan session is selected by the user. The measurements **332** are illustrated near their respective icons **333** and the respective text labels **331** indicating the vital sign that was measured. The results of the scan are typically automatically saved. However, a function button may be required to delete those scan results from the wireless portable multi-function device **104** or alternately a button to upload those results to a storage server.

The interpretive message slide **351** includes a medical information disclaimer **361**, a medical interpretive message **362**, and a learn more link **363**. The medical information disclaimer **361A** in the interpretive message slide **351** may be a message such as "while this is not a medical device, you should probably be informed of something we've noticed". The medical interpreter message **362** may be something such as "your systolic blood pressure is above the normal range, as indicated by the National Institutes of Health, for someone of your age, gender, height and weight." The learn more link **363** may include a selectable icon or text to transfer the user to a web browser and a health link where

he may learn more about his or her condition indicated by the medical interpreter message **362**.

The health status report slide **352** includes health status response buttons **372**. Health status response buttons **372** may include a symptoms button **372A** to enter health symptoms, such as a headache or a cough for example, when the scan was taken. A medication button **372C** may be used to indicate a vital signs scan was performed after taking medication. A sleeping response button **372B** may be used to indicate the number of hours of sleep for a night prior to performing the scan.

The scan summary information slide **353** includes a scan summary **381** of a selected scan session. The scan summary may include the time and date stamp **383A**, the location **383B** of the scan, the type of scan **383C** (e.g., head or chest), and the duration **383D** of the scan, such as thirteen (13) seconds. The scan summary **381** may further indicate user biometrics **383E** such as the gender, age, weight, and height of the user being scanned. The scan summary may further indicate whom **383F** performed the scan, such as the user or a family member. In the scan summary example in the scan summary slide **353** shown in FIG. 3C, the user Mimi was scanned by her Mom on Aug. 14, 2013 at 8:29 AM in Campbell, Calif. The scan of Mimi was a head scan having a duration of thirteen (13) seconds. Mimi's user biometrics indicates she is five (5) years old, weighs forty-eight (48) pounds, and a height of three feet, six inches (3', 6").

FIG. 3D is an illustration of an exemplary window of the vital signs scanning application on the portable wireless device. In this exemplary window displayed on touch screen **202** of the multifunction device **104**, the vital signs scanning application **140** is prompting the user to select a second scan. A second scan may be selected by touching scan virtual button **342** or using a finger gesture on the touch screen. A third scan may also be selected after the second by touching scan virtual button **342** or using a finger gesture on the touch screen. The third scan may be performed at the chest region to measure respiration rate and collect body sounds. The user may desire to skip a secondary scan by touching a skip scan virtual button **344**.

Referring now to FIGS. 4A-4B, a temperature averaging window **140T** is shown being illustrated in the touch screen **202** by the scanning application software **140**. This may be displayed as a result of selecting the graph button **165** of the initial scanning window **140I**. The temperature averaging window **140T** could include a textual heading **400** illustrating the types of graph that are plotted below. The textual heading **400** may recite "seven-day average" to let a user know that one or more seven-day average graphs are being displayed below. The portable vital signs scanner **102** may be used periodically throughout a 24-hour period each day. The seven day average may look back over a seven day window and time, plotting an average curve **401A**, a maximum curve **401M**, and a minimum curve **401S**. The vital sign measurements are plotted on the Y-axis **411** and a time as the time of day on the X-axis **410**. The portable wireless vital signs scanner **102** is expected to be used daily at multiple times during a day. In this, manner the vital signs of the user are captured periodically during the day by the vital signs scanner **102** and the personal portable wireless device **104** of the scanning system **100**. The maximum curve **401M** and the minimum curve **401S** may be illustrating plots of the maximum value and minimum values over all scans that were previously performed. The time of day axis **410** illustrates periodic time values during the span of a 24-hour day. In one embodiment, the far most right point of the curves represents the given time of day **415** of a sliding

window. In another embodiment, the time axis is fixed and the curve **401A** grows from left to right during the time period as scans are made and time actually progresses. The scan points **420A-420N** are illustrated along the average curve **401A**. The scan points **420A-420N** may represent actual scans during the day or some measure of average during the preceding seven-day period. Interpolation lines **421A-421M** may be inserted between each scan point to show a trend line of how the vital sign that is measured varies during times of the day. For example, scanning point **420J** may represent a scan that took place between 4:00 and 7:00 pm and how the body trends towards that during that time of day.

The illustrated seven day average graph illustrated in FIGS. 4A-4B shows a body temperature graph. This is for illustration purposes only. The vital sign measurement curves could be temperature curves, blood pressure curves, oxygenation curves, heart rate curves, breathing/respiration rate curves, for example, that represent measurements that are scanned by the vital signs scanner **102**.

As more information is captured by the scanner **102** and stored in the personal portable multi-function device **104**, additional results may be plotted over time to generate the vital signs curves for display by an averaging window, such as vital signs window **140T**.

Referring now to FIG. 5A-5E, a plurality of prognosis windows **140D-140H** are illustrated. In FIG. 5A, the heart rate prognosis window is shown. In FIG. 5B, the temperature prognosis window **140E** is illustrated. In FIG. 5C, a breathing rate prognosis window **140F** is illustrated. In FIG. 5D, a blood pressure prognosis window **140G** is illustrated. In FIG. 5E, a blood oxygenation window **140H** is illustrated. These windows may be selected through the use of the vital signs icons **333A-333E** acting as buttons to display the respective prognosis window.

As illustrated in FIG. 5B, each prognosis screen **140D-140H**, may include a navigation bar **502**, one or more function buttons **503**, a vital signs icon **504**, a return button **505**, a conditions indicator **506**, a vital signs indicator **507**, a measurements value indication **508**, and a vital signs bar **510**. The navigation bar **502** may allow a user to navigate the various screens of the vital signs application scanning software **140**. For example, a scan screen icon/button **521** may be provided to jump to the scanning screen. A prognosis screen icon/button **522** may be provided to jump to the prognosis screens **140D-140H**.

The vital signs bar **510** may be provided to navigate through the various vital signs prognosis windows/screens **140D-140H** as well as providing a snapshot of the values of each of the vital sign measurements. In that case the vital signs bar **510** includes a measurement value indicator **512** and a vital signs icon **511** for each of the vital signs that are scanned and captured by the vital signs scanning system **100**.

The return button **505** may be used to return to the previous screen that was displayed by the user interface of the scanning application software **140**. The function button **503** may be an add a note button to add text about a user's condition or circumstances under which a scan was taken. The vital signs icon **504** indicates at a glance what prognosis window is being displayed.

The conditions indicator **506** for each prognosis screen will provide an indication of the most recent scan in comparison with an expected average value for a given user. For example, a temperature's vital sign is illustrated in FIG. 5B as having the condition indication of high due to a measured value of 101° F.

In the vital signs bar **510** the measurement indicator **512** and the vital signs icon **511** may be highlighted to indicate which prognosis screen is being illustrated at a glance.

Referring now to FIG. 6A-6D, respective use of the portable wireless vital signs scanner **102** are illustrated. In FIG. 6A, a top front perspective view, the wireless vital signs scanner **102** includes a front electrode **610**, and a front sensor **612** on a front side. The front electrode **610** is pressed against the user's forehead/temple, preferably at the temple, in order for the scanner **102** to make an electrical connection to the body of the user.

In one embodiment the scanner **102**, a top sensor window **621** and a top electrode **622** are provided in the top side of the scanner **102**. A top sensor **121** may be located underneath the top sensor window **621** to obtain a vital signs measurement from a user's finger that may be pressed on top of the window **621**. A top electrode **622** may be used to form an electrical connection to a user's finger and complete a circuit of the user's body such as illustrated in FIG. 1A.

The housing **600** of the vital signs scanner **102** may generally be circular shaped and include a circular top housing **620G**, a circular bottom housing **620B**, and a hollow cylindrical surface **620S**. The side cylindrical ring **620S** may be concave, or convex over a portion of the surface. Alternatively, the cylinder side surface **620S** may be a toroid shape over a portion of its body.

In FIG. 6B, a top back perspective view of the wireless vital signs scanner **102** is illustrated. The wireless vital signs scanner **102** illustrate various aspects of the invention in the side cylindrical surface **620S**. The wireless vital signs scanner **102** includes a power button **613**, a serial port connector **614**, an optional wireless connection LED **618**, and a power light-emitting diode **616**. The power button **613** may be pressed to power the wireless vital signs scanner **102** on. The serial port connector **614** may be a micro universal serial bus connector to allow a micro USB cable to plug thereto. The micro USB port may provide an external power source to charge the rechargeable battery within the wireless vital signs scanner **102** and also may serve as a wired data port for updating firmware or transferring data to a computer or storage device. The optional wireless connection light-emitting diode **618** provides a visual indicator that the wireless vital signs scanner **102** is coupled to the wireless personal portable multi-function device **104** over its wireless communications channel **103A** as illustrated in FIG. 1A. The power light-emitting diode **616** provides an indicator that the wireless vital signs scanner is powered on by the power button **613**.

In FIG. 6C, a vital signs wireless scanner **102'** is illustrated having a generally diamond shaped body housing **620**. In this case the housing top **620T** and the housing bottom **620B** generally have a diamond or a square shape to match that of the side cylindrical surface **620S**. The top or bottom housing portion **620T** may each include a gripping surface **624** with corrugations or channels so that a user may comfortably and securely hold the wireless vital signs scanner **102'**. The gripping surface **624** may be formed of a conductive material to aid the top and or bottom electrodes in forming an electrical connection to a user's body.

Referring now to FIG. 6D, a top front perspective view of the wireless vital signs scanner **102'** is illustrated. The wireless vital signs scanner **102'** includes the front electrode **610** and front sensor **612**.

While the electrode **622** and the gripping surface **624** are illustrated in the top housing **620T**, they may also be implemented in the bottom housing portion **620B** instead of the top. Instead of an index finger making a connection with

a top electrode **622**, a thumb finger may couple to a bottom electrode (not shown) to provide a larger surface area contact to the body in the bottom housing portion **620B**.

Referring now to FIG. 7A, an exploded view of the wireless vital signs scanner **102** is illustrated. The exterior components of the wireless vital signs scanner **102** are formed of parts that can be wiped clean by a damp towelette or a disinfecting wipe. In this manner, the scanner **102** may be shared by users in a family with less worry about spreading bacteria and germs. Each user may have a personal profile or preferences stored in the scanning software application **140**.

The wireless vital signs scanner **102** includes a main printed circuit board **701A** and a daughter printed circuit board **701B** coupled perpendicular to the main circuit board **701A**. Because the scanner **102** is wireless, it includes a rechargeable battery and a connector port to which a cable may connect to recharge the battery. Preferably the battery may be charged in an hour or less. If the scanner **102** is used a few times a day, the charge of the rechargeable battery may last about a week. The main print circuit board **701A**, the daughter printed circuit board **701B**, and the rechargeable battery form an electronic sub-assembly **701**.

The electronic sub-assembly **701** is inserted into a housing **702** of the vital signs scanner **102**. The sensors on the front daughter board **701B** are aligned into a front sensor opening **710** in the side housing ring **702C** of the housing **702**. A ribbon cable **720** electrically connects the front daughter board **701B** to the main print circuit board **701A**. A sensor **812** in the front daughter board **701B** includes electrical leads that are coupled to the main printed circuit board **701A**.

The main printed circuit board **701A** is inserted into the housing ring **702C** so that a serial bus connector **612** aligns with the connector opening **722** and the front sensor **812** is aligned into the front sensor opening **710**. A top/bottom electrode **806B** covers over an opening **704** and is electrically coupled to the main printed circuit board **701A** and an ECG circuit mounted thereto.

The housing **702** of the wireless vital signs scanner **102** includes a top housing portion **702T** with a top electrode **806B**, a side housing ring **702C**, and a base housing portion **702B**. The orientation of the housing **702** for the scanner **102** may be altered such that the housing base **702B** becomes the housing top **702T** and the housing top **702T** becomes the housing base **702B** with a bottom electrode **806B** to couple to a thumb. Electrodes may also be in both the housing base **702B** and the housing top **702T** to provide a lower resistive coupling to the user's body.

The top housing portion **702T** includes a microphone opening **717T** and a plurality of posts **725** and an electrical sensor opening **704**. The housing base **702B** may include a microphone opening **717B** and a plurality of pillars **726** that can interface to the posts **725** when the housing is assembled together about the printed circuit boards.

The wireless vital signs scanner further includes a front cover **711** to fill in the front sensor opening **710** in the side housing ring **702C**. The front side cover **711** includes a plastic cover portion **712** and a front electrode portion **727** with a lens **715** transparent to thermal wavelengths to allow the sensor **812** beneath it to capture a measure of temperature. The plastic cover **712** is also transparent to various wavelengths of light that are used by the vital signs sensors. The front electrode portion **727** of the front cover **711** is formed of a conductive material, such as stainless steel metal, to form a circuit when pressed up against the user's body at the forehead/temple, finger, chest or elsewhere. The

shape of the front electrode **727** can vary with the shape of the wireless vital signs scanner **102**.

The side housing ring **702C** includes one or more LED openings **712** to receive the power light-emitting diode **616** and the optional wireless connection light-emitting diode **618**. The side housing ring **702C** further includes a power button opening **723** through which the power button **613** may extend.

FIG. 7B illustrates a partially assembled wireless vital signs scanner **102**. Through the front opening **710** in the side housing ring **702C**, the front daughter printed circuit board **701B** includes a slot opening **721**. The slot opening **721** may be used to receive a shade **708** that separates the LEDs **808A-808B** from the photo diode **810**. The shade **708** deters light emitted by the LEDs **808A-808B** from directly being impinged onto the photo diode **810**. The wire (not shown in FIG. 7B) from the front electrode **727** may be inserted through the opening **706** and then coupled to the main PCB and the ECG circuit. The front cover **711** can then be assembled to cover over the front opening in the side housing ring **702C** of the housing.

The daughter printed circuit board **701B** is arranged to be substantially perpendicular with the main printed circuit board **701A**. As previously discussed, the front cover **711** includes a transparent cover portion **712** and a metallic conductor portion **727**, and the lens **715**. The transparent cover portion **712** covers over one or more light-emitting diodes **808A-808B** generating various wavelengths of light, and a photo diode **810** that receives various wavelengths of light. The light generated by the light-emitting diodes **808A-808B** is shined onto the user's forehead/temple and reflected back to the photo diode **810**. Light with known time periods may be generated by the light emitting diodes (LEDs) **808A-808B** with different wavelengths and radiated onto a user's forehead/temple. The reflection is detected by the photo diode **810** to form an electrical signal that is analyzed. In this analysis of the signal generated by the reflected lights of different wavelengths, a measure of oxygenation in the blood stream may be generated.

The front side cover **711** includes the transparent lens **715** with a center aligned into the optical axis of the front side sensor **812** so that additional vital signs measurement may be made from the forehead/temple of the user. An opening **706** in the daughter board **701B** allows a wire to pass through from the front electrode **727** and be coupled to a wire trace on the main PCB that is coupled to the ECG circuitry mounted thereto. When pressed against the user, the metallic electrode portion **727** of the front side cover **711** makes an electrical contact to the forehead/temple or other body portion of the user. An insulating ring **736** under the electrode portion **727** of the front side cover may be used to isolate any metal of the infrared thermometer **812** from the electrode portion **727**.

FIG. 8A illustrates a functional block diagram of electronic circuitry **800** within the portable wireless vital signs scanner **102**. The personal portable wireless vital signs scanner **102** associated with a given user profile stored in the user data of the wireless personal multifunction device **104**. The wireless communication channel **103A** between the scanner **102** and the multifunction device **104** may be a secure connection with information passed between each. The devices are typically paired to each other by a code so that no other wireless device may utilize the wireless communication channel **103A**. A different wireless communication channel **103B** may be generated between the vital signs scanner **102** and a personal computer **150**, for example. Each of the wireless communication channels **103A**, **103B** may be

a Bluetooth communication channel, for example, in which case the signal strength between each over a Bluetooth communication channel is relatively short with a limited distance over a range between zero and twenty-five feet, for example.

Referring now to FIG. 8A, electronic circuitry **800** of the portable wireless vital signs scanner **102** includes a processor **840** at the heart of the system. The processor **840** may be a reduced instruction set processor operating with embedded operating system software. In one embodiment of the invention, the processor is an ARM processor operating with MICRIUM's embedded real time operating system (RTOS).

To provide the wireless communication channels **103A**, **103B**, a wireless radio **870** is coupled to the processor **841**. The wireless radio **870** is coupled to an antenna **871** that could be internal, as part of an overall radio system, or external to the wireless radio **870**. An optional light emitting diode **848**, used as a wireless connection indicator, is coupled to the wireless radio to indicate a successful pairing with the personal portable wireless digital multifunction device **104**. To scan for vital signs over a period of time such as 10 seconds, the electronic system **800** includes an infrared thermometer **812**, an accelerometer **885**, a pulse oximetry sensor and a pulse oximetry circuit **880**, and analog electrocardiogram circuitry **860**. Coupled to the electrocardiogram circuitry **860** is the bottom or top electrode **806B**, the front electrode **711**, bottom/top electrode connection, and the front electrode connection **806F**. As shown in FIG. 1A, a portion of a human body is coupled to the front electrode **711** and the top/bottom electrode **806B** to form a circuit.

The pulse oximetry circuit **880** is coupled to a pair of light emitting diodes **808A-808B**. Each of these emit light patterns that are reflected off of the user's forehead/temple internally. The reflected light is captured by a photodiode **810** and coupled to the circuit **880**. That is, incident light **891** from the light emitting diodes **808A-808B** reflects internally off the user's head **116** as reflective light **892** which is received by the photodiode (PD) **810**.

The infrared thermometer **812** detects the surface temperature of a use's forehead/temple (or elsewhere) by measuring thermal radiation (referred to as Blackbody radiation) **813** emanating from the head **116** (or other body portion to which the scanner is pressed) of a user.

To power the circuits in the system **800** of the personal portable wireless vital signs scanner **102**, a rechargeable battery **850** and a voltage regulator and battery charge controller **854** are coupled together into the circuits in the system **800** when the switch **852** is closed. The battery charge controller **854** is coupled to power pins of a serial connector **856** to receive an external DC voltage supply. The external voltage supply may be used to recharge the battery and power the system **800** when it is connected. The rechargeable battery **850** may hold a charge for a period of seven days, even while scanning multiple times during each day, due to the low power consumption of the circuitry and the limited period of time needed to perform a scan of the vital signs of a user. That is, the vital signs scanner **102** is not expected to be continuously powered on during a day, but powered up periodically to perform the scans as needed.

The processor **840** may include a processor memory **841** to store system instructions to control the circuitry in the system to obtain the scans and process the information obtained through those scans into a proper user format. To store the user data from each of these scans, a nonvolatile memory **844** is coupled to the processor **840**. The nonvolatile memory **844** may be soldered to a printed circuit board with the processor **840**. In an alternate embodiment of the

invention, a connector **845** is provided so that the nonvolatile memory **844** is a removable memory card so that a user's data may be transferred from one scanner to the next, if needed.

A power LED **851** may be coupled to the processor **840** to provide an indication that the electronic system **800** is powered up. The system can be manually shut down via the scanning software application **140** so that the scanner **102** powers off. However, the scanner **102** can also automatically shut off after a predetermined period of time to conserve power and a charge on the rechargeable battery **850**. The user then just needs to press the power switch **852**, once again, to turn the system back on and scan for vital signs of a user.

The processor **840** includes one or more analog digital converters **842** in order to receive analog signals from the infrared thermometer **812**, accelerometer **885**, pulse oximetry circuits **880**, and ECG analog circuits **860**. Electronic system **800** may further include a stereo microphone **875** consisting of a top microphone **875T** and a bottom microphone **875B** each coupled to a stereo microphone amplifier **874**. The stereo microphone amplifier may have its own analog to digital converter, or the processor's analog digital converter **842** may be used to convert analog signals into digital signals. For example, an ECG analog signal may be converted into digital signals with the analog digital converter **842** of the processor. The stereo microphone **875** captures audio signals near the wireless vital signs scanner **102**. The accelerometer **885** captures movement of the portable wireless vital signs scanner **102**.

The combination of the audio information and the movement information may be utilized to determine the quality of the scanning information being obtained by the vital signs capturing circuitry. For example, the stereo microphone **875** may be used to capture noise from a user talking and plot that on a graph indicating noise spikes, or noise lines **330**, such as shown in FIG. 3A. This provides feedback to a user about the quality of the scan at these intervals. The accelerometer **885** and the motion information may be similarly used to make a judgment about the quality of the vital signs scanned information being captured by the vital signs circuitry of the infrared thermometer **812**, the pulse oximetry circuits **880**, and the ECG analog circuits **860**.

The microphones **875** in the portable wireless scanner **120** may also be used to capture body sounds such as shown in FIGS. 1E-1F and store the captured body sounds in memory **844** as a potential symptom of a medical condition of the user's body. For example, heart beat sounds **155** may be captured by the microphones **875** when the scanner **102** is positioned against skin of the chest **114** near one's heart **156**, as is illustrated in FIG. 1E. As another example, lung or breathing of air entering and exiting one's lungs, respiration sounds **157**, may be captured by the microphones **875** when the scanner **102** is positioned against skin of the chest **114** near a lung **158** in one's body, as is illustrated in FIG. 1F.

To further optimize scanning results, scan quality algorithm monitor the vital signs scanning process and can provide feedback (visual and/or audible) to the user, such as through the multifunction device **104**.

An optional audible sound generator **847** in the scanner **102** may be coupled to the processor **840** to provide audible user feedback to the user during the scanning process. The user feedback may help the user to perform better vital signs scan with the wireless vital signs scanner **102** and acquire a higher quality of vital signs measurements. The audible sound generator **847** may generate alert sounds indicating when the scanning process begins and ends. It may also

generate an error signal indicating to the user that he is not properly using the scanner **102** and look for instructions on the device **104**.

Referring now to FIG. 8B, a block diagram of the electronic circuits **800** is shown mounted onto the main printed circuit board **801A** and the daughter printed circuit board **801B**. FIG. 8B also illustrates alternate locations for electronic circuits in the system **800** for alternate embodiments of the vital sign scanners **102**, **102'**.

A slot **803** in the daughter printed circuit board **801B** receives a shade device **708**. Light emitted by the LEDs **808A-808B** is shaded by the shade device **708** so that it may not directly impinge onto the photo diode **810** in the daughter PCB **801B**. Reflected light, reflected off the user's body, is desirable to be captured by the photo diode **810**.

Wire leads **830** of the IR sensor **812** and the front electrode contact **806F** are coupled to pads **831** of the main printed circuit board **801A**. First and second LEDs **808A-808B** and the photodiode **810** are coupled to connector **821** by conductive traces **819B** on the daughter printed circuit board **801B**.

The main printed circuit board **801A** has a plurality of wire traces **819A** coupling circuits mounted thereto together. The daughter printed circuit board **801B** includes a plurality of traces **819B** coupling circuits mounted thereto to connector **821**. A ribbon cable **820** is used to couple signals between the daughter memory card **801B** and the main printed circuit board **801A** for the oximetry circuit **880**. The oximetry electronic circuit **880** is coupled between the connector **822** and the processor **840** on the main printed circuit board **801A**. One set of one or more wire traces **819A** couple the oximetry electronic circuit PPG **880** to the connector **822**. Another set of one or more wire traces **819A** couple the oximetry electronic circuit PPG **880** to the processor **840**.

In accordance with one embodiment of the invention, if the oximetry sensors are moved to a top portion of the housing to sense oximetry through a finger, with the IR LEDs **801A'-801B'** and the IR photodiode **810'**, the oximetry circuitry may be moved to the opposite side as the oximetry electronic circuit PPG **880'** coupled between the processors **840** and the LEDs **808A'-808B'**, IR photodiode **810'** and mounted in the top portion of the housing.

The bottom or top electrode **806B** is formed of stainless steel to provide a good connection to either a thumb finger or an index finger. The electrode **806B** is coupled to a connector **823** and to the ECG circuitry **860** on the main printed circuit board **801A**.

The main printed circuit board **801A** includes the processor **840**, the wireless radio **870**, the microprocessor memory **841** (either internal or external as shown mounted to the printed circuit board), an accelerometer **885**, an amplifier **874**, oximetry circuitry **880**, **880'**, user memory **844**, and battery charge circuit **854**.

Top and bottom microphones **875T** and **875B** extend out from the main printed circuit board **801A** by ribbon cables so that they may be mounted into the respective openings in the housing top and housing bottom. The microphones **875T**, **875B** may be coupled to the amplifier **874** which in turn may couple audio signals into the microprocessor **840**. Mounted to the main printed circuit board is the power LED **851** and the connection LED **848**. Further mounted to the main printed circuit board is a power on/off switch **852** coupled to the voltage regulator battery charge circuit **854** to signal for it to turn power on or off to components with the scanner **102**. Additionally, mounted to the main printed circuit board **801A** is a serial connector **856** coupled to the microproces-

sor. In one embodiment invention, the serial connector **856** is a micro universal serial bus connector.

An optional audible sound generator **847** may be mounted to the main PCB **801A** and coupled to the processor **840** as shown. To avoid interference, the sound generator **847** may be positioned away from the microphones **875**.

Main printed circuit board **801A** includes a plurality of openings **826** that receive the pillars **725**, **726** of the housing top **702T** and housing base **702 B**.

The daughter printed circuit board **801B** includes a connector **821**, light emitting diodes **801A-801B**, and a photodiode **810** mounted thereto. The IR sensor **812** is inserted through a hole in the daughter PCB **801B**, attached thereto with an adhesive, and supported thereby. The front electrode **806F** around the IR sensor **812** is attached with an adhesive to the daughter PCB **801B** for support.

The ribbon cable **820** couples signals of the light emitting diodes **801A-801B** and the photodiode **810** regarding oximetry between the daughter board **801B** and the main printed circuit board **801A** for the oximetry circuit **880**. With the terminals **830** of the IR sensor **812** coupled to the pads **831** of the main PCB **801A**, signals of the IR sensor **812** regarding temperature are coupled into the processor **840**. With the terminals **830** of the front electrode **806F** coupled to one or more pads **831** of the main PCB **801A**, signals of the ECG circuit **860** to measure heart activity (e.g., heart rhythm, heart rate, etc.) may be coupled into and out of a users body.

Thus, the personal portable wireless vital signs scanner integrates a plurality of sensors and a controller/processor together to synchronously obtain a plurality of vital signs at different times during a users day. Despite the integration of multiple sensors and a controller/processor into the scanner, the vital signs scanning device has a relatively low production cost. The integration with a ubiquitous consumer electronic device pre-owned by many users, the personal wireless multifunction device (e.g. smartphones, tablets, etc.), to display the vital signs data with vital signs scanning software, also keeps the costs low of the overall personal vital signs scanning system. The low costs of production of the vital signs scanner can allow lower retail pricing and higher volume of sales, enabling an average consumer to afford the vital signs scanning system to personally scan and monitor trends of their vital signs for as an important part of preventive medical care of their own bodies.

Referring now to FIG. 9, a diagram illustrating an exemplary hierarchy of windows provided by the scanning application software **140** is illustrated. A variety of vital sign scanning user interface windows of the scanning application software **140** have been described. The vital signs scanning application software **140** executed by a processor provides a user interface hierarchy of the vital sign scanning user interface (VSUI) windows. For example after the vital sign scanning application is opened at process **900**, a scanning login button **902** may be presented to the user by the scanning application software **140**. If the user is properly selected he chooses the login button to transition to a user home screen **140H**.

In the user home screen **140H**, a user inputs his login identification and password to gain access to personal vital signs scan data stored in the device **104**. If the user is a different user a different user button **903** may be selected or a horizontal swipe finger gesture **940H** may be used to go to a select user window **140L**. If the user is not listed and is a new user, the select user window **140L** may have a new user button **905** that jumps to a new user window **904U** that is displayed to the user.

In the new user window **940U**, the new user may input his login user ID and password that he desires to use with the scanning software application to identify his personal vital signs scan data. Other information, such as sex, height, weight associated with a time and date may be entered by the user. As the days and/or years go by, the user may update this information in the profile so that the vital signs scanning system better knows what conditions might occur for the given user. The login and profile windows can also allow the scanning system to be shared with other users in a family. After logging in with user ID and password through the home screen, the scanning system application may display the initial scanning window **140A**.

By using a horizontal finger gesture **940H** over the scan type slider **171**, the user may select a head scan **173A**, a chest scan **173B**, the results window **940RW** (e.g., windows **307,350-353** in FIGS. 3B-3C, windows **140D-140H** in FIGS. 5A-5E), or the graphs window **940GW** (e.g., window **140T** shown in FIGS. 4A-4B). If at any point in time the user feels the need to terminate the scanning process, the done button **190** in the user interface may be selected. By means of a vertical finger gesture **940V** in the scanning window **140A** during a head scan **173A** or chest scan **173B**, or the results window **940RW**, the health status window **140B** may be displayed. Alternatively, a health status button **180**, such as shown in FIG. 1C, may be selected to display the health status window **140B**.

Each of the screens/windows/slides of the vital signs scanning application may be navigated by pressing one or more virtual graphical buttons (e.g., back, done) and/or making one or more finger gestures **940F** (e.g., vertically up/down **940V**, horizontally left/right **940H**) dragged across a touch screen. A navigation bar may alternatively be provided with navigation buttons to navigate between selected windows. The menu button may also be used to navigate to different windows. In other cases, pressing a button displays a different screen/window/slide such as the done button.

After scanning is completed, the scanning application software can automatically display the results window **140RW**. Additional buttons in the results window **140RW** may be used to navigate to various graph windows **140GW**, such as the temperature graph window shown in FIGS. 4A-4B. Additional buttons in the results window **140RW** may be used to navigate to various prognosis windows, such as prognosis windows **140D-140H** shown in FIGS. 5A-5B. In this manner, vital signs data and information can be displayed to the user in various ways.

The scanning software application **140** includes a number of instructions and routines that are executed by a personal wireless multifunction device **104**. The personal wireless multifunction device **104** may include a smart phone, an APPLE IPHONE 5, IPHONE 4S and SAMSUNG GALAXY S III that support Bluetooth Smart. To help everyone use the device, assistive technology may be added to the scanning software application **140**.

The significant software routines of the scanning software application **140** include a scan procedure controller based on scan quality algorithm, UI implementation, wide area network interfacing to cloud services, scan results interpretation, and trend charting.

Interactive Scanning and Quality User Feedback

The forehead and temple (forehead/temple) of a user has been identified as place to concurrently acquire multiple vital sign measurements of a user's body over a period of time (e.g., a ten or thirty second scan). The relatedness in time between the multiple vital sign measurements allows

them to be use together to determine scan quality. The scanner has integrated sensors for concurrent data capture, making the scanner more capable than a single sensor alone, not only for multiple vital signs measurements but also for quality feedback regarding data capture.

There are a number of operating conditions that may not provide optimal scan data and scan results when the portable vital signs scanner **102** is scanning. If these operating conditions can be avoided, the scan data and the scan results obtained therefrom can be improved. It is desirable to provide vital sign scan quality control for a better user experience. It is desirable to provide vital sign scan quality feedback to a user. The multiple sensors in the vital signs scanner **102** that concurrently acquire data enable a vital sign scan quality control. Integrated user interface devices (e.g., sound generator **847**) in the scanner **102** and the vital signs user interface **140** provided by the portable multifunction device **104** and the software executed therein may provide an interactive scanning process to improve the user experience during a vital signs scan.

User feedback regarding the quality of a scan, quality feedback, can be provided in real time by the scanner **102** and the vital signs user interface **140** provided by the device. For example, a text message could be displayed or a voice message could be audibly generated such as "Please hold the scanner still for good scan" if the user's hand is detected to be shaking it. A text message could be displayed or a voice message could be audibly generated such as "Please touch the scanner against your forehead/temple to start scan", for example, if feedback suggest that the scanner is not touching the forehead/temple of the user.

Quality feedback can be provided by fusing motion detection of the scanner and individual evaluation of signal deviation of each vital sign sensor data from an expected normal range. There are three general observations that can be made into an algorithm regarding data capture quality in the portable vital signs scanner: 1) Significant motion from the accelerometer indicates that the data capture of ECG and Pulse oximetry data will not be good; 2) The signal quality from ECG, Pulse oximeter and IR thermometer sensors are independently evaluated; and 3) For high-quality data capture, data from all vital sign sensors should be good.

Referring now to FIGS. **10A-10B**, sounds and movement of a user's head may affect the quality of information that can be captured by the vital signs scanner. In FIG. **10A**, a user is talking and moving his mouth **1001** while holding the vital signs scanner **102** against his forehead/temple **116**. The movement of the users mouth can create vibrations that may disturb the electrical connections between scanner and body as well as the infrared scans between the vital signs scanner **102** and the forehead/temple **116** of the users head. The microphone **875** in the vital signs scanner **800** can help detect people talking during forehead/temple scan.

Referring now to FIG. **10B**, a user may also shake his head and forehead/temple **116** left and right as shown by the left and right arrows, such as when talking with another or lacking in attention. A user may also nod his/her head and forehead/temple **116** up-and-down as shown by the up and down arrows, such as when talking or lacking in attention. The movement of a user's head and forehead/temple can also cause the vital signs scanner **102** to unreliably record vital signs data.

Referring now to FIGS. **11A-11C**, the degree to which the vital signs scanner **102** is pressed against the user's forehead/temple **116** can also affect the reliability of the data recorded by the vital signs scanner **102**.

In FIG. **11A**, the vital signs scanner **102** does not touch the forehead/temple **116** of the user, making no contact, and thus the scanner cannot complete a circuit with the body or reliably detect temperature. Scan data captured by the vital signs scanner **102** in this case would not be valid.

In FIG. **11B**, the vital signs scanner **102** only lightly touches the forehead/temple **116** of the user being too gentle such that a poor contact is made between the vital signs scanner and the user's body. The electrical connection between the forehead/temple and the vital signs scanner is overly resistive. The angle the infrared scanner makes with the skin of the users forehead/temple is not substantially perpendicular. In this case, the vital signs data captured by the vital signs scanner are poor and unreliable.

In FIG. **11C**, the vital signs scanner **102** is pressed overly hard against the user's forehead/temple **116**. In this case, the vital signs scanner **102** may be pressed too hard against skin causing it to bulge inward away from the sensors/contacts and/or cut off blood circulation in a vein underneath the sensors. With reduced skin contact, the electrical connection between the forehead/temple and the vital signs scanner may be overly resistive and the ECG scan data may be poor or invalid. A distance the infrared scanner makes with the skin of the user's forehead/temple may be overly large such that poor temperature measurements may be made. With reduced blood circulation underneath the pulseOX sensor, the pulseOx scan data may be poor. In this case, the vital signs data that is captured by the vital signs scanner is poor and unreliable.

It is desirable, to provide an interactive scanning system with user feedback. When the vital signs scanner **102** is being improperly utilized, user feedback may be provided so that the user can alter his/her manner of using the vital signs scanner **102** so that better data quality is achieved to enable reliable vital signs data capture.

As shown in FIG. **8A**, The vital signs scanner **102** includes a processor **840** and a memory **841,844** to store software program instructions for execution by the processor. The software program instructions may provide an interactive scanning process and user feedback (with or without the digital device **104** and its scanning user interface) to improve the quality of scanning data and results.

The microphone **875** in the vital signs scanner **800,102** may be used to detect the sounds of a human body to determine new vital sign values or information when placed at an appropriate body part, for example, neck or chest. The audio samples can be analyzed for and detect specific sounds of the human body. The information obtained from the sounds may be fused together with other data to determine a new vital sign value or a diagnosis of a user's body. The microphone **875** may optionally be used to detect sounds of a user talking during a forehead/temple scan, for example, to aid in improving the quality of vital signs measurements and vital signs data.

The scanner **102** includes an accelerometer **885**. The accelerometer **885** senses acceleration due to the movement of the scanner. The accelerometer **885** can be used to improve the quality of vital signs data. For example, the accelerometer **885** in the vital signs scanner **800, 102** can be used to detect movement of the users head and forehead/temple **116** that is to contact the scanner. The accelerometer is preferably a three-axis accelerometer measuring acceleration (in units of gravity g) in three orientations generating three acceleration output signals. With three-axis accelerometer information, the orientation of the scanner with respect to earth and user can be determined in the typical scan scenario. The three-axis accelerometer information can

help determine whether the user is using the scanner properly. To measure the total acceleration without knowing the specific orientation of the accelerometer in the scanner, the square root of sum of squares (RSS) formula may be applied to all three outputs to form a single acceleration measurement of the scanner. As the gravitation force (g-force) at the surface of the earth is typically one (1) g (9.80665 meters per second squared), the relative acceleration of the scanner **102** may be determined by simple comparison of the single acceleration measurement with earth's surface gravitational force of one g.

The measured relative acceleration by the accelerometer **885** may be categorized into relative degrees of motion based on the results of the comparison earth's gravitational surface force of one g. The relative degrees of motion that may be detected by the accelerometer **885** and the vital signs scanner **800**, **102** are still (also referred to as no motion) **1217S**, small or minor motion **1217M**, and big or significant motion **1217B**. Significant or big motion **1217B** may be on the order of one tenth g (0.1 g) or greater deviation from one g (1 g), for example. Small or minor motion **1217M** may be on the order from two hundredths g (0.02 g) up to one tenth g (0.1 g) deviation from one g (1 g), for example. Still or no motion **1217S** may be a smaller deviation on the order of less than two hundredths g (0.02 g) deviation from one g (1 g), for example.

The detected motion by using the relative acceleration by the accelerometer **885** can be combined or fused together with the sensor data from the vital sign sensors to be a collaborative decision regarding the quality of vital signs data during a scanning session by the user.

One of a user's fingers not only serves to hold and support the scanner **102**, but also as one contact point for the ECG circuit **860** (the other one-lead ECG contact point is forehead/temple). The ECG circuit **860** and its electrodes **711**, **806F**, **806B** may be used to determine how well (resistivity) an electrical contact is formed with the forehead/temple and finger of the user's body during the scanning process over a period of time.

Scan data from the PPG sensor and/or the ECG sensor and their respective circuits may also be used to determine scan data quality. If the PPG scan data is off scale (saturated), then it provides an indication that there is no or too loose of a contact of the scanner **102** with a user's skin. If there is no PPG scan data signal but a good ECG scan data signal is present, this provides an indication that too much pressure being is applied and hence no pulse recording is possible to generate PPG scan data. Accordingly, the ECG scan data and the PPG scan data can be checked in this manner, fusing together the outcome to determine if an appropriate amount of pressure is being applied to the scanner to press it against the user's body to obtain quality scan data for ECG and PPG measurements.

The vital signs scanning user interface **140** executed by the portable digital device **104** is used to provide user feedback on its touchscreen display device **202** or its speaker **216**. The user uses one hand to hold the vital signs scanner **102** while his/her other hand holds the portable wireless device **104** (e.g., a smartphone) to view the touchscreen display device **202**. Alternatively or additionally, the audio sound generator **847**, a speaker, in the vital signs scanner **102** may be used to provide user feedback.

User feedback may also be visually provided to a user by use of text messages on the display **202** of the device **104** during the interactive scanning process and data acquisition by the scanner **102**. User feedback may also be visually provided to a user by use of color coding on the display **202**

of the device **104** during the interactive scanning process and data acquisition by the scanner **102**. For example, the color code of green on a field or an object in the user interface can indicate that the proper amount of pressure is being applied to the scanner to press it against the user's body. A color code of red on a field or an object in the user interface, for example, may indicate that too much pressure is being applied to the scanner to press it against the user's body. A color code of yellow on a field or an object in the user interface, for example, may indicate that not enough pressure is being applied to the scanner to press it against the user's body.

Referring now to FIG. **12**, a functional block diagram of an exemplary interactive vital signs scanning control system **1200** is illustrated. The vital signs scanning control system **1200** is a quick screening process before measurement are taken to decide in advance if a scan of vital signs data would be good, poor, or invalid. The screening process evaluates one or more short screening windows of time (e.g., **WT1**, **WT2**) to determine the quality of vital signs data that is being captured. The one or more short screening windows of time may be on the order of a second or two for example. Assuming a one second window and a sampling rate or frequency of 500 Hertz (Hz) or a two second window and a sampling frequency of 250 Hz, 500 data samples are used for the screening process. After the initial screening process provided by the interactive vital signs scanning control system **1200** determines that good signal data is being captured, a valid vital signs data capture occurs with the vital signs scanner. The data samples in the one or more short screening windows of time may be shared or overlap with the valid vital signs data capture if good signal data is being captured.

The vital signs scanning control system **1200** is executed by the vital signs scanner **102** in communication with the portable wireless device **104** (e.g., a smartphone). The vital signs scanning control system **1200** may be implemented in software, firmware, hardware, or a combination thereof. As mentioned herein, the vital signs scanning user interface **140** executed by the portable digital device **104** may be used to provide visual user feedback through the touchscreen display device **202** and audible user feedback through its speaker **216**. Alternatively or additionally, the audio sound generator **847** of the vital signs scanner **102** may also be used to provide audible user feedback.

The vital signs scanning control system **1200** includes a sensor data fusion process **1201**, and a scan state machine **1220** coupled in communication together. Data samples from the ECG sensor, the pulse oximeter sensor, and the accelerometer are received by the vital signs scanning control system **1200**. Data samples from the ECG sensor are used in an ECG data evaluation process **1203E** in the sensor data fusion process **1201**. Data samples from the pulse-oximeter are used in a PulseOx data evaluation process **1203O** in the sensor data fusion process **1201**. Data samples from the accelerometer are used in a motion detection process **1207** in the sensor data fusion process **1201**. Data samples from the temperature sensor may optionally be used in a temperature data evaluation process **1203T** in the sensor data fusion process **1201**.

The fusion process **1201** combines or fuses together the results of the ECG data evaluation process **1203E** and the PulseOx data evaluation process **1203O** to determine good, poor, or invalid scan signal data for each. The results of temperature data evaluation process **1203T** may also be combined or fused together with that of the ECG data evaluation process **1203E** and the PulseOx data evaluation

process 1203O. As further described herein, the results may be logically fused together to determine good, poor, or invalid scan signal data.

The vital signs scanning control system 1200 further fuses together the results of the motion detection process 1207 with the ECG data evaluation process 1203E, the PulseOx data evaluation process 1203O, and optionally the temperature data evaluation process 1203T through the use of a state machine 1220.

The vital signs scanning control system may perform a signal processing technique of envelope detection 1202 upon the data samples associated with ECG, pulse oximeter, accelerometer, and optionally temperature. Envelope detection can be used to determine signal quality without having to analyze the content details of the signals. Envelope detection helps to remove signal variations of high frequency. While envelope detection and other techniques and processes are described herein, other known signal processing techniques may be used by the one or more embodiments of the invention to implement the data quality screening process. For example, a mean value may be subtracted from a sensor signal that may reach full range/scale or maximum amplitude values (e.g., digital 8 bit signal with 256 maximum value), for simpler processing. For example, a constant of 128 (256/2) may be subtracted from the signal value at each time step to reduce the signal range after forming an absolute value to be between 0 and a maximum value of 128. For motion detection, a mean constant of one (1) g may be subtracted from values generated by the accelerometer. After subtracting the mean value, envelope detection may be performed.

One method of implementing envelope detection is to apply a mathematical function to the input signals and then a low pass filter on the resultant mathematical signal output to form a portion of an envelope curve so that the envelope data can be further evaluated. A Hilbert Transform method of envelope detection may alternatively be used. After performing envelope detection 1202, the interactive vital signs scanning control system then performs various evaluations 1204-1207 on the detected envelope curves.

Generally, the system performs a temperature evaluation 1204 upon the temperature envelope curve. The system performs an ECG evaluation 1205 on the ECG envelope curve. The system also performs a pulse oximeter evaluation 1206 on the pulse oximeter envelope curve. The system further performs a motion detection 1207 upon the acceleration envelope curve. The system then makes a determination of the quality of the evaluations made of each envelope curve. The determination of the quality of the vital signs data may be made based upon a range of expected data, based upon an expected curve, or based upon one or more threshold numbers. Other known methods of determining the quality of the vital signs data may be used. Exemplary methods of how to determine the quality of the vital signs data are now described.

Referring now to FIGS. 13A-13B, the quality of a vital sign VS is determined using an expected range 1350. In FIG. 13A, data samples 1301A of the vital sign VS captured by the vital signs scanner 102 are plotted against an axis of time T or data sample number. The data samples 1301A undergo envelope detection to generate an envelope curve 1302A of measured data. The envelope curve 1302A is compared with the expected range 1350. If the envelope curve 1302A over a given period of time (e.g., time windows WT1, WT2) is within the expected range 1350, then the vital sign is determined to be within range 1214G. For example, an expected temperature range may be between 80 and 115

degrees Fahrenheit. An envelope curve for temperature measurement within this expected range would be deemed within temperature range 1214G.

In FIG. 13B, data samples 1301B of the vital sign VS are plotted against the axis of time T. The expected range 1350 remains the same. However, the envelope detection 1202 generates an envelope curve 1302B of measured data. In this case, the envelope curve 1302B over a period of time (e.g., time windows WT1, WT2) is outside the expected range 1350. In which case, the quality of the vital sign VS is determined to be outside range 1214P. Consider for example, the same expected temperature range between 80 and 115 degrees Fahrenheit. An envelope curve for temperature measurement well below 80 degrees Fahrenheit, such as shown at time periods WT1, WT2 of FIG. 13B, would be unexpected and deemed outside temperature range 1214P.

When screening data samples of the vital signs scanner, it is desirable to quickly determine the quality. Thus, the sample size is somewhat small and does not lend itself to be properly aligned in time with an expected curve. An expected range may be used to determine quality of the vital sign data samples.

Referring now to FIGS. 14A-14B, the quality of a vital sign VS is determined using envelope detection and thresholds. In FIG. 14A, data samples 1401A of the vital sign VS captured by the vital signs scanner 102 over a window of time (a number of samples) are plotted against an axis of time T to form the curve 1410. The data samples 1401A undergo envelope detection to generate an envelope curve 1430 for the sampled data. In this case, intermediate data and its curve 1420 can be generated from the data samples 1401A of curve 1410 using a mathematical function. An exemplary mathematical function for intermediate data (ID) is $ID = \sqrt{(RD - EA)^2}$ where the difference between raw data samples (RD) 1401A and an expected average value (EA) 1412 is squared and then a square root is taken to determine an intermediate data value (ID) 1402A for the intermediate curve 1420. Squaring shifts half the energy of the signal to higher frequency and half towards zero frequency or direct current DC signal. A low pass filter may then be used to filter out high frequency energy to determine the envelope curve 1430. Down sampling may also be employed to assist in the generation of the envelope curve 1430 and its amplitude values of its data samples 1403A.

Referring now to FIG. 14B, after envelope detection, threshold levels 1460-1461 may be used to distinguish between good, poor and invalid signal quality in the vital signs sensor data. A poor threshold level 1461 and an invalid threshold level 1460 may be established to distinguish between good, poor and invalid signal quality. The levels may be established based on the expected range around an expected average.

In one embodiment, if the actual measurements are fully or substantially saturated, the signal quality is deemed invalid. Assuming an 8 bit amplitude signal, a maximum value is 256. Further assume that the expected average is 128. An invalid signal with full saturation would be the outside range of positive 128 and negative 128 around the expected average of 128. Assume that a range within positive 50 and negative 50 around the expected average of 128 to be good signal quality. Translating this example to the envelope curve, amplitude values between zero and 49 may be good signals, amplitude values between 50 and 127 may be poor signals, and amplitude values from 128 and above

may be invalid signals. Accordingly, the poor threshold level **1461** would be set to 50 and the invalid threshold level set to 128, for example.

The data samples **1403A** during time window **WT1** are substantially at the invalid threshold level **1460**, in some cases exceeding it. If the circuit generating these sample values was expected to generate signal levels well below a saturation level, then the quality of the signals being generated substantially at or above the saturation level may be deemed as having an invalid signal or data quality.

The data samples **1403C** during time window **WT3** are below the invalid threshold level **1460** and meet or exceed the poor threshold level **1461**. Accordingly, the data samples **1403C** during time window **WT3** may be deemed having a poor signal or data quality.

The data samples **1403B** during time window **WT2** are below the poor threshold level **1461**. A signal with data samples below the lower threshold level **1461** may be deemed to have a good signal or data quality.

In this manner, quality of initial scan data from vital sign sensors during an interactive screening process can be quantified into invalid, poor, or good signal data.

Regarding the Pulse oximeter sensor, the RED and IR output signals for its RED LED and IR LED are expected to be good signals because the controller is designed to control the current used by the RED and IR LEDs. In accordance with one aspect of the invention, the RED and IR output signals have a good dynamic range and avoid full signal saturation during normal measurements. Thus, the evaluation of invalid signal quality for pulse oximetry may be based on whether or not the actual signal measurements are fully saturated. If not fully or substantially saturated, the signal quality of the pulse oximeter sensor data is not invalid. If fully or substantially saturated, then the signal quality of the pulse oximeter sensor data may be deemed invalid. For poor signal quality of the pulse oximeter sensor data, the data samples may meet or exceed a lower poor threshold level but not the full saturation level. For good signal quality of pulse oximeter sensor data, the data samples may not meet or exceed both the lower poor threshold level and the full saturation level.

Similar to the Pulse oximeter, in accordance with one aspect of the invention, the ECG circuitry in the scanner is designed to output signals that have good dynamic range and avoid full saturation. Accordingly, the evaluation of invalid ECG data can be based on whether or not the actual measurements are fully saturated or substantially saturated. If not fully or substantially saturated, the signal quality of the ECG sensor data is not invalid. If fully or substantially saturated, then the signal quality of the ECG sensor data may be deemed invalid. For poor signal quality of the ECG sensor data, the data samples may meet or exceed a lower poor threshold level but not the full saturation level. For good signal quality of ECG sensor data, the data samples may not meet or exceed both the lower poor threshold level and the full saturation level.

Referring back to FIG. 12, other known methods may be used to quickly determine a quality of scan data (e.g., good, poor, or invalid scan signal data) that is being captured by each sensor. Regardless, the results of the evaluation processes **1203E** and **1203O**, and optionally the results of the temperature evaluation process **1203T**, may be logically fused together to determine an overall quality of good, poor, or invalid scan signal data being captured by the vital signs scanner.

To determine overall that good signal data is being captured, a logical AND operation is performed ANDing

together the conditions of good PulseOX **1216G** and good ECG **1215G**. Optionally, the condition of temperature within range **1214G** may also be ANDed together with good PulseOX **1216G** and good ECG **1215G** to determine that good scan signal data is being obtained. For example, if all of temperature within range **1214G**, good PulseOX **1216G**, and good ECG **1215G** are generated, then the overall scanned signal result is good. This overall result can then be fused together with the detected motion condition through the state machine **1220** to further refine the state and quality of scan signal data being captured by the vital signs scanner.

To determine overall that poor signal data is being captured, a logical OR operation is performed ORing together the conditions of poor PulseOX **1216P** and poor ECG **1215P**.

Optionally, the condition of temperature within range **1214G** may also be ANDed with the logic OR of the poor PulseOX **1216P** and the poor ECG **1215P** to determine that poor scan signal data is being obtained. Even though good temperature data may be scanned within temperature range **1214G**, poor PulseOX **1216P** or poor ECG **1215P** due to the scanner being pressed too hard or too light, the overall scanned signal data result is poor. This overall result can then be fused together with the detected motion condition through the state machine **1220** to further refine the state and quality of scan signal data being captured by the vital signs scanner.

To determine overall that invalid signal data is being captured, a logical OR operation is performed ORing together the conditions of invalid PulseOX **1216I** and invalid ECG **1215I**. For example, if either invalid PulseOX **1216I** or invalid ECG **1215I** are generated or true, the overall scanned signal result is invalid. Optionally, the condition of temperature outside range **1214P** may also be logically ORed together with invalid PulseOX **1216I** and invalid ECG **1215I**, to determine that invalid scan signal data is being obtained. In this case, if temperature outside range **1214P**, invalid PulseOX **1216I**, or invalid ECG **1215I** are generated or true, the overall scanned signal result is invalid. The overall scan signal result can then be fused together with the detected motion condition through the state machine **1220** to further refine the state and quality of scan signal data being captured by the vital signs scanner.

After evaluation of the acceleration envelope curve by the motion detection process **1207**, a condition **1217B**, **1217M**, or **1217S** of the detected motion can be assigned during the interactive scanning process. The detected motion conditions of the current scanning process include significant motion (big motion) **1217B**, minor motion (small motion) **1217M**, or no motion (still) **1217S**.

The detected motion condition may be assigned based upon an analysis of the envelope curves for the overall acceleration of the scanner in comparison with normal gravity. If there is a significant change or difference in overall acceleration of the scanner in comparison with gravity in a window of time, then significant or big motion **1217B** may be assigned. If there is a minor variation in overall acceleration of the scanner in comparison with gravity over a window of time, then the condition of minor motion **1217M** may be assigned. If there is little difference in overall acceleration of the scanner in comparison with gravity over a window of time, e.g., a steady state, then still or no motion **1217S** may be assigned.

The concurrent detected motion condition and the evaluation of each vital signs measurement for the given scanning session are combined together by a scan state machine **1220** to be a collaborative decision on the quality of the given scanning session. In response to the detected motion condition and the initial quality screening of vital signs data, the

current interactive scanning process may be assigned a state within the scan state machine **1220**. Evaluation of the audio sounds captured by the microphone of the scanner or portable device may also be considered in assigning a state for the scan state machine **1220**.

If the detected motion condition is significant or big motion **1217B**, none of the vital sign measurements are deemed accurate. The scan state machine **1220** may be assigned a scan state of significant motion **1221**, regardless of the results of the sensor data quality screening.

If the detected motion condition is small or minor motion **1217M** or no motion (still) **1217S**, the vital sign data quality plays a role in determining the fused scan state of the scan state machine **1220**. Methods of determining how the data quality states of good ECG data **1215G**, poor ECG data **1215P**, and invalid data ECG **1215I** were previously described. Methods of determining how the data quality states of good PulseOX data **1216G**, poor PulseOX data **1216P**, and invalid PulseOX data **1216I** were previously described. Methods of determining how the data quality states of within temperature range **1214G** and outside temperature range **1214P** were previously described.

If the detected motion condition is minor motion **1217M**, the quality of the vital signs data can cause the scan state machine **1220** to have the states good signal with motion **1224A**, poor signal with motion **1224B**, or invalid signal with motion **1224C** depending upon the screened quality of the vital sign data. If either the pulse oximeter data has a data quality state of invalid PulseOX data **1216I** or the ECG data has a data quality state of invalid ECG data **1215I**, then the scan state machine **1220** of the interactive scanning process may be assigned the scan state of invalid signal with motion **1224C**. If the pulse oximeter data has a data quality state of poor PulseOX data **1216P**, the ECG data has a data quality state of poor ECG data **1215P**, or the temperature data has a data quality state of outside temperature range **1214P**, then the scan state machine **1220** of the interactive scanning process may be assigned the scan state of poor signal with motion **1224B**. If the pulse oximeter data has a data quality state of good PulseOX data **1216G**, the ECG data has a data quality state of good ECG data **1215G**, and the temperature data has a data quality state of within temperature range **1214G**, then the scan state machine **1220** of the interactive scanning process may be assigned the scan state of good signal with motion **1224A**.

If the detected motion condition is still or no motion **1217S**, the quality of the vital signs data can cause the scan state machine **1220** to have the scan states of good signal **1226A**, poor signal **1226B**, or invalid signal **1226C**. If either the pulse oximeter (PulseOX) data has a data quality state of invalid PulseOX data **1216I** or the ECG data has a data quality state of invalid ECG data **1215I**, then the scan state machine **1220** of the interactive scanning process may be assigned the scan state of invalid signal **1226C**. If the pulse oximeter data has a data quality state of poor PulseOX data **1216P**, the ECG data has a data quality state of poor ECG data **1215P**, or the temperature data has a data quality state of outside temperature range **1214P**, then the scan state machine **1220** of the interactive scanning process may be assigned the scan state of poor signal **1226B**. If the pulse oximeter data has a data quality state of good PulseOX data **1216G**, the ECG data has a data quality state of good ECG data **1215G**, and the temperature data has a data quality state of within temperature range **1214G**, then the scan state machine **1220** of the interactive scanning process may be assigned the scan state of good signal **1226A**.

If the scan state machine **1220** reaches the scan state of good signal **1226A**, the interactive scanning process continues with the data being evaluated and measures a plurality of vital signs data that is saved and delivered to the digital device **104** from the scanner **102**. If any other state is assigned, user feedback may be generated to instruct the user on how to reach the good signal state **1226A**.

Referring now to FIGS. **15A-15B**, state diagrams for the scan state machine **1220** are illustrated to further explain the interactive scanning process provided by the portable vital signs scanner **102** and the vital signs scanning user interface **140**. FIG. **15A** illustrates the interactive scanning process, user feedback, and determinations made to maintain the same state. Previously the logic used to enter the states of the scan state machine **1220** was described in response to the quality of vital signs data and the motion detected of the scanner **102**. If the quality of scan data changes or the motion condition changes, the state machine transitions from one scan state to another. FIG. **15B** illustrates the interactive scanning process and the user feedback that may be generated during transitions between scan states.

An element of time (e.g., number of time windows, or a number of data samples) may be used by the state machines to determine if the scan state remains the same or transition to another states as the screening process continues. Furthermore, different user feedback may be generated in response to the scan state to interactively instruct the user on how to more properly use the scanner **102** and obtain better data quality. The scan state machine keeps track of the current scan state and the number of time windows over which the state machine has been in the current scan state. Time limits may be used in order to determine when to re-evaluate the current scan state (e.g., see determination blocks **1502,1506-1510** in FIG. **15A**) and if a transition to another scan state should be made. If a transition to another scan state is made, the time window count of the current scan state is reinitialized (e.g., see initialization blocks **1590A-1590F** in FIG. **15A**), such as to zero. The state machine may further keep track of history of past scan states to make various decisions regarding the user feedback to be generated.

The scanning process is initiated by the user by pressing the scan button in the user interface **140** on the device **104**. The scanner **102** is moved by the user towards his/her forehead temple for the primary scan or his/her chest for the secondary scan. The accelerometer sensor senses the substantial motion made to position the scanner **102** against the user's body establishing a big motion condition **1217B**. As the scanner **102** is pressed against the user's body, the motion detected by the accelerometer and the interactive scanning process over a time window may be reduced to the small motion condition **1217M** or the no motion condition **1217S**. With an initial motion condition of the big motion condition **1217B**, the state of the scan state machine **1220** has a big motion scan state **1221** as its initial state.

Assume the state of the scan state machine **1220** is the big motion scan state **1221**. After a first time limit **A** has been exceeded while in the big motion scan state **1221**, a determination is made at process **1502** if the scan state continues to be the big motion scan state **1221**. If yes, user feedback **1523** is generated asking the user if he/she is playing with the scanner. The counter is incremented to keep a current count of the number of time windows the state machine remains in the big motion scan state **1221**. If the scan state is no longer in the big motion scan state **1221**, the counter is cleared or reinitialized by the initialization block **1590A**. The scan state may no longer be in the big motion scan state

1221 if the accelerometer sensor no longer senses big motion. The scan state machine goes to a different scan state in response to the fused scan data quality and the motion condition.

The invalid signal with motion state 1224C and the invalid signal state 1226C form an invalid super state 1540. Assume the scan state is in the invalid super state 1540 of either the invalid signal with motion state 1224C or the invalid signal state 1226C. Next at process 1506, after a second time limit B has been exceeded while in the super state 1540, a determination is made if the fused scan data quality and motion condition continues to form the invalid super state 1540. If yes, user feedback 1524C is generated asking the user to please make contact with the scanner. The counter is incremented to keep a current count of the number of time windows the state machine remains in the invalid super state 1540. If the scan state is no longer in the invalid super state 1540, the counter is cleared or reinitialized by the initialization block 1590B. The scan state may no longer be in the invalid super state 1540 if a better scan data quality is determined by the screening process. For example, the scan state machine may go to a poor signal with motion state 1224B or a poor signal state 1226B. Alternatively, with still better scan data quality, the scan state machine may go to a good signal with motion state 1224A or a good signal state 1226A.

Assume the scan state machine is in the poor signal with motion state 1224B. At process 1507, after a third time limit C has been exceeded while in the poor signal with motion state 1224B, a determination is made if the fused scan data quality and motion condition continues to form the poor signal with motion state 1224B. If yes, user feedback 1524B is generated asking the user if he is pressing too gently in order to prompt him to press harder to make better contact. The counter is incremented to keep a current count of the number of time windows the state machine remains in the poor signal with motion state 1224B. If the scan state is no longer in the poor signal with motion state 1224B, the counter is cleared or reinitialized by the initialization block 1590C. The scan state may no longer be in the poor signal with motion state 1224B if either the accelerometer sensor no longer senses small motion and the scan state machine goes to the poor signal state 1226B in response to the change in the motion condition or to a different scan signal state in response to a better scan data quality or worse can data quality. For example, the scan state machine may go to a poor signal state 1226B if motion condition goes to a still or no motion condition 1217S. With better scan data quality, the scan state machine may go to a good signal with motion state 1224A or a good signal state 1226A if the motion condition also changes to the no motion condition 1217S. With poorer scan data quality, the scan state machine may go to the invalid signal with motion state 1224C or the invalid signal state 1226C if the motion condition also changes to the no motion condition 1217S.

Assume the scan state machine is in the poor signal state 1226B. At process 1508, after a fourth time limit D has been exceeded while in the poor signal state 1226B, a determination is made if the fused scan data quality and motion condition continues to form the poor signal state 1226B. If yes, user feedback 1524D is generated asking the user if he is pressing too tight in order to prompt him to press less hard to make a better contact. The counter is incremented to keep a current count of the number of time windows the state machine remains in the poor signal state 1226B. If the scan state is no longer in the poor signal state 1226B, the counter is cleared or reinitialized by the initialization block 1590D.

The scan state may no longer be in the poor signal state 1226B, if the accelerometer sensor no longer senses absence of motion and either the scan state machine goes to the poor signal with motion state 1224B in response to the change in the motion condition, or the scan state machine goes to a different scan signal state in response to a better or worse can data quality. For example, the scan state machine may go to a poor signal with motion state 1224B if motion condition goes to a small or minor motion condition 1217M. With better scan data quality, the scan state machine may go to a good signal state 1226A or a good signal with motion state 1224A if the motion condition also changes to the minor motion condition 1217M. With poorer scan data quality, the scan state machine may go to the invalid signal state 1226C or the invalid signal with motion state 1224C if the motion condition also changes to the minor motion condition 1217M.

Assume the scan state machine is in the good signal with motion state 1224A. At process 1509, after a fifth time limit E has been exceeded while in the good signal with motion state 1224B, a determination is made if the fused scan data quality and motion condition continues to form the good signal with motion state 1224A. If yes, user feedback 1524A is generated asking the user to hold still for a good scan. The counter is incremented to keep a current count of the number of time windows the state machine remains in the good signal with motion state 1224A. If the scan state is no longer in the good signal with motion state 1224A, the counter is cleared or reinitialized by the initialization block 1590E. The scan state may no longer be in the good signal with motion state 1224A if either the accelerometer sensor no longer senses small motion and the scan state machine goes to the good signal state 1226A in response to the change in the motion condition or to a different scan signal state in response to worse scan data quality. For example, the scan state machine may go to a good signal state 1226A if the motion condition goes to a still or no motion condition 1217S. With poorer scan data quality, the scan state machine may go to the poor signal with motion state 1224B or the poor signal state 1226B, or the invalid super state 1540.

Assume the scan state machine is in the good signal state 1226A. At process 1510, a determination is made if the fused scan data quality and motion condition continues to form the good signal state 1226A. If yes, user feedback may be generated in the form of a scan progress bar 1599 or otherwise inform the user that good scan data quality is being achieved. The counter is incremented to keep a current count of the number of time windows the state machine remains in the good signal state 1226A. If the scan state is no longer in the good signal state 1226A, the counter is cleared or reinitialized by the initialization block 1590F. The scan state may no longer be in the good signal state 1226A if the accelerometer sensor no longer senses absence of motion and the scan state machine goes to the good signal with motion state 1224A in response to the change in the motion condition. The scan state may no longer be in the good signal state 1226A in response to a poorer can data quality. For example, the scan state machine may go to the poor signal state 1226B, the poor signal with motion state 1224B, or the invalid signal super state 1540.

Referring now to FIG. 15B, user feedback (positive user feedback or negative user feedback) may be generated and presented to a user as the scan data quality causes a transition between scan signal states or the motion condition changes to cause a transition between scan signal states. As mentioned previously, audible user feedback may be generated by a speaker or audible generator in the scanner 102

or the device **104**. Visual user feedback may be generated by the user interface **140** on the display of the device **104**.

Scan signal states **1224A-1224C** associated with the minor motion condition **1217M** may be collectively referred to as a minor motion super state **1570A**. Scan signal states **1226A-1226C** associated with the still motion condition **1217S** may be collectively referred to as a no motion super state **1570B**.

User feedback may be generated and presented to a user as a change in the motion condition causes a transition between scan states. The occurrence of big motion **1217B** can result in a jump to the big motion scan state **1221** from either the minor motion super state **1570A** or the no motion super state **1570B**. User feedback **1516A** may be generated asking the user audibly and/or visually if he/she is shaking the scanner **102**.

If the scan state is one of the no motion super states **1570B** and if motion is detected by the accelerometer over a time window such that the interactive scanning process reverts back to one of the scan states in the minor motion super states **1570A**, user feedback **1516B** may be generated. The user feedback **1516B** may be presented to the user audibly and/or visually asking him/her to please hold still.

If in the good signal with motion scan state **1224A**, the motion detected by the accelerometer and the interactive scanning process over a time window is substantially reduced to still or no motion, the scan state may transition to the good scan state **1226A**. In this case, user feedback **1516C** may be generated during the transition providing positive user feedback, such as great job, and presented to the user audibly or visually on the display device **202** of the device **104**.

In FIG. **15B**, user feedback may be generated and presented to a user as the scan data quality causes a transition between scan signal states. For example, a transition from either the invalid signal with motion state **1224C** or the invalid signal state **1226C** to a better level of scan data quality and scan state, positive user feedback **1525B** may be generated and inform the user that he/she is making better contact to reinforce the improvement. On the other hand, a transition from either the good signal with motion state **1224A** or the good signal state **1226A** to a poorer level of scan data quality and scan state, negative user feedback **1525A** may be generated and inform the user that he/she is losing good contact with the scanner **102** to alter the behavior of the user.

Referring now back momentarily to FIG. **15A**, if the vital signs control system goes to the good signal state **1226A**, then the scanning process can continue and start making measurement calculations for the vital signs. Some of the data in the screening process if of good quality may be used to perform the calculation. If not, added time is used to obtain the needed data to perform the calculations. In the good signal state **1226A**, user feedback **1599** is generated by displaying a scan progress bar to user, for example. While in the good signal state **1226A**, the scan state is continuously reevaluated by the state machine **1220**. For example if small motion **1217M** or big motion **1217B** are detected, measurement calculations may be paused due to a transition away from the good signal state **1226A**. The scan states may revert to states other than the good signal state **1226A**. In which case, the scan progress bar **1599** is interrupted and additional user feedback may be provided on how to continue or restart the scanning process. For example, the scan progress bar **1599** may be reset if the scanning process is restarted from the beginning.

Referring now back momentarily to FIG. **15A**, before measurement calculations are presented to the user, the scan quality may optionally be confirmed at block **1560** of the interactive scanning process. If the scan quality cannot be confirmed, the scan progress bar may be interrupted and additional user feedback may be provided on how to continue or restart the scanning process. For example, the scan progress bar **1599** may be reset if the scanning process is restarted from the beginning.

Scan quality can be confirmed by performing additional measurement calculations. Alternatively or additionally, scan quality can be confirmed by using multiple time windows. The multiple time windows may be fused together to confirm that the scan data is really good by measuring the scan data against expected curve. An element of time is aligned between the scan data curve and an expected curve. Time alignment between curves is possible for both ECG and PPG curves because the shape and peaks of the curves are distinct and can be detected, for example, by match filtering.

Referring now to FIGS. **17A-17C**, the quality of a vital sign VS measurement calculations that were made can be confirmed using an expected curve **1750**. In FIG. **17A**, data samples **1701A** of the vital sign VS captured by the vital signs scanner **102** are plotted against an axis of time T. The data samples **1701A** undergo envelope detection to generate an envelope curve **1702A** of measured data. The envelope curve **1702A** is compared with the expected curve **1750**. If the pattern of the envelope curve **1702A** over a given period of time matches the pattern of the expected curve **1750**, then the good quality of the vital sign is confirmed.

In FIG. **17B**, data samples **1701B** of the vital sign VS captured by the vital signs scanner **102** are plotted against an axis of time T. The data samples **1701B** undergo envelope detection to generate an envelope curve **1702B** of measured data. The envelope curve **1702B** of the vital sign is compared with the expected curve **1750**. If the pattern of the envelope curve **1702B** over a given period of time does not match the pattern of the expected curve **1750**, then the good quality of the vital sign is not confirmed.

In FIG. **17C**, data samples **1701C** of the vital sign VS captured by the vital signs scanner **102** are plotted against an axis of time T. The data samples **1701C** undergo envelope detection in an attempt to generate an envelope curve **1702C** of measured data. The envelope curve **1702C** of the vital sign is compared with the expected curve **1750**. If the pattern of the envelope curve **1702C** over a given period of time has no bearing whatsoever to the expected curve **1750**, then again the good quality of the vital sign is not confirmed.

The quality of the sensor data for the ECG sensor and the quality of the sensor data for the pulse oximeter sensor may both be determined by comparing against expected curves.

If the pattern of the envelope curve of the sensor data for the ECG sensor over a given period of time matches the pattern of an expected ECG curve, then the quality of the ECG data for the ECG vital sign is confirmed to be good. If the pattern of the envelope curve of the sensor data for the ECG sensor over a given period of time does not match the pattern of the expected ECG curve, then the good quality of the of the ECG data is not confirmed. If the pattern of the envelope curve of the sensor data for the ECG sensor over a given period of time has no bearing whatsoever to the expected ECG curve, then a good quality of the of the ECG data for the vital sign is not confirmed.

If the pattern of the envelope curve of the sensor data for the pulse oximeter sensor over a given period of time matches the pattern of an expected pulse oximeter curve,

then the quality of the pulse oximeter data for a vital sign is confirmed to be good. If the pattern of the envelope curve of the sensor data for the pulse oximeter sensor over a given period of time does not match the pattern of the expected pulse oximeter curve, then a good quality of the of the pulse oximeter data for the vital signs is not confirmed. If the pattern of the envelope curve of the sensor data for the pulse oximeter sensor over a given period of time has no bearing whatsoever to the expected pulse oximeter curve, then a good quality of the of the pulse oximeter sensor data for the vital signs is not confirmed.

If the measurement calculations are optionally confirmed at block 1560 during the interactive scanning process, the measurement calculations may be presented to the user.

Sensor Data Fusion for Improved Vital Signs Measurements

While user feedback may be used during an interactive scanning process to improve scan quality, the plurality of different types of vital signs data may also be used to improve the data quality by combining or fusing data together.

Referring now to FIG. 16, a flow chart of methods including sensor data fusion to improve vital sign measurements is illustrated. The vital signs scanner 120 integrates a plurality of vital sign sensors 812, 880, 885, 860, 875 into a low cost finger held device. The plurality of vital signs sensors concurrently sense data over one or more periods of time generating sensor data 1650 associated with vital signs of a human body. The sensor data 1650 includes sensed data 1602, 1603A-1603D, 1604A-1604C, 1605A-1605C, 1606A-1606B from each of the respective vital signs sensors 812, 880, 885, 860, 875.

The sensed data 1602, 1603A-1603D, 1604A-1604C, 1605A-1605C, 1606A-1606B from each of the respective vital signs sensors 812, 880, 885, 860, 875 is used to concurrently determine a plurality of vital signs values for a respective plurality of vital signs for a given time and date. Internal logic within the vital signs scanner 120 generates values for vital signs such as surface temperature 1612, pulse blood volume 1613, and pulse rate 1614, for example.

As the vital sign data is concurrently determined from each sensor, they are related by time and date. There may be a further relatedness between two or more sensed data types or two or more vital sign values. This relatedness may be exploited by fusing together two or more types of sensed data or two or more vital sign values together to improve accuracy/quality or to form a new, different, or related vital sign.

For example, PPG sensor data 1603C, accelerometer data of the chest area, and ECG sensor data 1605 may be fused together to determine pulse wave transit time (PWTT) 1616 that is directly related to blood pressure. PWTT can also be calculated non-invasively from ECG sensor data and SpO2 sensor data. The technology employed for blood pressure measurement may be based on the PWTT technology described in U.S. Pat. No. 5,564,427 filed by Aso et al. incorporated herein by reference. The PWTT technology described in U.S. Pat. No. 5,564,427 may be modified to improve PWTT measurements.

The precision of a PWTT measurement may be enhanced by particular methods of cross-correlation. Additionally, epidemic biometrics (user biometrics) 1617 may also be fused together with the PWTT data 1616 (derived from accelerometer data, ECG data, and PPG sensor data) by a blood pressure algorithm 1627. For example, one or more of a user's biometrics of age, height, and weight (user biometrics) may be fused together with the PWTT data 1616 to determine blood pressure. Large scale curated datasets or

databases of hypertension may be fused along with the blood pressure. Likewise temperature may be used as an additional input in order to enhance the accuracy of both systolic and diastolic blood pressure measurements.

Two or more vital sign values of different vital signs may be fused together by mathematical algorithms to improve the accuracy or quality of the values of the one or more vital signs. Alternatively, two or more vital sign values may be fused together by mathematical algorithms to form a value for a new and different vital sign for which data is not sensed. For example, surface body temperature 1612 sensed by the infrared thermometer sensor 812 may be fused together with pulse blood volume 1613 sensed by the PPG sensor 880.

Knowing the volume of blood at a core temperature that enters the microcirculation under a probed region, and knowing the external surface body temperature, the value of core temperature T_{core} can be obtained. Internal core temperature can be computed if the ambient temperature and the Skin surface temperature are known both of which we get from the Melexis sensor. Heat flux q passes from the core temp (T_a) through the skin to the ambient environment (T_a) where the skin surface temp (T_s) is held at some intermediary temp between core and ambient temp. An equation for core temperature is $T_c = (h/pc)(T_s - T_a) + T_s$ where h/pc is a weighting coefficient that weights the difference in skin surface and ambient temperature and is determined empirically on a statistical basis over different patients and different clinical situations.

In this manner, the surface body temperature and the pulse blood volume may be fused together by the temperature algorithm 1622 to determine core body temperature as well as improve the surface temperature 1632. U.S. Pat. No. 7,787,938 issued to Franceso Pompei on Aug. 31, 2010 describes further details of determining temperature in this manner and is incorporated by reference.

Acceleration data (motion) 1604A from the accelerometer 885 and acoustic sensor data 1606A from the stereo microphone 875 may also be fused together by mathematical algorithms, with or without the vital sign values from the vital sign sensors, to improve the accuracy or quality of vital sign values or form a value for a different vital sign. For example, a fusion formula 1626 may be used to fuse acoustic sensor data 1606A and an axis of acceleration data to determine respiration rate 1636. A 3D splitter 1615 splits up three axes of data from a tri-axis accelerometer 885.

The formula 1623 that may be used to convert PPG sensor data 1603A-1603D into SPO2 data 1633 is described for example in "Pulse Oximetry: Theory and Applications for Noninvasive Monitoring" by Yitzhak Mendelson, CLIN. CHEM. 38/9, 1601-1607 (1992); and Noninvasive Pulse Oximetry Utilizing Skin Reflectance Photoplethysmography" by Yitzhak Mendelson and Burt D. Ochs, IEEE Trans. On Biomedical Engineering, Vol. 35, No. 10, October 1988, pages 798-805.

A comparator formula 1624 can fuse pulse rate 1614, accelerometer data 1604, and ECG sensor data 1605 together to obtain heart rate information 1634. Electrocardiogram (ECG) data 1605 can be further evaluated with formulas 1625 to obtain the PR interval, the QRS shape, the ST interval, and more ECG information 1635 that is used to determine heart activity. This ECG information can be further processed by algorithms 1639 to determine heart rate variability (HRV), the variation in the time interval between heartbeats, or other conditions of a users heart, as well as stress 1649.

41

One or more algorithms **1628** may be used to extract sound signals from well defined frequency bands relative to wheezing and murmurs. Wheezings and murmurs have very different pitches and can be easily separated on a frequency basis, even without their full spectral envelopes. The extracted sounds of wheezings and murmurs may be used to diagnose chronic obstructive pulmonary disease (COPD) or asthma **1638**.

The vital signs user interface (VSUI) **140** can be used to store and present much of the vital signs data to a user including core temperature **1642**, SPO2 data **1643**, heart rate **1644**, ECG data **1645**, respiration rate **1646**, blood pressure **1647**, and stress levels **1649**.

Additional information may be requested by the user by using the vital signs user interface (VSUI) through information requests **1643**, **1652**, and **1657A-1657B** to better diagnose a condition.

CONCLUSION

Various specific materials, designs, dimensions, etc. are provided and are considered highly beneficial embodiments of the present disclosure in one regard. However, in other regard, such specifics are also merely illustrative of broader aspects of the present disclosure and should not be considered to necessarily limit to such broader aspects unless expressly specified to be required. In particular, the various specific dimensions provided as such examples are intended to be about any particular values provided, with typical tolerances and ranges of suitable alternatives as would be apparent to one of ordinary skill. Where particular combinations of such dimensions are provided for exemplary illustration of certain embodiments, the relative relationships between them are also contemplated as having been herein disclosed as additional beneficial aspects (even if the specific values of the relative dimensions change). For example, certain lengths, widths, and/or depths of particular components shown and described for a particular assembly provide overall geometries which may be varied by changing certain sub-sets of such dimensions, but may also be fixed relative to the ratios of these values despite the valued changing (so long as their general relationship remains). Similarly, such dimensions of different component parts also have similar relative relationships which are similarly contemplated, also as apparent to one of ordinary skill.

When implemented in software, the elements of the embodiments of the invention are essentially the code segments or instructions to perform the functional tasks described herein. The code segments or instructions are executable by a processor, such as processor **206**, **840**, and can be stored in a storage device or a processor readable storage medium, such as memory **208**, **841**, awaiting execution. The processor readable storage medium may include any medium that can store information. Examples of the processor readable storage medium include an electronic circuit, a semiconductor memory device, a read only memory (ROM), a flash memory, an erasable programmable read only memory (EPROM), a floppy diskette, a CD-ROM, an optical disk, a hard disk. The code segments or instructions may be downloaded via computer networks such as the Internet, Intranet, etc. into the processor readable storage medium.

Various combinations and sub-combinations, and modifications as may be made, of the presently disclosed components and embodiments and aspects are contemplated whether or not specifically disclosed hereunder, to the extent and as would be apparent to one of ordinary skill based upon

42

review of this disclosure and in order to suit a particular intended purpose or application.

While certain embodiments of the disclosure have been described, these embodiments have been presented by way of example only, and are not intended to limit the scope of the disclosure. Indeed, the novel methods, systems, and devices described herein may be embodied in a variety of other forms. Furthermore, various omissions, substitutions and changes in the form of the methods, systems, and devices described herein may be made without departing from the spirit of the disclosure. For example, certain features that are described in this specification in the context of separate implementations may also be implemented in combination in a single implementation. Conversely, various features that are described in the context of a single implementation may also be implemented in multiple implementations, separately or in sub-combination. Moreover, although features may be described above as acting in certain combinations and even initially claimed as such, one or more features from a claimed combination may in some cases be excised from the combination, and the claimed combination may be directed to a sub-combination or variations of a sub-combination. Accordingly, the claimed invention is to be limited only by patented claims that follow below.

What is claimed is:

1. A method comprising:

concurrently scanning for a plurality of vital signs with a plurality of sensors of a portable vital signs scanner to generate vital signs scan data;

detecting movement with an accelerometer of the portable vital signs scanner during the scanning for the plurality of vital signs;

generating first scan data from the vital signs scan data, the first scan data comprising a first category of health status information;

based upon the first scan data, selecting a first scan state from a set of stored scan states;

tracking a number of time windows for the first scan state, the time windows being for measuring a quality of the vital signs scan data;

comparing the first scan data to a stored predetermined range for the first category of health information to generate a scan comparison; and

in response to the scan comparison and the detected movement, determining a measure of quality of the vital signs scan data.

2. The method of claim 1, further comprising:

generating user feedback to present to a user in response to the determined measure of quality of the concurrent scan for the plurality of vital signs.

3. The method of claim 1, further comprising:

generating user feedback to present to a user in response to determining an invalid or unreliable measure of quality of the concurrent scan for the plurality of vital signs.

4. The method of claim 1, further comprising:

generating user feedback to present to a user in response to determining a reliable measure of quality of the concurrent scan for the plurality of vital signs and minor movement of the portable vital signs scanner.

5. The method of claim 1, further comprising:

generating user feedback to present to a user in response to determining significant movement of the portable vital signs scanner, regardless of the measure of quality of the concurrent scan for the plurality of vital signs.

43

6. The method of claim 1, further comprising:
generating user feedback to present to a user in response
to repeatedly determining a reliable measure of quality
of the concurrent scan for the plurality of vital signs
without movement of the portable vital signs scanner. 5
7. The method of claim 6, wherein
the measure of quality of the scan for the plurality of vital
signs during the period of time is reliable if the scan
data for a pulse oximeter vital sign and the scan data for
an electrocardiogram (ECG) vital sign is evaluated to
be reliable scan data. 10
8. The method of claim 6, wherein
the measure of quality of the scan for the plurality of vital
signs during the period of time is reliable if the scan
data for a pulse oximeter vital sign is evaluated to be
reliable scan data, the scan data for an electrocardio-
gram (ECG) vital sign is evaluated to be reliable scan
data, and if scan data for a temperature vital sign is
within an expected range. 15 20
9. The method of claim 6, wherein
the user feedback that is generated is a scan progress bar
that is filled in as a fraction of progress is made in
generating measurements for the plurality of vital
signs. 25
10. The method of claim 9, wherein
the fraction is each tenth of progress made in generating
measurements for the plurality of vital signs.
11. The method of claim 9, wherein
during a second period of time, the measure of quality of
the scan for the plurality of vital signs becomes unre-
liable; and 30
- the scan progress bar is paused or reset in response to the
unreliable measure of scan quality. 35
12. The method of claim 3, wherein
the measure of quality of the scan for the plurality of vital
signs during the period of time is unreliable if either the
scan data for a pulse oximeter vital sign or the scan data
for an electrocardiogram (ECG) vital sign is evaluated
to be unreliable scan data. 40
13. The method of claim 3, wherein
the measure of quality of the scan for the plurality of vital
signs during the period of time is unreliable if scan data
for a temperature vital sign is within an expected range
and either the scan data for a pulse oximeter vital sign
is evaluated to be unreliable scan data or the scan data
for an electrocardiogram (ECG) vital sign is evaluated
to be unreliable scan data. 45
14. The method of claim 2, further comprising: 50
determining that significant motion of the portable vital
signs scanner was detected during a period of time; and
wherein the user feedback is generated to inquire of a user
if he is playing with the portable vital signs scanner.
15. The method of claim 2, further comprising: 55
determining that the measure of quality of the scan for the
plurality of vital signs during a period of time is invalid;
and
wherein the user feedback is generated to instruct a user
to make contact with the portable vital signs scanner to
the user's body. 60
16. The method of claim 15, wherein
the measure of quality of the of the scan for the plurality
of vital signs during the period of time is invalid if
either scan data for a pulse oximeter vital sign or scan
data for an electrocardiogram (ECG) vital sign is
evaluated to be invalid scan data. 65

44

17. The method of claim 15, wherein
the measure of quality of the scan for the plurality of vital
signs during the period of time is invalid if either scan
data for a pulse oximeter vital sign is evaluated to be
invalid scan data, scan data for an electrocardiogram
(ECG) vital sign is evaluated to be invalid scan data, or
scan data for a temperature vital sign is outside an
expected range.
18. The method of claim 2, further comprising:
determining that the measure of quality of the scan for the
plurality of vital signs during a period of time is
unreliable with minor motion; and
wherein the user feedback is generated to inquire if a user
is pressing the scanner too lightly and instruct the user
to press the portable vital signs scanner tighter against
the user's body.
19. The method of claim 2, further comprising:
determining that the measure of quality of the scan for the
plurality of vital signs during a period of time is
unreliable without motion; and
wherein the user feedback is generated to inquire if a user
is pressing the scanner too tightly and instruct the user
to press the scanner with less force against the user's
body.
20. The method of claim 2, further comprising:
determining that the measure of quality of the scan for the
plurality of vital signs during a period of time is reliable
with motion; and
wherein the user feedback is generated to instruct a user
to hold still for a reliable scan.
21. The method of claim 2, further comprising:
determining that the measure of quality of the scan for the
plurality of vital signs transitions between levels of
quality from reliable to unreliable or unreliable to
invalid; and
the user feedback is generated to instruct a user that the
portable vital signs scanner is losing reliable contact.
22. The method of claim 2, wherein
determining that the measure of quality of the scan for the
plurality of vital signs transitions between levels of
quality from invalid to unreliable or unreliable to
reliable; and
the user feedback is generated to instruct a user that the
portable vital signs scanner is making better contact.
23. The method of claim 2, further comprising:
determining that the measure of quality of the scan for the
plurality of vital signs transitions between from reliable
with motion to reliable without motion; and
the user feedback is generated to instruct a user that he/she
has done a great job reaching the reliable scan state.
24. The method of claim 23, wherein
determining that the measure of quality of the scan for the
plurality of vital signs transitions between from a still
super state to a minor motion super state; and
the user feedback is generated to instruct a user to please
hold still.
25. The method of claim 2, further comprising:
determining that the measure of quality of the scan for the
plurality of vital signs transitions between from a still
super state to a big motion state or from a minor motion
super state to the big motion state; and
the user feedback is generated to inquire of a user if he/she
is shaking the portable vital signs scanner.
26. The method of claim 1, wherein
the concurrent scanning for the plurality of vital signs
with the portable vital signs scanner generates a plu-
rality of data samples of each vital sign; and

45

the determining of the measure of quality of the scanning for the plurality of vital signs includes detecting an envelope curve of amplitude from the plurality of data samples for each vital sign.

27. The method of claim 26, wherein the detecting of the movement of the portable vital signs scanner includes detecting acceleration of the portable vital signs scanner to obtain a plurality of data samples associated with movement of the portable vital signs scanner, and detecting an envelope curve of amplitude from the plurality of data samples associated with the movement of the portable vital signs scanner.

28. The method of claim 27, wherein the detecting of the movement of the portable vital signs scanner further includes determining a level of movement of the portable vital signs scanner.

29. The method of claim 28, wherein the level of movement of the portable vital signs scanner is big motion if the detected acceleration is greater than or equal to one-tenth of gravitational force.

30. The method of claim 28, wherein the level of movement of the portable vital signs scanner is minor motion if the detected acceleration is greater than or equal to two hundredths of gravitational force and less than one-tenth of gravitational force.

46

31. The method of claim 30, wherein the level of movement of the portable vital signs scanner is no motion or absence of motion if the detected acceleration is less than two hundredths of gravitational force.

32. The method of claim 26, wherein the determining of the measure of quality of the scanning for at least one vital sign includes comparing an amplitude of a data sample of the at least one vital sign with a first threshold level to determine an invalid scan data quality.

33. The method of claim 32, wherein the determining of the measure of quality of the scanning for at least one vital sign further includes comparing the amplitude of the data sample of the at least one vital sign with a second threshold level to discriminate between an unreliable scan data quality and a reliable scan data quality for the at least one vital sign.

34. The method of claim 26, wherein the at least one vital sign is body temperature, and the normal average body temperature taken at a forehead of an adult is ninety-seven and seven-tenths degrees Fahrenheit (97.7 F) with an expected range of plus and minus twelve degrees Fahrenheit (12 F) such that the expected temperature range is between one-hundred nine and seven-tenths degrees Fahrenheit (109.7 F) and eighty-five and seven-tenths degrees Fahrenheit (85.7 F).

* * * * *

专利名称(译)	个人便携式无线生命体征扫描仪的数据采集质量和数据融合方法		
公开(公告)号	US10143425	公开(公告)日	2018-12-04
申请号	US14/292820	申请日	2014-05-30
[标]申请(专利权)人(译)	思勘度股份有限公司		
申请(专利权)人(译)	SCANADU INCORPORATED		
当前申请(专利权)人(译)	SCANADU INCORPORATED		
[标]发明人	ZHAO WENYI WOOLSEY BRANDON DENNIS DE BROUWER WALTER VILLARREAL ERON ANTHONY ZIZI MARTIN		
发明人	ZHAO, WENYI WOOLSEY, BRANDON DENNIS DE BROUWER, WALTER VILLARREAL, ERON ANTHONY MCGOWAN, WHITNEY MORGAN ZIZI, MARTIN		
IPC分类号	A61B5/00 A61B5/0205 A61B5/11 A61B5/1455 A61B5/0402		
CPC分类号	A61B5/7221 A61B5/02055 A61B5/0402 A61B5/14551 A61B5/742 A61B5/11 A61B5/0024 A61B5/0295 A61B5/6826 A61B5/7282 A61B5/7405 A61B2562/04 A61B2562/162 A61B2562/166 G16H10/20 G16H20/30 G16H40/63		
优先权	61/924230 2014-01-06 US 61/875681 2013-09-09 US		
外部链接	Espacenet		

摘要(译)

在本发明的一个实施例中，公开了一种交互式生命体征扫描方法，包括用便携式生命体征扫描仪同时扫描多个生命体征；在扫描多个生命体征期间检测便携式生命体征扫描仪的移动；并且利用便携式生命体征扫描仪确定多个生命体征的扫描质量的度量。在另一个实施例中，公开了一种改善生命体征数据质量的方法，包括利用便携式生命体征扫描仪在一段时间内同时感测来自多个生命体征传感器的数据；响应于在一段时间内来自多个生命体征传感器的感测数据，确定相应多个生命体征的多个生命体征值；并且为相应的多个生命体征融合多个生命体征值的至少两个生命体征值。

