



US009492110B2

(12) **United States Patent**
Al-Ali et al.

(10) **Patent No.:** **US 9,492,110 B2**
(45) **Date of Patent:** ***Nov. 15, 2016**

(54) **PHYSIOLOGICAL MONITOR**

(71) Applicant: **Masimo Corporation**, Irvine, CA (US)

(72) Inventors: **Ammar Al-Ali**, Tustin, CA (US);
Mohamed K. Diab, Ladera Ranch, CA
(US); **Massi E. Kiani**, Laguna Niguel,
CA (US); **Robert James Kopotic**,
Jamul, CA (US); **David Tobler**,
Westminster, CO (US)

(73) Assignee: **MASIMO CORPORATION**, Irvine,
CA (US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 0 days.

This patent is subject to a terminal dis-
claimer.

(21) Appl. No.: **14/275,691**

(22) Filed: **May 12, 2014**

(65) **Prior Publication Data**

US 2015/0018650 A1 Jan. 15, 2015

Related U.S. Application Data

(63) Continuation of application No. 13/745,590, filed on
Jan. 18, 2013, now Pat. No. 8,721,541, which is a
(Continued)

(51) **Int. Cl.**
A61B 5/00 (2006.01)
A61B 5/1455 (2006.01)
(Continued)

(52) **U.S. Cl.**
CPC **A61B 5/14551** (2013.01); **A61B 5/0205**
(2013.01); **A61B 5/1459** (2013.01); **A61B**

5/6814 (2013.01); **A61B 5/6815** (2013.01);
A61B 5/6819 (2013.01); **A61B 5/6825**
(2013.01); **A61B 5/6826** (2013.01); **A61B**
5/6829 (2013.01); **A61B 5/6838** (2013.01);
A61B 5/742 (2013.01); **A61B 5/746** (2013.01);
(Continued)

(58) **Field of Classification Search**

None
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,704,706 A 12/1972 Herczfeld et al.
3,847,483 A 11/1974 Shaw et al.
(Continued)

FOREIGN PATENT DOCUMENTS

EP 0 555 553 8/1993
EP 0 807 402 11/1997
(Continued)

OTHER PUBLICATIONS

US 8,845,543, 09/2014, Diab et al. (withdrawn)
(Continued)


Primary Examiner — Etsub Berhanu

(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson
& Bear, LLP

(57) **ABSTRACT**

A patient monitor has multiple sensors adapted to attach to
tissue sites of a living subject. The sensors generate sensor
signals that are responsive to at least two wavelengths of
optical radiation after attenuation by pulsatile blood within
the tissue sites.

15 Claims, 25 Drawing Sheets

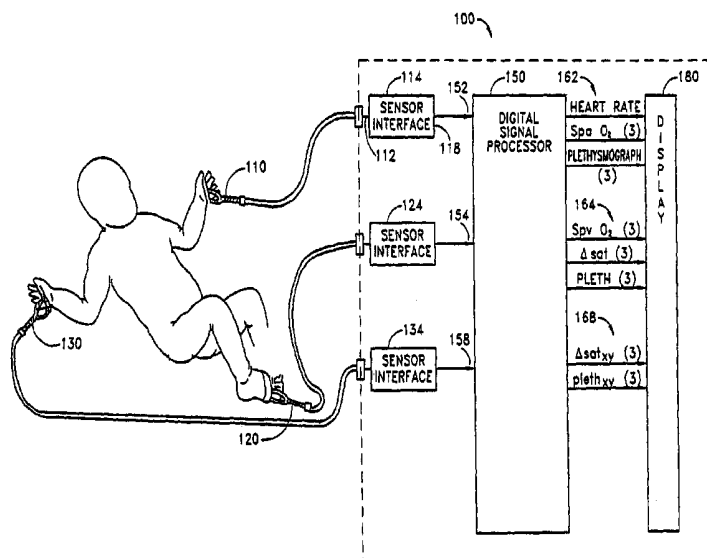

Related U.S. Application Data

continuation of application No. 11/417,931, filed on May 3, 2006, now Pat. No. 8,364,223, which is a continuation of application No. 11/104,720, filed on Apr. 13, 2005, now Pat. No. 7,761,128, which is a continuation of application No. 10/668,487, filed on Sep. 22, 2003, now Pat. No. 6,898,452, which is a continuation of application No. 10/026,013, filed on Dec. 21, 2001, now Pat. No. 6,714,804, which is a continuation of application No. 09/323,176, filed on May 27, 1999, now Pat. No. 6,334,065.

- (60) Provisional application No. 60/087,802, filed on Jun. 3, 1998.

(51) **Int. Cl.**

A61B 5/0205 (2006.01)

A61B 5/1459 (2006.01)

A61B 5/024 (2006.01)

A61M 16/00 (2006.01)

(52) **U.S. Cl.**

CPC *A61B 5/02416* (2013.01); *A61M 16/00* (2013.01); *A61M 2230/205* (2013.01)

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,109,643 A 8/1978 Bond et al.
 4,653,498 A 3/1987 New, Jr. et al.
 4,854,699 A 8/1989 Edgar, Jr.
 4,869,253 A 9/1989 Craig, Jr. et al.
 4,911,167 A 3/1990 Corenman et al.
 4,927,264 A 5/1990 Shiga et al.
 4,934,372 A 6/1990 Corenman et al.
 4,960,128 A 10/1990 Gordon et al.
 4,964,408 A 10/1990 Hink et al.
 5,020,516 A 6/1991 Biondi et al.
 5,041,187 A 8/1991 Hink et al.
 5,069,213 A 12/1991 Polczynski
 5,078,136 A 1/1992 Stone et al.
 5,163,438 A 11/1992 Gordon et al.
 5,218,962 A * 6/1993 Mannheimer et al. 600/331
 5,233,991 A * 8/1993 Wright 600/410
 5,251,632 A 10/1993 Delpy
 5,253,645 A 10/1993 Friedman et al.
 5,273,036 A 12/1993 Kronberg et al.
 5,308,919 A 5/1994 Minnich
 5,319,355 A 6/1994 Russek
 5,337,744 A 8/1994 Branigan
 5,341,805 A 8/1994 Stavridi et al.
 D353,195 S 12/1994 Savage et al.
 D353,196 S 12/1994 Savage et al.
 5,377,676 A 1/1995 Vari et al.
 5,385,144 A 1/1995 Yamanishi et al.
 5,396,893 A 3/1995 Oberg et al.
 D359,546 S 6/1995 Savage et al.
 5,431,170 A 7/1995 Mathews
 D361,840 S 8/1995 Savage et al.
 D362,063 S 9/1995 Savage et al.
 5,448,991 A 9/1995 Polson et al.
 5,448,999 A 9/1995 Teare et al.
 5,452,717 A 9/1995 Branigan et al.
 D363,120 S 10/1995 Savage et al.
 5,456,252 A 10/1995 Vari et al.
 5,479,934 A 1/1996 Imran
 5,482,036 A 1/1996 Diab et al.
 5,490,505 A 2/1996 Diab et al.
 5,494,043 A 2/1996 O'Sullivan et al.
 5,533,511 A 7/1996 Kaspari et al.
 5,534,851 A 7/1996 Russek
 5,542,421 A 8/1996 Erdman
 5,561,275 A 10/1996 Savage et al.
 5,562,002 A 10/1996 Lalin

5,575,284 A 11/1996 Athan et al.
 5,590,649 A 1/1997 Caro et al.
 5,602,924 A 2/1997 Durand et al.
 5,632,272 A 5/1997 Diab et al.
 5,638,816 A 6/1997 Kiani-Azarbayjany et al.
 5,638,818 A 6/1997 Diab et al.
 5,645,440 A 7/1997 Tobler et al.
 5,647,359 A 7/1997 Kohno et al.
 5,682,877 A 11/1997 Mondry
 5,685,299 A 11/1997 Diab et al.
 5,715,816 A 2/1998 Mainiero et al.
 D393,830 S 4/1998 Tobler et al.
 5,743,261 A 4/1998 Mainiero et al.
 5,743,262 A 4/1998 Lepper, Jr. et al.
 5,743,857 A 4/1998 Shinoda et al.
 5,758,644 A 6/1998 Diab et al.
 5,760,910 A 6/1998 Lepper, Jr. et al.
 5,769,785 A 6/1998 Diab et al.
 5,782,757 A 7/1998 Diab et al.
 5,785,659 A 7/1998 Caro et al.
 5,791,347 A 8/1998 Flaherty et al.
 5,810,734 A 9/1998 Caro et al.
 5,823,950 A 10/1998 Diab et al.
 5,827,181 A 10/1998 Dias et al.
 5,827,196 A 10/1998 Yeo et al.
 5,830,131 A 11/1998 Caro et al.
 5,830,135 A * 11/1998 Bosque et al. 600/323
 5,833,618 A 11/1998 Caro et al.
 5,846,190 A 12/1998 Woehrle
 5,860,919 A 1/1999 Kiani-Azarbayjany et al.
 5,876,335 A 3/1999 Handy et al.
 5,890,929 A 4/1999 Mills et al.
 5,904,654 A 5/1999 Wohltmann et al.
 5,919,134 A 7/1999 Diab
 5,934,925 A 8/1999 Tobler et al.
 5,940,182 A 8/1999 Lepper, Jr. et al.
 5,954,053 A 9/1999 Chance et al.
 5,995,855 A 11/1999 Kiani et al.
 5,997,343 A 12/1999 Mills et al.
 6,002,952 A 12/1999 Diab et al.
 6,011,986 A 1/2000 Diab et al.
 6,027,452 A 2/2000 Flaherty et al.
 6,036,642 A 3/2000 Diab et al.
 6,045,509 A 4/2000 Caro et al.
 6,067,462 A 5/2000 Diab et al.
 6,081,735 A 6/2000 Diab et al.
 6,083,172 A 7/2000 Baker, Jr. et al.
 6,088,607 A 7/2000 Diab et al.
 6,094,592 A 7/2000 Yorkey et al.
 6,110,522 A 8/2000 Lepper, Jr. et al.
 6,122,535 A 9/2000 Kaestle et al.
 6,124,597 A 9/2000 Shehada
 6,128,521 A 10/2000 Marro et al.
 6,129,675 A 10/2000 Jay
 6,144,868 A 11/2000 Parker
 6,151,516 A 11/2000 Kiani-Azarbayjany et al.
 6,152,754 A 11/2000 Gerhardt et al.
 6,157,850 A 12/2000 Diab et al.
 6,165,005 A 12/2000 Mills et al.
 6,184,521 B1 2/2001 Coffin, IV et al.
 6,206,830 B1 3/2001 Diab et al.
 6,229,856 B1 5/2001 Diab et al.
 6,232,609 B1 5/2001 Snyder et al.
 6,236,872 B1 5/2001 Diab et al.
 6,241,683 B1 6/2001 Macklem et al.
 6,253,097 B1 6/2001 Aronow et al.
 6,256,523 B1 7/2001 Diab et al.
 6,263,222 B1 7/2001 Diab et al.
 6,278,522 B1 8/2001 Lepper, Jr. et al.
 6,280,213 B1 8/2001 Tobler et al.
 6,285,896 B1 9/2001 Tobler et al.
 6,301,493 B1 10/2001 Marro et al.
 6,317,627 B1 11/2001 Ennen et al.
 6,321,100 B1 11/2001 Parker
 6,325,761 B1 12/2001 Jay
 6,334,065 B1 12/2001 Al-Ali et al.
 6,343,224 B1 1/2002 Parker
 6,349,228 B1 2/2002 Kiani et al.
 6,360,114 B1 3/2002 Diab et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,368,283	B1	4/2002	Xu et al.	7,003,338	B2	2/2006	Weber et al.
6,371,921	B1	4/2002	Caro et al.	7,003,339	B2	2/2006	Diab et al.
6,377,829	B1	4/2002	Al-Ali	7,015,451	B2	3/2006	Dalke et al.
6,388,240	B2	5/2002	Schulz et al.	7,024,233	B2	4/2006	Ali et al.
6,397,091	B2	5/2002	Diab et al.	7,027,849	B2	4/2006	Al-Ali
6,430,437	B1	8/2002	Marro	7,030,749	B2	4/2006	Al-Ali
6,430,525	B1	8/2002	Weber et al.	7,039,449	B2	5/2006	Al-Ali
6,463,311	B1	10/2002	Diab	7,041,060	B2	5/2006	Flaherty et al.
6,470,199	B1	10/2002	Kopotic et al.	7,044,918	B2	5/2006	Diab
6,501,975	B2	12/2002	Diab et al.	7,067,893	B2	6/2006	Mills et al.
6,505,059	B1	1/2003	Kollias et al.	7,096,052	B2	8/2006	Mason et al.
6,515,273	B2	2/2003	Al-Ali	7,096,054	B2	8/2006	Abdul-Hafiz et al.
6,519,487	B1	2/2003	Parker	7,132,641	B2	11/2006	Schulz et al.
6,525,386	B1	2/2003	Mills et al.	7,142,901	B2	11/2006	Kiani et al.
6,526,300	B1	2/2003	Kiani et al.	7,149,561	B2	12/2006	Diab
6,541,756	B2	4/2003	Schulz et al.	7,186,966	B2	3/2007	Al-Ali
6,542,764	B1	4/2003	Al-Ali et al.	7,190,261	B2	3/2007	Al-Ali
6,580,086	B1	6/2003	Schulz et al.	7,215,984	B2	5/2007	Diab
6,584,336	B1	6/2003	Ali et al.	7,215,986	B2	5/2007	Diab
6,595,316	B2	7/2003	Cybulski et al.	7,221,971	B2	5/2007	Diab
6,597,932	B2	7/2003	Tian et al.	7,225,006	B2	5/2007	Al-Ali et al.
6,597,933	B2	7/2003	Kiani et al.	7,225,007	B2	5/2007	Al-Ali
6,606,511	B1	8/2003	Ali et al.	RE39,672	E	6/2007	Shehada et al.
6,632,181	B2	10/2003	Flaherty et al.	7,239,905	B2	7/2007	Kiani-Azarbayjany et al.
6,639,668	B1	10/2003	Trepagnier	7,245,953	B1	7/2007	Parker
6,640,116	B2	10/2003	Diab	7,254,429	B2	8/2007	Schurman et al.
6,643,530	B2	11/2003	Diab et al.	7,254,431	B2	8/2007	Al-Ali et al.
6,650,917	B2	11/2003	Diab et al.	7,254,433	B2	8/2007	Diab et al.
6,654,624	B2	11/2003	Diab et al.	7,254,434	B2	8/2007	Schulz et al.
6,658,276	B2	12/2003	Kianl et al.	7,272,425	B2	9/2007	Al-Ali
6,661,161	B1	12/2003	Lanzo et al.	7,274,955	B2	9/2007	Kiani et al.
6,671,531	B2	12/2003	Al-Ali et al.	D554,263	S	10/2007	Al-Ali et al.
6,678,543	B2	1/2004	Diab et al.	7,280,858	B2	10/2007	Al-Ali et al.
6,684,090	B2	1/2004	Ali et al.	7,289,835	B2	10/2007	Mansfield et al.
6,684,091	B2	1/2004	Parker	7,292,883	B2	11/2007	De Felice et al.
6,697,656	B1	2/2004	Al-Ali	7,295,866	B2	11/2007	Al-Ali
6,697,657	B1	2/2004	Shehada et al.	7,328,053	B1	2/2008	Diab et al.
6,697,658	B2	2/2004	Al-Ali	7,332,784	B2	2/2008	Mills et al.
RE38,476	E	3/2004	Diab et al.	7,340,287	B2	3/2008	Mason et al.
6,699,194	B1	3/2004	Diab et al.	7,341,559	B2	3/2008	Schulz et al.
6,714,804	B2	3/2004	Al-Ali et al.	7,343,186	B2	3/2008	Lamego et al.
RE38,492	E	4/2004	Diab et al.	D566,282	S	4/2008	Al-Ali et al.
6,721,582	B2	4/2004	Trepagnier et al.	7,355,512	B1	4/2008	Al-Ali
6,721,585	B1	4/2004	Parker	7,356,365	B2	4/2008	Schurman
6,725,075	B2	4/2004	Al-Ali	7,371,981	B2	5/2008	Abdul-Hafiz
6,728,560	B2	4/2004	Kollias et al.	7,373,193	B2	5/2008	Al-Ali et al.
6,735,459	B2	5/2004	Parker	7,373,194	B2	5/2008	Weber et al.
6,745,060	B2	6/2004	Diab et al.	7,376,453	B1	5/2008	Diab et al.
6,760,607	B2	7/2004	Al-Ali	7,377,794	B2	5/2008	Al-Ali et al.
6,770,028	B1	8/2004	Ali et al.	7,377,899	B2	5/2008	Weber et al.
6,771,994	B2	8/2004	Kiani et al.	7,383,070	B2	6/2008	Diab et al.
6,792,300	B1	9/2004	Diab et al.	7,415,297	B2	8/2008	Al-Ali et al.
6,813,511	B2	11/2004	Diab et al.	7,428,432	B2	9/2008	Ali et al.
6,816,741	B2	11/2004	Diab	7,438,683	B2	10/2008	Al-Ali et al.
6,822,564	B2	11/2004	Al-Ali	7,440,787	B2	10/2008	Diab
6,826,419	B2	11/2004	Diab et al.	7,454,240	B2	11/2008	Diab et al.
6,830,711	B2	12/2004	Mills et al.	7,467,002	B2	12/2008	Weber et al.
6,850,787	B2	2/2005	Weber et al.	7,469,157	B2	12/2008	Diab et al.
6,850,788	B2	2/2005	Al-Ali	7,471,969	B2	12/2008	Diab et al.
6,852,083	B2	2/2005	Caro et al.	7,471,971	B2	12/2008	Diab et al.
6,861,639	B2	3/2005	Al-Ali	7,483,729	B2	1/2009	Al-Ali et al.
6,898,452	B2	5/2005	Al-Ali et al.	7,483,730	B2	1/2009	Diab et al.
6,920,345	B2	7/2005	Al-Ali et al.	7,489,958	B2	2/2009	Diab et al.
6,931,268	B1	8/2005	Kiani-Azarbayjany et al.	7,496,391	B2	2/2009	Diab et al.
6,934,570	B2	8/2005	Kiani et al.	7,496,393	B2	2/2009	Diab et al.
6,939,305	B2	9/2005	Flaherty et al.	D587,657	S	3/2009	Al-Ali et al.
6,943,348	B1	9/2005	Coffin, IV	7,499,741	B2	3/2009	Diab et al.
6,950,687	B2	9/2005	Al-Ali	7,499,835	B2	3/2009	Weber et al.
6,961,598	B2	11/2005	Diab	7,500,950	B2	3/2009	Al-Ali et al.
6,970,792	B1	11/2005	Diab	7,509,154	B2	3/2009	Diab et al.
6,979,812	B2	12/2005	Al-Ali	7,509,494	B2	3/2009	Al-Ali
6,985,764	B2	1/2006	Mason et al.	7,510,849	B2	3/2009	Schurman et al.
6,993,371	B2	1/2006	Kiani et al.	7,526,328	B2	4/2009	Diab et al.
6,996,427	B2	2/2006	Ali et al.	7,530,942	B1	5/2009	Diab
6,999,904	B2	2/2006	Weber et al.	7,530,949	B2	5/2009	Al Ali et al.
				7,530,955	B2	5/2009	Diab et al.
				7,563,110	B2	7/2009	Al-Ali et al.
				7,596,398	B2	9/2009	Al-Ali et al.
				7,618,375	B2	11/2009	Flaherty

(56)

References Cited

U.S. PATENT DOCUMENTS

D606,659 S	12/2009	Kiani et al.	8,229,533 B2	7/2012	Diab et al.
7,647,083 B2	1/2010	Al-Ali et al.	8,233,955 B2	7/2012	Al-Ali et al.
D609,193 S	2/2010	Al-Ali et al.	8,244,325 B2	8/2012	Al-Ali et al.
D614,305 S	4/2010	Al-Ali et al.	8,255,026 B1	8/2012	Al-Ali
RE41,317 E	5/2010	Parker	8,255,027 B2	8/2012	Al-Ali et al.
7,729,733 B2	6/2010	Al-Ali et al.	8,255,028 B2	8/2012	Al-Ali et al.
7,734,320 B2	6/2010	Al-Ali	8,260,577 B2	9/2012	Weber et al.
7,761,127 B2	7/2010	Al-Ali et al.	8,265,723 B1	9/2012	McHale et al.
7,761,128 B2	7/2010	Al-Ali et al.	8,274,360 B2	9/2012	Sampath et al.
7,764,982 B2	7/2010	Dalke et al.	8,301,217 B2	10/2012	Al-Ali et al.
D621,516 S	8/2010	Kiani et al.	8,306,596 B2	11/2012	Schurman et al.
7,791,155 B2	9/2010	Diab	8,310,336 B2	11/2012	Muhsin et al.
7,801,581 B2	9/2010	Diab	8,315,683 B2	11/2012	Al-Ali et al.
7,822,452 B2	10/2010	Schurman et al.	RE43,860 E	12/2012	Parker
RE41,912 E	11/2010	Parker	8,337,403 B2	12/2012	Al-Ali et al.
7,844,313 B2	11/2010	Kiani et al.	8,346,330 B2	1/2013	Lamego
7,844,314 B2	11/2010	Al-Ali	8,353,842 B2	1/2013	Al-Ali et al.
7,844,315 B2	11/2010	Al-Ali	8,355,766 B2	1/2013	MacNeish, III et al.
7,865,222 B2	1/2011	Weber et al.	8,359,080 B2	1/2013	Diab et al.
7,873,497 B2	1/2011	Weber et al.	8,364,223 B2	1/2013	Al-Ali et al.
7,880,606 B2	2/2011	Al-Ali	8,364,226 B2	1/2013	Diab et al.
7,880,626 B2	2/2011	Al-Ali et al.	8,374,665 B2	2/2013	Lamego
7,891,355 B2	2/2011	Al-Ali et al.	8,385,995 B2	2/2013	Al-Ali et al.
7,894,868 B2	2/2011	Al-Ali et al.	8,385,996 B2	2/2013	Smith et al.
7,899,507 B2	3/2011	Al-Ali et al.	8,388,353 B2	3/2013	Kiani et al.
7,899,518 B2	3/2011	Trepagnier et al.	8,399,822 B2	3/2013	Al-Ali
7,904,132 B2	3/2011	Weber et al.	8,401,602 B2	3/2013	Kiani
7,909,772 B2	3/2011	Popov et al.	8,405,608 B2	3/2013	Al-Ali et al.
7,910,875 B2	3/2011	Al-Ali	8,414,499 B2	4/2013	Al-Ali et al.
7,919,713 B2	4/2011	Al-Ali et al.	8,418,524 B2	4/2013	Al-Ali
7,937,128 B2	5/2011	Al-Ali	8,423,106 B2	4/2013	Lamego et al.
7,937,129 B2	5/2011	Mason et al.	8,428,967 B2	4/2013	Olsen et al.
7,937,130 B2	5/2011	Diab et al.	8,430,817 B1	4/2013	Al-Ali et al.
7,941,199 B2	5/2011	Kiani	8,437,825 B2	5/2013	Dalvi et al.
7,942,824 B1	5/2011	Kayyali et al.	8,455,290 B2	6/2013	Siskavich
7,951,086 B2	5/2011	Flaherty et al.	8,457,703 B2	6/2013	Al-Ali
7,957,780 B2	6/2011	Lamego et al.	8,457,707 B2	6/2013	Kiani
7,962,188 B2	6/2011	Kiani et al.	8,463,349 B2	6/2013	Diab et al.
7,962,190 B1	6/2011	Diab et al.	8,466,286 B2	6/2013	Bellott et al.
7,976,472 B2	7/2011	Kiani	8,471,713 B2	6/2013	Poeze et al.
7,988,637 B2	8/2011	Diab	8,473,020 B2	6/2013	Kiani et al.
7,990,382 B2	8/2011	Kiani	8,483,787 B2	7/2013	Al-Ali et al.
7,991,446 B2	8/2011	Ali et al.	8,489,364 B2	7/2013	Weber et al.
8,000,761 B2	8/2011	Al-Ali	8,498,684 B2	7/2013	Weber et al.
8,008,088 B2	8/2011	Bellott et al.	8,504,128 B2	8/2013	Blank et al.
RE42,753 E	9/2011	Kiani-Azarbayjany et al.	8,509,867 B2	8/2013	Workman et al.
8,019,400 B2	9/2011	Diab et al.	8,515,509 B2	8/2013	Bruinsma et al.
8,028,701 B2	10/2011	Al-Ali et al.	8,523,781 B2	9/2013	Al-Ali
8,029,765 B2	10/2011	Bellott et al.	8,529,301 B2	9/2013	Al-Ali et al.
8,036,727 B2	10/2011	Schurman et al.	8,532,727 B2	9/2013	Ali et al.
8,036,728 B2	10/2011	Diab et al.	8,532,728 B2	9/2013	Diab et al.
8,046,040 B2	10/2011	Ali et al.	D692,145 S	10/2013	Al-Ali et al.
8,046,041 B2	10/2011	Diab et al.	8,547,209 B2	10/2013	Kiani et al.
8,046,042 B2	10/2011	Diab et al.	8,548,548 B2	10/2013	Al-Ali
8,048,040 B2	11/2011	Kiani	8,548,549 B2	10/2013	Schurman et al.
8,050,728 B2	11/2011	Al-Ali et al.	8,548,550 B2	10/2013	Al-Ali et al.
RE43,169 E	2/2012	Parker	8,560,032 B2	10/2013	Al-Ali et al.
8,118,620 B2	2/2012	Al-Ali et al.	8,560,034 B1	10/2013	Diab et al.
8,126,528 B2	2/2012	Diab et al.	8,570,167 B2	10/2013	Al-Ali
8,128,572 B2	3/2012	Diab et al.	8,570,503 B2	10/2013	Vo et al.
8,130,105 B2	3/2012	Al-Ali et al.	8,571,617 B2	10/2013	Reichgott et al.
8,145,287 B2	3/2012	Diab et al.	8,571,618 B1	10/2013	Lamego et al.
8,150,487 B2	4/2012	Diab et al.	8,571,619 B2	10/2013	Al-Ali et al.
8,175,672 B2	5/2012	Parker	8,577,431 B2	11/2013	Lamego et al.
8,180,420 B2	5/2012	Diab et al.	8,584,345 B2	11/2013	Al-Ali et al.
8,182,443 B1	5/2012	Kiani	8,588,880 B2	11/2013	Abdul-Hafiz et al.
8,185,180 B2	5/2012	Diab et al.	8,600,467 B2	12/2013	Al-Ali et al.
8,190,223 B2	5/2012	Al-Ali et al.	8,606,342 B2	12/2013	Diab
8,190,227 B2	5/2012	Diab et al.	8,626,255 B2	1/2014	Al-Ali et al.
8,203,438 B2	6/2012	Kiani et al.	8,630,691 B2	1/2014	Lamego et al.
8,203,704 B2	6/2012	Merritt et al.	8,634,889 B2	1/2014	Al-Ali et al.
8,204,566 B2	6/2012	Schurman et al.	8,641,631 B2	2/2014	Sierra et al.
8,219,172 B2	7/2012	Schurman et al.	8,652,060 B2	2/2014	Al-Ali
8,224,411 B2	7/2012	Al-Ali et al.	8,663,107 B2	3/2014	Kiani
8,228,181 B2	7/2012	Al-Ali	8,666,468 B1	3/2014	Al-Ali
			8,667,967 B2	3/2014	Al-Ali et al.
			8,670,811 B2	3/2014	O'Reilly
			8,670,814 B2	3/2014	Diab et al.
			8,676,286 B2	3/2014	Weber et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

8,682,407 B2	3/2014	Al-Ali	2011/0208015 A1	8/2011	Welch et al.
RE44,823 E	4/2014	Parker	2011/0209915 A1	9/2011	Telfort et al.
RE44,875 E	4/2014	Kiani et al.	2011/0213212 A1	9/2011	Al-Ali
8,690,799 B2	4/2014	Telfort et al.	2011/0230733 A1	9/2011	Al-Ali
8,700,112 B2	4/2014	Kiani	2011/0237911 A1	9/2011	Lamego et al.
8,702,627 B2	4/2014	Telfort et al.	2012/0059267 A1	3/2012	Lamego et al.
8,706,179 B2	4/2014	Parker	2012/0116175 A1	5/2012	Al-Ali et al.
8,712,494 B1	4/2014	MacNeish, III et al.	2012/0179006 A1	7/2012	Jansen et al.
8,715,206 B2	5/2014	Telfort et al.	2012/0209082 A1	8/2012	Al-Ali
8,718,735 B2	5/2014	Lamego et al.	2012/0209084 A1	8/2012	Olsen et al.
8,718,737 B2	5/2014	Diab et al.	2012/0227739 A1	9/2012	Kiani
8,718,738 B2	5/2014	Blank et al.	2012/0265039 A1	10/2012	Kiani
8,720,249 B2	5/2014	Al-Ali	2012/0283524 A1	11/2012	Kiani et al.
8,721,541 B2	5/2014	Al-Ali et al.	2012/0286955 A1	11/2012	Welch et al.
8,721,542 B2	5/2014	Al-Ali et al.	2012/0296178 A1	11/2012	Lamego et al.
8,723,677 B1	5/2014	Kiani	2012/0319816 A1	12/2012	Al-Ali
8,740,792 B1	6/2014	Kiani et al.	2012/0330112 A1	12/2012	Lamego et al.
8,754,776 B2	6/2014	Poeze et al.	2013/0023775 A1	1/2013	Lamego et al.
8,755,535 B2	6/2014	Telfort et al.	2013/0041591 A1	2/2013	Lamego
8,755,856 B2	6/2014	Diab et al.	2013/0045685 A1	2/2013	Kiani
8,755,872 B1	6/2014	Marinow	2013/0046204 A1	2/2013	Lamego et al.
8,761,850 B2	6/2014	Lamego	2013/0060108 A1	3/2013	Schurman et al.
8,764,671 B2	7/2014	Kiani	2013/0060147 A1	3/2013	Welch et al.
8,768,423 B2	7/2014	Shakespeare et al.	2013/0096405 A1	4/2013	Garfio
8,771,204 B2	7/2014	Telfort et al.	2013/0096936 A1	4/2013	Sampath et al.
8,777,634 B2	7/2014	Kiani et al.	2013/0109935 A1	5/2013	Al-Ali et al.
8,781,543 B2	7/2014	Diab et al.	2013/0162433 A1	6/2013	Muhsin et al.
8,781,544 B2	7/2014	Al-Ali et al.	2013/0190581 A1	7/2013	Al-Ali et al.
8,781,549 B2	7/2014	Al-Ali et al.	2013/0197328 A1	8/2013	Diab et al.
8,788,003 B2	7/2014	Schurman et al.	2013/0211214 A1	8/2013	Olsen
8,790,268 B2	7/2014	Al-Ali	2013/0243021 A1	9/2013	Siskavich
8,801,613 B2	8/2014	Al-Ali et al.	2013/0253334 A1	9/2013	Al-Ali et al.
8,821,397 B2	9/2014	Al-Ali et al.	2013/0274571 A1	10/2013	Diab et al.
8,821,415 B2	9/2014	Al-Ali et al.	2013/0296672 A1	11/2013	O'Neil et al.
8,830,449 B1	9/2014	Lamego et al.	2013/0317370 A1	11/2013	Dalvi et al.
8,831,700 B2	9/2014	Schurman et al.	2013/0324808 A1	12/2013	Al-Ali et al.
8,840,549 B2	9/2014	Al-Ali et al.	2013/0331670 A1	12/2013	Kiani
8,847,740 B2	9/2014	Kiani et al.	2013/0338461 A1	12/2013	Lamego et al.
8,849,365 B2	9/2014	Smith et al.	2014/0012100 A1	1/2014	Al-Ali et al.
8,852,094 B2	10/2014	Al-Ali et al.	2014/0025306 A1	1/2014	Weber et al.
8,852,994 B2	10/2014	Wojtczuk et al.	2014/0034353 A1	2/2014	Al-Ali et al.
8,868,147 B2	10/2014	Stippick et al.	2014/0051952 A1	2/2014	Reichgott et al.
8,868,150 B2	10/2014	Al-Ali et al.	2014/0051953 A1	2/2014	Lamego et al.
8,870,792 B2	10/2014	Al-Ali et al.	2014/0051954 A1	2/2014	Al-Ali et al.
8,886,271 B2	11/2014	Kiani et al.	2014/0058230 A1	2/2014	Abdul-Hafiz et al.
8,888,539 B2	11/2014	Al-Ali et al.	2014/0066783 A1	3/2014	Kiani et al.
8,888,708 B2	11/2014	Diab et al.	2014/0077956 A1	3/2014	Sampath et al.
8,892,180 B2	11/2014	Weber et al.	2014/0081100 A1	3/2014	Muhsin et al.
8,897,847 B2	11/2014	Al-Ali	2014/0081175 A1	3/2014	Telfort
8,909,310 B2	12/2014	Lamego et al.	2014/0094667 A1	4/2014	Schurman et al.
8,911,377 B2	12/2014	Al-Ali	2014/0100434 A1	4/2014	Diab et al.
8,912,909 B2	12/2014	Al-Ali et al.	2014/0114199 A1	4/2014	Lamego et al.
8,920,317 B2	12/2014	Al-Ali et al.	2014/0120564 A1	5/2014	Workman et al.
8,921,699 B2	12/2014	Al-Ali et al.	2014/0121482 A1	5/2014	Merritt et al.
8,922,382 B2	12/2014	Al-Ali et al.	2014/0121483 A1	5/2014	Kiani
8,929,964 B2	1/2015	Al-Ali et al.	2014/0125495 A1	5/2014	Al-Ali
8,942,777 B2	1/2015	Diab et al.	2014/0127137 A1	5/2014	Bellott et al.
8,948,834 B2	2/2015	Diab et al.	2014/0128696 A1	5/2014	Al-Ali
8,948,835 B2	2/2015	Diab	2014/0128699 A1	5/2014	Al-Ali et al.
8,965,471 B2	2/2015	Lamego	2014/0129702 A1	5/2014	Lamego et al.
8,983,564 B2	3/2015	Al-Ali	2014/0135588 A1	5/2014	Al-Ali et al.
8,989,831 B2	3/2015	Al-Ali et al.	2014/0142401 A1	5/2014	Al-Ali et al.
8,996,085 B2	3/2015	Kiani et al.	2014/0142402 A1	5/2014	Al-Ali et al.
8,998,809 B2	4/2015	Kiani	2014/0163344 A1	6/2014	Al-Ali
2004/0054261 A1	3/2004	Kamatagi et al.	2014/0163402 A1	6/2014	Lamego et al.
2004/0097797 A1	5/2004	Porges et al.	2014/0166076 A1	6/2014	Kiani et al.
2009/0247984 A1	10/2009	Lamego et al.	2014/0171763 A1	6/2014	Diab
2009/0275844 A1	11/2009	Al-Ali	2014/0180038 A1	6/2014	Kiani
2009/0299157 A1	12/2009	Telfort et al.	2014/0180154 A1	6/2014	Sierra et al.
2010/0004518 A1	1/2010	Vo et al.	2014/0194709 A1	7/2014	Al-Ali et al.
2010/0030040 A1	2/2010	Poeze et al.	2014/0194711 A1	7/2014	Al-Ali
2010/0261979 A1	10/2010	Kiani	2014/0194766 A1	7/2014	Al-Ali et al.
2011/0001605 A1	1/2011	Kiani et al.	2014/0200420 A1	7/2014	Al-Ali
2011/0082711 A1	4/2011	Poeze et al.	2014/0200422 A1	7/2014	Weber et al.
2011/0105854 A1	5/2011	Kiani et al.	2014/0206963 A1	7/2014	Al-Ali
			2014/0213864 A1	7/2014	Abdul-Hafiz et al.
			2014/0243627 A1	8/2014	Diab et al.
			2014/0266790 A1	9/2014	Al-Ali et al.
			2014/0275808 A1	9/2014	Poeze et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2014/0275835	A1	9/2014	Lamego et al.
2014/0275871	A1	9/2014	Lamego et al.
2014/0275872	A1	9/2014	Merritt et al.
2014/0275881	A1	9/2014	Lamego et al.
2014/0288400	A1	9/2014	Diab et al.
2014/0296664	A1	10/2014	Bruinsma et al.
2014/0303520	A1	10/2014	Telfort et al.
2014/0309506	A1	10/2014	Lamego et al.
2014/0309559	A1	10/2014	Telfort et al.
2014/0316228	A1	10/2014	Blank et al.
2014/0323825	A1	10/2014	Al-Ali et al.
2014/0330092	A1	11/2014	Al-Ali et al.
2014/0330098	A1	11/2014	Merritt et al.
2014/0330099	A1	11/2014	Al-Ali et al.
2014/0333440	A1	11/2014	Kiani
2014/0336481	A1	11/2014	Shakespeare et al.
2014/0343436	A1	11/2014	Kiani
2015/0018650	A1	1/2015	Al-Ali et al.

FOREIGN PATENT DOCUMENTS

EP	2319398	5/2011
WO	WO 96/12435	5/1996

OTHER PUBLICATIONS

Confidential Declaration of Michelle Armond in Support of Masimo Corporation's Responsive Claim Construction Brief, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Nov. 19, 2010.

Declaration of Perry D. Oldham in Support of Masimo Corporation's Opening Claim Construction Brief, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Oct. 19, 2010.

Declaration of Robert T. Stone in Support of Philips' Responsive Markman Brief, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Nov. 15, 2010.

Dudell, Glode et al., "What Constitutes Adequate Oxygenation?" *Pediatrics*, Jan. 1990, pp. 39-41.

Mallinckrodt inc. v. Masimo Corp., 147 Fed. Appx. 158, 2005 WL 2139867 (Fed. Cir. 2005).

Mallinckrodt inc. v. Masimo Corp., 2004 U.S. Dist. LEXIS 28518 (C.D. Cal. Jul. 12, 2004).

Mallinckrodt inc. v. Masimo Corp., 254 F. Supp.2d 1140 (C.D. Cal. 2003).

Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH, (District of Delaware, Case No. 09-00080(JJF)) Complaint for Patent Infringement dated Feb. 3, 2009, pp. 1-13.

Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH, (District of Delaware, Case No. 09-00080(JJF)) First Amended Complaint for Patent Infringement dated May 12, 2009, pp. 1-16.

Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH, (District of Delaware, Case No. 09-00080(JJF)) Defendants' Answer and Philips Electronics North America Corporation's Counterclaims to Masimo's First Amended Complaint dated Jun. 15, 2009, pp. 1-65.

Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH, (District of Delaware, Case No. 09-00080(JJF)) Masimo's Answer to Philips' Counterclaims dated Jul. 9, 2009, pp. 1-68.

Plaintiff Philips Electronics North America Corporation Answer to Masimo's Counterclaims dated Aug. 3, 2009, pp. 1-23.

Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH, (District of Delaware, Case No. 09-00080(JJF)) Defendants' Answer and Philips Electronics North America Corporation's Amended Counterclaims to Masimo's First Amended Complaint, dated Apr. 21, 2010, pp. 1-62.

Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH, (District of Delaware, Case No. 09-00080(JJF)) Masimo's Answer to Philips' Amended Counterclaims, dated May 10, 2010, pp. 1-76.

Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH, (District of Delaware, Case No. 09-00080(JJF)) Philips Electronics North America Corporation's Answer to Masimo's Amended Counterclaims (D.I. 102) dated May 27, 2010, pp. 1-24.

Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH, (District of Delaware, Case No. 09-00080(JJF)) Philips North America Corporation and Philips Medizin Systeme Böttingen GMBH's Seventh Supplemental Objections and Responses to Masimo Corporation's First Set of Interrogatories (Nos. 1-8) dated Jun. 30, 2010, pp. 1-40 (redacted).

Masimo Corporation's Opening Claim Construction Brief, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Oct. 19, 2010.

Masimo Corporation's Responsive Claim Construction Brief, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Nov. 19, 2010 (Redacted).

Masimo's Technical Tutorial, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Dec. 1, 2010.

Murray, Willie et al., The Peripheral Pulse Wave: Information Overlooked, *Journal of Clinical Monitoring*, vol. 12, pp. 365-377, Sep. 1996.

Neuhof, H. et al., "Simultaneous Continuous Measurement of Arterial and Mixed Venous Partial O₂ Saturation", *The Oxygen Status of Arterial Blood*, Zander, Mertzluft (eds.), pp. 273-278 (Karger, Basel 1991).

Philips' Claim Construction Hearing, Presentaion Materials, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Dec. 1, 2010.

Philips' Opening Markman Brief, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Oct. 19, 2010.

Philips' Responsive Markman Brief, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Nov. 22, 2010.

Report and Recommendation re Claim Construction, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Feb. 18, 2011.

Revised Joint Claim Construction Chart, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Oct. 19, 2010.

Steinke, John M., Comparison of Mie Theory and the Light Scattering of Red Blood Cells, *Applied Optics*, vol. 27, No. 19, Oct. 1, 1998, pp. 4027-4033.

Transcript of Markman Hearing, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Dec. 1, 2010.

(56)

References Cited

OTHER PUBLICATIONS

Vjayakumar, E. et al., "Pulse Oximetry in Infants of <1500 gm Birth Weight on Supplemental Oxygen: A national Survey", *Journal of Perinatology*, vol. 17, No. 5, 1997, pp. 341-345.

White, Katherine, "Completing the Hemodynamic Picture: SV_{ox} ", *Heart & Lung*, May 1985, vol. 14, No. 3.

Wolf, Martin et al., "Continuous Noninvasive Measurement of Cerebral Arterial and Venous Oxygen Saturation at the Bedside in Mechanically Ventilated Neonates", *Critical Care Med*, 1997, vol. 25, No. 9, pp. 1579-1582.


Granelli A.D., Mellander et al., "Screening for duct-dependent congenital heart disease with pulse oximetry: A critical evaluation of strategies to maximize sensitivity", *Acta Paediatrica*, Nov. 2005; 94:1590-1596, http://www.masimo.com/pdf/Granelli_Article.pdf, 1 page downloaded and printed from the World Wide Web.


Hoke, et al., "Oxygen Saturation as a Screening Test for Critical Congenital Heart Disease: A Preliminary Study", *Pediatr Cardiol*, 23(4):403-409, Jul.-Aug. 2002.

Koppel, Robert I et al., "Effective of Pulse Oximetry Screening for Congenital Heart Disease in Asymptomatic Newborns", *Pediatrics*, Mar. 2003, vol. 111, No. 3, 451-455.

PCT International Search Report and Written Opinion, dated Apr. 17, 2013, re: PCT Application No. PCT/US2013/020377, application dated Jan. 4, 2013, in 14 pages.

* cited by examiner

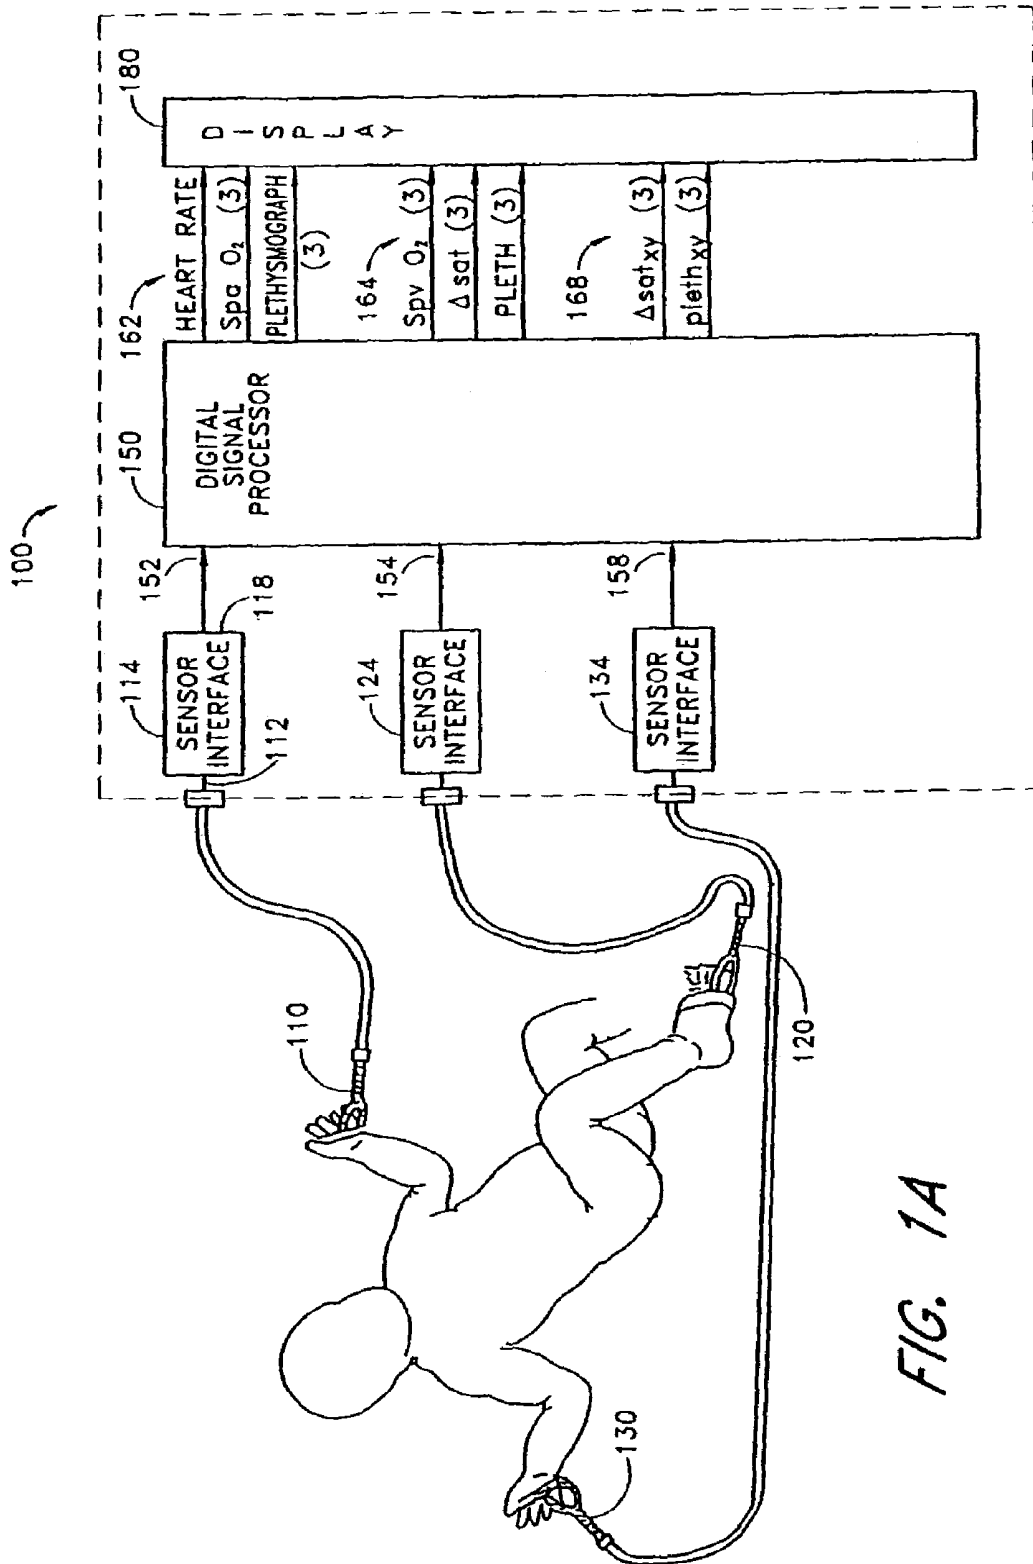

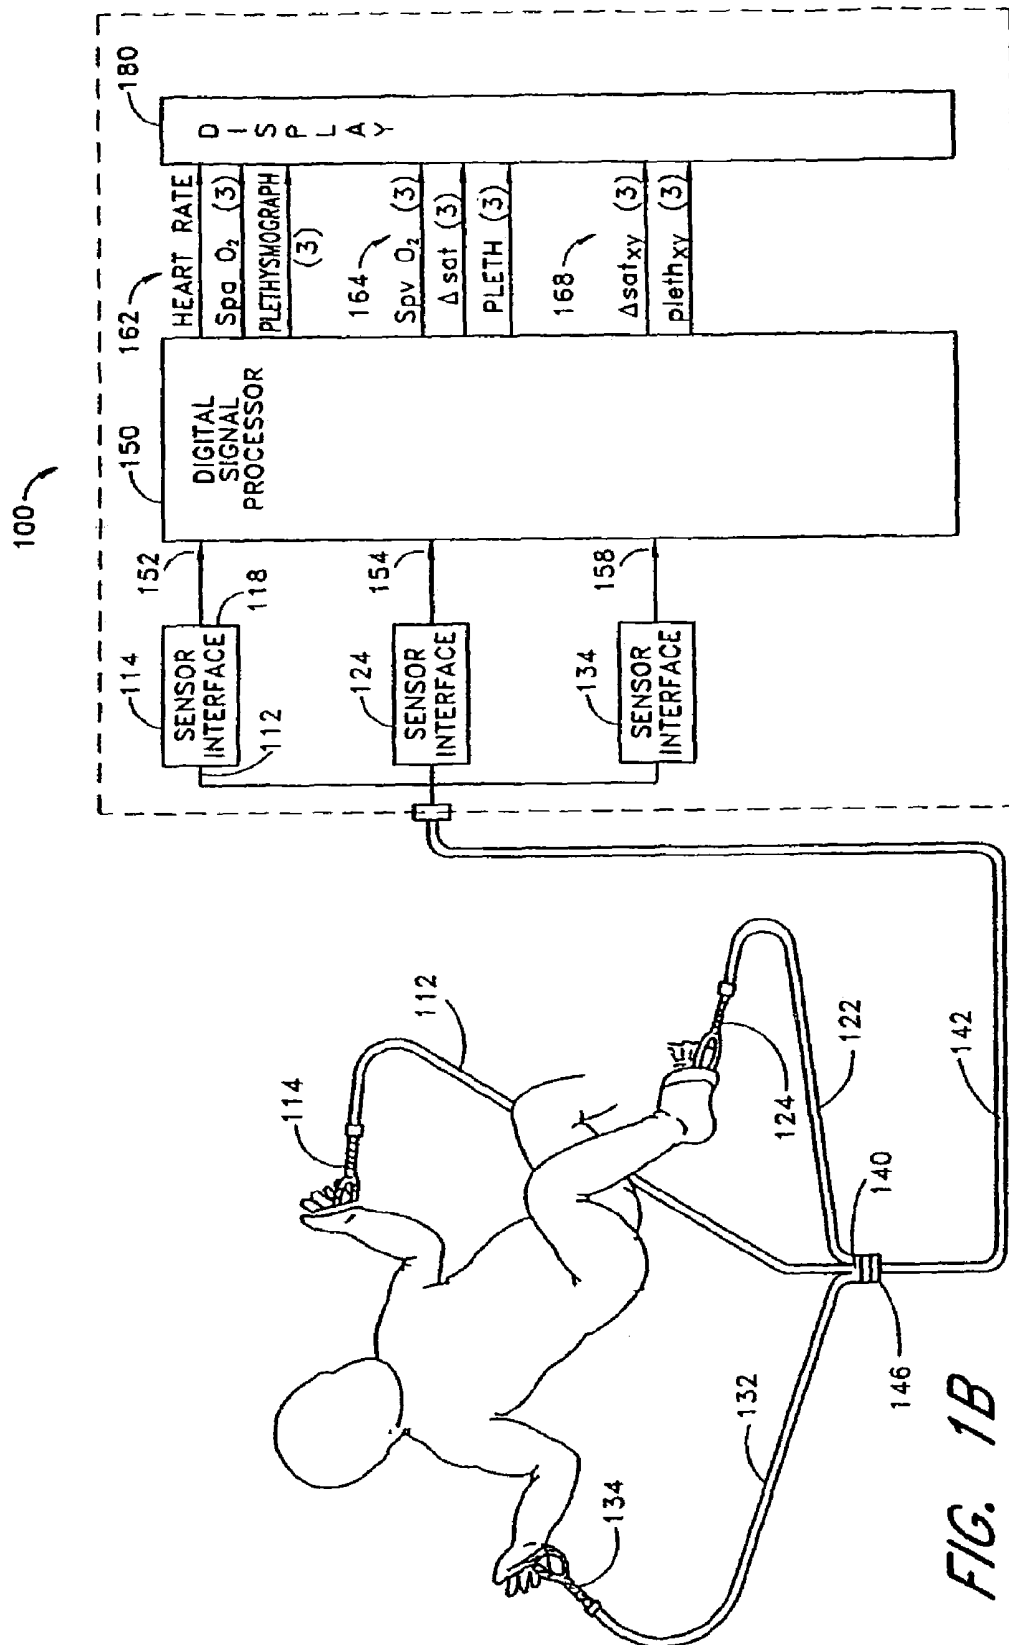

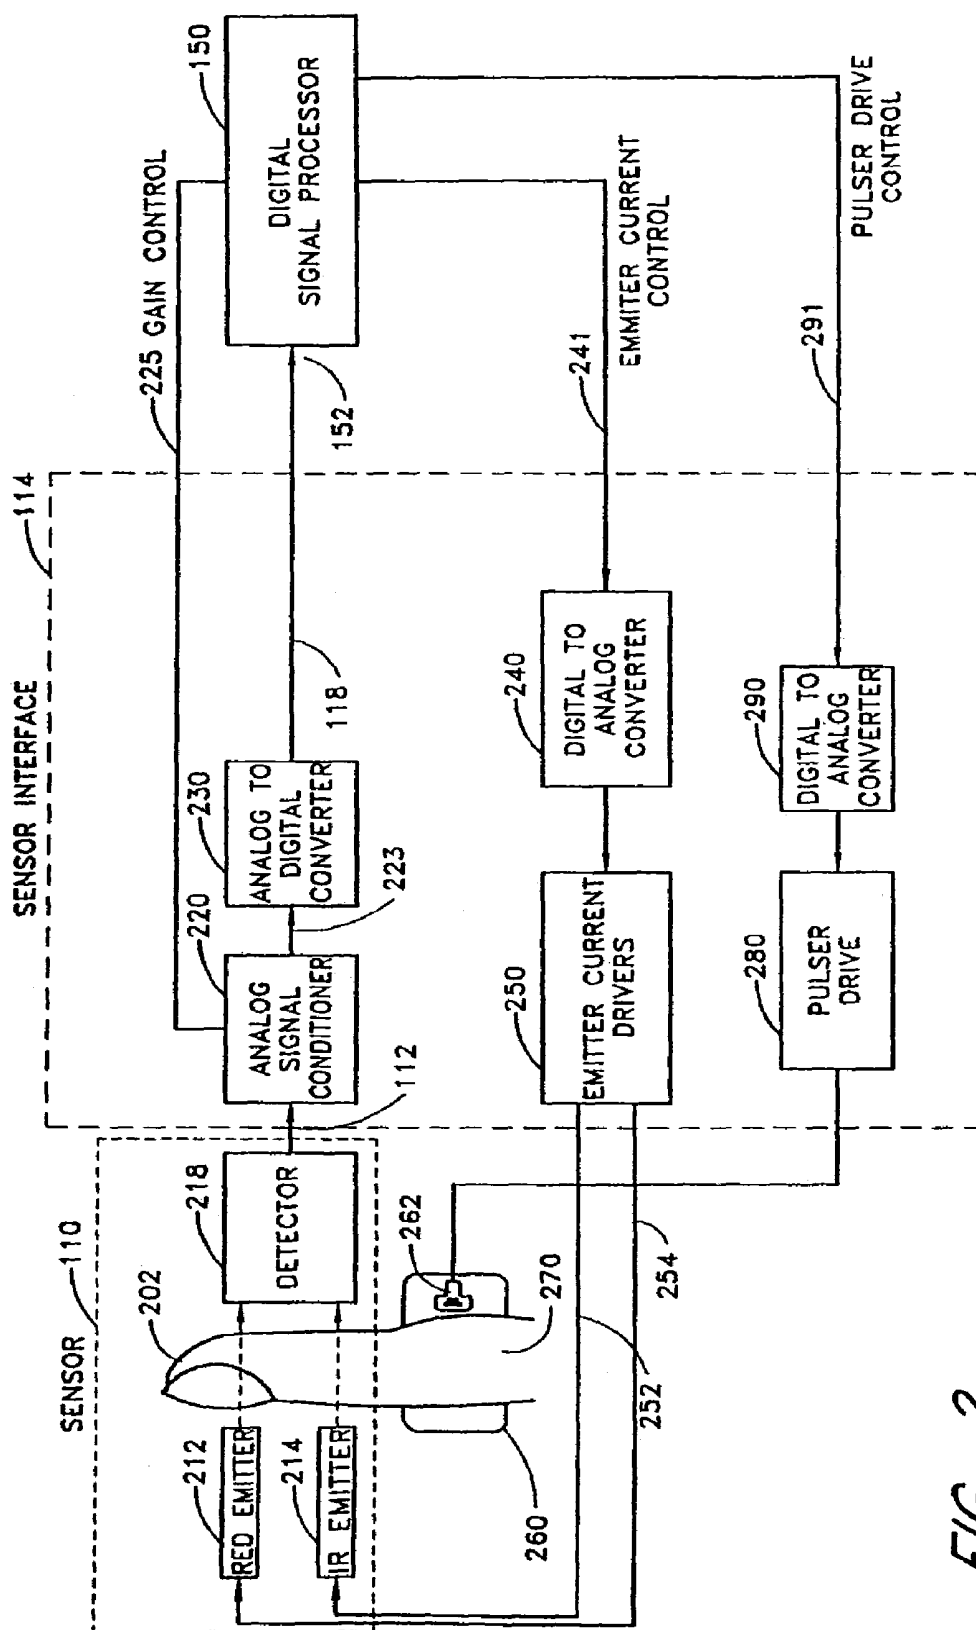


FIG. 2

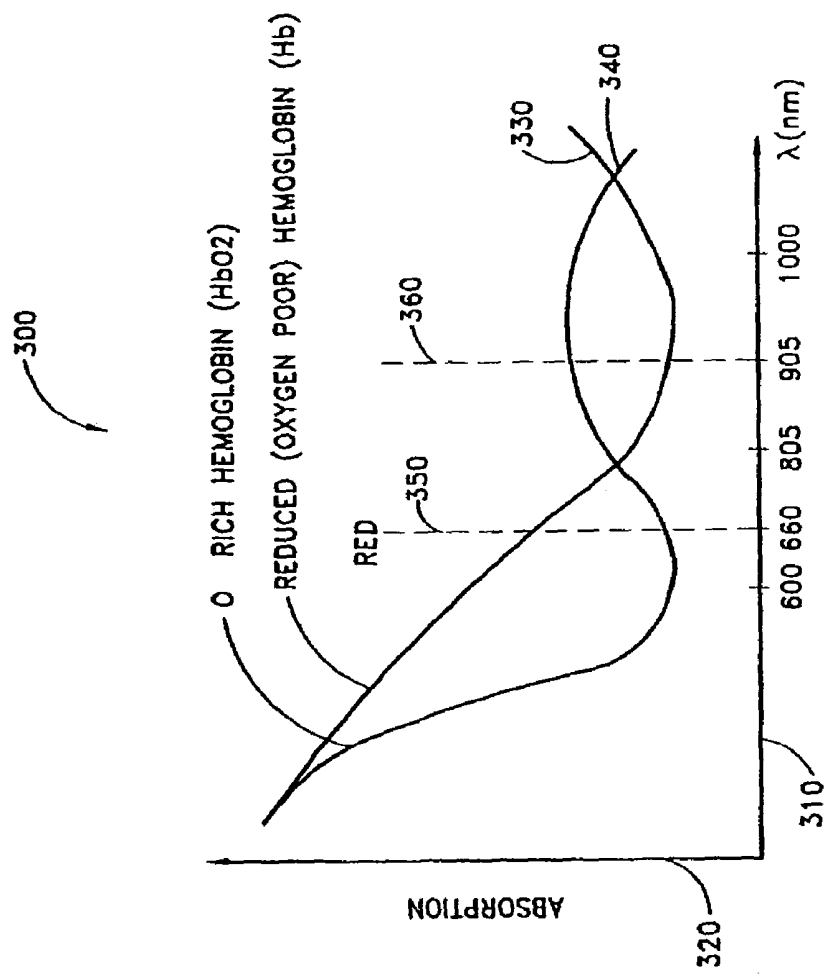


FIG. 3

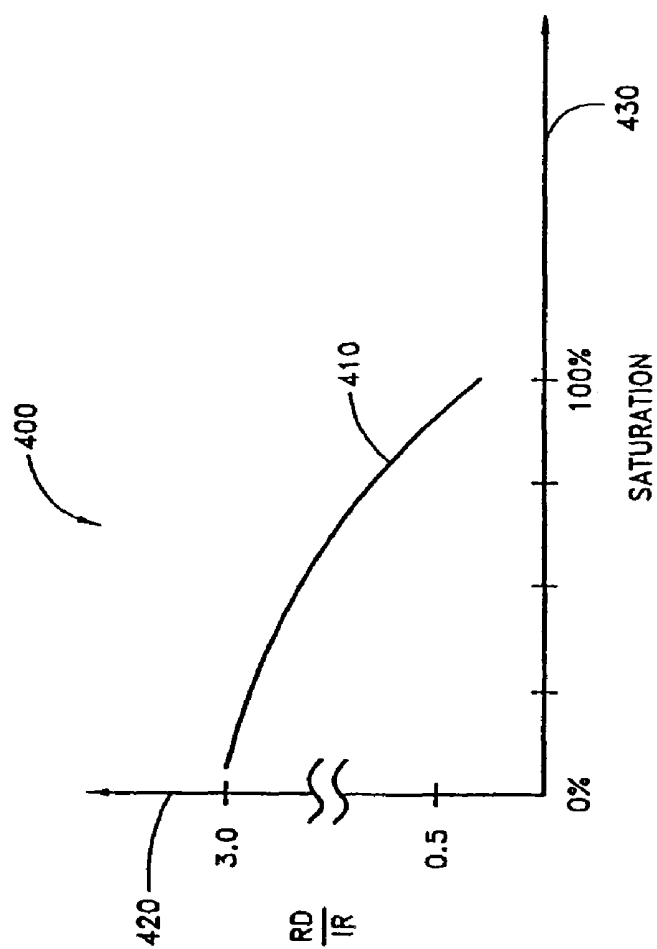


FIG. 4

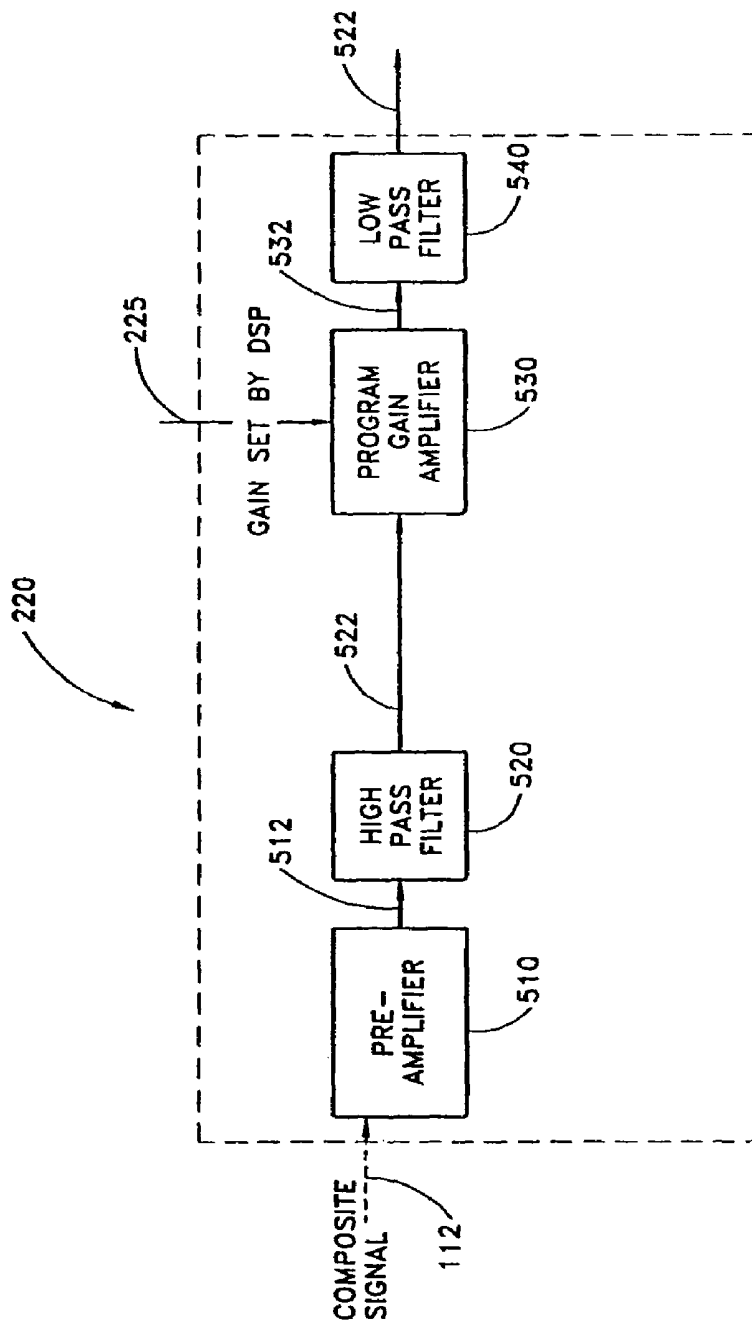


FIG. 5

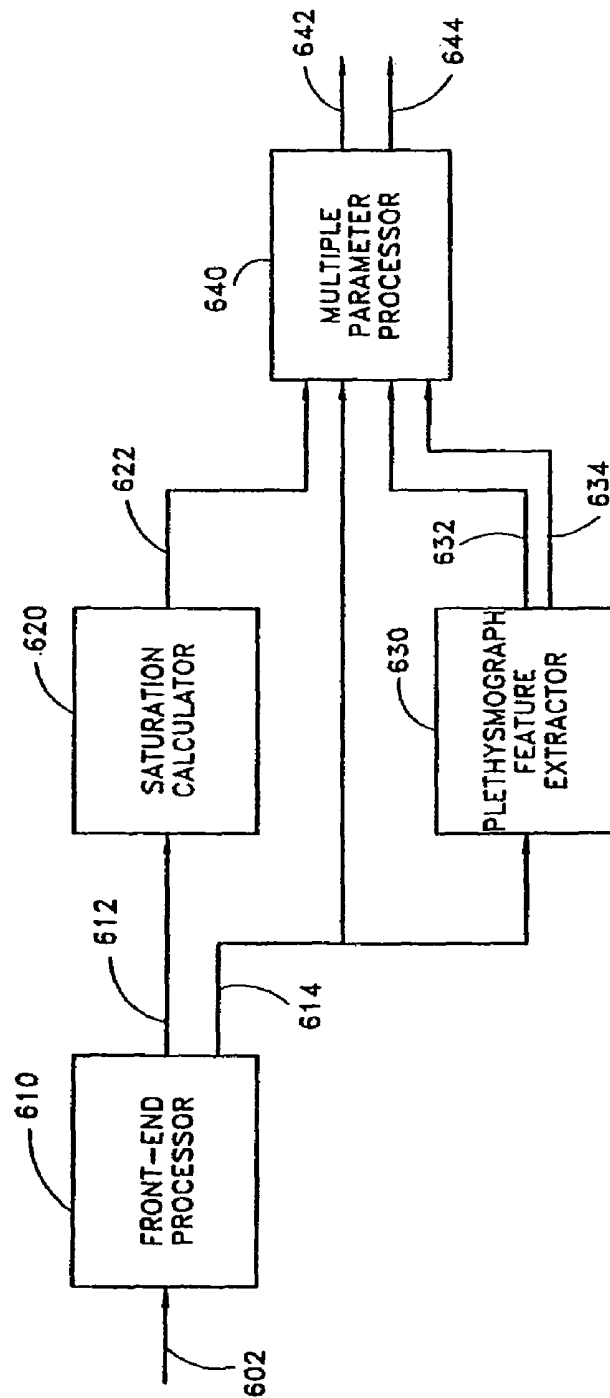


FIG. 6

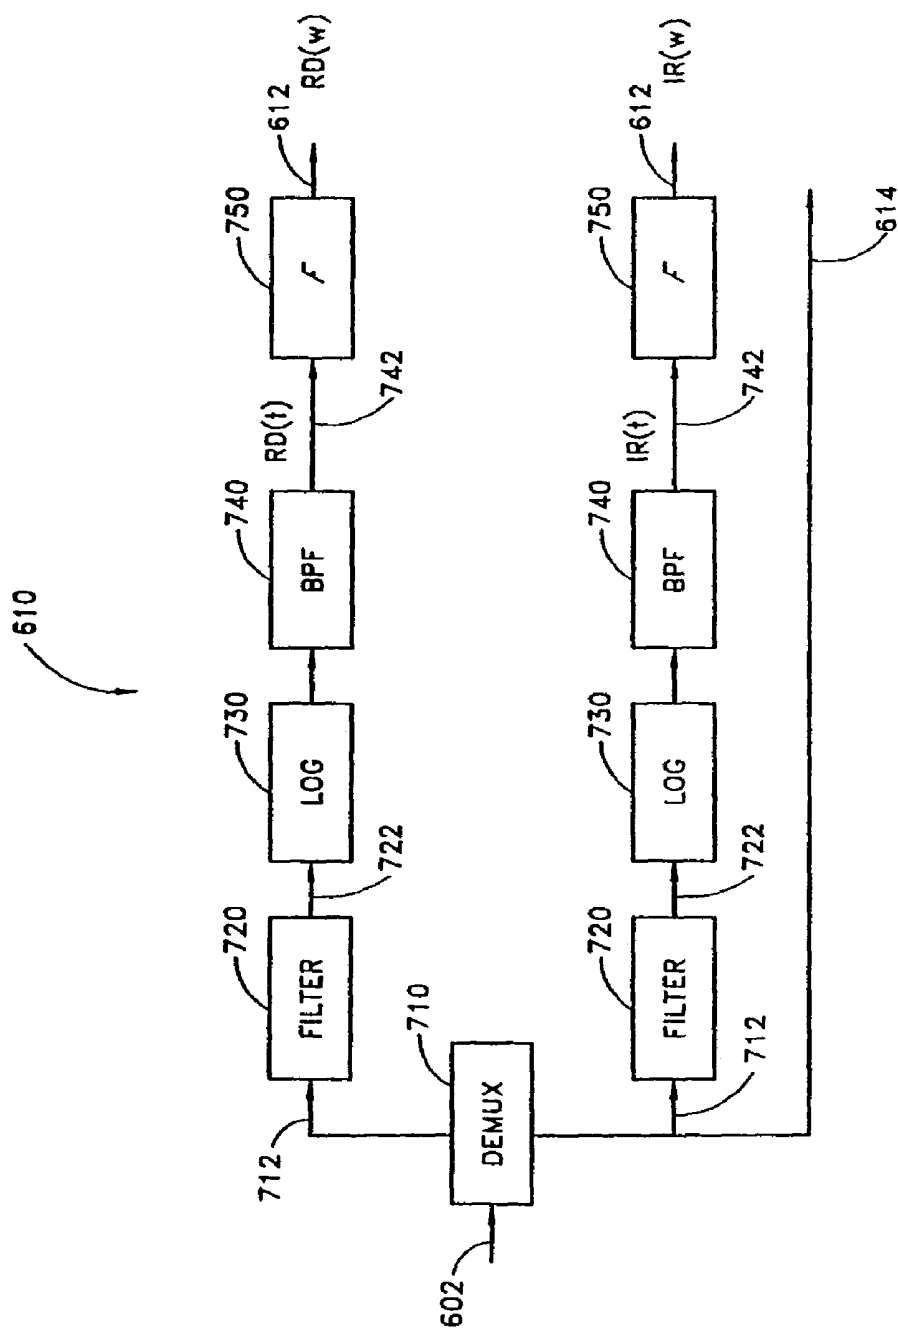


FIG. 7

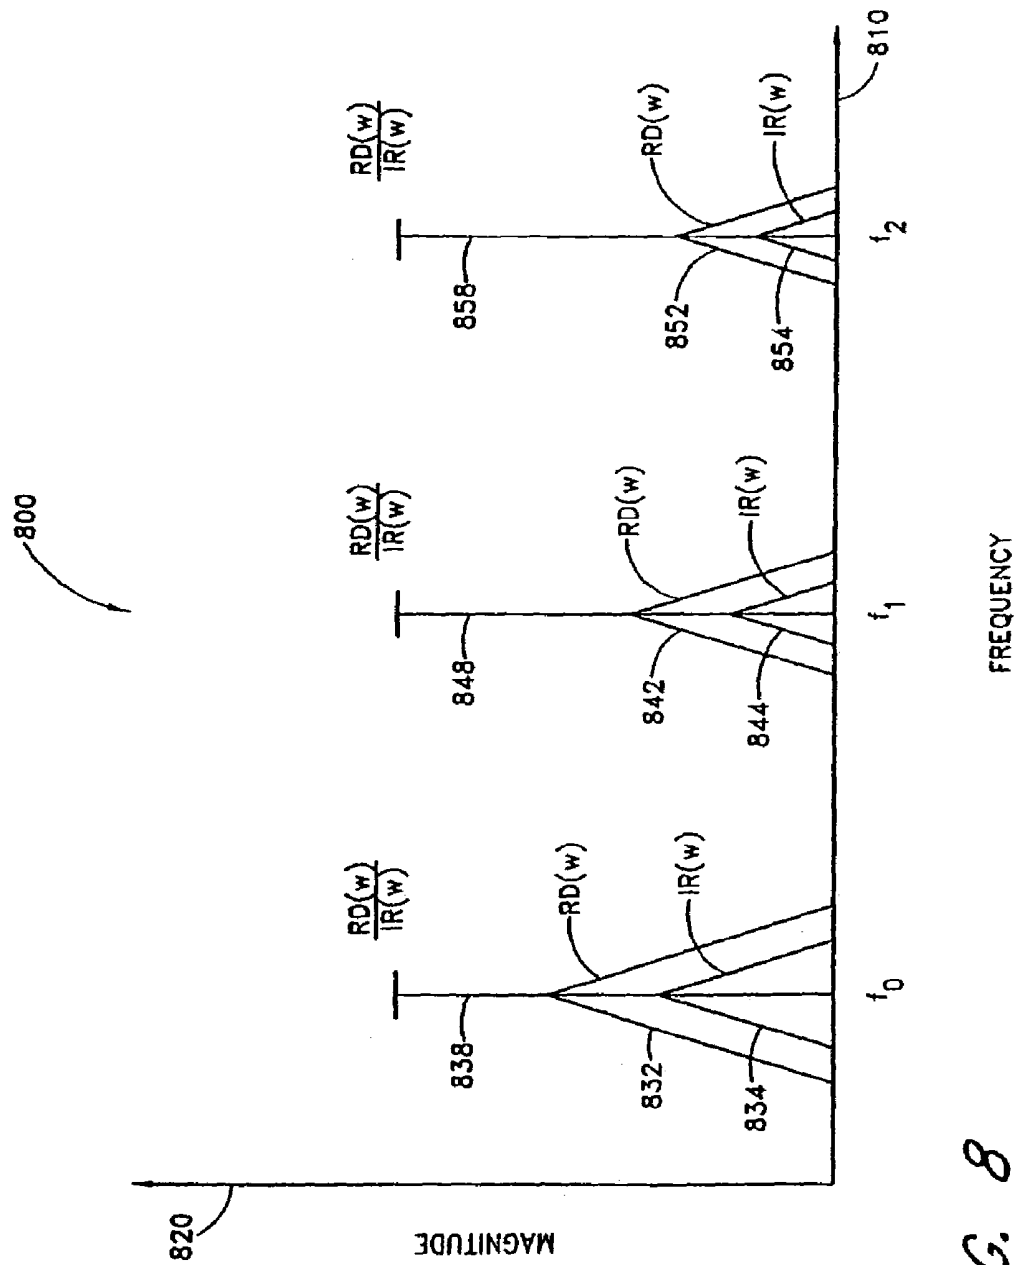


FIG. 8

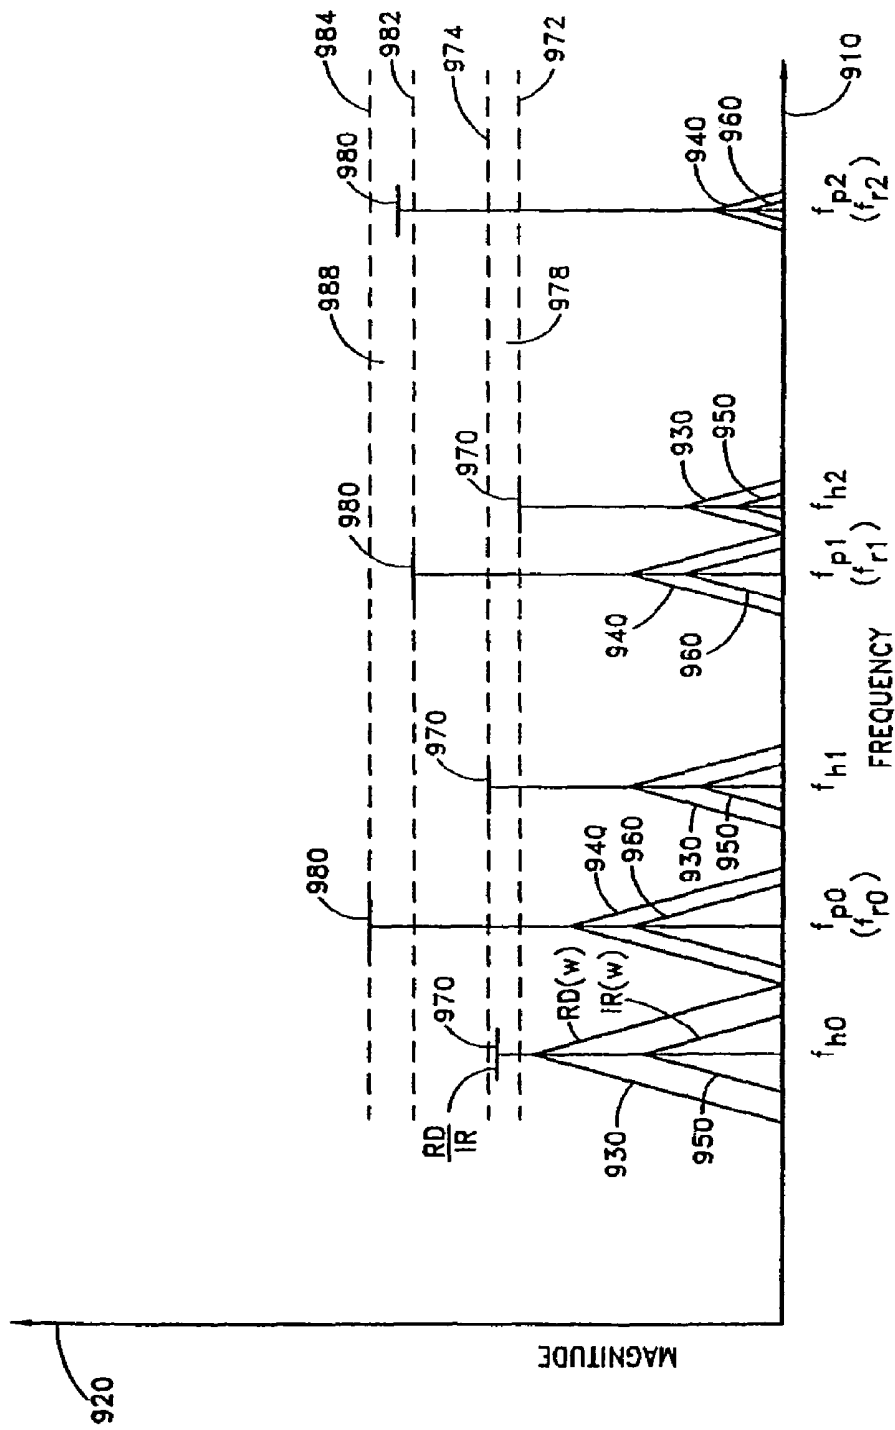


FIG. 9

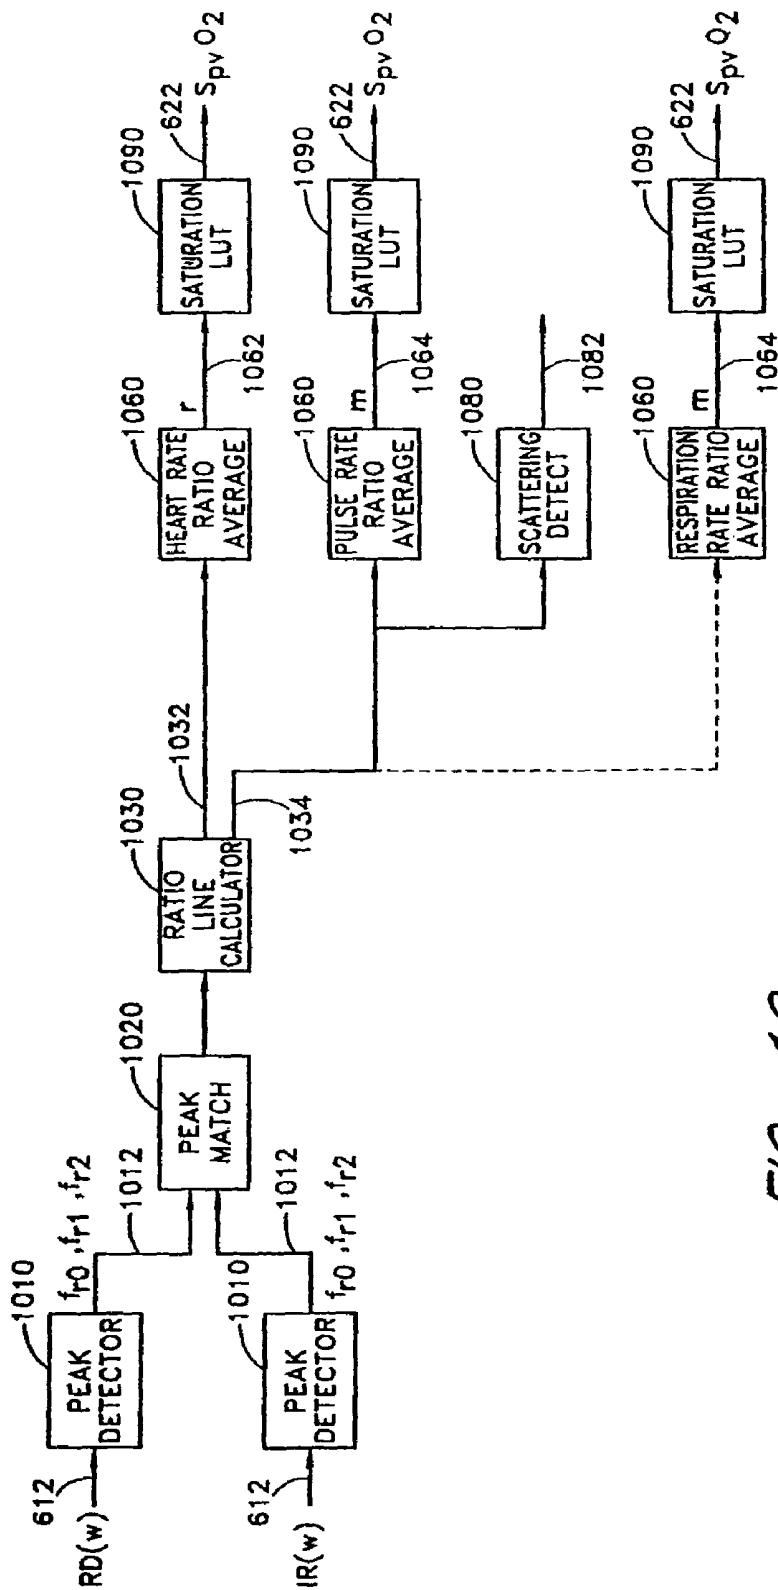


FIG. 10

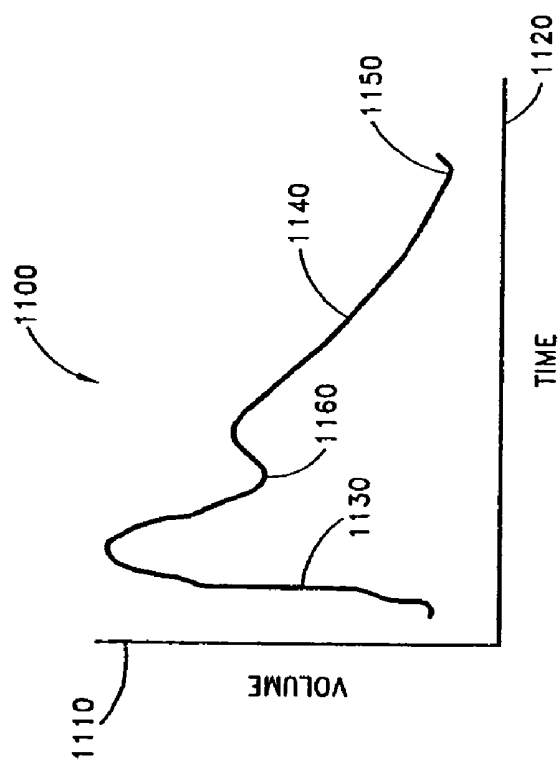


FIG. 11

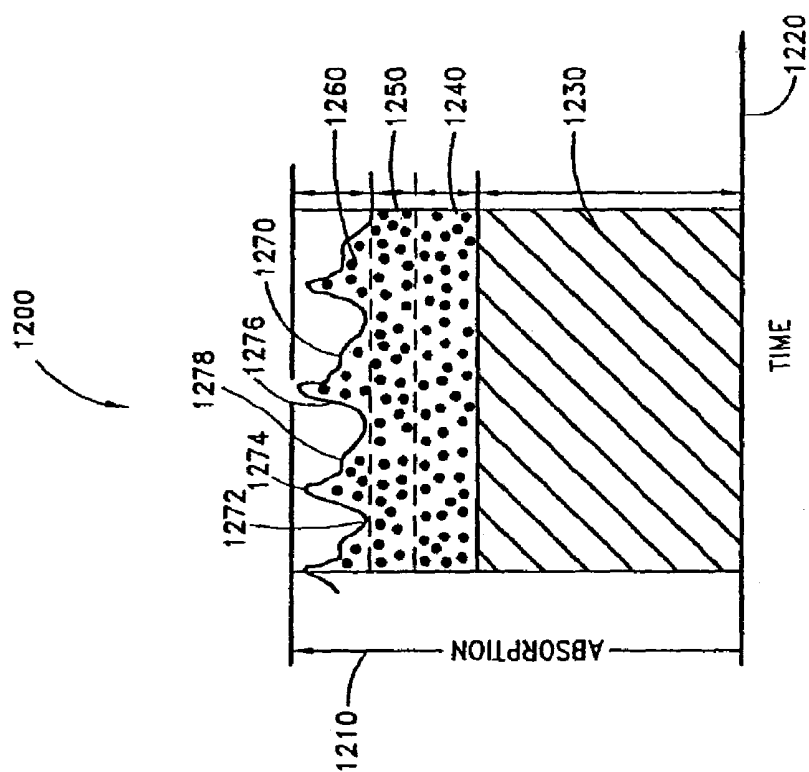


FIG. 12

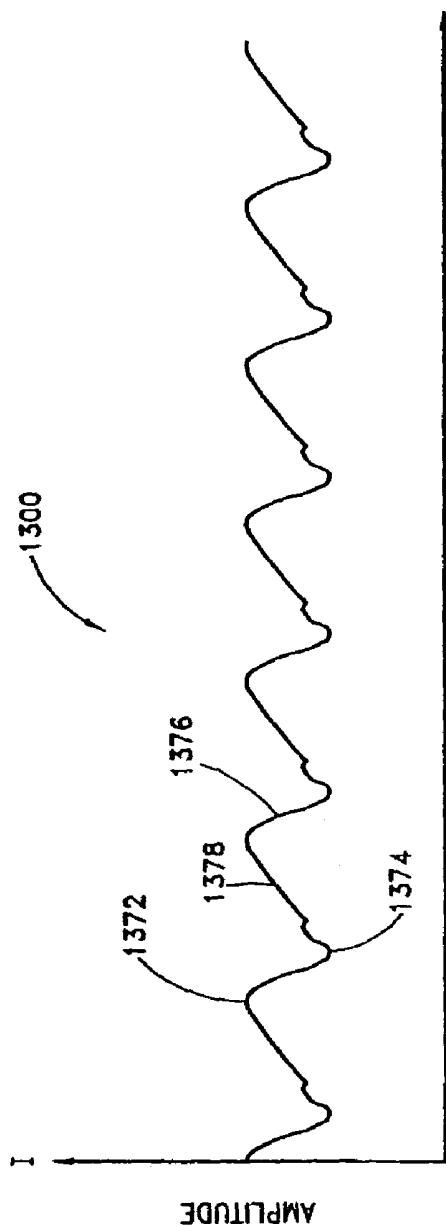


FIG. 13

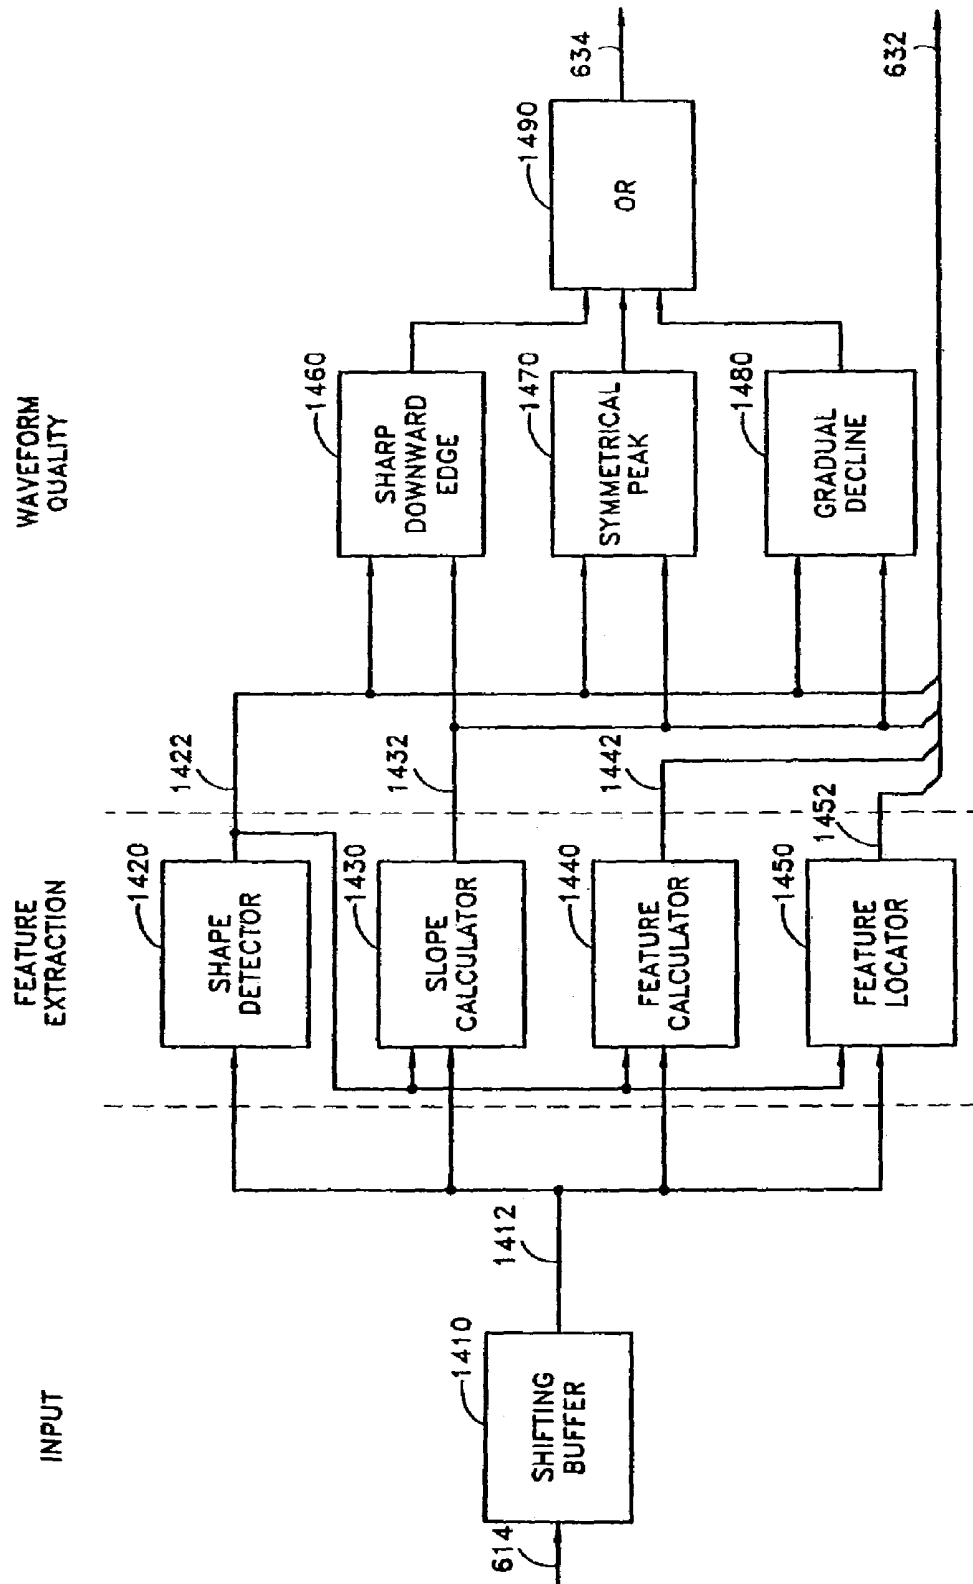


FIG. 14

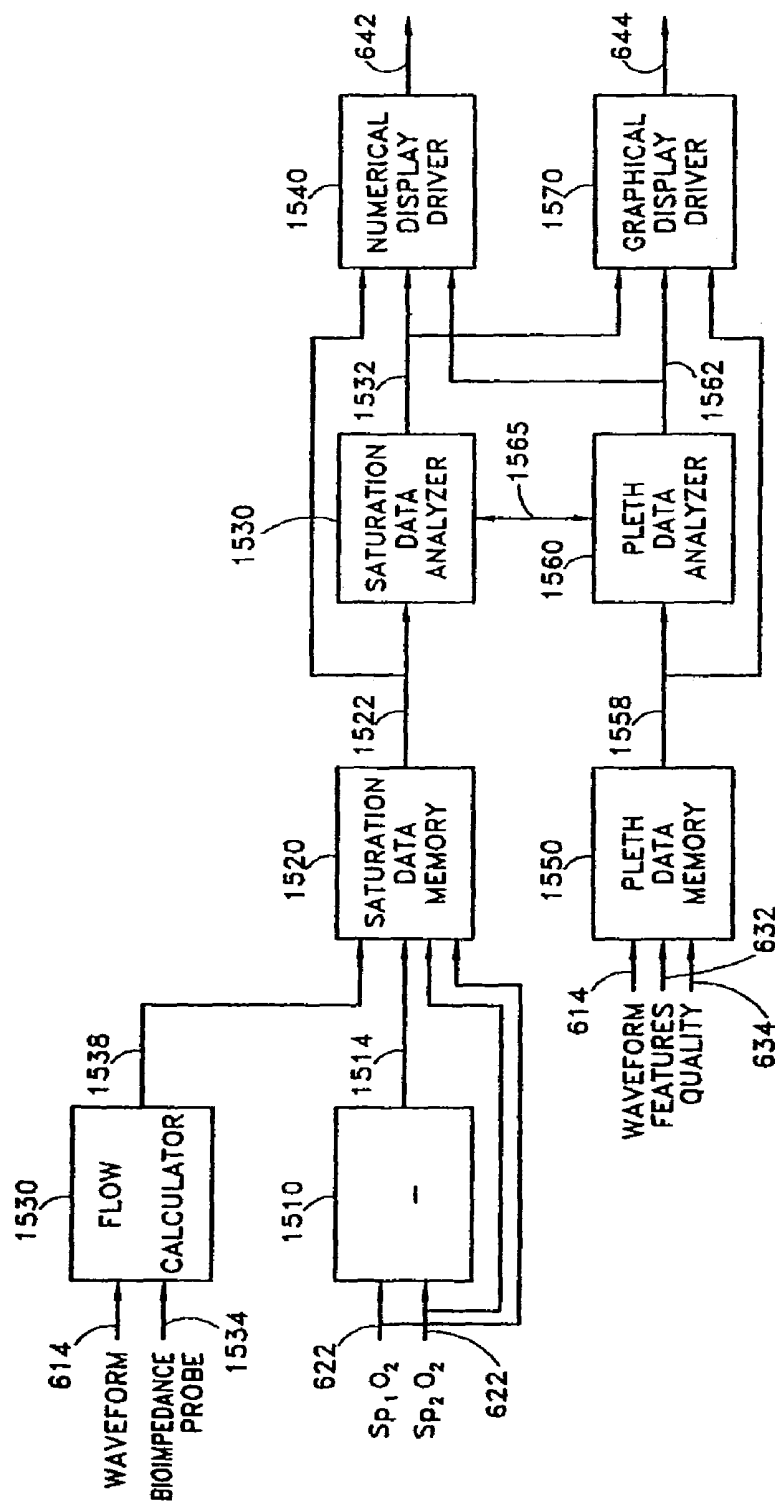


FIG. 15

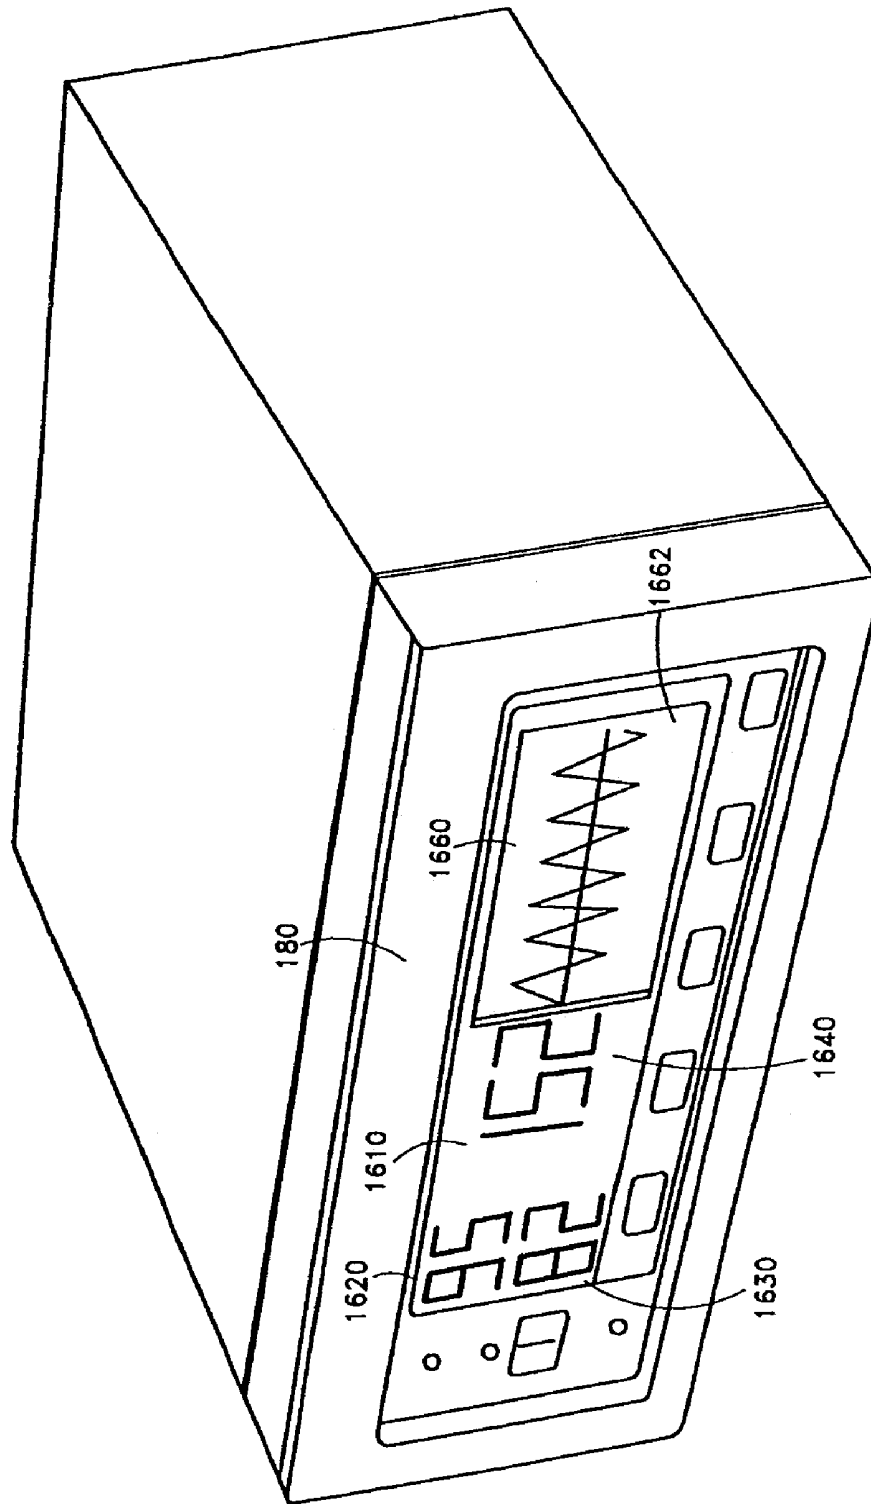


FIG. 16A

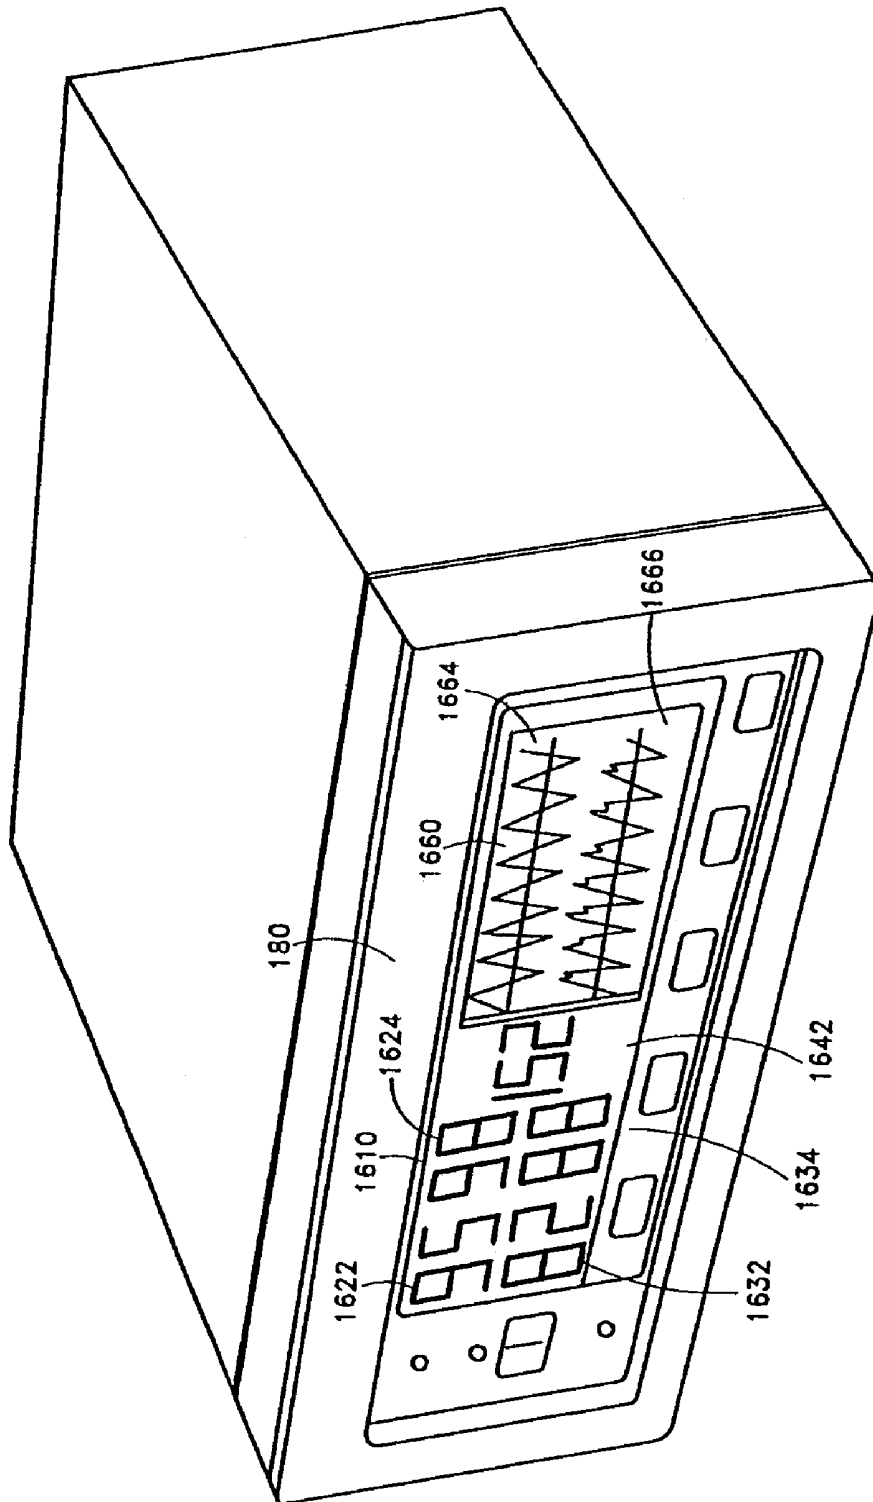


FIG. 16B

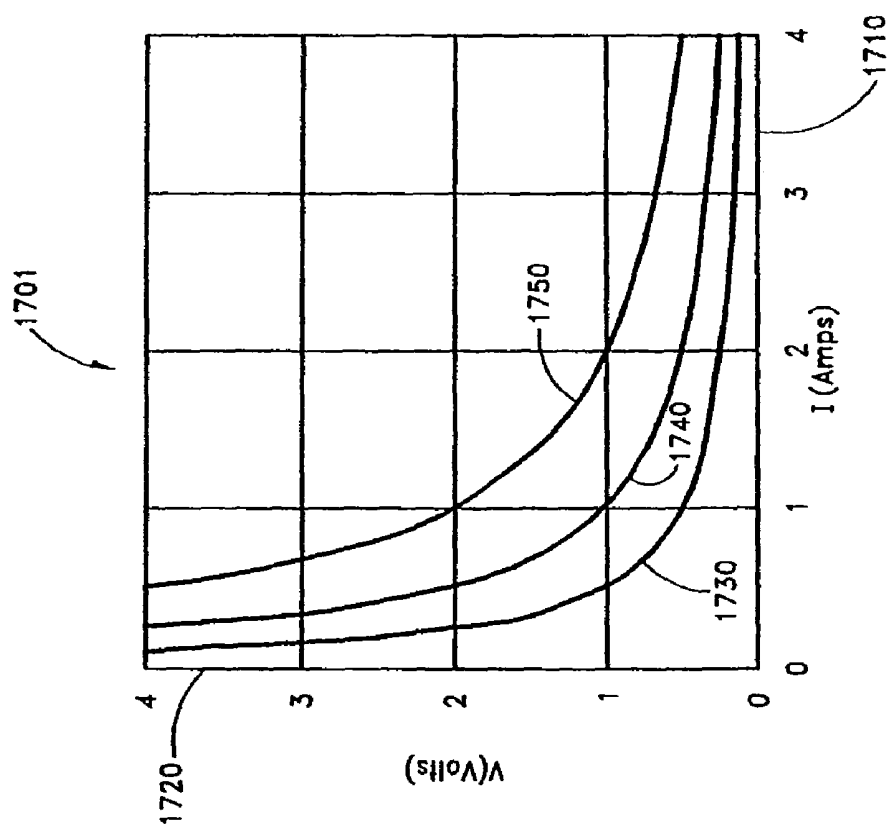


FIG. 17A

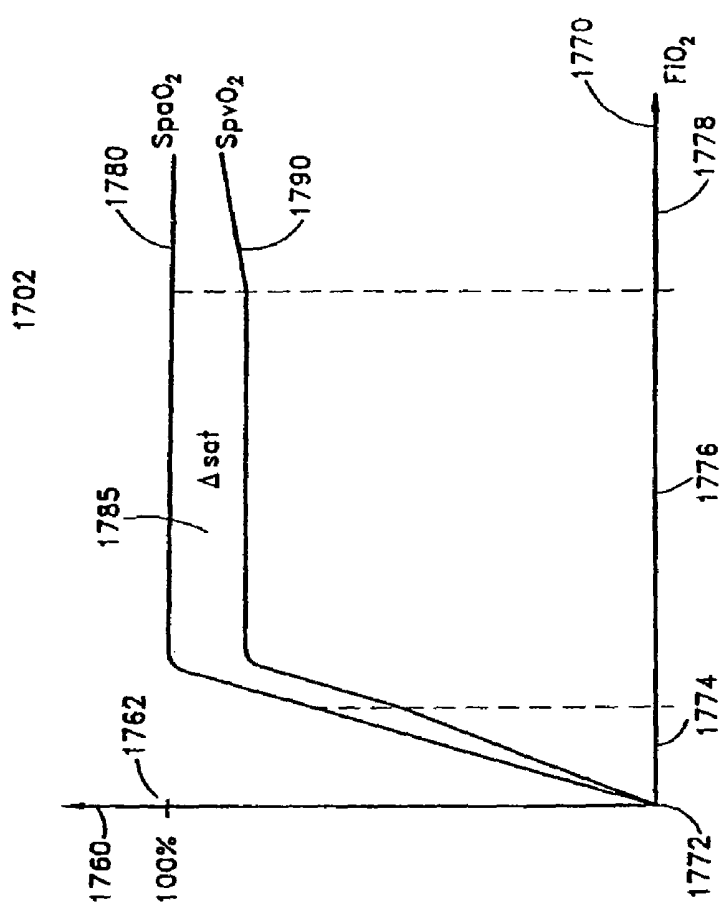
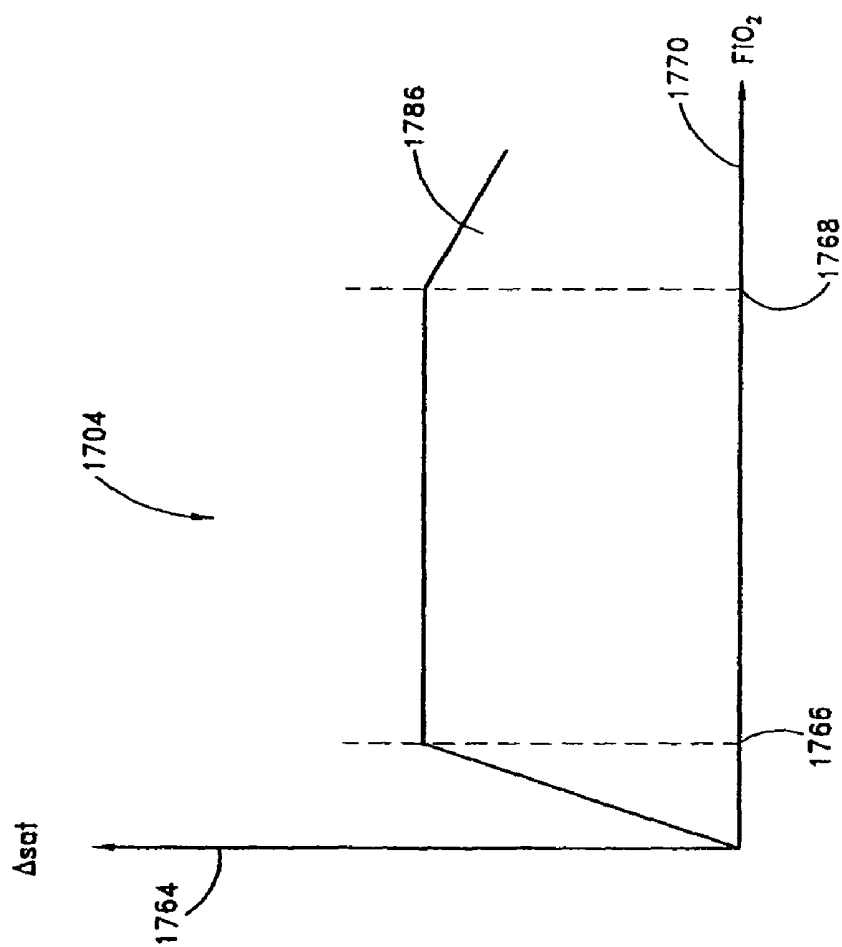


FIG. 17B



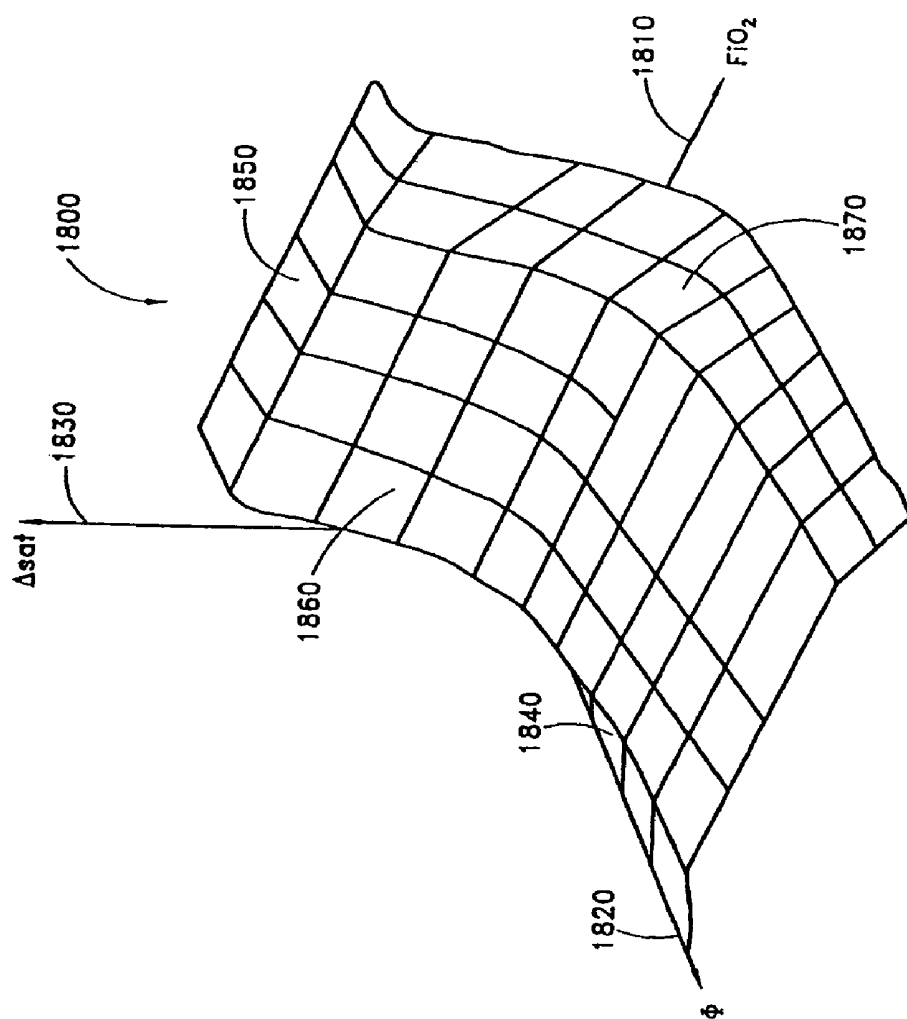


FIG. 18

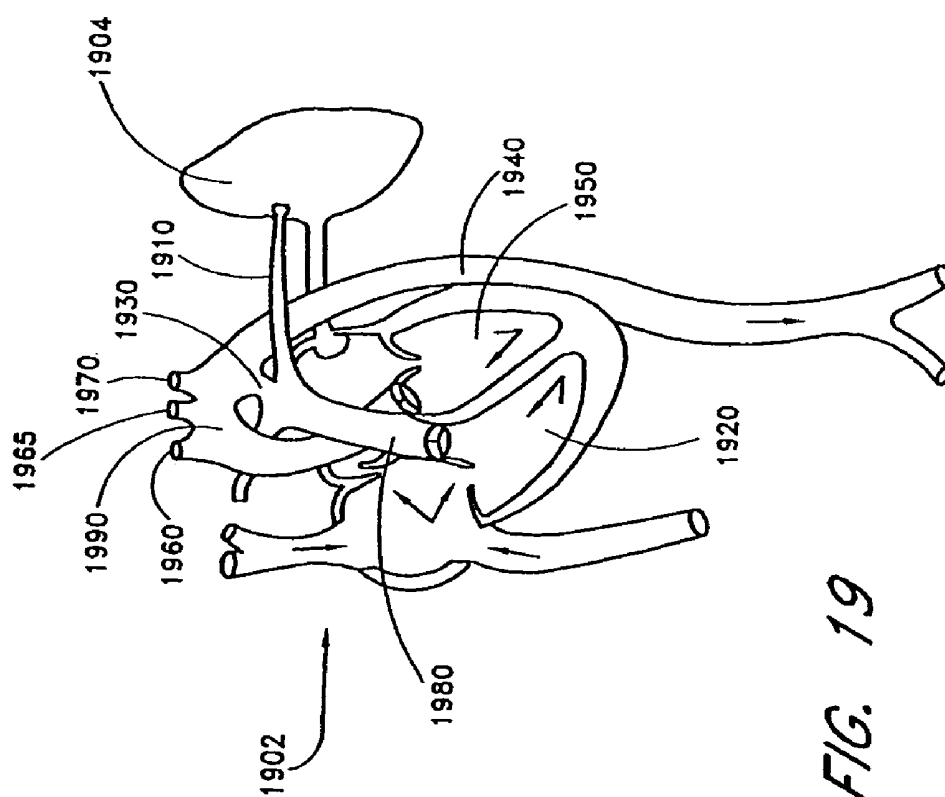


FIG. 19


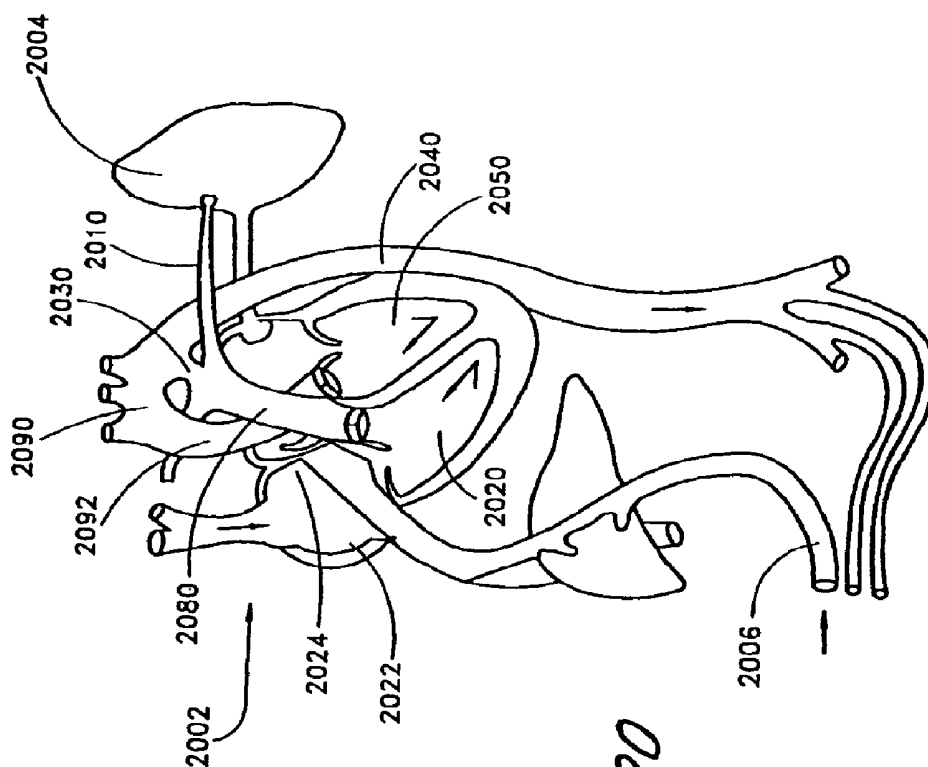


FIG. 20

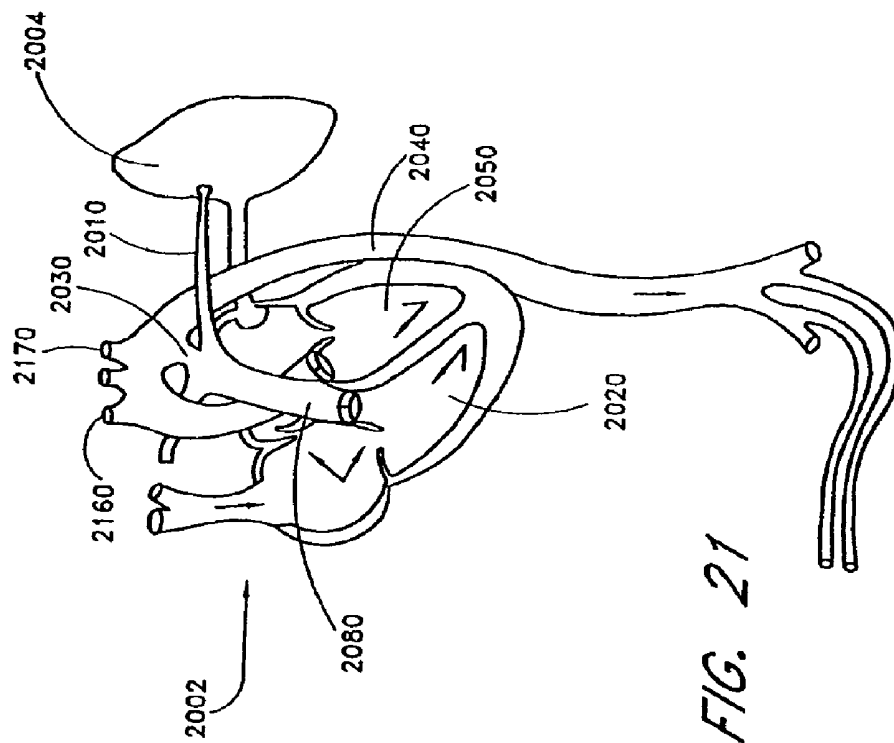

PHYSIOLOGICAL MONITOR

CROSS-REFERENCE TO RELATED APPLICATIONS

This application is a continuation of U.S. application Ser. No. 13/745,590, filed Jan. 18, 2013, which is a continuation of U.S. application Ser. No. 11/417,931, filed May 3, 2006, now U.S. Pat. No. 8,364,223, which is a continuation of U.S. application Ser. No. 11/104,720, filed Apr. 13, 2005, now U.S. Pat. No. 7,761,128, which is a continuation of U.S. application Ser. No. 10/668,487, filed Sep. 22, 2003, now U.S. Pat. No. 6,898,452, which is a continuation of U.S. application Ser. No. 10/026,013, filed Dec. 21, 2001, now U.S. Pat. No. 6,714,804, which is a continuation of U.S. application Ser. No. 09/323,176, filed May 27, 1999, now U.S. Pat. No. 6,334,065, which claims priority from U.S. Provisional No. 60/087,802, filed Jun. 3, 1998.

BACKGROUND

The measurement of oxygen delivery to the body and the corresponding oxygen consumption by its organs and tissues is vitally important to medical practitioners in the diagnosis and treatment of various medical conditions. Oxygen delivery, the transport of oxygen from the environment to organs and tissues, depends on the orchestration of several interrelated physiologic systems. Oxygen uptake is determined by the amount of oxygen entering the lung and the adequacy of gas exchange within the lung. This gas exchange is determined by the diffusion of oxygen from the alveolar space to the blood of the pulmonary capillaries. Oxygen is subsequently transported to all organs and tissues by blood circulation maintained by the action of the heart. The availability of oxygen to the organs and tissues is determined both by cardiac output and by the oxygen content in the blood. Oxygen content, in turn, is affected by the concentration of available hemoglobin and hemoglobin oxygen saturation. Oxygen consumption is related to oxygen delivery according to Fick's axiom, which states that oxygen consumption in the peripheral tissues is equal to oxygen delivery via the airway.

Oxygen delivery and oxygen consumption can be estimated from a number of measurable parameters. Because of the diagnostic impracticalities of measuring oxygen uptake and cardiac output, oxygen delivery is typically assessed from the oxygen status of arterial blood alone, such as arterial oxygen partial pressure, P_aO_2 , and arterial oxygen saturation, S_aO_2 . P_aO_2 represents the relatively small amount of oxygen dissolved in the blood plasma. S_aO_2 represents the much larger amount of oxygen chemically bound to the blood hemoglobin. Oxygen consumption is typically assessed from the oxygen status of mixed venous blood, i.e. the oxygen saturation of blood from the pulmonary artery, S_vO_2 , which is used to estimate the O_2 concentration of blood returning from all tissues and organs of the body. These parameters can be measured by both invasive and non-invasive techniques, except S_vO_2 , which requires an invasive measurement.

Invasive techniques include blood gas analysis using the in vitro measurement of extracted arterial or venous blood, drawn with a syringe and needle or an intervascular catheter. Arterial blood is commonly obtained by puncturing the brachial, radial or femoral artery. Venous blood can be obtained from an arm vein, but such a sample reflects only local conditions. To obtain mixed venous blood, which represents the composite of all venous blood, a long catheter

is typically passed through the right heart and into the main pulmonary artery from a peripheral vein. Extracted blood gas analysis utilizes blood gas machines or oximeters. A blood gas machine measures the partial pressure of oxygen, PO_2 , using a "Clark electrode" that detects the current generated by oxygen diffusing to a sealed platinum electrode across a gas permeable membrane. An oximeter measures the oxygen saturation, SO_2 , of oxygenated and deoxygenated hemoglobin using spectrophotometry techniques that detect the differential absorption of particular wavelengths of light by these blood components.

Invasive monitoring also includes the in vivo monitoring of blood gas via a catheter sensor inserted into an artery or vein. Miniaturization of the Clark electrode allows placement of the electrode in a catheter for continuous measurement of PO_2 . A fiber optic equipped catheter attached to an external oximeter allows continuous measurement of oxygen saturation. Because of risks inherent in catheterization and the promotion of blood coagulation by certain sensors, these techniques are typically only used when vitally indicated.

Non-invasive techniques include pulse oximetry, which allows the continuous in vivo measurement of arterial oxygen saturation and pulse rate in conjunction with the generation of a photoplethysmograph waveform. Measurements rely on sensors which are typically placed on the fingertip of an adult or the foot of an infant. Non-invasive techniques also include transcutaneous monitoring of PO_2 , accomplished with the placement of a heated Clark electrode against the skin surface. These non-invasive oxygen status measurement techniques are described in further detail below.

SUMMARY

Prior art invasive oxygen assessment techniques are inherently limited. Specifically, in vitro measurements, that is, blood extraction and subsequent analysis in a blood gas machine or an oximeter, are non-simultaneous and non-continuous. Further, in vivo measurements through catheterization are not casual procedures and are to be particularly avoided with respect to neonates. Prior art noninvasive techniques are also limited. In particular, conventional pulse oximeters are restricted to measurement of arterial oxygen saturation at a single patient site. Also, transcutaneous monitoring is similarly restricted to the measurement of an estimate of arterial partial pressure at a single patient site, among other limitations discussed further below.

The stereo pulse oximeter according to the present invention overcomes many of the limitations of prior art oxygen status measurements. The word "stereo" comes from the Greek word stereos, which means "solid" or three-dimensional. For example, stereophonic systems use two or more channels to more accurately reproduce sound. The stereo pulse oximeter is similarly multi-dimensional, providing simultaneous, continuous, multiple-site and multiple-parameter oxygen status and plethysmograph (photoplethysmograph) measurements. The stereo pulse oximeter provides a benefit in terms of cost and patient comfort and safety over invasive oxygen status estimation techniques. The multi-dimensional aspects of this invention further provide oxygen status and plethysmograph measurements not available from current noninvasive techniques. In addition, the stereo pulse oximeter allows the isolation of noise artifacts, providing more accurate oxygen status and plethysmograph measurements than available from conventional techniques. The

result is improved patient outcome based on a more accurate patient assessment and better management of patient care.

In one aspect of the stereo pulse oximeter, data from a single sensor is processed to advantageously provide continuous and simultaneous multiple-parameter oxygen status and plethysmograph measurements from a particular tissue site. This is in contrast to a conventional pulse oximeter that provides only arterial oxygen saturation data from a tissue site. In particular a physiological monitor comprises a sensor interface and a signal processor. The sensor interface is in communication with a peripheral tissue site and has an output responsive to light transmitted through the site. The signal processor is in communication with the sensor interface output and provides a plurality of parameters corresponding to the oxygen status of the site, the plethysmograph features of the site or both. The parameters comprise a first value and a second value related to the peripheral tissue site. In one embodiment, the first value is an arterial oxygen saturation and the second value is a venous oxygen saturation. In this embodiment, another parameter provided may be the difference between arterial oxygen saturation and venous oxygen saturation at the tissue site. The venous oxygen saturation is derived from an active pulse generated at the site. The signal processor output may further comprise a scattering indicator corresponding to the site, and the sensor interface may further comprise a pulser drive, which is responsive to the scattering indicator to control the amplitude of the active pulse. One of the parameter values may also be an indication of perfusion.

In another aspect of the stereo pulse oximeter, data from multiple sensors is processed to advantageously provide continuous and simultaneous oxygen status measurements from several patient tissue sites. This is in contrast to a conventional pulse oximeter that processes data from a single sensor to provide oxygen status at a single tissue site. In particular, a physiological monitor comprises a plurality of sensor interfaces each in communications with one of a plurality of peripheral tissue sites. Each of the sensor interfaces has one of a plurality of outputs responsive to light transmitted through a corresponding one of the tissue sites. A signal processor is in communication with the sensor interface outputs and has a processor output comprising a plurality of parameters corresponding to the oxygen status of the sites, the plethysmograph features of the sites or both. The parameters may comprise a first value relating to a first of the peripheral tissue sites and a second value relating to a second of the peripheral tissue sites. In one embodiment, the first value and the second value are arterial oxygen saturations. In another embodiment, the first value and the second value are plethysmograph waveform phases. The physiological monitor may further comprise a sensor attachable to each of the tissue sites. This sensor comprises a plurality of emitters and a plurality of detectors, where at least one of the emitters and at least one of the detectors is associated with each of the tissue sites. The sensor also comprises a connector in communications with the sensor interfaces. A plurality of signal paths are attached between the emitters and the detectors at one end of the sensor and the connector at the other end of the sensor.

In yet another aspect of the stereo pulse oximeter, data from multiple sensors is processed to advantageously provide a continuous and simultaneous comparison of the oxygen status between several tissue sites. A conventional oximeter, limited to measurements at a single tissue site, cannot provide these cross-site comparisons. In particular a physiological monitoring method comprises the steps of deriving a reference parameter and a test parameter from

oxygen status measured from at least one of a plurality of peripheral tissue sites and comparing that reference parameter to the test parameter so as to determine a patient condition. The reference parameter may be a first oxygen saturation value and the test parameter a second oxygen saturation value. In that case, the comparing step computes a delta oxygen saturation value equal to the arithmetic difference between the first oxygen saturation value and the second oxygen saturation value. In one embodiment, the reference parameter is an arterial oxygen saturation measured at a particular one the tissue sites and the test parameter is a venous oxygen saturation measured at that particular site. In another embodiment, the reference parameter is a first arterial oxygen saturation value at a first of the tissue sites, the test parameter is a second arterial oxygen saturation value at a second of the tissue sites. In yet another embodiment, the reference parameter is a plethysmograph feature measured at a first of the sites, the test parameter is a plethysmograph feature measured at a second of the sites and the monitoring method comparison step determines the phase difference between plethysmographs at the first site and the second site. In a further embodiment, the comparing step determines a relative amount of damping between plethysmographs at the first site and the second site. The multi-dimensional features of these embodiments of the stereo pulse oximeter can be advantageously applied to the diagnosis and managed medical treatment of various medical conditions. Particularly advantageous applications of stereo pulse oximetry include oxygen titration during oxygen therapy, nitric oxide titration during therapy for persistent pulmonary hypertension in neonates (PPHN), detection of a patent ductus arteriosus (PDA), and detection of an aortic coarctation.

BRIEF DESCRIPTION OF THE DRAWINGS

The present invention will be described in detail below in connection with the following drawing figures in which:

FIG. 1A is a top-level block diagram of a stereo pulse oximeter according to the present invention;

FIG. 1B shows a single-sensor alternative embodiment to FIG. 1A;

FIG. 2 is a block diagram of the stereo pulse oximeter sensor interface;

FIG. 3 is a graph illustrating the absorption of red and infrared wavelengths by both oxygenated and deoxygenated hemoglobin;

FIG. 4 is a graph showing the empirical relationship between the "red over infrared" ratio and arterial oxygen saturation;

FIG. 5 is a block diagram of the analog signal conditioning for the sensor interface;

FIG. 6 is a functional block diagram of the stereo pulse oximeter signal processing;

FIG. 7 is a functional block diagram of the front-end signal processing;

FIG. 8 is a graph depicting the frequency spectrum of an arterial intensity signal;

FIG. 9 is a graph depicting the frequency spectrum of a combined arterial and venous intensity signal;

FIG. 10 is a functional block diagram of the saturation calculation signal processing;

FIG. 11 is a graph illustrating a plethysmograph waveform;

FIG. 12 is a graph illustrating the absorption contribution of various blood and tissue components;

5

FIG. 13 is a graph illustrating an intensity “plethysmograph” pulse oximetry waveform;

FIG. 14 is a functional block diagram of the plethysmograph feature extraction signal processing;

FIG. 15 is a functional block diagram of the multiple parameter signal processing;

FIG. 16A is an illustration of a single-site stereo pulse oximeter display screen;

FIG. 16B is an illustration of a multi-site stereo pulse oximeter display screen;

FIG. 17A is a graph depicting a family of constant power curves for the electrical analog of constant oxygen consumption;

FIG. 17B is a graph depicting arterial and venous oxygen saturation versus fractional inspired oxygen;

FIG. 17C is a graph depicting arterial minus venous oxygen saturation versus fractional inspired oxygen;

FIG. 18 is a three-dimensional graph depicting a delta oxygen saturation surface;

FIG. 19 is an illustration of a neonatal heart depicting a pulmonary hypertension condition;

FIG. 20 is an illustration of a fetal heart depicting the ductus arteriosus; and

FIG. 21 is an illustration of a neonatal heart depicting a patent ductus arteriosus (PDA).

DETAILED DESCRIPTION

Stereo Pulse Oximetry

FIG. 1A illustrates the multi-dimensional features of a stereo pulse oximeter 100 according to the present invention. Shown in FIG. 1A is an exemplary stereo pulse oximeter configuration in which a first sensor 110 is attached to a neonate's left hand, a second sensor 120 is attached to one of the neonate's feet, and a third sensor 130 is attached to the neonate's right hand. In general, these sensors are used to obtain oxygen status and photoplethysmograph measurements at peripheral sites, including a person's ears and face, such as the nose and regions of the mouth in addition to hands, feet and limbs, but not including internal sites such as internal organs and the brain.

Each sensor 110, 120, 130 provides a stream of data through a corresponding sensor interface 114, 124, 134 to the digital signal processor (DSP) 150. For example, the first sensor 110 is connected to an input 112 of the first sensor interface 114, and the output 118 of the first sensor interface 114 is attached to a first data channel input 152 of the DSP 150. Similarly, the second sensor 120 provides data to a second data channel input 154 and the third sensor 130 provides data to a third data channel input 158.

FIG. 1B illustrates an alternative embodiment of the separate sensors 110, 120, 130 (FIG. 1A). A stereo sensor 140 has multiple branches 112, 122, 132 each terminating in a sensor portion 114, 124, 134. Each sensor portion 114, 124, 134 has two light emitters and a light detector, as described below, and is attachable to a separate patient site. Thus, the stereo sensor 140 advantageously provides a single sensor device having multiple light emitters and multiple light detectors for attachment to multiple patient tissue sites. A combination of the stereo sensor 140 and a single patient cable 142 advantageously allows a single connection 144 at the stereo pulse oximeter 100 and a single connection 146 at the stereo sensor 140.

The DSP 150 can independently process each data channel input 152, 154, 158 and provide outputs 162 typical of pulse oximetry outputs, such as arterial oxygen saturation, Sp_aO_2 , the associated plethysmograph waveform and the

6

derived pulse rate. In contrast with a conventional pulse oximeter, however, these outputs 162 include simultaneous measurements at each of several patient tissue sites. That is, for the configuration of FIG. 1A, the stereo pulse oximeter 100 simultaneously displays Sp_aO_2 and an associated plethysmograph waveform for three tissue sites in addition to the patient's pulse rate obtained from any one of sites. Further, the DSP 150 can provide unique outputs unavailable from conventional pulse oximeters. These outputs 164 include venous oxygen saturation, Sp_vO_2 , a comparison of arterial and venous oxygen saturation, $\Delta sat = Sp_aO_2 - Sp_vO_2$, and pleth, which denotes plethysmograph shape parameters, for each site. In addition, the DSP 150 can provide cross-site outputs that are only available using stereo pulse oximetry. These unique cross-site outputs 168 include $\Delta sat_{xy} = Sp_{ax}O_2 - Sp_{ay}O_2$, which denotes the arterial oxygen saturation at site x minus the arterial oxygen saturation at site y. Also included in these outputs 168 is $\Delta pleth_{xy}$, which denotes a comparison of plethysmograph shape parameters measured at site x and site y, as described in detail below. The stereo pulse oximeter also includes a display 180 capable of showing the practitioner the oxygen status and plethysmograph parameters described above. The display 180 has a multiple channel graphical and numerical display capability as described in more detail below.

Pulse Oximetry Sensor

FIG. 2 depicts one stereo pulse oximeter data channel having a sensor 110 and a sensor interface 114 providing a single data channel input 152 to the DSP 150. The sensor 110 is used to measure the intensity of red and infrared light after transmission through a portion of the body where blood flows close to the surface, such as a fingertip 202. The sensor 110 has two light emitters, each of which may be, for example, a light-emitting diode (LED). A red emitter 212, which transmits light centered at a red wavelength and an infrared (IR) emitter 214, which transmits light centered at an infrared wavelength are placed adjacent to, and illuminate, a tissue site. A detector 218, which may be a photodiode, is used to detect the intensity of the emitted light after it passes through, and is partially absorbed by, the tissue site. The emitters 212, 214 and detector 218 are secured to the tissue site, with the emitters 212, 214 typically spaced on opposite sides of the tissue site from the detector 218.

To distinguish between tissue absorption at the two wavelengths, the red emitter 212 and infrared emitter 214 are modulated so that only one is emitting light at a given time. In one embodiment, the red emitter 212 is activated for a first quarter cycle and is off for the remaining three-quarters cycle; the infrared emitter 214 is activated for a third quarter cycle and is off for the remaining three-quarters cycle. That is, the emitters 212, 214 are cycled on and off alternately, in sequence, with each only active for a quarter cycle and with a quarter cycle separating the active times. The detector 218 produces an electrical signal corresponding to the red and infrared light energy attenuated from transmission through the patient tissue site 202. Because only a single detector 218 is used, it receives both the red and infrared signals to form a time-division-multiplexed (TDM) signal. This TDM signal is coupled to the input 112 of the sensor interface 114. One of ordinary skill in the art will appreciate alternative activation sequences for the red emitter 212 and infrared emitter 214 within the scope of this invention, each of which provides a time multiplexed signal from the detector 218 allowing separation of red and infrared signals and determination and removal of ambient light levels in downstream signal processing.

To compute Sp_aO_2 , pulse oximetry relies on the differential light absorption of oxygenated hemoglobin, HbO_2 , and deoxygenated hemoglobin, Hb , to compute their respective concentrations in the arterial blood. This differential absorption is measured at the red and infrared wavelengths of the sensor **110**. The relationship between arterial oxygen saturation and hemoglobin concentration can be expressed as:

$$Sp_aO_2 = 100 \frac{C_{HbO_2}}{C_{Hb} + C_{HbO_2}} \quad (1)$$

That is, arterial oxygen saturation is the percentage concentration of oxygenated hemoglobin compared to the total concentration of oxygenated hemoglobin and deoxygenated hemoglobin in the arterial blood. Sp_aO_2 is actually a measure of the partial oxygen saturation of the hemoglobin because other hemoglobin derivatives, such as COHb and MetHb, are not taken into consideration.

FIG. **3** shows a graph **300** of the optical absorption properties of HbO_2 and Hb . The graph **300** has an x-axis **310** corresponding to wavelength and a y-axis **320** corresponding to hemoglobin absorption. An Hb curve **330** shows the light absorption properties of deoxygenated hemoglobin. An HbO_2 curve **340** shows the light absorption properties of oxygenated hemoglobin. Pulse oximetry measurements are advantageously made at a red wavelength **350** corresponding to 660 nm and an infrared wavelength **360** corresponding to 905 nm. This graph **300** shows that, at these wavelengths **350**, **360**, deoxygenated hemoglobin absorbs more red light than oxygenated hemoglobin, and, conversely, oxygenated hemoglobin absorbs more infrared light than deoxygenated hemoglobin.

In addition to the differential absorption of hemoglobin derivatives, pulse oximetry relies on the pulsatile nature of arterial blood to differentiate hemoglobin absorption from absorption of other constituents in the surrounding tissues. Light absorption between systole and diastole varies due to the blood volume change from the inflow and outflow of arterial blood at a peripheral tissue site. This tissue site might also comprise skin, muscle, bone, venous blood, fat, pigment, etc., each of which absorbs light. It is assumed that the background absorption due to these surrounding tissues is invariant and can be ignored. Thus, blood oxygen saturation measurements are based upon a ratio of the time-varying or AC portion of the detected red and infrared signals with respect to the time-invariant or DC portion. This AC/DC ratio normalizes the signals and accounts for variations in light pathlengths through the measured tissue. Further, a ratio of the normalized absorption at the red wavelength over the normalized absorption at the infrared wavelength is computed:

$$\frac{RD}{IR} = \frac{\left(\frac{Red_{AC}}{Red_{DC}} \right)}{\left(\frac{IR_{AC}}{IR_{DC}} \right)} \quad (2)$$

where Red_{AC} and IR_{AC} are the root-mean-square (RMS) of the corresponding time-varying signals. This “red-over-infrared, ratio-of-ratios” cancels the pulsatile signal. The desired Sp_aO_2 measurement is then computed from this ratio.

FIG. **4** shows a graph **400** depicting the relationship between RD/IR and Sp_aO_2 . This relationship can be approximated from Beer-Lambert’s Law, as outlined below. However, it is most accurately determined by statistical regression of experimental measurements obtained from human volunteers and calibrated measurements of oxygen saturation. The result can be depicted as a curve **410**, with measured values of RD/IR shown on a y-axis **420** and corresponding saturation values shown on an x-axis **430**. In a pulse oximeter device, this empirical relationship can be stored in a read-only memory (ROM) look-up table so that Sp_aO_2 can be directly read-out from input RD/IR measurements.

According to the Beer-Lambert law of absorption, the intensity of light transmitted through an absorbing medium is given by:

$$I = I_0 \exp \left(- \sum_{i=1}^N \epsilon_{i\lambda} c_i x_i \right) \quad (3)$$

where I_0 is the intensity of the incident light, $\epsilon_{i\lambda}$ is the absorption coefficient of the i^{th} constituent at a particular wavelength λ , c_i is the concentration coefficient of the i^{th} constituent and x_i is the optical path length of the i^{th} constituent. As stated above, assuming the absorption contribution by all constituents but the arterial blood is constant, taking the natural logarithm of both sides of equation (3) and removing time invariant terms yields:

$$\ln(I) = -[\epsilon_{HbO_2,\lambda} C_{HbO_2} + \epsilon_{Hb,\lambda} C_{hb}] x(t) \quad (4)$$

Measurements taken at both red and infrared wavelengths yield:

$$RD(t) = -[\epsilon_{HbO_2,RD} C_{HbO_2} + \epsilon_{Hb,RD} C_{hb}] x_{RD}(t) \quad (5)$$

$$IR(t) = -[\epsilon_{HbO_2,IR} C_{HbO_2} + \epsilon_{Hb,IR} C_{hb}] x_{IR}(t) \quad (6)$$

Taking the ratio $RD(t)/IR(t)$ and assuming $x_{RD}(t) \approx x_{IR}(t)$ yields:

$$\frac{RD}{IR} = \frac{[\epsilon_{HbO_2,RD} C_{HbO_2} + \epsilon_{Hb,RD} C_{hb}]}{[\epsilon_{HbO_2,IR} C_{HbO_2} + \epsilon_{Hb,IR} C_{hb}]} \quad (7)$$

Assuming further that:

$$C_{HbO_2} + C_{Hb} = 1 \quad (8)$$

then equation (1) can be solved in terms of RD/IR yielding a curve similar to the graph **400** of FIG. **4**.

Sensor Interface

FIG. **2** also depicts the sensor interface **114** for one data channel. An interface input **112** from the sensor **110** is coupled to an analog signal conditioner **220**. The analog signal conditioner **220** has an output **223** coupled to an analog-to-digital converter (ADC) **230**. The ADC output **118** is coupled to the DSP **150**. The analog signal conditioner also has a gain control input **225** from the DSP **150**. The functions of the analog signal conditioner **220** are explained in detail below. The ADC **230** functions to digitize the input signal **112** prior to further processing by the DSP **150**, as described below. The sensor interface **114** also has an emitter current control input **241** coupled to a digital-to-analog converter (DAC) **240**. The DSP provides control information to the DAC **240** via the control input **241** for a pair of emitter current drivers **250**. One driver output **252** couples to the red emitter **212** of the sensor **110**, and another driver output **254** couples to the IR emitter **214** of the sensor **110**.

FIG. 5 illustrates one embodiment of the analog signal conditioner 220. The analog signal conditioner 220 receives a composite intensity signal 112 from the sensor detector 218 (FIG. 2) and then filters and conditions this signal prior to digitization. The embodiment shown has a preamplifier 510, a high pass filter 520, a programmable gain amplifier 530 and a low pass filter 540. The low pass filter output 223 is coupled to the ADC 230 (FIG. 2). The preamplifier 510 converts the current signal 112 from the detector 218 (FIG. 2) to a corresponding amplified voltage signal. The gain in the preamplifier 510 is selected in order to prevent ambient light in the signal 112 from saturating the preamplifier 510 under normal operating conditions. The preamplifier output 512 is coupled to the high pass filter 520, which removes the DC component of the detector signal 112. The corner frequency of the high pass filter 520 is set well below the multiplexing frequency of the red and infrared emitters 212, 214 (FIG. 2). The high pass filter output 522 couples to the programmable gain amplifier 530, which also accepts a programming input 225 from the DSP 150 (FIG. 2). This gain is set at initialization or at sensor placement to compensate for variations from patient to patient. The programmable gain amplifier output 532 couples to a low-pass filter 540 to provide anti-aliasing prior to digitization.

As described above, pulse oximetry measurements rely on the existence of a pulsatile signal. The natural heart beat provides a pulsatile signal that allows measurement of arterial oxygen saturation. In the systemic circulation, all arterial pulsations are damped before flow enters the capillaries, and none are transmitted into the veins. Thus, there is no arterial pulse component in the venous blood and absorption caused by venous blood is assumed canceled by the ratio-of-ratio operation described above. Venous blood, being at a relatively low pressure, will “slosh back and forth” during routine patient motions, such as shivering, waving and tapping. This venous blood sloshing creates a time-varying signal that is considered “noise” and can easily overwhelm conventional ratio-based pulse oximeters. Advanced pulse oximetry techniques allow measurement of Sp_o_2 under these circumstances. For example, such advanced techniques are disclosed in U.S. Pat. No. 5,632,272, which is assigned to the assignee of the current application. This measurement is only available during motion or other physiological events causing a time-varying venous signal.

The venous blood may also have a pulsatile component at the respiration rate, which can be naturally induced or ventilator induced. In adults, the natural respiration rate is 10-15 beats per minute (bpm). In neonates, this natural respiration rate is 30-60 bpm. The ventilator induced pulse rate depends on the ventilator frequency. If this respiration induced venous pulse is of sufficient magnitude, advanced pulse oximetry techniques, described below, allow measurement of Sp_o_2 .

A controlled physiological event, however, can be created that allows for a continuous measurement of venous oxygen saturation, independent of motion or respiration. U.S. Pat. No. 5,638,816, which is assigned to the assignee of the current application discloses a technique for inducing an intentional active perturbation of the blood volume of a patient, and is referred to as an “active pulse.” Because peripheral venous oxygen saturation, Sp_o_2 , is a desirable parameter for stereo pulse oximetry applications, it is advantageous to provide for a continuous and controlled pulsatile venous signal.

FIG. 2 depicts an active pulse mechanism used in conjunction with a pulse oximetry sensor. An active pulser 260

physically squeezes or otherwise perturbs a portion of patient tissue 270 in order to periodically induce a “pulse” in the blood at the tissue site 202. A pulser drive 280 generates a periodic electrical signal to a transducer 262 attached to the patient. The transducer 262 creates a mechanical force against the patient tissue 270. For example, the pulser 260 could be a solenoid type device with a plunger that presses against the fleshy tissue to which it is attached. The DSP 150 provides pulse drive control information to a digital to analog converter (DAC) 290 via the control input 291. The DAC output 292 is coupled to the pulser drive 280. This allows the processor to advantageously control the magnitude of the induced pulse, which moderates scattering as described below. The pulser 260 could be a pressure device as described above. Other pressure mechanisms, for example a pressure cuff, could be similarly utilized. Other methods, such as temperature fluctuations or other physiological changes, which physiologically alter a fleshy medium of the body on a periodic basis to modulate blood volume at a nearby tissue site could also be used. Regardless of the active pulse mechanism, this modulated blood volume is radiated by a pulse oximeter sensor and the resulting signal is processed by the signal processing apparatus described below to yield Sp_o_2 .

Signal Processor

FIG. 6 illustrates the processing functions of the digital signal processor (DSP) 150 (FIG. 1A). Each data channel input 152, 154, 158 (FIG. 1A) is operated on by one or more of the front-end processor 610, saturation calculator 620, plethysmograph feature extractor 630 and multiple parameter processor 640 functions of the DSP 150. First, a digitized signal output from the ADC 230 (FIG. 2) is input 602 to the front-end processor 610, which demultiplexes, filters, normalizes and frequency transforms the signal, as described further below. A front-end output 612 provides a red signal spectrum and an IR signal spectrum for each data channel as inputs to the saturation calculator 620. Another front-end output 614 provides a demultiplexed, normalized IR plethysmograph for each data channel as an input to the feature extractor 630. The saturation calculator output 622 provides arterial and venous saturation data for each data channel as input to the multiple parameter processor 640. One feature extractor output 632 provides data on various plethysmograph shape parameters for each data channel as input into the multiple parameter processor 640. Another feature extractor output 634, also coupled to multiple parameter processor 640, provides an indication of plethysmograph quality and acts as a threshold for determining whether to ignore portions of the input signal 602. The multiple parameter processor has a numerical output 642 that provides same-channel Δsat parameters and cross-channel parameters, such as Δsat_{xy} or $\Delta pleth_{xy}$, to a display 180 (FIG. 1A). The numeric output 642 may also provide saturation and plethysmograph parameters directly from the saturation calculator 620 or the feature extractor 630 without further processing other than data buffering. The multiple parameter processor also has a graphical output 644 that provides plethysmograph waveforms for each data channel in addition to graphics, depending on a particular application, the indicate the trend of the numerical parameters described above.

Front-End Processor

FIG. 7 is a functional block diagram of the front-end processor 610 for the stereo pulse oximeter. The digitized sensor output 118 (FIG. 2) is an input signal 602 to a demultiplexer 710, which separates the input signal 602 into a red signal 712 and an infrared signal 714. The separated

red and infrared signals **712**, **714** are each input to a filter **720** to remove unwanted artifacts introduced by the demultiplexing operation. In one embodiment, the filter **720** is a finite-impulse-response, low-pass filter that also “decimates” or reduces the sample rate of the red and infrared signals **712**, **714**. The filtered signals **722** are then each normalized by a series combination of a log function **730** and bandpass filter **740**. The normalized signals, RD(t), IR(t) **742** are coupled to a Fourier transform **750**, which provides red frequency spectrum and infrared frequency spectrum outputs, RD(ω), IR(ω) **612**. A demultiplexed infrared signal output **614** is also provided.

Saturation Calculator

FIG. **8** shows a graph **800** illustrating idealized spectrums of RD(t) and IR(t) **752** (FIG. **7**). The graph has an x-axis **810** that corresponds to the frequency of spectral components in these signals and a y-axis **820** that corresponds to the magnitude of the spectral components. The spectral components are the frequency content of RD(t) and IR(t), which are plethysmograph signals corresponding to the patient's pulsatile blood flow, as described below. Thus, the frequencies shown along the x-axis **810**, i.e. f_0 , f_1 , f_2 , are the fundamental and harmonics of the patient's pulse rate. The spectrum of RD(t), denoted RD(ω) **612** (FIG. **7**), is shown as a series of peaks, comprising a first peak **832** at a fundamental frequency, f_0 , a second peak **842** at a first harmonic, f_1 and a third peak **852** at a second harmonic, f_2 . Similarly, the spectrum of IR(t), denoted IR(ω) **612** (FIG. **7**), is shown as another series of peaks, comprising a first peak **834** at a fundamental frequency, f_0 , a second peak **844** at a first harmonic, f_1 and a third peak **854** at a second harmonic, f_2 . Also shown in FIG. **8** is the ratio of the spectral peaks of RD(t) and IR(t), denoted RD(ω)/IR(ω). This ratio is shown as a first ratio line **838** at the fundamental frequency f_0 , a second ratio line **848** at the first harmonic f_1 , and a third ratio line **858** at the second harmonic f_2 .

The magnitude of these ratio lines RD(ω)/IR(ω) corresponds to the ratio RD/IR defined by equation (2), and, hence, can be used to determine Sp_aO_2 . This can be seen from Parseval's relation for a periodic signal, $x(t)$, having a period T, where X_k is the spectral component at the kth harmonic of $x(t)$:

$$\frac{1}{T} \int_0^T (|x(t)|)^2 dt = \sum_k (|X_k|)^2 \quad (9)$$

Equation (9) relates the energy in one period of the signal $x(t)$ to the sum of the squared magnitudes of the spectral components. The term $|X_k|^2$ can be interpreted as that part of the energy per period contributed by the kth harmonic. In an ideal measurement, the red and infrared signals are the same to within a constant scale factor, which corresponds to the arterial oxygen saturation. Likewise, the red and infrared spectra are also the same to within a constant scale factor. Thus, in an ideal measurement, all of the ratio lines **838**, **848**, **858** have substantially the same amplitude. Any differences in the amplitude of the ratio lines is likely due to motion, scattering or other noise contaminations, as discussed further below. Accordingly, any of the RD(ω)/IR(ω) ratio lines is equivalent to the ratio, RD/IR, of equation (2) and can be used to derive Sp_aO_2 .

One skilled in the art will recognize that the representations in FIG. **8** are idealized. In particular, in actual measured data, especially if contaminated by noise, the frequencies of the peaks of RD(ω) do not correspond exactly to the

frequencies of the peaks of IR(ω). For example, the fundamental frequency, f_0 , found for RD(ω) will often be different from the fundamental frequency, f_0' , found for IR(ω) and similarly for the harmonics of f_0 .

FIG. **9** shows a graph **900** illustrating idealized spectrums RD(ω) and IR(ω) and associated ratio lines measured with an active pulse sensor. The graph **900** has an x-axis **910** that corresponds to the frequency of spectral components in these signals and a y-axis **920** that corresponds to the magnitude of the spectral components. The spectrum, RD(ω), is shown as two series of peaks. One series of peaks **930** occurs at a fundamental frequency, f_{h0} , and associated harmonics, f_{h1} and f_{h2} , of the patient's pulse (heart) rate. Another series of peaks **940** occurs at a fundamental frequency, f_{p0} , and associated harmonics, f_{p1} and f_{p2} , of the active pulse rate. Similarly, the spectrum, IR(ω), is shown as two series of peaks. One series of peaks **950** occurs at a fundamental frequency, f_{h0} , and associated harmonics, f_{h1} and f_{h2} , of the patient's pulse rate. Another series of peaks **960** occurs at a fundamental frequency, f_{p0} , and associated harmonics, f_{p1} and f_{p2} , of the active pulse rate. Accordingly, there are two series of RD/IR ratio lines. One series of ratio lines **970** are at the patient's pulse rate and associated harmonics, and another series of ratio lines **980** are at the active pulser rate and associated harmonics.

Because only the arterial blood is pulsatile at the patient's pulse rate, the ratio lines **970** are only a function of the arterial oxygen saturation. Accordingly, Sp_aO_2 can be derived from the magnitude of these ratio lines **970**, as described above. Further, a modulation level for the active pulse is selected which insignificantly perturbs the arterial blood while providing a measurable venous signal. This is possible because the arterial blood pressure is significantly larger than the venous pressure. The modulation level is regulated as described above with respect to FIG. **2**, i.e. the DSP **150**, via a pulser drive control **291**, sets the magnitude of the pulser drive **280** to the pulse inducing mechanism **262**. Assuming that the active pulse modulation of the arterial blood is insignificant, only the venous blood is pulsatile at the active pulser rate. Hence, the ratio lines **980** are only a function of the venous oxygen saturation. Accordingly, Sp_aO_2 can be derived from the magnitude of the pulse rate related ratio lines **980** in the same manner as Sp_aO_2 is derived from the magnitude of the pulse rate related ratio lines.

Scattering

Propagation of optical radiation through tissue is affected by absorption and scattering processes. The operation of pulse oximeters was described qualitatively above using an analysis based on the Beer-Lambert law of absorption, equation (3). This approach, however, fails to account for the secondary effects of light scattering at pulse oximeter wavelengths. The primary light scatterer in blood is erythrocytes, i.e. red blood cells. A qualitative understanding of the effects of scattering on pulse oximetry is aided by a description of red blood cell properties within flowing blood.

Human blood is a suspension of cells in an aqueous solution. The cellular contents are essentially all red blood cells, with white cells making up less than 1/600th of the total cellular volume and platelets less than 1/800th of the total cellular volume. Normally the hematocrit, which is the percentage of the total volume of blood occupied by cells, is about 50% in large vessels and 25% in small arterioles or venules.

Red blood cells are extremely deformable, taking on various shapes in response to the hydrodynamic stresses created by flowing blood. For example, assuming a laminar

blood flow within a vessel, a parabolic velocity profile exists that is greatest in the vessel center and smallest along the vessel walls. Nominally, red blood cells are shaped as biconcave disks with a diameter of 7.6 μm and thickness of 2.8 μm . Exposed to this velocity profile, the red blood cells become parachute-shaped and aligned in the direction of the blood flow. Thus, during systole, transmitted light is scattered by aligned, parachute-shaped cells. During diastole, the light is scattered by biconcave disks having a more or less random alignment.

The time-varying shape and alignment of the red blood cells can have a significant effect on measured values of oxygen saturation if scattering is ignored. Analogous to the analysis using the Beer-Lambert absorption law, scattering can be qualitatively understood as a function of the scattering coefficients of various tissues. Specifically, the bulk scattering coefficient can be written as:

$$\mu_s = V_b \mu_{sb} + V_t \mu_{st} \quad (10)$$

where V_b is the blood volume, μ_{sb} is the scattering coefficient of blood, V_t is the surrounding tissue volume and μ_{st} is the scattering coefficient of the surrounding tissue. The volume, V_t , and scattering coefficient, μ_{st} , of the surrounding tissue are time invariant. The blood volume, V_b , however, is pulsatile. The ratio of ratios computation, RD/IR, results in normalization of the time invariant or DC tissue absorption and cancellation of the time varying or AC pulsatile blood volume absorption to yield a number related to oxygen saturation. This computational approach is valid because the absorption coefficients of blood, $\epsilon_{HbO_2, \lambda}$, $\epsilon_{Hb, \lambda}$, given in equation (4) were assumed to change only slowly over time. The scattering coefficient of blood μ_{sb} , however, is time variant. As described above, this variation is due to the time-varying alignment and shape of the red blood cells. This time variation in the detected intensity of light transmitted through a tissue site is not normalized or canceled by the RD/IR calculation. Further, because the magnitude of the scattering coefficient variations is a function of blood flow, these variations become more pronounced with larger pulses in the blood supply. As a result, scattering produces frequency-dependent magnitude variations in the ratio lines RD(ω)/IR(ω).

FIG. 9 illustrates the effect of scattering on the spectra of the detected red and infrared intensity waveforms. When these waveforms are transformed into the frequency domain, the time varying component of scattering manifests itself as spreads **978**, **988** in the RD/IR ratio lines at each harmonic of the plethysmograph or active pulse rate. The magnitude of the ratio lines **970** at the fundamental and harmonics of the patient's pulse rate varies between a minimum **972** and a maximum **974**, resulting in a magnitude spread **978**. Similarly, the magnitude of the ratio lines **980** at the fundamental and harmonics of the active pulse rate varies between a minimum **982** and a maximum **984**, resulting in a magnitude spread **988**. Normally, absent motion artifact or noise contamination, the spread **978**, **988** in the ratio lines is quiet small, but the magnitude of these spreads **978**, **988**, increases with larger blood flows or pulse magnitudes. Scattering attributable to an active pulse can be regulated by adjusting the magnitude of the active pulse modulation based upon the amount of spread **978**, **988** of the ratio line magnitudes. Thus, the active pulse magnitude can be increased to obtain a larger detected AC signal, but limited to below the point at which scattering becomes significant.

FIG. 10 depicts an embodiment of the signal processing for determining oxygen saturation from the ratio lines of RD(ω)/RD(ω). The red spectrum RD(ω) **612** and infrared

spectrum IR(ω) **612**, computed as described above with respect to FIG. 7, are input to a peak detector **1010**. The peak detector **1010** separately calculates localized maximums for RD(ω) and IR(ω). The peak detector output **1012** is a series of frequencies corresponding to the patient pulse rate fundamental and harmonics. If an active pulse is used, the peak detector output **1012** is also a series of frequencies corresponding to the active pulse rate. Although the active pulse rate is known, the detected peaks may have been shifted due to noise, motion artifact or other signal contamination. The peak detector output **1012** is coupled to a series combination of peak matcher **1020** and ratio line calculator **1030**. The ratio lines RD/IR are calculated by matching the frequency peaks of RD(ω) with the nearest frequency peaks of IR(ω). The ratio lines associated with the pulse rate harmonics **1032** are then separated into a different set from the ratio lines associated with the active pulse harmonics **1034**, assuming an active pulse is utilized. An average ratio line for each set **1032**, **1034** is calculated by averaging **1060** all ratio lines in a set. The magnitude of the average ratio line **r 1062** for the pulse rate set **1032** is then fed to a look-up table (LUT) **1090**, which provides an output **622** of the measured value of Sp_aO_2 . Similarly, if an active pulse is used, the magnitude of the average ratio line μ **1064** for the active pulse rate set **1034** is then fed to a LUT **1090**, which provides an output **622** of the measured value of Sp_vO_2 . A scattering detector **1080** computes the spread **988** (FIG. 9) in the set of ratio lines associated with the active pulse and provides this value **1082** to the DSP **150** (FIG. 2) so that the DSP can set the pulser drive control **291** (FIG. 2) to regulate the magnitude of the active pulse.

Alternatively, Sp_vO_2 may be measured from respiration-induced pulses in the venous blood, described above, without utilizing an active pulse sensor. Specifically, a series of ratio lines **980** (FIG. 9) would occur at a fundamental frequency, f_{r0} , and associated harmonics, f_{r1} and f_{r2} , of the respiration rate, which is either known from the ventilator frequency or derived from a separate measurement of the natural respiration. As shown in FIG. 10, the ratio lines associated with the respiration rate harmonics **1034** are then separated into a different set from the ratio lines associated with the pulse rate harmonics **1032**. An average ratio line for the respiration rate set **1034** is calculated by averaging **1060** all ratio lines in that set. The magnitude of the average ratio line μ **1064** for the respiration rate set **1034** is then fed to a look-up table (LUT) **1090**, which provides an output **622** of the measured value of Sp_vO_2 .

Plethysmograph Feature Extractor

FIG. 11 illustrates the standard plethysmograph waveform **1100**, which can be derived from a pulse oximeter. The waveform **1100** is a visualization of blood volume change in the illuminated peripheral tissue caused by arterial blood flow, shown along the y-axis **1110**, over time, shown along the x-axis **1120**. The shape of the plethysmograph waveform **1100** is a function of heart stroke volume, pressure gradient, arterial elasticity and peripheral resistance. The ideal waveform **1100** displays a broad peripheral flow curve, with a short, steep inflow phase **1130** followed by a 3 to 4 times longer outflow phase **1140**. The inflow phase **1130** is the result of tissue distention by the rapid blood volume inflow during ventricular systole. During the outflow phase **1140**, blood flow continues into the vascular bed during diastole. The end diastolic baseline **1150** indicates the minimum basal tissue perfusion. During the outflow phase **1140** is a dicrotic notch **1160**, the nature of which is disputed. Classically, the dicrotic notch **1160** is attributed to closure of the aortic valve at the end of ventricular systole. However, it may also be the

result of reflection from the periphery of an initial, fast propagating, pressure pulse that occurs upon the opening of the aortic valve and that precedes the arterial flow wave. A double dicrotic notch can sometimes be observed, although its explanation is obscure, possibly the result of reflections reaching the sensor at different times.

FIG. 12 is a graph 1200 illustrating the absorption of light at a tissue site illuminated by a pulse oximetry sensor. The graph 1200 has a y-axis 1210 representing the total amount of light absorbed the tissue site, with time shown along an x-axis 1220. The total absorption is represented by layers including the static absorption layers due to tissue 1230, venous blood 1240 and a baseline of arterial blood 1250. Also shown is a variable absorption layer due to the pulse-added volume of arterial blood 1260. The profile 1270 of the pulse-added arterial blood 1260 is seen as the plethysmograph waveform 1100 depicted in FIG. 11.

FIG. 13 illustrates the photoplethysmograph intensity signal 1300 detected by a pulse oximeter sensor. A pulse oximeter does not directly detect absorption, and hence does not directly measure the standard plethysmograph waveform 1100 (FIG. 11). However, the standard plethysmograph can be derived by observing that the detected intensity signal 1300 is merely an out of phase version of the absorption profile 1270. That is, the peak detected intensity 1372 occurs at minimum absorption 1272 (FIG. 12), and minimum detected intensity 1374 occurs at maximum absorption 1274 (FIG. 12). Further, a rapid rise in absorption 1276 (FIG. 12) during the inflow phase of the plethysmograph is reflected in a rapid decline 1376 in intensity, and the gradual decline 1278 (FIG. 12) in absorption during the outflow phase of the plethysmograph is reflected in a gradual increase 1378 in detected intensity.

FIG. 14 illustrates the digital signal processing for plethysmograph feature extraction 630 (FIG. 6). The input 614 is the IR signal output from the demultiplexer 710 (FIG. 7). This signal is shifted into a first-in, first-out (FIFO) buffer, which allows fixed-length portions of the input signal 614 to be processed for feature extraction. The buffered output signal 1412 is coupled to a shape detector 1420, slope calculator 1430, feature width calculator 1440 and a notch locator 1450, which perform the core feature extraction functions. The shape detector 1420 determines if a particular buffered signal portion 1412 contains specific gross features, such as a peak, a valley, an upward slope, a downward slope, a dicrotic notch or a multiple dicrotic notch. A detected shape output 1422 containing one or more flags indicating the gross feature content of the current signal portion 1412 is coupled to the other feature extraction functions 1430, 1440, 1450 and to the waveform quality determination functions 1460, 1470, 1480. A slope calculator 1430 determines the amount of positive or negative slope in the signal portion 1412 if the shape detector output 1422 indicates a slope is present. The output slope value 1432 is coupled to the waveform quality functions 1460, 1470, 1480 in addition to the feature extraction output 632. A feature calculator 1440 quantifies a feature in one or more signal portions 1412 specified by the shape detector 1420, such as the magnitude, the area under, or the width of a peak or notch. The feature calculator output 1442 is a code indicating the feature and its value, which is coupled to the feature extraction output 632. A feature locator 1450 quantifies the time of occurrence of one or more features of a signal portion 1412 as specified by the shape detector 1420. The feature locator output 1452, which is coupled to the feature extraction output 632, is a code indicating a feature and an associated code indicating time of occurrence in reference to a particular epoch. The

feature locator output 1452 allows a determination of the relative location of plethysmograph features in addition to a phase comparison of plethysmographs derived from two or more tissue sites. Another feature extraction output 634, which is coupled to the multiple parameter processor 640 (FIG. 6), provides an indication of waveform quality. Input signals portions 1412 not having either a sharp downward edge 1460, a symmetrical peak 1470 or a gradual decline 1480 are not processed further.

Multiple Parameter Processor

FIG. 15 illustrates the multiple parameter processing portion 640 (FIG. 6) of the signal processing. A differencing function 1510 has as inputs a first saturation value, Sp_1O_2 , and a second saturation value, Sp_2O_2 , 622. The saturation input values 622 can be arterial and venous saturation values from a single data channel, arterial saturation values from two different data channels or venous saturation values from two different data channels. The differences of the saturation value inputs 622 are provided as an output 1514, which is coupled to a saturation data memory 1520. The saturation values 622 are also directly coupled to the saturation data memory 1520. The memory 1520 stores a record of saturation values, SpO_2 , for each channel, delta saturation values, Δsat , for each channel and cross-channel delta saturation values, Δsat_{xy} , as required for a particular application. A flow calculator 1530 utilizes a plethysmograph input 614 or a bio-impedance probe input 1534 to provide a flow value 1538, which is also coupled to the saturation data memory 1520. For example, the flow value 1538 may be a perfusion index, PI, defined as follows:

$$PI = \frac{IR_{max} - IR_{min}}{IR_{DC}} \quad (11)$$

where IR_{max} is the maximum value, IR_{min} is the minimum value, and IR_{DC} is the average value of the IR plethysmograph signal 614 (FIG. 7).

The saturation data memory 1520 provides a buffered output 1522 that is coupled to a numerical display driver 1540. The numerical display driver 1540 provides an output 642 to a standard display, such as LED or LCD numerical display modules or a CRT monitor. The memory output 1522 is also coupled to a saturation data analyzer 1530, one function of which calculates a long-term trend of the values in memory 1520. For example, the saturation data analyzer may average a saturation value over time, or provide samples of the saturation values taken at regular time intervals. The output 1532 can either be numerical, which is coupled to the numerical display driver 1540, or graphical, which is coupled to the graphical display driver 1570. The graphical display driver 1570 provides an output 644 to a standard graphical display device, such as LED or LCD graphical display modules or a CRT monitor.

A pleth data memory 1550 has as inputs the IR plethysmograph signals 614 (FIG. 7) from each data channel and the associated extracted features 632 (FIG. 14). The memory 1550 also has an input indicating waveform quality 634 (FIG. 14). The pleth memory 1550 provides a buffered output 1558 that is coupled to the graphical display driver 1570, allowing display of the plethysmograph waveforms for each data channel. The memory output 1558 is also coupled to a pleth data analyzer 1560, one function of which calculates a long-term trend of the plethysmograph and shape parameters in pleth memory 1520. For example, the pleth data analyzer 1560 may provide an average of par-

ticular shape parameters over time. As another example, the pleth data analyzer **1560** may provide a graphic showing an accumulation of many overlaid plethysmographs. The output **1562** can either be numerical, which is coupled to the numerical display driver **1540**, or graphical, which is coupled to the graphical display driver **1570**.

Another function of the saturation data analyzer **1530** and the pleth data analyzer **1560** is to compare oxygen status and plethysmograph parameters derived from multiple sites in order to isolate noise artifacts and to derive a more accurate estimate of these parameters. For example, it is unlikely that motion artifact will affect each peripheral site in the same manner. If the quality input **634** indicates a noisy plethysmograph for one channel during a particular time period, the pleth data analyzer **1560** can exchange this information **1565** with the saturation data analyzer **1530**. The saturation data analyzer **1530** can then ignore the saturation data for that channel for that time period in lieu of saturation data from another channel. In a similar fashion, noisy data from multiple channels can be averaged, correlated or otherwise processed to provide an estimate of Sp_aO_2 , Sp_vO_2 or pulse rate, or to provide a plethysmograph that is more accurate than can be derived from a single data channel.

FIG. **16A** illustrates detail of a single-site display screen **180** for the stereo pulse oximeter. The display has a numerical display portion **1610** controlled by the numerical display driver **1540** (FIG. **15**) and a graphical display portion **1660** controlled by the graphical display driver **1570** (FIG. **15**). The numerical display portion **1610** displays a value for Sp_aO_2 **1620**, Sp_vO_2 **1630** and pulse rate **1640** for a particular tissue site. The graphical display portion **1660** displays a plethysmograph **1662** for the corresponding tissue site, which can be displayed as a single waveform or an accumulated multiple of overlaid waveforms that may reveal a waveform trend. A push button or menu selection allows the user to switch to a display of data from any single one of the multiple tissue sites to which a sensor is attached.

FIG. **16B** illustrates detail of a multi-site display screen **180** for the stereo pulse oximeter. The numerical display portion **1610** displays a value for Sp_aO_2 **1622** and Sp_vO_2 **1632** for a first tissue site. Also displayed is a value for Sp_aO_2 **1624** and Sp_vO_2 **1634** for a second tissue site. In addition, a value for pulse rate **1642** derived from either the first or second tissue site, or both, is displayed. The graphical display portion **1660** displays a first plethysmograph **1664** and a second plethysmograph **1666** corresponding to the first and second tissue sites, respectively. A push button, menu selection allows the user to manually switch between the single site display (FIG. **16A**) and the multi-site display (FIG. **16B**). Also, a triggering event, such as an alarm based on multiple-site oxygen status parameters, causes the display to automatically switch from the single-site display to the multi-site display, enabling the user better view the conditions that caused the triggering event.

One of ordinary skill will appreciate many display screens variations from those shown in FIGS. **16A** and **16B** that are within the scope of this invention. For example, the stereo pulse oximeter could be configured to provide several push button or menu selectable display screens. One display screen might display more than two channels of oxygen status data. Another display screen could display cross-channel parameters such as Δsat_{xy} , or a comparison of plethysmograph shape parameters from two channels. One of ordinary skill will also appreciate many variations and

modifications of layout and design for the graphical and numerical displays within the scope of this invention.

Stereo Pulse Oximetry Applications

Oxygen Titration

Oxygen is one of the most commonly used drugs in an intensive care unit and is an integral part of all respiratory support. The goal of oxygen therapy is to achieve adequate delivery of oxygen to the tissues without creating oxygen toxicity. Too little oxygen results in organ damage and, in particular, brain damage. Too much oxygen can result in, for example, pulmonary edema and, in neonates, retinopathy of prematurity (ROP). Infants receiving oxygen therapy, in particular, must have inspired oxygen concentration and blood oxygen levels monitored closely.

Oxygen titration in neonates is currently accomplished with either transcutaneous monitoring or monitoring with a conventional pulse oximeter. As mentioned above, transcutaneous monitoring involves the placement of a heated Clark electrode against the skin surface. The electrode is secured to the skin surface with an airtight seal to eliminate contamination by room air gases. The skin surface beneath the electrode is then heated, which opens pre-capillary sphincters allowing localized arteriolar blood flow beneath the sensor. The so-called T_cO_2 value that is measured correlates well with P_aO_2 . However, there are several drawbacks to this approach. Because the skin surface must be heated, a fifteen minute elapsed time after application is necessary before stable readings are acquired. Further, the required temperature is 43-45° C. (110° F.), with an associated risk of burns. In addition, titration is often accomplished by simply maintaining T_cO_2 within acceptable limits for this parameter, e.g. an equivalent P_aO_2 of 50-80 mm Hg for neonates. However, P_aO_2 alone does not provide an indication of balance between inspired oxygen and the rate of tissue oxygen consumption. If the patient is particularly anemic or hypovolemic, has an abnormal hemoglobin, or a small cardiac output, then oxygen delivery may be inadequate even in the presence of a normal P_aO_2 . Titration with a conventional pulse oximeter is similarly accomplished by maintaining Sp_aO_2 within acceptable limits, which also fails to consider tissue oxygen consumption.

Oxygen titration can be more adequately monitored with a continuous indication of oxygen consumption, which is equal to oxygen delivery according to Fick's algorithm, as noted above. Further, continuous monitoring of oxygen consumption at a peripheral tissue site, although not necessarily indicative of overall oxygen consumption, may be indicative of an oxygen supply dependency. A measure of peripheral oxygen consumption can be expressed in terms of $\Delta sat = Sp_aO_2 - Sp_vO_2$ and perfusion, which, as noted above, are parameters advantageously provided by the stereo pulse oximeter according to the present invention. Oxygen consumption at a peripheral site is obtained by multiplying the difference between peripheral arterial and venous oxygen content by perfusion at the site.

$$VpO_2 = [O_2 \text{ content (arterial)} - O_2 \text{ content (venous)}] \Phi \quad (12)$$

where oxygen content is measured in milliliters (ml) of O_2 per deciliters (dl) of blood and Φ denotes perfusion in deciliters per minute. Oxygen content, however, can be expressed in terms of the amount of oxygen bound to the hemoglobin plus the amount of oxygen dissolved in the plasma. The amount of bound oxygen is equal to the hemoglobin concentration, C_{hb} , in grams per deciliter of blood, times the hemoglobin carrying capacity, which is 1.34 milliliters of O_2 per gram of hemoglobin times the hemoglobin oxygen saturation, SO_2 . The amount of dissolved

oxygen is simply the partial pressure of oxygen, PO_2 , times the O_2 solubility coefficient in blood, which is 0.003 milliliters of O_2 per deciliter. The sum of these two terms yields:

$$O_2 \text{ content} = 1.34C_{Hb}SO_2 + 0.003PO_2 \quad (13)$$

Substituting equation (13) into equation (12) yields the following equation for tissue oxygen consumption:

$$VpO_2 = [1.34C_{Hb}(Sp_aO_2 - Sp_vO_2) + 0.003(P_aO_2 - P_vO_2)]\Phi \quad (14)$$

Except when the fractional inspired oxygen, FiO_2 , is high, blood plasma plays a minimal role in oxygen delivery. Thus, peripheral oxygen consumption is approximately:

$$VpO_2 = [1.34C_{Hb}\Delta sat]\Phi \quad (15)$$

In order to illustrate a schema of oxygen titration, it is convenient to characterize the relationship between oxygen supplied at the airway to oxygen consumed at a peripheral tissue site. Specifically, characterization of the relationship between Δsat , Φ and FiO_2 is useful. Assuming constant oxygen consumption at the tissue site, equation (15) is:

$$\Delta sat \Phi = \text{constant} \quad (16)$$

Equation (16) has a simple analog in electronic circuits, i.e. a variable resistor across a current or voltage source adjusted to maintain constant power. In this analog circuit, the current through the resistor, I , is equivalent to perfusion, the voltage across the resistor, V , is equivalent to Δsat and the constant of equation (16) is equivalent to the constant power, P , consumed by the resistor. The equation representing this electrical analog is:

$$V \times I = P \quad (17)$$

FIG. 17A shows a graph 1701 that depicts a family of curves each corresponding to different values of P in equation (17). The graph 1701 has an x-axis 1710 indicating current, I , and a y-axis 1720 indicating voltage, V . A first curve 1730 shows V versus I for a constant power, P , of 0.5 watts; a second curve 1740 shows V versus I for a constant P of 1 watt; and a third curve 1750 shows V versus I for a constant P of 2 watts. Using the analogy between equations (16) and equation (17), whenever Φ (current) is small, the Δsat (voltage) is large and vice-a-versa. Also, a change in consumption (power) causes a shift in the curve along with a change in its curvature. That is, if the body suddenly changes its metabolic rate at the peripheral tissue site, the curve will accordingly shift up or shift down and will change its shape. Equation (16) and the analogous constant consumption curves of FIG. 17A assume a supply independent condition, i.e. that peripheral oxygen consumption is satisfied by peripheral oxygen delivery. If the peripheral tissue site is starved for oxygen, then the locus of points for Δsat versus Φ is quite different from a hyperbola. The amount of tissue oxygen extraction is at a maximum and is independent of Φ . Accordingly Δsat is at a maximum and independent of Φ . The above analysis provides insight into the relationship between Δsat and Φ . The relationship between Δsat and FiO_2 can also be characterized.

FIG. 17B shows a graph 1702 of saturation along a y-axis 1760 and fractional inspired oxygen along an x-axis 1770. A curve of Sp_aO_2 1780 and a curve of Sp_vO_2 1790 are depicted versus FiO_2 . The difference between these curves 1780, 1790 yields Δsat 1785 versus FiO_2 . When FiO_2 is zero 1772, oxygen saturation and, hence, both Sp_aO_2 1780 and Sp_vO_2 1790 are zero. As FiO_2 is increased, Sp_aO_2 1780 also increases until virtually reaching 100 percent saturation 1762. As FiO_2 increases further, Sp_aO_2 1780 stays at virtually 100 percent saturation 1762. As FiO_2 is increased from

zero 1772, Sp_vO_2 1790 also increases. In this low FiO_2 region 1774, the peripheral tissue site is supply dependent and Δsat 1785 also increases. At a certain point, the tissue site oxygen demand is met by supply. In this supply independent region 1776, oxygen consumption is constant and equation (16) is valid. Also, Δsat 1785 is at a constant maximum, which is a function of the metabolism at the tissue site. As FiO_2 increases further, eventually the partial pressure of oxygen becomes significant and the second term of equation (14) must be considered. In this high FiO_2 region 1778, Δsat 1785 decreases because some of the tissue oxygen consumption is supplied by oxygen dissolved in the plasma.

FIG. 17C shows a graph 1704 of saturation difference along a y-axis 1764 and fractional inspired oxygen along an x-axis 1770. A curve of Δsat 1786 is depicted versus FiO_2 , corresponding to the region Δsat 1785 depicted in FIG. 17B. The curve 1786 has a first deflection point 1766 occurring at the transition between the low FiO_2 region 1774 (FIG. 17B) and the supply independent region 1776 (FIG. 17B). The curve 1786 also has a second deflection point 1768 occurring at the transition between the supply independent region 1776 (FIG. 17B) and the high FiO_2 region 1778 (FIG. 17B). The curve 1786 illustrates how the trend for Δsat , as measured by the stereo pulse oximeter, can be used to accurately titrate oxygen. The goal of oxygen titration is to supply sufficient oxygen to supply tissue demand and avoid unnecessarily high amounts of FiO_2 . Thus, the Δsat parameter should be monitored so that FiO_2 is adjusted between the two deflection points 1766, 1768. For neonates, FiO_2 should be adjusted just beyond the first deflection point 1766. For adults, FiO_2 should be adjusted just before the second deflection point 1768.

FIG. 18 illustrates a graph having a three-dimensional surface 1800 generally depicting the relationship between Δsat , Φ and FiO_2 from the combined graphs of FIGS. 17A and 17C. The graph has an x-axis 1810 showing FiO_2 , a y-axis 1820 showing Φ and a z-axis 1830 showing Δsat . The surface 1800 has a supply dependent region 1840, a perfusion-limited region 1850, a constant consumption region 1860 and a plasma dependent region 1870. The surface describes the oxygen status of a peripheral tissue site. The supply dependent region 1840 corresponds to the low FiO_2 region 1774 (FIG. 17B) described above. That is, inspired oxygen into the lungs is so low that, at the tissue site, oxygen extraction by the tissues is limited by oxygen delivery, and Δsat falls rapidly as FiO_2 is reduced. The perfusion-limited region 1850 along the x-axis 1810 represents a low perfusion state where equation (16) is not valid. That is, perfusion at the tissue site is so low that oxygen extraction by the tissues is at a maximum, and, hence, Δsat is at a maximum and is independent of FiO_2 . A cross-section of the surface taken parallel to the y-axis 1820 yields a hyperbole-shaped constant consumption region 1860, consistent with the constant metabolic rate curves illustrated above with respect to FIG. 17A. The plasma dependent region 1870 corresponds to the high FiO_2 region 1778 (FIG. 17B) described above. That is, inspired oxygen into the lungs is so high that the tissue site is partially dependent on oxygen dissolved in the plasma. The surface 1800 illustrates that perfusion should be monitored simultaneously with Δsat to avoid the perfusion-limited region 1850, where Δsat is an unresponsive indicator of FiO_2 , and to avoid misinterpreting hyperbolic changes in Δsat that result from changes in perfusion.

Persistent Pulmonary Hypertension in Neonates

FIG. 19 illustrates the heart/lung circulation of a hypertensive neonate. Persistent Pulmonary Hypertension in Neo-

nates (PPHN) is a neonatal condition with persistent elevation of pulmonary vascular resistance and pulmonary artery pressure. Shown is a neonatal heart **1902** and a portion of a neonatal lung **1904**. The pulmonary artery **1910** that normally feeds oxygen depleted "blue" blood from the right ventricle **1920** to the lung **1904** is constricted. The back pressure from the constricted artery **1910** results in a right-to-left shunting of this oxygen depleted blood through the ductus arteriosus **1930**, causing it to mix with oxygen rich "red" blood flowing through the descending aorta **1940**. PPHN treatment options include vasodilators, such as nitric oxide (NO). Inhaled exogenous NO causes a dose-dependent decrease in pulmonary artery pressure and pulmonary vascular resistance, as well as a parallel increase in pulmonary blood flow, without affecting systemic arterial pressure. However, the response to NO therapy is a function of the cause of the PPHN as well as the time elapsed before initiation of therapy. Potential toxic effects of NO dictate the proper titration of NO gas. Too little NO may not effectively relieve pulmonary hypertension, and too much NO may cause cellular injury or toxicity. NO therapy is currently monitored using intermittent ultrasound imaging and/or in vitro blood gas measurements. The drawbacks to these techniques are noncontinuous monitoring and disturbances to the neonate that can exacerbate or not reflect the hypertension in the non-disturbed state.

The stereo pulse oximeter according to the present invention allows noninvasive, continuous monitoring of a neonate for detection and managed treatment of PPHN that does not disturb the patient. A right hand sensor **130** (FIG. 1) provides arterial oxygen saturation and a plethysmograph for blood circulating from the left ventricle **1950** through the innominate artery **1960**, which supplies the right subclavian artery. Because the innominate artery **1960** is upstream from the shunt at the ductus arteriosus **1930**, the oxygen saturation value and plethysmograph waveform obtained from the right hand are relatively unaffected by the shunt and serve as a baseline or reference for comparison with readings from other tissue sites. Alternatively, a reference sensor can be placed on a facial site, such as an ear, the nose or the lips. These sites provide arterial oxygen saturation and a plethysmograph for blood circulating from the left ventricle **1950** to the innominate artery **1960**, which supplies the right common carotid artery (not shown), or to the left common carotid artery **1965**.

A foot sensor **120** (FIG. 1) provides oxygen status for blood supplied from the descending aorta **1940**. The shunt **1930** affects both the oxygen saturation and the blood flow in the descending aorta **1940**. As stated above, the shunt **1930** causes oxygen-depleted blood to be mixed with oxygen-rich blood in the descending aorta **1940**. Because the descending aorta **1940** supplies blood to the legs, the oxygen saturation readings at the foot will be lowered accordingly. The PPHN condition, therefore, is manifested as a higher arterial oxygen saturation at the right hand reference site and a lower saturation at the foot site.

The shunt also allows a transitory left to right flow during systole, which distends the main pulmonary artery **1980** as the result of the blood flow pressure at one end from the right ventricle and at the other end from the aortic arch **1990**. A left-to-right flow through the shunt **1930** into the distended artery **1980** alters the flow in the descending aorta **1940** and, as a result, the plethysmograph features measured at the foot. The PPHN condition, therefore, also is manifested as a plethysmograph with a narrow peak and possibly a well-defined dirotic notch at the left hand baseline site and a broadened peak and possibly no notch at the foot site.

An optional left hand sensor **110** (FIG. 1) provides oxygen status for blood circulating from the left ventricle through the left subclavian artery **1970** that supplies the left arm. Because the left subclavian artery **1970** is nearer the shunt **1930** than the further upstream innominate artery **1960**, it may experience some mixing of deoxygenated blood and an alteration in flow due to the shunt **1930**. The PPHN condition, therefore, may also be manifested as a reduced saturation and an altered plethysmograph waveform at the left hand site as compared with the right hand baseline site, although to a lesser degree than with a foot site. Thus, the PPHN condition can be detected and its treatment monitored from Δ sat and plethysmograph morphology comparisons between a right hand baseline sensor site and one or more other sites, such as the left hand or foot.

Patent Ductus Arteriosus

FIG. 20 illustrates the fetal heart/lung circulation. Shown is a fetal heart **2002** and a portion of a fetal lung **2004**. The lung **2004** is non-functional and fluid-filled. Instead, oxygenated blood is supplied to the fetus from gas-exchange in the placenta with the mother's blood supply. Specifically, oxygenated blood flows from the placenta, through the umbilical vein **2006** and into the right atrium **2022**. There, it flows via the foramen **2024** into the left atrium **2052**, where it is pumped into the left ventricle **2050** and then into the aortic trunk **2092**. Also, oxygenated blood is pumped from the right atrium **2022** into the right ventricle **2020** and directly into the descending aorta **2040** via the main pulmonary artery **2080** and the ductus arteriosus **2030**. Normally, the ductus arteriosus **2030** is only open (patent) during fetal life and the first 12 to 24 hours of life in term infants. The purpose of the ductus arteriosus **2030** is to shunt blood pumped by the right ventricle **2020** past the constricted pulmonary circulation **2010** and into the aorta **2040**.

FIG. 21 illustrates a neonatal heart **2002** with a patent ductus arteriosus **2030**. The ductus arteriosus frequently fails to close in premature infants, allowing left-to-right shunting, i.e. oxygenated "red" blood flows from the aorta **2040** to the now unobstructed pulmonary artery **2010** and recirculates through the lungs **2004**. A persistent patent ductus arteriosus (PDA) results in pulmonary hyperperfusion and an enlarged right ventricle **2020**, which leads to a variety of abnormal respiratory, cardiac and genitourinary symptoms. Current PDA diagnosis involves physical examination, chest x-ray, blood gas analysis, echocardiogram, or a combination of the above. For example, large PDAs may be associated with a soft, long, low-frequency murmur detectable with a stethoscope. As another example, two-dimensional, color Doppler echocardiography may show a retrograde flow from the ductus arteriosus **2030** into the main pulmonary artery **2080**. Once a problematic PDA is detected, closure can be effected medically with indomethacin or ibuprofen or surgically by ligation. Multiple doses of indomethacin are commonplace but can still result in patency, demanding ligation. A drawback to current diagnostic techniques is that clinical symptoms of a PDA can vary on an hourly basis, requiring extended and inherently intermittent testing.

The stereo pulse oximeter according to the present invention allows for continuous evaluation of PDA symptoms using non-invasive techniques. A right hand sensor **130** (FIG. 1) provides arterial oxygen saturation and a plethysmograph for blood circulating from the left ventricle **2050** through the innominate artery **2160**, which supplies the right subclavian artery leading to the right arm. Because the innominate artery **2160** is upstream from the shunt at the ductus arteriosus **2030**, the oxygen saturation value and

plethysmograph waveform obtained from the right hand are relatively unaffected by the shunt and serve as a baseline for comparison with readings from other tissue sites.

A foot sensor **120** (FIG. 1) provides oxygen status for blood supplied from the descending aorta **2040**. Unlike a PPHN condition, the shunt **2030** does not affect oxygen saturation in the descending aorta **2040**, because the relatively low pressure in the pulmonary artery **2010** does not allow a mixing of deoxygenated blood into the relatively high pressure flow of oxygenated blood in the aorta **2040**. However, like a PPHN condition, the shunt **2030** does affect the aortic flow. In particular, the shunt allows a transitory left-to-right flow during systole from the high pressure aorta **2040** to the low pressure pulmonary circulation **2010**. This left-to-right flow through the shunt **1930** alters the flow in the descending aorta **1940** and, as a result, the plethysmograph features measured at the foot. The PDA condition, therefore, is manifested as a normal plethysmograph with a characteristically narrow peak and well-defined dicrotic notch at the right-hand baseline site compared with a damped plethysmograph with a broadened peak and reduced or missing notch at the foot site. Further, the foot site waveform is phase shifted from the baseline waveform. These plethysmograph differences are accompanied by comparable arterial oxygen saturation values between the right-hand site and the foot site.

An optional left hand sensor **110** (FIG. 1) provides oxygen status for blood circulating from the left ventricle through the left subclavian artery **2170** that supplies the left arm. Because the left subclavian artery **2170** is nearer the shunt **2030** than the further upstream innominate artery **2160**, it may experience some alteration in flow due to the shunt **2030**. The PDA condition, therefore, may also be manifested as an altered plethysmograph waveform at a left hand site as compared with the right hand baseline site, although to a lesser degree than with a foot site. Thus, the PDA condition can be detected and its treatment monitored from $\Delta\text{sat}_{xy} \approx 0$ and plethysmograph morphology and phase comparisons between a right hand baseline sensor site and one or more other sites, such as the left hand or foot. One of ordinary skill will recognize that multiple site comparisons using the stereo pulse oximeter of the current invention may also be used to detect other cardiac abnormalities that cause mixing of oxygenated and deoxygenated blood, such as a ventricular hole or a patent foramen. Further, abnormal mixing of oxygenated and deoxygenated blood may also be manifested in measurements provided by the stereo oximeters other than Δsat_{xy} and Δpleth_{xy} as described above. For example, an inversion in Δsat at a particular tissue site, i.e., Sp_aO_2 being larger than Sp_tO_2 at that site, would indicate such an abnormal condition.

Aortic Coarctation

Coarctation of the aorta is a congenital cardiac anomaly in which obstruction or narrowing occurs in the distal aortic arch or proximal descending aorta. It occurs as either an isolated lesion or coexisting with a variety of other congenital cardiac anomalies, such as a PDA. If the constriction is preductal, lower-trunk blood flow is supplied predominantly by the right ventricle via the ductus arteriosus, and cyanosis, i.e. poorly oxygenated blood, is present distal to the coarctation. This can be detected by the stereo pulse oximeter from a comparison of Sp_aO_2 between an upper body and a lower body site. If the constriction is postductal, blood supply to the lower trunk is supplied via the ascending aorta. Differential plethysmographs between the upper and lower extremities may not exist if the ductus is widely patent. If the ductus closes, however, this condition can be detected by the

stereo pulse oximeter as a reduced amplitude and phase delay between the plethysmographs measured at a lower body site with respect to an upper body site.

The stereo pulse oximeter has been disclosed in detail in connection with various embodiments of the present invention. These embodiments are disclosed by way of examples only and are not to limit the scope of the present invention, which is defined by the claims that follow. One of ordinary skill in the art will appreciate many variations and modifications within the scope of this invention.

What is claimed is:

1. A method for determining a congenital cardiac anomaly in an infant, the method comprising:

using a pulse oximeter to determine a first oxygen saturation measurement from a first tissue site on a first limb of a patient;

using the pulse oximeter to determine a second oxygen saturation measurement from at least one additional tissue site on a second limb of the patient;

automatically comparing said first oxygen saturation measurement to said second oxygen saturation measurement to determine the presence of a congenital cardiac anomaly of an infant, wherein said comparing computes a difference between said first oxygen saturation measurement and said second oxygen saturation measurement; and

determining and displaying an indication of the congenital cardiac anomaly on a display device of the pulse oximeter.

2. The method of claim 1, further comprising detecting a patent ductus arteriosus, based at least in part, on a determination that said difference between said first oxygen saturation measurement and said second oxygen saturation measurement is substantially zero.

3. The method of claim 2, wherein detecting a patent ductus arteriosus is further based on a determination of a phase difference between a first plethysmograph measurement at said first tissue site and a second plethysmograph measurement at said second tissue site.

4. The method of claim 3, wherein said phase difference is substantially non-zero.

5. The method of claim 2, wherein detecting a patent ductus arteriosus is further based on a determination of a relative amount of damping between a first plethysmograph measurement at said first tissue site and a second plethysmograph measurement at said second tissue site.

6. The method of claim 5, wherein said relative amount of damping is substantially non-zero.

7. The method of claim 1, wherein said first limb of a patient is a right arm and said second limb of a patient is at least one of a left foot or a left hand.

8. A physiological monitor comprising:

interface componentry in communication with at least two sensors adapted to be positioned on tissue sites of a patient, said interface componentry having at least two outputs corresponding to signals received from said sensors and responsive to light transmitted through said tissue sites; and

at least one signal processor in communication with said interface componentry outputs, said at least one signal processor configured to:

receive a first output, from said interface componentry, associated with a first tissue site on a first limb of the patient;

receive a second output, from said interface componentry, associated with a second tissue site on a second limb of the patient;

25

determine at least one first oxygen saturation measurement from said first tissue site and at least one second oxygen saturation measurement from said second tissue site in response to said first output and said second output; and

compare said at least one first oxygen saturation measurement with said at least one second oxygen saturation measurement to determine the presence of a congenital cardiac anomaly of an infant and display an indication of the congenital cardiac anomaly.

9. The physiological monitor of claim 8, wherein the at least one signal processor is further configured to determine said congenital cardiac anomaly is a patent ductus arteriosus, based, at least in part, on a determination that a difference between said at least one first oxygen saturation measurement and said at least one second oxygen saturation measurement is substantially zero.

10. The physiological monitor of claim 9, wherein said at least one signal processor is further configured to:

determine plethysmograph measurements from said first tissue site and said second tissue site; and

compare at least one first plethysmograph measurement from said first tissue site with a second plethysmograph measurement from said second tissue site,

26

wherein said determination of said patent ductus arteriosus is further based on said comparison between said at least one first plethysmograph measurement and said at least one second plethysmograph measurement.

11. The physiological monitor of claim 10, wherein said comparison between said at least one first plethysmograph measurement and said at least one second plethysmograph measurement identifies a phase difference between said at least one first plethysmograph measurement and said at least one second plethysmograph measurement.

12. The physiological monitor of claim 11, wherein said phase difference is substantially non-zero.

13. The physiological monitor of claim 10, wherein said comparison between said at least one first plethysmograph measurement and said at least one second plethysmograph measurement identifies a relative amount of damping between said at least one first plethysmograph measurement and said at least one second plethysmograph measurement.

14. The physiological monitor of claim 13, wherein said relative amount of damping is substantially non-zero.

15. The physiological monitor of claim 8, wherein said first limb of said patient is a right arm and said second limb of said patient is at least one of a left foot or a left hand.

* * * * *

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : 9,492,110 B2
APPLICATION NO. : 14/275691
DATED : November 15, 2016
INVENTOR(S) : Ammar Al-Ali et al.

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

In the Specification


In Column 7 at Line 63 (approx.), Change “Red_{AC},” to --Red_{AC}--.

In Column 13 at Line 20, Change “ μ_t ,” to -- μ_b --.

In Column 19 at Line 60, Change “Sp_aO₂1790” to --Sp_aO₂ 1790--.

In Column 19 at Line 66, Change “Sp_aO₂1780” to --Sp_aO₂ 1780--.

Signed and Sealed this
Twenty-third Day of May, 2017



Michelle K. Lee
Director of the United States Patent and Trademark Office

专利名称(译)	生理监测		
公开(公告)号	US9492110	公开(公告)日	2016-11-15
申请号	US14/275691	申请日	2014-05-12
[标]申请(专利权)人(译)	梅西莫股份有限公司		
申请(专利权)人(译)	Masimo公司		
当前申请(专利权)人(译)	Masimo公司		
[标]发明人	AL ALI AMMAR DIAB MOHAMED K KIANI MASSI E KOPOTIC ROBERT JAMES TOBLER DAVID		
发明人	AL-ALI, AMMAR DIAB, MOHAMED K. KIANI, MASSI E. KOPOTIC, ROBERT JAMES TOBLER, DAVID		
IPC分类号	A61B5/00 A61B5/1455 A61B5/0205 A61B5/1459 A61B5/024 A61M16/00 A61B5/145		
CPC分类号	A61B5/6838 A61B5/742 A61B5/746 A61B5/6815 A61B5/6819 A61B5/6825 A61B5/6826 A61B5/6829 A61B5/14551 A61B5/0205 A61B5/1459 A61B5/6814 A61B5/02416 A61M16/00 A61M2230/205 A61M16/021		
优先权	11/417931 2013-01-29 US 11/104720 2010-07-20 US 10/668487 2005-05-24 US 10/026013 2004-03-30 US 09/323176 2001-12-25 US 60/087802 1998-06-03 US		
其他公开文献	US20150018650A1		
外部链接	Espacenet USPTO		

摘要(译)

患者监测器具有多个适于附着到活体的组织部位的传感器。传感器产生传感器信号，其在组织部位内的脉动血液衰减之后响应于至少两个波长的光辐射。

