



US009990468B2

(12) **United States Patent**
Lane et al.

(10) **Patent No.:** **US 9,990,468 B2**
(45) **Date of Patent:** ***Jun. 5, 2018**

(54) **MEDICAL INSTRUMENT WITH
REMAINING VISITS INDICATOR**

(71) Applicant: **Welch Allyn, Inc.**, Skaneateles Falls,
NY (US)

(72) Inventors: **John A. Lane**, Weedsport, NY (US);
Craig M. Meyerson, Syracuse, NY
(US); **David M. Fallat**, Auburn, NY
(US); **Vuong B. Nguyen**, Liverpool,
NY (US); **Shawn C. St. Pierre**,
Syracuse, NY (US); **Kenneth V. Coon**,
III, Jordan, NY (US); **Michael D.**
Garrant, Marcellus, NY (US)

(73) Assignee: **WELCH ALLYN, INC.**, Skaneateles
Falls, NY (US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 0 days. days.

This patent is subject to a terminal dis-
claimer.

(21) Appl. No.: **15/390,177**

(22) Filed: **Dec. 23, 2016**

(65) **Prior Publication Data**

US 2017/0109489 A1 Apr. 20, 2017

Related U.S. Application Data

(62) Division of application No. 14/079,388, filed on Nov.
13, 2013, now Pat. No. 9,560,976.

(51) **Int. Cl.**
A61B 5/02 (2006.01)
G06F 19/00 (2018.01)

(Continued)

(52) **U.S. Cl.**
CPC **G06F 19/3412** (2013.01); **A61B 5/02055**
(2013.01); **A61B 5/14552** (2013.01); **A61B**
5/742 (2013.01); **G06F 19/327** (2013.01);
A61B 5/022 (2013.01); **A61B 5/024** (2013.01);
A61B 2560/0204 (2013.01); **A61B 2560/0437**
(2013.01)

(58) **Field of Classification Search**
CPC . A61B 5/02055; A61B 5/14552; A61B 5/742;
A61B 5/021; A61B 2560/0204; A61B
2560/0437; G06F 19/327; G06F 19/3412
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,693,119 A 9/1987 Johnson
7,657,273 B2 2/2010 Haartsen
(Continued)

FOREIGN PATENT DOCUMENTS

JP 11289677 A 10/1999

OTHER PUBLICATIONS

Cardiac Science, Instruction Manual for Cardiac Science 5300 and
Cardiac Science 5350 Vital Signs Monitor (70-00582-01 A), date
accessed May 14, 2013, 182 pgs.

(Continued)

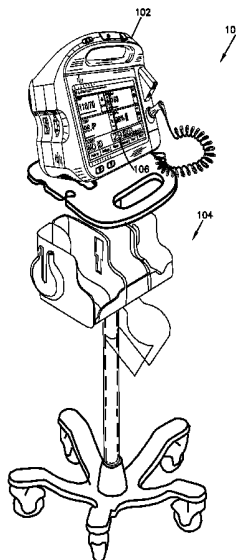
Primary Examiner — Rex R Holmes

(74) *Attorney, Agent, or Firm* — Merchant & Gould P.C.

(57) **ABSTRACT**

A medical instrument includes a remaining visits indicator.
The remaining visits indicator visually identifies a number of
patient visits that can be completed before recharging the
medical instrument.

19 Claims, 10 Drawing Sheets



(51) **Int. Cl.**

A61B 5/0205 (2006.01)
A61B 5/1455 (2006.01)
A61B 5/00 (2006.01)
A61B 5/022 (2006.01)
A61B 5/024 (2006.01)

(56) **References Cited**

U.S. PATENT DOCUMENTS


8,332,342	B1	12/2012	Saha et al.	
9,560,976	B2 *	2/2017	Lane	A61B 5/02055
2008/0312852	A1 *	12/2008	Maack	A61N 1/3708
				702/63
2009/0062887	A1	3/2009	Mass	
2011/0040572	A1	2/2011	Chmiel et al.	
2011/0153154	A1	6/2011	Hagenbuch	
2012/0003933	A1	1/2012	Baker	
2012/0095312	A1	4/2012	Ramey et al.	
2012/0210325	A1	8/2012	De Lind van Wijngaarden	
2012/0215075	A1	8/2012	Surace et al.	

OTHER PUBLICATIONS

Welch Allyn, Vital Signs Monitor 300 Series Directions for Use,
date accessed May 14, 2013, 108 pgs.

* cited by examiner

FIG. 1

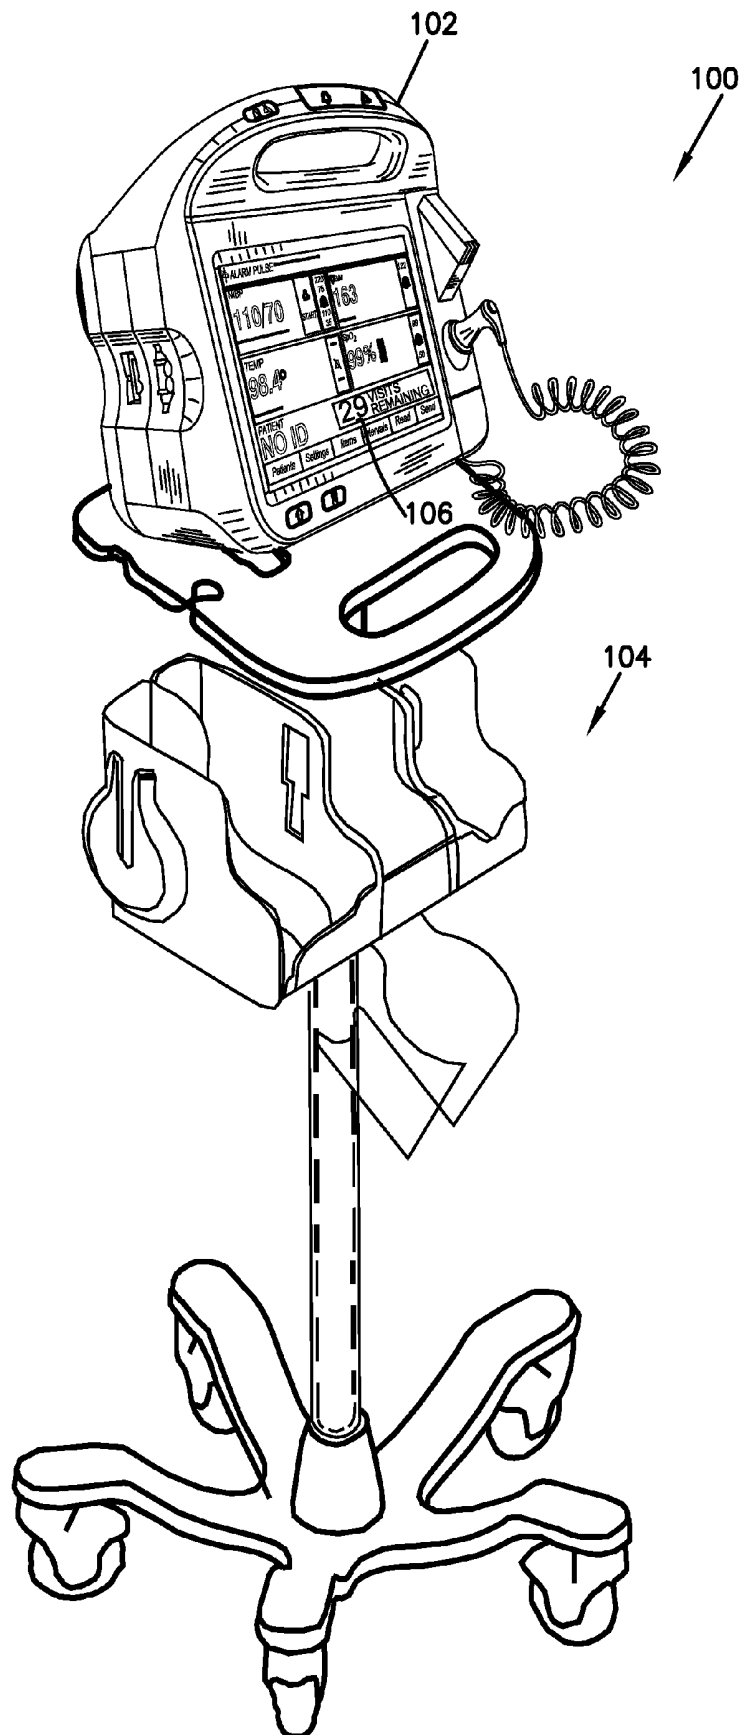


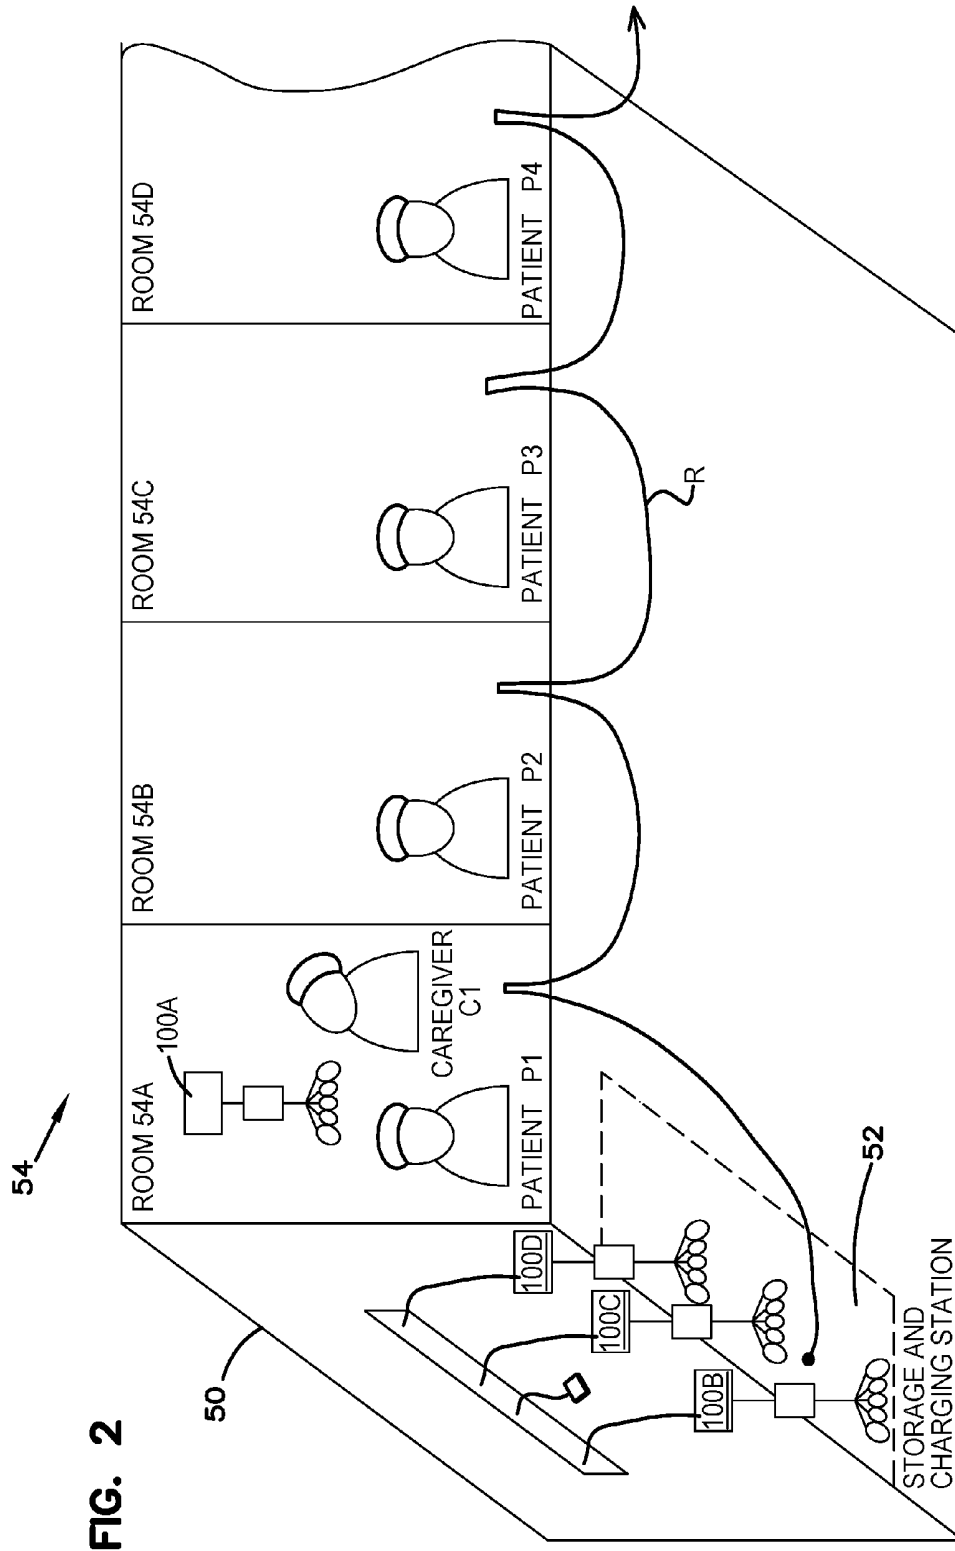


FIG. 3

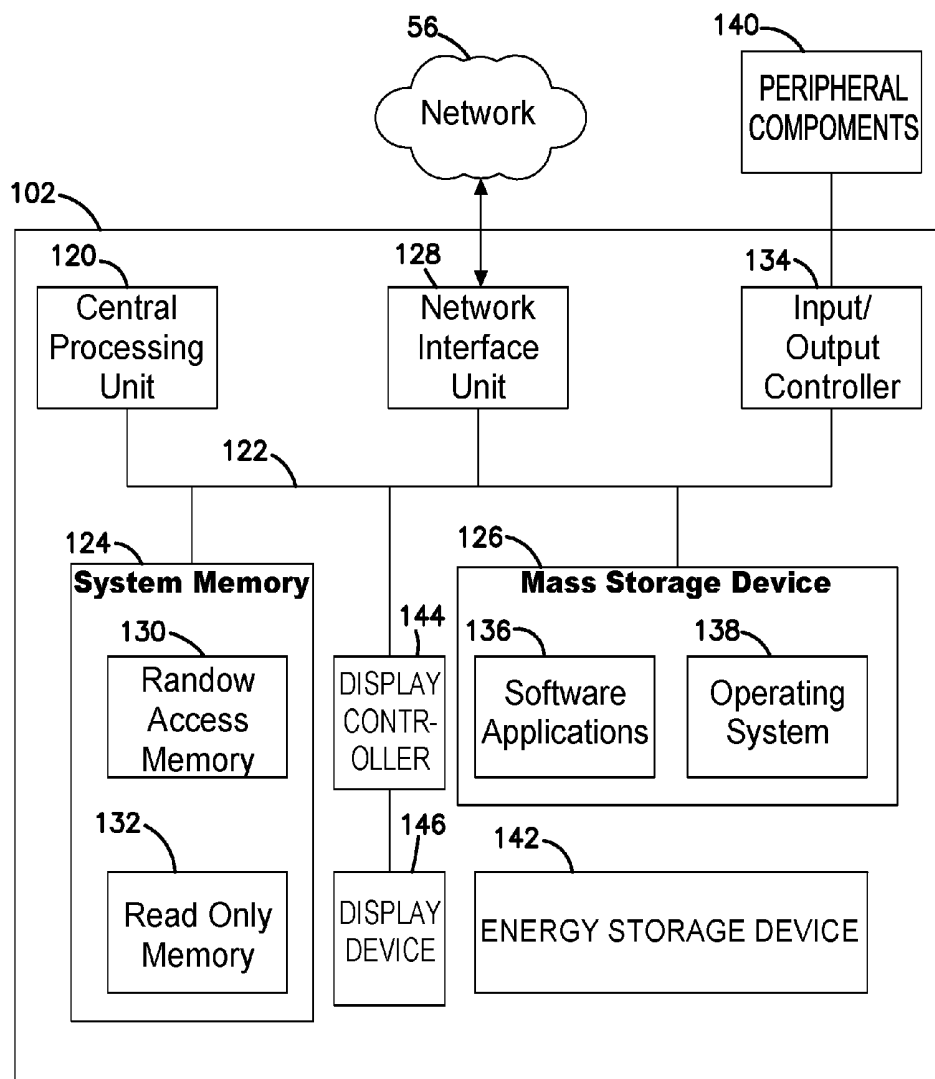

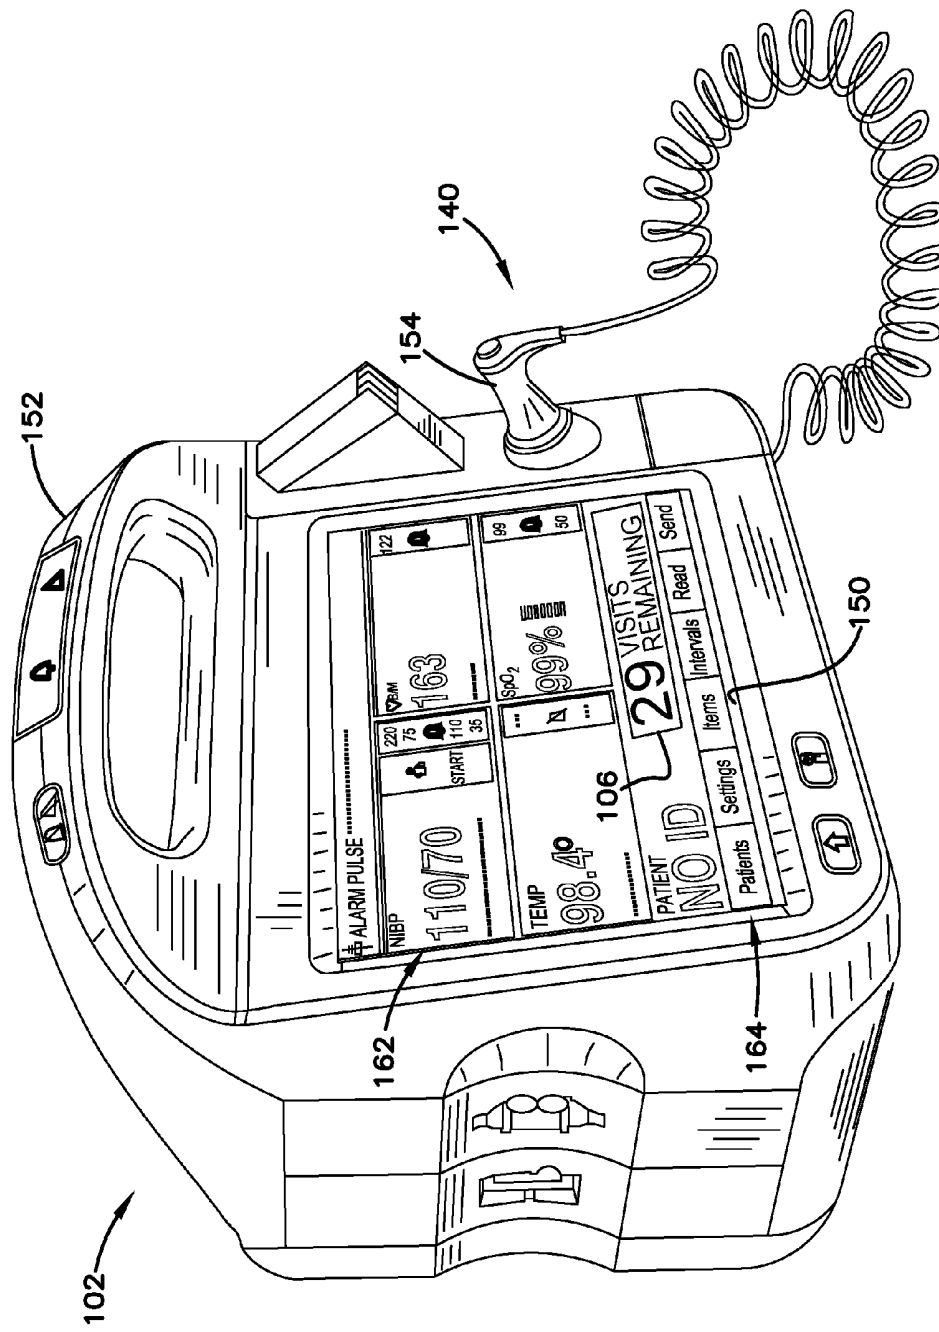


FIG. 4

FIG. 5

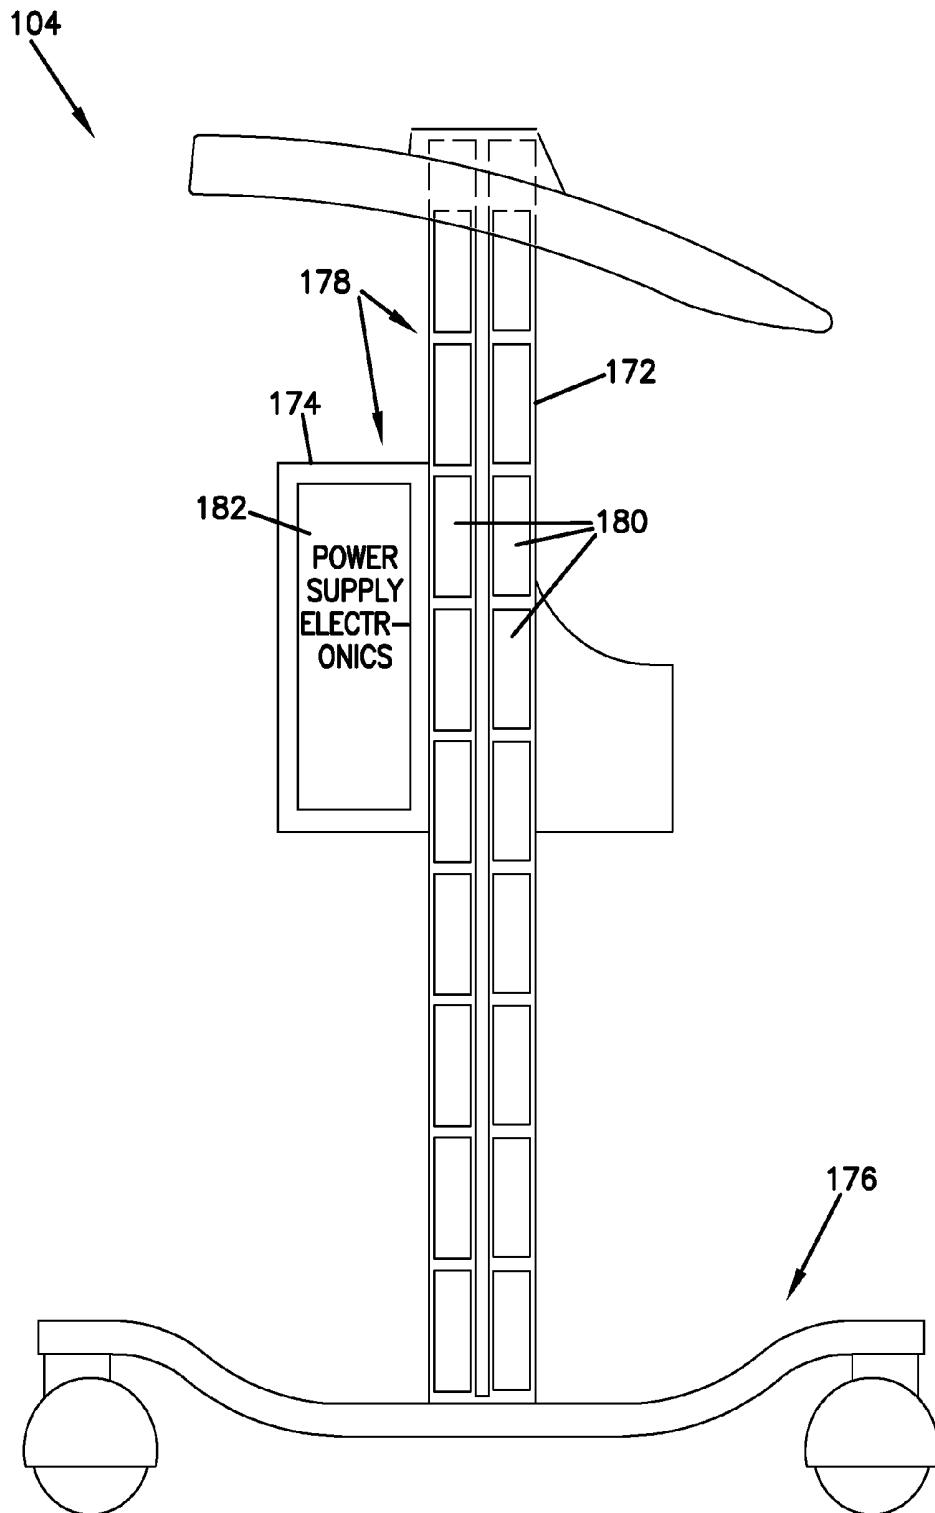


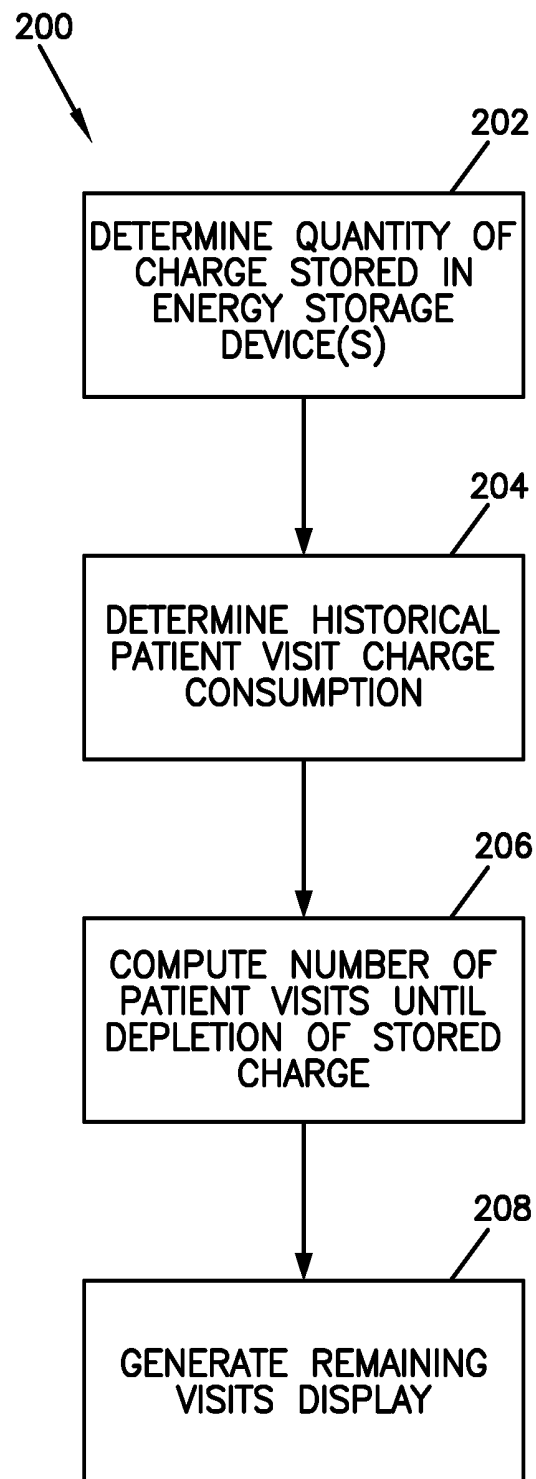
FIG. 6

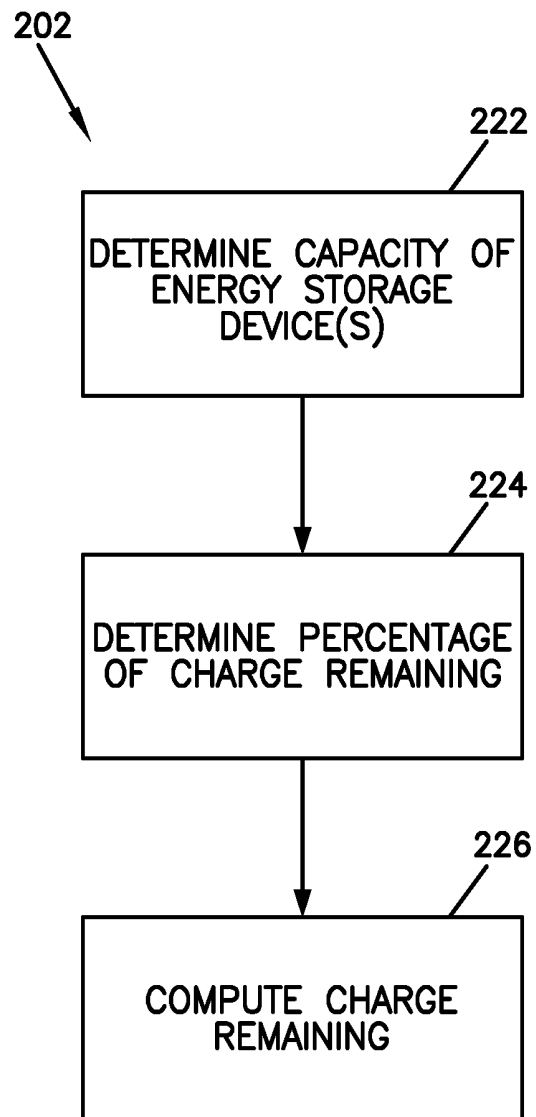
FIG. 7


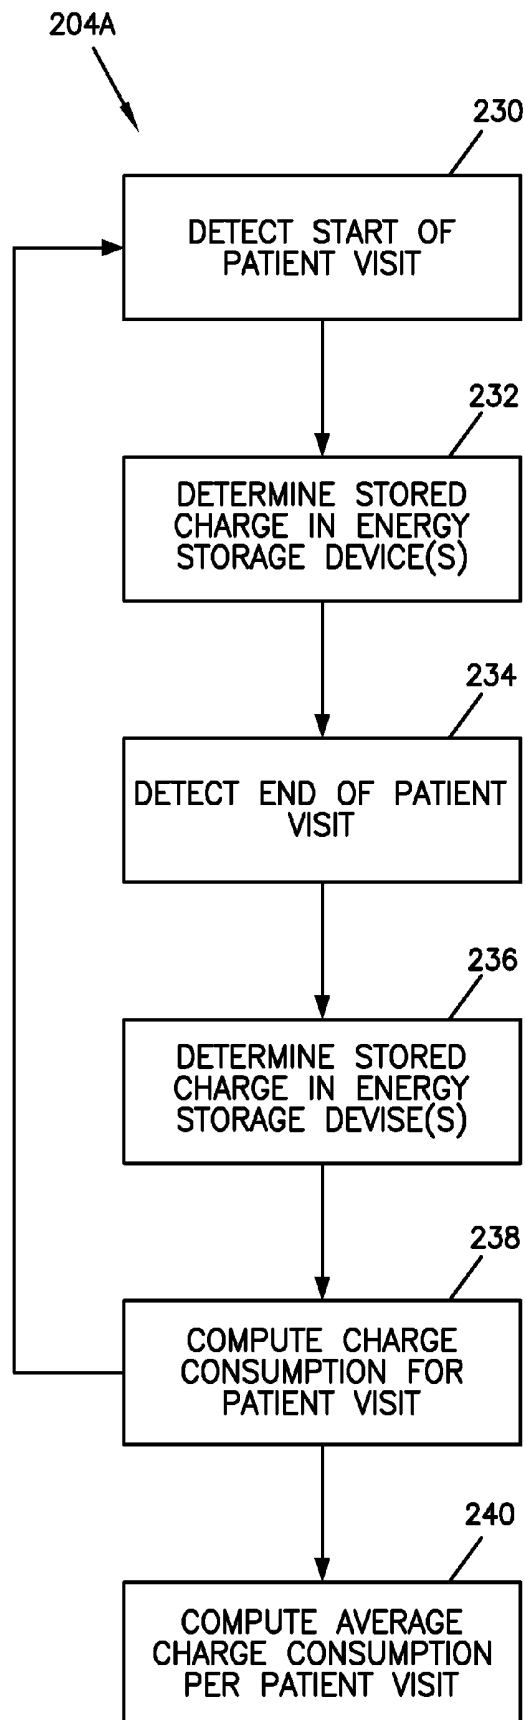
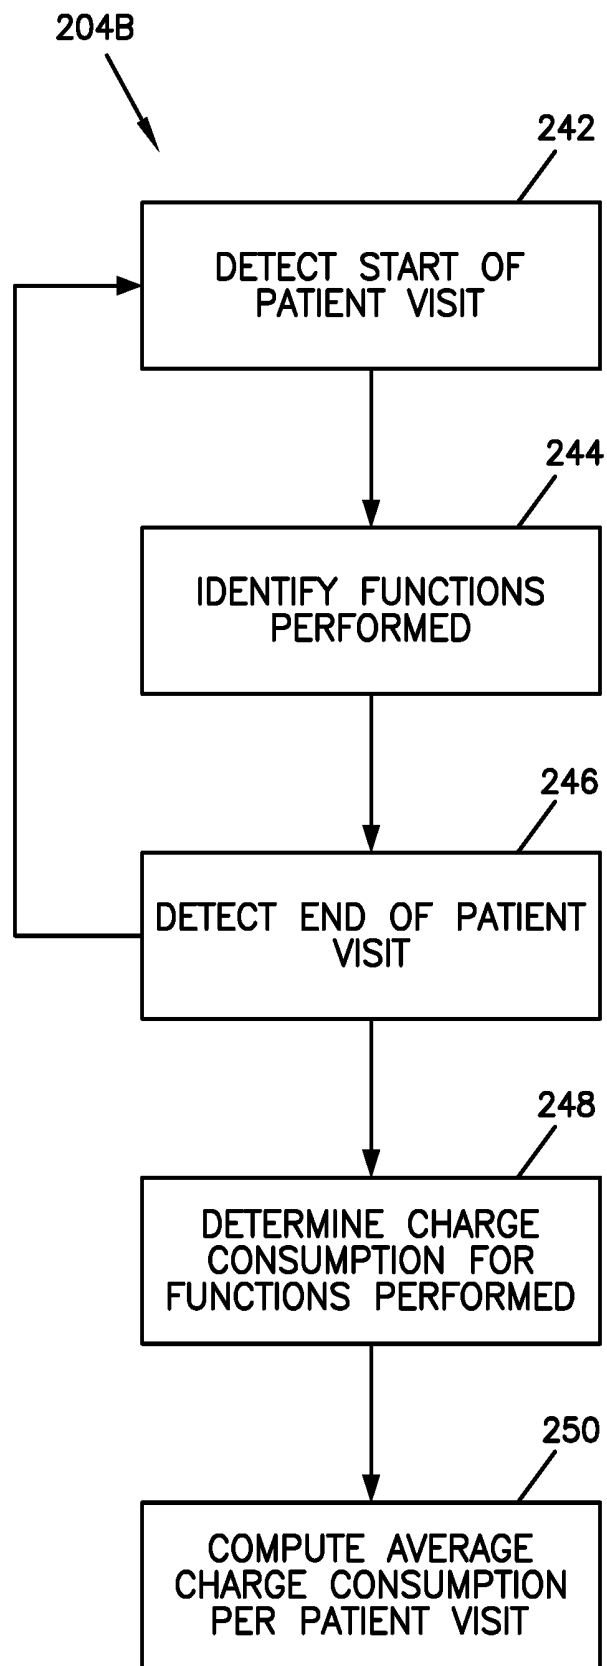
FIG. 8

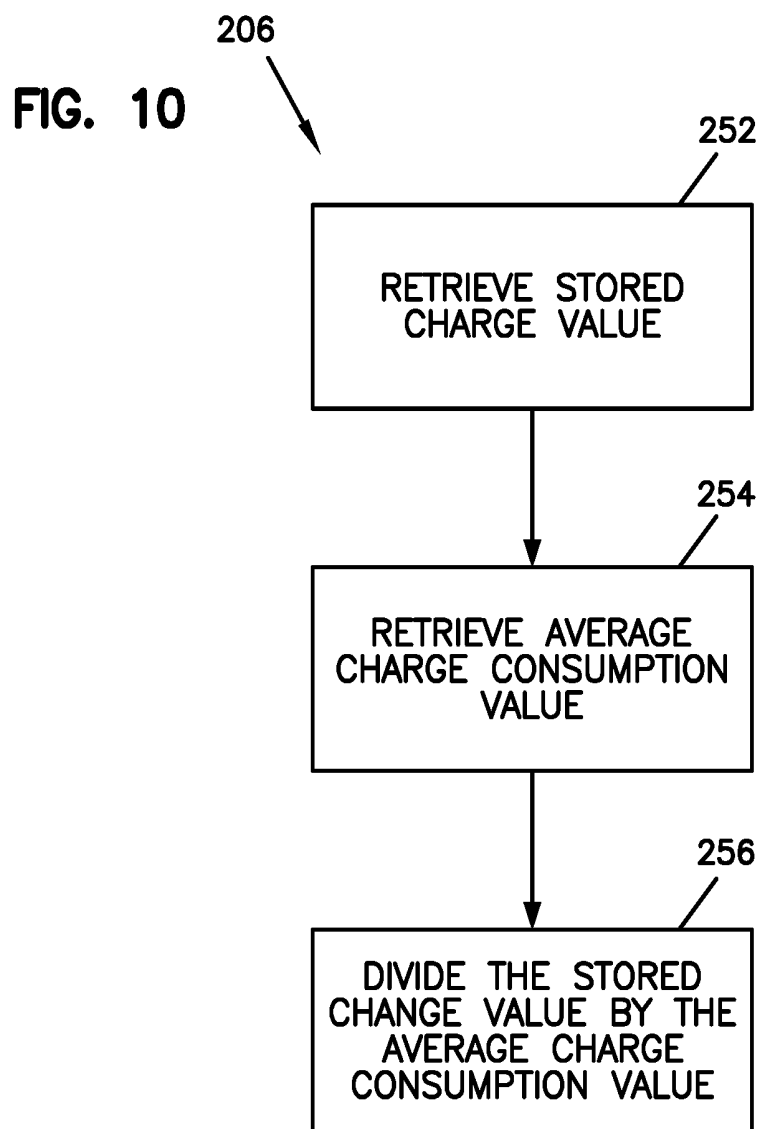FIG. 9



1

**MEDICAL INSTRUMENT WITH
REMAINING VISITS INDICATOR****CROSS-REFERENCE TO RELATED
APPLICATION**

This application is a divisional of U.S. patent application Ser. No. 14/079,388 filed on Nov. 13, 2013 and entitled MEDICAL INSTRUMENT WITH REMAINING VISITS INDICATOR, the disclosure of which is hereby incorporated by reference in its entirety.

BACKGROUND

Batteries are commonly used to power mobile medical instruments to permit the mobile medical instruments to be moved independent of stationary power sources.

A visual indicator is sometimes provided on mobile medical instruments to identify the amount of charge remaining in the batteries. Such an indicator may indicate whether the battery is fully charged, partially charged, or nearly depleted, for example.

SUMMARY

In general terms, this disclosure is directed to a medical instrument with a remaining visits indicator. In one possible configuration and by non-limiting example, the remaining visits indicator visually identifies an estimated number of patient visits that can be completed before recharging the medical instrument. Various aspects are described in this disclosure, which include, but are not limited to, the following aspects.

One aspect is a mobile medical instrument configured for use by a caregiver during patient visits, the mobile medical instrument comprising: a measuring device configured to perform physiological measurements on patients during the patient visits; one or more energy storage devices configured to store energy therein to power the measuring device when performing the physiological measurements; and a display device configured to generate a remaining visits indicator identifying an estimated number of patient visits that can be completed by the instrument before the energy stored in the one or more energy storage devices is depleted.

Another aspect is a method of operating a mobile medical instrument, the method comprising: determining a quantity of charge stored in one or more energy storage devices; determining historical patient visit charge consumption; computing an estimated number of remaining patient visits until the stored charge is depleted; and generating a remaining visits indicator identifying the estimated number of remaining patient visits.

A further aspect is a mobile medical instrument configured for use by a caregiver during patient visits, the mobile medical instrument comprising: a measuring device, the measuring device comprising: a housing; a processing device; peripheral components controlled by the processing device and including one or more sensors configured to cooperate with the measuring device to measure one or more physiological characteristics of patients, the peripheral components including a thermometer, a blood pressure cuff, and a pulse oximeter; a first energy storage device; and a display device operatively connected to the processing device and operable to generate a remaining visits indicator, the remaining visits indicator identifying an estimated number of patient visits that can be completed by the measuring device before recharging the mobile medical instrument; a mobile

2

stand, the mobile stand comprising: a wheeled base comprising a plurality of wheels; a support structure coupled to the wheeled base and configured to support the measuring device in an elevated position; a second energy storage device contained in the support structure; and power supply electronics electrically coupled to the second energy storage device and configured to deliver power from the second energy storage device to the measuring device.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a perspective view of an example mobile medical instrument including a measuring device and a mobile stand.

FIG. 2 illustrates an example of a health care facility in which the mobile medical instrument, shown in FIG. 1, can be used.

FIG. 3 is a schematic block diagram illustrating an example of the measuring device shown in FIG. 1.

FIG. 4 is a front view of another example of the measuring device shown in FIG. 1.

FIG. 5 is a schematic diagram illustrating an example of the mobile stand shown in FIG. 1.

FIG. 6 is a flow chart illustrating a method of operating the mobile medical instrument shown in FIG. 1.

FIG. 7 is a flow chart illustrating a method of determining a quantity of charge stored in one or more energy storage devices.

FIG. 8 is a flow chart illustrating an example method of determining historical patient visit charge consumption.

FIG. 9 is a flow chart illustrating another method of determining historical patient visit charge consumption.

FIG. 10 is a flow chart illustrating an example method of computing a number of patient visits that can be completed before the stored charge is depleted.

DETAILED DESCRIPTION

Various embodiments will be described in detail with reference to the drawings, wherein like reference numerals represent like parts and assemblies throughout the several views. Reference to various embodiments does not limit the scope of the claims attached hereto. Additionally, any examples set forth in this specification are not intended to be limiting and merely set forth some of the many possible embodiments for the appended claims.

FIG. 1 is a perspective view of an example mobile medical instrument 100. In some embodiments, the mobile medical instrument includes a measuring device 102, and a mobile stand 104. The mobile medical instrument 100 also includes a remaining visits indicator 106.

The mobile medical instrument 100 typically includes a measuring device 102. In some embodiments, the measuring device 102 is a physiological measuring platform device. Some embodiments include a multi-function device configured to perform more than one function. An example of a multi-function device is a physiological measuring platform device that is operable to measure one or more of temperature, heart rate, blood pressure, and blood oxygen level, for example. Examples of the measuring device 102 are illustrated and described in more detail with reference to FIGS. 3-4.

In some embodiments the mobile medical instrument 100 further includes a mobile stand 104. The mobile stand 104 is configured to support the measuring device 102 in an elevated position where a caregiver can more easily interact with it. In some embodiments the mobile stand 104 includes

wheels to permit the mobile medical instrument **100** to be easily moved around a health care facility. Examples of the mobile stand **104** are illustrated and described in more detail with reference to FIG. 5.

In the example shown in FIG. 1, the mobile medical instrument **100** includes a remaining visits indicator **106**. In some embodiments the remaining visits indicator **106** visually identifies an estimated number of patient visits that can be completed before recharging the medical instrument, as discussed in more detail herein.

FIG. 2 illustrates an example of a health care facility **50** to depict one example of an environment in which the mobile medical instrument **100** can be used. In this example, the health care facility **50** is a portion of a building including a storage and charging station **52** and patient rooms **54** (including rooms **54A**, **54B**, **54C**, and **54D**). Several mobile medical instruments **100** (including **100A**, **100B**, **100C**, and **100D**) are within the health care facility **50**. Also shown are patients P1, P2, P3, and P4, and a caregiver C1.

The storage and charging station **52** is a designated space in the health care facility **50** in which the mobile medical instruments **100** are stored when not being used by a caregiver. The storage and charging station **52** is a physical space sufficient to store one or more of the mobile medical instruments **100**. In some embodiments the storage and charging station **52** also provides access to a power source that can be used to recharge the mobile medical instruments **100**. For example, the charging station **52** can include electrical outlets or cords that can be electrically connected to the mobile medical instruments **100** to provide a connection to mains power. In another possible embodiment, the charging station **52** includes charging electronics configured for connection to and recharging of the mobile medical instruments **100**.

The following hypothetical scenario is provided to illustrate an exemplary use of the mobile medical instrument **100**. In this example, a caregiver C1 arrives at the health care facility **50** to begin a shift of providing care to a plurality of patients. The caregiver is assigned to perform rounds R to check up on a set of patients, including patients P1, P2, P3, P4, etc.

Before beginning the rounds, the caregiver C1 goes to the storage and charging station **52** to retrieve a mobile medical instrument **100**.

If the mobile medical instruments **100** did not have the remaining visits indicator **106** (shown in FIG. 1), it would be difficult for the caregiver C1 to determine whether a mobile medical instrument **100** has sufficient charge remaining to permit the caregiver C1 to complete the rounds R. In some cases, the mobile medical instrument may not have been plugged in by the previous caregiver. Even if the mobile medical instrument is charging, it may have only been charging for a short time. A battery charge indicator does not convey adequate information. Although a battery charge indicator may depict whether the battery is fully charged, partially charged, or nearly depleted, such an indicator does not allow the caregiver to directly determine whether the charge is sufficient to complete the rounds R.

Therefore, the remaining visits indicator **106**, such as shown in FIG. 1, is provided to identify the estimated number of patient visits that can be completed before the mobile medical instrument **100** needs to be recharged.

As one example, if the caregiver C1 knows that the rounds R requires the caregiver C1 to visit 25 patients, the caregiver C1 can check the remaining visits indicator **106** and see the number of patient visits that can be completed on the current charge. If the remaining visits indicator **106** shows a number

greater than or equal to the number of patients in the rounds R, then the caregiver C1 can determine that he or she can complete the rounds R with the current charge of the mobile medical instrument **100**. If the remaining visits indicator **106** shows a number less than the number of patients in the rounds R, then the caregiver C1 can determine that he or she cannot complete the rounds R with the current charge of the mobile medical instrument **100**, and should either plan to return part of the way through when the charge is depleted, or should consider taking a different mobile medical instrument **100** that will allow the rounds R to be completed.

In the illustrated example, the caregiver C1 selected the mobile medical instrument **100A** to take on the rounds, after checking the remaining visits indicator **106** and determining that the number of remaining visits identified was greater than or equal to the number of patients in the rounds R. This will permit the caregiver C1 to complete the rounds R without having to return to the storage and charging station **52** before the rounds R have been completed.

While on the rounds, the caregiver C1 uses the mobile medical instrument **100** to obtain measurements associated with the patients P. In the illustrated example, the first stop on the caregiver's C1 rounds R is room **54A**, which is currently occupied by patient P1. The caregiver enters the room **54A** and uses the mobile medical instrument **100A** to perform a set of measurements on the patient, such as to check the patient's vital signs. Examples of the vital signs include temperature, heart rate, blood pressure, and blood oxygen level. Other embodiments include other measurements.

Different vital signs measurements require different amounts of charge to complete. For example, a blood pressure reading may require more charge in order to inflate a cuff around the limb of the person to a sufficient pressure, and to operate one or more sensors that detect the patient's heart rate and blood pressure. Accordingly, the amount of charge consumed through the performance of a set of vital signs measurements will vary depending on the particular set of tests that are performed.

Even if the same set of measurements is performed, the amount of charge consumed by the measurements can still vary. Multiple variables can impact the amount of charge consumed, such as how tightly a blood pressure cuff is originally applied, and whether the measurement is repeated one or more times. In some embodiments the mobile medical instrument can include a printer, and different amounts of charge can be consumed depending on whether or not the printer is used after taking measurements for a particular patient. Other functions, such as wireless communication functions and internal processing functions can also adjust charge consumption.

Therefore, in some embodiments the mobile medical instrument **100** stores historical usage data, as discussed in further detail herein, which can be used to determine average charge consumption over a period of time, or across a number of patient visits. This information is then used to predict future usage, so as to permit the mobile medical instrument to predict the number of visits that can be completed before the charge in the mobile medical instrument is depleted.

FIGS. 3-4 illustrate examples of the measuring device **102**.

FIG. 3 is a schematic block diagram illustrating an example of the measuring device **102**. In this example, the measuring device **102** includes at least one central processing unit ("CPU") **120**, a system memory **124**, and a system bus **122** that couples the system memory **124** to the CPU

120. The CPU **120** is an example of a processing device. The system memory **124** includes a random access memory ("RAM") **130** and a read-only memory ("ROM") **132**. A basic input/output system containing the basic routines that help to transfer information between elements within the measuring device **102**, such as during startup, is stored in the ROM **132**. The measuring device **102** further includes a mass storage device **126**. The mass storage device **126** is able to store software instructions and data.

The mass storage device **126** is connected to the CPU **120** through a mass storage controller (not shown) connected to the bus **122**. The mass storage device **126** and its associated computer-readable data storage media provide non-volatile, non-transitory storage for the measuring device **102**. Although the description of computer-readable data storage media contained herein refers to a mass storage device, such as a hard disk or CD-ROM drive, it should be appreciated by those skilled in the art that computer-readable data storage media can be any available non-transitory, physical device or article of manufacture from which the measuring device **102** can read data and/or instructions.

Computer-readable data storage media include volatile and non-volatile, removable and non-removable media implemented in any method or technology for storage of information such as computer-readable software instructions, data structures, program modules or other data. Example types of computer-readable data storage media include, but are not limited to, RAM, ROM, EPROM, EEPROM, flash memory or other solid state memory technology, CD-ROMs, digital versatile discs ("DVDs"), other optical storage media, magnetic cassettes, magnetic tape, magnetic disk storage or other magnetic storage devices, or any other medium which can be used to store the desired information and which can be accessed by the measuring device **102**.

According to various embodiments, the measuring device **102** may operate in a networked environment using logical connections to remote network devices through the network **56**, such as a local network, the Internet, or another type of network. The measuring device **102** connects to the network **56** through a network interface unit **128** connected to the bus **122**. It should be appreciated that the network interface unit **128** may also be utilized to connect to other types of networks and remote computing systems. The measuring device **102** also includes an input/output controller **134** for receiving and processing input from a number of other devices, such as peripheral components **140**. In some embodiments, peripheral components **140** include sensors that can be used by the measuring device **102** to determine one or more physical characteristics of the patient. In some embodiments, the peripheral components **140** are used by the measuring device **102** to perform physiological measurements on the patient. Examples of peripheral components **140** include a thermometer (oral, rectal, temporal, ear, etc.), a blood pressure cuff, and a pulse oximeter. Other peripheral components **140** are used in other embodiments.

In some embodiments the input/output controller **134** is configured to communicate with input devices including a keyboard, a mouse, a touch sensitive user interface display screen, or another type of input device. Similarly, the input/output controller **134** may provide output to a touch sensitive user interface display device **146**, a printer, or other type of output device.

As mentioned briefly above, the mass storage device **126** and the RAM **130** of the measuring device **102** can store software instructions and data. The software instructions include an operating system **138** suitable for controlling the

operation of the measuring device **102** and software applications **136**. The mass storage device **126** and/or the RAM **130** also store software instructions, that when executed by the CPU **120**, cause the measuring device **102** to provide the functionality of the measuring device **102** discussed in this document. For example, the mass storage device **126** and/or the RAM **130** can store software instructions that, when executed by the CPU **120**, cause the measuring device **102** to display a graphical user interface **150**, shown in FIG. 4, including the remaining visits indicator **106**, and/or other screens or displays on the display device **146**.

In some embodiments the measuring device **102** includes an energy storage device **142**. An example of the energy storage device **142** is a rechargeable battery. Rechargeable batteries of a variety of different types can be used. One suitable example is a Lithium-ion type battery. Such batteries can have any desired numbers of cells, and accordingly any desired capacity limited primarily by cost, size, and weight constraints defined for the particular implementation. Another example of the energy storage device **142** is a capacitor, such as a super- or ultra-capacitor.

In some embodiments the energy storage device **142** also includes electronics, such as a processor and electronic circuitry. The central processing unit **120** can communicate with the energy storage device **142** through the electronics to obtain data relating to the energy storage device **142**, such as the total energy capacity of the energy storage device **142** and the present charge stored in the energy storage device **142**, or alternatively the percentage of the charge that is remaining. An example of a suitable energy storage device **142** is any one of the variety of smart battery packs available from Inspired Energy LLC of Newberry, Fla.

In this example the measuring device **102** also includes a display controller **144** and display device **146** that operate to generate a graphical user interface **150**, and present that graphical user interface **150** to the caregiver C1, shown in FIG. 2.

FIG. 4 is a front view of an example measuring device **102**. In this example, the measuring device **102** includes the peripheral components **140** (such as a thermometer **154**) and the display device **146**, as previously discussed, and further includes a housing **152**.

In this example, the display device **146** generates a graphical user interface **150** that is displayed on a face of the measuring device **102**. In some embodiments, the graphical user interface **150** includes measurement displays **162**, remaining visits indicator **106**, and selectable controls **164**.

The measurement display **162** present measurement data obtained through the peripheral components **140**. In this example, the measurement display **162** shows the blood pressure, heart rate, temperature, and SpO2 measurement data. Other measurement data is displayed in other embodiments.

The remaining visits indicator **106** identifies the number of patient visits that can be completed on the present charge (e.g., stored in the energy storage device **142**, shown in FIG. 3), before the mobile medical instrument **100** will need to be recharged. The remaining visits indicator **106** is discussed in further detail herein.

The selectable controls **164** provide a menu for accessing other possible functions of the measurement device, such as to change settings, alarms, intervals, or calibration, or to send measurement data through the network **56**, shown in FIG. 3.

FIG. 5 is a schematic diagram illustrating an example of the mobile stand **104**. In this example, the mobile stand **104** includes a support structure **172**, a storage region **174**, and

a wheeled base **176**. In addition, in some embodiments the mobile stand **104** includes an integral power supply **178**.

In some embodiments, the mobile stand **104** operates to support the measuring device **102** in an elevated position above the ground. To do so, the measuring device **102** is placed on the mobile stand **104** and fastened thereto, as shown in FIG. 1. The support structure **172** supports the measuring device **102** in the elevated position.

A wheeled base **176** is provided in some embodiments to permit the mobile medical instrument **100** to be easily moved within a health care facility **50**, such as shown in FIG. 2. The wheeled base **176** includes one or more wheels. The support structure **172** is connected to the wheeled base **176**.

A storage region **174** is provided in some embodiments for the storage of additional items, such as peripheral components, medical records, or any other items. In some embodiments the storage region **174** also includes an interior space in which portions of the power supply **178** can be housed.

In some embodiments the mobile stand **104** includes an integral power supply **178**, which stores electrical energy that can be used to power the measuring device **102**. The power supply **178** includes one or more energy storage devices **180** that store electrical energy. Examples of the energy storage devices **180** are batteries and capacitors.

In some embodiments the energy storage devices **180** are housed within an interior space of the support structure **172**, or alternatively within an interior space of the storage region **174**, or both.

Some embodiments further include power supply electronics **182**. In some configurations, the power supply electronics **182** include a processing device that monitors the status of the energy storage devices **180**, such as to identify the capacity of the energy storage devices **180** and a charge level of the energy storage devices **180**. In some embodiments the measuring device **102** communicates with the power supply electronics **182**, such as through wired or wireless connections, to obtain data relating to the energy storage devices **180**.

One example of a suitable mobile stand **104** is described in U.S. Ser. No. 13/718,869, filed on Dec. 18, 2012, titled MOBILE CART WITH CAPACITIVE POWER SUPPLY, the disclosure of which is hereby incorporated by reference in its entirety.

Although in the example shown in FIG. 5 the power supply electronics **182** are illustrated as being located within the storage region **173**, the power supply electronics **182** (or other electronic components discussed herein) can be arranged in other locations within the mobile stand **104** or measuring device **102**. For example, in some embodiments electronics are arranged within the upper work surface of the mobile stand **104**.

FIG. 6 is a flow chart illustrating a method **200** of operating a mobile medical instrument **100**. In this example, the method includes operations **202**, **204**, **206**, and **208**.

The operation **202** is performed to determine a quantity of charge store in one or more energy storage devices. An example of operation **202** is illustrated and described in more detail with reference to FIG. 7.

The operation **204** is performed to determine historical patient visit charge consumption. Examples of operation **204** are illustrated and described in more detail with reference to FIGS. 8-9.

The operation **206** is performed to compute an estimated number of patient visits that can be completed using the mobile medical instrument until the stored charge is

depleted. An example of the operation **206** is illustrated and described in more detail with reference to FIG. 10.

The operation **208** is performed to generate a remaining visits indicator. An example of the remaining visits indicator **106** is shown in FIG. 4.

In some embodiments, one or more of the operations **202**, **204**, **206**, and **208** are performed using a processing device, such as a processing device of the measuring device **102** or of the mobile stand **104**, shown in FIG. 1. The remaining visits indicator **106** is displayed on a display device of the mobile medical instrument **100**, such as of the measuring device **102** or of the mobile stand **104**.

In some embodiments, the remaining visits indicator **106** is part of the mobile stand **104**. For example, the remaining visits indicator **106** is arranged in or adjacent a handle (shown in FIG. 1) of the mobile stand **104**. The remaining visits indicator **106** can be implemented with a variety of different display devices, such as an LCD or LED panel display device. A LED text display including multi-segment LEDs is used in some embodiments. Any other display technology can also be used in other embodiments. In some embodiments the remaining visits indicator **106** is coupled with one or more other indicators, which may be provided adjacent to one another, or may be combined into the single display, such as by cycling through multiple different indicators through the same display. For example, in some embodiments the indicator also displays one or more of: a battery power remaining, an estimated amount of time remaining, and a date/time indicator. Some embodiments include the remaining visits indicator **106** along with a date and/or time indicator. In some embodiments multiple indicators are contained in and included in single display.

FIG. 7 is a flow chart illustrating a method **202** of determining a quantity of charge stored in one or more energy storage devices. FIG. 7 also illustrates an example of the operation **202**, shown in FIG. 6. In this example, the method **202** includes operations **222**, **224**, and **226**.

The operation **222** is performed to determine a capacity of one or more energy storage device(s) that are available to supply power to the mobile medical instrument **100**. In some embodiments, operation **222** involves querying the energy storage devices, such as by sending a message to the energy storage device **142**, shown in FIG. 3, and/or to the energy storage device **180**, shown in FIG. 5. In some embodiments, the energy storage devices provide their capacities in response. In other embodiments, the energy storage devices provide an identifier of a type of the energy storage device, which permits the mobile medical instrument to determine the capacity, such as using a lookup table that maps types of energy storage devices with their capacities. For example, in some embodiments the energy storage devices can include various numbers of cells, such as 3, 5, 7, or 9 cells. Each cell has a known capacity, and therefore once the type of energy storage device is known, and the number of cells in that type, the capacity can be determined.

The operation **224** is performed to determine a percentage of charge remaining in the energy storage device(s). In some embodiments, operation **224** involves querying the energy storage devices, such as by sending a message to the energy storage device **142**, shown in FIG. 3, and/or to the energy storage device **180**, shown in FIG. 5, requesting that the energy storage devices identify the current percentage of charge remaining. In some embodiments, the energy storage devices reply with a percentage of charge remaining.

The operation **226** is performed to compute the charge remaining in the energy storage device(s). As one example, the operation **226** multiplies the capacity from operation **222**

by the percentage of charge remaining to determine the total charge remaining in the energy storage device. When multiple energy storage devices are present, the total charge remaining is computed as the sum of the individual charges remaining in each of the energy storage devices. A stored charge value is stored in a computer readable storage device that identifies the total charge stored in the energy storage devices.

FIG. 8 is a flow chart illustrating an example method 204A of determining historical patient visit charge consumption. FIG. 8 is also an example of the operation 204, shown in FIG. 7. In this example, the method 204A includes operations 230, 232, 234, 236, 238, and 240.

The operations 230, 232, 234, 236, and 238 are performed to evaluate the charge consumption during an individual patient visit. The operation 240 is then performed to use this data to determine an average charge consumption per patient visit.

The operation 230 is performed to detect the start of a patient visit. In some embodiments, the start of a patient visit occurs when the caregiver C1 (shown in FIG. 2) provides an input into the mobile medical instrument, such as by pressing a physical button or selectable control on the measuring device 102. In some embodiments, the mobile medical instrument 100 operates in a sleep mode (e.g., a low power consumption mode) when not in use, and the mobile medical instrument 100 returns to the normal operating mode upon receipt of an input from the caregiver C1.

In some embodiments, after detection of the start of the patient visit in the operation 230, the operation 232 is performed to determine the amount of charge stored in the energy storage device(s). One possible process for doing so is illustrated in FIG. 7. The stored charge value representing the amount of charge stored at the beginning of the patient visit is then stored in a computer readable storage device for subsequent use.

The mobile medical instrument 100 is then operated to perform the desired functions as directed by the caregiver C1, such as to take one or more measurements using the peripheral components 140 and measuring device 102. As the functions are performed, energy is consumed from the energy storage devices.

The operation 234 is performed to detect the end of a patient visit. There are multiple different ways that the end of a patient visit can be determined. One possible way is to detect that a predetermined period of time (such as in a range from about 1 minute to about 5 minutes) has elapsed without receiving any inputs from the caregiver C1 into the mobile medical instrument 100. Once the predetermined period of time has elapsed, the mobile medical instrument 100 determines that the patient visit has been completed. In some embodiments, the mobile medical instrument 100 returns to a sleep mode of operation after the predetermined period of time has elapsed.

In another possible embodiment, the mobile medical instrument detects the receipt of an input from a caregiver C1. The input can be, for example, the selection of a power button, a sleep button, or an end button, any of which signal to the mobile medical instrument that the caregiver C1 has completed the patient visit.

In yet another possible embodiment, the mobile medical instrument 100 includes an accelerometer which operates to detect movement of the mobile medical instrument. Typically during a patient visit the mobile medical instrument 100 will be substantially stationary. At the end of the patient visit, the caregiver C1 will move the mobile medical instrument 100 from one room (such as room 54A, shown in FIG.

2) to another room (such as room 54B, shown in FIG. 2). In order to avoid incorrect determinations of the end of the patient visit, the operation 234 can monitor the movement data from the accelerometer to identify movement that occurs for more than a predetermined period of time (e.g., in a range from about 3 seconds to about 30 seconds), and/or greater than a predetermined magnitude. Once movement is detected that satisfies the predefined criteria, the mobile medical instrument 100 determines that the patient visit has ended.

The accelerometer can also or alternatively be used for other purposes. For example, in some embodiments the remaining visits indicator 106 is activated upon the detection of movement (including pulling, tapping, shaking, nudging, etc.) of the mobile medical instrument 100, by the accelerometer.

In other embodiments, the remaining visits indicator 106 is activated by a touch or proximity sensor, for example. When not activated, the remaining visits indicator 106 can be turned off, or placed into a low power sleep mode to conserve energy. In some embodiments the remaining visits indicator is displayed by a display device separate from a primary user interface display device of the measuring device 102.

In some embodiments the remaining visits indicator 106 can be displayed separate from the measuring device 102. An advantage of the separate display is that the remaining visits indicator 106 can be displayed promptly upon the receipt of an input, without having to wait for the measuring device 102 to be powered on and complete a boot process, for example. Instead, the remaining visits indicator 106 can be immediately displayed upon the receipt of an input, which can include detected movement, a tap input onto the remaining visits indicator, pressing or selecting a button, switch, or other input device, and the like. This allows the caregiver to quickly determine the number of remaining visits available on the mobile medical instrument 100, to determine whether the remaining visits are adequate for his or her needs, or whether a different mobile medical instrument 100 should be selected.

At the conclusion of the patient visit, operation 236 is performed to determine the amount of charge stored in the energy storage device(s). One possible process for doing so is illustrated in FIG. 7. The stored charge value representing the amount of charge stored at the end of the patient visit is stored in a computer readable storage device for subsequent use.

When the process of operations 230, 232, 234, 236, and 238 is repeated, as graphically illustrated in FIG. 8, the determination of the stored charge in both of operations 232 and 236 is not required. Instead, in some embodiments only one of operations 232 and 236 can be performed. For example, the result of operation 236 can also be identified and used as the starting charge (operation 232) for the next patient visit.

The operation 238 is performed to compute the charge consumption for the concluded patient visit. As one example, the stored charge value at the end of the patient visit (operation 236) is subtracted from the stored charge value at the start of the patient visit (operation 232). The difference represents the amount of charge consumed during the patient visit. The charge consumption value representing the amount of charge consumed during the patient visit is stored in a computer readable storage device.

The process involving some or all of operations **230**, **232**, **234**, **236**, and **238** is repeated for each subsequent patient visit to generate historical patient visit charge consumption data.

Once the historical patient visit charge consumption data has been generated, the operation **240** is performed to compute an average charge consumption per patient visit. In one example, the historical patient visit charge consumption data is evaluated over a set of patient visits to determine an average charge consumption per patient visit. As one example, a set of the 10 most recent patient visits is evaluated. Other embodiments use other set sizes, such as in a range from about 3 to about 30 or more. An average charge consumption value is stored in a computer readable storage device identifying the average charge consumed per patient visit.

Other factors can also be considered in other embodiments. Several examples of other factors include the time of day, the identity of the current caregiver C1 operating the mobile medical instrument, and an identified set of tests and measurements that are to be performed during the rounds R (FIG. 2).

FIG. 9 is a flow chart illustrating another method **204B** of determining historical patient visit charge consumption. FIG. 9 is also another example of the operation **204**, shown in FIG. 7. In this example, the method **204B** includes operations **242**, **244**, **246**, **248**, and **250**.

In this example, rather than determining the charge consumption of each patient visit directly, operations **242**, **244**, and **246** operate to identify a set of functions performed by the mobile medical instrument during a patient visit. Using this information, a typical set of functions that are performed during a patient visit can be identified. Once the typical set of functions is known, the charge consumption can be determined in operation **248**, such as by retrieving an estimated charge consumption value for each of these functions from a lookup table, or alternatively from historical data. An average charge consumption per patient visit is then computed in operation **250** based on the typical set of functions that are performed.

FIG. 10 is a flow chart illustrating an example method **206** of computing an estimated number of patient visits that can be completed before the stored charge is depleted, and before recharging is needed. FIG. 10 is also an example of the operation **206**, shown in FIG. 6. In this example, the method **206** includes operations **252**, **254**, and **256**.

The operation **252** is performed to retrieve the stored charge value from the computer readable storage device. The stored charge value indicates the amount of charge currently stored in the energy storage device(s), such as determined using the operation **202**, shown in FIG. 6.

The operation **254** is performed to retrieve the average charge consumption value from the computer readable storage device. The average charge consumption value indicates the average charge consumed per patient visit, such as determined using the operation **204**, shown in FIG. 6.

The operation **256** is performed to compute the number of patient visits remaining on the current charge. In one example, the computation occurs by dividing the stored charge value by the average charge consumption value to generate an estimate of the number of patient visits that can be completed by the mobile medical instrument on the current charge.

Once the estimated number of patient visits remaining has been computed, the remaining visits indicator **106** can be generated as represented by operation **208**, shown in FIG. 6. An example of the remaining visits indicator **106** is shown

in FIG. 3. The remaining visits indicator **106** can be presented anywhere on the mobile medical instrument **100**, such as through the graphical user interface **150** of the measuring device **102**, or on a separate display of the measuring device **102** or mobile stand **104**. In some embodiments the remaining visits indicator **106** is displayed by an electronic display device including an electronic paper display. Other display devices are used in other embodiments.

In some embodiments, the remaining visits indicator **106** is visible whether or not the mobile medical instrument **100** is plugged into the charging station or not. In some embodiments the remaining visits indicator **106** is illuminated continuously when the mobile medical instrument **100** is plugged in, but flashes when not plugged in to conserve energy. As one example, the display flashes at a rate of $\frac{1}{5}^{th}$ of a second. In some embodiments the remaining visits indicator **106** has a different graphical presentation when the remaining number of patient visits available on the current charge is reduced below a predetermined value. As one example, the remaining visits indicator **106** is backlit with a multi-colored (e.g., two or more) LED, such that a second color (e.g., red) is illuminated when the number of remaining patient visits goes below the threshold value.

In some embodiments the remaining visits indicator graphically displays a numerical value. In other embodiments, the remaining visits indicator conveys a number in a non-numerical form. One example of a non-numerical form is the illumination of a number of LEDs, where each illuminated LED represents one remaining patient visit. A graphical user interface can similarly display dots or other non-numerical graphical elements representing remaining patient visits, in yet other embodiments.

The various embodiments described above are provided by way of illustration only and should not be construed to limit the claims attached hereto. Those skilled in the art will readily recognize various modifications and changes that may be made without following the example embodiments and applications illustrated and described herein, and without departing from the true spirit and scope of the following claims.

What is claimed is:

1. A method of operating a mobile medical instrument, the method comprising:

determining a quantity of charge stored in one or more energy storage devices;

determining historical patient visit charge consumption through:

detecting a start of a patient visit;

determining a starting charge stored in the one or more energy storage devices;

detecting an end of the patient visit;

determining an ending charge stored in the one or more energy storage devices; and

computing a difference between the starting charge and the ending charge;

computing an estimated number of remaining patient visits until the stored charge is depleted; and
generating a remaining visits indicator identifying the estimated number of remaining patient visits.

2. The method of claim 1, wherein determining a quantity of charge stored in one or more energy storage devices comprises:

determining a capacity of the one or more energy storage devices;

determining a percentage of charge remaining in the one or more energy storage devices; and

computing the quantity of charge stored.

13

3. The method of claim 1, wherein determining historical patient visit charge consumption comprises computing an average charge consumption across a predetermined set of prior patient visits.

4. The method of claim 1, further comprising:
storing the difference as a charge consumption value; and
using two or more charge consumption values of two or more patient visits to determine an average charge consumption per patient visit.

5. The method of claim 1, wherein computing a remaining number of patient visits until the stored charge is depleted comprises:

retrieving a stored charge value;
retrieving an average charge consumption value; and
dividing the stored charge value by the average charge consumption value.

6. The method of claim 1, wherein detecting the start of the patient visit comprises receiving a caregiver input to the mobile medical instrument indicative of the start of the patient visit.

7. The method of claim 1, wherein detecting the end of the patient visit comprises receiving a caregiver input to the mobile medical instrument indicative of the end of the patient visit.

8. The method of claim 1, wherein detecting the end of the patient visit comprises determining that a predetermined time has passed from the start of the patient visit.

9. The method of claim 1, wherein detecting the end of the patient visit comprises detecting movement of the mobile medical instrument.

10. A method of operating a mobile medical instrument, the method comprising:

determining a quantity of charge stored in one or more energy storage devices;
determining historical patient visit charge consumption through:
detecting a start of a patient visit;
determining a set of functions performed during the patient visit; and
detecting an end of the patient visit;
computing an estimated number of remaining patient visits until the stored charge is depleted; and
generating a remaining visits indicator identifying the estimated number of remaining patient visits.

11. The method of claim 10, further comprising determining a typical set of functions performed from the historical patient visits, and computing an average charge consumption based on the typical set of functions performed.

12. A method of operating a mobile medical instrument, the method comprising:

14

determining a quantity of charge stored in one or more energy storage devices;

storing a history of patient visit charge consumption for a plurality of patient visits;

determining an average charge consumption per patient visit based on the stored history of patient visit charge consumption; and

generating a remaining visits indicator based on the average charge consumption, the remaining visits indicator identifying an estimated number of additional patient visits that can be completed before the energy stored in the one or more energy storage devices is depleted.

13. The method of claim 12, wherein the mobile medical instrument is a multi-function physiological measuring platform device configured to perform more than one function selected from a temperature measurement, a heart rate measurement, a blood pressure measurement, and a blood oxygen level measurement.

14. The method of claim 13, wherein the multi-function physiological measuring platform device includes peripheral components including a thermometer, a blood pressure cuff, and a pulse oximeter.

15. The method of claim 12, wherein the mobile medical instrument further comprises a mobile stand comprising:

a wheeled base including a plurality of wheels; and
a support structure supported on the wheeled base, wherein the support structure is configured to support the mobile measuring device in an elevated position during the patient visits.

16. The method of claim 12, wherein the average charge consumption per patient visit is determined based on a predetermined set size of patients.

17. The method of claim 12, wherein the patient visit charge consumption is determined based on a difference in charge between a stored charge value at the start of a patient visit and a stored charge value at the end of the patient visit.

18. The method of claim 12, wherein the patient visit charge consumption is determined based on a predetermined set of physiological measurements performed on patients during the plurality of patient visits, wherein each physiological measurement of the predetermined set corresponds to a charge consumption value.

19. The method of claim 12, wherein the estimated number of additional patient visits is calculated by dividing the quantity of charge stored in the one or more energy storage devices by the average charge consumption per patient visit.

* * * * *

专利名称(译)	具有剩余访问指标的医疗器械		
公开(公告)号	US9990468	公开(公告)日	2018-06-05
申请号	US15/390177	申请日	2016-12-23
[标]申请(专利权)人(译)	伟伦公司		
申请(专利权)人(译)	伟伦 , INC.		
当前申请(专利权)人(译)	伟伦 , INC.		
[标]发明人	LANE JOHN A MEYERSON CRAIG M FALLAT DAVID M NGUYEN VUONG B ST PIERRE SHAWN C COON III KENNETH V GARRANT MICHAEL D		
发明人	LANE, JOHN A. MEYERSON, CRAIG M. FALLAT, DAVID M. NGUYEN, VUONG B. ST. PIERRE, SHAWN C. COON, III, KENNETH V. GARRANT, MICHAEL D.		
IPC分类号	A61B5/02 G06F19/00 A61B5/0205 A61B5/1455 A61B5/00 A61B5/022 A61B5/024		
CPC分类号	A61B5/02055 A61B5/14552 A61B5/742 G16H40/20 G16H40/40 A61B5/022 A61B2560/0204 A61B2560/0437 A61B5/024 A61B5/021 G06F19/327 G06F19/3412 G06F19/00		
代理机构(译)	商户德律P.C.		
其他公开文献	US20170109489A1		
外部链接	Espacenet USPTO		

摘要(译)

医疗器械包括剩余的访问指示器。剩余的访问指示器在视觉上识别可以在对医疗器械充电之前完成的患者访问的数量。

