



US 20170055851A1

(19) **United States**

(12) **Patent Application Publication**
Al-Ali

(10) **Pub. No.: US 2017/0055851 A1**
(43) **Pub. Date: Mar. 2, 2017**

(54) **PATIENT-WORN WIRELESS
PHYSIOLOGICAL SENSOR**

A61B 5/0408 (2006.01)
A61B 5/113 (2006.01)

(71) Applicant: **Masimo Corporation**, Irvine, CA (US)

(52) **U.S. Cl.**
CPC *A61B 5/02055* (2013.01); *A61B 5/0408*
(2013.01); *A61B 5/1116* (2013.01); *A61B*
5/1117 (2013.01); *A61B 5/113* (2013.01);
A61B 5/0022 (2013.01); *A61B 5/05* (2013.01);
A61B 5/053 (2013.01); *A61B 5/447* (2013.01);
A61B 5/743 (2013.01); *A61B 5/14552*
(2013.01); *A61B 5/746* (2013.01)

(72) Inventor: **Ammar Al-Ali**, San Juan Capistrano,
CA (US)

(21) Appl. No.: **15/253,536**

(22) Filed: **Aug. 31, 2016**

Related U.S. Application Data


(60) Provisional application No. 62/212,467, filed on Aug. 31, 2015, provisional application No. 62/212,472, filed on Aug. 31, 2015, provisional application No. 62/212,484, filed on Aug. 31, 2015, provisional application No. 62/212,480, filed on Aug. 31, 2015.

Publication Classification

(51) **Int. Cl.**
A61B 5/0205 (2006.01)
A61B 5/11 (2006.01)
A61B 5/1455 (2006.01)
A61B 5/00 (2006.01)
A61B 5/05 (2006.01)
A61B 5/053 (2006.01)

(57) **ABSTRACT**

A wireless, patient-worn, physiological sensor configured to, among other things, help manage a patient that is at risk of forming one or more pressure ulcers is disclosed. According to an embodiment, the sensor includes a base having a top surface and a bottom surface. The sensor also includes a substrate layer including conductive tracks and connection pads, a top side, and a bottom side, where the bottom side of the substrate layer is disposed above the top side of the base. Mounted on the substrate layer are a processor, a data storage device, a wireless transceiver, an accelerometer, and a battery. In use, the sensor senses a patient's motion and wirelessly transmits information indicative of the sensed motion to, for example, a patient monitor. The patient monitor receives, stores, and processes the transmitted information.

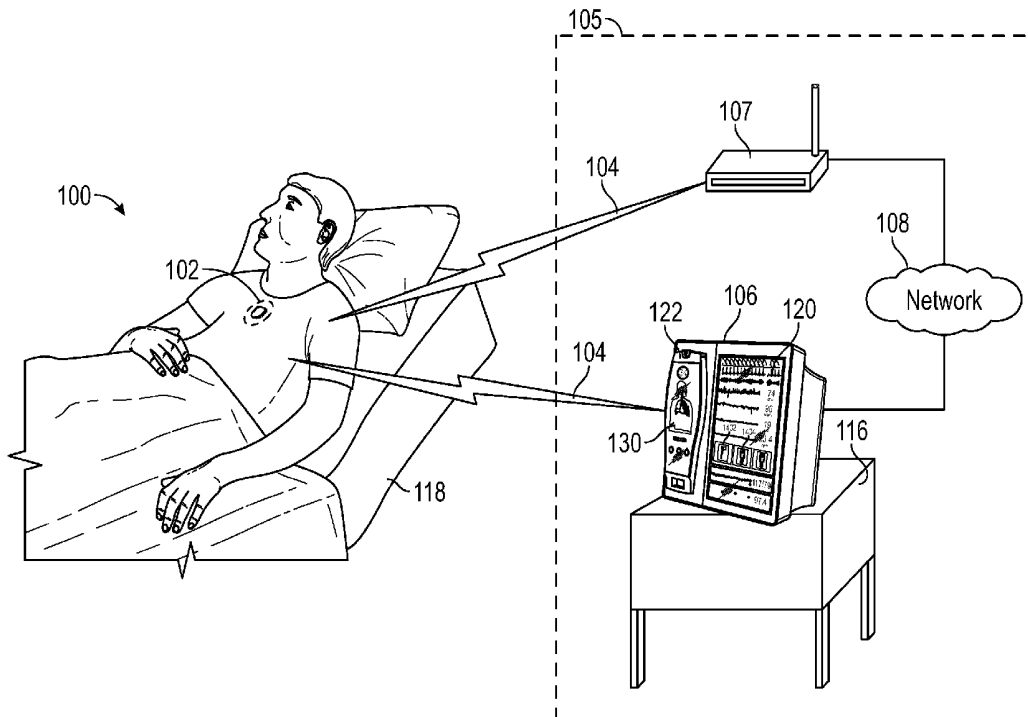

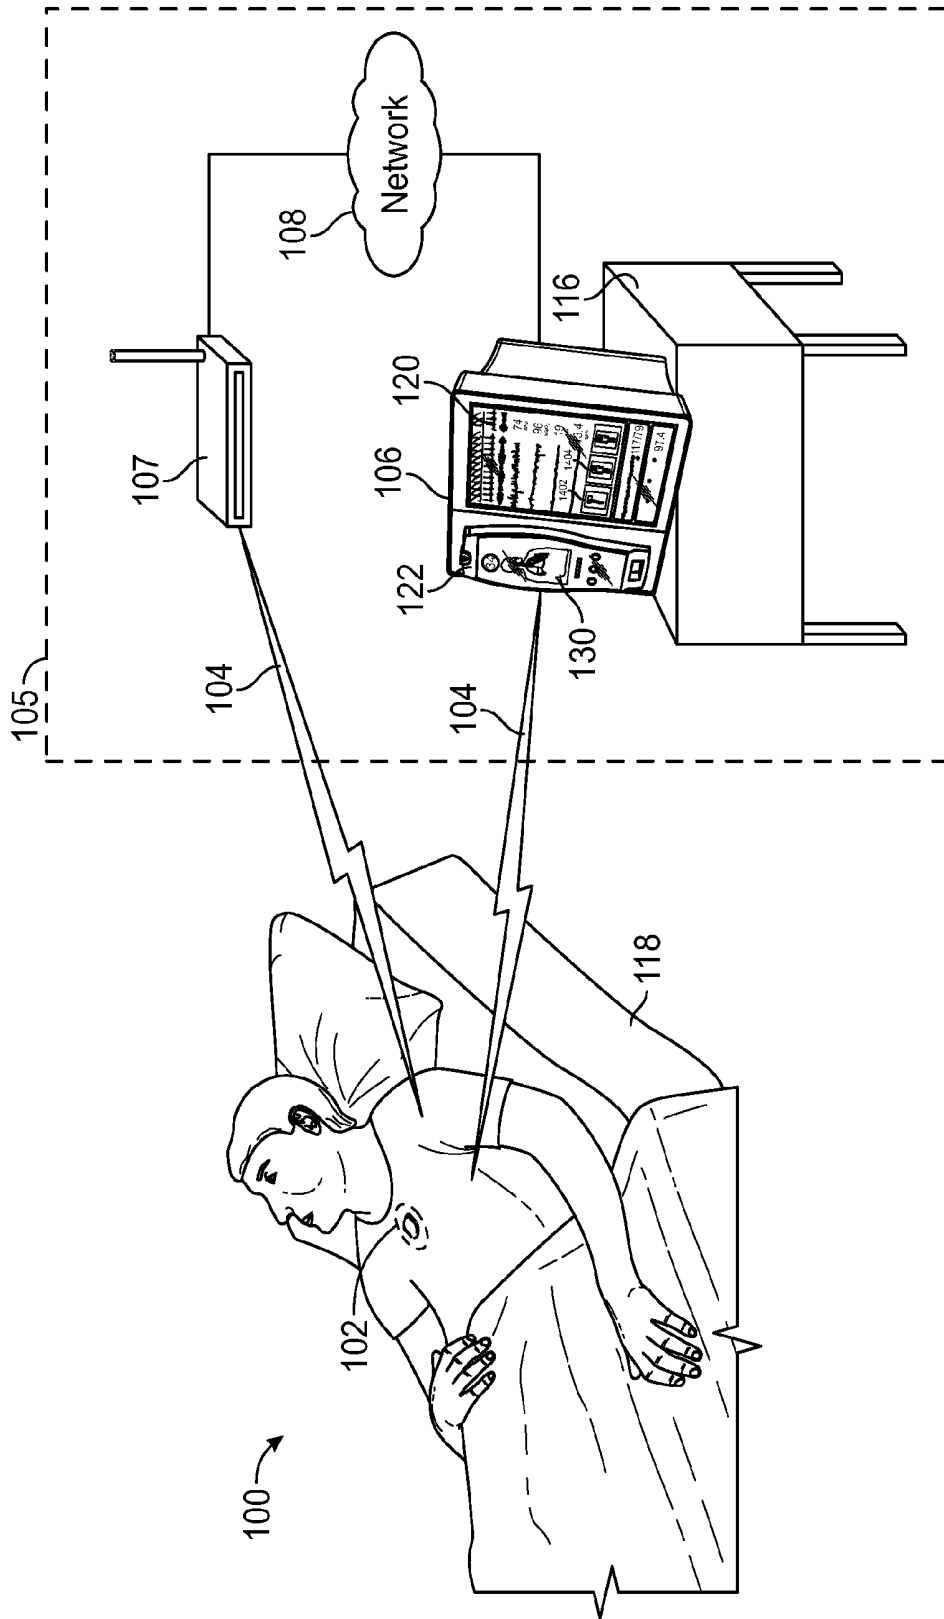


FIG. 1A

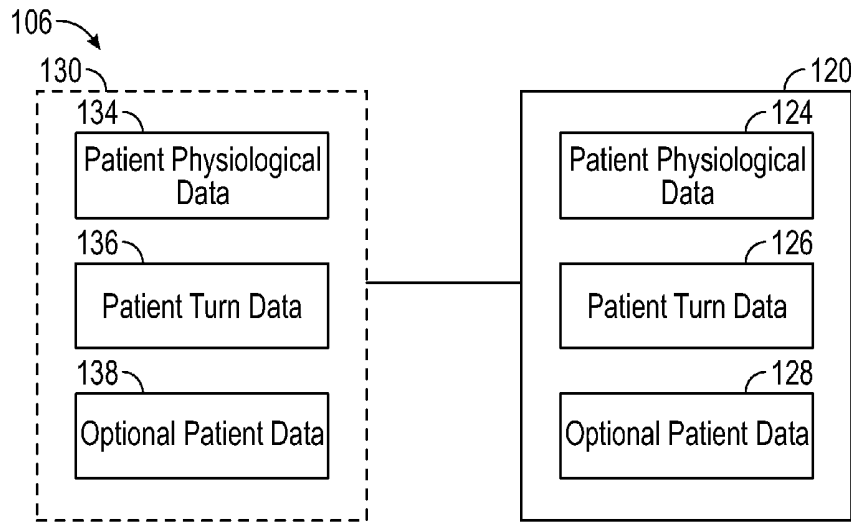


FIG. 1B

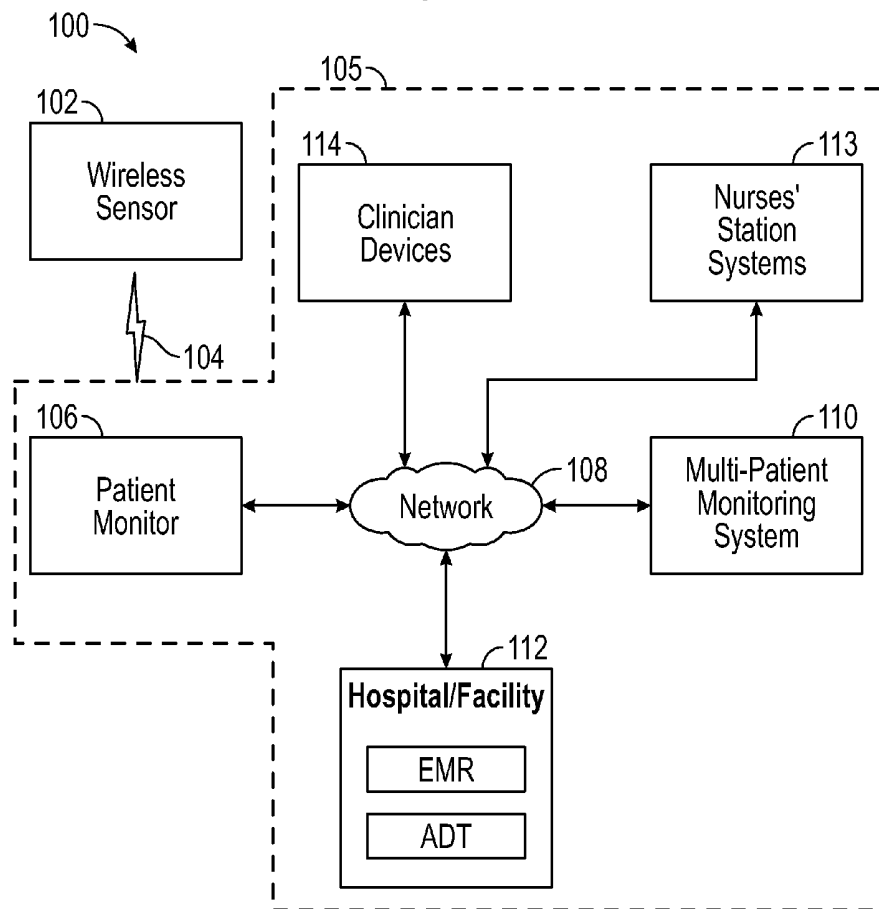


FIG. 1C

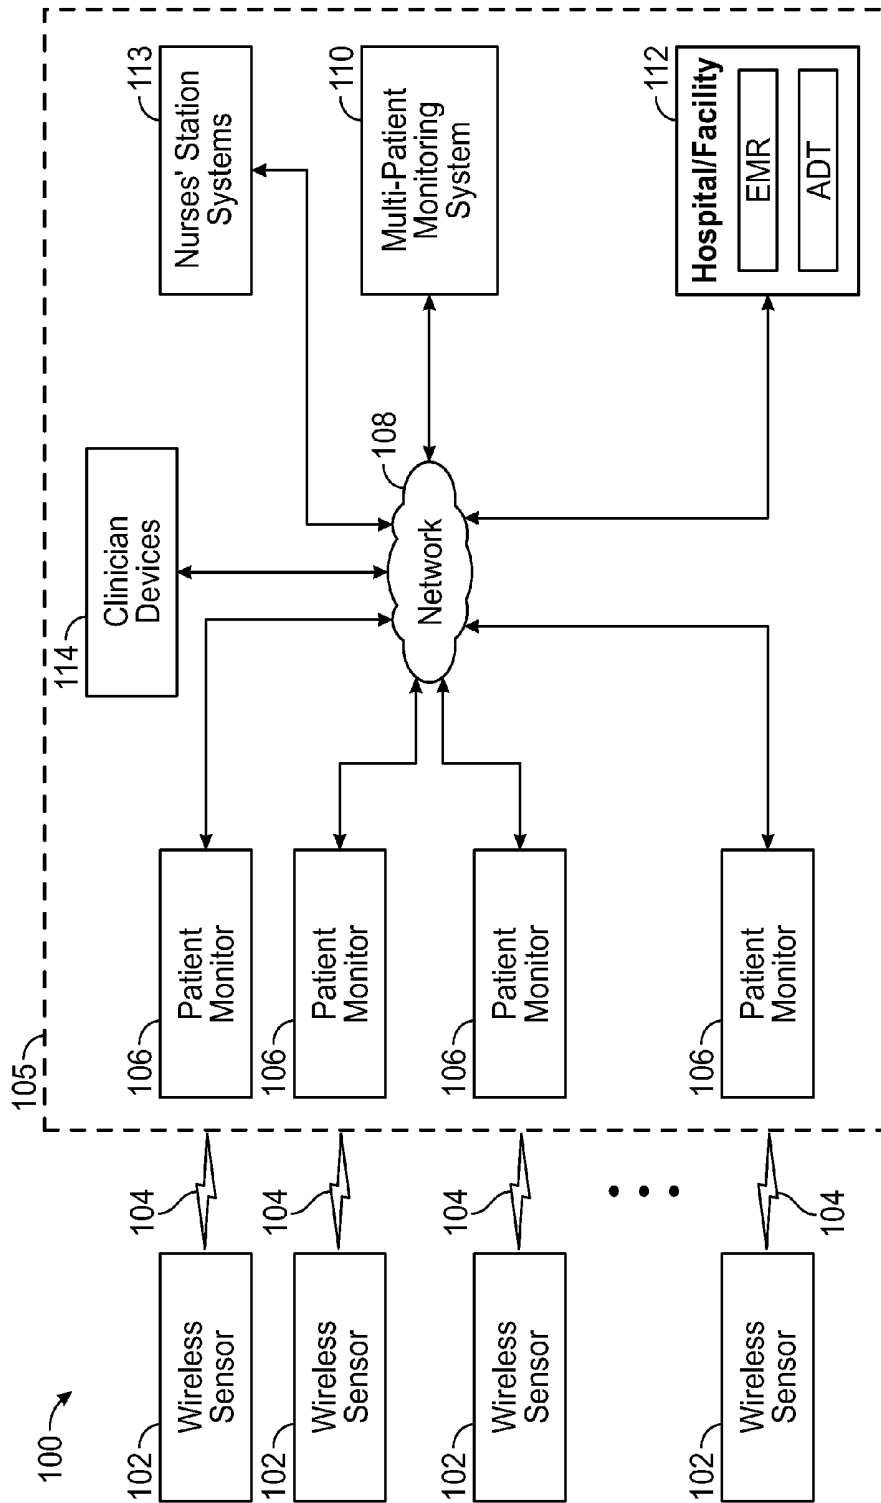


FIG. 1D

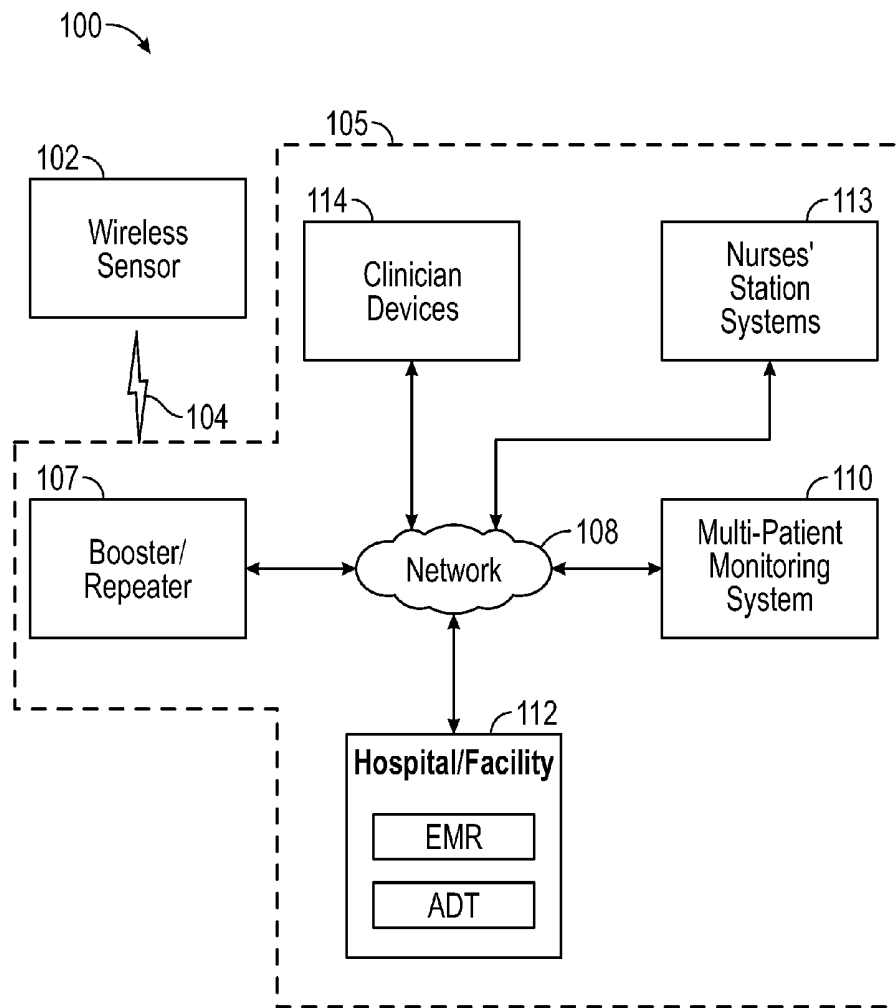


FIG. 1E

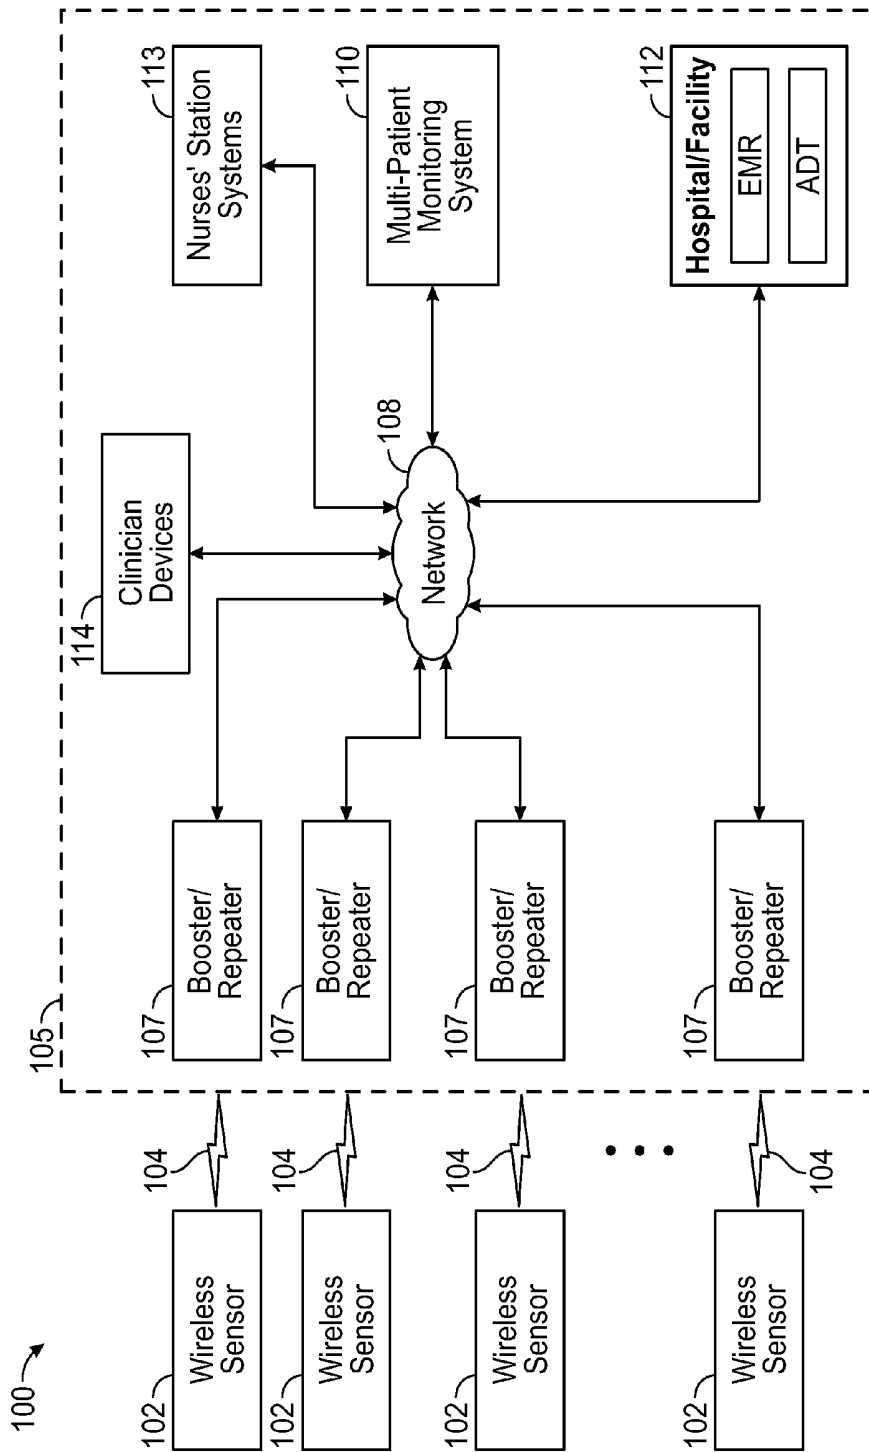


FIG. 1F

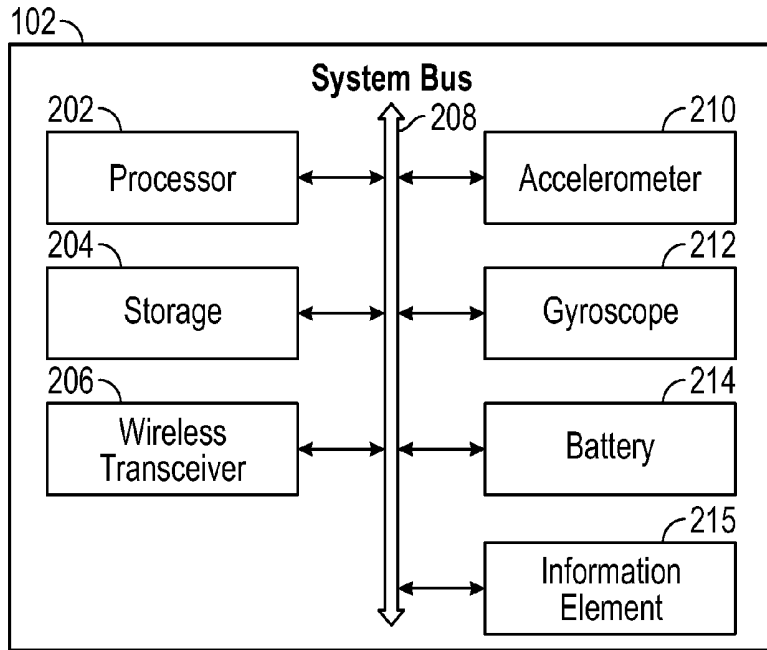


FIG. 2A

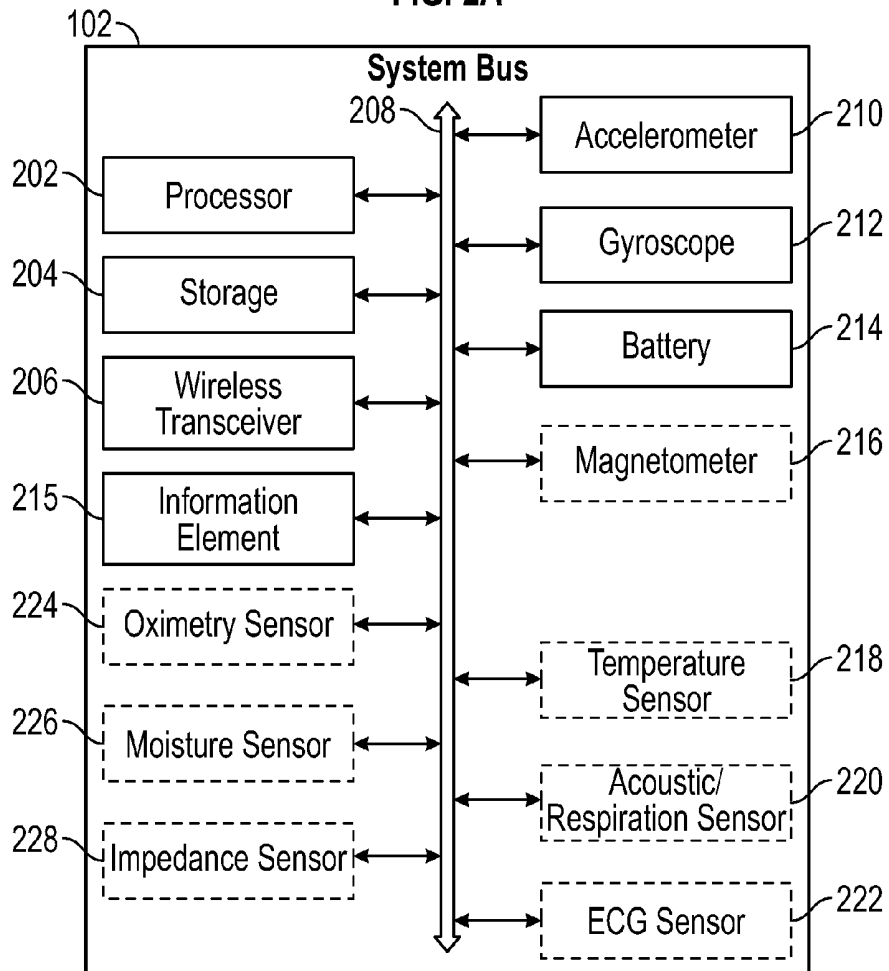


FIG. 2B

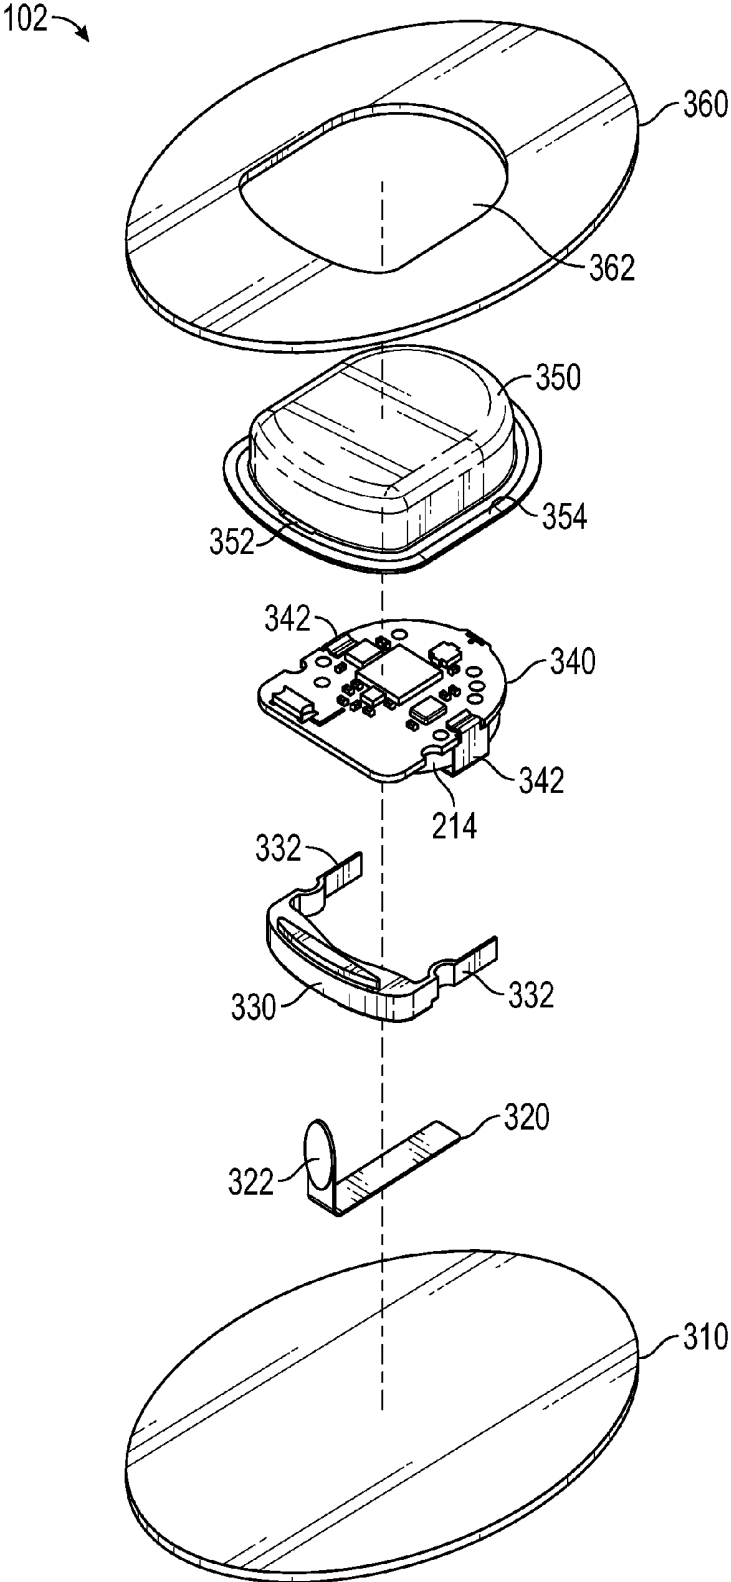


FIG. 3A

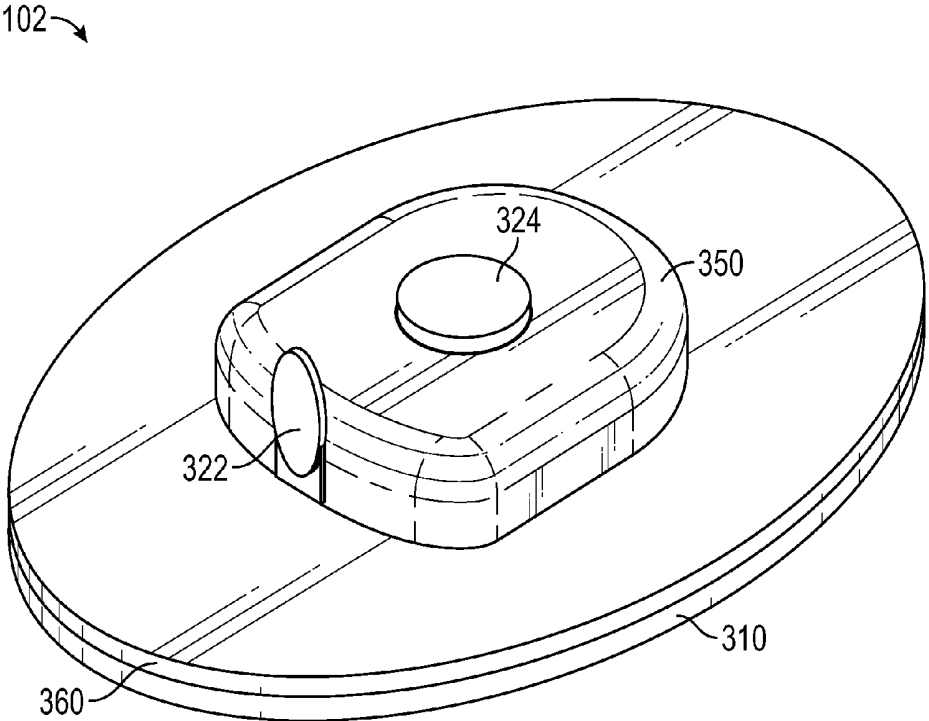


FIG. 3B

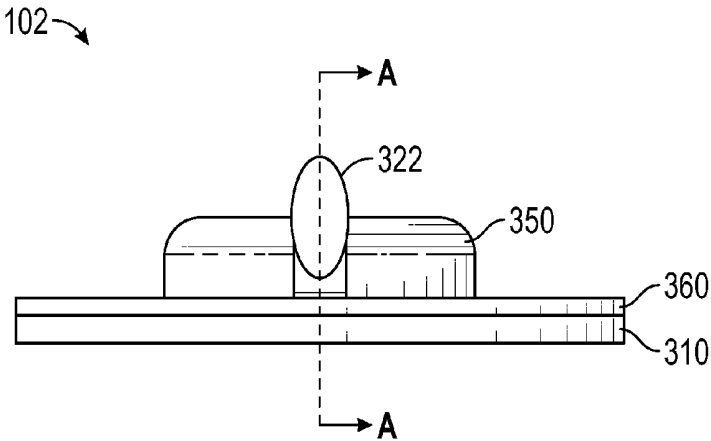


FIG. 3C

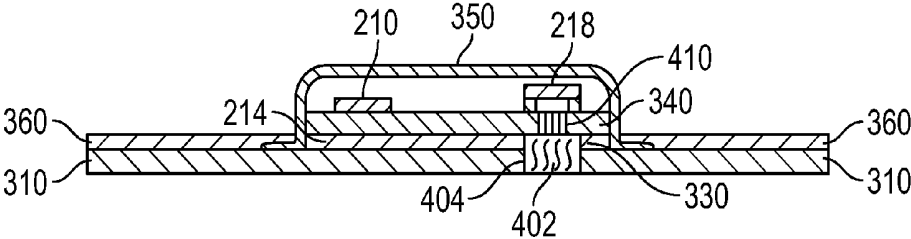


FIG. 4A

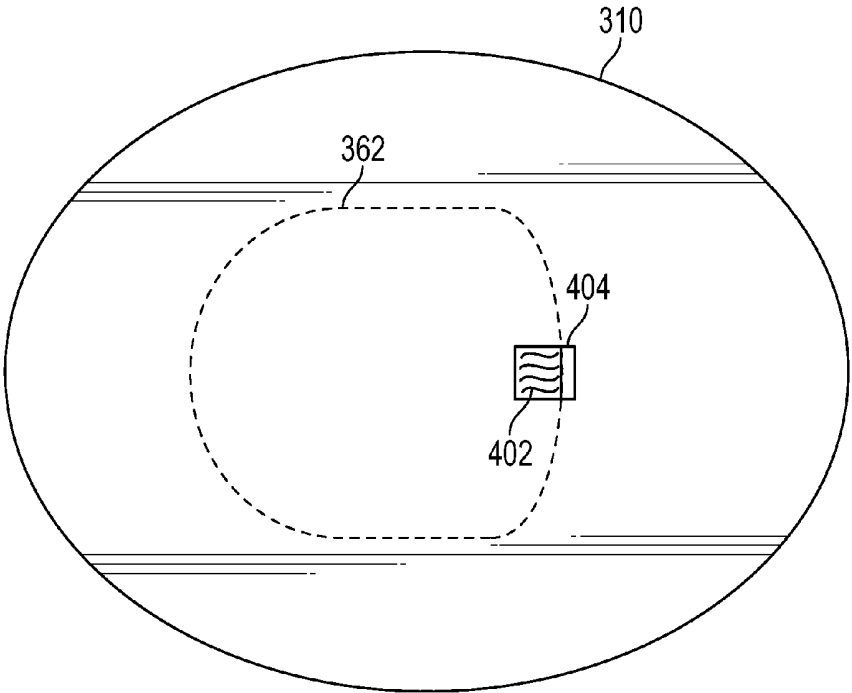


FIG. 4B

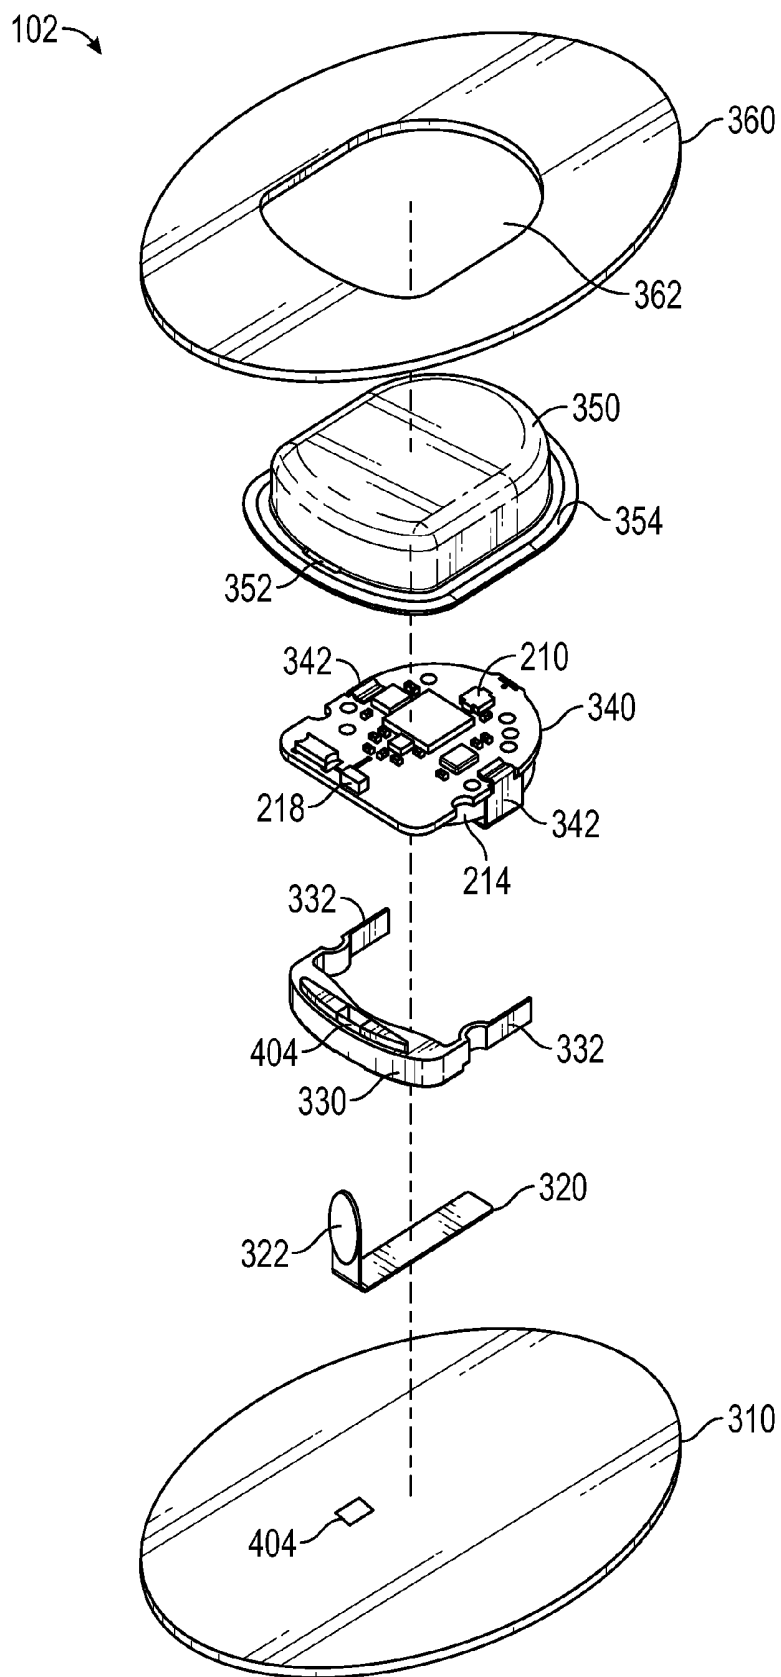


FIG. 4C

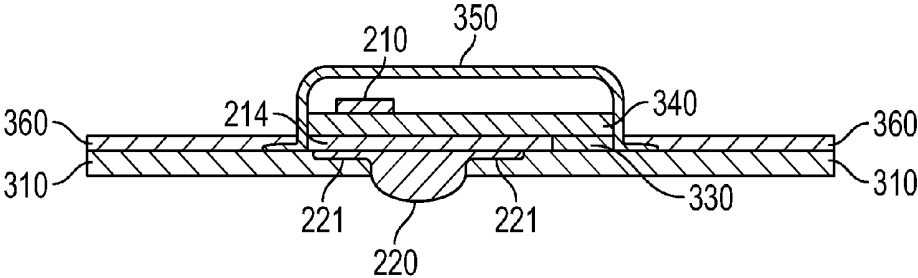


FIG. 5A

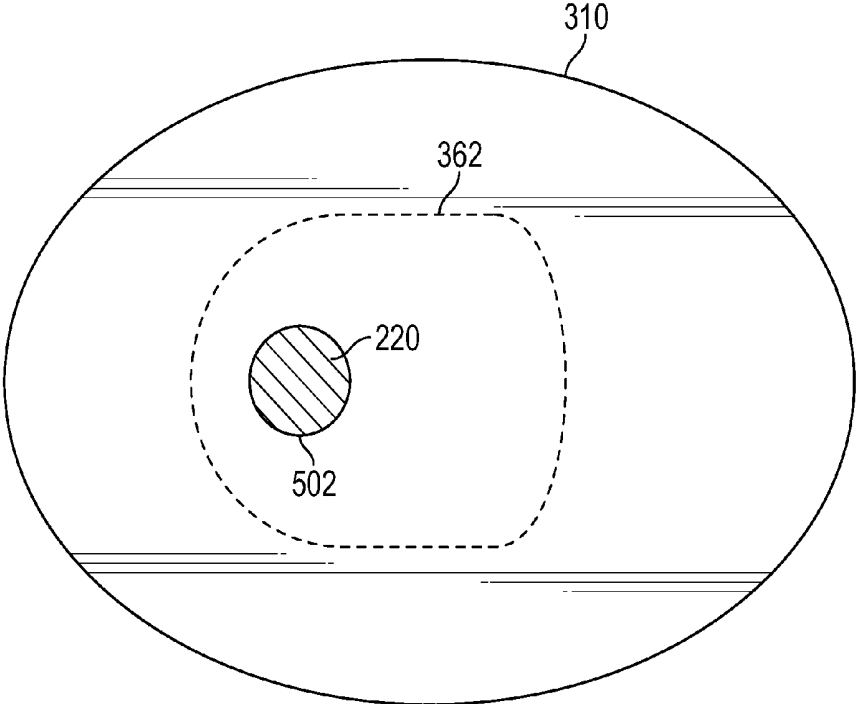


FIG. 5B

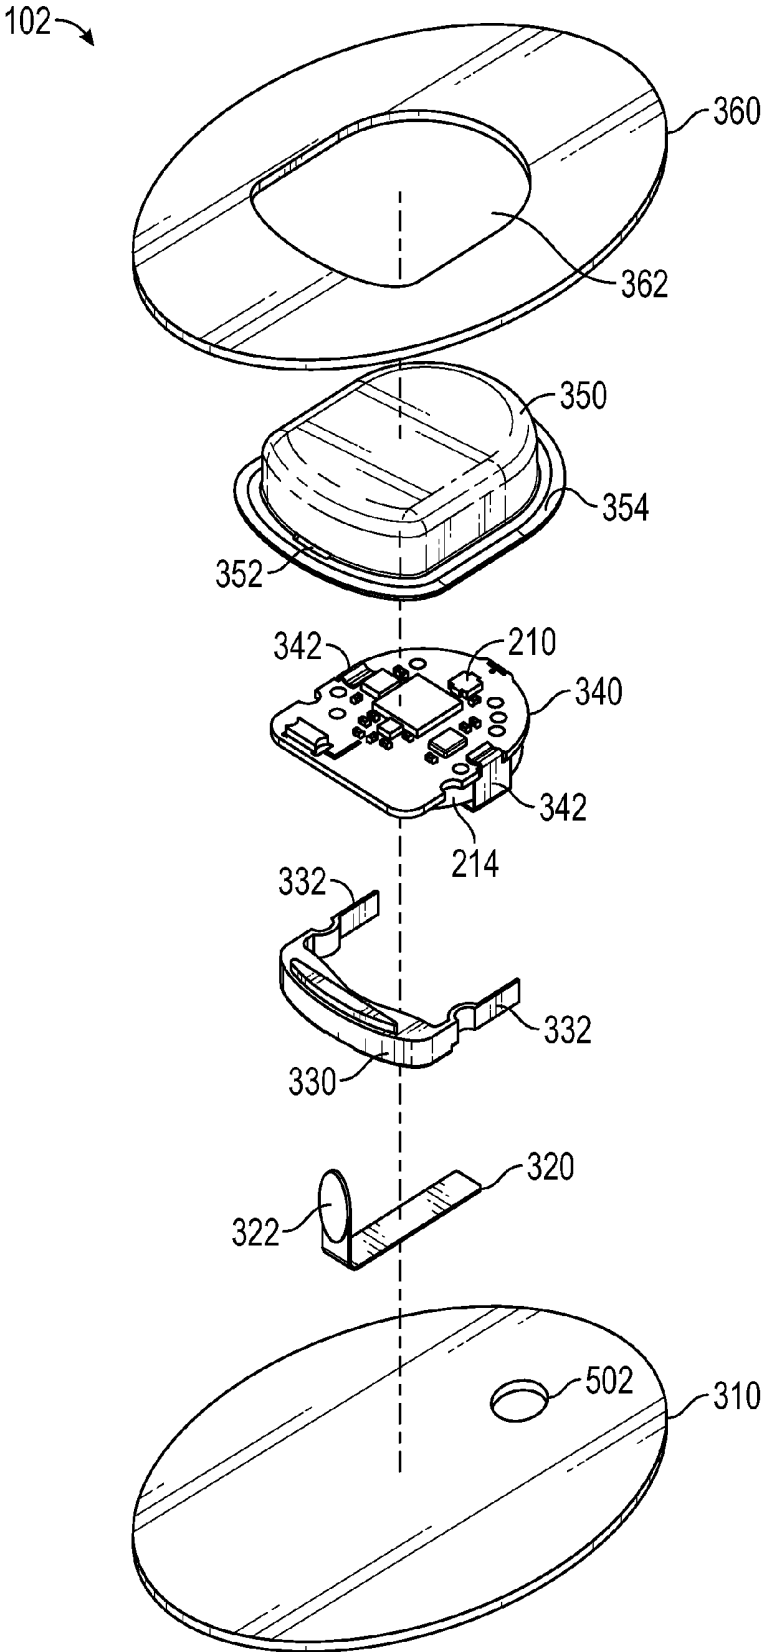


FIG. 5C

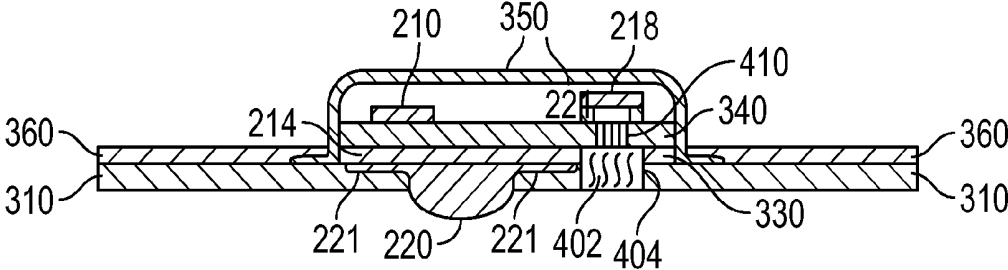


FIG. 6A

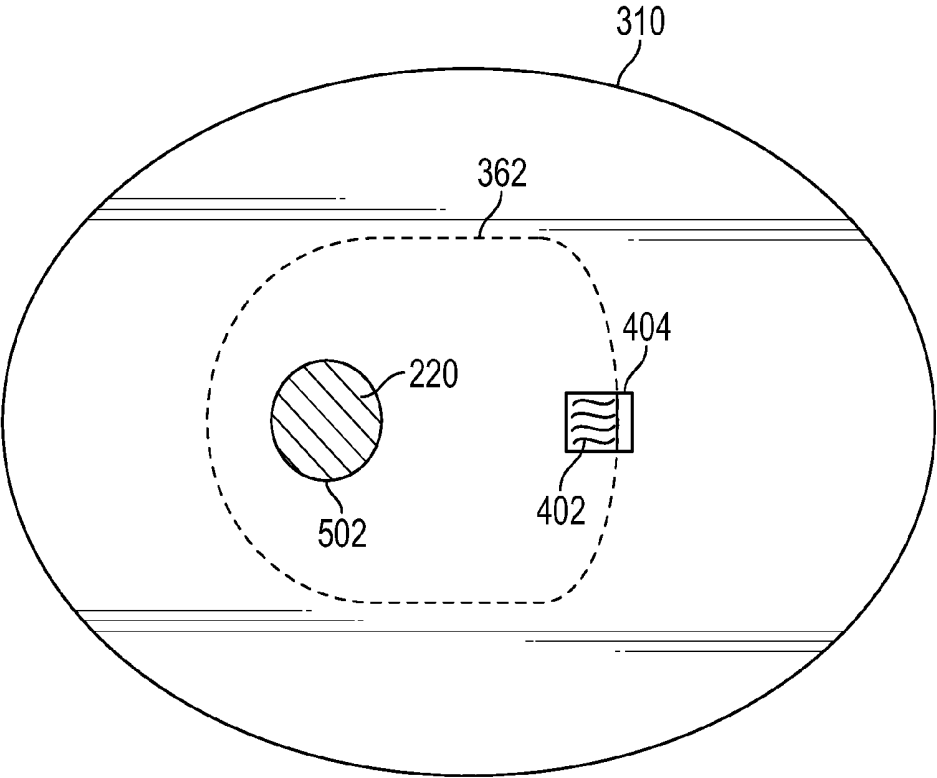


FIG. 6B

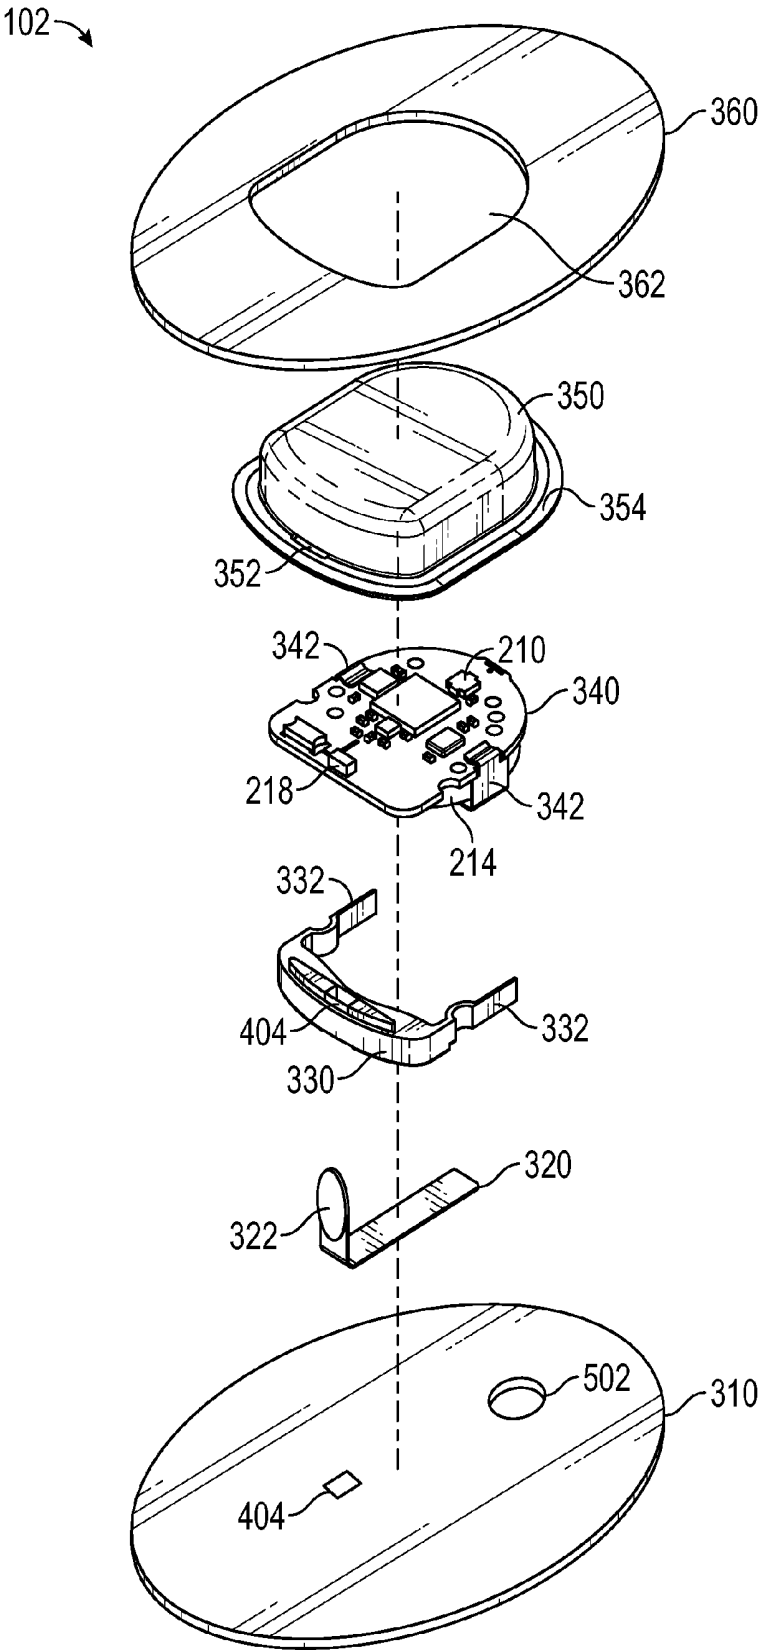


FIG. 6C

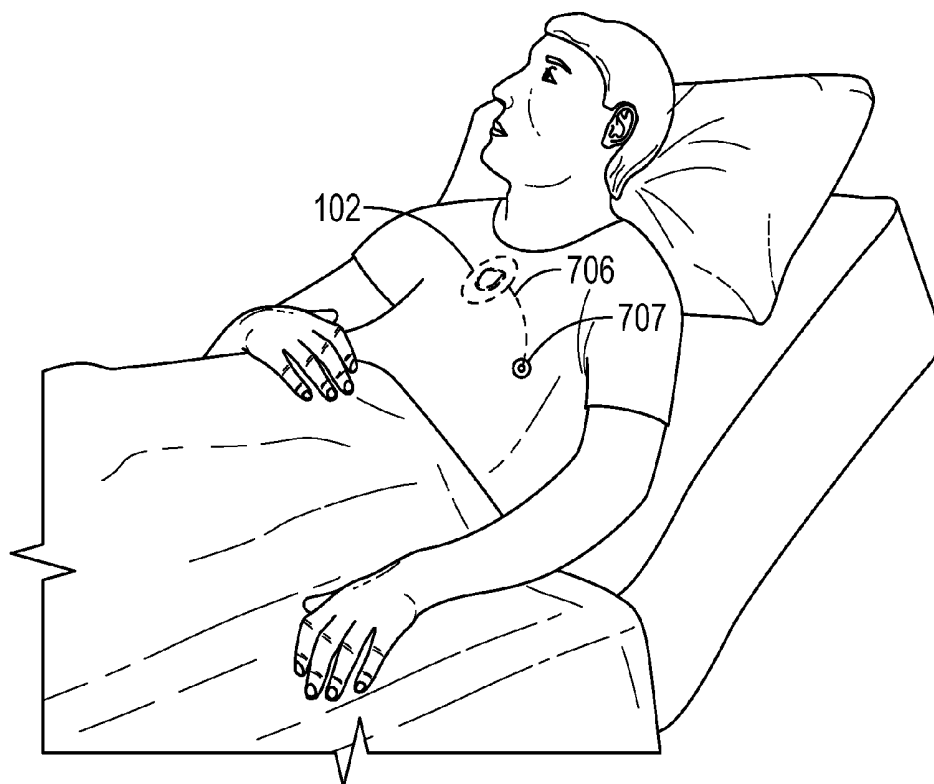


FIG. 7A

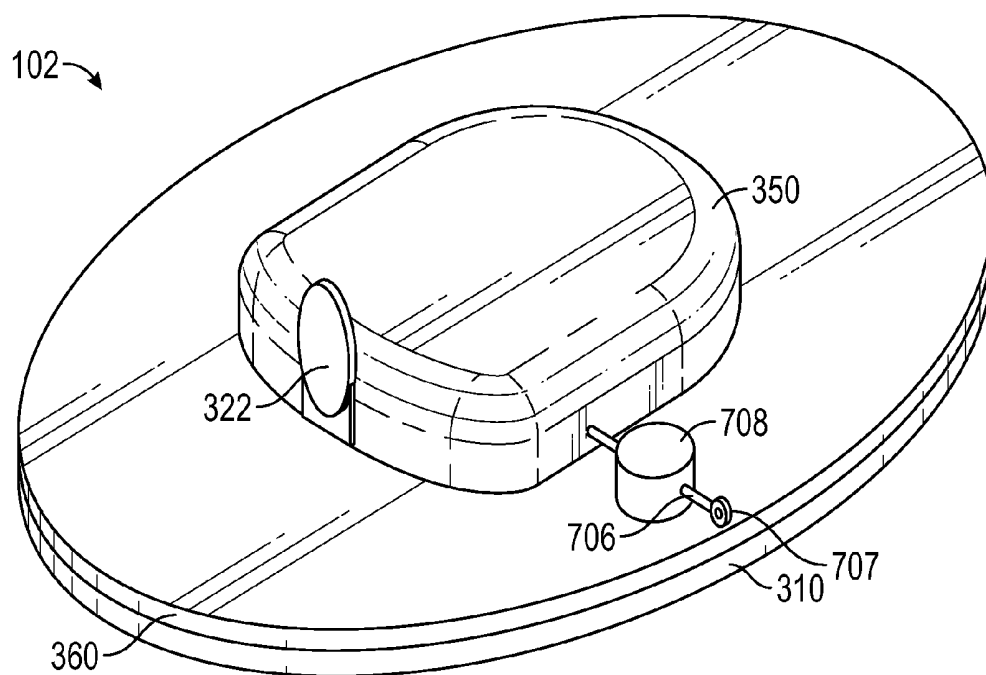


FIG. 7B

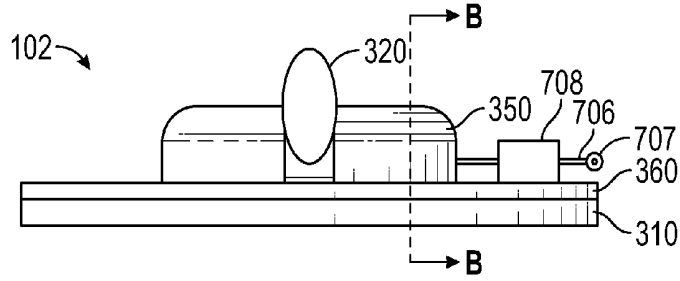


FIG. 7C

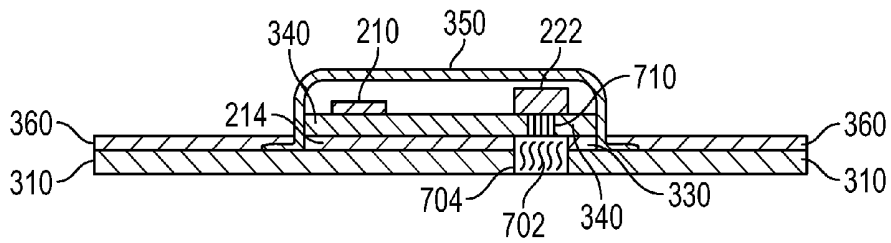


FIG. 7D

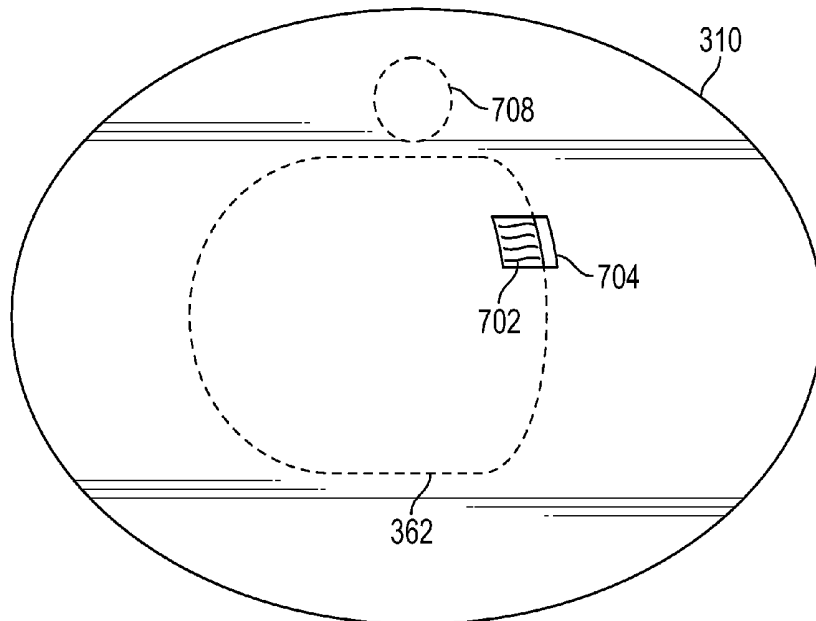


FIG. 7E

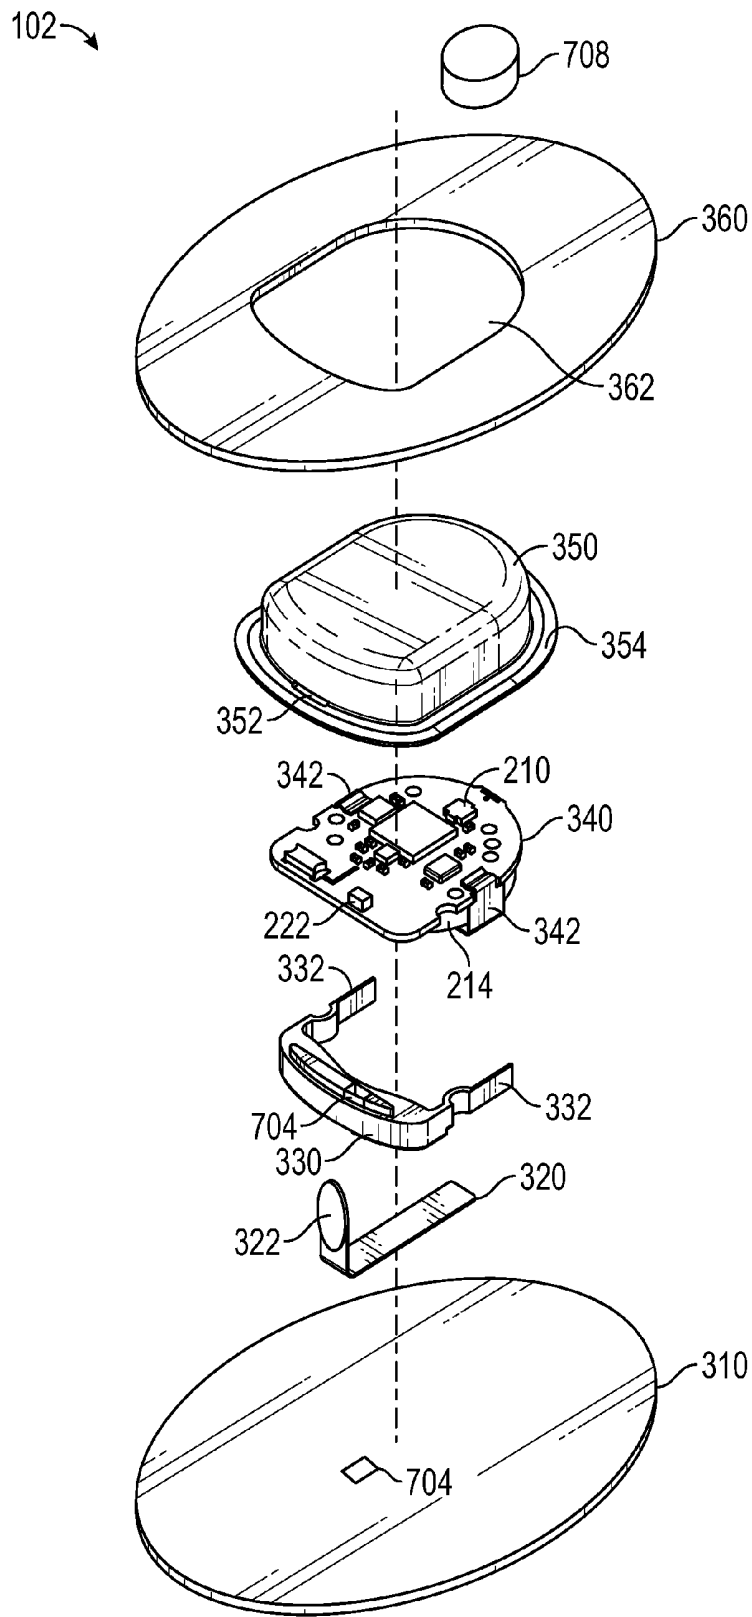


FIG. 7F

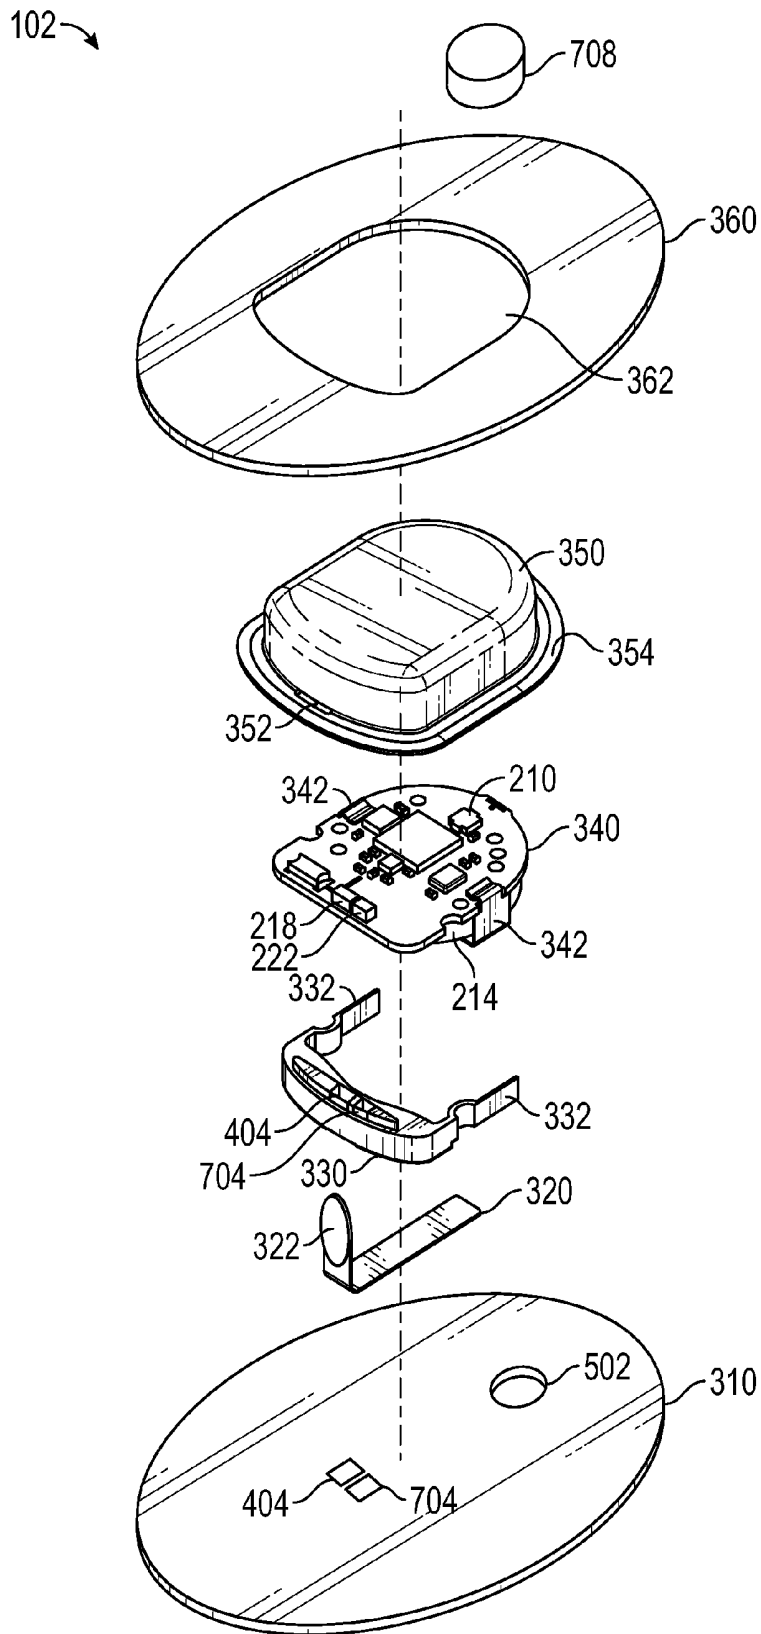


FIG. 8A

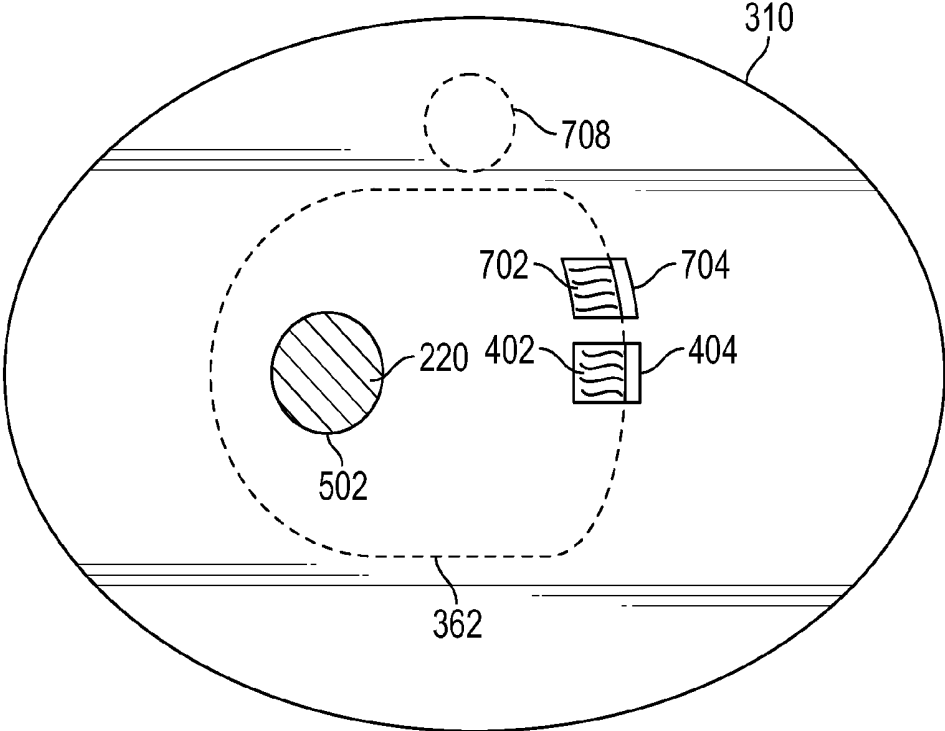


FIG. 8B

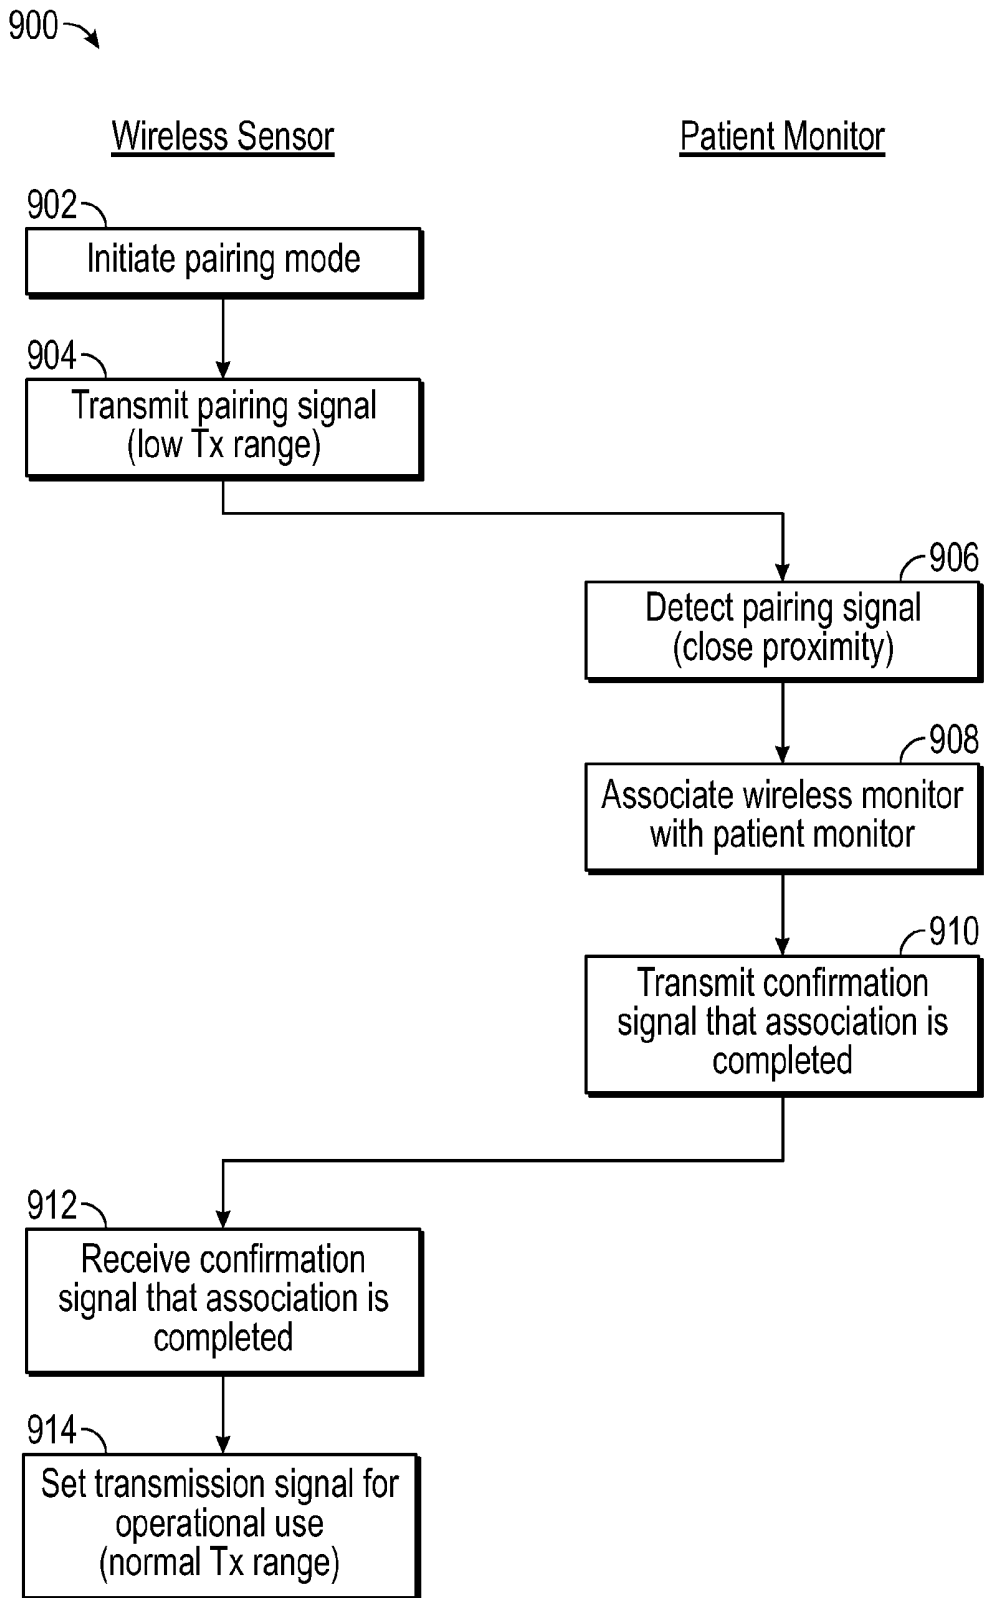


FIG.9

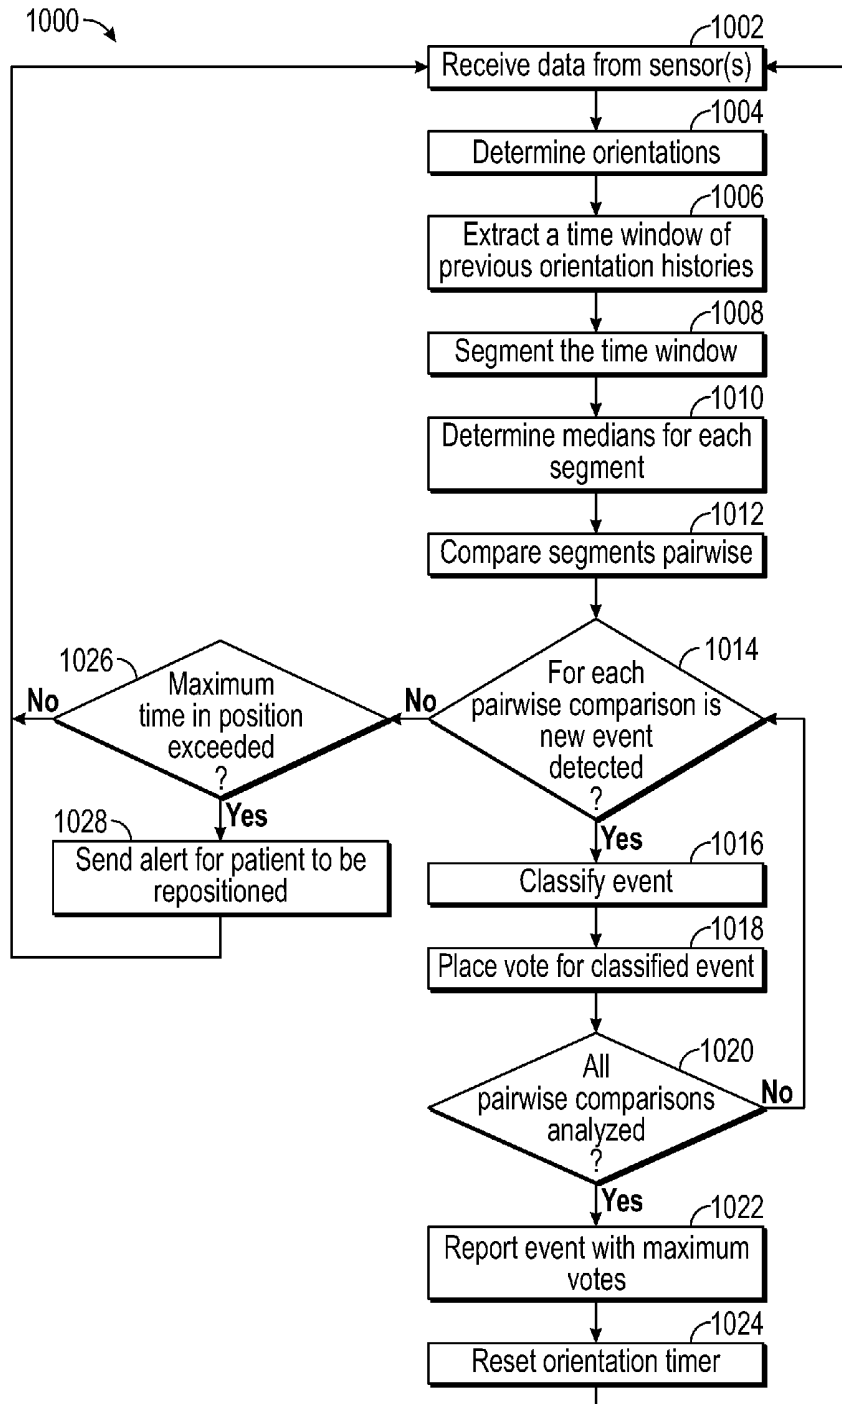


FIG. 10

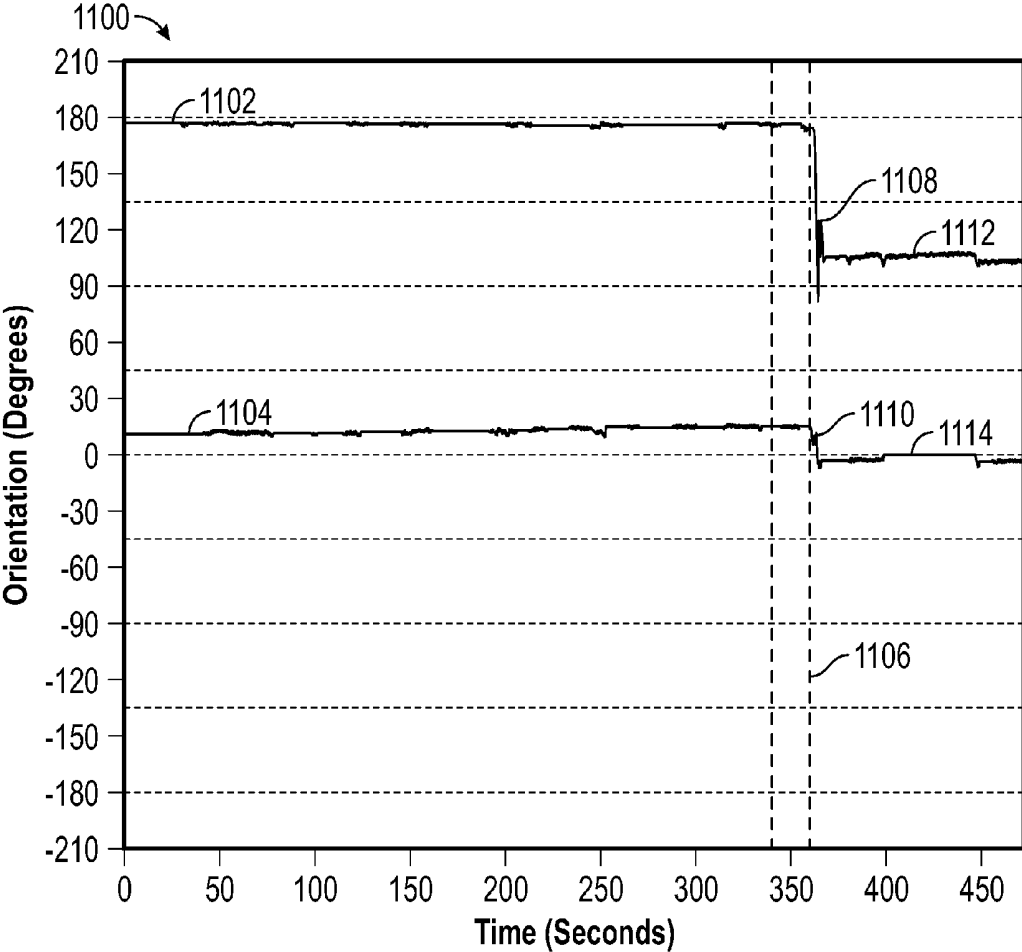
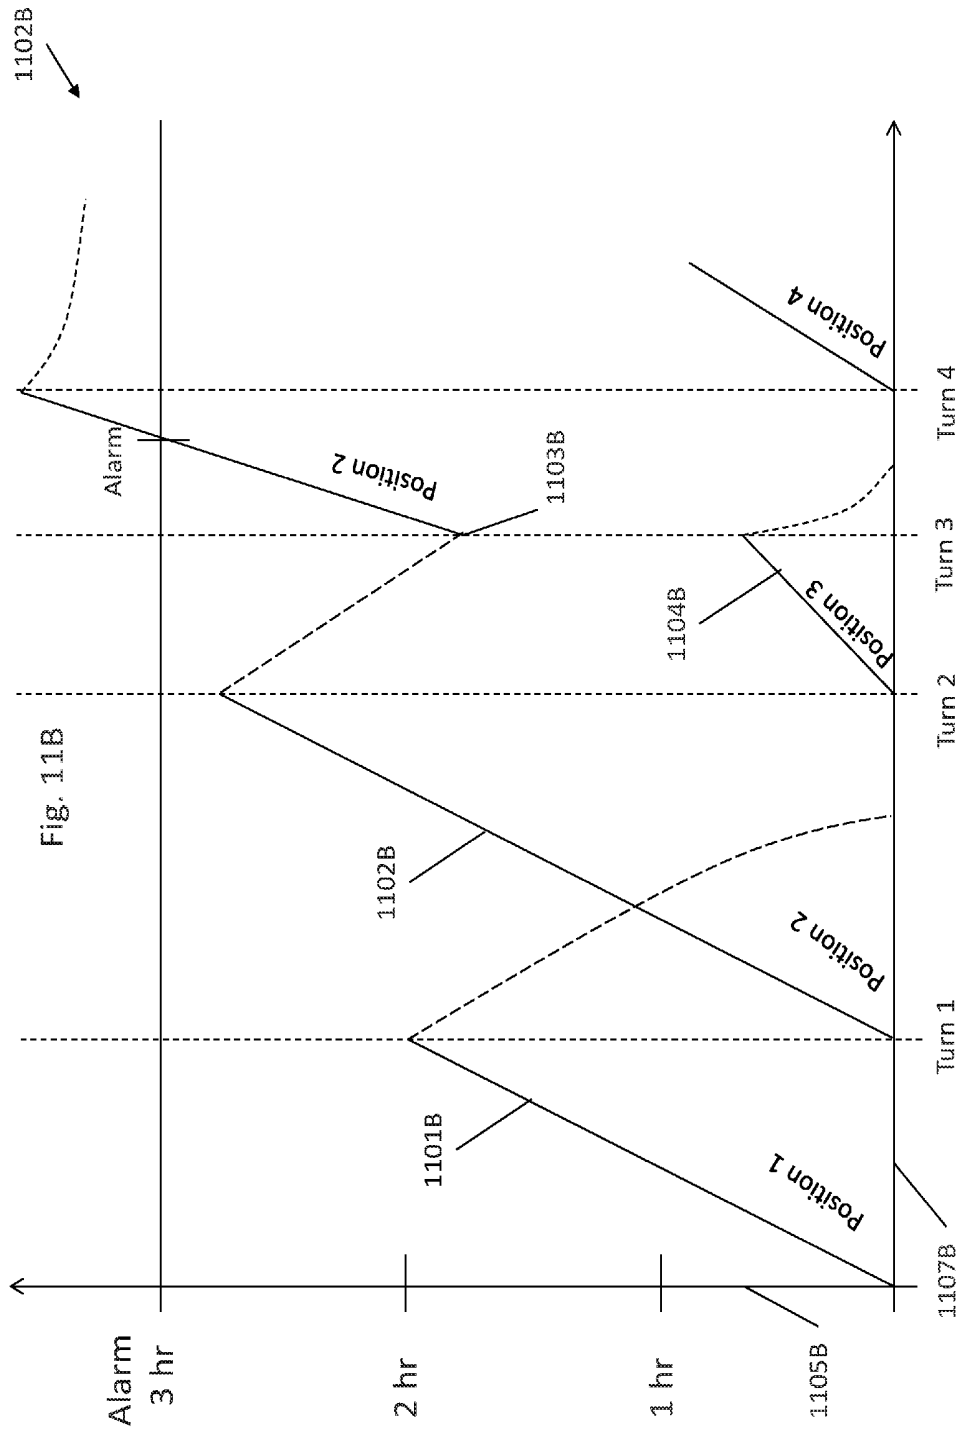


FIG.11A



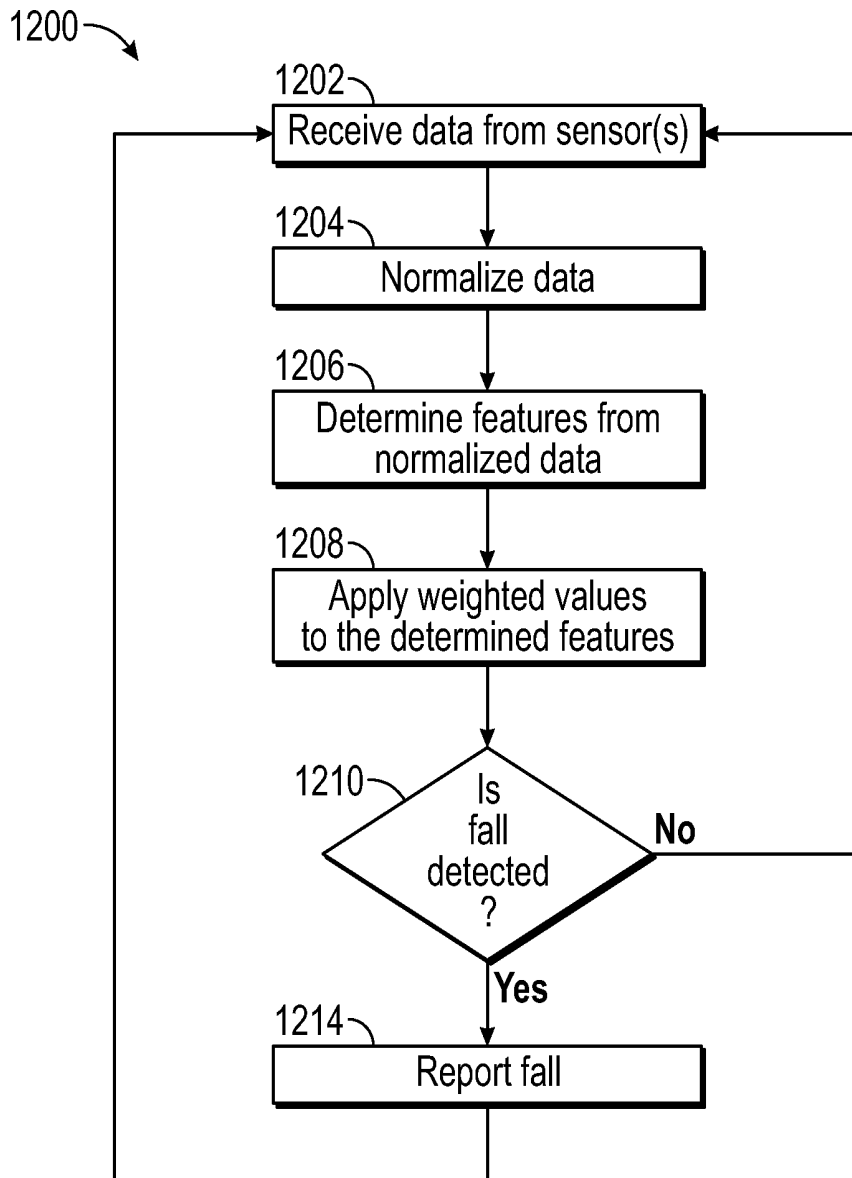


FIG.12

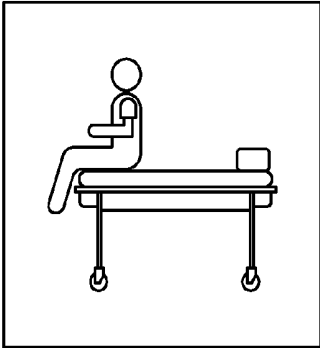


FIG. 13A

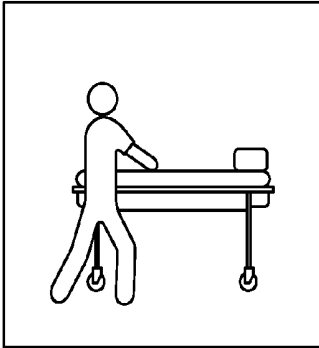


FIG. 13B

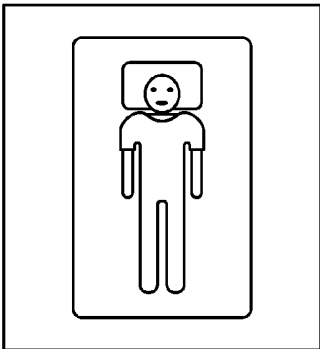


FIG. 13C

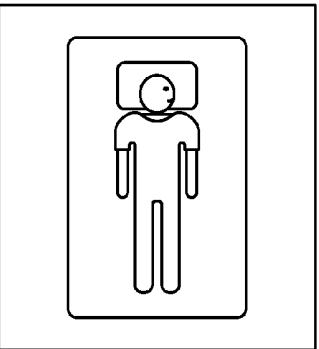


FIG. 13D

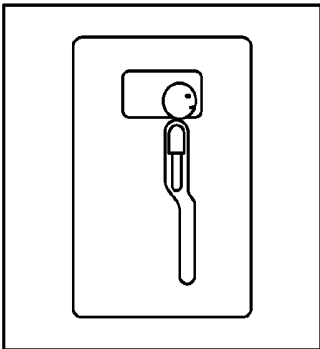


FIG. 13E

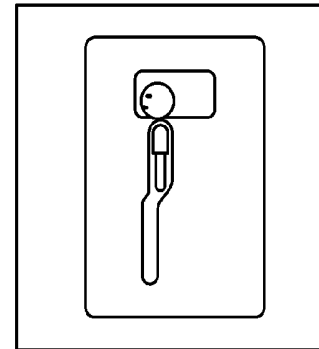


FIG. 13F

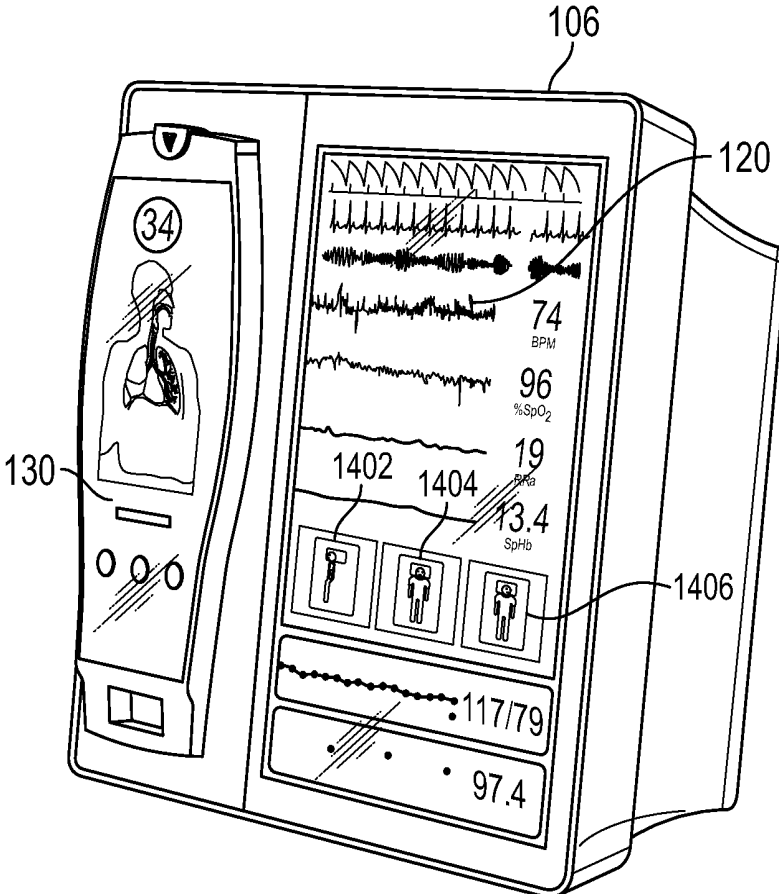


FIG. 14

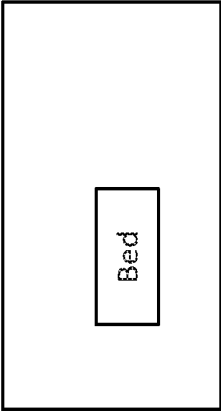


Fig. 15A

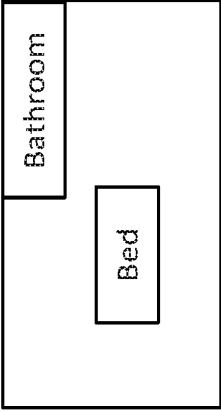


Fig. 15E

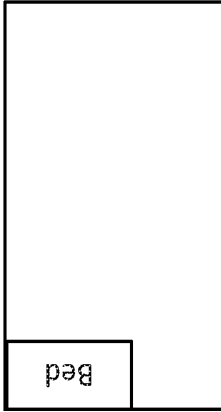


Fig. 15B



Fig. 15F

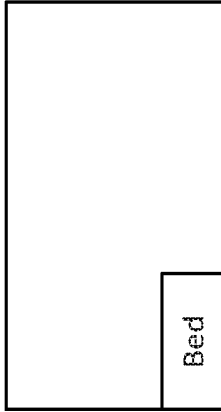


Fig. 15C

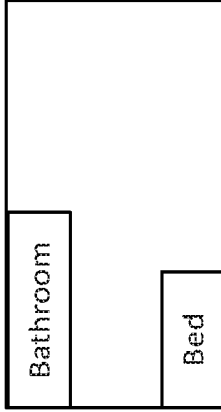


Fig. 15G

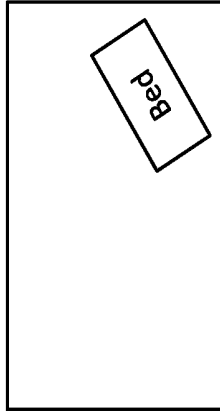


Fig. 15D

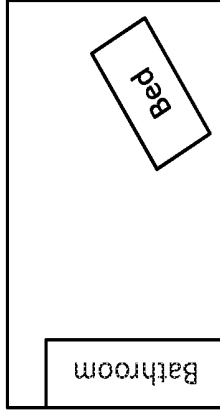


Fig. 15H

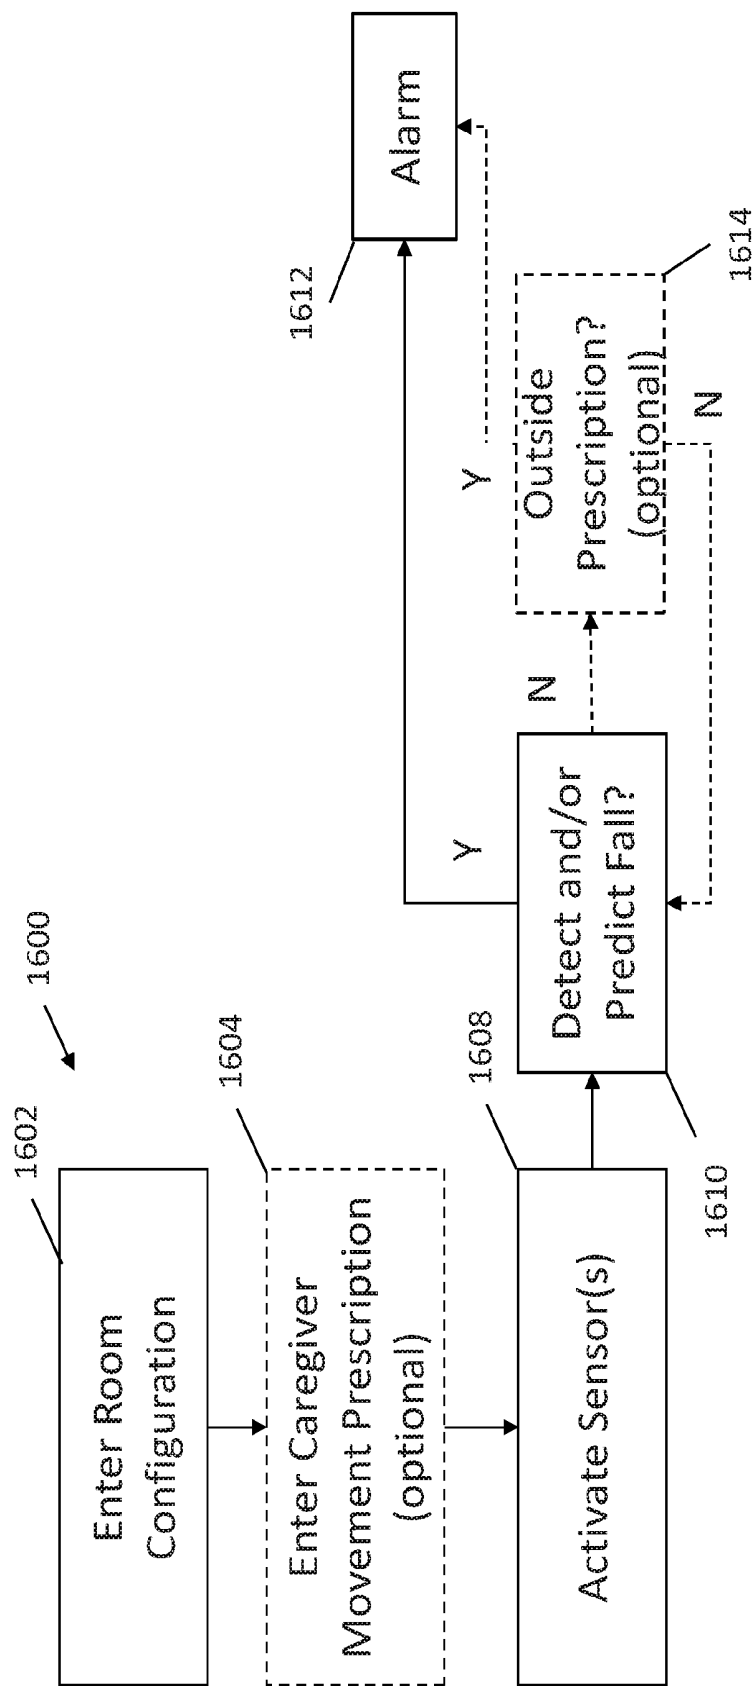


Fig. 16

**PATIENT-WORN WIRELESS
PHYSIOLOGICAL SENSOR****INCORPORATION BY REFERENCE TO ANY
PRIORITY APPLICATIONS**

[0001] The present application claims priority benefit under 35 U.S.C. §119(e) to U.S. Provisional Application No. 62/212,467, filed Aug. 31, 2015, U.S. Provisional Application No. 62/212,472, filed Aug. 31, 2015, U.S. Provisional Application No. 62/212,484, filed Aug. 31, 2015, and U.S. Provisional Application No. 62/212,480, filed Aug. 31, 2015, which are hereby incorporated by reference herein in entirety.

FIELD OF THE DISCLOSURE

[0002] The present disclosure relates to the field of patient monitoring. More specifically, the disclosure describes among other things a wearable sensor that measures a patient's position, orientation, and movement and wirelessly communicates the measured information to a patient monitoring system.

BACKGROUND

[0003] In clinical settings, such as hospitals, nursing homes, convalescent homes, skilled nursing facilities, post-surgical recovery centers, and the like, patients are frequently confined to bed for extended periods of time. Sometimes the patients are unconscious or sedated to such an extent that they have limited ability to change or control their position in the bed. These patients can be at risk of forming pressure ulcers, which pose a serious risk to the patient's health and well-being. Pressure ulcers, which may also be referred to as "bed sores," "pressure sores," and "decubitus ulcers," comprise injury to a patient's skin, and often the underlying tissue, which results from prolonged pressure forces applied to a site on the patient's body. Frequently, pressure ulcers develop on skin that covers bony areas of the body which have less muscle and/or fat tissue below the surface to distribute pressure applied thereto resulting from prolonged contact with the surface of a bed or chair. Examples of such body locations include the back or side of the head, shoulders, shoulder blades, elbows, spine, hips, lower back, tailbone, heels, ankles, and skin behind the knees.

[0004] Pressure ulcers are caused by application of pressure at an anatomical site that occludes blood flow to the skin and other tissue near the location. Sustained pressure between a structural surface (such as a bed) and a particular point on the patient's body can restrict blood flow when the applied pressure is greater than the blood pressure flowing through the capillaries that deliver oxygen and other nutrients to the skin and other tissue. Deprived of oxygen and nutrients, the skin cells can become damaged, leading to tissue necrosis in as few as 2 to 6 hours. Despite commonly occurring in elderly and mobility-impaired populations, hospital-acquired pressure ulcers are considered to be preventable and have been termed "never events." Insurers have imposed restrictions on the amount they will reimburse a hospital for pressure ulcer treatment, and state and federal legislation now requires hospitals to report the occurrence of pressure ulcers in their facilities.

[0005] Risk factors for pressure ulcers can be categorized as modifiable and non-modifiable. Modifiable risk factors

include actions that healthcare providers can take, while non-modifiable risk factors include aspects of patient health and behavior. It is valuable to document such non-modifiable risk factors so that caregivers can identify and attend to patients at risk of developing pressure ulcers. It is recommended that caregivers develop a documented risk assessment policy to predict the risk of a patient developing a pressure ulcer. Such an assessment can encompass all aspects of a patient's health and environment, and may employ commonly used measures in the field, such as the Braden and Norton scales. The risk assessment tool may be used to direct preventative strategies not only when a patient is at rest in his or her bed, but also when undergoing surgery.

[0006] Additional factors that can contribute to the formation of pressure ulcers include friction and shear forces. Friction can occur when skin is dragged across a surface which can happen when patients are moved, especially when the skin is moist. Such frictional forces can damage the skin and make it more vulnerable to injury, including formation of a pressure ulcer. A shear is when two forces move in opposite directions. For example, when the head portion of a bed is elevated at an incline, the patient's spine, tailbone, and hip regions tend to slide downward due to gravity. As the bony portion of the patient's body moves downward, the skin covering the area can stay in its current position, thereby pulling in the opposite direction of the skeletal structure. Such shear motion can injure the skin and blood vessels at the site, causing the skin and other local tissue to be vulnerable to formation of a pressure ulcer.

[0007] An established practice for patients at risk of forming pressure ulcers is to follow a turning protocol by which the patient is periodically repositioned, or "turned" to redistribute pressure forces placed on various points of the patient's body. Individuals at risk for a pressure ulcer are repositioned regularly. It is commonly suggested that patients be repositioned every 2 hours at specific inclination angles, and that the method of doing so minimizes the amount of friction and shear on the patient's skin. A repositioning log can be maintained and include key information, such as the time, body orientation, and outcome.

[0008] Pressure ulcer prevention programs have been effective and can reduce long-term costs associated with treatment. A 2002 study employed a comprehensive prevention program in two long-term care facilities, costing \$519.73 per resident per month. Results of the program revealed pressure ulcer prevalence to be reduced by 87% and 76% in the two facilities. A later study found that prevention strategies were able to reduce pressure ulcer prevalence from 29.6% to 0% in a medical intensive care unit, and from 9.2% to 6.6% across all units of the hospital. These interventions employed strategies such as manual patient repositioning and logging, tissue visualization and palpation, pressure-reducing mattresses, and use of risk assessment tools.

[0009] Turning protocols, however, do not take into consideration position changes made by the patient between established turn intervals, which are neither observed nor recorded. Thus it is possible that in some circumstances, the act of following a turn protocol can have an unintended negative clinical effect.

SUMMARY

[0010] This disclosure describes, among other things, embodiments of systems, devices, and methods for moni-

toring the position and orientation of a patient at risk of forming one or more pressure ulcers.

[0011] One aspect of the present disclosure comprises a patient turn and movement monitoring system configured to help manage a patient that is at risk of forming one or more pressure ulcers. Some embodiments of the patient turn and monitoring system include a patient-worn, wireless sensor having one or more sensors configured to obtain information describing the patient's orientation and to wirelessly transmit information indicative of the sensed orientation information. The system also includes a patient monitor configured to receive, store, and process the information transmitted by the wireless sensor and to display and transmit information (or data) indicative of the patient's orientation to help caregivers manage the patient's risk of formation of one or more pressure ulcers. The patient turn and movement monitoring system can identify the present orientation of the patient and determine how long the patient has been in the present orientation. If the patient remains in an orientation beyond a predefined, clinician-prescribed patient orientation duration, the system can notify the patient and/or caretakers that the patient is due to be repositioned. In certain embodiments, a patient orientation duration timer is used to monitor such orientation times. In certain embodiments of the disclosed patient turn and movement monitoring system, a signal repeater, located within reception range of the wireless sensor, is used to receive and forward the information indicative of the sensed orientation information from the wireless sensor to a network-based processing node.

[0012] Another aspect of the present disclosure includes a wireless sensor including one or more sensors configured to obtain position, orientation, and motion information from the patient. The one or more sensors can include an accelerometer, a gyroscope, and a magnetometer, which are configured to determine the patient's position and orientation in three-dimensional space. The wireless sensor is configured to wirelessly transmit the sensor data, and/or information representative of the sensor data, to a patient monitor. The patient monitor can be configured to process the received information, to display information indicative of, or derived from the received data, and to transmit information—including displays, alarms, alerts, and notifications—to a multi-patient monitoring system which may be located, for example, at a nurse's station.

[0013] Another aspect of the present disclosure is directed to a system and method for associating the wireless sensor with a patient monitor. In some embodiments, the wireless sensor includes an activation tab which, when removed, activates the wireless sensor. Upon activation, a wireless transceiver in the wireless sensor emits a low-power pairing signal having a pairing signal transmission range of up to approximately three inches. In some embodiments, the wireless sensor has a switch or button which, when depressed, places the wireless sensor in a pairing mode of operation, causing the wireless sensor to emit the low-power pairing signal. When the patient monitor is within range of the wireless sensor (e.g., within the about three-inch range), the wireless sensor and the patient monitor associate, thereby configuring the wireless sensor and patient monitor to communicate with each other. Once the pairing between the wireless sensor and the patient monitor is completed, the wireless sensor changes into a patient parameter sensing mode of operation in which the wireless sensor transmits a

patient parameter sensing signal. The patient parameter sensing signal has a patient signal transmission range that is substantially greater than the pairing signal transmission range. The wireless sensor is then in condition to be placed on the patient.

[0014] In some aspects of the present disclosure the patient's position and orientation are monitored and recorded. Once the wireless sensor is affixed to the patient's body, such as, for example, the patient's torso, sensor data corresponding to the patient's motion (e.g., acceleration and angular velocity) are obtained, pre-processed, and transmitted to the patient monitor. The patient monitor stores and further processes the received data to determine the patient's orientation. Illustratively, the patient monitor can determine whether the patient is standing, sitting, or lying down in the prone, supine, left side, or right side positions.

[0015] In some embodiments, the patient monitor determines the precise orientation of the patient's body. For example, the patient monitor can determine the degree to which the patient's body is inclined, vertically and/or horizontally, thereby generating an accurate description of the patient's position relative to the support structure (such as a bed) upon which the patient lies.

[0016] In another aspect of the present disclosure the patient monitor stores the determined position and orientation information and keeps track of how long the patient remains in each determined position, thereby creating a continuous record of the patient's positional history. The patient monitor analyzes and processes the stored data to provide clinically-relevant, actionable information to the patient's care providers. Illustratively, the patient monitor counts the number of in-bed turns performed by the patient and monitors and displays the amount of time that has elapsed since the patient last turned. When the elapsed time exceeds a clinician-defined duration (e.g., two hours), the patient monitor displays an indication that the maximum time between patient turns has been exceeded. The patient monitor can also transmit a notification to one or more clinicians responsible for caring for the patient via, for example, a multi-patient monitoring system, a clinician notification device, or the like. The patient monitor can also determine and display statistical information, such as the average, minimum, and maximum amount of time between turns for a given clinician-defined time period, such as for example, twenty-four hours. The patient monitor can also determine and display the number of turns in the same position and orientation over a clinician-defined period of time. Similarly, the patient monitor can display the total amount of time the patient remained in each specific position within a clinician-defined period. Moreover, the patient monitor can determine the frequency and duration of periods during which the patient remained in clinically-defined acceptable positions.

[0017] In yet another aspect of the present disclosure the patient monitor determines the mobility status of the patient, e.g., whether the patient is ambulatory, standing, sitting, reclining, or falling. In certain aspects, the wireless monitoring system can include an alert system to alert the caregiver that the patient is falling, getting out of bed, or otherwise moving in a prohibited manner or in a manner that requires caregiver attention. The alert can be an audible and/or visual alarm on the monitoring system, or the alert can be transmitted to a caregiver (e.g., nurses' station, clinician device, pager, cell phone, computer, or otherwise).

Illustratively, the patient monitor can display the patient's mobility status and transmit a notification that the patient is active and away from the bed. In some circumstances, the patient monitor can determine whether the patient contravenes a clinician's order, such as, for example, instructions to remain in bed, or to walk to the bathroom only with the assistance of an attendant. In such circumstances, a notification, alert, or alarm can be transmitted to the appropriate caregivers.

[0018] In certain aspects, the information received by the wireless sensor can be used to create a time-sequenced representation of the patient's movement. This representation can be displayed on the patient monitor or transmitted to a nurses' station or other processing nodes to enable the caregiver to monitor the patient. The time-sequenced representation can be viewed in real time and/or be recorded for playback. For example, if an alarm alerts the caregiver that the patient has fallen out of bed, the caregiver can access and review the historical sequence of the patient's movements prior to and during that period of time.

[0019] Another aspect of the present disclosure is directed to predicting a patient's risk of falling based on the patient's gait and other information (such as, for example, the patient's current medication regimen). When the patient monitor determines that the patient's risk of falling is above a predetermined threshold, the patient monitor can issue an alarm or alert to notify care providers of the identified risk in an effort to anticipate and therefore prevent a patient fall. Additionally, the patient monitor can determine when a patient has fallen and issue the appropriate alarms and alerts to summon care provider assistance.

[0020] In an aspect of the present disclosure the patient monitor accesses the patient's health records and clinician input via a network. Illustratively, the patients' positional history data, analyzed in view of the patient's health records, may reveal or suggest a turning protocol (or other treatment protocol) that will likely yield favorable clinical outcomes for the particular patient. Accordingly, the patient monitor analyzes the accessed information in conjunction with the received information from the wireless sensor to determine a recommended patient turn protocol (or other treatment protocol) for the patient.

[0021] In still another aspect of the present disclosure, the patient monitor assesses caregiver and facility compliance with the clinician-defined patient turn protocol established for the patient. For example, the patient monitor can identify the number of times that the patient remains in a position for a period greater than the prescribed duration, indicating a patient turn protocol violation, as well as the length of each such overexposure. The patient monitor can also track the clinician's response time upon issuance of a notification, alert, or alarm.

[0022] According to another aspect of the present disclosure, care provider workflow productivity, efficiency, and effectiveness can be determined, based on aggregated positional history data corresponding to multiple patients wherein each patient is equipped with the disclosed wireless sensor. Additionally, care for patients in a particular location, such as a hospital ward or nursing home floor where the ratio of patients to staff is relatively high, can be prioritized based on the determined risk of formation of pressure ulcers. Thus, patients determined to have the highest risk are designated to receive attention first.

[0023] In yet another aspect of the present disclosure, the wireless sensor includes sensors to obtain additional physiological measurements from the patient. For example, the wireless sensor can include a temperature sensor configured to measure the patient's body core body temperature by insulating the patient's skin surface around the temperature sensor. As a result of the insulation surrounding the temperature sensor, the natural temperature difference between the patient's skin surface and body core reach equilibrium, thereby arriving at the patient's body core temperature (which is typically higher in temperature than the patient's skin surface). The wireless sensor can also include an acoustic respiration sensor configured to sense vibrational motion generated by the patient's chest. The acoustic respiration sensor is configured to mechanically transmit the sensed vibrations through rigid structures of the device to the accelerometer. Processing of the accelerometer signal can provide, among other things, the patient's respiration and heart rates. An electrocardiogram (ECG) sensor, configured to sense electrical signals from two or more electrodes in electrical contact with the patient's chest may also be included in the wireless sensor. The ECG signal can be processed to detect arrhythmias, such as bradycardia, tachyarrhythmia, ventricular fibrillation and the like. Additionally, the accelerometer signal (containing information indicative of the mechanically-transmitted vibrations from the acoustic respiration sensor) and/or the ECG signal can be processed to identify respiratory distress or dysfunction, including without limitation, snoring, coughing, choking, wheezing, apneic events, and airway obstruction.

[0024] In another aspect of the present disclosure, the patient monitor can determine a score that describes the patient's wellness/sickness state, which may also be referred to as a "Halo Index." Illustratively, the patient monitor accesses and analyzes the patient's health records, clinician input, positional history data provided by the wireless sensor, surface structure pressure data, and other physiological parameter data collected and provided by the wireless sensor (such as, by way of non-limiting example, the patient's temperature, respiration rate, heart rate, ECG signal, and the like) to assess the patient's overall health condition.

[0025] In an aspect of the present disclosure, the patient monitor accesses information provided by the patient's support structure (e.g., bed, mattress, bed sheet, mattress pad, and the like) to determine the extent of pressure forces exerted on particular anatomical sites of the patient's body. Illustratively, the patient's support structure can be configured with an array of pressure sensors that measure the pressure force exerted on the support structure by the patient at specific locations. The patient monitor can analyze the patient's postural history data in conjunction with the information provided by the support structure to determine a likelihood of pressure ulcer formation at a specific anatomical location based on the measured amount of pressure exerted on the anatomical location multiplied by the amount of time the anatomical location has been under such pressure. When the evaluated risk exceeds a predetermined threshold, the patient monitor can issue an alarm and/or an alert to reposition the patient so as to avoid formation of a pressure ulcer in the specified anatomical location. Additionally, the patient monitor can suggest particular positions and/or a patient turn protocol based on the combined analysis of pressure force exerted and length of time under such pressure.

[0026] For purposes of summarizing the disclosure, certain aspects, advantages, and novel features have been described herein. Of course, it is to be understood that not necessarily all such aspects, advantages, or features will be embodied in any particular embodiment.

BRIEF DESCRIPTION OF THE DRAWINGS

[0027] Various embodiments will be described hereinafter with reference to the accompanying drawings. The drawings and the associated descriptions are provided to illustrate embodiments of the present disclosure and do not limit the scope of the claims. In the drawings, similar elements have similar reference numerals.

[0028] FIG. 1A is a perspective view of an embodiment of the disclosed patient monitoring system including a patient-worn wireless sensor in proximity to a patient monitor.

[0029] FIG. 1B is a functional block diagram of an embodiment of the display of the disclosed patient monitor.

[0030] FIG. 1C is a functional block diagram of an embodiment of the disclosed patient monitoring system.

[0031] FIG. 1D is a functional block diagram of an embodiment of the disclosed patient monitoring system.

[0032] FIG. 1E is a functional block diagram of an embodiment of the disclosed patient monitoring system.

[0033] FIG. 1F is a functional block diagram of an embodiment of the disclosed patient monitoring system.

[0034] FIG. 2A is a functional block diagram of an embodiment of the disclosed wireless sensor.

[0035] FIG. 2B is a functional block diagram of an embodiment of the disclosed wireless sensor including optional sensing components.

[0036] FIG. 3A is a schematic exploded perspective view of an embodiment of the disclosed wireless sensor.

[0037] FIG. 3B is a schematic assembled perspective view of the embodiment of the disclosed wireless sensor of FIG. 3A.

[0038] FIG. 3C is a schematic side view of the embodiment of the disclosed wireless sensor of FIGS. 3A and 3B.

[0039] FIG. 4A is a schematic cross-sectional view of an embodiment of the disclosed wireless sensor which includes a temperature sensor.

[0040] FIG. 4B is a schematic bottom view of the embodiment of the disclosed wireless sensor of FIG. 4A.

[0041] FIG. 4C is a schematic exploded perspective view of the embodiment of the disclosed wireless sensor of FIGS. 4A-B.

[0042] FIG. 5A is a schematic cross-sectional view of an embodiment of the disclosed wireless sensor which includes an acoustic respiration sensor.

[0043] FIG. 5B is a schematic bottom view of the embodiment of the disclosed wireless sensor of FIG. 5A.

[0044] FIG. 5C is a schematic exploded perspective view of the embodiment of the disclosed wireless sensor of FIGS. 5A-B.

[0045] FIG. 6A is a schematic cross-sectional view of an embodiment of the disclosed wireless sensor which includes a temperature sensor and an acoustic respiration sensor.

[0046] FIG. 6B is a schematic bottom view of the embodiment of the disclosed wireless sensor of FIG. 6A.

[0047] FIG. 6C is a schematic exploded perspective view of the embodiment of the disclosed wireless sensor of FIGS. 6A-B.

[0048] FIG. 7A is a perspective view of an embodiment of the disclosed patient monitoring system including a patient-worn wireless sensor having an ECG sensor in proximity to a patient monitor.

[0049] FIG. 7B is a schematic assembled perspective view of the embodiment of the disclosed wireless sensor of FIG. 7A.

[0050] FIG. 7C is a schematic side view of the embodiment of the disclosed wireless sensor of FIGS. 7A and 7B.

[0051] FIG. 7D is a cross-sectional view of an embodiment of the disclosed wireless sensor of FIGS. 7A-C.

[0052] FIG. 7E is a schematic bottom perspective view of the embodiment of the disclosed wireless sensor of FIGS. 7A-D.

[0053] FIG. 7F is a schematic exploded perspective view of the embodiment of the disclosed wireless sensor of FIGS. 7A-7E.

[0054] FIG. 8A is a schematic exploded perspective view of an embodiment of the disclosed wireless sensor having a temperature sensor, an acoustic respiration sensor, and an ECG sensor.

[0055] FIG. 8B is a schematic bottom view of the disclosed wireless sensor of FIG. 8A.

[0056] FIG. 9 is a flow diagram describing a process to associate a wireless sensor with a patient monitor according to an embodiment of the present disclosure.

[0057] FIG. 10 is a flow diagram describing a process to determine whether a patient has changed orientation according to an embodiment of the present disclosure.

[0058] FIG. 11A is an exemplary plot of processed accelerometer data over time used to determine a patient's orientation according to an embodiment of the present disclosure.

[0059] FIG. 11B is an exemplary plot of the duration of a patient's orientation according to an embodiment of the present disclosure.

[0060] FIG. 12 is a flow diagram describing a process to determine whether a patient has fallen according to an embodiment of the present disclosure.

[0061] FIGS. 13A-F illustrate embodiments of displays reflecting a patient's position according to an embodiment of the present disclosure.

[0062] FIG. 14 illustrates an example display of a patient monitor incorporating the icons illustrated in FIGS. 13A-F according to an embodiment of the present disclosure.

[0063] FIGS. 15A-15H illustrate various configurations of a room display displayed on a patient display monitor according to an embodiment of the present disclosure.

[0064] FIG. 16 illustrates an example method according to an embodiment of the present disclosure.

DETAILED DESCRIPTION

[0065] Embodiments of the present disclosure will now be described with reference to the accompanying figures, wherein like numerals refer to like elements throughout. The following description is merely illustrative in nature and is in no way intended to limit the disclosure, its application, or uses. It should be understood that steps within a method may be executed in different order without altering the principles of the present disclosure. Furthermore, embodiments disclosed herein can include several novel features, no single one of which is solely responsible for its desirable attributes or which is essential to practicing the systems, devices, and methods disclosed herein.

[0066] The present disclosure relates to systems, devices, methods, and computer-readable media to monitor and manage the position, orientation, and movement of a patient who is at risk of forming one or more pressure ulcers. In one embodiment, the system comprises a patient-worn, wireless sensor including one or more sensors configured to obtain position, orientation and movement information from the patient. The one or more sensors can include one or more accelerometers, gyroscopes, and magnetometers (i.e., compasses). Illustratively, the sensors continuously or periodically (e.g., every second) obtain information that describes the patient's orientation in three dimensions. The wireless sensor includes a processor that is configured to process the obtained sensor information. The wireless sensor also includes a transceiver configured to wirelessly transmit the processed sensor data, and/or information representative of the sensor data, to a patient monitor (or other processing device) for further processing. The patient monitor can be configured to store and further process the received information, to display information indicative of or derived from the received data, and to transmit information—including displays, alarms, alerts, and notifications—to other patient care systems including a multi-patient monitoring system which may be accessible from, for example, a nurses' station.

[0067] FIG. 1A is a perspective illustration of an embodiment of the disclosed patient monitoring system **100** in a clinical setting. The patient monitoring system **100** includes a wireless sensor **102** worn by a patient, in proximity to a patient monitor **106** located on a table **116** at the side of the patient's bed **118**. The wireless sensor **102** may also be referred to herein as “a wireless physiological sensor **102**,” “a patient-worn sensor **102**,” “a movement sensor **102**,” and “a wearable wireless sensor **102**.” The wireless sensor **102** includes one or more sensors configured to measure the patient's position, orientation, and motion. In some embodiments, the wireless sensor **102** includes an accelerometer configured to measure linear acceleration of the patient and a gyroscope configured to measure angular velocity of the patient. The measured linear acceleration and angular velocity information can be processed to determine the patient's orientation in three dimensions. In some embodiments, a magnetometer is included in the wireless sensor **102** to measure the Earth's gravitational field. Information measured by the magnetometer can be used to improve accuracy of the determined orientation of the patient.

[0068] The wireless sensor **102** also includes a wireless transceiver **206** (shown in FIGS. 2A and 2B) which can transmit to the patient monitor **106** information representative of sensor data obtained by the wireless sensor **102** from the patient. Advantageously, the patient is not physically coupled to the bedside patient monitor **106** and can therefore move freely into different positions on the bed **118**.

[0069] In accordance with certain embodiments of the present disclosure, the wireless sensor **102** is affixed to the skin of the patient's body under the patient's garment as reflected in FIG. 1A by the phantom drawing of the wireless sensor **102**. More particularly, the wireless sensor **102** can be placed on the patient's chest over the patient's manubrium, the broad upper portion of the sternum. In this position, the wireless sensor **102** is approximately centered relative to the longitudinal axis of the patient's body and near the patient's center of mass, a position that is useful in determining the patient's orientation when, for example, the patient is in bed.

[0070] The wireless sensor **102** can be affixed to the patient's skin using any form of medically-appropriate adherent material, including a pressure-sensitive adhesive that is coated or applied to the bottom surface of the wireless sensor **102**. One skilled in the art will appreciate that many other materials and techniques can be used to affix the wireless sensor **102** to the patient without departing from the scope of the present disclosure.

[0071] Frequently in clinical settings, multiple medical sensors are attached or adhered to a patient to concurrently monitor multiple physiological parameters. Some examples of medical sensors include, but are not limited to, position, orientation, and movement sensors, temperature sensors, respiration sensors, heart rate sensors, blood oxygen sensors (such as pulse oximetry sensors), acoustic sensors, EEG sensors, ECG sensors, blood pressure sensors, sedation state sensors, to name a few. Typically, each sensor that is attached to a patient transmits, often by cable, the obtained physiological data to a nearby monitoring device configured to receive and process the sensor data, and transform it into clinical information to be used by the care providers to monitor and manage the patient's condition. When a patient is concurrently monitored by several physiological sensors, the number of cables and the number of bedside monitoring devices used can be excessive and can limit the patient's freedom of movement and impede care providers' access to the patient. The cables connecting the patient to the bedside monitoring devices can also make it more difficult to move the patient from room to room or to switch to different bedside monitors.

[0072] Advantageously, the disclosed wireless sensor **102** can transmit data, wirelessly, to a patient data processing environment **105** in which the sensor data can be processed using one or more processing capabilities. As illustrated in FIG. 1A, the wireless sensor **102** transmits data via a wireless communications link **104**. The wireless communications link **104** can be received by the bedside patient monitor **106**, and/or by an extender/repeater **107**. Both the patient monitor **106** and extender/repeater **107** provide access, by way of high-speed and reliable communications interfaces, to the patient data processing environment **105**. For illustration purposes, both the patient monitor **106** and the extender/repeater **107** are illustrated in FIG. 1A. However, typically only one such device is required to establish a wireless connection between the wireless sensor **102** and the patient data processing environment **105**. The wireless communications link **104** can use any of a variety of wireless technologies, such as Wi-Fi (802.11x), Bluetooth, ZigBee, cellular telephony, infrared, RFID, satellite transmission, proprietary protocols, combinations of the same, and the like. The wireless sensor **102** can be configured to perform telemetry functions, such as measuring and reporting position, orientation, and movement information about the patient. According to one embodiment, the wireless sensor **102** uses the Bluetooth wireless communications standard to communicate wirelessly with the patient monitor **106**.

[0073] The extender/repeater **107** can receive sensor data from the wireless sensor **102** by way of the wireless communications link **104** and forward the received sensor data, via the network **108**, to one or more processing nodes within the patient data processing environment **105**. For example, the extender/repeater **107** can forward the received sensor data to a patient monitor **106** that might be located beyond the range of the wireless communications link **104** of a

particular wireless sensor **102**. Alternatively, the extender/repeater **107** can route the sensor data to other processing nodes within the patient data processing environment **105**, such as, for example, a multi-patient monitoring system **110** or a nurses' station system **113**. A skilled artisan will appreciate that numerous processing nodes and systems can be used to process the data transmitted by the wireless sensor **102**.

[0074] FIG. 1A also illustrates an embodiment of the patient monitor **106**, which may also be referred to herein as "a processing device **106**," "a portable computing device **106**," and "a patient monitoring device **106**." Examples of a patient monitor **106** are disclosed in U.S. Pat. Pub. Nos. 2013/0262730 and 2015/0099955, assigned to the assignee of the present disclosure, and which are incorporated by reference herein in their entirety. The patient monitor **106** is a processing device, and therefore includes the necessary components to perform the functions of a processing device, including at least one processor, a memory device, a storage device, input/output devices, and communications connections, all connected via one or more communication buses. Thus, in certain embodiments, the patient monitor **106** is configured to process the sensor data provided by the wireless sensor **102**. In other embodiments, processing of the sensor data can be performed by other processing nodes within the patient data processing environment **105**. The patient monitor **106** is configured to wirelessly communicate with the wireless sensor **102**. The patient monitor **106** includes a display **120**, and a docking station, which is configured to mechanically and electrically mate with a portable patient monitor **122** also having a display **130**. The patient monitor **106** is housed in a movable, mountable, and portable housing formed in a generally upright, inclined shape configured to rest on a horizontal flat surface, as shown in FIG. 1A. Of course, a person skilled in the art will appreciate that the housing can be affixed in a wide variety of positions and mountings and can comprise a wide variety of shapes and sizes.

[0075] In an embodiment, the display **120**, alone or in combination with the display **130** of the portable patient monitor **122**, may present a wide variety of measurement and/or treatment data in numerical, graphical, waveform, or other display indicia. For example, the display **120** can display a variety of patient-specific configurations and/or parameters, such as the patient's weight, age, type of treatment, type of disease, type of medical condition, nutrition, hydration and/or length of stay, among others. In an embodiment, the display **120** occupies much of a front face of the housing, although an artisan will appreciate the display **120** may comprise a table or tabletop horizontal configuration, a laptop-like configuration, or the like. Other embodiments may include communicating display information and data to a tablet computer, smartphone, television, or any display system recognizable to an artisan. Advantageously, the upright inclined configuration of the patient monitor **106**, as illustrated in FIG. 1A, displays information to a caregiver in an easily viewable manner.

[0076] The portable patient monitor **122** of FIG. 1A may advantageously include an oximeter, co-oximeter, respiratory monitor, depth of sedation monitor, noninvasive blood pressure monitor, vital signs monitor or the like, such as those commercially available from Masimo Corporation of Irvine, Calif., and/or disclosed in U.S. Pat. Pub. Nos. 2002/0140675, 2010/0274099, 2011/0213273, 2012/0226117,

2010/0030040; U.S. patent application Ser. Nos. 61/242,792, 61/387457, 61/645,570, 13/554,908 and U.S. Pat. Nos. 6,157,850, 6,334,065, the contents of which are incorporated herein by reference in their entirety. The portable patient monitor **122** may communicate with a variety of noninvasive and/or minimally invasive devices such as, by way of non-limiting example, wireless sensor **102**, optical sensors with light emission and detection circuitry, acoustic sensors, devices that measure blood parameters from a finger prick, cuffs, ventilators, and the like. The portable patient monitor **122** may include its own display **130** presenting its own display indicia. The display indicia may change based on a docking state of the portable patient monitor **122**. When undocked, the display **130** may include parameter information and may alter its display orientation based on information provided by, for example, a gravity sensor or an accelerometer. Although disclosed with reference to particular portable patient monitors **122**, an artisan will recognize from the disclosure herein there is a large number and wide variety of medical devices that may advantageously dock with the patient monitor **106**.

[0077] FIG. 1B is a functional block diagram of an embodiment of the display **120** of the disclosed patient monitor **106** and the display **130** of the portable patient monitor **122**. Display **120** of the patient monitor **106** can be configured to present patient physiological data **124**, patient turn data **126**, and/or additional, optional patient data **128**. Patient physiological data can include, by way of non-limiting example, oxygen saturation, pulse rate, respiration rate, fractional arterial oxygen saturation, total hemoglobin, plethysmograph variability index, methemoglobin, carboxy-hemoglobin, perfusion index, and oxygen content. Advantageously, the display **120** is configurable to permit the user to adjust the manner by which the physiologic parameters **124**, patient turn data **126**, and optional patient data **128** are presented on the display **120**. In particular, information of greater interest or importance to the clinician may be displayed in larger format and may also be displayed in both numerical and graphical formats to convey the current measurement as well as the historical trend of measurements for a period of time, such as, for example, the preceding hour.

[0078] As illustrated by dotted lines in FIG. 1B, the display **130** of the portable patient monitor **130** is an optional feature of the patient monitor **106** which may be configured to present patient physiological data **134**, patient turn data **136**, and additional, optional patient data **138**.

[0079] FIG. 1C is a simplified functional block diagram of an embodiment of the disclosed patient monitoring system **100**. The system includes the patient-worn wireless sensor **102** having one or more sensors, a wireless communications link **104**, through which sensor data from the wireless sensor **102** accesses the patient data processing environment **105** which includes a patient monitor **106**, a communications network **108**, a multi-patient monitoring system **110**, a hospital or facility information system **112**, one or more nurses' station systems **113**, and one or more clinician devices **114**. An artisan will appreciate that numerous other computing systems, servers, processing nodes, display devices, printers, and the like can be included in the disclosed patient monitoring system **100**.

[0080] The wireless sensor **102** is worn by a patient who has been determined to be at risk of forming one or more pressure ulcers, e.g., a patient who is confined to bed for an

extended period of time. The wireless sensor **102** is capable of monitoring on a continuous or periodic (e.g., every second) basis the orientation of the patient to help determine whether the patient is repositioned frequently enough to reduce the patient's risk of forming a pressure ulcer. In certain embodiments, the wireless sensor **102** minimally processes measured acceleration and/or angular velocity data and wirelessly transmits the minimally-processed data to the patient monitor **106** by way of the wireless communications link **104**.

[0081] The wireless sensor **102** and the patient monitor **106** can be configured to utilize different wireless technologies to form the wireless communications link **104**. In certain scenarios, it may be desirable to transmit data over Bluetooth or ZigBee, for example, when the distance between the wireless sensor **102** and the patient monitor **106** is within range of Bluetooth or ZigBee communication. Transmitting data using Bluetooth or ZigBee is advantageous because these technologies require less power than other wireless technologies. Accordingly, longevity of embodiments of the disclosed wireless sensor **102** using batteries may be increased by using Bluetooth or ZigBee protocols.

[0082] In other scenarios, it may be desirable to transmit data using Wi-Fi or cellular telephony, for example, when the distance between the wireless sensor **102** and the patient monitor **106** is out of range of communication for Bluetooth or ZigBee. A wireless sensor **102** may be able to transmit data over a greater distance using Wi-Fi or cellular telephony than other wireless technologies. In still other scenarios, it may be desirable to transmit data using a first wireless technology and then automatically switching to a second wireless technology in order to maximize data transfer and/or energy efficiency.

[0083] In some embodiments, the wireless sensor **102** automatically transmits data over Bluetooth or ZigBee when the wireless sensor **102** is within a pre-determined distance from the bedside patient monitor **106**. The wireless sensor **102** automatically transmits data over Wi-Fi or cellular telephony when the wireless sensor **102** is beyond a pre-determined distance away from the bedside patient monitor **106**. In certain embodiments, the wireless sensor **102** can automatically convert from Bluetooth or ZigBee to Wi-Fi or cellular telephony, and vice versa, depending on the distance between the wireless sensor **102** and the bedside patient monitor **106**.

[0084] In some embodiments, the wireless sensor **102** automatically transmits data over Bluetooth or ZigBee when the Bluetooth or ZigBee signal strength is sufficiently strong or when there is interference with Wi-Fi or cellular telephony. The wireless sensor **102** automatically transmits data over Wi-Fi or cellular telephony when the Bluetooth or ZigBee signal strength is not sufficiently strong. In certain embodiments, the wireless sensor **102** can automatically convert from Bluetooth or ZigBee to Wi-Fi or cellular telephony, and vice versa, depending on signal strength.

[0085] The patient monitor **106** can be operable to receive, store and process the measured acceleration and angular velocity data transmitted by the wireless sensor **102** to determine the patient's orientation. Once determined, the patient monitor **106** can display the patient's current orientation. In some embodiments, the patient monitor **106** displays the patient's current orientation along with the patient's previous orientations over time, thereby providing

the user the ability to view a historical record of the patient's orientation. In certain embodiments, e.g., as illustrated in FIGS. **13A-F** and **14**, the patient orientation is displayed by icons, such as stick figures, enabling the clinician to readily understand the patient's present positional state and the patient's positional history. The patient monitor **106** can also be configured to keep track of the length of time the patient remains in a particular orientation. In some embodiments the patient monitor **106** displays the amount of time the patient has been in the current orientation. Additionally, the patient monitor **106** can determine when the patient remains in a particular orientation for a duration greater than that prescribed by a clinician according to a repositioning protocol. Under such conditions, the patient monitor **106** can issue alarms, alerts, and/or notifications to the patient and/or to caregivers indicating that the patient should be repositioned to adhere to the prescribed repositioning protocol to reduce the risk of pressure ulcer formation.

[0086] As illustrated in FIG. **1C**, the patient monitor **106** communicates over a network **108** with a patient data processing environment **105** that includes a multi-patient monitoring system **110**, a hospital/facility system **112**, nurses' station systems **113**, and clinician devices **114**. Examples of network-based clinical processing environments, including multi-patient monitoring systems **110**, are disclosed in U.S. Pat. Pub. Nos. 2011/0105854, 2011/0169644, and 2007/0180140, which are incorporated herein by reference in their entirety. In general, the multi-patient monitoring system **110** communicates with a hospital/facility system **112**, the nurses' station systems **113**, and clinician devices **114**. The hospital/facility system **112** can include systems such as electronic medical record (EMR) and/or admit, discharge, and transfer (ADT) systems. The multi-patient monitoring system **110** may advantageously obtain through push, pull or combination technologies patient information entered at patient admission, such as patient identity information, demographic information, billing information, and the like. The patient monitor **106** can access this information to associate the monitored patient with the hospital/facility systems **112**. Communication between the multi-patient monitoring system **110**, the hospital/facility system **112**, the nurses' station systems **113**, the clinician devices **114**, and the patient monitor **106** may be accomplished by any technique recognizable to an artisan from the disclosure herein, including wireless, wired, over mobile or other computing networks, or the like.

[0087] FIG. **1D** is a simplified functional block diagram of the disclosed patient monitoring system **100** of FIG. **1C** expanded to illustrate use of multiple wireless sensors **102** with multiple patients within a caretaking environment. Advantageously, the patient monitoring system **100** can provide individual patient information on, for example, a patient monitor **106**, as well as aggregated patient information on, for example, a nurses' station server or system **114**. Thus a caretaker can have an overview of positional information corresponding to a population of patients located, for example, in a hospital floor or unit.

[0088] In some circumstances, there may not be the need, desire, or resources available to employ a bedside patient monitor **106** associated with a wireless sensor **102** being worn by a patient. For example, the clinical environment might be staffed such that patient data are collected, analyzed, displayed, and monitored at a central observation station, such as a nurses' station, rather than at the patient's

bedside. Moreover, when the information is to be accessed by a clinician at the bedside, portable clinician devices 114, such as, for example, tablets, PDAs or the like, may be used by caregivers to access the required patient-specific information while at the patient's bedside.

[0089] In such situations, as illustrated in FIGS. 1E and 1F, the wireless sensor 102 can communicate to the various systems of the clinical computing environment by way of a signal extender/repeater 107. The extender/repeater 107 is located within range of the wireless sensor 102 (e.g., near the patient's bed 118) and configured to relay data, via the network 108, between the wireless sensor 102 and one or more computing systems capable of processing, storing, displaying, and/or transmitting the data collected by the wireless sensor 102. Advantageously, a relatively low cost extender/repeater 107 can be used to receive signals transmitted from one or more wireless sensors 102 over the wireless communications link(s) 104 using a shorter-range, lower-power-consuming transmission mode, such as for example, Bluetooth or ZigBee. The extender/repeater 107 can then retransmit the received signals to one or more computing systems in the patient data processing environment 105 over the network 108. In accordance with some embodiments, the extender/repeater 107 is a Bluetooth-to-Ethernet gateway that retransmits signals received from the wireless sensor 102 to computing nodes, such as, for example, the multi-patient monitoring system 110, over the network 108. In some embodiments, the extender/repeater 107 is a Bluetooth-to-WiFi bridge that provides access to the network 108 for the wireless sensor 102. Of course, a skilled artisan will recognize that there are numerous ways to implement the extender/repeater 107.

[0090] FIG. 2A illustrates a simplified hardware block diagram of an embodiment of the disclosed wireless sensor 102. As shown in FIG. 2A, the wireless sensor 102 can include a processor 202, a data storage device 204, a wireless transceiver 206, a system bus 208, an accelerometer 210, a gyroscope 212, a battery 214, and an information element 215. The processor 202 can be configured, among other things, to process data, execute instructions to perform one or more functions, such as the methods disclosed herein, and control the operation of the wireless sensor 102. The data storage device 204 can include one or more memory devices that store data, including without limitation, random access memory (RAM) and read-only memory (ROM). The wireless transceiver 206 can be configured to use any of a variety of wireless technologies, such as Wi-Fi (802.11x), Bluetooth, ZigBee, cellular telephony, infrared, RFID, satellite transmission, proprietary protocols, combinations of the same, and the like. The components of the wireless sensor 102 can be coupled together by way of a system bus 208, which may represent one or more buses. The battery 214 provides power for the hardware components of the wireless sensor 102 described herein. As illustrated in FIG. 2A, the battery 214 communicates with other components over system bus 208. One skilled in the art will understand that the battery 214 can communicate with one or more of the hardware functional components depicted in FIG. 2A by one or more separate electrical connections. The information element 215 can be a memory storage element that stores, in non-volatile memory, information used to help maintain a standard of quality associated with the wireless sensor 102. Illustratively, the information element 215 can store information regarding whether the sensor 102 has been previ-

ously activated and whether the sensor 102 has been previously operational for a prolonged period of time, such as, for example, four hours. The information stored in the information element 215 can be used to help detect improper re-use of the wireless sensor 102.

[0091] In some embodiments, the accelerometer 210 is a three-dimensional (3D) accelerometer. The term 3D accelerometer as used herein includes its broad meaning known to a skilled artisan. The accelerometer 210 provides outputs responsive to acceleration of the wireless sensor 102 in three orthogonal axes, sometimes denoted as the "X," "Y," and "Z" axes. An accelerometer 210 may measure acceleration that it experiences relative to Earth's gravity. An accelerometer 210 may provide acceleration information along three axes, and it may provide acceleration information which is the equivalent of inertial acceleration minus local gravitational acceleration. Accelerometers 210 are well known to those skilled in the art. The accelerometer 210 may be a micro-electromechanical system (MEMS), and it may include piezo-resistors, among other forms of implementation. The accelerometer 210 may be a high-impedance charge output or a low-impedance charge output accelerometer 210. In some embodiments, the accelerometer 210 may be a tri-axis accelerometer, and the output of the accelerometer 210 may include three signals, each of which represents measured acceleration in particular axis. The output of the accelerometer 210 may be 8-bit, 12-bit, or any other appropriate-sized output signal. The outputs of the accelerometer may be in analog or digital form. The accelerometer 210 may be used to determine the position, orientation, and/or motion of the patient to which the wireless sensor 102 is attached.

[0092] In some embodiments, the gyroscope 212 is a three-axis digital gyroscope with angle resolution of two degrees and with a sensor drift adjustment capability of one degree. The term three-axis gyroscope as used herein includes its broad meaning known to a skilled artisan. The gyroscope 212 provides outputs responsive to sensed angular velocity of the wireless sensor 102 (as affixed to the patient) in three orthogonal axes corresponding to measurements of pitch, yaw, and roll. A skilled artisan will appreciate that numerous other gyroscopes 212 can be used in the wireless sensor 102 without departing from the scope of the disclosure herein. In certain embodiments, the accelerometer 210 and gyroscope 212 can be integrated into a single hardware component which may be referred to as an inertial measurement unit (IMU). In some embodiments, the IMU can also include an embedded processor that handles, among other things, signal sampling, buffering, sensor calibration, and sensor fusion processing of the sensed inertial data. In other embodiments, the processor 202 can perform these functions. And in still other embodiments, the sensed inertial data are minimally processed by the components of the wireless sensor 102 and transmitted to an external system, such as the patient monitor 106, for further processing, thereby minimizing the complexity, power consumption, and cost of the wireless sensor 102, which may be a single-use, disposable product.

[0093] FIG. 2B is a simplified hardware functional block diagram of an embodiment of the disclosed wireless sensor 102 that includes the following optional (as reflected by dotted lines) sensing components: a magnetometer 216 which may also be referred to as a compass, a temperature sensor 218, an acoustic respiration sensor 220, an electro-

cardiogram (ECG) sensor **222**, one or more oximetry sensors **224**, a moisture sensor **226**, and an impedance sensor **228**. In some embodiments, the magnetometer **216** is a three-dimensional magnetometer that provides information indicative of magnetic fields, including the Earth's magnetic field. While depicted in FIG. 2B as separate functional elements, a skilled artisan will understand that the accelerometer **210**, gyroscope **212**, and magnetometer **214** can be integrated into a single hardware component such as an inertial measurement unit.

[0094] According to an embodiment, a system and method are described herein to calculate three-dimensional position and orientation of an object derived from inputs from three sensors attached to the object: an accelerometer **210** configured to measure linear acceleration along three axes; a gyroscope **212** configured to measure angular velocity around three axes; and a magnetometer **214** configured to measure the strength of a magnetic field (such as the Earth's magnetic field) along three axes. In an embodiment, the three sensors **210**, **212**, and **214** are attached to the wireless sensor **102** which is affixed to the patient. According to an embodiment, the sensors **210**, **212**, and **214** are sampled at a rate between approximately 10 Hz and approximately 100 Hz. One skilled in the art will appreciate that the sensors **210**, **212**, and **214** can be sampled at different rates without deviating from the scope of the present disclosure. The sampled data from the three sensors **210**, **212**, and **214**, which provide nine sensor inputs, are processed to describe the patient's position and orientation in three-dimensional space. In an embodiment, the patient's position and orientation are described in terms of Euler angles as a set of rotations around a set of X-Y-Z axes of the patient.

[0095] Also illustrated in FIG. 2B is a temperature sensor **218** which may be used to measure the patient's body core temperature which is a vital sign used by clinicians to monitor and manage patients' conditions. The temperature sensor **218** can include a thermocouple, a temperature-measuring device having two dissimilar conductors or semi-conductors that contact each other at one or more spots. A temperature differential is experienced by the different conductors. The thermocouple produces a voltage when the contact spot differs from a reference temperature. Advantageously, thermocouples are self-powered and therefore do not require an external power source for operation. In an embodiment, the temperature sensor **218** includes a thermistor. A thermistor is a type of resistor whose resistance value varies depending on its temperature. Thermistors typically offer a high degree of precision within a limited temperature range.

[0096] The acoustic respiration sensor **220** can be used to sense vibrational motion from the patient's body (e.g., the patient's chest) that are indicative of various physiologic parameters and/or conditions, including without limitation, heart rate, respiration rate, snoring, coughing, choking, wheezing, and respiratory obstruction (e.g., apneic events). The ECG sensor **222** can be used to measure the patient's cardiac activity. According to an embodiment, the ECG sensor **222** includes two electrodes and a single lead. The oximetry sensor(s) **224** can be used to monitor the patient's pulse oximetry, a widely accepted noninvasive procedure for measuring the oxygen saturation level of arterial blood, an indicator of a person's oxygen supply. A typical pulse oximetry system utilizes an optical sensor clipped onto a portion of the patient's body (such as, for example, a

finger tip, an ear lobe, a nostril, and the like) to measure the relative volume of oxygenated hemoglobin in pulsatile arterial blood flowing within the portion of the body being sensed. Oxygen saturation (SpO₂), pulse rate, a plethysmograph waveform, perfusion index (PI), pleth variability index (PVI), methemoglobin (MetHb), carboxyhemoglobin (CoHb), total hemoglobin (tHb), glucose, and/or otherwise can be measured and monitored using the oximetry sensor(s) **224**. The moisture sensor **226** can be used to determine a moisture content of the patient's skin which is a relevant clinical factor in assessing the patient's risk of forming a pressure ulcer. The impedance sensor **228** can be used to track fluid levels of the patient. For example, the impedance sensor **228** can monitor and detect edema, heart failure progression, and sepsis in the patient.

[0097] FIG. 3A is a schematic exploded perspective view of an embodiment of the disclosed wireless sensor **102** including a bottom base **310**, a removable battery isolator **320**, a mounting frame **330**, a circuit board **340**, a housing **350**, and a top base **360**. The bottom base **310** is a substrate having a top surface on which various components of the wireless sensor **102** are positioned, and a bottom surface that is used to affix the wireless sensor **102** to the patient's body. The bottom base **310** and top base **360** can be made of medical-grade foam material such as white polyethylene, polyurethane, or reticulated polyurethane foams, to name a few. As illustrated in the embodiment illustrated in FIG. 3A, the bottom base **310** and the top base **360** are each in a substantially oval shape, with a thickness of approximately 1 mm. The top base **360** includes a cut-out **362** through which the housing **350** fits during assembly. Of course, a skilled artisan will understand that there are numerous sizes and shapes suitable for the top and bottom bases **310** and **360** that can be employed without departing from the scope of the present disclosure. The bottom surface of the bottom base **310** is coated with a high tack, medical-grade adhesive, which when applied to the patient's skin, is suitable for long-term monitoring, such as, for example two days or longer. Portions of the top surface of the bottom base **310** are also coated with a medical-grade adhesive, as the bottom base **310** and the top base **360** are adhered together during assembly of the wireless sensor **102**.

[0098] The removable battery isolator **320** is a flexible strip made of an electrically insulating material that serves to block electrical communication between the battery **214** and an electrical contact (not shown) on the circuit board **340**. The battery isolator **320** is used to preserve battery power until the wireless sensor **102** is ready for use. The battery isolator **320** blocks electrical connection between the battery **214** and the circuit board **340** until the battery isolator **320** is removed from the wireless sensor **102**. The battery isolator **320** can be made of any material that possesses adequate flexibility to be slidably removed from its initial position and adequate dielectric properties so as to electrically isolate the battery from the circuit board **340**. For example, the battery isolator can be made of plastic, polymer film, paper, foam, combinations of such materials, or the like. The battery isolator **320** includes a pull tab **322** that extends through a slot **352** of the housing **350** when the wireless sensor **102** is assembled. The pull tab **322** can be textured to provide a frictional surface to aid in gripping and sliding the pull tab **322** out of its original assembled position. Once the battery isolator **320** is removed the battery

214 makes an electrical connection with the battery contact to energize the electronic components of the wireless sensor **102**.

[0099] The mounting frame **330** is a structural support element that helps secure the battery **214** to the circuit board **340**. The mounting frame **340** has wings **342** that, when assembled are slid between battery contacts **342** and the battery **214**. Additionally, the mounting frame **330** serves to provide rigid structure between the circuit board **340** and the bottom base **310**. According to some embodiments that include an acoustic respiratory sensor, the rigid structure transmits vibrational motion (vibrations) emanating from the patient (such as, for example, vibrational motions related to respiration, heartbeat, snoring, coughing, choking, wheezing, respiratory obstruction, and the like) to the accelerometer **210** positioned on the circuit board **340**.

[0100] The circuit board **340**, which may also be referred to herein as a substrate layer **340** and a circuit layer **340**, mechanically supports and electrically connects electrical components to perform many of the functions of the wireless sensor **102**. The circuit board **340** includes conduction tracks and connection pads. Such electrical components can include without limitation, the processor **202**, the storage device **204**, the wireless transceiver **206**, the accelerometer **210**, the gyroscope **212**, the magnetometer **214**, the temperature sensor **218**, the acoustic respiration sensor **220**, the ECG sensor **222**, the oximetry sensor **224**, the moisture sensor **226**, and the impedance sensor **228**. In an embodiment, the circuit board **340** is double sided having electronic components mounted on a top side and a battery contact (not shown) on a bottom side. Of course a skilled artisan will recognize other possibilities for mounting and interconnecting the electrical and electronic components of the wireless sensor **102**.

[0101] As illustrated in FIG. 3A, a battery holder **342** is attached to two sides of the top portion circuit board **340** and extends (forming a support structure) under the bottom side of the circuit board **340** to hold the battery **214** in position relative to the circuit board **340**. The battery holder **342** is made of electrically conductive material. In some embodiments, the battery **214** is a coin cell battery having a cathode on the top side and an anode on the bottom side. Electrical connection between the anode of the battery **214** and the circuit board **340** is made by way of the battery holder which is in electrical contact with the anode of the battery **214** and the circuit board **340**. The cathode of the battery **214** is positioned to touch a battery contact (not shown) on the bottom side of the circuit board **340**. In some embodiments, the battery contact includes a spring arm that applies force on the battery contact to ensure that contact is made between the anode of the battery **214** and the battery contact. During assembly and prior to use, the battery isolator **320** is inserted between the anode of the battery **214** and the battery connector to block electrical contact.

[0102] The housing **350** is a structural component that serves to contain and protect the components of the wireless sensor **102**. The housing **350** can be made of any material that is capable of adequately protecting the electronic components of the wireless sensor **102**. Examples of such materials include without limitation thermoplastics and thermosetting polymers. The housing **350** includes a slot **352** through which the battery isolator **320** is inserted during assembly. The housing **350** also includes a rim **354** that extends around the outer surface of the housing **350**. The rim

354 is used to secure the housing **350** in position relative to the bottom base **310** and the top base **360** when the wireless sensor **102** is assembled.

[0103] Assembly of the wireless sensor **102** is as follows: The circuit board **340** and battery holder **342** holding the battery **214** are placed into the housing **350**. The wings **332** of the mounting frame **330** are inserted in between the battery **214** and the battery holder **342**, so as to align the mounting frame **330** with the circuit board **340**. The battery isolator **320** is then positioned between the battery contact and the battery **214**. The pull tab **322** of the battery isolator **320** is then fed through the slot **352** in the housing **350**. The top base **360** is then positioned over the housing **350**, which now houses the assembled circuit board **340**, battery holder **342**, battery **214**, mounting frame **330**, and battery isolator **320**, using the cut-out **362** for alignment. The rim **354** of the housing **350** adheres to the bottom surface of the top base **360**, which is coated with high tack, medical-grade adhesive. The partial assembly, which now includes the top base **360**, the housing **350**, the circuit board **340**, the battery holder **342**, the battery **214**, the mounting frame **330**, and the battery isolator **320**, is positioned centrally onto the top surface of the bottom base **310**, aligning the edges of the base top **360** with the edges of the base bottom **310**. In some embodiments, a coupon (or die cutting tool) is used to cut away excess portions of the now combined top and bottom bases **360** and **310** to form a final shape of the wireless sensor **102**. The bottom surface of the bottom base **310** is then coated with a high tack, medical-grade adhesive, and a release liner (not shown) is placed on the bottom surface of the bottom base **310** to protect the adhesive until it is time for use.

[0104] A schematic perspective view of the assembled wireless sensor **102** is illustrated in FIG. 3B. Also illustrated in FIG. 3B is a button/switch **324** located on a top portion of the housing **350**. The button/switch **324** can be used to change modes of the wireless sensor **102**. For example, in some embodiments, pressing and holding the button/switch **324** can cause the wireless sensor **102** to switch into a pairing mode of operation. The pairing mode is used to associate the wireless sensor **102** with a patient monitor **106** or with an extender/repeater **107**. FIG. 3C provides a schematic side view of an embodiment of the assembled wireless sensor **102** with cross-section line A-A identified.

[0105] Referring now to FIGS. 4A and 4B, an embodiment of the wireless sensor **102** is disclosed which includes a temperature sensor **218**. FIG. 4A is a schematic cross-sectional view, sectioned along line A-A of FIG. 3C, illustrating an assembled embodiment of the disclosed wireless sensor **102** which includes the temperature sensor **218**. For easier visibility, the battery isolator **320** and the battery holder **342** are not illustrated. FIG. 4B is a schematic bottom view of the embodiment of the disclosed wireless sensor of FIG. 4A. The bottom surface of the bottom base **310** is illustrated. Also illustrated in phantom (i.e., dotted lines) is the outline of cut-out **362** which also indicates the position of the housing **350** in relation to the bottom surface of the bottom base **310**.

[0106] As explained above with respect to the assembly of the wireless sensor **102**, the top surface of the bottom base **310** is in contact with and adhered to the bottom surface of the top base **360**. The rim **354** of the housing **350** is sandwiched between the two bases **310** and **360** to secure the housing **350**. The housing **350** also protrudes through the

cut-out 362 of the top base 360. Within the housing, the battery 214 and the mounting frame 330 are adjacent the top surface of the bottom base 310.

[0107] As illustrated in FIG. 4A, the temperature sensor 218 is mounted on the circuit board 340. To perform its temperature sensing function, the temperature sensor 218 is in thermal contact with the patient's skin. To achieve this, structure to transmit thermal energy from the patient's body to the temperature sensor 218 is provided. In particular, inputs to the temperature sensor 218 are thermally connected to multiple through-hole vias 410 located in the circuit board 340. A through-hole via is a small vertical opening or pathway in the circuit board 340 through which thermally and/or electrically conductive material can be placed, thereby permitting transmission of thermal and/or electrical energy from one side of the circuit board 340 to the other side. Under the through-hole vias 410 is an aperture or opening 404 which extends through the mounting frame 330 (to form a mounting frame aperture) and through the bottom base 310 of the wireless sensor 102. The aperture 404 provides access from the temperature sensor 218 to the patient's skin when the wireless sensor 102 is worn by the patient. The aperture 404 and the through-hole vias 410 are filled with thermally conductive material 402. Thermally conductive materials are well known in the art and can include, by way of non-limiting example, thermally conductive elastomers, polymers, and resins, to name a few. Illustratively, in operation, the wireless sensor 102 is affixed to the patient's skin. The thermally conductive material 402, exposed to the patient's skin, transmits thermal energy from the patient's body through the aperture 404 and the through-hole vias 410 to arrive at the inputs to the temperature sensor 218.

[0108] Advantageously, the disclosed wireless sensor 102 can measure the patient's body core temperature (an established and useful vital sign) with the temperature sensor 218 using a technique by which deep tissue temperature can be measured from the skin surface. In the human body, there is a natural heat flux between the body core and the skin surface because the body core temperature is typically at a higher temperature than that of the skin surface. Thus heat flows from the body core to the skin. By insulating the skin surface at and around the point at which the skin temperature is measured—thereby blocking heat from escaping—the temperature gradient between the body core and the skin surface will decrease. The skin temperature, under the insulated area will rise until it reaches equilibrium with the warmest region (i.e., the body core) under the insulation, thereby approaching the body core temperature. When equilibrium is reached, the skin temperature is equal to the core body temperature. Advantageously, the bottom base 310 and top base 360 of the wireless sensor 102, which are in contact with the patient's skin around the temperature sensor 218, possess thermal insulation properties. Illustratively, by way of non-limiting example, the bottom base 310 and top base 360 can be made thermally insulating materials including polyurethane foam, polystyrene foam, neoprene foam, neoprene rubber, polyester (Mylar), polytetrafluoroethylene (PTFE), silicone foam, silicone rubber, or the like. Accordingly, the temperature sensor 218 can measure the patient's body core temperature.

[0109] FIG. 4C is a schematic exploded perspective view of the embodiment of the disclosed wireless sensor of FIGS. 4A and 4B. As shown, the temperature sensor 218 is

mounted on the top surface of the circuit board 340. The aperture 404 extends through the mounting frame 330 and the bottom base 310 and is aligned vertically with the through-hole vias 410 (not shown in FIG. 4C) and the temperature sensor 218. The aperture 404 and the through-hole vias 410 are filled with thermally conductive material 402. Thus the disclosed structure provides thermal connectivity between the patient's skin and the temperature sensor 218.

[0110] Referring now to FIGS. 5A and 5B, an embodiment of the wireless sensor 102 is disclosed which includes an acoustic respiration sensor 220. FIG. 5A is a schematic cross-sectional view, sectioned along line A-A of FIG. 3C, illustrating an assembled embodiment of the disclosed wireless sensor 102 which includes the acoustic respiration sensor 220. For easier visibility, the battery isolator 320 and the battery holder 342 are not illustrated. FIG. 5B is a schematic bottom view of the embodiment of the disclosed wireless sensor of FIG. 5A. The bottom surface of the bottom base 310 is illustrated. Also illustrated in phantom (i.e., dotted lines) is the outline of cut-out 362 which indicates the position of the housing 350 in relation to the bottom surface of the bottom base 310.

[0111] As illustrated in FIG. 5A, the acoustic respiration sensor 220 is mounted underneath the battery 214. Operationally, the acoustic respiration sensor 220 detects vibratory motion emanating from the patient's body (e.g., the patient's chest) and mechanically transmits the detected vibratory motion to the accelerometer 210. The accelerometer 210 senses the mechanically transmitted vibratory motion. The signal collected by accelerometer 210 can be processed to extract the vibratory motion from other sensed acceleration signals. Examples of such vibratory motion can include, without limitation, heart beats, respiration activity, coughing, wheezing, snoring, choking, and respiratory obstruction (e.g., apneic events). To mechanically transmit the sensed vibratory motion effectively, the acoustic respiration sensor 220 is in rigid structural contact with the accelerometer 210. To achieve this, the acoustic respiration sensor 220 is mounted to the bottom side of the battery 214. In particular, the acoustic respiration sensor 220 includes a rim 221 that is sandwiched between the bottom surface of the battery 214 and the bottom base 310. Accordingly, the rim 221 serves to rigidly secure the acoustic respiration sensor 220 to the bottom surface of the battery 214.

[0112] As illustrated in FIG. 5A, the acoustic respiration sensor 220 protrudes through an aperture or opening 502 in the bottom base 310, beyond the plane created by the bottom base 310. This is to ensure that the acoustic respiration sensor 220 is in direct contact with the patient's body (e.g., chest) so as to sense the vibrational motion emanating from the patient. Within the acoustic respiration sensor 220 is a flexible wire or other such structure under slight tension such that when the wire is exposed to vibratory motion, it will vibrate in a manner that is proportional to the sensed vibratory motion with respect to both frequency and magnitude of the sensed vibratory motion. The acoustic respiration sensor 220 is configured to transmit the sensed vibratory motion through rigid structures of the wireless sensor 102 such that the transmitted vibratory motion is sensed by the accelerometer 210. The rigid structure includes the battery 214 and the circuit board 340.

[0113] FIG. 5C is a schematic exploded perspective view of the embodiment of the disclosed wireless sensor of FIGS.

5A-B. As shown, the accelerometer 210 is mounted on the top surface of the circuit board 340 over the battery 214 which is secured underneath the circuit board 340. The acoustic respiration sensor 220 (not shown in FIG. 5C) fits between the battery 214 and the bottom base 310. The aperture 502 extends through the bottom base 310 and is aligned vertically with battery 214 such that the acoustic respiration sensor 220 is secured to rigid structure of the wireless sensor 102. Thus the disclosed structure provides the ability for the acoustic respiration sensor 220 to mechanically transmit vibratory motion from the patient's chest to the accelerometer 210.

[0114] FIGS. 6A-C illustrate an embodiment of the disclosed wireless sensor 102 which includes a temperature sensor 218 and an acoustic respiration sensor 220. FIG. 6A is a schematic cross-sectional view, sectioned along line A-A of FIG. 3C, illustrating an assembled embodiment of the disclosed wireless sensor 102 which includes the temperature sensor 218 and acoustic respiration sensor 220. For easier visibility, the battery isolator 320 and the battery holder 342 are not illustrated. FIG. 6B is a schematic bottom view of the embodiment of the disclosed wireless sensor of FIG. 6A. FIG. 6C is a schematic exploded perspective view of the embodiment of the disclosed wireless sensor 102 of FIGS. 6A and 6B.

[0115] Structurally, the embodiment depicted in FIGS. 6A-C is a combination of the embodiments depicted in FIGS. 4A-C and 5A-C. As illustrated in FIGS. 6A-B, the temperature sensor 218 is mounted on the circuit board 340. As previously described, inputs to the temperature sensor 218 are thermally coupled to multiple through-hole vias 410 located in the circuit board 340. Under the through-hole vias 410 is an aperture 404 which extends through the mounting frame 330 and through the bottom base 310 of the wireless sensor 102. The aperture 404 provides access from the temperature sensor 218 to the patient's skin when the wireless sensor 102 is worn by the patient. The aperture 404 and the through-hole vias 410 are filled with thermally conductive material 402. In operation, the wireless sensor 102 is affixed to the patient's skin. The thermally conductive material 402, exposed to the patient's skin, transmits thermal energy from the patient's body through the aperture 404 and the through-hole vias 410 to arrive at the inputs to the temperature sensor 218.

[0116] Also as illustrated in FIGS. 6A-B, the acoustic respiration sensor 220 is mounted underneath the battery 214. In particular, the acoustic respiration sensor 220 includes rim 221 that is sandwiched between the bottom surface of the battery 214 and the bottom base 310. Accordingly, the rim 221 serves to rigidly secure the acoustic respiration sensor 220 to the bottom surface of the battery 214. The acoustic respiration sensor 220 protrudes through the aperture 502 in the bottom base 310, beyond the plane created by the bottom base 310. The acoustic respiration sensor 220 is configured to transmit vibratory motion sensed from the patient (e.g., from the patient's chest) through rigid structures of the wireless sensor 102 such that the transmitted vibratory motion is sensed by the accelerometer 210. The rigid structure includes the battery 214 and the circuit board 340.

[0117] FIG. 6C is a schematic exploded perspective view of the embodiment of the disclosed wireless sensor of FIGS. 6A and 6B. As shown, the temperature sensor 218 is mounted on the top surface of the circuit board 340. The

aperture 404 extends through the mounting frame 330 and the bottom base 310 and is aligned vertically with the through-hole vias 410 (not shown in FIG. 4C) and the temperature sensor 218. The aperture 404 and the through-hole vias 410 are filled with thermally conductive material 402. Additionally, the accelerometer 210 is mounted on the top surface of the circuit board 340 over the battery 214 which is secured underneath the circuit board 340. The acoustic respiration sensor 220 (not shown in FIG. 6C) fits between the battery 214 and the bottom base 310. In some embodiments, the acoustic respiration sensor 220 abuts against the mounting frame 330 in a manner such that the acoustic respiration sensor 220, the mounting frame 330, the battery 214 and the circuit board 340 form a rigid structure capable of mechanically transmitting vibratory motion sensed by the acoustic respiration sensor 220 to the accelerometer 210 mounted on the circuit board 340. The aperture 502 extends through the bottom base 310 and is aligned vertically with battery 214 such that the acoustic respiration sensor 220 is secured to rigid structure of the wireless sensor 102. Thus the disclosed embodiment provides thermal connectivity between the patient's skin and the temperature sensor 218 and the ability for the acoustic respiration sensor 220 to mechanically transmit vibratory motion from the patient's chest to the accelerometer 210.

[0118] Advantageously, the embodiment disclosed in FIGS. 6A-C is capable of providing, among other things, three vital signs: body core temperature, pulse rate, and respiration rate. Vital signs are measurements of the body's most basic functions and are used routinely by healthcare providers to assess and monitor a patient's status. The patient's body core temperature can be provided by the temperature sensor 218. The patient's pulse rate and respiration rate can be provided by the acoustic respiration sensor 220 in combination with the accelerometer 210.

[0119] Referring to FIGS. 7A-F, an embodiment of the disclosed wireless sensor 102 is shown which includes an electrocardiogram (ECG) sensor 222. Chip-scale and/or component-scale ECG sensors, suitable for mounting on circuit boards are known in the art. Illustratively, by way of non-limiting example, solid state ECG sensors are offered by Texas Instruments and by Plessey Semiconductors Ltd., to name a few. FIG. 7A is a perspective view of the embodiment of the disclosed patient-worn wireless sensor 102 having an ECG sensor 222 including an ECG lead 706 that extends from the housing 350. The wireless sensor 102 is adhered to the patient's chest, for example, over the manubrium as illustrated in FIG. 7A. The ECG lead 706 extends from the housing 350 of the wireless sensor 102 to a location on the patient's chest suitable to sense electrical signals generated by the patient's heart. The ECG lead 706 is in electrical communication with an ECG electrode 707 which, in operation, is adhered to the patient's chest. In certain embodiments, the ECG electrode 707 includes conducting gel embedded in the middle of a self-adhesive pad. The ECG electrode 707 senses electrical signals from the patient's chest and transmits the sensed signals, via the lead 706, to the ECG sensor 222. The electrode 707 adheres to the patient's skin and senses electrical signals therefrom. A skilled artisan will appreciate that many structures, forms, and formats of ECG electrodes are well known in the art and can be used to implement the ECG electrode 707.

[0120] As illustrated in FIG. 7A, the ECG lead 706 extends to the left side of the patient's chest to a position

across the heart from where the wireless sensor 102 is located. Another ECG electrode 702 (described below), also in contact with the patient's skin, is formed beneath the housing 350 at the bottom base 310. Thus, a vector is formed between the ECG lead electrode 707 and the ECG electrode 702 by which the electrical signals of the patient's heart can be sensed. Illustratively, when the electrodes 702 and 707 are positioned as depicted in FIG. 7A, the ECG sensor 222 can sense ECG signals that are similar in morphology to ECG signals detected on Lead I or Lead II of a standard 12-lead ECG.

[0121] FIG. 7B is a schematic assembled perspective view of the embodiment of the disclosed wireless sensor 102 of FIG. 7A. The ECG lead 706 is connected to the ECG sensor 222 (shown in FIG. 7D) which is mounted on the circuit board 340. As illustrated in FIG. 7B, the ECG lead extends through the housing 350 to a lockable retractable reel 708 that stores the ECG lead 706 in a coil when not in use. The ECG lead 706 can be extended from the reel 708 and locked in the desired position, thereby enabling placement of the ECG lead electrode 707 at a desired location on the patient's chest. In some embodiments, the locking mechanism is engaged and disengaged by applying a pulling force on the lead 706. Various forms and versions of lockable retractable reels are well known in the art and may be used to implement the reel 708.

[0122] FIG. 7C provides a schematic side view of the embodiment of the assembled wireless sensor 102 of FIGS. 7A and 7B with cross-section line B-B identified. FIG. 7D is a cross-sectional view of the embodiment of FIGS. 7A-C sectioned along line B-B. As illustrated in FIG. 7D, the ECG sensor 222 is mounted on the circuit board 340. To perform its sensing function, the ECG sensor 222 is in electrical contact with at least two points on the patient's skin. Two electrodes 702 and 707 are provided to achieve this purpose. While ECG electrode 707 has been described above, description of the ECG electrode 702 follows herewith.

[0123] ECG electrode 702 is located within the bottom base 310 of the wireless sensor 102. An input to the ECG sensor 222 is electrically connected to multiple through-hole vias 710 located in the circuit board 340. As previously described, through-hole vias are small vertical openings, or pathways, in the circuit board 340 through which electrically conductive material can be placed, thereby permitting transmission of electrical signals from one side of the circuit board 340 to the other side. Under the through-hole vias 710 is an aperture or opening 704 which extends through the mounting frame 330 (to form a mounting frame aperture) and through the bottom base 310 of the wireless sensor 102. The aperture 704 provides access from the ECG sensor 222 to the patient's skin when the wireless sensor 102 is worn by the patient. The aperture 704 and the through-hole vias 710 are filled with electrically conductive material to form the ECG electrode 702. Electrically conductive materials are well known in the art and can include, by way of non-limiting example, electrically conductive silicones, elastomers, polymers, epoxies, and resins, to name a few. In operation, the wireless sensor 102 is affixed to the patient's skin and the ECG electrode 702, exposed to the patient's skin, senses and transmits electrical signals from the patient's skin surface through the aperture 704 and the through-hole vias 710 to arrive at an input to the ECG sensor 222.

[0124] FIG. 7E is a schematic bottom view of the embodiment of the disclosed wireless sensor of FIGS. 7A-D. The bottom surface of the bottom base 310 is illustrated. Also illustrated in phantom (i.e., dotted lines) are the outline of cut-out 362 which also indicates the position of the housing 350 in relation to the bottom surface of the bottom base 310, and the lockable retractable reel 708. The ECG electrode 702 is also illustrated as it is positioned to make contact with the patient's skin. In some embodiments, the ECG electrode may be coated with a conducting gel to improve the electrode-to-skin interface.

[0125] FIG. 7F is a schematic exploded perspective view of the embodiment of the disclosed wireless sensor of FIGS. 7A-7E. As shown, the ECG sensor 222 is mounted on the top surface of the circuit board 340. The aperture 704 extends through the mounting frame 330 and the bottom base 310 and is aligned vertically with the through-hole vias 710 (not shown in FIG. 7F) and the ECG sensor 222. The aperture 704 and the through-hole vias 710 are filled with electrically conductive material to form electrode 702. Thus the disclosed structure provides electrical connectivity between the patient's skin and the ECG sensor 222.

[0126] FIG. 8A is a schematic exploded perspective view of an embodiment of the disclosed wireless sensor having a temperature sensor 218, an acoustic respiration sensor 220, and an ECG sensor 222. FIG. 8B is a schematic bottom view of the disclosed wireless sensor of FIG. 8A. Structurally, the embodiment depicted in FIGS. 8A-B is a combination of the embodiments depicted in FIGS. 4A-C and 5A-C and 7A-F. As illustrated in FIGS. 8A-B, the temperature sensor 218 is mounted on the circuit board 340. As previously described, inputs to the temperature sensor 218 are thermally coupled to multiple through-hole vias 410 located in the circuit board 340. Under the through-hole vias 410 is an aperture 404 which extends through the mounting frame 330 and through the bottom base 310 of the wireless sensor 102. The aperture 404 provides access from the temperature sensor 218 to the patient's skin when the wireless sensor 102 is worn by the patient. The aperture 404 and the through-hole vias 410 are filled with thermally conductive material 402.

[0127] The acoustic respiration sensor 220 is mounted underneath the battery 214, held in place by rim 221 that is sandwiched between the bottom surface of the battery 214 and the bottom base 310. Accordingly, the rim 221 serves to rigidly secure the acoustic respiration sensor 220 to the bottom surface of the battery 214. The acoustic respiration sensor 220 protrudes through the aperture 502 in the bottom base 310, beyond the plane created by the bottom base 310. The acoustic respiration sensor 220 transmits vibratory motion sensed from the patient (e.g., from the patient's chest) through rigid structures of the wireless sensor 102 such that the transmitted vibratory motion is sensed by the accelerometer 210. The rigid structure through which the vibratory motion is transmitted includes the battery 214 and the circuit board 340.

[0128] The ECG electrode 702 is located within the bottom base 310 of the wireless sensor 102. An input to the ECG sensor 222 is electrically coupled to multiple through-hole vias 710 located in the circuit board 340. Under the through-hole vias 710 is an aperture or opening 704 which extends through the mounting frame 330 and through the bottom base 310 of the wireless sensor 102. The aperture 704 provides access from the ECG sensor 222 to the patient's skin when the wireless sensor 102 is worn by the

patient. The aperture 704 and the through-hole vias 710 are filled with electrically conductive material to form the ECG electrode 702.

[0129] In operation, the wireless sensor 102 is affixed to the patient's skin. The thermally conductive material 402, exposed to the patient's skin, transmits thermal energy from the patient's body through the aperture 404 and the through-hole vias 410 to arrive at the inputs to the temperature sensor 218. The acoustic respiratory sensor 220 senses vibratory motion from the patient and mechanically transmits the vibratory motion to the accelerometer 210 mounted on the circuit board. And the ECG electrodes 702 and 707, exposed to the patient's skin, sense and transmit electrical signals from the patient's skin surface to arrive at inputs to the ECG sensor 222.

[0130] FIG. 8B is a schematic bottom view of the embodiment of the disclosed wireless sensor of FIG. 8A. The bottom surface of the bottom base 310 is illustrated. Also illustrated in phantom (i.e., dotted lines) are the outline of cut-out 362 and the lockable retractable reel 708. Three sensor access points are shown in FIG. 8B. The thermally conductive material 402 provides a pathway for thermal energy to be transmitted from the patient's skin the temperature sensor 218 mounted on the circuit board 340. The acoustic respiration sensor 220 is in direct contact with the patient's skin and in rigid structural contact with the accelerometer 210 so as to mechanically transmit sensed vibratory motion emanating from the patient to the accelerometer 210 mounted on the circuit board 340. And the ECG electrode 702 provides a pathway for electrical signals to be transmitted from the patient's skin to the ECG sensor 220 mounted on the circuit board 340.

[0131] In some scenarios, it may be desirable to pair, or associate, the wireless sensor 102 with the bedside patient monitor 106 to avoid interference from other wireless devices and/or to associate patient-specific information (stored, for example, on the patient monitor 106) with the sensor data that is being collected and transmitted by the wireless sensor 102. Illustratively, such patient-specific information can include, by way of non-limiting example, the patient's name, age, gender, weight, identification number (e.g., social security number, insurance number, hospital identification number, or the like), admission date, length of stay, physician's name and contact information, diagnoses, type of treatment, perfusion rate, hydration, nutrition, pressure ulcer formation risk assessments, patient turn protocol instructions, treatment plans, lab results, health score assessments, and the like. One skilled in the art will appreciate that numerous types of patient-specific information can be associated with the described patient-worn sensor without departing from the scope of the present disclosure. Additionally, pairing the wireless sensor 102 with the patient monitor 106 can be performed to provide data security and to protect patient confidentiality. Some wireless systems require the care provider to program the wireless sensor 102 to communicate with the correct patient monitor 106. Other wireless systems require a separate token or encryption key and several steps to pair the wireless device 102 with the correct bedside patient monitors 106. Some systems require the token to be connected to the bedside patient monitor 106, then connected to the wireless device 102, and then reconnected to the bedside patient monitor 106. In certain scenarios, it may be desirable to share wireless communication information between a wireless sensor 102 and a bedside

patient monitor 106 without a separate token or encryption key. For security purposes, it may be desirable to use security tokens to ensure that the correct bedside patient monitor 106 receives the correct wirelessly transmitted data. Security tokens prevent the bedside patient monitor 106 from accessing the transmitted data unless the wireless sensor 102 and bedside patient monitor 106 share the same password. The password may be a word, passphrase, or an array of randomly chosen bytes.

[0132] FIG. 9 illustrates an exemplary method of associating a wireless sensor 102 with a patient monitor 106, which may be referred to as "pairing." At block 902 the wireless sensor 102 is set to operate in a pairing mode. In an embodiment, a user initiates the pairing mode of operation for the wireless sensor 102. This may include powering on the wireless sensor 102, switching the wireless sensor 102 to a special pairing state, and/or the like. For example, in certain embodiments, the wireless sensor 102 may include a battery isolator 320 which, when removed, activates the wireless sensor 102. Upon activation, the default mode of operation is the pairing mode. In some embodiments, the wireless sensor 102 may have a button/switch 324 that can be used to activate the wireless sensor 102 and place it in the pairing mode of operation. For example, a depressible button/switch 324 can be located on the top portion of the housing 350. When the button/switch 324 is depressed and continuously held down, the wireless sensor 102 enters into the pairing mode of operation and remains in the pairing mode of operation for as long as the button/switch 324 is depressed.

[0133] As reflected at block 904, the wireless sensor 102 transmits a pairing signal indicating that it is ready to pair, or associate, with a patient monitor 106. According to some embodiments, the wireless transceiver 206 of the wireless sensor 102 is configured to emit a low-power pairing signal having a limited pairing signal transmission range. The limited pairing signal transmission range helps to prevent unintended or incidental association of the wireless sensor 102 with a patient monitor 106 that might be nearby but which is not intended to be paired with the wireless sensor 102. Such circumstances can occur in hospitals, healthcare facilities, nursing homes, and the like where patients, sensors 102 patient monitors 106 are located in close physical proximity to one another. In certain embodiments, the low-power pairing signal has a pairing signal transmission range of up to approximately three inches. In other embodiments, the low-power pairing signal has a pairing signal transmission range of up to approximately six inches. In other embodiments, the low-power pairing signal has a pairing signal transmission range of up to approximately one foot (i.e., twelve inches). A skilled artisan will recognize that other ranges can be used for the pairing signal transmission range.

[0134] Next, at block 906, the patient monitor 106, when within the pairing signal transmission range, receives the pairing signal from the wireless sensor 102. Upon detection of the pairing signal, the patient monitor 106, at block 908, associates with the wireless sensor 102 thereby configuring the wireless sensor 102 and patient monitor 106 to communicate with each other. Once the pairing is completed, the patient monitor 106 transmits a confirmation signal confirming that the patient-worn sensor 102 is associated with the patient monitor 106, thereby indicating that the pairing process has been successfully completed, as reflected in block 910. At block 912, the wireless sensor 102 receives the

confirmation signal. And at block 914, the wireless sensor 102 exits the pairing mode of operation and enters into a patient parameter sensing mode of operation. In the patient parameter sensing mode of operation, the patient-worn sensor 102 transmits a patient parameter sensing signal having a patient parameter sensing signal transmission range. The wireless sensor 102 increases the power of the patient parameter sensing signal transmission range to a standard operating range, such as for example, approximately three meters. In some embodiments, the patient parameter sensing signal transmission range is approximately ten feet. In some embodiments, the patient parameter sensing signal transmission range is approximately thirty feet. In certain embodiments, the pairing signal transmission range is between approximately three and twelve inches, while the patient parameter sensing signal transmission range is approximately ten feet. In such embodiments, there is at least an order of magnitude difference between the pairing signal transmission range and the patient parameter sensing signal transmission range. Thus, the pairing signal transmission range is substantially less than the patient parameter sensing signal transmission range. Once the wireless sensor 102 enters into the patient parameter sensing mode of operation, the wireless sensor 102 is then in condition to be placed on the patient to perform sensing and monitoring functions.

[0135] In certain embodiments, an extender/repeater 107 is used to communicate with the wireless sensor 102 instead of than a patient monitor 106. Pairing with the booster/repeater may be performed in the same manner described above with respect to FIG. 9.

[0136] According to certain embodiments, the disclosed patient monitoring system 100 helps to manage a patient that is at risk of forming one or more pressure ulcers by, among other things, detecting changes in the patient's orientation and by determining how long the patient remains in the present orientation. Advantageously, the system 100 can detect when the patient is repositioned and begin timing the duration that the patient remains in that new orientation. Thus, if the patient repositions on his own without the observation of a care provider, the monitoring system 100 can detect the repositioning event and restart a timer.

[0137] The patient monitoring system 100 can aid in the administration of a clinician-established turning protocol for the patient. For example, if the patient remains in an orientation beyond a predefined, clinician-prescribed duration, the system 100 can notify the patient and/or caretakers that the patient is due to be repositioned. The wireless sensor 102 obtains sensor information indicative of the patient's orientation (e.g., acceleration data), pre-processes the sensed data, and transmits it to a processing device capable of processing the measurement data, such as, for example, the patient monitor 106. Other devices capable of processing the measurement data include, without limitation, clinician devices 114, nurses' station systems 113, the multi-patient monitoring system 110, a dedicated processing node, or the like. For ease of illustration, the description herein will describe the processing device as the patient monitor 106; however, a skilled artisan will appreciate that a large number of processing devices may be used to perform the described functions without departing from the scope of the present disclosure.

[0138] The patient monitor 106 stores and further processes the received data to determine the patient's orientation. According to some embodiments, the patient monitor

106 can determine whether the patient is standing, sitting, or lying in the prone, supine, left side, or right side positions. The patient monitor 106 can store the determined orientation information and keep track of how long the patient remains in each determined orientation, thereby creating a continuous record of the patient's positional history. In certain embodiments, the information received from the wireless sensor 102 can be used to create a time-sequenced representation of the patient's positional history. This representation can be displayed on the patient monitor 106 or transmitted to a nurses' station or other processing node to enable caregivers to monitor the patient's position in bed. The time-sequenced representation can be viewed in real time and/or be accessed for playback. For example, if an alarm alerts the caregiver that the patient has exceeded the maximum amount of time to remain in the present orientation, the caregiver can access and review the historical sequence of the patient's orientations prior to and during that period of time to determine the next orientation to which the patient may be repositioned. In some embodiments, the system 100 suggests the orientation to which the patient may be repositioned.

[0139] Illustratively, the patient monitor 106 counts the number of in-bed turns performed by the patient and displays the amount of time that has elapsed since the patient last turned. When the elapsed time exceeds a clinician-defined duration (e.g., two hours), the patient monitor 106 displays an indication that the maximum time between patient turns has been exceeded. The patient monitor 106 can also transmit a notification to clinicians responsible for caring for the patient via, for example, the multi-patient monitoring system 110, a clinician notification device 114, or the like. The patient monitor 106 can also determine and display statistical information, such as the average, minimum, and maximum amount of time between turns for a given clinician-defined time period, such as for example, twenty-four hours. The patient monitor 106 can also determine and display the number of patient turns in the same orientation over a clinician-defined period of time. Similarly, the patient monitor 106 can display the total amount of time the patient has remained in each specific orientation within a clinician-defined period. Moreover, the patient monitor 106 can determine the frequency and duration of periods that the patient remained in clinically-defined acceptable orientations.

[0140] In some embodiments of the present disclosure, the patient monitor 106 accesses the patient's health records and clinician input via the network 108. Illustratively, the patients' positional history data, analyzed in view of the patient's health records, may reveal or suggest a turning protocol (or other treatment protocol) that will likely yield favorable clinical outcomes for the particular patient. Accordingly, the patient monitor 106 analyzes the accessed information in conjunction with the received information from the wireless sensor 102 to determine a recommended patient turn protocol (or other treatment protocol) for the patient.

[0141] According to some embodiments of the present disclosure, the patient monitor 106 assesses caregiver and facility compliance with the clinician-defined turning protocol established for the patient. For example, the patient monitor 106 can identify the number of times that the patient remains in a position for a period greater than the prescribed duration, as well as the length of each such overexposure.

The patient monitor **106** can also track the time between issuance of a notification, alert, or alarm and action taken in response to the event that triggered the issuance, corresponding to clinician response time.

[**0142**] FIG. **10** illustrates a method **1000** of estimating and monitoring the orientation of a patient in bed according to an embodiment of the present disclosure. The method **1000** also identifies when the patient changes orientation and keeps track of the amount of time the patient spends in that orientation. The patient orientations that may be determined include, without limitation, whether the patient is prone, supine, on the left side, on the right side, sitting, and lying. In some embodiments, the patient monitor **106** determines the precise orientation of the patient's body. For example, the patient monitor **106** can determine the degree to which the patient's body is inclined, vertically and/or horizontally, thereby generating an accurate description of the patient's orientation relative to the support structure (such as a bed) upon which the patient lies.

[**0143**] According to an embodiment of the present disclosure, measurements from the accelerometer **210** of the wireless sensor **102** are used to determine the patient's orientation. The accelerometer **210** measures linear acceleration of the patient with respect to gravity. In some embodiments the accelerometer **210** measures linear acceleration in three axes. One axis, referred to as "roll," corresponds to the longitudinal axis of the patient's body. Accordingly, the roll reference measurement is used to determine whether the patient is in the prone position (i.e., face down), the supine position (i.e., face up), or on a side. Another reference axis of the accelerometer **210** is referred to as "pitch." The pitch axis corresponds to the locations about the patient's hip. Thus, the pitch measurement is used to determine whether the patient is sitting up or lying down. A third reference axis of the accelerometer **210** is referred to as "yaw." The yaw axis corresponds to the horizontal plane in which the patient is located. When in bed, the patient is supported by a surface structure that generally fixes the patient's orientation with respect to the yaw axis. Thus, in certain embodiments of the disclosed method **1000**, the yaw measurement is not used to determine the patient's orientation when in bed.

[**0144**] Illustratively, the described method **1000** continuously or periodically (e.g., every second) determines the patient's orientation based on the measurements of pitch and roll provided by the accelerometer **210**. The measurements are tracked over time, and the current measurement is compared to one or more measurements in the recent past (e.g., the previous few seconds) to determine whether an orientation change event has occurred.

[**0145**] The method **1000** is described in further detail herein with respect to FIG. **10**. The method **1000** begins at block **1002** in which acceleration measurement data are received from the wireless sensor **102** by a device capable of processing the measurement data, such as, for example, the patient monitor **106**. Other devices capable of processing the measurement data include, without limitation, clinician devices **114**, nurses' station systems **113**, the multi-patient monitoring system **110**, a processing node, or the like. For ease of illustration, the description herein will describe the processing device as the patient monitor **106**; however, a skilled artisan will appreciate that a large number of devices may be used to perform the described method **1000** without departing from the scope of the present disclosure.

[**0146**] The acceleration measurement data may be provided directly from the wireless sensor **102** to the patient monitor **106**, or the measurement data may be relayed over a network such as network **108**, by an extender/repeater **107**, for example. The acceleration measurement data may be initially sampled at a sampling rate suitable to provide an acceptable degree of precision, such as for example, 100 Hz. In some embodiments, the measured data are sub-sampled by the wireless sensor **102** before being transmitted in order to reduce power consumption of the battery **214** of the wireless sensor **102**. In an embodiment, the acceleration measurement data are initially sampled at 100 Hz and subsequently down-sampled, for transmission purposes, to a rate of 26 Hz. In an embodiment, the acceleration measurement data are initially sampled at a range between approximately 10 Hz and approximately 200 Hz and subsequently down-sampled, for transmission purposes, at a rate between approximately 5 Hz and approximately 40 Hz. A skilled artisan will understand that many other sampling rates and sub-sampling rates may be used.

[**0147**] At block **1004**, the patient monitor **106** determines the present orientation of the patient. The received acceleration measurement data are processed to determine orientation values for the roll and pitch axes. The processed acceleration measurement data are provided in units of degrees, ranging from -180 degrees to +180 degrees. A lookup table, based on empirical data, provides a correlation between pairs of roll and pitch measurements and patient orientations. Illustratively, by way of non-limiting example, a roll measurement of 180 degrees can mean that the patient is on his back, and a pitch measurement of 0 degrees can mean that the patient is lying down. Thus the combination of a roll measurement of 180 degrees and a pitch measurement of 0 degrees can correspond to an orientation in which the patient is lying down on his back. Similarly, a combination of a roll measurement of 180 degrees and a pitch measurement of 90 degrees can correspond to an orientation in which the patient is lying on his right side.

[**0148**] FIG. **11A** illustrates an exemplary plot **1100** of processed accelerometer **210** data over time (from 0 to 450 seconds) used to determine a patient's orientation according to an embodiment of the present disclosure. Initially, at for example, 50 seconds, the data corresponding to the roll (i.e., body length) axis **1102** is at approximately 180 degrees, indicating that the patient is on his back (i.e., in the supine orientation). The data corresponding to the pitch (i.e., hip rotation) axis **1104** is at approximately 0 degrees, indicating that the patient is reclining. Thus, combining the orientation information provided by the accelerometer **210** with respect to the roll and pitch axes **1102** and **1104**, the patient is determined to be lying on his back. At approximately 360 seconds on the plot, denoted by vertical line **1106**, we see that the patient changes orientation. During a short transition period, the data oscillates, as illustrated in the data representing the pitch axis at transition point **1108** and in the data representing the roll axis at transition point **1110**. The oscillations can be caused by, among other things, jostling of the patient while moving from one position to the next. Shortly thereafter, the data achieves a steady state, as reflected by relatively stable graphs **1112** and **1114**. Notably, the data indicative of the pitch axis **1102** has moved from approximately 180 degrees to approximately 90 degrees. This corresponds to a ninety-degree rotation of the patient's longitudinal body axis to the patient's right side. The data

indicative of the roll axis remains at approximately zero degrees, indicating that the patient remains in the reclining position. Thus, combining the orientation information provided by the accelerometer 210 with respect to the roll and pitch axes 1112 and 1114, the patient is determined to be lying on his right side. In this manner, a lookup table of patient orientation change actions can be created. The table identifies profiles (e.g., combinations of pitch and roll axis measurements, within certain tolerances) of various possible orientations that a patient can assume while in bed. The table of profiles of patient orientation change actions can be based on empirical data that is collected and analyzed.

[0149] Referring back to FIG. 10, at block 1006, previous patient orientation determinations are extracted and combined with the current orientation determinations to form a time window of patient orientation information. For example, the time window can include information indicative of the patient's orientation from one or more time periods that are in close temporal proximity to the present information indicative of the patient's orientation, such as for example, the previous few seconds. Of course, any number of previous patient orientations can be selected for the time window. In an embodiment, the patient's orientation determinations for the previous two seconds are combined with the present determination to create a three-second time window of the patient's orientation. The purpose for creating the time window is to determine whether the patient has recently repositioned.

[0150] At block 1008, the time window is divided into segments for purposes of analysis. Any number of segments can be used for such analysis of the time window data. In an embodiment, the time window is segmented into three segments. In another embodiment, the time window is segmented into two segments. As illustrated in FIG. 11A at transition points 1108 and 1110, it is possible that the measured data used for the time window contains multiple sources of noise, some of which can have spikes of notable magnitude. To reduce the impact of the noise in the analysis, a segment value for each segment is determined. As disclosed at block 1010, the median value of the sampled data within each segment is used to determine the segment values for each segment. By taking the median value of each segment, a segment value is determined with minimal impact of potential noisy spikes. In certain embodiments, the segment value is a vector comprising values corresponding to each axis of measured data. Illustratively, by way of non-limiting example, each segment value comprises a vector including a roll axis segment component and a pitch axis segment component. According to some embodiments, the units of the determined segment values and/or segment components are in units of degrees ranging from -180 degrees to +180 degrees.

[0151] At block 1012 the median values of each segment are pairwise compared. Illustratively, by way of non-limiting example, a time window that is segmented into three sections would have three pairwise comparisons: the first segment value compared to the second segment value, the first segment value compared to the third segment value, and the second segment value compared to the third segment value.

[0152] At block 1014, each pairwise comparison is analyzed to determine whether an orientation change event occurred. The determination is made by comparing the magnitude of the difference of each pairwise comparison

with a predetermined threshold value. If the magnitude of the difference of a pairwise comparison exceeds the threshold, then an orientation change event is considered to have occurred. If the magnitude of the difference of a pairwise comparison does not exceed the threshold, then no change in orientation is considered to have occurred. Thus, a change that exceeds a certain threshold in the roll dimension corresponds to an orientation change event that includes a rotation about the longitudinal axis of the patient's body. Similarly, a change that exceeds a certain threshold in the pitch dimension corresponds to an orientation change event that includes a transition from sitting up to lying down, or vice versa. A change that exceeds a certain threshold in both the roll and pitch dimensions corresponds to an orientation change event that includes a rotation about the longitudinal axis of the patient's body and a transition from sitting up to lying down, or vice versa. According to an embodiment, the threshold is 45 degrees and thus, if the magnitude of difference between any two segment values is greater than 45 degrees, then an orientation change event is determined to have occurred. In another embodiment, an additional comparison is made between consecutive one-second segments of data to determine whether a change of at least 30 degrees has occurred. This is to prevent repeated posture changes, when for instance, the patient is in a posture near 135 degrees, that is, right in the middle between two postures.

[0153] If an orientation change event is determined to have occurred, then at block 1016, the detected event is classified. Reference is made to a look-up table of events which includes a set of profiles of orientation change actions or activities. In an embodiment, each profile includes four data points: a "before" and an "after" measurement for the roll axis, and a "before" and an "after" measurement for the pitch axis. For example, as illustrated in FIG. 11A, the profile of the orientation event activity of turning from lying on the back to lying on the right side can be as follows:

TABLE 1

Roil Before	Roil After	Pitch Before	Pitch After
180 degrees	90 degrees	0 degrees	0 degrees

[0154] As illustrated in Table 1, the roll axis changes from 180 degrees to 90 degrees indicating that the patient rotated from lying on his back to lying on his right side. The pitch axis does not change because the patient remains in a reclining orientation. The table of events is developed and updated off-line and is based on the analysis of empirical data of known orientation change events. Accordingly, classification of orientation change events can be performed by identifying in the look-up table of events the orientation event profile that matches the data of the pairwise comparison when the magnitude of the difference of the pairwise comparison exceeds the predetermined threshold.

[0155] At block 1018, a vote is placed for the classified event. Illustratively, for the example described with respect to Table 1, the vote would be for the orientation change event profile of turning from lying on the back to lying on the right side. At block 1020, the method 1000 repeats the acts of determining whether an orientation change event occurred, classifying the orientation change event (if an event occurred), and voting for the classified orientation change event (again, if an event occurred), for each pairwise

comparison. The maximum number of iterations for these blocks will be equal to the number of segments in the time window.

[0156] Once all of the pairwise comparisons have been analyzed, at block 1022, the method 1000 tallies the votes recorded at block 1018. The orientation change event that has the most votes is determined to be the orientation change event that occurred. The determined orientation change event is then reported as the orientation of the patient. At block 1024, an orientation duration timer is reset to keep track of the time the patient remains in the new orientation. The method 1000 then returns to block 1002 to begin the analysis again with respect to the next incremental (e.g., second) of measurement data.

[0157] If at block 1014, none of the pairwise comparisons result in a detected orientation change event (i.e., the patient has remained in the same orientation throughout the entire time window) then the method 1000 progresses to block 1026 to determine whether the patient has remained in the present orientation for a period of time greater than a predefined maximum duration, which may also be referred to herein as a predetermined duration or a predetermined maximum duration. If not, the method 1000 returns to block 1002 to begin the analysis again with respect to the next incremental set (e.g., second) of measurement data. If the patient has remained in the present orientation for a period of time greater than the predefined maximum duration, then at block 1028, an alert is sent to, for example, the patient's caregiver, to notify the caregiver that the patient should be repositioned. The method 1000 then returns to block 1002 to begin the analysis again with respect to the next incremental (e.g., second) of measurement data.

[0158] FIG. 11B is an exemplary plot of an embodiment of a patient position monitoring paradigm for determining when a patient's orientation needs to be changed, according to an embodiment of the present disclosure. In an embodiment, the plot 1102B may be part of a display to a caregiver on a bedside monitor, a multi-room monitor, both, or the like. The plot can be updated in real time, at predefined intervals, and/or manually. In other embodiments, the paradigm may be illustrative of the signal processing performed by a signal processor to determine when to activate an alarm informing a caregiver of the potential of a pressure ulcer if a patient is not repositioned. In these embodiments, each portion of the paradigm may be customized to a particular patient, patient demographics, hospital protocol, unit protocol such as, for example, a protocol specific to a surgical IOU or other hospital unit, home care, or the like.

[0159] In the illustrated embodiment, a patient's position is monitored over time. A vertical axis 1105B represents time and a horizontal axis 1107B represents a patient movement event, such as, for example, In the illustrated embodiment, an alarm is set to alert a caregiver when a patient has been in a certain position for 3 hours or more. The illustrated embodiment is a non-limiting example, as the alarm can be set to alert the caregiver at 1 hour, 2 hours, 3 hours, 4 hours, 5 hours, 6 hours, 7 hours, 8 hours, 9 hours, and/or 10 or more hours. The alarm can include a noise, color, and/or other indicator that will alert the caregiver. In some embodiments, the alarm can indicate to the caregiver that the patient has remained in the same position for a threshold amount of time (e.g., 3 hours). The threshold amount of time can be predefined or adjusted over time. In some embodiments, the alarm indicates to the caregiver that the patient has fallen,

moved into an incorrect position, left the bed and/or the like. In an embodiment, empirical data about a particular patient, or a group of like patients, can be used to customized some or all of the parameters for the alarm discussed herein.

[0160] As shown in FIG. 11B, the monitor begins monitoring a patient as the patient is in Position 1 (e.g., the patient is lying on their back, side, front, sitting slightly up, sitting mostly up, or the like). As the patient remains in Position 1, a timing mechanism starts and a line 1101B as its growth line. The slope of the line 1101B depicts a growth rate as the patient remains in the same position. As shown in the illustrated embodiment, the growth rate can be depicted linearly. In some embodiments, the growth rate can be linear, non-linear, exponential, and/or the like. In some embodiments, the growth rate is predefined. In some embodiments, the growth rate can change in real time and/or adjust to various physiological parameters and/or empirical data, as described below. The growth rate can depend on a number of factors and empirical data already known and/or determined by the system, depending on for example, how the patient's skin reacts to remaining in a single position, how fast negative effects experienced by the patient (e.g., pressure sores) form or heal, the particular position the patient is lying in, and/or demographic information about the patient, including the patient's age, health, blood perfusion rates, hydration, and/or nutrition, among others. Accordingly, in some embodiments, the growth rate can indicate a growth rate of the effects (e.g. bed sores) as the patient remains in the same position (e.g., Position 1) over a period of time.

[0161] As illustrated in FIG. 11B, the patient remains in Position 1 for approximately 2 hours. At that time, the patient turns and/or is turned by a caregiver to Position 2. In the illustrated embodiment, Position 2 is a different position from Position 1. When the patient turns and/or is turned, the timing mechanism can restart a new line 1102B and begin to measure, track, monitor, and/or calculate the amount of time the patient remains in Position 2.

[0162] At the same time, line 1101B transforms into its decay line. The decay line of line 1101B can comprise data relating to a decay rate of a bed sore, potential bed sore, particular area of a patient's skin, and/or the amount of time the patient or a group of like patients, or all patients, takes to recover from remaining in a particular position (e.g., Position 1), among other things. Similar to the growth rate, the decay rate can be linear, non-linear, and/or exponential, among others. In some embodiments, the decay rate is predefined. In some embodiments, the decay rate can change in real time and/or adjust to various physiological parameters and/or empirical data, as described below. The decay rate may depend on a number of factors and empirical data, depending on for example, how the patient's skin reacts to remaining in a single position, how fast negative effects experienced by the patient (e.g., pressure sores) heal, how quickly the patient recovers, the particular position the patient is lying in, and/or demographic information about the patient, including the patient's age, health, blood perfusion rates, hydration, and/or nutrition, among others. As shown in the illustrated embodiment, when the patient is in one or more positions that are not Position 1, the decay line of Position 1 continues to decay at the decay rate. That is, in an embodiment, the decay line of Position 1 will continue to decay at its decay rate through one or multiple other positions until it approaches zero so long as that other one or multiple positions do not include Position 1. In this example,

the decay rate, or recovery rate for example, approaches zero more quickly the longer the patient remains not in Position 1.

[0163] In the illustrated embodiment, the patient turns and/or is turned again at Turn 2. Turn 2 occurs at a time before the threshold amount of time is reached, and therefore, before the alarm alerts the caregiver to turn the patient. At Turn 2, the patient turns/is turned to Position 3. In some examples, Position 3 is the same as Position 1. In such embodiments, because the decay line of line 1101B associated with the previous Position 1 has reached zero, a line 1104B starts at zero as its growth line for Position 3/1. However in some examples, Position 3 is a different position from Position 1. In the illustrated example, Position 3 is different from Position 1 and its growth rate for line 1104B is different from that of Position 1. In some examples, the decay line of Position 1 can continue to decay as the decay line of Position 2 continues to decay when the patient turns and/or is turned to Position 3 as long as Position 3 is different from Positions 1 and 2. In this example, the patient can continue to heal as a result of the effects of remaining in both Positions 1 and 2. In some examples, Position 1 continues to decay as the patient turned and/or is turned to multiple positions, such as a second, third, fourth, and/or fifth or more positions.

[0164] As shown in the illustrated embodiment, the patient remains in Position 3 for a relatively short period of time. During that time, any effects of remaining in Position 2 begin to decay. Thereafter, however the patient turns and/or is turned back to Position 2. Advantageously, rather than restarting at time zero, the system can determine that the patient has turned back to Position 2 and the timing mechanism begins timing from the current value of the decay line of Line 1102B, which corresponds to point or time 1103B. Time 1103B is greater than zero in this example, but less than the threshold amount of time. Additionally, in this example, the time 1103B is less than the amount of time the patient originally remained in Position 2. In some embodiments time 1103B can be equal to the time the patient turned from Position 2. However, in the illustrated embodiment, the system can take into account the decay rate and the time the patient has spent recovering from remaining in Position 2. Thus, in the illustrated embodiment, Time 1103B can be determined by the system through a number of methods. For example, the system can subtract the recovery time from the growth time, and/or count down from the time of the turn (e.g., Turn 2), among other methods. Advantageously, the preferred embodiment of the system can ensure the patient does not exceed the threshold total time, taking into account the growth and decay rate, a patient spends in a particular location. Although in an embodiment, the system restarts the timer at each turn, without accounting for the previous time the patient spent at a particular position, such embodiments may not be as precise in allowing adequately recovery of tissue, blood pooling, or the like caused by the previous position, and therefore, a patient may be more likely to experience negative effects (e.g., bed sores). Accordingly, the preferred embodiment of the system can more precisely reduce a likelihood of a patient developing harmful effects, such as bed sores by ensuring a patient would not remain in a particular position for too long. Once the total time spent in a position, taking into account the patient's growth and decay rates, reaches the threshold time (e.g. 3 hours in this example), an alarm can alert the caregiver.

[0165] In some embodiments, the alarm will alert the caregiver until the patient turns and/or is turned again, for example as illustrated by Turn 4 in FIG. 11B. In some embodiments, the growth line will continue to grow, thus requiring longer for the line to decay, when a patient has not been turned within the threshold time. Such continued growth ensures that a patient will not be too soon returned to a position where the patient spent too much time and can help ensure that the corresponding tissue has sufficient time to recover from a particular patient position. In an embodiment, the decay rate of the line is adjusted to account for exceed the threshold limit. As shown in the illustrated embodiment, the decay rate is reduced after exceed a threshold, meaning it will take longer for the line corresponding to the alarmed position to reach zero.

[0166] As discussed, in an embodiment, when the patient turns and/or is turned after the time of the alarm, the growth line will exceed the threshold time, as indicated by the plot of FIG. 11B. Once the patient turns and/or is turned, the decay line can be shown above the threshold (e.g. alarm) line. In some examples, the patient may take longer to recover when the time spent in a particular position exceeds the threshold time. In some examples, the alarm can alert the caregiver that the decay line has reached the threshold time as the line continues to decay towards zero and the patient remains in a different position. In some embodiments, the alarm does not alert the caregiver that the decay line has passed the threshold time.

[0167] According to certain embodiments of the present disclosure, the patient monitor 106 determines the mobility status of the patient, e.g., whether the patient is ambulatory, standing, sitting, reclining, or falling. The wireless monitoring system 100 can include an alert system to alert the caregiver that the patient is falling, getting out of bed, or otherwise moving in a prohibited manner or in a manner that requires caregiver attention. The alert can be an audible and/or visual alarm on the monitoring system or transmitted to a caregiver (e.g., nurses' station system 113, clinician device 114, pager, cell phone, computer, or otherwise). Illustratively, the patient monitor 106 can display the patient's mobility status and transmit a notification that the patient is active and away from the bed. In some circumstances, the patient monitor 106 can determine whether the patient contravenes a clinician's order, such as, for example, instructions to remain in bed, or to walk to the bathroom only with the assistance of an attendant. In such circumstances, a notification, alert, or alarm can be transmitted to the appropriate caregivers.

[0168] In certain aspects, the information received from the wireless sensor 102 can be used to create a time-sequenced representation of the patient's movement. This representation can be displayed on the patient monitor or transmitted to a nurses' station or other processing node to enable the caregiver to monitor the patient. The time-sequenced representation can be viewed in real time and/or be recorded for playback. For example, if an alarm alerts the caregiver that the patient has fallen, the caregiver can access and review the historical sequence of the patient's movements prior to and during that period of time.

[0169] In some embodiments, the patient monitoring system 100 can predict a patient's risk of falling based on analysis of the patient's movement (e.g., gait) and other information (such as, for example, the patient's current medication regimen). When the patient monitor 106 deter-

mines that the patient's risk of falling is above a predetermined threshold, the patient monitor **106** can issue an alarm or alert to notify care providers of the identified risk in an effort to anticipate and therefore prevent a patient fall. Additionally, the patient monitor **106** can determine when a patient has fallen and issue the appropriate alarms and alerts to summon care provider assistance.

[0170] FIG. 12 illustrates a method **1200** of determining whether a patient has fallen according to an embodiment of the present disclosure. The method **1200** uses, among other things, information sensed by the accelerometer **210** and by the gyroscope **212** of the wireless sensor **102** to determine whether the patient has fallen. The method **1200** can be performed by the wireless sensor **102**, using its processor **202** and storage device **204**, or it can be performed by an external processing device that receives the sensed information from the wireless sensor **102**, such as, for example, the patient monitor **106**.

[0171] According to an embodiment of the present disclosure, measurements from the accelerometer **210** and the gyroscope **212** of the wireless sensor **102** are used, among other things, to determine whether the patient has fallen. As discussed above, the accelerometer **210** measures linear acceleration of the patient with respect to gravity in three axes. The three axes of the accelerometer **210** are represented in fixed, inertial references. The roll axis corresponds to the longitudinal axis of the patient's body. Accordingly, the roll reference measurement is used to determine whether the patient is in the prone position (i.e., face down), the supine position (i.e., face up), or on a side. The pitch axis corresponds to the locations about the patient's hip. Thus, the pitch measurement is used to determine whether the patient is upright or lying down. Advantageously, the pitch axis provided by the accelerometer **210** can be a useful source of information in determining whether a patient has fallen because it can indicate a change in the patient's orientation from standing to lying, a frequently-seen scenario when a patient falls. The yaw axis corresponds to the horizontal plane in which the patient is located.

[0172] The gyroscope **212** provides outputs responsive to sensed angular velocity of the wireless sensor **102**, as positioned on the patient, in three orthogonal axes corresponding to measurements of pitch, yaw, and roll. In contrast to the fixed, inertial reference frame relative to gravity of the accelerometer **210**, the frame of reference provided by the gyroscope is relative to the patient's body, which moves.

[0173] At block **1202**, the method **1200** begins in which acceleration measurement data and angular velocity data are received from the wireless sensor **102** by a device capable of processing the measurement data, such as, for example, the patient monitor **106**. Other devices capable of processing the measurement data include, without limitation, clinician devices **114**, nurses' station systems **113**, the multi-patient monitoring system **110**, or the like. For ease of illustration, the description herein will describe the processing device as the patient monitor **106**. A skilled artisan will appreciate that a large number of devices may be used to perform the described method **1200** without departing from the scope of the present disclosure.

[0174] At block **1204**, the received data are normalized, which may also be referred to as "scaling," to adjust values measured on different scales to a common scale, prior to further processing. According to an embodiment, training data are used to normalize the received data. The training

data can include empirical data of multiple fall scenarios as well as non-fall scenarios that can be challenging to discriminate from fall scenarios. The training data are collected and analyzed to serve as the basis for establishing a weight vector (discussed below with respect to block **1208**) used to determine whether a patient has fallen. The training data can include multiple falling and non-falling scenarios, performed multiple times, by multiple subjects. Illustratively, by way of non-limiting example, the training data can include the fall and non-fall scenarios described in Table 2.

TABLE 2

Fall and Non-Fall Scenarios
Fall forward from vertical, ending in left/right lateral position
Fall forward from vertical, ending in prone position
Fall backward, from vertical, ending in left/right lateral position
Fall backward from vertical, ending in supine position
Fall to left/right from vertical, ending in left/right lateral position
Fall to left/right from vertical, ending in prone position
Fall to left/right from vertical falling, ending in supine position
Collapse from vertical, ending in left/right lateral position
Collapse from vertical, ending in prone position
Collapse from vertical, ending in supine position
Fall from vertical onto knees
Fall from vertical to the left/right against a wall, sliding down
Take a step down repeatedly from a podium with left foot first
Take a step down repeatedly from a podium with right foot first
In bed: roll onto left/right side, falling out of bed
Sit down from vertical into a chair
Jump off mattress repeatedly
Stand quietly
Stumble vigorously and fall onto mattress

[0175] As with the received data, each sample of the training data includes six dimensions of information, corresponding to the three axes of accelerometer **210** data, and the three axes of gyroscope **212** data. Normalizing the received data standardizes the range of the variables of the received data. Since the range of values of raw data can vary widely, analytical algorithms may not work properly without normalization. For example, many classifiers calculate the distance between two points. If one of the independent variables has a broad range of values, the distance will be governed by this particular variable. Therefore, the range of all variables can be normalized so that each feature contributes approximately proportionately to the final distance. Normalization causes the values of each variable in the data to have zero-mean (when subtracting the mean in the numerator) and unit-variance. This can be performed by calculating standard scores. The general method of calculation is to determine the distribution mean and standard deviation for each variable of the entire set of training data. Next each determined mean is subtracted from the corresponding variable of the received data. Then the new value of each variable (having the mean already subtracted) is divided by the determined standard deviation. The result is a normalized set of values that can be further processed by the method **1200**.

[0176] At block **1206**, the normalized set of values is processed to determine features that are useful in determin-

ing whether a patient is falling. According to an embodiment, the method determines the following five features: the magnitude of the acceleration data (provided by the accelerometer **210**), the magnitude of the angular velocity data (provided by the gyroscope **212**), the magnitude of the jerk (i.e., the rate of change of acceleration); the fall duration which is used to characterize a fall starting point and a fall impact point, and the change in pitch between two consecutively received data points. Other features can be used in determining whether a patient is falling such as, by way of non-limiting example, vertical velocities.

[0177] The magnitude of the received acceleration data is determined by calculating the Euclidian norm of the three-dimensional vector made up of the measurements from the accelerometer's **210** three axes. As is well understood by an artisan, this corresponds to the square root of the sum of the squares of the three accelerometer values, pitch, roll and yaw. Similarly, the magnitude of the angular velocity data is determined by calculating the Euclidian norm of the three-dimensional vector made up of the measurements from the gyroscope's **212** three axes. The magnitude of the jerk, which can also be referred to as "jolt," "surge," or "lurch," is calculated by taking the derivative of the acceleration vector, and then calculating the Euclidean norm of the derivative.

[0178] The fall duration, which is a scalar value, is determined by evaluating the acceleration magnitude profile of the patient's motion over a short duration of time. In particular, as the fall begins, acceleration of the patient relative to gravity decreases because the patient is falling. (A patient that is not falling would register an acceleration value in the up and down dimension equal to the force of gravity (i.e., 1 g or approximately 9.80665 m/s²). Thus, if the magnitude of the acceleration is below a first threshold, then it is considered to be a starting point of a fall, and the value of the fall duration is incremented by 1. If the magnitude of the acceleration is above the first threshold, then the value of the fall duration is decremented by 1. In an embodiment, the first threshold is 0.6 g (or approximately 5.88399 m/s²). A second threshold is used to determine the impact point of the fall. In an embodiment, the second threshold is 0.8 g (or approximately 7.84532 m/s²). If the magnitude of the acceleration is below the second threshold, then it is considered to be an impact point of the fall, and the value of the fall duration is incremented by 1. If the magnitude of the acceleration is above the second threshold, then the value of the fall duration is decremented by 1.

[0179] The pitch change feature is the result of a comparison of the present pitch orientation (as determined by the accelerometer **210** data) with the pitch orientation determined one second earlier. As discussed above, the pitch dimension of the accelerometer data is useful in detecting a fall because it distinguishes between the patient being in an upright position (e.g., standing up or sitting up) and reclining. Thus a change in pitch from being upright to reclining can indicate that a fall has occurred. The output of block **1206** is a five-dimensional feature vector made up of the five determined features.

[0180] At block **1208**, a weight vector of values is applied to the determined features. According to certain embodiments, the inner product of the received five-dimensional feature vector and a weight vector is calculated. In certain embodiments, the weight vector is derived using a machine learning algorithm. Machine learning is a sub-field of com-

puter science based on the study of pattern recognition and computational learning theory in artificial intelligence. It includes the development of algorithms that can learn from and make predictions on data. Algorithms developed through machine learning operate by building a model from example inputs in order to make data-driven predictions or decisions, rather than following strictly static program instructions. Machine learning is employed in a range of computing tasks where use of explicit computer programs is infeasible. When employed in industrial contexts, machine learning methods may be referred to as predictive analytics or predictive modelling. As applied in the present disclosure, the machine learning system includes supervised learning, where the machine learning algorithm is presented with training data that include example inputs and their known outputs, given by a "teacher", and the goal is to learn a general rule that maps the inputs to the outputs. In an embodiment, Fisher's linear discriminant is employed to derive the weight vector. Fisher's linear discriminant is a method used to find a linear combination of features that characterizes or separates two or more classes of objects or events. The resulting combination may be used as a linear classifier or for dimensionality reduction before later classification. Other methods of machine learning that can be used with the present disclosure include, without limitation, linear discriminant analysis, analysis of variance, regression analysis, logistic regression, and probit regression, to name a few. A skilled artisan will recognize that many other machine learning algorithms can be used to determine the weight vector without departing from the scope of the present disclosure.

[0181] The training data, described above, include empirical data collected from multiple fall and non-fall scenarios which can be used to identify the predictive indicators of patient falls. Illustratively, for each training scenario, the five features described above with respect to block **1206** are determined and provided as input to the machine learning system. Additionally, an output is provided for each training scenario that identifies whether the scenario describes a falling event or a non-falling event. The machine learning system analyzes the training data to derive a rule that maps the inputs to the outputs. According to certain embodiments of the present disclosure, the output of the machine learning system is five-dimensional weight vector that weights each of the five features according to their relative value in determining whether or not a fall has occurred. The weight vector is determined off-line and is provided as a fixed, five-dimensional vector to the method **1200**. Of course, the weight vector can be updated, based on analysis of additional empirical data.

[0182] The inner product (also referred to as the "dot product" and the "scalar product") of the received five-dimensional feature vector and the weight vector is calculated in a manner well understood by skilled artisans. The inner product yields a scalar value, also referred to herein as an activation value, that may be either positive or negative. At block **1210**, the method **1200** determines whether a fall has been detected. According to some embodiments, the sign of the inner product of the received five-dimensional feature vector and the weight vector indicates whether a fall has occurred. If the inner product is less than zero, then no fall has been detected, and the method returns to block **1202** to begin analyzing the next set of data from the wireless sensor **102**. If the inner product is greater than zero, then a fall has

been detected and the method **1200** progresses to block **1214**, where a notification, alarm, and/or alert indicating that the patient has fallen is transmitted to, for example, clinician devices **114**, nurses' station systems **113**, multi-patient monitoring system **110**, and the like. The method returns to block **1202** to begin analyzing the next set of data from the wireless sensor **102**.

[**0183**] In some embodiments, the system can determine a spatial location of the patient within the patient's room. The system can monitor the room and spatially monitor and/or calculate how long the patient has been in a position, when the patient was in the position, and/or how long the patient was in the position, among other parameters. As discussed above, the system uses, among other things, information sensed by the accelerometer **210** and by the gyroscope **212** of the wireless sensor **102** to track the patient. This method can be performed by the wireless sensor **102**, using its processor **202** and storage device **204**, or it can be performed by an external processing device that receives the sensed information from the wireless sensor **102**, such as, for example, the patient monitor **106**.

[**0184**] In some embodiments, the system can determine the position of the patient within the patient's room, relative to certain features of the patient's room, such as the patient's bed, a bathroom, a monitor, a doorway, and/or a window, among other room feature. In particular, using methods described herein, the system can determine a patient's vertical position, vertical displacement, horizontal position, horizontal displacement, angular position and/or angular displacement in the patient's room. For example, the accelerometer **210** and/or the gyroscope **212** can monitor the patient's movements as the patient walks throughout the patient's room. The system can determine whether the patient is falling, getting out of bed, or otherwise moving in a prohibited manner or in a manner that requires caregiver attention.

[**0185**] According to some embodiments, measurements from the accelerometer **210** and the gyroscope **212** of the wireless sensor **102** are used, among other things, to determine whether the patient is bending down and/or has fallen and/or where the patient has fallen (for example, by measuring the vertical displacement of the patient and/or the height of the patient relative to the floor). In some embodiments in which the patient has fallen, the clinician can determine the location of the fall according to an embodiment of the present disclosure. As discussed above, the accelerometer **210** measures linear acceleration of the patient with respect to gravity in three axes. The three axes of the accelerometer **210** are represented in fixed, inertial references. The gyroscope **212** provides outputs responsive to sensed angular velocity of the wireless sensor **102**, as positioned on the patient, in three orthogonal axes corresponding to measurements of pitch, yaw, and roll. Based on these measurements, the system can determine whether the patient has fallen according to methods described herein.

[**0186**] In such configurations, the system can record the position of the patient. In certain aspects, the information received from the wireless sensor **102** can be used to create a time-sequenced representation of the patient's movement. This representation can be displayed on the display **120** or transmitted to a nurses' station or other processing node to enable the caregiver to monitor the patient. The time-sequenced representation can be viewed in real time and/or be recorded for playback. For example, if an alarm alerts the

caregiver that the patient has fallen, the caregiver can access and review the historical sequence of the patient's movements prior to and during that period of time.

[**0187**] FIGS. **15A-H** illustrate various configurations of a room display displayed on the patient display monitor. As illustrated in FIGS. **15A-H**, the caregiver and/or patient can select any number of room items and/or configurations of the room items. The caregiver can select a room item, and place it within the room on the room display. The caregiver can rotate and/or place the room item in any configuration. In an embodiment, the caregiver could select the location of a major element of a room at a time. For example, the caregiver could select a position of the bed, then a position of the bathroom, then a position of the door, equipment, tables, chairs, couches, etc. In other embodiments, various room layout approximation are some to fully presented in selection screens and the determination of layout is made in one or just a few caregiver selections.

[**0188**] FIG. **16** illustrates an example method **1600** for detecting and/or predicting a patient's fall, determining a particular location of a patient within a patient's room, and/or determining whether the patient has moved outside of a prescribed movement of the patient, among others, for example.

[**0189**] At block **1602**, the caregiver can enter a room configuration. For example, the caregiver can select any number of room items to be displayed in any number of configurations within a patient room display. The room items can include a patient's bed, a bathroom, a monitor, a doorway, and/or a window, among other room items. The caregiver can select a room item by selecting, dragging, and/or dropping each room item around the room display. In some embodiments, the caregiver can select a certain size for each room item. In some embodiments, the caregiver can simply select a room item and select the location within the room display for the room item to be oriented and displayed. In some embodiments, the room item can be snapped into place in the room display.

[**0190**] At block **1604**, the caregiver can optionally enter a movement prescription. For example, the caregiver can enter instructions to the patient, including instructions to remain in bed, and/or to walk to the bathroom only with the assistance of an attendant.

[**0191**] At block **1608**, one or more of the sensors described herein can be activated. In some examples, the caregiver manually activates the one or more sensors. In some examples, the system activates the one or more sensors automatically to begin tracking, monitoring, measuring, and/or calculating certain physiological parameters, according to methods described herein.

[**0192**] At block **1610**, the patient monitoring system **100** can predict and/or detect a patient's fall and/or risk of falling based on analysis of the patient's movement (e.g., gait) and other information (such as, for example, the patient's current medication regimen). At block **1612**, when the patient monitor **106** determines that the patient's risk of falling is above a predetermined threshold, the patient monitor **106** can issue an alarm or alert to notify care providers of the identified risk in an effort to anticipate and therefore prevent a patient fall. Additionally, the patient monitor **106** can determine when a patient has fallen and issue the appropriate alarms and alerts to summon care provider assistance. The alert system can alert the caregiver that the patient is falling, getting out of bed, or otherwise moving in a prohibited

manner or in a manner that requires caregiver attention. The alert can be an audible and/or visual alarm on the monitoring system or transmitted to a caregiver (e.g., nurses' station system 113, clinician device 114, pager, cell phone, computer, or otherwise).

[0193] If the patient monitoring system has not detected a patient's fall, the patient monitoring system 100 can optionally determine whether the patient has moved outside of the movement prescription. For example, as described above, the patient monitor 106 can determine the mobility status of the patient, e.g., whether the patient is ambulatory, standing, sitting, reclining, or falling.

[0194] If the patient monitoring system 100 determines that the patient has contravened a caregiver's order, such as, for example, instructions to remain in bed, or to walk to the bathroom only with the assistance of an attendant, a notification, alert, or alarm can be transmitted to the appropriate caregivers at block 1612.

[0195] If the patient monitoring system 100 determines that the patient has not contravened a caregiver's order, the system will return to block 1610 to detect and/or predict whether the patient has fallen.

[0196] FIGS. 13A-F illustrate embodiments of icon displays reflecting a patient's position according to an embodiment of the present disclosure. According to some embodiments, the graphical icons are used to visually depict the detected orientation of the patient. In particular, the icons of FIGS. 13A-F show, in stick figure-type format, the patient sitting, standing, and lying in the supine position (on the back), the prone position (on the belly), on the left side, and on the right side, respectively.

[0197] FIG. 14 illustrates an example of how the icons described with respect to FIGS. 13A-F can be presented on the display 120 of the patient monitor 106. Toward the bottom of the main display 120 are a set of 3 icons 1402, 1404, and 1406 indicating the patient's position. The left-most icon 1404 shows the patient lying on his right side. The two icons to the right of the left-most icon 1404 and 1406 show the patient lying on his back. According to certain embodiments, the display 120 of the patient monitor 106 can include a touchscreen interface. The touchscreen interface can enable finger controls, including a touch gesture, a touch and move gesture, and a flick gesture. Illustratively, a clinician may use the touch gesture on an icon 1406 to expand the icon in the display 120 to include additional information associated with that icon 1406. For example, additional information associated with the "touched" icon 1406 can include, the time at which the patient assumed the particular orientation, the time (if available) at which the patient moved from the orientation, the total duration of time the patient spent in the particular orientation, the number of discrete times that the patient has been in the particular orientation over a defined period (such as 24 hours), the total duration of time that the patient has been in the particular orientation over a defined period (such as 24 hours), and the like. The clinician may also use the flick finger gesture to scroll right and left, corresponding to moving forward and backward in time, to access the historical positional record of the patient.

[0198] The service life of the wireless sensor 102 disclosed herein can vary depending on, among other things, battery size, and data transmission characteristics such as data rate, frequency of transmission, and quantity of data transmitted. According to one embodiment, the wireless

sensor 102 is configured to operate continuously or near continuously (e.g., waking up every second or so to sense and transmit the patient's physiological data) for approximately two days, after which the wireless sensor 102 is to be disposed of properly. Other embodiments of the wireless sensor 102, equipped with a larger battery, for example, are configured to operate for longer periods of time before disposal. Some embodiments can be configured for sterilization and reuse.

[0199] Certain medical device manufacturers implement quality control measures for disposable medical devices, such as embodiments of the disclosed wireless sensor 102, to carefully control and manage the performance characteristics of their disposable devices. In particular, there is a risk that used and disposed-of wireless sensors 102 can be salvaged and refurbished or retrofitted for additional use beyond the defined and intended service life of the wireless sensor 102. Features can be included in the disclosed patient monitoring system 100 to help prevent improper use of the wireless sensor 102 beyond its defined service life.

[0200] According to one embodiment of the patient monitoring system 100, the wireless sensor 102 is configured to set an activation flag in the storage device 204 of the wireless sensor 102 upon initial activation, indicating that the wireless sensor 102 has been activated for use. In some embodiments, the activation flag is set in an information element 215 which is provided to store information about the usage of the wireless sensor 102 to help maintain quality control. Advantageously, the activation flag is set in non-volatile memory of the storage device 204, or in the information element 215, so that disconnection from the battery 214 will not disrupt or erase the set activation flag. Thus, if the wireless sensor 102 is reconditioned such that it may be activated a second time, the activation flag will indicate, through a standard sensor 102 start-up routine, that the sensor 102 has been previously activated. Upon detection of the activation flag, the wireless sensor 102 can transmit a prior activation message and/or alert which can serve as a warning notification that the quality of the sensor 102 may be compromised. The transmitted warning or alert can be received by, for example, a patient monitor 106 which can then provide a menu of actions that the user may take in response to the transmitted quality warning or alert. The menu of actions can include the option to shut down the wireless sensor 102. In certain situations it may be desirable to continue to use the wireless sensor 102. Illustratively, it is possible that the battery 214 connection to the wireless sensor 102 is established and then unintentionally disconnected. For example, a battery isolator 322 may be initially removed from the sensor 102 but then re-inserted so as to once again isolate the battery 214 from the electronic circuitry of the wireless sensor 102. Removing the battery isolator 322 a second time will result in transmission of a quality warning or alert as described above. In such a situation the user, being aware of the circumstances that led to the quality warning, may choose to continue to use the wireless sensor 102.

[0201] According to another embodiment, the wireless sensor 102 is configured to set a prolonged service flag, after the wireless sensor has been in an activated state for a predefined period of time, such as, for example, four hours. The prolonged service flag can serve to indicate upon start-up that the sensor 102 has previously been active for a prolonged duration of time. In another embodiment, the

wireless sensor **102** tracks and records on the storage device **204** the duration of time that the sensor **102** has been active. Advantageously, the sensor **102** can issue notifications and/or alerts to the user that the sensor **102** is nearing the end of service life, providing the user an opportunity to take steps to replace the wireless sensor **102** before it ceases to operate. Additionally, the recorded duration of time that the sensor **102** has been active can serve to detect when a sensor **102** has been refurbished to operate beyond its intended service life. The appropriate warning can then be transmitted to the user. According to some embodiments, once the wireless sensor has been active for a period of time equal to a maximum service life duration, the sensor **102** sets a flag in the storage device **204**, or otherwise configures itself to prohibit the sensor **102** from operating further.

[0202] In other embodiments, the wireless sensor **102** transmits to the patient monitor **106** a unique identifier such as, for example, a product serial number that is encoded in one of the hardware components of the wireless sensor **102**. Once the wireless sensor **102** is paired with a patient monitor or with an expander/repeater **107** and is operational, the patient monitor **106** or the expander/repeater **107** can transmit the sensor's **102** unique identifier to a central repository that lists the unique identifiers of sensors **102** known to have been operational. Illustratively, during the pairing operation, the patient monitor **106** or the expander/repeater **107** can check the central repository to determine whether the wireless sensor **102** that is attempting to pair has been listed on in the central repository, thereby indicating that the wireless sensor **102** might have quality issues.

[0203] In other various embodiments, the wireless sensor **102** includes a sensor information element **215**, which can be provided through an active circuit such as a transistor network, memory chip, EEPROM (electronically erasable programmable read-only memory), EPROM (erasable programmable read-only memory), or other identification device, such as multi-contact single wire memory devices or other devices, such as those commercially available from Dallas Semiconductor or the like. The sensor information element **215** may advantageously store some or all of a wide variety of information, including, for example, sensor type designation, sensor configuration, patient information, sensor characteristics, software such as scripts or executable code, algorithm upgrade information, software or firmware version information, or many other types of data. In a preferred embodiment, the sensor information element **215** may also store useful life data indicating whether some or all of the sensor components have expired.

[0204] Many other variations than those described herein will be apparent from this disclosure. For example, depending on the embodiment, certain acts, events, or functions of any of the algorithms described herein can be performed in a different sequence, can be added, merged, or left out altogether (e.g., not all described acts or events are necessary for the practice of the algorithms). Moreover, in certain embodiments, acts or events can be performed concurrently, e.g., through multi-threaded processing, interrupt processing, or multiple processors or processor cores or on other parallel architectures, rather than sequentially. In addition, different tasks or processes can be performed by different machines and/or computing systems that can function together.

[0205] The various illustrative logical blocks, modules, and algorithm steps described in connection with the

embodiments disclosed herein can be implemented as electronic hardware, computer software, or combinations of both. To clearly illustrate this interchangeability of hardware and software, various illustrative components, blocks, modules, and steps have been described above generally in terms of their functionality. Whether such functionality is implemented as hardware or software depends upon the particular application and design constraints imposed on the overall system. The described functionality can be implemented in varying ways for each particular application, but such implementation decisions should not be interpreted as causing a departure from the scope of the disclosure.

[0206] The various illustrative logical blocks and modules described in connection with the embodiments disclosed herein can be implemented or performed by a machine, such as a general purpose processor, a digital signal processor (DSP), an application specific integrated circuit (ASIC), a field programmable gate array (FPGA) or other programmable logic device, discrete gate or transistor logic, discrete hardware components, or any combination thereof designed to perform the functions described herein. A general purpose processor can be a microprocessor, but in the alternative, the processor can be a controller, microcontroller, or state machine, combinations of the same, or the like. A processor can include electrical circuitry configured to process computer-executable instructions. In another embodiment, a processor includes an FPGA or other programmable device that performs logic operations without processing computer-executable instructions. A processor can also be implemented as a combination of computing devices, e.g., a combination of a DSP and a microprocessor, a plurality of microprocessors, one or more microprocessors in conjunction with a DSP core, or any other such configuration. A computing environment can include any type of computer system, including, but not limited to, a computer system based on a microprocessor, a mainframe computer, a digital signal processor, a portable computing device, a device controller, or a computational engine within an appliance, to name a few.

[0207] The steps of a method, process, or algorithm described in connection with the embodiments disclosed herein can be embodied directly in hardware, in a software module stored in one or more memory devices and executed by one or more processors, or in a combination of the two. A software module can reside in RAM memory, flash memory, ROM memory, EPROM memory, EEPROM memory, registers, hard disk, a removable disk, a CD-ROM, or any other form of non-transitory computer-readable storage medium, media, or physical computer storage known in the art. An example storage medium can be coupled to the processor such that the processor can read information from, and write information to, the storage medium. In the alternative, the storage medium can be integral to the processor. The storage medium can be volatile or nonvolatile. The processor and the storage medium can reside in an ASIC.

[0208] Conditional language used herein, such as, among others, "can," "might," "may," "e.g.," and the like, unless specifically stated otherwise, or otherwise understood within the context as used, is generally intended to convey that certain embodiments include, while other embodiments do not include, certain features, elements and/or states. Thus, such conditional language is not generally intended to imply that features, elements and/or states are in any way required for one or more embodiments or that one or more embodi-

ments necessarily include logic for deciding, with or without author input or prompting, whether these features, elements and/or states are included or are to be performed in any particular embodiment. The terms “comprising,” “including,” “having,” and the like are synonymous and are used inclusively, in an open-ended fashion, and do not exclude additional elements, features, acts, operations, and so forth. Also, the term “or” is used in its inclusive sense (and not in its exclusive sense) so that when used, for example, to connect a list of elements, the term “or” means one, some, or all of the elements in the list. Further, the term “each,” as used herein, in addition to having its ordinary meaning, can mean any subset of a set of elements to which the term “each” is applied.

[0209] While the above detailed description has shown, described, and pointed out novel features as applied to various embodiments, it will be understood that various omissions, substitutions, and changes in the form and details of the systems, devices or methods illustrated can be made without departing from the spirit of the disclosure. As will be recognized, certain embodiments described herein can be embodied within a form that does not provide all of the features and benefits set forth herein, as some features can be used or practiced separately from others.

[0210] The term “and/or” herein has its broadest, least limiting meaning which is the disclosure includes A alone, B alone, both A and B together, or A or B alternatively, but does not require both A and B or require one of A or one of B. As used herein, the phrase “at least one of” A, B, “and” C should be construed to mean a logical A or B or C, using a non-exclusive logical or.

[0211] The apparatuses and methods described herein may be implemented by one or more computer programs executed by one or more processors. The computer programs include processor-executable instructions that are stored on a non-transitory tangible computer readable medium. The computer programs may also include stored data. Non-limiting examples of the non-transitory tangible computer readable medium are nonvolatile memory, magnetic storage, and optical storage.

[0212] Although the foregoing disclosure has been described in terms of certain preferred embodiments, other embodiments will be apparent to those of ordinary skill in the art from the disclosure herein. Additionally, other combinations, omissions, substitutions and modifications will be apparent to the skilled artisan in view of the disclosure herein. Accordingly, the present invention is not intended to be limited by the description of the preferred embodiments, but is to be defined by reference to claims.

What is claimed is:

1. A wireless physiological sensor for measuring acceleration of a patient, the physiological sensor comprising:

a base including a bottom surface and a top surface, said base also including a first aperture, a second aperture, and a third aperture, wherein each of said first, second, and third apertures extends between said bottom surface and said top surface of said base;

a substrate layer including conductive tracks and connection pads, a top side, and a bottom side, said bottom side of said substrate layer being disposed above said top surface of said base, said substrate layer also including a first through-hole via and a second through-hole via, wherein each of said first and second through-

hole vias extends through said substrate layer between said top and bottom sides of said substrate layer;

a temperature sensor responsive to thermal energy of said patient, said temperature sensor mounted on said top side of said substrate layer, said temperature sensor including a thermal contact in thermal communication with said top side of said substrate layer, wherein said first through-hole via is aligned with said thermal contact of said temperature sensor on said top side of said substrate layer and with said first aperture of said base on said bottom side of said substrate layer, and wherein said first aperture of said base and said first through-hole via of said substrate layer are filled with at least a thermally conductive material to cause said temperature sensor to be in thermal communication with a portion of said bottom surface of said base corresponding to said first aperture;

an ECG sensor mounted on said top side of said substrate layer, said ECG sensor responsive to electrical signals generated by said patient's heart, said ECG sensor including an extendible lead with an electrode responsive to said electrical signals, said ECG sensor also including an electrical contact in electrical communication with said top side of said substrate layer, wherein said second through-hole via is aligned with said electrical contact of said ECG sensor on said top side of said substrate layer and with said second aperture of said base on said bottom side of said substrate layer, and wherein said second aperture of said base and said second through-hole via of said substrate layer are filled with at least an electrically conductive material to cause said ECG sensor to be in electrical communication with a portion of said bottom surface of said base corresponding to said second aperture;

an accelerometer, mounted on said substrate layer, said accelerometer responsive to a linear acceleration of said patient; and

an acoustic respiration sensor responsive to vibrational motion generated by said patient, said acoustic respiration sensor being disposed on said bottom side of said substrate layer and extending through said third aperture in said base and beyond said bottom surface of said base, said acoustic respiration sensor being in structural communication with said substrate layer so as to mechanically transmit vibrational motion to said accelerometer.

2. The physiological sensor of claim 1, further comprising an information element configured to store information indicative of whether said physiological sensor has been previously activated.

3. The physiological sensor of claim 1, further comprising a gyroscope, mounted on said substrate layer, said gyroscope responsive to an angular velocity of said patient.

4. The physiological sensor of claim 1, wherein said base insulates a portion of said patient's body surrounding said portion of said bottom surface of said base corresponding to said first aperture.

5. The physiological sensor of claim 1, further comprising a wireless transceiver configured to wirelessly transmit information representative of said thermal energy, said electrical signals, said linear acceleration, and said vibrational motion.

6. The physiological sensor of claim 5, wherein said wireless transceiver is configured to transmit a pairing signal.

7. The physiological sensor of claim 5, wherein said wireless transceiver is configured to transmit a message indicating that said physiological sensor has been previously activated.

8. The physiological sensor of claim 5, wherein said wireless transceiver is configured to transmit a notification that a quality standard associated with said physiological sensor is compromised.

9. The physiological sensor of claim 1, further comprising:

a battery, mounted on said bottom side of said substrate layer and between said bottom side of said substrate layer and said top surface of said base, said battery being in electrical contact with said substrate layer, wherein said battery forms a recess between a portion of said bottom side of said substrate layer and said top surface of said base; and

a mounting frame, disposed to fill said formed recess, said mounting frame configured to provide rigid structural support between said base and said substrate layer.

10. The physiological sensor of claim 9, wherein said mounting frame further comprises:

a first mounting frame aperture aligned with said first through-hole via and with said first aperture of said base, wherein said first mounting aperture is at least filled with said thermally conductive material to cause said temperature sensor to be in thermal communication with said portion of said bottom surface of said base corresponding to said first aperture; and

a second mounting frame aperture aligned with said second through-hole via and with said second aperture of said base, wherein said second mounting aperture is at least filled with said electrically conductive material to cause said ECG sensor to be in electrical communication with said portion of said bottom surface of said base corresponding to said second aperture.

11. The physiological sensor of claim 1, further comprising:

a gyroscope, mounted on said substrate layer, said gyroscope responsive to an angular velocity of said patient;

a magnetometer, mounted on said substrate layer, said magnetometer responsive to a magnetic field;

a processor, mounted on said substrate layer and in communication with said temperature sensor, ECG sensor, accelerometer, gyroscope, and magnetometer, said processor configured to generate signals representative of said thermal energy, electrical signals, linear acceleration, vibratory motion, angular velocity, and magnetic field; and

a wireless transceiver, mounted on said substrate layer and in communication with said processor, said wireless transceiver configured to transmit said generated signals representative of said thermal energy, electrical signals, linear acceleration, vibrational motion, angular velocity and magnetic field.

12. The physiological sensor of claim 11, further comprising:

an impedance sensor, mounted on said substrate layer and in electrical communication with said portion of said bottom surface of said base corresponding to said second aperture.

13. The physiological sensor of claim 11, wherein said accelerometer is a three-dimensional accelerometer and said gyroscope is a three-dimensional gyroscope.

14. A wearable wireless sensor for monitoring at least one of pressure ulcer risk, fall detection, or fall risk, said physiological sensor comprising:

a base including a first aperture;

a circuit layer including a first through-hole via extending through said circuit layer; and

a temperature sensor responsive to a thermal energy of a patient, said temperature sensor mounted on said circuit layer, said temperature sensor including a thermal contact in thermal communication with said circuit layer,

wherein said first through-hole via is aligned with said thermal contact of said temperature sensor and with said first aperture of said base, and

wherein said first aperture and said first through-hole via include a thermally conductive material to cause said temperature sensor to be in thermal communication with a portion of said base corresponding to said first aperture.

15. The sensor of claim 14, wherein said base insulates a portion of said patient's body surrounding said portion of said base corresponding to said first aperture.

16. The sensor of claim 14, further comprising:

a second aperture in said base;

a second through-hole via extending through said circuit layer between said top side and bottom side of said circuit layer;

an ECG sensor mounted on said circuit layer, said ECG sensor responsive to electrical signals, said ECG sensor including an extendible lead with an electrode responsive to said electrical signals, said ECG lead also including an electrical contact in electrical communication with said circuit layer,

wherein said second through-hole via is aligned with said electrical contact of said ECG sensor on said circuit layer and with said second aperture of said base, and wherein said second aperture of said base and said second through-hole via of said circuit layer include an electrically conductive material, said ECG sensor in electrical communication with a portion of said base corresponding to said second aperture through said conductive material.

17. The sensor of claim 14, further comprising:

an accelerometer, mounted on said circuit layer, said accelerometer responsive to a linear acceleration of said patient;

a third aperture in said base; and

an acoustic respiration sensor responsive to vibrational motion of said patient, said acoustic respiration sensor being disposed on said circuit layer and extending through said third aperture in said base, wherein said acoustic respiration sensor is in rigid structural communication with said circuit layer so as to mechanically transmit sensed vibrational motion to said accelerometer.

18. The sensor of claim 14, further comprising a gyroscope mounted on said circuit layer, said gyroscope responsive to an angular velocity of said patient.

19. The sensor of claim 18, wherein said accelerometer comprises a three-dimensional accelerometer and said gyroscope comprises a three-dimensional gyroscope.

20. The sensor of claim 19, further comprising an information element configured to store information indicative of whether said physiological sensor has been previously activated.

* * * * *

专利名称(译)	耐用的无线生理传感器		
公开(公告)号	US20170055851A1	公开(公告)日	2017-03-02
申请号	US15/253536	申请日	2016-08-31
[标]申请(专利权)人(译)	梅西莫股份有限公司		
申请(专利权)人(译)	Masimo公司		
当前申请(专利权)人(译)	Masimo公司		
[标]发明人	AL ALI AMMAR		
发明人	AL-ALI, AMMAR		
IPC分类号	A61B5/0205 A61B5/11 A61B5/1455 A61B5/00 A61B5/05 A61B5/053 A61B5/0408 A61B5/113		
CPC分类号	A61B5/02055 A61B5/0408 A61B5/1116 A61B5/1117 A61B5/113 A61B5/746 A61B5/05 A61B5/053 A61B5/447 A61B5/743 A61B5/14552 A61B5/0022 A61B5/002 A61B5/1113 A61B5/1118 A61B5/6801 A61B5/7275 A61B2562/0219 A61G7/057 G16H50/30 A61B5/0004 A61B5/0015 A61B5/01 A61B5/0205 A61B5/0402 A61B5/0816 A61B5/1121 A61B5/1126 A61B5/14551 A61B5/6833 A61B5/7264 A61B5/7282 A61B5/742 A61B2560/0475 A61B2562/0204 A61B2562/0223 A61B2562/0271 A61B2562/029 A61G2203/32 A61G2203/36 A61G2203/42 A61G2203/46		
优先权	62/212467 2015-08-31 US 62/212472 2015-08-31 US 62/212484 2015-08-31 US 62/212480 2015-08-31 US		
其他公开文献	US10226187		
外部链接	Espacenet USPTO		

摘要(译)

公开了一种无线的，患者佩戴的生理传感器，其被配置为尤其帮助管理处于形成一个或多个压疮的危险中的患者。根据实施例，传感器包括具有顶表面和底表面的基部。传感器还包括包括导电轨道和连接垫的衬底层，顶侧和底侧，其中衬底层的底侧布置在基底的顶侧上方。安装在基板层上的是处理器，数据存储设备，无线收发器，加速度计和电池。在使用中，传感器感测患者的运动，并将指示感测的运作的信息无线地传送到例如患者监视器。患者监视器接收，存储和处理所发送的信息。

