



US 20150080699A1


(19) **United States**(12) **Patent Application Publication**
Kaib et al.(10) **Pub. No.: US 2015/0080699 A1**(43) **Pub. Date: Mar. 19, 2015**(54) **METHOD OF DETECTING SIGNAL
CLIPPING IN A WEARABLE AMBULATORY
MEDICAL DEVICE****Publication Classification**

(51) **Int. Cl.**
A61B 5/04 (2006.01)
A61B 5/00 (2006.01)
A61B 5/0408 (2006.01)

(52) **U.S. Cl.**
CPC *A61B 5/04014* (2013.01); *A61B 5/04085*
(2013.01); *A61B 5/6831* (2013.01); *A61B*
5/4836 (2013.01)
USPC 600/393

(71) Applicant: **ZOLL MEDICAL CORPORATION,**
Chelmsford, MA (US)(72) Inventors: **Thomas E. Kaib**, North Huntingdon, PA
(US); **Shane S. Volpe**, Saltsburg, PA
(US); **John D. Macho**, Farmington, PA
(US)(21) Appl. No.: **14/451,046**(22) Filed: **Aug. 4, 2014****Related U.S. Application Data**(60) Continuation of application No. 14/064,403, filed on
Oct. 28, 2013, now Pat. No. 8,798,729, which is a
division of application No. 13/428,891, filed on Mar.
23, 2012, now Pat. No. 8,600,486.(60) Provisional application No. 61/467,532, filed on Mar.
25, 2011.(57) **ABSTRACT**

A wearable medical device and method of detecting clipping of ECG signals is disclosed. In one embodiment, the wearable medical device comprises a plurality of ECG sensing electrodes configured to sense an ECG of a patient and an ECG acquisition circuit electrically coupled to a pair of the plurality of ECG sensing electrodes and configured to provide an amplified and conditioned analog ECG signal, a programmable attenuation/gain stage electrically coupled between a first gain stage and a second gain stage, an ADC electrically coupled to the ECG acquisition circuit to receive and digitize the amplified and conditioned analog ECG signal and provide a digitized ECG signal, and a signal conditioning to and control unit electrically coupled to the ECG acquisition circuit and the ADC to receive and monitor the digitized ECG signal and to detect clipping of the amplified and conditioned analog ECG signal based upon the digitized ECG signal.

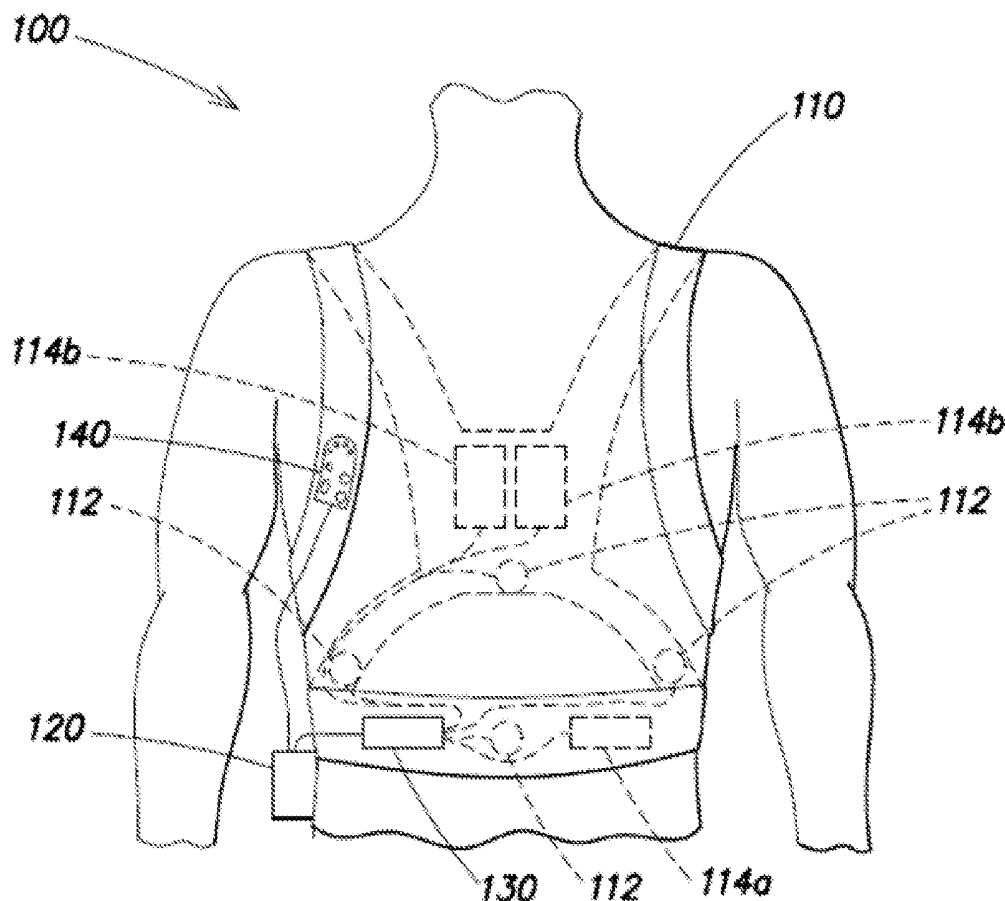

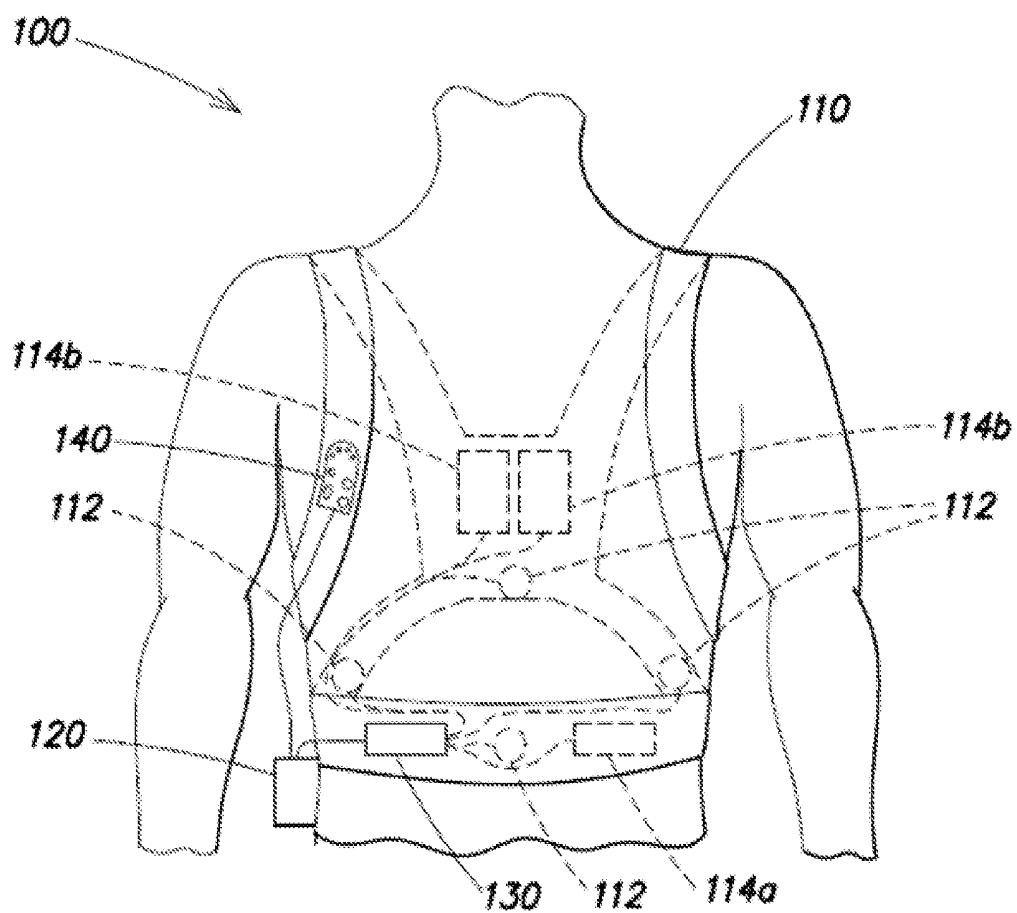


FIG. 1

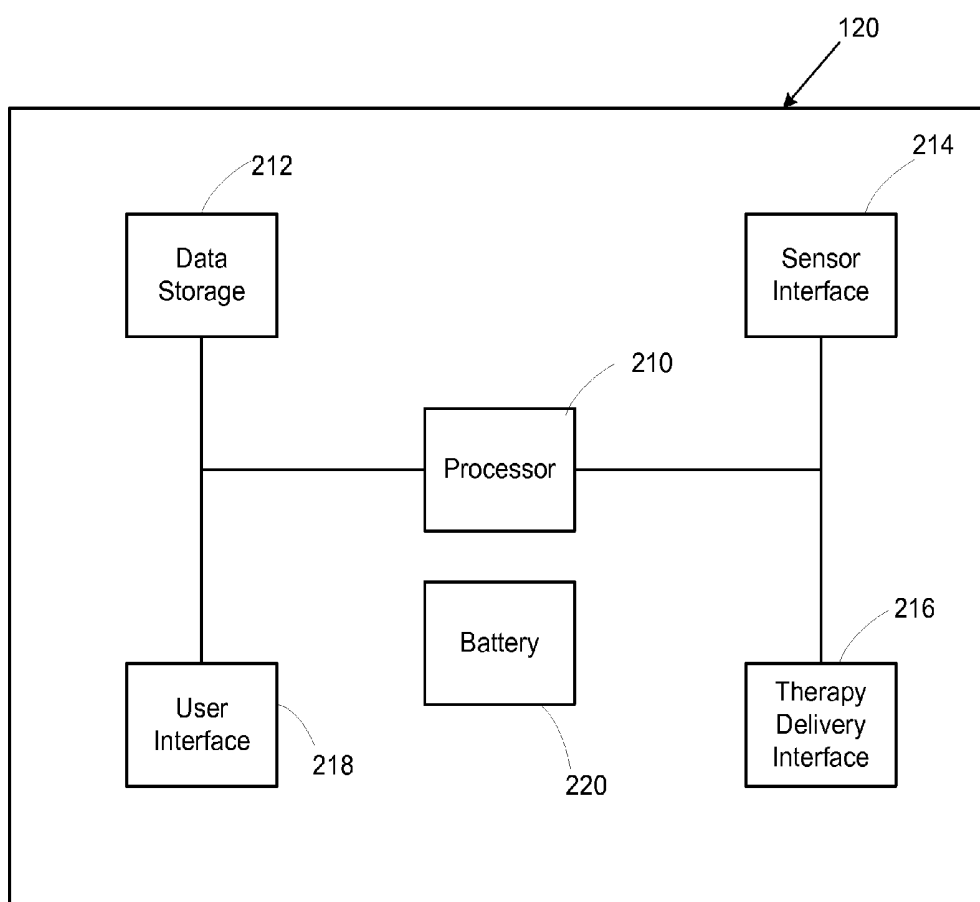


FIG. 2

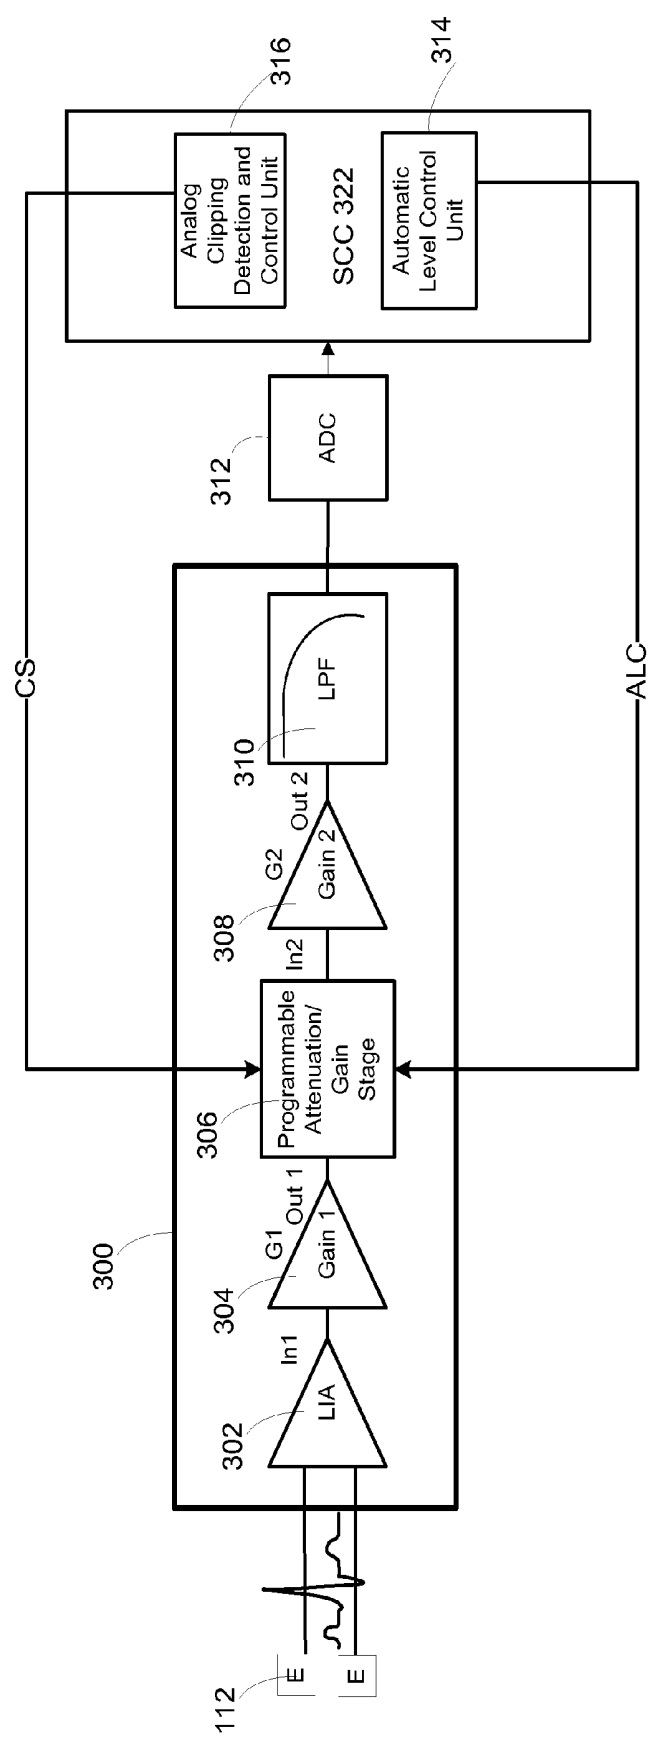


FIG. 3

METHOD OF DETECTING SIGNAL CLIPPING IN A WEARABLE AMBULATORY MEDICAL DEVICE

RELATED APPLICATIONS

[0001] This application is a continuation of U.S. patent application Ser. No. 14/064,403, titled "METHOD OF DETECTING SIGNAL CLIPPING IN A WEARABLE AMBULATORY MEDICAL DEVICE," filed Oct. 28, 2013, which is a division of U.S. patent application Ser. No. 13/428,891, titled "METHOD OF DETECTING SIGNAL CLIPPING IN A WEARABLE AMBULATORY MEDICAL DEVICE," filed Mar. 23, 2012, which claims priority under 35 U.S.C. § 119(e) to U.S. Provisional Application Ser. No. 61/467,532, titled "METHOD OF DETECTING SIGNAL CLIPPING IN A WEARABLE AMBULATORY MEDICAL DEVICE," filed on Mar. 25, 2011, each of which is hereby incorporated herein by reference in its entirety.

BACKGROUND

[0002] 1. Field of the Invention

[0003] The present invention is generally directed to the processing of electrical signals, and more particularly to the processing of ECG signals and the treatment of cardiac conditions in an ambulatory medical device, such as a wearable defibrillator.

[0004] 2. Discussion of the Related Art

[0005] To protect against cardiac arrest and other cardiac health ailments, some at-risk patients may use a wearable defibrillator, such as the LifeVest® wearable cardioverter defibrillator available from ZOLL Medical Corporation of Chelmsford, Mass. To remain protected, the patient wears the device nearly continuously while going about their normal daily activities.

[0006] With an ambulatory medical device, such as a wearable defibrillator, the patient's electrocardiogram (ECG) signal is obtained from body surface electrodes. When the ECG signal is obtained in this manner, electrical noise frequently degrades the quality of the ECG signal. The challenge becomes one of extracting a clean ECG signal from the sometimes noisy signals derived from the body-surface electrodes. A typical ECG measurement system includes a signal acquisition circuit (also called an analog front end (AFE)) that amplifies the ECG signals gathered by the electrodes, an analog-to-digital converter (ADC) that digitizes the amplified ECG signals and a processor that analyzes the ECG signals and controls the ambulatory medical device based on the processed ECG signals.

[0007] The ECG signals provided by the electrodes are typically about 80 microvolts to about 2 millivolts in signal amplitude. The typical signal acquisition circuit amplifies the ECG signals received from the body surface electrodes by about 500 to 1000 times before providing the amplified ECG signal to the ADC to digitize the ECG signal. Unfortunately, any to amplification of the ECG signal also amplifies any noise present in the ECG signal. To maximize the signal-to-noise ratio and reduce noise in the system, the amplification of the ECG signal is completed in multiple stages. These multiple stages typically include one or more amplifier or gain stages and a controlled or programmable attenuation stage. However, these multiple amplifier stages can make the system susceptible to analog and/or digital signal clipping. As defined herein, clipping is a form of signal distortion that cuts

off or "clips" the signal once the gain of the amplifier exceeds a certain threshold or when the ADC is at its minimum or maximum voltage range. Typically, the threshold above which analog clipping occurs is the maximum output level of the amplifier.

[0008] Consequences of analog clipping can include distorted ECG signals presented to the ADC input. In addition, once analog clipping starts to occur, the ECG signal being processed by the signal acquisition circuit will no longer respond to the control signals sent by the system and can cause the signal acquisition system to malfunction.

SUMMARY

[0009] At least one aspect is directed to a wearable medical device. The wearable medical device comprises a plurality of ECG sensing electrodes configured to sense an ECG of a patient and an ECG acquisition circuit electrically coupled to a pair of the plurality of ECG sensing electrodes and configured to provide an amplified and conditioned analog ECG signal. The ECG acquisition circuit including a programmable attenuation/gain stage electrically coupled between a first gain stage and a second gain stage. The wearable medical device also includes an analog to digital converter electrically coupled to the ECG acquisition circuit to receive and digitize the amplified and conditioned analog ECG signal and provide a digitized ECG signal. The wearable medical device further includes a signal conditioning and control unit electrically coupled to the ECG acquisition circuit and the analog to digital converter to receive and monitor the digitized ECG signal and to detect clipping of the amplified and conditioned analog ECG signal based upon the digitized ECG signal.

[0010] In some embodiments, the signal conditioning and control unit includes an automatic level control unit electrically coupled to the programmable attenuation/gain stage, and configured to vary an amount of attenuation/gain provided by the programmable to attenuation/gain stage based on the digitized ECG signal.

[0011] In one embodiment, the automatic level control unit is configured to determine whether a voltage level of the digitized ECG signal is above a threshold level and configured to increase the amount of attenuation provided by the programmable attenuation/gain stage. The automatic level control unit can be configured to determine whether a voltage level of the digitized ECG signal is below a threshold level and configured to decrease the amount of attenuation provided by the programmable attenuation/gain stage.

[0012] In another embodiment, the signal conditioning and control unit includes an analog clipping detection and control unit electrically coupled to the programmable attenuation/gain stage, and configured to determine whether a voltage level is approaching a clipping threshold. The analog clipping detection and control unit can be configured to determine the voltage level before programmable attenuation/gain stage. The amplified and conditioned analog ECG signal can be marked as compromised in response to a determination that the voltage level is approaching the clipping threshold before the programmable attenuation/gain stage.

[0013] In some embodiments, the analog clipping detection and control unit is configured to determine the voltage level after the programmable attenuation/gain stage. The analog clipping detection and control unit can attenuate the amplified and conditioned analog ECG signal in response to a determination that the voltage level is approaching the clipping threshold after the programmable attenuation/gain stage. The

clipping threshold can be determined based on a voltage range of an ECG of a human patient, a maximum output voltage level and a current gain setting of at least one of the first gain, the programmable attenuation/gain stage and the second gain stage.

[0014] The wearable medical device can include a low noise instrumentation amplifier electrically coupled to the pair of the plurality of ECG sensing electrodes and the first gain stage. The wearable medical device can also include a low pass filter electrically coupled to at least one of the second gain stage and the analog to digital converter.

[0015] At least one aspect is directed to a method of detecting clipping of ECG signals in a wearable medical device. The method comprises acts of sensing an ECG signal of a patient using ECG sensing electrodes and amplifying the sensed ECG signal using a first gain stage. The method also includes an act of conditioning the amplified ECG signal from the first gain stage using a programmable attenuation/gain stage and amplifying the conditioned ECG signal from the programmable attenuation/gain stage using a second gain stage. The method further includes an act of receiving and digitizing the amplified and conditioned analog ECG signal to provide a digitized ECG signal and monitoring the digitized ECG signal to detect clipping of the amplified and conditioned analog ECG signal based upon the digitized ECG signal.

[0016] The method further includes an act of varying an amount of attenuation applied by the programmable attenuation/gain stage based on the digitized ECG signal. The act of varying the amount may include an act of determining whether a voltage level of the digitized ECG signal is above a threshold level and increasing the amount of attenuation applied by the programmable attenuation/gain stage.

[0017] In one embodiment, the act of varying the amount includes the acts of determining whether a voltage level of the digitized ECG signal is below a threshold level and decreasing the amount of attenuation applied by the programmable attenuation/gain stage. In some embodiments, the act of varying the amount includes the acts of determining whether a voltage level is approaching a clipping threshold. In one embodiment, method further includes determining the clipping threshold based on a voltage range of an ECG of a human patient, a current gain setting and a maximum output voltage level of at least one of the first gain stage, the programmable attenuation/gain stage and the second gain stage.

[0018] In some embodiments, the act of determining includes the act of marking the amplified and conditioned analog ECG signal as compromised in response to a determination that the voltage level is approaching the clipping threshold before programmable attenuation/gain stage. The act of determining can include the act of attenuating the amplified and conditioned analog ECG signal in response to a determination that the voltage level is approaching the clipping threshold after the programmable attenuation/gain stage. Still other aspects, embodiments, and advantages of these exemplary aspects and embodiments, are discussed in detail below. Any embodiment disclosed herein may be combined with any other embodiment in any manner consistent with at least one of the objects, aims, and needs disclosed herein, and references to "an embodiment," "some embodiments," "an alternate embodiment," "various embodiments," "one embodiment" or the like are not to necessarily mutually exclusive and are intended to indicate that a particular feature, structure, or characteristic described in connection with the

embodiment may be included in at least one embodiment. The appearances of such terms herein are not necessarily all referring to the same embodiment. The accompanying drawings are included to provide illustration and a further understanding of the various aspects and embodiments, and are incorporated in and constitute a part of this specification. The drawings, together with the remainder of the specification, serve to explain principles and operations of the described and claimed aspects and embodiments.

BRIEF DESCRIPTION OF THE DRAWINGS

[0019] The accompanying drawings are not intended to be drawn to scale. In the drawings, each identical or nearly identical component that is illustrated in various figures is represented by a like numeral. For purposes of clarity, not every component may be labeled in every drawing. In the drawings:

[0020] FIG. 1 illustrates a wearable medical device, such as a wearable defibrillator, in accordance with an embodiment of the present invention;

[0021] FIG. 2 is a functional block diagram of a control unit that may be used with embodiments of present invention; and

[0022] FIG. 3 illustrates a functional block diagram of a signal acquisition circuit to detect and control analog clipping for use with a wearable medical device in accordance with an embodiment of the present invention.

DETAILED DESCRIPTION

[0023] Applicant has appreciated that because any amount of clipping can distort the quality of the ECG signal, it would be desirable to detect such clipping, and where possible, to mitigate it. It would also be desirable to have the ECG signal detected by the analog signal acquisition circuit to be free of clipping distortions before that ECG signal passes to the analog-to-digital converter (ADC). Distortion of the ECG signal in the signal acquisition circuit can result in any processing that is based upon that distorted ECG signal being unreliable. For example, in a wearable defibrillator, the distortion of the ECG signal due to clipping may result in a false to positive detection of arrhythmia, or worse, the failure to detect an arrhythmia. A false positive detection of arrhythmia can result in the wearable defibrillator initiating a treatment sequence, which if not terminated by the patient, could deliver an unnecessary shock to the patient. The amplification of noise present in the ECG signal may also overdrive the signal acquisition circuitry, resulting in a near zero output, causing the system to falsely detect a state of no cardiac electrical activity (asystole). Conversely, a failure to detect an actual arrhythmia can result in a failure to initiate a treatment sequence and result in serious risk for the patient.

[0024] Accordingly, a system and method is described herein that can detect whether clipping of the ECG signal has occurred at any of the amplification or gain stages of a signal acquisition circuit. The system and method are able to either correct the ECG signal, to warn a control unit of the unreliability of the ECG signal, or both.

[0025] This invention is not limited in its application to the details of construction and the arrangement of components set forth in the following description or illustrated in the drawings. The invention is capable of other embodiments and of being practiced or of being carried out in various ways. Also, the phraseology and terminology used herein is for the purpose of description and should not be regarded as limiting.

The use of “including,” “comprising,” “having,” “containing,” “involving,” and variations thereof herein is meant to encompass the items listed thereafter and equivalents thereof as well as additional items.

[0026] Moreover, it is to be understood that both the foregoing information and the following detailed description are merely illustrative examples of various aspects and embodiments of the present invention, and are intended to provide an overview or framework for understanding the nature and character of the claimed aspects and embodiments. Any embodiment disclosed herein may be combined with any other embodiment in any manner consistent with at least one of the aspects disclosed herein, and references to “an embodiment,” “some embodiments,” “an alternate embodiment,” “various embodiments,” “one embodiment,” “at least one embodiment,” “this and other embodiments” or the like are not necessarily mutually exclusive and are intended to indicate that a particular feature, structure, or characteristic described in connection with the embodiment may be included in at least one embodiment. The appearance of such terms herein is not necessarily all referring to the same embodiment.

[0027] Embodiments of the present invention are directed to an electrode system that may be used in a wearable medical device, such as that described in U.S. Pat. No. 5,944,669 (hereinafter “the ‘669 patent”), which is incorporated herein by reference in its entirety, to monitor cardiac function, to initiate treatment of a detected cardiac condition, or both. The ‘669 patent describes a method and apparatus for sensing cardiac function in a patient that may be used to initiate treatment of a detected cardiac condition. ECG sensing electrodes are used to obtain ECG signals from the heart of the patient and those ECG signals are analyzed using various techniques to provide information indicative of the operation of the patient’s heart, and whether a treatable cardiac condition is present for which treatment should be initiated. In accordance with an aspect of the present invention, the signals received from the pairs of ECG sensing electrodes described in the ‘669 patent may be processed in a manner described in detail below so that the presence of ECG signal clipping is identified and/or corrected thereby improving reliability in detection of the ECG signals and any further processing of those ECG signals.

[0028] As described in more detail below, although embodiments of the present invention are primarily described in terms of detecting analog clipping and controlling analog clipping of ECG sensor signals, it should be appreciated that the techniques described herein may readily be extended for use with other types of signals, from sensors other than ECG sensing electrodes. For example, aspects of the present invention may be used wherever multiple gain stages are used to amplify signals from other types of sensors, such as activity sensors, multiple axis accelerometers, pulse oxygen sensors, temperature sensors, respiratory rate sensors, thoracic impedance sensors, blood pressure sensors, acoustic sensors, etc.

[0029] FIG. 1 illustrates a wearable medical device, such as a LifeVest® Wearable Cardioverter Defibrillator available from ZOLL Medical Corporation of Chelmsford, Mass. in which various aspects of the present invention may be incorporated. As shown, the wearable medical device 100 includes a harness 110 having a pair of shoulder straps and a belt that is worn about the torso of a patient. The harness 110 is typically made from a material, such as cotton, that is breathable, and unlikely to cause skin irritation, even when worn for

prolonged periods of time. The wearable medical device 100 includes a plurality of ECG sensing electrodes 112 that are attached to the harness 110 at various positions about the patient’s body and electrically coupled to a control unit 120 via a connection pod 130. The plurality of ECG sensing electrodes 112, which may be dry-sensing capacitance electrodes, are used by the control unit 120 to monitor the cardiac function of the patient and generally include a front/back pair of ECG sensing electrodes and a side/side pair of ECG sensing electrodes. It should be appreciated that additional ECG sensing electrodes may be provided, and the plurality of ECG sensing electrodes 112 may be disposed at varying locations about the patient’s body.

[0030] The wearable medical device 100 also includes a plurality of therapy electrodes 114 that are electrically coupled to the control unit 120 via the connection pod 130 and which are capable of delivering one or more therapeutic defibrillating shocks to the body of the patient, if it is determined that such treatment is warranted. As shown, the plurality of therapy electrodes 114 includes a first therapy electrode 114a that is disposed on the front of the patient’s torso and a second therapy electrode 114b that is disposed on the back of the patient’s torso. The second therapy electrode 114b includes a pair of therapy electrodes that are electrically coupled together and act as the second therapy electrode 114b. The use of two therapy electrodes 114a, 114b permits a biphasic shock to be delivered to the body of the patient, such that a first of the two therapy electrodes can deliver a first phase of the biphasic shock with the other therapy electrode acting as a return, and the other therapy electrode can deliver the second phase of the biphasic shock with the first therapy electrode acting as the return.

[0031] The connection pod 130 electrically couples the plurality of ECG sensing electrodes 112 and the plurality of therapy electrodes 114 to the control unit 120, and may include electronic circuitry. For example, in one implementation, the connection pod 130 includes signal acquisition circuitry, such as a plurality of differential amplifiers to receive ECG signals from different ones of the plurality of ECG sensing electrodes 112 and to provide a differential ECG signal to the control unit 120 based on the difference therebetween. The connection pod 130 may also include other electronic circuitry, such as a motion sensor or accelerometer by which patient activity may be monitored.

[0032] As shown in FIG. 1, the wearable medical device 100 may also include a user interface pod 140 that is electrically coupled to the control unit 120. The user interface pod 140 can be attached to the patient’s clothing or to the harness 110, for example, via a clip (not shown) that is attached to a portion of the interface pod 140. Alternatively, the user interface pod 140 may simply be held in a person’s hand. The user interface pod 140 typically includes a number of buttons by which the patient, or a bystander can communicate with the control unit 120, and a speaker by which the control unit 120 may communicate with the patient or the bystander. In certain models of the LifeVest® Wearable Cardioverter Defibrillator, the functionality of the user interface pod 140 is incorporated into the control unit 120.

[0033] Where the control unit 120 determines that the patient is experiencing arrhythmia, the control unit 120 may issue an audible alarm via a loudspeaker (not shown) on the control unit 120 and/or the user interface pod 140 alerting the patient and any bystanders to the patient’s medical condition. The control unit 120 may also instruct the patient to press and

hold one or more buttons on the control unit **120** or on the user interface pod **140** to indicate that the patient is conscious, thereby instructing the control unit **120** to withhold the delivery of one or more therapeutic defibrillating shocks. If the patient does not respond, the device may presume that the patient is unconscious, and proceed with the treatment sequence, culminating in the delivery of one or more defibrillating shocks to the body of the patient.

[0034] FIG. 2 functionally illustrates a control unit, such as the control unit **120** depicted in FIG. 1 that may be used by a portable medical device, such as a wearable defibrillator, in accordance with the present invention. As shown, the control unit **120** includes at least one processor **210**, a battery **220**, data storage **212**, a sensor interface **214**, a therapy delivery interface **216**, and a user interface **218**. The battery **220** may be any type of battery capable of providing electrical power to the other device components, and in one implementation includes a rechargeable three cell 2200 mAh lithium ion battery pack that provides electrical power to the other device components. The data storage **212**, the sensor interface **214**, the therapy delivery interface **216**, and the user interface **218** are coupled to the at least one processor **210**. The data storage **212** includes a computer readable and writeable data storage medium configured to store non-transitory instructions and other data, and can include both nonvolatile storage media, such as optical or magnetic disk, ROM or flash memory, as well as volatile memory, such as RAM. The instructions may include executable programs or other code that can be executed by the at least one processor **210** to perform any of the functions described here below.

[0035] The at least one processor **210** may be any type of processor, microprocessor, or to controller, such as a microprocessor commercially available from such companies such as Texas Instruments, Intel, AMD, Sun, IBM, Motorola, Freescale, ARM Holdings, etc. In one implementation, the at least one processor **210** includes a power conserving processor arrangement that comprises a general purpose processor, such as an Intel® PXA270 processor and a special purpose processor, such as a Freescale DSP56311 Digital Signal Processor. Such a power conserving processor arrangement is described in co-pending application Ser. No. 12/833,096, titled SYSTEM AND METHOD FOR CONSERVING POWER IN A MEDICAL DEVICE, filed Jul. 9, 2010 (hereinafter the “096 application”) which is incorporated by reference herein in its entirety. The at least one processor of the control unit **120** is configured to monitor the patient’s medical condition, to perform medical data logging and storage, and to provide medical treatment to the patient in response to a detected medical condition, such as cardiac arrhythmia.

[0036] The therapy delivery interface **216** couples one or more therapy delivery devices, such as defibrillator therapy electrodes **114**, to the at least one processor **210**. The user interface **218** includes a combination of hardware and software components that allow the control unit **120** to communicate with an external entity, such as a user. These components are configured to receive information from actions such as physical movement or verbal intonation. In addition, the components of the user interface **218** can provide information to external entities, for example, in a manner such as described in U.S. Pat. No. 6,681,003, which is incorporated herein by reference. Examples of the components that may be employed within the user interface **218** include keyboards, mouse devices, trackballs, microphones, electrodes, touch screens, printing devices, display screens and speakers.

[0037] The sensor interface **214** couples the at least one processor **210** to a plurality of physiological sensors, such as the plurality of ECG sensing electrodes **112**. In some embodiments, the sensor interface **214** may also couple the at least one processor **210** to other physiological sensors, such as activity sensors, pulse oxygen sensors, temperature sensors, respiratory rate sensors, thoracic impedance sensors, blood pressure sensors, acoustic sensors, etc. The sensor interface **214** can include a signal acquisition circuit, such as the signal acquisition circuit shown in FIG. 3 and described further in detail below. The signal acquisition circuit conditions or adjusts the ECG signals before providing the signals to the at least one processor **210**.

[0038] FIG. 3 illustrates a signal acquisition circuit **300** that may be used with a plurality of ECG sensors in accordance with an aspect of the present invention to condition or adjust the ECG signal. Although only a single signal acquisition circuit **300** is depicted in FIG. 3, it should be appreciated that in a typical implementation, multiple signal acquisition circuits **300** would be provided for each pair of ECG sensing electrodes **112**. As shown, the signal acquisition circuit **300** includes a low noise instrumentation amplifier (LIA) **302**, a first gain stage **304**, a programmable attenuation/gain stage **306**, a second gain stage **308**, and a low pass filter (LPF) **310**. The signal acquisition circuit **300** is electrically coupled to an analog to digital converter **312** (ADC) that provides a digitized ECG signal to the at least one processor **210** (FIG. 2). The digitized ECG signal is also provided to a signal conditioning and control unit (SCC) **322** that is responsible for monitoring and controlling the ECG signal at various stages of the signal acquisition circuit. The SCC **322** includes an automatic level control unit (ALC) **314** and an analog clipping detection and control unit (ACDC) **316**. In accordance with one embodiment, the SCC unit **322** is capable of controlling the ECG signal at each stage of the signal acquisition circuit, as described further below. The SCC unit **322** may be implemented as a series of instructions that are performed by the at least one processor **210** or as a dedicated logic circuit.

[0039] In one embodiment, the signals from each of the plurality of ECG sensing electrodes **112** are provided to a respective input of the LIA **302** of the signal acquisition circuit **300**. Although not depicted in FIG. 3, each of the plurality of ECG sensing electrodes **112** may be electrically coupled to a respective buffer amplifier, with the output of each respective buffer amplifier being electrically coupled to a respective input of the LIA **302**. The inclusion of such a buffer amplifier, which may have unity gain, provides a very high impedance input to each respective output of an ECG sensing electrode. The LIA **302** is a differential amplifier that obtains the difference between the signals received on each respective input of the LIA **302**, which typically, are 180 degrees out of phase with one another. The LIA **302** automatically cancels out the common mode noise from the incoming ECG signal. The LIA **302** may be selected for additional desirable characteristics such as low DC offset, low drift, low noise, and to high common-mode rejection ratio. In some embodiments, the LIA **302** may also provide some amount of gain, which in one embodiment, may be approximately five times the input.

[0040] In one embodiment, the LIA **302** is electrically coupled to the first gain stage **304** that further amplifies the ECG signal. The first gain stage **304** may be a single amplifier or a series of amplifiers. The first gain stage **304** multiplies the input voltage level obtained from the LIA **302** by a predeter-

mined amount of gain, G1. In one embodiment, the first gain stage provides a gain of approximately 28 times the input.

[0041] The first gain stage 304 is electrically coupled to the programmable attenuation/gain stage 306 that applies a varying amount of attenuation to the ECG signal based on a control signal from the ALC 314. The programmable attenuation/gain stage 306 may alternatively provide some amount of gain.

[0042] Although not depicted in FIG. 3, in accordance with one embodiment, a programmable filter may be electrically coupled between the first gain stage 304 and the programmable attenuation/gain stage 306. The programmable filter may be a programmable low pass filter with a programmable cut-off frequency, or a programmable notch filter with a programmable center frequency. For example, where there is an indication of high frequency noise at the output of the first gain stage 304, the cutoff frequency of the programmable filter may be lowered (or the center frequency adjusted) to filter out the noise. The programmable filter may also be comprised of multiple filters such as a band pass filter with an integrated band stop filter to reject a specific frequency or frequencies such as 60 and 120 Hz while allowing other frequencies in a range from about 0.5 Hz to 100 Hz or from about 0.5 Hz to 200 Hz.

[0043] The ECG signal may experience rapid and wide variations in amplitude due to interference from unrelated signals. For example, the ECG signal may include noise due to a nearby electronic device. ECG signal noise can also be caused by electrodes sliding on the patient's body due to extreme patient movement, such as vigorous exercise. A poorly fit electrode belt or garment can allow the electrodes to slide on the patient's body even with minor patient movement. Typically, the dynamic range of the signal acquisition circuit 300 is limited and not suited to accommodate large fluctuations of the signal input. The ALC 314 allows the signal acquisition circuit 300 to use the entire dynamic range of the ECG signal by controlling the amount of attenuation provided at the programmable attenuation/gain stage 306. The signal acquisition circuit 300 is configured to detect ECG signals between the range of about 100 microvolts and about 5 millivolts, with signals below about 80 microvolts being considered to be indicative of an asystolic condition. To perform automatic level control of the ECG signal, the ALC 314 varies the amount of attenuation applied at the programmable attenuation/gain stage 306 depending on the level of the output signal provided by the ADC 312. If the ALC 314 determines that the voltage level of the ECG signal provided by the ADC is too high, the ALC 314 can send a control signal to the programmable attenuation/gain stage 306 to increase the amount of attenuation applied to the ECG signal. In contrast, if the voltage level of the ECG signal is too low, the ALC 314 can send a control signal to the programmable attenuation/gain stage 306 to decrease the amount of attenuation to the ECG signal.

[0044] The programmable attenuation/gain stage 306 is electrically coupled to the second gain stage 308 that further amplifies the ECG signal. Similar to the first gain stage 304, the second gain stage 308 may include a single amplifier or a series of amplifiers. The second gain stage 308 multiplies the input voltage level received from the programmable attenuation/gain stage 306 by a predetermined amount of gain, G2. In one embodiment, the second gain stage 308 provides a gain of approximately 12 times the input. It is appreciated, that in some embodiments the programmable attenuation/gain stage

306 may be included as one of the amplifiers in the first gain stage 304, or the second gain stage 308. In some embodiments, the first gain stage 304 and the second gain stage 308 may include a programmable gain stage.

[0045] The second gain stage 308 is electrically coupled to the LPF 310. The LPF 310 is designed to reduce or eliminate high frequency noise and to protect the ADC 312 from ECG signals that would cause aliasing. For example, ECG signals having a frequency of more than half of the sample rate of the ADC can cause aliasing. In one exemplary embodiment, the LPF 310 has a bandwidth of approximately 100 Hz and a cutoff frequency at approximately 100 Hz. In some implementations, the LPF may be implemented as part of the second gain stage 308. In accordance with one embodiment, the LPF may be a programmable LPF having a programmable cutoff frequency that can be controlled by the SCC 322. The LPF 310 is electrically coupled to an input of the ADC 312. The ADC 312 digitizes the analog ECG signal to a digital signal and may further condition the signal prior for further analysis and monitoring by the at least one processor 210, as described above.

[0046] The functionality of the ACDC 316 to detect and correct analog clipping is described below. For clarity, the voltage level at the input of second gain stage 308 is labeled as IN2, the gain of the second gain stage 308 as G2 and the voltage level at the output of the second gain stage 308 as OUT2. The voltage level at the input of first gain stage 304 is labeled as IN1, the gain of the first gain stage 304 as G1 and the voltage level at the output of the first gain stage 304 as OUT1.

[0047] The ACDC 316 unit first calculates ECG voltage levels IN1, IN2, OUT1 and OUT2 at each of the gain stages based upon the voltage levels of the ECG signal at the output of the ADC 312 and the predetermined gain values, G1 and G2, as well as, the attenuation setting set by the ALC 314. The ACDC 316 then determines whether the voltage levels at each of the gain stages are approaching or are at the analog clipping thresholds at the first and second gain stages.

[0048] If the voltage level is approaching the clipping threshold after the programmable attenuation/gain stage 306, the ACDC 316 can send a control signal (CS) to the programmable attenuation/gain stage 306 to provide additional attenuation to the ECG signal provided at OUT1. Additional attenuation will prevent analog clipping of the signal at the second gain stage 308, IN2. In addition, where a programmable LPF 310 is used and the SCC 322 detects the presence of high frequency noise, additional analysis of the LPF input and output may be performed to determine if the high frequency noise is causing clipping. Should it be determined that high frequency noise is causing clipping, the SCC 322 may lower the cutoff frequency of the LPF 310.

[0049] By contrast, if the voltage levels are approaching or are at the clipping threshold before the programmable attenuation/gain stage 306, the sampled data at the ADC 312 is marked as compromised or corrupted to prevent mis-detection by the at least one processor 210. The ACDC 316 will continue to monitor the analog signal at the first gain stage 304 until the ECG signal returns to a level sufficiently below the analog clipping threshold. The ALC 314 functionality may be turned off until the ECG voltage level returns to below the threshold levels. Once the ECG signal at the first gain stage 304 is sufficiently below the threshold, the ALC 314 may be turned on and normal operation of the system may resume.

[0050] In some embodiments, where the first gain stage **304** and the second gain stage **308** are to both programmable gain/attenuation stages, the programmable attenuation/gain stage **306** may not be needed. In this embodiment, the ACDC **316** can determine whether voltage levels are approaching or are at the analog clipping thresholds at either the first or second programmable attenuation/gain stages. Where it is determined that the voltage level is approaching the clipping threshold at the first attenuation/gain stage, the ACDC **316** can send a control signal to the first attenuation/gain stage to reduce the amount of gain at the first attenuation/gain stage. Where it is determined that the voltage level is approaching the clipping threshold at the second attenuation/gain stage, the ACDC **316** can send a control signal to the second attenuation/gain stage to reduce the amount of gain at the second attenuation/gain stage. The reduction in gain can prevent analog clipping of the signal at either the first or the second attenuation/gain stages.

[0051] Values for the clipping threshold for the first gain stage **304** may be predetermined based on the voltage range of a typical human ECG and the maximum output level of the gain stage amplifiers that are used in the signal acquisition circuit **300**. For example, human ECG voltage levels are typically between about 80 microvolts and about 2 millivolts in amplitude. Due to the high gain required for processing the ECG signal, the gain stage amplifiers may start clipping when the analog signals received by the LIA **302** have amplitude of about 70 millivolts or more. Because ECG signals above approximately 2 millivolts are well outside the normal range of a human ECG signal, any input voltages provided to the LIA **302** that exceed this value may be considered corrupted. Such corrupted data can be flagged or marked to indicate to the at least one processor **210** that the data should not be used to determine proper treatment procedure. During this period of time, the functionality of the ALC **314** may be disabled until normal levels at the output of the LIA **302** return.

[0052] Having thus described several aspects of at least one embodiment of this invention, it is to be appreciated various alterations, modifications, and improvements will readily occur to those skilled in the art. Such alterations, modifications, and improvements are intended to be part of this disclosure, and are intended to be within the scope of the invention. Accordingly, the foregoing description and drawings are by way of example only.

What is claimed is:

1-19. (canceled)

20. A wearable medical device, comprising:

a plurality of ECG sensing electrodes configured to sense an ECG signal of a patient;

an ECG acquisition circuit electrically coupled to a pair of the plurality of ECG sensing electrodes including a first gain stage to amplify the ECG signal, a programmable attenuation/gain stage coupled to the first gain stage to condition the amplified ECG signal, and a second gain stage coupled to the programmable attenuation/gain stage to amplify the conditioned ECG signal;

an analog to digital converter electrically coupled to the ECG acquisition circuit to receive and digitize the amplified and conditioned analog ECG signal and provide a digitized ECG signal; and

a signal conditioning and control unit electrically coupled to the ECG acquisition circuit and the analog to digital converter to monitor the digitized ECG signal, to determine whether a voltage level of the ECG signal is

approaching a first threshold in the first gain stage based on at least the digitized ECG signal, and to mark the amplified and conditioned analog ECG signal as compromised in response to a determination that the voltage level of the ECG signal is approaching the first threshold.

21. The wearable medical device of claim **20**, wherein the signal conditioning and control unit is configured to vary an amount of attenuation/gain provided by the programmable attenuation/gain stage based on the digitized ECG signal.

22. The wearable medical device of claim **21**, wherein the signal conditioning and control unit is configured to determine whether a voltage level of the digitized ECG signal is above a second threshold, and to increase the amount of attenuation provided by the programmable attenuation/gain stage.

23. The wearable medical device of claim **21**, wherein the signal conditioning and control unit is configured to determine whether a voltage level of the digitized ECG signal is below a second threshold, and to decrease the amount of attenuation provided by the programmable attenuation/gain stage.

24. The wearable medical device of claim **20**, wherein the signal conditioning and control unit is configured to determine the first threshold based on at least one of a voltage range of an ECG of a human patient, a current gain setting and a maximum output voltage level of at least one of the first gain stage, the programmable attenuation/gain stage and the second gain stage.

25. The wearable medical device of claim **20**, wherein the signal conditioning and control unit is configured to determine whether a voltage level of the conditioned ECG signal is approaching a second threshold based on at least the digitized ECG signal.

26. The wearable medical device of claim **25**, wherein the signal conditioning and control unit is configured to attenuate the amplified and conditioned analog ECG signal in response to a determination that the voltage level is approaching the second threshold.

27. The wearable medical device of claim **25**, wherein the signal conditioning and control unit is configured to determine the second threshold based on at least one of a voltage range of an ECG of a human patient, a current gain setting and a maximum output voltage level of at least one of the first gain stage, the programmable attenuation/gain stage and the second gain stage.

28. The wearable medical device of claim **20**, wherein the signal conditioning and control unit is configured to detect high frequency noise in the ECG signal and adjusting a cutoff frequency of a filter responsive to detecting the high frequency noise.

29. A wearable medical device, comprising:

a plurality of ECG sensing electrodes configured to sense an ECG signal of a patient;

an ECG acquisition circuit electrically coupled to a pair of the plurality of ECG sensing electrodes and including a first gain stage to amplify the ECG signal, a programmable attenuation/gain stage coupled to the first gain stage to condition the amplified ECG signal, and a second gain stage coupled to the programmable attenuation/gain stage to amplify the conditioned ECG signal;

an analog to digital converter electrically coupled to the ECG acquisition circuit to receive and digitize the

amplified and conditioned analog ECG signal and provide a digitized ECG signal; and
a signal conditioning and control unit electrically coupled to the ECG acquisition circuit and the analog to digital converter to monitor the digitized ECG signal and to determine whether at least one of the ECG signal, the amplified ECG signal, the amplified and conditioned ECG signal, and the digitized ECG signal is approaching at least one clipping threshold based upon the digitized ECG signal, the at least one clipping threshold being determined based on at least one of a voltage range of an ECG human patient, a maximum output voltage level and a current gain setting of each of the first gain stage, the programmable attenuation/gain stage and the second gain stage.

30. The wearable medical device of claim **29**, wherein the at least one clipping threshold includes a first clipping threshold indicative of clipping in the first gain stage and a second clipping threshold indicative of clipping in the second gain stage.

31. The wearable medical device of claim **30**, wherein the signal conditioning and control unit is configured to identify that the ECG signal is compromised in response to a determination that a voltage level of the ECG signal is above the first clipping threshold.

32. The wearable medical device of claim **30**, wherein the signal conditioning and control unit is configured to vary an amount of attenuation applied by the programmable attenuation/gain stage based on the digitized ECG signal.

33. The wearable medical device of claim **32**, wherein the signal conditioning and control unit is configured to determine whether a voltage level of the conditioned ECG signal is above the second clipping threshold and wherein the signal conditioning and control unit is configured to vary the amount of attenuation at least in part by increasing the amount of attenuation applied by the programmable attenuation/gain stage in response to a determination that the voltage level of the conditioned ECG signal is above the second clipping threshold.

34. The wearable medical device of claim **32**, wherein the signal conditioning and control unit is configured to determine whether a voltage level of the conditioned ECG signal is below the second clipping threshold and wherein the signal conditioning and control unit is configured to vary the amount of attenuation at least in part by decreasing the amount of attenuation applied by the programmable attenuation/gain stage in response to a determination that the voltage level of the conditioned ECG signal is below the second clipping threshold.

35. The wearable medical device of claim **29**, wherein the signal conditioning and control unit is configured to determine whether clipping of the amplified and conditioned ECG signal occurred before or after the programmable attenuation/gain stage.

36. The wearable medical device of claim **35**, wherein the signal conditioning and control unit is configured to identify that the amplified and conditioned ECG signal is compromised in response to a determination that the clipping of the amplified and conditioned ECG signal occurred before the programmable attenuation/gain stage.

37. The wearable medical device of claim **35**, wherein the signal conditioning and control unit is configured to attenuate the amplified and conditioned ECG signal in response to a determination that the clipping of the amplified and conditioned ECG signal occurred after the programmable attenuation/gain stage.

38. The wearable medical device of claim **35**, wherein the signal conditioning and control unit is configured to attenuate the amplified and conditioned ECG signal in response to a determination that the clipping of the amplified and conditioned ECG signal occurred after the programmable attenuation/gain stage and wherein the signal conditioning and control unit is configured to identify that the amplified and conditioned ECG signal is compromised in response to a determination that the clipping of the amplified and conditioned ECG signal occurred before the programmable attenuation/gain stage.

* * * * *

| | | | |
|----------------|--|---------|------------|
| 专利名称(译) | 检测可穿戴移动医疗设备中的信号削波的方法 | | |
| 公开(公告)号 | US20150080699A1 | 公开(公告)日 | 2015-03-19 |
| 申请号 | US14/451046 | 申请日 | 2014-08-04 |
| [标]申请(专利权)人(译) | 卓尔医学产品公司 | | |
| 申请(专利权)人(译) | ZOLL医疗公司 | | |
| 当前申请(专利权)人(译) | ZOLL医疗公司 | | |
| [标]发明人 | KAIB THOMAS E VOLPE SHANE S MACHO JOHN D | | |
| 发明人 | KAIB, THOMAS E. VOLPE, SHANE S. MACHO, JOHN D. | | |
| IPC分类号 | A61B5/04 A61B5/00 A61B5/0408 | | |
| CPC分类号 | A61B5/04014 A61B5/4836 A61B5/6831 A61B5/04085 A61B5/7203 A61B5/02055 A61B5/021 A61B5/0402 A61B5/0408 A61B5/04286 A61B5/053 A61B5/14552 A61B5/6801 A61B5/6805 A61B7/04 A61B2562/0204 A61N1/3987 H03G7/002 H03G7/005 | | |
| 优先权 | 61/467532 2011-03-25 US | | |
| 其他公开文献 | US9204813 | | |
| 外部链接 | Espacenet USPTO | | |

摘要(译)

公开了一种可穿戴医疗设备和检测ECG信号的削波的方法。在一个实施例中，可穿戴医疗设备包括：多个ECG感测电极，被配置为感测患者的ECG；以及ECG采集电路，电耦合到一对多个ECG感测电极，并被配置为提供放大和调节的模拟ECG信号。信号，电耦合在第一增益级和第二增益级之间的可编程衰减/增益级，电耦合到ECG采集电路的ADC，用于接收和数字化放大和调节的模拟ECG信号并提供数字化ECG信号，以及信号调节到和控制单元电耦合到ECG采集电路和ADC，以接收和监测数字化ECG信号，并基于数字化ECG信号检测放大和调节的模拟ECG信号的削波。

A wearable medical device and method of detecting clipping of ECG signals is disclosed. In one embodiment, the wearable medical device comprises a plurality of ECG sensing electrodes configured to sense an ECG of a patient and an ECG acquisition circuit electrically coupled to a pair of the plurality of ECG sensing electrodes and configured to provide an amplified and conditioned analog ECG signal, a programmable attenuation/gain stage electrically coupled between a first gain stage and a second gain stage, an ADC electrically coupled to the ECG acquisition circuit to receive and digitize the amplified and conditioned analog ECG signal and provide a digitized ECG signal, and a signal conditioning to and control unit electrically coupled to the ECG acquisition circuit and the ADC to receive and monitor the digitized ECG signal and to detect clipping of the amplified and conditioned analog ECG signal based upon the digitized ECG signal.