



US 20190091476A1

(19) **United States**

(12) **Patent Application Publication**  
**HERNANDEZ et al.**

(10) **Pub. No.: US 2019/0091476 A1**  
(43) **Pub. Date: Mar. 28, 2019**

(54) **SYSTEM COMPRISING A PROBE FOR DETECTING A MASS DISCHARGE OF ACTION POTENTIALS AND A PROBE FOR STIMULATING A VAGUS NERVE OF AN EPILEPSY PATIENT**

**Publication Classification**

(51) **Int. Cl.**  
*A61N 1/36* (2006.01)  
*A61B 5/04* (2006.01)  
*A61B 5/00* (2006.01)  
(52) **U.S. Cl.**  
CPC ..... *A61N 1/36053* (2013.01); *A61B 5/04001* (2013.01); *A61B 5/4836* (2013.01); *A61N 1/36064* (2013.01); *A61B 5/4094* (2013.01)

(71) Applicants: **UNIVERSITE DE RENNES 1**, Rennes (FR); **INSERM (INSTITUT NATIONAL DE LA SANTE ET DE LA RECHERCHE MEDICALE)**, Paris (FR); **CNRS (CENTRE NATIONAL DE LA RECHERCHE SCIENTIFIQUE)**, Paris (FR); **CHU DE RENNES (CENTRE HOSPITALIER UNIVERSITAIRE DE RENNES)**, Rennes (FR)

(57) **ABSTRACT**

A treatment system for stimulating the vagus nerves is described, comprising the following elements: -a detection and control unit (20); -at least one detection probe (10d, 10g) connected to the detection and control unit and intended to be applied to at least one of the two vagus nerves of a patient; -means (24) provided in the detection and control unit for detecting a phenomenon of mass discharge of action potentials in at least one vagus nerve using the detection probe or detection probes; -stimulation probes (10d, 10g) for stimulating vagus nerves, and -means (24) provided in the detection and control unit that are capable, in response to the detection of a mass discharge, of applying predefined asymmetric stimulation signals to said stimulation probes capable of causing a depolarization and/or hyperpolarization of the vagus nerves and of blocking the conduction of the action potentials at least in the efferent direction. The system is intended for preventing the risk of sudden death in the event of an epileptic seizure in epilepsy patients.

(72) Inventors: **Alfredo HERNANDEZ**, Cesson-sevigne (FR); **Benoit MARTIN**, Meung-sur-loire (FR); **Arnaud BIRABEN**, Rennes (FR)

(21) Appl. No.: **16/076,410**  
(22) PCT Filed: **Feb. 13, 2017**  
(86) PCT No.: **PCT/EP2017/053156**  
§ 371 (c)(1),  
(2) Date: **Aug. 8, 2018**

(30) **Foreign Application Priority Data**  
Feb. 12, 2016 (FR) ..... 16/70039

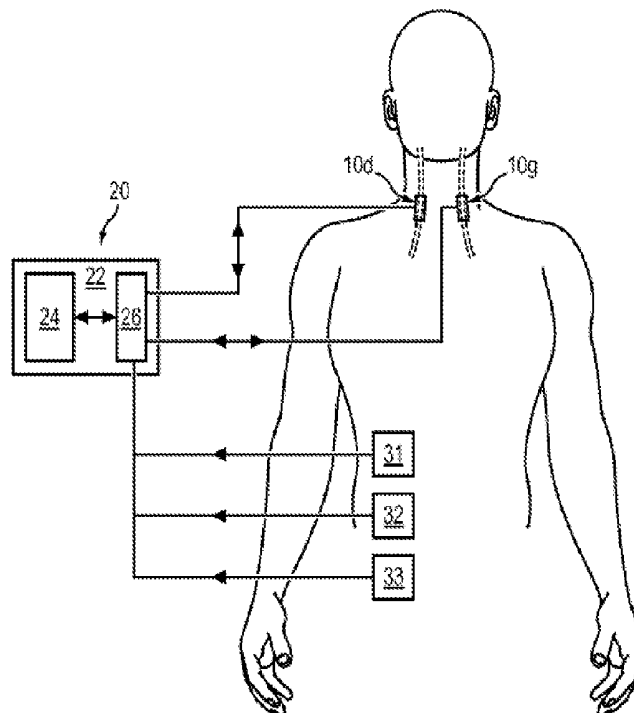


FIG. 1

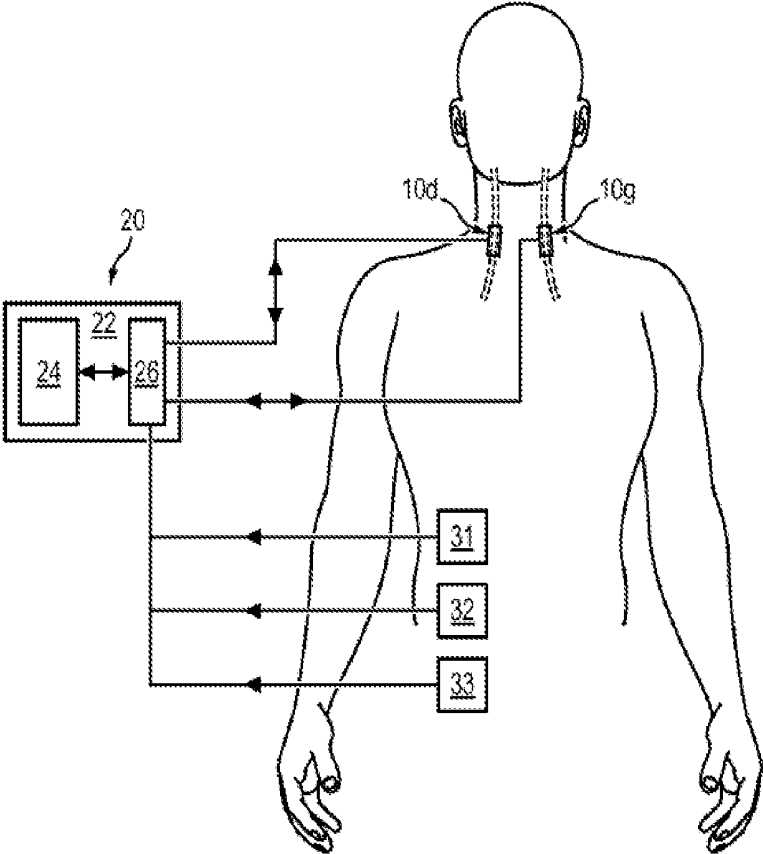


FIG. 2

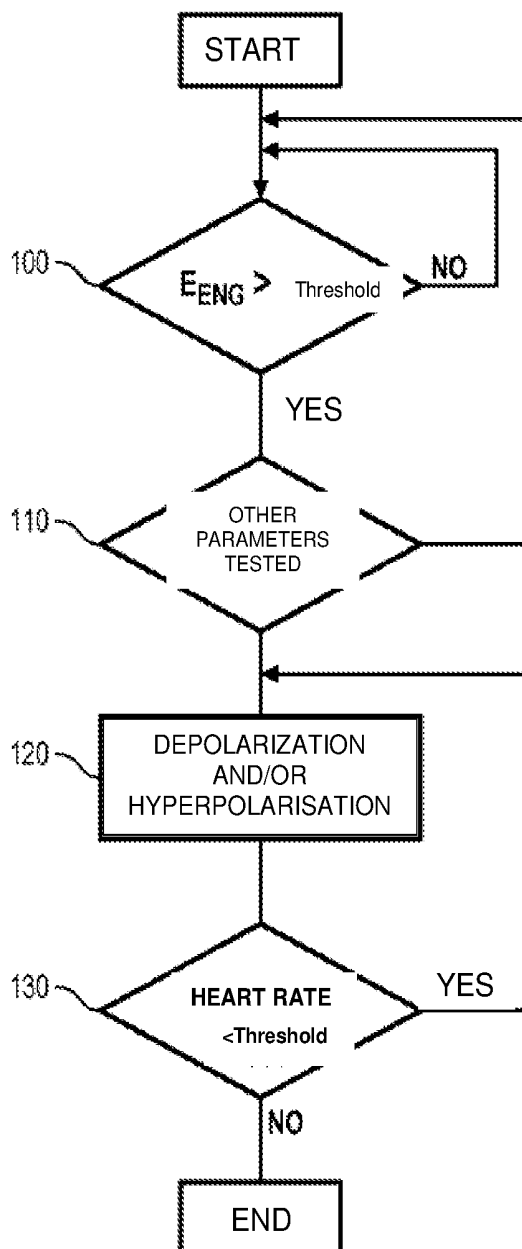


FIG. 3


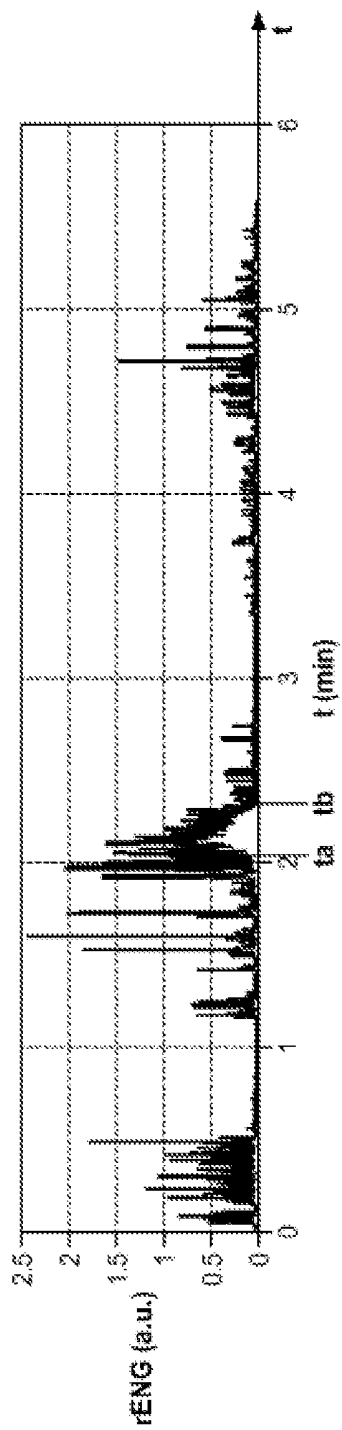


FIG. 4

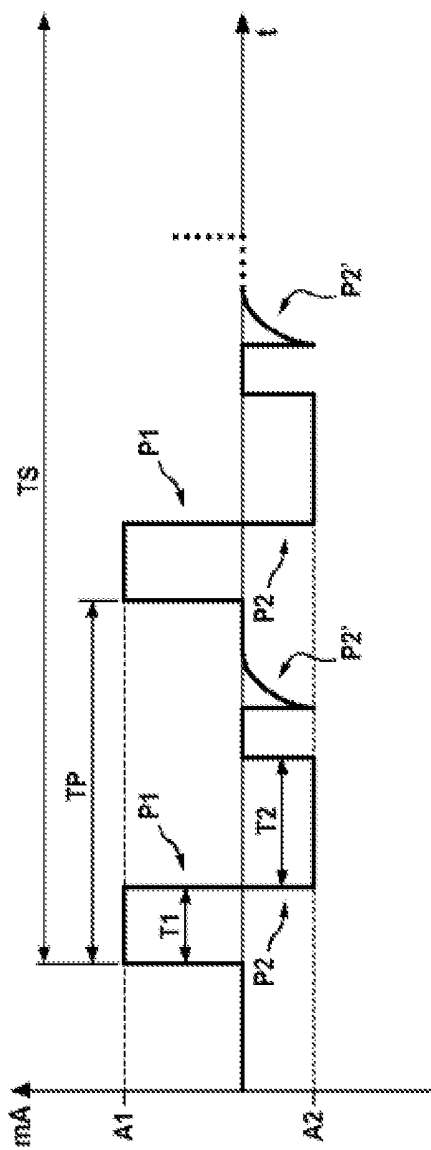

**SYSTEM COMPRISING A PROBE FOR  
DETECTING A MASS DISCHARGE OF  
ACTION POTENTIALS AND A PROBE FOR  
STIMULATING A VAGUS NERVE OF AN  
EPILEPSY PATIENT**

FIELD OF THE INVENTION

**[0001]** The present invention relates to the field of medical devices intended to prevent the most serious consequences of an epileptic seizure in humans.

**[0002]** More particularly, it relates to a medical device aimed, on the basis of the activity of at least one vagus nerve and preferably both vagus nerves, at identifying the occurrence of an abnormal activity that could be fatal, secondary to an epileptic seizure (the SUDEP phenomenon, which stands for "Sudden Unexpected Death in Epilepsy"), and at reducing this risk by acting on the vagus nerve(s) to eradicate this phenomenon.

STATE OF THE ART

**[0003]** Today, we do not know how to prevent the risk of sudden death, or to eradicate the phenomenon of epilepsy likely to cause sudden death when it occurs.

**[0004]** The closest state of the art is represented by the following documents:

**[0005]** a) document US2014/0142653A1 describes a method for treating a patient suffering from epilepsy, based on the measurement of a physiological signal (typically an electroencephalogram, possibly in combination with measurement of the heart rate) making it possible to determine whether the patient is undergoing a seizure, or has just undergone a seizure. Depending on the measurement obtained, the method applies a stimulation on one of the two vagus nerves, or on both, on one side in the efferent direction in order to act on the heart rate, and on the other side in the afferent direction in an attempt to reduce the epileptic phenomenon. This document gives no indication, however, on the way in which an actual risk of sudden death caused by epilepsy can be determined, or on the way in which a stimulation could reduce or even cancel out the risk, or even on the capacity of the method to reduce mortality other than by reducing the epileptic seizures. Thus, it relates only to the treatment of epileptic seizures in general.

**[0006]** b) Document U.S. Pat. No. 8,634,922B1 discloses a vagus nerve stimulation system for the treatment of epilepsy, which takes into account a measurement of the cardiac signal in order to optimize treatment, and more precisely in order to correct a stimulation intended to treat an epileptic seizure so as to prevent undesirable effects with respect to the heart rate. Furthermore, according to this document, only one stimulation in the afferent direction is appropriate for treating the epileptic seizure.

**[0007]** There are also numerous other documents on the stimulation of the vagus nerves, but none of them specifically deals with preventing the risk of sudden death when an epileptic seizure occurs. These include, in particular, US 2007/027486 A1 and US 2007/255320 A1.

**[0008]** Lastly, commercial solutions for stimulating the vagus nerve exist that aim to reduce the number of epileptic seizures in epilepsy patients, but these solutions are ineffectual in protecting patients against sudden death if a seizure occurs. An example of such a vagus-nerve neuro-

stimulation system is sold by Cyberonics and is indicated for incapacitating or pharmacoresistant epilepsy.

SUMMARY OF THE INVENTION

**[0009]** The present invention aims to enable, on the one hand, the detection at the vagus nerve or preferably at both vagus nerves, if necessary in combination with one or more other physiological signals, of the occurrence of an abnormal and intense paroxysmal activity, likely to cause death (this activity probably being linked to an epileptic seizure, but the subject of the invention not being in itself to detect the occurrence of epileptic seizures) and, on the other hand, by acting on the vagus nerve or preferably both vagus nerves, substantially to reduce this risk of hyperactivity and death.

**[0010]** According to the invention according to a first aspect, a system is thus proposed intended to limit the risks of sudden death in the event of an epileptic seizure, characterized in that it comprises:

**[0011]** a detection and control unit;

**[0012]** at least one detection probe connected to the detection and control unit and intended to be applied to at least one of the two vagus nerves of a patient,

**[0013]** means provided in the detection and control unit for detecting a phenomenon of mass discharge of action potentials in at least one vagus nerve using the detection probe or detection probes,

**[0014]** at least one stimulation probe for stimulating a vagus nerve, and

**[0015]** means provided in the detection and control unit that are capable, in response to the detection of a mass discharge, of applying predefined asymmetric stimulation signals to the stimulation probe(s) capable of causing a depolarization and/or hyperpolarization of the vagus nerve (s) and of blocking the conduction of the action potentials at least in the efferent direction.

**[0016]** The above system advantageously but optionally comprises the following additional characteristics, taken individually or in any combination that a person skilled in the art will deem technically compatible:

**[0017]** \* the detection probe(s) and the stimulation probe (s) constitute the same probes;

**[0018]** \* the mass discharge detection means are configured to determine an overall electrical energy density in at least one vagus nerve;

**[0019]** \* the mass discharge detection means comprise a means of comparing an electrical power in a set frequency band with a threshold;

**[0020]** \* the electrical power is determined by squaring and low-pass filtering a signal that has undergone low-pass filtering within said frequency band;

**[0021]** \* which comprises two probes for stimulating the left and right vagus nerves;

**[0022]** \* of which the stimulation signals are periodic and deterministic;

**[0023]** \* the asymmetry of the stimulation signals is chosen so as to achieve a depolarization of the nerve fibers of the vagus nerve(s);

**[0024]** \* the asymmetry of the stimulation signals is chosen so as to achieve a hyperpolarization of the nerve fibers of the vagus nerve(s);

**[0025]** \* the asymmetric periodic signals have a frequency of between around 15 and 300 kHz;

[0026] \* the stimulation signals comprise a succession of generally rectangular positive and negative current pulses, the amplitudes of the positive and negative pulses being different;

[0027] \* the current pulses of greater amplitude are shorter in duration than the current pulses of smaller amplitude;

[0028] \* the amplitudes and durations are chosen so that the balance of the electrical charges applied to the electrodes and taken from the electrodes is basically neutral;

[0029] \* the duration (TS) of the stimulation pulses is preset and lasts between around 0.5 and around 2 s;

[0030] \* the system comprises a means for determining the heart rate, and in which the pulses are applied until a heart rate above the threshold is resumed;

[0031] \* the detection and control unit also comprises an input for at least one signal chosen from a cardiac signal, a respiratory signal, an oxymetry signal and an electromyography signal;

[0032] \* the detection and control unit comprises an input for an electromyography signal, this signal being derived from the signal provided by the detection probe(s);

[0033] \* the system comprises detection probes configured to be positioned on both vagus nerves, and the mass discharge detection means are configured to operate on signals coming from both detection probes.

[0034] According to a second aspect of the invention, a method implemented in a system as described above is proposed for selectively generating electrical control signals of at least one probe of a vagus nerve of a patient with a view to containing the risks of sudden death in the event of an epileptic seizure, characterized in that it comprises the following steps:

[0035] detecting an electrical phenomenon supplied by at least one detection probe and representative of a mass discharge of action potentials in the vagus nerve;

[0036] in response to this detection, generating preset asymmetrical stimulation electrical signals intended to be applied to at least one stimulation probe and having the characteristics appropriate to cause on their application a depolarization and/or a hyperpolarization of the vagus nerve (s) and to block the conduction of the action potentials at least in the efferent direction.

[0037] Advantageously, the method also comprises a step of comparing a heart rate signal with a threshold, the generation of stimulation signals being performed in the event of detecting at the same time a mass discharge and the fact that the heart rate signal reveals a heart rate falling below a threshold.

[0038] In a similarly advantageous way, the method also comprises, after the step of generating stimulation signals, a step of comparing a heart rate signal with a threshold, and a new step of generating stimulation signals if the heart rate signal reveals a heart rate falling below a threshold.

[0039] Furthermore, the preferred but optional characteristics of the system apply equally to the above method.

#### BRIEF DESCRIPTION OF THE DRAWINGS

[0040] Further features, aims and advantages of the present invention will emerge more clearly from the following detailed description of a preferred embodiment thereof, given by way of non-limiting example with reference to the accompanying drawings, in which:

[0041] FIG. 1 is a schematic representation of a system according to the invention;

[0042] FIG. 2 shows a process implemented by the system according to the invention;

[0043] FIG. 3 gives an example of signals collected on a vagus nerve and showing a mass discharge phenomenon, and

[0044] FIG. 4 gives an example of the appearance of stimulation signals applied to a vagus nerve stimulation probe.

#### DETAILED DESCRIPTION OF A PREFERRED EMBODIMENT

##### a) General Principle

[0045] The object of the system according to the invention is to prevent risks of death connected with epileptic seizures (basically by the phenomenon of "SUDEP"), on the one hand thanks to a certain characterization of an electrophysiological signal collected at the vagus nerve, preferably at both vagus nerves, and on the other thanks to a certain electrical stimulation, in the efferent direction, applied to the vagus nerve(s).

[0046] The characterization is performed by detecting a mass discharge in the efferent direction of the vagus nerve, as will be described later, using a probe placed around one of the two vagus nerves or preferably two probes placed around the left and right vagus nerves.

[0047] Possibly, this characterization can be combined with one or more other physiological signals of the patient, and in particular a cardiac signal and/or a respiratory signal and/or an oxymetry signal and/or an electromyographic signal.

[0048] The action of reducing the risk of sudden death is performed according to the invention by electrical stimulation on one of the vagus nerves or preferably on both vagus nerves, in conditions appropriate to neutralize the signals conveyed in the nerves. This neutralization can be achieved either by applying to the nerve(s) a depolarization, so as to cause an instantaneous inhibition due to the refractory period, or by applying to the nerve(s) a hyperpolarization, having a blocking effect due to the inhibition of excitability, for a controlled period of time.

[0049] In order to determine the optimum conditions of a depolarization or a hyperpolarization, it is particularly helpful to refer to the document "Conduction block in myelinated axons induced by high-frequency (kHz) non-symmetric biphasic stimulation," Z. Zhao et al., *Frontiers in Computational Neuroscience*, July 2015, Volume 9, Article 86, which suggests the possibility of using non-symmetric alternating electric wave forms, with a preponderance of their positive component or their negative component, respectively, to achieve a blocking of the conduction of action potentials in the different nerve fibers.

[0050] More particularly, a non-symmetric biphasic electrical action can be used, in a first approach, with an alternating signal having longer positive pulses than the negative pulses, in order to create a hyperpolarization, and in a second approach, with an alternating signal having shorter positive pulses than the negative pulses, in order to create a depolarization.

[0051] There now follows, with reference to FIG. 4, a concrete example of signals intended to cause a hyperpolarization of the vagus nerve.

[0052] Furthermore, it is possible to combine such stimulating electrical signal characteristics with the use of spatial

selectivity probes. In particular, it is now known, thanks to specific structures of probe electrodes, to apply a stimulation in a preferential manner onto certain sections of the vagus nerve, in order to achieve this spatial selectivity. The depolarization or hyperpolarization can thus be applied in a preferred way onto certain nerve fibers, causing less disturbance to other fibers of which the conduction of action potentials has not necessarily been blocked. This spatial selectivity also allows the amplitude of the current required to block conduction to be reduced.

[0053] It is also possible to use the time dimension by performing depolarizations and/or hyperpolarizations according to different timings in different regions of the vagus nerve(s).

#### b) Detailed Implementation

[0054] There now follows a description, with reference to FIGS. 1 and 2, of a more detailed implementation of the invention.

[0055] FIG. 1 shows the left and right vagus nerves of a patient, LVN and RVN respectively.

[0056] On each vagus nerve, a detection and neurostimulation probe has been implanted, 10g and 10d respectively. Each probe preferably comprises an electrode matrix specifically to create an electrical stimulation with spatial and/or temporal selectivity. Advantageously, the combination of electrodes, or possibly only one pair of this combination, is used also during periods of no treatment in order to detect mass discharge. This can be performed for one vagus nerve or both vagus nerves. In a particular embodiment, the invention can be implemented on only one of the two vagus nerves. In particular, as the right vagus nerve is basically responsible for the effects on heart rate (sinus node), a detection and a stimulation of depolarization and/or hyperpolarization can be envisaged on this nerve only. However, detection and stimulation can also be performed on the left vagus nerve, which is chiefly associated with the modulation of the atrioventricular node.

[0057] Both probes are connected by multi-stranded conductors to a unit 20, preferably of the portable or implantable type, comprising in a box 22 a central processing unit 24 and input/output circuits 26 through which the signals are applied to the probes 10g, 10d, and collected from said probes. A battery, not shown, powers the circuits of the unit 20.

[0058] The system also comprises a heart rate sensor 31 such as a pulse sensor or a cardiac probe, and if necessary a respiratory sensor 32 and/or an oxymetry sensor 33.

[0059] The heart rate sensor is used at least to determine, as will be seen later, whether a neutralization of the action potentials results in keeping the heart rate above a threshold, i.e. whether the risk of cardiac arrest has been eliminated.

[0060] It can also be used as an additional detector of an epileptic seizure likely to lead to sudden death, in combination with the detection of a mass discharge in at least one of the two vagus nerves. This additional detection can for example involve determining whether the heart rate exceeds the top and bottom preset thresholds, these excesses creating risk situations for the patient. It can also involve detecting the presence of atrioventricular blocks, which can be caused by a mass activation of a vagus nerve.

[0061] The respiratory sensor and/or oxymetry sensor make it possible to determine whether the respiratory function of the patient is being normally fulfilled. If a sensor is

provided, the detection of a respiratory failure (reduction or absence of respiration muscle movements, or drop in the rate of oxygen in the blood) is combined with the detection of a mass discharge using at least one of the probes 10g, 10d to identify an epileptic seizure with risk of sudden death.

[0062] According to another improvement, the unit 20 can comprise means to analyze the electromyography signals so as to detect an abnormal muscle activity, due for example to the generalized tonicoclonic seizure often present before an SUDEP event. These signals can often be obtained directly by using the electrodes present in the detection probe(s) on the vagus nerve (capture of an ENG+EMG composite signal) or even between the stimulation box and one of the peripheral electrodes on the detection probe(s).

[0063] Preferably, the electromyographic analysis is performed in connection with step 110 of FIG. 2, and the stimulation is performed only when a muscle activity above a threshold is detected at the same time as the mass discharge phenomenon or prior to this phenomenon.

[0064] With reference now to FIG. 2, a preferred and simplified example of a process implemented using the system of FIG. 1 will now be described.

[0065] At step 100, the unit 20, which periodically collects the signals coming from at least one of the probes 10g and 10d, performs a calculation of the overall energy of the action potentials in the respective vagus nerve. Advantageously, this calculation is performed digitally, the signals forming the object of an analog/digital conversion in the circuit 26. Advantageously, it implements a band-pass filtering, for example on a band of between around 300 Hz and 3 kHz, and a time adjustment and integration, in a known way in the field of signal processing.

[0066] So as long as this energy does not exceed a given threshold, the test is periodically repeated by a closed loop command, for example with a period of 0.5 to 10 seconds.

[0067] When the unit detects that this energy is above a threshold, the other physiological parameters are then tested at step 110, although this step is optional. In particular, unit 20 can detect a heart rate window output, an atrioventricular block, a drop in respiratory activity below a threshold or even a muscle activity above a threshold, as explained above.

[0068] As long as these parameters remain within the normal ranges, the process is redirected upstream of step 100 and the global energy of the action potentials is again monitored.

[0069] If step 110, when it is envisaged, confirms a cardiac or respiratory anomaly, a depolarization and/or hyperpolarization cycle of the two vagus nerves using probes 10g, 10d is performed at step 120 in order to neutralize the action potentials at least in the efferent direction in the vagus nerves, as explained above.

[0070] Following this cycle, which may involve applying short bursts of depolarization and/or hyperpolarization signals, alternating and asymmetric as described above, unit 20 uses the signals of sensor 31 to determine at step 130 whether the heart rate is dropping below a certain threshold, for example in the order of 20 to 30 bpm depending on the patient. If it is, this means that the risk of death is always high and a new depolarization or hyperpolarization cycle is implemented, and so on. If it is not, the risk of sudden death can be eliminated with a certain reliability and the process is ended and a new monitoring process can be undertaken according to the timing defined in unit 20.

**[0071]** FIG. 3 shows, by way of illustration, the signal resulting from processing by a band-pass filtering, then a quadratic (squared) function, then a low-pass filtering, of a signal acquired from a detection probe on a vagus nerve. This resulting signal incorporates elements of the electroencephalogram and electromyogram, which can however be separated by filtration and additional processing of the signal.

**[0072]** FIG. 3 shows, between the time points  $t_a$  and  $t_b$ , a mass discharge phenomenon. It will be understood that, by the above-described processing, it is possible to detect a mass discharge. It is when this resulting signal exceeds a given threshold that a risk of sudden death during an epileptic seizure is identified.

**[0073]** FIG. 4 shows an example of stimulation signals applied to a vagus nerve probe according to the invention, with a view to achieving a hyperpolarization of the nerve in the efferent direction.

**[0074]** These signals comprise a succession of positive pulses of current P1 and negative pulses of current P2 of different durations, pulse P2 being followed by a pulse P2' of passive discharge, in a known way. In the case in question, the positive pulses of current have a greater amplitude, but a shorter duration, than the negative pulses. Advantageously, these amplitudes and these durations are chosen so that the balance of electrical charges applied to the vagus nerve and taken from the vagus nerve is neutral, so as to prevent the stimulation from electrically charging this region of the body.

**[0075]** Preferably, the duration mismatch between the positive pulses P1 and negative pulses P2 is between around 1 and 4  $\mu$ s, depending on the frequency of the signal.

**[0076]** This frequency is advantageously between 15 and 300 kHz, and more preferably near 20 kHz or above 100 kHz in order to have the desired effect by minimizing the energy delivered.

**[0077]** Thus, for a frequency of 20 kHz, i.e. a total pulse duration of 50  $\mu$ s (period TP in FIG. 4), it is possible to envisage for example a positive pulse P1 of a duration of 15  $\mu$ s, a negative pulse of a duration of 18  $\mu$ s, the remaining 17  $\mu$ s being taken up by the passive discharge pulse and by a waiting time before the next positive pulse.

**[0078]** Depending on the nature and type of the probe, the electrical intensity of the stimulation signal can vary, but typically an intensity amplitude in the order of 3 to 5 mA is used. In order to obtain (at least approximately) the above-mentioned electrical neutrality, the amplitude of each positive pulse in the above-described digital example is 18-15 times greater than the amplitude of each negative pulse.

**[0079]** Moreover, the sequence of pulses P1, P2, P2' is repeated a certain number of times for a total duration (TS in FIG. 4) in the order of a few seconds, or even continuously until the mass discharge ceases or until a heart rate above the threshold is resumed.

**[0080]** In the above example, the stimulation performs a hyperpolarization of a vagus nerve in the efferent direction. By implementing negative pulses of current of greater amplitude than the positive pulses of current (more preferably of shorter durations), as a variation it is possible to achieve a depolarization of the vagus nerves in the efferent direction.

**[0081]** Clearly, numerous variations and modifications of the invention can be introduced. In particular:

**[0082]** the mass discharge likely to indicate a physiopathological activity connected to an epileptic seizure likely to engender a sudden death phenomenon can be detected in one vagus nerve or in both vagus nerves identically or differently;

**[0083]** the electrical action aimed at neutralizing the action potentials can be applied to both vagus nerves identically or differently;

**[0084]** the probe(s) used for detecting a mass discharge can be the same probes as those used for the neutralization of the action potentials, or different probes;

**[0085]** the criteria and values of the detection parameters, as well as the parameters of stimulation electrical action, can be adjusted by clinical trials in order to optimize the detection and action efficiency;

**[0086]** physiological parameters other than heart rate, respiratory activity and muscle activity can be used, if necessary, to contain or by contrast eliminate the risk of a sudden death caused by epilepsy.

1. System intended to limit the risks of sudden death in the event of an epileptic seizure, characterized in that it comprises:

a detection and control unit (20);

at least one detection probe (10g, 10d) connected to the detection and control unit and intended to be applied to at least one of the two vagus nerves of a patient,

means (24) provided in the detection and control unit for detecting a phenomenon of mass discharge of action potentials in at least one vagus nerve using the detection probe or detection probes,

at least one stimulation probe for stimulating a vagus nerve, and

means (24) provided in the detection and control unit that are capable, in response to the detection of a mass discharge, of applying predefined asymmetric stimulation signals to the stimulation probe(s) (10g, 10d) capable of causing a depolarization and/or hyperpolarization of the vagus nerve(s) and of blocking the conduction of the action potentials at least in the efferent direction.

2. System according to claim 1, wherein the detection probe(s) and the stimulation probe(s) constitute the same probes (10g, 10d).

3. System according to claim 1, wherein the mass discharge detection means are configured to determine an overall electrical energy density in at least one vagus nerve.

4. System according to claim 3, wherein the mass discharge detection means (24) comprise a means of comparing an electrical power in a set frequency band with a threshold.

5. System according to claim 4, wherein the electrical power is determined by squaring and low-pass filtering a signal that has undergone low-pass filtering within said frequency band.

6. System according to claim 1, which comprises two probes for stimulating the left and right vagus nerves.

7. System according to claim 1, wherein the stimulation signals are periodic and deterministic.

8. System according to claim 7, wherein the asymmetry of the stimulation signals is chosen so as to achieve a depolarization of the nerve fibers of the vagus nerve(s).

9. System according to claim 7, wherein the asymmetry of the stimulation signals is chosen so as to achieve a hyperpolarization of the nerve fibers of the vagus nerve(s).

10. System according to claim 7, wherein the asymmetric periodic signals have a frequency of between around 15 and 300 kHz.

11. System according to claim 8, wherein the stimulation signals comprise a succession of generally rectangular positive and negative current pulses, the amplitudes of the positive and negative pulses being different.

12. System according to claim 11, wherein the current pulses of greater amplitude are shorter in duration than the current pulses of smaller amplitude.

13. System according to claim 12, wherein the amplitudes and durations are chosen so that the balance of the electrical charges applied to the electrodes and taken from the electrodes is basically neutral.

14. System according to claim 11, wherein the duration (TS) of the stimulation pulses is preset and lasts between around 0.5 and around 2 s.

15. System according to claim 11, that comprises a means for determining the heart rate, and in which the pulses are applied until a heart rate above the threshold is resumed.

16. System according to claim 1, wherein the detection and control unit also comprises an input for at least one signal chosen from a cardiac signal, a respiratory signal, an oxymetry signal and an electromyography signal.

17. System according to claim 16, wherein the detection and control unit comprises an input for an electromyography signal, this signal being derived from the signal provided by the detection probe(s).

18. System according to claim 1, comprising detection probes configured to be positioned on both vagus nerves and

wherein the mass discharge detection means are configured to operate on signals coming from both detection probes.

19. Method implemented in a system according to claim 1 for selectively generating electrical control signals of at least one probe of a vagus nerve of a patient with a view to containing the risks of sudden death in the event of an epileptic seizure, characterized in that it comprises the following steps:

detecting an electrical phenomenon supplied by at least one detection probe (10g, 10d) and representative of a mass discharge of action potentials in the vagus nerve; in response to this detection, generating preset asymmetrical stimulation electrical signals intended to be applied to at least one stimulation probe and having the characteristics appropriate to cause on their application a depolarization and/or a hyperpolarization of the vagus nerve(s) and to block the conduction of the action potentials at least in the efferent direction.

20. Method according to claim 19, which also comprises a step of comparing a heart rate signal with a threshold, the generation of stimulation signals being performed in the event of detecting at the same time a mass discharge and the fact that the heart rate signal reveals a heart rate falling below a threshold.

21. Method according to claim 19, which also comprises, after the step of generating stimulation signals, a step of comparing a heart rate signal with a threshold, and a new step of generating stimulation signals if the heart rate signal reveals a heart rate falling below a threshold.

\* \* \* \* \*

专利名称(译)	系统包括用于检测动作电位的质量放电的探针和用于刺激癫痫患者的迷走神经的探针		
公开(公告)号	<a href="#">US20190091476A1</a>	公开(公告)日	2019-03-28
申请号	US16/076410	申请日	2017-02-13
[标]申请(专利权)人(译)	雷恩第一大学 法国国家健康医学研究院 法国国家科学研究中心		
申请(专利权)人(译)	UNIVERSITE 雷恩1 INSERM ( INSTITUT NATIONAL DE LA SANTE ET DE LA RECHERCHE MEDICALE ) 法国国家科学研究中心 ( CENTRE 法国国家科学研究 )		
当前申请(专利权)人(译)	法国国家科学研究中心 ( CENTRE 法国国家科学研究 ) INSERM ( INSTITUT NATIONAL DE LA SANTE ET DE LA RECHERCHE MEDICALE ) UNIVERSITE 雷恩1		
[标]发明人	HERNANDEZ ALFREDO MARTIN BENOIT BIRABEN ARNAUD		
发明人	HERNANDEZ, ALFREDO MARTIN, BENOIT BIRABEN, ARNAUD		
IPC分类号	A61N1/36 A61B5/04 A61B5/00		
CPC分类号	A61N1/36053 A61B5/04001 A61B5/4094 A61N1/36064 A61B5/4836		
优先权	2016070039 2016-02-12 FR		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

摘要(译)

描述了一种用于刺激迷走神经的治疗系统，包括以下元件：- 检测和控制单元 ( 20 )；- 至少一个检测探针 ( 10 10 ) 连接到检测和控制单元并且意图适用于患者的两个迷走神经中的至少一个；- 检测和控制单元中提供的用于检测至少一个迷走神经中的动作电位的质量放电现象的装置 ( 24 )，使用检测探针或检测探针；- 用于刺激迷走神经的刺激探针 ( 10 10 ) - 24 ) 在检测和控制单元中提供，其响应于质量放电的检测，能够将预定义的不对称刺激信号施加到能够引起迷走神经的去极化和/或超极化的所述刺激探针。并且至少在传出方向上阻止动作电位的传导。该系统旨在预防癫痫患者癫痫发作时猝死的风险。

