



US 20160106333A1

(19) **United States**

(12) **Patent Application Publication**
KANG et al.

(10) **Pub. No.: US 2016/0106333 A1**

(43) **Pub. Date: Apr. 21, 2016**

(54) **DETACHABLE BIOSIGNAL COMPLEX
SENSOR AND METHOD OF DETECTING
BIOSIGNAL INFORMATION USING THE
SAME**

Publication Classification

(71) Applicant: **SAMSUNG ELECTRONICS CO.,
LTD.**, Suwon-si (KR)

(51) **Int. Cl.**
A61B 5/0408 (2006.01)
A61B 5/117 (2006.01)
A61B 5/02 (2006.01)
A61B 5/026 (2006.01)
A61B 5/00 (2006.01)
A61B 5/0205 (2006.01)

(72) Inventors: **Jaemin KANG**, Seoul (KR); **Yongjoo
KWON**, Yongin-si (KR); **Sunkwon
KIM**, Suwon-si (KR); **Younho KIM**,
Hwaseong-si (KR); **Sangyun PARK**,
Hwaseong-si (KR)

(52) **U.S. Cl.**
CPC *A61B 5/04085* (2013.01); *A61B 5/681*
(2013.01); *A61B 5/0205* (2013.01); *A61B*
5/0082 (2013.01); *A61B 5/02007* (2013.01);
A61B 5/026 (2013.01); *A61B 5/117* (2013.01);
A61B 5/0537 (2013.01)

(73) Assignee: **SAMSUNG ELECTRONICS CO.,
LTD.**, Suwon-si (KR)

(57) **ABSTRACT**

(21) Appl. No.: **14/804,518**

A detachable biosignal complex sensor includes a clip type structure including: a circuit module configured to receive a biosignal of a subject and perform signal processing on the biosignal, a first plate, and a second plate having an end thereof which is rotatably connected to an end of the first plate so that the clip type structure is configured to be fastened to an item; and a sensor and electrodes provided on outer surfaces of the first plate and the second plate and configured to obtain the biosignal and transmit the obtained biosignal to the circuit module.

(22) Filed: **Jul. 21, 2015**

(30) **Foreign Application Priority Data**

Oct. 15, 2014 (KR) 10-2014-0139068

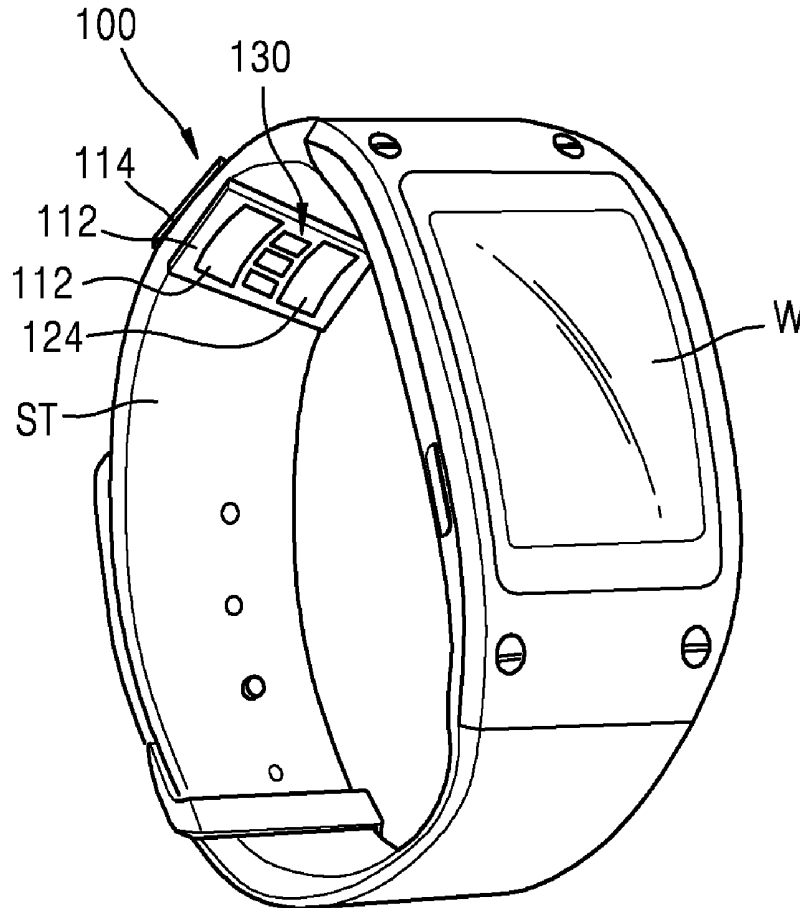


FIG. 1A

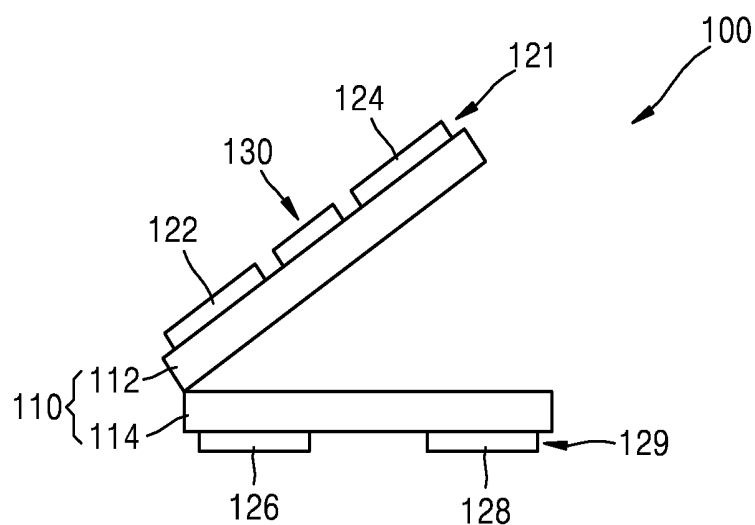


FIG. 1B

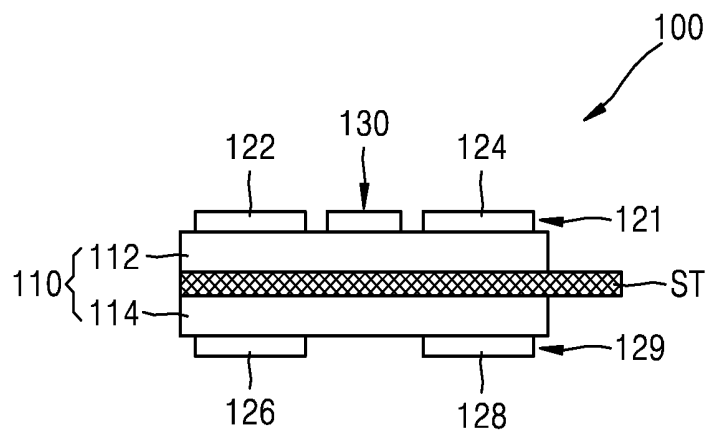


FIG. 2A

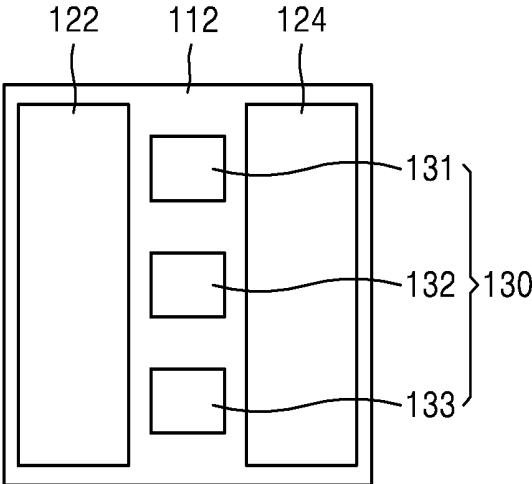


FIG. 2B

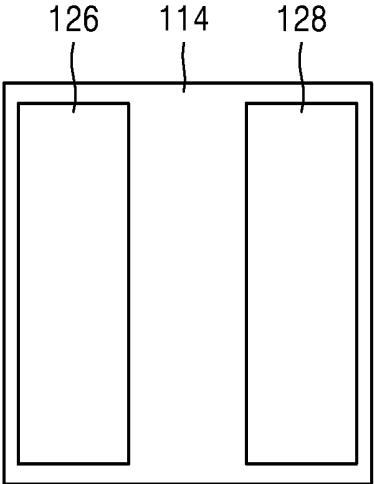


FIG. 3A

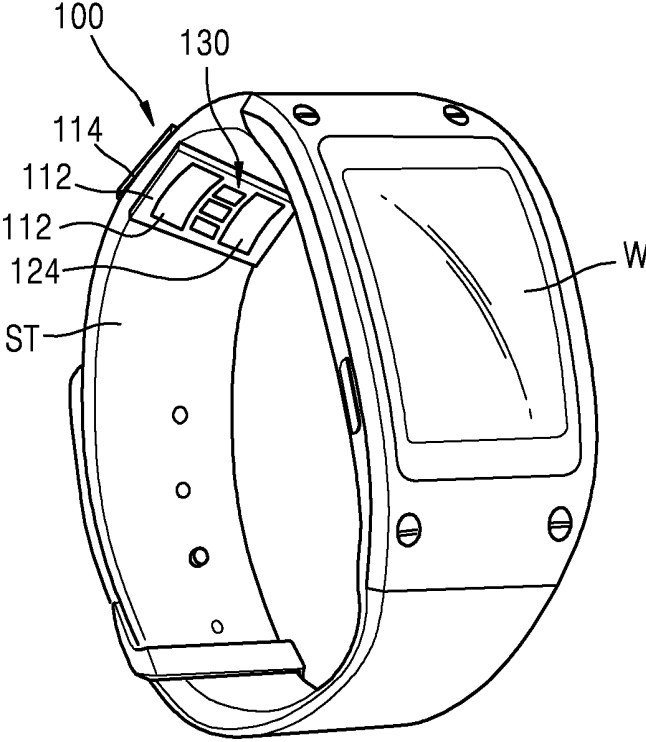


FIG. 3B

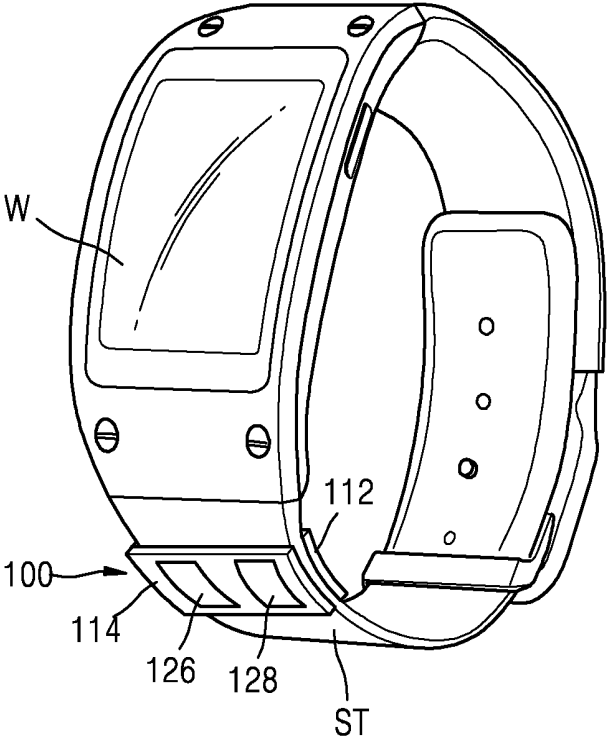


FIG. 4A

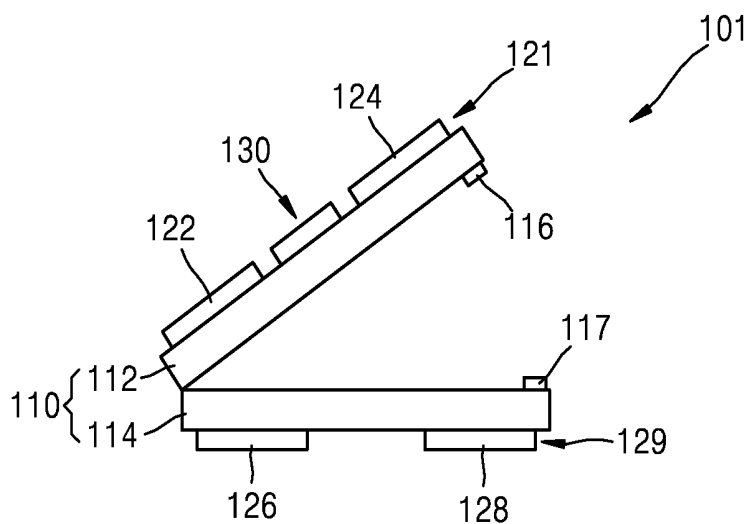


FIG. 4B

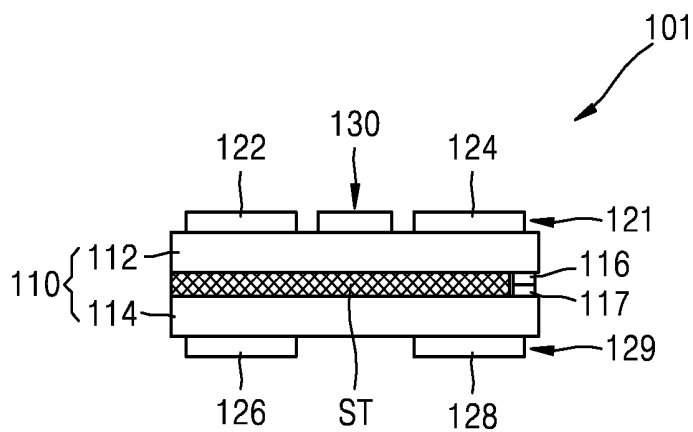


FIG. 5

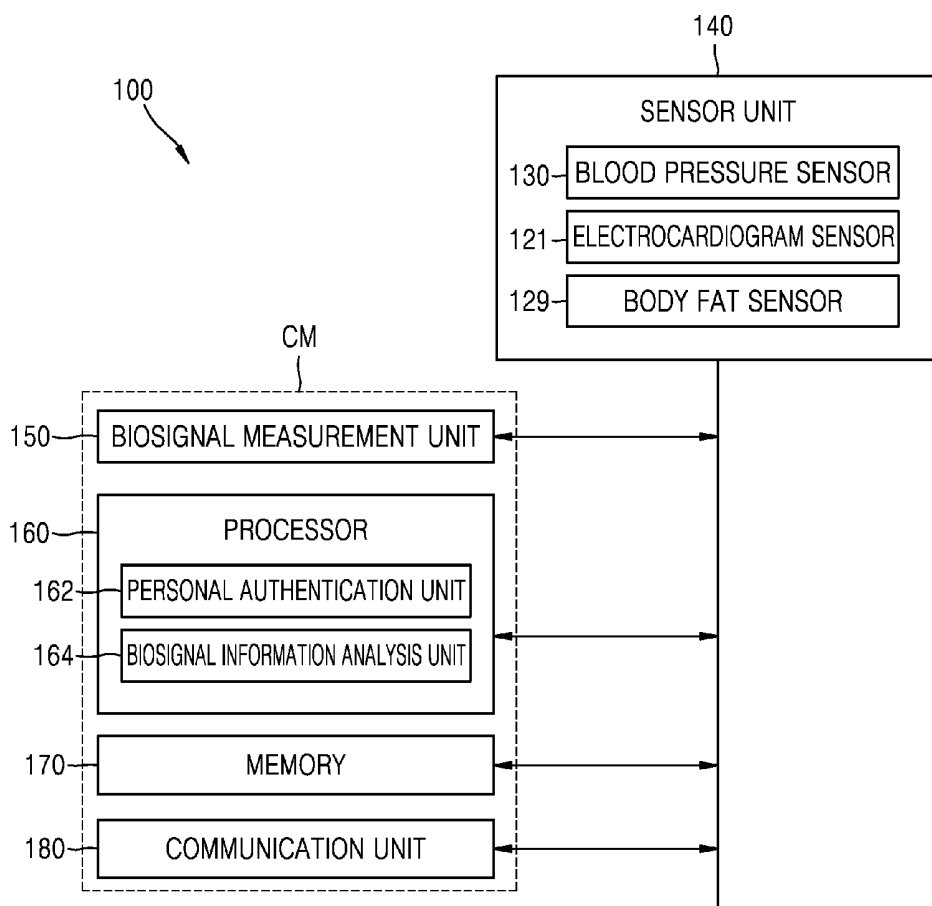


FIG. 6

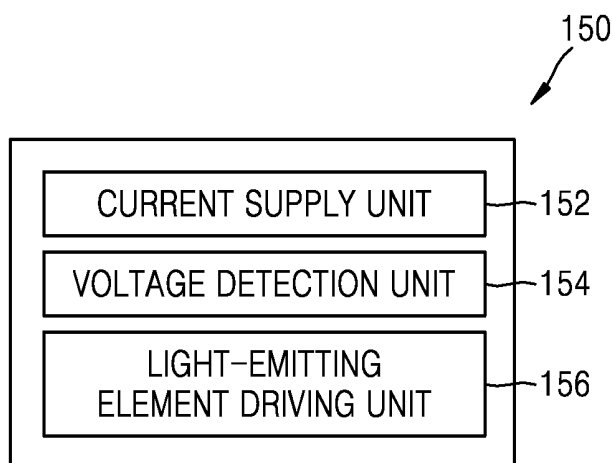


FIG. 7

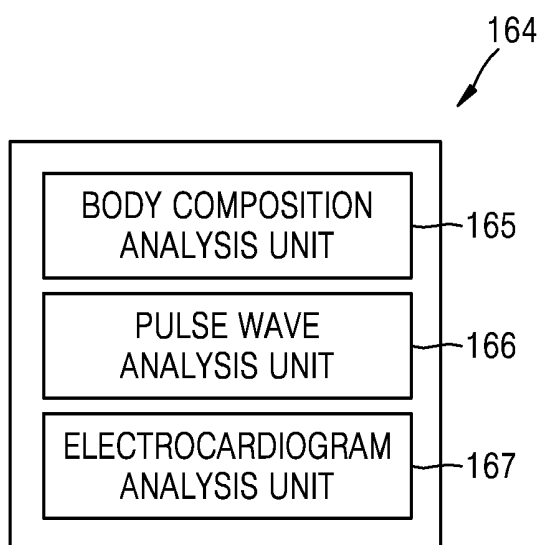


FIG. 8

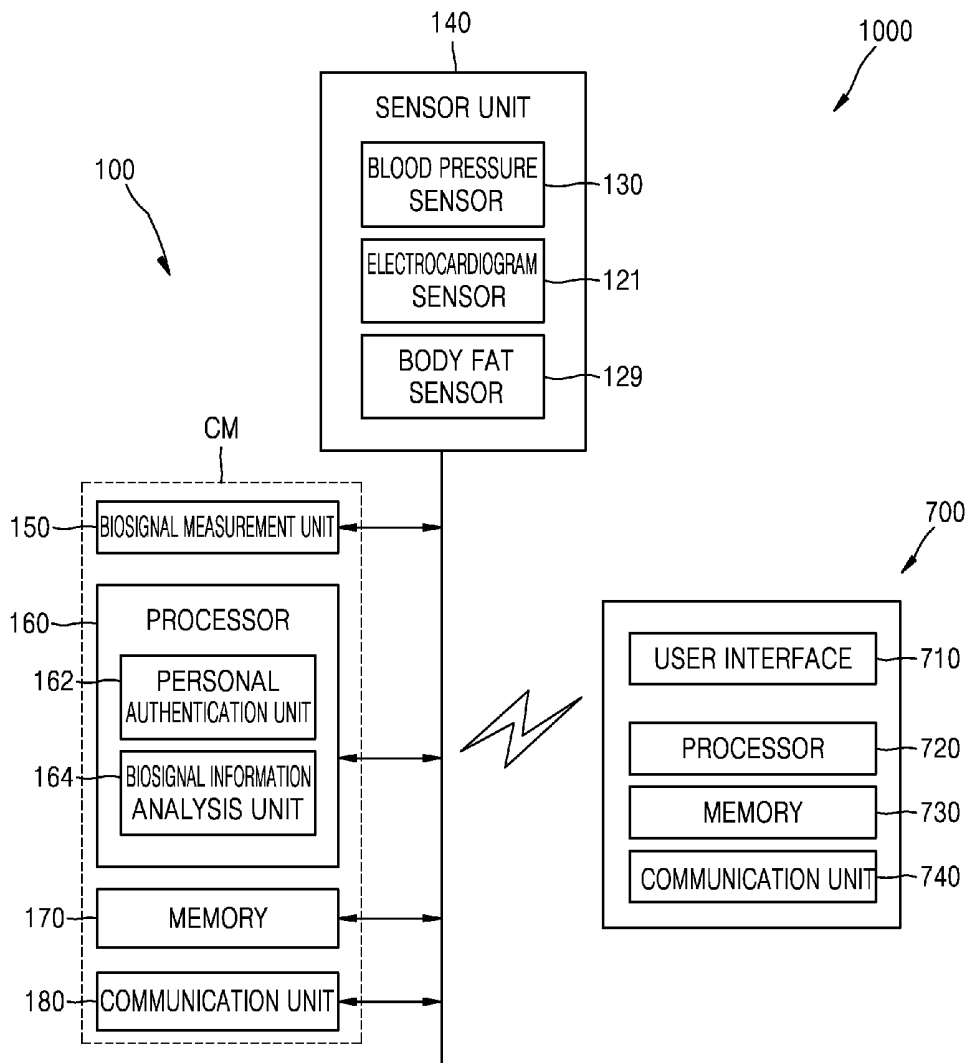


FIG. 9

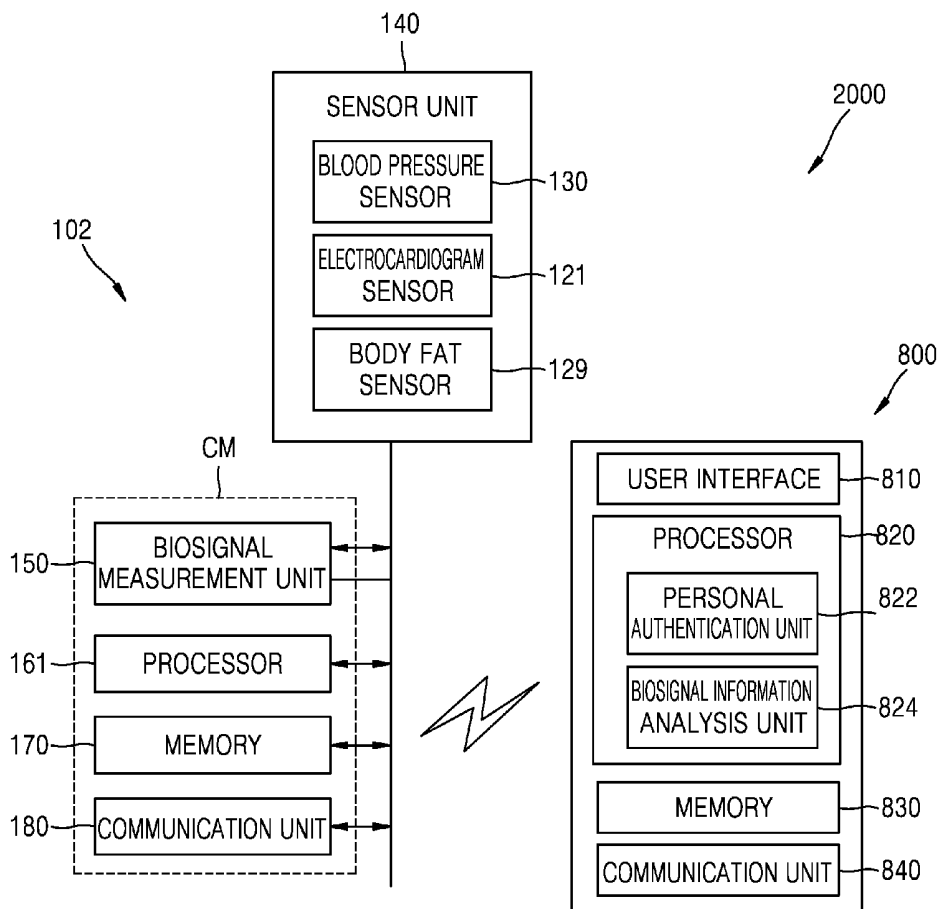


FIG. 10

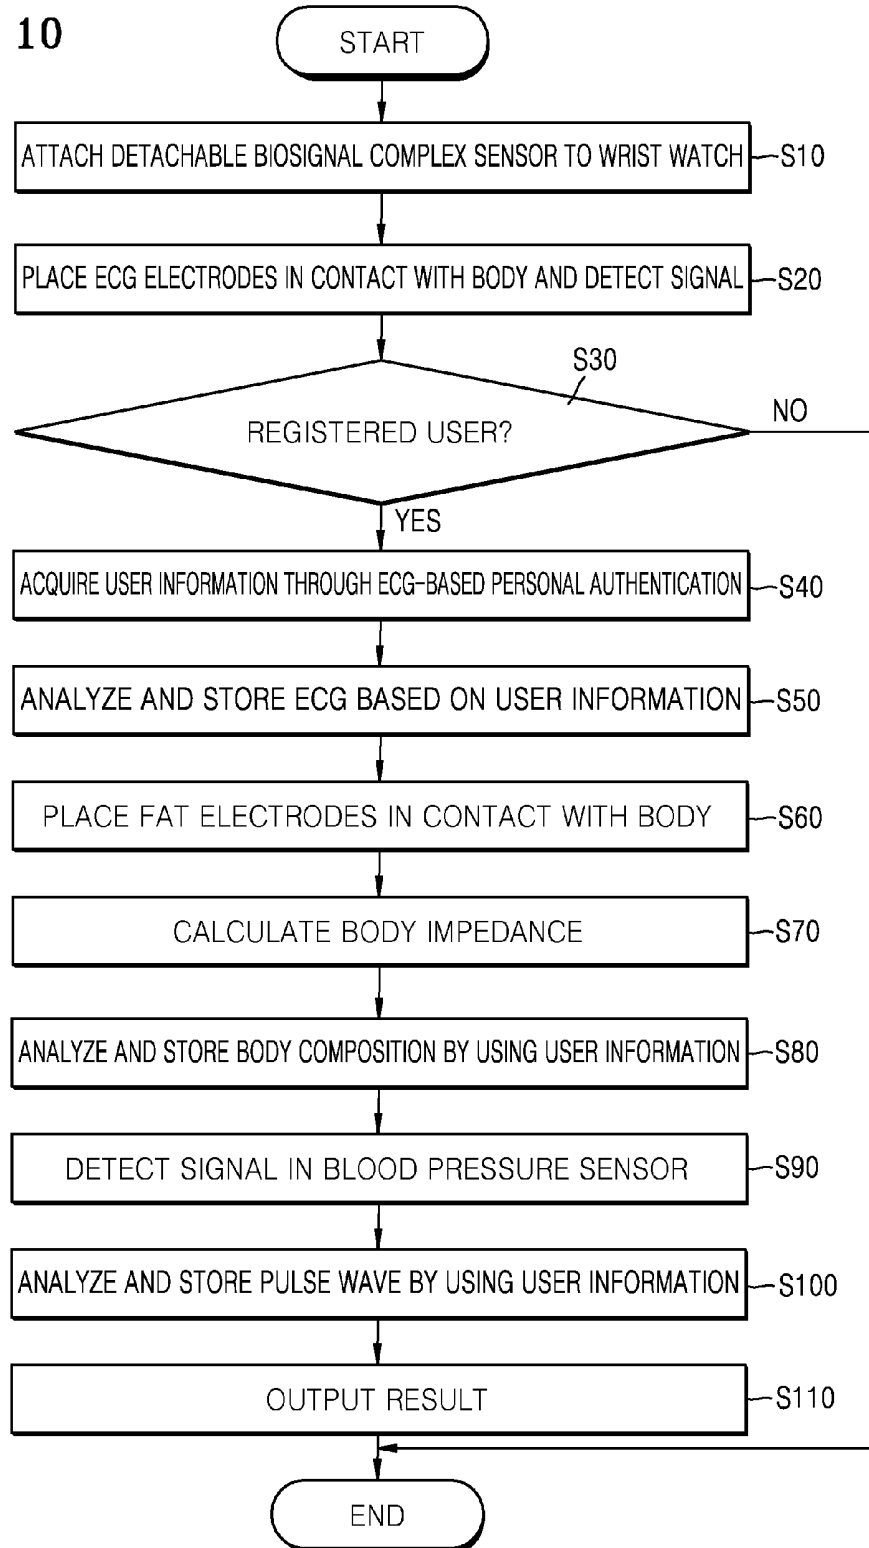


FIG. 11

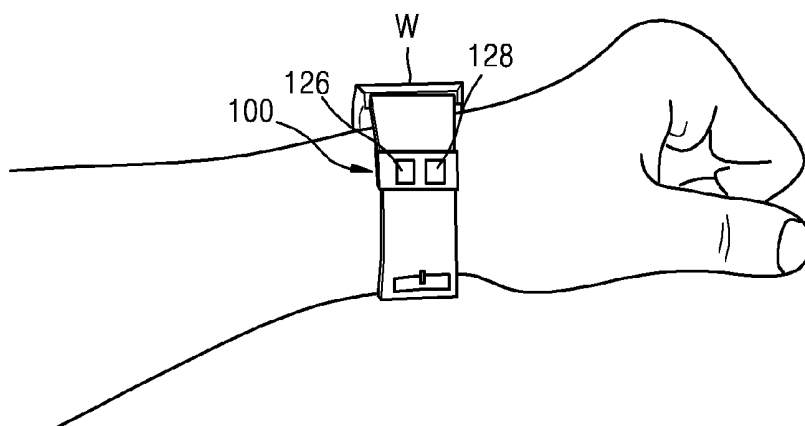


FIG. 12

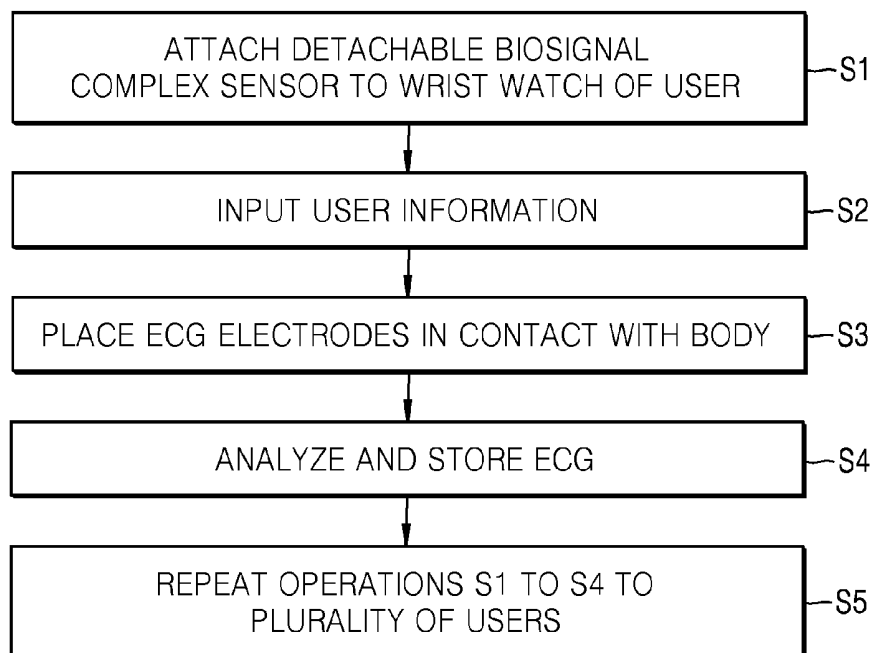


FIG. 13

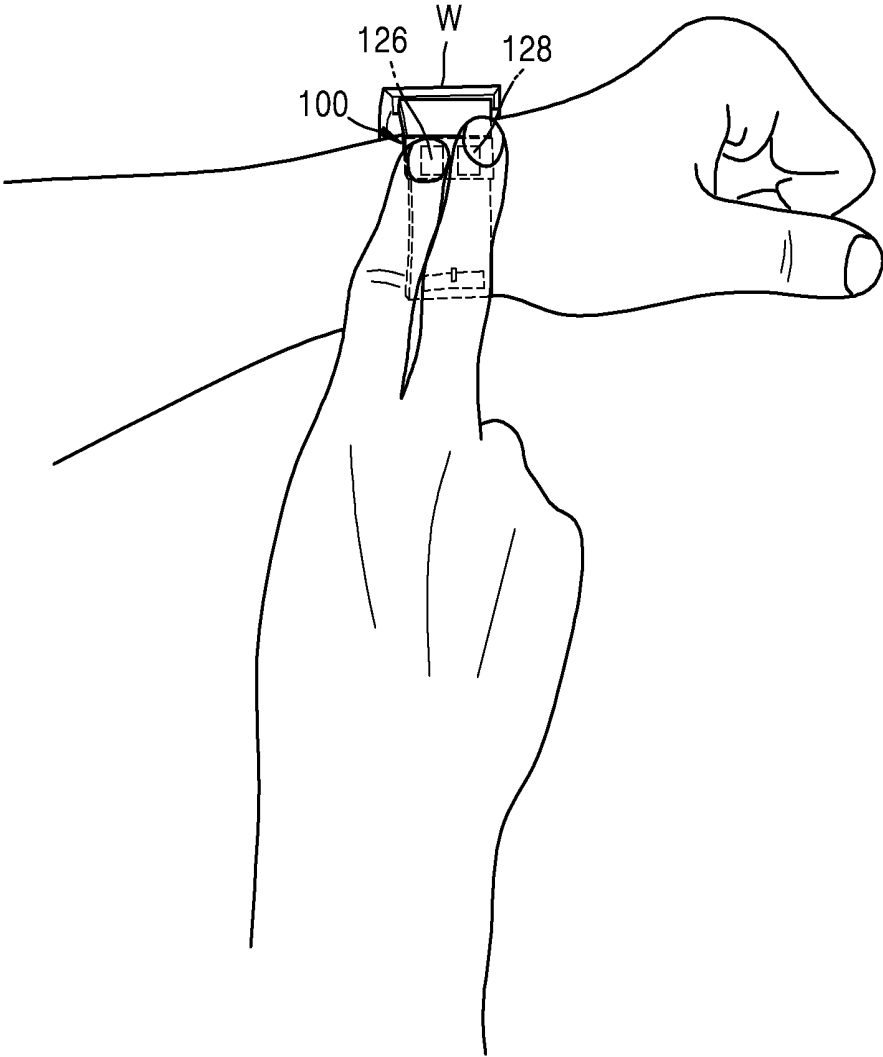


FIG. 14

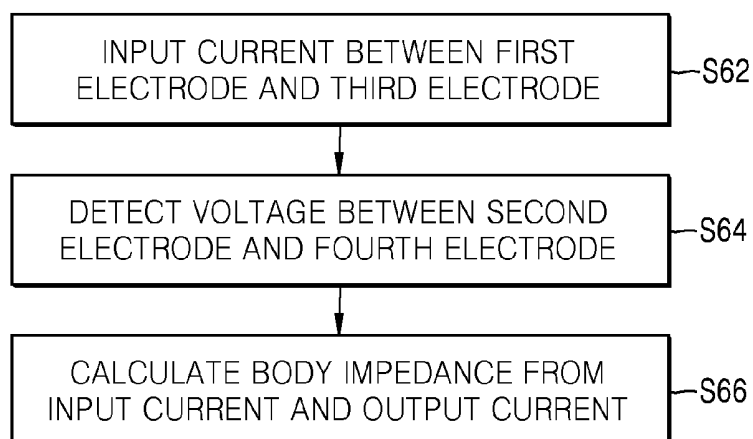


FIG. 15


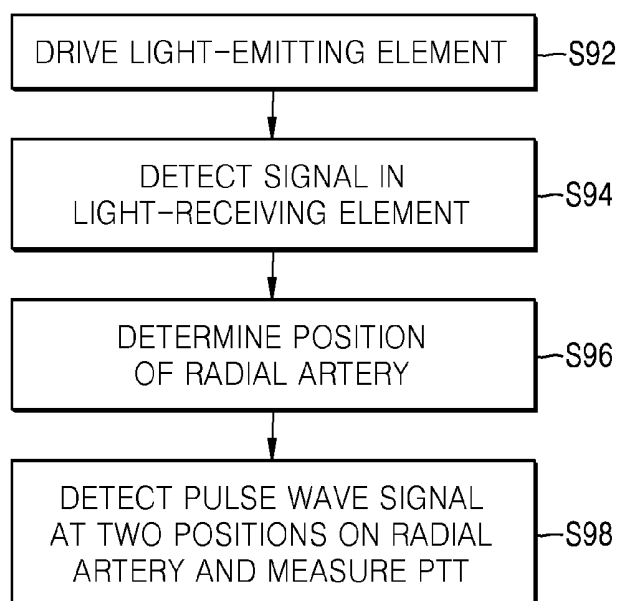


FIG. 16

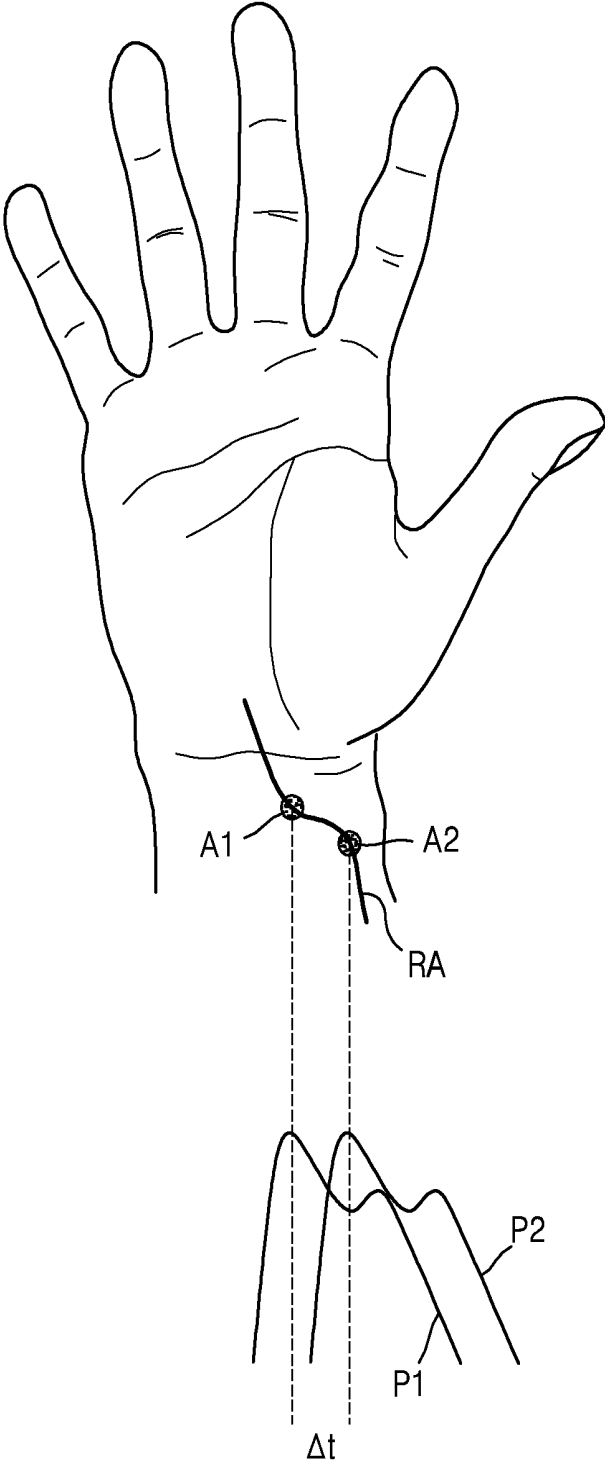

**DETACHABLE BIOSIGNAL COMPLEX
SENSOR AND METHOD OF DETECTING
BIOSIGNAL INFORMATION USING THE
SAME**

CROSS-REFERENCE TO RELATED
APPLICATION

[0001] This application claims the benefit of Korean Patent Application No. 10-2014-0139068, filed on Oct. 15, 2014, in the Korean Intellectual Property Office, the disclosure of which is incorporated herein in its entirety by reference.

BACKGROUND

[0002] 1. Field

[0003] The exemplary embodiments relate to detachable biosignal complex sensors and methods of detecting biosignal information using the same.

[0004] 2. Description of the Related Art

[0005] With the advances in medicine and increased lifespan of people, interest in health care has increased. Accordingly, interest in medical appliances has also increased. Examples of such medical appliances include various medical appliances used in hospitals or clinics, small- and medium-sized medical appliances installed in public institutions or the like, and small-sized medical appliances and health care devices that may be individually owned or used.

[0006] Regarding medical appliances or medical examinations, an invasive measurement method has been widely used. For example, when an invasive measurement method is used, a blood sample is collected from a subject and blood analysis is performed on the collected blood sample. However, such an invasive measurement method may be painful and inconvenient to use due to the need to employ a reagent that reacts with a specific substance in blood and a colorimetric assay and optical device.

SUMMARY

[0007] Exemplary embodiments may provide detachable biosignal complex sensors and methods of detecting biosignal information using the same.

[0008] Additional aspects will be set forth in part in the description which follows and, in part, will be apparent from the description, or may be learned by practice of the presented exemplary embodiments.

[0009] According to an aspect of an exemplary embodiment, there is provided a detachable biosignal complex sensor including: a clip type structure including a circuit module configured to receive a biosignal of a subject and perform signal processing on the biosignal, a first plate, and a second plate having an end thereof which is rotatably connected to an end of the first plate so that the clip type structure is configured to be fastened to an item; and a sensor and electrodes provided on outer surfaces of the first plate and the second plate and configured to obtain the biosignal and transmit the obtained biosignal to the circuit module.

[0010] The electrodes may include: a first electrode and a second electrode on the first plate; and a third electrode and a fourth electrode on the second plate.

[0011] The first electrode and the second electrode may be configured to function as an electrocardiogram sensor, and the first electrode, the second electrode, the third electrode, and the fourth electrode may be configured to function as a body fat sensor.

[0012] The sensor may be a blood pressure sensor provided on the first plate.

[0013] The blood pressure sensor may include a light-emitting element configured to emit light and a light-receiving element configured to receive light, wherein the biosignal is obtained based on the emitted and received light.

[0014] The blood pressure sensor may include a light-receiving element configured to receive light, and a first light-emitting element and a second light-emitting element which are respectively positioned on opposite sides of the light-receiving element and configured to emit light, wherein the biosignal is obtained based on the emitted and received light.

[0015] The first electrode and the second electrode may be spaced apart from each other in a first direction, and the first light-emitting element, the light-receiving element, and the second light-emitting element may be spaced apart from one another between the first electrode and the second electrode in a second direction perpendicular to the first direction.

[0016] The clip type structure may include a flexible material.

[0017] The detachable biosignal complex sensor may further include a pair of connection members respectively provided at other ends of the first plate and the second plate, the other ends being opposite to the ends at which the first plate and the second plate are connected.

[0018] The pair of connection members may include a magnet and magnetic material or male and female Velcro® parts.

[0019] The circuit module may include: a personal authenticator configured to perform personal authentication based on an electrocardiogram signal of the subject and thereby generate personal-authenticated user information; and a biosignal information analyzer configured to analyze biosignal information of the subject by using the personal-authenticated user information and the biosignal.

[0020] The detachable biosignal complex sensor may further include a communicator configured to output an analysis result of the biosignal information analyzer to an external device.

[0021] According to another exemplary embodiment, there is provided a biosignal information detection system including: any one of the above-described detachable biosignal complex sensors according to an exemplary embodiment; and an external electronic device including a user interface configured to receive an execution command which commands the detachable biosignal complex sensor to execute a process and outputs a command execution result of the process, and a communicator configured to communicate with the detachable biosignal complex sensor.

[0022] The circuit module of the detachable biosignal complex sensor may include: a personal authenticator configured to perform personal authentication based on an electrocardiogram signal of the subject and thereby generate personal-authenticated user information; and a biosignal information analyzer configured to analyze biosignal information of the subject by using personal-authenticated user information and the biosignal.

[0023] The external electronic device may include: a personal authenticator configured to perform personal authentication based on an electrocardiogram signal of the subject and thereby generate personal-authenticated user information; and a biosignal information analyzer configured to analyze biosignal information of the subject by using the personal-authenticated user information and the biosignal.

[0024] According to another exemplary embodiment, there is provided a method of detecting a biosignal including: attaching one of the above-described detachable biosignal complex sensors according to an exemplary embodiment to an item of a subject; performing personal authentication to determine whether the subject is a registered user of the detachable biosignal complex sensor; and acquiring the biosignal from the subject through the sensor and the electrodes, and analyzing biosignal information of the subject based on the acquired biosignal, according to whether the personal authentication indicates that the subject is the registered user.

[0025] The item includes a wrist watch.

[0026] The electrodes may include a first electrode, a second electrode, a third electrode, and a fourth electrode. The first electrode and the second electrode may be configured to detect an electrocardiogram signal. The first electrode, the second electrode, the third electrode, and the fourth may be configured to detect body fat.

[0027] The performing of the personal authentication may include using the electrocardiogram signal detected by the first electrode and the second electrode to determine whether the subject is the registered user.

[0028] The biosignal information may include one of a body composition, an electrocardiogram, a vascular compliance, a blood flow rate, arterial stiffness, a systolic blood pressure, or a diastolic blood pressure.

BRIEF DESCRIPTION OF THE DRAWINGS

[0029] These and/or other aspects will become apparent and more readily appreciated from the following description of the exemplary embodiments, taken in conjunction with the accompanying drawings in which:

[0030] FIGS. 1A and 1B are cross-sectional views of a detachable biosignal complex sensor according to an exemplary embodiment;

[0031] FIGS. 2A and 2B are plan views, respectively, illustrating a first plate and a second plate in a detachable biosignal complex sensor according to an exemplary embodiment;

[0032] FIGS. 3A and 3B are perspective views, respectively, illustrating an inner side and an outer side of a strap of a wrist watch as an example in which a detachable biosignal complex sensor according to an exemplary embodiment is attached to the wrist watch;

[0033] FIGS. 4A and 4B are cross-sectional views of a detachable biosignal complex sensor according to another exemplary embodiment;

[0034] FIG. 5 is a block diagram of a detachable biosignal complex sensor according to an exemplary embodiment;

[0035] FIG. 6 is a block diagram of a biosignal measurement unit of FIG. 5;

[0036] FIG. 7 is a block diagram of a biosignal information analysis unit of FIG. 5;

[0037] FIG. 8 is a block diagram of a biosignal information detection system according to an exemplary embodiment;

[0038] FIG. 9 is a block diagram of a biosignal information detection system according to another exemplary embodiment;

[0039] FIG. 10 is a flowchart of a method of detecting biosignal information by using a detachable biosignal complex sensor, according to an exemplary embodiment;

[0040] FIG. 11 is a diagram illustrating a case where a user wears a wrist watch to which a detachable biosignal complex sensor is attached;

[0041] FIG. 12 is a flowchart of a process of registering a user in a detachable biosignal complex sensor;

[0042] FIG. 13 is a diagram illustrating a case where a user who wears a wrist watch to which a detachable biosignal complex sensor is attached contacts a plurality of electrodes so as to analyze his or her body fat;

[0043] FIG. 14 is a flowchart of a process of analyzing body fat by using a body fat sensor in a detachable biosignal complex sensor;

[0044] FIG. 15 is a flowchart of a process of analyzing biosignal information by using a blood pressure sensor in a detachable biosignal complex sensor; and

[0045] FIG. 16 is a conceptual diagram of a method of analyzing a pulse wave signal in the flowchart of FIG. 15.

DETAILED DESCRIPTION

[0046] Reference will now be made in detail to exemplary embodiments, examples of which are illustrated in the accompanying drawings, wherein like reference numerals refer to like elements throughout. In this regard, the present exemplary embodiments may have different forms and should not be construed as being limited to the descriptions set forth herein. Accordingly, the exemplary embodiments are merely described below, by referring to the figures, to explain aspects of the exemplary embodiments. As used herein, the term “and/or” includes any and all combinations of one or more of the associated listed items.

[0047] It will be understood that when a layer, region, or component is referred to as being “formed on,” another layer, region, or component, the layer, region, or component can be directly or indirectly formed on the other layer, region, or component. That is, for example, intervening layers, regions, or components may be present.

[0048] It will be understood that, although the terms “first”, “second”, etc., may be used herein to describe various elements, these elements should not be limited by these terms. These terms are only used to distinguish one element from another.

[0049] The terminology used herein is for the purpose of describing particular exemplary embodiments only and is not intended to be limiting of the exemplary embodiments. As used herein, the singular forms “a”, “an”, and “the” are intended to include the plural forms as well, unless the context clearly indicates otherwise.

[0050] In addition, the terms “unit” and “module” may refer to a unit configured to process at least one function or operation and the “unit” and “module” may be implemented by hardware, software, or a combination thereof.

[0051] FIGS. 1A and 1B are cross-sectional views of a detachable biosignal complex sensor 100 according to an exemplary embodiment. Specifically, FIG. 1A illustrates a case where a clip type structure 110 is opened, and FIG. 1B illustrates a case where the clip type structure 110 is attached to a strap ST. FIGS. 2A and 2B are plan views, respectively, illustrating a first plate 112 and a second plate 114 in the detachable biosignal complex sensor 100 according to the exemplary embodiment.

[0052] The detachable biosignal complex sensor 100 may sense a biosignal from a subject and analyze biosignal information by using the sensed biosignal.

[0053] According to an exemplary embodiment, the term subject refers to an object from which biosignal information is to be detected. The subject may be a living body portion that can come in contact with the detachable biosignal complex

sensor **100** or be placed adjacent to the detachable biosignal complex sensor **100**. For example, the subject may be a living body portion from which a pulse wave or body fat is easily measured through photoplethysmography (PPG). For example, the subject may be a surface of a wrist. However, the subject is not limited thereto.

[0054] The biosignal information is unique information of the subject. For example, the biosignal information may be a signal based on a movement of a specific object (for example, a heart or a muscle) of the subject, such as an electrocardiogram (ECG), a ballistocardiogram (BCG), a photoplethysmograph (PPG), or an electromyogram (EMG), the biosignal information may be a blood pressure, and the biosignal information may be information on an amount of materials included in the subject, for example, a blood sugar, a cholesterol, and body fat.

[0055] Also, in the following exemplary description, a "user" may be a subject from which biosignal information is to be measured, but the user may also be a medical expert capable of using the detachable biosignal complex sensor **100**. That is, the term "user" according to an exemplary embodiment may refer to many types of people in addition to the subject.

[0056] Referring to FIGS. 1A and 1B, the detachable biosignal complex sensor **100** may include a clip type structure **110**, a blood pressure sensor **130** disposed on an outer surface of the clip type structure **110**, and a plurality of electrodes **122**, **124**, **126**, and **128**.

[0057] The clip type structure **110** may include a built-in circuit module (CM) that senses a biosignal from a subject and performs signal processing on the sensed biosignal. The clip type structure **110** may include a first plate **112** and a second plate **114**. One end of the first plate **112** and one end of the second plate **114** are rotatably connected together to form a pair of claws. Thus, items (e.g., straps, clothing, etc.) placed between the first plate **112** and second plate **114** may be caught between the first plate **112** and the second plate **114** when the first and second plates **114** are rotated in such a way to close the first and second plates **112** and **114** on the item.

[0058] As illustrated in FIG. 1A, a gap between the first plate **112** and the second plate **114** of the clip type structure **110** may be opened. Also, as illustrated in FIG. 1B, a gap between the first plate **112** and the second plate **114** of the clip type structure **110** may be closed with a strap **ST** disposed therebetween. The strap **ST** may be a watch strap of a wrist watch, a belt, or a waist portion of pants.

[0059] The first plate **112** and the second plate **114** may be made of a plastic material, a flexible polymer material, or a stretchable polymer material. For example, the first plate **112** and the second plate **114** may be made of a material selected from the group of poly(dimethylsiloxane)(PDMS), poly vinyl alcohol (PVA), polyurethane, polyurethane acrylate (PUA), poly(styrene-isoprene-styrene)(SIS), poly(styrene-butadiene-styrene)(SBS), poly(styrene-ethylene/butylene-styrene) (SEBS), polyvinylidene fluoride(PVDF), nitrile butadiene rubber(NBR), perfluoropolyether (PFPE), and polyester (PE).

[0060] Referring to FIG. 2A, the first electrode **122**, the second electrode **124**, and the blood pressure sensor **130** are disposed on the first plate **112**. Specifically, the first electrode **122**, the second electrode **124**, and the blood pressure sensor **130** are disposed on one surface of the first plate **112** that is the outer surface of the clip type structure **110**.

[0061] The first electrode **122** and the second electrode **124** may act as an ECG sensor. The ECG sensor **121** is configured to sense electrical activity of a heart. The ECG sensor **121** may detect a slight electrical signal that is sensed from a person's skin when myocardium is depolarized at every heartbeat. At the same time, the first electrode **122** and the second electrode **124** may also act as a part of a body fat sensor **129**.

[0062] The blood pressure sensor **130** may be disposed between the first electrode **122** and the second electrode **124**. The blood pressure sensor **130** may include light-emitting elements **131** and **133** and a light-receiving element **132**. Specifically, the blood pressure sensor **130** may include the light-receiving element **132**, and the first light-emitting element **131** and the second light-emitting element **133** disposed at opposite sides of the light-receiving element **132**. However, the number of the light-emitting elements and the light-receiving elements shown in FIG. 2A are merely exemplary. The blood pressure sensor **130** may include a single light-emitting element, or may include two or more light-emitting elements. In addition, the blood pressure sensor **130** may include a plurality of light-receiving elements.

[0063] The first electrode **122** and the second electrode **124** may be spaced apart from each other in a predetermined direction, and the first light-emitting element **131**, the light-receiving element **132**, and the second light-emitting element **133** may be spaced apart from one another in a direction perpendicular to the predetermined direction. However, such an arrangement is only for illustrative purposes and the exemplary embodiments are not limited thereto.

[0064] As the first and second light-emitting elements **131** and **133**, light-emitting diodes (LEDs) or laser diodes (LDs) may be used, although exemplary embodiments are not limited thereto. As the light-receiving element **132**, a photo diode (PD), a photo transistor (PTr), or a charge-coupled device (CCD) may be used, although exemplary embodiments are not limited thereto.

[0065] The first and second light-emitting elements **131** and **133** may irradiate light on the subject, and the light-receiving element **132** may sense an optical signal that is scattered or reflected from the subject. The sensed optical signal may be used for pulse wave analysis, and a variety of biosignal information may be analyzed from the sensed optical signal.

[0066] Referring to FIG. 2B, the third electrode **126** and the fourth electrode **128** are disposed on the second plate **114**. Specifically, the third electrode **126** and the fourth electrode **128** may be disposed on one surface of the second plate **114** that is the outer surface of the clip type structure **110**.

[0067] The third electrode **126** and the fourth electrode **128**, together with the first electrode **122** and the second electrode **124**, may constitute a body fat sensor. The body fat sensor may measure body fat based on bioelectrical impedance analysis (BIA). BIA is a method of calculating a ratio of body fat content and body water content by using a difference in electrical resistance between non-fat tissue and fat tissue when an AC wave having low energy passes through a body. That is, BIA allows current to flow through the body by taking into account that the body is a combination of impedances, measures a voltage through the current, and measures the impedance of the body based on the current and the voltage. In this manner, BIA may analyze body composition. The plurality of electrodes **122**, **124**, **126**, and **128** come into contact with the subject. Of the plurality of electrodes **122**,

124, **126**, and **128**, the two electrodes, for example, the first and third electrodes **122** and **126**, may serve as input electrodes for the input of the current, and the remaining electrodes, for example, the second and fourth electrodes **124** and **128**, may serve as output electrodes for the detection of the voltage. However, this description is merely exemplary, and other electrodes among the plurality of electrodes **122**, **124**, **126** and **128** may function as the input electrodes and the output electrodes in various combinations.

[0068] FIGS. 3A and 3B are perspective views illustrating an example in which the detachable biosignal complex sensor **100** according to the exemplary embodiment is attached to a wrist watch W. Specifically, FIGS. 3A and 3B are perspective views, respectively, illustrating the inner surface and the outer surface of the strap ST of the wrist watch W.

[0069] Referring to FIG. 3A, the detachable biosignal complex sensor **100** is attached such that the first plate **112** is disposed on the inner surface of the strap ST of the wrist watch W. That is, the first and second electrodes **122** and **124**, which may serve as the ECG sensor and the body fat sensor, and the first and second light-emitting elements **131** and **133** and the light-receiving element **132**, which constitute the blood pressure sensor **130**, come into contact with the wrist of the user who wears the wrist watch W.

[0070] Referring to FIG. 3B, the detachable biosignal complex sensor **100** is attached such that the second plate **114** is disposed on the outer surface of the strap ST of the wrist watch W. The third and fourth electrodes **126** and **128**, which may serve as elements of the body fat sensor **129**, are exposed to the outside.

[0071] FIGS. 4A and 4B are cross-sectional views of a detachable biosignal complex sensor **101** according to another exemplary embodiment. Specifically, FIG. 4A illustrates a case where a clip type structure **110** is opened, and FIG. 4B illustrates a case where the clip type structure **110** is attached to a strap ST.

[0072] The detachable biosignal complex sensor **101** of FIGS. 4A and 4B differs from the detachable biosignal complex sensor **100** of FIGS. 1A and 1B in that a pair of connection members **116** and **117** are further provided at one end of a first plate **112** and one end of a second plate **114**, respectively. In the clip type structure **110**, the connection members **116** and **117** may be provided at the other ends opposite to the ends to which the first plate **112** and the second plate **114** are connected. The connection members **116** and **117** may serve to stably maintain a state in which the strap ST is disposed between the first plate **112** and the second plate **114**. Examples of the connection members **116** and **117** may include magnet and magnetic material, or male and female Velcro® parts (e.g., hooks and loops). However, the connection members **116** and **117** are not limited thereto and various type of connection members may be implemented.

[0073] FIG. 5 is a block diagram of the detachable biosignal complex sensor **100** according to the exemplary embodiment, FIG. 6 is a block diagram of a biosignal measurement unit **150** of FIG. 5, and FIG. 7 is a block diagram of a biosignal information analysis unit **164** of FIG. 5.

[0074] As described above, the blood pressure sensor **130**, the ECG sensor **121**, and the body fat sensor **129**, which constitute a sensor unit **140** (e.g., sensor) of the detachable biosignal complex sensor **100**, are exposed to the outer surface of the clip type structure **110**.

[0075] The blood pressure sensor **130** may include a light-emitting element and a light-receiving element. The blood

pressure sensor **130** may irradiate light on the subject and sense an optical signal that is reflected or scattered from the subject. For example, the blood pressure sensor **130** may detect a laser speckle that is generated by scattering of a laser beam irradiated on the subject. According to an exemplary embodiment, the term laser speckle refers to irregular patterns that are generated by interference or scattering when a coherent laser beam is irradiated on a scattering body. The blood pressure sensor may detect an optical signal corresponding to laser speckle.

[0076] The ECG sensor **121** is configured to sense electrical activity of a heart. The ECG sensor **121** may detect a slight electrical signal that is sensed from a skin when myocardium is depolarized at every heartbeat.

[0077] The body fat sensor **129** may apply current to the subject and detect an output voltage from the subject.

[0078] A circuit module CM, which senses a biosignal from the subject and performs signal processing on the sensed biosignal, may be embedded in a first plate **112** and a second plate **114**, which constitutes the clip type structure **110**.

[0079] The circuit module CM may include a biosignal measurement unit **150** (e.g., biosignal measurer) that provides the sensor unit **140** with an input for sensing a biosignal and performs measurement on an output of the sensor unit **140**, and a processor **160** that performs a variety of processing for biosignal analysis according to the measurement result. The processor **160** may include a personal authentication unit **162** (e.g., personal authenticator) that performs personal authentication based on a sensed ECG signal, and a biosignal information analysis unit **264** that analyzes biosignal information by using personal-authenticated user information and sensed biosignal. In addition, the circuit module CM may further include a memory **170** and a communication unit **180** (e.g., communicator).

[0080] As illustrated in FIG. 6, the biosignal measurement unit **150** may include a current supply unit **152** (e.g., current supplier), a voltage detection unit **154** (e.g., voltage detector), and a light-emitting element driving unit **156** (e.g., light-emitting element driver). The current supply unit **152** may supply current to an input electrode of the body fat sensor **129**. The voltage detection unit **154** may measure a voltage between output electrodes of the body fat sensor **129**. The light-emitting element driving unit **156** may apply a voltage for driving the light-emitting element of the blood pressure sensor **130**. In addition, the biosignal measurement unit **150** may further include an amplifier that amplifies an electrical signal detected by the ECG sensor **121**.

[0081] The personal authentication unit **162** may perform personal authentication based on a sensed ECG signal. Specifically, the personal authentication unit **162** may determine whether the subject is a registered user, based on the ECG signal sensed by the ECG sensor **121**. When it is determined that the subject is the registered user, the personal authentication unit **162** may transmit a control signal for driving the blood pressure sensor **130** or the body fat sensor **129** to the biosignal measurement unit **150**. In addition, when the biosignal is sensed by the sensor unit **140**, the personal authentication unit **162** may transmit a related signal to the biosignal information analysis unit **164** (e.g., biosignal information analyzer) so as to perform biosignal information analysis by using the registered user information. For this purpose, the personal authentication unit **162** may perform ECG signal measurement on the user who will use the detachable biosig-

nal complex sensor **100**, and input the measurement result and related user information to the memory **170** in advance.

[0082] The biosignal information analysis unit **164** may analyze biosignal information by using the signals sensed by the blood pressure sensor **130**, the ECG sensor **121**, and the body fat sensor **129**. As illustrated in FIG. 7, the biosignal information analysis unit **164** may include a body composition analysis unit **165** (e.g., body composition analyzer), a pulse wave analysis unit **166** (e.g., pulse wave analyzer), and an ECG analysis unit **167** (e.g., ECG analyzer).

[0083] The body composition analysis unit **165** may calculate body impedance based on the input current applied to the body fat sensor **129** and the detected output voltage, and analyze the body composition based on the calculated body impedance.

[0084] The pulse wave analysis unit **166** may detect a pulse wave signal by analyzing an optical signal sensed by the blood pressure sensor **130**, and calculate a variety of types of biosignal information from the detected pulse wave signal. Specifically, the pulse wave analysis unit **166** may analyze a change in the intensity of the optical signal detected by the light-receiving element of the blood pressure sensor **130** with respect to time. The pulse wave analysis unit **166** may acquire a biosignal by analyzing laser speckle fluctuation corresponding to a change in a volume of a blood vessel (for example, radial artery) of an object. The acquired biosignal may be a PPG signal converted based on a correlation between the analyzed speckle fluctuation and the volume change. The pulse wave analysis unit **166** may analyze various parameters included in a PPG pulse wave signal by analyzing wavelength characteristics of the PPG pulse wave signal. For example, the pulse wave analysis unit **166** may calculate a delay time between pulse wave signals and calculate a pulse transit time (PTT) from the calculated delay time. During this process, various digital signal processing algorithms, such as a noise removal algorithm or a differential signal extraction algorithm, may be used. The extracted pulse wave signal analysis result may be used as an index for analyzing a variety of biosignal information. That is, the biosignal information may be analyzed by using a predetermined algorithm configured to calculate a variety of biosignal information from analyzed PTT. For example, a vascular compliance, a blood flow rate, arterial stiffness, a systolic blood pressure, or a diastolic blood pressure may be estimated.

[0085] The ECG analysis unit **167** may analyze an ECG based on an electrical signal sensed by the ECG sensor **121**. A healthy heart has an orderly depolarization waveform that spreads over a ventricle from a signal output from a sinoatrial node. A waveform of a small voltage sensed by two electrodes shows an entire rhythm of a heart. From the waveform, a rate or a consistency of a heartbeat may be analyzed, and damage to a specific part of myocardium may be analyzed.

[0086] The memory **170** may store a program to control processing operations and other operations of the processor **160**, and may store input/output data. For example, a program for the personal authentication and the biosignal information analysis to be performed by the processor **160** may be stored in a code form. In addition, the memory **170** may store the measurement results of the sensor unit **140** and the user information, which may be used for processing operations by the processor **160**.

[0087] The memory **170** may include a storage medium selected from among a flash memory, a hard disk, a multimedia card micro type memory, a card type memory (for

example, SD or XD memory), a random access memory (RAM), a static random access memory (SRAM), a read-only memory (ROM), an electrically erasable programmable read-only memory (EEPROM), a programmable read-only memory (PROM), a magnetic memory, a magnetic disk, and an optical disk.

[0088] The communication unit **180** may transmit the analysis result to an external device by wire or wireless. The external device may be a medical device that uses the analyzed biosignal information, a printer that prints the results, or a display device that displays the analysis results. In addition, the communication unit **180** may be a smartphone, a mobile phone, a personal digital assistant (PDA), a laptop computer, a personal computer (PC), or other mobile or non-mobile computing devices, but is not limited thereto.

[0089] The communication unit **180** may be connected to the external device by wire or in a wireless fashion. For example, the communication unit **180** may communicate with the external device through a Bluetooth communication scheme, a Bluetooth Low Energy (BLE) communication scheme, a near field communication (NFC) scheme, a WLAN (WiFi) communication scheme, a Zigbee communication scheme, an infrared data association (IrDA) communication scheme, a Wi-Fi Direct (WFD) communication scheme, an Ultra WideBand (UWB) communication scheme, an Ant+ communication scheme, or a WiFi communication scheme, but is not limited thereto.

[0090] FIG. 8 is a block diagram of a biosignal information detection system **1000** according to an exemplary embodiment.

[0091] The biosignal information detection system **1000** may include a detachable biosignal complex sensor **100** and an external electronic device **700** capable of communicating with the detachable biosignal complex sensor **100**.

[0092] The external electronic device **700** may include a user interface **710** that receives an execution command for the detachable biosignal complex sensor **100** and outputs a command execution result, and a communication unit **740** (e.g., communicator) that communicates with the detachable biosignal complex sensor **100**. In addition, the external electronic device **700** may include a processor **720** and a memory **730**.

[0093] The external electronic device **700** may be a wrist watch type device as illustrated in FIG. 3A, or may be a smartphone, a mobile phone, a PDA, a laptop computer, a PC, or other mobile or non-mobile computing devices, but exemplary embodiments are not limited thereto.

[0094] FIG. 9 is a block diagram of a biosignal information detection system **2000** according to another exemplary embodiment.

[0095] The biosignal information detection system **2000** according to the present exemplary embodiment may include a detachable biosignal complex sensor **102** and an external electronic device **800**. The biosignal information detection system **2000** differs from the biosignal information detection system **1000** of FIG. 8 in that the functions performed by a personal authentication unit **822** and a biosignal information analysis unit **824** are performed in the external electronic device **800**.

[0096] The detachable biosignal complex sensor **102** may include a sensor unit **140**, a biosignal measurement unit **150**, a processor **161**, a memory **170**, and a communication unit **180**.

[0097] The external electronic device **800** may include a user interface **810** that receives an execution command for the detachable biosignal complex sensor **102** and outputs a command execution result, a processor **820** including a personal authentication unit **822** and a biosignal information analysis unit **824**, a memory **830**, and a communication unit **840**.

[0098] The appearances and/or the functions of the detachable biosignal complex sensors **100**, **101**, and **102** have been described with reference to the block diagrams and may be mutually combined.

[0099] FIG. **10** is a flowchart of a method of detecting biosignal information by using a detachable biosignal complex sensor, according to an exemplary embodiment.

[0100] The method of detecting the biosignal information according to the exemplary embodiment may be performed by the above-described detachable biosignal complex sensor or the biosignal information detection system including the same.

[0101] Referring to FIG. **10**, in operation **S10**, the detachable biosignal complex sensor is attached to a wrist watch. The wrist watch, to which the detachable biosignal complex sensor is attached, may be worn by a user, that is, a subject.

[0102] FIG. **11** is a diagram illustrating a case where the user wears the wrist watch **W** to which the detachable biosignal complex sensor **100** is attached.

[0103] In operation **S20**, when the user wears the wrist watch **W**, the ECG sensor **121** of the detachable biosignal complex sensor **100** contacts a body of the subject, and an ECG signal is sensed by the ECG sensor **121**.

[0104] In operation **S30**, when the ECG signal is sensed, it is determined whether the subject is a registered user. In operation **S40**, when it is determined that the subject is not the registered user, the process is ended, and when it is determined that the subject is the registered user, user information is acquired through personal authentication based on ECG.

[0105] In order to acquire such personal authentication, a user may previously store information about the user who will use the detachable biosignal complex sensor **100**.

[0106] FIG. **12** is a flowchart of a process of registering a user in a detachable biosignal complex sensor.

[0107] In operation **S2**, the detachable biosignal complex sensor is attached to the wrist watch **W**, and the user information is input. The user refers to a subject from which biosignal information is to be measured. The user information may be weight, age, and gender of the subject.

[0108] In operation **S3**, the body of the subject contacts the ECG sensor. For example, the body of the subject may contact the ECG electrodes in such a manner that the subject wears the wrist watch **W** to which the detachable biosignal complex sensor is attached.

[0109] In operation **S4**, a signal from the ECG electrodes is analyzed and the analysis result is stored.

[0110] In operation **S5**, operations **S1** to **S4** may be repeated for a plurality of users.

[0111] Returning to FIG. **10**, in operation **S50**, after the user information is acquired, ECG analysis is performed and the ECG analysis result is stored.

[0112] In operations **S60** and **S70**, the body of the subject contacts the body fat electrodes, and body impedance is calculated.

[0113] FIG. **13** is a diagram illustrating a case where the user who wears the wrist watch **W** to which the detachable biosignal complex sensor **100** is attached contacts a plurality

of electrodes so as to analyze his or her body fat, and FIG. **14** is a flowchart of a process of analyzing the body fat by using the body fat sensor.

[0114] As illustrated in FIG. **13**, two fingers of the user may contact the third and fourth electrodes **126** and **128**. The body part contacting the third and fourth electrodes **126** and **128** is merely exemplary, and is not limited to the above example of two fingers.

[0115] In operations **S62** and **S64**, in a state in which the first and second electrodes **122** and **124** come into contact with the wrist of the user and the third and fourth electrodes **126** and **128** come into contact with the fingers of the user, current is input between the first electrode **122** and the third electrode **126**, and a voltage between the second electrode **124** and the fourth electrode **128** is detected. In operation **S66**, body impedance is calculated from the input current and the output voltage.

[0116] The first and third electrodes **122** and **126** may serve as input electrodes for the input of the current, and the second and fourth electrodes **124** and **128** may serve as output electrodes for the detection of the voltage, but the electrodes **122**, **124**, **126**, and **128** are not limited thereto. The input electrodes and the output electrodes may be set as another combination.

[0117] In operation **S80**, when the body impedance is calculated, the body composition may be analyzed using the user information and the analysis result may be stored. The body composition may include, for example, body fat, body water, muscle strength, or edema.

[0118] In operations **S90** and **S100**, a signal from the blood pressure sensor is detected and a pulse wave is analyzed from the detected signal. In addition, in this operation, a variety of biosignal information may be analyzed using the pulse wave.

[0119] FIG. **15** is a flowchart of a process of analyzing biosignal information by using the blood pressure sensor, and FIG. **16** is a conceptual diagram of a method of analyzing a pulse wave signal in the flowchart of FIG. **15**.

[0120] In operation **S92**, the light-emitting element of the blood pressure sensor is driven to irradiate light on the subject. In operation **S94**, an optical signal reflected or scattered from the subject is detected in the light-receiving element.

[0121] In operation **S96**, a position of a radial artery is determined. When a pulse wave is measured on a skin surface of the wrist, through which a radial artery passes, the influence of external factors causing an occurrence of measurement error in a thickness of a skin tissue inside the wrist may be reduced. It is known that the radial artery is a blood vessel at which a blood pressure can be measured more accurately than other types of blood vessels inside the wrist. Generally, since the position of the radial artery of the subject can be empirically estimated in advance, an exemplary embodiment may make it possible to perform a more accurate position control from the biosignal sensed by the light-receiving element of the blood pressure sensor.

[0122] In operation **S98**, pulse signals are detected at two positions on the radial artery and a PTT is measured. As illustrated in FIG. **16**, a time delay Δt is analyzed by comparing waveforms of two pulse signals **P1** and **P2** detected at two positions **A1** and **A2** on a radial artery **RA**. The time delay Δt is a parameter related to PTT information, and the PTT may be analyzed from the time delay Δt .

[0123] A variety of biosignal information may be analyzed using the analyzed pulse wave signal waveforms, the PTT information, or the like. The biosignal information may include a vascular compliance, a blood flow rate, arterial

stiffness, a systolic blood pressure, or a diastolic blood pressure. In addition, the biosignal information may include information regarding whether a current blood pressure state is normal or abnormal.

[0124] In the above description of certain exemplary embodiments, the order of the ECG analysis, the body composition analysis, and the pulse wave analysis is merely exemplary, and is not limited thereto. That is, the above-described order may be reversed, or certain operations or features may be omitted according to various criteria. In addition, the case where the detachable biosignal complex sensor is attached to the wrist watch and is worn on a wrist of a user has been described above, but the exemplary embodiments are not limited thereto. For example, the detachable biosignal complex sensor may be detachably attached to various wearable devices.

[0125] Since the detachable biosignal complex sensor according to exemplary embodiments may be attached to the wrist watch or the like only when the detachable biosignal complex sensor is being used, users do not have to experience the inconvenience of having to wear the biosignal sensor even when unnecessary.

[0126] In addition, the detachable biosignal complex sensor according to exemplary embodiments may have the personal authentication function. It is possible to measure biosignals of a plurality of users and analyze biosignal information thereof by using the personal authentication function.

[0127] It should be understood that the exemplary embodiments described therein should be considered in a descriptive sense only and not for purposes of limitation. Descriptions of features or aspects within each exemplary embodiment should typically be considered as available for other similar features or aspects in other exemplary embodiments.

[0128] While one or more exemplary embodiments have been described with reference to the figures, it will be understood by those of ordinary skill in the art that various changes in form and details may be made therein without departing from the spirit and scope as defined by the following claims.

What is claimed is:

1. A detachable biosignal complex sensor comprising:
 - a clip type structure comprising:
 - a circuit module configured to receive a biosignal of a subject and perform signal processing on the biosignal,
 - a first plate, and
 - a second plate having an end thereof which is rotatably connected to an end of the first plate so that the clip type structure is configured to be fastened to an item; and
 - a sensor and electrodes provided on outer surfaces of the first plate and the second plate and configured to obtain the biosignal and transmit the obtained biosignal to the circuit module.
2. The detachable biosignal complex sensor of claim 1, wherein the electrodes include:
 - a first electrode and a second electrode on the first plate; and
 - a third electrode and a fourth electrode on the second plate.
3. The detachable biosignal complex sensor of claim 2, wherein
 - the first electrode and the second electrode are configured to function as an electrocardiogram sensor, and

- the first electrode, the second electrode, the third electrode, and the fourth electrode are configured to function as a body fat sensor.

4. The detachable biosignal complex sensor of claim 3, wherein the sensor comprises a blood pressure sensor provided on the first plate.

5. The detachable biosignal complex sensor of claim 4, wherein the blood pressure sensor comprises a light-emitting element configured to emit light and a light-receiving element configured to receive light, wherein the biosignal is obtained based on the emitted and received light.

6. The detachable biosignal complex sensor of claim 4, wherein the blood pressure sensor comprises a light-receiving element configured to receive light, and a first light-emitting element and a second light-emitting element which are respectively positioned on opposite sides of the light-emitting element and configured to emit light, wherein the biosignal is obtained based on the emitted and received light.

7. The detachable biosignal complex sensor of claim 6, wherein

- the first electrode and the second electrode are spaced apart from each other in a first direction, and

- the first light-emitting element, the light-receiving element, and the second light-emitting element are spaced apart from one another between the first electrode and the second electrode in a second direction perpendicular to the first direction.

8. The detachable biosignal complex sensor of claim 1, wherein the clip type structure comprises a flexible material.

9. The detachable biosignal complex sensor of claim 1, further comprising a pair of connection members respectively provided at other ends of the first plate and the second plate, the other ends being opposite to the ends at which the first plate and the second plate are connected.

10. The detachable biosignal complex sensor of claim 9, wherein the pair of connection members comprise a magnet and magnetic material or male and female Velcro® parts.

11. The detachable biosignal complex sensor of claim 1, wherein the circuit module comprises:

- a personal authenticator configured to perform personal authentication based on an electrocardiogram signal of the subject and thereby generate personal-authenticated user information; and

- a biosignal information analyzer configured to analyze biosignal information of the subject by using the personal-authenticated user information and the biosignal.

12. The detachable biosignal complex sensor of claim 11, further comprising a communicator configured to output an analysis result of the biosignal information analyzer to an external device.

13. A biosignal information detection system comprising: a detachable biosignal complex sensor comprising:

- a clip type structure comprising:

- a circuit module configured to receive a biosignal of a subject and perform signal processing on the biosignal,

- a first plate, and

- a second plate having an end thereof which is rotatably connected to an end of the first plate so that the clip type structure is configured to be fastened to an item; and

- a sensor and electrodes provided on outer surfaces of the first plate and the second plate and configured to obtain the biosignal; and

an external electronic device comprising a user interface configured to receive an execution command which commands the detachable biosignal complex sensor to execute a process and outputs a command execution result of the process, and a communicator configured to communicate with the detachable biosignal complex sensor.

14. The biosignal information detection system of claim **13**, wherein the circuit module of the detachable biosignal complex sensor comprises:

a personal authenticator configured to perform personal authentication based on an electrocardiogram signal of the subject and thereby generate personal-authenticated user information; and

a biosignal information analyzer configured to analyze biosignal information of the subject by using personal-authenticated user information and the biosignal.

15. The biosignal information detection system of claim **13**, wherein the external electronic device comprises:

a personal authenticator configured to perform personal authentication based on an electrocardiogram signal of the subject and thereby generate personal-authenticated user information; and

a biosignal information analyzer configured to analyze biosignal information of the subject by using the personal-authenticated user information and the biosignal.

16. A method of detecting a biosignal, comprising:

attaching a detachable biosignal complex sensor to an item of a subject, the detachable biosignal complex sensor comprising a clip type structure comprising: a circuit module configured to receive a biosignal of the subject and perform signal processing on the biosignal, a first plate, and a second plate having an end thereof which is rotatably

connected to an end of the first plate so that the clip type structure is configured to be fastened to the item, and a sensor and electrodes provided on outer surfaces of the first plate and the second plate and configured to obtain the biosignal;

performing personal authentication to determine whether the subject is a registered user of the detachable biosignal complex sensor; and

acquiring the biosignal from the subject through the sensor and the electrodes, and analyzing biosignal information of the subject based on the acquired biosignal, according to whether the personal authentication indicates that the subject is the registered user.

17. The method of claim **16**, wherein the item comprises a wrist watch.

18. The method of claim **16**, wherein

the electrodes comprise a first electrode, a second electrode, a third electrode, and a fourth electrode, the first electrode and the second electrode are configured to detect an electrocardiogram signal, and the first electrode, the second electrode, the third electrode, and the fourth are configured to detect body fat.

19. The method of claim **18**, wherein the performing of the personal authentication comprises using the electrocardiogram signal detected by the first electrode and the second electrode to determine whether the subject is the registered user.

20. The method of claim **16**, wherein the biosignal information comprises one of a body composition, an electrocardiogram, a vascular compliance, a blood flow rate, arterial stiffness, a systolic blood pressure, or a diastolic blood pressure.

* * * * *

专利名称(译)	可拆卸的生物信号复合传感器和使用该传感器检测生物信号信息的方法		
公开(公告)号	US20160106333A1	公开(公告)日	2016-04-21
申请号	US14/804518	申请日	2015-07-21
[标]申请(专利权)人(译)	三星电子株式会社		
申请(专利权)人(译)	SAMSUNG ELECTRONICS CO. , LTD.		
当前申请(专利权)人(译)	SAMSUNG ELECTRONICS CO. , LTD.		
[标]发明人	KANG JAEMIN KWON YONGJOO KIM SUNKWON KIM YOUNHO PARK SANGYUN		
发明人	KANG, JAEMIN KWON, YONGJOO KIM, SUNKWON KIM, YOUNHO PARK, SANGYUN		
IPC分类号	A61B5/0408 A61B5/117 A61B5/02 A61B5/026 A61B5/00 A61B5/0205		
CPC分类号	A61B5/04085 A61B5/681 A61B5/0205 A61B5/0082 A61B5/021 A61B5/026 A61B5/117 A61B5/0537 A61B5/02007 A61B5/0059 A61B5/0285 A61B5/14551		
优先权	1020140139068 2014-10-15 KR		
其他公开文献	US10617316		
外部链接	Espacenet USPTO		

摘要(译)

一种可拆卸的生物信号复合传感器，包括：夹式结构，包括：电路模块，被配置为接收对象的生物信号并对生物信号进行信号处理，第一板和第二板，其一端可旋转地连接到一端第一板的一部分，使夹子式结构固定在物品上；传感器和电极设置在第一板和第二板的外表面上，并配置成获得生物信号并将获得的生物信号传输到电路模块。

