



US010271749B2

(12) **United States Patent**
Kiani

(10) **Patent No.:** **US 10,271,749 B2**
(45) **Date of Patent:** **Apr. 30, 2019**

- (54) **PATIENT MONITOR FOR MONITORING MICROCIRCULATION**
- (71) Applicant: **Masimo Corporation**, Irvine, CA (US)
- (72) Inventor: **Massi Joe E. Kiani**, Laguna Niguel, CA (US)
- (73) Assignee: **Masimo Corporation**, Irvine, CA (US)
- (*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.
- (21) Appl. No.: **15/797,839**
- (22) Filed: **Oct. 30, 2017**

(65) **Prior Publication Data**
US 2018/0184917 A1 Jul. 5, 2018

- Related U.S. Application Data**
- (63) Continuation of application No. 14/746,446, filed on Jun. 22, 2015, now Pat. No. 9,801,556, which is a continuation of application No. 13/369,773, filed on Feb. 9, 2012, now Pat. No. 9,066,666.
- (60) Provisional application No. 61/446,969, filed on Feb. 25, 2011.
- (51) **Int. Cl.**
A61B 5/1455 (2006.01)
A61B 5/026 (2006.01)
A61B 5/00 (2006.01)
- (52) **U.S. Cl.**
CPC *A61B 5/0261* (2013.01); *A61B 5/14551* (2013.01); *A61B 5/7271* (2013.01)
- (58) **Field of Classification Search**
None
See application file for complete search history.

(56) **References Cited**
U.S. PATENT DOCUMENTS

3,980,075 A	9/1976	Heule
4,960,128 A	10/1990	Gordon et al.
4,964,408 A	10/1990	Hink et al.
5,041,187 A	8/1991	Hink et al.
5,069,213 A	12/1991	Polczynski
5,163,438 A	11/1992	Gordon et al.
5,319,355 A	6/1994	Russek
5,337,744 A	8/1994	Branigan
5,341,805 A	8/1994	Stavridi et al.
D353,195 S	12/1994	Savage et al.
D353,196 S	12/1994	Savage et al.
5,377,676 A	1/1995	Vari et al.
D359,546 S	6/1995	Savage et al.
5,431,170 A	7/1995	Mathews
D361,840 S	8/1995	Savage et al.

(Continued)

OTHER PUBLICATIONS

US 8,845,543 B2, 09/2014, Diab et al. (withdrawn)

Primary Examiner — Eric F Winakur


Assistant Examiner — Marjan Fardanesh

(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson & Bear, LLP

(57) **ABSTRACT**

A patient monitor capable of measuring microcirculation at a tissue site includes a light source, a beam splitter, a photodetector and a patient monitor. Light emitted from the light source is split into a reference arm and a sample arm. The light in the sample arm is directed at a tissue site, such as an eyelid. The reflected light from the tissue site is interfered with the light from the reference arm. The photodetector measures the interference of the light from both the sample arm and the reference arm. The patient monitor uses the measurements from the photodetector to calculate the oxygen saturation at the tissue site and monitor the microcirculation at the tissue site.

21 Claims, 5 Drawing Sheets

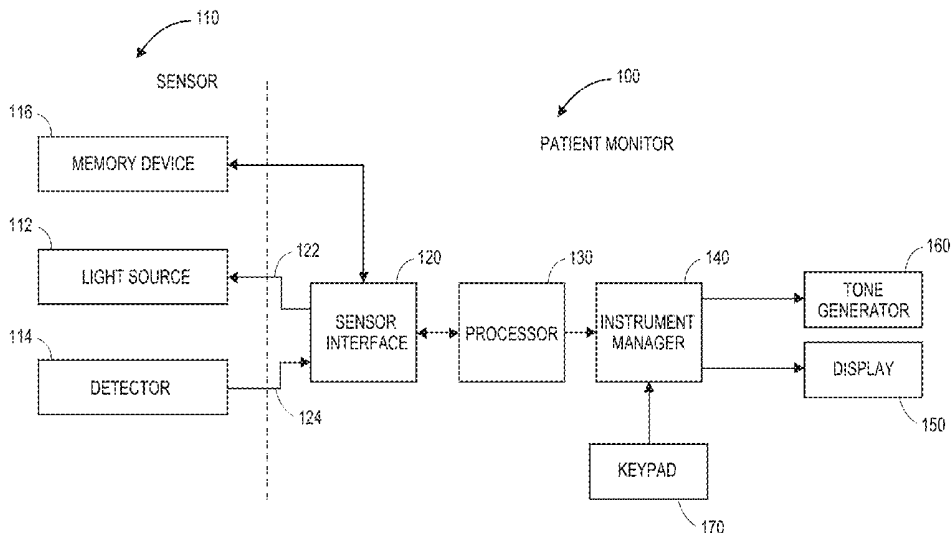

(56)

References Cited

U.S. PATENT DOCUMENTS

D362,063	S	9/1995	Savage et al.	6,343,224	B1	1/2002	Parker
5,452,717	A	9/1995	Branigan et al.	6,349,228	B1	2/2002	Kiani et al.
D363,120	S	10/1995	Savage et al.	6,360,114	B1	3/2002	Diab et al.
5,456,252	A	10/1995	Vari et al.	6,368,283	B1	4/2002	Xu et al.
5,479,934	A	1/1996	Imran	6,371,921	B1	4/2002	Caro et al.
5,482,036	A	1/1996	Diab et al.	6,377,829	B1	4/2002	Al-Ali
5,490,505	A	2/1996	Diab et al.	6,388,240	B2	5/2002	Schulz et al.
5,494,043	A	2/1996	O'Sullivan et al.	6,397,091	B2	5/2002	Diab et al.
5,533,511	A	7/1996	Kaspari et al.	6,430,437	B1	8/2002	Marro
5,534,851	A	7/1996	Russek	6,430,525	B1	8/2002	Weber et al.
5,561,275	A	10/1996	Savage et al.	6,463,311	B1	10/2002	Diab
5,562,002	A	10/1996	Lalin	6,470,199	B1	10/2002	Kopotic et al.
5,590,649	A	1/1997	Caro et al.	6,501,975	B2	12/2002	Diab et al.
5,602,924	A	2/1997	Durand et al.	6,505,059	B1	1/2003	Kollias et al.
5,632,272	A	5/1997	Diab et al.	6,515,273	B2	2/2003	Al-Ali
5,638,816	A	6/1997	Kiani-Azarbayjany et al.	6,519,487	B1	2/2003	Parker
5,638,818	A	6/1997	Diab et al.	6,525,386	B1	2/2003	Mills et al.
5,645,440	A	7/1997	Tobler et al.	6,526,300	B1	2/2003	Kiani et al.
5,685,299	A	11/1997	Diab et al.	6,541,756	B2	4/2003	Schulz et al.
D393,830	S	4/1998	Tobler et al.	6,542,764	B1	4/2003	Al-Ali et al.
5,743,262	A	4/1998	Lepper, Jr. et al.	6,580,086	B1	6/2003	Schulz et al.
5,758,644	A	6/1998	Diab et al.	6,584,336	B1	6/2003	Ali et al.
5,760,910	A	6/1998	Lepper, Jr. et al.	6,595,316	B2	7/2003	Cybulski et al.
5,769,785	A	6/1998	Diab et al.	6,597,932	B2	7/2003	Tian et al.
5,782,757	A	7/1998	Diab et al.	6,597,933	B2	7/2003	Kiani et al.
5,785,659	A	7/1998	Caro et al.	6,606,511	B1	8/2003	Ali et al.
5,791,347	A	8/1998	Flaherty et al.	6,632,181	B2	10/2003	Flaherty et al.
5,810,734	A	9/1998	Caro et al.	6,639,668	B1	10/2003	Trepagnier
5,823,950	A	10/1998	Diab et al.	6,640,116	B2	10/2003	Diab
5,830,131	A	11/1998	Caro et al.	6,643,530	B2	11/2003	Diab et al.
5,833,618	A	11/1998	Caro et al.	6,650,917	B2	11/2003	Diab et al.
5,860,919	A	1/1999	Kiani-Azarbayjany et al.	6,654,624	B2	11/2003	Diab et al.
5,890,929	A	4/1999	Mills et al.	6,658,276	B2	12/2003	Kiani et al.
5,904,654	A	5/1999	Wohltmann et al.	6,661,161	B1	12/2003	Lanzo et al.
5,919,134	A	7/1999	Diab	6,671,531	B2	12/2003	Al-Ali et al.
5,934,925	A	8/1999	Tobler et al.	6,678,543	B2	1/2004	Diab et al.
5,940,182	A	8/1999	Lepper, Jr. et al.	6,684,090	B2	1/2004	Ali et al.
5,987,343	A	11/1999	Kinast	6,684,091	B2	1/2004	Parker
5,995,855	A	11/1999	Kiani et al.	6,697,656	B1	2/2004	Al-Ali
5,997,343	A	12/1999	Mills et al.	6,697,657	B1	2/2004	Shehada et al.
6,002,952	A	12/1999	Diab et al.	6,697,658	B2	2/2004	Al-Ali
6,011,986	A	1/2000	Diab et al.	RE38,476	E	3/2004	Diab et al.
6,027,452	A	2/2000	Flaherty et al.	6,699,194	B1	3/2004	Diab et al.
6,036,642	A	3/2000	Diab et al.	6,714,804	B2	3/2004	Al-Ali et al.
6,045,509	A	4/2000	Caro et al.	RE38,492	E	4/2004	Diab et al.
6,067,462	A	5/2000	Diab et al.	6,721,582	B2	4/2004	Trepagnier et al.
6,081,735	A	6/2000	Diab et al.	6,721,585	B1	4/2004	Parker
6,088,607	A	7/2000	Diab et al.	6,725,075	B2	4/2004	Al-Ali
6,110,522	A	8/2000	Lepper, Jr. et al.	6,728,560	B2	4/2004	Kollias et al.
6,124,597	A	9/2000	Shehada	6,735,459	B2	5/2004	Parker
6,128,521	A	10/2000	Marro et al.	6,745,060	B2	6/2004	Diab et al.
6,129,675	A	10/2000	Jay	6,760,607	B2	7/2004	Al-Ali
6,144,868	A	11/2000	Parker	6,770,028	B1	8/2004	Ali et al.
6,151,516	A	11/2000	Kiani-Azarbayjany et al.	6,771,994	B2	8/2004	Kiani et al.
6,152,754	A	11/2000	Gerhardt et al.	6,792,300	B1	9/2004	Diab et al.
6,157,850	A	12/2000	Diab et al.	6,813,511	B2	11/2004	Diab et al.
6,165,005	A	12/2000	Mills et al.	6,816,741	B2	11/2004	Diab
6,184,521	B1	2/2001	Coffin, IV et al.	6,822,564	B2	11/2004	Al-Ali
6,206,830	B1	3/2001	Diab et al.	6,826,419	B2	11/2004	Diab et al.
6,229,856	B1	5/2001	Diab et al.	6,830,711	B2	12/2004	Mills et al.
6,232,609	B1	5/2001	Snyder et al.	6,850,787	B2	2/2005	Weber et al.
6,236,872	B1	5/2001	Diab et al.	6,850,788	B2	2/2005	Al-Ali
6,241,683	B1	6/2001	Macklem et al.	6,852,083	B2	2/2005	Caro et al.
6,253,097	B1	6/2001	Aronow et al.	6,861,639	B2	3/2005	Al-Ali
6,256,523	B1	7/2001	Diab et al.	6,898,452	B2	5/2005	Al-Ali et al.
6,263,222	B1	7/2001	Diab et al.	6,920,345	B2	7/2005	Al-Ali et al.
6,278,522	B1	8/2001	Lepper, Jr. et al.	6,931,268	B1	8/2005	Kiani-Azarbayjany et al.
6,280,213	B1	8/2001	Tobler et al.	6,934,570	B2	8/2005	Kiani et al.
6,285,896	B1	9/2001	Tobler et al.	6,939,305	B2	9/2005	Flaherty et al.
6,301,493	B1	10/2001	Marro et al.	6,943,348	B1	9/2005	Coffin, IV
6,308,089	B1	10/2001	von der Ruhr et al.	6,950,687	B2	9/2005	Al-Ali
6,317,627	B1	11/2001	Ennen et al.	6,961,598	B2	11/2005	Diab
6,321,100	B1	11/2001	Parker	6,970,792	B1	11/2005	Diab
6,325,761	B1	12/2001	Jay	6,979,812	B2	12/2005	Al-Ali
6,334,065	B1	12/2001	Al-Ali et al.	6,985,764	B2	1/2006	Mason et al.
				6,993,371	B2	1/2006	Kiani et al.
				6,996,427	B2	2/2006	Ali et al.
				6,999,904	B2	2/2006	Weber et al.
				7,003,338	B2	2/2006	Weber et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

7,003,339 B2	2/2006	Diab et al.	7,530,942 B1	5/2009	Diab
7,015,451 B2	2/2006	Dalke et al.	7,530,949 B2	5/2009	Al Ali et al.
7,024,233 B2	4/2006	Ali et al.	7,530,955 B2	5/2009	Diab et al.
7,027,849 B2	4/2006	Al-Ali	7,563,110 B2	7/2009	Al-Ali et al.
7,030,749 B2	4/2006	Al-Ali	7,596,398 B2	9/2009	Al-Ali et al.
7,039,449 B2	5/2006	Al-Ali	7,618,375 B2	11/2009	Flaherty
7,041,060 B2	5/2006	Flaherty et al.	D606,659 S	12/2009	Kiani et al.
7,044,918 B2	5/2006	Diab	7,647,083 B2	1/2010	Al-Ali et al.
7,048,687 B1	5/2006	Reuss et al.	D609,193 S	2/2010	Al-Ali et al.
7,067,893 B2	6/2006	Mills et al.	D614,305 S	4/2010	Al-Ali et al.
7,096,052 B2	8/2006	Mason et al.	RE41,317 E	5/2010	Parker
7,096,054 B2	8/2006	Abdul-Hafiz et al.	7,729,733 B2	6/2010	Al-Ali et al.
7,132,641 B2	11/2006	Schulz et al.	7,734,320 B2	6/2010	Al-Ali
7,142,901 B2	11/2006	Kiani et al.	7,761,127 B2	7/2010	Al-Ali et al.
7,149,561 B2	12/2006	Diab	7,761,128 B2	7/2010	Al-Ali et al.
7,186,966 B2	3/2007	Al-Ali	7,764,982 B2	7/2010	Dalke et al.
7,190,261 B2	3/2007	Al-Ali	D621,516 S	8/2010	Kiani et al.
7,215,984 B2	5/2007	Diab	7,791,155 B2	9/2010	Diab
7,215,986 B2	5/2007	Diab	7,801,581 B2	9/2010	Diab
7,221,971 B2	5/2007	Diab	7,822,452 B2	10/2010	Schurman et al.
7,225,006 B2	5/2007	Al-Ali et al.	RE41,912 E	11/2010	Parker
7,225,007 B2	5/2007	Al-Ali	7,844,313 B2	11/2010	Kiani et al.
RE39,672 E	6/2007	Shehada et al.	7,844,314 B2	11/2010	Al-Ali
7,239,905 B2	7/2007	Kiani-Azarbayjany et al.	7,844,315 B2	11/2010	Al-Ali
7,245,953 B1	7/2007	Parker	7,865,222 B2	1/2011	Weber et al.
7,254,429 B2	8/2007	Schurman et al.	7,873,497 B2	1/2011	Weber et al.
7,254,431 B2	8/2007	Al-Ali	7,880,606 B2	2/2011	Al-Ali
7,254,433 B2	8/2007	Diab et al.	7,880,626 B2	2/2011	Al-Ali et al.
7,254,434 B2	8/2007	Schulz et al.	7,891,355 B2	2/2011	Al-Ali et al.
7,272,425 B2	9/2007	Al-Ali	7,894,868 B2	2/2011	Al-Ali et al.
7,274,955 B2	9/2007	Kiani et al.	7,899,507 B2	3/2011	Al-Ali et al.
D554,263 S	10/2007	Al-Ali	7,899,518 B2	3/2011	Trepagnier et al.
7,280,858 B2	10/2007	Al-Ali	7,904,132 B2	3/2011	Weber et al.
7,289,835 B2	10/2007	Mansfield et al.	7,909,772 B2	3/2011	Popov et al.
7,292,883 B2	11/2007	De Felice et al.	7,910,875 B2	3/2011	Al-Ali
7,295,866 B2	11/2007	Al-Ali	7,919,713 B2	4/2011	Al-Ali et al.
7,328,053 B1	2/2008	Diab et al.	7,937,128 B2	5/2011	Al-Ali
7,332,784 B2	2/2008	Mills et al.	7,937,129 B2	5/2011	Mason et al.
7,338,447 B2	3/2008	Phillips	7,937,130 B2	5/2011	Diab et al.
7,340,287 B2	3/2008	Mason et al.	7,941,199 B2	5/2011	Kiani
7,341,559 B2	3/2008	Schulz et al.	7,951,086 B2	5/2011	Flaherty et al.
7,341,562 B2	3/2008	Pless et al.	7,957,780 B2	6/2011	Lamego et al.
7,343,186 B2	3/2008	Lamego et al.	7,962,188 B2	6/2011	Kiani et al.
D566,282 S	4/2008	Al-Ali et al.	7,962,190 B1	6/2011	Diab et al.
7,355,512 B1	4/2008	Al-Ali	7,976,472 B2	7/2011	Kiani
7,356,365 B2	4/2008	Schurman	7,988,637 B2	8/2011	Diab
7,371,981 B2	5/2008	Abdul-Hafiz	7,990,382 B2	8/2011	Kiani
7,373,193 B2	5/2008	Al-Ali et al.	7,991,446 B2	8/2011	Al-Ali et al.
7,373,194 B2	5/2008	Weber et al.	8,000,761 B2	8/2011	Al-Ali
7,376,453 B1	5/2008	Diab et al.	8,008,088 B2	8/2011	Bellott et al.
7,377,794 B2	5/2008	Al Ali et al.	RE42,753 E	9/2011	Kiani-Azarbayjany et al.
7,377,899 B2	5/2008	Weber et al.	8,019,400 B2	9/2011	Diab et al.
7,383,070 B2	6/2008	Diab et al.	8,028,701 B2	10/2011	Al-Ali et al.
7,415,297 B2	8/2008	Al-Ali et al.	8,029,765 B2	10/2011	Bellott et al.
7,428,432 B2	9/2008	Ali et al.	8,036,727 B2	10/2011	Schurman et al.
7,438,683 B2	10/2008	Al-Ali et al.	8,036,728 B2	10/2011	Diab et al.
7,440,787 B2	10/2008	Diab	8,046,040 B2	10/2011	Al-Ali et al.
7,454,240 B2	11/2008	Diab et al.	8,046,041 B2	10/2011	Diab et al.
7,467,002 B2	12/2008	Weber et al.	8,046,042 B2	10/2011	Diab et al.
7,469,157 B2	12/2008	Diab et al.	8,048,040 B2	11/2011	Kiani
7,471,969 B2	12/2008	Diab et al.	8,050,728 B2	11/2011	Al-Ali et al.
7,471,971 B2	12/2008	Diab et al.	RE43,169 E	2/2012	Parker
7,483,729 B2	1/2009	Al-Ali et al.	8,118,620 B2	2/2012	Al-Ali et al.
7,483,730 B2	1/2009	Diab et al.	8,126,528 B2	2/2012	Diab et al.
7,489,958 B2	2/2009	Diab et al.	8,128,572 B2	3/2012	Diab et al.
7,496,391 B2	2/2009	Diab et al.	8,130,105 B2	3/2012	Al-Ali et al.
7,496,393 B2	2/2009	Diab et al.	8,145,287 B2	3/2012	Diab et al.
D587,657 S	3/2009	Al-Ali et al.	8,150,487 B2	4/2012	Diab et al.
7,499,741 B2	3/2009	Diab et al.	8,175,672 B2	5/2012	Parker
7,499,835 B2	3/2009	Weber et al.	8,180,420 B2	5/2012	Diab et al.
7,500,950 B2	3/2009	Al-Ali et al.	8,182,443 B1	5/2012	Kiani
7,509,154 B2	3/2009	Diab et al.	8,185,180 B2	5/2012	Diab et al.
7,509,494 B2	3/2009	Al-Ali	8,190,223 B2	5/2012	Al-Ali et al.
7,510,849 B2	3/2009	Schurman et al.	8,190,227 B2	5/2012	Diab et al.
7,526,328 B2	4/2009	Diab et al.	8,203,438 B2	6/2012	Kiani et al.
			8,203,704 B2	6/2012	Merritt et al.
			8,204,566 B2	6/2012	Schurman et al.
			8,219,172 B2	7/2012	Schurman et al.
			8,224,411 B2	7/2012	Al-Ali et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

8,228,181	B2	7/2012	Al-Ali	8,652,060	B2	2/2014	Al-Ali
8,229,533	B2	7/2012	Diab et al.	8,663,107	B2	3/2014	Kiani
8,233,955	B2	7/2012	Al-Ali et al.	8,666,468	B1	3/2014	Al-Ali
8,244,325	B2	8/2012	Al-Ali et al.	8,667,967	B2	3/2014	Al-Ali et al.
8,255,026	B1	8/2012	Al-Ali	8,670,811	B2	3/2014	O'Reilly
8,255,027	B2	8/2012	Al-Ali et al.	8,670,814	B2	3/2014	Diab et al.
8,255,028	B2	8/2012	Al-Ali et al.	8,676,286	B2	3/2014	Weber et al.
8,260,577	B2	9/2012	Weber et al.	8,682,407	B2	3/2014	Al-Ali
8,265,723	B1	9/2012	McHale et al.	RE44,823	E	4/2014	Parker
8,274,360	B2	9/2012	Sampath et al.	RE44,875	E	4/2014	Kiani et al.
8,280,473	B2	10/2012	Al-Ali	8,690,799	B2	4/2014	Telfort et al.
8,301,217	B2	10/2012	Al-Ali et al.	8,700,112	B2	4/2014	Kiani
8,306,596	B2	11/2012	Schurman et al.	8,702,627	B2	4/2014	Telfort et al.
8,310,336	B2	11/2012	Muhsin et al.	8,706,179	B2	4/2014	Parker
8,315,683	B2	11/2012	Al-Ali et al.	8,712,494	B1	4/2014	MacNeish, III et al.
RE43,860	E	12/2012	Parker	8,715,206	B2	5/2014	Telfort et al.
8,337,403	B2	12/2012	Al-Ali et al.	8,718,735	B2	5/2014	Lamego et al.
8,346,330	B2	1/2013	Lamego	8,718,737	B2	5/2014	Diab et al.
8,353,842	B2	1/2013	Al-Ali et al.	8,718,738	B2	5/2014	Blank et al.
8,355,766	B2	1/2013	MacNeish, III et al.	8,720,249	B2	5/2014	Al-Ali
8,359,080	B2	1/2013	Diab et al.	8,721,541	B2	5/2014	Al-Ali et al.
8,364,223	B2	1/2013	Al-Ali et al.	8,721,542	B2	5/2014	Al-Ali et al.
8,364,226	B2	1/2013	Diab et al.	8,723,677	B1	5/2014	Kiani
8,374,665	B2	2/2013	Lamego	8,740,792	B1	6/2014	Kiani et al.
8,385,995	B2	2/2013	Al-Ali et al.	8,754,776	B2	6/2014	Poeze et al.
8,385,996	B2	2/2013	Smith et al.	8,755,535	B2	6/2014	Telfort et al.
8,388,353	B2	3/2013	Kiani et al.	8,755,856	B2	6/2014	Diab et al.
8,399,822	B2	3/2013	Al-Ali	8,755,872	B1	6/2014	Marinow
8,401,602	B2	3/2013	Kiani	8,761,850	B2	6/2014	Lamego
8,405,608	B2	3/2013	Al-Ali et al.	8,764,671	B2	7/2014	Kiani
8,414,499	B2	4/2013	Al-Ali et al.	8,768,423	B2	7/2014	Shakespeare et al.
8,418,524	B2	4/2013	Al-Ali	8,771,204	B2	7/2014	Telfort et al.
8,423,106	B2	4/2013	Lamego et al.	8,777,634	B2	7/2014	Kiani et al.
8,428,967	B2	4/2013	Olsen et al.	8,781,543	B2	7/2014	Diab et al.
8,430,817	B1	4/2013	Al-Ali et al.	8,781,544	B2	7/2014	Al-Ali et al.
8,437,825	B2	5/2013	Dalvi et al.	8,781,549	B2	7/2014	Al-Ali et al.
8,455,290	B2	6/2013	Siskavich	8,788,003	B2	7/2014	Schurman et al.
8,457,703	B2	6/2013	Al-Ali	8,790,268	B2	7/2014	Al-Ali
8,457,707	B2	6/2013	Kiani	8,801,613	B2	8/2014	Al-Ali et al.
8,463,349	B2	6/2013	Diab et al.	8,821,397	B2	9/2014	Al-Ali et al.
8,466,286	B2	6/2013	Bellot et al.	8,821,415	B2	9/2014	Al-Ali et al.
8,471,713	B2	6/2013	Poeze et al.	8,830,449	B1	9/2014	Lamego et al.
8,473,020	B2	6/2013	Kiani et al.	8,831,700	B2	9/2014	Schurman et al.
8,483,787	B2	7/2013	Al-Ali et al.	8,840,549	B2	9/2014	Al-Ali et al.
8,489,364	B2	7/2013	Weber et al.	8,847,740	B2	9/2014	Kiani et al.
8,498,684	B2	7/2013	Weber et al.	8,849,365	B2	9/2014	Smith et al.
8,504,128	B2	8/2013	Blank et al.	8,852,094	B2	10/2014	Al-Ali et al.
8,509,867	B2	8/2013	Workman et al.	8,852,994	B2	10/2014	Wojtczuk et al.
8,515,509	B2	8/2013	Bruinsma et al.	8,868,147	B2	10/2014	Stippick et al.
8,523,781	B2	9/2013	Al-Ali	8,868,150	B2	10/2014	Al-Ali et al.
8,529,301	B2	9/2013	Al-Ali et al.	8,870,792	B2	10/2014	Al-Ali et al.
8,532,727	B2	9/2013	Al-Ali et al.	8,886,271	B2	11/2014	Kiani et al.
8,532,728	B2	9/2013	Diab et al.	8,888,539	B2	11/2014	Al-Ali et al.
D692,145	S	10/2013	Al-Ali et al.	8,888,708	B2	11/2014	Diab et al.
8,547,209	B2	10/2013	Kiani et al.	8,892,180	B2	11/2014	Weber et al.
8,548,548	B2	10/2013	Al-Ali	8,897,847	B2	11/2014	Al-Ali
8,548,549	B2	10/2013	Schurman et al.	8,909,310	B2	12/2014	Lamego et al.
8,548,550	B2	10/2013	Al-Ali et al.	8,911,377	B2	12/2014	Al-Ali
8,560,032	B2	10/2013	Al-Ali et al.	8,912,909	B2	12/2014	Al-Ali et al.
8,560,034	B1	10/2013	Diab et al.	8,920,317	B2	12/2014	Al-Ali et al.
8,570,167	B2	10/2013	Al-Ali	8,921,699	B2	12/2014	Al-Ali et al.
8,570,503	B2	10/2013	Vo et al.	8,922,382	B2	12/2014	Al-Ali et al.
8,571,617	B2	10/2013	Reichgott et al.	8,929,964	B2	1/2015	Al-Ali et al.
8,571,618	B1	10/2013	Lamego et al.	8,942,777	B2	1/2015	Diab et al.
8,571,619	B2	10/2013	Al-Ali et al.	8,948,834	B2	2/2015	Diab et al.
8,577,431	B2	11/2013	Lamego et al.	8,948,835	B2	2/2015	Diab
8,581,732	B2	11/2013	Al-Ali et al.	8,965,471	B2	2/2015	Lamego
8,584,345	B2	11/2013	Al-Ali et al.	8,983,564	B2	3/2015	Al-Ali
8,588,880	B2	11/2013	Abdul-Hafiz et al.	8,989,831	B2	3/2015	Al-Ali et al.
8,600,467	B2	12/2013	Al-Ali et al.	8,996,085	B2	3/2015	Kiani et al.
8,606,342	B2	12/2013	Diab	8,998,809	B2	4/2015	Kiani
8,626,255	B2	1/2014	Al-Ali et al.	9,028,429	B2	5/2015	Telfort et al.
8,630,691	B2	1/2014	Lamego et al.	9,037,207	B2	5/2015	Al-Ali et al.
8,634,889	B2	1/2014	Al-Ali et al.	9,060,721	B2	6/2015	Reichgott et al.
8,641,631	B2	2/2014	Sierra et al.	9,066,666	B2	6/2015	Kiani
				9,066,680	B1	6/2015	Al-Ali et al.
				9,072,474	B2	7/2015	Al-Ali et al.
				9,078,560	B2	7/2015	Schurman et al.
				9,084,569	B2	7/2015	Weber et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

9,095,316 B2	8/2015	Welch et al.	9,591,975 B2	3/2017	Dalvi et al.
9,106,038 B2	8/2015	Telfort et al.	9,622,692 B2	4/2017	Lamego et al.
9,107,625 B2	8/2015	Telfort et al.	9,622,693 B2	4/2017	Diab
9,107,626 B2	8/2015	Al-Ali et al.	D788,312 S	5/2017	Al-Ali et al.
9,113,831 B2	8/2015	Al-Ali	9,636,055 B2	5/2017	Al-Ali et al.
9,113,832 B2	8/2015	Al-Ali	9,636,056 B2	5/2017	Al-Ali
9,119,595 B2	9/2015	Lamego	9,649,054 B2	5/2017	Lamego et al.
9,131,881 B2	9/2015	Diab et al.	9,662,052 B2	5/2017	Al-Ali et al.
9,131,882 B2	9/2015	Al-Ali et al.	9,668,679 B2	6/2017	Schurman et al.
9,131,883 B2	9/2015	Al-Ali	9,668,680 B2	6/2017	Bruinsma et al.
9,131,917 B2	9/2015	Telfort et al.	9,668,703 B2	6/2017	Al-Ali
9,138,180 B1	9/2015	Coverston et al.	9,675,286 B2	6/2017	Diab
9,138,182 B2	9/2015	Al-Ali et al.	9,687,160 B2	6/2017	Kiani
9,138,192 B2	9/2015	Weber et al.	9,693,719 B2	7/2017	Al-Ali et al.
9,142,117 B2	9/2015	Muhsin et al.	9,693,737 B2	7/2017	Al-Ali
9,153,112 B1	10/2015	Kiani et al.	9,697,928 B2	7/2017	Al-Ali et al.
9,153,121 B2	10/2015	Kiani et al.	9,717,425 B2	8/2017	Kiani et al.
9,161,696 B2	10/2015	Al-Ali et al.	9,717,458 B2	8/2017	Lamego et al.
9,161,713 B2	10/2015	Al-Ali et al.	9,724,016 B1	8/2017	Al-Ali et al.
9,167,995 B2	10/2015	Lamego et al.	9,724,024 B2	8/2017	Al-Ali
9,176,141 B2	11/2015	Al-Ali et al.	9,724,025 B1	8/2017	Kiani et al.
9,186,102 B2	11/2015	Bruinsma et al.	9,730,640 B2	8/2017	Diab et al.
9,192,312 B2	11/2015	Al-Ali	9,743,887 B2	8/2017	Al-Ali et al.
9,192,329 B2	11/2015	Al-Ali	9,749,232 B2	8/2017	Sampath et al.
9,192,351 B1	11/2015	Telfort et al.	9,750,442 B2	9/2017	Olsen
9,195,385 B2	11/2015	Al-Ali et al.	9,750,443 B2	9/2017	Smith et al.
9,211,072 B2	12/2015	Kiani	9,750,461 B1	9/2017	Telfort
9,211,095 B1	12/2015	Al-Ali	9,775,545 B2	10/2017	Al-Ali et al.
9,218,454 B2	12/2015	Kiani et al.	9,775,546 B2	10/2017	Diab et al.
9,226,696 B2	1/2016	Kiani	9,775,570 B2	10/2017	Al-Ali
9,241,662 B2	1/2016	Al-Ali et al.	9,778,079 B1	10/2017	Al-Ali et al.
9,245,668 B1	1/2016	Vo et al.	9,782,077 B2	10/2017	Lamego et al.
9,259,185 B2	2/2016	Abdul-Hafiz et al.	9,782,110 B2	10/2017	Kiani
9,267,572 B2	2/2016	Barker et al.	9,787,568 B2	10/2017	Lamego et al.
9,277,880 B2	3/2016	Poeze et al.	9,788,735 B2	10/2017	Al-Ali
9,289,167 B2	3/2016	Diab et al.	9,788,768 B2	10/2017	Al-Ali et al.
9,295,421 B2	3/2016	Kiani et al.	9,795,300 B2	10/2017	Al-Ali
9,307,928 B1	4/2016	Al-Ali et al.	9,795,310 B2	10/2017	Al-Ali
9,323,894 B2	4/2016	Kiani	9,795,358 B2	10/2017	Telfort et al.
D755,392 S	5/2016	Hwang et al.	9,795,739 B2	10/2017	Al-Ali et al.
9,326,712 B1	5/2016	Kiani	9,801,556 B2	10/2017	Kiani
9,333,316 B2	5/2016	Kiani	9,801,588 B2	10/2017	Weber et al.
9,339,220 B2	5/2016	Lamego et al.	9,808,188 B1	11/2017	Perea et al.
9,341,565 B2	5/2016	Lamego et al.	9,814,418 B2	11/2017	Weber et al.
9,351,673 B2	5/2016	Diab et al.	9,820,691 B2	11/2017	Kiani
9,351,675 B2	5/2016	Al-Ali et al.	9,833,152 B2	12/2017	Kiani et al.
9,364,181 B2	6/2016	Kiani et al.	9,833,180 B2	12/2017	Shakespeare et al.
9,368,671 B2	6/2016	Wojtczuk et al.	9,839,379 B2	12/2017	Al-Ali et al.
9,370,325 B2	6/2016	Al-Ali et al.	9,839,381 B1	12/2017	Weber et al.
9,370,326 B2	6/2016	McHale et al.	9,847,002 B2	12/2017	Kiani et al.
9,370,335 B2	6/2016	Al-Ali et al.	9,847,749 B2	12/2017	Kiani et al.
9,375,185 B2	6/2016	Ali et al.	9,848,800 B1	12/2017	Lee et al.
9,386,953 B2	7/2016	Al-Ali	9,848,806 B2	12/2017	Al-Ali et al.
9,386,961 B2	7/2016	Al-Ali et al.	9,848,807 B2	12/2017	Lamego
9,392,945 B2	7/2016	Al-Ali et al.	9,861,298 B2	1/2018	Eckerbom et al.
9,397,448 B2	7/2016	Al-Ali et al.	9,861,304 B2	1/2018	Al-Ali et al.
9,408,542 B1	8/2016	Kinast et al.	9,861,305 B1	1/2018	Weber et al.
9,436,645 B2	9/2016	Al-Ali et al.	9,867,578 B2	1/2018	Al-Ali et al.
9,445,759 B1	9/2016	Lamego et al.	9,872,623 B2	1/2018	Al-Ali
9,466,919 B2	10/2016	Kiani et al.	9,876,320 B2	1/2018	Coverston et al.
9,474,474 B2	10/2016	Lamego et al.	9,877,650 B2	1/2018	Muhsin et al.
9,480,422 B2	11/2016	Al-Ali	9,877,686 B2	1/2018	Al-Ali et al.
9,480,435 B2	11/2016	Olsen	9,891,079 B2	2/2018	Dalvi
9,492,110 B2	11/2016	Al-Ali et al.	9,895,107 B2	2/2018	Al-Ali et al.
9,510,779 B2	12/2016	Poeze et al.	2003/0069489 A1	4/2003	Abreu
9,517,024 B2	12/2016	Kiani et al.	2006/0161054 A1	7/2006	Reuss et al.
9,532,722 B2	1/2017	Lamego et al.	2007/0282478 A1	12/2007	Al-Ali et al.
9,538,949 B2	1/2017	Al-Ali et al.	2009/0143655 A1	6/2009	Shani
9,538,980 B2	1/2017	Telfort et al.	2009/0247984 A1	10/2009	Lamego et al.
9,549,696 B2	1/2017	Lamego et al.	2009/0275813 A1	11/2009	Davis
9,554,737 B2	1/2017	Schurman et al.	2009/0275844 A1	11/2009	Al-Ali
9,560,996 B2	2/2017	Kiani	2010/0004518 A1	1/2010	Vo et al.
9,560,998 B2	2/2017	Al-Ali et al.	2010/0030040 A1	2/2010	Poeze et al.
9,566,019 B2	2/2017	Al-Ali et al.	2010/0261979 A1	10/2010	Kiani
9,579,039 B2	2/2017	Jansen et al.	2011/0001605 A1	1/2011	Kiani et al.
			2011/0082711 A1	4/2011	Poeze et al.
			2011/0105854 A1	5/2011	Kiani et al.
			2011/0125060 A1	5/2011	Telfort et al.
			2011/0208015 A1	8/2011	Welch et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2011/0213212	A1	9/2011	Al-Ali	2014/0275871	A1	9/2014	Lamego et al.
2011/0230733	A1	9/2011	Al-Ali	2014/0275872	A1	9/2014	Merritt et al.
2011/0237911	A1	9/2011	Lamego et al.	2014/0275881	A1	9/2014	Lamego et al.
2012/0059267	A1	3/2012	Lamego et al.	2014/0276115	A1	9/2014	Dalvi et al.
2012/0116175	A1	5/2012	Al-Ali et al.	2014/0288400	A1	9/2014	Diab et al.
2012/0165629	A1	6/2012	Merritt et al.	2014/0296664	A1	10/2014	Bruinsma et al.
2012/0179006	A1	7/2012	Jansen et al.	2014/0303520	A1	10/2014	Telfort et al.
2012/0209082	A1	8/2012	Al-Ali	2014/0309506	A1	10/2014	Lamego et al.
2012/0209084	A1	8/2012	Olsen et al.	2014/0316217	A1	10/2014	Purdon et al.
2012/0227739	A1	9/2012	Kiani	2014/0316218	A1	10/2014	Purdon et al.
2012/0283524	A1	11/2012	Kiani et al.	2014/0316228	A1	10/2014	Blank et al.
2012/0296178	A1	11/2012	Lamego et al.	2014/0323825	A1	10/2014	Al-Ali et al.
2012/0319816	A1	12/2012	Al-Ali	2014/0323897	A1	10/2014	Brown et al.
2012/0330112	A1	12/2012	Lamego et al.	2014/0323898	A1	10/2014	Purdon et al.
2013/0023775	A1	1/2013	Lamego et al.	2014/0330092	A1	11/2014	Al-Ali et al.
2013/0041591	A1	2/2013	Lamego	2014/0330098	A1	11/2014	Merritt et al.
2013/0045685	A1	2/2013	Kiani	2014/0330099	A1	11/2014	Al-Ali et al.
2013/0046204	A1	2/2013	Lamego et al.	2014/0333440	A1	11/2014	Kiani
2013/0060147	A1	3/2013	Welch et al.	2014/0336481	A1	11/2014	Shakespeare et al.
2013/0096405	A1	4/2013	Garfio	2014/0343436	A1	11/2014	Kiani
2013/0096936	A1	4/2013	Sampath et al.	2014/0357966	A1	12/2014	Al-Ali et al.
2013/0109935	A1	5/2013	Al-Ali et al.	2015/0005600	A1	1/2015	Blank et al.
2013/0162433	A1	6/2013	Muhsin et al.	2015/0011907	A1	1/2015	Purdon et al.
2013/0190581	A1	7/2013	Al-Ali et al.	2015/0012231	A1	1/2015	Poeze et al.
2013/0197328	A1	8/2013	Diab et al.	2015/0018650	A1	1/2015	Al-Ali et al.
2013/0211214	A1	8/2013	Olsen	2015/0032029	A1	1/2015	Al-Ali et al.
2013/0243021	A1	9/2013	Siskavich	2015/0038859	A1	2/2015	Dalvi et al.
2013/0253334	A1	9/2013	Al-Ali et al.	2015/0080754	A1	3/2015	Purdon et al.
2013/0274571	A1	10/2013	Diab et al.	2015/0087936	A1	3/2015	Al-Ali et al.
2013/0296672	A1	11/2013	O'Neil et al.	2015/0094546	A1	4/2015	Al-Ali
2013/0296713	A1	11/2013	Al-Ali et al.	2015/0097701	A1	4/2015	Al-Ali et al.
2013/0317370	A1	11/2013	Dalvi et al.	2015/0099950	A1	4/2015	Al-Ali et al.
2013/0324808	A1	12/2013	Al-Ali et al.	2015/0099955	A1	4/2015	Al-Ali et al.
2013/0331660	A1	12/2013	Al-Ali et al.	2015/0101844	A1	4/2015	Al-Ali et al.
2013/0331670	A1	12/2013	Kiani	2015/0106121	A1	4/2015	Muhsin et al.
2013/0338461	A1	12/2013	Lamego et al.	2015/0112151	A1	4/2015	Muhsin et al.
2014/0012100	A1	1/2014	Al-Ali et al.	2015/0116076	A1	4/2015	Al-Ali et al.
2014/0025306	A1	1/2014	Weber et al.	2015/0126830	A1	5/2015	Schurman et al.
2014/0034353	A1	2/2014	Al-Ali et al.	2015/0165312	A1	6/2015	Kiani
2014/0051953	A1	2/2014	Lamego et al.	2015/0196249	A1	7/2015	Brown et al.
2014/0058230	A1	2/2014	Abdul-Hafiz et al.	2015/0216459	A1	8/2015	Al-Ali et al.
2014/0066783	A1	3/2014	Kiani et al.	2015/0238722	A1	8/2015	Al-Ali
2014/0077956	A1	3/2014	Sampath et al.	2015/0245773	A1	9/2015	Lamego et al.
2014/0081100	A1	3/2014	Muhsin et al.	2015/0245794	A1	9/2015	Al-Ali
2014/0081175	A1	3/2014	Telfort	2015/0257689	A1	9/2015	Al-Ali et al.
2014/0094667	A1	4/2014	Schurman et al.	2015/0272514	A1	10/2015	Kiani et al.
2014/0100434	A1	4/2014	Diab et al.	2015/0351697	A1	12/2015	Weber et al.
2014/0114199	A1	4/2014	Lamego et al.	2015/0359429	A1	12/2015	Al-Ali et al.
2014/0120564	A1	5/2014	Workman et al.	2015/0366507	A1	12/2015	Blank
2014/0121482	A1	5/2014	Merritt et al.	2016/0029932	A1	2/2016	Al-Ali
2014/0121483	A1	5/2014	Kiani	2016/0058347	A1	3/2016	Reichgott et al.
2014/0127137	A1	5/2014	Bellott et al.	2016/0066824	A1	3/2016	Al-Ali et al.
2014/0128696	A1	5/2014	Al-Ali	2016/0081552	A1	3/2016	Wojtczuk et al.
2014/0128699	A1	5/2014	Al-Ali et al.	2016/0095543	A1	4/2016	Telfort et al.
2014/0129702	A1	5/2014	Lamego et al.	2016/0095548	A1	4/2016	Al-Ali et al.
2014/0135588	A1	5/2014	Al-Ali et al.	2016/0103598	A1	4/2016	Al-Ali et al.
2014/0142401	A1	5/2014	Al-Ali et al.	2016/0143548	A1	5/2016	Al-Ali
2014/0142402	A1	5/2014	Al-Ali et al.	2016/0166182	A1	6/2016	Al-Ali et al.
2014/0163344	A1	6/2014	Al-Ali	2016/0166183	A1	6/2016	Poeze et al.
2014/0163402	A1	6/2014	Lamego et al.	2016/0192869	A1	7/2016	Kiani et al.
2014/0166076	A1	6/2014	Kiani et al.	2016/0196388	A1	7/2016	Lamego
2014/0171763	A1	6/2014	Diab	2016/0197436	A1	7/2016	Barker et al.
2014/0180038	A1	6/2014	Kiani	2016/0213281	A1	7/2016	Eckerbom et al.
2014/0180154	A1	6/2014	Sierra et al.	2016/0228043	A1	8/2016	O'Neil et al.
2014/0180160	A1	6/2014	Brown et al.	2016/0233632	A1	8/2016	Scruggs et al.
2014/0187973	A1	7/2014	Brown et al.	2016/0234944	A1	8/2016	Schmidt et al.
2014/0194709	A1	7/2014	Al-Ali et al.	2016/0270735	A1	9/2016	Diab et al.
2014/0194711	A1	7/2014	Al-Ali	2016/0283665	A1	9/2016	Sampath et al.
2014/0194766	A1	7/2014	Al-Ali et al.	2016/0287090	A1	10/2016	Al-Ali et al.
2014/0206963	A1	7/2014	Al-Ali	2016/0287786	A1	10/2016	Kiani
2014/0213864	A1	7/2014	Abdul-Hafiz et al.	2016/0296169	A1	10/2016	McHale et al.
2014/0243627	A1	8/2014	Diab et al.	2016/0310052	A1	10/2016	Al-Ali et al.
2014/0266790	A1	9/2014	Al-Ali et al.	2016/0314260	A1	10/2016	Kiani
2014/0275808	A1	9/2014	Poeze et al.	2016/0324486	A1	11/2016	Al-Ali et al.
2014/0275835	A1	9/2014	Lamego et al.	2016/0324488	A1	11/2016	Olsen
				2016/0327984	A1	11/2016	Al-Ali et al.
				2016/0328528	A1	11/2016	Al-Ali et al.
				2016/0331332	A1	11/2016	Al-Ali
				2016/0367173	A1	12/2016	Dalvi et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2017/0000394	A1	1/2017	Al-Ali et al.	2017/0196464	A1	7/2017	Jansen et al.
2017/0007134	A1	1/2017	Al-Ali et al.	2017/0196470	A1	7/2017	Lamego et al.
2017/0007198	A1	1/2017	Al-Ali et al.	2017/0202490	A1	7/2017	Al-Ali et al.
2017/0014083	A1	1/2017	Diab et al.	2017/0224262	A1	8/2017	Al-Ali
2017/0014084	A1	1/2017	Al-Ali et al.	2017/0228516	A1	8/2017	Sampath et al.
2017/0027456	A1	2/2017	Kinast et al.	2017/0245790	A1	8/2017	Al-Ali et al.
2017/0042488	A1	2/2017	Muhsin	2017/0251974	A1	9/2017	Shreim et al.
2017/0055851	A1	3/2017	Al-Ali	2017/0251975	A1	9/2017	Shreim et al.
2017/0055882	A1	3/2017	Al-Ali et al.	2017/0258403	A1	9/2017	Abdul-Hafiz et al.
2017/0055887	A1	3/2017	Al-Ali	2017/0311891	A1	11/2017	Kiani et al.
2017/0055896	A1	3/2017	Al-Ali et al.	2017/0325728	A1	11/2017	Al-Ali et al.
2017/0079594	A1	3/2017	Telfort et al.	2017/0332976	A1	11/2017	Al-Ali et al.
2017/0086723	A1	3/2017	Al-Ali et al.	2017/0340293	A1	11/2017	Al-Ali et al.
2017/0143281	A1	5/2017	Olsen	2017/0360310	A1	12/2017	Kiani et al.
2017/0147774	A1	5/2017	Kiani	2017/0367632	A1	12/2017	Al-Ali et al.
2017/0156620	A1	6/2017	Al-Ali et al.	2018/0008146	A1	1/2018	Al-Ali et al.
2017/0173632	A1	6/2017	Al-Ali	2018/0014752	A1	1/2018	Al-Ali et al.
2017/0187146	A1	6/2017	Kiani et al.	2018/0028124	A1	2/2018	Al-Ali et al.
2017/0188919	A1	7/2017	Al-Ali et al.	2018/0055385	A1	3/2018	Al-Ali
				2018/0055390	A1	3/2018	Kiani et al.
				2018/0055430	A1	3/2018	Diab et al.
				2018/0064381	A1	3/2018	Shakespeare et al.
				2018/0069776	A1	3/2018	Lamego et al.

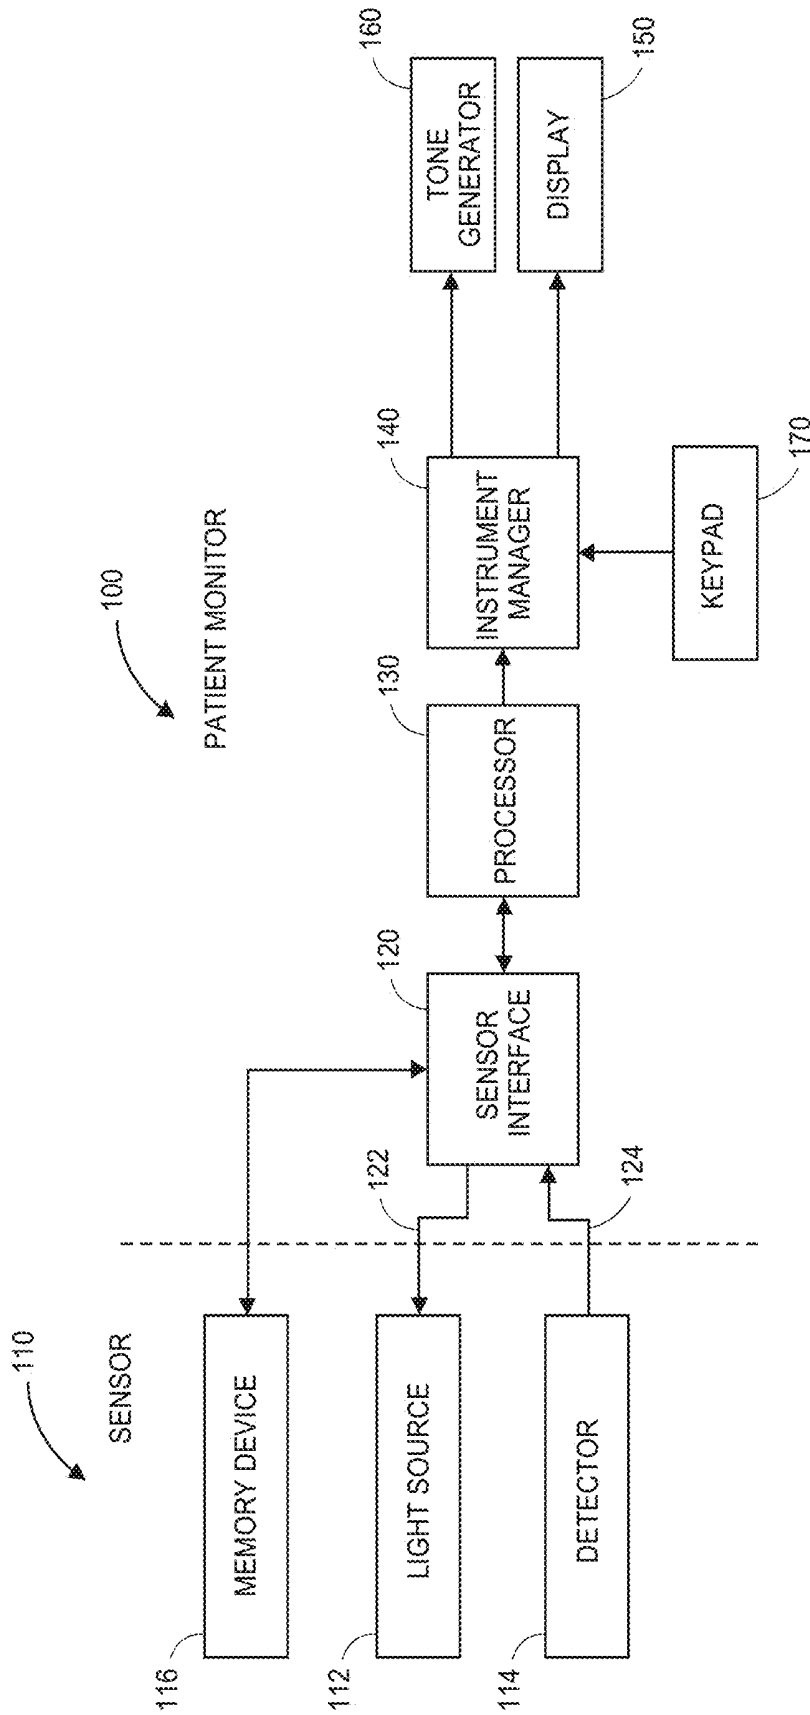


FIG. 1

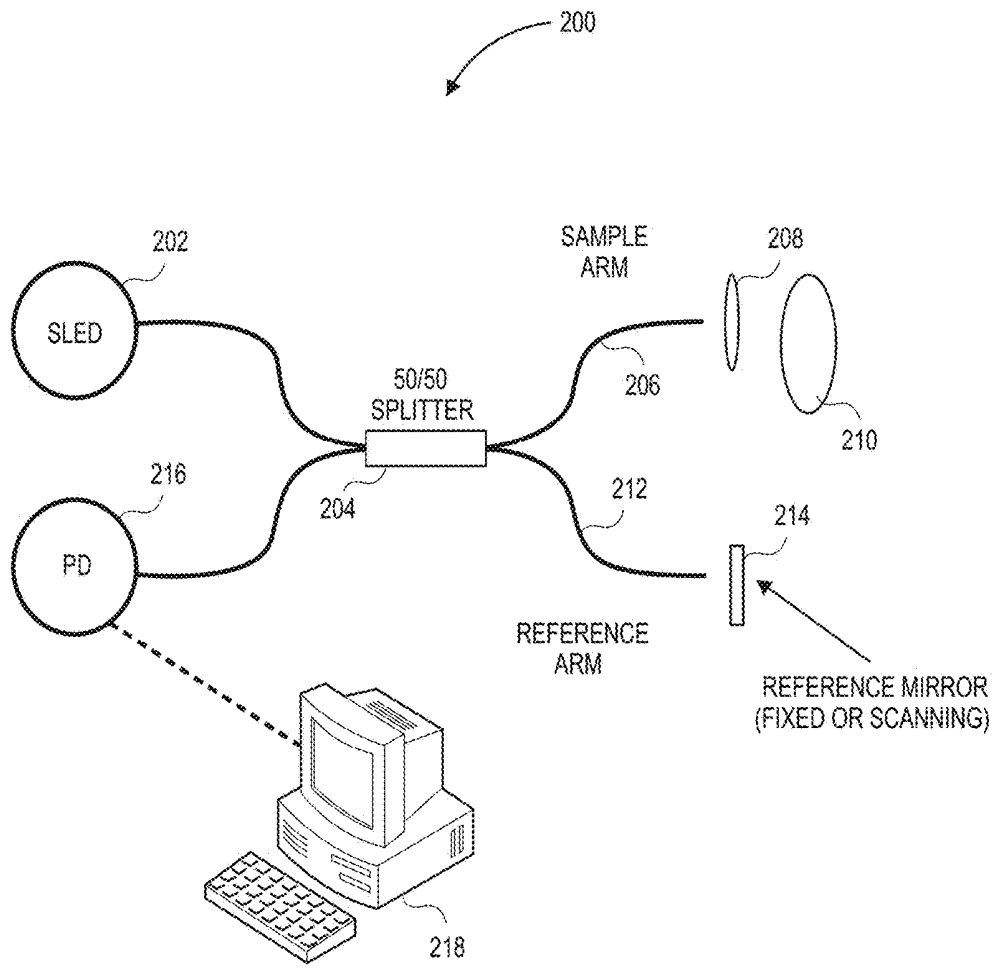


FIG. 2A

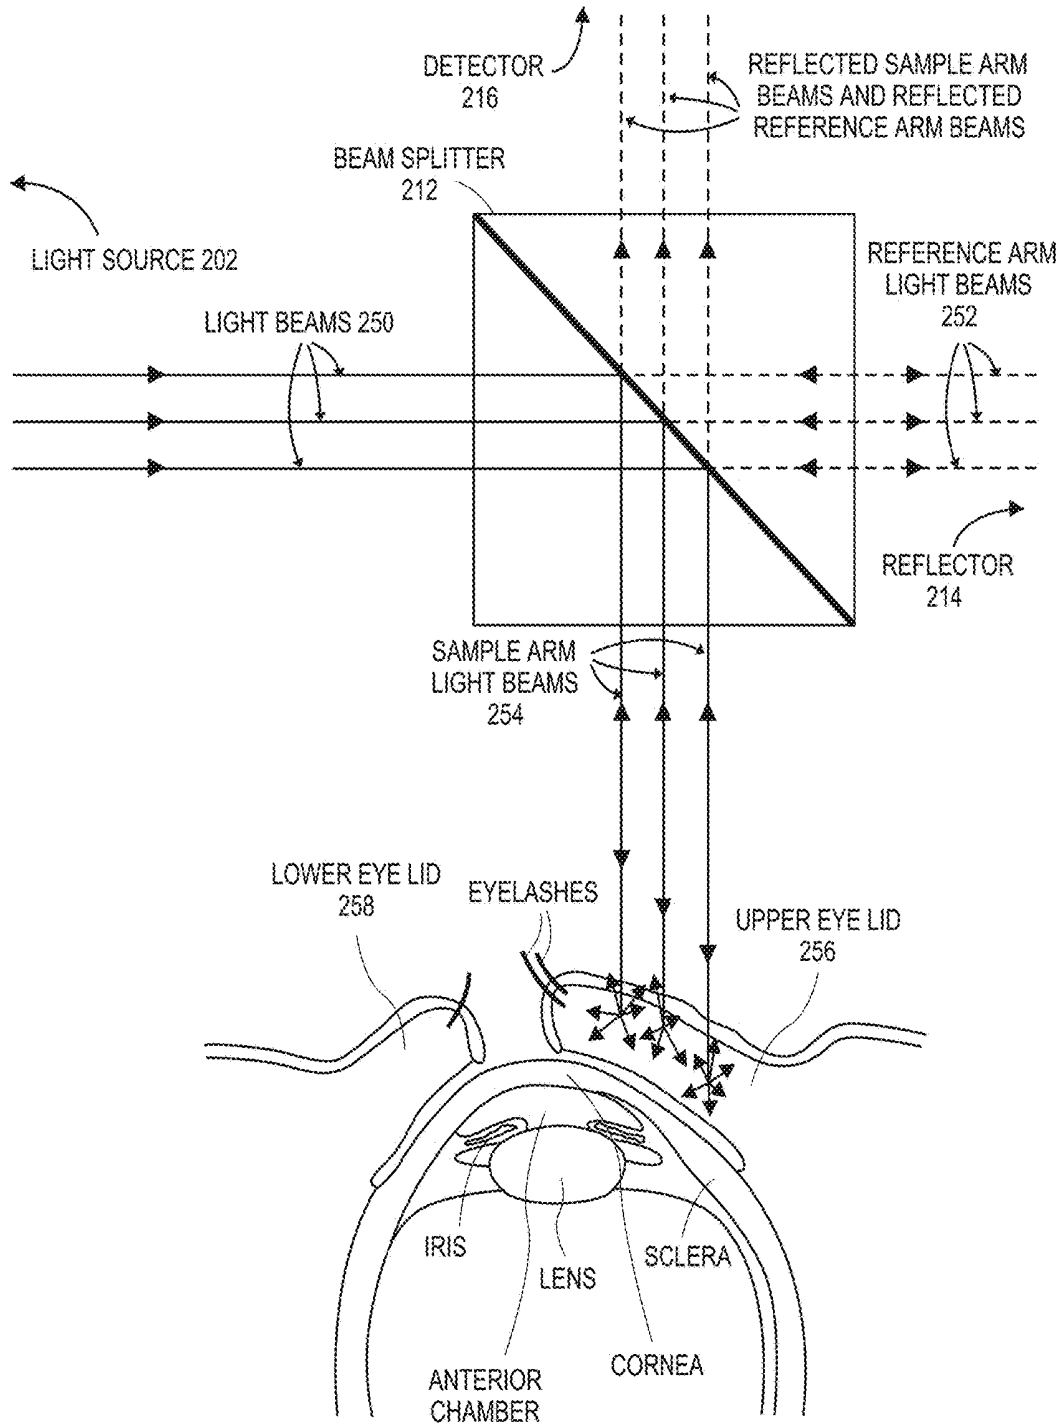


FIG. 2B

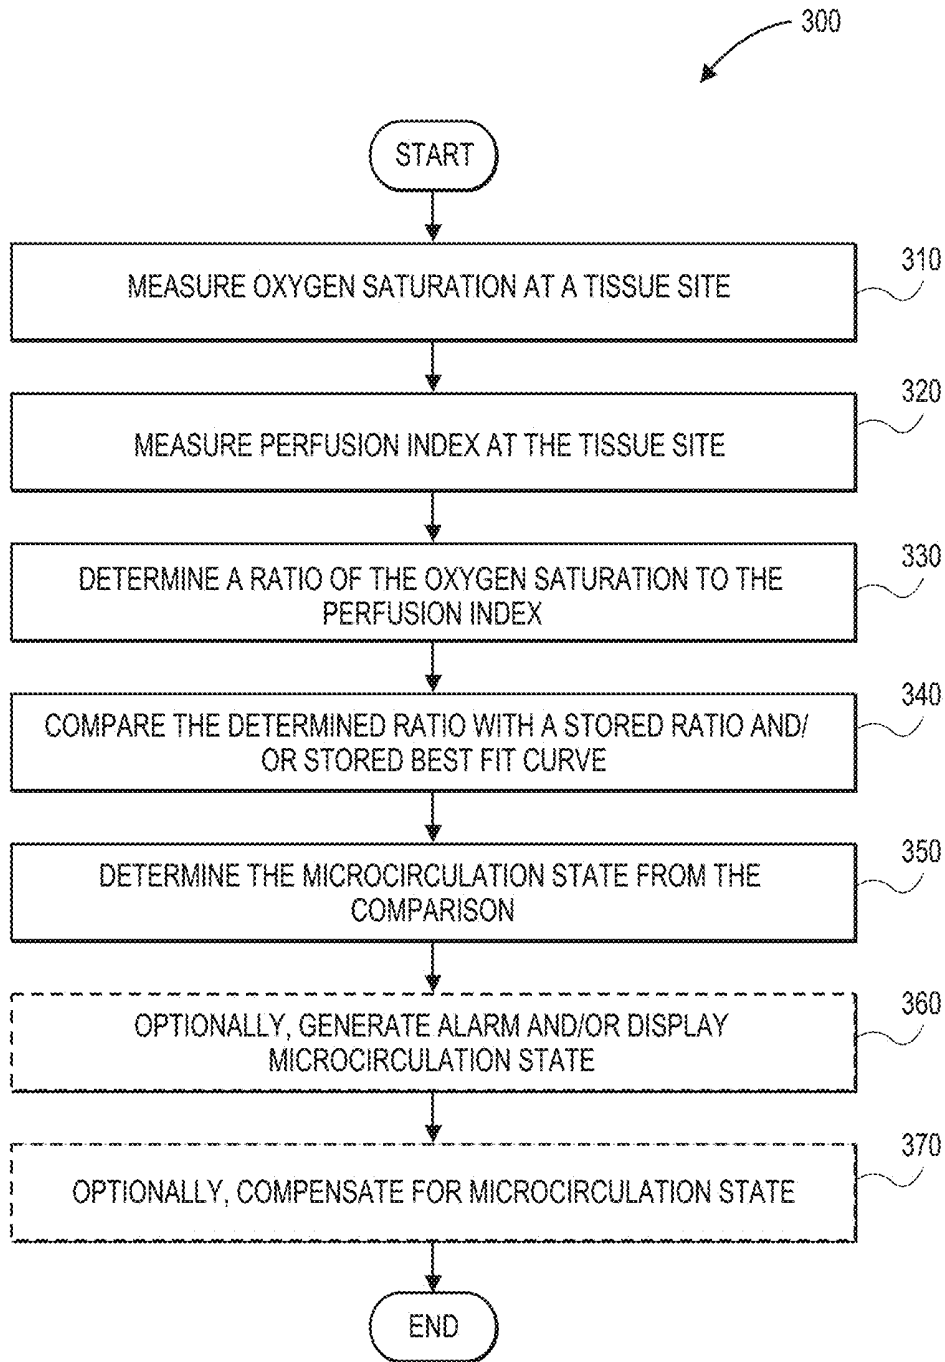


FIG. 3

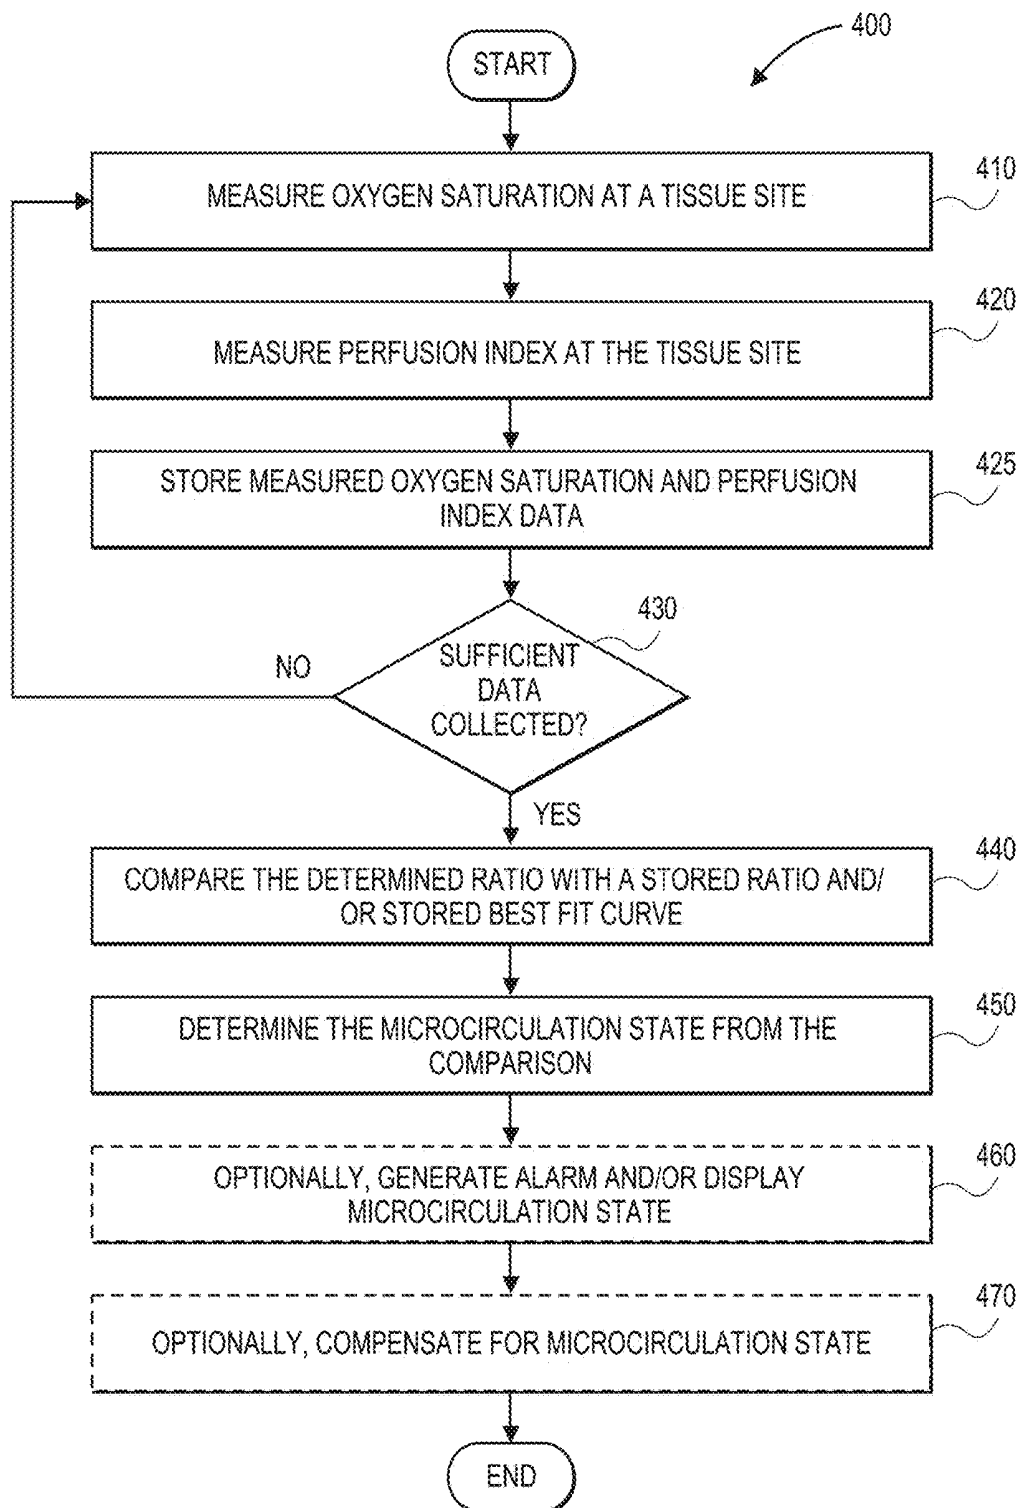


FIG. 4

PATIENT MONITOR FOR MONITORING MICROCIRCULATION

CROSS-REFERENCE TO RELATED APPLICATIONS

Any and all applications, for which a foreign or domestic priority claim is identified in the Application Data Sheet as filed with the present application, are hereby incorporated by reference. For example, this application is a continuation of U.S. patent application Ser. No. 14/746,446, filed Jun. 22, 2015, entitled "Patient Monitor For Monitoring Microcirculation," which is a continuation of U.S. patent application Ser. No. 13/369,773, filed Feb. 9, 2012, now issued as U.S. Pat. No. 9,066,666, entitled "Patient Monitor For Monitoring Microcirculation," which claims the benefit of U.S. Provisional Patent Application No. 61/446,969, filed Feb. 25, 2011, entitled "Patient Monitor for Monitoring Microcirculation," the entirety of each of which is hereby incorporated herein by reference to be considered a part of this specification.

FIELD

The present disclosure relates to medical sensors and specifically to a medical sensor and/or monitor for determining the circulation state in blood vessels.

BACKGROUND OF THE DISCLOSURE

Patient monitoring of various physiological parameters of a patient is important to a wide range of medical applications. Oximetry is one of the techniques that has developed to accomplish the monitoring of some of these physiological characteristics. It was developed to study and to measure, among other things, the oxygen status of blood. Pulse oximetry—a noninvasive, widely accepted form of oximetry—relies on a sensor attached externally to a patient to output signals indicative of various physiological parameters, such as a patient's constituents and/or analytes, including for example a percent value for arterial oxygen saturation, carbon monoxide saturation, methemoglobin saturation, fractional saturations, total hematocrit, bilirubins, perfusion quality, or the like. A pulse oximetry system generally includes a patient monitor, a communications medium such as a cable, and/or a physiological sensor having light emitters and a detector, such as one or more LEDs and a photodetector. The sensor is attached to a tissue site, such as a finger, toe, ear lobe, nose, hand, foot, or other site having pulsatile blood flow which can be penetrated by light from the emitters. The detector is responsive to the emitted light after attenuation by pulsatile blood flowing in the tissue site. The detector outputs a detector signal to the monitor over the communication medium, which processes the signal to provide a numerical readout of physiological parameters such as oxygen saturation (SpO₂) and/or pulse rate. The detector signal can also be used by the monitor to create an image on a display screen of the tissue being monitored.

High fidelity pulse oximeters capable of reading through motion induced noise are disclosed in U.S. Pat. Nos. 7,096,054, 6,813,511, 6,792,300, 6,770,028, 6,658,276, 6,157,850, 6,002,952, 5,769,785, and 5,758,644, which are assigned to Masimo Corporation of Irvine, Calif. ("Masimo Corp.") and are incorporated by reference herein. Advanced physiological monitoring systems can incorporate pulse oximetry in addition to advanced features for the calculation and display

of other blood parameters, such as carboxyhemoglobin (HbCO), methemoglobin (HbMet), total hemoglobin (Hbt), total Hematocrit (Hct), oxygen concentrations, glucose concentrations, blood pressure, electrocardiogram data, temperature, and/or respiratory rate as a few examples. Typically, the physiological monitoring system provides a numerical readout of and/or waveform of the measured parameter. Advanced physiological monitors and multiple wavelength optical sensors capable of measuring parameters in addition to SpO₂, such as HbCO, HbMet and/or Hbt are described in at least U.S. Pat. No. 7,764,982, and U.S. application Ser. No. 11/366,208, filed Mar. 1, 2006, titled Noninvasive Multi-Parameter Patient Monitor, assigned to Masimo Laboratories, Inc. and incorporated by reference herein. Further, noninvasive blood parameter monitors and optical sensors including Rainbow™ adhesive and reusable sensors and RAD-57™ and Radical-7™ monitors capable of measuring SpO₂, pulse rate, perfusion index (PI), signal quality (SiQ), pulse variability index (PVI), HbCO and/or HbMet, among other parameters, are also commercially available from Masimo Corp.

During blood circulation, arteries carry blood away from the heart in high volume and under high pressure. Arteries branch off into smaller blood vessels, called arterioles. Arterioles are well innervated, surrounded by smooth muscle cells, and are about 10-100 μm in diameter. Arterioles carry the blood to the capillaries, which are the smallest blood vessels, which are not innervated, have no smooth muscle, and are about 5-8 μm in diameter. Blood flows out of the capillaries into the venules, which have little smooth muscle and are about 10-200 μm in diameter. The blood flows from venules into the veins, which carry blood back to the heart. Arterioles, venules, and/or capillaries may also be referred to as microvessels.

Microcirculation generally refers to the vascular network lying between the arterioles and the venules, including the capillaries, as well as the flow of blood through this network. These small vessels can be found in the vasculature which are embedded within organs and are responsible for the distribution of blood within tissues as opposed to larger vessels in the macrocirculation which transport blood to and from the organs. One of the functions of microcirculation is to deliver oxygen and other nutrients to tissue. Sometimes, microcirculation in these small vessels can become blocked, interfering with the delivery of oxygen to the tissue.

SUMMARY

As placement of a physiological monitoring sensor is typically at a sensor site located at an extremity of the body, the state of microcirculation, such as whether vessels are blocked or open, can have a significant effect on the readings at the sensor site. It is therefore desirable to provide a patient monitor and/or physiological monitoring sensor capable of distinguishing the microcirculation state of blood vessels. In some embodiments, the patient monitor and/or sensor provide a warning and/or compensates a measurement based on the microcirculation state. In some embodiments, a microcirculation determination process implementable by the patient monitor and/or sensor is used to determine the state of microcirculation of the patient.

BRIEF DESCRIPTION OF THE DRAWINGS

Throughout the drawings, reference numbers may be re-used to indicate correspondence between referenced ele-

ments. The drawings are provided to illustrate embodiments of the disclosure described herein and not to limit the scope thereof.

FIG. 1 illustrates a block diagram of a patient monitor, such as a pulse oximeter, and associated sensor;

FIG. 2A is a schematic block diagram of a microcirculation monitoring device

FIG. 2B is a block illustrating an eyelid being monitored by a microcirculation monitoring device.

FIG. 3 illustrates a flow diagram for a process for determining the state of microcirculation usable by a pulse oximeter; and

FIG. 4 illustrates a flow diagram for a process for determining the state of microcirculation wherein multiple data points are collected.

DETAILED DESCRIPTION

FIG. 1 illustrates a block diagram of a patient monitor **100**, such as a microcirculation monitoring device, and associated non-invasive sensor **110**. Generally, in the case of a microcirculation monitoring device, the sensor **110** has a light source **112** and a photodiode detector **114**. In one embodiment, the light source **112** includes two LED emitters, generally one at a red wavelength and one at an infrared wavelength. In another embodiment, the light source **112** includes one light emitter that emits light at multiple wavelengths and a collimator and spectral filter. The sensor **110** can be attached to a patient in a number of different locations including a finger, an ear, an arm, a leg, a toe, a cheek, a lip, a tongue, a forehead, or an eyelid.

Typically, non-invasive sensors are attached to a finger, ear, forehead or cheek or other extremity. However, these locations can have a number of drawbacks. For example, signals measured at the ear can be very weak compared to other sites. In addition, cold temperatures can lead to poor perfusion at the ear. In some instances, the signal may be so weak that a non-invasive measurement is not feasible.

A non-invasive sensor placed at the finger can also have a number of disadvantages. Similar, to the ear, cold temperatures, or a cold patient, may result in poor perfusion at the finger. In addition, a patient experiencing shock may experience poor perfusion in the finger, as blood is directed away from the extremities and to the body's core during shock. Patient movement can also make it difficult to obtain accurate non-invasive readings at the finger.

Despite the disadvantages of measuring at fingers and ears, measuring oxygen saturation and monitoring microcirculation at the eyelid has a number of advantages. For example, similar to other parts of the head, the eyelids are generally well perfused. In addition, lower temperatures are less likely to effect perfusion in the eyelid than in the ear or finger. Furthermore, there is less likely to be patient movement at the eyelid than at a finger, resulting in more accurate readings. In addition, placement of a sensor on the head during surgery can decrease the probability of a cable obstructing access to the patient. The thickness of the eyelid (approximately 1 mm) can also be of benefit when using Optical Coherence Tomography (OCT) devices.

For an eyelid, the sensor **110** is configured so that the light source **112** projects light into the microvessels of the eyelid. The light source **112** is activated by drive signals **122** from the patient monitor **100**. The light entering the tissue is either absorbed, reflected, or refracted. After being reflected, some of the light returns in a direction that is substantially opposite from the direction it entered. The detector **114** is positioned in such a way so as to detect the reflected light as

it emerges from the eyelid tissues. The detector **114** generates a signal **124**, which is relayed by a cable or other means to the patient monitor **100**.

In one embodiment, the patient monitor **100** can include a pulse oximeter to determine oxygen saturation (SpO₂) by computing the differential absorption by arterial blood of the two wavelengths emitted by the LED emitters of the light source **112**. Additional information regarding the use of a pulse oximeter can be found in U.S. application Ser. No. 13/101,093, entitled "Patient Monitor for Determining Microcirculation State," filed May 4, 2011, and U.S. Pat. No. 7,356,365, issued Apr. 8, 2008, entitled "Method and Apparatus for Tissue Oximetry," both of which are hereby incorporated by reference in their entirety. The patient monitor can further include a sensor interface **120**, one or more processors **130**, such as a microcirculation processor, an instrument manager **140**, a display **150**, an audible indicator (tone generator) **160**, and a keypad **170**. The sensor interface **120** provides a light source drive current **122** which drives the light source **112**. The sensor interface **120** also has input circuitry for amplification and filtering of the signal **124** generated by the photodiode detector **114**, which corresponds to the light detected from the tissue after having been reflected and/or refracted by the eyelid. The microcirculation processor **130** calculates microcirculation states of the microvessels in the eyelid tissue, as will be described in greater detail below, and can also calculate the oxygen saturation, as described in greater detail in U.S. application Ser. No. 13/101,093 and U.S. Pat. No. 7,356,365, previously incorporated by reference in their entirety. The instrument manager **140** provides hardware and software interfaces for managing the display **150**, audible indicator **160**, and keypad **170**. The display **150** shows the computed oxygen saturation status, as described above, as well as the microcirculation status. The display **150** can also show an image of the microvessel. Similarly, other patient parameters including HbCO, HbMet, Hbt, Hct, oxygen concentrations, glucose concentrations, pulse rate, PI, SiQ, and/or PVI can be computed, as described in greater detail in U.S. application Ser. No. 13/101,093 and U.S. Pat. No. 7,356,365. The audible indicator **160** provides the pulse beep as well as alarms indicating desaturation and microcirculation events. The keypad **170** provides a user interface for such things as alarm thresholds, alarm enablement, and/or display options.

Computation of SpO₂ relies on the differential light absorption of oxygenated hemoglobin, HbO₂, and deoxygenated hemoglobin, Hb, to determine their respective concentrations in the arterial blood. Specifically, pulse oximetry measurements are made at red (R) and infrared (IR) wavelengths chosen such that deoxygenated hemoglobin absorbs more red light than oxygenated hemoglobin, and, conversely, oxygenated hemoglobin absorbs more infrared light than deoxygenated hemoglobin, for example 660 nm (R) and 905 nm (IR).

To distinguish between tissue absorption at the two wavelengths, in some embodiments, the red and infrared emitters of the light source **112** are provided drive current **122** so that only one is emitting light at a given time. For example, the emitters can be cycled on and off alternately, in sequence, with each only active for a quarter cycle and with a quarter cycle separating the active times. This allows for separation of red and infrared signals and removal of ambient light levels by downstream signal processing. Because only a single detector **114** is used, it responds to both the red and infrared emitted light and generates a time-division-multiplexed ("modulated") output signal **124**. This modulated signal **124** is coupled to the input of the sensor interface **120**.

In addition to the differential absorption of hemoglobin derivatives, pulse oximetry relies on the pulsatile nature of arterial blood to differentiate hemoglobin absorption from absorption of other constituents in the surrounding tissues. Light absorption between systole and diastole varies due to the blood volume change from the inflow and outflow of arterial blood at a peripheral tissue site. This tissue site might also comprise skin, muscle, bone, venous blood, fat, pigment, and/or the like, each of which absorbs light. It is assumed that the background absorption due to these surrounding tissues is invariant and can be ignored. Thus, blood oxygen saturation measurements are based upon a ratio of the time-varying or AC portion of the detected red and infrared signals with respect to the time-invariant or DC portion: $R/IR = (Red_{AC}/Red_{DC}) / (IR_{AC}/IR_{DC})$.

The desired SpO₂ measurement is then computed from this ratio. The relationship between R/IR and SpO₂ can be determined by statistical regression of experimental measurements obtained from human volunteers and calibrated measurements of oxygen saturation. In a pulse oximeter device, this empirical relationship can be stored as a "calibration curve" in a read-only memory (ROM) look-up table so that SpO₂ can be directly read-out of the memory in response to input R/IR measurements.

The patient monitor **100** can also measure perfusion index, PI, which is a numerical value that indicates the strength of the IR signal returned from a monitoring site and provides a relative assessment of the pulse strength at the monitoring site. The perfusion index can be defined as follows: $PI = (IR_{max} - IR_{min}) / IR_{DC}$, where IR_{max} is the maximum value, IR_{min} is the minimum value, and IR_{DC} is the average value of the invariant portion. As the light absorption characteristic of blood is typically "flatter" or less sensitive to oxygen saturation around the infrared wavelength, the infrared signal from a sensor is influenced primarily by the amount of the blood at the monitoring site, not by the level of oxygenation in the blood. Accordingly, the perfusion index, which is a numerical value that indicates the strength of the IR signal returned from a monitoring site, provides a relative assessment of the pulse strength at the monitoring site. PI values generally range from 0.02% (very weak pulse strength) to 20% (very strong pulse strength). In some embodiments, PI can be measured using other wavelengths. For example, red, near red, near IR, as well as other wavelengths can be used.

In an embodiment, the sensor **110** also includes a memory device **116**. The memory **116** can include any one or more of a wide variety of memory devices known to an artisan from the disclosure herein, including erasable programmable read-only memory (EPROM), electrically erasable programmable read-only memory (EEPROM), flash memory, other non-volatile memory, a combination of the same, or the like. The memory **116** can include a read-only device such as read-only memory (ROM), a read and write device such as random-access memory (RAM), combinations of the same, or the like. The remainder of the present disclosure will refer to such combination as simply EPROM for ease of disclosure; however, an artisan will recognize from the disclosure herein that the memory can include the ROM, the RAM, single wire memory, other types of memory, combinations of the same, or the like.

The memory device can advantageously store some or all of a wide variety data and information, including, for example, information on the type or operation of the sensor, type of patient or body tissue, buyer or manufacturer information, sensor characteristics including the number of wavelengths capable of being emitted, emitter specifica-

tions, emitter drive requirements, demodulation data, calculation mode data, calibration data, software such as scripts, executable code, or the like, sensor electronic elements, sensor life data indicating whether some or all sensor components have expired and should be replaced, encryption information, monitor or algorithm upgrade instructions or data, or the like. In an embodiment, the memory device can also include oxygen saturation to perfusion index and R/IR ratio to perfusion index ratios and/or data.

In certain situations, pulse oximetry sensors may produce anomalous readings, such as when a patient suffers from cyanosis. In a patient suffering from cyanosis, blood cells are uncharacteristically low on oxygen, leading to oxygen deficiency and giving the patient's skin a bluish-hue. One potential cause is that the patient's body produces too much hemoglobin, making the blood "thicker" or slower flowing, making microvessels more prone to blockage. Thus, a "blocked" microcirculation state can indicate cyanosis.

A "blocked" microcirculation state can also indicate other medical conditions, such as sepsis, systemic inflammatory response syndrome (SIRS), or septicemia. Sepsis is a potentially deadly medical condition that is characterized by a whole-body inflammatory state (called SIRS) and the presence of a known or suspected infection. The body may develop this inflammatory response by the immune system to microbes in the blood, urine, lungs, skin, or other tissue. Septicemia is a related medical term referring to the presence of pathogenic organisms in the bloodstream, which can lead to sepsis. Sepsis can also be referred to as blood poisoning. During sepsis or SIRS, inflammation in the body can cause constriction in blood vessels, leading to low blood pressure or insufficient blood flow.

During a "blocked" microcirculation state, blood cells can get blocked in the microvessels, such as the arterioles and capillaries. Blood cells can clump together or otherwise catch against the wall of blood vessels, creating a blockage that prevents blood cells, including red blood cells carrying hemoglobin, from passing through the blockage. However, plasma, which is composed of mostly water and in which the blood cells are suspended, is generally able to flow through passages in the blockage. In some situations, some blood vessels at the monitoring site may continue to have normal flow while some vessels are blocked. Thus, a "blocked" microcirculation state can indicate that some microvessels in an area are blocked and not necessarily all vessels in the area are blocked.

With the blockage preventing most or all the red blood cells from passing a blood vessel, at most only a limited amount of hemoglobin passes through a blocked blood vessel. In some situations, the blood vessel may only be partially blocked, where some hemoglobin passes through but less than when the blood vessel is unblocked. Normally, blood is made up of about 40-50% of red blood cells, of which about 95% is hemoglobin. Plasma, which is about 95% water, normally constitutes about 55% of the blood's volume.

Accordingly, a pulse oximeter sensor placed on a tissue site experiencing blockage in microcirculation vessels may detect mostly plasma passing through with no or only a small percentage of red blood cells, at least at part of the monitoring site. The resulting change in the normal composition of blood can cause anomalous readings in the patient monitor. As plasma has generally different absorption characteristics for red and infrared wavelengths than normal blood, pulse oximetry readings may become skewed. Red_{AC} and/or IR_{AC} can be affected, causing measured R/IR ratio to change. For example, if Red_{AC} rises or IR_{AC} drops,

the R/IR ratio increases. Alternatively, if Red_{AC} drops or IR_{AC} rises, the R/IR ratio decreases. Thus, the value of R/IR can change due to a change in the light absorption of blood even if the underlying oxygen saturation of the blood remains the same.

However, by comparing oxygen saturation and PI for normal microcirculation to the oxygen saturation and PI for blocked microcirculation, such as by calculating and comparing ratios, the monitor can determine the existence of an abnormal situation. Typically, SpO₂ is mostly independent of PI, with SpO₂ varying minimally as PI increases. However, SpO₂ varying by more than normal as PI increases can indicate an anomalous microcirculation state, such as a blockage. In one embodiment, by analyzing the measured ratios, the patient monitor 100 can determine the microcirculation state, such as whether a blocked vessel exists in the microvessels. Alternatively, multiple measurements of movement through the microvessels, such as the capillaries, can be used to determine the microcirculation state. For example, detected movement that is slower than normal can indicate blockage.

FIG. 2A is a schematic block diagram of a microcirculation monitoring device 200, which is described in greater detail in U.S. Pat. No. 7,356,365, previously incorporated by reference. The monitoring device 200 includes a light source 202, beam splitter 204, sample arm 206, imaging optics 208 in close proximity to the tissue 210, a reference arm 212, a reflector 214, a photodetector 216 and a patient monitor 218.

As described in greater detail in U.S. Pat. No. 7,356,365, the light source 202 can emit light having an approximately equal wavelength, a spectrum of wavelengths, or a few different wavelengths, e.g., two. The wavelengths can be selected based on the absorption spectrum of oxygenated hemoglobin and deoxygenated hemoglobin. For example, peak absorption for a oxygenated hemoglobin is approximately 940 nm and peak absorption for a deoxygenated hemoglobin is approximately 660 nm. Thus, wavelengths of 660 nm and 940 nm can be used. The light from the light source 202 is split by a beam splitter 204 between a sample arm 206 and a reference arm 212. Reflected signals from arms 206 and 212 interfere and are presented to photodetector 216 for measurement. Preferably, the end of the sample arm 206 can contain imaging optics 208 to tailor the spot size according to the tissue being measured. The imaging optics 208 can provide high coupling efficiency between the optical system and the tissue.

The tissue volume with which the light interacts (referred to as the interaction volume) is determined by the spot size of the imaging optics (surface area) and the coherence length of the light (depth). Reference arm 212 of the interferometer determines the phase shift applied to the reference beam which in turn determines which reflected light from the sample will constructively interfere with the shifted reference beam. Thus, the reference arm 212 determines the depth within the interaction volume from which scattered light is measured. The sample arm 206 can have either a fixed or scanning reflector 214 (such as a mirror). This can allow for a fixed sensor depth, adjustable sensor depth, or scan of multiple depths within the tissue.

The photodetector 216 measures the interference of the light from both the sample arm 206 and the reference arm 212. The patient monitor 218 uses the measured constructively interfered light at the different wavelengths to provide a measurement of the oxygen saturation, PI, and to monitor the microcirculation. Microcirculation measurements can

also be calculated by obtaining multiple images of the tissue site and analyzing the movement of blood cells between the images.

FIG. 2B illustrates a block drawing of an eyelid being monitored by a microcirculation monitoring device 200. As illustrated, light beams 250 from a light source 202 (FIG. 2A) are split using the beam splitter 204 into reference arm light beams 252 and sample arm light beams 254. After the light beams 250 are split, the reference arm light beams 252 travel down the reference arm 212 (FIG. 2A) to interact with the reflector 214 (FIG. 2A), and the sample arm light beams 254 travel down the sample arm 206 (FIG. 2A) to interact with the tissue from the upper eyelid 256. Although illustrated as interacting with the upper eyelid 256, it is to be understood that the lower eyelid 258 can also be used.

The upper eyelid 256 either absorbs, reflects and/or refracts the sample arm light beams 254. Some of the sample arm light beams 254 are reflected back to the beam splitter 212. The beam splitter 212 directs at least some of the reflected sample arm light beams 254 to the detector 216 (FIG. 2A).

The light beams traveling down the reference arm 212 (FIG. 2A) interact with a reflector 214 (FIG. 2A) and are reflected back to the beam splitter 212. Similar to the reflected sample arm light beams 254, the reflected reference arm light beams 252 are also directed to the detector 216 by the beam splitter 212. As discussed above, a patient monitor 200 (FIG. 2A) uses the detected signals obtained from the interference of the reflected sample arm light beams 254 and the reflected reference arm light beams 252 to calculate oxygen saturation, perfusion index and other physiological parameters. The patient monitor 200 (FIG. 2A) can also use the signals obtained from the detector 216 to monitor microcirculation in the eyelid. The microcirculation states can be monitored by comparing ratios of oxygen saturation and PI, as described in greater detail below, or comparing images obtained of the microvessels, as described above. If the microcirculation falls below a predetermined threshold, an alarm can be activated.

Although not illustrated in FIG. 2B, imaging optics 208 can also be used to focus the sample arm light beams 254 prior to interacting with the eyelids. Furthermore, the end of the sample arm 206 and imaging optics 208 can be placed in close proximity to the eyelid. In an embodiment, when a patient is unconscious, such as during a surgery, the end of the sample arm 206 and imaging optics 208 can be secured to the patient using an adhesive. The adhesive can attach to the patient's face, such as the cheek, forehead, ear or nose. Alternatively, the end of the sample arm 206 and imaging optics 208 can be fixedly attached to a pair of glasses or other device configured to cover a patient's eyes. The glasses or other device can be placed on the patient such that the sample arm light beams 254 interact with the eyelid tissue. The glasses or other placement device can be specially configured to ensure that the proper distance between the eyelid and the sample arm 206 and imaging optics 208 is achieved. The reference arm 212 and reflector 214 are configured and appropriate wavelength and polarization selected such that the appropriate depth of the eyelid tissue is measured.

Alternative designs can be used to monitor the microcirculation in an eyelid. For example, multiple images of a microvessel can be used to monitor the microcirculation. The images can be obtained using Optical Coherence Tomography (OCT), as is well known in the art. One method of obtaining images of microvessels is described in greater detail in U.S. application Ser. No. 11/524,866, entitled

“Microcirculation Imaging.” For example, a light source can output a beam of light having a broad spectrum of wavelengths. The beam of light can be collimated and pass through a spectral filter, and a beam splitter can split the light such that a beam of light having approximately one wavelength is directed towards microvessels of the eyelid. The light can be either polarized or non-polarized. A polarizer located on one edge of the beam splitter can polarize the light linearly, elliptically, or circularly, as desired. The wavelength and polarization of the light can be selected based on the desired measurement depth. The wavelength and polarization of the light can be altered using the spectral filter and/or polarizer. In one embodiment, the wavelength can be between 420 and 810 nm. In another embodiment, the wavelength can be in the light green spectrum (525-575 nm). The reflected light from the eyelid can be collected using a converging lens and a photodetector. A processor can use the signals from the photodetector to render an image of the eyelid tissue, or microvessels. Multiple images of the microvessels can be used to calculate the velocity of the microcirculation and detect blockage. For example, the distance traveled by the blood cells between measurements can be compared with the time between measurements to calculate velocity. If the velocity is below a certain threshold an alarm can be activated.

Other OCT methods can also be used to obtain images of the microvessels of the eyelid or other tissue. For example, multiple light emitters emitting different wavelengths of light can be used to obtain an image. Multiple images of the eyelid tissue can then be used by a patient monitor to calculate the velocity of the blood passing through the tissue, thereby monitoring the microcirculation of the eyelid.

FIG. 3 illustrates a flow diagram for a process 300 for determining the state of microcirculation usable by a pulse oximeter. Microcirculation state can be determined by comparison with microcirculation data stored on a patient monitor, such as the patient monitor 100 of FIG. 1. The process 300 can be implemented by embodiments of the sensor 110 and/or patient monitor 100 of FIG. 1 or other suitable device.

While in conventional pulse oximetry, measurements are generally taken pulse-by-pulse and averaged over pulses, microcirculation measurements can be measured using only a single pulse or a portion of a single pulse. This can be done, for example, at the minimum and/or maximum blood flow of a pulse. Microcirculation measurements can also be determined over multiple pulses. In some embodiments, microcirculation measurements are taken during a portion of the normal measurement time used by a physiological sensor to take a measurement of a parameter, thereby allowing detection of aberrant parameter measurements using the microcirculation measurements. For example, while a pulse oximeter is measuring SpO₂ over several pulses, microcirculation measurements can be taken per pulse and a warning given if an irregular microcirculation state is detected, thereby notifying a user of a possible aberration in the current SpO₂ reading.

At block 310, oxygen saturation is measured at a tissue monitoring site. In one embodiment, oxygen saturation is determined using a pulse oximeter sensor.

At block 320, perfusion index or pulse strength is measured. In one embodiment, the perfusion index is determined using the same sensor used to measure oxygen saturation so that readings are taken at the same monitoring site.

At block 330, a ratio of oxygen saturation to perfusion index is determined. Oxygen saturation can be a SpO₂ value based on the measured R/IR ratio looked-up against a calibration curve. Alternatively, the ratio can be perfusion

index to oxygen saturation. In other embodiments, the measured R/IR ratio can be used directly instead of SpO₂.

In some embodiments, multiple readings of perfusion index and oxygen saturation can be taken and averaged together before determining the ratio in order to account for outliers. The multiple readings can be filtered before averaging. For example, readings can first be filtered based on closeness of PI values before the readings are averaged together.

At block 340, the determined ratio in block 330 is compared to stored microcirculation data. The stored data can be data sets for microcirculation states. In some embodiments, a ratio, a curve, a line, table, data points, or formula can be stored that corresponds to a data set. The measured perfusion index and oxygen saturation can then be compared to the stored data. In some embodiments, multiple readings are taken and a best fit line or curve is generated and compared to a stored best fit line or curve. In some embodiments, readings are collected at various PI values in order to generate a trend line.

At block 350, the microcirculation state is determined from comparison of the stored microcirculation data. For example, if the determined ratio is similar to a stored ratio corresponding to a data set for unblocked microcirculation, the microcirculation state is determined to be unblocked. Other data sets for other microcirculation states, such as blocked and/or partially blocked can also be stored. Where multiple data sets are stored, the state can be determined by selecting the state corresponding to the stored ratio closest to the measured ratio.

At block 360, the monitor can optionally generate an alarm and/or display the microcirculation state. For example, an alarm signal and/or icon can be generated by the monitor to indicate that the readings may be anomalous, such as when a blocked or partially blocked microcirculation state is detected. The alarm can be a visual indicator (e.g., icon, message or image) and/or an audio indicator. In an embodiment, the alarm can indicate the detection of cyanosis, sepsis, SIRS or other medical condition based at least partly on the determined microcirculation state. In some embodiments, no action is taken, such as when readings are determined to be normal or non-threatening.

At block 370, the monitor can optionally compensate for the microcirculation state in order to improve accuracy of the readings. After the microcirculation state returns to normal, the compensation process can be ended.

In one embodiment, an offset can be added to the measured parameter value, such as SpO₂. The offset can be calculated based on data sets for microcirculation state. Different microcirculation states can have different offsets. For example, if a “blocked” microcirculation state produces high readings for low PI values, a negative offset can be used. However, if a “blocked” state produces a low value for high PI values, then a positive offset can be used. In one embodiment, a varying offset can be used depending on the value of PI.

In one embodiment, a different wavelength emitter can be used to compensate for a microcirculation state. For example, rather than using a regular infrared emitter, typically 905 nm, an emitter with a different infrared wavelength, such as 970 nm can be used. In one embodiment, the different wavelength is selected such that the wavelength is at a “flat” section of the light absorption curve for plasma, that is, where the light absorption is not much affected by changes in oxygen saturation, as described in greater detail in U.S. application Ser. No. 13/101,093. In one embodiment, the selected wavelength with regards to plasma mimics the

properties of the regular wavelength with regards to normal flowing blood. In some embodiments, a different wavelength red emitter can be used instead of the regular red wavelength emitter.

In some embodiments, the pulse oximeter sensor used to measure oxygen saturation and PI can be provided with an additional emitter at a different wavelength than the existing emitters. When a certain microcirculation state is detected, such as a “blocked” state, the additional emitter can be used. For example, a pulse oximetry sensor can be equipped with LED’s capable of emitting at 660 nm, 905 nm, and at 970 nm wavelengths. Under normal operation, the 660 nm and 905 nm emitters are active. However, upon detecting a blocked microcirculation state, the 905 nm emitter can be deactivated and the 970 nm emitter activated in its place. In some embodiments, a variable wavelength emitter can be used rather than separate emitters. In some embodiments, the additional emitter can be a red wavelength emitter.

FIG. 4 illustrates a flow diagram for a process 400 for determining the state of microcirculation wherein multiple data points are collected. The process 400 can be implemented by embodiments of the sensor 110 and/or patient monitor 100 of FIG. 1 or other suitable device.

At block 410 and block 420, oxygen saturation and perfusion index are measured. At block 425, measured values are stored in memory. Each paired measurement forms a data point.

At block 430, the number of stored data points is checked to determine if sufficient data has been collected to determine the microcirculation state. Data can be sufficient if a set number of data points have been collected, a set amount of time has passed, and/or a spectrum of data points have been collected, such as for differing values of PI.

At block 440, the stored measured data is compared with stored microcirculation data. Typically, the microcirculation data is pre-stored on the pulse oximeter before use, as opposed to collected during use. A comparison can involve generating a curve or line from the measured data, calculating a rate of change for the stored data, generating a trend line for the measured data or the like and comparing with the stored microcirculation data.

At block 450, the microcirculation state is determined from comparison of the stored microcirculation data. For example, if the measured data is similar to microcirculation data corresponding to a data set for unblocked microcirculation, the microcirculation state is determined to be unblocked. Other data sets for other microcirculation states, such as for blocked and/or partially blocked can also be stored. Where multiple data sets are stored, the state can be determined by selecting the state corresponding to the stored ratio closest to the measured ratio.

Blocks 460 and 470 are similar to steps 360 and 370 described in FIG. 3.

As will be apparent from the above description, the R/IR ratio corresponds to oxygen saturation or SpO₂ and can be used in place of oxygen saturation or SpO₂ for the above comparisons, and vice versa.

While the above systems and methods have been described in terms of oxygen saturation and PI, other physiological parameters can be measured in place of or in addition to oxygen saturation and/or perfusion index and used to determine microcirculation state. For example, perfusion index is an indication of amplitude and/or signal strength and other parameters or measurements indicating amplitude and/or signal strength can be used. In some embodiments, one or more different sensors can be used in place of or in addition to a pulse oximeter sensor.

In another embodiment, the microcirculation state can be calculated without calculating oxygen saturation. For example, using OCT, as described above, multiple measurements of the movement of blood within the microvessels can be taken. The multiple measurements can then be compared to determine the velocity of the blood traveling through the microvessels. For example, the distance traveled by the blood between measurements can be compared with the time between measurements to calculate velocity. In one embodiment, images of the microvessels are used to measure the movement of blood in the microvessels.

Conditional language used herein, such as, among others, “can,” “could,” “might,” “may,” “e.g.,” and the like, unless specifically stated otherwise, or otherwise understood within the context as used, is generally intended to convey that certain embodiments include, while other embodiments do not include, certain features, elements and/or states. Thus, such conditional language is not generally intended to imply that features, elements and/or states are in any way required for one or more embodiments or that one or more embodiments necessarily include logic for deciding, with or without author input or prompting, whether these features, elements and/or states are included or are to be performed in any particular embodiment. The terms “comprising,” “including,” “having,” and the like are synonymous and are used inclusively, in an open-ended fashion, and do not exclude additional elements, features, acts, operations, and so forth. Also, the term “or” is used in its inclusive sense (and not in its exclusive sense) so that when used, for example, to connect a list of elements, the term “or” means one, some, or all of the elements in the list.

Various systems and processes for determining microcirculation events have been disclosed in detail in connection with various embodiments. These embodiments are disclosed by way of examples only and are not to limit the scope of the claims that follow. Indeed, the novel methods and systems described herein can be embodied in a variety of other forms; furthermore, various omissions, substitutions and changes in the form of the methods and systems described herein can be made without departing from the spirit of the inventions disclosed herein. The claims and their equivalents are intended to cover such forms or modifications as would fall within the scope and spirit of certain of the inventions disclosed herein. One of ordinary skill in the art will appreciate the many variations, modifications and combinations. For example, the various embodiments of the microcirculation determination process can be used with oxygen saturation sensors and with both disposable and reusable sensors. In some embodiments, the determination process can be applied to other blood vessels to detect a blockage, even in vessels not involved in microcirculation.

Furthermore, in certain embodiments, the systems and methods described herein can advantageously be implemented using computer software, hardware, firmware, or any combination of software, hardware, and firmware. In one embodiment, the system includes a number of software modules that comprise computer executable code for performing the functions described herein. In certain embodiments, the computer-executable code is executed on one or more general purpose computers or processors. However, a skilled artisan will appreciate, in light of this disclosure, that any module that can be implemented using software can also be implemented using a different combination of hardware, software or firmware. For example, such a module can be implemented completely in hardware using a combination of integrated circuits. Alternatively or additionally, such a module can be implemented completely or partially using

specialized computers or processors designed to perform the particular functions described herein rather than by general purpose computers or processors.

Moreover, certain embodiments of the invention are described with reference to methods, apparatus (systems) and computer program products that can be implemented by computer program instructions. These computer program instructions can be provided to a processor of a general purpose computer, special purpose computer, or other programmable data processing apparatus to produce a machine, such that the instructions, which execute via the processor of the computer or other programmable data processing apparatus, create means for implementing the acts specified herein to transform data from a first state to a second state.

Each of the processes, methods, and algorithms described in the preceding sections may be embodied in, and fully or partially automated by, code modules executed by one or more computers or computer processors. The code modules may be stored on any type of non-transitory computer-readable medium or computer storage device, such as hard drives, solid state memory, optical disc, and/or the like. The processes and algorithms may be implemented partially or wholly in application-specific circuitry. The results of the disclosed processes and process steps may be stored, persistently or otherwise, in any type of non-transitory computer storage such as, e.g., volatile or non-volatile storage.

The various features and processes described above may be used independently of one another, or may be combined in various ways. All possible combinations and subcombinations are intended to fall within the scope of this disclosure. In addition, certain method or process blocks may be omitted in some implementations. The methods and processes described herein are also not limited to any particular sequence, and the blocks or states relating thereto can be performed in other sequences that are appropriate. For example, described blocks or states may be performed in an order other than that specifically disclosed, or multiple blocks or states may be combined in a single block or state. The example blocks or states may be performed in serial, in parallel, or in some other manner. Blocks or states may be added to or removed from the disclosed example embodiments. The example systems and components described herein may be configured differently than described. For example, elements may be added to, removed from, or rearranged compared to the disclosed example embodiments.

While certain example embodiments have been described, these embodiments have been presented by way of example only, and are not intended to limit the scope of the inventions disclosed herein. Thus, nothing in the foregoing description is intended to imply that any particular feature, characteristic, step, module, or block is necessary or indispensable. Indeed, the novel methods and systems described herein may be embodied in a variety of other forms; furthermore, various omissions, substitutions and changes in the form of the methods and systems described herein may be made without departing from the spirit of the inventions disclosed herein. The accompanying claims and their equivalents are intended to cover such forms or modifications as would fall within the scope and spirit of certain of the inventions disclosed herein.

What is claimed is:

1. A method for monitoring a patient and non-invasively determining a microcirculation state at an eyelid of the patient, the method comprising:

receiving, from a non-invasive physiological sensor, a signal responsive to light of at least a first wavelength

and a second wavelength that is transmitted by the non-invasive physiological sensor and detected by the non-invasive physiological sensor after the light interacts with tissue of an eyelid of a patient;

processing the signal to determine at least:

a first parameter indicative of a measure of perfusion of the tissue of the eyelid of the patient, and

a second parameter responsive to at least a ratio of the detected light at the first wavelength and the second wavelength;

determining a relationship between the first parameter and the second parameter;

comparing the determined relationship with at least some of a plurality of stored relationships corresponding to one or more microcirculation states; and

determining a microcirculation state at the eyelid based at least in part on the comparing the determined relationship with the at least some of the plurality of stored relationships.

2. The method of claim 1, wherein the second parameter comprises oxygen saturation and the first parameter comprises a perfusion index.

3. The method of claim 1, wherein the plurality of stored relationships comprises previously determined and stored relationships between first parameters and second parameters.

4. The method of claim 1, wherein at least some of the plurality of stored relationships correspond to an at least partially blocked microcirculation condition.

5. The method of claim 1, wherein at least some of the plurality of stored relationships correspond to an unblocked microcirculation condition.

6. The method of claim 1, wherein when the comparing indicates that the determined relationship is similar to at least one of the plurality of stored relationships, wherein at least one of the plurality of stored relationships corresponds to an at least partially blocked microcirculation condition.

7. The method of claim 1, wherein the microcirculation state at the eyelid comprises an at least partially blocked microcirculation state in at least a portion of blood vessels at the eyelid.

8. The method of claim 1, further comprising providing an electronic microcirculation condition warning.

9. The method of claim 1, causing the non-invasive physiological sensor to transmit at least a portion of the light at a wavelength that is different from the first wavelength and the second wavelength.

10. The method of claim 1, applying an offset to at least one of the first parameter or the second parameter to compensate for the microcirculation state at the eyelid.

11. A patient monitor, comprising:

a sensor interface configured to receive a signal from a physiological sensor, wherein the physiological sensor is configured to transmit light of at least a first wavelength and a second wavelength into tissue of an eyelid of a patient and to detect the light after it interacts with the tissue of the eyelid of the patient, wherein the signal is responsive to the detected light; and

one or more processors configured to:

determine a first parameter indicative of a measure of perfusion of the tissue of the eyelid of the patient and a second parameter responsive to at least a ratio of the detected light at the first wavelength and the second wavelength,

determine a relationship between the first parameter and the second parameter,

15

compare the determined relationship with at least some of a plurality of previously determined relationships corresponding to one or more microcirculation states, and

determine a microcirculation state at the eyelid based at least in part on the comparison of the determined relationship with the at least some of the plurality of previously determined relationships.

12. The patient monitor of claim 11, further comprising a memory storing the plurality of previously determined relationships, wherein the plurality of previously determined relationships comprise relationships between previously determined first parameters and previously determined second parameters.

13. The patient monitor of claim 11, wherein the second parameter comprises oxygen saturation and the first parameter comprises a perfusion index.

14. The patient monitor of claim 11, wherein at least some of the plurality of previously determined relationships correspond to an at least partially blocked microcirculation condition.

15. The patient monitor of claim 11, wherein at least some of the plurality of previously determined relationships correspond to an unblocked microcirculation condition.

16. The patient monitor of claim 11, wherein the comparison indicates that the determined relationship is similar

16

to at least one of the previously determined relationships, wherein the at least one of the previously determined relationships corresponds to an at least partially blocked microcirculation condition.

5 17. The patient monitor of claim 11, wherein the microcirculation state at the eyelid comprises an at least partially blocked microcirculation state in at least a portion of blood vessels at the eyelid.

10 18. The patient monitor of claim 11, wherein the processor is further configured to provide an electronic microcirculation condition warning.

15 19. The patient monitor of claim 11, wherein the processor is further configured to cause the physiological sensor to transmit at least a portion of the light at a wavelength that is different from the first wavelength and the second wavelength.

20 20. The patient monitor of claim 11, wherein the processor is further configured to apply an offset to at least one of the first parameter or the second parameter to compensate for the microcirculation state at the eyelid.

21. The patient monitor of claim 11, wherein the first wavelength comprises a red wavelength and the second wavelength comprises an infrared wavelength.

* * * * *

专利名称(译)	用于监测微循环的患者监测器		
公开(公告)号	US10271749	公开(公告)日	2019-04-30
申请号	US15/797839	申请日	2017-10-30
[标]申请(专利权)人(译)	梅西莫股份有限公司		
申请(专利权)人(译)	Masimo公司		
当前申请(专利权)人(译)	Masimo公司		
[标]发明人	KIANI MASSI JOE E		
发明人	KIANI, MASSI JOE E.		
IPC分类号	A61B5/1455 A61B5/026 A61B5/00		
CPC分类号	A61B5/0261 A61B5/7271 A61B5/14551		
优先权	61/446969 2011-02-25 US		
其他公开文献	US20180184917A1		
外部链接	Espacenet		

摘要(译)

能够测量组织部位处的微循环的患者监视器包括光源，分束器，光电检测器和患者监视器。从光源发出的光被分成参考臂和样品臂。样品臂中的光指向组织部位，例如眼睑。来自组织部位的反射光受到来自参考臂的光的干扰。光电探测器测量来自样品臂和参考臂的光的干涉。患者监视器使用来自光电探测器的测量值来计算组织部位处的氧饱和度并监测组织部位处的微循环。

