



US009820665B2

(12) **United States Patent**
Felix et al.

(10) **Patent No.:** **US 9,820,665 B2**
(45) **Date of Patent:** **Nov. 21, 2017**

(54) **REMOTE INTERFACING OF EXTENDED WEAR ELECTROCARDIOGRAPHY AND PHYSIOLOGICAL SENSOR MONITOR**

(56) **References Cited**

U.S. PATENT DOCUMENTS

(71) Applicant: **Bardy Diagnostics, Inc.**, Charlotte, NC (US)

3,215,136 A 11/1965 Holler et al.
3,699,948 A 10/1972 Ota et al.
(Continued)

(72) Inventors: **Jason Felix**, Vashon Island, WA (US);
Jon Mikalson Bishay, Seattle, WA (US);
Gust H. Bardy, Carnation, WA (US)

FOREIGN PATENT DOCUMENTS

DE 19955211 5/2001
EP 1859833 11/2007
(Continued)

(73) Assignee: **Bardy Diagnostics, Inc.**, Charlotte, NC (US)

OTHER PUBLICATIONS

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

US 6,527,714, 03/2003, Bardy (withdrawn)
(Continued)

(21) Appl. No.: **15/256,266**

Primary Examiner — George Manuel

(22) Filed: **Sep. 2, 2016**

(74) *Attorney, Agent, or Firm* — Patrick J.S. Inouye;
Krista A. Wittman

(65) **Prior Publication Data**

US 2016/0367164 A1 Dec. 22, 2016

Related U.S. Application Data

(63) Continuation of application No. 14/082,071, filed on Nov. 15, 2013, now Pat. No. 9,433,367, which is a (Continued)

(57) **ABSTRACT**

A remotely-interfaceable extended wear electrocardiography and physiological sensor monitor recorder is provided. A sealed housing forms on a bottom surface a cavity shaped to accommodate an upward projection of a battery compartment formed on a non-conductive receptacle of a disposable extended wear electrode patch and includes a set of electrical contacts that protrude from the bottom surface and are arranged in alignment with electrical pads provided on the non-conductive receptacle. Electronic circuitry is provided within the sealed housing and includes an externally-powered micro-controller operable to execute under micro-programmable control. An electrocardiographic front end circuit is electrically interfaced to the micro-controller. A wireless transceiver electrically interfaces with the micro-controller and externally-powered flash memory is electrically interfaced with the micro-controller and operable to store samples of the electrocardiographic signals.

(51) **Int. Cl.**

A61B 5/00 (2006.01)

A61B 5/0432 (2006.01)

(Continued)


(52) **U.S. Cl.**

CPC **A61B 5/04325** (2013.01); **A61B 5/0006** (2013.01); **A61B 5/0022** (2013.01);
(Continued)

(58) **Field of Classification Search**

CPC A61B 2560/0214; A61B 5/0006; A61B 5/0022; A61B 5/02055; A61B 5/021;
(Continued)

18 Claims, 8 Drawing Sheets

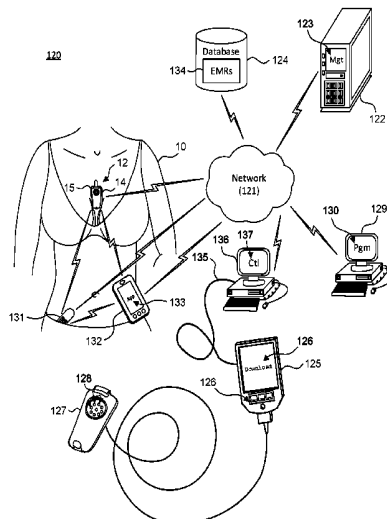

Related U.S. Application Data

- continuation-in-part of application No. 14/080,717, filed on Nov. 14, 2013, now Pat. No. 9,545,204, said application No. 14/082,071 is a continuation-in-part of application No. 14/080,725, filed on Nov. 14, 2013, now Pat. No. 9,730,593.
- (60) Provisional application No. 61/882,403, filed on Sep. 25, 2013.
- (51) **Int. Cl.**
A61B 5/0408 (2006.01)
A61B 5/0205 (2006.01)
A61B 5/145 (2006.01)
A61B 5/021 (2006.01)
A61B 5/03 (2006.01)
A61B 5/0452 (2006.01)
A61B 5/11 (2006.01)
A61B 5/1455 (2006.01)
A61B 5/08 (2006.01)
A61B 5/087 (2006.01)
- (52) **U.S. Cl.**
 CPC *A61B 5/02055* (2013.01); *A61B 5/04085* (2013.01); *A61B 5/04087* (2013.01); *A61B 5/14532* (2013.01); *A61B 5/14542* (2013.01); *A61B 5/6823* (2013.01); *A61B 5/7405* (2013.01); *A61B 5/7455* (2013.01); *A61B 5/7475* (2013.01); *A61B 5/021* (2013.01); *A61B 5/03* (2013.01); *A61B 5/0452* (2013.01); *A61B 5/087* (2013.01); *A61B 5/1118* (2013.01); *A61B 5/14551* (2013.01); *A61B 2560/0214* (2013.01)
- (58) **Field of Classification Search**
 CPC ... *A61B 5/03*; *A61B 5/04085*; *A61B 5/04087*; *A61B 5/04325*; *A61B 5/0452*; *A61B 5/0816*; *A61B 5/087*; *A61B 5/1118*; *A61B 5/14532*; *A61B 5/14542*; *A61B 5/14551*; *A61B 5/6823*; *A61B 5/7405*; *A61B 5/7455*; *A61B 5/7475*
 See application file for complete search history.
- (56) **References Cited**
 U.S. PATENT DOCUMENTS
- | | | | | | |
|-------------|---------|------------------|--------------|---------|------------------|
| 3,893,453 A | 7/1975 | Goldberg | 5,511,553 A | 4/1996 | Segalowitz |
| 4,123,785 A | 10/1978 | Cherry et al. | 5,540,733 A | 7/1996 | Testerman et al. |
| 4,328,814 A | 5/1982 | Arkans | 5,546,952 A | 8/1996 | Erickson |
| 4,441,500 A | 4/1984 | Sessions et al. | 5,549,655 A | 8/1996 | Erickson |
| 4,532,934 A | 8/1985 | Kelen | 5,579,919 A | 12/1996 | Gilman et al. |
| 4,550,502 A | 11/1985 | Grayzel | 5,582,181 A | 12/1996 | Ruess |
| 4,716,903 A | 1/1988 | Hansen | D377,983 S | 2/1997 | Sabri et al. |
| 4,809,705 A | 3/1989 | Ascher | 5,601,089 A | 2/1997 | Bledsoe et al. |
| 4,915,656 A | 4/1990 | Alferness | 5,623,935 A | 4/1997 | Faisandier |
| 5,025,794 A | 6/1991 | Albert et al. | 5,682,901 A | 11/1997 | Kamen |
| 5,168,876 A | 12/1992 | Quedens et al. | 5,697,955 A | 12/1997 | Stolte |
| 5,215,098 A | 6/1993 | Steinhaus | 5,749,902 A | 5/1998 | Olsen et al. |
| D341,423 S | 11/1993 | Bible | 5,817,151 A | 10/1998 | Olsen et al. |
| 5,265,579 A | 11/1993 | Ferrari | 5,819,741 A | 10/1998 | Karlsson et al. |
| 5,341,806 A | 8/1994 | Gadsby et al. | 5,850,920 A | 12/1998 | Gilman et al. |
| 5,355,891 A | 10/1994 | Wateridge et al. | D407,159 S | 3/1999 | Roberg |
| 5,365,934 A | 11/1994 | Leon et al. | 5,876,351 A | 3/1999 | Rohde |
| 5,392,784 A | 2/1995 | Gudaitis | 5,906,583 A | 5/1999 | Rogel |
| D357,069 S | 4/1995 | Plahn et al. | 5,951,598 A | 9/1999 | Bishay et al. |
| 5,402,780 A | 4/1995 | Faasse, Jr. | 5,957,857 A | 9/1999 | Hartley |
| 5,402,884 A | 4/1995 | Gilman et al. | 5,984,102 A | 11/1999 | Tay |
| 5,450,845 A | 9/1995 | Axelgaard | 6,032,064 A | 2/2000 | Devlin et al. |
| 5,458,141 A | 10/1995 | Neil | 6,038,469 A | 3/2000 | Karlsson et al. |
| 5,473,537 A | 12/1995 | Glazer et al. | 6,101,413 A | 8/2000 | Olsen et al. |
| 5,483,969 A | 1/1996 | Testerman et al. | 6,115,638 A | 9/2000 | Groenke |
| | | | 6,117,077 A | 9/2000 | Del Mar et al. |
| | | | 6,134,479 A | 10/2000 | Brewer et al. |
| | | | 6,148,233 A | 11/2000 | Owen et al. |
| | | | 6,149,602 A | 11/2000 | Arcelus |
| | | | 6,149,781 A | 11/2000 | Forand |
| | | | 6,188,407 B1 | 2/2001 | Smith et al. |
| | | | D443,063 S | 5/2001 | Pisani et al. |
| | | | 6,245,025 B1 | 6/2001 | Torok et al. |
| | | | 6,246,330 B1 | 6/2001 | Nielsen |
| | | | D445,507 S | 7/2001 | Pisani et al. |
| | | | 6,269,267 B1 | 7/2001 | Bardy et al. |
| | | | 6,272,385 B1 | 8/2001 | Bishay et al. |
| | | | 6,298,255 B1 | 10/2001 | Cordero et al. |
| | | | 6,301,502 B1 | 10/2001 | Owen et al. |
| | | | 6,304,773 B1 | 10/2001 | Taylor et al. |
| | | | 6,304,780 B1 | 10/2001 | Owen et al. |
| | | | 6,304,783 B1 | 10/2001 | Lyster et al. |
| | | | 6,374,138 B1 | 4/2002 | Owen et al. |
| | | | 6,416,471 B1 | 7/2002 | Kumar et al. |
| | | | 6,418,342 B1 | 7/2002 | Owen et al. |
| | | | 6,424,860 B1 | 7/2002 | Karlsson et al. |
| | | | 6,427,083 B1 | 7/2002 | Owen et al. |
| | | | 6,456,872 B1 | 9/2002 | Faisandier |
| | | | 6,463,320 B1 | 10/2002 | Xue et al. |
| | | | 6,546,285 B1 | 4/2003 | Owen et al. |
| | | | 6,605,046 B1 | 8/2003 | Del Mar |
| | | | 6,607,485 B2 | 8/2003 | Bardy |
| | | | 6,611,705 B2 | 8/2003 | Hopman et al. |
| | | | 6,671,545 B2 | 12/2003 | Fincke |
| | | | 6,671,547 B2 | 12/2003 | Lyster et al. |
| | | | 6,694,186 B2 | 2/2004 | Bardy |
| | | | 6,704,595 B2 | 3/2004 | Bardy |
| | | | 6,705,991 B2 | 3/2004 | Bardy |
| | | | 6,719,701 B2 | 4/2004 | Lade |
| | | | 6,754,523 B2 | 6/2004 | Toole |
| | | | 6,782,293 B2 | 8/2004 | Dupelle et al. |
| | | | 6,856,832 B1 | 2/2005 | Matsumura et al. |
| | | | 6,860,897 B2 | 3/2005 | Bardy |
| | | | 6,866,629 B2 | 3/2005 | Bardy |
| | | | 6,887,201 B2 | 5/2005 | Bardy |
| | | | 6,893,397 B2 | 5/2005 | Bardy |
| | | | 6,904,312 B2 | 6/2005 | Bardy |
| | | | 6,908,431 B2 | 6/2005 | Bardy |
| | | | 6,913,577 B2 | 7/2005 | Bardy |
| | | | 6,944,498 B2 | 9/2005 | Owen et al. |
| | | | 6,960,167 B2 | 11/2005 | Bardy |
| | | | 6,970,731 B1 | 11/2005 | Jayaraman et al. |
| | | | 6,978,169 B1 | 12/2005 | Guerra |
| | | | 6,993,377 B2 | 1/2006 | Flick et al. |
| | | | 7,020,508 B2 | 3/2006 | Stivoric et al. |
| | | | 7,027,864 B2 | 4/2006 | Snyder et al. |
| | | | 7,065,401 B2 | 6/2006 | Worden |
| | | | 7,085,601 B1 | 8/2006 | Bardy et al. |
| | | | 7,104,955 B2 | 9/2006 | Bardy |

(56)

References Cited

| U.S. PATENT DOCUMENTS | | | | | | |
|-----------------------|----|---------|---------------------|--------------|------------|---------------------|
| 7,134,996 | B2 | 11/2006 | Bardy | 2002/0184055 | A1 12/2002 | Naghavi et al. |
| 7,137,389 | B2 | 11/2006 | Berthon-Jones | 2002/0193668 | A1 12/2002 | Munneke |
| 7,147,600 | B2 | 12/2006 | Bardy | 2003/0004547 | A1 1/2003 | Owen et al. |
| 7,215,991 | B2 | 5/2007 | Besson et al. | 2003/0073916 | A1 4/2003 | Yonce |
| 7,248,916 | B2 | 7/2007 | Bardy | 2003/0083559 | A1 5/2003 | Thompson |
| 7,257,438 | B2 | 8/2007 | Kinast | 2003/0097078 | A1 5/2003 | Maeda |
| 7,277,752 | B2 | 10/2007 | Matos | 2003/0139785 | A1 7/2003 | Riff et al. |
| D558,882 | S | 1/2008 | Brady | 2003/0176802 | A1 9/2003 | Galen et al. |
| 7,328,061 | B2 | 2/2008 | Rowlandson et al. | 2003/0211797 | A1 11/2003 | Hill et al. |
| 7,412,395 | B2 | 8/2008 | Rowlandson et al. | 2004/0008123 | A1 1/2004 | Carrender |
| 7,429,938 | B1 | 9/2008 | Corndorf | 2004/0019288 | A1 1/2004 | Kinast |
| 7,552,031 | B2 | 6/2009 | Vock et al. | 2004/0034284 | A1 2/2004 | Aversano et al. |
| D606,656 | S | 12/2009 | Kobayashi et al. | 2004/0049132 | A1 3/2004 | Barron et al. |
| 7,706,870 | B2 | 4/2010 | Shieh et al. | 2004/0073127 | A1 4/2004 | Istvan et al. |
| 7,756,721 | B1 | 7/2010 | Falchuk et al. | 2004/0087836 | A1 5/2004 | Green et al. |
| 7,787,943 | B2 | 8/2010 | McDonough | 2004/0093192 | A1 5/2004 | Hasson et al. |
| 7,874,993 | B2 | 1/2011 | Bardy | 2004/0148194 | A1 7/2004 | Wellons et al. |
| 7,881,785 | B2 | 2/2011 | Nassif et al. | 2004/0207530 | A1 10/2004 | Nielsen |
| D639,437 | S | 6/2011 | Bishay et al. | 2004/0236202 | A1 11/2004 | Burton |
| 7,959,574 | B2 | 6/2011 | Bardy | 2004/0243435 | A1 12/2004 | Williams |
| 8,116,841 | B2 | 2/2012 | Bly et al. | 2004/0256453 | A1 12/2004 | Lammle |
| 8,150,502 | B2 | 4/2012 | Kumar et al. | 2004/0260188 | A1 12/2004 | Syed et al. |
| 8,160,682 | B2 | 4/2012 | Kumar et al. | 2004/0260192 | A1 12/2004 | Yamamoto |
| 8,172,761 | B1 | 5/2012 | Rulkov et al. | 2005/0096717 | A1 5/2005 | Bishay et al. |
| 8,180,425 | B2 | 5/2012 | Selvitelli et al. | 2005/0108055 | A1 5/2005 | Ott et al. |
| 8,200,320 | B2 | 6/2012 | Kovacs | 2005/0154267 | A1 7/2005 | Bardy |
| 8,231,539 | B2 | 7/2012 | Bardy | 2005/0182308 | A1 8/2005 | Bardy |
| 8,231,540 | B2 | 7/2012 | Bardy | 2005/0182309 | A1 8/2005 | Bardy |
| 8,239,012 | B2 | 8/2012 | Felix et al. | 2005/0215918 | A1 9/2005 | Frantz et al. |
| 8,249,686 | B2 | 8/2012 | Libbus et al. | 2005/0228243 | A1 10/2005 | Bardy |
| 8,260,414 | B2 | 9/2012 | Nassif et al. | 2005/0245839 | A1 11/2005 | Stivoric et al. |
| 8,266,008 | B1 | 9/2012 | Siegal et al. | 2006/0025696 | A1 2/2006 | Kurzweil et al. |
| 8,277,378 | B2 | 10/2012 | Bardy | 2006/0025824 | A1 2/2006 | Freeman et al. |
| 8,285,356 | B2 | 10/2012 | Bly et al. | 2006/0030767 | A1 2/2006 | Lang et al. |
| 8,285,370 | B2 | 10/2012 | Felix et al. | 2006/0041201 | A1 2/2006 | Behbehani et al. |
| 8,308,650 | B2 | 11/2012 | Bardy | 2006/0122469 | A1 6/2006 | Martel |
| 8,366,629 | B2 | 2/2013 | Bardy | 2006/0124193 | A1 6/2006 | Orr et al. |
| 8,374,688 | B2 | 2/2013 | Libbus et al. | 2006/0224072 | A1 10/2006 | Shennib |
| 8,412,317 | B2 | 4/2013 | Mazar | 2006/0235320 | A1 10/2006 | Tan et al. |
| 8,460,189 | B2 | 6/2013 | Libbus et al. | 2006/0253006 | A1 11/2006 | Bardy |
| 8,473,047 | B2 | 6/2013 | Chakravarthy et al. | 2006/0264730 | A1 11/2006 | Stivoric et al. |
| 8,478,418 | B2 | 7/2013 | Fahey | 2006/0264767 | A1 11/2006 | Shennib |
| 8,554,311 | B2 | 10/2013 | Warner et al. | 2007/0003115 | A1 1/2007 | Patton et al. |
| 8,591,430 | B2 | 11/2013 | Amurthur et al. | 2007/0038057 | A1 2/2007 | Nam et al. |
| 8,594,763 | B1 | 11/2013 | Bibian et al. | 2007/0050209 | A1 3/2007 | Yered |
| 8,600,486 | B2 | 12/2013 | Kaib et al. | 2007/0078324 | A1 4/2007 | Wijisiriwardana |
| 8,613,708 | B2 | 12/2013 | Bishay et al. | 2007/0093719 | A1 4/2007 | Nichols, Jr. et al. |
| 8,613,709 | B2 | 12/2013 | Bishay et al. | 2007/0100248 | A1 5/2007 | Van Dam et al. |
| 8,620,418 | B1 | 12/2013 | Kuppuraj et al. | 2007/0100667 | A1 5/2007 | Bardy |
| 8,626,277 | B2 | 1/2014 | Felix et al. | 2007/0123801 | A1 5/2007 | Goldberger et al. |
| 8,668,653 | B2 | 3/2014 | Nagata et al. | 2007/0136091 | A1 6/2007 | McTaggart |
| 8,684,925 | B2 | 4/2014 | Manicka et al. | 2007/0179357 | A1 8/2007 | Bardy |
| 8,688,190 | B2 | 4/2014 | Libbus et al. | 2007/0185390 | A1 8/2007 | Perkins et al. |
| 8,718,752 | B2 | 5/2014 | Libbus et al. | 2007/0203415 | A1 8/2007 | Bardy |
| 8,744,561 | B2 | 6/2014 | Fahey | 2007/0203423 | A1 8/2007 | Bardy |
| 8,774,932 | B2 | 7/2014 | Fahey | 2007/0208232 | A1 9/2007 | Kovacs |
| 8,790,257 | B2 | 7/2014 | Libbus et al. | 2007/0208233 | A1 9/2007 | Kovacs |
| 8,790,259 | B2 | 7/2014 | Katra et al. | 2007/0208266 | A1 9/2007 | Hadley |
| 8,795,174 | B2 | 8/2014 | Manicka et al. | 2007/0225611 | A1 9/2007 | Kumar et al. |
| 8,798,729 | B2 | 8/2014 | Kaib et al. | 2007/0244405 | A1 10/2007 | Xue et al. |
| 8,798,734 | B2 | 8/2014 | Kuppuraj et al. | 2007/0249946 | A1 10/2007 | Kumar et al. |
| 8,818,478 | B2 | 8/2014 | Scheffler et al. | 2007/0255153 | A1 11/2007 | Kumar et al. |
| 8,818,481 | B2 | 8/2014 | Bly et al. | 2007/0265510 | A1 11/2007 | Bardy |
| 8,823,490 | B2 | 9/2014 | Libbus et al. | 2007/0276270 | A1 11/2007 | Tran |
| 8,938,287 | B2 | 1/2015 | Felix et al. | 2007/0276275 | A1 11/2007 | Proctor et al. |
| 8,965,492 | B2 | 2/2015 | Baker et al. | 2007/0293738 | A1 12/2007 | Bardy |
| 9,066,664 | B2 | 6/2015 | Karjalainen | 2007/0293739 | A1 12/2007 | Bardy |
| 9,155,484 | B2 | 10/2015 | Baker et al. | 2007/0293740 | A1 12/2007 | Bardy |
| 9,204,813 | B2 | 12/2015 | Kaib et al. | 2007/0293741 | A1 12/2007 | Bardy |
| 9,277,864 | B2 | 3/2016 | Yang et al. | 2007/0293772 | A1 12/2007 | Bardy |
| 9,339,202 | B2 | 5/2016 | Brockway et al. | 2007/0293772 | A1 12/2007 | Bardy |
| 2002/0013538 | A1 | 1/2002 | Teller | 2007/0299325 | A1 12/2007 | Farrell et al. |
| 2002/0013717 | A1 | 1/2002 | Ando et al. | 2007/0299617 | A1 12/2007 | Willis |
| 2002/0103422 | A1 | 8/2002 | Harder et al. | 2007/0299617 | A1 12/2007 | Willis |
| 2002/0120310 | A1 | 8/2002 | Linden et al. | 2008/0051668 | A1 2/2008 | Bardy |
| | | | | 2008/0058661 | A1 3/2008 | Bardy |
| | | | | 2008/0091097 | A1 4/2008 | Linti et al. |
| | | | | 2008/0108890 | A1 5/2008 | Teng et al. |
| | | | | 2008/0139953 | A1 6/2008 | Baker et al. |
| | | | | 2008/0143080 | A1 6/2008 | Burr |
| | | | | 2008/0177168 | A1 7/2008 | Callahan et al. |

(56)

References Cited

U.S. PATENT DOCUMENTS

2008/0194927 A1 8/2008 KenKnight et al.
 2008/0208009 A1 8/2008 Shklarski
 2008/0208014 A1 8/2008 KenKnight et al.
 2008/0284599 A1 11/2008 Zdeblick et al.
 2008/0288026 A1 11/2008 Cross et al.
 2008/0306359 A1 12/2008 Zdeblick et al.
 2009/0054952 A1 2/2009 Glukhovsky et al.
 2009/0062897 A1 3/2009 Axelgaard
 2009/0069867 A1 3/2009 KenKnight et al.
 2009/0073991 A1 3/2009 Landrum et al.
 2009/0076336 A1 3/2009 Mazar et al.
 2009/0076341 A1 3/2009 James et al.
 2009/0076342 A1 3/2009 Amurthur et al.
 2009/0076343 A1 3/2009 James et al.
 2009/0076346 A1 3/2009 James et al.
 2009/0076349 A1 3/2009 Libbus et al.
 2009/0076397 A1 3/2009 Libbus et al.
 2009/0076401 A1 3/2009 Mazar et al.
 2009/0076559 A1 3/2009 Libbus et al.
 2009/0088652 A1 4/2009 Tremblay
 2009/0112116 A1 4/2009 Lee et al.
 2009/0131759 A1 5/2009 Sims et al.
 2009/0216132 A1 8/2009 Orbach
 2009/0264792 A1 10/2009 Mazar
 2009/0270708 A1 10/2009 Shen et al.
 2009/0270747 A1 10/2009 Van Dam et al.
 2009/0292194 A1 11/2009 Libbus et al.
 2010/0007413 A1 1/2010 Herleikson et al.
 2010/0022897 A1 1/2010 Parker et al.
 2010/0056881 A1 3/2010 Libbus et al.
 2010/0081913 A1 4/2010 Cross et al.
 2010/0185063 A1 7/2010 Bardy
 2010/0185076 A1 7/2010 Jeong et al.
 2010/0191154 A1 7/2010 Berger et al.
 2010/0191310 A1 7/2010 Bly
 2010/0234715 A1 9/2010 Shin et al.
 2010/0234716 A1 9/2010 Engel
 2010/0280366 A1 11/2010 Arne et al.
 2010/0324384 A1 12/2010 Moon et al.
 2011/0021937 A1 1/2011 Hugh et al.
 2011/0054286 A1 3/2011 Crosby et al.
 2011/0066041 A1 3/2011 Pandia et al.
 2011/0077497 A1 3/2011 Oster et al.
 2011/0144470 A1 6/2011 Mazar et al.
 2011/0160548 A1 6/2011 Forster et al.
 2011/0224564 A1 9/2011 Moon et al.
 2011/0237924 A1 9/2011 McGusty et al.
 2011/0245699 A1 10/2011 Snell et al.
 2011/0245711 A1 10/2011 Katra et al.
 2012/0003933 A1 1/2012 Baker et al.
 2012/0029306 A1 2/2012 Paquet et al.
 2012/0029315 A1* 2/2012 Raptis A61B 5/0022
 600/301
 2012/0029316 A1 2/2012 Raptis et al.
 2012/0035432 A1 2/2012 Katra et al.
 2012/0088998 A1 4/2012 Bardy et al.
 2012/0088999 A1 4/2012 Bishay et al.
 2012/0089000 A1 4/2012 Bishay et al.
 2012/0089001 A1 4/2012 Bishay et al.
 2012/0089037 A1 4/2012 Bishay et al.
 2012/0089412 A1 4/2012 Bardy et al.
 2012/0089417 A1 4/2012 Bardy et al.
 2012/0095352 A1 4/2012 Tran
 2012/0101358 A1 4/2012 Boettcher et al.
 2012/0101396 A1 4/2012 Solosko et al.
 2012/0165645 A1 6/2012 Russell et al.
 2012/0172695 A1 7/2012 Ko et al.
 2012/0302906 A1 11/2012 Felix et al.
 2013/0041272 A1 2/2013 Guillen Arredondo et al.
 2013/0077263 A1 3/2013 Oleson et al.
 2013/0079611 A1 3/2013 Besko
 2013/0085403 A1 4/2013 Gunderson et al.
 2013/0096395 A1 4/2013 Katra et al.
 2013/0116533 A1 5/2013 Lian et al.
 2013/0123651 A1 5/2013 Bardy

2013/0158361 A1 6/2013 Bardy
 2013/0225963 A1 8/2013 Kodandaramaiah et al.
 2013/0225966 A1 8/2013 Macia Barber et al.
 2013/0243105 A1 9/2013 Lei et al.
 2013/0274584 A1 10/2013 Finlay et al.
 2013/0275158 A1 10/2013 Fahey
 2013/0324809 A1 12/2013 Lisogurski et al.
 2013/0324855 A1 12/2013 Lisogurski et al.
 2013/0324856 A1 12/2013 Lisogurski et al.
 2013/0325359 A1 12/2013 Jarverud et al.
 2013/0331665 A1 12/2013 Libbus et al.
 2013/0338448 A1 12/2013 Libbus et al.
 2013/0338472 A1 12/2013 Macia Barber et al.
 2014/0012154 A1 1/2014 Mazar et al.
 2014/0140359 A1 5/2014 Kalevo et al.
 2014/0189928 A1 7/2014 Oleson et al.
 2014/0206977 A1 7/2014 Bahney et al.
 2014/0215246 A1 7/2014 Lee et al.
 2014/0358193 A1 12/2014 Lyons et al.
 2015/0048836 A1 2/2015 Guthrie et al.
 2015/0065842 A1 3/2015 Lee et al.
 2015/0257670 A1 9/2015 Ortega et al.
 2015/0359489 A1 12/2015 Baudenbacher et al.
 2016/0217691 A1 7/2016 Kadobayashi et al.

FOREIGN PATENT DOCUMENTS

EP 2438851 4/2012
 EP 2438852 4/2012
 EP 2465415 6/2012
 EP 2589333 5/2013
 JP H06319711 11/1994
 JP 2004129788 4/2004
 WO 0078213 12/2000
 WO 03032192 4/2003
 WO 2006009767 1/2006
 WO 2006014806 2/2006
 WO 2007066270 6/2007
 WO 2007092543 8/2007
 WO 2008010216 1/2008
 WO 2008057884 5/2008
 WO 2009036306 3/2009
 WO 2009036313 3/2009
 WO 2009036327 3/2009
 WO 2009112976 9/2009
 WO 2009112978 9/2009
 WO 2009112979 9/2009
 WO 2009142975 11/2009
 WO 2010066507 6/2010
 WO 2010105045 9/2010
 WO 2011047207 4/2011
 WO 2012140559 10/2012
 WO 2012146957 11/2012

OTHER PUBLICATIONS

15 of the Hottest Wearable Gadgets, URL <<http://thehottestgadgets.com/2008/09/the-15-hottest-wearable-gadgets-001253>> (Web page cached on Sep. 27, 2008).
 AliveCor's Heart Monitor for iPhone Receives FDA Clearance, URL <<http://www.businesswire.com/news/home/20121203005545/en/AliveCor%E2%80%99s-Heart-Monitor-iPhone-Receives-FDA-Clearance#U7rtq7FVtyF>> (Dec. 3, 2012).
 Bharadwaj et al., Techniques for Accurate ECG signal processing, EE Times, URL <www.eetimes.com/document.asp?doc_id=1278571> (Feb. 14, 2011).
 Chen et al., "Monitoring Body Temperature of Newborn Infants at Neonatal Intensive Care Units Using Wearable Sensors," BodyNets 2010, Corfu Island, Greece. (Sep. 10, 2010).
 Epstein, Andrew E. et al.; ACC/AHA/HRS 2008 Guidelines for Device-Based Therapy of Cardiac Rhythm Abnormalities. J. Am. Coll. Cardiol. 2008; 51; e1-e62, 66 Pgs.
 Fitbit automatically tracks your fitness and sleep, URL <<http://www.fitbit.com/>> (Web page cached on Sep. 10, 2008).
 Smith, Kevin, "Jawbone Up VS. Fitbit Flex: Which Is the Best Fitness Band?" URL <<http://www.businessinsider.com/fitbit-flex-vs-jawbone-up-2013-5?op=1>> (Jun. 1, 2013).

(56)

References Cited

OTHER PUBLICATIONS

Kligfield, Paul et al., Recommendations for the Standardization and Interpretation of the Electrocardiogram: Part I. *J.Am.Coll. Cardiol*; 2007; 49; 1109-27, 75 Pgs.

Lauren Gravitz, "When Your Diet Needs a Band-Aid," *Technology Review*, MIT. (May 1, 2009).

Lieberman, Jonathan, "How Telemedicine Is Aiding Prompt ECG Diagnosis in Primary Care," *British Journal of Community Nursing*, vol. 13, No. 3, Mar. 1, 2008 (Mar. 1, 2008), pp. 123-126, XP009155082, ISSN: 1462-4753.

McManus et al., "A Novel Application for the Detection of an Irregular Pulse using an iPhone 4S in Patients with Atrial Fibrillation," vol. 10(3), pp. 315-319 (Mar. 2013).

Nike+ Fuel Band, URL <http://www.nike.com/us/en_us/c/nikeplus-fuelband> (Web page cached on Jan. 11, 2013).

P. Libby et al., "Braunwald's Heart Disease—A Textbook of Cardiovascular Medicine," Chs. 11, pp. 125-148 and 12, pp. 149-193 (8th ed. 2008), American Heart Association.

Initial hands-on with Polar Loop activity tracker, URL <<http://www.drainmaker.com/2013/09/polar-loop-firstlook.html>> (Sep. 17, 2013).

Sittig et al., "A Computer-Based Outpatient Clinical Referral System," *International Journal of Medical Informatics*, Shannon, IR, vol. 55, No. 2, Aug. 1, 1999, pp. 149-158, X0004262434, ISSN: 1386-5056(99)00027-1.

Sleepview, URL <<http://www.clevedmed.com/sleepview/overview.shtml>> (Web pages cached on Feb. 23, 2010, Dec. 29, 2012 and Sep. 4, 2013).

Actigraphy/ Circadian Rhythm SOMNOWatch, URL <<http://www.somnomedics.eu/news-events/publications/somnowatchtm.html>> (Web page cached on Jan. 23, 2010).

Zio Event Card, URL <<http://www.irhythmtech.com/zio-solution/zio-event/>> (Web page cached on Mar. 11, 2013).

Zio Patch System, URL <<http://www.irhythmtech.com/zio-solution/zio-system/index.html>> (Web page cached on Sep. 8, 2013).

Libbus. "Adherent Cardiac Monitor With Wireless Fall Detection for Patients With Unexplained Syncope." Abstracts of the First AMA-IEEE Medical Technology Conference on Individualized Healthcare. May 22, 2010.

Daoud et al. "Fall Detection Using Shimmer Technology and Multiresolution Analysis." Aug. 2, 2013. URL: <https://decibel.ni.com/content/docs/DOC-26652>.

Chan et al. "Wireless Patch Sensor for Remote Monitoring of Heart Rate, Respiration, Activity, and Falls." pp. 6115-6118. 2013 35th Annual International Conference of the IEEE Engineering in Medical and Biology Society. Jul. 1, 2013.

Saadi et al. "Heart Rhythm Analysis Using ECG Recorded With a Novel Sternum Based Patch Technology—A Pilot Study." *Cardio technix 2013—Proceedings of the International Congress on Cardiovascular Technologies*, Sep. 20, 2013.

Anonymous. "Omegawave Launches Consumer App 2.0 in U.S. Endurance Sportswire—Endurance Sportswire." Jul. 11, 2013. URL:<http://endurancesportswire.com/omegawave-launches-consumer-app-2-0-in-u-s/>.

Duttweiler et al., "Probability Estimation in Arithmetic and Adaptive-Huffman Entropy Coders," *IEEE Transactions on Image Processing*, vol. 4, No. 3, Mar. 1, 1995, pp. 237-246.

Gupta et al., "An ECG Compression Technique for Telecardiology Application," *India Conference (INDICON), 2011 Annual IEEE*, Dec. 16, 2011, pp. 1-4.

Nave et al., "ECG Compression Using Long-Term Prediction," *IEEE Transactions on Biomedical Engineering*, IEEE Service Center, NY, USA, vol. 40, No. 9, Sep. 1, 1993, pp. 877-885.

Skretting et al., "Improved Huffman Coding Using Recursive Splitting," *NORSIG*, Jan. 1, 1999.

A Voss et al., "Linear and Nonlinear Methods for Analyses of Cardiovascular Variability in Bipolar Disorders," *Bipolar Disorders*, vol. 8, No. 5p1, Oct. 1, 2006, pp. 441-452, XP55273826, DK ISSN: 1398-5647, DOI: 10.1111/i.1399-5618.2006.00364.x.

"Varicrad-Kardi Software User's Manual Rev. 1.1", Jul. 8, 2009 (Jul. 8, 2009), XP002757888, retrieved from the Internet: URL:<http://www.ehrlich.tv/KARDiVAR-Software.pdf> [retrieved on May 20, 2016].

http://www.originlab.com/origin#Data_Exploration.

<https://web.archive.org/web/20130831204020/http://www.biopac.com/research.asp?CatID=37&Main=Software> (Aug. 2013).

<http://www.gtec.at/Products/Software/g.BSanalyze-Specs-Features> (2014).

ADInstruments:ECG Analysis Module for LabChart & PowerLab, 2008.

BIOPAC Systems, Inc. #AS148-Automated ECG Analysis, Mar. 24, 2006.

* cited by examiner

Fig. 1.

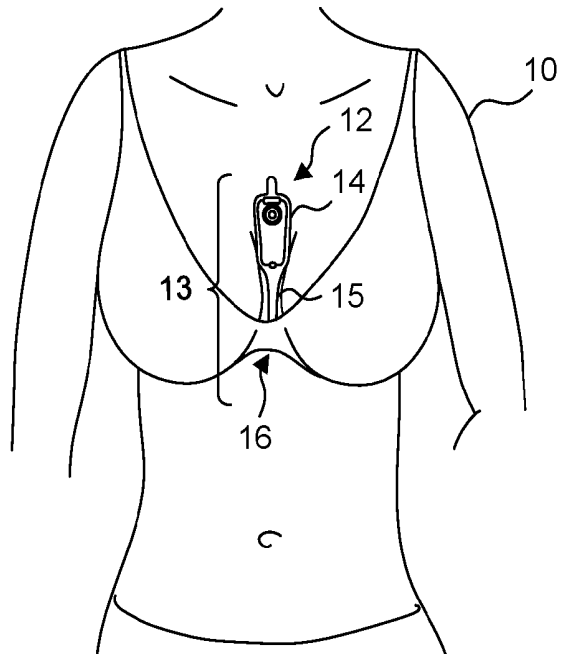


Fig. 2.

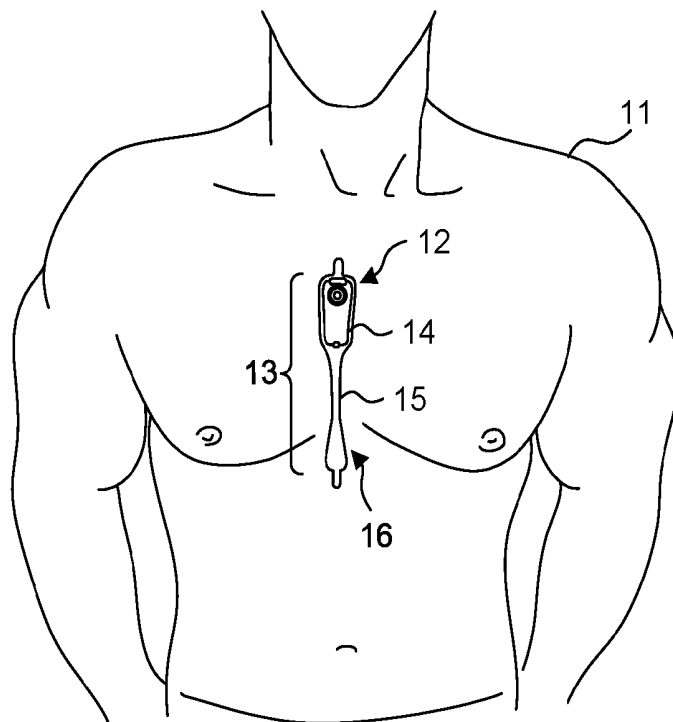


Fig. 3.

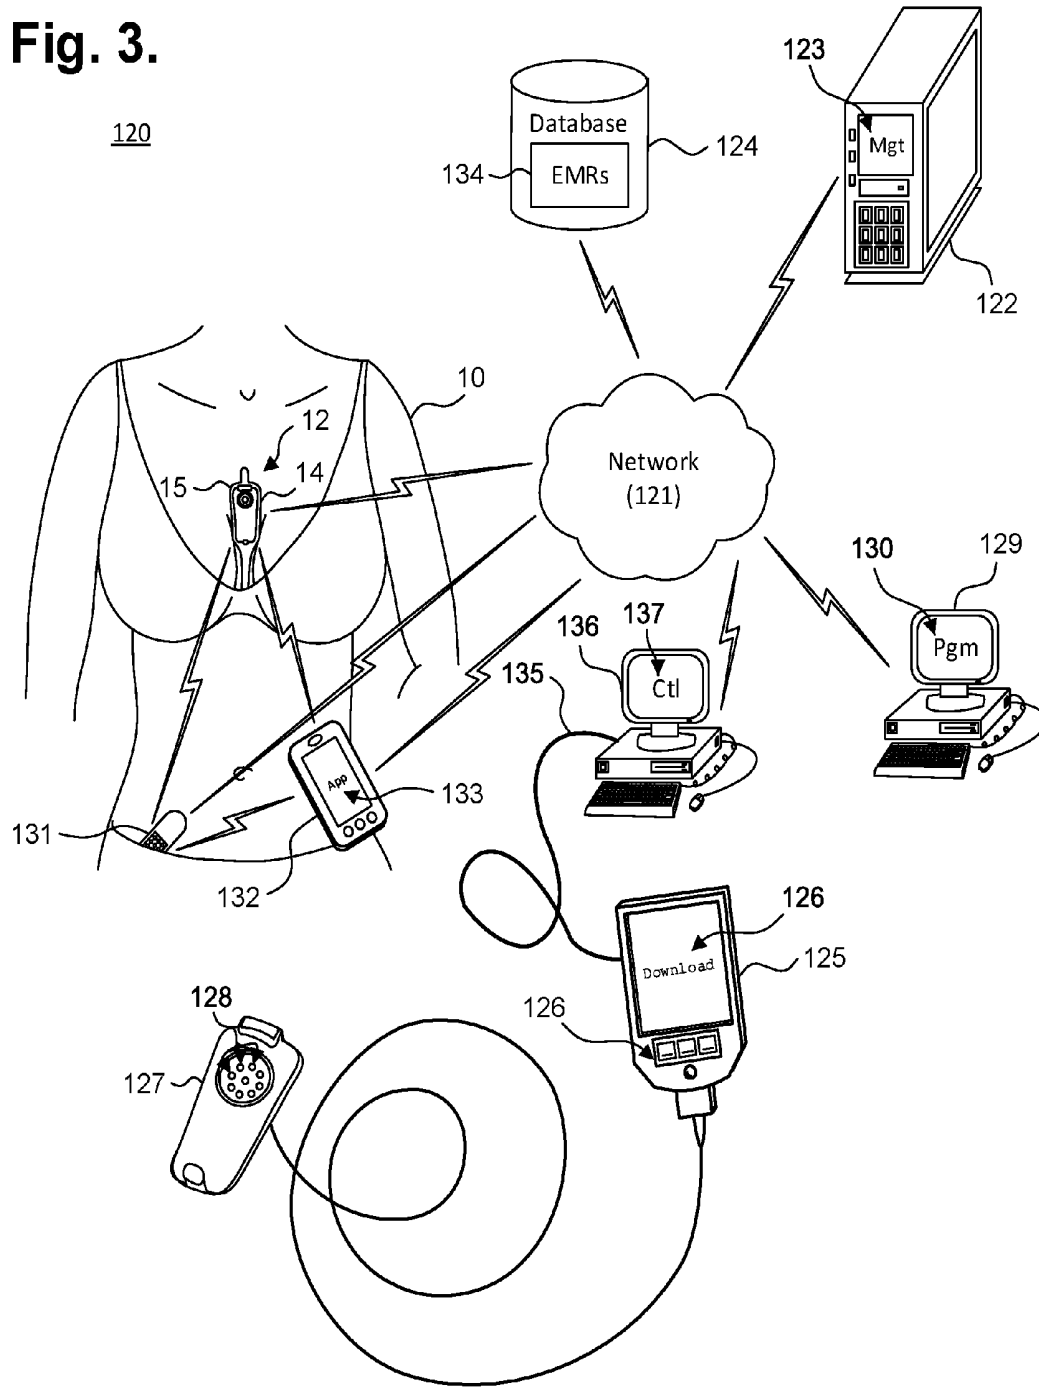


Fig. 4.

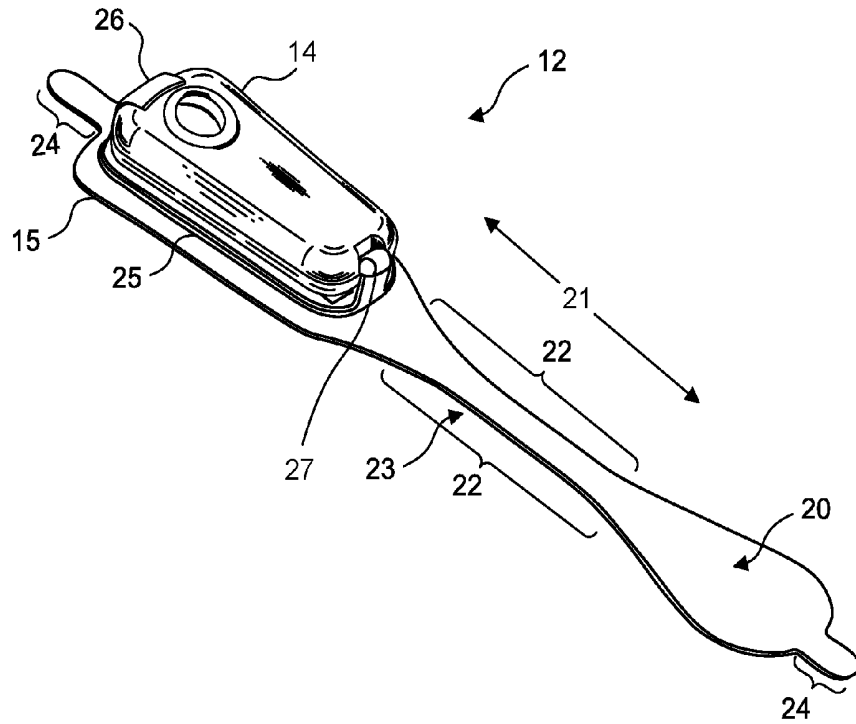


Fig. 5.

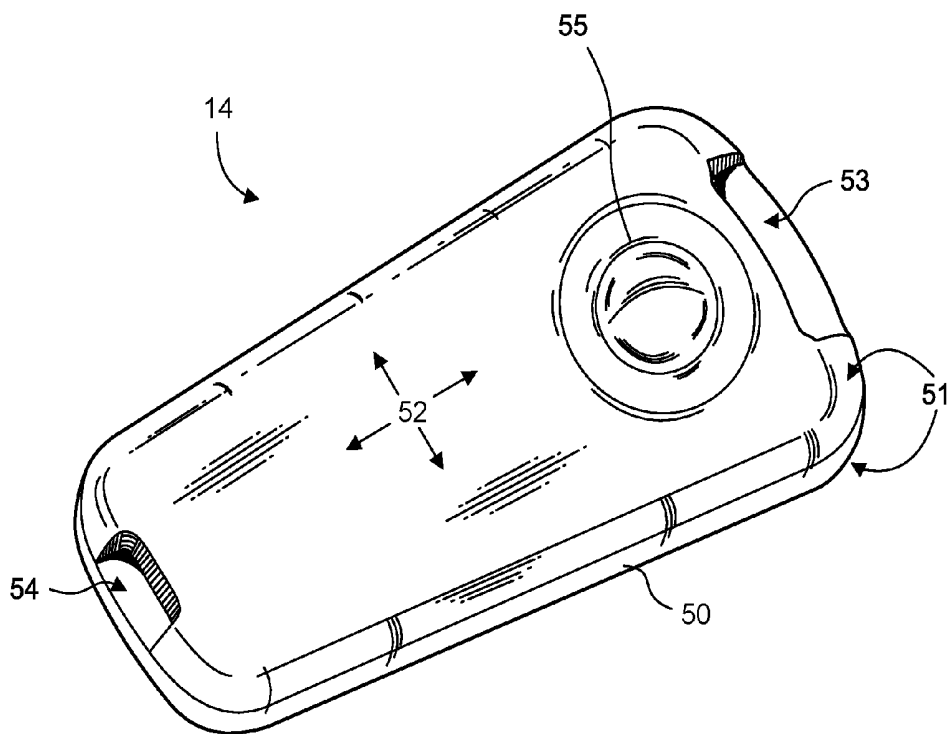


Fig. 6.

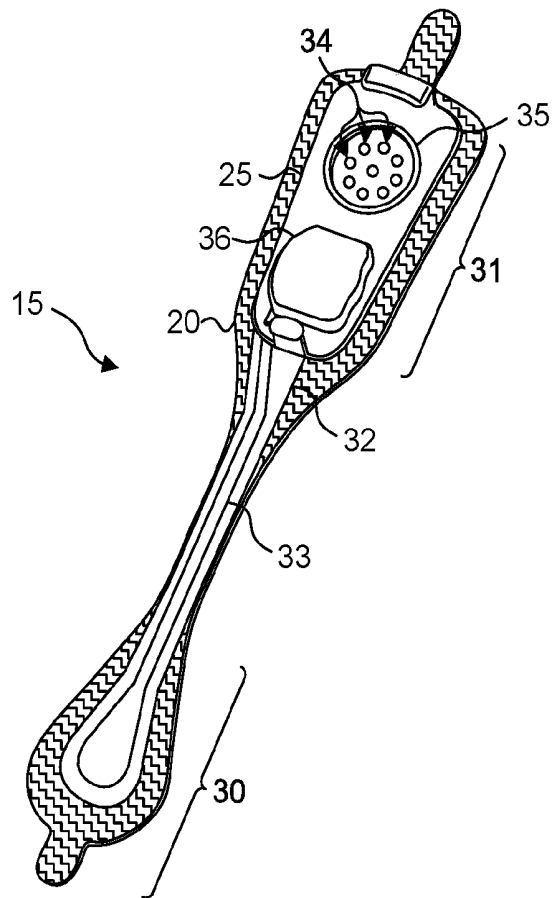


Fig. 7.

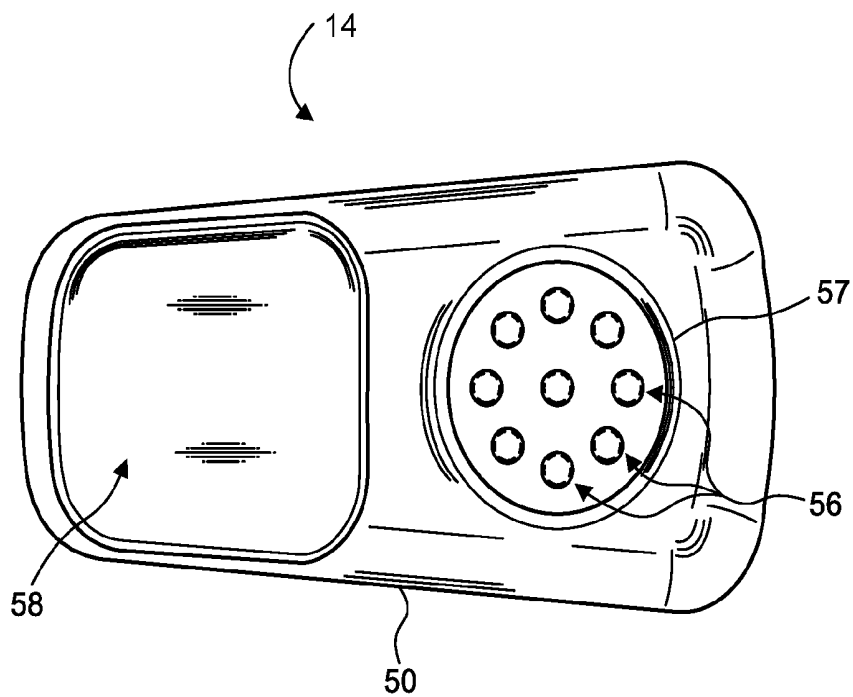


Fig. 8.

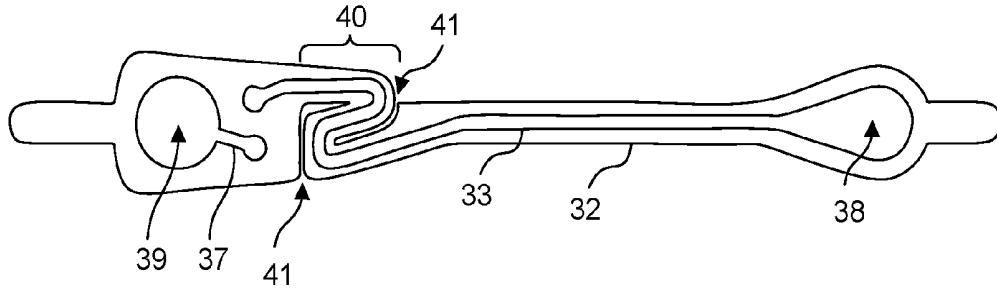


Fig. 9.

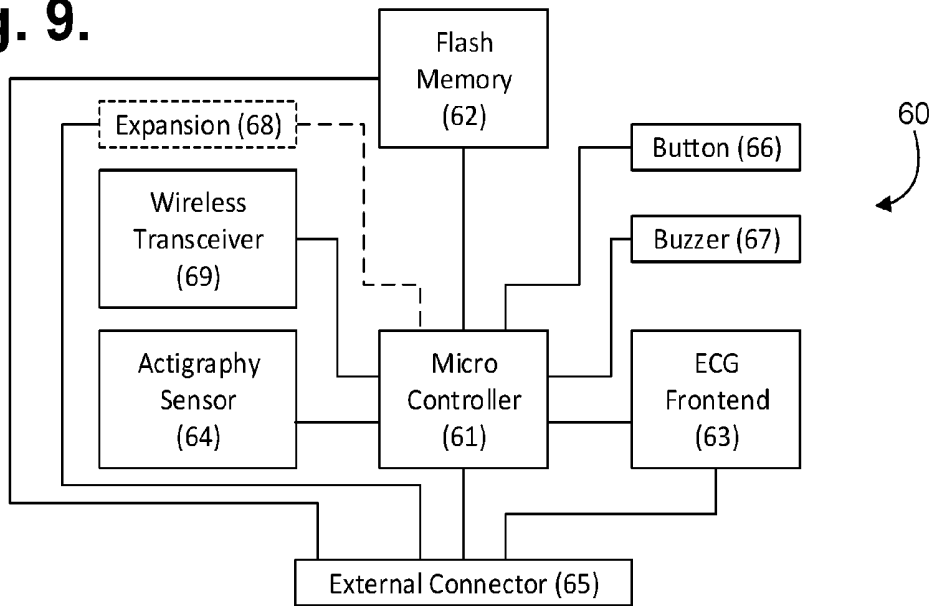


Fig. 10.

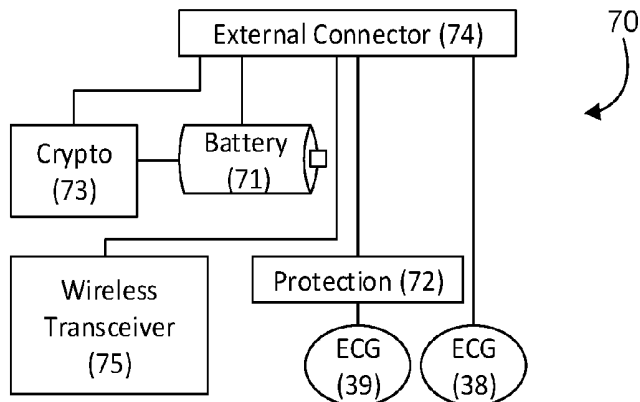


Fig. 11.

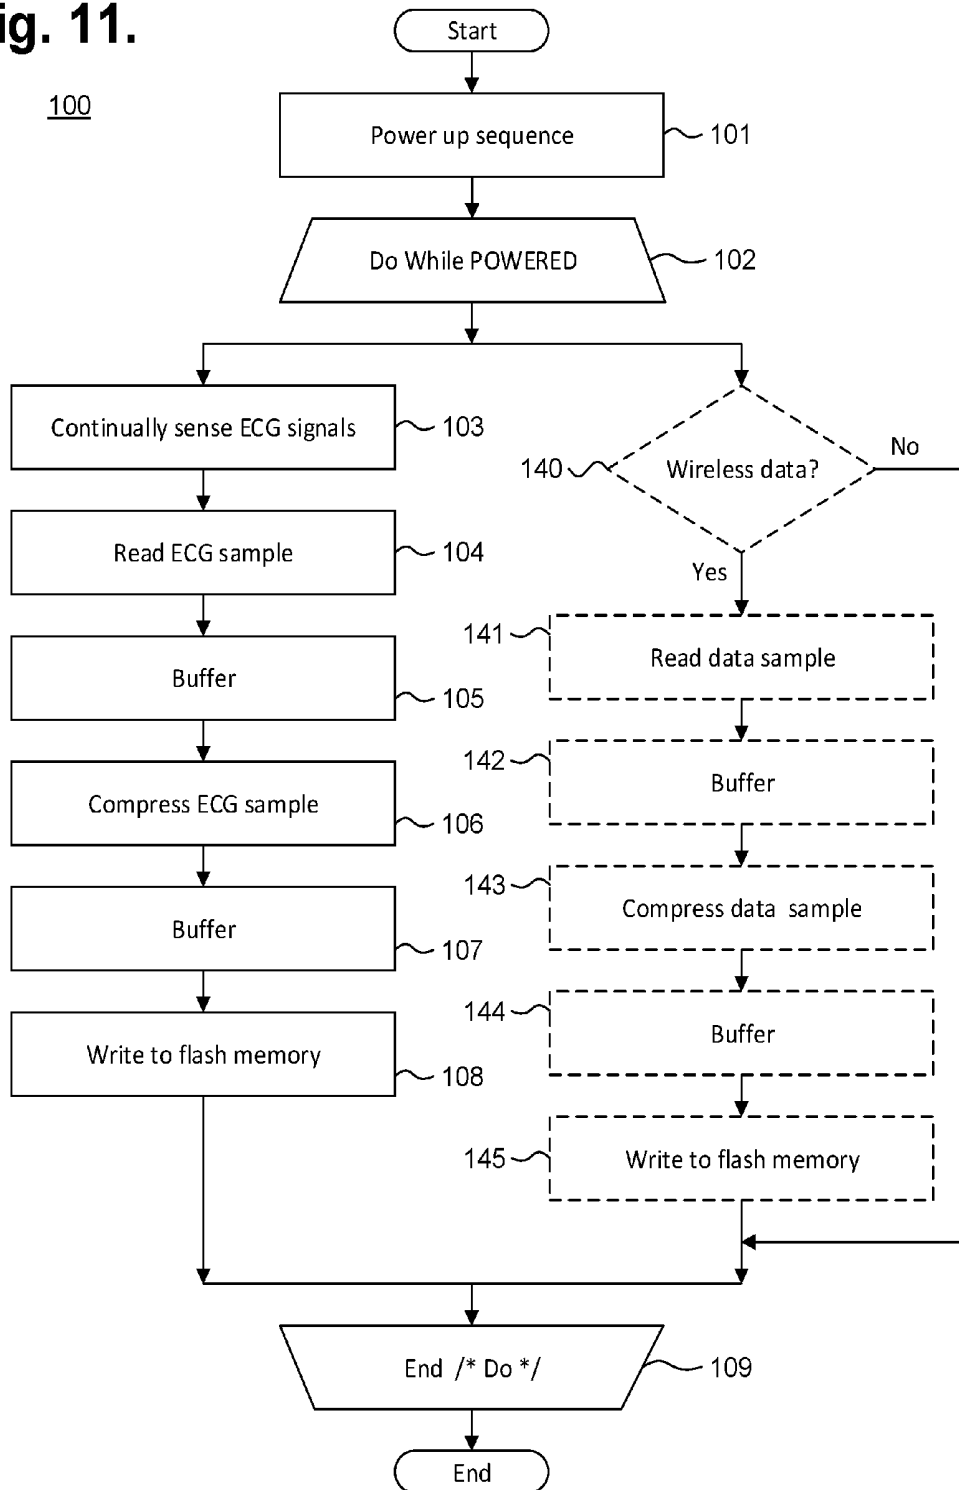


Fig. 12.


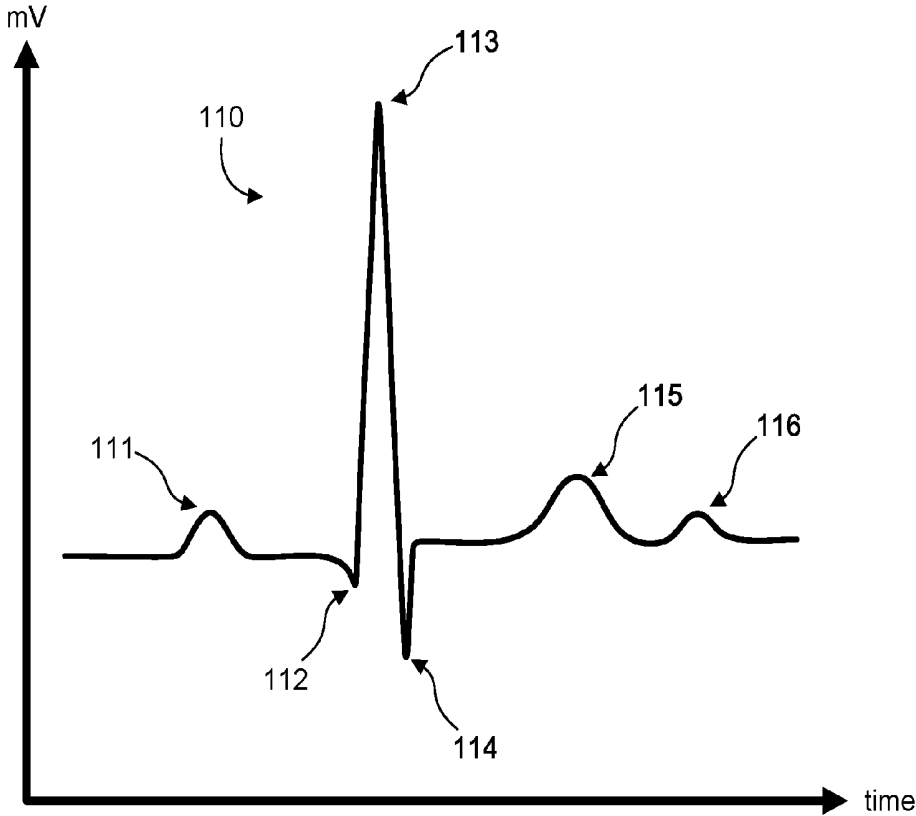


Fig. 13.

150

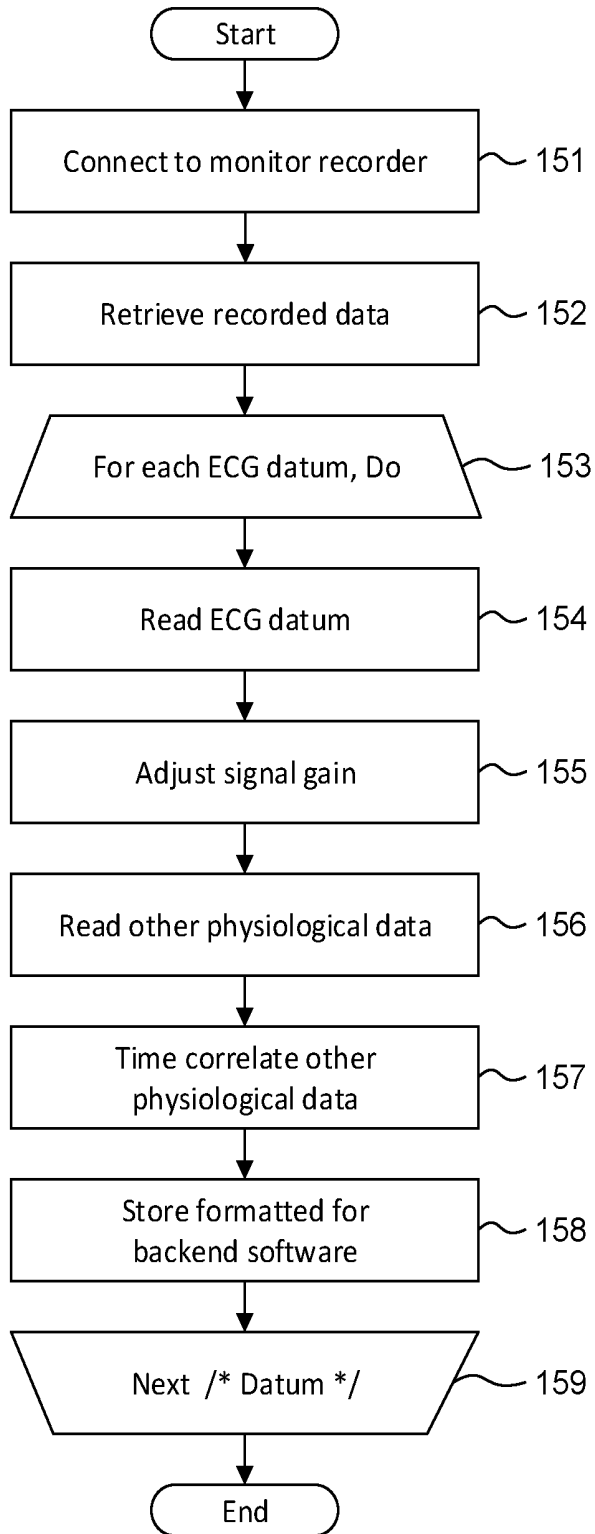

REMOTE INTERFACING OF EXTENDED WEAR ELECTROCARDIOGRAPHY AND PHYSIOLOGICAL SENSOR MONITOR

CROSS-REFERENCE TO RELATED APPLICATION

This non-provisional patent application is a continuation of U.S. patent application Ser. No. 14/082,071, filed Nov. 15, 2013, which is a continuation-in-part of U.S. patent application Ser. No. 14/080,717, filed Nov. 14, 2013, pending, and a continuation-in-part of U.S. patent application Ser. No. 14/080,725, filed Nov. 14, 2013, pending, and further claims priority under 35 U.S.C. §119(e) to U.S. Provisional Patent application, Ser. No. 61/882,403, filed Sep. 25, 2013, the disclosures of which are incorporated by reference.

FIELD

This application relates in general to electrocardiographic monitoring and, in particular, to remote interfacing of an extended wear electrocardiography and physiological sensor monitor.

BACKGROUND

The heart emits electrical signals as a by-product of the propagation of the action potentials that trigger depolarization of heart fibers. An electrocardiogram (ECG) measures and records such electrical potentials to visually depict the electrical activity of the heart over time. Conventionally, a standardized set format 12-lead configuration is used by an ECG machine to record cardiac electrical signals from well-established traditional chest locations. Electrodes at the end of each lead are placed on the skin over the anterior thoracic region of the patient's body to the lower right and to the lower left of the sternum, on the left anterior chest, and on the limbs. Sensed cardiac electrical activity is represented by PQRSTU waveforms that can be interpreted post-ECG recordation to derive heart rate and physiology. The P-wave represents atrial electrical activity. The QRSTU components represent ventricular electrical activity.

An ECG is a tool used by physicians to diagnose heart problems and other potential health concerns. An ECG is a snapshot of heart function, typically recorded over 12 seconds, that can help diagnose rate and regularity of heartbeats, effect of drugs or cardiac devices, including pacemakers and implantable cardioverter-defibrillators (ICDs), and whether a patient has heart disease. ECGs are used in-clinic during appointments, and, as a result, are limited to recording only those heart-related aspects present at the time of recording. Sporadic conditions that may not show up during a spot ECG recording require other means to diagnose them. These disorders include fainting or syncope; rhythm disorders, such as tachyarrhythmias and bradyarrhythmias; apneic episodes; and other cardiac and related disorders. Thus, an ECG only provides a partial picture and can be insufficient for complete patient diagnosis of many cardiac disorders.

Diagnostic efficacy can be improved, when appropriate, through the use of long-term extended ECG monitoring. Recording sufficient ECG and related physiology over an extended period is challenging, and often essential to enabling a physician to identify events of potential concern. A 30-day observation period is considered the "gold standard" of ECG monitoring, yet achieving a 30-day observa-

tion day period has proven unworkable because such ECG monitoring systems are arduous to employ, cumbersome to the patient, and excessively costly. Ambulatory monitoring in-clinic is implausible and impracticable. Nevertheless, if a patient's ECG could be recorded in an ambulatory setting, thereby allowing the patient to engage in activities of daily living, the chances of acquiring meaningful information and capturing an abnormal event while the patient is engaged in normal activities becomes more likely to be achieved.

For instance, the long-term wear of ECG electrodes is complicated by skin irritation and the inability ECG electrodes to maintain continual skin contact after a day or two. Moreover, time, dirt, moisture, and other environmental contaminants, as well as perspiration, skin oil, and dead skin cells from the patient's body, can get between an ECG electrode, the non-conductive adhesive used to adhere the ECG electrode, and the skin's surface. All of these factors adversely affect electrode adhesion and the quality of cardiac signal recordings. Furthermore, the physical movements of the patient and their clothing impart various compressional, tensile, and torsional forces on the contact point of an ECG electrode, especially over long recording times, and an inflexibly fastened ECG electrode will be prone to becoming dislodged. Moreover, dislodgment may occur unbeknownst to the patient, making the ECG recordings worthless. Further, some patients may have skin that is susceptible to itching or irritation, and the wearing of ECG electrodes can aggravate such skin conditions. Thus, a patient may want or need to periodically remove or replace ECG electrodes during a long-term ECG monitoring period, whether to replace a dislodged electrode, reestablish better adhesion, alleviate itching or irritation, allow for cleansing of the skin, allow for showering and exercise, or for other purpose. Such replacement or slight alteration in electrode location actually facilitates the goal of recording the ECG signal for long periods of time.

Conventionally, Holter monitors are widely used for long-term extended ECG monitoring. Typically, they are used for only 24-48 hours. A typical Holter monitor is a wearable and portable version of an ECG that include cables for each electrode placed on the skin and a separate battery-powered ECG recorder. The cable and electrode combination (or leads) are placed in the anterior thoracic region in a manner similar to what is done with an in-clinic standard ECG machine. The duration of a Holter monitoring recording depends on the sensing and storage capabilities of the monitor, as well as battery life. A "looping" Holter monitor (or event) can operate for a longer period of time by overwriting older ECG tracings, thence "recycling" storage in favor of extended operation, yet at the risk of losing event data. Although capable of extended ECG monitoring, Holter monitors are cumbersome, expensive and typically only available by medical prescription, which limits their usability. Further, the skill required to properly place the electrodes on the patient's chest hinders or precludes a patient from replacing or removing the precordial leads and usually involves moving the patient from the physician office to a specialized center within the hospital or clinic.

The ZIO XT Patch and ZIO Event Card devices, manufactured by iRhythm Tech., Inc., San Francisco, Calif., are wearable stick-on monitoring devices that are typically worn on the upper left pectoral region to respectively provide continuous and looping ECG recording. The location is used to simulate surgically implanted monitors. Both of these devices are prescription-only and for single patient use. The ZIO XT Patch device is limited to a 14-day monitoring period, while the electrodes only of the ZIO Event Card

device can be worn for up to 30 days. The ZIO XT Patch device combines both electronic recordation components, including battery, and physical electrodes into a unitary assembly that adheres to the patient's skin. The ZIO XT Patch device uses adhesive sufficiently strong to support the weight of both the monitor and the electrodes over an extended period of time and to resist disadherence from the patient's body, albeit at the cost of disallowing removal or relocation during the monitoring period. Moreover, throughout monitoring, the battery is continually depleted and battery capacity can potentially limit overall monitoring duration. The ZIO Event Card device is a form of downsized Holter monitor with a recorder component that must be removed temporarily during baths or other activities that could damage the non-waterproof electronics. Both devices represent compromises between length of wear and quality of ECG monitoring, especially with respect to ease of long term use, female-friendly fit, and quality of atrial (P-wave) signals.

In addition, with the advent of wireless communications and wearable computing, other types of personal ambulatory monitors, of varying degrees of sophistication, have become increasingly available. For example, adherents to the so-called "Quantified Self" movement combine wearable sensors and wearable computing to self-track activities of their daily lives, including inputs, states, and performance. The Nike+ FuelBand, manufactured by Nike Inc., Beaverton, Oreg., for instance, provides an activity tracker that is worn on the wrist and allows the wearer to temporally track the number of foot steps taken each day and an estimation of the calories burned. The activity tracker can interface with a smart phone device to allow a wearer to monitor their progress towards a fitness goal. Such quantified physiology, however, is typically tracked for only the personal use of the wearer and is not time-correlated to physician-supervised monitoring.

Therefore, a need remains for an extended wear continuously recording ECG monitor practicably capable of being worn for a long period of time in both men and women and capable of recording atrial signals reliably.

A further need remains for facilities to integrate wider-ranging physiological and "life tracking"-type data into long-term ECG and physiological data monitoring.

SUMMARY

Physiological monitoring can be provided through a wearable monitor that includes two components, a flexible extended wear electrode patch and a removable reusable monitor recorder. The wearable monitor sits centrally (in the midline) on the patient's chest along the sternum oriented top-to-bottom. The placement of the wearable monitor in a location at the sternal midline (or immediately to either side of the sternum), with its unique narrow "hourglass"-like shape, benefits long-term extended wear by removing the requirement that ECG electrodes be continually placed in the same spots on the skin throughout the monitoring period. Instead, the patient is free to place an electrode patch anywhere within the general region of the sternum, the area most likely to record high quality atrial signals or P-waves. The wearable monitor can also interoperate wirelessly with other wearable physiology and activity sensors and with wearable or mobile communications devices, including so-called "smart phones," to download monitoring data either in real-time or in batches. The monitor recorder can also be equipped with a wireless transceiver to either provide data or other information to, or receive data or other information

from, an interfacing wearable physiology and activity sensor, or wearable or mobile communications devices for relay to a further device, such as a server, analysis, or other purpose.

One embodiment provides a remotely-interfaceable extended wear electrocardiography and physiological sensor monitor recorder. A sealed housing forms on a bottom surface a cavity shaped to accommodate an upward projection of a battery compartment formed on a non-conductive receptacle of a disposable extended wear electrode patch and includes a set of electrical contacts that protrude from the bottom surface and are arranged in alignment with electrical pads provided on the non-conductive receptacle. Electronic circuitry is provided within the sealed housing and includes an externally-powered micro-controller operable to execute under micro programmable control. An electrocardiographic front end circuit is electrically interfaced to the micro-controller. A wireless transceiver electrically interfaces with the micro-controller and externally-powered flash memory is electrically interfaced with the micro-controller and operable to store samples of the electrocardiographic signals.

A further embodiment provides a remotely-interfaceable extended wear electrocardiography and physiological sensor monitor. A disposable extended wear electrode patch includes a flexible backing formed of an elongated strip of stretchable material with a narrow longitudinal midsection and, on each end, a contact surface is at least partially coated with an adhesive dressing provided as a crimp relief. A pair of electrocardiographic electrodes are conductively exposed on the contact surface of each end of the elongated strip, respectively. A non-conductive receptacle is adhered to an outward-facing surface of the elongated strip and includes a plurality of electrical pads. A flexible circuit is affixed on each end of the elongated strip as a strain relief and includes a pair of circuit traces electrically coupled to the pair of the electrocardiographic electrodes and a pair of the electrical pads. At least one of the circuit traces is adapted to extend along the narrow longitudinal midsection to serve as the strain relief. A reusable electrocardiography monitor includes a sealed housing that has formed on a bottom surface a cavity shaped to accommodate an upward projection of a battery compartment formed on a non-conductive receptacle of a disposable extended wear electrode patch and includes a set of electrical contacts that protrude from the bottom surface and are arranged in alignment with the electrical pads provided on the non-conductive receptacle. The reusable electrocardiography monitor includes electronic circuitry including a micro-controller operable to execute under micro programmable control and electrically interfaced to an electrocardiographic front end circuit that is operable to sense electrocardiographic signals through the electrocardiographic electrodes via the pair of the electrical pads. A wireless transceiver is electrically interfaced with the micro-controller and operable to wirelessly interface with an external wireless-enabled device to communicate samples of the electrocardiographic signals. A flash memory is electrically interfaced with the micro-controller and operable to store the samples of the electrocardiographic signals.

The monitoring patch is especially suited to the female anatomy. The narrow longitudinal midsection can fit nicely within the intermammary cleft of the breasts without inducing discomfort, whereas conventional patch electrodes are wide and, if adhered between the breasts, would cause chafing, irritation, frustration, and annoyance, leading to low patient compliance.

The foregoing aspects enhance ECG monitoring performance and quality, facilitating long-term ECG recording, critical to accurate arrhythmia diagnosis.

In addition, the foregoing aspects enhance comfort in women (and certain men), but not irritation of the breasts, by placing the monitoring patch in the best location possible for optimizing the recording of cardiac signals from the atrium, another feature critical to proper arrhythmia diagnosis.

Finally, the foregoing aspects as relevant to monitoring are equally applicable to recording other physiological measures, such as temperature, respiratory rate, blood sugar, oxygen saturation, and blood pressure, as well as other measures of body chemistry and physiology.

Still other embodiments will become readily apparent to those skilled in the art from the following detailed description, wherein are described embodiments by way of illustrating the best mode contemplated. As will be realized, other and different embodiments are possible and the embodiments' several details are capable of modifications in various obvious respects, all without departing from their spirit and the scope. Accordingly, the drawings and detailed description are to be regarded as illustrative in nature and not as restrictive.

BRIEF DESCRIPTION OF THE DRAWINGS

FIGS. 1 and 2 are diagrams showing, by way of examples, an extended wear electrocardiography and physiological sensor monitor respectively fitted to the sternal region of a female patient and a male patient.

FIG. 3 is a functional block diagram showing a system for remote interfacing of an extended wear electrocardiography and physiological sensor monitor in accordance with one embodiment.

FIG. 4 is a perspective view showing an extended wear electrode patch with a monitor recorder inserted.

FIG. 5 is a perspective view showing the monitor recorder of FIG. 4.

FIG. 6 is a perspective view showing the extended wear electrode patch of FIG. 4 without a monitor recorder inserted.

FIG. 7 is a bottom plan view of the monitor recorder of FIG. 4.

FIG. 8 is a top view showing the flexible circuit of the extended wear electrode patch of FIG. 4 when mounted above the flexible backing.

FIG. 9 is a functional block diagram showing the component architecture of the circuitry of the monitor recorder of FIG. 4.

FIG. 10 is a functional block diagram showing the circuitry of the extended wear electrode patch of FIG. 4.

FIG. 11 is a flow diagram showing a monitor recorder-implemented method for monitoring ECG data for use in the monitor recorder of FIG. 4.

FIG. 12 is a graph showing, by way of example, a typical ECG waveform.

FIG. 13 is a flow diagram showing a method for offloading and converting ECG and other physiological data from an extended wear electrocardiography and physiological sensor monitor in accordance with one embodiment.

DETAILED DESCRIPTION

Physiological monitoring can be provided through a wearable monitor that includes two components, a flexible extended wear electrode patch and a removable reusable monitor recorder. FIGS. 1 and 2 are diagrams showing, by

way of examples, an extended wear electrocardiography and physiological sensor monitor **12**, including a monitor recorder **14** in accordance with one embodiment, respectively fitted to the sternal region of a female patient **10** and a male patient **11**. The wearable monitor **12** sits centrally (in the midline) on the patient's chest along the sternum **13** oriented top-to-bottom with the monitor recorder **14** preferably situated towards the patient's head. In a further embodiment, the orientation of the wearable monitor **12** can be corrected post-monitoring, as further described infra. The electrode patch **15** is shaped to fit comfortably and conformal to the contours of the patient's chest approximately centered on the sternal midline **16** (or immediately to either side of the sternum **13**). The distal end of the electrode patch **15** extends towards the Xiphoid process and, depending upon the patient's build, may straddle the region over the Xiphoid process. The proximal end of the electrode patch **15**, located under the monitor recorder **14**, is below the manubrium and, depending upon patient's build, may straddle the region over the manubrium.

The placement of the wearable monitor **12** in a location at the sternal midline **16** (or immediately to either side of the sternum **13**) significantly improves the ability of the wearable monitor **12** to cutaneously sense cardiac electric signals, particularly the P-wave (or atrial activity) and, to a lesser extent, the QRS interval signals in the ECG waveforms that indicate ventricular activity, while simultaneously facilitating comfortable long-term wear for many weeks. The sternum **13** overlies the right atrium of the heart and the placement of the wearable monitor **12** in the region of the sternal midline **13** puts the ECG electrodes of the electrode patch **15** in a location better adapted to sensing and recording P-wave signals than other placement locations, say, the upper left pectoral region or lateral thoracic region or the limb leads. In addition, placing the lower or inferior pole (ECG electrode) of the electrode patch **15** over (or near) the Xiphoid process facilitates sensing of ventricular activity and provides superior recordation of the QRS interval.

When operated standalone, the monitor recorder **14** of the extended wear electrocardiography and physiological sensor monitor **12** senses and records the patient's ECG data into an onboard memory. In addition, the wearable monitor **12** can interoperate with other devices. FIG. 3 is a functional block diagram showing a system **120** for remote interfacing of an extended wear electrocardiography and physiological sensor monitor **12** in accordance with one embodiment. The monitor recorder **14** is a reusable component that can be fitted during patient monitoring into a non-conductive receptacle provided on the electrode patch **15**, as further described infra with reference to FIG. 4, and later removed for offloading of stored ECG data or to receive revised programming. The monitor recorder **14** can then be connected to a download station **125**, which could be a programmer or other device that permits the retrieval of stored ECG monitoring data, execution of diagnostics or programming of the monitor recorder **14**, or performance of other functions. The monitor recorder **14** has a set of electrical contacts (not shown) that enable the monitor recorder **14** to physically interface to a set of terminals **128** on a paired receptacle **127** of the download station **125**. In turn, the download station **125** executes a communications or offload program **126** ("Offload") or similar program that interacts with the monitor recorder **14** via the physical interface to retrieve the stored ECG monitoring data. The download station **125** could be a server, personal computer, tablet or handheld computer, smart mobile device, or purpose-built programmer designed

specific to the task of interfacing with a monitor recorder **14**. Still other forms of download station **125** are possible.

Upon retrieving stored ECG monitoring data from a monitor recorder **14**, middleware first operates on the retrieved data to adjust the ECG capture quality, as necessary, and to convert the retrieved data into a format suitable for use by third party post-monitoring analysis software, as further described infra with reference to FIG. **13**. The formatted data can then be retrieved from the download station **125** over a hard link **135** using a control program **137** (“Ctl”) or analogous application executing on a personal computer **136** or other connectable computing device, via a communications link (not shown), whether wired or wireless, or by physical transfer of storage media (not shown). The personal computer **136** or other connectable device may also execute middleware that converts ECG data and other information into a format suitable for use by a third-party post-monitoring analysis program, as further described infra with reference to FIG. **13**. Note that formatted data stored on the personal computer **136** would have to be maintained and safeguarded in the same manner as electronic medical records (EMRs) **134** in the secure database **124**, as further discussed infra. In a further embodiment, the download station **125** is able to directly interface with other devices over a computer communications network **121**, which could be some combination of a local area network and a wide area network, including the Internet, over a wired or wireless connection.

A client-server model could be used to employ a server **122** to remotely interface with the download station **125** over the network **121** and retrieve the formatted data or other information. The server **122** executes a patient management program **123** (“Mgt”) or similar application that stores the retrieved formatted data and other information in a secure database **124** cataloged in that patient’s EMRs **134**. In addition, the patient management program **123** could manage a subscription service that authorizes a monitor recorder **14** to operate for a set period of time or under pre-defined operational parameters.

The patient management program **123**, or other trusted application, also maintains and safeguards the secure database **124** to limit access to patient EMRs **134** to only authorized parties for appropriate medical or other uses, such as mandated by state or federal law, such as under the Health Insurance Portability and Accountability Act (HIPAA) or per the European Union’s Data Protection Directive. For example, a physician may seek to review and evaluate his patient’s ECG monitoring data, as securely stored in the secure database **124**. The physician would execute an application program **130** (“Pgm”), such as a post-monitoring ECG analysis program, on a personal computer **129** or other connectable computing device, and, through the application **130**, coordinate access to his patient’s EMRs **134** with the patient management program **123**. Other schemes and safeguards to protect and maintain the integrity of patient EMRs **134** are possible.

The wearable monitor **12** can interoperate wirelessly with other wearable physiology and activity sensors **131** and with wearable or mobile communications devices **133**. Wearable physiology and activity sensors **131** encompass a wide range of wirelessly interconnectable devices that measure or monitor data physical to the patient’s body, such as heart rate, temperature, blood pressure, and so forth; physical states, such as movement, sleep, footsteps, and the like; and performance, including calories burned or estimated blood glucose level. These devices originate both within the medical community to sense and record traditional medical

physiology that could be useful to a physician in arriving at a patient diagnosis or clinical trajectory, as well as from outside the medical community, from, for instance, sports or lifestyle product companies who seek to educate and assist individuals with self-quantifying interests.

Frequently, wearable physiology and activity sensors **131** are capable of wireless interfacing with wearable or mobile communications devices **133**, particularly smart mobile devices, including so-called “smart phones,” to download monitoring data either in real-time or in batches. The wearable or mobile communications device **133** executes an application (“App”) that can retrieve the data collected by the wearable physiology and activity sensor **131** and evaluate the data to generate information of interest to the wearer, such as an estimation of the effectiveness of the wearer’s exercise efforts. Still other wearable or mobile communications device **133** functions on the collected data are possible.

The wearable or mobile communications devices **133** could also serve as a conduit for providing the data collected by the wearable physiology and activity sensor **131** to a server **122**, or, similarly, the wearable physiology and activity sensor **131** could itself directly provide the collected data to the server **122**. The server **122** could then merge the collected data into the wearer’s EMRs **134** in the secure database **124**, if appropriate (and permissible), or the server **122** could perform an analysis of the collected data, perhaps based by comparison to a population of like wearers of the wearable physiology and activity sensor **131**. Still other server **122** functions on the collected data are possible.

Finally, the monitor recorder **14** can also be equipped with a wireless transceiver, as further described infra with reference to FIGS. **9** and **10**. Thus, when wireless-enabled, both wearable physiology and activity sensors **131** and wearable or mobile communications devices **133** could wirelessly interface with the monitor recorder **14**, which could either provide data or other information to, or receive data or other information from an interfacing device for relay to a further device, such as the server **122**, analysis, or other purpose. In addition, the monitor recorder **14** could wirelessly interface directly with the server **122**, personal computer **129**, or other computing device connectable over the network **121**, when the monitor recorder **14** is appropriately equipped for interfacing with such devices. Still other types of remote interfacing of the monitor recorder **14** are possible.

During use, the electrode patch **15** is first adhered to the skin along the sternal midline **16** (or immediately to either side of the sternum **13**). A monitor recorder **14** is then snapped into place on the electrode patch **15** to initiate ECG monitoring. FIG. **4** is a perspective view showing an extended wear electrode patch **15** with a monitor recorder **14** in accordance with one embodiment inserted. The body of the electrode patch **15** is preferably constructed using a flexible backing **20** formed as an elongated strip **21** of wrap knit or similar stretchable material with a narrow longitudinal mid-section **23** evenly tapering inward from both sides. A pair of cut-outs **22** between the distal and proximal ends of the electrode patch **15** create a narrow longitudinal midsection **23** or “isthmus” and defines an elongated “hour-glass”-like shape, when viewed from above.

The electrode patch **15** incorporates features that significantly improve wearability, performance, and patient comfort throughout an extended monitoring period. During wear, the electrode patch **15** is susceptible to pushing, pulling, and torquing movements, including compressional and torsional forces when the patient bends forward, and tensile and torsional forces when the patient leans backwards. To counter these stress forces, the electrode patch **15**

incorporates strain and crimp reliefs, such as described in commonly-assigned U.S. patent application, entitled "Extended Wear Electrocardiography Patch," Ser. No. 14/080,717, filed Nov. 14, 2013, pending, the disclosure of which is incorporated by reference. In addition, the cut-outs **22** and longitudinal midsection **23** help minimize interference with and discomfort to breast tissue, particularly in women (and gynecomastic men). The cut-outs **22** and longitudinal midsection **23** further allow better conformity of the electrode patch **15** to sternal bowing and to the narrow isthmus of flat skin that can occur along the bottom of the intermammary cleft between the breasts, especially in buxom women. The cut-outs **22** and longitudinal midsection **23** help the electrode patch **15** fit nicely between a pair of female breasts in the intermammary cleft. Still other shapes, cut-outs and conformities to the electrode patch **15** are possible.

The monitor recorder **14** removably and reusably snaps into an electrically non-conductive receptacle **25** during use. The monitor recorder **14** contains electronic circuitry for recording and storing the patient's electrocardiography as sensed via a pair of ECG electrodes provided on the electrode patch **15**, such as described in commonly-assigned U.S. patent application, entitled "Extended Wear Ambulatory Electrocardiography and Physiological Sensor Monitor," Ser. No. 14/080,725, filed Nov. 14, 2013, pending, the disclosure which is incorporated by reference. The non-conductive receptacle **25** is provided on the top surface of the flexible backing **20** with a retention catch **26** and tension clip **27** molded into the non-conductive receptacle **25** to conformably receive and securely hold the monitor recorder **14** in place.

The monitor recorder **14** includes a sealed housing that snaps into place in the non-conductive receptacle **25**. FIG. **5** is a perspective view showing the monitor recorder **14** of FIG. **4**. The sealed housing **50** of the monitor recorder **14** intentionally has a rounded isosceles trapezoidal-like shape **52**, when viewed from above, such as described in commonly-assigned U.S. Design patent application, entitled "Electrocardiography Monitor," Ser. No. 29/472,046, filed Nov. 7, 2013, pending, the disclosure of which is incorporated by reference. The edges **51** along the top and bottom surfaces are rounded for patient comfort. The sealed housing **50** is approximately 47 mm long, 23 mm wide at the widest point, and 7 mm high, excluding a patient-operable tactile-feedback button **55**. The sealed housing **50** can be molded out of polycarbonate, ABS, or an alloy of those two materials. The button **55** is waterproof and the button's top outer surface is molded silicon rubber or similar soft pliable material. A retention detent **53** and tension detent **54** are molded along the edges of the top surface of the housing **50** to respectively engage the retention catch **26** and the tension clip **27** molded into non-conductive receptacle **25**. Other shapes, features, and conformities of the sealed housing **50** are possible.

The electrode patch **15** is intended to be disposable. The monitor recorder **14**, however, is reusable and can be transferred to successive electrode patches **15** to ensure continuity of monitoring. The placement of the wearable monitor **12** in a location at the sternal midline **16** (or immediately to either side of the sternum **13**) benefits long-term extended wear by removing the requirement that ECG electrodes be continually placed in the same spots on the skin throughout the monitoring period. Instead, the patient is free to place an electrode patch **15** anywhere within the general region of the sternum **13**.

As a result, at any point during ECG monitoring, the patient's skin is able to recover from the wearing of an electrode patch **15**, which increases patient comfort and satisfaction, while the monitor recorder **14** ensures ECG monitoring continuity with minimal effort. A monitor recorder **14** is merely unsnapped from a worn out electrode patch **15**, the worn out electrode patch **15** is removed from the skin, a new electrode patch **15** is adhered to the skin, possibly in a new spot immediately adjacent to the earlier location, and the same monitor recorder **14** is snapped into the new electrode patch **15** to reinitiate and continue the ECG monitoring.

During use, the electrode patch **15** is first adhered to the skin in the sternal region. FIG. **6** is a perspective view showing the extended wear electrode patch **15** of FIG. **4** without a monitor recorder **14** inserted. A flexible circuit **32** is adhered to each end of the flexible backing **20**. A distal circuit trace **33** and a proximal circuit trace (not shown) electrically couple ECG electrodes (not shown) to a pair of electrical pads **34**. The electrical pads **34** are provided within a moisture-resistant seal **35** formed on the bottom surface of the non-conductive receptacle **25**. When the monitor recorder **14** is securely received into the non-conductive receptacle **25**, that is, snapped into place, the electrical pads **34** interface to electrical contacts (not shown) protruding from the bottom surface of the monitor recorder **14**, and the moisture-resistant seal **35** enables the monitor recorder **14** to be worn at all times, even during bathing or other activities that could expose the monitor recorder **14** to moisture.

In addition, a battery compartment **36** is formed on the bottom surface of the non-conductive receptacle **25**, and a pair of battery leads (not shown) electrically interface the battery to another pair of the electrical pads **34**. The battery contained within the battery compartment **35** can be replaceable, rechargeable or disposable.

The monitor recorder **14** draws power externally from the battery provided in the non-conductive receptacle **25**, thereby uniquely obviating the need for the monitor recorder **14** to carry a dedicated power source. FIG. **7** is a bottom plan view of the monitor recorder **14** of FIG. **4**. A cavity **58** is formed on the bottom surface of the sealed housing **50** to accommodate the upward projection of the battery compartment **36** from the bottom surface of the non-conductive receptacle **25**, when the monitor recorder **14** is secured in place on the non-conductive receptacle **25**. A set of electrical contacts **56** protrude from the bottom surface of the sealed housing **50** and are arranged in alignment with the electrical pads **34** provided on the bottom surface of the non-conductive receptacle **25** to establish electrical connections between the electrode patch **15** and the monitor recorder **14**. In addition, a seal coupling **57** circumferentially surrounds the set of electrical contacts **56** and securely mates with the moisture-resistant seal **35** formed on the bottom surface of the non-conductive receptacle **25**.

The placement of the flexible backing **20** on the sternal midline **16** (or immediately to either side of the sternum **13**) also helps to minimize the side-to-side movement of the wearable monitor **12** in the left- and right-handed directions during wear. To counter the dislodgment of the flexible backing **20** due to compressional and torsional forces, a layer of non-irritating adhesive, such as hydrocolloid, is provided at least partially on the underside, or contact surface of the flexible backing **20**, but only on the distal end **30** and the proximal end **31**. As a result, the underside, or contact surface of the longitudinal midsection **23** does not have an adhesive layer and remains free to move relative to the skin. Thus, the longitudinal midsection **23** forms a crimp

relief that respectively facilitates compression and twisting of the flexible backing 20 in response to compressional and torsional forces. Other forms of flexible backing crimp reliefs are possible.

Unlike the flexible backing 20, the flexible circuit 32 is only able to bend and cannot stretch in a planar direction. The flexible circuit 32 can be provided either above or below the flexible backing 20. FIG. 8 is a top view showing the flexible circuit 32 of the extended wear electrode patch 15 of FIG. 4 when mounted above the flexible backing 20. A distal ECG electrode 38 and proximal ECG electrode 39 are respectively coupled to the distal and proximal ends of the flexible circuit 32. A strain relief 40 is defined in the flexible circuit 32 at a location that is partially underneath the battery compartment 36 when the flexible circuit 32 is affixed to the flexible backing 20. The strain relief 40 is laterally extendable to counter dislodgment of the ECG electrodes 38, 39 due to tensile and torsional forces. A pair of strain relief cutouts 41 partially extend transversely from each opposite side of the flexible circuit 32 and continue longitudinally towards each other to define in 'S'-shaped pattern, when viewed from above. The strain relief respectively facilitates longitudinal extension and twisting of the flexible circuit 32 in response to tensile and torsional forces. Other forms of circuit board strain relief are possible.

ECG monitoring and other functions performed by the monitor recorder 14 are provided through a micro controlled architecture. FIG. 9 is a functional block diagram showing the component architecture of the circuitry 60 of the monitor recorder 14 of FIG. 4. The circuitry 60 is externally powered through a battery provided in the non-conductive receptacle 25 (shown in FIG. 6). Both power and raw ECG signals, which originate in the pair of ECG electrodes 38, 39 (shown in FIG. 8) on the distal and proximal ends of the electrode patch 15, are received through an external connector 65 that mates with a corresponding physical connector on the electrode patch 15. The external connector 65 includes the set of electrical contacts 56 that protrude from the bottom surface of the sealed housing 50 and which physically and electrically interface with the set of pads 34 provided on the bottom surface of the non-conductive receptacle 25. The external connector includes electrical contacts 56 for data download, microcontroller communications, power, analog inputs, and a peripheral expansion port. The arrangement of the pins on the electrical connector 65 of the monitor recorder 14 and the device into which the monitor recorder 14 is attached, whether an electrode patch 15 or download station (not shown), follow the same electrical pin assignment convention to facilitate interoperability. The external connector 65 also serves as a physical interface to a download station that permits the retrieval of stored ECG monitoring data, communication with the monitor recorder 14, and performance of other functions.

Operation of the circuitry 60 of the monitor recorder 14 is managed by a microcontroller 61. The micro-controller 61 includes a program memory unit containing internal flash memory that is readable and writeable. The internal flash memory can also be programmed externally. The microcontroller 61 draws power externally from the battery provided on the electrode patch 15 via a pair of the electrical contacts 56. The microcontroller 61 connects to the ECG front end circuit 63 that measures raw cutaneous electrical signals and generates an analog ECG signal representative of the electrical activity of the patient's heart over time.

The circuitry 60 of the monitor recorder 14 also includes a flash memory 62, which the micro-controller 61 uses for storing ECG monitoring data and other physiology and

information. The flash memory 62 also draws power externally from the battery provided on the electrode patch 15 via a pair of the electrical contacts 56. Data is stored in a serial flash memory circuit, which supports read, erase and program operations over a communications bus. The flash memory 62 enables the microcontroller 61 to store digitized ECG data. The communications bus further enables the flash memory 62 to be directly accessed externally over the external connector 65 when the monitor recorder 14 is interfaced to a download station.

The circuitry 60 of the monitor recorder 14 further includes an actigraphy sensor 64 implemented as a 3-axis accelerometer. The accelerometer may be configured to generate interrupt signals to the microcontroller 61 by independent initial wake up and free fall events, as well as by device position. In addition, the actigraphy provided by the accelerometer can be used during post-monitoring analysis to correct the orientation of the monitor recorder 14 if, for instance, the monitor recorder 14 has been inadvertently installed upside down, that is, with the monitor recorder 14 oriented on the electrode patch 15 towards the patient's feet, as well as for other event occurrence analyses, such as described in commonly-assigned U.S. Patent Application Publication No. 2015/0087923, issued Mar. 26, 2016, the disclosure of which is incorporated by reference.

The circuitry 60 of the monitor recorder 14 includes a wireless transceiver 69 that can provides wireless interfacing capabilities. The wireless transceiver 69 also draws power externally from the battery provided on the electrode patch 15 via a pair of the electrical contacts 56. The wireless transceiver 69 can be implemented using one or more forms of wireless communications, including the IEEE 802.11 computer communications standard, that is Wi-Fi; the 4G mobile phone mobile communications standard; the Bluetooth data exchange standard; or other wireless communications or data exchange standards and protocols. The type of wireless interfacing capability could limit the range of interoperability of the monitor recorder 14; for instance, Bluetooth-based implementations are designed for low power consumption with a short communications range.

The microcontroller 61 includes an expansion port that also utilizes the communications bus. External devices, separately drawing power externally from the battery provided on the electrode patch 15 or other source, can interface to the microcontroller 61 over the expansion port in half duplex mode. For instance, an external physiology sensor can be provided as part of the circuitry 60 of the monitor recorder 14, or can be provided on the electrode patch 15 with communication with the micro-controller 61 provided over one of the electrical contacts 56. The physiology sensor can include an SpO₂ sensor, blood pressure sensor, temperature sensor, respiratory rate sensor, glucose sensor, airflow sensor, volumetric pressure sensing, or other types of sensor or telemetric input sources. For instance, the integration of an airflow sensor is described in commonly-assigned U.S. Pat. No. 9,364,155, issued Jun. 14, 2016, the disclosure of which is incorporated by reference.

Finally, the circuitry 60 of the monitor recorder 14 includes patient-interfaceable components, including a tactile feedback button 66, which a patient can press to mark events or to perform other functions, and a buzzer 67, such as a speaker, magnetic resonator or piezoelectric buzzer. The buzzer 67 can be used by the microcontroller 61 to output feedback to a patient such as to confirm power up and initiation of ECG monitoring. Still other components as part of the circuitry 60 of the monitor recorder 14 are possible.

While the monitor recorder **14** operates under micro control, most of the electrical components of the electrode patch **15** operate passively. FIG. **10** is a functional block diagram showing the circuitry **70** of the extended wear electrode patch **15** of FIG. **4**. The circuitry **70** of the electrode patch **15** is electrically coupled with the circuitry **60** of the monitor recorder **14** through an external connector **74**. The external connector **74** is terminated through the set of pads **34** provided on the bottom of the non-conductive receptacle **25**, which electrically mate to corresponding electrical contacts **56** protruding from the bottom surface of the sealed housing **50** to electrically interface the monitor recorder **14** to the electrode patch **15**.

The circuitry **70** of the electrode patch **15** performs three primary functions. First, a battery **71** is provided in a battery compartment formed on the bottom surface of the non-conductive receptacle **25**. The battery **71** is electrically interfaced to the circuitry **60** of the monitor recorder **14** as a source of external power. The unique provisioning of the battery **71** on the electrode patch **15** provides several advantages. First, the locating of the battery **71** physically on the electrode patch **15** lowers the center of gravity of the overall wearable monitor **12** and thereby helps to minimize shear forces and the effects of movements of the patient and clothing. Moreover, the housing **50** of the monitor recorder **14** is sealed against moisture and providing power externally avoids having to either periodically open the housing **50** for the battery replacement, which also creates the potential for moisture intrusion and human error, or to recharge the battery, which can potentially take the monitor recorder **14** off line for hours at a time. In addition, the electrode patch **15** is intended to be disposable, while the monitor recorder **14** is a reusable component. Each time that the electrode patch **15** is replaced, a fresh battery is provided for the use of the monitor recorder **14**, which enhances ECG monitoring performance quality and duration of use. Finally, the architecture of the monitor recorder **14** is open, in that other physiology sensors or components can be added by virtue of the expansion port of the microcontroller **61**. Requiring those additional sensors or components to draw power from a source external to the monitor recorder **14** keeps power considerations independent of the monitor recorder **14**. Thus, a battery of higher capacity could be introduced when needed to support the additional sensors or components without effecting the monitor recorders circuitry **60**.

Second, the pair of ECG electrodes **38, 39** respectively provided on the distal and proximal ends of the flexible circuit **32** are electrically coupled to the set of pads **34** provided on the bottom of the non-conductive receptacle **25** by way of their respective circuit traces **33, 37**. The signal ECG electrode **39** includes a protection circuit **72**, which is an inline resistor that protects the patient from excessive leakage current.

Last, in a further embodiment, the circuitry **70** of the electrode patch **15** includes a cryptographic circuit **73** to authenticate an electrode patch **15** for use with a monitor recorder **14**. The cryptographic circuit **73** includes a device capable of secure authentication and validation. The cryptographic device **73** ensures that only genuine, non-expired, safe, and authenticated electrode patches **15** are permitted to provide monitoring data to a monitor recorder **14**, such as described in commonly-assigned U.S. Patent Application Publication No. 2015/0087950, issued Mar. 26, 2015, the disclosure which is incorporated by reference.

In a further embodiment, the circuitry **70** of the electrode patch **15** includes a wireless transceiver **75**, in lieu of including of the wireless transceiver **69** in the circuitry **60** of

the monitor recorder **14**, which interfaces with the microcontroller **61** over the microcontroller's expansion port via the external connector **74**.

The monitor recorder **14** continuously monitors the patient's heart rate and physiology. FIG. **11** is a flow diagram showing a monitor recorder-implemented method **100** for monitoring ECG data for use in the monitor recorder **14** of FIG. **4**. Initially, upon being connected to the set of pads **34** provided with the non-conductive receptacle **25** when the monitor recorder **14** is snapped into place, the microcontroller **61** executes a power up sequence (step **101**). During the power up sequence, the voltage of the battery **71** is checked, the state of the flash memory **62** is confirmed, both in terms of operability check and available capacity, and microcontroller operation is diagnostically confirmed. In a further embodiment, an authentication procedure between the microcontroller **61** and the electrode patch **15** are also performed.

Following satisfactory completion of the power up sequence, an iterative processing loop (steps **102-109**) is continually executed by the microcontroller **61**. During each iteration (step **102**) of the processing loop, the ECG frontend **63** (shown in FIG. **9**) continually senses the cutaneous ECG electrical signals (step **103**) via the ECG electrodes **38, 29** and is optimized to maintain the integrity of the P-wave. A sample of the ECG signal is read (step **104**) by the microcontroller **61** by sampling the analog ECG signal output front end **63**. FIG. **12** is a graph showing, by way of example, a typical ECG waveform **110**. The x-axis represents time in approximate units of tenths of a second. The y-axis represents cutaneous electrical signal strength in approximate units of millivolts. The P-wave **111** has a smooth, normally upward, that is, positive, waveform that indicates atrial depolarization. The QRS complex usually begins with the downward deflection of a Q wave **112**, followed by a larger upward deflection of an R-wave **113**, and terminated with a downward waveform of the S wave **114**, collectively representative of ventricular depolarization. The T wave **115** is normally a modest upward waveform, representative of ventricular depolarization, while the U wave **116**, often not directly observable, indicates the recovery period of the Purkinje conduction fibers.

Sampling of the R-to-R interval enables heart rate information derivation. For instance, the R-to-R interval represents the ventricular rate and rhythm, while the P-to-P interval represents the atrial rate and rhythm. Importantly, the PR interval is indicative of atrioventricular (AV) conduction time and abnormalities in the PR interval can reveal underlying heart disorders, thus representing another reason why the P-wave quality achievable by the extended wear ambulatory electrocardiography and physiological sensor monitor described herein is medically unique and important. The long-term observation of these ECG indicia, as provided through extended wear of the wearable monitor **12**, provides valuable insights to the patient's cardiac function and overall well-being.

Each sampled ECG signal, in quantized and digitized form, is temporarily staged in buffer (step **105**), pending compression preparatory to storage in the flash memory **62** (step **106**). Following compression, the compressed ECG digitized sample is again buffered (step **107**), then written to the flash memory **62** (step **108**) using the communications bus. Processing continues (step **109**), so long as the monitoring recorder **14** remains connected to the electrode patch **15** (and storage space remains available in the flash memory **62**), after which the processing loop is exited and execution terminates. Still other operations and steps are possible.

In a further embodiment, the monitor recorder **14** also continuously receives data from wearable physiology and activity sensors **131** and wearable or mobile communications devices **133** (shown in FIG. **3**). the data is received in a conceptually-separate execution thread as part of the iterative processing loop (steps **102-109**) continually executed by the microcontroller **61**. During each iteration (step **102**) of the processing loop, if wireless data is available (step **140**), a sample of the wireless is read (step **141**) by the microcontroller **61** and, if necessary, converted into a digital signal by the onboard ADC of the microcontroller **61**. Each wireless data sample, in quantized and digitized form, is temporarily staged in buffer (step **142**), pending compression preparatory to storage in the flash memory **62** (step **143**). Following compression, the compressed wireless data sample is again buffered (step **144**), then written to the flash memory **62** (step **145**) using the communications bus. Processing continues (step **109**), so long as the monitoring recorder **14** remains connected to the electrode patch **15** (and storage space remains available in the flash memory **62**), after which the processing loop is exited and execution terminates. Still other operations and steps are possible.

The monitor recorder **14** stores ECG data and other information in the flash memory **62** (shown in FIG. **9**) using a proprietary format that includes data compression. As a result, data retrieved from a monitor recorder **14** must first be converted into a format suitable for use by third party post-monitoring analysis software. FIG. **13** is a flow diagram showing a method **150** for offloading and converting ECG and other physiological data from an extended wear electrocardiography and physiological sensor monitor **12** in accordance with one embodiment. The method **150** can be implemented in software and execution of the software can be performed on a download station **125**, which could be a programmer or other device, or a computer system, including a server **122** or personal computer **129**, such as further described supra with reference to FIG. **3**, as a series of process or method modules or steps. For convenience, the method **150** will be described in the context of being performed by a personal computer **136** or other connectable computing device (shown in FIG. **3**) as middleware that converts ECG data and other information into a format suitable for use by a third-party post-monitoring analysis program. Execution of the method **150** by a computer system would be analogous mutatis mutandis.

Initially, the download station **125** is connected to the monitor recorder **14** (step **151**), such as by physically interfacing to a set of terminals **128** on a paired receptacle **127** or by wireless connection, if available. The data stored on the monitor recorder **14**, including ECG and physiological monitoring data, other recorded data, and other information are retrieved (step **152**) over a hard link **135** using a control program **137** ("Ctl") or analogous application executing on a personal computer **136** or other connectable computing device.

The data retrieved from the monitor recorder **14** is in a proprietary storage format and each datum of recorded ECG monitoring data, as well as any other physiological data or other information, must be converted, so that the data can be used by a third-party post-monitoring analysis program. Each datum of ECG monitoring data is converted by the middleware (steps **153-159**) in an iterative processing loop. During each iteration (step **153**), the ECG datum is read (step **154**) and, if necessary, the gain of the ECG signal is adjusted (step **155**) to compensate, for instance, for relocation or replacement of the electrode patch **15** during the monitoring period.

In addition, depending upon the configuration of the wearable monitor **12**, other physiological data (or other information), including patient events, such as a fall, peak activity level, sleep detection, Detection of patient activity levels and states, and so on, may be recorded along with the ECG monitoring data. For instance, actigraphy data may have been sampled by the actigraphy sensor **64** based on a sensed event occurrence, such as a sudden change in orientation due to the patient taking a fall. In response, the monitor recorder **14** will embed the actigraphy data samples into the stream of data, including ECG monitoring data, that is recorded to the flash memory **62** by the micro-controller **61**. Post-monitoring, the actigraphy data is temporally matched to the ECG data to provide the proper physiological context to the sensed event occurrence. As a result, the three-axis actigraphy signal is turned into an actionable event occurrence that is provided, through conversion by the middleware, to third party post-monitoring analysis programs, along with the ECG recordings contemporaneous to the event occurrence. Other types of processing of the other physiological data (or other information) are possible.

Thus, during execution of the middleware, any other physiological data (or other information) that has been embedded into the recorded ECG monitoring data is read (step **156**) and time-correlated to the time frame of the ECG signals that occurred at the time that the other physiological data (or other information) was noted (step **157**). Finally, the ECG datum, signal gain adjusted, if appropriate, and other physiological data, if applicable and as time-correlated, are stored in a format suitable to the backend software (step **158**) used in post-monitoring analysis.

In a further embodiment, the other physiological data, if apropos, is embedded within an unused ECG track. For example, the SCP-ENG standard allows multiple ECG channels to be recorded into a single ECG record. The monitor recorder **14**, though, only senses one ECG channel. The other physiological data can be stored into an additional ECG channel, which would otherwise be zero-padded or altogether omitted. The backend software would then be able to read the other physiological data in context with the single channel of ECG monitoring data recorded by the monitor recorder **14**, provided the backend software implemented changes necessary to interpret the other physiological data. Still other forms of embedding of the other physiological data with formatted ECG monitoring data, or of providing the other physiological data in a separate manner, are possible.

Processing continues (step **159**) for each remaining ECG datum, after which the processing loop is exited and execution terminates. Still other operations and steps are possible.

While the invention has been particularly shown and described as referenced to the embodiments thereof, those skilled in the art will understand that the foregoing and other changes in form and detail may be made therein without departing from the spirit and scope.

What is claimed is:

1. A remotely-interfaceable extended wear electrocardiography and physiological sensor monitor recorder, comprising:

a sealed housing forming on a bottom surface a cavity shaped to accommodate an upward projection of a battery compartment formed on a non-conductive receptacle of a disposable extended wear electrode patch and comprising a set of electrical contacts that protrude from the bottom surface and are arranged in alignment with electrical pads provided on the non-conductive receptacle;

a patient-operable tactile-feedback button provided on a top surface of the sealed housing; and electronic circuitry comprised within the sealed housing, comprising:

- an externally-powered micro-controller operable to execute under micro programmable control;
- an electrocardiographic front end circuit electrically interfaced to the micro-controller and operable to sense electrocardiographic signals through electrocardiographic electrodes provided on the disposable extended wear electrode patch;
- a wireless transceiver electrically interfaced with the micro-controller and operable to wirelessly interface with an external wireless-enabled device to communicate samples of the electrocardiographic signals; and
- externally-powered flash memory electrically interfaced with the micro-controller and operable to store the samples of the electrocardiographic signals.

2. An electrocardiography and physiological sensor monitor recorder according to claim 1, further comprising at least one of:

- a seal coupling circumferentially surrounding the set of electrical contacts.

3. An electrocardiography and physiological sensor monitor recorder according to claim 2, wherein the seal coupling securely mates with a moisture-resistant seal formed on the non-conductive receptacle.

4. An electrocardiography and physiological sensor monitor recorder according to claim 1, wherein a battery is provided in the battery compartment of the non-conductive receptacle of the extended wear electrode patch and powers the electronic circuitry.

5. An electrocardiography and physiological sensor monitor recorder according to claim 1, further comprising:

- a feedback buzzer utilized by the microcontroller.

6. An electrocardiography and physiological sensor monitor recorder according to claim 1, further comprising:

- an external physiological sensor provided with the circuitry and comprising at least one of an SpO2 sensor, blood pressure sensor, temperature sensor, respiratory rate sensor, glucose sensor, airflow sensor, and volumetric pressure sensor.

7. An electrocardiography and physiological sensor monitor recorder according to claim 1, wherein the sealed housing comprises a rounded isosceles trapezoidal-like shape.

8. An electrocardiography and physiological sensor monitor recorder according to claim 1, further comprising:

- a least one of a retention detent and a tension detent each molded along a top edge of a top surface of the sealed housing.

9. An electrocardiography and physiological sensor monitor recorder according to claim 8, wherein the retention detent and tension detent are shaped to engage respectively with a retention catch and a tension clip molded into the non-conductive receptacle.

10. A remotely-interfaceable extended wear electrocardiography and physiological sensor monitor, comprising:

- a disposable extended wear electrode patch comprising:
 - a flexible backing formed of an elongated strip of stretchable material with a narrow longitudinal mid-section and, on each end, a contact surface at least partially coated with an adhesive dressing provided as a crimp relief;
 - a pair of electrocardiographic electrodes conductively exposed on the contact surface of each end of the elongated strip, respectively;

- a non-conductive receptacle adhered to an outward-facing surface of the elongated strip and comprising a plurality of electrical pads; and
- a flexible circuit affixed on each end of the elongated strip as a strain relief and comprising a pair of circuit traces electrically coupled to the pair of the electrocardiographic electrodes and a pair of the electrical pads, at least one of the circuit traces adapted to extend along the narrow longitudinal midsection to serve as the strain relief; and

a reusable electrocardiography monitor having a sealed housing forming on a bottom surface a cavity shaped to accommodate an upward projection of a battery compartment formed on a non-conductive receptacle of a disposable extended wear electrode patch and comprising a patient-operable tactile-feedback button provided on a top surface of the sealed housing and a set of electrical contacts that protrude from the bottom surface and are arranged in alignment with the electrical pads provided on the non-conductive receptacle, wherein the reusable electrocardiography monitor comprises electronic circuitry, comprising:

- a micro-controller operable to execute under micro programmable control and electrically interfaced to an electrocardiographic front end circuit that is operable to sense electrocardiographic signals through the electrocardiographic electrodes via the pair of the electrical pads;
- a wireless transceiver electrically interfaced with the micro-controller and operable to wirelessly interface with an external wireless-enabled device to communicate samples of the electrocardiographic signals; and
- a flash memory electrically interfaced with the micro-controller and operable to store the samples of the electrocardiographic signals.

11. An electrocardiography and physiological sensor monitor according to claim 10, further comprising at least one of:

- a seal coupling circumferentially surrounding the set of electrical contacts.

12. An electrocardiography and physiological sensor monitor according to claim 11, wherein the seal coupling securely mates with a moisture-resistant seal formed on the non-conductive receptacle.

13. An electrocardiography and physiological sensor monitor according to claim 10, wherein a battery is provided in the battery compartment of the non-conductive receptacle of the extended wear electrode patch and powers the electronic circuitry.

14. An electrocardiography and physiological sensor monitor according to claim 10, further comprising:

- a feedback buzzer utilized by the microcontroller.

15. An electrocardiography and physiological sensor monitor according to claim 10, further comprising:

- an external physiological sensor provided with the circuitry and comprising at least one of an SpO2 sensor, blood pressure sensor, temperature sensor, respiratory rate sensor, glucose sensor, airflow sensor, and volumetric pressure sensor.

16. An electrocardiography and physiological sensor monitor according to claim 10, wherein the sealed housing comprises a rounded isosceles trapezoidal-like shape.

17. An electrocardiography and physiological sensor monitor according to claim 10, further comprising:

a least one of a retention detent and a tension detent each molded along a top edge of a top surface of the sealed housing.

18. An electrocardiography and physiological sensor monitor according to claim 17, wherein the retention detent and tension detent are shaped to engage respectively with a retention catch and a tension clip molded into the non-conductive receptacle.

* * * * *

| | | | |
|----------------|---|---------|------------|
| 专利名称(译) | 扩展磨损心电图与生理传感器监测仪的远程接口 | | |
| 公开(公告)号 | US9820665 | 公开(公告)日 | 2017-11-21 |
| 申请号 | US15/256266 | 申请日 | 2016-09-02 |
| [标]申请(专利权)人(译) | BARDY诊断 | | |
| 申请(专利权)人(译) | BARDY诊断, INC | | |
| 当前申请(专利权)人(译) | BARDY诊断, INC. | | |
| [标]发明人 | FELIX JASON BISHAY JON MIKALSON BARDY GUST H | | |
| 发明人 | FELIX, JASON BISHAY, JON MIKALSON BARDY, GUST H. | | |
| IPC分类号 | A61B5/00 A61B5/0432 A61B5/0408 A61B5/0205 A61B5/145 A61B5/021 A61B5/03 A61B5/0452 A61B5/11 A61B5/1455 A61B5/08 A61B5/087 | | |
| CPC分类号 | A61B5/04325 A61B5/0022 A61B5/02055 A61B5/04085 A61B5/04087 A61B5/14532 A61B5/14542 A61B5/6823 A61B5/7405 A61B5/7455 A61B5/7475 A61B5/0006 A61B2560/0214 A61B5/021 A61B5/03 A61B5/0452 A61B5/087 A61B5/0816 A61B5/1118 A61B5/14551 G06F19/00 G16H40/67 | | |
| 优先权 | 61/882403 2013-09-25 US | | |
| 其他公开文献 | US20160367164A1 | | |
| 外部链接 | Espacenet USPTO | | |

摘要(译)

提供了一种可远程连接的延长磨损心电图和生理传感器监视记录器。密封壳体在底表面上形成腔，该腔被成形为容纳形成在一次性延长耐磨电极贴片的非导电插座上的电池盒的向上突出，并且包括从底表面突出并被布置的一组电触点。与设置在非导电插座上的电焊盘对齐。电子电路设置在密封壳体内，并包括外部供电的微控制器，其可操作以在微可编程控制下执行。心电图前端电路与微控制器电连接。无线收发器与微控制器电连接，并且外部供电的闪存与微控制器电连接并且可操作以存储心电图信号的样本。

