



US 20150025403A1

(19) **United States**

(12) **Patent Application Publication**
CHANG et al.

(10) **Pub. No.: US 2015/0025403 A1**
(43) **Pub. Date: Jan. 22, 2015**

(54) **MOOD ANALYSIS METHOD, SYSTEM, AND APPARATUS**

(71) Applicants: **Chiun Mai Communication Systems, Inc.**, New Taipei (TW); **YongLin Biotech Corp.**, New Taipei (TW)

(72) Inventors: **MING-SHIUNG CHANG**, New Taipei (TW); **HSUN-KO CHAN**, New Taipei (TW); **DANIEL M. WENG**, Santa Clara, CA (US); **SHU-CHEN CHUANG**, New Taipei (TW); **TUAN-CHUN CHEN**, New Taipei (TW); **PEI-CHI HO**, New Taipei (TW); **HSIANG-I KAO**, New Taipei (TW); **SHING-HUEI LIN**, New Taipei (TW)

(73) Assignees: **YONGLIN BIOTECH CORP.**, New Taipei (TW); **CHIUN MAI COMMUNICATION SYSTEMS, INC.**, New Taipei (TW)

(21) Appl. No.: **14/253,822**

(22) Filed: **Apr. 15, 2014**

(30) **Foreign Application Priority Data**


Apr. 15, 2013 (TW) 102113369

Publication Classification

(51) **Int. Cl.**
A61B 5/16 (2006.01)
A61B 5/00 (2006.01)
A61B 5/0456 (2006.01)
(52) **U.S. Cl.**
CPC *A61B 5/165* (2013.01); *A61B 5/0456* (2013.01); *A61B 5/7271* (2013.01)
USPC **600/521**

(57) **ABSTRACT**

In a mood analysis method using an electrocardiogram of a user, RR intervals in the electrocardiogram are computed, and low-frequency (LF) values and high-frequency (HF) values are also computed according to the RR intervals. Standard values of sympathetic nervous system (SNS) activity and parasympathetic nervous system (PSNS) activity are acquired corresponding to age and sex data of the user, to establish a mood display coordinate system. Coordinates of the LF values and the HF values in the mood display coordinate system are computed to determine a mood of the user.

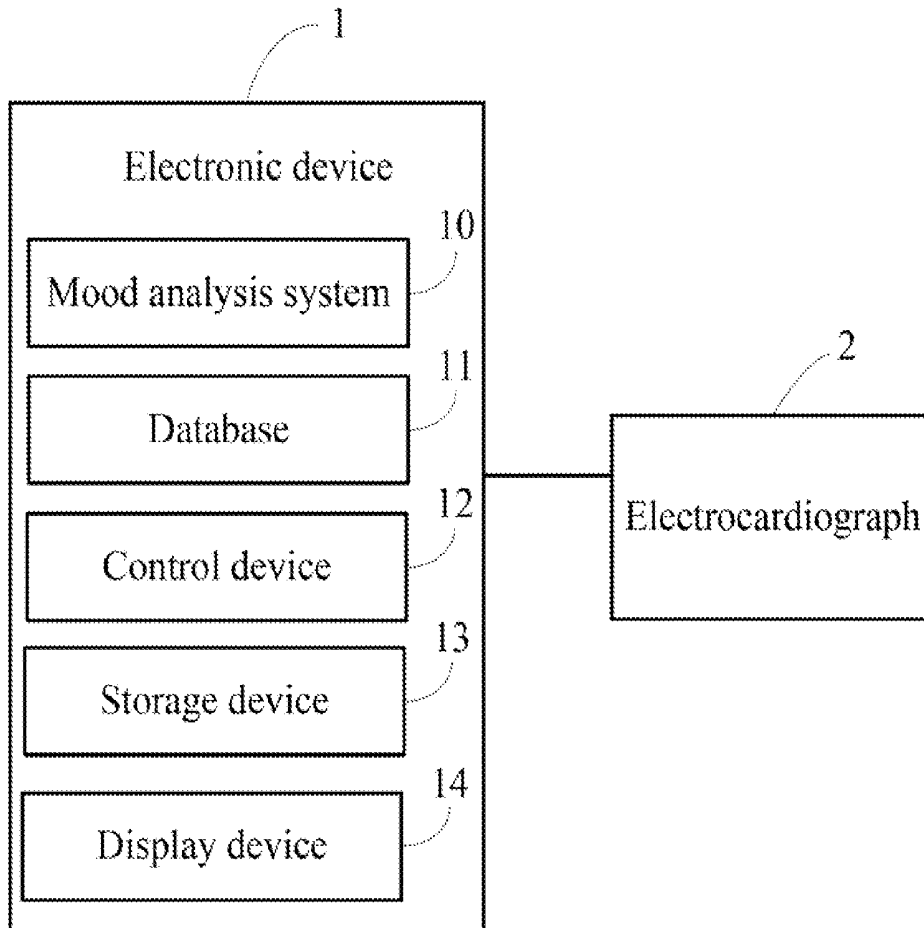

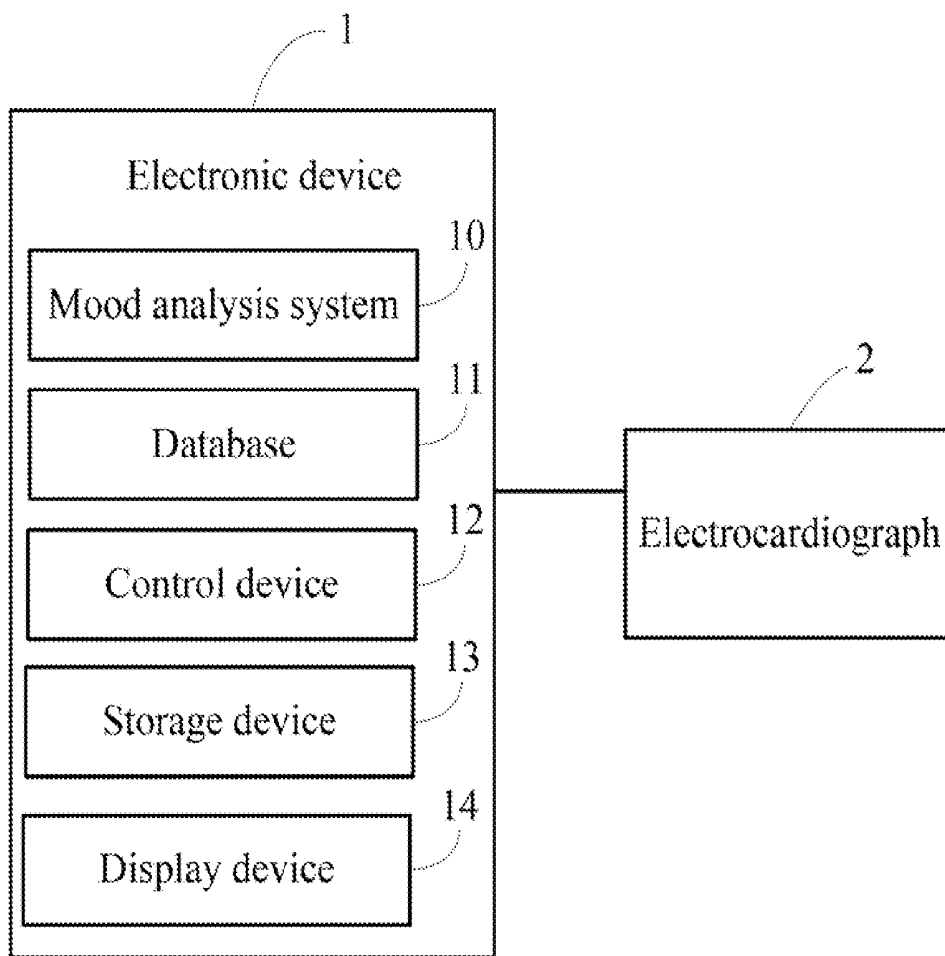


FIG. 1

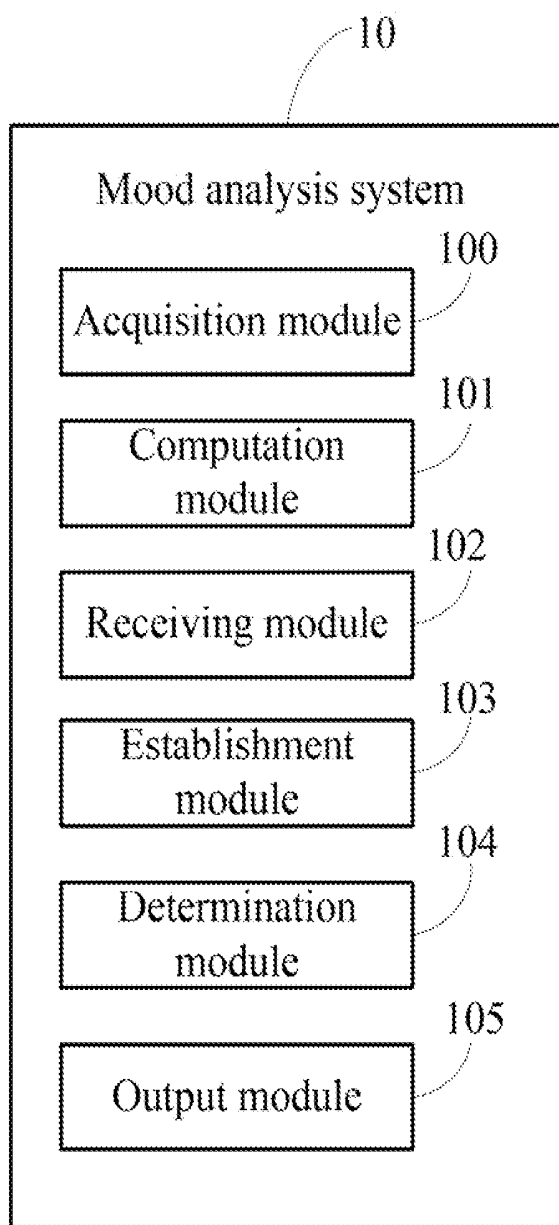


FIG. 2

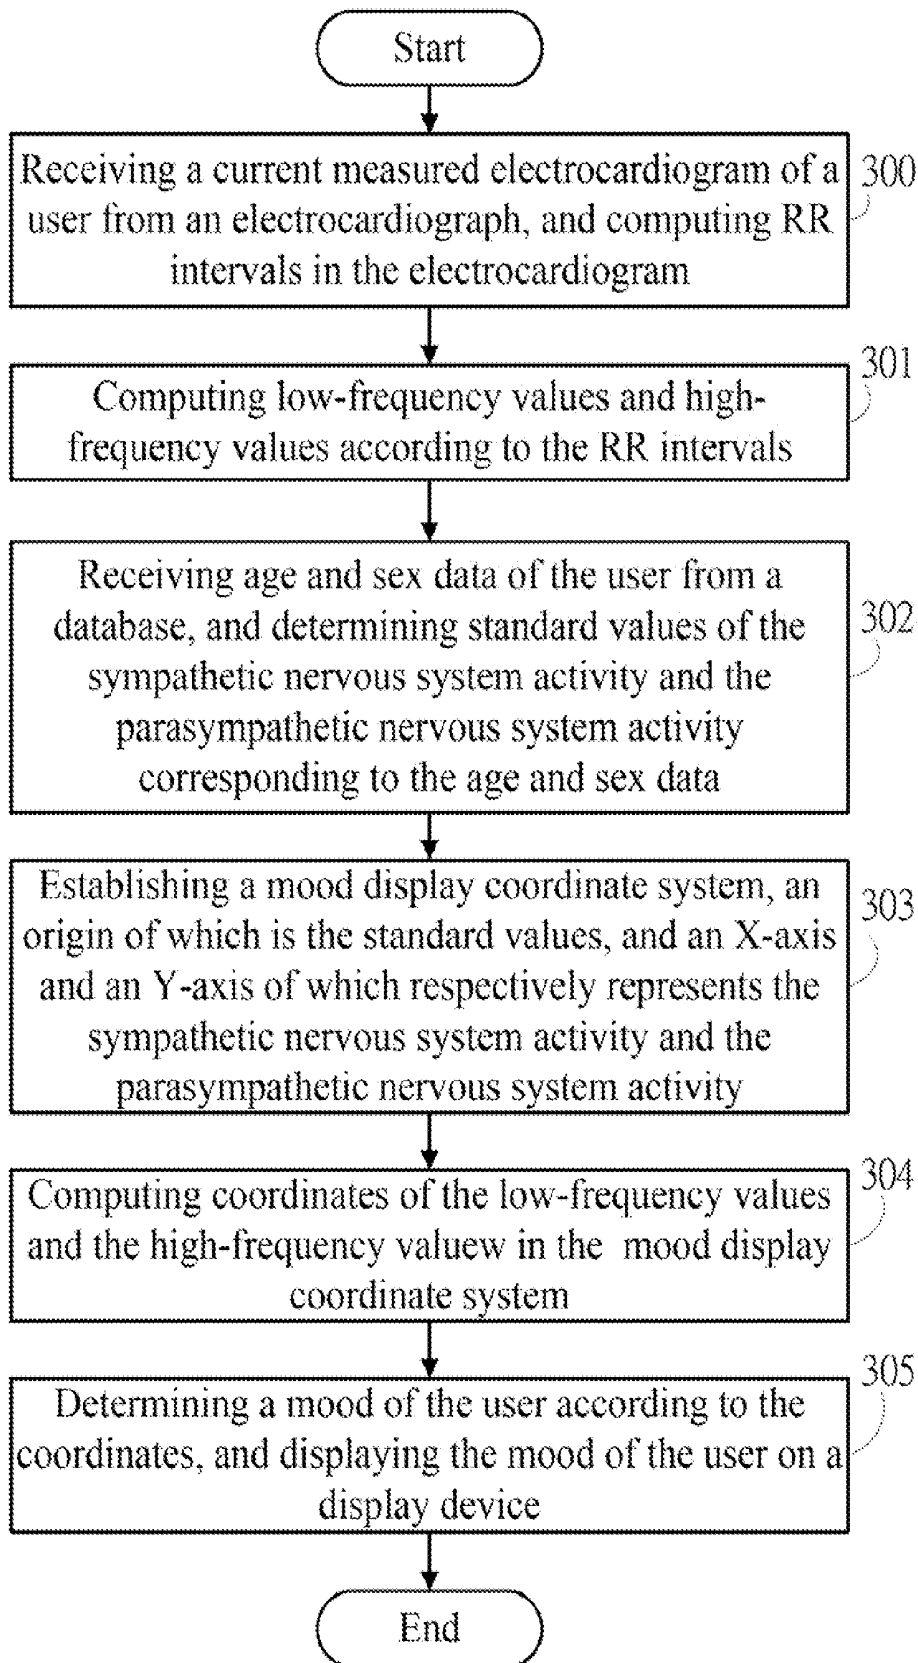


FIG. 3

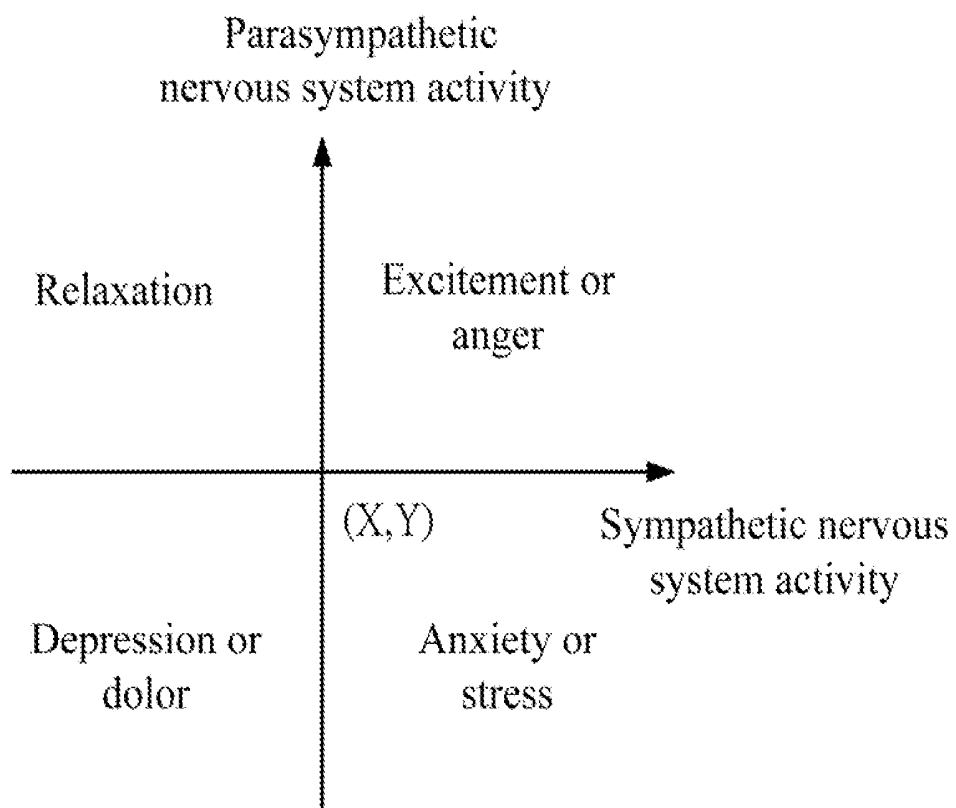


FIG. 4

MOOD ANALYSIS METHOD, SYSTEM, AND APPARATUS

FIELD

[0001] Embodiments of the present disclosure relate to an electrocardiogram (ECG) analysis technique, and more specifically relates to an apparatus, a method, and a system to analyze an ECG of a user to determine a mood of the user.

BACKGROUND

[0002] An electrocardiogram (ECG) is used to measure the heart's electrical conduction system. The ECG measures electrical impulses generated by the polarization and depolarization of cardiac tissue, and translates the electrical impulses into a wave, which is used to measure the rate and regularity of heartbeats. The wave comprises a P wave, a QRS complex, a T wave, and a U wave. The QRS complex includes a plurality of R waves.

[0003] A RR interval, namely the interval between two adjacent R waves, can be used to measure a heart rate. The heart rate can vary due to physical exercise, mood, and so on.

[0004] Usually, the ECG can only be read by experts, for example medical staffs.

BRIEF DESCRIPTION OF THE DRAWINGS

[0005] FIG. 1 is a block diagram of one example embodiment of a hardware environment for executing a mood analysis system.

[0006] FIG. 2 is a block diagram of one example embodiment of function modules of the mood analysis system in FIG. 1.

[0007] FIG. 3 is a flowchart of one example embodiment of a mood analysis method.

[0008] FIG. 4 illustrates an example mood display coordinate system.

DETAILED DESCRIPTION

[0009] The disclosure is illustrated by way of example and not by way of limitation in the figures of the accompanying drawings in which like references indicate similar elements. It should be noted that references to "an" or "one" embodiment in this disclosure are not necessarily to the same embodiment, and such references mean "at least one." The references "a plurality of" and "a number of" mean "at least two."

[0010] In general, the word "module," as used hereinafter, refers to logic embodied in hardware or firmware, or to a collection of software instructions, written in a programming language, such as, for example, Java, C, or assembly. One or more software instructions in the modules may be embedded in firmware. It will be appreciated that modules may comprise connected logic units, such as gates and flip-flops, and may comprise programmable units, such as programmable gate arrays or processors. The modules described herein may be implemented as either software and/or hardware modules and may be stored in any type of non-transitory computer-readable storage medium or other computer storage device.

[0011] FIG. 1 is a block diagram of one embodiment of a hardware environment for executing a mood analysis system 10. The mood analysis system 10 is installed and ran on an electronic device 1, for example a computer, a smart phone, server, or a smart TV. The electronic device 1 can include a database 11, a control device 12, a storage device 13, and a

display device 14. In one embodiment, the electronic device 1 is electrically connected to an electrocardiograph 2 for receiving an electrocardiogram (ECG) of one or more users.

[0012] The mood analysis system 10 can include a plurality of function modules (shown in FIG. 2) that analyze and display moods of users in accordance to users' ECGs.

[0013] The database 11 can be installed in the electronic device 1 or be externally connected with the electronic device 1. The database 11 stores standard values of the sympathetic nervous system (SNS) activity and the parasympathetic nervous system (PSNS) activity of users corresponding to a user's age and sex.

[0014] The control device 12 can be a processor, an application-specific integrated circuit (ASIC), or a field programmable gate array (FPGA), for example. The control device 12 can execute computerized codes of the function modules of the mood analysis system 10 to realize the functions of the electronic device 1.

[0015] The storage device 13 can include some type(s) of non-transitory computer-readable storage medium, for example a hard disk drive, a compact disc, a digital video disc, or a tape drive. The storage device 13 stores the computerized codes of the function modules of the mood analysis system 10.

[0016] FIG. 2 is a block diagram of one embodiment of function modules of the mood analysis system 10. The function modules can include an acquisition module 100, a computation module 101, a receiving module 102, an establishment module 103, a determination module 104, and an output module 105. The function modules 100-105 can include computerized codes in the form of one or more programs, which provide at least the functions needed to execute the steps illustrated in FIG. 3.

[0017] FIG. 3 is a flowchart of one example embodiment of a mood analysis method. In the embodiment, the method is performed by execution of computer-readable software program codes or instructions by at least one processor (i.e., the control device 12) of the electronic device 1. Depending on the embodiment, additional steps in FIG. 3 can be added, removed, and the ordering of the steps can be changed.

[0018] In 300, the acquisition module 100 receives a current measured electrocardiogram of a user from the electrocardiograph 2, and determines RR intervals in the electrocardiogram. In the embodiment, the RR interval is defined as an interval between two adjacent R waves in the electrocardiogram.

[0019] In 301, the computation module 101 computes low-frequency (LF) values and high-frequency (HF) values according to the RR intervals using Fourier transformation. The LF values represent current values of SNS activity, and the HF values represent current values of PSNS activity of the user.

[0020] In 302, the receiving module 102 acquires age and sex data of the user from the database 11, and determines standard values of the SNS activity and the PSNS activity corresponding to the age and sex data of the user. The age and sex data can be input by the user through a user interface (UI), or can be received from the database 11.

[0021] In 303, the establishment module 103 establishes a mood display coordinate system, wherein an origin of the mood display coordinate system is the standard values of the SNS activity and the PSNS activity corresponding to the age and sex data of the user, and an X-axis and Y-axis of the mood display coordinate system respectively represent the SNS

activity and the PSNS activity. FIG. 4 illustrates an example mood display coordinate system. Coordinates in the first quadrant of the mood display coordinate system can represent excitement or anger. Coordinates in the second quadrant can represent relaxation. Coordinates in the third quadrant can represent depression or dolor. Coordinates in the fourth quadrant can represent anxiety and stress.

[0022] In 304, the determination module 104 computes coordinates of the LF values and the HF values in the mood display coordinate system. The coordinates (X, Y) of the LF values and the HF values are represented by the following equations:

$$X = \text{LF values} - \text{the standard values of the SNS activity};$$

$$Y = \text{HF values} - \text{the standard values of the PSNS activity}.$$

[0023] In 305, the output module 105 determines a current mood of the user according to the computed coordinates, and displays the mood of the user on the display device 14. When the coordinates of the LF values and the HF values are in the first quadrant of the mood display coordinate system, the output module 105 determines that the current mood of the user is excitement or anger. When the coordinates of the LF values and the HF values are in the second quadrant of the mood display coordinate system, the output module 105 determines that the current mood of the user is relaxation.

[0024] When the coordinates of the LF values and the HF values are in the third quadrant of the mood display coordinate system, the output module 105 determines that the current mood of the user is depression or dolor. When the coordinates of the LF values and the HF values are in the fourth quadrant of the mood display coordinate system, the output module 105 determines that the current mood of the user is anxiety or stress.

[0025] It should be emphasized that the above-described embodiments of the present disclosure, including any particular embodiments, are merely possible examples of implementations, set forth for a clear understanding of the principles of the disclosure. Many variations and modifications may be made to the above-described embodiment(s) of the disclosure without departing substantially from the spirit and principles of the disclosure. All such modifications and variations are intended to be included herein within the scope of this disclosure and protected by the following claims.

What is claimed is:

1. A mood analysis method being executed by at least one processor of an electronic device, the method comprising:
 - receiving a current measured electrocardiogram of a user from an electrocardiograph, and computing RR intervals in the electrocardiogram;
 - computing low-frequency (LF) values and high-frequency (HF) values according to the RR intervals;
 - receiving age and sex data of the user from a database, and determining standard values of sympathetic nervous system (SNS) activity and parasympathetic nervous system (PSNS) activity corresponding to the age and sex data of the user;
 - establishing a mood display coordinate system using the standard values of the SNS activity and the PSNS activity;
 - computing coordinates of the LF values and the HF values in the mood display coordinate system; and

determining a current mood of the user according to the computed coordinates, and displaying the mood of the user on a display device of the electronic device.

2. The method according to claim 1, further comprising:
 - storing standard values of the SNS activity and the PSNS activity of users corresponding to different age and sex data into the database which is installed in the electronic device or externally connected with the electronic device.

3. The method according to claim 1, wherein an origin of the mood display coordinate system is the standard values of the SNS activity and the PSNS activity corresponding to the age and sex data of the user, and an X-axis and an Y-axis of the mood display coordinate system respectively represent the SNS activity and the PSNS activity.

4. The method according to claim 1, wherein the coordinates (X, Y) of the LF values and the HF values are computed by:

$$X = \text{LF values} - \text{the standard values of the SNS activity};$$

and

$$Y = \text{HF values} - \text{the standard values of the PSNS activity}.$$

5. The method according to claim 1, wherein the current mood of the user is determined as excitement or anger when the coordinates of the LF values and the HF values are in a first quadrant of the mood display coordinate system, the current mood of the user is determined as relaxation when the coordinates of the LF values and the HF values are in the second quadrant of the mood display coordinate system, the current mood of the user is determined as depression or dolor when the coordinates of the LF values and the HF values are in a third quadrant of the mood display coordinate system, and the current mood of the user is determined as anxiety or stress when the coordinates of the LF values and the HF values are in a fourth quadrant of the mood display coordinate system.

6. An apparatus, comprising:

- a display device;
- a control device; and
- a storage device storing one or more programs which when executed by the control device, causes the control device to:

- receive a current measured electrocardiogram of a user from an electrocardiograph, and compute RR intervals in the electrocardiogram;

- compute low-frequency (LF) values and high-frequency (HF) values according to the RR intervals;

- receive age and sex data of the user from a database, and determining standard values of sympathetic nervous system (SNS) activity and parasympathetic nervous system (PSNS) activity corresponding to the age and sex data of the user;

- establish a mood display coordinate system using the standard values of the SNS activity and the PSNS activity;
- compute coordinates of the LF values and the HF values in the mood display coordinate system; and

- determine a current mood of the user according to the computed coordinates, and display the mood of the user on the display device.

7. The apparatus according to claim 6, wherein the database is installed in the electronic device or externally connected with the electronic device, and stores standard values of the SNS activity and the PSNS activity of users corresponding to different age and sex data.

8. The apparatus according to claim 6, wherein an origin of the mood display coordinate system is the standard values of the SNS activity and the PSNS activity corresponding to the age and sex data of the user, and an X-axis and an Y-axis of the mood display coordinate system respectively represent the SNS activity and the PSNS activity.

9. The apparatus according to claim 6, wherein the coordinates (X, Y) of the LF values and the HF values are computed by:

X =LF values—the standard values of the SNS activity;
and

Y =HF values—the standard values of the PSNS activity.

10. The apparatus according to claim 6, wherein when the coordinates of the LF values and the HF values are in the first quadrant of the mood display coordinate system, the current mood of the user is determined as excitement or anger, when the coordinates of the LF values and the HF values are in the second quadrant of the mood display coordinate system, the current mood of the user is determined as relaxation, when the coordinates of the LF values and the HF values are in the third quadrant of the mood display coordinate system, the current mood of the user is determined as depression or dolor, and when the coordinates of the LF values and the HF values are in the fourth quadrant of the mood display coordinate system, the current mood of the user is determined as anxiety or stress.

11. A non-transitory storage medium having stored thereon instructions that, when executed by a processor of an electronic device, causes the processor to perform a mood analysis method, wherein the method comprises:

receiving a current measured electrocardiogram of a user from an electrocardiograph, and computing RR intervals in the electrocardiogram;

computing low-frequency (LF) values and high-frequency (HF) values according to the RR intervals;

receiving age and sex data of the user from a database, and determining standard values of sympathetic nervous system (SNS) activity and parasympathetic nervous system (PSNS) activity corresponding to the age and sex data of the user;

establishing a mood display coordinate system using the standard values of the SNS activity and the PSNS activity;

computing coordinates of the LF values and the HF values in the mood display coordinate system; and

determining a current mood of the user according to the computed coordinates, and displaying the mood of the user on a display device of the electronic device.

12. The non-transitory storage medium according to claim 11, wherein the method further comprises:

storing standard values of the SNS activity and the PSNS activity of users corresponding to different age and sex data into the database which is installed in the electronic device or externally connected with the electronic device.

13. The non-transitory storage medium according to claim 11, wherein an origin of the mood display coordinate system is the standard values of the SNS activity and the PSNS activity corresponding to the age and sex data of the user, and an X-axis and an Y-axis of the mood display coordinate system respectively represent the SNS activity and the PSNS activity.

14. The non-transitory storage medium according to claim 11, wherein the coordinates (X, Y) of the LF values and the HF values are computed by:

X =LF values—the standard values of the SNS activity;
and

Y =HF values—the standard values of the PSNS activity.

15. The non-transitory storage medium according to claim 11, wherein the current mood of the user is determined as excitement or anger when the coordinates of the LF values and the HF values are in a first quadrant of the mood display coordinate system, the current mood of the user is determined as relaxation when the coordinates of the LF values and the HF values are in the second quadrant of the mood display coordinate system, the current mood of the user is determined as depression or dolor when the coordinates of the LF values and the HF values are in a third quadrant of the mood display coordinate system, and the current mood of the user is determined as anxiety or stress when the coordinates of the LF values and the HF values are in a fourth quadrant of the mood display coordinate system.

* * * * *

专利名称(译)	情绪分析方法，系统和装置		
公开(公告)号	US20150025403A1	公开(公告)日	2015-01-22
申请号	US14/253822	申请日	2014-04-15
[标]申请(专利权)人(译)	奇美通讯股份有限公司		
申请(专利权)人(译)	CHIUN MAI通信系统，INC. 永林BIOTECH CORP.		
当前申请(专利权)人(译)	永林BIOTECH CORP. CHIUN MAI通信系统，INC.		
[标]发明人	CHANG MING SHIUNG CHAN HSUN KO M WENG DANIEL CHUANG SHU CHEN CHEN TUAN CHUN HO PEI CHI KAO HSIANG I LIN SHING HUEI		
发明人	CHANG, MING-SHIUNG CHAN, HSUN-KO M. WENG, DANIEL CHUANG, SHU-CHEN CHEN, TUAN-CHUN HO, PEI-CHI KAO, HSIANG-I LIN, SHING-HUEI		
IPC分类号	A61B5/0456 A61B5/00 A61B5/16 G16H10/60		
CPC分类号	A61B5/165 A61B5/7271 A61B5/0456 A61B5/7257		
优先权	102113369 2013-04-15 TW		
其他公开文献	US9398874		
外部链接	Espacenet USPTO		

摘要(译)

在使用用户的心电图的情绪分析方法中，计算心电图中的RR间隔，并且还根据RR间隔计算低频（LF）值和高频（HF）值。根据用户的年龄和性别数据获取交感神经系统（SNS）活动和副交感神经系统（PSNS）活动的标准值，以建立情绪显示坐标系。计算情绪显示坐标系中的LF值和HF值的坐标以确定用户的情绪。

