



US010492705B2

(12) **United States Patent**  
**Bank et al.**

(10) **Patent No.:** **US 10,492,705 B2**  
(45) **Date of Patent:** **Dec. 3, 2019**

(54) **ANTERIOR AND POSTERIOR ELECTRODE SIGNALS**

(71) Applicants: **REGENTS OF THE UNIVERSITY OF MINNESOTA**, Minneapolis, MN (US); **ALLINA HEALTH SYSTEM**, St. Paul, MN (US)

(72) Inventors: **Alan J. Bank**, Edina, MN (US); **Antonia E. Curtin**, Minneapolis, MN (US); **Ryan M. Gage**, Minneapolis, MN (US); **Kevin V. Burns**, St. Anthony, MN (US)

(73) Assignees: **REGENTS OF THE UNIVERSITY OF MINNESOTA**, Minneapolis, MN (US); **ALLINA HEALTH SYSTEM**, St. Paul, MN (US)

(\* ) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(21) Appl. No.: **16/229,256**

(22) Filed: **Dec. 21, 2018**

(65) **Prior Publication Data**

US 2019/0192035 A1 Jun. 27, 2019

**Related U.S. Application Data**

(60) Provisional application No. 62/609,935, filed on Dec. 22, 2017.

(51) **Int. Cl.**

**A61B 5/04** (2006.01)

**A61B 5/0408** (2006.01)

(Continued)

(52) **U.S. Cl.**

CPC ..... **A61B 5/04087** (2013.01); **A61B 5/04011** (2013.01); **A61B 5/0452** (2013.01);

(Continued)

(58) **Field of Classification Search**

CPC ..... A61B 5/04087; A61B 5/04011; A61B 5/7203; A61B 5/6823; A61B 5/6805; A61N 1/3904; A61N 1/3627; A61N 1/3956

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

4,233,987 A 11/1980 Feingold

4,402,323 A 9/1983 White

(Continued)

**FOREIGN PATENT DOCUMENTS**

CN 1043621 A 11/1990

CN 1253761 A 5/2000

(Continued)

**OTHER PUBLICATIONS**

International Search Report and Written Opinion dated May 3, 2012 for International Application No. PCT/US2012/036262; 9 pages.

(Continued)


*Primary Examiner* — Rex R Holmes

(74) *Attorney, Agent, or Firm* — Mueting, Raasch & Gebhardt, PA

(57) **ABSTRACT**

The exemplary systems, methods, and interfaces may obtain and analyze electrode signals from a plurality of external electrodes. The electrode signals may include at least an anterior set of electrode signals and a posterior set of electrode signals. The anterior and posterior sets of electrode signals may be used to generate, or provide, various metrics of cardiac electrical heterogeneity and various graphical depictions that may be useful in assessing a patient's cardiac functionality.

**22 Claims, 18 Drawing Sheets**

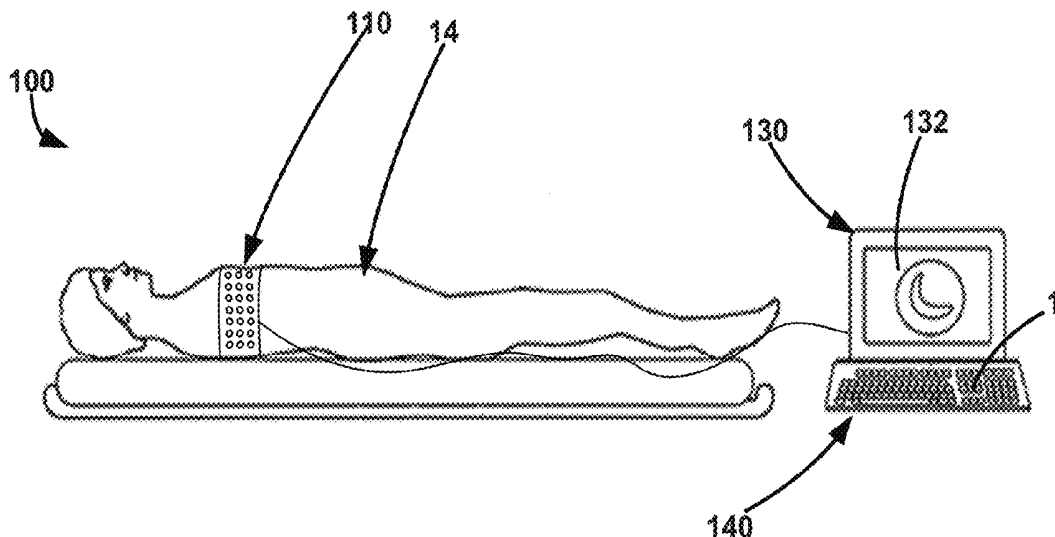

- (51) **Int. Cl.**  
*A61N 1/39* (2006.01)  
*A61B 5/00* (2006.01)  
*A61B 5/0452* (2006.01)  
*A61N 1/362* (2006.01)
- (52) **U.S. Cl.**  
 CPC ..... *A61B 5/04085* (2013.01); *A61B 5/7203*  
 (2013.01); *A61N 1/3904* (2017.08); *A61B*  
*5/6805* (2013.01); *A61B 5/6823* (2013.01);  
*A61N 1/3627* (2013.01); *A61N 1/3956*  
 (2013.01)
- (56) **References Cited**
- U.S. PATENT DOCUMENTS
- |           |    |         |                  |           |    |         |                   |
|-----------|----|---------|------------------|-----------|----|---------|-------------------|
| 4,428,378 | A  | 1/1984  | Anderson et al.  | 6,882,882 | B2 | 4/2005  | Struble et al.    |
| 4,497,326 | A  | 2/1985  | Curry            | 6,885,889 | B2 | 4/2005  | Chinchoy          |
| 4,566,456 | A  | 1/1986  | Koning et al.    | 6,915,149 | B2 | 7/2005  | Ben-Haim          |
| 4,593,702 | A  | 6/1986  | Kepski           | 6,968,237 | B2 | 11/2005 | Doan et al.       |
| 4,674,511 | A  | 6/1987  | Cartmell         | 6,975,900 | B2 | 12/2005 | Rudy et al.       |
| 4,763,660 | A  | 8/1988  | Kroll et al.     | 6,978,184 | B1 | 12/2005 | Marcus et al.     |
| 4,777,955 | A  | 10/1988 | Brayten et al.   | 6,980,675 | B2 | 12/2005 | Evron et al.      |
| 4,787,389 | A  | 11/1988 | Tarjan           | 7,016,719 | B2 | 3/2006  | Rudy et al.       |
| 4,979,507 | A  | 12/1990 | Heinz et al.     | 7,031,777 | B2 | 4/2006  | Hine et al.       |
| 5,052,388 | A  | 10/1991 | Sivula et al.    | 7,058,443 | B2 | 6/2006  | Struble           |
| 5,054,496 | A  | 10/1991 | Wen et al.       | 7,062,315 | B2 | 6/2006  | Koyrakh et al.    |
| 5,311,873 | A  | 5/1994  | Savard et al.    | 7,092,759 | B2 | 8/2006  | Nehls et al.      |
| 5,331,960 | A  | 7/1994  | Lavine           | 7,142,922 | B2 | 11/2006 | Spinelli et al.   |
| 5,334,220 | A  | 8/1994  | Sholder          | 7,184,835 | B2 | 2/2007  | Kramer et al.     |
| 5,443,492 | A  | 8/1995  | Stokes et al.    | 7,215,998 | B2 | 5/2007  | Wesselink et al.  |
| 5,485,849 | A  | 1/1996  | Panescu et al.   | 7,238,158 | B2 | 7/2007  | Abend             |
| 5,514,163 | A  | 5/1996  | Markowitz et al. | 7,286,866 | B2 | 10/2007 | Okerlund et al.   |
| 5,552,645 | A  | 9/1996  | Weng             | 7,308,297 | B2 | 12/2007 | Reddy et al.      |
| 5,628,778 | A  | 5/1997  | Kruse et al.     | 7,308,299 | B2 | 12/2007 | Burrell et al.    |
| 5,671,752 | A  | 9/1997  | Sinderby et al.  | 7,313,444 | B2 | 12/2007 | Pianca et al.     |
| 5,683,429 | A  | 11/1997 | Mehra            | 7,321,677 | B2 | 1/2008  | Evron et al.      |
| 5,683,432 | A  | 11/1997 | Goedeke et al.   | 7,346,381 | B2 | 3/2008  | Okerlund et al.   |
| 5,687,737 | A  | 11/1997 | Branham et al.   | 7,398,116 | B2 | 7/2008  | Edwards           |
| 5,810,740 | A  | 9/1998  | Paisner          | 7,426,412 | B1 | 9/2008  | Schechter         |
| 5,876,336 | A  | 3/1999  | Swanson et al.   | 7,454,248 | B2 | 11/2008 | Burrell et al.    |
| 5,891,045 | A  | 4/1999  | Albrecht et al.  | 7,499,743 | B2 | 3/2009  | Vass et al.       |
| 5,922,014 | A  | 7/1999  | Warman et al.    | 7,509,170 | B2 | 3/2009  | Zhang et al.      |
| 6,055,448 | A  | 4/2000  | Anderson et al.  | 7,565,190 | B2 | 7/2009  | Okerlund et al.   |
| 6,128,535 | A  | 10/2000 | Maarse et al.    | 7,587,074 | B2 | 9/2009  | Zarkh et al.      |
| 6,141,588 | A  | 10/2000 | Cox et al.       | 7,599,730 | B2 | 10/2009 | Hunter et al.     |
| 6,187,032 | B1 | 2/2001  | Ohyu et al.      | 7,610,088 | B2 | 10/2009 | Chinchoy          |
| 6,205,357 | B1 | 3/2001  | Ideker et al.    | 7,613,500 | B2 | 11/2009 | Vass et al.       |
| 6,226,542 | B1 | 5/2001  | Reisfeld         | 7,616,993 | B2 | 11/2009 | Müssig et al.     |
| 6,236,883 | B1 | 5/2001  | Ciaccio et al.   | 7,664,550 | B2 | 2/2010  | Ejck et al.       |
| 6,243,603 | B1 | 6/2001  | Ideker et al.    | 7,684,863 | B2 | 3/2010  | Pariikh et al.    |
| 6,246,898 | B1 | 6/2001  | Vesely et al.    | 7,742,629 | B2 | 6/2010  | Zarkh et al.      |
| 6,301,496 | B1 | 10/2001 | Reisfeld         | 7,747,047 | B2 | 6/2010  | Okerlund et al.   |
| 6,311,089 | B1 | 10/2001 | Mann et al.      | 7,751,882 | B1 | 7/2010  | Helland et al.    |
| 6,330,476 | B1 | 12/2001 | Ben-Haim et al.  | 7,769,451 | B2 | 8/2010  | Yang et al.       |
| 6,358,214 | B1 | 3/2002  | Tereschouk       | 7,778,685 | B2 | 8/2010  | Evron et al.      |
| 6,377,856 | B1 | 4/2002  | Carson           | 7,778,686 | B2 | 8/2010  | Vass et al.       |
| 6,381,493 | B1 | 4/2002  | Stadler et al.   | 7,787,951 | B1 | 8/2010  | Min               |
| 6,393,316 | B1 | 5/2002  | Gillberg et al.  | 7,813,785 | B2 | 10/2010 | Okerlund et al.   |
| 6,418,346 | B1 | 7/2002  | Nelson et al.    | 7,818,040 | B2 | 10/2010 | Spear et al.      |
| 6,442,433 | B1 | 8/2002  | Linberg          | 7,848,807 | B2 | 12/2010 | Wang              |
| 6,456,867 | B2 | 9/2002  | Reisfeld         | 7,860,580 | B2 | 12/2010 | Falk et al.       |
| 6,473,638 | B2 | 10/2002 | Ferek-Petric     | 7,894,889 | B2 | 2/2011  | Zhang             |
| 6,480,745 | B2 | 11/2002 | Nelson et al.    | 7,912,544 | B1 | 3/2011  | Min et al.        |
| 6,484,118 | B1 | 11/2002 | Govari           | 7,917,214 | B1 | 3/2011  | Gill et al.       |
| 6,507,756 | B1 | 1/2003  | Heynen et al.    | 7,941,213 | B2 | 5/2011  | Markowitz et al.  |
| 6,532,379 | B2 | 3/2003  | Stratbucker      | 7,953,475 | B2 | 5/2011  | Harlev et al.     |
| 6,584,343 | B1 | 6/2003  | Ransbury et al.  | 7,953,482 | B2 | 5/2011  | Hess              |
| 6,599,250 | B2 | 7/2003  | Webb et al.      | 7,983,743 | B2 | 7/2011  | Rudy et al.       |
| 6,625,482 | B1 | 9/2003  | Panescu et al.   | 7,996,063 | B2 | 8/2011  | Vass et al.       |
| 6,640,136 | B1 | 10/2003 | Helland et al.   | 7,996,070 | B2 | 8/2011  | van Dam et al.    |
| 6,650,927 | B1 | 11/2003 | Keidar           | 8,010,194 | B2 | 8/2011  | Muller            |
| 6,766,189 | B2 | 7/2004  | Yu et al.        | 8,019,402 | B1 | 9/2011  | Kryzpow et al.    |
| 6,772,004 | B2 | 8/2004  | Rudy             | 8,019,409 | B2 | 9/2011  | Rosenberg et al.  |
| 6,804,555 | B2 | 10/2004 | Warkentin        | 8,032,229 | B2 | 10/2011 | Gerber et al.     |
| 6,847,836 | B1 | 1/2005  | Sujdak           | 8,036,743 | B2 | 10/2011 | Savage et al.     |
| 6,856,830 | B2 | 2/2005  | He               | 8,060,185 | B2 | 11/2011 | Hunter et al.     |
|           |    |         |                  | 8,150,513 | B2 | 4/2012  | Chinchoy          |
|           |    |         |                  | 8,160,700 | B1 | 4/2012  | Ryu et al.        |
|           |    |         |                  | 8,175,703 | B2 | 5/2012  | Dong et al.       |
|           |    |         |                  | 8,180,428 | B2 | 5/2012  | Kaiser et al.     |
|           |    |         |                  | 8,195,292 | B2 | 6/2012  | Rosenberg et al.  |
|           |    |         |                  | 8,213,693 | B1 | 7/2012  | Li                |
|           |    |         |                  | 8,214,041 | B2 | 7/2012  | Van Gelder et al. |
|           |    |         |                  | 8,265,738 | B1 | 9/2012  | Min et al.        |
|           |    |         |                  | 8,285,377 | B2 | 10/2012 | Rosenberg et al.  |
|           |    |         |                  | 8,295,943 | B2 | 10/2012 | Eggen et al.      |
|           |    |         |                  | 8,326,419 | B2 | 12/2012 | Rosenberg et al.  |
|           |    |         |                  | 8,332,030 | B2 | 12/2012 | Hess et al.       |
|           |    |         |                  | 8,380,308 | B2 | 2/2013  | Rosenberg et al.  |
|           |    |         |                  | 8,401,616 | B2 | 3/2013  | Verard et al.     |
|           |    |         |                  | 8,478,388 | B2 | 7/2013  | Nguyen et al.     |
|           |    |         |                  | 8,509,896 | B2 | 8/2013  | Doerr et al.      |
|           |    |         |                  | 8,527,051 | B1 | 9/2013  | Hedberg et al.    |
|           |    |         |                  | 8,583,230 | B2 | 11/2013 | Ryu et al.        |

(56)

## References Cited

## U.S. PATENT DOCUMENTS

8,615,298 B2	12/2013	Ghosh et al.	2008/0269823 A1	10/2008	Burnes et al.
8,617,082 B2	12/2013	Zhang et al.	2008/0281195 A1	11/2008	Heimdal
8,620,433 B2	12/2013	Ghosh et al.	2008/0306567 A1	12/2008	Park et al.
8,639,333 B2	1/2014	Stadler et al.	2008/0306568 A1	12/2008	Ding et al.
8,694,099 B2	4/2014	Ghosh et al.	2009/0005832 A1	1/2009	Zhu et al.
8,738,132 B1	5/2014	Ghosh et al.	2009/0036947 A1	2/2009	Westlund et al.
8,744,576 B2	6/2014	Munsterman et al.	2009/0043352 A1	2/2009	Brooke et al.
8,768,465 B2	7/2014	Ghosh et al.	2009/0048528 A1	2/2009	Hopenfeld et al.
8,805,504 B2	8/2014	Sweeney	2009/0053102 A2	2/2009	Rudy et al.
8,972,228 B2	3/2015	Ghosh et al.	2009/0054941 A1	2/2009	Eggen et al.
9,037,238 B2	5/2015	Stadler et al.	2009/0054946 A1	2/2009	Sommer et al.
9,155,897 B2	10/2015	Ghosh et al.	2009/0084382 A1	4/2009	Jalde et al.
9,199,087 B2	12/2015	Stadler et al.	2009/0093857 A1	4/2009	Markowitz et al.
9,265,951 B2	2/2016	Sweeney	2009/0099468 A1	4/2009	Thiagalingam et al.
9,265,954 B2	2/2016	Ghosh	2009/0099469 A1	4/2009	Flores
9,265,955 B2	2/2016	Ghosh	2009/0099619 A1	4/2009	Lessmeier et al.
9,278,219 B2	3/2016	Ghosh	2009/0112109 A1	4/2009	Kuklik et al.
9,278,220 B2	3/2016	Ghosh	2009/0143838 A1	6/2009	Libbus et al.
9,282,907 B2	3/2016	Ghosh	2009/0157134 A1	6/2009	Ziglio et al.
9,320,446 B2	4/2016	Gillberg et al.	2009/0157136 A1	6/2009	Yang et al.
9,474,457 B2	10/2016	Ghosh et al.	2009/0198298 A1	8/2009	Kaiser et al.
9,486,151 B2	11/2016	Ghosh et al.	2009/0216112 A1	8/2009	Assis et al.
9,510,763 B2	12/2016	Gosh et al.	2009/0232448 A1	9/2009	Barmash et al.
9,586,050 B2	3/2017	Ghosh et al.	2009/0234414 A1	9/2009	Sambelashvili et al.
9,586,052 B2	3/2017	Gillberg et al.	2009/0254140 A1	10/2009	Rosenberg et al.
9,591,982 B2	3/2017	Ghosh et al.	2009/0270729 A1	10/2009	Corbucci et al.
9,764,143 B2	9/2017	Ghosh et al.	2009/0270937 A1	10/2009	Yonce et al.
9,776,009 B2	10/2017	Ghosh et al.	2009/0299201 A1	12/2009	Gunderson
9,877,789 B2	1/2018	Ghosh et al.	2009/0299423 A1	12/2009	Min
9,924,884 B2	3/2018	Ghosh et al.	2009/0306732 A1	12/2009	Rosenberg et al.
10,064,567 B2	9/2018	Ghosh et al.	2009/0318995 A1	12/2009	Keel et al.
2002/0072682 A1	6/2002	Hopman et al.	2010/0022873 A1	1/2010	Hunter et al.
2002/0087089 A1	7/2002	Ben-Haim	2010/0049063 A1	2/2010	Dobak, III
2002/0143264 A1	10/2002	Ding et al.	2010/0069987 A1	3/2010	Min et al.
2002/0161307 A1	10/2002	Yu et al.	2010/0087888 A1	4/2010	Maskara
2002/0169484 A1	11/2002	Mathis et al.	2010/0094149 A1	4/2010	Kohut et al.
2003/0018277 A1	1/2003	He	2010/0113954 A1	5/2010	Zhou
2003/0050670 A1	3/2003	Spinelli et al.	2010/0114229 A1	5/2010	Chinchoy
2003/0105495 A1	6/2003	Yu et al.	2010/0121403 A1	5/2010	Schecter et al.
2003/0236466 A1	12/2003	Tarjan et al.	2010/0145405 A1	6/2010	Min et al.
2004/0015081 A1	1/2004	Kramer et al.	2010/0174137 A1	7/2010	Shim
2004/0059237 A1	3/2004	Narayan et al.	2010/0198292 A1	8/2010	Honeck et al.
2004/0097806 A1	5/2004	Hunter et al.	2010/0228138 A1	9/2010	Chen
2004/0102812 A1	5/2004	Yonce et al.	2010/0234916 A1	9/2010	Turcott et al.
2004/0122479 A1	6/2004	Spinelli et al.	2010/0249622 A1	9/2010	Olson
2004/0162496 A1	8/2004	Yu et al.	2010/0254583 A1	10/2010	Chan et al.
2004/0172078 A1	9/2004	Chinchoy	2010/0268059 A1	10/2010	Ryu et al.
2004/0172079 A1	9/2004	Chinchoy	2011/0004111 A1	1/2011	Gill et al.
2004/0193223 A1	9/2004	Kramer et al.	2011/0004264 A1	1/2011	Siejko et al.
2004/0215245 A1	10/2004	Stahmann et al.	2011/0022112 A1	1/2011	Min
2004/0215252 A1	10/2004	Verbeek et al.	2011/0054286 A1	3/2011	Crosby
2004/0220635 A1	11/2004	Burnes	2011/0054559 A1	3/2011	Rosenberg et al.
2004/0267321 A1	12/2004	Boileau et al.	2011/0054560 A1	3/2011	Rosenberg et al.
2005/0008210 A1	1/2005	Evron et al.	2011/0075896 A1	3/2011	Matsumoto
2005/0027320 A1	2/2005	Nehls et al.	2011/0092809 A1	4/2011	Nguyen et al.
2005/0090870 A1	4/2005	Hine et al.	2011/0112398 A1	5/2011	Zarkh et al.
2005/0096522 A1	5/2005	Reddy et al.	2011/0118803 A1	5/2011	Hou et al.
2005/0107839 A1	5/2005	Sanders	2011/0137369 A1	6/2011	Ryu et al.
2005/0149138 A1	7/2005	Min et al.	2011/0144510 A1	6/2011	Ryu et al.
2006/0074285 A1	4/2006	Zarkh et al.	2011/0172728 A1	7/2011	Wang
2006/0224198 A1	10/2006	Dong et al.	2011/0190615 A1	8/2011	Phillips et al.
2006/0235478 A1	10/2006	Van Gelder et al.	2011/0201915 A1	8/2011	Gogin et al.
2006/0253162 A1	11/2006	Zhang et al.	2011/0213260 A1	9/2011	Keel et al.
2007/0142871 A1	6/2007	Libbus et al.	2011/0319954 A1	12/2011	Niazi et al.
2007/0167809 A1	7/2007	Dala-Krishna	2012/0004567 A1	1/2012	Eberle et al.
2007/0232943 A1	10/2007	Harel et al.	2012/0101543 A1	4/2012	Demmer et al.
2007/0250129 A1	10/2007	Van Oort	2012/0101546 A1	4/2012	Stadler et al.
2007/0265508 A1	11/2007	Sheikhzadeh-Nadjar et al.	2012/0203090 A1	8/2012	Min
2008/0021336 A1	1/2008	Dobak et al.	2012/0253419 A1	10/2012	Rosenberg et al.
2008/0058656 A1	3/2008	Costello et al.	2012/0283587 A1	11/2012	Ghosh et al.
2008/0119903 A1	5/2008	Arcot-Krishnamurthy et al.	2012/0284003 A1	11/2012	Ghosh et al.
2008/0140143 A1	6/2008	Ettori et al.	2012/0296387 A1	11/2012	Zhang et al.
2008/0146954 A1	6/2008	Bojovic et al.	2012/0296388 A1	11/2012	Zhang et al.
2008/0242976 A1	10/2008	Robertson et al.	2012/0302904 A1	11/2012	Lian et al.
2008/0269818 A1	10/2008	Sullivan et al.	2012/0303084 A1	11/2012	Kleckner et al.
			2012/0310297 A1	12/2012	Sweeney
			2012/0330179 A1	12/2012	Yuk et al.
			2013/0006332 A1	1/2013	Sommer et al.
			2013/0018250 A1	1/2013	Caprio et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

2013/0018251	A1	1/2013	Caprio et al.
2013/0030491	A1	1/2013	Stadler et al.
2013/0060298	A1	3/2013	Splett et al.
2013/0072790	A1	3/2013	Ludwig et al.
2013/0096446	A1	4/2013	Michael et al.
2013/0116739	A1	5/2013	Brada et al.
2013/0131529	A1	5/2013	Jia et al.
2013/0131749	A1	5/2013	Sheldon et al.
2013/0131751	A1	5/2013	Stadler et al.
2013/0136035	A1	5/2013	Bange et al.
2013/0150913	A1	6/2013	Bornzin et al.
2013/0165983	A1	6/2013	Ghosh et al.
2013/0165988	A1	6/2013	Ghosh
2013/0261471	A1	10/2013	Saha et al.
2013/0261688	A1	10/2013	Dong et al.
2013/0289640	A1	10/2013	Zhang et al.
2013/0296726	A1	11/2013	Niebauer et al.
2013/0304407	A1	11/2013	George et al.
2013/0324828	A1	12/2013	Nishiwaki et al.
2014/0005563	A1	1/2014	Ramanathan et al.
2014/0018872	A1	1/2014	Siejko et al.
2014/0135866	A1	5/2014	Ramanathan et al.
2014/0135867	A1	5/2014	Demmer et al.
2014/0163633	A1	6/2014	Ghosh et al.
2014/0222099	A1	8/2014	Sweeney
2014/0236252	A1	8/2014	Ghosh et al.
2014/0276125	A1	9/2014	Hou et al.
2014/0277233	A1	9/2014	Ghosh
2014/0323882	A1	10/2014	Ghosh et al.
2014/0323892	A1	10/2014	Ghosh et al.
2014/0323893	A1	10/2014	Ghosh et al.
2014/0371807	A1	12/2014	Ghosh et al.
2014/0371808	A1	12/2014	Ghosh et al.
2014/0371832	A1	12/2014	Ghosh et al.
2014/0371833	A1	12/2014	Ghosh et al.
2015/0032016	A1	1/2015	Ghosh
2015/0032171	A1	1/2015	Ghosh
2015/0032172	A1	1/2015	Ghosh
2015/0032173	A1	1/2015	Ghosh
2015/0045849	A1	2/2015	Ghosh et al.
2015/0142069	A1	5/2015	Sambelashvili
2015/0157225	A1	6/2015	Gillberg et al.
2015/0157231	A1	6/2015	Gillberg et al.
2015/0157232	A1	6/2015	Gillberg et al.
2015/0157865	A1	6/2015	Gillberg et al.
2015/0216434	A1	8/2015	Ghosh et al.
2015/0265840	A1*	9/2015	Ghosh ..... A61N 1/3702 607/27
2016/0030747	A1	2/2016	Thakur et al.
2016/0030751	A1	2/2016	Ghosh et al.
2016/0045737	A1	2/2016	Ghosh et al.
2016/0045738	A1	2/2016	Ghosh et al.
2016/0045744	A1	2/2016	Gillberg et al.
2016/0184590	A1	6/2016	Ghosh
2017/0246460	A1	8/2017	Ghosh
2017/0246461	A1	8/2017	Ghosh

## FOREIGN PATENT DOCUMENTS

CN	1878595	A	12/2006
CN	101073502	A	11/2007
EP	1 072 284	A2	1/2001
EP	1 504 713	A1	2/2005
EP	2 016 976	A1	1/2009
EP	2 391 270	A1	7/2011
EP	1 925 337	B1	3/2012
EP	2 436 309	A2	4/2012
EP	2 435 132	B1	8/2013
WO	WO 1998/026712	A1	6/1998
WO	WO 1999/006112	A1	2/1999
WO	WO 2000/045700	A1	8/2000
WO	WO 2001/067950	A1	9/2001
WO	WO 2003/070323	A1	8/2003
WO	WO 2005/056108	A2	6/2005

WO	WO 2006/069215	A2	6/2006
WO	WO 2006/069215	A3	6/2006
WO	WO 2006/105474	A2	10/2006
WO	WO 2006/115777	A1	11/2006
WO	WO 2006/117773	A1	11/2006
WO	WO 2007/013994	A2	2/2007
WO	WO 2007/027940	A2	3/2007
WO	WO 2007/013994	A3	4/2007
WO	WO 2007/027940	A3	6/2007
WO	WO 2007/139456	A1	12/2007
WO	WO 2008/151077	A2	12/2008
WO	WO 2009/079344	A1	6/2009
WO	WO 2009/139911	A2	11/2009
WO	WO 2009/148429	A1	12/2009
WO	WO 2010/019494	A1	2/2010
WO	WO 2010/071520	A1	6/2010
WO	WO 2010/088040	A1	8/2010
WO	WO 2010/088485	A1	8/2010
WO	WO 2011/070166	A1	6/2011
WO	WO 2011/090622	A1	7/2011
WO	WO 2011/099992	A1	8/2011
WO	WO 2012/037471	A2	3/2012
WO	WO 2012/037471	A3	6/2012
WO	WO 2012/106297	A2	8/2012
WO	WO 2012/106297	A3	8/2012
WO	WO 2012/109618	A2	8/2012
WO	WO 2012/110940	A1	8/2012
WO	WO 2012/109618	A3	11/2012
WO	WO 2012/151364	A1	11/2012
WO	WO 2012/151389	A1	11/2012
WO	WO 2013/006724	A2	1/2013
WO	WO 2013/010165	A1	1/2013
WO	WO 2013/010184	A1	1/2013
WO	WO 2013/006724	A3	4/2013
WO	WO 2014/179454	A1	11/2014
WO	WO 2014/179459	A2	11/2014
WO	WO 2014/179459	A3	1/2015
WO	WO 2015/013271	A1	1/2015
WO	WO 2015/013493	A1	1/2015
WO	WO 2015/013574	A1	1/2015

## OTHER PUBLICATIONS

International Search Report and Written Opinion dated May 3, 2012 for International Application No. PCT/US2012/036302; 9 pages.

International Search Report and Written Opinion dated Aug. 6, 2014 for International Application No. PCT/US2014/036153; 14 pages.

International Search Report and Written Opinion dated Nov. 7, 2014 for International Application No. PCT/US2014/036163; 12 pages.

International Search Report and Written Opinion dated Oct. 28, 2014 for International Application No. PCT/US2014/041928; 15 pages.

International Search Report and Written Opinion dated Oct. 24, 2014 for International Application No. PCT/US2014/041929; 14 pages.

International Search Report and Written Opinion dated Nov. 4, 2014 for International Application No. PCT/US2014/0247583; 7 pages.

International Search Report and Written Opinion dated Nov. 12, 2014 for International Application No. PCT/US2014/047971; 7 pages.

International Search Report and Written Opinion dated Nov. 12, 2014 for International Application No. PCT/US2014/048120; 7 pages.

International Search Report and Written Opinion dated Mar. 9, 2015 for International Application No. PCT/US2014/069214; 11 pages.

International Search Report and Written Opinion dated Mar. 17, 2015, for International Application No. PCT/US2014/069192; 11 pages.

International Search Report and Written Opinion dated Mar. 16, 2015 for International Application No. PCT/US2014/069182; 11 pages.

International Search Report and Written Opinion dated Apr. 8, 2015 for International Application No. PCT/US2014/069070; 11 pages.

International Search Report and Written Opinion dated Jun. 11, 2015 for International Application No. PCT/US2015/021442; 13 pages.

(56)

## References Cited

## OTHER PUBLICATIONS

- Bank, "Changes in electrical heterogeneity of body surface maps: Application for CRT optimization" Poster Presentation. HRS 2016 Annual Meeting. May 4-7; San Francisco, California.
- Bank, "Electrical dyssynchrony and optimization potential with and without Class I Indications for Cardiac Resynchronization Therapy" Cardiosim 2016 World Congress in Cardiac Electrophysiology and Cardiac Techniques. Jun. 8-11. Nice, France. Jun. 2016 Europace 18(suppl\_1):i50-i50.
- Bank, "Electrical heterogeneity varies using different pacing electrodes of left ventricular quadripolar leads" Poster Presentation. HRS 2016 Annual Meeting. May 4-7; San Francisco, California.
- Bank, "Optimization of VV timing in CRT using body surface mapping: Role of LV preactivation" Oral Presentation. HRS 2017 Annual Meeting. May 10-13; Chicago, Illinois.
- Bank, "Use of a novel noninvasive ECG mapping system to identify line of block and optimal CRT seBank-use-10tting" Poster Presentation. Cardiosim 2016 World Congress in Cardiac Electrophysiology and Cardiac Techniques. Jun. 8-11. Nice, France.
- Biffi et al., "Occurrence of Phrenic Nerve Stimulation in Cardiac Resynchronization Therapy Patients: the Role of Left Ventricular Lead Type and Placement Site," *Europace*, 2013; 15:77-82.
- Botker MD, PhD., et al., "Electromechanical Mapping for Detection of Myocardial Viability in Patients with ischemia Cardiomyopathy," *Circulation*, Mar. 2001; vol. 103, No. 12, pp.
- Burns, "Left ventricular-only pacing in heart failure patients with normal atrioventricular conduction improves global function and left ventricular regional mechanics compared with biventricular pacing: an adaptive cardiac resynchronization therapy sub-study" Oct. 2017 *Eur J Heart Fail.*, 19(10):1335-1343.
- "CardioGuide System Enables Real-Time Navigation of Left Ventricular Leads During Medtronic CRT Implants," Press Release, Apr. 9, 2013, Medtronic, Inc., 2 pgs.
- Cuculich, P.S., et al., "The Electrophysiological Cardiac Ventricular Substrate in Patients After Myocardial Infection" *J. Am. Coll. Cardiol.* 2011; 58:1893-1902.
- Curtin, "Description of body surface activation map patterns in patients grouped by 12-lead ECG morphology" HRS 2017 Annual Meeting. May 10-13; Chicago, Illinois.
- Curtin, "Electrical heterogeneity metrics from body surface mapping vs routine ECG measures before and after CRT" Poster Presentation. HRS 2016 Annual Meeting. May 4-7; San Francisco, California.
- Curtin, "Left ventricular orientation and position in an advanced heart failure population" Jun. 2017 *Translational Research in Anatomy*, 7:12-19.
- Curtin, "Use of body surface mapping to assess wavefront fusion in CRT" Poster Presentation. HRS 2016 Annual Meeting. May 4-7; San Francisco, California.
- Czerwinska et al., "Method of Segmentation of Thorax Organs Images Applied to Modeling the Cardiac Electrical Field," *Engineering in Medicine and Biology Society*, Proceedings of the 22<sup>nd</sup> Annual International Conference of the IEEE, vol. 1, 23, Jul. 23, 2000.; pp. 402-405.
- Dawoud, F. et al., "Inverse Electrocardiographic Imaging to Assess Electrical Dyssynchrony in Cardiac Resynchronization Therapy Patients," *Computing in Cardiology*, 2012; 39:993-996.
- Freund et al., "A Decision-Theoretic Generalization of Online Learning and an Application to Boosting," *Journal of Computer and System Sciences*, 1997; 55(1):119-139.
- Friedman, "Greedy Function Approximation: A Gradient Boosting Machine," *Annals of Statistics*, 2001; 29(5):1189-1232.
- Friedman, "Stochastic Gradient Boosting," *Computational Statistics and Data Analysis*, 2002; 38(4):367-378.
- Friedman et al., "Additive Logistic Regression: a Statistical View of Boosting," *Annals of Statistics*, 2000; 28(2):337-374.
- Fung et al., Chapter 20, Optimization of Cardiac Resynchronization Therapy, Cardiac Resynchronization Therapy, Second Edition, Copyright 2008, Blackwell Publishing Ltd., pp. 356-373.
- Gage, "Changes in electrical dyssynchrony by body surface mapping predict LV remodelling in CRT patients" 2016 HeartRhythm, 14(3):392-399.
- Gage, "Changes in electrical heterogeneity of body surface mapping predict LV remodeling in CRT patients" Poster Presentation. HRS 2016 Annual Meeting. May 4-7; San Francisco, California.
- Ghosh et al. "Accuracy of Quadratic Versus Linear Interpolation in Noninvasive Electrocardiographic Imaging (ECGI)," *Annals of Biomedical Engineering*, vol. 33, No. 9. Sep. 2005; pp. 1187-1201.
- Ghosh et al., "Cardiac Memory in Patients with Wolff-Parkinson-White Syndrome: Noninvasive Imaging of Activation and Repolarization Before and After Catheter Ablation" *Circulation*, 2008; 118:907-915. Published online Aug. 12, 2008.
- Ghosh et al. "Application of L1-Norm Regularization to Epicardial Potential Solution of the Inverse Electrocardiography Problem," *Annals of Biomedical Engineering*, vol. 37, No. 5, May 2009; pp. 902-912.
- Ghosh et al., "Electrophysiological Substrate and Intraventricular LV Dyssynchrony in Non-ischemic Heart Failure Patients Undergoing Cardiac Resynchronization Therapy," *Heart rhythm : the official journal of the Heart Rhythm Society*, 2011; 8(5):692-699.
- Gold et al., "Comparison of Stimulation Sites within Left Ventricular Veins on the Acute Hemodynamic Effects of Cardiac Resynchronization Therapy" *Heart Rhythm*, Apr. 2005; 2(4):376-381.
- Gulrajani, "The Forward and Inverse Problems of Electrocardiography," *IEEE Engineering in Medicine and Biology*, IEEE Service Center, vol. 17, No. 5, Sep. 1, 1988; pp. 84-101, 122.
- Hansen, "Regularization Tools: A Matlab Package for Analysis and Solution of Discrete Ill-Posed Problems," Version 4.1 for Matlab 7.3; Mar. 2008; 128 pages. Retrieved from the Internet: Jun. 19, 2014 <http://www.mathworks.com/matlabcentral/fileexchange/52-regtools>.
- Hayes et al., "Cardiac Resynchronization Therapy and the Relationship of Percent Biventricular Pacing to Symptoms and Survival," *Heart Rhythm*, Sep. 2011; 8(9):1469-1475.
- "Heart Failure Management" datasheet [online]. Medtronic, Minneapolis, Minnesota, [Last updated on Jun. 3, 2013]. Retrieved from the Internet: [www.medtronic.com](http://www.medtronic.com); 9 pages.
- Hopenfeld et al., "The Effect of Conductivity on ST-Segment Epicardial Potentials Arising from Subendocardial Ischemia," *Annals of Biomedical Eng.*, Jun. 2005; vol. 33, No. 6, pp. 751-763.
- Jia et al., "Electrocardiographic Imaging of Cardiac Resynchronization Therapy in Heart Failure: Observation of Variable Electrophysiologic Responses," *Heart Rhythm*, vol. 3, No. 3; Mar. 1, 2006, pp. 296-310.
- Johnson, "Body surface mapping using an ECG belt to characterize electrical heterogeneity for different left ventricular pacing sites during cardiac resynchronization: Relationship with acute hemodynamic improvement" Mar. 2017 *Heart Rhythm*, 14(3):385-391.
- Kornreich, "Body Surface Potential Mapping of ST Segment Changes in Acute Myocardial Infarction," *Circulation*, 1993; 87: 773-782.
- Lumason™, Brochure, Bracco Diagnostics. Oct. 2014.
- Medtronic Vitatron CARELINK ENCORE® Programmer Model 29901 Reference Manual, 2013, Medtronic, Inc., Minneapolis, MN.
- Miri et al., "Applicability of body surface potential map in computerized optimization of biventricular pacing," *Annals of Biomedical Engineering*, vol. 38, No. 3, Mar. 2010, pp. 865-875.
- Miri et al., "Comparison of the electrophysiologically based optimization methods with different pacing parameters in patient undergoing resynchronization treatment," 30th Annual International IEEE EMBS Conference, Aug. 2008, pp. 1741-1744.
- Miri et al., "Computerized Optimization of Biventricular Pacing Using Body Surface Potential Map," 31st Annual International Conference of the IEEE EMBS, Sep. 2009, pp. 2815-2818.
- Miri et al., "Efficiency of Timing Delays and Electrode Positions in Optimization of Biventricular Pacing: A Simulation Study," *IEEE Transactions on Biomedical Engineering*, Nov. 2009, pp. 2573-2582.
- Modre et al., "Noninvasive Myocardial Activation Time Imaging: A Novel Inverse Algorithm Applied to Clinical ECG Mapping Data" *IEEE Transactions on Biomedical Engineering*, vol. 49; No. 10, Oct. 2002; pp. 1153-1161.

(56)

**References Cited**

## OTHER PUBLICATIONS

- Nash et al., "An Experimental-Computational Framework for Validating in-vivo ECG Inverse Algorithms," *International Journal of Bioelectromagnetism*, vol. 2, No. 2, Dec. 31, 2000, 9 pp.
- Potse et al., "Mathematical Modeling and Simulation of Ventricular Activation Sequences: Implications for Cardiac Resynchronization Therapy," *J. of Cardiovasc. Trans. Res.*, 2012; 5:146-158.
- Prinzen et al., "Cardiac Resynchronization Therapy State-of-the-Art of Current Applications, Guidelines, Ongoing Trials, and Areas of Controversy" *Circulation*, 2013; 128: 2407-2418.
- Ridgeway, "The State of Boosting," *Computing Science and Statistics*, 1999; 31:172-181.
- Ryu et al., "Simultaneous Electrical and Mechanical Mapping Using 3D Cardiac Mapping System: Novel Approach for Optimal Cardiac Resynchronization Therapy," *Journal of Cardiovascular Electrophysiology*, Feb. 2010; 21(2):219-22.
- Silva et al., "Cardiac Resynchronization Therapy in Pediatric Congenital Heart Disease: Insights from Noninvasive Electrocardiographic Imaging" *Heart Rhythm*, vol. 6, No. 8. Aug. 1, 2009; pp. 1178-1185.
- Singh et al., "Left Ventricular Lead Position and Clinical Outcome in the Multicenter Automatic Defibrillator Implantation Trial-Cardiac Resynchronization Therapy (MADIT-CRT) Trial," *Circulation*, 2011; 123:1159-1166.
- Sperzel et al., "Intraoperative Characterization of Interventricular Mechanical Dyssynchrony Using Electroanatomic Mapping System—A Feasibility Study," *Journal of Interventional Cardiac Electrophysiology*, Nov. 2012; 35(2):189-96.
- Steinhaus BM., "Estimating cardiac transmembrane activation and recovery times from unipolar and bipolar extracellular electrograms: a simulation study," *Circulation Research*, 1989, 64:449-462.
- Strik et al., "Electrical and Mechanical Ventricular Activation During Left Bundle Branch Block and Resynchronization," *J. of Cardiovasc. Trans. Res.*, 2012; 5:117-126.
- Svendsen et al., "Computational Models of Cardiac Electrical Activation," Chapter 5, Computational Nov. 2010, pp. 73-88.
- Sweeney et al., "Analysis of Ventricular Activation Using Surface Electrocardiography to Predict Left Ventricular Reverse Volumetric Remodeling During Cardiac Resynchronization Therapy," *Circulation*, Feb. 9, 2010; 121(5):626-34. Available online Jan. 25, 2010.
- Sweeney et al., QRS Fusion Complex Analysis Using Wave Interference to Predict Reverse Remodeling During Cardiac Resynchronization Therapy, *Heart Rhythm*, 2014, 11:806-813.
- Turner et al., "Electrical and Mechanical Components of Dyssynchrony in Heart Failure Patients with Normal QRS Duration and Left Bundle-Branch Block," *Circulation* 2004; 109: 2544-2549.
- Van Deursen et al., "Vectorcardiography as a Tool for Easy Optimization of Cardiac Resynchronization Therapy in Canine LBBB Hearts," *Circulation Arrhythmia and Electrophysiology*, Jun. 1, 2012; 5(3):544-52. Available online Apr. 24, 2012.
- Vardas et al., The Task Force for Cardiac Pacing and Cardiac Resynchronization Therapy of the European Society of Cardiology. Developed in Collaboration with the European Heart Rhythm Association, *European Heart Journal*, 2007; 28:2256-2295.
- Varma et al., "Placebo CRT," *Journal of Cardiovascular Electrophysiology*, vol. 19, Aug. 2008; p. 878.
- Wang et al., "Application of the Method of Fundamental Solutions to Potential-based Inverse Electrocardiography," *Annals of Biomedical Engineering*, Aug. 2006, pp. 1272-1288.
- Wellens, MD et al., "The Electrocardiogram 102 Years After Einthoven," *Circulation*, Feb. 2004; vol. 109, No. 5, pp. 562-564.
- Williams et al., "Short-Term Hemodynamic Effects of Cardiac Resynchronization Therapy in Patients With Heart Failure, a Narrow QRS Duration, and No Dyssynchrony," *Circulation*, Oct. 27, 2009; 120: 1687-1694.

\* cited by examiner

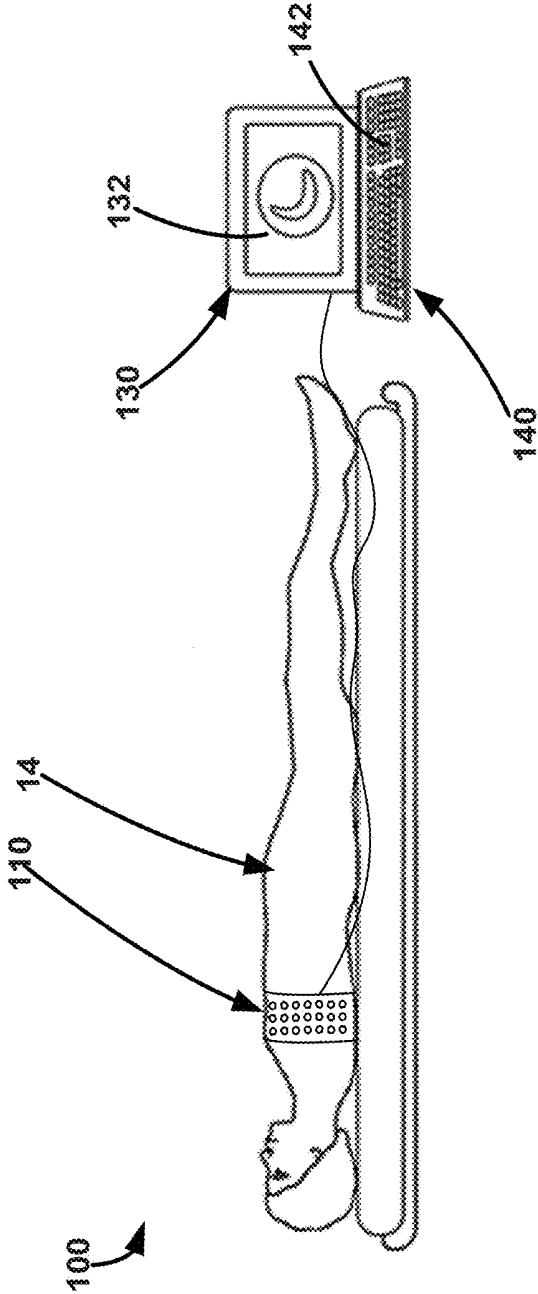


FIG. 1

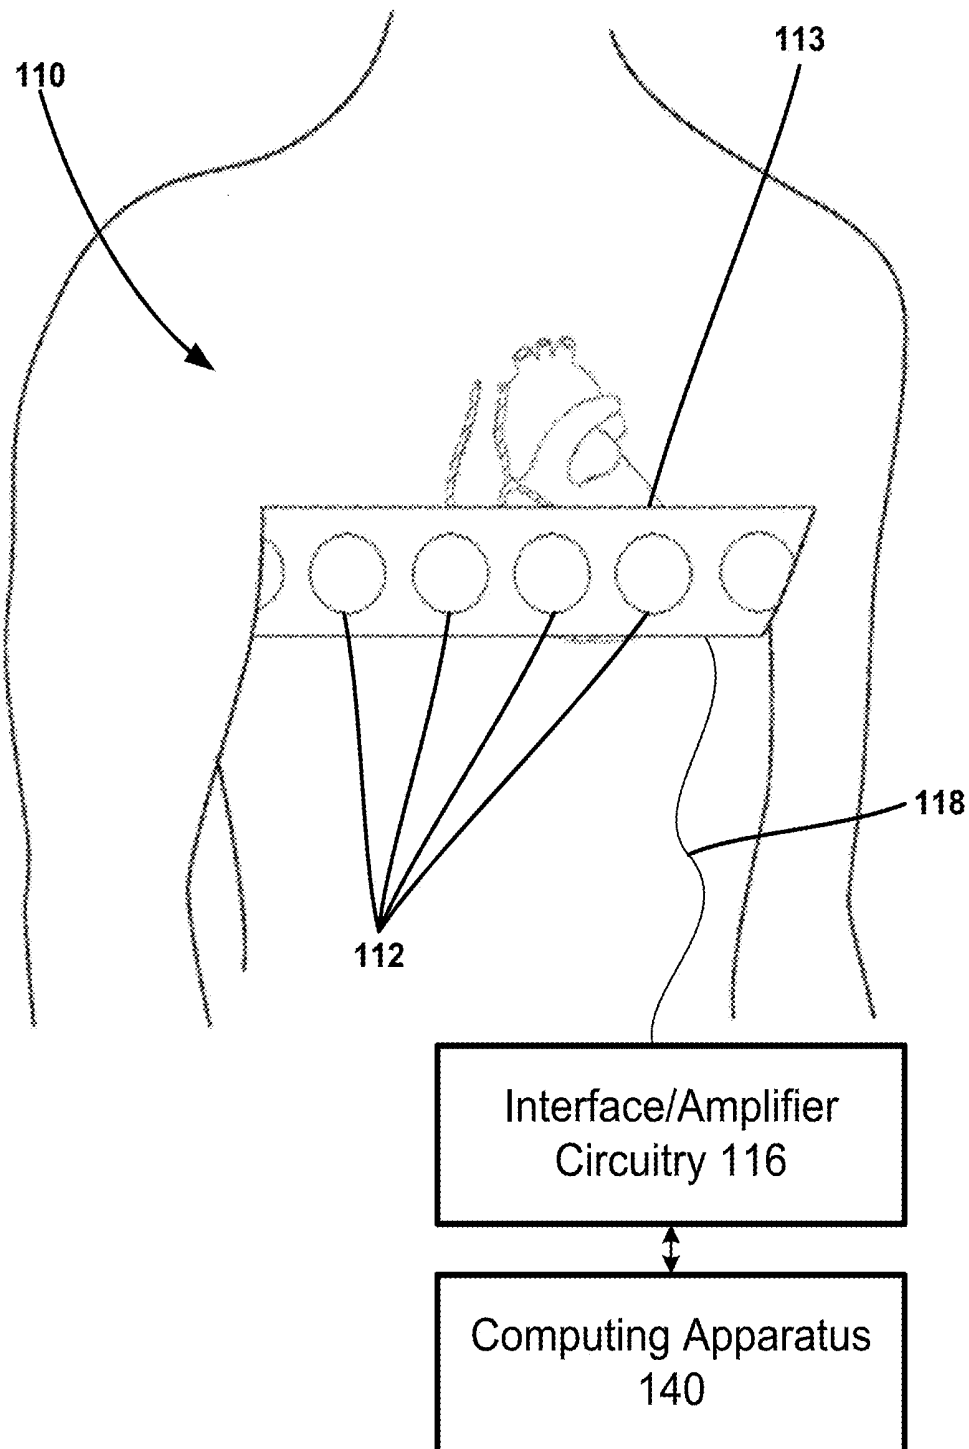
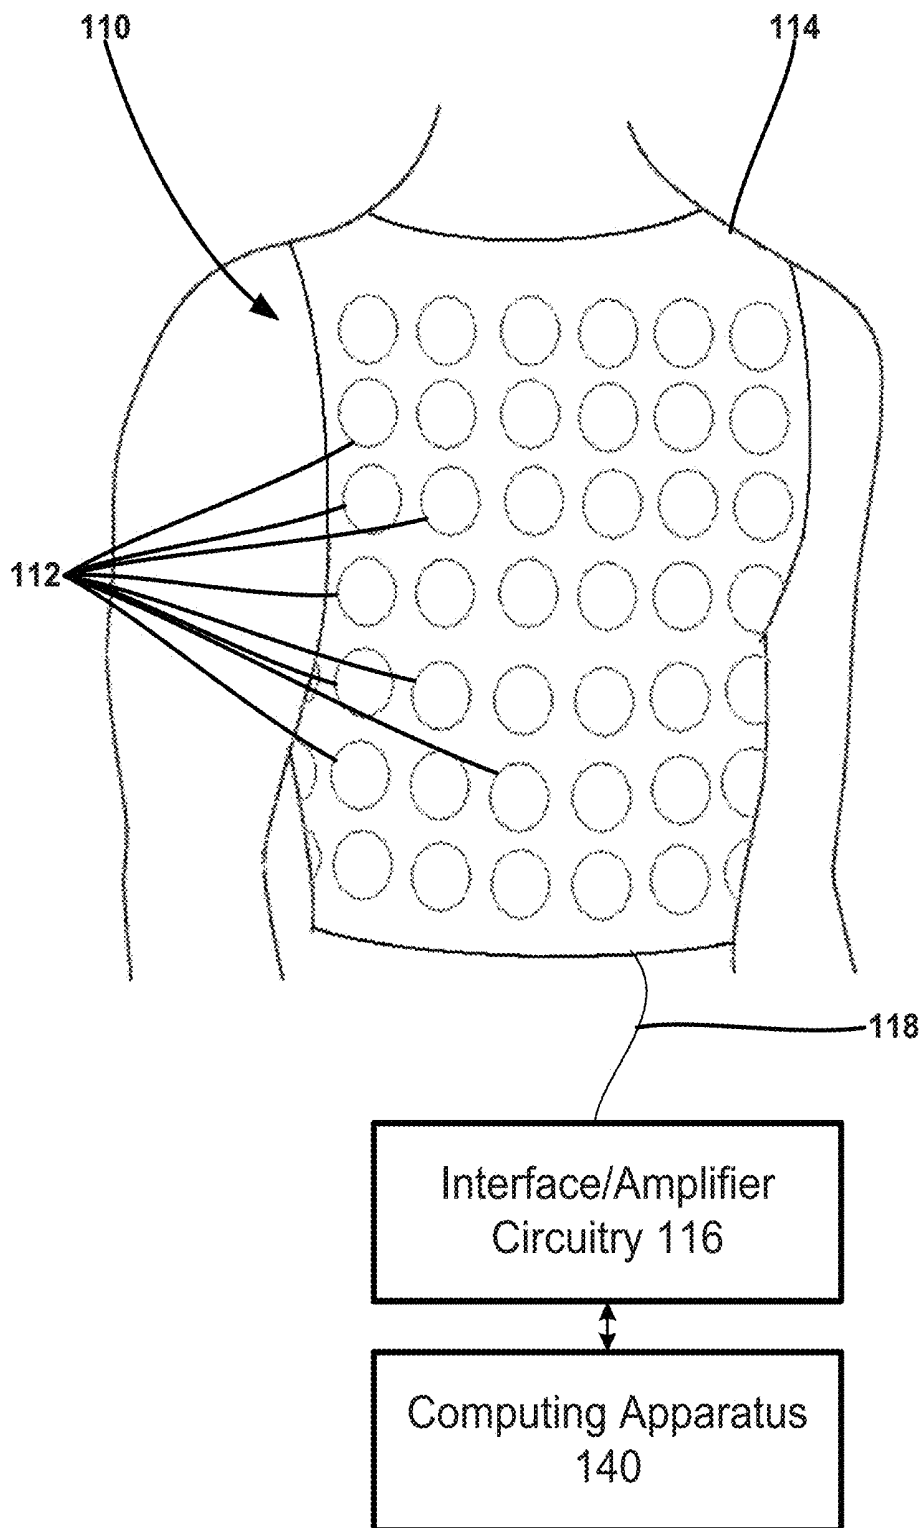


FIG. 2



**FIG. 3**

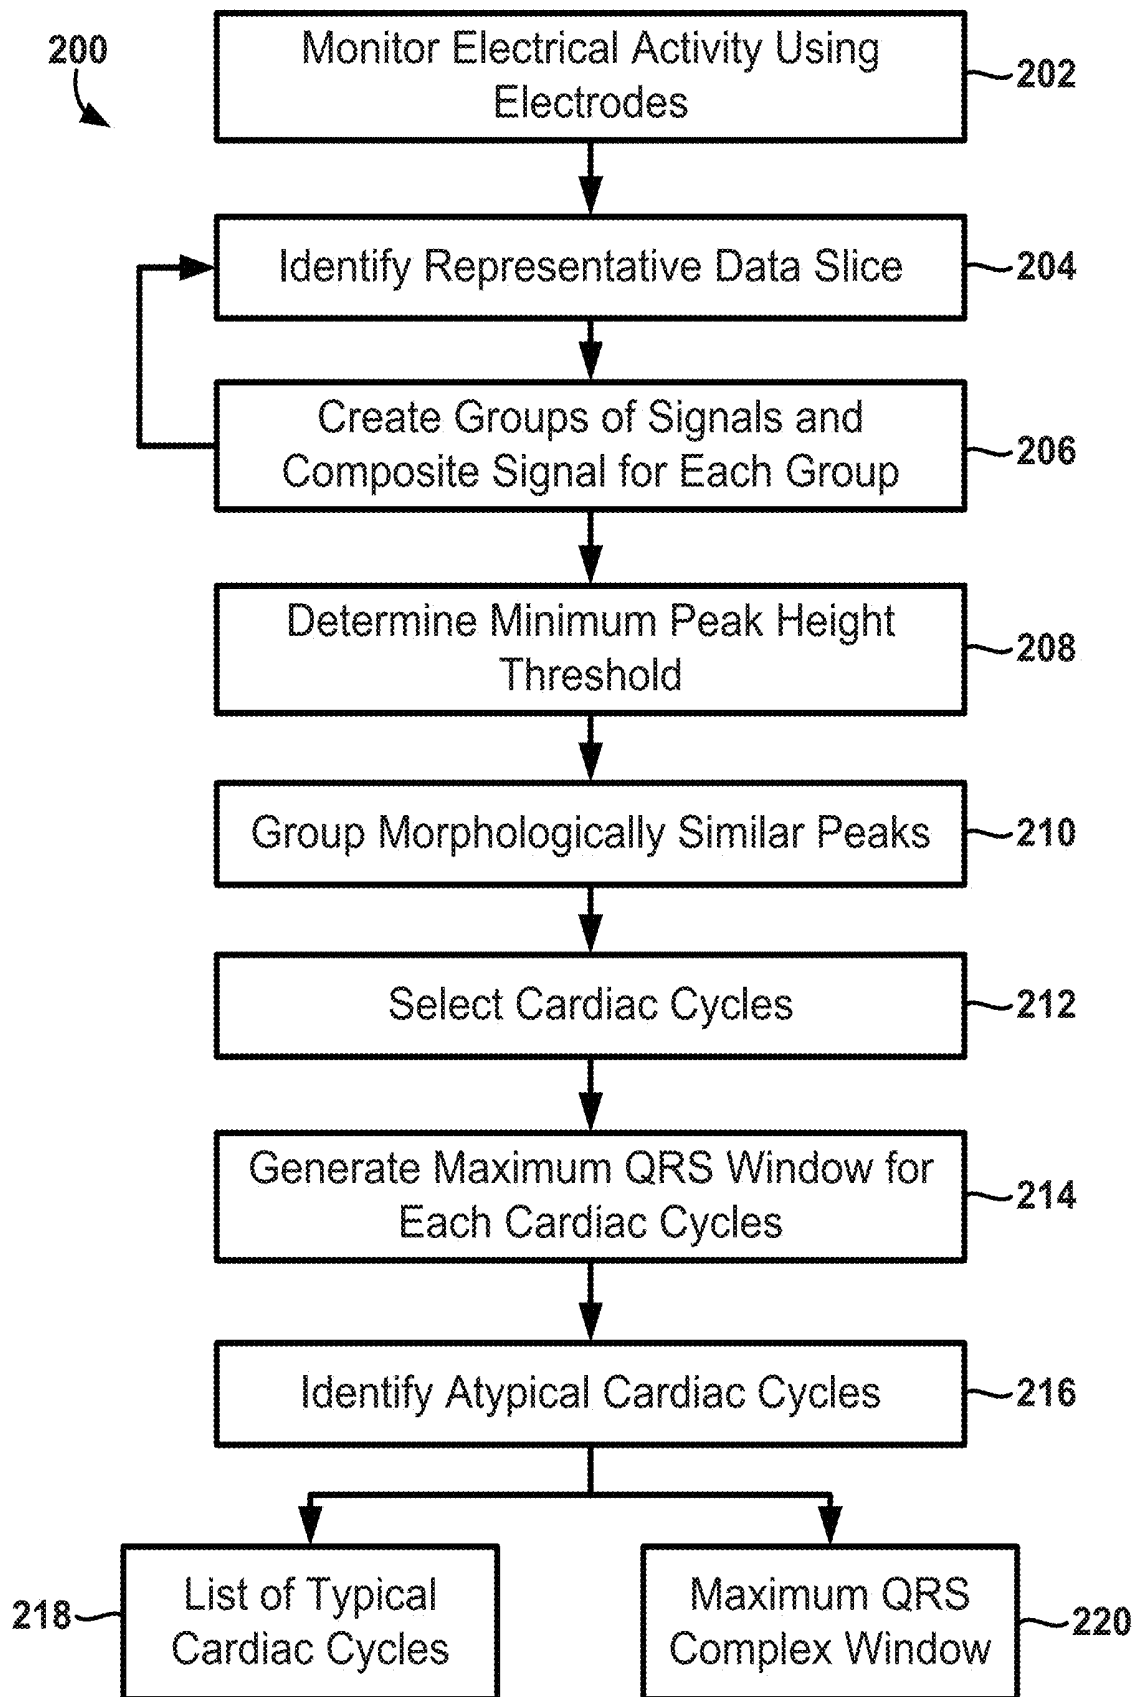


FIG. 4A

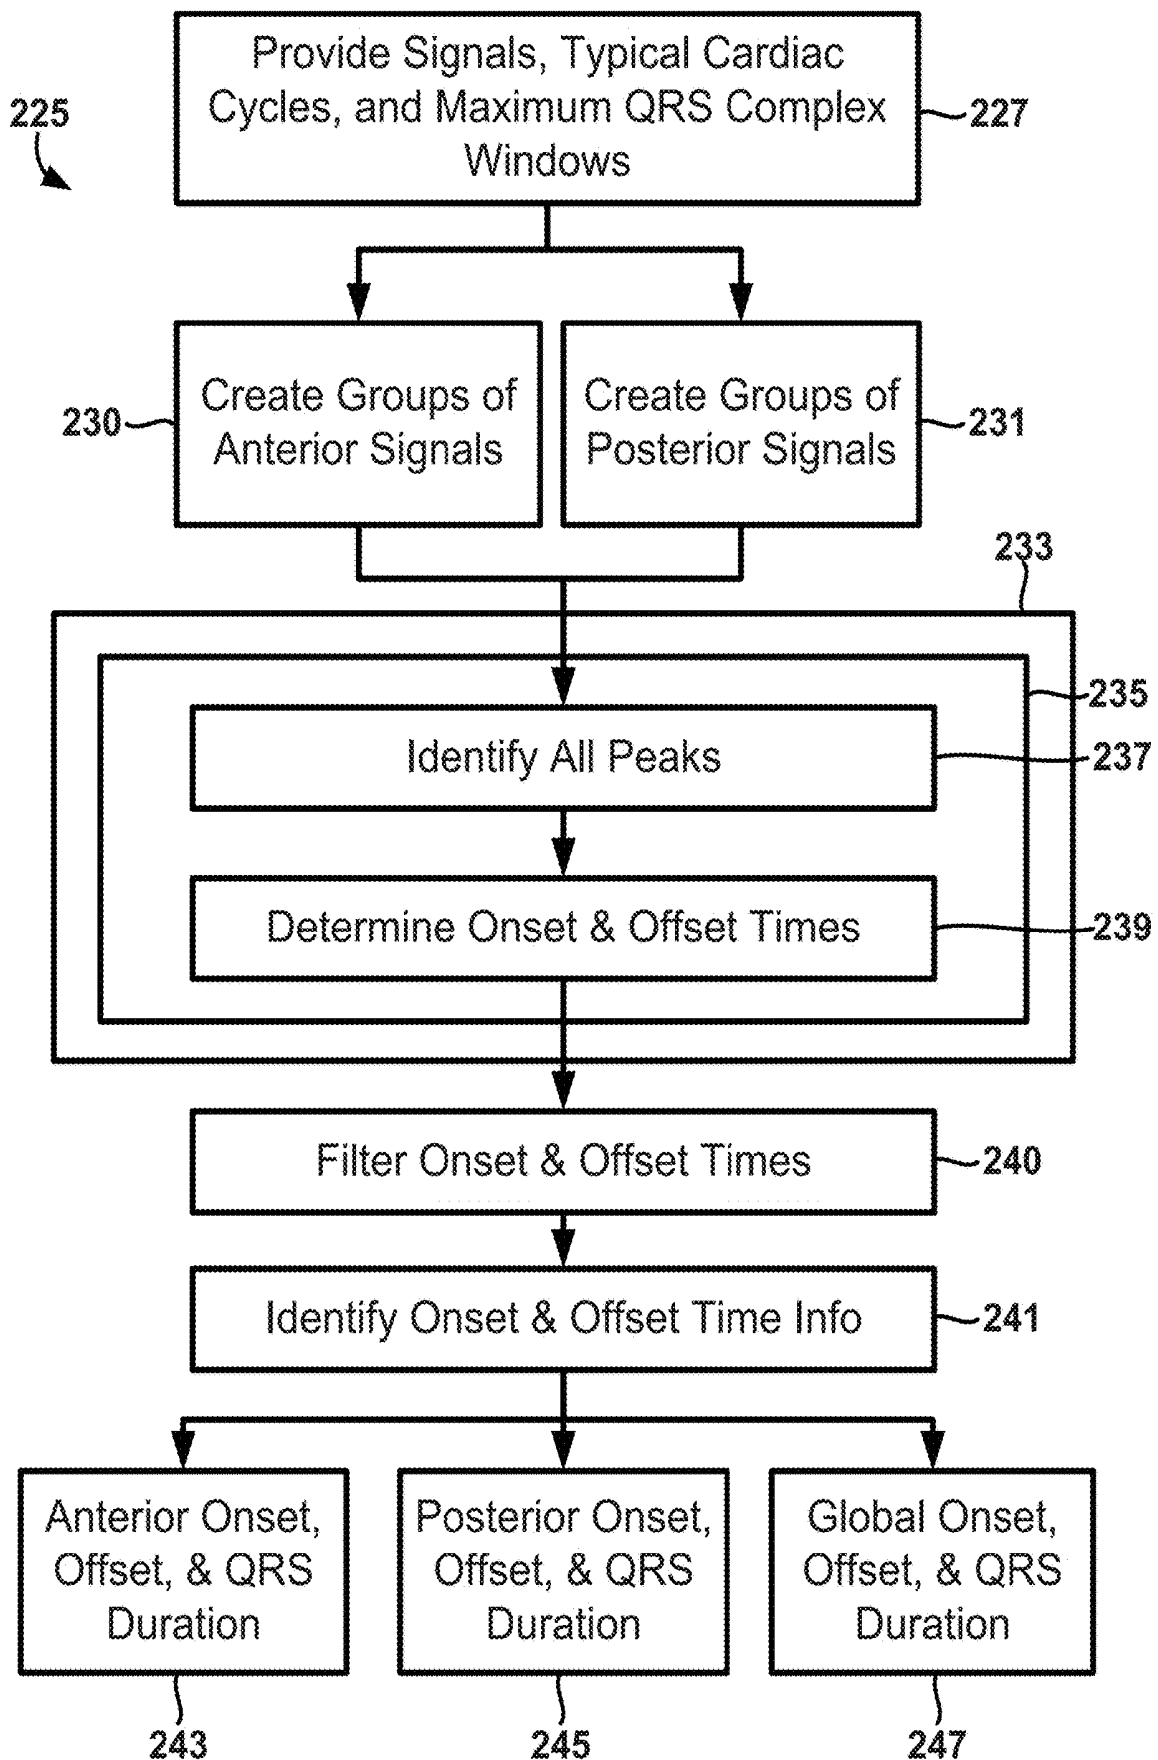


FIG. 4B

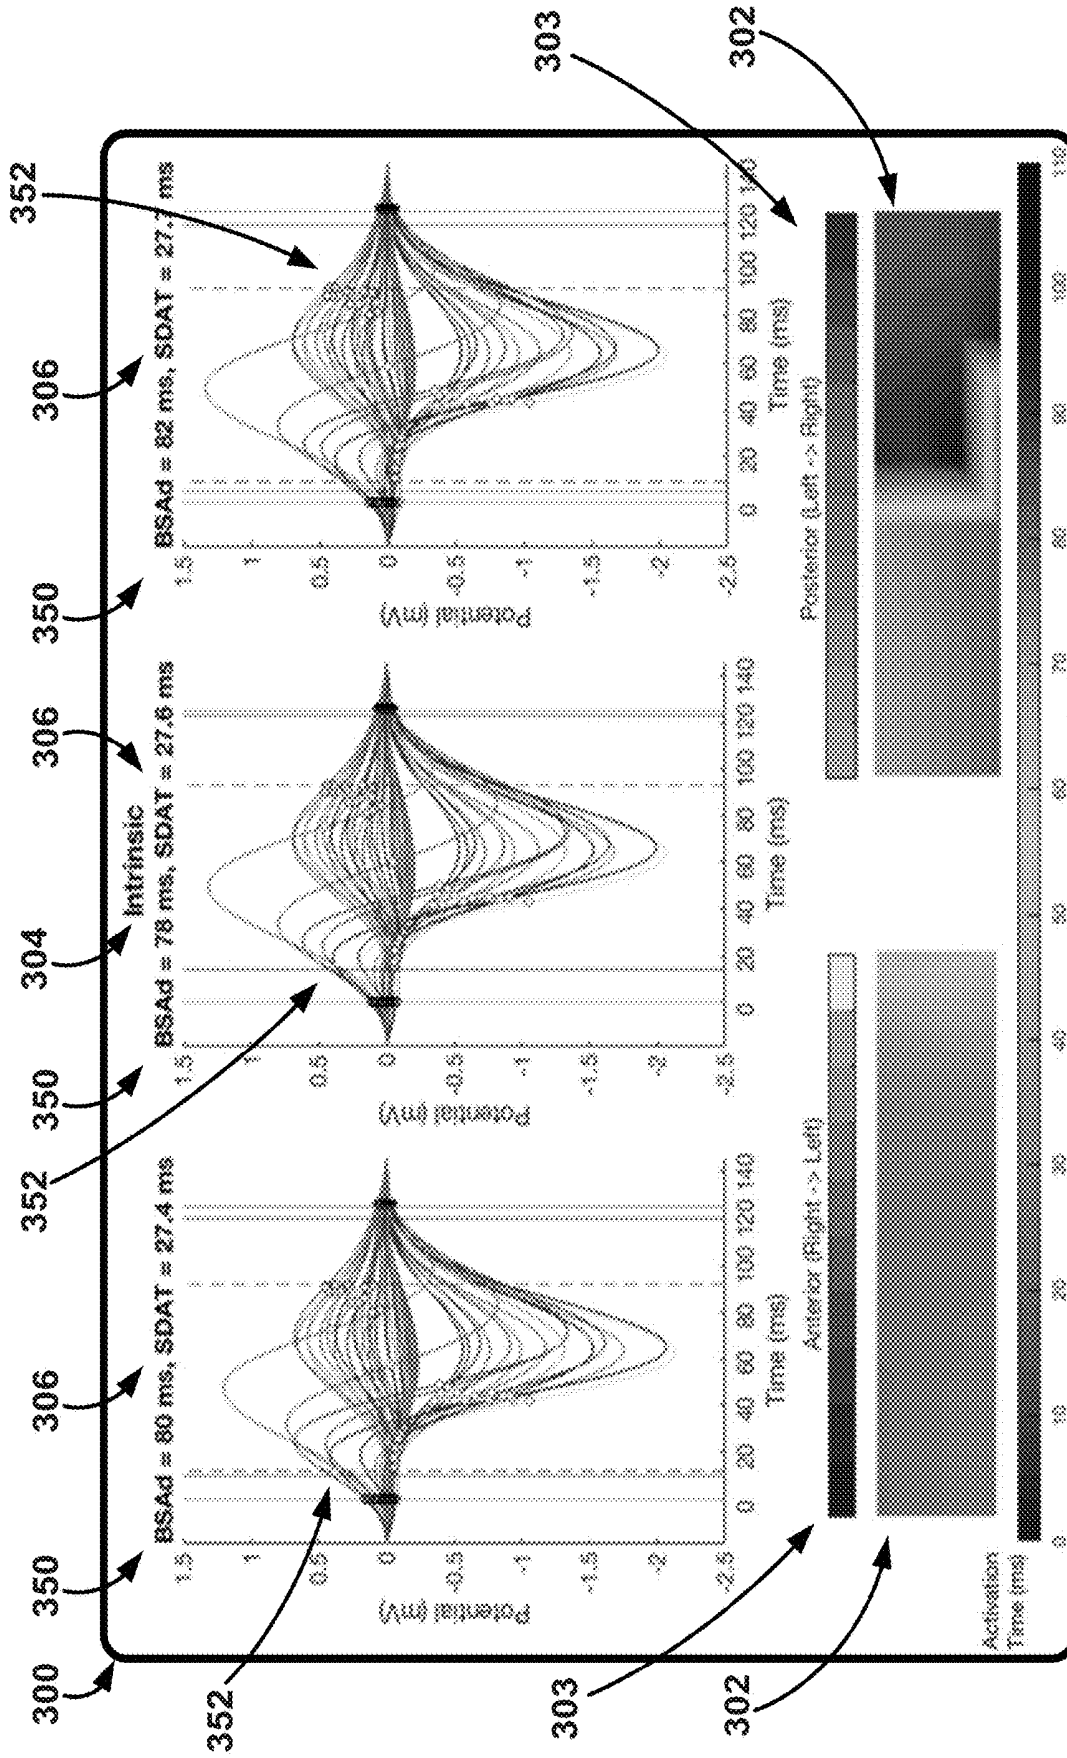
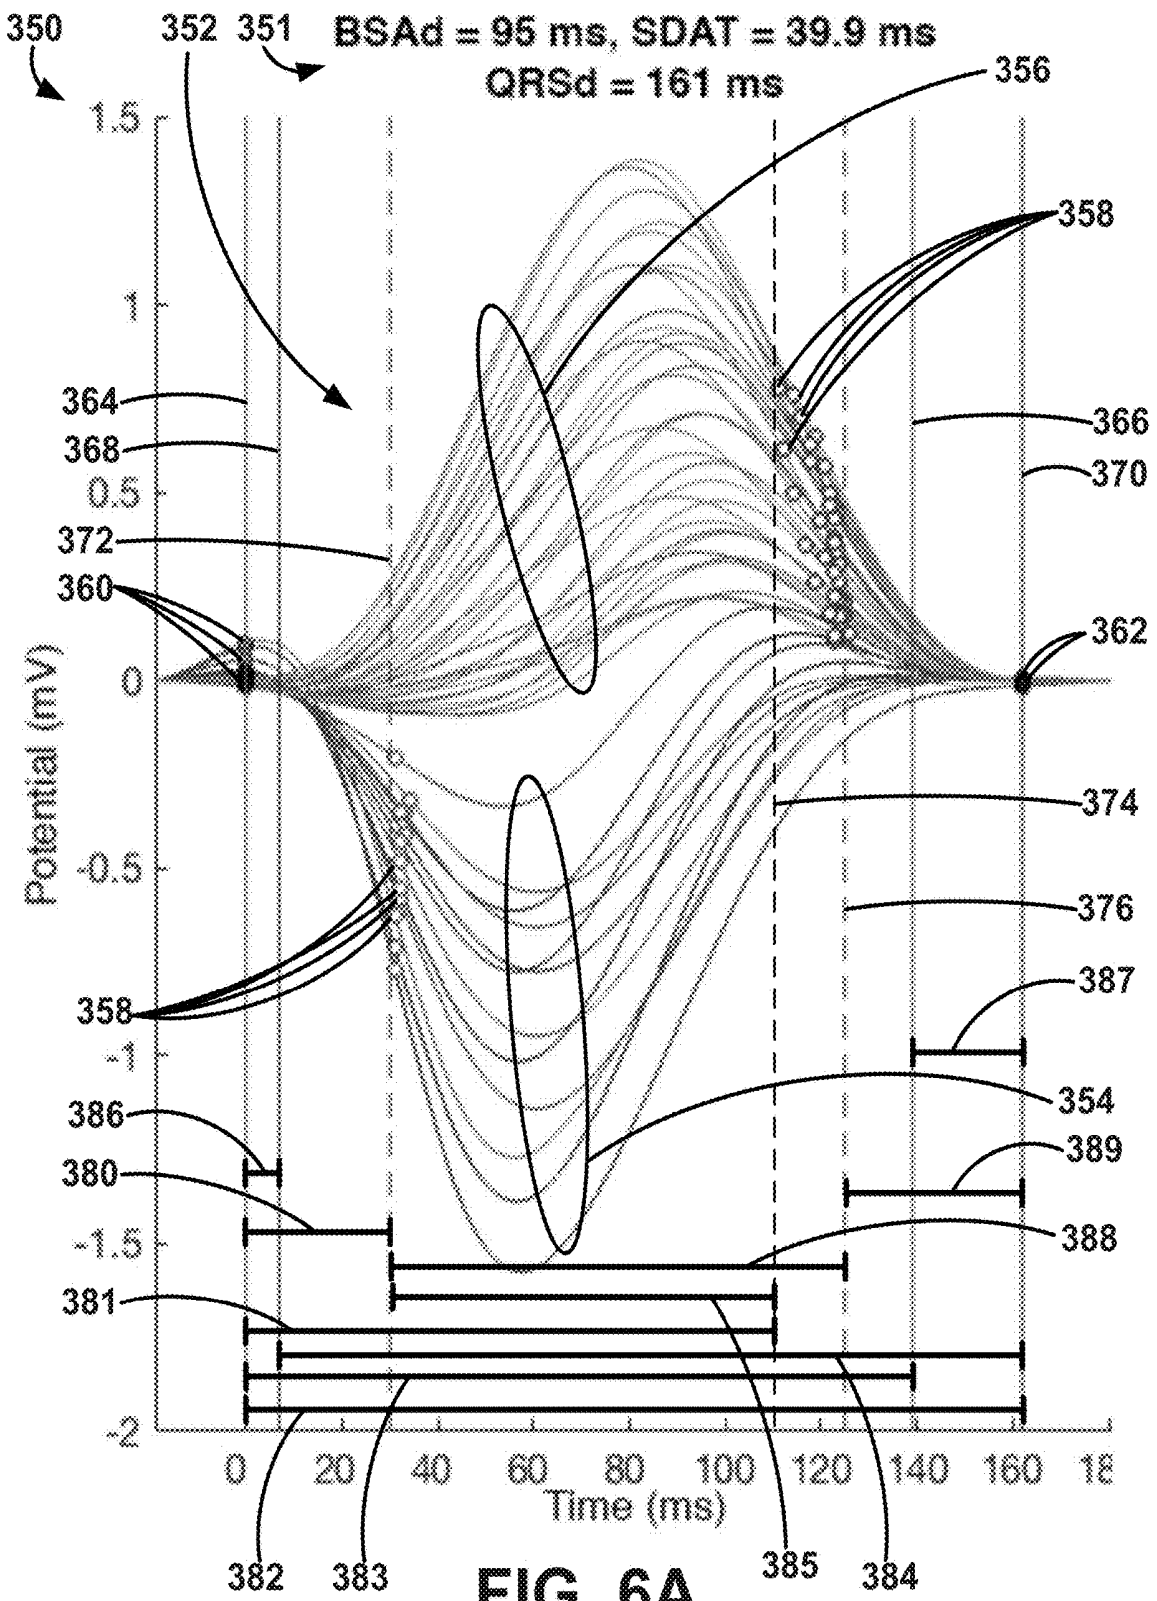


FIG. 5



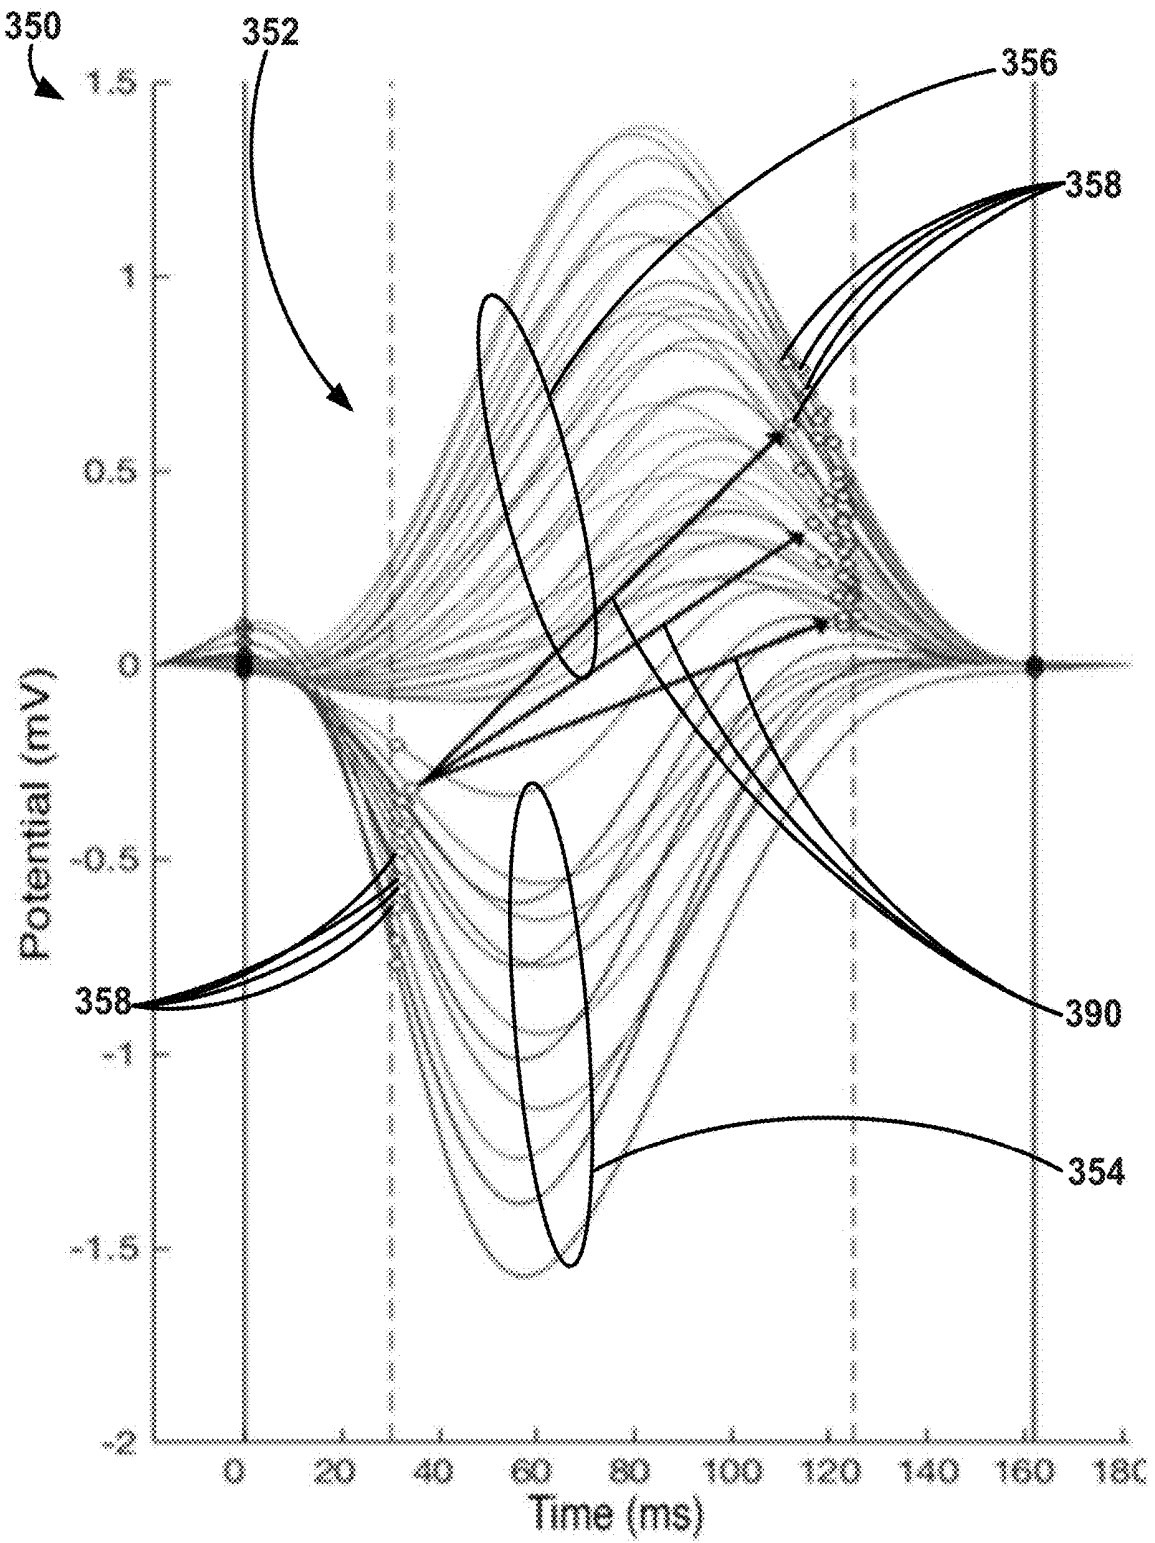
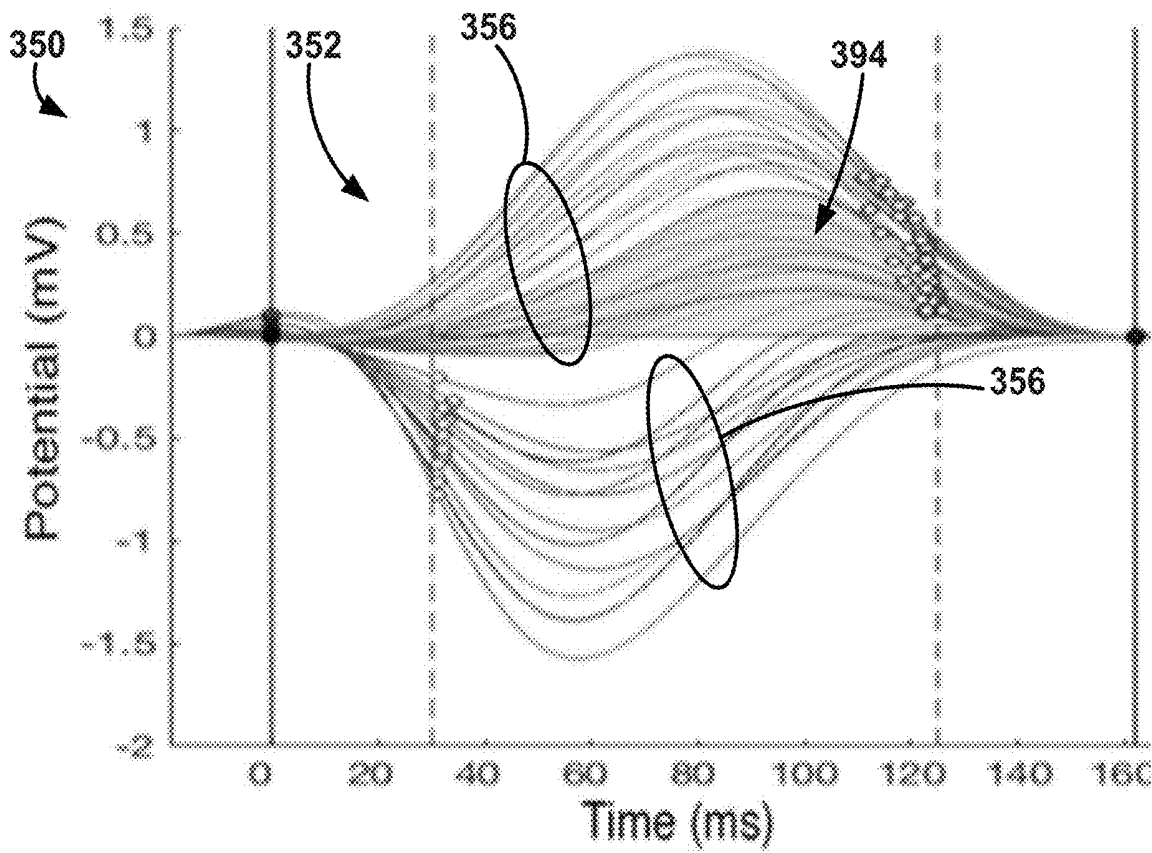
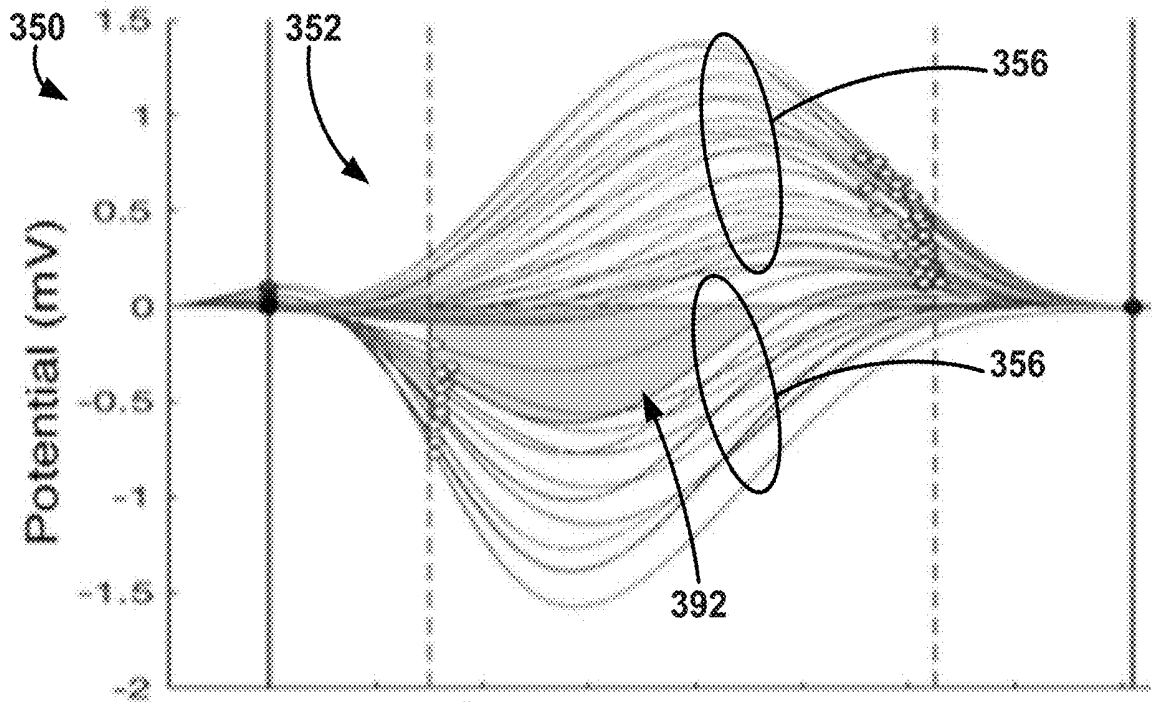


FIG. 6B



**FIG. 6C**

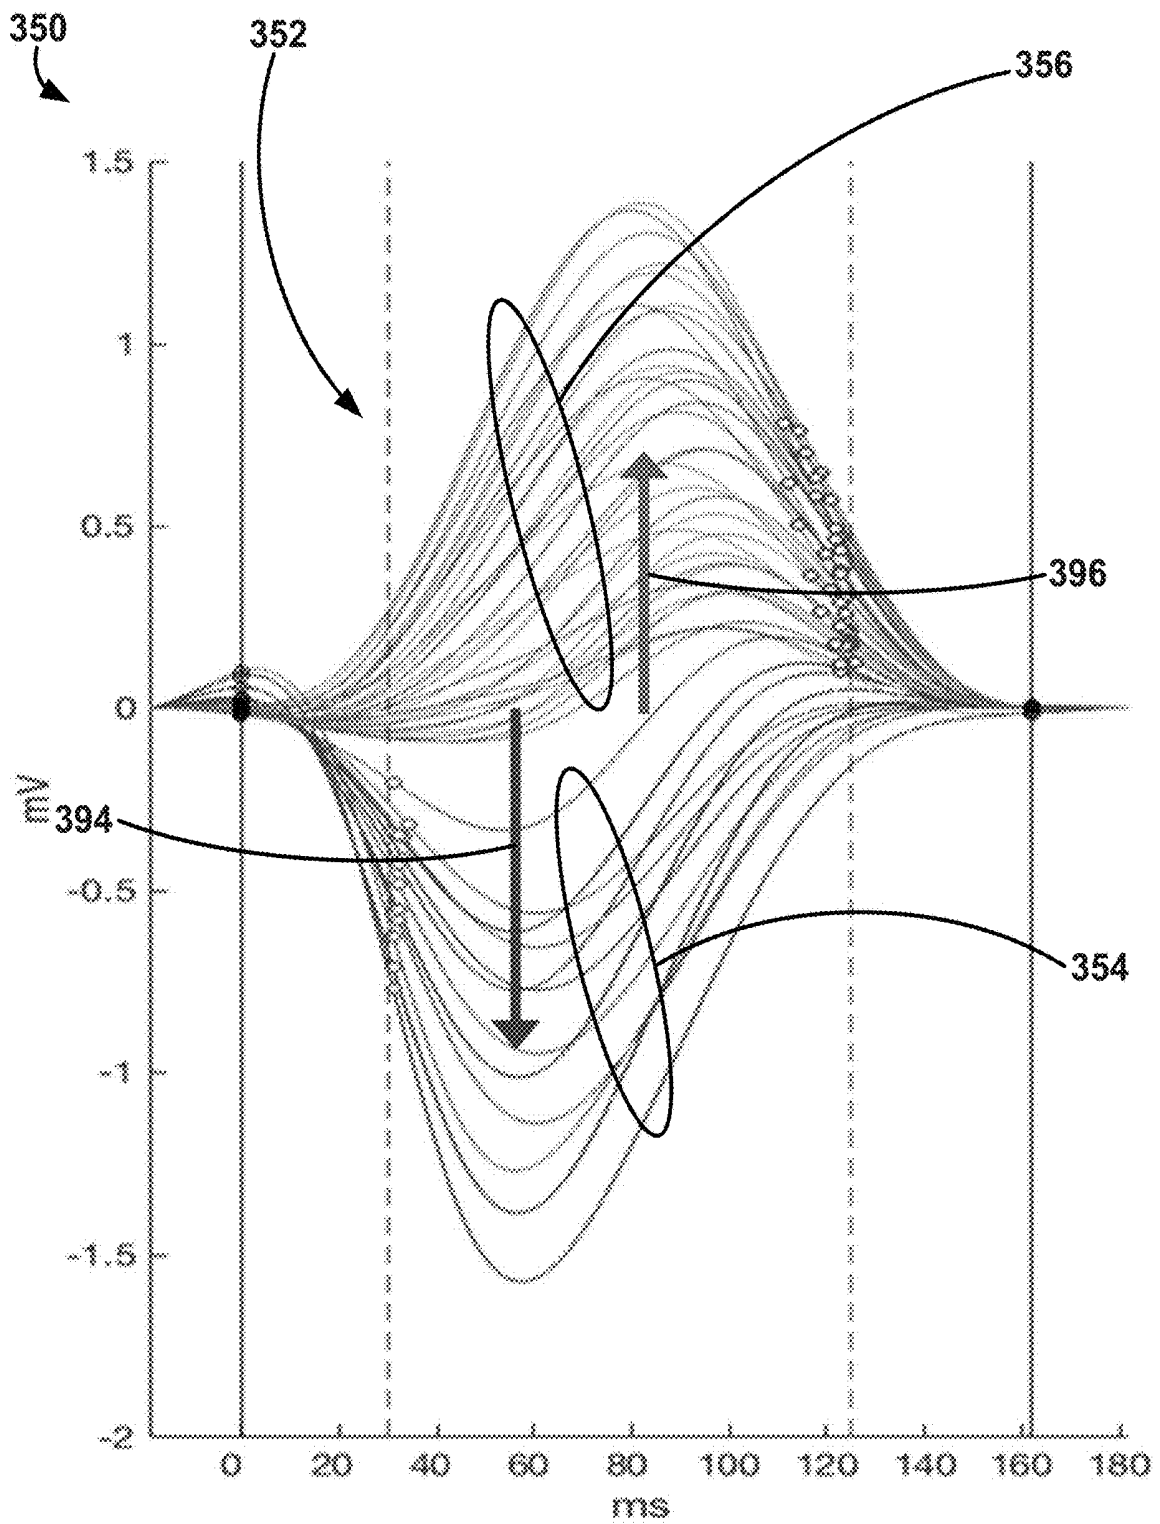


FIG. 6D

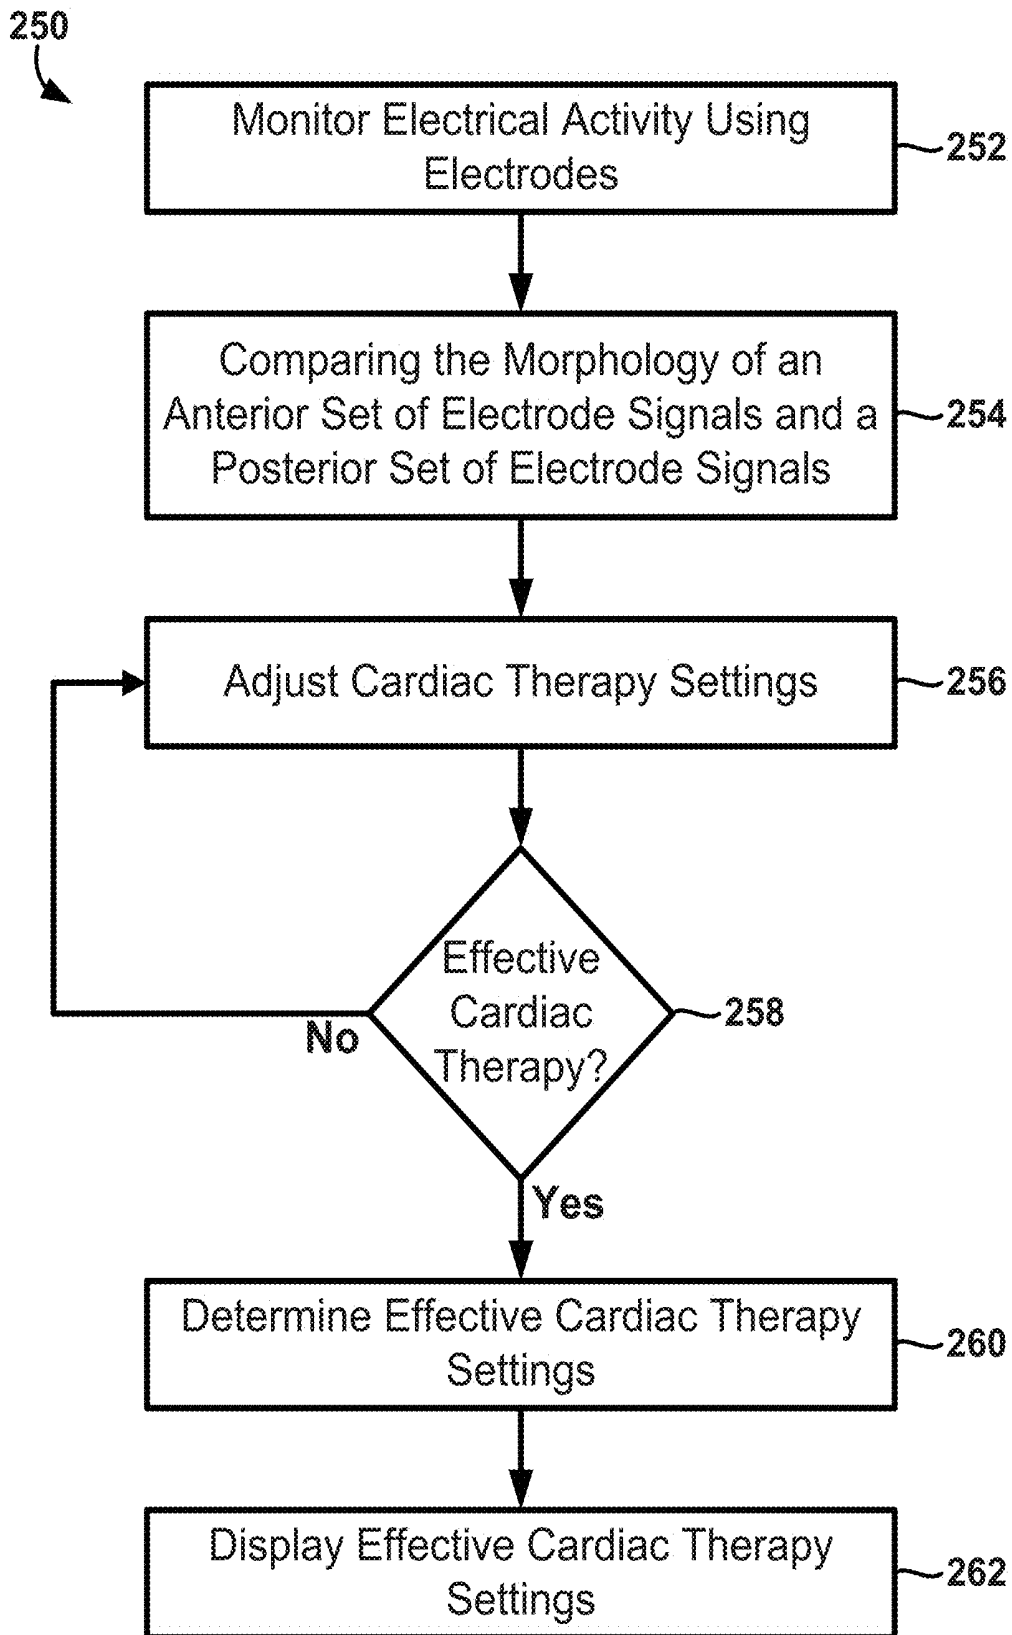


FIG. 7

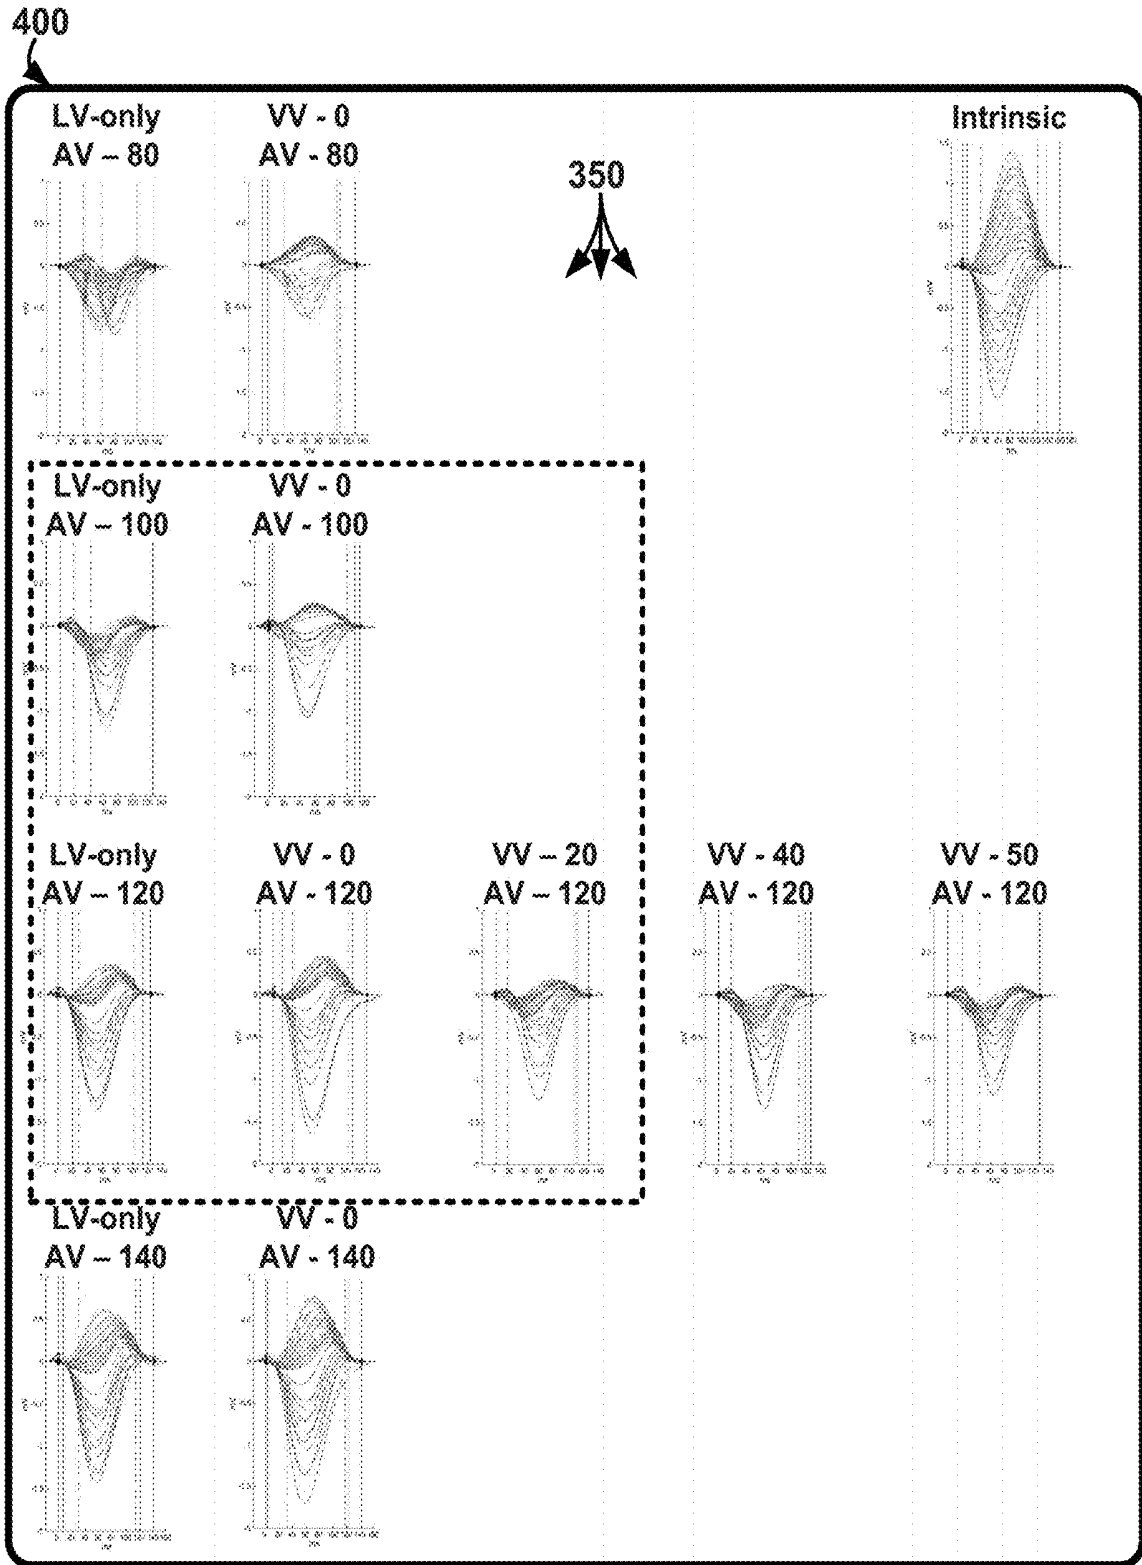


FIG. 8A

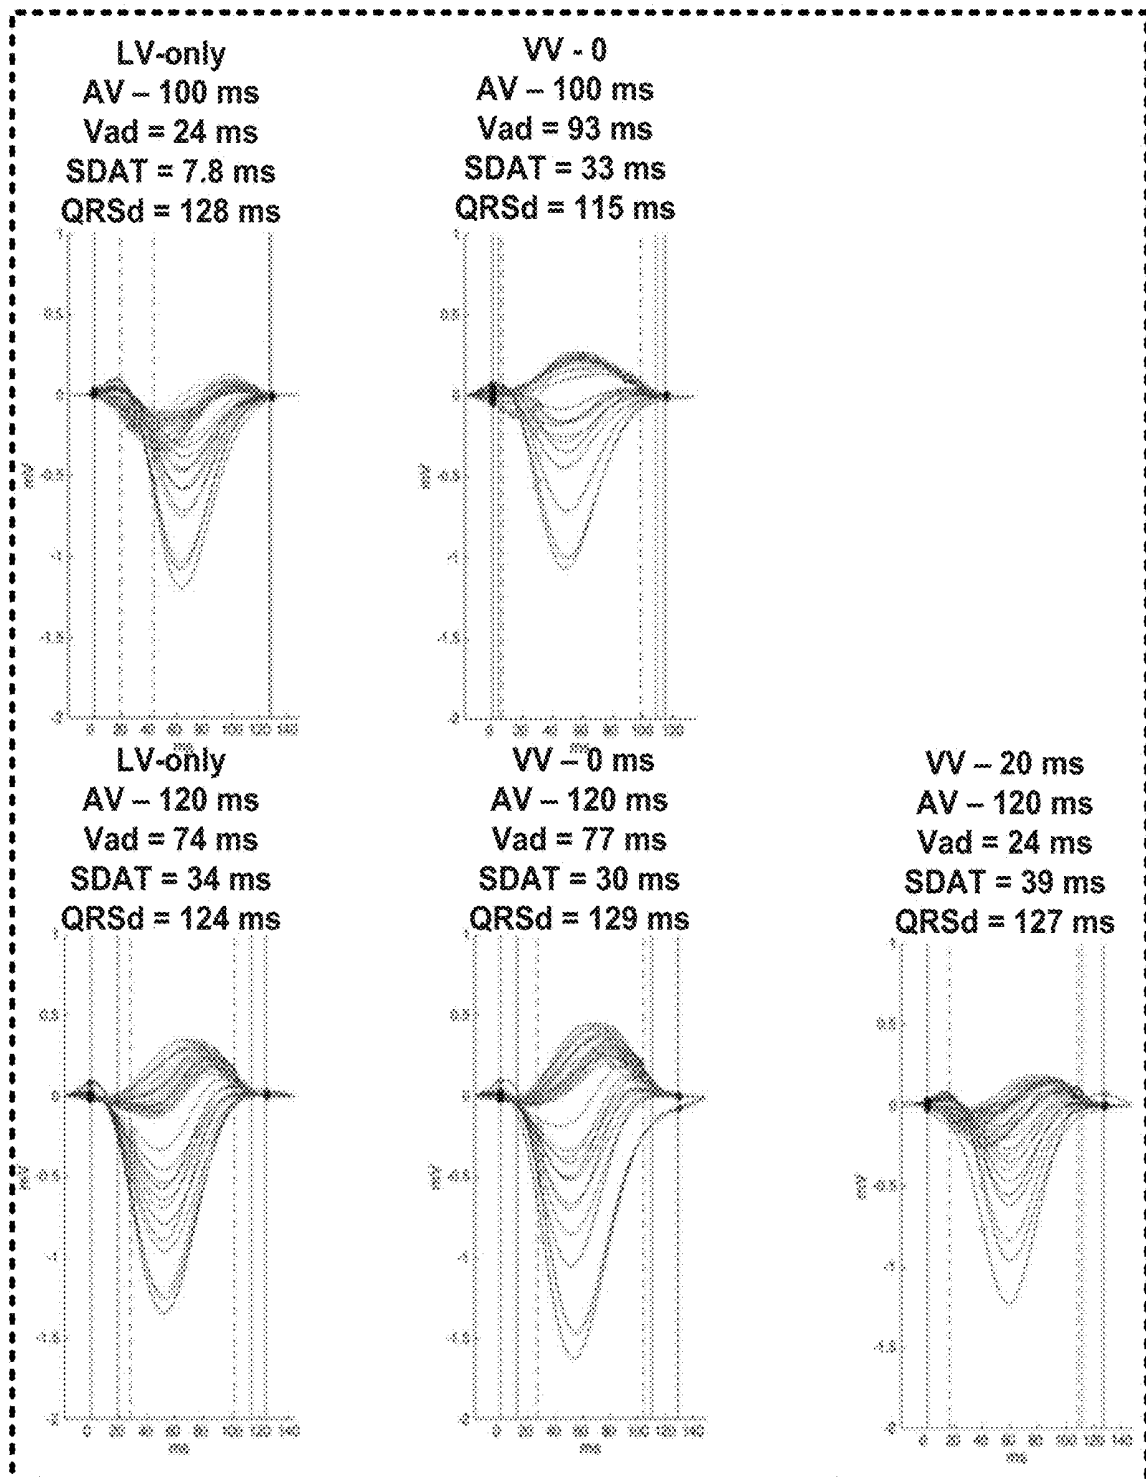


FIG. 8B

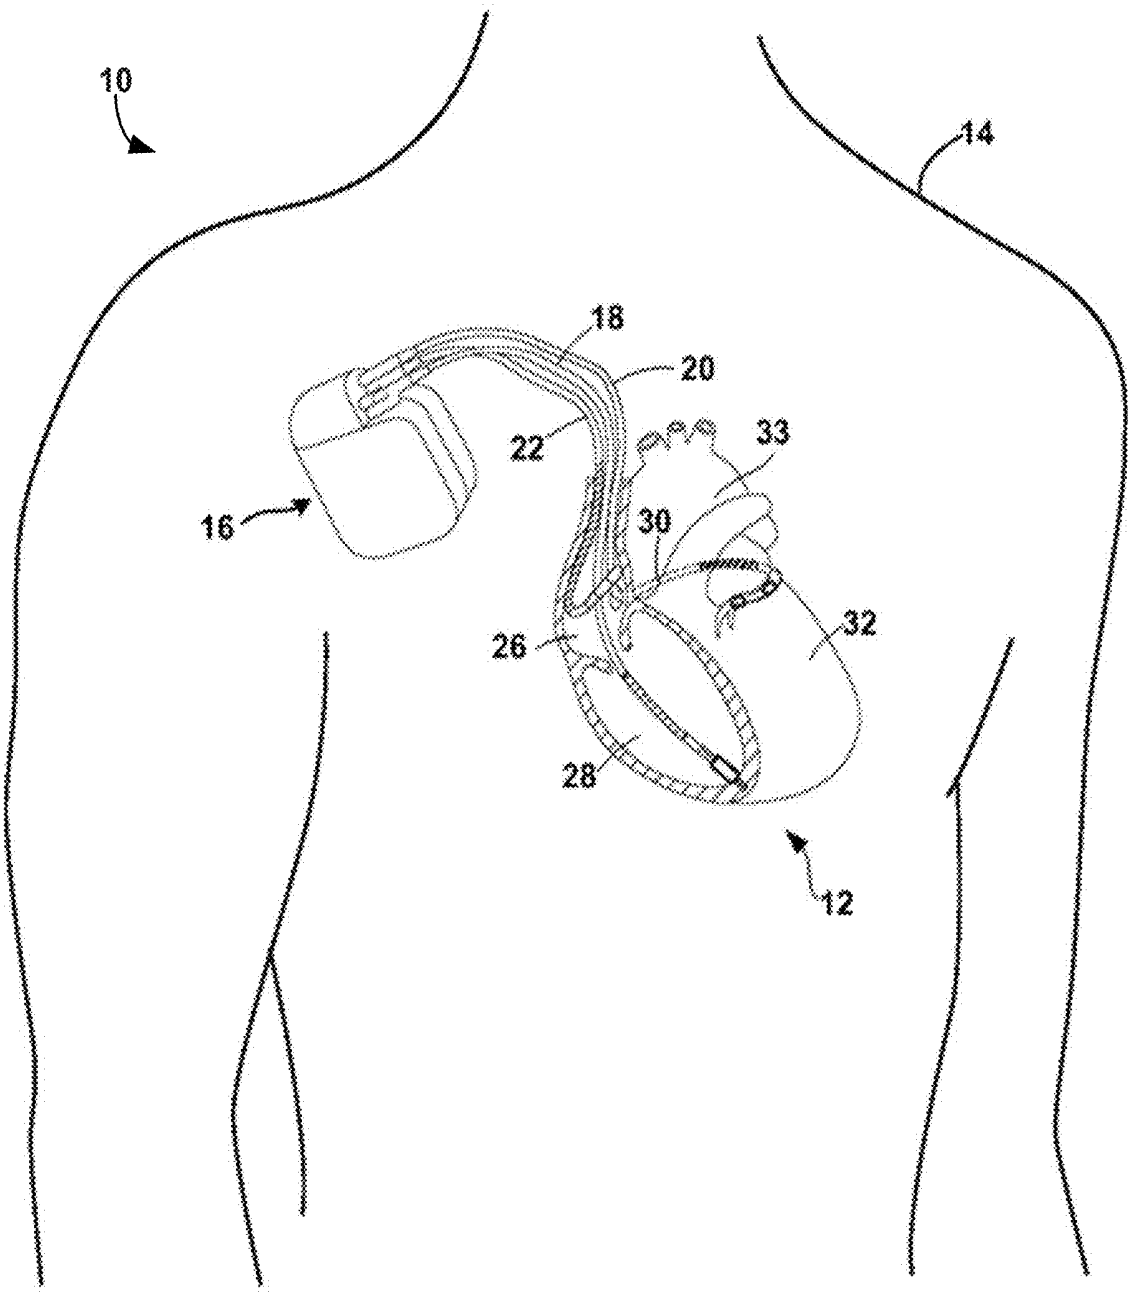


FIG. 9

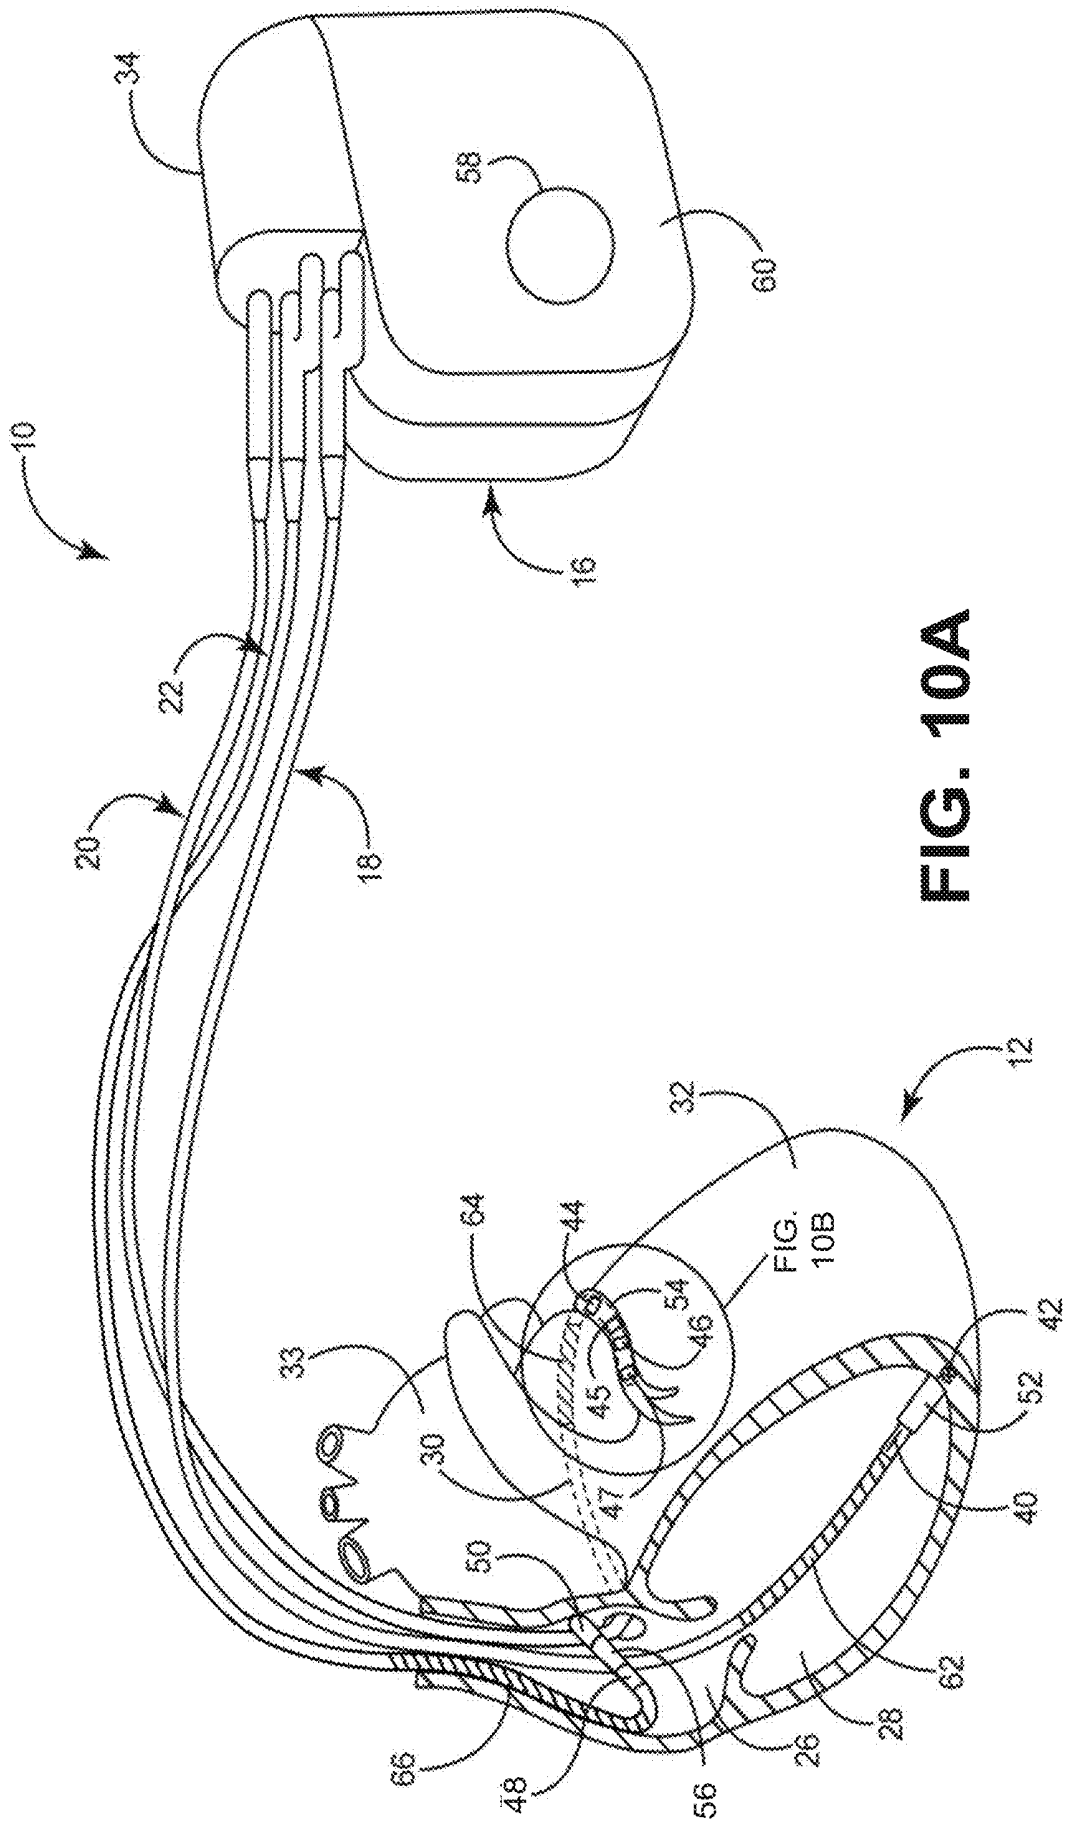
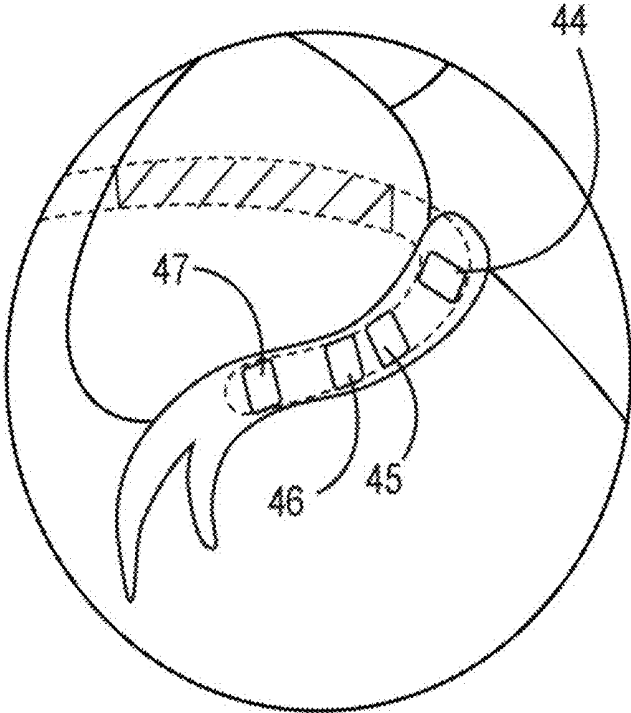


FIG. 10A



**FIG. 10B**

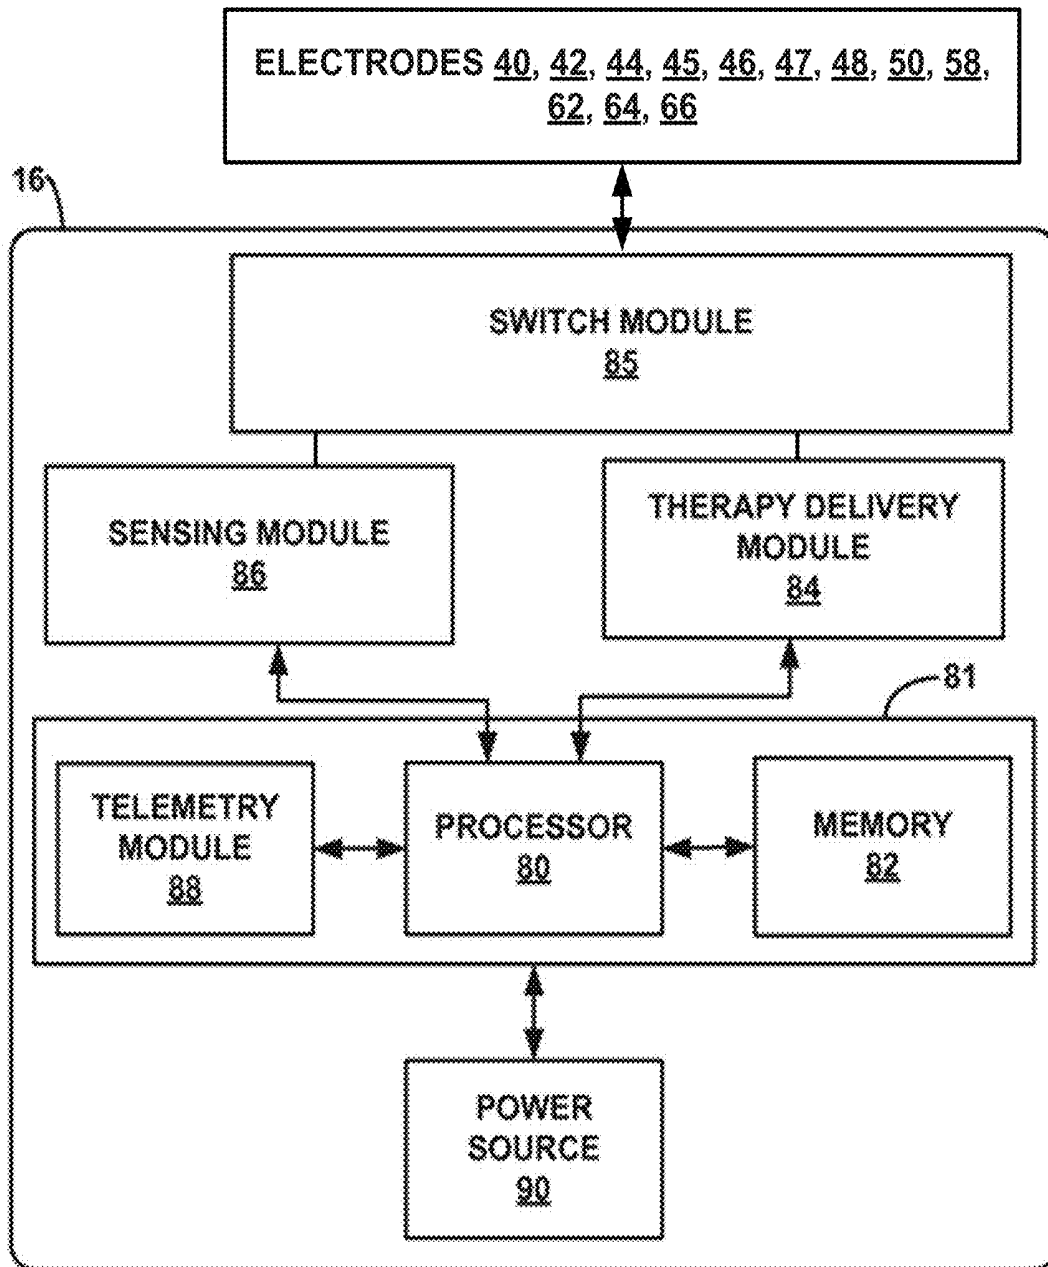


FIG. 11A

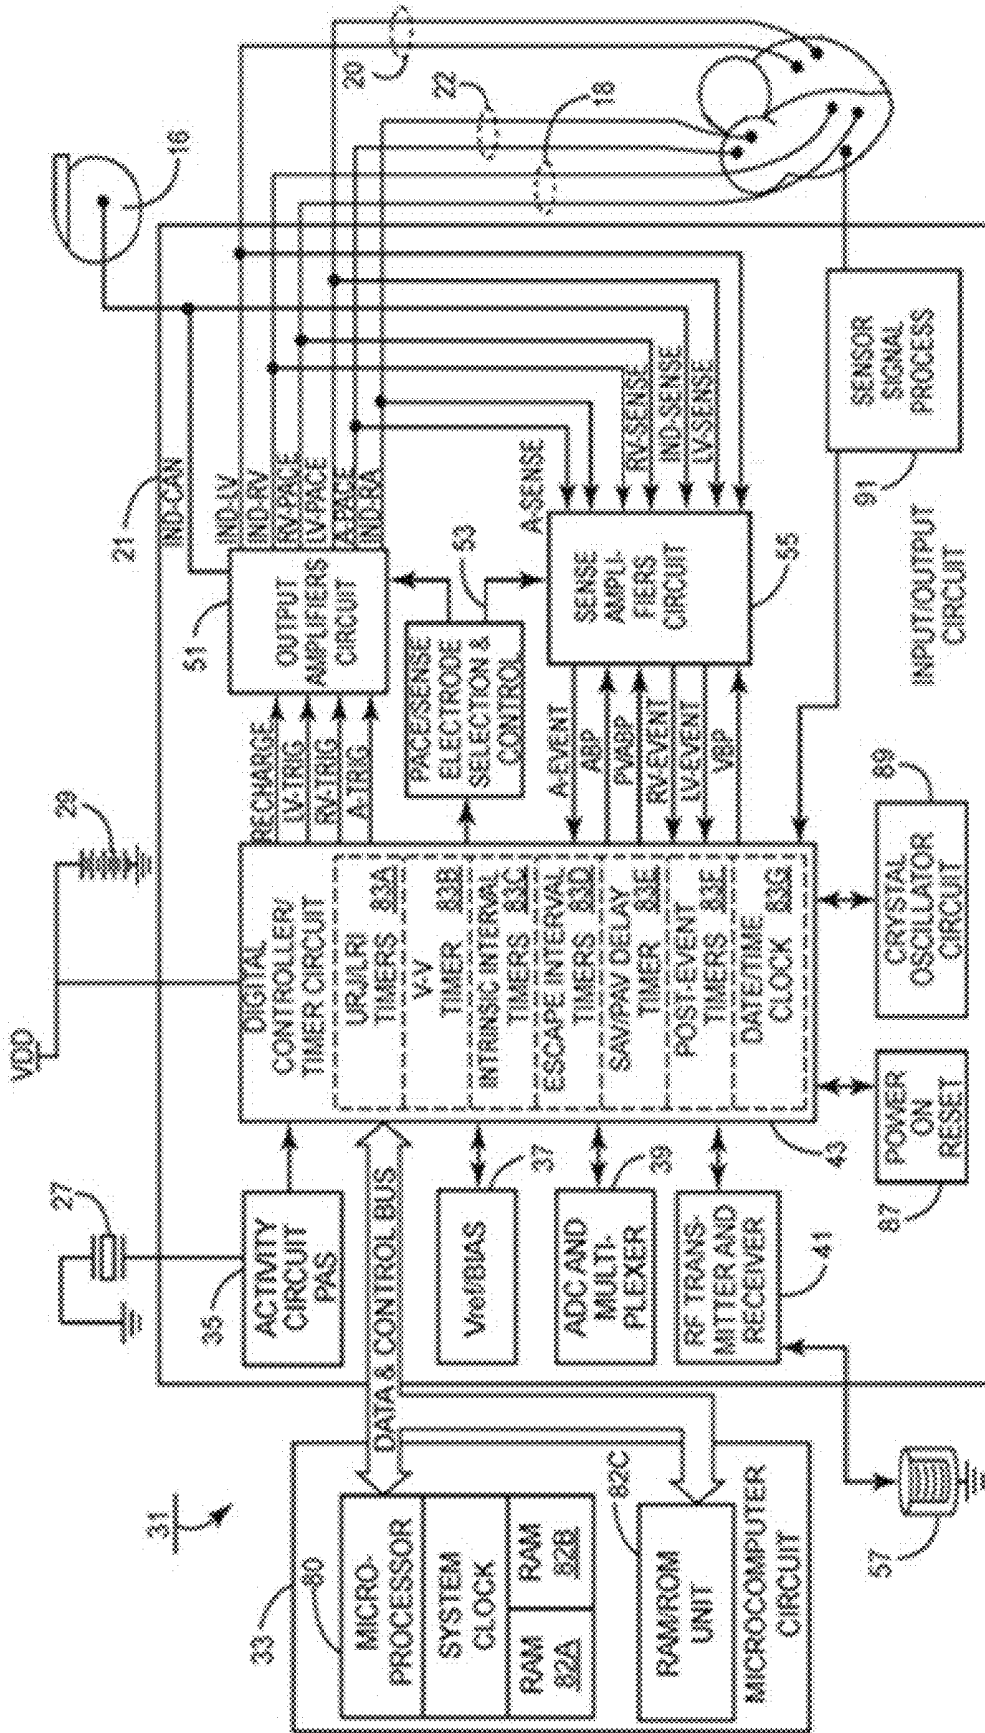


FIG. 11B

## ANTERIOR AND POSTERIOR ELECTRODE SIGNALS

This application claims the benefit of U.S. Provisional Patent Application Ser. No. 62/609,935 filed Dec. 22, 2017, entitled "Anterior and Posterior Electrode Signals," which is incorporated by reference herein in its entirety.

The disclosure herein relates to systems, methods, and interfaces for use in the analysis and processing of anterior and posterior electrode signals.

### SUMMARY

The exemplary systems, methods, and interfaces described herein may be configured to assist a user (e.g., a physician) in evaluating a patient and/or evaluating cardiac therapy (e.g., cardiac therapy being performed on a patient during and/or after implantation of cardiac therapy apparatus). In one or more embodiments, the systems, methods, and interfaces may be described as being noninvasive. For example, in some embodiments, the systems, methods, and interfaces may not need, or include, implantable devices such as leads, probes, sensors, catheters, implantable electrodes, etc. to monitor, or acquire, a plurality of cardiac signals from tissue of the patient for use in evaluating the patient and/or cardiac therapy being delivered to the patient. Instead, the systems, methods, and interfaces may use electrical measurements taken noninvasively using, e.g., a plurality of external electrodes attached to the skin of a patient about the patient's torso.

One exemplary system for use in cardiac evaluation may include electrode apparatus comprising a plurality of external electrodes to be located proximate a patient's skin. The plurality of external electrodes may include a posterior set of electrodes located proximate the patient's posterior and an anterior set of electrodes located proximate the patient's anterior. The computing apparatus may include processing circuitry and may be operably coupled to the electrode apparatus. The computing apparatus may be configured to monitor electrical activity from the patient's skin using the plurality of external electrodes over a cardiac cycle resulting in a posterior set of electrode signals monitored from one or more of the posterior set of electrodes and an anterior set of electrode signals monitored from one or more of the anterior set of electrodes and compare the morphology of the anterior set of electrode signals and the morphology of the posterior set of electrode signals to assist in determination of electrical heterogeneity.

One exemplary method for use in cardiac evaluation may include monitoring electrical activity from a patient's skin using a plurality of external electrodes over a cardiac cycle resulting in a posterior set of electrode signals monitored from one or more of posterior set of electrodes located proximate the patient's posterior and an anterior set of electrode signals monitored from one or more of an anterior set of electrodes located proximate the patient's anterior and comparing the morphology of the anterior set of electrode signals and the morphology of the posterior set of electrode signals to assist in determination of electrical heterogeneity.

The above summary is not intended to describe each embodiment or every implementation of the present disclosure. A more complete understanding will become apparent and appreciated by referring to the following detailed description and claims taken in conjunction with the accompanying drawings.

## BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a diagram of an exemplary system including electrode apparatus, display apparatus, and computing apparatus.

FIGS. 2-3 are diagrams of exemplary external electrode apparatus for measuring torso-surface potentials.

FIG. 4A is a block diagram of an exemplary method for determining typical cardiac cycles, or beats, and maximum QRS windows.

FIG. 4B is a block diagram of an exemplary method for determining various fiducial points within a QRS window of an electrode signal including QRS onset and offset.

FIG. 5 is an exemplary graphical user interface depicting three single-cycle graphs and activation time maps.

FIG. 6A is an exemplary single-cycle graph depicting a plurality of anterior and posterior electrode signals.

FIG. 6B is an exemplary single-cycle graph depicting a plurality of anterior and posterior electrode signals and few ventricular activation time distances.

FIG. 6C are exemplary single-cycle graphs depicting a plurality of anterior and posterior electrode signals and a few anterior and posterior areas under the curve.

FIG. 6D is an exemplary single-cycle graph depicting a plurality of anterior and posterior electrode signals and anterior and posterior net heights.

FIG. 7 is a block diagram of an exemplary method for comparing morphology of anterior and posterior sets of electrode signals and determining effective cardiac therapy settings.

FIG. 8A is an exemplary graphical user interface depicting a plurality of single-cycle graphs corresponding to various cardiac therapy settings.

FIG. 8B is an enlarged view of a portion of the graphical user interface of FIG. 8A.

FIG. 9 is a diagram of an exemplary system including an exemplary implantable medical device (IMD).

FIG. 10A is a diagram of the exemplary IMD of FIG. 9.

FIG. 10B is a diagram of an enlarged view of a distal end of the electrical lead disposed in the left ventricle of FIG. 10A.

FIG. 11A is a block diagram of an exemplary IMD, e.g., of the systems of FIGS. 9-10.

FIG. 11B is another block diagram of an exemplary IMD (e.g., an implantable pulse generator) circuitry and associated leads employed in the systems of FIGS. 9-10.

### DETAILED DESCRIPTION OF EXEMPLARY EMBODIMENTS

In the following detailed description of illustrative embodiments, reference is made to the accompanying figures of the drawing which form a part hereof, and in which are shown, by way of illustration, specific embodiments which may be practiced. It is to be understood that other embodiments may be utilized and structural changes may be made without departing from (e.g., still falling within) the scope of the disclosure presented hereby.

Exemplary systems, methods, and interfaces shall be described with reference to FIGS. 1-11. It will be apparent to one skilled in the art that elements or processes from one embodiment may be used in combination with elements or processes of the other embodiments, and that the possible embodiments of such methods and systems using combinations of features set forth herein is not limited to the specific embodiments shown in the Figures and/or described herein. Further, it will be recognized that the embodiments

described herein may include many elements that are not necessarily shown to scale. Still further, it will be recognized that timing of the processes and the size and shape of various elements herein may be modified but still fall within the scope of the present disclosure, although certain timings, one or more shapes and/or sizes, or types of elements, may be advantageous over others.

Cardiac electrical activation times can be detected or estimated in proximity of a reference location (e.g., which can be a chosen location for the left ventricle lead during implant) using unipolar electrocardiogram (ECG) recordings. Such electrical activation times may be measured and displayed, or conveyed, to an implanter by a system which acquires the ECG signals and generates the metric of electrical activation times (e.g., depolarization) measured from various ECG locations.

Various exemplary systems, methods, and interfaces may be configured to use electrode apparatus including external electrodes, display apparatus, and computing apparatus to noninvasively assist a user (e.g., a physician) in the evaluation of a patient's cardiac condition and/or cardiac therapy being performed on a patient. An exemplary system **100** including electrode apparatus **110**, display apparatus **130**, and computing apparatus **140** is depicted in FIG. 1.

The electrode apparatus **110** as shown includes a plurality of electrodes incorporated, or included, within a band wrapped around the chest, or torso, of a patient **14**. The electrode apparatus **110** is operatively coupled to the computing apparatus **140** (e.g., through one or wired electrical connections, wirelessly, etc.) to provide electrical signals (e.g., body-surface potentials) from each of the electrodes to the computing apparatus **140** for analysis, evaluation, etc. Exemplary electrode apparatus may be described in U.S. Pat. No. 9,320,446 entitled "Bioelectric Sensor Device and Methods" and issued on Apr. 26, 2016, which is incorporated herein by reference in its entirety. Further, exemplary electrode apparatus **110** will be described in more detail in reference to FIGS. 2-3.

Although not described herein, the exemplary system **100** may further include imaging apparatus. The imaging apparatus may be any type of imaging apparatus configured to image, or provide images of, at least a portion of the patient in a noninvasive manner. For example, the imaging apparatus may not use any components or parts that may be located within the patient to provide images of the patient except noninvasive tools such as contrast solution. It is to be understood that the exemplary systems, methods, and interfaces described herein may further use imaging apparatus to provide noninvasive assistance to a user (e.g., a physician) to locate or select a pacing electrode or pacing vector proximate the patient's heart in conjunction with the evaluation of cardiac therapy.

For example, the exemplary systems, methods, and interfaces may provide image-guided navigation that may be used to navigate leads including electrodes, leadless electrodes, wireless electrodes, catheters, etc., within the patient's body while also providing noninvasive cardiac therapy evaluation including determining location information (e.g., location information for the electrodes). Exemplary systems and methods that use imaging apparatus and/or electrode apparatus may be described in U.S. Pat. No. 9,877,789 issued Jan. 30, 2018, and entitled "Implantable Electrode Location Selection," U.S. Patent Application Pub. No. US 2014/0371833 A1 published Dec. 18, 2014, and entitled "Implantable Electrode Location Selection," U.S. Pat. No. 9,924,884 issued Mar. 27, 2018, and entitled "Systems, Methods, and Interfaces for Identifying Effective

Electrodes," U.S. Pat. No. 10,064,567 issued Sep. 4, 2018, and entitled "Systems, Methods, and Interfaces for Identifying Optical Electrical Vectors," each of which is incorporated herein by reference in its entirety.

Exemplary imaging apparatus may be configured to capture x-ray images and/or any other alternative imaging modality. For example, the imaging apparatus may be configured to capture images, or image data, using isocentric fluoroscopy, bi-plane fluoroscopy, ultrasound, computed tomography (CT), multi-slice computed tomography (MSCT), magnetic resonance imaging (MRI), high frequency ultrasound (HIFU), optical coherence tomography (OCT), intra-vascular ultrasound (IVUS), two dimensional (2D) ultrasound, three dimensional (3D) ultrasound, four dimensional (4D) ultrasound, intraoperative CT, intraoperative Mill, etc. Further, it is to be understood that the imaging apparatus may be configured to capture a plurality of consecutive images (e.g., continuously) to provide video frame data. In other words, a plurality of images taken over time using the imaging apparatus may provide video frame, or motion picture, data. Additionally, the images may also be obtained and displayed in two, three, or four dimensions. In more advanced forms, four-dimensional surface rendering of the heart or other regions of the body may also be achieved by incorporating heart data or other soft tissue data from a map or from pre-operative image data captured by MRI, CT, or echocardiography modalities. Image datasets from hybrid modalities, such as positron emission tomography (PET) combined with CT, or single photon emission computer tomography (SPECT) combined with CT, could also provide functional image data superimposed onto anatomical data, e.g., to be used to navigate treatment apparatus proximate target locations within the heart or other areas of interest.

Systems and/or imaging apparatus that may be used in conjunction with the exemplary systems and method described herein are described in U.S. Pat. App. Pub. No. 2005/0008210 to Evron et al. published on Jan. 13, 2005, U.S. Pat. App. Pub. No. 2006/0074285 to Zarkh et al. published on Apr. 6, 2006, U.S. Pat. No. 8,731,642 issued May 20, 2014, to Zarkh et al. U.S. Pat. No. 8,861,830 issued Oct. 14, 2014, to Brada et al. U.S. Pat. No. 6,980,675 to Evron et al. issued on Dec. 27, 2005, U.S. Pat. No. 7,286,866 to Okerlund et al. issued on Oct. 23, 2007, U.S. Pat. No. 7,308,297 to Reddy et al. issued on Dec. 11, 2011, U.S. Pat. No. 7,308,299 to Burrell et al. issued on Dec. 11, 2011, U.S. Pat. No. 7,321,677 to Evron et al. issued on Jan. 22, 2008, U.S. Pat. No. 7,346,381 to Okerlund et al. issued on Mar. 18, 2008, U.S. Pat. No. 7,454,248 to Burrell et al. issued on Nov. 18, 2008, U.S. Pat. No. 7,499,743 to Vass et al. issued on Mar. 3, 2009, U.S. Pat. No. 7,565,190 to Okerlund et al. issued on Jul. 21, 2009, U.S. Pat. No. 7,587,074 to Zarkh et al. issued on Sep. 8, 2009, U.S. Pat. No. 7,599,730 to Hunter et al. issued on Oct. 6, 2009, U.S. Pat. No. 7,613,500 to Vass et al. issued on Nov. 3, 2009, U.S. Pat. No. 7,742,629 to Zarkh et al. issued on Jun. 22, 2010, U.S. Pat. No. 7,747,047 to Okerlund et al. issued on Jun. 29, 2010, U.S. Pat. No. 7,778,685 to Evron et al. issued on Aug. 17, 2010, U.S. Pat. No. 7,778,686 to Vass et al. issued on Aug. 17, 2010, U.S. Pat. No. 7,813,785 to Okerlund et al. issued on Oct. 12, 2010, U.S. Pat. No. 7,996,063 to Vass et al. issued on Aug. 9, 2011, U.S. Pat. No. 8,060,185 to Hunter et al. issued on Nov. 15, 2011, and U.S. Pat. No. 8,401,616 to Verard et al. issued on Mar. 19, 2013, each of which is incorporated herein by reference in its entirety.

The display apparatus **130** and the computing apparatus **140** may be configured to display and analyze data such as,

e.g., electrical signals (e.g., electrocardiogram data), cardiac information representative of at least one of mechanical cardiac functionality and electrical cardiac functionality, etc. Cardiac information may include, e.g., electrical heterogeneity information or electrical dyssynchrony information, body surface cardiac activation information, surrogate cardiac electrical activation information or data, etc. that is generated using electrical signals (e.g., body-surface potentials) gathered, monitored, or collected, using the electrode apparatus **110**. In at least one embodiment, the computing apparatus **140** may be a server, a personal computer, or a tablet computer. The computing apparatus **140** may be configured to receive input from input apparatus **142** and transmit output to the display apparatus **130**. Further, the computing apparatus **140** may include data storage that may allow for access to processing programs or routines and/or one or more other types of data, e.g., for driving a graphical user interface configured to noninvasively assist a user in evaluating, selecting, and/or determining cardiac therapy settings (e.g., the location of an implantable electrode used for pacing, the location of pacing therapy delivered by a particular pacing vector, type of pacing therapy such as biventricular pacing, and left ventricular-only pacing, and various timings of pacing therapy such as atrioventricular (AV) delay, interventricular (VV) delay, pulse width, and/or voltage).

The computing apparatus **140** may be operatively coupled to the input apparatus **142** and the display apparatus **130** to, e.g., transmit data to and from each of the input apparatus **142** and the display apparatus **130**. For example, the computing apparatus **140** may be electrically coupled to each of the input apparatus **142** and the display apparatus **130** using, e.g., analog electrical connections, digital electrical connections, wireless connections, bus-based connections, network-based connections, internet-based connections, etc. As described further herein, a user may provide input to the input apparatus **142** to manipulate, or modify, one or more graphical depictions displayed on the display apparatus **130** and to view and/or select one or more pieces of information related to the cardiac therapy.

Although as depicted the input apparatus **142** is a keyboard, it is to be understood that the input apparatus **142** may include any apparatus capable of providing input to the computing apparatus **140** to perform the functionality, methods, and/or logic described herein. For example, the input apparatus **142** may include a mouse, a trackball, a touchscreen (e.g., capacitive touchscreen, a resistive touchscreen, a multi-touch touchscreen, etc.), etc. Likewise, the display apparatus **130** may include any apparatus capable of displaying information to a user, such as a graphical user interface **132** including cardiac information, textual instructions, graphical depictions of electrical activation information, graphical depictions of a plurality of signals including anterior and posterior electrode signals, graphical depictions of anatomy of a human heart, images or graphical depictions of the patient's heart, graphical depictions of locations of one or more electrodes, graphical depictions of a human torso, images or graphical depictions of the patient's torso, graphical depictions or actual images of implanted electrodes and/or leads, etc. Further, the display apparatus **130** may include a liquid crystal display, an organic light-emitting diode screen, a touchscreen, a cathode ray tube display, etc.

The processing programs or routines stored and/or executed by the computing apparatus **140** may include programs or routines for computational mathematics, matrix mathematics, dispersion determinations (e.g. standard

deviations, distances, areas under the curve, variances, ranges, interquartile ranges, mean absolute differences, average absolute deviations, etc.), filtering algorithms, maximum value determinations, minimum value determinations, threshold determinations, moving windowing algorithms, decomposition algorithms, compression algorithms (e.g., data compression algorithms), calibration algorithms, image construction algorithms, signal processing algorithms (e.g., various filtering algorithms, Fourier transforms, fast Fourier transforms, etc.), standardization algorithms, comparison algorithms, vector mathematics, or any other processing required to implement one or more exemplary methods and/or processes described herein. Data stored and/or used by the computing apparatus **140** may include, for example, electrical signal/waveform data from the electrode apparatus **110** (such as, e.g., anterior and posterior electrode signals over a plurality of cardiac cycles, over a single cardiac cycles, over various slices of time, etc.), parts or portions of various signals, electrical activation times from the electrode apparatus **110**, graphics (e.g., graphical elements, icons, buttons, windows, dialogs, pull-down menus, graphic areas, graphic regions, 3D graphics, etc.), graphical user interfaces, results from one or more processing programs or routines employed according to the disclosure herein (e.g., electrical signals, cardiac information, etc.), or any other data that may be necessary for carrying out the one and/or more processes or methods described herein.

In one or more embodiments, the exemplary systems, methods, and interfaces may be implemented using one or more computer programs executed on programmable computers, such as computers that include, for example, processing capabilities, data storage (e.g., volatile or non-volatile memory and/or storage elements), input devices, and output devices. Program code and/or logic described herein may be applied to input data to perform functionality described herein and generate desired output information. The output information may be applied as input to one or more other devices and/or methods as described herein or as would be applied in a known fashion.

The one or more programs used to implement the systems, methods, and/or interfaces described herein may be provided using any programmable language, e.g., a high-level procedural and/or object orientated programming language that is suitable for communicating with a computer system. Any such programs may, for example, be stored on any suitable device, e.g., a storage media, that is readable by a general or special purpose program running on a computer system (e.g., including processing apparatus) for configuring and operating the computer system when the suitable device is read for performing the procedures described herein. In other words, at least in one embodiment, the exemplary systems, methods, and/or interfaces may be implemented using a computer readable storage medium, configured with a computer program, where the storage medium so configured causes the computer to operate in a specific and predefined manner to perform functions described herein. Further, in at least one embodiment, the exemplary systems, methods, and/or interfaces may be described as being implemented by logic (e.g., object code) encoded in one or more non-transitory media that includes code for execution and, when executed by a processor, is operable to perform operations such as the methods, processes, and/or functionality described herein.

The computing apparatus **140** may be, for example, any fixed or mobile computer system (e.g., a controller, a micro-controller, a personal computer, minicomputer, tablet computer, etc.) and may be generally described as including

processing circuitry. The exact configuration of the computing apparatus 140 is not limiting, and essentially any device capable of providing suitable computing capabilities and control capabilities (e.g., graphics processing, etc.) may be used. As described herein, a digital file may be any medium (e.g., volatile or non-volatile memory, a CD-ROM, a punch card, magnetic recordable medium such as a disk or tape, etc.) containing digital bits (e.g., encoded in binary, trinary, etc.) that may be readable and/or writeable by computing apparatus 140 described herein. Also, as described herein, a file in user-readable format may be any representation of data (e.g., ASCII text, binary numbers, hexadecimal numbers, decimal numbers, graphically, etc.) presentable on any medium (e.g., paper, a display, etc.) readable and/or understandable by a user.

In view of the above, it will be readily apparent that the functionality as described in one or more embodiments according to the present disclosure may be implemented in any manner as would be known to one skilled in the art. As such, the computer language, the computer system, or any other software/hardware which is to be used to implement the processes described herein shall not be limiting on the scope of the systems, processes or programs (e.g., the functionality provided by such systems, processes or programs) described herein.

Electrical signal activity of the patient's heart monitored using electrode apparatus 110 as shown in FIG. 3 may be useful to evaluate a patient's cardiac condition and/or cardiac therapy being delivered to a patient. The exemplary electrode apparatus 110 may be configured to measure electrical activity (e.g., body-surface potentials) of a patient 14 and, more particularly, electrical activity (e.g., torso-surface potentials) of a patient 14. As shown in FIG. 2, the exemplary electrode apparatus 110 may include a set, or array, of electrodes 112, a strap 113, and interface/amplifier circuitry 116. The electrodes 112 may be attached, or coupled, to the strap 113 and the strap 113 may be configured to be wrapped around the torso of a patient 14 such that the electrodes 112 surround the patient's heart. As further illustrated, the electrodes 112 may be positioned around the circumference of a patient 14, including the posterior, lateral, posterolateral, anterolateral, and anterior locations of the torso of a patient 14. The electrodes 112 may be positioned proximate the tissue (e.g., skin) of the patient to acquire electrical signals or activity (e.g., body-surface potentials). In other words, the electrodes 112 may be positioned near or operably in contact with the tissue of the patient so as to be able to sense electrical signals or activity (e.g., body-surface potentials). Further, the electrodes 112 may be described as being "on" and/or secured to the skin of the patient. Still further, the electrodes 112 may be attached to the tissue of the patient using a conductive adhesive such as a conductive adhesive layer. Further the conductive adhesive and/or conductive adhesive layer may include conductive gel.

Further, the electrodes 112 may be electrically connected to interface/amplifier circuitry 116 via wired connection 118. The interface/amplifier circuitry 116 may be configured to amplify the signals from the electrodes 112 and provide the signals to the computing apparatus 140. Other exemplary systems may use a wireless connection to transmit the signals sensed by electrodes 112 to the interface/amplifier circuitry 116 and, in turn, the computing apparatus 140, e.g., as channels of data. For example, the interface/amplifier circuitry 116 may be electrically coupled to each of the computing apparatus 140 and the display apparatus 130 using, e.g., analog electrical connections, digital electrical

connections, wireless connections, bus-based connections, network-based connections, internet-based connections, etc.

Although in the example of FIG. 2 the electrode apparatus 110 includes a strap 113, in other examples any of a variety of mechanisms, e.g., tape or adhesives, may be employed to aid in the spacing and placement of electrodes 112. In some examples, the strap 113 may include an elastic band, strip of tape, or cloth. In other examples, the electrodes 112 may be placed individually on the torso of a patient 14. Further, in other examples, electrodes 112 (e.g., arranged in an array) may be part of, or located within, patches, vests, and/or other manners of securing the electrodes 112 to the torso of the patient 14.

The electrodes 112 may be configured to surround the heart of the patient 14 and record, or monitor, the electrical signals associated with the depolarization and repolarization of the heart after the signals have propagated through the torso of a patient 14. Each of the electrodes 112 may be used in a unipolar configuration to sense the torso-surface potentials that reflect the cardiac signals. The interface/amplifier circuitry 116 may also be coupled to a return or indifferent electrode (not shown) that may be used in combination with each electrode 112 for unipolar sensing. In some examples, there may be about 12 to about 50 electrodes 112 spatially distributed around the torso of patient. Other configurations may have more or fewer electrodes 112.

The computing apparatus 140 may record and analyze the electrical activity (e.g., torso-surface potential signals) sensed by electrodes 112 and amplified/conditioned by the interface/amplifier circuitry 116. The computing apparatus 140 may be configured to analyze the signals from the electrodes 112 to provide as anterior and posterior electrode signals, body surface cardiac electrical activation times, and surrogate cardiac electrical activation times, e.g., representative of actual, or local, electrical activation times of one or more regions of the patient's heart as will be further described herein. Further, the electrical signals measured at the left anterior surface location of a patient's torso may be representative, or surrogates, of electrical signals of the left anterior left ventricle region of the patient's heart, electrical signals measured at the left lateral surface location of a patient's torso may be representative, or surrogates, of electrical signals of the left lateral left ventricle region of the patient's heart, electrical signals measured at the left posterolateral surface location of a patient's torso may be representative, or surrogates, of electrical signals of the posterolateral left ventricle region of the patient's heart, and electrical signals measured at the posterior surface location of a patient's torso may be representative, or surrogates, of electrical signals of the posterior left ventricle region of the patient's heart. In one or more embodiments, measurement of activation times can be performed by measuring the period of time between an onset of cardiac depolarization (e.g., onset of QRS complex) and an appropriate fiducial point such as, e.g., a peak value, a minimum value, a minimum slope, a maximum slope, a zero crossing, a threshold crossing, etc. In one or more embodiments, activation times may be generally determined by measuring the time from the earliest onset time within electrical activity from a plurality of external electrodes over a cardiac cycle (e.g., a depolarization portion of the cardiac cycle, the QRS complex, etc.) to the steepest, or maximum, negative slope within the electrical activity monitored by the particular external electrode for which the activation time is being calculated for.

Additionally, the computing apparatus 140 may be configured to provide graphical user interfaces depicting the

body surface cardiac electrical activation times and/or surrogate cardiac electrical activation times obtained using the electrode apparatus **110**. Exemplary systems, methods, and/or interfaces may noninvasively use the electrical information collected using the electrode apparatus **110** to evaluate a patient's cardiac condition and/or cardiac therapy being delivered to the patient.

FIG. **3** illustrates another exemplary electrode apparatus **110** that includes a plurality of electrodes **112** configured to surround the heart of the patient **14** and record, or monitor, the electrical signals associated with the depolarization and repolarization of the heart after the signals have propagated through the torso of the patient **14**. The electrode apparatus **110** may include a vest **114** upon which the plurality of electrodes **112** may be attached, or to which the electrodes **112** may be coupled. In at least one embodiment, the plurality, or array, of electrodes **112** may be used to collect electrical information such as, e.g., anterior and posterior electrode signals, body surface cardiac electrical activation times and surrogate cardiac electrical activation times. Similar to the electrode apparatus **110** of FIG. **2**, the electrode apparatus **110** of FIG. **3** may include interface/amplifier circuitry **116** electrically coupled to each of the electrodes **112** through a wired connection **118** and be configured to transmit signals from the electrodes **112** to computing apparatus **140**. As illustrated, the electrodes **112** may be distributed over the torso of a patient **14**, including, for example, the anterior, lateral, posterolateral, anterolateral, and posterior surfaces of the torso of the patient **14**.

The vest **114** may be formed of fabric with the electrodes **112** attached to the fabric. The vest **114** may be configured to maintain the position and spacing of electrodes **112** on the torso of the patient **14**. Further, the vest **114** may be marked to assist in determining the location of the electrodes **112** on the surface of the torso of the patient **14**. In one or more embodiments, the vest **114** may include 17 or more anterior electrodes positionable proximate the anterior torso of the patient, and 39 or more posterior electrodes positionable proximate the posterior torso of the patient. In some examples, there may be about 25 electrodes **112** to about 256 electrodes **112** distributed around the torso of the patient **14**, though other configurations may have more or less electrodes **112**.

As described herein, the electrode apparatus **110** may be configured to measure electrical information (e.g., electrical signals) representing different regions of a patient's heart. For example, the electrical signals, or electrode signals, of different regions of a patient's heart can be approximated from surface electrocardiogram (ECG) signals measured using surface electrodes in proximity to surface areas corresponding to the different regions of the patient's heart.

As described herein, the exemplary systems, methods, and interfaces may be used to provide noninvasive assistance to a user in the evaluation of a patient's cardiac health or status, and/or the valuation of cardiac therapy (e.g., cardiac therapy being presently-delivered to a patient during implantation or after implantation). Further, the exemplary systems, methods, and interfaces may be used to assist a user in the configuration of the cardiac therapy being delivered to a patient. For instance, the exemplary systems, methods, and interfaces may be used to test a plurality of various cardiac therapy settings and present the results of the various cardiac therapy settings to a user via the graphical user interface. Further, for instance, the exemplary systems, methods, and interfaces may test a plurality of various cardiac therapy settings and present one or more effective cardiac therapy settings to the user. In at least one embodiment, the exem-

plary systems, methods, and interfaces may automatically program the cardiac therapy apparatus to use the effective cardiac therapy settings.

Exemplary method **200** depicted in FIG. **4A** may be used to determine typical cardiac cycles, or beats, and maximum QRS windows from a plurality of cardiac signals over a plurality of cardiac cycles. The exemplary method **200** may be generally described as being used in the evaluation of a patient's cardiac health and/or cardiac therapy being delivered to the patient. More specifically, the exemplary method **200** may be described as taking raw electrode signal data captured from a plurality of electrodes such as external, surface electrodes coupled to, or attached, to patient's skin, e.g., using the apparatus and systems described herein with respect to FIGS. **1-3**, and determining from the raw electrode signal data which of a plurality of cardiac cycles represent typical cardiac cycles, or beats, of a patient. Such typical cardiac cycles, or beats, may be useful in further analysis of the cardiac activity of the patient. In other words, the exemplary method **200** may be described as being a filter, or selection step, to determine what electrode signal data may be useful or helpful in the additional exemplary systems, methods, and interfaces described herein to assist in the evaluation of a patient's cardiac health and/or cardiac therapy being delivered to the patient.

Further, a typical cardiac cycle, or beat, may be described as being representative of a commonly occurring cardiac cycle of the patient so as to be useful or helpful in evaluating a patient's cardiac health and/or cardiac therapy being delivered to the patient. Since the exemplary method **200** may result in identification of one or more typical cardiac cycles, or beats, from a plurality of cardiac cycles, it may be described that some of the plurality of cardiac cycles were determined to be atypical or statistically not representative of a typical cardiac cycle of the patient so to be not useful or helpful in evaluating a patient's cardiac health and/or cardiac therapy being delivered to the patient.

The exemplary method **200** may include monitoring, or measuring, electrical activity using a plurality of electrodes **202** over a plurality of cardiac cycles or heart beats. As described herein, the plurality of electrodes may include external, surface electrodes coupled to, or attached, to patient's skin, e.g., using the apparatus and systems described herein with respect to FIGS. **1-3**. Additionally, although not further described herein with respect to the exemplary embodiments, the plurality of electrodes may include implantable electrodes implanted in one or more locations with a patient, e.g., using the apparatus and systems described herein with respect to FIGS. **9-11**. Still further, although not further described herein with respect to the exemplary embodiments, the plurality of electrodes may further include temporarily-implanted (e.g., non-permanent, not long term, etc.) electrodes such as, e.g., electrodes located in the cavity of a patient's heart using basket catheter or the like, electrodes located outside the heart but around the heart (e.g., epicardial space) using a "sock mapping" tool or the like. Yet still further, although not further described herein with respect to the exemplary embodiments, the electrodes, or electrode apparatus, may include a mix, or combination, of external and implanted electrodes. Regardless of the electrode apparatus utilized, the exemplary method **200** includes monitoring electrical activity **202**, and more specifically, cardiac signals or ECG signals, from at least two electrodes or channels.

Since the electrical activity is being monitored, or measured, **202** using a plurality of electrodes, the result may be a plurality of electrode signals from and affiliated, or cor-

responding to, such electrodes. For example, if the electrode apparatus includes 40 electrodes, the monitoring process 202 may result in 40 different electrode signals monitored over a plurality of cardiac cycles. Further, some electrodes may not provide a useful signal, e.g., if the electrode is not effectively in contact with the patient's tissue, the electrode is malfunctioning, etc., and it is to be understood that those such electrodes may be filtered out, or removed from, further consideration of the exemplary methods, systems, and interfaces described further herein.

Once the electrical activity has, or the electrode signals have, been captured (e.g., monitored, measured, recorded, etc.), the exemplary method 200 may identify a representative data slice, or electrode signal portion, of each of the plurality of electrode signals 204 that may be used to group the electrode signals 206. For example, a time period (e.g., window, slice, length, etc.) may be selected (e.g., automatically by the method, at least initially by a user, etc.), and each of the electrode signals may be "cut down" into an electrode signal slice, or portion, according to the selected time period. Generally, the selected time period may be described as an amount of time configured to capture a complete QRS complex (e.g., mainly non-isoelectric content), for example so as to be useful to compare one or more waveform features, or morphologies, of each electrode signal. For example, the selected time period, or slice, may be about 1000 milliseconds. Further, for example, the selected time period, or slice, may be greater than or equal to about 700 milliseconds, greater than or equal to about 800 milliseconds, greater than or equal to about 900 milliseconds, greater than or equal to about 950 milliseconds, etc. Further, for example, the selected time period, or slice, may be less than or equal to about 1300 milliseconds, less than or equal to about 1200 milliseconds, less than or equal to about 1100 milliseconds, less than or equal to about 1050 milliseconds, etc. Nonetheless, the selected time period used to identify the representative data slice 204 may be based on the patient's heart rate (e.g., paced heart rate or intrinsic heart rate). In at least one embodiment, the selected time period used to identify the representative data slice 204 may be selected, or picked, by a physician (e.g., who may review electrode signal data when making such selection). In at least one embodiment, the selected time period used to identify the representative data slice 204 may be selected, or determined, by an automated process executed by a computer processor or processing circuitry.

The exemplary method 200 may then attempt to group the electrode signal portions (e.g., within the slice, or time window, as previously identified 204) according to morphologic similarity into one or more morphologically similar groups, and create, or generate, one or more composite signal 206 from each of the morphologically similar groups. In other words, the morphology of a portion, or slice, of each of the electrode signals may be analyzed, the electrode signals may be grouped based on the morphology analysis, and then a composite signal for each different morphologically-similar group may be based on, or generated using, the entirety of each electrode signal of each different morphologically-similar group. Thus, each composite signal may be described as corresponding to a morphologically similar group of electrode signals (which are grouped based on a window, or slice, of each of the electrode signals).

For example, the morphology of each of the plurality of electrode signal portions may be compared to each other, and the electrode signal portions having similar morphology may be grouped. Each morphologically-similar group may then be used to generate the composite signal that, e.g., may

be representative of that particular morphologically similar group. In other words, the process 206 may result in one or more or a plurality of morphologically-similar groups, and (even though the grouping was based only on a data portion, or slice, of each electrode signal) the entire electrode signals of each of the morphologically-similar groups may be used to generate, or compute, a composite signal representative thereof. In at least one embodiment, the composite signal may be an average signal generated for each morphologically-similar group (e.g., based on each electrode signal of the morphologically similar group). In other embodiments, the composite signal may be a curve to fit the electrode signals of the morphologically similar group.

If no electrode signal portions or not enough electrode signal portions are morphologically similar so as to be grouped or too many morphologically distinct groups are identified in process 204, the method 200 may return to identifying a representative data slice 202 and changing the selected time period, or slice, to a different value than was previously used. For example, the previously-used selected time period, or slice, may be reduced or increased by a selected percentage or time value so as to reflect the most likely heart rate, or cardiac cycle length, for the patient. Then, the method 200 may again attempt to group the electrode signal portions according to morphologic similarity into one or more morphologically similar groups, and create, or generate, one or more composite signal 206 from each of the morphologically similar groups. In other words, the method 200 may re-slice the plurality of electrode signals using a different, or revised, time period 204 in response to unsuccessful grouping 206 of the plurality of electrode signal portions, and then re-try such grouping using the new data portion or slice 206. For example, if no groups are identified, a longer cycle length or slice may be used, and for example, if too many groups are identified (e.g., and if such groups include a small number of electrode signals), the shorter cycle length or slice may be used.

Thus, the processes 204 and 206 may result in a plurality of morphologically-similar groups of electrode signals and a plurality of composite signals corresponding to the morphologically similar groups. In one embodiment, an appropriate minimum peak height limit threshold may be determined 208 and set for each of the composite signals. The exemplary method 200 may then not analyze peaks or data below the minimum peak height limit threshold when determining peaks later thereon. In other words, the method 200 may simply not "look under" minimum peak height limit threshold within the duration of the composite signal.

The exemplary method 200 may then group morphologically similar peaks 210 that have features consistent with QRS complexes across two or more (e.g., all) composite signals. For example, one or more, or a plurality, of fiducial points, markers, or characteristics of the peaks in each composite signal may be compared to each other resulting in groups of morphologically similar peaks. In at least one embodiment, one or more of peak amplitude, width, and/or prevalence could be used to identify QRS-complexes associated peaks for each composite signal. Thus, the process 210 may be described as looking at all of the composite signals to identify groups of morphologically-similar peaks to be used to determine if each cardiac cycle, or beat, was present across all or more the composite signals.

From the groups of morphologically-similar peaks, the exemplary method 200 may further select typical cardiac cycles, or beats, 212 based at least on the comparison of peaks appearing in multiple composite signals. In other

words, typical cardiac cycles, or beats, may be selected **212** based on the groups of morphologically-similar peaks **210**.

After the selection of typical cardiac cycles, or beats, beat-to-beat spacing may be determined using one or more exemplary processes to select a QRS window. The maximum QRS window may be defined as a maximum time period within which the QRS complex of particular cardiac cycle occurs. The maximum QRS window determination, or calculation, may be configured so as to include at least the PQ and QT intervals of each cardiac cycle. Additionally, and more specifically, the exemplary method **200** may generate a maximum QRS window for each cardiac cycle, or beat, **214** based on the beat-to-beat interval and using various exemplary equations, or processes, relating heart rate to PQ and QT interval durations.

The exemplary method **200** may further include identifying additional, potentially atypical, cardiac cycles, or beats, **216**, which may be further analyzed if desired. For example, if gaps, or periods of time, longer than anticipated R-R intervals occur between identified typical beats, the exemplary method **200** may perform one or more similar or different processes as already performed on signal segments, or signal portions, that occur within such gaps. In one or more embodiments, different thresholds may be used when filtering **208** such atypical signal segments and/or grouping **210** the morphology of similar peaks in such atypical signal segments. In one or more embodiments, such identified additional cardiac cycles may be compared to one or more of the identified typical cardiac cycles to determine whether such additional cardiac cycles may be included in the result, or output, of method **200**.

The result of the exemplary method **200** may be a list of typical cardiac cycles, or beats, **218** and the corresponding maximum QRS complex windows **220** for each typical cardiac cycle, which may be used by the exemplary systems, methods, and interfaces described further herein.

An exemplary method **225** for determining various fiducial points within a QRS window of electrode signal including QRS onset and offset is depicted in FIG. 4B. The exemplary method **225** begins by providing a plurality of electrode signals, a list of typical cardiac cycles within the electrode signals, and a maximum QRS window for each of the typical cardiac cycles **227**. In at least one embodiment, such information may be provided by the exemplary method **200** of FIG. 4A.

The exemplary method **225** may then separate and group the plurality of electrode signals based on physical location of the electrode signal acquisition (e.g., location on the torso of the patient where each electrode is applied). As shown, such grouping may create at least one group of anterior signals **230** and at least one group of posterior signals **231** from the plurality of electrode signals. More specifically and as described herein with respect to the exemplary electrode apparatus of FIGS. 1-3, the one or more posterior sets of electrode signals may be monitored from one or more electrodes of the plurality of electrodes located proximate the patient's posterior and the one or more anterior sets of electrode signals may be monitored from one or more electrodes of the plurality of electrodes located proximate the patient's anterior.

Additionally, although not depicted in FIG. 4B, outlier signals may be removed, or filtered, from each group of the anterior and posterior signals by, for example, comparing the morphologic similarity of the electrode signals within each group. Thus, the group of anterior electrode signals may include electrode signals having morphologic similarity among their own anterior group and the group of posterior

electrode signals may include electrode signals having morphologic similarity among their own posterior group.

For each typical cardiac cycle **233** and for each electrode signal **235**, the exemplary method **225** may identify all of the peaks for each electrode signal within the maximum QRS window for the particular cardiac cycle **237**, and then identify a QRS onset time and a QRS offset time for each electrode signal within the maximum QRS window for the particular cardiac cycle **239**. The QRS onset times and QRS offset times may be determined using various fiducial points, various metrics, and the identified peaks. In at least one embodiment, QRS onset time may be determined using a derivative-based and/or amplitude-based cutoff preceding an initial peak within the maximum QRS window and QRS offset time may be determined using a derivative-based cutoff following a final peak within the maximum QRS window. In at least one embodiment, QRS onset time may be determined by a selected percentage change in area under the curve of the electrode signal and QRS offset time may be determined by a selected threshold of area remaining under the curve.

Thus, the result of processes **233**, **235**, **237**, **239** may be QRS onset and offset times for each cardiac cycle (e.g., each typical cardiac cycle) of each of the plurality of electrode signals. The exemplary method **225** may further include filtering the QRS onset and offset times **240** to, e.g., remove outliers. For example, the exemplary method **225** may determine a range of QRS onset and offset times for the posterior set of electrode signals and for the anterior set of electrode signals. In other words, a range of QRS onset times and a range of QRS offset times may be determined for the posterior set of electrodes, and likewise, a range of QRS onset times and a range of QRS offset times may be determined for the anterior set of electrodes. The range may be a selected period of time within which the most amount of QRS onset or offset times occur for the particular group of electrode signals. Any QRS onset and offset times for the particular group of electrode signals that fall outside (e.g., greater than or less than) of a selected range, or time window, may be removed.

For example, the selected range may be about 20 milliseconds. The 20-millisecond range may be positioned (e.g., slid along the X-axis or time) over a plurality of QRS onset or offset times for a particular set of electrode signals until the position is found that includes the greatest number of onset or offset times within the 20-millisecond range. The onset or offset times that occur later than or before the positioned 20 millisecond range may be removed. Further, for example, the selected range, or time window, may be greater than or equal to about 5 milliseconds, greater than or equal to about 10 milliseconds, greater than or equal to about 15 milliseconds, greater than or equal to about 20 milliseconds, etc. Further, for example, the selected range, or time window, may be less than or equal to about 40 milliseconds, less than or equal to about 30 milliseconds, less than or equal to about 25 milliseconds, etc.

The exemplary method **225** may then identify additional onset and offset time information **241** from the determined QRS onset and offset times such as, for example, a set QRS onset time and a set QRS offset time for each of the anterior set and posterior set of electrode signals (e.g., earliest QRS onset time within the set of electrode signals, latest QRS offset time within the set of electrode signals, etc.) and a global QRS onset time and a global QRS offset time for all of the electrode signals (e.g., earliest QRS onset time within the all of electrode signals, latest QRS offset time within the all of electrode signals, etc.). Further, a QRS duration, which

extends between an earliest QRS onset time and a latest QRS onset time may be determined for each set of electrode signals and all of the electrode signals. Thus, the method 225, as depicted, may result in an anterior QRS onset time, QRS offset time, and QRS duration 243, a posterior QRS onset time, QRS offset time, and QRS duration 245, and a global QRS onset time, QRS offset time, and QRS duration 247.

As described herein, the exemplary systems and methods may provide interfaces which may be used to display, or depict, various electrode signal information. An exemplary graphical user interface 300 depicting three single-cycle graphs 350 and corresponding electrical activation time maps 302 is depicted in FIG. 5. In at least one embodiment such as depicted, the corresponding electrical activation time maps 302 may be representative of average activation times from the three cardiac cycles shown on the three single-cycle graphs 350 (e.g., a three-beat average). It is to be understood that each of the single-cycle graphs 350 may depict less than an entire cardiac cycle, and for example, may depict the QRS complex portion of a cardiac cycle as depicted herein. Each of the single-cycle graphs 350 may depict, or include, a plurality of electrode signals 352 displayed over the same period of time for the same cardiac cycle or heart beat, which will be described further herein with respect to FIG. 6A. Nonetheless, generally, each of the single-cycle graphs 350 may depict each of an anterior set of electrode signals and a posterior set of electrode signals, and the anterior set of electrode signals may be graphically distinguishable from the posterior set of electrode signals as will be described further herein.

Three different single-cycle graphs 350 are depicted on the graphical user interface 300 of FIG. 5. Each of different single-cycle graphs 350 may correspond to a different cardiac cycle, or heart beat, of a single patient. The cardiac cycles may be selected using the exemplary method 200 described herein with respect to FIG. 4A, and may represent typical cardiac cycles of the patient that may be useful to assess the patient's cardiac health.

The graphical user interface 300 further includes a cardiac therapy indication 304, which, in this embodiment, is an alphanumeric depiction of the type, if any, of cardiac therapy being presently delivered to the patient. In this way, a practitioner may be able to quickly ascertain what, if any, cardiac therapy is being delivered to the patient. In this example, no cardiac therapy is being delivered to the patient, and thus, the cardiac therapy indication 304 includes the word "Intrinsic" to indicate that the patient is not receiving any cardiac therapy during the monitoring, or recording, of electrical activity (e.g., body-surface potentials) for analysis by the systems and methods described herein. Thus, the remainder of the information depicted on the graphical user interface 300 is reflective of the patient's intrinsic conduction and/or cardiac rhythm. In another example, the cardiac therapy indication 304 may include the words "A-V synchronous pacing" to indicate that the patient is receiving A-V synchronous pacing cardiac therapy.

Further, the graphical user interface 300 further includes one more metrics of electrical cardiac heterogeneity 306. In this embodiment, two metrics of electrical cardiac heterogeneity are depicted: namely, body surface activation duration (BSAd) and standard deviation of activation times (SDAT), each of which will be described further herein.

Still further, as described above, the graphical user interface 300 may include, or depict, one or more electrical activation maps 302. The electrical activation maps 302 may be maps, or plots, of body surface cardiac electrical activa-

tion as measured by the exemplary systems and methods described herein for one or more of the cardiac cycles depicted by the single-cycle graphs 350. The electrical activation maps 302 may indicate the electrical activation at various locations about the surface of the patient's body, which in turn, may be related to the epicardial surface of the patient's heart. As shown, the electrical activation maps 302 include an anterior map on the left of the graphical user interface 300 which corresponds to the anterior side of the patient (e.g., measured by the external surface electrodes positioned on the anterior torso of the patient), and a posterior map on the right of the graphical user interface 300 which corresponds to the posterior side of the patient (e.g., measured by the external surface electrodes positioned on the posterior torso of the patient). Further, in at least one embodiment each of the electrical activation maps 302 may represent an average of the three cardiac cycles depicted in the single-cycle graphs 350. In other embodiments, each of the electrical activation maps 302 may represent just one of the three cardiac cycles depicted in the single-cycle graphs 350 or a different composite value of more than one of the three cardiac cycles depicted in the single-cycle graphs 350.

Further, the electrical activation maps 302 may be described as being graphical representations of cardiac electrical activation times from the monitored electrical activity about a portion of human anatomy. In at least one embodiment, the cardiac electrical activation times may be represented about a portion of human anatomy by color scaling a portion of human anatomy on the graphical user interface 132 according to the body surface cardiac electrical activation times and/or surrogate cardiac electrical activation times. Additional exemplary graphical representations of body surface cardiac electrical activation times and/or surrogate electrical activation times that may utilize or be utilized by the exemplary systems and methods described herein may be described in U.S. Pat. No. 9,986,928 issued Jun. 5, 2018, U.S. Pat. No. 9,993,172 issued Jun. 12, 2018, U.S. Pat. No. 10,206,601 issued Feb. 19, 2019, and U.S. Pat. No. 9,591,982 issued Mar. 14, 2017, U.S. Pat. No. 8,972,228 issued Mar. 3, 2015 and entitled "Assessing Intra-Cardiac Activation Patterns" and U.S. Pat. No. 9,510,763 issued Dec. 6, 2016 and entitled "Assessing Intra-Cardiac Activation Patterns and Electrical Dyssynchrony," each of which is hereby incorporated by reference in its entirety.

A user may desire to know which of the plurality of electrode signals 352 depicted in the single-cycle graphs 350 corresponds to a specific location within the electrical activation maps 302. Thus, the exemplary graphical user interface 300 may allow a user to select (e.g., touch using a finger, click using a pointing device such as a mouse, etc.) any location, or area, of the electrical activation maps 302, and the electrode signal corresponding to the selected location, or area, (e.g., the electrode signal that is monitored closest to the selection) may be graphically emphasized among the plurality of electrode signals 352 on one or more of the single-cycle graphs 350 such that a practitioner may quickly ascertain (e.g., see or visualize) which of the plurality of electrode signals 352 on the single-cycle graphs 350 corresponds to the selected location, or area. For example, the corresponding electrode signal may change color, become highlighted, become animated (e.g., blink), etc. to indicate that it corresponds to the user selected location, or area, within the electrical activation maps 302. In other words, the corresponding electrode signal may be modified, or enhanced, to make it "stand out" among the plurality of electrode signals 352 of one or more single-cycle graphs 350.

Conversely, a user may desire to know where on the electrical activation maps 302 a particular electrode signal of the plurality of electrode signals 352 depicted in the single-cycle graphs 350 was derived, or measured, from. Thus, the exemplary graphical user interface 300 may allow a user to select (e.g., touch using a finger, click using a pointing device such as a mouse, etc.) any of the plurality of electrode signals 352 within the single-cycle graphs 350, and a location, or area, of the electrical activation maps 302 (e.g., the location or area where the electrode signal was obtained) may be graphically emphasized such that a practitioner may quickly ascertain (e.g., see or visualize) where on the electrical activation maps 304 the selected electrode signal corresponds to. For example, the corresponding location, or area, on the electrical activation maps 302 may change color, may be marked by a cross or circle, may become highlighted, may become animated (e.g., blink) to indicate that it corresponds to the selected electrode signal. In other words, the corresponding location, or area, of the electrical activations maps 302 may be modified, or enhanced, to make it “stand out.”

Exemplary single-cycle graphs 350, which may be used in or in conjunction to the graphical user interface of FIG. 5, depicting a plurality of electrode signals 352 are depicted in FIGS. 6A-6D. The single-cycle graphs 350 may include different sets, or groups, of electrode signals within the plurality of electrode signals 352 that are graphically distinguished from one another. In these examples (although not shown in the grayscale depictions), the anterior electrode signals 354 may be graphically distinguishable from the posterior electrode signals 356 by a change in color. In other words, the anterior electrode signals 354 may be a different color than the posterior electrode signals 356. For example, the anterior electrode signals 354 may be blue and the posterior electrode signals 356 may be green. In other embodiments, the anterior electrode signals 354 and the posterior electrode signals 356 may be graphically distinguishable from each other using different line weights, or widths, different line types such as, e.g., dashed lines, dotted lines, or wavy lines, different graphical animations such as blinking, flashing, twinkling, or highlighting, and/or different alphanumeric labeling.

Additionally, in one or more embodiments, each of the electrode signals within a graphical distinguished group, such as the anterior set of electrode signals 354, may be further graphically distinguished from the other electrode signals within the group based on various criteria such as, e.g., location. For example, a group, or set, of anterior electrode signals 352 may be graphically distinguished from the electrode signals 352 by being blue, and each of the anterior electrode signals 352 may be graphically distinguished from each other by being a different shade of blue. The shades of blue may be based on where the electrode signal was measured from about the patient's body. For example, anterior electrode signals 354 measured from electrodes proximate a right region of the patient's anterior torso may be darker than the anterior electrode signals 354 measured from electrodes proximate a left region of the patient's anterior torso. More specifically, the shades of blue of the anterior electrode signals 354 may range from darkest representing, or corresponding to, the right-most anterior electrode signals 354 to lightest representing, or corresponding to, the left-most anterior electrode signals 354. The graphical user interface 300 may further depict a color bar, or key, 303 for each of the anterior electrode signals 354 and the posterior electrode signals 352, which may be used by a user to determine where on the anterior and posterior each

electrode signal derives, or is measured, from. More specifically, as shown, the anterior color bar 303 extends from a dark end representing electrode signals measured from the right side of the anterior of the patient to a light end representing electrode signals measured from the left side of the anterior of the patient, and the posterior color bar 303 extends from a light end representing electrode signals measured from the left side of the posterior of the patient to a dark end representing electrode signals measured from the right side of the posterior of the patient.

In one or more embodiments, each of the electrode signals 352 may be a different color from each other and may correspond to an electrode map depicted on a graphical user interface (not shown) such that a user may ascertain where each of the electrode signals 352 was measured from by consulting the electrode map. For example, the electrode map may depict the electrodes positioned about a model of a patient's torso, and each of the electrodes may be a different color that corresponds to its electrode signal 352 depicted on the single-cycle graph 350.

As described herein, activation times (e.g., body surface cardiac activation times) may be determined for each of the plurality of electrode signals 352. The single-cycle graph 350 may include activation time indicators 358, a few of which are labeled in FIG. 6A, based on the determined activation time of each of the plurality of electrode signals 352. Although the activation time indicators 358 of the single-cycle graph 350 of FIGS. 6A-6D are shown as circles along each of the plurality of electrode signals 352, it is to be understood that the activation time indicators 358 may be graphically depicted, or indicated, in multiple different ways such as, e.g., crosses, tick marks, icons, squares, differently colored or otherwise graphically distinguished segments of the electrode signal, etc.

Additionally, a composite, or global, QRS onset time and a composite, or global, QRS offset time of the electrode signals 352 may be indicated, or shown, by composite, or global, QRS onset time indicators 360 (a few of which are labeled in FIG. 6A) and composite, or global, QRS offset time indicators 362 (a few of which are labeled in FIG. 6A) on one or more of the electrode signals 352 of the single-cycle graph 350. Similar to the activation time indicators 358, the composite QRS onset time indicators 360 and composite QRS offset time indicators 362 are shown as circles along each of the plurality of electrode signals 352, and also similar to the activation time indicators 358, it is contemplated that the composite QRS onset time indicators 360 and composite QRS offset time indicators 362 may be depicted in many different ways such as, e.g., crosses, tick marks, icons, squares, differently colored or otherwise graphically distinguished segments of the electrode signal, etc.

Further, the set QRS onset and offset time indicators may be indicated, or depicted, on the single-cycle graph 350. For example, a set QRS onset indicator and a set QRS offset time indicator may be displayed for each of the graphical distinguishable sets, or groups, of electrode signals 352. In this example, the single-cycle graph 350 includes an anterior set, or group, of electrode signals 354 and a posterior set, or group, of electrode signals 356, and thus, each of the anterior set 354 and the posterior set 356 may include a set QRS onset indicator and a set QRS offset time indicator. More specifically, an anterior set QRS onset time indicator 364, an anterior set QRS offset time indicator 366, a posterior set QRS onset time indicator 368, and a posterior set QRS offset time indicator 370 may be displayed. As shown, each of the set QRS onset and offset time indicators 364, 366, 368, 370

are solid vertical lines. In other embodiments, the set QRS onset and offset time indicators **364**, **366**, **368**, **370** may be any other graphical elements so to be able to be graphically distinguishable such that a user may determine that such indicators are indicative of the QRS onset and offset times for such sets, or groups, of electrode signals **352**. In this example, the anterior QRS onset and offset time indicators **364**, **366** may be the same color as the activation time indicators **358** of the anterior electrode signals **356** (e.g., orange), and the posterior QRS onset and offset time indicators **368**, **370** may be the same color as the activation time indicators **358** of the posterior electrode signals **356** (e.g., purple).

Still further, breakthrough times may be depicted, or indicated, on the single-cycle graph **350**. Breakthrough times may be described as the earliest activation time for a group, or set, of electrode signals **352**. In this example, an anterior breakthrough time indicator **372** is shown indicating the earliest activation of the plurality of anterior signals **356** and a posterior breakthrough time indicator **374** is shown indicating the earliest activation of the plurality of posterior signals **356**. As shown, the anterior and posterior breakthrough time indicators **372**, **374** are dashed vertical lines. In other embodiments, the anterior and posterior breakthrough time indicators **372**, **374** may be any other graphical elements so to be able to be graphically distinguishable such that a user may determine that such indicators are indicative of the breakthrough times for such sets, or groups, of electrode signals **352**. Yet still further, the latest activation time may also be indicated by a latest electrical activation time indicator **376**, which in this example is also a vertical dashed line but, in other embodiments, may be any suitable graphical indication.

From these various times and indicators displayed on the single-cycle graph **350**, various time intervals, or time durations, may be determined which may be useful in assisting a user in evaluating cardiac therapy settings, and/or in assisting a user in assessing a patient's cardiac health. For example and as depicted on the single-cycle graph **350** of FIG. **6A**, a global breakthrough duration, or time, **380** extending from earliest, or global, QRS onset time (as indicated by the earliest QRS onset time indicator **364**) to the earliest activation time (as indicated by the earliest activation time indicator **372**) may be determined. Further, for example, an anterior breakthrough duration, or time, may also be determined, which extends from earliest, or global, QRS onset time to the earliest anterior activation time may be determined. In this example, anterior breakthrough duration is the same as the global breakthrough duration **380**, and, thus not labeled as such. Additionally, for example, a posterior breakthrough duration, or time, **381** extending from earliest, or global, QRS onset time (as indicated by the earliest QRS onset time indicator **364**) to the earliest posterior activation time (as indicated by the earliest posterior activation time indicator **374**) may be determined as indicated on the single-cycle graph **350** of FIG. **6A**.

A global QRS duration **382** between the composite QRS onset time (as indicated by the earliest QRS onset time indicator **364**) and the composite QRS offset time (as indicated by the latest QRS offset time indicator **370**) may be determined as indicated on the single-cycle graph **350** of FIG. **6A**. Further, a QRS duration may be determined for each of the anterior set of electrode signals **354** and the posterior set of electrode signals **356**. For example, an anterior set QRS duration **383** between the anterior set QRS onset time (as indicated by the anterior QRS onset time indicator **364**) and the anterior set QRS offset time (as

indicated by the anterior QRS offset time indicator **366**) may be determined as indicated on the single-cycle graph **350** of FIG. **6A**. Further, for example, a posterior set QRS duration **384** between the posterior set QRS onset time (as indicated by the posterior QRS onset time indicator **368**) and the posterior set QRS offset time (as indicated by the posterior QRS offset time indicator **370**) may be determined as indicated on the single-cycle graph **350** of FIG. **6A**.

Further, for example, an intra-breakthrough time duration, or delay, **385** may be determined between the earliest anterior activation time (as indicated by the anterior breakthrough time indicator **372**) and the earliest posterior activation time (as indicated by the anterior breakthrough time indicator **374**) as indicated on the single-cycle graph **350** of FIG. **6A**. Still further, for example, an anterior-posterior QRS onset delay **386** may be determined between anterior and posterior QRS onset times (as indicated by the anterior and posterior onset time indicators **364**, **368**). And further, for example, an anterior-posterior QRS offset delay **387** may be determined between anterior and posterior QRS offset times (as indicated by the anterior and posterior offset time indicators **366**, **370**).

Still further, for example, an activation duration **388** may be determined between the earliest body surface activation time (as indicated by the earliest activation time indicator **372**) and the latest activation time (as indicated by the latest activation time indicator **376**) as indicated on the single-cycle graph **350** of FIG. **6A**. The activation time duration **388**, or body surface activation distance (BSAd), may be displayed on a graphical user interface proximate the single-cycle graph **350**, and for example, a BSAd of 95 milliseconds is depicted above the single-cycle graph **350** as shown in FIG. **6A**. Also, an activation duration to QRS end delay **389** may be determined between the latest activation time (as indicated by the latest activation time indicator **376**) and the latest QRS offset time (as indicated by the posterior offset time indicator **370**).

The exemplary single-cycle graph **350** is further depicted in FIGS. **6B-6D** for use when describing the generation, or determination, of various metrics of cardiac electrical heterogeneity from the plurality of electrode signals **352**. An exemplary method **250** comparing the morphology of anterior and posterior sets of electrode signals **354**, **356** for use with such metrics of cardiac electrical heterogeneity is depicted in FIG. **7**.

The exemplary method **250** includes monitoring electrical activity using the plurality of electrodes **252**, which may be similar to the monitoring and processes steps described herein with respect to methods **200**, **225** described herein with reference to FIGS. **4A-4B**. Regardless, the result of process **252** may be a plurality of electrode signals **352** over a single, typical cardiac cycle, which may be plotted, or depicted, on a single-cycle graph **350**.

The exemplary method **250** may then compare **254** the morphology of the anterior set of electrode signals **354** and the posterior set of electrode signals **356** to, e.g., assess the cardiac electrical heterogeneity of the patient. Generally, it may be described that if the posterior set of electrode signals **356** are "flipped," "squished," and "crunched" (in other words, "inverted," "compressed," and "reduced") to correspond to the anterior set of electrode signals **354**, then the cardiac electrical heterogeneity of the patient will have improved. Various metrics, or quantitative measures, may be reflective of the "flip," "squish," and "crunch" phenomenon. For example, changes in areas between the anterior and posterior waveforms, changes in distances between the anterior and posterior activation events, changes in body

surface activation duration (BSAd), changes in anterior and/or posterior amplitudes, changes in ratios of maximum amplitude to minimum amplitude, and/or a combination of changes in amplitudes and amplitude ratios may be indicative of the “flip,” “squish,” and “crunch” phenomenon, which may correlate to an improvement in the cardiac electrical heterogeneity of the patient.

Such comparison may be completed, or “take place,” automatically by a computing apparatus or partially by a computing apparatus with the assistance of a practitioner. For example, the computing apparatus may compare **254** the morphology of the anterior set of electrode signals **354** and the posterior set of electrode signals **356**, and output a result such as an indication of the cardiac electrical heterogeneity of the patient, which may indicate whether the patient’s cardiac health is acceptable and/or whether any presently-delivered cardiac therapy is effective. Further, for example, the computing apparatus may generate, or determine, and then display, or convey, one or more metrics of cardiac electrical heterogeneity that may be useful to a practitioner to determine the cardiac health of the patient and/or the effectiveness any presently-delivered cardiac therapy.

Cardiac electrical heterogeneity information and other cardiac therapy information may be described in U.S. Provisional Patent Application No. 61/834,133 entitled “METRICS OF ELECTRICAL DYSSYNCHRONY AND ELECTRICAL ACTIVATION PATTERNS FROM SURFACE ECG ELECTRODES” and filed on Jun. 12, 2013, which is hereby incorporated by reference in its entirety. Cardiac electrical heterogeneity information may be defined as information indicative of at least one of mechanical synchrony or dyssynchrony of the heart and/or electrical synchrony or dyssynchrony of the heart. In other words, cardiac electrical heterogeneity information may represent a surrogate of actual mechanical and/or electrical functionality. In at least one embodiment, the cardiac electrical heterogeneity information may include a standard deviation of ventricular activation times corresponding to some or all of the external electrodes, e.g., of the electrode apparatus **110**. Further, regional cardiac electrical heterogeneity information may include standard deviations and/or averages of activation times corresponding to electrodes located in certain anatomic areas of the torso. For example, external electrodes on the left side of the torso of a patient may be used to compute regional left electrical heterogeneity information.

The cardiac electrical heterogeneity information may be generated using one or more various systems and/or methods. Cardiac electrical heterogeneity information may be generated using an array, or a plurality, of surface electrodes and/or imaging systems as described in U.S. Pat. No. 9,510,763 issued Dec. 6, 2016 and entitled “ASSESSING INTRA-CARDIAC ACTIVATION PATTERNS AND ELECTRICAL DYSSYNCHRONY,” U.S. Pat. No. 8,972,228 issued Mar. 3, 2015 and entitled “ASSESSING INTRA-CARDIAC ACTIVATION PATTERNS”, and U.S. Pat. No. 8,180,428 B2 issued May 15, 2012 and entitled “METHODS AND SYSTEMS FOR USE IN SELECTING CARDIAC PACING SITES,” each of which is incorporated herein by reference in its entirety.

One exemplary metric of cardiac electrical heterogeneity may be a standard deviation of activation-times (SDAT) measured by some or all of the electrodes on the surface of the torso of patient. In some examples, the SDAT may be calculated using the estimated cardiac activation times over the surface of a model heart. Further, the metrics of cardiac electrical heterogeneity **351** may be displayed on a graphical user interface proximate the single-cycle graph **350**. For

example, the SDAT of 39.9 milliseconds is depicted above the single-cycle graph **350** as shown in FIG. 6A.

Another exemplary metric of cardiac electrical heterogeneity may be an inter-activation event distance. The inter-activation event distance may be a value derived from, or based, on activation distances between each of the plurality of activation times of the anterior electrode signals **354** and the plurality of activation times of the posterior electrode signals **356**. More specifically, an activation distance may be measured from each of the anterior activation times to each of the posterior activation times. Then, each of the activation distances may be used to generate an inter-activation event distance. For example, as shown in FIG. 6B, three activation distances **390** are depicted extending from a single anterior activation time indicator **358**. An Euclidean distance may be measured from that same single anterior activation time indicator **358** to each of the plurality of posterior activation time indicators **358**, and then the process may begin for the next anterior activation time indicator **358**. In this way, if there are 10 anterior electrode signals **354**, and thus, 10 anterior activation times, and 10 posterior electrode signals **356**, and thus, 10 posterior activation times, 100 activation time distances (10×10) may be determined. Further, it is to be understood that the activation time distances may be measured both in the X-axis and Y-axis directions in this embodiment, and as such, this metric may be useful for indicating whether the electrode signals **352** may be “flipped” and “squished” as will be further described herein. In other embodiment, the activation time distances may be only measured in one of the X-axis and Y-axis directions.

As noted earlier, the plurality of activation time distances may be used to generate, or determine, an inter-activation event distance. In one example, the plurality of activation time distances may be averaged to generate the inter-activation event distance.

In other words, the activation time distances **390** may be described as extending between each activation event of the anterior electrodes and each activation event of the posterior electrodes. The inter-activation event distance may be the average of all of the paired Euclidean activation time distances between each of the anterior activation events and each of the posterior activation events based on the electrogram plot.

Another exemplary metric of cardiac heterogeneity may be a composite area under the curve (AUC) metric based on of the areas under the curve of the anterior set of electrode signals and the areas under the curve of the posterior set of electrode signals. More specifically, an area under the curve **392** for each of the anterior electrode signals **354** and an area under the curve **394** for each of the posterior electrode signals **354** as depicted in FIG. 6C may be determined, or calculated. The areas under the curve for the anterior electrode signals **354** may then be compared to the areas under the curve for the posterior electrode signals **356** to generate the composite area under the curve (AUC) metric. In other words, a difference between the area under the curve **392** for each of the anterior electrode signals **354** and the area under the curve **394** for each of the posterior electrode signals **354** may be generated, or calculated, resulting in the composite AUC metric.

In at least one embodiment, each area under the curve for an anterior electrode signal **354** may be compared to each of the areas under the curve for the posterior electrode signal **354**. In this way, similar to the activation time distance metric, if there are 10 anterior electrode signals **354**, and thus, 10 anterior areas under curve, and 10 posterior electrode signals **356**, and thus, 10 posterior areas under curve,

100 area under curve metrics (10×10) may be determined by comparing the anterior electrode signals 354 to the posterior electrode signals 356.

In another embodiment, each anterior electrode signal 354 may be paired with only one posterior electrode signal 356, and their respective areas under curve may be compared. In this way, if there are 10 anterior electrode signals 354, and thus, 10 anterior areas under curve, and 10 posterior electrode signals 356, and thus, 10 posterior areas under curve, 10 pairs of signals may be compared resulting in 10 area under curve metrics. More specifically, the smallest area under the curve of the anterior electrode signals 354 may be compared to the smallest area under the curve of the posterior electrode signals 356, the second smallest area under the curve of the anterior electrode signals 354 may be compared to the second smallest area under the curve of the posterior electrode signals 356, and so on until areas under the curve of each pair of anterior and posterior signals 354, 356 is compared.

Then, a composite area under the curve metric may be determined based on the generated area under the curve metrics (e.g., based on each of the plurality of compared AUCs). In one example, the plurality of compared AUCs may be averaged to generate the composite area under the curve metric. It is to be understood, however, that any one more statistical computation may be used to generate the composite area under the curve metric from the plurality of compared AUCs. In other words, an average area between the anterior and posterior curves of the anterior and posterior electrode signals 354, 356 may be the average of all of the paired differences between each of the anterior curves and each of the posterior curves.

Another exemplary metric of cardiac heterogeneity may be a composite height metric based on the maximum heights of each of the anterior set of electrode signals 354 and the maximum heights of each of the posterior set of electrode signals 356. For example, the maximum heights of each of the plurality of electrode signals 352 may be determined, and then may be used to generate, or calculate, the composite height metric. More specifically, in one embodiment, the maximum height of the anterior electrode signals 354 may be compared to the minimum height of the anterior electrode signals 354 to provide a net maximum height of the anterior electrode signals 354 as indicated by the net anterior height 394 in FIG. 6D. Further, the maximum height of the posterior electrode signals 356 may be compared to the minimum height of the posterior electrode signals 356 to provide a net maximum height of the posterior electrode signals 356 as indicated by the net posterior height 396 in FIG. 6D. Then, a composite metric may be generated, or calculated, based the net maximum heights 394, 396 of the anterior and posterior electrode signals 354, 356. For example, the net direction of body surface cardiac electrical activity in the anterior-posterior plane may be determined using the average net posterior peak height minus the average anterior peak height.

Another exemplary metric of cardiac heterogeneity may be a ventricular electrical uncoupling (VEU) metric which may be a difference between the mean anterior and mean posterior activation times. The VEU may also be referred to as a body surface electrical uncoupling (BEU) since, e.g., the electrode signals may be captured from the body surface of the patient.

Thus, the method 250 may compare 254 the morphology of the anterior set of electrode signals 354 and the posterior set of electrode signals 356. The comparison 254 may provide one or more metrics of cardiac electrical heteroge-

neity, which may be used to assess the cardiac electrical heterogeneity of the patient. If the comparison 254 indicates that the patient's cardiac health may benefit from cardiac therapy or adjustment of the cardiac therapy being presently delivered, the method 250 may initiate or adjust cardiac therapy settings 256 and continue monitoring the electrical activity of the patient using the plurality of electrodes 252 and comparing the morphology of the anterior set of electrode signals 354 and the posterior set of electrode signals 356 to assess the newly-initiated cardiac therapy or newly-adjusted cardiac therapy.

The cardiac therapy may be adjusted, or modified, a plurality of different ways. For example, a pacing location may be changed (e.g., a pacing lead may be moved, different electrodes of a pacing lead may be used, a pacing vector may be changed, etc.). Further, for example, one or more timing intervals such as atrioventricular delay, intraventricular delay, etc. may be adjusted. Additionally, the type of cardiac therapy may also be adjusted. For instance, pacing therapy may be delivered as left-ventricle only pacing, biventricular pacing, multipoint pacing, etc., and each of the different types of pacing therapy may constitute an adjustment.

The method 250 may continue to adjust the cardiac therapy settings 256 until effective cardiac therapy (e.g., optimal cardiac therapy) is determined to be delivered 258 based on comparing 254 the morphology of the anterior set of electrode signals 354 and the posterior set of electrode signals 356. More specifically, the one or more metrics derived from the comparisons of the morphology of the anterior set of electrode signals 354 and the posterior set of electrode signals 356 may be used to determine whether the cardiac therapy being delivered at each of the adjusted cardiac therapy settings is effective. If the present cardiac therapy is determined to be ineffective (or less effective than optimal), the method 250 may return to adjusting the cardiac therapy settings 256. If the present cardiac therapy is determined to be effective (or more effective than other cardiac therapy settings) 260, the method 250 may display the effective cardiac therapy settings 262 to a practitioner, e.g., such that practitioner may program the cardiac therapy apparatus for the patient and/or may further evaluate the suggested effective cardiac therapy settings.

In one embodiment, the exemplary systems and methods may initiate cardiac therapy to a patient applying a plurality of different cardiac therapy settings over a plurality of cardiac cycles and display, on a graphical user interface, a plurality of single-cycle graphs 350 as shown on the graphical user interface 400 of FIG. 8A. As shown, each single-cycle graph 350 may correspond to a different cardiac cycle where different cardiac therapy settings are applied.

Further, the cardiac therapy settings (e.g., pacing settings) used for each of the plurality of single-cycle graphs 350 may be depicted proximate the corresponding single-cycle graphs 350. For example, the AV delay and VV delay are depicted above each of the single-cycle graphs 350 as shown in FIG. 8A.

The single-cycle graphs 350 may be deliberately arranged according to the cardiac therapy settings. For example, the single-cycle graphs 350 may be arranged in columns according to right ventricle pacing variations. As shown, the leftmost column may correspond to left ventricular pacing only and the right most column may correspond to a maximum intraventricular (VV) delay for biventricular pacing (which as shown in this example to be 50 milliseconds). The column immediately right of the left ventricular pacing only column may correspond to the first biventricular pacing settings where the VV delay is 0 milliseconds. For example,

the single-cycle graphs 350 may be arranged in rows according to left ventricle pacing variations. As shown, the top row may correspond to a minimum atrioventricular (AV) delay of 80 milliseconds and the bottom row may correspond to a maximum AV delay of 140 milliseconds.

Additionally, the graphical user interface 400 may further depict a single-cycle graph of typical cardiac cycle of the patient during intrinsic rhythm, which in this example, is depicted in the upper right corner.

A practitioner may be to view, or look at, the graphical user interface 400 and ascertain which of the plurality of various cardiac therapy settings results in improvement of cardiac electrical heterogeneity of the patient by comparing the single-cycle graphs. More specifically, for example, the single-cycle graphs that show an effective amount of “flipping,” “squishing,” and “crunching” may be determined to provide an improvement of cardiac electrical heterogeneity of the patient.

Although not depicted in FIG. 8A, one or more metrics of cardiac electrical heterogeneity including those derived from, or based on, comparisons of the anterior electrode signals 354 and the posterior electrode signals 356 may be depicted proximate each of the single-cycle graphs 350. For example, an enlarged view of a portion 402 of the graphical user interface 400 of FIG. 8A is depicted in FIG. 8B, which includes one or more metrics of cardiac electrical heterogeneity proximate each of the single-cycle graphs 350. As shown, the one or more metrics of cardiac electrical heterogeneity in this example are SDAT, QRSd, and VAd. It is to be understood that any other of the metrics of cardiac electrical heterogeneity described herein may be displayed proximate each of the single-cycle graphs 350 of the graphical user interface 400. Further, although not depicted herein, percentage improvements and other statistical values may be presented proximate each of the single-cycle graphs 350 so as to provide additional use information to practitioners.

Lastly, in at least one embodiment, single-cycle graph 350 corresponding to the determined most effective cardiac therapy settings may be indicated (e.g., highlighted, circle, animated, etc.) on the graphical user interface 400. In this way, a practitioner may be able to view the systems recommended cardiac settings in view of the other different cardiac settings.

Exemplary cardiac therapy may be further described herein with reference to FIGS. 9-11, which may be adjusted using the exemplary method 250. Additionally, the exemplary systems and methods described herein may further use or incorporate the systems and methods described in U.S. Pat. No. 9,764,143 issued Sep. 19, 2017, U.S. Pat. No. 9,586,050 issued Mar. 7, 2017, U.S. Pat. No. 9,586,052 issued Mar. 7, 2017, all of which are incorporated herein by reference in their entireties.

The exemplary systems, methods, and graphical user interfaces described herein may be used with respect to the implantation and configuration of an implantable medical device (IMD) and/or one or more leads configured to be located proximate one or more portions of a patient’s heart. For example, the exemplary systems, methods, and interfaces may be used in conjunction with an exemplary therapy system 10 described herein with reference to FIGS. 9-11.

FIG. 9 is a conceptual diagram illustrating an exemplary therapy system 10 that may be used to deliver pacing therapy to a patient 14. Patient 14 may, but not necessarily, be a human. The therapy system 10 may include an implantable medical device 16 (IMD), which may be coupled to leads 18, 20, 22. The IMD 16 may be, e.g., an implantable pacemaker, cardioverter, and/or defibrillator, that delivers, or provides,

electrical signals (e.g., paces, etc.) to and/or senses electrical signals from the heart 12 of the patient 14 via electrodes coupled to one or more of the leads 18, 20, 22.

The leads 18, 20, 22 extend into the heart 12 of the patient 14 to sense electrical activity of the heart 12 and/or to deliver electrical stimulation to the heart 12. In the example shown in FIG. 9, the right ventricular (RV) lead 18 extends through one or more veins (not shown), the superior vena cava (not shown), and the right atrium 26, and into the right ventricle 28. The left ventricular (LV) coronary sinus lead 20 extends through one or more veins, the vena cava, the right atrium 26, and into the coronary sinus 30 to a region adjacent to the free wall of the left ventricle 32 of the heart 12. The right atrial (RA) lead 22 extends through one or more veins and the vena cava, and into the right atrium 26 of the heart 12.

The IMD 16 may sense, among other things, electrical signals attendant to the depolarization and repolarization of the heart 12 via electrodes coupled to at least one of the leads 18, 20, 22. In some examples, the IMD 16 provides pacing therapy (e.g., pacing pulses) to the heart 12 based on the electrical signals sensed within the heart 12. The IMD 16 may be operable to adjust one or more parameters associated with the pacing therapy such as, e.g., AV delay and other various timings, pulse wide, amplitude, voltage, burst length, etc. Further, the IMD 16 may be operable to use various electrode configurations to deliver pacing therapy, which may be unipolar, bipolar, quadripolar, or further multipolar. For example, a multipolar lead may include several electrodes that can be used for delivering pacing therapy. Hence, a multipolar lead system may provide, or offer, multiple electrical vectors to pace from. A pacing vector may include at least one cathode, which may be at least one electrode located on at least one lead, and at least one anode, which may be at least one electrode located on at least one lead (e.g., the same lead, or a different lead) and/or on the casing, or can, of the IMD 16. While improvement in cardiac function as a result of the pacing therapy may primarily depend on the cathode, the electrical parameters like impedance, pacing threshold voltage, current drain, longevity, etc. may be more dependent on the pacing vector, which includes both the cathode and the anode. The IMD 16 may also provide defibrillation therapy and/or cardioversion therapy via electrodes located on at least one of the leads 18, 20, 22. Further, the IMD 16 may detect arrhythmia of the heart 12, such as fibrillation of the ventricles 28, 32, and deliver defibrillation therapy to the heart 12 in the form of electrical pulses. In some examples, IMD 16 may be programmed to deliver a progression of therapies, e.g., pulses with increasing energy levels, until a fibrillation of heart 12 is stopped.

FIGS. 10A-10B are conceptual diagrams illustrating the IMD 16 and the leads 18, 20, 22 of therapy system 10 of FIG. 9 in more detail. The leads 18, 20, 22 may be electrically coupled to a therapy delivery module (e.g., for delivery of pacing therapy), a sensing module (e.g., for sensing one or more signals from one or more electrodes), and/or any other modules of the IMD 16 via a connector block 34. In some examples, the proximal ends of the leads 18, 20, 22 may include electrical contacts that electrically couple to respective electrical contacts within the connector block 34 of the IMD 16. In addition, in some examples, the leads 18, 20, 22 may be mechanically coupled to the connector block 34 with the aid of set screws, connection pins, or another suitable mechanical coupling mechanism.

Each of the leads 18, 20, 22 includes an elongated insulative lead body, which may carry a number of conductors (e.g., concentric coiled conductors, straight conductors,

etc.) separated from one another by insulation (e.g., tubular insulative sheaths). In the illustrated example, bipolar electrodes **40**, **42** are located proximate to a distal end of the lead **18**. In addition, bipolar electrodes **44**, **45**, **46**, **47** are located proximate to a distal end of the lead **20** and bipolar electrodes **48**, **50** are located proximate to a distal end of the lead **22**.

The electrodes **40**, **44**, **45**, **46**, **47**, **48** may take the form of ring electrodes, and the electrodes **42**, **50** may take the form of extendable helix tip electrodes mounted retractably within the insulative electrode heads **52**, **54**, **56**, respectively. Each of the electrodes **40**, **42**, **44**, **45**, **46**, **47**, **48**, **50** may be electrically coupled to a respective one of the conductors (e.g., coiled and/or straight) within the lead body of its associated lead **18**, **20**, **22**, and thereby coupled to a respective one of the electrical contacts on the proximal end of the leads **18**, **20**, **22**.

Additionally, electrodes **44**, **45**, **46** and **47** may have an electrode surface area of about 5.3 mm<sup>2</sup> to about 5.8 mm<sup>2</sup>. Electrodes **44**, **45**, **46**, and **47** may also be referred to as LV1, LV2, LV3, and LV4, respectively. The LV electrodes (i.e., left ventricle electrode 1 (LV1) **44**, left ventricle electrode 2 (LV2) **45**, left ventricle electrode 3 (LV3) **46**, and left ventricle 4 (LV4) **47** etc.) on the lead **20** can be spaced apart at variable distances. For example, electrode **44** may be a distance of, e.g., about 21 millimeters (mm), away from electrode **45**, electrodes **45** and **46** may be spaced a distance of, e.g. about 1.3 mm to about 1.5 mm, away from each other, and electrodes **46** and **47** may be spaced a distance of, e.g. 20 mm to about 21 mm, away from each other.

The electrodes **40**, **42**, **44**, **45**, **46**, **47**, **48**, **50** may further be used to sense electrical signals (e.g., morphological waveforms within electrograms (EGM)) attendant to the depolarization and repolarization of the heart **12**. The electrical signals are conducted to the IMD **16** via the respective leads **18**, **20**, **22**. In some examples, the IMD **16** may also deliver pacing pulses via the electrodes **40**, **42**, **44**, **45**, **46**, **47**, **48**, **50** to cause depolarization of cardiac tissue of the patient's heart **12**. In some examples, as illustrated in FIG. **10A**, the IMD **16** includes one or more housing electrodes, such as housing electrode **58**, which may be formed integrally with an outer surface of a housing **60** (e.g., hermetically-sealed housing) of the IMD **16** or otherwise coupled to the housing **60**. Any of the electrodes **40**, **42**, **44**, **45**, **46**, **47**, **48**, **50** may be used for unipolar sensing or pacing in combination with the housing electrode **58**. It is generally understood by those skilled in the art that other electrodes can also be selected to define, or be used for, pacing and sensing vectors. Further, any of electrodes **40**, **42**, **44**, **45**, **46**, **47**, **48**, **50**, **58**, when not being used to deliver pacing therapy, may be used to sense electrical activity during pacing therapy.

As described in further detail with reference to FIG. **10A**, the housing **60** may enclose a therapy delivery module that may include a stimulation generator for generating cardiac pacing pulses and defibrillation or cardioversion shocks, as well as a sensing module for monitoring the electrical signals of the patient's heart (e.g., the patient's heart rhythm). The leads **18**, **20**, **22** may also include elongated electrodes **62**, **64**, **66**, respectively, which may take the form of a coil. The IMD **16** may deliver defibrillation shocks to the heart **12** via any combination of the elongated electrodes **62**, **64**, **66** and the housing electrode **58**. The electrodes **58**, **62**, **64**, **66** may also be used to deliver cardioversion pulses to the heart **12**. Further, the electrodes **62**, **64**, **66** may be fabricated from any suitable electrically conductive material, such as, but not limited to, platinum, platinum alloy,

and/or other materials known to be usable in implantable defibrillation electrodes. Since electrodes **62**, **64**, **66** are not generally configured to deliver pacing therapy, any of electrodes **62**, **64**, **66** may be used to sense electrical activity and may be used in combination with any of electrodes **40**, **42**, **44**, **45**, **46**, **47**, **48**, **50**, **58**. In at least one embodiment, the RV elongated electrode **62** may be used to sense electrical activity of a patient's heart during the delivery of pacing therapy (e.g., in combination with the housing electrode **58**, or defibrillation electrode-to-housing electrode vector).

The configuration of the exemplary therapy system **10** illustrated in FIGS. **9-11** is merely one example. In other examples, the therapy system may include epicardial leads and/or patch electrodes instead of or in addition to the transvenous leads **18**, **20**, **22** illustrated in FIG. **9**. Additionally, in other examples, the therapy system **10** may be implanted in/around the cardiac space without transvenous leads (e.g., leadless/wireless pacing systems) or with leads implanted (e.g., implanted transvenously or using approaches) into the left chambers of the heart (in addition to or replacing the transvenous leads placed into the right chambers of the heart as illustrated in FIG. **9**). Further, in one or more embodiments, the IMD **16** need not be implanted within the patient **14**. For example, the IMD **16** may deliver various cardiac therapies to the heart **12** via percutaneous leads that extend through the skin of the patient **14** to a variety of positions within or outside of the heart **12**. In one or more embodiments, the system **10** may utilize wireless pacing (e.g., using energy transmission to the intracardiac pacing component(s) via ultrasound, inductive coupling, RF, etc.) and sensing cardiac activation using electrodes on the can/housing and/or on subcutaneous leads.

In other examples of therapy systems that provide electrical stimulation therapy to the heart **12**, such therapy systems may include any suitable number of leads coupled to the IMD **16**, and each of the leads may extend to any location within or proximate to the heart **12**. For example, other examples of therapy systems may include three transvenous leads located as illustrated in FIGS. **9-11**. Still further, other therapy systems may include a single lead that extends from the IMD **16** into the right atrium **26** or the right ventricle **28**, or two leads that extend into a respective one of the right atrium **26** and the right ventricle **28**.

FIG. **11A** is a functional block diagram of one exemplary configuration of the IMD **16**. As shown, the IMD **16** may include a control module **81**, a therapy delivery module **84** (e.g., which may include a stimulation generator), a sensing module **86**, and a power source **90**.

The control module **81** may include a processor **80**, memory **82**, and a telemetry module **88**. The memory **82** may include computer-readable instructions that, when executed, e.g., by the processor **80**, cause the IMD **16** and/or the control module **81** to perform various functions attributed to the IMD **16** and/or the control module **81** described herein. Further, the memory **82** may include any volatile, non-volatile, magnetic, optical, and/or electrical media, such as a random-access memory (RAM), read-only memory (ROM), non-volatile RAM (NVRAM), electrically-erasable programmable ROM (EEPROM), flash memory, and/or any other digital media. An exemplary capture management module may be the left ventricular capture management (LVCM) module described in U.S. Pat. No. 7,684,863 entitled "LV THRESHOLD MEASUREMENT AND CAPTURE MANAGEMENT" and issued Mar. 23, 2010, which is incorporated herein by reference in its entirety.

The processor, or processing circuitry, **80** of the control module **81** may include any one or more of a microproces-

sor, a controller, a digital signal processor (DSP), an application specific integrated circuit (ASIC), a field-programmable gate array (FPGA), and/or equivalent discrete or integrated logic circuitry. In some examples, the processor, or processing circuitry, **80** may include multiple components, such as any combination of one or more microprocessors, one or more controllers, one or more DSPs, one or more ASICs, and/or one or more FPGAs, as well as other discrete or integrated logic circuitry. The functions attributed to the processor **80** herein may be embodied as software, firmware, hardware, or any combination thereof.

The control module **81** may control the therapy delivery module **84** to deliver therapy (e.g., electrical stimulation therapy such as pacing) to the heart **12** according to a selected one or more therapy programs, which may be stored in the memory **82**. More, specifically, the control module **81** (e.g., the processor **80**) may control various parameters of the electrical stimulus delivered by the therapy delivery module **84** such as, e.g., AV delays, VV delays, pacing pulses with the amplitudes, pulse widths, frequency, or electrode polarities, etc., which may be specified by one or more selected therapy programs (e.g., AV and/or VV delay adjustment programs, pacing therapy programs, pacing recovery programs, capture management programs, etc.). As shown, the therapy delivery module **84** is electrically coupled to electrodes **40, 42, 44, 45, 46, 47, 48, 50, 58, 62, 64, 66**, e.g., via conductors of the respective lead **18, 20, 22**, or, in the case of housing electrode **58**, via an electrical conductor disposed within housing **60** of IMD **16**. Therapy delivery module **84** may be configured to generate and deliver electrical stimulation therapy such as pacing therapy to the heart **12** using one or more of the electrodes **40, 42, 44, 45, 46, 47, 48, 50, 58, 62, 64, 66**.

For example, therapy delivery module **84** may deliver pacing stimulus (e.g., pacing pulses) via ring electrodes **40, 44, 45, 46, 47, 48** coupled to leads **18, 20, 22** and/or helical tip electrodes **42, 50** of leads **18, 22**. Further, for example, therapy delivery module **84** may deliver defibrillation shocks to heart **12** via at least two of electrodes **58, 62, 64, 66**. In some examples, therapy delivery module **84** may be configured to deliver pacing, cardioversion, or defibrillation stimulation in the form of electrical pulses. In other examples, therapy delivery module **84** may be configured to deliver one or more of these types of stimulation in the form of other signals, such as sine waves, square waves, and/or other substantially continuous time signals.

The IMD **16** may further include a switch module **85** and the control module **81** (e.g., the processor **80**) may use the switch module **85** to select, e.g., via a data/address bus, which of the available electrodes are used to deliver therapy such as pacing pulses for pacing therapy, or which of the available electrodes are used for sensing. The switch module **85** may include a switch array, switch matrix, multiplexer, or any other type of switching device suitable to selectively couple the sensing module **86** and/or the therapy delivery module **84** to one or more selected electrodes. More specifically, the therapy delivery module **84** may include a plurality of pacing output circuits. Each pacing output circuit of the plurality of pacing output circuits may be selectively coupled, e.g., using the switch module **85**, to one or more of the electrodes **40, 42, 44, 45, 46, 47, 48, 50, 58, 62, 64, 66** (e.g., a pair of electrodes for delivery of therapy to a bipolar or multipolar pacing vector). In other words, each electrode can be selectively coupled to one of the pacing output circuits of the therapy delivery module using the switching module **85**.

The sensing module **86** is coupled (e.g., electrically coupled) to sensing apparatus, which may include, among additional sensing apparatus, the electrodes **40, 42, 44, 45, 46, 47, 48, 50, 58, 62, 64, 66** to monitor electrical activity of the heart **12**, e.g., electrocardiogram (ECG)/electrogram (EGM) signals, etc. The ECG/EGM signals may be used to measure or monitor activation times (e.g., ventricular activations times, etc.), heart rate (HR), heart rate variability (HRV), heart rate turbulence (HRT), deceleration/acceleration capacity, deceleration sequence incidence, T-wave alternans (TWA), P-wave to P-wave intervals (also referred to as the P-P intervals or A-A intervals), R-wave to R-wave intervals (also referred to as the R-R intervals or V-V intervals), P-wave to QRS complex intervals (also referred to as the P-R intervals, A-V intervals, or P-Q intervals), QRS-complex morphology, ST segment (i.e., the segment that connects the QRS complex and the T-wave), T-wave changes, QT intervals, electrical vectors, etc.

The switch module **85** may also be used with the sensing module **86** to select which of the available electrodes are used, or enabled, to, e.g., sense electrical activity of the patient's heart (e.g., one or more electrical vectors of the patient's heart using any combination of the electrodes **40, 42, 44, 45, 46, 47, 48, 50, 58, 62, 64, 66**). Likewise, the switch module **85** may also be used with the sensing module **86** to select which of the available electrodes are not to be used (e.g., disabled) to, e.g., sense electrical activity of the patient's heart (e.g., one or more electrical vectors of the patient's heart using any combination of the electrodes **40, 42, 44, 45, 46, 47, 48, 50, 58, 62, 64, 66**), etc. In some examples, the control module **81** may select the electrodes that function as sensing electrodes via the switch module within the sensing module **86**, e.g., by providing signals via a data/address bus.

In some examples, sensing module **86** includes a channel that includes an amplifier with a relatively wider pass band than the R-wave or P-wave amplifiers. Signals from the selected sensing electrodes may be provided to a multiplexer, and thereafter converted to multi-bit digital signals by an analog-to-digital converter for storage in memory **82**, e.g., as an electrogram (EGM). In some examples, the storage of such EGMs in memory **82** may be under the control of a direct memory access circuit.

In some examples, the control module **81** may operate as an interrupt driven device, and may be responsive to interrupts from pacer timing and control module, where the interrupts may correspond to the occurrences of sensed P-waves and R-waves and the generation of cardiac pacing pulses. Any necessary mathematical calculations may be performed by the processor **80** and any updating of the values or intervals controlled by the pacer timing and control module may take place following such interrupts. A portion of memory **82** may be configured as a plurality of recirculating buffers, capable of holding one or more series of measured intervals, which may be analyzed by, e.g., the processor **80** in response to the occurrence of a pace or sense interrupt to determine whether the patient's heart **12** is presently exhibiting atrial or ventricular tachyarrhythmia.

The telemetry module **88** of the control module **81** may include any suitable hardware, firmware, software, or any combination thereof for communicating with another device, such as a programmer. For example, under the control of the processor **80**, the telemetry module **88** may receive downlink telemetry from and send uplink telemetry to a programmer with the aid of an antenna, which may be internal and/or external. The processor **80** may provide the data to be uplinked to a programmer and the control signals

for the telemetry circuit within the telemetry module **88**, e.g., via an address/data bus. In some examples, the telemetry module **88** may provide received data to the processor **80** via a multiplexer.

The various components of the IMD **16** are further coupled to a power source **90**, which may include a rechargeable or non-rechargeable battery. A non-rechargeable battery may be selected to last for several years, while a rechargeable battery may be inductively charged from an external device, e.g., on a daily or weekly basis.

FIG. 11B is another embodiment of a functional block diagram for IMD **16** that depicts bipolar RA lead **22**, bipolar RV lead **18**, and bipolar LV CS lead **20** without the LA CS pace/sense electrodes and coupled with an implantable pulse generator (IPG) circuit **31** having programmable modes and parameters of a biventricular DDD/R type known in the pacing art. In turn, the sensor signal processing circuit **91** indirectly couples to the timing circuit **43** and via data and control bus to microcomputer circuitry **33**. The IPG circuit **31** is illustrated in a functional block diagram divided generally into a microcomputer circuit **33** and a pacing circuit **21**. The pacing circuit **21** includes the digital controller/timer circuit **43**, the output amplifiers circuit **51**, the sense amplifiers circuit **55**, the RF telemetry transceiver **41**, the activity sensor circuit **35** as well as a number of other circuits and components described below.

Crystal oscillator circuit **89** provides the basic timing clock for the pacing circuit **21** while battery **29** provides power. Power-on-reset circuit **87** responds to initial connection of the circuit to the battery for defining an initial operating condition and similarly, resets the operative state of the device in response to detection of a low battery condition. Reference mode circuit **37** generates stable voltage reference and currents for the analog circuits within the pacing circuit **21**. Analog-to-digital converter (ADC) and multiplexer circuit **39** digitize analog signals and voltage to provide, e.g., real time telemetry of cardiac signals from sense amplifiers **55** for uplink transmission via RF transmitter and receiver circuit **41**. Voltage reference and bias circuit **37**, ADC and multiplexer **39**, power-on-reset circuit **87**, and crystal oscillator circuit **89** may correspond to any of those used in exemplary implantable cardiac pacemakers.

If the IPG is programmed to a rate responsive mode, the signals output by one or more physiologic sensors are employed as a rate control parameter (RCP) to derive a physiologic escape interval. For example, the escape interval is adjusted proportionally to the patient's activity level developed in the patient activity sensor (PAS) circuit **35** in the depicted, exemplary IPG circuit **31**. The patient activity sensor **27** is coupled to the IPG housing and may take the form of a piezoelectric crystal transducer. The output signal of the patient activity sensor **27** may be processed and used as a RCP. Sensor **27** generates electrical signals in response to sensed physical activity that are processed by activity circuit **35** and provided to digital controller/timer circuit **43**. Activity circuit **35** and associated sensor **27** may correspond to the circuitry disclosed in U.S. Pat. No. 5,052,388 entitled "METHOD AND APPARATUS FOR IMPLEMENTING ACTIVITY SENSING IN A PULSE GENERATOR" and issued on Oct. 1, 1991 and U.S. Pat. No. 4,428,378 entitled "RATE ADAPTIVE PACER" and issued on Jan. 31, 1984, each of which is incorporated herein by reference in its entirety. Similarly, the exemplary systems, apparatus, and methods described herein may be practiced in conjunction with alternate types of sensors such as oxygenation sensors, pressure sensors, pH sensors, and respiration sensors, for use in providing rate responsive pacing capabilities. Alternately,

QT time may be used as a rate indicating parameter, in which case no extra sensor is required. Similarly, the exemplary embodiments described herein may also be practiced in non-rate responsive pacemakers.

Data transmission to and from the external programmer is accomplished by way of the telemetry antenna **57** and an associated RF transceiver **41**, which serves both to demodulate received downlink telemetry and to transmit uplink telemetry. Uplink telemetry capabilities may include the ability to transmit stored digital information, e.g., operating modes and parameters, EGM histograms, and other events, as well as real time EGMs of atrial and/or ventricular electrical activity and marker channel pulses indicating the occurrence of sensed and paced depolarizations in the atrium and ventricle.

Microcomputer **33** contains a microprocessor **80** and associated system clock and on-processor RAM and ROM chips **82A** and **82B**, respectively. In addition, microcomputer circuit **33** includes a separate RAM/ROM chip **82C** to provide additional memory capacity. Microprocessor **80** normally operates in a reduced power consumption mode and is interrupt driven. Microprocessor **80** is awakened in response to defined interrupt events, which may include A-TRIG, RV-TRIG, LV-TRIG signals generated by timers in digital timer/controller circuit **43** and A-EVENT, RV-EVENT, and LV-EVENT signals generated by sense amplifiers circuit **55**, among others. The specific values of the intervals and delays timed out by digital controller/timer circuit **43** are controlled by the microcomputer circuit **33** by way of data and control bus from programmed-in parameter values and operating modes. In addition, if programmed to operate as a rate responsive pacemaker, a timed interrupt, e.g., every cycle or every two seconds, may be provided in order to allow the microprocessor to analyze the activity sensor data and update the basic A-A, V-A, or V-V escape interval, as applicable. In addition, the microprocessor **80** may also serve to define variable, operative AV delay intervals, V-V delay intervals, and the energy delivered to each ventricle and/or atrium.

In one embodiment, microprocessor **80** is a custom microprocessor adapted to fetch and execute instructions stored in RAM/ROM unit **82** in a conventional manner. It is contemplated, however, that other implementations may be suitable to practice the present invention. For example, an off-the-shelf, commercially available microprocessor or microcontroller, or custom application-specific, hardwired logic, or state-machine type circuit may perform the functions of microprocessor **80**.

Digital controller/timer circuit **43** operates under the general control of the microcomputer **33** to control timing and other functions within the pacing circuit **21** and includes a set of timing and associated logic circuits of which certain ones pertinent to the present invention are depicted. The depicted timing circuits include URI/LRI timers **83A**, V-V delay timer **83B**, intrinsic interval timers **83C** for timing elapsed V-EVENT to V-EVENT intervals or V-EVENT to A-EVENT intervals or the V-V conduction interval, escape interval timers **83D** for timing A-A, V-A, and/or V-V pacing escape intervals, an AV delay interval timer **83E** for timing the A-LVp delay (or A-RVp delay) from a preceding A-EVENT or A-TRIG, a post-ventricular timer **83F** for timing post-ventricular time periods, and a date/time clock **83G**.

The AV delay interval timer **83E** is loaded with an appropriate delay interval for one ventricular chamber (e.g., either an A-RVp delay or an A-LVp) to time-out starting from a preceding A-PACE or A-EVENT. The interval timer

**83E** triggers pacing stimulus delivery, and can be based on one or more prior cardiac cycles (or from a data set empirically derived for a given patient).

The post-event timer **83F** times out the post-ventricular time period following an RV-EVENT or LV-EVENT or a RV-TRIG or LV-TRIG and post-atrial time periods following an A-EVENT or A-TRIG. The durations of the post-event time periods may also be selected as programmable parameters stored in the microcomputer **33**. The post-ventricular time periods include the PVARP, a post-atrial ventricular blanking period (PAVBP), a ventricular blanking period (VBP), a post-ventricular atrial blanking period (PVARP) and a ventricular refractory period (VRP) although other periods can be suitably defined depending, at least in part, on the operative circuitry employed in the pacing engine. The post-atrial time periods include an atrial refractory period (ARP) during which an A-EVENT is ignored for the purpose of resetting any AV delay, and an atrial blanking period (ABP) during which atrial sensing is disabled. It should be noted that the starting of the post-atrial time periods and the AV delays can be commenced substantially simultaneously with the start or end of each A-EVENT or A-TRIG or, in the latter case, upon the end of the A-PACE which may follow the A-TRIG. Similarly, the starting of the post-ventricular time periods and the V-A escape interval can be commenced substantially simultaneously with the start or end of the V-EVENT or V-TRIG or, in the latter case, upon the end of the V-PACE which may follow the V-TRIG. The microprocessor **80** also optionally calculates AV delays, VV delays, post-ventricular time periods, and post-atrial time periods that vary with the sensor based escape interval established in response to the RCP(s) and/or with the intrinsic atrial and/or ventricular rate.

The output amplifiers circuit **51** contains a RA pace pulse generator (and a LA pace pulse generator if LA pacing is provided), a RV pace pulse generator, a LV pace pulse generator, and/or any other pulse generator configured to provide atrial and ventricular pacing. In order to trigger generation of an RV-PACE or LV-PACE pulse, digital controller/timer circuit **43** generates the RV-TRIG signal at the time-out of the A-RVp delay (in the case of RV pre-excitation) or the LV-TRIG at the time-out of the A-LVp delay (in the case of LV pre-excitation) provided by AV delay interval timer **83E** (or the V-V delay timer **83B**). Similarly, digital controller/timer circuit **43** generates an RA-TRIG signal that triggers output of an RA-PACE pulse (or an LA-TRIG signal that triggers output of an LA-PACE pulse, if provided) at the end of the V-A escape interval timed by escape interval timers **83D**.

The output amplifiers circuit **51** includes switching circuits for coupling selected pace electrode pairs from among the lead conductors and the IND-CAN electrode **20** to the RA pace pulse generator (and LA pace pulse generator if provided), RV pace pulse generator and LV pace pulse generator. Pace/sense electrode pair selection and control circuit **53** selects lead conductors and associated pace electrode pairs to be coupled with the atrial and ventricular output amplifiers within output amplifiers circuit **51** for accomplishing RA, LA, RV and LV pacing.

The sense amplifiers circuit **55** contains sense amplifiers for atrial and ventricular pacing and sensing. High impedance P-wave and R-wave sense amplifiers may be used to amplify a voltage difference signal that is generated across the sense electrode pairs by the passage of cardiac depolarization wavefronts. The high impedance sense amplifiers use high gain to amplify the low amplitude signals and rely on pass band filters, time domain filtering and amplitude thresh-

old comparison to discriminate a P-wave or R-wave from background electrical noise. Digital controller/timer circuit **43** controls sensitivity settings of the atrial and ventricular sense amplifiers **55**.

The sense amplifiers may be uncoupled from the sense electrodes during the blanking periods before, during, and after delivery of a pace pulse to any of the pace electrodes of the pacing system to avoid saturation of the sense amplifiers. The sense amplifiers circuit **55** includes blanking circuits for uncoupling the selected pairs of the lead conductors and the IND-CAN electrode **20** from the inputs of the RA sense amplifier (and LA sense amplifier if provided), RV sense amplifier and LV sense amplifier during the ABP, PVARP and VBP. The sense amplifiers circuit **55** also includes switching circuits for coupling selected sense electrode lead conductors and the IND-CAN electrode **20** to the RA sense amplifier (and LA sense amplifier if provided), RV sense amplifier and LV sense amplifier. Again, sense electrode selection and control circuit **53** selects conductors and associated sense electrode pairs to be coupled with the atrial and ventricular sense amplifiers within the output amplifiers circuit **51** and sense amplifiers circuit **55** for accomplishing RA, LA, RV, and LV sensing along desired unipolar and bipolar sensing vectors.

Right atrial depolarizations or P-waves in the RA-SENSE signal that are sensed by the RA sense amplifier result in a RA-EVENT signal that is communicated to the digital controller/timer circuit **43**. Similarly, left atrial depolarizations or P-waves in the LA-SENSE signal that are sensed by the LA sense amplifier, if provided, result in a LA-EVENT signal that is communicated to the digital controller/timer circuit **43**. Ventricular depolarizations or R-waves in the RV-SENSE signal are sensed by a ventricular sense amplifier result in an RV-EVENT signal that is communicated to the digital controller/timer circuit **43**. Similarly, ventricular depolarizations or R-waves in the LV-SENSE signal are sensed by a ventricular sense amplifier result in an LV-EVENT signal that is communicated to the digital controller/timer circuit **43**. The RV-EVENT, LV-EVENT, and RA-EVENT, LA-SENSE signals may be refractory or non-refractory, and can inadvertently be triggered by electrical noise signals or aberrantly conducted depolarization waves rather than true R-waves or P-waves.

The techniques described in this disclosure, including those attributed to the IMD **16**, the computing apparatus **140**, and/or various constituent components, may be implemented, at least in part, in hardware, software, firmware, or any combination thereof. For example, various aspects of the techniques may be implemented within one or more processors, including one or more microprocessors, DSPs, ASICs, FPGAs, or any other equivalent integrated or discrete logic circuitry, as well as any combinations of such components, embodied in programmers, such as physician or patient programmers, stimulators, image processing devices, or other devices. The term "module," "processor," or "processing circuitry" may generally refer to any of the foregoing logic circuitry, alone or in combination with other logic circuitry, or any other equivalent circuitry.

Such hardware, software, and/or firmware may be implemented within the same device or within separate devices to support the various operations and functions described in this disclosure. In addition, any of the described units, modules, or components may be implemented together or separately as discrete but interoperable logic devices. Depiction of different features as modules or units is intended to highlight different functional aspects and does not necessarily imply that such modules or units must be realized by

separate hardware or software components. Rather, functionality associated with one or more modules or units may be performed by separate hardware or software components, or integrated within common or separate hardware or software components.

When implemented in software, the functionality ascribed to the systems, devices and techniques described in this disclosure may be embodied as instructions on a computer-readable medium such as RAM, ROM, NVRAM, EEPROM, FLASH memory, magnetic data storage media, optical data storage media, or the like. The instructions may be executed by processing circuitry and/or one or more processors to support one or more aspects of the functionality described in this disclosure.

ILLUSTRATIVE EMBODIMENTS

Embodiment 1

A system for use in cardiac evaluation comprising:  
 electrode apparatus comprising a plurality of external electrodes to be located proximate a patient's skin, wherein the plurality of external electrodes comprises:  
 a posterior set of electrodes located proximate the patient's posterior, and an anterior set of electrodes located proximate the patient's anterior; and  
 computing apparatus comprising one or more processors, the computing apparatus operably coupled to the electrode apparatus and configured to:  
 monitor electrical activity from the patient's skin using the plurality of external electrodes over a cardiac cycle resulting in a posterior set of electrode signals monitored from one or more of the posterior set of electrodes and an anterior set of electrode signals monitored from one or more of the anterior set of electrodes, and  
 compare the morphology of the anterior set of electrode signals and the morphology of the posterior set of electrode signals to assist in determination of electrical heterogeneity.

Embodiment 2

The system as set forth embodiment 1, wherein comparing the morphology of the anterior set of electrode signals and the morphology of the posterior set of electrode signals comprises determining whether the morphology of the posterior set of electrode signals is similar to the morphology of the anterior set of electrode signals.

Embodiment 3

The system as set forth in any one of embodiments 1-2, wherein comparing the morphology of the anterior set of electrode signals and the morphology of the posterior set of electrode signals comprises determining whether the morphology of the posterior set of electrode signals is predominately opposite the morphology of the anterior set of electrode signals.

Embodiment 4

The system as set forth in any one of embodiments 1-3, wherein the computing apparatus is further configured to determine an activation time of the QRS complex of the cardiac cycle for each electrode signal of the anterior set of electrode signals and the posterior set of electrode signals, wherein comparing the morphology of the anterior set of electrode signals and the morphology of the posterior set of

electrode signals comprises comparing the activation times of the anterior set of electrode signals and the activation times of the posterior set of electrode signals.

Embodiment 5

The system as set forth in any one of embodiments 1-4, wherein the computing apparatus is further configured to determine an amplitude of the QRS complex of the cardiac cycle for each electrode signal of the anterior set of electrode signals and the posterior set of electrode signals, wherein comparing the morphology of the anterior set of electrode signals and the morphology of the posterior set of electrode signals comprises comparing the amplitudes of the anterior set of electrode signals and the amplitudes of the posterior set of electrode signals.

Embodiment 6

The system as set forth in any one of embodiments 1-5, wherein comparing the morphology of the anterior set of electrode signals and the morphology of the posterior set of electrode signals comprises determining a metric of electrical heterogeneity comparing the anterior set of electrode signals and the posterior set of electrode signals, wherein the metric of electrical heterogeneity comprises at least one of:  
 ventricular electrical uncoupling metric based in a difference between an average of activation times of the posterior set of electrode signals and an average of activation times of the anterior set of electrode signals;  
 composite area under the curve metric based on of the area under the curve of the anterior set of electrode signals and the area under the curve of the posterior set of electrode signals;  
 composite height metric based on the maximum heights of each of the anterior set of electrode signals and the maximum heights of each of the posterior set of electrode signals; and  
 composite inter-activation event activation distance based on the distance between each activation time of the anterior set of electrode signals and each activation time of the posterior set of electrode signals.

Embodiment 7

The system as set forth in any one of embodiments 1-6, the system further comprising a display comprising a graphical user interface to present cardiac signal information, wherein the computing apparatus is further configured to:  
 initiate cardiac therapy to the patient applying a plurality of different cardiac therapy settings over a plurality of cardiac cycles; and  
 display on the graphical user interface a plurality of single-cycle graphs, each single-cycle graph corresponding to a different cardiac cycle where different cardiac therapy settings are applied, each single-cycle graph including all of the posterior set of electrode signals and the anterior set of electrode signals.

Embodiment 8

The system as set forth in embodiment 7, wherein comparing the anterior set of electrode signals and the posterior set of electrode signals comprises determining a metric of electrical heterogeneity based on the anterior set of electrode signals and the posterior set of electrode signals for each different cardiac cycle where different cardiac therapy set-

tings are applied, wherein the computing apparatus is further configured to display the metric of electrical heterogeneity for each different cardiac cycle where different cardiac therapy settings are applied proximate the corresponding single-cycle graph, wherein the metric of electrical heterogeneity comprises at least one of:

ventricular electrical uncoupling metric based in a difference between an average of activation times of the posterior set of electrode signals and an average of activation times of the anterior set of electrode signals;

composite area under the curve metric based on of the area under the curve of the anterior set of electrode signals and the area under the curve of the posterior set of electrode signals;

composite height metric based on the maximum heights of each of the anterior set of electrode signals and the maximum heights of each of the posterior set of electrode signals; and

composite inter-activation event activation distance based on the distance between each activation time of the anterior set of electrode signals and each activation time of the posterior set of electrode signals.

#### Embodiment 9

The system as set forth in any one of embodiments 7-8, wherein the plurality of different cardiac settings comprises one or more of selection between intrinsic rhythm, left ventricular-only pacing and biventricular pacing, V-V pacing delay, and A-V pacing delay.

#### Embodiment 10

The system as set forth in any one of embodiments 7-9, wherein the computing apparatus is further configured to:

determine effective cardiac settings of the plurality of different cardiac therapy settings based the posterior set of electrode signals and the anterior set of electrodes; and

indicate a desired single-cycle graph of the plurality of single-cycle graphs on the graphical user interface that corresponds to the determined effective cardiac settings.

#### Embodiment 11

The system as set forth in any one of embodiments 1-9, wherein the computing apparatus is further configured to:

initiate cardiac therapy to the patient applying a plurality of different cardiac therapy settings over a plurality of cardiac cycles; and

determine effective cardiac settings of the plurality of different cardiac therapy settings based on the posterior set of electrode signals and the anterior set of electrodes.

#### Embodiment 12

A method for use in cardiac evaluation comprising:

monitoring electrical activity from a patient's skin using a plurality of external electrodes over a cardiac cycle resulting in a posterior set of electrode signals monitored from one or more of posterior set of electrodes located proximate the patient's posterior and an anterior set of electrode signals monitored from one or more of an anterior set of electrodes located proximate the patient's anterior; and

comparing the morphology of the anterior set of electrode signals and the morphology of the posterior set of electrode signals to assist in determination of electrical heterogeneity.

#### Embodiment 13

The method as set forth in embodiment 12, wherein comparing the morphology of the anterior set of electrode signals and the morphology of the posterior set of electrode signals comprises determining whether the morphology of the posterior set of electrode signals is similar to the morphology of the anterior set of electrode signals.

#### Embodiment 14

The method as set forth in any one of embodiments 12-3, wherein comparing the morphology of the anterior set of electrode signals and the morphology of the posterior set of electrode signals comprises determining whether the morphology of the posterior set of electrode signals is predominately opposite the morphology of the anterior set of electrode signals.

#### Embodiment 15

The method as set forth in any one of embodiments 12-14, the method further comprising determining an activation time of the QRS complex of the cardiac cycle for each electrode signal of the anterior set of electrode signals and the posterior set of electrode signals,

wherein comparing the morphology of the anterior set of electrode signals and the morphology of the posterior set of electrode signals comprises comparing the activation times of the anterior set of electrode signals and the activation times of the posterior set of electrode signals.

#### Embodiment 16

The method as set forth in any one of embodiments 12-15, the method further comprising determining an amplitude of the QRS complex of the cardiac cycle for each electrode signal of the anterior set of electrode signals and the posterior set of electrode signals,

wherein comparing the morphology of the anterior set of electrode signals and the morphology of the posterior set of electrode signals comprises comparing the amplitudes of the anterior set of electrode signals and the amplitudes of the posterior set of electrode signals.

#### Embodiment 17

The method as set forth in any one of embodiments 12-16, wherein comparing the morphology of the anterior set of electrode signals and the morphology of the posterior set of electrode signals comprises determining a metric of electrical heterogeneity comparing the anterior set of electrode signals and the posterior set of electrode signals, wherein the metric of electrical heterogeneity comprises at least one of:

ventricular electrical uncoupling metric based in a difference between an average of activation times of the posterior set of electrode signals and an average of activation times of the anterior set of electrode signals;

composite area under the curve metric based on of the area under the curve of the anterior set of electrode signals and the area under the curve of the posterior set of electrode signals;

composite height metric based on the maximum heights of each of the anterior set of electrode signals and the maximum heights of each of the posterior set of electrode signals; and

39

composite inter-activation event activation distance based on the distance between each activation time of the anterior set of electrode signals and each activation time of the posterior set of electrode signals.

## Embodiment 18

The method as set forth in any one of embodiments 12-17, the method further comprising:

initiating cardiac therapy to the patient applying a plurality of different cardiac therapy settings over a plurality of cardiac cycles; and

displaying on a graphical user interface a plurality of single-cycle graphs, each single-cycle graph corresponding to a different cardiac cycle where different cardiac therapy settings are applied, each single-cycle graph including all of the posterior set of electrode signals and the anterior set of electrode signals.

## Embodiment 19

The method as set forth in embodiment 18, wherein comparing the anterior set of electrode signals and the posterior set of electrode signals comprises determining a metric of electrical heterogeneity based on the anterior set of electrode signals and the posterior set of electrode signals for each different cardiac cycle where different cardiac therapy settings are applied, wherein the computing apparatus is further configured to display the metric of electrical heterogeneity for each different cardiac cycle where different cardiac therapy settings are applied proximate the corresponding single-cycle graph, wherein the metric of electrical heterogeneity comprises at least one of:

ventricular electrical uncoupling metric based in a difference between an average of activation times of the posterior set of electrode signals and an average of activation times of the anterior set of electrode signals;

composite area under the curve metric based on of the area under the curve of the anterior set of electrode signals and the area under the curve of the posterior set of electrode signals;

composite height metric based on the maximum heights of each of the anterior set of electrode signals and the maximum heights of each of the posterior set of electrode signals; and

composite inter-activation event activation distance based on the distance between each activation time of the anterior set of electrode signals and each activation time of the posterior set of electrode signals.

## Embodiment 20

The method as set forth in any one of embodiments 18-19, wherein the plurality of different cardiac settings comprises one or more of selection between intrinsic rhythm, left ventricular-only pacing and biventricular pacing, V-V pacing delay, and A-V pacing delay.

## Embodiment 21

The method as set forth in any one of embodiments 18-20, the method further comprising:

determining effective cardiac settings of the plurality of different cardiac therapy settings based the posterior set of electrode signals and the anterior set of electrodes; and

40

indicating a desired single-cycle graph of the plurality of single-cycle graphs on the graphical user interface that corresponds to the determined effective cardiac settings.

## Embodiment 22

The method as set forth in any one of embodiments 12-21, the method further comprising:

initiating cardiac therapy to the patient applying a plurality of different cardiac therapy settings over a plurality of cardiac cycles; and

determining effective cardiac settings of the plurality of different cardiac therapy settings based on the posterior set of electrode signals and the anterior set of electrodes.

This disclosure has been provided with reference to illustrative embodiments and is not meant to be construed in a limiting sense. As described previously, one skilled in the art will recognize that other various illustrative applications may use the techniques as described herein to take advantage of the beneficial characteristics of the apparatus and methods described herein. Various modifications of the illustrative embodiments, as well as additional embodiments of the disclosure, will be apparent upon reference to this description.

What is claimed:

1. A system for use in cardiac evaluation comprising:

electrode apparatus comprising a plurality of external electrodes to be located proximate a patient's skin, wherein the plurality of external electrodes comprises: a posterior set of electrodes located proximate the patient's posterior, and an anterior set of electrodes located proximate the patient's anterior; and

computing apparatus comprising processing circuitry, the computing apparatus operably coupled to the electrode apparatus and configured to:

monitor electrical activity from the patient's skin using the plurality of external electrodes over a cardiac cycle resulting in a posterior set of electrode signals monitored from one or more of the posterior set of electrodes and an anterior set of electrode signals monitored from one or more of the anterior set of electrodes, and

compare a morphology of the anterior set of electrode signals and a morphology of the posterior set of electrode signals to assist in determination of electrical heterogeneity.

2. The system of claim 1, wherein comparing the morphology of the anterior set of electrode signals and the morphology of the posterior set of electrode signals comprises determining whether the morphology of the posterior set of electrode signals is similar to the morphology of the anterior set of electrode signals.

3. The system of claim 1, wherein comparing the morphology of the anterior set of electrode signals and the morphology of the posterior set of electrode signals comprises determining whether the morphology of the posterior set of electrode signals is predominately opposite the morphology of the anterior set of electrode signals.

4. The system of claim 1, wherein the computing apparatus is further configured to determine an activation time of the QRS complex of the cardiac cycle for each electrode signal of the anterior set of electrode signals and the posterior set of electrode signals,

wherein comparing the morphology of the anterior set of electrode signals and the morphology of the posterior set of electrode signals comprises comparing the acti-

vation times of the anterior set of electrode signals and the activation times of the posterior set of electrode signals.

5. The system of claim 1, wherein the computing apparatus is further configured to determine an amplitude of the QRS complex of the cardiac cycle for each electrode signal of the anterior set of electrode signals and the posterior set of electrode signals,

wherein comparing the morphology of the anterior set of electrode signals and the morphology of the posterior set of electrode signals comprises comparing the amplitudes of the anterior set of electrode signals and the amplitudes of the posterior set of electrode signals.

6. The system of claim 1, wherein comparing the morphology of the anterior set of electrode signals and the morphology of the posterior set of electrode signals comprises determining a metric of electrical heterogeneity comparing the anterior set of electrode signals and the posterior set of electrode signals, wherein the metric of electrical heterogeneity comprises at least one of:

ventricular electrical uncoupling metric based on a difference between an average of activation times of the posterior set of electrode signals and an average of activation times of the anterior set of electrode signals;

composite area under the curve metric based on the area under the curve of the anterior set of electrode signals and the area under the curve of the posterior set of electrode signals;

composite height metric based on the maximum heights of each of the anterior set of electrode signals and the maximum heights of each of the posterior set of electrode signals; and

composite inter-activation event activation distance based on the distance between each activation time of the anterior set of electrode signals and each activation time of the posterior set of electrode signals.

7. The system of claim 1, the system further comprising a display comprising a graphical user interface to present cardiac signal information, wherein the computing apparatus is further configured to:

initiate cardiac therapy to the patient applying a plurality of different cardiac therapy settings over a plurality of cardiac cycles; and

display on the graphical user interface a plurality of single-cycle graphs, each single-cycle graph corresponding to a different cardiac cycle where different cardiac therapy settings are applied, each single-cycle graph including all of the posterior set of electrode signals and the anterior set of electrode signals.

8. The system of claim 7, wherein comparing the anterior set of electrode signals and the posterior set of electrode signals comprises determining a metric of electrical heterogeneity based on the anterior set of electrode signals and the posterior set of electrode signals for each different cardiac cycle where different cardiac therapy settings are applied, wherein the computing apparatus is further configured to display the metric of electrical heterogeneity for each different cardiac cycle where different cardiac therapy settings are applied proximate the corresponding single-cycle graph, wherein the metric of electrical heterogeneity comprises at least one of:

ventricular electrical uncoupling metric based on a difference between an average of activation times of the posterior set of electrode signals and an average of activation times of the anterior set of electrode signals;

composite area under the curve metric based on the area under the curve of the anterior set of electrode signals and the area under the curve of the posterior set of electrode signals;

composite height metric based on the maximum heights of each of the anterior set of electrode signals and the maximum heights of each of the posterior set of electrode signals; and

composite inter-activation event activation distance based on the distance between each activation time of the anterior set of electrode signals and each activation time of the posterior set of electrode signals.

9. The system of claim 7, wherein the plurality of different cardiac settings comprises one or more of selection between intrinsic rhythm, left ventricular-only pacing and biventricular pacing, V-V pacing delay, and A-V pacing delay.

10. The system of claim 7, wherein the computing apparatus is further configured to:

determine effective cardiac settings of the plurality of different cardiac therapy settings based on the posterior set of electrode signals and the anterior set of electrodes; and

indicate a desired single-cycle graph of the plurality of single-cycle graphs on the graphical user interface that corresponds to the determined effective cardiac settings.

11. The system of claim 1, wherein the computing apparatus is further configured to:

initiate cardiac therapy to the patient applying a plurality of different cardiac therapy settings over a plurality of cardiac cycles; and

determine effective cardiac settings of the plurality of different cardiac therapy settings based on the posterior set of electrode signals and the anterior set of electrodes.

12. A method for use in cardiac evaluation comprising: monitoring electrical activity from a patient's skin using a plurality of external electrodes over a cardiac cycle resulting in a posterior set of electrode signals monitored from one or more of a posterior set of electrodes located proximate the patient's posterior and an anterior set of electrode signals monitored from one or more of an anterior set of electrodes located proximate the patient's anterior; and

comparing a morphology of the anterior set of electrode signals and a morphology of the posterior set of electrode signals to assist in determination of electrical heterogeneity.

13. The method of claim 12, wherein comparing the morphology of the anterior set of electrode signals and the morphology of the posterior set of electrode signals comprises determining whether the morphology of the posterior set of electrode signals is similar to the morphology of the anterior set of electrode signals.

14. The method of claim 12, wherein comparing the morphology of the anterior set of electrode signals and the morphology of the posterior set of electrode signals comprises determining whether the morphology of the posterior set of electrode signals is predominately opposite the morphology of the anterior set of electrode signals.

15. The method of claim 12, the method further comprising determining an activation time of the QRS complex of the cardiac cycle for each electrode signal of the anterior set of electrode signals and the posterior set of electrode signals, wherein comparing the morphology of the anterior set of electrode signals and the morphology of the posterior set of electrode signals comprises comparing the acti-

vation times of the anterior set of electrode signals and the activation times of the posterior set of electrode signals.

16. The method of claim 12, the method further comprising determining an amplitude of the QRS complex of the cardiac cycle for each electrode signal of the anterior set of electrode signals and the posterior set of electrode signals, wherein comparing the morphology of the anterior set of electrode signals and the morphology of the posterior set of electrode signals comprises comparing the amplitudes of the anterior set of electrode signals and the amplitudes of the posterior set of electrode signals.

17. The method of claim 12, wherein comparing the morphology of the anterior set of electrode signals and the morphology of the posterior set of electrode signals comprises determining a metric of electrical heterogeneity comparing the anterior set of electrode signals and the posterior set of electrode signals, wherein the metric of electrical heterogeneity comprises at least one of:

- ventricular electrical uncoupling metric based on a difference between an average of activation times of the posterior set of electrode signals and an average of activation times of the anterior set of electrode signals;
- composite area under the curve metric based on the area under the curve of the anterior set of electrode signals and the area under the curve of the posterior set of electrode signals;
- composite height metric based on the maximum heights of each of the anterior set of electrode signals and the maximum heights of each of the posterior set of electrode signals; and
- composite inter-activation event activation distance based on the distance between each activation time of the anterior set of electrode signals and each activation time of the posterior set of electrode signals.

18. The method of claim 12, the method further comprising:

- initiating cardiac therapy to the patient applying a plurality of different cardiac therapy settings over a plurality of cardiac cycles; and
- displaying on a graphical user interface a plurality of single-cycle graphs, each single-cycle graph corresponding to a different cardiac cycle where different cardiac therapy settings are applied, each single-cycle graph including all of the posterior set of electrode signals and the anterior set of electrode signals.

19. The method of claim 18, wherein comparing the anterior set of electrode signals and the posterior set of electrode signals comprises determining a metric of electrical heterogeneity based on the anterior set of electrode

signals and the posterior set of electrode signals for each different cardiac cycle where different cardiac therapy settings are applied, wherein the computing apparatus is further configured to display the metric of electrical heterogeneity for each different cardiac cycle where different cardiac therapy settings are applied proximate the corresponding single-cycle graph, wherein the metric of electrical heterogeneity comprises at least one of:

- ventricular electrical uncoupling metric based on a difference between an average of activation times of the posterior set of electrode signals and an average of activation times of the anterior set of electrode signals;
- composite area under the curve metric based on the area under the curve of the anterior set of electrode signals and the area under the curve of the posterior set of electrode signals;
- composite height metric based on the maximum heights of each of the anterior set of electrode signals and the maximum heights of each of the posterior set of electrode signals; and
- composite inter-activation event activation distance based on the distance between each activation time of the anterior set of electrode signals and each activation time of the posterior set of electrode signals.

20. The method of claim 18, wherein the plurality of different cardiac settings comprises one or more of selection between intrinsic rhythm, left ventricular-only pacing and biventricular pacing, V-V pacing delay, and A-V pacing delay.

21. The method of claim 18, the method further comprising:

- determining effective cardiac settings of the plurality of different cardiac therapy settings based on the posterior set of electrode signals and the anterior set of electrodes; and
- indicating a desired single-cycle graph of the plurality of single-cycle graphs on the graphical user interface that corresponds to the determined effective cardiac settings.

22. The method of claim 12, the method further comprising:

- initiating cardiac therapy to the patient applying a plurality of different cardiac therapy settings over a plurality of cardiac cycles; and
- determining effective cardiac settings of the plurality of different cardiac therapy settings based on the posterior set of electrode signals and the anterior set of electrodes.

\* \* \* \* \*

专利名称(译)	前后电极信号		
公开(公告)号	<a href="#">US10492705</a>	公开(公告)日	2019-12-03
申请号	US16/229256	申请日	2018-12-21
[标]申请(专利权)人(译)	明尼苏达大学		
申请(专利权)人(译)	明尼苏达大学校董会		
当前申请(专利权)人(译)	明尼苏达大学校董会		
发明人	BANK, ALAN J. CURTIN, ANTONIA E. GAGE, RYAN M. BURNS, KEVIN V.		
IPC分类号	A61B5/04 A61B5/0452 A61B5/00 A61B5/0408 A61N1/39 A61N1/362		
CPC分类号	A61B5/04011 A61B5/04085 A61B5/0452 A61B5/04087 A61N1/3904 A61B5/7203 A61N1/3627 A61B5/6823 A61N1/3956 A61B5/6805 A61N1/362 A61N1/368		
优先权	62/609935 2017-12-22 US		
其他公开文献	US20190192035A1		
外部链接	<a href="#">Espacenet</a>		

摘要(译)

示例性系统，方法和接口可以从多个外部电极获得并分析电极信号。电极信号可以至少包括电极信号的前组和电极信号的后组。电极信号的前组和后组可用于生成或提供心脏电异质性的各种指标以及可用于评估患者心脏功能的各种图形描述。

