


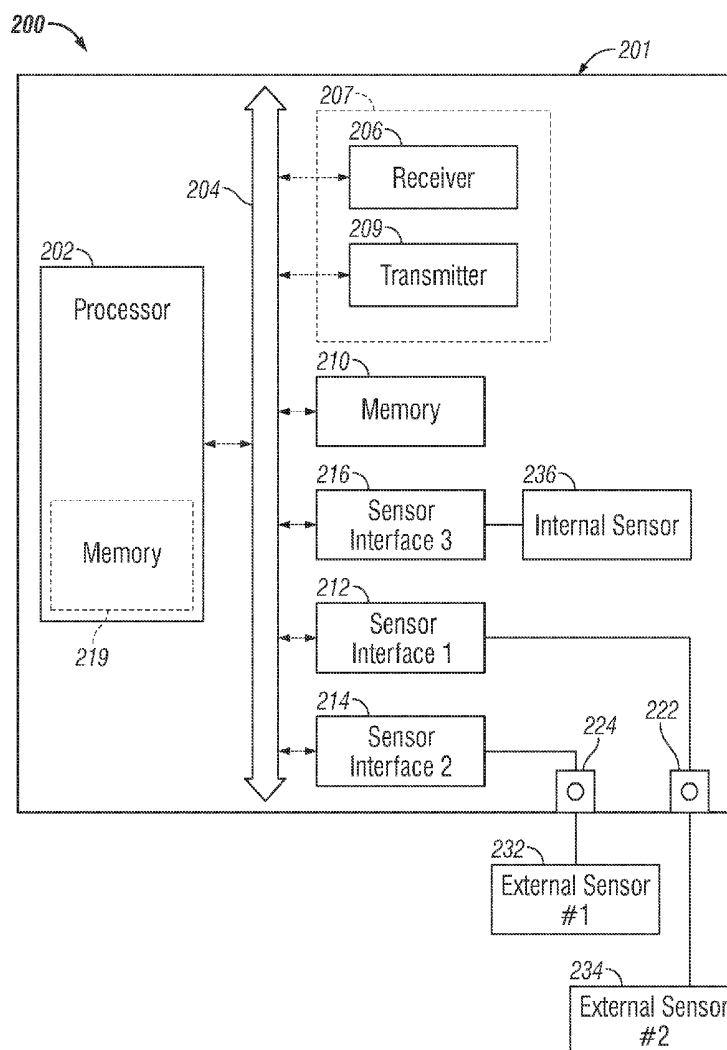

US 20150223706A1

(19) **United States**(12) **Patent Application Publication**
RAPTIS et al.(10) **Pub. No.: US 2015/0223706 A1**(43) **Pub. Date: Aug. 13, 2015**(54) **SYSTEM AND METHOD FOR SAVING
BATTERY POWER IN A PATIENT
MONITORING SYSTEM****Publication Classification**(51) **Int. Cl.***A61B 5/0205* (2006.01)*A61B 5/00* (2006.01)(52) **U.S. Cl.**CPC *A61B 5/02055* (2013.01); *A61B 5/6823*
(2013.01); *A61B 5/6833* (2013.01); *A61B*
5/746 (2013.01); *A61B 5/1116* (2013.01)(71) Applicant: **CAREFUSION 303, INC.**, San Diego,
CA (US)(72) Inventors: **Mark RAPTIS**, Valley Center, CA (US);
Amir JAFRI, San Diego, CA (US);
Ganesh KATHIRESAN, Osterley (GB);
Alison BURDETT, Oxford (GB);
Okundu OMENI, Hillingdon (GB);
Mathew KEY, Oxford (GB)(21) Appl. No.: **14/694,957**(22) Filed: **Apr. 23, 2015****Related U.S. Application Data**(62) Division of application No. 12/844,801, filed on Jul.
27, 2010, now Pat. No. 9,017,255.(57) **ABSTRACT**

A vital-signs patch for a patient monitoring system is disclosed. The patch consists of a housing that is configured to be worn on the skin of a patient. The housing contains a radio, one or more sensor interfaces, a processor, and a battery. The processor can selectably turn portions of the processor off and on and selectably turn power off and on to at least a portion of the sensor interfaces and radio. The processor includes a timer that, each time the timer times out, will turn all the parts of the processor on and start a new timing period. When the processor receives a signal, the processor will turn off power to at least a portion of the processor and at least a portion of the sensor interfaces.



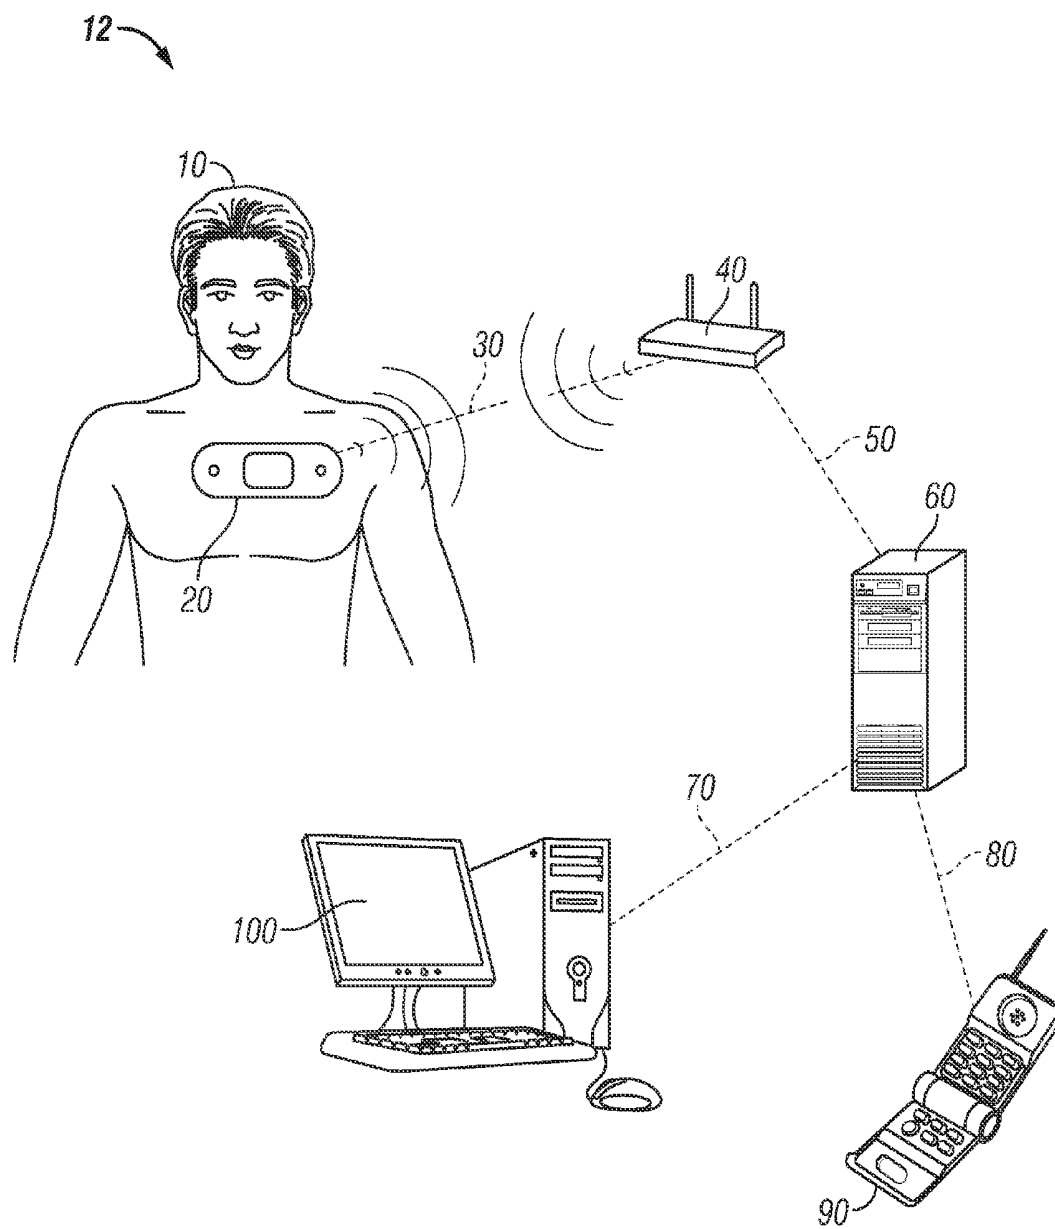


FIG. 1

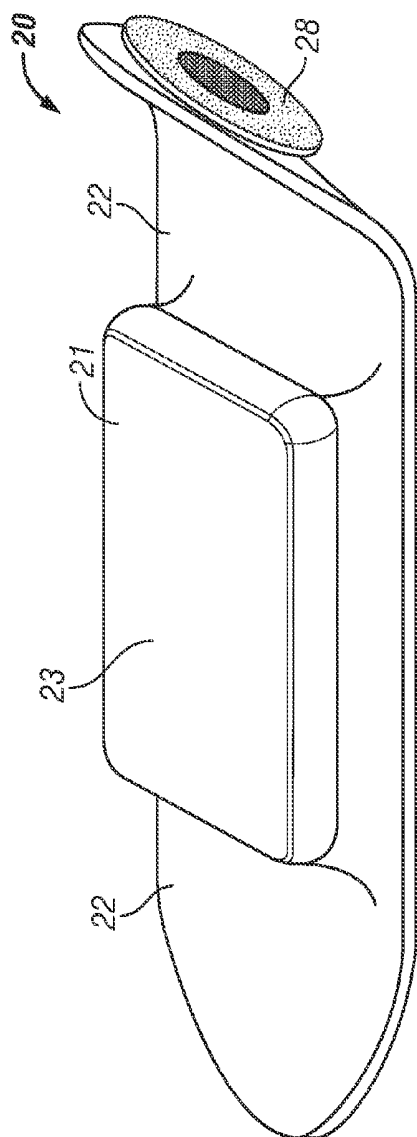


FIG. 2A

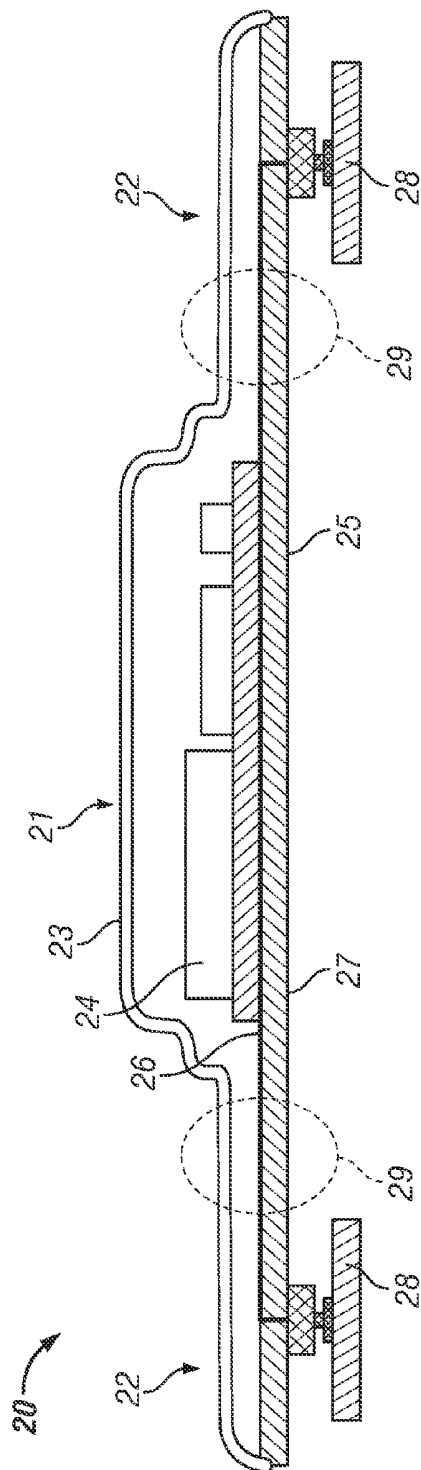


FIG. 2B

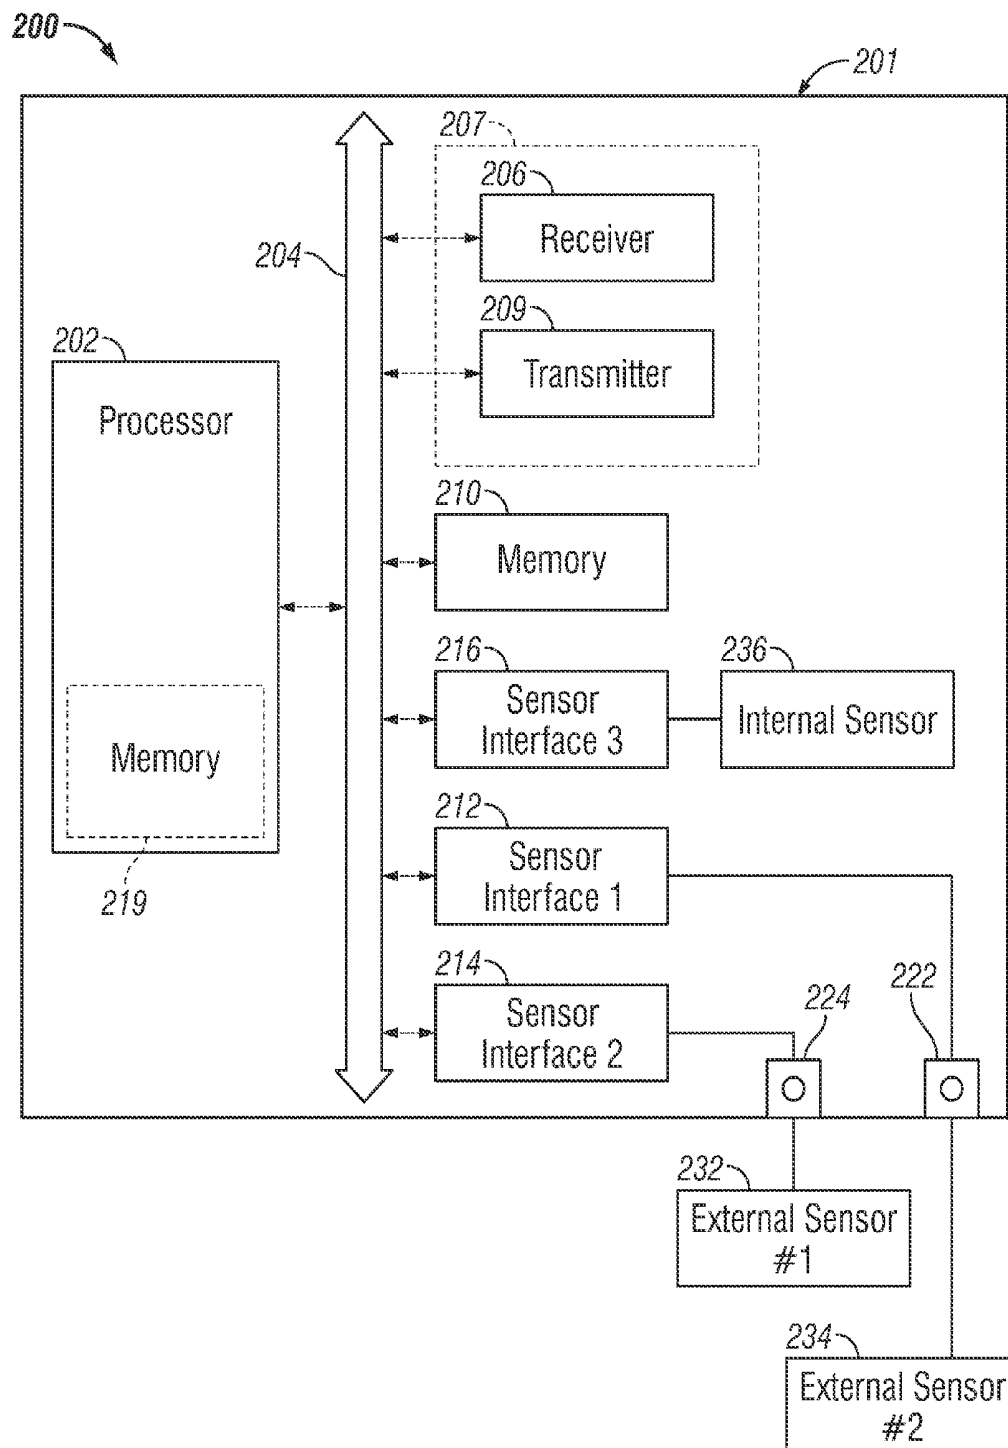


FIG. 2C

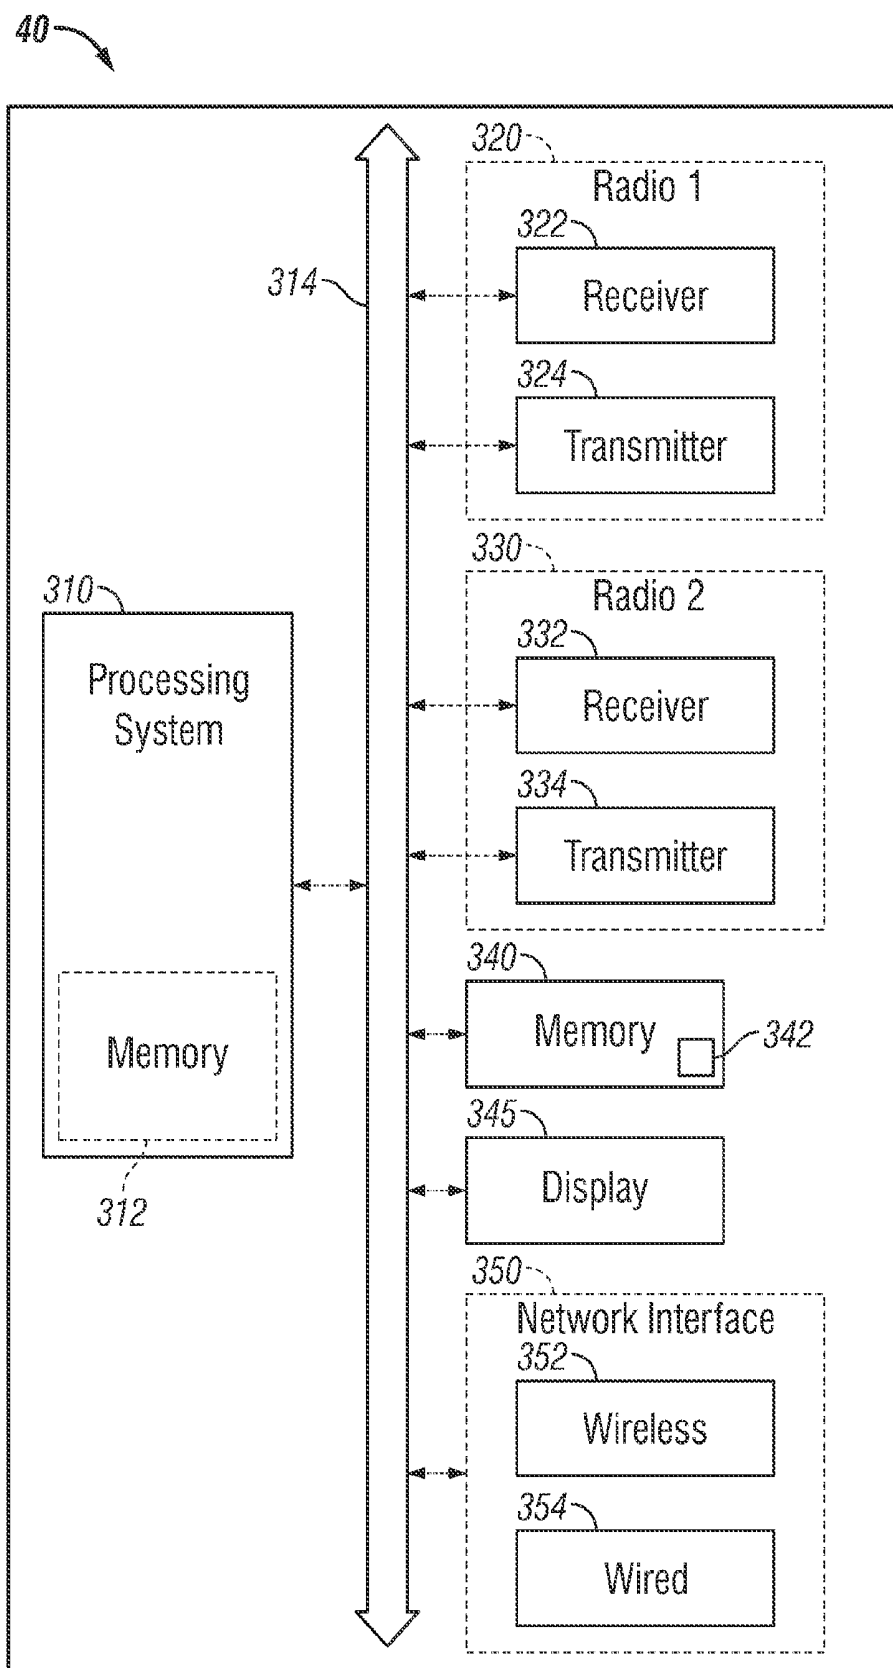


FIG. 3A

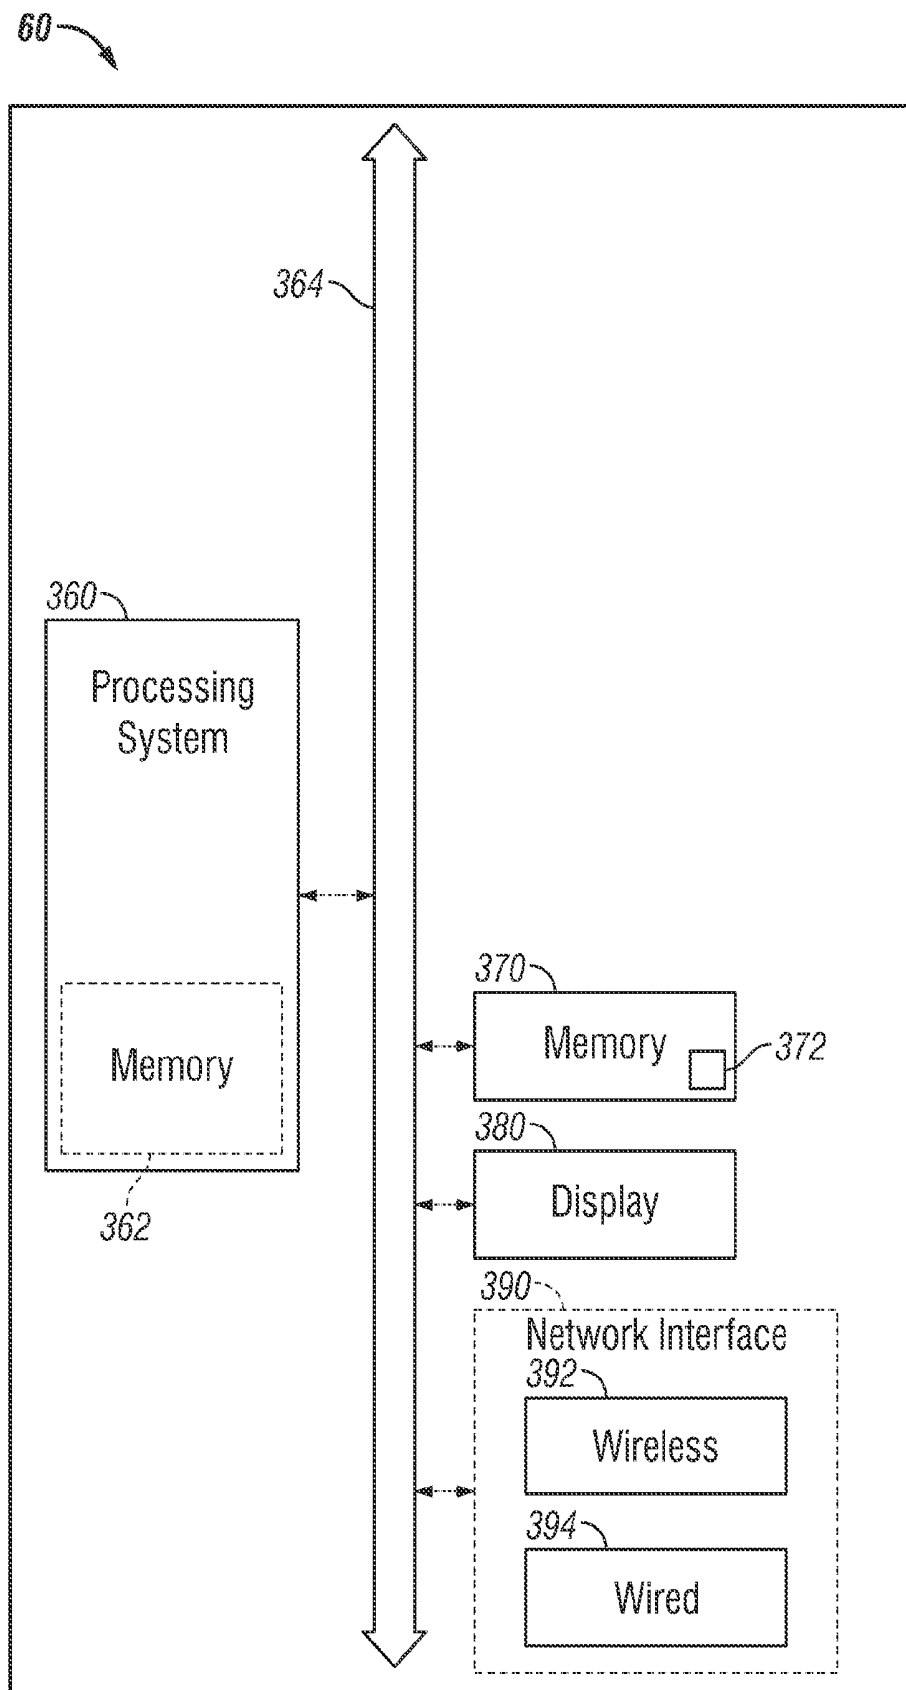


FIG. 3B

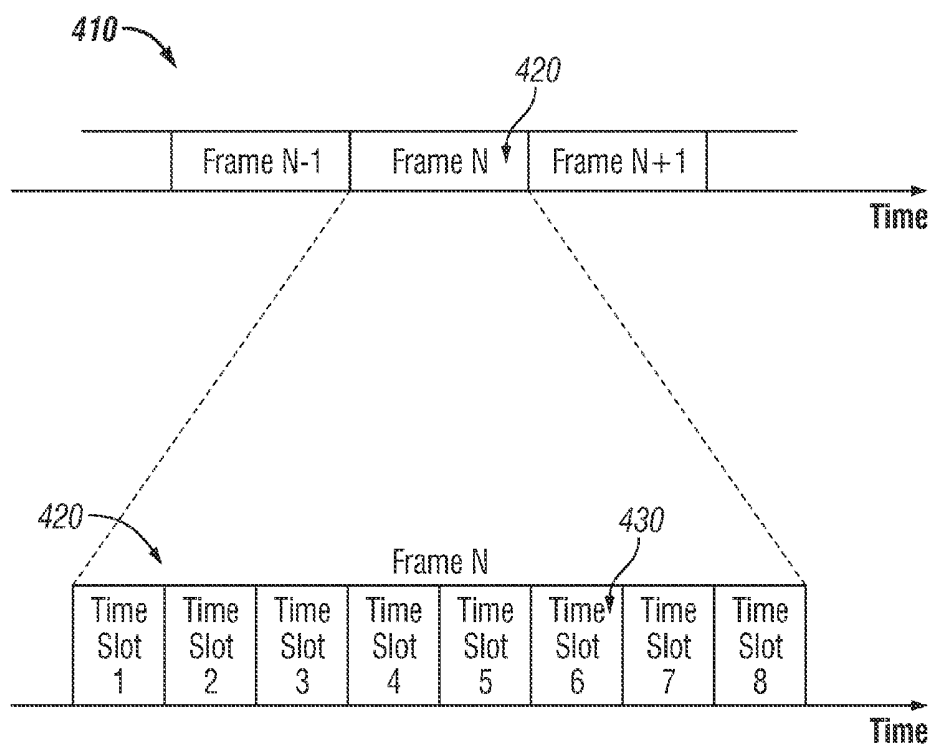


FIG. 4

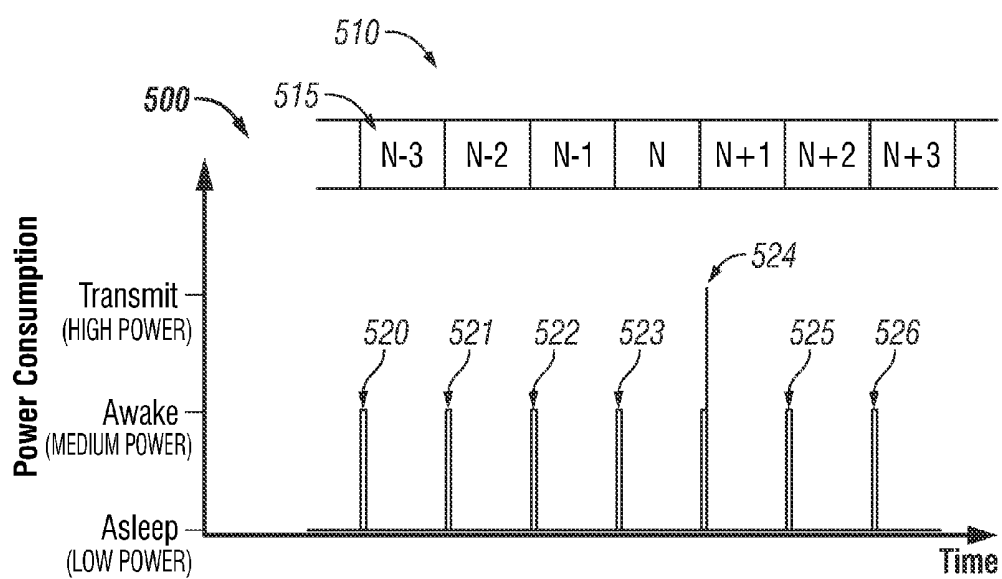


FIG. 5

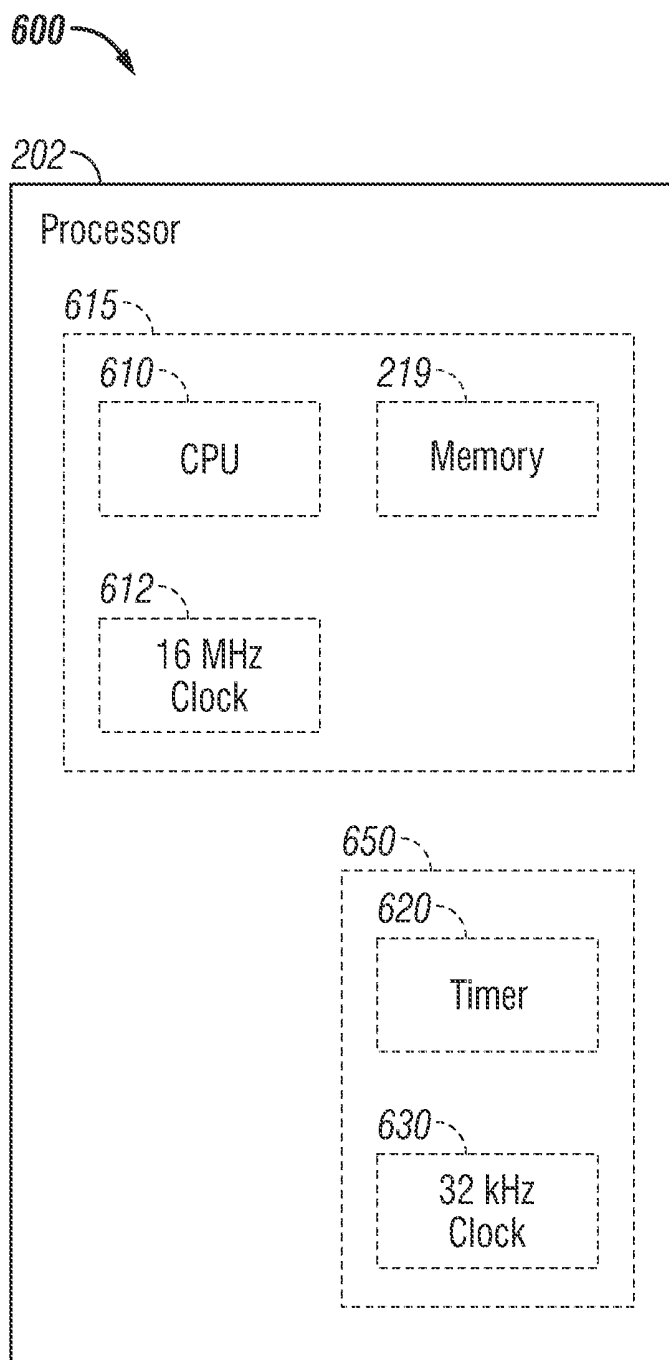


FIG. 6

SYSTEM AND METHOD FOR SAVING BATTERY POWER IN A PATIENT MONITORING SYSTEM

CROSS-REFERENCES TO RELATED APPLICATIONS

[0001] This application is a divisional of U.S. patent application Ser. No. 12/844,801 filed Jul. 27, 2010, which is herein incorporated by reference in its entirety for all purposes.

BACKGROUND

[0002] 1. Field

[0003] The present disclosure generally relates to systems and methods of physiological monitoring, and, in particular, relates to monitoring of vital signs of patients in hospitals.

[0004] 2. Description of the Related Art

[0005] Some of the most basic indicators of a person's health are those physiological measurements that reflect basic body functions and are commonly referred to as a person's "vital signs." The four measurements commonly considered to be vital signs are body temperature, pulse rate, blood pressure, and respiratory rate. Some clinicians consider oxygen saturation (S_{O_2}) to be a "fifth vital sign" particularly for pediatric or geriatric cases. Some or all of these measurements may be performed routinely upon a patient when they arrive at a healthcare facility, whether it is a routine visit to their doctor or arrival at an Emergency Room (ER).

[0006] Vital signs are frequently taken by a nurse using basic tools including a thermometer to measure body temperature, a sphygmomanometer to measure blood pressure, and a watch to count the number of breaths or the number of heart beats in a defined period of time which is then converted to a "per minute" rate. If a patient's pulse is weak, it may not be possible to detect a pulse by hand and the nurse may use a stethoscope to amplify the sound of the patient's heart beat so that she can count the beats. Oxygen saturation of the blood is most easily measured with a pulse oximeter.

[0007] When a patient is admitted to a hospital, it is common for vital signs to be measured and recorded at regular intervals during the patient's stay to monitor their condition. A typical interval is 4 hours, which leads to the undesirable requirement for a nurse to awaken a patient in the middle of the night to take vital sign measurements.

[0008] When a patient is admitted to an ER, it is common for a nurse to do a "triage" assessment of the patient's condition that will determine how quickly the patient receives treatment. During busy times in an ER, a patient who does not appear to have a life-threatening injury may wait for hours until more-serious cases have been treated. While the patient may be reassessed at intervals while awaiting treatment, the patient may not be under observation between these reassessments.

[0009] Measuring certain vital signs is normally intrusive at best and difficult to do on a continuous basis. Measurement of body temperature, for example, is commonly done by placing an oral thermometer under the tongue or placing an infrared thermometer in the ear canal such that the tympanic membrane, which shared blood circulation with the brain, is in the sensor's field of view. Another method of taking a body temperature is by placing a thermometer under the arm, referred to as an "axillary" measurement as axilla is the Latin word for armpit. Skin temperature can be measured using a

stick-on strip that may contain panels that change color to indicate the temperature of the skin below the strip.

[0010] Measurement of respiration is easy for a nurse to do, but relatively complicated for equipment to achieve. A method of automatically measuring respiration is to encircle the upper torso with a flexible band that can detect the physical expansion of the rib cage when a patient inhales. An alternate technique is to measure a high-frequency electrical impedance between two electrodes placed on the torso and detect the change in impedance created when the lungs fill with air. The electrodes are typically placed on opposite sides of one or both lungs, resulting in placement on the front and back or on the left and right sides of the torso, commonly done with adhesive electrodes connected by wires or by using a torso band with multiple electrodes in the strap.

[0011] Measurement of pulse is also relatively easy for a nurse to do and intrusive for equipment to achieve. A common automatic method of measuring a pulse is to use an electrocardiograph (ECG or EKG) to detect the electrical activity of the heart. An EKG machine may use 12 electrodes placed at defined points on the body to detect various signals associated with the heart function. Another common piece of equipment is simply called a "heart rate monitor." Widely sold for use in exercise and training, heart rate monitors commonly consist of a torso band, in which are embedded two electrodes held against the skin and a small electronics package. Such heart rate monitors can communicate wirelessly to other equipment such as a small device that is worn like a wristwatch and that can transfer data wirelessly to a PC.

[0012] Nurses are expected to provide complete care to an assigned number of patients. The workload of a typical nurse is increasing, driven by a combination of a continuing shortage of nurses, an increase in the number of formal procedures that must be followed, and an expectation of increased documentation. Replacing the manual measurement and logging of vital signs with a system that measures and records vital signs would enable a nurse to spend more time on other activities and avoid the potential for error that is inherent in any manual procedure.

SUMMARY

[0013] For some or all of the reasons listed above, there is a need for a hospital to be able to continuously monitor its patients in different settings within the hospital. In addition, it is desirable for this monitoring to be done with limited interference with a patient's mobility or interfering with their other activities.

[0014] Continuous monitoring implies that the sensors that measure the physiological characteristic of interest remain continuously in place on the patient. Periodic removal of a sensor, for such things as using the bathroom or showering, usually requires a nurse or other caregiver to reattach the sensor to ensure that the sensor is properly attached and may require replacement of the sensor each time the sensor is removed. The presence of wires between the sensors and the monitoring equipment makes it difficult for a patient to perform their normal activities and move around the hospital. An analogous situation exists in use of an intravenous (IV) system to continuously administer medication, where the patient is connected to an IV bag via a tube which remains continuously attached to the patient. Even when the IV bag is mounted on a mobile stand without connection to a fixed piece of equipment, this attached tube poses a significant

impediment to a patient in moving around the hospital, changing clothes, and taking a shower.

[0015] One solution to the problem of providing continuous monitoring without having wires connecting the patient to separate device is to use a battery-powered wireless device to measure the physiological characteristics of interest. The useful life of battery-powered devices is limited, however, by the capacity of the battery compared to the power consumption of the device. Providing a battery-powered device that can monitor the vital signs of a patient for a period of several days may require a battery so large that it is impractical for the patient to continuously wear the device. It is highly desirable to provide a vital-signs monitoring device that has a very low level of power consumption such that a very small battery, such as the “coin” batteries commonly used in watches, has enough power to continuously operate the device for several days.

[0016] Embodiments of the patient monitoring system disclosed herein measure certain vital signs of a patient, which include respiratory rate, pulse rate, and body temperature, on a regular basis and compare these measurements to preset limits.

[0017] In certain embodiments of the disclosure, a vital-signs patch for a patient monitoring system is disclosed. The patch consists of a housing that is configured to be worn on the skin of a patient. The housing contains a radio, one or more sensor interfaces, a processor, and a battery. The processor can selectably turn portions of the processor off and on and selectably turn power off and on to at least a portion of the sensor interfaces and radio. The processor includes a timer that, each time the timer times out, will turn all the parts of the processor on and start a new timing period. When the processor receives a signal, the processor will turn off power to at least a portion of the processor and at least a portion of the sensor interfaces.

[0018] In certain embodiments of the disclosure, a patient monitoring system is disclosed. The system includes a patch configured to turn off a portion of its circuitry for a period of time upon receipt of a sleep signal and then to turn on that portion of its circuitry after a period of time has elapsed, and a bridge configured to send the sleep signal to the patch. The bridge tracks when the period of time elapses and sends the sleep signal to the patch after the period of time elapses.

[0019] In certain embodiments of the disclosure, a method of conserving battery power in a patch in a patient monitoring system is disclosed. The method includes the steps of the patch receiving a sleep signal, turning off a portion of the circuitry of the patch and starting a timer, turning on the portion of the circuitry that was turned off upon the timer timing out, and resumption of monitoring for sleep signals.

[0020] It is understood that other configurations of the subject technology will become readily apparent to those skilled in the art from the following detailed description, wherein various configurations of the subject technology are shown and described by way of illustration. As will be realized, the subject technology is capable of other and different configurations and its several details are capable of modification in various other respects, all without departing from the scope of the subject technology. Accordingly, the drawings and detailed description are to be regarded as illustrative in nature and not as restrictive.

BRIEF DESCRIPTION OF THE DRAWINGS

[0021] The accompanying drawings, which are included to provide further understanding and are incorporated in and constitute a part of this specification, illustrate disclosed embodiments and together with the description serve to explain the principles of the disclosed embodiments. In the drawings:

[0022] FIG. 1 is a diagram illustrating an exemplary embodiment of a patient monitoring system according to certain aspects of the present disclosure.

[0023] FIG. 2A is a perspective view of the vital-signs monitor patch of FIG. 1 according to certain aspects of the present disclosure.

[0024] FIG. 2B is a cross-section of the vital-signs monitor patch of FIG. 1 according to certain aspects of the present disclosure.

[0025] FIG. 2C is a functional block diagram illustrating exemplary electronic and sensor components of the vital-signs monitor patch of FIG. 1 according to certain aspects of the present disclosure.

[0026] FIG. 3A is a functional schematic diagram of the bridge according to certain aspects of the subject disclosure.

[0027] FIG. 3B is a functional schematic diagram of an embodiment of the surveillance server according to certain aspects of the present disclosure.

[0028] FIG. 4 discloses an example of the communication protocol between the vital-signs patch and bridge according to certain aspects of the present disclosure.

[0029] FIG. 5 is a plot of power consumption vs. time illustrating that battery power in the vital-signs patch is conserved according to certain aspects of this disclosure.

[0030] FIG. 6 is a functional block diagram illustrating exemplary details of the processor of FIG. 2C according to certain aspects of the present disclosure.

DETAILED DESCRIPTION

[0031] Periodic monitoring of patients in a hospital is desirable at least to ensure that patients do not suffer an un-noticed sudden deterioration in their condition or a secondary injury during their stay in the hospital. It is impractical to provide continuous monitoring by a clinician and cumbersome to connect sensors to a patient, which are then connected to a fixed monitoring instrument by wires. Furthermore, systems that sound an alarm when the measured value exceeds a threshold value may sound alarms so often and in situations that are not truly serious that such alarms are ignored by clinicians.

[0032] Measuring vital signs is difficult to do on a continuous basis. Accurate measurement of cardiac pulse, for example, can be done using an electrocardiograph (ECG or EKG) to detect the electrical activity of the heart. An EKG machine may use up to 12 electrodes placed at various points on the body to detect various signals associated with the cardiac function. Another common piece of equipment is termed a “heart rate monitor.” Widely sold for use in exercise and physical training, heart rate monitors may comprise a torso band in which are embedded two electrodes held against the skin and a small electronics package. Such heart rate monitors can communicate wirelessly to other equipment such as a small device that is worn like a wristwatch and that can transfer data wirelessly to a personal computer (PC).

[0033] Monitoring of patients that is referred to as “continuous” is frequently periodic, in that measurements are

taken at intervals. In many cases, the process to make a single measurement takes a certain amount of time, such that even back-to-back measurements produce values at an interval equal to the time that it takes to make the measurement. For the purpose of vital sign measurement, a sequence of repeated measurements can be considered to be “continuous” when the vital sign is not likely to change an amount that is of clinical significance within the interval between measurements. For example, a measurement of blood pressure every 10 minutes may be considered “continuous” if it is considered unlikely that a patient’s blood pressure can change by a clinically significant amount within 10 minutes. The interval appropriate for measurements to be considered continuous may depend on a variety of factors including the type of injury or treatment and the patient’s medical history. Compared to intervals of 4-8 hours for manual vital sign measurement in a hospital, measurement intervals of 30 minutes to several hours may still be considered “continuous.”

[0034] Certain exemplary embodiments of the present disclosure include a system that comprises a vital-signs monitor patch that is attached to the patient, and a bridge that communicates with monitor patches and links them to a central server that processes the data, where the server can send data and alarms to a hospital system according to algorithms and protocols defined by the hospital.

[0035] The construction of the vital-signs monitor patch is described according to certain aspects of the present disclosure. As the patch may be worn continuously for a period of time that may be several days, as is described in the following disclosure, it is desirable to encapsulate the components of the patch such that the patient can bathe or shower and engage in their normal activities without degradation of the patch function. An exemplary configuration of the construction of the patch to provide a hermetically sealed enclosure about the electronics is disclosed.

[0036] In the following detailed description, numerous specific details are set forth to provide a full understanding of the present disclosure. It will be apparent, however, to one ordinarily skilled in the art that embodiments of the present disclosure may be practiced without some of the specific details. In other instances, well-known structures and techniques have not been shown in detail so as not to obscure the disclosure.

[0037] FIG. 1 discloses a vital sign monitoring system according to certain embodiments of the present disclosure. The vital sign monitoring system 12 includes vital-signs monitor patch 20, bridge 40, and surveillance server 60 that can send messages or interact with peripheral devices exemplified by mobile device 90 and workstation 100.

[0038] Monitor patch 20 resembles a large adhesive bandage and is applied to a patient 10 when in use. It is preferable to apply the monitor patch 20 to the upper chest of the patient 10 although other locations may be appropriate in some circumstances. Monitor patch 20 incorporates one or more electrodes (not shown) that are in contact with the skin of patient 10 to measure vital signs such as cardiac pulse rate and respiration rate. Monitor patch 20 also may include other sensors such as an accelerometer, temperature sensor, or oxygen saturation sensor to measure other characteristics associated with the patient. These other sensors may be internal to the monitor patch 20 or external sensors that are operably connected to the monitor patch 20 via a cable or wireless connection. Monitor patch 20 also includes a wireless transmitter that can both transmit and receive signals. This trans-

mitter is preferably a short-range, low-power radio frequency (RF) device operating in one of the unlicensed radio bands. One band in the United States (US) is, for example, centered at 915 MHz and designated for industrial, scientific and medical (ISM) purposes. An example of an equivalent band in the European Union (EU) is centered at 868 MHz. Other frequencies of operation may be possible dependent upon the International Telecommunication Union (ITU), local regulations and interference from other wireless devices.

[0039] Surveillance server 60 may be a standard computer server connected to the hospital communication network and preferably located in the hospital data center or computer room, although other locations may be employed. The server 60 stores and processes signals related to the operation of the patient monitoring system 12 disclosed herein including the association of individual monitor patches 20 with patients 10 and measurement signals received from multiple monitor patches 20. Hence, although only a single patient 10 and monitor patch 20 are depicted in FIG. 1, the server 60 is able to monitor the monitor patches 20 for multiple patients 10.

[0040] Bridge 40 is a device that connects, or “bridges”, between monitor patch 20 and server 60. Bridge 40 communicates with monitor patch 20 over communication link 30 operating, in these exemplary embodiments, at approximately 915 MHz and at a power level that enables communication link 30 to function up to a distance of approximately 10 meters. It is preferable to place a bridge 40 in each room and at regular intervals along hallways of the healthcare facility where it is desired to provide the ability to communicate with monitor patches 20. Bridge 40 also is able to communicate with server 60 over network link 50 using any of a variety of computer communication systems including hardwired and wireless Ethernet using protocols such as 802.11a/b/g or 802.3af. As the communication protocols of communication link 30 and network link 50 may be very different, bridge 40 provides data buffering and protocol conversion to enable bidirectional signal transmission between monitor patch 20 and server 60.

[0041] While the embodiments illustrated by FIG. 1 employ a bridge 20 to provide communication link between the monitor patch 20 and the server 60, in certain alternative embodiments, the monitor patch 20 may engage in direct wireless communication with the server 60. In such alternative embodiments, the server 60 itself or a wireless modem connected to the server 60 may include a wireless communication system to receive data from the monitor patch 20.

[0042] In use, a monitor patch 20 is applied to a patient 10 by a clinician when it is desirable to continuously monitor basic vital signs of patient 10 while patient 10 is, in this embodiment, in a hospital. Monitor patch 20 is intended to remain attached to patient 10 for an extended period of time, for example, up to 5 days in certain embodiments, limited by the battery life of monitor patch 20. In some embodiments, monitor patch 20 is disposable when removed from patient 10.

[0043] Server 60 executes analytical protocols on the measurement data that it receives from monitor patch 20 and provides this information to clinicians through external workstations 100, preferably personal computers (PCs), laptops, or smart phones, over the hospital network 70. Server 60 may also send messages to mobile devices 90, such as cell phones or pagers, over a mobile device link 80 if a measurement signal exceeds specified parameters. Mobile device link 80 may include the hospital network 70 and internal or external

wireless communication systems that are capable of sending messages that can be received by mobile devices 90.

[0044] FIG. 2A is a perspective view of the vital-signs monitor patch 20 shown in FIG. 1 according to certain aspects of the present disclosure. In the illustrated embodiment, the monitor patch 20 includes component carrier 23 comprising a central segment 21 and side segments 22 on opposing sides of the central segment 21. In certain embodiments, the central segment 21 is substantially rigid and includes a circuit assembly (24, FIG. 2B) having electronic components and battery mounted to a rigid printed circuit board (PCB). The side segments 22 are flexible and include a flexible conductive circuit (26, FIG. 2B) that connect the circuit assembly 24 to electrodes 28 disposed at each end of the monitor patch 20, with side segment 22 on the right shown as being bent upwards for purposes of illustration to make one of the electrodes 28 visible in this view.

[0045] FIG. 2B is a cross-sectional view of the vital-signs patch 20 shown in FIGS. 1 and 2A according to certain aspects of the present disclosure. The circuit assembly 24 and flexible conductive circuit 26 described above can be seen herein. The flexible conductive circuit 26 operably connects the circuit assembly 24 to the electrodes 28. Top and bottom layers 23 and 27 form a housing 25 that encapsulate circuit assembly 28 to provide a water and particulate barrier as well as mechanical protection. There are sealing areas on layers 23 and 27 that encircle circuit assembly 28 and is visible in the cross-section view of FIG. 2B as areas 29. Layers 23 and 27 are sealed to each other in this area to form a substantially hermetic seal. Within the context of certain aspects of the present disclosure, the term 'hermetic' implies that the rate of transmission of moisture through the seal is substantially the same as through the material of the layers that are sealed to each other, and further implies that the size of particulates that can pass through the seal are below the size that can have a significant effect on circuit assembly 24. Flexible conductive circuit 26 passes through portions of sealing areas 29 and the seal between layers 23 and 27 is maintained by sealing of layers 23 and 27 to flexible circuit assembly 28. The layers 23 and 27 are thin and flexible, as is the flexible conductive circuit 26, allowing the side segment 22 of the monitor patch 20 between the electrodes 28 and the circuit assembly 24 to bend as shown in FIG. 2A.

[0046] FIG. 2C is a functional block diagram 200 illustrating exemplary electronic and sensor components of the monitor patch 20 of FIG. 1 according to certain aspects of the present disclosure. The block diagram 200 shows a processing and sensor interface module 201 and external sensors 232, 234 connected to the module 201. In the illustrated example, the module 201 includes a processor 202, a wireless transceiver 207 having a receiver 206 and a transmitter 209, a memory 210, a first sensor interface 212, a second sensor interface 214, a third sensor interface 216, and an internal sensor 236 connected to the third sensor interface 216. The first and second sensor interfaces 212 and 214 are connected to the first and second external sensors 232, 234 via first and second connection ports 222, 224, respectively. In certain embodiments, some or all of the aforementioned components of the module 201 and other components are mounted on a PCB.

[0047] Each of the sensor interfaces 212, 214, 216 can include one or more electronic components that are configured to generate an excitation signal or provide DC power for the sensor that the interface is connected to and/or to condi-

tion and digitize a sensor signal from the sensor. For example, the sensor interface can include a signal generator for generating an excitation signal or a voltage regulator for providing power to the sensor. The sensor interface can further include an amplifier for amplifying a sensor signal from the sensor and an analog-to-digital converter for digitizing the amplified sensor signal. The sensor interface can further include a filter (e.g., a low-pass or bandpass filter) for filtering out spurious noises (e.g., a 60 Hz noise pickup).

[0048] The processor 202 is configured to send and receive data (e.g., digitized signal or control data) to and from the sensor interfaces 212, 214, 216 via a bus 204, which can be one or more wire traces on the PCB. Although a bus communication topology is used in this embodiment, some or all communication between discrete components can also be implemented as direct links without departing from the scope of the present disclosure. For example, the processor 202 may send data representative of an excitation signal to the sensor excitation signal generator inside the sensor interface and receive data representative of the sensor signal from the sensor interface, over either a bus or direct data links between processor 202 and each of sensor interface 212, 214, and 216.

[0049] The processor 202 is also capable of communication with the receiver 206 and the transmitter 209 of the wireless transceiver 207 via the bus 204. For example, the processor 202 using the transmitter and receiver 209, 206 can transmit and receive data to and from the bridge 40. In certain embodiments, the transmitter 209 includes one or more of a RF signal generator (e.g., an oscillator), a modulator (a mixer), and a transmitting antenna; and the receiver 206 includes a demodulator (a mixer) and a receiving antenna which may or may not be the same as the transmitting antenna. In some embodiments, the transmitter 209 may include a digital-to-analog converter configured to receive data from the processor 202 and to generate a base signal; and/or the receiver 206 may include an analog-to-digital converter configured to digitize a demodulated base signal and output a stream of digitized data to the processor 202. In other embodiments, the radio may comprise a direct sequence radio, a software-defined radio, or an impulse spread spectrum radio.

[0050] The processor 202 may include a general-purpose processor or a specific-purpose processor for executing instructions and may further include a memory 219, such as a volatile or non-volatile memory, for storing data and/or instructions for software programs. The instructions, which may be stored in a memory 219 and/or 210, may be executed by the processor 202 to control and manage the wireless transceiver 207, the sensor interfaces 212, 214, 216, as well as provide other communication and processing functions.

[0051] The processor 202 may be a general-purpose microprocessor, a microcontroller, a Digital Signal Processor (DSP), an Application Specific Integrated Circuit (ASIC), a Field Programmable Gate Array (FPGA), a Programmable Logic Device (PLD), a controller, a state machine, gated logic, discrete hardware components, or any other suitable device or a combination of devices that can perform calculations or other manipulations of information.

[0052] Information, such as program instructions, data representative of sensor readings, preset alarm conditions, threshold limits, may be stored in a computer or processor readable medium such as a memory internal to the processor 202 (e.g., the memory 219) or a memory external to the processor 202 (e.g., the memory 210), such as a Random Access Memory (RAM), a flash memory, a Read Only

Memory (ROM), a Programmable Read-Only Memory (PROM), an Erasable PROM (EPROM), registers, a hard disk, a removable disk, or any other suitable storage device.

[0053] In certain embodiments, the internal sensor 236 can be one or more sensors configured to measure certain properties of the processing and sensor interface module 201, such as a board temperature sensor thermally coupled to a PCB. In other embodiments, the internal sensor 236 can be one or more sensors configured to measure certain properties of the patient 10, such as a motion sensor (e.g., an accelerometer) for measuring the patient's motion or position with respect to gravity.

[0054] The external sensors 232, 234 can include sensors and sensing arrangements that are configured to produce a signal representative of one or more vital signs of the patient to which the monitor patch 20 is attached. For example, the first external sensor 232 can be a set of sensing electrodes that are affixed to an exterior surface of the monitor patch 20 and configured to be in contact with the patient for measuring the patient's respiratory rate, and the second external sensor 234 can include a temperature sensing element (e.g., a thermocouple or a thermistor or resistive thermal device (RTD)) affixed, either directly or via an interposing layer, to skin of the patient 10 for measuring the patient's body temperature. In other embodiments, one or more of the external sensors 232, 234 or one or more additional external sensors can measure other vital signs of the patient, such as blood pressure, pulse rate, or oxygen saturation.

[0055] FIG. 3A is a functional block diagram illustrating exemplary electronic components of bridge 40 of FIG. 1 according to certain aspects of the subject disclosure. Bridge 40 includes a processor 310, radio 320 having a receiver 322 and a transmitter 324, radio 330 having a receiver 332 and a transmitter 334, memory 340, display 345, and network interface 350 having a wireless interface 352 and a wired interface 354. In some embodiments, some or all of the aforementioned components of module 300 may be integrated into single devices or mounted on PCBs.

[0056] Processor 310 is configured to send data to and receive data from receiver 322 and transmitter 324 of radio 320, receiver 332 and transmitter 334 of radio 330 and wireless interface 352 and wired interface 354 of network interface 350 via bus 314. In certain embodiments, transmitters 324 and 334 may include a radio frequency signal generator (oscillator), a modulator, and a transmitting antenna, and the receivers 322 and 332 may include a demodulator and antenna which may or may not be the same as the transmitting antenna of the radio. In some embodiments, transmitters 324 and 334 may include a digital-to-analog converter configured to convert data received from processor 310 and to generate a base signal, while receivers 322 and 332 may include analog-to-digital converters configured to convert a demodulated base signal and sent a digitized data stream to processor 310.

[0057] Processor 310 may include a general-purpose processor or a specific-purpose processor for executing instructions and may further include a memory 312, such as a volatile or non-volatile memory, for storing data and/or instructions for software programs. The instructions, which may be stored in memories 312 or 340, may be executed by the processor 310 to control and manage the transceivers 320, 330, and 350 as well as provide other communication and processing functions.

[0058] Processor 310 may be a general-purpose microprocessor, a microcontroller, a Digital Signal Processor (DSP),

an Application Specific Integrated Circuit (ASIC), a Field Programmable Gate Array (FPGA), a Programmable Logic Device (PLD), a controller, a state machine, gated logic, discrete hardware components, or any other suitable device or a combination of devices that can perform calculations or other manipulations of information.

[0059] Information such as data representative of sensor readings may be stored in memory 312 internal to processor 310 or in memory 340 external to processor 310 which may be a Random Access Memory (RAM), flash memory, Read Only Memory (ROM), Programmable Read Only Memory (PROM), Erasable Programmable Read Only Memory (EPROM), registers, a hard disk, a removable disk, a Solid State Memory (SSD), or any other suitable storage device.

[0060] Memory 312 or 340 can also store a list or a database of established communication links and their corresponding characteristics (e.g., signal levels) between the bridge 40 and its related monitor patches 20. In the illustrated example of FIG. 3A, the memory 340 external to the processor 310 includes such a database 342; alternatively, the memory 312 internal to the processor 310 may include such a database.

[0061] FIG. 3B is a functional block diagram illustrating exemplary electronic components of server 60 of FIG. 1 according to one aspect of the subject disclosure. Server 60 includes a processor 360, memory 370, display 380, and network interface 390 having a wireless interface 392 and a wired interface 394. Processor 360 may include a general-purpose processor or a specific-purpose processor for executing instructions and may further include a memory 362, such as a volatile or non-volatile memory, for storing data and/or instructions for software programs. The instructions, which may be stored in memories 362 or 370, may be executed by the processor 360 to control and manage the wireless and wired network interfaces 392, 394 as well as provide other communication and processing functions.

[0062] Processor 360 may be a general-purpose microprocessor, a microcontroller, a Digital Signal Processor (DSP), an Application Specific Integrated Circuit (ASIC), a Field Programmable Gate Array (FPGA), a Programmable Logic Device (PLD), a controller, a state machine, gated logic, discrete hardware components, or any other suitable device or a combination of devices that can perform calculations or other manipulations of information.

[0063] Information such as data representative of sensor readings may be stored in memory 362 internal to processor 360 or in memory 370 external to processor 360 which may be a Random Access Memory (RAM), flash memory, Read Only Memory (ROM), Programmable Read Only Memory (PROM), Erasable Programmable Read Only Memory (EPROM), registers, a hard disk, a removable disk, a Solid State Memory (SSD), or any other suitable storage device.

[0064] Memory 362 or 370 can also store a database of communication links and their corresponding characteristics (e.g., signal levels) between monitor patches 20 and bridges 40. In the illustrated example of FIG. 3B, the memory 370 external to the processor 360 includes such a database 372; alternatively, the memory 362 internal to the processor 360 may include such a database.

[0065] FIG. 4 discloses certain aspects of the communication protocol between patch 20 and bridge 40. Bridge 40 may be configured to communicate with multiple patches 20. Bridge 40 will define a length of time during which it will allocate time to communicate with each patch 20. This defined period of time 420 is termed a 'frame' and FIG. 4

illustrates how a data stream **410** is segmented into frames **420** that are sequentially arranged and numbered. Frame **N** is preceded by frame **N-1** and followed by frame **N+1**. Each frame **420** has an identical internal structure which, in this example, has been configured to enable bridge **40** to communicate with up to eight patches. Frame **420** has been segmented into eight time slots **430**, numbered 1-8 in this example, as shown in the expanded view of frame **420**. Each patch **20** which is in communication with bridge **40** is assigned to a time slot **430** by bridge **40**.

[0066] FIG. 5 discloses how battery power is conserved according to certain aspects of this disclosure. Plot **500** illustrates the instantaneous power consumption of a patch **20**, with time plotted on the horizontal axis and power plotted on the vertical axis. The frame sequence **410** from FIG. 4 is repeated as timeline **510** as a reference. In timeline **510**, the patch **20** whose power is plotted in plot **500** has been assigned to time slot **515** which is the first time slot in each frame and is darkened in each frame of timeline **510**.

[0067] At the beginning of each time slot **430**, the entire electronics of patch **20** are turned on. Patch **20** sends a very short message announcing that it is awake. When bridge **40** receives this signal, it will send a command signal to patch **20**. If bridge **40** watches patch **20** to perform an operation, such as reporting its configuration or status or uploading measurements, bridge **40** sends a command to perform this function. If no action by patch **20** is desired at this time, bridge **40** sends a 'sleep' command. Upon receiving a sleep command, patch **20** turns off power to a portion of the electronics including, in this example and referring to FIG. 2C, all power to the transmitter **206**, receiver **209**, sensor interfaces **212**, **214**, and **216** which also removes power from sensors **232**, **234**, and **236**. The patch also turns off a portion of the processor **202**, which is described in more detail in FIG. 6. Patch **20** remains in this sleep state until the portion of processor **202** that is still on wakes up patch **20** by turning on the rest of the processor and the other electronics that have been turned off. The time of this sleep state is selected such that patch **20** wakes up at the beginning of the next time slot.

[0068] Referring to FIG. 6, processor **202** may have more than one section of circuitry that can be independently operated. In this example, there is a high-power section **615**, which contains the CPU **610** and memory **219** and is driven by a 16 MHz crystal clock **612**, and a low-power section **650**, which contains a timer **620** which is driven by a 32 kHz crystal clock **630**. Section **615** can be turned off by CPU **610**. Crystal clocks consume more power relative than other types of semiconductor devices, and the amount of power consumed by a crystal clock is proportional to the frequency of the crystal, as a fixed amount of electrical charge is consumed to switch states at every oscillation. A 16 MHz crystal will usually consume much more power than a 32 kHz crystal as the frequency of the crystal is 500 times higher. Section **650**, in this example, contains low-power fixed-duration hardware timer **620** and low-power clock **630**.

[0069] In this example, timer **620** runs continuously and sends out an 'interrupt' signal every 8 seconds. If section **615** is off when the interrupt signal is sent out by timer **620**, section **615** turns on and then CPU **610** sends out commands to turn on the rest of the electronic components of patch **20**. The state of patch **20** is termed "awake" when both section **615** and section **650** are on and "asleep" when only the low-

power section **650** is on. The power consumption while the patch **20** is awake is higher than the power consumption while patch **20** is asleep.

[0070] Referring again to FIG. 5, exemplary power levels of the three states of patch **20** are marked on the vertical axis—'asleep', 'awake' during which patch **20** can receive signals, and 'transmit' during which patch **20** is transmitting signals to bridge **40**. Initially, patch **20** is asleep and the power consumption level is low. At the beginning of time slot **1** in frame **N-2**, timer **620** in processor **202** times out and sends out its interrupt, turning on the high-power section **615** of processor **202** and the rest of the circuitry of patch **20**. This is shown as event **520**. Bridge **40** is synchronized with patch **20** and knows that time slot **1** is assigned to this patch **20**. In this example, bridge **40** sends a 'sleep' command to patch **20**, patch **20** turns off its high-power section and associated circuitry and the power level drops back to the initial low level. Patch **20** remains asleep until the timer again times out and patch **20** wakes up at event **521**. Bridge **40** again sends a 'sleep' command. This repeats, in this example, through events **522** and **523**. When patch **20** wakes up at event **524**, however, bridge **40** sends a command to upload stored measurement data. This is reflected in the power level of event **524** rising to the 'transmit' level of power consumption. After the data is received, bridge **40** sends a 'sleep' command and patch **20** goes to sleep. When patch **20** wakes up at events **525** and **526**, the bridge sends a 'sleep' command.

[0071] As timer **620** is running continuously, the interrupt signal that timer **620** ends out remains synchronized with frame sequence **410** independent of how long patch **20** remains awake in each time slot **430**.

[0072] As can be seen from plot **510**, the average power consumption of patch **20** is much lower in this mode of operation that it would be if patch **20** was awake for the entire time. For the example in which the duration of the time that patch **20** is awake during events **520-523** and **525-526** is 0.5 seconds, and the duration of a frame **420** is 8 seconds, and if the power consumption when patch **20** is asleep is 10% of the power consumption while the patch is awake, then the average power consumption of this configuration will be $(0.5/8.0) \times 0.10 = 0.00625$ or approximately 0.6% of the power that would be consumed if patch **20** was awake the entire time. It can be seen that implementation of this mode of operation has the potential to extend the battery life by a factor of more than 100× compared to a similar unit that is continuously awake. This reduced level of average power consumption of this example would enable a battery-powered device to operate for 100× longer than a similar unit that is continuously awake or, alternately, the use of a 100× smaller battery to provide an equivalent operating life to a similar unit that is continuously awake. A smaller battery enables the overall size and weight of patch **20** to be smaller which is less intrusive and more comfortable to the patient **10** who is wearing the patch **20**.

[0073] It can be seen that the disclosed embodiments of the vital-signs monitor patch provide a mobile solution to monitoring the vital signs of a patient. The design of the vital-signs monitor patch frees nurses, or other caregivers, from the task of repetitively measuring the vital signs of their patients, allowing the caregivers to spend more time on other duties. The ability to continuously monitor a patient's vital signs using a monitor patch, together with the rest of the patient monitoring system, increases the ability of the nurse to respond quickly to a sudden change in a patient's condition, resulting in improved care for the patient.

[0074] The reduction of power consumption in the vital-signs monitoring patch enables the patch to be smaller and lighter than it would be if the disclosed features were not utilized. A smaller patch will be more comfortable to wear and less intrusive in normal activities of the patient as well as less expensive to manufacture. Increased comfort by the user and reduced cost to the facility providing the care will result in an increased likelihood that the device will be used, resulting in improved patient safety.

[0075] The previous description is provided to enable any person skilled in the art to practice the various aspects described herein. While the foregoing has described what are considered to be the best mode and/or other examples, it is understood that various modifications to these aspects will be readily apparent to those skilled in the art, and the generic principles defined herein may be applied to other aspects. Thus, the claims are not intended to be limited to the aspects shown herein, but is to be accorded the full scope consistent with the language claims, wherein reference to an element in the singular is not intended to mean “one and only one” unless specifically so stated, but rather “one or more.” Unless specifically stated otherwise, the term “some” refers to one or more. Pronouns in the masculine (e.g., his) include the feminine and neuter gender (e.g., her and its) and vice versa. Headings and subheadings, if any, are used for convenience only and do not limit the invention.

[0076] The term ‘battery’ is intended to encompass all energy storage devices which deliver electricity. These energy storage devices may be rechargeable or single-use. This includes but is not limited to batteries using lead-acid, zinc-carbon, alkaline, nickel cadmium, lithium, and lithium-ion technologies, capacitors, generators powered by springs or compressed gas or other mechanical energy storage mechanisms, and fuel cells.

[0077] Those of skill in the art will appreciate that the various illustrative functional blocks, modules, components, methods, and algorithms described herein may be implemented as hardware, software, or a combination of the two. Various components and functional elements may be arranged in a different configuration or partitioned in a different way without departing from the scope of the claimed invention.

[0078] It is understood that the specific order or hierarchy of steps in the processes disclosed is an illustration of exemplary approaches. Based upon design preferences, it is understood that the specific order or hierarchy of steps in the processes may be rearranged. Some of the steps may be performed simultaneously. The accompanying method claims present elements of the various steps in a sample order, and are not meant to be limited to the specific order or hierarchy presented.

[0079] Terms such as “top,” “bottom,” “front,” “rear” and the like as used in this disclosure should be understood as referring to an arbitrary frame of reference, rather than to the ordinary gravitational frame of reference. Thus, a top surface, a bottom surface, a front surface, and a rear surface may extend upwardly, downwardly, diagonally, or horizontally in a gravitational frame of reference.

[0080] A phrase such as an “aspect” does not imply that such aspect is essential to the subject technology or that such aspect applies to all configurations of the subject technology. A disclosure relating to an aspect may apply to all configurations, or one or more configurations. A phrase such as an aspect may refer to one or more aspects and vice versa. A

phrase such as an “embodiment” does not imply that such embodiment is essential to the subject technology or that such embodiment applies to all configurations of the subject technology. A disclosure relating to an embodiment may apply to all embodiments, or one or more embodiments. A phrase such as an embodiment may refer to one or more embodiments and vice versa.

[0081] The word “exemplary” is used herein to mean “serving as an example or illustration.” Any aspect or design described herein as “exemplary” is not necessarily to be construed as preferred or advantageous over other aspects or designs.

[0082] All structural and functional equivalents to the elements of the various aspects described throughout this disclosure that are known or later come to be known to those of ordinary skill in the art are expressly incorporated herein by reference and are intended to be encompassed by the claims. Moreover, nothing disclosed herein is intended to be dedicated to the public regardless of whether such disclosure is explicitly recited in the claims. No claim element is to be construed under the provisions of 35 U.S.C. §112, sixth paragraph, unless the element is expressly recited using the phrase “means for” or, in the case of a method claim, the element is recited using the phrase “step for.” Furthermore, to the extent that the term “include,” “have,” or the like is used in the description or the claims, such term is intended to be inclusive in a manner similar to the term “comprise” as “comprise” is interpreted when employed as a transitional word in a claim.

What is claimed is:

1. A vital-signs patch for a patient monitoring system, comprising:
 - a housing configured for wearing on the skin of a patient, the housing containing:
 - a radio configured to receive signals;
 - a sensor interface;
 - a processor connected to the radio and the sensor interface, wherein:
 - the processor is configured to selectably turn portions of the processor off and on and to selectably turn power off and on to at least a portion of the sensor interface and radio; and
 - the processor comprises a timer that is configured to time out after a specified time period and cause the processor to turn on all the parts of the processor, sensor interface, and radio and start a new timing period; and
 - a battery selectively operably connected to the radio, sensor interface, and processor, wherein the processor is further configured to, upon receipt of a sleep signal received by the radio, turn off at least a portion of the processor and turn off at least a portion of the sensor interface and radio.
2. The vital-signs patch of claim 1, wherein the timer is configured to time out after a fixed period of time.
3. The vital-signs patch of claim 1, wherein the timer is configured to provide a periodic interrupt signal that turns a first portion of the radio on when the first portion of the radio is off.
4. The vital-signs patch of claim 3, wherein the second portion of the radio puts the first portion of the radio to sleep at the end of a time slot assigned to the vital-signs patch.
5. The vital-signs patch of claim 3, further configured so that a rate of power consumption by the patch while the first

portion of the radio is turned off is lower than a rate of power consumption while the entire radio is turned on.

6. The vital-signs patch of claim 1, wherein the specified time period to time out the timer is synchronized with a sleep signal transmitted by a bridge device.

7. The vital-signs patch of claim 1, further configured to consume power at a first rate when the radio, sensor interface, and processor are fully turned on and consumes power at a second rate when at least a portion of the radio, sensor interface, and processor are turned off, wherein the second rate of power consumption is lower than the first rate of power consumption.

8. The vital-signs patch of claim 1, wherein:

the processor comprises a first clock and a second clock, wherein the first clock consumes more power than the second clock, the portion of the processor that is turned off comprising the first clock and the portion of the processor that is not turned off comprising the second clock; and

the timer is configured to operate from the second clock.

9. The vital-signs patch of claim 1, wherein the timer is configured to run continuously and automatically start a new timing period when it times out.

10. The vital-signs patch of claim 1, wherein the sensor interface is configured to monitor at least one of an accelerometer, a temperature sensor, or an oxygen saturation sensor.

11. The vital-signs patch of claim 1, wherein the sensor interface is coupled to an external sensor that is operably coupled with the vital-signs patch via one of a cable or a wireless coupling.

12. The vital-signs patch of claim 1, wherein the sensor interface comprises an electronic component configured to perform one of generating an excitation signal to a sensor or providing a direct-current (DC) power to a sensor.

13. The vital-signs patch of claim 1, wherein the sensor interface comprises one of a signal generator for generating an excitation signal to a sensor coupled to the sensor interface, a voltage regulator for providing power to the sensor, an amplifier for amplifying a sensor signal from the sensor, an analog-to-digital converter for digitizing an amplified sensor signal, or a filter for filtering out noise from the sensor.

14. The vital-signs patch of claim 1, wherein the sensor interface is coupled with an internal sensor configured to

measure one of a board temperature of the vital-signs patch or a patient's motion and position.

15. A method of conserving battery power in a patch having a wireless receiver and vital-signs monitoring circuitry, comprising the steps of:

receiving a sleep signal,

turning off the wireless receiver and a portion of the vital-signs monitoring circuitry on the patch,

starting a timer on the patch with a determined period of time to generate an interrupt signal,

turning on the portion of the vital-signs monitoring circuitry that was turned off upon generating the interrupt signal,

monitoring for a sleep signal;

synchronizing the interrupt signal from the patch with the sleep signal when the sleep signal is present; and

forming a signal representative of one or more vital-signs of a patient to which the patch is attached when the portion of the vital-signs monitoring circuitry is turned on.

16. The method of claim 15, wherein forming a signal representative of one or more vital-signs comprises receiving, in a sensor interface circuit, one of a measurement of the patient's respiratory rate or a measurement of the patient's temperature.

17. The method of claim 15, further comprising generating an alarm in a hospital system when a vital-signs data read from the patch when the portion of the vital-signs monitoring circuitry is on, triggers at least one preset alarm condition.

18. The method of claim 15, wherein synchronizing the interrupt signal from the patch with the sleep signal comprises adjusting the periodicity of the sleep signal so that a rate of power consumption while the portion of the vital-signs monitoring circuitry is turned off is lower than a rate of power consumption while the entire patch is turned on.

19. The method of claim 15, wherein starting a timer on the patch comprises generating a clock signal in a portion of the patch that remains on after receiving the sleep signal.

20. The method of claim 19, wherein starting a timer comprises continuously running the timer for at least a plurality of periods of the sleep signal, the plurality of periods of the sleep signal comprising a period when the portion of the vital-signs monitoring circuitry is off.

* * * * *

专利名称(译)	用于在患者监测系统中节省电池电力的系统和方法		
公开(公告)号	US20150223706A1	公开(公告)日	2015-08-13
申请号	US14/694957	申请日	2015-04-23
申请(专利权)人(译)	CAREFUSION 303 , INC.		
当前申请(专利权)人(译)	CAREFUSION 303 , INC.		
[标]发明人	RAPTIS MARK JAFRI AMIR KATHIRESAN GANESH BURDETT ALISON OMENI OKUNDU KEY MATHEW		
发明人	RAPTIS, MARK JAFRI, AMIR KATHIRESAN, GANESH BURDETT, ALISON OMENI, OKUNDU KEY, MATHEW		
IPC分类号	A61B5/0205 A61B5/00		
CPC分类号	A61B5/02055 A61B5/6823 A61B5/6833 A61B2560/0209 A61B5/1116 A61B5/14542 A61B5/0816 A61B5/746 A61B5/0002 A61B5/002 A61B5/01 A61B5/02438 A61B5/0402 A61B5/14551 A61B2562 /0219 A61B2562/0271 G06F19/3418 G16H40/67 H04W52/0206 H04W52/0235 H04W52/0274 Y02D70 /26 Y10S370/913		
外部链接	Espacenet USPTO		

摘要(译)

公开了一种用于患者监测系统的生命体征贴片。贴片包括壳体，该壳体构造成佩戴在患者的皮肤上。外壳包含收音机，一个或多个传感器接口，处理器和电池。处理器可以选择性地关闭和打开处理器的一些部分，并可选择地关闭电源并打开至传感器接口和无线电的至少一部分。处理器包括一个定时器，每当定时器超时，它将打开处理器的所有部分并开始新的定时周期。当处理器接收到信号时，处理器将关闭至处理器的至少一部分和传感器接口的至少一部分的电源。

