



US 20190083016A1

(19) **United States**(12) **Patent Application Publication**
UEDA et al.(10) **Pub. No.: US 2019/0083016 A1**
(43) **Pub. Date: Mar. 21, 2019**(54) **MEDICAL PHOTOMETER AND MEDICAL
PHOTOMETRY SYSTEM**(71) Applicant: **NIHON KOHDEN CORPORATION,**
Tokyo (JP)(72) Inventors: **Yoshinori UEDA,** Tokorozawa-shi (JP);
Naoki KOBAYASHI, Tokorozawa-shi
(JP); **Kazumasa ITO,** Tokorozawa-shi
(JP); **Hideki FUJISAKI,**
Tokorozawa-shi (JP); **Teiji UKAWA,**
Tokorozawa-shi (JP)(73) Assignee: **NIHON KOHDEN CORPORATION,**
Tokyo (JP)(21) Appl. No.: **16/134,539**(22) Filed: **Sep. 18, 2018**(30) **Foreign Application Priority Data**

Sep. 20, 2017 (JP) 2017-180016

Publication Classification(51) **Int. Cl.**
A61B 5/1455 (2006.01)
A61B 5/00 (2006.01)
A61M 16/00 (2006.01)(52) **U.S. Cl.**CPC **A61B 5/14552** (2013.01); **A61B 5/0053**
(2013.01); **A61M 16/024** (2017.08); **A61M**
2230/205 (2013.01); **A61M 2202/0208**
(2013.01); **A61M 2205/3313** (2013.01); **A61B**
2562/0238 (2013.01)

(57)

ABSTRACT

A medical photometer includes a signal producing section that produces a first control signal to emit a first light having a first wavelength, a second control signal to emit a second light having a second wavelength, a third control signal to emit a third light having a third wavelength, and a fourth control signal to emit a fourth light having a fourth wavelength, a signal acquiring section that acquires a first to fourth intensity signals, a processor, and a memory that stores instructions. In the medical photometer, the first wavelength and the second wavelength are selected as two wavelengths at each of which an extinction coefficient of blood is a first value. The third wavelength and the fourth wavelength are selected as two wavelengths at each of which the extinction coefficient of the blood is a second value which is different from the first value.

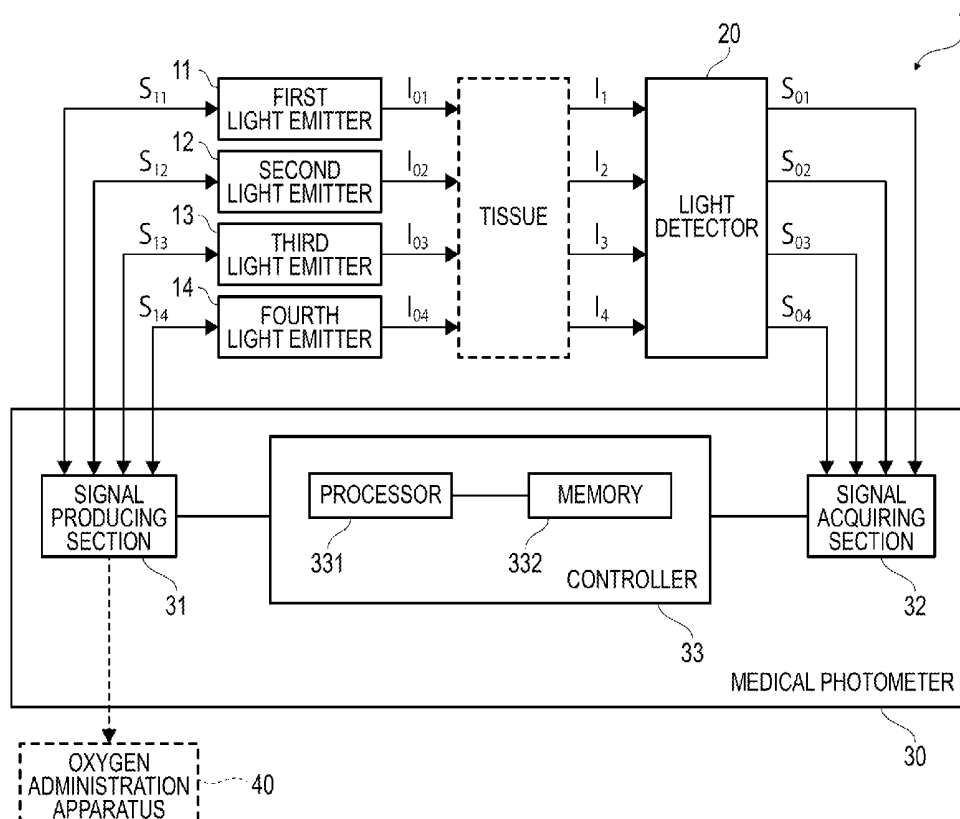


FIG. 1

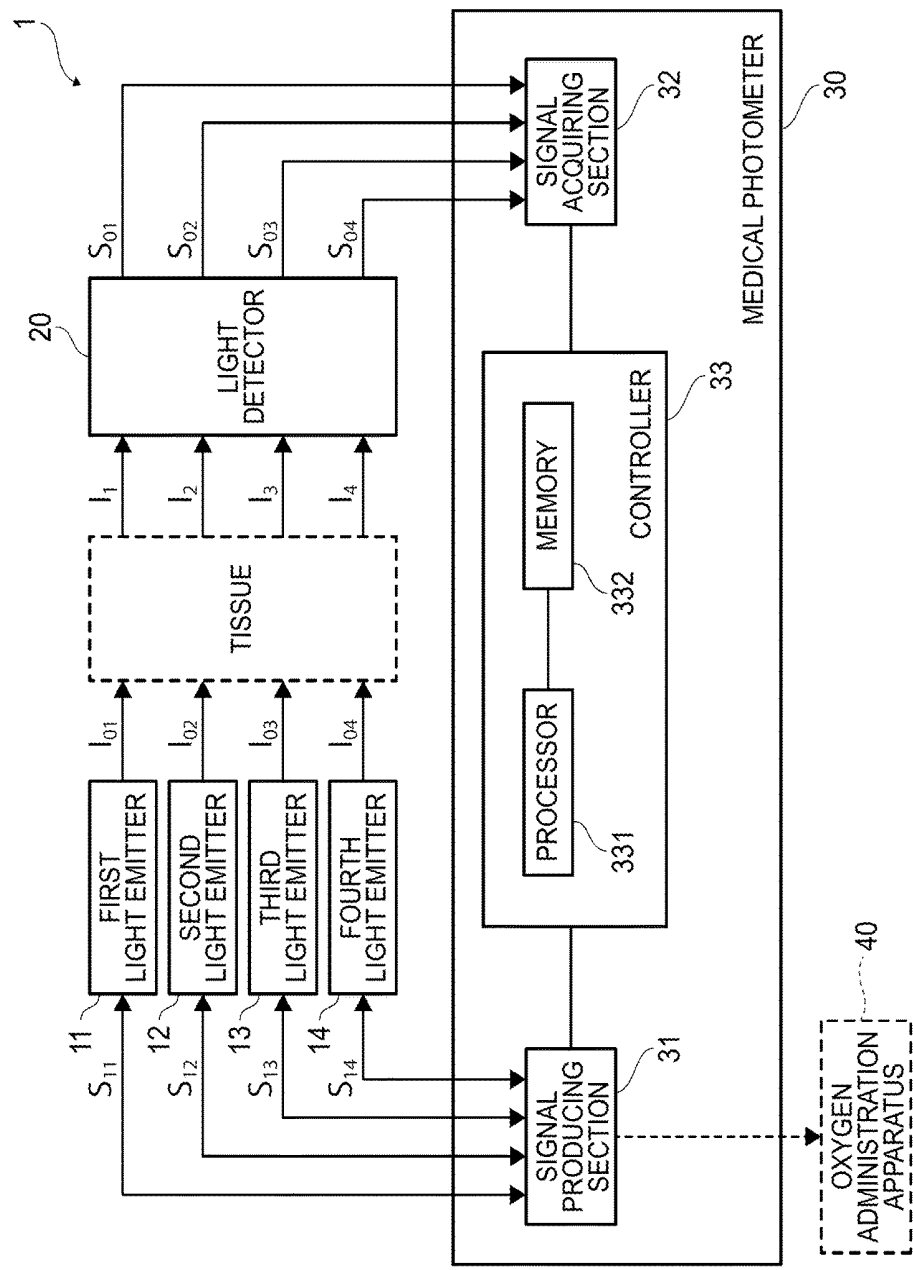


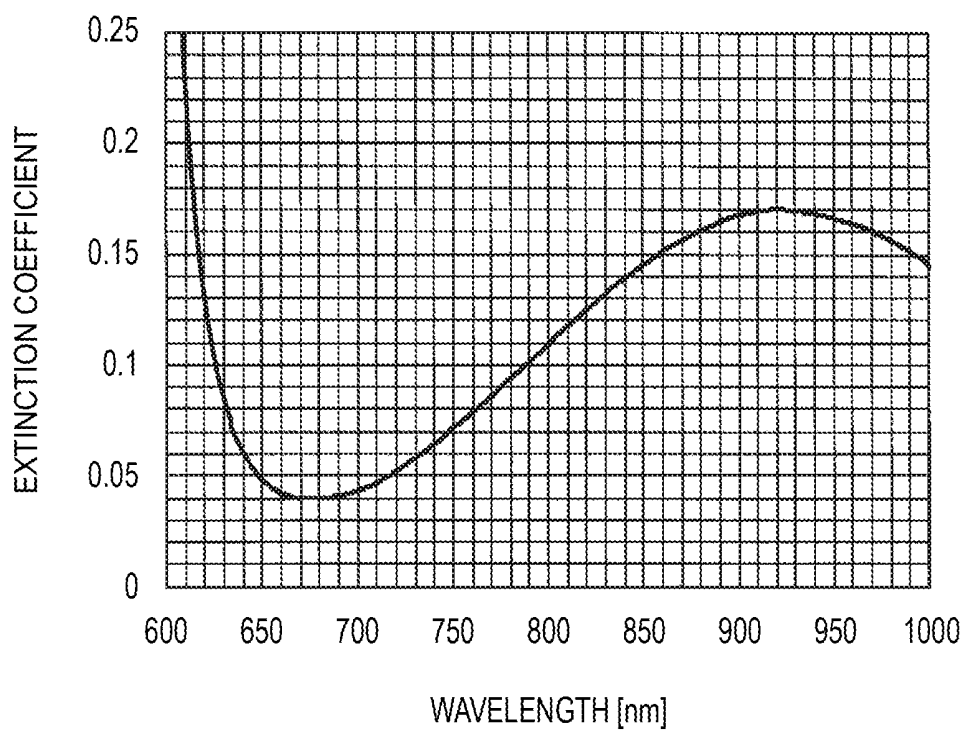
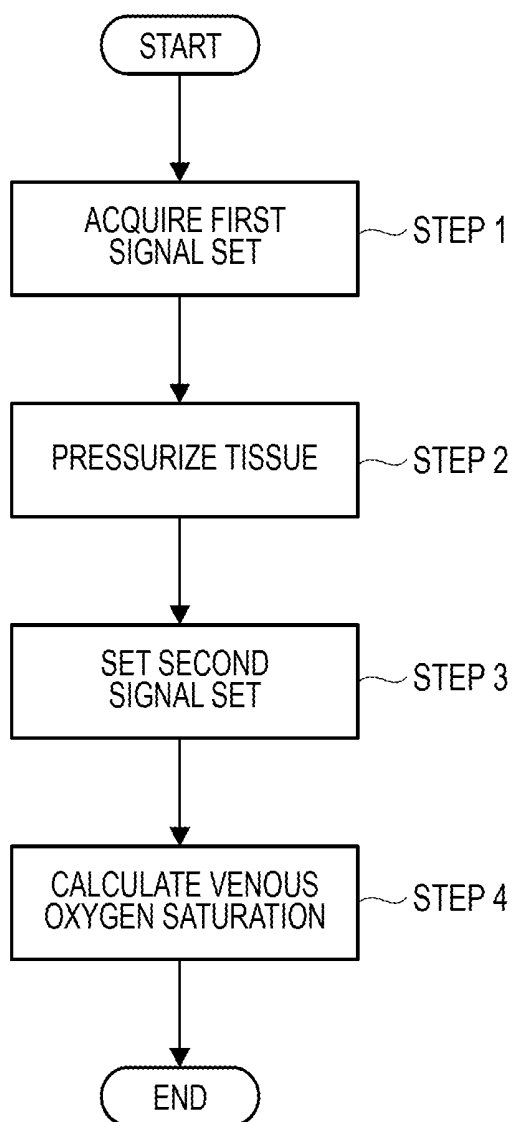
FIG. 2

FIG. 3



MEDICAL PHOTOMETER AND MEDICAL PHOTOMETRY SYSTEM

CROSS REFERENCE TO RELATED APPLICATION

[0001] This application is based on Japanese Patent Applications No. 2017-180016 filed on Sep. 20, 2017, the contents of which are incorporated herein by reference.

BACKGROUND

[0002] The presently disclosed subject matter relates to a medical photometer, and a medical photometry system including the medical photometer.

[0003] Japanese Patent No. 4,196,209 discloses a pulse photometer which is an example of a medical photometer. A pulse photometer is a device for calculating the arterial oxygen saturation of a subject as an example of the photometry. Specifically, the tissue of the subject is irradiated with light beams respectively having a plurality of wavelengths at which ratios of the extinction coefficients of the blood are different from each other. The quantities of the light beams of the respective wavelengths which are transmitted through or reflected from are detected. The quantities of the light beams of the respective wavelengths are changed in accordance with the pulsation of the blood of the subject.

[0004] Therefore, temporal changes of the quantities of the light beams of the respective wavelengths are acquired as pulse wave signals. The amplitude of the pulse wave signal relating to each of the wavelengths corresponds to the light attenuation variation at the wavelength. The arterial oxygen saturation is calculated based on a ratio of the light attenuation variations at the wavelengths.

[0005] Recently, it has been known that excessive administration of oxygen to a subject imposes a burden on the subject. In accordance with administration of oxygen, the arterial oxygen saturation in the blood of the subject is increased. Namely, the arterial oxygen saturation can be used as an index of knowing the level of administration of oxygen to the subject. When the arterial oxygen saturation reaches 100%, however, it is difficult to determine whether administration of oxygen is excessive.

[0006] A novel index which, when the arterial oxygen saturation of a subject is 100%, enables to determine whether the amount of administration of oxygen to the subject is adequate is provided.

SUMMARY

[0007] According to an aspect of the presently disclosed subject matter, a medical photometer includes:

[0008] a signal producing section that produces:

[0009] a first control signal that causes a first light emitter to emit a first light beam having a first wavelength;

[0010] a second control signal that causes a second light emitter to emit a second light beam having a second wavelength;

[0011] a third control signal that causes a third light emitter to emit a third light beam having a third wavelength; and

[0012] a fourth control signal that causes a fourth light emitter to emit a fourth light beam having a fourth wavelength;

[0013] a signal acquiring section that acquires:

[0014] a first intensity signal corresponding to an intensity of the first light beam which is transmitted through or reflected from tissue of a subject;

[0015] a second intensity signal corresponding to an intensity of the second light beam which is transmitted through or reflected from the tissue;

[0016] a third intensity signal corresponding to an intensity of the third light beam which is transmitted through or reflected from the tissue; and

[0017] a fourth intensity signal corresponding to an intensity of the fourth light beam which is transmitted through or reflected from the tissue;

[0018] a processor; and

[0019] a memory that stores instructions executable by the processor,

[0020] wherein the first wavelength and the second wavelength are selected as two wavelengths at each of which an extinction coefficient of blood in a state where an oxygen saturation is 100% is a first value,

[0021] the third wavelength and the fourth wavelength are selected as two wavelengths at each of which the extinction coefficient of the blood in a state where the oxygen saturation is 100% has a second value which is different from the first value, and,

[0022] when the instructions are executed by the processor, a venous oxygen saturation in a state where an arterial oxygen saturation of the subject is 100% is calculated based on the first control signal, the second control signal, the third control signal, the fourth control signal, the first intensity signal, the second intensity signal, the third intensity signal, and the fourth intensity signal.

[0023] According to another aspect of the presently disclosed subject matter, a medical photometry system includes:

[0024] a first light emitter that emits a first light beam having a first wavelength;

[0025] a second light emitter that emits a second light beam having a second wavelength;

[0026] a third light emitter that emits a third light beam having a third wavelength;

[0027] a fourth light emitter that emits a fourth light beam having a fourth wavelength;

[0028] a light detector that outputs a first intensity signal corresponding to an intensity of the first light beam that is transmitted through or reflected from tissue of a subject, a second intensity signal corresponding to an intensity of the second light beam that is transmitted through or reflected from the tissue, a third intensity signal corresponding to an intensity of the third light beam that is transmitted through or reflected from the tissue, and a fourth intensity signal corresponding to an intensity of the fourth light beam that is transmitted through or reflected from the tissue; and

[0029] a medical photometer to which the first light emitter, the second light emitter, the third light emitter, the fourth light emitter, and the light detector are connected with wire or wireless connection,

[0030] wherein the medical photometer includes:

[0031] a signal producing section that produces a first control signal that causes the first light emitter to emit the first light beam, a second control signal that causes the second light emitter to emit the second light beam, a third control signal that causes the third light emitter

- to emit the third light beam, and a fourth control signal that causes the fourth light emitter to emit the fourth light beam;
- [0032] a signal acquiring section that acquires the first intensity signal, the second intensity signal, the third intensity signal, and the fourth intensity signal;
- [0033] a processor; and
- [0034] a memory that stores instructions executable by the processor,
- [0035] the first wavelength and the second wavelength are selected as two wavelengths at each of which an extinction coefficient of blood in a state where an oxygen saturation is 100% has a first value,
- [0036] the third wavelength and the fourth wavelength are selected as two wavelengths at each of which the extinction coefficient of the blood in a state where the oxygen saturation is 100% has a second value that is different from the first value, and,
- [0037] when the instructions are executed by the processor, a venous oxygen saturation in a state where an arterial oxygen saturation of the subject is 100% is calculated based on the first control signal, the second control signal, the third control signal, the fourth control signal, the first intensity signal, the second intensity signal, the third intensity signal, and the fourth intensity signal.
- [0038] According to another aspect of the presently disclosed subject matter, a medical photometer includes:
- [0039] a signal acquiring section that acquires:
- [0040] a first intensity signal corresponding to an intensity of a first light beam which is transmitted through or reflected from tissue of a subject, and which has a first wavelength;
- [0041] a second intensity signal corresponding to an intensity of a second light beam which is transmitted through or reflected from the tissue, and which has a second wavelength;
- [0042] a third intensity signal corresponding to an intensity of a third light beam which is transmitted through or reflected from the tissue, and which has a third wavelength; and
- [0043] a fourth intensity signal corresponding to an intensity of a fourth light beam which is transmitted through or reflected from the tissue, and which has a fourth wavelength;
- [0044] a processor; and
- [0045] a memory that stores instructions executable by the processor,
- [0046] wherein the first wavelength and the second wavelength are selected as two wavelengths at each of which an extinction coefficient of blood in a state where an oxygen saturation is 100% has a first value,
- [0047] the third wavelength and the fourth wavelength are selected as two wavelengths at each of which the extinction coefficient of the blood in a state where the oxygen saturation is 100% has a second value that is different from the first value, and,
- [0048] when the instructions are executed by the processor, the medical photometer
- [0049] acquires a first signal set including the first intensity signal, second intensity signal, third intensity signal, and fourth intensity signal in a state where the tissue is not pressurized,
- [0050] acquires a second signal set including the first intensity signal, second intensity signal, third intensity signal, and fourth intensity signal in a state where the tissue is pressurized, and
- [0051] calculates a venous oxygen saturation in a state where an arterial oxygen saturation of the subject is 100%, based on the first signal set and the second signal set.
- [0052] According to another aspect of the presently disclosed subject matter, a medical photometry system includes:
- [0053] a first light emitter that emits a first light beam having a first wavelength;
- [0054] a second light emitter that emits a second light beam having a second wavelength;
- [0055] a third light emitter that emits a third light beam having a third wavelength;
- [0056] a fourth light emitter that emits a fourth light beam having a fourth wavelength;
- [0057] a light detector that outputs a first intensity signal corresponding to an intensity of the first light beam that is transmitted through or reflected from tissue of a subject, a second intensity signal corresponding to an intensity of the second light beam that is transmitted through or reflected from the tissue, a third intensity signal corresponding to an intensity of the third light beam that is transmitted through or reflected from the tissue, and a fourth intensity signal corresponding to an intensity of the fourth light beam that is transmitted through or reflected from the tissue; and
- [0058] a medical photometer to which the first light emitter, the second light emitter, the third light emitter, the fourth light emitter, and the light detector are connected with wire or wireless connection,
- [0059] wherein the medical photometer includes:
- [0060] a signal acquiring section that acquires the first intensity signal, the second intensity signal, the third intensity signal, and the fourth intensity signal;
- [0061] a processor; and
- [0062] a memory that stores instructions executable by the processor,
- [0063] the first wavelength and the second wavelength are selected as two wavelengths at each of which an extinction coefficient of blood in a state where an oxygen saturation is 100% has a first value.
- [0064] the third wavelength and the fourth wavelength are selected as two wavelengths at each of which the extinction coefficient of the blood in a state where the oxygen saturation is 100% has a second value that is different from the first value, and,
- [0065] when the instructions are executed by the processor, the medical photometer
- [0066] acquires a first signal set including the first intensity signal, second intensity signal, third intensity signal, and fourth intensity signal in a state where the tissue is not pressurized,
- [0067] acquires a second signal set including the first intensity signal, second intensity signal, third intensity signal, and fourth intensity signal in a state where the tissue is pressurized, and
- [0068] calculates a venous oxygen saturation in a state where an arterial oxygen saturation of the subject is 100%, based on the first signal set and the second signal set.

[0069] According to the above-described modes, even when the arterial oxygen saturation of a subject is 100%, it is possible to determine whether the amount of administration of oxygen to the subject is adequate, based on the calculated venous oxygen saturation. In other words, a novel index is provided which, when the arterial oxygen saturation of a subject is 100%, enables to determine whether the amount of administration of oxygen to the subject is adequate.

BRIEF DESCRIPTION OF DRAWINGS

[0070] FIG. 1 is a functional diagram illustrating a functional configuration of a medical photometry system of an embodiment.

[0071] FIG. 2 is a graph for explaining a principle of calculating a venous oxygen saturation.

[0072] FIG. 3 is a flowchart illustrating an operation example of a medical photometer in FIG. 1.

DETAILED DESCRIPTION OF EMBODIMENTS

[0073] Hereinafter, an embodiment will be described in detail with reference to the accompanying drawings. FIG. 1 illustrates the functional configuration of a medical photometry system 1 of the embodiment.

[0074] The medical photometry system 1 includes a first light emitter 11, a second light emitter 12, a third light emitter 13, a fourth light emitter 14, a light detector 20, and a medical photometer 30.

[0075] The first light emitter 11 is configured so as to emit a first light beam having a first wavelength λ_1 . An example of the first wavelength λ_1 is 660 nm. The first light emitter 11 is a semiconductor light emitting element which emits the first light beam. Examples of the semiconductor light emitting element are a light emitting diode (LED), a laser diode, and an organic electroluminescence (EL) element.

[0076] The second light emitter 12 is configured so as to emit a second light beam having a second wavelength λ_2 . An example of the second wavelength λ_2 is 700 nm. The second light emitter 12 is a semiconductor light emitting element which emits the second light beam. Examples of the semiconductor light emitting element are a light emitting diode (LED), a laser diode, and an organic electroluminescence (EL) element.

[0077] The third light emitter 13 is configured so as to emit a third light beam having a third wavelength λ_3 . An example of the third wavelength λ_3 is 645 nm. The third light emitter 13 is a semiconductor light emitting element which emits the third light beam. Examples of the semiconductor light emitting element are a light emitting diode (LED), a laser diode, and an organic electroluminescence (EL) element.

[0078] The fourth light emitter 14 is configured so as to emit a fourth light beam having a fourth wavelength λ_4 . An example of the fourth wavelength λ_4 is 730 nm. The fourth light emitter 14 is a semiconductor light emitting element which emits the fourth light beam. Examples of the semiconductor light emitting element are a light emitting diode (LED), a laser diode, and an organic electroluminescence (EL) element.

[0079] The light detector 20 is an optical sensor having sensitivities to the first wavelength λ_1 , the second wavelength λ_2 , the third wavelength λ_3 , and the fourth wavelength λ_4 . The light detector may be configured so as to

further have sensitivities to other wavelengths. Examples of the optical sensor are a photodiode, a phototransistor, and a photoresistor.

[0080] The light detector 20 is configured so as to output a first intensity signal S_{o1} corresponding to the intensity I_1 of the first light beam which is transmitted through or reflected from tissue of a subject. The fingertip or earlobe of the subject may be used as an example of the tissue. The light detector 20 is configured so as to output a second intensity signal S_{o2} corresponding to the intensity I_2 of the second light beam which is transmitted through or reflected from the tissue. The light detector 20 is configured so as to output a third intensity signal S_{o3} corresponding to the intensity I_3 of the third light beam which is transmitted through or reflected from the tissue. The light detector 20 is configured so as to output a fourth intensity signal S_{o4} corresponding to the intensity I_4 of the fourth light beam which is transmitted through or reflected from the tissue.

[0081] The medical photometer 30 has wired or wireless connections to the first light emitter 11, the second light emitter 12, the third light emitter 13, the fourth light emitter 14, and the light detector 20. The medical photometer 30 includes a signal producing section 31, a signal acquiring section 32, and a controller 33.

[0082] The signal producing section 31 is configured so as to produce a first control signal S_{i1} , a second control signal S_{i2} , a third control signal S_{i3} , and a fourth control signal S_{i4} . The first control signal S_{i1} causes the first light emitter 11 to emit the first light beam at a first intensity I_{o1} . The second control signal S_{i2} causes the second light emitter 12 to emit the second light beam at a second intensity I_{o2} . The third control signal S_{i3} causes the third light emitter 13 to emit the third light beam at a third intensity I_{o3} . The fourth control signal S_{i4} causes the fourth emitter 14 to emit the fourth light beam at a fourth intensity I_{o4} . The signal producing section 31 includes a circuit which produces the first control signal S_{i1} , the second control signal S_{i2} , the third control signal S_{i3} , and the fourth control signal S_{i4} in accordance with instructions from the controller 33, and an interface for outputting these signals.

[0083] The signal acquiring section 32 is configured so as to acquire the first intensity signal S_{o1} , the second intensity signal S_{o2} , the third intensity signal S_{o3} , and the fourth intensity signal S_{o4} which are output from the light detector 20. The signal acquiring section 32 includes an interface which receives inputs of the first intensity signal S_{o1} , the second intensity signal S_{o2} , the third intensity signal S_{o3} , and the fourth intensity signal S_{o4} , and a signal transmission circuit which transmits the signals to the controller 33.

[0084] The controller 33 is communicable with the signal producing section 31 and the signal acquiring section 32. The controller 33 can include one or more processor 331 and one or more memory 332.

[0085] Examples of the processor 331 include a CPU and an MPU. The memory 332 is configured so as to store instructions which may be executed by the processor 331. Examples of the memory 332 include a ROM which stores various instructions, and a RAM having a work area in which various instructions to be executed by the processor 331 are stored.

[0086] When instructions stored in the memory 332 are executed by the processor 331, the medical photometer 30 executes the following process.

[0087] The controller 33 causes the signal producing section 31 to produce the first control signal S_{i1} . Therefore, the first light emitter 11 emits the first light beam having the first wavelength λ_1 , at the first intensity I_{01} . The light detector 20 receives the first light beam which is transmitted through or reflected from the tissue of the subject, and outputs the first intensity signal S_{o1} corresponding to the intensity I_1 of the first light beam. The controller 33 causes the signal acquiring section 32 to acquire the first intensity signal S_{o1} .

[0088] A light attenuation (first light attenuation) A_1 of the first light beam by transmission through or reflection from the tissue is acquired based on the first intensity signal S_{o1} . The first light attenuation A_1 is expressed by the following expression. Namely, the first light attenuation A_1 may be acquired based on the first control signal S_{i1} and the first intensity signal S_{o1} .

$$A_1 = \ln(I_{01}/I_1) \quad (1)$$

[0089] The controller 33 causes the signal producing section 31 to produce the second control signal S_{i2} . Therefore, the second light emitter 12 emits the second light beam having the second wavelength λ_2 , at the second intensity I_{02} . The light detector 20 receives the second light beam which is transmitted through or reflected from the tissue of the subject, and outputs the second intensity signal S_{o2} corresponding to the intensity I_2 of the second light beam. The controller 33 causes the signal acquiring section 32 to acquire the second intensity signal S_{o2} .

[0090] A light attenuation (second light attenuation) A_2 of the second light beam due to transmission through or reflection from the tissue is acquired based on the second intensity signal S_{o2} . The second light attenuation A_2 is expressed by the following expression. Namely, the second light attenuation A_2 may be acquired based on the second control signal S_{i2} and the second intensity signal S_{o2} .

$$A_2 = \ln(I_{02}/I_2) \quad (2)$$

[0091] The first light attenuation A_1 and the second light attenuation A_2 may be expressed by the following expressions, respectively:

$$A_1 = (E_{a1} \cdot Hb \cdot D_a + E_{v1} \cdot Hb \cdot D_v + \Sigma_{t1} \cdot D_t) \quad (3)$$

$$A_2 = (E_{a2} \cdot Hb \cdot D_a + E_{v2} \cdot Hb \cdot D_v + \Sigma_{t2} \cdot D_t) \quad (4)$$

[0092] In the above expressions, E_a indicates the extinction coefficient ($\text{dl g}^{-1} \text{cm}^{-1}$) of the arterial blood, E_v indicates the extinction coefficient ($\text{dl g}^{-1} \text{cm}^{-1}$) of the venous blood, and Σ_t indicates the absorption coefficient (cm^{-1}) due to tissue other than the blood. The suffix “1” indicates the first light beam, and the suffix “2” indicates the second light beam. Hb indicates the hemoglobin concentration in blood (g dl^{-1}), D_a indicates the thickness (cm) of the arterial blood, D_v indicates the thickness (cm) of the venous blood, and D_t indicates the thickness (cm) of the tissue other than the blood.

[0093] In Expressions (3) and (4), namely, the first term of the right side corresponds to the extent of contribution of the arterial blood of the subject to the light attenuation, the second term of the right side corresponds to the extent of contribution of the venous blood of the subject to the light attenuation, and the third term of the right side corresponds to the extent of contribution of the tissue of the subject other than the blood to the light attenuation.

[0094] FIG. 2 illustrates the wavelength dependency of the extinction coefficient of the blood in a state where the

oxygen saturation is 100%. In the embodiment, the first wavelength λ_1 (660 nm) and the second wavelength λ_2 (700 nm) are selected as two wavelengths at which the extinction coefficients of the blood in a state where the oxygen saturation is 100% have first values that are substantially equal to each other.

[0095] Under conditions that the oxygen saturation of the blood of the subject is 100%, namely, E_{a1} and E_{a2} in Expressions (3) and (4) may be deemed to be approximately equal to each other. When also Σ_{t1} and Σ_{t2} are deemed to be approximately equal to each other, the following expression is obtained:

$$A_1 - A_2 \approx E_{v1} \cdot Hb \cdot D_v - E_{v2} \cdot Hb \cdot D_v = (E_{v1} - E_{v2}) Hb \cdot D_v \quad (5)$$

[0096] From Expressions (1) and (2), the left side of Expression (5) may be rewritten as follows:

$$\ln(I_2/I_1) - \ln(I_{02}/I_{01}) = (E_{v1} - E_{v2}) Hb \cdot D_v \quad (6)$$

[0097] In Expression (6), the first term of the left side corresponds to the ratio of the first intensity signal S_{o1} and second intensity signal S_{o2} which are acquired by the signal acquiring section 32. The values of I_{01} and I_{02} are already known, and therefore the second term of the left side is constant. When first and second light beams are selected as two beams for which the extinction coefficients of the blood in a state where the oxygen saturation is 100% are substantially equal to each other, namely, it is possible to offset influences on extinction due to the arterial blood and the tissue relating to the first and second light beams.

[0098] The controller 33 causes the signal producing section 31 to produce the third control signal S_{i3} . Therefore, the third light emitter 13 emits the third light beam having the third wavelength λ_3 , at the third intensity I_{03} . The light detector 20 receives the third light beam which is transmitted through or reflected from the tissue of the subject, and outputs the third intensity signal S_{o3} corresponding to the intensity I_3 of the third light beam. The controller 33 causes the signal acquiring section 32 to acquire the third intensity signal S_{o3} .

[0099] A light attenuation (third light attenuation) A_3 of the third light beam due to transmission through or reflection from the tissue is acquired based on the third intensity signal S_{o3} . The third light attenuation A_3 is expressed by the following expression. Namely, the third light attenuation A_3 may be acquired based on the third control signal S_{i3} and the third intensity signal S_{o3} .

$$A_3 = \ln(I_{03}/I_3) \quad (7)$$

[0100] The controller 33 causes the signal producing section 31 to produce the fourth control signal S_{i4} . Therefore, the fourth light emitter 14 emits the fourth light beam having the fourth wavelength λ_4 , at the fourth intensity I_{04} . The light detector 20 receives the fourth light beam which is transmitted through or reflected from the tissue of the subject, and outputs the fourth intensity signal S_{o4} corresponding to the intensity I_4 of the fourth light beam. The controller 33 causes the signal acquiring section 32 to acquire the fourth intensity signal S_{o4} .

[0101] A light attenuation (fourth light attenuation) A_4 of the fourth light beam due to transmission through or reflection from the tissue is acquired based on the fourth intensity signal S_{o4} . The fourth light attenuation A_4 is expressed by the following expression. Namely, the fourth light attenuation A_4 may be acquired based on the fourth control signal S_{i4} and the fourth intensity signal S_{o4} .

$$A_4 = \ln(I_{04}/I_4) \quad (8)$$

[0102] The third light attenuation A_3 and the fourth light attenuation A_4 may be expressed by the following expressions, respectively:

$$A_3 = (E_{a3} \cdot Hb \cdot D_a + E_{v3} \cdot Hb \cdot D_v + \Sigma_{t3} \cdot D_t) \quad (9)$$

$$A_4 = (E_{a4} \cdot Hb \cdot D_a + E_{v4} \cdot Hb \cdot D_v + \Sigma_{t4} \cdot D_t) \quad (10)$$

[0103] In the above expressions, E_a indicates the extinction coefficient ($\text{dl g}^{-1} \text{cm}^{-1}$) of the arterial blood, E_v indicates the extinction coefficient ($\text{dl g}^{-1} \text{cm}^{-1}$) of the venous blood, and Σ_t indicates the absorption coefficient (cm^{-1}) due to tissue other than the blood. The suffix “3” indicates the third light beam, and the suffix “4” indicates the fourth light beam. Hb indicates the hemoglobin concentration in blood (g dl^{-1}), D_a indicates the thickness (cm) of the arterial blood, D_v indicates the thickness (cm) of the venous blood, and D_t indicates the thickness (cm) of the tissue other than the blood.

[0104] In Expressions (9) and (10), namely, the first term of the right side corresponds to the extent of contribution of the arterial blood of the subject to the light attenuation, the second term of the right side corresponds to the extent of contribution of the venous blood of the subject to the light attenuation, and the third term of the right side corresponds to the extent of contribution of the tissue of the subject other than the blood to the light attenuation.

[0105] As illustrated in FIG. 2, the third wavelength λ_3 (645 nm) and the fourth wavelength λ_4 (730 nm) are selected as two wavelengths at which the extinction coefficients of the blood in a state where the oxygen saturation is 100% have second values that are substantially equal to each other. The second values are different from the above-described first values.

[0106] Under the conditions that the oxygen saturation of the blood of the subject is 100%, namely, E_{a3} and E_{a4} in Expressions (9) and (10) may be deemed to be approximately equal to each other. When also Σ_{t3} and Σ_{t4} are deemed to be approximately equal to each other, the following expression is obtained:

$$A_3 - A_4 \approx E_{v3} \cdot Hb \cdot D_v - E_{v4} \cdot Hb \cdot D_v = (E_{v3} - E_{v4}) Hb \cdot D_v \quad (11)$$

[0107] From Expressions (7) and (8), the left side of Expression (11) may be rewritten as follows:

$$\ln(I_4/I_3) - \ln(I_{04}/I_{03}) = (E_{v3} - E_{v4}) Hb \cdot D_v \quad (12)$$

[0108] In Expression (12), the first term of the left side corresponds to the ratio of the third intensity signal S_{o3} and fourth intensity signal S_{o4} which are acquired by the signal acquiring section 32. The values of I_{03} and I_{04} are already known, and therefore the second term of the left side is constant. When first and second light beams are selected as two beams for which the extinction coefficients of the blood in a state where the oxygen saturation is 100% are substantially equal to each other, namely, it is possible to offset influences on extinction due to the arterial blood and the tissue relating to the third and fourth light beams.

[0109] From Expressions (6) and (12), moreover, the following expression is obtained:

$$\frac{[\ln(I_4/I_3) - \ln(I_{04}/I_{03})] / [\ln(I_2/I_1) - \ln(I_{02}/I_{01})]}{(E_{v1} - E_{v2})} = (E_{v3} - E_{v4}) \quad (13)$$

[0110] When two sets of two light beams for which the extinction coefficients of the blood in a state where the oxygen saturation is 100% are substantially equal to each

other are used, namely, it is possible to offset influences on extinction due to at least one of the thickness variation of the venous blood and the variation of the hemoglobin concentration in blood. The venous oxygen saturation of the subject may be expressed as the function of the right side of Expression (13).

[0111] When instructions stored in the memory 332 are executed by the processor 331, the medical photometer 30 calculates the venous oxygen saturation in a state where the arterial oxygen saturation of the subject is 100%, based on the first control signal S_{i1} , the second control signal S_{i2} , the third control signal S_{i3} , the fourth control signal S_{i4} , the first intensity signal S_{o1} , the second intensity signal S_{o2} , the third intensity signal S_{o3} , and the fourth intensity signal S_{o4} .

[0112] According to the configuration, even when the arterial oxygen saturation of a subject is 100%, it is possible to determine whether the amount of administration of oxygen to the subject is adequate, based on the calculated venous oxygen saturation. In other words, a novel index is provided which, when the arterial oxygen saturation of a subject is 100%, enables to determine whether the amount of administration of oxygen to the subject is adequate.

[0113] Although not illustrated, the medical photometer 30 includes a notifying section. The notifying section notifies the user of the calculated venous oxygen saturation by using at least one of visual notification, audible notification, and haptic notification. The notifying section may be configured so as to perform the notification only in the case where the calculated venous oxygen saturation suggests excessive administration of oxygen to the subject.

[0114] As illustrated by the broken line in FIG. 1, the medical photometer 30 may be connected to an oxygen administration apparatus 40 with wire or wireless connection. The oxygen administration apparatus 40 is an apparatus for administering oxygen to the subject. In this case, the medical photometer 30 may cause the signal producing section 31 to produce a control signal S which controls the operation of the oxygen administration apparatus 40, based on the calculated venous oxygen saturation.

[0115] In the case where the calculated venous oxygen saturation suggests insufficient administration of oxygen, for example, the signal producing section 31 is caused to produce a control signal which controls the oxygen administration apparatus 40 so as to increase the amount of administration of oxygen. In the case where the calculated venous oxygen saturation suggests excessive administration of oxygen, the signal producing section 31 is caused to produce a control signal which controls the oxygen administration apparatus 40 so as to decrease the amount of administration of oxygen.

[0116] According to the configuration, adequate administration of oxygen under a situation where the arterial oxygen saturation of a subject is 100% can be automated.

[0117] JP-A-2014-147473 discloses a technique in which an influence on extinction due to the tissue of the subject in calculation of the arterial oxygen saturation is eliminated by pressurizing the tissue to evacuate the blood. Specifically, the tissue of the subject is irradiated by first and second light beams of different wavelengths. In a first state where the tissue is not pressurized, received light intensities of the first and second light beams are acquired. In a second state where the tissue is pressurized, then, received light intensities of the first and second light beams are acquired. A first light attenuation is acquired from the received light intensity of

the first light beam which is acquired in the first state, and that of the first light beam which is acquired in the second state. A second light attenuation is acquired from the received light intensity of the second light beam which is acquired in the first state, and that of the second light beam which is acquired in the second state. The arterial oxygen saturation of the subject is calculated based on the difference between the first light attenuation and the second light attenuation.

[0118] Referring to the technique, Expressions (1), (2), (7), and (8) may be rewritten respectively as follows:

$$A_1 = \ln(I_{21}/I_{11}) \quad (14)$$

$$A_2 = \ln(I_{22}/I_{12}) \quad (15)$$

$$A_3 = \ln(I_{23}/I_{13}) \quad (16)$$

$$A_4 = \ln(I_{24}/I_{14}) \quad (17)$$

In the above, I_{11} , I_{12} , I_{13} , and I_{14} indicate the intensities of the first, second, third, and fourth light beams which are acquired by the light detector 20 in a first state, respectively, and I_{21} , I_{22} , I_{23} , and I_{24} indicate the intensities of the first, second, third, and fourth light beams which are acquired by the light detector 20 in a second state, respectively. The first state corresponds to a state where the tissue of the subject is not pressurized. The second state corresponds to a state where the tissue of the subject is pressurized.

[0119] Expression (18) is obtained based on the description referring to Expressions (3) to (6). Similarly, Expression (19) is obtained based on the description referring to Expressions (9) to (12).

$$\ln(I_{12}/I_{11}) - \ln(I_{22}/I_{21}) = (E_{v1} - E_{v2})Hb \cdot D_v \quad (18)$$

$$\ln(I_{14}/I_{13}) - \ln(I_{24}/I_{23}) = (E_{v1} - E_{v2})Hb \cdot D_v \quad (19)$$

[0120] Then, the following expression is obtained based on the description referring to Expression (13):

$$[\ln(I_{14}/I_{13}) - \ln(I_{24}/I_{23})] / [\ln(I_{12}/I_{11}) - \ln(I_{22}/I_{21})] = (E_{v3} - E_{v4}) / (E_{v1} - E_{v2}) \quad (20)$$

[0121] The intensity I_{11} of the first light beam, intensity I_{12} of the second light beam, intensity I_{13} of the third light beam, and intensity I_{14} of the fourth light beam which are acquired by the light detector 20 in the first state correspond to the first intensity signal S_{o1} , the second intensity signal S_{o2} , the third intensity signal S_{o3} , and the fourth intensity signal S_{o4} which are acquired from the light detector 20 in the first state, respectively. The intensity I_{21} of the first light beam, intensity I_{22} of the second light beam, intensity I_{23} of the third light beam, and intensity I_{24} of the fourth light beam which are acquired by the light detector 20 in the second state correspond to the first intensity signal S_{o1} , the second intensity signal S_{o2} , the third intensity signal S_{o3} , and the fourth intensity signal S_{o4} which are acquired from the light detector 20 in the second state, respectively.

[0122] Therefore, the venous oxygen saturation in a state where the arterial oxygen saturation of the subject is 100% may be calculated based on: a first signal set including the first intensity signal S_{o1} , the second intensity signal S_{o2} , the third intensity signal S_{o3} , and the fourth intensity signal S_{o4} which are acquired in the first state; and a second signal set including the first intensity signal S_{o1} , the second intensity signal S_{o2} , the third intensity signal S_{o3} , and the fourth intensity signal S_{o4} which are acquired in the second state.

FIG. 3 illustrates an example of the operation of the medical photometer 30 which is based on the technique.

[0123] In the state where the tissue is not pressurized, firstly, the first signal set including the first intensity signal S_{o1} , the second intensity signal S_{o2} , the third intensity signal S_{o3} , and the fourth intensity signal S_{o4} is acquired (STEP 1).

[0124] Then, the tissue is pressurized (STEP 2). The pressurization may be performed by the hand of the user, or by a cuff

[0125] In the case where the pressurization is performed by the hand of the user, it is preferable to notify the user of the timing of the pressurization by using at least one of visual notification, audible notification, and haptic notification. The notification may function as a trigger for the medical photometer 30 to acquire the second signal set. Alternatively, the user may input the timing of pressurization to the medical photometer 30 by operating a button or the like.

[0126] In the case where the pressurization is performed by a cuff, the medical photometer 30 may include a pressure controller which controls the internal pressure of the cuff. The pressure controller may include a pump. The operation of the pressure controller may be controlled by the controller 33. The pressurization by the cuff may be performed in response to, for example, a button operation conducted by the user, or automatically by the controller 33.

[0127] In the state where the tissue is pressurized, the second signal set including the first intensity signal S_{o1} , the second intensity signal S_{o2} , the third intensity signal S_{o3} , and the fourth intensity signal S_{o4} is acquired (STEP 3).

[0128] Then, the venous oxygen saturation in a state where the arterial oxygen saturation of the subject is 100% is calculated based on the acquired first and second signal sets (STEP 4).

[0129] According to the configuration, simply by changing the pressurization state of the tissue, the venous oxygen saturation in a state where the arterial oxygen saturation of the subject is 100% may be calculated based on only the first intensity signal S_{o1} , the second intensity signal S_{o2} , the third intensity signal S_{o3} , and the fourth intensity signal S_{o4} which are acquired from the light detector 20. Even when the arterial oxygen saturation of a subject is 100%, namely, it is possible to determine whether the amount of administration of oxygen to the subject is adequate, based on the calculated venous oxygen saturation.

[0130] In the example, the state where the tissue is not pressurized corresponds to the first signal set, and the state where the tissue is pressurized corresponds to the second signal set. Alternatively, the state where the tissue is pressurized may correspond to the first signal set, and the state where the tissue is not pressurized may correspond to the second signal set.

[0131] The above-described embodiment is a mere example for facilitating understanding of the presently disclosed subject matter. The configuration of the embodiment may be adequately changed or improved without departing from the spirit of the presently disclosed subject matter. It is obvious that equivalents are included within the technical scope of the presently disclosed subject matter.

[0132] In the above-described embodiment, 660 nm and 700 nm are selected as the set of the first wavelength λ_1 and the second wavelength λ_2 , and 645 nm and 730 nm are selected as the set of the third wavelength λ_3 and the fourth wavelength λ_4 . However, at least one of the two sets may be

changed to arbitrary two wavelengths at which the extinction coefficients of the blood in a state where the oxygen saturation is 100% are substantially equal to each other.

[0133] Only the configuration for calculating the venous oxygen saturation of a subject is disposed in the above-described embodiment. However, a configuration for calculating the arterial oxygen saturation of the subject may be disposed. In this case, at least one of components (light emitters, a light detector, a signal producing section, a signal acquiring section, a controller, and the like) may be shared with a corresponding component in the embodiment and for calculating the venous oxygen saturation. The value of the calculated arterial oxygen saturation may be used for determining insufficient administration of oxygen to the subject.

What is claimed is:

1. A medical photometer comprising:

a signal producing section configured to produce:

- a first control signal that causes a first light emitter to emit a first light beam having a first wavelength;
- a second control signal that causes a second light emitter to emit a second light beam having a second wavelength;
- a third control signal that causes a third light emitter to emit a third light beam having a third wavelength; and
- a fourth control signal that causes a fourth light emitter to emit a fourth light beam having a fourth wavelength;

a signal acquiring section configured to acquire:

- a first intensity signal corresponding to an intensity of the first light beam which is transmitted through or reflected from tissue of a subject;
- a second intensity signal corresponding to an intensity of the second light beam which is transmitted through or reflected from the tissue;
- a third intensity signal corresponding to an intensity of the third light beam which is transmitted through or reflected from the tissue; and
- a fourth intensity signal corresponding to an intensity of the fourth light beam which is transmitted through or reflected from the tissue;

a processor; and

a memory that stores instructions executable by the processor,

wherein the first wavelength and the second wavelength are selected as two wavelengths at each of which an extinction coefficient of blood in a state where an oxygen saturation is 100% has a first value,

the third wavelength and the fourth wavelength are selected as two wavelengths at each of which the extinction coefficient of the blood in a state where the oxygen saturation is 100% has a second value which is different from the first value, and,

when the instructions are executed by the processor, a venous oxygen saturation in a state where an arterial oxygen saturation of the subject is 100% is calculated based on the first control signal, the second control signal, the third control signal, the fourth control signal, the first intensity signal, the second intensity signal, the third intensity signal, and the fourth intensity signal.

2. The medical photometer according to claim 1, wherein the first wavelength is 660 nm, the second wavelength is 700 nm,

the third wavelength is 645 nm, and the fourth wavelength is 730 nm.

3. The medical photometer according to claim 1, wherein, when the instructions are executed by the processor, the signal producing section is caused to produce a control signal which controls an operation of an oxygen administration apparatus for administering oxygen to the subject, based on the calculated venous oxygen saturation.

4. A medical photometry system comprising:

- a first light emitter that emits a first light beam having a first wavelength;
- a second light emitter that emits a second light beam having a second wavelength;
- a third light emitter that emits a third light beam having a third wavelength;
- a fourth light emitter that emits a fourth light beam having a fourth wavelength;

a light detector that outputs a first intensity signal corresponding to an intensity of the first light beam that is transmitted through or reflected from tissue of a subject, a second intensity signal corresponding to an intensity of the second light beam that is transmitted through or reflected from the tissue, a third intensity signal corresponding to an intensity of the third light beam that is transmitted through or reflected from the tissue, and a fourth intensity signal corresponding to an intensity of the fourth light beam that is transmitted through or reflected from the tissue; and

a medical photometer to which the first light emitter, the second light emitter, the third light emitter, the fourth light emitter, and the light detector are connected with wire or wireless connection,

wherein the medical photometer includes:

a signal producing section configured to produce a first control signal that causes the first light emitter to emit the first light beam, a second control signal that causes the second light emitter to emit the second light beam, a third control signal that causes the third light emitter to emit the third light beam, and a fourth control signal that causes the fourth light emitter to emit the fourth light beam;

a signal acquiring section configured to acquire the first intensity signal, the second intensity signal, the third intensity signal, and the fourth intensity signal;

a processor; and

a memory that stores instructions executable by the processor,

the first wavelength and the second wavelength are selected as two wavelengths at each of which an extinction coefficient of blood in a state where an oxygen saturation is 100% has a first value,

the third wavelength and the fourth wavelength are selected as two wavelengths at each of which the extinction coefficient of the blood in a state where the oxygen saturation is 100% has a second value that is different from the first value, and,

when the instructions are executed by the processor, a venous oxygen saturation in a state where an arterial oxygen saturation of the subject is 100% is calculated based on the first control signal, the second control signal, the third control signal, the fourth control signal, the first intensity signal, the second intensity signal, the third intensity signal, and the fourth intensity signal.

5. A medical photometer comprising:
 a signal acquiring section configured to acquire:
 a first intensity signal corresponding to an intensity of
 a first light beam which is transmitted through or
 reflected from tissue of a subject, and which has a
 first wavelength;
 a second intensity signal corresponding to an intensity
 of a second light beam which is transmitted through
 or reflected from the tissue, and which has a second
 wavelength;
 a third intensity signal corresponding to an intensity of
 a third light beam which is transmitted through or
 reflected from the tissue, and which has a third
 wavelength; and
 a fourth intensity signal corresponding to an intensity
 of a fourth light beam which is transmitted through
 or reflected from the tissue, and which has a fourth
 wavelength;
 a processor; and
 a memory that stores instructions executable by the pro-
 cessor,
 wherein the first wavelength and the second wavelength
 are selected as two wavelengths at each of which an
 extinction coefficient of blood in a state where an
 oxygen saturation is 100% has a first value,
 the third wavelength and the fourth wavelength are
 selected as two wavelengths at each of which the
 extinction coefficient of the blood in a state where the
 oxygen saturation is 100% has a second value that is
 different from the first value, and,
 when the instructions are executed by the processor, the
 medical photometer
 acquires a first signal set including the first intensity
 signal, second intensity signal, third intensity signal,
 and fourth intensity signal in a state where the tissue
 is not pressurized,
 acquires a second signal set including the first intensity
 signal, second intensity signal, third intensity signal,
 and fourth intensity signal in a state where the tissue
 is pressurized, and
 calculates a venous oxygen saturation in a state where
 an arterial oxygen saturation of the subject is 100%,
 based on the first signal set and the second signal set.

6. The medical photometer according to claim 5, wherein
 the first wavelength is 660 nm,
 the second wavelength is 700 nm,
 the third wavelength is 645 nm, and
 the fourth wavelength is 730 nm.

7. The medical photometer according to claim 5 further
 comprising a signal producing section that produces a con-
 trol signal which controls an operation of an oxygen admin-
 istration apparatus for administering oxygen to the subject,
 and,
 when the instructions are executed by the processor, the
 signal producing section is caused to produce the
 control signal, based on the calculated venous oxygen
 saturation.

8. A medical photometry system comprising:
 a first light emitter that emits a first light beam having a
 first wavelength;
 a second light emitter that emits a second light beam
 having a second wavelength;
 a third light emitter that emits a third light beam having
 a third wavelength;
 a fourth light emitter that emits a fourth light beam having
 a fourth wavelength;
 a light detector that outputs a first intensity signal corre-
 sponding to an intensity of the first light beam that is
 transmitted through or reflected from tissue of a sub-
 ject, a second intensity signal corresponding to an
 intensity of the second light beam that is transmitted
 through or reflected from the tissue, a third intensity
 signal corresponding to an intensity of the third light
 beam that is transmitted through or reflected from the
 tissue, and a fourth intensity signal corresponding to an
 intensity of the fourth light beam that is transmitted
 through or reflected from the tissue; and
 a medical photometer to which the first light emitter, the
 second light emitter, the third light emitter, the fourth
 light emitter, and the light detector are connected with
 wire or wireless connection,
 wherein the medical photometer includes:
 a signal acquiring section configured to acquire the first
 intensity signal, the second intensity signal, the third
 intensity signal, and the fourth intensity signal;
 a processor; and
 a memory that stores instructions executable by the
 processor,
 the first wavelength and the second wavelength are
 selected as two wavelengths at each of which an
 extinction coefficient of blood in a state where an
 oxygen saturation is 100% has a first value,
 the third wavelength and the fourth wavelength are
 selected as two wavelengths at each of which the
 extinction coefficient of the blood in a state where the
 oxygen saturation is 100% has a second value that is
 different from the first value, and,
 when the instructions are executed by the processor, the
 medical photometer
 acquires a first signal set including the first intensity
 signal, second intensity signal, third intensity signal,
 and fourth intensity signal in a state where the tissue
 is not pressurized,
 acquires a second signal set including the first intensity
 signal, second intensity signal, third intensity signal,
 and fourth intensity signal in a state where the tissue
 is pressurized, and
 calculates a venous oxygen saturation in a state where
 an arterial oxygen saturation of the subject is 100%,
 based on the first signal set and the second signal set.

* * * * *

专利名称(译)	医用光度计和医学测光系统		
公开(公告)号	US20190083016A1	公开(公告)日	2019-03-21
申请号	US16/134539	申请日	2018-09-18
[标]申请(专利权)人(译)	日本光电工业株式会社		
申请(专利权)人(译)	日本光电公司		
当前申请(专利权)人(译)	日本光电公司		
[标]发明人	UEDA YOSHINORI KOBAYASHI NAOKI ITO KAZUMASA FUJISAKI HIDEKI UKAWA TEIJI		
发明人	UEDA, YOSHINORI KOBAYASHI, NAOKI ITO, KAZUMASA FUJISAKI, HIDEKI UKAWA, TEIJI		
IPC分类号	A61B5/1455 A61B5/00 A61M16/00		
CPC分类号	A61B5/14552 A61B5/0053 A61M16/024 A61B2562/0238 A61M2202/0208 A61M2205/3313 A61M2230/205 A61B2562/04		
优先权	2017180016 2017-09-20 JP		
外部链接	Espacenet USPTO		

摘要(译)

医用光度计包括：信号产生部分，其产生第一控制信号以发射具有第一波长的第一光；第二控制信号以发射具有第二波长的第二光；第三控制信号以发射具有第三波长的第三光。波长和用于发射具有第四波长的第四光的第四控制信号，获取第一至第四强度信号的信号获取部分，处理器和存储指令的存储器。在医用光度计中，选择第一波长和第二波长作为两个波长，在每个波长处血液的消光系数是第一值。选择第三波长和第四波长作为两个波长，在每个波长处血液的消光系数是与第一值不同的第二值。

