



US 20200022606A1

(19) **United States**

(12) **Patent Application Publication**
Barbre et al.

(10) **Pub. No.: US 2020/0022606 A1**

(43) **Pub. Date: Jan. 23, 2020**

(54) **METHODS AND APPARATUS FOR IMPROVED SIGNAL ROBUSTNESS FOR A WEARABLE NEUROMUSCULAR RECORDING DEVICE**

Publication Classification

(51) **Int. Cl.**
A61B 5/0488 (2006.01)
A61B 5/00 (2006.01)
(52) **U.S. Cl.**
CPC *A61B 5/0488* (2013.01); *A61B 2562/04* (2013.01); *A61B 2560/0406* (2013.01); *A61B 5/6801* (2013.01)

(71) Applicant: **CTRL-labs Corporation**, New York, NY (US)

(72) Inventors: **Curtis Barbre**, Brooklyn, NY (US);
Jonathan Reid, Brooklyn, NY (US);
Ning Guo, Brooklyn, NY (US);
Brandon Pool, New York, NY (US)

(73) Assignee: **CTRL-labs Corporation**, New York, NY (US)

(21) Appl. No.: **16/516,777**


(22) Filed: **Jul. 19, 2019**

Related U.S. Application Data

(60) Provisional application No. 62/700,434, filed on Jul. 19, 2018.

(57) **ABSTRACT**

Arrangements for improving neuromuscular recording electrode contact with a body surface are described. According to some aspects, a sensor assembly may include a housing and one or more electrodes that are moveable relative to the housing. The electrodes may rotate and/or translate relative to the housing and/or have at least two degrees of freedom relative to the housing. The sensor may include a spring element that stores potential energy and biases the electrodes toward a starting position in which the electrodes extend at least partially out of the sensor housing. In some embodiments, application of a contact force to one or more of the electrodes of the sensor compresses the spring element, causing the spring element to store potential energy.

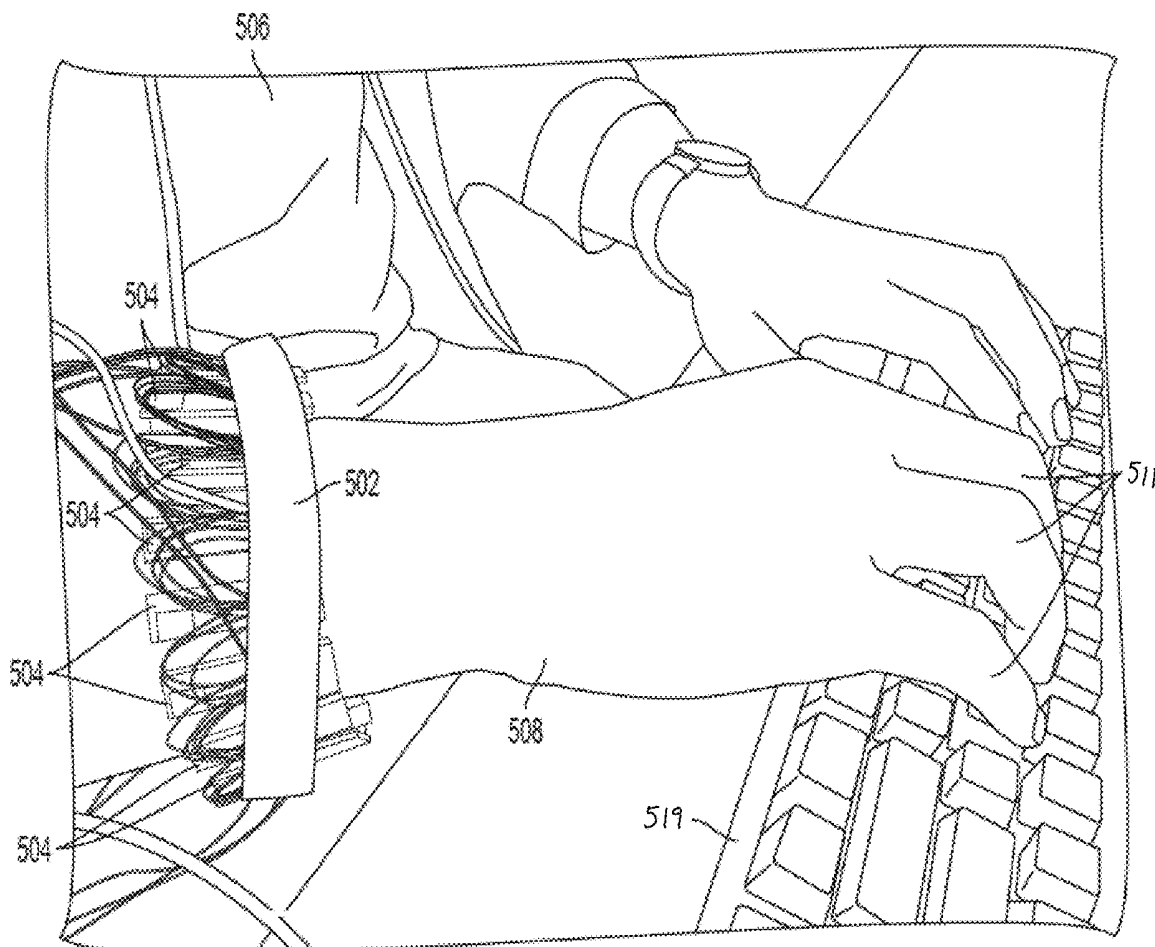

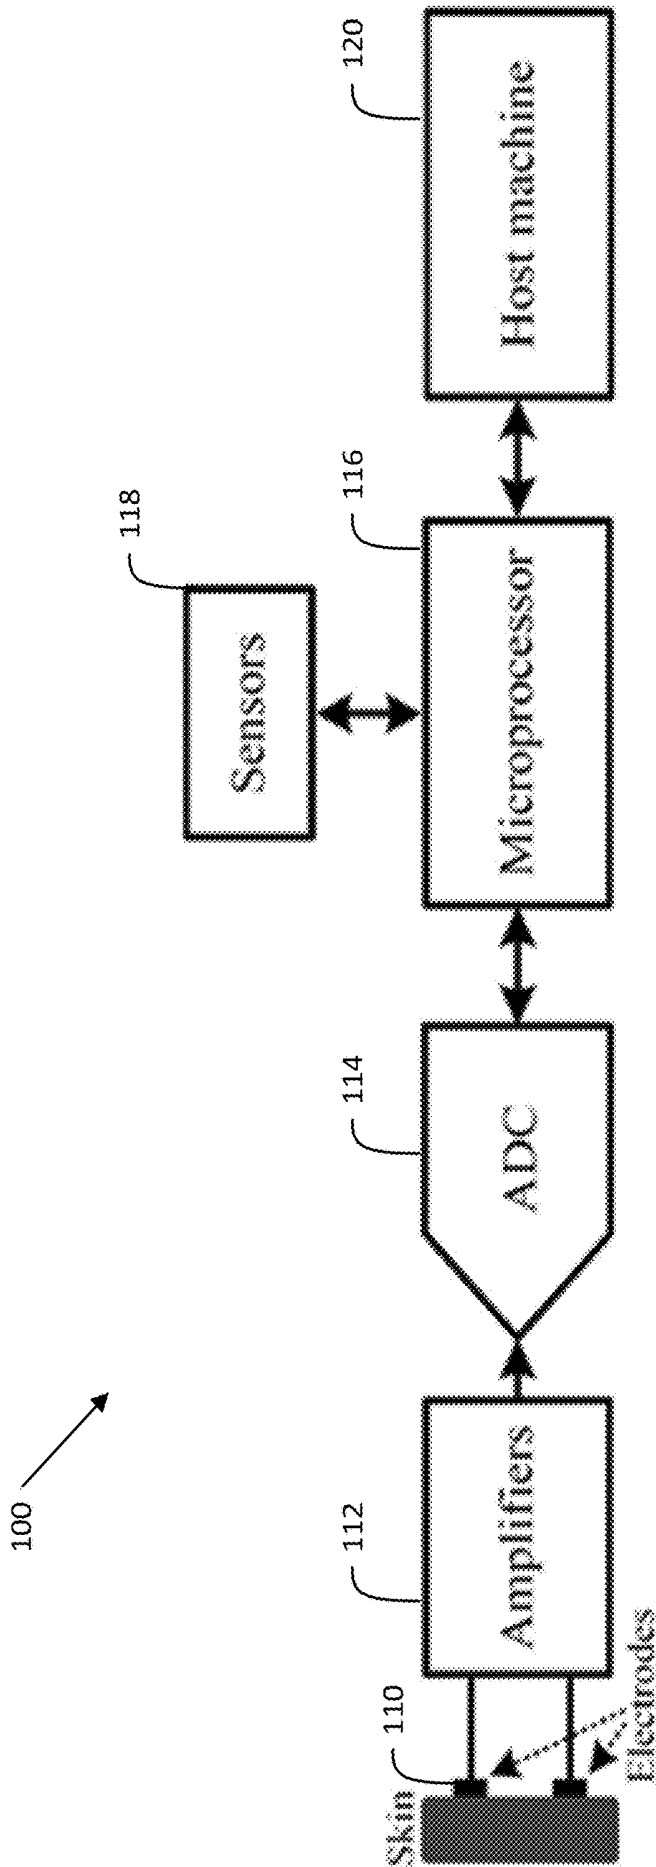


FIG. 1

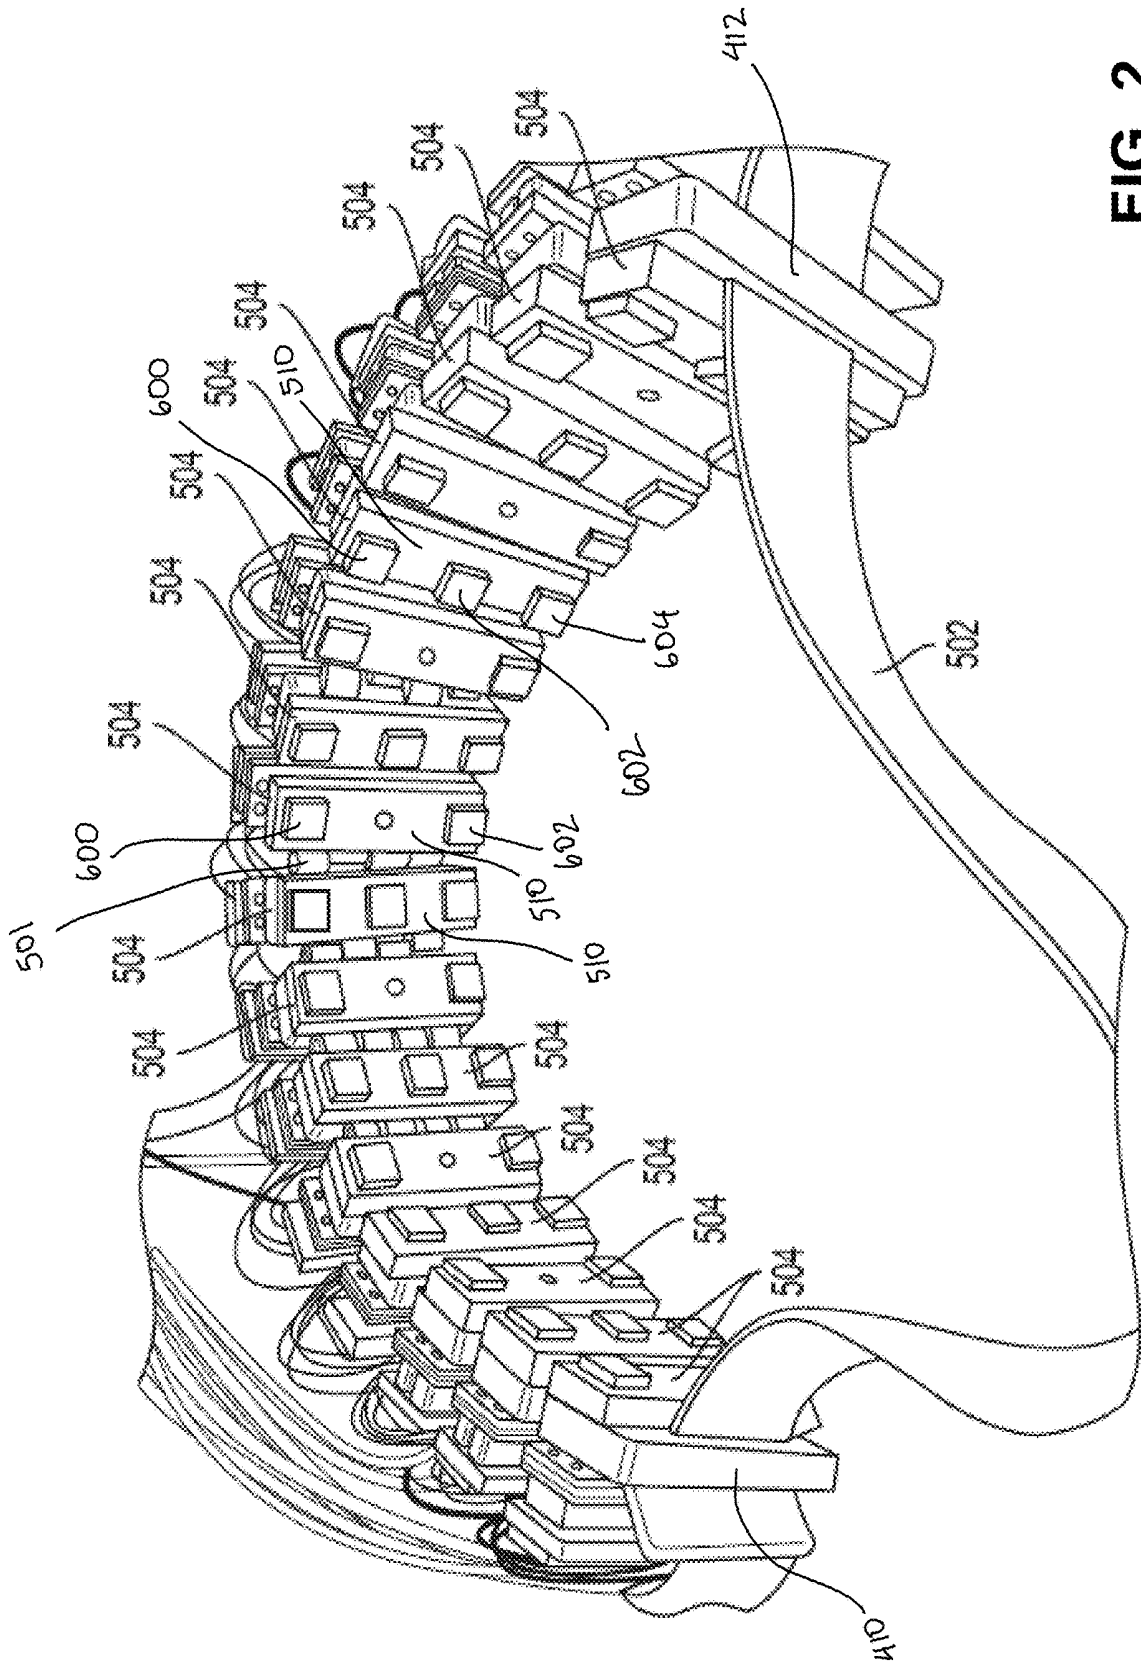


FIG. 2

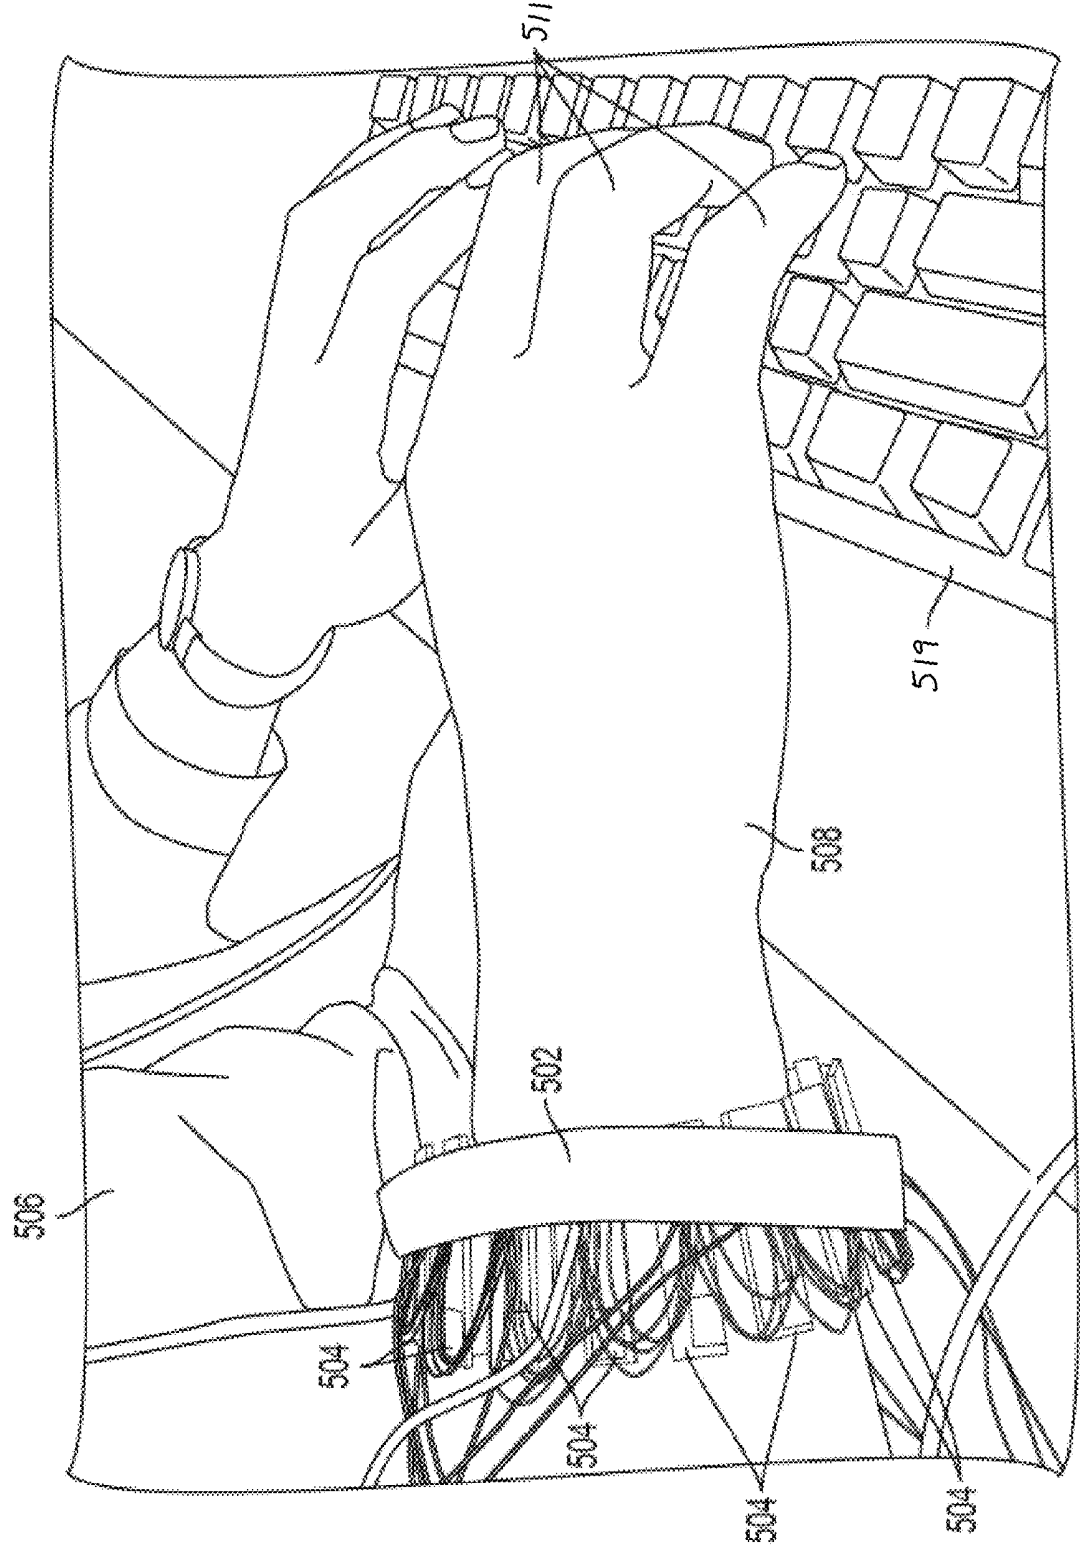


FIG. 3

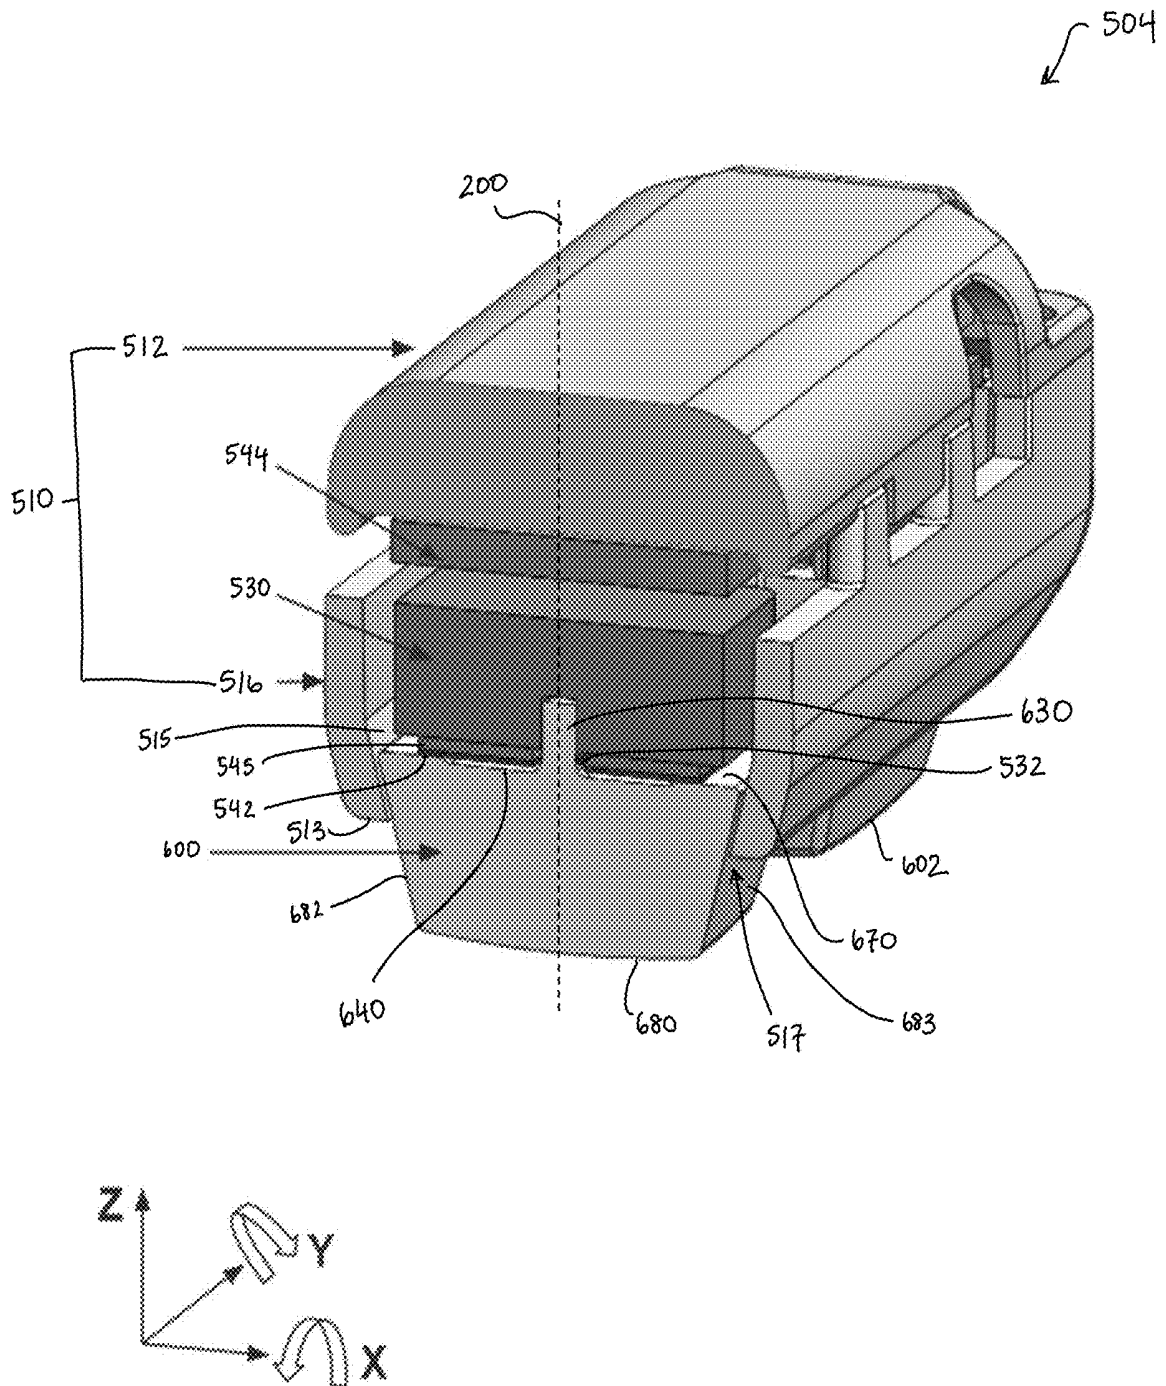


FIG. 4

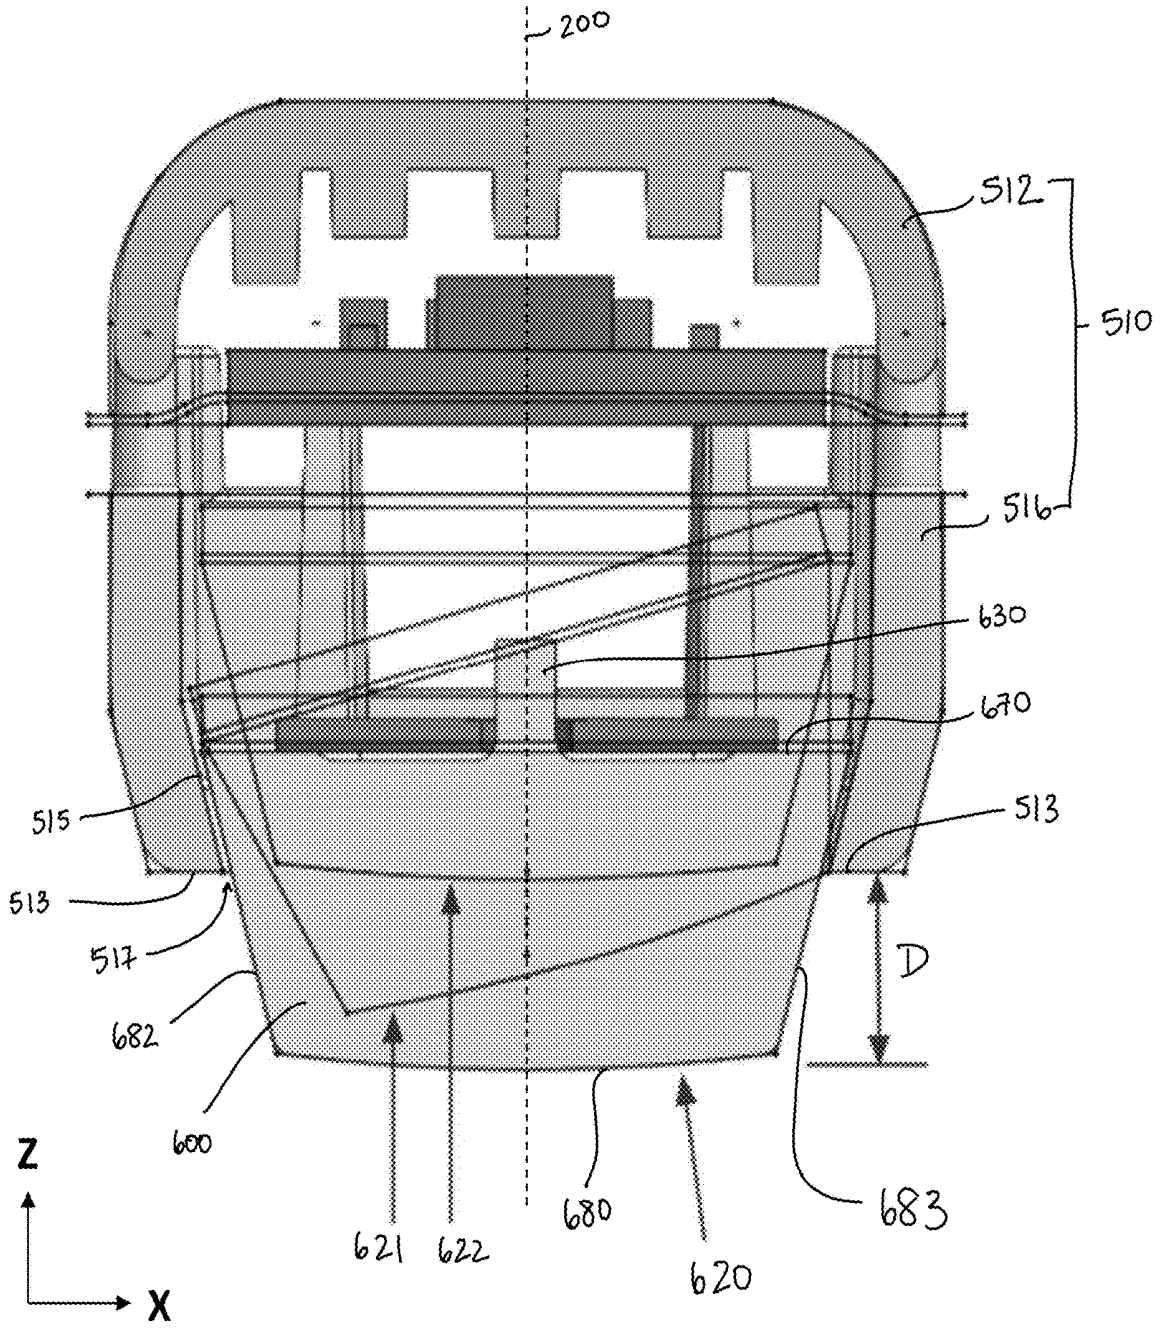


FIG. 5

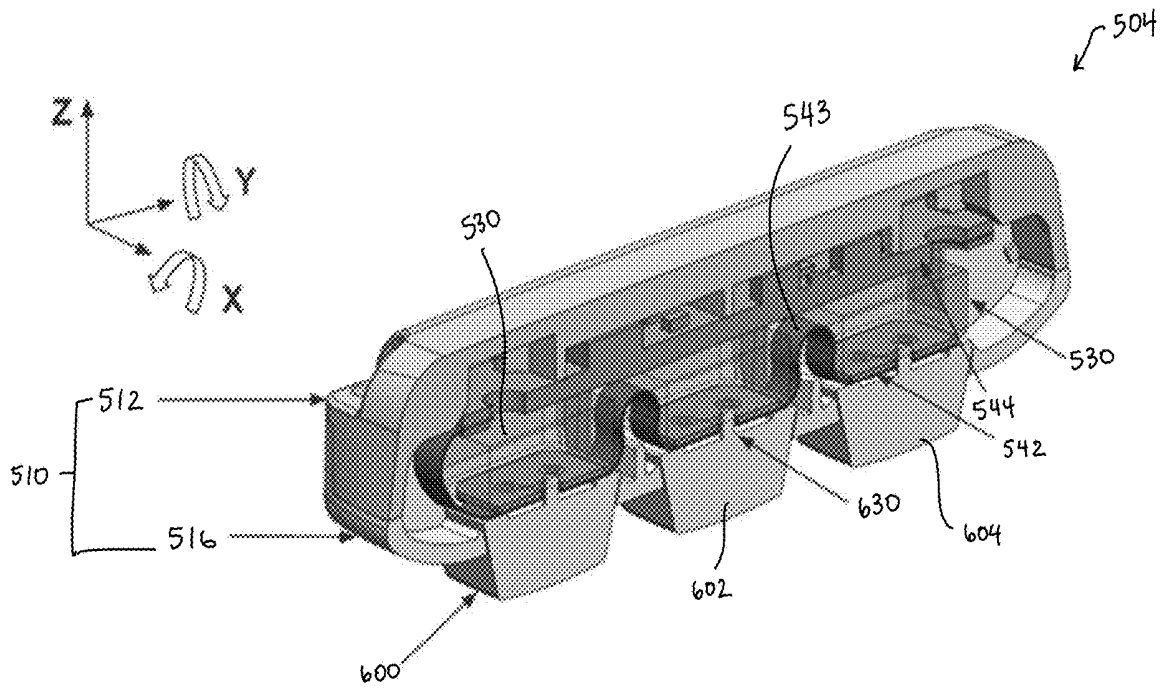


FIG. 6A

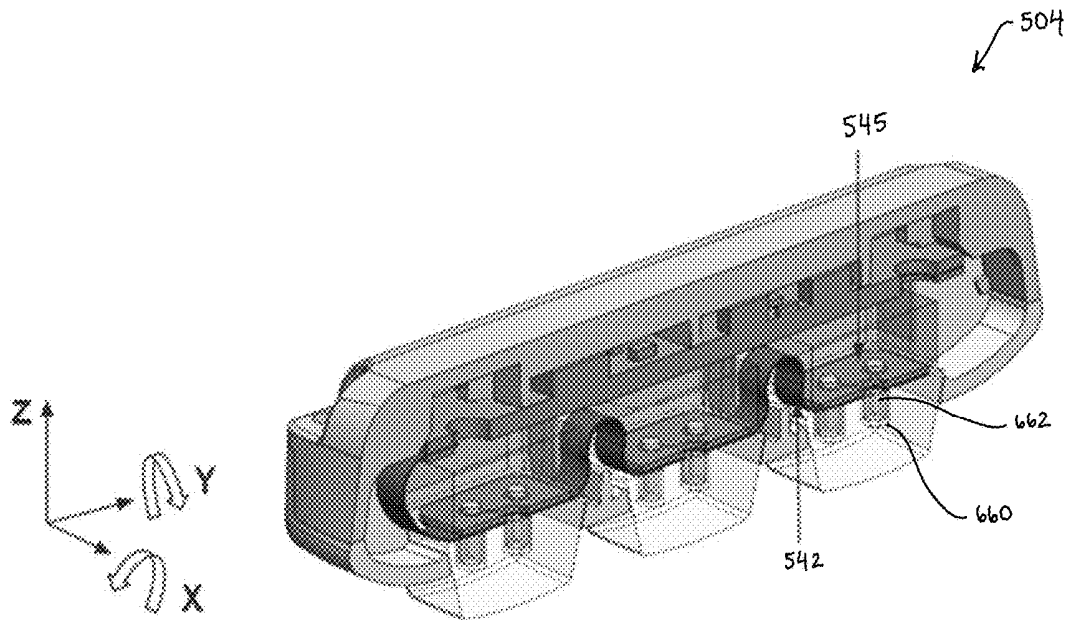
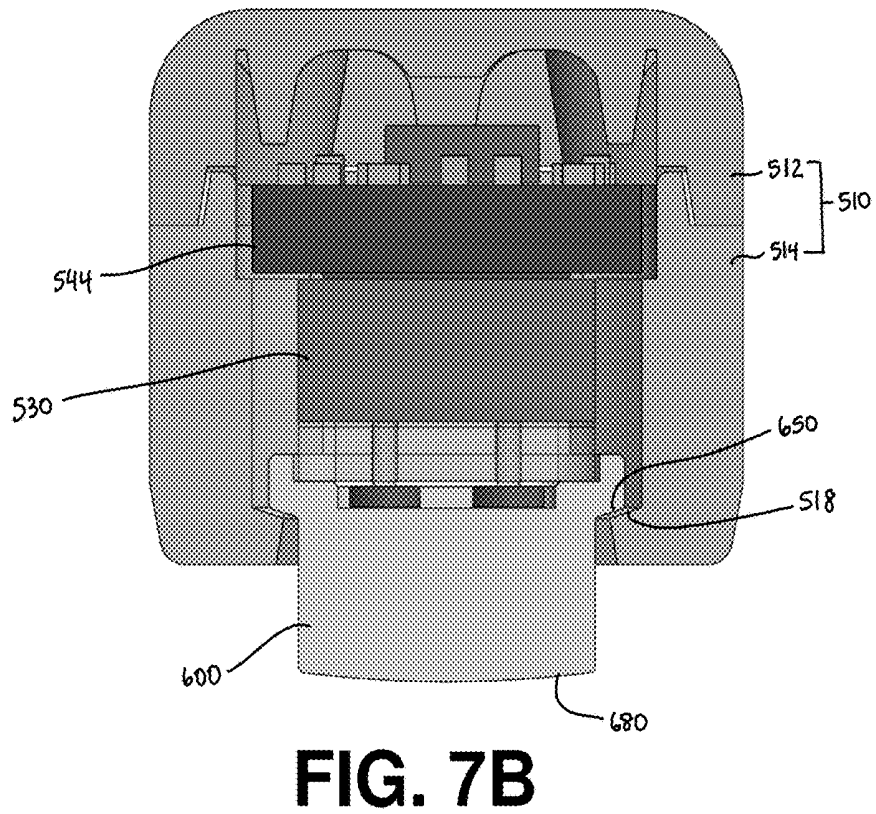
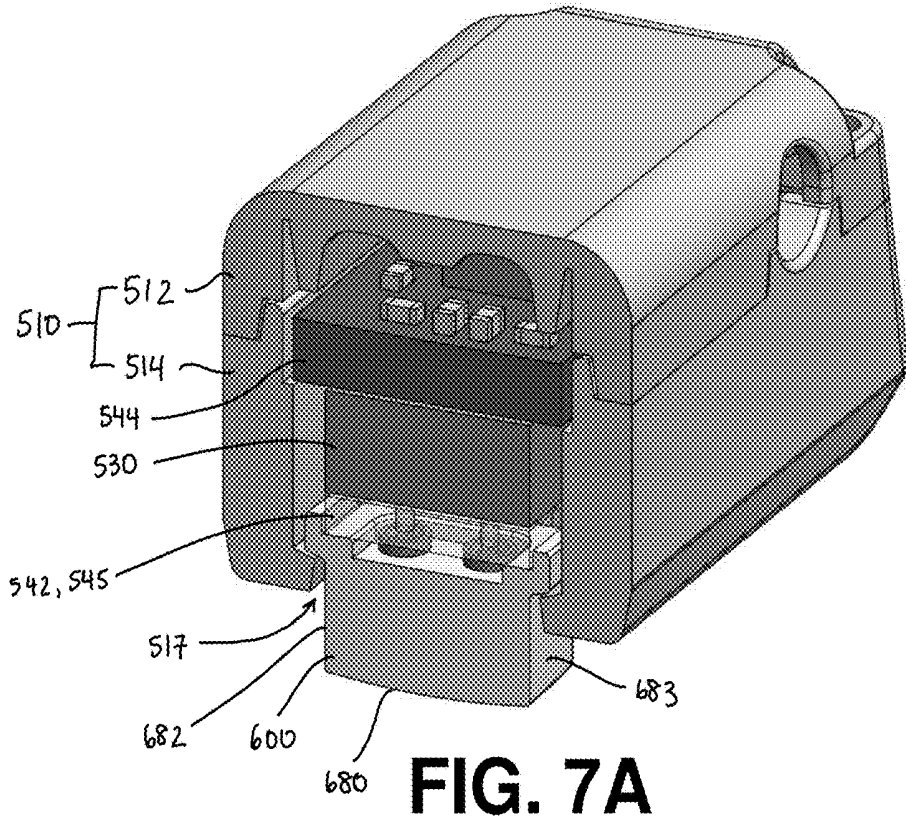


FIG. 6B



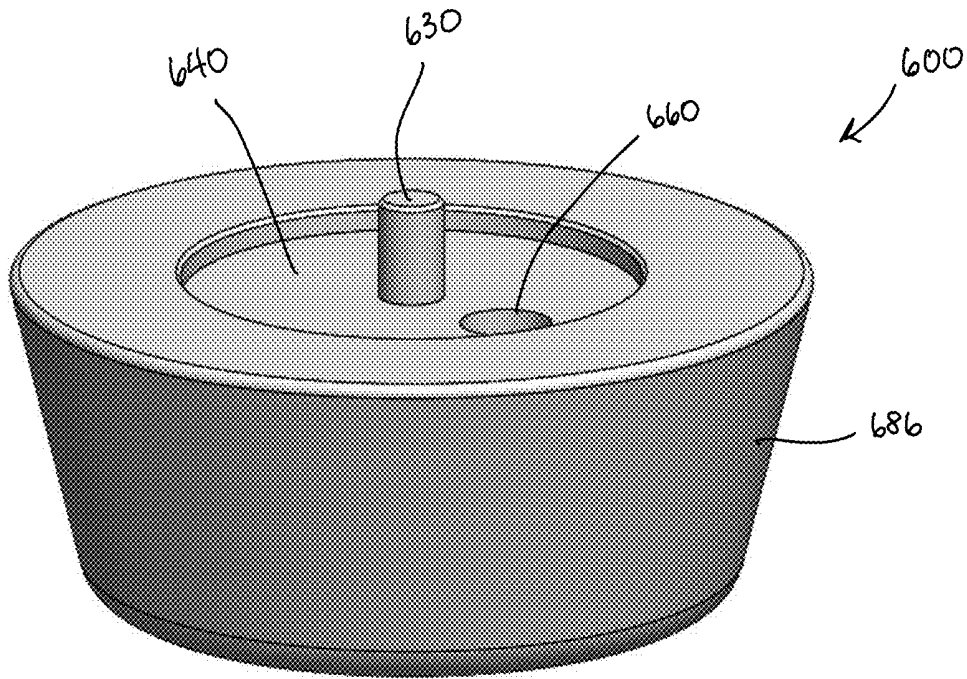


FIG. 8A

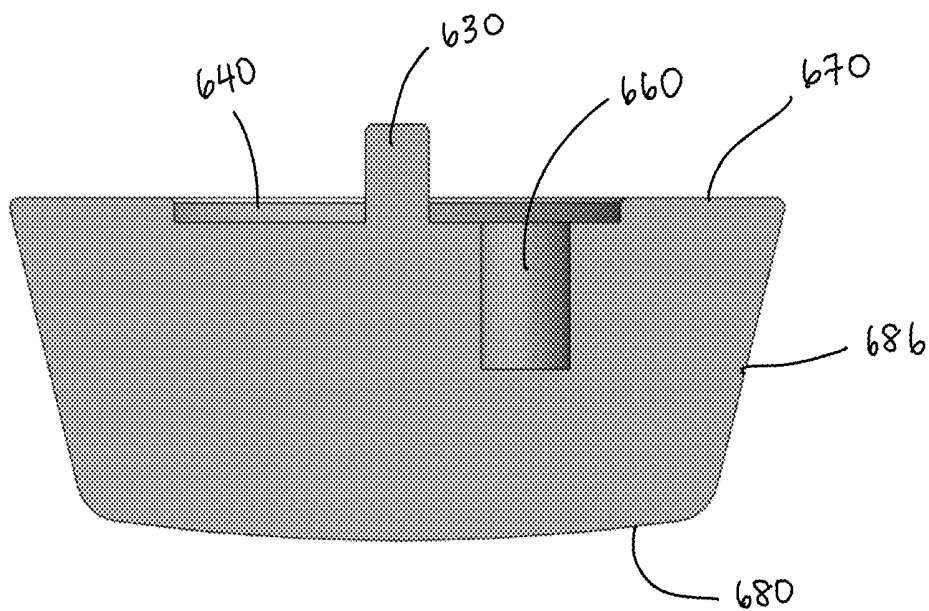


FIG. 8B

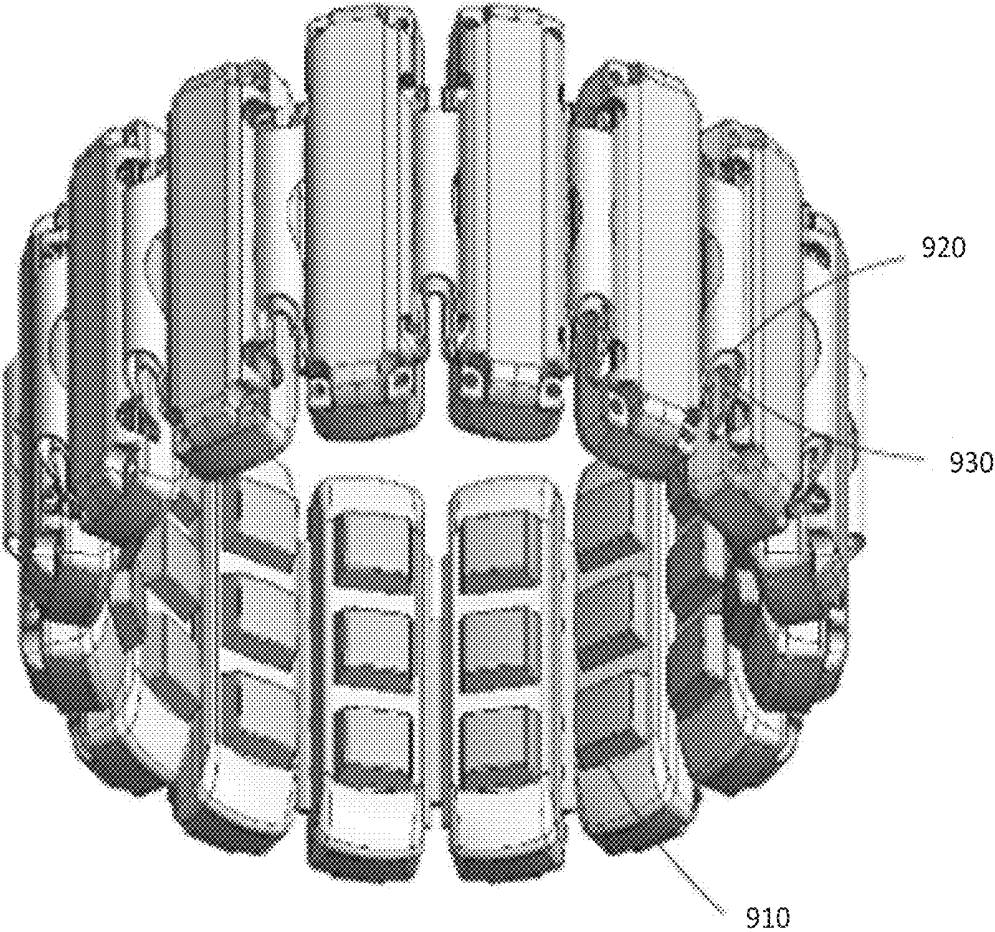


FIG. 9A

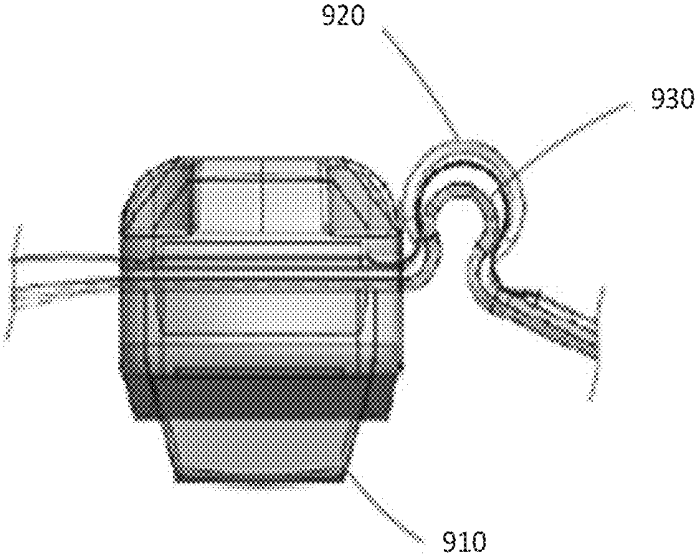


FIG. 9B

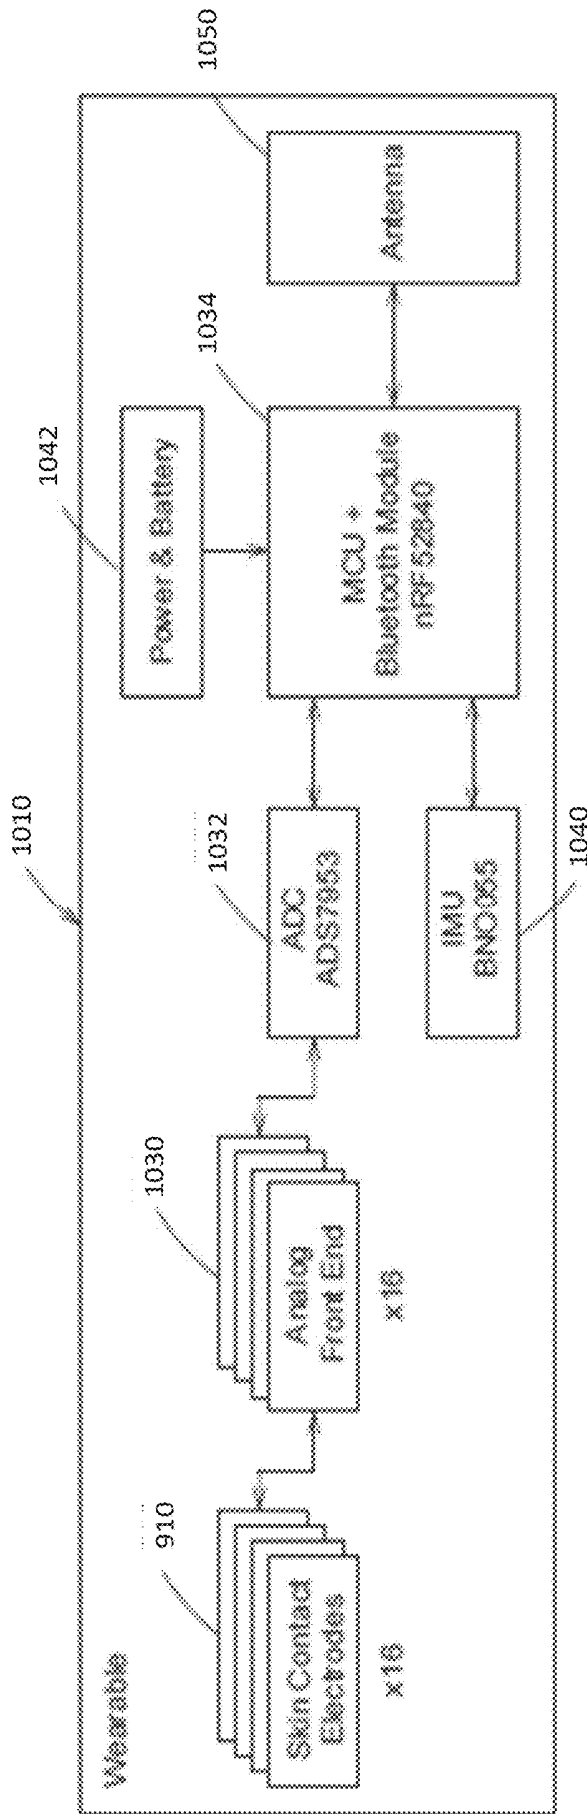


FIG. 10A

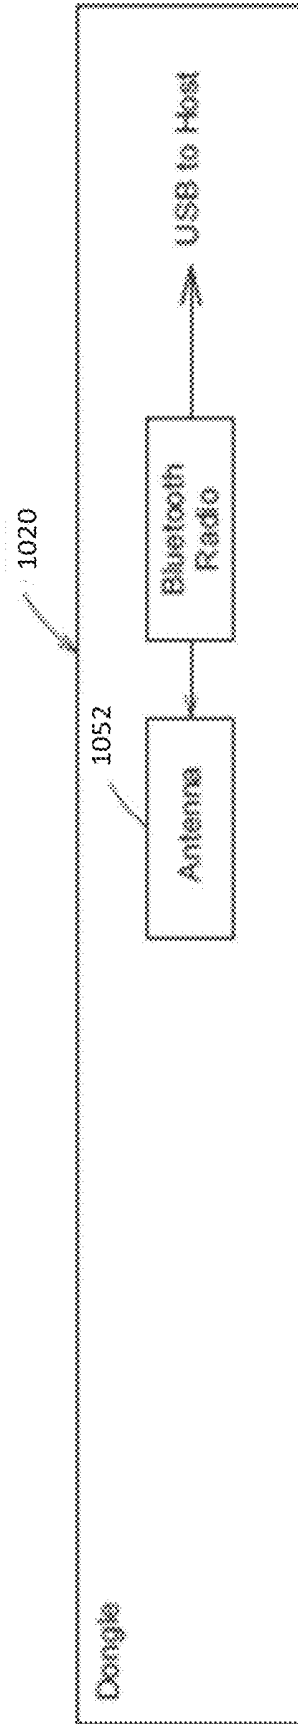


FIG. 10B

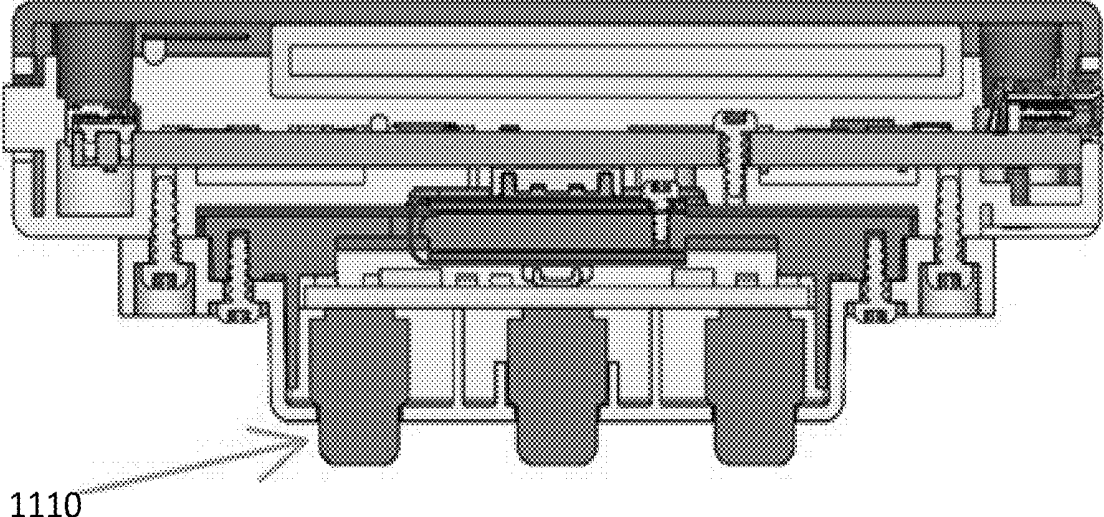


FIG. 11A

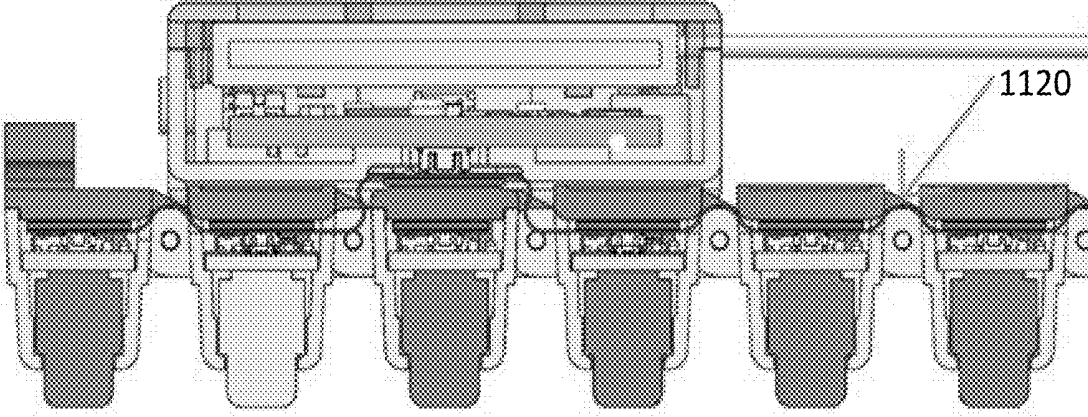


FIG. 11B

**METHODS AND APPARATUS FOR
IMPROVED SIGNAL ROBUSTNESS FOR A
WEARABLE NEUROMUSCULAR
RECORDING DEVICE**

RELATED APPLICATIONS

[0001] This application claims priority under 35 U.S.C. § 119(e) to U.S. Provisional Application No. 62/700,434 filed Jul. 19, 2018 and titled, “METHODS AND APPARATUS FOR IMPROVED SIGNAL ROBUSTNESS FOR A WEARABLE NEUROMUSCULAR DEVICE,” the entire contents of which is incorporated by reference herein.

BACKGROUND

[0002] Neuromuscular signals arising from the human central nervous system may reflect neural activation that results in the contraction of one or more muscles in the human body. Neuromuscular recording sensors, an example of which includes surface electromyography (sEMG) sensors, placed on the surface of the human body record neuromuscular activity produced when skeletal muscle cells are activated. The neuromuscular activity measured by neuromuscular recording sensors may result from neural activation, muscle excitation, muscle contraction, or a combination of the neural activation and muscle excitation and contraction. Signals recorded by neuromuscular recording sensors are routinely used to assess neuromuscular dysfunction in patients with motor control disorders and have been used in some applications as control signals for devices such as prosthetic limbs. High quality surface electromyography (sEMG) signals are typically acquired from wet electrodes in a laboratory setting using skin preparations that require application of a gel or paste at the electrode-skin interface to improve the conductivity between the skin and the electrodes.

SUMMARY

[0003] Coordinated movements of skeletal muscles in the human body that collectively result in the performance of a motor task originate with neural signals arising in the central nervous system. The neural signals travel from the central nervous system to muscles via spinal motor neurons, each of which has a cell body in the spinal cord and axon terminals on one or more muscle fibers. In response to receiving the neural signals, the muscle fibers contract resulting in muscle movement. A spinal motor neuron and the muscle fiber(s) it innervates are collectively referred to as a “motor unit.” Muscles typically include muscle fibers from hundreds of motor units and simultaneous contraction of muscle fibers in multiple motor units is usually required for muscle contraction that results in movement and forces in the musculo-skeletal system.

[0004] Neuromuscular recording sensors such as EMG sensors record biological signals that result in motor activity, such as contraction of a muscle. In the case of EMG sensors arranged on the surface of the human body, the biological signals recorded relate to the generation of action potentials in motor units, though the signals are dominated by signals originating from muscle fibers. Some embodiments are directed to analyzing neuromuscular signals to identify patterns of activation associated with sub-muscular biological structures (e.g., individual motor units or groups of motor units). Control signals determined based on activation

of muscle groups or sub-muscular structures may be used to control the operation of devices.

[0005] According to some aspects, a wearable bioelectrical sensing device is provided. The wearable bioelectrical sensing device comprises a plurality of electrodes including a first electrode, a second electrode, a third electrode, and a fourth electrode. The wearable bioelectrical sensing device further comprises a first housing containing at least a portion of the first electrode and at least a portion of the second electrode, each of the first and second electrode being configured to rotate relative to the first housing from a starting position to a rotated position, and a second housing containing at least a portion of the third electrode and at least a portion of the fourth electrode, each of the third and fourth electrodes being configured to rotate relative to the second housing, wherein the first housing and the second housing are coupled to each other in an arrangement that enables the first, second, third, and fourth electrode to contact a body part of a user when the wearable bioelectrical sensing device is worn around the body part of the user. The wearable bioelectrical sensing device further comprises a first flexible circuit electrically connecting the first electrode to the second electrode within the first housing, a second flexible circuit electrically connecting the third electrode to the fourth electrode within the second housing, and a spring element configured to bias the first electrode toward the starting position of the first electrode.

[0006] According to some aspects, a wearable bioelectrical sensing device is provided. The wearable bioelectrical sensing device comprises a plurality of electrodes including a first electrode, a second electrode, a third electrode, and a fourth electrode. The wearable bioelectrical sensing device further comprises a first housing containing at least a portion of the first electrode and at least a portion of the second electrode, each of the first and second electrodes being movable relative to the first housing with at least one degree of freedom such that each of the first electrode and second electrode is movable from a starting position to a different position relative to the first housing. The wearable bioelectrical sensing device further comprises a second housing containing at least a portion of the third electrode and at least a portion of the fourth electrode, each of the third and fourth electrodes being movable relative to the second housing with at least one degree of freedom such that each of the third electrode and the fourth electrode is movable from a starting position to a different position relative to the second housing, wherein the first housing and the second housing are coupled to each other in an arrangement that enables the first, second, third, and fourth electrode to contact a body part of a user when the wearable bioelectrical sensing device is worn around the body part of the user. The wearable bioelectrical sensing device further comprises, a first flexible circuit electrically connecting the first electrode to the second electrode within the first housing, a second flexible circuit electrically connecting the third electrode to the fourth electrode within the second housing, and a spring element configured to bias the first electrode toward the starting position of the first electrode.

[0007] According to some aspects, a method of using a wearable bioelectrical sensing device is provided. The method comprises wearing the wearable bioelectrical sensing device to contact a first electrode, a second electrode, a third electrode, and a fourth electrode of the device with skin, wherein the wearable bioelectrical sensing device

includes a first housing containing at least a portion of the first electrode and at least a portion of the second electrode, and a second housing containing at least a portion of the third electrode and at least a portion of the fourth electrode, and rotating the first electrode relative to the first housing from a starting position to a rotated position while keeping the first electrode in contact with the skin throughout the rotation.

[0008] According to some aspects, a method of using a wearable bioelectrical sensing device is provided. The method comprises wearing the wearable bioelectrical sensing device to contact a first electrode, a second electrode, a third electrode, and a fourth electrode of the device with skin, wherein the wearable bioelectrical sensing device includes a first housing containing at least a portion of the first electrode and at least a portion of the second electrode, and a second housing containing at least a portion of the third electrode and at least a portion of the fourth electrode, and moving the first electrode relative to the first housing with at least two degrees of freedom from a starting position to a different position.

[0009] According to some aspects, a wearable device is provided, including a first electrode and a first housing containing at least a portion of the first electrode. The first electrode is configured to rotate relative to the first housing from a starting position to a rotated position. The wearable device also includes a band that is coupled to the first housing and is configured to be worn by a user.

[0010] According to some aspects, a wearable device is provided, including a first electrode and a first housing containing at least a portion of the first electrode. The first electrode is movable relative to the first housing with at least two degrees of freedom such that the first electrode is movable from a starting position to a different position relative to the first housing. The wearable device also includes a band that is coupled to the first housing and is configured to be worn by a user.

[0011] According to some aspects, a method of using a wearable device is provided, including: wearing a band to contact a first electrode with skin, where a first housing is coupled to the band and the first housing contains at least a portion of the first electrode, and rotating the first electrode relative to the first housing from a starting position to a rotated position.

[0012] According to some aspects, a method of using a wearable device is provided, including: wearing a band to contact a first electrode with skin, where a first housing is coupled to the band and the first housing contains at least a portion of the first electrode, and moving the first electrode relative to the first housing with at least two degrees of freedom from a starting position to a different position.

[0013] It should be appreciated that all combinations of the foregoing concepts and additional concepts discussed in greater detail below (provided such concepts are not mutually inconsistent) are contemplated as being part of the inventive subject matter disclosed herein. In particular, all combinations of claimed subject matter appearing at the end of this disclosure are contemplated as being part of the inventive subject matter disclosed herein.

BRIEF DESCRIPTION OF DRAWINGS

[0014] Various non-limiting embodiments of the technology will be described with reference to the following figures. It should be appreciated that the figures are not necessarily drawn to scale.

[0015] FIG. 1 is a schematic diagram of components of a neuromuscular recording system in accordance with some embodiments of the technology described herein;

[0016] FIG. 2 illustrates a wristband having neuromuscular recording sensors arranged circumferentially thereon, in accordance with some embodiments of the technology described herein;

[0017] FIG. 3 illustrates a user wearing the wristband of FIG. 2 while typing on a keyboard, in accordance with some embodiments of the technology described herein;

[0018] FIG. 4 depicts an illustrative embodiment of a neuromuscular recording sensor having moveable electrodes, according to some embodiments;

[0019] FIG. 5 depicts a cross-sectional view of the sensor shown in FIG. 4 along the X-Z plane, with the moveable electrode shown in three different positions;

[0020] FIG. 6A depicts a perspective section view of the sensor shown in FIG. 4;

[0021] FIG. 6B depicts the neuromuscular recording sensor of FIG. 6A with the electrodes shown in phantom;

[0022] FIG. 7A depicts an illustrative embodiment of a neuromuscular recording sensor according to an alternative embodiment;

[0023] FIG. 7B depicts a cross-sectional view of the neuromuscular recording sensor shown in FIG. 7A;

[0024] FIG. 8A depicts an illustrative embodiment of an electrode for neuromuscular recording sensor according to an alternative embodiment;

[0025] FIG. 8B depicts a cross-sectional view of the neuromuscular recording sensor shown in FIG. 8A;

[0026] FIG. 9A illustrates a wearable system with sixteen neuromuscular recording sensors arranged circumferentially around an elastic band configured to be worn around a user's lower arm or wrist, in accordance with some embodiments of the technology described herein;

[0027] FIG. 9B is a cross-sectional view through one of the sixteen neuromuscular recording sensors illustrated in FIG. 9A;

[0028] FIGS. 10A and 10B schematically illustrate components of a computer-based system on which some embodiments are implemented. FIG. 10A illustrates a wearable portion of the computer-based system and FIG. 10B illustrates a dongle portion connected to a computer, wherein the dongle portion is configured to communicate with the wearable portion;

[0029] FIG. 11A shows a cross-sectional view through a neuromuscular recording sensor and its associated sensor housing, in accordance with some embodiments of the technology described herein; and

[0030] FIG. 11B shows a cross-sectional view through a plurality of neuromuscular recording sensors coupled via hinge structures, in accordance with some embodiments of the technology described herein.

DETAILED DESCRIPTION

[0031] Obtaining consistent high-quality neuromuscular (e.g., sEMG) signals using neuromuscular recording (e.g., sEMG) electrodes and conventional signal processing tech-

niques is challenging, in part due to the difficulty of maintaining sufficient contact between a neuromuscular recording electrode and a moving body surface, e.g., skin.

[0032] Aspects herein relate to the use of sensors to detect biological signals resulting from the activation of motor unit. The sensors may include a plurality of neuromuscular recording sensors configured to detect signals arising from neuromuscular activity in skeletal muscle of a human body. The term “neuromuscular activity” as used herein refers to neural activation of spinal motor neurons that innervate a muscle, muscle activation, muscle contraction, or any combination of neural activation, muscle activation, and muscle contraction. In some embodiments, the plurality of neuromuscular recording sensors may be used to sense sub-muscular activity associated with a sub-muscular structure (e.g., a motor unit or set of motor units). In various embodiments of the systems, apparatuses, and methods described herein, neuromuscular signals may be used to derive control signals for machine control, to create an immersive rendering of a virtual hand (e.g., a rendering of the user’s ‘hand-state’), or other applications. In general, consistent and high-quality neuromuscular signals (e.g., high signal-to-noise ratio (SNR), consistent noise characteristics in the frequency-domain, etc.) enable the neuromuscular signals to be more effectively used for immersive, control, and other applications. The inventors have recognized that in at least some instances, motion artifacts may cause an epoch of recorded data to be unsatisfactory or unusable (e.g., on one or more channels of a neuromuscular recording sensor array) due to the magnitude of the artifact being larger than the biological signals of interest. Motion artifacts may change the baseline (e.g., direct current level) of a recording. In some instances, motion artifacts may cause an amplifier in a neuromuscular recording system to saturate, rendering the underlying biological signal completely unresolvable.

[0033] To detect signals arising from neuromuscular activity, neuromuscular recording electrodes are held in contact against a body surface (e.g., skin). When the contact between skin and an electrode changes, motion artifacts may be generated. For example, an electrode may partially or fully lift off of the skin due to movement of a wearable neuromuscular recording device and/or conformational changes in a user’s body due to movement, muscle contraction, or other reason. Motion artifacts may also be generated from a change in the pressure between electrode and skin, a change of the orientation (e.g., an angle as parametrized by pitch, yaw, and roll) of an electrode relative to the skin, a translation of the electrode (e.g., a change in the position of the electrode on the skin), or a conformational change in the tissue underlying the electrode due to a muscle contraction, movement, or other reason.

[0034] Dry biosensor electrodes that interface mechanically with skin for recording neuromuscular activity are preferred relative to electrodes that require the use of adhesive and/or conductive gels (i.e., ‘wet electrodes’). Compared to wet electrodes, dry electrodes require less set up time, can be re-used numerous times without degrading signal quality, and provide a more pleasant user experience due to the absence of residue on the skin after an electrode has been removed. The inventors have appreciated that dry electrodes or those that interface with a body surface without the use of adhesive and/or conductive gels are susceptible to signal variations—in part due to several kinds of motion artifacts—that make downstream processing of biological

signals challenging. For example, the neuromuscular recording sensors (i.e., electrodes) may interface with a part of the body that changes in size and cross-section during muscle contractions, or the electrodes may be integrated in a wearable form factor that shifts relative to the skin due to movements and forces of a user’s musculoskeletal system. For example, as the body part changes conformation, the electrodes may lift off of the body part surface (fully or partially), become further pressed into the surface (possibly changing the impedance of the skin-electrode contact), shift laterally across the skin, or otherwise experience a change in the recording contact with the skin.

[0035] The inventors have recognized that variable pressure across electrodes can cause inaccuracies and motion artifacts. The inventors have also appreciated that an electrode lifting off the body surface may permit electrical line noise (e.g., 50 Hz or 60 Hz noise) to completely infiltrate the signal, reducing the fidelity of the neuromuscular recordings.

[0036] The inventors have also recognized that body hair can contribute to reduced quality of neuromuscular recordings because hair between the electrode surface and the skin is not conductive, which may have one or more deleterious effects on the quality of neuromuscular signals, including: increased noise (e.g., electrical line noise) and a propensity for exacerbated motion artifacts when the hairs between an electrode and the skin shift or otherwise change in position and/or composition.

[0037] The inventors have observed that epochs of poor signal quality in neuromuscular recordings often coincide with muscle contractions that cause the body surface to pull away from the electrode surface. Mechanical or other strategies to maintain a consistent electrode-skin interface for neuromuscular recording despite conformational changes or movement of a user’s body would improve the quality and consistency of neuromuscular recordings.

[0038] In addition to signal variations due to hair or movement of the subject’s skin and muscle, the inventors have also recognized that movement of the housing or other component of a wearable neuromuscular recording apparatus mechanically coupled to a neuromuscular recording sensor (e.g., an sEMG electrode) may impart an inertial moment at the electrode-skin interface and can likewise cause motion artifacts in the recorded neuromuscular signals.

[0039] In addition to being undesirable in the resulting signal, the inventors have also recognized that large artifacts and shifts in the baseline of a signal often dictate choice of an amplifier gain and filter components such that the amplifier will not saturate and/or will recover quickly. Reducing motion artifacts, electrode contact issues, 50 or 60 Hz noise, and amplifier saturation allows for more flexibility in the choice of circuit components and allows for use of a larger portion of the ADC (analog digital converter) dynamic range for biosignal recording, resulting in finer resolution/precision in the neuromuscular (e.g., sEMG) signal output from a recording system such as that shown in FIG. 1 and FIGS. 10A-B.

[0040] In some clinical applications, wet contact electrodes containing a hydrogel or other conductive material at the dermal surface are often used in combination with adhesive pads for signal stability. The inventors have appreciated that these electrodes can be time consuming to apply and are usually single use due to the degradation of the

hydrogel (or other 'wet') interface and adhesive due to dirt and oils on the skin. The inventors have also recognized that, in some clinical applications, semi-dry electrodes are used instead of wet contact electrodes. The inventors have appreciated that, while semi-dry electrodes are not typically applied with adhesive and may be multi-use, they may require maintenance, proper storage, and can be less durable than a dry electrode.

[0041] The inventors have thus recognized the need for an arrangement that provides improved contact between electrodes for neuromuscular and other biosignal recording and a user's body surface. The systems and methods described herein may be used for any bioelectrical surface recording, including neuromuscular recordings (e.g., electromyography, electrical impedance tomography) and other biosignal recordings.

[0042] FIG. 1 schematically depicts components of an illustrative neuromuscular recording system 100, in accordance with some embodiments. System 100 includes a pair of neuromuscular recording (e.g., dry sEMG) electrodes 110. In some embodiments, electrodes 110 may be arranged as a portion of a wearable device configured to be worn on or around a part of a user's body. For example, in one non-limiting example, a plurality of neuromuscular recording sensors including neuromuscular recording electrodes (e.g., electrodes 110) are arranged circumferentially around an adjustable and/or elastic band such as a wristband or armband configured to be worn around a user's wrist or arm. Alternatively, at least some of the neuromuscular recording sensors may be arranged on a wearable patch configured to be affixed to a portion of the user's body.

[0043] Surface potentials recorded by neuromuscular recording electrodes are typically small (μV to mV) and amplification of the signals recorded by the neuromuscular recording electrodes is typically desired. As shown in FIG. 1, neuromuscular recording (e.g., dry sEMG) electrodes 110 are coupled to amplification circuitry 112, configured to amplify the neuromuscular signals recorded by the electrodes. The output of the amplification circuitry 112 is provided to analog-to-digital converter (ADC) circuitry 114, which converts the amplified neuromuscular signals to digital signals for further processing by microprocessor 116. Microprocessor 116 may be implemented by one or more hardware processors. The processed signals output from microprocessor 116 may be interpreted by host machine 120, examples of which include, but are not limited to, a desktop computer, a laptop computer, a smartwatch, a smartphone, or any other computing device. In some implementations, host machine 120 may be configured to output one or more control signals for controlling a physical or virtual device based, at least in part, on an analysis of the signals output from microprocessor 116.

[0044] As shown, neuromuscular recording system 100 also includes sensors 118, which may be configured to record types of information about a state of a user other than neuromuscular information. For example, sensors 118 may include, but are not limited to, temperature sensors configured to measure skin/electrode temperature, inertial measurement unit (IMU) sensors configured to measure movement information such as rotation and acceleration, humidity sensors, heart-rate monitor sensors, camera and video input, and other bio-chemical sensors configured to provide information about the user and/or the user's environment.

[0045] In one implementation, sixteen neuromuscular recording sensors including neuromuscular recording (e.g., dry sEMG) electrodes are arranged circumferentially around an elastic band configured to be worn around a body part, such as a user's lower arm. For example, FIG. 2 shows neuromuscular recording sensors 504 coupled to a band 502, which may be an elastic band. The sensors may be arranged circumferentially around the band. It should be appreciated that any suitable number of neuromuscular recording sensors having any suitable number of neuromuscular recording (e.g., dry sEMG) electrodes may be used and the number and arrangement of sensors/electrodes may depend on the particular application for which the wearable device is used. For example, as shown in FIG. 2, some of the neuromuscular recording sensors 504 include two neuromuscular recording electrodes 600 and 602, whereas others of the neuromuscular recording sensors 504 include three neuromuscular recording electrodes 600, 602, and 604, with the middle of the three electrodes being a ground or reference electrode. The ground electrode may be included on one or more of the neuromuscular recording sensors 504 to, for example, further bias the skin potential and/or to filter out noise. Each of the sensors 504 may include a sensor housing 510. Although the schematic diagram in FIG. 1 illustrates only two or three electrodes being connected to an amplifier, it should be appreciated that for sEMG sensors 504 in which one, two, three, or more than three electrodes are used, a corresponding number of connections between the electrodes and the amplification circuitry would be included.

[0046] In one example application of the technology described herein, FIG. 3 shows a user 506 wearing elastic band 502 on hand 508. In this way, neuromuscular recording sensors 504 may be configured to record neuromuscular signals as a user controls keyboard 519 using fingers 511.

[0047] FIG. 9A shows an alternate configuration of a wearable bioelectrical recording system with sixteen neuromuscular recording sensors 910 (e.g., sEMG sensors) arranged circumferentially around an elastic band 920 configured to be worn around a user's lower arm or wrist in accordance with some embodiments. As shown, neuromuscular recording sensors 910 are arranged circumferentially around elastic band 920. It should be appreciated that any suitable number of neuromuscular recording sensors may be used. The number and arrangement of neuromuscular recording sensors may depend on the particular application for which the wearable system is used. For example, a wearable armband or wristband can be used to generate control information for controlling an augmented reality system, a robot, controlling a vehicle, scrolling through text, controlling a virtual avatar, or any other suitable control task. As shown, the sensors may be coupled together using flexible electronics incorporated into the wireless device, FIG. 9B illustrates a cross-sectional view through one of the sensors of the wearable system shown in FIG. 9A.

[0048] In some embodiments, the output of one or more of the sensing components can be optionally processed using hardware signal processing circuitry (e.g., to perform amplification, filtering, and/or rectification). In other embodiments, at least some signal processing of the output of the sensing components can be performed in software. Thus, signal processing of signals sampled by the sensors can be performed in hardware, software, or by any suitable combination of hardware and software, as aspects of the technology described herein are not limited in this respect. A

non-limiting example of a signal processing chain used to process recorded data from sensors 910 are discussed in more detail below with reference to FIGS. 10A and 10B.

[0049] FIGS. 10A and 10B illustrate a schematic diagram with internal components of a wearable system with sixteen sEMG sensors. As shown, the wearable system includes a wearable portion 1010 (FIG. 10A) and a dongle portion 1020 (FIG. 10B) in communication with the wearable portion 1010 (e.g., via Bluetooth or another suitable short range wireless communication technology). As shown in FIG. 10A, the wearable portion 1010 includes sensors 910, examples of which are described in connection with FIGS. 9A and 9B. The output of the sensors 910 is provided to analog front end 1030 configured to perform analog processing (e.g., noise reduction, filtering, etc.) on the recorded signals. The processed analog signals are then provided to analog-to-digital converter 1032, which converts the analog signals to digital signals that can be processed by one or more computer processors. An example of a computer processor that may be used in accordance with some embodiments is microcontroller (MCU) 1034 illustrated in FIG. 10A. As shown, MCU 1034 may also include inputs from other sensors (e.g., IMU sensor 1040), and power and battery module 1042. The output of the processing performed by MCU may be provided to antenna 1050 for transmission to dongle portion 1020 shown in FIG. 10B.

[0050] Dongle portion 1020 includes antenna 1052 configured to communicate with antenna 1050 included as part of wearable portion 1010. Communication between antenna 1050 and 1052 may occur using any suitable wireless technology and protocol, non-limiting examples of which include radiofrequency signaling and Bluetooth. As shown, the signals received by antenna 1052 of dongle portion 1020 may be provided to a host computer for further processing, display, and/or for effecting control of a particular physical or virtual object or objects.

[0051] Although the examples provided with reference to FIGS. 9A, 9B and FIGS. 10A, 10B are discussed in the context of interfaces with EMG sensors, it is understood that the techniques described herein for reducing electromagnetic interference can also be implemented in wearable interfaces with other types of sensors including, but not limited to, mechanomyography (MMG) sensors, sonomyography (SMG) sensors, and electrical impedance tomography (EIT) sensors.

[0052] When a user performs a motor task, such as moving their arm, a group of muscles necessary to perform the motor task is activated. When the motor task is performed while the user is wearing a wearable device that includes neuromuscular recording sensors, the neuromuscular signals recorded by the sensors on the surface of the body correspond to superimposed and spatiotemporally filtered activity of all motor units in the muscles in the group activated during performance of the motor task. The neuromuscular signals may be analyzed and mapped to control signals to control a device based on the type of movement, pose, force, or gesture that the user performs. For example, if the user performs a thumbs-up gesture with their hand, a corresponding control signal to select an object in a user interface may be generated. The mapping between sensor signals and control signals may be implemented, for example, using an inferential model trained to associate particular sensor signal inputs with control signal outputs. In some embodiments, the output of the trained inferential model may be muscu-

loskeletal position information that describes, for example, the positions and/or forces of elements in a computer-implemented musculoskeletal model. As neuromuscular signals are continuously recorded, the musculoskeletal model may be updated with predictions of the musculoskeletal position information (e.g., joint angles and/or forces) output from the inferential model. Control signals may then be generated based on the updated musculoskeletal position information. In other embodiments, the output of the trained inferential model may be the control information itself, such that a separate musculoskeletal model is not used.

[0053] Described herein are neuromuscular (e.g., sEMG) sensor arrangements that provide improved contact between sensor electrodes and a user's body surface (e.g., skin) for improved signal detection.

[0054] According to one aspect, some embodiments described herein are directed to a neuromuscular recording sensor having electrodes that are moveable relative to the sensor housing to permit the electrodes to remain in contact with the body surface as the body portion changes conformation and/or the sensor housing moves relative to the body surface (e.g., due to a user moving their arm about their shoulder joint to wave and causing inertial forces on the housing of the neuromuscular recording sensor(s) to translate the position of an electrode relative to a portion of the surface of the user's body (e.g., skin)). In some embodiments, the electrodes may be configured in an assembly that permits them to rotate relative to the sensor housing. In some embodiments, the electrodes may be configured in an assembly that permits them to rotate and translate relative to the sensor housing. The electrodes may have at least two, at least three, at least four, at least five, or six degrees of freedom relative to the sensor housing. In some embodiments, where an electrode has five degrees of freedom relative to the sensor housing, the electrode may translate along three perpendicular axes (i.e., in three dimensions) and rotate about two of these axes relative to the sensor housing. In some embodiments, an electrode may have three degrees of freedom comprising rotation about three axes (i.e. pitch, yaw, and roll). In general, an electrode for neuromuscular recording configured in a wearable assembly or housing may rotate in any or all of the three translational axes (i.e. translating laterally along the skin in two dimensions or vertically as the skin position moves in the vertical plane relative to the housing of the neuromuscular recording system) and/or in any or all of the rotational axes (pitch, yaw, and roll).

[0055] In some embodiments, the electrodes may have a starting position in which at least a portion of the electrodes extend out of an opening of the housing, and the electrodes may be configured to move inwardly into the housing through the opening during application of force upon the electrodes. The electrodes and the housing may each be shaped to cooperate with one another to permit movement of the electrodes and to guide the electrode toward a starting position in which the electrode is seated within the housing when the contact force applied to the electrode is removed.

[0056] In some embodiments, the electrodes may be free of attachments from the sensor housing, allowing the electrodes to move relative to the housing. In other embodiments, however, the electrodes may be physically attached to the housing, but with slack and/or elasticity in the attachment arrangement (e.g., via a spring) to permit movement of the electrodes relative to the housing.

[0057] According to another aspect, in some embodiments described herein, a neuromuscular (e.g., sEMG) electrode (also referred to herein as a sensor) arrangement includes a spring element that biases the neuromuscular electrode to press against the body surface when the neuromuscular recording system that contains the neuromuscular electrode is worn by a user. The spring element may be configured to bias the electrode in a starting position in which the electrode extends outwardly from the sensor housing, while permitting the electrode to move inwardly into the housing upon application of sufficient force against the electrode.

[0058] One illustrative implementation of the neuromuscular (e.g., sEMG) electrode (also referred to herein as a sensor) 504 shown in FIGS. 2, 3, and 9A-B is provided in FIG. 4, according to some embodiments. The neuromuscular recording sensor 504 includes dry electrodes 600, 602 and a housing 510, which may be made up of an upper housing 512 and a lower housing 516. The electrodes 600, 602 are moveable relative to the housing 510. In the embodiment shown in FIG. 4, the electrodes are free from attachment to the housing. The sensor housing 510 defines an opening 517 through which the electrode extends and/or moves through. The sensor includes a spring element 530 to bias the electrodes 600, 602 in a stationary starting position relative to the housing. At least a portion of the spring element may be contained within the housing 510. The inventors have recognized that other materials that function as a spring may be used instead of or in addition to the spring element 530. For example, a foam component may be positioned above the electrode within the housing.

[0059] When a force is applied to the electrodes 600, 602, e.g., due to contact of skin against the electrodes, the electrodes move relative to the housing, e.g. by rotating, translating, or both. Movement of the electrodes relative to the housing compresses the spring element 530, causing the spring element to store potential energy. When the force applied to the electrodes decreases, the spring element releases the stored potential energy and decompresses, pushing the electrodes back toward their starting positions.

[0060] In the illustrative embodiment shown in FIG. 4, the electrodes 600, 602 have five degrees of freedom relative to the housing 510. The electrodes can translate in the X, Y, and Z axes, and rotate about the X and Y axes. The vertical Z axis is oriented along the height of the sensor, the Y axis is oriented along the depth of the sensor, and the X axis is oriented along the width of the sensor. In some embodiments, the electrode has a longitudinal axis 200 that passes through a center of the electrode. The longitudinal axis 200 may bisect the electrode. The longitudinal axis is parallel to the Z axis when the electrode is in the starting position. In some embodiments, the plane of the opening 517 is parallel with the X-Y plane, and an axis normal to the plane of the opening 517 is parallel with the Z axis and with the longitudinal axis 200 of the electrode.

[0061] In some embodiments, the electrode is configured to translate relative to the housing in a direction perpendicular to the plane of the opening of the housing. In some embodiments, the electrode is configured to translate relative to the housing in a direction parallel to the plane of the opening of the housing.

[0062] In some embodiments, such as that shown in FIG. 4, the electrode is prohibited from rotation about the Z axis (yaw rotation). However, in other embodiments, the electrode is permitted to rotate about the Z axis.

[0063] FIG. 5 illustrates a few examples of different positions to which an electrode 600 in an assembly configured according to some embodiments may move during use. At rest, without any contact forces being applied to the electrode, the electrode is in the starting position 620, in which the electrode extends through the opening 517 of the housing, where a portion of the electrode is positioned within the housing 510 and a portion of the electrode is positioned outside the housing. In some embodiments, in the starting position, the portion of the electrode positioned outside the housing is larger than the portion of the electrode positioned inside the housing. In some embodiments, in the starting position, the electrode is aligned with the opening of the housing such that the longitudinal axis 200 of the electrode is parallel to the plane of the opening 517. If the opening 517 has a midpoint, the longitudinal axis of the electrode may extend through the midpoint of the opening.

[0064] Upon an application of force to the electrode, the electrode may move into an intermediate position 621 in which a greater portion of the electrode is positioned within the housing 510 as compared to the starting position 620. In the intermediate position 621 shown in FIG. 5, the electrode is both rotated and raised relative to the original starting position 620.

[0065] Finally, with an increase of force to the electrode, the electrode may move into a compressed position 622 in which an entirety of the electrode is positioned within the housing. In some embodiments, the position 622 shown in FIG. 5 is a fully raised position such that the electrode cannot move any further into the housing. However, in other embodiments, the electrode is able to move still further into the housing. In yet other embodiments, when the electrode is in the fully raised position, a portion of the electrode remains outside the housing.

[0066] Distance D shown in FIG. 5 is the distance of travel of the electrode from the starting position 620 to the compressed position 622. Distance D is also the distance from the bottom surface 680 of the electrode to the bottom surface 513 of the housing 510. In some embodiments, distance D is also the maximum travel distance of the electrode. The inventors recognize that larger values of D permit a larger range of motion of the electrode in the Z-dimension upon a force being exerted upon the electrode (e.g., due to a change in the relative force between the portion of a user's body underlying the electrode and the housing of a wearable neuromuscular recording device that contains the electrode), while also enabling electrode contact to be maintained if the housing of the wearable neuromuscular recording apparatus is positioned such that a particular electrode of the apparatus is relatively far (e.g., having a distance D) from the surface of the body (e.g., skin). The inventors have recognized that a larger value of D requires a larger housing for that section of the wearable neuromuscular recording device to permit movement of the electrode into the housing up to a distance of D. The inventors have recognized that the value of D should be selected to balance the various constraints listed above for a given form factor of a neuromuscular recording apparatus and portion of the body on which it is intended to be worn.

[0067] In some embodiments, different electrodes of a neuromuscular recording device that includes a plurality of electrodes may be configured with different values of D based on the expected range of motion required for that electrode given the form factor of the apparatus and the

portion of the body on which it is meant to be worn. For example, an apparatus for neuromuscular recording on the wrist may be configured with electrodes having a larger distance D for electrodes overlying the top and bottom of the wrist and a smaller distance D for electrodes overlying the sides of the wrist, because relative movement of tissue is generally larger at the top and bottom of the wrist where soft tissue (tendons, muscles, etc.) is present than for the side of the wrist where bones are present with less soft tissue.

[0068] In some embodiments, distance D may be at least about 0.01 mm, at least about 0.1 mm, at least about 1 mm, at least about 1.2 mm, at least about 1.4 mm, at least about 1.6 mm, at least about 1.8 mm, at least about 2 mm, at least about 2.2 mm, or at least about 2.4 mm. In some embodiments, distance D may be less than or equal to about 4 mm, less than or equal to about 3 mm, less than or equal to about 2.8 mm, less than or equal to about 2.6 mm, less than or equal to about 2.4 mm, less than or equal to about 2.2 mm, less than or equal to about 2 mm, or less than or equal to about 1.8 mm. Combinations of the above-referenced ranges are also possible. For example, in some embodiments, the distance D may be about 1 mm to about 4 mm, or about 1.2 mm to about 3 mm, or about 1.4 mm to about 2.6 mm, or about 1.6 mm to about 2.4 mm, or about 1.8 mm to about 2.2 mm, or about 2 mm.

[0069] In some embodiments, the electrode must move a threshold distance in the Z direction along the height of the sensor (e.g. in a direction perpendicular to the plane of the opening into the housing) before the electrode is free to translate and rotate on the other two axes perpendicular to the Z axis. In other embodiments, no threshold distance is needed.

[0070] The electrodes may be configured to contour to the body, e.g., by reaching into a valley or cleft between muscles and maintain contact while the user moves and contracts muscles in the body part to which the electrodes are coupled to, e.g., the arm. Thus, the inventors have recognized that the assemblies of neuromuscular recording devices that permit movement (e.g., translation and/or rotation) of one or more electrodes as described herein must have dynamics that are responsive (e.g., via appropriate selection of spring constants of materials) at the timescales of movement of the musculoskeletal system (e.g., hundreds of milliseconds to seconds).

[0071] In some embodiments, the electrode 600 has a contact surface 680 that is configured to make contact with the body surface, e.g., skin. In some embodiments, the contact surface 680 may have a surface that is curved in a convex shape to help the electrode roll along the body surface during muscle movements to decrease sliding artifacts. The surface may be contoured in a variety of ways, such as to avoid hair, and to move with the skin. For example, instead of having a uniformly curved convex shape, the surface of the electrode may have some sections that are concave or otherwise have a different curvature/contour to facilitate movement relative to the skin.

[0072] It should be appreciated that different degree of freedom arrangements are contemplated. In some embodiments, an electrode rotates relative to the sensor housing. In some embodiments, an electrode has at least two degrees of freedom relative to the sensor housing. For example, the electrode may translate and rotate, or, the electrode may translate along two axes, or, the electrode may rotate about two axes. In some embodiments, an electrode has at least

two degree of freedom, or, at least three degrees of freedom, or at least four degrees of freedom, or at least five degrees of freedom, or six degrees of freedom relative to the housing.

[0073] In some embodiments, the sensor includes a flexible circuit that permits movement of the electrode relative to the housing. In embodiments with the sensor having a plurality of electrodes, the flexible circuit connects the electrodes together. In some embodiments, a portion of the circuit includes one or more rigid printed circuit boards (“PCBs”) and a portion of the circuit includes one or more flexible PCBs. In some embodiments, a rigid PCB is fixed to each of the electrodes, and the flexible PCBs connect the rigid PCBs to one another. In some embodiments, the flexible PCB is also connected to each of the electrodes. The inventors recognize that the use of one or more flexible PCBs in the mechanical assemblies for a wearable neuromuscular recording device as described herein enable movement of electrodes relative to rigid elements and the housing, so that the electrode is able to maintain contact with the skin as the wearable device moves relative to the user’s body surface (e.g., skin).

[0074] In the illustrative embodiment shown in FIG. 4, the sensor 504 has a rigid PCB 545 and a flexible PCB 542 attached to the electrode 600 on the longer base 670 side of the electrode. The sensor 504 also includes another rigid PCB 544 in an upper portion of the sensor, above the spring element 530. The flexible PCB 542 may also connect to the upper rigid PCB 544.

[0075] The illustrative embodiment shown in FIGS. 6A and 6B shows an example of how a flexible circuit may be used to connect the electrodes together. As best seen in FIG. 6A, a rigid PCB 544 may be attached to each of the electrodes, and a flexible PCB 542 connects each of the rigid PCBs 544 together. The flexible PCB is also connected to each of the electrodes 600, 602, 604, with the flexible PCB between each of the electrodes and their associated rigid PCB. The flexible PCB also connects to an upper rigid PCB 544.

[0076] The flexible PCB may include portions of slack 543 between the electrodes that allow for independent movement between the electrodes. The portions of slack may form a curved arc shape when each of the electrodes are in a starting position. When one electrode moves relative to another, the portions of slack may change conformation from a curved shape to more of a linear shape.

[0077] In some embodiments, the electrodes are manufactured as a single, monolithic piece of metal, and connected to the flexible circuit. The electrodes may be soldered to the flexible circuit using fabrication techniques such as wave or reflow soldering, or pin/socket connectorization.

[0078] In the illustrative embodiment shown in FIG. 6B, the electrodes 600, 602, 604 each include a socket 660. For each of the electrodes, a pin 662 is passed through the socket of the electrode and through the rigid and flexible PCBs, connecting the electrodes to the PCBs.

[0079] In some embodiments, the electrode interacts with the spring element via a pin and socket relationship. For example, the electrode may have a protruding post, and the spring element may have a socket that is sized to receive the post of the electrode. In some embodiments, the diameter of the socket is larger than the diameter of the post such that there is some clearance around the post when the post sits within the socket. In some embodiments, the diameter of the

socket is equal to the diameter of the post. In some embodiments, the diameter of the socket is smaller than the diameter of the post to create an interference fit between the socket and the post.

[0080] In the illustrative embodiment shown in FIG. 4, the electrode 600 has a post 630 that is received within a socket 532 of the spring element. In some embodiments, the post is integrally formed with the electrode as a single, monolithic component.

[0081] In some embodiments, a thermal relief is positioned between the electrode and the PCB. A thermal relief may be, for example, an indentation or cutout in a surface of an electrode. For example, as shown in the FIG. 4 embodiment, a thermal relief 640 is an indentation in the 670 surface of the electrode and is located between the electrode 600 and the PCBs 542 and 545. The thermal relief may be located at the surface of the electrode that faces the PCBs. The thermal relief may span across an area that is smaller than the area of overlap between the PCBs and the electrode, such that direct contact may be made between the electrode and the PCBs.

[0082] In some embodiments, the electrode and post is soldered to the PCBs of the circuit. The thermal relief 640 may help to dissipate heat from the soldering process to decrease the amount of heat that is transferred to the PCBs. In some embodiments, movement of the electrode may cause the post to heat up, e.g. due to friction. The thermal relief 640 of the electrode may serve to dissipate the heat from the post to decrease the amount of heat that is transferred to the PCBs. In some embodiments, spring element 530 may be made of an insulating material that absorbs heat from the post.

[0083] A wearable device may incorporate a plurality of neuromuscular recording (e.g., sEMG) sensors having moveable electrodes. Each of the sensors may be electrically connected with one another. The housings of each of the sensors may be coupled to one another to form the wearable device. In some embodiments, the housings of adjacent sensors may be attached to one another while remaining moveable relative to one another. The housings of adjacent sensors may have one, two, three, four, five, or six degrees of freedom relative to one another. In some embodiments, the housings of adjacent sensors are attached to one another via a hinge and are free to pivot relative to one another. In some embodiments, the housings of adjacent sensors are attached to one another via an elastic band and are free to pivot and translate relative to one another.

[0084] In the illustrative embodiment shown in FIG. 2, adjacent sensor housings are attached to one another via joints 501. Sensors are connected to one another via joints to form a curveable array of sensors extending from a first end 410 to a second end 420. To form a closed loop, a band 502 may be used to connect the ends 410, 412 of the arc of sensors. The joints 501 between the sensors may have the ability to permit adjacent sensors to pivot relative to one another and/or be pulled away from one another. The band may form a complete loop that is coupled to the array of sensors, as best seen in FIG. 3. The band 502 may have elastic properties to create a biasing force that provides continuous pressure of the electrodes against the wearer's body surface, e.g., the skin of the wearer's arm. This continuous pressure provided by the elastic band is opposed by the biasing force provided by the spring elements in each of the sensors. The pressure of the electrodes against the

body surface created by the elastic band may cause the electrodes of the sensors 504 to move relative to the sensor housings, causing the spring elements of the sensors to compress. As the wearer moves and/or contracts muscles in the body part on which the device is worn, the continuous pressure provided by the elastic band, along with the ability of the electrodes to move relative to the sensor housings with the moving skin, help to keep the electrodes in contact with the skin. In some embodiments, the housings themselves and the joints that connect them form a wearable device such that a separate band coupled to the housings is not required.

[0085] The spring element 530 is a component that is capable of storing potential energy. In the illustrative embodiments shown in the figures, the spring element is an elastically compressible block of material. Examples of possible materials for the spring element include, but are not limited to, neoprene, EPDM, foam, silicone rubber, natural rubber, synthetic rubber, sponge rubber, foam rubber, other rubbers, PVC, thermoplastic polymers. The spring element may take on different forms other than a block of material. For example, the spring element may be a helical spring such as a coil spring, tapered spring, or hourglass spring, or the spring element may be a leaf spring, torsion spring, disc spring, clock spring, flat spring, wave spring, hourglass spring, a stretchable fabric, an elastically compressible component, or any other component that can be used to store potential energy.

[0086] The spring element may be a single component, as with the compressible block shown in the figures, or may be a collection of multiple components, such as a plurality of spring coils spread out over an area of the electrode, e.g., one on each corner of the upper surface of the electrode and one or more coils in a central region of the upper surface of the electrode.

[0087] As discussed above, in some embodiments, the housings of adjacent sensors are attached to one another via a hinge and are free to pivot relative to one another. In some embodiments, the electrode within the sensor housing only has one degree of freedom relative to the sensor housing, with extra degrees of freedom provided by the hinge connecting adjacent sensors. For example, a spring element 1110 oriented in the axis normal to the sensor housing may provide the single degree of freedom for the electrode relative to the housing as shown, for example, in FIG. 11A. As shown in FIG. 11B, hinge 1120 may provide additional degree(s) of freedom. In such an arrangement, the combination of the single degree of freedom provided by the spring element 1110 and the additional one or more degrees of freedom provided by the hinge 1120 provide a wearable biosensor recording device with multiple degrees of freedom to enable electrodes to remain in contact with the body surface (e.g., the skin) during movements and/or muscle contractions, as described herein.

[0088] In some embodiments, the spring element may be made of a material having a Young's Modulus of at least about 0.5 MPa, at least about 1 MPa, at least about 1.5 MPa, at least about 2 MPa, at least about 2.5 MPa, at least about 3 MPa, at least about 3.5 MPa, at least about 4 MPa, at least about 4.5 MPa, at least about 5 MPa, at least about 5.5 MPa, at least about 6 MPa, at least about 6.5 MPa, at least about 7 MPa, at least about 7.5 MPa, at least about 8 MPa, at least about 8.5 MPa, at least about 9 MPa, at least about 9.5 MPa, or at least about 10 MPa. In some embodiments, the spring element may be made of a material having a Young's

Modulus of less than or equal to about 10 MPa, less than or equal to about 9.5 MPa, less than or equal to about 9 MPa, less than or equal to about 8.5 MPa, less than or equal to about 8 MPa, less than or equal to about 7.5 MPa, less than or equal to about 7 MPa, less than or equal to about 6.5 MPa, less than or equal to about 6 MPa, less than or equal to about 5.5 MPa, less than or equal to about 5 MPa, less than or equal to about 4.5 MPa, less than or equal to about 4 MPa, less than or equal to about 3.5 MPa, less than or equal to about 3 MPa, less than or equal to about 2.5 MPa, less than or equal to about 2 MPa, less than or equal to about 1.5 MPa, or less than or equal to about 1 MPa. Combinations of the above-referenced ranges are also possible. For example, in some embodiments, the spring element may be made of a material having a Young's Modulus of about 0.5 MPa to about 10 MPa, or about 1.5 MPa to about 9 MPa, or about 2.5 MPa to about 8 MPa, or about 3.5 MPa to about 7 MPa, or about 5 MPa to about 6.5 MPa, or about 5 to 7 MPa, or about 6 MPa.

[0089] In some embodiments, the spring element may have a spring constant k of at least about 1.5 N/mm, 2 N/mm, 2.5 N/mm, 3 N/mm, 3.5 N/mm, 3.75 N/mm, 4 N/mm, 4.5 N/mm, or 5 N/mm. In some embodiments, the spring element may have a spring constant k of less than or equal to about 10 N/mm, 9 N/mm, 8 N/mm, 7 N/mm, 6 N/mm, 5 N/mm, 4 N/mm, 3.75 N/mm, 3.5 N/mm, 3 N/mm, or 2 N/mm. Combinations of the above-referenced ranges are also possible. For example, in some embodiments, the spring element may have a spring constant k of about 1.5 N/mm to about 10 N/mm, or about 2 N/mm to about 8 N/mm, or about 2.5 N/mm to about 6 N/mm, or about 3 N/mm to about 4 N/mm, or about 3.5 N/mm to about 4 N/mm, or about 3.75 N/mm.

[0090] In some embodiments, the spring element may behave as a nonlinear spring.

[0091] In some embodiments, the spring element may provide different spring forces and/or mechanical resistances on different axes. This may be accomplished by a spring element that is a single component, or a spring element that is a collection of components.

[0092] In some embodiments, the spring element is unattached to the electrode and/or to the housing. In some embodiments, the spring element is not physically attached to any components of the sensor. Instead, the spring element is free-floating. The spring element may be constrained from movement due to the physical presence of other components arranged on either side and/or surrounding the spring element. For example, in the embodiment shown in FIG. 4, the spring element 530 is sandwiched between rigid PCB 544 and rigid PCB 545. In some embodiments, the sides of the spring element may be constrained from lateral movement by the inner surfaces of the housing.

[0093] According to some aspects, in some embodiments, physical interaction between the housing and the electrode determines the starting position of the electrode. The housing may be shaped to accommodate the shape of the electrode such that the housing guides the electrode back into its starting position when the electrode is no longer subjected to a contact force. In some embodiments, the electrode has only a single starting position.

[0094] In some embodiments, the housing has an inner surface with sloped walls that serve as a funnel to guide the electrode back toward its starting position. For example, in the illustrative embodiment shown in FIGS. 4 and 5, the

housing 510 has inner surfaces 515 adjacent to the opening 517 into the housing. The inner surfaces are angled inwardly toward one another to create a funnel effect. To cooperate with these inner surfaces, the electrode has side surfaces 682, 683 that are also sloped inwardly toward one another. The side surfaces of the electrode may be sloped at a same angle as that of the inner walls of the housing. As a result, when the spring element releases potential energy and pushes the electrode back out of the housing toward the starting position, the inner surfaces of the housing may help to properly seat the electrode within the opening 517 of the housing into the starting position.

[0095] The electrodes shown in FIGS. 4-6B have a trapezoidal prism shape. In some embodiments, when the electrode is in the starting position, the longer base 670 of the trapezoidal prism is located within the housing 510 and the shorter base is the contact surface 680, which is located outside the housing, and the two side surface 682 and 683 connect the longer base 670 to the shorter base/contact surface 680. Note that, in embodiments where contact surface 680 is curved in a convex shape, the approximate shape of the electrode is still considered to be trapezoidal even though the two bases 670, 680 are not technically parallel to one another.

[0096] It should be appreciated that different electrode shapes and housing shapes are contemplated. For example, the electrode may have a cross-sectional shape that is or is approximately trapezoidal, triangular, rectangular, square, semicircular, semi-elliptical, domed, round, or any other suitable shape. The electrode may be or may approximate the shape of: a cylinder, prism (including rectangular prism and trapezoidal prism), cube, cuboid, conical frustum, square frustum, pentagonal frustum, a hemisphere, a dome, an elongated dome, egg-shaped, an ellipsoid, a semi-ellipsoid, or any other suitable shape.

[0097] In one illustrative embodiment shown in FIGS. 7A and 7B, an electrode 600 may have side surfaces 682, 683 that are parallel to one another rather than sloped. As seen in FIG. 7B, the electrode 600 has an approximately rectangular cross-section, with the contact surface 680 being outwardly curved in a convex shape.

[0098] In the embodiment shown in FIGS. 7A and 7B, without sloped side surfaces to provide a funneling effect, the electrode may include a different feature to permit the electrode to be seated within the opening of the housing. The electrode includes shoulders 650 that interact with the housing to seat the electrode in place. The housing has contact surfaces in the form of ledges 518 protruding from the inner surface of the housing, where the ledges are sized and shaped to receive the shoulders 650 of the electrode. As seen in FIG. 7B, with the electrode 600 in the starting position, the shoulders 650 of the electrode are pushed by the spring element 530 against the ledges 518 of the housing to seat the electrode in place within the opening 517 of the housing. The shoulders of the electrode may protrude outwardly beyond the side surfaces 682, 683 of the electrode, as shown in FIG. 7B.

[0099] In another illustrative embodiment shown in FIGS. 8A and 8B, electrode 600 has a round form. The electrode has one continuous sidewall 686 that extends around the entire electrode. The electrode 600 has an approximately frustoconical shape, with a longer base 670 and a shorter base 680 that serves as a contact surface. The contact surface

680 may be curved outwardly in a convex shape. As seen in FIG. **8B**, the cross-sectional shape of the electrode is approximately trapezoidal.

[0100] A housing shaped to accommodate a frustoconical electrode such as the one shown in FIGS. **8A** and **8B** may have a circular inner wall surface that is slanted to match the angle of the sidewall **686** of the electrode. The opening defined by the housing through which the electrode extends and moves may be circular.

[0101] It should be appreciated that different electrode shapes may be used for the sensor, and the sensor housing may have different conformations to accommodate and guide movement of such electrodes.

[0102] Having thus described several aspects of at least one embodiment of this invention, it is to be appreciated that various alterations, modifications, and improvements will readily occur to those skilled in the art.

[0103] Such alterations, modifications, and improvements are intended to be part of this disclosure, and are intended to be within the spirit and scope of the invention. Further, though advantages of the present invention are indicated, it should be appreciated that not every embodiment of the technology described herein will include every described advantage. Some embodiments may not implement any features described as advantageous herein and in some instances one or more of the described features may be implemented to achieve further embodiments. Accordingly, the foregoing description and drawings are by way of example only.

[0104] Various aspects of the apparatus and techniques described herein may be used alone, in combination, or in a variety of arrangements not specifically discussed in the embodiments described in the foregoing description and is therefore not limited in its application to the details and arrangement of components set forth in the foregoing description or illustrated in the drawings. For example, aspects described in one embodiment may be combined in any manner with aspects described in other embodiments.

[0105] Use of ordinal terms such as “first,” “second,” “third,” etc., in the claims to modify a claim element does not by itself connote any priority, precedence, or order of one claim element over another or the temporal order in which acts of a method are performed, but are used merely as labels to distinguish one claim element having a certain name from another element having a same name (but for use of the ordinal term) to distinguish the claim elements.

[0106] Also, the phraseology and terminology used herein is for the purpose of description and should not be regarded as limiting. The use of “including,” “comprising,” or “having,” “containing,” “involving,” and variations thereof herein, is meant to encompass the items listed thereafter and equivalents thereof as well as additional items.

1. A wearable bioelectrical sensing device comprising:
 - a plurality of electrodes including a first electrode, a second electrode, a third electrode, and a fourth electrode;
 - a first housing containing at least a portion of the first electrode and at least a portion of the second electrode, each of the first and second electrode being configured to rotate relative to the first housing from a starting position to a rotated position;
 - a second housing containing at least a portion of the third electrode and at least a portion of the fourth electrode, each of the third and fourth electrodes being configured

to rotate relative to the second housing, wherein the first housing and the second housing are coupled to each other in an arrangement that enables the first, second, third, and fourth electrode to contact a body part of a user when the wearable bioelectrical sensing device is worn around the body part of the user;

- a first flexible circuit electrically connecting the first electrode to the second electrode within the first housing;
 - a second flexible circuit electrically connecting the third electrode to the fourth electrode within the second housing; and
 - a spring element configured to bias the first electrode toward the starting position of the first electrode.
2. The wearable bioelectrical sensing device of claim 1, wherein at least a portion of the spring element is contained within the first housing.
 3. The wearable bioelectrical sensing device of claim 1, wherein the spring element comprises foam or neoprene.
 4. The wearable bioelectrical sensing device of claim 1, wherein the first housing defines an opening and, in the starting position, the first electrode extends through the opening of the first housing.
 5. The wearable bioelectrical sensing device of claim 4, wherein the first electrode is configured to translate relative to the first housing in a direction perpendicular to a plane of the opening.
 6. The wearable bioelectrical sensing device of claim 4, wherein the first electrode is configured to translate relative to the first housing in a direction parallel to a plane of the opening.
 7. The wearable bioelectrical sensing device of claim 1, wherein the first electrode is configured to translate relative to the first housing.
 8. The wearable bioelectrical sensing device of claim 7, wherein the first electrode is configured to translate a distance relative to the first housing before the first electrode is permitted to rotate relative to the first housing.
 9. The wearable bioelectrical sensing device of claim 1, wherein the first electrode is configured to rotate relative to the first housing about a first axis and a second axis that is perpendicular to the first axis.
 10. The wearable bioelectrical sensing device of claim 9, wherein the first electrode is prohibited from rotating about a third axis perpendicular to the first axis and the second axis.
 11. The wearable bioelectrical sensing device of claim 10, wherein the first housing defines an opening and, in the starting position, the first electrode extends through the opening of the first housing, and the third axis comprises a vertical axis that is perpendicular to a plane of the opening.
 12. The wearable bioelectrical sensing device of claim 11, wherein the first electrode is prohibited from yaw rotation about the vertical axis.
 13. The wearable bioelectrical sensing device of claim 1, wherein the first electrode is configured to translate relative to the first housing in three dimensions.
 14. The wearable bioelectrical sensing device of claim 1, further comprising a post attached to the first electrode and extending through the spring element.
 15. The wearable bioelectrical sensing device of claim 14, wherein the post is integrally formed with the first electrode as a single, monolithic component.

16. The wearable bioelectrical sensing device of claim 1, wherein a range of movement of the first electrode relative to the first housing is different than a range of movement of the third electrode relative to the second housing.

17. The wearable bioelectrical sensing device of claim 1, wherein a cross section of the first electrode has a shape selected from the group consisting of a trapezoidal shape, a rectangular shape, a circular shape, and an elliptical shape.

18. The wearable bioelectrical sensing device of claim 17, wherein the first electrode has a curved contact surface.

19. The wearable bioelectrical sensing device of claim 1, further comprising a band coupled to the first housing and the second housing to provide the arrangement that enables the first, second, third, and fourth electrode to contact the body part of the user when the wearable bioelectrical sensing device is worn around the body part of the user.

20. The wearable bioelectrical sensing device of claim 1, further comprising a hinge coupling the first housing and the second housing to provide the arrangement that enables the first, second, third, and fourth electrode to contact the body part of the user when the wearable bioelectrical sensing device is worn around the body part of the user.

21. A wearable bioelectrical sensing device, comprising:
a plurality of electrodes including a first electrode, a second electrode, a third electrode, and a fourth electrode;

a first housing containing at least a portion of the first electrode and at least a portion of the second electrode, each of the first and second electrodes being movable relative to the first housing with at least one degree of freedom such that each of the first electrode and second electrode is movable from a starting position to a different position relative to the first housing;

a second housing containing at least a portion of the third electrode and at least a portion of the fourth electrode, each of the third and fourth electrodes being movable relative to the second housing with at least one degree of freedom such that each of the third electrode and the fourth electrode is movable from a starting position to a different position relative to the second housing, wherein the first housing and the second housing are coupled to each other in an arrangement that enables the first, second, third, and fourth electrode to contact a body part of a user when the wearable bioelectrical sensing device is worn around the body part of the user;
a first flexible circuit electrically connecting the first electrode to the second electrode within the first housing;

a second flexible circuit electrically connecting the third electrode to the fourth electrode within the second housing; and

a spring element configured to bias the first electrode toward the starting position of the first electrode.

22. The wearable bioelectrical sensing device of claim 21, wherein each of the first and second electrodes is movable relative to the first housing with at least two degrees of freedom.

23. The wearable bioelectrical sensing device of claim 21, wherein the first electrode is movable relative to the first housing with five degrees of freedom, and wherein the five degrees of freedom comprise translation along a first axis, a

second axis, and a third axis, and rotation about the first axis and the second axis, wherein the first axis, second axis and third axis are perpendicular to one another.

24. The wearable bioelectrical sensing device of claim 21, further comprising a hinge coupling the first housing and the second housing to provide the arrangement that enables the first, second, third, and fourth electrode to contact the body part of the user when the wearable bioelectrical sensing device is worn around the body part of the user.

25. The wearable bioelectrical sensing device of claim 24, wherein the hinge is configured to enable the first electrode to move relative to the first housing with at least one additional degree of freedom.

26. A method of using a wearable bioelectrical sensing device, the method comprising:

wearing the wearable bioelectrical sensing device to contact a first electrode, a second electrode, a third electrode, and a fourth electrode of the device with skin, wherein the wearable bioelectrical sensing device includes a first housing containing at least a portion of the first electrode and at least a portion of the second electrode, and a second housing containing at least a portion of the third electrode and at least a portion of the fourth electrode; and

rotating the first electrode relative to the first housing from a starting position to a rotated position while keeping the first electrode in contact with the skin throughout the rotation.

27. The method of claim 26, further comprising:

compressing a spring element contained within the first housing while rotating the first electrode relative to the first housing, the spring element being configured to bias the first electrode toward the starting position.

28. The method of claim 26, wherein rotating the first electrode relative to the first housing occurs about a first axis, and wherein the method further comprises rotating the first electrode relative to the first housing about a second axis that is perpendicular to the first axis while keeping the first electrode in contact with the skin throughout the rotation.

29. A method of using a wearable bioelectrical sensing device, the method comprising:

wearing the wearable bioelectrical sensing device to contact a first electrode, a second electrode, a third electrode, and a fourth electrode of the device with skin, wherein the wearable bioelectrical sensing device includes a first housing containing at least a portion of the first electrode and at least a portion of the second electrode, and a second housing containing at least a portion of the third electrode and at least a portion of the fourth electrode; and

moving the first electrode relative to the first housing with at least two degrees of freedom from a starting position to a different position.

30. The method of claim 29, further comprising moving the first electrode with five degrees of freedom relative to the first housing, wherein the five degrees of freedom comprise translation along a first axis, a second axis, and a third axis, and rotation about the first axis and the second axis, wherein the first axis, second axis and third axis are perpendicular to one another.

专利名称(译)	用于可穿戴神经肌肉记录设备的改善信号鲁棒性的方法和设备		
公开(公告)号	US20200022606A1	公开(公告)日	2020-01-23
申请号	US16/516777	申请日	2019-07-19
[标]发明人	BARBRE CURTIS REID JONATHAN GUO NING		
发明人	BARBRE, CURTIS REID, JONATHAN GUO, NING POOL, BRANDON		
IPC分类号	A61B5/0488 A61B5/00		
CPC分类号	A61B5/0488 A61B2560/0406 A61B5/6801 A61B2562/04 A61B5/01 A61B5/02438 A61B5/11 A61B5/6824		
优先权	62/700434 2018-07-19 US		
外部链接	Espacenet USPTO		

摘要(译)

描述了用于改善神经肌肉记录电极与身体表面接触的布置。根据一些方面，一种传感器组件可以包括壳体和多个相对于壳体可移动的电极。电极可以相对于壳体旋转和/或平移和/或相对于壳体具有至少两个自由度。传感器可以包括弹簧元件，该弹簧元件存储势能并将电极偏置到起始位置，在该起始位置中，电极至少部分地延伸出传感器壳体。在一些实施例中，对传感器的一个或多个电极施加接触力会压缩弹簧元件，从而导致弹簧元件存储势能。

