



US010206602B2

(12) **United States Patent**
Ren et al.

(10) **Patent No.:** **US 10,206,602 B2**
(45) **Date of Patent:** **Feb. 19, 2019**

(54) **HYBRID ELECTROMAGNETIC FIELD SIGNAL DETECTION SYSTEM FOR HUMAN BIOELECTRICAL SIGNAL MONITORING**

(71) Applicant: **LR Technologies, Inc.**, Rockville, MD (US)

(72) Inventors: **Eugene Yu-Jiun Ren**, San Marcos, CA (US); **Yexian Qin**, Tucson, AZ (US); **Chiehping Lai**, Rockville, MD (US)

(73) Assignee: **LR TECHNOLOGIES, INC.**, Rockville, MD (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(21) Appl. No.: **15/946,715**

(22) Filed: **Apr. 5, 2018**

(65) **Prior Publication Data**
US 2018/0289279 A1 Oct. 11, 2018

Related U.S. Application Data
(60) Provisional application No. 62/482,123, filed on Apr. 5, 2017.

(51) **Int. Cl.**
A61B 5/05 (2006.01)
H01Q 1/27 (2006.01)
H04Q 9/02 (2006.01)
A61B 5/0464 (2006.01)
A61B 5/00 (2006.01)
A61B 5/0476 (2006.01)

(52) **U.S. Cl.**
CPC **A61B 5/05** (2013.01); **A61B 5/0464** (2013.01); **A61B 5/0476** (2013.01); **A61B 5/6804** (2013.01); **A61B 5/721** (2013.01); **A61B 5/7264** (2013.01); **H01Q 1/273** (2013.01); **H04Q 9/02** (2013.01); **H04Q 2209/40** (2013.01)

(58) **Field of Classification Search**
CPC A61B 5/05; A61B 5/7264; A61B 5/0476; A61B 5/6804; A61B 5/721; A61B 5/0464; H04Q 9/02; H04Q 2209/40; H01Q 1/273
See application file for complete search history.

(56) **References Cited**

PUBLICATIONS

Sullivan, Thomas J., et al., "A Low-Noise, Non-Contact EEG/ECG Sensor", IEEE Biomedical Circuits and System Conference 2007, Montreal, Quebec, Canada, Nov. 27-30, 2007, pp. 154-157.


Primary Examiner — Rex R Holmes

(74) *Attorney, Agent, or Firm* — Perkins Coie LLP

(57) **ABSTRACT**

The present disclosure includes an electromagnetic field detection and monitoring system. The system includes passive detection, active detection, and signal processing capabilities. At least one embodiment includes a body worn system with sensing, processing, communications, and data storage capabilities. The system provides wearable antennas to transfer the EMF energy in its electrical or magnetic forms into the sensor efficiently. A specially designed processing algorithm can process the collected data and generated the results for medical professionals to read and make decisions.

26 Claims, 11 Drawing Sheets

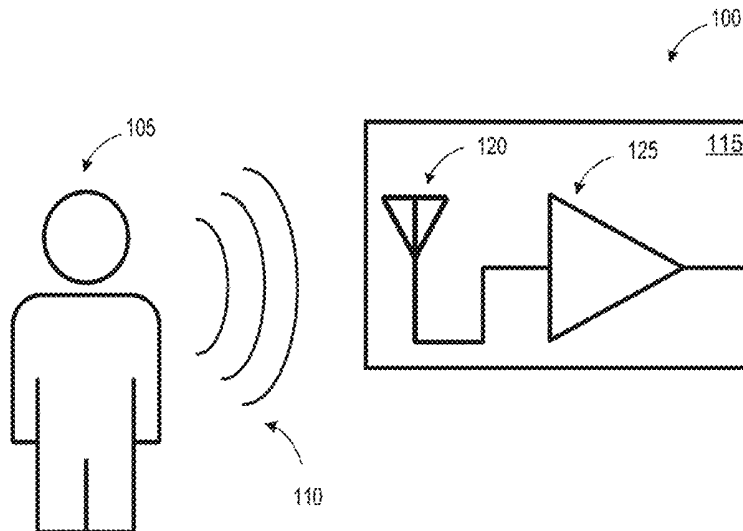

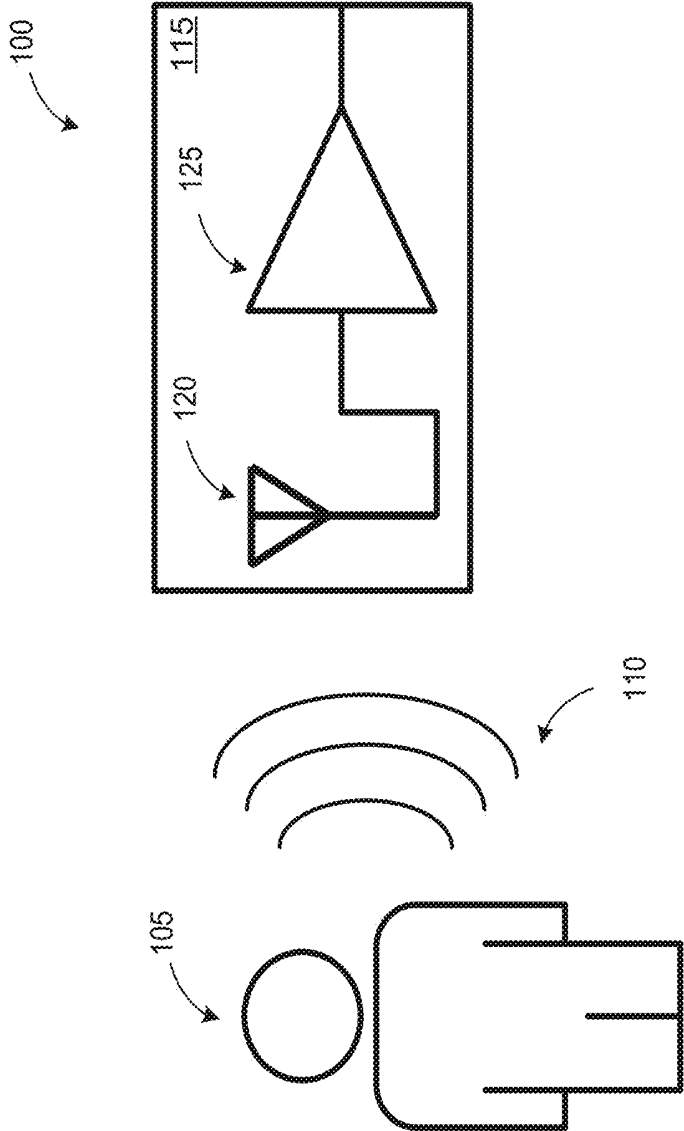


FIG. 1

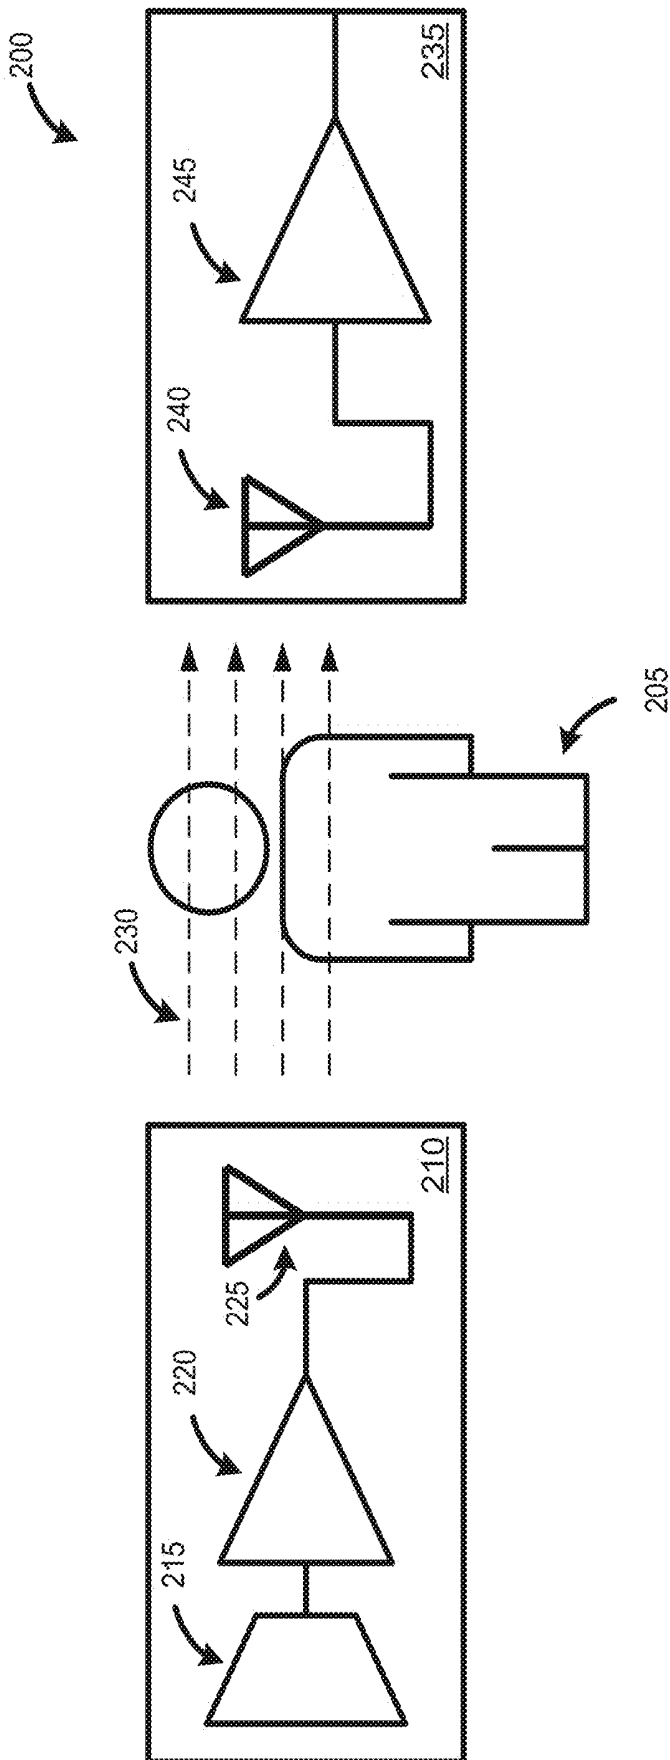


FIG. 2

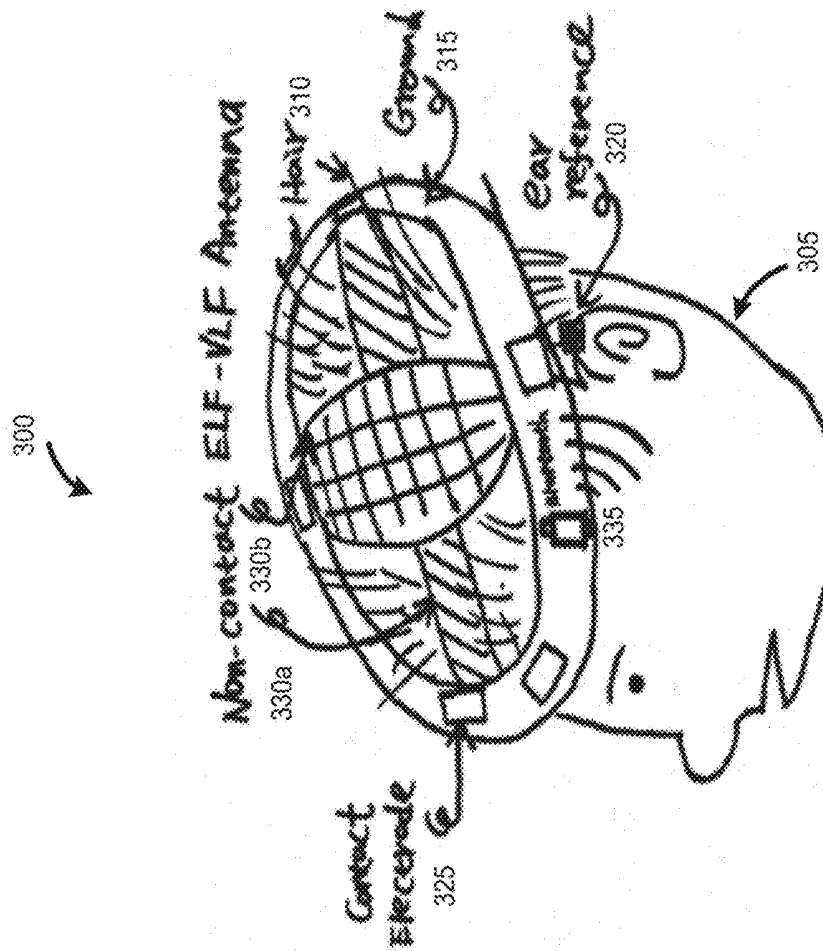


FIG. 3

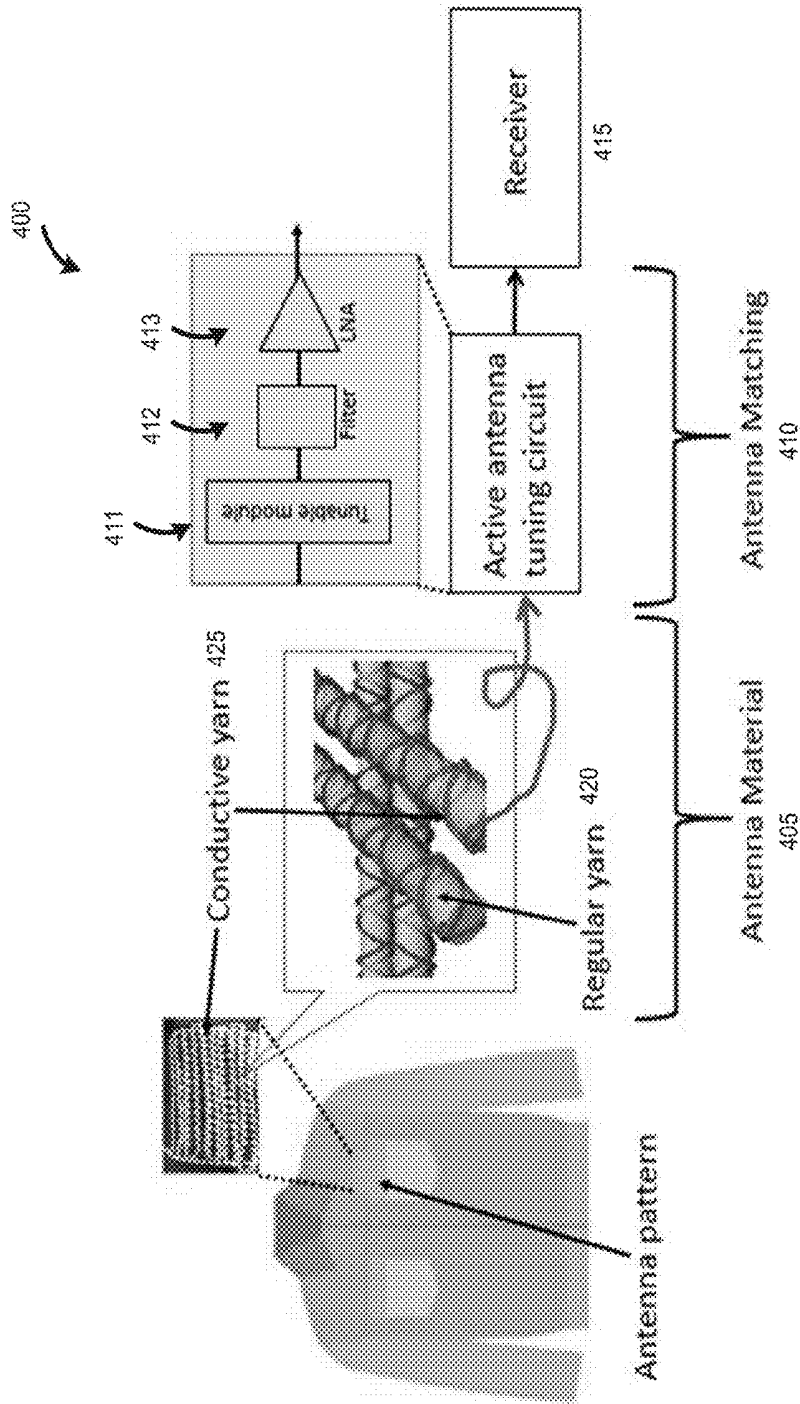


FIG. 4

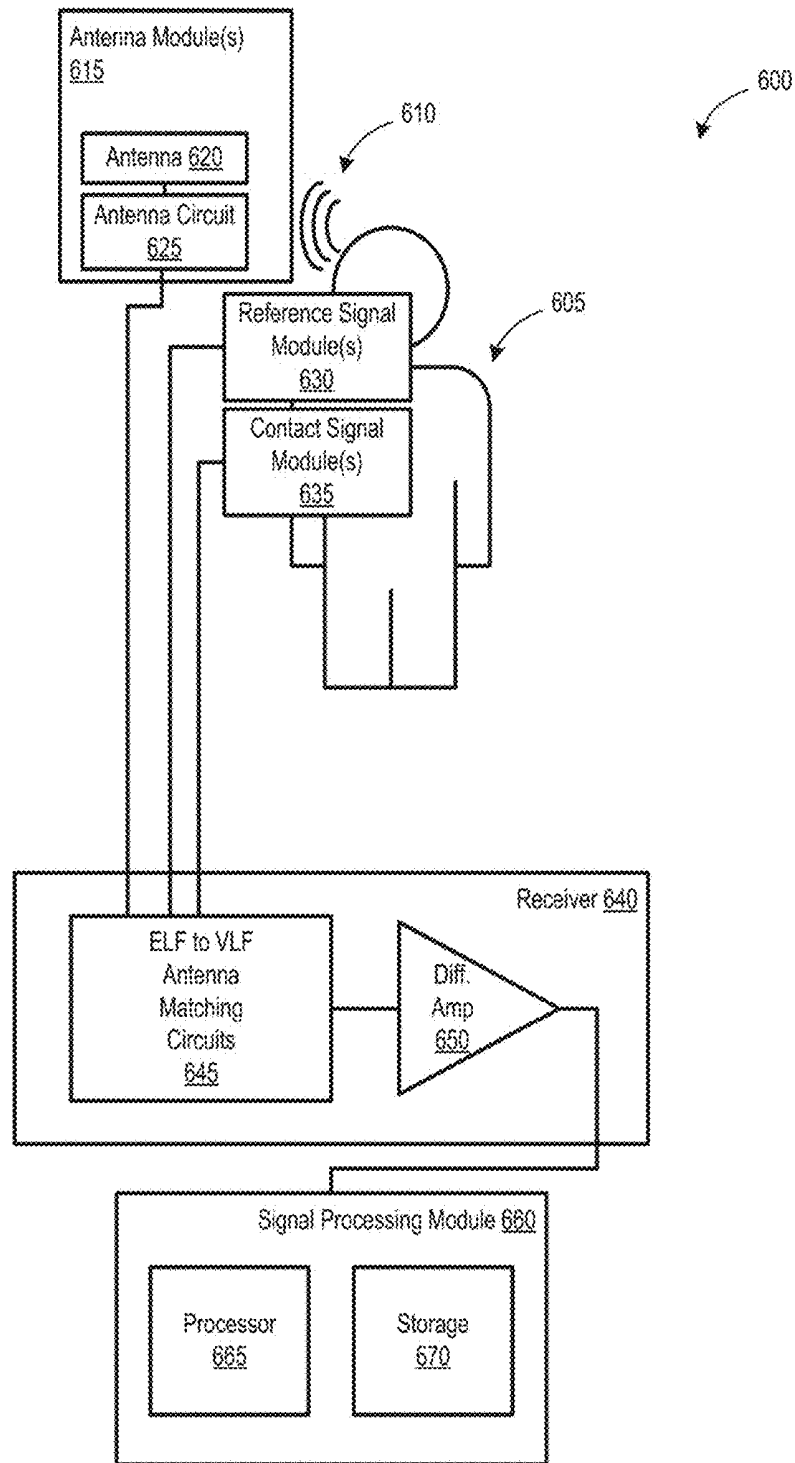


FIG. 6

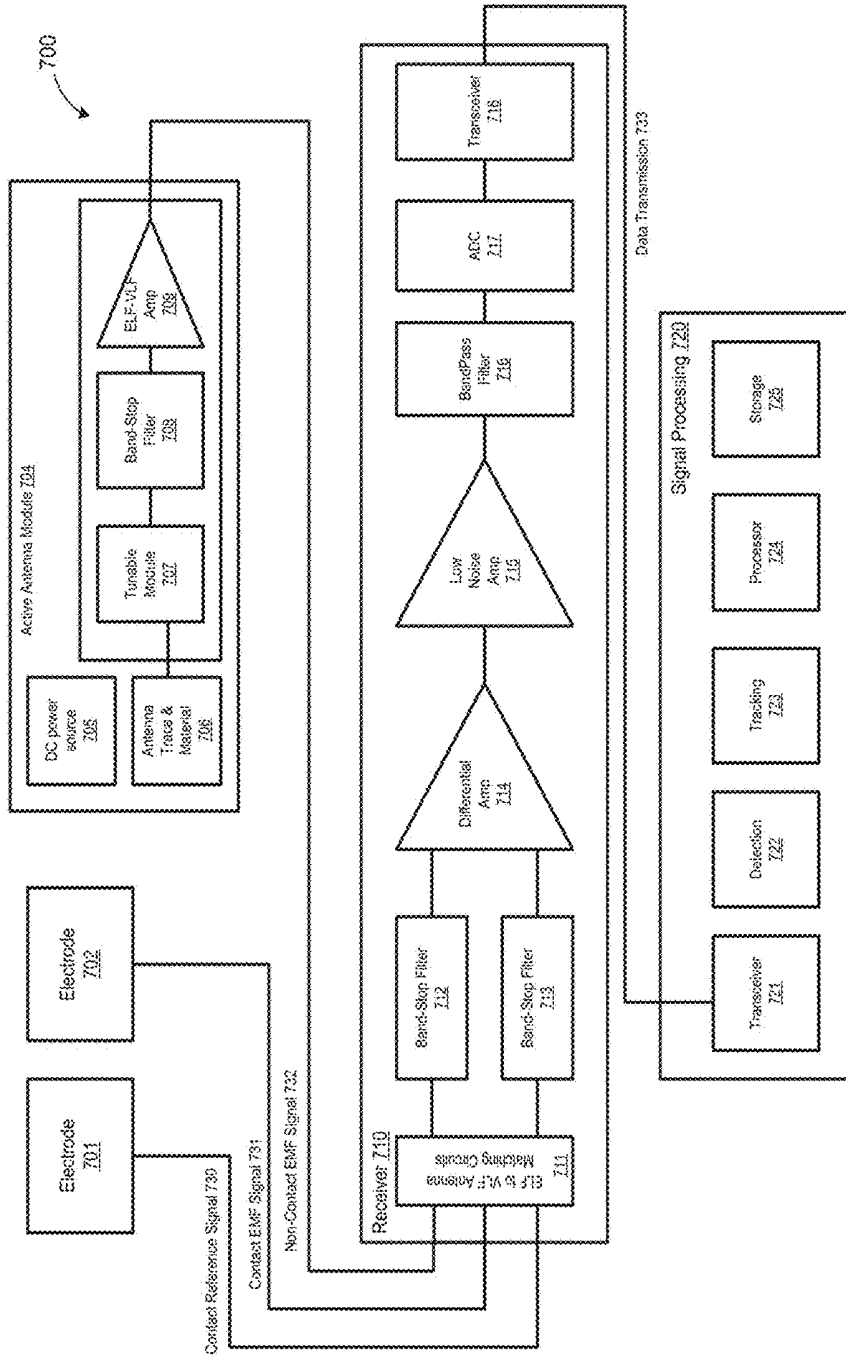


FIG. 7

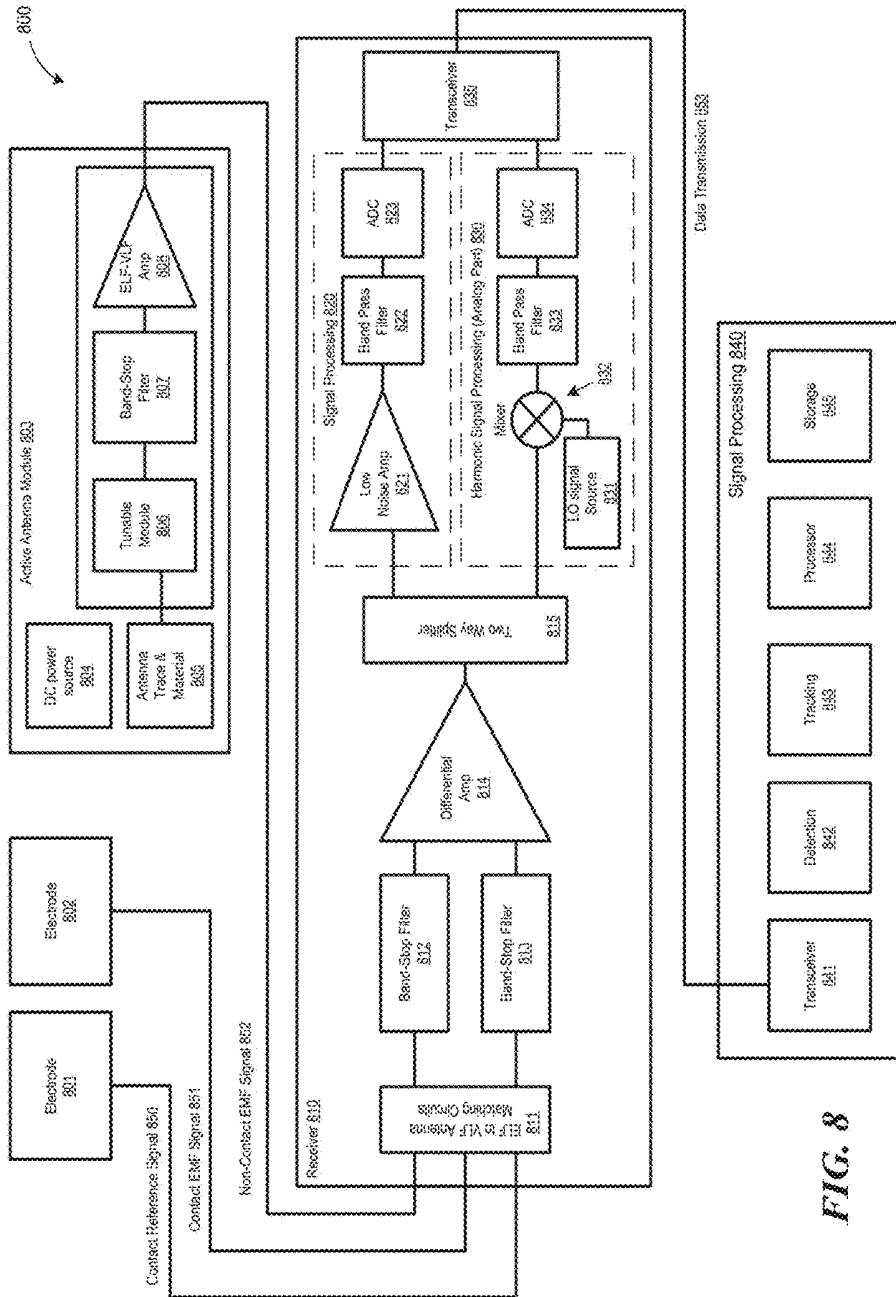


FIG. 8

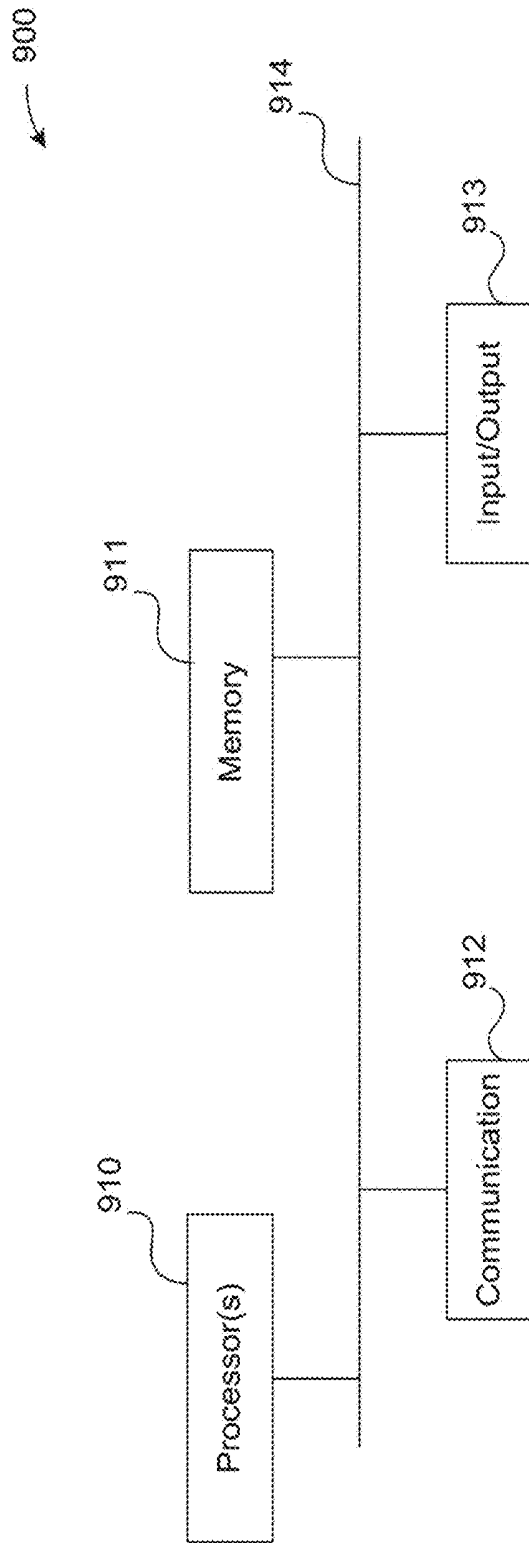


FIG. 9

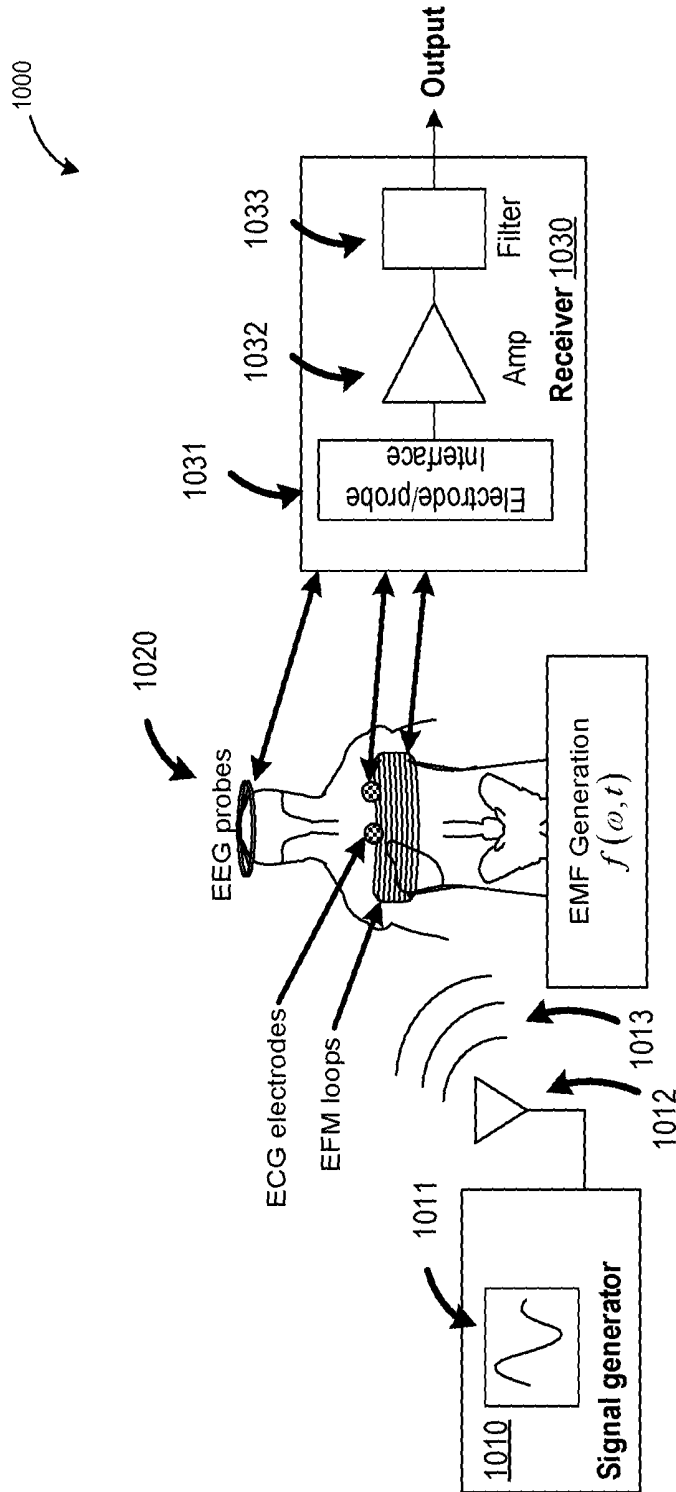


FIG. 10

HYBRID ELECTROMAGNETIC FIELD SIGNAL DETECTION SYSTEM FOR HUMAN BIOELECTRICAL SIGNAL MONITORING

CROSS REFERENCE TO RELATED APPLICATIONS

This application claims priority to U.S. Provisional Patent Application Ser. No. 62/482,123, filed on Apr. 5, 2017, the entire contents of which are hereby incorporated by reference.

GOVERNMENT LICENSE RIGHTS

Some embodiments of the invention were made with government support under W81XWH-17-C-0133 awarded by the U.S. Army Medical Research and Materiel Command. The government has certain rights in the invention.

TECHNICAL FIELD

The present disclosure is directed generally to electromagnetic field detection and monitoring system, and more specifically, to monitor a soldier or field operator's health condition based on electromagnetics field (EMF) signals emitted from the human body.

BACKGROUND

In a dynamic, fast changing environment, and especially a hostile one such as a warzone, it is preferable to be able to accurately, timely, and reliably monitor the health condition of a field operator.

The EMF signals from the human body are emitted at two extreme ends of the electromagnetic spectrum. The two extremes correspond to very low (e.g., KHz to Hz range) and very high (e.g., equal or higher than THz) frequencies on the electromagnetic spectrum. In order to detect bioelectrical signals from the human body, infrared radiation (e.g., THz range) may be projected on, and electrodes attached to, the skin for obtaining electroencephalogram (EEG) or electrocardiography (ECG) signals.

There are technical difficulties in implementing a health monitoring system that is based on monitoring these electromagnetic signals of two extreme ends and nevertheless suitable for said dynamic, fast changing environment.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a diagram of a passive detection environment in accordance with one or more embodiments of the present disclosure.

FIG. 2 is a diagram of an active detection environment in accordance with one or more embodiments of the present disclosure.

FIG. 3 depicts a diagram of an antenna system in accordance with one or more embodiments of the present disclosure.

FIG. 4 depicts an antenna signal path in accordance with one or more embodiments of the present disclosure.

FIG. 5 depicts a circuit diagram of antenna circuit in accordance with one or more embodiments of the present disclosure.

FIG. 6 depicts a block diagram of an EMF signal path in accordance with one or more embodiments of the present disclosure.

FIG. 7 depicts a block diagram of an EMF signal path in accordance with one or more embodiments of the present disclosure.

FIG. 8 depicts a block diagram of an EMF signal path in accordance with one or more embodiments of the present disclosure.

FIG. 9 is a high-level block diagram illustrating an example of a processing system in which at least some operations described herein can be implemented, consistent with various embodiments.

FIG. 10 is an active detection environment in accordance with one or more embodiments of the present disclosure.

FIG. 11 depicts a chart of contact points in accordance with one or more embodiments of the present disclosure.

DETAILED DESCRIPTION

In order to achieve the goal of detecting the physical conditions of a human body in a fast changing and dynamic environment, such as a warzone, there are a number of technical hurdles. First, the wearable antennas should be thin, lightweight, low maintenance, robust, inexpensive and easily integrated in sensing circuits. Second, the system should be able to detect a frequency range between the extremely low frequency (ELF) band to the very low frequency (VLF) band. ELF is defined by the International Telecommunication Union (ITU) as electromagnetic radio waves with frequencies from 3 to 30 Hz. VLF is defined by the International Telecommunication Union (ITU) as electromagnetic radio waves with frequencies from 3 kHz to 30 kHz. Third, system must be able to exclude uncertainty from weak EMF signals. Fourth, the detected EMF signals must be processed to obtain bioelectrical signals that are useful for health monitoring and medical diagnostics. Last but not least, the detection system needs to be non-intrusive so as not to adversely affect the subject's performance, and yet maintains an acceptable level of accuracy. There are additional challenges for the selection of textile materials, circuit assembly, manufacturing, and performance reliability.

Traditional EMF signal detection utilizes contact-based electrodes. The electrode can be a tiny patch that connects to the patient for sensing bioelectric potential. This electrical activity can be viewed as a small electric field or flux of charge-carrying particles (i.e., current). The electrodes work as transducers that convert the current flow from the body into the electron flow of the metallic wire. Often a high ionic concentration gel is used in the skin-electrode interface to increase conductivity due to small signal magnitude.

However, such an implementation faces several disadvantages. For example, one disadvantage is the time and effort necessary to create an initial contact between the electrode and the skin. Another disadvantage is that the connection between the electrode and the skin may deteriorate over time. This may occur when the high ionic concentration gel dries over time. This may also occur if the electrode is pulled away from the skin. When the contact deteriorates, the quality of the signal falls drastically. This concern is especially important in a fast changing and dynamic environment, such as a warzone where the electrode's contact to the patient's skin deteriorates rapidly. Additionally, the electrode may impede movement of the subject resulting in undesirable and dangerous loss of performance in the environment.

There have been implementations that attempt contactless EMF detection by using traditional electrodes and operates by capacitive coupling. In other words, the electrode that operates by capacitive coupling treats the gap

between the electrode and the skin as a large capacitor. Such a model has the drawback that the coupling capacitance decreases rapidly as the distance between the electrode and the skin increases. Therefore, the electrode may only operate in a limited distance from the skin. Also, it is difficult to discern the locations of the signal sources in such implementation. These limitations make this model not suitable for EMF detection in a fast changing and dynamic environment.

Traditionally, only contact-based electrodes have been used for bioelectrical signal detection because there are several challenges to non-contact EMF detection. Antenna-based EEG/ECG signal detection occurs at a distance from the skin that is greater than the distance between a contact-based electrode and the skin. The antenna frequency is very low (10 Hz to 10 KHz) and thus its wavelength is long (e.g., the wavelength of a 5 KHz signal is about 60,000 meters and the wavelength of a 10 Hz signal is about 30,000,000 meters). Additionally, the minimum required electrical wavelength for the traditional antenna is 0.1 wavelength to guarantee an efficient radiation efficiency. Therefore, antenna-based EEG/ECG has not been implemented because the large size of the antenna would be cumbersome and dangerous in a fast changing and dynamic environment.

Accordingly, introduced here is a technique to measure and track EMF signals, which is based on a new concept of detecting both contact and non-contact EMF signals. Additionally, signal processing can be performed by one or more embodiments for signature extraction and for rejecting interference from EMF signals. More specifically, the embodiments disclosed here can use a single or multiple EMF sensors that can be placed at various strategic locations, where the locations can enable the sensors to detect valuable signs of trauma and forecast physical conditions impacting the human's ability to operate missions in the field or during training process. The placement of such sensors can be part of an electro-textile combat and operations uniform. Some embodiments provide a body worn system equipped with sensing, processing, communications, and storage capabilities. The concept of the disclosed sensing system is to have wearable antennas capable of transferring the EMF energy in its electrical or magnetic forms into the sensors. The EMF energy is then processed to obtain bioelectrical signals indicating the physical conditions of the monitored human body.

EMF can be acquired from self-emission (i.e., passive detection) and reflection (i.e., active detection) from the human body. EMF self-emission is a function of numerous components. For example, random or pseudo noise can be induced by human muscle activities, minor currents near brain or heart, and body static excitations. Electromagnetic (EM) reflection is induced by the incoming EM energy from an external EM source coupling to the human body then the re-emission is excited. Both self and reflected EMF can be measured using electrical probes, magnetic loops, and antenna systems with good receiver sensitivity at the low end of the EM spectrum. Between two extremes of EM spectrum, these signals are usually very weak due to no-higher-frequency human energy emission (e.g., muscle pulse). Additionally, most of the non-linear effects in higher frequency are happening very short in time and narrow in its dynamic range in terms of amplitude.

Passive measurements may play a critical role in defining the state of the biological system. Active measurements on dead systems or selected organic chemical solutions along with passive intermodulation measurements and signal processing is used to further define the biological system in

detail. ECG/EEG signals vary from the microvolt to the millivolt range and are the relatively stronger signal in human tissue. Due to this small voltage, the signals measured need to be amplified for better access.

In accordance with some embodiments, biopotential amplifiers may have high input impedance and are designed for safety, since excessive induced current may produce a significant shock to the living organism. Isolation and protection circuitry limit the any currents through the electrodes to safe levels. For proper interface to outside circuits, the output impedance of the amplifier desirably should be very low, allowing to drive any external loads with a minimal distortion. The amplifiers desirably should have a high rejection ratio (e.g., in differential mode) to eliminate large offset signals. Generally speaking, a rejection ratio of 30 db (i.e., 1000 times) may be considered "high." One of the most factors of EMF detection is the noise level, or noise floor, which is highest at lower frequencies. Therefore, according to one or more embodiments, biopotential amplifiers are differential which can minimize noise from the ground.

Further, in some embodiments, the EMF detection system can perform active harmonic signal calibration in order to understand and calibrate the intermodulation from the mixer, cables, signal generators, and digitizer. In particular, the system can perform a two-tone measurement around the frequency range of the interested signals and, in some implementations, up to the 7th order of its harmonics. For example, the test starts with two-tone signals feeding into the RF mixer in its working frequency range. The frequency mixer may have a low-frequency local oscillator (LO) signal, which may be as low as 500 Hz, in some examples. The system can also feed two tones above 500 Hz and can, for example, sweep the LO with a 100-Hz step frequency from 5 kHz to 5.5 kHz and keep the input signal at 1000 Hz.

The EMF detection system can also perform vital signal generation by waveform generator and active measurement. In some examples, the system generates a body signal (e.g., an ECG signal) and then measures the detected signal. In order to differentiate a normal ECG signal and arrhythmias signal, the system generates three different ECGs. One is a normal ECG signal, and the other two are arrhythmias (e.g., tachycardia and bradycardia). Each signal contains different features in both the time and frequency domain (e.g., such as the bandwidth changes). For example, tachycardia has a wider bandwidth than the normal ECG, and bradycardia has a narrower bandwidth than the normal one.

Finally, the EMF detection system can perform ECG signal detection at different locations of the body. At each measurement point, ECG may be recorded for 10 seconds at the sampling rate of 1000 samples/second. A low pass filter is applied to clean the signal. Both the original ECG signal and filtered signal may be plotted together for comparison. Additionally, the FFT spectrum of each original ECG signal may be used to analyze the results. Depending on the implementation, the system can also measure vital signals measured at different body positions. It is observed that ECG signal typically still dominates the vital signal detection, but other types of vital signal from the frequency domain, such as a 20 Hz signal around the stomach. This 20 Hz vital signal may be generated from stomach or intestine activities.

As described in further detail below, the disclosed embodiments here can further include a hybrid sensor system and signal processing to capture the EMF effects and track the EMF signatures in time and time-frequency domains. Notably, the disclosed system design makes the EMF tractable and repeatable.

In the following, numerous specific details are set forth to provide a thorough understanding of the presently disclosed technology. In other embodiments, the techniques introduced here can be practiced without these specific details. In other instances, well-known features, such as specific fabrication techniques, are not described in detail in order to avoid unnecessarily obscuring the present disclosure. References in this description to “an embodiment,” “one embodiment,” or the like, mean that a particular feature, structure, material, or characteristic being described is included in at least one embodiment of the present disclosure. Thus, the appearances of such phrases in this specification do not necessarily all refer to the same embodiment. On the other hand, such references are not necessarily mutually exclusive either. Furthermore, the particular features, structures, materials, or characteristics can be combined in any suitable manner in one or more embodiments. Also, it is to be understood that the various embodiments shown in the figures are merely illustrative representations and are not necessarily drawn to scale.

Several details describing structures or processes that are well-known and often associated with EMF detection and corresponding systems and subsystems, but that can unnecessarily obscure some significant aspects of the disclosed techniques, are not set forth in the following description for purposes of clarity. Moreover, although the following disclosure sets forth several embodiments of different aspects of the present disclosure, several other embodiments can have different configurations or different components than those described in this section. Accordingly, the introduced techniques can have other embodiments with additional elements or without several of the elements described below.

Many embodiments of the present disclosure described below can take the form of computer- or controller-executable instructions, including routines executed by a programmable computer or controller. Those skilled in the relevant art will appreciate that the introduced techniques can be practiced on computer or controller systems other than those shown and described below. The techniques introduced herein can be embodied in a special-purpose computer or data processor that is specifically programmed, configured or constructed to perform one or more of the computer-executable instructions described below. Accordingly, the terms “computer” and “controller” as generally used herein refer to any data processor and can include Internet appliances and handheld devices (including palm-top computers, wearable computers, cellular or mobile phones, multi-processor systems, processor-based or programmable consumer electronics, network computers, mini computers and the like). Information handled by these computers and controllers can be presented at any suitable display medium, including a liquid crystal display (LCD). Instructions for performing computer- or controller-executable tasks can be stored in or on any suitable computer-readable medium, including hardware, firmware or a combination of hardware and firmware. Instructions can be contained in any suitable memory device, including, for example, a flash drive, USB device, and/or other suitable medium.

The terms “coupled” and “connected,” along with their derivatives, can be used herein to describe structural relationships between components. It should be understood that these terms are not intended as synonyms for each other. Rather, in particular embodiments, “connected” can be used to indicate that two or more elements are in direct contact with each other. Unless otherwise made apparent in the context, the term “coupled” can be used to indicate that two or more elements are in either direct or indirect (with other

intervening elements between them) contact with each other, or that the two or more elements co-operate or interact with each other (e.g., as in a cause and effect relationship), or both.

5 Passive Detection Configuration

FIG. 1 is a diagram of a passive detection environment **100** for receiving EMF signals to obtain bioelectrical signals, according to some embodiments. The environment **100** can perform passive detection using an EMF sensor system to obtain bioelectrical signals such as EEG and ECG signals. The environment **100** includes a body **105** that emits EMF signals **100**. The EMF signals **100** can be detected by the passive detection system **115**. The passive detection system **115** includes an antenna **120** and an amplifier **125**.

The antenna **120** can be a radio-frequency (RF) antenna or magnetic probe placed close to the human body. The placement may be determined by defined locations that maximize detection of EMF signals associated with various parts of the body, e.g., head, upper torso, and/or wrist. The body **105** emits EMF signals **110** that can be received by the antenna **120** of a passive detection system **115**.

The received signal is then passed to amplifier **125** where the gain of the received signal is increased for further signal processing. For example, the signal detected by antenna may be amplified by a low noise amplifier (LNA). With proper frequency down-conversion, the signal can be observed and recorded for analysis.

Active Detection Configuration

FIG. 2 is a diagram of an active detection environment **200**, in accordance with some embodiments. The active detection environment **200** can utilize RF antennas to send custom or arbitrary RF waveforms and receive EMF signals from the body. Arbitrary signal generation is used to generate RF harmonic signals to propagate through the human body from RF antennas. For example, arbitrary signal generation can generate different waveforms from mathematical modeling along with different amplitudes, bandwidths, and frequencies. The environment **200** includes a human **205**, an active detection transmission module **210**, and an active detection reception module **235**.

The active detection transmission module **210** may be used to reflect or excite EMF signals from the human body when a wideband or narrowband external transmission source is placed near the human body. For example, a very wideband transmission may include signals from DC to 10 KHz. A narrowband transmission may be a single tone (e.g., 100 MHz). The active detection transmission module **210** includes a signal generator **215**, amplifier **220**, and transmission antenna **225**. The signal generator **215** generates an EMF signal **230** near body **205**. For example, the signal generator **215** is used to send a single tone (e.g., 100 MHz) signal to a VHF antenna.

The generated signal is amplified by amplifier **220** and transmitted using antenna **225**. In some embodiments, more than one antenna may be used to transmit RF signals. Additionally, the antennas may be placed around the human body. For example, antennas may be placed around the head, heart, chest, and abdomen. The custom magnetic and RF antennas are designed for high efficiency and compensate for body impedance at desired frequency bands.

The active detection reception module **235** receives the EMF signals transmitted by the active detection transmission module **210** and reflected or excited by body **205**. The active detection reception module **235** includes antenna **240** and amplifier **245**. The antenna **240** may be a radio-frequency (RF) antenna or magnetic probe placed close to the human body. The placement may be determined by defined

locations that maximize detection of EMF signals associated with various parts of the body. The body **205** reflects EMF signals **230** that are received by antenna **240** of active detection reception module **235**.

The received signal is then passed to amplifier **245** where the gain of the received signal is increased for further signal processing. For example, the signal detected by antenna may be amplified by a low noise amplifier (LNA). With proper frequency down-conversion, the signal can be observed and recorded for analysis

Active detection using an active source enhances the weak signal signature by using a carrier signal. The transmitted carrier signal has stronger amplitude and a controlled frequency. In this setting, the introduced embodiments may use a mixer such that the human body behaves like a non-linear channel, which can generate harmonics signals when a single tone signal passes through the human body channel. The signal may be mixed with other environmental signals that enter the human body (e.g., WiFi, 4G, VHF, and/or other RF signals) or another designed test tone signal. The product of this mixing is called intermodulation (IMD) tones, which, in some cases, fall in different receive bands of the communication system.

The weak EMF signals coupled with stronger harmonic signals become new modulation signals with detectable power levels seen by a receiver. The new modulation signals include high-order intermodulated signals, including the input tones, third-order products, and high-order products. They have lower amplitudes from the carrier tones but still have a 20-dB dynamic range referring to the carrier signal amplitude level. The modulated EMF signal can be detected by the receiver and put into the demodulation process by using signal processing algorithm.

Note, however, that an active detection configuration with transmitted carrier signal may be less desirable, as compared to a passive detection configuration, in an environment where unnecessary EMF emission should be avoided (e.g., in a hostile, combative environment).

Hybrid Antenna System

Embodiments of the disclosed antenna system can detect EMF signals with different frequency ranges. Additionally, the antenna can be designed in a loop, monopole, dipole, or wire antenna placed in a certain distance from the human body. In some embodiments, the antenna may be an array or grid structure to scan the human body. In yet other embodiments, the antenna may be conformal or wearable structure embedded with textile.

The antenna system can be integrated into a body suit without inhibiting the movement of the user. The bandwidth of probe antenna and RF components are typically narrowband. Therefore, to detect and observe the whole spectrum of triggered or induced signals, very wideband components are needed. For example, very wideband components can support EMF signals from DC to 10 KHz. Contact based electrodes attach directly to the body surface. However, to use a probe antenna integrated with a textile worn by the human body, there is a gap between the sensor and the body. Therefore, non-contact antenna is provided to detect EMF signals without degradation of bio-signals.

For purposes of the present disclosure, an EMF antenna system that includes at least a contact input source (e.g., an electrode) and a non-contact input source (e.g., an antenna) may be referred to herein as a "hybrid" antenna system.

FIG. 3 depicts a diagram of a hybrid antenna system **300** worn on the head **305** of a user to monitor the EMF signals of the user.

Hybrid antenna system **300** may use the mechanisms of EMF generation linked to the muscle electro-impulse response and energy conversions from body electrochemistry effects. The hybrid antenna system **300** uses both contact electrodes and non-contact antennas (i.e., a hybrid approach) to detect vital EMF signals. The non-contact antennas use active circuits to detect signals at such low frequencies. Hybrid antenna system **300** also detects common ground and reference signals, which are critical since they are the reference signals used to cancel the commonly seen noise (e.g., powerline noise, such as 60 Hz).

The example antenna system **300** includes a ground contact **315**, an ear reference module **320**, a contact electrode **325**, non-contact antennas **330a** and **330b**, and a Bluetooth™ module **335**. The entire system may be worn over the head which may include hair **310**, where contact electrode placement is not suitable.

The ground contact **315** provides a return path for the signals detected by antenna system **300**. The ear reference module **320** is a contact-based electrode for receiving EMF signals emitted from head **305**. For example, ear reference module **320** uses traditional electrodes to connect to the skin to detect reference signals. The contact electrode **325** is also a contact-based electrode for receiving EMF signals emitted from head **305**. For example, ear reference module **320** uses traditional electrodes to connect to the skin to detect EEG/ECG signals.

Many of contact-based biomonitoring electrodes of ECG and EEG are comprised of a plastic substrate covered with an Ag/AgCl compound. The electrode can be assembled with an electrolyte gel since the skin interface may contain an excess of chloride ions in solution such as perspiration. Such combination can be done by coating those compounds on the plastic substrate (i.e., stud). The gel is also used on the skin of patients when checking their ECG. However, the gel may dry out or only can last a few hours or days after placed on the patient. The conductive carbon fiber, or other conductive materials, should be qualified to replace current compound and metal materials used in current electrodes or new probes. The probe-to-skin impedance and its dimension will be decided by contact area, skin properties, and the materials used.

The electrode used in ECG detection can be a tiny patch which connects to the patient. ECG electrodes are used for sensing bioelectric potential, generally the electrical activity, caused by cardiac muscle. This electrical activity can be viewed as a small electric field or flux of charge-carrying particles (i.e., current). The electrodes work as transducers converting this current flow from the body into the electron flow of the metallic wire. After amplified and processed, the ECG signal can be observed. Very often a high ionic concentration gel is used in the skin-electrode interface to increase conductivity due to small signal magnitude. The electrode may be a silver-silver chloride electrode.

In some embodiments, the electrode module includes a plastic substrate covered with an Ag/AgCl compound, an electrolyte gel coated on the plastic substrate to provide a high ionic concentration, and a conductive material to detect EMF signals when the electrode module is in contact with a human surface. In some embodiments, an electrode module includes two pre-gel (i.e., prior to gel being applied) electrodes placed on the head of a human body to detect the vital signs of the human body.

In some embodiments, the electrode may be placed in contact with the ear to detect a reference signal. The ear is a suitable location to detect EMF signals from the body because it has relatively less noise. This is because the ear

does not have any muscles and thus would not introduce EMF signals resulting from the muscle. However, other nodes can be used as needed.

The non-contact antennas **330a** and **330b** detect EMF signals without requiring direct contact to the human body. The non-contact antennas **330a** and **330b** use low frequency antennas, from extreme low frequency (ELF) to very low frequency (VLF), to collect the bioelectrical signals such as EEG/ECG signals. The antenna does not need to contact the skin directly. Thus, the antenna performs EEG/ECG signal detection at a distance from the skin that is greater than the distance between a contact-based electrode and the skin. The antenna frequency is very low (10 Hz to 10 KHz) and thus its wavelength is long (e.g., the wavelength of a 5 KHz signal is about 60,000 meters and the wavelength of a 10 Hz signal is about 30,000,000 meters). Additionally, the minimum required electrical wavelength for the traditional antenna is 0.1 wavelength to guarantee an efficient radiation efficiency.

The Bluetooth module **335** can be provided to transmit and receive data related to the signals detected by the ear reference module **320**, contact electrode **325**, and non-contact antennas **330a** and **330b**. For example, the Bluetooth module **335** may transmit the detected signals to a signal processing module for signal processing, analysis, and data storage.

The various components of the antenna system **300** can be implemented in a manner that is consistent with the various embodiments described herein.

Antenna Signal Path

FIG. 4 depicts an antenna signal path **400** that includes antenna material **405**, an antenna matching circuits **410**, and a receiver **415**. The signal path **400** represents the path of the EMF signal originating from a monitored body to an amplified for signal processing.

Antenna Material

Antenna material **405** includes a conductive material that receives EMF signals from a monitored human body. In some embodiments, the antenna is an electro-textile based antenna including non-conductive, interlacing fibers **420** and conductive yarn **425**. In some embodiments, the flexible antenna patch is embedded in a flexible substrate. For example, non-conductive, interlacing fibers **420** may form a flexible antenna patch integrated into clothing worn by the monitored human body. The conductive yarn **425** may be wound around individual fibers of the non-conductive interlacing fibers **420**, such that the non-conductive fiber **425** and conductive fiber **425** form a textile patch for receiving EMF signals from a human body without contact with the human body.

Antenna material **405** may use a variety of elements or materials. In some embodiments, silver ink and copper wires are good conductors but they are less suitable to be implemented on or be part of fabric for clothing. Conductive fiber materials (e.g., electro-textile) may be used as conductive yarn so that the antenna radiator pattern can be built with the clothes in a weaving process. In some embodiments, the antenna material **405** may be a meshed antenna using conductive fiber was made by a very fine conductive silver thread (e.g., Agsis Silver AGSIS100D-1KAG).

Conductive thread is suitable since it can be used to modify existing clothing. Silver is ideal since silver oxide is highly conductive possesses excellent RF properties. Additionally, the cost of silver is significantly less than alternative conductive material such as gold.

Antenna material **405** may be used in a variety of shapes. For example, a planar antenna can be integrated with a

conformal patch that fits in existing clothing. This conformal structure may cause additional resonances which may be generally undesirable. However, this property is good in this application because a wider bandwidth is desired. In some embodiments, to fit the property of the textile material, a meshed texture antenna can be used to replace the conventional patch antenna with a solid surface. Additionally, antenna material **405** may use flexible PCB materials to fabricate the meshed antenna.

In some embodiments, the antenna material **405** may be formed as a non-uniform meshed path antenna. Non-uniform meshed patch antennas have significantly less conductor coverage than a conventional meshed patch antenna. Less conductor coverage reduces the usage of the specialized conductive fiber materials, which in turn can reduce the cost of the antenna material.

Active Antenna Circuits

The antenna system uses two ways to reduce the electrical wavelength. First, the antenna system changes the transmission line materials to increase the effective electrical length. Second, the antenna system connects the shortened antenna with active antenna circuits. With the above two factors, the physical length can be greatly reduced to use a shorter antenna length to receive the vital signal from the human body. Additionally, while the environment is changing, such as when the user is in motion, the antenna system may become detuned and mismatched to the RF circuit front-end. The resulting signal loss may be significant in specific frequency ranges. Furthermore, when there is gap or other media between the body and the antenna, additional loss will result in lower signal to be received. To mitigate this impact, the active antenna circuits actively compensate for the changing conditions using the components described below.

Antenna circuits **410** includes electronic circuits that can obtain the signals received by antenna material **405** and process the signals so that they are suitable for further signal processing (e.g., at a subsequent stage, such as at the receiver module and/or the signal processing module). Antenna circuits **410** may include tunable module **411**, filter **412**, and amplifier **413**.

Tunable module **411** facilitates wideband tuning and signal amplification. and may be implemented with tunable capacitors. Wideband tuning may facilitate reception of signals at frequencies between and including the ELF and VLF frequency bands. In some embodiments, the tunable capacitors extend the bandwidth of the antenna to include the ELF frequency band and the VLF frequency band. Filter **412** may be a band-pass or band-rejection filter that passes the input signal in most frequencies but filters signals in specific frequency bands. For example, filter **412** may pass the detected EMF signal but attenuate one or more predetermined frequencies (or frequency range(s)) for background noise suppression. Commonly seen background EMF noise can include those signals in the 60 Hz frequency band, which are typically introduced by the powerline power supply. Amplifier **413** increases the power of the signal output of filter **412**. For example, amplifier **413** may amplify low frequency signals with frequencies from 5 Hz-1 KHz. Receiver

Receiver **415** can include impedance matching modules, differential amplifiers, and filters for processing the received EMF signals from the antenna system. For example, the impedance matching module maximizes the power transfer of the received signal by matching the source load of the antenna system.

The differential amplifier enhances the gain of the received signal based upon the received reference signal.

The non-contact signal and contact signal enter the instrument amplifier such as differential amplifiers. Since the amplitude from the non-contact node is amplified to a similar level of the contact node (e.g., the reference signal), the noise and interference cancellation can be performed inside the differential amplifier circuits. The filters reduce noise such as powerline noise (e.g., noise at 60 Hz).

The various components of the antenna signal patch **400** can be implemented in a manner that is consistent with the various embodiments described herein.

Antenna Circuit Embodiment

FIG. 5 depicts a circuit diagram of antenna circuit **500** consistent with various embodiments disclosed herein. The active antenna circuit **500** includes various circuit components that may be adjusted to perform antenna matching, wideband tuning, and signal amplification. Antenna circuit **500** shown in FIG. 5 may be an embodiment of circuit **410** described above. For example, tuning circuit **510** is an embodiment of tuning circuit **411**, filter circuit **520** is an embodiment of filter **412**, and voltage amplifier **530** and emitter-follower amplifier **540** is an embodiment of amplifier **413**. An active antenna circuit is distinguished from a passive antenna because the circuits utilize an external power source (e.g. DC power source **804**) to power an amplifier. Additionally, the antenna circuit **500** may use bipolar junction transistors (BJT) transistors with lump elements to perform the antenna matching.

Since the body signal typically has a weak signal strength, the received signal must be amplified and filtered before the signal processing can be applied. The RF path is the first opportunity to moderate the loss and noise. For example, a high efficiency antenna and differential amplifiers may be used to maintain gain, reduce noise, and increase the chance to detect weak bioelectrical signals.

Instead of using discrete components, the antenna tuner can be a highly integrated module consisted of several switches and tunable capacitors for more flexible tuning. The bipolar junction transistor (BJT) or field emitter transistor (FET) based active circuit is used to enhance the gain and filtering. Additionally, the bandwidth of the antenna is extended while minimizing the reduction in antenna efficiency.

The various components of active antenna circuit **500** can be implemented in a manner that is consistent with the various embodiments described herein.

EMF Signal Path

FIG. 6 depicts a block diagram of an EMF signal path **600** consistent with various embodiments disclosed herein. EMF signal path **600** is a signal path starting from the EMF signals **610** emitted from human body **605**. The signals are detected by an antenna module **615**, a reference signal module **630**, and a contact signal module **635**. The detected signals then proceed along the EMF signal path **600** to a receiver **640** and a signal processing module **650**.

Antenna signal module **615** includes an antenna **620** and an antenna circuit module **625**. According to one or more embodiments, the antenna **620** detects a non-contact EMF signal, and the antenna circuit module **625** performs wideband tuning and amplifies the non-contact EMF signal. For example, wideband tuning may facilitate reception of signals at frequencies between and including the ELF and VLF frequency bands.

Reference signal module **630** includes an electrode to detect a reference signal from the human body **605**. For example, the electrode may be a contact-based electrode that is placed on the ear of the human body **605**. The contact signal module **635** includes an electrode to detect an EMF

signal from the human body **605**. For example, the electrode may be a contact-based electrode placed on various parts of the human body **635** to detect localized EMF signals.

Receiver module **640**, in some implementations, includes an impedance matching module **645** and differential amplifier **650**. Impedance matching module **645** improves the power transfer of the EMF signals by matching the source impedance of the antenna module. Differential amplifier **650** generates bioelectrical signals including a contact bioelectrical signal by amplifying the contact EMF signal and a non-contact EMF signals

Signal processing module **650**, in some implementations, includes processor **665** and storage **670**. Processor **665** applies a filtering algorithm to improve the signal-to-noise ratio of the bioelectrical EMF signals and to perform digital signal processing on the bioelectrical EMF signals. Storage **670** provides data storage to maintain data regarding the detected EMF signals. The stored data may be used to perform further signal processing in the future. For example, signals may be stored until enough signal data is gathered to perform comparison or correlation related analysis.

The various components of the EMF signal path **600** can be implemented in a manner that is consistent with the various embodiments described herein.

EMF Detection System

FIG. 7 depicts a block diagram of an EMF detection system **700** consistent with various embodiments disclosed herein. EMF detection system **700** includes an electrode **701**, an electrode **702**, an active antenna module **705**, a receiver **710**, and a signal processing module **720**.

Electrode **701** may include a contact-based electrode to detect a reference signal **730** from a human body. In some embodiments, the electrode may be a contact-based electrode that is placed on the ear of the human body. The ear is a suitable contact point for the electrode because it does not contain muscle tissue which emits EMF signals. Thus, the detected signal includes the desired EMF signals indicating the physical condition of the monitored body and contains less noise that interferes with the desired signal. In other embodiments, electrode **701** may be placed on the neck or other locations that allow direct contact with the skin of the body. Electrode **701** outputs contact reference signal **730**, which is based on the detected reference signal. For example, electrode **701** outputs reference signal **730** to receiver **710** to prepare the signal for signal processing.

Electrode **702** may include an electrode to detect an EMF signal from a human body. For example, the electrode may be a contact-based electrode that is placed on the head of the human body to measure EEG signals. The contact-based electrode is placed in direct contact with skin in order to detect the EEG signals such as on the forehead or neck. The placement of the contact-based electrode should avoid hair because hair does not conduct current and thus does not transmit EMF signals. More than one contact-based electrode may be placed on the head to collect more than one EMF signals from the human body. For example, the contact-based electrode may be placed on various parts of the head to detect localized EEG signals. This is important because EEG activity in different parts of the brain may indicate distinguishable physical conditions or brain activities. Electrode **702** outputs contact EMF signal **731**. For example, electrode **702** outputs contact signal **731** to receiver **710** to prepare the signal for signal processing.

Active antenna module **704** includes direct current (DC) power source **705**, antenna trace and material **706**, tunable module **707**, band-stop filter **708**, and ELF-VLF Amplifier **709**. DC power source **705** provides power to operate the

antenna circuits (e.g., tunable module **707**, band-stop filter **708**, and ELF-VLF Amplifier **709**).

Antenna trace and material **706** facilitates the detection of non-contact based EMF signals. In some embodiments, antenna trace and material **706** includes a conductive material that receives EMF signals received from a monitored human body. For example, the antenna may an electro-textile based antenna forms a flexible antenna patch. In some embodiments, the conductive yarn may be wound around individual fibers of the non-conductive interlacing fibers, such that the non-conductive fiber and conductive fiber form a textile patch for receiving EMF signals from a human body without contact with the human body. The various components of the antenna signal patch **400** can be implemented in a manner that is consistent with the various embodiments described herein, such as those described at FIG. 4.

Tunable module **707** facilitates wideband tuning and signal amplification. Tunable module **707** includes tunable capacitors. In some embodiments, the tunable capacitors extend the bandwidth of the antenna to include the ELF frequency band and the VLF frequency band. Band-stop filter **708** passes the signal in most frequencies unaltered but filters signals in specific frequency bands. A band-stop filter may also be a band-rejection filter. For example, band-stop filter **708** may pass the detected EMF signal from antenna trace and material **706** but attenuates the signal in the 60 Hz frequency band. This reduces the noise introduced by the powerline power supply (e.g., DC power source **705**). ELF-VLF amplifier **709** increases the power of the signal output of band-stop filter **708**. For example, ELF-VLF amplifier **709** may amplify low frequency signals with frequencies from 5 Hz-1 KHz. As described above, ELF is defined by the ITU as electromagnetic radio waves with frequencies from 3 to 30 Hz. VLF is defined by the ITU as electromagnetic radio waves with frequencies from 3 kHz to 30 kHz. Thus, ELF-VLF amplifier **709** may amplify frequencies from 5 Hz-1 KHz in order to amplify all signals between the ELF and VLF frequency bands. Also noted above, ELF-VLF amplifier **709** is powered by DC power source **705**.

After passing the non-contact EMF signal through antenna trace and material **706**, tunable module **707**, band-stop filter **708**, and ELF-VLF Amplifier **709**, the active antenna module **704** outputs non-contact EMF signal **732** to receiver **710** to prepare the signal for signal processing.

Receiver **710** processes the detected EMF signals to prepare the signals for signal processing. To achieve this, receiver **710** includes antenna matching module **711**, band-stop filter **712**, band-stop filter **713**, differential amplifier **714**, low noise amplifier **715**, bandpass filter **716**, analog-to-digital converter (ADC) **717** and transceiver **718**.

Antenna matching module **711** ensures adequate power transfer from active antenna module **704**. This is accomplished by matching the source load of the antenna module. In some embodiments, antenna matching module includes a resistor, inductor, and capacitor connected in series to create a resistor-inductor-capacitor (RLC) circuit network that is tuned to match the source load of the antenna module.

Band-stop filter **712** takes the output of antenna matching circuit **711** corresponding to contact EMF signal **731** or non-contact EMF signal **732**. Similarly, band-stop filter **713** takes the output of antenna matching circuit **711** corresponding to contact reference signal **730**. For example, band-stop filter **712** and band-stop filter **713** may attenuate the signal in the 60 Hz frequency band to perform powerline noise rejection.

Differential amplifier **714** is an amplifier that amplifies the difference between two input voltages and attenuates the

voltage common to the two inputs. In some embodiments, differential amplifier **714** amplifies the difference between the reference signal and non-contact EMF signal to produce a non-contact bioelectrical signal and amplify the difference between the reference signal and contact EMF signal to produce a contact bioelectrical signal. In other words, a non-contact bioelectrical signal is produced by using differential amplifier **714** to amplify the difference between the non-contact EMF signal and the reference signal. Similarly, contact bioelectrical signal is produced by using differential amplifier **714** to amplify the difference between the contact EMF signal and the reference signal. Although differential amplifier **714** is depicted as a signal amplifier, differential amplifier **714** may be implemented as multiple amplifiers. Each amplifier takes as input the reference signal and a detected EMF signal. As such, bioelectrical signals are generated by amplifying the difference between a detected EMF signal and the reference signal.

Low noise amplifier **715** amplifies a low-power signal without degrading the signal-to-noise (SNR) of the signal. In some embodiments, low noise amplifier **715** amplifies the output of differential amplifier **714**. The amplified signal output is provided as input into bandpass filter **716**. Bandpass filter **716** passes frequencies within a certain range but attenuates the signal outside of the range. In some embodiments, bandpass filter **716** passes frequencies between 5 Hz-10 KHz. This range allows signals from the ELF frequency band to the VLF frequency band to pass through. The signal passed from bandpass filter **716** is provided as input into analog-to-digital converter **717**. The analog-to-digital converter **717** converts the detected EMF signals into a digital signal for digital signal processing at signal processing module **720**. The digital signal output by analog-to-digital converter **717** is provided to transceiver **718** for transmission as data transmission signal **733** to signal processing module **720**. In some embodiments, transceiver **718** may transmit data transmission signal **733** to signal processing module **720** via wireless transmissions. For example, transceiver **718** may be a Bluetooth enabled module that transmits data transmission signal **733** to signal processor **720** via Bluetooth. In other embodiments, transceiver **718** may transmit data transmission signal **733** to signal processing module **720** using a wired transmission.

Signal processing module **720** may include transceiver **721**, detection module **722**, tracking module **723**, processor **724**, and storage module **725**. Depending on the implementation, one or more modules can be added or removed to suit the purpose of a specific field application. Signal processing module **720** receives data transmission signal **733** from receiver **710**. Signal processing module **720** applies digital signal processing, signal analysis, and data storage on received data transmission **733**. Signal processing includes preliminary EMF detection and processing. Multiple measurements are performed with a variety of sampling rates and signal durations. Each measurement is analyzed using human EMF decomposition algorithm. In some frequency bands, the signals measured with or without a monitored human body show repeatable differences.

First, transceiver **721** facilitates the reception of data transmission **733**. Data transmission **733** includes the digital signals produced by receiver **710**. In particular, data transmission signal **733** may include contact and non-contact bioelectrical signals based on the contact reference signal **730**, contact EMF signal **731**, and non-contact EMF signal **732**. Once data transmission signal **733** is received, trans-

ceiver **721** provides the data for processing and storage by detection module **722**, tracking module **723**, processor **724**, and storage module **725**.

Detection module **722** detects characteristics of the bioelectrical signals to identify physical conditions of the monitored body that correspond to the detected bioelectrical signals. For example, detection module **722** may perform peak detection, sampling rate control, and/or digital filtering on the amplified bioelectrical signals.

Additionally, detection module **722** searches the EEG signal patterns with the extreme conditions. For example, besides observing the traditional EEG spectrum from DC to 100 Hz, detection module **722** scans wideband spectrums up to several kHz. This design can cover the spectral range from DC to 10 kHz with 10000 (40 dB) voltage gain.

Tracking module **723** tracks changes in the bioelectrical signals. In particular, tracking module **723** tracks and associates signatures extracted from active and passive systems. In other words, tracking module **723** performs a correlation function on the bioelectrical signals with known bioelectrical signal sets to exclude uncertainty in the bioelectrical signals. The types of received signals are mostly non-stationary and instantaneous with non-periodic features. Since most signal processing algorithms are designed for stationary and periodic waveforms with at least some identifiable features, knowledge of the waveforms must first be acquired in order to apply the algorithms to non-stationary, non-periodic waveforms. After acquiring knowledge of the signal properties and being able to estimate the signal resolution in time or frequency domain in advance, the system is able to capture the signal. In some embodiments, tracking module **723** applies weighted decisions and loop detection to enhance the detection of bioelectrical signals corresponding to known bioelectrical signals. Additionally, tracking module **723** may apply machine learning and feedback to dynamically enhance the detection of known bioelectrical signals.

As described above, most of the EMF signals from the human body fall between two extremes (i.e., between ELF and VLF). Additionally, the EMF signals are generally non-stationary and non-periodic. To make data from the signal useful and reliable, the detected EMF signals may be tracked with tracking algorithms. Here the specially designed tracking filter is applied, which can be designed for multiple target tracking to associate the relevant EMF data in same track. It can be easier to track and update tracking along time, analyze the signal signature, and track the differences.

In some embodiments, tracking module **723** performs correlation function on the EMF signals with known EMF signals to exclude uncertainty in the bioelectrical signals. Correlation functions measures the similarity of two signals as a function of the displacement of one signal relative to another. For example, correlation may be performed using a sliding dot product or sliding inner-product calculation. In some embodiments, the tracking module uses intermodulation techniques. The intermodulation techniques are applied by performing measurements at the range of frequencies of the signals to be detected and up the 7th order of harmonics of the signals to be detected.

Processor **724** analyzes the characteristics and changes of the bioelectrical signals. For example, processor **724** analyzes the EMF signals to detect EMF signals corresponding to physical conditions such as injury, health status, and physical activities.

Processor **724** performs human EMF mode decomposition to decompose a signal into intrinsic mode functions

(IMF) along with a trend, and obtain instantaneous frequency data. It is designed to work well for data that is nonstationary and nonlinear. Empirical mode decomposition (EMD) may be used to decompose the signal into different IMFs. The IMFs which may contain possible EMF modulations can be selected into next stage for post signal processing.

Processor **724** performs signal enhancements. One effective way to enhance the signal is to apply a matched filter. A matched filter is a signal processing technique used to increase the signal to noise ratio (SNR). Usually a perfectly matched filter can increase the signal level by 50 dB. To get ideal signal enhancement, a long sequence waveform is stored in correlation memory. In some embodiments, the long sequence waveform may be stored in data storage module **725**.

To characterize the EEG signals, processor **724** uses an 8 dB wavelet function to decompose the EEG signals into bandwidths known as alpha, beta, theta, delta, and gamma waves. The decomposed signals and FFT spectra may be analyzed. For example, the alpha wave, which can associate with eye closing, has a larger amplitude when the monitored body performs an eye blink compared to when the monitored body is in a relaxed state without performing an eye blink. In some embodiments, processor **724** applies a filtering algorithm to remove noise in a time-frequency domain to perform spectrogram digital signal processing on the bioelectrical signals. Processor **724** may also apply a filtering algorithm in a time domain and frequency domain to perform time domain and frequency domain digital signal processing on the bioelectrical signals.

The various components of the EMF detection system **700** can be implemented in a manner that is consistent with the various embodiments described herein.

FIG. **8** depicts a block diagram of an EMF detection system **800** consistent with various embodiments disclosed herein. Many of components disclosed in EMF detection system **800** are consistent with the components disclosed in EMF detection system **700**. In addition to components common to both systems, EMF detection system **800** also includes additional harmonic signal processing module **830**. Harmonic signal processing is based on the concept that a signal is composed of a sum of oscillatory components.

The output of differential amplifier **814** is input into two-way splitter **815**. Two-way splitter **815** then outputs the input to both signal processing module **820** and harmonic signal processing module **830**. Harmonic signal processing **830** receives a signal to perform harmonic signal processing.

Harmonic signal processing **830** includes a LO signal source **831**, mixer **832**, band pass filter **833**, and ADC **834**. LO signal source **831** comprises a local oscillator that is used with mixer **832** to change the frequency of a signal. The local oscillator may be a crystal oscillator that provides stability and high performance for a fixed frequency. Alternatively, the oscillator may be a variable-frequency oscillator to provide signals at different frequencies. Together, the LO signal source **831** and mixer **832** functions as a converter that converts the frequency of the signal received from two-way splitter **815**. The converted signal is then sent through band-pass filter **833** and ADC **834**.

Band pass filters passes frequencies within a certain range but attenuates the signal outside of the range. In some embodiments, bandpass filter **833** passes frequencies between 0.8-10 KHz. The signal passed from bandpass filter **833** is provided as input into analog-to-digital converter **834**. The analog-to-digital converter **834** converts the EMF sig-

nals into a digital signal for digital signal processing (DSP) at signal processing module **840**.

Using the harmonic signal processing module **830**, harmonic testing harmonic testing may be performed using: (1) signal tone sine wave, (2) frequency modulated continuous-wave (FMCW) signal with a 3-kHz bandwidth, (3) noise with a 3-kHz bandwidth, and (4) an up-converted ECG signal. Each waveform can be mixed with a 10-kHz LO signal by mixer **832**. The time domain, frequency domain and the 3rd harmonics for each scenario are examined to find the signature of ECG waveform after mixing with the designated LO signal. Based upon harmonic testing, it is determined that the 3rd harmonic spectral signature of the up-converted ECG signal is like a single-tone waveform.

Harmonic signal processing can be performed in order to understand and calibrate the intermodulation from the mixer, cables, signal generators, and digitizer of the system. In one or more examples, a two-tone measurement around the frequency range of the interested signals and up to the 7th order of its harmonics is performed.

The various components of the EMF detection system **800** can be implemented in a manner that is consistent with the various embodiments described herein.

FIG. **9** is a high-level block diagram illustrating an example of a processing system in which at least some operations described herein can be implemented (e.g., signal processing modules **660**, **720**, **840**), consistent with various embodiments. The processing system can be processing device **900**, which represents a system that can run any of the methods/algorithms described above. A system may include two or more processing devices such as represented in FIG. **9**, which may be coupled to each other via a network or multiple networks. A network can be referred to as a communication network.

In the illustrated embodiment, the processing device **900** includes one or more processors **910**, memory **911**, a communication device **912**, and one or more input/data (I/O) devices **913**, all coupled to each other through an interconnect **914**. The interconnect **914** may be or include one or more conductive traces, buses, point-to-point connections, controllers, adapters and/or other conventional connection devices. Each of the processors **910** may be or include, for example, one or more general-purpose programmable microprocessors or microprocessor cores, microcontrollers, application specific integrated circuits (ASICs), programmable gate arrays, or the like, or a combination of such devices. The processor(s) **910** control the overall operation of the processing device **900**. Memory **911** may be or include one or more physical storage devices, which may be in the form of random access memory (RAM), read-only memory (ROM) (which may be erasable and programmable), flash memory, miniature hard disk drive, or other suitable type of storage device, or a combination of such devices. Memory **911** may store data and instructions that configure the processor(s) **910** to execute operations in accordance with the techniques described above. The communication device **912** may be or include, for example, an Ethernet adapter, cable modem, Wi-Fi adapter, cellular transceiver, Bluetooth transceiver, or the like, or a combination thereof. Depending on the specific nature and purpose of the processing device **900**, the I/O devices **913** can include devices such as a display (which may be a touch screen display), audio speaker, keyboard, mouse or other pointing device, microphone, camera, etc.

While processes or blocks are presented in a given order, alternative embodiments may perform routines having steps, or employ systems having blocks, in a different order, and

some processes or blocks may be deleted, moved, added, subdivided, combined, and/or modified to provide alternative or sub-combinations, or may be replicated (e.g., performed multiple times). Each of these processes or blocks may be implemented in a variety of different ways. In addition, while processes or blocks are at times shown as being performed in series, these processes or blocks may instead be performed in parallel, or may be performed at different times. When a process or step is "based on" a value or a computation, the process or step should be interpreted as based at least on that value or that computation.

Software or firmware to implement the techniques introduced here may be stored on a machine-readable storage medium and may be executed by one or more general-purpose or special-purpose programmable microprocessors. A "machine-readable medium", as the term is used herein, includes any mechanism that can store information in a form accessible by a machine (a machine may be, for example, a computer, network device, cellular phone, personal digital assistant (PDA), manufacturing tool, any device with one or more processors, etc.). For example, a machine-accessible medium includes recordable/non-recordable media (e.g., read-only memory (ROM), random access memory (RAM), magnetic disk storage media, optical storage media, flash memory devices, etc.).

FIG. **10** is an active detection environment **1000** in accordance with one or more embodiments of the present disclosure. Active detection environment **1000** includes a signal generator **1010**, a monitored subject **1020**, and a receiver **1030**.

Signal generator **1010** includes a signal source **1011** to produce a source signal, background noise signal, and/or interference signal. The generated signal is then provided to antenna **1012** for transmission as propagated signal **1012** through monitored subject **1020**. Monitored body **1020** can be treated as a communication channel. The antenna system **1030** includes an electrode/antenna interface **1021**, amplifier **1032**, and filter **1033**. Electrode/antenna interface **1021** performs electrode/antenna matching on the electrodes and/or antennas (not shown) that detects the signals propagated across monitor subject **1020**. Amplifier **1032** and filter **1033** modifies the received signal such that it is suitable for signal processing. The various components of active detection environment **1000** can be implemented in a manner that is consistent with the various embodiments described herein.

FIG. **11** depicts a chart of contact points where electrodes may be placed for performing contact-based EMF detection in accordance with one or more embodiments of the present disclosure. The chart shows a side-view representation of a head **1100**. Contact points include the nasion **1110**, preauricular point **1120**, mastoid process **1130**, andinion **1140**. Electrodes may be used at one or more of the contact points to detect EMF and reference signals. The placement of multiple electrodes allows detection of localized EMF signals around the brain. Additionally, each contact point has different characteristics that provide different signal characteristics. For example, placement of electrodes on the ear produces less noise because there is less muscle current at that contact point. The various components disclosed in FIG. **11** can be implemented in a manner that is consistent with the various embodiments described herein.

CONCLUSION

From the foregoing, it will be appreciated that specific embodiments of the technology have been described herein for purposes of illustration, but that various modifications

can be made without deviating from the technology. In representative embodiments, the EMF detection system can have configurations other than those specifically shown and described herein, including other circuit designs. The various modules and circuits described herein may have other configurations in other embodiments, which also produce the desired characteristics described herein.

Certain aspects of the technology described in the context of particular embodiments may be combined or eliminated in other embodiments. Further, while advantages associated with certain embodiments of the technology have been described in the context of those embodiments, other embodiments may also exhibit such advantages, and not all embodiments need necessarily exhibit such advantages to fall within the scope of the present disclosure. Accordingly, the present disclosure and associated technology can encompass other embodiments not expressly shown or described herein. For example, while processes or blocks are presented in a given order, alternative embodiments may perform routines having steps, or employ systems having blocks, in a different order, and some processes or blocks may be deleted, moved, added, subdivided, combined, and/or modified to provide alternative or sub combinations. Each of these processes or blocks may be implemented in a variety of different ways. Also, while processes or blocks are at times shown as being performed in series, these processes or blocks may instead be performed in parallel, or may be performed at different times. Further, any specific numbers noted herein are only examples: alternative implementations may employ differing values or ranges.

To the extent any materials incorporated herein conflict with the present disclosure, the present disclosure controls.

We claim:

1. A system for detecting bioelectrical signal, the system comprising:

a reference module having a first electrode to detect a reference electrical signal;

a contact module having a second electrode to detect a contact electrical signal;

an antenna module, the antenna module including (1) an antenna to detect a non-contact EMF signal, and (2) an antenna circuit module to perform wideband tuning and amplify the non-contact EMF signal;

a receiver module, the receiver module including (1) an impedance matching module to match a source impedance of the antenna module, the reference module, and the contact module; and (2) a differential amplifier to amplify the difference between the reference signal and the non-contact EMF signal to produce a non-contact bioelectrical signal, and to amplify the difference between the reference signal and contact signal to produce a contact bioelectrical signal; and

a signal processing module including a processor (1) to apply a filtering algorithm to increase the signal-to-noise ratio of the bioelectrical signals, including the non-contact and contact bioelectrical signals, and (2) to perform digital signal processing on the bioelectrical signals.

2. The system of claim 1, wherein the antenna is an electro-textile based antenna including (1) non-conductive fibers, and (2) conductive fibers wound around individual non-conductive fibers, such that the non-conductive fiber and conductive fiber form a textile patch for receiving EMF signals from a human body without contact with the human body.

3. The system of claim 2, wherein the antenna is a conformal patch that is embedded in clothing material.

4. The system of claim 1, wherein the antenna is configured to receive signals from the extremely low frequency (ELF) band to the very low frequency (VLF) band to detect electroencephalography (EEG) signals and electrocardiography (ECG) signals.

5. The system of claim 1, wherein the antenna is one of dipole, monopole, or loop antenna.

6. The system of claim 1, wherein the antenna is a meshed patch antenna embedded in a flexible substrate.

7. The system of claim 1, wherein the antenna module includes a direct current (DC) power source to power the antenna circuit.

8. The system of claim 1, wherein the antenna circuit module includes (1) a tunable module including a tunable capacitor, (2) a band-stop filter to reject a predetermined frequency of noise, and (3) an amplifier to amplify the non-contact EMF signals.

9. The system of claim 8, wherein the tunable capacitor is operable to adjust the bandwidth of the antenna to include the extremely low frequency (ELF) band and the very low frequency (VLF) band.

10. The system of claim 1, wherein the impedance matching module includes an RLC circuit network that is tuned to match the source load of the antenna module.

11. The system of claim 1, wherein the receiver module includes a band-stop filter to reduce or suppress a predetermined noise frequency from the non-contact EMF signals.

12. The system of claim 1, wherein the receiver module includes a transceiver to transmit the contact bioelectrical signal and non-contact bioelectrical signals to the signal processing module.

13. The system of claim 1, wherein the signal processing module analyzes data related to the bioelectrical signals, the signal processing module including (1) a detection module to detect characteristics of the bioelectrical signals, (2) a tracking module to track the changes to the bioelectrical signals, and (3) a processor for analyzing the characteristics and changes of the bioelectrical signals.

14. The system of claim 13, wherein the detection module performs peak detection, sampling rate control, and/or digital filtering on the bioelectrical signals.

15. The system of claim 13, wherein the tracking module performs a correlation function on EMF signals with known EMF signals to exclude uncertainty in the bioelectrical signals.

16. The system of claim 13, wherein the tracking module applies weighted decisions and loop detection to enhance detection of bioelectrical signals corresponding to known bioelectrical signals.

17. The system of claim 13, wherein the processor applies machine learning and feedback to dynamically enhance the detection of known bioelectrical signals.

18. The system of claim 13, wherein the processor analyzes EMF signals to detect EMF signals corresponding to physical conditions indicative of injury, health status, and/or physical activities.

19. The system of claim 13, wherein the processor applies a filtering algorithm to remove noise in a time-frequency domain, and performs spectrogram digital signal processing on the bioelectrical signals.

20. The system of claim 13, wherein the processor applies a filtering algorithm in a time domain and frequency domain, and performs time domain and frequency domain digital signal processing on the bioelectrical signals.

21. The system of claim 13, wherein the processor applies a matched filter to improve the signal-to-noise ratio of the bioelectrical signals.

22. The system of claim **13**, wherein the processor applies a matched filter by sampling a bioelectrical signal measured from the human body to produce a known bioelectrical signal used to perform a correlation function.

23. The system of claim **13**, wherein the processor decomposes EEG signals extracted from the bioelectrical signals into alpha, beta, theta, delta, and/or gamma signals. 5

24. The system of claim **23**, wherein the processor decomposes the EEG signals using an 8 dB wavelet function.

25. The system of claim **13**, wherein the processor applies intermodulation techniques to the bioelectrical signals, the intermodulation technique applied by performing measurements at the range of frequencies of the signals to be detected and up a predetermined order of harmonics of the signals to be detected. 10 15

26. The system of claim **1**, wherein an electrode includes (1) a plastic substrate covered with an Ag/AgCl compound, (2) an electrolyte gel coated on the plastic substrate to provide a high ionic concentration, and (3) a conductive material to detect EMF signals when the electrode is in contact with a human surface. 20

* * * * *

专利名称(译)	用于人体生物电信号监测的混合电磁场信号检测系统		
公开(公告)号	US10206602	公开(公告)日	2019-02-19
申请号	US15/946715	申请日	2018-04-05
[标]发明人	REN EUGENE YU JIUN QIN YEXIAN LAI CHIEHPING		
发明人	REN, EUGENE YU-JIUN QIN, YEXIAN LAI, CHIEHPING		
IPC分类号	A61B5/05 H01Q1/27 H04Q9/02 A61B5/0464 A61B5/00 A61B5/0476		
CPC分类号	A61B5/05 A61B5/0464 A61B5/0476 A61B5/6804 A61B5/7264 H01Q1/273 H04Q9/02 A61B5/721 H04Q2209/40 A61B5/0408 G16H50/20 H01Q1/2291 H01Q1/48 H01Q5/335 H01Q21/28 H04Q9/00		
代理机构(译)	博钦律师事务所		
优先权	62/482123 2017-04-05 US		
其他公开文献	US20180289279A1		
外部链接	Espacenet		

摘要(译)

本公开包括电磁场检测和监测系统。该系统包括被动检测，主动检测和信号处理功能。至少一个实施例包括具有感测，处理，通信和数据存储能力的体戴系统。该系统提供可穿戴天线，以将电或磁形式的EMF能量有效地传输到传感器中。专门设计的处理算法可以处理收集的数据并生成结果，供医疗专业人员阅读和做出决策。

