



US009498147B2

(12) **United States Patent**
Massarwa et al.

(10) **Patent No.:** **US 9,498,147 B2**
(45) **Date of Patent:** **Nov. 22, 2016**

(54) **ENHANCED ECG CHART PRESENTATION**

(71) Applicant: **BIOSENSE WEBSTER (ISRAEL) LTD.**, Yokneam (IL)

(72) Inventors: **Fady Massarwa**, Baka El Gharbiya (IL); **Akram Zoabi**, Kfar Masser (IL)

(73) Assignee: **BIOSENSE WEBSTER (ISRAEL) LTD.**, Yokneam (IL)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 122 days.

(21) Appl. No.: **14/168,291**

(22) Filed: **Jan. 30, 2014**

(65) **Prior Publication Data**

US 2015/0208935 A1 Jul. 30, 2015

(51) **Int. Cl.**

A61B 5/044 (2006.01)
A61B 5/0205 (2006.01)
A61B 5/00 (2006.01)
A61B 5/0432 (2006.01)
A61B 5/06 (2006.01)
A61B 5/0408 (2006.01)
A61B 5/0452 (2006.01)
A61B 18/14 (2006.01)
A61B 18/00 (2006.01)
A61B 5/053 (2006.01)
A61B 5/01 (2006.01)
A61B 5/05 (2006.01)

(52) **U.S. Cl.**

CPC **A61B 5/044** (2013.01); **A61B 5/02055** (2013.01); **A61B 5/0432** (2013.01); **A61B 5/0452** (2013.01); **A61B 5/04085** (2013.01); **A61B 5/062** (2013.01); **A61B 5/6852** (2013.01); **A61B 5/6885** (2013.01); **A61B 5/7221** (2013.01); **A61B 5/7435** (2013.01); **A61B 18/1492** (2013.01); **A61B 5/01** (2013.01); **A61B 5/05** (2013.01); **A61B 5/0538**

(2013.01); **A61B 5/06** (2013.01); **A61B 5/6823** (2013.01); **A61B 5/6869** (2013.01); **A61B 2018/00357** (2013.01); **A61B 2018/00577** (2013.01); **A61B 2034/2051** (2016.02); **A61B 2034/2063** (2016.02); **A61B 2090/065** (2016.02); **A61B 2218/002** (2013.01); **A61B 2562/0223** (2013.01)

(58) **Field of Classification Search**

None

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,391,199 A 2/1995 Ben-Haim
5,443,489 A 8/1995 Ben-Haim
5,558,091 A 9/1996 Acker
5,803,084 A 9/1998 Olson

(Continued)

FOREIGN PATENT DOCUMENTS

EP 2057942 A1 5/2009
WO WO 2007/015139 A2 2/2007

(Continued)

OTHER PUBLICATIONS


European Search Report dated Jun. 22, 2015 for corresponding Application No. EP15153012.

Primary Examiner — Erica Lee

(57) **ABSTRACT**

A method, including collecting first data samples of electrical potentials produced by a heart at a sequence of sampling times, and collecting second data samples of ancillary data with respect to the heart at the sampling times. Based on the first and second data samples, a trace of the electrical potentials collected at the sampling times is presented, on a display, the trace having a pseudo-three-dimensional (3D) characteristic that varies responsively to the ancillary data collected at each of the sampling times.

13 Claims, 3 Drawing Sheets

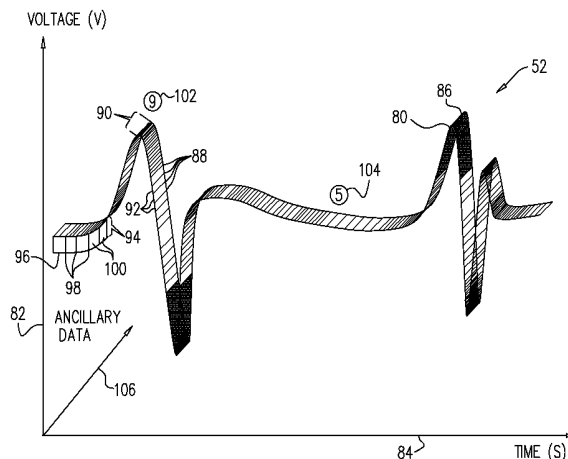

(56)

References Cited

U.S. PATENT DOCUMENTS


5,944,022	A	8/1999	Nardella
5,983,126	A	11/1999	Wittkamp
6,172,499	B1	1/2001	Ashe
6,177,792	B1	1/2001	Govari
6,456,864	B1	9/2002	Swanson
6,471,693	B1	10/2002	Carroll et al.
6,690,963	B2	2/2004	Ben-Haim
6,788,967	B2	9/2004	Ben-Haim
2003/0028119	A1	2/2003	Xue et al.
2004/0111021	A1	6/2004	Olson

2006/0258947	A1	11/2006	Olson	
2008/0058656	A1 *	3/2008	Costello et al.	600/508
2009/0093806	A1	4/2009	Govari	
2009/0138007	A1	5/2009	Govari	
2013/0109988	A1 *	5/2013	Kim et al.	600/515
2013/0190637	A1	7/2013	Zhang	
2014/0125477	A1 *	5/2014	Kasuya et al.	340/525

FOREIGN PATENT DOCUMENTS

WO	WO 2008/008796	A2	1/2008
WO	WO 2008/135731	A1	11/2008

* cited by examiner

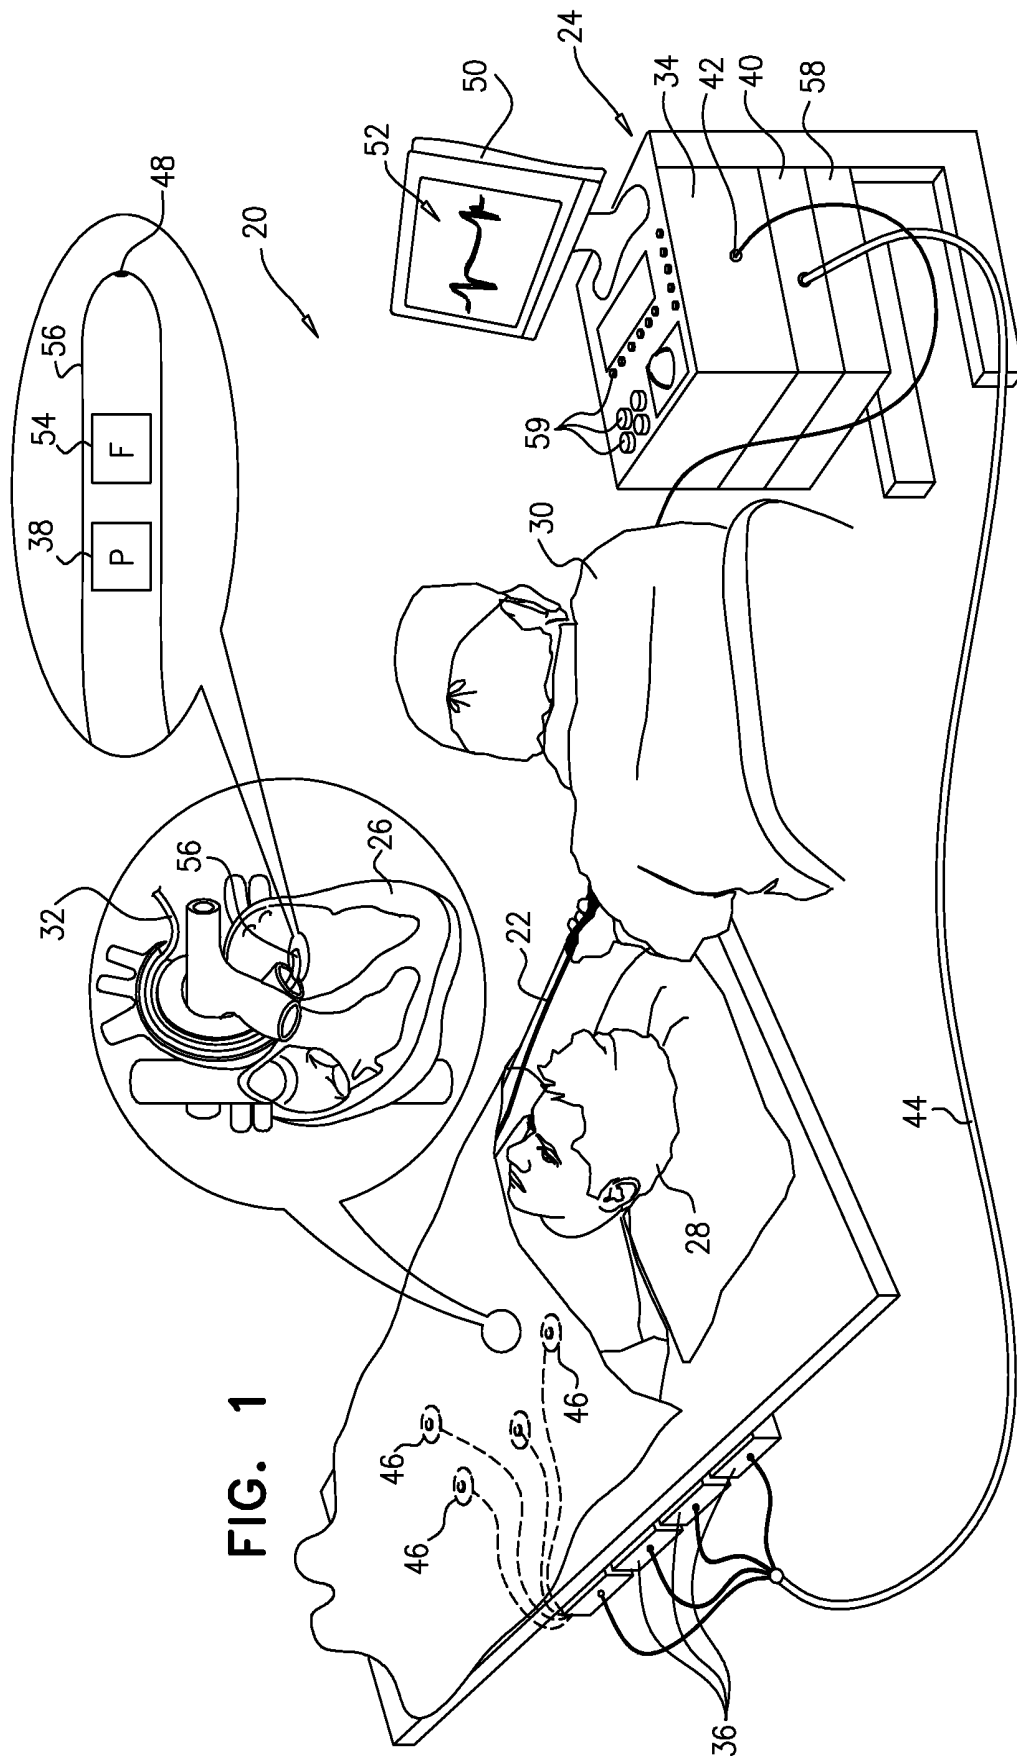

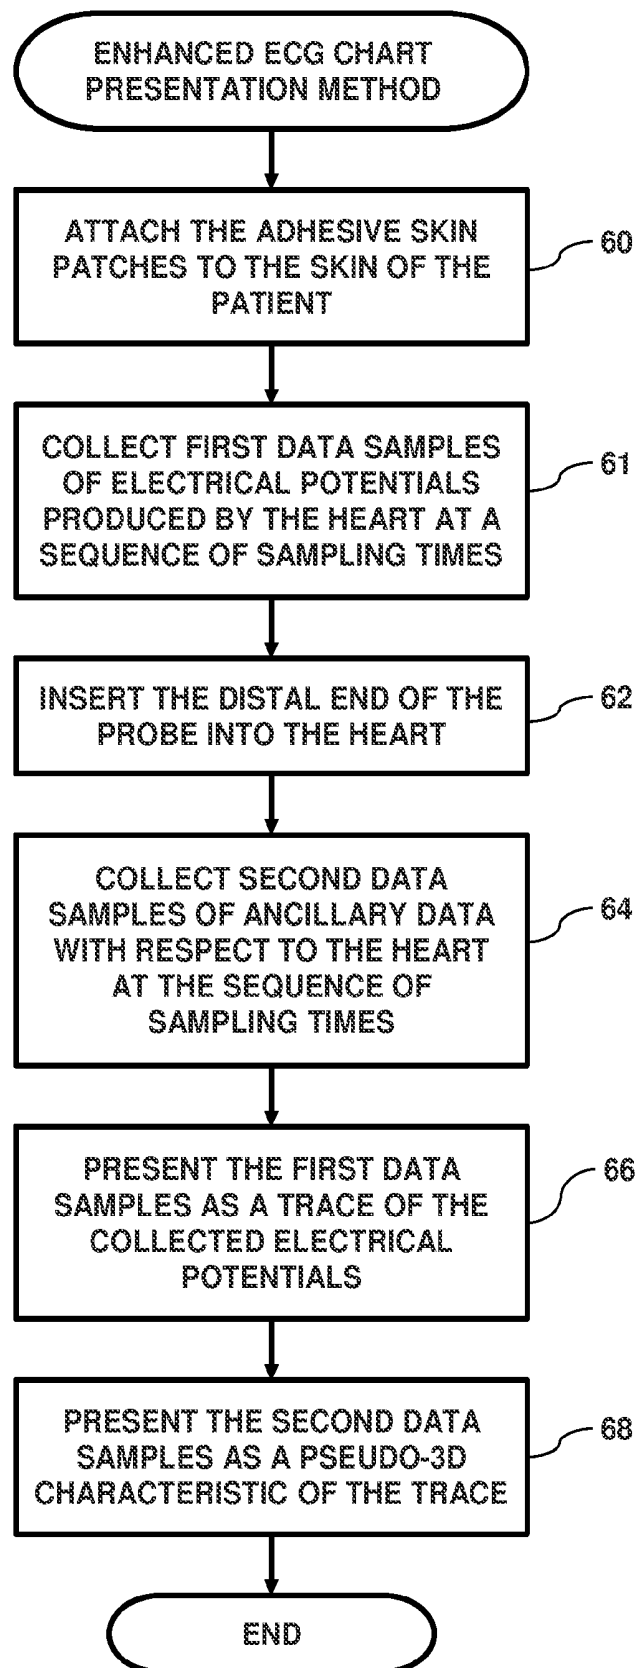


FIG. 2

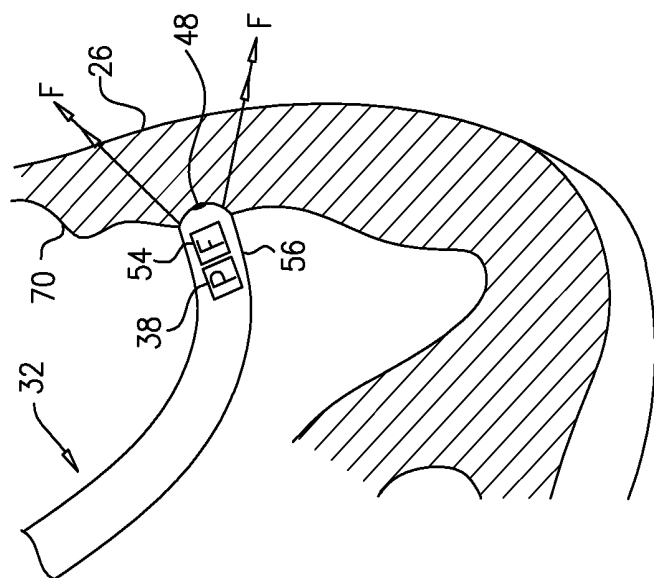


FIG. 3

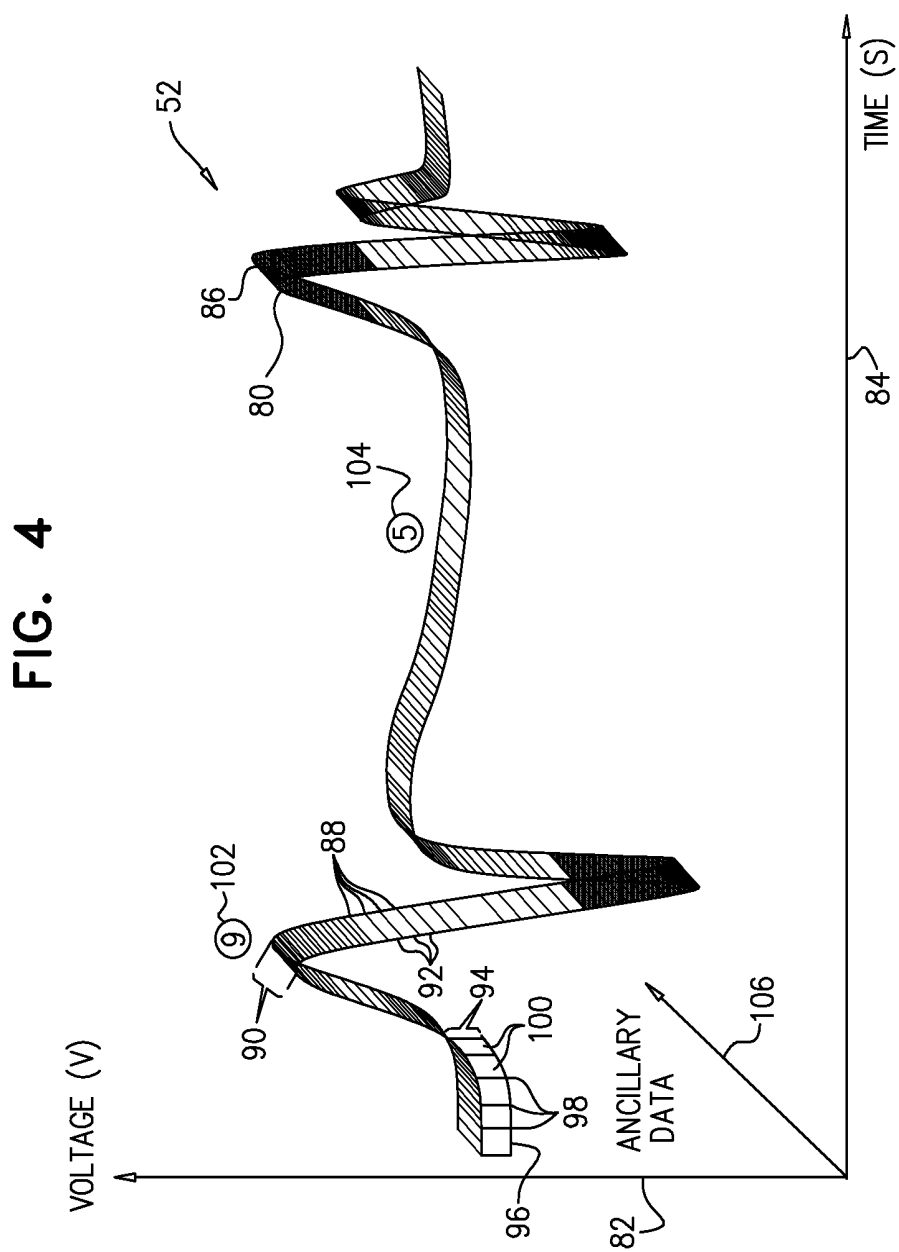


FIG. 4

ENHANCED ECG CHART PRESENTATION**FIELD OF THE INVENTION**

The present invention relates generally to electrocardiography (ECG), and specifically to a system that presents ECG and ancillary electrophysiological data in a single chart.

BACKGROUND OF THE INVENTION

During a medical procedure such as cardiac ablation, there are typically simultaneous streams of real-time data that an operator (e.g., a physician) monitors while performing the procedure. For example, while using an intracardiac catheter to perform an ablation on intracardiac tissue, the operator may want to keep track of real-time electrophysiological (EP) data such as electrocardiography (ECG) data, and ancillary data such as locations of the catheter's distal tip and ablation energy being delivered to the heart tissue.

Documents incorporated by reference in the present patent application are to be considered an integral part of the application except that to the extent any terms are defined in these incorporated documents in a manner that conflicts with the definitions made explicitly or implicitly in the present specification, only the definitions in the present specification should be considered.

SUMMARY OF THE INVENTION

There is provided, in accordance with an embodiment of the present invention a method, including collecting first data samples of electrical potentials produced by a heart at a sequence of sampling times, collecting second data samples of ancillary data with respect to the heart at the sampling times, and presenting, on a display, based on the first and second data samples, a trace of the electrical potentials collected at the sampling times, the trace having a pseudo-three-dimensional (3D) characteristic that varies responsively to the ancillary data collected at each of the sampling times.

In some embodiments, the first data samples include electrical impulses conveyed from body surface electrodes, and the ancillary data includes measurements collected from one or more sensors contained within a distal end of a flexible insertion tube configured for insertion into a heart. In additional embodiments, the measurements can be selected from a list consisting of ablation energy, a location of a distal end of the catheter, a measurement of a force exerted by the distal end on endocardial tissue of the heart, a quality of contact between the distal end and the endocardial tissue, a magnitude and a phase of impedance detected by the body surface electrodes, a temperature of the endocardial tissue, a Force Power Time Integral, and irrigation fluid parameters.

In some embodiments, presenting the trace having the pseudo-3D characteristic includes presenting, on the display, a ribbon chart having a ribbon including first and second lines, the second line following a contour of the first line. In additional embodiments, the pseudo-3D characteristics can be selected from a list consisting of third lines connecting the first and the second lines, a shading of one or more regions between the first and the second lines, a thickness of the ribbon, shading the thickness of the ribbon, and a color of the ribbon. In further embodiments, the ribbon chart has multiple axes including a vertical axis, a horizontal axis and a pseudo-depth axis, and the method includes presenting a rotation of the ribbon chart along one of the axes.

In supplementary embodiments, the method includes presenting an icon on the ribbon chart indicating an occurrence of one or more events, and presenting information on the one or more events upon receiving an input selecting the icon. In additional embodiments, the method includes saving the first and the second data samples to a memory.

There is also provided, in accordance with an embodiment of the present invention apparatus, including a display, and a processor configured to collect first data samples of electrical potentials produced by a heart of a patient at a sequence of sampling times, to collect second data samples of ancillary data with respect to the heart at the sampling times, and to present, on the display, based on the first and second data samples, a trace of the electrical potentials collected at the sampling times, the trace having a pseudo-three-dimensional (3D) characteristic that varies responsively to the ancillary data collected at each of the sampling times.

There is further provided, in accordance with an embodiment of the present invention a computer software product, the product including a non-transitory computer-readable medium, in which program instructions are stored, which instructions, when read by a computer, cause the computer to collect first data samples of electrical potentials produced by a heart at a sequence of sampling times, to collect second data samples of ancillary data with respect to the heart at the sampling times, and to present, on a display, based on the first and second data samples, a trace of the electrical potentials collected at the sampling times, the trace having a pseudo-three-dimensional (3D) characteristic that varies responsively to the ancillary data collected at each of the sampling times.

BRIEF DESCRIPTION OF THE DRAWINGS

The disclosure is herein described, by way of example only, with reference to the accompanying drawings, wherein:

FIG. 1 is a schematic, pictorial illustration of a medical system configured to present an enhanced electrocardiography (ECG) chart, in accordance with an embodiment of the present invention;

FIG. 2 is a flow diagram that schematically illustrates a method of presenting the ECG chart that includes ancillary data, in accordance with an embodiment of the present invention;

FIG. 3 is a schematic view showing a distal tip of a catheter in contact with endocardial tissue of a cardiac chamber, in accordance with an embodiment of the present invention; and

FIG. 4 is a schematic view of the enhanced chart showing ECG and ancillary data, in accordance with an embodiment of the present invention.

DETAILED DESCRIPTION OF EMBODIMENTS**Overview**

Embodiments of the present invention provide methods and systems for presenting ECG and ancillary data as a single chart on a display. During a medical procedure such as cardiac tissue, the ancillary data may comprise measurements received from a distal end of an intracardiac catheter within a cardiac chamber, such as a temperature of intracardiac tissue, positions of the distal end, and a measurement of ablation energy delivered by the distal end to the intracardiac tissue.

In some embodiments, the ECG data can be presented as a chart (e.g., a line chart) on the display, and the ancillary data can be presented as a pseudo-three-dimensional (3D) enhancement of the chart. By combining ECG and ancillary data into a single chart, embodiments of the present invention enable an operator to track multiple ECG and ancillary data parameters by looking at a single chart.

As described hereinbelow, upon collecting first data samples of electrical potentials produced by a heart at a sequence of sampling times, the first data samples are presented as an ECG chart on a display, the ECG chart comprising a trace of the electrical potentials collected at the sampling times. In addition to collecting the first data, second data samples of ancillary data with respect to the heart are also collected at the sampling times, and the second data is presented as a pseudo-three-dimensional trace that varies responsively to the ancillary data collected at each of the sampling times.

System Description

FIG. 1 is a schematic, pictorial illustration of a medical system 20 configured to present an enhanced ECG chart 52, in accordance with an embodiment of the present invention. System 20 comprises a probe 22, such as an intracardiac catheter, and a control console 24. In embodiments described hereinbelow, it is assumed that probe 22 is used for diagnostic or therapeutic treatment, such as for mapping electrical potentials in a heart 26 of a patient 28. Alternatively, probe 22 may be used, mutatis mutandis, for other therapeutic and/or diagnostic purposes in the heart or in other body organs.

An operator 30 inserts probe 22 through the vascular system of patient 28 so that a distal end 32 of probe 22 enters a chamber of heart 26. Console 24 typically uses magnetic position sensing to determine position coordinates of distal end inside heart 26. To determine the position coordinates, a driver circuit 34 in console 24 drives field generators 36 to generate magnetic fields within the body of patient 28. Typically, field generators 36 comprise coils, which are placed below the patient's torso at known positions external to patient 28. These coils generate magnetic fields in a predefined working volume that contains heart 26.

A magnetic field sensor 38 (also referred to herein as location sensor 38) within distal end 32 of probe 22 generates electrical signals in response to these magnetic fields. A signal processor 40 processes these signals in order to determine the position coordinates of distal end 32, typically including both location and orientation coordinates. The method of position sensing described hereinabove is implemented in the CARTO™ mapping system produced by Biosense Webster Inc., of Diamond Bar, Calif., and is described in detail in the patents and the patent applications cited herein.

Location sensor 38 transmits a signal to console 24 that is indicative of the location coordinates of distal end 32. Location sensor 38 may comprise one or more miniature coils, and typically comprises multiple coils oriented along different axes. Alternatively, location sensor 38 may comprise either another type of magnetic sensor, or position transducers of other types, such as impedance-based or ultrasonic location sensors. Although FIG. 1 shows a probe with a single location sensor, embodiments of the present invention may utilize probes with more than one location sensor.

Although in the present example system 20 measures the position of distal end 32 using magnetic-based sensors, other

position tracking techniques may be used (e.g., impedance-based sensors). Magnetic position tracking techniques are described, for example, in U.S. Pat. Nos. 5,391,199, 5,443, 489, 6,788,967, 6,690,963, 5,558,091, 6,172,499, 6,177,792, whose disclosures are incorporated herein by reference. Impedance-based position tracking techniques are described, for example, in U.S. Pat. Nos. 5,983,126, 6,456, 864 and 5,944,022, whose disclosures are incorporated herein by reference.

Processor 40 typically comprises a general-purpose computer, with suitable front end and interface circuits for receiving signals from probe 22 and controlling the other components of console 24. Processor 40 may be programmed in software to carry out the functions that are described herein. The software may be downloaded to console 24 in electronic form, over a network, for example, or it may be provided on non-transitory tangible media, such as optical, magnetic or electronic memory media. Alternatively, some or all of the functions of processor 40 may be carried out by dedicated or programmable digital hardware components.

In the example of FIG. 1, console 24 is also connected by a cable 44 to body surface electrodes, which typically comprise adhesive skin patches 46 attached to the patient's skin. In embodiments of the present invention, the surface electrodes can pick up electrical impulses generated by the polarization and depolarization of cardiac tissue, and convey the impulses to console 24 via cable 44.

An input/output (I/O) interface 42 enables console 24 to interact with probe 22 and the surface electrodes. Based on the electrical impulses received from the surface electrodes and signals received from probe 22 (via interface 42 and other components of system 20), processor 40 drives a display 50 to present operator 30 with chart 52 (also referred to herein as an enhanced ECG chart 52), as described in detail hereinbelow.

Probe 22 also comprises a force sensor 54 contained within distal end 32. Force sensor 54 measures a force applied by a distal tip 56 of probe 22 to the endocardial tissue of heart 26 by generating a signal to the console that is indicative of the force exerted by the distal tip on the endocardial tissue. In one embodiment, the force sensor may comprise a magnetic field transmitter and receiver connected by a spring in distal end 32, and may generate an indication of the force based on measuring the deflection of the spring. Further details of this sort of probe and force sensor are described in U.S. Patent Application Publications 2009/0093806 and 2009/0138007, whose disclosures are incorporated herein by reference. Alternatively, distal end 32 may comprise another type of force sensor.

In some embodiments, probe 22 may comprise an electrode 48 coupled to the distal end and configured to function as an impedance-based position transducer. Additionally or alternatively, electrode 48 can be configured to measure a certain physiological property (e.g., the local surface electrical potential) at each of the multiple locations. In further embodiments, electrode 48 can be used to ablate endocardial tissue in heart 26.

During the diagnostic treatment, processor 40 presents chart 52 and stores data representing the chart in a memory 58. Memory 58 may comprise any suitable volatile and/or non-volatile memory, such as random access memory or a hard disk drive. In some embodiments, operator 30 can manipulate chart 52 using one or more input devices 59.

FIG. 2 is a flow diagram that schematically illustrates a method of presenting chart 52 showing ECG and ancillary data collected during a procedure on heart 26, FIG. 3 is a

schematic detail view showing distal tip **56** in contact with endocardial tissue **70** of the heart, and FIG. **4** is a schematic detail view of the enhanced ECG chart, in accordance with an embodiment of the present invention. In the example described herein, processor **40** presents chart **52** as a pseudo-

three-dimensional ribbon chart, as described hereinbelow. In an initial step **60**, operator **30** attaches adhesive skin patches **46** to the skin of patient **28**, and in a first collection step **61**, processor **40** collects, from the surface electrodes in the adhesive skin patches, first data samples comprising electrical potentials produced by heart **26** at a sequence of sampling times. In an insertion step **62**, operator **30** inserts probe **22** into a chamber of heart **26** (also referred to herein as the cardiac chamber), and in a second collection step **64**, the processor collects second data samples of ancillary data with respect to heart **26** at the sampling times.

In embodiments of the present invention, the second data samples may comprise measurements received from one or more sensors mounted in the distal end of probe **22**. For example as operator **30** advances probe **22** so that distal tip **56** engages endocardial tissue **70** and exerts force **F** on the endocardial tissue, as shown in FIG. **3**, the ancillary data may comprise force measurements received from force sensor **54** that indicate force **F**. Additional examples of ancillary data that processor can receive from probe **22** or other elements of console **24** include, but are not limited to:

A magnitude and phase of an impedance detected by the surface electrodes in adhesive skin patches **46**.

A position of distal tip **56**. In some embodiments, position signals received from location sensor **38** can indicate a distance between distal tip **56** and endocardial tissue **70**.

A quality of contact between distal tip **56** and endocardial tissue **70**, as indicated by force signals received from force sensor **54**. The quality of contact may comprise a magnitude and a direction of force **F**.

A measurement of ablation energy delivered by electrode **48** to endocardial tissue. Typically, the ablation energy varies during an ablation procedure.

Starting and ending times indicating when ablation energy is delivered to the endocardial tissue.

Irrigation parameters such as starting and ending times, indicating when probe **22** is delivering irrigation fluid to endocardial tissue **70**, as well as pressures and temperatures of the irrigation fluid.

A temperature of the endocardial tissue in contact with the distal tip.

Force Power Time Integral (FPTI). FPTI is a scalar value that represents the force power time integral during ablation. During an ablation procedure, the FPTI value indicates a quality of an ablation lesion.

Based on the first data samples, processor **40** presents, on display **50**, a trace of the electrical potentials collected at the sampling times in a first presentation step **66**. In the example shown in FIG. **4**, the trace comprises a first line **80** that plots potentials along a vertical axis **82** against time along a horizontal axis **84**, wherein the potentials are measured as voltages **V** and the time is measured in seconds **S**. Finally, based on the second data samples, processor **40** presents a pseudo-three-dimensional characteristic that varies responsively to the ancillary data collected at each of the sampling times in a second presentation step **68**, and the method ends. In some embodiments, processor **40** can save the first and the second data samples to memory **58**.

In the example shown in FIG. **4**, processor **40** presents a second line **86** that is that follows the contour of line **80**, and presents slanted connecting lines **88** that connect the first

line to the second line. Processor **40** presents the combination of lines **80**, **86** and **88** as a “ribbon” having a pseudo-depth **90** along a “pseudo-depth” ancillary data axis **106**.

While the example shown in FIG. **4** shows the ribbon having a uniform pseudo-depth **90**, processor **40** can vary the pseudo-depth of the ribbon in order to indicate values of the ancillary data. For example, as operator **30** presses distal tip **56** against endocardial tissue **70**, processor **40** can vary pseudo-depth **90** based on the force **F**. Additionally or alternatively processor **40** can vary the spacing between connecting lines **88** in order to indicate the values of the ancillary data. In some embodiments, processor **40** can vary the spacing between the connecting lines in order to indicate a distance between distal tip **56** and the endocardial tissue. For example, processor **40** can reduce the spacing between the connecting lines as distal tip **56** moves closer to and engages endocardial tissue **70**.

Additional pseudo-3D effects, that processor **40** can use to present the ancillary data, include, but are not limited to:

Depth shading. In the example shown in FIG. **4**, processor shades some regions **92** that are bounded by the first, the second and the connected lines. In some embodiments, processor **40** can shade a given region **92** with different colors and/or patterns to indicate when ablation energy was delivered to the endocardial tissue.

Thickness. Processor **40** can vary a vertical thickness (also referred to herein as height) **94** of line **80** by varying height **94** between line **80** and a line **96**. In some embodiments, processor **40** can vary thickness **94** to indicate a pressure of irrigation fluid conveyed by probe **22** to endocardial tissue **70**. Processor **40** can present the thickness as a rectangular “tube”, and in some embodiments operator **30** can use input devices **59** to select and/or change which “sides” of the tube are visible to the operator.

Vertical lines. Processor **40** can present vertical lines **98**, thereby defining regions **100**. In some embodiments, processor **40** can present lines **98** in different colors to indicate when distal tip **56** engages and disengages from endocardial tissue **70**.

Vertical shading. Processor **40** can shade regions **100** with different colors and/or patterns. In some embodiments, the shading can indicate a temperature of endocardial tissue **70** in contact with distal tip **56**.

Line color. Processor can change colors of lines **80**, **86**, **88**, **96** and **98** in the ribbon based on values of the ancillary data.

As described supra, chart **52** comprises axes **82**, **84** and **106**. In some embodiments, operator **30** can instruct, using input device(s) **50**, processor **40** to “rotate” chart **52** along one (or more) of the axes.

In some embodiments, the ancillary data collected by system **20** may have a binary state, such as a touch/no touch parameter (i.e., between the distal tip and the endocardial tissue). For ancillary data having a binary state, processor **40** can present any changes to the binary data as a change of transparency (e.g., transparent or opaque).

Chart **52** may incorporate a visual indication of an occurrence of an event, such as when ablation power is delivered to endocardial tissue **70**. In the example shown in FIG. **4**, processor **40** presents icons **102** and **104** to indicate an occurrence of multiple events such as:

Acquiring mapping points.

Starting and stopping an ablation procedure.

Creating a site that presents parameters of lesion formation. The CARTO™ mapping system referenced above provides such a site as a VisiTag™ site.

Distal tip **56** exerting a high (i.e., excessive) force on endocardial tissue **70**.

A system error.

Detecting a severe inaccuracy.

Starting and stopping pacing of heart **26**.

Detecting that the patient's respiration needs training.

In some embodiments, icons **102** and **104** can indicate a corresponding number of the events transpiring at a given time. In additional embodiments, operator **30** use a given input device **59** to select one of the icons, and upon processor **40** receiving a signal from the given input device, the processor can present, on the display, more information of the events/occurrences. In the example shown in FIG. **4**, icon **102** indicates an occurrence of nine events at a first given time, and icon **104** indicates an occurrence of five events at a second given time.

While embodiments herein describe processor **40** presenting chart **52** on display **50**, presenting two-dimensional chart **52** with pseudo-3D characteristics on other types of two-dimensional output devices is considered to be within the spirit and scope of the present invention. For example, processor **40** can present chart **52** with pseudo-3D characteristics on a printer or as an image projected on a flat surface by a projector.

It will be appreciated that the embodiments described above are cited by way of example, and that the present invention is not limited to what has been particularly shown and described hereinabove. Rather, the scope of the present invention includes both combinations and subcombinations of the various features described hereinabove, as well as variations and modifications thereof which would occur to persons skilled in the art upon reading the foregoing description and which are not disclosed in the prior art.

The invention claimed is:

1. A method, comprising:

receiving first data samples of electrical potentials produced by a heart at a sequence of sampling times, wherein the first data samples are collected from body surface electrodes;

receiving second data samples of ancillary data with respect to the heart at the sampling times, wherein the second data samples are collected by one or more sensors contained within a distal end of a flexible probe inserted into the heart; and

generating, based on the first and second data samples, a trace of the electrical potentials collected at the sampling times, the trace having a pseudo-three-dimensional (pseudo-3D) characteristic that varies responsively to the ancillary data collected at each of the sampling times, the trace comprising a ribbon chart having a ribbon including a first line and a second line following a contour of the first line, the first and second lines defining a depth along a pseudo-depth ancillary data axis of the ribbon chart.

2. The method according to claim 1, wherein the ancillary data comprises measurements selected from a list consisting of ablation energy, a location of the distal end of the flexible probe, a measurement of a force exerted by the distal end on endocardial tissue of the heart, a quality of contact between the distal end and the endocardial tissue, a magnitude and a phase of impedance detected by the body surface electrodes, a temperature of the endocardial tissue, a Force Power Time Integral, and irrigation fluid parameters.

3. The method according to claim 1, wherein the pseudo-3D characteristic is selected from a list consisting of third lines connecting the first and the second lines, a shading of one or more regions between the first and the second lines,

a thickness of the ribbon, shading the thickness of the ribbon, and a color of the ribbon.

4. The method according to claim 1, wherein the ribbon chart has multiple axes comprising a vertical axis, a horizontal axis and the pseudo-depth ancillary data axis, and further comprises rotating the ribbon chart along one of the axes.

5. The method according to claim 1, and comprising generating an icon on the ribbon chart indicating an occurrence of one or more events, and providing information on the one or more events upon receiving an input selecting the icon.

6. The method according to claim 1, and comprising saving the first and the second data samples to a memory.

7. An apparatus, comprising:

a console having one or more processors; and

a non-transitory computer readable medium storing a plurality of instructions, which when executed, cause the one or more processors to:

receive first data samples of electrical potentials produced by a heart of a patient at a sequence of sampling times, wherein the first data samples are collected by a plurality of surface electrodes,

receive second data samples of ancillary data with respect to the heart at the sampling times, wherein the second data samples are collected by one or more sensors at the distal end of a flexible probe; and

generate, based on the first and second data samples, a trace of the electrical potentials collected at the sampling times, the trace having a pseudo-three-dimensional (3D) characteristic that varies responsively to the ancillary data collected at each of the sampling times, the trace comprising a ribbon chart having a ribbon including a first line and a second line following a contour of the first line, the first and second lines defining a depth along a pseudo-depth ancillary data axis of the ribbon chart.

8. The apparatus according to claim 7, wherein the ancillary data comprises measurements selected from a list consisting of ablation energy, a location of a distal end of the catheter, a measurement of a force exerted by the distal end on endocardial tissue of the heart, a quality of contact between the distal end and the endocardial tissue, a magnitude and a phase of impedance detected by the body surface electrodes, a temperature of the endocardial tissue, a Force Power Time Integral, and irrigation fluid parameters.

9. The apparatus according to claim 7, wherein the pseudo-3D characteristic is selected from a list consisting of third lines connecting the first and the second lines, a shading of one or more regions between the first and the second lines, varying a thickness of the ribbon, a shading of the thickness of the ribbon, and a color of the ribbon.

10. The apparatus according to claim 7, wherein the ribbon chart has multiple axes comprising a vertical axis, a horizontal axis and the pseudo-depth ancillary data axis, and wherein the instructions, when executed, further cause the one or more processors to rotate the ribbon chart along one of the axes.

11. The apparatus according to claim 7, wherein the instructions, when executed, further cause the one or more processors to generate an icon on the ribbon chart indicating an occurrence of one or more events, and to provide information on the one or more events upon receiving an input selecting the icon.

12. The apparatus according to claim 7, wherein the instructions, when executed, further cause the one or more processors to save the first and the second data samples to a memory.

13. A computer software product comprising computer-readable program code to be executed by one or more processors when retrieved from a non-transitory computer-readable medium, the program code including instructions to:

receive first data samples of electrical potentials produced by a heart of a patient at a sequence of sampling times, wherein the first data samples are collected by the plurality of surface electrodes,

receive second data samples of ancillary data with respect to the heart at the sampling times, wherein the second data samples are collected by the one or more sensors at the distal end of the flexible probe; and

generate, based on the first and second data samples, a trace of the electrical potentials collected at the sampling times, the trace having a pseudo-three-dimensional (pseudo-3D) characteristic that varies responsively to the ancillary data collected at each of the sampling times, the trace comprising a ribbon chart having a ribbon including a first line and a second line following a contour of the first line, the first and second lines defining a depth along a pseudo-depth ancillary data axis of the ribbon chart.

* * * * *

专利名称(译)	增强的ECG图表演示		
公开(公告)号	US9498147	公开(公告)日	2016-11-22
申请号	US14/168291	申请日	2014-01-30
[标]申请(专利权)人(译)	韦伯斯特生物官能(以色列)有限公司		
申请(专利权)人(译)	生物传感韦伯斯特 (以色列) LTD.		
当前申请(专利权)人(译)	生物传感韦伯斯特 (以色列) LTD.		
[标]发明人	MASSARWA FADY ZOABI AKRAM		
发明人	MASSARWA, FADY ZOABI, AKRAM		
IPC分类号	A61B5/044 A61B5/0408 A61B5/0452 A61B5/00 A61B5/06 A61B5/0205 A61B5/0432 A61B18/14 A61B5/053 A61B5/01 A61B5/05 A61B18/00		
CPC分类号	A61B5/062 A61B5/6852 A61B5/044 A61B5/02055 A61B5/0432 A61B5/0452 A61B5/04085 A61B5/6885 A61B5/7221 A61B5/7435 A61B18/1492 A61B5/01 A61B5/05 A61B5/0538 A61B5/06 A61B5/6823 A61B5/6869 A61B2018/00357 A61B2018/00577 A61B2034/2051 A61B2034/2063 A61B2090/065 A61B2218/002 A61B2562/0223 A61B5/063		
审查员(译)	LEE , ERICA		
其他公开文献	US20150208935A1		
外部链接	Espacenet USPTO		

摘要(译)

一种方法，包括：在一系列采样时间采集由心脏产生的电势的第一数据样本，以及在采样时间采集相对于心脏的辅助数据的第二数据采样。基于第一和第二数据样本，在显示器上呈现在采样时间收集的电势的迹线，所述迹线具有响应于在每个采集时间收集的辅助数据而变化的伪三维 (3D) 特性的采样时间。

