



US010159460B2

(12) **United States Patent**
Ingold, Jr. et al.

(10) **Patent No.:** **US 10,159,460 B2**
(45) **Date of Patent:** ***Dec. 25, 2018**

(54) **METHOD FOR LOCATING A CATHETER TIP USING AUDIO DETECTION**

(71) Applicant: **AngioDynamics, Inc.**, Latham, NY (US)

(72) Inventors: **James E. Ingold, Jr.**, Hillsborough, NC (US); **Thomas Vincent Casey, II**, Troy, NY (US); **Brian F. Nentwick**, Greenfield Center, NY (US)

(73) Assignee: **AngioDynamics, Inc.**, Latham, NY (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 102 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **15/165,770**

(22) Filed: **May 26, 2016**

(65) **Prior Publication Data**
US 2016/0270759 A1 Sep. 22, 2016

Related U.S. Application Data
(63) Continuation of application No. 14/272,890, filed on May 8, 2014, now Pat. No. 9,351,663, which is a continuation of application No. 13/251,686, filed on Oct. 3, 2011, now Pat. No. 8,753,292.

(51) **Int. Cl.**
A61B 5/00 (2006.01)
A61B 8/08 (2006.01)
A61B 5/06 (2006.01)
A61B 5/0205 (2006.01)
A61B 5/0402 (2006.01)
A61B 7/04 (2006.01)
A61M 25/01 (2006.01)
A61B 34/20 (2016.01)

(52) **U.S. Cl.**
CPC **A61B 8/0841** (2013.01); **A61B 5/0205** (2013.01); **A61B 5/0402** (2013.01); **A61B 5/061** (2013.01); **A61B 7/04** (2013.01); **A61M 25/0108** (2013.01); **A61B 2034/2063** (2016.02); **A61B 2562/0204** (2013.01); **A61M 2025/0166** (2013.01); **A61M 2205/0294** (2013.01)

(58) **Field of Classification Search**
CPC **A61B 5/06**; **A61B 5/061**; **A61B 5/0205**; **A61B 5/0402**; **A61B 7/04**; **A61B 8/0841**
USPC **600/586**
See application file for complete search history.


(56) **References Cited**
U.S. PATENT DOCUMENTS
5,161,536 A * 11/1992 Vilkomerson A61B 8/0833
600/443
5,280,786 A * 1/1994 Wlodarczyk A61B 5/1459
356/41
5,386,828 A * 2/1995 Owens A61B 5/06
600/13

(Continued)

Primary Examiner — Max Hindenburg
(74) *Attorney, Agent, or Firm* — Zachary F. Madonna, Esq.

(57) **ABSTRACT**
A method for locating a catheter tip within a human body is disclosed. An audio sensor is positioned at a site on the human body. An audio signal is detected by the audio sensor, and transmitted to an audio signal processing unit. The audio signal processing unit determines if the audio signal corresponds to a target location of the catheter tip, and transmits a notification signal to a user notification unit. An infusion of fluid or an audio emitting element can be used to generate the audio signal at the catheter tip.

18 Claims, 9 Drawing Sheets

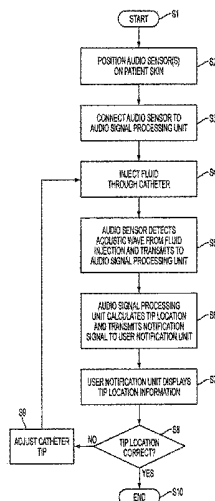

(56)

References Cited

U.S. PATENT DOCUMENTS

5,425,367 A * 6/1995 Shapiro A61B 5/06
128/899
5,526,820 A * 6/1996 Khoury A61B 5/0215
600/561
5,592,939 A * 1/1997 Martinelli A61B 34/20
128/899
5,622,169 A * 4/1997 Golden A61B 5/06
128/899
5,645,065 A * 7/1997 Shapiro A61B 5/06
128/899
5,666,958 A * 9/1997 Rothenberg A61N 1/056
439/909
5,727,552 A * 3/1998 Ryan A61N 1/372
128/899
5,727,553 A * 3/1998 Saad A61B 5/06
128/899
5,749,835 A * 5/1998 Glantz A61B 5/06
600/424
5,843,076 A * 12/1998 Webster, Jr. A61B 18/1492
600/439
6,409,674 B1 * 6/2002 Brockway A61B 5/0028
600/486
7,572,597 B2 * 8/2009 Lalvani G01N 33/505
424/248.1
7,909,772 B2 * 3/2011 Popov A61B 5/021
600/485
9,351,663 B2 * 5/2016 Ingold, Jr. A61B 5/061
9,752,914 B2 * 9/2017 Levine G01F 23/02
9,770,190 B2 * 9/2017 Herscovici-Cohen ... A61B 5/08

* cited by examiner

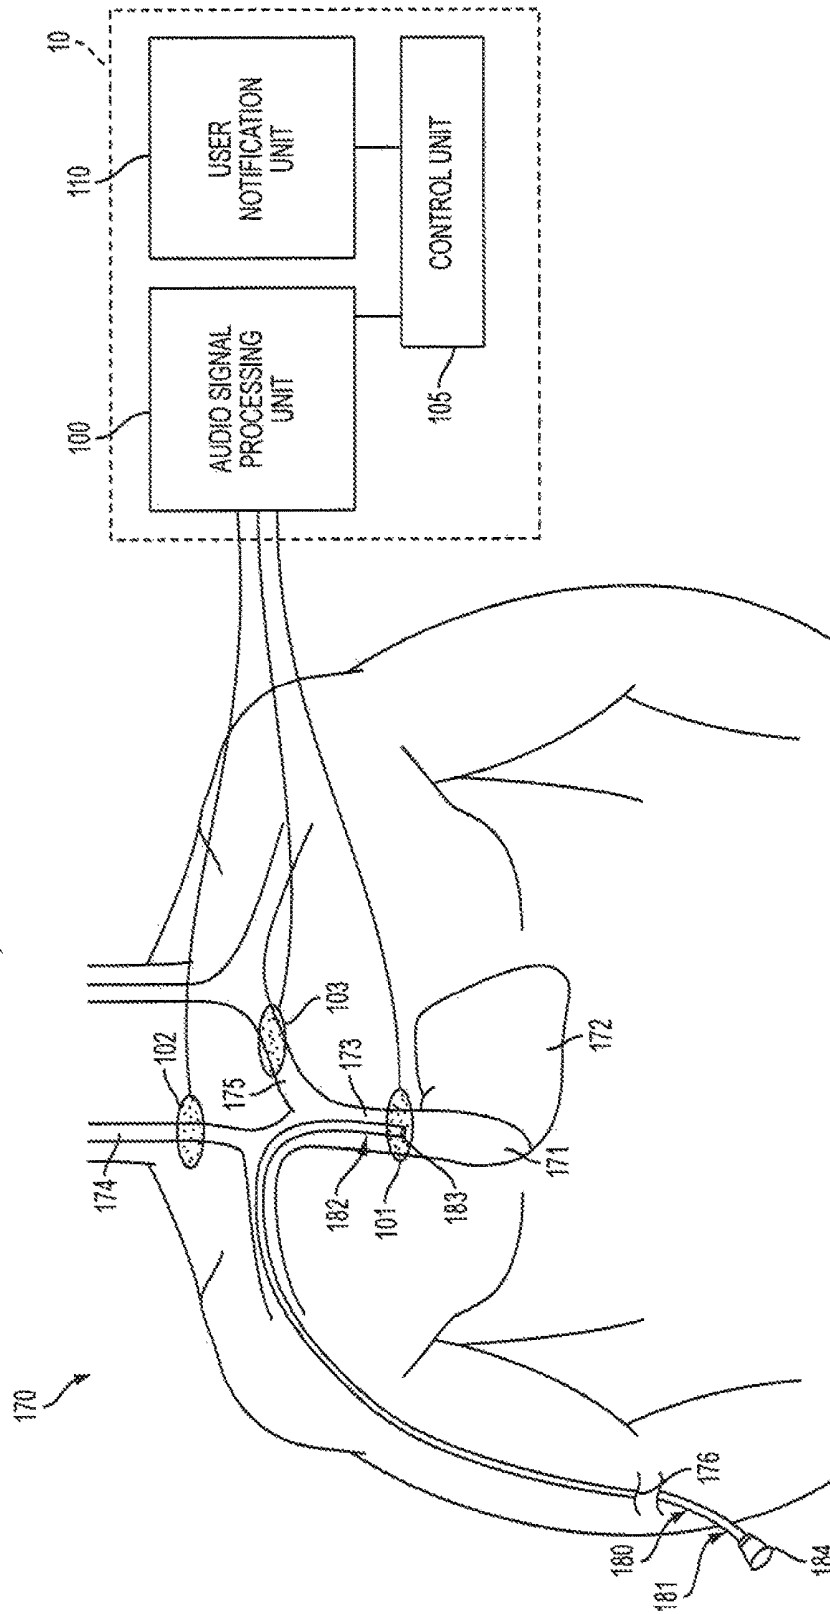


FIG. 1

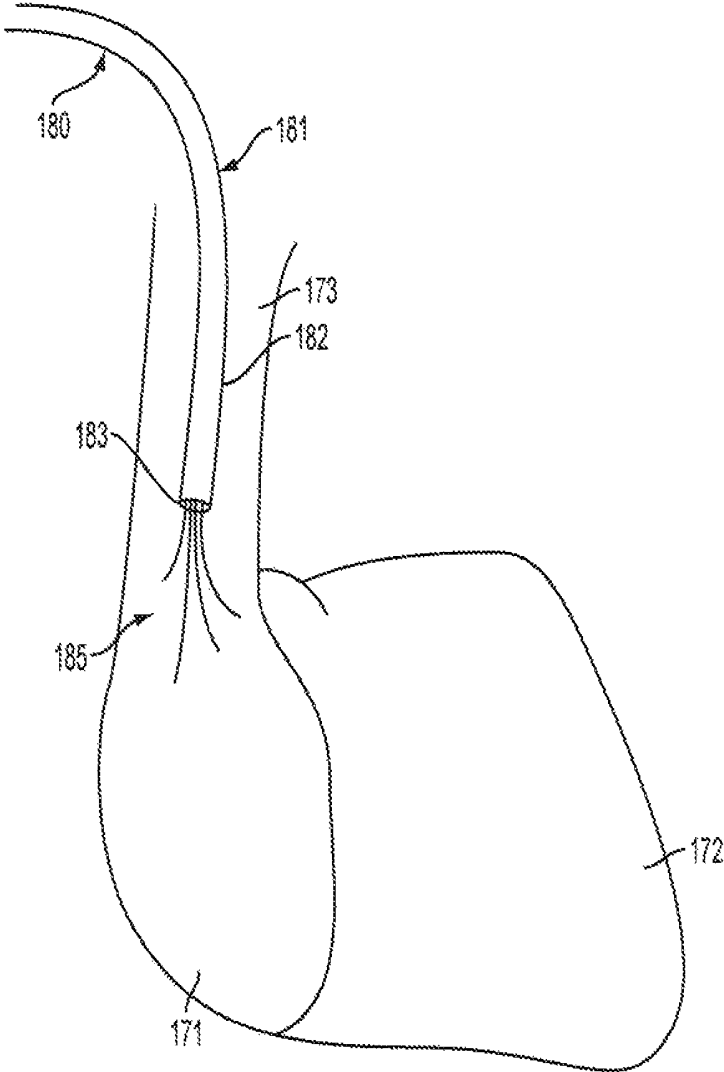


FIG. 2

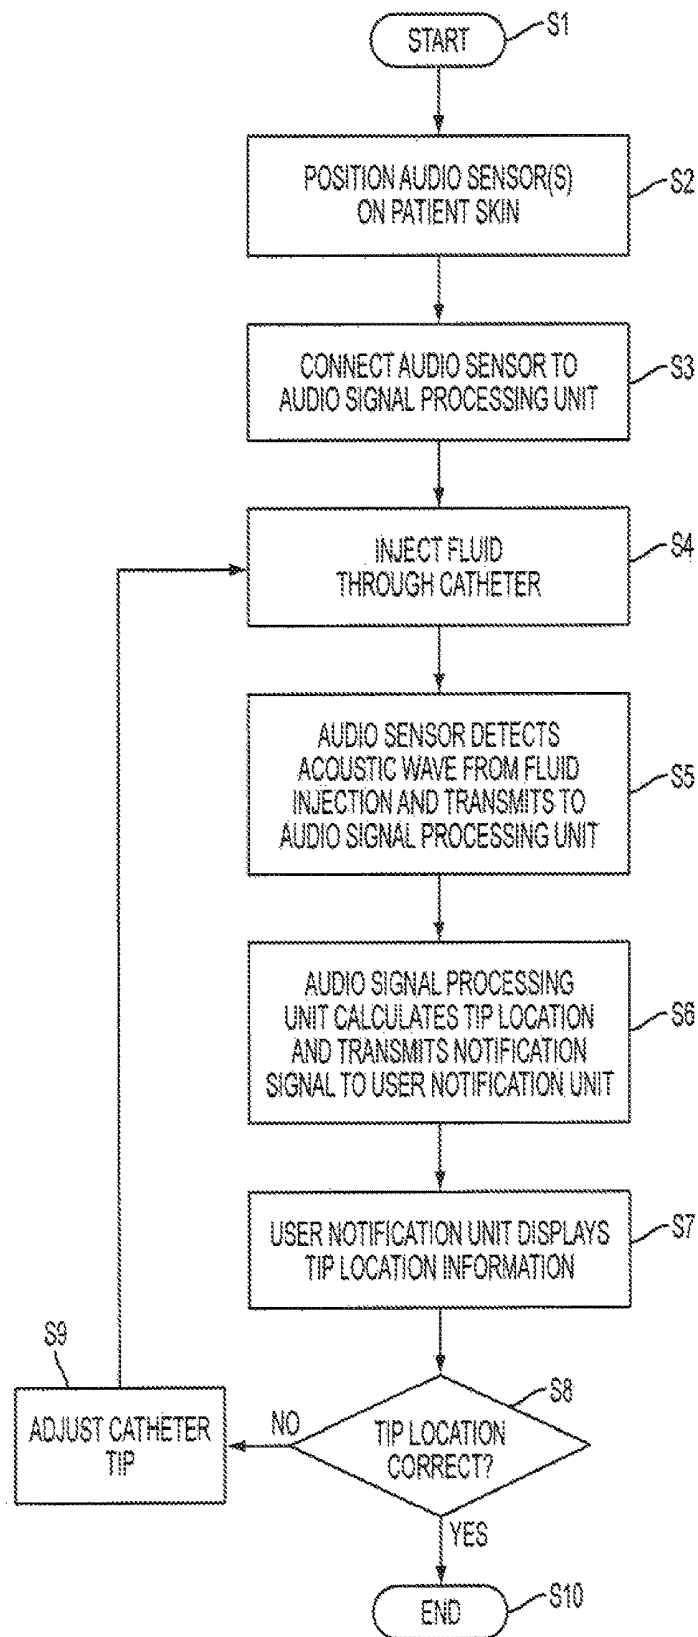


FIG. 3

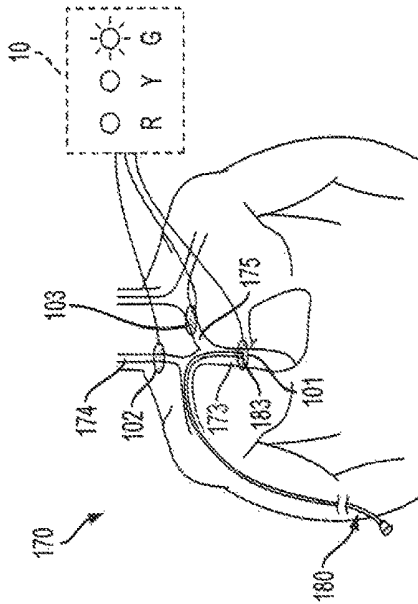


FIG. 4A

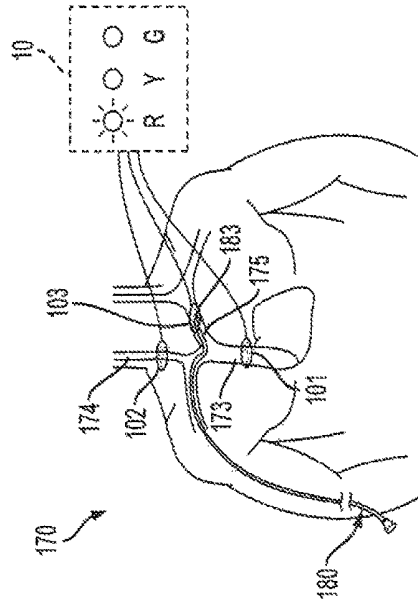


FIG. 4B

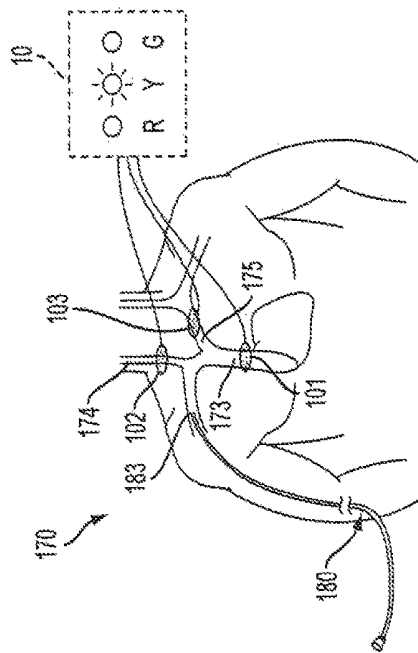


FIG. 4C

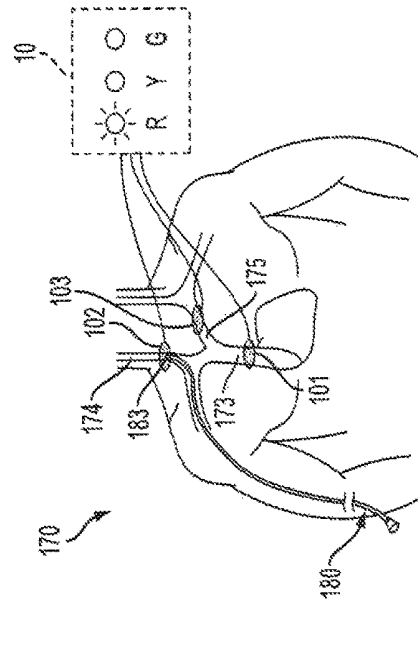


FIG. 4D

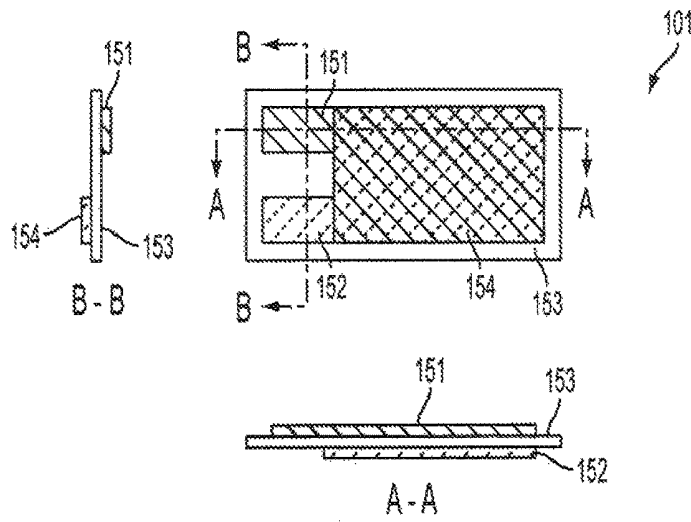


FIG. 5A

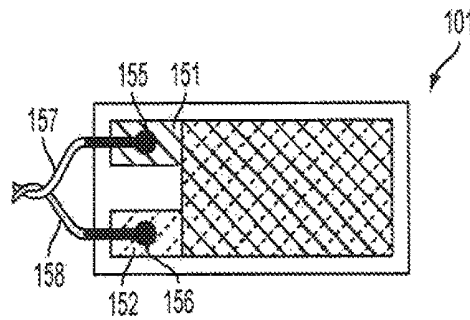


FIG. 5B

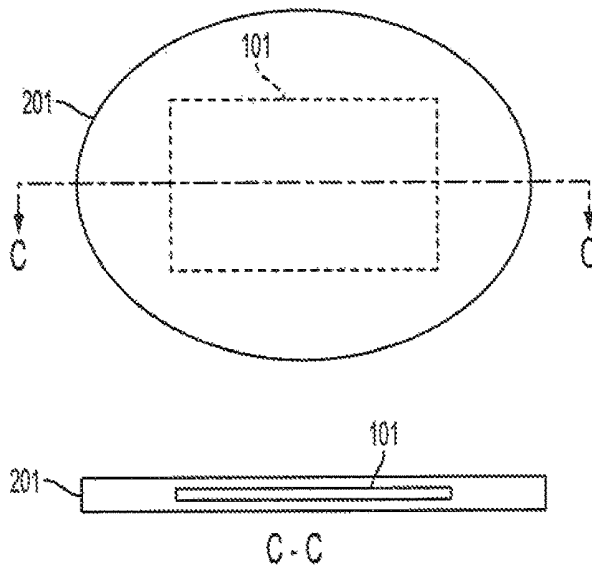


FIG. 5C

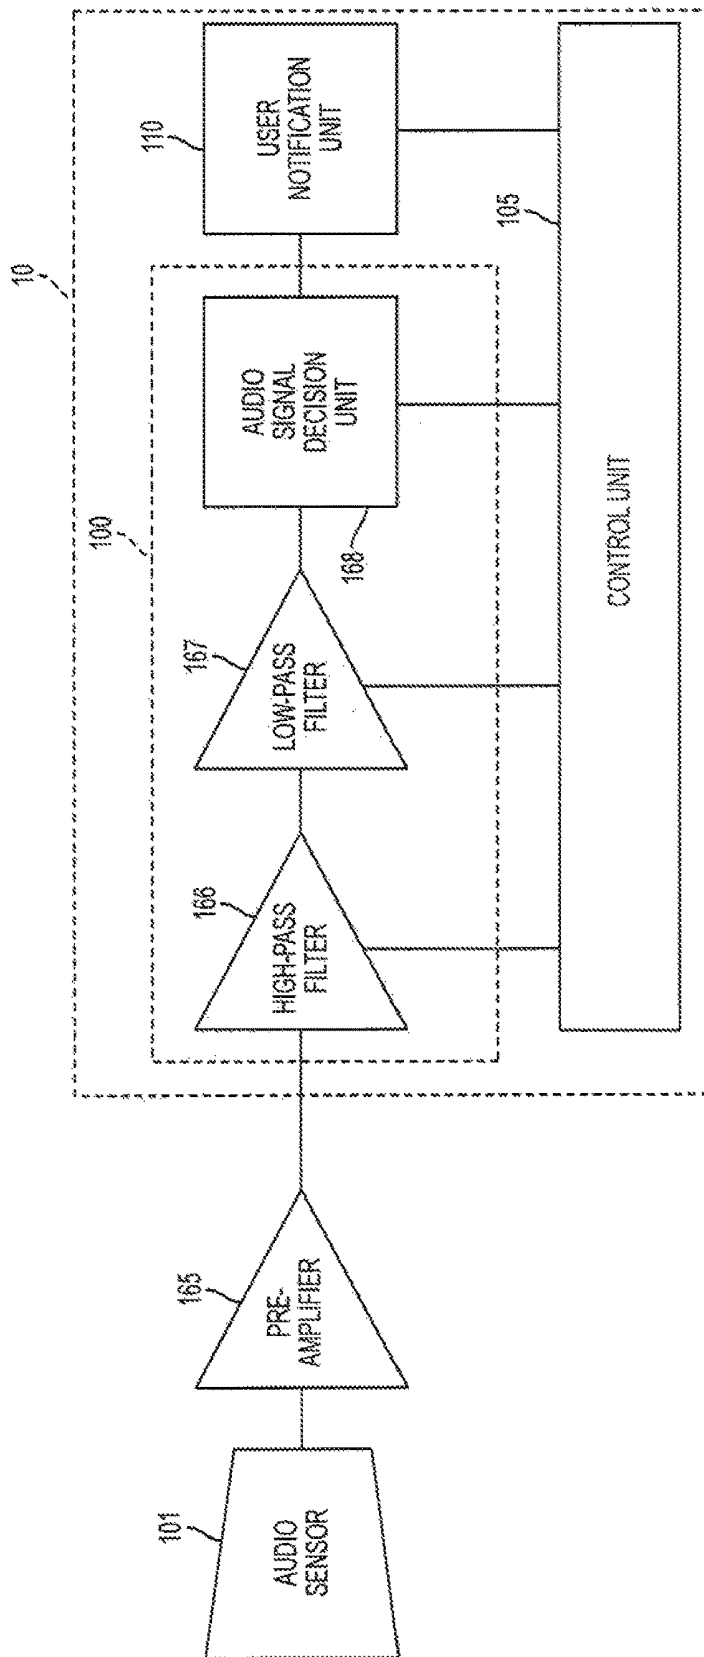


FIG. 6

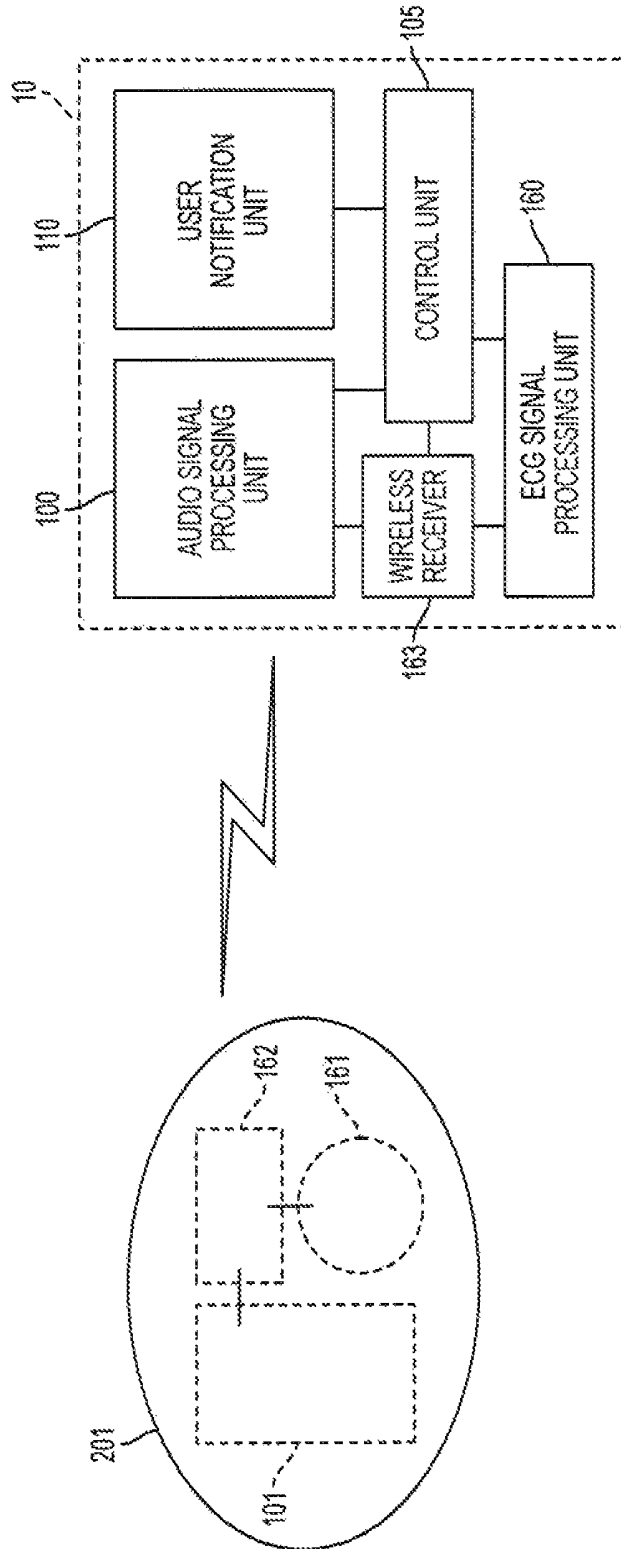


FIG. 7

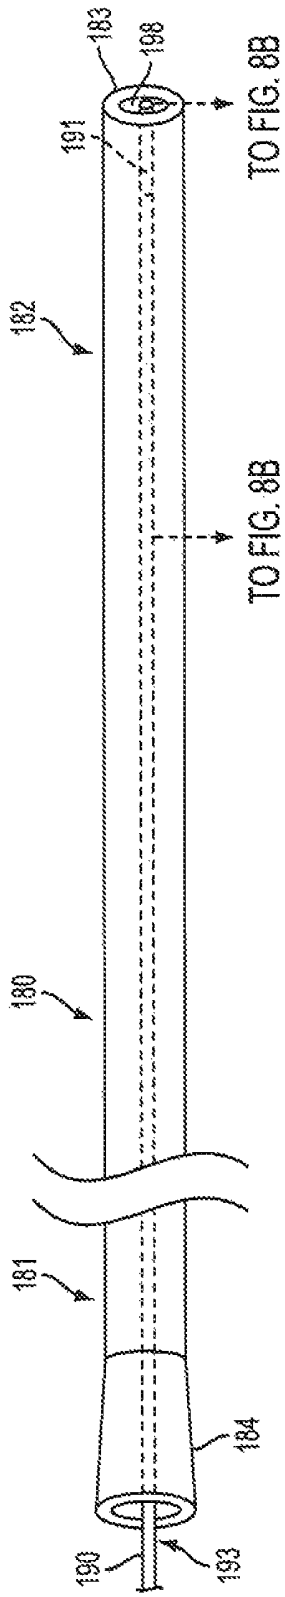


FIG. 8A

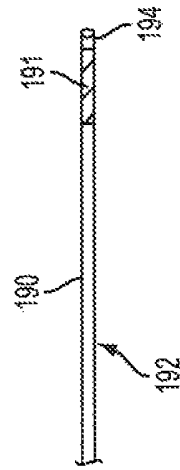


FIG. 8B

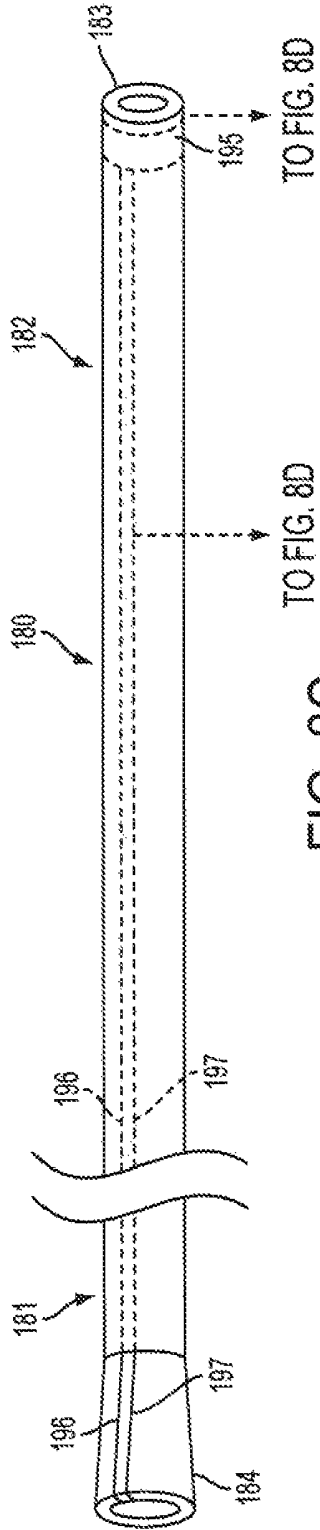


FIG. 8C

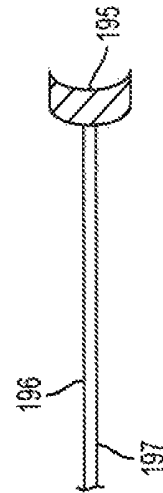


FIG. 8D

METHOD FOR LOCATING A CATHETER TIP USING AUDIO DETECTION

CROSS-REFERENCE TO RELATED APPLICATIONS

This application claims priority to U.S. provisional application No. 61/388,675 filed on Oct. 1, 2010 incorporated herein by reference in its entirety.

TECHNICAL FIELD

The present invention relates generally to a method for locating a catheter tip within a human body. More specifically, the invention relates to a method for locating a catheter tip by detecting audio signals emitted from the catheter tip, processing the detected audio signals, and verifying that the catheter tip is at the target location.

BACKGROUND OF THE INVENTION

Medical professionals commonly use catheters for gaining prolonged access to an area within the body. Once the catheter tip is positioned at the target location, treatments such as antibiotics, chemotherapy, pain medicine, and nutrition can be administered. However, if the catheter tip is improperly positioned during insertion, or if the catheter tip migrates out of position after insertion, various risks arise, including a fluid infusion that causes pain or injury to the patient, complications due to increased thrombosis rates, delays in therapy, catheter malfunction and additional costs.

The general standard for proper catheter insertion depends on the type of catheter and the type of treatment. For example, peripherally inserted central catheters (or PICC lines) are commonly inserted into a brachial, cephalic or basilic vein in the arm and advanced through the venous system towards the superior vena cava. Current medical standards recommended that the distal tip of the catheter terminate in the lower $\frac{1}{3}$ of the superior vena cava, close to the junction of the superior vena cava and the right atrium. However, since PICCs are commonly inserted into a vein in the arm and advanced through the venous system to reach the superior vena cava, the PICC line tip may be inadvertently positioned in a non-target area, such as the internal jugular or subclavian vein. Further, even if a PICC is properly inserted, the catheter tip could later shift out of position if for example the patient coughs violently, moves a lot, or experiences severe vomiting. Therefore, verifying that the catheter tip is in the correct location is essential for safe operation of the catheter.

Catheter tip location techniques have improved the ability of medical professionals to verify the location of the catheter tip. One technique uses fluoroscopy to confirm tip location. Fluoroscopy provides the operator with real-time images of the patient's anatomy using a fluoroscope. Another technique uses electromagnetic detection and a stylet having an electromagnetic sensor placed inside the lumen of the catheter tip. Electromagnetic systems use an external device positioned directly over the internal target area for generating a magnetic field outside of the body. The electromagnetic sensor on the stylet is then inserted into the body through the catheter lumen and measures when the magnetic flux is at its greatest. A monitor indicates to the user when the electromagnetic sensor on the stylet is centered underneath the external device. In a variation of this technique, the external device senses the electromagnetic field, and an element at the tip of the stylet generates the electromagnetic

field. Another technique uses ultrasound for guidance and determining catheter tip location. Electrocardiogram technology is also used to determine catheter tip location by measuring the change of the P wave as the catheter progresses down the superior vena cava.

However, the systems and techniques described above have numerous deficiencies. Fluoroscopy requires a facility with fluoroscopy machine, and poses x-ray risks for both the patient and the operator. Further, interpreting the image in fluoroscopy and ultrasound can be difficult, and requires special training. Electromagnetic detection requires a stylet having an electromagnetic detecting or emitting component, and measurement accuracy can be disrupted by electromagnetic interference. Further, for patients with pacemakers or skin disorders, or for patients that are obese, device operability may dramatically decrease or be contraindicated. Electrocardiogram detection requires a normal sinus rhythm, and cannot indicate when the catheter tip is in locations including the jugular vein and the subclavian. Additionally, the technology associated with the tip location systems mentioned above can be cost prohibitive, decreasing the number of facilities properly equipped to perform catheter insertion and maintenance procedures.

Therefore, a new method of locating a catheter tip within a human body is desired in order to overcome or minimize the deficiencies described above.

SUMMARY

The present invention is directed to a method of locating a catheter tip within a human body using audio detection.

In one embodiment, a method for locating a catheter tip within a human body includes positioning an audio sensor at a site on the human body and infusing fluid through an opening in the catheter tip. An audio signal is detected through and transmitted to an audio signal processing unit. The audio signal processing unit determines if the audio signal corresponds to a target location of the catheter tip, and transmits a notification signal to a user notification unit.

In another embodiment, a method for locating a catheter tip within a human body includes inserting a catheter into a hollow anatomical structure of the human body. The catheter includes an elongated body having a proximal end and a distal end terminating in a catheter tip, a lumen having an opening disposed at the distal end, and an audio emitting element configured at a distal portion of the elongated body. The catheter is advanced at least partially through the hollow anatomical structure. An audio sensor is positioned at a site on the human body. An audio beacon signal is emitted from the audio emitting element, and an audio signal is detected through the audio sensor and transmitted to the audio signal processing unit. The audio signal processing unit determines if the audio signal corresponds to a target location of the catheter tip, and transmits a notification signal to a user notification unit.

In another embodiment, a method for locating a catheter tip within a human body includes inserting a catheter into a hollow anatomical structure of the human body. The catheter includes an elongated body having a proximal end and a distal end terminating in a catheter tip, and a lumen having an opening disposed at the distal end. An audio emitting element is positioned at the catheter tip. The catheter is advanced at least partially through the hollow anatomical structure. An audio sensor is positioned at a site on the human body. An audio beacon signal is emitted from the audio emitting element and an audio signal is detected through the audio sensor and transmitted to an audio signal

processing unit. The audio signal processing unit determines if the first audio signal corresponds to a target location of the catheter tip, and transmits a notification signal to a user notification unit.

BRIEF DESCRIPTION OF THE DRAWINGS

The foregoing purposes and features, as well as other purposes and features, will become apparent with reference to the description and accompanying figures below, which are included to provide an understanding of the invention and constitute a part of the specification, in which like numerals represent like elements, and in which:

FIG. 1 is a view illustrating an application of the method according to an example embodiment of the present invention.

FIG. 2 is a cutaway view of a heart being accessed by a catheter infusing a fluid bolus.

FIG. 3 is a flow chart of the method according to an example embodiment of the present invention.

FIGS. 4A-4D show various catheter tip positions and a corresponding user console display according to an example embodiment. FIG. 4A shows a user console display when a catheter tip is positioned in a vein in the shoulder. FIG. 4B shows a user console display when a catheter tip is positioned in the lower $\frac{1}{3}$ of the superior vena cava. FIG. 4C shows a user console display when a catheter tip is positioned in the internal jugular vein. FIG. 4D shows a user console display when a catheter tip is positioned in the subclavian vein.

FIGS. 5A-5C show a piezo film audio sensor. FIG. 5A is a top view of a piezo film audio sensor, including cross-sectional views A-A and B-B. FIG. 5B is a top view of a piezo film audio sensor with lead attachments. FIG. 5C is a top view of an audio sensor within a protective layer, including cross-sectional views C-C.

FIG. 6 is a block diagram of audio signal processing according to an example embodiment.

FIG. 7 illustrates an electrocardiogram electrode and an audio sensor communicating wirelessly with a user console according to an example embodiment.

FIGS. 8A-8D show example embodiments of an audio emitting element located at the catheter tip. FIG. 8A is a side view of a catheter with a flexible elongated member having a piezo audio emitting element configured at the distal portion extended through a lumen in the catheter. FIG. 8B is a side view of the distal portion of the flexible elongated member having a piezo audio emitting element. FIG. 8C is a side view of a catheter having a piezo film audio emitting element configured at the distal portion. FIG. 8D is a side view of a piezo film element with communication elements extending proximally.

DETAILED DESCRIPTION OF THE INVENTION

The present invention can be understood more readily by reference to the following detailed description, the examples included therein, and to the Figures and their following description. The drawings, which are not necessarily to scale, depict selected preferred embodiments and are not intended to limit the scope of the invention. The detailed description illustrates by way of example, not by way of limitation, the principles of the invention. The skilled artisan will readily appreciate that the devices and methods described herein are merely examples and that variations can be made without departing from the spirit and scope of the

invention. It is also to be understood that the terminology used herein is for the purpose of describing particular embodiments only and is not intended to be limiting.

Referring now in detail to the drawings, in which like reference numerals indicate like parts or elements throughout the several views, in various embodiments, presented herein is a method for locating a catheter tip by audio detection.

FIG. 1 shows a human body 170 with a catheter 180 inserted at a site 176 in the right arm. The catheter 180 has a proximal portion 181 and a distal portion 182. In the present embodiment, the catheter 180 is a single lumen catheter, but it can have multiple lumens. The proximal portion 181 of the catheter 180 terminates at the luer 184. The distal portion 182 of the catheter 180 terminates in a catheter tip 183. As shown in FIG. 1, the catheter 180 can be advanced to a target location, such as the superior vena cava 173, or some other site within the human body 170, for delivery of fluids such as antibiotics, chemotherapy, pain medicine, nutrition or for withdrawing blood. The user console 10 is a device, such as a handheld tablet device, which houses the audio signal processing unit 100 and a user notification unit 110 for communicating with a user. Audio signals emitted from the catheter tip 183 are detected by one or more audio sensors 101, 102 or 103, transmitted to the audio signal processing unit 100, and processed for determining the location of a catheter tip 183. Once the catheter tip location is determined, the audio signal processing unit 100 sends a user notification signal to the control unit 105, which communicates with the user notification unit 110 to notify the user. The user notification unit 110 can utilize a visual display, a sound notification, or some combination of the two for communicating with the user.

As illustrated in FIG. 2 fluid can be rapidly injected into the lumen of catheter 180 and infused through an opening in the catheter tip 183. As the fluid 185 ejects through the opening, an audio frequency sound wave is generated. A fluid injection technique called push pause or push stop can be used to infuse fluid through the catheter 180. The push pause technique creates fluid turbulence at the catheter tip 183 generating an audio frequency sound wave. Increased fluid turbulence facilitates an increase in the intensity of the generated audio frequency sound wave. For example, a 10 mL syringe can be filled with 10 mL of saline and connected to the luer 184. Cycles of 2 mL of saline infused over 0.5 seconds followed by a 0.5 second pause can be repeated until the 10 mL of saline is fully infused. Other techniques for fluid infusion may be used according to the present invention so that an audio frequency signal capable of detection is generated at the catheter tip. Additionally, the viscosity of the fluid and the pressure applied to the syringe by the user can be manipulated to increase the flow rate of the fluid. An increased flow rate may also increase the intensity of the generated audio frequency sound wave, facilitating stronger detection signals.

Referring back to FIG. 1, the target location for the catheter tip 183 is just outside of the heart 172 in the lower $\frac{1}{3}$ of the superior vena cava 173. A first audio sensor 101 is placed on the anterior side of the body 170, positioned directly above the lower $\frac{1}{3}$ of the superior vena cava 173. When a saline bolus is flushed through the opening in the catheter tip 183, the first audio sensor 101 will detect and measure the emitted audio frequency signal. Utilizing only the first audio sensor 101, the audio signal processing unit 100 can indicate whether or not the catheter tip 183 is the lower $\frac{1}{3}$ of the superior vena cava. The determination can be made by implementing audio signal processing techniques

known in the art described in further detail below, including filtering the detected audio signal to detect the saline bolus, and comparing the intensity of the detected audio signal to a baseline signal or a predetermined threshold level.

In an alternative embodiment, a second audio sensor **102** is placed on the skin above the internal jugular vein **174**. If, for example, the catheter tip **183** is unintentionally advanced to the internal jugular vein **174**, the second audio sensor **102** will detect the audio signal emitted from the saline bolus. Additionally, an absent or weak audio signal will be detected by the first audio sensor **101**, since the audio signal will attenuate over distance. The absent or attenuated audio signal detected by the first audio sensor **101** is an indication that the catheter tip is in the wrong position. Additionally, if the catheter is fully inserted, the absence of a detected audio signal from both audio sensors could indicate that the catheter tip has advanced to the subclavian vein, a malfunction occurred in one of the sensors, or that the catheter is malfunctioning, blocking the saline bolus from infusing through the opening in the catheter tip.

In an alternative embodiment, a third audio sensor **103** is placed on the skin above the subclavian vein **175**. Thus, if the catheter tip **183** is unintentionally advanced to the subclavian vein **175**, or becomes mispositioned after insertion, the third audio sensor **103** will detect the audio signal from the saline bolus. Additionally, with respect to the first and second audio sensors, no audio signal, or a weak audio signal attenuated by distance may be detected. Further, when the catheter tip is positioned in a non-target location (e.g. the internal jugular vein or the subclavian vein), the addition of the third sensor provides the audio signal processing unit **100** with enough data for identifying specifically which non-target position the catheter tip is located in.

In an alternative embodiment, first and second audio sensors **101** and **102** can be strategically placed for comparing detected audio signals and localizing the position of the catheter tip **183**. For example, the right third intercostal space is commonly used by medical professionals as an external reference point for locating the superior vena cava **173**. Accordingly, a first audio sensor **101** can be positioned on the skin directly above the second intercostal space and a second audio sensor **102** can be positioned on the skin directly above the fourth intercostal space. The first and second audio sensors **101** and **102** should be in alignment with each other and consequently roughly equidistant from the third intercostal space. As the catheter tip **183** is advanced down the superior vena cava **173**, the intensity of the audio signal detected from the first audio sensor **101** will reach a maximum once the catheter tip **183** is directly under the second intercostal space. As the catheter **180** advances from the second intercostal space towards the third intercostal space, the intensity of the audio signal detected by the first audio sensor **101** will decrease as the intensity of the audio signal detected by the second audio sensor **102** increases. Eventually, the intensity of the signals detected by the first and second audio sensors **101** and **102** will equalize as the catheter tip **183** is centered directly below the third intercostal space. According to this alternative embodiment, the audio signal processing unit **100** can compare the first and second detected audio signals for localizing the catheter tip **183**.

In an alternative embodiment, a fourth audio sensor can be placed on the skin above a right portion of the subclavian vein. In some instances, the catheter tip **183** returns down the same path from which it was inserted, for example, in a right portion of the subclavian. This could happen if for example the patient moves a lot during insertion and the catheter tip

changes 180 degrees in direction, or the catheter tip become mispositioned after initial insertion. Thus, by placing a fourth audio sensor over a right portion of the subclavian, the audio signal processing unit **100** can detect the catheter tip **183** and alert the user.

Referring now to FIG. 3, a flow chart shows an example embodiment of the method according to the present invention. The patient may be undergoing a procedure for catheter insertion, or maintenance of a previously inserted catheter **S1**. At least one audio sensor **101** is placed above the patient's skin over the target area of the catheter tip **183 S2**. The audio sensor **101** is connected or synced to the audio signal processing unit **100 S3**. Fluid is injected through the catheter **180 S4** so that an audio frequency sound wave is generated at the catheter tip **183**. The audio sensor **101** will detect the audio frequency sound wave generated from the fluid infusion, and the detected audio signal will be transmitted to the audio signal processing unit **100 S5**. The audio signal processing unit **100** processes the detected audio signal and transmits a determination regarding tip location to the user notification unit **110 S6**. The user notification unit **110** displays the tip location determination to the user **S7**. If the tip location is in the target location **S8**, the process has ended **S10**, as the catheter tip **183** is determined to be in the target location. If the catheter tip **183** is in a non-target location, or if the tip location cannot be determined **S8**, the user adjusts the catheter tip **183 S9** and injects more fluid through the catheter **180 S4**. A new audio frequency sound wave generated from the fluid infusion is detected and transmitted to the audio signal processing unit **100 S5**. The audio signal processing unit **100** processes the new signal, sends the determination of tip location to the user notification unit **110 S6**, and communicates that determination to the user **S7**. If the tip is in the target location **S8**, the process ends **S10**. Otherwise, the user may repeat steps **S4** through **S9** multiple times until the catheter tip **183** is in the target location. Thus several advantages of one or more aspects according to this example embodiment are that the catheter tip of any catheter can be located, regardless of length, size or manufacturer. Further, there is no need for a separate stylet component, electromagnetic detecting or emitting components, or a patient with a normal sinus rhythm. In addition, the patient is not exposed to harmful radiation, and the operator does not need special training in interpreting x-ray or ultrasound images.

After the audio signal processing unit **100** determines whether or not the detected audio signal corresponds to the target catheter tip location, a notification signal is sent to a user notification unit **110**. The notification signal can be sent either directly to the user notification unit **110**, or sent to a control unit **105** that communicates with the user notification unit **110**. The user notification unit **110** can have a visual display for indicating when the catheter tip **183** is in proper position. FIGS. 4A-4D illustrate a user notification display on the user console **10** according to an example embodiment. Depending on the determination made by the audio signal processing unit **100**, the user notification unit **110** will display a red light indicating that the catheter tip **183** has been located and is not in the target location, a yellow light indicating that the catheter tip **183** has not been located, or a green light indicating that the catheter tip **183** has been located and is in the target location. Thus, as shown in FIG. 4A, if the catheter tip **183** is located too far away from any one of the sensors, an audio signal emitted from the saline bolus will not be detected, and the yellow light will activate. FIG. 4B shows the catheter tip **183** in the target location of the lower $\frac{1}{3}$ of the superior vena cava. The audio signal

processing unit **100** will verify that catheter tip in the proper location, thus activating the green light. FIGS. **4C** and **4D** show the catheter tip **183** after being mispositioned or migrating to the internal jugular vein **174** and the subclavian vein **175** respectively, activating the red light. The user notification signal can also take other forms, including an audio notification or a message display.

FIGS. **5A-5C** show an example embodiment of an audio sensor **101**. The audio sensor **101** can be any audio sensor or microphone element capable of detecting audio signals emitted from within the human body. In the present embodiment, the audio sensor is made of piezoelectric polyvinylidene fluoride polymer film (PVDF or piezo film). Piezo film is used for various acoustic applications, including contact microphones for detecting sounds emitted from within a human body. Piezo film is a flexible, lightweight, highly sensitive thin film capable of being used as an audio sensor. Piezo film is also immune to moisture, and requires no external power to function, unlike electrostatic types of audio sensors. FIG. **5A** shows an example embodiment of a piezo film audio sensor, with an upper electrode **151**, a lower electrode **152**, and a piece of piezo film **153** configured between the upper and lower electrodes. The electrodes are silver ink screen printed electrodes, which offer high conductivity, high flexibility and a thin profile. The upper electrode **151** and lower electrode **152** overlap at the active piezo film area **154**. When the piezo film **153** is stretched, an electrical signal is generated between the upper electrode **151** and lower electrode **152** surfaces at the active piezo film area **154**. The electrical signal is proportional to the amount of elongation of the piezo film **153**. The piezo film sensor may be combined with a low-noise electronic preamplifier, and designed to minimize external acoustic noise.

Transmission of detected audio signals to the audio signal processing unit **100** can be accomplished by either hard wired or wireless transmission. As shown in FIG. **5B**, lead attachments **155** and **156** can be configured on the upper electrode **151** and lower electrode **152** using a number of methods, including for example, eyelets, compression clamping, rivets, crimping, eyelet holes or low temperature solders. The example embodiment in FIG. **5B** shows first rivet **155** connecting a first wire **157** to the upper electrode **151** and a second rivet **156** connecting a second wire **158** to the lower electrode **152**. Lightweight shielded cable or twisted wire pairs can be used to connect the audio sensor **101** to the audio signal processing unit **100** while also reducing vulnerability from unwanted electromagnetic interference.

Now with reference to FIG. **5C**, the audio sensor **101** can be designed to vibrate the piezo film through a medium, such as a pad, protective coating or protective layer **201**. The protective layer **201** may be in direct physical contact with the skin when placed on the body. The protective layer **201** can be made of a material compatible for measuring the audio signal, for example, rubber, a polyester reinforcing member or a thin urethane layer. The protective layer can also be combined with an adhesive for mounting the audio sensor on or near a surface of the skin. Additionally, shielded and low-noise elements can be used to minimize the amount of ambient noise and interference detected by the audio sensor.

Referring to FIG. **6**, detected audio signals are transmitted to the audio signal processing unit **100** and processed for determining whether or not the catheter tip **183** is in the target location. In one example embodiment, the audio frequency range associated with the sound wave generated by a saline bolus is identified. A high-pass filter **166** and a

low-pass filter **167** are implemented to remove any frequencies outside of that range, such as audio frequencies detected from breathing, blood flow, body movement or ambient environmental noise. A preamplifier **165** can also be connected to the audio sensor to amplify the detected audio signal. Once frequencies outside of the desired frequency range are filtered out, an audio signal decision unit **168** determines if the remaining isolated frequencies representing the saline bolus are above a predetermined threshold.

The predetermined threshold can be set based on various factors corresponding with the catheter tip being located in the target location, including for example a comparison to a baseline audio signal. The baseline audio signal can be established by detecting an audio signal from the audio sensor before or after the saline bolus is injected. The detected baseline audio signal can be transmitted to the audio signal processing unit **100** and stored in memory. The baseline audio signal can also be manually programmed into the memory of the audio signal processing unit **100**. The above described technique audio signal processing is one of many known in the art, however, any compatible technique can be used according to the present invention.

Referring to FIG. **7**, in an alternative embodiment, an electrocardiogram electrode **161** can be incorporated into the protective layer **201** for tracking electrical activity of the heart. As already known in the art, electrocardiograms can be used for locating catheter tip locations near the heart by tracking the change of the P wave as the catheter is advanced from the upper $\frac{1}{3}$ of the superior vena cava down to through the lower $\frac{1}{3}$ of the superior vena cava, and into the right atrium **171**. The change in the P wave on an electrocardiogram monitor correlates to the position of the catheter tip, typically spiking as the catheter tip enters the right atrium **171**. The P wave is reduced as the catheter tip is pulled back from the entrance to the right atrium **171**. Thus, the reduced P wave should indicate that the catheter tip is terminated at the junction of the right atrium and the superior vena cava. In the present embodiment, an electrocardiogram electrode **161** is positioned in the protective layer **201** next to the first audio sensor **101**. The electrocardiogram electrode **161** transmits detected electrocardiogram signals to the electrocardiogram signal processing unit **160**. The signal is processed and a control unit **105** can verify that the catheter tip location determined by the audio signal processing unit **100** is consistent with the catheter tip location determined by the electrocardiogram signal processing unit **160**. Transmission of the electrocardiogram signal and detected audio signal can be by a wireless transmitter **162**. The wireless transmitter **162** can be built into the protective layer **201** and can communicate with a wireless receiver **163** built into the user console **10**. The electrocardiogram electrode **161** can also detect a signal before or after the saline bolus is administered for monitoring the heartbeat or establishing an electrocardiogram baseline.

The user console **10** can be a stationary unit, or a mobile unit such as handheld device. Further, the audio signal processing unit **100**, control unit **105**, user notification unit **110** and electrocardiogram signal processing unit **115** can be implemented in hardware, software, or some combination. For example, in a wireless transmission embodiment, the user console **10** is a handheld tablet device, and the audio sensors transmit the measured audio signals to the handheld tablet device using a wireless protocol such as Bluetooth. The user notification unit **110** could incorporate the display of handheld tablet device to communicate with the user.

Although a saline bolus has been used in example embodiments, the present invention is not limited to requir-

ing a saline bolus. Any fluid infused from a catheter tip will generate an audio signal. Other fluids may include heparin based solutions, including for example Lactated Ringer's solution and Hartmann's Solution. With respect to infusion rates, although a bolus or rapid infusion of fluid will improve clarity of the detected audio signal, infusion rates may vary depending on various factors including the pickup ability of the audio sensors. Further, the audio signal processing unit **100** can be programed to compensate for changes in fluids and infusion rates.

In an alternative embodiment, a method for locating a catheter tip **183** using audio detection uses an audio emitting element positioned at the catheter tip **183**, thus no fluid infusion is required. In an example embodiment shown in FIGS. **8A** and **8B**, a flexible elongated member **190** has a proximal portion **193** and distal portion **192**, terminating in a tip **194** at the distal portion **192**. Proximate to the tip **194** is an audio emitting element **191**, such as a piezo crystal or a piece of piezo film. The flexible elongated member **190** can be made of a medical grade flexible material having a diameter smaller than the diameter of the lumen **198** in the catheter **180**. The regions along the flexible elongated member **190** can vary in stiffness, depending on the application. The flexible elongated member **190** may also be made from a guide wire like material. According to the present embodiment, the user console **10** can communicate with the audio emitting element **191** through communication elements such as conductive wire or ink that extend through the flexible elongated member **190**. The communication elements can extend to the proximal portion **193** of the flexible elongated member **190**, and can be connected to an audio signal generating unit in the user console **10**. The audio signal generating unit can set the audio emitting element **191** to emit an audio beacon signal at a frequency distinct from the audio frequencies of ambient noise. For example, consideration should be given to blood flow, breathing, bodily movements and ambient environmental noise. Consideration should also be given to audio sensor position and the impact that anatomical factors such as body density and bone structure will have on detection of particular beacon frequencies. According to this method, the location of any catheter tip can be located, regardless of length, size or manufacturer.

Alternatively, the sound emitting element can be attached to the catheter. In the example embodiment shown in FIGS. **8C** and **8D**, an audio emitting element **195** such as piezo film is attached to or embedded in a wall of the catheter distal end portion **182**. A first and second elongated transmission element **196** and **197** extend from the sound emitting element proximally through the catheter wall exiting the catheter at its proximal end. The exposed communication elements at the luer **184** can be connected to an audio signal generating unit in the user console **10**. The user console **10** can thus communicate with the audio emitting element **195** to set an audio beacon signal at a distinct audio frequency. According to these methods for locating the catheter tip, a saline bolus or infusion of fluid from the catheter tip is not required, since the sound emitting element acts as a beacon for the audio sensors. Further, the location of a catheter tip can be determined on initial placement and subsequent maintenance, and does not require a separately stocked stylet component.

Some or all of the components mentioned above could be included in a kit. The kit may include a user console, audio sensors, wired or wireless signal transmission elements, and

instructions for use. The kit may also include PICC catheters with or without an audio emitting element, and a stylet with an audio emitting element.

Although it is common to have the catheter tip terminate in a lower $\frac{1}{3}$ of the superior vena cava, or at the junction of the superior vena cava and the right atrium, the method according to the present invention can be used for procedures that target any site within the body. Further, any type of catheter tip can be located, including acute and chronic dialysis catheters, subcutaneous port catheters, and central venous catheters. In addition, access sites do not need to be in the arm. For example, for a patient with amputated arms, the access site may be in the groin or in the back.

What is claimed is:

1. A method for locating a catheter tip within a human body comprising:

positioning a first audio sensor at a first site, infusing fluid through an opening in the catheter tip, the infusion of fluid creating a first audio signal, detecting the first audio signal through the first audio sensor, transmitting the first audio signal wirelessly from the first audio sensor to an audio signal processing unit, and displaying a notification signal from the audio signal processing unit on a user console.

2. The method of claim 1, wherein the first site is located substantially over a lower $\frac{1}{3}$ of a superior vena cava of the human body.

3. The method of claim 1, wherein the first audio sensor comprises a piezo film element.

4. The method of claim 1, further comprising: detecting a first baseline audio signal through the first audio sensor, transmitting the first baseline audio signal wirelessly from the first audio sensor to the audio signal processing unit, and comparing the first baseline audio signal to the first audio signal using the audio signal processing unit.

5. The method of claim 1, further comprising: detecting a first electrocardiogram signal through a first electrocardiogram electrode, and transmitting the first electrocardiogram signal wirelessly from the first electrocardiogram electrode to an electrocardiogram signal processing unit.

6. The method of claim 5, wherein the first audio sensor and the first electrocardiogram electrode are operably connected to a first pad member, and wherein the first pad member is positioned at the first site.

7. The method of claim 5, further comprising: detecting a first baseline electrocardiogram signal through the first electrocardiogram sensor, transmitting the first baseline electrocardiogram signal wirelessly from the first electrocardiogram sensor to the electrocardiogram signal processing unit, and comparing the first baseline electrocardiogram signal to the first electrocardiogram signal using the electrocardiogram signal processing unit.

8. The method of claim 1, wherein the fluid is a saline bolus.

9. The method of claim 1, further comprising: positioning a second audio sensor at a second site, detecting a second audio signal through the second audio sensor, and transmitting the second audio signal wirelessly from the second audio sensor to the audio signal processing unit.

11

10. The method of claim 9, wherein the second site is located substantially over an internal jugular vein.

11. The method of claim 9, further comprising:

detecting a second baseline audio signal through the second audio sensor,

transmitting the second baseline audio signal wirelessly from the second audio sensor to the audio signal processing unit, and

comparing the second baseline audio signal to the second audio signal using the audio signal processing unit.

12. The method of claim 9, wherein the first site and the second site are located on opposite sides of a third intercostal space.

13. The method of claim 9, further comprising:

detecting a second electrocardiogram signal through a second electrocardiogram electrode, and

transmitting the second electrocardiogram signal wirelessly from the second electrocardiogram electrode to an electrocardiogram signal processing unit.

14. The method of claim 13, wherein the second audio sensor and the second electrocardiogram electrode are operably connected to a second pad member, and wherein the second pad member is positioned at the second site.

12

15. The method of claim 13, further comprising: detecting a second baseline electrocardiogram signal through the second electrocardiogram sensor,

transmitting the second baseline electrocardiogram signal wirelessly from the second electrocardiogram sensor to the electrocardiogram signal processing unit, and

comparing the second baseline electrocardiogram signal to the second electrocardiogram signal using the electrocardiogram signal processing unit.

16. The method of claim 9, further comprising:

positioning a third audio sensor at a third site,

detecting a third audio signal through the third audio sensor, and

transmitting the third audio signal wirelessly from the third audio sensor to the audio signal processing unit.

17. The method of claim 16, wherein the third site is located substantially over a subclavian vein.

18. The method of claim 16, further comprising:

detecting a third baseline audio signal through the third audio sensor,

transmitting the third baseline audio signal wirelessly from the third audio sensor to the audio signal processing unit, and

comparing the third baseline audio signal to the third audio signal using the audio signal processing unit.

* * * * *

专利名称(译)	使用音频检测定位导管尖端的方法		
公开(公告)号	US10159460	公开(公告)日	2018-12-25
申请号	US15/165770	申请日	2016-05-26
申请(专利权)人(译)	ANGIODYNAMICS INC.		
当前申请(专利权)人(译)	ANGIODYNAMICS INC.		
[标]发明人	INGOLD JR JAMES E CASEY II THOMAS VINCENT NENTWICK BRIAN F		
发明人	INGOLD, JR., JAMES E. CASEY, II, THOMAS VINCENT NENTWICK, BRIAN F.		
IPC分类号	A61B5/00 A61M25/01 A61B7/04 A61B5/0402 A61B5/0205 A61B5/06 A61B8/08 A61B34/20		
CPC分类号	A61B8/0841 A61B5/0205 A61B5/0402 A61B5/061 A61M25/0108 A61B7/04 A61M2205/0294 A61B2034/2063 A61B2562/0204 A61M2025/0166		
其他公开文献	US20160270759A1		
外部链接	Espacenet		

摘要(译)

公开了一种用于将导管尖端定位在人体内的方法。音频传感器位于人体上的一个位置。音频信号由音频传感器检测，并发送到音频信号处理单元。音频信号处理单元确定音频信号是否对应于导管尖端的目标位置，并将通知信号发送到用户通知单元。输注流体或音频发射元件可用于在导管尖端处产生音频信号。

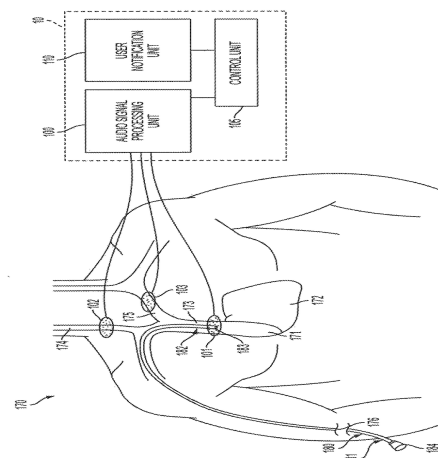


FIG. 1