



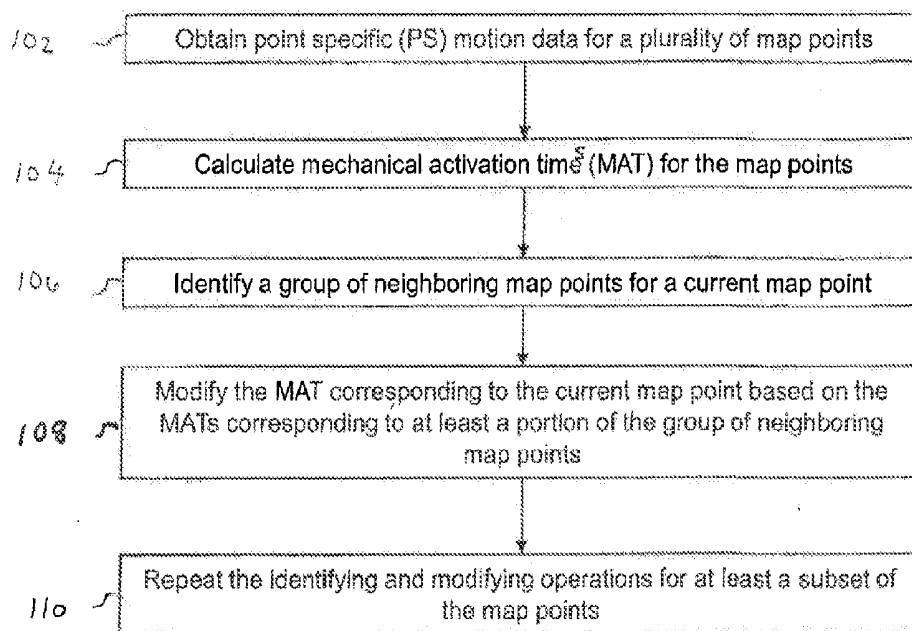


Fig. 1

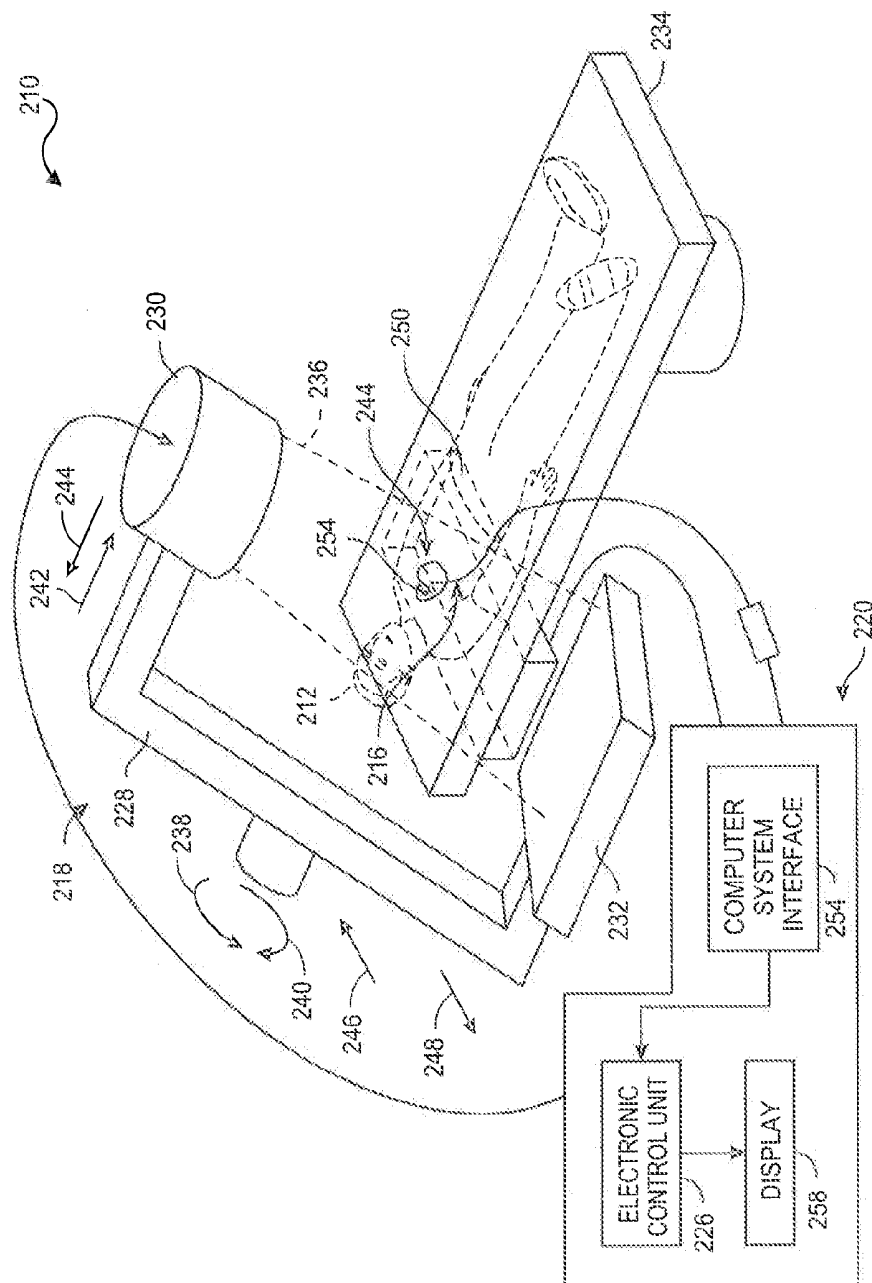


FIG. 2

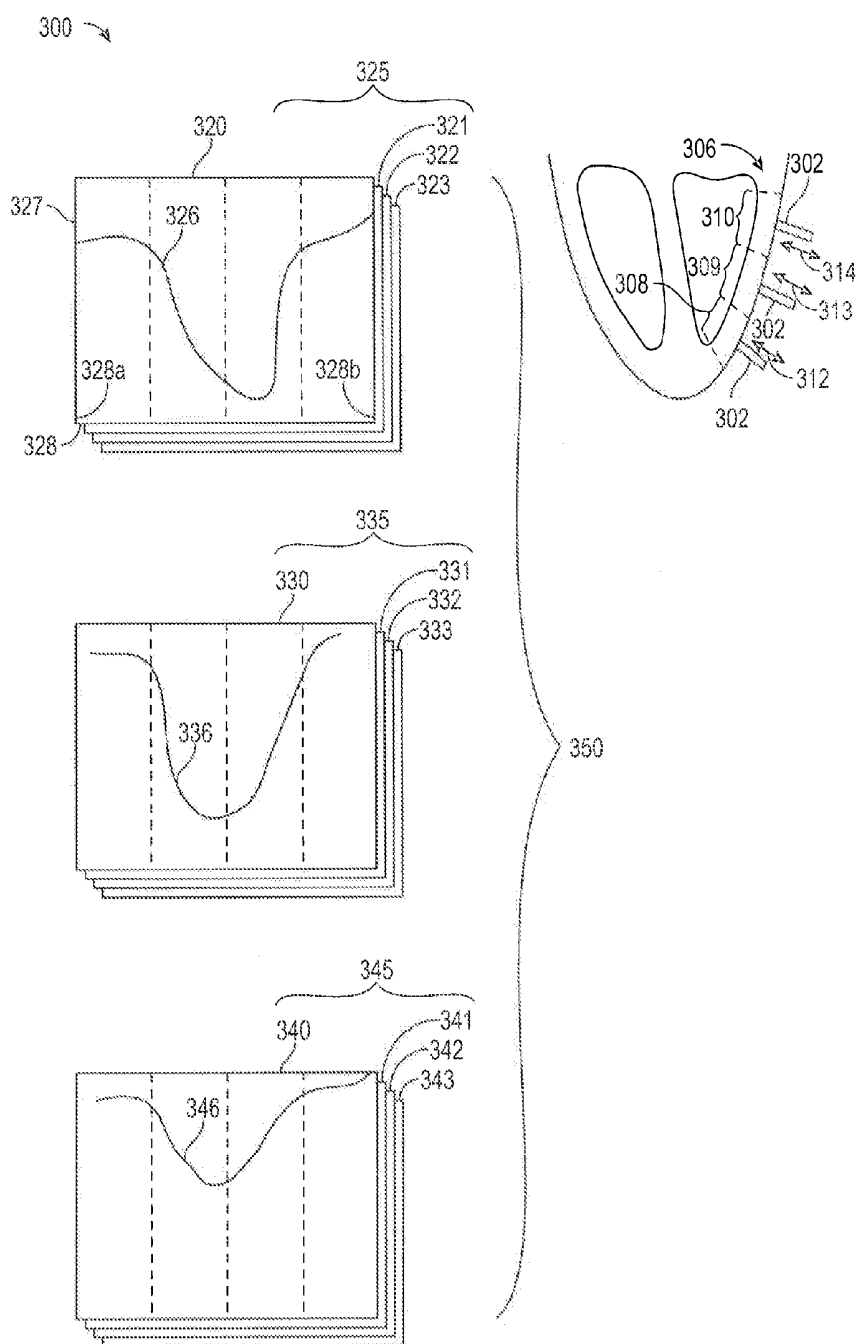


FIG. 3

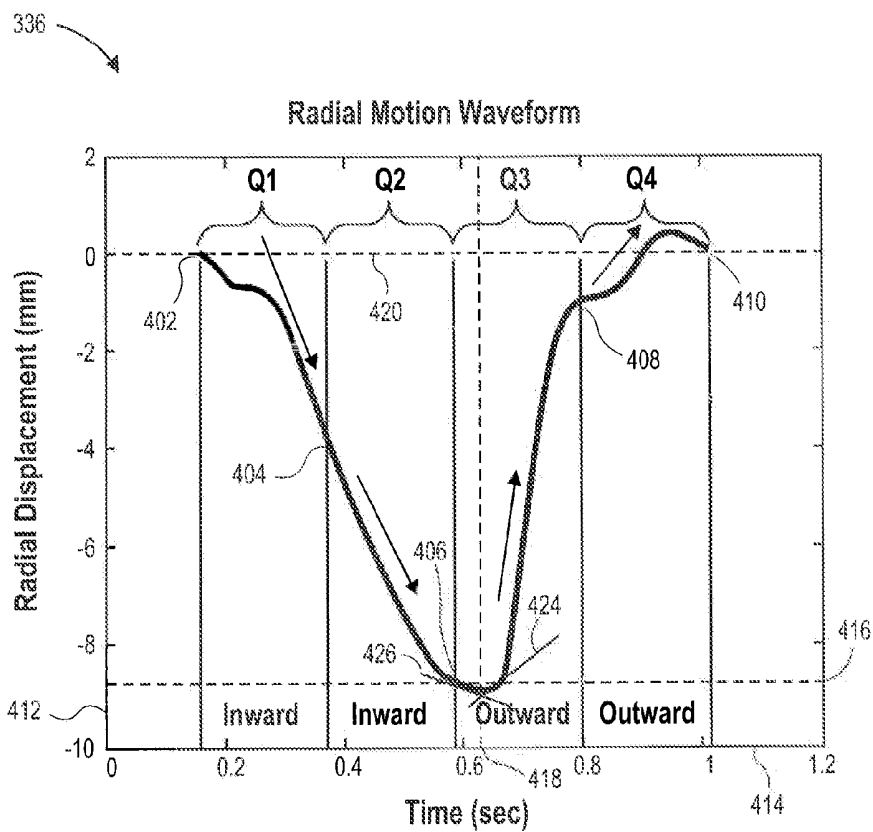


FIG. 4


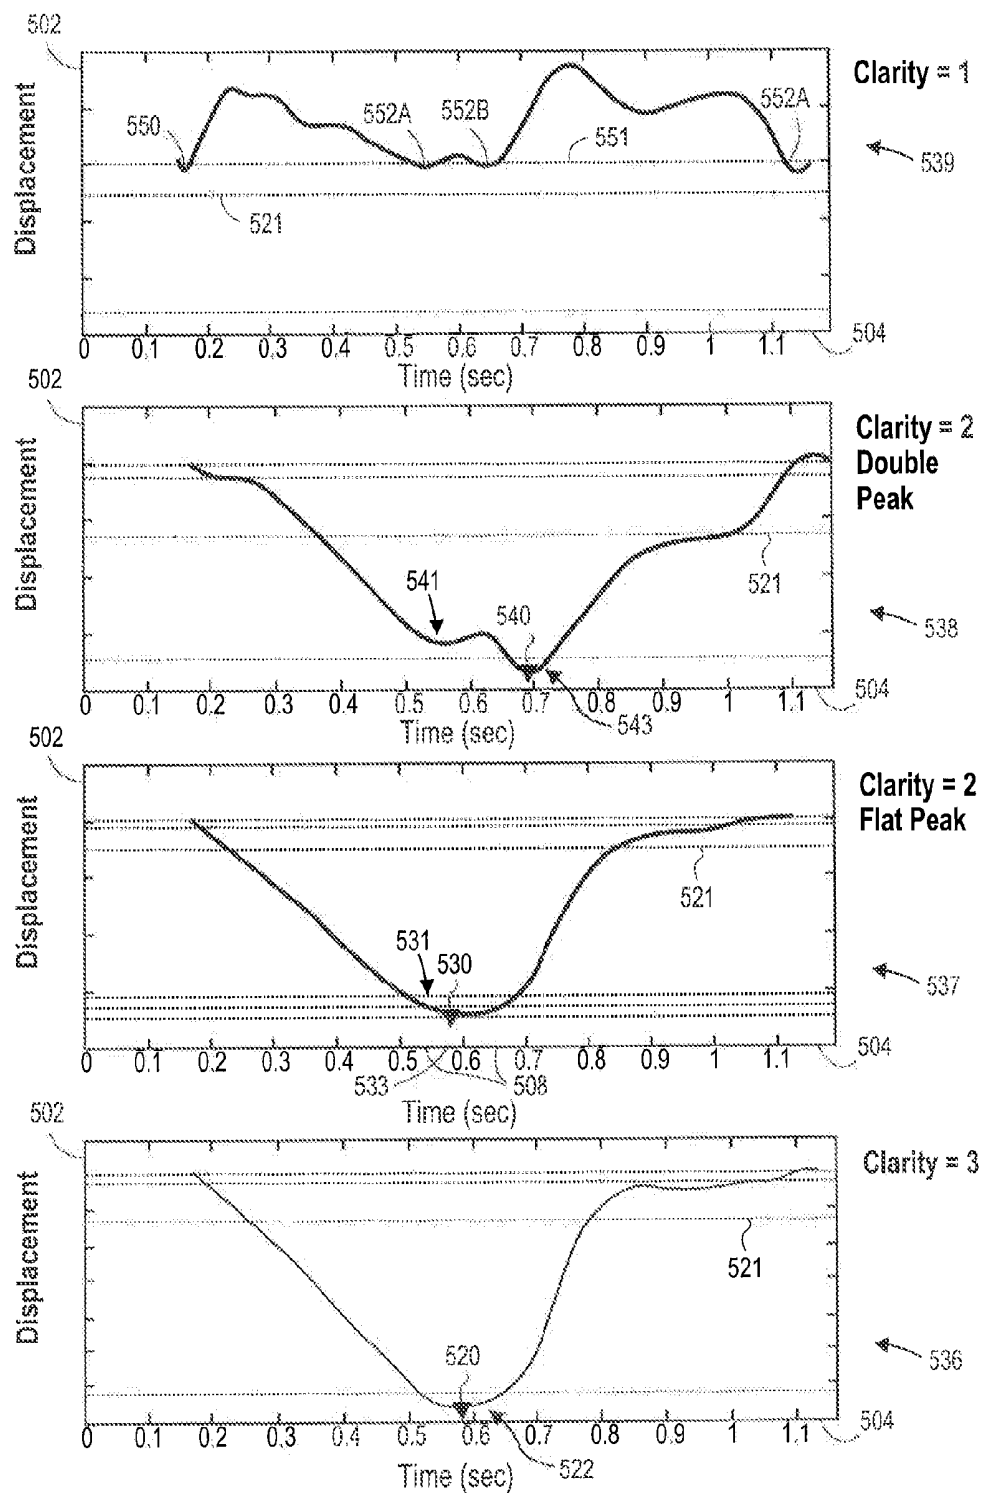


FIG. 5

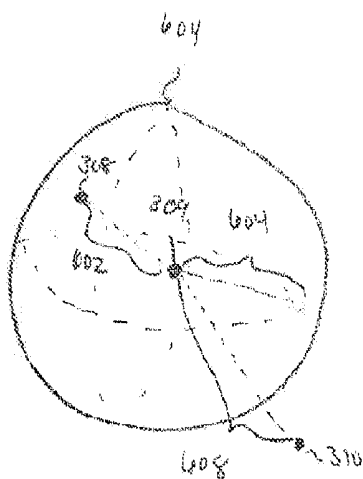

5.6

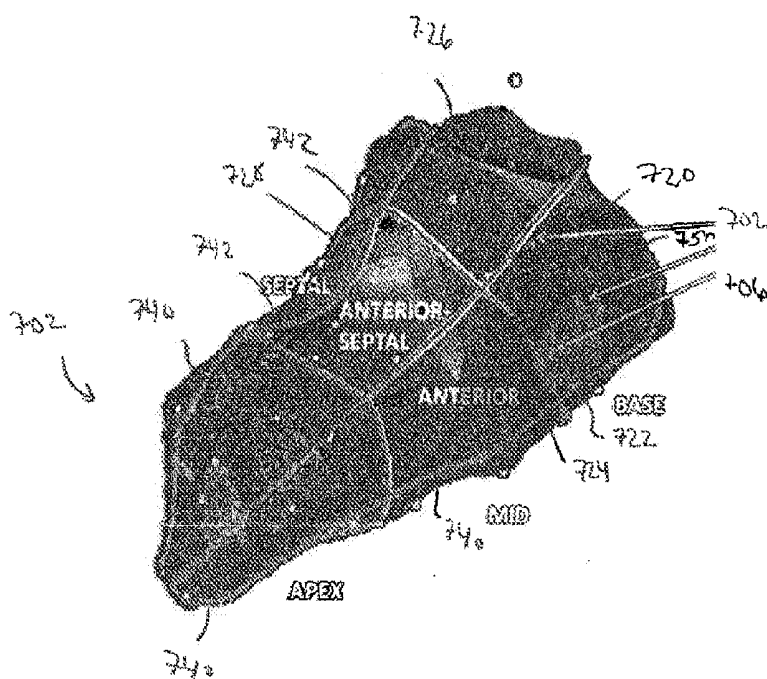


Fig. 7

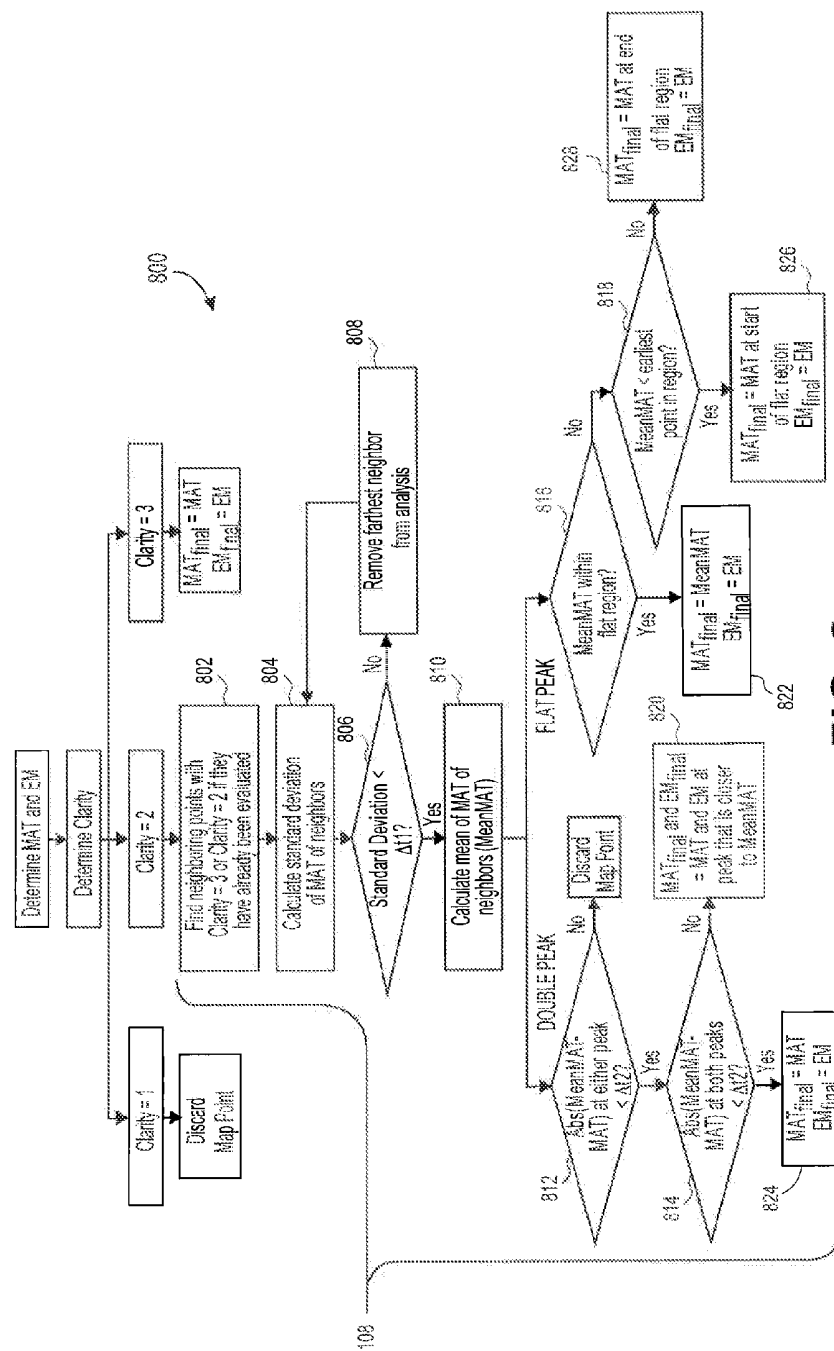


FIG. 8



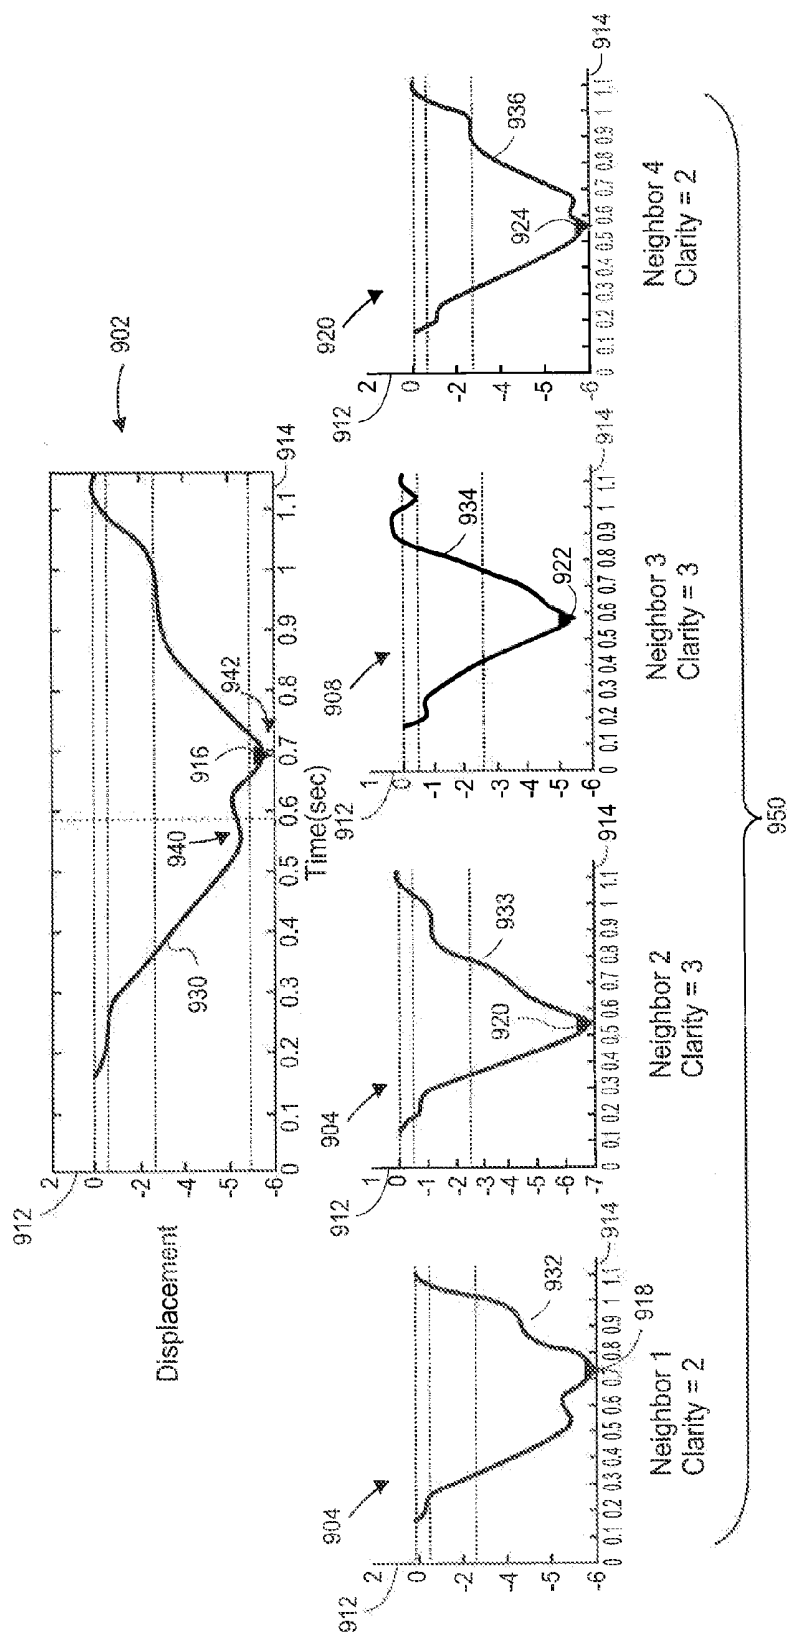


FIG. 9

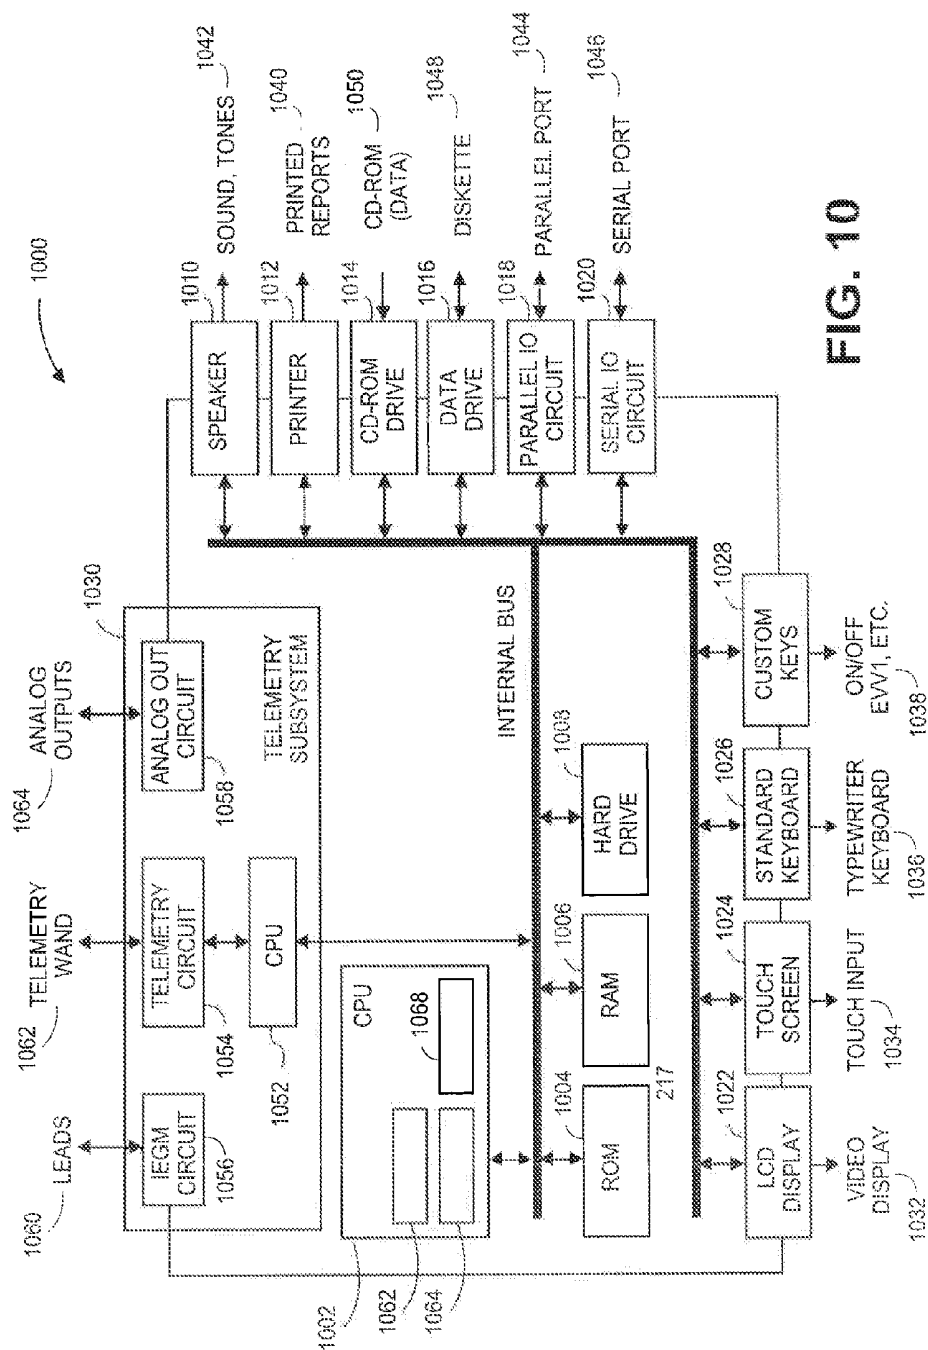


FIG. 10

## METHOD AND SYSTEM TO CHARACTERIZE MOTION DATA BASED ON NEIGHBORING MAP POINTS

### RELATED APPLICATION DATA

**[0001]** The present application is related to the following applications: U.S. provisional application Ser. No. 61/906,311, filed Nov. 19, 2013, titled "METHOD AND SYSTEM TO ASSESS MECHANICAL DYSSYNCHRONY BASED ON MOTION DATA COLLECTED BY A NAVIGATION SYSTEM" having docket number A13P3017, U.S. provisional application Ser. No. 61/910,630, filed Nov. 19, 2013, titled "METHOD TO MEASURE CARDIAC MOTION USING A CARDIOVASCULAR NAVIGATION SYSTEM" having docket number A13P3015, U.S. provisional application Ser. No. 61/906,305, filed Nov. 19, 2013, titled "METHOD TO IDENTIFY CARDIAC CYCLES WITH CONSISTENT ELECTRICAL RHYTHM AND MECHANICAL BEHAVIOR FOR COMPILATION INTO A REPRESENTATIVE CHARACTERIZATION OF CARDIAC MOTION" having docket number A13P3016, U.S. patent application titled "METHOD AND SYSTEM FOR CALCULATING STRAIN FROM CHARACTERIZATION DATA OF A CARDIAC CHAMBER" having docket number A14P3010, which is filed on or about the same day as the present application, U.S. patent application titled "METHOD AND SYSTEM FOR DISPLAYING A THREE DIMENSIONAL VISUALIZATION OF CARDIAC MOTION" having docket number A14P3008, which is filed on or about the same day as the present application, and U.S. patent application titled "METHOD AND SYSTEM TO AUTOMATICALLY ASSIGN MAP POINTS TO ANATOMICAL SEGMENTS" having docket number A14P3011, which is filed on or about the same day as the present application, all of which are expressly incorporated herein by reference in their entirety.

### BACKGROUND OF THE INVENTION

**[0002]** Embodiments of the present invention generally relate to methods and systems for cardiovascular navigation, and more particularly for characterizing motion in a cardiac chamber or organ.

**[0003]** Cardiovascular navigation systems (CNS) provide real-time position and orientation information in relation to a part of the cardiovascular system, such as, the heart based on sensors placed at various locations within the cardiovascular system. The CNS may be integrated with a fluoroscopic (or other diagnostic) imaging system and track the sensors continuously within an imaging volume defined by the fluoroscopic system, on both live and recorded background diagnostic images.

**[0004]** Recently, it has been proposed to utilize the CNS to evaluate the motion of the heart and identify a desired (e.g., optimal) location for placement of a left ventricular (LV) lead. For example, the CNS may systematically record information, such as displacement of the sensors, associated with various endocardial and epicardial locations of the LV. Depending on the size of the heart and other factors during the procedure, there may be between 40 and 120 endocardial LV locations and up to 10 epicardial locations at which the CNS obtains recordings for each patient.

**[0005]** Systems have been proposed to characterize the motion of the heart, based on mechanical activation that is

determined from sensor information at various endocardial and epicardial locations. The mechanical activation is used to measure the maximum extent of motion of the heart. However, the sensor information may include a complex pattern with multiple displacement apexes or peaks making determination of the mechanical activation point difficult. A need exists for improved methods and systems that utilize cardiovascular navigation systems for characterizing motion data having complex patterns.

### SUMMARY

**[0006]** In accordance with an embodiment herein, a method is provided for characterizing motion data. The method includes obtaining point specific (PS) motion data for a plurality of map points. The PS motion data indicates an amount of motion that occurred at the corresponding map point on a wall of the heart during at least one cardiac cycle. The method also includes, calculating mechanical activation times (MAT) for the map points, identifying a group of neighbor map points for a current map point, and modifying the MAT corresponding to the current map point based on the MATs corresponding to at least a portion of the group of neighboring map points. Further, the method repeats the identifying and modifying operations for at least a subset of the map points.

**[0007]** Optionally, the PS motion data defines a motion waveform at the corresponding map point. The motion waveform represent displacement over a select period of time, such that, the calculating operation above that calculates the MATs is based on the motion waveforms. Further, the method may include assigning clarity scores to each of the motion waveforms based on a distinctiveness of a feature of interest within the motion waveforms used to determine the MATs. The clarity scores represent confidence levels in the corresponding MATs.

**[0008]** In an embodiment, a system for characterizing motion data collected by cardiovascular navigation system (CNS). The system including a plurality of physiological sensors. The physiological sensors are positioned adjacent to a plurality of map points and acquire point specific (PS) motion data at corresponding map points. The PS motion data indicates an amount of motion that occurred at the map points on a wall of the heart during at least one cardiac cycle. The system includes a PS motion data analysis circuit module. The PS motion data analysis circuit module is configured to determine, from the map points, a mechanical activation time (MAT). Further, the system includes a MAT modification circuit module. The MAT modification circuit module is configured to modify the MAT of a selected map point based on the MATs corresponding to at least a subset of the map points.

### BRIEF DESCRIPTION OF THE DRAWINGS

**[0009]** FIG. 1 illustrates a flow chart of a method for characterizing motion data collected by a cardiovascular navigation system, in accordance with an embodiment herein.

**[0010]** FIG. 2 illustrates a cardiovascular navigation system for use in imaging an anatomical region of the heart and to collect motion data, in accordance with an embodiment herein.

**[0011]** FIG. 3 illustrates a graphical representation of a plurality of map points of a heart.

**[0012]** FIG. 4 illustrates a motion waveform associated with one wall map point and collected during a single cardiac cycle, in accordance with an embodiment herein.

[0013] FIG. 5 illustrates motion waveforms at different map points during a single cardiac cycle with corresponding clarity scores in accordance with an embodiment herein.

[0014] FIG. 6 illustrates map points and a predetermined radius defining a group of neighboring map points in accordance with an embodiment herein.

[0015] FIG. 7 illustrates map points on the wall of a segmented left ventricular in accordance with an embodiment herein.

[0016] FIG. 8 illustrates motion waveforms at different map points during a single cardiac cycle with corresponding clarity scores in accordance with an embodiment herein.

[0017] FIG. 9 illustrates a flow chart of a method for characterizing motion data collected by a cardiovascular navigation system, in accordance with an embodiment herein.

[0018] FIG. 10 illustrates a system for analyzing motion data in accordance with an embodiment.

#### DETAILED DESCRIPTION

[0019] The description that follows sets forth one or more illustrative embodiments. It will be apparent that the teachings herein may be embodied in a wide variety of forms, some of which may appear to be quite different from those of the disclosed embodiments. Consequently, the specific structural and functional details disclosed herein are merely representative and do not limit the scope of the disclosure. For example, based on the teachings herein one skilled in the art should appreciate that the various structural and functional details disclosed herein may be incorporated in an embodiment independently of any other structural or functional details. Thus, an apparatus may be implemented or a method practiced using any number of the structural or functional details set forth in any disclosed embodiment(s). Also, an apparatus may be implemented or a method practiced using other structural or functional details in addition to or other than the structural or functional details set forth in any disclosed embodiment(s).

[0020] The methods herein may be implemented as a software algorithm, package, or system that directs one or more hardware circuits or circuitry to perform the actions described herein. For example, the operations of the methods herein may represent actions to be performed by one or more circuits that include or are connected with processors, microprocessors, controllers, microcontrollers, Application Specific Integrated Circuits (ASICs), Field-Programmable Gate Arrays (FPGAs), or other logic-based devices that operate using instructions stored on a tangible and non-transitory computer readable medium (e.g., a computer hard drive, ROM, RAM, EEPROM, flash drive, or the like), such as software, and/or that operate based on instructions that are hardwired into the logic of the.

[0021] At least one technical effect of at least one portion of the methods and systems described herein is at least (i) obtaining point specific (PS) motion data for a plurality of map points, (ii) calculating mechanical activation times (MAT) for the map points, (iii) identifying a group of neighboring map points at least partially surrounding a current map point, (iv) modifying the MAT corresponding to the current map point based on MATs corresponding to at least a portion of the group of neighboring map points, and (v) repeat the identifying and modifying operations for at least a subset of the map points thereby deriving updated MAT's based on neighboring MAT's.

[0022] FIG. 1 illustrates a flowchart of a method 100 for characterizing motion data collected by a cardiovascular navigation system (CNS). The method 100, for example, may employ structures or aspects of various embodiments (e.g., systems and/or methods) discussed herein (e.g., the CNS 210 in FIG. 2). In various embodiments, certain steps (or operations) may be omitted or added, certain steps may be combined, certain steps may be performed simultaneously, certain steps may be performed concurrently, certain steps may be split into multiple steps, certain steps may be performed in a different order, or certain steps or series of steps may be re-performed in an iterative fashion. Furthermore, it is noted that the following is just one possible method of characterizing motion data collected by the CNS. It should be noted, other methods may be used, in accordance with an embodiment herein.

[0023] Beginning at 102, the method obtains point specific (PS) motion data for a plurality of map points. The PS motion data may be acquired or collected using a cardiovascular navigation system (CNS) 210 with an electrophysiological sensor 252 in real-time or prior to implementation of FIG. 1. At 104, the method 100 calculates mechanical activation times (MAT) for the map points. At 106, the method 100 identifies a group of neighboring map points (e.g. the map points) for a current map point (e.g., the map point). At 108, the method 100 modifies an MAT corresponding to a current map point based on the calculated MATs corresponding to at least a portion of the group of neighboring map points. At 110, the method 100 repeats the identifying and modifying operations for at least a subset of the map points (e.g., the map point). For example, an alternative current map point is selected and the operation at 106 and 108 is repeated with the alternative current map point. Next, the method of FIG. 1 is discussed in more detail in connection with FIGS. 2-10.

[0024] FIG. 2 illustrates a cardiovascular navigation system (CNS) 210, of an embodiment, for use in imaging an anatomical region of a patient 212, such as, a heart 214. A medical tool 216 is placed within the anatomical region, such as for example, an electrophysiological (EP) mapping catheter or a catheter generally described or shown in U.S. Pat. No. 7,881,769, which is expressly incorporated herein by reference. The medical tool 216 includes a plurality of electrophysiological sensors 252 that may be placed on the endocardial or epicardial surface of the left ventricle (LV) of the heart 214. The electrophysiological sensors 252 may be attached to the distal or proximal end of the medical tool 216, or any point in between. The electrophysiological sensors 252 measure a position and an electrical potential or an electric current of biological cells and tissues. The electrophysiological sensors 252 transmits the position and electrical potential information to an electronic control unit (ECU) 226. For example, the electrophysiological sensors 252 may be positioned by the medical tool 216 to measure PS motion data for a plurality of map points of the wall of the heart 214. It should be understood, however, that the electrophysiological sensors 252 could be used in a variety of anatomical regions or alternative map points within the heart 214 or other organs in which motion characterization may be of interest. Additionally or alternatively, the electrophysiological sensors 252 may be replaced by separate motion sensors and electrical sensors. The motion sensors in contact with the region of interest (e.g., the LV of the heart 214) measuring the position sensors as well as the electrical sensors that are measuring the PS motion data of the region of interest. Optionally, the ECU

**226** may receive the PS motion data and electrical sensor measurements simultaneously from the motion sensors and electrical sensors.

**[0025]** A navigation system **220** is provided to determine the position and orientation of the medical tool **216** within the body of the patient **212**. In the illustrated embodiment, the navigation system **220** comprises a magnetic navigation system in which magnetic fields are generated in the anatomical region and position sensors associated with the medical tool **216** generate an output that is responsive to the position of the sensors within the magnetic field. The navigation system **220** may comprise, for example, the systems generally shown and described in, for example, U.S. Pat. Nos. 6,233,476, 7,197,354, 7,386,339, and 7,505,809 all of which are expressly incorporated by reference in their entirety. Although a magnetic navigation system is shown in the illustrated embodiment, it should be understood that the embodiments could find use with a variety of navigation systems including those based on the creation and detection of axes specific electric fields. The navigation system **220** may include a transmitter assembly **250**.

**[0026]** The transmitter assembly **250** may include a plurality of coils arranged orthogonally to one another to produce a magnetic field in and/or around the anatomical region of interest. It should be noted that, although the transmitter assembly **250** is shown under the body of the patient **212** and under the table **234** in FIG. 2, the transmitter assembly **250** may be placed in another location, such as, attached to the radiation emitter **230**, from which the magnetic field generators can project a magnetic field in the anatomical region of interest. In accordance with certain embodiments the transmitter assembly **250** is within the field of view **236**. The ECU **226** may control the generation of magnetic fields by transmitter assembly **250**.

**[0027]** The electrophysiological sensors **252** are configured to generate an output dependent on the relative position of electrophysiological sensors **252** within the field generated by the transmitter assembly **250**. In FIG. 2, the electrophysiological sensor **252** and the medical tool **216** are shown disposed around the heart **214**. The navigation system **220** determines the location of the electrophysiological sensors **252** within the generated field, and thus the position of the medical tool **216** as well. The navigation system **220** may further determine navigation coordinates, such as a Cartesian coordinate (e.g., (X, Y, Z), of the navigation coordinate system.

**[0028]** The ECU **226** of the navigation system **220** may include or represent hardware circuits or circuitry that include and/or are connected with one or more logic based devices, such as processors, microprocessors, controllers, microcontrollers, or other logic based devices (and/or associated hardware, circuitry, and/or software stored on a tangible and non-transitory computer readable medium or memory). The ECU **226** may receive a plurality of input signals including signals generated by the medical tool **216**, the electrophysiological sensors **252**, an operator system interface **254**, and one or more patient reference sensors (not shown) and generate a plurality of output signals including those used to control the medical tool **216** and/or the display **258**. The ECU **226** may also receive an input signal from an organ monitor (not shown), such as an ECG monitor, and sort or segregate images from an imaging system **218** based on a timing signal of a monitored organ. For example, ECU **226** may sort images based on the phase of the patient's cardiac cycle at which each

image was collected, as more fully described in U.S. Pat. No. 7,697,973, which is hereby incorporated by reference in its entirety.

**[0029]** The ECU **226** may acquire measurements from the electrophysiological sensors **252** of PS motion data indicating an amount of motion that occurred at the corresponding map point on a wall of the heart **214** during at least one cardiac cycle. The heart may be divided into numerous map points along the wall of the various chambers.

**[0030]** FIG. 3 illustrates a graphical representation of a plurality of map points associated with a portion of a heart **300**, such as heart wall **306**, for which it is desirable to measure PS motion data. The term "point specific" is used to indicate that the motion data is associated with a single select location on the heart wall. The data values represent positions of the single select location over one or more cardiac cycles. The heart wall **306** may be separated into map points **308-310**. The example of FIG. 3 shows three map points of interest **308-310** along the wall of the LV. Optionally, more or fewer map points of interest may be designated. A tool **302** (e.g., the medical tool **216** with the plurality of electrophysiology sensors **252**) is positioned directly against the heart wall **306** at one or more points within each map point of interest **308-310**. The tool **302** measures movement of the one or more points over a select period of time. In the example of FIG. 3, the tool **302** is shown positioned against a point of interest in each map point **308-310** at different points in time.

**[0031]** For example, the tool **302** is positioned, during a first measuring operation, at a point within the map point **308** while collecting PS motion data associated with movement (e.g., along the arrow **312**) by the map point **308**. The movement may be in various linear, transverse, or rotational directions. Next, the tool **302** may be positioned, during a second measuring operation, at a point within the map point **309** while collecting PS motion data associated with movement (e.g., along the arrow **313**) by the map point **309**. Next, the tool **302** is positioned, during a third measuring operation, at a point within the map point **310** while collecting PS motion data associated with movement (e.g., along the arrow **314**) by the map point **310**.

**[0032]** The position of the tool **302** may be continuously monitored by a navigation system (e.g., the navigation system **220**) to obtain sets of motion data associated with each map point **308-310** over a select period of time, such as, during at least one cardiac cycle. In FIG. 3, a motion waveform subset **320** is collected during one cardiac cycle while the tool **302** is held against the LV wall acquiring PS motion data for a point within the map point **308**. The PS motion data may define a motion waveform **326** at the map point **308**. The motion waveform **326** represents a displacement of the map point **308**, illustrated with respect to a vertical axis **327** axis representing an amount of displacement of the map point **308** from a start reference position, during the cardiac cycle, illustrated along a horizontal axis **328** representing time from a beginning **328a** to an end **328b** of the cardiac cycle. Optionally, the tool **302** may be held against the LV wall at a point within the map point **308** for multiple heart beats or cardiac cycles thereby generating multiple motion waveform subsets **320-323** (e.g., for four consecutive heart beats). Optionally, the PS motion data subsets **320-323** may be collected for fewer than or more than four heart beats. The PS motion data subsets **320-323** associated with the map point **308** may be grouped to form a collection **325** of motion waveform subsets **320-323** associated with a single map point **308**.

[0033] Additionally or alternatively, the motion waveform 326 of the PS motion at the map point 308 may represent a waveform indicative of strain (e.g., tissue deformation) or strain rate at the map point 308 from the beginning 328a to the end 328b of the cardiac cycle, traversing along an axis formed by longitudinal divisions 742 (FIG. 7)), a radial direction, and/or a circumferential direction (e.g., traversing along an axis formed by circumferential divisions 740 (FIG. 7)). Strain rate is the rate at which the tissue deformation or strain occurs over time. Strain rate may be measured as the difference, in velocity between two map points (e.g., toward each other, away from each other) along the heart wall, normalized to the distance between the two map points.

[0034] For example, the ECU 226 may set a position reference point at the beginning 328a of the cardiac cycle. During the cardiac cycle, the ECU 226 may compare instantaneous positions of the tool 302 at the map point 308, over the cardiac cycle, against the positions of surrounding map points to acquire the PS motion data representing strain of the map point 308. The PS motion data may define the strain over the cardiac cycle. Optionally, the ECU 226 may determine the strain rate of the map point 308 by calculating the derivative or change in the strain over time. The strain or strain rate at a select map point may be relative to one or more other map points. Optionally, the select map point may have multiple strains or strain rates associated there with.

[0035] Once a desired amount of motion data is collected for the map point 308, the tool 302 is moved to a next desired position, such as at a point within the map point 309. Next, the data collection process is repeated to obtain PS motion data forming a motion waveform 336 indicative of an amount of motion experienced or displacement of the map point 309 over a cardiac cycle (e.g., heart beat). Optionally, the tool 302 may be held for multiple heart beats to obtain PS motion data subsets 330-333 over a corresponding number of heart beats (e.g., cardiac cycles).

[0036] Once a desired amount of motion data is collected for the map point 309, the tool 302 is moved to a next desired position such as at a point within the map point 310. Next, the data collection process is repeated to obtain PS motion data forming a motion waveform 346 indicative of an amount of motion experienced or a displacement of the map point 310 over a cardiac cycle (e.g., heart beat). Optionally, the tool 302 may be held for multiple heart beats to obtain PS motion data subsets 340-343 over a corresponding number of heart beats (e.g., cardiac cycles). The motion waveform subsets 330-333, and 340-343, which are associated with map points 309 and 310, may be grouped to form collections 335 and 345, respectively, associated with single map points 309 and 310. The plurality of motion waveform subsets 320-343 for all map points 308-310 of interest of the heart wall 306 may collectively define a motion data set 350.

[0037] Optionally, more map points of the heart wall 306 may be studied to collect additional motion waveform subsets of motion data. For example, the walls of the right ventricular, right atrium, and/or left atrium may also be divided into map points, for which motion data is collected.

[0038] A cardiovascular navigation system (e.g., CNS 110) collects the motion data from one or more tools 302. The motion data 350 may be analyzed to identify and remove non-ectopic beats and to eliminate beats with abrupt mechanical movement. Optionally, the motion data 350 may include averages of motion data collected over multiple heart beats (cardiac cycles). For example, the motion waveform

subsets 320-323 may be combined through averaging or otherwise. Optionally, the motion data 350, which is utilized in connection with embodiments described hereafter, may include information indicative of a radial component of wall movement, and/or may include information indicative of a longitudinal component of wall movement. Optionally, the motion data may include information associated with 3-dimensional (3-D) movement calculated as a 3-D distance from an initial position at a select starting point in the cardiac cycle, such as an R-wave or local electrical activation time.

[0039] Optionally, the CNS 110 may adjust the motion waveform subsets 325, 335, 345 to extend over a common time interval. For example, the motion waveform subsets 325, 335, 345 may be temporally equalized by "stretching" the motion waveforms that have shorter cycle lengths until the shorter motion waveform subsets have a length equal to the predetermined interval. The common time interval may be predetermined, or automatically selected, such as by choosing a length corresponding to the longest, shortest, or average length of the motion waveform subset 320-323. The time interval may be set to begin at a point in time defined by a global signal such as the peak of the R-wave as detected by using the Electrocardiogram (ECG) or Intracardiac Electrogram (IEGM) signals as described in the provisional application titled "METHOD TO MEASURE CARDIAC MOTION USING A CARDIOVASCULAR NAVIGATION SYSTEM," having docket number A13E3025, which is expressly incorporated herein by reference in its entirety. Optionally, the time interval may be defined to begin based on another global marker of electrical activity (e.g., the T-wave, P-wave).

[0040] Returning to FIG. 1, at 104, the method 100 calculates mechanical activation times (MAT) for the map points 308-310. FIG. 4 illustrates an expanded view of the motion waveform 336 associated with the map point 309 and collected during a single cardiac cycle (e.g., heart beat). The motion waveform 336 plots radial displacement (e.g., in millimeters) of the map point of interest along a vertical axis 412 and time along a horizontal axis 414. The direction of movement is illustrated from a beginning/zero point in time until completion of a cardiac cycle (e.g., after 1 sec.). The motion waveform 336 is divided into sectors Q1-Q4 that are associated with portions or phases of the cardiac cycle. The motion waveform 336 exhibits an amount of radial motion during each sector Q1-Q4.

[0041] The ECU 226 may determine a magnitude and/or direction of radial motion corresponding to the map point (e.g., the map point 308, 309, 310) of the wall of the heart during the associated phases of the cardiac cycle. The radial motion may be quantified in terms of the direction of motion and/or the amplitude/magnitude of motion. Optionally, motion may occur in directions other than radially. With reference to FIG. 4, the motion may be determined by finding net movement during the sector Q1, Q2, Q3 or Q4. For example, in sector Q1 the net movement is determined by identifying a location (displacement) of the first point 402 in the sector Q1 and identifying a location of the last point 404 in the sector Q1. The points 402-410 represent sector transition points and can be compared to determine the net movement. For example, in sector Q3, the net movement is approximately 8 mm, as the wall map point moved from a radial displacement of -9.0 at the beginning of sector Q3 to a radial displacement of -1.0 at the end of sector Q3 (corresponding to the beginning of sector Q4).

[0042] Further, the ECU 226 may determine the MAT for the map point 309 based on the change in direction of motion and/or the amplitude/magnitude of motion of the waveform. The MAT may represent a point in time when the wall of the heart, measured at the map point, transitions from a systole to diastole stage. During the transition, the displacement of the map point may shift from a radially inward direction that is away from the electrophysiological sensor 252 to a radially outward direction that is towards the direction of the electrophysiological sensor 252. Optionally, a time of the transition may be determined by correlating the electrical information of the heart measured by the ECG monitor to the mechanical information measured by the electrophysiological sensors 252. The ECU 226 may determine the MAT as a time at which the electrical information from the ECG monitor that correlates to the systole to diastole transition of the wall at the map point.

[0043] Additionally or alternatively, the MAT for the map point 309 may represent a time when the motion waveform 336 reaches a minimum displacement along the vertical axis 412. For example, the motion waveform 336 reached the minimum displacement along the vertical axis 412, within sector Q3, at a displacement 412 and time 418. The ECU 226 may determine that the MAT to be at the time 418 representing the time when the minimum displacement, the displacement 412, occurred.

[0044] Optionally, the MAT for the map point 309 may represent a time when the motion waveform 336 is at a maximum displacement from a predetermined reference line 420. For example, the ECU 226 may have the predetermined reference line 420. The predetermined reference line 420 may be set by a user of the CNS 210 using the operator system interface 254. Optionally, the predetermined reference line 420 may be set at the displacement of the sector transition point 402 or 410. The ECU 226 may calculate the displacement of the PS motion data points along the motion waveform 336 from the predetermined reference line 420 and select the PS motion data point that has the greatest or maximum displacement relative to the remaining PS motion data point from the predetermined reference line 420. The ECU 226 may select the PS motion data point occurring at the time 418, and designate the time 418 as the MAT for the map point 309.

[0045] Optionally, the MAT of the map point 309 may represent a time when the motion waveform 336 has an initial deviation towards a baseline 416 representing the onset of an opposing motion. The ECU 226 may set the baseline 416 at a sector transition point located between sectors with opposing net movements, which would indicate the opposing motion of the map point 309. For example, Q2 has an inward net movement and is adjacent to Q3 that has an outward net movement. The ECU 226 may select the displacement of the transition point 406, which is between Q2 and Q3, as the baseline 416. The ECU 226 may compare the displacement of each PS motion data points with adjacent PS motion data points below the baseline 416 to determine the time of a PS motion data point with lower distance indicating movement towards the baseline 416 and may be determined as the MAT.

[0046] Additionally or alternatively, the ECU 226 may calculate slopes or gradients of the PS motion data point. A zero slope or opposing slopes from two sets of adjacent PS motion data points may indicate the onset of an opposing motion, which may be used to calculate the MAT for the map point. For example, the ECU 226 may calculate slopes traversing along the horizontal axis 414 from continuous sets of adjacent

PS motion data points that are below the baseline 416. The ECU 226 may calculate a negative slope 426 and a positive slope 424 from two adjacent sets of PS motion data points that are below the baseline 416. The ECU 226 may calculate that the MAT is the time point between the two adjacent sets of PS motion data points or the time point that is located at the intersection of the positive and negative slopes 424 and 426.

[0047] Optionally, the ECU 226 may determine an extent of motion (EM) of the map points from the PS motion data forming the motion waveform. The EM may represent the maximum extent of motion of the map point. The EM may be calculated based on a comparison of the maximum and minimum displacements of the PS motion data at the map point.

[0048] In an embodiment, the ECU 226 may assign a clarity score to the motion waveform based on a distinctiveness of a feature of interest within the motion waveform. The clarity score represents a level of confidence that a MAT value is correct. The confidence (and clarity score) increases or decreases based on a shape of the motion waveform, and thus the distinctiveness of the feature of interest. The distinctive feature of interest may represent a region of the motion waveform used to determine the MAT of the map point. For example, the distinctive feature may represent a peak or vertex of the motion waveform having a U-shape or parabolic shape. Optionally, the clarity score may be associated with both the MAT and EM at the corresponding map point. Additionally or alternatively, the distinctive feature of interest may be a line symmetry of the motion waveform such that the motion waveform has at most two PS motion data points at a common level of displacement. Optionally, the distinctive feature may be based on the slopes of the PS motion data points within the motion waveform.

[0049] Deviations from the distinctive feature may indicate unclear motion waveform morphology that may be caused by errors in the acquired PS motion data for the map point that defines the motion waveform. For example, if the electrophysiological sensor 252 is not directly against the heart wall during the entire cardiac cycle the motion waveform may have a flat peak, multiple peaks, lack of line symmetry, or the like. The ECU 226, for example, may detect or identify the deviations from the distinctive feature and designate a lower confidence of the calculated MAT by with a corresponding clarity score.

[0050] FIG. 5 illustrates motion waveforms 536-539 defined from PS data points measured at different map points (e.g., the map points 308, 309, 310) during a single cardiac cycle in accordance with an embodiment herein. The motion waveform 536-539 plots radial displacement (e.g., in millimeters) of the map point of interest each along a vertical axis 502 and time along a horizontal axis 504. Each of the map points have a calculated MAT 520, 530, 540, 550 with a corresponding clarity score. The clarity score may be a numerical number representing a predetermined level of confidence in the corresponding MAT of the map point. For example, clarity scores may range from a clarity score of 1 through 3. A clarity score of 1 indicates that there is a low confidence level in the MAT value calculated for the map point. A clarity score of 2 indicates that there is a medium confidence level in the MAT calculated for the map point, but the MAT may be verified or corrected based one or more other map points or calculated MATs. A clarity score of 3 indicates that there is a high confidence level in the MAT value calculated for the map point. It should be noted, that alternative

embodiments may have more than or fewer than three levels of clarity scores for the calculated MATs.

**[0051]** The MAT **520** is shown having a clarity score of 3. As described above, the clarity score of 3 may indicate that the ECU **226** has assigned a high confidence in the MAT **520** calculated for the map point. The confidence level of the MAT **520** is based on the distinctive feature of the motion waveform **536**, for example, due to the number of peaks of the motion waveform **536**. The number of peaks may be determined by the ECU **226** as the number of peaks below a predetermined threshold **521**. Additionally or alternatively, the ECU **226** may determine the number of peaks as the number of occurrences, at which the motion waveform **536** has a slope of zero or is parallel to the horizontal axis **504** and falls below the predetermined threshold **521**. The motion waveform **536** has a single peak or vertex **522**, which has a slope of zero, surrounded by PS motion data points with opposing slopes representing a set minimum displacement for the motion waveform **536**.

**[0052]** The MAT **530** is shown having a clarity score of 2. As described above, the clarity score of 2 may indicate that the ECU **226** has assigned a medium confidence in the MAT **530** calculated for the map point. The confidence level of the MAT **530** is based on a feature of the motion waveform **537** that has average distinctiveness, for example, due to the flatness of a peak **531**. The distinctiveness of a feature of interest is reduced when the motion wave form includes clouding components, such as flatness, extra peaks and the like. As described above, the ECU **226** may determine the number of peaks, peak **531**, as the number of peaks or number of occurrences of zero slope that are below the predetermined threshold **521**. The motion waveform **537** is illustrated with one peak, the peak **531**. The ECU **226** may determine the flatness of the peak **531** by monitoring displacement values of the PS motion data within the peak **531**. The ECU **226** may determine a time period **508** of which the peak **531** or the displacement values of the PS motion data remains within a predetermined displacement range **532**. The time period **508** may be compared with a predetermined peak period **533**. If the time period **508** is larger than the predetermined peak period **533**, as shown in FIG. 5, the peak **531** is flat and an imperfect distinctive feature of the motion waveform **537**. Alternatively, if the time period **508** is smaller than the predetermined peak period **533**, the peak **531** would be a determined sharp or not flat.

**[0053]** The MAT **540** is shown having a clarity score of 2. The clarity score of the MAT **540** is based on a feature of the motion waveform **538** that has average distinctiveness, for example, due to the number of peaks of the motion waveform **538**. As described above, ECU **226** may determine the number of peaks as the number of peaks below the predetermined threshold **521**. The motion waveform **538** has two peaks below the predetermined threshold **521**, the peaks **541** and **543**, which affords as medium distinctive feature.

**[0054]** The MAT **550** is shown having a clarity score of 1. The clarity score of the MAT **550** is based on the lack of a distinctive feature of the motion waveform **539**. The motion waveform **539** has no peaks below the predetermined threshold **521**. Further, the motion waveform is not line symmetric. For example, at the calculated MAT **550** the PS motion data point is at a displacement value **561**. The motion waveform **539** as more than one other PS motion data point **552a-c** at the displacement value **551**.

**[0055]** Returning to FIG. 1, at **106**, the method **100** identifies a group of neighboring map points (e.g., the map points **308-310**) for a current map point (e.g., the map point **309**). Optionally, the group of neighboring map points (e.g., the map points **308-310**) may be any map point that is within a predetermined radius **604** (also referred to as neighborhood limit) from the current map point (e.g., the map point **309**). For example, the map point **309** may be designated as the current map point and as illustrated in FIG. 6, centered within the predetermined radius **604**. The predetermined radius **604** may be 7 mm, such that, any map point outside the predetermined radius **604** or have a distance greater than the predetermined radius **604** from the current map point is excluded from the group of the neighboring map points. The current map point and the predetermined radius **604** may be designated by the user via the operator system interlace **254**.

**[0056]** The ECC **226** may calculate a three-dimension (3D) physical distance between pairs of the map points such as between the current map point **309** and another map point **308** and **10** (FIG. 3) using the 3D distance formula of equation 1 below.

$$3D \text{ Distance} = \sqrt{(x_1 - x_2)^2 + (y_1 - y_2)^2 + (z_1 - z_2)^2} \quad (\text{Equation 1})$$

**[0057]** The cartesian coordinates (e.g., (X, Y, Z)) of each map point **308**, **309**, and **310** may be determined by the navigation system **220**, as described above, by measuring the position of the electrophysiological sensors **252**. For example, the map point **309** may be positioned at coordinate (2, 5, 6), the map point **308** may be positioned at coordinate (1, 2, 2), and the map point **310** may be positioned at coordinate (4, 9, 12). The ECC **226** may determine a distance **602** and **608** between the map point **309** and the map points **308** and **310**, respectively, using equation 1. For example, 1, the ECC **266** may calculate the distance **602** to be approximately 5.1 mm and the distance **608** to be approximately 7.48 mm. The ECC **266** then will only use the group of neighboring map points **308** and **309**. The map point **310** will be excluded from the group of neighboring map points. It should be noted, that the distance to and number of map points will vary.

**[0058]** Optionally, the predetermined radius **604** may vary depending on the location of the current map point. For example, the predetermined radius **604** may be smaller with a current map point at an apical point of the left ventricular relative to a current map point at a basal point of the left ventricular.

**[0059]** Optionally, the predetermined radius **604** may be the radial distance or a proportion of the radial distance from the current map point to a select point on the heart such as the central axis between the apex and the mitral annulus of the left ventricular. Additionally or alternatively, the predetermined radius **604** may be based on a percentage of the surface area of the heart or a portion of the heart, such as the left ventricular, or percentage of the distance from the apex to the mitral annulus measured at a certain point in time.

**[0060]** Optionally, the group of neighboring map points may be limited based on predefined segments of the heart wall. FIG. 7 illustrates a left ventricular **702** of the heart divided into 18 segments (not all segments shown) formed from 6 circumferential divisions **740** (not all divisions shown) and 3 longitudinally divisions **742**. A current map point **706** may be at a selected position within segment **720**. The group of neighboring map points may be any map point positioned within the segment **720**. Additionally or alternatively, the group of neighboring map points may be defined as any map



point within segment 720 and map points within segments (e.g., segments 724-728) that are adjacent to the segment 720. Additionally or alternatively, map points may be excluded from the group of neighboring map points when a non-tissue area exists between the potential neighbor map points and the current map point 706. For example, if a blood pool 750 separates the current map point 706 from the potential neighbor map point 702, the map point 702 would not be included within the group of neighboring map points (even though the map point 702 is within the segment 720). Additionally or alternatively, map points may be excluded from the group of neighboring map points when other structures are located between the map points that cause the map points to move relatively independently even during normal cardiac motion.

[0061] At 108, the method 100 modifies an MAT 916 corresponding to a current map point 902 based on the calculated MATs 918-924 corresponding to at least a portion of the group of neighboring map points in real-time or prior to implementation of FIG. 1. FIG. 8 illustrates a flow chart of a method 800 for modifying the MAT 916 in accordance with an embodiment based on the calculated MATs 918-924.

[0062] At 802, the method 800 selects a portion or a subset of the map points 906-910 from a group of neighboring map points 950, specifically, selecting only map points with a clarity score of 3 (e.g., the map points 906-908 and/or a clarity score of 2 with a re-evaluated MAT (e.g., the map point 910). Map points with a clarity score of 1 and clarity score of 2 without re-evaluation MAT (e.g., the map point 904) are excluded from the portion or subset. FIG. 9 illustrates the motion waveforms 930-936 that are defined from PS data points measured at different map points 902-910 during a single cardiac cycle in accordance with an embodiment herein. The motion waveforms 930-936 plots radial displacement (e.g., in millimeters) of the map points 902-910 of interest on a graph having displacement along a vertical axis 912 and time along a horizontal axis 914.

[0063] At 804, the method 800 calculates a standard deviation of the calculated MATs 920-924 for the map points 906-910 from the group of neighboring map points 950. At 806, if the standard deviation of the calculated MATs 920-924 is not within a predetermined threshold  $\Delta t_1$ , the method removes the farthest map point neighbor (e.g., the map point 910) from the portion or subset and recalculates the standard deviation of the MATs for the remaining map points (e.g., the map points 906-908).

[0064] If the standard deviation of the calculated MATs 920-924 from the portion of the map points 906-910 is within the predetermined threshold  $\Delta t_1$ , at 808, the methods calculates a mean or MeanMAT of the MATs 920-924. Optionally, the mean or average may be a weighted mean based on a distance of each of the map points 906-910 within the subset from the current map point 902. Optionally, a map point closest to the current map point 902 will be weighted more than a map point further away, relatively, from the current map point 902.

[0065] The modification of the MAT 916 may be based on the deviations from the distinctive feature or the unclear motion waveform morphology of the motion waveform 930, such as, a motion waveform with multiple peaks or a flat peak. At 812 and 814, for the motion waveform 930 includes multiple peaks 940 and 942, the MeanMAT is compared with either of the peaks 940 and 942. If neither peak 940, 942 is within a predetermined period  $\Delta t_2$  of the MeanMAT the map point is discarded. If one of the peaks 940, 942 is within the

predetermined period  $\Delta t_2$ , then, at 820, the one peak is set as the MAT for the map point 902. If both peaks 940 and 942 are within the predetermined period  $\Delta t_2$  then, at 824, the peak 940, 942 closest to the MeanMAT is set as the MAT for the map point 902.

[0066] At 816, for a motion waveform with a flat peak (e.g., the motion waveform 537), if the MeanMAT is within the flat region (e.g., the time period 508) the MAT 916 is shifted to MeanMAT (at 822). At 818, determine if the MeanMAT is before an earliest part of the flat region, if so, then at 826 the MAT is shifted to the start of the flat region. If not, then at 828, the MAT of the motion waveform (e.g., the motion waveform 537) is shifted to the end of the flat region.

[0067] At 110, the method 100 repeats the identifying and modifying operations for at least a subset of the map points (e.g., the map point 310). For example, an alternative current map point is selected and the operation at 106 and 108 is repeated with the alternative current map point.

[0068] Optionally, the CNS 210 (FIG. 2) may also include an imaging system 218. The CNS 210 may further include a registration system for registering a group of images of the anatomical region of the patient 212 in a navigation coordinate system of the medical device navigation system 220 as generally described and shown in U.S. Patent Publication 2013/0272592 and International Pub. No. WO 2012090148, the entire disclosure of which is expressly incorporated herein by reference.

[0069] The imaging system 218 may be provided to acquire images of heart 214 or another anatomical region of interest. The imaging system 210 may, for example, comprise of a fluoroscopic imaging system. Additionally or alternatively, rather than a fluoroscopic imaging system, computed tomography (CT) imaging systems, a three-dimensional radio angiography (3DRA) system, and the like may be used. Although the imaging system 218 is described herein for an exemplary embodiment of the invention, the imaging system 218 is not required for the inventive subject matter described within this application.

[0070] The imaging system 218 may include a C-arm support structure 228, a radiation emitter 230, and a radiation detector 232. The emitter 230 and detector 232 are disposed on opposite ends of the support structure 228 and disposed on opposite sides of the patient 212 as the patient 212 lays on an operation table 234. The emitter 230 and detector 232 define a field of view 236 and are positioned such that the field of view 236 includes the anatomical region of interest as the patient 212 lays on the operation table 234. The imaging system 218 is configured to capture images of anatomical features and other objects within the field of view 236. The support structure 228 may have freedom to rotate about the patient 212 as shown by lines 238 and 240. The support structure 228 may also have freedom to slide along lines 242 and 244 (e.g., along the cranio-caudal axis of the patient 212) and/or along lines 246 and 248 (e.g., perpendicular to the cranio-caudal axis of the patient 212). Rotational and translational movement of the support structure 228 yields corresponding rotational and translational movement of the field of view 236.

[0071] The imaging system 218 may acquire a group of images of an anatomical region of the patient 212 by first shifting along lines 242, 244, 246, and/or 248 to place the anatomical region of interest within the field of view 236. Second, the support structure 228 may rotate the radiation emitter 230 and the radiation detector 232 about the patient

**212**, keeping the anatomical region within the field of view **236**. The imaging system **218** may capture images of the anatomical region as the support structure **228** rotates, providing a group of two-dimensional images of the anatomical region from a variety of angles. The group of images may be communicated to the ECU **226** for image processing and display. The group of images may comprise a sequence of images taken over a predetermined time period.

[0072] Additionally, one or more patient reference sensors (not shown) may be on the body of the patient **212**, for example, on the chest. The patient reference sensors measure a displacement and orientation of the patient reference sensors relative to a predetermined reference point, such as, the electrophysiological sensors **252** or the transmitter assembly **250**.

[0073] FIG. 10 illustrates a functional block diagram of an embodiment of an electronic control unit (ECU) **1000** that is operated in accordance with the processes described herein to analyze motion data and to interface with the CNS **210**. The ECU **1000** may be a workstation, a portable computer, a PDA, a cell phone and the like. The ECU **1000** includes an internal bus that connects/interfaces with a Central Processing Unit (CPU) **1002**, ROM **1004**, RAM **1006**, a hard drive **1008**, the speaker **1010**, a printer **1012**, a CD-ROM drive **1014**, a floppy drive **1016**, a parallel I/O circuit **1018**, a serial I/O circuit **1020**, the display **1022**, a touch screen **1024**, a standard keyboard connection **1026**, custom keys **1028**, and a telemetry subsystem **1030**. The internal bus is an address/data bus that transfers information between the various components described herein. The hard drive **1008** may store operational programs as well as data, such as waveform templates and detection thresholds.

[0074] The CPU **1002** typically includes a microprocessor, a microcontroller, or equivalent control circuitry, and may interface with the CNS **210**. The CPU **1002** may include RAM or ROM memory, logic and timing circuitry, state machine circuitry, and I/O circuitry to interface with the CNS **210**. The display **1022** (e.g., may be connected to the video display **1032**). The touch screen **1024** may display graphic information relating to the CNS **210**. The display **1022** displays various information related to the processes described herein. The touch screen **1024** accepts a user's touch input **1034** when selections are made. The keyboard **1026** (e.g., a typewriter keyboard **1036**) allows the user to enter data to the displayed fields, as well as interface with the telemetry subsystem **1030**. Furthermore, custom keys **1028** turn on/off **1038** (e.g., EVVI) the ECU **1000**. The printer **1012** prints copies of reports **1040** for a physician to review or to be placed in a patient file, and speaker **1010** provides an audible warning (e.g., sounds and tones **1042**) to the user. The parallel I/O circuit **1018** interfaces with a parallel port **1044**. The serial I/O circuit **1020** interfaces with a serial port **1046**. The floppy drive **1016** accepts diskettes **1048**. Optionally, the floppy drive **1016** may include a USB port or other interface capable of communicating with a USB device such as a memory stick. The CD-ROM drive **1014** accepts CD ROMs **1050**.

[0075] The CPU **1002** is configured to analyze PS motion data collected by the CNS **210** for a plurality of map points to determine a MAT for the map points. The CPU **1002** includes a PS motion data analysis circuit module **1062** that may calculate the MAT as explained herein. Further, the circuit module **1062** may determine the distinctive features of the motion waveform defined by the PS motion data. For

example, the circuit module **1062** may determine the number of peaks, flatness, and the slope of the motion waveform defined by the PS motion data that corresponds to a tmap point on the wall of the heart during at least one cardiac cycle. The CPU **1002** includes a MAT analysis circuit module **1064** that is configured to analyze the MAT calculation in relation to the circuit module **1062** to determine a clarity score for the calculated MATs.

[0076] A MAT modification circuit module **1068** may identify a group of neighboring map points for a current map point and modify the current map point based on the MAT corresponding to at least a portion of the group of neighboring map points. Optionally, the MAT modification circuit module **1068** may calculate a standard deviation for the neighboring map points.

[0077] As one example, the measure circuit module **1068** may determine, as the measure of dyssynchrony, a proportion of the map points that are moving in the select direction which represents at least one of inward during a systole phase and outward during a diastole phase. As another example, the measure circuit module **1068** may calculate, as the measure, a proportion of a number of map points that move in the select direction out of a total number of map points.

[0078] The display **1022** displays a dyssynchrony score based on the measure of dyssynchrony in connection with at least one of lead placement for a cardiac resynchronization therapy (CRT) device or programming optimization for a CRT device.

[0079] The telemetry subsystem **1030** includes a central processing unit (CPU) **1052** in electrical communication with a telemetry circuit **1054**, which communicates with both an IEGM circuit **1056** and an analog out circuit **658**. The circuit **1056** may be connected to leads **1060**. The circuit **1056** may also be connected to implantable leads to receive and process IEGM cardiac signals. Optionally, the IEGM cardiac signals sensed by the leads may be collected by the CNS **210** and then transmitted, to the ECU **1000**, wirelessly to the telemetry subsystem **1030** input.

[0080] The telemetry circuit **1054** is connected to a telemetry wand **1062**. The analog out circuit **1058** includes communication circuits to communicate with analog outputs **1064**. The ECU **1000** may wirelessly communicate with the CNS **210** and utilize protocols, such as Bluetooth, GSM, infrared wireless LANs, HIPERLAN, 3G, satellite, as well as circuit and packet data protocols, and the like. Alternatively, a hard-wired connection may be used to connect the ECU **1000** to the CNS **210**.

[0081] One or more of the operations described above in connection with the methods may be performed using one or more processors. The different devices in the systems described herein may represent one or more processors, and two or more of these devices may include at least one of the same processors. In one embodiment, the operations described herein may represent actions performed when one or more processors (e.g., of the devices described herein) are hardwired to perform the methods or portions of the methods described herein, and/or when the processors (e.g., of the devices described herein) operate according to one or more software programs that are written by one or more persons of ordinary skill in the art to perform the operations described in connection with the methods.

[0082] It is to be understood that the above description is intended to be illustrative, and not restrictive. For example, the above-described embodiments (and/or aspects thereof)

may be used in combination with each other. In addition, many modifications may be made to adapt a particular situation or material to the teachings of the inventive subject matter without departing from its scope. While the dimensions and types of materials described herein are intended to define the parameters of the inventive subject matter, they are by no means limiting and are exemplary embodiments. Many other embodiments will be apparent to one of ordinary skill in the art upon reviewing the above description. The scope of the inventive subject matter should, therefore, be determined with reference to the appended claims, along with the full scope of equivalents to which such claims are entitled. In the appended claims, the terms “including” and “in which” are used as the plain-English equivalents of the respective terms “comprising” and “wherein.” Moreover, in the following claims, the terms “first,” “second,” and “third,” etc. are used merely as labels, and are not intended to impose numerical requirements on their objects. Further, the limitations of the following claims are not written in means-plus-function format and are not intended to be interpreted based on 35 U.S.C. § 112(f), unless and until such claim limitations expressly use the phrase means for followed by a statement of function void of further structure.

**[0083]** This written description uses examples to disclose several embodiments of the inventive subject matter and also to enable a person of ordinary skill in the art to practice the embodiments of the inventive subject matter, including making and using any devices or systems and performing any incorporated methods. The patentable scope of the inventive subject matter is defined by the claims, and may include other examples that occur to those of ordinary skill in the art. Such other examples are intended to be within the scope of the claims if they have structural elements that do not differ from the literal language of the claims, or if they include equivalent structural elements with insubstantial differences from the literal languages of the claims.

**[0084]** The foregoing description of certain embodiments of the inventive subject matter will be better understood when read in conjunction with the appended drawings. To the extent that the figures illustrate diagrams of the functional blocks of various embodiments, the functional blocks are not necessarily indicative of the division between hardware circuitry. Thus, for example, one or more of the functional blocks (for example, processors or memories) may be implemented in a single piece of hardware (for example, a general purpose signal processor, microcontroller, random access memory, hard disk, and the like). Similarly, the programs may be stand-alone programs, may be incorporated as subroutines in an operating system, may be functions in an installed software package, and the like. The various embodiments are not limited to the arrangements and instrumentality shown in the drawings.

**[0085]** As used herein, an element or step recited in the singular and proceeded with the word “a” or “an” should be understood as not excluding plural of said elements or steps, unless such exclusion is explicitly stated. Furthermore, references to “one embodiment” of the inventive subject matter are not intended to be interpreted as excluding the existence of additional embodiments that also incorporate the recited features. Moreover, unless explicitly stated to the contrary, embodiments “comprising,” “including,” or “having” an element or a plurality of elements having a particular property may include additional such elements not having that property.

**[0086]** In some embodiments, code including instructions (e.g., software, firmware, middleware, etc.) may be executed on one or more processing devices to implement one or more of the described functions or components. The code and associated components (e.g., data structures and other components used by the code or used to execute the code) may be stored in an appropriate data memory that is readable by a processing device (e.g., commonly referred to as a computer-readable medium).

**[0087]** The components and functions described herein may be connected or coupled in many different ways. The manner in which this is done may depend, in part, on whether and how the components are separated from the other components. In some embodiments some of the connections or couplings represented by the lead lines in the drawings may be in an integrated circuit, on a circuit board or implemented as discrete wires or in other ways.

1. A method for characterizing motion data collected by a cardiovascular navigation system, the method comprising:

obtaining point specific (PS) motion data for a plurality of map points, wherein the PS motion data indicates an amount of motion that occurred at the corresponding map point on a wall of the heart during at least one cardiac cycle;

calculating mechanical activation times (MAT) for the map points;

identifying a group of neighboring map points for a current map point;

modifying the MAT corresponding to the current map point based on the MATs corresponding to at least a portion of the group of neighboring map points; and

repeat the identifying and modifying operations for at least a subset of the map points.

2. The method of claim 1, wherein the calculating operation comprises calculating a three-dimension (3D) physical distance between pairs of map points.

3. The method of claim 1, wherein the PS motion data defines a motion waveform at the corresponding map point, where the motion waveform represents at least one of displacement, strain, or strain rate over a select period of time, the calculating operation calculating the MATs based on the motion waveforms.

4. The method of claim 3, further comprising assigning clarity scores to each of the motion waveforms based on a distinctiveness of a feature of interest within the motion waveforms used to determine the MATs, the clarity scores representing confidence levels in the corresponding MATs.

5. The method of claim 4, wherein the assigning operation assigns the clarity scores based on at least one of a number of peaks, flatness, and a number of zero slopes in the motion waveform.

6. The method of claim 1, further comprising assigning clarity scores to the MATs associated with the map points.

7. The method of claim 6, wherein, when a first map point has a corresponding clarity above a select first level indicative of a clear motion waveform morphology, a MAT associated with the first map point is not modified based on MATs for the corresponding neighboring map points.

8. The method of claim 6, wherein, when a second map point has a corresponding clarity below a select second level indicative of an unclear motion waveform morphology, a MAT associated with the second map point is modified based

on MATs for the corresponding neighboring map points that have higher clarity relative to the clarity of the second map point.

9. The method of claim 6, wherein, when a third map point has a corresponding clarity below a select third level indicative of an unclear motion waveform morphology, a MAT associated with the third map point is discarded and excluded from analysis.

10. The method of claim 1, wherein the identifying operation excludes from the group of the neighboring map points any map points that are further than a predetermined radius away from the current map point.

11. The method of claim 1, further comprising calculating extents of motion (EMs) for the corresponding map points.

12. The method of claim 5, further comprising assigning clarity scores to the MATs and the EMs associated with the corresponding map points.

13. A system for characterizing motion data collected by cardiovascular navigation system (CNS), the system comprising:

- a plurality of physiological sensors configured to be positioned adjacent to a plurality of map points on a heart, wherein the physiological sensors acquire point specific (PS) motion data at the corresponding map points, the PS motion data indicates an amount of motion that occurred at the map points on a wall of the heart during at least one cardiac cycle;
- a PS motion data analysis circuit module configured to determine from the map points a mechanical activation time (MAT); and
- a MAT modification circuit module configured to modify the MAT of a selected map point based on the MATs corresponding to at least a subset of the map points.

14. The system of claim 13, wherein the PS motion data defines a motion waveform at the corresponding map point, where the motion waveform represents at least one of a displacement, strain, or strain rate over a select period of time, the calculating operation calculating the MATs based on the motion waveforms.

15. The system of claim 14, further comprising a MAT analysis circuit configured to assign a clarity score to the motion waveform based on a distinctiveness of a feature of interest within the motion waveforms used to determine the MATs and at least one of a number of peaks, flatness, and a number of zero slopes in the motion waveform.

16. The system of claim 13, further comprising a MAT analysis circuit configured to assign a clarity score to the calculated MATs.

17. The system of claim 13, wherein the subset of the map points are within a predetermined radius of the selected map point.

18. The system of claim 17, wherein the subset of the map points and the select map point does not include map points having a corresponding clarity score below a select third level indicative of an unclear motion waveform morphology.

19. The system of claim 17, wherein the select map point has a corresponding clarity score below a select second level indicative of an unclear motion waveform morphology, the subset of the map points have higher clarity scores relative to the select map point.

20. The system of claim 17, wherein the select map point does not have a corresponding clarity score above a select first level indicative of a clear motion waveform morphology.

\* \* \* \* \*

|                |                                                                                                               |         |            |
|----------------|---------------------------------------------------------------------------------------------------------------|---------|------------|
| 专利名称(译)        | 基于相邻地图点来表征运动数据的方法和系统                                                                                          |         |            |
| 公开(公告)号        | <a href="#">US20150313511A1</a>                                                                               | 公开(公告)日 | 2015-11-05 |
| 申请号            | US14/270181                                                                                                   | 申请日     | 2014-05-05 |
| [标]申请(专利权)人(译) | 标兵                                                                                                            |         |            |
| 申请(专利权)人(译)    | PACESETTER INC.                                                                                               |         |            |
| 当前申请(专利权)人(译)  | PACESETTER , INC.                                                                                             |         |            |
| [标]发明人         | NABUTOVSKY YELENA<br>RAZAVI HODA                                                                              |         |            |
| 发明人            | NABUTOVSKY, YELENA<br>RAZAVI, HODA                                                                            |         |            |
| IPC分类号         | A61B5/11 A61B5/06 A61B5/00 A61B5/042                                                                          |         |            |
| CPC分类号         | A61B5/1102 A61B5/7278 A61B5/061 A61B5/042 A61B5/1126 A61B5/0422 A61B5/062 A61B5/1107<br>A61B5/6869 A61B5/7289 |         |            |
| 其他公开文献         | US9364170                                                                                                     |         |            |
| 外部链接           | <a href="#">Espacenet</a> <a href="#">USPTO</a>                                                               |         |            |

#### 摘要(译)

提供了一种用于表征运动数据的方法和系统。该方法和系统获得多个地图点的点特定 ( PS ) 运动数据。 PS 运动数据指示在至少一个心动周期期间在心脏壁上的相应地图点处发生的运动量。该方法和系统, 计算地图点的机械激活时间 ( MAT ), 识别当前地图点的一组相邻地图点, 并基于对应于至少一部分的 MAT 修改对应于当前地图点的 MAT 相邻地图点组的一部分。此外, 该方法和系统针对至少一部分地图点重复识别和修改操作。

