



US 20170042488A1

(19) **United States**

(12) **Patent Application Publication**  
**Muhsin**

(10) **Pub. No.: US 2017/0042488 A1**  
(43) **Pub. Date: Feb. 16, 2017**

(54) **MEDICAL MONITORING ANALYSIS AND  
REPLAY INCLUDING INDICIA RESPONSIVE  
TO LIGHT ATTENUATED BY BODY TISSUE**

*A61B 5/1455* (2006.01)  
*A61B 5/024* (2006.01)

(52) **U.S. Cl.**  
CPC ..... *A61B 5/7445* (2013.01); *A61B 5/14551*  
(2013.01); *A61B 5/02416* (2013.01); *A61B*  
*5/0008* (2013.01); *A61B 5/0022* (2013.01);  
*A61B 5/4839* (2013.01); *A61B 5/08* (2013.01);  
*A61B 5/746* (2013.01); *G06T 11/206*  
(2013.01)

(71) Applicant: **Masimo Corporation**, Irvine, CA (US)

(72) Inventor: **Bilal Muhsin**, San Clemente, CA (US)

(21) Appl. No.: **15/233,244**

(22) Filed: **Aug. 10, 2016**

(57) **ABSTRACT**


**Related U.S. Application Data**

(60) Provisional application No. 62/203,792, filed on Aug. 11, 2015.

The present disclosure includes a medical monitoring hub as the center of monitoring for a monitored patient. The hub is configured to receive and process a plurality of physiological parameters associated with the patient. The hub includes advanced analytical presentation views configured to provide timely, clinically-relevant, actionable information to care providers. In certain embodiments, the monitoring hub stores and is able to replay previously presented data reflective of the patient's condition.

**Publication Classification**

(51) **Int. Cl.**  
*A61B 5/00* (2006.01)  
*G06T 11/20* (2006.01)  
*A61B 5/08* (2006.01)

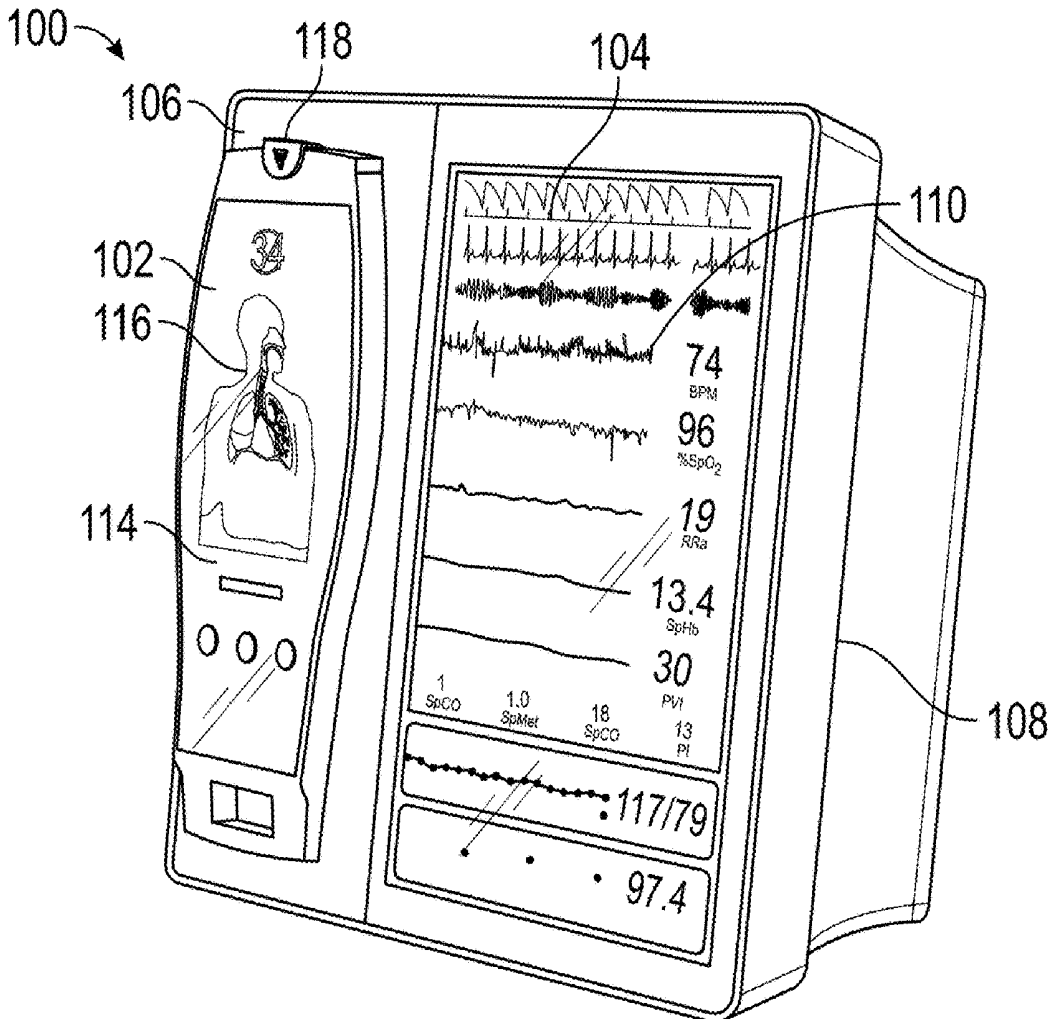

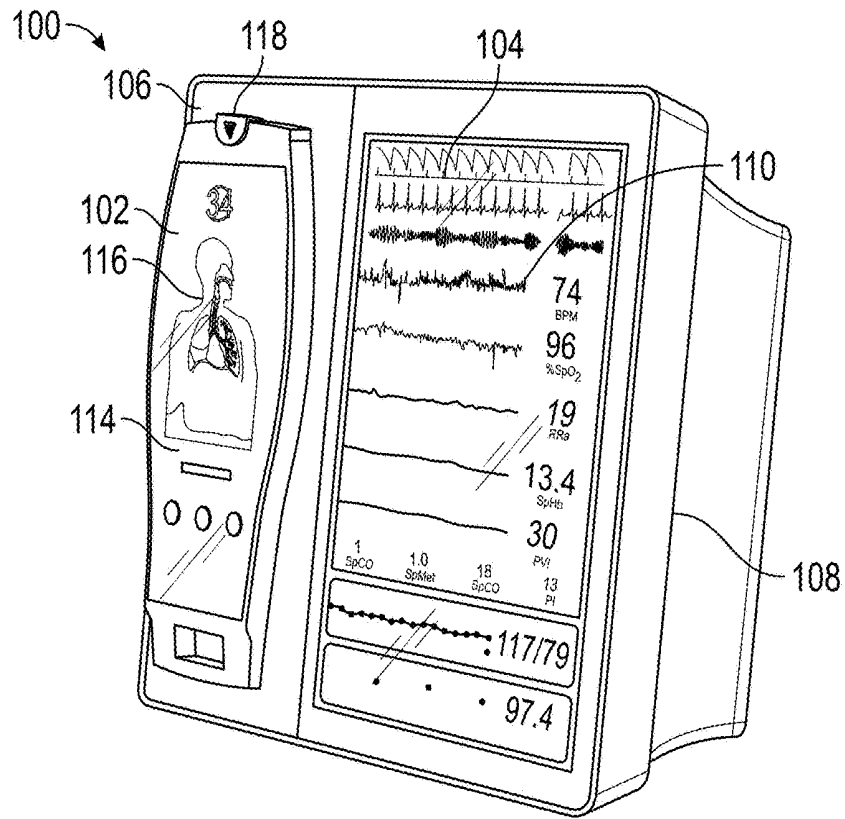


FIG. 1A

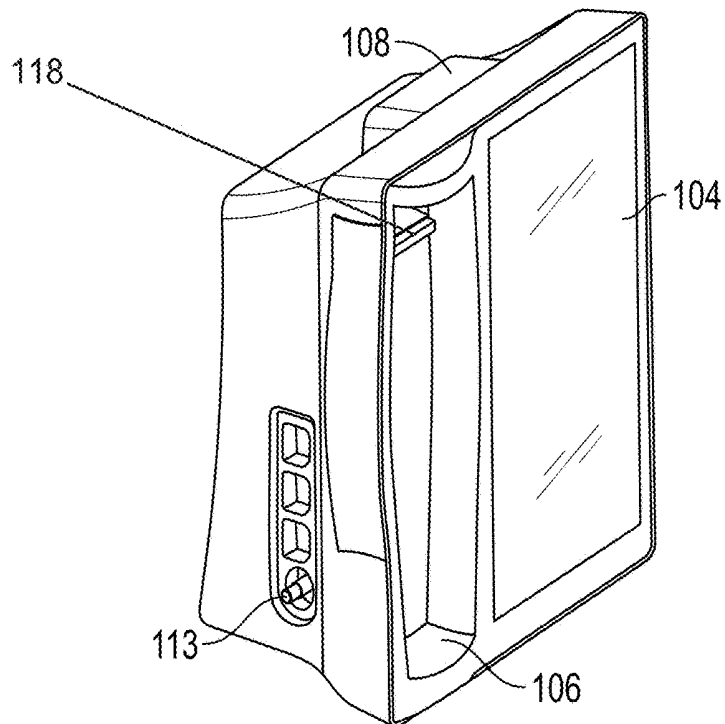


FIG. 1B

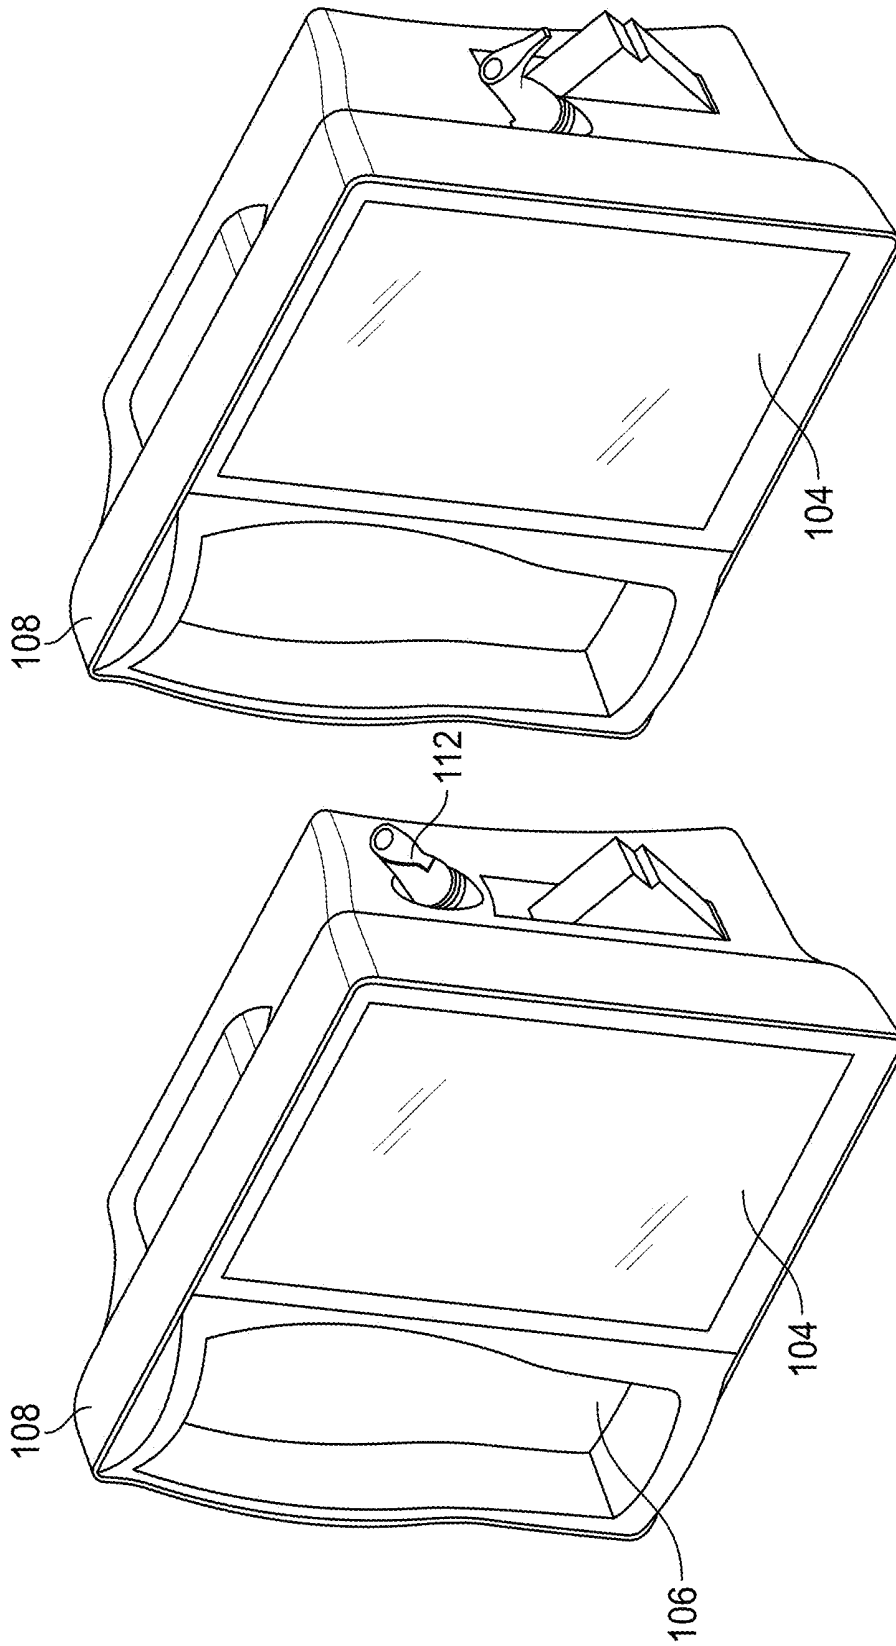


FIG. 1C

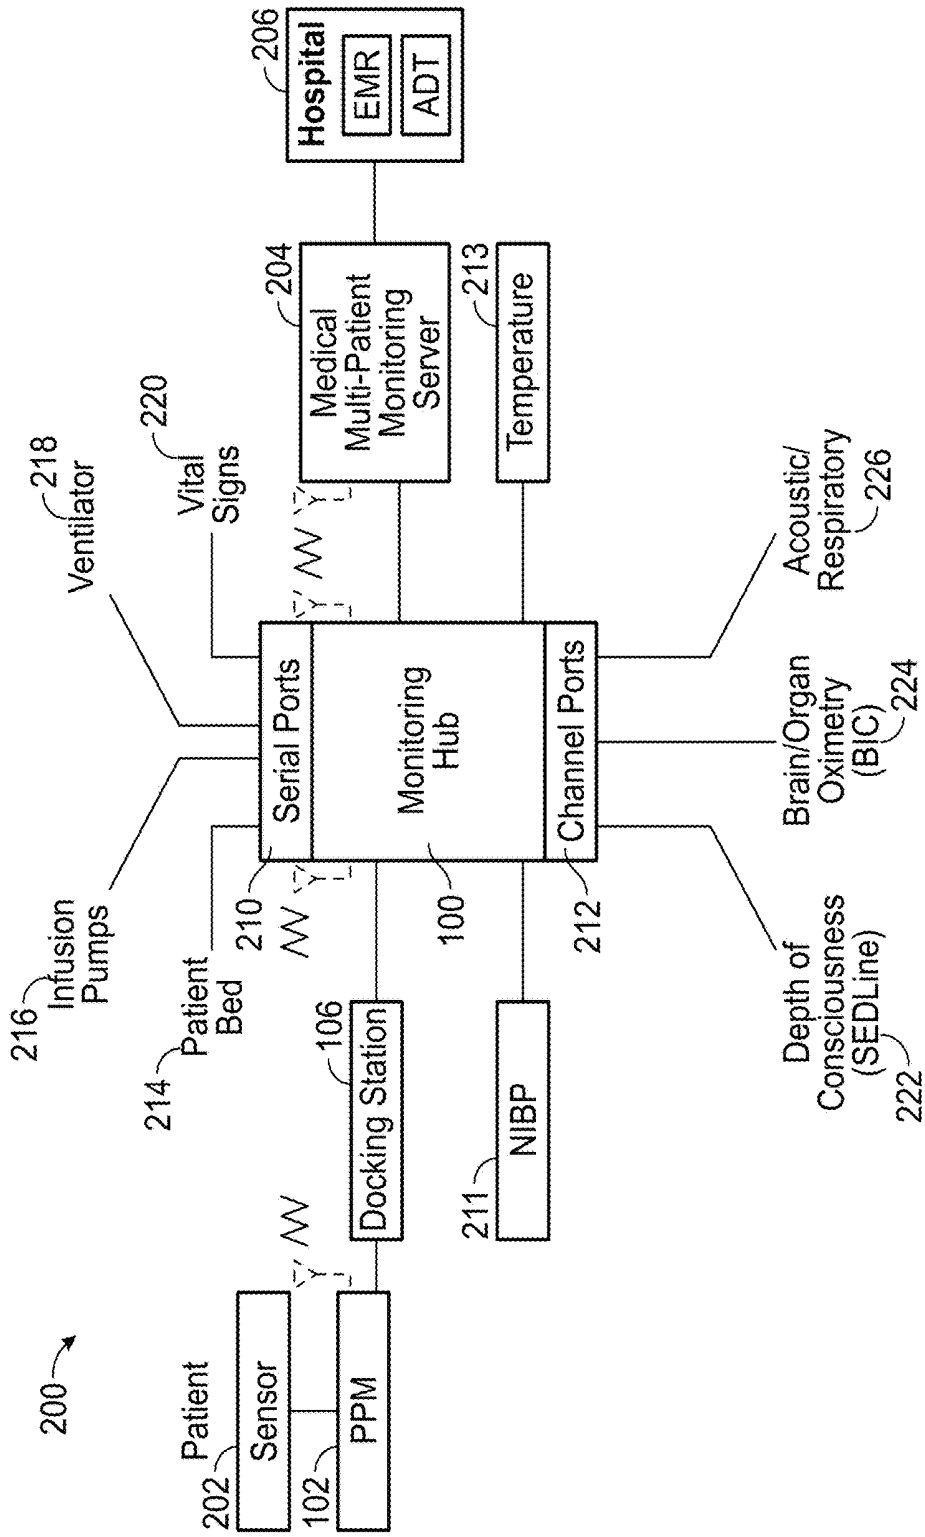


FIG. 2

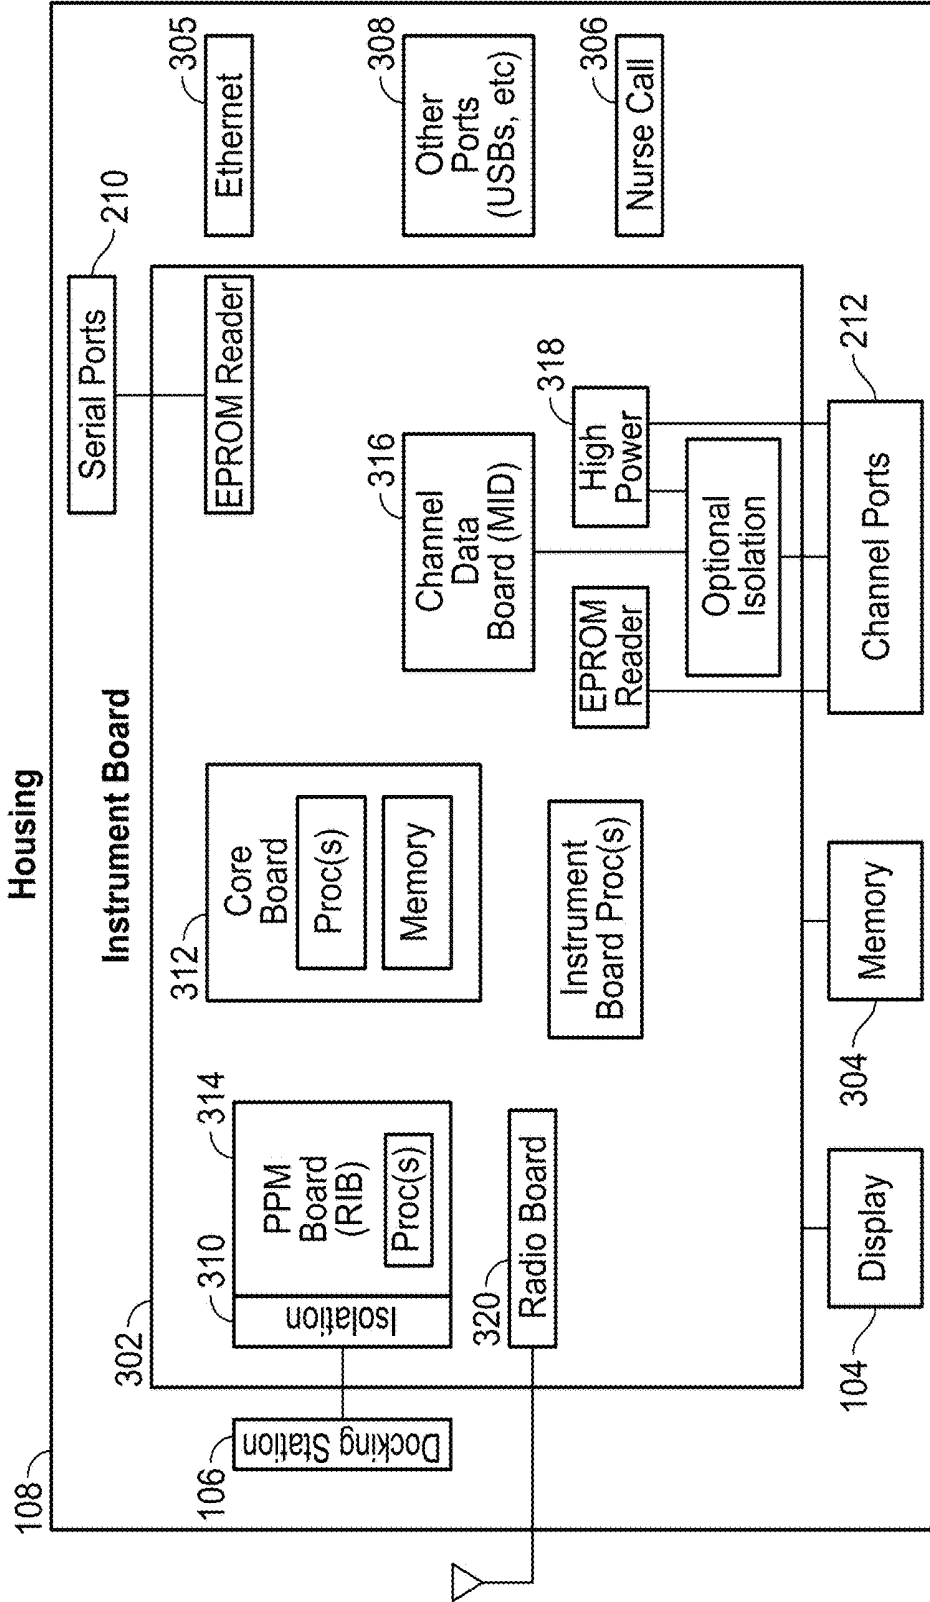


FIG. 3

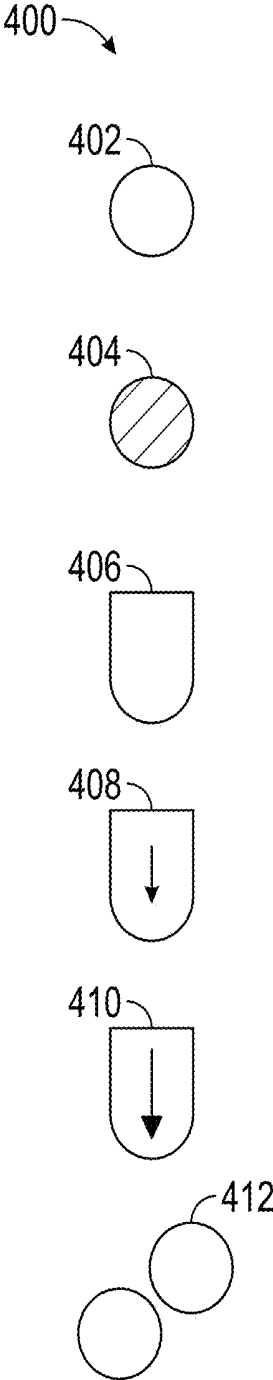


FIG. 4

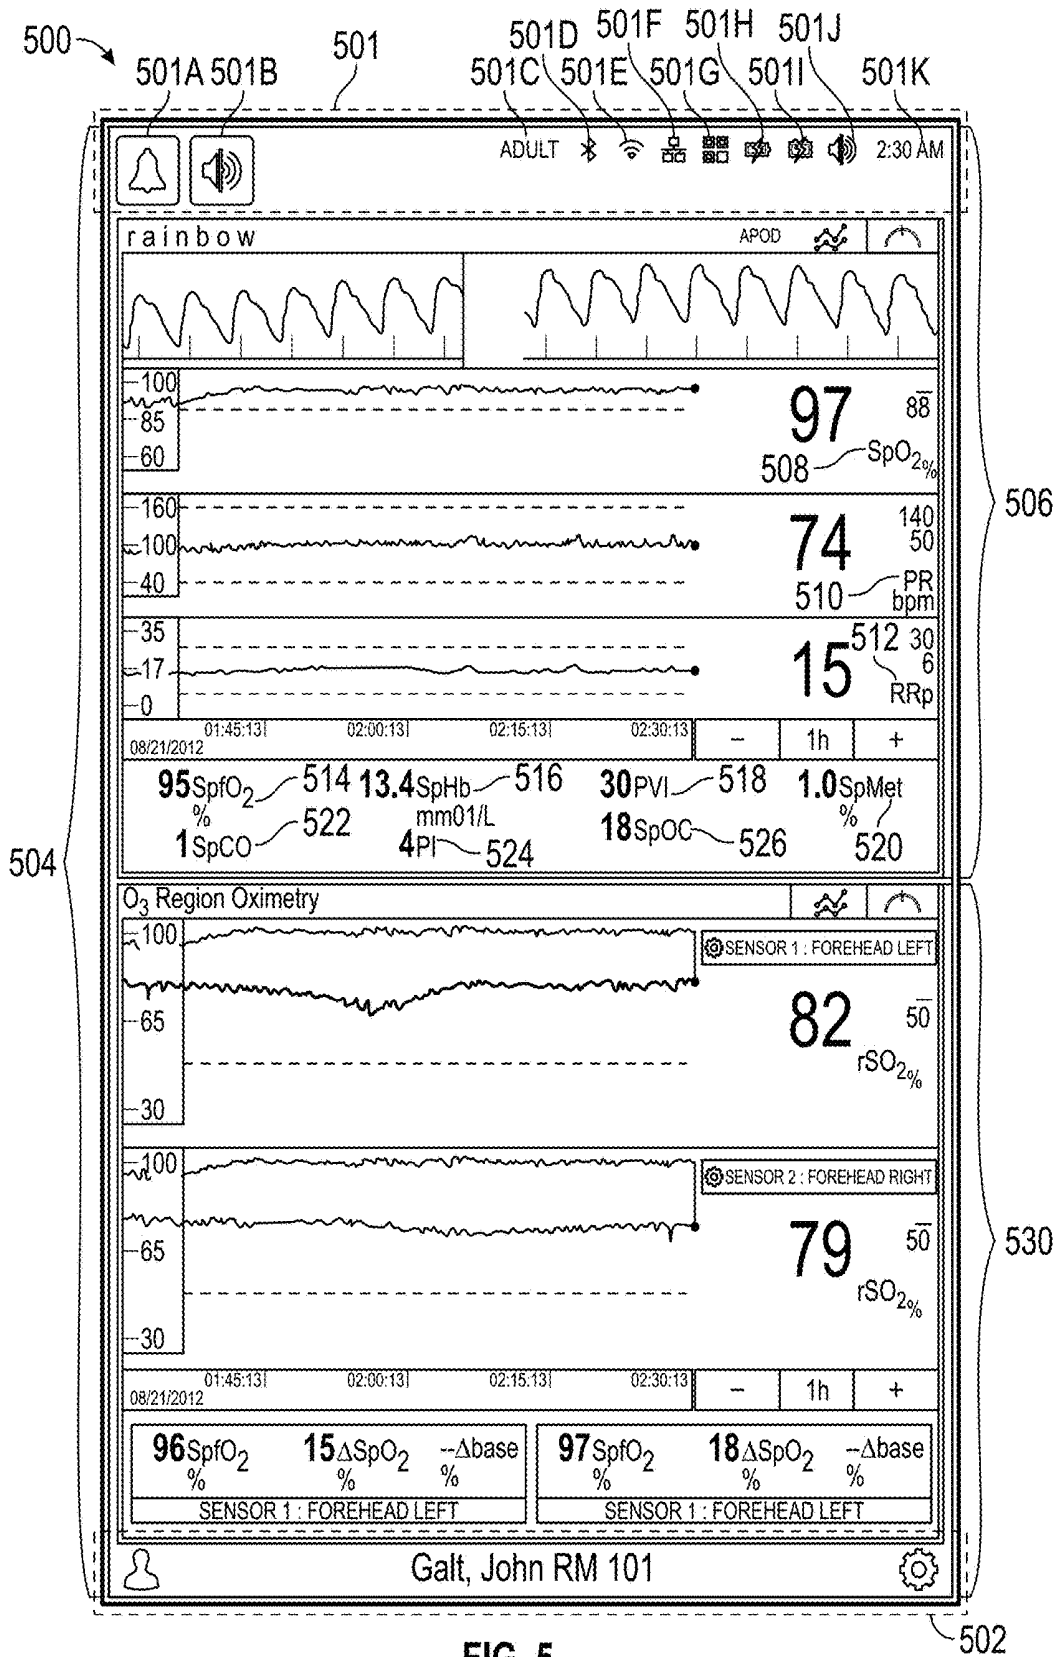


FIG. 5

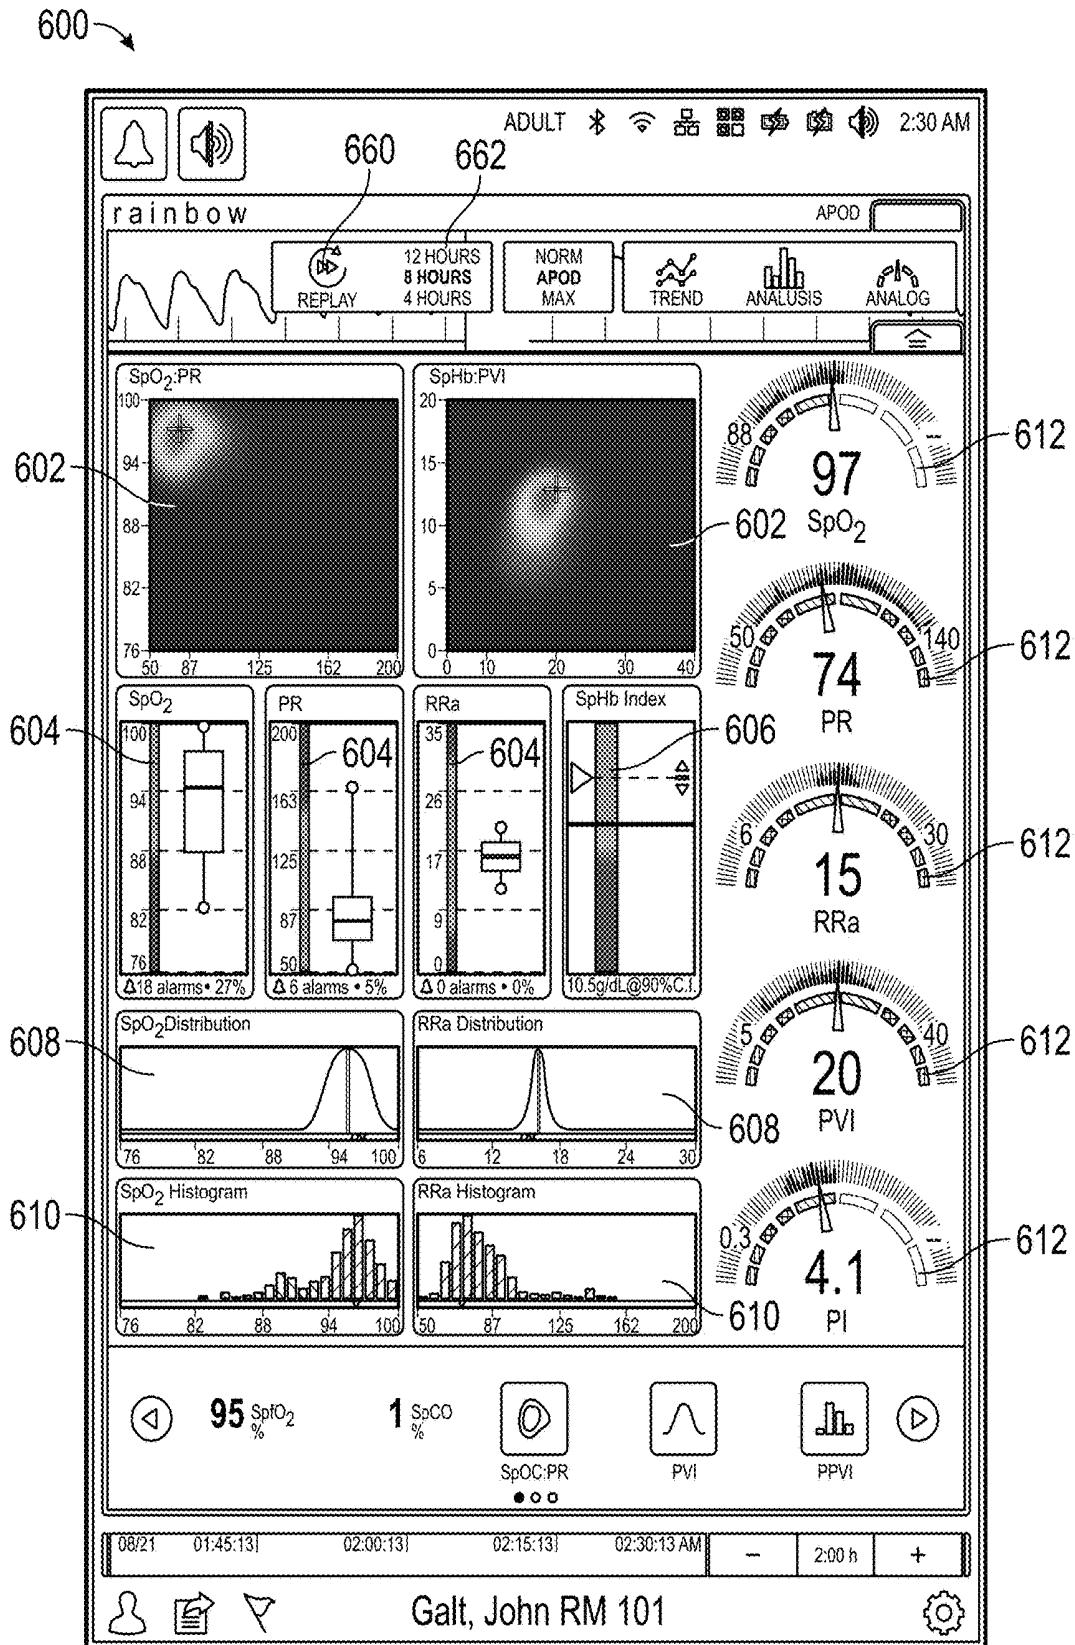


FIG. 6A

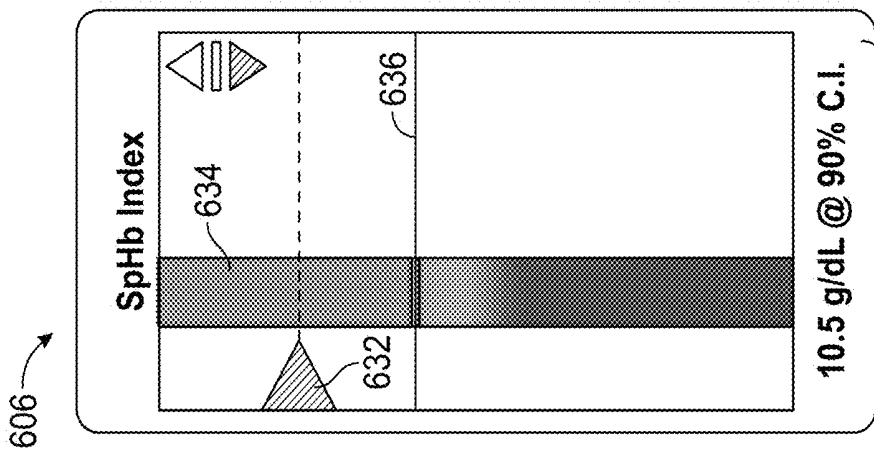


FIG. 6D

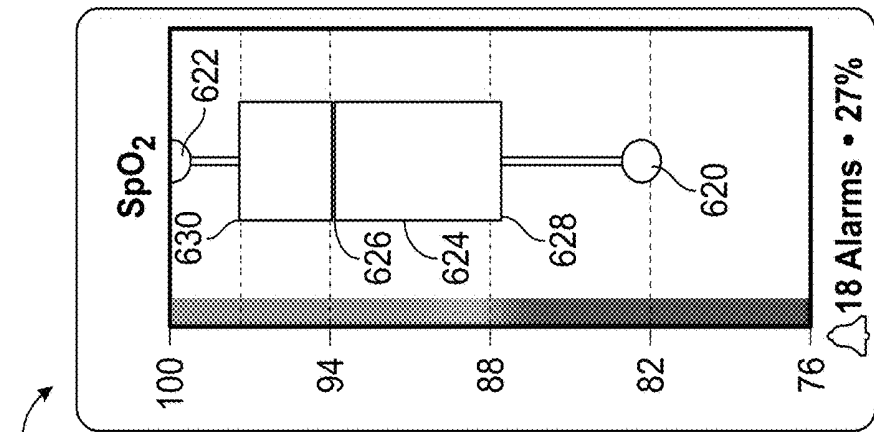


FIG. 6C

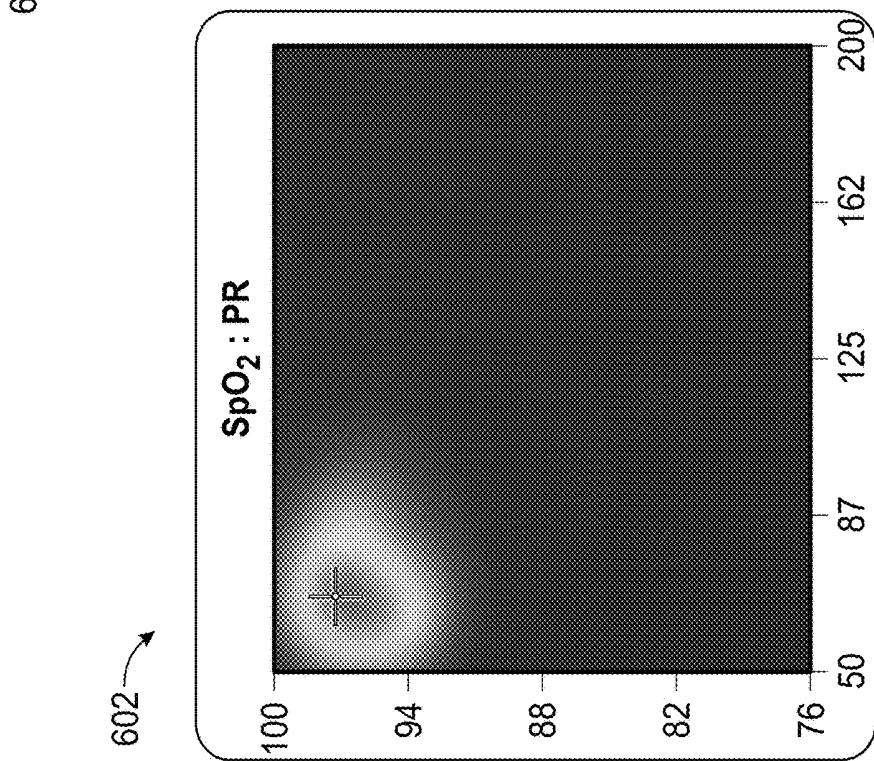


FIG. 6B

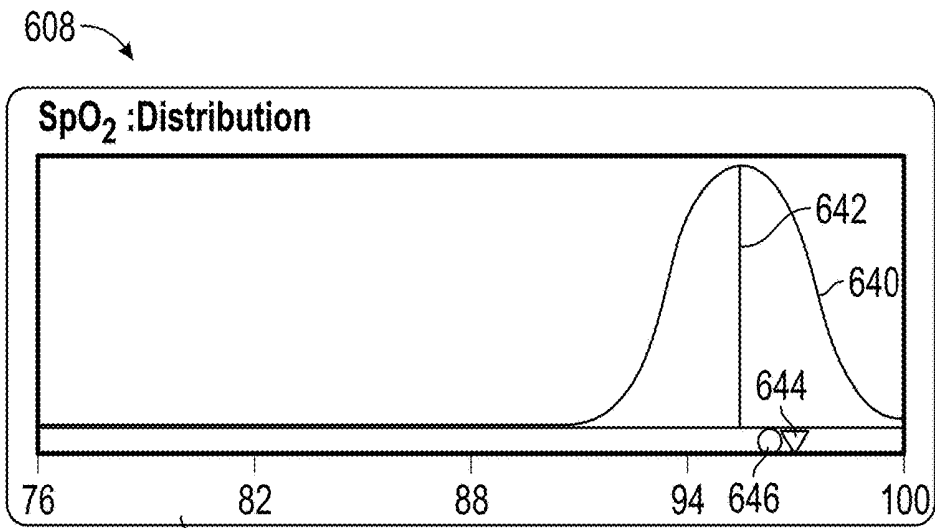


FIG. 6E

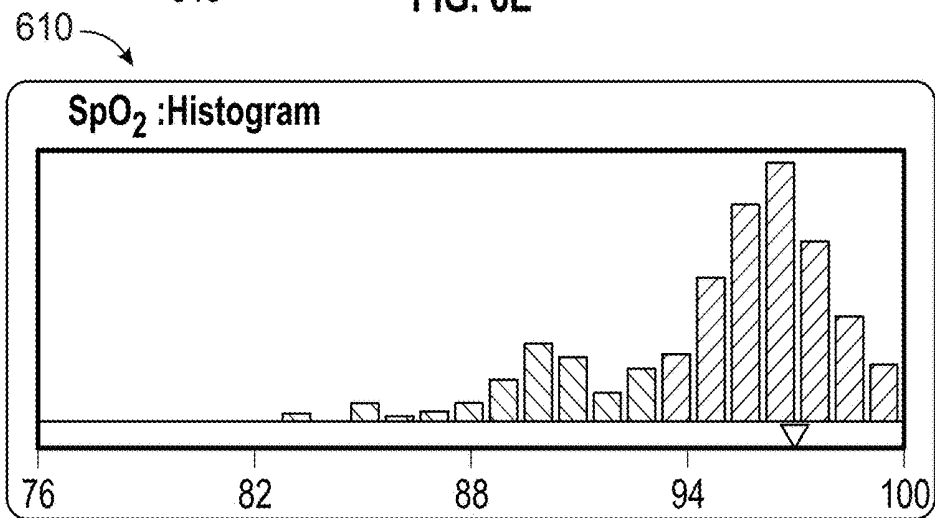


FIG. 6F

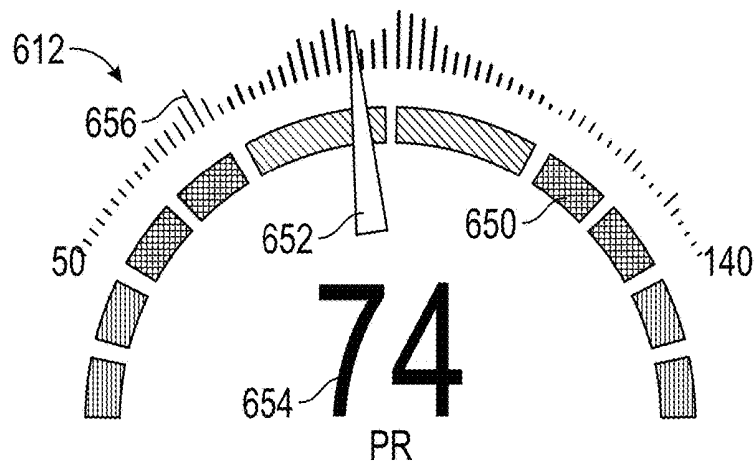


FIG. 6G

700

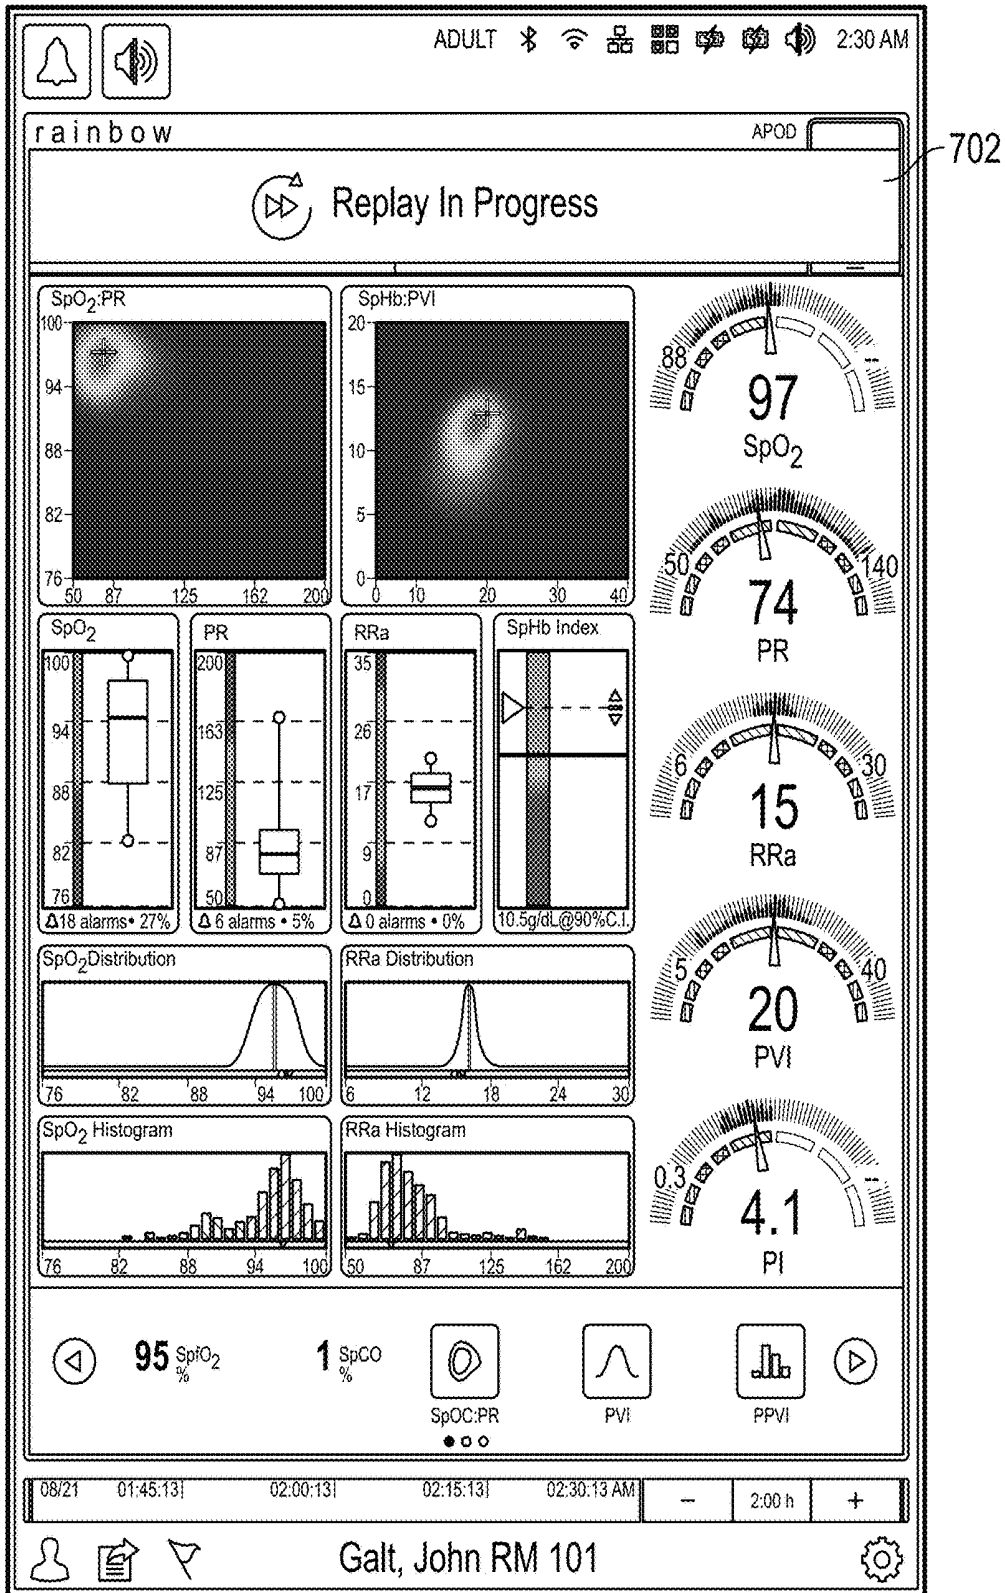


FIG. 7

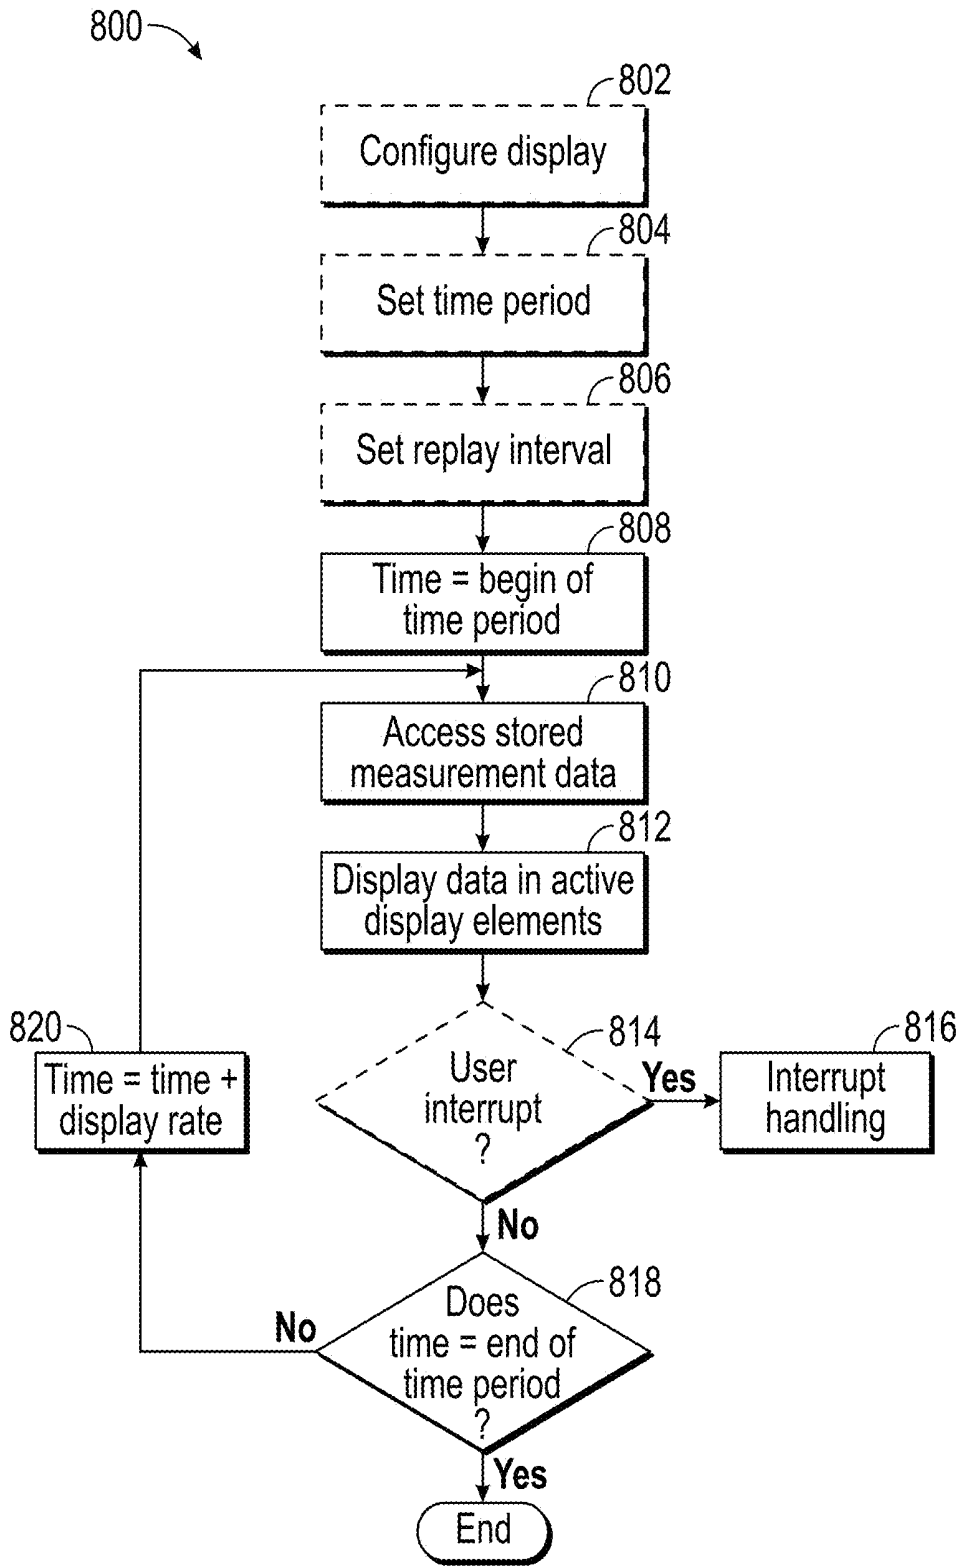


FIG. 8

**MEDICAL MONITORING ANALYSIS AND  
REPLAY INCLUDING INDICIA RESPONSIVE  
TO LIGHT ATTENUATED BY BODY TISSUE**

**INCORPORATION BY REFERENCE TO ANY  
PRIORITY APPLICATIONS**

[0001] The present application claims priority benefit under 35 U.S.C. §119(e) to U.S. Provisional Application No. 62/203,792, filed Aug. 11, 2015, which is hereby incorporated by reference in its entirety herein. Any and all applications for which a foreign or domestic priority claim is identified in the Application Data Sheet as filed with the present application are hereby incorporated by reference under 37 CFR 1.57.

**FIELD**

[0002] The present disclosure relates generally to a patient monitor and medical data communication hub and specifically to a patient monitor including display elements for presenting measurement information, often over a time period, to a caregiver.

**BACKGROUND**

[0003] Today's patient monitoring environments are crowded with sophisticated and often electronic medical devices servicing a wide variety of monitoring and treatment endeavors for a given patient. Generally, many if not all of the devices are from differing manufactures, and many may be portable devices. The devices may not communicate with one another and each may include its own control, display, alarms, configurations and the like. Complicating matters, caregivers often desire to associate all types of measurement and data from these devices with a specific patient. Patient information entry often occurs at each device. Sometimes, the disparity in devices leads to a need to simply print and store paper from each device in a patient's file for caregiver review.

[0004] Thus, while the electronic collection of physiological data associated with the patient's condition has increased, the ability to synthesize the collected patient data into timely, clinically-relevant, actionable information remains a challenge.

**SUMMARY**

[0005] Based on at least the foregoing, a solution is needed that coordinates the various medical devices treating or monitoring a patient and the measurement data being generated by such devices. Embodiments of such a solution may include a medical hub that presents, via graphical display, a variety of analytical presentation views that deliver to the caregiver easily-seen, intuitive, visual indications of the status and condition of the patient being monitored. In an embodiment, the analytical graphical views may advantageously be replayed for analysis of critical events in the patient's care, or to simply review the patient's physiological activity over a period of time. In an embodiment, the replays of several physiological parameters may be played synchronously, providing a broad perspective of the patient's historical activity.

[0006] According to an embodiment of the present disclosure, a medical monitoring hub is configured to monitor physiological parameters of a patient. The hub includes a first communication port configured to receive a first signal

indicative a first physiological parameter associated with the patient. The monitor also includes a display configured to present analytical presentation views to the user. The monitor includes at least one processor configured to process the received first signal and to cause a first view to be presented on at least a portion of the display. The first view is adapted to present first data indicative of the first physiological parameter collected over a first period of time. The hub includes a storage device configured to store the presented first data, and the processor is further configured to replay the stored first data on the display.

[0007] In certain embodiments of the present disclosure, various analytical presentation views are disclosed to help clinicians easily and intuitively interpret the patient data that is received by the monitoring hub. Heat maps are disclosed which provide a two-dimensional graphical representation of a relationship between two measured physiological parameters over a specified period of time. Advantageously, heat maps use color to identify areas in the graph where the data is concentrated. For example, areas where the data is highly concentrated can be presented in a first color (e.g., red), while areas in which the data is less highly concentrated can be presented in a second color (e.g., blue).

[0008] Also disclosed are box-and-whisker plots which visually present the range of physiological parameter measurements received over a specified or pre-determined period of time. Additionally, the boundaries of the quartiles in which the data lies are presented by the box-and-whisker plots. Advantageously, the box-and-whisker plot readily presents to the user the degree of spread, or dispersion of the measured data, as well as the skewness in the data, including outlier measurements.

[0009] Index box views are disclosed as well. An index box view presents a current measured state of a physiological parameter relative to ranges identified as, for example, acceptable, cautionary, and emergent, using colors and other visual cues to readily indicate the measured state of the patient.

[0010] The present disclosure also describes distribution analytical presentation views which present a statistical distribution (e.g., a Gaussian distribution) of physiological parameter measurements over a specified or pre-defined period of time. Similarly, the present disclosure describes histogram analytical presentation views which provide yet another graphical representation of a measured physiological parameter data. A histogram represents an estimate of the statistical (or probability) distribution of a continuous variable, such as a continuously measured physiological parameter. Thus, rather than providing a statistical distribution (i.e., a probabilistic model) that best fits or corresponds to the measured data, the histogram reflects the actual measured data collected.

[0011] The present disclosure also includes gauge-histogram analytical presentation views, which provide a combination of analog, digital, and histogram display indicia. Advantageously, the gauge-histogram analytical presentation view provides to the clinician a substantial amount of information related to the measured physiological parameter in an intuitive and visually accessible format.

[0012] In use, the clinician is provided a great deal of flexibility in arranging and configuring the disclosed analytical presentation views of the present disclosure. Thus,

the clinician is provided a monitoring environment that can be customized to the clinician's and/or patient's specific needs.

[0013] For purposes of summarizing the disclosure, certain aspects, advantages and novel features are discussed herein. It is to be understood that not necessarily all such aspects, advantages or features will be embodied in any particular embodiment of the invention, and an artisan would recognize from the disclosure herein a myriad of combinations of such aspects, advantages or features.

#### BRIEF DESCRIPTION OF THE DRAWINGS

[0014] Various embodiments will be described hereinafter with reference to the accompanying drawings. The drawings and the associated descriptions are provided to illustrate embodiments of the present disclosure and do not limit the scope of the claims. In the drawings, similar elements have similar reference numerals.

[0015] FIGS. 1A-1C illustrate perspective views of an exemplary medical monitoring hub according to an embodiment of the disclosure. For example, FIG. 1A illustrates the hub with an exemplary docked portable patient monitor; FIG. 1B illustrates the hub with a set of medical ports and a noninvasive blood pressure input; and FIG. 1C illustrates the hub with various exemplary temperature sensors attached thereto, all according to various embodiments of the disclosure.

[0016] FIG. 2 illustrates a simplified block diagram of an exemplary monitoring environment including the hub of FIG. 1, according to an embodiment of the disclosure.

[0017] FIG. 3 illustrates a simplified exemplary hardware block diagram of the hub of FIG. 1, according to an embodiment of the disclosure.

[0018] FIG. 4 is a finger control gesture legend for a touchscreen interface according to an embodiment of the disclosure.

[0019] FIG. 5 is an illustration of a display view according to an embodiment of the disclosure.

[0020] FIG. 6A illustrates an exemplary display screen showing various analytical presentation views for presenting received and processed data according to an embodiment of the disclosure.

[0021] FIG. 6B illustrates a heat map analytical presentation view according to an embodiment of the disclosure.

[0022] FIG. 6C illustrates a box-and-whisker analytical presentation view according to an embodiment of the disclosure.

[0023] FIG. 6D illustrates an index analytical presentation view according to an embodiment of the disclosure.

[0024] FIG. 6E illustrates a distribution analytical presentation view according to an embodiment of the disclosure.

[0025] FIG. 6F illustrates a histogram analytical presentation view according to an embodiment of the disclosure.

[0026] FIG. 6G illustrates a gauge-histogram analytical presentation view according to an embodiment of the disclosure.

[0027] FIG. 7 illustrates an exemplary display screen showing a replay feature according to an embodiment of the disclosure.

[0028] FIG. 8 is a flowchart illustrating a replay process according to an embodiment of the disclosure.

[0029] While the foregoing "Brief Description of the Drawings" references generally various embodiments of the disclosure, an artisan will recognize from the disclosure

herein that such embodiments are not mutually exclusive. Rather, the artisan would recognize a myriad of combinations of some or all of such embodiments.

#### DETAILED DESCRIPTION

[0030] The present disclosure relates to a medical monitoring hub configured to be the center of monitoring activity for a given patient. In an embodiment, the hub comprises a large easily readable display, such as an about ten (10) inch display dominating the majority of real estate on a front face of the hub. The display could be much larger or much smaller depending upon design constraints. However, for portability and current design goals, the preferred display is roughly sized proportional to the vertical footprint of one of a dockable portable patient monitor. Other considerations are recognizable from the disclosure herein by those in the art.

#### Configurable Replay Display

[0031] In an embodiment, the display is configurable by dragging and dropping gestures to populate the display with elements a caregiver prefers to view for a particular user. The elements may include some or all of a heat map, a box-and-whisker plot, a distribution plot, a histogram, an analog gage, and an analog gage combined with a histogram. Once configured, the hub processor may allow for the replay of selected measurement data, data responsive to the measurement data, or combinations of measurement data over a selected or default time period at a selected or default display rate. Advantageously, such configuration and replay provide a powerful tool for a caregiver to review the patient's condition over virtually any period of time desired.

#### Monitoring Hub

[0032] The display provides measurement data for a wide variety of monitored parameters for the patient under observation in numerical or graphic form, and in various embodiments, is automatically configured based on the type of data and information being received at the hub. In an embodiment, the hub is moveable, portable, and mountable so that it can be positioned to convenient areas within a caregiver environment. For example, the hub is collected within a singular housing.

[0033] In an embodiment, the hub may advantageously receive data from a portable patient monitor while docked or undocked from the hub. Typical portable patient monitors, such as oximeters or co-oximeters can provide measurement data for a large number of physiological parameters derived from signals output from optical and/or acoustic sensors, electrodes, or the like. The physiological parameters include, but not limited to oxygen saturation, carboxy hemoglobin, methemoglobin, total hemoglobin, glucose, pH, bilirubin, fractional saturation, pulse rate, respiration rate, components of a respiration cycle, indications of perfusion including perfusion index, signal quality and/or confidences, plethysmograph data, indications of wellness or wellness indexes or other combinations of measurement data, audio information responsive to respiration, ailment identification or diagnosis, blood pressure, patient and/or measurement site temperature, depth of sedation, organ or brain oxygenation, hydration, measurements responsive to metabolism, combinations of the same or the like, to name a few. In other

embodiments, the hub may output data sufficient to accomplish closed-loop drug administration in combination with infusion pumps or the like.

**[0034]** In an embodiment, the hub communicates with other devices in a monitoring environment that are interacting with the patient in a number of ways. For example, the hub advantageously receives serial data from other devices without necessitating their reprogramming or that of the hub. Such other devices include pumps, ventilators, all manner of monitors monitoring any combination of the foregoing parameters, ECG/EEG/EKG devices, electronic patient beds, and the like. Moreover, the hub advantageously receives channel data from other medical devices without necessitating their reprogramming or that of the hub. When a device communicates through channel data, the hub may advantageously alter the large display to include measurement information from that device. Additionally, the hub accesses nurse call systems to ensure that nurse call situations from the device are passed to the appropriate nurse call system.

**[0035]** The hub also communicates with hospital systems to advantageously associate incoming patient measurement and treatment data with the patient being monitored. For example, the hub may communicate wirelessly or otherwise to a multi-patient monitoring system, such as a server or collection of servers, which in turn many communicate with a caregiver's data management systems, such as, for example, an Admit, Discharge, Transfer ("ADT") system and/or an Electronic Medical Records ("EMR") system. The hub advantageously associates the data flowing through it with the patient being monitored thereby providing the electronic measurement and treatment information to be passed to the caregiver's data management systems without the caregiver associating each device in the environment with the patient.

**[0036]** In an embodiment, the hub advantageously includes a reconfigurable and removable docking station. The docking station may dock additional layered docking stations to adapt to different patient monitoring devices. Additionally, the docking station itself is modularized so that it may be removed if the primary dockable portable patient monitor changes its form factor. Thus, the hub is flexible in how its docking station is configured.

**[0037]** In an embodiment, the hub includes a large memory for storing some or all of the data it receives, processes, and/or associates with the patient, and/or communications it has with other devices and systems. Some or all of the memory may advantageously comprise removable SD memory.

**[0038]** The hub communicates with other devices through at least (1) the docking station to acquire data from a portable monitor, (2) innovative universal medical connectors to acquire channel data, (3) serial data connectors, such as RJ ports to acquire output data, (4) Ethernet, USB, and nurse call ports, (5) Wireless devices to acquire data from a portable monitor, (6) other wired or wireless communication mechanisms known to an artisan. The universal medical connectors advantageously provide optional electrically isolated power and communications, are designed to be smaller in cross section than isolation requirements. The connectors and the hub communicate to advantageously translate or configure data from other devices to be usable and displayable for the hub. In an embodiment, a software developers kit ("SDK") is provided to a device manufacturer to estab-

lish or define the behavior and meaning of the data output from their device. When the output is defined, the definition is programmed into a memory residing in the cable side of the universal medical connector and supplied as an original equipment manufacturer ("OEM") to the device provider. When the cable is connected between the device and the hub, the hub understands the data and can use it for display and processing purposes without necessitating software upgrades to the device or the hub. In an embodiment, the hub can negotiate the schema and even add additional compression and/or encryption. Through the use of the universal medical connectors, the hub organizes the measurement and treatment data into a single display and alarm system effectively and efficiently bringing order to the monitoring environment.

**[0039]** As the hub receives and tracks data from other devices according to a channel paradigm, the hub may advantageously provide processing to create virtual channels of patient measurement or treatment data. In an embodiment, a virtual channel may comprise a non-measured parameter that is, for example, the result of processing data from various measured or other parameters. An example of such a parameter includes a wellness indicator derived from various measured parameters that give an overall indication of the wellbeing of the monitored patient. An example of a wellness parameter is disclosed in U.S. patent application Ser. Nos. 13/269,296, 13/371,767 and 12/904,925, by the assignee of the present disclosure and incorporated by reference herein. By organizing data into channels and virtual channels, the hub may advantageously time-wise synchronize incoming data and virtual channel data.

**[0040]** The hub also receives serial data through serial communication ports, such as RJ connectors. The serial data is associated with the monitored patient and passed on to the multi-patient server systems and/or caregiver backend systems discussed above. Through receiving the serial data, the caregiver advantageously associates devices in the caregiver environment, often from varied manufacturers, with a particular patient, avoiding a need to have each individual device associated with the patient and possible communicating with hospital systems. Such association is vital as it reduces caregiver time spent entering biographic and demographic information into each device about the patient. Moreover, in an embodiment, through the SDK the device manufacturer may advantageously provide information associated with any measurement delay of their device, thereby further allowing the hub to advantageously time-wise synchronize serial incoming data and other data associated with the patient.

**[0041]** In an embodiment, when a portable patient monitor is docked, and it includes its own display, the hub effectively increases its display real estate. For example, in an embodiment, the portable patient monitor may simply continue to display its measurement and/or treatment data, which may be now duplicated on the hub display, or the docked display, may alter its display to provide additional information. In an embodiment, the docked display, when docked, presents anatomical graphical data of, for example, the heart, lungs, organs, the brain, or other body parts being measured and/or treated. The graphical data may advantageously animate similar to and in concert with the measurement data. For example, lungs may inflate in approximate correlation to the measured respiration rate and/or the determined inspiration/expiration portions of a respiration cycle, the heart may beat

according to the pulse rate, may beat generally along understood actual heart contraction patterns, the brain may change color or activity based on varying depths of sedation, or the like. In an embodiment, when the measured parameters indicate a need to alert a caregiver, a changing severity in color may be associated with one or more displayed graphics, such as the heart, lungs, brain, organs, circulatory system or portions thereof, respiratory system or portions thereof, other body parts or the like. In still other embodiments, the body portions may include animations on where, when or how to attach measurement devices.

[0042] The hub may also advantageously overlap parameter displays to provide additional visual information to the caregiver. Such overlapping may be user definable and configurable. The display may also incorporate analog-appearing icons or graphical indicia.

[0043] In the interest of clarity, not all features of an actual implementation are described in this specification. An artisan will of course be appreciate that in the development of any such actual implementation (as in any development project), numerous implementation-specific decisions must be made to achieve a developers' specific goals and sub-goals, such as compliance with system- and business-related constraints, which will vary from one implementation to another. Moreover, it will be appreciated that such a development effort might be complex and time-consuming, but would nevertheless be a routine undertaking of device engineering for those of ordinary skill having the benefit of this disclosure.

[0044] To facilitate a complete understanding of the disclosure, the remainder of the detailed description describes the disclosure with reference to the drawings, wherein like reference numbers are referenced with like numerals throughout.

#### Embodiments of Monitoring Hub

[0045] FIG. 1A illustrates a perspective view of an exemplary medical monitoring hub 100, which may also be referred to herein as a monitor 100, with an exemplary docked portable patient monitor 102 according to an embodiment of the disclosure. The hub 100 includes a display 104, and a docking station 106, which in an embodiment is configured to mechanically and electrically mate with the portable patient monitor 102, each housed in a movable, mountable and portable housing 108. The housing 108 includes a generally upright inclined shape configured to rest on a horizontal flat surface, although the housing 108 can be affixed in a wide variety of positions and mountings and comprise a wide variety of shapes and sizes.

[0046] In an embodiment, the display 104 may present a wide variety of measurement and/or treatment data in numerical, graphical, waveform, or other display indicia 110. In an embodiment, the display 104 occupies much of a front face of the housing 108, although an artisan will appreciate the display 104 may comprise a tablet or tabletop horizontal configuration, a laptop-like configuration or the like. Other embodiments may include communicating display information and data to a table computer, smartphone, television, or any display system recognizable to an artisan. The upright inclined configuration of FIG. 1A presents display information to a caregiver in an easily viewable manner.

[0047] FIG. 1B shows a perspective side view of an embodiment of the hub 100 including the housing 108, the

display 104, and the docking station 106 without a portable monitor docked. Also shown is a connector for noninvasive blood pressure 113.

[0048] In an embodiment, the housing 108 may also include pockets or indentations to hold additional medical devices, such as, for example, a blood pressure monitor or temperature sensor 112, such as that shown in FIG. 1C.

[0049] The monitor 102 may communicate with a variety of noninvasive and/or minimally invasive devices such as optical sensors with light emission and detection circuitry, acoustic sensors, devices that measure blood parameters from a finger prick, cuffs, ventilators, and the like. The monitor 102 may include its own display 114 presenting its own display indicia 116, discussed below with reference to FIGS. 19A-19J. The display indicia may advantageously change based on a docking state of the monitor 102. When undocked, the display indicia may include parameter information and may alter orientation based on, for example, a gravity sensor or accelerometer.

[0050] In an embodiment, the docking station 106 of the hub 100 includes a mechanical latch 118, or mechanically releasable catch to ensure that movement of the hub 100 doesn't mechanically detach the monitor 102 in a manner that could damage the same.

[0051] Although disclosed with reference to particular portable patient monitors 102, an artisan will recognize from the disclosure herein a large number and wide variety of medical devices that may advantageously dock with the hub 100. Moreover, the docking station 106 may advantageously electrically and not mechanically connect with the monitor 102, and/or wirelessly communicate with the same.

[0052] FIG. 2 illustrates a simplified block diagram of an exemplary monitoring environment 200 including the hub 100 of FIG. 1, according to an embodiment of the disclosure. As shown in FIG. 2, the environment may include the portable patient monitor 102 communicating with one or more patient sensors 202, such as, for example, oximetry optical sensors, acoustic sensors, blood pressure sensors, respiration sensors or the like. In an embodiment, additional sensors, such as, for example, a NIBP sensor or system 211 and a temperature sensor or sensor system 213 may communicate directly with the hub 100. The sensors 202, 211 and 213 when in use are typically in proximity to the patient being monitored if not actually attached to the patient at a measurement site.

[0053] As disclosed, the portable patient monitor 102 communicates with the hub 100, in an embodiment, through the docking station 106 when docked and, in an embodiment, wirelessly when undocked, however, such undocked communication is not required. The hub 100 communicates with one or more multi-patient monitoring servers 204 or server systems, such as, for example, those disclosed with in U.S. Pat. Pub. Nos. 2011/0105854, 2011/0169644, and 2007/0180140. In general, the server 204 communicates with caregiver backend systems 206 such as EMR and/or ADT systems. The server 204 may advantageously obtain through push, pull or combination technologies patient information entered at patient admission, such as demographical information, billing information, and the like. The hub 100 accesses this information to seamlessly associate the monitored patient with the caregiver backend systems 206. Communication between the server 204 and the monitoring hub 100 may be any recognizable to an artisan from

the disclosure herein, including wireless, wired, over mobile or other computing networks, or the like.

**[0054]** FIG. 2 also shows the hub 100 communicating through its serial data ports 210 and channel data ports 212. As disclosed in the foregoing, the serial data ports 210 may provide data from a wide variety of patient medical devices, including electronic patient bed systems 214, infusion pump systems 216 including closed loop control systems, ventilator systems 218, blood pressure or other vital sign measurement systems 220, or the like. Similarly, the channel data ports 212 may provide data from a wide variety of patient medical devices, including any of the foregoing, and other medical devices. For example, the channel data ports 212 may receive data from depth of consciousness monitors 222, such as those commercially available from SEDLine, brain or other organ oximeter devices 224, noninvasive blood pressure or acoustic devices 226, or the like. In an embodiment, channel device may include board-in-cable (“BIC”) solutions where the processing algorithms and the signal processing devices that accomplish those algorithms are mounted to a board housed in a cable or cable connector, which in some embodiments has no additional display technologies. The BIC solution outputs its measured parameter data to the channel port 212 to be displayed on the display 104 of hub 100. In an embodiment, the hub 100 may advantageously be entirely or partially formed as a BIC solution that communicates with other systems, such as, for example, tablets, smartphones, or other computing systems.

**[0055]** Although disclosed with reference to a single docking station 106, the environment 200 may include stacked docking stations where a subsequent docking station mechanically and electrically docks to a first docking station to change the form factor for a different portable patient monitor as discussed with reference to FIG. 5. Such stacking may include more than 2 docking stations, may reduce or increase the form factor for mechanical compliance with mating mechanical structures on a portable device.

**[0056]** FIG. 3 illustrates a simplified exemplary hardware block diagram of the hub 100 of FIG. 1, according to an embodiment of the disclosure. As shown in FIG. 3, the housing 108 of the hub 100 positions and/or encompasses an instrument board 302, the display 104, memory 304, and the various communication connections, including the serial ports 210, the channel ports 212, Ethernet ports 305, nurse call port 306, other communication ports 308 including standard USB or the like, and the docking station interface 310. The instrument board 302 comprises one or more substrates including communication interconnects, wiring, ports and the like to enable the communications and functions described herein, including inter-board communications. A core board 312 includes the main parameter, signal, and other processor(s) and memory, a portable monitor board (“RIB”) 314 includes patient electrical isolation for the monitor 102 and one or more processors, a channel board (“MID”) 316 controls the communication with the channel ports 212 including optional patient electrical isolation and power supply 318, and a radio board 320 includes components configured for wireless communications. Additionally, the instrument board 302 may advantageously include one or more processors and controllers, busses, all manner of communication connectivity and electronics, memory, memory readers including EPROM readers, and other electronics recognizable to an artisan from the disclosure herein. Each board comprises substrates for positioning and sup-

port, interconnect for communications, electronic components including controllers, logic devices, hardware/software combinations and the like to accomplish the tasks designated above and others.

**[0057]** An artisan will recognize from the disclosure herein that the instrument board 302 may comprise a large number of electronic components organized in a large number of ways. Using different boards such as those disclosed above advantageously provides organization and compartmentalization to the complex system.

#### Embodiments of Touch Screen Controls Including Certain Gestures

**[0058]** FIG. 4 illustrates a legend of finger control gestures 400 for use with a touchscreen display 104 according to an embodiment. The finger control gestures 400 include a touch 402, a touch and hold 404, a touch and move 406, a flick 408, a drag and drop 410, and a pinch 412. A touch 402 is a finger control gesture that executes the desired action once the user's finger is released from the screen. A touch and hold 404 is a finger control gesture that executes the desired action once the user has held his or her finger on the screen continuously for a predetermined duration (e.g., a few seconds), received a “hold completion” notification, and has released his or her finger from the screen. A touch and move 406 is a finger control gesture that manipulates and/or translates objects across the display 104 in the desired and permitted direction to a deliberate stopping point. To execute a touch and move finger control gesture 406, the user touches an object, moves the object (left, right, up, down, diagonally, etc.), and releases the object. A flick 408 is a finger control gesture comprising contact of an object on the display 104 in conjunction with a quick finger movement in a particular direction, typically along a single vector. To execute a flick 408 finger control gesture the user touches an object on the display 104, moves the object (typically, but not necessarily in a single direction) and releases the finger from the display 104 quickly, in a manner such that the contact point has a velocity throughout its path of motion. A drag and drop 410 is a finger control gesture by which the user moves an object to another location or to another object (e.g., a folder) and positions it there by releasing it. To execute a drag and drop 410 finger control gesture, the user touches, holds, drags and drops the object. A pinch 412 is a finger control gesture that expands or contracts the field of view on the display 104. To execute a pinch 412 finger control gesture, the user touches the display 104 at two touch points using two fingers, for example, the thumb and index finger of a user's hand. Moving the touch points apart from each other zooms in on the field of view, enlarging it, while moving the touch points together zooms out on the field of view, contracting it.

**[0059]** In an embodiment the user interface includes multiple controls. For example, a toggle control enables a user to slide a knob to switch between toggle states. The toggle control also enables the user to press left or right of the toggle to quickly move the toggle left or right. If the toggle control is labeled, the user can press the label to quickly move the knob left or right.

**[0060]** The following paragraphs include a description of additional touch screen controls that can be used with the system of the present disclosure. The system can include any combination of the following controls and the present dis-

closure is not intended to be limited by the following descriptions of various controls.

[0061] In some embodiments, a spinner control enables the user to press a center (focused) tile to expand a spinner when the spinner is closed and to collapse a spinner when the spinner is opened. The spinner control enables the user to swipe up or down which, when the spinner is open, scrolls through spinner tiles. The spinner control enables the user to press an unfocused tile which then scrolls the tile into a center, focused position. And the spinner control enables the user to collapse an open spinner by pressing anywhere outside the spinner.

[0062] A slider control enables the user to move a knob by sliding the knob. The slider control also enables the user to quickly move the knob to a specific position by pressing anywhere along the slider path.

[0063] A slider spinner control combines the control capabilities of the spinner control and the slider control.

[0064] A button control enables a user to perform an action, as defined by the button description, by pressing the button.

[0065] An icon menu control enables the user to open a specified menu by pressing a tile. The icon menu control enables the user to scroll icons left or right by swiping left or right anywhere on the display. The icon menu control enables the user to quickly center a tile corresponding to an indicator icon by pressing an indicator button.

[0066] A window control enables the user to open a parameter or measurement window when no parameter or measurement alarm is present, by pressing the parameter or measurement. The window control enables the user to silence a parameter or measurement alarm when a parameter or measurement alarm is present, by pressing the parameter or measurement. The window control enables a parameter or measurement to be moved to a different location on the display 104 by using a drag and drop 410 finger control gesture.

[0067] A well control enables the user to open a parameter or measurement menu when no parameter or measurement alarm is present, by pressing the parameter or measurement. The well control enables the user to silence a parameter or measurement alarm when a parameter or measurement alarm is present, by pressing the parameter or measurement.

[0068] A live waveform control enables the user to separate waveforms by swiping down. The live waveform control enables the user to combine waveforms by swiping up.

[0069] A trend line control enables the user to zoom in by pinching in, zoom out by pinching out, change a time range by panning, and open a parameter or measurement trend menu by pressing the y-axis.

[0070] An alarm silence icon control enables the user to silence all alarms by pressing the alarm silence icon.

[0071] An audio pause icon control enables the user to pause audio for a predetermined period of time, by pressing the audio pause icon.

[0072] Other status bar icon controls enable the user to open the relevant menu, by pressing the relevant status bar icon.

[0073] A back arrow control enables the user to exit a menu or abandon any changes made, by pressing a back arrow icon.

[0074] A confirm-or-cancel control enables the user to confirm changes to settings by pressing an OK button. The

confirm-or-cancel control enables the user to cancel changes to settings by pressing a cancel button.

[0075] A home control enables the user to navigate to the main screen at any time by pressing a home button.

#### Embodiments of Configurable Replay Display

[0076] FIG. 5 illustrates an embodiment of a user interface 500 displayed on the display 104 of the hub 100. In an embodiment the display 104 comprises a color, modular, touchscreen integral to the hub 100. Positioned horizontally along the top of the display 104 is a top status line 501 that displays system status as well as that provides shortcuts to menu items or actions. In an embodiment the icons presented on the top status line 501 include alarm silence 501A, audio pause 501B, profiles 501C, Bluetooth 501D, Wi-Fi 501E, Ethernet 501F, connectivity gateway 501G, portable patient monitor battery status 501H, monitoring hub battery status 501I, sounds 501J, and current time 501K.

[0077] The alarm silence icon 501A displays alarm status and mutes all audible alarms for monitoring devices connected to the hub 100. The audio pause icon 501B displays audio pause status and temporarily silences an alarm event. The profiles icon 501C provides access to a profiles screen; the example shown illustrates that the profile is set to "Adult" for an adult patient. The Bluetooth icon 501D provides access to a Bluetooth screen. If this icon is visible on the status line 501, then Bluetooth connectivity has been enabled. The Wi-Fi icon 501E provides access to a Wi-Fi screen. If this icon is visible on the status line 501, then Wi-Fi connectivity has been enabled. The icon itself also indicates the strength of the wireless signal. The Ethernet icon 501F provides access to an Ethernet screen. If this icon is visible on the status line 501, then Ethernet connectivity has been enabled.

[0078] The connectivity gateway icon 501G provides access to a connectivity gateway screen. The example illustrated indicates that standalone devices are connected to three of the available four ports. The color of the icon matches the status colors of the connected standalone devices. The portable patient monitor battery status icon 501H displays the charging status of the portable patient monitor 102 and provides access to a portable patient monitor battery screen. The example illustrates that the battery is currently charging. The monitoring hub battery status icon 501I displays the charging status of the monitoring hub 100 and provides access to a monitoring hub battery screen. The example illustrates that the battery is currently charging. The sounds icon 501J provides access to a sounds screen to adjust alarm and pulse tone volume. In an embodiment the sounds icon 501J does not indicate the actual volume level of the alarm and the pulse tone. The current time icon 501K displays the current time and provides access to a localization screen which contains settings related to local time, language and geography.

[0079] Positioned horizontally along the bottom of the display 104 is a bottom status line 502 that displays additional icons and information including a main menu icon, a gender icon, and a patient identifier that includes patient-specific information, such as, for example, the patient's name and room location. Although the disclosed embodiment employs status lines 501, 502 oriented horizontally along the top and bottom of the display 104, one skilled in the art would readily appreciate that information of the type presented in the top status line 501 and in the bottom status

line 502 may be presented in numerous different formats, combinations and configurations, including without limitation, one or more status bars positioned vertically on the display 104. Moreover a skilled artisan will appreciate that other useful information may be displayed in status bars 501, 502.

[0080] In an embodiment the user interface can create a window for every monitoring device connected to the hub 100. Parameters or measurements can be expanded within a window to customize views. A central portion 504 of the display 104 presents patient measurement data, in this example, in two windows 506, 530. Illustratively, by way of non-limiting example, an upper window 506 presents patient data measured by an a noninvasive monitoring platform, such as the Rainbow® Pulse CO-Oximetry™ monitoring platform by Masimo Corporation of Irvine, Calif., which enables the assessment of multiple blood constituents and physiologic parameters including oxygen saturation (SpO<sub>2</sub>) 508, pulse rate (PR) 510, respiration rate (RRp) 512, fractional arterial oxygen saturation (SpfO<sub>2</sub>) 514, total hemoglobin (SpHb) 516, plethysmograph variability index (PVI) 518, methemoglobin (SpMet) 520, carboxyhemoglobin (SpCO) 522, perfusion index (PI) 524, oxygen content (SpOC) 526, or others. In the illustrated example, the lower window 530 of the display 104 presents patient data measured by a regional oximetry platform, such as the O<sub>3</sub>™ regional oximetry module by Masimo Corporation of Irvine, Calif., which allows the continuous assessment of tissue oxygenation beneath one or more sensors placed on the patient's skin to help clinicians detect regional hypoxemia.

[0081] Advantageously, the display 104 is configurable to permit the user to adjust the manner by which the physiologic parameters are presented on the display 104. In particular, physiologic measurements of greater interest or importance to the clinician may be displayed in larger format and may also be displayed in both numerical and graphical formats to convey the current measurement as well as the historical trend of measurements for a period of time, such as, for example, the preceding hour. In an embodiment the oxygen saturation 508, pulse rate 510, and respiration rate 512 measurements are displayed in such a manner, taking up a larger portion of the upper portion 506 of the display 104, while the fractional arterial oxygen saturation 514, total hemoglobin 516, plethysmograph variability index 518, methemoglobin 520, carboxyhemoglobin 522, perfusion index 524, and oxygen content 526 measurements are displayed as numbers, taking up a smaller portion of the upper portion 506 of the display 104.

[0082] In an embodiment the presentation of measurement information may be adjusted easily by using the finger control gestures 400. For example, the touch and move 406 finger control gesture may be used to move an object on the display 104 representing a measurement from one location of the display 104 to another location of the display 104. Advantageously, when the object is moved, the display 104 automatically scales its presentation of information based upon the parameters that are active. For example, fewer parameters result in the presentation of larger digits, trend lines, and waveform cycles. In an embodiment the location to which an object is moved determines, at least in part, the manner by which that object will be presented on the display 104.

[0083] Attention is now directed to a plurality of analysis presentation views that may be presented on the disclosed

monitoring hub 100. Advantageously, the disclosed monitoring hub 100 provides many analytical formats by which measured physiological parameters, as well as other data, can be displayed to the user. Size, format, color, and location on the display, among other things, can be easily set and modified by the clinician-user to readily customize the manner by which monitored physiological parameter data, as well as information derived therefrom, can be displayed.

[0084] FIG. 6A is an illustration of an exemplary display screen 600 showing various formats of analytical presentation views for illustrating received physiological parameter data, according to an embodiment of the disclosure. The exemplary display screen 600 includes heat map analytical presentation views 602, box-and-whisker analytical presentation views 604, an index analytical presentation view 606, distribution analytical presentation views 608, histogram analytical presentation views 610, and gauge-histogram analytical presentation views 612. The positions of each analytical presentation view may be adjusted and the format of each analytical presentation view may be substituted with other formats, advantageously resulting in a high degree of customization for the user. For example, the gauge-histogram presentation views 612 are situated vertically in a right side panel portion of the screen 600, but may instead be situated in any formation and in any position on the screen 600.

[0085] Heat Maps

[0086] A heat map 602 analytical presentation view provides a two-dimensional graphical representation of a relationship between two measured parameters over a specified period of time, using color to identify areas in the graph where the data is concentrated. For example, as illustrated in FIG. 6B, the heat map 602 presents the relationship between measured oxygen saturation (SpO<sub>2</sub>) and pulse rate (PR) at specific points in time. Illustratively, by way of non-limiting example, an area on the graph corresponding to the highest concentration of correlated values between measured oxygen saturation and pulse rate is colored in a first color (e.g., red). FIG. 6B shows the heat map centered around an SpO<sub>2</sub> value of about 98% and a PR value of about 61 bpm. Moreover, FIG. 6B shows that as the concentration of correlated measurements decreases, the colors on the heat map change (e.g., from red to orange, then to yellow, then to green, and finally to blue) indicating progressively lower concentrations of correlated values between the two measured parameters.

[0087] Heat maps 602 advantageously provide a trend of multiple monitored values or physiological parameters at a mere glimpse. For example, FIG. 6B shows a caregiver that while the PR for the patient may be a little low, depending on age, fitness, activity level during monitoring, or the like, the patient was almost if not entirely fully saturated with oxygen. Thus, because the body appears to be oxygenated, additional PR may not be needed during the time period presented. Accordingly and advantageously, the heat map 602 delivers a visual summary of the data that enables the user to intuitively understand and analyze complex relationships between data sets.

[0088] Box-and-Whisker Plots

[0089] In descriptive statistics, a box plot or boxplot is a convenient way of graphically depicting groups of numerical data through their quartiles. Box plots may also have lines extending vertically from the boxes (whiskers) indicating variability outside the upper and lower quartiles,

these are often called box-and-whisker plots or diagrams. The spacings between the different parts of the box indicate the degree of dispersion (spread) and skewness in the data, and show outliers.

[0090] As shown in FIG. 6C, a box-and-whisker plot analytical presentation view **604** visually presents the range of measurements received over a specified or pre-determined period of time, and the boundaries of the quartiles in which the data lies. Advantageously, the box-and-whisker view **604** readily presents to the user the degree of spread, or dispersion, of the measured data, as well as the skewness in the data, including outlier measurements. The whiskers **620** and **622** identify the low end and high end, respectively, of the range of measurements displayed.

[0091] By way of illustrative example, as depicted in FIG. 6C, the range of measured SpO<sub>2</sub> data for a given patient may extend from 82% to 100%. An artisan will recognize other patient's may have many other ranges. The box **624** identifies the median line **626** of the measured SpO<sub>2</sub> parameter data. Thus, half of the measured SpO<sub>2</sub> data represented by the view **604** falls above the median line **626** and half of the measured SpO<sub>2</sub> data falls below the median. The lower edge **628** and the upper edge **630** of the box **624** identify the medians of the lower and upper half of the measured SpO<sub>2</sub> data, respectively. Thus, as illustrated in FIG. 6C, a first quartile of measured SpO<sub>2</sub> data lies between the end point of the bottom whisker **620** and the bottom edge **628** of the box **624**; a second quartile of measured SpO<sub>2</sub> data lies between the bottom edge **628** of the box **624** and the median line **626**; a third quartile of measured SpO<sub>2</sub> data lies between the median line **626** and the top edge **630** of the box **624**; and a fourth quartile of measured SpO<sub>2</sub> data lies between the top edge **630** of the box **624** and the end point of the top whisker **622**.

[0092] Again, box-and-whisper plots **604** advantageously provide a trend of a monitored value or physiological parameter at a mere glimpse. For example, FIG. 6C shows a caregiver that while SpO<sub>2</sub> varied somewhat, at least half the time it was above about 94% and a quarter of the monitored window SpO<sub>2</sub> was between about 94% and about 98%. While about half of the time, SpO<sub>2</sub> was lower than perhaps desired.

[0093] Index Views

[0094] An index analytical presentation view **606**, such as the continuous, noninvasive measurement of arterial hemoglobin concentration, which may also be referred to as a "total hemoglobin" (SpHb) index **606**, exemplarily illustrated in FIG. 6D, presents a current measured state of a physiological parameter (SpHb, in this example) relative to ranges identified as acceptable, cautionary, and emergent. As illustrated in FIG. 6D, an indicator **632** shows a current measured parameter level relative to a vertical bar **634**. The vertical bar **634** is shaded in different colors, such as, for example, green, yellow and red. The colors can be used to identify different regions or zones corresponding to, for example, acceptable, cautionary, and emergent values of the measured parameter. A threshold line **636** can be set to visually identify one zone from another. Illustratively, by way of non-limiting example, the threshold line **636** can identify the boundary between the range of acceptable values and the range of cautionary values of the measured parameter. In an embodiment, the user can set the ranges and boundary conditions for such ranges. In other embodiments, the ranges and boundary conditions for a given physiologi-

cal parameter are set to default values corresponding to generally clinically accepted values for such ranges. The units of the measured parameter can be presented in a well **638** at the bottom of the index analytical presentation view **606**. For example, as illustrated in FIG. 6D, the units of the physiological parameter being measured (total hemoglobin, SpHb) are in grams per deciliter (g/dL) at a confidence interval (C.I.) of ninety percent. Advantageously, the index analytical display provides to the user an easily-interpreted presentation of the measured physiological parameter.

[0095] Distribution Views

[0096] A distribution analytical presentation view **608**, such as the SpO<sub>2</sub> distribution display **608** illustrated in FIG. 6E, presents a statistical distribution of a set of physiological parameter measurements over a specified or pre-defined period of time. The distribution analytical presentation view **608** provides the user a visual representation of the range of physiological parameter measurements collected as well as a statistical distribution associated with such measurements. Illustratively, by way of non-limiting example, the distribution analytical presentation view **608** shown in FIG. 6E presents a distribution **640** of the oxygen saturation (SpO<sub>2</sub>) parameter measurements over a period of time. In the example depicted in FIG. 6E, the distribution **640** is substantially normal (or Gaussian) with its mean (or expected value) **642** illustrated as well. A current measured value indicator **644** informs the user of the present state of the patient, and a standard deviation indicator **646** indicates the degree to which the measured data varies or disperses over the range of values. A well **648** toward the bottom of the distribution analytical display **608** provides numerical units of the measured physiological parameter, such as percentage for the oxygen saturation measurement.

[0097] Histogram Views

[0098] A histogram analytical presentation view **610**, as illustrated in FIG. 6F, provides another graphical representation of a collection of measured physiological parameter data. A histogram represents an estimate of the statistical (or probability) distribution of a continuous variable, such as a continuously measured physiological parameter. Thus, rather than providing a statistical distribution (i.e., a probabilistic model) that best fits or corresponds to the measured data, the histogram reflects the actual measured data collected. To form a histogram, the entire range of values to be measured is divided into a series of often equally-spaced, often consecutive, often non-overlapping intervals, referred to as "bins." Each physiological parameter measurement value is then allocated to one of the bins. A bar is drawn for each bin, where the height of the bar corresponds to the number of discrete physiological parameter measurements that fall within that bin's particular range. In an embodiment, the width of each bar is constant, corresponding to the ranges of the equally-spaced intervals. The histogram may also be normalized to display the relative frequency or proportion of measurements that fall into each of the several bins. Advantageously, the histogram analytical presentation view **610** provides the user a visual representation of the actual frequencies of the observed physiological parameter measurements in certain ranges of values.

[0099] Analog Gages Including Histogram Views

[0100] A gauge-histogram analytical presentation view **612**, as illustrated in FIG. 6G, provides a combination of analog, digital and histogram display indicia in one presentational format view. Advantageously, the gauge-histogram

analytical presentation view **612** provides to the user a substantial amount of information related to the measured physiological parameter in an intuitive and visually accessible format. The gauge-histogram **612** includes an analog indicator forming, for example, a semi-circular arc **650**. Portions of the arc **650** can be differentiated by use of various colors or shading to indicate different regions of measured parameter values, such as, for example, acceptable, cautionary and emergent regions of the gauge. Illustratively, by way of non-limiting example, the acceptable range of values can be colored green, and can be located generally centrally within the arc **650**, while cautionary ranges of values can be colored yellow and located beyond the acceptable range of values, and emergent ranges of values can be colored red and located beyond the cautionary value ranges toward the two ends of the arc **650**. Of course, one skilled in the art will appreciate that many other colors and range formats may be used without departing from the scope of the present disclosure.

[0101] The gauge-histogram analytical presentation view **612** can include a dial marker **652** that moves about the arc **650** reflecting the current measured level of the monitored physiological parameter. Illustratively, by way of non-limiting example, as the measured physiological parameter level increases, the dial can move clockwise, and as the measured physiological parameter level decreases, the dial can move counter-clockwise, or vice versa. In this way, a user can quickly determine the patient's status by looking at the analog indicator. For example, if the dial marker **652** is in the center of the arc **650**, the observer can be assured that the current physiological parameter measurement falls within the acceptable range. If the dial marker **652** is skewed too far to the left or right, the observer can quickly assess the severity of the physiological parameter level and take appropriate action. In other embodiments, acceptable parameter measurements can be indicated when the dial marker **652** is to the right or left, etc.

[0102] In some embodiments, the dial marker **652** can be implemented as a dot, a dash, an arrow, or the like, and the arc **650** can be implemented as a circle, a spiral, a pyramid, or any other shape, as desired. Furthermore, the entire arc **650** can be illuminated or only portions of the arc **650** can be illuminated, based for example, on the current physiological parameter being measured. Additionally, the arc **650** can turn colors or be highlighted based on the current measured physiological parameter level. For example, as the dial marker **652** approaches a threshold level, the arc **650** and/or the dial marker **652** can turn from green, to yellow, to red, shine brighter, flash, be enlarged, move to the center of the display, sound an alarm, or the like.

[0103] Different physiological parameters can have different thresholds indicating abnormal conditions. For example, some physiological parameters may have upper and lower threshold levels, while other physiological parameters may only have an upper threshold or a lower threshold level. Accordingly, each gauge-histogram analytical presentation view **612** can be adjusted based on the particular physiological parameter being monitored. Illustratively, by way of non-limiting example, an SpO<sub>2</sub> gauge-histogram presentation view **612** can have a lower threshold, which when met, activates an alarm, while a respiration rate gauge-histogram presentation view **612** can have both a lower and an upper threshold, and when either threshold is met, an alarm can be activated. The thresholds for each physiological parameter

can be based on typical, expected thresholds, or they can be set to user-specified threshold levels.

[0104] In certain embodiments, such as the embodiment illustrated in FIG. 6G, the gauge-histogram analytical presentation view **612** includes a digital indicator **654**. The analog arc **650** and digital indicator **654** can be positioned in any number of formations relative to each other, such as side-by-side, above, below, transposed, etc. In the illustrated embodiment, the analog arc **650** is positioned above the digital indicator **654**. As described above, the analog arc **650** and dial marker **652** may include colored warning sections, indicating a current position on the graph. The digital information designates quantitative information from the graph. In FIG. 6G, for example, the gauge-histogram analytical presentation view **612** displays pulse rate information. The arc **650** shows that from about 50 to about 140 beats per minute, the measured pulse rate physiological parameter is either in the acceptable range or beginning to enter the cautionary range, whereas in the regions outside those numbers, the arc **650** is colored to indicate an emergent or severe condition. Thus, as the dial marker **652** moves along the arc, **650**, a caregiver can readily see where in the ranges of acceptable, cautionary, and emergent pulse rate values the current measurement falls. The digital indicator **654** provides a numerical representation of the current measured value of the physiological parameter being displayed. The digital indicator **654** may indicate an actual measured value or a normalized value, and it can also be used to quickly assess the severity of a patient's condition.

[0105] As illustrated in FIG. 6G, a histogram arc **656** is located above and surrounding the arc **650**, having multiple radially-extending lines that correspond to histogram bins (as described above with respect to FIG. 6F) for the measured physiological parameter. The bins of the histogram arc **656** can be illuminated to reflect the distribution of measured parameter values in the manner described above with respect to the histogram analytical presentation view **610**. In the embodiment illustrated in FIG. 6G, the bins are illuminated in colors corresponding to the ranges along the arc **650** in which they fall. Thus, the disclosed gauge-histogram analytical presentation view **612** provides analog and digital indicia of the current measured physiological parameter, correlated with range information indicative of the level of urgency required for the measured parameter, as well as a visual display of the actual distribution of the patient's parameter measurements over a period of time.

[0106] Advantageously, the hub **100** stores the measured data that it has presented on the display screen **600** over time. In certain embodiments, the data is stored in the memory **304** of the instrument board **302**. In certain embodiments, the stored externally and accessed by the monitoring hub **100** via a network connection, such as, for example, an Ethernet connection. In still other embodiments, the data is stored in both on-board memory **304** and external storage devices.

[0107] Drag and Drop

[0108] Referring back to FIG. 6A, each of the foregoing display elements **6B**, **6C**, **6D**, **6E**, **6F** and **6G** can be dragged onto the screen and dropped to create a customized view to match a caregiver's preferences for a particular monitored patient. In an embodiment, a display element and its particular displayed parameters are shown as icons along a bottom horizontally scrollable menu. When a caregiver wishes to place, for example, a Perfusion Variability Index

(PVI) distribution view on the screen, he or she could select the PVI distribution icon from the bottom well, scroll, and drag it to the screen to, for example, replace any existing display element. In another embodiment, a caregiver may select a display element and then select the parameter or parameters to be provided to the element.

[0109] **Replay**

[0110] FIG. 6A also shows the display screen 600 provides a replay feature, which permits the clinician to review a historical record of the patient data collected and processed by the monitor 100. A user may select a time frame 662 for a replay period. For example, a user may select between replaying a previous ten-minute period, a four-hour period, or an eight-hour period. Any amount of time may be a suitable replay period. In an embodiment, the screen 600 may provide a default time frame 662, for example eight hours. After a replay period is selected or a default period is determined, a user may select a replay icon 660 to begin replay.

[0111] In certain embodiments, the stored data may be replayed on different monitor hubs or on different displays (such as, for example, a display connected to a multi-patient monitoring server 204), to permit clinicians who are remote from the patient's care environment to access and review the monitored data.

[0112] During a replay period, stored data may be displayed on the screen 600 at different rates. For example, the replayed data can be displayed at the same rate of time in which the data was originally presented. Thus, replaying one hour of recorded data would take one hour to fully replay. Alternatively, the replayed data can be displayed in slow-motion (slower than real-time), or in a time-lapse (faster than real-time) formats. For example, to replay in slow-motion, the screen 600 may present each frame of data for a longer period of time than originally presented. Illustratively, by way of non-limiting example, slow-motion replay can be useful to review and analyze portions of the recorded physiological parameter data in which abrupt changes occur. Time-lapse replay permits the clinician to review a period of recorded data over a shorter period of time than the data was originally presented. In an embodiment, to replay in time-lapse mode, a screen 600 may accelerate a speed at which frames are displayed. In another embodiment, to replay in time-lapse mode, a screen 600 may display only a sampling of frames from a set of data. For example, a screen 600 may display every fifteenth frame so that data may be presented in a shorter time while still providing a useful illustration of the stored data. In an embodiment, the user can select the rate at which the time-lapse replay will progress. For example, by way of illustration, the user might choose to view one minute's worth of real-time data in one second or in ten seconds. This information may be particularly useful to a care provider who would like to quickly review a patient's physiological conditions from a previous time period when, for example, the care provider was not present to observe the data as it was originally presented.

[0113] In certain embodiments, multiple parameter displays presented on the screen 600 may synchronously replay stored data during a replay period, while other parameter displays may present live data. This allows the clinician to concurrently monitor the present condition of the patient and review (i.e., replay) past measurement data. Illustratively, by way of non-limiting example, a series of analytical displays in a center portion of the screen 600 may replay stored data,

while a series of gauge-histogram analytical displays 612, located in a side panel, may present live data. In another embodiment, every feature on the screen 600 may replay stored data during a replay period. FIG. 7 illustrates such an example, and the display 700 provides a message 702 indicating that the displayed data is being replayed. In yet another embodiment, any single analytical display or combination of analytical displays on the screen 600 may present live data during a replay period. In some embodiments, individual analytical displays may have individual icons or indicators (not shown) associated with them to indicate whether the analytical presentation view is presenting live or stored and replayed data. In some embodiments, an individual display element may include both replayed and live data.

[0114] FIG. 8 is a flowchart illustrating a replay process 800 according to an embodiment of the present disclosure. At optional block 802, a user configures the display 600 with the display elements a caregiver desires for the monitored patient. The drag and drop functionality allows the user to straightforwardly drag the display elements to the portion of the screen desired. In an embodiment, a default screen layout could be implemented. Alternatively or additionally, the screen may be set to the most recent replay configuration, a replay configuration matched to a known user, known caregiver, or the patient, or some or all of the foregoing.

[0115] In optional block 804, the user sets a time period for replay. As discussed above, any amount of time may be a suitable time period. For example, a user may choose between a two-hour, four-hour, eight-hour, or ten-minute replay period. In an embodiment, a user may select a timeframe icon 662 to set the time period. In other embodiments, the user can scroll backward on a timeline (not shown) to select a starting point and ending point for the replay. In other embodiments, the user can input a start time and end time for the replay.

[0116] At optional block 806, the user may select a replay interval which defines the rate at which the replay displays. In certain embodiments, the replay interval includes real-time, slow-motion, and time-lapse intervals. Illustratively, a replay interval may be indicative of the number of frames of stored data which are displayed when selecting a time-lapse mode of replay. For example, a user may choose to have every fifteenth frame or every tenth frame of recorded data to be displayed in order to shorten the time required to replay stored data. In other embodiments, the user may be presented a timeline the width of the optionally selected time period and the user may pinch the timeline bigger or smaller to automatically adjust the interval.

[0117] At block 808, time is set to the start of the time period. At block 810, measurement data is accessed. In an embodiment, a processor accesses only the data used in the active display elements; in other embodiments, all the data associated with a particular time is accessed. In an embodiment, the processor synchronizes data to the display time even though such data may not be from the same measurement device. In other embodiments, synchronization data may be stored along with the original measurement data for use when accessed during the replay process 800.

[0118] At block 812, the data is displayed to the user through the configured display elements. At optional block 814, a user may interrupt replay to pause, speed up or slow down the replay, zoom in or out on a time period, switch to another time period, end replay, change display elements, or

otherwise manipulate the data being replayed. In optional block **816**, such interrupts are handled and appropriate action is taken, such as, for example, restarting replay with new configuration or time parameters.

**[0119]** At block **818**, the process **800** determines if playback has reached the end of the selected playback time period. If so, the process **800** ends; if not, the display rate is added to the current display time and the process **800** returns to block **810** to access additional data.

**[0120]** Advantageously, process **800** allows a caregiver to straightforwardly monitor a wide variety of measurements and combinations of measurements for a particular time period. For example, the caregiver may see during replay a heat map **602** fluctuate in color and/or position, pulse or otherwise show how the body of the patient is oxygenated and what pulse rate it is using for such oxygenation. Likewise, box-and-whisker plots **604** may have portions that grow, shrink, and move in rhythm with, for example, the heat map **602**. Distributions **608** may change and histograms along with their analog gages may provide indications of how the body is reacting over a course of pre-selected time.

**[0121]** As discussed above, a user may run a replay process by selecting a replay icon **660**. Once the replay process is complete, a user may choose whether to repeat the process, at block **808**. If the user chooses to repeat the process, the process **800** will again run at step **806**. If the user chooses not to repeat the process, the process will end at block **810**.

**[0122]** Thus, a patient monitoring hub that serves as the center of patient monitoring and treatment activities for a given patient is disclosed. Embodiments of the patient monitoring hub include a large visual display that dynamically provides information to a caregiver about a wide variety of physiological measurements or otherwise-determined parameters. Advantageously, the display can be customized by the clinician-user to present the desired physiological parameters (and other relevant information) in the formats and at the locations on the display that the clinician desires. Numerous analytical presentation views are provided to present the monitored physiological parameters (and other information) in visual formats that provide timely, clinically-relevant, and actionable information to the care provider. Additionally, the disclosed monitoring hub allows for replay of all or portions of the monitored data in a synchronized manner. The embodiments disclosed herein are presented by way of examples only and not to limit the scope of the claims that follow. One of ordinary skill in the art will appreciate from the disclosure herein that many variations and modifications can be realized without departing from the scope of the present disclosure.

**[0123]** The term “and/or” herein has its broadest least limiting meaning which is the disclosure includes A alone, B alone, both A and B together, or A or B alternatively, but does not require both A and B or require one of A or one of B. As used herein, the phrase “at least one of” A, B, “and” C should be construed to mean a logical A or B or C, using a non-exclusive logical or.

**[0124]** The term “plethysmograph” includes its ordinary broad meaning known in the art which includes data responsive to changes in volume within an organ or whole body (usually resulting from fluctuations in the amount of blood or air it contains).

**[0125]** The following description is merely illustrative in nature and is in no way intended to limit the disclosure, its

application, or uses. For purposes of clarity, the same reference numbers will be used in the drawings to identify similar elements. It should be understood that steps within a method may be executed in different order without altering the principles of the present disclosure.

**[0126]** As used herein, the term module may refer to, be part of, or include an Application Specific Integrated Circuit (ASIC); an electronic circuit; a combinational logic circuit; a field programmable gate array (FPGA); a processor (shared, dedicated, or group) that executes code; other suitable components that provide the described functionality; or a combination of some or all of the above, such as in a system-on-chip. The term module may include memory (shared, dedicated, or group) that stores code executed by the processor.

**[0127]** The term code, as used above, may include software, firmware, and/or microcode, and may refer to programs, routines, functions, classes, and/or objects. The term shared, as used above, means that some or all code from multiple modules may be executed using a single (shared) processor. In addition, some or all code from multiple modules may be stored by a single (shared) memory. The term group, as used above, means that some or all code from a single module may be executed using a group of processors. In addition, some or all code from a single module may be stored using a group of memories.

**[0128]** The apparatuses and methods described herein may be implemented by one or more computer programs executed by one or more processors. The computer programs include processor-executable instructions that are stored on a non-transitory tangible computer readable medium. The computer programs may also include stored data. Non-limiting examples of the non-transitory tangible computer readable medium are nonvolatile memory, magnetic storage, and optical storage. Although the foregoing invention has been described in terms of certain preferred embodiments, other embodiments will be apparent to those of ordinary skill in the art from the disclosure herein. Additionally, other combinations, omissions, substitutions and modifications will be apparent to the skilled artisan in view of the disclosure herein. Accordingly, the present invention is not intended to be limited by the reaction of the preferred embodiments, but is to be defined by reference to claims.

**[0129]** Additionally, all publications, patents, and patent applications mentioned in this specification are herein incorporated by reference to the same extent as if each individual publication, patent, or patent application was specifically and individually indicated to be incorporated by reference.

What is claimed is:

1. A medical monitor configured to analyze and present indicia reflective of physiological parameters of a patient, said parameters including oxygen saturation, the monitor comprising:

a first communication port configured to receive a first signal indicative of a first physiological parameter associated with the patient, said first signal responsive to light attenuated by body tissue;

a display;

a processor configured to process said received first signal and to cause a first view to be presented on at least a portion of said display, said first view adapted to present first data indicative of said first physiological parameter over a first period of time; and

- a storage device configured to store said presented first data;
- wherein said processor is further configured to replay said stored first data on said display.
2. The monitor of claim 1, wherein said processor is configured to cause said replayed first data to be presented for a duration that is shorter than said first period of time.
3. The monitor of claim 1, wherein said processor is configured to cause said replayed first data to be presented for a duration that is longer than said first period of time.
4. The monitor of claim 1, wherein said processor is configured to cause said replayed first data to be presented for a duration that is equal to said first period of time.
5. The monitor of claim 1, further comprising:  
a second communication port configured to receive a second signal indicative of a second physiological parameter associated with said patient;  
wherein said processor is further configured to process said received second signal, to cause a second view to be presented on at least a portion of said display, the view adapted to present second data indicative of said second physiological parameter over said first period of time;  
wherein said storage device is further configured to store said presented second data; and  
wherein said processor is further configured to synchronously replay said stored first and second data.
6. The monitor of claim 1, wherein said second data is indicative of a relationship between said first physiological parameter and said second physiological parameter.
7. The monitor of claim 6, wherein said second view is further configured to present a graph of said relationship between said physiological parameters and to identify an area in said graph in which said second data is concentrated.
8. The monitor of claim 7, wherein said second view uses a color to identify said area in which said second data is concentrated.
9. The monitor of claim 6, wherein said second view is further configured to identify a first area in said graph associated with a first concentration of said second data and a second area in said graph associated with a second concentration of said second data, wherein said first area is presented in a first color and said second area is presented in a second color.
10. The monitor of claim 6, wherein said first physiological parameter is oxygen saturation and said second physiological parameter is pulse rate.
11. The monitor of claim 6, wherein said first physiological parameter is total hemoglobin and said second physiological parameter is plethysmograph variability index.
12. The monitor of claim 6, wherein said second view comprises a heat map analytical presentation view.
13. The monitor of claim 1, wherein said first view comprises a box-and-whisker analytical presentation view.
14. The monitor of claim 1, wherein said first view comprises an index analytical presentation view.
15. The monitor of claim 1, wherein said first view comprises a distribution analytical presentation view.
16. The monitor of claim 1, wherein said first view comprises a histogram analytical presentation view.
17. The monitor of claim 1, wherein said first view comprises a gauge-histogram analytical presentation view.
18. The monitor of claim 1, wherein said first view comprises a gauge-histogram analytical presentation view further comprising a digital indicator.
19. The monitor of claim 1, wherein said first view comprises an analog gauge showing measurement data, said analog gauge comprising an arc and a dial marker.
20. The monitor of claim 1, wherein said communication port comprises a serial port.
21. The monitor of claim 1, wherein said hub communicates with one or more medical sensors.
22. A method of monitoring physiological parameters of a patient, the method comprising:  
receiving, at a first communication port from a first physiological sensor, a first signal indicative a first physiological parameter associated with said patient;  
processing, with a processor, said received first signal to generate first data indicative of said first physiological parameter over a first period of time;  
causing, with said processor, said first data to be presented on at least a portion of a display;  
storing, in a data storage device, said presented first data; and  
replaying, on said display, said stored first data.
23. The method of claim 22, further comprising:  
receiving, at a second communication port from a second physiological sensor, a second signal indicative of a second physiological parameter associated with said patient;  
processing, with said processor, said received second signal to generate second data indicative of said second physiological parameter over said first period of time;  
causing, with said processor, said second data to be presented on at least a portion of said display;  
storing, in said data storage device, said presented second data; and  
replaying synchronously, on said display, said stored first and second data.
24. The method of claim 22, comprising causing said replayed first data to be presented for a duration that is shorter than said first period of time.
25. The method of claim 22, comprising causing said replayed first data to be presented for a duration that is longer than said first period of time.
26. The method of claim 22, comprising causing said replayed first data to be presented for a duration that is equal to said first period of time.
27. The method of claim 23, wherein the causing said second data to be presented further comprises:  
processing, with said processor, said received first and second signals to generate second data indicative of a relationship between said first physiological parameter and said second physiological parameter;  
presenting a graph indicative of said second data; and  
identifying, on said graph, an area in which said second data is concentrated.
28. The method of claim 27, further comprising identifying a first area in said graph associated with a first concentration of said second data and a second area in said graph associated with a second concentration of said second data, wherein said first area is presented in a first color and said second area is presented in a second color.
29. The method of claim 22, wherein causing said first data to be presented further comprises:

presenting, on said display, a first whisker having an upper end and an opposite end, said upper end being indicative of an upper point of a data range of said first data;

presenting, on said display, a second whisker having a lower end and an opposite end, said lower end being indicative of a lower point of said data range; and

presenting, on said display, between said first and second whiskers, a box having an upper edge, a median line, and a lower edge, said upper edge connected to said opposite end of said first whisker and indicative of a first separation line between a first quartile and a second quartile of said data range, said lower edge connected to said opposite end of said second whisker and indicative of a second separation line between a third quartile and a fourth quartile of said data range, and said median line indicative of a third separation line between said second and third quartiles of said data range.

**30.** The method of claim **22**, wherein causing said first data to be presented comprises presenting, on said display, a measurement marker, a value bar, and a threshold line, wherein the value bar is divided into a plurality of regions, and wherein the threshold line is associated with a boundary between two adjacent regions.

**31.** The method of claim **22**, wherein causing said first data to be presented further comprises presenting, on said display, a distribution graph indicative of said first data.

**32.** The method of claim **22**, wherein causing said first data to be presented further comprises presenting, on said display, a histogram graph indicative of said first data.

**33.** The method of claim **22**, wherein causing said first data to be presented further comprises presenting, on said display, a gauge-histogram indicative of said first data.

\* \* \* \* \*

|                |  |         |            |
|----------------|--|---------|------------|
| 专利名称(译)        | 医学监测分析和重放，包括对身体组织减弱的光敏感的标记   |         |            |
| 公开(公告)号        | <a href="#">US20170042488A1</a>  | 公开(公告)日 | 2017-02-16 |
| 申请号            | US15/233244  | 申请日     | 2016-08-10 |
| [标]申请(专利权)人(译) | 梅西莫股份有限公司  |         |            |
| 申请(专利权)人(译)    | Masimo公司   |         |            |
| 当前申请(专利权)人(译)  | Masimo公司   |         |            |
| [标]发明人         | MUHSIN BILAL   |         |            |
| 发明人            | MUHSIN, BILAL  |         |            |
| IPC分类号         | A61B5/00 G06T11/20 A61B5/08 A61B5/1455 A61B5/024   |         |            |
| CPC分类号         | A61B5/7445 A61B5/14551 A61B5/02416 A61B5/0008 G06T11/206 A61B5/4839 A61B5/08 A61B5/746 A61B5/0022 A61B5/0205 A61B5/742 |         |            |
| 优先权            | 62/203792 2015-08-11 US  |         |            |
| 外部链接           | <a href="#">Espacenet</a> <a href="#">USPTO</a>  |         |            |

摘要(译)

本公开包括作为被监测患者的监测中心的医疗监测集线器。集线器被配置为接收和处理与患者相关联的多个生理参数。中心包括高级分析表示视图，配置为向护理提供者提供及时，临床相关，可操作的信息。在某些实施例中，监视中心存储并且能够回放反映患者状况的先前呈现的数据。

