



US009714969B2

(12) **United States Patent**  
**Kosturko**

(10) **Patent No.:** **US 9,714,969 B2**  
(45) **Date of Patent:** **Jul. 25, 2017**

(54) **SYSTEMS AND METHODS FOR SPECTROSCOPIC MEASUREMENT OF A CHARACTERISTIC OF BIOLOGICAL TISSUE**

USPC ..... 702/191; 356/28.5; 600/476, 323, 301, 600/309, 473  
See application file for complete search history.

(71) Applicant: **CAS Medical Systems, Inc.**, Branford, CT (US)

(56) **References Cited**

(72) Inventor: **William Kosturko**, Milford, CT (US)

U.S. PATENT DOCUMENTS

(73) Assignee: **CAS Medical Systems, Inc.**, Branford, CT (US)

4,476,875 A \* 10/1984 Nilsson ..... A61B 5/02416 356/28.5  
5,760,942 A 6/1998 Bryant  
5,801,826 A 9/1998 Williams  
7,139,603 B2 \* 11/2006 Chance ..... A61B 5/0073 600/473

(\* ) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 579 days.

(Continued)

FOREIGN PATENT DOCUMENTS

(21) Appl. No.: **14/041,733**

GB 760729 11/1956

(22) Filed: **Sep. 30, 2013**

OTHER PUBLICATIONS

(65) **Prior Publication Data**

US 2014/0100823 A1 Apr. 10, 2014

EP search report for EP13186637.8.

**Related U.S. Application Data**

*Primary Examiner* — Aditya Bhat

(60) Provisional application No. 61/707,138, filed on Sep. 28, 2012.

(74) *Attorney, Agent, or Firm* — O'Shea Getz P.C.

(51) **Int. Cl.**

**H03F 1/26** (2006.01)  
**G01R 29/26** (2006.01)  
**A61B 5/00** (2006.01)  
**A61B 5/1455** (2006.01)  
**G01N 21/00** (2006.01)

(57) **ABSTRACT**

A method and system for spectroscopic measurement of a characteristic of a biological tissue is provided. The method includes the steps of: (1) using at least one light source to emit light that penetrates the biological tissue; (2) using at least one light detector to detect light emitted by the at least one light source and passed through the biological tissue, and to convert the detected light into a detection signal, the detection signal including an unwanted noise component; and (3) using a processor to process the detection signal and to determine an adjusted peak-to-peak amplitude value that is representative of an amplitude of the detection signal adjusted for the unwanted noise component.


(52) **U.S. Cl.**

CPC ..... **G01R 29/26** (2013.01); **A61B 5/0075** (2013.01); **A61B 5/14553** (2013.01); **G01N 21/00** (2013.01); **A61B 5/7225** (2013.01); **A61B 2576/026** (2013.01)

(58) **Field of Classification Search**

CPC ..... G01N 21/00; G01R 29/26; A61B 5/0075; A61B 5/14553; A61B 5/7225; A61B 2576/026

**7 Claims, 11 Drawing Sheets**

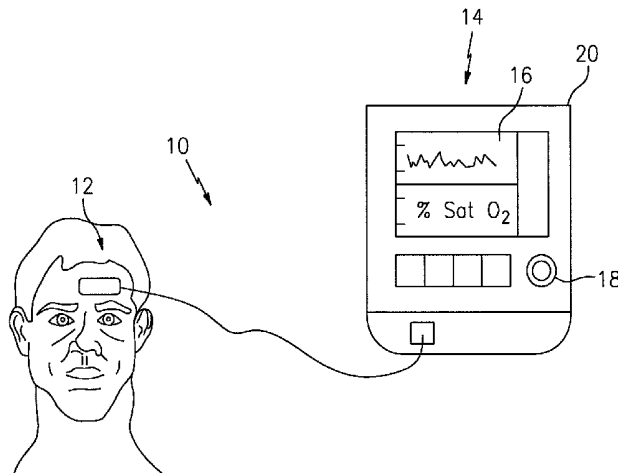

(56)

**References Cited**

U.S. PATENT DOCUMENTS

8,188,433	B2	5/2012	Gonopolskiy et al.	
2006/0058683	A1*	3/2006	Chance .....	A61B 5/0059 600/476
2007/0135694	A1	6/2007	Sato	
2008/0015424	A1*	1/2008	Bernreuter .....	A61B 5/14551 600/323
2008/0255433	A1*	10/2008	Prough .....	A61B 5/0095 600/301
2008/0319285	A1*	12/2008	Hancock .....	A61B 5/0507 600/309
2015/0282716	A1*	10/2015	Smeltzer .....	G01N 33/569 600/431

\* cited by examiner

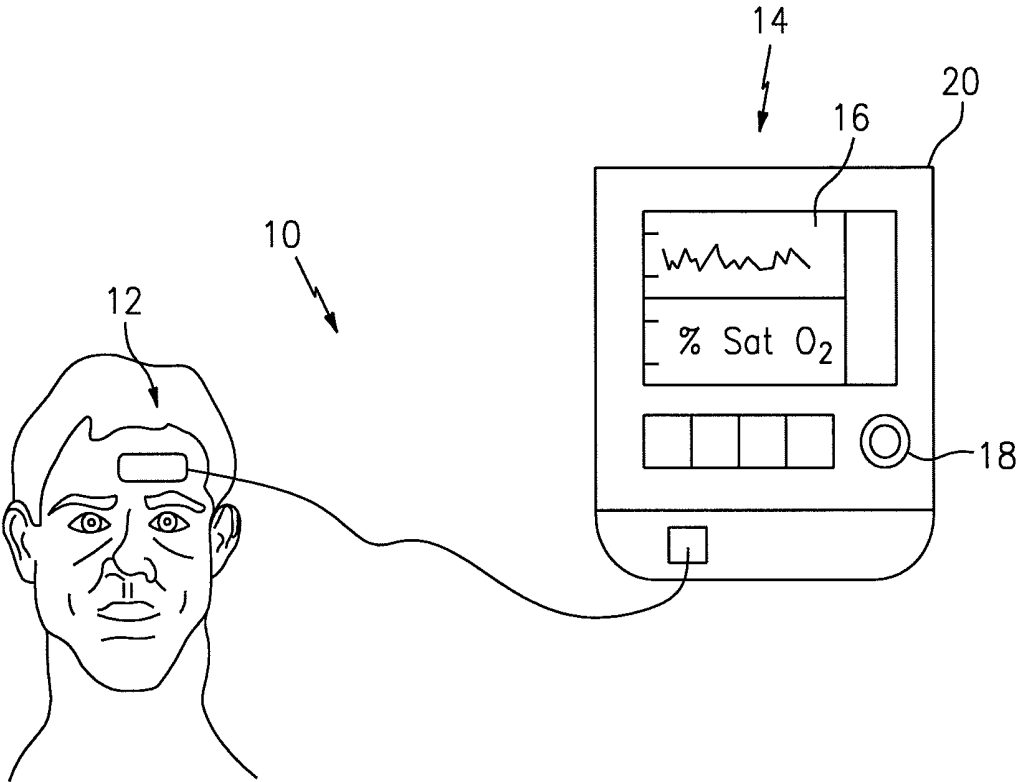


FIG. 1

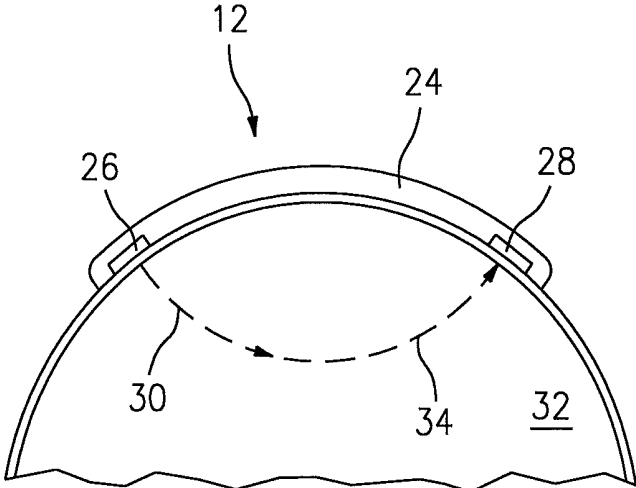


FIG. 2

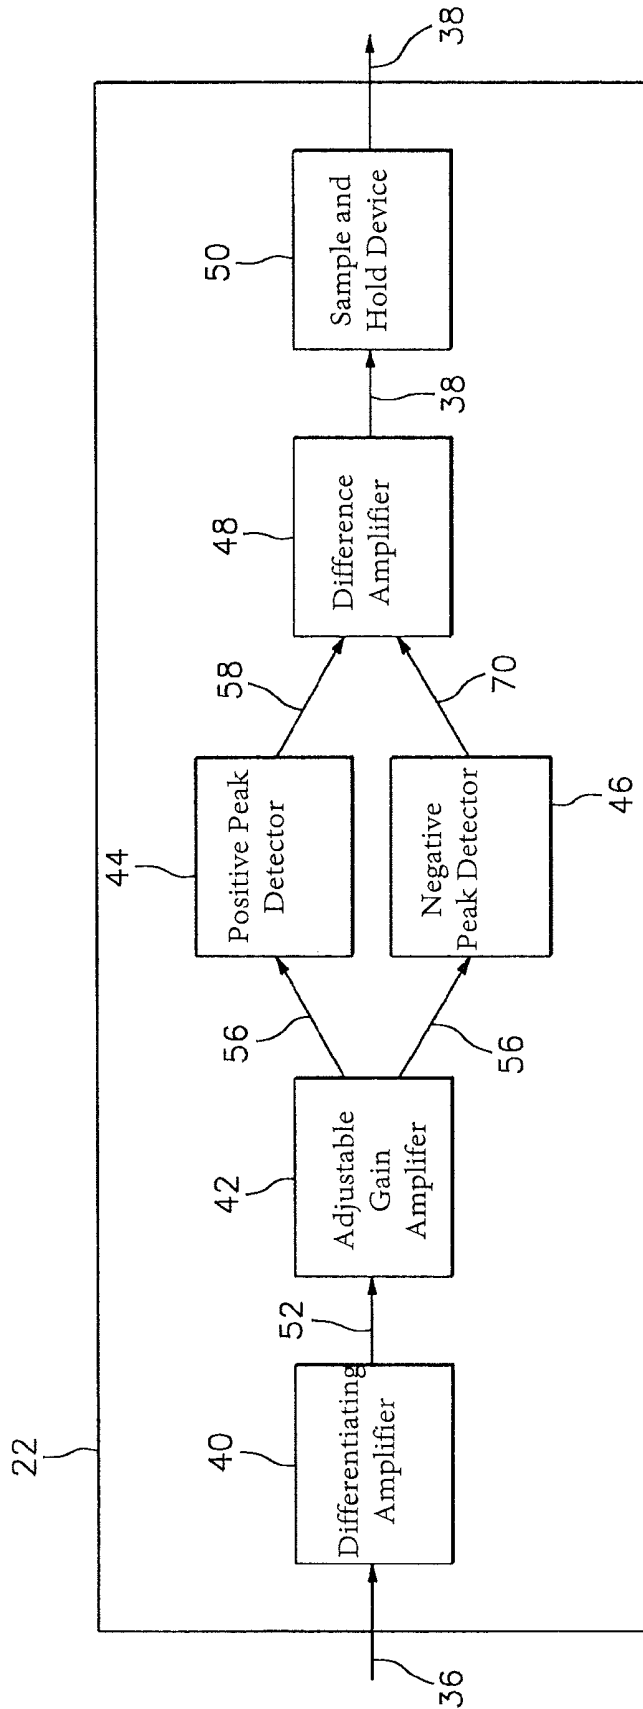


FIG. 3

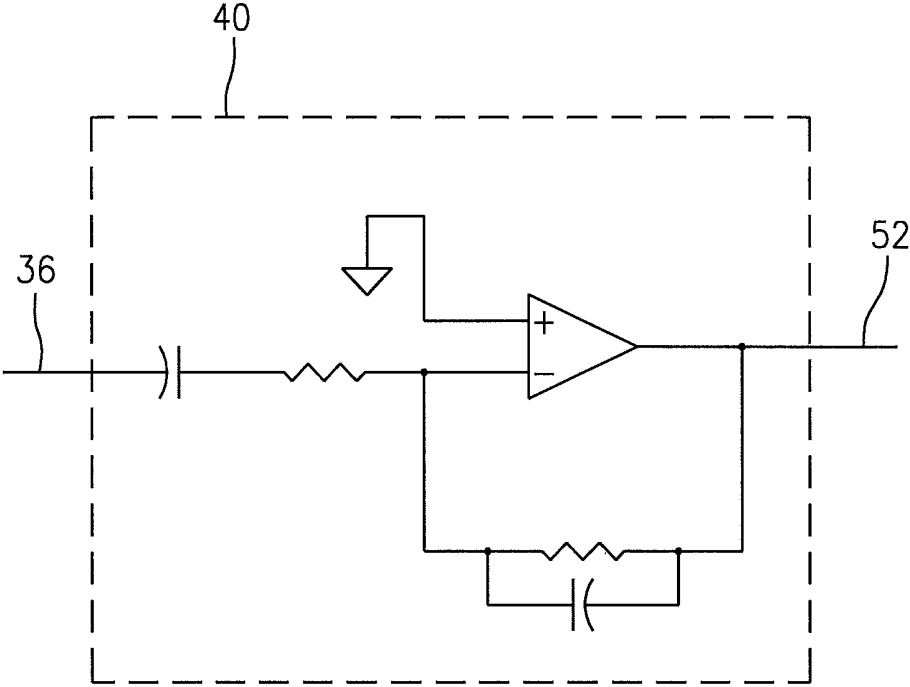


FIG. 4

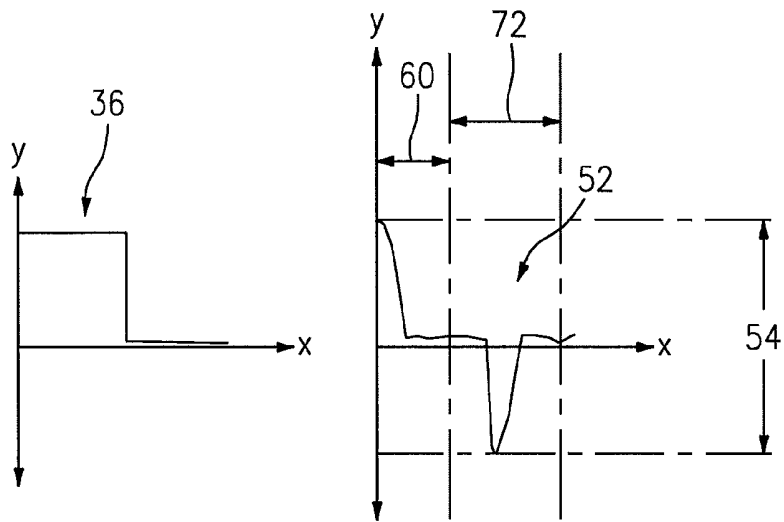


FIG. 5

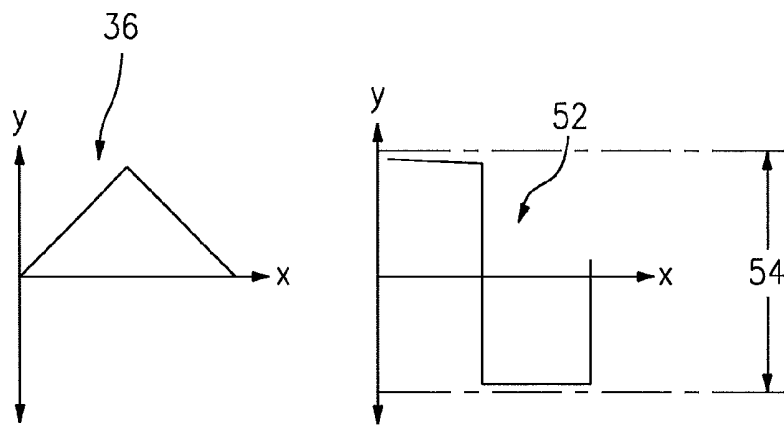


FIG. 6

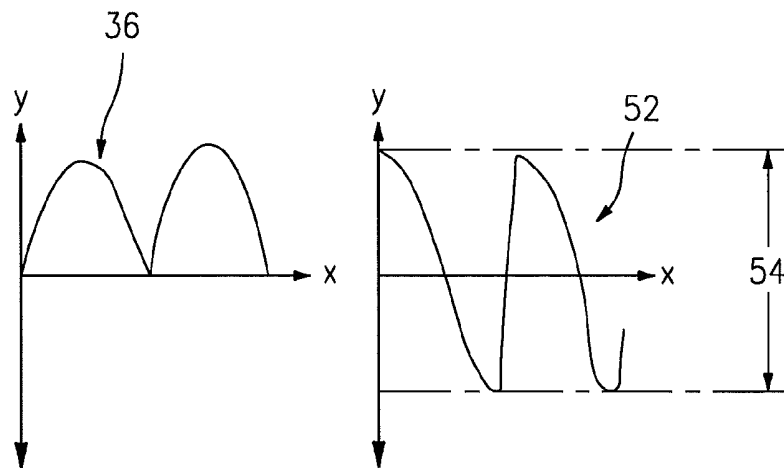


FIG. 7

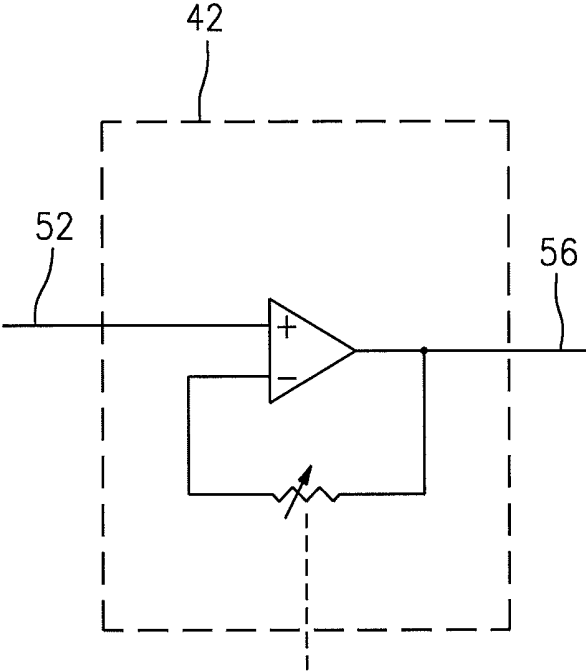


FIG. 8

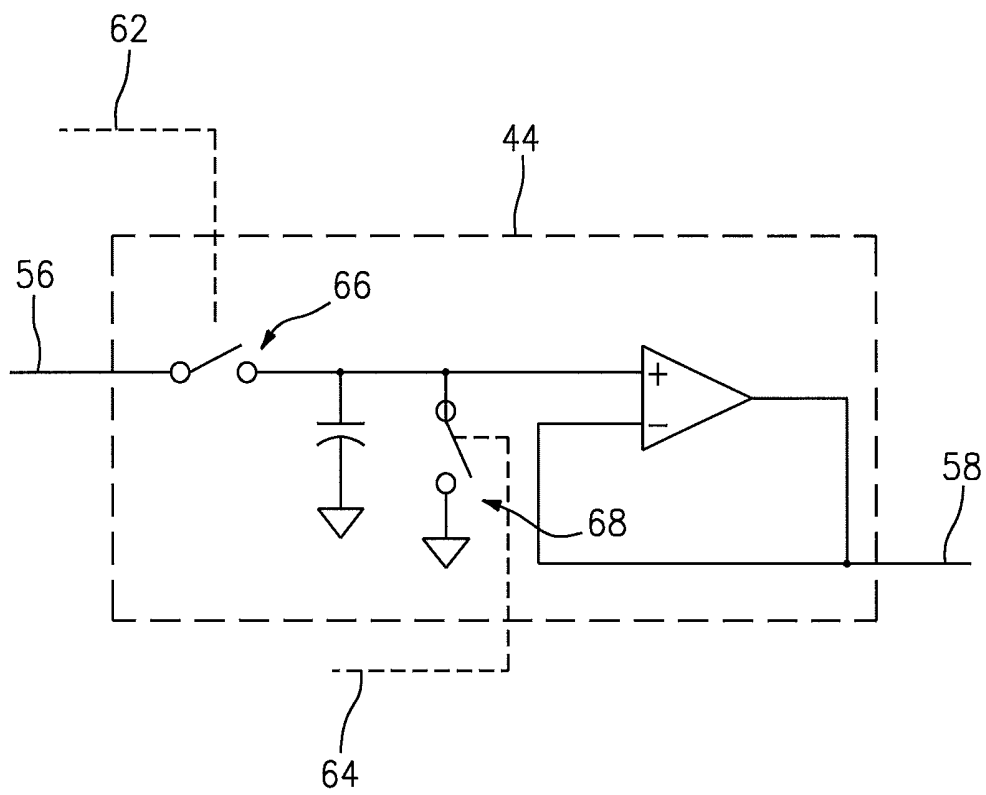


FIG. 9

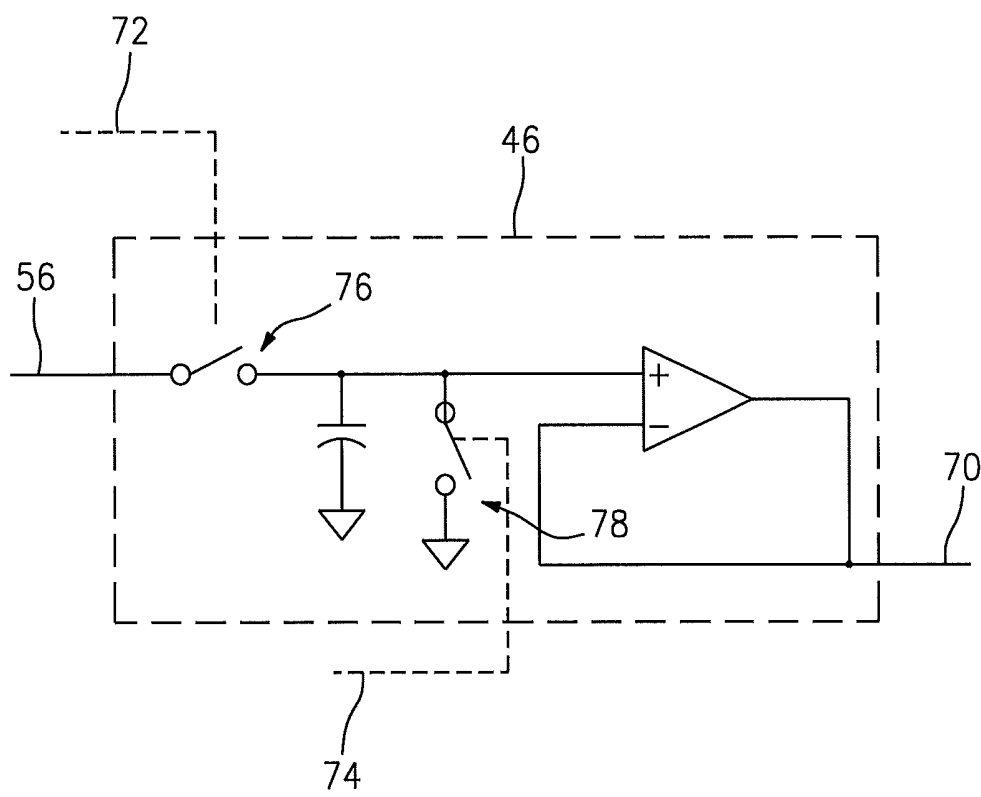


FIG. 10

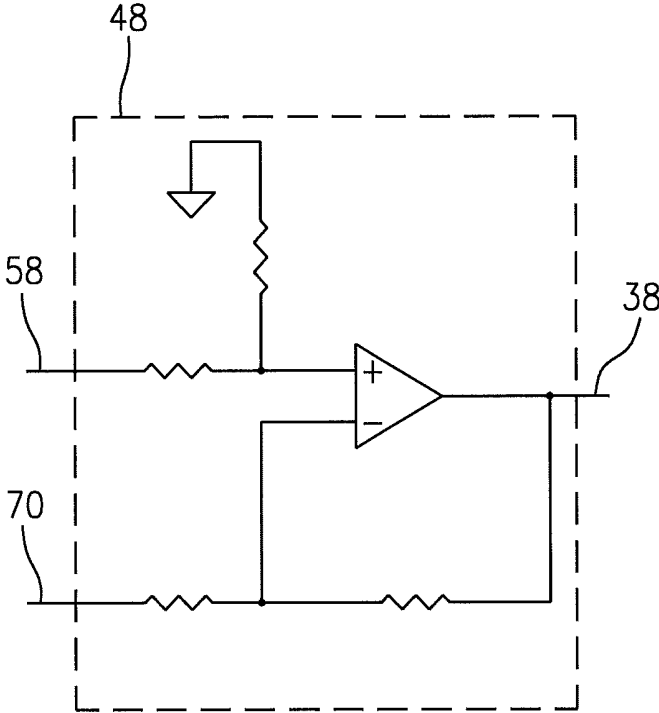


FIG. 11

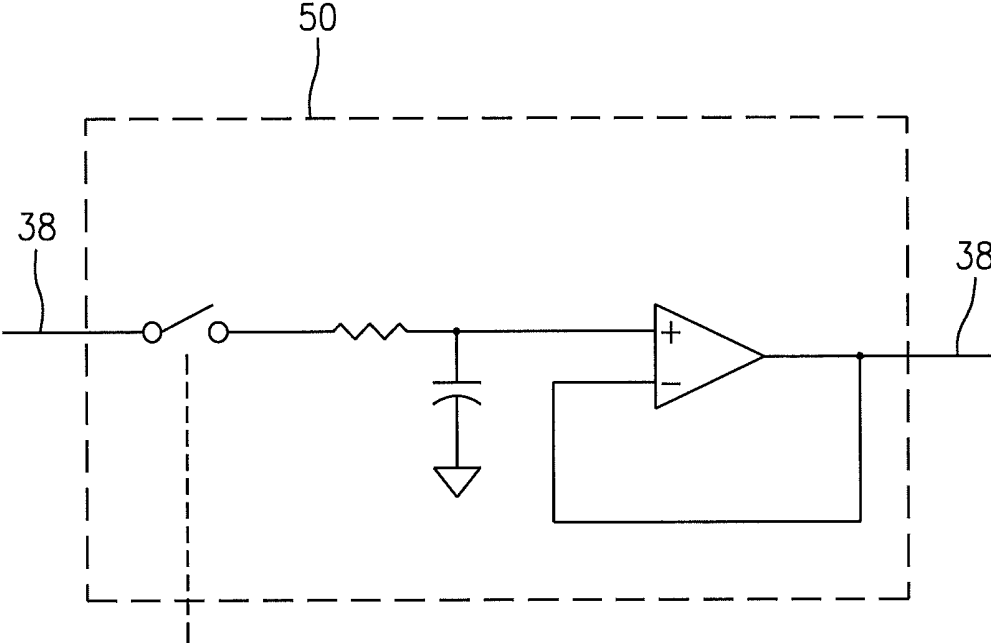


FIG. 12

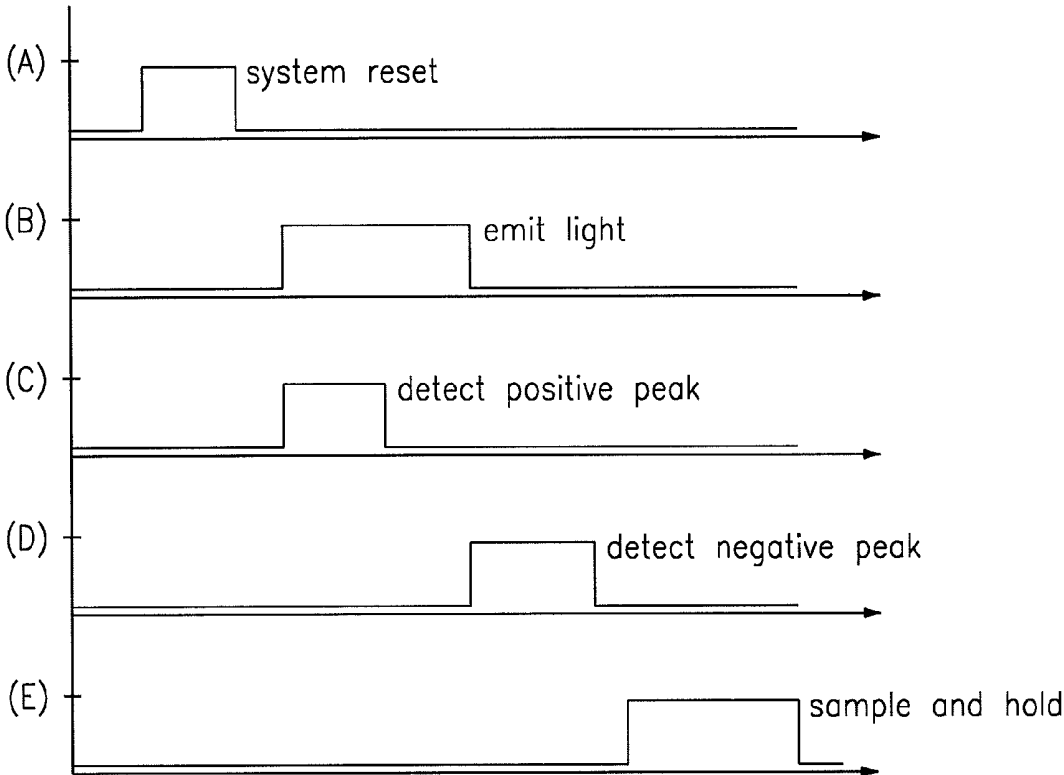


FIG. 13

# SYSTEMS AND METHODS FOR SPECTROSCOPIC MEASUREMENT OF A CHARACTERISTIC OF BIOLOGICAL TISSUE

This application claims priority to U.S. Patent Appln. No. 61/707,138 filed Sep. 28, 2012.

## BACKGROUND INFORMATION

Spectroscopic devices are commonly used to non-invasively measure a characteristic of biological tissue. Spectroscopic devices emit light into biological tissue and detect differences in light absorption to determine the concentration of certain constituents in the biological tissue (e.g., oxygen, hemoglobin, melanin, etc.). The performance of a spectroscopic device is dependent upon its ability to generate sufficient optical power to penetrate the biological tissue of interest and to distinguish against confounding noise (e.g., caused by background light or electrical interference within the environment). Signal-to-noise considerations favor maximizing the optical power of the light emitted into the biological tissue. However, problems can arise when spectroscopic devices output high optical power light for extended periods of time or at fast repetition rates. For example, under certain operation conditions, spectroscopic devices may become undesirably hot. To avoid such problems, spectroscopic devices may be configured to output high optical power light for only short, sequential durations of time. Such spectroscopic devices detect light signals over short, sequential durations of time. The short duration of the detected light signals can make it difficult to use aggressive filtering techniques to remove confounding noise from the detected light signals; e.g., aggressive filtering techniques may add distortion to short duration detected light signals. Aspects of the present invention are directed to systems and methods for spectroscopic measurement of a characteristic of biological tissue which involve output of light having high optical power, short duration, and/or fast repetition rate, which prevent a spectroscopic device from becoming undesirably hot, which involve filtering detected light signals to remove confounding noise, and which account for distortion added to detected light signals during filtering.

## SUMMARY OF THE INVENTION

According to an aspect of the present invention, a system for spectroscopic measurement of a characteristic of a biological tissue is provided. The system includes at least one light source, at least one light detector, and a processor. The at least one light source is operable to emit light that penetrates the biological tissue. The at least one light detector is operable to detect light emitted by the at least one light source and passed through the biological tissue, and is operable to convert the detected light into a detection signal, the detection signal including an unwanted noise component. The processor is operable to receive the detection signal, and is operable to determine an adjusted peak-to-peak amplitude value that is representative of an amplitude of the detection signal adjusted for the unwanted noise component.

According to another aspect of the present invention, a method for spectroscopic measurement of a characteristic of a biological tissue is provided. The method includes the steps of: (1) using at least one light source to emit light that penetrates the biological tissue; (2) using at least one light detector to detect light emitted by the at least one light

source and passed through the biological tissue, and to convert the detected light into a detection signal, the detection signal including an unwanted noise component; and (3) using a processor to process the detection signal and to determine an adjusted peak-to-peak amplitude value that is representative of an amplitude of the detection signal adjusted for the unwanted noise component.

These and other features and advantages of the present invention will become apparent in light of the drawings and detailed description of the present invention provided below.

## BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a diagrammatic illustration of a spectroscopy system embodiment.

FIG. 2 is a diagrammatic illustration of a sensor assembly embodiment applied to a subject.

FIG. 3 is a diagrammatic illustration of a detection circuit embodiment.

FIG. 4 is a diagrammatic illustration of a differentiating amplifier embodiment.

FIG. 5 is a plot showing a detection signal and its corresponding differentiated detection signal.

FIG. 6 is a plot showing a detection signal and its corresponding differentiated detection signal.

FIG. 7 is a plot showing a detection signal and its corresponding differentiated detection signal.

FIG. 8 is a diagrammatic illustration of an adjustable gain amplifier embodiment.

FIG. 9 is a diagrammatic illustration of a positive peak detector embodiment.

FIG. 10 is a diagrammatic illustration of a negative peak detector embodiment.

FIG. 11 is a diagrammatic illustration of a difference amplifier embodiment.

FIG. 12 is a diagrammatic illustration of a sample and hold device embodiment.

FIG. 13 is a timing diagram for the spectroscopy system.

## DESCRIPTION OF THE INVENTION

Referring to FIG. 1, an embodiment of the present spectroscopy system 10 includes at least one sensor assembly 12 connected to a base unit 14. In FIG. 1, the sensor assembly 12 is applied to a subject. The base unit 14 includes a display 16, operator controls 18, and a processor 20 for providing signals to and/or receiving signals from the sensor assembly 12. The processor 20 is configured to selectively perform the functions necessary to operate the sensor assembly 12. For ease of description, the functionality of the processor 20 will be described herein as being implemented at least in part using hardware—specifically, a detection circuit 22, discussed in detail below. A person skilled in the art will recognize that the functionality of the processor 20 might alternatively be implemented using other hardware, software, firmware, or a combination thereof.

FIG. 2 illustrates a sensor assembly 12 embodiment applied to a subject. The sensor assembly 12 includes a pad 24, a light source 26, and a light detector 28. The light source 26 and the light detector 28 are mounted to the pad 24. The light source 26 may be any device operable to emit light; e.g., the light source 26 may be a laser, a light emitting diode (LED), or another device. The light source 26 may emit light at one or more wavelengths. The light detector 28 may be any device operable to detect light emitted by the light source 26; e.g., the light detector 28 may be a photodiode, or another device. Although the system 10 illustrated in FIG.

1 includes only one light source **26** and one light detector **28**, in some embodiments the system **10** may include more than one light source **26** and/or more than one light detector **28**.

Referring to FIG. **2**, the sensor assembly **12** may be applied to a user so that the light source **26** emits input light **30** that penetrates a biological tissue of interest **32**. In FIG. **2**, the biological tissue of interest **32** is the brain. In alternative embodiments, the biological tissue of interest **32** may be tissue of the human finger, tissue of the human abdomen, or some other biological tissue. The input light **30** travels through the tissue **32** where it is attenuated, and subsequently exits the tissue as output light **34**, and is detected by the light detector **28**. The light detector **28** converts the detected output light **34** into a detection signal **36** (see FIG. **3**). The detection signal **36** may include an unwanted noise component that results, for example, from background light detected by the light detector **28**. As shown in FIG. **3**, the detection signal **36** is input to the detection circuit **22**. As will be discussed in detail below, the detection circuit **22** outputs an adjusted peak-to-peak amplitude value **38** that is representative of the amplitude of the detection signal **36** adjusted for an unwanted noise component that may be included in the detection signal **36**. The adjusted peak-to-peak amplitude value **38** thus provides an accurate measurement of a characteristic of the biological tissue of interest **32** (e.g., oxygen concentration, hemoglobin concentration, melanin concentration, etc.).

Referring to FIGS. **3-12**, an embodiment of the detection circuit **22** includes a differentiating amplifier **40**, an adjustable gain amplifier **42**, a positive peak detector **44**, a negative peak detector **46**, a difference amplifier **48**, and a sample and hold device **50**.

Referring to FIGS. **3** and **4**, the differentiating amplifier **40** receives the detection signal **36** and outputs a differentiated detection signal **52**. The differentiated detection signal **52** is the first derivative of the detection signal **36**. Whereas the detection signal **36** is a unipolar waveform, the differentiated detection signal **52** is a bipolar waveform. The differentiating amplifier **40** functions like a high-pass filter, removing some or all of the low frequency components of the detection signal **36**, which low frequency components may correspond to an unwanted noise component that may be included in the detection signal **36**. FIGS. **5-7** each illustrate a plot of a detection signal **36** and its corresponding differentiated detection signal **52**. In FIGS. **5-7**, the x-axes represent time and the y-axes represent voltage. The differentiated detection signal **52** includes a peak-to-peak amplitude **54**. FIGS. **5-7** each illustrate the peak-to-peak amplitude **54** of the respective differentiated detection signals **52**. The peak-to-peak amplitude **54** of the differentiated detection signal **52** is representative of the detection signal **36**, but may include an unwanted distortion component added by the differentiating amplifier **40**. Other components of the detection circuit **22** (e.g., the adjustable gain amplifier **42**, the positive peak detector **44**, the negative peak detector **46**, the difference amplifier **48**, etc.) work together to determine the adjusted peak-to-peak amplitude value **38**. The adjusted peak-to-peak amplitude value **38** accounts for an unwanted distortion component that may be added by the differentiating amplifier **40**. Also, as indicated above, the adjusted peak-to-peak amplitude value **38** is representative of the amplitude of the detection signal **36** adjusted for an unwanted noise component that may be included in the detection signal **36**. The differentiating amplifier **40** is not limited to the embodiment illustrated in FIG. **4**.

Referring to FIGS. **3** and **8**, the adjustable gain amplifier **42** receives the differentiated detection signal **52** and outputs

the differentiated and gain-adjusted detection signal **56**. The adjustable gain amplifier **42** multiplies the differentiated detection signal **52** by a multiplication factor to produce the differentiated and gain-adjusted detection signal **56**. The multiplication factor is selected to optimize the system **10** and to enable the system **10** to achieve a maximum dynamic range under most operational conditions. The adjustable gain amplifier **42** is not limited to the embodiment illustrated in FIG. **8**.

Referring to FIGS. **3** and **9**, the positive peak detector **44** receives the differentiated and gain-adjusted detection signal **56**. At an appropriate time period relating to a transition of the differentiated and gain-adjusted detection signal **56**, the positive peak detector **44** captures, holds, and ultimately outputs the maximum value of the differentiated and gain-adjusted detection signal **56** (hereinafter referred to as the "positive peak **58**" of the differentiated and gain-adjusted detection signal **56**). The positive peak detector **44** may capture and hold the positive peak **58**, for example, by charging a capacitor. Referring to FIG. **5**, the appropriate time period for detecting the positive peak **58** is identified by reference element "**60**". Timing control of the positive peak detector **44** can be implemented, for example, using a microcontroller or programmable logic. In the embodiment illustrated in FIG. **9**, inputs **62**, **64** received from a microcontroller are operable to open and close CMOS analog switches **66**, **68** of the positive peak detector **44**, respectively. The positive peak detector **44** is not limited to the embodiment illustrated in FIG. **9**.

Referring to FIGS. **3** and **10**, the negative peak detector **46** receives the differentiated and gain-adjusted detection signal **56**. At an appropriate time period relating to a transition of the differentiated and gain-adjusted detection signal **56**, the negative peak detector **46** captures, holds, and ultimately outputs the minimum value of the differentiated and gain-adjusted detection signal **56** (hereinafter referred to as the "negative peak **70**" of the differentiated and gain-adjusted detection signal **56**). The negative peak detector **46** may capture and hold the negative peak **70**, for example, by charging a capacitor. Referring to FIG. **5**, the appropriate time period for detecting the negative peak **70** is identified by reference element "**72**". In the embodiment illustrated in FIG. **10**, inputs **72**, **74** received from a microcontroller are operable to open and close CMOS analog switches **76**, **78** of the negative peak detector **46**, respectively. The negative peak detector **46** is not limited to the embodiment illustrated in FIG. **10**.

Referring to FIGS. **3** and **11**, the difference amplifier **48** receives as inputs the positive peak **58** and the negative peak **70** output by the positive peak detector **44** and the negative peak detector **46**, respectively. The difference amplifier **48** determines the absolute value of the sum of the positive peak **58** and the negative peak **70**, and outputs this value as the adjusted peak-to-peak amplitude value **38** described above. In some instances, unwanted signal components (e.g., unwanted noise components, unwanted distortion components, etc.) may be present in the differentiated and gain-adjusted detection signal **56**. Such unwanted signal components are processed by both the positive peak detector **44** and the negative peak detector **46**, and thus are cancelled out when the difference amplifier **48** determines the absolute value of the sum of the positive peak **58** and the negative peak **70**. The difference amplifier **48** is not limited to the embodiment illustrated in FIG. **11**.

Referring to FIGS. **3** and **12**, the sample and hold device **50** receives the adjusted peak-to-peak amplitude value **38** that is output by the difference amplifier **48**. The sample and

hold device 50 captures and holds the adjusted peak-to-peak amplitude value 38 until it can be read by the processor 20 of the system 10, at which time the sample and hold device 50 outputs the adjusted peak-to-peak amplitude value 38. The sample and hold device 50 is not limited to the embodiment illustrated in FIG. 12.

#### Operation

FIG. 13 illustrates a timing diagram for the system 10 illustrated in FIGS. 1-12. In FIG. 13, steps (A) through (E) are illustrated. In step (A), the system 10 is reset; e.g., any values previously captured and held by the positive peak detector 44, the negative peak detector 46, and the sample and hold device 50 are erased or reset. In step (B), for a predetermined period of time, the light source 26 emits input light 30 that penetrates the biological tissue of interest 32. In step (C), towards the beginning of the predetermined period of time of light emission by the light source 26, the light detector 28 detects the attenuated output light 34 exiting the biological tissue of interest 32, and converts the output light 34 into a detection signal 36, and the detection circuit 22 captures and holds the positive peak 58. In step (D), towards the end of the predetermined period of time of light emission by the light source 26, the detection circuit 22 captures and holds the negative peak 70. In step (E), the sample and hold device 50 receives from the difference amplifier 48 the adjusted peak-to-peak amplitude value 38, which is representative of the absolute value of the sum of the positive peak 58 and the negative peak 70. In step (E), the sample and hold device 50 captures and holds the adjusted peak-to-peak amplitude value 38 until it can be read by the processor 20 of the system 10. Steps (A) through (E) are sequentially repeated, providing the processor 20 with a plurality of adjusted peak-to-peak amplitude values 38, each being representative of the amplitude of the detection signal 36 adjusted for an unwanted noise component that may be included in the detection signal 36.

While various embodiments of the present invention have been disclosed, it will be apparent to those of ordinary skill in the art that many more embodiments and implementations are possible within the scope of the invention. Accordingly, the present invention is not to be restricted except in light of the attached claims and their equivalents.

What is claimed is:

1. A system for spectroscopic measurement of a characteristic of a biological tissue, the system comprising:  
 at least one light source operable to emit light that penetrates the biological tissue;  
 at least one light detector operable to detect light emitted by the at least one light source and passed through the biological tissue, and operable to convert the detected light into a detection signal; and  
 a processor operable to receive the detection signal, and operable to determine an adjusted peak-to-peak amplitude value that is representative of an amplitude of the detection signal adjusted to account for an unwanted noise component present in the detection signal, wherein the processor includes a detector circuit, the detector circuit comprising:  
 a differentiating amplifier operable to receive the detection signal, and operable to convert the detection signal into a differentiated detection signal;  
 an adjustable gain amplifier operable to receive the differentiated detection signal, and operable to convert the differentiated detection signal into a differentiated and gain-adjusted detection signal;

a positive peak detector operable to receive the differentiated and gain-adjusted detection signal, and operable to determine a maximum value of the differentiated and gain-adjusted detection signal; and  
 a negative peak detector operable to receive the differentiated and gain-adjusted detection signal, and operable to determine a minimum value of the differentiated and gain-adjusted detection signal.

2. The system of claim 1, the detector circuit comprising:  
 a difference amplifier operable to determine the adjusted peak-to-peak amplitude value using the maximum value received from the positive peak detector and the minimum value received from the negative peak detector; and

a sample and hold device operable to receive and hold the adjusted peak-to-peak amplitude value.

3. The system of claim 1, wherein the characteristic of the biological tissue is selected from the group consisting of: oxygen saturation, hemoglobin concentration, and melanin concentration.

4. The system of claim 1, wherein the processor is operable to determine the adjusted peak-to-peak amplitude value using the maximum value and the minimum value.

5. A method for spectroscopic measurement of a characteristic of a biological tissue, the method comprising the steps of:

using at least one light source to emit light that penetrates the biological tissue;

using at least one light detector to detect light emitted by the at least one light source and passed through the biological tissue, and to convert the detected light into a detection signal, the detection signal including an unwanted noise component; and

using a processor to process the detection signal and to determine an adjusted peak-to-peak amplitude value that is representative of an amplitude of the detection signal adjusted for the unwanted noise component present within the detection signal,

wherein the processor includes a detector circuit, the detector circuit comprising:

a differentiating amplifier that receives the detection signal and converts the detection signal into a differentiated detection signal;

an adjustable gain amplifier that receives the differentiated detection signal and converts the differentiated detection signal into a differentiated and gain-adjusted detection signal;

a positive peak detector that receives the differentiated and gain-adjusted detection signal and determines a maximum value of the differentiated and gain-adjusted detection signal; and

a negative peak detector that receives the differentiated and gain-adjusted detection signal and determines a minimum value of the differentiated and gain-adjusted detection signal.

6. The method of claim 5, wherein the characteristic of the biological tissue is selected from the group consisting of: oxygen saturation, hemoglobin concentration, and melanin concentration.

7. The method of claim 5, wherein the step of using the processor to process the detection signal and to determine the adjusted peak-to-peak amplitude value includes determining the adjusted peak-to-peak amplitude value using the maximum value and the minimum value.

专利名称(译)	用于光谱测量生物组织特征的系统和方法		
公开(公告)号	<a href="#">US9714969</a>	公开(公告)日	2017-07-25
申请号	US14/041733	申请日	2013-09-30
申请(专利权)人(译)	CAS医疗系统, INC.		
当前申请(专利权)人(译)	CAS医疗系统, INC.		
[标]发明人	KOSTURKO WILLIAM		
发明人	KOSTURKO, WILLIAM		
IPC分类号	H03F1/26 A61B5/1455 G01N21/00 A61B5/00 G01R29/26		
CPC分类号	G01R29/26 A61B5/0075 A61B5/14553 G01N21/00 A61B5/7225 A61B2576/026 G16H30/40		
审查员(译)	BHAT, ADITYA		
优先权	61/707138 2012-09-28 US		
其他公开文献	US20140100823A1		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

摘要(译)

提供了一种用于光谱测量生物组织特征的方法和系统。该方法包括以下步骤：(1)使用至少一个光源发射穿透生物组织的光；(2)使用至少一个光检测器检测由至少一个光源发出并通过生物组织的光，并将检测到的光转换为检测信号，检测信号包括不需要的噪声成分；(3)使用处理器处理检测信号并确定调整的峰峰值幅度值，该峰值幅度值表示针对不想要的噪声分量调整的检测信号的幅度。

