



US009848807B2

(12) **United States Patent**  
**Lamego**

(10) **Patent No.:** **US 9,848,807 B2**  
(45) **Date of Patent:** **\*Dec. 26, 2017**

(54) **TISSUE PROFILE WELLNESS MONITOR**

5/742 (2013.01); *A61B 5/7405* (2013.01);  
*A61B 5/746* (2013.01); *A61B 5/7475*  
(2013.01)

(71) Applicant: **Masimo Corporation**, Irvine, CA (US)

(72) Inventor: **Marcelo M. Lamego**, Cupertino, CA (US)

(58) **Field of Classification Search**

CPC ... A61B 5/0059; A61B 5/0075; A61B 5/1455;  
A61B 5/14551; A61B 5/75; A61B  
5/7405; A61B 5/742; A61B 5/746; A61B  
5/7271; A61B 5/7275

(73) Assignee: **MASIMO CORPORATION**, Irvine, CA (US)

See application file for complete search history.

(\* ) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 380 days.

(56) **References Cited**

This patent is subject to a terminal disclaimer.

U.S. PATENT DOCUMENTS

3,910,701 A 10/1975 Henderson et al.  
3,998,550 A 12/1976 Konishi et al.  
4,014,321 A 3/1977 March

(Continued)

(21) Appl. No.: **14/599,342**

(22) Filed: **Jan. 16, 2015**

FOREIGN PATENT DOCUMENTS

(65) **Prior Publication Data**

US 2015/0196237 A1 Jul. 16, 2015

DE 3244695 C2 10/1985  
EP 0 231 379 8/1987

(Continued)

**Related U.S. Application Data**

OTHER PUBLICATIONS

(63) Continuation of application No. 13/764,007, filed on Feb. 11, 2013, now Pat. No. 8,965,471, which is a continuation of application No. 12/106,969, filed on Apr. 21, 2008, now Pat. No. 8,374,665.

US 8,845,543, 09/2014, Diab et al. (withdrawn)

(Continued)

(60) Provisional application No. 60/925,811, filed on Apr. 21, 2007.

*Primary Examiner* — Eric Winakur

(74) *Attorney, Agent, or Firm* — Knobbe Martens Olson & Bear LLP

(51) **Int. Cl.**

*A61B 5/1455* (2006.01)  
*A61B 5/00* (2006.01)  
*A61B 5/024* (2006.01)  
*A61B 5/0295* (2006.01)


(57) **ABSTRACT**

A tissue profile wellness monitor measures a physiological parameter, generates a tissue profile, defines limits and indicates when the tissue profile exceeds the defined limits. The physiological parameter is responsive to multiple wavelengths of optical radiation after attenuation by constituents of pulsatile blood flowing within a tissue site. The tissue profile is responsive to the physiological parameter. The limits are defined for at least a portion of the tissue profile.

(52) **U.S. Cl.**

CPC ..... *A61B 5/14551* (2013.01); *A61B 5/0295* (2013.01); *A61B 5/02416* (2013.01); *A61B 5/72* (2013.01); *A61B 5/7275* (2013.01); *A61B*

**15 Claims, 5 Drawing Sheets**

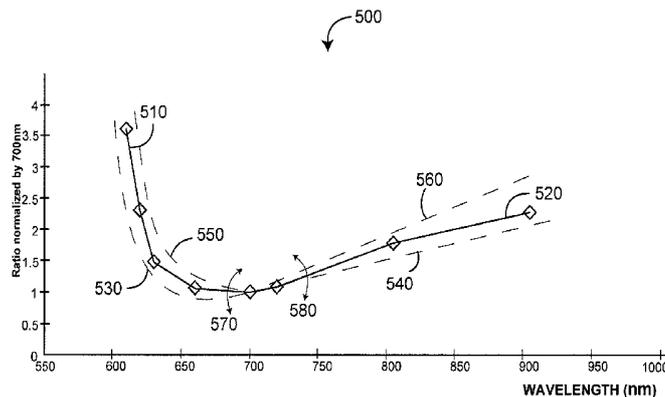

(56)

## References Cited

## U.S. PATENT DOCUMENTS

4,051,522 A	9/1977	Healy et al.	5,259,381 A	11/1993	Chung
4,157,708 A	6/1979	Imura	5,267,562 A	12/1993	Ukawa et al.
4,167,331 A	9/1979	Nielsen	5,267,563 A	12/1993	Swedlow et al.
4,266,554 A	5/1981	Hamaguri	5,278,627 A	1/1994	Aoyagi
4,267,844 A	5/1981	Yamanishi	5,297,548 A	3/1994	Pologe
4,295,475 A	10/1981	Torzala	5,313,940 A	5/1994	Fuse et al.
4,331,161 A	5/1982	Patel	5,319,355 A	6/1994	Russek
4,399,824 A	8/1983	Davidson	5,331,549 A	7/1994	Crawford, Jr.
4,446,871 A	5/1984	Imura	5,335,659 A	8/1994	Pologe et al.
4,531,527 A	7/1985	Reinhold, Jr. et al.	5,337,744 A	8/1994	Branigan
4,561,440 A	12/1985	Kubo et al.	5,337,745 A	8/1994	Benaron
4,586,513 A	5/1986	Hamaguri	5,341,805 A	8/1994	Stavridi et al.
4,603,700 A	8/1986	Nichols et al.	5,348,004 A	9/1994	Hollub
4,621,643 A	11/1986	New et al.	5,351,685 A	10/1994	Potratz
4,653,498 A	3/1987	New, Jr. et al.	5,355,129 A	10/1994	Baumann
4,655,225 A	4/1987	Dahne et al.	5,355,880 A	10/1994	Thomas et al.
4,685,464 A	8/1987	Goldberger et al.	5,355,882 A	10/1994	Ukawa et al.
4,694,833 A	9/1987	Hamaguri	5,361,758 A	11/1994	Hall et al.
4,695,955 A	9/1987	Faisandier	5,368,041 A	11/1994	Shambroom
4,700,708 A	10/1987	New et al.	5,368,224 A	11/1994	Richardson et al.
4,714,341 A	12/1987	Hamaguri et al.	D353,195 S	12/1994	Savage et al.
4,770,179 A	9/1988	New et al.	D353,196 S	12/1994	Savage et al.
4,773,422 A	9/1988	Isaacson et al.	5,370,114 A	12/1994	Wong et al.
4,781,195 A	11/1988	Martin	5,372,136 A	12/1994	Steuer et al.
4,800,885 A	1/1989	Johnson	5,377,676 A	1/1995	Vari et al.
4,805,623 A	2/1989	Jobsis	5,383,874 A	1/1995	Jackson et al.
4,822,997 A	4/1989	Fuller et al.	5,385,143 A	1/1995	Aoyagi
4,832,484 A	5/1989	Aoyagi et al.	5,387,122 A	2/1995	Goldberger et al.
4,846,183 A	7/1989	Martin	5,392,777 A	2/1995	Swedlow et al.
4,854,328 A	8/1989	Pollack	5,400,267 A	3/1995	Denen et al.
4,863,265 A	9/1989	Flower et al.	5,413,101 A	5/1995	Sugiura
4,867,571 A	9/1989	Frick et al.	D359,546 S	6/1995	Savage et al.
4,868,476 A	9/1989	Respaut	5,421,329 A	6/1995	Casciani et al.
4,869,254 A	9/1989	Stone et al.	5,424,545 A	6/1995	Block et al.
4,890,306 A	12/1989	Noda	5,425,362 A	6/1995	Siker et al.
4,907,876 A	3/1990	Suzuki et al.	5,425,375 A	6/1995	Chin et al.
4,911,167 A	3/1990	Corenman et al.	5,427,093 A	6/1995	Ogawa et al.
4,934,372 A	6/1990	Corenman et al.	5,429,128 A	7/1995	Cadell et al.
4,938,218 A	7/1990	Goodman et al.	5,431,170 A	7/1995	Mathews
4,942,877 A	7/1990	Sakai et al.	5,435,309 A	7/1995	Thomas et al.
4,955,379 A	9/1990	Hall	D361,840 S	8/1995	Savage et al.
4,960,126 A	10/1990	Conlon et al.	D362,063 S	9/1995	Savage et al.
4,960,128 A	10/1990	Gordon et al.	5,452,717 A	9/1995	Branigan et al.
4,964,010 A	10/1990	Miyasaka et al.	D363,120 S	10/1995	Savage et al.
4,964,408 A	10/1990	Hink et al.	5,456,252 A	10/1995	Vari et al.
4,967,571 A	11/1990	Sporri	5,469,845 A	11/1995	DeLonzor et al.
4,975,581 A	12/1990	Robinson et al.	RE35,122 E	12/1995	Corenman et al.
4,975,647 A	12/1990	Downer et al.	5,479,934 A	1/1996	Imran
4,986,665 A	1/1991	Yamanishi et al.	5,482,036 A	1/1996	Diab et al.
4,996,975 A	3/1991	Nakamura	5,487,386 A	1/1996	Wakabayashi et al.
4,997,769 A	3/1991	Lundsgaard	5,490,505 A	2/1996	Diab et al.
5,003,979 A	4/1991	Merickel et al.	5,490,523 A	2/1996	Isaacson et al.
5,025,791 A	6/1991	Niwa	5,494,032 A	2/1996	Robinson et al.
RE33,643 E	7/1991	Isaacson et al.	5,494,043 A	2/1996	O'Sullivan et al.
5,028,787 A	7/1991	Rosenthal et al.	5,503,148 A	4/1996	Pologe et al.
5,033,472 A	7/1991	Sato et al.	5,520,177 A	5/1996	Ogawa
5,041,187 A	8/1991	Hink et al.	5,528,519 A	6/1996	Ohkura et al.
5,054,495 A	10/1991	Uemura et al.	5,533,507 A	7/1996	Potratz
5,058,588 A	10/1991	Kaestle	5,533,511 A	7/1996	Kaspari et al.
5,069,213 A	12/1991	Polczynski	5,534,851 A	7/1996	Russek
5,077,476 A	12/1991	Rosenthal	5,551,423 A	9/1996	Sugiura
5,078,136 A	1/1992	Stone et al.	5,553,615 A	9/1996	Carim et al.
5,101,825 A	4/1992	Gravenstein et al.	5,555,882 A	9/1996	Richardson et al.
5,137,023 A	8/1992	Mendelson et al.	5,561,275 A	10/1996	Savage et al.
5,155,697 A	10/1992	Bunsen	5,562,002 A	10/1996	Lalin
5,162,725 A	11/1992	Hodson et al.	5,575,284 A	11/1996	Athan et al.
5,163,438 A	11/1992	Gordon et al.	5,577,500 A	11/1996	Potratz
5,188,108 A	2/1993	Secker	5,584,299 A	12/1996	Sakai et al.
5,189,609 A	2/1993	Tivig et al.	5,588,427 A	12/1996	Tien
5,190,040 A	3/1993	Aoyagi	5,590,649 A	1/1997	Caro et al.
5,209,230 A	5/1993	Swedlow et al.	5,590,652 A	1/1997	Inai
5,226,053 A	7/1993	Cho et al.	5,595,176 A	1/1997	Yamaura
5,226,417 A	7/1993	Swedlow et al.	5,596,992 A	1/1997	Haaland et al.
5,246,002 A	9/1993	Prosser	5,602,924 A	2/1997	Durand et al.
5,247,931 A	9/1993	Norwood	5,603,323 A	2/1997	Pflugrath et al.
			5,603,623 A	2/1997	Nishikawa et al.
			5,615,672 A	4/1997	Braig et al.
			5,617,857 A	4/1997	Chader et al.
			5,630,413 A	5/1997	Thomas et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

5,632,272 A	5/1997	Diab et al.	5,885,213 A	3/1999	Richardson et al.
5,638,816 A	6/1997	Kiani-Azarbayjany et al.	5,890,929 A	4/1999	Mills et al.
5,638,818 A	6/1997	Diab et al.	5,891,022 A	4/1999	Pologe
5,645,059 A	7/1997	Fein et al.	5,891,024 A	4/1999	Jarman et al.
5,645,060 A	7/1997	Yorkey	5,900,632 A	5/1999	Sterling et al.
5,645,440 A	7/1997	Tobler et al.	5,904,654 A	5/1999	Wohltmann et al.
5,651,780 A	7/1997	Jackson et al.	5,910,108 A	6/1999	Solenberger
5,658,248 A	8/1997	Klein et al.	5,916,154 A	6/1999	Hobbs et al.
5,660,567 A	8/1997	Nierlich et al.	5,919,133 A	7/1999	Taylor
5,662,106 A	9/1997	Swedlow et al.	5,919,134 A	7/1999	Diab
5,676,139 A	10/1997	Goldberger et al.	5,921,921 A	7/1999	Potratz et al.
5,676,141 A	10/1997	Hollub	5,934,277 A	8/1999	Mortz
5,678,544 A	10/1997	Delonzor et al.	5,934,925 A	8/1999	Tobler et al.
5,685,299 A	11/1997	Diab et al.	5,939,609 A	8/1999	Knapp et al.
5,685,301 A	11/1997	Klomhaus	5,940,182 A	8/1999	Lepper, Jr. et al.
5,687,719 A	11/1997	Sato et al.	5,954,644 A	9/1999	Dettling
5,687,722 A	11/1997	Tien et al.	5,976,466 A	11/1999	Ratner et al.
5,690,104 A	11/1997	Kanemoto et al.	5,978,691 A	11/1999	Mills
5,692,503 A	12/1997	Kuenstner	5,983,122 A	11/1999	Jarman et al.
5,697,371 A	12/1997	Aoyagi	5,987,343 A	11/1999	Kinast
5,713,355 A	2/1998	Richardson et al.	5,991,355 A	11/1999	Dahlke
5,719,589 A	2/1998	Norman et al.	5,995,855 A	11/1999	Kiani et al.
5,720,284 A	2/1998	Aoyagi et al.	5,995,856 A	11/1999	Mannheimer et al.
5,720,293 A	2/1998	Quinn et al.	5,995,859 A	11/1999	Takahashi
D393,830 S	4/1998	Tobler et al.	5,997,343 A	12/1999	Mills et al.
5,742,718 A	4/1998	Harman et al.	5,999,841 A	12/1999	Aoyagi et al.
5,743,262 A	4/1998	Lepper, Jr. et al.	6,002,952 A	12/1999	Diab et al.
5,743,263 A	4/1998	Baker, Jr.	6,006,119 A	12/1999	Soller et al.
5,746,206 A	5/1998	Mannheimer	6,011,986 A	1/2000	Diab et al.
5,746,697 A	5/1998	Swedlow et al.	6,014,576 A	1/2000	Raley
5,752,914 A	5/1998	Delonzor et al.	6,018,673 A	1/2000	Chin et al.
5,755,226 A	5/1998	Carim et al.	6,018,674 A	1/2000	Aronow
5,758,644 A	6/1998	Diab et al.	6,023,541 A	2/2000	Merchant et al.
5,760,910 A	6/1998	Lepper, Jr. et al.	6,027,452 A	2/2000	Flaherty et al.
5,769,785 A	6/1998	Diab et al.	6,035,223 A	3/2000	Baker, Jr.
5,772,587 A	6/1998	Gratton et al.	6,036,642 A	3/2000	Diab et al.
5,779,630 A	7/1998	Fein et al.	6,045,509 A	4/2000	Caro et al.
5,782,237 A	7/1998	Casciani et al.	6,064,898 A	5/2000	Aldrich
5,782,756 A	7/1998	Mannheimer	6,067,462 A	5/2000	Diab et al.
5,782,757 A	7/1998	Diab et al.	6,068,594 A	5/2000	Schloemer et al.
5,785,659 A	7/1998	Caro et al.	6,073,037 A	6/2000	Alam et al.
5,790,729 A	8/1998	Pologe et al.	6,081,735 A	6/2000	Diab et al.
5,791,347 A	8/1998	Flaherty et al.	6,083,172 A	7/2000	Baker, Jr. et al.
5,792,052 A	8/1998	Isaacson et al.	6,088,607 A	7/2000	Diab et al.
5,793,485 A	8/1998	Gourley	6,094,592 A	7/2000	Yorkey et al.
5,800,348 A	9/1998	Kaestle et al.	6,104,938 A	8/2000	Huiku
5,800,349 A	9/1998	Isaacson et al.	6,110,522 A	8/2000	Lepper, Jr. et al.
5,803,910 A	9/1998	Potratz	6,112,107 A	8/2000	Hannula
5,807,246 A	9/1998	Sakaguchi et al.	6,122,042 A	9/2000	Wunderman et al.
5,807,247 A	9/1998	Merchant et al.	6,124,597 A	9/2000	Shehada et al.
5,810,723 A	9/1998	Aldrich	6,128,521 A	10/2000	Marro et al.
5,810,724 A	9/1998	Gronvall	6,129,675 A	10/2000	Jay
5,810,734 A	9/1998	Caro et al.	6,132,363 A	10/2000	Freed et al.
5,817,010 A	10/1998	Hibl	6,144,868 A	11/2000	Parker
5,818,985 A	10/1998	Merchant et al.	6,149,588 A	11/2000	Noda et al.
5,823,950 A	10/1998	Diab et al.	6,151,516 A	11/2000	Kiani-Azarbayjany et al.
5,823,952 A	10/1998	Levinson et al.	6,151,518 A	11/2000	Hayashi
5,827,182 A	10/1998	Raley et al.	6,152,754 A	11/2000	Gerhardt et al.
5,830,121 A	11/1998	Enomoto et al.	6,154,667 A	11/2000	Miura et al.
5,830,131 A	11/1998	Caro et al.	6,157,041 A	12/2000	Thomas et al.
5,830,137 A	11/1998	Sharf	6,157,850 A	12/2000	Diab et al.
5,833,618 A	11/1998	Caro et al.	6,163,715 A	12/2000	Larsen et al.
5,839,439 A	11/1998	Nierlich et al.	6,165,005 A	12/2000	Mills et al.
RE36,000 E	12/1998	Swedlow et al.	6,165,173 A	12/2000	Kamdar et al.
5,842,979 A	12/1998	Jarman	6,174,283 B1	1/2001	Nevo et al.
5,846,190 A	12/1998	Woehrle	6,175,752 B1	1/2001	Say et al.
5,850,443 A	12/1998	Van Oorschot et al.	6,184,521 B1	2/2001	Coffin et al.
5,851,178 A	12/1998	Aronow	6,192,261 B1	2/2001	Gratton et al.
5,851,179 A	12/1998	Ritson et al.	6,206,830 B1	3/2001	Diab et al.
5,853,364 A	12/1998	Baker, Jr. et al.	6,226,539 B1	5/2001	Potratz
5,857,462 A	1/1999	Thomas et al.	6,229,856 B1	5/2001	Diab et al.
5,860,099 A	1/1999	Milios et al.	6,230,035 B1	5/2001	Aoyagi et al.
5,860,919 A	1/1999	Kiani-Azarbayjany et al.	6,232,609 B1	5/2001	Snyder et al.
5,865,736 A	2/1999	Baker, Jr. et al.	6,236,872 B1	5/2001	Diab et al.
5,876,348 A	3/1999	Sugo	6,237,604 B1	5/2001	Burnside et al.
			6,241,683 B1	6/2001	Macklem et al.
			6,248,083 B1	6/2001	Smith et al.
			6,253,097 B1	6/2001	Aronow et al.
			6,256,523 B1	7/2001	Diab et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

6,262,698	B1	7/2001	Blum	6,528,809	B1	3/2003	Thomas et al.
6,263,222	B1	7/2001	Diab et al.	6,537,225	B1	3/2003	Mills
6,266,551	B1	7/2001	Osadchy et al.	6,541,756	B2	4/2003	Schulz et al.
6,272,363	B1	8/2001	Casciani et al.	6,542,763	B1	4/2003	Yamashita et al.
6,278,522	B1	8/2001	Lepper, Jr. et al.	6,542,764	B1	4/2003	Al-Ali et al.
6,280,213	B1	8/2001	Tobler et al.	6,545,652	B1	4/2003	Tsuji
6,285,895	B1	9/2001	Ristolainen et al.	6,546,267	B1	4/2003	Sugiura
6,285,896	B1	9/2001	Tobler et al.	6,553,241	B2	4/2003	Mannheimer et al.
6,295,330	B1	9/2001	Skog et al.	6,564,077	B2	5/2003	Mortara
6,298,252	B1	10/2001	Kovach et al.	6,571,113	B1	5/2003	Fein et al.
6,298,255	B1	10/2001	Cordero et al.	6,580,086	B1	6/2003	Schulz et al.
6,301,493	B1	10/2001	Marro et al.	6,582,964	B1	6/2003	Samsoundar et al.
6,304,675	B1	10/2001	Osbourm et al.	6,584,336	B1	6/2003	Ali et al.
6,304,767	B1	10/2001	Soller et al.	6,584,413	B1	6/2003	Keenan et al.
6,308,089	B1	10/2001	von der Ruhr	6,591,123	B2	7/2003	Fein et al.
6,317,627	B1	11/2001	Ennen et al.	6,594,511	B2	7/2003	Stone et al.
6,321,100	B1	11/2001	Parker	6,594,518	B1	7/2003	Benaron et al.
6,325,761	B1	12/2001	Jay	6,595,316	B2	7/2003	Cybulski et al.
6,330,468	B1	12/2001	Scharf	6,597,932	B2	7/2003	Tian et al.
6,334,065	B1	12/2001	Al-Ali et al.	6,597,933	B2	7/2003	Kiani et al.
6,336,900	B1	1/2002	Alleckson et al.	6,600,940	B1	7/2003	Fein et al.
6,339,715	B1	1/2002	Bahr et al.	6,606,509	B2	8/2003	Schmitt
6,341,257	B1	1/2002	Haaland	6,606,510	B2	8/2003	Swedlow et al.
6,343,224	B1	1/2002	Parker	6,606,511	B1	8/2003	Ali et al.
6,349,228	B1	2/2002	Kiani et al.	6,609,016	B1	8/2003	Lynn
6,351,658	B1	2/2002	Middleman et al.	6,611,698	B1	8/2003	Yamashita et al.
6,356,774	B1	3/2002	Bernstein et al.	6,614,521	B2	9/2003	Samsoundar et al.
6,360,113	B1	3/2002	Dettling	6,615,064	B1	9/2003	Aldrich
6,360,114	B1	3/2002	Diab et al.	6,615,151	B1	9/2003	Seccina et al.
6,363,269	B1	3/2002	Hanna et al.	6,618,602	B2	9/2003	Levin
6,368,283	B1	4/2002	Xu et al.	6,622,095	B2	9/2003	Kobayashi et al.
6,371,921	B1	4/2002	Caro et al.	6,628,975	B1	9/2003	Fein et al.
6,374,129	B1	4/2002	Chin et al.	6,631,281	B1	10/2003	Kastle
6,377,828	B1	4/2002	Chaiken et al.	6,632,181	B2	10/2003	Flaherty et al.
6,377,829	B1	4/2002	Al-Ali	6,639,668	B1	10/2003	Trepagnier
6,388,240	B2	5/2002	Schulz et al.	6,640,116	B2	10/2003	Diab
6,393,310	B1	5/2002	Kuenstner	6,643,530	B2	11/2003	Diab et al.
6,397,091	B2	5/2002	Diab et al.	6,645,142	B2	11/2003	Braig et al.
6,397,092	B1	5/2002	Norris et al.	6,650,917	B2	11/2003	Diab et al.
6,397,093	B1	5/2002	Aldrich	6,654,623	B1	11/2003	Kastle
6,408,198	B1	6/2002	Hanna et al.	6,654,624	B2	11/2003	Diab et al.
6,411,833	B1	6/2002	Baker, Jr. et al.	6,657,717	B2	12/2003	Cadell et al.
6,415,166	B1	7/2002	Van Hoy et al.	6,658,276	B2	12/2003	Kianl et al.
6,415,233	B1	7/2002	Haaland	6,658,277	B2	12/2003	Wasserman
6,415,236	B2	7/2002	Kobayashi et al.	6,661,161	B1	12/2003	Lanzo et al.
6,421,549	B1	7/2002	Jacques	6,662,033	B2	12/2003	Casciani et al.
6,430,437	B1	8/2002	Marro	6,665,551	B1	12/2003	Suzuki
6,430,525	B1	8/2002	Weber et al.	6,668,183	B2	12/2003	Hicks et al.
6,434,408	B1	8/2002	Heckel	6,671,526	B1	12/2003	Aoyagi et al.
6,441,388	B1	8/2002	Thomas et al.	6,671,531	B2	12/2003	Al-Ali et al.
6,453,184	B1	9/2002	Hyogo et al.	6,675,031	B1	1/2004	Porges et al.
6,455,340	B1	9/2002	Chua et al.	6,675,106	B1	1/2004	Keenan et al.
6,463,310	B1	10/2002	Swedlow et al.	6,676,600	B1	1/2004	Conero et al.
6,463,311	B1	10/2002	Diab	6,678,543	B2	1/2004	Diab et al.
6,466,824	B1	10/2002	Struble	6,681,126	B2	1/2004	Solenberger
6,470,199	B1	10/2002	Kopotic et al.	6,684,090	B2	1/2004	Ali et al.
6,480,729	B2	11/2002	Stone	6,684,091	B2	1/2004	Parker
6,490,466	B1	12/2002	Fein et al.	6,687,620	B1	2/2004	Haaland et al.
6,490,684	B1	12/2002	Fenstemaker et al.	6,690,466	B2	2/2004	Miller et al.
6,497,659	B1	12/2002	Rafert	6,694,157	B1	2/2004	Stone et al.
6,501,974	B2	12/2002	Huiku	6,697,655	B2	2/2004	Sueppel et al.
6,501,975	B2	12/2002	Diab et al.	6,697,656	B1	2/2004	Al-Ali
6,504,943	B1	1/2003	Sweatt et al.	6,697,657	B1	2/2004	Shehada et al.
6,505,059	B1	1/2003	Kollias et al.	6,697,658	B2	2/2004	Al-Ali
6,505,060	B1	1/2003	Norris	RE38,476	E	3/2004	Diab et al.
6,505,061	B2	1/2003	Larson	6,699,194	B1	3/2004	Diab et al.
6,505,133	B1	1/2003	Hanna	6,701,170	B2	3/2004	Stetson
6,510,329	B2	1/2003	Heckel	6,708,049	B1	3/2004	Berson et al.
6,515,273	B2	2/2003	Al-Ali	6,711,503	B2	3/2004	Haaland
6,519,486	B1	2/2003	Edgar, Jr. et al.	6,714,803	B1	3/2004	Mortz
6,519,487	B1	2/2003	Parker	6,714,804	B2	3/2004	Al-Ali et al.
6,522,398	B2	2/2003	Cadell et al.	6,714,805	B2	3/2004	Jeon et al.
6,525,386	B1	2/2003	Mills et al.	RE38,492	E	4/2004	Diab et al.
6,526,300	B1	2/2003	Kiani et al.	6,719,705	B2	4/2004	Mills
6,526,301	B2	2/2003	Larsen et al.	6,720,734	B2	4/2004	Norris
				6,721,582	B2	4/2004	Trepagnier et al.
				6,721,584	B2	4/2004	Baker, Jr. et al.
				6,721,585	B1	4/2004	Parker
				6,725,074	B1	4/2004	Kastle

(56)

## References Cited

## U.S. PATENT DOCUMENTS

6,725,075	B2	4/2004	Al-Ali	7,003,338	B2	2/2006	Weber et al.
6,726,634	B2	4/2004	Freeman	7,003,339	B2	2/2006	Diab et al.
6,728,560	B2	4/2004	Kollias et al.	7,006,856	B2	2/2006	Baker, Jr. et al.
6,735,459	B2	5/2004	Parker	7,015,451	B2	3/2006	Dalke et al.
6,741,875	B1	5/2004	Pawluczyk et al.	7,024,233	B2	4/2006	Ali et al.
6,741,876	B1	5/2004	Seccina et al.	7,027,849	B2	4/2006	Al-Ali
6,743,172	B1	6/2004	Blike	7,030,749	B2	4/2006	Al-Ali
6,745,060	B2	6/2004	Diab et al.	7,039,449	B2	5/2006	Al-Ali
6,745,061	B1	6/2004	Hicks et al.	7,041,060	B2	5/2006	Flaherty et al.
6,748,253	B2	6/2004	Norris et al.	7,044,918	B2	5/2006	Diab
6,748,254	B2	6/2004	O'Neil et al.	7,067,893	B2	6/2006	Mills et al.
6,754,515	B1	6/2004	Pologe	7,096,052	B2	8/2006	Mason et al.
6,754,516	B2	6/2004	Mannheimer	7,096,054	B2	8/2006	Abdul-Hafiz et al.
6,760,607	B2	7/2004	Al-Ali	7,132,641	B2	11/2006	Schulz et al.
6,760,609	B2	7/2004	Jacques	7,142,901	B2	11/2006	Kiani et al.
6,770,028	B1	8/2004	Ali et al.	7,149,561	B2	12/2006	Diab
6,771,994	B2	8/2004	Kiani et al.	7,186,966	B2	3/2007	Al-Ali
6,773,397	B2	8/2004	Kelly	7,190,261	B2	3/2007	Al-Ali
6,778,923	B2	8/2004	Norris et al.	7,215,984	B2	5/2007	Diab et al.
6,780,158	B2	8/2004	Yarita	7,215,986	B2	5/2007	Diab et al.
6,788,849	B1	9/2004	Pawluczyk	7,221,971	B2	5/2007	Diab et al.
6,792,300	B1	9/2004	Diab et al.	7,225,006	B2	5/2007	Al-Ali et al.
6,800,373	B2	10/2004	Gorczyca	7,225,007	B2	5/2007	Al-Ali et al.
6,801,797	B2	10/2004	Mannheimer et al.	RE39,672	E	6/2007	Shehada et al.
6,801,799	B2	10/2004	Mendelson	7,239,905	B2	7/2007	Kiani-Azarbayjany et al.
6,810,277	B2	10/2004	Edgar, Jr. et al.	7,245,953	B1	7/2007	Parker
6,813,511	B2	11/2004	Diab et al.	7,254,429	B2	8/2007	Schurman et al.
6,816,741	B2	11/2004	Diab	7,254,431	B2	8/2007	Al-Ali et al.
6,819,950	B2	11/2004	Mills	7,254,433	B2	8/2007	Diab et al.
6,822,564	B2	11/2004	Al-Ali	7,254,434	B2	8/2007	Schulz et al.
6,825,619	B2	11/2004	Norris	7,272,425	B2	9/2007	Al-Ali
6,826,419	B2	11/2004	Diab et al.	7,274,955	B2	9/2007	Kiani et al.
6,829,496	B2	12/2004	Nagai et al.	D554,263	S	10/2007	Al-Ali
6,829,501	B2	12/2004	Nielsen et al.	7,280,858	B2	10/2007	Al-Ali et al.
6,830,711	B2	12/2004	Mills et al.	7,289,835	B2	10/2007	Mansfield et al.
6,836,679	B2	12/2004	Baker, Jr. et al.	7,292,883	B2	11/2007	De Felice et al.
6,839,579	B1	1/2005	Chin	7,295,866	B2	11/2007	Al-Ali
6,839,580	B2	1/2005	Zonios et al.	7,299,080	B2	11/2007	Acosta et al.
6,839,582	B2	1/2005	Heckel	7,328,053	B1	2/2008	Diab et al.
6,842,702	B2	1/2005	Haaland et al.	7,332,784	B2	2/2008	Mills et al.
6,845,256	B2	1/2005	Chin et al.	7,340,287	B2	3/2008	Mason et al.
6,847,835	B1	1/2005	Yamanishi	7,341,559	B2	3/2008	Schulz et al.
6,850,787	B2	2/2005	Weber et al.	7,343,186	B2	3/2008	Lamego et al.
6,850,788	B2	2/2005	Al-Ali	D566,282	S	4/2008	Al-Ali et al.
6,852,083	B2	2/2005	Caro et al.	7,355,512	B1	4/2008	Al-Ali
6,861,639	B2	3/2005	Al-Ali	7,356,365	B2	4/2008	Schurman
6,861,641	B1	3/2005	Adams	7,371,981	B2	5/2008	Abdul-Hafiz
6,869,402	B2	3/2005	Arnold	7,373,193	B2	5/2008	Al-Ali et al.
6,882,874	B2	4/2005	Huiku	7,373,194	B2	5/2008	Weber et al.
6,898,452	B2	5/2005	Al-Ali et al.	7,376,453	B1	5/2008	Diab et al.
6,912,049	B2	6/2005	Pawluczyk et al.	7,377,794	B2	5/2008	Al-Ali et al.
6,917,422	B2	7/2005	Samsoundar et al.	7,377,899	B2	5/2008	Weber et al.
6,919,566	B1	7/2005	Cadell	7,383,070	B2	6/2008	Diab et al.
6,920,345	B2	7/2005	Al-Ali et al.	7,415,297	B2	8/2008	Al-Ali et al.
6,921,367	B2	7/2005	Mills	7,428,432	B2	9/2008	Ali et al.
6,922,645	B2	7/2005	Haaland et al.	7,438,683	B2	10/2008	Al-Ali et al.
6,928,311	B1	8/2005	Pawluczyk et al.	7,440,787	B2	10/2008	Diab
6,931,268	B1	8/2005	Kiani-Azarbayjany et al.	7,454,240	B2	11/2008	Diab et al.
6,931,269	B2	8/2005	Terry	7,457,652	B2	11/2008	Porges et al.
6,934,570	B2	8/2005	Kiani et al.	7,467,002	B2	12/2008	Weber et al.
6,939,305	B2	9/2005	Flaherty et al.	7,469,157	B2	12/2008	Diab et al.
6,943,348	B1	9/2005	Coffin, IV	7,471,969	B2	12/2008	Diab et al.
6,944,487	B2	9/2005	Maynard et al.	7,471,971	B2	12/2008	Diab et al.
6,950,687	B2	9/2005	Al-Ali	7,483,729	B2	1/2009	Al-Ali et al.
6,956,572	B2	10/2005	Zaleski	7,483,730	B2	1/2009	Diab et al.
6,961,598	B2	11/2005	Diab	7,489,958	B2	2/2009	Diab et al.
6,970,792	B1	11/2005	Diab	7,496,391	B2	2/2009	Diab et al.
6,975,891	B2	12/2005	Pawluczyk	7,496,393	B2	2/2009	Diab et al.
6,979,812	B2	12/2005	Al-Ali	D587,657	S	3/2009	Al-Ali et al.
6,985,764	B2	1/2006	Mason et al.	7,499,741	B2	3/2009	Diab et al.
6,987,994	B1	1/2006	Mortz	7,499,835	B2	3/2009	Weber et al.
6,993,371	B2	1/2006	Kiani et al.	7,500,950	B2	3/2009	Al-Ali et al.
6,996,427	B2	2/2006	Ali et al.	7,509,154	B2	3/2009	Diab et al.
6,999,904	B2	2/2006	Weber et al.	7,509,494	B2	3/2009	Al-Ali
7,001,337	B2	2/2006	Dekker	7,510,849	B2	3/2009	Schurman et al.
				7,526,328	B2	4/2009	Diab et al.
				7,530,942	B1	5/2009	Diab
				7,530,949	B2	5/2009	Al Ali et al.
				7,530,955	B2	5/2009	Diab et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

7,563,110	B2	7/2009	Al-Ali et al.	8,203,704	B2	6/2012	Merritt et al.
7,596,398	B2	9/2009	Al-Ali et al.	8,204,566	B2	6/2012	Schurman et al.
7,606,861	B2	10/2009	Killcommons et al.	8,219,172	B2	7/2012	Schurman et al.
7,618,375	B2	11/2009	Flaherty et al.	8,224,411	B2	7/2012	Al-Ali et al.
D606,659	S	12/2009	Kiani et al.	8,228,181	B2	7/2012	Al-Ali
7,647,083	B2	1/2010	Al-Ali et al.	8,229,532	B2	7/2012	Davis
D609,193	S	2/2010	Al-Ali et al.	8,229,533	B2	7/2012	Diab et al.
7,670,726	B2	3/2010	Lu	8,233,955	B2	7/2012	Al-Ali et al.
7,679,519	B2	3/2010	Lindner et al.	8,244,325	B2	8/2012	Al-Ali et al.
D614,305	S	4/2010	Al-Ali et al.	8,255,026	B1	8/2012	Al-Ali
RE41,317	E	5/2010	Parker	8,255,027	B2	8/2012	Al-Ali et al.
7,729,733	B2	6/2010	Al-Ali et al.	8,255,028	B2	8/2012	Al-Ali et al.
7,734,320	B2	6/2010	Al-Ali	8,260,577	B2	9/2012	Weber et al.
7,761,127	B2	7/2010	Al-Ali et al.	8,265,723	B1	9/2012	McHale et al.
7,761,128	B2	7/2010	Al-Ali et al.	8,274,360	B2	9/2012	Sampath et al.
7,764,982	B2	7/2010	Dalke et al.	8,301,217	B2	10/2012	Al-Ali et al.
D621,516	S	8/2010	Kiani et al.	8,306,596	B2	11/2012	Schurman et al.
7,791,155	B2	9/2010	Diab	8,310,336	B2	11/2012	Muhsin et al.
7,801,581	B2	9/2010	Diab	8,315,683	B2	11/2012	Al-Ali et al.
7,822,452	B2	10/2010	Schurman et al.	RE43,860	E	12/2012	Parker
RE41,912	E	11/2010	Parker	8,337,403	B2	12/2012	Al-Ali et al.
7,844,313	B2	11/2010	Kiani et al.	8,346,330	B2	1/2013	Lamego
7,844,314	B2	11/2010	Al-Ali	8,353,842	B2	1/2013	Al-Ali et al.
7,844,315	B2	11/2010	Al-Ali	8,355,766	B2	1/2013	MacNeish, III et al.
7,865,222	B2	1/2011	Weber et al.	8,359,080	B2	1/2013	Diab et al.
7,873,497	B2	1/2011	Weber et al.	8,364,223	B2	1/2013	Al-Ali et al.
7,880,606	B2	2/2011	Al-Ali	8,364,226	B2	1/2013	Diab et al.
7,880,626	B2	2/2011	Al-Ali et al.	8,374,665	B2	2/2013	Lamego
7,891,355	B2	2/2011	Al-Ali et al.	8,385,995	B2	2/2013	Al-Ali et al.
7,894,868	B2	2/2011	Al-Ali et al.	8,385,996	B2	2/2013	Dalke et al.
7,899,507	B2	3/2011	Al-Ali et al.	8,388,353	B2	3/2013	Kiani et al.
7,899,518	B2	3/2011	Trepagnier et al.	8,399,822	B2	3/2013	Al-Ali
7,904,132	B2	3/2011	Weber et al.	8,401,602	B2	3/2013	Kiani
7,909,772	B2	3/2011	Popov et al.	8,405,608	B2	3/2013	Al-Ali et al.
7,910,875	B2	3/2011	Al-Ali	8,414,499	B2	4/2013	Al-Ali et al.
7,919,713	B2	4/2011	Al-Ali et al.	8,418,524	B2	4/2013	Al-Ali
7,937,128	B2	5/2011	Al-Ali	8,423,106	B2	4/2013	Lamego et al.
7,937,129	B2	5/2011	Mason et al.	8,428,967	B2	4/2013	Olsen et al.
7,937,130	B2	5/2011	Diab et al.	8,430,817	B1	4/2013	Al-Ali et al.
7,941,199	B2	5/2011	Kiani	8,437,825	B2	5/2013	Dalvi et al.
7,951,086	B2	5/2011	Flaherty et al.	8,455,290	B2	6/2013	Siskavich
7,957,780	B2	6/2011	Lamego et al.	8,457,703	B2	6/2013	Al-Ali
7,962,188	B2	6/2011	Kiani et al.	8,457,707	B2	6/2013	Kiani
7,962,190	B1	6/2011	Diab et al.	8,463,349	B2	6/2013	Diab et al.
7,976,472	B2	7/2011	Kiani	8,466,286	B2	6/2013	Bellott et al.
7,988,637	B2	8/2011	Diab	8,471,713	B2	6/2013	Poeze et al.
7,990,382	B2	8/2011	Kiani	8,473,020	B2	6/2013	Kiani et al.
7,991,446	B2	8/2011	Al-Ali et al.	8,483,787	B2	7/2013	Al-Ali et al.
8,000,761	B2	8/2011	Al-Ali	8,489,364	B2	7/2013	Weber et al.
8,008,088	B2	8/2011	Bellott et al.	8,498,684	B2	7/2013	Weber et al.
RE42,753	E	9/2011	Kiani-Azarbayjany et al.	8,504,128	B2	8/2013	Blank et al.
8,019,400	B2	9/2011	Diab et al.	8,509,867	B2	8/2013	Workman et al.
8,028,701	B2	10/2011	Al-Ali et al.	8,515,509	B2	8/2013	Bruinsma et al.
8,029,765	B2	10/2011	Bellott et al.	8,523,781	B2	9/2013	Al-Ali
8,036,727	B2	10/2011	Schurman et al.	8,529,301	B2	9/2013	Al-Ali et al.
8,036,728	B2	10/2011	Diab et al.	8,532,727	B2	9/2013	Al-Ali et al.
8,046,040	B2	10/2011	Ali et al.	8,532,728	B2	9/2013	Diab et al.
8,046,041	B2	10/2011	Diab et al.	D692,145	S	10/2013	Al-Ali et al.
8,046,042	B2	10/2011	Diab et al.	8,547,209	B2	10/2013	Kiani et al.
8,048,040	B2	11/2011	Kiani	8,548,548	B2	10/2013	Al-Ali
8,050,728	B2	11/2011	Al-Ali et al.	8,548,549	B2	10/2013	Schurman et al.
RE43,169	E	2/2012	Parker	8,548,550	B2	10/2013	Al-Ali et al.
8,118,620	B2	2/2012	Al-Ali et al.	8,560,032	B2	10/2013	Al-Ali et al.
8,126,528	B2	2/2012	Diab et al.	8,560,034	B1	10/2013	Diab et al.
8,128,572	B2	3/2012	Diab et al.	8,570,167	B2	10/2013	Al-Ali
8,130,105	B2	3/2012	Al-Ali et al.	8,570,503	B2	10/2013	Vo et al.
8,145,287	B2	3/2012	Diab et al.	8,571,617	B2	10/2013	Reichgott et al.
8,150,487	B2	4/2012	Diab et al.	8,571,618	B1	10/2013	Lamego et al.
8,175,672	B2	5/2012	Parker	8,571,619	B2	10/2013	Al-Ali et al.
8,180,420	B2	5/2012	Diab et al.	8,577,431	B2	11/2013	Lamego et al.
8,182,443	B1	5/2012	Kiani	8,581,732	B2	11/2013	Al-Ali et al.
8,185,180	B2	5/2012	Diab et al.	8,584,345	B2	11/2013	Al-Ali et al.
8,190,223	B2	5/2012	Al-Ali et al.	8,588,880	B2	11/2013	Abdul-Hafiz et al.
8,190,227	B2	5/2012	Diab et al.	8,600,467	B2	12/2013	Al-Ali et al.
8,203,438	B2	6/2012	Kiani et al.	8,606,342	B2	12/2013	Diab
				8,626,255	B2	1/2014	Al-Ali et al.
				8,630,691	B2	1/2014	Lamego et al.
				8,634,889	B2	1/2014	Al-Ali et al.
				8,641,631	B2	2/2014	Sierra et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

8,652,060	B2	2/2014	Al-Ali	9,072,474	B2	7/2015	Al-Ali et al.
8,663,107	B2	3/2014	Kiani	9,078,560	B2	7/2015	Schurman et al.
8,666,468	B1	3/2014	Al-Ali	9,084,569	B2	7/2015	Weber et al.
8,667,967	B2	3/2014	Al-Ali et al.	9,095,316	B2	8/2015	Welch et al.
8,670,811	B2	3/2014	O'Reilly	9,106,038	B2	8/2015	Telfort et al.
8,670,814	B2	3/2014	Diab et al.	9,107,625	B2	8/2015	Telfort et al.
8,676,286	B2	3/2014	Weber et al.	9,107,626	B2	8/2015	Al-Ali et al.
8,682,407	B2	3/2014	Al-Ali	9,113,831	B2	8/2015	Al-Ali
RE44,823	E	4/2014	Parker	9,113,832	B2	8/2015	Al-Ali
RE44,875	E	4/2014	Kiani et al.	9,119,595	B2	9/2015	Lamego
8,690,799	B2	4/2014	Telfort et al.	9,131,881	B2	9/2015	Diab et al.
8,700,112	B2	4/2014	Kiani	9,131,882	B2	9/2015	Al-Ali et al.
8,702,627	B2	4/2014	Telfort et al.	9,131,883	B2	9/2015	Al-Ali
8,706,179	B2	4/2014	Parker	9,131,917	B2	9/2015	Telfort et al.
8,712,494	B1	4/2014	MacNeish, III et al.	9,138,180	B1	9/2015	Coverston et al.
8,715,206	B2	5/2014	Telfort et al.	9,138,182	B2	9/2015	Al-Ali et al.
8,718,735	B2	5/2014	Lamego et al.	9,138,192	B2	9/2015	Weber et al.
8,718,737	B2	5/2014	Diab et al.	9,142,117	B2	9/2015	Muhsin et al.
8,718,738	B2	5/2014	Blank et al.	9,153,112	B1	10/2015	Kiani et al.
8,720,249	B2	5/2014	Al-Ali	9,153,121	B2	10/2015	Kiani et al.
8,721,541	B2	5/2014	Al-Ali et al.	9,161,696	B2	10/2015	Al-Ali et al.
8,721,542	B2	5/2014	Al-Ali et al.	9,161,713	B2	10/2015	Al-Ali et al.
8,723,677	B1	5/2014	Kiani	9,167,995	B2	10/2015	Lamego et al.
8,740,792	B1	6/2014	Kiani et al.	9,176,141	B2	11/2015	Al-Ali et al.
8,754,776	B2	6/2014	Poeze et al.	9,186,102	B2	11/2015	Bruinsma et al.
8,755,535	B2	6/2014	Telfort et al.	9,192,312	B2	11/2015	Al-Ali
8,755,856	B2	6/2014	Diab et al.	9,192,329	B2	11/2015	Al-Ali
8,755,872	B1	6/2014	Marinow	9,192,351	B1	11/2015	Telfort et al.
8,761,850	B2	6/2014	Lamego	9,195,385	B2	11/2015	Al-Ali et al.
8,764,671	B2	7/2014	Kiani	9,211,072	B2	12/2015	Kiani
8,768,423	B2	7/2014	Shakespeare et al.	9,211,095	B1	12/2015	Al-Ali
8,771,204	B2	7/2014	Telfort et al.	9,218,454	B2	12/2015	Kiani et al.
8,777,634	B2	7/2014	Kiani et al.	9,226,696	B2	1/2016	Kiani
8,781,543	B2	7/2014	Diab et al.	9,241,662	B2	1/2016	Al-Ali et al.
8,781,544	B2	7/2014	Al-Ali et al.	9,245,668	B1	1/2016	Vo et al.
8,781,549	B2	7/2014	Al-Ali et al.	9,259,185	B2	2/2016	Abdul-Hafiz et al.
8,788,003	B2	7/2014	Schurman et al.	9,267,572	B2	2/2016	Barker et al.
8,790,268	B2	7/2014	Al-Ali	9,277,880	B2	3/2016	Poeze et al.
8,801,613	B2	8/2014	Al-Ali et al.	9,289,167	B2	3/2016	Diab et al.
8,821,397	B2	9/2014	Al-Ali et al.	9,295,421	B2	3/2016	Kiani et al.
8,821,415	B2	9/2014	Al-Ali et al.	9,307,928	B1	4/2016	Al-Ali et al.
8,830,449	B1	9/2014	Lamego et al.	9,323,894	B2	4/2016	Kiani
8,831,700	B2	9/2014	Schurman et al.	D755,392	S	5/2016	Hwang et al.
8,840,549	B2	9/2014	Al-Ali et al.	9,326,712	B1	5/2016	Kiani
8,847,740	B2	9/2014	Kiani et al.	9,333,316	B2	5/2016	Kiani
8,849,365	B2	9/2014	Smith et al.	9,339,220	B2	5/2016	Lamego et al.
8,852,094	B2	10/2014	Al-Ali et al.	9,341,565	B2	5/2016	Lamego et al.
8,852,994	B2	10/2014	Wojtczuk et al.	9,351,673	B2	5/2016	Diab et al.
8,868,147	B2	10/2014	Stippick et al.	9,351,675	B2	5/2016	Al-Ali et al.
8,868,150	B2	10/2014	Al-Ali et al.	9,364,181	B2	6/2016	Kiani et al.
8,870,792	B2	10/2014	Al-Ali et al.	9,368,671	B2	6/2016	Wojtczuk et al.
8,886,271	B2	11/2014	Kiani et al.	9,370,325	B2	6/2016	Al-Ali et al.
8,888,539	B2	11/2014	Al-Ali et al.	9,370,326	B2	6/2016	McHale et al.
8,888,708	B2	11/2014	Diab et al.	9,370,335	B2	6/2016	Al-Ali et al.
8,892,180	B2	11/2014	Weber et al.	9,375,185	B2	6/2016	Al-Ali et al.
8,897,847	B2	11/2014	Al-Ali	9,386,953	B2	7/2016	Al-Ali
8,909,310	B2	12/2014	Lamego et al.	9,386,961	B2	7/2016	Al-Ali et al.
8,911,377	B2	12/2014	Al-Ali	9,392,945	B2	7/2016	Al-Ali et al.
8,912,909	B2	12/2014	Al-Ali et al.	9,397,448	B2	7/2016	Al-Ali et al.
8,920,317	B2	12/2014	Al-Ali et al.	9,436,645	B2	9/2016	Al-Ali et al.
8,921,699	B2	12/2014	Al-Ali et al.	9,474,474	B2	10/2016	Lamego et al.
8,922,382	B2	12/2014	Al-Ali et al.	9,480,422	B2	11/2016	Al-Ali
8,929,964	B2	1/2015	Al-Ali et al.	9,480,435	B2	11/2016	Olsen
8,942,777	B2	1/2015	Diab et al.	9,517,024	B2	12/2016	Kiani et al.
8,948,834	B2	2/2015	Diab et al.	9,532,722	B2	1/2017	Lamego et al.
8,948,835	B2	2/2015	Diab	9,538,949	B2	1/2017	Al-Ali et al.
8,983,564	B2	3/2015	Al-Ali	9,538,980	B2	1/2017	Telfort et al.
8,989,831	B2	3/2015	Al-Ali et al.	9,549,696	B2	1/2017	Lamego et al.
8,996,085	B2	3/2015	Kiani et al.	9,554,737	B2	1/2017	Schurman et al.
8,998,809	B2	4/2015	Kiani	9,560,996	B2	2/2017	Kiani
9,028,429	B2	5/2015	Telfort et al.	9,579,039	B2	2/2017	Jansen et al.
9,037,207	B2	5/2015	Al-Ali et al.	2001/0044700	A1	11/2001	Kobayashi et al.
9,060,721	B2	6/2015	Reichgott et al.	2001/0045532	A1	11/2001	Schulz et al.
9,066,666	B2	6/2015	Kiani	2002/0021269	A1	2/2002	Rast
9,066,680	B1	6/2015	Al-Ali et al.	2002/0026107	A1	2/2002	Kiani et al.
				2002/0035315	A1	3/2002	Ali et al.
				2002/0035318	A1	3/2002	Mannheimer et al.
				2002/0038078	A1	3/2002	Ito
				2002/0038081	A1	3/2002	Fein et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

2002/0051290	A1	5/2002	Hannington	2005/0187452	A1	8/2005	Petersen et al.
2002/0059047	A1	5/2002	Haaland	2005/0187453	A1	8/2005	Petersen et al.
2002/0068858	A1	6/2002	Braig et al.	2005/0197549	A1	9/2005	Baker, Jr.
2002/0082488	A1	6/2002	Al-Ali et al.	2005/0197579	A1	9/2005	Baker, Jr.
2002/0095077	A1	7/2002	Swedlow et al.	2005/0197793	A1	9/2005	Baker, Jr.
2002/0095078	A1	7/2002	Mannheimer et al.	2005/0203357	A1	9/2005	Debreczeny et al.
2002/0111748	A1	8/2002	Kobayashi et al.	2005/0209515	A1	9/2005	Hockersmith et al.
2002/0115919	A1	8/2002	Al-Ali	2005/0228253	A1	10/2005	Debreczeny
2002/0154665	A1	10/2002	Funabashi et al.	2005/0250997	A1	11/2005	Takedo et al.
2002/0156353	A1	10/2002	Larson	2006/0030764	A1	2/2006	Porges et al.
2002/0159002	A1	10/2002	Chang	2006/0210120	A1	9/2006	Rowe et al.
2002/0161291	A1	10/2002	Kiani et al.	2006/0211922	A1	9/2006	Al-Ali et al.
2002/0165440	A1	11/2002	Mason et al.	2006/0211923	A1	9/2006	Al-Ali et al.
2002/0183819	A1	12/2002	Struble	2006/0211924	A1	9/2006	Smith et al.
2003/0045784	A1	3/2003	Palatnik et al.	2006/0211925	A1	9/2006	Lamego et al.
2003/0045785	A1	3/2003	Diab et al.	2006/0211932	A1	9/2006	Al-Ali et al.
2003/0049232	A1	3/2003	Page et al.	2006/0226992	A1	10/2006	Al-Ali et al.
2003/0109775	A1	6/2003	O'Neil et al.	2006/0229509	A1	10/2006	Al-Ali et al.
2003/0116769	A1	6/2003	Song et al.	2006/0238358	A1	10/2006	Al-Ali et al.
2003/0117296	A1	6/2003	Seely	2006/0241358	A1	10/2006	Al-Ali et al.
2003/0120160	A1	6/2003	Yarita	2006/0241363	A1	10/2006	Al-Ali et al.
2003/0120164	A1	6/2003	Nielsen et al.	2006/0264718	A1	11/2006	Ruchti et al.
2003/0135099	A1	7/2003	Al-Ali	2007/0078311	A1	4/2007	Al-Ali et al.
2003/0139657	A1	7/2003	Solenberger	2007/0149864	A1	6/2007	Laakkonen
2003/0160257	A1	8/2003	Bader et al.	2007/0185397	A1	8/2007	Govari et al.
2003/0195402	A1	10/2003	Fein et al.	2007/0282478	A1	12/2007	Al-Ali et al.
2004/0006261	A1	1/2004	Swedlow et al.	2009/0247984	A1	10/2009	Lamego et al.
2004/0033618	A1	2/2004	Haass et al.	2009/0275844	A1	11/2009	Al-Ali
2004/0034898	A1	2/2004	Bruegl	2010/0004518	A1	1/2010	Vo et al.
2004/0059209	A1	3/2004	Al Ali et al.	2010/0030040	A1	2/2010	Poeze et al.
2004/0064259	A1	4/2004	Haaland et al.	2011/0009719	A1	1/2011	Al-Ali et al.
2004/0081621	A1	4/2004	Arndt et al.	2011/0082711	A1	4/2011	Poeze et al.
2004/0092805	A1	5/2004	Yarita	2011/0105854	A1	5/2011	Kiani et al.
2004/0097797	A1	5/2004	Porges et al.	2011/0125060	A1	5/2011	Telfort et al.
2004/0133087	A1	7/2004	Al Ali et al.	2011/0208015	A1	8/2011	Welch et al.
2004/0138538	A1	7/2004	Stetson	2011/0213212	A1	9/2011	Al-Ali
2004/0138540	A1	7/2004	Baker, Jr. et al.	2011/0230733	A1	9/2011	Al-Ali
2004/0147822	A1	7/2004	Al-Ali et al.	2011/0237914	A1	9/2011	Lamego
2004/0147823	A1	7/2004	Kiani et al.	2011/0237969	A1	9/2011	Eckerbom et al.
2004/0158132	A1	8/2004	Zaleski	2011/0288383	A1	11/2011	Diab
2004/0158134	A1	8/2004	Diab et al.	2012/0041316	A1	2/2012	Al-Ali et al.
2004/0158135	A1	8/2004	Baker, Jr. et al.	2012/0046530	A1	2/2012	Al-Ali
2004/0158162	A1	8/2004	Narimatsu	2012/0046557	A1	2/2012	Kiani
2004/0162472	A1	8/2004	Berson et al.	2012/0059267	A1	3/2012	Lamego et al.
2004/0167382	A1	8/2004	Gardner et al.	2012/0088984	A1	4/2012	Al-Ali et al.
2004/0171940	A1	9/2004	Narimatsu	2012/0161970	A1	6/2012	Al-Ali
2004/0176670	A1	9/2004	Takamura et al.	2012/0165629	A1	6/2012	Merritt et al.
2004/0181134	A1	9/2004	Baker, Jr. et al.	2012/0179006	A1	7/2012	Jansen et al.
2004/0199063	A1	10/2004	O'Neil et al.	2012/0209082	A1	8/2012	Al-Ali
2004/0204639	A1	10/2004	Casciani et al.	2012/0209084	A1	8/2012	Olsen et al.
2004/0204868	A1	10/2004	Maynard et al.	2012/0232359	A1	9/2012	Al-Ali et al.
2004/0229391	A1	11/2004	Ohya et al.	2012/0232363	A1	9/2012	Al-Ali et al.
2004/0262046	A1	12/2004	Simon et al.	2012/0283524	A1	11/2012	Kiani et al.
2004/0267103	A1	12/2004	Li et al.	2012/0296178	A1	11/2012	Lamego et al.
2004/0267140	A1	12/2004	Ito et al.	2012/0319816	A1	12/2012	Al-Ali
2005/0011488	A1	1/2005	Doucet	2013/0023775	A1	1/2013	Lamego et al.
2005/0033128	A1	2/2005	Ali et al.	2013/0041591	A1	2/2013	Lamego
2005/0043902	A1	2/2005	Haaland et al.	2013/0046204	A1	2/2013	Lamego et al.
2005/0049469	A1	3/2005	Aoyagi et al.	2013/0060147	A1	3/2013	Welch et al.
2005/0054908	A1	3/2005	Blank et al.	2013/0096405	A1	4/2013	Garfio
2005/0070773	A1	3/2005	Chin et al.	2013/0096936	A1	4/2013	Sampath et al.
2005/0070775	A1	3/2005	Chin et al.	2013/0172701	A1	7/2013	Smith
2005/0075546	A1	4/2005	Samsoondar et al.	2013/0178749	A1	7/2013	Lamego
2005/0085704	A1	4/2005	Schulz et al.	2013/0243021	A1	9/2013	Siskavich
2005/0085735	A1	4/2005	Baker, Jr. et al.	2013/0253334	A1	9/2013	Al-Ali et al.
2005/0115561	A1	6/2005	Stahmann et al.	2013/0267804	A1	10/2013	Al-Ali
2005/0124871	A1	6/2005	Baker, Jr. et al.	2013/0274572	A1	10/2013	Al-Ali et al.
2005/0143634	A1	6/2005	Baker, Jr. et al.	2013/0296672	A1	11/2013	O'Neil et al.
2005/0143943	A1	6/2005	Brown	2013/0296713	A1	11/2013	Al-Ali et al.
2005/0148834	A1	7/2005	Hull et al.	2013/0317370	A1	11/2013	Dalvi et al.
2005/0184895	A1	8/2005	Petersen et al.	2013/0324808	A1	12/2013	Al-Ali et al.
2005/0187447	A1	8/2005	Chew et al.	2013/0331660	A1	12/2013	Al-Ali et al.
2005/0187448	A1	8/2005	Petersen et al.	2013/0331670	A1	12/2013	Kiani
2005/0187449	A1	8/2005	Chew et al.	2014/0012100	A1	1/2014	Al-Ali et al.
2005/0187450	A1	8/2005	Chew et al.	2014/0034353	A1	2/2014	Al-Ali et al.
				2014/0051953	A1	2/2014	Lamego et al.
				2014/0066783	A1	3/2014	Kiani et al.
				2014/0077956	A1	3/2014	Sampath et al.
				2014/0081100	A1	3/2014	Muhsin et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

2014/0081175 A1 3/2014 Telfort  
 2014/0100434 A1 4/2014 Diab et al.  
 2014/0114199 A1 4/2014 Lamego et al.  
 2014/0120564 A1 5/2014 Workman et al.  
 2014/0121482 A1 5/2014 Merritt et al.  
 2014/0127137 A1 5/2014 Bellott et al.  
 2014/0129702 A1 5/2014 Lamego et al.  
 2014/0135588 A1 5/2014 Al-Ali et al.  
 2014/0142401 A1 5/2014 Al-Ali et al.  
 2014/0142402 A1 5/2014 Al-Ali et al.  
 2014/0163344 A1 6/2014 Al-Ali  
 2014/0163402 A1 6/2014 Lamego et al.  
 2014/0166076 A1 6/2014 Kiani et al.  
 2014/0171763 A1 6/2014 Diab  
 2014/0180038 A1 6/2014 Kiani  
 2014/0180154 A1 6/2014 Sierra et al.  
 2014/0180160 A1 6/2014 Brown et al.  
 2014/0187973 A1 7/2014 Brown et al.  
 2014/0194709 A1 7/2014 Al-Ali et al.  
 2014/0266790 A1 9/2014 Al-Ali et al.  
 2014/0275808 A1 9/2014 Poeze et al.  
 2014/0275835 A1 9/2014 Lamego et al.  
 2014/0275871 A1 9/2014 Lamego et al.  
 2014/0275872 A1 9/2014 Merritt et al.  
 2014/0276115 A1 9/2014 Dalvi et al.  
 2014/0288400 A1 9/2014 Diab et al.  
 2014/0309506 A1 10/2014 Lamego  
 2014/0309559 A1 10/2014 Telfort et al.  
 2014/0316217 A1 10/2014 Purdon et al.  
 2014/0316218 A1 10/2014 Purdon et al.  
 2014/0316228 A1 10/2014 Blank et al.  
 2014/0323825 A1 10/2014 Al-Ali et al.  
 2014/0323897 A1 10/2014 Brown et al.  
 2014/0323898 A1 10/2014 Purdon et al.  
 2014/0330092 A1 11/2014 Al-Ali et al.  
 2014/0330098 A1 11/2014 Merritt et al.  
 2014/0330099 A1 11/2014 Al-Ali et al.  
 2014/0336481 A1 11/2014 Shakespeare et al.  
 2014/0357966 A1 12/2014 Al-Ali et al.  
 2015/0005600 A1 1/2015 Blank et al.  
 2015/0011907 A1 1/2015 Purdon et al.  
 2015/0012231 A1 1/2015 Poeze et al.  
 2015/0025406 A1 1/2015 Al-Ali  
 2015/0032029 A1 1/2015 Al-Ali et al.  
 2015/0038859 A1 2/2015 Dalvi et al.  
 2015/0045637 A1 2/2015 Dalvi  
 2015/0051462 A1 2/2015 Olsen  
 2015/0080754 A1 3/2015 Purdon et al.  
 2015/0087936 A1 3/2015 Al-Ali et al.  
 2015/0094546 A1 4/2015 Al-Ali  
 2015/0097701 A1 4/2015 Al-Ali et al.  
 2015/0099950 A1 4/2015 Al-Ali et al.  
 2015/0099951 A1 4/2015 Al-Ali et al.  
 2015/0099955 A1 4/2015 Al-Ali et al.  
 2015/0101844 A1 4/2015 Al-Ali et al.  
 2015/0106121 A1 4/2015 Muhsin et al.  
 2015/0112151 A1 4/2015 Muhsin et al.  
 2015/0116076 A1 4/2015 Al-Ali et al.  
 2015/0126830 A1 5/2015 Schurman et al.  
 2015/0133755 A1 5/2015 Smith et al.  
 2015/0141781 A1 5/2015 Weber et al.  
 2015/0165312 A1 6/2015 Kiani  
 2015/0196237 A1 7/2015 Lamego  
 2015/0201874 A1 7/2015 Diab  
 2015/0208966 A1 7/2015 Al-Ali  
 2015/0216459 A1 8/2015 Al-Ali et al.  
 2015/0230755 A1 8/2015 Al-Ali et al.  
 2015/0238722 A1 8/2015 Al-Ali  
 2015/0245773 A1 9/2015 Lamego et al.  
 2015/0245794 A1 9/2015 Al-Ali  
 2015/0257689 A1 9/2015 Al-Ali et al.  
 2015/0272514 A1 10/2015 Kiani et al.  
 2015/0351697 A1 12/2015 Weber et al.  
 2015/0351704 A1 12/2015 Kiani et al.  
 2015/0359429 A1 12/2015 Al-Ali et al.

2015/0366472 A1 12/2015 Kiani  
 2015/0366507 A1 12/2015 Blank  
 2015/0374298 A1 12/2015 Al-Ali et al.  
 2015/0380875 A1 12/2015 Coverston et al.  
 2016/0000362 A1 1/2016 Diab et al.  
 2016/0007930 A1 1/2016 Weber et al.  
 2016/0029932 A1 2/2016 Al-Ali  
 2016/0029933 A1 2/2016 Al-Ali et al.  
 2016/0045118 A1 2/2016 Kiani  
 2016/0051205 A1 2/2016 Al-Ali et al.  
 2016/0058338 A1 3/2016 Schurman et al.  
 2016/0058347 A1 3/2016 Reichgott et al.  
 2016/0066823 A1 3/2016 Al-Ali et al.  
 2016/0066824 A1 3/2016 Al-Ali et al.  
 2016/0066879 A1 3/2016 Telfort et al.  
 2016/0072429 A1 3/2016 Kiani et al.  
 2016/0081552 A1 3/2016 Wojtczuk et al.  
 2016/0095543 A1 4/2016 Telfort et al.  
 2016/0095548 A1 4/2016 Al-Ali et al.  
 2016/0103598 A1 4/2016 Al-Ali et al.  
 2016/0113527 A1 4/2016 Al-Ali et al.  
 2016/0143548 A1 5/2016 Al-Ali  
 2016/0166182 A1 6/2016 Al-Ali  
 2016/0296169 A1 10/2016 McHale et al.  
 2016/0310052 A1 10/2016 Al-Ali

## FOREIGN PATENT DOCUMENTS

EP 41 92 23 3/1991  
 EP 0 569 670 2/1993  
 EP 0 675 540 10/1995  
 EP 0 675 541 10/1995  
 EP 0469395 B1 2/1996  
 EP 0417447 B1 10/1997  
 EP 0606356 B1 6/1998  
 EP 0734221 B1 7/1998  
 EP 0 529 412 11/1998  
 EP 1 080 683 3/2001  
 EP 1 207 536 5/2002  
 EP 1 860 989 12/2007  
 EP 1 860 990 12/2007  
 EP 1 860 994 12/2007  
 EP 1 860 995 12/2007  
 EP 1 860 996 12/2007  
 EP 1 860 997 12/2007  
 EP 1 863 380 12/2007  
 EP 1 895 892 5/2010  
 EP 2 286 721 2/2011  
 EP 2 305 104 4/2011  
 EP 2 476 369 7/2012  
 EP 2 139 383 2/2013  
 EP 2 476 369 10/2014  
 JP 61-28172 2/1986  
 JP 62-000324 1/1987  
 JP 63-275327 11/1988  
 JP 64-500495 2/1989  
 JP 2-126829 5/1990  
 JP 2-145457 12/1990  
 JP 05-200017 8/1993  
 JP 05-207993 8/1993  
 JP H06-178776 6/1994  
 JP 6-505903 7/1994  
 JP 6-237013 8/1994  
 JP H07-391 1/1995  
 JP H07-171089 7/1995  
 JP H07-171090 7/1995  
 JP 7-281618 10/1995  
 JP 07-325546 12/1995  
 JP 09-108203 4/1997  
 JP 9-192120 7/1997  
 JP 09-308623 12/1997  
 JP 10-500026 1/1998  
 JP H10-500026 1/1998  
 JP 10-216112 8/1998  
 JP 10-509352 9/1998  
 JP 10-269344 A 10/1998  
 JP 10-295676 11/1998  
 JP 10-305026 11/1998  
 JP 11-037932 2/1999

(56)

## References Cited

## FOREIGN PATENT DOCUMENTS

JP	11-163412	6/1999
JP	11-164826	6/1999
JP	11-506834	6/1999
JP	11-183377	7/1999
JP	H11-508691	7/1999
JP	2000-116625	4/2000
JP	2002-516689	6/2002
JP	2002-228579	8/2002
JP	2002-525151	8/2002
JP	2002-315739	10/2002
JP	2003-507718	2/2003
JP	2003-084108	3/2003
JP	2003-521985	7/2003
JP	2004-070179	3/2004
JP	2004-510467	4/2004
JP	2004-173866	6/2004
JP	2004-226277	8/2004
JP	2004-296736	10/2004
JP	2004-532526	10/2004
JP	2004-327760	11/2004
JP	2005-501589	1/2005
JP	2005-253478	9/2005
JP	2008-505706	2/2008
JP	4865737	11/2011
JP	4879913	12/2011
JP	2012-110746	6/2012
JP	2012-130756	7/2012
JP	5096174	9/2012
JP	5166619	3/2013
JP	5456976	1/2014
WO	WO 88/01150	2/1988
WO	WO 88/002020	2/1988
WO	WO 92/16142	10/1992
WO	WO 93/06776	4/1993
WO	WO 95/16387	6/1995
WO	WO 96/013208	5/1996
WO	WO 96/41138	12/1996
WO	WO 97/01985	1/1997
WO	WO 97/29678	8/1997
WO	WO 97/029710	8/1997
WO	WO 98/43071	10/1998
WO	WO 00/18290	4/2000
WO	WO 00/42911	7/2000
WO	WO 00/59374	10/2000
WO	WO 01/13790	3/2001
WO	WO 01/30414	5/2001
WO	WO 01/058347	8/2001
WO	WO 02/017780	3/2002
WO	WO 02/026123	4/2002
WO	WO 02/089664	11/2002
WO	WO 03/020129	3/2003
WO	WO 03/068060	8/2003
WO	WO 03/077761	9/2003
WO	WO 04/034898	4/2004
WO	WO 04/038801	5/2004
WO	WO 05/004712	1/2005
WO	WO 05/011488	2/2005
WO	WO 06/017117	2/2006
WO	WO 06/094107	9/2006
WO	WO 06/094108	9/2006
WO	WO 06/094155	9/2006
WO	WO 06/094168	9/2006
WO	WO 06/094169	9/2006
WO	WO 06/094170	9/2006
WO	WO 06/094171	9/2006
WO	WO 06/094279	9/2006
WO	WO 06/115580	11/2006
WO	WO 09/013835	1/2009
WO	WO 09/137524	11/2009

## OTHER PUBLICATIONS

U.S. Appl. No. 14/472,760, filed Aug. 29, 2014, Smith et al.  
U.S. Appl. No. 14/557,761, filed Dec. 2, 2014, Al-Ali et al.

Burritt, Mary F.; Current Analytical Approaches to Measuring Blood Analytes; vol. 36; No. 8(B); 1990.

European Examination Report dated Apr. 1, 2010, re EP App. No. 08 744 412.1-2319.

European Examination Report dated Mar. 18, 2011, re EP App. No. 08 744 412.1-2319.

European Examination Report dated Sep. 2, 2010, re EP App. No. 08 744 412.1-2319.

European Examination Report, re EP Application No. 12163719.3, dated Feb. 6, 2013.

European Extended Search Report EPO App. No. 10162402.1, SR dated Aug. 9, 2010.

European Extended Search Report, re EP Application No. 12163719.3, dated Jun. 18, 2012.

European Office Action re EP Application No. 06 736 799.5, dated Nov. 30, 2012.

European Search Report, re EP Application No. 10 19 1029, dated Jun. 5, 2012.

Hall, et al., Jeffrey W.; Near-Infrared Spectrophotometry: A New Dimension in Clinical Chemistry; vol. 38; No. 9; 1992.

International Preliminary Report on Patentability for PCT/US2010/058981 dated Jun. 5, 2012, dated Jun. 14, 2012.

International Search Report for PCT/US2006/007516, dated Jan. 11, 2007, in 4 pages.

Japanese Office Action (Notice of Reasons for Rejection) re JP App. No. 2007-558246, dated Jun. 28, 2011.

Japanese Office Action (Official Inquiry) re JP App. No. 2007-558246, dated Dec. 11, 2012.

Japanese Office Action (Reasons for Rejection) re JP App. No. 2007-558246, dated Nov. 1, 2011.

Japanese Office Action, re JP Application No. 2012-045419, dated Jun. 26, 2012.

Japanese Office Action re JP Application No. JP 2007-558208, dated Aug. 23, 2011.

Japanese First Office Action (Notice of Reasons for Rejection), re JP App. No. 2007-558247, dated Jun. 28, 2011.

Japanese Office Action (Notice of Allowance), re JP App. No. 2007-558247, dated Oct. 24, 2011.

Japanese Office Action (Decision of Rejection), re JP Application No. JP 2007-558328, dated Jun. 25, 2013.

Japanese Office Action (Notice of Reasons for Rejection), re JP App. No. 2007-558238, dated Jun. 28, 2011.

Japanese Office Action (Official Inquiry), re JP App. No. 2007-558238/Appeal No. 2012-004053, dated Dec. 11, 2012.

Japanese Office Action re JP Application No. JP 2007-558248, dated Nov. 27, 2012.

Japanese Office Action re JP Application No. JP 2007-558248, dated Nov. 8, 2011.

Japanese First Office Action (Notice of Reasons for Rejection), re JP App. No. 2007-558207, dated Jun. 28, 2011.

Japanese Office Action, re JP Application No. 2007-558237, dated Aug. 1, 2011.

Japanese Office Action, re JP Application No. JP 2007-558237, dated Oct. 16, 2012.

Japanese Office Action re JP Application No. 2007-558209, dated Oct. 25, 2011.

Japanese Office Action re JP Application No. 2007-558209, dated Oct. 30, 2012.

Japanese Office Action re JP Application No. 2007-558245, dated Oct. 25, 2011.

Japanese Office Action re JP Application No. 2007-558245, dated Jan. 15, 2013.

Japanese Office Action re JP Application No. 2007-558245, dated Oct. 29, 2013.

Japanese Final Office Action re Amendments re JP Application No. 2007-558249, dated Apr. 17, 2012.

Japanese Office Action re JP Application No. 2007-558249, dated Aug. 28, 2012.

Japanese Office Action re JP Application No. 2007-558249, dated Jul. 13, 2011.

Japanese Office Action re JP Application No. 2007-558249, dated Nov. 8, 2011.

(56)

**References Cited**

## OTHER PUBLICATIONS

- Kuenstner, et al., J. Todd; Measurement of Hemoglobin in Unlysed Blood by Near-Infrared Spectroscopy; vol. 48; No. 4, 1994.
- Manzke, et al., B., Multi Wavelength Pulse OXimetry in the Measurement of Hemoglobin Fractions; vol. 2676, date unknown.
- Naumenko, E. K.; Choice of Wavelengths for Stable Determination of Concentrations of Hemoglobin Derivatives from Absorption Spectra of Erythrocytes; vol. 63; No. 1; pp. 60-66 Jan.-Feb. 1996; Original article submitted Nov. 3, 1994.
- PCT International Search Report; PCT/US 2006/007389; dated Jul. 17, 2006; pp. 1-9.
- PCT International Search Report; PCT/US2006/007387; dated Jul. 17, 2006; pp. 1-9.
- PCT International Search Report; PCT/US2006/007388; dated Jul. 17, 2006; pp. 1-9.
- PCT International Search Report; PCT/US2006/007506; dated Jul. 17, 2006; pp. 1-10.
- PCT International Search Report; PCT/US2006/007536; dated Jul. 17, 2006; pp. 1-9.
- PCT International Search Report; PCT/US2006/007537; dated Jul. 17, 2006; pp. 1-10.
- PCT International Search Report; PCT/US2006/007538; dated Jul. 17, 2006; pp. 1-9.
- PCT International Search Report; PCT/US2006/007539; dated Jul. 17, 2006; pp. 1-9.
- PCT International Search Report; PCT/US2006/007540; dated Jul. 17, 2006; pp. 1-9.
- PCT International Search Report; PCT/US2006/007958; dated Jul. 17, 2006; pp. 1-8.
- PCT Search Report of International Application No. PCT/US2008/058327, dated Aug. 12, 2008, in 12 pages.
- Schmitt, Joseph M.; Simple Photon Diffusion Analysis of the Effects of Multiple Scattering on Pulse Oximetry; Mar. 14, 1991; revised Aug. 30, 1991.
- Schmitt, Joseph M.; Zhou, Guan-Xiong; Miller, Justin, Measurement of Blood Hematocrit by Dual-wavelength Near-IR Photoplethysmography, published May 1992, Proc. SPIE vol. 1641, p. 150-161, Physiological Monitoring and Early Detection Diagnostic Methods, Thomas S. Mang; Ed. (SPIE homepage), in 12 pages.
- Schnapp, et al., L.M.; Pulse Oximetry. Uses and Abuses.; Chest 1990; 98; 1244-1250001 10.1378/Chest.98.5.1244.
- European Extended Search Report, re EP Application No. 10 18 1436, completion date Nov. 26, 2010.
- European Examination Report, re EP Application No. 06736799.5, dated Nov. 30, 2012.
- European Examination Report, re EP Application No. 06736799.5, dated Oct. 28, 2014.
- Japanese (Office Action) Notice of Reasons for Rejection, re App. No. 2000-606119, dated Nov. 4, 2009.
- PCT Report on Patentability of International Application No. PCT/US2008/058327, dated Jun. 30, 2009, in 12 pages.
- "Medical." 50 Ways to Touch Memory. 3rd ed. Dallas: Dallas Semiconductor Corporation, Aug. 1994; pp. 24-25. Print.
- "Application Note 84 Use of Add-Only Memory for Secure Storage of Monetary Equivalent Data," Dallas Semiconductor, Jun. 22, 1999, in 5 pages.
- Dallas Semiconductor Corp: DS2430A Announcement, retrieved Jun. 10, 1998, in 2 pages. <[https://web.archive.org/web/19980610045525/http://dalsemi.com/News\\_Center/New\\_Products/1996/2430a.html](https://web.archive.org/web/19980610045525/http://dalsemi.com/News_Center/New_Products/1996/2430a.html)>.
- Favennec, J.M. "Smart sensors in industry." J. Phys. E: Sci. Instrum. 20(9): Sep. 1987, pp. 1087-1090.
- Jones, K.L., et al. "A Protocol for Automatic Sensor Detection and Identification in a Wireless Biodevice Network," IEEE, Jun. 1998, 6 pages.
- Subramanian, S., et al. "Design for Constraint Violation Detection in Safety-Critical Systems," IEEE, Nov. 1998: pp. 1-8.

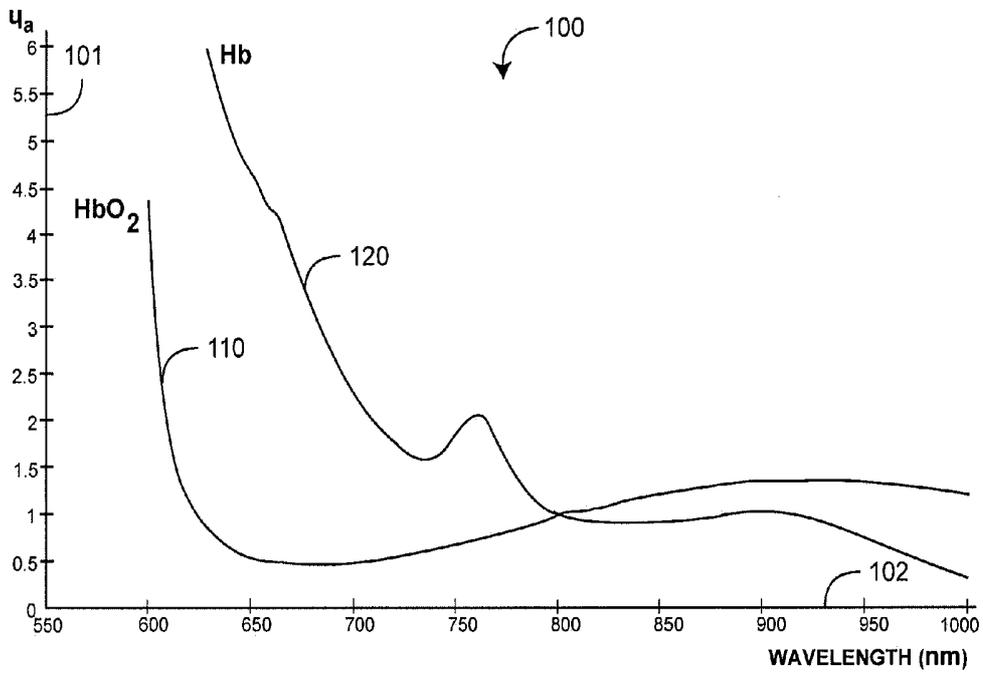


FIG. 1

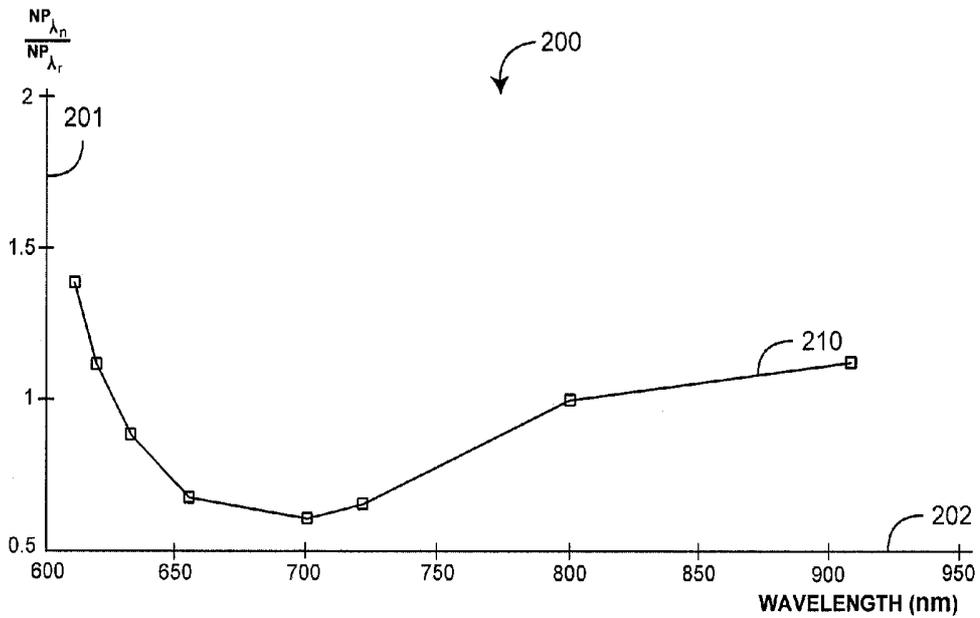


FIG. 2

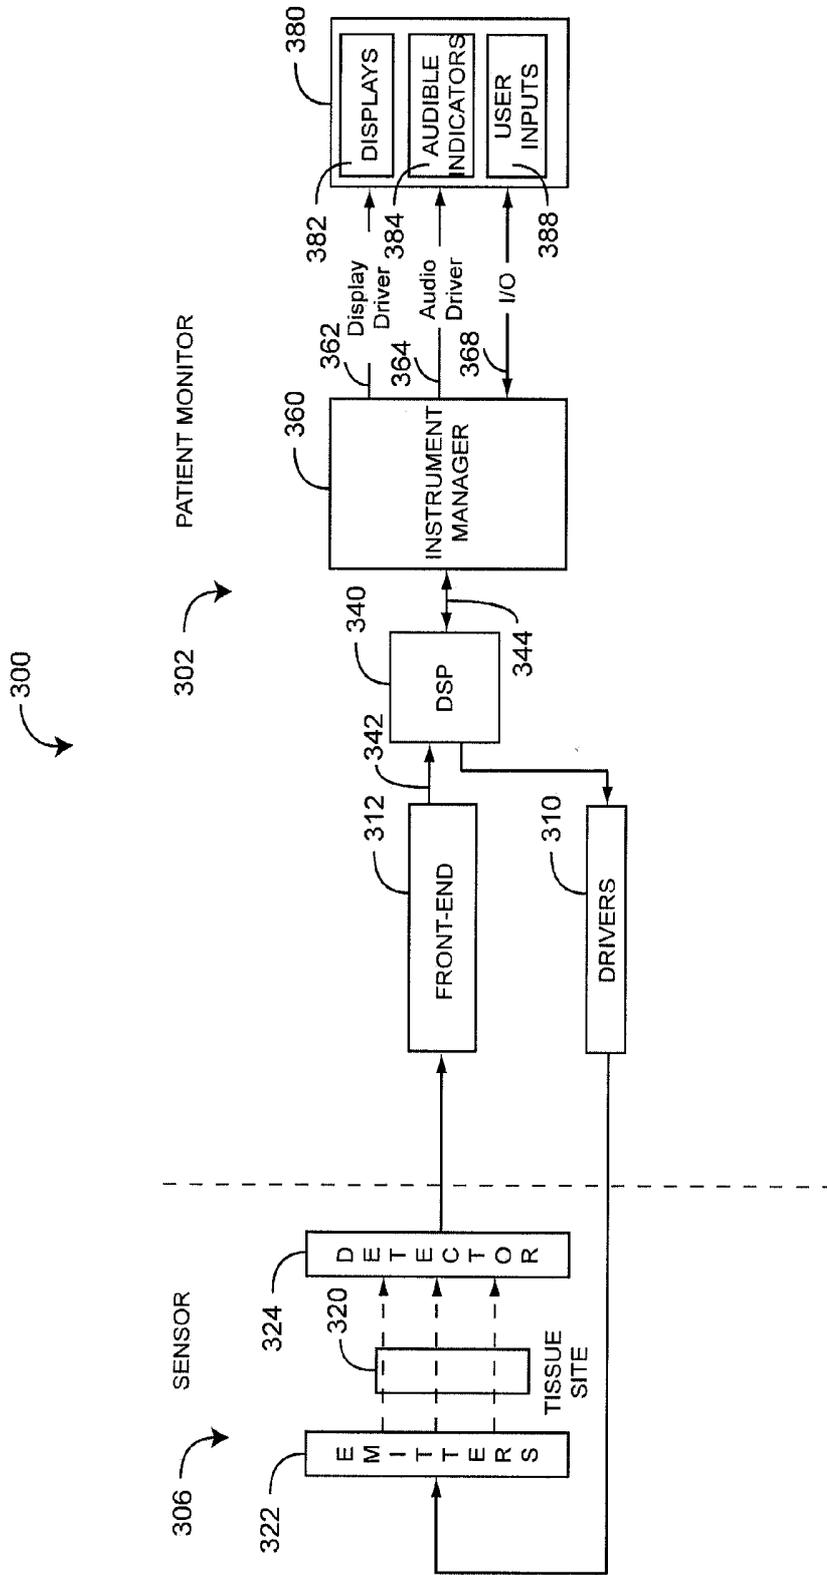


FIG. 3

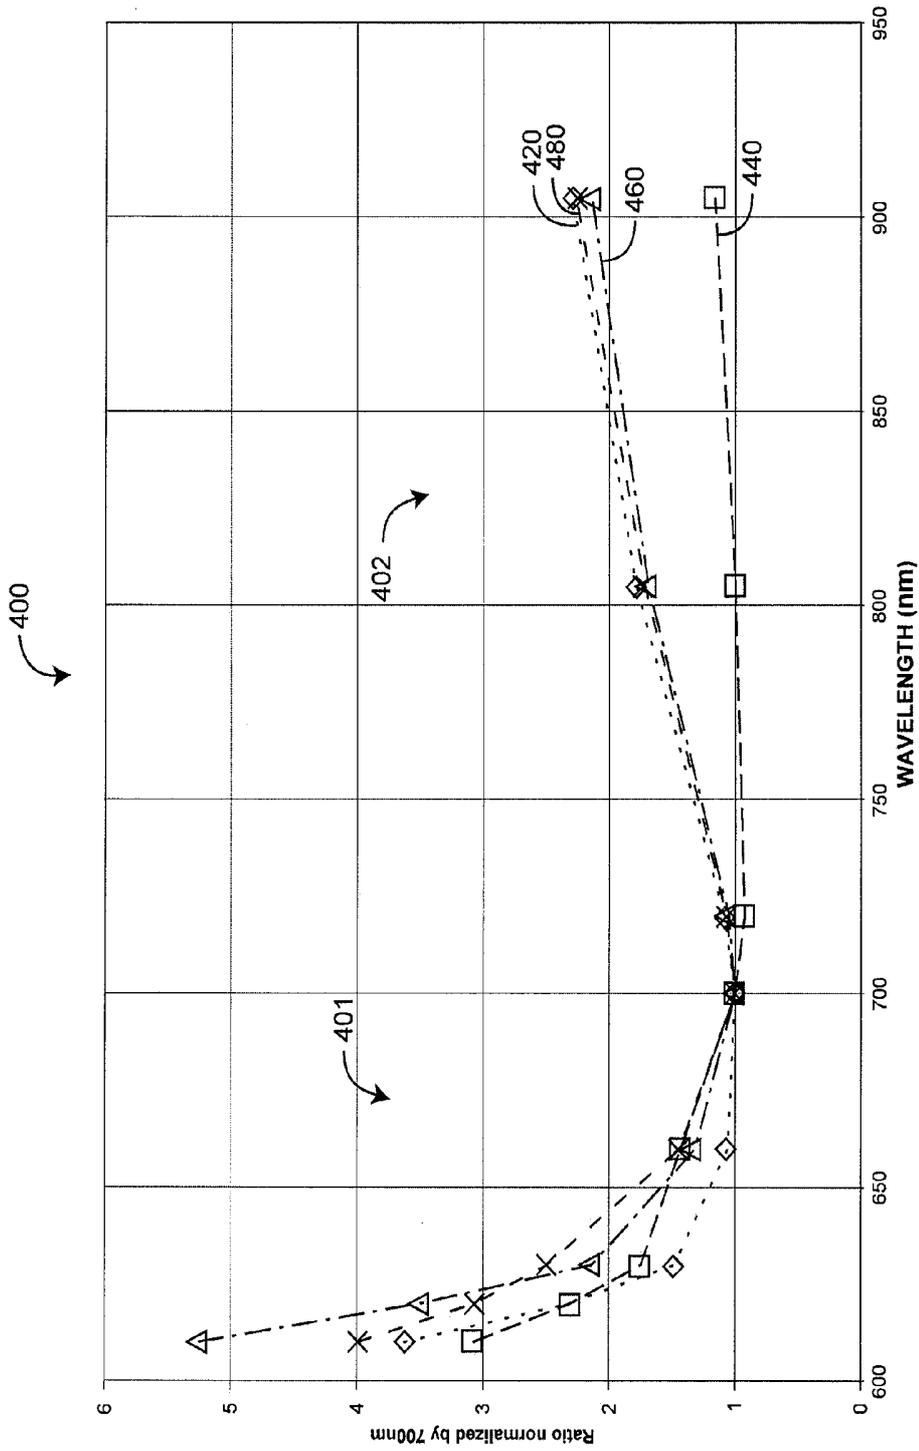


FIG. 4

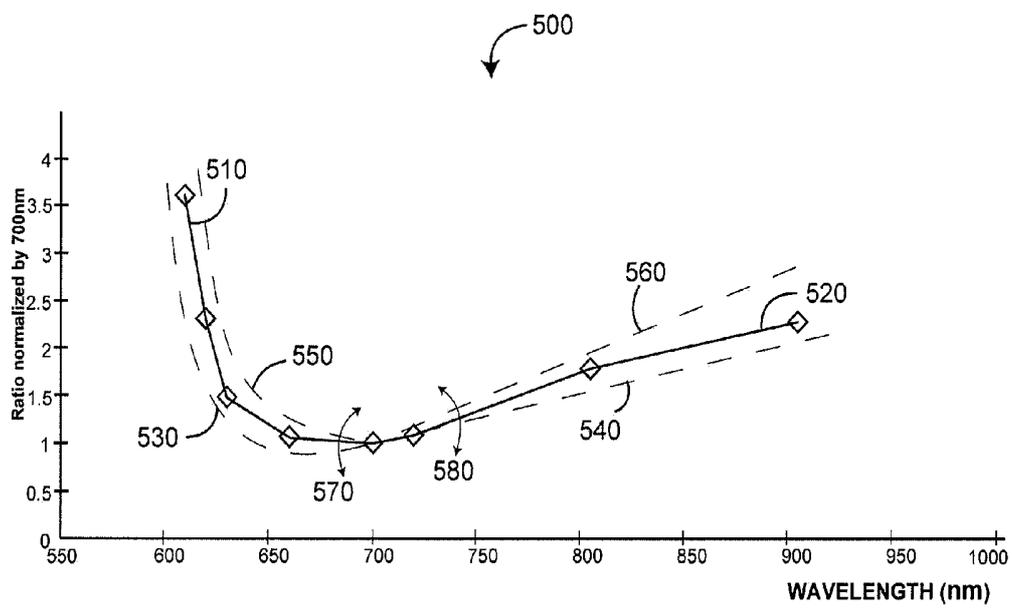


FIG. 5

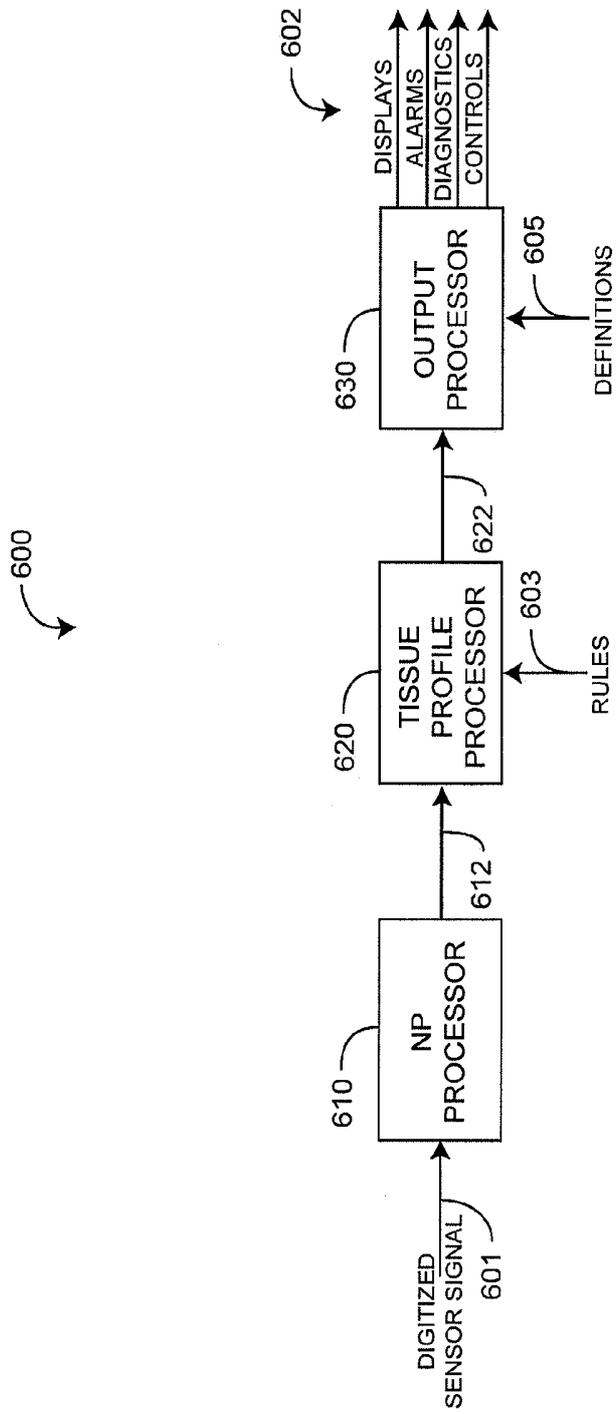


FIG. 6

## TISSUE PROFILE WELLNESS MONITOR

## CROSS-REFERENCE TO RELATED APPLICATIONS

The present application is a continuation of U.S. patent application Ser. No. 13/764,007, filed Feb. 11, 2013, entitled "TISSUE PROFILE WELLNESS MONITOR," which is a continuation of U.S. patent application Ser. No. 12/106,969, filed Apr. 21, 2008, entitled "TISSUE PROFILE WELLNESS MONITOR," which claims priority benefit under 35 U.S.C. §119(e) to U.S. Provisional Application Ser. No. 60/925,811, filed Apr. 21, 2007, entitled "TISSUE PROFILE WELLNESS MONITOR." All of the above referenced applications are hereby incorporated by reference in their entirety herein.

## BACKGROUND OF THE INVENTION

Spectroscopy is a common technique for measuring the concentration of organic and some inorganic constituents of a solution. The theoretical basis of this technique is the Beer-Lambert law, which states that the concentration  $c_i$  of an absorbent in solution can be determined by the intensity of light transmitted through the solution, knowing the path length  $d_\lambda$ , the intensity of the incident light  $I_{0,\lambda}$ , and the extinction coefficient  $\epsilon_{i,\lambda}$  at a particular wavelength  $\lambda$ . In generalized form, the Beer-Lambert law is expressed as:

$$I_\lambda = I_{0,\lambda} e^{-d_\lambda \mu_{a,\lambda}} \quad (1)$$

$$\mu_{a,\lambda} = \sum_{i=1}^n \epsilon_{i,\lambda} \cdot c_i \quad (2)$$

Where  $\mu_{a,\lambda}$  is the bulk absorption coefficient and represents the probability of absorption per unit length. The minimum number of discrete wavelengths that are required to solve EQS. 1-2 are the number of significant absorbers that are present in the solution.

A practical application of this technique is pulse oximetry, which utilizes a noninvasive sensor to measure oxygen saturation ( $SpO_2$ ) and pulse rate. The sensor has light emitting diodes (LEDs) that transmit optical radiation of red and infrared wavelengths into a tissue site and a detector that responds to the intensity of the optical radiation after attenuation by pulsatile arterial blood flowing within the tissue site. Based on this response, a processor determines measurements for  $SpO_2$  and pulse rate, and outputs representative plethysmographic waveforms. Thus, "pulse oximetry" as used herein encompasses its broad ordinary meaning known to one of skill in the art, which includes at least those noninvasive procedures for measuring parameters of circulating blood through spectroscopy. Moreover, "plethysmograph" as used herein encompasses its broad ordinary meaning known to one of skill in the art, which includes at least data representative of a change in the absorption of particular wavelengths of light as a function of the changes in body tissue resulting from pulsing blood.

Pulse oximeters capable of reading through motion induced noise are available from Masimo Corporation ("Masimo") of Irvine, Calif. Moreover, portable and other oximeters capable of reading through motion induced noise are disclosed in at least U.S. Pat. Nos. 6,770,028, 6,658,276, 6,584,336, 6,263,222, 6,157,850, 5,769,785, and 5,632,272, which are owned by Masimo, and are incorporated by

reference herein. Such reading through motion oximeters have gained rapid acceptance in a wide variety of medical applications, including surgical wards, intensive care and neonatal units, general wards, home care, physical training, and virtually all type of monitoring scenarios.

FIG. 1 illustrates an absorption graph **100** having a dimensionless vertical axis **101** of relative light absorption and a horizontal axis **102** of transmitted wavelength in nm. Shown is a plot of  $HbO_2$  absorption **110** and Hb absorption **120** versus wavelength, both normalized to the absorption at 800 nm. At red and near IR wavelengths below 970 nm, where water has a significant peak, Hb and  $HbO_2$  are the only significant absorbers normally present in the blood. Thus, typically only two wavelengths are needed to resolve the concentrations of Hb and  $HbO_2$ , e.g. a red (RD) wavelength at 660 nm and an infrared (IR) wavelength at 940 nm. In particular,  $SpO_2$  is computed based upon a red ratio  $Red_{AC}/Red_{DC}$  and an IR ratio  $IR_{AC}/IR_{DC}$ , which are the AC detector response magnitude at a particular wavelength normalized by the DC detector response at that wavelength. The normalization by the DC detector response reduces measurement sensitivity to variations in tissue thickness, emitter intensity and detector sensitivity, for example. The AC detector response is a plethysmograph, as described above. Thus, the red and IR ratios can be denoted as  $NP_{RD}$  and  $NP_{IR}$  respectively, where NP stands for "normalized plethysmograph." In pulse oximetry, oxygen saturation is calculated from the ratio  $NP_{RD}/NP_{IR}$ .

## SUMMARY OF THE INVENTION

Oxygen saturation is a very useful physiological parameter for indicating the cardiovascular status of a patient, but allows healthcare providers only a few minutes warning that a patient is potentially having a medical crisis. A wellness indicator advantageously monitors changes in a patient's "tissue profile" so as to provide an advance warning of a deteriorating medical condition. This tissue profile is provided by a multiple wavelength sensor and a noninvasive multi-parameter patient monitor, which make blood absorption measurements at more than a red wavelength and an IR wavelength of conventional pulse oximetry. In one embodiment, described below, blood absorption measurements are made at eight wavelengths. Advantageously, this rich wavelength data characterizes a tissue site over a wavelength spectrum.

FIG. 2 illustrates an example of a tissue profile. In this example, the sensor emits eight wavelengths (610, 620, 630, 655, 700, 720, 800 and 905 nm). A tissue profile graph **200** has a NP ratio axis **201** and a wavelength axis **202**, where the NP ratios are of the form  $NP_{\lambda_1}/NP_{\lambda_2}$ . This is a generalization to multiple wavelengths of the ratio  $NP_{RD}/NP_{IR}$  described above for two (red and IR) wavelengths. In order to provide a common scale for these NP ratios, the ratios are calculated with respect to a reference wavelength,  $\lambda_r$ , which may be any of the available wavelengths. Thus, the plotted NP ratios **210** are denoted  $NP_{\lambda_r}/NP_{\lambda_r}$ . Note that the NP ratio at the reference wavelength is  $NP_{\lambda_r}/NP_{\lambda_r}=1$ , which is 700 nm in this example. In this example, a tissue profile **210** is plotted for  $SpO_2=97\%$ .

Not surprisingly, the tissue profile **210** has the same general shape as the absorption curves **110**, **120** of FIG. 1. In particular, the AC component of the detector signal relative to the DC component (NP) for a specific wavelength is proportional to the light absorption at that wavelength. Thus, the NP ratio magnitudes and hence the points along a tissue profile curve are proportional to absorption. Assuming

negligible abnormal Hb species, if SpO<sub>2</sub> is close to 100%, most of the absorption is due to HbO<sub>2</sub> and, accordingly, the tissue profile is shaped closely to the HbO<sub>2</sub> absorption curve. As SpO<sub>2</sub> decreases from 100%, the tissue profile shape is increasing influenced by the shape of the Hb absorption curve.

In one embodiment, the tissue profile **210** consists solely of the measured NP ratios at the sensor wavelengths, i.e. a finite set of discrete values. In another embodiment, the tissue profile **210** consists of the measured NP ratios and defined NP ratio values between the sensor wavelengths, which are based upon tissue absorption characteristics. That is, the tissue profile **210** is a curve defined over a continuous range of wavelengths, including the sensor wavelengths. Although described above with respect to NP ratios derived from the AC component of the detector signal, a DC tissue profile may also be defined and applied to patient monitoring, as described below.

A tissue profile or tissue characterization is described in U.S. patent application Ser. No. 11/367,034, filed Mar. 1, 2006 entitled Physiological Parameter Confidence Measure; a multiple wavelength sensor is disclosed in U.S. patent application Ser. No. 11/367,013, filed Mar. 1, 2006 entitled Multiple Wavelength Sensor Emitters; and a multi-parameter patient monitor is disclosed in U.S. patent application Ser. No. 11/367,033, filed Mar. 1, 2006 entitled Noninvasive Multi-Parameter Patient Monitor, all of the aforementioned applications are assigned to Masimo Laboratories, Inc., Irvine, Calif. and all are incorporated by reference herein.

One aspect of a tissue profile wellness monitor comprises generating a tissue profile, predetermining rules and applying the rules to the tissue profile. The tissue profile is responsive to absorption of emitted wavelengths of optical radiation by pulsatile blood flowing within a tissue site. The rules are used to evaluate at least a portion of the tissue profile. A patient condition is indicated according to the applied rules.

Another aspect of a tissue profile wellness monitor comprises measuring a normalized plethysmograph (NP) to generate a tissue profile, testing the tissue profile and outputting the test results. The NP is measured at each of multiple wavelengths of optical radiation, and the NP is responsive to attenuation of the optical radiation by constituents of pulsatile blood flowing within a tissue site illuminated by the optical radiation. The tissue profile is tested against predetermined rules. The test results are output as at least one of a display, alarm, diagnostic and control.

A further aspect of a tissue profile wellness monitor comprises measuring a physiological parameter, generating a tissue profile, defining limits and indicating when the tissue profile exceeds the defined limits. The physiological parameter is responsive to multiple wavelengths of optical radiation after attenuation by constituents of pulsatile blood flowing within a tissue site. The tissue profile is responsive to the physiological parameter. The limits are defined for at least a portion of the tissue profile.

#### BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a graph of oxyhemoglobin and reduced hemoglobin light absorption versus wavelength across portions of the red and IR spectrum;

FIG. 2 is a graph of normalized plethysmograph (NP) ratios versus wavelength illustrating a tissue profile for 97% oxygen saturation;

FIG. 3 is a general block diagram of a patient monitoring system embodiment that implements a tissue profile wellness monitor;

FIG. 4 is a graph of tissue profiles for high saturation, low saturation, high carboxyhemoglobin (HbCO) and high methemoglobin (MetHb);

FIG. 5 is a graph illustrating tissue profile changes indicative of patient wellness; and

FIG. 6 is a block diagram of a tissue profile wellness monitor embodiment.

#### DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

FIG. 3 illustrates a patient monitoring system **300**, which generates NP ratios and blood parameter measurements, such as SpO<sub>2</sub>, HbCO and HbMet, accordingly. The patient monitoring system is advantageously adapted as a tissue profile wellness monitor, as described below. The patient monitoring system **300** has a patient monitor **302** and a sensor **306**. The sensor **306** attaches to a tissue site **320** and includes a plurality of emitters **322** capable of irradiating the tissue site **320** with differing wavelengths of light, perhaps including the red and infrared wavelengths utilized in pulse oximeters. The sensor **306** also includes one or more detectors **324** capable of detecting the light after attenuation by the tissue site **320**. A multiple wavelength sensor is disclosed in U.S. application Ser. No. 11,367,013, filed on Mar. 1, 2006, titled Multiple Wavelength Sensor Emitters, cited above. Multiple wavelength sensors, such as Rainbow™-brand adhesive and reusable sensors are available from Masimo Corporation, Irvine, Calif.

As shown in FIG. 3, the patient monitor **302** communicates with the sensor **306** to receive one or more intensity signals indicative of one or more physiological parameters. Drivers **310** convert digital control signals into analog drive signals capable of driving the sensor emitters **322**. A front-end **312** converts composite analog intensity signal(s) from light sensitive detector(s) **324** into digital data **342** input to the DSP **340**. The DSP **340** may comprise a wide variety of data and/or signal processors capable of executing programs for determining physiological parameters from input data. In an embodiment, the DSP **340** executes the processors **610**, **620**, **630** (FIG. 6), described below.

The instrument manager **360** may comprise one or more microcontrollers providing system management, such as monitoring the activity of the DSP **340**. The instrument manager **360** also has an input/output (I/O) port **368** that provides a user and/or device interface for communicating with the monitor **302**. In an embodiment, the I/O port **368** provides threshold settings via a user keypad, network, computer or similar device, as described below.

Also shown in FIG. 3 are one or more user I/O devices **380** including displays **382**, audible indicators **384** and user inputs **388**. The displays **382** are capable of displaying indicia representative of calculated physiological parameters such as one or more of a pulse rate (PR), plethysmograph (pleth), perfusion index (PI), signal quality and values of blood constituents in body tissue, including for example, oxygen saturation (SpO<sub>2</sub>), carboxyhemoglobin (HbCO) and methemoglobin (HbMet). The monitor **302** may also be capable of storing or displaying historical or trending data related to one or more of the measured parameters or combinations of the measured parameters. The monitor **302** may also provide a trigger for the audible indicators **384**, which operate beeps, tones and alarms, for example. Displays **382** include for example readouts, colored lights or

graphics generated by LEDs, LCDs or CRTs to name a few. Audible indicators 384 include speakers or other audio transducers. User input devices 388 may include, for example, keypads, touch screens, pointing devices, voice recognition devices, or the like.

FIG. 4 illustrates tissue profile curves 400, which are responsive to Hb constituents. In this example, the sensor emits eight wavelengths (610, 620, 630, 660, 700, 720, 805, 905 nm), which are normalized at 700 nm. Shown is a high saturation profile curve 420, e.g. SpO2≈100% (◇); a low saturation profile curve 440, e.g. SpO2=70% (□); a high HbCO profile curve 460, e.g. HbCO=30% (Δ); and a high HbMet profile curve 480, e.g. HbMet=6% (X). The profile curves 420-480 each has a head portion 401 at wavelengths less than 700 nm and a corresponding tail portion 402 at wavelengths of greater than 700 nm. As shown in FIG. 4, a tissue profile head portion 401 has higher values when HbCO (Δ) or HbMet (X) has a higher percentage value. The head portion 401 has lower values when HbCO or HbMet has a lower percentage value. Also, both the head portion 401 and the tail portion 402 have higher values when SpO2 is a high percentage (◇) and lower values when SpO2 is a low percentage (□).

FIG. 5 illustrates an example tissue profile 500 utilized as a wellness indicator. As described with respect to FIG. 4 above, the position or shape of the tissue profile or changes in the position or shape of the tissue profile provide an indication of patient wellness. In particular, position, shape or relative movements of the curve “head” 510 or the curve “tail” 520 or both indicate potentially detrimental values or changes in values of hemoglobin constituents. For example, a drop in the tissue profile head 510 or tail 520 below a predefined boundary 530, 540 may indicate reduced oxygen saturation. As another example, a rise in the tissue profile head 510 above a predefined boundary 550 may indicate increased concentrations of abnormal hemoglobin species, such as carboxyhemoglobin (HbCO) and methemoglobin (HbMet). Further, relative movements 570, 580 of the tissue profile 500 faster than a predefined rate may indicate potentially serious trends in the concentrations of normal or abnormal hemoglobin species.

FIG. 6 illustrates a tissue profile wellness monitor 600 having a NP processor 610, a tissue profile processor 620 and an output processor 630. In an embodiment, these processors 610-630 execute in the DSP 340 (FIG. 3) to monitor tissue profile changes. The NP processor 610 has digitized sensor signal input 601 from one or more sensor channels, such as described with respect to FIG. 3, above, and generates normalized plethysmograph (NP) calculations 612 as described with respect to FIG. 1, above.

As shown in FIG. 6, the tissue profile processor 620 is configured to compare tissue profile changes 612 with respect to predetermined rules 603 and communicate the test results 622 to the output processor 630. As an example, the tissue profile processor 620 may communicate to the output processor 630 when a tissue profile portion changes faster than a predetermined rate.

Also shown in FIG. 6, the output processor 630 inputs the tissue profile processor results 622 and generates outputs 602 based upon predetermined output definitions 605. For example, if a test profile result is “true”, it might trigger an audible alarm. Rules and corresponding outputs are described in further detail with respect to TABLE 1, below.

In an embodiment, the tissue profile wellness monitor 600 provides outputs 602 according to TABLE 1, below. The terms listed in TABLE 1 are described with respect to FIG. 6, above. Various other indicators, alarms, controls and

diagnostics in response to various combinations of rules and output definitions can be substituted for, or added to, the rule-based outputs illustrated in TABLE 1.

In an embodiment, the tissue profile wellness monitor 600 grades a patient with respect to wellness utilizing green, yellow and red indicators. For example, a green panel light signals that the tissue profile is indicative of normal blood hemoglobin. A yellow panel light signals that changes in the tissue profile shape or position are indicative of potentially problematic changes in blood hemoglobin. A red panel light signals that the tissue profile is indicative of blood hemoglobin outside of normal ranges.

TABLE 1

Tissue Profile Rules and Outputs	
TISSUE PROFILE RULES	OUTPUTS
If all portions of tissue profile are within boundaries and relatively unchanging over time	Then illuminate green indicator.
If tail drops faster than tail trend limit; or head rises faster than head trend limit	Then illuminate yellow indicator
If tail or head are outside of boundaries	Then illuminate red indicator

A tissue profile wellness monitor has been disclosed in detail in connection with various embodiments. These embodiments are disclosed by way of examples only and are not to limit the scope of the claims that follow. One of ordinary skill in art will appreciate many variations and modifications.

What is claimed is:

1. A patient monitor comprising:

a front-end interface configured to receive, from a sensor comprising a light source that emits light into a tissue site of a patient and a detector that detects a plurality of wavelengths of the emitted light after attenuation by the tissue site, a signal indicative of the detected light at each of the plurality of wavelengths; and

a processor configured to: determine, at each of the plurality of wavelengths and based on the signal, normalized plethysmographs (NPs);

normalize each of the determined NPs based on a reference wavelength;

determine a tissue profile curve based on the normalized NPs at the plurality of wavelengths;

analyze a shape of the tissue profile curve relative to a predefined boundary curve to determine patient wellness; and

output an indication in response to determining the shape of the tissue profile curve exceeds the predefined boundary curve.

2. The patient monitor of claim 1, wherein the indication comprises at least one of a display, an alarm, a diagnostic, or a control.

3. The patient monitor of claim 1, wherein determining the tissue profile curve comprises:

measuring, from the signal, values indicative of an amount of light attenuation for at least some of the plurality wavelengths;

defining, based on characteristics of the tissue site, additional values corresponding to at least a portion of a wavelength spectrum between the respective wavelengths associated with the at least some of the plurality of wavelengths; and

7

combining the measured values at each of the at least some of the plurality of wavelengths with the additional values.

4. The patient monitor of claim 1, wherein the processor is further configured to:

output a first signal indicative of patient normalcy when the tissue profile curve is within the predefined boundary curve and a rate of change of the tissue profile curve is less than a maximum rate of change; and

output a second signal indicative of alert when at least a portion of the tissue profile curve is outside of the predefined boundary curve and the rate of change of the tissue profile curve is greater than the maximum rate of change.

5. The patient monitor of claim 1, wherein the tissue profile curve is indicative of at least one of oxygen saturation of the patient, carboxyhemoglobin of the patient, or methemoglobin of the patient.

6. The patient monitor of claim 1, wherein the tissue profile curve comprises a first portion and a second portion, and wherein the first portion is analyzed in comparison to a first portion predefined boundary curve, and the second portion is analyzed in comparison to a second portion predefined boundary curve.

7. The patient monitor of claim 6, wherein the processor is further configured to:

provide a first indication in response to the first and second portions not exceeding the respective first and second portion predefined boundary curves;

provide a second indication in response to one of the first or second portions exceeding the respective first or second portion predefined boundary curves; and

provide a third indication in response to both of the first and second portions exceeding the respective first and second portion predefined boundary curves.

8. The patient monitor of claim 1, wherein the reference wavelength is one of the plurality of wavelengths.

9. A patient monitor comprising:

a front-end interface configured to receive, from a sensor comprising a light source that emits light into a tissue site of a patient and a detector that detects a plurality of wavelengths of the emitted light after attenuation by the tissue site, a signal indicative of the detected light at each of the plurality of wavelengths; and

a processor configured to:

determine, at each of the plurality of wavelengths and based on the signal, normalized plethysmographs (NPs);

normalize each of the determined NPs based on a reference wavelength;

8

determine a tissue profile curve indicative of a relationship among the normalized NPs at the plurality of wavelengths;

evaluate a trend in movement of the tissue profile curve relative to a predetermined trend limit to determine patient wellness; and

output an indication in response to determining the trend in movement of the tissue profile curve exceeds the predetermined trend limit.

10. The patient monitor of claim 9, wherein the trend in movement of the tissue profile curve exceeding the predetermined trend limit indicates advance warning of deteriorating patient wellness.

11. The patient monitor of claim 9, wherein the reference wavelength divides the tissue profile curve into a first portion and a second portion, and wherein the first portion is evaluated in relation to a first portion predetermined trend limit, and the second portion is evaluated in relation to a second portion predetermined trend limit.

12. The patient monitor of claim 11, wherein the processor is further configured to:

provide a first indication in response to the first and second portions not exceeding the respective first and second portion predetermined trend limits;

provide a second indication in response to one of the first or second portions exceeding the respective first or second portion predetermined trend limits; and

provide a third indication in response to both of the first and second portions exceeding the respective first and second portion predetermined trend limits.

13. The patient monitor of claim 9, wherein the reference wavelength is one of the plurality of wavelengths.

14. The patient monitor of claim 9, wherein determining the tissue profile curve indicative of the relationship among the normalized NPs at the plurality of wavelengths comprises:

defining continuous normalized NP values corresponding to at least a portion of a wavelength spectrum between the two or more of the at least some of the plurality of wavelengths based at least in part on characteristics of the tissue site; and

combining the normalized NP values at each of the at least some of the plurality of wavelengths with the defined continuous normalized NP values.

15. The patient monitor of claim 9, wherein the tissue profile curve is indicative of at least one of oxygen saturation of the patient, carboxyhemoglobin of the patient, or methemoglobin of the patient.

\* \* \* \* \*

专利名称(译)	组织配置文件健康监视器		
公开(公告)号	<a href="#">US9848807</a>	公开(公告)日	2017-12-26
申请号	US14/599342	申请日	2015-01-16
[标]申请(专利权)人(译)	CERCACOR LAB		
申请(专利权)人(译)	CERCACOR LABORATORIES , INC.		
当前申请(专利权)人(译)	Masimo公司		
[标]发明人	LAMEGO MARCELO M		
发明人	LAMEGO, MARCELO M.		
IPC分类号	A61B5/1455 A61B5/024 A61B5/0295 A61B5/00		
CPC分类号	A61B5/14551 A61B5/0295 A61B5/02416 A61B5/72 A61B5/7475 A61B5/742 A61B5/7405 A61B5/746 A61B5/7275		
优先权	12/106969 2013-02-13 US 60/925811 2007-04-21 US		
其他公开文献	US20150196237A1		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

摘要(译)

组织轮廓健康监测器测量生理参数，生成组织轮廓，定义限制并指示组织轮廓何时超过限定的界限。在由组织部位内流动的脉动血液的成分衰减之后，生理参数响应于多个波长的光学辐射。组织轮廓响应于生理参数。限制是针对组织轮廓的至少一部分定义的。

