



US008764675B2

(12) **United States Patent**
Palti

(10) **Patent No.:** **US 8,764,675 B2**
(45) **Date of Patent:** **Jul. 1, 2014**

- (54) **COMPOSITE ELECTRODE**
- (71) Applicant: **Novocure LTD**, St. Helier (JE)
- (72) Inventor: **Yoram Palti**, Haifa (IL)
- (73) Assignee: **Novocure Ltd**, St. Helier (JE)
- (*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

- (21) Appl. No.: **13/790,258**
- (22) Filed: **Mar. 8, 2013**

- (65) **Prior Publication Data**
US 2013/0190847 A1 Jul. 25, 2013

- Related U.S. Application Data**
- (63) Continuation of application No. 11/856,277, filed on Sep. 17, 2007.

- (51) **Int. Cl.**
A61B 5/103 (2006.01)
A61B 5/00 (2006.01)
- (52) **U.S. Cl.**
CPC *A61B 5/441* (2013.01); *A61B 5/411* (2013.01)


- USPC **600/549**; 600/556
- (58) **Field of Classification Search**
USPC 600/395, 549
See application file for complete search history.

- (56) **References Cited**
U.S. PATENT DOCUMENTS
4,809,707 A * 3/1989 Kraft et al. 600/549
2003/0029569 A1* 2/2003 Natsuhara et al. 156/345.51
* cited by examiner

Primary Examiner — Carl H Layno
Assistant Examiner — Jon Eric C Morales
 (74) *Attorney, Agent, or Firm* — Proskauer

- (57) **ABSTRACT**
An electrode for applying electric fields to a patient includes a plurality of ceramic elements (e.g., ceramic discs) that are designed to be positioned against the patient's skin. Electrical connections are made to the ceramic elements (e.g., using a flex circuit). Temperature sensors (e.g., thermistors) are preferably provided at at least some of the ceramic elements to sense the temperature at the skin beneath the ceramic elements, so that appropriate action can be taken if an overtemperature condition is detected.

27 Claims, 5 Drawing Sheets

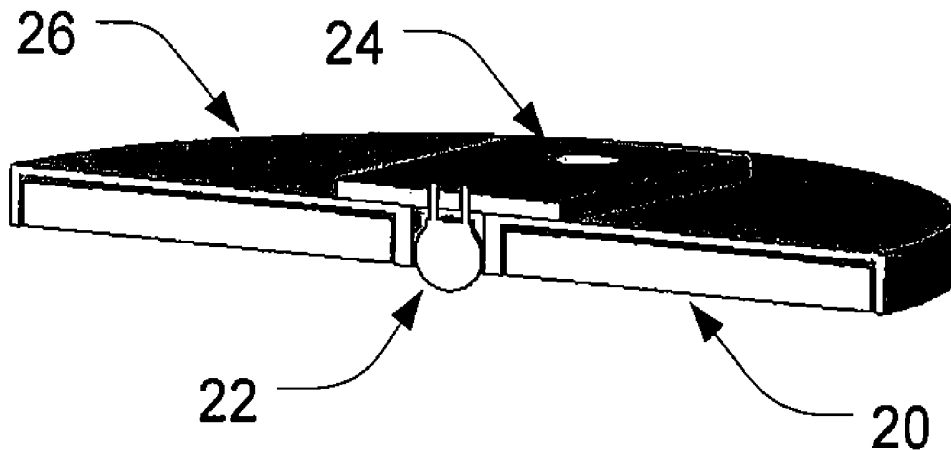

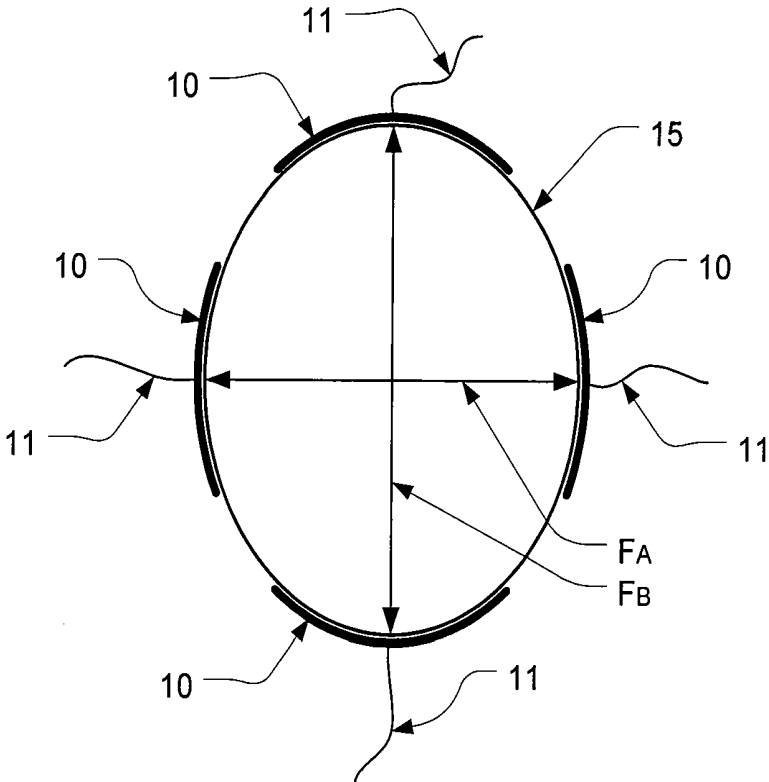


FIG. 1

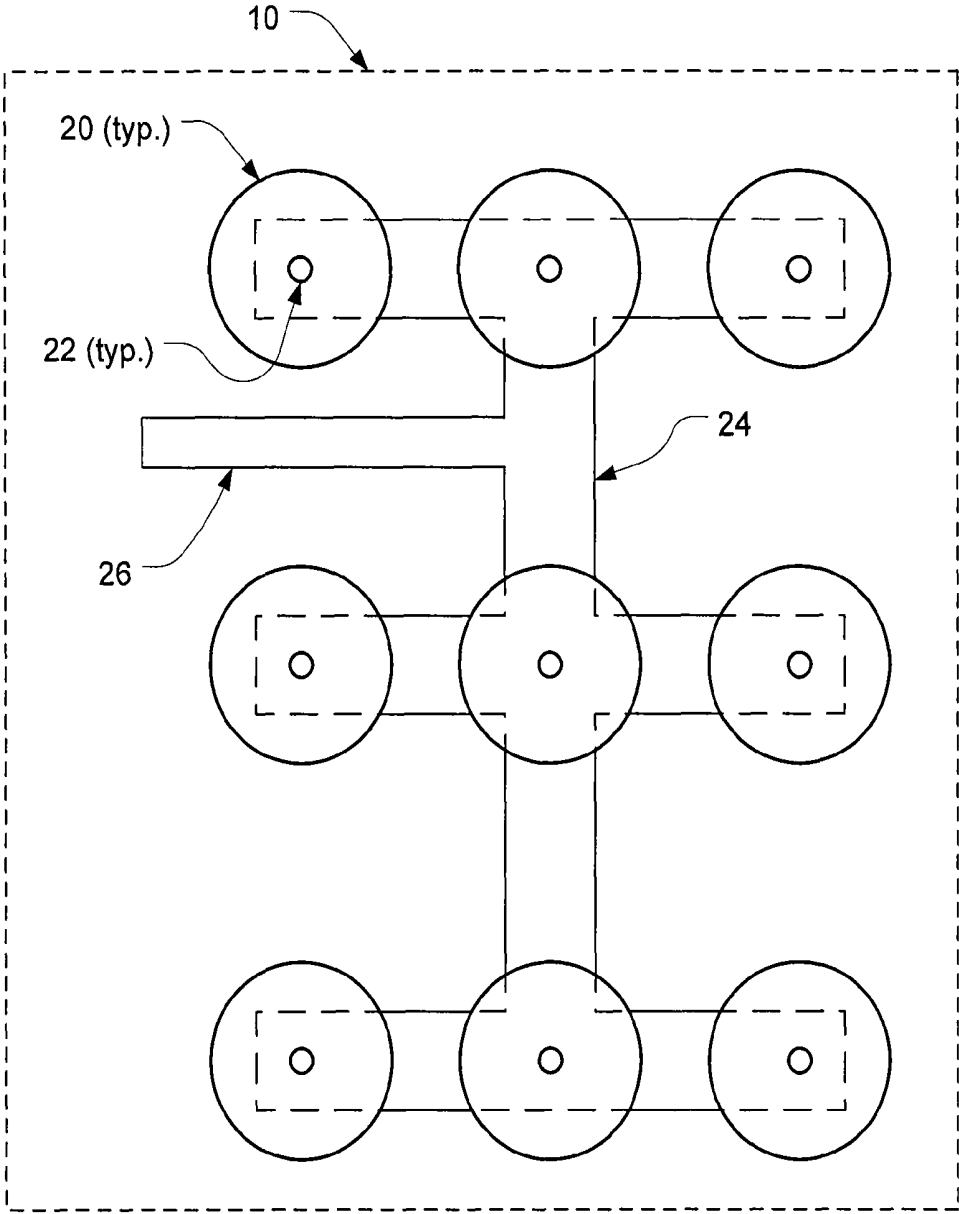


FIG. 2

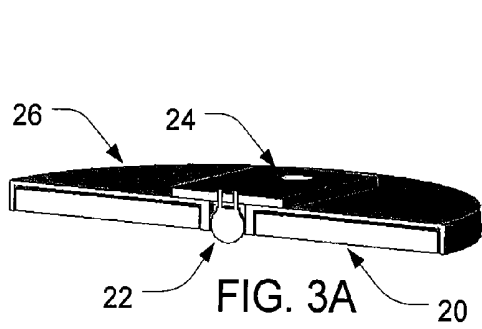


FIG. 3A

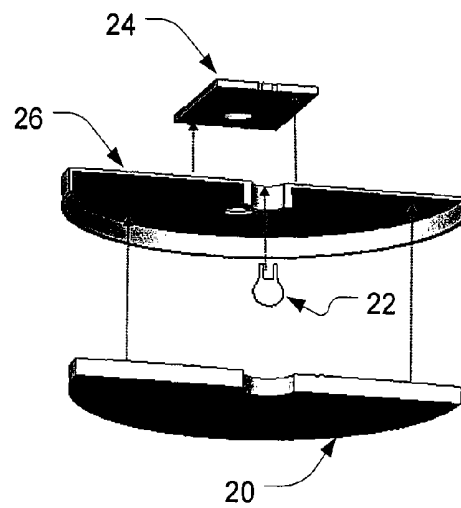


FIG. 3B

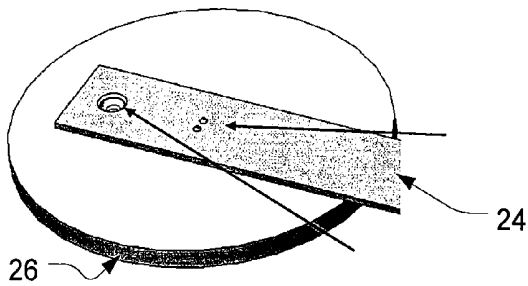


FIG. 3C

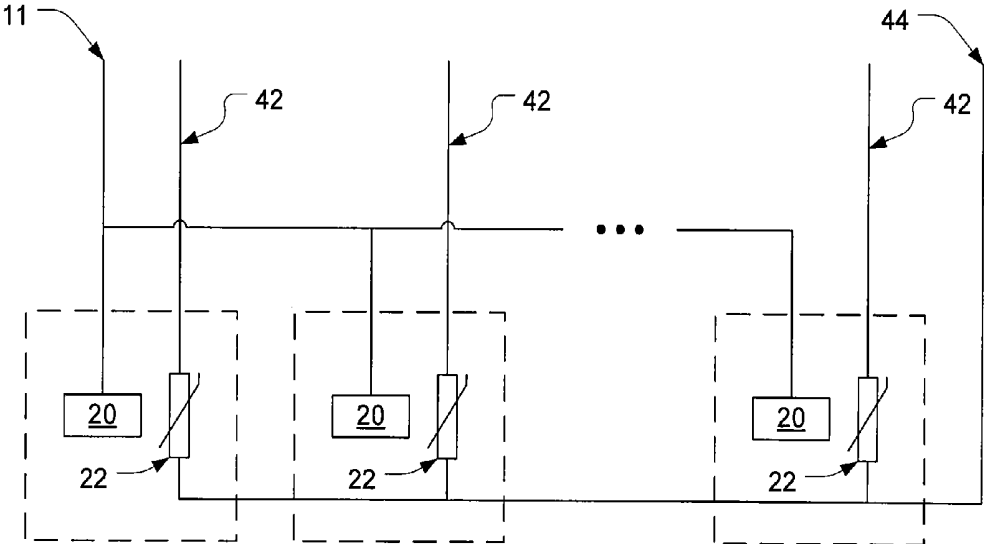


FIG. 4

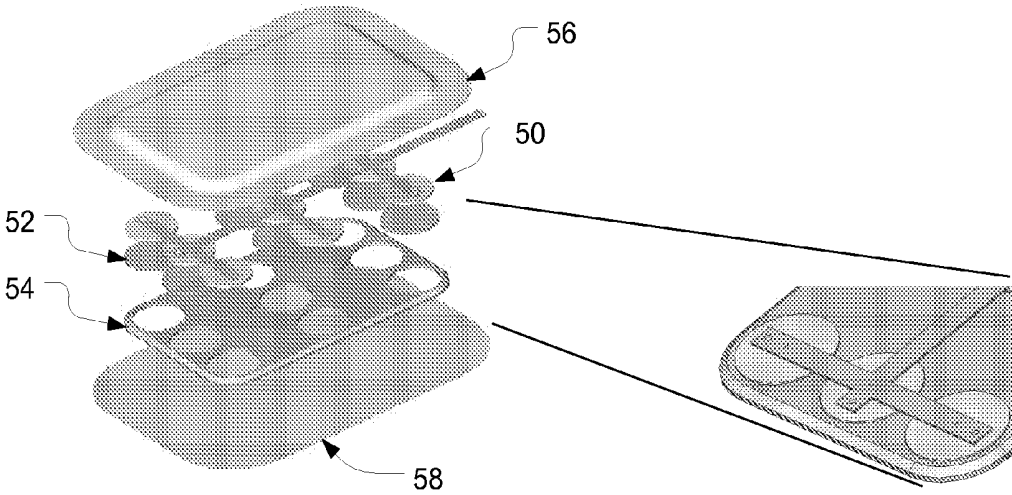


FIG. 5

COMPOSITE ELECTRODE

CROSS REFERENCE TO RELATED APPLICATIONS

This Application is a continuation of U.S. application Ser. No. 11/856,277, filed Sep. 17, 2007, which is incorporated herein by reference.

BACKGROUND

U.S. Pat. Nos. 7,136,699 and 7,146,210, each of which is incorporated herein by reference, describe treating tumors or other rapidly dividing cells with AC electric fields at particular frequencies and field strengths. This application relates to an improved electrode that is particularly well-suited for applying those electric fields.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 shows a set of electrodes being used to apply electric fields to a subject.

FIG. 2 is a mechanical schematic diagram of an electrode in accordance with a first embodiment of the invention.

FIG. 3A is a cross section view of a subsection of the electrode shown in FIG. 2.

FIG. 3B is an exploded cross section view of the same subsection of the electrode.

FIG. 3C is a rear view of the same subsection of the electrode.

FIG. 4 is an electrical schematic of the electrode shown in FIG. 2.

FIG. 5 is a perspective view of the electrode shown FIG. 2 together with a preferred set of accessories for use therewith.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

FIG. 1 depicts a set of electrodes **10** that are used to apply electric fields to a body part **15** of a subject. Each of the electrodes **10** has at least **11** associated therewith. As described in US Application No. 2005/0209642, which is incorporated herein by reference, a preferred approach for treating tumors using electric fields is to sequentially apply the field to the body part **15** being treated in different directions in an alternating pattern. One preferred approach to applying the field in different directions is to applying the field between a first set of electrodes for a period of time (e.g., 1/4 second), then applying a field between a second set of electrodes for a period of time (e.g., 1/4 second), then repeating that cycle for an extended duration (e.g., over a period of days or weeks). For example, with the electrode configuration depicted in FIG. 1, a horizontal electric field F_A can be induced in the body part **15** by applying an AC voltage between the left and right leads **11** using an appropriate voltage source. Similarly, a vertical electric field F_B can be induced in the body part **15** by applying an AC voltage between the top and bottom leads **11** using the same (or a different) voltage source.

FIG. 2 is a mechanical schematic diagram of a preferred embodiment of each of the electrodes **10**. The electrode **10** includes a plurality of ceramic elements **20**, each of which is preferably disc shaped. The ceramic elements **20** are preferably arranged in an array. Note that while FIG. 2 illustrates a 3x3 array of ceramic elements **20**, arrays of other sizes may be substituted therefor, such as a 2x2 array or a 2x3 array.

The ceramic elements **20** must be mechanically supported and electrical connections must be made to each element. A wide variety of approaches can be readily envisioned for mechanically supporting and electrically making connections to the ceramic elements **20**. One preferred approach that performs both of these functions is to use a flex circuit **24** to both mechanically support the ceramic element **20** and provide the electrical connections. However, a wide variety of alternative approaches can be readily envisioned, including but not limited to discrete wiring, ribbon cable, etc.

Preferably, temperature sensors **22** are incorporated into the electrode **10**, so that appropriate action (e.g., shutting off or lowering the AC voltage, or sounding an alarm) can be taken if an overtemperature condition is detected. In the illustrated embodiment a temperature sensor **22** is provided at each of the ceramic elements. However, in alternative embodiments temperature sensors may be provided only at selected ones of the ceramic elements **20**. For example, when a 3x3 array of ceramic elements **20** are used, a temperature sensor may be provided for the eight outer ceramic elements **20**, and omitted for the center ceramic element. When a flex circuit **24** is used to provide the electrical connection to the ceramic element, additional traces may be provided on the flex circuit to interface with the temperature sensors **22**.

FIG. 3A is a cross section view of one of the ceramic elements **20** with a temperature sensor **22**. Each of the ceramic elements **20** preferably has a conductive backing on the side that faces away from the patient, and this conductive backing is electrically connected to a contact on the flex circuit **24** using any conventional technique (e.g., solder). The conductive backing of the ceramic elements **20** may be implemented by using a ceramic disc that is silvered on one side. A cap **26** is preferably provided to mechanically support each of the ceramic elements **20**. The caps are preferably made of an insulating material e.g., plastic.

In one preferred embodiment, the ceramic elements **20** are implemented using EC99 discs that are about 2 cm in diameter and are silvered on the side that faces away from the patient. In alternative embodiments, the ceramic discs **20** are implemented using ceramic discs that are between about 1.5 cm and about 2.5 cm, with a capacitance of at least 10 nF per disc, so as to provide an array with a capacitance of at least 120 nF. In alternative embodiments, higher capacitance discs may be used (e.g., at least 15 or at least 20 nF per disc). Preferably, the resistance of the ceramic discs should be as high as possible, and they should have a dielectric breakdown voltage of at least 4000 V.

Preferably, the ceramic elements **20** and the caps **26** have holes at their centers that are sized to accommodate the temperature sensors **22**. The temperature sensors are preferably positioned in these holes, and the leads are mounted and electrically connected to respective traces on the flex circuit **24**.

In some preferred embodiments, a thermistor is used as the temperature sensor, in which case two solder connections are needed to connect each thermistor to the flex circuit **24**—one for each lead. However, persons skilled in the relevant arts will appreciate that a wide variety of alternative temperature sensors other than thermistors may also be used, including but not limited to temperature sensing integrated circuits, RTDs, etc. In some preferred embodiments, type NTC thermistors in a surface-mount package are used, with a nominal resistance value of 10 k Ω at 25° C. The operating range is preferably wide enough to sense the expected range temperatures (e.g., from 20-50° C.). Of course, wider operating ranges (e.g., -40° C. to 150° C.) may also be used.

FIG. 3B is an exploded view of the same components depicted in FIG. 3B, and FIG. 3C is a rear view of the same components. Note, however, that in the FIG. 3C view, the ceramic disc 20 and the temperature sensor 22 are obscured by the cap 26.

FIG. 4 is an electrical schematic depicting how the various components of the electrode are connected, in an embodiment where the temperature sensors are implemented using thermistors. The main lead 11 is connected to one side of each of the ceramic elements 20, and the other side of each of the ceramic elements 20 is exposed for placement against the patient's body. When a pair such electrodes are applied to a patient's body, an AC voltage is applied between the main lead 11 of a first electrode and a main lead (not shown) of a similar electrode (not shown). An electric field is generated between the ceramic elements of the first electrodes (depicted in FIG. 4) and the second electrode (of similar configuration). As discussed above, temperature sensors 22 are preferably provided at some or all of the ceramic elements. Preferably, the temperature sensors are configured so that an individual temperature reading can be obtained from each temperature sensor 22. One way to implement this in embodiments that use thermistors for the temperature sensors is to route a lead 42 from one end of each of the thermistors to external circuitry (not shown), and use a common return lead 44 that is shared by all the thermistors. Any conventional circuitry for interfacing with the thermistors may be used.

Of course, persons skilled in the relevant arts will recognize that when alternative temperature sensors are used, the electrical interface to the temperature sensor will have to be adjusted accordingly from the one depicted in FIG. 4. For example, if temperature sensing integrated circuits that communicate over a serial interface bus are used, an appropriate power supply and serial bus must be provided, the implementation of which will be apparent to persons skilled in the relevant arts.

FIG. 5 depicts an electrode that is similar to the electrode 10 discussed above in connection with FIGS. 2-4, together with a preferred set of accessories for use therewith. The electrode 50 is preferably packaged with a layer 52 of biocompatible hydrogel (e.g., Amgel AG603) disposed beneath each of the ceramic discs, and the ceramic discs preferably rest in a filler layer 54 (e.g., 3M 1773 foam tape) with an adhesive bottom and cutouts dimensioned to accept the ceramic discs. A layer of adhesive tape 56 (e.g., 3M 1776 non-woven medical tape) is positioned above the electrode 50, with the adhesive side facing down towards the patient. The adhesive tape 56 preferably extends laterally beyond the electrode 50 and the filler layer 54. A peel-away backing 58 (e.g., #53 white poly-coated kraft paper) is provided beneath all the other components 52-56. To use the electrode, the backing 58 is peeled away, which exposes the bottom of the hydrogel layer 52, the adhesive bottom of the filler layer 54, and uncovered portions of the adhesive tape 56. That entire assembly is then pressed against the patient's skin (which has preferably been shaved) so as to adhere thereto. An electrical connection is then made to the electrode 50 using an appropriate electrical connector.

While the present invention has been disclosed with reference to certain embodiments, numerous modifications, alterations, and changes to the described embodiments are possible without departing from the scope of the present invention, as defined in the appended claims. Accordingly, it is intended that the present invention not be limited to the described embodiments, but that it has the full scope defined by the language of the following claims, and equivalents thereof.

I claim:

1. A composite electrode comprising:
 - a plurality of ceramic elements, each of the ceramic elements having (a) a lower surface configured to rest on a patient's body and (b) an upper surface with a conductive backing disposed thereon;
 - a first lead;
 - at least one electrical conductor configured to make a direct electrical connection between the upper surface of each of the ceramic elements and the first lead; and
 - a support structure configured to mechanically connect the plurality of ceramic elements during use, with the lower surface of each of the plurality of ceramic elements resting on the patient's body.
2. The composite electrode of claim 1, further comprising at least one temperature sensor configured to sense the temperature beneath at least one of the ceramic elements.
3. The composite electrode of claim 1, wherein the least one electrical conductor and the support structure are both implemented using a flex circuit.
4. The composite electrode of claim 1, wherein the plurality of ceramic elements comprises at least 4 ceramic elements.
5. The composite electrode of claim 1,
 - wherein the plurality of ceramic elements comprises at least 4 ceramic discs, each having a diameter between about 1.5 cm and about 2.5 cm and a capacitance of at least 20 nF, and
 - wherein the least one electrical conductor and the support structure are both implemented using a flex circuit.
6. The composite electrode of claim 5, further comprising at least two thermistors configured to sense the temperature beneath at least two of the ceramic discs, respectively.
7. The composite electrode of claim 5, further comprising a covering disposed above the ceramic elements and the support structure, the covering having an adhesive lower surface that is configured to hold the ceramic elements and the support structure against the patient's body.
8. The composite electrode of claim 7, wherein the ceramic elements rest in a filler layer with an adhesive bottom and cutouts dimensioned to accept the ceramic elements.
9. The composite electrode of claim 8, further comprising at least one temperature sensor configured to sense the temperature beneath at least one of the ceramic elements.
10. The composite electrode of claim 9, wherein the ceramic elements are disc-shaped and are silvered on their upper surface.
11. The composite electrode of claim 1,
 - wherein the plurality of ceramic elements consists of nine ceramic discs, each having a diameter between about 1.5 cm and about 2.5 cm and a capacitance of at least 20 nF, wherein the least one electrical conductor and the support structure are both implemented using a flex circuit, and wherein the composite electrode further comprises at least four thermistors configured to sense the temperature beneath at least four of the ceramic discs, respectively.
12. The composite electrode of claim 1, wherein the direct electrical connection between the upper surface of each of the ceramic elements and the first lead is made using a flex circuit that is soldered to the conductive backing.
13. A composite electrode comprising:
 - at least four ceramic elements, each of the ceramic elements having (a) a lower surface configured to rest on a patient's body and (b) an upper surface with a conductive backing disposed thereon;
 - a first lead;

5

at least one electrical conductor configured to make a direct electrical connection between the upper surface of each of the ceramic elements and the first lead; and

a support structure configured to mechanically connect the ceramic elements during use, with the lower surface of each of the ceramic elements resting on the patient's body;

at least two temperature sensors configured to sense the temperature beneath at least two of the ceramic elements, respectively;

a layer of electrically conductive hydrogel disposed on the lower surface of each of the ceramic elements;

a covering disposed above the ceramic elements and the support structure, the covering having an adhesive lower surface that is configured to hold the ceramic elements and the support structure against the patient's body.

14. The composite electrode of claim 13, further comprising a backing disposed beneath the ceramic elements, the support structure, and the covering, wherein the adhesive lower surface of the covering is easily removable from the backing.

15. The composite electrode of claim 13, wherein the temperature sensors comprise thermistors.

16. The composite electrode of claim 13, wherein the least one electrical conductor and the support structure are both implemented using a flex circuit.

17. The composite electrode of claim 13, wherein there are 9 ceramic elements.

18. The composite electrode of claim 13, wherein there are 9 ceramic elements that are each round and have a diameter between about 1.5 cm and about 2.5 cm and a capacitance of at least 20 nF, and

wherein the least one electrical conductor and the support structure are both implemented using a flex circuit, and

6

wherein there are at least four temperature sensors configured to sense the temperature beneath at least four of the ceramic elements, respectively.

19. The composite electrode of claim 18, wherein the ceramic elements rest in a foam filler layer with an adhesive bottom and cutouts dimensioned to accept the ceramic elements.

20. The composite electrode of claim 18, wherein the ceramic elements are disc-shaped and are silvered on their upper surface.

21. The composite electrode of claim 20, wherein the ceramic elements have holes in their centers and the temperature sensors are positioned in the holes.

22. The composite electrode of claim 13, wherein the ceramic elements are disc-shaped and are silvered on their upper surface.

23. The composite electrode of claim 22, wherein the ceramic elements have holes in their centers and the temperature sensors are positioned in the holes.

24. The composite electrode of claim 13, wherein the ceramic elements rest in a filler layer.

25. The composite electrode of claim 13, wherein the ceramic elements rest in a filler layer with an adhesive bottom and cutouts dimensioned to accept the ceramic elements.

26. The composite electrode of claim 13, wherein the ceramic elements rest in a foam filler layer with an adhesive bottom and cutouts dimensioned to accept the ceramic elements.

27. The composite electrode of claim 13, wherein the direct electrical connection between the upper surface of each of the ceramic elements and the first lead is made using a flex circuit that is soldered to the conductive backing.

* * * * *

专利名称(译)	复合电极		
公开(公告)号	US8764675	公开(公告)日	2014-07-01
申请号	US13/790258	申请日	2013-03-08
[标]申请(专利权)人(译)	诺沃库勒有限公司		
当前申请(专利权)人(译)	NOVOCURE有限公司		
[标]发明人	PALTI YORAM		
发明人	PALTI, YORAM		
IPC分类号	A61B5/00 A61B5/103		
CPC分类号	A61N1/40 A61N1/32 A61N1/048 A61B5/441 A61N1/0492 A61N1/0408 A61N1/0476 A61N1/326 A61N1/0472 A61B5/411		
代理机构(译)	普罗斯考尔		
其他公开文献	US20130190847A1		
外部链接	Espacenet USPTO		

摘要(译)

用于向患者施加电场的电极包括多个陶瓷元件（例如，陶瓷盘），其被设计成抵靠患者的皮肤定位。对陶瓷元件进行电连接（例如，使用柔性电路）。温度传感器（例如，热敏电阻）优选地设置在至少一些陶瓷元件上以感测陶瓷元件下方的皮肤处的温度，从而如果检测到过温条件则可以采取适当的动作。

