



US009649042B2

(12) **United States Patent**
Albert et al.

(10) **Patent No.:** **US 9,649,042 B2**
(45) **Date of Patent:** ***May 16, 2017**

(54) **HEART MONITORING SYSTEM USABLE WITH A SMARTPHONE OR COMPUTER**

(58) **Field of Classification Search**
CPC A61B 5/024; A61B 5/0245; A61B 5/0404
See application file for complete search history.

(71) Applicant: **AliveCor, Inc.**, San Francisco, CA (US)

(56) **References Cited**

(72) Inventors: **David Albert**, Oklahoma City, OK (US); **Bruce Richard Satchwell**, Carrara (AU); **Kim Norman Barnett**, Mt. Tamborine (AU)

U.S. PATENT DOCUMENTS

3,717,857 A 2/1973 Evans
3,731,311 A 5/1973 Williams
(Continued)

(73) Assignee: **ALIVECOR, INC.**, San Francisco, CA (US)

FOREIGN PATENT DOCUMENTS

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 239 days.

CH 675675 A5 10/1990
CN 101828915 A 9/2010
(Continued)

This patent is subject to a terminal disclaimer.

OTHER PUBLICATIONS

(21) Appl. No.: **13/964,490**

Adidas miCoach Pacer Review: Like Nike+, Only Better; printed from website <http://gizmodo.com/5479456/adidas> on Mar. 4, 2010; 5 pgs.

(22) Filed: **Aug. 12, 2013**

(Continued)

(65) **Prior Publication Data**

US 2013/0331663 A1 Dec. 12, 2013

Primary Examiner — Edward Moran
Assistant Examiner — Elizabeth K So
(74) *Attorney, Agent, or Firm* — Wison Sonsini Goodrich & Rosati

Related U.S. Application Data

(62) Division of application No. 12/796,188, filed on Jun. 8, 2010, now Pat. No. 8,509,882.


(57) **ABSTRACT**

(51) **Int. Cl.**
A61B 5/04 (2006.01)
A61B 5/0402 (2006.01)
(Continued)

A personal monitoring device has a sensor assembly configured to sense physiological signals upon contact with a user's skin. The sensor assembly produces electrical signals representing the sensed physiological signals. A converter assembly, integrated with, and electrically connected to the sensor assembly, converts the electrical signals generated by the sensor assembly to a frequency modulated physiological audio signal having a carrier frequency in the range of from about 6 kHz to about 20 kHz.

(52) **U.S. Cl.**
CPC **A61B 5/0402** (2013.01); **A61B 5/0404** (2013.01); **A61B 5/6898** (2013.01);
(Continued)

14 Claims, 4 Drawing Sheets

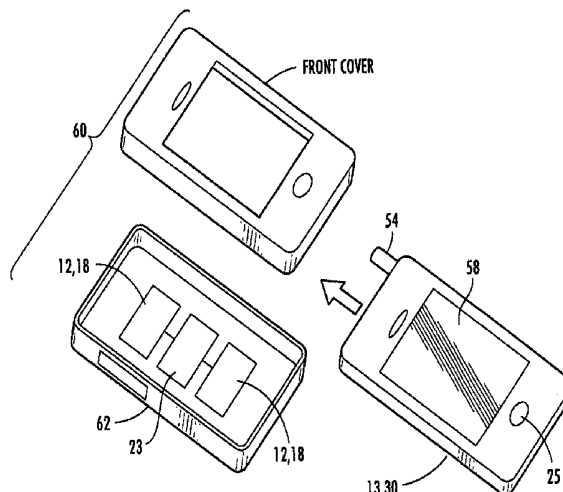

(51)	Int. Cl.						
	<i>A61B 5/0404</i>	(2006.01)		5,343,869 A	9/1994	Pross et al.	
	<i>A61B 5/00</i>	(2006.01)		5,343,870 A	9/1994	Gallant et al.	
	<i>A61B 5/055</i>	(2006.01)		5,348,008 A	9/1994	Bornn et al.	
(52)	U.S. Cl.			5,360,005 A	11/1994	Wilk	
	CPC	<i>A61B 5/055</i> (2013.01); <i>A61B 2505/07</i>		5,365,935 A	11/1994	Righter et al.	
		(2013.01); <i>A61B 2560/045</i> (2013.01); <i>A61B</i>		5,410,587 A	4/1995	Grunwell	
		<i>2560/0468</i> (2013.01)		5,417,222 A	5/1995	Dempsey et al.	
				5,433,736 A	7/1995	Nilsson	
				5,452,356 A	9/1995	Albert	
				5,466,246 A	11/1995	Silvian	
				5,467,773 A	11/1995	Bergelson et al.	
				5,481,255 A	1/1996	Albert et al.	
				5,503,158 A	4/1996	Coppock et al.	
				5,518,001 A	5/1996	Snell	
				5,522,396 A	6/1996	Langer et al.	
				5,539,705 A	7/1996	Akerman et al.	
				D372,785 S	8/1996	Sabri et al.	
				5,544,661 A	8/1996	Davis et al.	
				5,551,953 A	9/1996	Lattin et al.	
				5,561,712 A	10/1996	Nishihara	
				5,568,448 A	10/1996	Tanigushi et al.	
				5,579,284 A	11/1996	May	
				D377,983 S	2/1997	Sabri et al.	
				5,608,723 A	3/1997	Felsenstein	
				5,634,468 A	6/1997	Platt et al.	
				5,652,570 A	7/1997	Lepkofker	
				5,661,699 A	8/1997	Sutton	
				5,675,325 A	10/1997	Taniguchi et al.	
				5,678,562 A	10/1997	Sellers	
				5,701,894 A	12/1997	Cherry et al.	
				5,704,364 A	1/1998	Saltzstein et al.	
				5,724,025 A	3/1998	Tavori	
				5,730,143 A	3/1998	Schwarzberg	
				5,735,285 A *	4/1998	Albert	G06F 19/3418
							128/904
(56)	References Cited						
	U.S. PATENT DOCUMENTS						
	3,768,014 A	10/1973	Smith et al.				
	3,776,228 A	12/1973	Semler				
	3,779,237 A	12/1973	Goeltz et al.				
	3,779,249 A	12/1973	Semler				
	3,782,367 A	1/1974	Hochberg et al.				
	3,805,227 A	4/1974	Lester				
	3,882,277 A	5/1975	DePedro et al.				
	3,885,552 A	5/1975	Kennedy				
	3,898,984 A	8/1975	Mandel et al.				
	3,909,599 A	9/1975	Trott, Jr. et al.				
	4,027,146 A	5/1977	Gilmore				
	4,045,767 A	8/1977	Nishihara et al.				
	4,083,366 A	4/1978	Gombrich et al.				
	4,095,050 A	6/1978	Beachem et al.				
	4,221,223 A	9/1980	Linden				
	4,230,127 A	10/1980	Larson				
	4,231,031 A	10/1980	Crowther et al.				
	4,250,888 A	2/1981	Grosskopf				
	4,281,664 A	8/1981	Duggan				
	4,295,472 A	10/1981	Adams				
	4,312,358 A	1/1982	Barney	5,742,251 A	4/1998	Gerber	
	4,318,130 A	3/1982	Heuer	5,748,103 A	5/1998	Flach et al.	
	4,364,397 A	12/1982	Citron et al.	5,764,763 A	6/1998	Jensen et al.	
	4,367,752 A	1/1983	Jimenez et al.	5,772,586 A	6/1998	Heinonen et al.	
	4,409,984 A	10/1983	Dick	5,818,788 A	10/1998	Kimura et al.	
	4,531,527 A	7/1985	Reinhold, Jr. et al.	5,825,718 A	10/1998	Ueki et al.	
	4,567,883 A	2/1986	Langer et al.	5,827,179 A	10/1998	Lichter et al.	
	4,572,182 A	2/1986	Royse	5,840,020 A	11/1998	Heinonen et al.	
	4,580,250 A	4/1986	Kago et al.	5,844,997 A	12/1998	Murphy, Jr.	
	4,583,553 A	4/1986	Shah et al.	5,861,018 A	1/1999	Feierbach	
	4,622,979 A	11/1986	Katchis et al.	5,873,369 A	2/1999	Laniado et al.	
	4,625,730 A	12/1986	Fountain et al.	5,876,351 A	3/1999	Rohde	
	4,803,625 A	2/1989	Fu et al.	5,877,675 A	3/1999	Rebstock et al.	
	4,889,131 A	12/1989	Salem et al.	5,889,730 A	3/1999	May	
	4,920,489 A	4/1990	Hubelbank et al.	5,929,761 A	7/1999	Van Der Laan et al.	
	4,938,228 A	7/1990	Righter et al.	D414,870 S	10/1999	Saltzstein et al.	
	4,938,229 A	7/1990	Bergelson et al.	5,970,388 A	10/1999	Will	
	4,958,641 A	9/1990	Digby et al.	5,976,083 A	11/1999	Richardson et al.	
	4,977,899 A	12/1990	Digby et al.	5,982,297 A	11/1999	Welle	
	4,981,141 A	1/1991	Segalowitz	5,983,127 A	11/1999	Depinto	
	5,012,814 A	5/1991	Mills et al.	6,008,703 A	12/1999	Perrott et al.	
	5,023,906 A	6/1991	Novas	6,024,705 A	2/2000	Schlager et al.	
	5,025,794 A	6/1991	Albert et al.	6,037,704 A	3/2000	Welle	
	5,058,597 A	10/1991	Onoda et al.	6,047,206 A	4/2000	Albrecht et al.	
	5,090,418 A	2/1992	Squires et al.	6,047,257 A	4/2000	Dewaele	
	5,111,396 A	5/1992	Mills et al.	6,048,319 A	4/2000	Hudgins et al.	
	5,128,552 A	7/1992	Fang et al.	D427,315 S	6/2000	Saltzstein et al.	
	5,136,555 A	8/1992	Gardos	6,072,396 A	6/2000	Gaukel	
	5,181,519 A	1/1993	Bible	6,083,248 A	7/2000	Thompson	
	5,191,891 A	3/1993	Righter	6,084,510 A	7/2000	Lemelson et al.	
	5,201,321 A	4/1993	Fulton	6,102,856 A	8/2000	Groff et al.	
	5,218,969 A	6/1993	Bredesen et al.	6,153,532 A	11/2000	Dow et al.	
	5,226,424 A	7/1993	Bible	6,159,147 A	12/2000	Lichter et al.	
	5,238,001 A	8/1993	Gallant et al.	6,198,394 B1	3/2001	Jacobsen et al.	
	D341,659 S	11/1993	Homayoun et al.	6,224,548 B1	5/2001	Gopinathan et al.	
	5,259,387 A	11/1993	Depinto	6,236,889 B1	5/2001	Soykan et al.	
	5,301,679 A	4/1994	Taylor	6,264,614 B1	7/2001	Albert et al.	
	5,304,186 A	4/1994	Semler et al.	6,282,440 B1	8/2001	Brodnick et al.	
	5,313,953 A	5/1994	Yomtov et al.	6,282,441 B1	8/2001	Raymond et al.	
	5,321,618 A	6/1994	Gessman	6,289,238 B1	9/2001	Besson et al.	
	5,333,616 A	8/1994	Mills et al.	6,319,201 B1	11/2001	Wilk	
	5,336,245 A	8/1994	Adams et al.	6,343,049 B1	1/2002	Toda	
	5,337,752 A	8/1994	Reeves	6,363,139 B1	3/2002	Zurek et al.	
	5,339,824 A	8/1994	Engira	6,364,834 B1	4/2002	Reuss et al.	

(56)

References Cited

U.S. PATENT DOCUMENTS

6,366,871	B1	4/2002	Geva	7,819,814	B2	10/2010	Gavriely et al.
6,377,843	B1	4/2002	Naydenov et al.	7,846,104	B2	12/2010	Macquarrie et al.
6,418,394	B1	7/2002	Puolakanaho et al.	7,846,106	B2	12/2010	Andrews et al.
6,433,689	B1	8/2002	Hovind et al.	7,904,160	B2	3/2011	Brodnick et al.
6,453,164	B1	9/2002	Fuller et al.	7,945,064	B2	5/2011	O'Brien et al.
6,478,736	B1	11/2002	Mault	7,946,959	B2	5/2011	Shum et al.
6,485,416	B1	11/2002	Platt et al.	7,955,273	B2	6/2011	Rahe-Meyer
6,507,734	B1	1/2003	Berger et al.	7,983,749	B2	7/2011	Warren
6,513,532	B2	2/2003	Mault et al.	8,019,609	B2	9/2011	Tamir et al.
6,549,756	B1	4/2003	Engstrom	8,034,006	B2	10/2011	Celik-Butler et al.
6,558,320	B1	5/2003	Causey et al.	8,062,090	B2	11/2011	Atsmon et al.
6,579,231	B1	6/2003	Phipps	8,078,136	B2	12/2011	Atsmon et al.
6,595,929	B2	7/2003	Stivoric et al.	8,078,278	B2	12/2011	Penner
6,600,471	B2	7/2003	Lee et al.	8,126,526	B2	2/2012	Kitajima et al.
6,605,038	B1	8/2003	Teller et al.	8,126,566	B2	2/2012	Stahmann et al.
6,612,985	B2	9/2003	Eiffert et al.	8,126,728	B2	2/2012	Dicks et al.
6,616,613	B1	9/2003	Goodman	8,130,093	B2	3/2012	Mazar et al.
6,636,761	B2	10/2003	Brodnick	8,150,750	B2	4/2012	Ray
6,685,633	B2	2/2004	Albert et al.	8,160,276	B2	4/2012	Liao et al.
6,717,983	B1	4/2004	Toda	8,165,677	B2	4/2012	Von et al.
6,790,178	B1	9/2004	Mault et al.	8,216,136	B2	7/2012	Addison et al.
6,804,558	B2	10/2004	Haller et al.	8,224,429	B2	7/2012	Prstojevich et al.
6,820,057	B1	11/2004	Loch et al.	8,265,907	B2	9/2012	Nanikashvili et al.
6,845,263	B2	1/2005	Kawaguchi	8,275,553	B2	9/2012	Ochs et al.
6,893,396	B2	5/2005	Schulze et al.	8,275,635	B2	9/2012	Stivoric et al.
6,928,535	B2	8/2005	Yamashita et al.	8,282,550	B2	10/2012	Rasdal et al.
6,950,681	B2	9/2005	Hofmann	8,285,356	B2	10/2012	Bly et al.
6,970,737	B1	11/2005	Brodnick et al.	8,301,232	B2	10/2012	Albert et al.
6,987,965	B2	1/2006	Ng et al.	8,301,236	B2	10/2012	Baumann et al.
7,018,339	B2	3/2006	Birnbaum et al.	8,323,188	B2	12/2012	Tran
7,020,508	B2	3/2006	Stivoric et al.	8,328,718	B2	12/2012	Tran
7,031,745	B2	4/2006	Shen	8,332,233	B2	12/2012	Ott et al.
7,061,381	B2	6/2006	Forcier et al.	8,364,250	B2	1/2013	Moon et al.
7,103,407	B2	9/2006	Hjelt et al.	8,369,936	B2	2/2013	Farringdon et al.
7,107,095	B2	9/2006	Manolas	8,374,688	B2	2/2013	Libbus et al.
7,108,659	B2	9/2006	Ross et al.	8,449,471	B2	5/2013	Tran
7,153,262	B2	12/2006	Stivoric et al.	8,500,636	B2	8/2013	Tran
7,162,291	B1	1/2007	Nachaliel	8,509,882	B2*	8/2013	Albert A61B 5/0404 600/509
7,162,294	B2	1/2007	Rowlandson et al.	8,519,835	B2	8/2013	Dunko
7,188,151	B2	3/2007	Kumar et al.	8,543,185	B2	9/2013	Yuen et al.
7,222,054	B2	5/2007	Geva	8,548,770	B2	10/2013	Yuen et al.
7,236,818	B2	6/2007	Mcleod et al.	8,700,137	B2	4/2014	Albert
7,257,448	B2	8/2007	Crowe et al.	8,725,229	B2	5/2014	Furue et al.
7,260,429	B2	8/2007	Siejko et al.	8,755,871	B2	6/2014	Weng et al.
7,261,690	B2	8/2007	Teller et al.	8,923,958	B2	12/2014	Gupta et al.
7,285,090	B2	10/2007	Stivoric et al.	8,951,189	B2	2/2015	Osorio
7,319,425	B2	1/2008	Fiorenza et al.	8,951,192	B2	2/2015	Osorio
7,324,836	B2	1/2008	Steenstra et al.	8,974,396	B1	3/2015	Brady et al.
7,349,574	B1	3/2008	Sodini et al.	8,977,347	B2	3/2015	Mestha et al.
7,351,207	B2	4/2008	Priemer	9,026,202	B2	5/2015	Albert
7,354,400	B2	4/2008	Asafusa et al.	9,351,654	B2	5/2016	Albert
7,382,247	B2	6/2008	Welch et al.	9,420,956	B2	8/2016	Gopalakrishnan et al.
7,383,297	B1	6/2008	Atsmon et al.	2001/0027384	A1	10/2001	Schulze et al.
7,398,115	B2	7/2008	Lynn	2001/0031998	A1	10/2001	Nelson et al.
7,415,304	B2	8/2008	Rowlandson et al.	2001/0051766	A1	12/2001	Gazdzinski
7,444,116	B2	10/2008	Ivanov et al.	2002/0016541	A1	2/2002	Glossop
7,460,899	B2	12/2008	Almen	2002/0032386	A1	3/2002	Sackner et al.
7,502,643	B2	3/2009	Farringdon et al.	2002/0111556	A1	8/2002	Wegner
7,509,159	B2	3/2009	Xue et al.	2002/0143576	A1	10/2002	Nolvak et al.
7,515,043	B2	4/2009	Welch et al.	2003/0004425	A1	1/2003	Narimatsu et al.
7,515,044	B2	4/2009	Welch et al.	2003/0093002	A1	5/2003	Kuo
7,520,860	B2	4/2009	Guion-Johnson et al.	2003/0107487	A1	6/2003	Korman et al.
7,542,878	B2	6/2009	Nanikashvili	2003/0117987	A1	6/2003	Brebner
7,548,623	B2	6/2009	Manabe	2003/0149344	A1	8/2003	Nizan
7,596,405	B2	9/2009	Kurzweil et al.	2003/0193839	A1	10/2003	Singh
7,603,148	B2	10/2009	Michalak	2004/0034284	A1	2/2004	Aversano et al.
7,647,185	B2	1/2010	Tarassenko et al.	2004/0044292	A1	3/2004	Yasushi et al.
7,654,148	B2	2/2010	Tomlinson, Jr. et al.	2004/0059205	A1	3/2004	Carlson et al.
7,657,479	B2	2/2010	Henley	2004/0117212	A1	6/2004	Kong et al.
7,668,589	B2	2/2010	Bauer	2004/0120356	A1	6/2004	Davenport et al.
7,689,437	B1	3/2010	Teller et al.	2004/0143403	A1	7/2004	Brandon et al.
7,701,895	B2	4/2010	Gehasie et al.	2004/0215088	A1	10/2004	Hubelbank
7,733,224	B2	6/2010	Tran	2004/0215094	A1	10/2004	Baumer et al.
7,742,808	B2	6/2010	Nissilä	2004/0220487	A1	11/2004	Vyshedskiy et al.
7,806,832	B2	10/2010	Gallagher et al.	2004/0220488	A1	11/2004	Vyshedskiy et al.
				2004/0225199	A1	11/2004	Evanyk et al.
				2004/0228217	A1	11/2004	Szeto
				2004/0236819	A1	11/2004	Anati et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2004/0266407 A1 12/2004 Lee et al.
 2004/0266480 A1 12/2004 Hjelt et al.
 2005/0014531 A1 1/2005 Findikli
 2005/0027207 A1 2/2005 Westbrook et al.
 2005/0078533 A1 4/2005 Vyshedskiy et al.
 2005/0124864 A1 6/2005 Mack et al.
 2005/0234353 A1 10/2005 Xue et al.
 2005/0239493 A1 10/2005 Batkin et al.
 2006/0022833 A1 2/2006 Ferguson et al.
 2006/0047215 A1 3/2006 Newman et al.
 2006/0173259 A1 8/2006 Flaherty et al.
 2006/0190045 A1 8/2006 Marcus et al.
 2006/0193270 A1 8/2006 Gehasie et al.
 2006/0252999 A1 11/2006 Devaul et al.
 2007/0021677 A1 1/2007 Markel
 2007/0027386 A1 2/2007 Such et al.
 2007/0032731 A1 2/2007 Lovejoy et al.
 2007/0063850 A1 3/2007 Devaul et al.
 2007/0073266 A1 3/2007 Chmiel et al.
 2007/0106179 A1 5/2007 Bagha et al.
 2007/0156060 A1 7/2007 Cervantes
 2007/0254604 A1 11/2007 Kim
 2007/0265038 A1 11/2007 Kim
 2008/0009759 A1 1/2008 Chetham
 2008/0058670 A1 3/2008 Mainini
 2008/0112885 A1 5/2008 Okunev et al.
 2008/0146890 A1 6/2008 LeBoeuf et al.
 2008/0146892 A1 6/2008 LeBoeuf et al.
 2008/0171945 A1 7/2008 Dotter
 2008/0177162 A1 7/2008 Bae et al.
 2008/0198872 A1 8/2008 Pierce
 2008/0214903 A1 9/2008 Orbach
 2008/0228045 A1 9/2008 Gao et al.
 2008/0293453 A1 11/2008 Atlas et al.
 2009/0010461 A1 1/2009 Klinghult et al.
 2009/0024045 A1 1/2009 Prakash et al.
 2009/0037575 A1 2/2009 Crystal et al.
 2009/0117883 A1 5/2009 Coffing et al.
 2009/0144080 A1 6/2009 Gray et al.
 2009/0149767 A1 6/2009 Rossetti
 2009/0156908 A1 6/2009 Belalcazar et al.
 2009/0171170 A1 7/2009 Li et al.
 2009/0209873 A1 8/2009 Pinter et al.
 2009/0273467 A1 11/2009 Elixmann et al.
 2009/0279389 A1 11/2009 Irie
 2009/0287067 A1 11/2009 Dorogusker et al.
 2009/0306485 A1 12/2009 Bell
 2009/0312655 A1 12/2009 Lo
 2010/0027379 A1 2/2010 Saulnier et al.
 2010/0033303 A1 2/2010 Dugan et al.
 2010/0035927 A1 2/2010 Ojika et al.
 2010/0042008 A1 2/2010 Amitai et al.
 2010/0049006 A1 2/2010 Magar et al.
 2010/0049037 A1 2/2010 Pinter et al.
 2010/0063381 A1 3/2010 Greiser
 2010/0069735 A1 3/2010 Berkner
 2010/0076276 A1 3/2010 Gilland
 2010/0094152 A1 4/2010 Semmflow
 2010/0113950 A1 5/2010 Lin et al.
 2010/0148956 A1 6/2010 Song et al.
 2010/0184479 A1 7/2010 Griffin, Jr.
 2010/0204758 A1 8/2010 Boon et al.
 2010/0208434 A1 8/2010 Kim et al.
 2010/0217099 A1 8/2010 LeBoeuf et al.
 2010/0217100 A1 8/2010 LeBoeuf et al.
 2010/0217345 A1 8/2010 Wolfe et al.
 2010/0234746 A1 9/2010 Sebelius et al.
 2010/0256509 A1 10/2010 Kuo et al.
 2010/0256976 A1 10/2010 Atsmon et al.
 2010/0281261 A1 11/2010 Razzell
 2010/0298711 A1 11/2010 Pedersen et al.
 2010/0324378 A1 12/2010 Tran et al.
 2010/0331631 A1 12/2010 Maclaughlin
 2011/0015496 A1 1/2011 Sherman et al.
 2011/0035927 A1 2/2011 Griffin et al.

2011/0060251 A1 3/2011 Verma et al.
 2011/0066042 A1 3/2011 Pandia et al.
 2011/0117529 A1 5/2011 Barash et al.
 2011/0134725 A1 6/2011 Su et al.
 2011/0160601 A1 6/2011 Wang et al.
 2011/0182445 A1 7/2011 Atsmon et al.
 2011/0208076 A1 8/2011 Fong et al.
 2011/0235466 A1 9/2011 Booij et al.
 2011/0275950 A1 11/2011 Xue et al.
 2011/0288425 A1 11/2011 Stewart
 2011/0301435 A1 12/2011 Albert et al.
 2011/0301439 A1 12/2011 Albert et al.
 2012/0051187 A1 3/2012 Paulson et al.
 2012/0053424 A1 3/2012 Kenalty et al.
 2012/0071734 A1 3/2012 Shimuta et al.
 2012/0083705 A1 4/2012 Yuen et al.
 2012/0101396 A1 4/2012 Solosko et al.
 2012/0108916 A1 5/2012 Riftine
 2012/0123891 A1 5/2012 Patel
 2012/0127833 A1 5/2012 Ghen et al.
 2012/0143018 A1 6/2012 Skidmore et al.
 2012/0147921 A1 6/2012 Conti et al.
 2012/0157019 A1 6/2012 Li
 2012/0158090 A1 6/2012 Chavan et al.
 2012/0171963 A1 7/2012 Tsfaty
 2012/0172689 A1 7/2012 Albert et al.
 2012/0179056 A1 7/2012 Moulder et al.
 2012/0197148 A1 8/2012 Levitan et al.
 2012/0285588 A1 11/2012 Sheppard
 2012/0289790 A1 11/2012 Jain et al.
 2012/0316413 A1 12/2012 Liu et al.
 2013/0003852 A1 1/2013 Yamamoto
 2013/0030259 A1 1/2013 Thomsen et al.
 2013/0085364 A1 4/2013 Lu et al.
 2013/0122810 A1 5/2013 Kaufman
 2013/0156194 A1 6/2013 Tanioka
 2013/0159699 A1 6/2013 Torkkel
 2013/0197320 A1 8/2013 Albert et al.
 2013/0236980 A1 9/2013 Moretti et al.
 2013/0261414 A1 10/2013 Tal et al.
 2013/0281816 A1 10/2013 Strauss et al.
 2013/0289366 A1 10/2013 Chua et al.
 2014/0050321 A1 2/2014 Albert et al.
 2014/0051941 A1 2/2014 Messerschmidt
 2014/0051946 A1 2/2014 Arne et al.
 2014/0066798 A1 3/2014 Albert
 2014/0073969 A1 3/2014 Zou et al.
 2014/0114166 A1 4/2014 Baxi
 2014/0163927 A1 6/2014 Molettiere et al.
 2014/0221859 A1 8/2014 Albert
 2014/0276162 A1 9/2014 Albert et al.
 2015/0018660 A1 1/2015 Thomson et al.
 2015/0073285 A1 3/2015 Albert et al.
 2015/0087952 A1 3/2015 Albert et al.
 2015/0182132 A1 7/2015 Harris et al.
 2015/0265164 A1 9/2015 Gopalakrishnan et al.
 2015/0297134 A1 10/2015 Albert et al.
 2016/0235319 A1 8/2016 Albert
 2016/0331247 A1 11/2016 Albert

FOREIGN PATENT DOCUMENTS

CN 201918016 U 8/2011
 CN 102347804 A 2/2012
 CN 105338892 A 2/2016
 DE 2506936 A1 9/1976
 DE 4212670 A1 1/1994
 EP 0631226 A1 12/1994
 EP 1782229 A 5/2007
 EP 1181888 B1 9/2007
 EP 1238633 B1 10/2008
 EP 2030565 A1 3/2009
 EP 2192526 A2 6/2010
 EP 2116183 B1 2/2012
 EP 2986204 A1 2/2016
 EP 3079571 A1 10/2016
 FR 2740426 A1 4/1997
 GB 2181554 A 4/1987
 GB 2408105 A 5/2005

(56)

References Cited

FOREIGN PATENT DOCUMENTS

JP	S59122032	A	7/1984
JP	S59190742	A	10/1984
JP	S63072231	A	4/1988
JP	S63294044	A	11/1988
JP	H01244328	A	9/1989
JP	H05167540	A	7/1993
JP	H06326669	A	11/1994
JP	2002191562	A	7/2002
JP	2002261731	A	9/2002
JP	2003010177	A	1/2003
JP	2005295378	A	10/2005
JP	2006180899	A	7/2006
JP	2008532587	A	8/2008
JP	2010166961	A	8/2010
JP	2012065073	A	3/2012
KR	20100059198	A	6/2010
MX	2009011781	A	5/2011
WO	WO-8200910	A1	3/1982
WO	WO88/05282	A1	7/1988
WO	WO90/08361	A1	7/1990
WO	WO92/06551	A1	4/1992
WO	WO-9731437	A1	8/1997
WO	WO98/38611	A1	9/1998
WO	WO99/44494	A1	9/1999
WO	WO00/41620	A1	7/2000
WO	WO01/47597	A2	7/2001
WO	WO-0157619	A2	8/2001
WO	WO02/080762	A1	10/2002
WO	WO03/075118	A2	9/2003
WO	WO03/094720	A1	11/2003
WO	WO2004/037080	A1	5/2004
WO	WO2006/001005	A2	1/2006
WO	WO-2006021956	A2	3/2006
WO	WO-2006090371	A2	8/2006
WO	WO2007/014545	A2	2/2007
WO	WO2007/088315	A1	8/2007
WO	WO2008/005015	A1	1/2008
WO	WO-2008066682	A2	6/2008
WO	WO-2009112976	A1	9/2009
WO	WO2010/025166	A1	3/2010
WO	WO2010/108287	A1	9/2010
WO	WO-2010099066	A2	9/2010
WO	WO2010/113354		10/2010
WO	WO 2010/144626	A1	12/2010
WO	WO 2011/006356	A1	1/2011
WO	WO 2011/008838	A1	1/2011
WO	WO 2011/014292	A1	2/2011
WO	WO 2011/022942	A1	3/2011
WO	WO 2011/040877	A1	4/2011
WO	WO2011/040878	A1	4/2011
WO	WO2011/113070	A1	9/2011
WO	WO-2011137375	A2	11/2011
WO	WO-2011156374	A2	12/2011
WO	WO-2012046158	A1	4/2012
WO	WO-2012108895	A1	8/2012
WO	WO-2012129413	A1	9/2012
WO	WO-2012160550	A1	11/2012
WO	WO-2013028960	A1	2/2013
WO	WO-2013036307	A1	3/2013
WO	WO-2013066642	A1	5/2013
WO	WO-2013093690	A1	6/2013
WO	WO-2013122788	A1	8/2013
WO	WO-2013138500	A1	9/2013
WO	WO-2013155196	A2	10/2013
WO	WO-2013192166	A1	12/2013
WO	WO-2014172451	A1	10/2014
WO	WO-2016183515	A1	11/2016

OTHER PUBLICATIONS

Australian Design Awards; Heartplus Micro; printed from website <http://www.designawards.com/au> on Apr. 12, 2002; 6 pgs.

Bajaj, M.D.; Event Recording in Ambulatory Patients with Syncope Events; University of Kansas; Wichita, Kansas; (no date); pp. 15-18; printed on or before Apr. 14, 2010.

Bluetooth; Headset Profile (HSP); printed from website <http://bluetooth.com/English/Technology/Works/Pates/HSP.aspx>, printed May 12, 2010; 1 pg.

Bramanti et al.; Multichannel telemetric system for biomedical signals via switched telephone lines; Medical and Biological Engineering and Computing, Sep. 1982, vol. 20, No. 5, pp. 653-656.

Vitaphone; Telemedicine since 1999: Modern health management is our special subject; 3 pgs; retrieved Mar. 19, 2014 from the internet (<http://www.vitaphone.de/en/company/history-of-vitaphone/>).

Albert et al.; U.S. Appl. No. 14/217,032 entitled "Systems and methods for processing and analyzing medical data," filed Mar. 17, 2014.

Albert, David E.; U.S. Appl. No. 14/252,044 entitled "Cardiac performance monitoring system for use with mobile communications devices," filed Apr. 14, 2014.

MacFarlane et al.; Resting 12-lead ECG electrode placement and associated problems; SCST Update 1995; 15 pgs.; printed Feb. 18, 2014 from www.scst.org.uk/resources/RESTING_12.pdf? (year of pub. sufficiently earlier than effective US filed and any foreign priority date).

Galloway et al.; U.S. Appl. No. 14/076,076 entitled "Electrocardiogram Signal Detection," filed Nov. 8, 2013.

Albert et al.; U.S. Appl. No. 14/149,242 entitled "Methods and systems for electrode placement," filed Jan. 7, 2014.

Burke, A Micropower Dry-Electrode ECG Preamplifier; IEEE Transactions on Biomedical Engineering, Feb. 2000, vol. 47, No. 2, pp. 155-162.

Card Guard; CG-6108 ACT Ambulatory Cardiac Telemetry Brochure; Card Guard, The Telemedicine Company; Switzerland; (year of publication is sufficiently earlier than the effective U.S. filing date and any foreign priority date) 2006; 2 pgs.

Cardiocomm Solutions; GEMS Air (PC based ECG management); printed from website <http://www.cardiocommsolutions.com> on Mar. 19, 2010; 1 pg.

Charuvastra; Transtelephonic Cardiac Event Recording for Arrhythmia Surveillance; printed from website http://tchin.org/resource_room/c_art on Mar. 26, 2010; 2 pgs.

Cheng, Allen C.; Real-Time Cardiovascular Diseases Detection on a Smartphone; printed Apr. 14, 2010.

Company-Bosch et al.; ECG Front-End Design is Simplified with MicroConverter; Analog Dialogue; Nov. 2003; vol. 37(11); pp. 1-5. Creative; PC-80B Portable ECG Monitor w/sd card extension slot; printed from website www.amazon.com/Portable-Monitor-extension-leather-shipping/dp/B001OjWKUE on Feb. 4, 2010; 3 pgs.

Deveau, Health care eyes smart phones to heal ills (posted Sep. 15, 2009); printed from website <http://www.theQiobeandmail.com> on Sep. 17, 2009, 4 pages.

Dobrev, et al.; Bootstrapped two-electrode biosignal amplifier; Med Biol Eng Comput; vol. 46(6); Jun. 2008, pp. 613-619.

Elert, Glenn (Editor); Frequency Range of Human Hearing; The Physics Factbook; web version as of Mar. 29, 2010; 2 pgs.; printed Jun. 6, 2012 (<http://web.archive.org/web/20100329141847/http://hypertextbook.com/facts/2003/ChrisDAmbrose.shtml>).

Favorite Plus; Handheld Easy ECG Monitor; (Product ID: FP180); printed from website www.favoriteplus.com/easy-ecg-handheld-monitor-fp180 on Feb. 4, 2010; 2 pgs.

Favorite Plus; Handheld ECG Monitor—Handheld EKG Monitor at Favoriteplus.com (Products: FP180, FP-RMH and FP-ICH); printed from website www.favoriteplus.com/handheld-ecg-ekg-monitor.php on Feb. 4, 2010; 3 pgs.

Favorite Plus; Handheld EKG Monitor InstantCheck; (Product ID: FP-ICH); printed from website <http://www.favoriteplus.com/instancheck-hand-held-ecg-ekg-monitor> on Feb. 4, 2010; 2 pgs.

Ferrick, M.D.; Holter Monitoring and Cardiac Event Recording in Assessing Symptomatic Patients; Albert Einstein College of Medicine; Bronx, New York; (no date); pp. 11-14; printed on or before Apr. 14, 2010.

Fulford-Jones, et al., A Portable, Low-Power, Wireless Two-Lead EKG System; Proc. of the 26th Ann. Int. Conf. IEEE EMBS; San Francisco, CA, USA; Sep. 1-5, 2004, pp. 2141-2144.

(56)

References Cited

OTHER PUBLICATIONS

- Gillette, M.D.; Diagnosis of Pediatric Arrhythmias with Event Recording; Medical University of South Carolina; Charleston, South Carolina; (no date); pp. 25-32; printed on or before Apr. 14, 2010.
- Grier, James W.; How to use 1-lead ECG recorders to obtain 12-lead resting ECGs and exercise ("stress") ECGs; printed from website <http://www.ndsu.edu/pubweb/grier> on Jun. 7, 2010; 13 pgs.
- Hannaford, Kat; How to Turn Your iPhone Into A Laser, Fan or Flashlight; printed from website <http://m.gizmodo.com/5534904>; printed Feb. 3, 2011.
- Hayes, M.D., Approaches to Diagnosing Transient Arrhythmias—An Overview; Mayo Clinic; Rochester, Minnesota; (no date); pp. 7-10; printed on or before Apr. 14, 2010.
- Hearing Loss Assoc. of Kentuckiana; Decibel Ratings/Hazardous Time Exposures of Common Noise (excerpt from Survivor's Manual); web version as of Oct. 5, 2008; 2 pgs.; printed Jun. 6, 2012 (<http://web.archive.org/web/20081005143856/http://www.hearinglossky.org/hlasurvival1.html>).
- Huang, Tina; Age-related hearing loss; Minnesota Medicine; 90(10); pp. 48-50; Oct. 2007; printed Jun. 6, 2012 from: <http://www.minnesotamedicine.com/PastIssues/PastIssues2007/October2007/ClinicalHuangOctober2007.aspx>).
- IMEC News; IMEC extends flexible ECG patch to enable arrhythmia detection; printed from website <http://www2.imec.be/imec> on Aug. 18, 2009; 1 pg.
- Instromedix; Cardiac Event Recording FAQs; Instromedix: A Card Guard Company, San Diego, CA; printed from website www.instromedix.com/pdf/products/cardiac; printed on or before Apr. 14, 2010.
- Instromedix; The Arrhythmia Monitoring System; King of Hearts Express AF Recorder Brochure; from Instromedix; A CardGuard Company; Rosemont IL; (year of publication is sufficiently earlier than the effective U.S. filing date and any foreign priority date) 2004; 3 pgs.
- iRHYTHM; Zio(TM) Patch; printed from website <http://www.irhythmtech.com/zio-solution/zio-pach/>; printed Apr. 12, 2010.
- Kim, et al., Detection of Atrial Fibrillation Episodes using Multiple Heart Rate Variability Features in Different Time Periods; Conf Proc IEEE Eng Med Biol Soc.; EMBS; 30th Ann. Int. Conf.; Aug. 20-25, 2008, 5482-5485.
- Koerner; The Author's Metrics; Wired Magazine Article; New York, NY; Jul. 2009; pp. 93-126.
- Kumarak, Greg; Visa officially announces their case that turns your iPhone into a credit card (and we've got pics!); May 17, 2010; www.mobilecrunch.com; printed Feb. 3, 2011.
- Leijdekkers et al., Trial Results of a Novel Cardiac Rhythm Management System using Smart Phones and Wireless ECG Sensors; Proc. of the 7th Int. Conf. on Smart homes and health Telematics., Tours, France; Jul. 1-3, 2009; 8 pgs.
- Levkov et al., Removal of power-line interference from the ECG: a review of the subtraction procedure; BioMedical Engineering Online; 4:50; Aug. 23, 2005; 18 pgs.; (printed from website <http://www.biomedical-engineeringonline.com/content/4/1/50>).
- M Med Choice; (company information page) Beijing Choice Electronic Technology Co., Ltd.; printed from website <http://www.choicemed.com/lxwm.asp>; printed Dec. 28, 2009; 1 page.
- M Med Choice; Handheld ECG Monitor Brochure; MD100 Products; Beijing Choice Electronic Technology Co. Ltd.; 6 pgs; published on or before Apr. 14, 2010.
- M Med Choice; Handheld ECG Monitor MD100A1; printed from website <http://www.choicemed.com/productshow.asp> on Dec. 28, 2009; 2 pgs.
- M Med Choice; Handheld ECG Monitor MD100B; printed from website <http://www.choicemed.com/productshow.asp> on Dec. 28, 2009; 2 pgs.
- Mauvila; Mauvila ECG Tutorial; Basic ECG Interpretation Tutorial; Sections 1-12; 2004; printed from website <http://mauvila.com/ECG/ecg.htm> on Mar. 26, 2010; 57 pgs.
- Medgadget; Zio(TM) Patch Wins Medical Design Award; MedGadget internet journal of emerging medical technologies; printed from website <http://medgadget.com/archives/2010/04/zio-patch-wins-medial-desian-award-1.html> on Apr. 12, 2010; 1 pg.
- MiCardioMobile: Remote Wireless Cardiac Rehabilitation Monitoring printed from website; <http://alivetec.cable.nu/cardiomobile>; 1 page; printed Apr. 14, 2010.
- Mobility Mind; Use your Treo 650 as a portable ECG monitoring device; Mobility Mind; Sep. 14, 2005, printed from website <http://www.treotoday.net/2005/09/14/use-your-treo-650-as-a-portable-ecg-monitoring-device/> (accessed Mar. 26, 2010); 1 pg.
- Modem Protocols Explained; <ftp://kermit.columbia.edu/kermit/cu/protocol.html>; 5 pgs.; printed Oct. 2, 2013.
- Modem Tutorial; <http://www.lsu.edu/OCS/its/unix/tutorial/ModemTutorial/ModemTutorial.html>; 2 pgs.; printed Oct. 2, 2013.
- Muench, Frederick PhD; HRV: The Manufacturers and Vendors Speak; The portable StressEraser Heart Rate Variability Biofeedback Device: Background and Research; Biofeedback; vol. 36, Iss. 1; pp. 35-39; Spring 2008.
- Murph; RedEye mini converts iPhone, iPad or iPod touch into IR-beaming universal remote; printed from website <http://www.engadget.com/2010/03/02/redeye> on Mar. 2, 2010; 2 pgs.
- Nam et al.; An Ultrasonic Sensor Based Low-Power Acoustic Modem for Underwater Communication in Underwater Wireless Sensor Networks; Computer Network Lab, Dept. of Elec. Eng., Korea Univ.; pp. 494-504; Dec. 2007 (http://nesl.ee.ucla.edu/fw/torres/home/Dropbox/good_paper_mico_controller.pdf); 11 pgs.; printed Oct. 2, 2013).
- Neuroreille; Audiometry; web version as of Oct. 14, 2008; 1 pg.; printed Jun. 6, 2012 (<http://www.neuroreille.com/promenade/english/audiometry/audiometry.htm>).
- Omron; Omron Portable ECG EKG Handheld HCG-801 Monitor; printed from website <http://www.amazon.com/Omron-Portable-Handheld-HCG-801-Monitor/dp/B0019WH3EO> on Feb. 24, 2010; 4 pgs.
- Omron; Omron Portable ECG Monitor; printed from website <http://www.target.com/gp/detail.html> on Mar. 26, 2010; 1 pg.
- Oresko, et al., Detecting Cardiovascular Diseases via Real-Time Electrocardiogram Processing on a Smartphone; 2009 Workshop on Biomedicine in Computing: Systems, Architectures, and Circuits (BiC); Austin, TX; Jun. 2009; pp. 13-16.
- Perez, Sarah; No NFC? No Problem; New Startup Zoosh Provides Workaround Technology (Jun. 20, 2011); printed on or before Jun. 27, 2011 from website; 2 pgs.; (<http://www.readwriteweb.com/archives>).
- Prystowsky, M.D., Chairmans Introduction; Duke University Medical Center; Indianapolis, Indiana; pp. 5-6; printed on or before Apr. 14, 2010.
- Prystowsky, M.D., Chairmans Summary; Duke University Medical Center; Indianapolis Indiana; (no date); pp. 39-40; printed on or before Apr. 14, 2010.
- Prystowsky, M.D., The Clinical Application, Diagnostic Yield and Cost Considerations of Cardiac Event Recorders; Duke University Medical Center; Indianapolis Indiana; (no date); pp. 19-23* printed on or before Apr. 14, 2010.
- Puurtinen, et al., Best Electrode Locations for a Small Bipolar ECG Device: Signal Strength Analysis of Clinical Data, Annals of Biomedical Engineering, vol. 37, No. 2, Feb. 2009; pp. 331-336.
- Raju; Heart-Rate and EKG Monitor Using the MSP430FG439 (Application Report); Texas Instruments; SLAA280-Oct. 2005-(Revised Sep. 2007); 11 pgs.
- Read-My-Heart; ECG Machine Handheld Read My Heart; (Product Item No. HH-3413); printed from website <http://www.helioliving.com/ECG-Machine-Handheld-ReadMyHeart> on Feb. 4, 2010; 1 pg.
- Read-My-Heart; ReadMyHeart Personal Handheld ECG Monitor with Free Illustrator Book & Free Electrodes V2.2; printed from website <http://www.amazon.com/Readmyheart-Personal-Handheld-illustrator-Electrodes/dp/B0010AN63W> on Mar. 26, 2010; 1 pg.
- Ricker; Square payment dongle demoed for iPhone toting hippies and you (video); printed from website <http://www.engadget.com/2010/01/18/square-payment> on Jan. 18, 2010; 6 pgs.

(56)

References Cited

OTHER PUBLICATIONS

- Rockwood; Interviews: The Networked Body Magazine Article from FAST TALK Magazine; Jul. 2009; pp. 19-26.
- Salahuddin, et al., Ultra Short Term Analysis of Heart Rate Variability using Normal Sinus Rhythm and Atrial Fibrillation ECG Data; e-Health Networking, App. and Services; 9th Int. Conf.; IEEE; Taipei, TW; pp. 240-243; Jun. 19-22, 2007.
- Semler, M.D.; The Future of Cardiac Event Monitoring; St. Vincent Hospital and Medical Center; Portland, Oregon; (no date); pp. 33-37; printed on or before Apr. 14, 2010.
- SFO Medical; Choice Portable Handheld ECG EKG Monitor; printed from website <http://www.amazon.com/Choice-Portable-Handheld-ECG-Monitor/dp/B001Q74VOM> on Mar. 26, 2010; 1 page.
- Shenzen New Element Med. Equipment; Wireless ECG Monitoring System; printed from website <http://www.alibaba.com/product-gs/248168581/Wireless-ECG-Monitoring-system.html>. On Mar. 26, 2010.
- Smith; Smartphone may keep the cardiologist away; The Independent; Mar. 5, 2010; printed from website <http://www.independent.co.uk/life-style/health-and-families/health-news/smartphone-may-keep-the-cardiologist-away-1916652.html> on Mar. 26, 2010.
- Stevens, Tim; Apple's Seamlessly Embedded Heart Rate Monitor could turn the iPhone into a new-age mood ring (posted May 6, 2010); printed from website www.engadget.com on May 6, 2010; 3 pgs.
- Taleb Medical; Observer Hand-held ECG Monitor MD100B; printed on or before Apr. 14, 2010.
- Tei, et al., New index of combined systolic and diastolic myocardial performance: a simple and reproducible measure of cardiac function—a study in normals and dilated cardiomyopathy; *J Cardiol.*; 26(6):357-366; Dec. 1995.
- Texas Instruments; Information for Medical Applications, Biophysical Monitoring—Electrocardiogram (ECG) Front End; Apr. 2004, pp. 17-18.
- Tschida (posted by); Power A's New Case Turns Your iPhone Into a Universal Remote; printed from website <http://appadvice.com/appnn> on Mar. 1, 2010; 2 pgs.
- Vanhemert, Kyle; XWave Headset Lets You Control iPhone Apps With Your BRAIN; Sep. 8, 2010; printed from website <http://gizmodo.com>; printed Sep. 8, 2010.
- FREE2MOVE; Vitaphone 2300; www.free2move.us/News/NewsVitaphone240105.htm; printed May 12, 2010; 2 pgs.
- Wikimedia Laboratories; Acoustics; web archive version dated Jan. 25, 2009; 2 pgs.; printed Jun. 6, 2012 (<http://liveweb.archive.org/http://en.labs.wikimedia.org/wiki/Acoustics>).
- Wikipedia; Aliasing; web version as of Apr. 3, 2011; 5 pgs.; printed Jun. 6, 2012 (<http://liveweb.archive.org/http://en.wikipedia.org/w/index.php?title=Aliasing&oldid=422141882>).
- Wikipedia; Hearing Range; web version as of Feb. 6, 2010; 5 pgs.; printed Jun. 6, 2012 (http://web.archive.org/web/20100206213741/http://en.wikipedia.org/wiki/Hearing_range).
- Wikipedia; Pulse oximetry; printed from website <http://en.wikipedia.org> on May 10, 2010, 4 pages.
- Wisneski, C.; Ultrasonic Local Area Communication; <http://alumni.media.mit.edu/~wiz/ultra.com.html>; 2 pgs.; printed Oct. 2, 2013.
- Woodward et al.; Bio-Potential-To-Frequency Converter/Modulator; *Electronic Design*; Aug. 9, 1999; p. 117.
- Ziegler, Chris; EPI Life phone sports ECG function, can let doctors know if you're not gonna make it; printed from website <http://www.engadget.com/2010/06/16/epi-life-phonesports> on Jun. 17, 2010; 4 pgs.
- Albert et al.; U.S. Appl. No. 13/969,446 entitled "Ultrasonic Transmission of Signals," filed Aug. 16, 2013.
- Albert, David E.; U.S. Appl. No. 14/015,303 entitled "Cardiac Performance Monitoring System for Use with Mobile Communications Devices," filed Aug. 30, 2013.
- Chinese Patent Application No. 2013800135500 First Office Action dated Oct. 20, 2015.
- Dinh. Heart activity monitoring on smartphone. IPCBEE-Int conf Biomedical Eng and Technol. Jun. 17-19, 2011. 11:45-49.
- Dolan; Qualcomm launches ECG smartphone program in China; Sep. 8, 2011; 11 pgs.; retrieved Mar. 19, 2014 from the internet (<http://mobihealthnews.com/13092/qualcomm-launches-ecg-smartphone-program-in-china/>).
- European search report and opinion dated Nov. 21, 2014 for EP Application No. 11865699.0.
- Garabelli et al. Accuracy and Novelty of an Inexpensive iPhone-based Event Recorder (Presentation Poster/Abstract) Heart Rhythm 2012, 33rd Annual Scientific Session. SP23. Innovation Poster Session II. No. IA02-1; May 11, 2012.
- GBI Portal. Qualcomm's wireless reach mHealth project to improve cardiovascular disease in resource scarce China; Feb. 17, 2012; 7 pgs. Retrieved Mar. 19, 2014 from www.intergrallc.com/2012/02/17/qualcooms-wireless-reach-mhealth-project-to-improve-cardiovascular-disease-in-resource-scarce-china/.
- Ge; Healthcare., "Marquette heart rate turbulence analysis program", 2005, DC-0160-12.05-EN-US. 4 pages.
- International preliminary report on patentability dated Jul. 29, 2014 for PCT/US2013/023370.
- International search report and written opinion dated Feb. 12, 2015 for PCT Application No. US2014/054414.
- International search report and written opinion dated Feb. 17, 2012 for PCT/US2011/039445.
- International search report and written opinion dated Apr. 27, 2012 for PCT/US2011/053708.
- International search report and written opinion dated Apr. 30, 2015 for PCT/US2014/070170.
- International search report and written opinion dated May 15, 2013 for PCT/US2013/023370.
- International search report and written opinion dated Dec. 17, 2013 for PCT/US2013/055458.
- International search report dated Sep. 1, 2014 for PCT/US2014/034350.
- Jenkins II, W.; Time/Frequency Relationships for an FFT-Based Acoustic Modem; Naval Postgraduate School; pp. 1-102; Sep. 2010 (http://edocs.nps.edu/npspubs/scholarly/theses/2010/Sep/1_OSEP_Jenkins.pdf) printed Oct. 2, 2013.
- Lau, et al. iPhone ECG application for community screening to detect silent atrial fibrillation: A novel technology to prevent stroke. *Int J Cardiol.* Apr. 30, 2013;165(1):193-4.
- Lau, et al. Performance of an Automated iPhone ECG Algorithm to Diagnose Atrial Fibrillation in a Community AF Screening Program (SEARCH-AF). *Heart, Lung and Circulation.* 2013; 22:S205.
- Lau et al. Validation of an iPhone ECG application suitable for community screening for silent atrial fibrillation—A novel way to prevent stroke (Presentation Abstract 16810); American Heart Association 2012 Scientific Sessions and Resuscitation Science Symposium; 126(1); Nov. 20, 2012, 2 pages.
- Lin; et al., "An intelligent telecardiology system using a wearable and wireless ECG to detect atrial fibrillation." 14(3), 726-33, 2010.
- Lowres, et al. Screening Education And Recognition in Community Pharmacies of Atrial Fibrillation to prevent stroke in an ambulant population aged =65 years (SEARCH-AF stroke prevention study): a cross-sectional study protocol. *BMJ Open.* Jun. 25, 2012; 2(3)e001355.
- New Professional Quality ECGEKG Portable Heart Monitor; printed from website <http://cgibay.com/ws/eBayISAPI.dll> printed on Feb. 4, 2010• 3 pages.
- Notice of allowance dated Jan. 8, 2014 for U.S. Appl. No. 14/015,303.
- Notice of allowance dated Jan. 27, 2014 for U.S. Appl. No. 14/015,303.
- Notice of allowance dated Feb. 26, 2014 for U.S. Appl. No. 14/015,303.
- Notice of allowance dated May 23, 2014 for U.S. Appl. No. 13/108,738.
- Notice of allowance dated Jul. 9, 2013 for U.S. Appl. No. 12/796,188.
- Notice of allowance dated Aug. 28, 2012 for U.S. Appl. No. 13/420,520.

(56)

References Cited

OTHER PUBLICATIONS

Notice of allowance dated Dec. 4, 2013 for U.S. Appl. No. 14/015,303.

Office action dated Jan. 2, 2014 for U.S. Appl. No. 13/108,738.

Office action dated Jun. 18, 2012 for U.S. Appl. No. 13/420,520.

Office action dated Sep. 12, 2014 for U.S. Appl. No. 13/108,738.

Office action dated Oct. 6, 2014 for U.S. Appl. No. 14/252,044.

Office action dated Oct. 29, 2012 for U.S. Appl. No. 12/796,188.

Office action dated Nov. 19, 2014 for U.S. Appl. No. 13/969,446.

PCT/US2014/054414 International Preliminary Report on Patentability mailed Mar. 17, 2016.

Saxon, et al. iPhone rhythm strip—the implications of wireless and ubiquitous heart rate monitoring. *JACC*; 59(13): E726; Mar. 2012.

Saxon. Ubiquitous Wireless ECG Recording: A Powerful Tool Physicians Should Embrace. *J Cardiovasc Electrophysiol*. 24(4): pp. 480-483; Apr. 2013.

Shumaker, J.; Designing an Ultrasonic Modem for Robotic Communications; Army Research Laboratory; 26 pgs.; Mar. 2009 (<http://www.dtic.mil/cgi-bin/GetTRDoc?AD=ADA499556>) printed Oct. 2, 2013.

U.S. Appl. No. 13/752,048 Office Action dated May 18, 2015.

U.S. Appl. No. 14/730,122 Office Action dated Feb. 24, 2016.

U.S. Appl. No. 14/730,122 Office Action dated Jun. 13, 2016.

Carpenter and Frontera, Smart-watches: a potential challenger to the implantable loop recorder? *Europace*, 18:791-793, 2016.

European Patent Application No. 11793020.6 extended European Search Report dated Jan. 10, 2017.

European Patent Application No. 11865699.0 Communication dated Dec. 19, 2016.

European Patent Application No. 14785223.0 extended European Search Report dated Aug. 23, 2016.

Japanese Patent Application No. 2014-511335 Decision of Rejection dated Jul. 28, 2016.

Japanese Patent Application No. 2014-554916 Office Action dated Sep. 26, 2016.

Notice of Allowance issued Mar. 29, 2016 for U.S. Appl. No. 14/254,310.

Office Action dated Aug. 25, 2015 for U.S. Appl. No. 14/479,105.

PCT Patent Application No. PCT/US2014/070170 International Preliminary Report on Patentability dated Jun. 23, 2016.

PCT/US2016/032524 International Search Report and Written Opinion dated, Aug. 19 2016.

U.S. Appl. No. 14/479,105 Office Action dated Jul. 22, 2016.

U.S. Appl. No. 14/494,191 Office Action dated Jul. 20, 2016.

U.S. Appl. No. 14/730,122 Notice of Allowance mailed Dec. 6, 2016.

U.S. Appl. No. 15/140,072 Office Action dated Dec. 23, 2016.

* cited by examiner

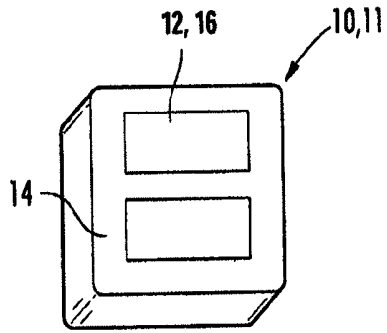


FIG. 1

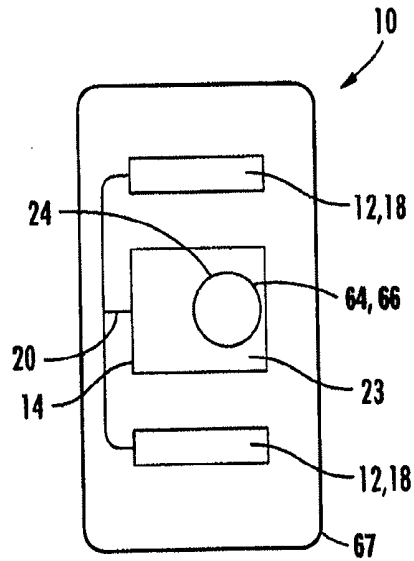


FIG. 2

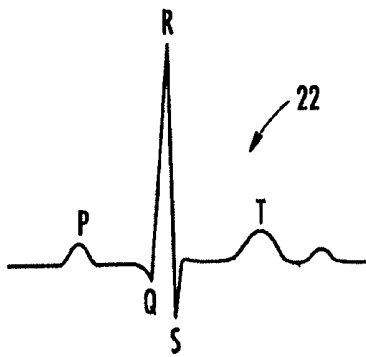


FIG. 3

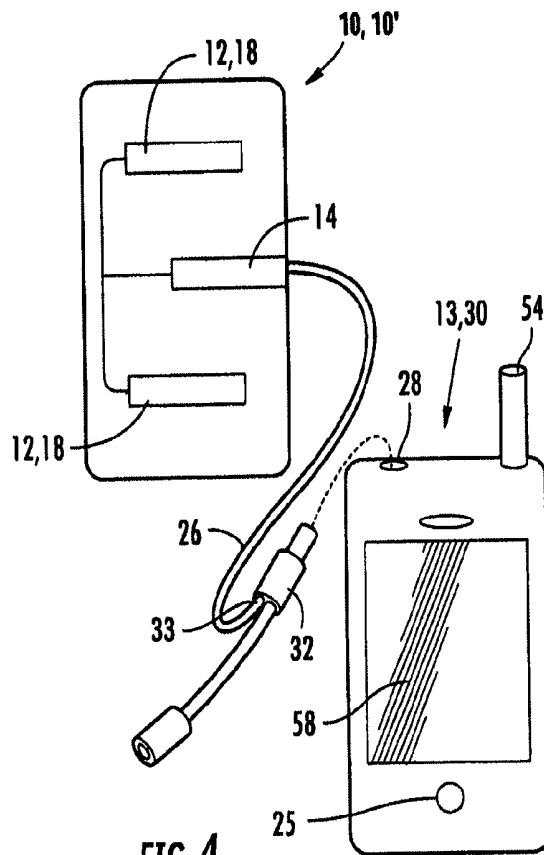


FIG. 4

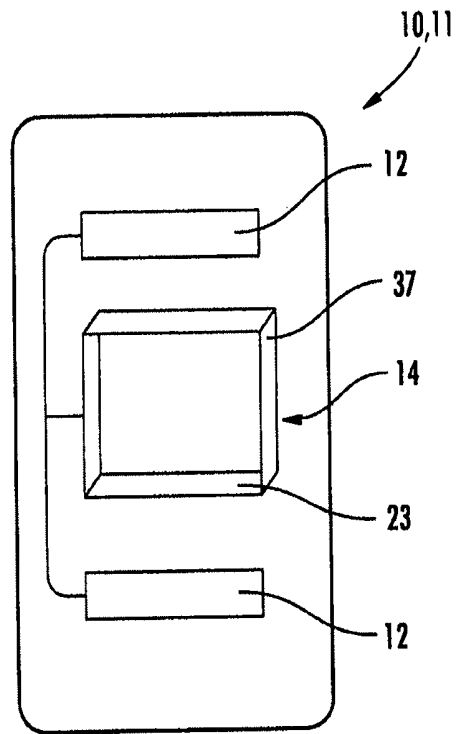


FIG. 5

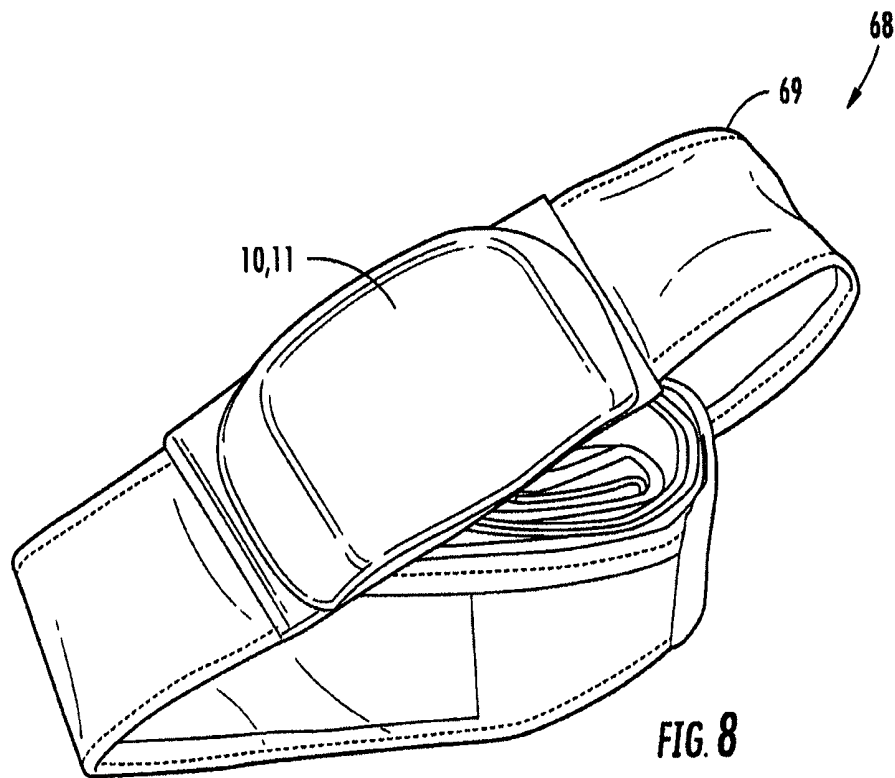


FIG. 8

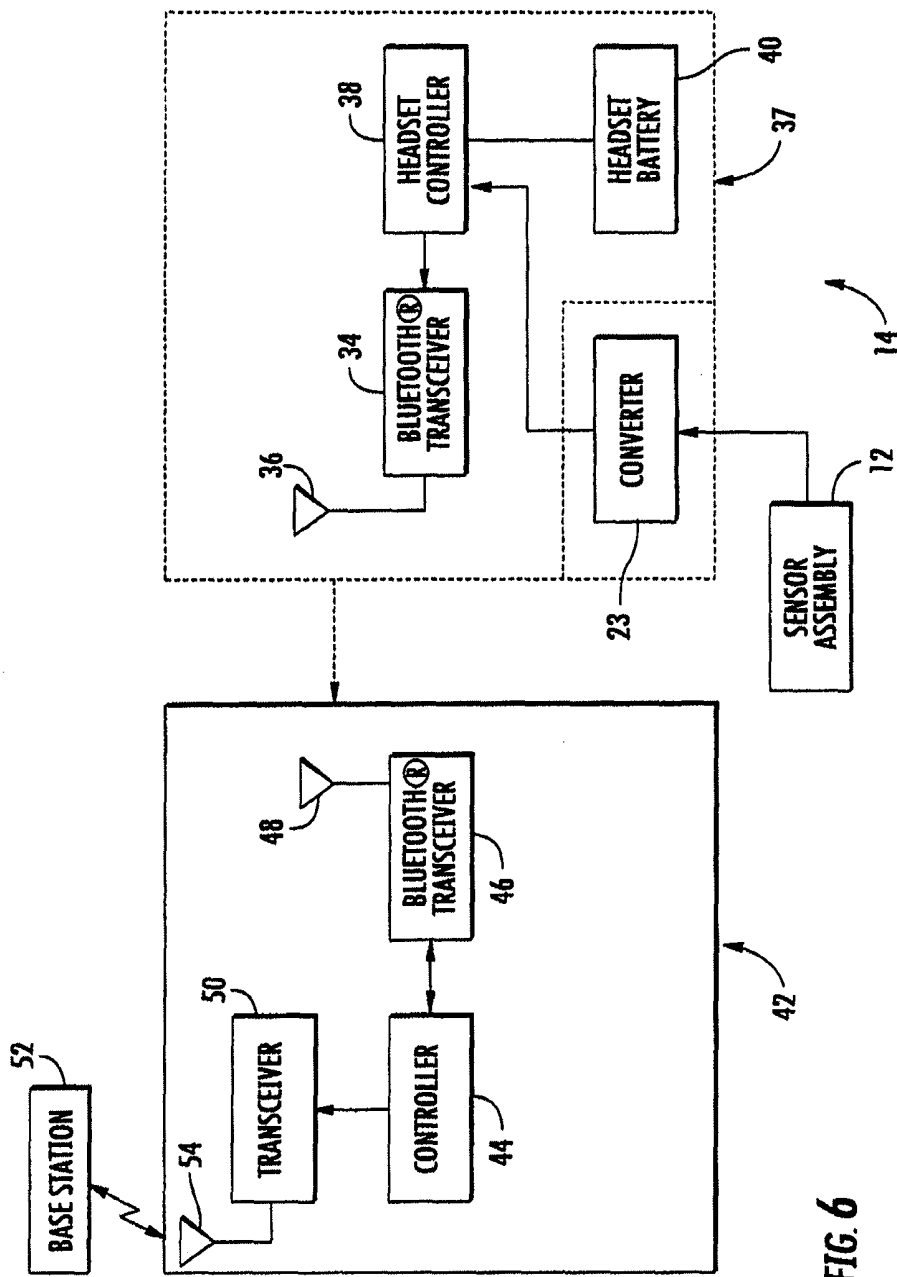


FIG. 6

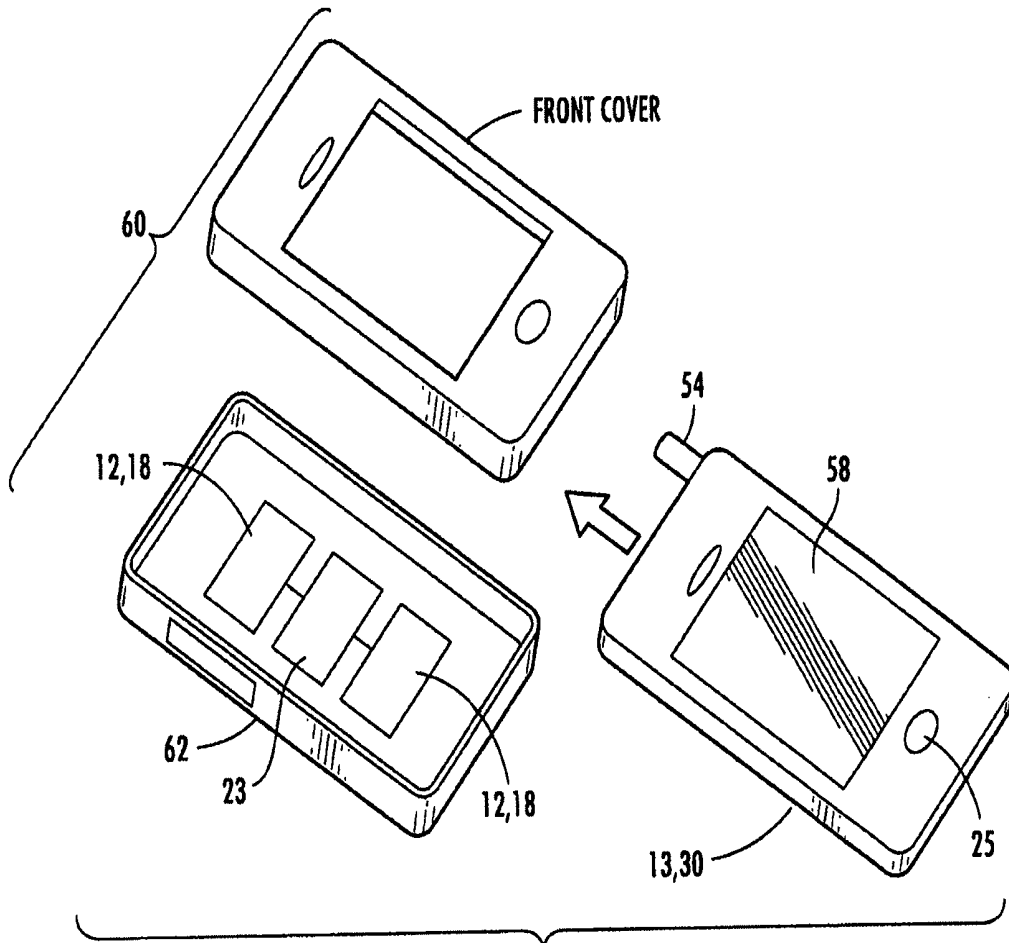


FIG. 7

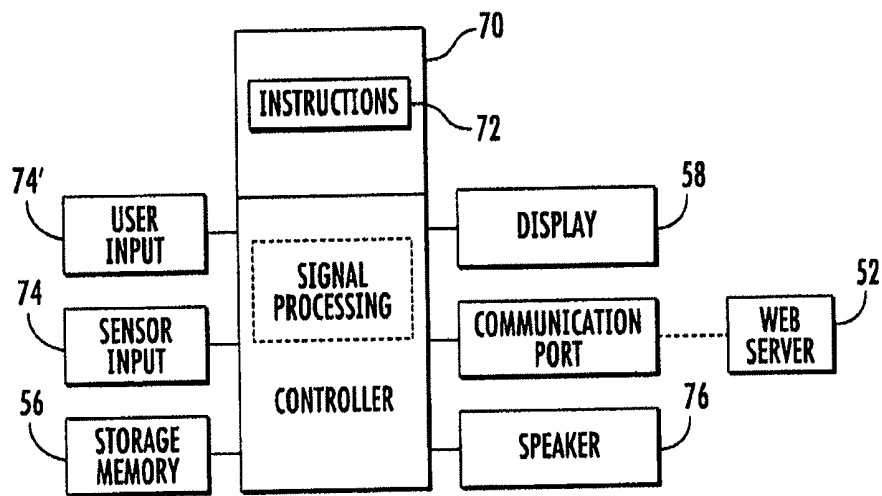


FIG. 9

**HEART MONITORING SYSTEM USABLE
WITH A SMARTPHONE OR COMPUTER****CROSS REFERENCE TO RELATED
APPLICATIONS**

This application is a divisional of U.S. patent application Ser. No. 12/796,188 (now U.S. Pat. No. 8,509,882), filed Jun. 8, 2010, titled "HEART MONITORING SYSTEM USABLE WITH A SMARTPHONE OR COMPUTER," Publication No. US-2011-0301435-A1, which is herein incorporated by reference in its entirety.

INCORPORATION BY REFERENCE

All publications and patent applications mentioned in this specification are herein incorporated by reference to the same extent as if each individual publication or patent application was specifically and individually indicated to be incorporated by reference.

**STATEMENT REGARDING FEDERALLY
SPONSORED RESEARCH OR DEVELOPMENT**

Not applicable.

BACKGROUND**1. Field of Invention**

The presently claimed and disclosed inventive concept(s) relates generally to personal physiology monitoring devices and methods and, more particularly, but not by way of limitation, to devices, systems and software for providing ECG, heart rate and cardiac arrhythmia monitoring utilizing a computing device such as a smartphone.

2. Background of the Invention

The prior art includes numerous systems wherein ECG data or the like is monitored and/or transmitted from a patient to a particular doctor's office or health service center. For example, U.S. Pat. No. 5,735,285 discloses use of a handheld device that converts a patient's ECG signal into a frequency modulated audio signal that may then be analyzed by audio inputting via a telephone system to a selected handheld computer device or to a designated doctor's office. Similarly, U.S. Pat. No. 6,264,614 discloses a heart monitor, which is manipulated by the patient to sense a biological function such as a heart beat, and outputs an audible signal to a computer microphone. The computer processes the audible signal and sends resulting data signals over a network or Internet. U.S. Pat. No. 6,685,633 discloses a heart monitor that a patient can hold against his or her chest. The device outputs an audible signal responsive to the function or condition, such as the beating of the heart, to a microphone connected to a computer.

U.S. Pat. App. Publication No. 20100113950 discloses an electronic device having a heart sensor including several leads for detecting a user's cardiac signals. The leads are coupled to interior surfaces of the electronic device housing to hide the sensor from view. Using the detected signals, the electronic device can then identify or authenticate the user.

Limitations of the prior art utilizing acoustic signals include a signal to noise ratio that is diminished by talking or any other noisy activity in the vicinity, thus potentially jeopardizing the integrity of the heart monitoring data signals. Additionally, the audible signals can be heard by anyone in the vicinity of the computer and heart monitor, which can be bothersome to the user as well as to others in

the vicinity. Other applications fail to provide a reliable, inexpensive personal monitoring device that is readily compatible with existing computing devices such as smartphones. It would be advantageous if these issues were addressed in a personal monitoring device transmitting real time physiological data.

SUMMARY OF THE INVENTION

Embodiments of the presently claimed and disclosed invention are directed to a personal monitoring device having a sensor assembly configured to sense physiological signals upon contact with a user's skin. The sensor assembly produces electrical signals representing the sensed physiological signals. A converter assembly, integrated with, and electrically connected to the sensor assembly, converts the electrical signals generated by the sensor assembly to a frequency modulated physiological audio signal. In one embodiment, the frequency modulated physiological audio signal has a carrier frequency in the range of from about 6 kHz to about 20 kHz.

In another embodiment, the personal monitoring device includes a cable connected to the converter assembly for transmitting the frequency modulated physiological audio signal to a 3.5 mm headphone jack on a smartphone, wherein the converter assembly is electrically isolated from the smartphone by an audio isolation transformer. In this case, the frequency modulated physiological audio signal has a carrier frequency in the range of from about 1 kHz to about 20 kHz.

In yet another embodiment, the personal monitoring device includes a wireless radio transmitter configured to utilize Bluetooth® headset technology to transmit the frequency modulated physiological audio signal, having a carrier frequency in the range of from about 1 kHz to about 20 kHz, to a Bluetooth® enabled computing device.

An ECG device of the presently claimed and disclosed inventive concept(s) includes an electrode assembly configured to sense heart-related signals upon contact with a user's skin, and to convert the sensed heart-related signals to an ECG electric signal. A converter assembly, integrated with, and electrically connected to the electrode assembly, is configured to convert the electric ECG signal generated by electrode assembly to a frequency modulated ECG audio signal having a carrier frequency in the range of from about 6 kHz to about 20 kHz.

In one embodiment, a smartphone protective case, usable as an ECG device, is provided. An electrode assembly, configured to sense heart-related signals upon contact with a user's skin, and to convert the sensed heart-related signals to an ECG electric signal, is provided. A converter assembly, integrated with, and electrically connected to the electrode assembly, is configured to convert the electric ECG signal generated by the electrode assembly to a frequency modulated ECG audio signal having a carrier frequency in the range of from about 6 kHz to about 20 kHz, and further configured to output the ECG audio signal through an audio transmitter at a signal strength capable of being received by a smartphone positioned within the smartphone protective case.

In a second embodiment, an ECG device is provided in a housing having an electrode assembly configured to sense heart-related signals upon contact with a user's skin, and to convert the sensed heart-related signals to an ECG electric signal. A converter assembly integrated with, and electrically connected to the electrode assembly, is configured to convert the electric ECG signal generated by electrode

assembly to a frequency modulated ECG audio signal having a carrier frequency in the range of from about 6 kHz to about 20 kHz, and further configured to output the ECG audio signal through an audio transmitter at a signal strength capable of being received by a smartphone located near the ECG device.

In another embodiment, an ECG device is provided having an electrode assembly configured to sense heart-related signals upon contact with a user's skin, and to convert the sensed heart-related signals to an ECG electric signal. A converter assembly integrated with, and electrically connected to the electrode assembly, is configured to convert the electric ECG signal generated by electrode assembly to a frequency modulated ECG audio signal. A cable is provided for transmitting the frequency modulated ECG audio signal to a 3.5 mm headphone jack on a smartphone, wherein the converter assembly is electrically isolated from the smartphone by an audio isolation transformer.

In yet another embodiment, a computer-readable storage medium is provided for storing a set of instructions capable of being executed by one or more computing devices, causing the one or more computing devices to digitize and demodulate a frequency modulated ECG audio signal having a carrier frequency in the range of from about 6 kHz to about 20 kHz to produce real time demodulated digital ECG data, and to display on a display screen of the computing device, the real time ECG signal represented by the demodulated digital ECG data.

Thus, utilizing (1) the technology known in the art; (2) the above-referenced general description of the presently claimed and disclosed inventive concept(s); and (3) the detailed description of the invention that follows, the advantages and novelties of the presently claimed and disclosed inventive concept(s) would be readily apparent to one of ordinary skill in the art.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a schematic representation of an embodiment of a personal monitoring device of the present invention.

FIG. 2 is a schematic representation of another embodiment of a personal monitoring device of the present invention.

FIG. 3 is an example of graphical ECG representation.

FIG. 4 is a schematic representation of an embodiment wherein a personal monitoring device includes an audio cable that can input to a smartphone.

FIG. 5 is a schematic representation of an embodiment of an ECG device of the present invention utilizing a wireless radio transmitter.

FIG. 6 is a schematic representation of an embodiment of a personal monitoring device of the present invention connecting via Bluetooth® to a computing device.

FIG. 7 is a schematic representation of an embodiment of a personal monitoring device of the present invention.

FIG. 8 is a schematic representation of an embodiment of an ECG device of the present invention included positioned within a chest strap.

FIG. 9 is a schematic representation of a computer-readable storage medium embodiment of the present invention.

DETAILED DESCRIPTION OF THE INVENTION

Before explaining at least one embodiment of the invention in detail, it is to be understood that the invention is not

limited in its application to the details of construction, experiments, exemplary data, and/or the arrangement of the components set forth in the following description. The invention is capable of other embodiments or of being practiced or carried out in various ways. Also, it is to be understood that the terminology employed herein is for purpose of description and should not be regarded as limiting.

The presently claimed and disclosed inventive concepts provide a personal monitoring device **10**, embodiments of which are shown schematically in FIGS. 1 and 2. The acquisition electronics **11** of the monitoring device **10** includes a sensor assembly **12** configured to sense physiological signals upon contact with a user's skin. The sensor assembly **12** produces electrical signals representing the sensed physiological signals, which input to a converter assembly **14**, integrated with the sensor assembly **12**. Converter assembly **14** converts the electrical signals generated by the sensor assembly **12** to a frequency modulated physiological audio signal having a carrier frequency in the range of from about 1 kHz to about 20 kHz. In one embodiment, the frequency modulated physiological audio signal has a carrier frequency in the range of from about 6 kHz to about 20 kHz.

The sensor assembly **12** can include any suitable sensor operative to detect a physiological signal that a user desires to monitor. Nonlimiting examples of such physiological signals include, but are not limited to, respiration, heart beat, heart rate, electrocardiogram (ECG), electromyogram (EMG), electrooculogram (EOG), pulse oximetry, photoplethysmogram (PPG) and electroencephalogram (EEG).

A respiration detector can be a conventional microphone assisted stethoscope **16**. Heart beat and heart rate can be detected as well using a conventional microphone assisted stethoscope **16**, or by using an electrode assembly **18** to sense electrical signals generated by the heart over time. Such electrodes **18** can also be used to detect the electrical activity of the heart over time for electrocardiography (ECG). An ECG is a measurement of the small electrical changes on the skin generated when the heart muscle depolarizes during each heart beat. The output from a pair of electrodes **18** is known as a lead **20**. Small rises and falls in the voltage between two electrodes placed on either side of the heart can be processed to produce a graphical ECG representation **22** such as the example ECG shown in FIG. 3.

Electromyography (EMG) detects the electrical potential generated by muscle cells when the cells are electrically or neurologically activated. The signals can be analyzed to detect medical abnormalities. Electrooculography (EOG) is a technique for measuring the resting potential of the retina. Usually, pairs of electrodes **18** are placed either above and below the eye, or to the left and right of the eye, and a potential difference measurement is a measure for the eye position.

The oxygenation of a person's hemoglobin can be monitored indirectly in a noninvasive manner using a pulse oximetry sensor, rather than measuring directly from a blood sample. The sensor is placed on a thin part of the person's body, such as a fingertip or earlobe, and a light containing both red and infrared wavelengths is passed from one side to the other. The change in absorbance of each of the two wavelengths is measured and the difference used to estimate oxygen saturation of a person's blood and changes in blood volume in the skin. A photoplethysmogram (PPG) can then be obtained using the pulse oximeter sensor or with an optical sensor using a single light source. The PPG can be

used to measure blood flow and heart rate. An electroencephalogram (EEG) can be monitored using electrodes attached to the scalp and measures voltages generated by brain activity.

The converter assembly **14** converts the electrical signals generated by the sensor assembly **12** to a frequency modulated physiological audio signal that can be received by a computing device **13**. In the embodiment shown in FIG. **2**, the converter assembly **14** includes a converter **23** and an audio transmitter **24** for outputting frequency modulated physiological signals having a carrier frequency in the range of from about 6 kHz to about 20 kHz as frequency modulated acoustic signals. Nonlimiting examples of suitable audio transmitters **24** include, but are not limited to, miniature speakers, piezoelectric buzzers, and the like. The acoustic signals can be received by, for example, a microphone **25** in a computing device **13** such as a smartphone, personal digital assistant (PDA), tablet personal computer, pocket personal computer, notebook computer, desktop computer, server computer, and the like.

Prior art devices have used frequency modulated physiological signals to communicate between acquisition hardware and a computing device. The signals have a carrier frequency within the audible range such as the traditional 1.9 kHz FM frequency used to transmit ECG signals. However, it has been discovered that by using “high frequency” audio frequencies as the carrier, such as frequencies in the range of from about 6 kHz to about 20 kHz, the acoustic communication between the acquisition electronics **11** of the personal monitoring device **10**, and a computing device **13** such as a smartphone, is virtually silent and far more noise-immune than the traditional 1.9 kHz FM ECG frequency. In fact, measurements of the audio signal power in the 1.5 kHz to 15 kHz range determined that carrier frequencies of 6 kHz and higher provide communication that is immune to ambient and voice “noise” contamination. Also, by using a carrier frequency in the 10 kHz to 15 kHz range, we create both a lower noise and a silent communication between the acquisition electronics **11** and the computing device **13** or smartphone. An additional reason for using high carrier frequencies, such as in the 6 kHz to 15 kHz range or in the 10 kHz to 15 kHz range, is to allow simultaneous recording of voice and physiological signals over a single audio channel, where voice and the FM signal are in different frequency bands that can be filtered and separated. The clinical applications of this embodiment can include fast and inexpensive cardiac rhythm diagnosis for physicians as well as personal ECG acquisition for patients.

In another embodiment, such as that shown in FIG. **4**, the converter assembly **14** is configured to convert the electrical signals generated by the sensor assembly **12** to a frequency modulated physiological audio signal which is transmitted by a cable **26** to a 3.5 mm headphone jack **28** on a smartphone **30**. This configuration is totally silent and immune to ambient acoustic noise. In this embodiment the converter assembly **14** is electrically isolated from the smartphone **30** by an audio isolation transformer **32**. The audio isolation transformer **32** preferably conforms to medical safety performance standards such as, for example, those outlined in IEC 60601 along with national and regional deviations. The cable **26** for transmitting the frequency modulated ECG audio signal to the 3.5 mm headphone jack **28** on the smartphone **30** can include a splitter **33** configured, as understood by those skilled in the art, to allow the user to listen to music and voice messages while transmitting the frequency modulated ECG audio signal. The splitter **33** can also allow the user to utilize a mic or headset to record

spoken voice messages, such as comments and notes regarding physical symptoms, simultaneously with the ECG audio signal. Using a high carrier frequency of around 10 kHz, or in the 6 kHz to 20 kHz range, allows simultaneous recording of voice and physiological signals over a single audio channel, where the voice and the frequency modulated signal are in different frequency bands that can be readily filtered and separated.

In yet another embodiment, shown in FIGS. **5** and **6**, the converter assembly **14** includes a wireless radio transmitter **37** configured to convert and transmit the electrical signals generated by the sensor assembly **12** using a headset profile (HSP) of the Bluetooth® wireless communications standard is defined by the Bluetooth Special Interest Group (SIG) and available at URL address www.bluetooth.org. The electrical signals generated by the sensor assembly **12** are converted and transmitted using a Bluetooth® transceiver **34** and antenna **36** and communicated to the computing device **13**, preferably a smartphone **30**, according to instructions provided by a headset controller **38**. Economy, as well as isolation and convenience, are provided by using a commercially available headset controller **38**, Bluetooth® transceiver **34**, and antenna **36**, powered by a headset battery **40**, wherein the electronics are commercially configured and mass-produced for communicating with computing devices **13** such as smartphones **30**.

Computing device electronics **42** typically include a controller **44**, a Bluetooth® transceiver **46** and antenna **48** for receiving input from a wireless Bluetooth® device. Most computing devices, and all smartphones, include a memory **56**, a display screen **58**, and a transceiver **50** for transmitting/receiving information signals to/from a base station or web server **52** via a cellular antenna **54**. Thus, the computing device electronics **42** can be used to store information from the personal monitoring device **10** in memory **56**, and/or transmit the information to the base station **52** or a specific communication address via wireless communication technology well understood by those skilled in the art.

In some cases, the personal monitoring device **10** can be considered an ECG device **10'** and includes an electrode assembly **18** configured to sense heart-related signals upon contact with a user's skin, and to convert the sensed heart-related signals to an ECG electric signal. As discussed in detail hereinafter, the ECG device **10'** transmits a frequency modulated ECG audio signal to a smartphone **30** via a wired audio jack connection, a wireless headset, or acoustically. Software running on the smartphone **30** digitizes and processes the audio in real-time, where the frequency modulated ECG signal is demodulated. The ECG can be further processed using algorithms to calculate heart rate and identify arrhythmias. The ECG, heart rate, and rhythm information can be displayed on the smartphone **30**, stored locally for later retrieval, and/or transmitted in real-time to a web server **52** via a 2G/3G, WiFi or other Internet connection on the smartphone **30**. In addition to the display and local processing of the ECG data, the smartphone **30** can transmit, in real-time, the ECG, heart rate and rhythm data via a secure web connection for viewing, storage and further analysis via a web browser interface (using the 2G/3G or WiFi connectivity of the smartphone **30**). Server software provides for storage, further processing, real-time or retrospective display and formulation of a PDF ECG rhythm strip document and/or other reports and formats for printing remotely or locally.

In one embodiment, the converter assembly **14** of ECG device **10'** is integrated with, and electrically connected to the electrode assembly **18** and is configured to convert the

electric ECG signal generated by electrode assembly 18 to a frequency modulated ECG audio signal having a carrier frequency in the range of from about 6 kHz to about 20 kHz. It is sometimes desirable to utilize a carrier frequency in the 10 kHz to 15 kHz range in order to create both a lower noise and a silent communication between the acquisition electronics 11 and the computing device 13 or smartphone 30.

In one configuration, the ECG device 10' is usable as a smartphone protective case 60 as shown in FIG. 7. One example configuration utilizes a "slip-on" protective case 60 for an iPhone® or other smartphone 30, the protective case 60 including an integrated ECG electrode assembly 18 and acquisition electronics 11 (2, 3 or 4 electrodes for generating a single lead of ECG data). The ECG electrodes are located on the side 62 of the case 60 opposite of the display screen 58. The smartphone 30, in its ECG-adapted protective case 60, is held in both hands (generating a lead one, Left Arm minus Right Arm) or is placed on a person's chest to generate a modified chest lead. The ECG is measured by the acquisition electronics 11 and converted into a frequency modulated signal with a carrier or center frequency from about 6 kHz to 20 kHz, or in some embodiments from 10 kHz to 15 kHz. The frequency modulated signal is output by a miniature speaker 64 or a piezoelectric buzzer 66.

In another configuration, the ECG device 10', as shown schematically in FIG. 2, is usable as a standalone real-time ECG acquisition device. The ECG device is identical to the "case" electronics, but is present in its own housing 67 rather than being integrated into a protective case 60 for a smartphone 30. This embodiment allows for use of the device to acquire ECG data and have it communicated acoustically to a PC or other computing device for demodulation, processing, storage and display via a web application and connection.

In either configuration, the smartphone 30 utilizes its built-in microphone 25 and CPU to acquire, digitize, demodulate, process and then display the ECG data in real-time. Also, the smartphone 30 can calculate a real-time heart rate measurement and determine a cardiac rhythm diagnosis like atrial fibrillation. The smartphone 30 can utilize its 2G, 3G, Bluetooth® and WiFi connectivity to transmit the ECG and other data to a secure web server 52 for real-time distant display, storage and analysis. Also, the ECG data can be stored locally on the smartphone 30 for later review or transmission.

In another embodiment, shown schematically in FIG. 8, the ECG device 10' is usable as a chest strap device 68 like a fitness heart rate monitor. The chest strap 69 with integrated ECG electrode assembly 18 and acquisition electronics 11 "pod" generate the frequency modulated ECG signal and send it by one of two modes to the smartphone 30. In one mode, a cable 26, as described above, plugs into the 3.5 mm headphone jack 28 on the iPhone®, Blackberry® or other smartphone 30 which provides an audio input (normally used for a headphone mic). This configuration is totally silent and immune to ambient acoustic noise. The ECG data is isolated from the smartphone 30 by an audio isolation transformer 32. In another mode, the frequency modulated audio signal is transmitted by a Bluetooth® headset chip, as described above, and the smartphone 30 receives it and performs the other processing steps. This configuration preferably makes use of mass-produced headset electronics and includes a rechargeable battery. This configuration is wireless, which provides isolation and convenience.

Software on the smartphone 30 can also combine data and signals from other sensors built into the smartphone 30 such

as a GPS and accelerometer. Further processing of this data provides additional information related to the user, such as speed, location, distance, steps, cadence, body position, fall detection and energy expenditure. The raw signals from the sensors and derived information can be displayed and stored locally on the smartphone 30, as well as being transmitted to the web server 52 over an Internet connection. Software on the web server 52 provides a web browser interface for real-time or retrospective display of the signals and information received from the smartphone 30, and also includes further analysis and reporting.

Referring now to FIG. 9, a computer-readable storage medium 56 stores a set of instructions 72, wherein the instructions 72 are capable of being executed by one or more computing devices 13. Nonlimiting examples of suitable computing devices 13 include smartphones 30, personal digital assistants (PDAs), tablet personal computers, pocket personal computers, notebook computers, desktop computers, and server computers. When executed, the one or more computing devices 13 is caused to digitize and demodulate a sensor input 74 such as a frequency modulated ECG audio signal having a carrier frequency in the range of from about 6 kHz to about 20 kHz to produce real-time demodulated digital ECG data. The instructions 72 can cause the real-time demodulated digital ECG data to display on a display screen 58 of the computing device 13.

Sensor input 74 can also include real-time information from additional sensors as well as user input 74'. For example, in embodiments wherein the computing device 13 is a smartphone 30, the input 74 can include real-time information from a GPS and/or accelerometer in the smartphone 30 in addition to the demodulated digital ECG data. User input 74' can also include spoken voice messages entered through a microphone of the computing device 13. Instructions 72 can cause the sensor and/or user input 74 and 74' to be recorded and maintained in a storage memory 56 of the computing device 13.

In one embodiment, the set of instructions 72, when executed by the one or more computing devices 13, can further cause the one or more computing devices 13 to calculate and display in real-time, a heart rate represented by the frequency modulated ECG audio signal. In addition, demodulated digital ECG data can be processed to identify the occurrence of an arrhythmia. In such designs, the storage medium 70 can include instructions 72 to cause the computing device 13 to display a warning on a display screen 58 or emit an audible alert through the speaker 76 at the occurrence of an arrhythmia.

Instructions 72 can cause the computing device 13 to store the demodulated digital ECG data in a memory 56 of the one or more computing devices 13 for later retrieval. The set of instructions 72 can further cause the one or more computing devices 13 to retrieve and transmit, upon demand, the stored demodulated digital ECG data to a web server 52 via an internet connection on the computing device 13. Recorded spoken voice messages can be stored and transmitted to the web server 52, simultaneously with the demodulated digital ECG data.

In other embodiments, the instructions 72 can cause the one or more computing devices 13 to transmit the demodulated digital ECG data, and/or voice messages, to the web server 52 in real-time.

A version of the smartphone software is packaged as a software library that can be integrated with other third party software applications. This provides a simplified and standard method for third party applications to use the ECG device 10' to obtain heart rate and other derived information

without having to develop their own data acquisition, demodulation, and signal processing algorithms.

A version of the software also runs on a PC and includes demodulation, processing, storage and transmission to the web server 52. The software includes the audio acquisition, demodulation, ECG analysis, and acceleration analysis modules.

The audio acquisition module selects the appropriate audio input and samples the audio. On the iPhone®, audio is sampled and processed using the audio unit framework, which provides low latency audio acquisition and processing. The audio unit framework also allows automatic selection of the appropriate audio source, internal mic, audio jack connection, or Bluetooth® headset. The sampling rate will typically be at 44 kHz when the modulation carrier frequency is greater than 10 kHz, but for lower carrier frequencies, it may use a lower audio sampling rate. On other devices this module will use the most appropriate API's for efficient, low latency audio sampling.

The demodulation module demodulates a frequency modulated ECG audio signal, using a linear approximation and zero crossings algorithm. The demodulator allows selection of different modulation parameters to match the particular ECG device. Demodulation using zero crossings and linear approximation works well for carrier frequencies 6 kHz and lower and has the advantage that it is simple and fast. Above 10 kHz with 44 kHz sampling, the errors from linear approximation become large, although the effect is somewhat reduced if applying a 40 Hz filter to the demodulated ECG. Application of sine or other curve fitting methods can be used to reduce the error associated with linear approximation for carrier frequencies above 10 kHz. Audio samples from the audio acquisition module are first passed through a digital band-pass filter to remove unwanted frequencies outside the modulation range. The digital band-pass filter is most effective when receiving acoustically coupled audio which can be contaminated with noise. When using a center frequency above 6 kHz, the band-pass filter is able to provide good noise immunity from voice and background ambient noise which is typically below 5 kHz. The band-pass filter stage could be eliminated to save processing power when receiving audio via a wired or Bluetooth® connection which would not be susceptible to background noise contamination. To demodulate the signal it is necessary to estimate the frequency of the audio waveform. The algorithm looks at the sign of incoming data. When the sign changes it draws a straight line between the two points and interpolates the zero value. It uses this to determine the average frequency over a 3.333 ms interval, which provides ECG data at the output sampling rate of 300 Hz.

The ECG analysis module includes algorithms that process the ECG to detect and classify beats, and provides a heart rate estimate. Beat-to-beat heart rate is calculated from the interval between beats and a more robust measurement of heart rate is calculated using median filtering of the RR intervals.

The acceleration analysis module includes algorithms that process signals from the built-in 3 axis accelerometer sensor in the smartphone 30, to derive an estimate of a person's energy expenditure, steps, cadence, and body position and to detect falls.

From the above descriptions, it is clear that the presently disclosed and claimed inventive concept(s) are well-adapted to carry out the objects and to attain the advantages mentioned herein, as well as those inherent in the presently disclosed and claimed inventive concept(s). While the presented embodiments have been described for purposes of

this disclosure, it will be understood that numerous changes may be made which will readily suggest themselves to those skilled in the art and which are accomplished within the spirit of the presently disclosed and claimed inventive concept(s).

What is claimed is:

1. An ECG device comprising:

- a computing device comprising a display;
- an electrode assembly configured to sense heart-related signals upon contact with a user's skin, and to convert the sensed heart-related signals to an ECG signal; and
- a converter assembly integrated with, and electrically connected to the electrode assembly, the converter assembly configured to convert the ECG signal generated by the electrode assembly to a frequency modulated ECG audio signal having a carrier frequency in the range of from about 6 kHz to about 20 kHz;
- a transmitter configured to transmit the frequency modulated ECG audio signal having a carrier frequency in the range of from about 6 kHz to about 20 kHz to the computing device;
- a housing containing the electrode assembly, the converter assembly, and the transmitter, and configured to couple the electrode assembly, the converter assembly, and the transmitter to a surface of the computing device; and

wherein the computing device is configured to receive the frequency modulated ECG audio signal having a carrier frequency in the range of from about 6 kHz to about 20 kHz and display an ECG signal on the display.

2. The ECG device of claim 1, wherein the frequency modulated ECG audio signal has a carrier frequency in the range of from about 10 kHz to about 15 kHz.

3. The ECG device of claim 1, wherein the electrode assembly comprises two electrodes.

4. The ECG device of claim 1, wherein the transmitter is a speaker.

5. The ECG device of claim 1, wherein the transmitter is a piezoelectric buzzer.

6. The ECG device of claim 1, wherein the transmitter is configured to output the ECG signal to a microphone in the computing device.

7. The ECG device of claim 6, wherein the computing device is selected from the group consisting of smartphones, personal digital assistants (PDAs), tablet personal computers, pocket personal computers, notebook computers, desktop computers, and server computers.

8. The ECG device of claim 1, wherein the housing comprises a smartphone protective case.

9. The ECG device of claim 1, wherein the frequency modulated ECG audio signal has a carrier frequency in the range of from about 10 kHz to about 15 kHz.

10. The ECG device of claim 1, wherein the computing device comprises an accelerometer.

11. The ECG device of claim 10, wherein the computing device comprises:

- a processor; and
- a non-transitory computer readable storage medium encoded with a computer program including instructions configured to cause the processor to receive data from the accelerometer; and determine an energy expenditure.

12. The ECG device of claim 10, wherein the computing device comprises:

a processor; and

a non-transitory computer readable storage medium encoded with a computer program including instructions configured to cause the processor to receive data from the accelerometer; and determine a body position. 5

13. The ECG device of claim 1, wherein the ECG device comprises a microphone assisted stethoscope. 10

14. The ECG device of claim 1, wherein the computing device is configured to display the ECG signal in real time.

* * * * *

专利名称(译)	心脏监测系统可用于智能手机或计算机		
公开(公告)号	US9649042	公开(公告)日	2017-05-16
申请号	US13/964490	申请日	2013-08-12
[标]申请(专利权)人(译)	ALBERT DAVID 英维思楼宇系统RICHARD BRUCE 巴尼特KIM NORMAN		
申请(专利权)人(译)	ALBERT, DAVID 英维思楼宇系统, BRUCE RICHARD 巴尼特KIM NORMAN		
当前申请(专利权)人(译)	ALIVECOR INC.		
[标]发明人	ALBERT DAVID SATCHWELL BRUCE RICHARD BARNETT KIM NORMAN		
发明人	ALBERT, DAVID SATCHWELL, BRUCE RICHARD BARNETT, KIM NORMAN		
IPC分类号	A61B5/04 A61B5/0404 A61B5/00 A61B5/0402 A61B5/055		
CPC分类号	A61B5/0402 A61B5/0404 A61B5/6898 A61B5/055 A61B2505/07 A61B2560/045 A61B2560/0468 A61B5/0205 A61B5/02416 A61B5/02438 A61B5/04085 A61B5/0476 A61B5/0488 A61B5/0816 A61B5/742		
审查员(译)	MORAN, EDWARD		
其他公开文献	US20130331663A1		
外部链接	Espacenet USPTO		

摘要(译)

个人监测设备具有传感器组件，该传感器组件被配置为在与用户的皮肤接触时感测生理信号。传感器组件产生表示所感测的生理信号的电信号。与传感器组件集成并电连接的转换器组件将由传感器组件产生的电信号转换成频率调制的生理音频信号，其载波频率在约6kHz至约20kHz的范围内。

