



US009931077B2

(12) **United States Patent**  
**Kaula et al.**

(10) **Patent No.:** **US 9,931,077 B2**  
 (45) **Date of Patent:** **\*Apr. 3, 2018**

(54) **SYSTEM AND METHODS FOR  
 DETERMINING NERVE PROXIMITY,  
 DIRECTION AND PATHOLOGY DURING  
 SURGERY**

(58) **Field of Classification Search**  
 CPC . A61B 5/4893; A61B 5/04001; A61B 5/0488;  
 A61B 5/04836; A61B 17/00;  
 (Continued)

(71) Applicant: **NuVasive, Inc.**, San Diego, CA (US)

(56) **References Cited**

(72) Inventors: **Norbert F. Kaula**, Arvada, CO (US);  
**Jeffrey J. Blewett**; **James Gharib**, San  
 Diego, CA (US); **Allen Farquhar**

U.S. PATENT DOCUMENTS

208,227 A 9/1878 Dorr  
 509,226 A 11/1893 Kellogg  
 (Continued)

(73) Assignee: **NuVasive, Inc.**, San Diego, CA (US)

FOREIGN PATENT DOCUMENTS

(\*) Notice: Subject to any disclaimer, the term of this  
 patent is extended or adjusted under 35  
 U.S.C. 154(b) by 0 days.

This patent is subject to a terminal dis-  
 claimer.

DE 299 08 259 7/1999  
 DE 100 48 790 4/2002  
 (Continued)

(21) Appl. No.: **15/258,434**

OTHER PUBLICATIONS

(22) Filed: **Sep. 7, 2016**

Anatomy of the Lumbar Spine in MED TM MicroEndoscopic  
 Discectomy (1997 Ludann Grand Rapids MI), 14 pgs.

(65) **Prior Publication Data**

(Continued)

US 2016/0374613 A1 Dec. 29, 2016

**Related U.S. Application Data**

*Primary Examiner* — Catherine Voorhees

(60) Continuation of application No. 14/687,745, filed on  
 Apr. 15, 2015, now Pat. No. 9,456,783, which is a  
 (Continued)

(74) *Attorney, Agent, or Firm* — Rory Schermerhorn;  
 NuVasive, Inc.


(51) **Int. Cl.**  
**A61B 5/00** (2006.01)  
**A61B 5/04** (2006.01)  
 (Continued)

(57) **ABSTRACT**

The present invention involves systems and methods for  
 determining nerve proximity, nerve direction, and pathology  
 relative to a surgical instrument based on an identified  
 relationship between neuromuscular responses and the  
 stimulation signal that caused the neuromuscular responses.

(52) **U.S. Cl.**  
 CPC ..... **A61B 5/4893** (2013.01); **A61B 5/04001**  
 (2013.01); **A61B 5/0488** (2013.01);  
 (Continued)

**18 Claims, 15 Drawing Sheets**

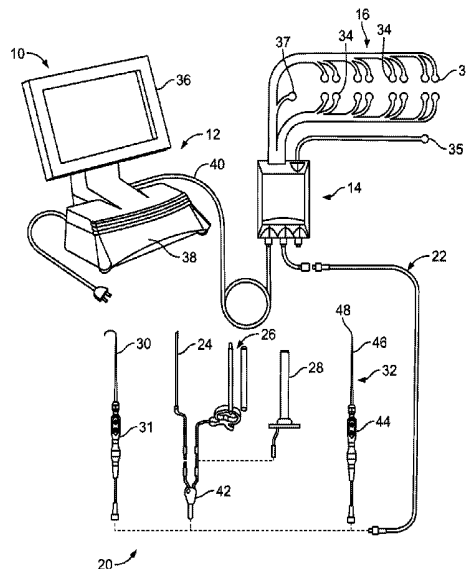

**Related U.S. Application Data**

continuation of application No. 13/767,355, filed on Feb. 14, 2013, now Pat. No. 9,037,250, which is a continuation of application No. 13/465,666, filed on May 7, 2012, now Pat. No. 8,812,116, which is a continuation of application No. 13/292,065, filed on Nov. 8, 2011, now Pat. No. 8,634,904, which is a continuation of application No. 13/080,493, filed on Apr. 5, 2011, now Pat. No. 8,055,349, which is a division of application No. 12/711,937, filed on Feb. 24, 2010, now Pat. No. 7,920,922, which is a continuation of application No. 10/754,899, filed on Jan. 9, 2004, now Pat. No. 8,068,912, which is a continuation of application No. PCT/US02/22247, filed on Jul. 11, 2002.

- (60) Provisional application No. 60/305,041, filed on Jul. 11, 2001.

(51) **Int. Cl.**

*A61B 5/0488* (2006.01)  
*A61N 1/08* (2006.01)  
*A61N 1/36* (2006.01)  
*A61B 17/00* (2006.01)  
*A61B 17/02* (2006.01)  
*A61B 5/11* (2006.01)

(52) **U.S. Cl.**

CPC ..... *A61B 5/4836* (2013.01); *A61B 17/00* (2013.01); *A61B 17/02* (2013.01); *A61N 1/08* (2013.01); *A61N 1/36* (2013.01); *A61B 5/1106* (2013.01); *A61B 5/7217* (2013.01); *A61B 5/743* (2013.01); *A61B 2017/00039* (2013.01)

(58) **Field of Classification Search**

CPC ..... *A61B 17/02*; *A61B 2017/00039*; *A61B 5/1106*; *A61B 5/743*; *A61N 1/08*; *A61N 1/36*

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

972,983	A	10/1910	Arthur	4,291,705	A	9/1981	Severinghaus et al.
1,003,232	A	10/1910	Cerbo	4,449,532	A	5/1984	Storz
1,044,348	A	6/1912	Cerbo	4,461,300	A	7/1984	Christensen
1,328,624	A	1/1920	Graham	4,512,351	A	4/1985	Pohndorf
1,548,184	A	8/1925	Cameron	4,515,168	A	5/1985	Chester et al.
1,919,120	A	7/1933	O'Connor et al.	4,519,403	A	5/1985	Dickhudt
2,594,086	A	4/1952	Smith	4,545,373	A	10/1985	Christoudias
2,704,061	A	3/1955	Amspacker	4,545,374	A	10/1985	Jacobson
2,704,064	A	3/1955	Fizzell et al.	4,561,445	A	12/1985	Berke et al.
2,736,002	A	2/1956	Oriel	4,562,832	A	1/1986	Wilder et al.
2,808,826	A	10/1957	Reiner et al.	4,573,448	A	3/1986	Kambin
2,840,082	A	6/1958	Salvatore	4,592,369	A	6/1986	Davis et al.
3,364,929	A	1/1968	Ide et al.	4,595,013	A	6/1986	Jones et al.
3,664,329	A	5/1972	Naylor	4,595,018	A	6/1986	Rantala
3,682,162	A	8/1972	Colyer	4,611,597	A	9/1986	Kraus
3,740,839	A	6/1973	Otte et al.	4,616,635	A	10/1986	Caspar et al.
3,785,368	A	1/1974	McCarthy et al.	4,633,889	A	1/1987	Talalla
3,803,716	A	4/1974	Garnier	4,658,835	A	4/1987	Pohndorf
3,830,226	A	8/1974	Staub et al.	D295,445	S	4/1988	Freeman
3,957,036	A	5/1976	Normann	4,744,371	A	5/1988	Harris
D245,789	S	9/1977	Shea et al.	4,753,223	A	6/1988	Bremer
4,099,519	A	7/1978	Warren	4,759,377	A	7/1988	Dykstra
4,164,214	A	8/1979	Stark et al.	4,784,150	A	11/1988	Voorhies et al.
4,207,897	A	6/1980	Lloyd et al.	4,807,642	A	2/1989	Brown
4,224,949	A	9/1980	Scott et al.	D300,561	S	4/1989	Asa et al.
4,226,228	A	10/1980	Shin et al.	4,817,587	A	4/1989	Janese
4,226,288	A	10/1980	Collins, Jr.	4,892,105	A	1/1990	Prass
4,235,242	A	11/1980	Howson et al.	4,913,134	A	4/1990	Luque
4,285,347	A	8/1981	Hess	4,917,274	A	4/1990	Asa et al.
				4,917,704	A	4/1990	Frey et al.
				4,926,865	A	5/1990	Oman
				4,945,896	A	8/1990	Gade
				4,950,257	A	8/1990	Hibbs et al.
				4,962,766	A	10/1990	Herzon
				4,964,411	A	10/1990	Johnson et al.
				5,007,902	A	4/1991	Witt
				5,015,247	A	5/1991	Michelson
				5,045,054	A	9/1991	Hood et al.
				5,052,373	A	10/1991	Michelson
				5,058,602	A	10/1991	Brody
				5,081,990	A	1/1992	Deletis
				5,092,344	A	3/1992	Lee
				5,127,403	A	7/1992	Brownlee
				5,161,533	A	11/1992	Prass et al.
				5,171,279	A	12/1992	Mathews
				5,178,133	A	1/1993	Pena
				5,190,561	A	3/1993	Graber
				5,192,327	A	3/1993	Brantigan
				5,195,541	A	3/1993	Obenchain
				5,196,015	A	3/1993	Neubardt
				5,215,100	A	6/1993	Spitz et al.
				5,231,974	A	8/1993	Giglio et al.
				RE34,390	E	9/1993	Culver
				D340,521	S	10/1993	Heinzelman et al.
				5,255,691	A	10/1993	Otten
				5,261,918	A	11/1993	Phillips et al.
				5,282,468	A	2/1994	Klepinski
				5,284,153	A	2/1994	Raymond et al.
				5,284,154	A	2/1994	Raymond et al.
				5,295,994	A	3/1994	Bonutti
				5,299,563	A	4/1994	Seton
				5,312,417	A	5/1994	Wilk
				5,313,956	A	5/1994	Knutsson et al.
				5,313,962	A	5/1994	Obenchain
				5,327,902	A	7/1994	Lemmen
				5,331,975	A	7/1994	Bonutti
				5,333,618	A	8/1994	Lekhtman et al.
				5,342,384	A	8/1994	Sugarbaker
				5,357,983	A	10/1994	Mathews
				5,375,067	A	12/1994	Berchin
				5,375,594	A	12/1994	Cueva
				5,383,876	A	1/1995	Nardella
				5,395,317	A	3/1995	Kambin
				5,425,772	A	6/1995	Brantigan
				5,433,739	A	7/1995	Sluijter et al.
				5,450,845	A	9/1995	Alexgaard
				5,458,638	A	10/1995	Kuslich et al.
				5,472,426	A	12/1995	Bonati et al.
				5,474,057	A	12/1995	Makower et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

5,474,558 A	12/1995	Neubardt	5,993,474 A	11/1999	Ouchi
5,480,440 A	1/1996	Kambin	6,004,262 A	12/1999	Putz et al.
5,482,038 A	1/1996	Ruff	6,004,312 A	12/1999	Finneran
5,484,437 A	1/1996	Michelson	6,004,326 A	12/1999	Castro et al.
5,487,739 A	1/1996	Aebischer et al.	6,007,487 A	12/1999	Foley et al.
5,509,893 A	4/1996	Pracas	6,008,433 A	12/1999	Stone
5,514,153 A	5/1996	Bonutti	6,010,520 A	1/2000	Pattison
5,540,235 A	7/1996	Wilson	6,015,436 A	1/2000	Schonhoffer
5,545,222 A	8/1996	Bonutti	6,024,696 A	2/2000	Hoftman et al.
5,549,656 A	8/1996	Reiss	6,024,697 A	2/2000	Pisarik
5,560,372 A	10/1996	Cory	6,027,456 A	2/2000	Feler et al.
5,562,736 A	10/1996	Ray et al.	6,033,405 A	3/2000	Winslow et al.
5,566,678 A	10/1996	Cadwell	6,036,638 A	3/2000	Nwawka
5,569,290 A	10/1996	McAfee	6,038,469 A	3/2000	Karlsson et al.
5,571,149 A	11/1996	Liss et al.	6,038,477 A	3/2000	Kayyali
5,579,781 A	12/1996	Cooke	6,039,761 A	3/2000	Li et al.
5,593,429 A	1/1997	Ruff	6,042,582 A	3/2000	Ray
5,599,279 A	2/1997	Slotman et al.	6,045,580 A	4/2000	Scarborough et al.
5,630,813 A	5/1997	Kieturakis	6,048,342 A	4/2000	Zucherman et al.
5,653,761 A	8/1997	Pisharodi	6,050,992 A	4/2000	Nichols
5,653,762 A	8/1997	Pisharodi	6,059,829 A	5/2000	Schlapfer et al.
5,667,508 A	9/1997	Errico et al.	6,063,088 A	5/2000	Winslow
5,669,909 A	9/1997	Zdeblick et al.	6,074,343 A	6/2000	Nathanson et al.
5,671,752 A	9/1997	Sinderby et al.	6,080,105 A	6/2000	Spears
5,681,265 A	10/1997	Maeda et al.	6,083,154 A	7/2000	Liu et al.
5,688,223 A	11/1997	Rosendahl	6,083,225 A	7/2000	Winslow et al.
5,707,359 A	1/1998	Bufalini	6,095,987 A	8/2000	Schmulewitz
5,711,307 A	1/1998	Smits	6,096,080 A	8/2000	Nicholson et al.
5,716,415 A	2/1998	Steffee	6,104,957 A	8/2000	Alo et al.
5,720,751 A	2/1998	Jackson	6,104,960 A	8/2000	Duysens et al.
5,728,046 A	3/1998	Mayer et al.	6,113,638 A	9/2000	Williams et al.
5,728,159 A	3/1998	Stroever et al.	6,120,503 A	9/2000	Michelson
5,741,253 A	4/1998	Michelson	6,120,506 A	9/2000	Kohrs et al.
5,741,261 A	4/1998	Moskovitz et al.	6,126,660 A	10/2000	Dietz
5,759,159 A	6/1998	Masreliez	6,132,386 A	10/2000	Gozani et al.
5,762,629 A	6/1998	Kambin	6,132,387 A	10/2000	Gozani et al.
5,766,252 A	6/1998	Henry et al.	6,135,965 A	10/2000	Turner et al.
5,772,661 A	6/1998	Michelson	6,139,493 A	10/2000	Koros et al.
5,775,331 A	7/1998	Raymond et al.	6,142,931 A	11/2000	Kaji
5,776,144 A	7/1998	Leysieffer et al.	6,146,335 A	11/2000	Gozani
5,779,642 A	7/1998	Nightengale	6,152,871 A	11/2000	Foley et al.
5,785,658 A	7/1998	Benaron	6,159,179 A	12/2000	Simonson
5,792,044 A	8/1998	Foley et al.	6,159,211 A	12/2000	Boriani et al.
5,797,854 A	8/1998	Hedgecock	6,159,215 A	12/2000	Urbahns et al.
5,797,909 A	8/1998	Michelson	6,159,230 A	12/2000	Samuels
5,800,550 A	9/1998	Sertich	6,161,047 A	12/2000	King et al.
5,813,978 A	9/1998	Jako	6,174,311 B1	1/2001	Branch et al.
5,814,073 A	9/1998	Bonutti	6,181,961 B1	1/2001	Prass
5,814,084 A	9/1998	Grivas et al.	6,187,000 B1	2/2001	Davison et al.
5,830,151 A	11/1998	Hadzic et al.	6,193,756 B1	2/2001	Studer et al.
5,851,191 A	12/1998	Gozani	6,196,969 B1	3/2001	Bester et al.
5,851,208 A	12/1998	Trott	6,200,347 B1	3/2001	Anderson et al.
5,853,373 A	12/1998	Griffith et al.	6,206,826 B1	3/2001	Mathews et al.
5,860,973 A	1/1999	Michelson	6,206,922 B1	3/2001	Zdeblick et al.
5,862,314 A	1/1999	Jeddeloh	6,217,509 B1	4/2001	Foley et al.
5,865,845 A	2/1999	Thalgott	6,224,545 B1	5/2001	Cocchia et al.
5,872,314 A	2/1999	Clinton	6,224,549 B1	5/2001	Drongelen
5,885,210 A	3/1999	Cox	6,224,607 B1	5/2001	Michelson
5,885,219 A	3/1999	Nightengale	6,224,631 B1	5/2001	Kohrs
5,888,196 A	3/1999	Bonutti	6,241,771 B1	6/2001	Gresser et al.
5,888,224 A	3/1999	Beckers et al.	6,245,082 B1	6/2001	Gellman et al.
5,891,147 A	4/1999	Moskovitz et al.	6,251,140 B1	6/2001	Marino et al.
5,893,890 A	4/1999	Pisharodi	6,258,125 B1	7/2001	Paul et al.
5,902,231 A	5/1999	Foley et al.	6,259,945 B1	7/2001	Epstein et al.
5,910,315 A	6/1999	Stevenson et al.	6,264,651 B1	7/2001	Underwood et al.
5,928,139 A	7/1999	Koros et al.	6,266,558 B1	7/2001	Gozani et al.
5,928,158 A	7/1999	Aristides	6,273,905 B1	8/2001	Streeter
5,931,777 A	8/1999	Sava	6,277,149 B1	8/2001	Boyle et al.
5,935,131 A	8/1999	Bonutti et al.	6,292,701 B1	9/2001	Prass et al.
5,938,688 A	8/1999	Schiff	6,306,100 B1	10/2001	Prass
5,944,658 A	8/1999	Koros et al.	6,308,712 B1	10/2001	Shaw
5,954,769 A	9/1999	Rosenlicht	6,312,392 B1	11/2001	Herzon
5,968,098 A	10/1999	Winslow	6,319,257 B1	11/2001	Carignan et al.
5,976,094 A	11/1999	Gozani et al.	6,325,764 B1	12/2001	Griffith et al.
5,976,146 A	11/1999	Ogawa et al.	6,334,068 B1	12/2001	Hacker
			6,348,058 B1	2/2002	Melkent et al.
			6,360,750 B1	3/2002	Gerber et al.
			6,371,968 B1	4/2002	Kogasaka et al.
			6,371,989 B1	4/2002	Chauvin et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

6,383,221 B1	5/2002	Scarborough et al.	7,166,113 B2	1/2007	Arambula et al.
6,395,007 B1	5/2002	Bhatnagar et al.	7,177,677 B2	2/2007	Kaula et al.
6,409,766 B1	6/2002	Brett	7,198,598 B2	4/2007	Smith et al.
6,416,465 B2	7/2002	Brau	7,207,949 B2	4/2007	Miles et al.
6,425,859 B1	7/2002	Foley et al.	7,226,451 B2	6/2007	Shluzas et al.
6,425,887 B1	7/2002	McGuckin et al.	7,261,688 B2	8/2007	Smith et al.
6,425,901 B1	7/2002	Zhu et al.	7,470,236 B1	12/2008	Kelleher et al.
6,432,048 B1	8/2002	Francois	7,473,222 B2	1/2009	Dewey et al.
6,432,140 B1	8/2002	Lin	7,481,766 B2	1/2009	Lee et al.
6,440,142 B1	8/2002	Ralph et al.	7,522,953 B2	4/2009	Kaula et al.
6,442,814 B1	9/2002	Landry et al.	7,556,601 B2	7/2009	Branch et al.
6,450,952 B1	9/2002	Rioux et al.	7,582,058 B1	9/2009	Miles et al.
6,451,015 B1	9/2002	Rittman, III et al.	7,643,884 B2	1/2010	Pond et al.
6,454,806 B1	9/2002	Cohen et al.	7,691,057 B2	4/2010	Miles et al.
6,466,817 B1	10/2002	Kaula et al.	7,693,562 B2	4/2010	Marino et al.
6,468,205 B1	10/2002	Mollenauer et al.	7,717,959 B2	5/2010	William et al.
6,468,207 B1	10/2002	Fowler, Jr.	7,819,801 B2	10/2010	Miles et al.
6,468,311 B2	10/2002	Boyd et al.	7,892,173 B2	2/2011	Miles et al.
6,491,724 B1	12/2002	Ferree	7,905,840 B2	3/2011	Pimenta et al.
6,500,116 B1	12/2002	Knapp	7,918,891 B1	4/2011	Curran et al.
6,500,128 B2	12/2002	Marino	7,920,922 B2	4/2011	Kaula et al.
6,520,907 B1	2/2003	Foley et al.	7,935,051 B2	5/2011	Miles et al.
6,524,320 B2	2/2003	DiPoto	7,962,191 B2	6/2011	Marino et al.
6,535,759 B1	3/2003	Epstein et al.	7,963,927 B2	6/2011	Kelleher et al.
D472,634 S	4/2003	Anderson	7,991,463 B2	8/2011	Kelleher et al.
D472,650 S	4/2003	Green	8,000,782 B2	8/2011	Gharib et al.
6,564,078 B1	5/2003	Marino et al.	8,005,535 B2	8/2011	Gharib et al.
6,579,244 B2	6/2003	Goodwin	8,016,767 B2	9/2011	Miles et al.
6,595,998 B2	7/2003	Johnson et al.	8,021,430 B2	9/2011	Michelson
6,599,294 B2	7/2003	Fuss et al.	8,055,349 B2	11/2011	Kaula et al.
6,620,157 B1	9/2003	Dabney et al.	8,068,912 B2 *	11/2011	Kaula ..... A61B 5/0488 600/554
6,626,905 B1	9/2003	Schmiel et al.	8,114,019 B2	2/2012	Miles et al.
6,635,086 B2	10/2003	Lin	8,133,173 B2	3/2012	Miles et al.
6,645,194 B2	11/2003	Briscoe et al.	8,137,284 B2	3/2012	Miles et al.
6,648,895 B2	11/2003	Burkus et al.	8,172,750 B2	5/2012	Miles et al.
6,672,019 B1	1/2004	Wenz et al.	8,182,423 B2	5/2012	Miles et al.
6,676,703 B2	1/2004	Biscup	8,187,179 B2	5/2012	Miles et al.
6,679,833 B2	1/2004	Smith et al.	8,187,334 B2	5/2012	Curran et al.
6,706,067 B2	3/2004	Shimp et al.	8,192,356 B2	6/2012	Miles et al.
6,719,692 B2	4/2004	Kleffner et al.	8,192,357 B2	6/2012	Miles et al.
6,746,484 B1	6/2004	Liu et al.	8,244,343 B2	8/2012	Gharib et al.
6,755,841 B2	6/2004	Fraser et al.	8,246,686 B1	8/2012	Curran et al.
6,760,616 B2	7/2004	Hoey et al.	8,251,997 B2	8/2012	Michelson
6,761,739 B2	7/2004	Shepard	8,303,458 B2	11/2012	Fukano et al.
6,770,074 B2	8/2004	Michelson	8,303,498 B2	11/2012	Miles et al.
6,796,985 B2	9/2004	Bolger et al.	8,303,515 B2	11/2012	Pimenta et al.
6,810,281 B2	10/2004	Brock et al.	8,337,410 B2	12/2012	Kelleher et al.
6,819,956 B2	11/2004	DiLorenzo	8,343,046 B2	1/2013	Miles et al.
6,824,564 B2	11/2004	Crozet	8,343,224 B2	1/2013	Lynn et al.
6,829,508 B2	12/2004	Schulman et al.	8,355,780 B2	1/2013	Miles et al.
6,830,570 B1	12/2004	Frey et al.	8,361,156 B2	1/2013	Curran et al.
6,847,849 B2	1/2005	Mamo et al.	8,388,527 B2	3/2013	Miles
6,849,047 B2	2/2005	Goodwin	8,403,841 B2	3/2013	Miles et al.
6,855,105 B2	2/2005	Jackson, III et al.	8,439,832 B2	5/2013	Miles et al.
6,869,398 B2	3/2005	Obenchain	8,489,170 B2	7/2013	Marino et al.
6,871,099 B1	3/2005	Whitehurst et al.	8,500,634 B2	8/2013	Miles et al.
D503,801 S	4/2005	Jackson	8,512,235 B2	8/2013	Miles et al.
6,902,569 B2	6/2005	Parmer et al.	8,523,768 B2	9/2013	Miles et al.
6,916,330 B2	7/2005	Simonson	8,548,579 B2	10/2013	Gharib et al.
6,926,728 B2	8/2005	Zucherman et al.	8,550,994 B2	10/2013	Miles et al.
6,929,606 B2	8/2005	Ritland	8,556,808 B2	10/2013	Miles et al.
6,942,698 B1	9/2005	Jackson	8,562,521 B2	10/2013	Miles et al.
6,945,933 B2	9/2005	Branch	8,574,301 B2	11/2013	Curran et al.
6,951,538 B2	10/2005	Ritland	8,591,432 B2	11/2013	Pimenta et al.
6,964,687 B1	11/2005	Bernard et al.	8,602,982 B2	12/2013	Miles et al.
6,979,353 B2	12/2005	Bresina	8,608,804 B2	12/2013	Curran et al.
6,984,245 B2	1/2006	McGahan et al.	8,628,469 B2	1/2014	Miles et al.
6,986,788 B2	1/2006	Paul et al.	8,634,904 B2 *	1/2014	Kaula ..... A61B 5/0488 600/546
6,989,031 B2	1/2006	Michelson	8,663,100 B2	3/2014	Miles et al.
7,018,416 B2	3/2006	Hanson et al.	8,672,840 B2	3/2014	Miles et al.
7,047,082 B1	5/2006	Schrom et al.	8,673,005 B1	3/2014	Pimenta et al.
7,050,848 B2	5/2006	Hoey et al.	8,679,006 B2	3/2014	Miles et al.
7,079,883 B2	7/2006	Marino et al.	8,685,105 B2	4/2014	Curran et al.
7,089,059 B1	8/2006	Pless	8,696,559 B2	4/2014	Miles et al.
D530,423 S	10/2006	Miles et al.	8,708,899 B2	4/2014	Miles et al.
			8,738,123 B2	5/2014	Gharib et al.
			8,740,783 B2	6/2014	Gharib et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

8,747,307 B2 6/2014 Miles et al.  
 8,753,270 B2 6/2014 Miles et al.  
 8,753,271 B1 6/2014 Miles et al.  
 8,764,649 B2 7/2014 Miles et al.  
 8,768,450 B2 7/2014 Gharib et al.  
 8,780,899 B2 7/2014 Tillman et al.  
 8,812,116 B2 8/2014 Kaula et al.  
 8,814,940 B2 8/2014 Curran et al.  
 8,821,396 B1 9/2014 Miles et al.  
 8,915,846 B2 12/2014 Miles et al.  
 8,942,801 B2 1/2015 Miles et al.  
 8,945,004 B2 2/2015 Miles et al.  
 8,956,283 B2 2/2015 Miles et al.  
 8,958,869 B2 2/2015 Kelleher et al.  
 8,977,352 B2 3/2015 Gharib et al.  
 9,014,776 B2 4/2015 Marino et al.  
 9,037,250 B2 5/2015 Kaula et al.  
 9,180,021 B2 11/2015 Curran et al.  
 9,186,261 B2 11/2015 Pimenta et al.  
 9,204,871 B2 12/2015 Miles et al.  
 9,265,493 B2 2/2016 Miles et al.  
 9,301,743 B2 4/2016 Miles et al.  
 9,314,152 B2 4/2016 Pimenta et al.  
 9,387,090 B2 7/2016 Arnold et al.  
 9,456,783 B2 10/2016 Kaula et al.  
 9,468,405 B2 10/2016 Miles et al.  
 9,474,627 B2 10/2016 Curran et al.  
 9,486,329 B2 11/2016 Pimenta et al.  
 9,572,562 B2 2/2017 Miles et al.  
 9,610,071 B2 4/2017 Miles et al.  
 9,636,233 B2 5/2017 Arnold et al.  
 2001/0037123 A1 11/2001 Hancock  
 2001/0039949 A1 11/2001 Loubser  
 2001/0056280 A1 12/2001 Underwood et al.  
 2002/0007129 A1 1/2002 Marino  
 2002/0010392 A1 1/2002 Desai  
 2002/0016592 A1 2/2002 Branch et al.  
 2002/0065481 A1 5/2002 Cory et al.  
 2002/0072686 A1 6/2002 Hoey et al.  
 2002/0077632 A1 6/2002 Tsou  
 2002/0123744 A1 9/2002 Reynard  
 2002/0123780 A1 9/2002 Grill et al.  
 2002/0147387 A1 10/2002 Paolitto et al.  
 2002/0161415 A1 10/2002 Cohen et al.  
 2002/0193843 A1 12/2002 Hill et al.  
 2003/0032966 A1 2/2003 Foley et al.  
 2003/0070682 A1 4/2003 Wilson et al.  
 2003/0083688 A1 5/2003 Simonson  
 2003/0105503 A1 6/2003 Marino  
 2003/0105528 A1 6/2003 Shimp et al.  
 2003/0109928 A1 6/2003 Pasquet et al.  
 2003/0139648 A1 7/2003 Foley et al.  
 2003/0149341 A1 8/2003 Clifton  
 2003/0225405 A1 12/2003 Weiner  
 2003/0236544 A1 12/2003 Lunsford et al.  
 2004/0181165 A1 9/2004 Hoey et al.  
 2004/0199084 A1 10/2004 Kelleher et al.  
 2004/0225228 A1 11/2004 Ferree  
 2004/0230191 A1 11/2004 Frey et al.  
 2005/0004593 A1 1/2005 Simonson  
 2005/0004623 A1 1/2005 Miles et al.  
 2005/0033380 A1 2/2005 Tanner et al.  
 2005/0060006 A1 3/2005 Pflueger et al.  
 2005/0075578 A1 4/2005 Gharib et al.  
 2005/0080320 A1 4/2005 Lee et al.  
 2005/0149035 A1 7/2005 Pimenta et al.  
 2005/0149054 A1 7/2005 Gorek  
 2005/0182454 A1 8/2005 Gharib et al.  
 2005/0192575 A1 9/2005 Pacheco  
 2005/0203538 A1 9/2005 Lo et al.  
 2005/0228232 A1 10/2005 Gillinov et al.  
 2005/0277812 A1 12/2005 Myles  
 2006/0025703 A1 2/2006 Miles et al.  
 2006/0052826 A1 3/2006 Kim et al.  
 2006/0052828 A1 3/2006 Kim et al.

2006/0069315 A1 3/2006 Miles et al.  
 2006/0224078 A1 10/2006 Hoey et al.  
 2006/0235529 A1 10/2006 Ralph et al.  
 2006/0247658 A1 11/2006 Pond et al.  
 2007/0016097 A1 1/2007 Farquhar et al.  
 2007/0049931 A1 3/2007 Justis et al.  
 2007/0049962 A1 3/2007 Marino et al.  
 2007/0072475 A1 3/2007 Justin et al.  
 2007/0100212 A1 5/2007 Pimenta et al.  
 2007/0198062 A1 8/2007 Miles et al.  
 2007/0208228 A1 9/2007 Pavento et al.  
 2007/0260317 A1 11/2007 Ankney et al.  
 2007/0270842 A1 11/2007 Bankoski et al.  
 2007/0293782 A1 12/2007 Marino  
 2008/0058606 A1 3/2008 Miles et al.  
 2008/0058838 A1 3/2008 Steinberg  
 2008/0064976 A1 3/2008 Kelleher et al.  
 2008/0064977 A1 3/2008 Kelleher et al.  
 2008/0065135 A1 3/2008 Marino et al.  
 2008/0065144 A1 3/2008 Marino et al.  
 2008/0065178 A1 3/2008 Kelleher et al.  
 2008/0071191 A1 3/2008 Kelleher et al.  
 2008/0077138 A1 3/2008 Cohen et al.  
 2008/0097164 A1 4/2008 Miles et al.  
 2008/0103601 A1 5/2008 Biro et al.  
 2008/0146885 A1 6/2008 Protopsaltis  
 2008/0183214 A1 7/2008 Copp et al.  
 2008/0221394 A1 9/2008 Melkent et al.  
 2008/0288077 A1 11/2008 Reo et al.  
 2008/0300465 A1 12/2008 Feigenwinter et al.  
 2009/0030519 A1 1/2009 Falahee  
 2009/0124860 A1 5/2009 Miles et al.  
 2009/0132049 A1 5/2009 Carver et al.  
 2009/0138050 A1 5/2009 Ferree  
 2009/0138090 A1 5/2009 Hurlbert et al.  
 2009/0192403 A1 7/2009 Gharib et al.  
 2009/0204016 A1 8/2009 Gharib et al.  
 2010/0069783 A1 3/2010 Miles et al.  
 2010/0106251 A1 4/2010 Kast  
 2010/0130827 A1 5/2010 Pimenta et al.  
 2010/0152603 A1 6/2010 Miles et al.  
 2010/0160738 A1 6/2010 Miles et al.  
 2010/0174146 A1 7/2010 Miles  
 2010/0174148 A1 7/2010 Miles et al.  
 2010/0228350 A1 9/2010 Gornet et al.  
 2011/0046448 A1 2/2011 Paolitto et al.  
 2011/0218631 A1 9/2011 Woodburn, Sr. et al.  
 2011/0313530 A1 12/2011 Gharib et al.  
 2012/0238822 A1 9/2012 Miles  
 2012/0238893 A1 9/2012 Farquhar et al.  
 2013/0331943 A1 12/2013 Arnold et al.  
 2014/0235950 A1 8/2014 Miles et al.  
 2014/0288374 A1 9/2014 Miles et al.  
 2014/0288375 A1 9/2014 Miles et al.  
 2015/0150693 A1 6/2015 Gharib et al.  
 2015/0157227 A1 6/2015 Kelleher et al.  
 2015/0157228 A1 6/2015 Marino et al.  
 2015/0282948 A1 10/2015 Arnold et al.  
 2016/0120530 A1 5/2016 Miles et al.  
 2016/0174958 A1 6/2016 Miles et al.  
 2016/0174959 A1 6/2016 Miles et al.  
 2016/0192921 A1 7/2016 Pimenta et al.  
 2016/0374613 A1 12/2016 Kaula et al.  
 2017/0007421 A1 1/2017 Curran et al.  
 2017/0020503 A1 1/2017 Miles et al.  
 2017/0027712 A1 2/2017 Pimenta et al.  
 2017/0143514 A1 5/2017 Gharib et al.  
 2017/0143515 A1 5/2017 Gharib et al.  
 2017/0156580 A1 6/2017 Miles et al.  
 2017/0164938 A1 6/2017 Miles et al.  
 2017/0172558 A1 6/2017 Miles et al.

## FOREIGN PATENT DOCUMENTS

EP 0 334 116 9/1989  
 EP 0 567 424 10/1993  
 EP 0 972 538 1/2000  
 EP 1 002 500 5/2000  
 FR 2 795 624 1/2001

## (56) References Cited

## FOREIGN PATENT DOCUMENTS

JP	793186	5/1990
JP	10-14928	3/1996
KR	3019990007098	11/1999
WO	94/28824	12/1994
WO	97/00702	1/1997
WO	98/23324	6/1998
WO	99/52446	10/1999
WO	00/27291	5/2000
WO	00/38574	7/2000
WO	00/44288	8/2000
WO	WO-0062660 A1	10/2000
WO	00/66217	11/2000
WO	00/67645	11/2000
WO	01/08563	2/2001
WO	01/37728	5/2001
WO	01/60263	8/2001
WO	02/054960	7/2002
WO	02/058780	8/2002
WO	02/71953	9/2002
WO	02/87678	11/2002
WO	03/005887	1/2003
WO	03/026482	4/2003
WO	03/037170	5/2003
WO	WO-03084398 A1	10/2003
WO	WO-2004064634 A1	8/2004
WO	05/013805	2/2005
WO	05/030318	4/2005
WO	06/042241	4/2006
WO	06/066217	6/2006
WO	WO-2007035925 A2	3/2007
WO	WO-2007136784 A2	11/2007
WO	WO-2009055034 A1	4/2009
WO	WO-2011059491 A1	5/2011
WO	WO-2011059498 A1	5/2011
WO	WO-2012026981 A1	3/2012
WO	WO-2012103254 A2	8/2012
WO	WO-2013028571 A1	2/2013

## OTHER PUBLICATIONS

Dirksmeier et al., "Microendoscopic and Open Laminotomy and Discectomy in Lumbar Disc Disease" *Seminars in Spine Surgery*, 1999, 11(2): 138-146.

METRx Delivered Order Form, 1999, 13 pages.

Medtronic Sofamor Danek "METRx™ MicroDiscectomy System," Medtronic Sofamor Danek USA, 2000, 21 pgs.

Medtronic Sofamor Danek "METRx System Surgical Technique," 2004, 22 pages.

"MetRx System MicroEndoscopic Discectomy: An Evolution in Minimally Invasive Spine Surgery," Sofamor Danek, 1999, 6 pages.

Smith and Foley "MetRx System MicroEndoscopic Discectomy: Surgical Technique" Medtronic Sofamor Danek, 2000, 24 pages.

"Sofamor Danek MED Microendoscopic Discectomy System Brochure" including Rapp "New endoscopic lumbar technique improves access preserves tissue" Reprinted with permission from: *Orthopedics Today*, 1998, 18(1): 2 pages.

Japanese Patent Office JP Patent Application No. 2006-528306 Office Action with English Translation, Jun. 10, 2009, 4 pages.

Plaintiffs' Preliminary Invalidation Contentions re U.S. Pat. No. 7,207,949; U.S. Pat. No. 7,470,236 and U.S. Pat. No. 7,582,058, Sep. 18, 2009, 19 pages.

Plaintiffs' Preliminary Invalidation Contentions-Appendices, Sep. 18, 2009, 191 pages.

Plaintiffs' Supplemental Preliminary Invalidation Contentions re U.S. Pat. No. 7,207,949, U.S. Pat. No. 7,470,236, and U.S. Pat. No. 7,582,058, Sep. 29, 2009, 21 pages.

Plaintiffs' Supplemental Preliminary Invalidation Contentions-Appendices, Sep. 29, 2009, 294 pages.

Axon 501(k) Notification: Epoch 2000 Neurological Workstation, Dec. 3, 1997, 464 pages.

Foley and Smith, "Microendoscopic Discectomy," *Techniques in Neurosurgery*, 1997, 3(4):301-307.

Medtronic Sofamor Danek "UNION™/ UNION-LTM Anterior & Lateral Impacted Fusion Devices: Clear choice of stabilization," Medtronic Sofamor Danek, 2000, 4 pages.

NuVasive Vector™ Cannulae, 2000, 1 page.

NuVasive Triad™ Tri-Columnar Spinal EndoArthrodesis™ via Minimally Invasive Guidance, 2000, 1 page (prior to Sep. 25, 2003).

NuVasive Triad™ Cortical Bone Allograft, 2000, 1 page (prior to Sep. 25, 2003).

NuVasive Vertebral Body Access System, 2000, 1 page.

Marina, "New Technology for Guided Navigation with Real Time Nerve Surveillance for Minimally Invasive Spine Discectomy & Arthrodesis," *Spine*, 2000, p. 39.

NuVasive "INS-1 Screw Test," 2001, 10 pages.

NuVasive letter re 510k Neuro Vision JJB System, Oct. 16, 2001, 5 pages.

NuVasive letter re 510k Guided Arthroscopy System, Oct. 5, 1999, 6 pages.

NuVasive letter re 510k INS-1 Intraoperative Nerve Surveillance System, Nov. 13, 2000, 7 pages.

"NuVasive™ Receives Clearance to Market Two Key Elem Minimally Invasive Spine Surgery System," Nov. 27, 2001, 20 pages.

Schick et al., "Microendoscopic lumbar discectomy versus open surgery: an intraoperative EMG study," *Eur Spine J*, 2002, 11: 20-26.

NuVasive letter re: 510(k) for Neurovision JJB System (Summary), Sep. 25, 2001, 28 pages.

NuVasive letter re: Special 510(k) Premarket Notification: Neurovision JJB System (Device Description), Jul. 3, 2003, 18 pages.

NuVasive letter re: Special 510(k) Premarket Notification: Neurovision JJB System (Device Description), Mar. 1, 2004, 16 pages.

NuVasive letter re: Special 510(k) Premarket Notification: Neurovision JJB System (Device Description), May 26, 2005, 17 pages.

NuVasive letter re: 510(k) Premarket Notification: Neurovision JJB System (Device Description), Jun. 24, 2005, 16 pages.

NuVasive letter re: Special 510(k) Premarket Notification: Neurovision JJB System (Device Description), Sep. 14, 2006, 17 pages.

NuVasive 510(k) Premarket Notification: Neurovision JJB System (Device Description), Aug. 20, 2007, 8 pages.

NuVasive letter re: 510(k) Premarket Notification: Guided Spinal Arthroscopy System (Device Description), Feb. 1, 1999, 40 pages.

NuVasive 510(k) Premarket Notification: Spinal System (Summary), Apr. 12, 2004, 10 pages.

NuVasive 510(k) Summary NIM Monitor, Sep. 4, 1998, 4 pages.

NuVasive correspondence re 510(k) Premarket Notification INS-1 Intraoperative Nerve Surveillance System: Section IV Device Description, pp. 12-51 (prior to Sep. 25, 2003).

Mathews et al., "Laparoscopic Discectomy with Anterior Lumbar Interbody Fusion," *SPINE*, 1995, 20(16): 1797-1802.

Rose et al., "Persistently Electrified Pedicle Stimulation Instruments in Spinal Instrumentation: Techniques and Protocol Development," *SPINE*, 1997, 22(3): 334-343.

"Electromyography System," International Search report from International Application No. PCT/US00/32329, dated Apr. 27, 2001, 9 pages.

"Nerve Proximity and Status Detection System and Method," International Search Report from International Application No. PCT/US01/18606, dated Oct. 18, 2001, 6 pages.

"Relative Nerve Movement and Status Detection System and Method," International Search Report from International Application No. PCT/US01/18579, dated Jan. 15, 2002, 6 pages.

"System and Method for Determining Nerve Proximity Direction and Pathology During Surgery," International Search Report from International Application No. PCT/US02/22247, dated Mar. 27, 2003, 4 pages.

"System and Methods for Determining Nerve Direction to a Surgical Instrument," International Search Report from International Application No. PCT/US03/02056, dated Aug. 12, 2003, 5 pages.

"Systems and Methods for Performing Percutaneous Pedicle Integrity Assessments," International Search Report from International Application No. PCT/US02/35047, dated Aug. 11, 2003, 5 pages.

(56)

## References Cited

## OTHER PUBLICATIONS

- "Systems and Methods for Performing Surgery Procedures and Assessments," International Search Report from International Application No. PCT/US02/30617, dated Jun. 5, 2003, 4 pages.
- Lenke et al., "Triggered Electromyographic Threshold for Accuracy of Pedicle Screw Placement," *Spine*, 1995, 20(4): 1585-1591.
- "Brackmann II EMG System," Medical Electronics, 1999, 4 pages.
- "Neurovision SE Nerve Locator/Monitor", RLN Systems Inc. Operators Manual, 1999, 22 pages.
- "The Brackmann II EMG Monitoring System," Medical Electronics Co. Operator's Manual Version 1.1, 1995, 50 pages.
- "The Nicolet Viking IV," Nicolet Biomedical Products, 1999, 6 pages.
- Anderson et al., "Pedicle screws with high electrical resistance: a potential source of error with stimulus-evoked EMG," *Spine*, Department of Orthopaedic Surgery University of Virginia, Jul. 15, 2002, 27(14): 1577-1581.
- Bose et al., "Neurophysiologic Monitoring of Spinal Nerve Root Function During Instrumented Posterior Lumbar Spine Surgery," *Spine*, 2002, 27(13): 1444-1450.
- Calancie et al., "Stimulus-Evoked EMG Monitoring During Transpedicular Lumbosacral Spine Instrumentation" *Spine*, 1994, 19(24): 2780-2786.
- Clements et al., "Evoked and Spontaneous Electromyography to Evaluate Lumbosacral Pedicle Screw Placement," *Spine*, 1996, 21(5): 600-604.
- Danesh-Clough et al., "The Use of Evoked EMG in Detecting Misplaced Thoracolumbar Pedicle Screws," *Spine*, Orthopaedic Department Dunedin Hospital, Jun. 15, 2001, 26(12): 1313-1316.
- Darden et al., "A Comparison of Impedance and Electromyogram Measurements in Detecting the Presence of Pedicle Wall Break-through," *Spine*, Charlotte Spine Center, North Carolina, Jan. 15, 1998, 23(2): 256-262.
- Ebraheim et al., "Anatomic Relations Between the Lumbar Pedicle and the Adjacent Neural Structures," *Spine*, Department of Orthopaedic Surgery Medical College of Ohio, Oct. 15, 1997, 22(20): 2338-2341.
- Ford et al., "Electrical Characteristics of Peripheral Nerve Stimulators Implications for Nerve Localization," *Regional Anesthesia*, 1984, 9: 73-77.
- Glassman et al., "A Prospective Analysis of Intraoperative Electromyographic Monitoring of Pedicle Screw Placement With Computed Tomographic Scan Confirmation," *Spine*, 1995, 20(12): 1375-1379.
- Greenblatt et al., "Needle Nerve Stimulator-Locator: Nerve Blocks with a New Instrument for Locating Nerves," *Anesthesia & Analgesia*, 1962, 41(5): 599-602.
- Haig, "Point of view," *Spine*, 2002, 27(24): 2819.
- Haig et al., "The Relation Among Spinal Geometry on MRI, Paraspinal Electromyographic Abnormalities, and Age in Persons Referred for Electrodiagnostic Testing of Low Back Symptoms," *Spine*, Department of Physical Medicine and Rehabilitation University of Michigan, Sep. 1, 2002, 27(17): 1918-1925.
- Holland et al., "Higher Electrical Stimulus Intensities are Required to Activate Chronically Compressed Nerve Roots: Implications for Intraoperative Electromyographic Pedicle Screw Testing," *Spine*, Department of Neurology, Johns Hopkins University School of Medicine, Jan. 15, 1998, 23(2): 224-227.
- Holland, "Intraoperative Electromyography During Thoracolumbar Spinal Surgery," *Spine*, 1998, 23(17): 1915-1922.
- Journee et al., "System for Intra-Operative Monitoring of the Cortical Integrity of the Pedicle During Pedicle Screw Placement in Low-Back Surgery: Design and Clinical Results," *Sensory and Neuromuscular Diagnostic Instrumentation and Data Analysis I*, 18th Annual International Conference on Engineering in Medicine and Biology Society, Amsterdam, 1996, pp. 144-145.
- Maguire et al., "Evaluation of Intrapedicular Screw Position Using Intraoperative Evoked Electromyography," *Spine*, 1995, 20(9): 1068-1074.
- Martin et al., "Initiation of Erection and Semen Release by Rectal Probe Electrostimulation (RPE)," *The Journal of Urology*, The Williams & Wilkins Co., 1983, 129: 637-642.
- Minahan et al., "The Effect of Neuromuscular Blockade on Pedicle Screw Stimulation Thresholds" *Spine*, Department of Neurology, Johns Hopkins University School of Medicine, Oct. 1, 2000, 25(19): 2526-2530.
- Pither et al., "The Use of Peripheral Nerve Stimulators for Regional Anesthesia: Review of Experimental Characteristics Technique and Clinical Applications," *Regional Anesthesia*, 1985, 10:49-58.
- Raj et al., "Infralavicular Brachial Plexus Block—A New Approach" *Anesthesia and Analgesia*, 1973, (52)6: 897-904.
- Raj et al., "The Use of Peripheral Nerve Stimulators for Regional Anesthesia," *Clinical Issues in Regional Anesthesia*, 1985, 1(4):1-6.
- Raj et al., "Use of the Nerve Stimulator for Peripheral Blocks," *Regional Anesthesia*, Apr.-Jun. 1980, pp. 14-21.
- Raymond et al., "The Nerve Seeker: A System for Automated Nerve Localization," *Regional Anesthesia*, 1992, 17(3): 151-162.
- Shafik, "Cavernous Nerve Stimulation through an Extrapelvic Subpubic Approach: Role in Penile Erection," *Eur. Urol*, 1994, 26: 98-102.
- Toleikis et al., "The Usefulness of Electrical Stimulation for Assessing Pedicle Screw Replacements," *Journal of Spinal Disorder*, 2000, 13(4): 283-289.
- Medtronic Sofamor Danek "UNION™ / UNION-LTM Anterior & Lateral Impacted Fusion Devices: Surgical Technique" Medtronic Sofamor Danek, 2001, 20 pages.
- Defendant's Disclosure of Asserted Claims and Preliminary Infringement Contentions Regarding U.S. Pat. No. 7,207,949; U.S. Pat. No. 7,470,236 and U.S. Pat. No. 7,582,058, Aug. 31, 2009, 21 pages.
- Bergey et al., "Endoscopic Lateral Transpsoas Approach to the Lumbar Spine," *Spine*, 2004, 29(15): 1681-1688.
- Dezawa et al., "Retroperitoneal Laparoscopic Lateral Approach to the Lumbar Spine: A New Approach, Technique, and Clinical Trial," *Journal of Spinal Disorders*, 2000, 13(2): 138-143.
- Gardocki, "Tubular disectomy minimizes collateral damage: A logical progression moves spine surgery forward," *AAOS Now*, 2009, 5 pages.
- Hovorka et al., "Five years' experience of retroperitoneal lumbar and thoracolumbar surgery," *Eur Spine J.*, 2000, 9(1): S30-S34.
- Kossmann et al., "The use of a retractor system (SynFrame) for open, minimal invasive reconstruction of the anterior column of the thoracic and lumbar spine," *Eur Spine J.*, 2001, 10: 396-402.
- Mayer, "A New Microsurgical Technique for Minimally Invasive Anterior Lumbar Interbody Fusion," *Spine*, 1997, 22(6): 691-699.
- Mayer, "The ALIF Concept," *Eur Spine J.*, 2000, 9(1): S35-S43.
- Mayer and Wiechert, "Microsurgical Anterior Approaches to the Lumbar Spine for Interbody Fusion and Total Disc Replacement," *Neurosurgery*, 2002, 51(2): 159-165.
- McAfee et al., "Minimally Invasive Anterior Retroperitoneal Approach to the Lumbar Spine: Emphasis on the Lateral BAK," *Spine*, 1998, 23(13): 1476-1484.
- Rao, et al., "Dynamic retraction of the psoas muscle to expose the lumbar spine using the retroperitoneal approach," *J. Neurosurg Spine*, 2006, 5: 468-470.
- Wolfla et al., "Retroperitoneal lateral lumbar interbody fusion with titanium threaded fusion cages," *J. Neurosurg (Spine 1)*, 2002, 96: 50-55.
- Larson and Maiman, "Surgery of the Lumbar Spine," Thieme Medical Publishers, Inc., 1999, pp. 305-319.
- Medtronic XOMED Surgical Products, Inc., NIM-Response Nerve Integrity Monitor Intraoperative EMG Monitor User's Guide, Revision B, 2000, 47 pages.
- "NuVasive's spine surgery system cleared in the US," *Pharm & Medical Industry Week*, Dec. 10, 2001, 1 page.
- Pimenta, "Initial Clinical Results of Direct Lateral, Minimally Invasive Access to the Lumbar Spine for Disc Nucleus Replacement Using a Novel Neurophysiological Monitoring System," *The 9th IMAST*, May 2002, 1 page.

(56)

## References Cited

## OTHER PUBLICATIONS

- Pimenta et al., "The Lateral Endoscopic Transpoas Retroperitoneal Approach (Letra) for Implants in the Lumbar Spine," *World Spine II—Second Interdisciplinary Congress on Spine Care*, Aug. 2003, 2 pages.
- Crock, H.V. MD., "Anterior Lumbar Interbody Fusion," *Clinical Orthopaedics and Related Research*, No. One Hundred Sixty Five, 1982, pp. 157-163, 13 pages.
- Mayer and Brock, "Percutaneous endoscopic discectomy: surgical technique and preliminary results compared to microsurgical discectomy," *J. Neurosurg.*, 1993, 78: 216-225.
- Schaffer and Kambin, "Percutaneous Posterolateral Lumbar Discectomy and Decompression with a 6.9-Millimeter Cannula," *The Journal of Bone and Joint Surgery*, 1991, 73A(6): 822-831.
- Friedman, "Percutaneous discectomy: An alternative to chemonucleolysis," *Neurosurgery*, 1983, 13(5): 542-547.
- Request for Inter Partes Reexamination in re U.S. Pat. No. 7,905,840, dated Feb. 8, 2012, 204 pages.
- Brau, "Chapter 22: Anterior Retroperitoneal Muscle-Sparing approach to L2-S1 of the Lumbar Spine," *Surgical Approaches to the Spine*. Robert G. Watkins, MD. (ed) 2003. pp. 165-181.
- Kossmann et al., "Minimally Invasive Vertebral Replacement with Cages in Thoracic and Lumbar Spine," *European Journal of Trauma*, 2001, 27: 292-300.
- Mayer H. M. (ed.) *Minimally Invasive Spine Surgery: A Surgical Manual*. 2000. 51 pages.
- Pimenta et al., "Implante de protese de nucleo pulposo: analise inicial," *Journal Brasileiro de Neurocirurgia*, 2001, 12(2): 93-96.
- Traynelis, "Spinal Arthroplasty," *Neurological Focus*, 2002, 13(2): 12 pages.
- Zdeblick, Thomas A. (ed.). *Anterior Approaches to the Spine*. 1999. 43 pages.
- Amended Complaint for *NuVasive, Inc. v. Globus Medical, Inc.*, Case No. 1:10-cv-0849 (D. Del., Oct. 5, 2010), 28 pages.
- Request for Inter Partes Reexamination in re U.S. Pat. No. 7,819,801, dated Feb. 8, 2012, 89 pages.
- Kossmann et al., "The use of a retractor system (SynFrame) for open, minimal invasive reconstruction of the anterior column of the thoracic and lumbar spine," *Eur Spine J*, 2001, 10: 396-402.
- de Peretti et al., "New possibilities in L2-L5 lumbar arthrodesis using a lateral retroperitoneal approach assisted by laparoscopy: preliminary results," *Eur Spine J*, 1996, 5: 210-216.
- Litwin et al., "Hand-assisted laparoscopic surgery (HALS) with the handport system," *Annals of Surgery*, 2000, 231(5): 715-723.
- Acland's Video Atlas of Human Anatomy, Section 3.1.7: Paravertebral Muscles. Available online: <http://aclandanatomy.com/abstract/4010463>. Accessed Jul. 11, 2012.
- MedlinePlus, a Service of the U.S. National Library of Medicine and National Institutes of Health. Available online: <http://www.nlm.nih.gov/medlineplus/>. Accessed Jul. 11, 2012.
- Baulot et al., *Adjuvant Anterior Spinal Fusion Via Thoracoscopy*, *Lyon Chirurgical*, 1994, 90(5): 347-351 including English Translation and Certificate of Translation.
- Leu et al., "Percutaneous Fusion of the Lumbar Spine," *Spine*, 1992, 6(3): 593-604.
- Rosenthal et al., "Removal of a Protruded Thoracic Disc Using Microsurgical Endoscopy," *Spine*, 1994, 19(9): 1087-1091.
- Counterclaim Defendants' Corrected Amended Invalidity Contentions re U.S. Pat. No. 8,000,782; U.S. Pat. No. 8,005,535; U.S. Pat. No. 8,016,767; U.S. Pat. No. 8,192,356; U.S. Pat. No. 8,187,334; U.S. Pat. No. 8,361,156, D652,922; D666,294 re Case No. 3:12-cv-02738-CAB(MDD), dated Aug. 19, 2013, 30 pages.
- Petition for Inter Partes Review IPR2014-00034, filed Oct. 8, 2013, 65 pages.
- Petition for Inter Partes Review IPR2014-00035, filed Oct. 8, 2013, 65 pages.
- Declaration of Lee Grant, from IPR2014-00034, Oct. 7, 2013, 36 pages.
- Declaration of David Hacker from IPR2014-00034, Oct. 4, 2013, 64 pages.
- NuVasive, Inc.'s Opening Claim Construction Brief Regarding U.S. Pat. No. 8,000,782; U.S. Pat. No. 8,005,535; U.S. Pat. No. 8,016,767; U.S. Pat. No. 8,192,356; U.S. Pat. No. 8,187,334; U.S. Pat. No. 8,361,156; D652,922. and U.S. Pat. No. 5,676,146 C2, filed Sep. 3, 2013, in *Warsaw Orthopedic, Inc. v. NuVasive, Inc.*, No. 3:12-cv-02738-CAB-MDD (S.D. Cal.), 34 pages.
- Petition for Inter Partes Review IPR2014-00073, filed Oct. 18, 2013, 65 pages.
- Petition for Inter Partes Review IPR2014-00074, filed Oct. 18, 2013, 65 pages.
- Petition for Inter Partes Review IPR2014-00075, filed Oct. 21, 2013, 66 pages.
- Petition for Inter Partes Review IPR2014-00076, filed Oct. 21, 2013, 65 pages.
- Petition for Inter Partes Review IPR2014-00081, filed Oct. 22, 2013, 64 pages.
- Petition for Inter Partes Review IPR2014-00087, filed Oct. 22, 2013, 64 pages.
- Declaration of Lee Grant, from IPR2014-00073, Oct. 9, 2013, 36 pages.
- Declaration of David Hacker, from IPR2014-00073, Oct. 10, 2013, 64 pages.
- U.S. Appl. No. 60/392,214, filed Jun. 26, 2002, 97 pages.
- Amendment in reply to Feb. 15, 2012 Office Action in U.S. Appl. No. 12/635,418, dated Mar. 16, 2012, 24 pages.
- Decision on Appeal in Inter Partes Reexamination Control No. 95/001,247, dated Mar. 18, 2013, 49 pages.
- Declaration of Lee Grant, from IPR2014-00074, Oct. 9, 2013, 36 pages.
- Declaration of David Hacker, from IPR2014-00074, Oct. 10, 2013, 64 pages.
- Declaration of David Hacker, from IPR2014-00075, Oct. 10, 2013, 64 pages.
- Amendment in reply to Action of Feb. 7, 2011 and Notice of May 12, 2011, in U.S. Appl. No. 11/789,284, dated May 17, 2011, 16 pages.
- Notice of Allowance in U.S. Appl. No. 11/789,284, dated Jul. 18, 2011, 8 pages.
- Office action from U.S. Appl. No. 11/789,284, dated Feb. 7, 2011, 10 pages.
- Merriam-Webster's Collegiate Dictionary, p. 65 (10th ed. 1998).
- Declaration of Lee Grant, from IPR2014-00076, Oct. 9, 2013, 36 pages.
- Moed et al., "Evaluation of Intraoperative Nerve-Monitoring During Insertion of an Iliosacral Implant in an Animal Model, *Journal of Bone and Joint Surgery*," 1999, 81-A(11): 9.
- Declaration of Lee Grant, from IPR2014-00081, Oct. 9, 2013, 36 pages.
- Declaration of David Hacker from IPR2014-00081, Oct. 10, 2013, 64 pages.
- U.S. Appl. No. 60/325,424, filed Sep. 25, 2001, 346 pages.
- Declaration of Lee Grant, from IPR2014-00087, Oct. 9, 2013, 36 pages.
- Declaration of David Hacker from IPR2014-00087, Oct. 10, 2013, 64 pages.
- Request for Inter Partes Reexamination in re: U.S. Pat. No. 7,691,057, dated Feb. 8, 2012, 50 pages.
- Declaration of Daniel Schwartz, Ph.D. from IPR2014-00034, Oct. 7, 2013, 1056 pages.
- Declaration of Daniel Schwartz, Ph.D. from IPR2014-00035, Oct. 7, 2013, 661 pages.
- 510(K) No. K002677, approved by the FDA on Nov. 13, 2000, 634 pages.
- 510(K) No. K013215, approved by the FDA on Oct. 16, 2001, 376 pages.
- Declaration of Robert G. Watkins, from IPR2014-00073, Oct. 18, 2013, 1101 pages.
- Declaration of Daniel Schwartz, from IPR2014-00073, Oct. 12, 2013, 1226 pages.
- Declaration of Robert G. Watkins, from IPR2014-00074, Oct. 18, 2013, 548 pages.
- Declaration of Daniel Schwartz, from IPR2014-00074, Oct. 12, 2013, 565 pages.



(56)

**References Cited**

## OTHER PUBLICATIONS

Declaration of Robert G. Watkins, from IPR2014-00075, Oct. 18, 2013, 674 pages.

Declaration of Daniel Schwartz, from IPR2014-00075, Oct. 12, 2013, 1107 pages.

Declaration of Robert G. Watkins, from IPR2014-00076, Oct. 18, 2013, 543 pages.

Declaration of Daniel Schwartz, from IPR2014-00076, Oct. 12, 2013, 1247 pages.

Declaration of David Hacker, from IPR2014-00076, Oct. 10, 2013, 64 pages.

Declaration of Daniel Schwartz, from IPR2014-0081, Oct. 21, 2013, 585 pages.

Declaration of Daniel Schwartz from IPR2014-0087, Oct. 21, 2013, 585 pages.

Patent Owner NuVasive Inc's Preliminary Response from IPR2014-00034, dated Jan. 15, 2014, 66 pages.

Patent Trial and Appeal Board Decision from IPR 2014-00034, dated Apr. 8, 2014, 35 pages.

Patent Owner NuVasive Inc's Preliminary Response from IPR2014-00035, dated Jan. 15, 2014, 42 pages.

Patent Trial and Appeal Board Decision from IPR 2014-00035, dated Apr. 8, 2014, 12 pages.

Patent Owner NuVasive Inc's Preliminary Response from IPR2014-00073, dated Jan. 31, 2014, 64 pages.

Patent Trial and Appeal Board Decision from IPR 2014-00073, dated Apr. 8, 2014, 34 pages.

Patent Owner NuVasive Inc's Preliminary Response from IPR2014-00074, dated Jan. 31, 2014, 68 pages.

Patent Trial and Appeal Board Decision from IPR 2014-00074, dated Apr. 8, 2014, 28 pages.

Patent Owner NuVasive Inc's Preliminary Response from IPR2014-00075, dated Jan. 31, 2014, 54 pages.

Patent Trial and Appeal Board Decision from IPR 2014-00075, dated Apr. 8, 2014, 23 pages.

Patent Owner NuVasive Inc's Preliminary Response from IPR2014-00076, dated Jan. 31, 2014, 58 pages.

Patent Trial and Appeal Board Decision from IPR 2014-00076, dated Apr. 8, 2014, 11 pages.

Patent Owner NuVasive Inc's Preliminary Response from IPR2014-00081, dated Jan. 31, 2014, 47 pages.

Patent Trial and Appeal Board Decision from IPR 2014-00081, dated Apr. 8, 2014, 31 pages.

Patent Owner NuVasive Inc's Preliminary Response from IPR2014-00087, dated Jan. 31, 2014, 51 pages.

Patent Trial and Appeal Board Decision from IPR 2014-00087, dated Apr. 8, 2014, 31 pages.

Final Written Decision from IPR 2014-00034, dated Apr. 3, 2015, 48 pages.

Final Written Decision from IPR 2014-00073, dated Apr. 3, 2015, 36 pages.

Final Written Decision from IPR 2014-00074, dated Apr. 3, 2015, 31 pages.

Final Written Decision from IPR 2014-00075, dated Apr. 3, 2015, 39 pages.

Final Written Decision from IPR 2014-00081, dated Apr. 3, 2015, 44 pages.

Final Written Decision from IPR 2014-00087, dated Apr. 3, 2015, 36 pages.

INS-I Guide Dec. 31, 2000, Part III.

Co-pending U.S. Appl. No. 15/498,296, filed Apr. 26, 2017.

Co-pending U.S. Appl. No. 90/013,464, filed Mar. 6, 2015.

Co-pending U.S. Appl. No. 90/013,546, filed Jul. 8, 2015.

Co-pending U.S. Appl. No. 90/013,605, filed Oct. 8, 2015.

Co-pending U.S. Appl. No. 95/001,247, filed Oct. 27, 2009.

Co-pending U.S. Appl. No. 95/001,888, filed Feb. 9, 2012.

Co-pending U.S. Appl. No. 95/001,890, filed Feb. 9, 2012.

European Search Report dated Apr. 7, 2015 for EP Application No. 12826211.0.

European Search Report dated Aug. 2, 2012 for EP Application No. 12001129.1.

European Search Report dated Sep. 28, 2009 for EP Application No. 02778359.6.

In re: NUVASIVE, Inc., in 2015-1670 decided on Dec. 7, 2016, 13 Pages.

In re: NUVASIVE, Inc., in 2015-1672, 2015-1673 decided on Nov. 9, 2016, 16 Pages.

In re: NUVASIVE, Inc., in 2015-1838 signed on May 10, 2017, 2 Pages.

In re: NUVASIVE, Inc., in 2015-1839, 2015-1840 signed on May 10, 2017, 2 Pages.

In re: NUVASIVE, Inc., in 2015-1841 decided on May 31, 2017, 16 Pages.

In re: NUVASIVE, Inc., in 2015-1842, 2015-1843 signed on May 10, 2017, 2 Pages.

In re: Warsaw Orthopedic, Inc. in 15-1050 filed Oct. 14, 2014.

In re: Warsaw Orthopedic, Inc. in 15-1058 filed Oct. 17, 2014.

INS-I Guide Dec. 31, 2000, Part I.

INS-I Guide Dec. 31, 2000, Part II.

International Search Report dated Jan. 12, 2011 for International Application No. PCT/US2010/002960.

International Search Report dated Feb. 9, 2005 for International Application PCT/US2004/031768.

International Search Report dated Jul. 24, 2012 for International Application No. PCT/US2012/022600.

International Search Report dated Oct. 29, 2012 for International Application No. PCT/US2012/051480.

International Search Report dated Dec. 13, 2011 for International Application No. PCT/US2011/001489.

International Search Report dated Dec. 24, 2008 for International Application No. PCT/US2008/012121.

International Search Report dated Mar. 23, 2011 for International Application No. PCT/US2010/002951.

Isley et al., "Recent Advances in Intraoperative Neuromonitoring of Spinal Cord Function: Pedicle Screw Stimulation Techniques," American Journal of Electroneurodiagnostic Technology, Jun. 1997, 37(2): 93-126.

Matthews et al., "Laparoscopic Discectomy with Anterior Lumbar Interbody Fusion," SPINE, 1995, 20(16): 1797-1802.

Notice of Allowance dated Mar. 30, 2017 for U.S. Appl. No. 14/263,797.

Notice of Allowance dated Apr. 12, 2017 for U.S. Appl. No. 15/272,071.

*NuVasive, Inc. v. Medtronic, Inc.* in 15-1674 filed May 26, 2015, Individual documents of the referenced court case are not being submitted herewith, as Applicant understands the documents to be readily accessible by the Examiner. However, Applicant can provide any of the documents upon request.

*NuVasive, Inc. v. Medtronic, Inc.* in 15-1712 filed Jun. 8, 2015, Individual documents of the referenced court case are not being submitted herewith, as Applicant understands the documents to be readily accessible by the Examiner. However, Applicant can provide any of the documents upon request.

*NuVasive, Inc. v. Warsaw Orthopedic, Inc.* in 15-1049 filed Oct. 14, 2014, Individual documents of the referenced court case are not being submitted herewith, as Applicant understands the documents to be readily accessible by the Examiner. However, Applicant can provide any of the documents upon request.

Office Action dated Jan. 11, 2012 for U.S. Appl. No. 11/982,185.

Office Action dated Jan. 12, 2012 for U.S. Appl. No. 11/489,020.

Office Action dated Jan. 21, 2011 for U.S. Appl. No. 11/982,185.

Office Action dated Feb. 26, 2016 for U.S. Appl. No. 14/622,585.

Office Action dated Mar. 16, 2009 for U.S. Appl. No. 11/489,020.

Office Action dated Mar. 29, 2017 for U.S. Appl. No. 15/448,395.

Office Action dated Apr. 5, 2017 for U.S. Appl. No. 15/445,854.

Office Action dated Apr. 6, 2017 for U.S. Appl. No. 15/439,889.

Office Action dated Apr. 7, 2017 for U.S. Appl. No. 15/059,215.

Office Action dated Apr. 29, 2010 for U.S. Appl. No. 11/982,185.

Office Action dated May 6, 2010 for U.S. Appl. No. 11/489,020.

Office Action dated May 8, 2014 for U.S. Appl. No. 13/964,836.

Office Action dated Jun. 17, 2009 for U.S. Appl. No. 11/982,185.

Office Action dated Sep. 15, 2008 for U.S. Appl. No. 11/489,020.

(56)

**References Cited**

## OTHER PUBLICATIONS

Office Action dated Sep. 19, 2016 for U.S. Appl. No. 14/263,797.  
Office Action dated Sep. 23, 2016 for U.S. Appl. No. 14/622,585.  
Office Action dated Oct. 9, 2009 for U.S. Appl. No. 11/489,020.  
Office Action dated Oct. 20, 2016 for U.S. Appl. No. 14/297,369.  
Office Action dated Nov. 28, 2016 for U.S. Appl. No. 14/994,640.  
Office Action dated Nov. 4, 2016 for U.S. Appl. No. 14/297,438.  
Office Action dated Dec. 19, 2014 for U.S. Appl. No. 13/964,836.  
Petition for Inter Partes Review by Medtronic, Inc. in IPR2013-00504 filed Aug. 14, 2013, Individual documents of the referenced court case are not being submitted herewith, as Applicant understands the documents to be readily accessible by the Examiner. However, Applicant can provide any of the documents upon request.  
Petition for Inter Partes Review by Medtronic, Inc. in IPR2013-00506 filed Aug. 14, 2013, Individual documents of the referenced court case are not being submitted herewith, as Applicant understands the documents to be readily accessible by the Examiner. However, Applicant can provide any of the documents upon request.  
Petition for Inter Partes Review by Medtronic, Inc. in IPR2013-00507 filed Aug. 14, 2013, Individual documents of the referenced court case are not being submitted herewith, as Applicant understands the documents to be readily accessible by the Examiner. However, Applicant can provide any of the documents upon request.  
Petition for Inter Partes Review by Medtronic, Inc. in IPR2013-00508 filed Aug. 14, 2013, Individual documents of the referenced court case are not being submitted herewith, as Applicant understands the documents to be readily accessible by the Examiner. However, Applicant can provide any of the documents upon request.  
Petition for Inter Partes Review by Medtronic, Inc. in IPR2014-00071 filed Oct. 16, 2013, Individual documents of the referenced court case are not being submitted herewith, as Applicant understands the documents to be readily accessible by the Examiner. However, Applicant can provide any of the documents upon request.  
Petition for Inter Partes Review by Medtronic, Inc. in IPR2014-00487 filed Mar. 5, 2014, Individual documents of the referenced

court case are not being submitted herewith, as Applicant understands the documents to be readily accessible by the Examiner. However, Applicant can provide any of the documents upon request.  
Petition for Inter Partes Review by NuVasive, Inc. in IPR2013-00206 filed Mar. 22, 2013, Individual documents of the referenced court case are not being submitted herewith, as Applicant understands the documents to be readily accessible by the Examiner. However, Applicant can provide any of the documents upon request.  
Petition for Inter Partes Review by NuVasive, Inc. in IPR2013-00208 filed Mar. 22, 2013, Individual documents of the referenced court case are not being submitted herewith, as Applicant understands the documents to be readily accessible by the Examiner. However, Applicant can provide any of the documents upon request.  
Petition for Inter Partes Review by NuVasive, Inc. in IPR2013-00395 filed Jun. 27, 2013, Individual documents of the referenced court case are not being submitted herewith, as Applicant understands the documents to be readily accessible by the Examiner. However, Applicant can provide any of the documents upon request.  
Petition for Inter Partes Review by NuVasive, Inc. in IPR2013-00396 filed Jun. 27, 2013, Individual documents of the referenced court case are not being submitted herewith, as Applicant understands the documents to be readily accessible by the Examiner. However, Applicant can provide any of the documents upon request.  
Petition for Inter Partes Review by NuVasive, Inc. in IPR2015-00502 filed Dec. 24, 2014, Individual documents of the referenced court case are not being submitted herewith, as Applicant understands the documents to be readily accessible by the Examiner. However, Applicant can provide any of the documents upon request.  
*Warsaw Orthopedic, Inc. v. NuVasive, Inc.* in 12-1263 filed Mar. 15, 2012.  
*Warsaw Orthopedic, Inc. v. NuVasive, Inc.* in 12-1266 filed Mar. 15, 2012.  
*Warsaw Orthopedic, Inc. v. NuVasive, Inc.* in 13-1576 filed Aug. 21, 2013.  
*Warsaw Orthopedic, Inc. v. NuVasive, Inc.* in 13-1577 filed Aug. 21, 2013.

\* cited by examiner

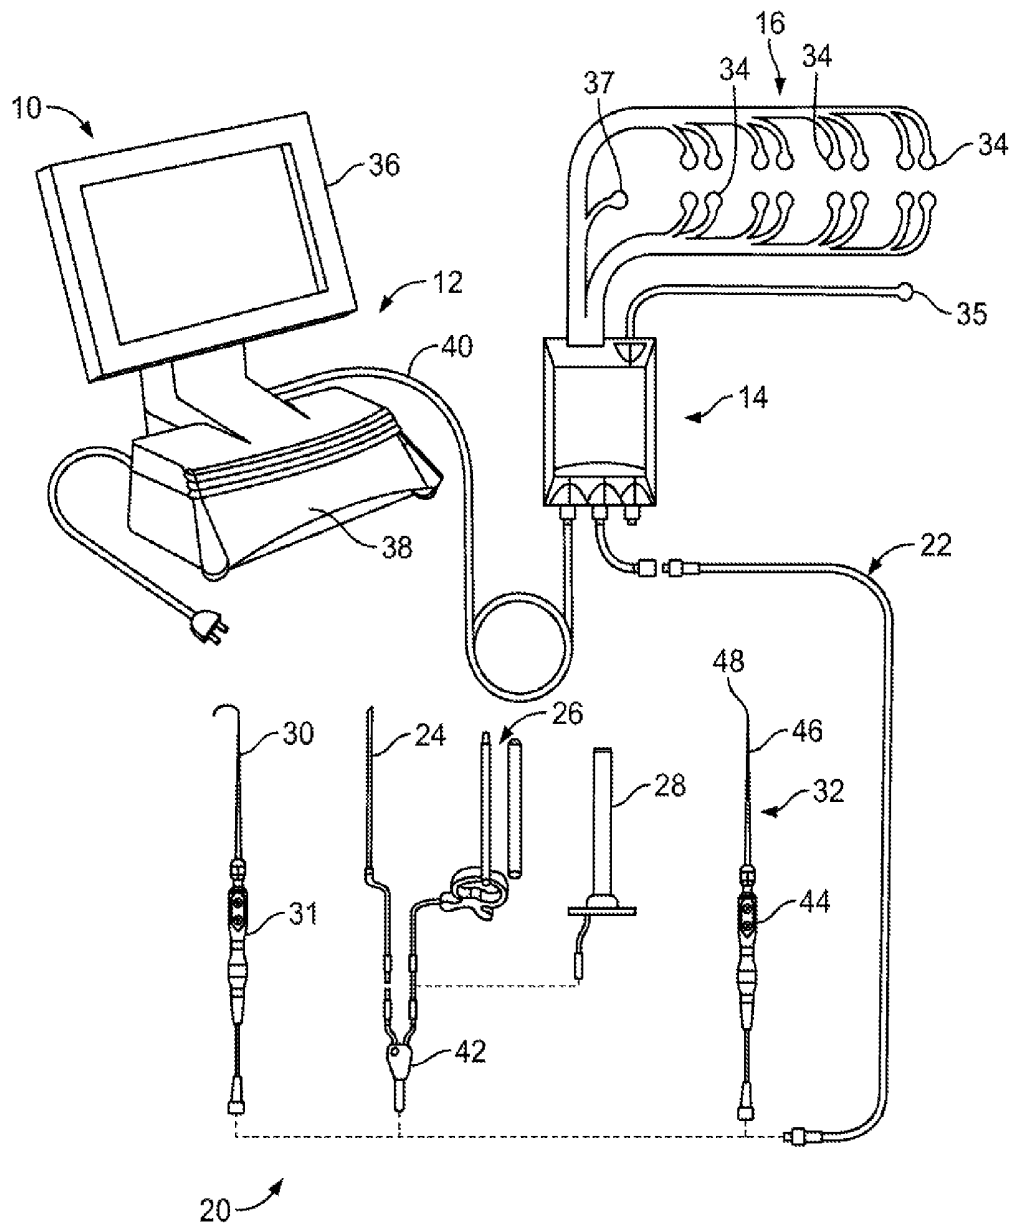


FIG. 1

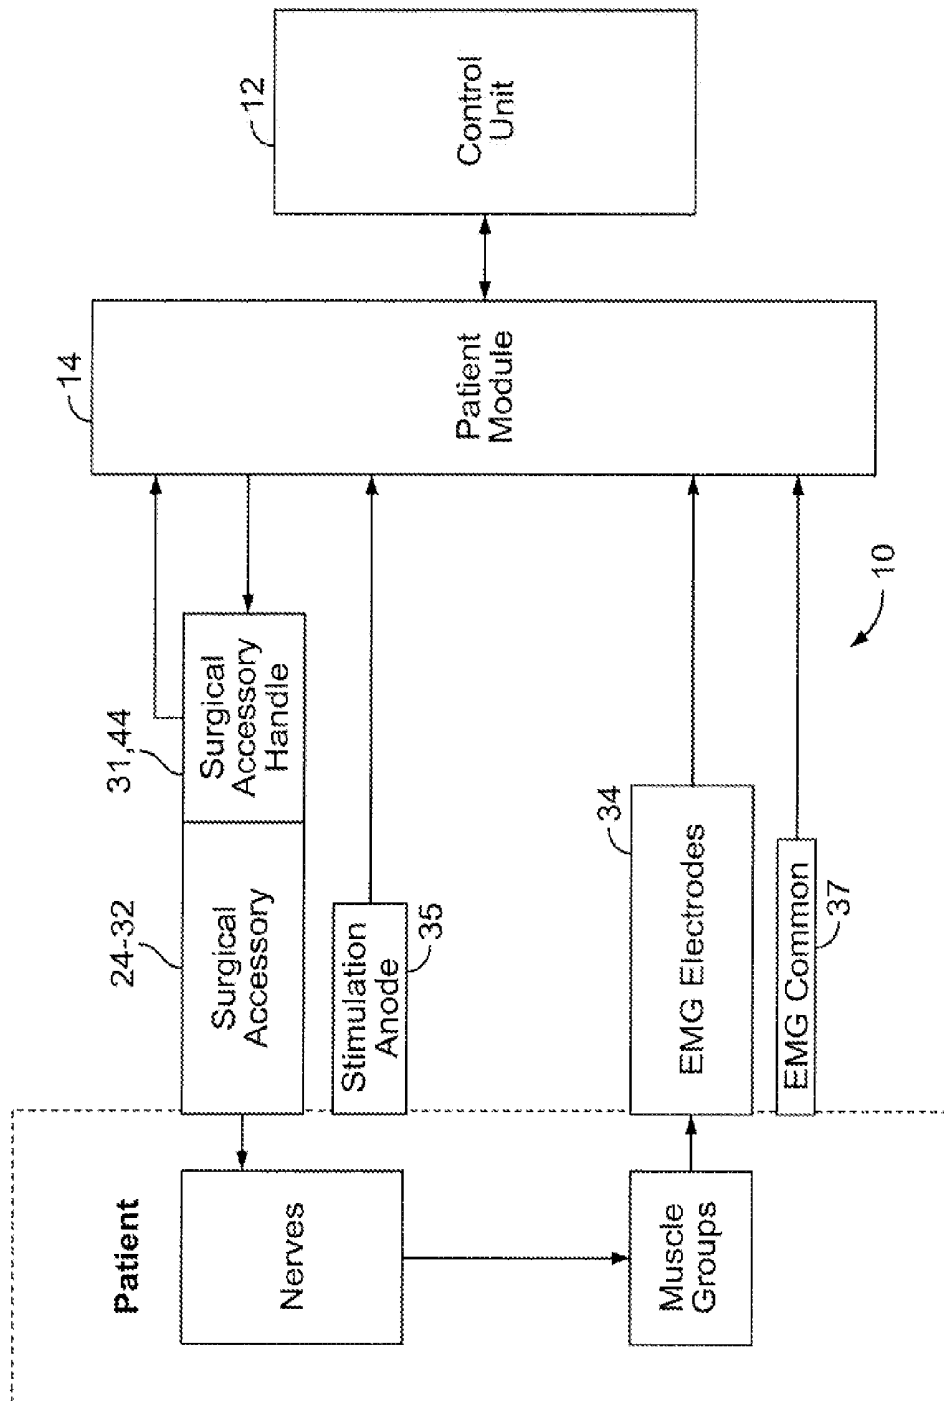


FIG. 2

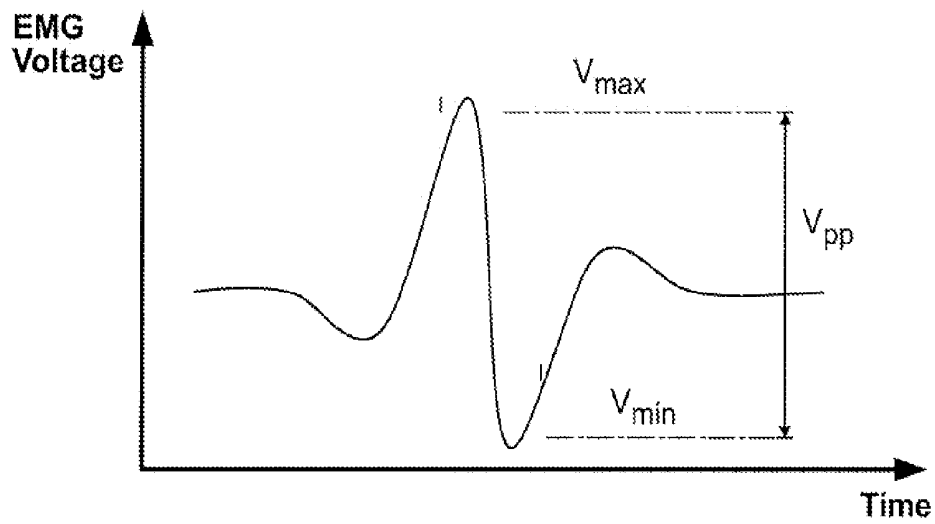


FIG. 3

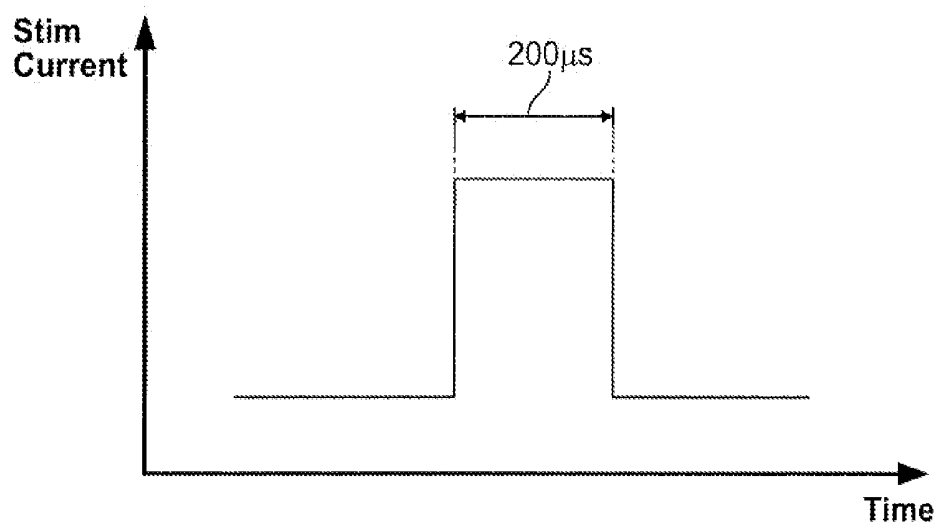


FIG. 4

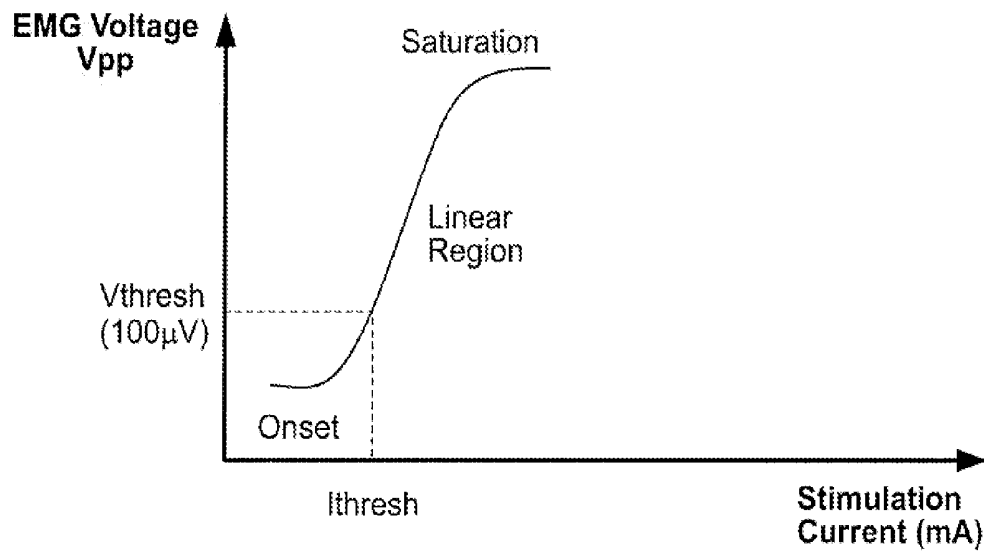


FIG. 5

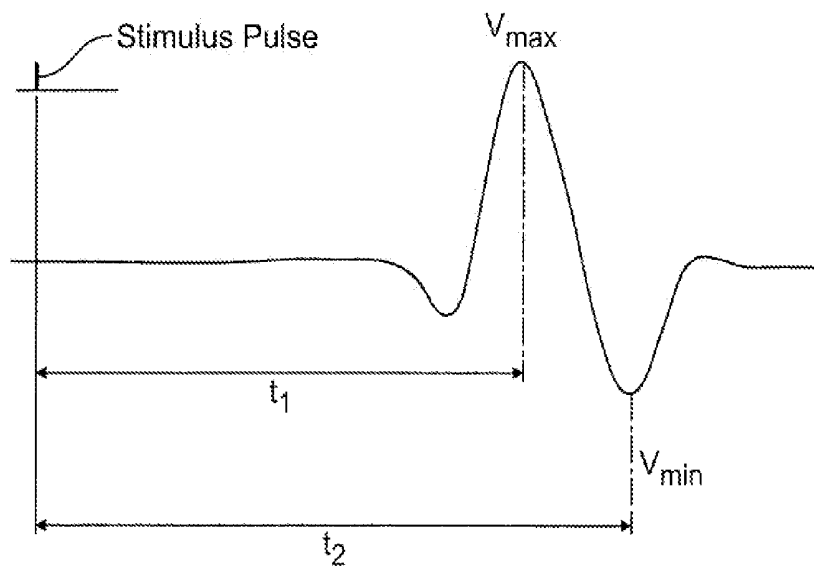


FIG. 6

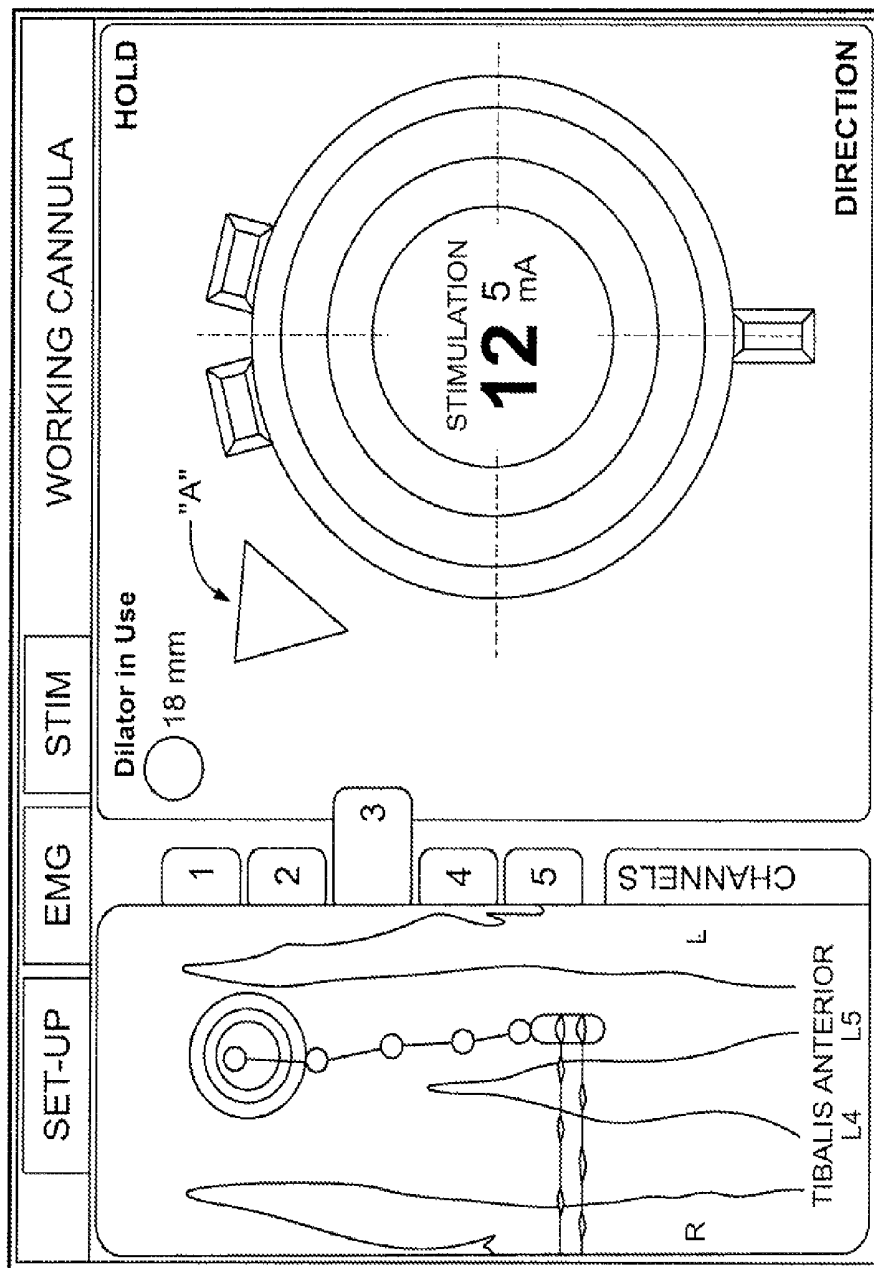


FIG. 7

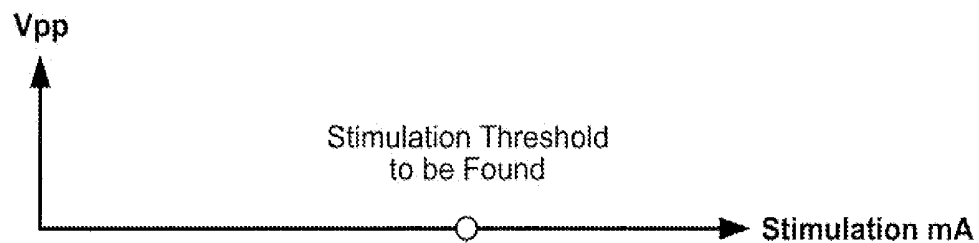


FIG. 8A

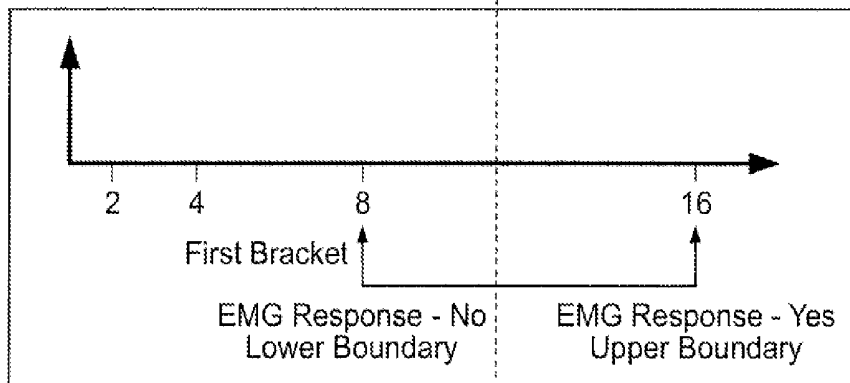


FIG. 8B

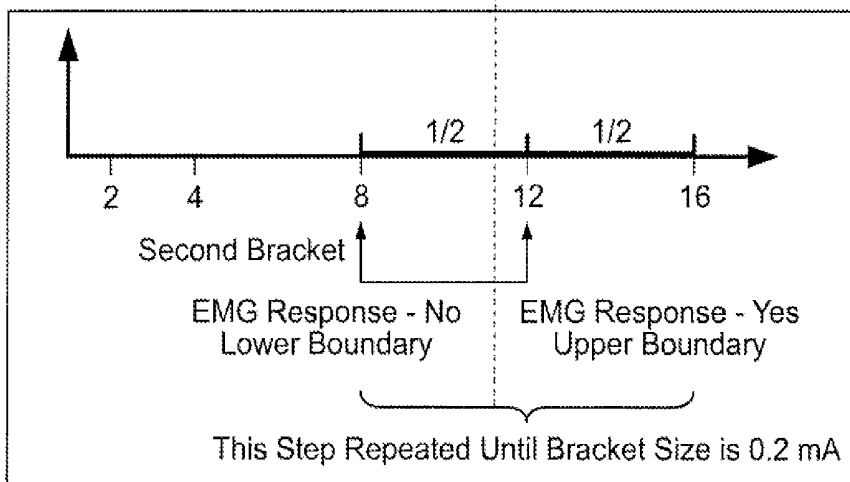


FIG. 8C






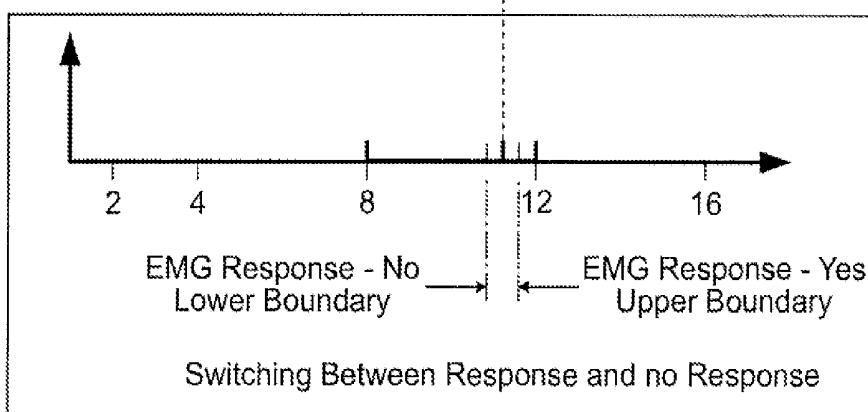


FIG. 8E

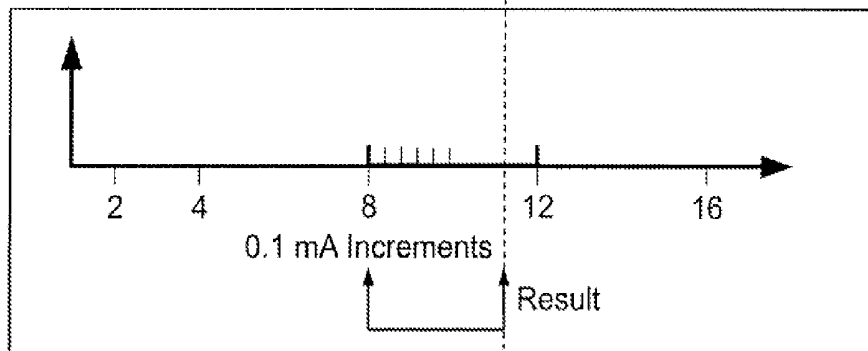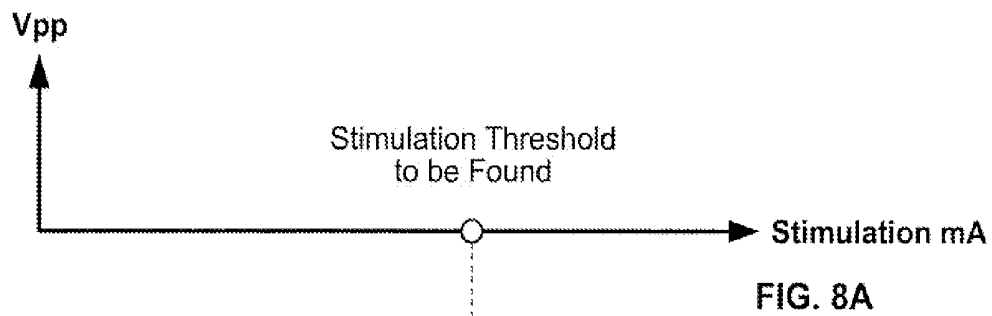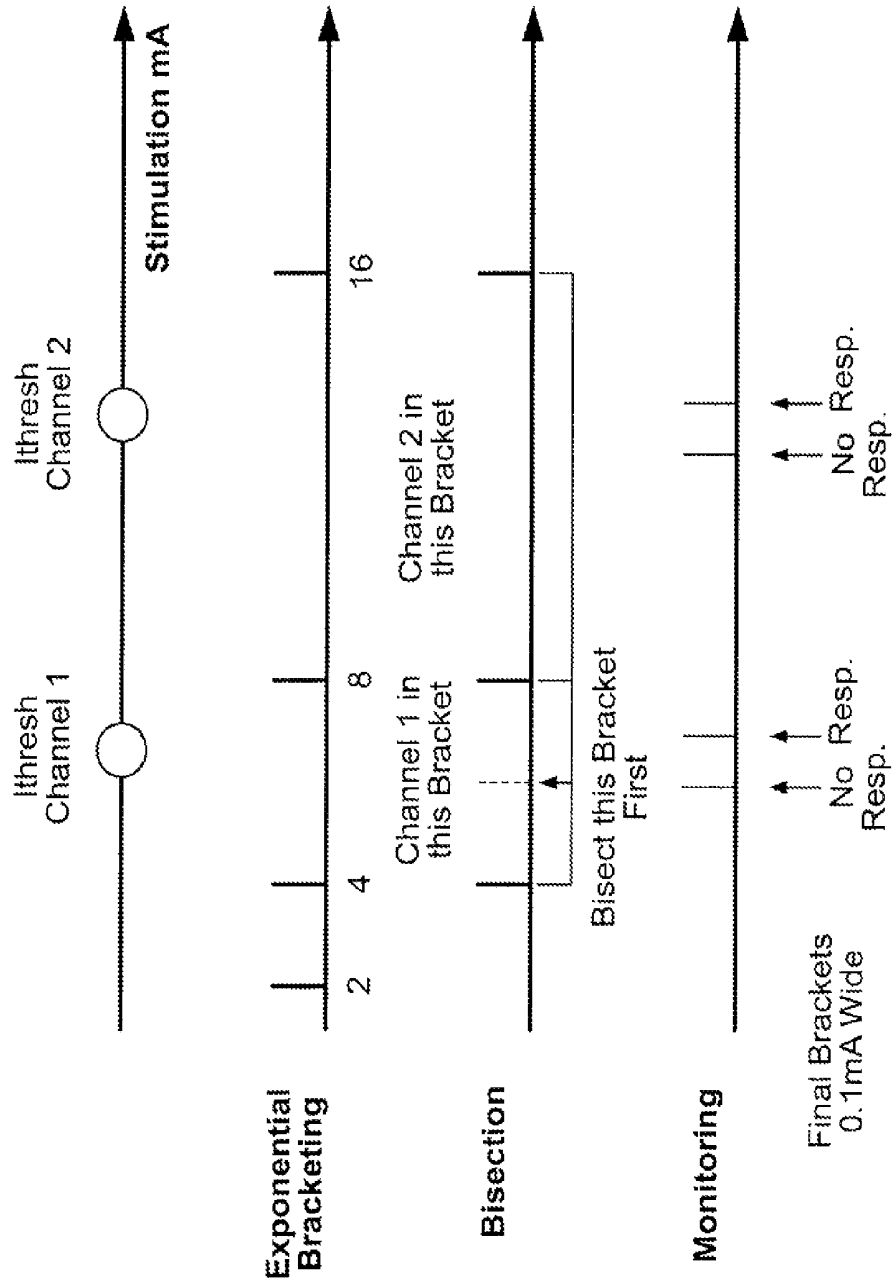

Note: not to scale

FIG. 9

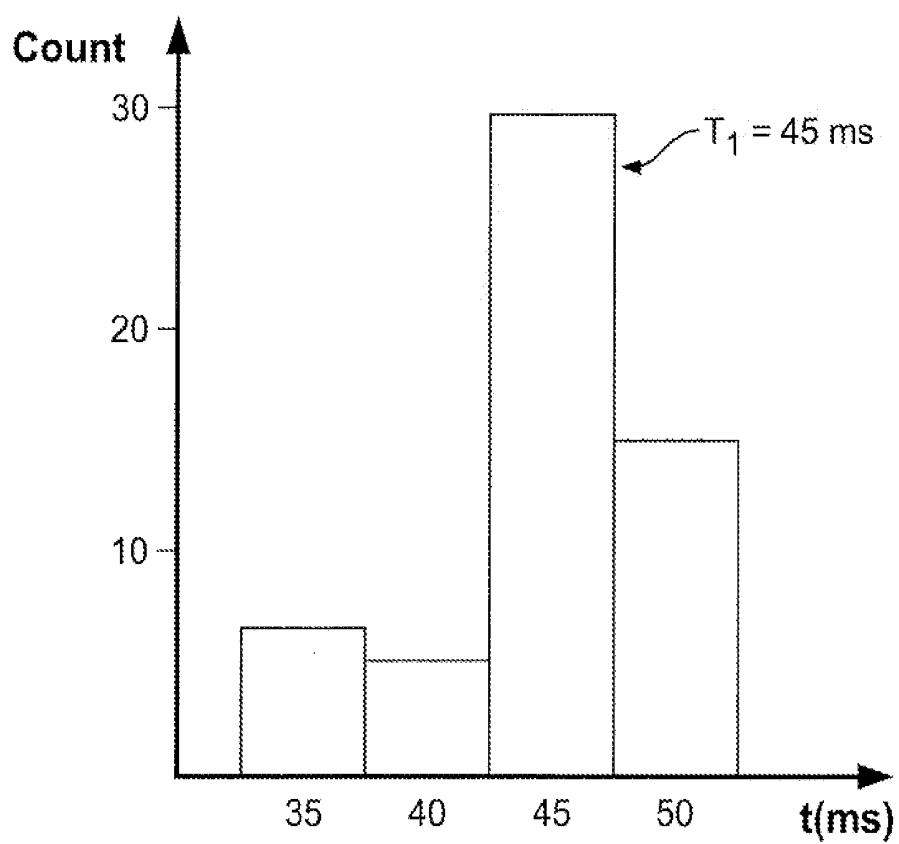


FIG. 10

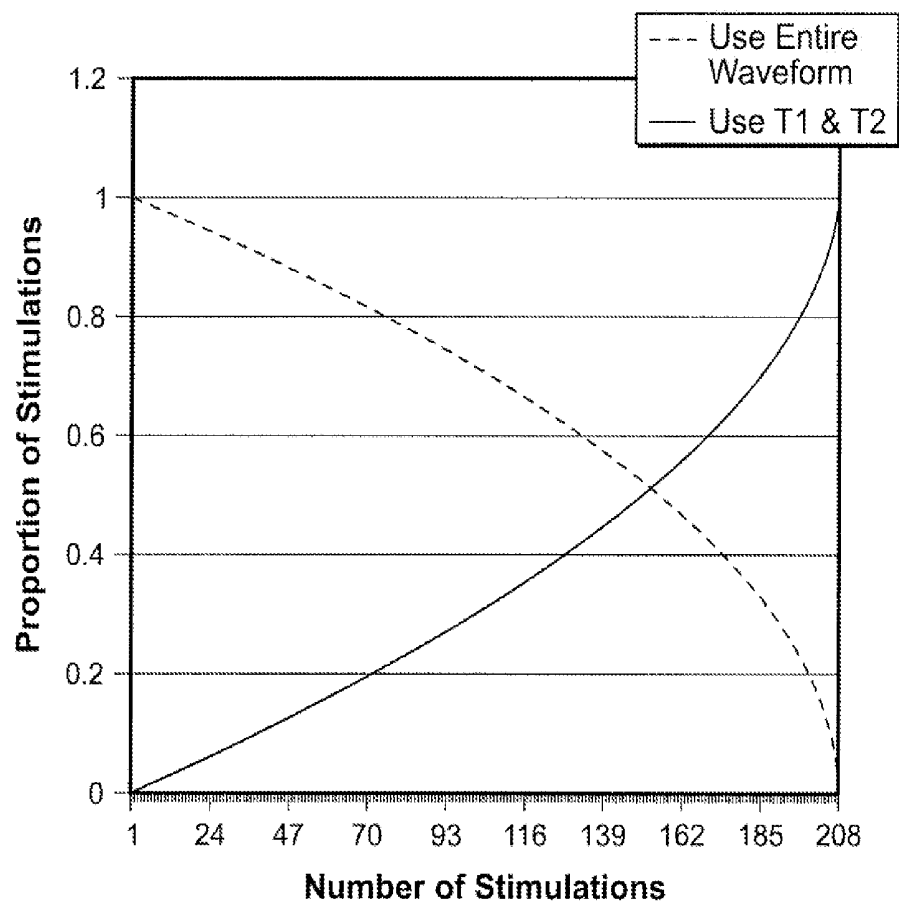


FIG. 11

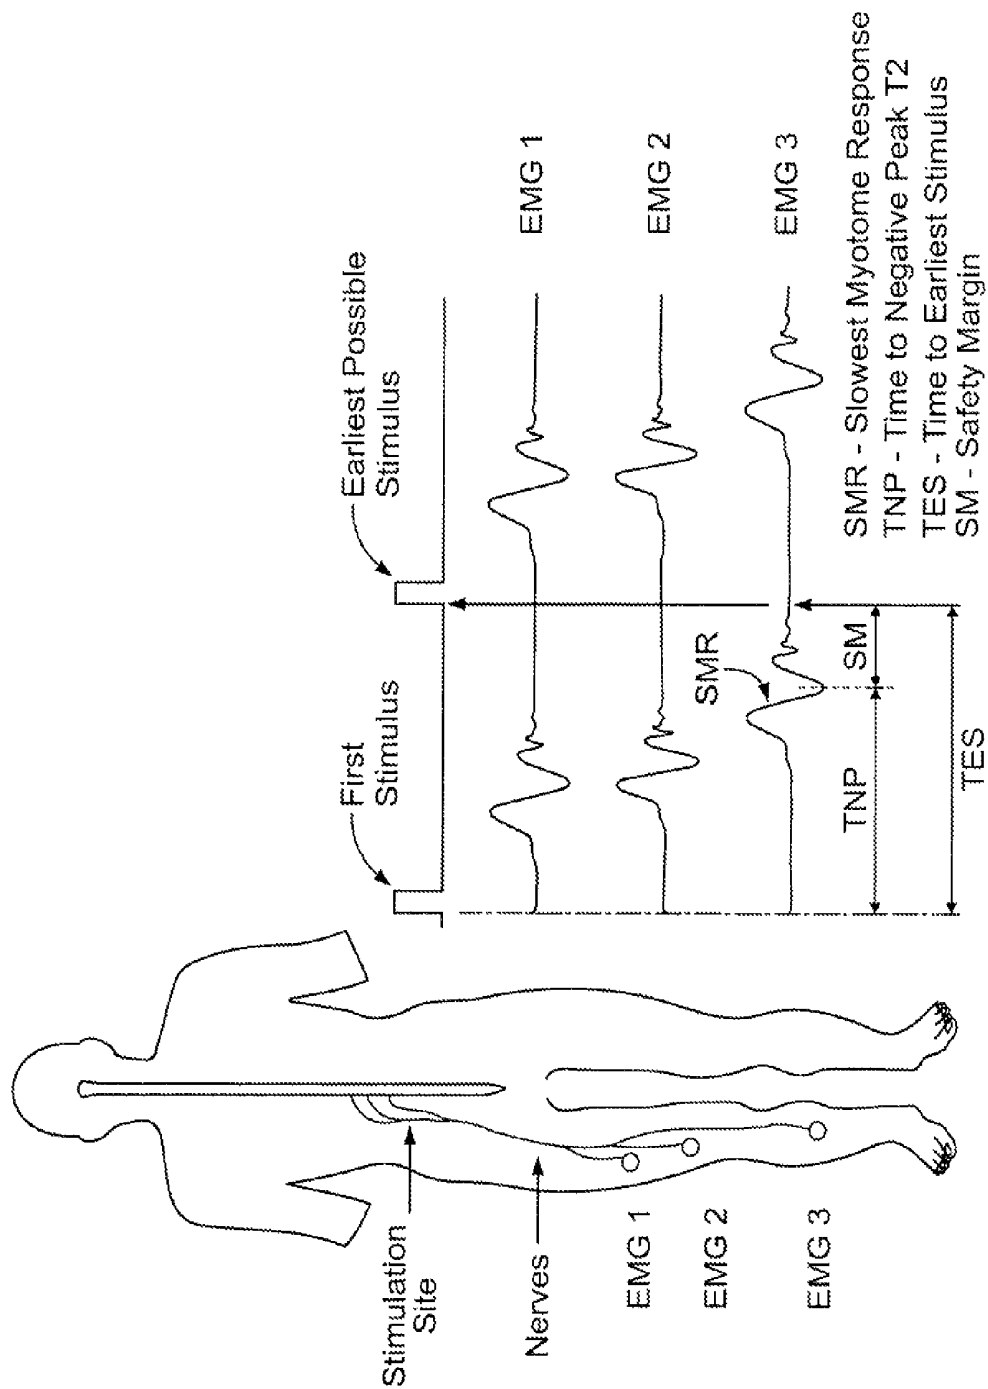


FIG. 12

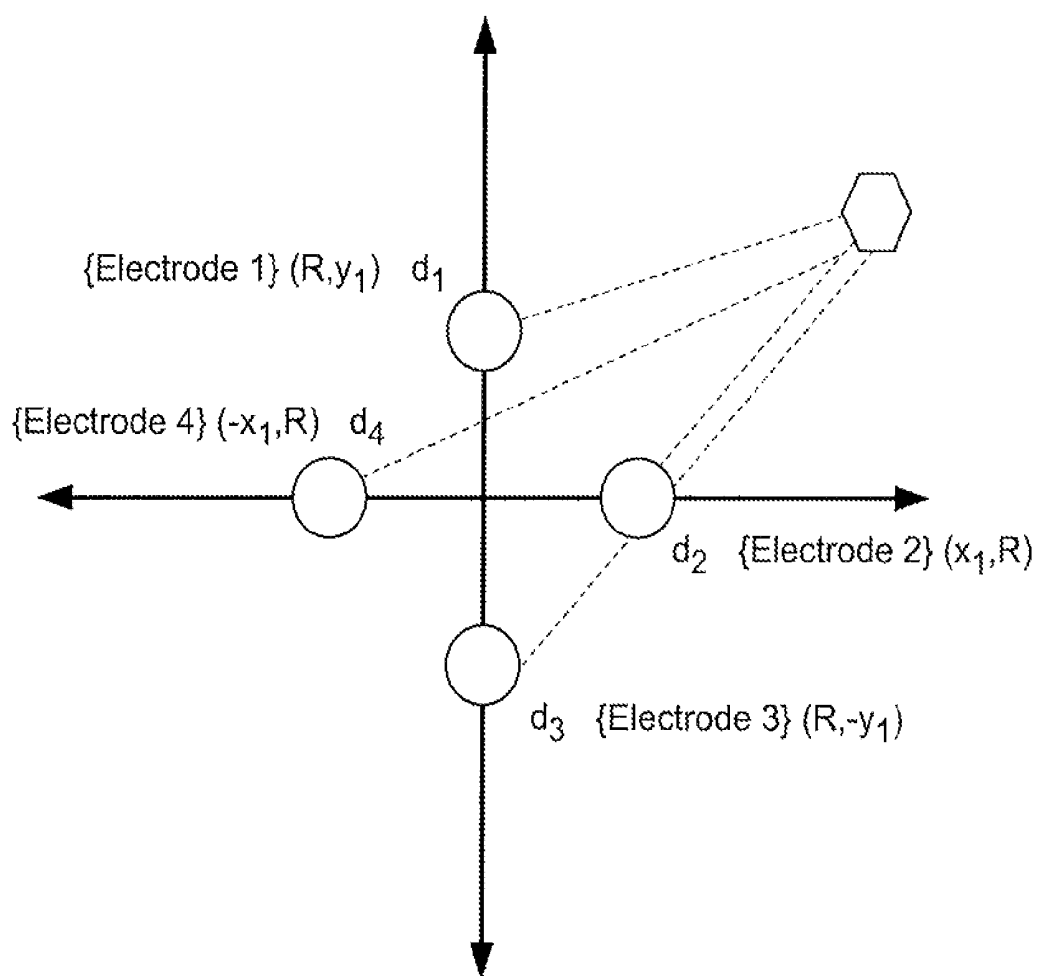


FIG. 13

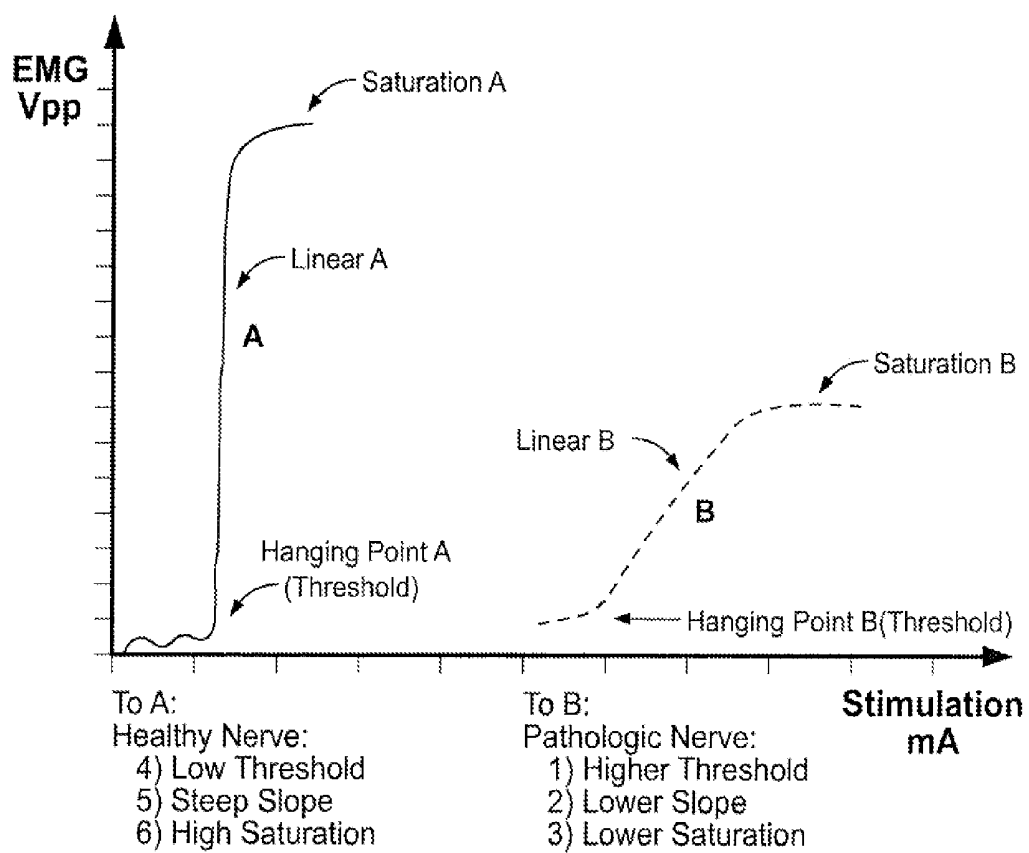


FIG. 14


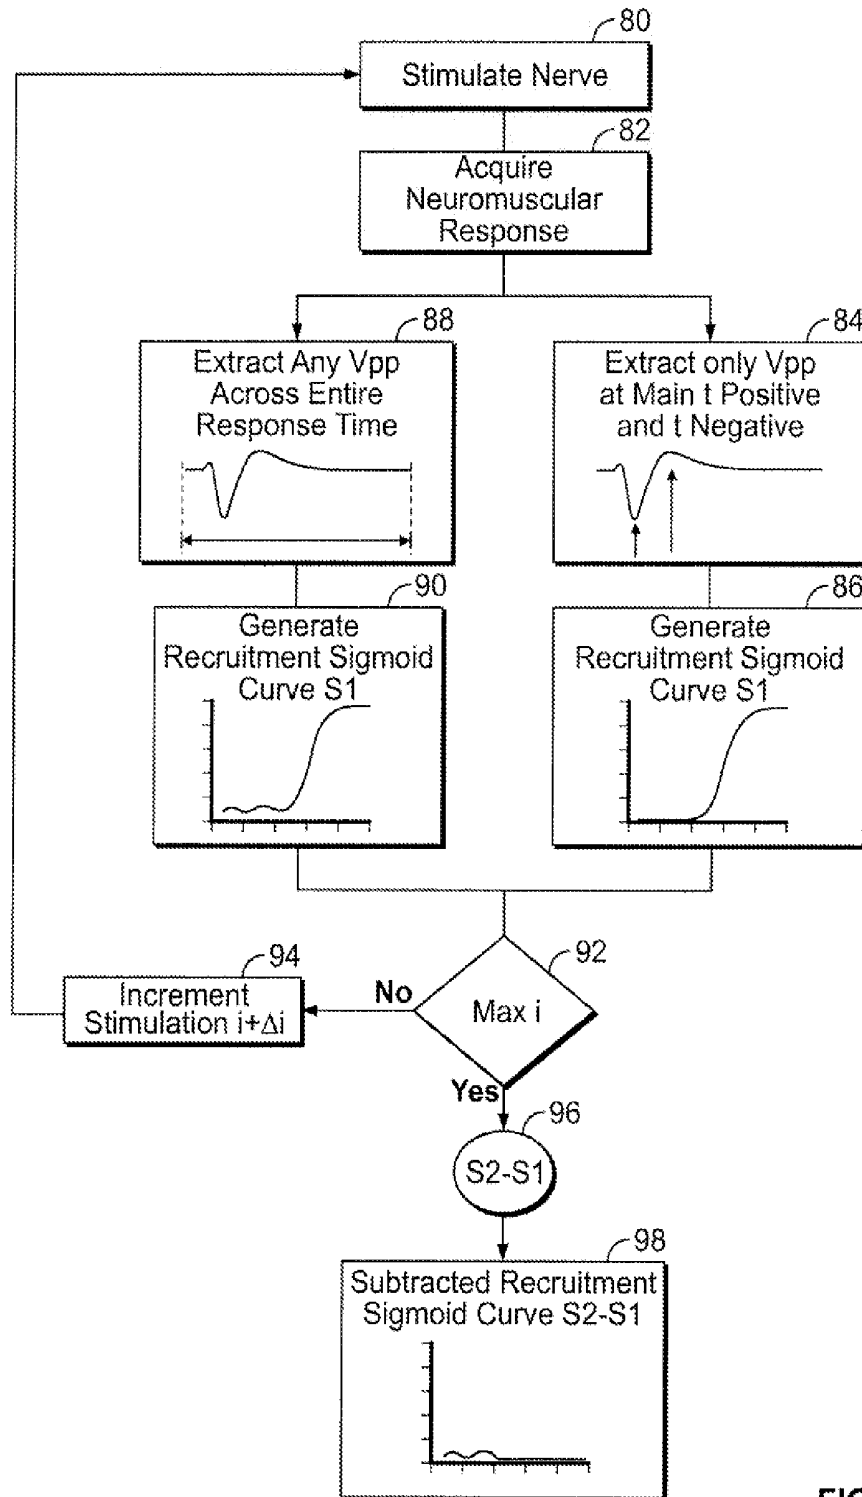


FIG. 15



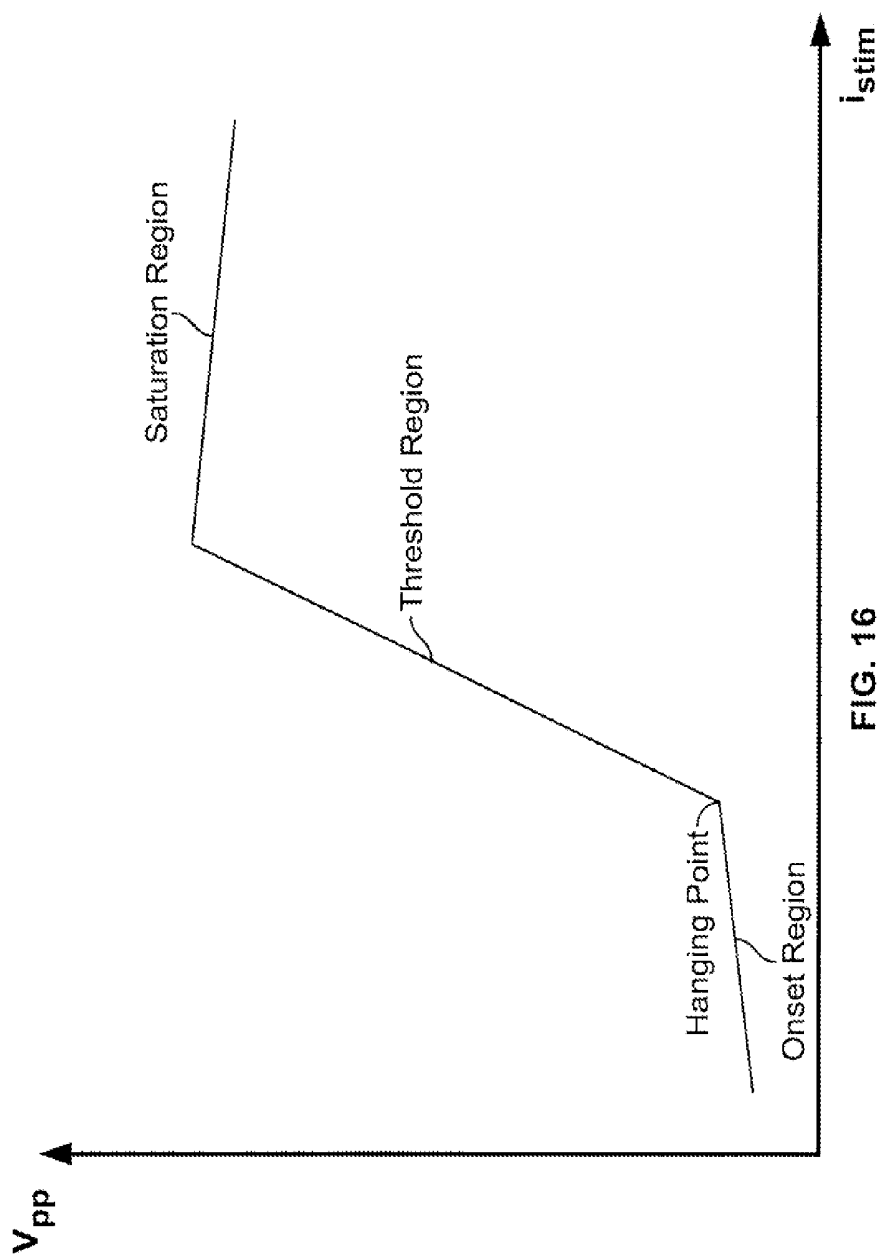

# SYSTEM AND METHODS FOR DETERMINING NERVE PROXIMITY, DIRECTION AND PATHOLOGY DURING SURGERY

## CROSS-REFERENCES TO RELATED APPLICATIONS

This application is a continuation of U.S. patent application Ser. No. 14/687,745 filed on Apr. 15, 2015, (the contents being incorporated herein by reference), which is a continuation of U.S. patent application Ser. No. 13/767,355 filed on Feb. 14, 2013, (the contents being incorporated herein by reference), which is a continuation of U.S. patent application Ser. No. 13/465,666 filed on May 7, 2012 (the contents being incorporated herein by reference), which is a continuation of U.S. patent application Ser. No. 13/292,065 filed on Nov. 8, 2011 (the contents being incorporated herein by reference), which is a continuation of U.S. patent application Ser. No. 13/080,493 (now U.S. Pat. No. 8,055,349) filed on Apr. 5, 2011 (the contents being incorporated herein by reference), which is a division of U.S. patent application Ser. No. 12/711,937 (now U.S. Pat. No. 7,920,922) filed on Feb. 24, 2010 (the contents being incorporated herein by reference), which is a continuation of U.S. patent application Ser. No. 10/754,899 (now U.S. Pat. No. 8,068,912) filed on Jan. 9, 2004 (the contents being incorporated herein by reference), which is a continuation of PCT Patent Application Ser. No. PCT/US02/22247 filed on Jul. 11, 2002 and published as WO03/005887 (the contents being incorporated herein by reference), which claims priority to U.S. Provisional Patent Application Ser. No. 60/305,041 filed Jul. 11, 2001 (the contents being incorporated herein by reference).

## BACKGROUND OF THE INVENTION

### I. Field of the Invention

This invention relates to nerve monitoring systems and to nerve muscle monitoring systems, and more particularly to systems and methods for determining nerve proximity, nerve direction, and pathology during surgery.

### II. Description of Related Art

Systems and methods exist for monitoring nerves and nerve muscles. One such system determines when a needle is approaching a nerve. The system applies a current to the needle to evoke a muscular response. The muscular response is visually monitored, typically as a shake or "twitch." When such a muscular response is observed by the user, the needle is considered to be near the nerve coupled to the responsive muscle. These systems require the user to observe the muscular response (to determine that the needle has approached the nerve). This may be difficult depending on the competing tasks of the user. In addition, when general anesthesia is used during a procedure, muscular response may be suppressed, limiting the ability of a user to detect the response.

While generally effective (although crude) in determining nerve proximity, such existing systems are incapable of determining the direction of the nerve to the needle or instrument passing through tissue or passing by the nerves. This can be disadvantageous in that, while the surgeon may appreciate that a nerve is in the general proximity of the instrument, the inability to determine the direction of the nerve relative to the instrument can lead to guess work by the surgeon in advancing the instrument and thereby raise the specter of inadvertent contact with, and possible damage to, the nerve.

Another nerve-related issue in existing surgical applications involves the use of nerve retractors. A typical nerve retractor serves to pull or otherwise maintain the nerve outside the area of surgery, thereby protecting the nerve from inadvertent damage or contact by the "active" instrumentation used to perform the actual surgery. While generally advantageous in protecting the nerve, it has been observed that such retraction can cause nerve function to become impaired or otherwise pathologic over time due to the retraction. In certain surgical applications, such as spinal surgery, it is not possible to determine if such retraction is hurting or damaging the retracted nerve until after the surgery (generally referred to as a change in "nerve health" or "nerve status"). There are also no known techniques or systems for assessing whether a given procedure is having a beneficial effect on a nerve or nerve root known to be pathologic (that is, impaired or otherwise unhealthy).

Based on the foregoing, a need exists for a better system and method that can determine the proximity of a surgical instrument (including but not limited to a needle, catheter, cannula, probe, or any other device capable of traversing through tissue or passing near nerves or nerve structures) to a nerve or group of nerves during surgery. A need also exists for a system and method for determining the direction of the nerve relative to the surgical instrument. A still further need exists for a manner of monitoring nerve health or status during surgical procedures.

The present invention is directed at eliminating, or at least reducing the effects of, the above-described problems with the prior art, as well as addressing the above-identified needs.

## SUMMARY OF THE INVENTION

The present invention includes a system and related methods for determining nerve proximity and nerve direction to surgical instruments employed in accessing a surgical target site, as well as monitoring the status or health (pathology) of a nerve or nerve root during surgical procedures.

According to a broad aspect, the present invention includes a surgical system, comprising a control unit and a surgical instrument. The control unit has at least one of computer programming software, firmware and hardware capable of delivering a stimulation signal, receiving and processing neuromuscular responses due to the stimulation signal, and identifying a relationship between the neuromuscular response and the stimulation signal. The surgical instrument has at least one stimulation electrode electrically coupled to said control unit for transmitting the stimulation signal, wherein said control unit is capable of determining at least one of nerve proximity, nerve direction, and nerve pathology relative to the surgical instrument based on the identified relationship between the neuromuscular response and the stimulation signal.

In a further embodiment of the surgical system of the present invention, the control unit is further equipped to communicate at least one of alpha-numeric and graphical information to a user regarding at least one of nerve proximity, nerve direction, and nerve pathology.

In a further embodiment of the surgical system of the present invention, the surgical instrument may comprise at least one of a device for maintaining contact with a nerve during surgery, a device for accessing a surgical target site, and a device for testing screw placement integrity.

In a further embodiment of the surgical system of the present invention, the surgical instrument comprises a nerve root retractor and wherein the control unit determines nerve

pathology based on the identified relationship between the neuromuscular response and the stimulation signal.

In a further embodiment of the surgical system of the present invention, the surgical instrument comprises a dilating instrument and wherein the control unit determines at least one of proximity and direction between a nerve and the instrument based on the identified relationship between the neuromuscular response and the stimulation signal.

In a further embodiment of the surgical system of the present invention, the dilating instrument comprises at least one of a K-wire, an obturator, a dilating cannula, and a working cannula.

In a further embodiment of the surgical system of the present invention, the surgical instrument comprises a screw test probe and wherein the control unit determines the proximity between the screw test probe and an exiting spinal nerve root to assess whether a medial wall of a pedicle has been breached by at least one of hole formation and screw placement.

### BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a perspective view of a surgical system 10 capable of determining, among other things, nerve proximity, direction, and pathology according to one aspect of the present invention;

FIG. 2 is a block diagram of the surgical system 10 shown in FIG. 1;

FIG. 3 is a graph illustrating a plot of the neuromuscular response (EMG) of a given myotome over time based on a current stimulation pulse (similar to that shown in FIG. 4) applied to a nerve bundle coupled to the given myotome;

FIG. 4 is a graph illustrating a plot of a stimulation current pulse capable of producing a neuromuscular response (EMG) of the type shown in FIG. 3;

FIG. 5 is a graph illustrating a plot of peak-to-peak voltage ( $V_{pp}$ ) for each given stimulation current level ( $I_{stim}$ ) forming a stimulation current pulse train according to the present invention (otherwise known as a “recruitment curve”);

FIG. 6 is a graph illustrating a plot of a neuromuscular response (EMG) over time (in response to a stimulus current pulse) showing the manner in which maximum voltage ( $V_{Max}$ ) and minimum voltage ( $V_{Min}$ ) occur at times T1 and T2, respectively;

FIG. 7 is an exemplary touch-screen display according to the present invention, capable of communicating a host of alpha-numeric and/or graphical information to a user and receiving information and/or instructions from the user during the operation of the surgical system 10 of FIG. 1;

FIGS. 8A-8E are graphs illustrating a rapid current threshold-hunting algorithm according to one embodiment of the present invention;

FIG. 9 is a series of graphs illustrating a multi-channel rapid current threshold-hunting algorithm according to one embodiment of the present invention;

FIG. 10 is a graph illustrating a T1, T2 artifact rejection technique according to one embodiment of the present invention via the use of histograms;

FIG. 11 is a graph illustrating the proportion of stimulations versus the number of stimulations employed in the T1, T2 artifact rejection technique according to the present invention;

FIG. 12 is an illustrating (graphical and schematic) of a method of automatically determining the maximum frequency ( $F_{Max}$ ) of the stimulation current pulses according to one embodiment of the present invention;

FIG. 13 is a graph illustrating a method of determining the direction of a nerve (denoted as an “octagon”) relative to an instrument having four (4) orthogonally disposed stimulation electrodes (denoted by the “circles”) according to one embodiment of the present invention;

FIG. 14 is a graph illustrating recruitment curves for a generally healthy nerve (denoted “A”) and a generally unhealthy nerve (denoted “B”) according to the nerve pathology determination method of the present invention;

FIG. 15 is flow chart illustrating an alternate method of determining the hanging point of a recruitment curve according to an embodiment of the present invention; and

FIG. 16 is a graph illustrating a simulated recruitment curve generated by a “virtual patient” device and method according to the present invention.

### DESCRIPTION OF THE SPECIFIC EMBODIMENTS

Illustrative embodiments of the invention are described below. In the interest of clarity, not all features of an actual implementation are described in this specification. It will of course be appreciated that in the development of any such actual embodiment, numerous implementation-specific decisions must be made to achieve the developers’ specific goals, such as compliance with system-related and business-related constraints, which will vary from one implementation to another. Moreover, it will be appreciated that such a development effort might be complex and time-consuming, but would nevertheless be a routine undertaking for those of ordinary skill in the art having the benefit of this disclosure. The systems disclosed herein boast a variety of inventive features and components that warrant patent protection, both individually and in combination.

FIG. 1 illustrates, by way of example only, a surgical system 10 capable of employing the nerve proximity, nerve direction, and nerve pathology assessments according to the present invention. As will be explained in greater detail below, the surgical system 10 is capable of providing safe and reproducible access to any number of surgical target sites, and well as monitoring changes in nerve pathology (health or status) during surgical procedures. It is expressly noted that, although described herein largely in terms of use in spinal surgery, the surgical system 10 and related methods of the present invention are suitable for use in any number of additional surgical procedures wherein tissue having significant neural structures must be passed through (or near) in order to establish an operative corridor, or where neural structures are retracted.

The surgical system 10 includes a control unit 12, a patient module 14, an EMG harness 16 and return electrode 35 coupled to the patient module 14, and a host of surgical accessories 20 capable of being coupled to the patient module 14 via one or more accessory cables 22. The surgical accessories 20 may include, but are not necessarily limited to, surgical access components (such as a K-wire 24, one or more dilating cannula 26, and a working cannula 28), neural pathology monitoring devices (such as nerve root retractor 30), and devices for performing pedicle screw test (such as screw test probe 32). A block diagram of the surgical system 10 is shown in FIG. 2, the operation of which is readily apparent in view of the following description.

The control unit 12 includes a touch screen display 36 and a base 38. The touch screen display 36 is preferably equipped with a graphical user interface (GUI) capable of communicating information to the user and receiving instructions from the user. The base 38 contains computer

hardware and software that commands the stimulation sources, receives digitized signals and other information from the patient module 14, and processes the EMG responses to extract characteristic information for each muscle group, and displays the processed data to the operator via the display 36. The primary functions of the software within the control unit 12 include receiving user commands via the touch screen display 36, activating stimulation in the requested mode (nerve proximity, nerve detection, nerve pathology, screw test), processing signal data according to defined algorithms (described below), displaying received parameters and processed data, and monitoring system status and report fault conditions.

The patient module 14 is connected via a serial cable 40 to the control unit 12, and contains the electrical connections to all electrodes, signal conditioning circuitry, stimulator drive and steering circuitry, and a digital communications interface to the control unit 12. In use, the control unit 12 is situated outside but close to the surgical field (such as on a cart adjacent the operating table) such that the display 36 is directed towards the surgeon for easy visualization. The patient module 14 should be located between the patient's legs, or may be affixed to the end of the operating table at mid-leg level using a bedrail clamp. The position selected should be such that the EMG leads can reach their farthest desired location without tension during the surgical procedure.

In a significant aspect of the present invention, the information displayed to the user on display 36 may include, but is not necessarily limited to, alpha-numeric and/or graphical information regarding nerve proximity, nerve direction, nerve pathology, stimulation level, myotome/EMG levels, screw testing, advance or hold instructions, and the instrument in use. In one embodiment (set forth by way of example only) the display includes the following components as set forth in Table 1:

TABLE 1

Screen Component	Description
Menu/Status Bar	The mode label may include the surgical accessory attached, such as the surgical access components (K-Wire, Dilating Cannula, Working Cannula), nerve pathology monitoring device (Nerve Root Retractor), and/or screw test device (Screw Test Probe) depending on which is attached.
Spine Image	An image of a human body/skeleton showing the electrode placement on the body, with labeled channel number tabs on each side (1-4 on left and right). Left and Right labels will show the patient orientation. The Channel number tabs may be highlighted or colored depending on the specific function being performed.
Display Area	Shows procedure-specific information.
Myotome & Level Names	A label to indicate the Myotome name and corresponding Spinal Level(s) associated with the channel of interest.
Advance/Hold	When in the Detection mode, an indication of "Advance" will show when it is safe to move the cannula forward (such as when the minimum stimulation current threshold $I_{Thresh}$ (described below) is greater than a predetermined value, indicating a safe distance to the nerve) and "Hold" will show when it is unsafe to advance the cannula (such as when the minimum stimulation current threshold $I_{Thresh}$ (described below) is less than a predetermined value, indicating that the nerve is relatively close to the cannula) and during proximity calculations.
Function	Indicates which function is currently active (Direction, Detection, Pathology Monitoring, Screw Test).

TABLE 1-continued

Screen Component	Description
Dilator In Use	A colored circle to indicate the inner diameter of the cannula, with the numeric size. If cannula is detached, no indicator is displayed.

The surgical system 10 accomplishes safe and reproducible access to a surgical target site by detecting the existence of (and optionally the distance and/or direction to) neural structures before, during, and after the establishment of an operative corridor through (or near) any of a variety of tissues having such neural structures which, if contacted or impinged, may otherwise result in neural impairment for the patient. The surgical system 10 does so by electrically stimulating nerves via one or more stimulation electrodes at the distal end of the surgical access components 24-28 while monitoring the EMG responses of the muscle groups innervated by the nerves. In a preferred embodiment, this is accomplished via 8 pairs of EMG electrodes 34 placed on the skin over the major muscle groups on the legs (four per side), an anode electrode 35 providing a return path for the stimulation current, and a common electrode 37 providing a ground reference to pre-amplifiers in the patient module 14. By way of example, the placement of EMG electrodes 34 may be undertaken according to the manner shown in Table 2 below for spinal surgery:

TABLE 2

Color	Channel ID	Myotome	Nerve	Spinal Level
Red	Right 1	Right Vastus Medialis	Femoral	L2, L3, L4
Orange	Right 2	Right Tibialis Anterior	Peroneal	L4, L5
Yellow	Right 3	Right Biceps Femoris	Sciatic	L5, S1, S2
Green	Right 4	Right Gastroc. Medial	Post Tibialis	S1, S2
Blue	Left 1	Left Vastus Medialis	Femoral	L2, L3, L4
Violet	Left 2	Left Tibialis Anterior	Peroneal	L4, L5
Gray	Left 3	Left Biceps Femoris	Sciatic	L5, S1, S2
White	Left 4	Left Gastroc. Medial	Post Tibialis	S1, S2

Although not shown, it will be appreciated that any of a variety of electrodes can be employed, including but not limited to needle electrodes. The EMG responses provide a quantitative measure of the nerve depolarization caused by the electrical stimulus. Analysis of the EMG responses is then used to determine the proximity and direction of the nerve to the stimulation electrode, as will be described with particularity below.

The surgical access components 24-28 are designed to bluntly dissect the tissue between the patient's skin and the surgical target site. An initial dilating cannula 26 is advanced towards the target site, preferably after having been aligned using any number of commercially available surgical guide frames. An obturator (not shown) may be included inside the initial dilator 26 and may similarly be equipped with one or more stimulating electrodes. Once the proper location is achieved, the obturator (not shown) may be removed and the K-wire 24 inserted down the center of the initial dilating cannula 26 and docked to the given surgical target site, such as the annulus of an intervertebral disc. Cannulae of increasing diameter are then guided over the previously installed cannula 26 until the desired lumen is installed. By way of example only, the dilating cannulae 26 may range in diameter from 6 mm to 30 mm. In one embodiment, each cannula 26 has four orthogonal stimulating electrodes at the tip to allow detection and direction evaluation, as will be

described below. The working cannula **28** is installed over the last dilating cannula **26** and then all the dilating cannulae **26** are removed from inside the inner lumen of the working cannula **28** to establish the operative corridor therethrough. A stimulator driver **42** is provided to electrically couple the particular surgical access component **24-28** to the patient module **14** (via accessory cable **22**). In a preferred embodiment, the stimulator driver **42** includes one or more buttons for selectively activating the stimulation current and/or directing it to a particular surgical access component.

The surgical system **10** accomplishes neural pathology monitoring by electrically stimulating a retracted nerve root via one or more stimulation electrodes at the distal end of the nerve root retractor **30** while monitoring the EMG responses of the muscle group innervated by the particular nerve. The EMG responses provide a quantitative measure of the nerve depolarization caused by the electrical stimulus. Analysis of the EMG responses may then be used to assess the degree to which retraction of a nerve or neural structure affects the nerve function over time, as will be described with greater particularity below. One advantage of such monitoring, by way of example only, is that the conduction of the nerve may be monitored during the procedure to determine whether the neurophysiology and/or function of the nerve changes (for the better or worse) as the result of the particular surgical procedure. For example, it may be observed that the nerve conduction increases as the result of the operation, indicating that the previously inhibited nerve has been positively affected by the operation. The nerve root retractor **30** may comprise any number of suitable devices capable of maintaining contact with a nerve or nerve root. The nerve root retractor **30** may be dimensioned in any number of different fashions, including having a generally curved distal region (shown as a side view in FIG. **1** to illustrate the concave region where the nerve will be positioned while retracted), and of sufficient dimension (width and/or length) and rigidity to maintain the retracted nerve in a desired position during surgery. The nerve root retractor **30** may also be equipped with a handle **31** having one or more buttons for selectively applying the electrical stimulation to the stimulation electrode(s) at the end of the nerve root retractor **30**. In one embodiment, the nerve root retractor **30** is disposable and the handle **31** is reusable and autoclavable.

The surgical system **10** can also be employed to perform screw test assessments via the use of screw test probe **32**. The screw test probe **32** is used to test the integrity of pedicle holes (after formation) and/or screws (after introduction). The screw test probe **32** includes a handle **44** and a probe member **46** having a generally ball-tipped end **48**. The handle **44** may be equipped with one or more buttons for selectively applying the electrical stimulation to the ball-tipped end **48** at the end of the probe member **46**. The ball tip **48** of the screw test probe **32** is placed in the screw hole prior to screw insertion or placed on the installed screw head. If the pedicle wall has been breached by the screw or tap, the stimulation current will pass through to the adjacent nerve roots and they will depolarize at a lower stimulation current.

Upon pressing the button on the screw test handle **44**, the software will execute an algorithm that results in all channel tabs being color-coded to indicate the detection status of the corresponding nerve. The channel with the "worst" (lowest) level will be highlighted (enlarged) and that myotome name will be displayed, as well as graphically depicted on the spine diagram. A vertical bar chart will also be shown, to depict the stimulation current required for nerve depolarization in mA for the selected channel. The screw test algorithm

preferably determines the depolarization (threshold) current for all 8 EMG channels. The surgeon may also set a baseline threshold current by stimulating a nerve root directly with the screw test probe **32**. The surgeon may choose to display the screw test threshold current relative to this baseline. The handle **44** may be equipped with a mechanism (via hardware and/or software) to identify itself to the system when it is attached. In one embodiment, the probe member **46** is disposable and the handle **44** is reusable and autoclavable.

An audio pick-up (not shown) may also be provided as an optional feature according to the present invention. In some cases, when a nerve is stretched or compressed, it will emit a burst or train of spontaneous nerve activity. The audio pick-up is capable of transmitting sounds representative of such activity such that the surgeon can monitor this response on audio to help him determine if there has been stress to the nerve.

Analysis of the EMG responses according to the present invention will now be described. The nerve proximity, nerve direction, and nerve pathology features of the present invention are based on assessing the evoked response of the various muscle myotomes monitored by the surgical system **10**. This is best shown in FIGS. **3-4**, wherein FIG. **3** illustrates the evoked response (EMG) of a monitored myotome to the stimulation current pulse shown in FIG. **4**. The EMG response can be characterized by a peak to peak voltage of  $V_{pp} = V_{max} - V_{min}$ . The stimulation current is preferably DC coupled and comprised of monophasic pulses of 200 microsecond duration with frequency and amplitude that is adjusted by the software. For each nerve and myotome there is a characteristic delay from the stimulation current pulse to the EMG response.

As shown in FIG. **5**, there is a threshold stimulation current required to depolarize the main nerve trunk. Below this threshold, current stimulation does not evoke a significant  $V_{pp}$  response. Once the stimulation threshold is reached, the evoked response is reproducible and increases with increasing stimulation, as shown in FIG. **5**. This is known as a "recruitment curve." In one embodiment, a significant  $V_{pp}$  is defined to be a minimum of 100  $\mu V$ . The lowest stimulation current that evoked this threshold voltage is called  $I_{thresh}$ .  $I_{thresh}$  decreases as the stimulation electrode approaches the nerve. This value is useful to surgeons because it provides a relative indication of distance (proximity) from the electrode to the nerve.

As shown in FIG. **6**, for each nerve/myotome combination there is a characteristic delay from the stimulation current pulse to the EMG response. For each stimulation current pulse, the time from the current pulse to the first max/min is  $T_1$  and to the second max/min is  $T_2$ . The first phase of the pulse may be positive or negative. As will be described below, the values of  $T_1$ ,  $T_2$  are each compiled into a histogram with bins as wide as the sampling rate. New values of  $T_1$ ,  $T_2$  are acquired with each stimulation and the histograms are continuously updated. The value of  $T_1$  and  $T_2$  used is the center value of the largest bin in the histogram. The values of  $T_1$ ,  $T_2$  are continuously updated as the histograms change. Initially  $V_{pp}$  is acquired using a window that contains the entire EMG response. After 20 samples, the use of  $T_1$ ,  $T_2$  windows is phased in over a period of 200 samples.  $V_{max}$  and  $V_{min}$  are then acquired only during windows centered around  $T_1$ ,  $T_2$  with widths of, by way of example only, 5 msec. This method of acquiring  $V_{pp}$  is advantageous in that it automatically performs artifact rejection (as will be described in greater detail below).

As will be explained in greater detail below, the use of the "recruitment curve" according to the present invention is

advantageous in that it provides a great amount of useful data from which to make various assessments (including, but not limited to, nerve detection, nerve direction, and nerve pathology monitoring). Moreover, it provides the ability to present simplified yet meaningful data to the user, as opposed to the actual EMG waveforms that are displayed to the users in traditional EMG systems. Due to the complexity in interpreting EMG waveforms, such prior art systems typically require an additional person specifically trained in such matters. This, in turn, can be disadvantageous in that it translates into extra expense (having yet another highly trained person in attendance) and oftentimes presents scheduling challenges because most hospitals do not retain such personnel. To account for the possibility that certain individuals will want to see the actual EMG waveforms, the surgical system 10 includes an Evoked Potentials display that shows the voltage waveform for all 8 EMG channels in real time. It shows the response of each monitored myotome to a current stimulation pulse. The display is updated each time there is a stimulation pulse. The Evoked Potentials display may be accessed during Detection, Direction, or Nerve Pathology Monitoring.

#### Nerve Detection (Proximity)

The Nerve Detection function of the present invention is used to detect a nerve with a stimulation electrode (i.e. those found on the surgical access components 24-28) and to give the user a relative indication of the proximity of the nerve to the electrode are advanced toward the surgical target site. A method of nerve proximity detection according one embodiment of the present invention is summarized as follows: (1) stimulation current pulses are emitted from the electrode with a fixed pulse width of 200  $\mu$ s and a variable amplitude; (2) the EMG response of the associated muscle group is measured; (3) the Vpp of the EMG response is determined using T1, T2, and Fmax (NB: before T2 is determined, a constant Fsafe is used for Fmax); (4) a rapid hunting detection algorithm is used to determine  $I_{Thresh}$  for a known Vthresh minimum; (5) the value of  $I_{Thresh}$  is displayed to the user as a relative indication of the proximity of the nerve, wherein the  $I_{Thresh}$  is expected to decrease as the probe gets closer to the nerve. A detailed description of the algorithms associated with the foregoing steps will follow after a general description of the manner in which this proximity information is communicated to the user.

The Detection Function displays the value of  $I_{Thresh}$  to the surgeon along with a color code so that the surgeon may use this information to avoid contact with neural tissues. This is shown generally in FIG. 7, which illustrates an exemplary screen display according to the present invention. Detection display is based on the amplitude of the current ( $I_{Thresh}$ ) required to evoke an EMG Vpp response greater than Vthresh (nominally 100  $\mu$ V). According to one embodiment, if  $I_{Thresh}$  is  $\leq 4$  mA red is displayed, the absolute value of  $I_{Thresh}$  is displayed. If  $4 \text{ mA} < I_{Thresh} < 10$  mA yellow is displayed. If  $I_{Thresh} \geq 10$  mA green is displayed. Normally,  $I_{Thresh}$  is only displayed when it is in the red range. However, the surgeon has the option of displaying  $I_{Thresh}$  for all three ranges (red, yellow, green). The maximum stimulation current is preferably set by the user and is preferably within the range of between 0-100 mA. Detection is performed on all 4 channels of the selected side. EMG channels on the opposite side are not used. The first dilator 26 may use an obturator having an electrode for stimulation. In one embodiment, all subsequent dilators 26 and the working cannula 28 use four electrodes for stimulation. The lowest value of  $I_{Thresh}$  from the 4 electrodes is used for display. There is an "Advance/Hold"

display that tells the surgeon when the calculations are finished and he may continue to advance the instrument.

The threshold-hunting algorithm employs a series of monopolar stimulations to determine the stimulation current threshold for each EMG channel that is in scope. The nerve is stimulated using current pulses with amplitude of  $I_{stim}$ . The muscle groups respond with an evoked potential that has a peak to peak voltage of Vpp. The object of this algorithm is to quickly find  $I_{Thresh}$ . This is the minimum  $I_{stim}$  that results in a Vpp that is greater than a known threshold voltage Vthresh. The value of  $I_{stim}$  is adjusted by a bracketing method as follows. The first bracket is 0.2 mA and 0.3 mA. If the Vpp corresponding to both of these stimulation currents is lower than Vthresh, then the bracket size is doubled to 0.2 mA and 0.4 mA. This exponential doubling of the bracket size continues until the upper end of the bracket results in a Vpp that is above Vthresh. The size of the brackets is then reduced by a bisection method. A current stimulation value at the midpoint of the bracket is used and if this results in a Vpp that is above Vthresh, then the lower half becomes the new bracket. Likewise, if the midpoint Vpp is below Vthresh then the upper half becomes the new bracket. This bisection method is used until the bracket size has been reduced to Ires mA.  $I_{Thresh}$  is the value of  $I_{stim}$  that is the higher end of the bracket.

More specifically, with reference to FIGS. 8A-8E, the threshold hunting will support three states: bracketing, bisection, and monitoring. A stimulation current bracket is a range of stimulation currents that bracket the stimulation current threshold  $I_{Thresh}$ . The upper and/or lower boundaries of a bracket may be indeterminate. The width of a bracket is the upper boundary value minus the lower boundary value. If the stimulation current threshold  $I_{Thresh}$  of a channel exceeds the maximum stimulation current, that threshold is considered out-of-range. During the bracketing state, threshold hunting will employ the method below to select stimulation currents and identify stimulation current brackets for each EMG channel in scope.

The method for finding the minimum stimulation current uses the methods of bracketing and bisection. The "root" is identified for a function that has the value -1 for stimulation currents that do not evoke adequate response; the function has the value +1 for stimulation currents that evoke a response. The root occurs when the function jumps from -1 to +1 as stimulation current is increased: the function never has the value of precisely zero. The root will not be known precisely, but only with some level of accuracy. The root is found by identifying a range that must contain the root. The upper bound of this range is the lowest stimulation current  $I_{Thresh}$  where the function returns the value +1, i.e. the minimum stimulation current that evokes response.

The proximity function begins by adjusting the stimulation current until the root is bracketed (FIG. 8B). The initial bracketing range may be provided in any number of suitable ranges. In one embodiment, the initial bracketing range is 0.2 to 0.3 mA. If the upper stimulation current does not evoke a response, the upper end of the range should be increased. The range scale factor is 2. The stimulation current should never be increased by more than 10 mA in one iteration. The stimulation current should never exceed the programmed maximum stimulation current. For each stimulation, the algorithm will examine the response of each active channel to determine whether it falls within that bracket. Once the stimulation current threshold of each channel has been bracketed, the algorithm transitions to the bisection state.

During the bisection state (FIGS. 8C and 8D), threshold hunting will employ the method described below to select stimulation currents and narrow the bracket to a width of 0.1 mA for each EMG channel with an in-range threshold. After the minimum stimulation current has been bracketed (FIG. 8B), the range containing the root is refined until the root is known with a specified accuracy. The bisection method is used to refine the range containing the root. In one embodiment, the root should be found to a precision of 0.1 mA. During the bisection method, the stimulation current at the midpoint of the bracket is used. If the stimulation evokes a response, the bracket shrinks to the lower half of the previous range. If the stimulation fails to evoke a response, the bracket shrinks to the upper half of the previous range. The proximity algorithm is locked on the electrode position when the response threshold is bracketed by stimulation currents separated by 0.1 mA. The process is repeated for each of the active channels until all thresholds are precisely known. At that time, the algorithm enters the monitoring state.

During the monitoring state (FIG. 8E), threshold hunting will employ the method described below to select stimulation currents and identify whether stimulation current thresholds are changing. In the monitoring state, the stimulation current level is decremented or incremented by 0.1 mA, depending on the response of a specific channel. If the threshold has not changed then the lower end of the bracket should not evoke a response, while the upper end of the bracket should. If either of these conditions fail, the bracket is adjusted accordingly. The process is repeated for each of the active channels to continue to assure that each threshold is bracketed. If stimulations fail to evoke the expected response three times in a row, then the algorithm transitions back to the bracketing state in order to reestablish the bracket.

When it is necessary to determine the stimulation current thresholds ( $I_r$ ) for more than one channel, they will be obtained by time-multiplexing the threshold-hunting algorithm as shown in FIG. 9. During the bracketing state, the algorithm will start with a stimulation current bracket of 0.2 mA and increase the size of the bracket exponentially. With each bracket, the algorithm will measure the  $V_{pp}$  of all channels to determine which bracket they fall into. After this first pass, the algorithm will know which exponential bracket contains the  $I_r$  for each channel. Next, during the bisection state, the algorithm will start with the lowest exponential bracket that contains an  $I_r$  and bisect it until  $I_r$  is found within 0.1 mA. If there are more than one  $I_r$  within an exponential bracket, they will be separated out during the bisection process, and the one with the lowest value will be found first. During the monitoring state, the algorithm will monitor the upper and lower boundaries of the brackets for each  $I_r$ , starting with the lowest. If the  $I_r$  for one or more channels is not found in its bracket, then the algorithm goes back to the bracketing state to re-establish the bracket for those channels.

The method of performing automatic artifact rejection according to the present invention will now be described. As noted above, acquiring  $V_{pp}$  according to the present invention (based on T1, T2 shown in FIG. 6) is advantageous in that, among other reasons, it automatically performs artifact rejection. The nerve is stimulated using a series of current pulses above the stimulation threshold. The muscle groups respond with an evoked potential that has a peak to peak voltage of  $V_{pp}$ . For each EMG response pulse, T1 is the time is measured from the stimulus pulse to the first extremum ( $V_{max}$  or  $V_{min}$ ). T2 is the time measured from the current

pulse to the second extremum ( $V_{max}$  or  $V_{min}$ ). The values of T1 and T2 are each compiled into a histogram with Tbin msec bin widths. The value of T1 and T2 used for artifact rejection is the center value of the largest bin in the histogram. To reject artifacts when acquiring the EMG response,  $V_{max}$  and  $V_{min}$  are acquired only during windows that are  $T1 \pm T_{win}$  and  $T2 \pm T_{win}$ . Again, with reference to FIG. 6,  $V_{pp}$  is  $V_{max} - V_{min}$ .

The method of automatic artifact rejection is further explained with reference to FIG. 10. While the threshold hunting algorithm is active, after each stimulation, the following steps are undertaken for each EMG sensor channel that is in scope: (1) the time sample values for the waveform maximum and minimum (after stimulus artifact rejection) will be placed into a histogram; (2) the histogram bin size will be the same granularity as the sampling period; (3) the histogram will be emptied each time the threshold hunting algorithm is activated; (4) the histogram will provide two peaks, or modes, defined as the two bins with the largest counts; (5) the first mode is defined as T1; the second mode is defined as T2; (6) a (possibly discontinuous) range of waveform samples will be identified; (7) for the first stimulation after the threshold hunting algorithm is activated, the range of samples will be the entire waveform; (8) after a specified number of stimulations, the range of samples will be limited to  $T1 \pm 0.5$  ms and  $T2 \pm 0.5$  ms; and (9) before the specified number of stimulations, either range may be used, subject to this restriction: the proportion of stimulations using the entire waveform will decrease from 100% to 0% (a sample of the curve governing this proportion is shown in FIG. 11). Peak-to-peak voltage ( $V_{pp}$ ) will be measured either over the identified range of waveform samples. The specified number of stimulations will preferably be between 220 and 240.

According to another aspect of the present invention, the maximum frequency of the stimulation pulses is automatically obtained with reference to FIG. 12. After each stimulation,  $F_{max}$  will be computed as:  $F_{max} = 1 / (T2 + \text{Safety Margin})$  for the largest value of T2 from each of the active EMG channels. In one embodiment, the Safety Margin is 5 ms, although it is contemplated that this could be varied according to any number of suitable durations. Before the specified number of stimulations, the stimulations will be performed at intervals of 100-120 ms during the bracketing state, intervals of 200-240 ms during the bisection state, and intervals of 400-480 ms during the monitoring state. After the specified number of stimulations, the stimulations will be performed at the fastest interval practical (but no faster than  $F_{max}$ ) during the bracketing state, the fastest interval practical (but no faster than  $F_{max}/2$ ) during the bisection state, and the fastest interval practical (but no faster than  $F_{max}/4$ ) during the monitoring state. The maximum frequency used until  $F_{max}$  is calculated is preferably 10 Hz, although slower stimulation frequencies may be used during some acquisition algorithms. The value of  $F_{max}$  used is periodically updated to ensure that it is still appropriate. This feature is represented graphically, by way of example only, in FIG. 12. For physiological reasons, the maximum frequency for stimulation will be set on a per-patient basis. Readings will be taken from all myotomes and the one with the slowest frequency (highest T2) will be recorded.

#### Nerve Direction

Once a nerve is detected using the working cannula 28 or dilating cannulae 26, the surgeon may use the Direction Function to determine the angular direction to the nerve relative to a reference mark on the access components 24-28. This is also shown in FIG. 7 as the arrow A pointing to the

direction of the nerve. This information helps the surgeon avoid the nerve as he or she advances the cannula. The direction from the cannula to a selected nerve is estimated using the 4 orthogonal electrodes on the tip of the dilating cannula 26 and working cannulae 28. These electrodes are preferably scanned in a monopolar configuration (that is, using each of the 4 electrodes as the stimulation source). The nerve's threshold current ( $I_{thresh}$ ) is found for each of the electrodes by measuring the muscle evoked potential response  $V_{pp}$  and comparing it to a known threshold  $V_{thresh}$ . This algorithm is used to determine the direction from a stimulation electrode to a nerve.

As shown in FIG. 13, the four (4) electrodes are placed on the x and y axes of a two dimensional coordinate system at radius R from the origin. A vector is drawn from the origin along the axis corresponding to each electrode that has a length equal to  $I_{Thresh}$  for that electrode. The vector from the origin to a direction pointing toward the nerve is then computed. This algorithm employs the T1/T2 algorithm discussed above with reference to FIG. 6. Using the geometry shown in FIG. 10, the (x,y) coordinates of the nerve, taken as a single point, can be determined as a function of the distance from the nerve to each of four electrodes. This can be expressly mathematically as follows:

Where the "circles" denote the position of the electrode respective to the origin or center of the cannula and the "octagon" denotes the position of a nerve, and  $d_1$ ,  $d_2$ ,  $d_3$ , and  $d_4$  denote the distance between the nerve and electrodes 1-4 respectively, it can be shown that:

$$x = \frac{d_1^2 - d_3^2}{-4R} \text{ and } y = \frac{d_2^2 - d_4^2}{-4R}$$

Where R is the cannula radius, standardized to 1, since angles and not absolute values are measured.

After conversion from (x,y) to polar coordinates (r,θ), then θ is the angular direction to the nerve. This angular direction is then displayed to the user as shown in FIG. 7, by way of example only, as arrow A pointing towards the nerve. In this fashion, the surgeon can actively avoid the nerve, thereby increasing patient safety while accessing the surgical target site. The surgeon may select any one of the 4 channels available to perform the Direction Function. The surgeon should preferably not move or rotate the instrument while using the Direction Function, but rather should return to the Detection Function to continue advancing the instrument.

Insertion and advancement of the access instruments 24-28 should be performed at a rate sufficiently slow to allow the surgical system 10 to provide real-time indication of the presence of nerves that may lie in the path of the tip. To facilitate this, the threshold current  $I_{Thresh}$  may be displayed such that it will indicate when the computation is finished and the data is accurate. For example, when the detection information is up to date and the instrument such that it is now ready to be advanced by the surgeon, it is contemplated to have the color display show up as saturated to communicate this fact to the surgeon. During advancement of the instrument, if a channel's color range changes from green to yellow, advancement should proceed more slowly, with careful observation of the detection level. If the channel color stays yellow or turns green after further advancement, it is a possible indication that the instrument tip has passed, and is moving farther away from the nerve. If after further advancement, however, the channel color

turns red, then it is a possible indication that the instrument tip has moved closer to a nerve. At this point the display will show the value of the stimulation current threshold in mA. Further advancement should be attempted only with extreme caution, while observing the threshold values, and only if the clinician deems it safe. If the clinician decides to advance the instrument tip further, an increase in threshold value (e.g. from 3 mA to 4 mA) may indicate the Instrument tip has safely passed the nerve. It may also be an indication that the instrument tip has encountered and is compressing the nerve. The latter may be detected by listening for sporadic outbursts, or "pops", of nerve activity on the free running EMG audio output (as mentioned above). If, upon further advancement of the instrument, the alarm level decreases (e.g., from 4 mA to 3 mA), then it is very likely that the instrument tip is extremely close to the spinal nerve, and to avoid neural damage, extreme caution should be exercised during further manipulation of the Instrument. Under such circumstances, the decision to withdraw, reposition, or otherwise maneuver the instrument is at the sole discretion of the clinician based upon available information and experience. Further radiographic imaging may be deemed appropriate to establish the best course of action.

#### Nerve Pathology

As noted above, the surgical system 10 accomplishes neural pathology monitoring by electrically stimulating a retracted nerve root via one or more stimulation electrodes at the distal end of the nerve root retractor 30 while monitoring the EMG responses of the muscle group innervated by the particular nerve. FIG. 14 shows the differences between a healthy nerve (A) and a pathologic or unhealthy nerve (B). The inventors have found through experimentation that information regarding nerve pathology (or "health" of "status") can be extracted from the recruitment curves generated according to the present invention (see, e.g., discussion accompanying FIGS. 3-5). In particular, it has been found that a health nerve or nerve bundle will produce a recruitment curve having a generally low threshold or "hanging point" (in terms of both the y-axis or  $V_{pp}$  value and the x-axis or  $I_{stim}$  value), a linear region having a relatively steep slope, and a relatively high saturation region (similar to those shown on recruitment curve "A" in FIG. 14). On the contrary, a nerve or nerve bundle that is unhealthy or whose function is otherwise compromised or impaired (such as being impinged by spinal structures or by prolonged retraction) will produce recruitment curve having a generally higher threshold (again, in terms of both the y-axis or  $V_{pp}$  value and the x-axis or  $I_{stim}$  value), a linear region of reduced slope, and a relatively low saturation region (similar to those shown on recruitment curve "B" in FIG. 14). By recognizing these characteristics, one can monitor nerve root being retracted during a procedure to determine if its pathology or health is affected (i.e. negatively) by such retraction. Moreover, one can monitor a nerve root that has already been deemed pathologic or unhealthy before the procedure (such as may be caused by being impinged by bony structures or a bulging annulus) to determine if its pathology or health is affected (i.e. positively) by the procedure.

The surgical system 10 and related methods have been described above according to one embodiment of the present invention. It will be readily appreciated that various modifications may be undertaken, or certain steps or algorithms omitted or substituted, without departing from the scope of the present invention. By way of example only, certain of these alternate embodiments or methods will be described below.



## a. Hanging Point Detection Via Linear Regression

As opposed to identifying the stimulation current threshold ( $I_{Thresh}$ ) based on a predetermined  $V_{Thresh}$  (such as described above and shown in FIG. 5), it is also within the scope of the present invention to determine  $I_{Thresh}$  via linear regression. This may be accomplished via, by way of example only, the linear regression technique disclosed in commonly owned U.S. patent application Ser. No. 09/877, 713 (now U.S. Pat. No. 6,500,128), filed Jun. 8, 2001 and entitled "Relative Nerve Movement and Status Detection System and Methods," the entire contents of which is hereby expressly incorporated by reference as if set forth in this disclosure in its entirety.

## b. Hanging Point Detection Via Dynamic Sweep Subtraction

With reference to FIG. 15, the hanging point or threshold may also be determined by the following dynamic sweep subtraction method. The nerve is stimulated in step 80 using current pulses that increase from  $I_{Min}$  to  $I_{Max}$  (as described above). The resulting the neuromuscular response (evoked EMG) for the associated muscles group is acquired in step 82. The peak-to-peak voltage ( $V_{pp}$ ) is then extracted in step 84 for each current pulse according to the T1, T2 algorithm described above with reference to FIGS. 3-6. A first recruitment curve (S1) is then generated by plotting  $V_{pp}$  vs.  $I_{Stim}$  in step 86. The same nerve is then stimulated such that, in step 88, the peak-to-peak voltage ( $V_{pp}$ ) may be extracted by subtracting the  $V_{Max}$  from  $V_{Min}$  of each EMG response without the T1, T2 filters employed in step 84. A second recruitment curve (S2) is then generated in step 90 by plotting  $V_{pp}$  vs.  $I_{stim}$ . The generation of both recruitment curves S1, S2 continues until the maximum stimulation current ( $I_{Max}$ ) is reached (per the decision step 92). If  $I_{Max}$  is not reached, the stimulation current  $I_{stim}$  is incremented in step 94. If  $I_{Max}$  is reached, then the first recruitment curve S1 is subtracted from the second recruitment curve S2 in step 96 to produce the curve "C" shown in step 98. By subtracting S1 from S2, the resulting curve "C" is actually the onset portion of the recruitment curve (that is, the portion before the threshold is reached) for that particular nerve. In this fashion, the last point in the curve "C" is the point with the greatest value of  $I_{stim}$  and hence the hanging point.

## c. Peripheral Nerve Pathology Monitoring

Similar to the nerve pathology monitoring scheme described above, the present invention also contemplates the use of one or more electrodes disposed along a portion or portions of an instrument (including, but not limited to, the access components 24-28 described above) for the purpose of monitoring the change, if any, in peripheral nerves during the course of the procedure. In particular, this may be accomplished by disposing one or more stimulation electrodes a certain distance from the distal end of the instrument such that, in use, they will likely come in contact with a peripheral nerve. For example, a mid-shaft stimulation electrode could be used to stimulate a peripheral nerve during the procedure. In any such configuration, a recruitment curve may be generated for the given peripheral nerve such that it can be assessed in the same fashion as described above with regard to the nerve root retractor, providing the same benefits of being able to tell if the contact between the instrument and the nerve is causing pathology degradation or if the procedure itself is helping to restore or improve the health or status of the peripheral nerve.

## d. Virtual Patient for Evoked Potential Simulation

With reference to FIG. 16, the present invention also contemplates the use of a "virtual patient" device for simulating a naturally occurring recruitment curve. This is advan-

tageous in that it provides the ability to test the various systems disclosed herein, which one would not be able to test without an animal and/or human subject. Based on the typically high costs of obtaining laboratory and/or surgical time (both in terms of human capital and overhead), eliminating the requirement of performing actual testing to obtain recruitment curves is a significant offering. According to the present invention, this can be accomplished by providing a device (not shown) having suitable software and/or hardware capable of producing the signal shown in FIG. 16. The device will preferably accept a sweeping current signal according to the present invention (that is, 200 microseconds width pulses sweeping in amplitude from 0-100 mA) and produce a voltage pulse having a peak-to-peak voltage ( $V_{pp}$ ) that varies with the amplitude of the current input pulse. The relationship of the output  $V_{pp}$  and the input stimulation current will produce a recruitment curve similar to that shown. In one embodiment, the device includes various adjustments such that the features of the recruitment curve may be selectively modified. For example, the features capable of being modified may include, but are not necessarily limited to,  $V_{pp}$  at onset, maximum stimulation current of onset (hanging point), the slope of the linear region and/or the  $V_{pp}$  of the saturation region.

While this invention has been described in terms of a best mode for achieving this invention's objectives, it will be appreciated by those skilled in the art that variations may be accomplished in view of these teachings without deviating from the spirit or scope of the present invention. For example, the present invention may be implemented using any combination of computer programming software, firmware or hardware. As a preparatory step to practicing the invention or constructing an apparatus according to the invention, the computer programming code (whether software or firmware) according to the invention will typically be stored in one or more machine readable storage mediums such as fixed (hard) drives, diskettes, optical disks, magnetic tape, semiconductor memories such as ROMs, PROMs, etc., thereby making an article of manufacture in accordance with the invention. The article of manufacture containing the computer programming code is used by either executing the code directly from the storage device, by copying the code from the storage device into another storage device such as a hard disk, RAM, etc. or by transmitting the code on a network for remote execution. As can be envisioned by one of skill in the art, many different combinations of the above may be used and accordingly the present invention is not limited by the scope of the appended claims.

What is claimed is:

1. A nerve monitoring system comprising a control unit having a display and a plurality of leg muscle sensor electrodes in communication with the control unit, the nerve monitoring system being configured to (a) deliver a plurality of electrical stimulation signals so that when a surgical access instrument adapted to transmit electrical signals received from the nerve monitoring system through a stimulation electrode on the surgical access instrument is connected to the nerve monitoring system and positioned along a selected path within tissue of a patient that contains one or more motor nerves, the plurality of electrical stimulation signals are delivered to the patient tissue, (b) in response to delivery of each one of the plurality of electrical stimulation signals, receive a plurality of voltage response values detected by the plurality of leg muscle sensors coupled to different leg muscles, (c) determine the amplitude value of an unknown stimulation threshold required to evoke a threshold response from any of the leg muscles, d) enter a

17

monitoring mode in response to determining the value of the unknown stimulation threshold, and e) as the surgical access instrument is advanced along the selected path toward a targeted intervertebral disc detect whether stimulation thresholds are changing by incrementing or decrementing the amplitude of the stimulation signal delivered.

2. The system of claim 1, wherein the value of the unknown stimulation threshold determined using the steps of bracketing the unknown stimulation threshold by determining a first stimulation amplitude that does not evoke the threshold response from any of the leg muscles and a second stimulation amplitude that does evoke the threshold response from at least one of the leg muscles, repeatedly bisecting the bracket that includes the stimulation threshold until a final bracket of a predetermined width is reached, and selecting the stimulation threshold from the final bracket.

3. The system of claim 1, wherein the nerve monitoring system is further configured to (d) determine which range from a predetermined group of ranges the determined stimulation threshold is located in, and (e) communicate on the display an indicator corresponding to the determined range from the predetermined group of ranges as an indicator of nerve proximity to the surgical access instrument.

4. The system of claim 1, wherein whether the stimulation amplitude is incremented or decremented is determined as a function of evoked responses from one or more of the leg muscle sensor electrodes.

5. The system of claim 1, wherein the monitoring mode is configured to detect whether stimulation thresholds are changing as the surgical access instrument is advanced along the selected path toward the targeted intervertebral disc by incrementing or decrementing the stimulation amplitude delivered by the stimulation electrode on the surgical access instrument by 0.1 mA.

6. The system of claim 2, wherein monitoring is continued while the stimulation threshold remains in the final bracket and wherein steps (a)-(e) are repeated in response to the stimulation threshold being determined to be outside the final bracket.

7. The system of claim 6, wherein the stimulation threshold is determined to be outside the final bracket when the threshold nerve stimulation amplitude fails to fall within upper and lower ends of the final bracket three times.

8. The system of claim 3, wherein the indicator corresponding to the determined range from the predetermined group of ranges includes a color display.

9. The system of claim 8, wherein the predetermined group of ranges includes three predetermined ranges and the

18

color displayed is one of three different colors, each of the three different colors corresponding to one of the three predetermined ranges.

10. The system of claim 9, wherein the color is one of red, yellow, and green depending on the applicable range.

11. The system of claim 1, with further instructions that cause the display to display at least one of a name and a symbol representative of the surgical access instrument being used.

12. The system of claim 1, wherein the threshold response is a voltage response of a predetermined peak-to-peak voltage.

13. The system of claim 12, wherein the predetermined peak-to-peak voltage is approximately 100  $\mu$ V.

14. The system of claim 1, wherein the threshold response is a peak-to-peak voltage with peaks at a time T1 and a time T2 relative to a stimulation delivery time.

15. The system of claim 1, wherein the surgical access instrument is a dilator cannula.

16. The system of claim 1, and further comprising:

a surgical access instrument in communication with the control unit and deliverable through bodily tissue having neural structures in the selected path toward the targeted intervertebral disc of a spine, the surgical access instrument having a stimulation electrode positioned along a distal tip region to deliver a stimulation signal to the bodily tissue when the surgical access instrument is positioned in the selected path toward the targeted intervertebral disc of the spine;

a plurality of sequential dilator cannulas deliverable through the bodily tissue having neural structures in the selected path toward the targeted intervertebral disc of the spine, the plurality of sequential dilator cannulas including at least the surgical access instrument and the outer dilator cannula configured to be guided over the previously delivered surgical access instrument; and

a working corridor instrument deliverable over the outer dilator cannula of the plurality of sequential dilator cannulas toward the targeted intervertebral disc of the spine, wherein the working corridor instrument is configured to establish an operative corridor to the targeted intervertebral disc of the spine.

17. The system of claim 1, wherein the stimulation signal amplitudes are current amplitudes.

18. The system of claim 17, wherein the current amplitudes are measured in units of mA.

\* \* \* \* \*

专利名称(译)	用于确定手术期间神经接近，方向和病理的系统和方法		
公开(公告)号	<a href="#">US9931077</a>	公开(公告)日	2018-04-03
申请号	US15/258434	申请日	2016-09-07
[标]申请(专利权)人(译)	NUVASIVE		
申请(专利权)人(译)	NUVASIVE INC.		
当前申请(专利权)人(译)	NUVASIVE INC.		
[标]发明人	KAULA NORBERT F BLEWETT JEFFREY J GHARIB JAMES FARQUHAR ALLEN		
发明人	KAULA, NORBERT F. BLEWETT, JEFFREY J. GHARIB, JAMES FARQUHAR, ALLEN		
IPC分类号	A61B5/00 A61B5/0488 A61N1/08 A61N1/36 A61B17/00 A61B5/04 A61B17/02 A61B5/11 A61B5/05 A61B19/00 A61N1/10 A61N1/18		
CPC分类号	A61B5/4893 A61B5/04001 A61B5/0488 A61B5/4836 A61B17/00 A61N1/08 A61N1/36 A61B17/02 A61B2017/00039 A61B5/1106 A61B5/7217 A61B5/743 A61N1/36017		
代理机构(译)	NUVASIVE INC.		
代理人(译)	舍默霍恩，RORY		
优先权	13/767355 2015-05-19 US 13/465666 2014-08-19 US 13/292065 2014-01-21 US 13/080493 2011-11-08 US 12/711937 2011-04-05 US 10/754899 2011-11-29 US 60/305041 2001-07-11 US		
其他公开文献	US20160374613A1		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

#### 摘要(译)

本发明涉及用于基于神经肌肉响应与引起神经肌肉响应的刺激信号之间所识别的关系来确定相对于手术器械的神经接近度，神经方向和病理的系统和方法。

