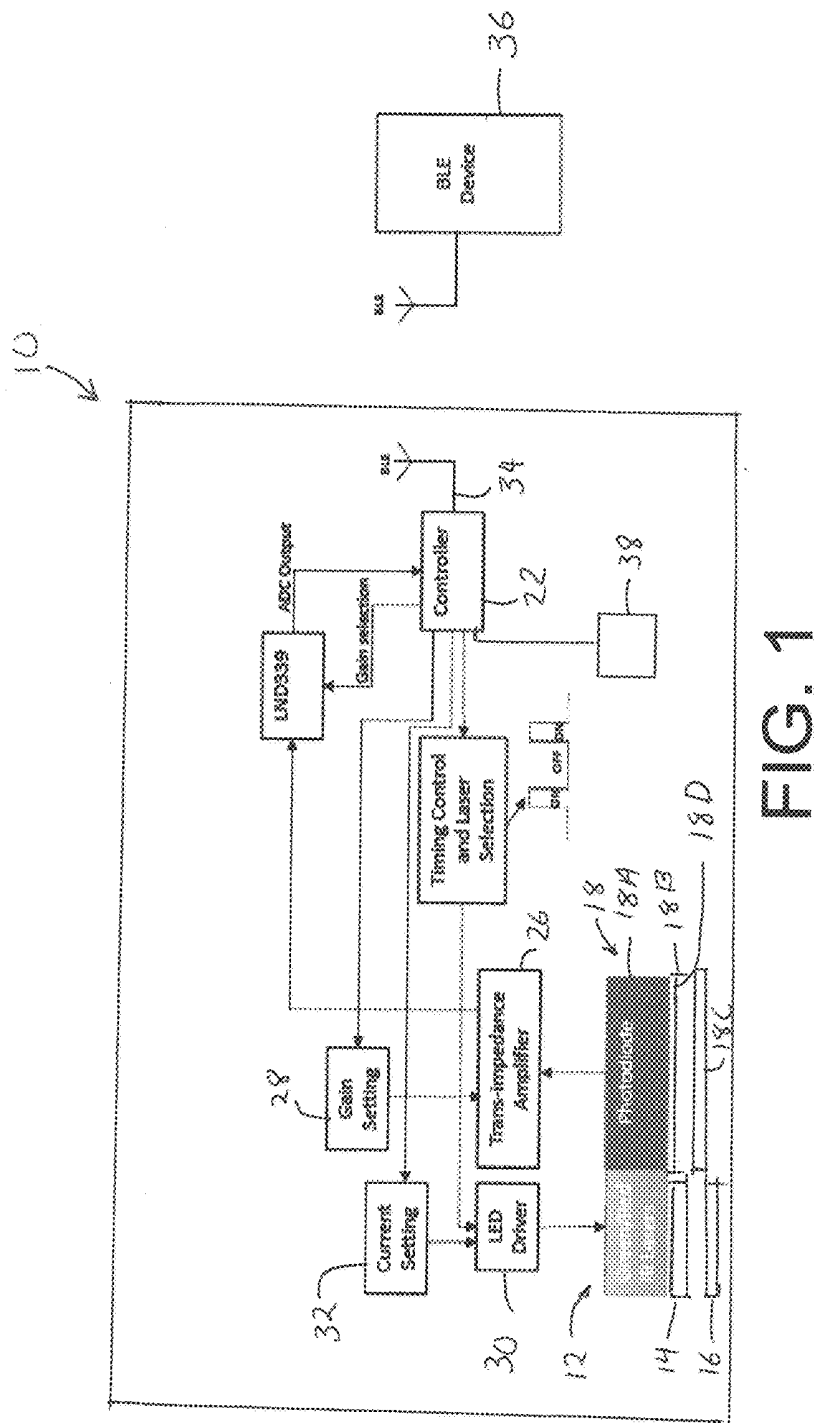




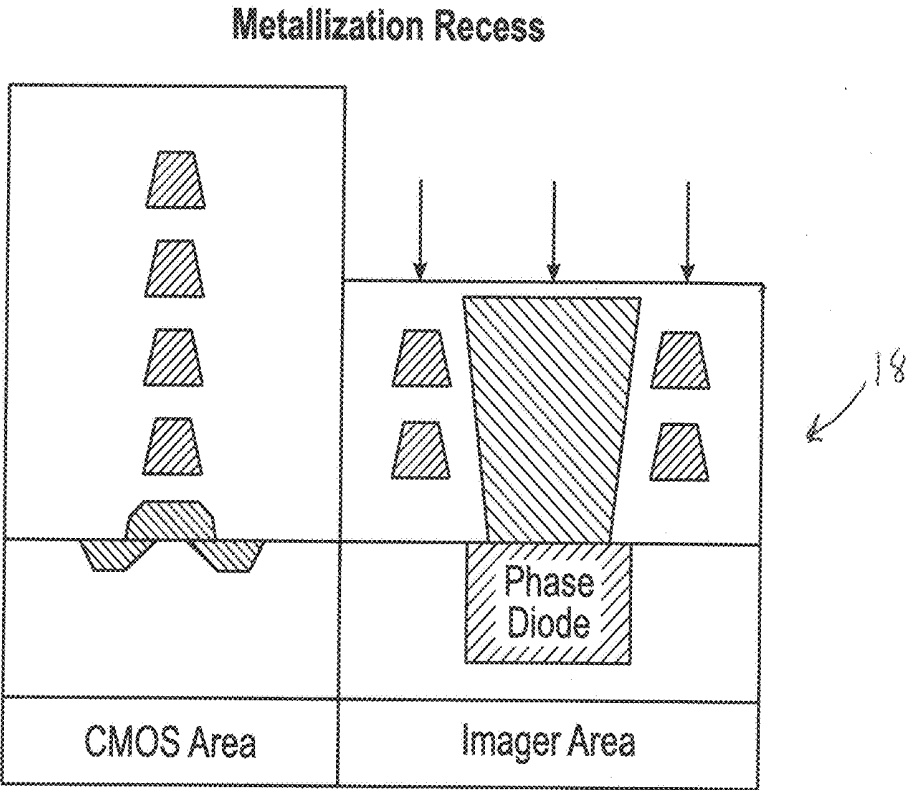


FIG. 2

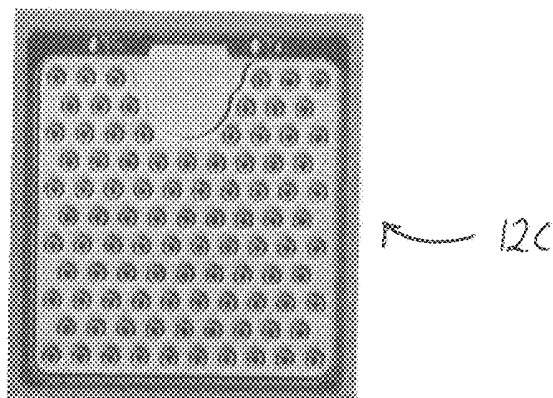


FIG. 3

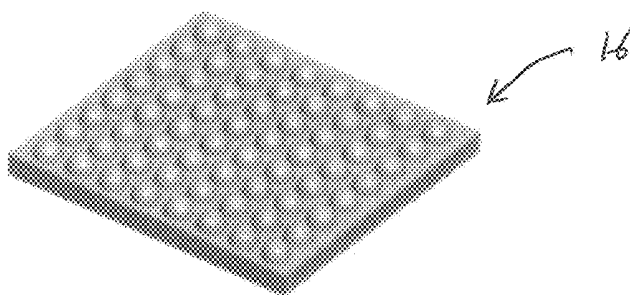


FIG. 4

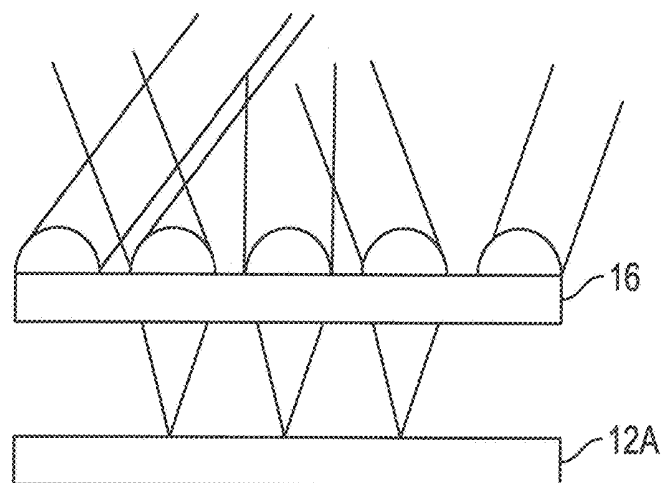


FIG. 5

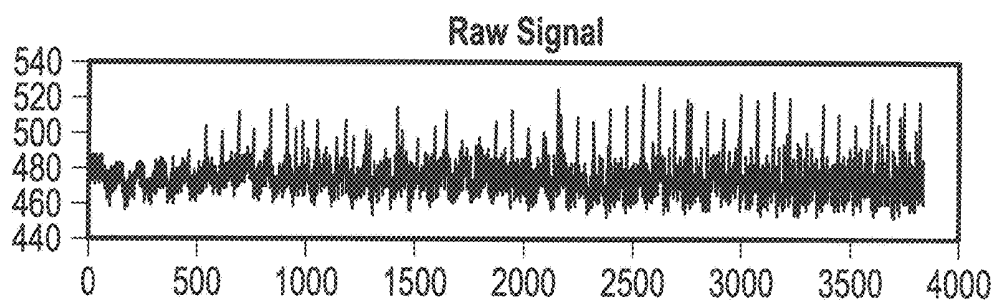


FIG. 6A

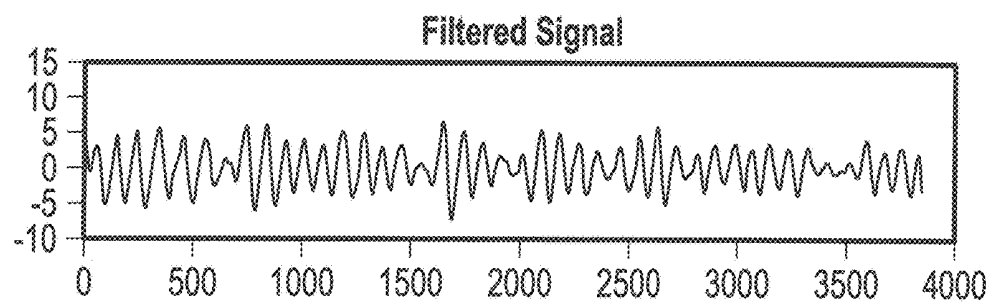


FIG. 6B

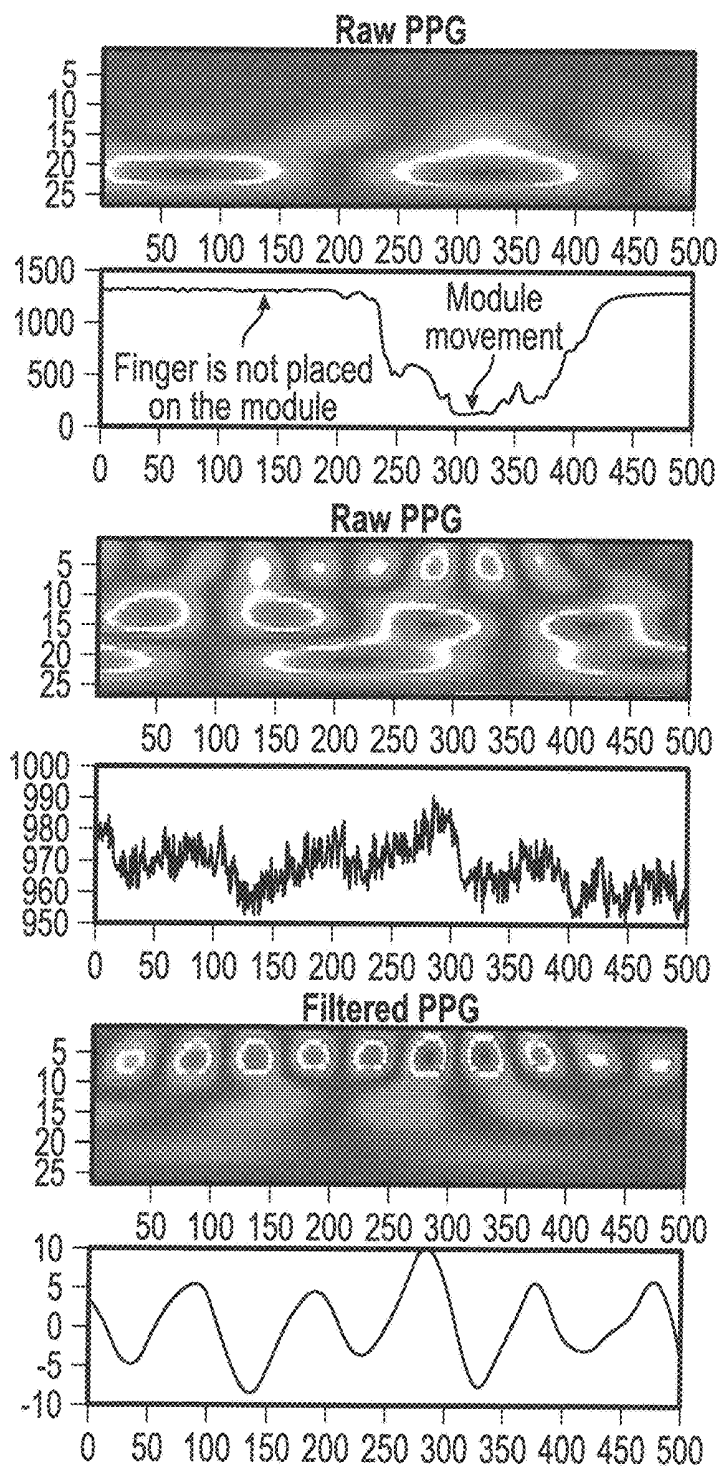


FIG. 7



FIG. 8

60

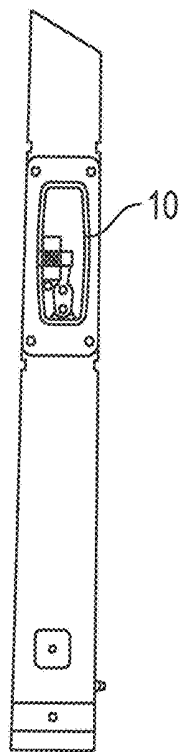


FIG. 9

70

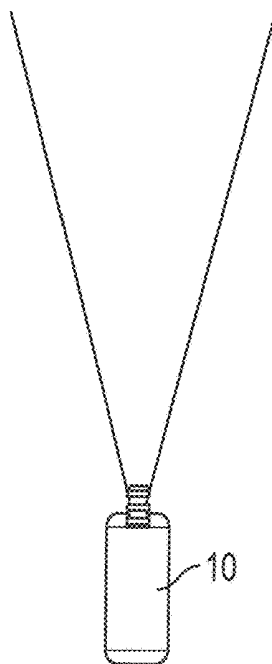
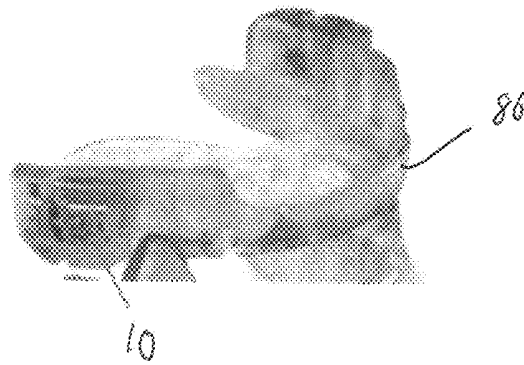


FIG. 10

**FIG. 11**

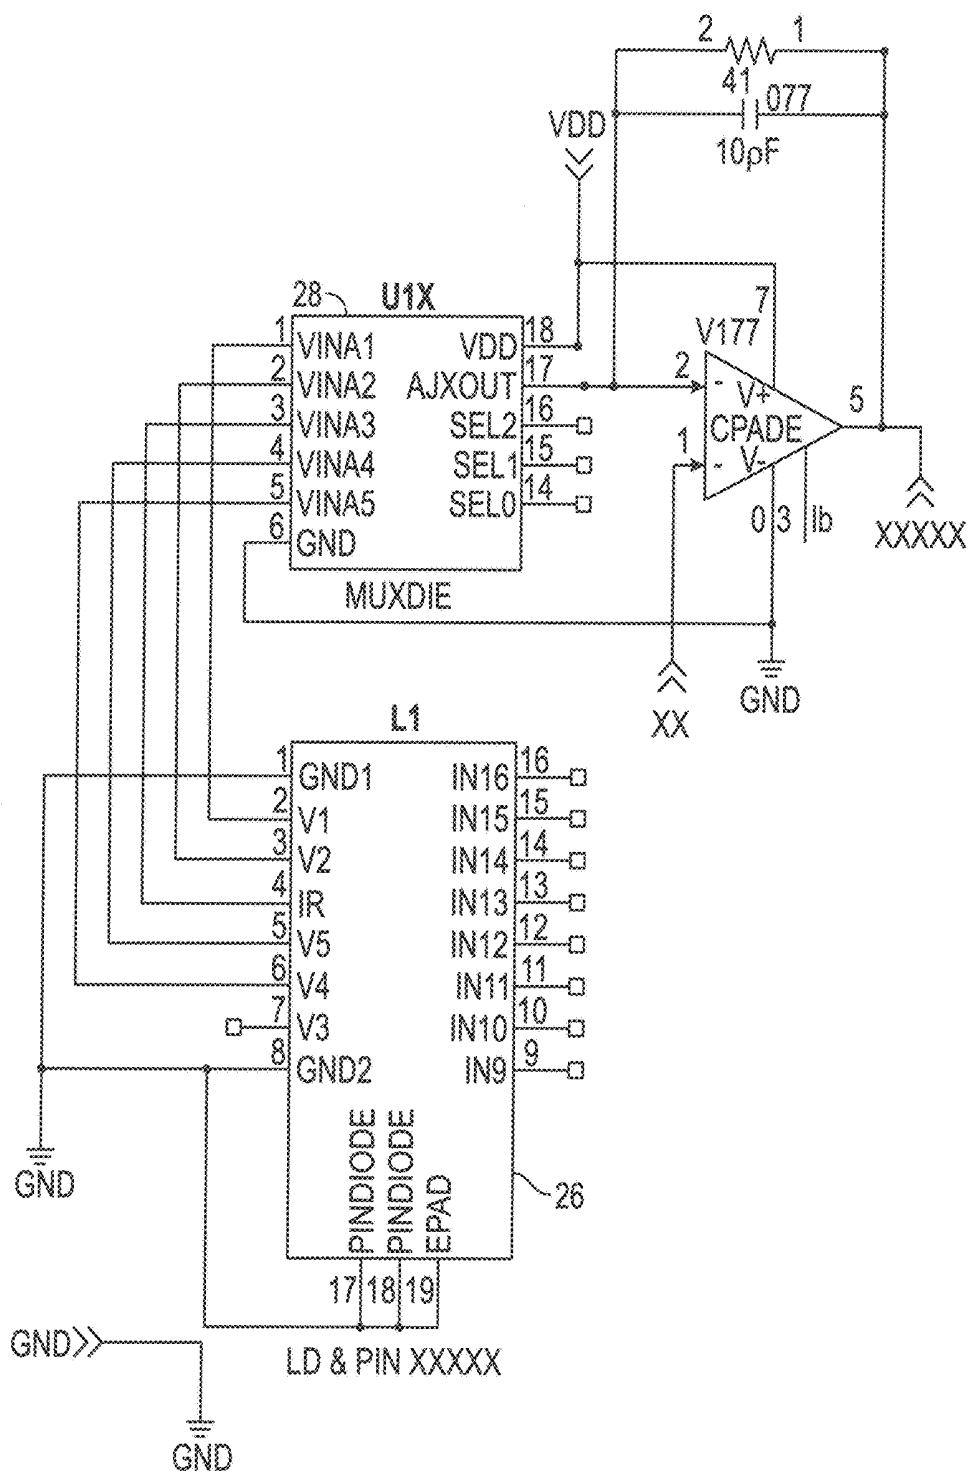


FIG. 12

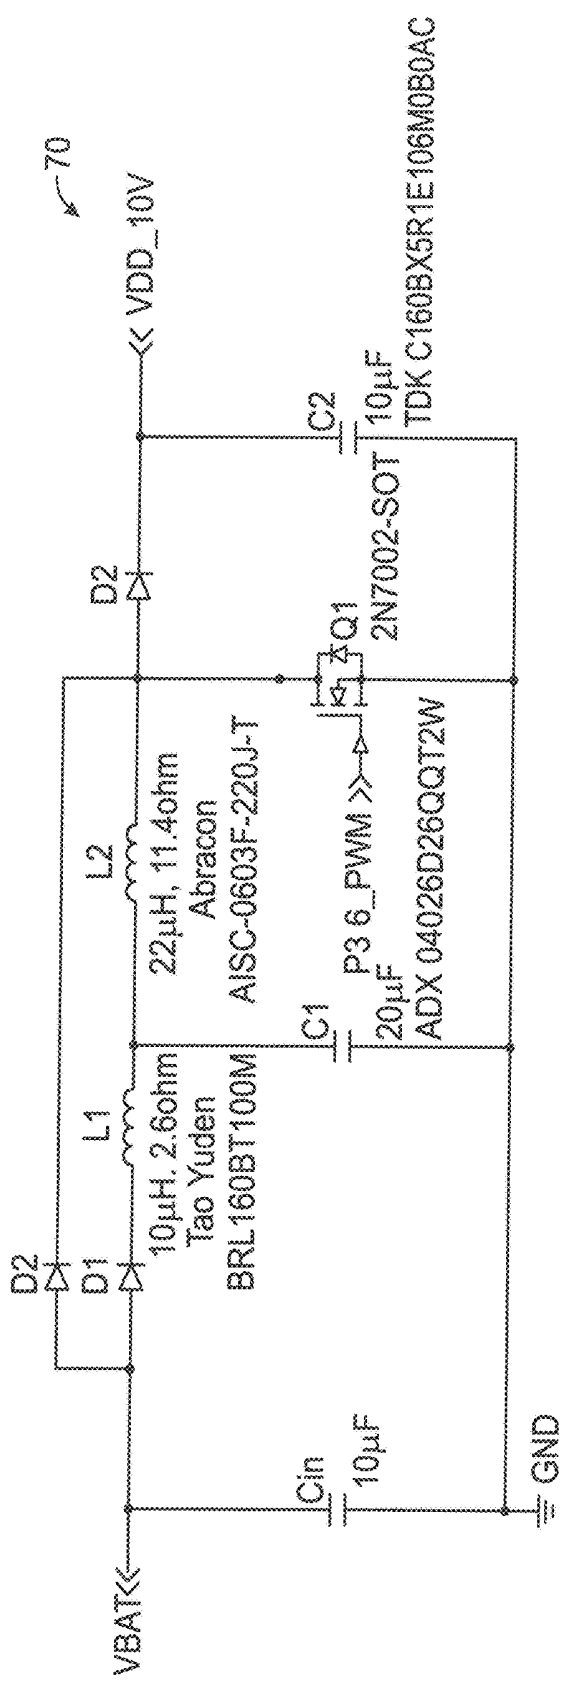


FIG. 13

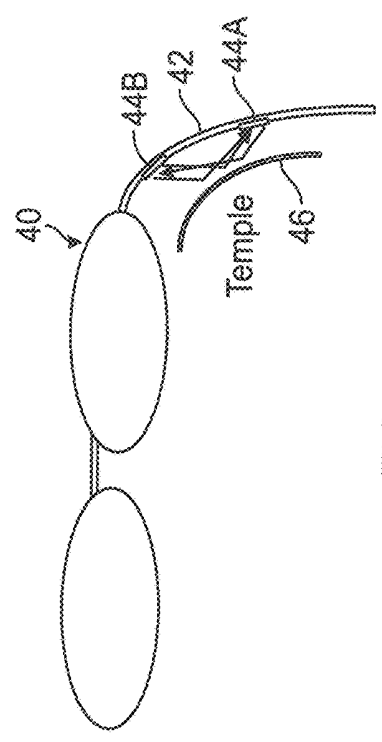


FIG. 14

Algorithmic Flow Chart

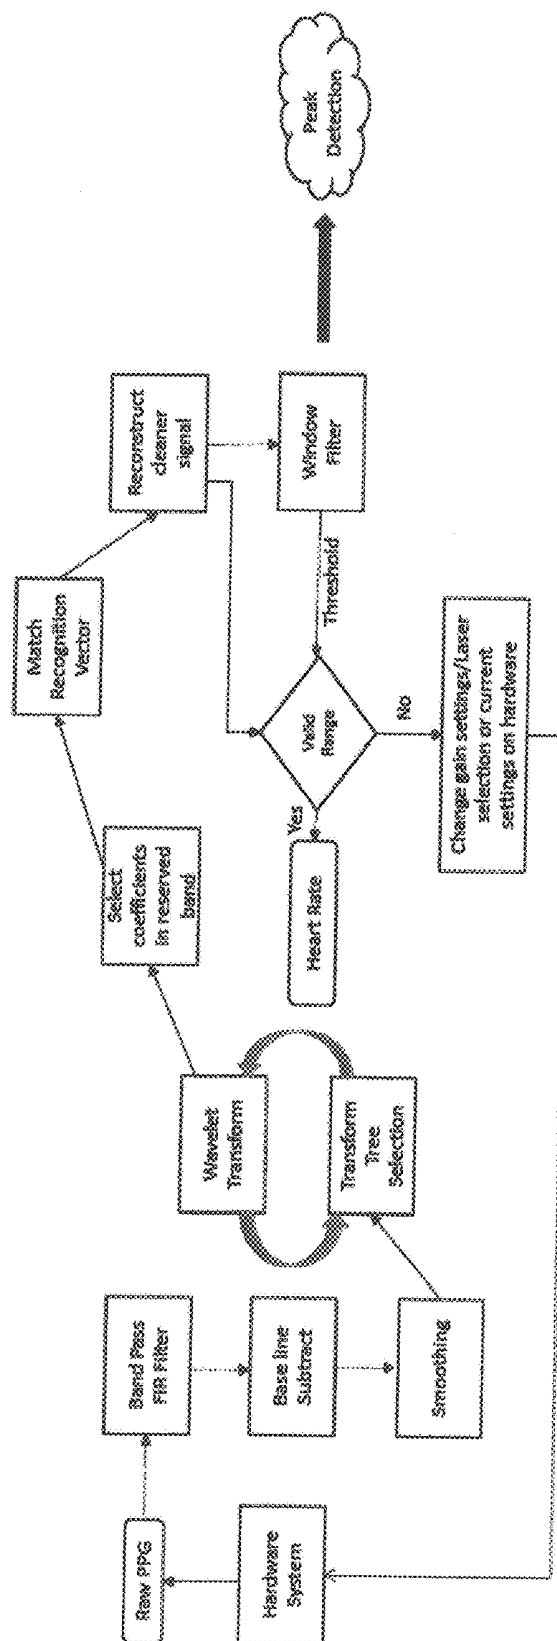


FIG. 15

DEVICE TO EXTRACT PHYSIOLOGICAL INFORMATION AND METHOD THEREFOR

RELATED APPLICATIONS

[0001] This patent application is related to U.S. Provisional Application No. 62/458,465 filed Feb. 13, 2017, entitled "HEART WAVEFORM & BLOOD ALCOHOL EXTRACTION FROM A DISTANCE" in the name of the same inventor, and which is incorporated herein by reference in its entirety. The present patent application claims the benefit under 35 U.S.C § 119(e).

TECHNICAL FIELD

[0002] The present application relates generally to the technical field of medical and wearable devices, and more specifically, to the technical field of a device using laser emitters to extract physiological information from a user.

BACKGROUND

[0003] Many medical and/or wearable devices utilize optical means coupled to the skin to extract physiological information from a living subject. For example, a fitness tracker utilizes the change in optical power as light absorption varies with blood flow through arteries and veins. Heart rate information is then used to measure stress (HRV), fatigue, activities or illness. Similar means exist to determine other factors such as oxygenation, blood alcohol content, glucose, keytones, and the like.

[0004] Many medical and wearable devices utilize optical emitters and optical detectors such as photodetectors as the optical means to extract physiological information. Unfortunately, these types of devices have historically had several significant problems. Medical and wearable devices utilizing optical emitters and optical detectors generally do not work more than 1-2 mm away from the skin or the wearer. Further, optical detectors such as photodetectors are easily saturated by side light. For example, when photodetectors are moved away from the skin of the wearer, side light may be detected by the photodetectors rather than just the reflected light. As a result, the photodetectors may saturate or have a limited operation range. To overcome this, the optical emitters must be physically and optically separated by a barrier from the optical detector resulting in a much larger surface area for the assembly and the photodetector kept close to the skin to ensure light from the outside environment and side light from emitters is blocked.

[0005] Another issue is that medical and wearable devices generally use light emitting diode emitters. The light emitting diodes generate widely scattered light requiring optics that force deep recessing of 5 mm or more into typical form factors and often external lensing. However, the light emitting diodes do not elicit reflections from more than 1-2 mm away strong enough to measure. Thus, the result is that bands or watches which extract information like heart rate using light emitting diodes have to be pulled very tight against the skin of the wearer and form factors such as jewelry or glasses are not compatible with these types of emitter/detector systems. Additionally, form factors such as glasses are not possible because head shapes variation is too great to ensure that the light emitted from the light emitting diodes will reflect back into the detector from the skin once distance starts to exceed 1-2 mm, non-withstanding the risk of saturation by side light.

[0006] Therefore, it would be desirable to provide a system and method that overcomes the above.

SUMMARY

[0007] In accordance with one embodiment, a device to extract physiological information is disclosed. The device has at least one laser emitter. At least one optical detector is provided to detect a change in optical power absorption. The at least one laser emitter and the at least one optical detector are wire bonded into a chip scale module.

[0008] In accordance with one embodiment, a device to extract physiological information is disclosed. The device has a processor. At least one laser emitter is coupled to the processor. At least one optical detector detects a change in optical power absorption and is coupled to the processor. A passive optical device directs light beams from the at least one laser. A lenslet collimates and directs the light beams from the one or more laser emitters at one or more different angles.

[0009] In accordance with one embodiment, a device to extract blood chemistry information is disclosed. The device has a means by which to measure light in the approximately 9.5 um and 10.4 um range and emitters all of which may be tunable. An example is a 9.5 um QCL and a 10.4 um DFB QCL emitter. Detectors may be a HgCdTe photodetector or a tunable detector such as a MOEMS fabry-perot interferometer. The at least one detector detects at least one of thermal infrared waves or radiation resulting from excitation by the 9.5 um QCL and a 10.4 um DFB QCL. Differences in the measurements may be used to measure alcohol, glucose/glucogens, keytones or other blood chemistry.

BRIEF DESCRIPTION OF THE DRAWINGS

[0010] The present application is further detailed with respect to the following drawings. These figures are not intended to limit the scope of the present application but rather illustrate certain attributes thereof. The same reference numbers will be used throughout the drawings to refer to the same or like parts.

[0011] FIG. 1 is an exemplary block diagram of device to extract physiological information from a user in accordance with one aspect of the present application;

[0012] FIG. 2 is an exemplary device to extract physiological information from a user in accordance with one aspect of the present application;

[0013] FIG. 3 is an exemplary laser emitter array used in the device in accordance with one aspect of the present invention;

[0014] FIG. 4 is an exemplary lenslet used in the device in accordance with one aspect of the present invention;

[0015] FIG. 5 is an exemplary lenslet used in the device in accordance with one aspect of the present invention;

[0016] FIG. 6A-6B show reflected light signals received by the device in accordance with one aspect of the present invention;

[0017] FIG. 7 shows wavelet processed reflected light wave signals including motion artifact rejection in accordance with one aspect of the present invention;

[0018] FIG. 7 is an exemplary device placed within a glasses frame in accordance with one aspect of the present invention; a

[0019] FIG. 9 is an exemplary device placed within a watch band/bracelet in accordance with one aspect of the present invention;

[0020] FIG. 10 is an exemplary device placed within a piece of jewelry in accordance with one aspect of the present invention;

[0021] FIG. 11 is an exemplary device placed within an oral appliance in accordance with one aspect of the present invention;

[0022] FIG. 12 is an exemplary multiplexed transconductor used in the device in accordance with one aspect of the present invention;

[0023] FIG. 13 is an exemplary quadratic converter used in the device in accordance with one aspect of the present invention;

[0024] FIG. 14 is an exemplary two chip scale devices placed within a glasses frame in accordance with one aspect of the present invention; and

[0025] FIG. 15 is an exemplary flow chart showing operation of a processor used in the device in the device in accordance with one aspect of the present invention.

DESCRIPTION OF THE APPLICATION

[0026] The description set forth below in connection with the appended drawings is intended as a description of presently preferred embodiments of the disclosure and is not intended to represent the only forms in which the present disclosure can be constructed and/or utilized. The description sets forth the functions and the sequence of steps for constructing and operating the disclosure in connection with the illustrated embodiments. It is to be understood, however, that the same or equivalent functions and sequences can be accomplished by different embodiments that are also intended to be encompassed within the spirit and scope of this disclosure.

[0027] The present disclosure discloses a device to extract physiological information from a user which utilizes laser emitters instead of light emitting diodes. The device may contain various other components to direct the light from the laser emitters and to send multiple beam angles out to ensure some of the beams will reflect back into the detector.

[0028] Referring to FIGs., a device 10 to extract physiological information from a user is shown. The device 10 uses laser emitters 12 instead of light emitting diodes. The laser emitters 12 may emit a green laser, infrared laser or the like. The laser emitters 12 may be Quantum Cascade Lasers (QCL), distributed feedback (DFB) laser or the like including tunable lasers. In accordance with one embodiment, a 9.5 um Fabry-Perot QCL or equivalent wavelength and a 10.4 um DFB QCL or equivalent wavelength are used. The laser emitters 12 may be a vertical-cavity surface-emitting laser (VCSEL) 12A. VCSELs 12A are a type of semiconductor laser diode where light beam emission is perpendicular to the surface of the wafer. Alternately, or in addition to, the laser emitter 12 may be a side emitting laser 12B where the light beam may emit from surfaces formed by cleaving the individual chip out of a wafer such as a side emitting green laser or the like. The laser emitter 12 maintain a much tighter beam compared to LEDs and thus may be used at greater distances than LEDs. In general, the laser emitter 12 may be an array of laser emitters 12C as shown in FIG. 3. In accordance with one embodiment, the laser emitters 12 may be tunable laser emitters whose wavelength of operation may be tunable over a desired wavelength range.

Similarly, the detectors may be tunable detectors whose wavelength of operation may be tunable over a desired wavelength range.

[0029] The laser emitters 12 may be coupled to a passive optical component 14. The passive optical component 14 may be used to direct the light beam emitted by the laser emitters 12. The passive optical component 14 may be devices such as a prism, cylinders, mirrors or similar devices used to direct light beams. The laser emitters 12 may be coupled to a lenslet 16. The lenslet 16 is an array of small lenses located in the same plane. The lenslet 16 may be used to collimate the light beam emitted by the laser emitter 12 and to send out multiple light beam angles out to ensure some of the light beams will reflect back into a detector 18 by the topologies of many different temples, wrists, chests or other skin areas as may be seen in FIG. 5.

[0030] By having the laser emitters 12 illuminate the skin of the user, the detector 18 can measure changes over time in the optical power of the light beam reflected back which provides information such as photoplethysmogram heart information. Alternatively, a processor 22 may measure differences in the amount of light absorbed at different wavelengths. For example, alcohol content in blood may be measured by the difference between light absorbed at 9.5 um vs that at 10.4 um. A processor 22 may then be able to analyze this information to extract physiological information from the user. The processor 22 may calculate the change in optical power as light absorption varies with blood flow or excitation frequency through arteries and veins to monitor changes in blood flow, heart rate, oxygenation, blood alcohol content and the like. The processor 22 may use wavelet processing and machine learning to extract signals of interest from noise and motion artifacts without the disadvantages of frequency based filtering which tend to damage the signal of interest and struggle to separate other physiological sources such as EMG or movement (see FIG. 5A-6). The processor 22 may have a transmitter 34. The transmitter 34 may be used to wirelessly transmit data from the device 10 to a device 36. The device 36 may be used to read and display the data collected and calculated by the device 10. The device 36 may be a smartphone, tablet or similar device. In accordance with one embodiment, Bluetooth standards may be used for transmitting the data from the device 10. The device 10 may have a power source 38. The power source 38 may be a battery or the like used to power the non-passive devices.

[0031] To allow the laser emitters 12 to be placed in close proximity and without optical separation the device 10 uses a photodetector 18A as the detector 18. The photodetector 18 may be silicon detector, an HgCdTe photodetector or tunable IR filter detector such as a Micro-Opto-Electromechanical System (MOEMS) fabry-perot interferometer. HgCdTe or mercury cadmium telluride is useful for infrared detection because of: (1) Adjustable bandgap from 0.7 to 25 um; (2) Direct bandgap with high absorption coefficient; (3) Moderate dielectric constant/index of refraction, (4) Moderate thermal coefficient of expansion and (5) Availability of wide bandgap lattice-matched substrates for epitaxial growth.

[0032] The photodetector 18A is configured to block side light. The photodetector 18A may include on chip side light blocking 18B, light pipe 18C, anti-glare/anti-refraction coating 18D, on chip lensing and other means to reduce the incidence of side light being gathered and to reduce distortion. Side light blocking 18B may be edging or the like

formed around the photodetector **18A** to prevent side light from entering the photodetector **18A**, light pipes **18C** which only allow light vertically to fall upon the photodetector **18A**, one or two layers of on chip lensing and anti-glare/anti-refraction coating reduce the incidence of side light being gathered and to reduce distortion.

[0033] Using the above, the device **10** may be utilized more than 1-2 mm from the skin without saturating. FIG. 6A-6B, show the reflected light signal received when the device **10** is 7 mm away from the skin of the user. FIG. 6A show the raw light signal reflected back to the device **10** while FIG. 6B shows the extracted filtered signal. As one can see, even at 7 mm away, the device **10** is able to receive and read the reflected light signal.

[0034] By being able to receive the reflected light signal from greater distances, the device **10** may be used in different form factors and applications. For example, the device may allow uses such as, but not limited to: i) glasses **50** measuring heart rate or creating a photoplethysmogram (PPG), blood alcohol, glucose and glucogens, peripheral capillary oxygen saturation (SPO₂), ketones, respiration, diet, and the like from the temple of a user as shown in FIG. 8; ii) bands/watches **60** which may be worn loosely FIG. 8; iii) jewelry such as necklaces **70** (FIG. 10), rings or ear rings which may be worn loosely and require small electronic assemblies; iv) clothing and apparel which may be worn loosely; v) information may be extracted from within the mouth by coupling to an oral appliance **80** as shown in FIG. 10; vi) skin cancer may be detected using measured optical information compared against a database of such information from by a machine learning algorithm; and vii) compatibility of a person's skin with different cosmetics may be provided by comparing the optical information compared against a database of optical information favoring different cosmetic products by a machine learning algorithm; vii) optical detectors focused on the UV bands can measure and time the hazards of damaging sun exposure; viii) in combination with these optical detectors an ECG detector elsewhere on the body may be combined with the optical information to measure pulse wave velocity, arterial stiffness and these may be converted into blood pressure; ix) cardiac and capillary based authentication or identification information may be extracted. By taking the time between the electrical ECG peak current and the fastest derivative of the PPG waveform (the time the heart pushes the blood to the time it arrives and dividing by the distance from the heart to the point of measurement, we get Pulse Wave Velocity (PWV). PWV is the velocity at which the arterial pulse propagates through the circulatory system. PWV may be used as a measure of arterial stiffness and may have a correlation with cardiovascular events and an indicator of target organ damage.

[0035] As may be seen in the FIGs., to further reduce size of the device **10** a hybrid substrate and wire bonding techniques may be used where the laser emitters **12**, passive optical component **14**, processor **22** and other components may be wire bonded directly to the substrate to avoid typical plastic, ceramic or plastic packaging area spacings. Using these techniques, modules of significantly less than 5 mm thick and less than 3×3 mm in surface area may be constructed. The use of laser emitters **12** may allow very thin packaging by eliminating the optics normally required by LEDs. Laser emitters **12** such as IR VCSELs **12A** for example are available with multiple emitters as shown in

FIG. 3 which might emit a $\pm 17^\circ$ beam which may be collimated by the lenslet **16** designed to interface to a multi-element laser die.

[0036] By creating device **10** using wire bond techniques, typical called chip scale modules or multi-chip modules, with the side light blocking photodetector **18A** and placing the laser emitters **12** next to the detector **18** it is possible to minimize module size compared with solutions which must separate emitters from the detector, and to make thinner modules compared to those utilizing LED emitters. These modules may use "glob top" opaque materials to block light over active components such as transconductors, op-amps, gain devices or multiplexers and the entire assembly may be encapsulated by a transparent coating material for mechanical resilience and waterproofing or optical components may be "glob topped" with a transparent coating. Additionally, physiological information can be extracted from more than 1-2 mm away from the module. Combining this with a processor **22** capable of processing wavelet and other information allows extraction during motion and in real world environments where noise is present. Finally, coupling the device **10** to a portable form factor such a band or glasses and operating them from a battery allows the device **10** to be widely and convenient to used.

[0037] In addition, multiple laser emitters **12** or detectors **18** might be used emitting and detecting different wavelengths. If multiple detectors **18** are used, to couple these detectors **18** to a transconductor **26**, a multiplexer **28** may be used as shown in FIG. 12. The transconductor **26** may be used to generate a voltage signal proportional to the reflected light signal received. The transconductor **26** might have a programmable gain **28** or might have a fixed gain and be followed by a voltage gain device. The output of the transconductor **26** or voltage gain means might in be coupled to an A/D converter for compatibility with digital processors. Current drivers **30** may also be used which provide a programmable current source **32** for ensuring the laser emitters **12** are working in the lasing region of operation and further are producing the correct amount of light. These drivers **30** may pulse the laser emitters **12** to reduce power consumption and heat. A DC/DC converter may be included in the chip scale module to generate the power rails for the ICs and the LEDs. This DC/DC may be dynamically controlled by the processor **22** so that voltage levels are only generated when required. For example, an ARM microcontroller may need only 1.6V for general computation but must be increased to 2.4V when outputting a DAC value or reading using an ADC. A green laser may require 6V to operate but only for a short time. To minimize components sizes the DC/DC converter may utilize a quadratic converter topology **70** as shown in FIG. 13. This device **10** may be controlled by an intelligent processor **22** to implement an algorithmic methodology as shown in FIG. 15. The system may also include a frequency-based filter to bandpass the response of interest before utilizing the wavelet processing means. The overall wire bonded chip scale module might appear similar to that shown in FIG. 2.

[0038] Two or more chip scale devices may be used where the lenslet **18C** directs light to the user's skin such that it may reflect from the skin and be detected by the photodetector **18A** on the second module as shown in FIG. 14. For example, on the temple **42** of glasses **40**, the device **10** may be formed of two modules **44A** and **44B**. The two modules **44A** and **44B** may be spaced apart such that module **44A**

could light up the temple 46 of the user from one side and be picked up by the module 44B or vice versa to increase the area that is illuminated and the chance of one of the lenslet beams reflecting from the skin into the other photodetector 18A is increased.

[0039] Many of the methods described in the text above may be extended to extract physiological information from animals. For example, a dog or cat collar or harness might utilize these methods to extract heart rate, diet or health related information from those animals or an ear sensor on a cow or horse might help separate sick animals from the rest of the herd by looking at their HRV and heart rate or SPO2 (stress, fatigue, sickness, blood oxygen, respiration, etc.).

[0040] The foregoing description is illustrative of particular embodiments of the application, but is not meant to be a limitation upon the practice thereof. The following claims, including all equivalents thereof, are intended to define the scope of the application.

What is claimed is:

1. A device to extract physiological information comprising:

- at least one laser emitter; and
- at least one optical detector detecting at least one of a change or difference in optical power absorption;
- wherein the at least one laser emitter and at least one optical detector are wire bonded into a chip scale module.

2. The device of claim 1, comprising a passive optical device directing a light from the at least one laser, the passive optical device configured into the chip scale module.

3. The device of claim 1, wherein the at least one laser emitter is one of a VCSEL or side emitting laser.

4. The device of claim 2, wherein the passive optical device is one of a prism, cylinder or mirror.

5. The device of claim 1, comprising a lenslet, the lenslet collimates and directs light from the one or more laser emitters at one or more different angles.

6. The device of claim 1, wherein the at least one optical detector is a photodetector, the photodetector having at least one of: side blocking edging and light tubes directing reflected light to the photodetector.

7. The device of claim 1, comprising:

- a passive optical device directing a light from the at least one laser; and

- at least one of: side blocking edging and light tubes directing reflected light to the at least one optical detector,

wherein the passive optical device and at least one of: side blocking edging and light tubes allowing the at least one laser emitter and at least one optical detector to be co-located in a single window.

8. The device of claim 1, wherein the device is coupled to a temple of an eyewear.

9. The device of claim 1, wherein the device is coupled to one of jewelry or an oral appliance to extract physiological information from distances greater than 2 mm.

10. The device of claim 1, wherein the at least one optical detector is a photodetector, the photodetector monitoring at least one of variations or differences in optical power reflected from the user to determine at least one of: change in blood flow, heart rate, oxygenation, blood alcohol level, keytones, glucogens and other body readings.

11. The device of claim 1, comprising:

- a plurality of optical detectors, wherein the plurality of optical detectors are photodetectors;
- a transconductor coupled to the plurality of photodetectors to generate a voltage signal proportional to a reflected light signal received.

12. The device of claim 11, comprising a multiplexer coupled to the transconductor.

13. The device of claim 11, comprising a programmable current driver coupled to the at one laser emitter.

14. The device of claim 1, comprising a transmitter wirelessly transmitting data from the device.

15. A device to extract physiological information comprising:

- a processor,
- at least one laser emitter coupled to the processor,
- at least one optical detector detecting at least one of a change or difference in optical power absorption coupled to the processor;
- a passive optical device directing light beams from the at least one laser, and
- a lenslet collimating and directing the light beams from the one or more laser emitters at one or more different angles.

16. The device of claim 15, wherein the at least one laser emitter, at least one optical detector and the passive optical device are wire bonded into a chip scale module.

17. The device of claim 15, wherein the passive optical device is one of a prism, cylinder or mirror.

18. The device of claim 15, comprising:

- a plurality of optical detectors, wherein the plurality of optical detectors are photodetectors;
- a transconductor coupled to the plurality of photodetectors to generate a voltage signal proportional to a reflected light signal received; and
- a multiplexer coupled to the transconductor.

19. The device of claim 15, wherein the at least one laser emitter is a tunable laser emitter.

20. The device of claim 15, comprising a transmitter wirelessly transmitting data from the device.

21. The device of claim 15, wherein the photodetector is one of an HgCdTe photodetector, a Micro-Opto-Electromechanical System (MOEMS) fabry-perot interferometer, or other tunable detector.

22. The device of claim 15, wherein the processor uses wavelet processing and machine learning to extract signals from noise and motion artifacts.

23. A device to extract blood chemistry information comprising:

- a 9.5 μm QCL;
- a 10.4 μm DFB QCL;
- at least one HgCdTe photodetector or MOEMS fabry-perot interferometer, and
- wherein said at least one photodetector detects at least one of thermal infrared waves or radiation resulting from excitation by the optical emitters to determine or correlate blood chemistry.

24. The device of claim 23, comprising:

- a passive optical device directing light from the 9.5 μm QCL and the 10.4 μm DFB QCL; and
- at least one of: side blocking edging and light tubes directing reflected light to the at least one HgCdTe photodetector or MOEMS fabry-perot interferometer; wherein the passive optical device and at least one of: side blocking edging and light tubes allowing the 9.5 μm

QCL and the 10.4 μm DFB QCL and at least one HgCdTe photodetector or MOEMS fabry-perot interferometer to be co-located in a single window.

25. The device of claim 1, wherein the at least one optical detector detecting the change in optical power absorption at distances greater than 2 mm.

* * * * *

专利名称(译)	提取生理信息的装置及其方法		
公开(公告)号	US20180242892A1	公开(公告)日	2018-08-30
申请号	US15/895401	申请日	2018-02-13
[标]申请(专利权)人(译)	SCHIE DAVID		
申请(专利权)人(译)	SCHIE , DAVID		
当前申请(专利权)人(译)	SCHIE , DAVID		
[标]发明人	SCHIE DAVID		
发明人	SCHIE, DAVID		
IPC分类号	A61B5/1455 A61B5/0205 A61B5/026 A61B5/00 H01S5/022 H01S5/00 G01N33/49		
CPC分类号	A61B5/14552 A61B5/0205 A61B5/0261 A61B5/4845 A61B5/6803 A61B5/7278 A61B5/7207 A61B5/726 A61B5/7267 H01S5/02276 H01S5/0071 G01N33/49 A61B5/02427 A61B5/14532 A61B5/14546 A61B2562/0238 G02C11/10		
优先权	62/458465 2017-02-13 US		
外部链接	Espacenet USPTO		

摘要(译)

提取生理信息的装置具有至少一个激光发射器。至少一个光学检测器用于检测光功率吸收的变化。激光发射器和光学检测器被线接合到芯片级模块中。

